

Prüfbericht-Nr.: Test report no.:	CN25HSWX 004	Auftrags-Nr.: Order no.:	168571276	Seite 1 von 31 Page 1 of 31
Kunden-Referenz-Nr.: Client reference no.:		Auftragsdatum: Order date:	2025-08-24	
Auftraggeber: Client:	Jovistar Inc. 2108 N ST STE C SACRAMENTO, CA 95816			
Prüfgegenstand: Test item:	Remote Controller			
Bezeichnung / Typ-Nr.: Identification / Type no.:	YZAWZJO			
Auftrags-Inhalt: Order content:	SAR Test Report			
Prüfgrundlage: Test specification:	FCC 47 CFR § 2.1093 IEEE Std 1528-2013 Published RF exposure KDB procedures			
Wareneingangsdatum: Date of sample receipt:	2025-08-21	Please refer to Photo Document		
Prüfmuster-Nr.: Test sample no.:	A004079298-001, 003, 004			
Prüfzeitraum: Testing period:	2025-09-17 - 2025-09-18			
Ort der Prüfung: Place of testing:	TÜV Rheinland (Shenzhen) Co., Ltd.			
Prüflaboratorium: Testing laboratory:	TÜV Rheinland (Shenzhen) Co., Ltd.			
Prüfergebnis*: Test result*:	Pass			
geprüft von: tested by:	x <u>Bell Hu</u>		genehmigt von: authorized by:	x <u>Jonathan Li</u>
Datum: Date:	2025-09-19	Signed by: Bell Hu		Ausstellungsdatum: Issue date:
		2025-09-19		Signed by: Jonathan Li
Stellung / Position:	Sachverständige(r)/Expert		Stellung / Position:	Sachverständige(r)/Expert
Sonstiges / Other:	FCC ID: 2BRGW-YZAWZJO			
Zustand des Prüfgegenstandes bei Anlieferung: Condition of the test item at delivery:	Prüfmuster vollständig und unbeschädigt Test item complete and undamaged			
* Legende:	P(ass) = entspricht o.g. Prüfgrundlage(n)	F(ail) = entspricht nicht o.g. Prüfgrundlage(n)	N/A = nicht anwendbar	N/T = nicht getestet
* Legend:	P(ass) = passed a.m. test specification(s)	F(ail) = failed a.m. test specification(s)	N/A = not applicable	N/T = not tested
Dieser Prüfbericht bezieht sich nur auf das o.g. Prüfmuster und darf ohne Genehmigung der Prüfstelle nicht auszugsweise vervielfältigt werden. Dieser Bericht berechtigt nicht zur Verwendung eines Prüfzeichens. This test report only relates to the above mentioned test sample. Without permission of the test center this test report is not permitted to be duplicated in extracts. This test report does not entitle to carry any test mark.				

Prüfbericht-Nr.: CN25HSWX 004
Test report no.:

Seite 2 von 31
Page 2 of 31

Anmerkungen
Remarks

1	Alle eingesetzten Prüfmittel waren zum angegebenen Prüfzeitraum gemäß eines festgelegten Kalibrierungsprogramms unseres Prüfhauses kalibriert. Sie entsprechen den in den Prüfprogrammen hinterlegten Anforderungen. Die Rückverfolgbarkeit der eingesetzten Prüfmittel ist durch die Einhaltung der Regelungen unseres Managementsystems gegeben. Detaillierte Informationen bezüglich Prüfkonditionen, Prüfequipment und Messunsicherheiten sind im Prüflabor vorhanden und können auf Wunsch bereitgestellt werden. <i>The equipment used during the specified testing period was calibrated according to our test laboratory calibration program. The equipment fulfils the requirements included in the relevant standards. The traceability of the test equipment used is ensured by compliance with the regulations of our management system. Detailed information regarding test conditions, equipment and measurement uncertainty is available in the test laboratory and could be provided on request.</i>
2	Wie vertraglich vereinbart, wurde dieses Dokument nur digital unterzeichnet. Der TÜV Rheinland hat nicht überprüft, welche rechtlichen oder sonstigen diesbezüglichen Anforderungen für dieses Dokument gelten. Diese Überprüfung liegt in der Verantwortung des Benutzers dieses Dokuments. Auf Verlangen des Kunden kann der TÜV Rheinland die Gültigkeit der digitalen Signatur durch ein gesondertes Dokument bestätigen. Diese Anfrage ist an unseren Vertrieb zu richten. Eine Umweltgebühr für einen solchen zusätzlichen Service wird erhoben. Informationen zur Verifizierung der Authentizität unserer Dokumente erhalten Sie auf folgender Webseite: go.tuv.com/digital-signature <i>As contractually agreed, this document has been signed digitally only. TUV Rheinland has not verified and unable to verify which legal or other pertaining requirements are applicable for this document. Such verification is within the responsibility of the user of this document. Upon request by its client, TUV Rheinland can confirm the validity of the digital signature by a separate document. Such request shall be addressed to our Sales department. An environmental fee for such additional service will be charged. For information on verifying the authenticity of our documents, please visit the following website: go.tuv.com/digital-signature</i>
3	Prüfklausel mit der Note * wurden an qualifizierte Unterauftragnehmer vergeben und sind unter der jeweiligen Prüfklausel des Berichts beschrieben. Abweichungen von Prüfspezifikation(en) oder Kundenanforderungen sind in der jeweiligen Prüfklausel im Bericht aufgeführt. <i>Test clauses with remark of * are subcontracted to qualified subcontractors and described under the respective test clause in the report.</i> <i>Deviations of testing specification(s) or customer requirements are listed in specific test clause in the report.</i>
4	Die Entscheidungsregel für Konformitätserklärungen basierend auf numerischen Messergebnissen in diesem Prüfbericht basiert auf der "Null-Grenzwert-Regel" und der "Einfachen Akzeptanz" gemäß ILAC G8:2019 und IEC Guide 115:2021, es sei denn, in der auf Seite 1 dieses Berichts genannten angewandten Norm ist etwas anderes festgelegt oder vom Kunden gewünscht. Dies bedeutet, dass die Messunsicherheit nicht berücksichtigt wird und daher auch nicht im Prüfbericht angegeben wird. Zu weiteren Informationen bezüglich des Risikos durch diese Entscheidungsregel siehe ILAC G8:2019. <i>The decision rule for statements of conformity, based on numerical measurement results, in this test report is based on the "Zero Guard Band Rule" and "Simple Acceptance" in accordance with ILAC G8:2019 and IEC Guide 115:2021, unless otherwise specified in the applied standard mentioned on Page 1 of this report or requested by the customer. This means that measurement uncertainty is not taken in account and hence also not declared in the test report. For additional information to the resulting risk based of this decision rule please refer to ILAC G8:2019.</i>

Table of Contents

1.	GENERAL INFORMATION.....	5
1.1.	STATEMENT OF COMPLIANCE	5
1.2.	EQUIPMENT UNDER TEST (EUT) INFORMATION.....	6
1.2.1.	<i>General Information</i>	<i>6</i>
1.2.2.	<i>Wireless Technologies.....</i>	<i>6</i>
2.	TEST SITES	8
2.1.	TEST FACILITIES.....	8
2.2.	AMBIENT CONDITION.....	8
2.3.	LIST OF TEST AND MEASUREMENT INSTRUMENTS.....	9
3.	MEASUREMENT UNCERTAINTY.....	10
4.	TEST SPECIFICATION, METHODS AND PROCEDURES.....	12
5.	SAR MEASUREMENT SYSTEM.....	13
5.1.	DEFINITION OF SPECIFIC ABSORPTION RATE (SAR).....	13
5.2.	SPEAG DASY SYSTEM	13
5.2.1.	<i>Robot.....</i>	<i>14</i>
5.2.2.	<i>Probes.....</i>	<i>15</i>
5.2.3.	<i>Data Acquisition Electronics (DAE)</i>	<i>15</i>
5.2.4.	<i>Phantoms.....</i>	<i>16</i>
5.2.5.	<i>Device Holder</i>	<i>17</i>
5.2.6.	<i>System Validation Dipoles</i>	<i>17</i>
5.2.7.	<i>Tissue Simulating Liquids</i>	<i>18</i>
5.2.8.	<i>SAR System Verification.....</i>	<i>20</i>
6.	SAR MEASUREMENT PROCEDURE	21
6.1.	AREA & ZOOM SCAN PROCEDURE	21
6.2.	VOLUME SCAN PROCEDURE.....	21
6.3.	POWER DRIFT MONITORING	22
6.4.	SPATIAL PEAK SAR EVALUATION	22
6.5.	SAR AVERAGED METHODS.....	22
7.	SAR MEASUREMENT EVALUATION	23
7.1.	EUT CONFIGURATION AND SETTING	23
7.2.	EUT TESTING POSITION.....	23
7.2.1.	<i>Body Exposure Conditions.....</i>	<i>23</i>
7.2.2.	<i>Extremity Exposure Conditions.....</i>	<i>23</i>
7.3.	TISSUE VERIFICATION	24
7.4.	SYSTEM VALIDATION.....	24
7.5.	SYSTEM VERIFICATION.....	24
8.	SAR MEASUREMENT EVALUATION	25
8.1.	CONDUCTED POWER.....	25

Prüfbericht - Nr.: CN25D56X 004
Test Report No.

Seite 4 von 31
Page 4 of 31

8.2. SAR TESTING RESULTS.....	27
8.2.1. SAR Test Reduction Considerations	27
8.2.2. SAR Results for Body Exposure Condition (Separation Distance is 0 cm Gap)	27
8.2.3. SAR Results for Extremity Exposure Condition (Separation Distance is 0 cm Gap)	28
8.2.4. SAR Measurement Variability	29
8.2.5. MIMO Evaluation	30

APPENDIXES.....	31
------------------------	-----------

Appendix A: SAR Plots of System Verification

Appendix B: SAR Plots of SAR Measurement

Appendix C: Calibration Certificate for probe and Dipole

Appendix D: Photographs of EUT and setup

1. General Information

1.1. Statement of Compliance

The maximum results of Specific Absorption Rate (SAR) found during testing for the EUT are as follows:

Operating Mode	Highest Body SAR _{1g} (0 cm Gap) (W/kg)	Highest Extremity SAR _{10g} (0 cm Gap) (W/kg)
SDR-2.4G	0.28	0.49
SDR-5.1G	0.16	0.43
SDR-5.8G	0.72	1.29
Highest MIMO Transmission SAR	Body SAR _{1g} (W/kg)	Extremity SAR _{10g} (W/kg)
MIMO_SDR 2.4GHz	0.54	0.95
MIMO_SDR 5.1GHz	0.30	0.80
MIMO_SDR 5.8GHz	1.36	2.58

Note:

1. This device is in compliance with Specific Absorption Rate (SAR) for general population/uncontrolled exposure limits (1.6W/kg as averaged over any 1 gram of tissue; 10-gram SAR for Product Specific 10g SAR, limit: 4.0W/kg) specified in FCC 47 CFR part 2 (2.1093) and ANSI/IEEE C95.1-1992, and had been tested in accordance with the measurement methods and procedures specified in IEEE 1528-2013 and FCC KDB publications.
2. This device is a hand-held remote controller, all required sides were considered for limb-worn mode with 0mm distance. Only the rear and bottom sides may have probability to keep towards with body/lap, thus body-SAR considered for them as well, detailed description listed on Appendix D.

1.2. Equipment Under Test (EUT) Information

1.2.1. General Information

The EUT (Equipment Under Test) is Remote Controller. It supports 2.4GHz SDR, 5.1GHz SDR and 5.8GHz SDR.

1.2.2. Wireless Technologies

General Information of EUT	Value
Kind of Equipment	Remote Controller
Type Designation	YZAWZJO
FCC ID	2BRGW-YZAWZJO
Operating Voltage	AC 100-240V, 50/60Hz input via AC/DC adapter` or Battery operated (DC 3.6V)
Testing Voltage	AC 120V, 60Hz or Built-in battery
Operating Temperature Range	-10°C ~ 40 °C
Radiofrequency operating mode	1) 2.4GHz SDR: operating within 2400-2483.5MHz, supports 1.4MHz/3MHz/5MHz/10MHz/20MHz/40MHz/60MHz Bandwidth 2) 5.1GHz SDR: operating within 5150-5250MHz, supports 10MHz/20MHz/40MHz Bandwidth 3) 5.8GHz SDR: operating within 5725-5850MHz, supports 1.4MHz/3MHz/5MHz/10MHz/20MHz/40MHz/60MHz/80MHz Bandwidth
Technical Specification of 2.4GHz SDR	
Operating Frequency	2403.5-2467.5MHz for 1.4MHz Bandwidth 2405.5-2465.5MHz for 3MHz Bandwidth 2404.5-2469.5MHz for 5MHz Bandwidth 2407.5-2467.5MHz for 10MHz Bandwidth 2412.5-2462.5MHz for 20MHz Bandwidth 2422.5-2452.5MHz for 40MHz Bandwidth 2432.5-2442.5MHz for 60MHz Bandwidth
Type of Modulation	OFDM
Channel Number	34 channels for 1.4MHz Bandwidth 21 channels for 3MHz Bandwidth 14 channels for 5MHz Bandwidth 61 channels for 10MHz Bandwidth 51 channels for 20MHz Bandwidth 31 channels for 40MHz Bandwidth 11 channels for 60MHz Bandwidth
Antenna Type	Integral Antennas
Antenna Number	1Tx1Rx for SISO mode (ANT1 or ANT0) 2Tx2Rx for MIMO mode (ANT1+ANT0, completely uncorrelated signals)
Antenna Gain	3 dBi for ANT1/0(Provided by the Client)
The type of wideband data transmission equipment:	DTS
Technical Specification of 5.1GHz SDR	
Operating Frequency	5157-5245MHz for 10MHz Bandwidth 5161-5240MHz for 20MHz Bandwidth 5170-5230MHz for 40MHz Bandwidth
Type of Modulation	OFDM
Channel Number	89 channels for 10MHz Bandwidth 80 channels for 20MHz Bandwidth

	61 channels for 40MHz Bandwidth
Antenna Type	Integral Antenna
Antenna Number	1Tx1Rx for SISO mode (ANT1 or ANT0) 2Tx2Rx for MIMO mode (ANT1+ANT0, Completely uncorrelated signals)
Antenna Gain	1.5 dBi for ANT1/0(Provided by the Client)
The type of wideband data transmission equipment	NII
Technical Specification of 5.8GHz SDR	
Operating Frequency	5728.5-5844.5MHz for 1.4MHz Bandwidth 5727.5-5844.5MHz for 3MHz Bandwidth 5732.5-5842.5MHz for 5MHz Bandwidth 5730.5-5844.5MHz for 10MHz Bandwidth 5735.5-5839.5MHz for 20MHz Bandwidth 5745.5-5829.5MHz for 40MHz Bandwidth 5755.5-5819.5MHz for 60MHz Bandwidth 5765.5-5809.5MHz for 80MHz Bandwidth
Type of Modulation	OFDM
Channel Number	59 channels for 1.4MHz Bandwidth 40 channels for 3MHz Bandwidth 23 channels for 5MHz Bandwidth 115 channels for 10MHz Bandwidth 105 channels for 20MHz Bandwidth 85 channels for 40MHz Bandwidth 65 channels for 60MHz Bandwidth 45 channels for 80MHz Bandwidth
Antenna Type	Integral Antenna
Antenna Number	1Tx1Rx for SISO mode (ANT1 or ANT0) 2Tx2Rx for MIMO mode (ANT1+ANT0, Completely uncorrelated signals)
Antenna Gain	4 dBi for ANT1/0(Provided by the Client)
The type of wideband data transmission equipment	NII

Note:

- The above EUT information is declared by manufacturer and for more detailed features description please refers to the manufacturer's specifications or User's Manual.

2. Test Sites

2.1. Test Facilities

Error! Reference source not found.

2-3F, 101 & 102, No.2, Nuclear Power Industrial Park, Fuming Community, Fucheng Street, Longhua District, Shenzhen 518000, People's Republic of China

A2LA Cert. No.: 5162.01

FCC Registration No.: 694916

IC Registration No.: 25069

2.2. Ambient Condition

Ambient Temperature	20.9°C
Relative Humidity	48%

2.3. List of Test and Measurement Instruments

Equipment	Manufacturer	Model	SN	Cal. Date	Cal. Interval
System Validation Dipole	SPEAG	D2450V2	1014	Jun. 06, 2024	3 years
System Validation Dipole	SPEAG	D5GHzV2	1280	Jun. 06, 2024	3 years
Dosimetric E-Field Probe	SPEAG	EX3DV4	7506	Nov. 12, 2024	1 year
Data Acquisition Electronics	SPEAG	DAE4	1557	Oct. 08, 2024	1 year
Signal Analyzer	R&S	FSV 7	103665	Sep. 29, 2024	1 year
Vector Network Analyzer	R&S	ZNB 8	107040	Sep. 29, 2024	1 year
Dielectric assessment Kit	SPEAG	DAK-3.5	1269	Oct. 09, 2024	1 year
Signal Generator	R&S	SMB 100A	180840	Sep. 29, 2024	1 year
EPM Series Power Meter	Keysight	N1914A	MY58240005	Oct. 29, 2024	1 year
Power Sensor	Keysight	N8481H	MY58250002	Oct. 29, 2024	1 year
Power Sensor	Keysight	N8481H	MY58250006	Oct. 29, 2024	1 year
DC Power Supply	Topward	3303D	809332	Oct. 29, 2024	1 year
Coaxial Directional Coupler	Keysight	773D	MY52180552	Oct. 29, 2024	1 year
Coaxial Directional Coupler	shhuaxiang	DTO-0.4/3.9-10	18052101	Oct. 29, 2024	1 year
Coaxial attenuator	Keysight	8491A	MY52463219	Oct. 29, 2024	1 year
Coaxial attenuator	Keysight	8491A	MY52463210	Oct. 29, 2024	1 year
Coaxial attenuator	Keysight	8491A	MY52463222	Oct. 29, 2024	1 year
Digital Thermometer	LKM	DTM3000	3116	Nov. 04, 2024	1 year
Power Amplifier Mini circuit	mini-circuits	ZHL-42W	SN002101809	N/A	N/A
Power Amplifier Mini circuit	mini-circuits	ZVE-8G	SN070501814	N/A	N/A
PHANTOM	SPEAG	ELI V8.0	2094	N/A	N/A
PHANTOM	SPEAG	SAM-Twin V8.0	1961	N/A	N/A

3. Measurement Uncertainty

Source of Uncertainty	Tolerance (± %)	Probability Distribution	Divisor	Ci (1g)	Ci (10g)	Standard Uncertainty (1g)	Standard Uncertainty (10g)	Vi Veff
Measurement System Errors								
Probe Calibration	±12.7%	Normal (k=2)	2	1	1	± 6.35 %	± 6.35 %	∞
Probe Calibration Drift	±1.7%	Rectangular	√3	1	1	±1.0%	±1.0%	∞
Probe Linearity	±4.7%	Rectangular	√3	1	1	±2.7%	±2.7%	∞
Broadband Signal	±3.0%	Rectangular	√3	1	1	±1.7%	±1.7%	∞
Probe Isotropy	±7.6%	Rectangular	√3	1	1	±4.4%	±4.4%	∞
Other Probe + Electronic	±0.7%	Normal	1	1	1	±0.7%	±0.7%	∞
RF Ambient	±1.8%	Normal	1	1	1	±1.8%	±1.8%	∞
Probe Positioning	±0.006mm	Normal	1	0.14	0.14	±0.10%	±0.10%	∞
Data Processing	±1.2%	Normal	1	1	1	±1.2%	±1.2%	∞
Phantom and Device Errors								
Conductivity (meas.) ^{DAK}	±2.5%	Normal	1	0.78	0.71	±2.0%	±1.8%	100
Conductivity (temp.) ^{BB}	±3.3%	Rectangular	√3	0.78	0.71	±1.5%	±1.4%	∞
Phantom Permittivity	±14.0%	Rectangular	√3	0	0	±0%	±0%	∞
Distance DUT – TSL	±2.0%	Normal	1	2	2	±4.0%	±4.0%	∞
Device Positioning	±2.4%/±2.8%	Normal	1	1	1	±2.8%	±2.8%	30
Device Holder	±3.4%/±3.5%	Normal	1	1	1	±3.5%	±3.5%	30
DUT Modulation ^m	±2.4%	Rectangular	√3	1	1	±1.4%	±1.4%	∞
Time-average SAR	±1.7%	Rectangular	√3	1	1	±1.0%	±1.0%	∞
DUT drift	±2.5%	Normal	1	1	1	±2.5%	±2.5%	30
Val Antenna Unc. ^{val}	±0.0%	Normal	1	1	1	±0%	±0%	
Unc. Input Power ^{val}	±0.0%	Normal	1	1	1	±0%	±0%	
Correction to the SAR results								
C(ε,σ)	±1.9%	Normal	1	1	0.84	±1.9%	±1.6%	
SAR scaling ^p	±0.0%	Rectangular	√3	1	1	±0%	±0%	
Combined Standard Uncertainty (K = 1)						±12.54%	±12.44%	
Expanded Uncertainty (K = 2)						±25.1%	±24.9%	

Uncertainty budget for frequency range 300 MHz to 3 GHz

Source of Uncertainty	Tolerance (± %)	Probability Distribution	Divisor	Ci (1g)	Ci (10g)	Standard Uncertainty (1g)	Standard Uncertainty (10g)	Vi Veff
Measurement System Errors								
Probe Calibration	±13.9%	Normal (k=2)	2	1	1	± 6.95 %	± 6.95 %	∞
Probe Calibration Drift	±1.7%	Rectangular	√3	1	1	±1.0%	±1.0%	∞
Probe Linearity	±4.7%	Rectangular	√3	1	1	±2.7%	±2.7%	∞
Broadband Signal	±2.6%	Rectangular	√3	1	1	±1.5%	±1.5%	∞
Probe Isotropy	±7.6%	Rectangular	√3	1	1	±4.4%	±4.4%	∞
Other Probe + Electronic	±1.2%	Normal	1	1	1	±1.2%	±1.2%	∞
RF Ambient	±1.8%	Normal	1	1	1	±1.8%	±1.8%	∞
Probe Positioning	±0.005mm	Normal	1	0.29	0.29	±0.15%	±0.15%	∞
Data Processing	±2.3%	Normal	1	1	1	±2.3%	±2.3%	∞
Phantom and Device Errors								
Conductivity (meas.) ^{DAK}	±2.5%	Normal	1	0.78	0.71	±2.0%	±1.8%	60
Conductivity (temp.) ^{BB}	±3.3%	Rectangular	√3	0.78	0.71	±1.5%	±1.4%	∞
Phantom Permittivity	±14.0%	Rectangular	√3	0.25	0.25	±2%	±2%	∞
Distance DUT – TSL	±2.0%	Normal	1	2	2	±4.0%	±4.0%	∞
Device Positioning	±2.4%/±2.8%	Normal	1	1	1	±2.8%	±2.8%	30
Device Holder	±3.4%/±3.5%	Normal	1	1	1	±3.5%	±3.5%	30
DUT Modulation ^m	±2.4%	Rectangular	√3	1	1	±1.4%	±1.4%	∞
Time-average SAR	±1.7%	Rectangular	√3	1	1	±1.0%	±1.0%	∞
DUT drift	±2.5%	Normal	1	1	1	±2.5%	±2.5%	30
Val Antenna Unc. ^{val}	±0.0%	Normal	1	1	1	±0%	±0%	
Unc. Input Power ^{val}	±0.0%	Normal	1	1	1	±0%	±0%	
Correction to the SAR results								
Deviation to Target	±1.9%	Normal	1	1	0.84	±1.9%	±1.6%	
SAR scaling ^p	±0.0%	Rectangular	√3	1	1	±0%	±0%	
Combined Standard Uncertainty (K = 1)						±12.8%	±12.7%	
Expanded Uncertainty (K = 2)						±25.6%	±25.4%	

Uncertainty budget for frequency range 3 GHz to 6 GHz

4. Test Specification, Methods and Procedures

The tests documented in this report were performed in accordance with FCC 47 CFR § 2.1093, IEEE STD 1528- 2013, the following FCC Published RF exposure KDB procedures & manufacturer KDB inquiries:

- KDB 865664 D01 SAR Measurement 100 MHz to 6 GHz v01r04
- KDB 865664 D02 RF Exposure Reporting v01r02
- KDB 447498 D04 Interim General RF Exposure Guidance v01

In addition to the above, the following information was used:

- [TCB workshop](#) April, 2019; Page 19, Tissue Simulating Liquids(TSL)

5. SAR Measurement System

5.1. Definition of Specific Absorption Rate (SAR)

SAR is related to the rate at which energy is absorbed per unit mass in an object exposed to a radio field. The SAR distribution in a biological body is complicated and is usually carried out by experimental techniques or numerical modeling. The standard recommends limits for two tiers of groups, occupational/controlled and general population/uncontrolled, based on a person's awareness and ability to exercise control over his or her exposure. In general, occupational/controlled exposure limits are higher than the limits for general population/uncontrolled.

The SAR definition is the time derivative (rate) of the incremental energy (dW) absorbed by (dissipated in) an incremental mass (dm) contained in a volume element (dv) of a given density (ρ). The equation description is as below:

$$\text{SAR} = \frac{d}{dt} \left(\frac{dW}{dm} \right) = \frac{d}{dt} \left(\frac{dW}{\rho dv} \right)$$

SAR is expressed in units of Watts per kilogram (W/kg)


SAR measurement can be related to the electrical field in the tissue by

$$\text{SAR} = \frac{\sigma |E|^2}{\rho}$$

Where: σ is the conductivity of the tissue, ρ is the mass density of the tissue and E is the RMS electrical field strength.

5.2. SPEAG DASY System

DASY system consists of high precision robot, probe alignment sensor, phantom, robot controller, controlled measurement server and near-field probe. The robot includes six axes that can move to the precision position of the DASY5 software defined. The DASY software can define the area that is detected by the probe. The robot is connected to controlled box. Controlled measurement server is connected to the controlled robot box. The DAE includes amplifier, signal multiplexing, AD converter, offset measurement and surface detection. It is connected to the Electro-optical coupler (ECO). The ECO performs the conversion from the optical into digital electric signal of the DAE and transfers data to the PC.

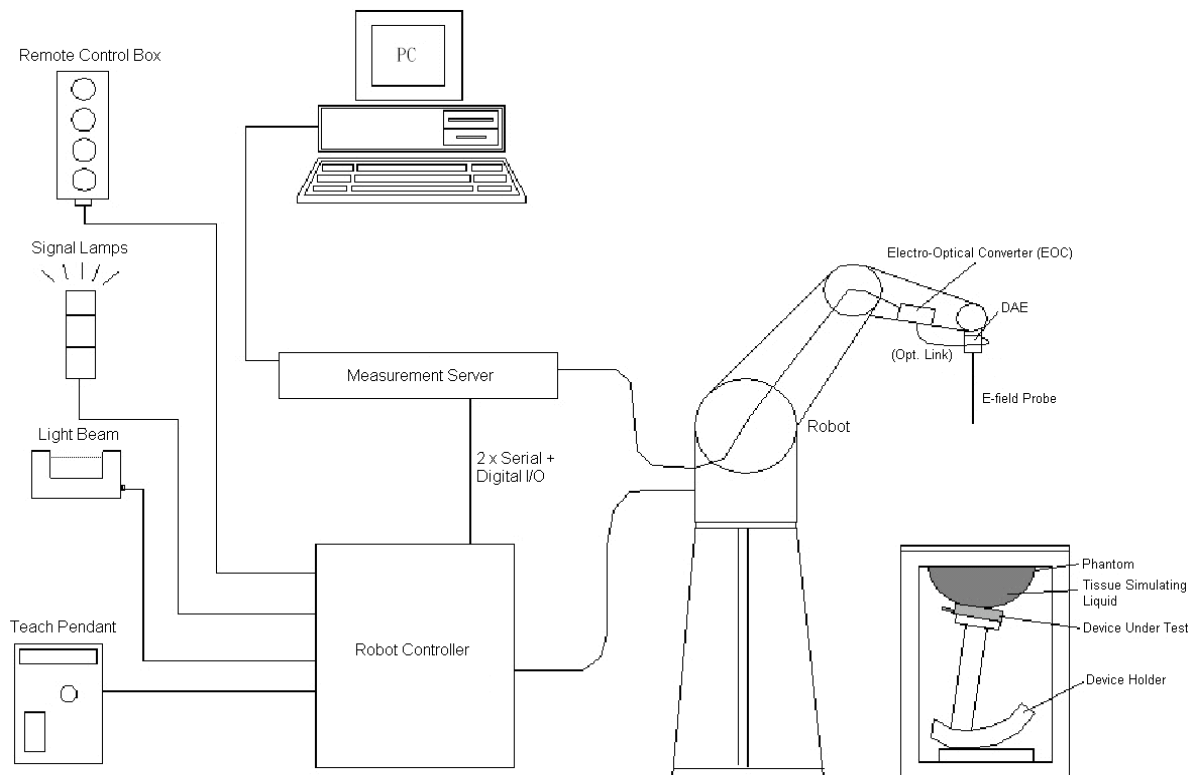


DASY System Setup

5.2.1. Robot

The DASY system uses the high precision robots from Stäubli SA (France). For the 6-axis controller system, the robot controller version (DASY5: CS8c) from Stäubli is used. The Stäubli robot series have many features that are important for our application:

- High precision (repeatability ± 0.035 mm)
- High reliability (industrial design)
- Jerk-free straight movements
- Low ELF interference (the closed metallic construction shields against motor control fields)

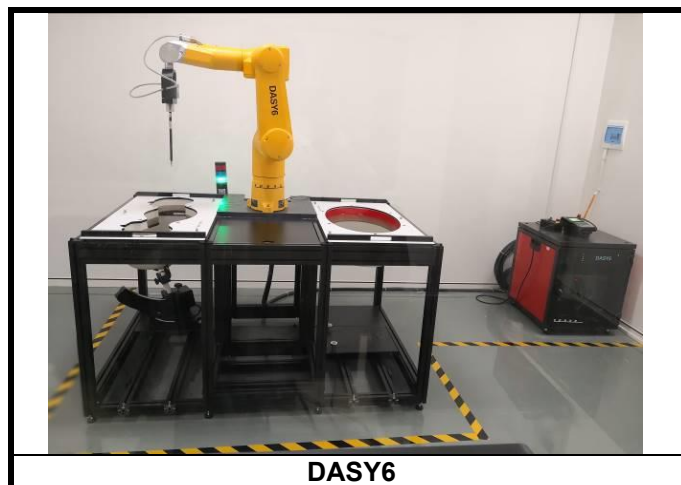

DASY6

5.2.2. Probes

The SAR measurement is conducted with the dosimetric probe. The probe is specially designed and calibrated for use in liquid with high permittivity. The dosimetric probe has special calibration in liquid at different frequency.

Model	EX3DV4	
Construction	Symmetrical design with triangular core. Built-in shielding against static charges. PEEK enclosure material (resistant to organic solvents, e.g., DGBE).	
Frequency	4 MHz – 10 GHz Linearity: ± 0.2 dB (30 MHz – 10 GHz)	
Directivity	± 0.1 dB in TSL (rotation around probe axis) ± 0.3 dB in TSL (rotation normal to probe axis)	
Dynamic Range	10 μ W/g – >100 mW/g Linearity: ± 0.2 dB (noise: typically <1 μ W/g)	
Dimensions	Overall length: 337 mm (tip: 20 mm) Tip diameter: 2.5 mm (body: 12 mm) Typical distance from probe tip to dipole centers: 1 mm	

5.2.3. Data Acquisition Electronics (DAE)

Model	DAE4	
Construction	Signal amplifier, multiplexer, A/D converter and control logic. Serial optical link for communication with DASY embedded system (fully remote controlled). Two step probe touch detector for mechanical surface detection and emergency robot stop.	
Measurement Range	-100 to +300 mV (16 bit resolution and two range settings: 4mV, 400mV)	
Input Offset Voltage	< 5 μ V (with auto zero)	
Input Bias Current	< 50 fA	
Dimensions	60 x 60 x 68 mm	

5.2.4. Phantoms

Model	Twin SAM	
Construction	The shell corresponds to the specifications of the Specific Anthropomorphic Mannequin (SAM) phantom defined in IEC/IEEE 62209-1528. It enables the dosimetric evaluation of left and right hand phone usage as well as body-mounted usage at the flat phantom region. A cover prevents evaporation of the liquid. Reference markings on the phantom allow the complete setup of all predefined phantom positions and measurement grids by teaching three points with the robot.	
Material	Vinylester, glass fiber reinforced (VE-GF)	
Shell Thickness	2 ± 0.2 mm (6 ± 0.2 mm at ear point)	
Dimensions	Length: 1000 mm Width: 500 mm Height: adjustable feet	
Filling Volume	approx. 25 liters	

Model	ELI	
Construction	The ELI phantom is used for compliance testing of handheld and body-mounted wireless devices in the frequency range of 4 MHz to 10 GHz. ELI is fully compatible with the IEC/IEEE 62209-1528 standard and all known tissue simulating liquids. ELI has been optimized regarding its performance and can be integrated into our standard phantom tables. A cover prevents evaporation of the liquid. Reference markings on the phantom allow installation of the complete setup, including all predefined phantom positions and measurement grids, by teaching three points. The phantom is compatible with all of SPEAG's dosimetric probes and dipoles.	
Material	Vinylester, glass fiber reinforced (VE-GF)	
Shell Thickness	2.0 ± 0.2 mm (bottom plate)	
Dimensions	Major axis: 600 mm Minor axis: 400 mm	
Filling Volume	approx. 30 liters	

5.2.5. Device Holder

Model	Mounting Device	
Construction	In combination with the Twin SAM Phantom or ELI4, the Mounting Device enables the rotation of the mounted transmitter device in spherical coordinates. Rotation point is the ear opening point. Transmitter devices can be easily and accurately positioned according to IEC, IEEE, FCC or other specifications. The device holder can be locked for positioning at different phantom sections (left head, right head, flat).	
Material	POM	

Model	Laptop Extensions Kit	
Construction	Simple but effective and easy-to-use extension for Mounting Device that facilitates the testing of larger devices according to IEC 62209-1528 (e.g., laptops, cameras, etc.). It is lightweight and fits easily on the upper part of the Mounting Device in place of the phone positioner.	
Material	POM, Acrylic glass, Foam	

5.2.6. System Validation Dipoles

Model	D-Serial	
Construction	Symmetrical dipole with 1/4 balun. Enables measurement of feed point impedance with NWA. Matched for use near flat phantoms filled with tissue simulating solutions.	
Frequency	750 MHz to 5800 MHz	
Return Loss	> 20 dB	
Power Capability	> 100 W (f < 1GHz), > 40 W (f > 1GHz)	

5.2.7. Tissue Simulating Liquids

For SAR measurement of the field distribution inside the phantom, the phantom must be filled with homogeneous tissue simulating liquid to a depth of at least 15 cm. For head SAR testing, the liquid height from the ear reference point (ERP) of the phantom to the liquid top surface is larger than 15 cm. For body SAR testing, the liquid height from the center of the flat phantom to the liquid top surface is larger than 15 cm. The nominal dielectric values of the tissue simulating liquids in the phantom and the tolerance of 5% are listed.

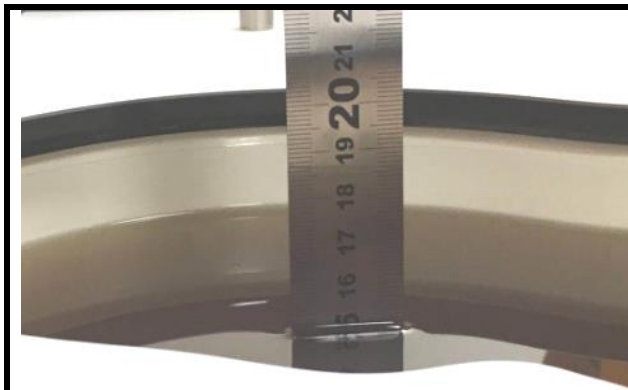


Photo of Liquid Height for Head Position

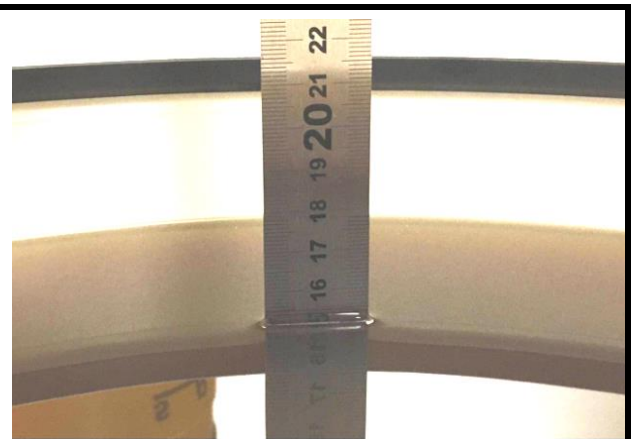


Photo of Liquid Height for Body Position

The dielectric properties of the head tissue simulating liquids are defined in IEEE 1528. The dielectric properties of the tissue simulating liquids were verified prior to the SAR evaluation using a dielectric assessment kit and a network analyzer.

Targets of Tissue Simulating Liquid

Frequency (MHz)	Target Permittivity	Range of $\pm 5\%$	Target Conductivity	Range of $\pm 5\%$
For Head				
750	41.9	39.8 ~ 44.0	0.89	0.85 ~ 0.93
835	41.5	39.4 ~ 43.6	0.90	0.86 ~ 0.95
900	41.5	39.4 ~ 43.6	0.97	0.92 ~ 1.02
1450	40.5	38.5 ~ 42.5	1.20	1.14 ~ 1.26
1640	40.3	38.3 ~ 42.3	1.29	1.23 ~ 1.35
1750	40.1	38.1 ~ 42.1	1.37	1.30 ~ 1.44
1800	40.0	38.0 ~ 42.0	1.40	1.33 ~ 1.47
1900	40.0	38.0 ~ 42.0	1.40	1.33 ~ 1.47
2000	40.0	38.0 ~ 42.0	1.40	1.33 ~ 1.47
2300	39.5	37.5 ~ 41.5	1.67	1.59 ~ 1.75
2450	39.2	37.2 ~ 41.2	1.80	1.71 ~ 1.89
2600	39.0	37.1 ~ 41.0	1.96	1.86 ~ 2.06
3500	37.9	36.0 ~ 39.8	2.91	2.76 ~ 3.06
5200	36.0	34.2 ~ 37.8	4.66	4.43 ~ 4.89
5300	35.9	34.1 ~ 37.7	4.76	4.52 ~ 5.00
5500	35.6	33.8 ~ 37.4	4.96	4.71 ~ 5.21
5600	35.5	33.7 ~ 37.3	5.07	4.82 ~ 5.32
5800	35.3	33.5 ~ 37.1	5.27	5.01 ~ 5.53

The following table gives the recipes for tissue simulating liquids.

Recipes of Tissue Simulating Liquid


Tissue Type	Bactericide	DGBE	HEC	NaCl	Sucrose	Triton X-100	Water	Diethylene Glycol Mono-hexylether
H750	0.2	-	0.2	1.5	56.0	-	42.1	-
H835	0.2	-	0.2	1.5	57.0	-	41.1	-
H900	0.2	-	0.2	1.4	58.0	-	40.2	-
H1450	-	43.3	-	0.6	-	-	56.1	-
H1640	-	45.8	-	0.5	-	-	53.7	-
H1750	-	47.0	-	0.4	-	-	52.6	-
H1800	-	44.5	-	0.3	-	-	55.2	-
H1900	-	44.5	-	0.2	-	-	55.3	-
H2000	-	44.5	-	0.1	-	-	55.4	-
H2300	-	44.9	-	0.1	-	-	55.0	-
H2450	-	45.0	-	0.1	-	-	54.9	-
H2600	-	45.1	-	0.1	-	-	54.8	-
H3500	-	8.0	-	0.2	-	20.0	71.8	-
H5G	-	-	-	-	-	17.2	65.5	17.3

Simulating Head Liquid (HBBL600-6000MHz), Manufactured by SPEAG:

Water (% by weight)	Esters, Emulsifiers, Inhibitors (% by weight)	Sodium salt (% by weight)
50 - 65%	10 - 30%	8 - 25%

5.2.8.SAR System Verification

The system check verifies that the system operates within its specifications. It is performed daily or before every SAR measurement. The system check uses normal SAR measurements in the flat section of the phantom with a matched dipole at a specified distance. The system verification setup is shown as below.

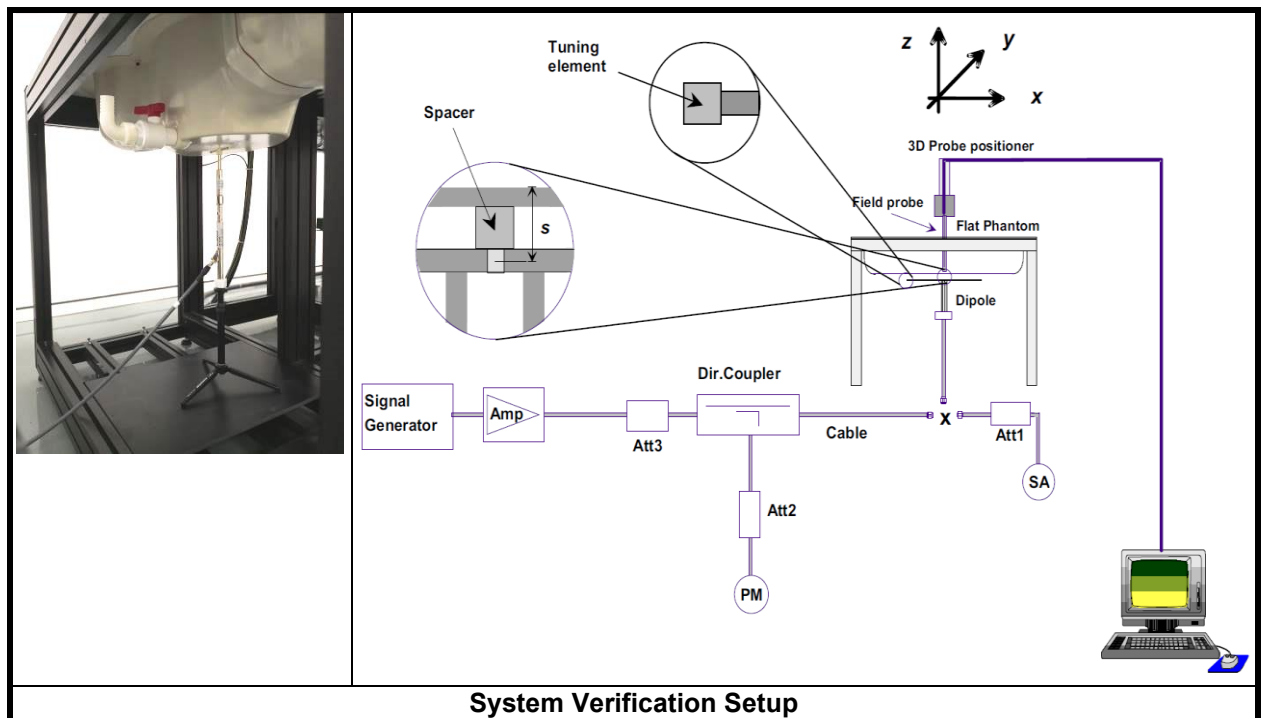

The validation dipole is placed beneath the flat phantom with the specific spacer in place. The distance spacer is touch the phantom surface with a light pressure at the reference marking and be oriented parallel to the long side of the phantom. The spectrum analyzer measures the forward power at the location of the system check dipole connector. The signal generator is adjusted for the desired forward power (250 mW is used for 700 MHz to 2 GHz, 100 mW is used for 2 GHz to 6 GHz) at the dipole connector and the power meter is read at that level. After connecting the cable to the dipole, the signal generator is readjusted for the same reading at power meter.

After system check testing, the SAR result will be normalized to 1W forward input power and compared with the reference SAR value derived from validation dipole certificate report. The deviation of system check should be within 10 %.

6. SAR Measurement Procedure

According to the SAR test standard, the recommended procedure for assessing the peak spatial-average SAR value consists of the following steps:

- (a) Power reference measurement
- (b) Area scan
- (c) Zoom scan
- (d) Power drift measurement

The SAR measurement procedures for each of test conditions are as follows:

- (a) Make EUT to transmit maximum output power
- (b) Measure conducted output power through RF cable
- (c) Place the EUT in the specific position of phantom
- (d) Perform SAR testing steps on the DASY system
- (e) Record the SAR value

6.1. Area & Zoom Scan Procedure

First Area Scan is used to locate the approximate location(s) of the local peak SAR value(s). The measurement grid within an Area Scan is defined by the grid extent, grid step size and grid offset. Next, in order to determine the EM field distribution in a three-dimensional spatial extension, Zoom Scan is required. The Zoom Scan is performed around the highest E-field value to determine the averaged SAR-distribution over 10 g. According to KDB 865664 D01, the resolution for Area and Zoom scan is specified in the table below.

Items	<= 2 GHz	2-3 GHz	3-4 GHz	4-5 GHz	5-6 GHz
Area Scan ($\Delta x, \Delta y$)	<= 15 mm	<= 12 mm	<= 12 mm	<= 10 mm	<= 10 mm
Zoom Scan ($\Delta x, \Delta y$)	<= 8 mm	<= 5 mm	<= 5 mm	<= 4 mm	<= 4 mm
Zoom Scan (Δz)	<= 5 mm	<= 5 mm	<= 4 mm	<= 3 mm	<= 2 mm
Zoom Scan Volume	>= 30 mm	>= 30 mm	>= 28 mm	>= 25 mm	>= 22 mm

Note:

When zoom scan is required and report SAR is <= 1.4 W/kg, the zoom scan resolution of $\Delta x / \Delta y$ (2-3GHz: <= 8 mm, 3-4GHz: <= 7 mm, 4-6GHz: <= 5 mm) may be applied.

6.2. Volume Scan Procedure

The volume scan is used for assess overlapping SAR distributions for antennas transmitting in different frequency bands. It is equivalent to an oversized zoom scan used in standalone measurements. The measurement volume will be used to enclose all the simultaneous transmitting antennas. For antennas transmitting simultaneously in different frequency bands, the volume scan is measured separately in each frequency band. In order to sum correctly to compute the 1g aggregate SAR, the EUT remain in the same test position for all measurements and all volume scan use the same spatial resolution and grid spacing. When all volume scan were completed, the software, SEMCAD postprocessor can combine and subsequently superpose these measurement data to calculating the multiband SAR.

6.3. Power Drift Monitoring

All SAR testing is under the EUT install full charged battery and transmit maximum output power. In DASY measurement software, the power reference measurement and power drift measurement procedures are used for monitoring the power drift of EUT during SAR test. Both these procedures measure the field at a specified reference position before and after the SAR testing. The software will calculate the field difference in dB. If the power drift more than 5%, the SAR will be retested.

6.4. Spatial Peak SAR Evaluation

The procedure for spatial peak SAR evaluation has been implemented according to the test standard. It can be conducted for 1g and 10g, as well as for user-specific masses. The DASY software includes all numerical procedures necessary to evaluate the spatial peak SAR value.

The base for the evaluation is a "cube" measurement. The measured volume must include the 1g and 10g cubes with the highest averaged SAR values. For that purpose, the center of the measured volume is aligned to the interpolated peak SAR value of a previously performed area scan.

The entire evaluation of the spatial peak values is performed within the post-processing engine (SEMCAD). The system always gives the maximum values for the 1g and 10g cubes. The algorithm to find the cube with highest averaged SAR is divided into the following stages:

- (a) Extraction of the measured data (grid and values) from the Zoom Scan
- (b) Calculation of the SAR value at every measurement point based on all stored data (A/D values and measurement parameters)
- (c) Generation of a high-resolution mesh within the measured volume
- (d) Interpolation of all measured values from the measurement grid to the high-resolution grid
- (e) Extrapolation of the entire 3-D field distribution to the phantom surface over the distance from sensor to surface
- (f) Calculation of the averaged SAR within masses of 1g and 10g

6.5. SAR Averaged Methods

In DASY, the interpolation and extrapolation are both based on the modified Quadratic Shepard's method. The interpolation scheme combines a least-square fitted function method and a weighted average method which are the two basic types of computational interpolation and approximation.

Extrapolation routines are used to obtain SAR values between the lowest measurement points and the inner phantom surface. The extrapolation distance is determined by the surface detection distance and the probe sensor offset. The uncertainty increases with the extrapolation distance. To keep the uncertainty within 1% for the 1 g and 10 g cubes, the extrapolation distance should not be larger than 5 mm.

7. SAR Measurement Evaluation

7.1.EUT Configuration and Setting


<Considerations Related to SDR for Setup and Testing>

This device has installed SDR engineering testing software which can provide continuous transmitting RF signal. During SDR SAR testing, this device was operated to transmit continuously at the maximum transmission duty with specified transmission mode, operating frequency, lowest data rate, and maximum output power.

7.2.EUT Testing Position

7.2.1. Body Exposure Conditions

For this device, The antenna bracket is stretchable, We evaluate the normal state and longest state of the antenna stand stretch, SAR evaluation is required on all sides and edges without Top Side with a transmitting antenna within 25 mm from that surface or edge, at 0 mm separation from a flat phantom, Next to the Body exposure requires 1-g SAR, add worst with phone state, for the data modes, wireless technologies and frequency bands supported by the device to determine SAR compliance.

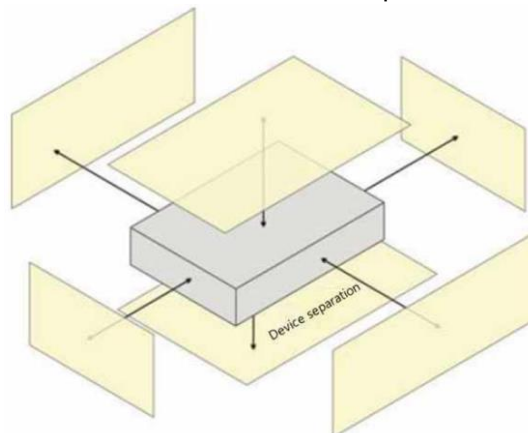

Based on the antenna location shown on Appendix D, the SAR testing required for Body mode is listed as below.

Antenna	Front Face	Rear Face	Left Side	Right Side	Top Side	Bottom Side
SDR antenna	V	V				

7.2.2. Extremity Exposure Conditions

For this device, The antenna bracket is stretchable, We evaluate the normal state and longest state of the antenna stand stretch, SAR evaluation is required on Top Side, at 0 mm separation from a flat phantom, Next to the Hand exposure requires 10-g SAR, add worst with phone state, for the data modes, wireless technologies and frequency bands supported by the device to determine SAR compliance.

7.3. Tissue Verification

The measuring results for tissue simulating liquid are shown as below.

Test Date	Tissue Type	Frequency (MHz)	Measured Conductivity (σ)	Measured Permittivity (ϵ_r)	Target Conductivity (σ)	Target Permittivity (ϵ_r)	Conductivity Deviation (%)	Permittivity Deviation (%)
Sep. 13, 2025	H2450	2450	1.827	37.964	1.80	39.20	1.50	-3.15
Sep. 13, 2025	H5G	5250	4.568	37.454	4.71	35.90	-3.01	4.33
Sep. 13, 2025	H5G	5800	5.165	36.367	5.27	35.30	-1.99	3.02

Note:

The dielectric properties of the tissue simulating liquid must be measured within 24 hours before the SAR testing and within $\pm 5\%$ of the target values. Liquid temperature during the SAR testing must be within $\pm 2^\circ\text{C}$.

7.4. System Validation

The SAR measurement system was validated according to procedures in KDB 865664 D01. The validation status in tabulated summary is as below.

Test Date	Probe S/N	Calibration Point		Measured Conductivity (σ)	Measured Permittivity (ϵ_r)	Validation for CW			Validation for Modulation		
						Sensitivity Range	Probe Linearity	Probe Isotropy	Modulation Type	Duty Factor	PAR
Sep. 13, 2025	7506	Head	2450	1.827	37.964	Pass	Pass	Pass	OFDM	N/A	Pass
Sep. 13, 2025	7506	Head	5250	4.568	37.454	Pass	Pass	Pass	OFDM	N/A	Pass
Sep. 13, 2025	7506	Head	5800	5.165	36.367	Pass	Pass	Pass	OFDM	N/A	Pass

7.5. System Verification

The measuring result for system verification is tabulated as below.

Test Date	Frequency (MHz)	1W Target SAR-1g (W/kg)	Measured SAR-1g (W/kg)	Normalized to 1W SAR-1g (W/kg)	Deviation (%)	Dipole S/N	Probe S/N	DAE S/N
Sep. 13, 2025	2450	51.80	5.21	52.10	0.58	1014	7506	1557
Sep. 13, 2025	5250	79.30	8.05	80.50	1.51	1280	7506	1557
Sep. 13, 2025	5800	80.60	7.86	78.60	-2.48	1280	7506	1557

Note:

Comparing to the reference SAR value provided by SPEAG, the validation data should be within its specification of 10 %. The result indicates the system check can meet the variation criterion and the plots can be referred to Appendix A of this report.

8. SAR Measurement Evaluation

8.1. Conducted Power

All Rate have been tested, the Worst average power (Unit: dBm) is shown as below.

<SDR - 2.4G Ant 1/0>

Testcase	Frequency (MHz)	POWER	Tune-up
SRD 1.4M	2403.5	21.68	22.0
	2437.5	21.88	
	2467.5	21.26	
SRD 3M	2405.5	23.95	24.5
	2435.5	24.02	
	2465.5	23.71	
SRD 5MHz	2404.5	23.76	24.0
	2434.5	23.88	
	2469.5	23.81	
SRD 10MHz	2407.5	19.88	20.5
	2437.5	24.90	25.0
	2467.5	16.94	17.0
SRD 20MHz	2412.5	17.26	18.0
	2437.5	24.61	25.0
	2462.5	13.48	14.0
SRD 40MHz	2422.5	10.80	11.0
	2437.5	18.09	18.5
	2452.5	10.00	10.5
SRD 60MHz	2432.5	10.81	11.5
	2437.5	10.90	
	2442.5	10.92	

<SDR – 5.1G Ant 1/0>

Testcase	Frequency (MHz)	POWER	Tune-up
SRD 10MHz	5157	1.44	2.0
	5200	14.33	15.0
	5245	14.65	
SRD 20MHz	5161	2.16	2.5
	5200	16.6	17.0
	5240	16.07	
SRD 40MHz	5170	6.99	7.5
	5200	16.05	16.5
	5230	16.31	

<SDR – 5.8G Ant 1/0>

Testcase	Frequency (MHz)	POWER	Tune-up
SRD 1.4M	5728.5	23.88	24.0
	5786.5	23.72	
	5844.5	23.75	
SRD 3M	5727.5	24.1	24.5
	5784.5	23.73	
	5844.5	23.93	
SRD 5M	5732.5	23.73	24.0
	5787.5	23.81	
	5842.5	23.66	
SRD 10MHz	5730.5	24.26	24.5
	5787.5	24.05	
	5844.5	24.1	
SRD 20MHz	5735.5	24.28	24.5
	5787.5	24.18	
	5839.5	24.17	
SRD 40MHz	5745.5	19.06	19.5
	5787.5	21.71	22.0
	5829.5	18.68	19.0
SRD 60MHz	5755.5	20.13	20.5
	5787.5	19.53	
	5819.5	19.64	
SRD 80MHz	5765.5	20.09	20.5
	5787.5	19.91	
	5809.5	19.76	

8.2. SAR Testing Results

8.2.1. SAR Test Reduction Considerations

<KDB 447498 D01, General RF Exposure Guidance>

Testing of other required channels within the operating mode of a frequency band is not required when the reported SAR for the mid-band or highest output power channel is:

- (1) ≤ 0.8 W/kg or 2.0 W/kg, for 1-g or 10-g respectively, when the transmission band is ≤ 100 MHz
- (2) ≤ 0.6 W/kg or 1.5 W/kg, for 1-g or 10-g respectively, when the transmission band is between 100 MHz and 200 MHz
- (3) ≤ 0.4 W/kg or 1.0 W/kg, for 1-g or 10-g respectively, when the transmission band is ≥ 200 MHz

8.2.2. SAR Results for Body Exposure Condition (Separation Distance is 0 cm Gap)

Plot No.	Band	Mode	Test Position	Frequency (MHz)	State	Antenna	Normal Duty Cycle	Max. Tune-up Power (dBm)	Measured Conducted Power (dBm)	Scaling Factor	Power Drift (dB)	Measured SAR-1g (W/kg)	Scaled SAR-1g (W/kg)
	SDR 2.4G	20M	Front Face	2437.5	normal	0	10.0%	25.0	24.61	1.09	0.02	0.582	0.06
	SDR 2.4G	20M	Front Face	2437.5	Longest	0	10.0%	25.0	24.61	1.09	0.08	0.579	0.06
	SDR 2.4G	20M	Rear Face	2437.5	normal	0	10.0%	25.0	24.61	1.09	0.01	2.21	0.24
	SDR 2.4G	20M	Rear Face	2437.5	Longest	0	10.0%	25.0	24.61	1.09	0.16	2.34	0.26
	SDR 2.4G	20M	Front Face	2437.5	normal	1	10.0%	25.0	24.61	1.09	0.06	0.566	0.06
	SDR 2.4G	20M	Front Face	2437.5	Longest	1	10.0%	25.0	24.61	1.09	0.04	0.572	0.06
	SDR 2.4G	20M	Rear Face	2437.5	normal	1	10.0%	25.0	24.61	1.09	0.08	2.56	0.28
1	SDR 2.4G	20M	Rear Face	2437.5	Longest	1	10.0%	25.0	24.61	1.09	-0.07	2.6	0.29
	SDR 2.4G	20M	Rear Face	2437.5	With Phone	1	10.0%	25.0	24.61	1.09	0.06	2.54	0.28
	SDR 5.1G	20M	Front Face	5200	normal	0	10.0%	17.0	16.6	1.10	0.05	0.324	0.04
	SDR 5.1G	20M	Front Face	5200	Longest	0	10.0%	17.0	16.6	1.10	0.08	0.335	0.04
	SDR 5.1G	20M	Rear Face	5200	normal	0	10.0%	17.0	16.6	1.10	-0.06	1.41	0.15
2	SDR 5.1G	20M	Rear Face	5200	Longest	0	10.0%	17.0	16.6	1.10	0.08	1.45	0.16
	SDR 5.1G	20M	Front Face	5200	normal	1	10.0%	17.0	16.6	1.10	0.04	0.334	0.04
	SDR 5.1G	20M	Front Face	5200	Longest	1	10.0%	17.0	16.6	1.10	-0.04	0.342	0.04
	SDR 5.1G	20M	Rear Face	5200	normal	1	10.0%	17.0	16.6	1.10	0.02	1.21	0.13
	SDR 5.1G	20M	Rear Face	5200	Longest	1	10.0%	17.0	16.6	1.10	0.14	1.28	0.14
	SDR 5.1G	20M	Rear Face	5200	With Phone	0	10.0%	17.0	16.6	1.10	-0.05	1.42	0.16
	SDR 5.8G	20M	Front Face	5787.5	normal	0	10.0%	24.5	24.18	1.08	0.09	1.33	0.14
	SDR 5.8G	20M	Front Face	5787.5	Longest	0	10.0%	24.5	24.18	1.08	-0.11	1.37	0.15
	SDR 5.8G	20M	Rear Face	5787.5	normal	0	10.0%	24.5	24.18	1.08	0.02	5.78	0.62
	SDR 5.8G	20M	Rear Face	5787.5	Longest	0	10.0%	24.5	24.18	1.08	0.05	5.94	0.64
	SDR 5.8G	20M	Front Face	5787.5	normal	1	10.0%	24.5	24.18	1.08	-0.06	1.74	0.19
	SDR 5.8G	20M	Front Face	5787.5	Longest	1	10.0%	24.5	24.18	1.08	0.04	1.79	0.19
	SDR 5.8G	20M	Rear Face	5787.5	normal	1	10.0%	24.5	24.18	1.08	-0.05	6.32	0.68
3	SDR 5.8G	20M	Rear Face	5787.5	Longest	1	10.0%	24.5	24.18	1.08	-0.03	6.69	0.72
	SDR 5.8G	20M	Rear Face	5787.5	With Phone	1	10.0%	24.5	24.18	1.08	-0.02	6.61	0.71

Note: This device is a hand-held remote controller, all required sides were considered for limb-worn mode with 0mm distance. Only the rear and bottom sides may have probability to keep towards with body/lap, thus body-SAR considered for them as well, detailed description listed on Appendix D.

The side far away from the antenna is not required.

8.2.3.SAR Results for Extremity Exposure Condition (Separation Distance is 0 cm Gap)

Plot No.	Band	Mode	Test Position	Frequency (MHz)	State	Normal Duty Cycle	Normal Duty Cycle	Max. Tune-up Power (dBm)	Measured Conducted Power (dBm)	Scaling Factor	Power Drift (dB)	Measured SAR-10g (W/kg)	Scaled SAR-10g (W/kg)
4	SDR 2.4G	20M	Top Side	2437.5	normal	0	10.00%	25.0	24.61	1.09	0.05	4.36	0.48
	SDR 2.4G	20M	Top Side	2437.5	Longest	0	10.00%	25.0	24.61	1.09	-0.06	4.45	0.49
	SDR 2.4G	20M	Top Side	2437.5	normal	1	10.00%	25.0	24.61	1.09	0.03	4.35	0.47
	SDR 2.4G	20M	Top Side	2437.5	Longest	1	10.00%	25.0	24.61	1.09	0.05	4.25	0.46
	SDR 2.4G	20M	Top Side	2437.5	With Phone	0	10.00%	25.0	24.61	1.09	0.04	4.37	0.48
5	SDR 5.1G	20M	Top Side	5200	normal	0	10.00%	17.0	16.6	1.10	0.06	3.8	0.42
	SDR 5.1G	20M	Top Side	5200	Longest	0	10.00%	17.0	16.6	1.10	-0.01	3.87	0.43
	SDR 5.1G	20M	Top Side	5200	normal	1	10.00%	17.0	16.6	1.10	0.05	3.21	0.35
	SDR 5.1G	20M	Top Side	5200	Longest	1	10.00%	17.0	16.6	1.10	0.04	3.35	0.37
	SDR 5.1G	20M	Top Side	5200	With Phone	0	10.00%	17.0	16.6	1.10	0.08	3.72	0.41
6	SDR 5.8G	20M	Top Side	5787.5	normal	0	10.00%	24.5	24.18	1.05	0.05	12.2	1.28
	SDR 5.8G	20M	Top Side	5787.5	Longest	0	10.00%	24.5	24.18	1.05	-0.02	12.3	1.29
	SDR 5.8G	20M	Top Side	5787.5	normal	1	10.00%	24.5	24.18	1.05	0.04	12.1	1.27
	SDR 5.8G	20M	Top Side	5787.5	Longest	1	10.00%	24.5	24.18	1.05	0.02	12.1	1.27
	SDR 5.8G	20M	Top Side	5787.5	With Phone	0	10.00%	24.5	24.18	1.05	0.01	11.9	1.25

Note: This device is a hand-held remote controller, all required sides were considered for limb-worn mode with 0mm distance. Only the rear and bottom sides may have probability to keep towards with body/lap, thus body-SAR considered for them as well, detailed description listed on Appendix D.

As for SAR evaluations on rear and front sides, they satisfy the body-SAR limit under 0mm distance, thus needless to consider the Extremity Exposure Condition.

The side far away from the antennas is not required.

Max normal duty cycle is 10% for 2.4GHz, 5.1GHz and 5.8GHz SDR bands.

1) 2.4GHz SDR

Ton (ms)	T(Total) ms	Duty cycle (%)
0.502*2	10.2	10%

2) 5.2GHz SDR

Ton (ms)	T(Total) ms	Duty cycle (%)
0.502*2	10.2	10%

2) 5.8GHz SDR

Ton (ms)	T(Total) ms	Duty cycle (%)
0.502*2	10.2	10%

8.2.4. SAR Measurement Variability

According to KDB 865664 D01, SAR measurement variability was assessed for each frequency band, which is determined by the SAR probe calibration point and tissue-equivalent medium used for the device measurements. When both head and body tissue-equivalent media are required for SAR measurements in a frequency band, the variability measurement procedures should be applied to the tissue medium with the highest measured SAR, using the highest measured SAR configuration for that tissue-equivalent medium. Alternatively, if the highest measured SAR for both head and body tissue-equivalent media are ≤ 1.45 W/kg and the ratio of these highest SAR values, i.e., largest divided by smallest value, is ≤ 1.10 , the highest SAR configuration for either head or body tissue-equivalent medium may be used to perform the repeated measurement. These additional measurements are repeated after the completion of all measurements requiring the same head or body tissue-equivalent medium in a frequency band. The test device should be returned to ambient conditions (normal room temperature) with the battery fully charged before it is re-mounted on the device holder for the repeated measurement(s) to minimize any unexpected variations in the repeated results.

Since all the Body SAR are less than 0.8 W/kg and Limb SAR are less than 2.0 W/kg, the repeated measurement is not required.

8.2.5.MIMO Evaluation
<SAR Summation Analysis>

Simultaneous transmission SAR test exclusion is determined for each operating configuration and exposure condition according to the reported standalone SAR of each applicable simultaneous transmitting antenna. When the sum of SAR_{1g} of all simultaneously transmitting antennas in an operating mode and exposure condition combination is within the SAR limit (SAR_{1g} 1.6 W/kg), the simultaneous transmission SAR is not required. When the sum of SAR_{1g} is greater than the SAR limit (SAR_{1g} 1.6 W/kg), SAR test exclusion is determined by the SPLSR.

No.	Conditions (SAR1 + SAR2)	Exposure Condition	Test Position	Max. SAR1	Max. SAR2	SAR Summation	SPLSR Analysis
1	SDR 2.4GHz	Body	Front Face	0.06	0.06	0.12	Σ SAR < 1.6, Not required
			Rear Face	0.26	0.28	0.54	Σ SAR < 1.6, Not required
2	SDR 2.4GHz	Extremity	Top Side	0.48	0.47	0.95	Σ SAR < 4.0, Not required
3	SDR 5.1GHz	Body	Front Face	0.04	0.04	0.08	Σ SAR < 1.6, Not required
			Rear Face	0.16	0.14	0.30	Σ SAR < 1.6, Not required
4	SDR 5.1GHz	Extremity	Top Side	0.43	0.37	0.80	Σ SAR < 4.0 Not required
5	SDR 5.8GHz	Body	Front Face	0.14	0.19	0.33	Σ SAR < 1.6, Not required
			Rear Face	0.64	0.72	1.36	Σ SAR < 1.6, Not required
6	SDR 5.8GHz	Extremity	Top Side	1.30	1.28	2.58	Σ SAR < 4.0, Not required

Test Engineer: Warren Xiong,

Appendixes

All attachments are integral parts of this test report. This applies especially to the following appendix:

Appendix A: SAR Plots of System Verification

The plots for system verification with largest deviation for each SAR system combination are shown as follows.

Appendix B: SAR Plots of SAR Measurement

The SAR plots for highest measured SAR in each exposure configuration, wireless mode and frequency band combination, and measured SAR > 1.5 W/kg are shown as follows.

Appendix C: Calibration Certificate for probe and Dipole

Appendix D: Photographs of EUT and setup

Test Laboratory: TÜV Rheinland (Shenzhen) Co., Ltd.

Date: 2025/9/18

System Check-D2450V2_H2450

DUT: Dipole 2450 MHz D2450V2 SN:1014

Communication System: UID 0, CW; Frequency: 2450 MHz; Duty Cycle: 1:1

Medium: H2450 Medium parameters used: $f = 2450$ MHz; $\sigma = 1.795$ S/m; $\epsilon_r = 38.824$; $\rho = 1000$ kg/m³

DASY5 Configuration:

- Probe: EX3DV4 - SN7506; ConvF(6.78, 7.22, 6.73) @ 2450 MHz; Calibrated: 2024/11/12
- Sensor-Surface: 1.4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn1557; Calibrated: 2024/10/8
- Phantom: SAM 1; Type: QD 000 P40 CB; Serial: 1961
- Measurement SW: DASY52, Version 52.10 (4); SEMCAD X Version 14.6.14 (7483)

Pin=100 mW/Area Scan (71x81x1): Interpolated grid: dx=1.200 mm, dy=1.200 mm

Maximum value of SAR (interpolated) = 8.00 W/kg

Pin=100 mW/Zoom Scan (7x7x7)/Cube 0: Measurement grid: dx=5mm, dy=5mm, dz=5mm

Reference Value = 68.20 V/m; Power Drift = -0.01 dB


Peak SAR (extrapolated) = 9.22 W/kg

SAR(1 g) = 5.15 W/kg; SAR(10 g) = 2.39 W/kg

Smallest distance from peaks to all points 3 dB below = 8.9 mm

Ratio of SAR at M2 to SAR at M1 = 54.6%

Maximum value of SAR (measured) = 7.81 W/kg

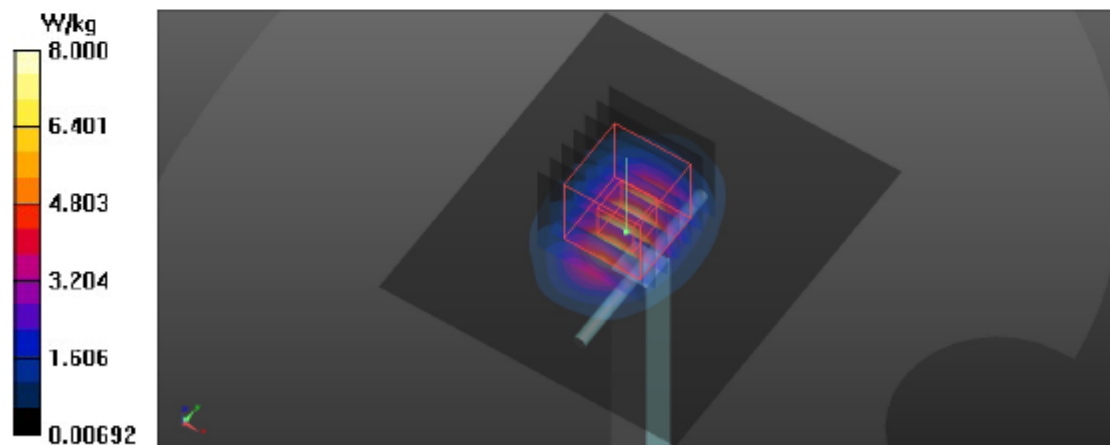

Test Laboratory: TÜV Rheinland (Shenzhen) Co., Ltd.

Date: 2025/9/18

System Check-D5GHz_H5250

DUT: Dipole D5GHzV2 SN:1280

Communication System: UID 0, CW; Frequency: 5250 MHz; Duty Cycle: 1:1


Medium: H5G Medium parameters used: $f = 5250 \text{ MHz}$; $\sigma = 4.561 \text{ S/m}$; $\epsilon_r = 37.438$; $\rho = 1000 \text{ kg/m}^3$

DASY5 Configuration:

- Probe: EX3DV4 - SN7506; ConvF(5.63, 6, 5.58) @ 5250 MHz; Calibrated: 2024/11/12
- Sensor-Surface: 1.4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn1557; Calibrated: 2024/10/8
- Phantom: SAM 1; Type: QD 000 P40 CB; Serial: 1961
- Measurement SW: DASY52, Version 52.10 (4); SEMCAD X Version 14.6.14 (7483)

Pin=100mW/Area Scan (91x91x1): Interpolated grid: $dx=1.000 \text{ mm}$, $dy=1.000 \text{ mm}$
Maximum value of SAR (interpolated) = 19.0 W/kg

Pin=100mW/Zoom Scan (8x8x8)/Cube 0: Measurement grid: $dx=4\text{mm}$, $dy=4\text{mm}$, $dz=1.4\text{mm}$
Reference Value = 66.69 V/m; Power Drift = -0.01 dB
Peak SAR (extrapolated) = 31.8 W/kg
SAR(1 g) = 8.04 W/kg; SAR(10 g) = 2.33 W/kg
Smallest distance from peaks to all points 3 dB below = 7.4 mm
Ratio of SAR at M2 to SAR at M1 = 65.6%
Maximum value of SAR (measured) = 18.4 W/kg

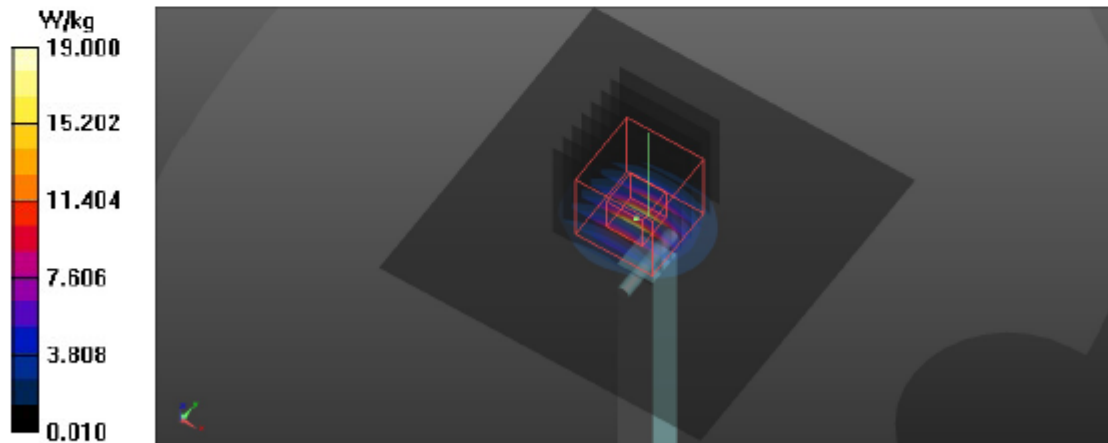

Test Laboratory: TÜV Rheinland (Shenzhen) Co., Ltd.

Date: 2025/9/18

System Check-D5GHz_H5800

DUT: Dipole D5GHzV2 SN:1280

Communication System: UID 0, CW; Frequency: 5800 MHz; Duty Cycle: 1:1

Medium: H5G Medium parameters used: $f = 5800 \text{ MHz}$; $\sigma = 5.145 \text{ S/m}$; $\epsilon_r = 36.469$; $\rho = 1000 \text{ kg/m}^3$

DASY5 Configuration:

- Probe: EX3DV4 - SN7506; ConvF(5.12, 5.45, 5.08) @ 5800 MHz; Calibrated: 2024/11/12
- Sensor-Surface: 1.4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn1557; Calibrated: 2024/10/8
- Phantom: SAM 1; Type: QD 000 P40 CB; Serial: 1961
- Measurement SW: DASY52, Version 52.10 (4); SEMCAD X Version 14.6.14 (7483)

Pin=100mW/Area Scan (91x91x1): Interpolated grid: $dx=1.000 \text{ mm}$, $dy=1.000 \text{ mm}$

Maximum value of SAR (interpolated) = 19.6 W/kg

Pin=100mW/Zoom Scan (8x8x8)/Cube 0: Measurement grid: $dx=4\text{mm}$, $dy=4\text{mm}$, $dz=1.4\text{mm}$

Reference Value = 62.74 V/m; Power Drift = 0.00 dB


Peak SAR (extrapolated) = 35.9 W/kg

SAR(1 g) = 7.83 W/kg; SAR(10 g) = 2.22 W/kg

Smallest distance from peaks to all points 3 dB below = 7.4 mm

Ratio of SAR at M2 to SAR at M1 = 60.8%

Maximum value of SAR (measured) = 18.8 W/kg

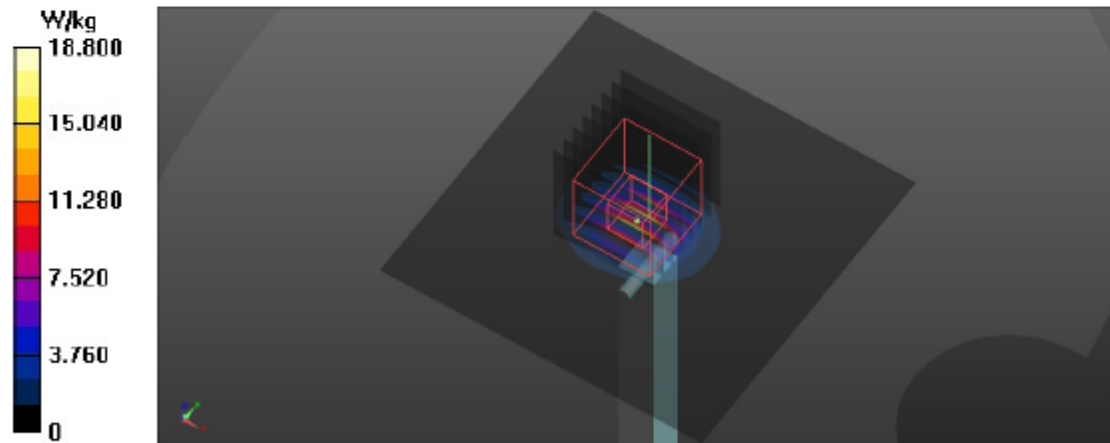

Test Laboratory: TÜV Rheinland (Shenzhen) Co., Ltd.

Date: 2025/9/18

P01 SDR 2.4G_20M_Rear Face_0cm_F 2437.5_Longest_Ant 1

DUT: EUT


Communication System: UID 0, SDR; Frequency: 2437.5 MHz; Duty Cycle: 1:1
Medium: H2450 Medium parameters used: $f = 2437.5$ MHz; $\sigma = 1.781$ S/m; $\epsilon_r = 38.873$; $\rho = 1000$ kg/m³

DASY5 Configuration:

- Probe: EX3DV4 - SN7506; ConvF(6.78, 7.22, 6.73) @ 2437.5 MHz; Calibrated: 2024/11/12
- Sensor-Surface: 1.4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn1557; Calibrated: 2024/10/8
- Phantom: SAM 1; Type: QD 000 P40 CB; Serial: 1961
- Measurement SW: DASY52, Version 52.10 (4); SEMCAD X Version 14.6.14 (7483)

- **Area Scan (81x81x1):** Interpolated grid: $dx=1.200$ mm, $dy=1.200$ mm
Maximum value of SAR (interpolated) = 5.12 W/kg

- **Zoom Scan (7x7x7)/Cube 0:** Measurement grid: $dx=5$ mm, $dy=5$ mm, $dz=5$ mm
Reference Value = 20.02 V/m; Power Drift = -0.07 dB
Peak SAR (extrapolated) = 8.85 W/kg
SAR(1 g) = 2.6 W/kg; SAR(10 g) = 1.15 W/kg
Smallest distance from peaks to all points 3 dB below = 5.2 mm
Ratio of SAR at M2 to SAR at M1 = 36.2%
Maximum value of SAR (measured) = 5.99 W/kg

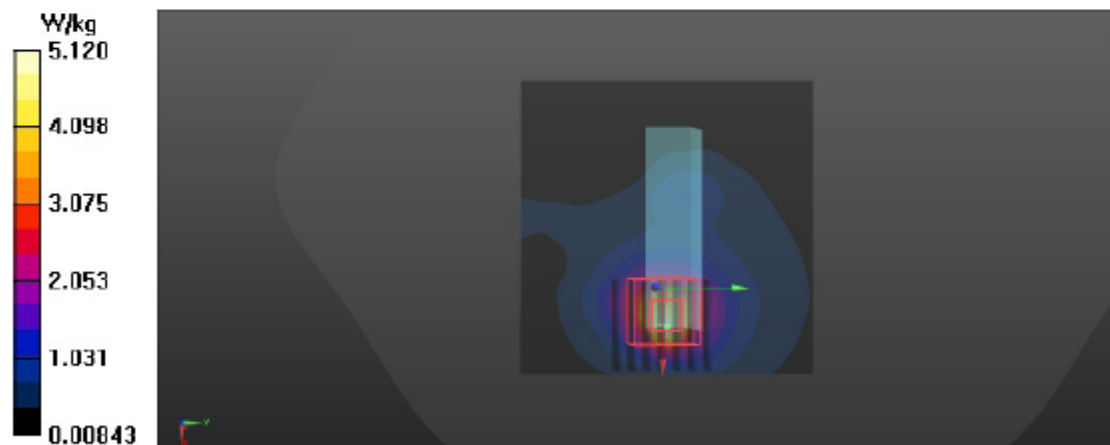

Test Laboratory: TÜV Rheinland (Shenzhen) Co., Ltd.

Date: 2025/9/18

P02 SDR 5.1G_20M_Rear Face_0cm_F 5200_Longest_Ant 0

DUT: EUT

Communication System: UID 0, SDR; Frequency: 5200 MHz; Duty Cycle: 1:1


Medium: H5G Medium parameters used: $f = 5200 \text{ MHz}$; $\sigma = 4.517 \text{ S/m}$; $\epsilon_r = 37.57$; $\rho = 1000 \text{ kg/m}^3$

DASY5 Configuration:

- Probe: EX3DV4 - SN7506; ConvF(5.63, 6, 5.58) @ 5200 MHz; Calibrated: 2024/11/12
- Sensor-Surface: 1.4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn1557; Calibrated: 2024/10/8
- Phantom: SAM 1; Type: QD 000 P40 CB; Serial: 1961
- Measurement SW: DASY52, Version 52.10 (4); SEMCAD X Version 14.6.14 (7483)

- **Area Scan (101x101x1):** Interpolated grid: $dx=1.000 \text{ mm}$, $dy=1.000 \text{ mm}$
Maximum value of SAR (interpolated) = 3.00 W/kg

- **Zoom Scan (8x8x7)/Cube 0:** Measurement grid: $dx=4\text{mm}$, $dy=4\text{mm}$, $dz=1.4\text{mm}$
Reference Value = 17.70 V/m ; Power Drift = 0.08 dB
Peak SAR (extrapolated) = 5.36 W/kg
 $\text{SAR}(1 \text{ g}) = 1.45 \text{ W/kg}$; $\text{SAR}(10 \text{ g}) = 0.603 \text{ W/kg}$
Smallest distance from peaks to all points 3 dB below = 9.6 mm
Ratio of SAR at M2 to SAR at M1 = 62.9%
Maximum value of SAR (measured) = 3.14 W/kg

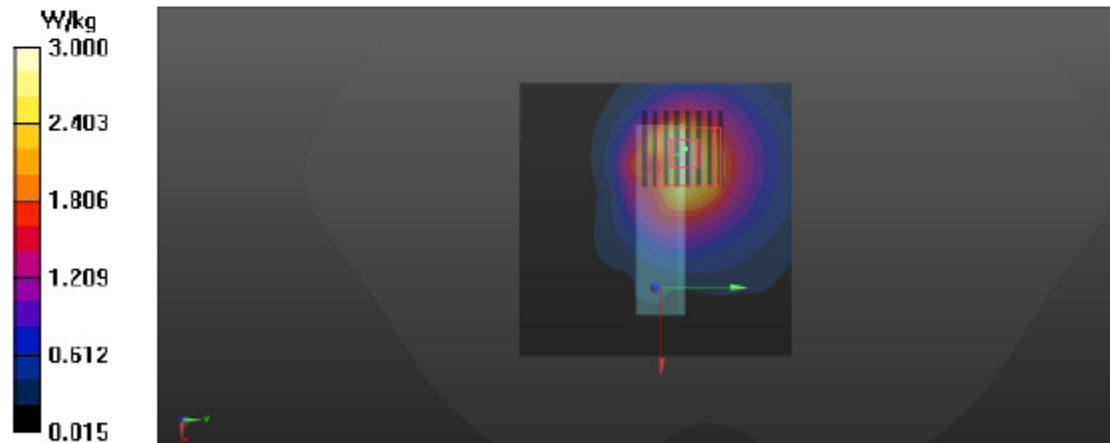

Test Laboratory: TÜV Rheinland (Shenzhen) Co., Ltd.

Date: 2025/9/18

P03 SDR 5.8G_20M_Rear Face_0cm_F 5787.5_Longest_Ant 1

DUT: EUT


Communication System: UID 0, SDR; Frequency: 5787.5 MHz; Duty Cycle: 1:1
Medium: HSG Medium parameters used: $f = 5787.5$ MHz; $\sigma = 5.134$ S/m; $\epsilon_r = 36.488$; $\rho = 1000$ kg/m³

DASY5 Configuration:

- Probe: EX3DV4 - SN7506; ConvF(5.12, 5.45, 5.08) @ 5787.5 MHz; Calibrated: 2024/11/12
- Sensor-Surface: 1.4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn1557; Calibrated: 2024/10/8
- Phantom: SAM 1; Type: QD 000 P40 CB; Serial: 1961
- Measurement SW: DASY52, Version 52.10 (4); SEMCAD X Version 14.6.14 (7483)

- **Area Scan (101x101x1):** Interpolated grid: dx=1.000 mm, dy=1.000 mm
Maximum value of SAR (interpolated) = 15.8 W/kg

- **Zoom Scan (8x8x7)/Cube 0:** Measurement grid: dx=4mm, dy=4mm, dz=1.4mm
Reference Value = 32.96 V/m; Power Drift = -0.03 dB
Peak SAR (extrapolated) = 29.7 W/kg
SAR(1 g) = 6.69 W/kg; SAR(10 g) = 2.73 W/kg
Smallest distance from peaks to all points 3 dB below = 8.7 mm
Ratio of SAR at M2 to SAR at M1 = 57.7%
Maximum value of SAR (measured) = 15.5 W/kg

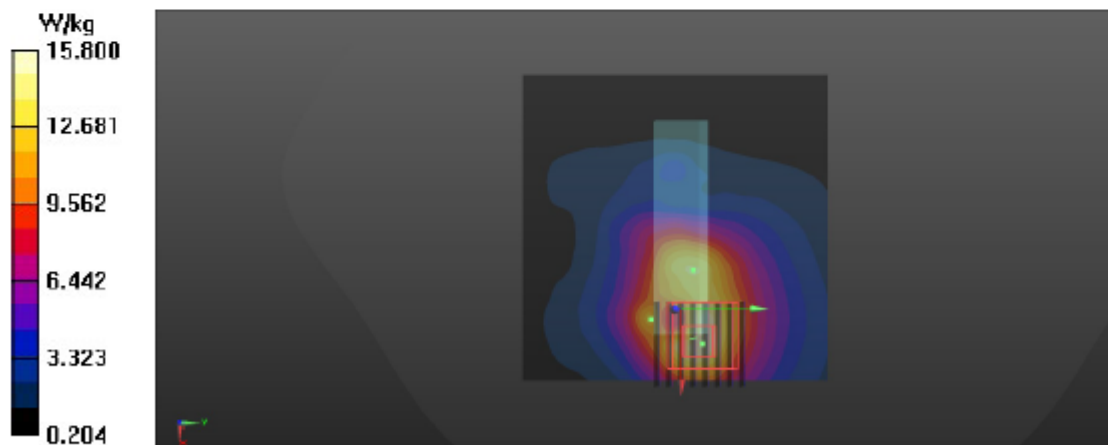

Test Laboratory: TÜV Rheinland (Shenzhen) Co., Ltd.

Date: 2025/9/18

P04 SDR 2.4G_20M_Top Side_0cm_F 2437.5_Longest_Ant 0

DUT: EUT


Communication System: UID 0, SDR; Frequency: 2437.5 MHz; Duty Cycle: 1:1
Medium: H2450 Medium parameters used: $f = 2437.5$ MHz; $\sigma = 1.781$ S/m; $\epsilon_r = 38.873$; $\rho = 1000$ kg/m³

DASY5 Configuration:

- Probe: EX3DV4 - SN7506; ConvF(6.78, 7.22, 6.73) @ 2437.5 MHz; Calibrated: 2024/11/12
- Sensor-Surface: 1.4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn1557; Calibrated: 2024/10/8
- Phantom: SAM 1; Type: QD 000 P40 CB; Serial: 1961
- Measurement SW: DASY52, Version 52.10 (4); SEMCAD X Version 14.6.14 (7483)

- **Area Scan (71x101x1):** Interpolated grid: $dx=1.200$ mm, $dy=1.200$ mm
Maximum value of SAR (interpolated) = 30.3 W/kg

- **Zoom Scan (7x7x7)/Cube 0:** Measurement grid: $dx=5$ mm, $dy=5$ mm, $dz=5$ mm
Reference Value = 22.55 V/m; Power Drift = -0.06 dB
Peak SAR (extrapolated) = 30.4 W/kg
SAR(1 g) = 11.8 W/kg; SAR(10 g) = 4.45 W/kg
Smallest distance from peaks to all points 3 dB below = 7 mm
Ratio of SAR at M2 to SAR at M1 = 40%
Maximum value of SAR (measured) = 23.3 W/kg

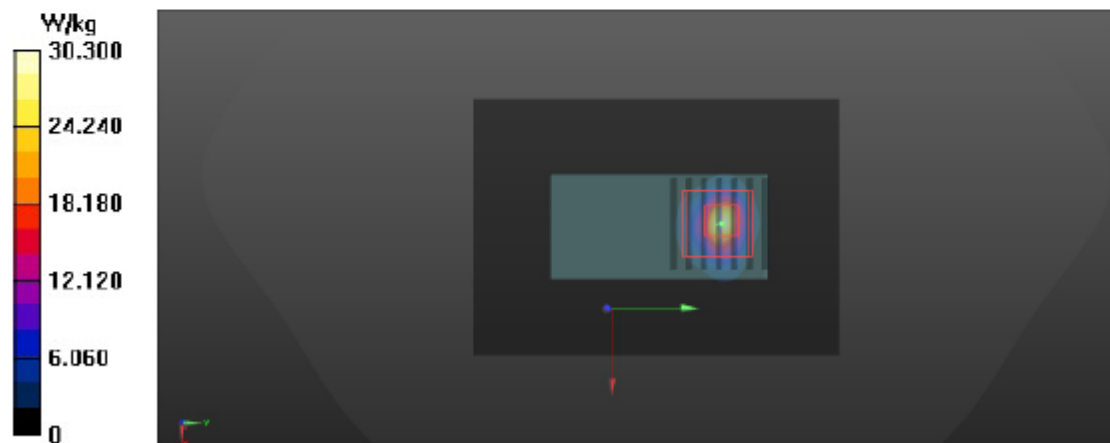

Test Laboratory: TÜV Rheinland (Shenzhen) Co., Ltd.

Date: 2025/9/18

P05 SDR 5.1G_20M_Top Side_0cm_F 5200_Longest

DUT: EUT

Communication System: UID 0, SDR; Frequency: 5200 MHz; Duty Cycle: 1:1

Medium: H5G Medium parameters used: $f = 5200$ MHz; $\sigma = 4.517$ S/m; $\epsilon_r = 37.57$; $\rho = 1000$ kg/m³

DASY5 Configuration:

- Probe: EX3DV4 - SN7506; ConvF(5.63, 6, 5.58) @ 5200 MHz; Calibrated: 2024/11/12
- Sensor-Surface: 1.4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn1557; Calibrated: 2024/10/8
- Phantom: SAM 1; Type: QD 000 P40 CB; Serial: 1961
- Measurement SW: DASY52, Version 52.10 (4); SEMCAD X Version 14.6.14 (7483)

- **Area Scan (81x121x1):** Interpolated grid: $dx=1.000$ mm, $dy=1.000$ mm

Maximum value of SAR (interpolated) = 59.3 W/kg

- **Zoom Scan (8x8x7)/Cube 0:** Measurement grid: $dx=4$ mm, $dy=4$ mm, $dz=1.4$ mm

Reference Value = 7.538 V/m; Power Drift = -0.01 dB


Peak SAR (extrapolated) = 118 W/kg

SAR(1 g) = 19.9 W/kg; SAR(10 g) = 3.87 W/kg

Smallest distance from peaks to all points 3 dB below = 4.9 mm

Ratio of SAR at M2 to SAR at M1 = 59.9%

Maximum value of SAR (measured) = 58.3 W/kg

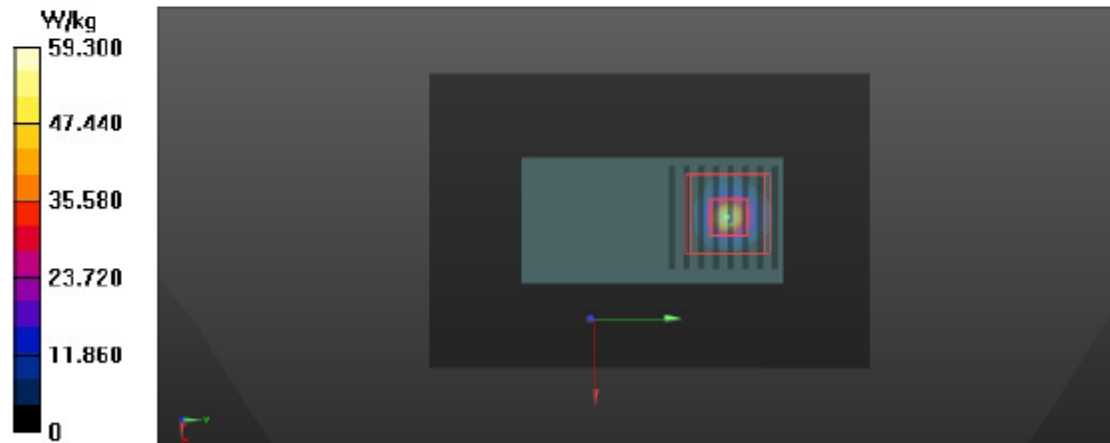

Test Laboratory: TÜV Rheinland (Shenzhen) Co., Ltd.

Date: 2025/9/18

P06 SDR 5.8G_20M_Top Side_0cm_F 5787.5_Longest_Ant 0

DUT: EUT


Communication System: UID 0, SDR; Frequency: 5787.5 MHz; Duty Cycle: 1:1
Medium: HSG Medium parameters used: $f = 5787.5$ MHz; $\sigma = 5.134$ S/m; $\epsilon_r = 36.488$; $\rho = 1000$ kg/m³

DASY5 Configuration:

- Probe: EX3DV4 - SN7506; ConvF(5.12, 5.45, 5.08) @ 5787.5 MHz; Calibrated: 2024/11/12
- Sensor-Surface: 1.4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn1557; Calibrated: 2024/10/8
- Phantom: SAM 1; Type: QD 000 P40 CB; Serial: 1961
- Measurement SW: DASY52, Version 52.10 (4); SEMCAD X Version 14.6.14 (7483)

- **Area Scan (81x121x1):** Interpolated grid: dx=1.000 mm, dy=1.000 mm
Maximum value of SAR (interpolated) = 185 W/kg

- **Zoom Scan (8x8x7)/Cube 0:** Measurement grid: dx=4mm, dy=4mm, dz=1.4mm
Reference Value = 28.49 V/m; Power Drift = -0.02 dB
Peak SAR (extrapolated) = 389 W/kg
SAR(1 g) = 59.1 W/kg; SAR(10 g) = 12.3 W/kg
Smallest distance from peaks to all points 3 dB below = 5.1 mm
Ratio of SAR at M2 to SAR at M1 = 55.6%
Maximum value of SAR (measured) = 160 W/kg

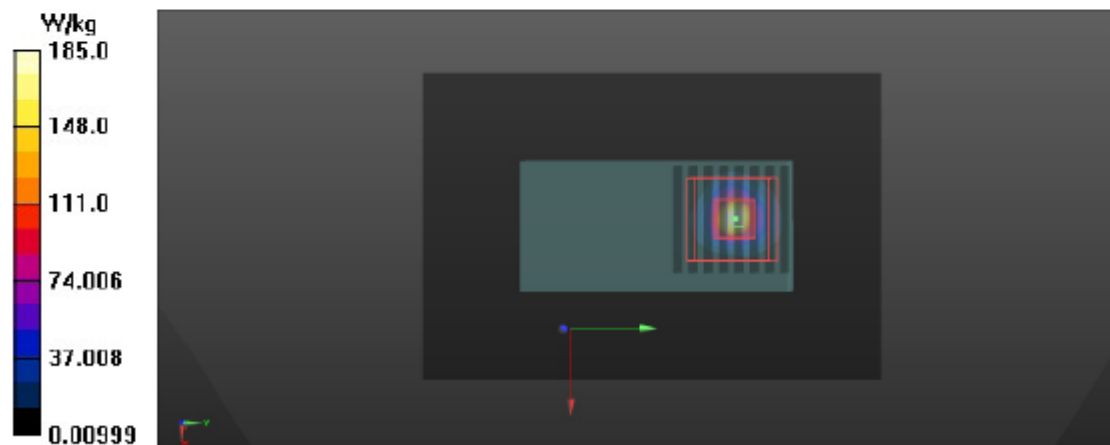

**Calibration Laboratory of
Schmid & Partner
Engineering AG**
Zeughausstrasse 43, 8004 Zurich, Switzerland



S Schweizerischer Kalibrierdienst
C Service suisse d'étalonnage
S Servizio svizzero di taratura
S Swiss Calibration Service

Accreditation No.: **SCS 0108**

Accredited by the Swiss Accreditation Service (SAS)
The Swiss Accreditation Service is one of the signatories to the EA
Multilateral Agreement for the recognition of calibration certificates

Client **TUV**
Shenzhen

Certificate No. **D5GHzV2-1280_Jun24**

CALIBRATION CERTIFICATE

Object **D5GHzV2 - SN:1280**

Calibration procedure(s) **QA CAL-22.v7**
Calibration Procedure for SAR Validation Sources between 3-10 GHz

Calibration date: **June 06, 2024**

This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI).
The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility: environment temperature (22 ± 3)°C and humidity < 70%.

Calibration Equipment used (M&TE critical for calibration)

Primary Standards	ID #	Cal Date (Certificate No.)	Scheduled Calibration
Power meter NRP2	SN: 104778	26-Mar-24 (No. 217-04036/04037)	Mar-25
Power sensor NRP-Z91	SN: 103244	26-Mar-24 (No. 217-04036)	Mar-25
Power sensor NRP-Z91	SN: 103245	26-Mar-24 (No. 217-04037)	Mar-25
Reference 20 dB Attenuator	SN: BH9394 (20k)	26-Mar-24 (No. 217-04046)	Mar-25
Type-N mismatch combination	SN: 310982 / 06327	26-Mar-24 (No. 217-04047)	Mar-25
Reference Probe EX3DV4	SN: 3503	07-Mar-24 (No. EX3-3503_Mar24)	Mar-25
DAE4	SN: 601	22-May-24 (No. DAE4-601_May24)	May-25
Secondary Standards	ID #	Check Date (in house)	Scheduled Check
Power meter E4419B	SN: GB39512475	30-Oct-14 (in house check Oct-22)	In house check: Oct-24
Power sensor HP 8481A	SN: US37292783	07-Oct-15 (in house check Oct-22)	In house check: Oct-24
Power sensor HP 8481A	SN: MY41093315	07-Oct-15 (in house check Oct-22)	In house check: Oct-24
RF generator R&S SMT-06	SN: 100972	15-Jun-15 (in house check Oct-22)	In house check: Oct-24
Network Analyzer Agilent E8358A	SN: US41080477	31-Mar-14 (in house check Oct-22)	In house check: Oct-24

	Name	Function	Signature
Calibrated by:	Joanna Llesha	Laboratory Technician	
Approved by:	Sven Kühn	Technical Manager	

Issued: June 6, 2024

This calibration certificate shall not be reproduced except in full without written approval of the laboratory.

**Calibration Laboratory of
Schmid & Partner
Engineering AG**
Zeughausstrasse 43, 8004 Zurich, Switzerland



S Schweizerischer Kalibrierdienst
C Service suisse d'étalonnage
S Servizio svizzero di taratura
S Swiss Calibration Service

Accredited by the Swiss Accreditation Service (SAS)
The Swiss Accreditation Service is one of the signatories to the EA
Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: **SCS 0108**

Glossary:

TSL	tissue simulating liquid
ConvF	sensitivity in TSL / NORM x,y,z
N/A	not applicable or not measured

Calibration is Performed According to the Following Standards:

- IEC/IEEE 62209-1528, "Measurement Procedure For The Assessment Of Specific Absorption Rate Of Human Exposure To Radio Frequency Fields From Hand-Held And Body-Worn Wireless Communication Devices - Part 1528: Human Models, Instrumentation And Procedures (Frequency Range of 4 MHz to 10 GHz)", October 2020.
- KDB 865664, "SAR Measurement Requirements for 100 MHz to 6 GHz"

Additional Documentation:

- DASY System Handbook

Methods Applied and Interpretation of Parameters:

- Measurement Conditions:** Further details are available from the Validation Report at the end of the certificate. All figures stated in the certificate are valid at the frequency indicated.
- Antenna Parameters with TSL:** The dipole is mounted with the spacer to position its feed point exactly below the center marking of the flat phantom section, with the arms oriented parallel to the body axis.
- Feed Point Impedance and Return Loss:** These parameters are measured with the dipole positioned under the liquid filled phantom. The impedance stated is transformed from the measurement at the SMA connector to the feed point. The Return Loss ensures low reflected power. No uncertainty required.
- Electrical Delay:** One-way delay between the SMA connector and the antenna feed point. No uncertainty required.
- SAR measured:** SAR measured at the stated antenna input power.
- SAR normalized:** SAR as measured, normalized to an input power of 1 W at the antenna connector.
- SAR for nominal TSL parameters:** The measured TSL parameters are used to calculate the nominal SAR result.

The reported uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor $k=2$, which for a normal distribution corresponds to a coverage probability of approximately 95%.

Measurement Conditions

DASY system configuration, as far as not given on page 1.

DASY Version	DASY52	V52.10.4
Extrapolation	Advanced Extrapolation	
Phantom	Modular Flat Phantom V5.0	
Distance Dipole Center - TSL	10 mm	with Spacer
Zoom Scan Resolution	dx, dy = 4.0 mm, dz = 1.4 mm	Graded Ratio = 1.4 (Z direction)
Frequency	5250 MHz ± 1 MHz 5600 MHz ± 1 MHz 5800 MHz ± 1 MHz	

Head TSL parameters at 5250 MHz

The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Head TSL parameters	22.0 °C	35.9	4.71 mho/m
Measured Head TSL parameters	(22.0 ± 0.2) °C	36.0 ± 6 %	4.57 mho/m ± 6 %
Head TSL temperature change during test	< 0.5 °C	----	----

SAR result with Head TSL at 5250 MHz

SAR averaged over 1 cm ³ (1 g) of Head TSL	Condition	
SAR measured	100 mW input power	7.93 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	79.3 W/kg ± 19.9 % (k=2)

SAR averaged over 10 cm ³ (10 g) of Head TSL	condition	
SAR measured	100 mW input power	2.27 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	22.7 W/kg ± 19.5 % (k=2)

Head TSL parameters at 5600 MHz

The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Head TSL parameters	22.0 °C	35.5	5.07 mho/m
Measured Head TSL parameters	(22.0 ± 0.2) °C	35.3 ± 6 %	4.94 mho/m ± 6 %
Head TSL temperature change during test	< 0.5 °C	----	----

SAR result with Head TSL at 5600 MHz

SAR averaged over 1 cm ³ (1 g) of Head TSL	Condition	
SAR measured	100 mW input power	8.35 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	83.3 W/kg ± 19.9 % (k=2)

SAR averaged over 10 cm ³ (10 g) of Head TSL	condition	
SAR measured	100 mW input power	2.38 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	23.7 W/kg ± 19.5 % (k=2)

Head TSL parameters at 5800 MHz

The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Head TSL parameters	22.0 °C	35.3	5.27 mho/m
Measured Head TSL parameters	(22.0 ± 0.2) °C	35.1 ± 6 %	5.15 mho/m ± 6 %
Head TSL temperature change during test	< 0.5 °C	----	----

SAR result with Head TSL at 5800 MHz

SAR averaged over 1 cm ³ (1 g) of Head TSL	Condition	
SAR measured	100 mW input power	8.09 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	80.7 W/kg ± 19.9 % (k=2)

SAR averaged over 10 cm ³ (10 g) of Head TSL	condition	
SAR measured	100 mW input power	2.29 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	22.8 W/kg ± 19.5 % (k=2)

Appendix (Additional assessments outside the scope of SCS 0108)

Antenna Parameters with Head TSL at 5250 MHz

Impedance, transformed to feed point	48.2 Ω - 2.7 j Ω
Return Loss	- 29.5 dB

Antenna Parameters with Head TSL at 5600 MHz

Impedance, transformed to feed point	50.6 Ω + 1.5 j Ω
Return Loss	- 35.7 dB

Antenna Parameters with Head TSL at 5800 MHz

Impedance, transformed to feed point	53.2 Ω + 4.5 j Ω
Return Loss	- 25.5 dB

General Antenna Parameters and Design

Electrical Delay (one direction)	1.188 ns
----------------------------------	----------

After long term use with 100W radiated power, only a slight warming of the dipole near the feedpoint can be measured.

The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals. On some of the dipoles, small end caps are added to the dipole arms in order to improve matching when loaded according to the position as explained in the "Measurement Conditions" paragraph. The SAR data are not affected by this change. The overall dipole length is still according to the Standard.

No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feedpoint may be damaged.

Additional EUT Data

Manufactured by	SPEAG
-----------------	-------

DASY5 Validation Report for Head TSL

Date: 06.06.2024

Test Laboratory: SPEAG, Zurich, Switzerland

DUT: Dipole D5GHzV2; Type: D5GHzV2; Serial: D5GHzV2 - SN:1280

Communication System: UID 0 - CW; Frequency: 5250 MHz, Frequency: 5600 MHz, Frequency: 5800 MHz

Medium parameters used: $f = 5250$ MHz; $\sigma = 4.57$ S/m; $\epsilon_r = 36$; $\rho = 1000$ kg/m³,

Medium parameters used: $f = 5600$ MHz; $\sigma = 4.94$ S/m; $\epsilon_r = 35.3$; $\rho = 1000$ kg/m³,

Medium parameters used: $f = 5800$ MHz; $\sigma = 5.15$ S/m; $\epsilon_r = 35.1$; $\rho = 1000$ kg/m³

Phantom section: Flat Section

Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2011)

DASY52 Configuration:

- Probe: EX3DV4 - SN3503; ConvF(5.39, 5.39, 5.39) @ 5250 MHz, ConvF(5, 5, 5) @ 5600 MHz, ConvF(4.86, 4.86, 4.86) @ 5800 MHz; Calibrated: 07.03.2024
- Sensor-Surface: 1.4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn601; Calibrated: 22.05.2024
- Phantom: Flat Phantom 5.0 (front); Type: QD000P50AA; Serial: 1001
- DASY52 52.10.4(1535); SEMCAD X 14.6.14(7501)

Dipole Calibration for Head Tissue/Pin=100mW, dist=10mm, f=5250 MHz/Zoom Scan, dist=1.4mm (8x8x7)/Cube 0: Measurement grid: dx=4mm, dy=4mm, dz=1.4mm

Reference Value = 76.44 V/m; Power Drift = 0.05 dB

Peak SAR (extrapolated) = 26.9 W/kg

SAR(1 g) = 7.93 W/kg; SAR(10 g) = 2.27 W/kg

Smallest distance from peaks to all points 3 dB below = 6.9 mm

Ratio of SAR at M2 to SAR at M1 = 70.5%

Maximum value of SAR (measured) = 17.6 W/kg

Dipole Calibration for Head Tissue/Pin=100mW, dist=10mm, f=5600 MHz/Zoom Scan, dist=1.4mm (8x8x7)/Cube 0: Measurement grid: dx=4mm, dy=4mm, dz=1.4mm

Reference Value = 76.25 V/m; Power Drift = 0.07 dB

Peak SAR (extrapolated) = 30.8 W/kg


SAR(1 g) = 8.35 W/kg; SAR(10 g) = 2.38 W/kg

Smallest distance from peaks to all points 3 dB below = 7.2 mm


Ratio of SAR at M2 to SAR at M1 = 67.7%

Maximum value of SAR (measured) = 19.1 W/kg

Dipole Calibration for Head Tissue/Pin=100mW, dist=10mm, f=5800 MHz/Zoom Scan, dist=1.4mm (8x8x7)/Cube 0: Measurement grid: dx=4mm, dy=4mm, dz=1.4mm
Reference Value = 74.03 V/m; Power Drift = 0.06 dB
Peak SAR (extrapolated) = 31.7 W/kg
SAR(1 g) = 8.09 W/kg; SAR(10 g) = 2.29 W/kg
Smallest distance from peaks to all points 3 dB below = 7.2 mm
Ratio of SAR at M2 to SAR at M1 = 65.8%
Maximum value of SAR (measured) = 18.9 W/kg

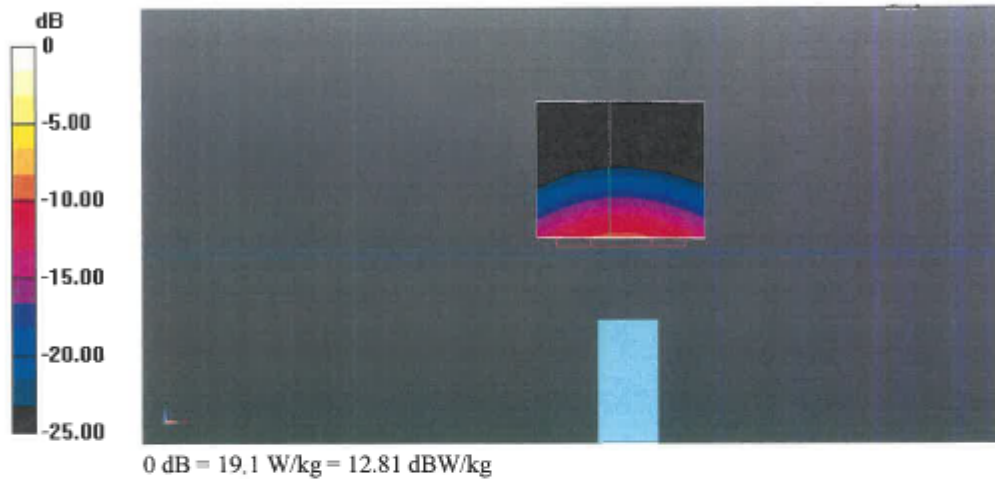

Impedance Measurement Plot for Head TSL

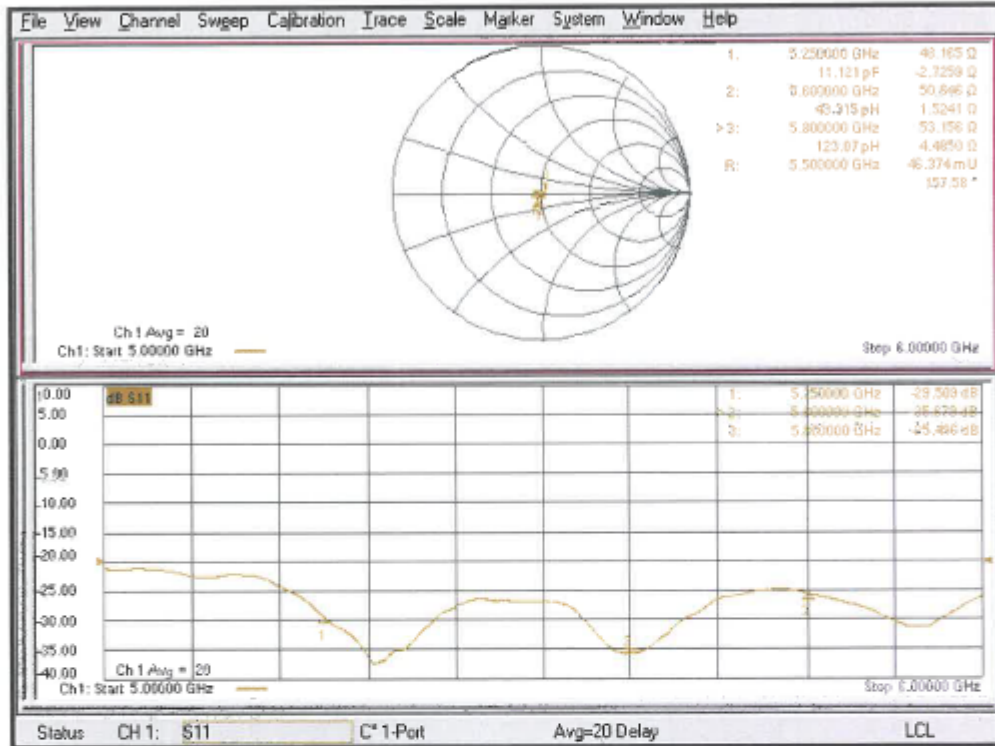

Justification for Extended SAR Dipole Calibrations

Dipole	Date of Measurement	Return Loss (dB)	Delta (%)	Impedance (ohm)	Delta (ohm)
Head 5250MHz	Jun 06, 2024	-29.50	-5.22	48.20	-0.59
	Jun 09, 2025	-27.96		47.61	
Head 5600MHz	Jun 06, 2024	-35.70	-8.68	50.60	-2.04
	Jun 09, 2025	-32.60		48.56	
Head 5800MHz	Jun 06, 2024	-25.50	6.78	53.20	-3.66
	Jun 09, 2025	-27.23		49.54	

Note: The return loss is <-20dB, within 20% of prior calibration; the impedance is within 5 ohm of prior calibration. Therefore the verification results meet the requirement of extended calibration.



**Calibration Laboratory of
Schmid & Partner
Engineering AG**
Zeughausstrasse 43, 8004 Zurich, Switzerland



S Schweizerischer Kalibrierdienst
C Service suisse d'étalonnage
S Servizio svizzero di taratura
S Swiss Calibration Service

Accredited by the Swiss Accreditation Service (SAS)
The Swiss Accreditation Service is one of the signatories to the EA
Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: **SCS 0108**

Client **TUV
Shenzhen**

Certificate No. **EX-7506_Nov24**

CALIBRATION CERTIFICATE

Object **EX3DV4 - SN:7506**

Calibration procedure(s) **QA CAL-01.v10, QA CAL-12.v10, QA CAL-14.v7, QA CAL-23.v6,
QA CAL-25.v8
Calibration procedure for dosimetric E-field probes**

Calibration date **November 12, 2024**

This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI).
The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.
All calibrations have been conducted in the closed laboratory facility: environment temperature $(22 \pm 3)^\circ\text{C}$ and humidity $< 70\%$.
Calibration Equipment used (M&TE critical for calibration)

Primary Standards	ID	Cal Date (Certificate No.)	Scheduled Calibration
Power meter NRP2	SN: 104778	26-Mar-24 (No. 217-04036/04037)	Mar-25
Power sensor NRP-Z91	SN: 103244	26-Mar-24 (No. 217-04036)	Mar-25
OCP DAK-3.5 (weighted)	SN: 1249	23-Sep-24 (OCP-DAK3.5-1249_Sep24)	Sep-25
OCP DAK-12	SN: 1016	24-Sep-24 (OCP-DAK12-1016_Sep24)	Sep-25
Reference 20 dB Attenuator	SN: CC2552 (20x)	26-Mar-24 (No. 217-04046)	Mar-25
DAE4	SN: 660	23-Feb-24 (No. DAE4-660_Feb24)	Feb-25
Reference Probe EX3DV4	SN: 7349	03-Jun-24 (No. EX3-7349_Jun24)	Jun-25

Secondary Standards	ID	Check Date (in house)	Scheduled Check
Power meter E4419B	SN: GB41293874	06-Apr-16 (in house check Jun-24)	In house check: Jun-26
Power sensor E4412A	SN: MY41498087	06-Apr-16 (in house check Jun-24)	In house check: Jun-26
Power sensor E4412A	SN: 000110210	06-Apr-16 (in house check Jun-24)	In house check: Jun-26
RF generator HP 8648C	SN: US3642U01700	04-Aug-99 (in house check Jun-24)	In house check: Jun-26
Network Analyzer E8358A	SN: US41080477	31-Mar-14 (in house check Sep-24)	In house check: Sep-26

	Name	Function	Signature
Calibrated by	Krešimir Franjić	Laboratory Technician	
Approved by	Sven Kühn	Technical Manager	

Issued: November 12, 2024

This calibration certificate shall not be reproduced except in full without written approval of the laboratory.

**Calibration Laboratory of
Schmid & Partner
Engineering AG**

Zeughausstrasse 43, 8004 Zurich, Switzerland



S Schweizerischer Kalibrierdienst
C Service suisse d'étalonnage
S Servizio svizzero di taratura
S Swiss Calibration Service

Accredited by the Swiss Accreditation Service (SAS)
The Swiss Accreditation Service is one of the signatories to the EA
Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: SCS 0108

Glossary

TSL	tissue simulating liquid
NORM _{x,y,z}	sensitivity in free space
ConvF	sensitivity in TSL / NORM _{x,y,z}
DCP	diode compression point
CF	crest factor (1/duty_cycle) of the RF signal
A, B, C, D	modulation dependent linearization parameters
Polarization φ	φ rotation around probe axis
Polarization θ	θ rotation around an axis that is in the plane normal to probe axis (at measurement center), i.e., $\theta = 0$ is normal to probe axis
Connector Angle	information used in DASY system to align probe sensor X to the robot coordinate system

Calibration is Performed According to the Following Standards:

- IEC/IEEE 62209-1528, "Measurement Procedure For The Assessment Of Specific Absorption Rate Of Human Exposure To Radio Frequency Fields From Hand-Held And Body-Worn Wireless Communication Devices – Part 1528: Human Models, Instrumentation And Procedures (Frequency Range of 4 MHz to 10 GHz)", October 2020.
- KDB 865664, "SAR Measurement Requirements for 100 MHz to 6 GHz"

Methods Applied and Interpretation of Parameters:

- NORM_{x,y,z}**: Assessed for E-field polarization $\theta = 0$ ($f \leq 900$ MHz in TEM-cell; $f > 1800$ MHz: R22 waveguide). NORM_{x,y,z} are only intermediate values, i.e., the uncertainties of NORM_{x,y,z} does not affect the E²-field uncertainty inside TSL (see below ConvF).
- NORM(f)_{x,y,z} = NORM_{x,y,z} * frequency_response** (see Frequency Response Chart). This linearization is implemented in DASY4 software versions later than 4.2. The uncertainty of the frequency response is included in the stated uncertainty of ConvF.
- DCP_{x,y,z}**: DCP are numerical linearization parameters assessed based on the data of power sweep with CW signal. DCP does not depend on frequency nor media.
- PAR**: PAR is the Peak to Average Ratio that is not calibrated but determined based on the signal characteristics
- A_{x,y,z}; B_{x,y,z}; C_{x,y,z}; D_{x,y,z}; VR_{x,y,z}**: A, B, C, D are numerical linearization parameters assessed based on the data of power sweep for specific modulation signal. The parameters do not depend on frequency nor media. VR is the maximum calibration range expressed in RMS voltage across the diode.
- ConvF and Boundary Effect Parameters**: Assessed in flat phantom using E-field (or Temperature Transfer Standard for $f \leq 800$ MHz) and inside waveguide using analytical field distributions based on power measurements for $f > 800$ MHz. The same setups are used for assessment of the parameters applied for boundary compensation (alpha, depth) of which typical uncertainty values are given. These parameters are used in DASY4 software to improve probe accuracy close to the boundary. The sensitivity in TSL corresponds to NORM_{x,y,z} * ConvF whereby the uncertainty corresponds to that given for ConvF. A frequency dependent ConvF is used in DASY version 4.4 and higher which allows extending the validity from ± 50 MHz to ± 100 MHz.
- Spherical isotropy (3D deviation from isotropy)**: in a field of low gradients realized using a flat phantom exposed by a patch antenna.
- Sensor Offset**: The sensor offset corresponds to the offset of virtual measurement center from the probe tip (on probe axis). No tolerance required.
- Connector Angle**: The angle is assessed using the information gained by determining the NORM_x (no uncertainty required).

EX3DV4 - SN:7506

November 12, 2024

Parameters of Probe: EX3DV4 - SN:7506

Basic Calibration Parameters

	Sensor X	Sensor Y	Sensor Z	Unc (k = 2)
Norm ($\mu\text{V}/(\text{V}/\text{m})^2$) ^A	0.59	0.62	0.56	±10.1%
DCP (mV) ^B	103.8	104.2	108.4	±4.7%

Calibration Results for Modulation Response

UID	Communication System Name		A dB	B dB $\sqrt{\mu\text{V}}$	C	D dB	VR mV	Max dev.	Max Unc ^E k = 2
0	CW	X	0.00	0.00	1.00	0.00	132.9	±2.4%	±4.7%
		Y	0.00	0.00	1.00		149.2		
		Z	0.00	0.00	1.00		135.9		

The reported uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor k=2, which for a normal distribution corresponds to a coverage probability of approximately 95%.

^A The uncertainties of Norm X,Y,Z do not affect the E²-field uncertainty inside TSL (see Page 5).

^B Linearization parameter uncertainty for maximum specified field strength.

^E Uncertainty is determined using the max. deviation from linear response applying rectangular distribution and is expressed for the square of the field value.

EX3DV4 - SN:7506

November 12, 2024

Parameters of Probe: EX3DV4 - SN:7506

Other Probe Parameters

Sensor Arrangement	Triangular
Connector Angle	37.9°
Mechanical Surface Detection Mode	enabled
Optical Surface Detection Mode	disabled
Probe Overall Length	337 mm
Probe Body Diameter	10 mm
Tip Length	9 mm
Tip Diameter	2.5 mm
Probe Tip to Sensor X Calibration Point	1 mm
Probe Tip to Sensor Y Calibration Point	1 mm
Probe Tip to Sensor Z Calibration Point	1 mm
Recommended Measurement Distance from Surface	1.4 mm

Note: Measurement distance from surface can be increased to 3–4 mm for an Area Scan job.

EX3DV4 - SN:7506

November 12, 2024

Parameters of Probe: EX3DV4 - SN:7506

Calibration Parameter Determined in Head Tissue Simulating Media

f (MHz) ^C	Relative Permittivity ^F	Conductivity ^F (S/m)	ConvF X	ConvF Y	ConvF Z	Alpha ^G	Depth ^G (mm)	Unc ^H (k = 2)
450	43.5	0.87	10.72	10.72	10.72	0.16	1.30	±13.3%
750	41.9	0.89	9.35	9.96	9.27	0.38	1.27	±11.0%
835	41.5	0.90	9.12	9.72	9.05	0.38	1.27	±11.0%
900	41.5	0.97	8.98	9.56	8.91	0.38	1.27	±11.0%
1450	40.5	1.20	8.04	8.56	7.97	0.37	1.27	±11.0%
1750	40.1	1.37	7.70	8.21	7.64	0.37	1.27	±11.0%
1900	40.0	1.40	7.37	7.85	7.31	0.37	1.27	±11.0%
2000	40.0	1.40	7.27	7.75	7.21	0.37	1.27	±11.0%
2300	39.5	1.67	7.01	7.47	6.95	0.36	1.27	±11.0%
2450	39.2	1.80	6.78	7.22	6.73	0.36	1.27	±11.0%
2600	39.0	1.96	6.70	7.14	6.64	0.36	1.27	±11.0%
3500	37.9	2.91	6.40	6.82	6.35	0.35	1.27	±13.1%
3700	37.7	3.12	6.18	6.58	6.13	0.34	1.27	±13.1%
5250	35.9	4.71	5.63	6.00	5.58	0.31	1.27	±13.1%
5600	35.5	5.07	5.26	5.60	5.22	0.28	1.27	±13.1%
5800	35.3	5.27	5.12	5.45	5.08	0.26	1.27	±13.1%

^C Frequency validity above 300 MHz of ±100 MHz only applies for DASY v4.4 and higher (see Page 2), else it is restricted to ±50 MHz. The uncertainty is the RSS of the ConvF uncertainty at calibration frequency and the uncertainty for the indicated frequency band. Frequency validity below 300 MHz is ±10, 25, 40, 50 and 70 MHz for ConvF assessments at 30, 64, 128, 150 and 220 MHz respectively. Validity of ConvF assessed at 6 MHz is 4–9 MHz, and ConvF assessed at 13 MHz is 9–19 MHz. Above 5 GHz frequency validity can be extended to ±110 MHz.

^F The probes are calibrated using tissue simulating liquids (TSL) that deviate for ϵ and σ by less than ±5% from the target values (typically better than ±3%) and are valid for TSL with deviations of up to ±10% if SAR correction is applied.

^G Alpha/Depth are determined during calibration. SPEAG warrants that the remaining deviation due to the boundary effect after compensation is always less than ±1% for frequencies below 3 GHz and below ±2% for frequencies between 3–6 GHz at any distance larger than half the probe tip diameter from the boundary.


^H The stated uncertainty is the total calibration uncertainty (k = 2) of Norm-ConvF. This is equivalent to the uncertainty component with the symbol CF in Table 9 of IEC/IEEE 62209-1528:2020.

EX3DV4 - SN:7506

November 12, 2024

Frequency Response of E-Field

(TEM-Cell:If1110 EXX, Waveguide:R22)


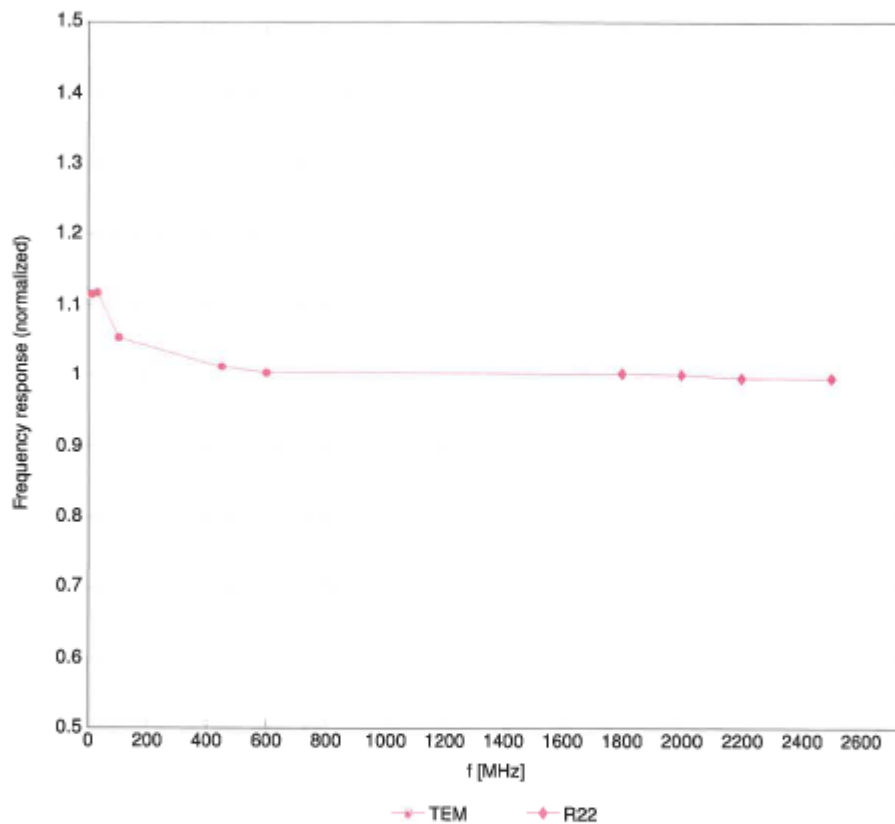


Uncertainty of Frequency Response of E-field: $\pm 6.3\%$ ($k=2$)

EX3DV4 - SN:7506

November 12, 2024

Receiving Pattern (ϕ), $\theta = 0^\circ$

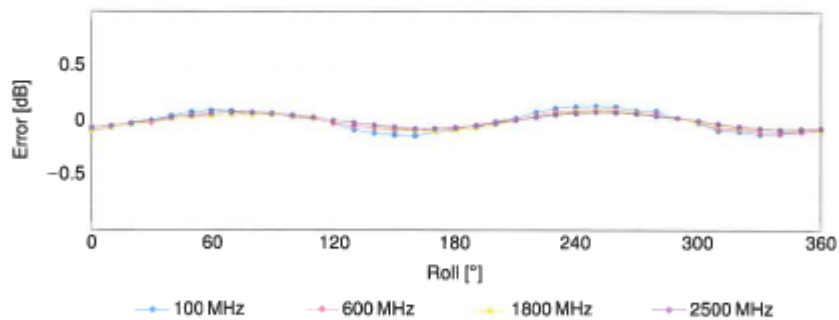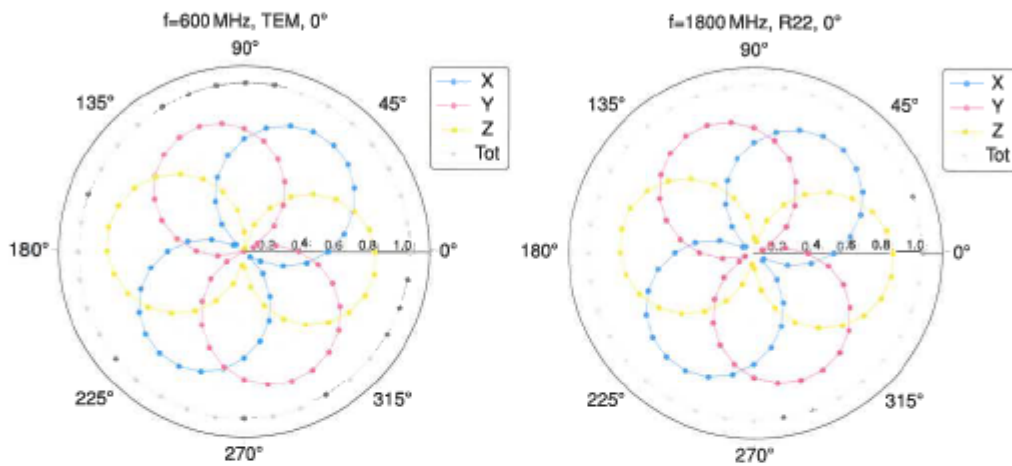



Uncertainty of Axial Isotropy Assessment: $\pm 0.5\%$ ($k=2$)

EX3DV4 - SN:7506

November 12, 2024

Dynamic Range $f(\text{SAR}_{\text{head}})$

(TEM cell, $f_{\text{eval}} = 1900 \text{ MHz}$)

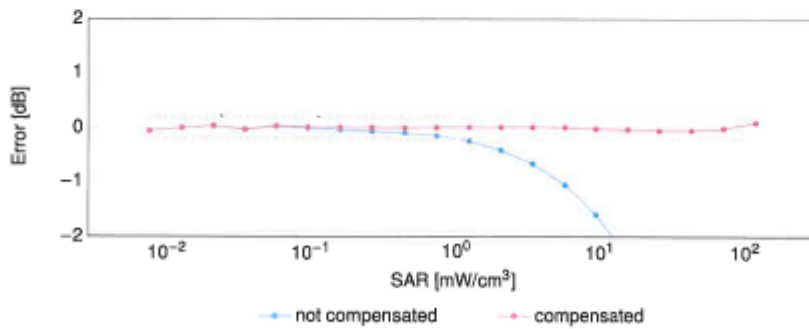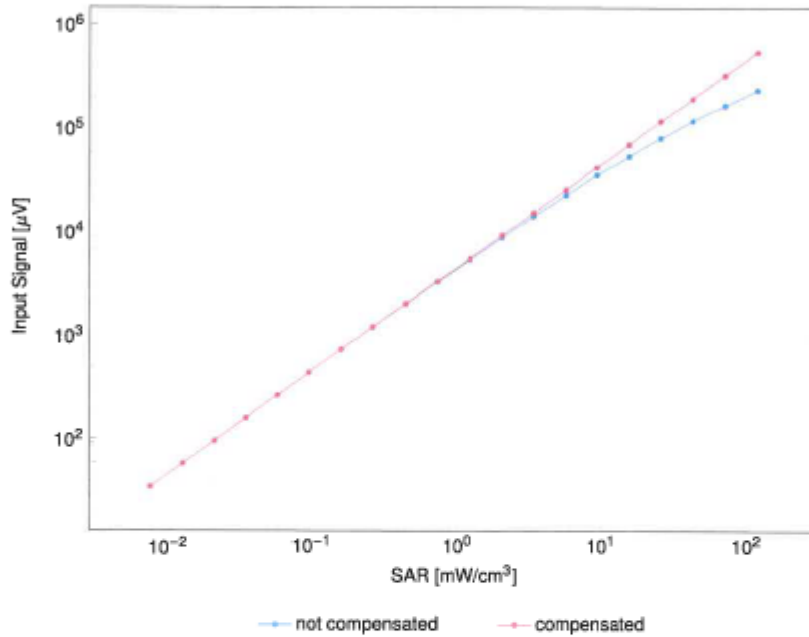


Uncertainty of Linearity Assessment: $\pm 0.6\%$ ($k=2$)

EX3DV4 - SN:7506


November 12, 2024

Conversion Factor Assessment

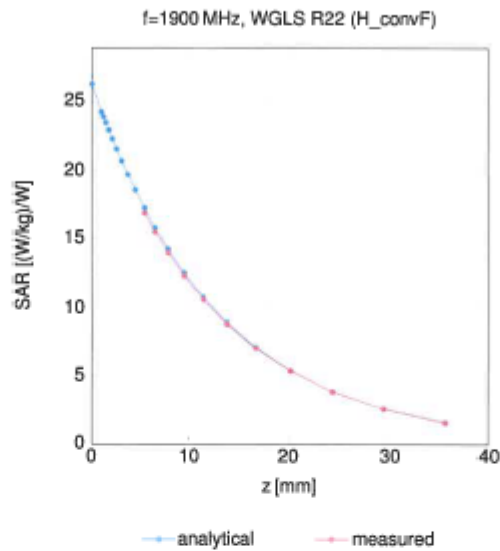

Deviation from Isotropy in Liquid

Error (ϕ, θ), $f = 900\text{ MHz}$

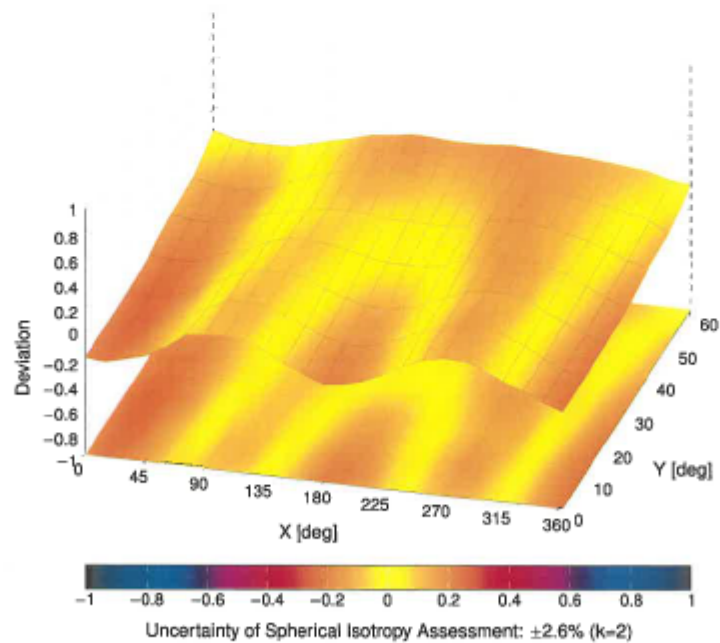

Schmid & Partner Engineering AG

Zeughausstrasse 43, 8004 Zurich, Switzerland
Phone +41 44 245 9700, Fax +41 44 245 9779
www.speag.swiss, info@speag.swiss

s p e a g

IMPORTANT NOTICE

USAGE OF THE DAE4

The DAE unit is a delicate, high precision instrument and requires careful treatment by the user. There are no serviceable parts inside the DAE. Special attention shall be given to the following points:

Battery Exchange: The battery cover of the DAE4 unit is closed using a screw, over tightening the screw may cause the threads inside the DAE to wear out.

Shipping of the DAE: Before shipping the DAE to SPEAG for calibration, remove the batteries and pack the DAE in an antistatic bag. This antistatic bag shall then be packed into a larger box or container which protects the DAE from impacts during transportation. The package shall be marked to indicate that a fragile instrument is inside.

E-Stop Failures: Touch detection may be malfunctioning due to broken magnets in the E-stop. Rough handling of the E-stop may lead to damage of these magnets. Touch and collision errors are often caused by dust and dirt accumulated in the E-stop. To prevent E-stop failure, the customer shall always mount the probe to the DAE carefully and keep the DAE unit in a non-dusty environment if not used for measurements.

Repair: Minor repairs are performed at no extra cost during the calibration. However, SPEAG reserves the right to charge for any repair especially if rough unprofessional handling caused the defect.

DASY Configuration Files: Since the exact values of the DAE input resistances, as measured during the calibration procedure of a DAE unit, are not used by the DASY software, a nominal value of 200 MOhm is given in the corresponding configuration file.

Important Note:

Warranty and calibration is void if the DAE unit is disassembled partly or fully by the Customer.

Important Note:

Never attempt to grease or oil the E-stop assembly. Cleaning and readjusting of the E-stop assembly is allowed by certified SPEAG personnel only and is part of the calibration procedure.

Important Note:

To prevent damage of the DAE probe connector pins, use great care when installing the probe to the DAE. Carefully connect the probe with the connector notch oriented in the mating position. Avoid any rotational movement of the probe body versus the DAE while turning the locking nut of the connector. The same care shall be used when disconnecting the probe from the DAE.

**Calibration Laboratory of
Schmid & Partner
Engineering AG**
Zeughausstrasse 43, 8004 Zurich, Switzerland



S Schweizerischer Kalibrierdienst
C Service suisse d'étalonnage
S Servizio svizzero di taratura
S Swiss Calibration Service

Accredited by the Swiss Accreditation Service (SAS)
The Swiss Accreditation Service is one of the signatories to the EA
Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: **SCS 0108**

Client **TUV**
Shenzhen

Certificate No: **DAE4-1557_Oct24**

CALIBRATION CERTIFICATE

Object **DAE4 - SD-000 D04 BN - SN: 1557**

Calibration procedure(s) **QA CAL-06.v30**
Calibration procedure for the data acquisition electronics (DAE)

Calibration date: **October 08, 2024**

This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI).
The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility: environment temperature (22 ± 3)°C and humidity < 70%.

Calibration Equipment used (M&TE critical for calibration)

Primary Standards	ID #	Cal Date (Certificate No.)	Scheduled Calibration
Keithley Multimeter Type 2001	SN: 0810278	27-Aug-24 (No:40547)	Aug-25
Secondary Standards	ID #	Check Date (in house)	Scheduled Check
Auto DAE Calibration Unit	SE UWS 053 AA 1001	23-Jan-24 (in house check)	In house check: Jan-25
Calibrator Box V2.1	SE UMS 006 AA 1002	23-Jan-24 (in house check)	In house check: Jan-25

Calibrated by:	Name Adrian Gehring	Function Laboratory Technician	Signature 
Approved by:	Sven Kühn	Technical Manager	

Issued: October 8, 2024

This calibration certificate shall not be reproduced except in full without written approval of the laboratory.

**Calibration Laboratory of
Schmid & Partner
Engineering AG**
Zeughausstrasse 43, 8004 Zurich, Switzerland



S Schweizerischer Kalibrierdienst
C Service suisse d'étalonnage
S Servizio svizzero di taratura
S Swiss Calibration Service

Accredited by the Swiss Accreditation Service (SAS)

The Swiss Accreditation Service is one of the signatories to the EA
Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: **SCS 0108**

Glossary

DAE data acquisition electronics
Connector angle information used in DASY system to align probe sensor X to the robot
coordinate system.

Methods Applied and Interpretation of Parameters

- **DC Voltage Measurement:** Calibration Factor assessed for use in DASY system by comparison with a calibrated instrument traceable to national standards. The figure given corresponds to the full scale range of the voltmeter in the respective range.
- **Connector angle:** The angle of the connector is assessed measuring the angle mechanically by a tool inserted. Uncertainty is not required.
- The following parameters as documented in the Appendix contain technical information as a result from the performance test and require no uncertainty.
 - **DC Voltage Measurement Linearity:** Verification of the Linearity at +10% and -10% of the nominal calibration voltage. Influence of offset voltage is included in this measurement.
 - **Common mode sensitivity:** Influence of a positive or negative common mode voltage on the differential measurement.
 - **Channel separation:** Influence of a voltage on the neighbor channels not subject to an input voltage.
 - **AD Converter Values with inputs shorted:** Values on the internal AD converter corresponding to zero input voltage
 - **Input Offset Measurement:** Output voltage and statistical results over a large number of zero voltage measurements.
 - **Input Offset Current:** Typical value for information; Maximum channel input offset current, not considering the input resistance.
 - **Input resistance:** Typical value for information: DAE input resistance at the connector, during internal auto-zeroing and during measurement.
 - **Low Battery Alarm Voltage:** Typical value for information. Below this voltage, a battery alarm signal is generated.
 - **Power consumption:** Typical value for information. Supply currents in various operating modes.

DC Voltage Measurement

A/D - Converter Resolution nominal

High Range: 1LSB = 6.1µV , full range = -100...+300 mV

Low Range: 1LSB = 61nV , full range = -1.....+3mV

DASY measurement parameters: Auto Zero Time: 3 sec; Measuring time: 3 sec

Calibration Factors	X	Y	Z
High Range	405.027 ± 0.02% (k=2)	404.694 ± 0.02% (k=2)	404.784 ± 0.02% (k=2)
Low Range	3.97303 ± 1.50% (k=2)	4.00504 ± 1.50% (k=2)	3.99067 ± 1.50% (k=2)

Connector Angle

Connector Angle to be used in DASY system	52.5 ° ± 1 °
---	--------------

Appendix (Additional assessments outside the scope of SCS0108)

1. DC Voltage Linearity

High Range	Reading (μV)	Difference (μV)	Error (%)
Channel X + Input	199998.64	2.42	0.00
Channel X + Input	20004.22	1.33	0.01
Channel X - Input	-19998.68	3.45	-0.02
Channel Y + Input	199997.78	1.71	0.00
Channel Y + Input	20002.60	-0.05	-0.00
Channel Y - Input	-20002.53	-0.09	0.00
Channel Z + Input	199997.83	1.48	0.00
Channel Z + Input	20000.83	-1.79	-0.01
Channel Z - Input	-20002.41	0.05	-0.00

Low Range	Reading (μV)	Difference (μV)	Error (%)
Channel X + Input	2001.16	-0.00	-0.00
Channel X + Input	202.26	0.97	0.48
Channel X - Input	-197.33	1.15	-0.58
Channel Y + Input	2001.07	-0.02	-0.00
Channel Y + Input	200.67	-0.49	-0.24
Channel Y - Input	-199.11	-0.64	0.32
Channel Z + Input	2001.03	-0.01	-0.00
Channel Z + Input	200.51	-0.64	-0.32
Channel Z - Input	-199.71	-1.07	0.54

2. Common mode sensitivity

DASY measurement parameters: Auto Zero Time: 3 sec; Measuring time: 3 sec

	Common mode Input Voltage (mV)	High Range Average Reading (μV)	Low Range Average Reading (μV)
Channel X	200	0.08	-2.12
	- 200	4.52	2.85
Channel Y	200	4.23	4.10
	- 200	-5.11	-5.78
Channel Z	200	2.94	2.93
	- 200	-5.29	-5.31

3. Channel separation

DASY measurement parameters: Auto Zero Time: 3 sec; Measuring time: 3 sec

	Input Voltage (mV)	Channel X (μV)	Channel Y (μV)	Channel Z (μV)
Channel X	200	-	-1.30	-1.62
Channel Y	200	5.72	-	0.28
Channel Z	200	10.64	2.33	-

4. AD-Converter Values with inputs shorted

DASY measurement parameters: Auto Zero Time: 3 sec; Measuring time: 3 sec

	High Range (LSB)	Low Range (LSB)
Channel X	15803	16236
Channel Y	15752	14466
Channel Z	16034	16152

5. Input Offset Measurement

DASY measurement parameters: Auto Zero Time: 3 sec; Measuring time: 3 sec

Input 10MΩ

	Average (μV)	min. Offset (μV)	max. Offset (μV)	Std. Deviation (μV)
Channel X	0.84	0.22	1.36	0.23
Channel Y	-1.95	-3.47	-1.17	0.33
Channel Z	-2.19	-3.07	-1.00	0.41

6. Input Offset Current

Nominal Input circuitry offset current on all channels: <25fA

7. Input Resistance (Typical values for information)

	Zeroing (kOhm)	Measuring (MOhm)
Channel X	200	200
Channel Y	200	200
Channel Z	200	200

8. Low Battery Alarm Voltage (Typical values for information)

Typical values	Alarm Level (VDC)
Supply (+ Vcc)	+7.9
Supply (- Vcc)	-7.6

9. Power Consumption (Typical values for information)

Typical values	Switched off (mA)	Stand by (mA)	Transmitting (mA)
Supply (+ Vcc)	+0.01	+6	+14
Supply (- Vcc)	-0.01	-8	-9