

Date: 2025-03-21

System Check_Head_2450MHz**DUT: D2450V2 - SN929**

Communication System: CW; Frequency: 2450.000 MHz

Medium: HSL_2450_250321 Medium parameters used: $f = 2450.000$ MHz; $\sigma = 1.83$ S/m; $\epsilon_r = 39.0$

Ambient Temperature: 23.1°C; Liquid Temperature: 22.1°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7785; ConvF(6.25, 6.58, 6.44); Calibrated: 2024-11-28
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1694; Calibrated: 2024-11-19
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2126; Section: Flat
- Measurement Software: 16.2.4.2524
- UID: CW, 0--

Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 2.49 W/kg; SAR (10g) = 1.14 W/kg;


Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.5 mm

Power Drift = 0.01 dB

SAR (1g) = 2.50 W/kg; SAR (8g) = 1.33 W/kg; SAR (10g) = 1.21 W/kg

Smallest distance from peaks to all points 3 dB below = 9.0 mm

Ratio of SAR at M2 to SAR at M1 = 83.3 %

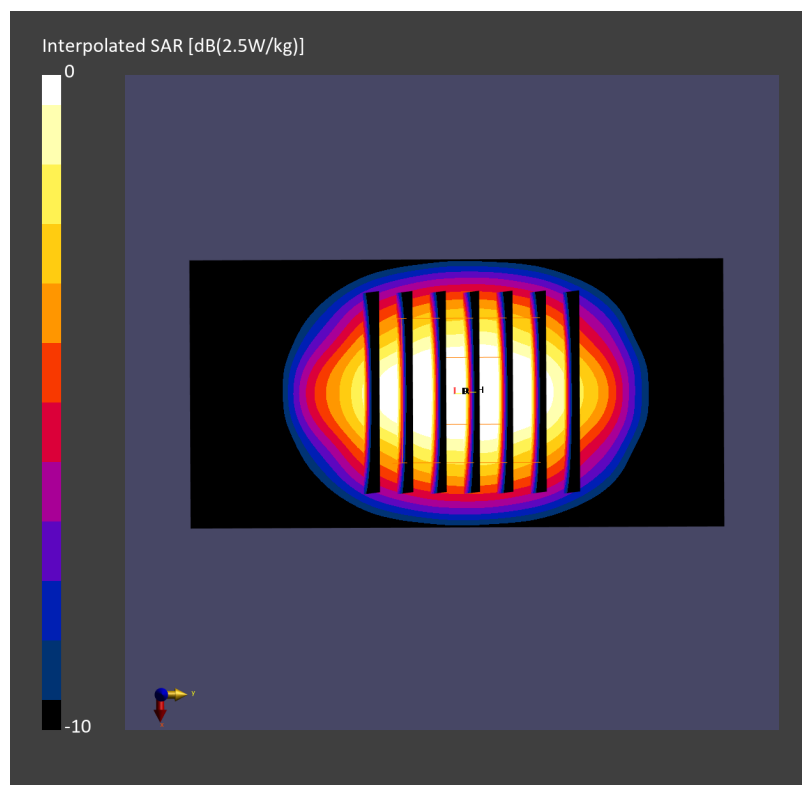

Date: 2025-04-01

System Check_Head_5250MHz**DUT: D5GHzV2 - SN1006**

Communication System: CW; Frequency: 5250.000 MHz

Medium: HSL_5G_250401 Medium parameters used: $f = 5250.000$ MHz; $\sigma = 4.68$ S/m; $\epsilon_r = 36.9$

Ambient Temperature: 23.5°C; Liquid Temperature: 22.5°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7694; ConvF(5.25, 5.13, 5.73); Calibrated: 2024-11-18
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1697; Calibrated: 2024-11-14
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2127; Section: Flat
- Measurement Software: 16.2.4.2524
- UID: CW, 0--

Pin=20.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 7.02 W/kg; SAR (10g) = 2.00 W/kg;


Pin=20.0dBm/Zoom Scan (22.0 mm x 22.0 mm x 22.0 mm): Measurement Grid: 4.0 mm x 4.0 mm x 1.4 mm

Power Drift = 0.02 dB

SAR (1g) = 7.61 W/kg; SAR (8g) = 2.53 W/kg; SAR (10g) = 2.16 W/kg

Smallest distance from peaks to all points 3 dB below = 7.4 mm

Ratio of SAR at M2 to SAR at M1 = 62.3 %

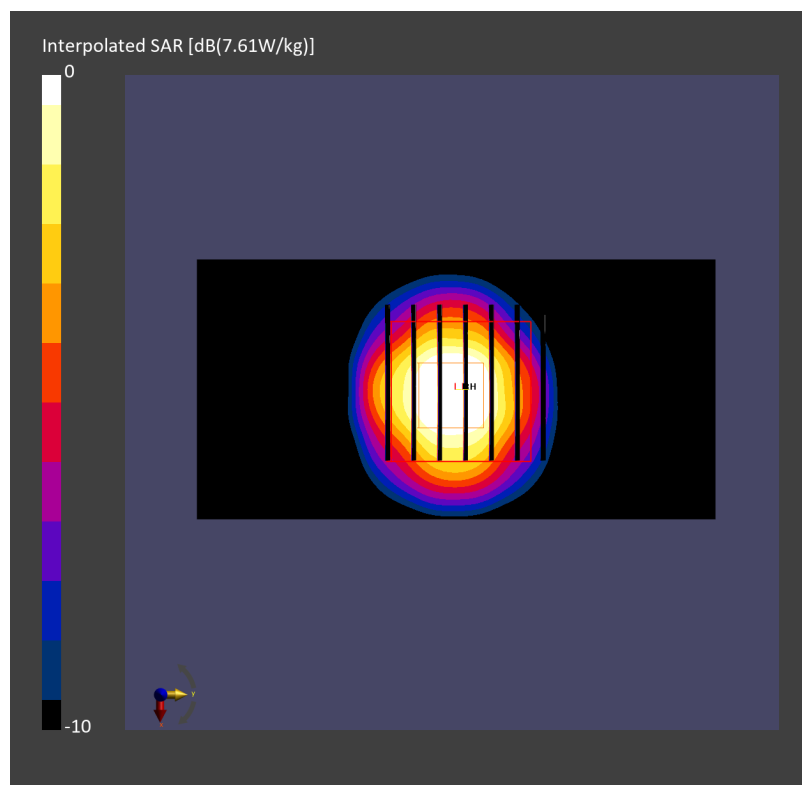

Date: 2025-04-01

System Check_Head_5600MHz**DUT: D5GHzV2 - SN1006**

Communication System: CW; Frequency: 5600.000 MHz

Medium: HSL_5G_250401 Medium parameters used: $f = 5600.000$ MHz; $\sigma = 5.06$ S/m; $\epsilon_r = 36.4$

Ambient Temperature: 23.5°C; Liquid Temperature: 22.5°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7694; ConvF(4.9, 4.79, 5.35); Calibrated: 2024-11-18
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1697; Calibrated: 2024-11-14
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2127; Section: Flat
- Measurement Software: 16.2.4.2524
- UID: CW, 0--

Pin=20.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 6.93 W/kg; SAR (10g) = 1.96 W/kg;


Pin=20.0dBm/Zoom Scan (22.0 mm x 22.0 mm x 22.0 mm): Measurement Grid: 4.0 mm x 4.0 mm x 1.4 mm

Power Drift = 0.07 dB

SAR (1g) = 7.62 W/kg; SAR (8g) = 2.51 W/kg; SAR (10g) = 2.14 W/kg

Smallest distance from peaks to all points 3 dB below = 7.4 mm

Ratio of SAR at M2 to SAR at M1 = 59.5 %

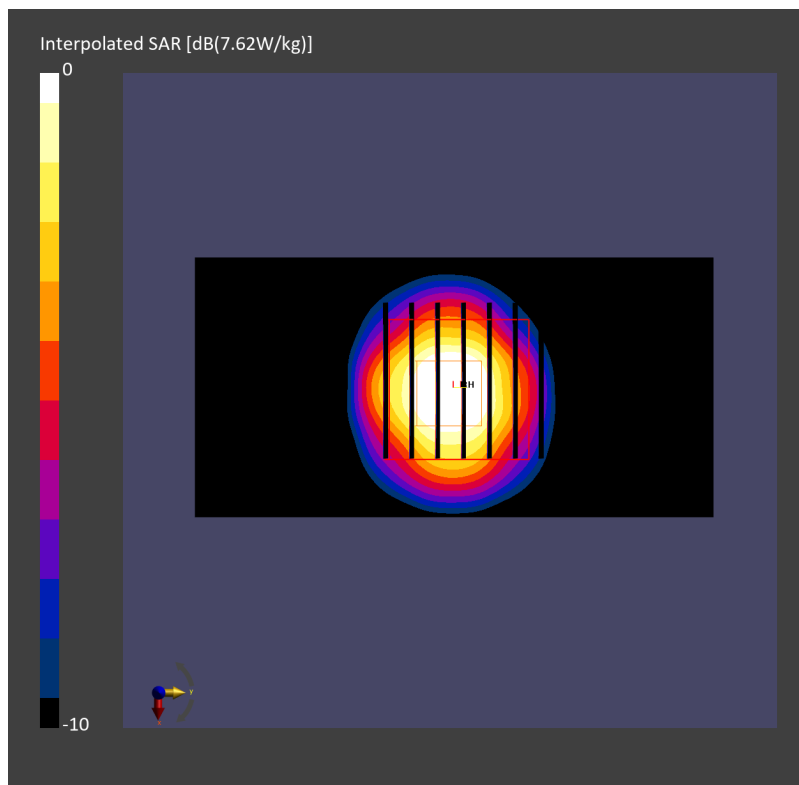

Date: 2025-04-01

System Check_Head_5800MHz**DUT: D5GHzV2 - SN1006**

Communication System: CW; Frequency: 5800.000 MHz

Medium: HSL_5G_250401 Medium parameters used: $f = 5800.000$ MHz; $\sigma = 5.27$ S/m; $\epsilon_r = 36.1$

Ambient Temperature: 23.5°C; Liquid Temperature: 22.5°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7694; ConvF(4.82, 4.7, 5.25); Calibrated: 2024-11-18
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1697; Calibrated: 2024-11-14
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2127; Section: Flat
- Measurement Software: 16.2.4.2524
- UID: CW, 0--

Pin=20.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 6.57 W/kg; SAR (10g) = 1.86 W/kg;

Pin=20.0dBm/Zoom Scan (22.0 mm x 22.0 mm x 22.0 mm): Measurement Grid: 4.0 mm x 4.0 mm x 1.4 mm

Power Drift = 0.06 dB

SAR (1g) = 7.58 W/kg; SAR (8g) = 2.49 W/kg; SAR (10g) = 2.13 W/kg

Smallest distance from peaks to all points 3 dB below = 7.4 mm

Ratio of SAR at M2 to SAR at M1 = 57.8 %

