

Date: 2025-01-22

System Check_Head_750MHz**DUT: D750V3 - SN1107**

Communication System: CW; Frequency: 750.000 MHz

Medium: HSL_750_250122 Medium parameters used: $f = 750.000$ MHz; $\sigma = 0.877$ S/m; $\epsilon_r = 41.8$

Ambient Temperature: 23.4°C; Liquid Temperature: 22.4°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7694; ConvF(9.17, 8.96, 10.01); Calibrated: 2024-11-18
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1697; Calibrated: 2024-11-14
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2127; Section: Flat
- Measurement Software: 16.2.4.2524
- UID: CW, 0

Pin=24.0dBm/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 2.06 W/kg; SAR (10g) = 1.37 W/kg;


Pin=24.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm

Power Drift = -0.01 dB

SAR (1g) = 2.07 W/kg; SAR (8g) = 1.46 W/kg; SAR (10g) = 1.39 W/kg

Smallest distance from peaks to all points 3 dB below = 20.5 mm

Ratio of SAR at M2 to SAR at M1 = 87.7 %

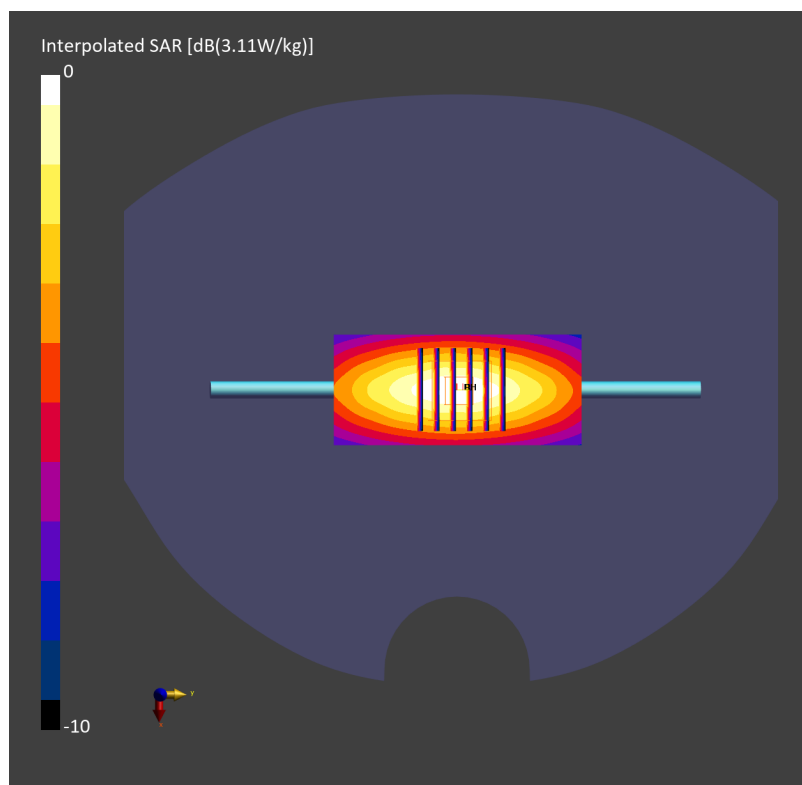

Date: 2025-01-23

System Check_Head_750MHz**DUT: D750V3 - SN1107**

Communication System: CW; Frequency: 750.000 MHz

Medium: HSL_750_250123 Medium parameters used: $f = 750.000$ MHz; $\sigma = 0.875$ S/m; $\epsilon_r = 41.7$

Ambient Temperature: 23.3°C; Liquid Temperature: 22.3°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7694; ConvF(9.17, 8.96, 10.01); Calibrated: 2024-11-18
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1697; Calibrated: 2024-11-14
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2127; Section: Flat
- Measurement Software: 16.2.4.2524
- UID: CW, 0

Pin=24.0dBm/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 2.09 W/kg; SAR (10g) = 1.39 W/kg;


Pin=24.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm

Power Drift = -0.01 dB

SAR (1g) = 2.10 W/kg; SAR (8g) = 1.49 W/kg; SAR (10g) = 1.42 W/kg

Smallest distance from peaks to all points 3 dB below = 20.5 mm

Ratio of SAR at M2 to SAR at M1 = 87.8 %

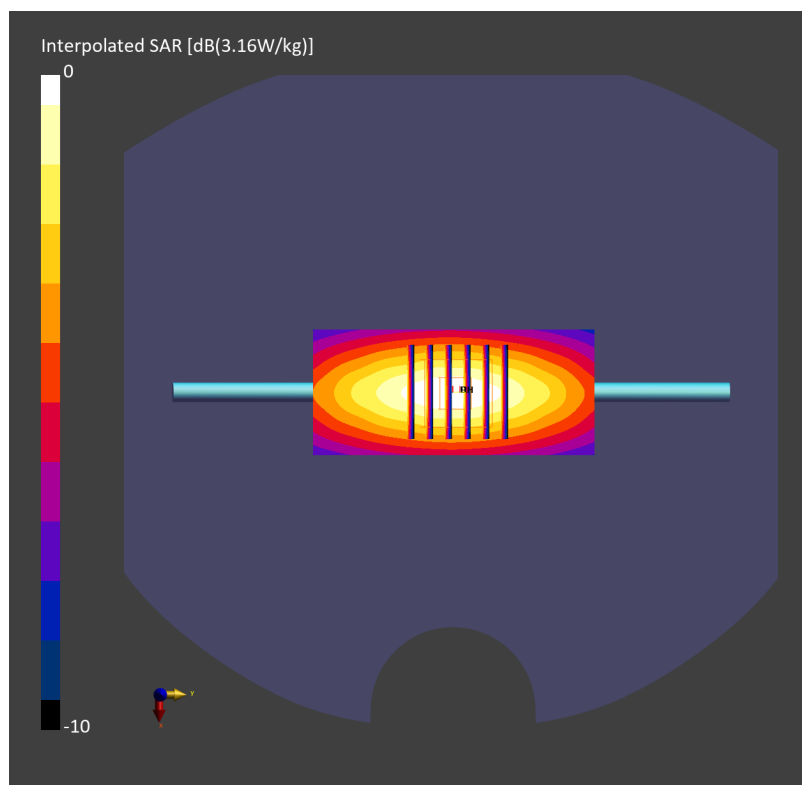

Date: 2025-01-24

System Check_Head_750MHz

DUT: D750V3 - SN1107

Communication System: CW; Frequency: 750.000 MHz

Medium: HSL_750_250124 Medium parameters used: $f = 750.000$ MHz; $\sigma = 0.872$ S/m; $\epsilon_r = 41.6$

Ambient Temperature: 23.6°C; Liquid Temperature: 22.6°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7694; ConvF(9.17, 8.96, 10.01); Calibrated: 2024-11-18
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1697; Calibrated: 2024-11-14
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2127; Section: Flat
- Measurement Software: 16.2.4.2524
- UID: CW, 0

Pin=24.0dBm/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 2.09 W/kg; SAR (10g) = 1.39 W/kg;


Pin=24.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm

Power Drift = 0.00 dB

SAR (1g) = 2.10 W/kg; SAR (8g) = 1.49 W/kg; SAR (10g) = 1.42 W/kg

Smallest distance from peaks to all points 3 dB below = 21.3 mm

Ratio of SAR at M2 to SAR at M1 = 87.1 %

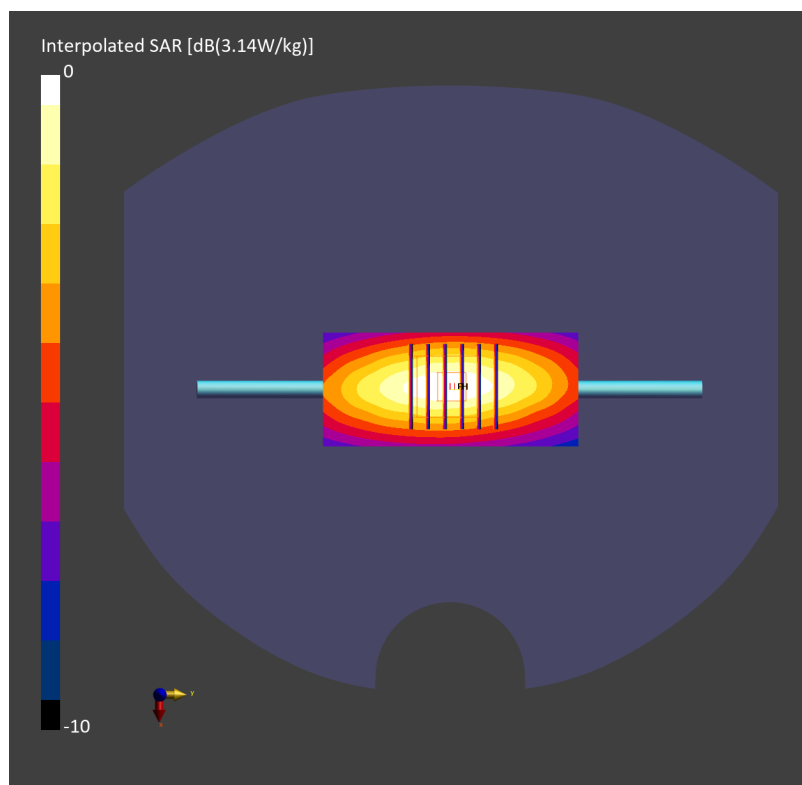

Date: 2025-02-02

System Check_Head_750MHz**DUT: D750V3 - SN1107**

Communication System: CW; Frequency: 750.000 MHz

Medium: HSL_750_250202 Medium parameters used: $f = 750.000$ MHz; $\sigma = 0.898$ S/m; $\epsilon_r = 43.1$

Ambient Temperature: 23.3°C; Liquid Temperature: 22.3°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7625; ConvF(9.22, 9.0, 9.74); Calibrated: 2024-12-13
- Sensor-Surface: 1.4 mm
- Electronics: DAE4ip Sn1800; Calibrated: 2024-06-18
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2144; Section: Flat
- Measurement Software: 16.2.4.2524
- UID: CW, 0

Pin=24.0dBm/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 2.25 W/kg; SAR (10g) = 1.50 W/kg;


Pin=24.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm

Power Drift = -0.02 dB

SAR (1g) = 2.26 W/kg; SAR (8g) = 1.60 W/kg; SAR (10g) = 1.52 W/kg

Smallest distance from peaks to all points 3 dB below = > 15.0 mm

Ratio of SAR at M2 to SAR at M1 = 87.5 %

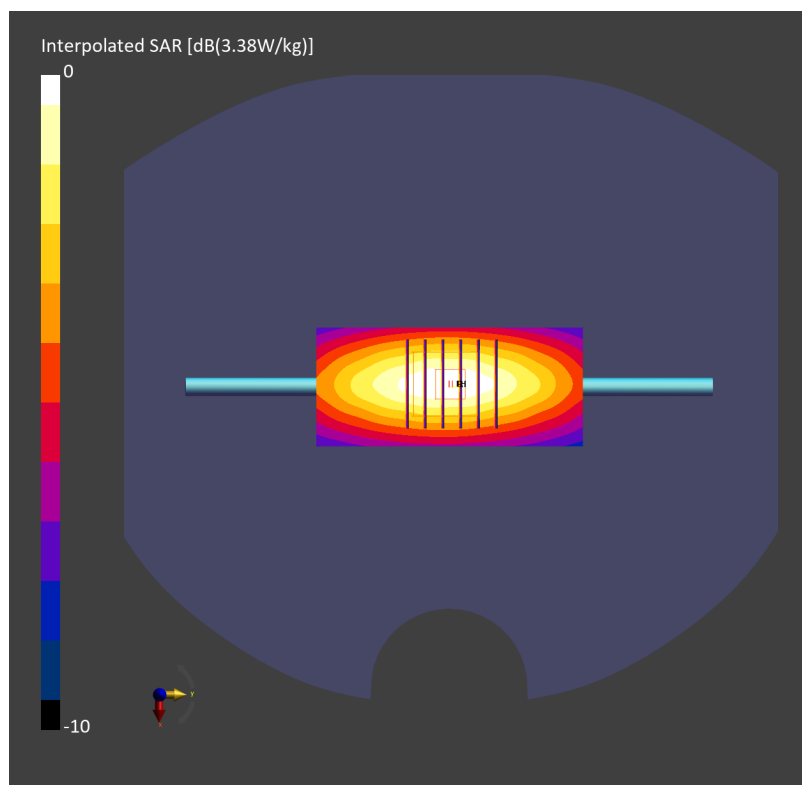

Date: 2025-02-10

System Check_Head_750MHz**DUT: D750V3 - SN1107**

Communication System: CW; Frequency: 750.000 MHz

Medium: HSL_750_250210 Medium parameters used: $f = 750.000$ MHz; $\sigma = 0.894$ S/m; $\epsilon_r = 43.0$

Ambient Temperature: 23.3°C; Liquid Temperature: 22.3°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7625; ConvF(9.22, 9.0, 9.74); Calibrated: 2024-12-13
- Sensor-Surface: 1.4 mm
- Electronics: DAE4ip Sn1800; Calibrated: 2024-06-18
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2144; Section: Flat
- Measurement Software: 16.2.4.2524
- UID: CW, 0

Pin=24.0dBm/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 2.13 W/kg; SAR (10g) = 1.42 W/kg;


Pin=24.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm

Power Drift = 0.04 dB

SAR (1g) = 2.17 W/kg; SAR (8g) = 1.54 W/kg; SAR (10g) = 1.46 W/kg

Smallest distance from peaks to all points 3 dB below = > 15.0 mm

Ratio of SAR at M2 to SAR at M1 = 87.3 %

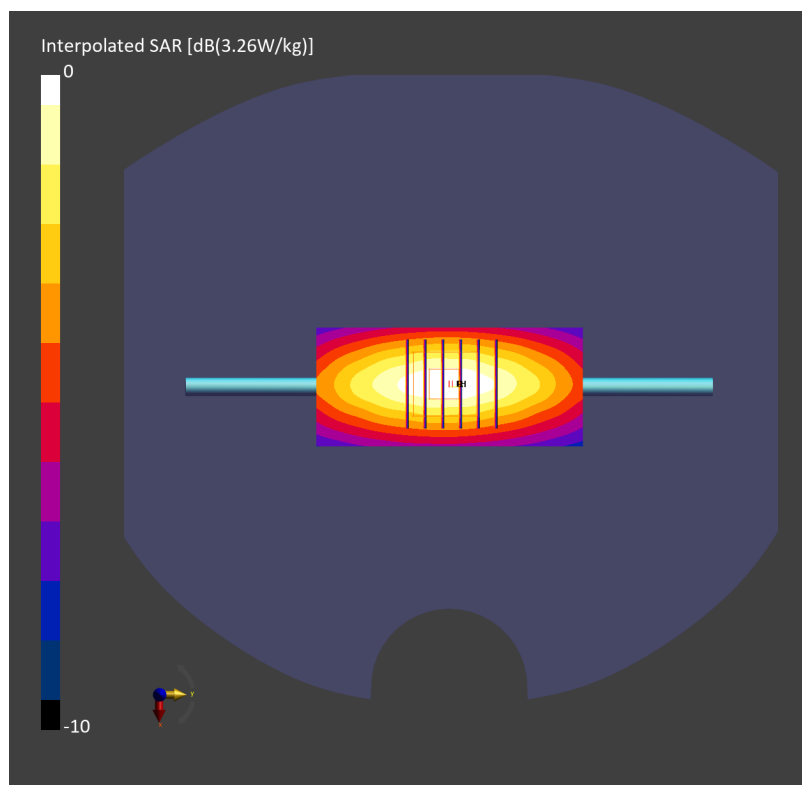

Date: 2025-02-14

System Check_Head_750MHz**DUT: D750V3 - SN1107**

Communication System: CW; Frequency: 750.000 MHz

Medium: HSL_750_250214 Medium parameters used: $f = 750.000$ MHz; $\sigma = 0.892$ S/m; $\epsilon_r = 43.1$

Ambient Temperature: 23.7°C; Liquid Temperature: 22.7°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7625; ConvF(9.22, 9.0, 9.74); Calibrated: 2024-12-13
- Sensor-Surface: 1.4 mm
- Electronics: DAE4ip Sn1800; Calibrated: 2024-06-18
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2144; Section: Flat
- Measurement Software: 16.2.4.2524
- UID: CW, 0

Pin=24.0dBm/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 2.04 W/kg; SAR (10g) = 1.36 W/kg;


Pin=24.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm

Power Drift = 0.01 dB

SAR (1g) = 2.06 W/kg; SAR (8g) = 1.46 W/kg; SAR (10g) = 1.39 W/kg

Smallest distance from peaks to all points 3 dB below = > 15.0 mm

Ratio of SAR at M2 to SAR at M1 = 87.3 %

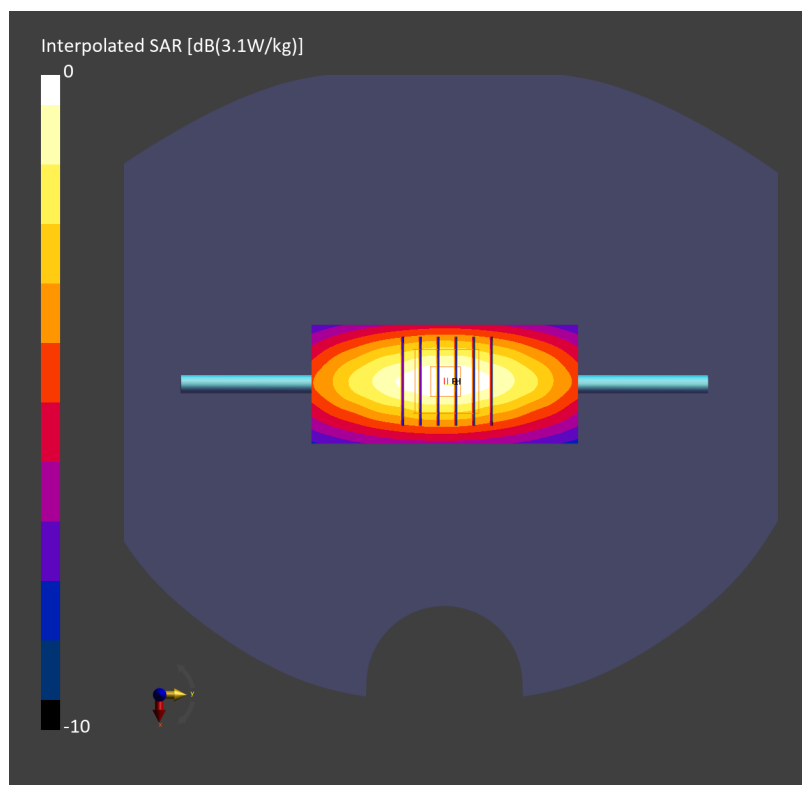

Date: 2025-02-18

System Check_Head_750MHz**DUT: D750V3 - SN1107**

Communication System: CW; Frequency: 750.000 MHz

Medium: HSL_750_250218 Medium parameters used: $f = 750.000$ MHz; $\sigma = 0.902$ S/m; $\epsilon_r = 40.2$

Ambient Temperature: 23.6°C; Liquid Temperature: 22.6°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7625; ConvF(9.22, 9.0, 9.74); Calibrated: 2024-12-13
- Sensor-Surface: 1.4 mm
- Electronics: DAE4ip Sn1800; Calibrated: 2024-06-18
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2144; Section: Flat
- Measurement Software: 16.2.4.2524
- UID: CW, 0

Pin=24.0dBm/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 2.23 W/kg; SAR (10g) = 1.48 W/kg;


Pin=24.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm

Power Drift = 0.00 dB

SAR (1g) = 2.26 W/kg; SAR (8g) = 1.60 W/kg; SAR (10g) = 1.52 W/kg

Smallest distance from peaks to all points 3 dB below = > 15.0 mm

Ratio of SAR at M2 to SAR at M1 = 87.1 %

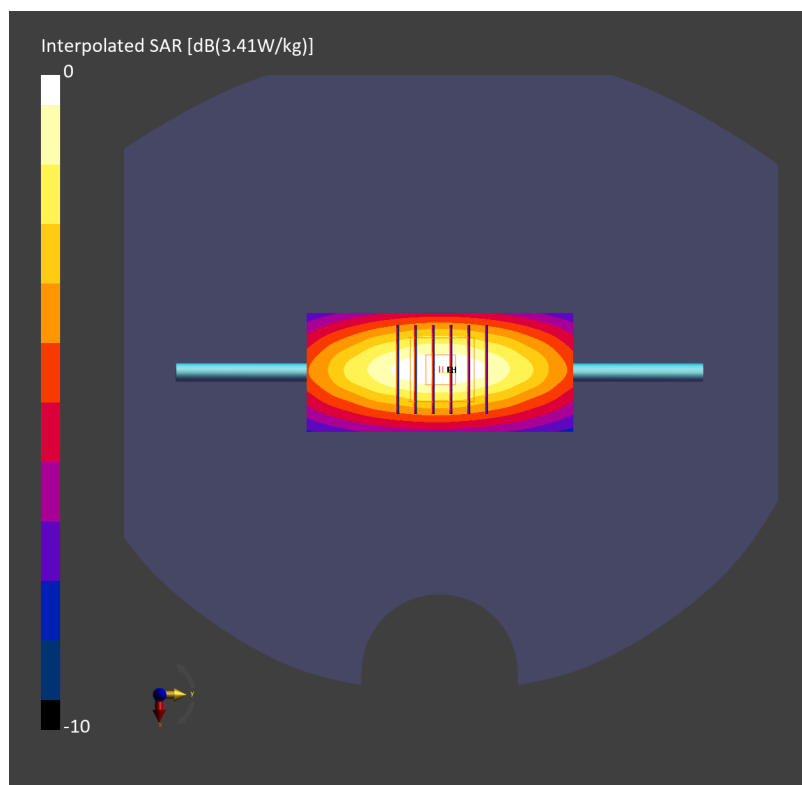

Date: 2025-03-26

System Check_Head_750MHz

DUT: D750V3 - SN1107

Communication System: CW; Frequency: 750.000 MHz

Medium: HSL_750_250326 Medium parameters used: $f = 750.000$ MHz; $\sigma = 0.885$ S/m; $\epsilon_r = 42.8$

Ambient Temperature: 23.6°C; Liquid Temperature: 22.6°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7785; ConvF(8.06, 8.49, 8.31); Calibrated: 2024-11-28
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1694; Calibrated: 2024-11-19
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2126; Section: Flat
- Measurement Software: 16.2.4.2524
- UID: CW, 0

Pin=24.0dBm/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 2.11 W/kg; SAR (10g) = 1.41 W/kg;


Pin=24.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm

Power Drift = -0.02 dB

SAR (1g) = 2.11 W/kg; SAR (8g) = 1.50 W/kg; SAR (10g) = 1.43 W/kg

Smallest distance from peaks to all points 3 dB below = > 15.0 mm

Ratio of SAR at M2 to SAR at M1 = 87.7 %

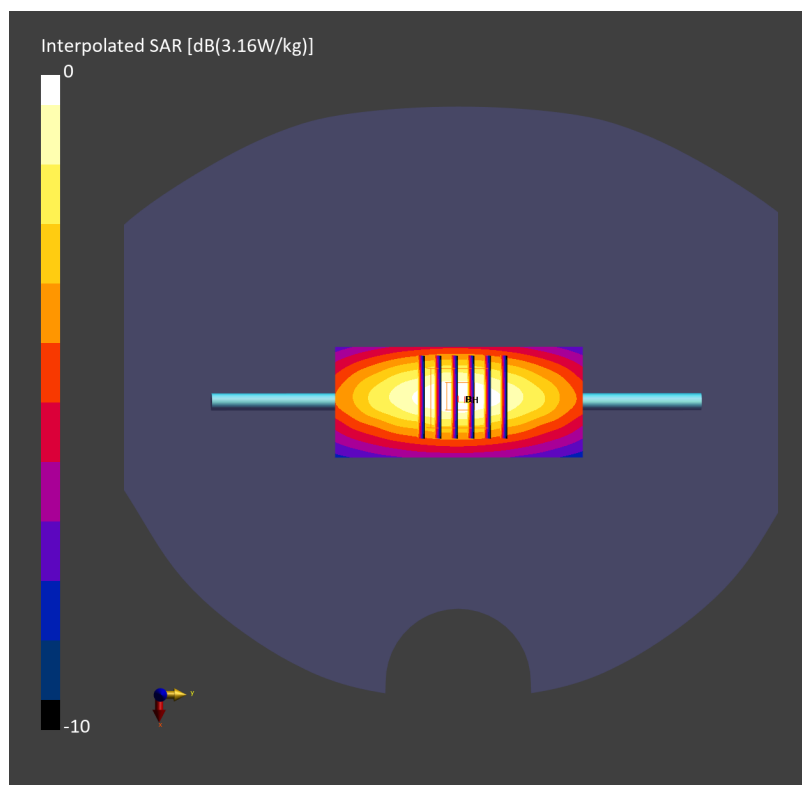

Date: 2025-01-21

System Check_Head_835MHz**DUT: D835V2 - SN4d167**

Communication System: CW; Frequency: 835.000 MHz

Medium: HSL_850_250121 Medium parameters used: $f = 835.000$ MHz; $\sigma = 0.923$ S/m; $\epsilon_r = 42.5$

Ambient Temperature: 23.1°C; Liquid Temperature: 22.1°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7694; ConvF(8.87, 8.66, 9.68); Calibrated: 2024-11-18
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1697; Calibrated: 2024-11-14
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2127; Section: Flat
- Measurement Software: 16.2.4.2524
- UID: CW, 0

Pin=24.0dBm/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 2.28 W/kg; SAR (10g) = 1.50 W/kg;


Pin=24.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm

Power Drift = -0.00 dB

SAR (1g) = 2.28 W/kg; SAR (8g) = 1.61 W/kg; SAR (10g) = 1.53 W/kg

Smallest distance from peaks to all points 3 dB below = 17.8 mm

Ratio of SAR at M2 to SAR at M1 = 87.9 %

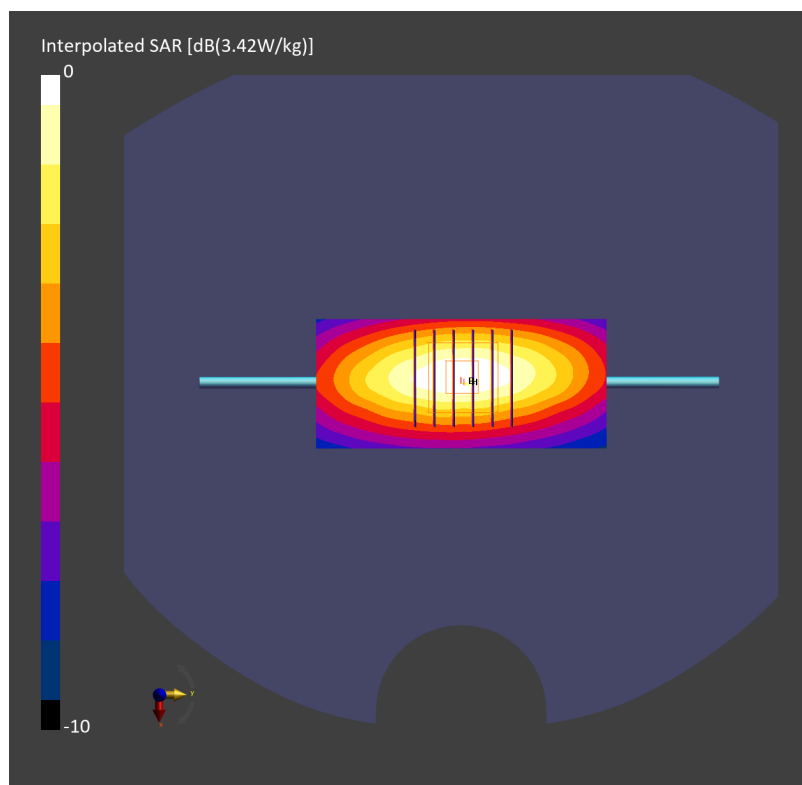

Date: 2025-01-25

System Check_Head_835MHz**DUT: D835V2 - SN4d167**

Communication System: CW; Frequency: 835.000 MHz

Medium: HSL_850_250125 Medium parameters used: $f = 835.000$ MHz; $\sigma = 0.914$ S/m; $\epsilon_r = 41.5$

Ambient Temperature: 23.5°C; Liquid Temperature: 22.5°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7694; ConvF(8.87, 8.66, 9.68); Calibrated: 2024-11-18
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1697; Calibrated: 2024-11-14
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2127; Section: Flat
- Measurement Software: 16.2.4.2524
- UID: CW, 0

Pin=24.0dBm/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 2.36 W/kg; SAR (10g) = 1.56 W/kg;


Pin=24.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm

Power Drift = -0.01 dB

SAR (1g) = 2.38 W/kg; SAR (8g) = 1.67 W/kg; SAR (10g) = 1.59 W/kg

Smallest distance from peaks to all points 3 dB below = 17.8 mm

Ratio of SAR at M2 to SAR at M1 = 88.1 %

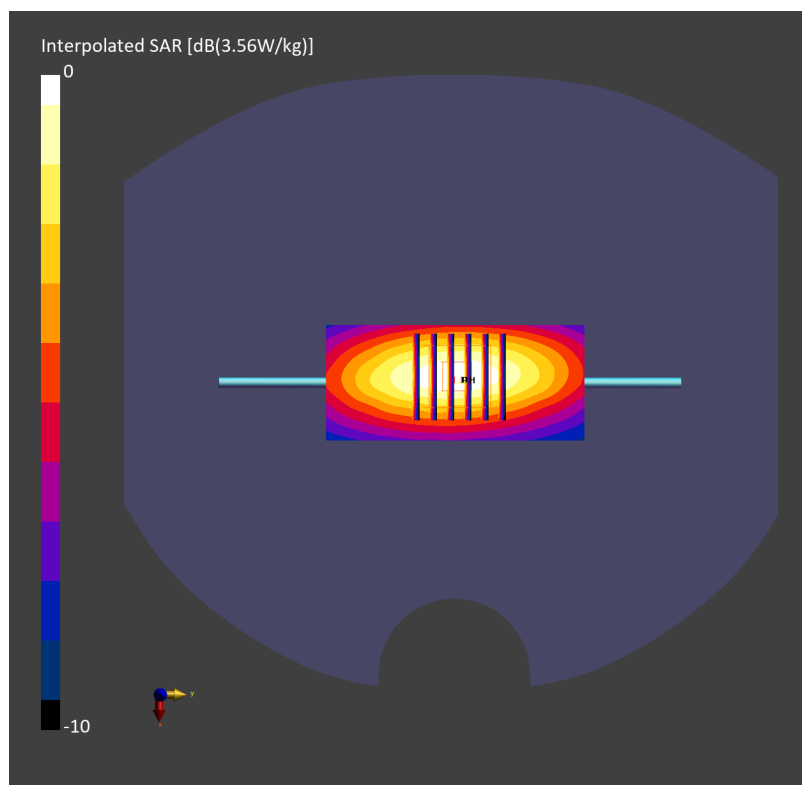

Date: 2025-01-28

System Check_Head_835MHz**DUT: D835V2 - SN4d167**

Communication System: CW; Frequency: 835.000 MHz

Medium: HSL_850_250128 Medium parameters used: $f = 835.000$ MHz; $\sigma = 0.929$ S/m; $\epsilon_r = 41.5$

Ambient Temperature: 23.4°C; Liquid Temperature: 22.4°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7625; ConvF(8.91, 8.7, 9.42); Calibrated: 2024-12-13
- Sensor-Surface: 1.4 mm
- Electronics: DAE4ip Sn1800; Calibrated: 2024-06-18
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2144; Section: Flat
- Measurement Software: 16.2.4.2524
- UID: CW, 0

Pin=24.0dBm/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 2.58 W/kg; SAR (10g) = 1.70 W/kg;


Pin=24.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm

Power Drift = -0.00 dB

SAR (1g) = 2.61 W/kg; SAR (8g) = 1.84 W/kg; SAR (10g) = 1.75 W/kg

Smallest distance from peaks to all points 3 dB below = 19.0 mm

Ratio of SAR at M2 to SAR at M1 = 87.5 %

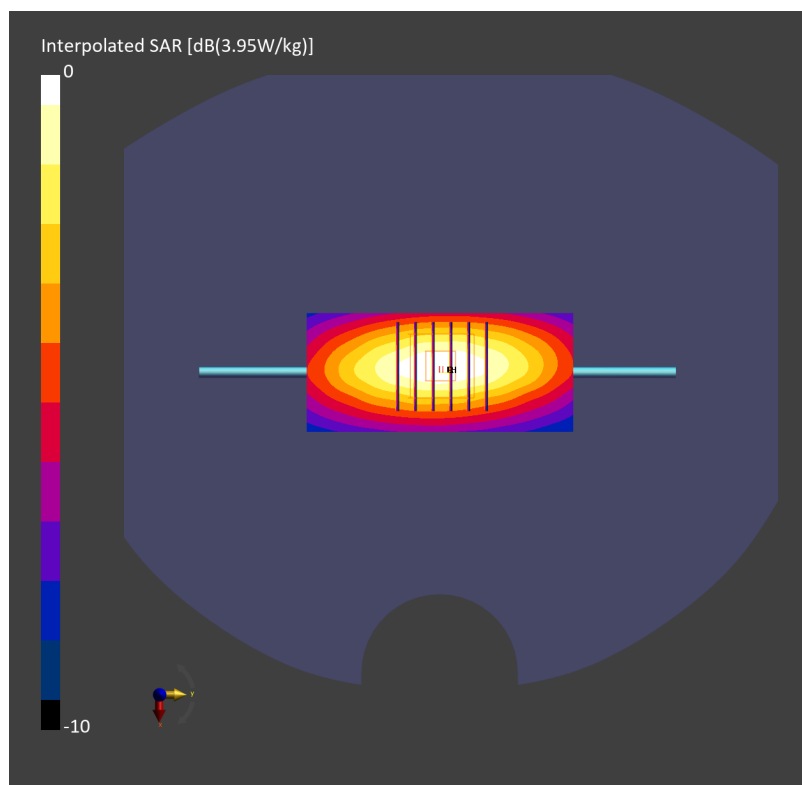

Date: 2025-02-01

System Check_Head_835MHz

DUT: D835V2 - SN4d167

Communication System: CW; Frequency: 835.000 MHz

Medium: HSL_850_250201 Medium parameters used: $f = 835.000$ MHz; $\sigma = 0.941$ S/m; $\epsilon_r = 41.8$

Ambient Temperature: 23.5°C; Liquid Temperature: 22.5°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7625; ConvF(8.91, 8.7, 9.42); Calibrated: 2024-12-13
- Sensor-Surface: 1.4 mm
- Electronics: DAE4ip Sn1800; Calibrated: 2024-06-18
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2144; Section: Flat
- Measurement Software: 16.2.4.2524
- UID: CW, 0

Pin=24.0dBm/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 2.42 W/kg; SAR (10g) = 1.59 W/kg;


Pin=24.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm

Power Drift = -0.01 dB

SAR (1g) = 2.44 W/kg; SAR (8g) = 1.72 W/kg; SAR (10g) = 1.63 W/kg

Smallest distance from peaks to all points 3 dB below = 19.0 mm

Ratio of SAR at M2 to SAR at M1 = 87.5 %

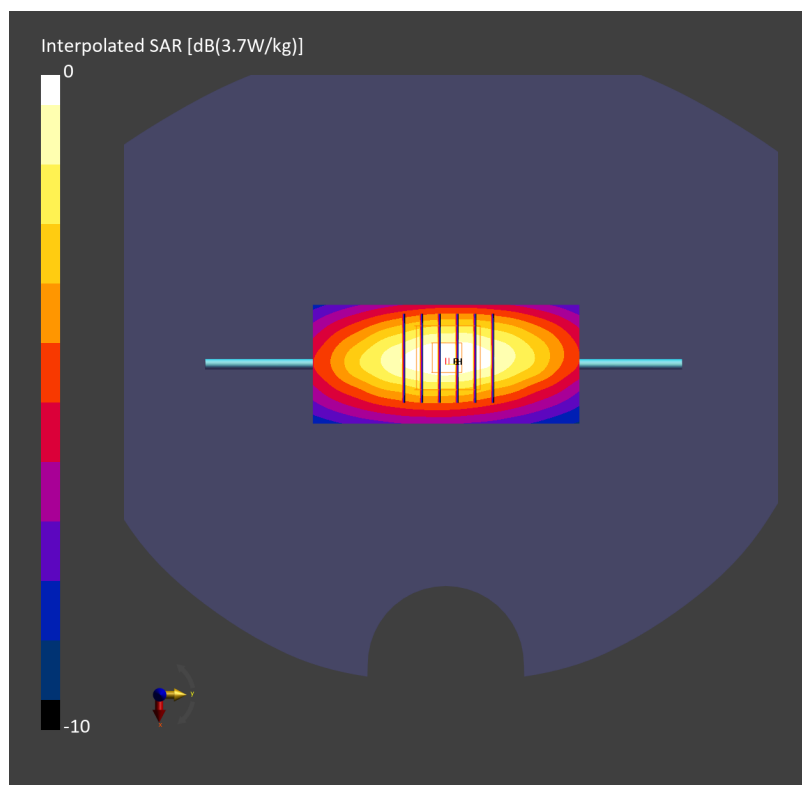

Date: 2025-02-02

System Check_Head_835MHz**DUT: D835V2 - SN4d167**

Communication System: CW; Frequency: 835.000 MHz

Medium: HSL_850_250202 Medium parameters used: $f = 835.000$ MHz; $\sigma = 0.933$ S/m; $\epsilon_r = 42.8$

Ambient Temperature: 23.3°C; Liquid Temperature: 22.3°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7625; ConvF(8.91, 8.7, 9.42); Calibrated: 2024-12-13
- Sensor-Surface: 1.4 mm
- Electronics: DAE4ip Sn1800; Calibrated: 2024-06-18
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2144; Section: Flat
- Measurement Software: 16.2.4.2524
- UID: CW, 0

Pin=24.0dBm/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 2.33 W/kg; SAR (10g) = 1.54 W/kg;


Pin=24.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm

Power Drift = -0.00 dB

SAR (1g) = 2.35 W/kg; SAR (8g) = 1.65 W/kg; SAR (10g) = 1.57 W/kg

Smallest distance from peaks to all points 3 dB below = 19.0 mm

Ratio of SAR at M2 to SAR at M1 = 87.3 %

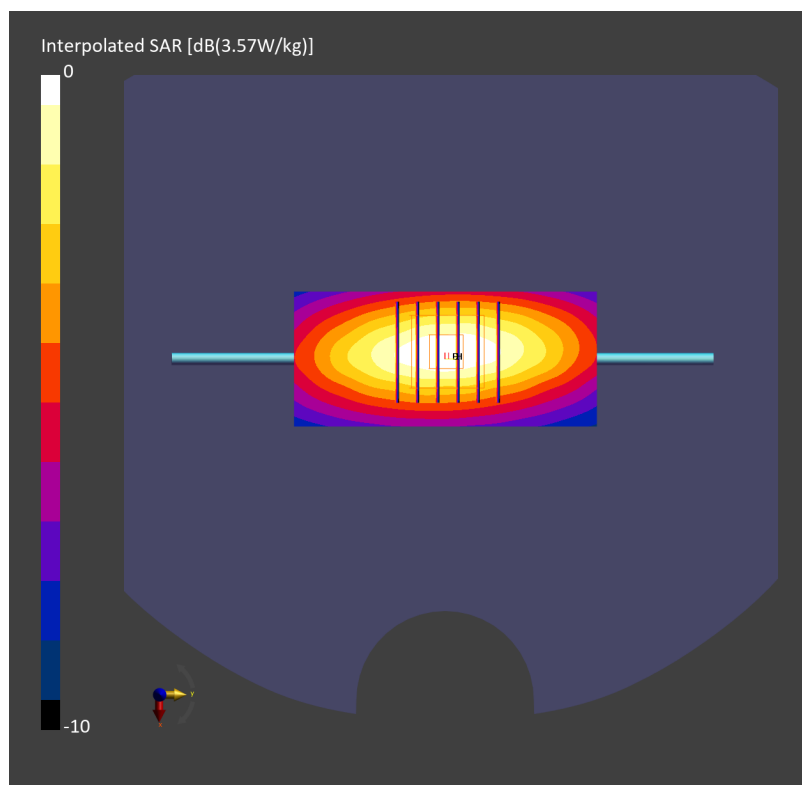

Date: 2025-02-10

System Check_Head_835MHz**DUT: D835V2 - SN4d167**

Communication System: CW; Frequency: 835.000 MHz

Medium: HSL_850_250210 Medium parameters used: $f = 835.000$ MHz; $\sigma = 0.928$ S/m; $\epsilon_r = 42.7$

Ambient Temperature: 23.3°C; Liquid Temperature: 22.3°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7625; ConvF(8.91, 8.7, 9.42); Calibrated: 2024-12-13
- Sensor-Surface: 1.4 mm
- Electronics: DAE4ip Sn1800; Calibrated: 2024-06-18
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2144; Section: Flat
- Measurement Software: 16.2.4.2524
- UID: CW, 0

Pin=24.0dBm/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 2.54 W/kg; SAR (10g) = 1.67 W/kg;


Pin=24.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm

Power Drift = -0.02 dB

SAR (1g) = 2.56 W/kg; SAR (8g) = 1.81 W/kg; SAR (10g) = 1.72 W/kg

Smallest distance from peaks to all points 3 dB below = 19.6 mm

Ratio of SAR at M2 to SAR at M1 = 87.6 %

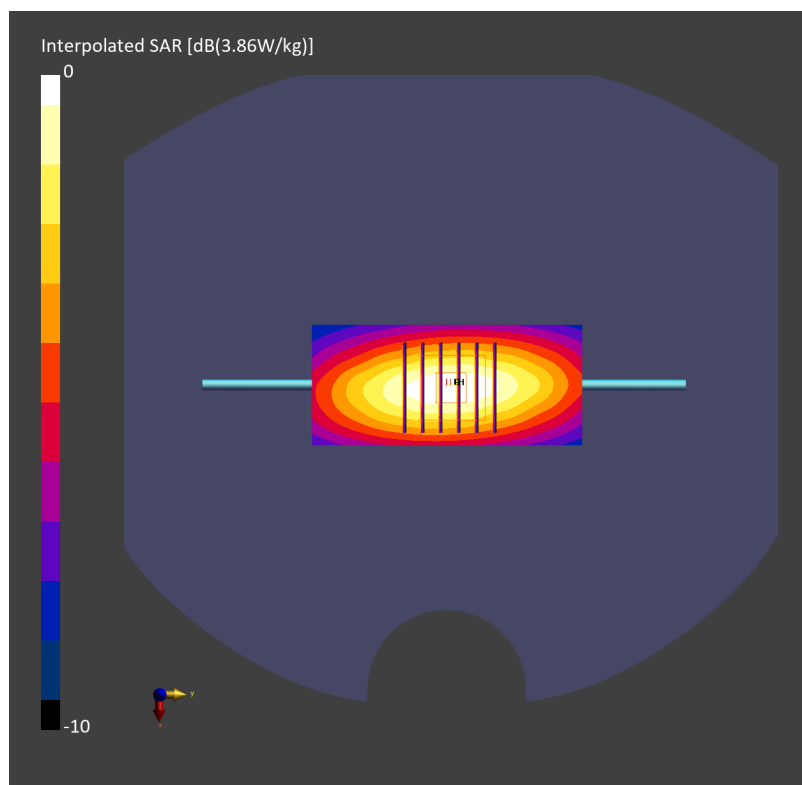

Date: 2025-02-15

System Check_Head_835MHz**DUT: D835V2 - SN4d167**

Communication System: CW; Frequency: 835.000 MHz

Medium: HSL_850_250215 Medium parameters used: $f = 835.000$ MHz; $\sigma = 0.916$ S/m; $\epsilon_r = 42.4$

Ambient Temperature: 23.5°C; Liquid Temperature: 22.5°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7625; ConvF(8.91, 8.7, 9.42); Calibrated: 2024-12-13
- Sensor-Surface: 1.4 mm
- Electronics: DAE4ip Sn1800; Calibrated: 2024-06-18
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2144; Section: Flat
- Measurement Software: 16.2.4.2524
- UID: CW, 0

Pin=24.0dBm/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 2.26 W/kg; SAR (10g) = 1.48 W/kg;


Pin=24.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm

Power Drift = 0.01 dB

SAR (1g) = 2.27 W/kg; SAR (8g) = 1.60 W/kg; SAR (10g) = 1.52 W/kg

Smallest distance from peaks to all points 3 dB below = 18.4 mm

Ratio of SAR at M2 to SAR at M1 = 87.6 %

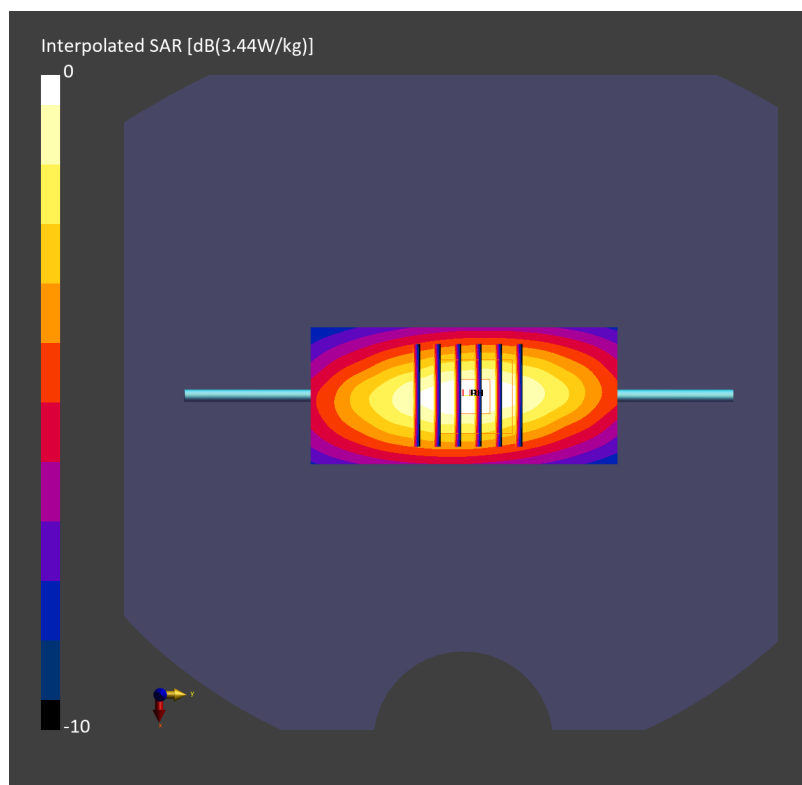

Date: 2025-02-18

System Check_Head_835MHz**DUT: D835V2 - SN4d167**

Communication System: CW; Frequency: 835.000 MHz

Medium: HSL_850_250218 Medium parameters used: $f = 835.000$ MHz; $\sigma = 0.937$ S/m; $\epsilon_r = 40.3$

Ambient Temperature: 23.6°C; Liquid Temperature: 22.6°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7625; ConvF(8.91, 8.7, 9.42); Calibrated: 2024-12-13
- Sensor-Surface: 1.4 mm
- Electronics: DAE4ip Sn1800; Calibrated: 2024-06-18
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2144; Section: Flat
- Measurement Software: 16.2.4.2524
- UID: CW, 0

Pin=24.0dBm/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 2.47 W/kg; SAR (10g) = 1.62 W/kg;


Pin=24.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm

Power Drift = 0.01 dB

SAR (1g) = 2.48 W/kg; SAR (8g) = 1.75 W/kg; SAR (10g) = 1.66 W/kg

Smallest distance from peaks to all points 3 dB below = 20.5 mm

Ratio of SAR at M2 to SAR at M1 = 87.1 %

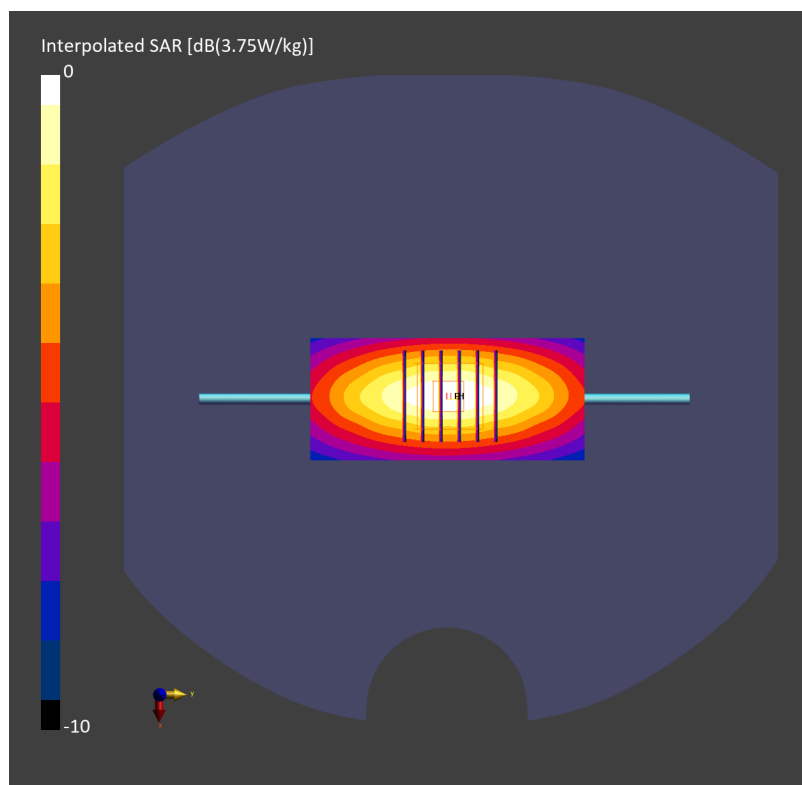

Date: 2025-03-05

System Check_Head_835MHz**DUT: D835V2 - SN4d167**

Communication System: CW; Frequency: 835.000 MHz

Medium: HSL_850_250305 Medium parameters used: $f = 835.000$ MHz; $\sigma = 0.926$ S/m; $\epsilon_r = 40.1$

Ambient Temperature: 23.5°C; Liquid Temperature: 22.5°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7625; ConvF(8.91, 8.7, 9.42); Calibrated: 2024-12-13
- Sensor-Surface: 1.4 mm
- Electronics: DAE4ip Sn1800; Calibrated: 2024-06-18
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2144; Section: Flat
- Measurement Software: 16.2.4.2524
- UID: CW, 0

Pin=24.0dBm/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 2.54 W/kg; SAR (10g) = 1.67 W/kg;


Pin=24.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm

Power Drift = -0.01 dB

SAR (1g) = 2.54 W/kg; SAR (8g) = 1.79 W/kg; SAR (10g) = 1.70 W/kg

Smallest distance from peaks to all points 3 dB below = 20.5 mm

Ratio of SAR at M2 to SAR at M1 = 87.0 %

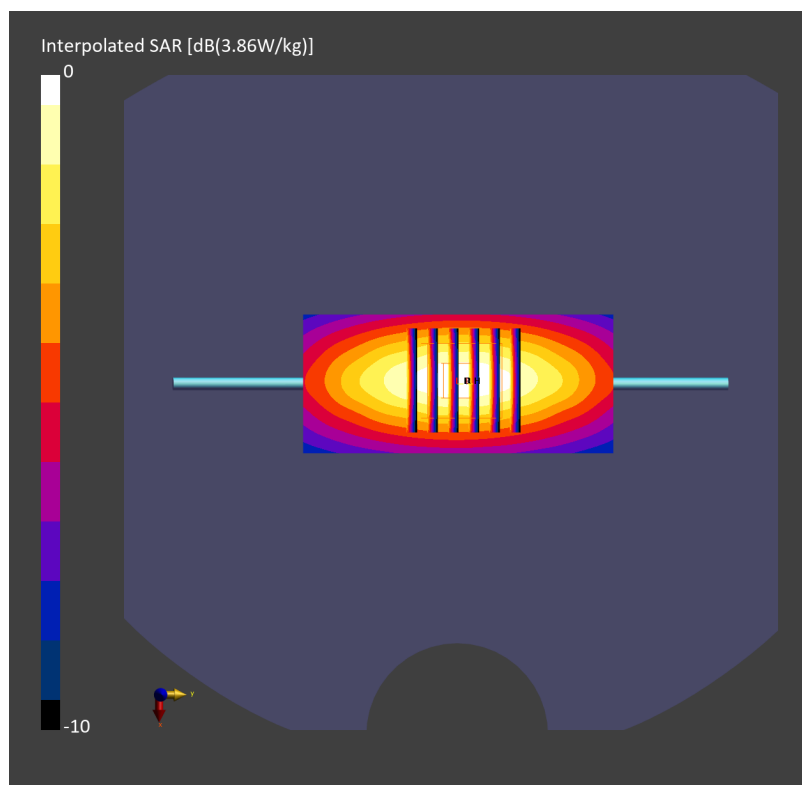

Date: 2025-02-18

System Check_Head_1640MHz**DUT: D1640V2 - SN346**

Communication System: CW; Frequency: 1640.000 MHz

Medium: HSL_1640_250218 Medium parameters used: $f = 1640.000$ MHz; $\sigma = 1.26$ S/m; $\epsilon_r = 39.9$

Ambient Temperature: 23.8°C; Liquid Temperature: 22.8°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7785; ConvF(6.85, 7.21, 7.06); Calibrated: 2024-11-28
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1694; Calibrated: 2024-11-19
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2126
- Measurement Software: 16.2.4.2524
- UID: CW

Pin=17.0dBm/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 1.64 W/kg; SAR (10g) = 0.892 W/kg;


Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm

Power Drift = 0.01 dB

SAR (1g) = 1.64 W/kg; SAR (8g) = 0.979 W/kg; SAR (10g) = 0.908 W/kg

Smallest distance from peaks to all points 3 dB below = 10.8 mm

Ratio of SAR at M2 to SAR at M1 = 85.3 %

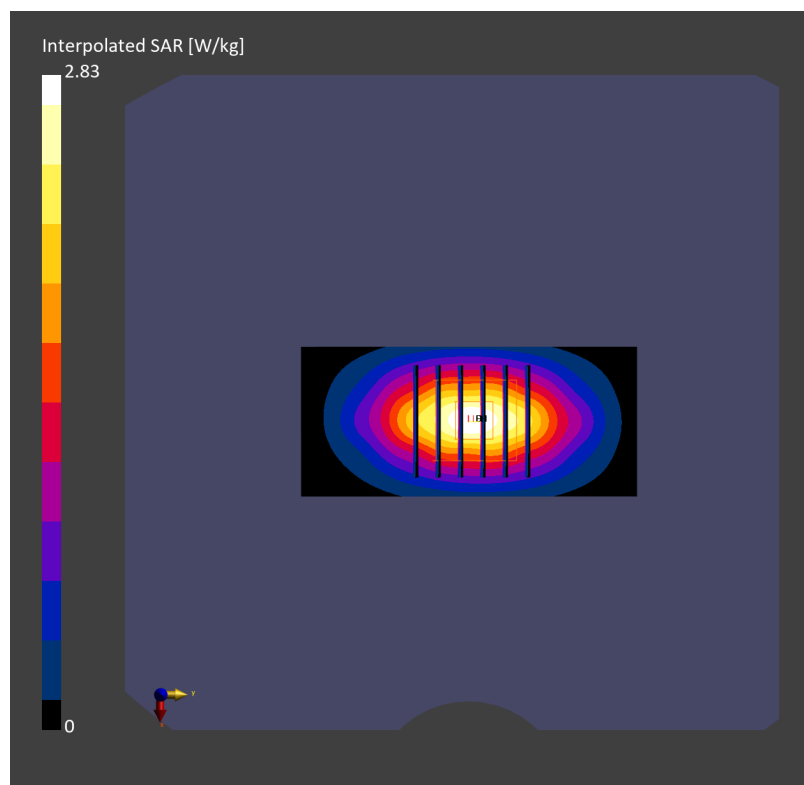

Date: 2025-01-31

System Check_Head_1750MHz**DUT: D1750V2 - SN1120**

Communication System: CW; Frequency: 1750.000 MHz

Medium: HSL_1750_250131 Medium parameters used: $f = 1750.000$ MHz; $\sigma = 1.37$ S/m; $\epsilon_r = 40.8$

Ambient Temperature: 23.4°C; Liquid Temperature: 22.4°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7625; ConvF(7.8, 7.61, 8.24); Calibrated: 2024-12-13
- Sensor-Surface: 1.4 mm
- Electronics: DAE4ip Sn1800; Calibrated: 2024-06-18
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2144
- Measurement Software: 16.2.4.2524
- UID: CW

Pin=17.0dBm/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 1.88 W/kg; SAR (10g) = 1.00 W/kg;


Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm

Power Drift = 0.00 dB

SAR (1g) = 1.87 W/kg; SAR (8g) = 1.08 W/kg; SAR (10g) = 1.00 W/kg

Smallest distance from peaks to all points 3 dB below = 9.7 mm

Ratio of SAR at M2 to SAR at M1 = 83.6 %

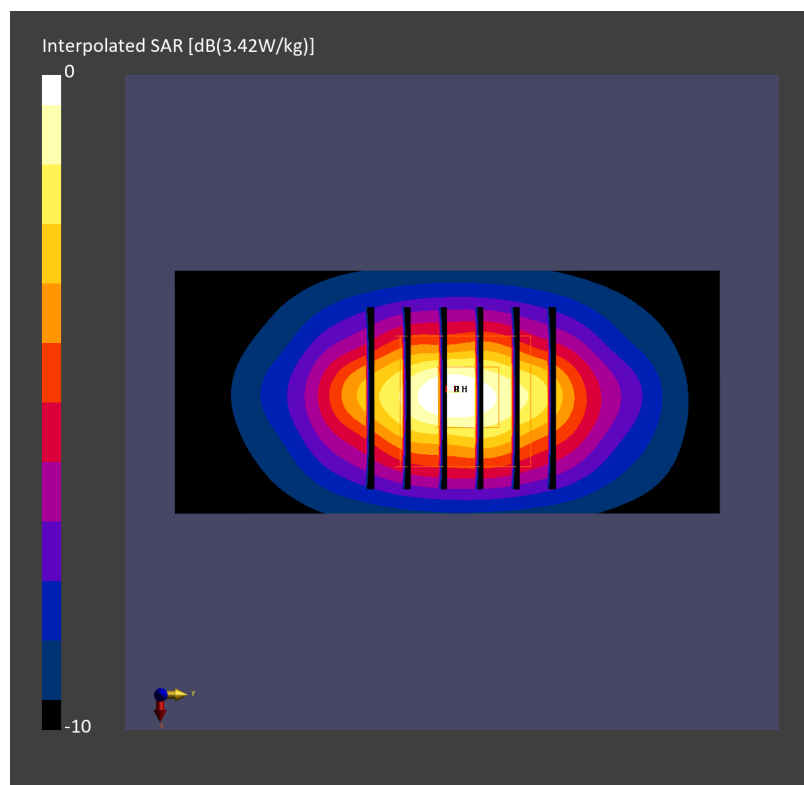

Date: 2025-02-04

System Check_Head_1750MHz**DUT: D1750V2 - SN1120**

Communication System: CW; Frequency: 1750.000 MHz

Medium: HSL_1750_250204 Medium parameters used: $f = 1750.000$ MHz; $\sigma = 1.37$ S/m; $\epsilon_r = 40.5$

Ambient Temperature: 23.4°C; Liquid Temperature: 22.4°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7625; ConvF(7.8, 7.61, 8.24); Calibrated: 2024-12-13
- Sensor-Surface: 1.4 mm
- Electronics: DAE4ip Sn1800; Calibrated: 2024-06-18
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2144
- Measurement Software: 16.2.4.2524
- UID: CW

Pin=17.0dBm/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 1.86 W/kg; SAR (10g) = 1.00 W/kg;


Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm

Power Drift = -0.00 dB

SAR (1g) = 1.87 W/kg; SAR (8g) = 1.08 W/kg; SAR (10g) = 0.999 W/kg

Smallest distance from peaks to all points 3 dB below = 9.7 mm

Ratio of SAR at M2 to SAR at M1 = 83.3 %

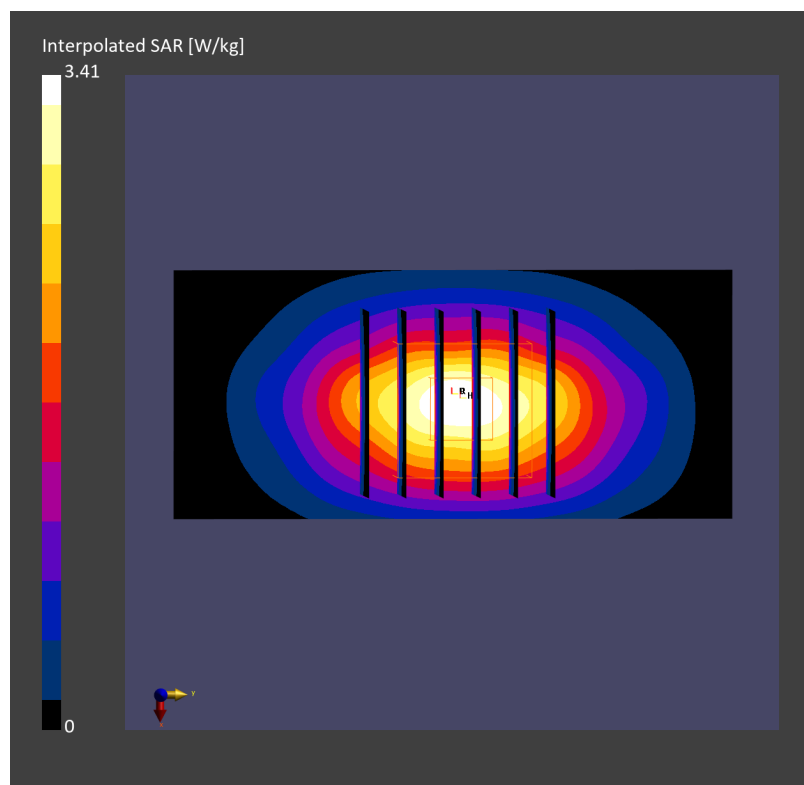

Date: 2025-02-07

System Check_Head_1750MHz**DUT: D1750V2 - SN1120**

Communication System: CW; Frequency: 1750.000 MHz

Medium: HSL_1750_250207 Medium parameters used: $f = 1750.000$ MHz; $\sigma = 1.35$ S/m; $\epsilon_r = 40.9$

Ambient Temperature: 23.3°C; Liquid Temperature: 22.3°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7625; ConvF(7.8, 7.61, 8.24); Calibrated: 2024-12-13
- Sensor-Surface: 1.4 mm
- Electronics: DAE4ip Sn1800; Calibrated: 2024-06-18
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2144
- Measurement Software: 16.2.4.2524
- UID: CW

Pin=17.0dBm/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 1.80 W/kg; SAR (10g) = 0.962 W/kg;


Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm

Power Drift = 0.04 dB

SAR (1g) = 1.78 W/kg; SAR (8g) = 1.03 W/kg; SAR (10g) = 0.947 W/kg

Smallest distance from peaks to all points 3 dB below = 10.9 mm

Ratio of SAR at M2 to SAR at M1 = 83.4 %

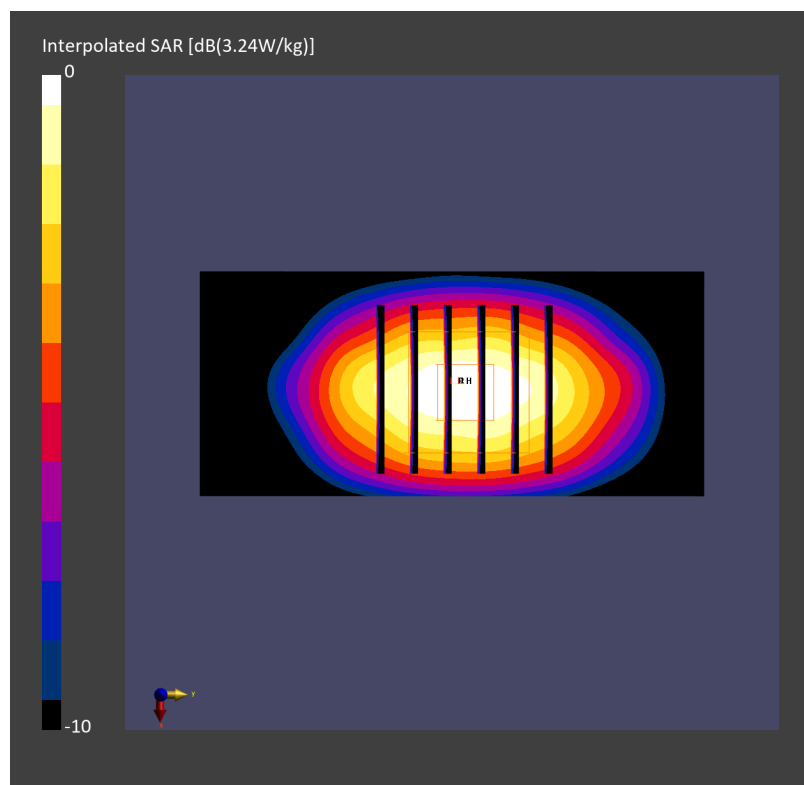

Date: 2025-02-13

System Check_Head_1750MHz**DUT: D1750V2 - SN1120**

Communication System: CW; Frequency: 1750.000 MHz

Medium: HSL_1750_250213 Medium parameters used: $f = 1750.000$ MHz; $\sigma = 1.38$ S/m; $\epsilon_r = 40.9$

Ambient Temperature: 23.6°C; Liquid Temperature: 22.6°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7625; ConvF(7.8, 7.61, 8.24); Calibrated: 2024-12-13
- Sensor-Surface: 1.4 mm
- Electronics: DAE4ip Sn1800; Calibrated: 2024-06-18
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2144
- Measurement Software: 16.2.4.2524
- UID: CW

Pin=17.0dBm/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 1.88 W/kg; SAR (10g) = 1.00 W/kg;


Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm

Power Drift = 0.01 dB

SAR (1g) = 1.88 W/kg; SAR (8g) = 1.09 W/kg; SAR (10g) = 1.01 W/kg

Smallest distance from peaks to all points 3 dB below = 10.8 mm

Ratio of SAR at M2 to SAR at M1 = 83.2 %

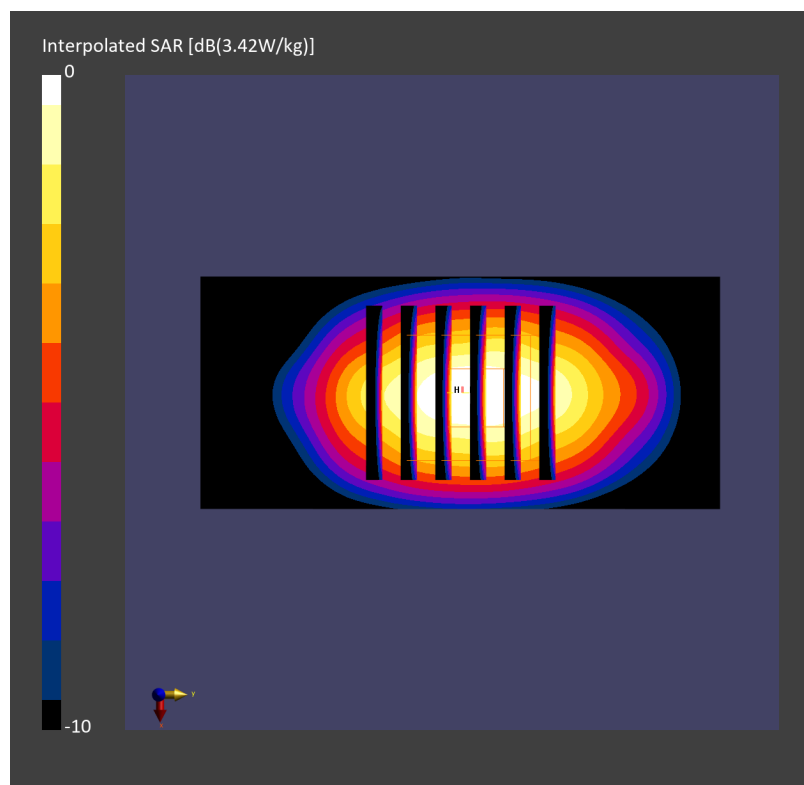

Date: 2025-02-26

System Check_Head_1750MHz**DUT: D1750V2 - SN1120**

Communication System: CW; Frequency: 1750.000 MHz

Medium: HSL_1750_250226 Medium parameters used: $f = 1750.000$ MHz; $\sigma = 1.36$ S/m; $\epsilon_r = 40.9$

Ambient Temperature: 23.6°C; Liquid Temperature: 22.6°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7625; ConvF(7.8, 7.61, 8.24); Calibrated: 2024-12-13
- Sensor-Surface: 1.4 mm
- Electronics: DAE4ip Sn1800; Calibrated: 2024-06-18
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2144; Section: Flat
- Measurement Software: 16.2.4.2524
- UID: CW

Pin=17.0dBm/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 1.75 W/kg; SAR (10g) = 0.955 W/kg;

Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5


mm

Power Drift = -0.01 dB

SAR (1g) = 1.78 W/kg; SAR (8g) = 1.03 W/kg; SAR (10g) = 0.952 W/kg

Smallest distance from peaks to all points 3 dB below = 9.9 mm

Ratio of SAR at M2 to SAR at M1 = 83.6 %

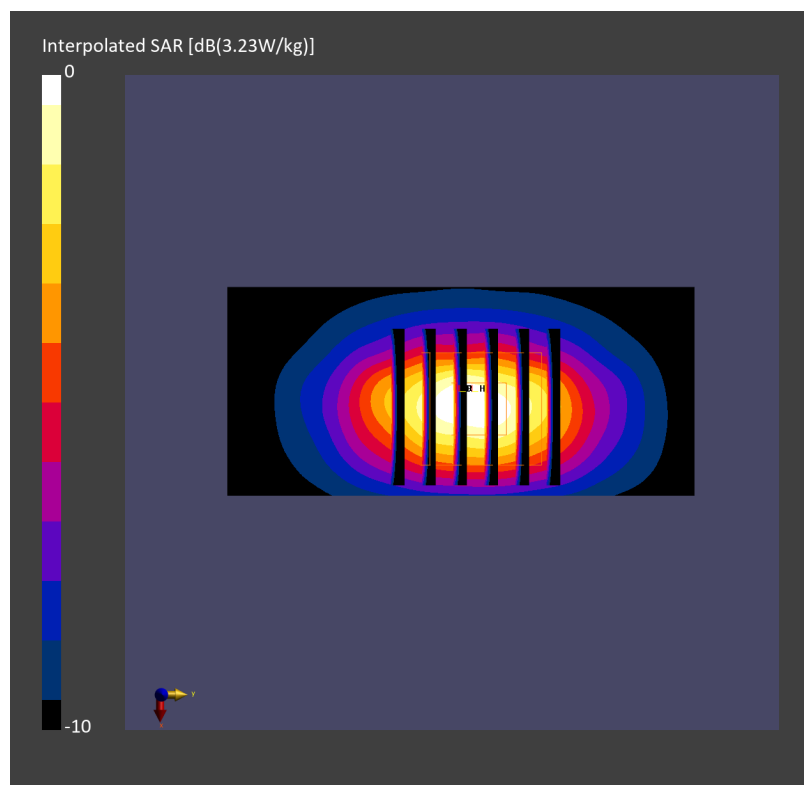

Date: 2025-02-27

System Check_Head_1750MHz**DUT: D1750V2 - SN1120**

Communication System: CW; Frequency: 1750.000 MHz

Medium: HSL_1750_250227 Medium parameters used: $f = 1750.000$ MHz; $\sigma = 1.35$ S/m; $\epsilon_r = 40.8$

Ambient Temperature: 23.7°C; Liquid Temperature: 22.7°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7625; ConvF(7.8, 7.61, 8.24); Calibrated: 2024-12-13
- Sensor-Surface: 1.4 mm
- Electronics: DAE4ip Sn1800; Calibrated: 2024-06-18
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2144
- Measurement Software: 16.2.4.2524
- UID: CW

Pin=17.0dBm/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 1.73 W/kg; SAR (10g) = 0.947 W/kg;


Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm

Power Drift = -0.04 dB

SAR (1g) = 1.76 W/kg; SAR (8g) = 1.02 W/kg; SAR (10g) = 0.943 W/kg

Smallest distance from peaks to all points 3 dB below = 9.9 mm

Ratio of SAR at M2 to SAR at M1 = 83.6 %

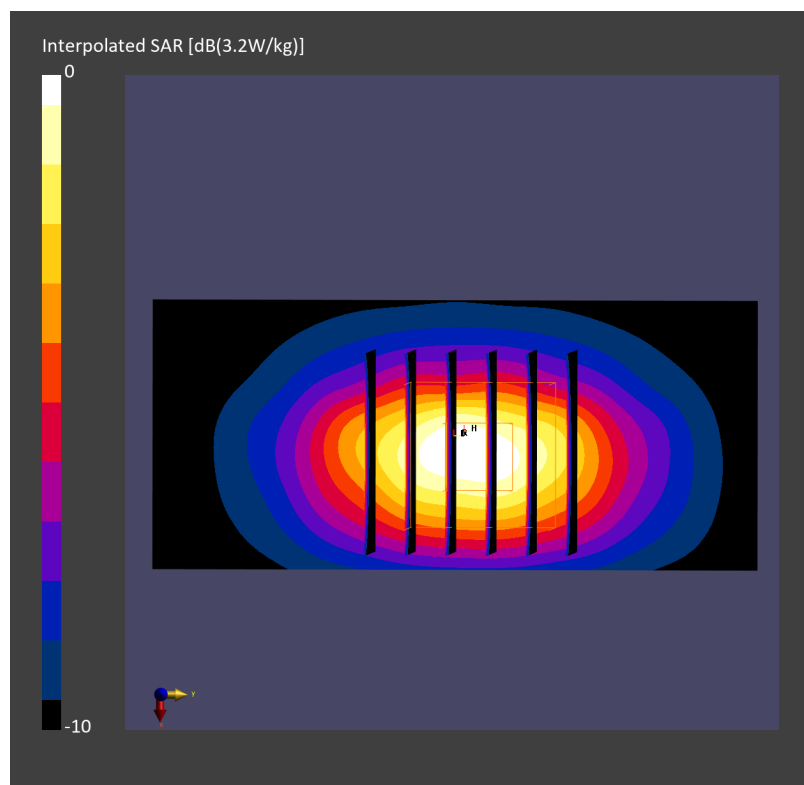

Date: 2025-01-29

System Check_Head_1900MHz**DUT: D1900V2 - SN5d093**

Communication System: CW; Frequency: 1900.000 MHz

Medium: HSL_1900_250129 Medium parameters used: $f = 1900.000$ MHz; $\sigma = 1.40$ S/m; $\epsilon_r = 39.2$

Ambient Temperature: 23.6°C; Liquid Temperature: 22.6°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7625; ConvF(7.49, 7.31, 7.91); Calibrated: 2024-12-13
- Sensor-Surface: 1.4 mm
- Electronics: DAE4ip Sn1800; Calibrated: 2024-06-18
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2144
- Measurement Software: 16.2.4.2524
- UID: CW

Pin=17.0dBm/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 1.91 W/kg; SAR (10g) = 1.02 W/kg;


Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm

Power Drift = 0.02 dB

SAR (1g) = 1.97 W/kg; SAR (8g) = 1.12 W/kg; SAR (10g) = 1.03 W/kg

Smallest distance from peaks to all points 3 dB below = 9.7 mm

Ratio of SAR at M2 to SAR at M1 = 82.8 %

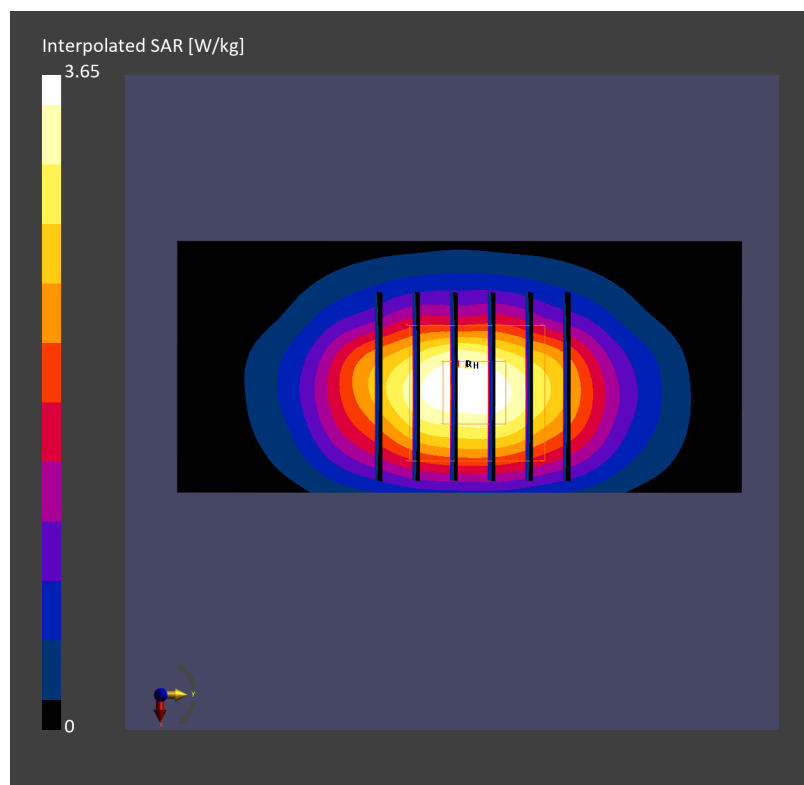

Date: 2025-01-30

System Check_Head_1900MHz**DUT: D1900V2 - SN5d093**

Communication System: CW; Frequency: 1900.000 MHz

Medium: HSL_1900_250130 Medium parameters used: $f = 1900.000$ MHz; $\sigma = 1.39$ S/m; $\epsilon_r = 40.9$

Ambient Temperature: 23.5°C; Liquid Temperature: 22.5°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7625; ConvF(7.49, 7.31, 7.91); Calibrated: 2024-12-13
- Sensor-Surface: 1.4 mm
- Electronics: DAE4ip Sn1800; Calibrated: 2024-06-18
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2144
- Measurement Software: 16.2.4.2524
- UID: CW

Pin=17.0dBm/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 1.98 W/kg; SAR (10g) = 1.03 W/kg;


Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm

Power Drift = 0.01 dB

SAR (1g) = 1.99 W/kg; SAR (8g) = 1.12 W/kg; SAR (10g) = 1.03 W/kg

Smallest distance from peaks to all points 3 dB below = 9.7 mm

Ratio of SAR at M2 to SAR at M1 = 82.9 %

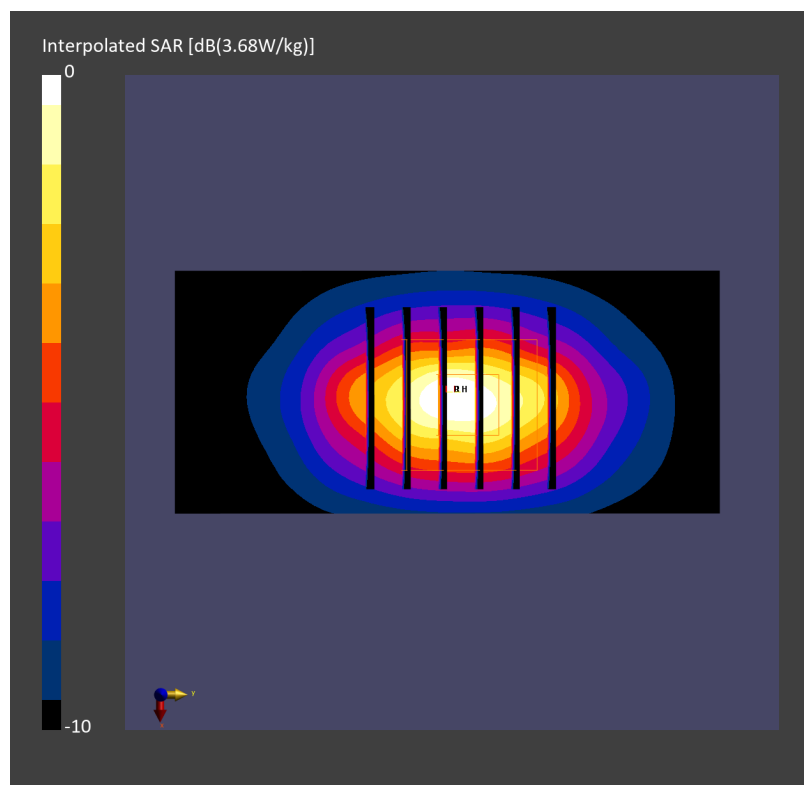

Date: 2025-02-03

System Check_Head_1900MHz**DUT: D1900V2 - SN5d093**

Communication System: CW; Frequency: 1900.000 MHz

Medium: HSL_1900_250203 Medium parameters used: $f = 1900.000$ MHz; $\sigma = 1.43$ S/m; $\epsilon_r = 39.4$

Ambient Temperature: 23.5°C; Liquid Temperature: 22.5°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7625; ConvF(7.49, 7.31, 7.91); Calibrated: 2024-12-13
- Sensor-Surface: 1.4 mm
- Electronics: DAE4ip Sn1800; Calibrated: 2024-06-18
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2144
- Measurement Software: 16.2.4.2524
- UID: CW

Pin=17.0dBm/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 2.02 W/kg; SAR (10g) = 1.05 W/kg;


Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm

Power Drift = -0.00 dB

SAR (1g) = 2.03 W/kg; SAR (8g) = 1.15 W/kg; SAR (10g) = 1.05 W/kg

Smallest distance from peaks to all points 3 dB below = 9.7 mm

Ratio of SAR at M2 to SAR at M1 = 83.0 %

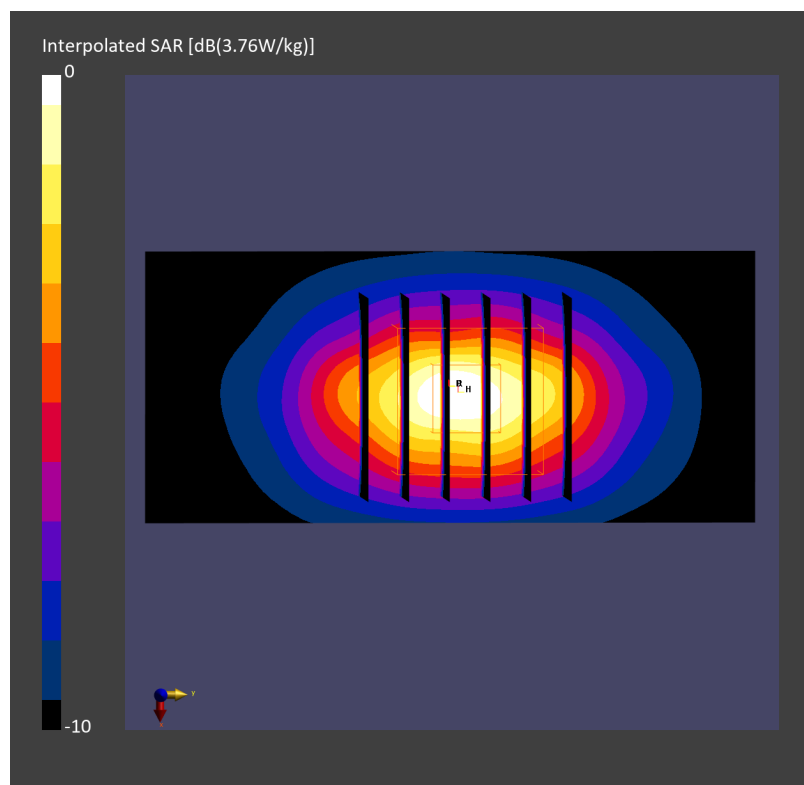

Date: 2025-02-06

System Check_Head_1900MHz**DUT: D1900V2 - SN5d185**

Communication System: CW; Frequency: 1900.000 MHz

Medium: HSL_1900_250206 Medium parameters used: $f = 1900.000$ MHz; $\sigma = 1.39$ S/m; $\epsilon_r = 40.1$

Ambient Temperature: 23.3°C; Liquid Temperature: 22.3°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7625; ConvF(7.49, 7.31, 7.91); Calibrated: 2024-12-13
- Sensor-Surface: 1.4 mm
- Electronics: DAE4ip Sn1800; Calibrated: 2024-06-18
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2144
- Measurement Software: 16.2.4.2524
- UID: CW

Pin=17.0dBm/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 1.93 W/kg; SAR (10g) = 0.998 W/kg;


Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm

Power Drift = 0.02 dB

SAR (1g) = 1.94 W/kg; SAR (8g) = 1.10 W/kg; SAR (10g) = 1.01 W/kg

Smallest distance from peaks to all points 3 dB below = 9.7 mm

Ratio of SAR at M2 to SAR at M1 = 82.7 %

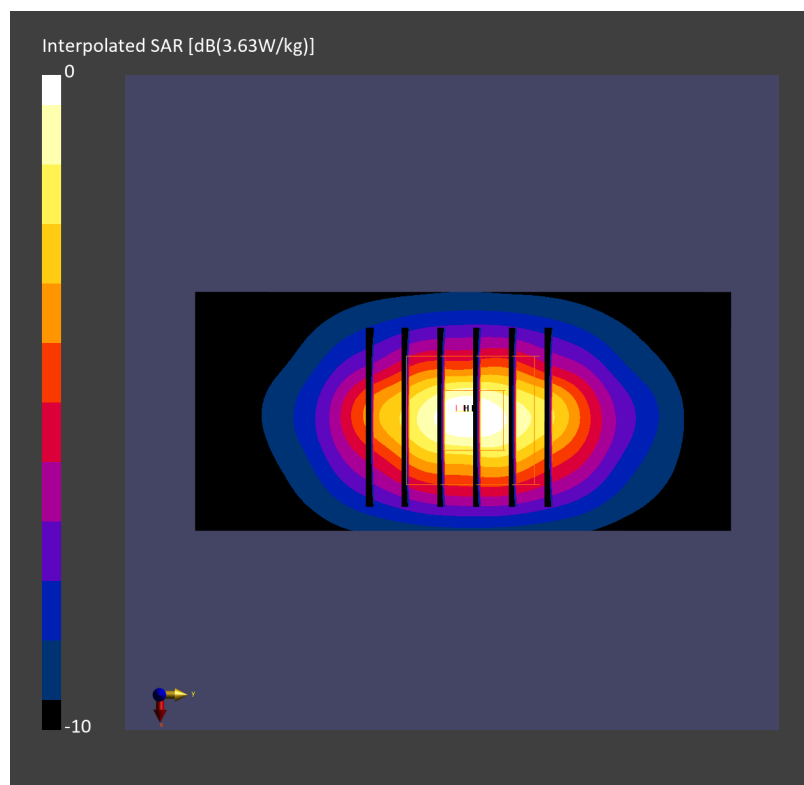

Date: 2025-02-17

System Check_Head_1900MHz**DUT: D1900V2 - SN5d185**

Communication System: CW; Frequency: 1900.000 MHz

Medium: HSL_1900_250217 Medium parameters used: $f = 1900.000$ MHz; $\sigma = 1.43$ S/m; $\epsilon_r = 40.9$

Ambient Temperature: 23.2°C; Liquid Temperature: 22.2°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7625; ConvF(7.49, 7.31, 7.91); Calibrated: 2024-12-13
- Sensor-Surface: 1.4 mm
- Electronics: DAE4ip Sn1800; Calibrated: 2024-06-18
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2144
- Measurement Software: 16.2.4.2524
- UID: CW

Pin=17.0dBm/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 1.96 W/kg; SAR (10g) = 1.01 W/kg;


Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm

Power Drift = -0.01 dB

SAR (1g) = 1.98 W/kg; SAR (8g) = 1.12 W/kg; SAR (10g) = 1.03 W/kg

Smallest distance from peaks to all points 3 dB below = 9.7 mm

Ratio of SAR at M2 to SAR at M1 = 82.9 %

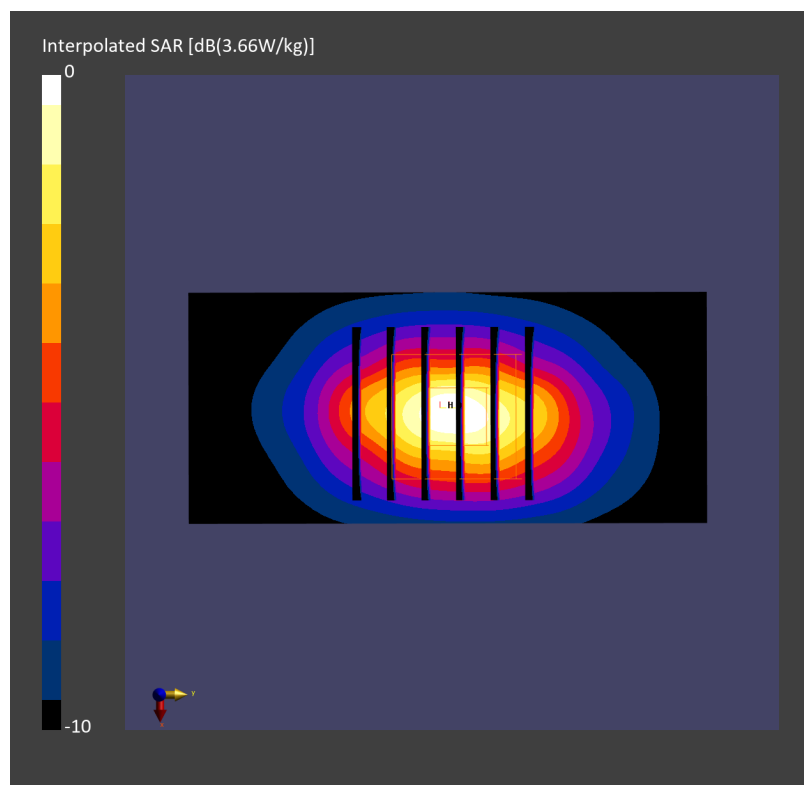

Date: 2025-02-26

System Check_Head_1900MHz**DUT: D1900V2 - SN5d093**

Communication System: CW; Frequency: 1900.000 MHz

Medium: HSL_1900_250226 Medium parameters used: $f = 1900.000$ MHz; $\sigma = 1.38$ S/m; $\epsilon_r = 40.6$

Ambient Temperature: 23.6°C; Liquid Temperature: 22.6°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7625; ConvF(7.49, 7.31, 7.91); Calibrated: 2024-12-13
- Sensor-Surface: 1.4 mm
- Electronics: DAE4ip Sn1800; Calibrated: 2024-06-18
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2144; Section: Flat
- Measurement Software: 16.2.4.2524
- UID: CW

Pin=17.0dBm/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 1.91 W/kg; SAR (10g) = 0.998 W/kg;


Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm

Power Drift = 0.01 dB

SAR (1g) = 1.92 W/kg; SAR (8g) = 1.09 W/kg; SAR (10g) = 1.00 W/kg

Smallest distance from peaks to all points 3 dB below = 9.7 mm

Ratio of SAR at M2 to SAR at M1 = 82.9 %

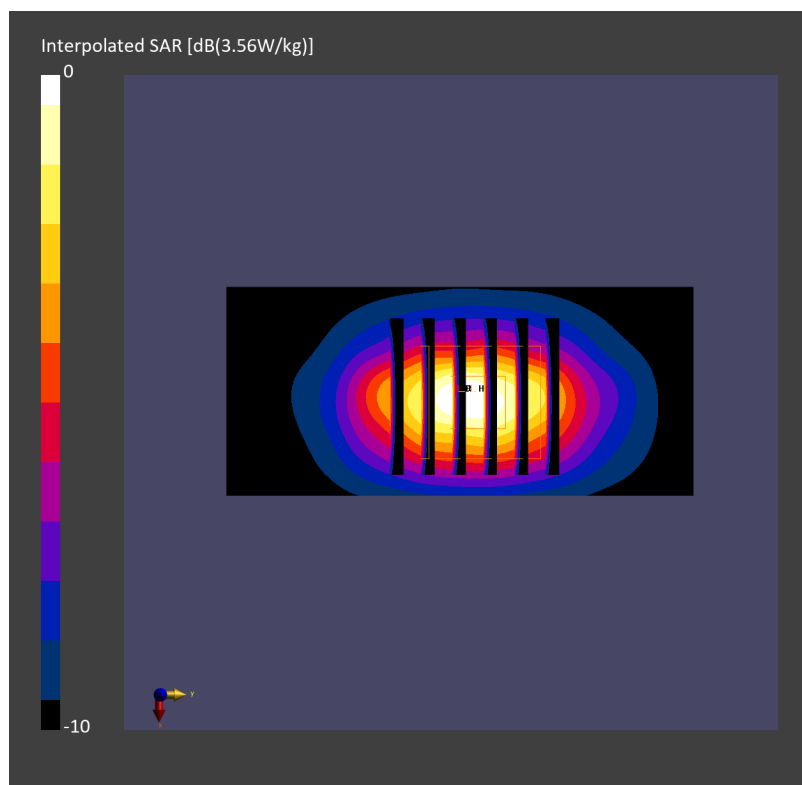

Date: 2025-02-18

System Check_Head_2000MHz**DUT: D2000V2 - SN1010**

Communication System: CW; Frequency: 2000.000 MHz

Medium: HSL_2000_250218 Medium parameters used: $f = 2000.000$ MHz; $\sigma = 1.43$ S/m; $\epsilon_r = 39.3$

Ambient Temperature: 23.8°C; Liquid Temperature: 22.8°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7785; ConvF(6.69, 7.05, 6.9); Calibrated: 2024-11-28
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1694; Calibrated: 2024-11-19
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2126
- Measurement Software: 16.2.4.2524
- UID: CW

Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 1.89 W/kg; SAR (10g) = 0.959 W/kg;


Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.5 mm

Power Drift = 0.02 dB

SAR (1g) = 1.89 W/kg; SAR (8g) = 1.07 W/kg; SAR (10g) = 0.986 W/kg

Smallest distance from peaks to all points 3 dB below = 10.0 mm

Ratio of SAR at M2 to SAR at M1 = 83.8 %

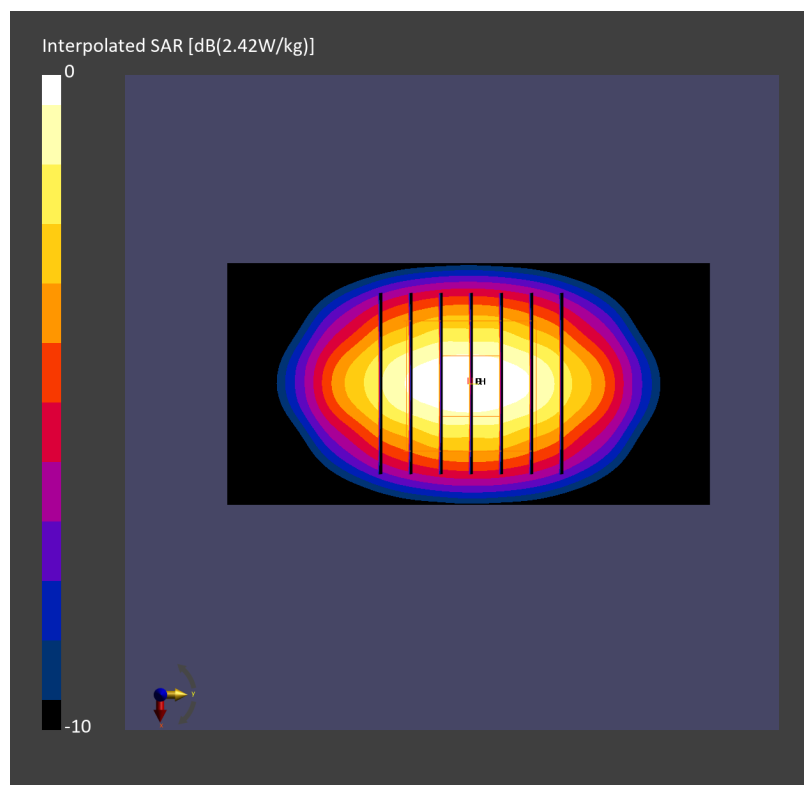

Date: 2025-02-12

System Check_Head_2300MHz**DUT: D2300V2 - SN1088**

Communication System: CW; Frequency: 2300.000 MHz

Medium: HSL_2300_250212 Medium parameters used: $f = 2300.000$ MHz; $\sigma = 1.67$ S/m; $\epsilon_r = 40.5$

Ambient Temperature: 23.6°C; Liquid Temperature: 22.6°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7625; ConvF(7.16, 6.99, 7.56); Calibrated: 2024-12-13
- Sensor-Surface: 1.4 mm
- Electronics: DAE4ip Sn1800; Calibrated: 2024-06-18
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2144
- Measurement Software: 16.2.4.2524
- UID: CW

Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 2.73 W/kg; SAR (10g) = 1.35 W/kg;


Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.5 mm

Power Drift = -0.16 dB

SAR (1g) = 2.52 W/kg; SAR (8g) = 1.32 W/kg; SAR (10g) = 1.20 W/kg

Smallest distance from peaks to all points 3 dB below = 9.0 mm

Ratio of SAR at M2 to SAR at M1 = 80.5 %

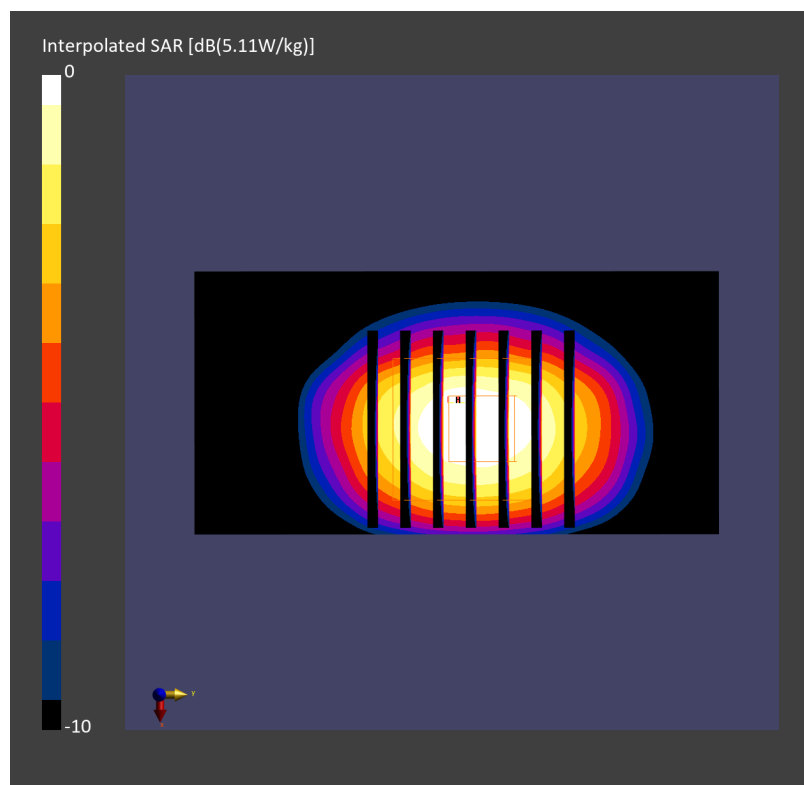

Date: 2025-02-27

System Check_Head_2300MHz**DUT: D2300V2 - SN1088**

Communication System: CW; Frequency: 2300.000 MHz

Medium: HSL_2300_250227 Medium parameters used: $f = 2300.000$ MHz; $\sigma = 1.64$ S/m; $\epsilon_r = 39.6$

Ambient Temperature: 23.7°C; Liquid Temperature: 22.7°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7625; ConvF(7.16, 6.99, 7.56); Calibrated: 2024-12-13
- Sensor-Surface: 1.4 mm
- Electronics: DAE4ip Sn1800; Calibrated: 2024-06-18
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2144
- Measurement Software: 16.2.4.2524
- UID: CW

Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 2.69 W/kg; SAR (10g) = 1.33 W/kg;


Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.5 mm

Power Drift = -0.08 dB

SAR (1g) = 2.48 W/kg; SAR (8g) = 1.30 W/kg; SAR (10g) = 1.18 W/kg

Smallest distance from peaks to all points 3 dB below = 9.0 mm

Ratio of SAR at M2 to SAR at M1 = 80.5 %

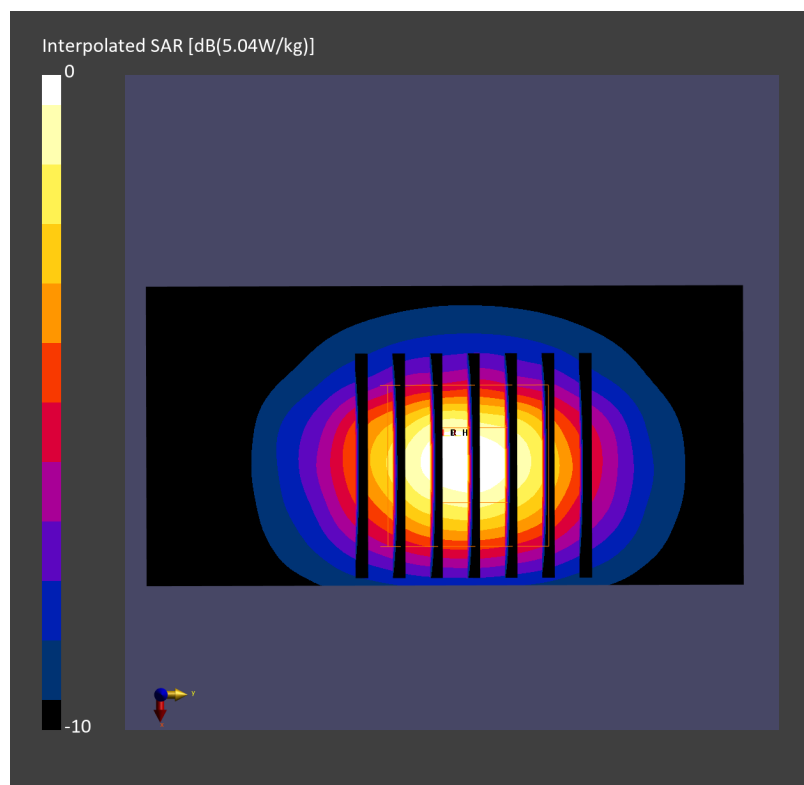

Date: 2025-01-27

System Check_Head_2600MHz**DUT: D2600V2 - SN1089**

Communication System: CW; Frequency: 2600.000 MHz

Medium: HSL_2600_250127 Medium parameters used: $f = 2600.000$ MHz; $\sigma = 1.98$ S/m; $\epsilon_r = 38.2$

Ambient Temperature: 23.3°C; Liquid Temperature: 22.3°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7625; ConvF(6.85, 6.68, 7.24); Calibrated: 2024-12-13
- Sensor-Surface: 1.4 mm
- Electronics: DAE4ip Sn1800; Calibrated: 2024-06-18
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2144
- Measurement Software: 16.2.4.2524
- UID: CW

Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 2.67 W/kg; SAR (10g) = 1.18 W/kg;


Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.5 mm

Power Drift = 0.04 dB

SAR (1g) = 2.65 W/kg; SAR (8g) = 1.33 W/kg; SAR (10g) = 1.20 W/kg

Smallest distance from peaks to all points 3 dB below = 9.0 mm

Ratio of SAR at M2 to SAR at M1 = 80.1 %

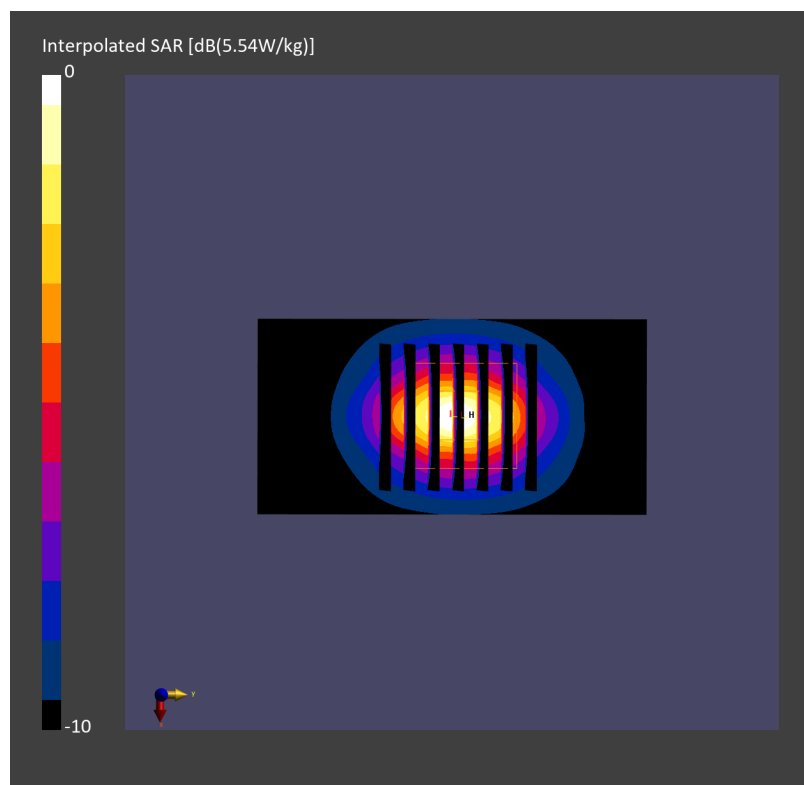

Date: 2025-02-08

System Check_Head_2600MHz**DUT: D2600V2 - SN1089**

Communication System: CW; Frequency: 2600.000 MHz

Medium: HSL_2600_250208 Medium parameters used: $f = 2600.000$ MHz; $\sigma = 2.00$ S/m; $\epsilon_r = 39.5$

Ambient Temperature: 23.3°C; Liquid Temperature: 22.3°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7625; ConvF(6.85, 6.68, 7.24); Calibrated: 2024-12-13
- Sensor-Surface: 1.4 mm
- Electronics: DAE4ip Sn1800; Calibrated: 2024-06-18
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2144
- Measurement Software: 16.2.4.2524
- UID: CW

Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 2.76 W/kg; SAR (10g) = 1.22 W/kg;


Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.5 mm

Power Drift = 0.01 dB

SAR (1g) = 2.71 W/kg; SAR (8g) = 1.35 W/kg; SAR (10g) = 1.21 W/kg

Smallest distance from peaks to all points 3 dB below = 9.0 mm

Ratio of SAR at M2 to SAR at M1 = 79.6 %

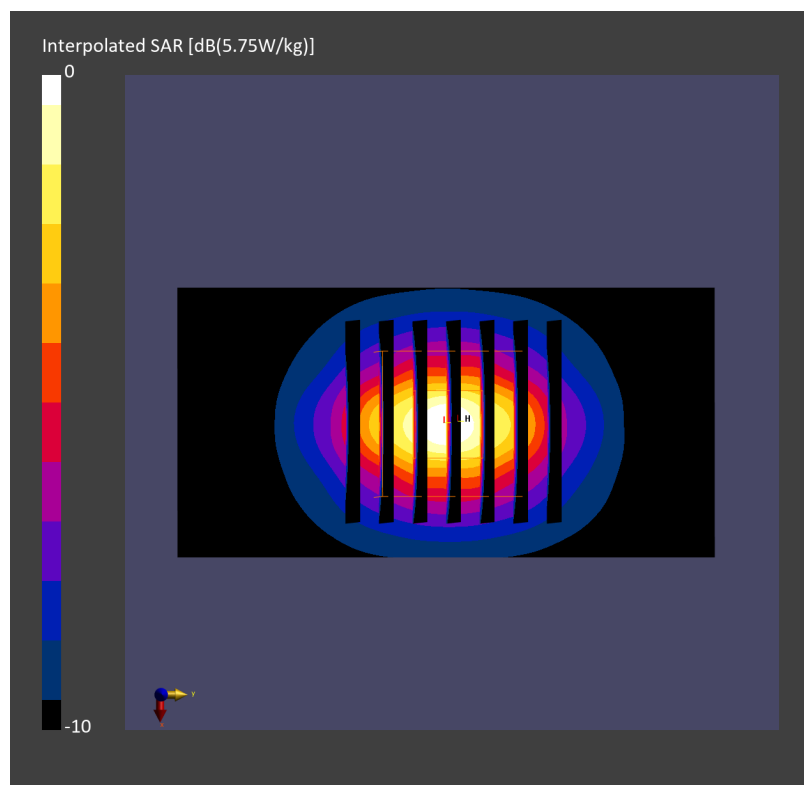

Date: 2025-02-14

System Check_Head_2600MHz**DUT: D2600V2 - SN1008**

Communication System: CW; Frequency: 2600.000 MHz

Medium: HSL_2600_250214 Medium parameters used: $f = 2600.000$ MHz; $\sigma = 1.96$ S/m; $\epsilon_r = 39.2$

Ambient Temperature: 23.5°C; Liquid Temperature: 22.5°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7694; ConvF(7.12, 6.95, 7.76); Calibrated: 2024-11-18
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1697; Calibrated: 2024-11-14
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2127; Section: Flat
- Measurement Software: 16.2.4.2524
- UID: CW, 0--

Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 2.56 W/kg; SAR (10g) = 1.14 W/kg;


Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.5 mm

Power Drift = 0.01 dB

SAR (1g) = 2.61 W/kg; SAR (8g) = 1.31 W/kg; SAR (10g) = 1.18 W/kg

Smallest distance from peaks to all points 3 dB below = 9.0 mm

Ratio of SAR at M2 to SAR at M1 = 79.1 %

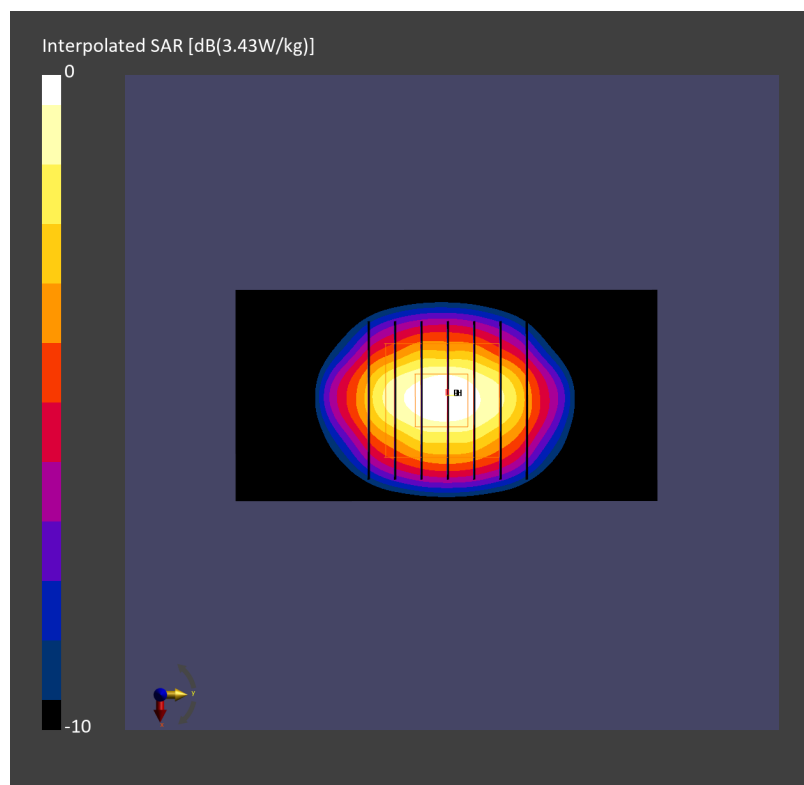

Date: 2025-02-16

System Check_Head_2600MHz**DUT: D2600V2 - SN1008**

Communication System: CW; Frequency: 2600.000 MHz

Medium: HSL_2600_250216 Medium parameters used: $f = 2600.000$ MHz; $\sigma = 1.98$ S/m; $\epsilon_r = 38.6$

Ambient Temperature: 23.4°C; Liquid Temperature: 22.4°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7625; ConvF(6.85, 6.68, 7.24); Calibrated: 2024-12-13
- Sensor-Surface: 1.4 mm
- Electronics: DAE4ip Sn1800; Calibrated: 2024-06-18
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2144
- Measurement Software: 16.2.4.2524
- UID: CW

Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 2.64 W/kg; SAR (10g) = 1.21 W/kg;


Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.5 mm

Power Drift = -0.01 dB

SAR (1g) = 2.71 W/kg; SAR (8g) = 1.35 W/kg; SAR (10g) = 1.22 W/kg

Smallest distance from peaks to all points 3 dB below = 9.0 mm

Ratio of SAR at M2 to SAR at M1 = 79.5 %

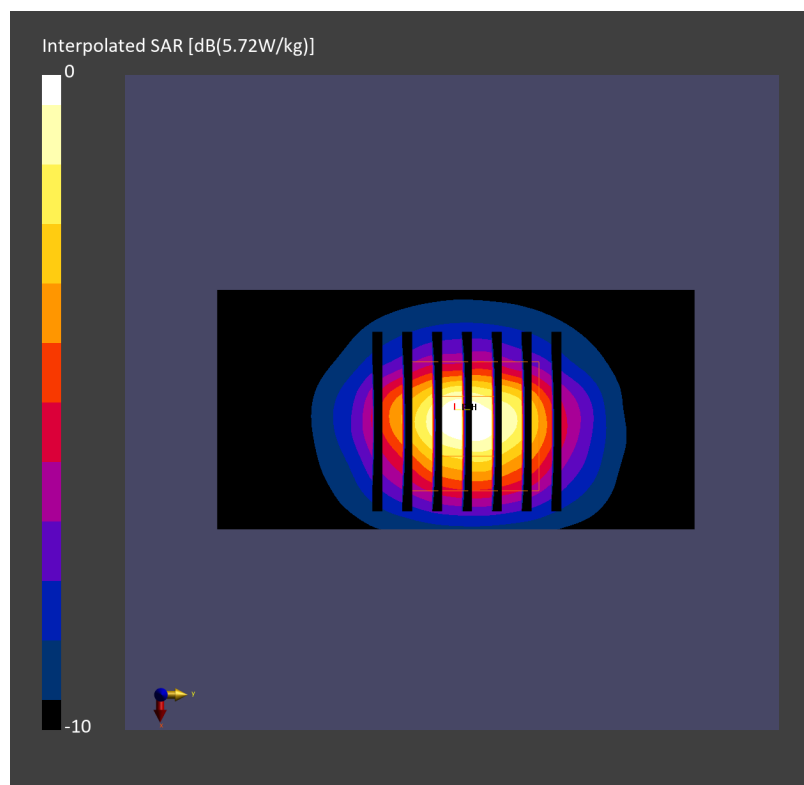

Date: 2025-02-23

System Check_Head_2600MHz**DUT: D2600V2 - SN1008**

Communication System: CW; Frequency: 2600.000 MHz

Medium: HSL_2600_250223 Medium parameters used: $f = 2600.000$ MHz; $\sigma = 1.97$ S/m; $\epsilon_r = 39.2$

Ambient Temperature: 23.4°C; Liquid Temperature: 22.4°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7625; ConvF(6.85, 6.68, 7.24); Calibrated: 2024-12-13
- Sensor-Surface: 1.4 mm
- Electronics: DAE4ip Sn1800; Calibrated: 2024-06-18
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2144
- Measurement Software: 16.2.4.2524
- UID: CW

Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 2.57 W/kg; SAR (10g) = 1.19 W/kg;


Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.5 mm

Power Drift = -0.00 dB

SAR (1g) = 2.67 W/kg; SAR (8g) = 1.33 W/kg; SAR (10g) = 1.20 W/kg

Smallest distance from peaks to all points 3 dB below = 9.0 mm

Ratio of SAR at M2 to SAR at M1 = 79.4 %

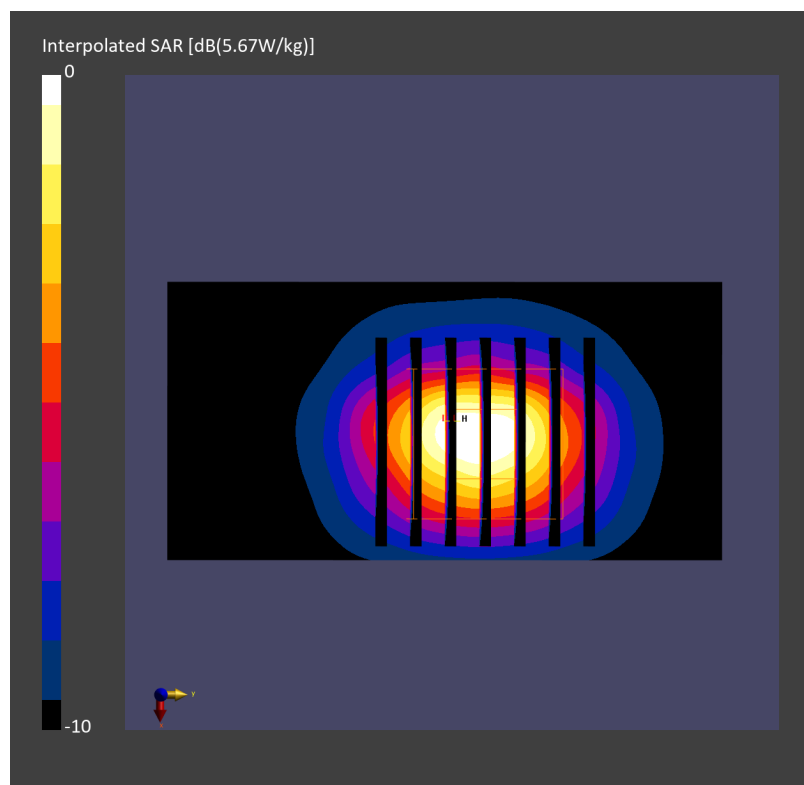

Date: 2025-02-24

System Check_Head_2600MHz**DUT: D2600V2 - SN1008**

Communication System: CW; Frequency: 2600.000 MHz

Medium: HSL_2600_250224 Medium parameters used: $f = 2600.000$ MHz; $\sigma = 1.95$ S/m; $\epsilon_r = 38.3$

Ambient Temperature: 23.6°C; Liquid Temperature: 22.6°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7625; ConvF(6.85, 6.68, 7.24); Calibrated: 2024-12-13
- Sensor-Surface: 1.4 mm
- Electronics: DAE4ip Sn1800; Calibrated: 2024-06-18
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2144
- Measurement Software: 16.2.4.2524
- UID: CW

Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 2.51 W/kg; SAR (10g) = 1.16 W/kg;


Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.5 mm

Power Drift = 0.01 dB

SAR (1g) = 2.60 W/kg; SAR (8g) = 1.30 W/kg; SAR (10g) = 1.17 W/kg

Smallest distance from peaks to all points 3 dB below = 9.1 mm

Ratio of SAR at M2 to SAR at M1 = 80.0 %

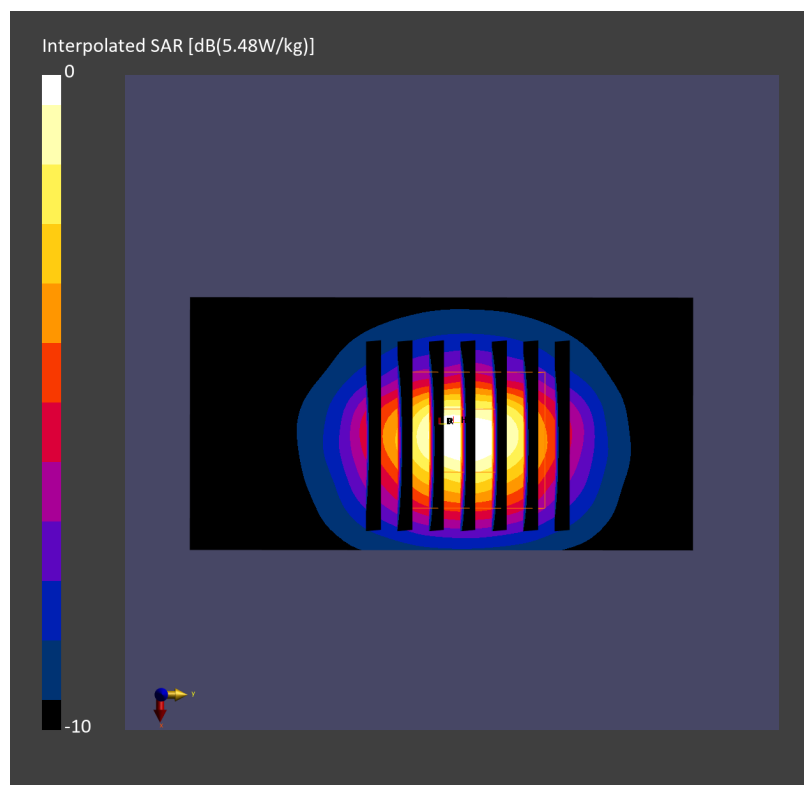

Date: 2025-01-26

System Check_Head_3500MHz**DUT: D3500V2 - SN1036**

Communication System: CW; Frequency: 3500.000 MHz

Medium: HSL_3500_250126 Medium parameters used: $f = 3500.000$ MHz; $\sigma = 2.92$ S/m; $\epsilon_r = 37.6$

Ambient Temperature: 23.5°C; Liquid Temperature: 22.5°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7694; ConvF(6.36, 6.21, 6.93); Calibrated: 2024-11-18
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1697; Calibrated: 2024-11-14
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2127; Section: Flat
- Measurement Software: 16.2.4.2524
- UID: CW, 0

Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 3.10 W/kg; SAR (10g) = 1.18 W/kg;


Pin=17.0dBm/Zoom Scan (28.0 mm x 28.0 mm x 28.0 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.4 mm

Power Drift = 0.02 dB

SAR (1g) = 3.14 W/kg; SAR (8g) = 1.37 W/kg; SAR (10g) = 1.21 W/kg

Smallest distance from peaks to all points 3 dB below = 8.0 mm

Ratio of SAR at M2 to SAR at M1 = 76.2 %

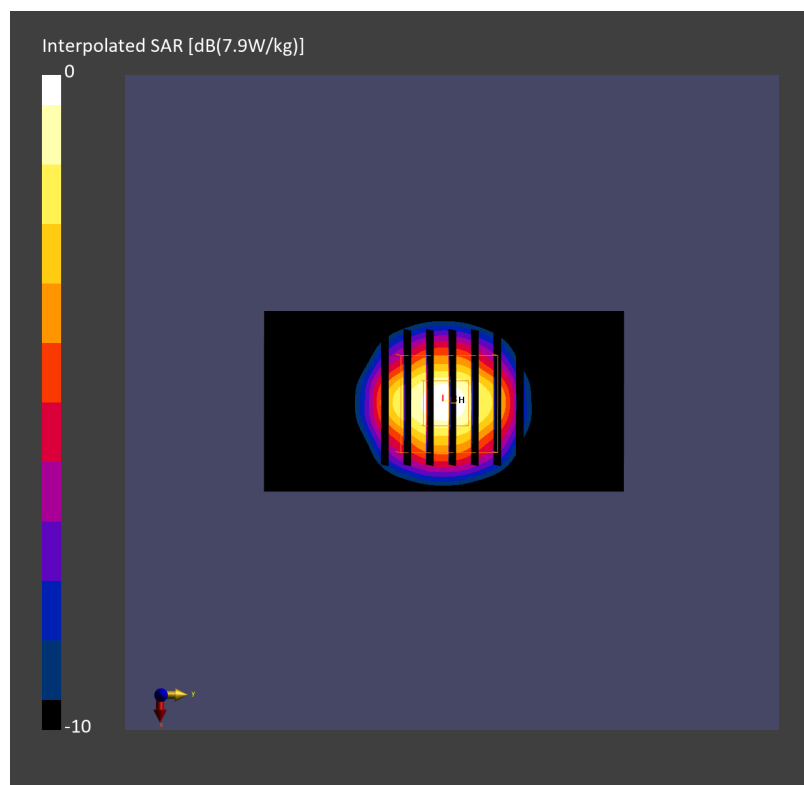

Date: 2025-01-27

System Check_Head_3500MHz**DUT: D3500V2 - SN1036**

Communication System: CW; Frequency: 3500.000 MHz

Medium: HSL_3500_250127 Medium parameters used: $f = 3500.000$ MHz; $\sigma = 2.95$ S/m; $\epsilon_r = 37.8$

Ambient Temperature: 23.5°C; Liquid Temperature: 22.5°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7694; ConvF(6.36, 6.21, 6.93); Calibrated: 2024-11-18
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1697; Calibrated: 2024-11-14
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2127
- Measurement Software: 16.2.4.2524
- UID: CW

Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 3.11 W/kg; SAR (10g) = 1.18 W/kg;


Pin=17.0dBm/Zoom Scan (28.0 mm x 28.0 mm x 28.0 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.4 mm

Power Drift = 0.01 dB

SAR (1g) = 3.15 W/kg; SAR (8g) = 1.37 W/kg; SAR (10g) = 1.21 W/kg

Smallest distance from peaks to all points 3 dB below = 8.0 mm

Ratio of SAR at M2 to SAR at M1 = 76.0 %

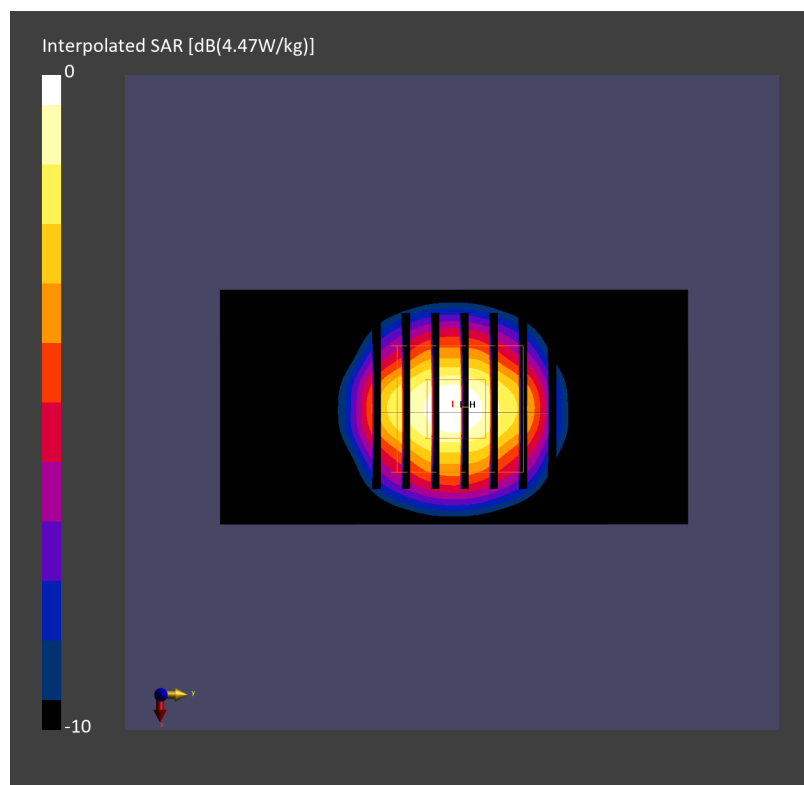

Date: 2025-01-27

System Check_Head_3500MHz**DUT: D3500V2 - SN1036**

Communication System: CW; Frequency: 3500.000 MHz

Medium: HSL_3500_250127 Medium parameters used: $f = 3500.000$ MHz; $\sigma = 2.99$ S/m; $\epsilon_r = 37.8$

Ambient Temperature: 23.3°C; Liquid Temperature: 22.3°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7625; ConvF(6.51, 6.36, 6.88); Calibrated: 2024-12-13
- Sensor-Surface: 1.4 mm
- Electronics: DAE4ip Sn1800; Calibrated: 2024-06-18
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2144
- Measurement Software: 16.2.4.2524
- UID: CW

Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 3.12 W/kg; SAR (10g) = 1.18 W/kg;


Pin=17.0dBm/Zoom Scan (28.0 mm x 28.0 mm x 28.0 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.4 mm

Power Drift = 0.00 dB

SAR (1g) = 3.24 W/kg; SAR (8g) = 1.39 W/kg; SAR (10g) = 1.23 W/kg

Smallest distance from peaks to all points 3 dB below = 8.3 mm

Ratio of SAR at M2 to SAR at M1 = 75.7 %

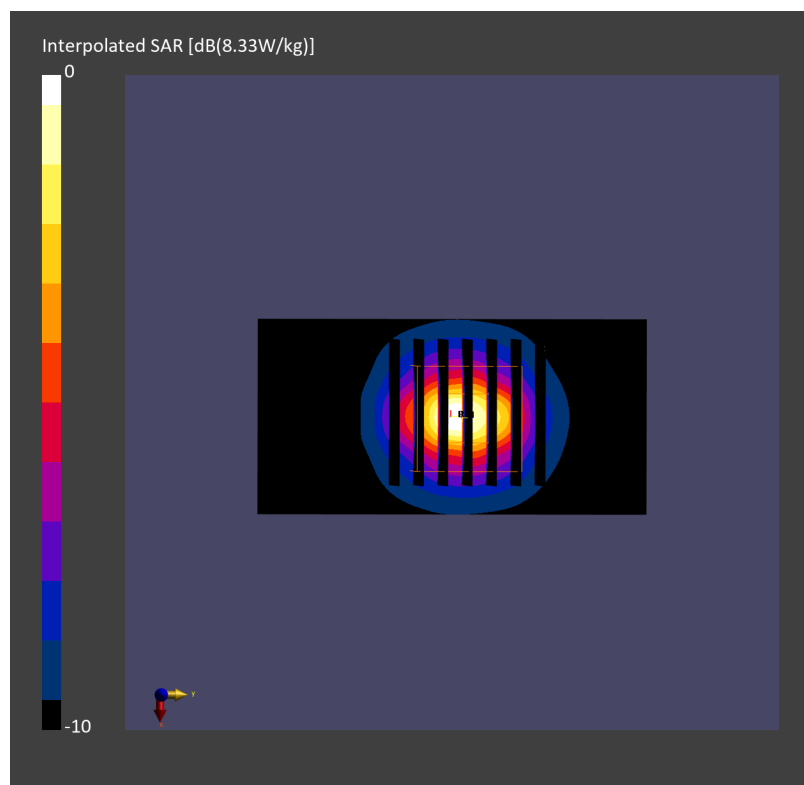

Date: 2025-02-05

System Check_Head_3500MHz**DUT: D3500V2 - SN1036**

Communication System: CW; Frequency: 3500.000 MHz

Medium: HSL_3500_250205 Medium parameters used: $f = 3500.000$ MHz; $\sigma = 2.99$ S/m; $\epsilon_r = 38.2$

Ambient Temperature: 23.6°C; Liquid Temperature: 22.6°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7625; ConvF(6.51, 6.36, 6.88); Calibrated: 2024-12-13
- Sensor-Surface: 1.4 mm
- Electronics: DAE4ip Sn1800; Calibrated: 2024-06-18
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2144
- Measurement Software: 16.2.4.2524
- UID: CW

Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 3.35 W/kg; SAR (10g) = 1.30 W/kg;


Pin=17.0dBm/Zoom Scan (28.0 mm x 28.0 mm x 28.0 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.4 mm

Power Drift = 0.01 dB

SAR (1g) = 3.46 W/kg; SAR (8g) = 1.49 W/kg; SAR (10g) = 1.32 W/kg

Smallest distance from peaks to all points 3 dB below = 8.3 mm

Ratio of SAR at M2 to SAR at M1 = 76.0 %

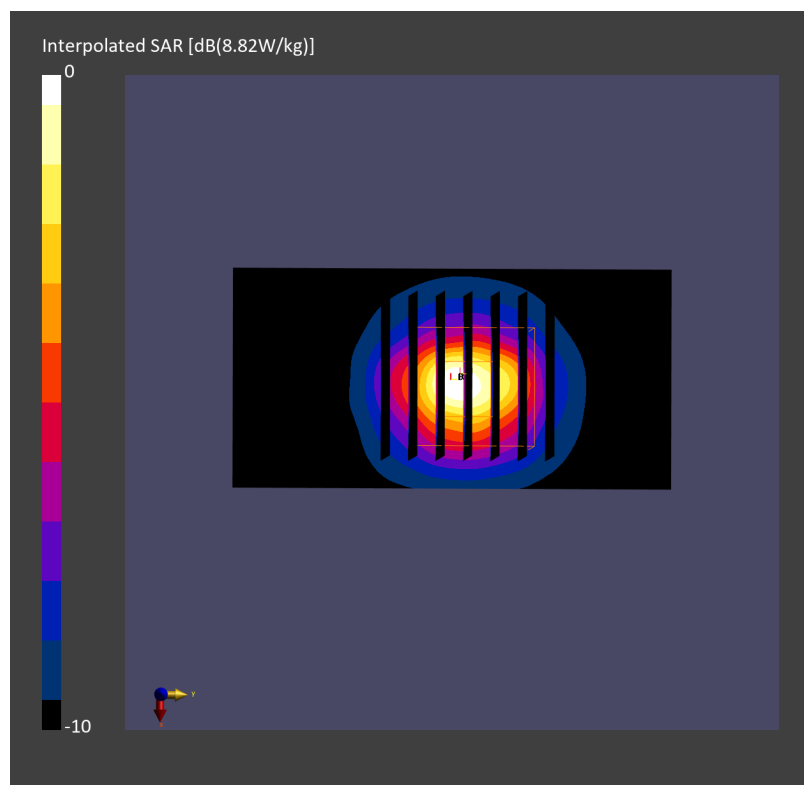

Date: 2025-02-09

System Check_Head_3500MHz**DUT: D3500V2 - SN1036**

Communication System: CW; Frequency: 3500.000 MHz

Medium: HSL_3500_250209 Medium parameters used: $f = 3500.000$ MHz; $\sigma = 2.91$ S/m; $\epsilon_r = 37.3$

Ambient Temperature: 23.3°C; Liquid Temperature: 22.3°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7625; ConvF(6.51, 6.36, 6.88); Calibrated: 2024-12-13
- Sensor-Surface: 1.4 mm
- Electronics: DAE4ip Sn1800; Calibrated: 2024-06-18
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2144
- Measurement Software: 16.2.4.2524
- UID: CW

Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 3.20 W/kg; SAR (10g) = 1.23 W/kg;


Pin=17.0dBm/Zoom Scan (28.0 mm x 28.0 mm x 28.0 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.4 mm

Power Drift = -0.13 dB

SAR (1g) = 3.30 W/kg; SAR (8g) = 1.42 W/kg; SAR (10g) = 1.25 W/kg

Smallest distance from peaks to all points 3 dB below = 8.0 mm

Ratio of SAR at M2 to SAR at M1 = 75.3 %

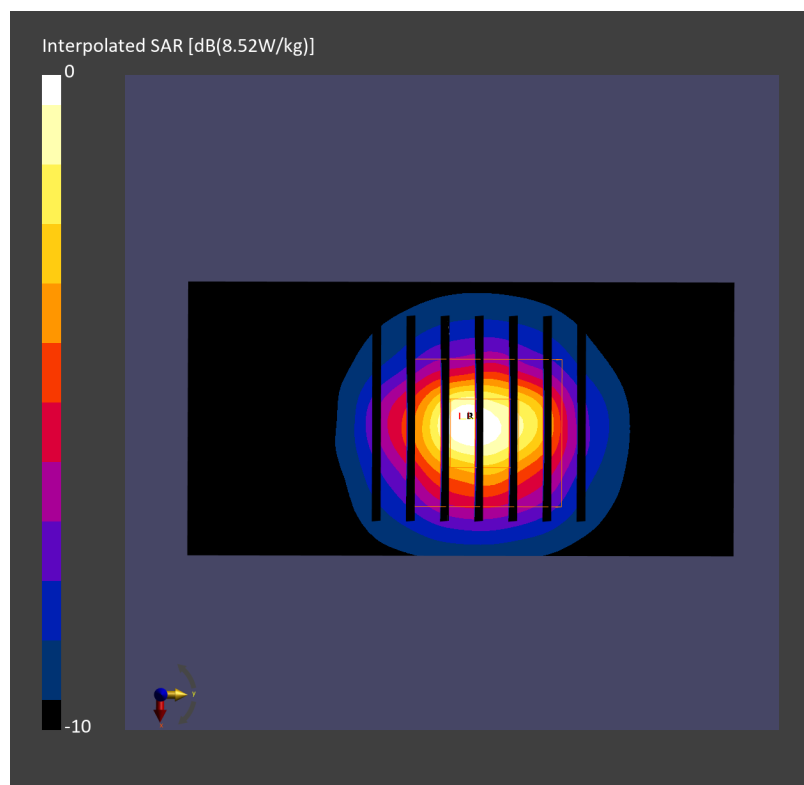

Date: 2025-02-10

System Check_Head_3500MHz**DUT: D3500V2 - SN1036**

Communication System: CW; Frequency: 3500.000 MHz

Medium: HSL_3500_250210 Medium parameters used: $f = 3500.000$ MHz; $\sigma = 2.95$ S/m; $\epsilon_r = 38.3$

Ambient Temperature: 23.5°C; Liquid Temperature: 22.5°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7694; ConvF(6.36, 6.21, 6.93); Calibrated: 2024-11-18
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1697; Calibrated: 2024-11-14
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2127; Section: Flat
- Measurement Software: 16.2.4.2524
- UID: CW, 0--

Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 3.10 W/kg; SAR (10g) = 1.18 W/kg;


Pin=17.0dBm/Zoom Scan (28.0 mm x 28.0 mm x 28.0 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.4 mm

Power Drift = -0.01 dB

SAR (1g) = 3.13 W/kg; SAR (8g) = 1.36 W/kg; SAR (10g) = 1.20 W/kg

Smallest distance from peaks to all points 3 dB below = 8.6 mm

Ratio of SAR at M2 to SAR at M1 = 76.5 %

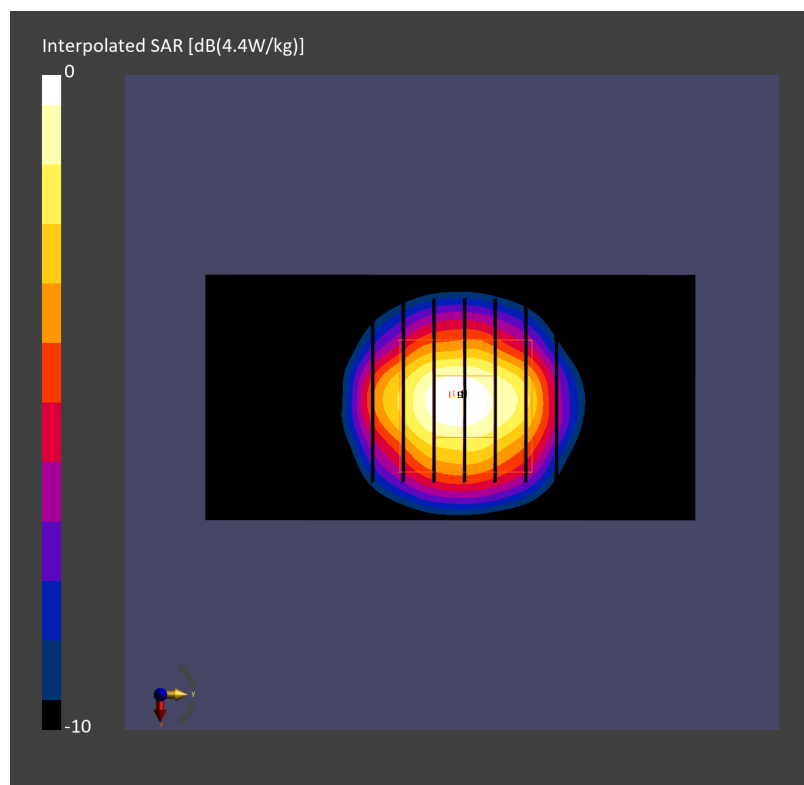

Date: 2025-02-19

System Check_Head_3500MHz**DUT: D3500V2 - SN1036**

Communication System: CW; Frequency: 3500.000 MHz

Medium: HSL_3500_250219 Medium parameters used: $f = 3500.000$ MHz; $\sigma = 3.01$ S/m; $\epsilon_r = 37.9$

Ambient Temperature: 23.7°C; Liquid Temperature: 22.7°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7625; ConvF(6.51, 6.36, 6.88); Calibrated: 2024-12-13
- Sensor-Surface: 1.4 mm
- Electronics: DAE4ip Sn1800; Calibrated: 2024-06-18
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2144
- Measurement Software: 16.2.4.2524
- UID: CW

Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 3.35 W/kg; SAR (10g) = 1.28 W/kg;


Pin=17.0dBm/Zoom Scan (28.0 mm x 28.0 mm x 28.0 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.4 mm

Power Drift = -0.01 dB

SAR (1g) = 3.43 W/kg; SAR (8g) = 1.48 W/kg; SAR (10g) = 1.31 W/kg

Smallest distance from peaks to all points 3 dB below = 8.0 mm

Ratio of SAR at M2 to SAR at M1 = 75.8 %

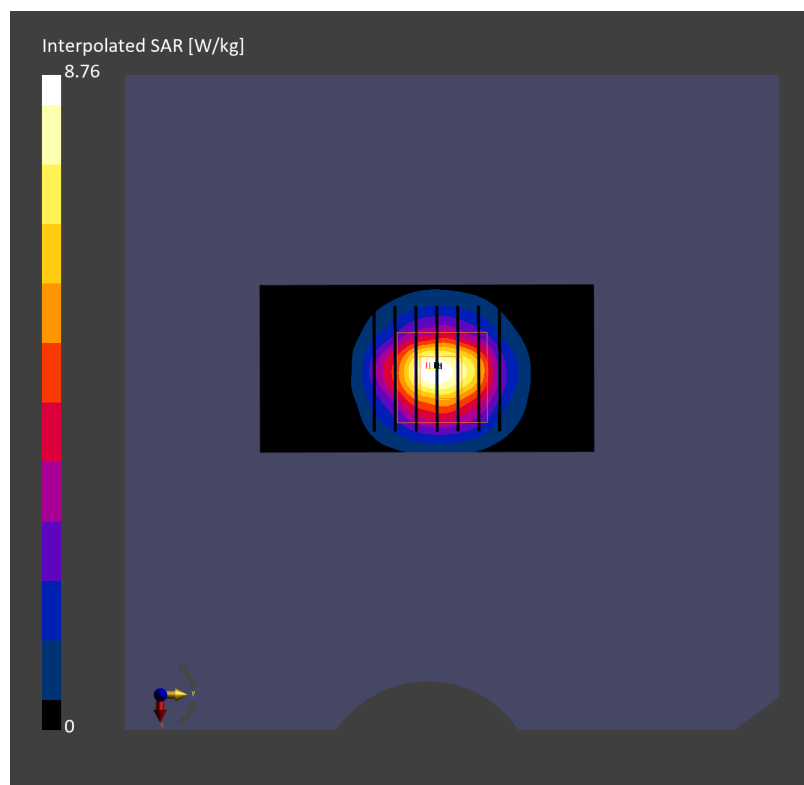

Date: 2025-02-20

System Check_Head_3500MHz**DUT: D3500V2 - SN1036**

Communication System: CW; Frequency: 3500.000 MHz

Medium: HSL_3500_250220 Medium parameters used: $f = 3500.000$ MHz; $\sigma = 2.97$ S/m; $\epsilon_r = 38.4$

Ambient Temperature: 23.5°C; Liquid Temperature: 22.5°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7625; ConvF(6.51, 6.36, 6.88); Calibrated: 2024-12-13
- Sensor-Surface: 1.4 mm
- Electronics: DAE4ip Sn1800; Calibrated: 2024-06-18
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2144
- Measurement Software: 16.2.4.2524
- UID: CW

Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 3.47 W/kg; SAR (10g) = 1.31 W/kg;


Pin=17.0dBm/Zoom Scan (28.0 mm x 28.0 mm x 28.0 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.4 mm

Power Drift = -0.05 dB

SAR (1g) = 3.38 W/kg; SAR (8g) = 1.46 W/kg; SAR (10g) = 1.29 W/kg

Smallest distance from peaks to all points 3 dB below = 8.0 mm

Ratio of SAR at M2 to SAR at M1 = 75.8 %

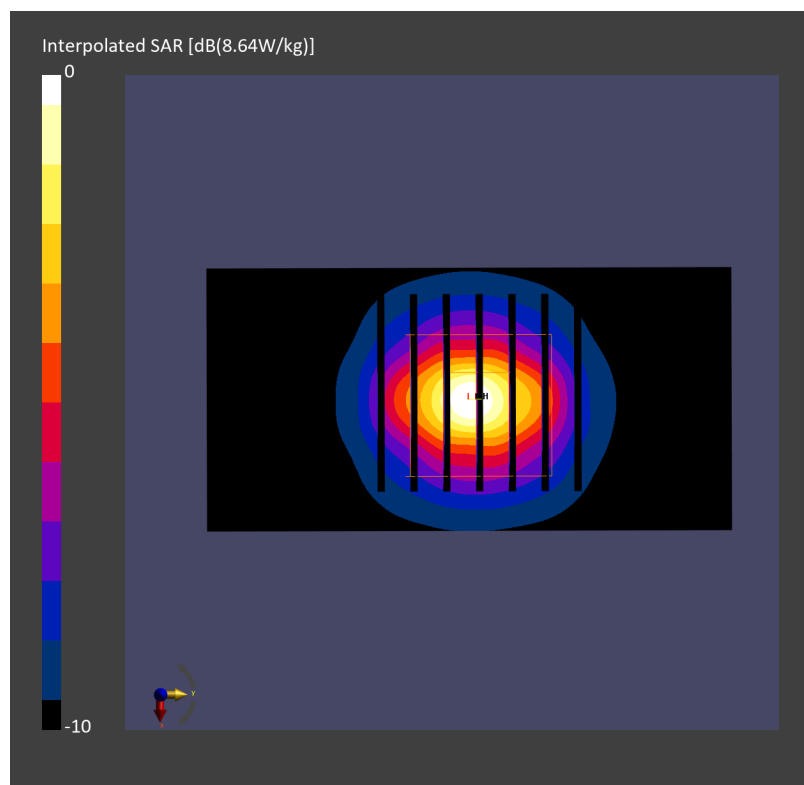

Date: 2025-02-21

System Check_Head_3500MHz**DUT: D3500V2 - SN1036**

Communication System: CW; Frequency: 3500.000 MHz

Medium: HSL_3500_250221 Medium parameters used: $f = 3500.000$ MHz; $\sigma = 2.94$ S/m; $\epsilon_r = 37.5$

Ambient Temperature: 23.6°C; Liquid Temperature: 22.6°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7625; ConvF(6.51, 6.36, 6.88); Calibrated: 2024-12-13
- Sensor-Surface: 1.4 mm
- Electronics: DAE4ip Sn1800; Calibrated: 2024-06-18
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2144
- Measurement Software: 16.2.4.2524
- UID: CW

Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 3.34 W/kg; SAR (10g) = 1.27 W/kg;


Pin=17.0dBm/Zoom Scan (28.0 mm x 28.0 mm x 28.0 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.4 mm

Power Drift = -0.01 dB

SAR (1g) = 3.37 W/kg; SAR (8g) = 1.45 W/kg; SAR (10g) = 1.28 W/kg

Smallest distance from peaks to all points 3 dB below = 8.0 mm

Ratio of SAR at M2 to SAR at M1 = 75.5 %

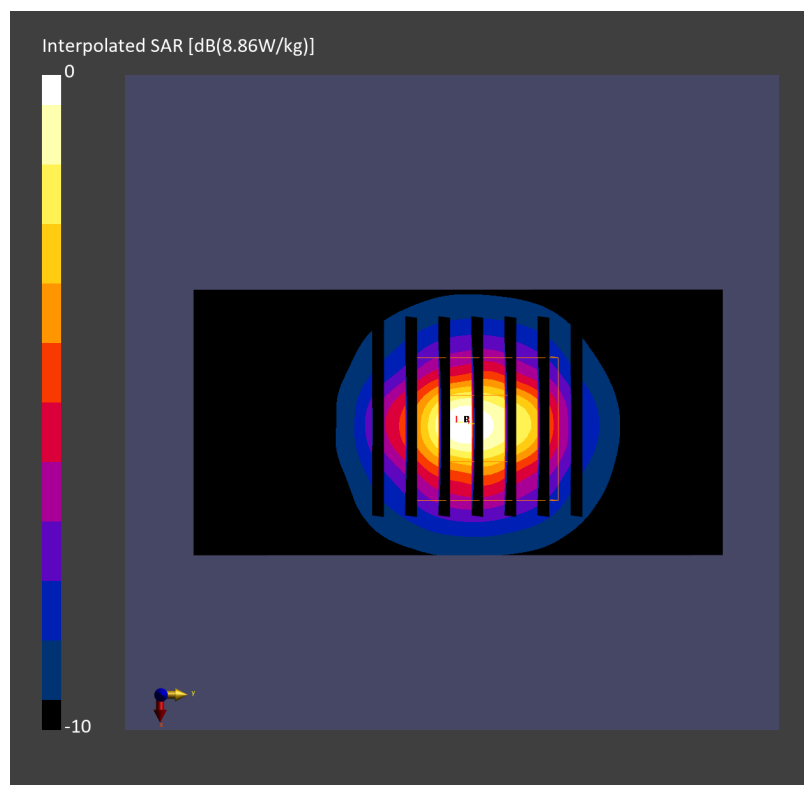

Date: 2025-02-22

System Check_Head_3500MHz**DUT: D3500V2 - SN1036**

Communication System: CW; Frequency: 3500.000 MHz

Medium: HSL_3500_250222 Medium parameters used: $f = 3500.000$ MHz; $\sigma = 2.87$ S/m; $\epsilon_r = 37.1$

Ambient Temperature: 23.7°C; Liquid Temperature: 22.7°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7625; ConvF(6.51, 6.36, 6.88); Calibrated: 2024-12-13
- Sensor-Surface: 1.4 mm
- Electronics: DAE4ip Sn1800; Calibrated: 2024-06-18
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2144; Section: Flat
- Measurement Software: 16.2.4.2524
- UID: CW, 0--

Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 3.02 W/kg; SAR (10g) = 1.19 W/kg;


Pin=17.0dBm/Zoom Scan (28.0 mm x 28.0 mm x 28.0 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.4 mm

Power Drift = 0.02 dB

SAR (1g) = 3.17 W/kg; SAR (8g) = 1.37 W/kg; SAR (10g) = 1.21 W/kg

Smallest distance from peaks to all points 3 dB below = 8.3 mm

Ratio of SAR at M2 to SAR at M1 = 75.9 %

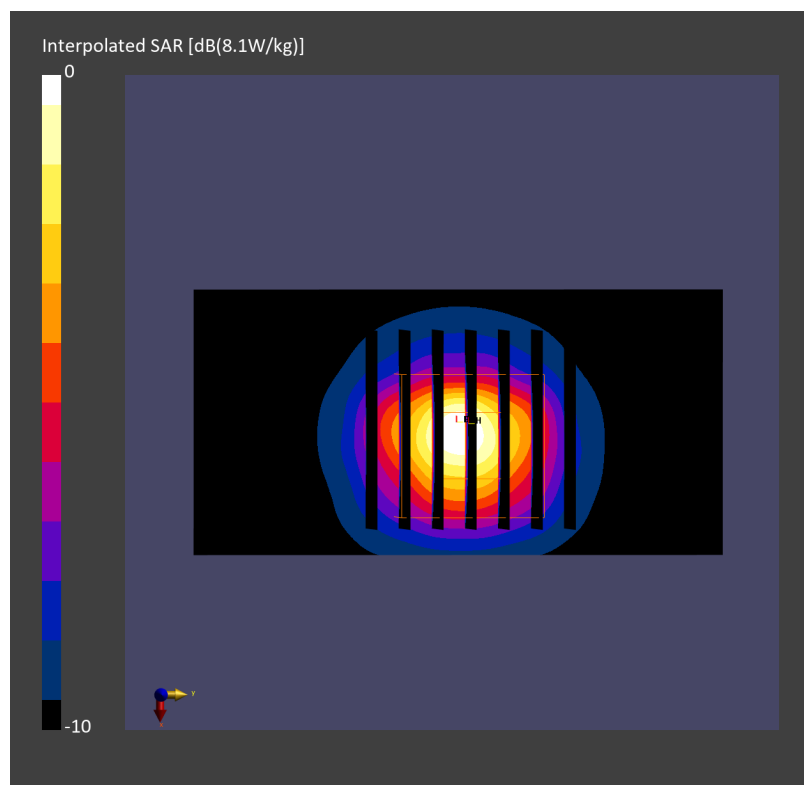

Date: 2025-02-24

System Check_Head_3500MHz**DUT: D3500V2 - SN1014**

Communication System: CW; Frequency: 3500.000 MHz

Medium: HSL_3500_250224 Medium parameters used: $f = 3500.000$ MHz; $\sigma = 2.96$ S/m; $\epsilon_r = 37.7$

Ambient Temperature: 23.6°C; Liquid Temperature: 22.6°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7625; ConvF(6.51, 6.36, 6.88); Calibrated: 2024-12-13
- Sensor-Surface: 1.4 mm
- Electronics: DAE4ip Sn1800; Calibrated: 2024-06-18
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2144
- Measurement Software: 16.2.4.2524
- UID: CW

Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 3.06 W/kg; SAR (10g) = 1.24 W/kg;


Pin=17.0dBm/Zoom Scan (28.0 mm x 28.0 mm x 28.0 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.4 mm

Power Drift = -0.00 dB

SAR (1g) = 3.29 W/kg; SAR (8g) = 1.41 W/kg; SAR (10g) = 1.25 W/kg

Smallest distance from peaks to all points 3 dB below = 8.3 mm

Ratio of SAR at M2 to SAR at M1 = 76.1 %

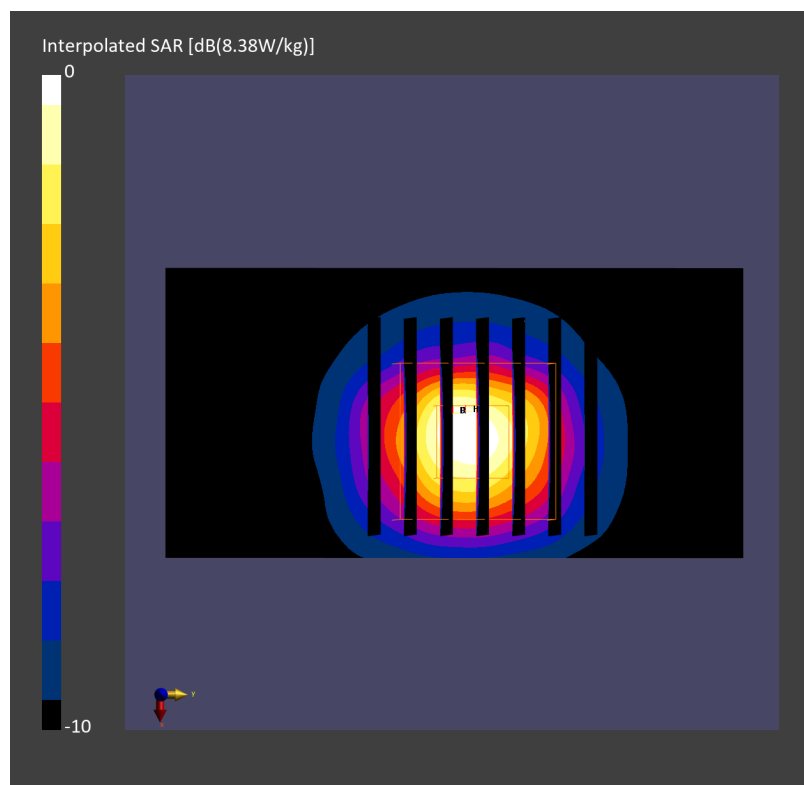

Date: 2025-02-25

System Check_Head_3500MHz**DUT: D3500V2 - SN1014**

Communication System: CW; Frequency: 3500.000 MHz

Medium: HSL_3500_250225 Medium parameters used: $f = 3500.000$ MHz; $\sigma = 2.91$ S/m; $\epsilon_r = 37.4$

Ambient Temperature: 23.5°C; Liquid Temperature: 22.5°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7625; ConvF(6.51, 6.36, 6.88); Calibrated: 2024-12-13
- Sensor-Surface: 1.4 mm
- Electronics: DAE4ip Sn1800; Calibrated: 2024-06-18
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2144
- Measurement Software: 16.2.4.2524
- UID: CW

Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 3.01 W/kg; SAR (10g) = 1.22 W/kg;


Pin=17.0dBm/Zoom Scan (28.0 mm x 28.0 mm x 28.0 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.4 mm

Power Drift = 0.01 dB

SAR (1g) = 3.24 W/kg; SAR (8g) = 1.39 W/kg; SAR (10g) = 1.23 W/kg

Smallest distance from peaks to all points 3 dB below = 8.1 mm

Ratio of SAR at M2 to SAR at M1 = 75.9 %

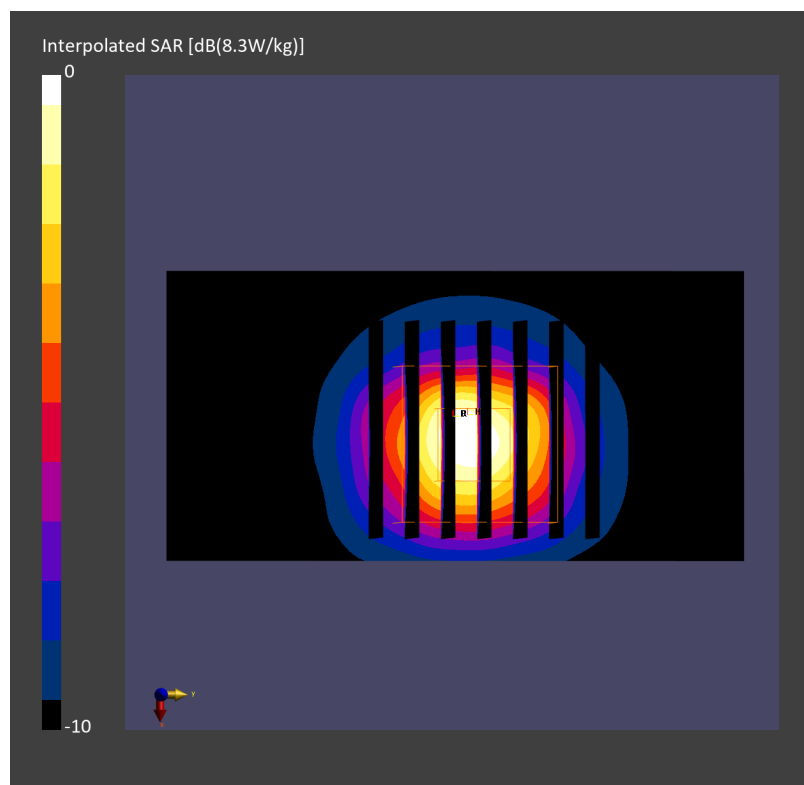

Date: 2025-03-12

System Check_Head_3500MHz**DUT: D3500V2 - SN1014**

Communication System: CW; Frequency: 3500.000 MHz

Medium: HSL_3500_250312 Medium parameters used: $f = 3500.000$ MHz; $\sigma = 2.90$ S/m; $\epsilon_r = 38.0$

Ambient Temperature: 23.5°C; Liquid Temperature: 22.5°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7694; ConvF(6.36, 6.21, 6.93); Calibrated: 2024-11-18
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1697; Calibrated: 2024-11-14
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2127; Section: Flat
- Measurement Software: 16.2.4.2524
- UID: CW, 0--

Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 3.08 W/kg; SAR (10g) = 1.18 W/kg;


Pin=17.0dBm/Zoom Scan (28.0 mm x 28.0 mm x 28.0 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.4 mm

Power Drift = -0.03 dB

SAR (1g) = 3.14 W/kg; SAR (8g) = 1.39 W/kg; SAR (10g) = 1.23 W/kg

Smallest distance from peaks to all points 3 dB below = 8.6 mm

Ratio of SAR at M2 to SAR at M1 = 76.9 %

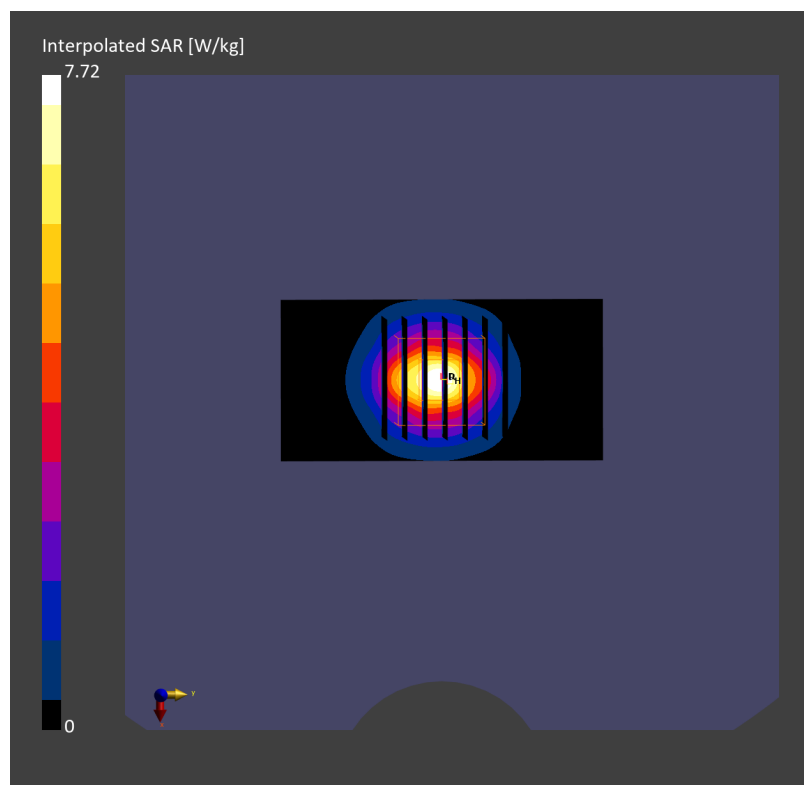

Date: 2025-03-13

System Check_Head_3500MHz**DUT: D3500V2 - SN1014**

Communication System: CW; Frequency: 3500.000 MHz

Medium: HSL_3500_250313 Medium parameters used: $f = 3500.000$ MHz; $\sigma = 2.94$ S/m; $\epsilon_r = 38.3$

Ambient Temperature: 23.3°C; Liquid Temperature: 22.3°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7694; ConvF(6.36, 6.21, 6.93); Calibrated: 2024-11-18
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1697; Calibrated: 2024-11-14
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2127; Section: Flat
- Measurement Software: 16.2.4.2524
- UID: CW, 0

Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 3.06 W/kg; SAR (10g) = 1.17 W/kg;


Pin=17.0dBm/Zoom Scan (28.0 mm x 28.0 mm x 28.0 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.4 mm

Power Drift = -0.01 dB

SAR (1g) = 3.13 W/kg; SAR (8g) = 1.38 W/kg; SAR (10g) = 1.23 W/kg

Smallest distance from peaks to all points 3 dB below = 8.0 mm

Ratio of SAR at M2 to SAR at M1 = 76.9 %

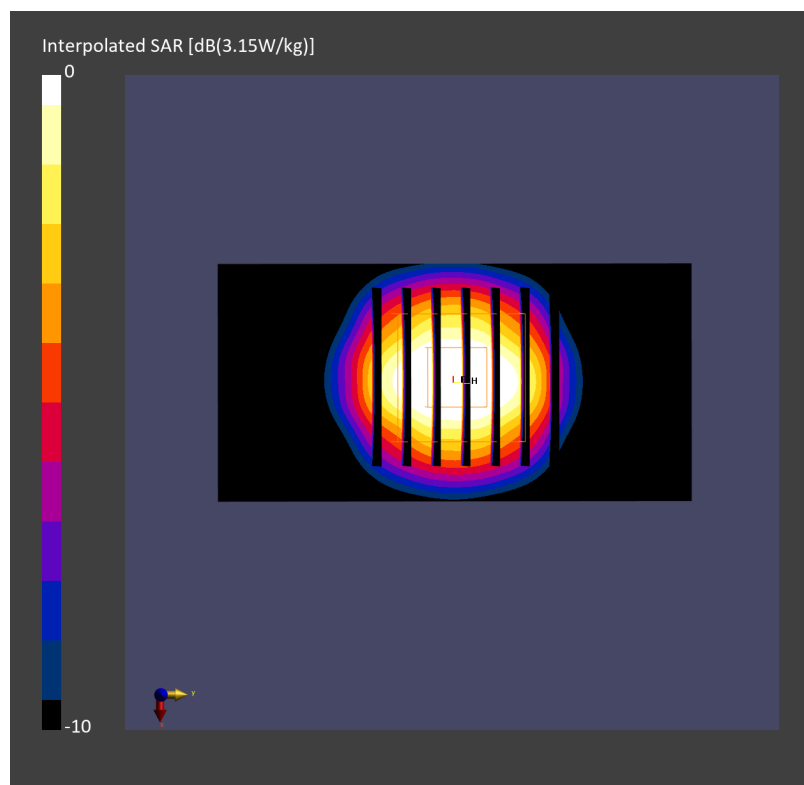

Date: 2025-03-16

System Check_Head_3500MHz**DUT: D3500V2 - SN1014**

Communication System: CW; Frequency: 3500.000 MHz

Medium: HSL_3500_250316 Medium parameters used: $f = 3500.000$ MHz; $\sigma = 3.01$ S/m; $\epsilon_r = 37.8$

Ambient Temperature: 23.5°C; Liquid Temperature: 22.5°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7785; ConvF(5.42, 5.71, 5.59); Calibrated: 2024-11-28
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1694; Calibrated: 2024-11-19
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2126; Section: Flat
- Measurement Software: 16.2.4.2524
- UID: CW, 0--

Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 3.38 W/kg; SAR (10g) = 1.28 W/kg;

Pin=17.0dBm/Zoom Scan (28.0 mm x 28.0 mm x 28.0 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.4 mm

Power Drift = 0.03 dB

SAR (1g) = 3.45 W/kg; SAR (8g) = 1.53 W/kg; SAR (10g) = 1.36 W/kg

Smallest distance from peaks to all points 3 dB below = 8.1 mm

Ratio of SAR at M2 to SAR at M1 = 77.3 %

