

# PCTEST Engineering Lab.

## SPECTRUM ANALYZER PRESENTATION

FCC ID:ACJ96NKX-TD7680

PANASONIC


FCC 15.247

POWER OUT C-91

Operating Frequency: 2479.680 MHz

Output Power : -20.0 dBm

Test Mode:Other Transmitter

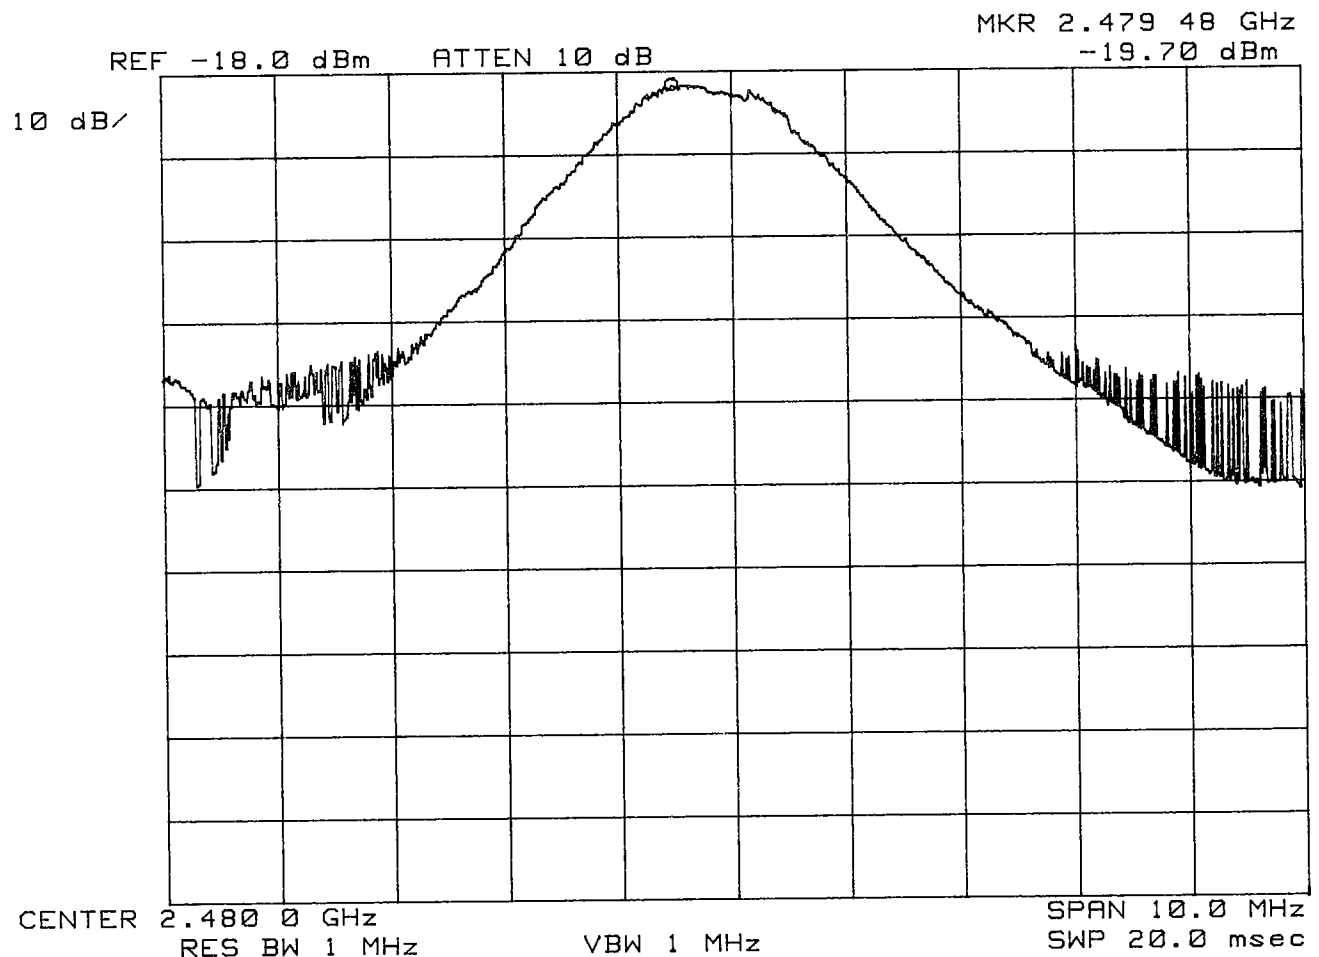



# PCTEST Engineering Lab.

## SPECTRUM ANALYZER PRESENTATION

FCC ID:ACJ96NKX-TD7680

PANASONIC HANDSET


FCC 15.247

POWER OUT C-01

Operating Frequency: 2401.056 MHz

Output Power : -20.0 dBm

Test Mode:Other Transmitter

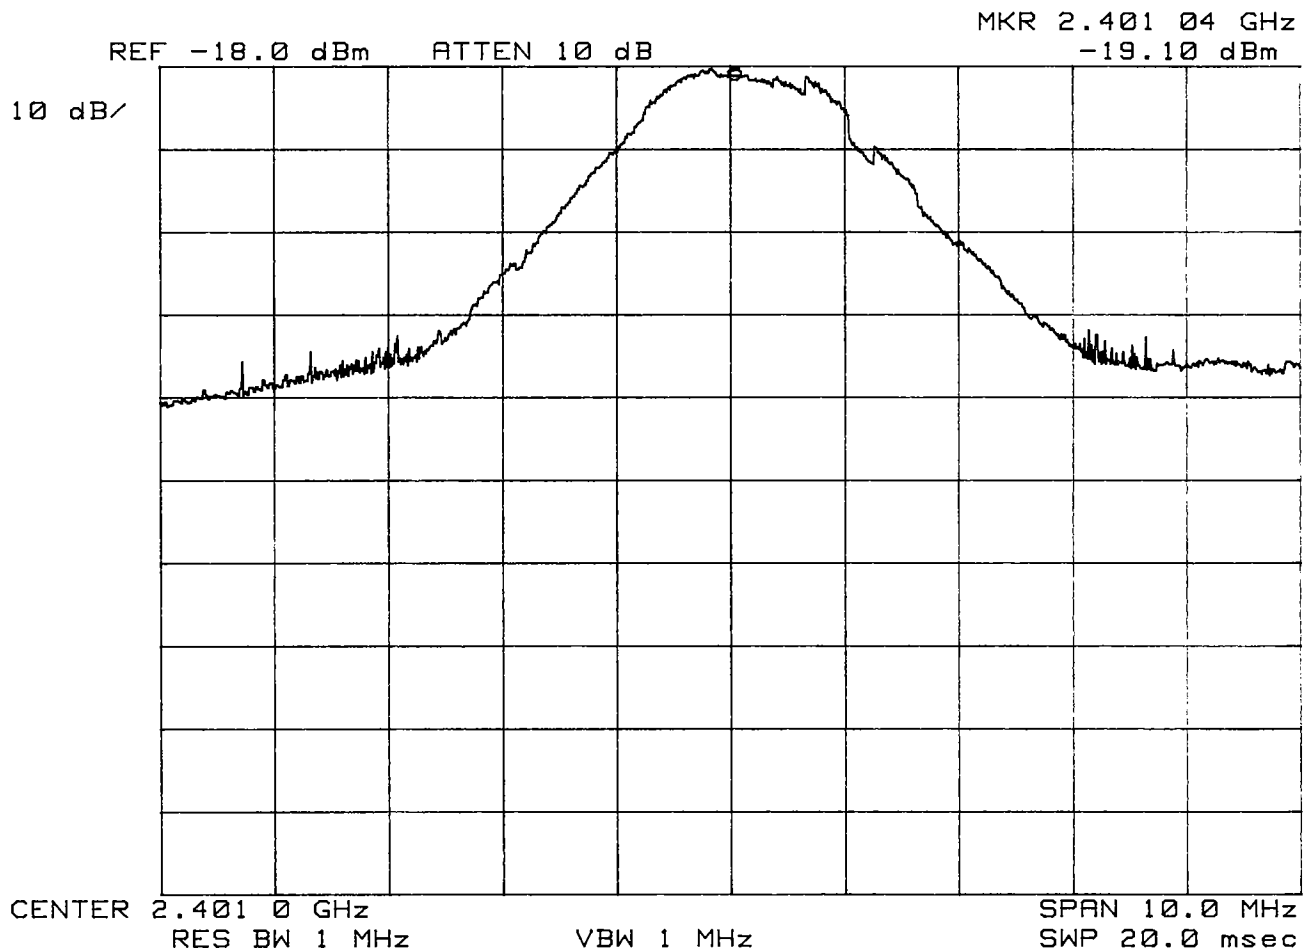

# PCTEST Engineering Lab.

## SPECTRUM ANALYZER PRESENTATION

FCC ID:ACJ96NKX-TD7680

PANASONIC


FCC 15.247

BAND EDGE C-1

Operating Frequency: 2401.056 MHz

Output Power : -20.0 dBm

Test Mode:Other Transmitter

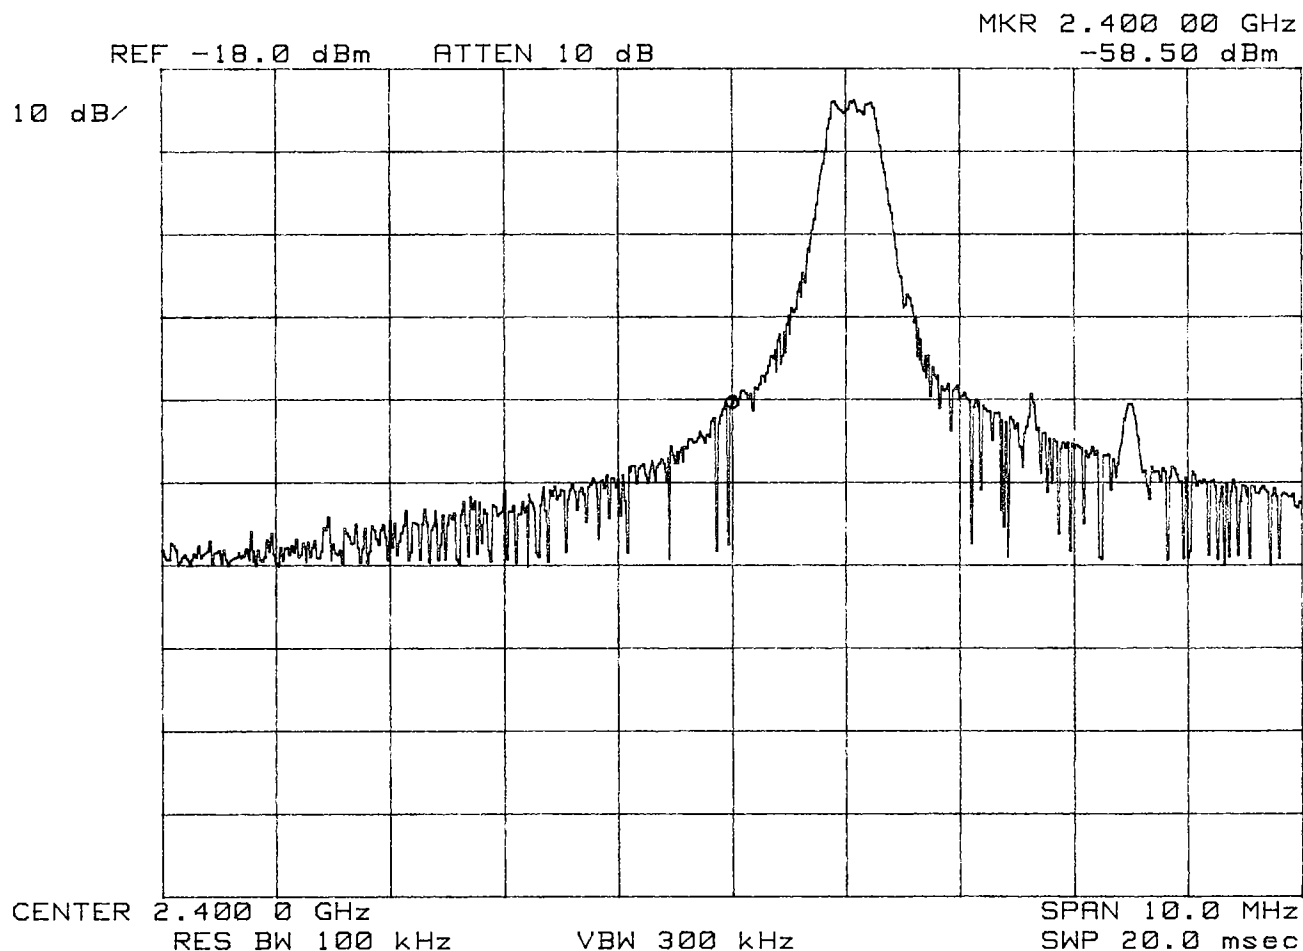

# PCTEST Engineering Lab.

## SPECTRUM ANALYZER PRESENTATION

FCC ID:ACJ96NKX-TD7680

PANASONIC


FCC 15.247

BAND EDGE C-91


Operating Frequency: 2479.680 MHz

Output Power : -20.0 dBm

Test Mode:Other Transmitter

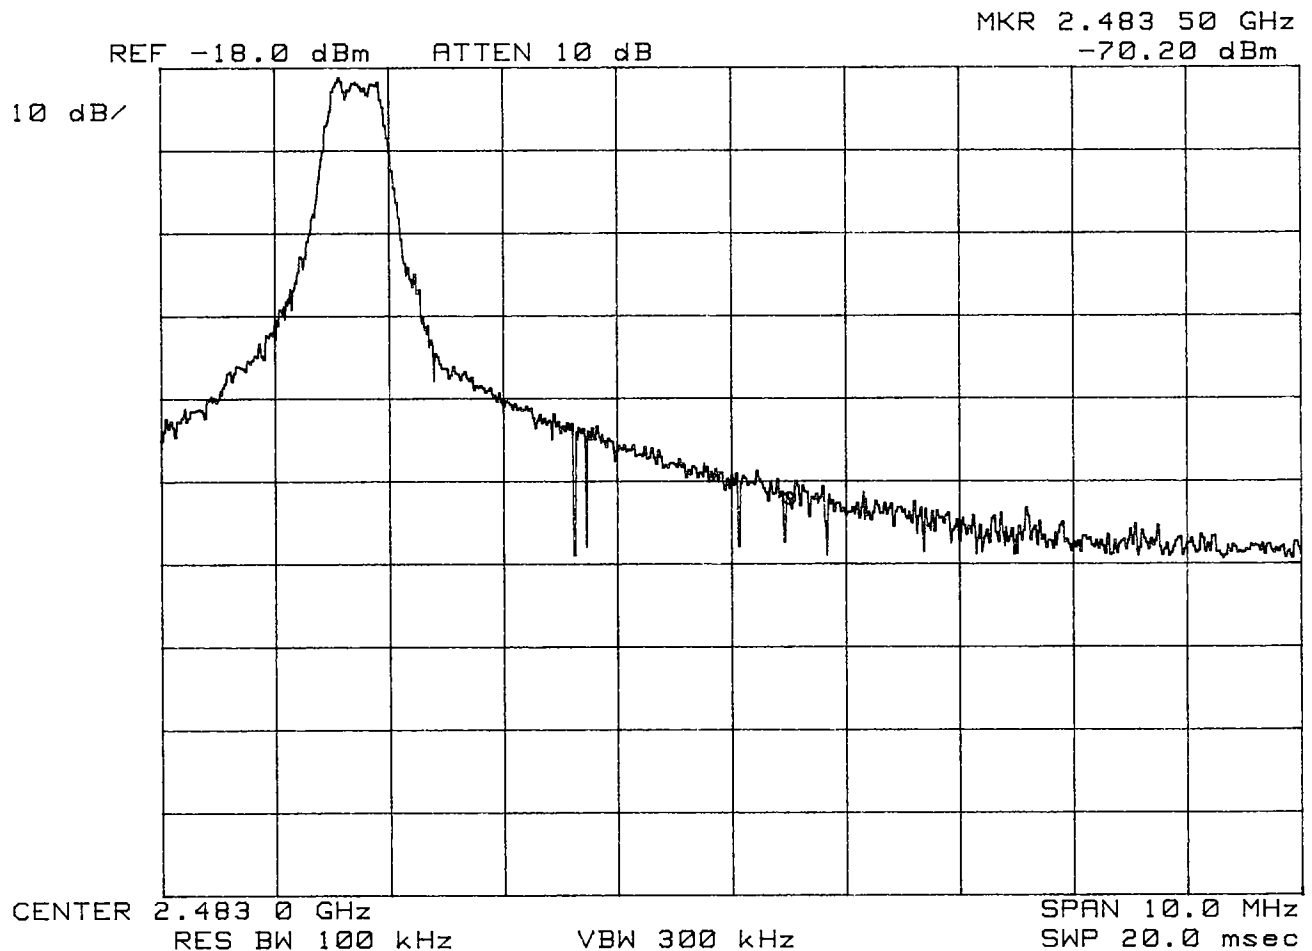

Agilent

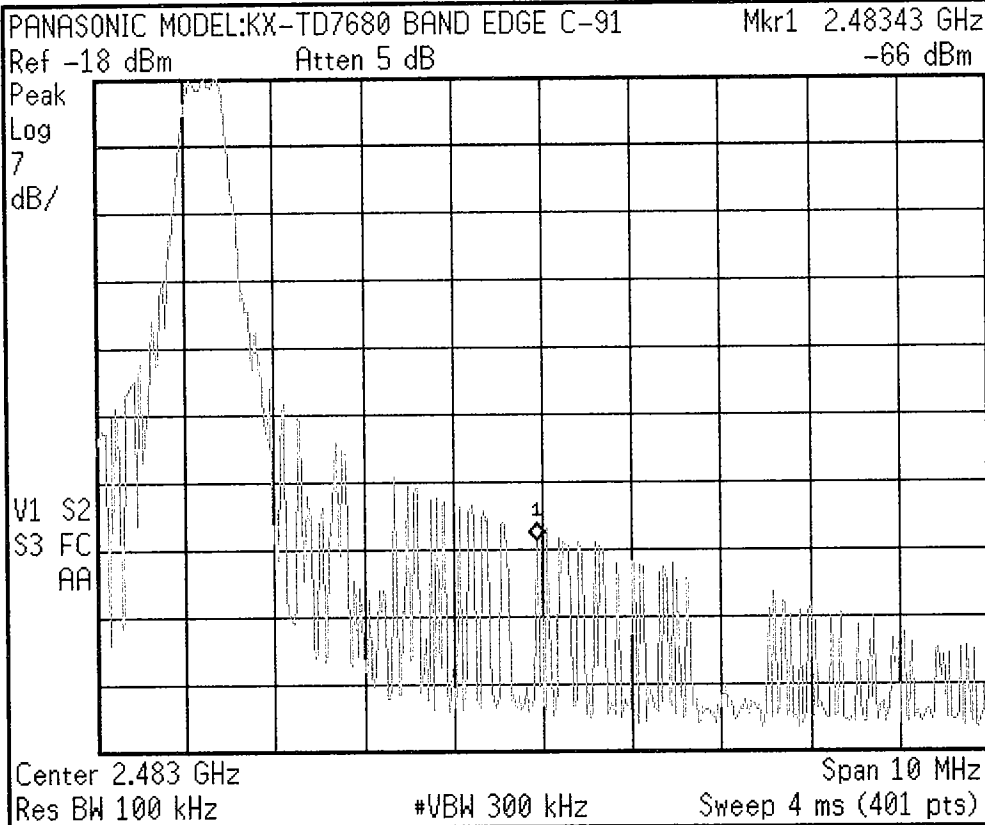

Freq/Channel

Center Freq  
2.48350000 GHz

Start Freq  
2.47850000 GHz

Stop Freq  
2.48850000 GHz


CF Step  
1.00000000 MHz  
Auto Man

Freq Offset  
0.00000000 Hz

Signal Track  
On Off

Scale Type  
Log Lin

Agilent

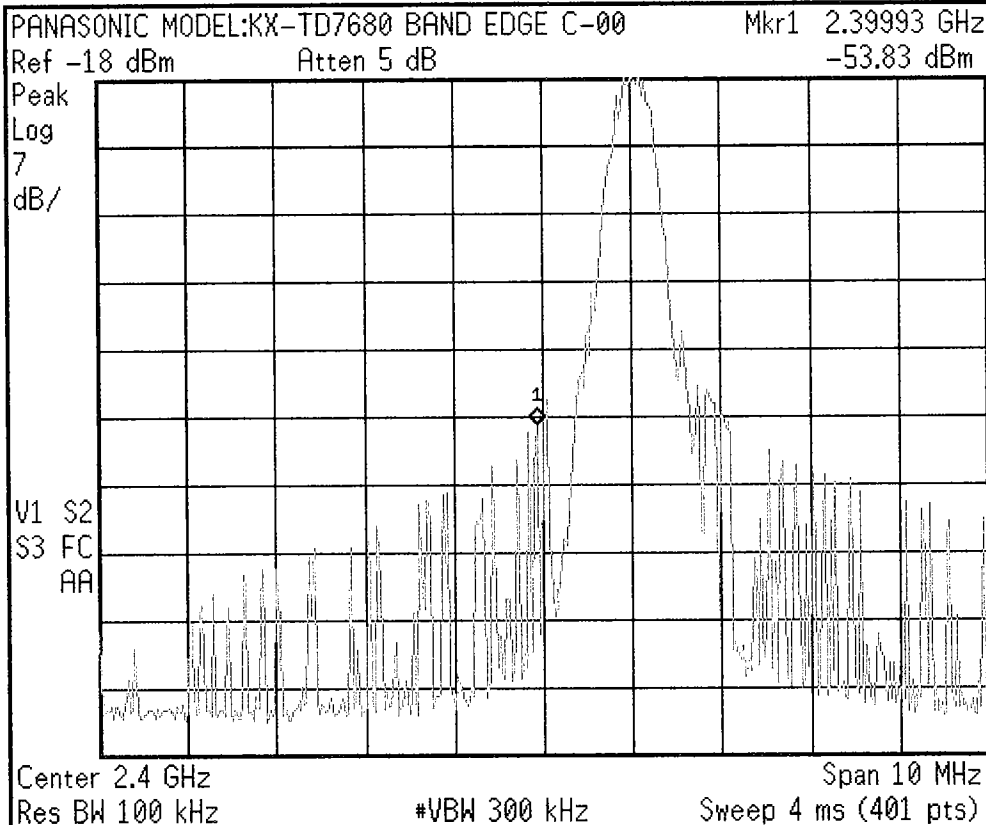

Freq/Channel

Center Freq  
2.40000000 GHz

Start Freq  
2.39500000 GHz

Stop Freq  
2.40500000 GHz


CF Step  
1.00000000 MHz  
Auto Man

Freq Offset  
0.00000000 Hz

Signal Track  
On Off


Scale Type  
Log Lin

Agilent

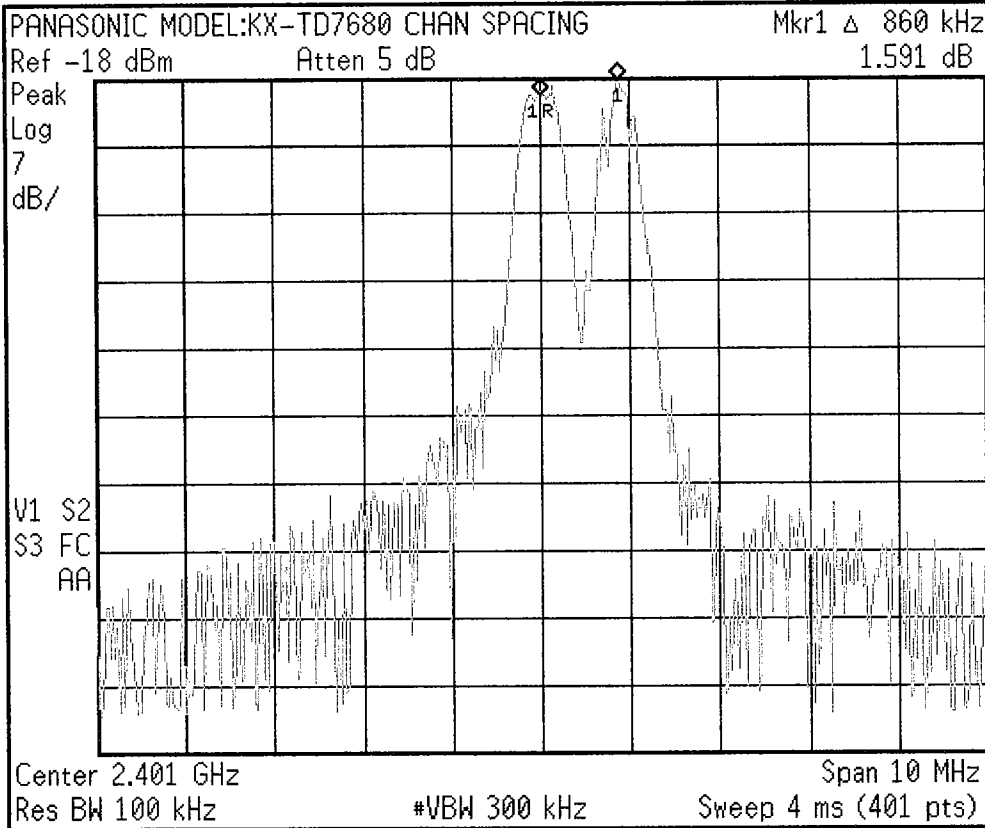


<b>Freq/Channel</b>
<b>Center Freq</b> 2.40100000 GHz
<b>Start Freq</b> 2.39600000 GHz
<b>Stop Freq</b> 2.40600000 GHz
<b>CF Step</b> 1.00000000 MHz Auto Man
<b>Freq Offset</b> 0.00000000 Hz
<b>Signal Track</b> On Off
<b>Scale Type</b> Log Lin

Agilent

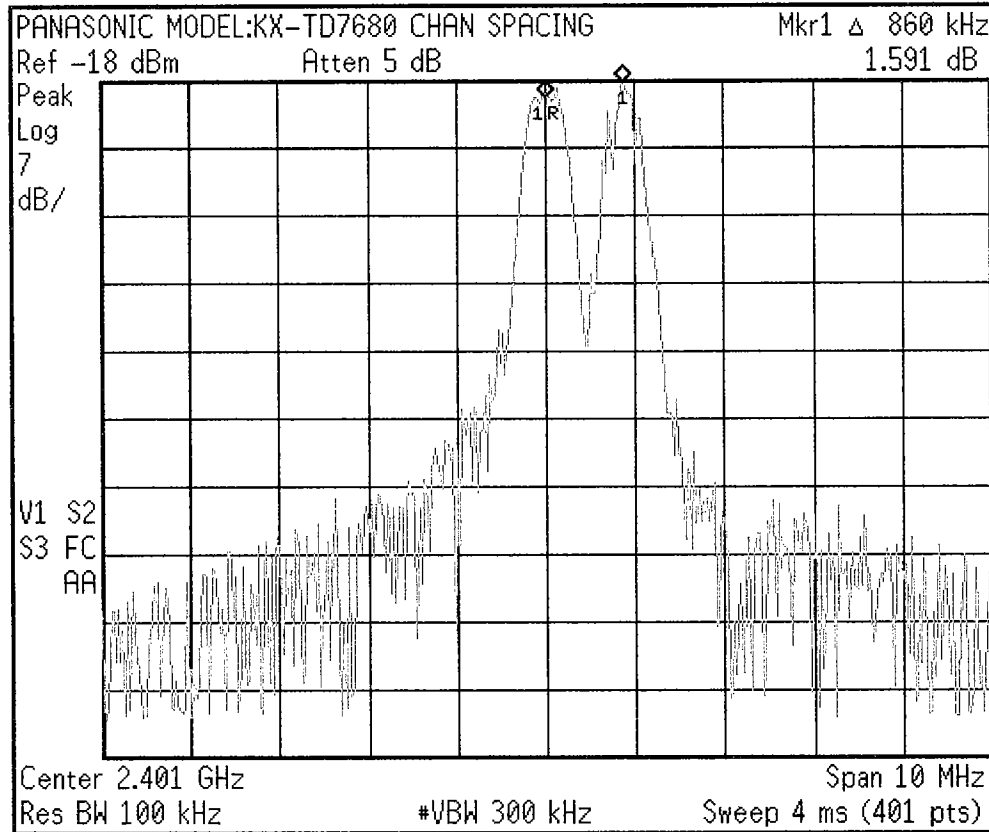

<b>Marker</b>
<b>Select Marker</b> 1 2 3 4
<b>Normal</b>
<b>Delta</b>
<b>Delta Pair</b> (Tracking Ref) Ref Delta
<b>Span Pair</b> Span Center
<b>Off</b>
<b>More</b> 1 of 2

Agilent

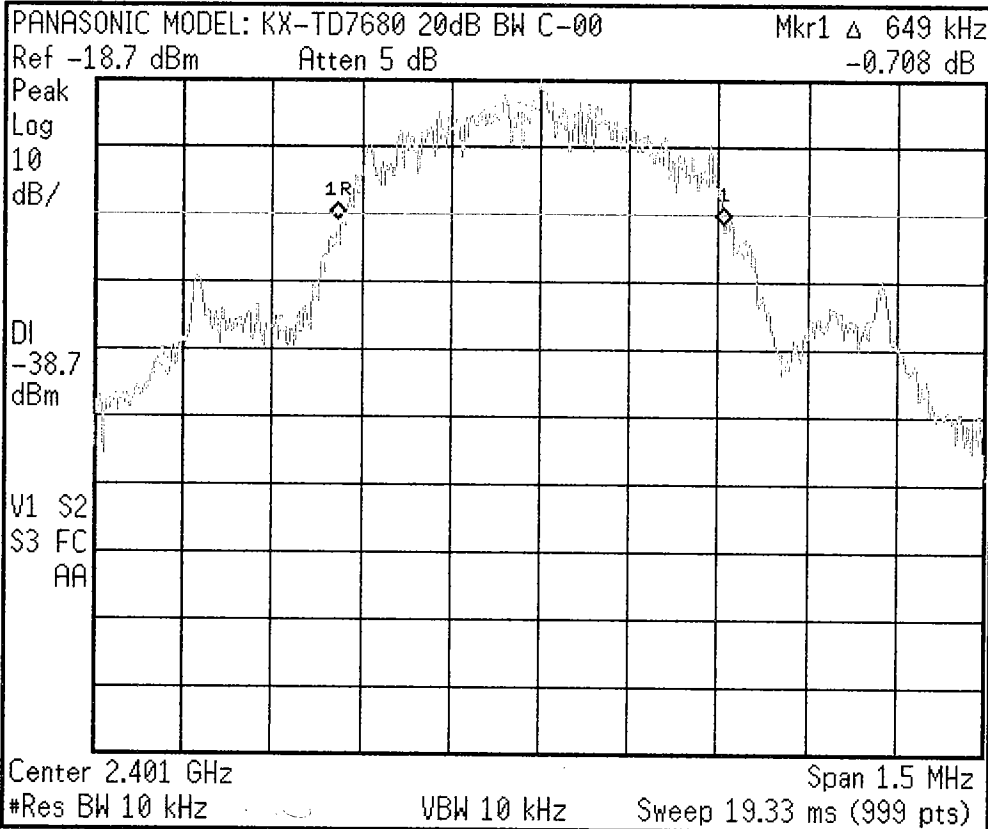

Freq/Channel

Center Freq  
2.40101700 GHz

Start Freq  
2.40026700 GHz

Stop Freq  
2.40176700 GHz


CF Step  
150.000000 kHz  
Auto Man

Freq Offset  
0.00000000 Hz

Signal Track  
On Off

Scale Type  
Log Lin

Agilent

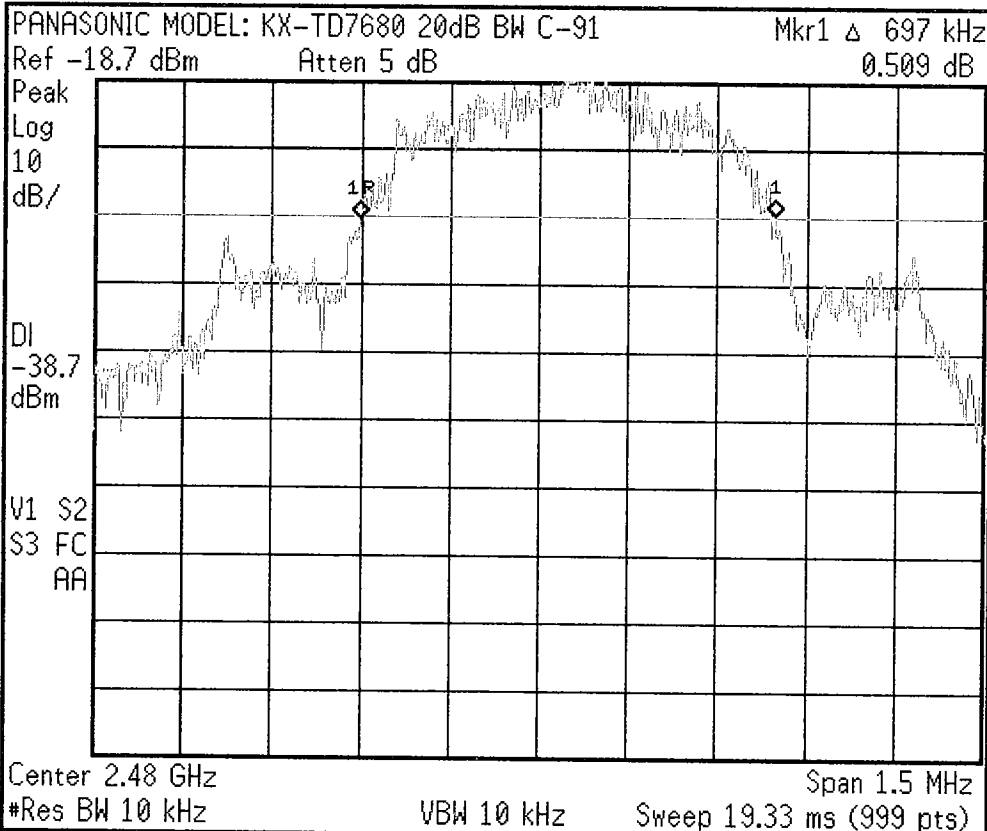

Freq/Channel

Center Freq  
2.47968000 GHz

Start Freq  
2.47893000 GHz

Stop Freq  
2.48043000 GHz


CF Step  
150.000000 kHz  
Auto Man

Freq Offset  
0.00000000 Hz

Signal Track  
On Off


Scale Type  
Log Lin

Agilent

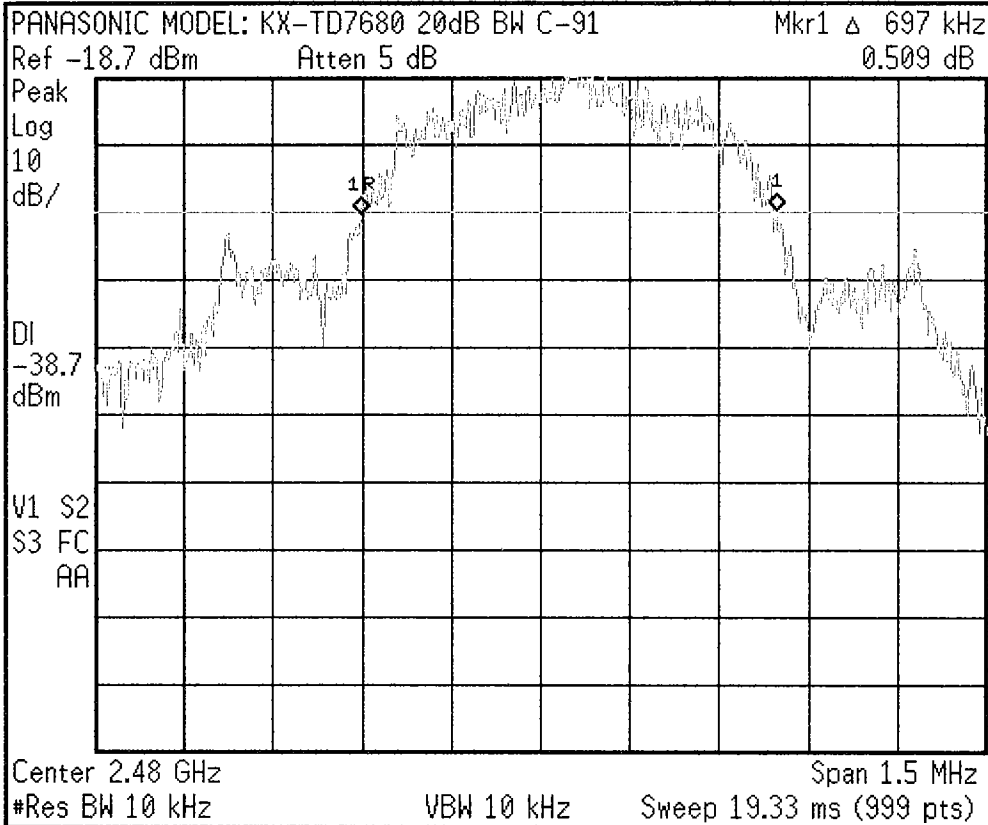


<b>Freq/Channel</b>
<b>Center Freq</b> 2.47968000 GHz
<b>Start Freq</b> 2.47893000 GHz
<b>Stop Freq</b> 2.48043000 GHz
<b>CF Step</b> 150.000000 kHz Auto Man
<b>Freq Offset</b> 0.00000000 Hz
<b>Signal Track</b> On Off
<b>Scale Type</b> Log Lin

Agilent

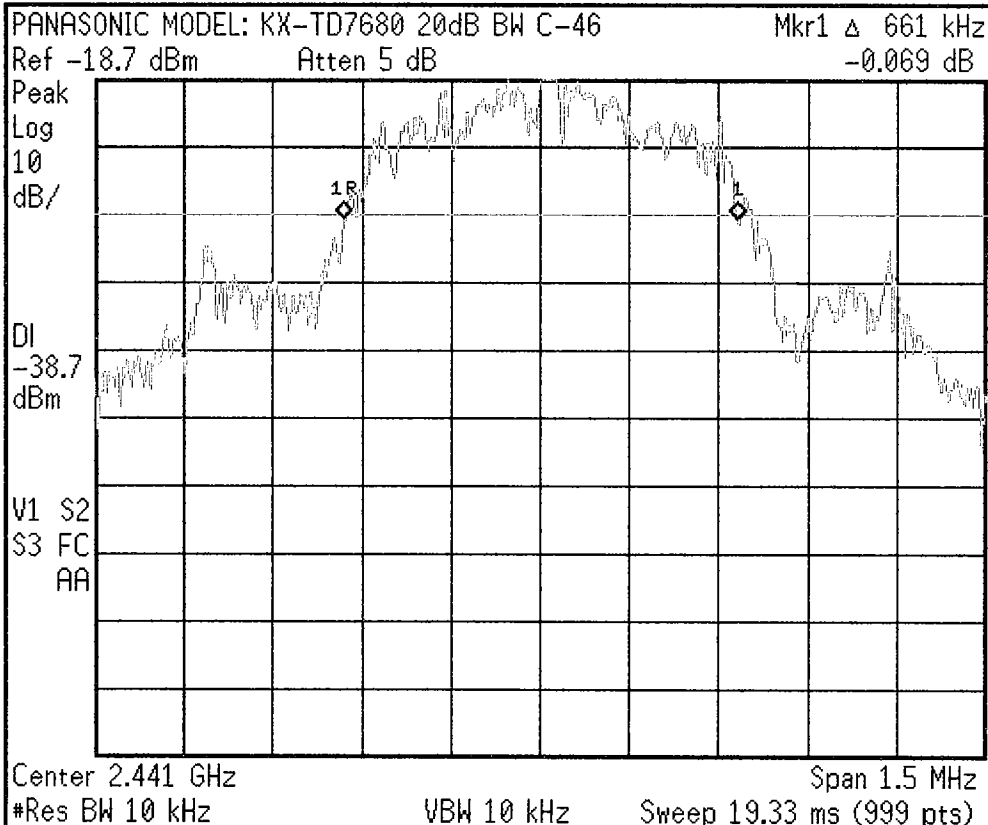


<b>Freq/Channel</b>
<b>Center Freq</b> 2.44080000 GHz
<b>Start Freq</b> 2.44005000 GHz
<b>Stop Freq</b> 2.44155000 GHz
<b>CF Step</b> 150.000000 kHz Auto Man
<b>Freq Offset</b> 0.00000000 Hz
<b>Signal Track</b> On Off
<b>Scale Type</b> Log Lin

\* Agilent

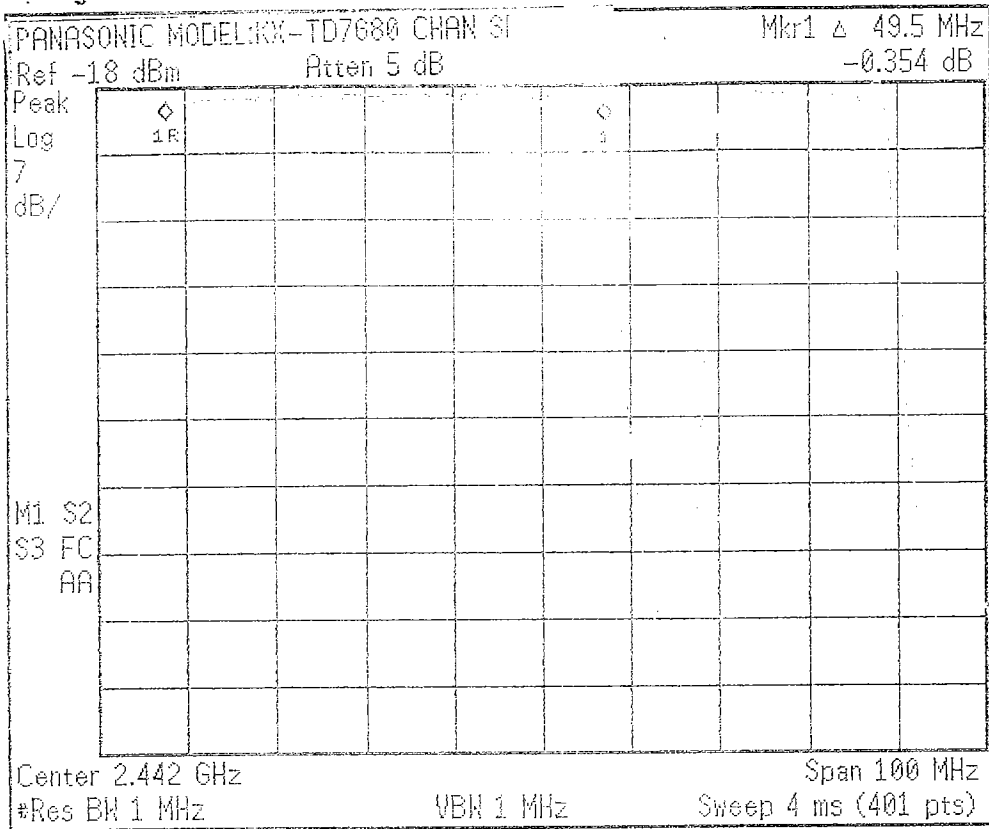

Marker			
Select Marker			
1	2	3	4
Normal			
Delta			
Delta Pair (Tracking Ref) Ref Delta			
Span Pair Span Center			
Off			
More 1 of 2			

\* Agilent

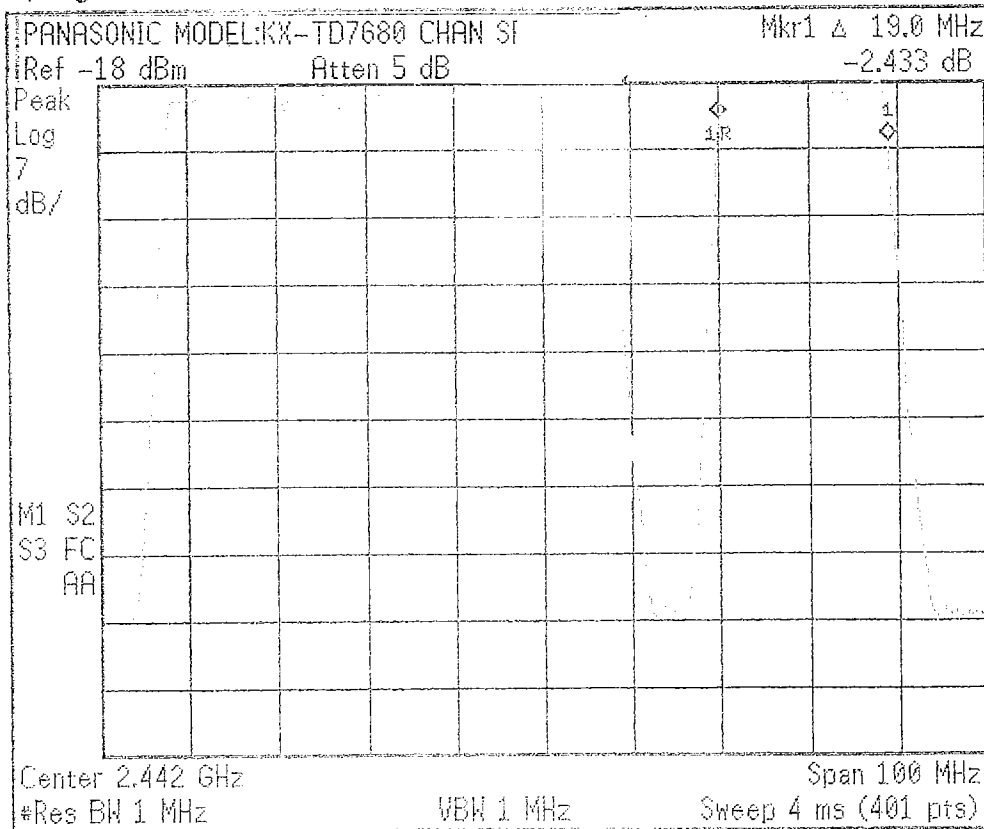

Marker			
Select Marker			
1	2	3	4
Normal			
Delta			
Delta Pair (Tracking Ref) Ref Delta			
Span Pair Span Center			
Off			
More 1 of 2			