

## DASY5 Validation Report for Head TSL

Date: 11.05.2021

Test Laboratory: SPEAG, Zurich, Switzerland

**DUT: Dipole 750 MHz; Type: D750V3; Serial: D750V3 - SN:1058**

Communication System: UID 0 - CW; Frequency: 750 MHz

Medium parameters used:  $f = 750 \text{ MHz}$ ;  $\sigma = 0.90 \text{ S/m}$ ;  $\epsilon_r = 42.6$ ;  $\rho = 1000 \text{ kg/m}^3$

Phantom section: Flat Section

Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2011)

DASY52 Configuration:

- Probe: EX3DV4 - SN7349; ConvF(10.11, 10.11, 10.11) @ 750 MHz; Calibrated: 28.12.2020
- Sensor-Surface: 1.4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn601; Calibrated: 02.11.2020
- Phantom: Flat Phantom 4.9 (front); Type: QD 00L P49 AA; Serial: 1001
- DASY52 52.10.4(1527); SEMCAD X 14.6.14(7483)

### Dipole Calibration for Head Tissue/Pin=250 mW, $d=15\text{mm}$ /Zoom Scan (7x7x7)/Cube 0:

Measurement grid:  $dx=5\text{mm}$ ,  $dy=5\text{mm}$ ,  $dz=5\text{mm}$

Reference Value = 60.16 V/m; Power Drift = -0.03 dB


Peak SAR (extrapolated) = 3.28 W/kg

**SAR(1 g) = 2.17 W/kg; SAR(10 g) = 1.41 W/kg**


Smallest distance from peaks to all points 3 dB below = 20.6 mm

Ratio of SAR at M2 to SAR at M1 = 65.9%

Maximum value of SAR (measured) = 2.90 W/kg

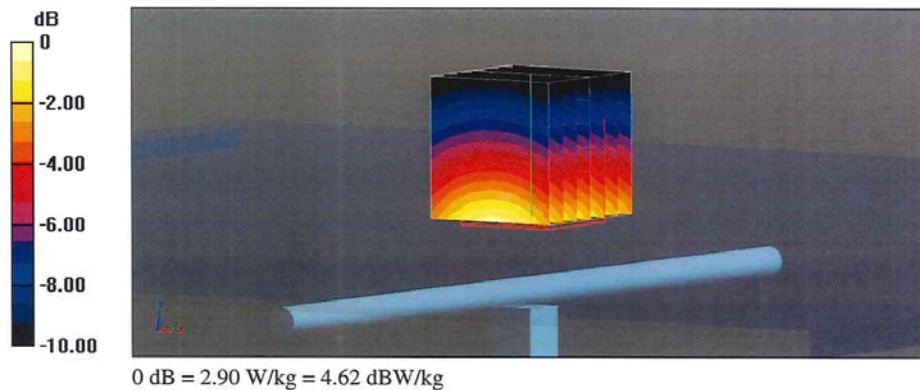

# Impedance Measurement Plot for Head TSL

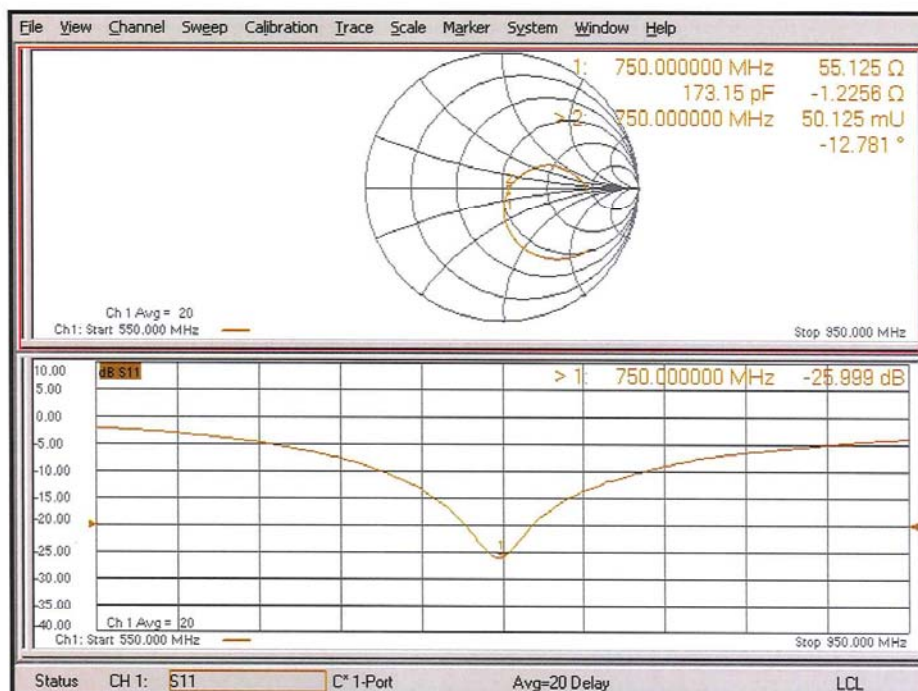

## DASY5 Validation Report for Body TSL

Date: 11.05.2021

Test Laboratory: SPEAG, Zurich, Switzerland

**DUT: Dipole 750 MHz; Type: D750V3; Serial: D750V3 - SN:1058**

Communication System: UID 0 - CW; Frequency: 750 MHz

Medium parameters used:  $f = 750$  MHz;  $\sigma = 0.97$  S/m;  $\epsilon_r = 55.8$ ;  $\rho = 1000$  kg/m<sup>3</sup>

Phantom section: Flat Section

Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2011)

DASY52 Configuration:

- Probe: EX3DV4 - SN7349; ConvF(10.23, 10.23, 10.23) @ 750 MHz; Calibrated: 28.12.2020
- Sensor-Surface: 1.4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn601; Calibrated: 02.11.2020
- Phantom: Flat Phantom 4.9 (Back); Type: QD 00R P49 AA; Serial: 1005
- DASY52 52.10.4(1527); SEMCAD X 14.6.14(7483)

### Dipole Calibration for Body Tissue/Pin=250 mW, d=15mm/Zoom Scan (7x7x7)/Cube 0:

Measurement grid: dx=5mm, dy=5mm, dz=5mm

Reference Value = 54.81 V/m; Power Drift = 0.01 dB


Peak SAR (extrapolated) = 3.37 W/kg

**SAR(1 g) = 2.23 W/kg; SAR(10 g) = 1.47 W/kg**

Smallest distance from peaks to all points 3 dB below = 16.5 mm


Ratio of SAR at M2 to SAR at M1 = 66.3%

Maximum value of SAR (measured) = 2.98 W/kg

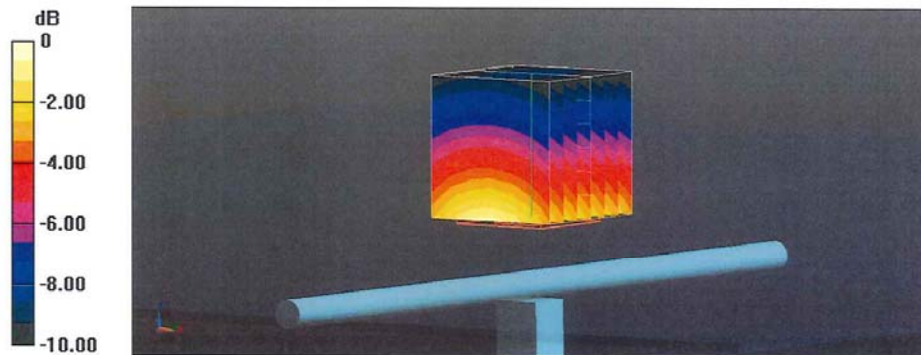

0 dB = 2.98 W/kg = 4.74 dBW/kg

## Impedance Measurement Plot for Body TSL

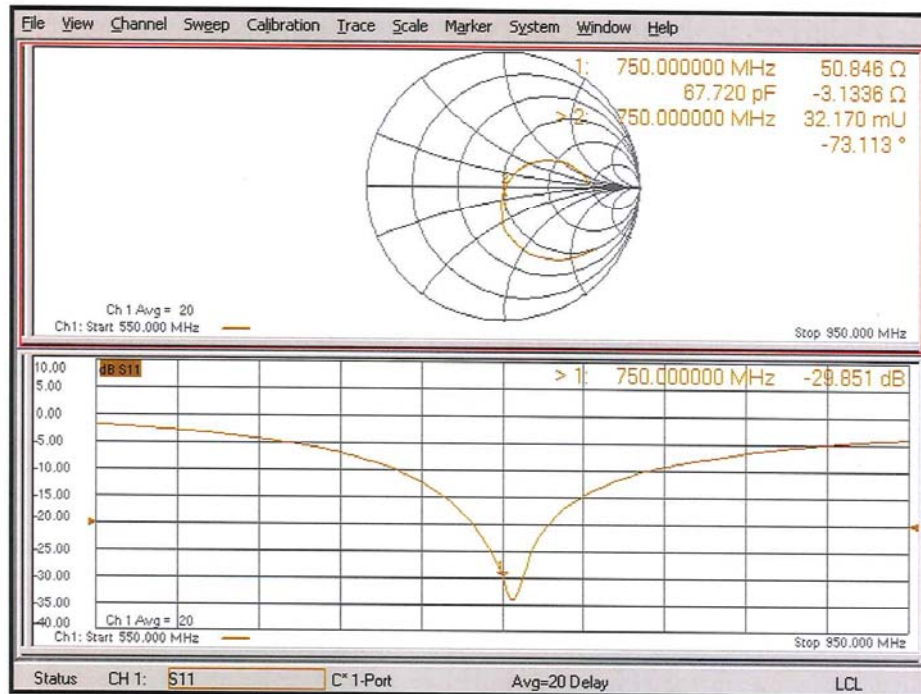

## D750V3 Calibration for Impedance and Return-loss

|             |                                 |        |        |
|-------------|---------------------------------|--------|--------|
| Equipment   | Dipole Antenna                  | Model  | D750V3 |
| Manufacture | Schmid & Partner Engineering AG | Serial | 1058   |
| Tested by   | Hisayoshi Sato                  |        |        |

### 1. Test environment

|                     |              |                   |        |
|---------------------|--------------|-------------------|--------|
| Date                | May 19, 2022 |                   |        |
| Ambient Temperature | 24.0 deg.C   | Relative humidity | 40 %RH |
| Date                | May 15, 2023 |                   |        |
| Ambient Temperature | 24.0 deg.C   | Relative humidity | 40 %RH |

### 2. Equipment used

#### May 19, 2022

| Local Id       | LIMS ID | Description            | Manufacturer                    | Model           | Serial        | Last Cal Date | Interval |
|----------------|---------|------------------------|---------------------------------|-----------------|---------------|---------------|----------|
| MPF-03         | 142057  | 2mm Oval Flat Phantom  | Schmid&Partner Engineering AG   | QDOVA001BB      | 1203          | 2021/05/28    | 12       |
| MOS-33         | 88581   | Thermo-Hygrometer      | CUSTOM. Inc                     | CTH-201         | -             | 2021/07/08    | 12       |
| MPF-02         | 142056  | 2mm Oval Flat Phantom  | Schmid&Partner Engineering AG   | QDOVA001BB      | 1045          | 2021/05/28    | 12       |
| MMBBL600-6000  | 176483  | Body Simulating Liquid | Schmid & Partner Engineering AG | MBBL600-6000    | SL AAM U16 BC | -             | -        |
| MHBBL600-10000 | 176484  | Head Simulating Liquid | Schmid & Partner Engineering AG | HBBL600-10000V6 | SL AAH U16 BC | -             | -        |
| EST-63         | 150815  | Network Analyzer       | Keysight Technologies Inc       | E5071C          | MY46523746    | 2021/07/02    | 12       |
| EST-57         | 141991  | 2.4mm Calibration Kit  | Keysight Technologies Inc       | 85056A          | MY44300225    | 2021/08/31    | 12       |

#### May 15, 2023

| Local Id       | LIMS ID | Description            | Manufacturer                    | Model           | Serial        | Last Cal Date | Interval |
|----------------|---------|------------------------|---------------------------------|-----------------|---------------|---------------|----------|
| MOS-33         | 88581   | Thermo-Hygrometer      | CUSTOM. Inc                     | CTH-201         | -             | 2022/07/03    | 12       |
| MPF-02         | 142056  | 2mm Oval Flat Phantom  | Schmid & Partner Engineering AG | QDOVA001BB      | 1045          | 2023/05/10    | 12       |
| MHBBL600-10000 | 176484  | Head Simulating Liquid | Schmid & Partner Engineering AG | HBBL600-10000V6 | SL AAH U16 BC | -             | -        |
| EST-63         | 150815  | Network Analyzer       | Keysight Technologies Inc       | E5071C          | MY46523746    | 2022/08/23    | 12       |
| EST-57         | 141991  | 2.4mm Calibration Kit  | Keysight Technologies Inc       | 85056A          | MY44300225    | 2022/08/18    | 12       |
| MPSAM-02       | 142060  | SAM Phantom            | Schmid & Partner Engineering AG | QD000P40CB      | 1333          | 2023/05/10    | 12       |
| MMBBL600-6000  | 176483  | Body Simulating Liquid | Schmid & Partner Engineering AG | MBBL600-6000    | SL AAM U16 BC | -             | -        |

### 3. Test Result

| Impeadance,Transformed to feed point | cal day   | Head<br>(real part) [Ω] | Head<br>(img part) [jΩ] | Deviation<br>(real part) [Ω] | Deviation<br>(img part) [jΩ] | Tolerance        | Result   |
|--------------------------------------|-----------|-------------------------|-------------------------|------------------------------|------------------------------|------------------|----------|
| Calibration (SPEAG)                  | 2021/5/11 | 55.10                   | -1.20                   | -                            | -                            | -                | -        |
| Calibration(ULJ)                     | 2022/5/19 | 54.11                   | -0.35                   | -0.99                        | 0.85                         | +/- 5 Ω +/- 5 jΩ | Complied |
| Calibration(ULJ)                     | 2023/5/15 | 54.84                   | -2.74                   | -0.26                        | -1.54                        | +/- 5 Ω +/- 5 jΩ | Complied |

| Return loss         | cal day   | Head<br>[dB] | Deviation<br>[%] | Deviation<br>[dB] | Tolerance<br>[%] | Tolerance<br>[+/- dB] | Result   |
|---------------------|-----------|--------------|------------------|-------------------|------------------|-----------------------|----------|
| Calibration (SPEAG) | 2021/5/11 | -26.00       | -                | -                 | -                | -                     | -        |
| Calibration(ULJ)    | 2022/5/19 | -28.02       | -7.77            | -2.02             | +/- 20.00        | 5.20                  | Complied |
| Calibration(ULJ)    | 2023/5/15 | -25.51       | 1.88             | 0.49              | +/- 20.00        | 5.60                  | Complied |


| Impeadance,Transformed to feed point | cal day   | Body<br>(real part) [Ω] | Body<br>(img part) [jΩ] | Deviation<br>(real part) [Ω] | Deviation<br>(img part) [jΩ] | Tolerance        | Result   |
|--------------------------------------|-----------|-------------------------|-------------------------|------------------------------|------------------------------|------------------|----------|
| Calibration (SPEAG)                  | 2021/5/11 | 50.80                   | -3.10                   | -                            | -                            | -                | -        |
| Calibration(ULJ)                     | 2022/5/19 | 49.83                   | -3.56                   | -0.97                        | -0.46                        | +/- 5 Ω +/- 5 jΩ | Complied |
| Calibration(ULJ)                     | 2023/5/15 | 49.70                   | -2.68                   | -1.10                        | 0.42                         | +/- 5 Ω +/- 5 jΩ | Complied |

| Return loss         | cal day   | Body<br>[dB] | Deviation<br>[%] | Deviation<br>[dB] | Tolerance<br>[%] | Tolerance<br>[+/- dB] | Result   |
|---------------------|-----------|--------------|------------------|-------------------|------------------|-----------------------|----------|
| Calibration (SPEAG) | 2021/5/11 | -29.90       | -                | -                 | -                | -                     | -        |
| Calibration(ULJ)    | 2022/5/19 | -28.83       | 3.59             | 1.07              | +/- 20.00        | 5.98                  | Complied |
| Calibration(ULJ)    | 2023/5/15 | -31.39       | -4.99            | -1.49             | +/- 20.00        | 5.77                  | Complied |


Tolerance: According to the KDB 865664 D1

## Measurement Plots (May 13, 2022)

### <Head Liquid>

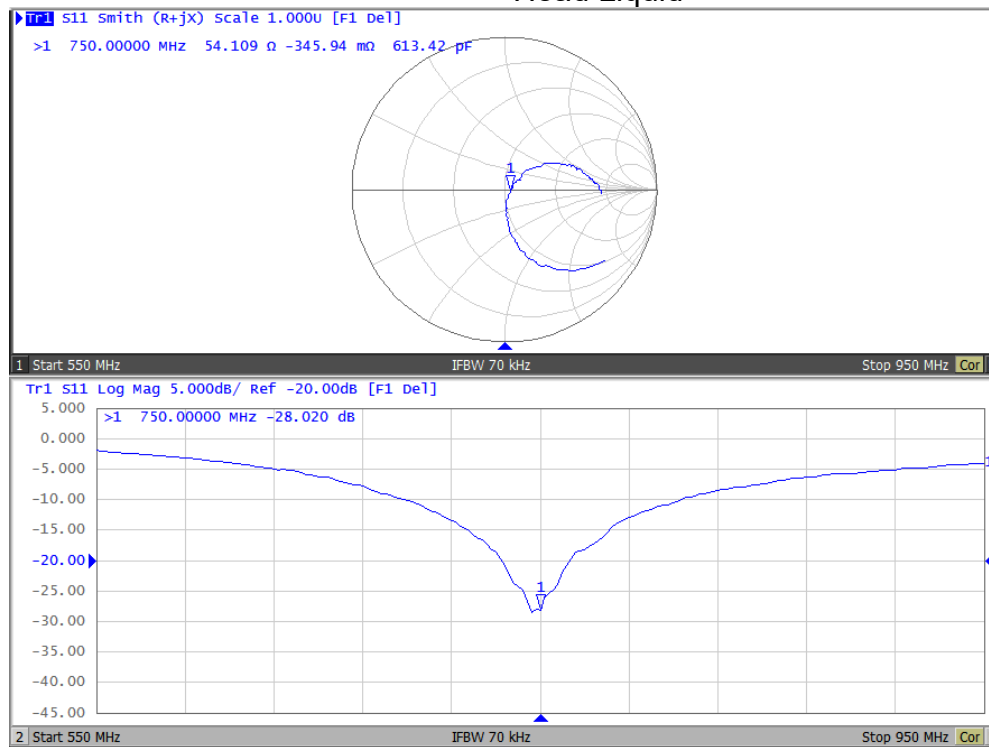


### <Body Liquid>

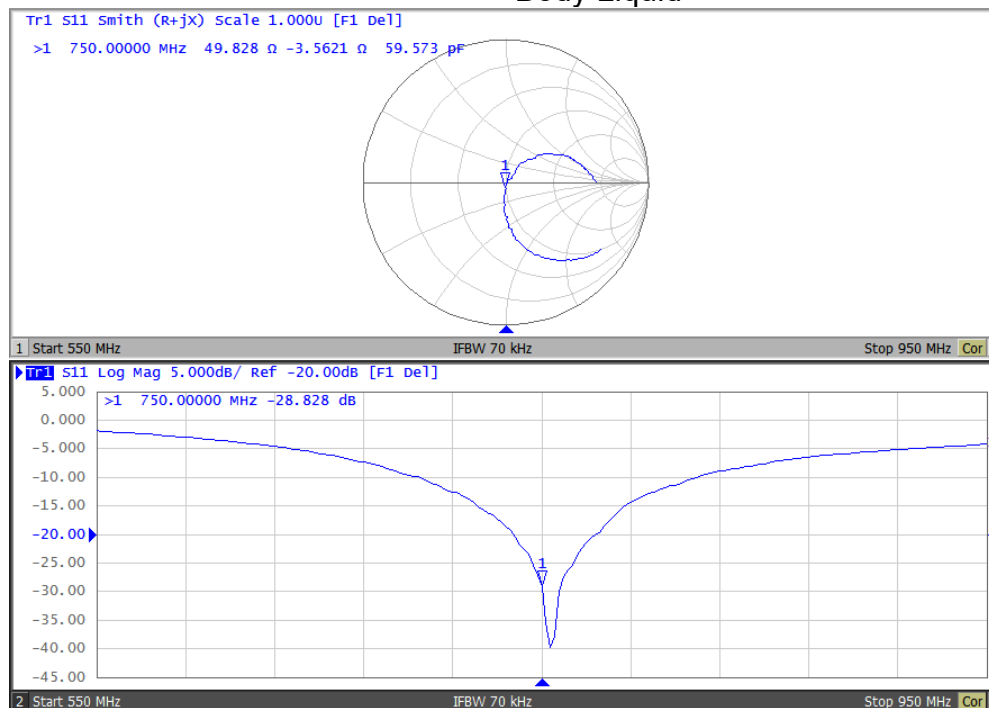


## Measurement Plots (May 15, 2023)

### <Head Liquid>

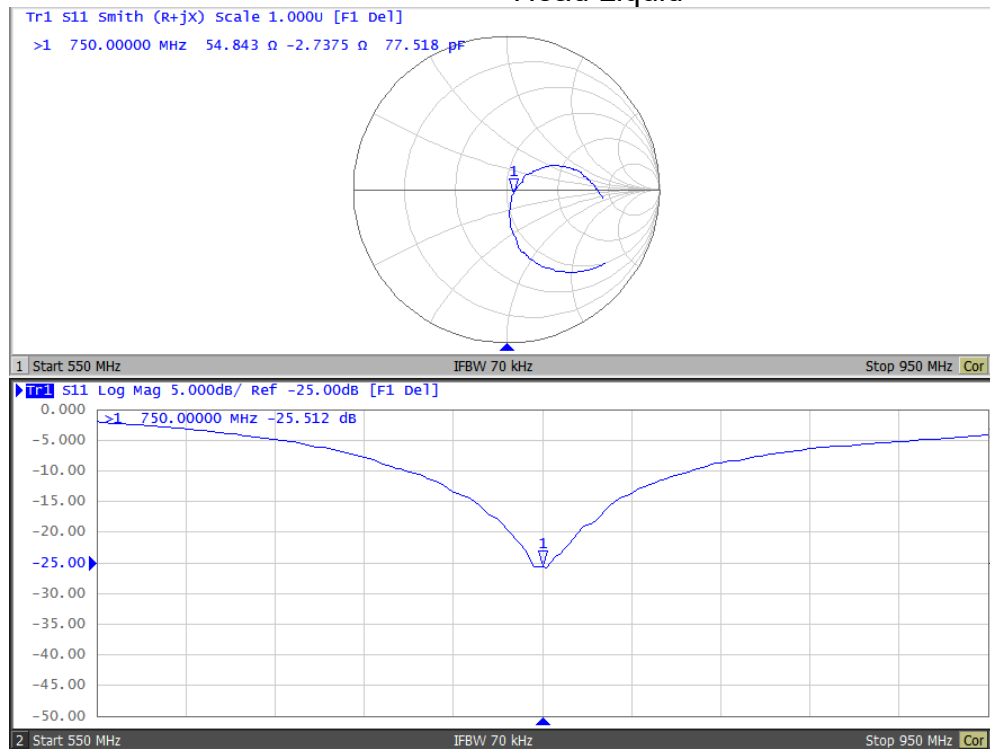

### <Body Liquid>

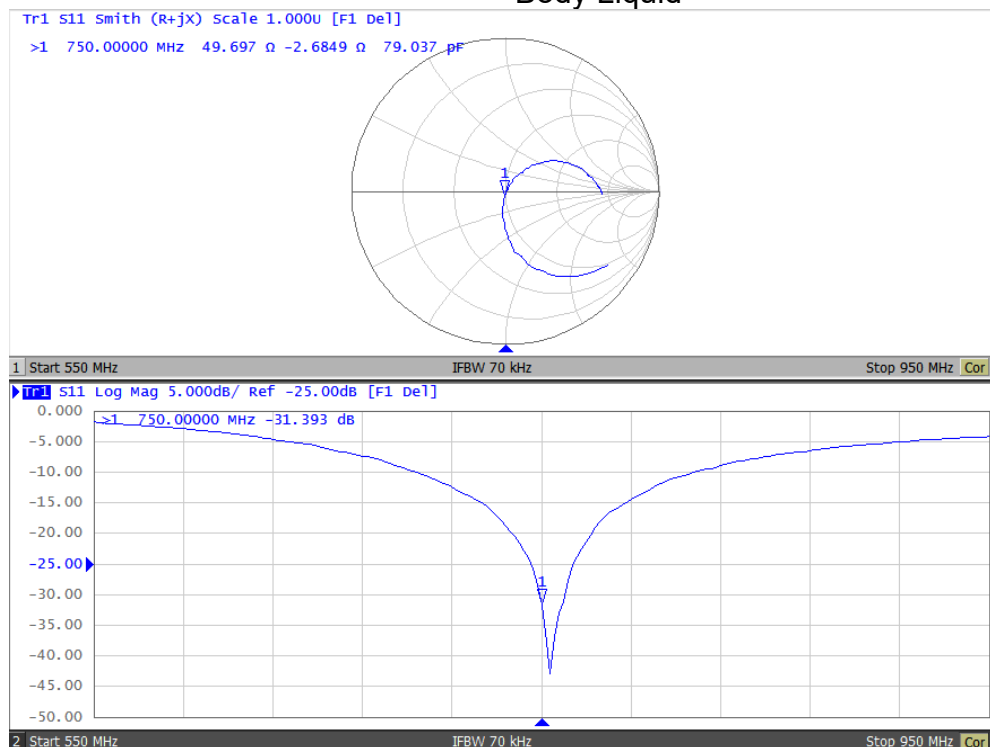



# F.4 System Check Dipole SAR Calibration Certificate -Dipole 835 MHz (D835V2 S/N: 4d149)

**Calibration Laboratory of  
Schmid & Partner  
Engineering AG**  
Zeughausstrasse 43, 8004 Zurich, Switzerland



**S** Schweizerischer Kalibrierdienst  
**C** Service suisse d'étalonnage  
**S** Servizio svizzero di taratura  
**S** Swiss Calibration Service

Accredited by the Swiss Accreditation Service (SAS)  
The Swiss Accreditation Service is one of the signatories to the EA  
Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: **SCS 0108**

Client **UL Japan Head Office (RCC)**

Certificate No: **D835V2-4d149\_Mar22**

## CALIBRATION CERTIFICATE

Object **D835V2 - SN:4d149**

Calibration procedure(s) **QA CAL-05.v11  
Calibration Procedure for SAR Validation Sources between 0.7-3 GHz**

Calibration date: **March 14, 2022**

This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI).  
The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility: environment temperature (22 ± 3)°C and humidity < 70%.

Calibration Equipment used (M&TE critical for calibration)

| Primary Standards               | ID #               | Cal Date (Certificate No.)        | Scheduled Calibration  |
|---------------------------------|--------------------|-----------------------------------|------------------------|
| Power meter NRP                 | SN: 104778         | 09-Apr-21 (No. 217-03291/03292)   | Apr-22                 |
| Power sensor NRP-Z91            | SN: 103244         | 09-Apr-21 (No. 217-03291)         | Apr-22                 |
| Power sensor NRP-Z91            | SN: 103245         | 09-Apr-21 (No. 217-03292)         | Apr-22                 |
| Reference 20 dB Attenuator      | SN: BH9394 (20k)   | 09-Apr-21 (No. 217-03343)         | Apr-22                 |
| Type-N mismatch combination     | SN: 310982 / 06327 | 09-Apr-21 (No. 217-03344)         | Apr-22                 |
| Reference Probe EX3DV4          | SN: 7349           | 31-Dec-21 (No. EX3-7349_Dec21)    | Dec-22                 |
| DAE4                            | SN: 601            | 01-Nov-21 (No. DAE4-601_Nov21)    | Nov-22                 |
| Secondary Standards             | ID #               | Check Date (in house)             | Scheduled Check        |
| Power meter E4419B              | SN: GB39512475     | 30-Oct-14 (in house check Oct-20) | In house check: Oct-22 |
| Power sensor HP 8481A           | SN: US37292783     | 07-Oct-15 (in house check Oct-20) | In house check: Oct-22 |
| Power sensor HP 8481A           | SN: MY41093315     | 07-Oct-15 (in house check Oct-20) | In house check: Oct-22 |
| RF generator R&S SMT-06         | SN: 100972         | 15-Jun-15 (in house check Oct-20) | In house check: Oct-22 |
| Network Analyzer Agilent E8358A | SN: US41080477     | 31-Mar-14 (in house check Oct-20) | In house check: Oct-22 |

Calibrated by: **Name: Michael Weber, Function: Laboratory Technician, Signature: [Signature]**

Approved by: **Name: Sven Kühn, Function: Deputy Manager, Signature: [Signature]**

Issued: March 22, 2022

This calibration certificate shall not be reproduced except in full without written approval of the laboratory.

**Calibration Laboratory of**  
**Schmid & Partner**  
**Engineering AG**  
Zeughausstrasse 43, 8004 Zurich, Switzerland



**S** Schweizerischer Kalibrierdienst  
**C** Service suisse d'étalonnage  
**S** Servizio svizzero di taratura  
**S** Swiss Calibration Service

Accredited by the Swiss Accreditation Service (SAS)  
The Swiss Accreditation Service is one of the signatories to the EA  
Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: **SCS 0108**

**Glossary:**

|       |                                 |
|-------|---------------------------------|
| TSL   | tissue simulating liquid        |
| ConvF | sensitivity in TSL / NORM x,y,z |
| N/A   | not applicable or not measured  |

**Calibration is Performed According to the Following Standards:**

- a) IEC/IEEE 62209-1528, "Measurement Procedure For The Assessment Of Specific Absorption Rate Of Human Exposure To Radio Frequency Fields From Hand-Held And Body-Worn Wireless Communication Devices - Part 1528: Human Models, Instrumentation And Procedures (Frequency Range of 4 MHz to 10 GHz)", October 2020.
- b) KDB 865664, "SAR Measurement Requirements for 100 MHz to 6 GHz"

**Additional Documentation:**

- c) DASY System Handbook

**Methods Applied and Interpretation of Parameters:**

- *Measurement Conditions:* Further details are available from the Validation Report at the end of the certificate. All figures stated in the certificate are valid at the frequency indicated.
- *Antenna Parameters with TSL:* The source is mounted in a touch configuration below the center marking of the flat phantom.
- *Return Loss:* This parameter is measured with the source positioned under the liquid filled phantom (as described in the measurement condition clause). The Return Loss ensures low reflected power. No uncertainty required.
- *SAR measured:* SAR measured at the stated antenna input power.
- *SAR normalized:* SAR as measured, normalized to an input power of 1 W at the antenna connector.
- *SAR for nominal TSL parameters:* The measured TSL parameters are used to calculate the nominal SAR result.

The reported uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor  $k=2$ , which for a normal distribution corresponds to a coverage probability of approximately 95%.

### Measurement Conditions

DASY system configuration, as far as not given on page 1.

|                              |                        |             |
|------------------------------|------------------------|-------------|
| DASY Version                 | DASY52                 | V52.10.4    |
| Extrapolation                | Advanced Extrapolation |             |
| Phantom                      | Modular Flat Phantom   |             |
| Distance Dipole Center - TSL | 15 mm                  | with Spacer |
| Zoom Scan Resolution         | dx, dy, dz = 5 mm      |             |
| Frequency                    | 835 MHz $\pm$ 1 MHz    |             |

### Head TSL parameters

The following parameters and calculations were applied.

|                                         | Temperature         | Permittivity   | Conductivity         |
|-----------------------------------------|---------------------|----------------|----------------------|
| Nominal Head TSL parameters             | 22.0 °C             | 41.5           | 0.90 mho/m           |
| Measured Head TSL parameters            | (22.0 $\pm$ 0.2) °C | 41.8 $\pm$ 6 % | 0.92 mho/m $\pm$ 6 % |
| Head TSL temperature change during test | < 0.5 °C            | ----           | ----                 |

### SAR result with Head TSL

|                                                       |                    |                              |
|-------------------------------------------------------|--------------------|------------------------------|
| SAR averaged over 1 cm <sup>3</sup> (1 g) of Head TSL | Condition          |                              |
| SAR measured                                          | 250 mW input power | 2.46 W/kg                    |
| SAR for nominal Head TSL parameters                   | normalized to 1W   | 9.69 W/kg $\pm$ 17.0 % (k=2) |

|                                                         |                    |                              |
|---------------------------------------------------------|--------------------|------------------------------|
| SAR averaged over 10 cm <sup>3</sup> (10 g) of Head TSL | condition          |                              |
| SAR measured                                            | 250 mW input power | 1.61 W/kg                    |
| SAR for nominal Head TSL parameters                     | normalized to 1W   | 6.35 W/kg $\pm$ 16.5 % (k=2) |

### Body TSL parameters

The following parameters and calculations were applied.

|                                         | Temperature         | Permittivity   | Conductivity         |
|-----------------------------------------|---------------------|----------------|----------------------|
| Nominal Body TSL parameters             | 22.0 °C             | 55.2           | 0.97 mho/m           |
| Measured Body TSL parameters            | (22.0 $\pm$ 0.2) °C | 54.8 $\pm$ 6 % | 1.00 mho/m $\pm$ 6 % |
| Body TSL temperature change during test | < 0.5 °C            | ----           | ----                 |

### SAR result with Body TSL

|                                                       |                    |                              |
|-------------------------------------------------------|--------------------|------------------------------|
| SAR averaged over 1 cm <sup>3</sup> (1 g) of Body TSL | Condition          |                              |
| SAR measured                                          | 250 mW input power | 2.49 W/kg                    |
| SAR for nominal Body TSL parameters                   | normalized to 1W   | 9.72 W/kg $\pm$ 17.0 % (k=2) |

|                                                         |                    |                              |
|---------------------------------------------------------|--------------------|------------------------------|
| SAR averaged over 10 cm <sup>3</sup> (10 g) of Body TSL | condition          |                              |
| SAR measured                                            | 250 mW input power | 1.64 W/kg                    |
| SAR for nominal Body TSL parameters                     | normalized to 1W   | 6.44 W/kg $\pm$ 16.5 % (k=2) |

---

## Appendix (Additional assessments outside the scope of SCS 0108)

### Antenna Parameters with Head TSL

|                                      |                                |
|--------------------------------------|--------------------------------|
| Impedance, transformed to feed point | 50.5 $\Omega$ - 3.7 j $\Omega$ |
| Return Loss                          | - 28.6 dB                      |

### Antenna Parameters with Body TSL

|                                      |                                |
|--------------------------------------|--------------------------------|
| Impedance, transformed to feed point | 48.6 $\Omega$ - 6.5 j $\Omega$ |
| Return Loss                          | - 23.5 dB                      |

### General Antenna Parameters and Design

|                                  |          |
|----------------------------------|----------|
| Electrical Delay (one direction) | 1.390 ns |
|----------------------------------|----------|

After long term use with 100W radiated power, only a slight warming of the dipole near the feedpoint can be measured.

The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals. On some of the dipoles, small end caps are added to the dipole arms in order to improve matching when loaded according to the position as explained in the "Measurement Conditions" paragraph. The SAR data are not affected by this change. The overall dipole length is still according to the Standard.

No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feedpoint may be damaged.

### Additional EUT Data

|                 |       |
|-----------------|-------|
| Manufactured by | SPEAG |
|-----------------|-------|

## DASY5 Validation Report for Head TSL

Date: 14.03.2022

Test Laboratory: SPEAG, Zurich, Switzerland

**DUT: Dipole 835 MHz; Type: D835V2; Serial: D835V2 - SN:4d149**

Communication System: UID 0 - CW; Frequency: 835 MHz

Medium parameters used:  $f = 835$  MHz;  $\sigma = 0.92$  S/m;  $\epsilon_r = 41.8$ ;  $\rho = 1000$  kg/m<sup>3</sup>

Phantom section: Flat Section

Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2011)

DASY52 Configuration:

- Probe: EX3DV4 - SN7349; ConvF(9.69, 9.69, 9.69) @ 835 MHz; Calibrated: 31.12.2021
- Sensor-Surface: 1.4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn601; Calibrated: 01.11.2021
- Phantom: Flat Phantom 4.9 (front); Type: QD 00L P49 AA; Serial: 1001
- DASY52 52.10.4(1535); SEMCAD X 14.6.14(7501)

### Dipole Calibration for Head Tissue/Pin=250 mW, d=15mm/Zoom Scan (7x7x7)/Cube 0:

Measurement grid: dx=5mm, dy=5mm, dz=5mm

Reference Value = 63.61 V/m; Power Drift = -0.01 dB


Peak SAR (extrapolated) = 3.65 W/kg

**SAR(1 g) = 2.46 W/kg; SAR(10 g) = 1.61 W/kg**


Smallest distance from peaks to all points 3 dB below = 16 mm

Ratio of SAR at M2 to SAR at M1 = 67.2%

Maximum value of SAR (measured) = 3.24 W/kg

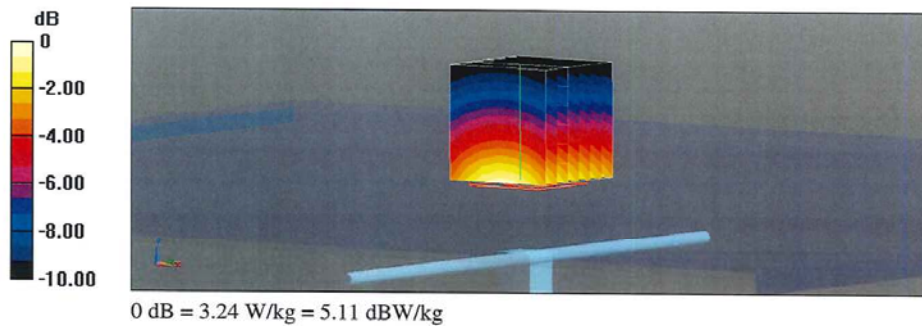

## Impedance Measurement Plot for Head TSL

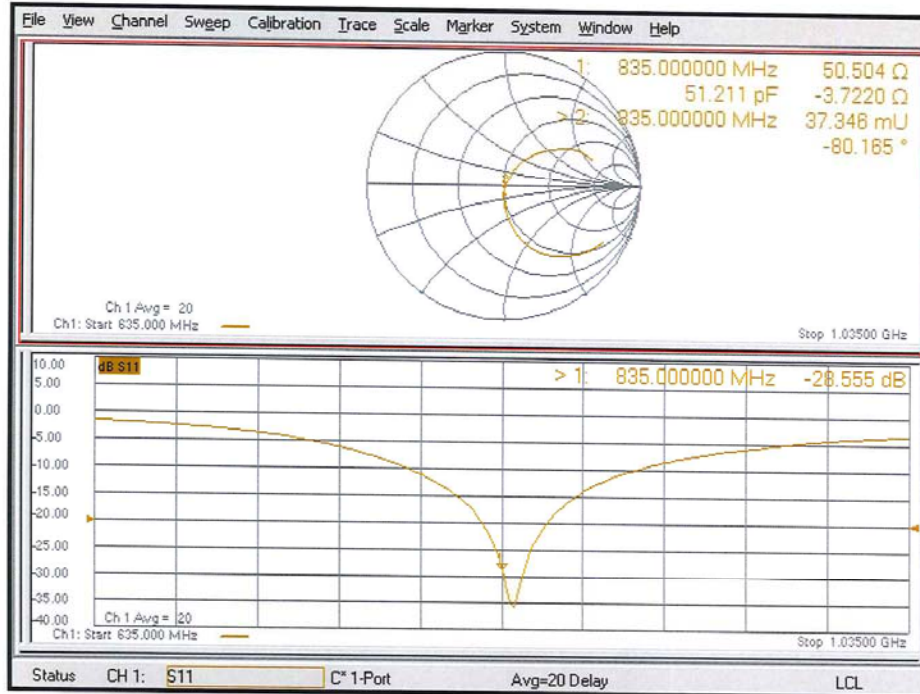



## DASY5 Validation Report for Body TSL

Date: 14.03.2022

Test Laboratory: SPEAG, Zurich, Switzerland

**DUT: Dipole 835 MHz; Type: D835V2; Serial: D835V2 - SN:4d149**

Communication System: UID 0 - CW; Frequency: 835 MHz

Medium parameters used:  $f = 835 \text{ MHz}$ ;  $\sigma = 1 \text{ S/m}$ ;  $\epsilon_r = 54.8$ ;  $\rho = 1000 \text{ kg/m}^3$

Phantom section: Flat Section

Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2011)

DASY52 Configuration:

- Probe: EX3DV4 - SN7349; ConvF(9.85, 9.85, 9.85) @ 835 MHz; Calibrated: 31.12.2021
- Sensor-Surface: 1.4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn601; Calibrated: 01.11.2021
- Phantom: Flat Phantom 4.9 (Back); Type: QD 00R P49 AA; Serial: 1005
- DASY52 52.10.4(1535); SEMCAD X 14.6.14(7501)

### Dipole Calibration for Body Tissue/Pin=250 mW, $d=15\text{mm}$ /Zoom Scan (7x7x7)/Cube 0:

Measurement grid:  $dx=5\text{mm}$ ,  $dy=5\text{mm}$ ,  $dz=5\text{mm}$

Reference Value = 58.79 V/m; Power Drift = -0.00 dB


Peak SAR (extrapolated) = 3.60 W/kg

**SAR(1 g) = 2.49 W/kg; SAR(10 g) = 1.64 W/kg**


Smallest distance from peaks to all points 3 dB below = 16 mm

Ratio of SAR at M2 to SAR at M1 = 69%

Maximum value of SAR (measured) = 3.26 W/kg

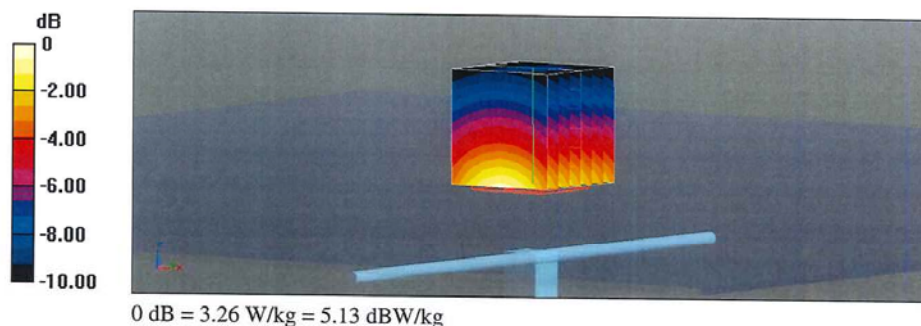

## Impedance Measurement Plot for Body TSL

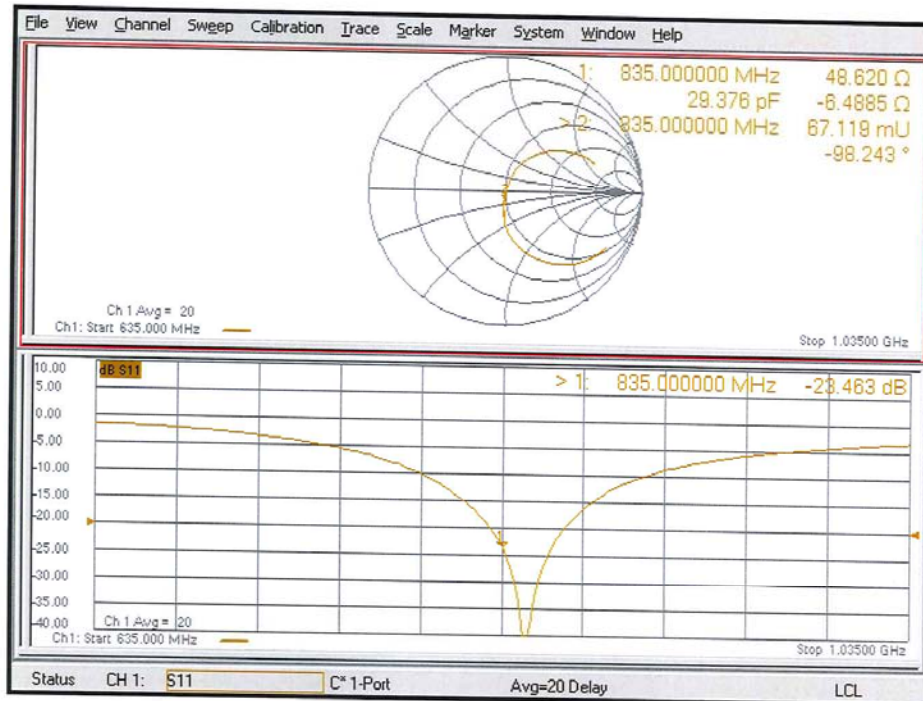



## Calibration for Impedance and Return-loss

|             |                                 |        |        |
|-------------|---------------------------------|--------|--------|
| Equipment   | Dipole Antenna                  | Model  | D835V2 |
| Manufacture | Schmid & Partner Engineering AG | Serial | 4d149  |
| Tested by   | Hisayoshi Sato in 2023          |        |        |
| Tested by   | Tomohisa Nakagawa in 2024       |        |        |

### 1. Test environment

|                     |                |                   |        |
|---------------------|----------------|-------------------|--------|
| Date                | March 23, 2023 |                   |        |
| Ambient Temperature | 24.0 deg.C     | Relative humidity | 40 %RH |
| Date                | March 12, 2024 |                   |        |
| Ambient Temperature | 24.0 deg.C     | Relative humidity | 40 %RH |

### 2. Equipment used

| LIMS ID      | Description            | Manufacturer                    | Model           | Serial        | Last Cal Date | Interval |
|--------------|------------------------|---------------------------------|-----------------|---------------|---------------|----------|
| Used in 2023 |                        |                                 |                 |               |               |          |
| 141574       | Digital thermometer    | LKM electronic                  | DTM3000         | -             | 2022/07/03    | 12       |
| 176484       | Head Simulating Liquid | Schmid & Partner Engineering AG | HBBL600-10000V6 | SL AAH U16 BC | -             | -        |
| 150815       | Network Analyzer       | Keysight Technologies Inc       | E5071C          | MY46523746    | 2022/08/23    | 12       |
| 141991       | 2.4mm Calibration Kit  | Keysight Technologies Inc       | 85056A          | MY44300225    | 2022/08/18    | 12       |
| 142060       | SAM Phantom            | Schmid & Partner Engineering AG | QD000P40CB      | 1333          | 2022/05/23    | 12       |
| Used in 2024 |                        |                                 |                 |               |               |          |
| 176484       | Head Simulating Liquid | Schmid & Partner Engineering AG | HBBL600-10000V6 | SL AAH U16 BC | -             | -        |
| 150815       | Network Analyzer       | Keysight Technologies Inc       | E5071C          | MY46523746    | 2023/08/11    | 12       |
| 88581        | Thermo-Hygrometer      | CUSTOM. Inc                     | CTH-201         | -             | 2023/07/18    | 12       |
| 142056       | 2mm Oval Flat Phantom  | Schmid & Partner Engineering AG | QDOVA001BB      | 1045          | 2023/05/10    | 12       |
| 150816       | Calibration Kit        | Keysight Technologies Inc       | 85032F          | MY53200995    | 2023/08/17    | 12       |


### 3. Test Result (only head condition)

| Impedance, Transformed to feed point | cal day   | Head (real part) [Ω] | Head (img part) [jΩ] | Deviation (real part) [Ω] | Deviation (img part) [jΩ] | Tolerance        | Result   |
|--------------------------------------|-----------|----------------------|----------------------|---------------------------|---------------------------|------------------|----------|
| Calibration (SPEAG)                  | 2022/3/14 | 50.50                | -3.72                | -                         | -                         | -                | -        |
| Calibration(ULJ)                     | 2023/3/23 | 54.17                | 0.50                 | 3.67                      | 4.22                      | +/- 5 Ω +/- 5 jΩ | Complied |
| Calibration(ULJ)                     | 2023/3/12 | 52.78                | 0.23                 | 2.28                      | 3.95                      | +/- 5 Ω +/- 5 jΩ | Complied |


| Return loss         | cal day   | Head [dB] | Deviation [%] | Deviation [dB] | Tolerance [%] | Tolerance [ +/- dB] | Result   |
|---------------------|-----------|-----------|---------------|----------------|---------------|---------------------|----------|
| Calibration (SPEAG) | 2022/3/14 | -28.56    | -             | -              | -             | -                   | -        |
| Calibration(ULJ)    | 2023/3/23 | -27.86    | 2.46          | 0.70           | +/- 20.00     | 5.71                | Complied |
| Calibration(ULJ)    | 2023/3/12 | -30.85    | -10.75        | -3.00          | +/- 20.00     | 5.71                | Complied |

Tolerance: According to the KDB 865664 D1

## Measurement Plots <Head Liquid> 2023

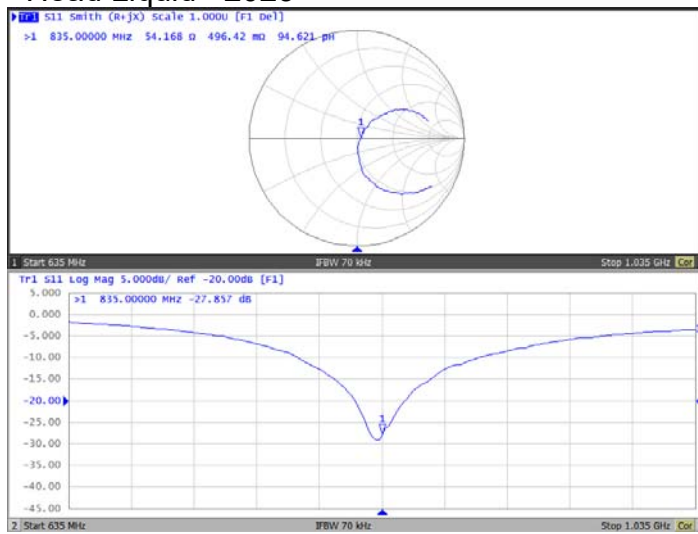

## <Head Liquid> 2024

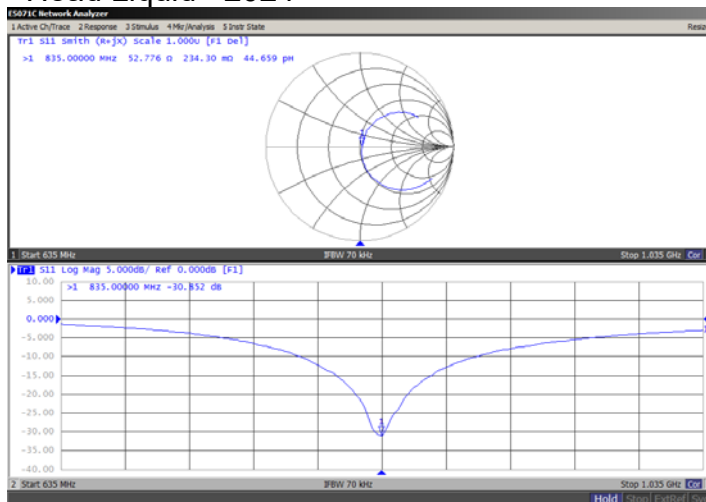

# F.5 System Check Dipole SAR Calibration Certificate -Dipole 1750 MHz (D1750V2 S/N: 1089)

**Calibration Laboratory of**  
**Schmid & Partner**  
**Engineering AG**  
 Zeughausstrasse 43, 8004 Zurich, Switzerland



**S** Schweizerischer Kalibrierdienst  
**C** Service suisse d'étalonnage  
**S** Servizio svizzero di taratura  
**S** Swiss Calibration Service

Accredited by the Swiss Accreditation Service (SAS)  
 The Swiss Accreditation Service is one of the signatories to the EA  
 Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: **SCS 0108**

Client **UL Japan Head Office (RCC)**

Certificate No: **D1750V2-1089\_Mar22**

## CALIBRATION CERTIFICATE

Object **D1750V2 - SN:1089**

Calibration procedure(s) **QA CAL-05.v11**  
**Calibration Procedure for SAR Validation Sources between 0.7-3 GHz**

Calibration date: **March 15, 2022**

This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI).  
 The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility: environment temperature ( $22 \pm 3$ )°C and humidity < 70%.

Calibration Equipment used (M&TE critical for calibration)

| Primary Standards               | ID #               | Cal Date (Certificate No.)        | Scheduled Calibration  |
|---------------------------------|--------------------|-----------------------------------|------------------------|
| Power meter NRP                 | SN: 104778         | 09-Apr-21 (No. 217-03291/03292)   | Apr-22                 |
| Power sensor NRP-Z91            | SN: 103244         | 09-Apr-21 (No. 217-03291)         | Apr-22                 |
| Power sensor NRP-Z91            | SN: 103245         | 09-Apr-21 (No. 217-03292)         | Apr-22                 |
| Reference 20 dB Attenuator      | SN: BH9394 (20k)   | 09-Apr-21 (No. 217-03343)         | Apr-22                 |
| Type-N mismatch combination     | SN: 310982 / 06327 | 09-Apr-21 (No. 217-03344)         | Apr-22                 |
| Reference Probe EX3DV4          | SN: 7349           | 31-Dec-21 (No. EX3-7349_Dec21)    | Dec-22                 |
| DAE4                            | SN: 601            | 01-Nov-21 (No. DAE4-601_Nov21)    | Nov-22                 |
| Secondary Standards             | ID #               | Check Date (in house)             | Scheduled Check        |
| Power meter E4419B              | SN: GB39512475     | 30-Oct-14 (in house check Oct-20) | In house check: Oct-22 |
| Power sensor HP 8481A           | SN: US37292783     | 07-Oct-15 (in house check Oct-20) | In house check: Oct-22 |
| Power sensor HP 8481A           | SN: MY41093315     | 07-Oct-15 (in house check Oct-20) | In house check: Oct-22 |
| RF generator R&S SMT-06         | SN: 100972         | 15-Jun-15 (in house check Oct-20) | In house check: Oct-22 |
| Network Analyzer Agilent E8358A | SN: US41080477     | 31-Mar-14 (in house check Oct-20) | In house check: Oct-22 |

|                | Name               | Function              | Signature |
|----------------|--------------------|-----------------------|-----------|
| Calibrated by: | Aidonia Georgiadou | Laboratory Technician |           |
| Approved by:   | Sven Kühn          | Deputy Manager        |           |

Issued: March 16, 2022

This calibration certificate shall not be reproduced except in full without written approval of the laboratory.

**Calibration Laboratory of**  
**Schmid & Partner**  
**Engineering AG**  
Zeughausstrasse 43, 8004 Zurich, Switzerland



**S** Schweizerischer Kalibrierdienst  
**C** Service suisse d'étalonnage  
**S** Servizio svizzero di taratura  
**S** Swiss Calibration Service

Accredited by the Swiss Accreditation Service (SAS)  
The Swiss Accreditation Service is one of the signatories to the EA  
Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: **SCS 0108**

**Glossary:**

|       |                                 |
|-------|---------------------------------|
| TSL   | tissue simulating liquid        |
| ConvF | sensitivity in TSL / NORM x,y,z |
| N/A   | not applicable or not measured  |

**Calibration is Performed According to the Following Standards:**

- a) IEC/IEEE 62209-1528, "Measurement Procedure For The Assessment Of Specific Absorption Rate Of Human Exposure To Radio Frequency Fields From Hand-Held And Body-Worn Wireless Communication Devices - Part 1528: Human Models, Instrumentation And Procedures (Frequency Range of 4 MHz to 10 GHz)", October 2020.
- b) KDB 865664, "SAR Measurement Requirements for 100 MHz to 6 GHz"

**Additional Documentation:**

- c) DASY System Handbook

**Methods Applied and Interpretation of Parameters:**

- *Measurement Conditions:* Further details are available from the Validation Report at the end of the certificate. All figures stated in the certificate are valid at the frequency indicated.
- *Antenna Parameters with TSL:* The source is mounted in a touch configuration below the center marking of the flat phantom.
- *Return Loss:* This parameter is measured with the source positioned under the liquid filled phantom (as described in the measurement condition clause). The Return Loss ensures low reflected power. No uncertainty required.
- *SAR measured:* SAR measured at the stated antenna input power.
- *SAR normalized:* SAR as measured, normalized to an input power of 1 W at the antenna connector.
- *SAR for nominal TSL parameters:* The measured TSL parameters are used to calculate the nominal SAR result.

The reported uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor  $k=2$ , which for a normal distribution corresponds to a coverage probability of approximately 95%.

### Measurement Conditions

DASY system configuration, as far as not given on page 1.

|                              |                        |             |
|------------------------------|------------------------|-------------|
| DASY Version                 | DASY52                 | V52.10.4    |
| Extrapolation                | Advanced Extrapolation |             |
| Phantom                      | Modular Flat Phantom   |             |
| Distance Dipole Center - TSL | 10 mm                  | with Spacer |
| Zoom Scan Resolution         | dx, dy, dz = 5 mm      |             |
| Frequency                    | 1750 MHz $\pm$ 1 MHz   |             |

### Head TSL parameters

The following parameters and calculations were applied.

|                                         | Temperature         | Permittivity   | Conductivity         |
|-----------------------------------------|---------------------|----------------|----------------------|
| Nominal Head TSL parameters             | 22.0 °C             | 40.1           | 1.37 mho/m           |
| Measured Head TSL parameters            | (22.0 $\pm$ 0.2) °C | 40.0 $\pm$ 6 % | 1.35 mho/m $\pm$ 6 % |
| Head TSL temperature change during test | < 0.5 °C            | ---            | ---                  |

### SAR result with Head TSL

|                                                       |                    |                              |
|-------------------------------------------------------|--------------------|------------------------------|
| SAR averaged over 1 cm <sup>3</sup> (1 g) of Head TSL | Condition          |                              |
| SAR measured                                          | 250 mW input power | 9.19 W/kg                    |
| SAR for nominal Head TSL parameters                   | normalized to 1W   | 37.1 W/kg $\pm$ 17.0 % (k=2) |

|                                                         |                    |                              |
|---------------------------------------------------------|--------------------|------------------------------|
| SAR averaged over 10 cm <sup>3</sup> (10 g) of Head TSL | condition          |                              |
| SAR measured                                            | 250 mW input power | 4.84 W/kg                    |
| SAR for nominal Head TSL parameters                     | normalized to 1W   | 19.5 W/kg $\pm$ 16.5 % (k=2) |

### Body TSL parameters

The following parameters and calculations were applied.

|                                         | Temperature         | Permittivity   | Conductivity         |
|-----------------------------------------|---------------------|----------------|----------------------|
| Nominal Body TSL parameters             | 22.0 °C             | 53.4           | 1.49 mho/m           |
| Measured Body TSL parameters            | (22.0 $\pm$ 0.2) °C | 53.4 $\pm$ 6 % | 1.48 mho/m $\pm$ 6 % |
| Body TSL temperature change during test | < 0.5 °C            | ---            | ---                  |

### SAR result with Body TSL

|                                                       |                    |                              |
|-------------------------------------------------------|--------------------|------------------------------|
| SAR averaged over 1 cm <sup>3</sup> (1 g) of Body TSL | Condition          |                              |
| SAR measured                                          | 250 mW input power | 9.24 W/kg                    |
| SAR for nominal Body TSL parameters                   | normalized to 1W   | 37.1 W/kg $\pm$ 17.0 % (k=2) |

|                                                         |                    |                              |
|---------------------------------------------------------|--------------------|------------------------------|
| SAR averaged over 10 cm <sup>3</sup> (10 g) of Body TSL | condition          |                              |
| SAR measured                                            | 250 mW input power | 4.90 W/kg                    |
| SAR for nominal Body TSL parameters                     | normalized to 1W   | 19.7 W/kg $\pm$ 16.5 % (k=2) |

---

## Appendix (Additional assessments outside the scope of SCS 0108)

### Antenna Parameters with Head TSL

|                                      |                                |
|--------------------------------------|--------------------------------|
| Impedance, transformed to feed point | 50.6 $\Omega$ - 1.0 j $\Omega$ |
| Return Loss                          | - 38.7 dB                      |

### Antenna Parameters with Body TSL

|                                      |                                |
|--------------------------------------|--------------------------------|
| Impedance, transformed to feed point | 46.8 $\Omega$ - 0.4 j $\Omega$ |
| Return Loss                          | - 29.5 dB                      |

### General Antenna Parameters and Design

|                                  |          |
|----------------------------------|----------|
| Electrical Delay (one direction) | 1.217 ns |
|----------------------------------|----------|

After long term use with 100W radiated power, only a slight warming of the dipole near the feedpoint can be measured.

The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals. On some of the dipoles, small end caps are added to the dipole arms in order to improve matching when loaded according to the position as explained in the "Measurement Conditions" paragraph. The SAR data are not affected by this change. The overall dipole length is still according to the Standard.

No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feedpoint may be damaged.

### Additional EUT Data

|                 |       |
|-----------------|-------|
| Manufactured by | SPEAG |
|-----------------|-------|

## DASY5 Validation Report for Head TSL

Date: 15.03.2022

Test Laboratory: SPEAG, Zurich, Switzerland

**DUT: Dipole 1750 MHz; Type: D1750V2; Serial: D1750V2 - SN:1089**

Communication System: UID 0 - CW; Frequency: 1750 MHz

Medium parameters used:  $f = 1750$  MHz;  $\sigma = 1.35$  S/m;  $\epsilon_r = 40$ ;  $\rho = 1000$  kg/m<sup>3</sup>

Phantom section: Flat Section

Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2011)

DASY52 Configuration:

- Probe: EX3DV4 - SN7349; ConvF(8.67, 8.67, 8.67) @ 1750 MHz; Calibrated: 31.12.2021
- Sensor-Surface: 1.4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn601; Calibrated: 01.11.2021
- Phantom: Flat Phantom 5.0 (front); Type: QD 000 P50 AA; Serial: 1001
- DASY52 52.10.4(1535); SEMCAD X 14.6.14(7501)

### Dipole Calibration for Head Tissue/Pin=250 mW, d=10mm/Zoom Scan (7x7x7)/Cube 0:

Measurement grid: dx=5mm, dy=5mm, dz=5mm

Reference Value = 106.2 V/m; Power Drift = 0.06 dB


Peak SAR (extrapolated) = 17.1 W/kg

**SAR(1 g) = 9.19 W/kg; SAR(10 g) = 4.84 W/kg**

Smallest distance from peaks to all points 3 dB below = 10 mm


Ratio of SAR at M2 to SAR at M1 = 54.2%

Maximum value of SAR (measured) = 14.2 W/kg

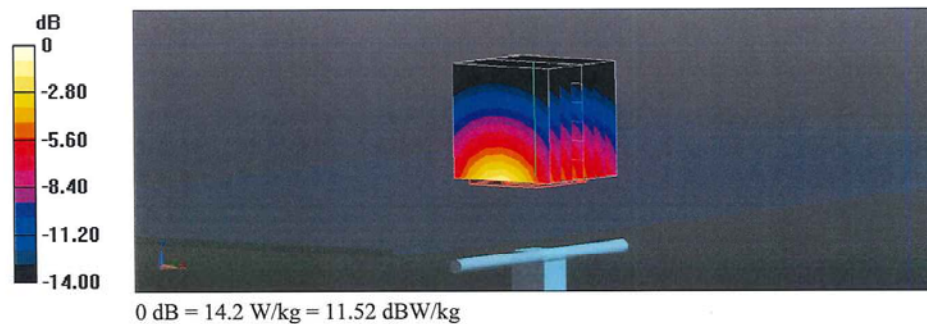



## Impedance Measurement Plot for Head TSL

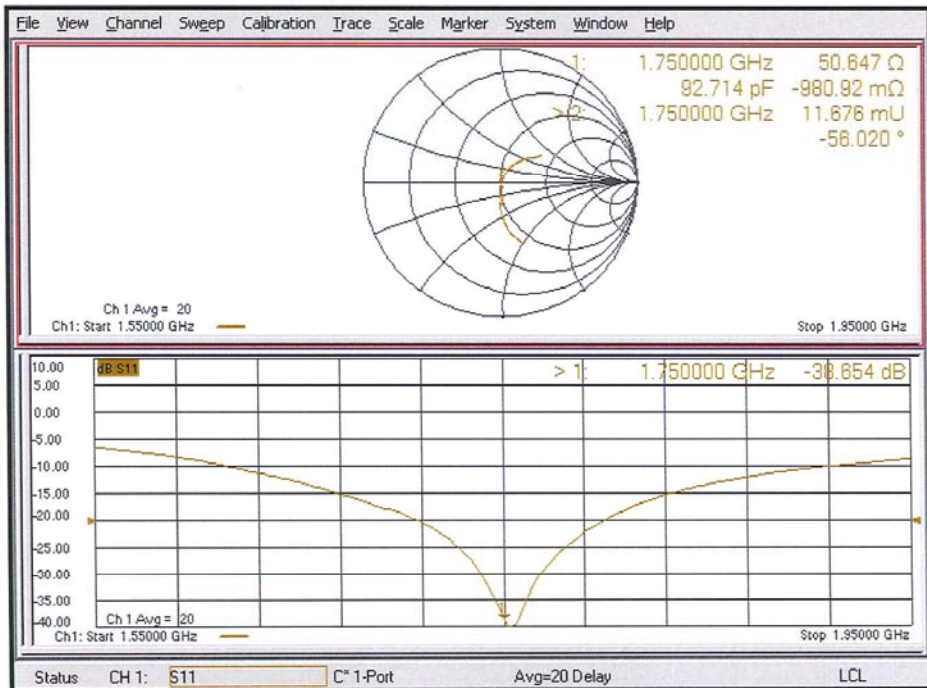

## DASY5 Validation Report for Body TSL

Date: 15.03.2022

Test Laboratory: SPEAG, Zurich, Switzerland

**DUT: Dipole 1750 MHz; Type: D1750V2; Serial: D1750V2 - SN:1089**

Communication System: UID 0 - CW; Frequency: 1750 MHz

Medium parameters used:  $f = 1750$  MHz;  $\sigma = 1.48$  S/m;  $\epsilon_r = 53.4$ ;  $\rho = 1000$  kg/m<sup>3</sup>

Phantom section: Flat Section

Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2011)

DASY52 Configuration:

- Probe: EX3DV4 - SN7349; ConvF(8.48, 8.48, 8.48) @ 1750 MHz; Calibrated: 31.12.2021
- Sensor-Surface: 1.4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn601; Calibrated: 01.11.2021
- Phantom: Flat Phantom 5.0 (back); Type: QD 000 P50 AA; Serial: 1002
- DASY52 52.10.4(1535); SEMCAD X 14.6.14(7501)

### Dipole Calibration for Body Tissue/Pin=250 mW, d=10mm/Zoom Scan (7x7x7)/Cube 0:

Measurement grid: dx=5mm, dy=5mm, dz=5mm

Reference Value = 102.8 V/m; Power Drift = -0.01 dB


Peak SAR (extrapolated) = 16.7 W/kg

**SAR(1 g) = 9.24 W/kg; SAR(10 g) = 4.90 W/kg**


Smallest distance from peaks to all points 3 dB below = 10 mm

Ratio of SAR at M2 to SAR at M1 = 56.3%

Maximum value of SAR (measured) = 14.1 W/kg

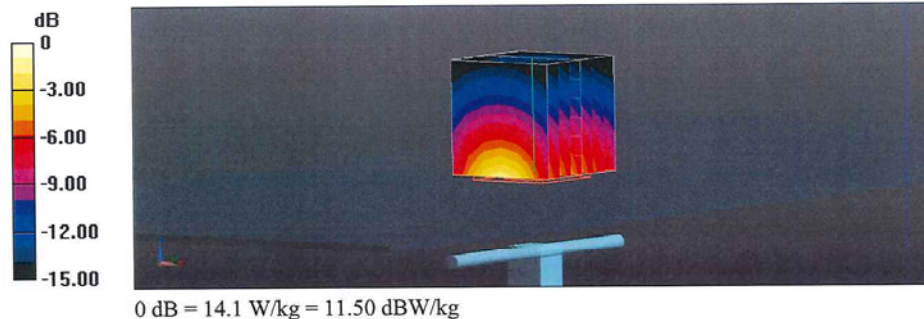

## Impedance Measurement Plot for Body TSL

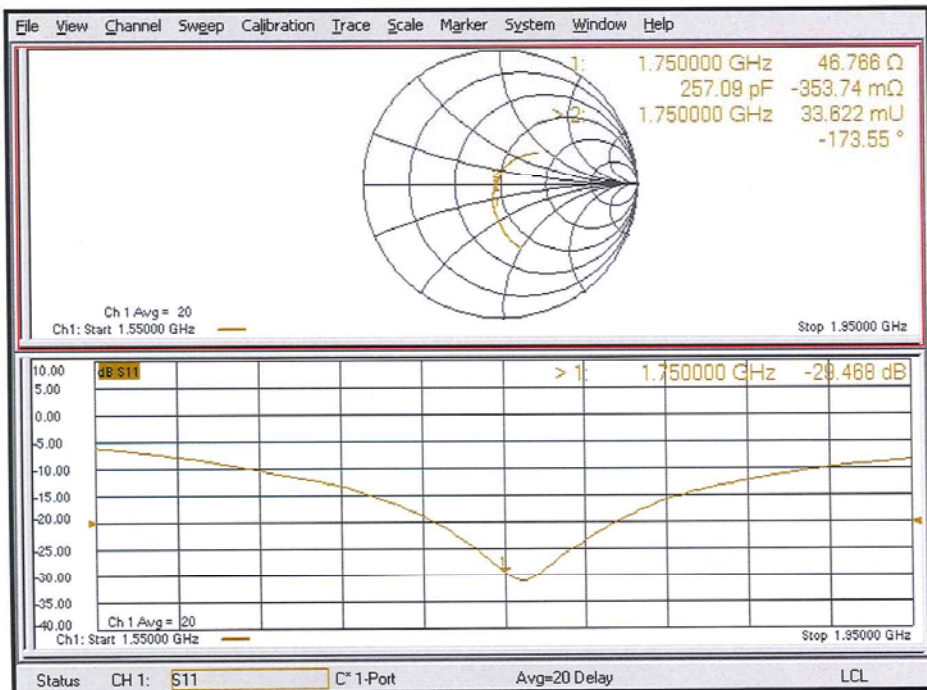

**Calibration for Impedance and Return-loss**

|             |                                 |        |         |
|-------------|---------------------------------|--------|---------|
| Equipment   | Dipole Antenna                  | Model  | D1750V2 |
| Manufacture | Schmid & Partner Engineering AG | Serial | 1089    |
| Tested by   | Hisayoshi Sato in 2023          |        |         |
| Tested by   | Tomohisa Nakagawa in 2024       |        |         |

**1. Test environment**

|                     |                |                   |        |
|---------------------|----------------|-------------------|--------|
| Date                | March 30, 2023 |                   |        |
| Ambient Temperature | 24.0 deg.C     | Relative humidity | 40 %RH |
| Date                | March 12, 2024 |                   |        |
| Ambient Temperature | 24.0 deg.C     | Relative humidity | 40 %RH |

**2. Equipment used**

| LIMS ID      | Description            | Manufacturer                    | Model           | Serial        | Last Cal Date | Interval |
|--------------|------------------------|---------------------------------|-----------------|---------------|---------------|----------|
| Used in 2023 |                        |                                 |                 |               |               |          |
| 88581        | Thermo-Hygrometer      | CUSTOM. Inc                     | CTH-201         | -             | 2022/07/03    | 12       |
| 176484       | Head Simulating Liquid | Schmid & Partner Engineering AG | HBBL600-10000V6 | SL AAH U16 BC | -             | -        |
| 150815       | Network Analyzer       | Keysight Technologies Inc       | E5071C          | MY46523746    | 2022/08/23    | 12       |
| 141991       | 2.4mm Calibration Kit  | Keysight Technologies Inc       | 85056A          | MY44300225    | 2022/08/18    | 12       |
| 142060       | SAM Phantom            | Schmid & Partner Engineering AG | QD000P40CB      | 1333          | 2022/05/23    | 12       |
| Used in 2024 |                        |                                 |                 |               |               |          |
| 176484       | Head Simulating Liquid | Schmid & Partner Engineering AG | HBBL600-10000V6 | SL AAH U16 BC | -             | -        |
| 150815       | Network Analyzer       | Keysight Technologies Inc       | E5071C          | MY46523746    | 2023/08/11    | 12       |
| 88581        | Thermo-Hygrometer      | CUSTOM. Inc                     | CTH-201         | -             | 2023/07/18    | 12       |
| 142056       | 2mm Oval Flat Phantom  | Schmid & Partner Engineering AG | QDOVA001BB      | 1045          | 2023/05/10    | 12       |
| 150816       | Calibration Kit        | Keysight Technologies Inc       | 85032F          | MY53200995    | 2023/08/17    | 12       |

**3. Test Result (Head condition only)**


| Impedance, Transformed to feed point | cal day   | Head (real part) [Ω] | Head (img part) [jΩ] | Deviation (real part) [Ω] | Deviation (img part) [jΩ] | Tolerance        | Result   |
|--------------------------------------|-----------|----------------------|----------------------|---------------------------|---------------------------|------------------|----------|
| Calibration (SPEAG)                  | 2022/3/15 | 50.65                | -0.98                | -                         | -                         | -                | -        |
| Calibration(ULJ)                     | 2023/3/30 | 49.49                | -1.52                | -1.16                     | -0.54                     | +/- 5 Ω +/- 5 jΩ | Complied |
| Calibration(ULJ)                     | 2024/3/12 | 47.16                | -2.38                | -3.49                     | -1.40                     | +/- 5 Ω +/- 5 jΩ | Complied |

| Return loss         | cal day   | Head [dB] | Deviation [%] | Deviation [dB] | Tolerance [%] | Tolerance [+/- dB] | Result   |
|---------------------|-----------|-----------|---------------|----------------|---------------|--------------------|----------|
| Calibration (SPEAG) | 2022/3/15 | -38.65    | -             | -              | -             | -                  | -        |
| Calibration(ULJ)    | 2023/3/30 | -35.76    | 7.49          | 2.89           | +/- 20.00     | 7.73               | Complied |
| Calibration(ULJ)    | 2024/3/12 | -34.78    | 3.88          | 3.88           | +/- 20.00     | 7.73               | Complied |


Tolerance: According to the KDB 865664 D1

## Measurement Plots

### <Head Liquid> in 2023

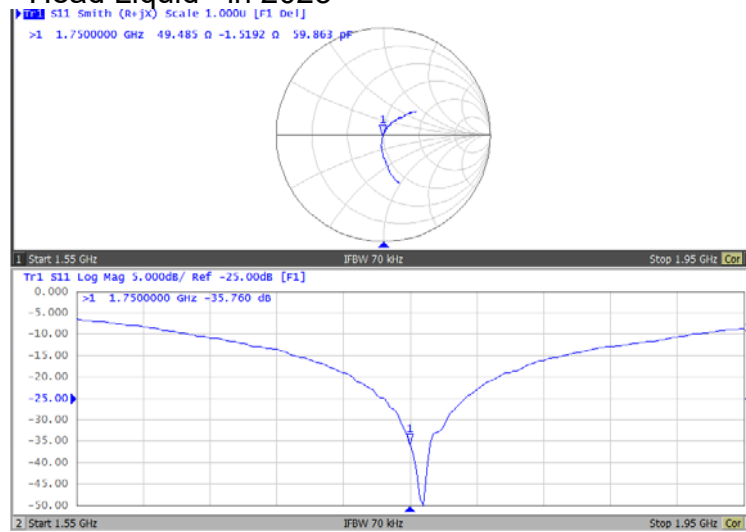

### <Head Liquid> in 2024

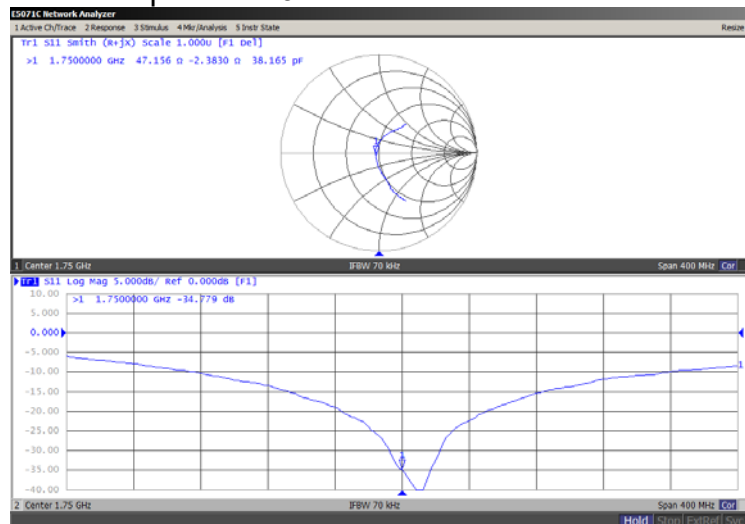

F.6 System Check Dipole SAR Calibration Certificate -DipoleD1900 (D1900V2 S/N: 5d169)

**Calibration Laboratory of**  
**Schmid & Partner**  
**Engineering AG**  
 Zeughausstrasse 43, 8004 Zurich, Switzerland



**S** Schweizerischer Kalibrierdienst  
**C** Service suisse d'étalonnage  
**S** Servizio svizzero di taratura  
**S** Swiss Calibration Service

Accredited by the Swiss Accreditation Service (SAS)  
 The Swiss Accreditation Service is one of the signatories to the EA  
 Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: **SCS 0108**

Client **UL Japan Head Office (RCC)**

Certificate No: **D1900V2-5d169\_Mar22**

## CALIBRATION CERTIFICATE

Object **D1900V2 - SN:5d169**

Calibration procedure(s) **QA CAL-05.v11**  
**Calibration Procedure for SAR Validation Sources between 0.7-3 GHz**

Calibration date: **March 15, 2022**

This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI).  
 The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility: environment temperature ( $22 \pm 3$ °C) and humidity < 70%.

Calibration Equipment used (M&TE critical for calibration)

| Primary Standards               | ID #               | Cal Date (Certificate No.)        | Scheduled Calibration  |
|---------------------------------|--------------------|-----------------------------------|------------------------|
| Power meter NRP                 | SN: 104778         | 09-Apr-21 (No. 217-03291/03292)   | Apr-22                 |
| Power sensor NRP-Z91            | SN: 103244         | 09-Apr-21 (No. 217-03291)         | Apr-22                 |
| Power sensor NRP-Z91            | SN: 103245         | 09-Apr-21 (No. 217-03292)         | Apr-22                 |
| Reference 20 dB Attenuator      | SN: BH9394 (20k)   | 09-Apr-21 (No. 217-03343)         | Apr-22                 |
| Type-N mismatch combination     | SN: 310982 / 06327 | 09-Apr-21 (No. 217-03344)         | Apr-22                 |
| Reference Probe EX3DV4          | SN: 7349           | 31-Dec-21 (No. EX3-7349_Dec21)    | Dec-22                 |
| DAE4                            | SN: 601            | 01-Nov-21 (No. DAE4-601_Nov21)    | Nov-22                 |
| Secondary Standards             | ID #               | Check Date (in house)             | Scheduled Check        |
| Power meter E4419B              | SN: GB39512475     | 30-Oct-14 (in house check Oct-20) | In house check: Oct-22 |
| Power sensor HP 8481A           | SN: US37292783     | 07-Oct-15 (in house check Oct-20) | In house check: Oct-22 |
| Power sensor HP 8481A           | SN: MY41093315     | 07-Oct-15 (in house check Oct-20) | In house check: Oct-22 |
| RF generator R&S SMT-06         | SN: 100972         | 15-Jun-15 (in house check Oct-20) | In house check: Oct-22 |
| Network Analyzer Agilent E8358A | SN: US41080477     | 31-Mar-14 (in house check Oct-20) | In house check: Oct-22 |

|                | Name               | Function              | Signature |
|----------------|--------------------|-----------------------|-----------|
| Calibrated by: | Aidonia Georgiadou | Laboratory Technician |           |
| Approved by:   | Sven Kühn          | Deputy Manager        |           |

Issued: March 15, 2022

This calibration certificate shall not be reproduced except in full without written approval of the laboratory.



**Calibration Laboratory of  
Schmid & Partner  
Engineering AG**  
Zeughausstrasse 43, 8004 Zurich, Switzerland



**S** Schweizerischer Kalibrierdienst  
**C** Service suisse d'étalonnage  
**S** Servizio svizzero di taratura  
**S** Swiss Calibration Service

Accredited by the Swiss Accreditation Service (SAS)  
The Swiss Accreditation Service is one of the signatories to the EA  
Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: **SCS 0108**

**Glossary:**

|       |                                 |
|-------|---------------------------------|
| TSL   | tissue simulating liquid        |
| ConvF | sensitivity in TSL / NORM x,y,z |
| N/A   | not applicable or not measured  |

**Calibration is Performed According to the Following Standards:**

- IEC/IEEE 62209-1528, "Measurement Procedure For The Assessment Of Specific Absorption Rate Of Human Exposure To Radio Frequency Fields From Hand-Held And Body-Worn Wireless Communication Devices - Part 1528: Human Models, Instrumentation And Procedures (Frequency Range of 4 MHz to 10 GHz)", October 2020.
- KDB 865664, "SAR Measurement Requirements for 100 MHz to 6 GHz"

**Additional Documentation:**

- DASY System Handbook

**Methods Applied and Interpretation of Parameters:**

- Measurement Conditions:** Further details are available from the Validation Report at the end of the certificate. All figures stated in the certificate are valid at the frequency indicated.
- Antenna Parameters with TSL:** The source is mounted in a touch configuration below the center marking of the flat phantom.
- Return Loss:** This parameter is measured with the source positioned under the liquid filled phantom (as described in the measurement condition clause). The Return Loss ensures low reflected power. No uncertainty required.
- SAR measured:** SAR measured at the stated antenna input power.
- SAR normalized:** SAR as measured, normalized to an input power of 1 W at the antenna connector.
- SAR for nominal TSL parameters:** The measured TSL parameters are used to calculate the nominal SAR result.

The reported uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor  $k=2$ , which for a normal distribution corresponds to a coverage probability of approximately 95%.



### Measurement Conditions

DASY system configuration, as far as not given on page 1.

|                              |                        |             |
|------------------------------|------------------------|-------------|
| DASY Version                 | DASY52                 | V52.10.4    |
| Extrapolation                | Advanced Extrapolation |             |
| Phantom                      | Modular Flat Phantom   |             |
| Distance Dipole Center - TSL | 10 mm                  | with Spacer |
| Zoom Scan Resolution         | dx, dy, dz = 5 mm      |             |
| Frequency                    | 1900 MHz $\pm$ 1 MHz   |             |

### Head TSL parameters

The following parameters and calculations were applied.

|                                         | Temperature         | Permittivity   | Conductivity         |
|-----------------------------------------|---------------------|----------------|----------------------|
| Nominal Head TSL parameters             | 22.0 °C             | 40.0           | 1.40 mho/m           |
| Measured Head TSL parameters            | (22.0 $\pm$ 0.2) °C | 39.4 $\pm$ 6 % | 1.40 mho/m $\pm$ 6 % |
| Head TSL temperature change during test | < 0.5 °C            | ---            | ---                  |

### SAR result with Head TSL

|                                                       |                    |                                                |
|-------------------------------------------------------|--------------------|------------------------------------------------|
| SAR averaged over 1 cm <sup>3</sup> (1 g) of Head TSL | Condition          |                                                |
| SAR measured                                          | 250 mW input power | 9.89 W/kg                                      |
| SAR for nominal Head TSL parameters                   | normalized to 1W   | <b>39.4 W/kg <math>\pm</math> 17.0 % (k=2)</b> |

|                                                         |                    |                                                |
|---------------------------------------------------------|--------------------|------------------------------------------------|
| SAR averaged over 10 cm <sup>3</sup> (10 g) of Head TSL | condition          |                                                |
| SAR measured                                            | 250 mW input power | 5.13 W/kg                                      |
| SAR for nominal Head TSL parameters                     | normalized to 1W   | <b>20.5 W/kg <math>\pm</math> 16.5 % (k=2)</b> |

### Body TSL parameters

The following parameters and calculations were applied.

|                                         | Temperature         | Permittivity   | Conductivity         |
|-----------------------------------------|---------------------|----------------|----------------------|
| Nominal Body TSL parameters             | 22.0 °C             | 53.3           | 1.52 mho/m           |
| Measured Body TSL parameters            | (22.0 $\pm$ 0.2) °C | 53.1 $\pm$ 6 % | 1.50 mho/m $\pm$ 6 % |
| Body TSL temperature change during test | < 0.5 °C            | ---            | ---                  |

### SAR result with Body TSL

|                                                       |                    |                                                |
|-------------------------------------------------------|--------------------|------------------------------------------------|
| SAR averaged over 1 cm <sup>3</sup> (1 g) of Body TSL | Condition          |                                                |
| SAR measured                                          | 250 mW input power | 10.0 W/kg                                      |
| SAR for nominal Body TSL parameters                   | normalized to 1W   | <b>40.4 W/kg <math>\pm</math> 17.0 % (k=2)</b> |

|                                                         |                    |                                                |
|---------------------------------------------------------|--------------------|------------------------------------------------|
| SAR averaged over 10 cm <sup>3</sup> (10 g) of Body TSL | condition          |                                                |
| SAR measured                                            | 250 mW input power | 5.21 W/kg                                      |
| SAR for nominal Body TSL parameters                     | normalized to 1W   | <b>20.9 W/kg <math>\pm</math> 16.5 % (k=2)</b> |

---

## Appendix (Additional assessments outside the scope of SCS 0108)

### Antenna Parameters with Head TSL

|                                      |                             |
|--------------------------------------|-----------------------------|
| Impedance, transformed to feed point | $54.5 \Omega + 4.9 j\Omega$ |
| Return Loss                          | - 23.9 dB                   |

### Antenna Parameters with Body TSL

|                                      |                             |
|--------------------------------------|-----------------------------|
| Impedance, transformed to feed point | $48.5 \Omega + 5.2 j\Omega$ |
| Return Loss                          | - 25.2 dB                   |

### General Antenna Parameters and Design

|                                  |          |
|----------------------------------|----------|
| Electrical Delay (one direction) | 1.204 ns |
|----------------------------------|----------|

After long term use with 100W radiated power, only a slight warming of the dipole near the feedpoint can be measured.

The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals. On some of the dipoles, small end caps are added to the dipole arms in order to improve matching when loaded according to the position as explained in the "Measurement Conditions" paragraph. The SAR data are not affected by this change. The overall dipole length is still according to the Standard.

No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feedpoint may be damaged.

### Additional EUT Data

|                 |       |
|-----------------|-------|
| Manufactured by | SPEAG |
|-----------------|-------|