

Product: RIGHTEST Continuous Glucose Monitoring System (CGMS)

Type Identification: HM312

Photograph 1: Test Setup for Spurious Emissions (Front View 1)




Photograph 2: Test Setup for Spurious Emissions (Front View 2)




Product: RIGHTEST Continuous Glucose Monitoring System (CGMS)

Type Identification: HM312

Photograph 3: Test Setup for Spurious Emissions (Back View 1)

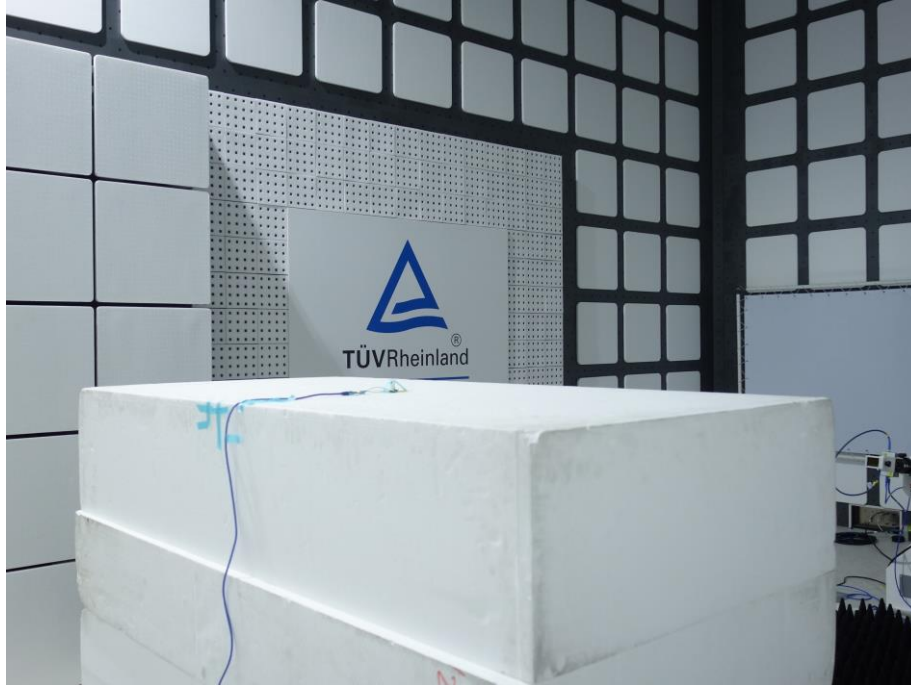


Photograph 4: Test Setup for Spurious Emissions (Back View 2)

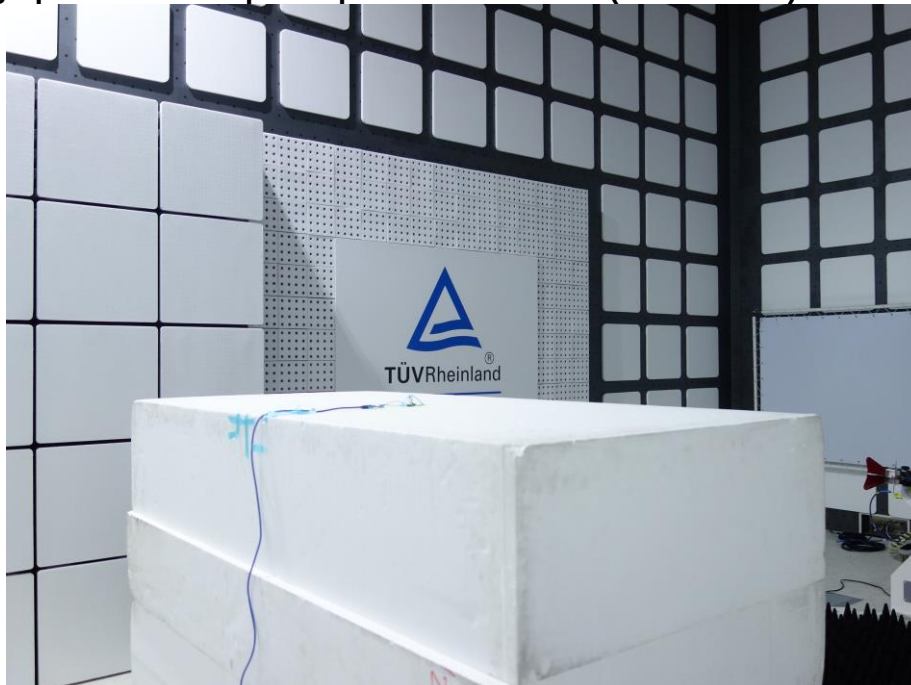


Product: RIGHTEST Continuous Glucose Monitoring System (CGMS)

Type Identification: HM312

Photograph 5: Test Setup for Spurious Emissions (Back View 3)

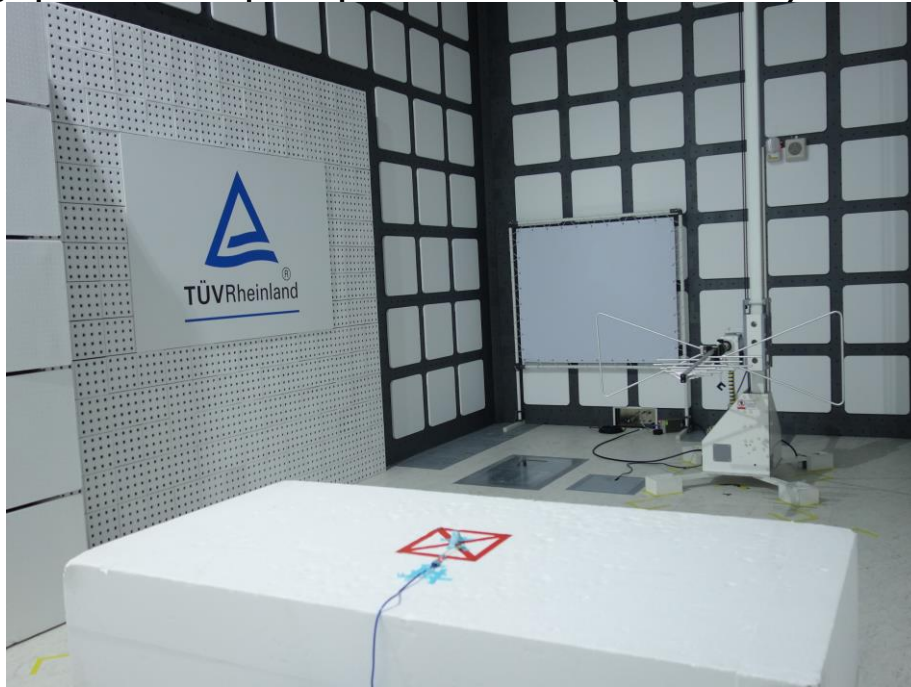

Photograph 6: Test Setup for Spurious Emissions (Back View 4)

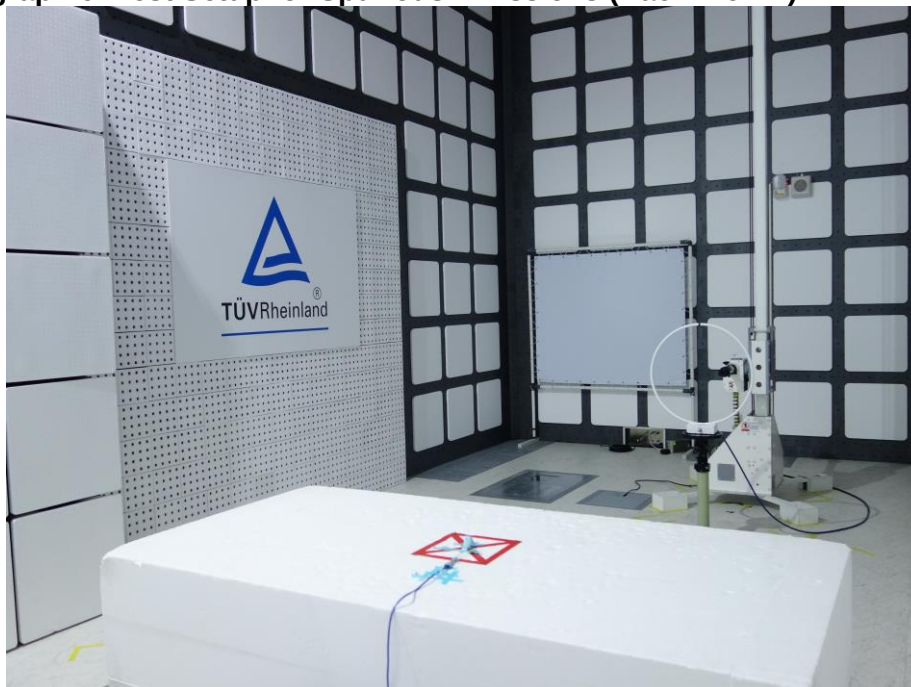

Product: RIGHTEST Continuous Glucose Monitoring System (CGMS)

Type Identification: HM312

Photograph 7: Test Setup for Mains Conducted Emissions (Front View)



Photograph 8: Test Setup for Mains Conducted Emissions (Back View)



Product: RIGHTEST Continuous Glucose Monitoring System (CGMS)

Type Identification: HM312

Support Unit

