

Test Laboratory: The name of your organization

D5GHzV2_M5200_031204

DUT: Dipole 5200-5800MHz; Type: D5GHzV2; Serial: 1003

Ambient temperature = 25.5 deg. C; Liquid temperature = 24.5 deg. C

Communication System: CW 5200MHz; Frequency: 5200 MHz; Duty Cycle: 1:1

Medium parameters used: $f = 5200$ MHz; $\sigma = 5.43$ mho/m; $\epsilon_r = 49$; $\rho = 1000$ kg/m³

Phantom section: Flat Section

Measurement Standard: DASY4 (High Precision Assessment)

DASY4 Configuration:

- Probe: ES3DV2 - SN3021; ConvF(1.4, 1.4, 1.4); Calibrated: 7/29/2003
- Sensor-Surface: 3mm (Mechanical Surface Detection)
- Electronics: DAE3 Sn500; Calibrated: 12/23/2003
- Phantom: SAM 2; Type: SAM 2; Serial: 1050
- Measurement SW: DASY4, V4.2 Build 37; Postprocessing SW: SEMCAD, V1.8 Build 109

d=10mm, Pin=250mW/Area Scan (8x8x1): Measurement grid: dx=10mm, dy=10mm

Reference Value = 85.5 V/m; Power Drift = -0.1 dB

Maximum value of SAR (measured) = 25.6 mW/g


d=10mm, Pin=250mW/Zoom Scan (7x7x8)/Cube 0: Measurement grid: dx=4.3mm, dy=4.3mm, dz=3mm

Reference Value = 85.5 V/m; Power Drift = -0.1 dB

Maximum value of SAR (measured) = 33.5 mW/g

Peak SAR (extrapolated) = 85.4 W/kg

SAR(1 g) = 22.3 mW/g; SAR(10 g) = 6.25 mW/g

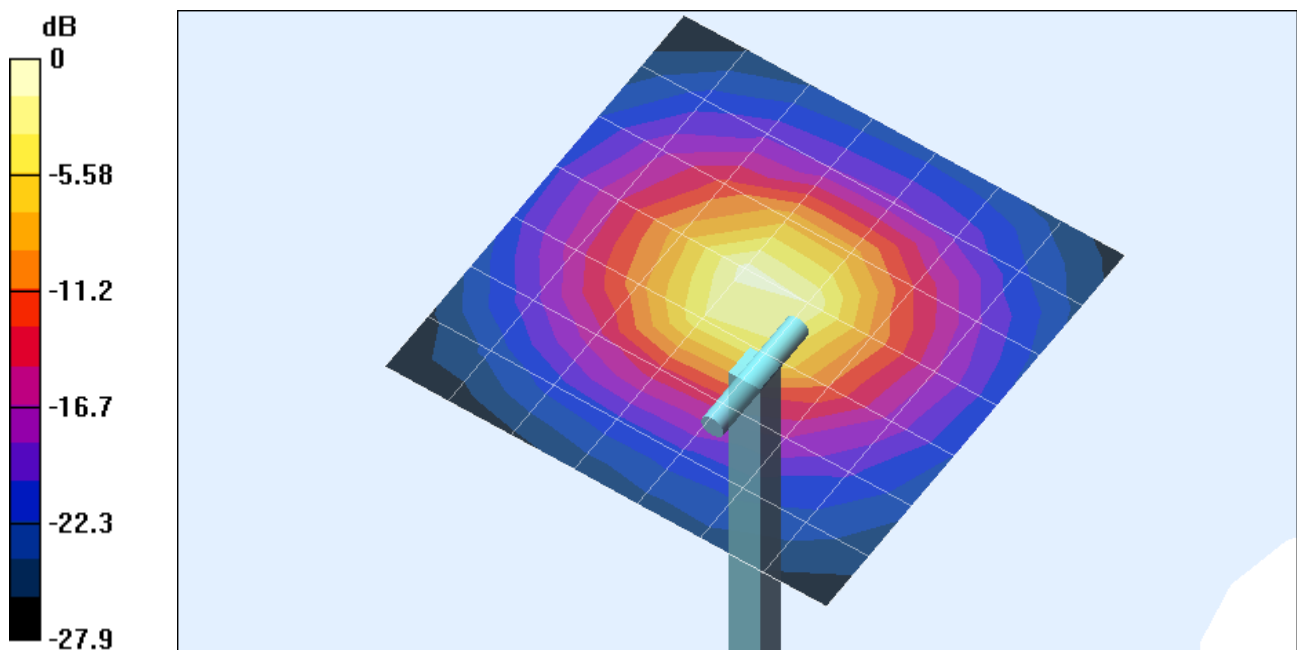

0 dB = 33.5mW/g

Test Laboratory: The name of your organization

D5GHzV2_M5200_031204

DUT: Dipole 5200-5800MHz; Type: D5GHzV2; Serial: 1003

DASY4 Configuration:

- Probe: ES3DV2 - SN3021; ConvF(1.4, 1.4, 1.4); Calibrated: 7/29/2003
- Sensor-Surface: 0mm (Fix Surface)
- Electronics: DAE3 Sn500; Calibrated: 12/23/2003
- Phantom: SAM 2; Type: SAM 2; Serial: 1050
- Measurement SW: DASY4, V4.2 Build 37; Postprocessing SW: SEMCAD, V1.8 Build 109

d=10mm, Pin=250mW 2/Z Scan (1x1x41): Measurement grid: dx=20mm, dy=20mm, dz=2.5mm
 Reference Value = 92.5 V/m; Power Drift = -0.1 dB
 Maximum value of SAR (measured) = 16 mW/g

