

Appendix C for KSCR221000194501

Calibration Certificate

Object	Apply	No	Model	SN	Calibration Date
Dipole	☐	1	CLA150	4025	2021/04/26
	☐	2	D450V3	1103	2021/04/21
	☐	3	D750V3	1188	2022/03/29
	☐	4	D835V2	4d114	2022/03/31
	☐	5	D900V2	1d079	2022/06/07
	☐	6	D1800V2	2d170	2022/03/31
	☐	7	D1900V2	5d1136	2022/06/07
	☐	8	D2000V2	1041	2022/06/06
	☐	9	D2300V2	1096	2022/03/31
	☒	10	D2450V2	817	2022/04/01
	☐	11	D2600V2	1158	2022/03/31
	☐	12	D5GHzV2	1095	2022/06/01
DAE	☒	13	DAE4	1245	2022/05/30
Probe	☒	14	EX3DV4	7346	2022/03/30



Unless otherwise agreed in writing, this document is issued by the Company subject to its General Conditions of Service printed overleaf, available on request or accessible at <http://www.sgs.com/en/Terms-and-Conditions.aspx> and, for electronic format documents, subject to Terms and Conditions for Electronic Documents at <http://www.sgs.com/en/Terms-and-Conditions/Terms-e-Documents.aspx>. Attention is drawn to the limitation of liability, indemnification and jurisdiction issues defined therein. Any holder of this document is advised that information contained hereon reflects the Company's findings at the time of its intervention only and within the limits of Client's instructions, if any. The Company's sole responsibility is to its Client and this document does not exonerate parties to a transaction from exercising all their rights and obligations under the transaction documents. This document cannot be reproduced except in full, without prior written approval of the Company. Any unauthorized alteration, forgery or falsification of the content or appearance of this document is unlawful and offenders may be prosecuted to the fullest extent of the law. Unless otherwise stated the results shown in this test report refer only to the sample(s) tested and such sample(s) are retained for 30 days only.

Attention: To check the authenticity of testing / inspection report & certificate, please contact us at telephone: (86-755) 8307 1443, or email: CN.Doccheck@sgs.com

No.10, Weiye Road, Innovation Park, Kunshan, Jiangsu, China 215300
中国·江苏·昆山市留学院创业园伟业路10号 邮编 215300

t(86-512)57355888 f(86-512)57370818 www.sgsgroup.com.cn
t(86-512)57355888 f(86-512)57370818 sgs.china@sgs.com

1 Dipole

1.1 CLA150 - SN 4025

Calibration Laboratory of Schmid & Partner Engineering AG Zugstrasse 43, 8004 Zurich, Switzerland		S Schweizerischer Kalibrierdienst Service suisse d'étalonnage Servizio svizzero di taratura S Swiss Calibration Service	
Accredited by the Swiss Accreditation Service (SAS) The Swiss Accreditation Service is one of the signatories to the EA Multilateral Agreement for the recognition of calibration certificates		Accreditation No.: SCS 0108	
Client: SGS-CN (Audeon)		Certificate No.: CLA150-4025_Apr21	
CALIBRATION CERTIFICATE			
Object: CLA150 - SN: 4025			
Calibration procedure(s): QA CAL-15.v9 Calibration Procedure for SAR Validation Sources below 700 MHz			
Calibration date: April 26, 2021			
The calibration certificate documents the traceability to national standards, which require the physical units of measurements (SI). The measurements and the uncertainties with confidence probability are given on the following pages and part of the certificate.			
All calibrations have been conducted in the closed laboratory facility; environment temperature (22 ± 3)°C and humidity < 70%.			
Calibration Equipment Used (M&E critical for calibration)			
Primary Standards	ID #	Cal Date (Certificate No.)	Scheduled Calibration
Power meter NRP	SN: 10475	06-Apr-21 (No. 217-03001/03002)	Apr-22
Power sensor NRP Z01	SN: 103844	06-Apr-21 (No. 217-03001)	Apr-22
Power sensor NRP Z01	SN: 103845	06-Apr-21 (No. 217-03002)	Apr-22
Reference 20 dB Attenuator	SN: C23602 (C03)	06-Apr-21 (No. 217-03003)	Apr-22
Type-N mismatch combination	SN: 310907 / 0007	06-Apr-21 (No. 217-03004)	Apr-22
Reference Probe EX3004	SN: 3877	30-Dec-20 (No. 203-3077_Dec20)	Dec-21
EXE4	SN: 661	16-Jan-20 (No. 19459-659_Jan20)	Jan-21
Secondary Standards	ID #	Check Date (in house)	Scheduled Check
Power meter S44195	SN: G341303024	06-Apr-15 (in house check Jun-20)	In house check Jun-20
Power sensor E413A	SN: MY4169007	06-Apr-15 (in house check Jun-20)	In house check Jun-20
Power sensor E413A	SN: 00010210	06-Apr-15 (in house check Jun-20)	In house check Jun-20
RF generator HP 8594C	SN: U504001709	04-Aug-19 (in house check Jun-20)	In house check Jun-20
Network Analyser Agilent T8368A	SN: U541000477	31-Mar-14 (in house check Oct-19)	In house check Oct-19
Calibrated by:	Janina Jathay Katsaros	Function: Laboratory Technician	Signature:
Approved by:	Kajko Polovic	Technical Manager	Signature:
This calibration certificate shall not be reproduced except in full without written approval of the laboratory.			
Issued: April 26, 2021			
Certificate No: CLA150-4025_Apr21		Page 1 of 5	

Calibration Laboratory of Schmid & Partner Engineering AG Zugstrasse 43, 8004 Zurich, Switzerland		S Schweizerischer Kalibrierdienst Service suisse d'étalonnage Servizio svizzero di taratura S Swiss Calibration Service	
Accredited by the Swiss Accreditation Service (SAS) The Swiss Accreditation Service is one of the signatories to the EA Multilateral Agreement for the recognition of calibration certificates		Accreditation No.: SCS 0108	
Glossary:			
TSL	Issue simulating liquid		
ConvF	sensitivity in TSL / NORM x,y,z		
N/A	not applicable or not measured		
Calibration is Performed According to the Following Standards:			
a) IEEE Std 1528-2013, "IEEE Recommended Practice for Determining the Peak Spatial-Averaged Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Technique", June 2013			
b) IEC 62209-1, "Measurement procedure for the assessment of Specific Absorption Rate (SAR) from hand-held and body-mounted devices used next to the ear (frequency range of 100 MHz to 6 GHz)", July 2016			
c) IEC 62209-2, "Procedure to determine the Specific Absorption Rate (SAR) for wireless communication devices used in close proximity to the human body (frequency range of 30 MHz to 6 GHz)", March 2010			
d) KDB 865864, "SAR Measurement Requirements for 100 MHz to 6 GHz"			
Additional Documentation:			
e) DASY4/5 System Handbook			
Methods Applied and Interpretation of Parameters:			
• Measurement Conditions: Further details are available from the Validation Report at the end of the certificate. All figures stated in the certificate are valid at the frequency indicated.			
• Antenna Parameters with TSL: The source is mounted in a touch configuration below the center marking of the flat phantom.			
• Return Loss: This parameter is measured with the source positioned under the liquid filled phantom (as described in the measurement condition clause). The Return Loss ensures low reflected power. No uncertainty required.			
• SAR measured: SAR measured at the stated antenna input power.			
• SAR normalized: SAR as measured, normalized to an input power of 1 W at the antenna connector.			
• SAR for nominal TSL parameters: The measured TSL parameters are used to calculate the nominal SAR result.			
The reported uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor k=2, which for a normal distribution corresponds to a coverage probability of approximately 95%.			
Certificate No: CLA150-4025_Apr21		Page 2 of 5	

Measurement Conditions		
DASY system configuration, as far as not given on page 1.		
DASY Version	DASY5	V52.10.4
Extrapolation	Advanced Extrapolation	
Phantom	ELIA Flat Phantom	Shell thickness: 2 ± 0.2 mm
EUT Positioning	Touch Position	
Zoom Scan Resolution	dx, dy = 4.0 mm, dz = 1.4 mm	Graded Ratio = 1.4 (Z direction)
Frequency	150 MHz ± 1 MHz	

Head TSL parameters			
The following parameters and calculations were applied.			
	Temperature	Permittivity	Conductivity
Nominal Head TSL parameters	22.0 °C	52.3	0.75 mho/m
Measured Head TSL parameters	(22.0 ± 0.2) °C	51.1 ± 6 %	0.75 mho/m ± 6 %
Head TSL temperature change during test	< 0.5 °C	---	---

SAR result with Head TSL		
SAR averaged over 1 cm³ (1 g) of Head TSL	Condition	
SAR measured	1 W input power	3.90 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	3.88 W/kg ± 19.4 % (k=2)
SAR averaged over 10 cm³ (10 g) of Head TSL	condition	
SAR measured	1 W input power	2.60 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	2.59 W/kg ± 18.0 % (k=2)

Appendix (Additional assessments outside the scope of SCS 0108)	
Antenna Parameters with Head TSL	
Impedance, transformed to feed point	47.9 Ω ± 1.5 Ω
Return Loss	-31.4 dB
Additional EUT Data	
Manufactured by	SPLEAG

Certificate No: CLA150-4025_Apr21	
Page 3 of 6	Page 4 of 6




Unless otherwise agreed in writing, this document is issued by the Company subject to its General Conditions of Service printed overleaf, available on request or accessible at <http://www.sgs.com/en/Terms-and-Conditions.aspx> and, for electronic format documents, subject to Terms and Conditions for Electronic Documents at <http://www.sgs.com/en/Terms-and-Conditions/Terms-e-Documents.aspx>. Attention is drawn to the limitation of liability, indemnification and jurisdiction issues defined therein. Any holder of this document is advised that information contained hereon reflects the Company's findings at the time of its intervention only and within the limits of Client's instructions, if any. The Company's sole responsibility is to its Client and this document does not exonerate parties to a transaction from exercising all their rights and obligations under the transaction documents. This document cannot be reproduced except in full, without prior written approval of the Company. Any unauthorized alteration, forgery or falsification of the content or appearance of this document is unlawful and offenders may be prosecuted to the fullest extent of the law. Unless otherwise stated the results shown in this test report refer only to the sample(s) tested and such sample(s) are retained for 30 days only.

Attention: To check the authenticity of testing / inspection report & certificate, please contact us by telephone: (86-755) 8307 1443, or email: CN.Doccheck@sgs.com

No.10, Weiye Road, Innovation Park, Kunshan, Jiangsu, China 215300
中国·江苏·昆山市留学生创业园伟业路10号 邮编 215300

t(86-512)57355888 f(86-512)57370818 www.sgsgroup.com.cn

t(86-512)57355888 f(86-512)57370818 sgs.china@sgs.com

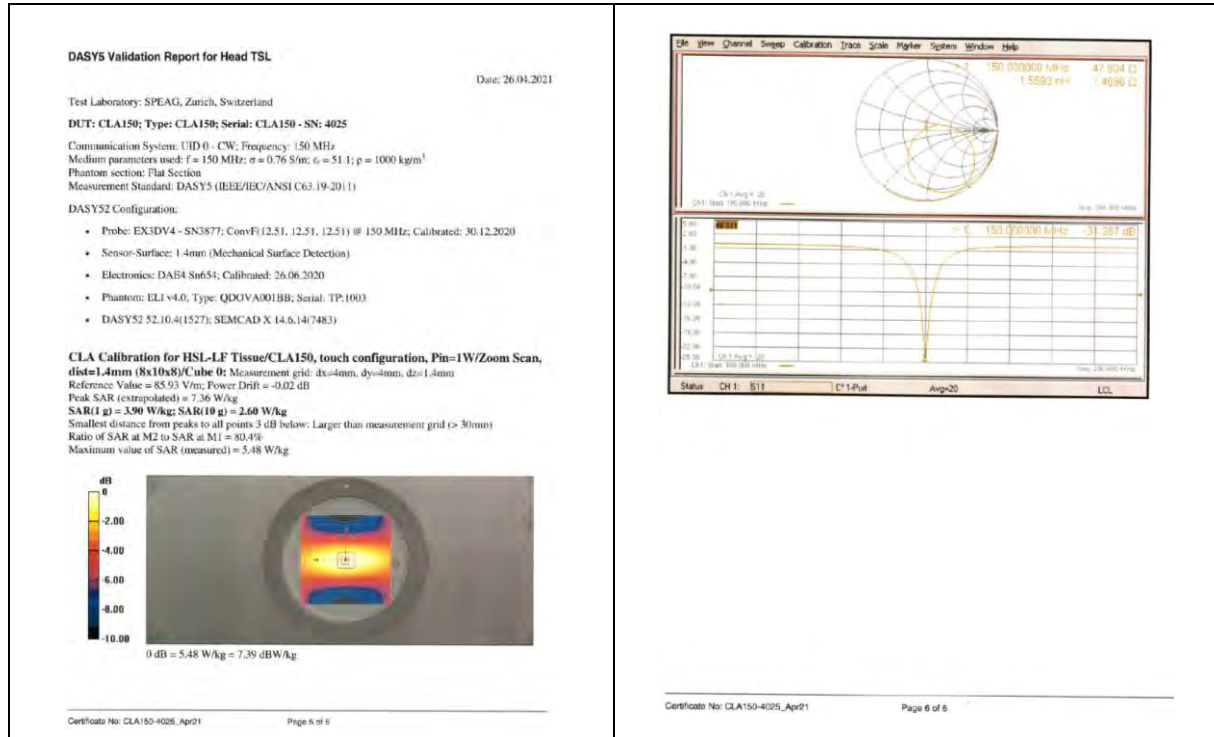

1.2 D450V3 - SN 1103

Calibration Laboratory of Schmid & Partner Engineering AG
Zughestrasse 43, 8004 Zurich, Switzerland

Accredited by the Swiss Accreditation Service (SAS)
The Swiss Accreditation Service is one of the signatories to the EA Multilateral Agreement for the recognition of calibration certificates

Client: **SGS-CN (Aiden)** Certificate No: **D450V3-1103_Apr21**

CALIBRATION CERTIFICATE

Object: **D450V3 - SN: 1103**

Calibration procedure(s): **QA CAL-15-V9**
Calibration Procedure for SAR Validation Sources below 700 MHz

Calibration date: **April 21, 2021**

This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI). The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility: environment temperature (20 ± 2) °C and humidity < 75%.

Calibration Equipment used (MPE critical for calibration)

Primary Standards	ID #	Cal Date (Certificate No.)	Scheduled Calibration
Power meter NRP	SN 104779	09-Apr-21 (No. 217-030110300)	Apr-22
Power sensor MNP-291	SN 103344	09-Apr-21 (No. 217-03011)	Apr-22
Power sensor MNP-291	SN 103345	09-Apr-21 (No. 217-03015)	Apr-22
Reference 20 dB Attenuator	SN C2552 (200)	09-Apr-21 (No. 217-03049)	Apr-22
Type-N impedance calibration	SN 310852 / 06327	09-Apr-21 (No. 217-03044)	Apr-22
Reference Probe EX3DV4	SN 3877	30-Dec-20 (No. EX3-2077 Dec20)	Dec-21
DAEA	SN 454	06-Jun-20 (No. D454-664-Jun20)	Jun-21

Secondary Standards

ID #	Cal Date (In House)	Scheduled Check
Power meter E41188	06-Apr-19 (In house check Jun-20)	In house check Jun-20
Power sensor E4112A	06-Apr-19 (In house check Jun-20)	In house check Jun-20
Power sensor E4112A	06-Apr-19 (In house check Jun-20)	In house check Jun-20
RF generator HP 8448C	06-Aug-19 (In house check Jun-20)	In house check Jun-20
Network Analyzer Agilent E8358A	31-Mar-14 (In house check Dec-20)	In house check Oct-21

Calibrated by: **Kuba Foltsek** Function: **Laboratory Technician**

Approved by: **Kuba Foltsek** Technical Manager

This calibration certificate shall not be reproduced except in full without written approval of the laboratory.

Certificate No: D450V3-1103_Apr21 Page 1 of 6

Calibration Laboratory of Schmid & Partner Engineering AG
Zughestrasse 43, 8004 Zurich, Switzerland

Accredited by the Swiss Accreditation Service (SAS)
The Swiss Accreditation Service is one of the signatories to the EA Multilateral Agreement for the recognition of calibration certificates

Client: **SGS-CN (Aiden)** Certificate No: **D450V3-1103_Apr21**

Glossary:

TSL: Issue simulating liquid sensitivity in TSL / NORM x,y,z

ConvF: not applicable or not measured

N/A: not applicable or not measured

Calibration is Performed According to the Following Standards:

- IEC 61010-1:2013, "IEEE Recommended Practice for Determining the Peak Spatial-Averaged Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques", June 2013
- IEC 62209-1, "Measurement procedure for the assessment of Specific Absorption Rate (SAR) from hand-held and body-mounted devices used next to the ear (frequency range of 300 MHz to 6 GHz)", July 2015
- IEC 62209-2, "Procedure to determine the Specific Absorption Rate (SAR) for wireless communication devices used in close proximity to the human body (frequency range of 30 MHz to 6 GHz)", March 2010
- KDB 665664, "SAR Measurement Requirements for 100 MHz to 6 GHz"

Additional Documentation:

e) DASY4/5 System Handbook

Methods Applied and Interpretation of Parameters:

- Measurement Conditions:** Further details are available from the Validation Report at the end of the certificate. All figures stated in the certificate are valid at the frequency indicated.
- Antenna Parameters with TSL:** The dipole is mounted with the spacer to position its feed point exactly below the center marking of the flat phantom section, with the arms oriented parallel to the body axis.
- Feed Point Impedance and Return Loss:** These parameters are measured with the dipole positioned under the liquid filled phantom. The impedance stated is transformed from the measurement at the SMA connector to the feed point. The Return Loss ensures low reflected power. No uncertainty required.
- Electrical Delay:** One-way delay between the SMA connector and the antenna feed point. No uncertainty required.
- SAR measured:** SAR measured at the stated antenna input power.
- SAR normalized:** SAR as measured, normalized to an input power of 1 W at the antenna connector.
- SAR for nominal TSL parameters:** The measured TSL parameters are used to calculate the nominal SAR result.

The reported uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor k=2, which for a normal distribution corresponds to a coverage probability of approximately 95%.

Certificate No: D450V3-1103_Apr21 Page 2 of 6



Unless otherwise agreed in writing, this document is issued by the Company subject to its General Conditions of Service printed overleaf, available on request or accessible at <http://www.sgs.com/en/Terms-and-Conditions.aspx>; and, for electronic format documents, subject to Terms and Conditions for Electronic Documents at <http://www.sgs.com/en/Terms-and-Conditions/Terms-e-Documents.aspx>. Attention is drawn to the limitation of liability, indemnification and jurisdiction issues defined therein. Any holder of this document is advised that information contained hereon reflects the Company's findings at the time of its intervention only and within the limits of Client's instructions, if any. The Company's sole responsibility is to its Client and this document does not exonerate parties to a transaction from exercising all their rights and obligations under the transaction documents. This document cannot be reproduced except in full, without prior written approval of the Company. Any unauthorized alteration, forgery or falsification of the content or appearance of this document is unlawful and offenders may be prosecuted to the fullest extent of the law. Unless otherwise stated the results shown in this test report refer only to the sample(s) tested and such sample(s) are retained for 30 days only.

Attention: To check the authenticity of testing / inspection report & certificate, please contact us at telephone: (86-755) 8307 1443, or email: CN.Doccheck@sgs.com

No.10, Weyue Road, Innovation Park, Kunshan, Jiangsu, China 215300

中国·江苏·昆山市留学生创业园伟业路10号 邮编 215300

t(86-512)57355888 f(86-512)57370818 www.sgs.com.cn

t(86-512)57355888 f(86-512)57370818 sgs.china@sgs.com

Measurement Conditions		
DASY system configuration, as far as not given on page 1.		
DASY Version	DASY5	V82.10.4
Extrapolation	Advanced Extrapolation	
Phantom	ELJ Flat Phantom	Shell thickness: 2 ± 0.2 mm
Distance Dipole Center - TSL	15 mm	with Spacer
Zoom Scan Resolution	$dx, dy, dz = 5$ mm	
Frequency	450 MHz ± 1 MHz	

Head TSL parameters			
The following parameters and calculations were applied:			
	Temperature	Permittivity	Conductivity
Nominal Head TSL parameters	22.0 °C	43.5	0.57 mho/m
Measured Head TSL parameters	(22.0 $\pm$ 0.2) °C	43.1 $\pm$ 6 %	0.57 mho/m $\pm$ 8 %
Head TSL temperature change during test	< 0.5 °C	---	---

SAR result with Head TSL		
SAR averaged over 1 cm ³ (1 g) of Head TSL	Condition	
SAR measured	250 mW input power	1.14 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	4.55 W/kg $\pm$ 18.1 % (k=2)

SAR result with Head TSL		
SAR averaged over 10 cm ³ (10 g) of Head TSL	Condition	
SAR measured	250 mW input power	0.757 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	3.06 W/kg $\pm$ 17.6 % (k=2)

Appendix (Additional assessments outside the scope of SCS 0108)	
Antenna Parameters with Head TSL	
Impedance, transformed to feed point	57.1 Ω - 2.8 j Ω
Return Loss	-23.0 dB

General Antenna Parameters and Design	
Electrical Delay (one direction)	1.346 ns

After long term use with 100W radiated power, only a slight warming of the dipole near the feedpoint can be measured.

The dipole is made of standard coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC signals. On some of the dipoles, small end caps are added to the dipole arms in order to improve matching when loaded according to the position as explained in the "Measurement Conditions" paragraph. The SAR data are not affected by this change. The overall dipole length is still according to the Standard.

No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feedpoint may be damaged.

Additional EUT Data	
Manufactured by	SPEAG

Certificate No: D450V3-1103_Apr21

Page 5 of 6

Certificate No: D450V3-1103_Apr21

Page 4 of 6

DASY5 Validation Report for Head TSL

Date: 21.04.2021

Test Laboratory: SPEAG, Zurich, Switzerland

DUT: Dipole 450 MHz; Type: D450V3; Serial: D450V3 - SN:1103

Communication System: UTD 0 - CW; Frequency: 450 MHz

Medium parameters used: $f = 450$ MHz, $\alpha = 0.87$ S/m; $\epsilon_r = 43.1$; $\rho = 1000$ kg/m³

Phantom section: Flat Section

Measurement Standard: DASY5 (IEC/IEC/ANSI C63.19-2011)

DASY52 Configuration:

- Probe: EX3DV4 - SN3877; ConvF [10.64, 10.64] @ 450 MHz; Calibrated: 30.12.2020
- Sensor-Surface: 1.4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn654; Calibrated: 26.06.2020
- Phantom: ELJ v4.0; Type: QDOVA001BB; Serial: TP:1003
- DASY52 52.10.4 (1527); SEMCAD X (4.6.14/7483)

Dipole Calibration for Head Tissue/d=15mm, Pin=250mW/Zoom Scan (7x7x7)/Cube 0:

Measurement grid: $dx=5$ mm, $dy=5$ mm, $dz=5$ mm

Reference Value = 39.18 V/m; Power DUT = 0.08 dB


Peak SAR (extrapolated) = 1.76 W/kg

SAR(1 g) = 1.14 W/kg; SAR(10 g) = 0.767 W/kg

Smallest distance from peaks to all points 3 dB below: Larger than measurement grid

Ratio of SAR at M2 to SAR at M1 = 64.9%

Maximum value of SAR (measured) = 1.53 W/kg

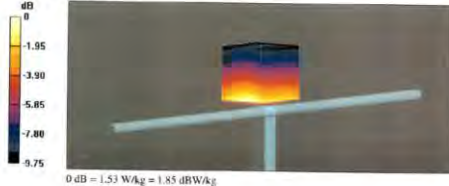


Certificate No: D450V3-1103_Apr21

Page 5 of 6

Certificate No: D450V3-1103_Apr21

Page 6 of 6

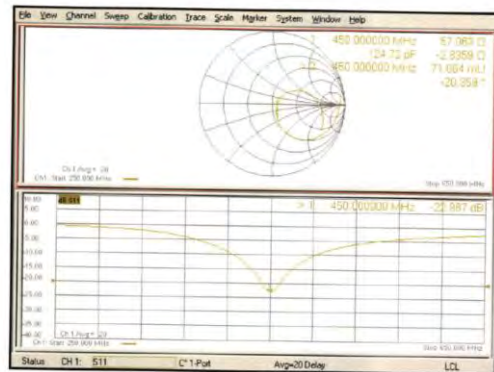

Unless otherwise agreed in writing, this document is issued by the Company subject to its General Conditions of Service printed overleaf, available on request or accessible at <http://www.sgs.com/en/Terms-and-Conditions.aspx> and, for electronic format documents, subject to Terms and Conditions for Electronic Documents at <http://www.sgs.com/en/Terms-and-Conditions/Terms-e-Documents.aspx>. Attention is drawn to the limitation of liability, indemnification and jurisdiction issues defined therein. Any holder of this document is advised that information contained hereon reflects the Company's findings at the time of its intervention only and within the limits of Client's instructions, if any. The Company's sole responsibility is to its Client and this document does not exonerate parties to a transaction from exercising all their rights and obligations under the transaction documents. This document cannot be reproduced except in full, without prior written approval of the Company. Any unauthorized alteration, forgery or falsification of the content or appearance of this document is unlawful and offenders may be prosecuted to the fullest extent of the law. Unless otherwise stated the results shown in this test report refer only to the sample(s) tested and such sample(s) are retained for 30 days only.

Attention: To check the authenticity of testing / inspection report & certificate, please contact us at telephone: (86-755) 8307 1443, or email: CN.Doccheck@sgs.com

No.10, Weiye Road, Innovation Park, Kunshan, Jiangsu, China 215300
中国·江苏·昆山市留学院创业园伟业路10号 邮编 215300

t(86-512)57355888 f(86-512)57370818 www.sgsgroup.com.cn
t(86-512)57355888 f(86-512)57370818 sgs.china@sgs.com

1.3 D750V3 - SN 1188



TTL Speag CALIBRATION LABORATORY		CAICT																																	
Add: No.52 HuaYuanli Road, Haidian District, Beijing, 100191 Tel: +86-10-4239613-2172 Fax: +86-10-4239613-2564 E-mail: cti@china-test.com http://www.china-test.com		Add: No.52 HuaYuanli Road, Haidian District, Beijing, 100191 Tel: +86-10-4239613-2079 Fax: +86-10-4239613-2564 E-mail: cti@china-test.com http://www.china-test.com																																	
Client: SGS-CN		Certificate No.: Z22-60103																																	
CALIBRATION CERTIFICATE																																			
Object: D750V3 - SN: 1188																																			
Calibration Procedure(s): FF-Z11-003-01 Calibration Procedures for dipole validation kits																																			
Calibration date: March 28, 2022																																			
This calibration Certificate documents the traceability to national standards, which realize the physical units of measurements (SI). The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.																																			
All calibrations have been conducted in the closed laboratory facility; environment temperature (22±3)°C and humidity <70%.																																			
Calibration Equipment used (M&TE critical for calibration)																																			
<table border="1"><thead><tr><th>Primary Standards</th><th>ID #</th><th>Cal Date (Calibrated by Certificate No.)</th><th>Scheduled Calibration</th></tr></thead><tbody><tr><td>Power Meter NRP2</td><td>104277</td><td>24-Sep-21 (CTTL No. J21X08328)</td><td>Sep-22</td></tr><tr><td>Power sensor NRP88</td><td>104291</td><td>24-Sep-21 (CTTL No. J21X08328)</td><td>Sep-22</td></tr><tr><td>Reference Probe EX30V4</td><td>SN 7307</td><td>26-May-21 (SPEAG No. EX3-7307_May21)</td><td>May-22</td></tr><tr><td>DAE4</td><td>SN 1556</td><td>12-Jan-22 (CTTL-SPEAG No. Z22-60007)</td><td>Jan-23</td></tr><tr><th>Secondary Standards</th><th>ID #</th><th>Cal Date (Calibrated by Certificate No.)</th><th>Scheduled Calibration</th></tr><tr><td>Signal Generator S4436C</td><td>MY48071430</td><td>13-Jan-22 (CTTL No. J22X00406)</td><td>Jan-23</td></tr><tr><td>Network Analyzer E5071C</td><td>MY46110673</td><td>14-Jan-22 (CTTL No. J22X00406)</td><td>Jan-23</td></tr></tbody></table>				Primary Standards	ID #	Cal Date (Calibrated by Certificate No.)	Scheduled Calibration	Power Meter NRP2	104277	24-Sep-21 (CTTL No. J21X08328)	Sep-22	Power sensor NRP88	104291	24-Sep-21 (CTTL No. J21X08328)	Sep-22	Reference Probe EX30V4	SN 7307	26-May-21 (SPEAG No. EX3-7307_May21)	May-22	DAE4	SN 1556	12-Jan-22 (CTTL-SPEAG No. Z22-60007)	Jan-23	Secondary Standards	ID #	Cal Date (Calibrated by Certificate No.)	Scheduled Calibration	Signal Generator S4436C	MY48071430	13-Jan-22 (CTTL No. J22X00406)	Jan-23	Network Analyzer E5071C	MY46110673	14-Jan-22 (CTTL No. J22X00406)	Jan-23
Primary Standards	ID #	Cal Date (Calibrated by Certificate No.)	Scheduled Calibration																																
Power Meter NRP2	104277	24-Sep-21 (CTTL No. J21X08328)	Sep-22																																
Power sensor NRP88	104291	24-Sep-21 (CTTL No. J21X08328)	Sep-22																																
Reference Probe EX30V4	SN 7307	26-May-21 (SPEAG No. EX3-7307_May21)	May-22																																
DAE4	SN 1556	12-Jan-22 (CTTL-SPEAG No. Z22-60007)	Jan-23																																
Secondary Standards	ID #	Cal Date (Calibrated by Certificate No.)	Scheduled Calibration																																
Signal Generator S4436C	MY48071430	13-Jan-22 (CTTL No. J22X00406)	Jan-23																																
Network Analyzer E5071C	MY46110673	14-Jan-22 (CTTL No. J22X00406)	Jan-23																																
Calibrated by: Zhao Jing SAR Test Engineer		Signature: [Signature]																																	
Reviewed by: Lin Hao SAR Test Engineer		Signature: [Signature]																																	
Approved by: Qi Dianyun SAR Project Leader		Signature: [Signature]																																	
Issued: April 3, 2022																																			
This calibration certificate shall not be reproduced except in full without written approval of the laboratory.																																			
Certificate No: Z22-60103		Page 1 of 6																																	
TTL Speag CALIBRATION LABORATORY		CAICT																																	
Add: No.52 HuaYuanli Road, Haidian District, Beijing, 100191, China Tel: +86-10-4239613-2079 Fax: +86-10-4239613-2564 E-mail: cti@china-test.com http://www.china-test.com		Add: No.52 HuaYuanli Road, Haidian District, Beijing, 100191, China Tel: +86-10-4239613-2079 Fax: +86-10-4239613-2564 E-mail: cti@china-test.com http://www.china-test.com																																	
Measurement Conditions DASY system configuration, as far as not given on page 1:																																			
<table border="1"><thead><tr><th>DASY Version</th><th>DASY52</th><th>V52.10.4</th></tr></thead><tbody><tr><td>Extrapolation</td><td>Advanced Extrapolation</td><td></td></tr><tr><td>Phantom</td><td>Triple Flat Phantom 5.1C</td><td></td></tr><tr><td>Distance Dipole Center - TSL</td><td>15 mm</td><td>with Spacer</td></tr><tr><td>Zoom Scan Resolution</td><td>dx, dy, dz = 5 mm</td><td></td></tr><tr><td>Frequency</td><td>750 MHz ± 1 MHz</td><td></td></tr></tbody></table>				DASY Version	DASY52	V52.10.4	Extrapolation	Advanced Extrapolation		Phantom	Triple Flat Phantom 5.1C		Distance Dipole Center - TSL	15 mm	with Spacer	Zoom Scan Resolution	dx, dy, dz = 5 mm		Frequency	750 MHz ± 1 MHz															
DASY Version	DASY52	V52.10.4																																	
Extrapolation	Advanced Extrapolation																																		
Phantom	Triple Flat Phantom 5.1C																																		
Distance Dipole Center - TSL	15 mm	with Spacer																																	
Zoom Scan Resolution	dx, dy, dz = 5 mm																																		
Frequency	750 MHz ± 1 MHz																																		
Head TSL parameters The following parameters and calculations were applied:																																			
<table border="1"><thead><tr><th></th><th>Temperature</th><th>Permittivity</th><th>Conductivity</th></tr></thead><tbody><tr><td>Nominal Head TSL parameters</td><td>22.0 °C</td><td>42.0</td><td>0.90 mho/m</td></tr><tr><td>Measured Head TSL parameters</td><td>(22.0 ± 0.2) °C</td><td>41.4 ± 0.5 %</td><td>0.89 mho/m ± 0.5 %</td></tr><tr><td>Head TSL temperature change during test</td><td><1.0 °C</td><td>---</td><td>---</td></tr></tbody></table>					Temperature	Permittivity	Conductivity	Nominal Head TSL parameters	22.0 °C	42.0	0.90 mho/m	Measured Head TSL parameters	(22.0 ± 0.2) °C	41.4 ± 0.5 %	0.89 mho/m ± 0.5 %	Head TSL temperature change during test	<1.0 °C	---	---																
	Temperature	Permittivity	Conductivity																																
Nominal Head TSL parameters	22.0 °C	42.0	0.90 mho/m																																
Measured Head TSL parameters	(22.0 ± 0.2) °C	41.4 ± 0.5 %	0.89 mho/m ± 0.5 %																																
Head TSL temperature change during test	<1.0 °C	---	---																																
SAR result with Head TSL																																			
<table border="1"><thead><tr><th></th><th>Condition</th><th></th></tr></thead><tbody><tr><td>SAR averaged over 1 cm² (1 g) of Head TSL</td><td></td><td></td></tr><tr><td>SAR measured</td><td>250 mW input power</td><td>2.07 W/kg</td></tr><tr><td>SAR for nominal Head TSL parameters</td><td>normalized to 1W</td><td>8.27 W/kg ± 18.8 % (k=2)</td></tr><tr><td>SAR averaged over 10 cm² (10 g) of Head TSL</td><td></td><td></td></tr><tr><td>SAR measured</td><td>250 mW input power</td><td>1.37 W/kg</td></tr><tr><td>SAR for nominal Head TSL parameters</td><td>normalized to 1W</td><td>5.48 W/kg ± 18.7 % (k=2)</td></tr></tbody></table>					Condition		SAR averaged over 1 cm ² (1 g) of Head TSL			SAR measured	250 mW input power	2.07 W/kg	SAR for nominal Head TSL parameters	normalized to 1W	8.27 W/kg ± 18.8 % (k=2)	SAR averaged over 10 cm ² (10 g) of Head TSL			SAR measured	250 mW input power	1.37 W/kg	SAR for nominal Head TSL parameters	normalized to 1W	5.48 W/kg ± 18.7 % (k=2)											
	Condition																																		
SAR averaged over 1 cm ² (1 g) of Head TSL																																			
SAR measured	250 mW input power	2.07 W/kg																																	
SAR for nominal Head TSL parameters	normalized to 1W	8.27 W/kg ± 18.8 % (k=2)																																	
SAR averaged over 10 cm ² (10 g) of Head TSL																																			
SAR measured	250 mW input power	1.37 W/kg																																	
SAR for nominal Head TSL parameters	normalized to 1W	5.48 W/kg ± 18.7 % (k=2)																																	
Certificate No: Z22-60103		Page 3 of 6																																	
TTL Speag CALIBRATION LABORATORY		CAICT																																	
Add: No.52 HuaYuanli Road, Haidian District, Beijing, 100191, China Tel: +86-10-4239613-2079 Fax: +86-10-4239613-2564 E-mail: cti@china-test.com http://www.china-test.com		Add: No.52 HuaYuanli Road, Haidian District, Beijing, 100191, China Tel: +86-10-4239613-2079 Fax: +86-10-4239613-2564 E-mail: cti@china-test.com http://www.china-test.com																																	
Appendix (Additional assessments outside the scope of CNAS L0570)																																			
Antenna Parameters with Head TSL																																			
<table border="1"><thead><tr><th>Impedance, transformed to feed point</th><th>53.60 - 1.13jΩ</th></tr><tr><th>Return Loss</th><th>>28.7dB</th></tr></thead></table>				Impedance, transformed to feed point	53.60 - 1.13jΩ	Return Loss	>28.7dB																												
Impedance, transformed to feed point	53.60 - 1.13jΩ																																		
Return Loss	>28.7dB																																		
General Antenna Parameters and Design																																			
<table border="1"><thead><tr><th>Electrical Delay (one direction)</th><th>0.947 ns</th></tr></thead></table>				Electrical Delay (one direction)	0.947 ns																														
Electrical Delay (one direction)	0.947 ns																																		
After long term use with 100W radiated power, only a slight warming of the dipole near the feed-point can be measured.																																			
The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals. On some of the dipoles, small and caps are added to the dipole arms in order to improve matching when placed according to the position as explained in the "Measurement Conditions" paragraph. The SAR data are not affected by this change. The overall dipole length is still according to the Standard. No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feed-point may be damaged.																																			
Additional EUT Data																																			
<table border="1"><thead><tr><th>Manufactured by</th><th>SPEAG</th></tr></thead></table>				Manufactured by	SPEAG																														
Manufactured by	SPEAG																																		
Certificate No: Z22-60103		Page 4 of 6																																	




Unless otherwise agreed in writing, this document is issued by the Company subject to its General Conditions of Service printed overleaf, available on request or accessible at <http://www.sgs.com/en/Terms-and-Conditions.aspx>; and, for electronic format documents, subject to Terms and Conditions for Electronic Documents at <http://www.sgs.com/en/Terms-and-Conditions/Terms-e-Documents.aspx>. Attention is drawn to the limitation of liability, indemnification and jurisdiction issues defined therein. Any holder of this document is advised that information contained hereon reflects the Company's findings at the time of its intervention only and within the limits of Client's instructions, if any. The Company's sole responsibility is to its Client and this document does not exonerate parties to a transaction from exercising all their rights and obligations under the transaction documents. This document cannot be reproduced except in full, without prior written approval of the Company. Any unauthorized alteration, forgery or falsification of the content or appearance of this document is unlawful and offenders may be prosecuted to the fullest extent of the law. Unless otherwise stated the results shown in this test report refer only to the sample(s) tested and such sample(s) are retained for 30 days only.

Attention: To check the authenticity of testing/inspection report & certificate, please contact us at telephone: (86-755) 8307 1443, or email: CN.Doccheck@sgs.com
No.10, Weiye Road, Innovation Park, Kunshan, Jiangsu, China 215300
中国·江苏·昆山市留学生创业园伟业路10号 邮编 215300

t(86-512)57355888 f(86-512)57370818 www.sgs.com.cn
t(86-512)57355888 f(86-512)57370818 sgs.china@sgs.com

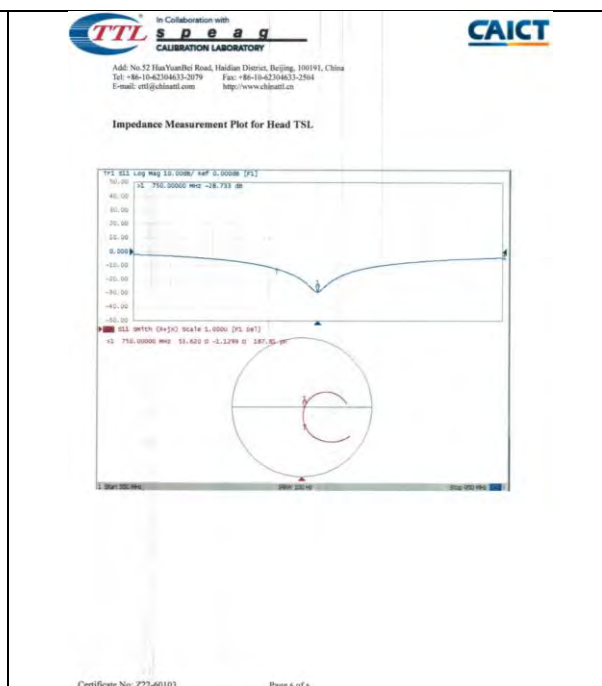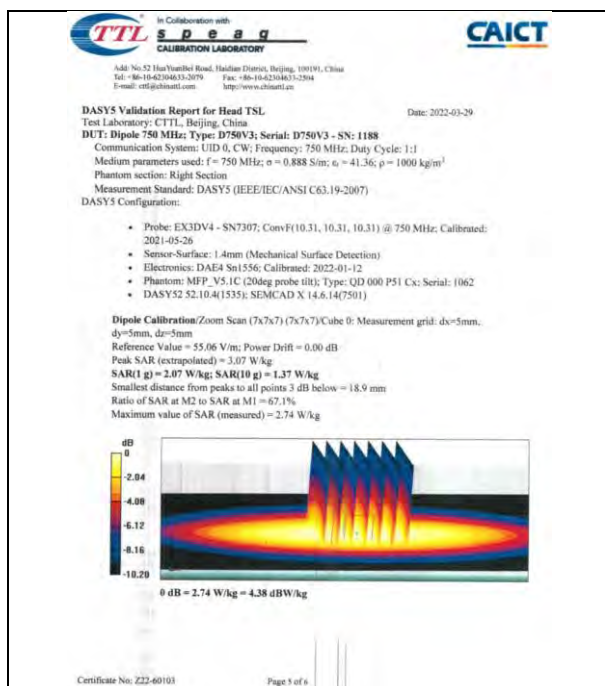

1.4 D835V2 - SN 4d114

 in Collaboration with TTSL Calibration Laboratory Add: No.32 HuaYuanJie, Haidian District, Beijing, 100191 Tel: +86-10-42304033-2312 Fax: +86-10-42304813-2504 E-mail: cttlg@china.com.cn http://www.chinaettlg.com	  中国认可 中国合格 校准 校准 校准 CNAS L8070	CAICT 中国信息通信研究院																				
Certification No: 223-60104																						
CALIBRATION CERTIFICATE																						
Client	SOS-CN																					
Object	D835V2 - SN: 41114																					
Calibration Procedure(s)	FF-Z11-003-01 Calibration Procedures for dipole validation kits																					
Calibration date	March 31, 2022																					
This calibration Certificate documents the traceability to national standards, which realize the physical units of measurements (SI). The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.																						
All calibrations have been conducted in the closed laboratory facility, environment temperature (22±3)°C and humidity<70%.																						
Calibration Equipment used (MATE critical for calibration)																						
<table border="1" style="width: 100%; border-collapse: collapse;"> <thead> <tr> <th style="text-align: left;">Primary Standards</th> <th style="text-align: left;">ID #</th> <th style="text-align: left;">Cal Date (Calibrated by Certificate No.)</th> <th style="text-align: left;">Scheduled Calibration</th> </tr> </thead> <tbody> <tr> <td>Power Meter NRP2</td> <td>100277</td> <td>24-Sep-21 (CTTL No.J21X08326)</td> <td>Sep-22</td> </tr> <tr> <td>Power sensor NRP35</td> <td>104291</td> <td>24-Sep-21 (CTTL No.J21X08326)</td> <td>Sep-22</td> </tr> <tr> <td>Reference Probe EX3DV4</td> <td>SN 7307</td> <td>26-May-21 (SPEAG No.EX3-7307_May21)</td> <td>May-22</td> </tr> <tr> <td>DAA4</td> <td>SN 1556</td> <td>12-Jan-22 (CTTL-SPEAG No.Z22-60007)</td> <td>Jan-23</td> </tr> </tbody> </table>			Primary Standards	ID #	Cal Date (Calibrated by Certificate No.)	Scheduled Calibration	Power Meter NRP2	100277	24-Sep-21 (CTTL No.J21X08326)	Sep-22	Power sensor NRP35	104291	24-Sep-21 (CTTL No.J21X08326)	Sep-22	Reference Probe EX3DV4	SN 7307	26-May-21 (SPEAG No.EX3-7307_May21)	May-22	DAA4	SN 1556	12-Jan-22 (CTTL-SPEAG No.Z22-60007)	Jan-23
Primary Standards	ID #	Cal Date (Calibrated by Certificate No.)	Scheduled Calibration																			
Power Meter NRP2	100277	24-Sep-21 (CTTL No.J21X08326)	Sep-22																			
Power sensor NRP35	104291	24-Sep-21 (CTTL No.J21X08326)	Sep-22																			
Reference Probe EX3DV4	SN 7307	26-May-21 (SPEAG No.EX3-7307_May21)	May-22																			
DAA4	SN 1556	12-Jan-22 (CTTL-SPEAG No.Z22-60007)	Jan-23																			
<table border="1" style="width: 100%; border-collapse: collapse;"> <thead> <tr> <th style="text-align: left;">Secondary Standards</th> <th style="text-align: left;">ID #</th> <th style="text-align: left;">Cal Date (Calibrated by Certificate No.)</th> <th style="text-align: left;">Scheduled Calibration</th> </tr> </thead> <tbody> <tr> <td>Signal Generator E438C</td> <td>MY49071430</td> <td>13-Jan-22 (CTTL No.Z22X0409)</td> <td>Jan-23</td> </tr> <tr> <td>Network Analyzer E5071C</td> <td>MY48110673</td> <td>14-Jan-22 (CTTL No.Z22X0409)</td> <td>Jan-23</td> </tr> </tbody> </table>			Secondary Standards	ID #	Cal Date (Calibrated by Certificate No.)	Scheduled Calibration	Signal Generator E438C	MY49071430	13-Jan-22 (CTTL No.Z22X0409)	Jan-23	Network Analyzer E5071C	MY48110673	14-Jan-22 (CTTL No.Z22X0409)	Jan-23								
Secondary Standards	ID #	Cal Date (Calibrated by Certificate No.)	Scheduled Calibration																			
Signal Generator E438C	MY49071430	13-Jan-22 (CTTL No.Z22X0409)	Jan-23																			
Network Analyzer E5071C	MY48110673	14-Jan-22 (CTTL No.Z22X0409)	Jan-23																			
<table style="width: 100%;"> <tr> <td style="width: 33%; vertical-align: top;"> Caribrated by: Reviewed by: Approved by: </td> <td style="width: 33%; vertical-align: top;"> <table border="0" style="width: 100%;"> <tr> <td style="width: 50%;">Name</td> <td style="width: 50%;">Function</td> </tr> <tr> <td>Zhao Jing</td> <td>SAR Test Engineer</td> </tr> <tr> <td>Lin Hao</td> <td>SAR Test Engineer</td> </tr> <tr> <td>Qi Dianyun</td> <td>SAR Project Leader</td> </tr> </table> </td> <td style="width: 33%; vertical-align: top;"> Signature:    </td> </tr> </table>			Caribrated by: Reviewed by: Approved by:	<table border="0" style="width: 100%;"> <tr> <td style="width: 50%;">Name</td> <td style="width: 50%;">Function</td> </tr> <tr> <td>Zhao Jing</td> <td>SAR Test Engineer</td> </tr> <tr> <td>Lin Hao</td> <td>SAR Test Engineer</td> </tr> <tr> <td>Qi Dianyun</td> <td>SAR Project Leader</td> </tr> </table>	Name	Function	Zhao Jing	SAR Test Engineer	Lin Hao	SAR Test Engineer	Qi Dianyun	SAR Project Leader	Signature:   									
Caribrated by: Reviewed by: Approved by:	<table border="0" style="width: 100%;"> <tr> <td style="width: 50%;">Name</td> <td style="width: 50%;">Function</td> </tr> <tr> <td>Zhao Jing</td> <td>SAR Test Engineer</td> </tr> <tr> <td>Lin Hao</td> <td>SAR Test Engineer</td> </tr> <tr> <td>Qi Dianyun</td> <td>SAR Project Leader</td> </tr> </table>	Name	Function	Zhao Jing	SAR Test Engineer	Lin Hao	SAR Test Engineer	Qi Dianyun	SAR Project Leader	Signature:   												
Name	Function																					
Zhao Jing	SAR Test Engineer																					
Lin Hao	SAR Test Engineer																					
Qi Dianyun	SAR Project Leader																					
Issued: April 6, 2022																						
This calibration certificate shall not be reproduced except in full without written approval of the laboratory.																						

	In Collaboration with:  CAICT CALIBRATION LABORATORY						
Address: 53 Huaibei Road, Haidian District, Beijing, 100190, P.R. China Tel: +86-10-84204631-2079 E-mail: cstj@caict.ac.cn	Fax: +86-10-84204631-2104 http://www.caict.ac.cn						
Glossary: <table border="0"> <tr> <td>TSL</td> <td>tissue simulating liquid</td> </tr> <tr> <td>Conf#</td> <td>sensitivity in TSL / NORMx.y.z</td> </tr> <tr> <td>N/A</td> <td>not applicable or not measured</td> </tr> </table>		TSL	tissue simulating liquid	Conf#	sensitivity in TSL / NORMx.y.z	N/A	not applicable or not measured
TSL	tissue simulating liquid						
Conf#	sensitivity in TSL / NORMx.y.z						
N/A	not applicable or not measured						
Calibration is Performed According to the Following Standards:							
a) IECIEEIE 62209-1528, "Measurement Procedure for The Assessment of Specific Absorption Rate of Human Exposure to Radio Frequency Fields from Hand-held and Body-mounted Wireless Communication Devices- Part 1528: Human Models, Instrumentation and Procedures" (Frequency range of 4 MHz to 10 GHz), October 2020 b) KDB 865664, "SAR Measurement Requirements for 100 MHz to 6 GHz"							
Additional Documentation:							
c) DAS7445 System Handbook							
Methods Applied and Interpretation of Parameters:							
• Measurement Conditions: Further details are available from the Validation Report at the end of the certificate. All figures stated in the certificate are valid at the frequency indicated. • Antenna Parameters with TSL: The dipole is mounted with the spacer to position its feed point exactly below the center marking of the flat phantom section, with the arms oriented parallel to the body axis. • Feed Point Impedance and Return Loss: These parameters are measured with the dipole positioned under the liquid filled phantom. The impedance stated is transformed from the measurement at the SMA connector to the feed point. The Return Loss ensures low reflected power. No uncertainty required. • Electrical Delay: One-way delay between the SMA connector and the antenna feed point. No uncertainty required. • SAR measured: SAR measured at the stated antenna input power. • SAR normalized: SAR as measured, normalized to an input power of 1 W at the antenna connector. • SAR for nominal TSL parameters: The measured TSL parameters are used to calculate the nominal SAR result.							
The reported uncertainty of measurement is stated as the standard uncertainty of Measurement multiplied by the coverage factor $k=2$, which for a normal distribution corresponds to a coverage probability of approximately 95%.							




Unless otherwise agreed in writing, this document is issued by the Company subject to its General Conditions of Service printed hereon, available on request or accessible at <http://www.sgs.com/en/Terms-and-Conditions.aspx>, and for electronic format documents, subject to Terms and Conditions for Electronic Documents at <http://www.sgs.com/en/Terms-and-Conditions/Terms-e-Documents.aspx>. Attention is drawn to the limitation of liability, indemnification and jurisdiction issues defined therein. Any holder of this document is advised that information contained herein reflects the Company's findings at the time of its intervention only and within the limits of the Company's instructions, if any. The Company's responsibility is to deliver and to accurately transcribe the data contained in the documents transmitted, not to raise or to defend against the legal rights and obligations arising from the transaction. This document cannot be reproduced except in full, without prior written approval of the Company. Any unauthorized alteration, forgery or falsification of the content or appearance of this document is unlawful and offenders may be prosecuted to the fullest extent of the law. Unless otherwise stated the results shown in this test report refer only to the sample(s) tested and such sample(s) are retained for 30 days only.


Attention: For any request for a copy of the test report, inspection report or certificate, please contact us at telephone: (86-755) 8307 1443, or email: CN.Doccheck@sgs.com.

No.10, Weiye Road, Innovation Park, Kunshan, Jiangsu, China 215300
中国·江苏·昆山市留学生创业园伟业路10号 邮编 215300

t(86-512)57355888 f(86-512)57370818 www.sgsgroup.com.cn
t(86-512)57355888 f(86-512)57370818 sqs.china@sqs.com

TTL Speag Calibration Laboratory		CAICT	
Add: No.52 HuaYuanhui Road, Haidian District, Beijing, 100191, China Tel: +86-10-42304633-2079 Fax: +86-10-42304633-2504 E-mail: cti@china.ttl.com http://www.china.ttl.com		Add: No.52 HuaYuanhui Road, Haidian District, Beijing, 100191, China Tel: +86-10-42304633-2079 Fax: +86-10-42304633-2504 E-mail: cti@china.ttl.com http://www.china.ttl.com	
Measurement Conditions DASY system configuration, as far as not given on page 1			
DASY Version	DASY52	VS2 10.4	
Extrapolation	Advanced Extrapolation		
Phantom	Triple Flat Phantom 5.1C		
Distance Dipole Center - TSL	15 mm	with Spacer	
Zoom Scan Resolution	dx, dy, dz = 5 mm		
Frequency	835 MHz ± 1 MHz		
Head TSL parameters The following parameters and calculations were applied:			
Nominal Head TSL parameters	Temperature	Permittivity	Conductivity
	22.0 °C	41.5	0.80 mho/m
Measured Head TSL parameters	(22.0 ± 0.2) °C	41.0 ± 0.5	0.81 mho/m ± 0.5%
Head TSL temperature change during last	< 1.0 °C	—	—
SAR result with Head TSL			
SAR averaged over 1 cm ³ (1 g) of Head TSL	Condition		
SAR measured	250 mW input power	2.37 W/kg	
SAR for nominal Head TSL parameters	normalized to 1W	9.40 W/kg ± 18.8 % (k=2)	
SAR averaged over 10 cm ³ (10 g) of Head TSL	Condition		
SAR measured	250 mW input power	1.54 W/kg	
SAR for nominal Head TSL parameters	normalized to 1W	6.12 W/kg ± 18.7 % (k=2)	
Appendix (Additional assessments outside the scope of CNAS L0570)			
Antenna Parameters with Head TSL			
Impedance, transformed to feed point	48.70 - j 22.0 Ω		
Return Loss	-25.3 dB		
General Antenna Parameters and Design			
Electrical Delay (one direction)	1.307 ns		
After long term use with 100W radiated power, only a slight warming of the dipole near the feed-point can be measured.			
The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals. On some of the dipoles, small end caps are added to the dipole arms in order to improve matching when loaded according to the position as explained in the "Measurement Conditions" paragraph. The SAR data are not affected by this change. The overall dipole length is still according to the Standard.			
No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feed-point may be damaged.			
Additional EUT Data			
Manufactured by	SPEAG		
Certificate No: Z22-60104 Page 1 of 6			

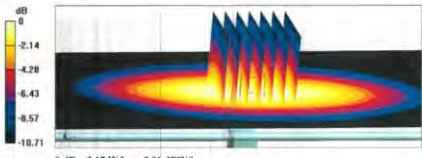TTL Speag Calibration Laboratory		CAICT	
Add: No.52 HuaYuanhui Road, Haidian District, Beijing, 100191, China Tel: +86-10-42304633-2079 Fax: +86-10-42304633-2504 E-mail: cti@china.ttl.com http://www.china.ttl.com		Add: No.52 HuaYuanhui Road, Haidian District, Beijing, 100191, China Tel: +86-10-42304633-2079 Fax: +86-10-42304633-2504 E-mail: cti@china.ttl.com http://www.china.ttl.com	
DASY5 Validation Report for Head TSL Test Laboratory: CTTL, Beijing, China DUT: Dipole 835 MHz; Type: D835V2; Serial: D835V2 - SN: 40114 Communication System: UHF 0, CW; Frequency: 835 MHz; Duty Cycle: 1:1 Medium parameters used: f = 835 MHz; σ = 0.907 S/m; ε = 40.98; ρ = 1000 kg/m ³ Phantom section: Right Section Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2007) DASY5 Configuration:			
• Probe: EX3DV4 - SN7307; ConvF(10.13, 10.13, 10.13) @ 835 MHz; Calibrated: 2021-05-26			
• Sensor Surface: 1.4mm (Mechanical Surface Detection)			
• Electronics: DA64 Sn1556; Calibrated: 2022-01-12			
• Phantom: MFP_V5.1C (20deg probe tilt); Type: QD 000 P51 Cx; Serial: 1062			
• DASY52 52.10.4(153); SEMCAD X 14.6.14(7501)			
Dipole Calibration/Zoom Scan (7x7x7) (7x7x7) Cube 0: Measurement grid: dx=5mm, dy=5mm, dz=5mm Reference Value = 57.88 V/m; Power Drift = 0.04 dB Peak SAR (extrapolated) = 3.56 W/kg SAR(1 g) = 2.37 W/kg; SAR(10 g) = 1.54 W/kg Smallest distance from peaks to all points 3 dB below = 15.8 mm Ratio of SAR at M2 to SAR at M1 = 66.2% Maximum value of SAR (measured) = 3.17 W/kg			
			
Certificate No: Z22-60104 Page 5 of 6			

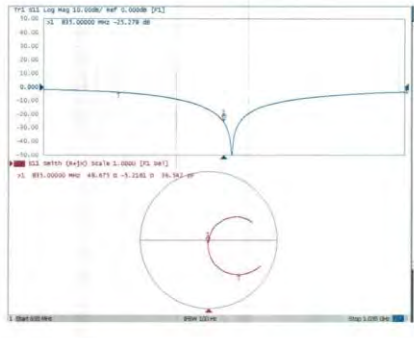TTL Speag Calibration Laboratory		CAICT	
Add: No.52 HuaYuanhui Road, Haidian District, Beijing, 100191, China Tel: +86-10-42304633-2079 Fax: +86-10-42304633-2504 E-mail: cti@china.ttl.com http://www.china.ttl.com		Add: No.52 HuaYuanhui Road, Haidian District, Beijing, 100191, China Tel: +86-10-42304633-2079 Fax: +86-10-42304633-2504 E-mail: cti@china.ttl.com http://www.china.ttl.com	
Impedance Measurement Plot for Head TSL			
			
Certificate No: Z22-60104 Page 6 of 6			



Unless otherwise agreed in writing, this document is issued by the Company subject to its General Conditions of Service printed overleaf, available on request or accessible at <http://www.sgs.com/en/Terms-and-Conditions.aspx>; and, for electronic format documents, subject to Terms and Conditions for Electronic Documents at <http://www.sgs.com/en/Terms-and-Conditions/Terms-e-Document.aspx>. Attention is drawn to the limitation of liability, indemnification and jurisdiction issues defined therein. Any holder of this document is advised that information contained hereon reflects the Company's findings at the time of its intervention only and within the limits of Client's instructions, if any. The Company's sole responsibility is to its Client and this document does not exonerate parties to a transaction from exercising all their rights and obligations under the transaction documents. This document cannot be reproduced except in full, without prior written approval of the Company. Any unauthorized alteration, forgery or falsification of the content or appearance of this document is unlawful and offenders may be prosecuted to the fullest extent of the law. Unless otherwise stated the results shown in this test report refer only to the sample(s) tested and such sample(s) are retained for 30 days only.

Attention: To check the authenticity of testing / inspection report & certificate, please contact us at telephone: (86-755) 8307 1443, or email: CN.Doccheck@sgs.com
No.10, Weiye Road, Innovation Park, Kunshan, Jiangsu, China 215300
中国·江苏·昆山市留学生创业园伟业路10号 邮编 215300

t(86-512)57355888 f(86-512)57370818 www.sgs.com
t(86-512)57355888 f(86-512)57370818 sgs.china@sgs.com

1.5 D900V2 - SN 1d079

TTL In Collaboration with SPS CALIBRATION LABORATORY Address: No.52 HuaYuan Road, Haidian District, Beijing, 100191 Tel: +86-10-42346323-117 E-mail: cti@sgs.com.cn Client: SGS-CN Certificate No: Z22-60184 CALIBRATION CERTIFICATE Object: D900V2 - SN: 1d079 Calibration Procedure(s): PF-Z11-003-01 Calibration Procedures for dipole validation kits Calibration date: June 7, 2022 The calibration Certificate documents the traceability to national standards, which realize the physical units of measurements (SI). The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate. All calibrations have been conducted in the closed laboratory facility, environment temperature (23±1°C) and humidity <70%. Calibration Equipment used (MATE critical for calibration) <table border="1"> <thead> <tr> <th>Primary Standards</th> <th>ID #</th> <th>Cal Date (Calibrated by Certificate No.)</th> <th>Scheduled Calibration</th> </tr> </thead> <tbody> <tr> <td>Power Meter: NRP2</td> <td>106277</td> <td>24-Sep-21 (CTTL No. Z21X08326)</td> <td>Sep-22</td> </tr> <tr> <td>Power sensor: NRP85</td> <td>104291</td> <td>24-Sep-21 (CTTL No. Z21X08326)</td> <td>Sep-22</td> </tr> <tr> <td>Reference Probe: EX32V4</td> <td>SN 7484</td> <td>26-Jan-22 (SPEAG No. EX3-7484_Jan22)</td> <td>Jan-23</td> </tr> <tr> <td>DAE4</td> <td>SN 1586</td> <td>12-Jan-22 (CTTL-SPEAG No. Z22-60007)</td> <td>Jan-23</td> </tr> </tbody> </table> <table border="1"> <thead> <tr> <th>Secondary Standards</th> <th>ID #</th> <th>Cal Date (Calibrated by Certificate No.)</th> <th>Scheduled Calibration</th> </tr> </thead> <tbody> <tr> <td>Signal Generator: E2438C</td> <td>MY48071430</td> <td>13-Jan-22 (CTTL No. Z22X00406)</td> <td>Jan-23</td> </tr> <tr> <td>Network Analyzer: E5071C</td> <td>MY48110473</td> <td>14-Jan-22 (CTTL No. Z22X00406)</td> <td>Jan-23</td> </tr> </tbody> </table> Calibrated by: Zhao Jing SAR Test Engineer Reviewed by: Lin Hao SAR Test Engineer Approved by: Qi Dianyan SAR Project Leader Issued: June 13, 2022 This calibration certificate shall not be reproduced except in full without written approval of the laboratory. Certificate No: Z22-60184 Page 1 of 4	Primary Standards	ID #	Cal Date (Calibrated by Certificate No.)	Scheduled Calibration	Power Meter: NRP2	106277	24-Sep-21 (CTTL No. Z21X08326)	Sep-22	Power sensor: NRP85	104291	24-Sep-21 (CTTL No. Z21X08326)	Sep-22	Reference Probe: EX32V4	SN 7484	26-Jan-22 (SPEAG No. EX3-7484_Jan22)	Jan-23	DAE4	SN 1586	12-Jan-22 (CTTL-SPEAG No. Z22-60007)	Jan-23	Secondary Standards	ID #	Cal Date (Calibrated by Certificate No.)	Scheduled Calibration	Signal Generator: E2438C	MY48071430	13-Jan-22 (CTTL No. Z22X00406)	Jan-23	Network Analyzer: E5071C	MY48110473	14-Jan-22 (CTTL No. Z22X00406)	Jan-23	TTL In Collaboration with SPS CALIBRATION LABORATORY Address: No.52 HuaYuan Road, Haidian District, Beijing, 100191 Tel: +86-10-42346323-117 E-mail: cti@sgs.com.cn Glossary: TSL: Issue simulating liquid ConvF: sensitivity in TSL / NORM.y,z N/A: not applicable or not measured Calibration is Performed According to the Following Standards: a) IEC/IEEE 62209-1528, "Measurement Procedure for The Assessment of Specific Absorption Rate of Human Exposure to Radio Frequency Fields from Hand-held and Body-mounted Wireless Communication Devices-Part 1528: Human Models, Instrumentation and Procedures (Frequency range of 4 MHz to 10 GHz)", October 2020 b) KDB 865664, "SAR Measurement Requirements for 100 MHz to 6 GHz" c) DASYS45 System Handbook Additional Documentation: c) DASYS45 System Handbook Methods Applied and Interpretation of Parameters: • Measurement Conditions: Further details are available from the Validation Report at the end of the certificate. All figures stated in the certificate are valid at the frequency indicated. • Antenna Parameters with TSL: The dipole is mounted with the spacer to position its feed point exactly below the center marking of the flat phantom section, with the arms oriented parallel to the body axis. • Feed Point Impedance and Return Loss: These parameters are measured with the dipole positioned under the liquid filled phantom. The impedance stated is transformed from the measurement at the SMA connector to the feed point. The Return Loss ensures low reflected power. No uncertainty required. • Electrical Delay: One-way delay between the SMA connector and the antenna feed point. No uncertainty required. • SAR measured: SAR measured at the stated antenna input power. • SAR normalized: SAR as measured, normalized to an input power of 1 W at the antenna connector. • SAR for nominal TSL parameters: The measured TSL parameters are used to calculate the nominal SAR result. The reported uncertainty of measurement is stated as the standard uncertainty of Measurement multiplied by the coverage factor k=2, which for a normal distribution corresponds to a coverage probability of approximately 95%. Certificate No: Z22-60184 Page 1 of 4																																		
Primary Standards	ID #	Cal Date (Calibrated by Certificate No.)	Scheduled Calibration																																																																
Power Meter: NRP2	106277	24-Sep-21 (CTTL No. Z21X08326)	Sep-22																																																																
Power sensor: NRP85	104291	24-Sep-21 (CTTL No. Z21X08326)	Sep-22																																																																
Reference Probe: EX32V4	SN 7484	26-Jan-22 (SPEAG No. EX3-7484_Jan22)	Jan-23																																																																
DAE4	SN 1586	12-Jan-22 (CTTL-SPEAG No. Z22-60007)	Jan-23																																																																
Secondary Standards	ID #	Cal Date (Calibrated by Certificate No.)	Scheduled Calibration																																																																
Signal Generator: E2438C	MY48071430	13-Jan-22 (CTTL No. Z22X00406)	Jan-23																																																																
Network Analyzer: E5071C	MY48110473	14-Jan-22 (CTTL No. Z22X00406)	Jan-23																																																																
TTL In Collaboration with SPS CALIBRATION LABORATORY Address: No.52 HuaYuan Road, Haidian District, Beijing, 100191 Tel: +86-10-42346323-117 E-mail: cti@sgs.com.cn Measurement Conditions DASYS system configuration, as far as not given on page 1: <table border="1"> <thead> <tr> <th>DASYS Version</th> <th>DASYS2</th> <th>52.10.4</th> </tr> </thead> <tbody> <tr> <td>Extrapolation</td> <td>Advanced Extrapolation</td> <td></td> </tr> <tr> <td>Phantom</td> <td>Tight Fit Phantom 5.1C</td> <td></td> </tr> <tr> <td>Distance Dipole Center - TSL</td> <td>15 mm</td> <td>with Spacer</td> </tr> <tr> <td>Zoom Scan Resolution</td> <td>0x, dy, dz = 5 mm</td> <td></td> </tr> <tr> <td>Frequency</td> <td>900 MHz ± 1 MHz</td> <td></td> </tr> </tbody> </table> Head TSL parameters The following parameters and calculations were applied: <table border="1"> <thead> <tr> <th></th> <th>Temperature</th> <th>Permittivity</th> <th>Conductivity</th> </tr> </thead> <tbody> <tr> <td>Nominal Head TSL parameters</td> <td>22.0 °C</td> <td>41.5</td> <td>0.97 mho/m</td> </tr> <tr> <td>Measured Head TSL parameters</td> <td>(22.0 ± 0.2) °C</td> <td>42.1 ± 6 %</td> <td>0.98 mho/m ± 6 %</td> </tr> <tr> <td>Head TSL temperature change during test</td> <td><+1.0 °C</td> <td>—</td> <td>—</td> </tr> </tbody> </table> SAR result with Head TSL <table border="1"> <thead> <tr> <th>SAR averaged over 1 cm³ (1 g) of Head TSL</th> <th>Condition</th> <th></th> </tr> </thead> <tbody> <tr> <td>SAR measured</td> <td>250 mW input power</td> <td>2.76 W/kg</td> </tr> <tr> <td>SAR for nominal Head TSL parameters</td> <td>normalized to 1W</td> <td>11.0 W/kg ± 18.8 % (k=2)</td> </tr> <tr> <td>SAR averaged over 10 cm³ (10 g) of Head TSL</td> <th>Condition</th> <th></th> </tr> <tr> <td>SAR measured</td> <td>250 mW input power</td> <td>1.75 W/kg</td> </tr> <tr> <td>SAR for nominal Head TSL parameters</td> <td>normalized to 1W</td> <td>7.09 W/kg ± 18.7 % (k=2)</td> </tr> </tbody> </table> Certificate No: Z22-60184 Page 1 of 4	DASYS Version	DASYS2	52.10.4	Extrapolation	Advanced Extrapolation		Phantom	Tight Fit Phantom 5.1C		Distance Dipole Center - TSL	15 mm	with Spacer	Zoom Scan Resolution	0x, dy, dz = 5 mm		Frequency	900 MHz ± 1 MHz			Temperature	Permittivity	Conductivity	Nominal Head TSL parameters	22.0 °C	41.5	0.97 mho/m	Measured Head TSL parameters	(22.0 ± 0.2) °C	42.1 ± 6 %	0.98 mho/m ± 6 %	Head TSL temperature change during test	<+1.0 °C	—	—	SAR averaged over 1 cm ³ (1 g) of Head TSL	Condition		SAR measured	250 mW input power	2.76 W/kg	SAR for nominal Head TSL parameters	normalized to 1W	11.0 W/kg ± 18.8 % (k=2)	SAR averaged over 10 cm ³ (10 g) of Head TSL	Condition		SAR measured	250 mW input power	1.75 W/kg	SAR for nominal Head TSL parameters	normalized to 1W	7.09 W/kg ± 18.7 % (k=2)	TTL In Collaboration with SPS CALIBRATION LABORATORY Address: No.52 HuaYuan Road, Haidian District, Beijing, 100191 Tel: +86-10-42346323-117 E-mail: cti@sgs.com.cn Appendix (Additional assessments outside the scope of CNAS L0670) Antenna Parameters with Head TSL <table border="1"> <thead> <tr> <th></th> <th>48 (10-9-450)</th> </tr> </thead> <tbody> <tr> <td>Impedance, transformed to feed point</td> <td></td> </tr> <tr> <td>Return Loss</td> <td>-23.3 dB</td> </tr> </tbody> </table> General Antenna Parameters and Design <table border="1"> <thead> <tr> <th>Electrical Delay (one direction)</th> <th>1.312 ns</th> </tr> </thead> <tbody> <tr> <td></td> <td></td> </tr> </tbody> </table> After long term use with 100W radiated power, only a slight warming of the dipole near the feed-point can be measured. The dipole is made of standard serringid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC signals. On some of the dipoles, small end caps are added to the dipole arms in order to improve matching when loaded according to the position as explained in the "Measurement Conditions" paragraph. The SAR data are not affected by this change. The overall dipole length is still according to the Standard. No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feed-point may be damaged. Additional EUT Data <table border="1"> <thead> <tr> <th>Manufactured by</th> <th>SPEAG</th> </tr> </thead> <tbody> <tr> <td></td> <td></td> </tr> </tbody> </table> Certificate No: Z22-60184 Page 1 of 6		48 (10-9-450)	Impedance, transformed to feed point		Return Loss	-23.3 dB	Electrical Delay (one direction)	1.312 ns			Manufactured by	SPEAG		
DASYS Version	DASYS2	52.10.4																																																																	
Extrapolation	Advanced Extrapolation																																																																		
Phantom	Tight Fit Phantom 5.1C																																																																		
Distance Dipole Center - TSL	15 mm	with Spacer																																																																	
Zoom Scan Resolution	0x, dy, dz = 5 mm																																																																		
Frequency	900 MHz ± 1 MHz																																																																		
	Temperature	Permittivity	Conductivity																																																																
Nominal Head TSL parameters	22.0 °C	41.5	0.97 mho/m																																																																
Measured Head TSL parameters	(22.0 ± 0.2) °C	42.1 ± 6 %	0.98 mho/m ± 6 %																																																																
Head TSL temperature change during test	<+1.0 °C	—	—																																																																
SAR averaged over 1 cm ³ (1 g) of Head TSL	Condition																																																																		
SAR measured	250 mW input power	2.76 W/kg																																																																	
SAR for nominal Head TSL parameters	normalized to 1W	11.0 W/kg ± 18.8 % (k=2)																																																																	
SAR averaged over 10 cm ³ (10 g) of Head TSL	Condition																																																																		
SAR measured	250 mW input power	1.75 W/kg																																																																	
SAR for nominal Head TSL parameters	normalized to 1W	7.09 W/kg ± 18.7 % (k=2)																																																																	
	48 (10-9-450)																																																																		
Impedance, transformed to feed point																																																																			
Return Loss	-23.3 dB																																																																		
Electrical Delay (one direction)	1.312 ns																																																																		
Manufactured by	SPEAG																																																																		




Unless otherwise agreed in writing, this document is issued by the Company subject to its General Conditions of Service printed overleaf, available on request or accessible at <http://www.sgs.com/en/Terms-and-Conditions.aspx>; and, for electronic format documents, subject to Terms and Conditions for Electronic Documents at <http://www.sgs.com/en/Terms-and-Conditions/Terms-e-Documents.aspx>. Attention is drawn to the limitation of liability, indemnification and jurisdiction issues defined therein. Any holder of this document is advised that information contained hereon reflects the Company's findings at the time of its intervention only and within the limits of Client's instructions, if any. The Company's sole responsibility is to its Client and this document does not exonerate parties to a transaction from exercising all their rights and obligations under the transaction documents. This document cannot be reproduced in full, without prior written approval of the Company. Any unauthorized alteration, forgery or falsification of the content or appearance of this document is unlawful and offenders may be prosecuted to the fullest extent of the law. Unless otherwise stated the results shown in this test report refer only to the sample(s) tested and such sample(s) are retained for 30 days only.

Attention: To check the authenticity of testing / inspection report & certificate, please contact us at telephone: (86-755) 8307 1443, or email: CN.Doccheck@sgs.com

No.10, Weyue Road, Innovation Park, Kunshan, Jiangsu, China 215300
中国·江苏·昆山市留学生创业园伟业路10号 邮编 215300

(86-512) 57355888 (86-512) 57370818 www.sgs.com.cn
(86-512) 57355888 (86-512) 57370818 sgs.china@sgs.com

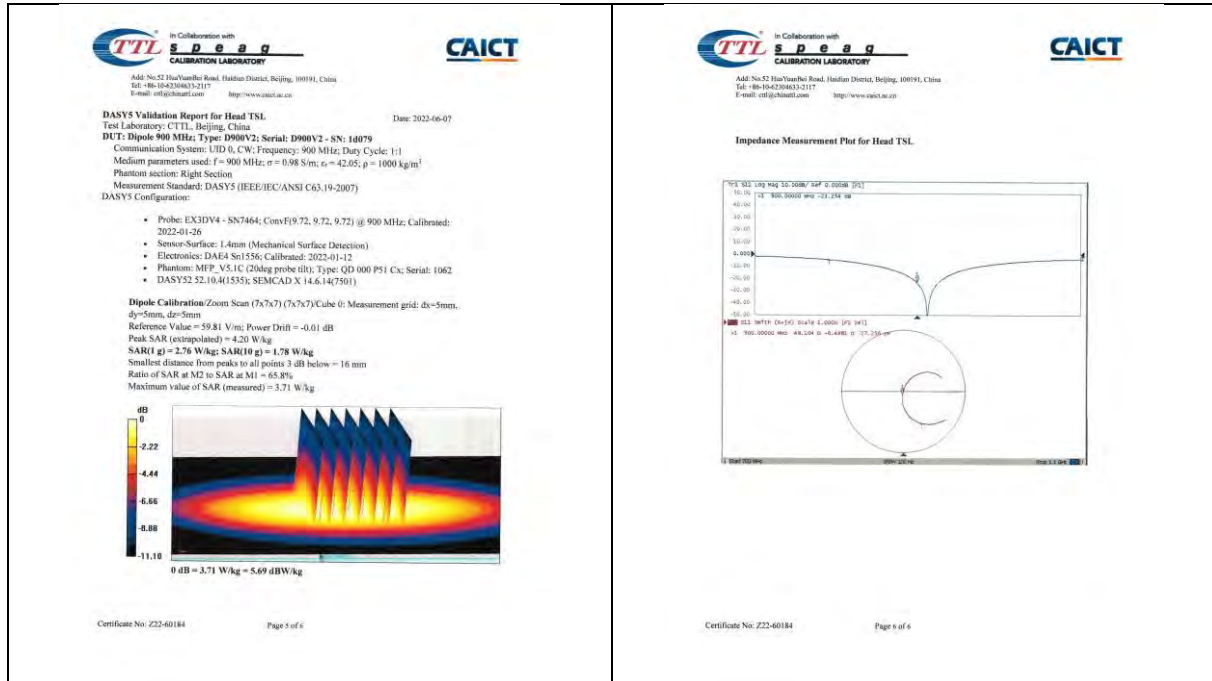

1.6 D1800V2 - SN 2d170

TTL Calibration Laboratory
Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China
Tel: +86-10-42306033-2117
E-mail: cti@china.ttl.com

CAICT

Client: **SGS-CN** Certificate No: **Z22-60105**

CALIBRATION CERTIFICATE

Object: **D1800V2 - SN: 2d170**

Calibration Procedure(s): **FF-Z11-003-01**
Calibration Procedures for dipole validation kits

Calibration date: **March 31, 2022**

This calibration Certificate documents the traceability to national standards, which realizes the physical units of measurements (SI). The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility, environment temperature (22±3)°C and humidity <70%.

Calibration Equipment used (M&TE critical for calibration)

Primary Standards	ID #	Cal Date (Calibrated by Certificate No.)	Scheduled Calibration
Power Meter NRP2	106277	24-Sep-21 (CTTL No.J21X08326)	Sep-22
Power sensor NRP8S	104291	24-Sep-21 (CTTL No.J21X08326)	Sep-22
Reference Probe EX3DV4	SN 7307	26-May-21 (SPEAG No.EX3-7307_May21)	May-22
DAE4	SN 1556	12-Jan-22 (CTTL-SPEAG No.Z22-60007)	Jan-23

Secondary Standards	ID #	Cal Date (Calibrated by Certificate No.)	Scheduled Calibration
Signal Generator E4438C	MY48071430	13-Jan-22 (CTTL No.J22X00409)	Jan-23
Network Analyzer E5071C	MY48110673	14-Jan-22 (CTTL No.J22X00409)	Jan-23

Calibrated by: **Zhao Jing** SAR Test Engineer
Reviewed by: **Lin Hao** SAR Test Engineer
Approved by: **Qi Diqian** SAR Project Leader

Issued: April 6, 2022
This calibration certificate shall not be reproduced except in full without written approval of the laboratory.

Certificate No: Z22-60105 Page 1 of 6

TTL Calibration Laboratory
Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China
Tel: +86-10-42306033-2117
E-mail: cti@china.ttl.com

CAICT

Glossary:
TSL: tissue simulating liquid
ConvF: sensitivity in TSL / NORM_{x,y,z}
N/A: not applicable or not measured

Calibration is Performed According to the Following Standards:
a) IEC/IEEE 62209-1528, "Measurement Procedure for The Assessment of Specific Absorption Rate of Human Exposure to Radio Frequency Fields from Hand-held and Body-mounted Wireless Communication Devices- Part 1528: Human Models, Instrumentation and Procedures (Frequency range of 4 MHz to 10 GHz)", October 2020
b) KDB 855664, "SAR Measurement Requirements for 100 MHz to 6 GHz"

Additional Documentation:
c) DASY4/5 System Handbook

Methods Applied and Interpretation of Parameters:

- Measurement Conditions:** Further details are available from the Validation Report at the end of the certificate. All figures stated in the certificate are valid at the frequency indicated.
- Antenna Parameters with TSL:** The dipole is mounted with the spacer to position its feed point exactly below the center marking of the flat phantom section, with the arms oriented parallel to the body axis.
- Feed Point Impedance and Return Loss:** These parameters are measured with the dipole positioned under the liquid filled phantom. The impedance stated is transformed from the measurement at the SMA connector to the feed point. The Return Loss ensures low reflected power. No uncertainty required.
- Electrical Delay:** One-way delay between the SMA connector and the antenna feed point. No uncertainty required.
- SAR measured:** SAR measured at the stated antenna input power.
- SAR normalized:** SAR as measured, normalized to an input power of 1 W at the antenna connector.
- SAR for nominal TSL parameters:** The measured TSL parameters are used to calculate the nominal SAR result.

The reported uncertainty of measurement is stated as the standard uncertainty of Measurement multiplied by the coverage factor k=2, which for a normal distribution corresponds to a coverage probability of approximately 95%.

Certificate No: Z22-60105 Page 2 of 6




Unless otherwise agreed in writing, this document is issued by the Company subject to its General Conditions of Service printed overleaf, available on request or accessible at <http://www.sgs.com/en/Terms-and-Conditions.aspx> and, for electronic format documents, subject to Terms and Conditions for Electronic Documents at <http://www.sgs.com/en/Terms-and-Conditions/Terms-e-Documents.aspx>. Attention is drawn to the limitation of liability, indemnification and jurisdiction issues defined therein. Any holder of this document is advised that information contained hereon reflects the Company's findings at the time of its intervention only and within the limits of Client's instructions, if any. The Company's sole responsibility is to its Client and this document does not exonerate parties to a transaction from exercising all their rights and obligations under the transaction documents. This document cannot be reproduced except in full, without prior written approval of the Company. Any unauthorized alteration, forgery or falsification of the content or appearance of this document is unlawful and offenders may be prosecuted to the fullest extent of the law. Unless otherwise stated the results shown in this test report refer only to the sample(s) tested and such sample(s) are retained for 30 days only.

Attention: To check the authenticity of testing/inspection report & certificate, please contact us at telephone: (86-755) 8307 1443, or email: CN.Doccheck@sgs.com

No.10, Weiye Road, Innovation Park, Kunshan, Jiangsu, China 215300
中国·江苏·昆山市留学生创业园伟业路10号 邮编 215300

t(86-512)57355888 f(86-512)57370818 www.sgsgroup.com.cn
t(86-512)57355888 f(86-512)57370818 sgs.china@sgs.com

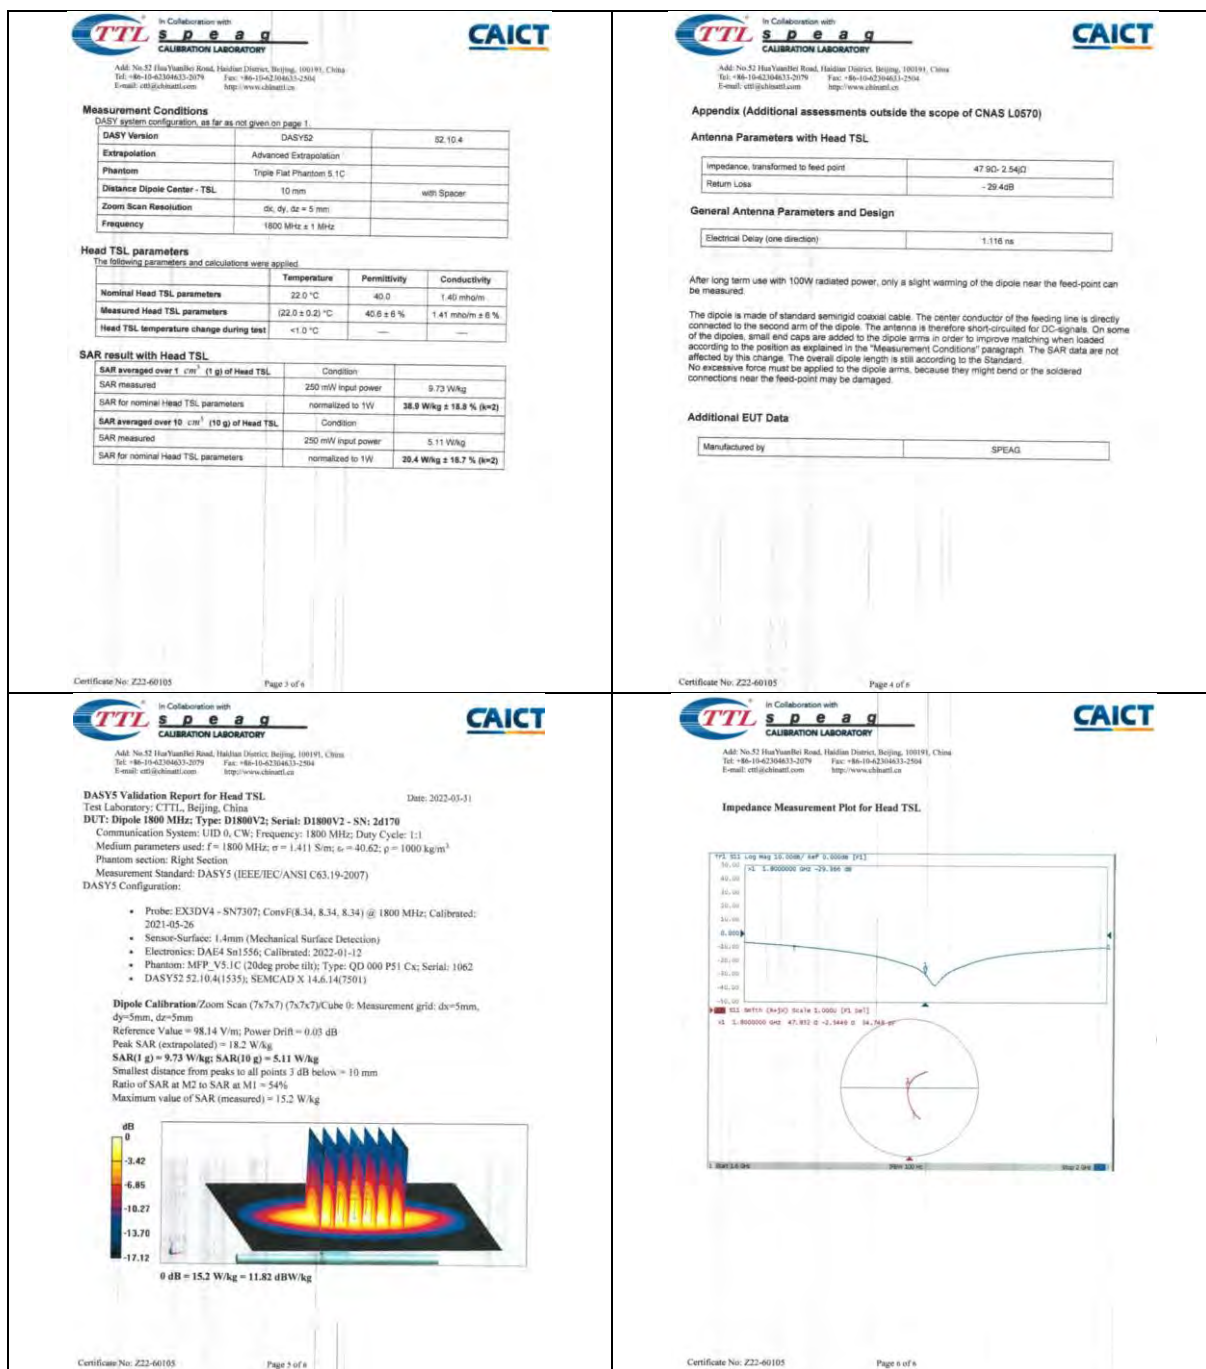

Unless otherwise agreed in writing, this document is issued by the Company subject to its General Conditions of Service printed overleaf, available on request or accessible at <http://www.sgs.com/en/Terms-and-Conditions.aspx> and, for electronic format documents, subject to Terms and Conditions for Electronic Documents at <http://www.sgs.com/en/Terms-and-Conditions/Terms-e-Documents.aspx>. Attention is drawn to the limitation of liability, indemnification and jurisdiction issues defined therein. Any holder of this document is advised that information contained hereon reflects the Company's findings at the time of its intervention only and within the limits of Client's instructions, if any. The Company's sole responsibility is to its Client and this document does not exonerate parties to a transaction from exercising all their rights and obligations under the transaction documents. This document cannot be reproduced except in full, without prior written approval of the Company. Any unauthorized alteration, forgery or falsification of the content or appearance of this document is unlawful and offenders may be prosecuted to the fullest extent of the law. Unless otherwise stated the results shown in this test report refer only to the sample(s) tested and such sample(s) are retained for 30 days only.

Attention: To check the authenticity of testing / inspection report & certificate, please contact us at telephone: (86-755) 8307 1443, or email: CN.Doccheck@sgs.com
No.10, Weiye Road, Innovation Park, Kunshan, Jiangsu, China 215300
中国·江苏·昆山市留学生创业园伟业路10号 邮编 215300

t(86-512)57355888 f(86-512)57370818 www.sgs.com.cn
t(86-512)57355888 f(86-512)57370818 sgs.china@sgs.com

1.7 D1900V2 - SN 5d136

TTL S p e a g CALIBRATION LABORATORY		CAICT																					
Add: No.52 Huayuan Road, Haidian District, Beijing, 101901 Tel: +86-10-4236403-2117 E-mail: csl@sgs.com.cn		Add: No.52 Huayuan Road, Haidian District, Beijing, 101901 Tel: +86-10-4236403-2117 E-mail: csl@sgs.com.cn																					
Client: SGS-CN		Certificate No: Z22-60185																					
CALIBRATION CERTIFICATE																							
Object: D1900V2 - SN 5d136																							
Calibration Procedure(s): FF-Z11-003-01 Calibration Procedures for dipole validation kits																							
Calibration date: June 7, 2022																							
This calibration Certificate documents the traceability to national standards, which realize the physical units of measurements (SI). The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.																							
All calibrations have been conducted in the closed laboratory facility, environment temperature (23±1)°C and humidity <70%.																							
Calibration Equipment used (M&E critical for calibration)																							
<table border="1"><thead><tr><th>Primary Standards</th><th>ID #</th><th>Cal Date (Calibrated by Certificate No.)</th><th>Scheduled Calibration</th></tr></thead><tbody><tr><td>Power Meter NRP2</td><td>106277</td><td>24-Sep-21 (CTTL No.J21X08326)</td><td>Sep-22</td></tr><tr><td>Power sensor NRP85</td><td>104291</td><td>24-Sep-21 (CTTL No.J21X08326)</td><td>Sep-22</td></tr><tr><td>Reference Probe EX3DV4</td><td>SN 7404</td><td>28-Jan-22 (SPEAG No EX3-7404_Jan22)</td><td>Jan-23</td></tr><tr><td>DAEA</td><td>SN 1558</td><td>12-Jan-22 (CTTL-SPEAG No Z22-60007)</td><td>Jan-23</td></tr></tbody></table>				Primary Standards	ID #	Cal Date (Calibrated by Certificate No.)	Scheduled Calibration	Power Meter NRP2	106277	24-Sep-21 (CTTL No.J21X08326)	Sep-22	Power sensor NRP85	104291	24-Sep-21 (CTTL No.J21X08326)	Sep-22	Reference Probe EX3DV4	SN 7404	28-Jan-22 (SPEAG No EX3-7404_Jan22)	Jan-23	DAEA	SN 1558	12-Jan-22 (CTTL-SPEAG No Z22-60007)	Jan-23
Primary Standards	ID #	Cal Date (Calibrated by Certificate No.)	Scheduled Calibration																				
Power Meter NRP2	106277	24-Sep-21 (CTTL No.J21X08326)	Sep-22																				
Power sensor NRP85	104291	24-Sep-21 (CTTL No.J21X08326)	Sep-22																				
Reference Probe EX3DV4	SN 7404	28-Jan-22 (SPEAG No EX3-7404_Jan22)	Jan-23																				
DAEA	SN 1558	12-Jan-22 (CTTL-SPEAG No Z22-60007)	Jan-23																				
<table border="1"><thead><tr><th>Secondary Standards</th><th>ID #</th><th>Cal Date (Calibrated by Certificate No.)</th><th>Scheduled Calibration</th></tr></thead><tbody><tr><td>Signal Generator E4438C</td><td>MY48071430</td><td>13-Jan-22 (CTTL No.J22X00409)</td><td>Jan-23</td></tr><tr><td>Network Analyser E5071C</td><td>MY48110073</td><td>14-Jan-22 (CTTL No.J22X00406)</td><td>Jan-23</td></tr></tbody></table>				Secondary Standards	ID #	Cal Date (Calibrated by Certificate No.)	Scheduled Calibration	Signal Generator E4438C	MY48071430	13-Jan-22 (CTTL No.J22X00409)	Jan-23	Network Analyser E5071C	MY48110073	14-Jan-22 (CTTL No.J22X00406)	Jan-23								
Secondary Standards	ID #	Cal Date (Calibrated by Certificate No.)	Scheduled Calibration																				
Signal Generator E4438C	MY48071430	13-Jan-22 (CTTL No.J22X00409)	Jan-23																				
Network Analyser E5071C	MY48110073	14-Jan-22 (CTTL No.J22X00406)	Jan-23																				
Calibrated by: Name: Zhao Jing, Function: SAR Test Engineer, Signature: [Signature]																							
Reviewed by: Lin Hao, SAR Test Engineer, Signature: [Signature]																							
Approved by: Qi Dianyan, SAR Project Leader, Signature: [Signature]																							
Issued: June 13, 2022																							
The calibration certificate shall not be reproduced except in full without written approval of the laboratory.																							
Certificate No: Z22-60185		Page 1 of 8																					

TTL S p e a g CALIBRATION LABORATORY		CAICT	
Add: No.52 Huayuan Road, Haidian District, Beijing, 101901 Tel: +86-10-4236403-2117 E-mail: csl@sgs.com.cn		Add: No.52 Huayuan Road, Haidian District, Beijing, 101901 Tel: +86-10-4236403-2117 E-mail: csl@sgs.com.cn	
Measurement Conditions		Appendix (Additional assessments outside the scope of CNAS L0570)	
DASY Version: DASY152, 52.10.4		Antenna Parameters with Head TSL	
Extrapolation: Advanced Extrapolation		Impedance, transformed to feed point: 51.0Ω ± 1.5Ω (D)	
Phantom: Triple Flat Phantom 5.1C		Return Loss: 22.4dB	
Distance Dipole Center - TSL: 10 mm, with Spacer		General Antenna Parameters and Design	
Zoom Scan Resolution: dx, dy, dz = 5 mm		Electrical Delay (one direction): 1.109 ns	
Frequency: 1900 MHz ± 1 MHz		After long term use with 100W radiated power, only a slight warming of the dipole near the feed-point can be measured.	
Head TSL parameters		The dipole is made of standard semirigid coaxial cable. The feeder conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC signals. On some of the dipoles, small caps are added to the dipole arms in order to improve matching when loaded according to the position as specified in the "Measurement Conditions" paragraph. The SAR data are not affected by this change. The overall dipole length is still according to the Standard. No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feed-point may be damaged.	
The following parameters and calculations were applied:		Additional EUT Data	
Nominal Head TSL parameters: 22.0 °C, 45.0, 1.40 return		Manufacturer by: SPEAG	
Measured Head TSL parameters: (22.0 ± 0.5) °C, 39.9 ± 0.5 %, 1.39 return ± 0.5 %			
Head TSL temperature change during test: +1.0 °C			
SAR result with Head TSL			
SAR averaged over 1 cm² (1 g) of Head TSL: Condition: 250 mW input power, 9.65 W/kg			
SAR for nominal Head TSL parameters: normalized to 1W, 40.0 W/kg ± 16.8 % (k=2)			
SAR averaged over 10 cm² (10 g) of Head TSL: Condition: 250 mW input power, 5.18 W/kg			
SAR for nominal Head TSL parameters: normalized to 1W, 20.9 W/kg ± 16.7 % (k=2)			
Certificate No: Z22-60185		Page 1 of 8	




Unless otherwise agreed in writing, this document is issued by the Company subject to its General Conditions of Service printed overleaf, available on request or accessible at <http://www.sgs.com/en/Terms-and-Conditions.aspx> and, for electronic format documents, subject to Terms and Conditions for Electronic Documents at <http://www.sgs.com/en/Terms-and-Conditions/Terms-e-Documents.aspx>. Attention is drawn to the limitation of liability, indemnification and jurisdiction issues defined therein. Any holder of this document is advised that information contained hereon reflects the Company's findings at the time of its intervention only and within the limits of Client's instructions, if any. The Company's sole responsibility is to its Client and this document does not exonerate parties to a transaction from exercising all their rights and obligations under the transaction documents. This document cannot be reproduced except in full, without prior written approval of the Company. Any unauthorized alteration, forgery or falsification of the content or appearance of this document is unlawful and offenders may be prosecuted to the fullest extent of the law. Unless otherwise stated the results shown in this test report refer only to the sample(s) tested and such sample(s) are retained for 30 days only.

Attention: To check the authenticity of testing/inspection report & certificate, please contact us at telephone: (86-755) 8307 1443, or email: CN.Doccheck@sgs.com

No.10, Weiye Road, Innovation Park, Kunshan, Jiangsu, China 215300
中国·江苏·昆山市留学生创业园伟业路10号 邮编 215300

(86-512) 57355888 (86-512) 57370818 www.sgs.com.cn
(86-512) 57355888 (86-512) 57370818 sgs.china@sgs.com

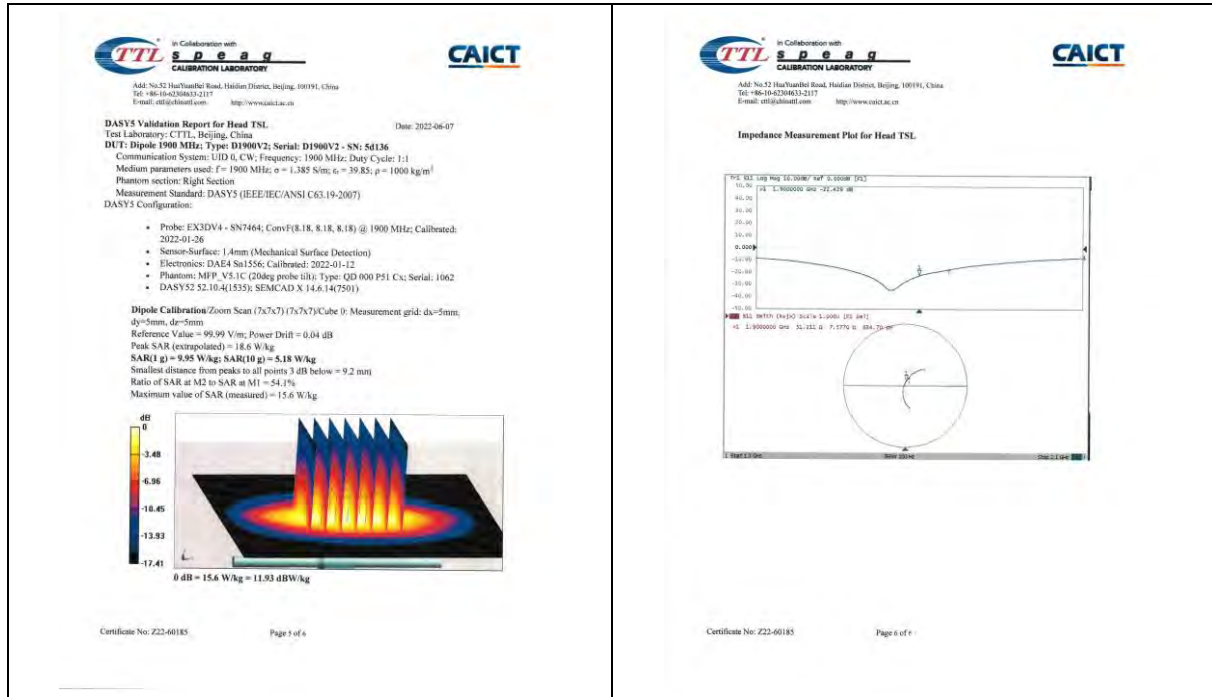

1.8 D2000V2 - SN 1041

TTLSPEAG Calibration Laboratory
 Add: No.52 Huayuan Road, Haidian District, Beijing, 100191, China
 Tel: +86-10-62586331-1117
 E-mail: cti@ttspeag.com

CAICT

Client: SGS-CN Certificate No: Z22-60186

CALIBRATION CERTIFICATE

Object: D2000V2 - SN: 1041

Calibration Procedure(s): FF-Z11-003-01
 Calibration Procedure for dipole validation kits

Calibration date: June 5, 2022

This calibration Certificate documents the traceability to national standards, which realize the physical units of measurements (SI). The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility: environment temperature (23±3)°C and humidity <70%.

Calibration Equipment used (MATE critical for calibration)

Primary Standards	ID #	Cal Date (Calibrated by Certificate No.)	Scheduled Calibration
Power Meter NRP2	106277	24-Sep-21 (CTTL No. J21X08328)	Sep-22
Power sensor NRP5	104291	24-Sep-21 (CTTL No. J21X08328)	Sep-22
Reference Probe EX3DV4	SN 7464	26-Jan-22 (SPEAG No. EX3-7464, Jan22)	Jan-23
DAE4	SN 1556	12-Jan-22 (CTTL-SPEAG No. Z22-60007)	Jan-23

Secondary Standards	ID #	Cal Date (Calibrated by Certificate No.)	Scheduled Calibration
Signal Generator E4438C	MY49071430	13-Jan-22 (CTTL No. Z22X00408)	Jan-23
Network Analyzer E5071C	MY46110673	14-Jan-22 (CTTL No. Z22X00408)	Jan-23

Calibrated by: Zhao Jing SAR Test Engineer

Reviewed by: Lin Hao SAR Test Engineer

Approved by: Qi Danyuan SAR Project Leader

Issued: June 13, 2022

This calibration certificate shall not be reproduced except in full without written approval of the laboratory.

Certificate No: Z22-60186 Page 1 of 6

TTLSPEAG Calibration Laboratory
 Add: No.52 Huayuan Road, Haidian District, Beijing, 100191, China
 Tel: +86-10-62586331-1117
 E-mail: cti@ttspeag.com

CAICT

Glossary:

TSL: Issue simulating liquid

ConvF: sensitivity in TSL / NORMx.y.z

N/A: not applicable or not measured

Calibration is Performed According to the Following Standards:

a) IEC/IEEE 62209-1528, "Measurement Procedure for The Assessment of Specific Absorption Rate of Human Exposure to Radio Frequency Fields from Hand-Head and Body-Mounted Wireless Communication Devices: Part 1528 Human Models, Instrumentation and Procedures (Frequency range of 4 MHz to 10 GHz)", October 2020

b) KDB 865564, "SAR Measurement Requirements for 100 MHz to 6 GHz"

Additional Documentation:

c) DASY4/S System Handbook

Methods Applied and Interpretation of Parameters:

- Measurement Conditions: Further details are available from the Validation Report at the end of the certificate. All figures stated in the certificate are valid at the frequency indicated.
- Antenna Parameter with TSL: The dipole is mounted with the spacer to position its feed point exactly below the center marking of the flat phantom section, with the arms oriented parallel to the body axis.
- Feed Point Impedance and Return Loss: These parameters are measured with the dipole positioned under the liquid filled phantom. The impedance stated is transformed from the measurement at the SMA connector to the feed point. The Return Loss ensures low reflected power. No uncertainty required.
- Electrical Delay: One-way delay between the SMA connector and the antenna feed point. No uncertainty required.
- SAR measured: SAR measured at the stated antenna input power.
- SAR normalized: SAR as measured, normalized to an input power of 1 W at the antenna connector.
- SAR for nominal TSL parameters: The measured TSL parameters are used to calculate the nominal SAR result.

The reported uncertainty of measurement is stated as the standard uncertainty of Measurement multiplied by the coverage factor k=2, which for a normal distribution corresponds to a coverage probability of approximately 95%.

Certificate No: Z22-60186 Page 2 of 6



Unless otherwise agreed in writing, this document is issued by the Company subject to its General Conditions of Service printed overleaf, available on request or accessible at <http://www.sgs.com/en/Terms-and-Conditions.aspx>; and, for electronic format documents, subject to Terms and Conditions for Electronic Documents at <http://www.sgs.com/en/Terms-and-Conditions/Terms-e-Documents.aspx>. Attention is drawn to the limitation of liability, indemnification and jurisdiction issues defined therein. Any holder of this document is advised that information contained hereon reflects the Company's findings at the time of its intervention only and within the limits of Client's instructions, if any. The Company's sole responsibility is to its Client and this document does not exonerate parties to a transaction from exercising all their rights and obligations under the transaction documents. This document cannot be reproduced except in full, without prior written approval of the Company. Any unauthorized alteration, forgery or falsification of the content or appearance of this document is unlawful and offenders may be prosecuted to the fullest extent of the law. Unless otherwise stated the results shown in this test report refer only to the sample(s) tested and such sample(s) are retained for 30 days only.


Attention: To check the authenticity of testing / inspection report & certificate, please contact us at telephone: (86-755) 8307 1443, or email: CN.Doccheck@sgs.com


No.10, Weiye Road, Innovation Park, Kunshan, Jiangsu, China 215300
 中国·江苏·昆山市留学生创业园伟业路10号 邮编 215300

(86-512)57355888 (86-512)57370818 www.sgsgroup.com.cn
 (86-512)57355888 (86-512)57370818 sgs.china@sgs.com

In Collaboration with TTL s p e a g CALIBRATION LABORATORY		CAICT	
Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China Tel: +86-10-6204832-2117 E-mail: en@sgs.com.cn http://www.sgscert.com.cn			
Measurement Conditions DASY system configuration, as for as not given on page 1.			
DASY Version	DASYV2	52.10.4	
Extrapolation	Advanced Extrapolation		
Phantom	Triple Flat Phantom S.1C		
Distance Dipole Center - TSL	10 mm	with Spacer	
Zoom Scan Resolution	dx, dy, dz = 5 mm		
Frequency	2000 MHz ± 1 MHz		
Head TSL parameters The following parameters and calculations were applied:			
Nominal Head TSL parameters	Temperature	Permittivity	Conductivity
	22.9 °C	40.0	1.40 mho/cm
Measured Head TSL parameters	(22.0 ± 0.2) °C	40.2 ± 0.6 %	1.36 mho/cm ± 0.6 %
Head TSL temperature change during test	<1.0 °C		
SAR result with Head TSL			
SAR averaged over 1 cm ³ (1 g) of Head TSL	Condition		
SAR measured	250 mW input power	10.4 W/kg	
SAR for nominal Head TSL parameters	normalized to 1W	41.8 W/kg ± 15.8 % (n=2)	
SAR averaged over 10 cm ³ (10 g) of Head TSL	Condition		
SAR measured	250 mW input power	5.30 W/kg	
SAR for nominal Head TSL parameters	normalized to 1W	21.3 W/kg ± 18.7 % (n=2)	
Certificate No: Z22-60186 Page 3 of 6			

In Collaboration with TTL s p e a g CALIBRATION LABORATORY		CAICT	
Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China Tel: +86-10-6204832-2117 E-mail: en@sgs.com.cn http://www.sgscert.com.cn			
Appendix (Additional assessments outside the scope of CNAS L0570)			
Antenna Parameters with Head TSL			
Impedance, transformed to feed point	48.4Ω ± 0.74Ω		
Return Loss	-34.8dB		
General Antenna Parameters and Design			
Electrical Delay (one direction)	1.08 ns		
After long term use with 100W radiated power, only a slight warming of the dipole near the feed-point can be measured.			
The dipole is made of standard semi-rigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals. On some of the dipoles, small and large are added to the dipole arms in order to improve matching when loaded according to the position as explained in the "Measurement Conditions" paragraph. The SAR data are not affected by this change. The overall dipole length is still according to the Standard.			
No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feed-point may be damaged.			
Additional EUT Data			
Manufactured by	SPEAG		
Certificate No: Z22-60188 Page 8 of 8			

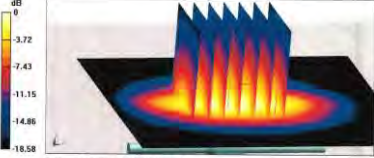In Collaboration with TTL s p e a g CALIBRATION LABORATORY		CAICT	
Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China Tel: +86-10-6204832-2117 E-mail: en@sgs.com.cn http://www.sgscert.com.cn			
DASY Validation Report for Head TSL Test Laboratory: CTTL, Beijing, China DUT: Dipole 2000 MHz; Type: D2000V2; Serial: D2000V2 - SN: 1041 Communication System: UTD 0; CW; Frequency: 2000 MHz; Duty Cycle: 1:1 Medium parameters used: f = 2000 MHz; σ = 1.392 S/m; ε = 40.21; ρ = 1000 kg/m ³ Phantom section: Right Section Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2007) DASY5 Configuration:			
• Probe: EX3DV4 - SN7464; ConvF(R2, R2, R2) @ 2000 MHz; Calibrated: 2022-01-26			
• Sensor Surface: 1.4mm (Mechanical Surface Detection)			
• Electronics: DA64 Sn1556; Calibrated: 2022-01-12			
• Phantom: MPP_V5.1C (20deg probe tilt); Type: QD 000 P51 Cx; Serial: 1062			
• DASY5: S2.10.4(1535); SEMCAD X 14.6.14(7501)			
Dipole Calibration/Zoom Scan (7x7x7) (7x7x7) Cube (0; Measurement grid: dx=5mm, dy=5mm, dz=5mm) Reference Value = 103.4 V/m; Power Drift = 0.03 dB Peak SAR (extrapolated) = 19.6 W/kg SAR(1 g) = 10.4 W/kg; SAR(10 g) = 5.3 W/kg Smallest distance from peaks to all points 3 dB below = 9.1 mm Ratio of SAR at M2 to SAR at M1 = 51.0%			
Maximum value of SAR (measured) = 16.3 W/kg			
			
0 dB = 16.3 W/kg = 12.12 dBW/kg			
Certificate No: Z22-60186 Page 5 of 6			

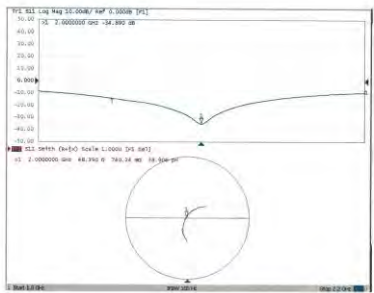In Collaboration with TTL s p e a g CALIBRATION LABORATORY		CAICT	
Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China Tel: +86-10-6204832-2117 E-mail: en@sgs.com.cn http://www.sgscert.com.cn			
Impedance Measurement Plot for Head TSL			
			
Certificate No: Z22-60188 Page 6 of 6			



Unless otherwise agreed in writing, this document is issued by the Company subject to its General Conditions of Service printed overleaf, available on request or accessible at <http://www.sgs.com/en/Terms-and-Conditions.aspx> and, for electronic format documents, subject to Terms and Conditions for Electronic Documents at <http://www.sgs.com/en/Terms-and-Conditions/Terms-e-Documents.aspx>. Attention is drawn to the limitation of liability, indemnification and jurisdiction issues defined therein. Any holder of this document is advised that information contained hereon reflects the Company's findings at the time of its intervention only and within the limits of Client's instructions, if any. The Company's sole responsibility is to its Client and this document does not exonerate parties to a transaction from exercising all their rights and obligations under the transaction documents. This document cannot be reproduced except in full, without prior written approval of the Company. Any unauthorized alteration, forgery or falsification of the content or appearance of this document is unlawful and offenders may be prosecuted to the fullest extent of the law. Unless otherwise stated the results shown in this test report refer only to the sample(s) tested and such sample(s) are retained for 30 days only.

Attention: To check the authenticity of testing / inspection report & certificate, please contact us at telephone: (86-755) 8307 1443, or email: CN.Doccheck@sgs.com

No.10, Weiye Road, Innovation Park, Kunshan, Jiangsu, China 215300
中国·江苏·昆山市留学生创业园伟业路10号 邮编 215300

t(86-512)57355888 f(86-512)57370818 www.sgsgroup.com.cn
t(86-512)57355888 f(86-512)57370818 sgs.china@sgs.com

1.9 D2300V2 - SN 1096


TTL Speaq CALIBRATION LABORATORY		CAICT	
Add: No.52 HuaYuanbei Road, Haidian District, Beijing, 100191, China Tel: +86-10-6230433-2512 Fax: +86-10-6230433-2504 E-mail: cti@chinaul.com http://www.chinaul.cn		Add: No.52 HuaYuanbei Road, Haidian District, Beijing, 100191, China Tel: +86-10-6230433-2579 Fax: +86-10-6230433-2504 E-mail: cti@chinaul.com http://www.chinaul.cn	
Client: SGS-CN		Certificate No: Z22-60106	
CALIBRATION CERTIFICATE			
Object	D2300V2 - SN 1096		
Calibration Procedure(s)	FF-Z11-003-01 Calibration Procedures for dipole validation kits		
Calibration date:	March 31, 2022		
This calibration Certificate documents the traceability to national standards, which realize the physical units of measurements (SI). The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.			
All calibrations have been conducted in the closed laboratory facility: environment temperature (22±3)°C and humidity <70%.			
Calibration Equipment used (M&TE critical for calibration)			
Primary Standards	ID #	Cal Date (Calibrated by Certificate No.)	Scheduled Calibration
Power Meter NRP2	108277	24-Sep-21 (CTTL No.J21X08328)	Sep-22
Power sensor NRP8	104291	24-Sep-21 (CTTL No.J21X08328)	Sep-22
Reference Probe EX30V4	SN 7307	26-May-21 (SPEAG No.EK3-7307_May21)	May-22
DAE4	SN 1556	12-Jan-22 (CTTL-SPEAG No.Z22-60007)	Jan-23
Secondary Standards	ID #	Cal Date (Calibrated by Certificate No.)	Scheduled Calibration
Signal Generator E4438C	MY49071430	13-Jan-22 (CTTL No.J22X00406)	Jan-23
Network Analyzer E5071C	MY48110673	14-Jan-22 (CTTL No.J22X00406)	Jan-23
Calibrated by:	Name	Function	Signature
	Zhao Jing	SAR Test Engineer	
Reviewed by:	Lin Hao	SAR Test Engineer	
Approved by:	Qi Dianyan	SAR Project Leader	
Issued: April 6, 2022			
This calibration certificate shall not be reproduced except in full without written approval of the laboratory			
Certificate No: Z22-60106		Page 1 of 6	
TTL Speaq CALIBRATION LABORATORY		CAICT	
Add: No.52 HuaYuanbei Road, Haidian District, Beijing, 100191, China Tel: +86-10-6230433-2579 Fax: +86-10-6230433-2504 E-mail: cti@chinaul.com http://www.chinaul.cn		Add: No.52 HuaYuanbei Road, Haidian District, Beijing, 100191, China Tel: +86-10-6230433-2579 Fax: +86-10-6230433-2504 E-mail: cti@chinaul.com http://www.chinaul.cn	
Measurement Conditions DASY system configuration, as far as not given on page 1:			
DASY Version	DASY2	52.10.4	
Extrapolation	Advanced Extrapolation		
Phantom	Triple Flat Phantom 5.1C		
Distance Dipole Center - TSL	10 mm	with Spacer	
Zoom Scan Resolution	dx, dy, dz = 5 mm		
Frequency	2300 MHz ± 1 MHz		
Head TSL parameters The following parameters and calculations were applied:			
	Temperature	Permittivity	Conductivity
Nominal Head TSL parameters	22.0 °C	39.5	1.67 mho/m
Measured Head TSL parameters	(22.0 ± 0.2) °C	39.8 ± 9 %	1.70 mho/m ± 6 %
Head TSL temperature change during test	<1.0 °C	—	
SAR result with Head TSL			
SAR averaged over 1 cm ² (1 g) of Head TSL	Condition		
SAR measured	250 mW input power	12.4 W/kg	
SAR for nominal Head TSL parameters	normalized to 1W	49.2 W/kg ± 18.8 % (k=2)	
SAR averaged over 10 cm ² (10 g) of Head TSL	Condition		
SAR measured	250 mW input power	5.88 W/kg	
SAR for nominal Head TSL parameters	normalized to 1W	23.4 W/kg ± 18.7 % (k=2)	
Certificate No: Z22-60106		Page 3 of 6	
TTL Speaq CALIBRATION LABORATORY		CAICT	
Add: No.52 HuaYuanbei Road, Haidian District, Beijing, 100191, China Tel: +86-10-6230433-2579 Fax: +86-10-6230433-2504 E-mail: cti@chinaul.com http://www.chinaul.cn		Add: No.52 HuaYuanbei Road, Haidian District, Beijing, 100191, China Tel: +86-10-6230433-2579 Fax: +86-10-6230433-2504 E-mail: cti@chinaul.com http://www.chinaul.cn	
Appendix (Additional assessments outside the scope of CNAS L0570)			
Antenna Parameters with Head TSL			
Impedance, transformed to feed point	49.20 - 4.50j		
Return Loss	-26.6dB		
General Antenna Parameters and Design			
Electrical Delay (one direction)	1.083 ns		
After long term use with 100W radiated power, only a slight warming of the dipole near the feed-point can be measured.			
The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals. On some of the dipoles, small end caps are added to the dipole arms in order to improve matching when backed according to the position as explained in the "Measurement Conditions" paragraph. The SAR data are not affected by this change. The overall dipole length is still according to the Standard. No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feed-point may be damaged.			
Additional EUT Data			
Manufactured by	SPEAG		
Certificate No: Z22-60106		Page 4 of 6	



Unless otherwise agreed in writing, this document is issued by the Company subject to its General Conditions of Service printed overleaf, available on request or accessible at <http://www.sgs.com/en/Terms-and-Conditions.aspx>; and, for electronic format documents, subject to Terms and Conditions for Electronic Documents at <http://www.sgs.com/en/Terms-and-Conditions/Terms-e-Documents.aspx>. Attention is drawn to the limitation of liability, indemnification and jurisdiction issues defined therein. Any holder of this document is advised that information contained hereon reflects the Company's findings at the time of its intervention only and within the limits of Client's instructions, if any. The Company's sole responsibility is to its Client and this document does not exonerate parties to a transaction from exercising all their rights and obligations under the transaction documents. This document cannot be reproduced except in full, without prior written approval of the Company. Any unauthorized alteration, forgery or falsification of the content or appearance of this document is unlawful and offenders may be prosecuted to the fullest extent of the law. Unless otherwise stated the results shown in this test report refer only to the sample(s) tested and such sample(s) are retained for 30 days only.

Attention: To check the authenticity of testing/inspection report & certificate, please contact us at telephone: (86-755) 8307 1443, or email: CN.Doccheck@sgs.com
No.10, Weiye Road, Innovation Park, Kunshan, Jiangsu, China 215300
中国·江苏·昆山市留学生创业园伟业路10号 邮编 215300

(86-512)57355888 (86-512)57370818 www.sgs.com.cn
(86-512)57355888 (86-512)57370818 sgs.china@sgs.com

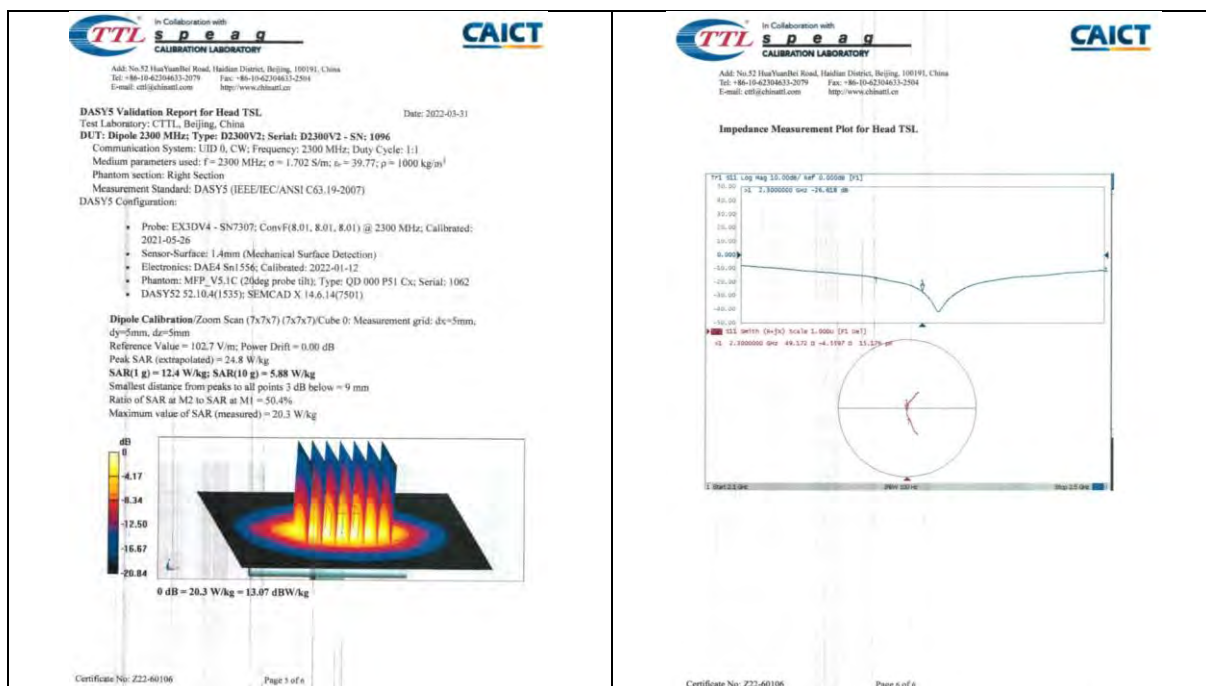

1.10 D2450V2 - SN 817

TTL *speaq* **CAICT**

Address: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China
Tel: +86-10-42504633-3079 Fax: +86-10-42504633-2504
E-mail: cti@china.ttl.com http://www.china.ttl.com

Client: **SGS-CN** Certificate No: **Z22-60107**

CALIBRATION CERTIFICATE

Object: **D2450V2 - SN 817**

Calibration Procedure(s): **FF-Z11-003-3**
Calibration Procedures for dipole validation kits

Calibration date: **April 1, 2022**

This calibration Certificate documents the traceability to national standards, which realize the physical units of measurements [B]. The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility: environment temperature (22±3)°C and humidity <70%.

Calibration Equipment used (M&E critical for calibration)

Primary Standards	ID #	Cal Date (Calibrated by: Certificate No.)	Scheduled Calibration
Power Meter: NRP2	106277	24-Sep-21 (CTTL No.J21X08320)	Sep-22
Power sensor: NRP8S	104291	24-Sep-21 (CTTL No.J21X08320)	Sep-22
Reference Probe EX3DV4	SN 7307	25-May-21(SPEAG No EX3-7307_May21)	May-22
DAE4	SN 1555	12-Jan-22(CTTL-SPEAG No Z22-60007)	Jan-23

Secondary Standards	ID #	Cal Date (Calibrated by: Certificate No.)	Scheduled Calibration
Signal Generator E4438C	MY49071430	13-Jan-22 (CTTL No.J22X00406)	Jan-23
Network Analyzer E5071C	MY46110673	14-Jan-22 (CTTL No.J22X00406)	Jan-23

Calibrated by: **Zhao Jing** SAR Test Engineer

Reviewed by: **Liu Hao** SAR Test Engineer

Approved by: **Qi Dianyan** SAR Project Leader

Issued: April 6, 2022

This calibration certificate shall not be reproduced except in full without written approval of the laboratory.

Certificate No: Z22-60107 Page 1 of 5

TTL *speaq* **CAICT**

Address: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China
Tel: +86-10-42504633-3079 Fax: +86-10-42504633-2504
E-mail: cti@china.ttl.com http://www.china.ttl.com

Glossary:

TSL: tissue simulating liquid
ConvF: sensitivity in TSL / NORMix.y.z
N/A: not applicable or not measured

Calibration is Performed According to the Following Standards:

a) IEC/IEEE 62209-1528, "Measurement Procedure for The Assessment of Specific Absorption Rate of Human Exposure to Radio Frequency Fields from Hand-held and Body-mounted Wireless Communication Devices- Part 1528: Human Models, Instrumentation and Procedures (Frequency range of 4 MHz to 10 GHz)", October 2020
b) KDB 865664, "SAR Measurement Requirements for 100 MHz to 5 GHz"

Additional Documentation:

c) DASY4/5 System Handbook

Methods Applied and Interpretation of Parameters:

- Measurement Conditions:** Further details are available from the Validation Report at the end of the certificate. All figures stated in the certificate are valid at the frequency indicated.
- Antenna Parameters with TSL:** The dipole is mounted with the spacer to position its feed point exactly below the center marking of the flat phantom section, with the arms oriented parallel to the body axis.
- Feed Point Impedance and Return Loss:** These parameters are measured with the dipole positioned under the liquid filled phantom. The impedance stated is transformed from the measurement at the SMA connector to the feed point. The Return Loss ensures low reflected power. No uncertainty required.
- Electrical Delay:** One-way delay between the SMA connector and the antenna feed point. No uncertainty required.
- SAR measured:** SAR measured at the stated antenna input power.
- SAR normalized:** SAR as measured, normalized to an input power of 1 W at the antenna connector.
- SAR for nominal TSL parameters:** The measured TSL parameters are used to calculate the nominal SAR result.

The reported uncertainty of measurement is stated as the standard uncertainty of Measurement multiplied by the coverage factor: $k=2$, which for a normal distribution Corresponds to a coverage probability of approximately 95%.

Certificate No: Z22-60107 Page 2 of 5





Unless otherwise agreed in writing, this document is issued by the Company subject to its General Conditions of Service printed overleaf, available on request or accessible at <http://www.sgs.com/en/Terms-and-Conditions.aspx> and, for electronic format documents, subject to Terms and Conditions for Electronic Documents at <http://www.sgs.com/en/Terms-and-Conditions/Terms-e-Documents.aspx>. Attention is drawn to the limitation of liability, indemnification and jurisdiction issues defined therein. Any holder of this document is advised that information contained hereon reflects the Company's findings at the time of its intervention only and within the limits of Client's instructions, if any. The Company's sole responsibility is to its Client and this document does not exonerate parties to a transaction from exercising all their rights and obligations under the transaction documents. This document cannot be reproduced except in full, without prior written approval of the Company. Any unauthorized alteration, forgery or falsification of the content or appearance of this document is unlawful and offenders may be prosecuted to the fullest extent of the law. Unless otherwise stated the results shown in this test report refer only to the sample(s) tested and such sample(s) are retained for 30 days only.

Attention: To check the authenticity of testing/inspection report & certificate, please contact us at telephone: (86-755) 8307 1443, or email: CN.Doccheck@sgs.com

No.10, Weiye Road, Innovation Park, Kunshan, Jiangsu, China 215300
中国·江苏·昆山市留学生创业园伟业路10号 邮编 215300

t(86-512)57355888 f(86-512)57370818 www.sgsgroup.com.cn
t(86-512)57355888 f(86-512)57370818 sgs.china@sgs.com

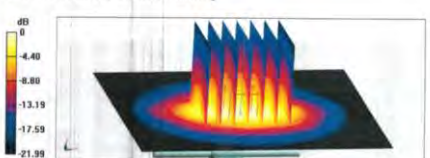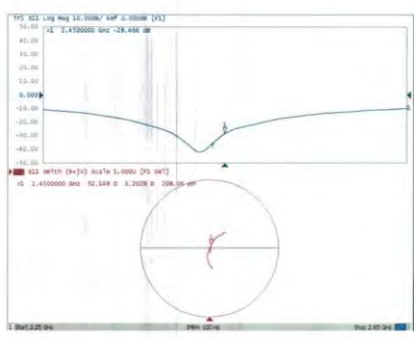TTL Speaq CALIBRATION LABORATORY		CAICT																		
Address: No. 52 HuaYuanBei Road, Haidian District, Beijing, 100191, China Tel: +86-10-42304633-2079 Fax: +86-10-42304633-2504 E-mail: cti@chinaul.com.cn http://www.chinaul.com.cn																				
Measurement Conditions DASY system configuration, as far as not given on page 1: <table border="1"> <tr> <td>DASY Version</td> <td>DASY52</td> <td>52.10.4</td> </tr> <tr> <td>Extrapolation</td> <td>Advanced Extrapolation</td> <td></td> </tr> <tr> <td>Phantom</td> <td>Triple Flat Phantom 5.1C</td> <td></td> </tr> <tr> <td>Distance Dipole Center - TSL</td> <td>10 mm</td> <td>with Spacer</td> </tr> <tr> <td>Zoom Scan Resolution</td> <td>dx, dy, dz = 5 mm</td> <td></td> </tr> <tr> <td>Frequency</td> <td>2450 MHz ± 1 MHz</td> <td></td> </tr> </table>			DASY Version	DASY52	52.10.4	Extrapolation	Advanced Extrapolation		Phantom	Triple Flat Phantom 5.1C		Distance Dipole Center - TSL	10 mm	with Spacer	Zoom Scan Resolution	dx, dy, dz = 5 mm		Frequency	2450 MHz ± 1 MHz	
DASY Version	DASY52	52.10.4																		
Extrapolation	Advanced Extrapolation																			
Phantom	Triple Flat Phantom 5.1C																			
Distance Dipole Center - TSL	10 mm	with Spacer																		
Zoom Scan Resolution	dx, dy, dz = 5 mm																			
Frequency	2450 MHz ± 1 MHz																			
Head TSL parameters The following parameters and calculations were applied: <table border="1"> <tr> <th></th> <th>Temperature</th> <th>Permittivity</th> <th>Conductivity</th> </tr> <tr> <td>Nominal Head TSL parameters</td> <td>22.0 °C</td> <td>39.2</td> <td>1.80 mho/m</td> </tr> <tr> <td>Measured Head TSL parameters</td> <td>(22.0 ± 0.2) °C</td> <td>39.5 ± 6 %</td> <td>1.79 mho/m ± 8 %</td> </tr> <tr> <td>Head TSL temperature change during test</td> <td><1.0 °C</td> <td>—</td> <td>—</td> </tr> </table>				Temperature	Permittivity	Conductivity	Nominal Head TSL parameters	22.0 °C	39.2	1.80 mho/m	Measured Head TSL parameters	(22.0 ± 0.2) °C	39.5 ± 6 %	1.79 mho/m ± 8 %	Head TSL temperature change during test	<1.0 °C	—	—		
	Temperature	Permittivity	Conductivity																	
Nominal Head TSL parameters	22.0 °C	39.2	1.80 mho/m																	
Measured Head TSL parameters	(22.0 ± 0.2) °C	39.5 ± 6 %	1.79 mho/m ± 8 %																	
Head TSL temperature change during test	<1.0 °C	—	—																	
SAR result with Head TSL <table border="1"> <tr> <th>SAR averaged over 1 cm³ (1 g) of Head TSL</th> <th>Condition</th> <th></th> </tr> <tr> <td>SAR measured</td> <td>250 mW input power</td> <td>13.2 W/kg</td> </tr> <tr> <td>SAR for nominal Head TSL parameters</td> <td>normalized to 1W</td> <td>53.0 W/kg ± 18.8 % (k=2)</td> </tr> <tr> <th>SAR averaged over 10 cm³ (10 g) of Head TSL</th> <th>Condition</th> <th></th> </tr> <tr> <td>SAR measured</td> <td>250 mW input power</td> <td>6.15 W/kg</td> </tr> <tr> <td>SAR for nominal Head TSL parameters</td> <td>normalized to 1W</td> <td>24.7 W/kg ± 18.7 % (k=2)</td> </tr> </table>			SAR averaged over 1 cm ³ (1 g) of Head TSL	Condition		SAR measured	250 mW input power	13.2 W/kg	SAR for nominal Head TSL parameters	normalized to 1W	53.0 W/kg ± 18.8 % (k=2)	SAR averaged over 10 cm ³ (10 g) of Head TSL	Condition		SAR measured	250 mW input power	6.15 W/kg	SAR for nominal Head TSL parameters	normalized to 1W	24.7 W/kg ± 18.7 % (k=2)
SAR averaged over 1 cm ³ (1 g) of Head TSL	Condition																			
SAR measured	250 mW input power	13.2 W/kg																		
SAR for nominal Head TSL parameters	normalized to 1W	53.0 W/kg ± 18.8 % (k=2)																		
SAR averaged over 10 cm ³ (10 g) of Head TSL	Condition																			
SAR measured	250 mW input power	6.15 W/kg																		
SAR for nominal Head TSL parameters	normalized to 1W	24.7 W/kg ± 18.7 % (k=2)																		
Appendix (Additional assessments outside the scope of CNAS L0570) Antenna Parameters with Head TSL <table border="1"> <tr> <td>Impedance, transformed to feed point</td> <td>52.10 ± 3.20j</td> </tr> <tr> <td>Return Loss</td> <td>~26.5dB</td> </tr> </table> General Antenna Parameters and Design <table border="1"> <tr> <td>Electrical Delay (one direction)</td> <td>1.006 ns</td> </tr> </table> After long term use with 100W radiated power, only a slight warming of the dipole near the feed-point can be measured. The dipole is made of standard serringid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals. On some of the dipoles, small end caps are added to the dipole arms in order to improve matching when loaded according to the position as explained in the "Measurement Conditions" paragraph. The SAR data are not affected by this change. The overall dipole length is still according to the Standard. No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feed-point may be damaged. Additional EUT Data <table border="1"> <tr> <td>Manufactured by</td> <td>SPEAG</td> </tr> </table>			Impedance, transformed to feed point	52.10 ± 3.20j	Return Loss	~26.5dB	Electrical Delay (one direction)	1.006 ns	Manufactured by	SPEAG										
Impedance, transformed to feed point	52.10 ± 3.20j																			
Return Loss	~26.5dB																			
Electrical Delay (one direction)	1.006 ns																			
Manufactured by	SPEAG																			
Certificate No: Z22-40107 Page 3 of 6																				
TTL Speaq CALIBRATION LABORATORY Address: No. 52 HuaYuanBei Road, Haidian District, Beijing, 100191, China Tel: +86-10-42304633-2079 Fax: +86-10-42304633-2504 E-mail: cti@chinaul.com.cn http://www.chinaul.com.cn																				
DASY5 Validation Report for Head TSL Date: 2022-04-01 Test Laboratory: CTTL, Beijing, China DUT: Dipole 2450 MHz; Type: D2450V2; Serial: D2450V2 - SN: 817 Communication System: UTD 0, CW; Frequency: 2450 MHz; Duty Cycle: 1:1 Medium parameters used: f = 2450 MHz; σ = 1.79 S/m; ε = 39.52; ρ = 1000 kg/m³ Phantom section: Right Section Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2007) DASY5 Configuration: - Probe: EX3DV4 - SN7307; ConvF(7.75, 7.75) @ 2450 MHz; Calibrated: 2021-05-26 - Sensor-Surface: 1.4mm (Mechanical Surface Detection) - Electronics: DA14 Snt 556; Calibrated: 2022-01-12 - Phantom: MFP, V5.1C (20deg probe tilt); Type: QD 000 P51 Cx; Serial: 1062 - DASY52 52.10.4(1535); SEMCAD X 14.6.14(7501) Dipole Calibration/Zoom Scan (7x7x7) (7x7x7)/Cube 0: Measurement grid: dx=5mm, dy=5mm, dz=5mm Reference Value = 104.6 V/m; Power Drift = -0.03 dB Peak SAR (extrapolated) = 27.0 W/kg SAR(1 g) = 13.2 W/kg; SAR(10 g) = 6.15 W/kg Smallest distance from peaks to all points 3 dB below = 8.9 mm Ratio of SAR at M2 to SAR at M1 = -49.2% Maximum value of SAR (measured) = 22.1 W/kg  0 dB = 22.1 W/kg = 13.44 dBW/kg																				
Certificate No: Z22-40107 Page 4 of 6																				
TTL Speaq CALIBRATION LABORATORY Address: No. 52 HuaYuanBei Road, Haidian District, Beijing, 100191, China Tel: +86-10-42304633-2079 Fax: +86-10-42304633-2504 E-mail: cti@chinaul.com.cn http://www.chinaul.com.cn																				
Impedance Measurement Plot for Head TSL 																				
Certificate No: Z22-40107 Page 5 of 6																				



Unless otherwise agreed in writing, this document is issued by the Company subject to its General Conditions of Service printed overleaf, available on request or accessible at <http://www.sgs.com/en/Terms-and-Conditions.aspx> and, for electronic format documents, subject to Terms and Conditions for Electronic Documents at <http://www.sgs.com/en/Terms-and-Conditions/Terms-e-Document.aspx>. Attention is drawn to the limitation of liability, indemnification and jurisdiction issues defined therein. Any holder of this document is advised that information contained hereon reflects the Company's findings at the time of its intervention only and within the limits of Client's instructions, if any. The Company's sole responsibility is to its Client and this document does not exonerate parties to a transaction from exercising all their rights and obligations under the transaction documents. This document cannot be reproduced except in full, without prior written approval of the Company. Any unauthorized alteration, forgery or falsification of the content or appearance of this document is unlawful and offenders may be prosecuted to the fullest extent of the law. Unless otherwise stated the results shown in this test report refer only to the sample(s) tested and such sample(s) are retained for 30 days only.

Attention: To check the authenticity of testing / inspection report & certificate, please contact us at telephone: (86-755) 8307 1443, or email: CN.Doccheck@sgs.com
No. 10, Weyue Road, Innovation Park, Kunshan, Jiangsu, China 215300
中国·江苏·昆山市留学生创业园伟业路10号 邮编 215300

t(86-512)57355888 t(86-512)57370818 www.sgs.com
t(86-512)57355888 t(86-512)57370818 sgs.china@sgs.com

1.11 D2600V2 - SN 1158

TTL S p e a g CALIBRATION LABORATORY		CAICT																					
Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191 Tel: +86-10-42304633-2512 Fax: +86-10-42304633-2504 E-mail: cti@sgs.com.cn http://www.sgslab.com.cn		Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191 Tel: +86-10-42304633-2079 Fax: +86-10-42304633-2504 E-mail: cti@sgs.com.cn http://www.sgslab.com.cn																					
Client: SGS-CN		Certificate No: Z22-40108																					
CALIBRATION CERTIFICATE																							
Object: D2600V2 - SN: 1158																							
Calibration Procedure(s): FF-Z11-003-01 Calibration Procedures for dipole validation kits																							
Calibration date: March 31, 2022																							
This calibration Certificate documents the traceability to national standards, which realize the physical units of measurements (SI). The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.																							
All calibrations have been conducted in the closed laboratory facility: environment temperature (23±3)°C and humidity <70%.																							
Calibration Equipment used (MSTE critical for calibration)																							
<table border="1"><thead><tr><th>Primary Standards</th><th>ID #</th><th>Cal Date (Calibrated by Certificate No.)</th><th>Scheduled Calibration</th></tr></thead><tbody><tr><td>Power Meter NRP2</td><td>102377</td><td>24-Sep-21 (CTTL No.J21X08326)</td><td>Sep-22</td></tr><tr><td>Power sensor NRP8S</td><td>104291</td><td>24-Sep-21 (CTTL No.J21X08326)</td><td>Sep-22</td></tr><tr><td>Reference Probe EX3/DVA</td><td>SN 7307</td><td>26-May-21 (SPEAG No.EX3-7307_May21)</td><td>May-22</td></tr><tr><td>DAE4</td><td>SN 1556</td><td>12-Jan-22 (CTTL-SPEAG No.Z22-60007)</td><td>Jan-23</td></tr></tbody></table>				Primary Standards	ID #	Cal Date (Calibrated by Certificate No.)	Scheduled Calibration	Power Meter NRP2	102377	24-Sep-21 (CTTL No.J21X08326)	Sep-22	Power sensor NRP8S	104291	24-Sep-21 (CTTL No.J21X08326)	Sep-22	Reference Probe EX3/DVA	SN 7307	26-May-21 (SPEAG No.EX3-7307_May21)	May-22	DAE4	SN 1556	12-Jan-22 (CTTL-SPEAG No.Z22-60007)	Jan-23
Primary Standards	ID #	Cal Date (Calibrated by Certificate No.)	Scheduled Calibration																				
Power Meter NRP2	102377	24-Sep-21 (CTTL No.J21X08326)	Sep-22																				
Power sensor NRP8S	104291	24-Sep-21 (CTTL No.J21X08326)	Sep-22																				
Reference Probe EX3/DVA	SN 7307	26-May-21 (SPEAG No.EX3-7307_May21)	May-22																				
DAE4	SN 1556	12-Jan-22 (CTTL-SPEAG No.Z22-60007)	Jan-23																				
<table border="1"><thead><tr><th>Secondary Standards</th><th>ID #</th><th>Cal Date (Calibrated by Certificate No.)</th><th>Scheduled Calibration</th></tr></thead><tbody><tr><td>Signal Generator E4438C</td><td>MY48071430</td><td>13-Jan-22 (CTTL No.Z22X00406)</td><td>Jan-23</td></tr><tr><td>Network Analyzer E5071C</td><td>MY48110673</td><td>14-Jan-22 (CTTL No.Z22X00406)</td><td>Jan-23</td></tr></tbody></table>				Secondary Standards	ID #	Cal Date (Calibrated by Certificate No.)	Scheduled Calibration	Signal Generator E4438C	MY48071430	13-Jan-22 (CTTL No.Z22X00406)	Jan-23	Network Analyzer E5071C	MY48110673	14-Jan-22 (CTTL No.Z22X00406)	Jan-23								
Secondary Standards	ID #	Cal Date (Calibrated by Certificate No.)	Scheduled Calibration																				
Signal Generator E4438C	MY48071430	13-Jan-22 (CTTL No.Z22X00406)	Jan-23																				
Network Analyzer E5071C	MY48110673	14-Jan-22 (CTTL No.Z22X00406)	Jan-23																				
<table border="1"><thead><tr><th>Calibrated by:</th><th>Name</th><th>Function</th><th>Signature</th></tr></thead><tbody><tr><td></td><td>Zhao Jing</td><td>SAR Test Engineer</td><td></td></tr><tr><td>Reviewed by:</td><td>Lin Hao</td><td>SAR Test Engineer</td><td></td></tr><tr><td>Approved by:</td><td>Qi Dianyan</td><td>SAR Project Leader</td><td></td></tr></tbody></table>				Calibrated by:	Name	Function	Signature		Zhao Jing	SAR Test Engineer		Reviewed by:	Lin Hao	SAR Test Engineer		Approved by:	Qi Dianyan	SAR Project Leader					
Calibrated by:	Name	Function	Signature																				
	Zhao Jing	SAR Test Engineer																					
Reviewed by:	Lin Hao	SAR Test Engineer																					
Approved by:	Qi Dianyan	SAR Project Leader																					
Issued: April 6, 2022																							
This calibration certificate shall not be reproduced except in full without written approval of the laboratory.																							
Certificate No: Z22-40108		Page 1 of 6																					

TTL S p e a g CALIBRATION LABORATORY		CAICT																						
Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China Tel: +86-10-42304633-2079 Fax: +86-10-42304633-2504 E-mail: cti@sgs.com.cn http://www.sgslab.com.cn		Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China Tel: +86-10-42304633-2079 Fax: +86-10-42304633-2504 E-mail: cti@sgs.com.cn http://www.sgslab.com.cn																						
Measurement Conditions DASY system configuration, as far as not given on page 1:																								
<table border="1"><thead><tr><th>DASY Version</th><th>DASY52</th><th>52.10.4</th></tr></thead><tbody><tr><td>Extrapolation</td><td>Advanced Extrapolation</td><td></td></tr><tr><td>Phantom</td><td>Triple Flat Phantom 5.1C</td><td></td></tr><tr><td>Distance Dipole Center - TSL</td><td>10 mm</td><td>with Spacer</td></tr><tr><td>Zoom Scan Resolution</td><td>dx, dy, dz = 5 mm</td><td></td></tr><tr><td>Frequency</td><td>2600 MHz ± 1 MHz</td><td></td></tr></tbody></table>		DASY Version	DASY52	52.10.4	Extrapolation	Advanced Extrapolation		Phantom	Triple Flat Phantom 5.1C		Distance Dipole Center - TSL	10 mm	with Spacer	Zoom Scan Resolution	dx, dy, dz = 5 mm		Frequency	2600 MHz ± 1 MHz						
DASY Version	DASY52	52.10.4																						
Extrapolation	Advanced Extrapolation																							
Phantom	Triple Flat Phantom 5.1C																							
Distance Dipole Center - TSL	10 mm	with Spacer																						
Zoom Scan Resolution	dx, dy, dz = 5 mm																							
Frequency	2600 MHz ± 1 MHz																							
Head TSL parameters The following parameters and calculations were applied:																								
<table border="1"><thead><tr><th></th><th>Temperature</th><th>Permittivity</th><th>Conductivity</th></tr></thead><tbody><tr><td>Nominal Head TSL parameters</td><td>22.0 °C</td><td>38.0</td><td>1.96 mho/m</td></tr><tr><td>Measured Head TSL parameters</td><td>(22.0 ± 0.2) °C</td><td>38.7 ± 8 %</td><td>1.96 mho/m ± 8 %</td></tr><tr><td>Head TSL temperature change during test</td><td>±1.0 °C</td><td>—</td><td>—</td></tr></tbody></table>			Temperature	Permittivity	Conductivity	Nominal Head TSL parameters	22.0 °C	38.0	1.96 mho/m	Measured Head TSL parameters	(22.0 ± 0.2) °C	38.7 ± 8 %	1.96 mho/m ± 8 %	Head TSL temperature change during test	±1.0 °C	—	—							
	Temperature	Permittivity	Conductivity																					
Nominal Head TSL parameters	22.0 °C	38.0	1.96 mho/m																					
Measured Head TSL parameters	(22.0 ± 0.2) °C	38.7 ± 8 %	1.96 mho/m ± 8 %																					
Head TSL temperature change during test	±1.0 °C	—	—																					
SAR result with Head TSL																								
<table border="1"><thead><tr><th></th><th>Condition</th><th></th></tr></thead><tbody><tr><td>SAR averaged over 1 cm² (1 g) of Head TSL</td><td></td><td></td></tr><tr><td>SAR measured</td><td>250 mW input power</td><td>13.7 W/kg</td></tr><tr><td>SAR for nominal Head TSL parameters</td><td>normalized to 1W</td><td>54.8 W/kg ± 18.8 % (k=2)</td></tr><tr><td>SAR averaged over 10 cm² (10 g) of Head TSL</td><td></td><td></td></tr><tr><td>SAR measured</td><td>250 mW input power</td><td>8.12 W/kg</td></tr><tr><td>SAR for nominal Head TSL parameters</td><td>normalized to 1W</td><td>24.5 W/kg ± 18.7 % (k=2)</td></tr></tbody></table>			Condition		SAR averaged over 1 cm ² (1 g) of Head TSL			SAR measured	250 mW input power	13.7 W/kg	SAR for nominal Head TSL parameters	normalized to 1W	54.8 W/kg ± 18.8 % (k=2)	SAR averaged over 10 cm ² (10 g) of Head TSL			SAR measured	250 mW input power	8.12 W/kg	SAR for nominal Head TSL parameters	normalized to 1W	24.5 W/kg ± 18.7 % (k=2)		
	Condition																							
SAR averaged over 1 cm ² (1 g) of Head TSL																								
SAR measured	250 mW input power	13.7 W/kg																						
SAR for nominal Head TSL parameters	normalized to 1W	54.8 W/kg ± 18.8 % (k=2)																						
SAR averaged over 10 cm ² (10 g) of Head TSL																								
SAR measured	250 mW input power	8.12 W/kg																						
SAR for nominal Head TSL parameters	normalized to 1W	24.5 W/kg ± 18.7 % (k=2)																						
Certificate No: Z22-40108		Page 3 of 6																						

TTL S p e a g CALIBRATION LABORATORY		CAICT	
Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China Tel: +86-10-42304633-2079 Fax: +86-10-42304633-2504 E-mail: cti@sgs.com.cn http://www.sgslab.com.cn		Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China Tel: +86-10-42304633-2079 Fax: +86-10-42304633-2504 E-mail: cti@sgs.com.cn http://www.sgslab.com.cn	
Glossary:			
TSL	tissue simulating liquid		
ConvF	sensitivity in TSL / NORM _{xy,z}		
N/A	not applicable or not measured		
Calibration is Performed According to the Following Standards:			
a) IEC/IEEE 62209-1528, "Measurement Procedure for The Assessment of Specific Absorption Rate of Human Exposure to Radio Frequency Fields from Hand-held and Body-mounted Wireless Communication Devices - Part 1528: Human Models, Instrumentation and Procedures (Frequency range of 4 MHz to 10 GHz)", October 2020			
b) KDB 865864, "SAR Measurement Requirements for 100 MHz to 6 GHz"			
Additional Documentation:			
c) DASY4/S System Handbook			
Methods Applied and Interpretation of Parameters:			
• Measurement Conditions: Further details are available from the Validation Report at the end of the certificate. All figures stated in the certificate are valid at the frequency indicated.			
• Antenna Parameters with TSL: The dipole is mounted with the spacer to position its feed point exactly below the center marking of the flat phantom section, with the arms oriented parallel to the body axis.			
• Feed Point Impedance and Return Loss: These parameters are measured with the dipole positioned under the liquid filled phantom. The impedance stated is transformed from the measurement at the SMA connector to the feed point. The Return Loss ensures low reflected power. No uncertainty required.			
• Electrical Delay: One-way delay between the SMA connector and the antenna feed point. No uncertainty required.			
• SAR measured: SAR measured at the stated antenna input power.			
• SAR normalized: SAR as measured, normalized to an input power of 1 W at the antenna connector.			
• SAR for nominal TSL parameters: The measured TSL parameters are used to calculate the nominal SAR result.			
The reported uncertainty of measurement is stated as the standard uncertainty of Measurement multiplied by the coverage factor k=2, which for a normal distribution corresponds to a coverage probability of approximately 95%.			
Certificate No: Z22-40108		Page 2 of 6	

TTL S p e a g CALIBRATION LABORATORY		CAICT					
Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China Tel: +86-10-42304633-2079 Fax: +86-10-42304633-2504 E-mail: cti@sgs.com.cn http://www.sgslab.com.cn		Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China Tel: +86-10-42304633-2079 Fax: +86-10-42304633-2504 E-mail: cti@sgs.com.cn http://www.sgslab.com.cn					
Appendix (Additional assessments outside the scope of CNAS L0570)							
Antenna Parameters with Head TSL							
<table border="1"><thead><tr><th>Impedance, transformed to feed point</th><th>49.90 - j6.48Ω</th></tr></thead><tbody><tr><td>Return Loss</td><td>-23.9dB</td></tr></tbody></table>		Impedance, transformed to feed point	49.90 - j6.48Ω	Return Loss	-23.9dB		
Impedance, transformed to feed point	49.90 - j6.48Ω						
Return Loss	-23.9dB						
General Antenna Parameters and Design							
<table border="1"><thead><tr><th>Electrical Delay (one direction)</th><th>1.053 ns</th></tr></thead></table>		Electrical Delay (one direction)	1.053 ns				
Electrical Delay (one direction)	1.053 ns						
After long term use with 100W radiated power, only a slight warming of the dipole near the feed-point can be measured.							
The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals. On some of the dipoles, small end caps are added to the dipole arms in order to improve matching when loaded according to the position as explained in the "Measurement Conditions" paragraph. The SAR data are not affected by this change. The overall dipole length is still according to the Standard. No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feed-point may be damaged.							
Additional EUT Data							
<table border="1"><thead><tr><th>Manufactured by</th><th>SPEAG</th></tr></thead></table>		Manufactured by	SPEAG				
Manufactured by	SPEAG						
Certificate No: Z22-40108		Page 4 of 6					




Unless otherwise agreed in writing, this document is issued by the Company subject to its General Conditions of Service printed overleaf, available on request or accessible at <http://www.sgs.com/en/Terms-and-Conditions.aspx> and, for electronic format documents, subject to Terms and Conditions for Electronic Documents at <http://www.sgs.com/en/Terms-and-Conditions/Terms-e-Documents.aspx>. Attention is drawn to the limitation of liability, indemnification and jurisdiction issues defined therein. Any holder of this document is advised that information contained hereon reflects the Company's findings at the time of its intervention only and within the limits of Client's instructions, if any. The Company's sole responsibility is to its Client and this document does not exonerate parties to a transaction from exercising all their rights and obligations under the transaction documents. This document cannot be reproduced except in full, without prior written approval of the Company. Any unauthorized alteration, forgery or falsification of the content or appearance of this document is unlawful and offenders may be prosecuted to the fullest extent of the law. Unless otherwise stated the results shown in this test report refer only to the sample(s) tested and such sample(s) are retained for 30 days only.

Attention: To check the authenticity of testing / inspection report & certificate, please contact us at telephone: (86-755) 8307 1443, or email: CN.Doccheck@sgs.com

No.10, Weiye Road, Innovation Park, Kunshan, Jiangsu, China 215300
中国·江苏·昆山市留学生创业园伟业路10号 邮编 215300

(86-512) 57355888 (86-512) 57370818 www.sgs.com.cn
(86-512) 57355888 (86-512) 57370818 sgs.china@sgs.com

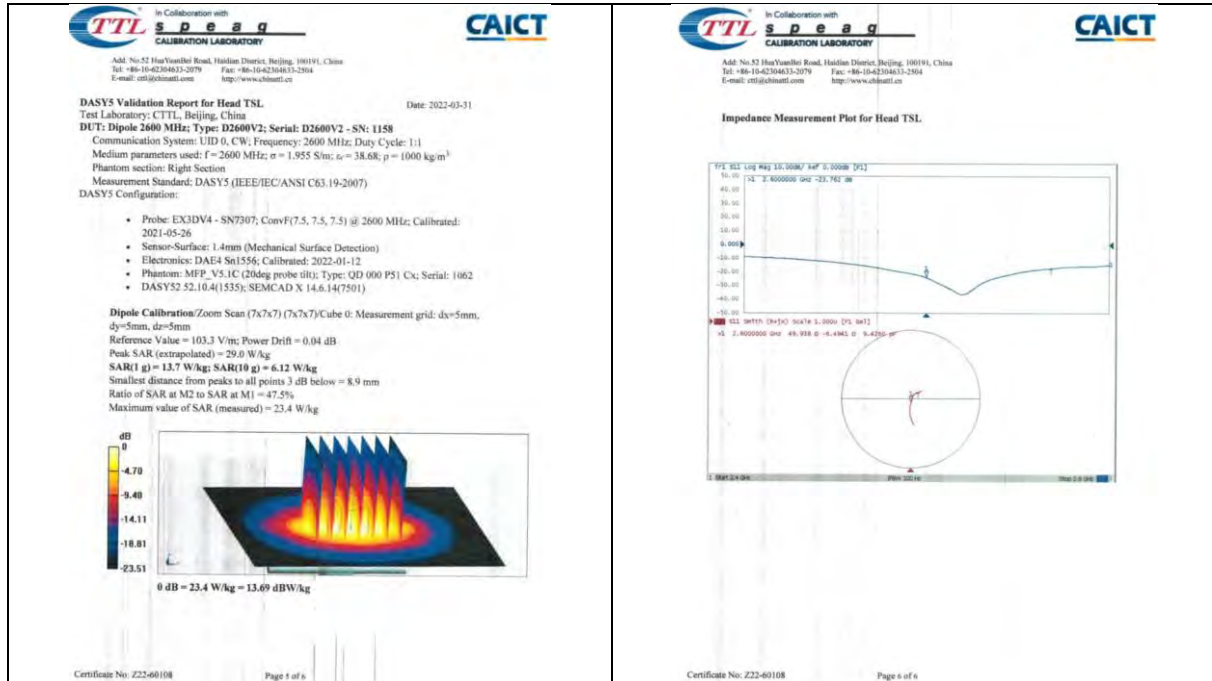

1.12 D5GHZV2 - SN 1095

TTL Speaq
CALIBRATION LABORATORY

Add: No.52 HuaYuanbei Road, Haidian District, Beijing, 100191, China
Tel: +86-10-62304633-2079 Fax: +86-10-62304633-2504
E-mail: cti@china.ttl.com.cn http://www.china.ttl.com.cn

CAICT

Client: SGS-CN Certificate No: Z22-60187

CALIBRATION CERTIFICATE

Object: D5GHZV2 - SN 1095

Calibration Procedure(s): FF-Z11-003-01
Calibration Procedures for dipole validation kit

Calibration date: June 1, 2022

This calibration Certificate documents the traceability to national standards, which realize the physical units of measurements (SI). The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility: environment temperature (23±3)°C and humidity <70%.

Calibration Equipment used (MSTE critical for calibration)

Primary Standards	ID #	Cal Date (Calibrated by: Certificate No.)	Scheduled Calibration
Power Meter NRP2	106277	24-Sep-21 (CCTL No. J21008328)	Sep-22
Power sensor NRP85	104201	24-Sep-21 (CCTL No. J21008328)	Sep-22
Reference Probe EX3DV4	SN 7464	26-Jan-22 (SPEAG No. EX3-7464, Jan22)	Jan-23
DA64	SN 1556	12-Jan-22 (CCTL-SPEAG No. Z22-60007)	Jan-23

Secondary Standards	ID #	Cal Date (Calibrated by: Certificate No.)	Scheduled Calibration
Signal Generator E4438C	MY48071430	13-Jan-22 (CCTL No. J22000409)	Jan-23
Network Analyzer E5071C	MY46110673	14-Jan-22 (CCTL No. J22000406)	Jan-23

Calibrated by: Zhao Jing SAR Test Engineer

Reviewed by: Lin Hao SAR Test Engineer

Approved by: Qi Dianyan SAR Project Leader

Issued: June 9, 2022

This calibration Certificate shall not be reproduced except in full without written approval of the laboratory.

Certificate No: Z22-60187 Page 1 of 10

TTL Speaq
CALIBRATION LABORATORY

Add: No.52 HuaYuanbei Road, Haidian District, Beijing, 100191, China
Tel: +86-10-62304633-2079 Fax: +86-10-62304633-2504
E-mail: cti@china.ttl.com.cn http://www.china.ttl.com.cn

CAICT

Glossary:

TSL: Issue simulating liquid

CompF: sensitivity in TSL + NORM(x,y,z)

N/A: not applicable or not measured

Calibration is Performed According to the Following Standards:

a) IEC/IEEE 62209-1528, "Measurement Procedure for the Assessment of Specific Absorption Rate of Human Exposure to Radio Frequency Fields from Hand-held and Body-mounted Wireless Communication Devices-Part 1528: Human Models, Instrumentation and Procedures (Frequency range of 4 MHz to 10 GHz)", October 2020

b) KDB 665664, "SAR Measurement Requirements for 100 MHz to 6 GHz"

Additional Documentation:

c) DASY5 System Handbook

Methods Applied and Interpretation of Parameters:

- Measurement Conditions: Further details are available from the Validation Report at the end of the certificate. All figures stated in the certificate are valid at the frequency indicated.
- Antenna Parameters with TSL: The dipole is mounted with the spacer to position its feed point exactly below the center marking of the flat phantom section, with the arms oriented parallel to the body axis.
- Feed Point Impedance and Return Loss: These parameters are measured with the dipole positioned under the liquid filled phantom. The impedance station is transformed from the measurement at the SMA connector to the feed point. The Return Loss ensures low reflected power. No uncertainty required.
- Electrical Delay: One-way delay between the SMA connector and the antenna feed point. No uncertainty required.
- SAR measured: SAR measured at the stated antenna input power.
- SAR normalized: SAR as measured, normalized to an input power of 1 W at the antenna connector.
- SAR for nominal TSL parameters: The measured TSL parameters are used to calculate the nominal SAR result.

The reported uncertainty of measurement is stated as the standard uncertainty of Measurement multiplied by the coverage factor $k=2$, which for a normal distribution Corresponds to a coverage probability of approximately 95%.

Certificate No: Z22-60187 Page 7 of 10



Unless otherwise agreed in writing, this document is issued by the Company subject to its General Conditions of Service printed overleaf, available on request or accessible at <http://www.sgs.com/en/Terms-and-Conditions.aspx>; and, for electronic format documents, subject to Terms and Conditions for Electronic Documents at <http://www.sgs.com/en/Terms-and-Conditions/Terms-e-Documents.aspx>. Attention is drawn to the limitation of liability, indemnification and jurisdiction issues defined therein. Any holder of this document is advised that information contained hereon reflects the Company's findings at the time of its intervention only and within the limits of Client's instructions, if any. The Company's sole responsibility is to its Client and this document does not exonerate parties to a transaction from exercising all their rights and obligations under the transaction documents. This document cannot be reproduced except in full, without prior written approval of the Company. Any unauthorized alteration, forgery or falsification of the content or appearance of this document is unlawful and offenders may be prosecuted to the fullest extent of the law. Unless otherwise stated the results shown in this test report refer only to the sample(s) tested and such sample(s) are retained for 30 days only.

Attention: To check the authenticity of testing/inspection report & certificate, please contact us at telephone: (86-755) 8307 1443, or email: CN.Doccheck@sgs.com

No.10, Weiye Road, Innovation Park, Kunshan, Jiangsu, China 215300
中国·江苏·昆山市留学生创业园伟业路10号 邮编 215300

t(86-512)57355888 f(86-512)57370818 www.sgs.com.cn
t(86-512)57355888 f(86-512)57370818 sgs.china@sgs.com

TTL Calibration Laboratory		CAICT	
In Collaboration with s p e a g Add: No.52 HuaYuan Road, Haidian District, Beijing, 100191, China Tel: +86-10-62420217 E-mail: info@speag.com http://www.speag.com		In Collaboration with s p e a g Add: No.52 HuaYuan Road, Haidian District, Beijing, 100191, China Tel: +86-10-62420217 E-mail: info@speag.com http://www.speag.com	
Measurement Conditions SAR system configuration, as for as not given on page 1.			
DASY Version	DASY2	52.10.4	
Extrapolation	Advanced Extrapolation		
Phantom	Triple Flat Phantom S.1C		
Distance Dipole Center - TSL	10 mm	with Spacer	
Zoom Scan Resolution	dx, dy = 4 mm, dz = 1.4 mm	Graded Ratio = 1.4 (Z direction)	
Frequency	500 MHz ± 1 MHz 800 MHz ± 1 MHz 1500 MHz ± 1 MHz 5600 MHz ± 1 MHz		
Head TSL parameters at 5200MHz The following parameters and calculations were applied:			
Nominal Head TSL parameters	Temperature	Permittivity	Conductivity
Measured Head TSL parameters	22.0 °C	35.9	4.76 mho/m
Head TSL temperature change during test	(22.0 ± 0.2) °C	35.4 ± 5 %	4.73 mho/m ± 5 %
Head TSL temperature change during test	<1.0 °C	—	—
SAR result with Head TSL at 5200MHz The following parameters and calculations were applied:			
SAR averaged over 1 cm ³ (1 g) of Head TSL	Condition		
SAR measured	250 mW input power	7.75 W/kg	
SAR for nominal Head TSL parameters	normalized to 1W	77.8 W/kg ± 24.4 % (k=2)	
SAR averaged over 10 cm ³ (10 g) of Head TSL	Condition		
SAR measured	250 mW input power	2.22 W/kg	
SAR for nominal Head TSL parameters	normalized to 1W	22.1 W/kg ± 24.2 % (k=2)	
Head TSL parameters at 5300MHz The following parameters and calculations were applied:			
Nominal Head TSL parameters	Temperature	Permittivity	Conductivity
Measured Head TSL parameters	22.0 °C	35.9	4.76 mho/m
Head TSL temperature change during test	(22.0 ± 0.2) °C	35.4 ± 5 %	4.73 mho/m ± 5 %
Head TSL temperature change during test	<1.0 °C	—	—
SAR result with Head TSL at 5300MHz The following parameters and calculations were applied:			
SAR averaged over 1 cm ³ (1 g) of Head TSL	Condition		
SAR measured	100 mW input power	7.84 W/kg	
SAR for nominal Head TSL parameters	normalized to 1W	78.1 W/kg ± 24.4 % (k=2)	
SAR averaged over 10 cm ³ (10 g) of Head TSL	Condition		
SAR measured	100 mW input power	2.27 W/kg	
SAR for nominal Head TSL parameters	normalized to 1W	22.6 W/kg ± 24.2 % (k=2)	
Head TSL parameters at 5500MHz The following parameters and calculations were applied:			
Nominal Head TSL parameters	Temperature	Permittivity	Conductivity
Measured Head TSL parameters	22.0 °C	35.8	4.88 mho/m
Head TSL temperature change during test	(22.0 ± 0.2) °C	34.8 ± 5 %	4.84 mho/m ± 5 %
Head TSL temperature change during test	<1.0 °C	—	—
SAR result with Head TSL at 5500MHz The following parameters and calculations were applied:			
SAR averaged over 1 cm ³ (1 g) of Head TSL	Condition		
SAR measured	100 mW input power	8.26 W/kg	
SAR for nominal Head TSL parameters	normalized to 1W	82.5 W/kg ± 24.4 % (k=2)	
SAR averaged over 10 cm ³ (10 g) of Head TSL	Condition		
SAR measured	100 mW input power	2.34 W/kg	
SAR for nominal Head TSL parameters	normalized to 1W	23.3 W/kg ± 24.2 % (k=2)	
Head TSL parameters at 5600MHz The following parameters and calculations were applied:			
Nominal Head TSL parameters	Temperature	Permittivity	Conductivity
Measured Head TSL parameters	22.0 °C	35.5	5.07 mho/m
Head TSL temperature change during test	(22.0 ± 0.2) °C	34.7 ± 5 %	5.05 mho/m ± 5 %
Head TSL temperature change during test	<1.0 °C	—	—
SAR result with Head TSL at 5600MHz The following parameters and calculations were applied:			
SAR averaged over 1 cm ³ (1 g) of Head TSL	Condition		
SAR measured	100 mW input power	8.12 W/kg	
SAR for nominal Head TSL parameters	normalized to 1W	80.8 W/kg ± 24.4 % (k=2)	
SAR averaged over 10 cm ³ (10 g) of Head TSL	Condition		
SAR measured	100 mW input power	2.30 W/kg	
SAR for nominal Head TSL parameters	normalized to 1W	22.9 W/kg ± 24.2 % (k=2)	
Head TSL parameters at 5800MHz The following parameters and calculations were applied:			
Nominal Head TSL parameters	Temperature	Permittivity	Conductivity
Measured Head TSL parameters	22.0 °C	35.3	5.27 mho/m
Head TSL temperature change during test	(22.0 ± 0.2) °C	34.4 ± 5 %	5.25 mho/m ± 5 %
Head TSL temperature change during test	<1.0 °C	—	—
SAR result with Head TSL at 5800MHz The following parameters and calculations were applied:			
SAR averaged over 1 cm ³ (1 g) of Head TSL	Condition		
SAR measured	100 mW input power	7.71 W/kg	
SAR for nominal Head TSL parameters	normalized to 1W	76.7 W/kg ± 24.4 % (k=2)	
SAR averaged over 10 cm ³ (10 g) of Head TSL	Condition		
SAR measured	100 mW input power	2.16 W/kg	
SAR for nominal Head TSL parameters	normalized to 1W	21.5 W/kg ± 24.2 % (k=2)	
Appendix (Additional assessments outside the scope of CNAS L0570)			
Antenna Parameters with Head TSL at 5200MHz			
Impedance, transformed to feed point	48.10-5.03jΩ		
Return Loss	-23.8dB		
Antenna Parameters with Head TSL at 5300MHz			
Impedance, transformed to feed point	47.80-2.42jΩ		
Return Loss	-23.5dB		
Antenna Parameters with Head TSL at 5500MHz			
Impedance, transformed to feed point	50.30-4.26jΩ		
Return Loss	-27.4dB		
Antenna Parameters with Head TSL at 5600MHz			
Impedance, transformed to feed point	54.80-4.86jΩ		
Return Loss	-24.6dB		
Antenna Parameters with Head TSL at 5800MHz			
Impedance, transformed to feed point	51.50-5.61jΩ		
Return Loss	-24.9dB		





Unless otherwise agreed in writing, this document is issued by the Company subject to its General Conditions of Service printed overleaf, available on request or accessible at <http://www.sgs.com/en/Terms-and-Conditions.aspx> and, for electronic format documents, subject to Terms and Conditions for Electronic Documents at <http://www.sgs.com/en/Terms-and-Conditions/Terms-e-Documents.aspx>. Attention is drawn to the limitation of liability, indemnification and jurisdiction issues defined therein. Any holder of this document is advised that information contained hereon reflects the Company's findings at the time of its intervention only and within the limits of Client's instructions, if any. The Company's sole responsibility is to its Client and this document does not exonerate parties to a transaction from exercising all their rights and obligations under the transaction documents. This document cannot be reproduced except in full, without prior written approval of the Company. Any unauthorized alteration, forgery or falsification of the content or appearance of this document is unlawful and offenders may be prosecuted to the fullest extent of the law. Unless otherwise stated the results shown in this test report refer only to the sample(s) tested and such sample(s) are retained for 30 days only.

Attention: To check the authenticity of testing / inspection report & certificate, please contact us at telephone: (86-755) 8307 1443, or email: CN.Doccheck@sgs.com

No.10, Weyue Road, Innovation Park, Kunshan, Jiangsu, China 215300
中国·江苏·昆山市留学院创业园伟业路10号 邮编 215300

t(86-512)57355888 f(86-512)57370818 www.sgs.com.cn
t(86-512)57355888 f(86-512)57370818 sgs.china@sgs.com

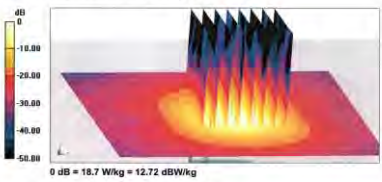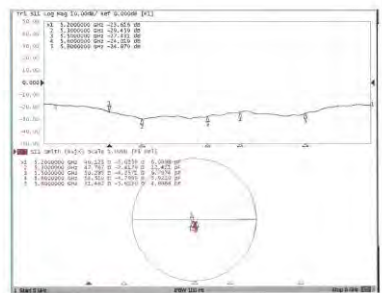In Collaboration with TTL speaq CALIBRATION LABORATORY Address: No.52 Huayuan Road, Haidian District, Beijing, 100191, China Tel: +86-10-62302117 E-mail: csl@speaq.com.cn http://www.speaq.com.cn CAICT General Antenna Parameters and Design Electrical Delay (one direction): 1.021 ns After long term use with 100W radiated power, only a slight warming of the dipole near the feed-point can be measured. The dipole is made of standard semirigid coaxial cable. The carrier conductor of the feeding line is directly connected to the second arm of the dipole. This antenna is therefore short-circuited for DC-signals. On some of the dipoles, small end caps are added to the dipole arms in order to improve matching when loaded according to the position as explained in the "Measurement Conditions" paragraph. The SAR data are not affected by this change. The overall dipole length is still according to the Standard. No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feed-point may be damaged. Additional EUT Data Manufactured by: SPEAQ Certificate No: Z22-60187 Page 1 of 10	In Collaboration with TTL speaq CALIBRATION LABORATORY Address: No.52 Huayuan Road, Haidian District, Beijing, 100191, China Tel: +86-10-62302117 E-mail: csl@speaq.com.cn http://www.speaq.com.cn CAICT DASY5 Validation Report for Head TSL Test Laboratory: CTTL, Beijing, China Date: 2022-09-01 DUT: Dipole 5GHz; Type: D5GHzV2; Serial: D5GHzV2 - SN: 1095 Communication System: CW; Frequency: 5200 MHz; Frequency: 5300 MHz; Frequency: 5500 MHz; Frequency: 5600 MHz; Frequency: 5800 MHz; Duty Cycle: 1:1 Medium parameters used: $f = 5200$ MHz; $\sigma = 4.82$ S/m; $\epsilon = 35.39$; $\rho = 1000$ kg/m³ Medium parameters used: $f = 5300$ MHz; $\sigma = 4.73$ S/m; $\epsilon = 35.19$; $\rho = 1000$ kg/m³ Medium parameters used: $f = 5500$ MHz; $\sigma = 4.939$ S/m; $\epsilon = 34.83$; $\rho = 1000$ kg/m³ Medium parameters used: $f = 5600$ MHz; $\sigma = 5.051$ S/m; $\epsilon = 34.89$; $\rho = 1000$ kg/m³ Medium parameters used: $f = 5800$ MHz; $\sigma = 5.247$ S/m; $\epsilon = 34.42$; $\rho = 1000$ kg/m³ Phantom section: Right Section Measurement Standard: DASY5 (IEEE/IEC/ANSI C38.19-2007) DASY5 Configuration: - Probe: EX3DV4 - SN7484; ConvF(5.6, 5.6, 5.6) @ 5200 MHz; ConvF(5.32, 5.32, 5.32) @ 5300 MHz; ConvF(5.11, 5.11, 5.11) @ 5500 MHz; ConvF(4.91, 4.91, 4.91) @ 5600 MHz; ConvF(5, 5, 5) @ 5800 MHz; Calibrated: 2022-01-28 - Sensor-Surface: 1.4mm (Mechanical Surface Detection) - Electronics: DA84 Sn1556; Calibrated: 2022-01-12 - Phantom: MPF_V5.1C (20deg probe tilt); Type: QD 000 P51 Cx; Serial: 1062 - DASY52 52.10.4(1535); SEMCAD X 14.6.14(7501) Dipole Calibration /Pin=100mW, d=10mm, f=5200 MHz/Zoom Scan, dist=1.4mm (8x8x7)/Cube 0; Measurement grid: dx=4mm, dy=4mm, dz=1.4mm; Reference Value = 60.80 V/m; Power Drift = -0.06 dB Peak SAR (extrapolated) = 29.8 W/kg SAR(1 g) = 7.73 W/kg; SAR(10 g) = 2.22 W/kg Smallest distance from peaks to all points 3 dB below = 7.2 mm Ratio of SAR at M2 to SAR at M1 = 66.8% Maximum value of SAR (measured) = 19.3 W/kg Dipole Calibration /Pin=100mW, d=10mm, f=5300 MHz/Zoom Scan, dist=1.4mm (8x8x7)/Cube 0; Measurement grid: dx=4mm, dy=4mm, dz=1.4mm; Reference Value = 61.08 V/m; Power Drift = -0.07 dB Peak SAR (extrapolated) = 31.5 W/kg SAR(1 g) = 7.94 W/kg; SAR(10 g) = 2.27 W/kg Smallest distance from peaks to all points 3 dB below = 7.2 mm Ratio of SAR at M2 to SAR at M1 = 65.5% Maximum value of SAR (measured) = 19.0 W/kg Certificate No: Z22-60187 Page 2 of 10
In Collaboration with TTL speaq CALIBRATION LABORATORY Address: No.52 Huayuan Road, Haidian District, Beijing, 100191, China Tel: +86-10-62302117 E-mail: csl@speaq.com.cn http://www.speaq.com.cn CAICT Dipole Calibration /Pin=100mW, d=10mm, f=5500 MHz/Zoom Scan, dist=1.4mm (8x8x7)/Cube 0; Measurement grid: dx=4mm, dy=4mm, dz=1.4mm; Reference Value = 61.92 V/m; Power Drift = -0.08 dB Peak SAR (extrapolated) = 34.7 W/kg SAR(1 g) = 8.28 W/kg; SAR(10 g) = 2.34 W/kg Smallest distance from peaks to all points 3 dB below = 7.2 mm Ratio of SAR at M2 to SAR at M1 = 63.9% Maximum value of SAR (measured) = 20.2 W/kg Dipole Calibration /Pin=100mW, d=10mm, f=5600 MHz/Zoom Scan, dist=1.4mm (8x8x7)/Cube 0; Measurement grid: dx=4mm, dy=4mm, dz=1.4mm; Reference Value = 65.08 V/m; Power Drift = -0.07 dB Peak SAR (extrapolated) = 35.3 W/kg SAR(1 g) = 8.12 W/kg; SAR(10 g) = 2.3 W/kg Smallest distance from peaks to all points 3 dB below = 7.2 mm Ratio of SAR at M2 to SAR at M1 = 62.5% Maximum value of SAR (measured) = 19.1 W/kg Dipole Calibration /Pin=100mW, d=10mm, f=5800 MHz/Zoom Scan, dist=1.4mm (8x8x7)/Cube 0; Measurement grid: dx=4mm, dy=4mm, dz=1.4mm; Reference Value = 62.13 V/m; Power Drift = -0.06 dB Peak SAR (extrapolated) = 34.8 W/kg SAR(1 g) = 7.71 W/kg; SAR(10 g) = 2.16 W/kg Smallest distance from peaks to all points 3 dB below = 7.2 mm Ratio of SAR at M2 to SAR at M1 = 61.6% Maximum value of SAR (measured) = 18.7 W/kg  Certificate No: Z22-60187 Page 3 of 10	In Collaboration with TTL speaq CALIBRATION LABORATORY Address: No.52 Huayuan Road, Haidian District, Beijing, 100191, China Tel: +86-10-62302117 E-mail: csl@speaq.com.cn http://www.speaq.com.cn CAICT Impedance Measurement Plot for Head TSL  Certificate No: Z22-60187 Page 4 of 10



Unless otherwise agreed in writing, this document is issued by the Company subject to its General Conditions of Service printed overleaf, available on request or accessible at <http://www.sgs.com/en/Terms-and-Conditions.aspx>; and, for electronic format documents, subject to Terms and Conditions for Electronic Documents at <http://www.sgs.com/en/Terms-and-Conditions/Terms-e-Documents.aspx>. Attention is drawn to the limitation of liability, indemnification and jurisdiction issues defined therein. Any holder of this document is advised that information contained hereon reflects the Company's findings at the time of its intervention only and within the limits of Client's instructions, if any. The Company's sole responsibility is to its Client and this document does not exonerate parties to a transaction from exercising all their rights and obligations under the transaction documents. This document cannot be reproduced except in full, without prior written approval of the Company. Any unauthorized alteration, forgery or falsification of the content or appearance of this document is unlawful and offenders may be prosecuted to the fullest extent of the law. Unless otherwise stated the results shown in this test report refer only to the sample(s) tested and such sample(s) are retained for 30 days only.

Attention: To check the authenticity of testing/inspection report & certificate, please contact us at telephone: (86-755) 8307 1443, or email: CN.Doccheck@sgs.com

No.10, Weiye Road, Innovation Park, Kunshan, Jiangsu, China 215300
中国·江苏·昆山市留学生创业园伟业路10号 邮编 215300

(86-512)57355888 (86-512)57370818 www.sgs.com.cn
(86-512)57355888 (86-512)57370818 sgs.china@sgs.com

2 DAE4 - SN 1245

Schmid & Partner Engineering AG Zugzwangstrasse 43, 8004 Zurich, Switzerland Phone +41 (0)43 9702, Fax +41 (0)43 9775 www.speag.ch, info@speag.ch s p e a g IMPORTANT NOTICE USAGE OF THE DAE4 The DAE4 unit is a delicate, high precision instrument and requires careful treatment by the user. There are no serviceable parts inside the DAE4. Special attention shall be given to the following points: Battery Exchange: The battery cover of the DAE4 unit is fixed using a screw, over tightening the screw may cause the threads inside the DAE4 to wear out. Shipping of the DAE4: Before shipping the DAE4 to SPEAG for calibration, remove the batteries and pack the DAE4 in an anti-static bag. This anti-static bag shall then be packed into a larger box or container which protects the DAE4 from impacts during transportation. The package shall be marked to indicate that a fragile instrument is inside. E-stop Failures: Touch detection may be malfunctioning due to broken magnets in the E-stop. Rough handling of the E-stop may lead to damage of these magnets. Touch and collision errors are often caused by dust and dirt accumulated in the E-stop. To prevent E-stop failure, the customer shall always mount the probe to the DAE4 carefully and keep the DAE4 unit in a non-dusty environment if not used for measurements. Repair: Minor repairs are performed at no extra cost during the annual calibration. However, SPEAG reserves the right to charge for any repair especially if rough unprofessional handling caused the defect. DASY Configuration Files: Since the exact values of the DAE input resistances, as measured during the calibration procedure of a DAE unit, are not used by the DASY software, a nominal value of 200 MOhm is given in the corresponding configuration file. Important Note: Warranty and calibration is void if the DAE unit is disassembled partly or fully by the Customer. Important Note: Never attempt to grease or oil the E-stop assembly. Cleaning and readjusting of the E-stop assembly is allowed by certified SPEAG personnel only and is part of the annual calibration procedure. Important Note: To prevent damage of the DAE probe connector pins, use great care when installing the probe to the DAE. Carefully connect the probe with the connector notch oriented in the mating position. Avoid any rotational movement of the probe body versus the DAE while turning the locking nut of the connector. The same care shall be used when disconnecting the probe from the DAE. TN_EH190306AE_DAE4.docx 07.03.2019	Calibration Laboratory of Schmid & Partner Engineering AG Zugzwangstrasse 43, 8004 Zurich, Switzerland Accredited by the Swiss Accreditation Service (SAS) The Swiss Accreditation Service is one of the signatories to the EA Multilateral Agreement for the recognition of calibration certificates Client: SGS-CN (Auden) Certificate No.: DAE4-1245_May22 Accreditation No.: SCS 0108 CALIBRATION CERTIFICATE Object: DAE4 - SD 000 D04 BM - SN: 1245 Calibration procedure(s): QA CAL-06 v30 Calibration procedure for the data acquisition electronics (DAE) Calibration date: May 30, 2022 This calibration certificate documents the traceability to national standards, which include the physical units of measurement (SI). The measurement and the uncertainties with confidence probability are given on the following pages and are part of the certificate. All calibrations have been conducted in the closed laboratory facility: environment temperature (22 ± 1)°C and humidity < 70%. Calibration Equipment used (MATE critical for calibration) <table border="1"> <tr> <th>Primary Standards</th> <th>ID #</th> <th>Due Date (Certificate No.)</th> <th>Scheduled Calibration</th> </tr> <tr> <td>Kettley Multimeter Type 2001</td> <td>SN: 0810278</td> <td>31-Aug-21 (No: 31368)</td> <td>Aug-22</td> </tr> <tr> <th>Secondary Standards</th> <th>ID #</th> <th>Check Date (in hours)</th> <th>Scheduled Check</th> </tr> <tr> <td>Auto DAE Calibration Unit</td> <td>SE LWS 05A AA 1001</td> <td>24-Jan-22 (in hours check)</td> <td>In house check: Jan-22</td> </tr> <tr> <td>Calibrator Box V2.1</td> <td>SE LWS 00B AA 1002</td> <td>24-Jan-22 (in hours check)</td> <td>In house check: Jan-22</td> </tr> </table> Calibrated by: Dominique Steiner Function: Laboratory Technician Signature: <i>[Signature]</i> Approved by: (Ben Kuhn) Technical Manager Signature: <i>[Signature]</i> This calibration certificate shall not be reproduced except in full without written approval of the laboratory. Certificate No.: DAE4-1245_May22 Page 1 of 5	Primary Standards	ID #	Due Date (Certificate No.)	Scheduled Calibration	Kettley Multimeter Type 2001	SN: 0810278	31-Aug-21 (No: 31368)	Aug-22	Secondary Standards	ID #	Check Date (in hours)	Scheduled Check	Auto DAE Calibration Unit	SE LWS 05A AA 1001	24-Jan-22 (in hours check)	In house check: Jan-22	Calibrator Box V2.1	SE LWS 00B AA 1002	24-Jan-22 (in hours check)	In house check: Jan-22
Primary Standards	ID #	Due Date (Certificate No.)	Scheduled Calibration																		
Kettley Multimeter Type 2001	SN: 0810278	31-Aug-21 (No: 31368)	Aug-22																		
Secondary Standards	ID #	Check Date (in hours)	Scheduled Check																		
Auto DAE Calibration Unit	SE LWS 05A AA 1001	24-Jan-22 (in hours check)	In house check: Jan-22																		
Calibrator Box V2.1	SE LWS 00B AA 1002	24-Jan-22 (in hours check)	In house check: Jan-22																		
Calibration Laboratory of Schmid & Partner Engineering AG Zugzwangstrasse 43, 8004 Zurich, Switzerland Accredited by the Swiss Accreditation Service (SAS) The Swiss Accreditation Service is one of the signatories to the EA Multilateral Agreement for the recognition of calibration certificates Accreditation No.: SCS 0108 Glossary DAE: data acquisition electronics Connector angle: information used in DASY system to align probe sensor X to the robot coordinate system. Methods Applied and Interpretation of Parameters • DC Voltage Measurement: Calibration Factor assessed for use in DASY system by comparison with a calibrated instrument traceable to national standards. The figure given corresponds to the full scale range of the voltmeter in the respective range. • Connector angle: The angle of the connector is assessed measuring the angle mechanically by a tool inserted. Uncertainty is not required. • The following parameters as documented in the Appendix contain technical information as a result from the performance test and require no uncertainty. • DC Voltage Measurement Linearity: Verification of the Linearity at +10% and -10% of the nominal calibration voltage. Influence of offset voltage is included in this measurement. • Common mode sensitivity: Influence of a positive or negative common mode voltage on the differential measurement. • Channel separation: Influence of a voltage on the neighbor channels not subject to an input voltage. • AD Converter Values with inputs shorted: Values on the internal AD converter corresponding to zero input voltage. • Input Offset Measurement: Output voltage and statistical results over a large number of zero voltage measurements. • Input Offset Current: Typical value for information; Maximum channel input offset current, not considering the input resistance. • Input resistance: Typical value for information; DAE input resistance at the connector, during internal auto-zeroing and during measurement. • Low Battery Alarm Voltage: Typical value for information. Below this voltage, a battery alarm signal is generated. • Power consumption: Typical value for information. Supply currents in various operating modes. Certificate No.: DAE4-1245_May22 Page 2 of 5	DC Voltage Measurement AD - Converter Resolution nominal High Range: 1LSB = 6.1µV, full range = -190...+320 mV Low Range: 1LSB = 61µV, full range = -1...+32mV DASY measurement parameters: Auto Zero-Time: 3 sec; Measuring time: 3 sec <table border="1"> <tr> <th>Calibration Factors</th> <th>X</th> <th>Y</th> <th>Z</th> </tr> <tr> <td>High Range</td> <td>405.265 ± 0.02% (k=2)</td> <td>403.974 ± 0.02% (k=2)</td> <td>406.092 ± 0.02% (k=2)</td> </tr> <tr> <td>Low Range</td> <td>3.99534 ± 1.50% (k=2)</td> <td>3.99508 ± 1.50% (k=2)</td> <td>4.01015 ± 1.50% (k=2)</td> </tr> </table> Connector Angle <table border="1"> <tr> <td>Connector Angle to be used in DASY system</td> <td>30.0° ± 1°</td> </tr> </table> Certificate No.: DAE4-1245_May22 Page 3 of 5	Calibration Factors	X	Y	Z	High Range	405.265 ± 0.02% (k=2)	403.974 ± 0.02% (k=2)	406.092 ± 0.02% (k=2)	Low Range	3.99534 ± 1.50% (k=2)	3.99508 ± 1.50% (k=2)	4.01015 ± 1.50% (k=2)	Connector Angle to be used in DASY system	30.0° ± 1°						
Calibration Factors	X	Y	Z																		
High Range	405.265 ± 0.02% (k=2)	403.974 ± 0.02% (k=2)	406.092 ± 0.02% (k=2)																		
Low Range	3.99534 ± 1.50% (k=2)	3.99508 ± 1.50% (k=2)	4.01015 ± 1.50% (k=2)																		
Connector Angle to be used in DASY system	30.0° ± 1°																				



Unless otherwise agreed in writing, this document is issued by the Company subject to its General Conditions of Service printed overleaf, available on request or accessible at <http://www.sgs.com/en/Terms-and-Conditions.aspx>; and, for electronic format documents, subject to Terms and Conditions for Electronic Documents at <http://www.sgs.com/en/Terms-and-Conditions/Terms-e-Documents.aspx>. Attention is drawn to the limitation of liability, indemnification and jurisdiction issues defined therein. Any holder of this document is advised that information contained hereon reflects the Company's findings at the time of its intervention only and within the limits of Client's instructions, if any. The Company's sole responsibility is to its Client and this document does not exonerate parties to a transaction from exercising all their rights and obligations under the transaction documents. This document cannot be reproduced except in full, without prior written approval of the Company. Any unauthorized alteration, forgery or falsification of the content or appearance of this document is unlawful and offenders may be prosecuted to the fullest extent of the law. Unless otherwise stated the results shown in this test report refer only to the sample(s) tested and such sample(s) are retained for 30 days only.

Attention: To check the authenticity of testing/inspection report & certificate, please contact us at telephone: (86-755) 8307 1443, or email: CN.Doccheck@sgs.com

No.10, Weiye Road, Innovation Park, Kunshan, Jiangsu, China 215300
中国·江苏·昆山市留学生创业园伟业路10号 邮编 215300

t(86-512)57355888 f(86-512)57370818 www.sgsgroup.com.cn
t(86-512)57355888 f(86-512)57370818 sgs.china@sgs.com

Appendix (Additional assessments outside the scope of SCS0108)

1. DC Voltage Linearity

High Range	Reading (µV)	Difference (µV)	Error (%)
Channel X + Input	19994.45	1.52	0.00
Channel X - Input	20004.58	2.22	0.01
Channel X + Input	-20000.14	1.12	-0.01
Channel Y + Input	19994.72	1.58	0.00
Channel Y - Input	20001.22	-1.00	-0.00
Channel Y + Input	-20003.05	-1.57	0.01
Channel Z + Input	19992.44	0.19	0.00
Channel Z - Input	20003.09	0.58	0.00
Channel Z + Input	-20001.73	-0.27	0.00

Low Range	Reading (µV)	Difference (µV)	Error (%)
Channel X + Input	2001.91	0.41	0.02
Channel X - Input	200.54	0.65	0.32
Channel X + Input	-197.86	0.07	-0.04
Channel Y + Input	2002.05	0.58	0.03
Channel Y - Input	201.27	-0.67	-0.28
Channel Y + Input	-196.23	-0.06	0.03
Channel Z + Input	2001.96	0.08	0.00
Channel Z - Input	200.09	-1.03	-0.76
Channel Z + Input	-199.85	-1.57	0.79

2. Common mode sensitivity

Channel	Common mode Input Voltage (mV)	High Range Average Reading (µV)	Low Range Average Reading (µV)
Channel X	200	-5.87	-7.69
	-200	9.12	7.79
Channel Y	200	-8.68	-9.28
	-200	8.52	6.36
Channel Z	200	-5.36	-5.60
	-200	3.58	3.06

3. Channel separation

Channel	Input Voltage (mV)	Channel X (µV)	Channel Y (µV)	Channel Z (µV)
Channel X	200	-	4.07	-3.14
Channel Y	200	9.36	-	4.07
Channel Z	200	10.11	7.14	-

Certificate No: DAE4-1245_May22

Page 4 of 5

4. AD-Converter Values with inputs shorted

DASY measurement parameters: Auto Zero Time: 3 sec; Measuring time: 3 sec

	High Range (LSB)	Low Range (LSB)
Channel X	15984	17040
Channel Y	16562	16768
Channel Z	16035	15968

5. Input Offset Measurement

DASY measurement parameters: Auto Zero Time: 3 sec; Measuring time: 3 sec

Input (mV)	Average (µV)	min. Offset (µV)	max. Offset (µV)	Std. Deviation (µV)
Channel X	1.00	-0.15	1.93	0.45
Channel Y	-0.18	-1.28	0.94	0.45
Channel Z	-0.58	-2.81	0.58	0.60

6. Input Offset Current

Nominal input circuitry offset current on all channels: <25nA

7. Input Resistance (Typical values for information)

	Zeroing (kOhm)	Measuring (MOhm)
Channel X	200	200
Channel Y	200	200
Channel Z	200	200

8. Low Battery Alarm Voltage (Typical values for information)

Typical values	Alarm Level (VDC)
Supply (+ Vcc)	+7.9
Supply (- Vcc)	-7.6

9. Power Consumption (Typical values for information)

Typical values	Switched off (mA)	Stand by (mA)	Transmitting (mA)
Supply (+ Vcc)	+0.01	+8	+14
Supply (- Vcc)	-0.01	-8	-9

Certificate No: DAE4-1245_May22

Page 5 of 5

3 EX3DV4 - SN 7346

Calibration Laboratory of Schmid & Partner Engineering AG
Zürcherstrasse 6, 8004 Zürich, Switzerland

Accredited by the Swiss Accreditation Service (SAS)
The Swiss Accreditation Service is one of the signatories to the EA Multilateral Agreement for the recognition of calibration certificates

Client: **Auden** Certificate No: **EX3-7346_May22**

Accreditation No.: **SCS 0108**

Calibration Certificate

Object: **EX3DV4 - SN 7346**

Calibration procedure: **QA CAL-01 vs. QA CAL-14 vs. QA CAL-23 vs. QA CAL-25-V Calibration procedure for domestic E-field probes**

Calibration date: **March 30, 2022**

This calibration certificate documents the traceability to national standards, which requires the physical units of measurement (SI). The measurement and the uncertainty with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility, environment temperature (22 ± 0.5 °C and humidity < 70%).

Calibration Equipment used (MPE: usual for calibration):

Primary Standards	SI	Cal Date (Certificate No.)	Scheduled Calibration
Power meter M4P	58, 10479	08-Apr-21 (No. 217-0501-0303)	Apr-22
Power sensor HP-291	58, 10304	08-Apr-21 (No. 217-0501-0303)	Apr-22
Power sensor MPT-291	58, 10304	08-Apr-21 (No. 217-0501-0303)	Apr-22
Reference DUT attenuator	58, C22821 (20)	08-Apr-21 (No. 217-0501-0303)	Apr-22
DUT	58, 460	13-Dec-21 (No. DAE4-460, 0401)	Dec-22
Reference Probe (S202)	58, 3013	27-Dec-21 (No. E53-3013, 0401)	Dec-22

Secondary Standards

SI	Check Date (in house)	Scheduled Date
Power meter E413B	08-Apr-21 (in house check, Jan-22)	In house check, Jan-22
Power meter E413B	08-Apr-21 (in house check, Jan-22)	In house check, Jan-22
Power sensor E413A	08-Apr-21 (in house check, Jan-22)	In house check, Jan-22
Power sensor E413A	08-Apr-21 (in house check, Jan-22)	In house check, Jan-22
RF generator HP 8447A	08-Apr-21 (in house check, Jan-22)	In house check, Jan-22
RF generator HP 8447A	08-Apr-21 (in house check, Jan-22)	In house check, Jan-22
Network Analyzer B1300A	08-Apr-21 (in house check, Jan-22)	In house check, Jan-22

Calibrated by: **Heidi Schmid** Function: **Laboratory Technician** Signature: *[Signature]*

Approved by: **Oliver Koller** Function: **Quality Manager** Signature: *[Signature]*

This calibration certificate and not the reproduced image of it is valid without approval of the laboratory.

Certificate No: EX3-7346_May22 Page 1 of 24

Calibration Laboratory of Schmid & Partner Engineering AG
Zürcherstrasse 6, 8004 Zürich, Switzerland

Accredited by the Swiss Accreditation Service (SAS)
The Swiss Accreditation Service is one of the signatories to the EA Multilateral Agreement for the recognition of calibration certificates

Client: **Auden** Certificate No: **EX3-7346_May22**

Accreditation No.: **SCS 0108**

Glossary:

- TSL: traceability to national standards
- NORM(x,y,z): sensitivity in free space
- Comp: correction factor
- OCF: correction factor (15dB, cycle) of the RF signal
- A, B, C, D: modulation dependent parameters
- Polarization: rotation around probe axis
- Connector Angle: rotation around axis that is in the plane normal to probe axis (in measurement center)

Information used in DASY system to align probe sensor X to the robot coordinate system.

Calibration is performed according to the following standards:

- ISO/IEC 17025:2017, Measurement Procedure for the Assessment of Specific Absorption Rate of Human Exposure to Radio Frequency Fields From Hand-Held And Body-Worn Wireless Communication Devices, Part 1: Test Methods, Implementation And Procedures (Frequency Range of 4 MHz to 10 GHz), October 2020
- ISO 9001:2015, "SAE Measurement Requirements for 100 MHz to 6 GHz"

Methods Applied and Interpretation of Parameters:

- NORM(x,y,z): Assessed for E-field polarization: $E = 0$ (1 = 1000 MHz in TEM-cell; 1 = 1000 MHz R22 waveguide). NORM(x,y,z) are only reference values, i.e., the uncertainties of NORM(x,y,z) does not affect the E-field uncertainty model TSL (see below Comp).
- NORM(x,y,z) = NORM(x,y,z) * frequency response (see Frequency Response Chart). The frequency response is implemented in DASY software version 1.0. The uncertainty of the frequency response is included in the stated uncertainty of Comp.
- OCF(x,y,z): OCF is a nominalization parameter assessed based on the data of power sweep with CW signal (no uncertainty required). OCF does not depend on frequency nor media.
- PAC: PAC is the Peak to Average Ratio that is not calculated but determined based on the signal characteristics.
- A(x,y,z), B(x,y,z), C(x,y,z), D(x,y,z), V(x,y,z), A, B, C, D are numerical (scalar) parameters assessed based on the data of power sweep for specific modulation signal. The parameters do not depend on frequency nor media. V(x,y,z) is the maximum calibration range assessed in RMS voltage across the probe.
- Comp and Boundary Effect Parameters: Assessed in the probe using E-field (or Temperature Transfer Standard for f < 400 MHz) and inside waveguide using analytical field distributions based on power measurements for f > 400 MHz. The same values are used for assessment of the parameters applied by boundary compensation (alpha, depth) of which typical uncertainty values are given. These parameters are NORM(x,y,z) * Comp. The uncertainty of NORM(x,y,z) is not given for Comp. A frequency dependent Comp is used in DASY version 1.0 and higher which allows assessing the validity from > 50 MHz to > 100 MHz.
- Sensor Offset: The sensor offset corresponds to the effect of virtual measurement center from the probe tip (see probe axis). No tolerance required.
- Connector Angle: The angle is assessed using the information given by determining the NORM(x,y,z) uncertainty required.

Certificate No: EX3-7346_May22 Page 2 of 24



Unless otherwise agreed in writing, this document is issued by the Company subject to its General Conditions of Service printed overleaf, available on request or accessible at <http://www.sgs.com/en/Terms-and-Conditions.aspx> and, for electronic format documents, subject to Terms and Conditions for Electronic Documents at <http://www.sgs.com/en/Terms-and-Conditions/Terms-e-Documents.aspx>. Attention is drawn to the limitation of liability, indemnification and jurisdiction issues defined therein. Any holder of this document is advised that information contained hereon reflects the Company's findings at the time of its intervention only and within the limits of Client's instructions, if any. The Company's sole responsibility is to its Client and this document does not exonerate parties to a transaction from exercising all their rights and obligations under the transaction. This document cannot be reproduced except in full, without prior written approval of the Company. Any unauthorized alteration, forgery or falsification of the content or appearance of this document is unlawful and offenders may be prosecuted to the fullest extent of the law. Unless otherwise stated the results shown in this test report refer only to the sample(s) tested and such sample(s) are retained for 30 days only.


Attention: To check the authenticity of testing/inspection report & certificate, please contact us at telephone: (86-755) 8307 1443, or email: CN.Doccheck@sgs.com

No.10, Weyue Road, Innovation Park, Kunshan, Jiangsu, China 215300
中国·江苏·昆山市留学生创业园伟业路10号 邮编 215300

(86-512) 57355888 (86-512) 57370818 www.sgsgroup.com.cn
(86-512) 57355888 (86-512) 57370818 sgs.china@sgs.com

Page 3 of 24Page 4 of 24Page 5 of 24

Step 6 of 24

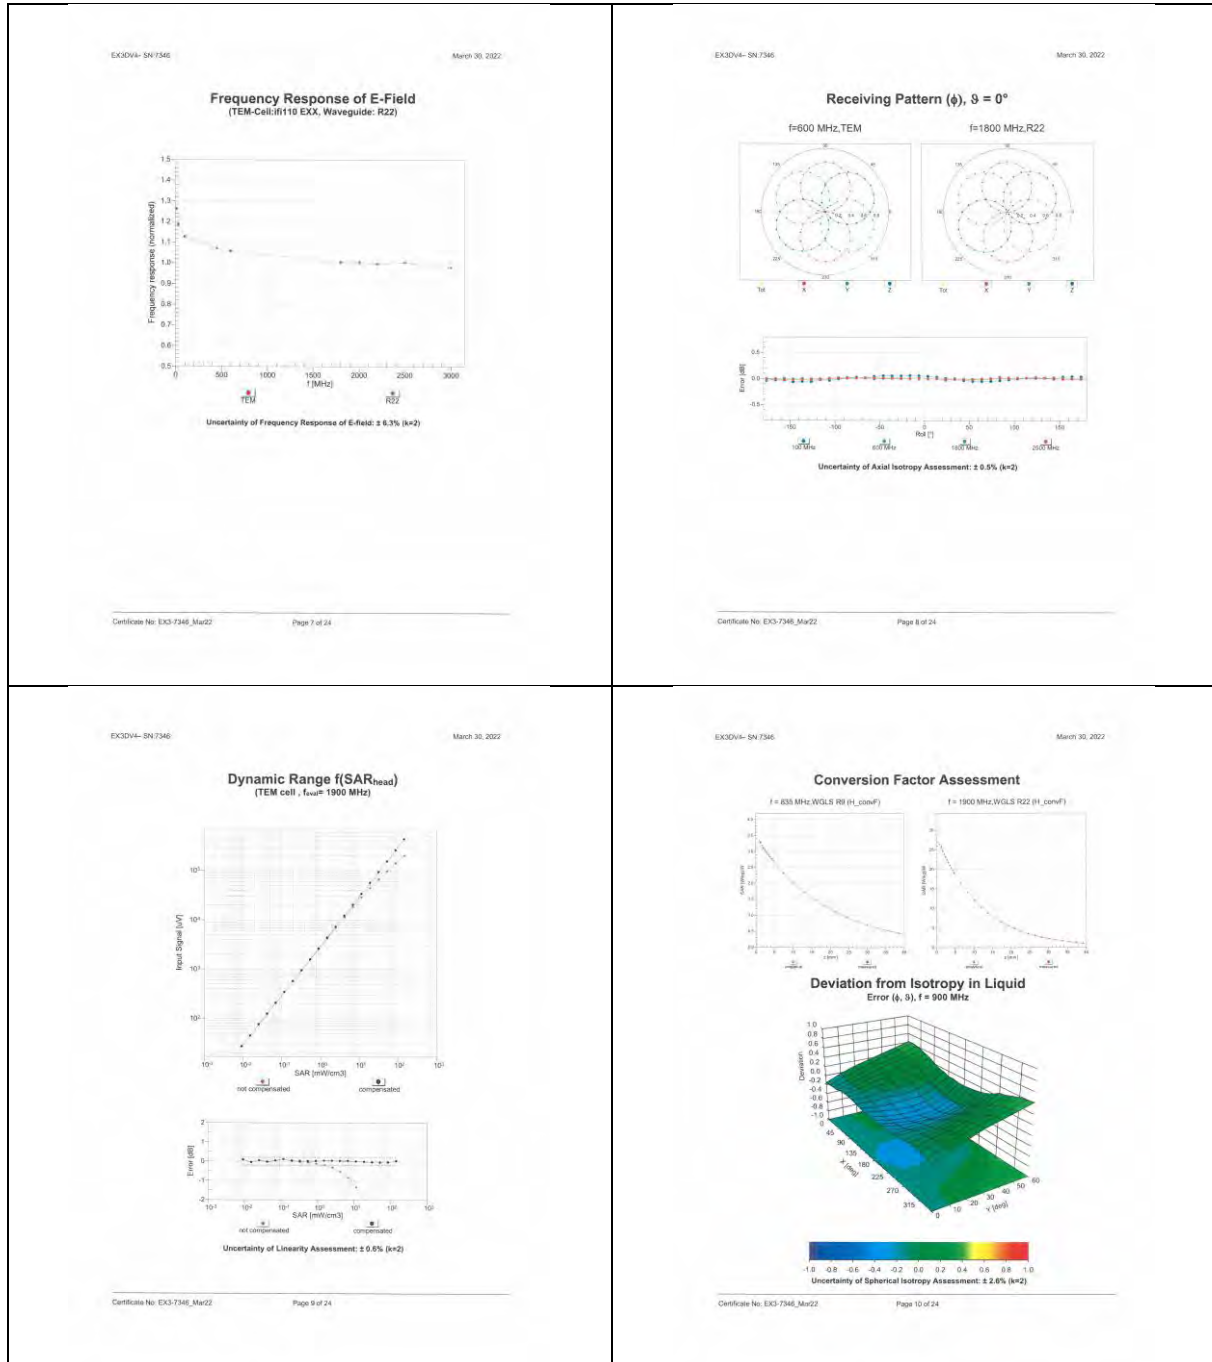

Unless otherwise agreed in writing, this document is issued by the Company subject to its General Conditions of Service printed overleaf, available on request or accessible at <http://www.sgs.com/en/Terms-and-Conditions.aspx> and, for electronic format documents, subject to Terms and Conditions for Electronic Documents at <http://www.sgs.com/en/Terms-and-Conditions/Terms-e-Documents.aspx>. Attention is drawn to the limitation of liability, indemnification and jurisdiction issues defined therein. Any holder of this document is advised that information contained hereon reflects the Company's findings at the time of its intervention only and within the limits of Client's instructions, if any. The Company's sole responsibility is to its Client and this document does not exonerate parties to a transaction from exercising all their rights and obligations under the transaction documents. This document cannot be reproduced except in full, without prior written approval of the Company. Any unauthorized alteration, forgery or falsification of the content or appearance of this document is unlawful and offenders may be prosecuted to the fullest extent of the law. Unless otherwise stated the results shown in this test report refer only to the sample(s) tested and such sample(s) are retained for 30 days only.

Attention: To check the authenticity of testing / inspection report & certificate, please contact us at telephone: (86-755) 8307 1443, or email: CN.Doccheck@sgs.com

No.10, Weiye Road, Innovation Park, Kunshan, Jiangsu, China 215300
中国·江苏·昆山市留学院创业园伟业路10号 邮编 215300

t(86-512)57355888 f(86-512)57370818 www.sgsgroup.com.cn
t(86-512)57355888 f(86-512)57370818 sgs.china@sgs.com

EX3034-EN7346

March 30, 2022

Append: Modulation Calibration Parameters

Uplink	Res	Communication System Name	Stream	PAIR	Mod	Mod	Mod	Mod	Mod
10000	CA	IEEE 802.11n HT Channel 1 (15 MHz)	CA	15.0	15.0	15.0	15.0	15.0	15.0
10001	CA	IEEE 802.11n HT Channel 2 (15 MHz)	CA	15.0	15.0	15.0	15.0	15.0	15.0
10002	CA	IEEE 802.11n HT Channel 3 (15 MHz)	CA	15.0	15.0	15.0	15.0	15.0	15.0
10003	CA	IEEE 802.11n HT Channel 4 (15 MHz)	CA	15.0	15.0	15.0	15.0	15.0	15.0
10004	CA	IEEE 802.11n HT Channel 5 (15 MHz)	CA	15.0	15.0	15.0	15.0	15.0	15.0
10005	CA	IEEE 802.11n HT Channel 6 (15 MHz)	CA	15.0	15.0	15.0	15.0	15.0	15.0
10006	CA	IEEE 802.11n HT Channel 7 (15 MHz)	CA	15.0	15.0	15.0	15.0	15.0	15.0
10007	CA	IEEE 802.11n HT Channel 8 (15 MHz)	CA	15.0	15.0	15.0	15.0	15.0	15.0
10008	CA	IEEE 802.11n HT Channel 9 (15 MHz)	CA	15.0	15.0	15.0	15.0	15.0	15.0
10009	CA	IEEE 802.11n HT Channel 10 (15 MHz)	CA	15.0	15.0	15.0	15.0	15.0	15.0
10010	CA	IEEE 802.11n HT Channel 11 (15 MHz)	CA	15.0	15.0	15.0	15.0	15.0	15.0
10011	CA	IEEE 802.11n HT Channel 12 (15 MHz)	CA	15.0	15.0	15.0	15.0	15.0	15.0
10012	CA	IEEE 802.11n HT Channel 13 (15 MHz)	CA	15.0	15.0	15.0	15.0	15.0	15.0
10013	CA	IEEE 802.11n HT Channel 14 (15 MHz)	CA	15.0	15.0	15.0	15.0	15.0	15.0
10014	CA	IEEE 802.11n HT Channel 15 (15 MHz)	CA	15.0	15.0	15.0	15.0	15.0	15.0
10015	CA	IEEE 802.11n HT Channel 16 (15 MHz)	CA	15.0	15.0	15.0	15.0	15.0	15.0
10016	CA	IEEE 802.11n HT Channel 17 (15 MHz)	CA	15.0	15.0	15.0	15.0	15.0	15.0
10017	CA	IEEE 802.11n HT Channel 18 (15 MHz)	CA	15.0	15.0	15.0	15.0	15.0	15.0
10018	CA	IEEE 802.11n HT Channel 19 (15 MHz)	CA	15.0	15.0	15.0	15.0	15.0	15.0
10019	CA	IEEE 802.11n HT Channel 20 (15 MHz)	CA	15.0	15.0	15.0	15.0	15.0	15.0
10020	CA	IEEE 802.11n HT Channel 21 (15 MHz)	CA	15.0	15.0	15.0	15.0	15.0	15.0
10021	CA	IEEE 802.11n HT Channel 22 (15 MHz)	CA	15.0	15.0	15.0	15.0	15.0	15.0
10022	CA	IEEE 802.11n HT Channel 23 (15 MHz)	CA	15.0	15.0	15.0	15.0	15.0	15.0
10023	CA	IEEE 802.11n HT Channel 24 (15 MHz)	CA	15.0	15.0	15.0	15.0	15.0	15.0
10024	CA	IEEE 802.11n HT Channel 25 (15 MHz)	CA	15.0	15.0	15.0	15.0	15.0	15.0
10025	CA	IEEE 802.11n HT Channel 26 (15 MHz)	CA	15.0	15.0	15.0	15.0	15.0	15.0
10026	CA	IEEE 802.11n HT Channel 27 (15 MHz)	CA	15.0	15.0	15.0	15.0	15.0	15.0
10027	CA	IEEE 802.11n HT Channel 28 (15 MHz)	CA	15.0	15.0	15.0	15.0	15.0	15.0
10028	CA	IEEE 802.11n HT Channel 29 (15 MHz)	CA	15.0	15.0	15.0	15.0	15.0	15.0
10029	CA	IEEE 802.11n HT Channel 30 (15 MHz)	CA	15.0	15.0	15.0	15.0	15.0	15.0
10030	CA	IEEE 802.11n HT Channel 31 (15 MHz)	CA	15.0	15.0	15.0	15.0	15.0	15.0
10031	CA	IEEE 802.11n HT Channel 32 (15 MHz)	CA	15.0	15.0	15.0	15.0	15.0	15.0
10032	CA	IEEE 802.11n HT Channel 33 (15 MHz)	CA	15.0	15.0	15.0	15.0	15.0	15.0
10033	CA	IEEE 802.11n HT Channel 34 (15 MHz)	CA	15.0	15.0	15.0	15.0	15.0	15.0
10034	CA	IEEE 802.11n HT Channel 35 (15 MHz)	CA	15.0	15.0	15.0	15.0	15.0	15.0
10035	CA	IEEE 802.11n HT Channel 36 (15 MHz)	CA	15.0	15.0	15.0	15.0	15.0	15.0
10036	CA	IEEE 802.11n HT Channel 37 (15 MHz)	CA	15.0	15.0	15.0	15.0	15.0	15.0
10037	CA	IEEE 802.11n HT Channel 38 (15 MHz)	CA	15.0	15.0	15.0	15.0	15.0	15.0
10038	CA	IEEE 802.11n HT Channel 39 (15 MHz)	CA	15.0	15.0	15.0	15.0	15.0	15.0
10039	CA	IEEE 802.11n HT Channel 40 (15 MHz)	CA	15.0	15.0	15.0	15.0	15.0	15.0
10040	CA	IEEE 802.11n HT Channel 41 (15 MHz)	CA	15.0	15.0	15.0	15.0	15.0	15.0
10041	CA	IEEE 802.11n HT Channel 42 (15 MHz)	CA	15.0	15.0	15.0	15.0	15.0	15.0
10042	CA	IEEE 802.11n HT Channel 43 (15 MHz)	CA	15.0	15.0	15.0	15.0	15.0	15.0
10043	CA	IEEE 802.11n HT Channel 44 (15 MHz)	CA	15.0	15.0	15.0	15.0	15.0	15.0
10044	CA	IEEE 802.11n HT Channel 45 (15 MHz)	CA	15.0	15.0	15.0	15.0	15.0	15.0
10045	CA	IEEE 802.11n HT Channel 46 (15 MHz)	CA	15.0	15.0	15.0	15.0	15.0	15.0
10046	CA	IEEE 802.11n HT Channel 47 (15 MHz)	CA	15.0	15.0	15.0	15.0	15.0	15.0
10047	CA	IEEE 802.11n HT Channel 48 (15 MHz)	CA	15.0	15.0	15.0	15.0	15.0	15.0
10048	CA	IEEE 802.11n HT Channel 49 (15 MHz)	CA	15.0	15.0	15.0	15.0	15.0	15.0
10049	CA	IEEE 802.11n HT Channel 50 (15 MHz)	CA	15.0	15.0	15.0	15.0	15.0	15.0
10050	CA	IEEE 802.11n HT Channel 51 (15 MHz)	CA	15.0	15.0	15.0	15.0	15.0	15.0
10051	CA	IEEE 802.11n HT Channel 52 (15 MHz)	CA	15.0	15.0	15.0	15.0	15.0	15.0
10052	CA	IEEE 802.11n HT Channel 53 (15 MHz)	CA	15.0	15.0	15.0	15.0	15.0	15.0
10053	CA	IEEE 802.11n HT Channel 54 (15 MHz)	CA	15.0	15.0	15.0	15.0	15.0	15.0
10054	CA	IEEE 802.11n HT Channel 55 (15 MHz)	CA	15.0	15.0	15.0	15.0	15.0	15.0
10055	CA	IEEE 802.11n HT Channel 56 (15 MHz)	CA	15.0	15.0	15.0	15.0	15.0	15.0
10056	CA	IEEE 802.11n HT Channel 57 (15 MHz)	CA	15.0	15.0	15.0	15.0	15.0	15.0
10057	CA	IEEE 802.11n HT Channel 58 (15 MHz)	CA	15.0	15.0	15.0	15.0	15.0	15.0
10058	CA	IEEE 802.11n HT Channel 59 (15 MHz)	CA	15.0	15.0	15.0	15.0	15.0	15.0
10059	CA	IEEE 802.11n HT Channel 60 (15 MHz)	CA	15.0	15.0	15.0	15.0	15.0	15.0
10060	CA	IEEE 802.11n HT Channel 61 (15 MHz)	CA	15.0	15.0	15.0	15.0	15.0	15.0
10061	CA	IEEE 802.11n HT Channel 62 (15 MHz)	CA	15.0	15.0	15.0	15.0	15.0	15.0
10062	CA	IEEE 802.11n HT Channel 63 (15 MHz)	CA	15.0	15.0	15.0	15.0	15.0	15.0
10063	CA	IEEE 802.11n HT Channel 64 (15 MHz)	CA	15.0	15.0	15.0	15.0	15.0	15.0
10064	CA	IEEE 802.11n HT Channel 65 (15 MHz)	CA	15.0	15.0	15.0	15.0	15.0	15.0
10065	CA	IEEE 802.11n HT Channel 66 (15 MHz)	CA	15.0	15.0	15.0	15.0	15.0	15.0
10066	CA	IEEE 802.11n HT Channel 67 (15 MHz)	CA	15.0	15.0	15.0	15.0	15.0	15.0
10067	CA	IEEE 802.11n HT Channel 68 (15 MHz)	CA	15.0	15.0	15.0	15.0	15.0	15.0
10068	CA	IEEE 802.11n HT Channel 69 (15 MHz)	CA	15.0	15.0	15.0	15.0	15.0	15.0
10069	CA	IEEE 802.11n HT Channel 70 (15 MHz)	CA	15.0	15.0	15.0	15.0	15.0	15.0
10070	CA	IEEE 802.11n HT Channel 71 (15 MHz)	CA	15.0	15.0	15.0	15.0	15.0	15.0
10071	CA	IEEE 802.11n HT Channel 72 (15 MHz)	CA	15.0	15.0	15.0	15.0	15.0	15.0
10072	CA	IEEE 802.11n HT Channel 73 (15 MHz)	CA	15.0	15.0	15.0	15.0	15.0	15.0
10073	CA	IEEE 802.11n HT Channel 74 (15 MHz)	CA	15.0	15.0	15.0	15.0	15.0	15.0
10074	CA	IEEE 802.11n HT Channel 75 (15 MHz)	CA	15.0	15.0	15.0	15.0	15.0	15.0
10075	CA	IEEE 802.11n HT Channel 76 (15 MHz)	CA	15.0	15.0	15.0	15.0	15.0	15.0
10076	CA	IEEE 802.11n HT Channel 77 (15 MHz)	CA	15.0	15.0	15.0	15.0	15.0	15.0
10077	CA	IEEE 802.11n HT Channel 78 (15 MHz)	CA	15.0	15.0	15.0	15.0	15.0	15.0
10078	CA	IEEE 802.11n HT Channel 79 (15 MHz)	CA	15.0	15.0	15.0	15.0	15.0	15.0
10079	CA	IEEE 802.11n HT Channel 80 (15 MHz)	CA	15.0	15.0	15.0	15.0	15.0	15.0
10080	CA	IEEE 802.11n HT Channel 81 (15 MHz)	CA	15.0	15.0	15.0	15.0	15.0	15.0
10081	CA	IEEE 802.11n HT Channel 82 (15 MHz)	CA	15.0	15.0	15.0	15.0	15.0	15.0
10082	CA	IEEE 802.11n HT Channel 83 (15 MHz)	CA	15.0	15.0	15.0	15.0	15.0	15.0
10083	CA	IEEE 802.11n HT Channel 84 (15 MHz)	CA	15.0	15.0	15.0	15.0	15.0	15.0
10084	CA	IEEE 802.11n HT Channel 85 (15 MHz)	CA	15.0	15.0	15.0	15.0	15.0	15.0
10085	CA	IEEE 802.11n HT Channel 86 (15 MHz)	CA	15.0	15.0	15.0	15.0	15.0	15.0
10086	CA	IEEE 802.11n HT Channel 87 (15 MHz)	CA	15.0	15.0	15.0	15.0	15.0	15.0
10087	CA	IEEE 802.11n HT Channel 88 (15 MHz)	CA	15.0	15.0	15.0	15.0	15.0	15.0
10088	CA	IEEE 802.11n HT Channel 89 (15 MHz)	CA	15.0	15.0	15.0	15.0	15.0	15.0
10089	CA	IEEE 802.11n HT Channel 90 (15 MHz)	CA	15.0	15.0	15.0	15.0	15.0	15.0
10090	CA	IEEE 802.11n HT Channel 91 (15 MHz)	CA	15.0	15.0	15.0	15.0	15.0	15.0
10091	CA	IEEE 802.11n HT Channel 92 (15 MHz)	CA	15.0	15.0	15.0	15.0	15.0	15.0
10092	CA	IEEE 802.11n HT Channel 93 (15 MHz)	CA	15.0	15.0	15.0	15.0	15.0	15.0
10093	CA	IEEE 802.11n HT Channel 94 (15 MHz)	CA	15.0	15.0	15.0	15.0	15.0	15.0
10094	CA	IEEE 802.11n HT Channel 95 (15 MHz)	CA	15.0	15.0	15.0	15.0	15.0	15.0
10095	CA	IEEE 802.11n HT Channel 96 (15 MHz)	CA	15.0	15.0	15.0	15.0	15.0	15.0
10096	CA	IEEE 802.11n HT Channel 97 (15 MHz)	CA	15.0	15.0	15.0	15.0	15.0	15.0
10097	CA	IEEE 802.11n HT Channel 98 (15 MHz)	CA	15.0	15.0	15.0	15.0	15.0	15.0
10098	CA	IEEE 802.11n HT Channel 99 (15 MHz)	CA	15.0	15.0	15.0	15.0	15.0	15.0
10099	CA	IEEE 802.11n HT Channel 100 (15 MHz)	CA	15.0	15.0	15.0	15.0	15.0	15.0
10100	CA	IEEE 802.11n HT Channel 101 (15 MHz)	CA	15.0	15.0	15.0	15.0	15.0	15.0
10101	CA	IEEE 802.11n HT Channel 102 (15 MHz)	CA	15.0	15.0	15.0	15.0	15.0	15.0
10102	CA	IEEE 802.11n HT Channel 103 (15 MHz)	CA	15.0	15.0	15.0	15.0	15.0	15.0
10103	CA	IEEE 802.11n HT Channel 104 (15 MHz)	CA	15.0	15.0	15.0	15.0	15.0	15.0
10104	CA	IEEE 802.11n HT Channel 105 (15 MHz)	CA	15.0	15.0	15.0	15.0	15.0	15.0
10105	CA	IEEE 802.11n HT Channel 106 (15 MHz)	CA	15.0	15.0	15.0	15.0	15.0	15.0
10106	CA	IEEE 802.11n HT Channel 107 (15 MHz)	CA	15.0	15.0	15.0	15.0	15.0	15.0
10107	CA	IEEE 802.11n HT Channel 108 (15 MHz)	CA	15.0	15.0	15.0	15.0	15.0	15.0
10108	CA	IEEE 802.11n HT Channel 109 (15 MHz)	CA	15.0	15.0	15.0	15.0	15.0	15.0
10109	CA	IEEE 802.11n HT Channel 110 (15 MHz)	CA	15.0	15.0	15.0	15.0	15.0	15.0
10110	CA	IEEE 802.11n HT Channel 111 (15 MHz)	CA	15.0	15.0	15.0	15.0	15.0	15.0
10111	CA	IEEE 802.11n HT Channel 112 (15 MHz)	CA	15.0	15.0	15.0	15.0	15.0	15.0
10112	CA	IEEE 802.11n HT Channel 113 (15 MHz)	CA	15.0	15.0	15.0	15.0	15.0	15.0
10113	CA	IEEE 802.11n HT Channel 114 (15 MHz)	CA	15.0	15.0	15.0	15.0	15.0	15.0
10114	CA	IEEE 802.11n HT Channel 115 (15 MHz)	CA	15.0	15.0	15.0	15.0	15.0	15.0
10115	CA	IEEE 802.11n HT Channel 116 (15 MHz)	CA	15.0	15.0	15.0	15.0	15	



EX3034-SN-7346							March 30, 2022	
10414	AAA	WLAN CDF4 64-QAM 40MHz	Generic	8.54	± 0.6 %			
10415	AAA	IEEE 802.11b WFI 2.4 GHz (DSSS, 1 Mbps, R90c-d)	WLAN	1.54	± 0.6 %			
10416	AAA	IEEE 802.11g WFI 2.4 GHz (DSSS-OFDM, 5.5 Mbps, R90c-d)	WLAN	8.23	± 0.6 %			
10417	AAC	IEEE 802.11n WFI 5 GHz (OFDM, 6 Mbps, R90c-d)	WLAN	8.23	± 0.6 %			
10418	AAA	IEEE 802.11g WFI 2.4 GHz (DSSS-OFDM, 5.5 Mbps, R90c-d)	WLAN	8.14	± 0.6 %			
10419	AAA	IEEE 802.11g WFI 2.4 GHz (DSSS-OFDM, 6 Mbps, R90c-d)	WLAN	8.19	± 0.6 %			
10420	AAC	IEEE 802.11n HT Overhead, 7.2 Mbps, R90c-d	WLAN	8.32	± 0.6 %			
10421	AAC	IEEE 802.11n HT Overhead, 6.3 Mbps, 16-QAM	WLAN	8.47	± 0.6 %			
10424	AAC	IEEE 802.11n HT Overhead, 7.2 Mbps, 64-QAM	WLAN	8.40	± 0.6 %			
10425	AAC	IEEE 802.11n HT Overhead, 14 Mbps, R90c-d	WLAN	8.41	± 0.6 %			
10426	AAC	IEEE 802.11n HT Overhead, 30 Mbps, 16-QAM	WLAN	8.45	± 0.6 %			
10427	AAC	IEEE 802.11n HT Overhead, 130 Mbps, 64-QAM	WLAN	8.41	± 0.6 %			
10430	AAD	LTE-FDD OFDMA, 5 MHz, E-TRP 3.1	LTE-FDD	8.28	± 0.6 %			
10431	AAD	LTE-FDD OFDMA, 10 MHz, E-TRP 3.1	LTE-FDD	8.38	± 0.6 %			
10432	AAC	LTE-FDD OFDMA, 15 MHz, E-TRP 3.1	LTE-FDD	8.34	± 0.6 %			
10433	AAC	LTE-FDD OFDMA, 20 MHz, E-TRP 3.1	LTE-FDD	8.34	± 0.6 %			
10434	AAA	WCDMA (BS Test Model 1, 64 DPCCH)	WCDMA	8.60	± 0.6 %			
10435	AAF	LTE-TDD (SC-FDMA, 1 RB, 20 MHz, QPSK, UL Sub)	LTE-TDD	7.82	± 0.6 %			
10447	AAD	LTE-FDD OFDMA, 5 MHz, E-TRP 3.1, Clipping 44%	LTE-FDD	7.86	± 0.6 %			
10448	AAD	LTE-FDD OFDMA, 10 MHz, E-TRP 3.1, Clipping 44%	LTE-FDD	7.93	± 0.6 %			
10449	AAC	LTE-FDD OFDMA, 15 MHz, E-TRP 3.1, Clipping 44%	LTE-FDD	7.91	± 0.6 %			
10450	AAC	LTE-FDD OFDMA, 20 MHz, E-TRP 3.1, Clipping 44%	LTE-FDD	7.88	± 0.6 %			
10451	AAA	WCDMA (BS Test Model 1, 64 DPCCH, Clipping 44%)	WCDMA	7.89	± 0.6 %			
10452	AAD	Validation (Spurious, 10ms, 1ms)	Test	10.00	± 0.6 %			
10453	AAC	IEEE 802.11ac WFI (80MHz, 64-QAM, R90c-d)	WLAN	8.63	± 0.6 %			
10457	AAA	UMTS FDD (SC-HSPA)	WCDMA	6.62	± 0.6 %			
10458	AAA	CDMA2000 (1xEV-DO, Rev. 8, 3 carriers)	CDMA2000	8.58	± 0.6 %			
10459	AAA	CDMA2000 (1xEV-DO, Rev. 8, 3 carriers)	CDMA2000	8.25	± 0.6 %			
10462	AAA	UMTS FDD (HSPA, R90c-d)	WCDMA	2.39	± 0.6 %			
10463	AAB	LTE-TDD (SC-FDMA, 1 RB, 1.4 MHz, QPSK, UL Sub)	LTE-TDD	7.82	± 0.6 %			
10462	AAB	LTE-TDD (SC-FDMA, 1 RB, 1.4 MHz, 16-QAM, UL Sub)	LTE-TDD	8.30	± 0.6 %			
10463	AAB	LTE-TDD (SC-FDMA, 1 RB, 1.4 MHz, 64-QAM, UL Sub)	LTE-TDD	8.30	± 0.6 %			
10464	AAC	LTE-TDD (SC-FDMA, 1 RB, 3.1 MHz, QPSK, UL Sub)	LTE-TDD	7.82	± 0.6 %			
10465	AAC	LTE-TDD (SC-FDMA, 1 RB, 3.1 MHz, 16-QAM, UL Sub)	LTE-TDD	8.32	± 0.6 %			
10466	AAC	LTE-TDD (SC-FDMA, 1 RB, 3.1 MHz, 64-QAM, UL Sub)	LTE-TDD	8.32	± 0.6 %			
10467	AAF	LTE-TDD (SC-FDMA, 1 RB, 3.1 MHz, QPSK, UL Sub)	LTE-TDD	7.82	± 0.6 %			
10468	AAF	LTE-TDD (SC-FDMA, 1 RB, 3.1 MHz, 16-QAM, UL Sub)	LTE-TDD	8.32	± 0.6 %			
10469	AAF	LTE-TDD (SC-FDMA, 1 RB, 3.1 MHz, 64-QAM, UL Sub)	LTE-TDD	8.32	± 0.6 %			
10470	AAF	LTE-TDD (SC-FDMA, 1 RB, 3.1 MHz, QPSK, UL Sub)	LTE-TDD	7.82	± 0.6 %			
10471	AAF	LTE-TDD (SC-FDMA, 1 RB, 3.1 MHz, 16-QAM, UL Sub)	LTE-TDD	8.32	± 0.6 %			
10472	AAF	LTE-TDD (SC-FDMA, 1 RB, 3.1 MHz, 64-QAM, UL Sub)	LTE-TDD	8.32	± 0.6 %			
10473	AAB	LTE-TDD (SC-FDMA, 1 RB, 3.1 MHz, QPSK, UL Sub)	LTE-TDD	7.82	± 0.6 %			
10474	AAB	LTE-TDD (SC-FDMA, 1 RB, 3.1 MHz, 16-QAM, UL Sub)	LTE-TDD	8.32	± 0.6 %			
10475	AAB	LTE-TDD (SC-FDMA, 1 RB, 3.1 MHz, 64-QAM, UL Sub)	LTE-TDD	8.32	± 0.6 %			
10476	AAF	LTE-TDD (SC-FDMA, 1 RB, 3.1 MHz, QPSK, UL Sub)	LTE-TDD	7.82	± 0.6 %			
10477	AAF	LTE-TDD (SC-FDMA, 1 RB, 3.1 MHz, 16-QAM, UL Sub)	LTE-TDD	8.32	± 0.6 %			
10478	AAF	LTE-TDD (SC-FDMA, 1 RB, 3.1 MHz, 64-QAM, UL Sub)	LTE-TDD	8.32	± 0.6 %			
10479	AAB	LTE-TDD (SC-FDMA, 1 RB, 3.1 MHz, QPSK, UL Sub)	LTE-TDD	7.82	± 0.6 %			
10480	AAB	LTE-TDD (SC-FDMA, 1 RB, 3.1 MHz, 16-QAM, UL Sub)	LTE-TDD	8.32	± 0.6 %			
10481	AAB	LTE-TDD (SC-FDMA, 1 RB, 3.1 MHz, 64-QAM, UL Sub)	LTE-TDD	8.32	± 0.6 %			
10482	AAC	LTE-TDD (SC-FDMA, 1 RB, 3.1 MHz, QPSK, UL Sub)	LTE-TDD	7.82	± 0.6 %			
10483	AAC	LTE-TDD (SC-FDMA, 1 RB, 3.1 MHz, 16-QAM, UL Sub)	LTE-TDD	8.32	± 0.6 %			
10484	AAC	LTE-TDD (SC-FDMA, 1 RB, 3.1 MHz, 64-QAM, UL Sub)	LTE-TDD	8.32	± 0.6 %			
10485	AAF	LTE-TDD (SC-FDMA, 1 RB, 3.1 MHz, QPSK, UL Sub)	LTE-TDD	7.82	± 0.6 %			
10486	AAF	LTE-TDD (SC-FDMA, 1 RB, 3.1 MHz, 16-QAM, UL Sub)	LTE-TDD	8.32	± 0.6 %			
10487	AAF	LTE-TDD (SC-FDMA, 1 RB, 3.1 MHz, 64-QAM, UL Sub)	LTE-TDD	8.32	± 0.6 %			
10488	AAF	LTE-TDD (SC-FDMA, 1 RB, 3.1 MHz, QPSK, UL Sub)	LTE-TDD	7.82	± 0.6 %			
Certificate No. EX3-7346_Mar22							Page 15 of 24	
EX3034-SN-7346							March 30, 2022	
10487	AAC	IEEE 802.11ac WFI (80MHz, MCS9, R90c-d)	WLAN	8.49	± 0.6 %			
10488	AAC	IEEE 802.11ac WFI (80MHz, MCS9, R90c-d)	WLAN	8.37	± 0.6 %			
10489	AAC	IEEE 802.11ac WFI (80MHz, MCS9, R90c-d)	WLAN	8.39	± 0.6 %			
10490	AAC	IEEE 802.11ac WFI (80MHz, MCS9, R90c-d)	WLAN	8.39	± 0.6 %			
10491	AAC	IEEE 802.11ac WFI (80MHz, MCS9, R90c-d)	WLAN	8.39	± 0.6 %			
10492	AAC	IEEE 802.11ac WFI (80MHz, MCS9, R90c-d)	WLAN	8.42	± 0.6 %			
10493	AAC	IEEE 802.11ac WFI (80MHz, MCS9, R90c-d)	WLAN	8.42	± 0.6 %			
10494	AAC	IEEE 802.11ac WFI (80MHz, MCS9, R90c-d)	WLAN	8.48	± 0.6 %			
10495	AAD	IEEE 802.11ac WFI (160MHz, MCS9, R90c-d)	WLAN	8.47	± 0.6 %			
10496	AAD	IEEE 802.11ac WFI (160MHz, MCS9, R90c-d)	WLAN	8.47	± 0.6 %			
10497	AAD	IEEE 802.11ac WFI (160MHz, MCS9, R90c-d)	WLAN	8.50	± 0.6 %			
10498	AAD	IEEE 802.11ac WFI (160MHz, MCS9, R90c-d)	WLAN	8.52	± 0.6 %			
10499	AAD	IEEE 802.11ac WFI (160MHz, MCS9, R90c-d)	WLAN	8.52	± 0.6 %			
10500	AAD	IEEE 802.11ac WFI (160MHz, MCS9, R90c-d)	WLAN	8.52	± 0.6 %			
10501	AAD	IEEE 802.11ac WFI (160MHz, MCS9, R90c-d)	WLAN	8.52	± 0.6 %			
10502	AAD	IEEE 802.11ac WFI (160MHz, MCS9, R90c-d)	WLAN	8.52	± 0.6 %			
10503	AAD	IEEE 802.11ac WFI (160MHz, MCS9, R90c-d)	WLAN	8.52	± 0.6 %			
10504	AAD	IEEE 802.11ac WFI (160MHz, MCS9, R90c-d)	WLAN	8.52	± 0.6 %			
10505	AAA	IEEE 802.11g WFI 2.4 GHz (DSSS-OFDM, 12 Mbps, R90c-d)	WLAN	8.45	± 0.6 %			
10506	AAA	IEEE 802.11g WFI 2.4 GHz (DSSS-OFDM, 18 Mbps, R90c-d)	WLAN	8.13	± 0.6 %			
10507	AAA	IEEE 802.11g WFI 2.4 GHz (DSSS-OFDM, 24 Mbps, R90c-d)	WLAN	8.09	± 0.6 %			
10508	AAA	IEEE 802.11g WFI 2.4 GHz (DSSS-OFDM, 36 Mbps, R90c-d)	WLAN	8.37	± 0.6 %			
10509	AAA	IEEE 802.11g WFI 2.4 GHz (DSSS-OFDM, 48 Mbps, R90c-d)	WLAN	8.10	± 0.6 %			
10510	AAA	IEEE 802.11g WFI 2.4 GHz (DSSS-OFDM, 54 Mbps, R90c-d)	WLAN	8.30	± 0.6 %			
10511	AAA	IEEE 802.11g WFI 2.4 GHz (DSSS, 1 Mbps, R90c-d)	WLAN	1.99	± 0.6 %			
10512	AAA	IEEE 802.11g WFI 2.4 GHz (DSSS, 2 Mbps, R90c-d)	WLAN	1.99	± 0.6 %			
10513	AAA	IEEE 802.11g WFI 2.4 GHz (DSSS, 5.5 Mbps, R90c-d)	WLAN	1.98	± 0.6 %			
10514	AAA	IEEE 802.11g WFI 2.4 GHz (DSSS, 11 Mbps, R90c-d)	WLAN	1.98	± 0.6 %			
10515	AAA	IEEE 802.11g WFI 2.4 GHz (DSSS-OFDM, 6 Mbps, R90c-d)	WLAN	8.89	± 0.6 %			
10516	AAA	IEEE 802.11g WFI 2.4 GHz (DSSS-OFDM, 9 Mbps, R90c-d)	WLAN	8.80	± 0.6 %			
10517	AAA	IEEE 802.11g WFI 2.4 GHz (DSSS-OFDM, 12 Mbps, R90c-d)	WLAN	8.79	± 0.6 %			
10518	AAA	IEEE 802.11g WFI 2.4 GHz (DSSS-OFDM, 18 Mbps, R90c-d)	WLAN	8.49	± 0.6 %			
10519	AAA	IEEE 802.11g WFI 2.4 GHz (DSSS-OFDM, 24 Mbps, R90c-d)	WLAN	8.49	± 0.6 %			
10520	AAA	IEEE 802.11g WFI 2.4 GHz (DSSS-OFDM, 36 Mbps, R90c-d)	WLAN	8.76	± 0.6 %			
10521	AAA	IEEE 802.11g WFI 2.4 GHz (DSSS-OFDM, 48 Mbps, R90c-d)	WLAN	8.75	± 0.6 %			
10522	AAA	IEEE 802.11g WFI 2.4 GHz (DSSS-OFDM, 54 Mbps, R90c-d)	WLAN	8.67	± 0.6 %			
10523	AAA	IEEE 802.11g WFI 5 GHz (OFDM, 6 Mbps, R90c-d)	WLAN	8.89	± 0.6 %			
10524	AAA	IEEE 802.11g WFI 5 GHz (OFDM, 9 Mbps, R90c-d)	WLAN	8.89	± 0.6 %			
10525	AAA	IEEE 802.11g WFI 5 GHz (OFDM, 12 Mbps, R90c-d)	WLAN	8.70	± 0.6 %			
10526	AAC	IEEE 802.11n WFI 5 GHz (OFDM, 18 Mbps, R90c-d)	WLAN	8.49	± 0.6 %			
10527	AAC	IEEE 802.11n WFI 5 GHz (OFDM, 24 Mbps, R90c-d)	WLAN	8.36	± 0.6 %			
10528	AAC	IEEE 802.11n WFI 5 GHz (OFDM, 36 Mbps, R90c-d)	WLAN	8.76	± 0.6 %			
10529	AAC	IEEE 802.11n WFI 5 GHz (OFDM, 48 Mbps, R90c-d)	WLAN	8.76	± 0.6 %			
10530	AAC	IEEE 802.11n WFI 5 GHz (OFDM, 54 Mbps, R90c-d)	WLAN	8.67	± 0.6 %			
10531	AAC	IEEE 802.11n HT WFI 5 GHz (OFDM, 12 Mbps, R90c-d)	WLAN	8.63	± 0.6 %			
10532	AAC	IEEE 802.11n HT WFI 5 GHz (OFDM, 18 Mbps, R90c-d)	WLAN	8.79	± 0.6 %			
10533	AAC	IEEE 802.11n HT WFI 5 GHz (OFDM, 24 Mbps, R90c-d)	WLAN	8.74	± 0.6 %			
10534	AAC	IEEE 802.11n HT WFI 5 GHz (OFDM, 36 Mbps, R90c-d)	WLAN	8.74	± 0.6 %			
10535	AAC	IEEE 802.11n HT WFI 5 GHz (OFDM, 48 Mbps, R90c-d)	WLAN	8.71	± 0.6 %			
10536	AAC	IEEE 802.11n HT WFI 5 GHz (OFDM, 54 Mbps, R90c-d)	WLAN	8.72	± 0.6 %			
10537	AAC	IEEE 802.11n HT WFI 5 GHz (OFDM, 12 Mbps, R90c-d)	WLAN	8.50	± 0.6 %			
10538	AAC	IEEE 802.11n HT WFI 5 GHz (OFDM, 18 Mbps, R90c-d)	WLAN	8.79	± 0.6 %			
10539	AAC	IEEE 802.11n HT WFI 5 GHz (OFDM, 24 Mbps, R90c-d)	WLAN	8.88	± 0.6 %			
10540	AAC	IEEE 802.11n HT WFI 5 GHz (OFDM, 36 Mbps, R90c-d)	WLAN	8.88	± 0.6 %			
10541	AAC	IEEE 802.11n HT WFI 5 GHz (OFDM, 48 Mbps, R90c-d)	WLAN	8.84	± 0.6 %			
10542	AAC	IEEE 802.11n HT WFI 5 GHz (OFDM, 54 Mbps, R90c-d)	WLAN	8.83	± 0.6 %			
10543	AAC	IEEE 802.11n HT WFI 5 GHz (OFDM, 12 Mbps, R90c-d)	WLAN	8.84	± 0.6 %			
10544	AAC	IEEE 802.11n HT WFI 5 GHz (OFDM, 18 Mbps, R90c-d)	WLAN	8.83	± 0.6 %			
10545	AAC	IEEE 802.11n HT WFI 5 GHz (OFDM, 24 Mbps, R90c-d)	WLAN	8.83	± 0.6 %			
10546	AAC	IEEE 802.11n HT WFI 5 GHz (OFDM, 36 Mbps, R90c-d)	WLAN	8.83	± 0.6 %			
10547	AAC	IEEE 802.11n HT WFI 5 GHz (OFDM, 48 Mbps, R90c-d)	WLAN	8.83	± 0.6 %			
10548	AAA	CDMA2000 (1xEV-DO, Rev. 8, 3 carriers)	CDMA2000	8.45	± 0.6 %			
10549	AAA	CDMA2000 (1xEV-DO, Rev. 8, 3 carriers)	CDMA2000	8.45	± 0.6 %			
10550	AAA	CDMA2000 (1xEV-DO, Rev. 8, 3 carriers)	CDMA2000	8.45	± 0.6 %			
10551	AAA	CDMA2000 (1xEV-DO, Rev. 8, 3 carriers)	CDMA2000	8.45	± 0.6 %			
10552	AAA	CDMA2000 (1xEV-DO, Rev. 8, 3 carriers)	CDMA2000	8.45	±			

ECS04v4-047346			March 30, 2022			ECS04v4-047346			March 30, 2022		
106751	AAC	IEEE 802.11ax (QOMM, MCS2, 90pc dc)	WLAN	8.78	± 0.6 %	107229	AAC	IEEE 802.11ax (BOMM, MCS31, 90pc dc)	WLAN	8.64	± 0.6 %
106752	AAC	IEEE 802.11ax (QOMM, MCS3, 90pc dc)	WLAN	8.74	± 0.6 %	107230	AAC	IEEE 802.11ax (BOMM, MCS31, 90pc dc)	WLAN	8.67	± 0.6 %
106753	AAC	IEEE 802.11ax (QOMM, MCS4, 90pc dc)	WLAN	8.80	± 0.6 %	107231	AAC	IEEE 802.11ax (BOMM, MCS31, 90pc dc)	WLAN	8.43	± 0.6 %
106754	AAC	IEEE 802.11ax (QOMM, MCS5, 90pc dc)	WLAN	8.77	± 0.6 %	107232	AAC	IEEE 802.11ax (BOMM, MCS31, 90pc dc)	WLAN	8.46	± 0.6 %
106755	AAC	IEEE 802.11ax (QOMM, MCS6, 90pc dc)	WLAN	8.73	± 0.6 %	107233	AAC	IEEE 802.11ax (BOMM, MCS31, 90pc dc)	WLAN	8.40	± 0.6 %
106756	AAC	IEEE 802.11ax (QOMM, MCS7, 90pc dc)	WLAN	8.78	± 0.6 %	107234	AAC	IEEE 802.11ax (BOMM, MCS31, 90pc dc)	WLAN	8.27	± 0.6 %
106757	AAC	IEEE 802.11ax (QOMM, MCS8, 90pc dc)	WLAN	8.89	± 0.6 %	107235	AAC	IEEE 802.11ax (BOMM, MCS31, 90pc dc)	WLAN	8.73	± 0.6 %
106802	AAC	IEEE 802.11ax (QOMM, MCS10, 90pc dc)	WLAN	8.80	± 0.6 %	107236	AAC	IEEE 802.11ax (BOMM, MCS31, 90pc dc)	WLAN	8.47	± 0.6 %
106801	AAC	IEEE 802.11ax (QOMM, MCS10, 90pc dc)	WLAN	8.62	± 0.6 %	107237	AAC	IEEE 802.11ax (BOMM, MCS31, 90pc dc)	WLAN	8.78	± 0.6 %
106802	AAC	IEEE 802.11ax (QOMM, MCS11, 90pc dc)	WLAN	8.83	± 0.6 %	107238	AAC	IEEE 802.11ax (BOMM, MCS31, 90pc dc)	WLAN	8.45	± 0.6 %
106803	AAC	IEEE 802.11ax (QOMM, MCS9, 90pc dc)	WLAN	8.43	± 0.6 %	107239	AAC	IEEE 802.11ax (BOMM, MCS31, 90pc dc)	WLAN	8.29	± 0.6 %
106804	AAC	IEEE 802.11ax (QOMM, MCS11, 90pc dc)	WLAN	8.26	± 0.6 %	107240	AAC	IEEE 802.11ax (BOMM, MCS31, 90pc dc)	WLAN	8.48	± 0.6 %
106805	AAC	IEEE 802.11ax (QOMM, MCS2, 90pc dc)	WLAN	8.33	± 0.6 %	107241	AAC	IEEE 802.11ax (BOMM, MCS31, 90pc dc)	WLAN	8.40	± 0.6 %
106806	AAC	IEEE 802.11ax (QOMM, MCS3, 90pc dc)	WLAN	8.28	± 0.6 %	107242	AAC	IEEE 802.11ax (BOMM, MCS31, 90pc dc)	WLAN	8.44	± 0.6 %
106807	AAC	IEEE 802.11ax (QOMM, MCS4, 90pc dc)	WLAN	8.45	± 0.6 %	107243	AAC	IEEE 802.11ax (BOMM, MCS31, 90pc dc)	WLAN	8.76	± 0.6 %
106808	AAC	IEEE 802.11ax (QOMM, MCS5, 90pc dc)	WLAN	8.29	± 0.6 %	107244	AAC	IEEE 802.11ax (BOMM, MCS31, 90pc dc)	WLAN	8.56	± 0.6 %
106809	AAC	IEEE 802.11ax (QOMM, MCS6, 90pc dc)	WLAN	8.55	± 0.6 %	107245	AAC	IEEE 802.11ax (BOMM, MCS31, 90pc dc)	WLAN	8.85	± 0.6 %
106810	AAC	IEEE 802.11ax (QOMM, MCS7, 90pc dc)	WLAN	8.29	± 0.6 %	107246	AAC	IEEE 802.11ax (BOMM, MCS31, 90pc dc)	WLAN	8.71	± 0.6 %
106811	AAC	IEEE 802.11ax (QOMM, MCS8, 90pc dc)	WLAN	8.25	± 0.6 %	107247	AAC	IEEE 802.11ax (BOMM, MCS31, 90pc dc)	WLAN	7.65	± 0.6 %
106812	AAC	IEEE 802.11ax (QOMM, MCS9, 90pc dc)	WLAN	8.29	± 0.6 %	107248	AAC	IEEE 802.11ax (BOMM, MCS31, 90pc dc)	WLAN	8.53	± 0.6 %
106813	AAC	IEEE 802.11ax (QOMM, MCS10, 90pc dc)	WLAN	8.25	± 0.6 %	107249	AAC	IEEE 802.11ax (BOMM, MCS31, 90pc dc)	WLAN	8.88	± 0.6 %
106814	AAC	IEEE 802.11ax (QOMM, MCS11, 90pc dc)	WLAN	8.57	± 0.6 %	107250	AAC	IEEE 802.11ax (BOMM, MCS31, 90pc dc)	WLAN	8.79	± 0.6 %
106905	AAC	IEEE 802.11ax (QOMM, MCS6, 90pc dc)	WLAN	8.78	± 0.6 %	107251	AAC	IEEE 802.11ax (BOMM, MCS31, 90pc dc)	WLAN	8.62	± 0.6 %
106906	AAC	IEEE 802.11ax (QOMM, MCS11, 90pc dc)	WLAN	8.91	± 0.6 %	107252	AAC	IEEE 802.11ax (BOMM, MCS31, 90pc dc)	WLAN	8.61	± 0.6 %
106907	AAC	IEEE 802.11ax (QOMM, MCS2, 90pc dc)	WLAN	8.61	± 0.6 %	107253	AAC	IEEE 802.11ax (BOMM, MCS31, 90pc dc)	WLAN	8.50	± 0.6 %
106908	AAC	IEEE 802.11ax (QOMM, MCS4, 90pc dc)	WLAN	8.89	± 0.6 %	107254	AAC	IEEE 802.11ax (BOMM, MCS31, 90pc dc)	WLAN	8.56	± 0.6 %
106909	AAC	IEEE 802.11ax (QOMM, MCS4, 90pc dc)	WLAN	8.82	± 0.6 %	107255	AAC	IEEE 802.11ax (BOMM, MCS31, 90pc dc)	WLAN	8.84	± 0.6 %
107000	AAC	IEEE 802.11ax (QOMM, MCS6, 90pc dc)	WLAN	8.73	± 0.6 %	107256	AAC	IEEE 802.11ax (BOMM, MCS31, 90pc dc)	WLAN	8.77	± 0.6 %
107001	AAC	IEEE 802.11ax (QOMM, MCS6, 90pc dc)	WLAN	8.86	± 0.6 %	107257	AAC	IEEE 802.11ax (BOMM, MCS31, 90pc dc)	WLAN	8.77	± 0.6 %
107002	AAC	IEEE 802.11ax (QOMM, MCS7, 90pc dc)	WLAN	8.70	± 0.6 %	107258	AAC	IEEE 802.11ax (BOMM, MCS31, 90pc dc)	WLAN	8.68	± 0.6 %
107003	AAC	IEEE 802.11ax (QOMM, MCS8, 90pc dc)	WLAN	8.62	± 0.6 %	107259	AAC	IEEE 802.11ax (BOMM, MCS31, 90pc dc)	WLAN	8.58	± 0.6 %
107004	AAC	IEEE 802.11ax (QOMM, MCS8, 90pc dc)	WLAN	8.56	± 0.6 %	107260	AAC	IEEE 802.11ax (BOMM, MCS31, 90pc dc)	WLAN	8.40	± 0.6 %
107005	AAC	IEEE 802.11ax (QOMM, MCS10, 90pc dc)	WLAN	8.69	± 0.6 %	107261	AAC	IEEE 802.11ax (BOMM, MCS31, 90pc dc)	WLAN	8.58	± 0.6 %
107006	AAC	IEEE 802.11ax (QOMM, MCS11, 90pc dc)	WLAN	8.68	± 0.6 %	107262	AAC	IEEE 802.11ax (BOMM, MCS31, 90pc dc)	WLAN	8.49	± 0.6 %
107007	AAC	IEEE 802.11ax (QOMM, MCS9, 90pc dc)	WLAN	8.32	± 0.6 %	107263	AAC	IEEE 802.11ax (BOMM, MCS31, 90pc dc)	WLAN	8.53	± 0.6 %
107008	AAC	IEEE 802.11ax (QOMM, MCS9, 90pc dc)	WLAN	8.55	± 0.6 %	107264	AAC	IEEE 802.11ax (BOMM, MCS31, 90pc dc)	WLAN	8.40	± 0.6 %
107009	AAC	IEEE 802.11ax (QOMM, MCS2, 90pc dc)	WLAN	8.33	± 0.6 %	107265	AAC	IEEE 802.11ax (BOMM, MCS31, 90pc dc)	WLAN	8.54	± 0.6 %
107010	AAC	IEEE 802.11ax (QOMM, MCS3, 90pc dc)	WLAN	8.29	± 0.6 %	107266	AAC	IEEE 802.11ax (BOMM, MCS31, 90pc dc)	WLAN	8.51	± 0.6 %
107111	AAC	IEEE 802.11ax (QOMM, MCS4, 90pc dc)	WLAN	8.39	± 0.6 %	107267	AAC	IEEE 802.11ax (BOMM, MCS31, 90pc dc)	WLAN	8.58	± 0.6 %
107112	AAC	IEEE 802.11ax (QOMM, MCS5, 90pc dc)	WLAN	8.67	± 0.6 %	107268	AAC	IEEE 802.11ax (BOMM, MCS31, 90pc dc)	WLAN	8.61	± 0.6 %
107113	AAC	IEEE 802.11ax (QOMM, MCS6, 90pc dc)	WLAN	8.33	± 0.6 %	107269	AAC	IEEE 802.11ax (BOMM, MCS31, 90pc dc)	WLAN	8.61	± 0.6 %
107114	AAC	IEEE 802.11ax (QOMM, MCS7, 90pc dc)	WLAN	8.26	± 0.6 %	107270	AAC	IEEE 802.11ax (BOMM, MCS31, 90pc dc)	WLAN	8.61	± 0.6 %
107115	AAC	IEEE 802.11ax (QOMM, MCS8, 90pc dc)	WLAN	8.43	± 0.6 %	107271	AAC	IEEE 802.11ax (BOMM, MCS31, 90pc dc)	WLAN	8.62	± 0.6 %
107116	AAC	IEEE 802.11ax (QOMM, MCS9, 90pc dc)	WLAN	8.30	± 0.6 %	107272	AAC	IEEE 802.11ax (BOMM, MCS31, 90pc dc)	WLAN	8.29	± 0.6 %
107117	AAC	IEEE 802.11ax (QOMM, MCS10, 90pc dc)	WLAN	8.48	± 0.6 %	107273	AAC	IEEE 802.11ax (BOMM, MCS31, 90pc dc)	WLAN	8.63	± 0.6 %
107118	AAC	IEEE 802.11ax (QOMM, MCS10, 90pc dc)	WLAN	8.24	± 0.6 %	107274	AAC	IEEE 802.11ax (BOMM, MCS31, 90pc dc)	WLAN	8.26	± 0.6 %
107119	AAC	IEEE 802.11ax (BOMM, MCS6, 90pc dc)	WLAN	8.81	± 0.6 %	107275	AAC	IEEE 802.11ax (BOMM, MCS31, 90pc dc)	WLAN	8.61	± 0.6 %
107200	AAC	IEEE 802.11ax (QOMM, MCS1, 90pc dc)	WLAN	8.67	± 0.6 %	107276	AAC	IEEE 802.11ax (BOMM, MCS31, 90pc dc)	WLAN	8.56	± 0.6 %
107201	AAC	IEEE 802.11ax (QOMM, MCS2, 90pc dc)	WLAN	8.78	± 0.6 %	107277	AAC	IEEE 802.11ax (BOMM, MCS31, 90pc dc)	WLAN	8.65	± 0.6 %
107202	AAC	IEEE 802.11ax (QOMM, MCS3, 90pc dc)	WLAN	8.55	± 0.6 %	107278	AAC	IEEE 802.11ax (BOMM, MCS31, 90pc dc)	WLAN	8.64	± 0.6 %
107203	AAC	IEEE 802.11ax (QOMM, MCS4, 90pc dc)	WLAN	8.79	± 0.6 %	107279	AAC	IEEE 802.11ax (BOMM, MCS31, 90pc dc)	WLAN	8.65	± 0.6 %
107204	AAC	IEEE 802.11ax (QOMM, MCS5, 90pc dc)	WLAN	8.90	± 0.6 %	107280	AAC	IEEE 802.11ax (BOMM, MCS31, 90pc dc)	WLAN	8.65	± 0.6 %
107205	AAC	IEEE 802.11ax (QOMM, MCS6, 90pc dc)	WLAN	8.74	± 0.6 %	107281	AAC	IEEE 802.11ax (BOMM, MCS31, 90pc dc)	WLAN	8.67	± 0.6 %
107206	AAC	IEEE 802.11ax (QOMM, MCS7, 90pc dc)	WLAN	8.72	± 0.6 %	107282	AAC	IEEE 802.11ax (BOMM, MCS31, 90pc dc)	WLAN	8.63	± 0.6 %
107207	AAC	IEEE 802.11ax (QOMM, MCS8, 90pc dc)	WLAN	8.66	± 0.6 %	107283	AAC	IEEE 802.11ax (BOMM, MCS31, 90pc dc)	WLAN	8.37	± 0.6 %
107208	AAC	IEEE 802.11ax (QOMM, MCS9, 90pc dc)	WLAN	8.65	± 0.6 %	107284	AAC	IEEE 802.11ax (BOMM, MCS31, 90pc dc)	WLAN	8.25	± 0.6 %

Certificate No: E3X-7346_Mar22
Page 19 of 24

Certificate No: E3X-7346_Mar22
Page 20 of 24



Unless otherwise agreed in writing this document is issued by the Company subject to its General Conditions of Service printed overleaf, available on request or accessible at <http://www.sgs.com/en/Terms-and-Conditions.aspx> and, for electronic format documents, subject to Terms and Conditions for Electronic Documents at <http://www.sgs.com/en/Terms-and-Conditions/Terms-e-Documents.aspx>. Attention is drawn to the limitation of liability, indemnification and jurisdiction issues defined therein. Any holder of this document is aware that the information contained herein reflects the Company's findings at the time of its intervention only and within the limits of its client's instructions. The Company's responsibility is limited to the performance of its services and does not extend to any transaction from exercising all their rights and obligations under the transaction documents. This document cannot be reproduced except in full, without prior written approval of the Company. Any unauthorized alteration, forgery or falsification of the content or appearance of this document is unlawful and may be prosecuted to the fullest extent of the law. If the document was otherwise stated the Company's consent is given for the reproduction of the sample for the purpose of the sample for 30 days only.

Attention: To check the authenticity of testing /inspection report
or email: CN.Doccheck@sgs.com
No.10, Weiye Road, Innovation Park, Kunshan, Jiangsu, China 215300
中国·江苏·昆山市留学院创业园伟业路10号 邮编 215300

t(86-512)57355888 f(86-512)57370818 www.sgsgroup.com.cn
t(86-512)57355888 f(86-512)57370818 sqs.china@sqs.com

EX3DV4 – SN7346

March 30, 2022

10985	AAA	SG NR DL (CP-OPDM, TN3 3.1, 40 MHz, 64-QAM, 30 MHz)	SG NR FR1 TDD 9.54 ± 9.6 %
10986	AAA	SG NR DL (CP-OPDM, TN3 3.1, 30 MHz, 64-QAM, 30 MHz)	SG NR FR1 TDD 9.50 ± 9.6 %
10987	AAA	SG NR DL (CP-OPDM, TN3 3.1, 30 MHz, 64-QAM, 30 MHz)	SG NR FR1 TDD 9.53 ± 9.6 %
10988	AAA	SG NR DL (CP-OPDM, TN3 3.1, 70 MHz, 64-QAM, 30 MHz)	SG NR FR1 TDD 9.56 ± 9.6 %
10989	AAA	SG NR DL (CP-OPDM, TN3 3.1, 80 MHz, 64-QAM, 30 MHz)	SG NR FR1 TDD 9.53 ± 9.6 %
10990	AAA	SG NR DL (CP-OPDM, TN3 3.1, 90 MHz, 64-QAM, 30 MHz)	SG NR FR1 TDD 9.50 ± 9.6 %

† Uncertainty is determined using the max. deviation from linear response applying rectangular distribution and is expressed for the square of the field value.

EX3DV4 – SN7346

March 30, 2022

10991	AAB	SG NR CP (CP-OPDM, TN3 3.1, 40 MHz, 64-QAM, 30 MHz)	SG NR FR1 TDD 9.54 ± 9.6 %
10992	AAB	SG NR CP (CP-OPDM, TN3 3.1, 30 MHz, 64-QAM, 30 MHz)	SG NR FR1 TDD 9.50 ± 9.6 %
10993	AAB	SG NR CP (CP-OPDM, TN3 3.1, 30 MHz, 64-QAM, 30 MHz)	SG NR FR1 TDD 9.53 ± 9.6 %
10994	AAB	SG NR CP (CP-OPDM, TN3 3.1, 70 MHz, 64-QAM, 30 MHz)	SG NR FR1 TDD 9.56 ± 9.6 %
10995	AAB	SG NR CP (CP-OPDM, TN3 3.1, 80 MHz, 64-QAM, 30 MHz)	SG NR FR1 TDD 9.53 ± 9.6 %
10996	AAB	SG NR CP (CP-OPDM, TN3 3.1, 90 MHz, 64-QAM, 30 MHz)	SG NR FR1 TDD 9.50 ± 9.6 %
10997	AAC	SG NR CP (CP-OPDM, TN3 3.1, 40 MHz, 64-QAM, 30 MHz)	SG NR FR1 TDD 9.54 ± 9.6 %
10998	AAC	SG NR CP (CP-OPDM, TN3 3.1, 30 MHz, 64-QAM, 30 MHz)	SG NR FR1 TDD 9.50 ± 9.6 %
10999	AAC	SG NR CP (CP-OPDM, TN3 3.1, 30 MHz, 64-QAM, 30 MHz)	SG NR FR1 TDD 9.53 ± 9.6 %
11000	AAC	SG NR CP (CP-OPDM, TN3 3.1, 70 MHz, 64-QAM, 30 MHz)	SG NR FR1 TDD 9.56 ± 9.6 %
11001	AAC	SG NR CP (CP-OPDM, TN3 3.1, 80 MHz, 64-QAM, 30 MHz)	SG NR FR1 TDD 9.53 ± 9.6 %
11002	AAC	SG NR CP (CP-OPDM, TN3 3.1, 90 MHz, 64-QAM, 30 MHz)	SG NR FR1 TDD 9.50 ± 9.6 %
11003	AAD	SG NR CP (CP-OPDM, TN3 3.1, 40 MHz, 64-QAM, 30 MHz)	SG NR FR1 TDD 9.54 ± 9.6 %
11004	AAD	SG NR CP (CP-OPDM, TN3 3.1, 30 MHz, 64-QAM, 30 MHz)	SG NR FR1 TDD 9.50 ± 9.6 %
11005	AAD	SG NR CP (CP-OPDM, TN3 3.1, 30 MHz, 64-QAM, 30 MHz)	SG NR FR1 TDD 9.53 ± 9.6 %
11006	AAD	SG NR CP (CP-OPDM, TN3 3.1, 70 MHz, 64-QAM, 30 MHz)	SG NR FR1 TDD 9.56 ± 9.6 %
11007	AAD	SG NR CP (CP-OPDM, TN3 3.1, 80 MHz, 64-QAM, 30 MHz)	SG NR FR1 TDD 9.53 ± 9.6 %
11008	AAD	SG NR CP (CP-OPDM, TN3 3.1, 90 MHz, 64-QAM, 30 MHz)	SG NR FR1 TDD 9.50 ± 9.6 %
11009	AAD	SG NR CP (CP-OPDM, TN3 3.1, 40 MHz, 64-QAM, 30 MHz)	SG NR FR1 TDD 9.54 ± 9.6 %
11010	AAD	SG NR CP (CP-OPDM, TN3 3.1, 30 MHz, 64-QAM, 30 MHz)	SG NR FR1 TDD 9.50 ± 9.6 %
11011	AAD	SG NR CP (CP-OPDM, TN3 3.1, 30 MHz, 64-QAM, 30 MHz)	SG NR FR1 TDD 9.53 ± 9.6 %
11012	AAD	SG NR CP (CP-OPDM, TN3 3.1, 70 MHz, 64-QAM, 30 MHz)	SG NR FR1 TDD 9.56 ± 9.6 %
11013	AAD	SG NR CP (CP-OPDM, TN3 3.1, 80 MHz, 64-QAM, 30 MHz)	SG NR FR1 TDD 9.53 ± 9.6 %
11014	AAD	SG NR CP (CP-OPDM, TN3 3.1, 90 MHz, 64-QAM, 30 MHz)	SG NR FR1 TDD 9.50 ± 9.6 %
11015	AAD	SG NR CP (CP-OPDM, TN3 3.1, 40 MHz, 64-QAM, 30 MHz)	SG NR FR1 TDD 9.54 ± 9.6 %
11016	AAD	SG NR CP (CP-OPDM, TN3 3.1, 30 MHz, 64-QAM, 30 MHz)	SG NR FR1 TDD 9.50 ± 9.6 %
11017	AAD	SG NR CP (CP-OPDM, TN3 3.1, 30 MHz, 64-QAM, 30 MHz)	SG NR FR1 TDD 9.53 ± 9.6 %
11018	AAD	SG NR CP (CP-OPDM, TN3 3.1, 70 MHz, 64-QAM, 30 MHz)	SG NR FR1 TDD 9.56 ± 9.6 %
11019	AAD	SG NR CP (CP-OPDM, TN3 3.1, 80 MHz, 64-QAM, 30 MHz)	SG NR FR1 TDD 9.53 ± 9.6 %
11020	AAD	SG NR CP (CP-OPDM, TN3 3.1, 90 MHz, 64-QAM, 30 MHz)	SG NR FR1 TDD 9.50 ± 9.6 %
11021	AAD	SG NR CP (CP-OPDM, TN3 3.1, 40 MHz, 64-QAM, 30 MHz)	SG NR FR1 TDD 9.54 ± 9.6 %
11022	AAD	SG NR CP (CP-OPDM, TN3 3.1, 30 MHz, 64-QAM, 30 MHz)	SG NR FR1 TDD 9.50 ± 9.6 %
11023	AAD	SG NR CP (CP-OPDM, TN3 3.1, 30 MHz, 64-QAM, 30 MHz)	SG NR FR1 TDD 9.53 ± 9.6 %
11024	AAD	SG NR CP (CP-OPDM, TN3 3.1, 70 MHz, 64-QAM, 30 MHz)	SG NR FR1 TDD 9.56 ± 9.6 %
11025	AAD	SG NR CP (CP-OPDM, TN3 3.1, 80 MHz, 64-QAM, 30 MHz)	SG NR FR1 TDD 9.53 ± 9.6 %
11026	AAD	SG NR CP (CP-OPDM, TN3 3.1, 90 MHz, 64-QAM, 30 MHz)	SG NR FR1 TDD 9.50 ± 9.6 %
11027	AAD	SG NR CP (CP-OPDM, TN3 3.1, 40 MHz, 64-QAM, 30 MHz)	SG NR FR1 TDD 9.54 ± 9.6 %
11028	AAD	SG NR CP (CP-OPDM, TN3 3.1, 30 MHz, 64-QAM, 30 MHz)	SG NR FR1 TDD 9.50 ± 9.6 %
11029	AAD	SG NR CP (CP-OPDM, TN3 3.1, 30 MHz, 64-QAM, 30 MHz)	SG NR FR1 TDD 9.53 ± 9.6 %
11030	AAD	SG NR CP (CP-OPDM, TN3 3.1, 70 MHz, 64-QAM, 30 MHz)	SG NR FR1 TDD 9.56 ± 9.6 %
11031	AAD	SG NR CP (CP-OPDM, TN3 3.1, 80 MHz, 64-QAM, 30 MHz)	SG NR FR1 TDD 9.53 ± 9.6 %
11032	AAD	SG NR CP (CP-OPDM, TN3 3.1, 90 MHz, 64-QAM, 30 MHz)	SG NR FR1 TDD 9.50 ± 9.6 %
11033	AAD	SG NR CP (CP-OPDM, TN3 3.1, 40 MHz, 64-QAM, 30 MHz)	SG NR FR1 TDD 9.54 ± 9.6 %
11034	AAD	SG NR CP (CP-OPDM, TN3 3.1, 30 MHz, 64-QAM, 30 MHz)	SG NR FR1 TDD 9.50 ± 9.6 %
11035	AAD	SG NR CP (CP-OPDM, TN3 3.1, 30 MHz, 64-QAM, 30 MHz)	SG NR FR1 TDD 9.53 ± 9.6 %
11036	AAD	SG NR CP (CP-OPDM, TN3 3.1, 70 MHz, 64-QAM, 30 MHz)	SG NR FR1 TDD 9.56 ± 9.6 %
11037	AAD	SG NR CP (CP-OPDM, TN3 3.1, 80 MHz, 64-QAM, 30 MHz)	SG NR FR1 TDD 9.53 ± 9.6 %
11038	AAD	SG NR CP (CP-OPDM, TN3 3.1, 90 MHz, 64-QAM, 30 MHz)	SG NR FR1 TDD 9.50 ± 9.6 %
11039	AAD	SG NR CP (CP-OPDM, TN3 3.1, 40 MHz, 64-QAM, 30 MHz)	SG NR FR1 TDD 9.54 ± 9.6 %
11040	AAD	SG NR CP (CP-OPDM, TN3 3.1, 30 MHz, 64-QAM, 30 MHz)	SG NR FR1 TDD 9.50 ± 9.6 %
11041	AAD	SG NR CP (CP-OPDM, TN3 3.1, 30 MHz, 64-QAM, 30 MHz)	SG NR FR1 TDD 9.53 ± 9.6 %
11042	AAD	SG NR CP (CP-OPDM, TN3 3.1, 70 MHz, 64-QAM, 30 MHz)	SG NR FR1 TDD 9.56 ± 9.6 %
11043	AAD	SG NR CP (CP-OPDM, TN3 3.1, 80 MHz, 64-QAM, 30 MHz)	SG NR FR1 TDD 9.53 ± 9.6 %
11044	AAD	SG NR CP (CP-OPDM, TN3 3.1, 90 MHz, 64-QAM, 30 MHz)	SG NR FR1 TDD 9.50 ± 9.6 %
11045	AAD	SG NR CP (CP-OPDM, TN3 3.1, 40 MHz, 64-QAM, 30 MHz)	SG NR FR1 TDD 9.54 ± 9.6 %
11046	AAD	SG NR CP (CP-OPDM, TN3 3.1, 30 MHz, 64-QAM, 30 MHz)	SG NR FR1 TDD 9.50 ± 9.6 %
11047	AAD	SG NR CP (CP-OPDM, TN3 3.1, 30 MHz, 64-QAM, 30 MHz)	SG NR FR1 TDD 9.53 ± 9.6 %
11048	AAD	SG NR CP (CP-OPDM, TN3 3.1, 70 MHz, 64-QAM, 30 MHz)	SG NR FR1 TDD 9.56 ± 9.6 %
11049	AAD	SG NR CP (CP-OPDM, TN3 3.1, 80 MHz, 64-QAM, 30 MHz)	SG NR FR1 TDD 9.53 ± 9.6 %
11050	AAD	SG NR CP (CP-OPDM, TN3 3.1, 90 MHz, 64-QAM, 30 MHz)	SG NR FR1 TDD 9.50 ± 9.6 %
11051	AAD	SG NR CP (CP-OPDM, TN3 3.1, 40 MHz, 64-QAM, 30 MHz)	SG NR FR1 TDD 9.54 ± 9.6 %
11052	AAD	SG NR CP (CP-OPDM, TN3 3.1, 30 MHz, 64-QAM, 30 MHz)	SG NR FR1 TDD 9.50 ± 9.6 %
11053	AAD	SG NR CP (CP-OPDM, TN3 3.1, 30 MHz, 64-QAM, 30 MHz)	SG NR FR1 TDD 9.53 ± 9.6 %
11054	AAD	SG NR CP (CP-OPDM, TN3 3.1, 70 MHz, 64-QAM, 30 MHz)	SG NR FR1 TDD 9.56 ± 9.6 %
11055	AAD	SG NR CP (CP-OPDM, TN3 3.1, 80 MHz, 64-QAM, 30 MHz)	SG NR FR1 TDD 9.53 ± 9.6 %
11056	AAD	SG NR CP (CP-OPDM, TN3 3.1, 90 MHz, 64-QAM, 30 MHz)	SG NR FR1 TDD 9.50 ± 9.6 %
11057	AAD	SG NR CP (CP-OPDM, TN3 3.1, 40 MHz, 64-QAM, 30 MHz)	SG NR FR1 TDD 9.54 ± 9.6 %
11058	AAD	SG NR CP (CP-OPDM, TN3 3.1, 30 MHz, 64-QAM, 30 MHz)	SG NR FR1 TDD 9.50 ± 9.6 %
11059	AAD	SG NR CP (CP-OPDM, TN3 3.1, 30 MHz, 64-QAM, 30 MHz)	SG NR FR1 TDD 9.53 ± 9.6 %
11060	AAD	SG NR CP (CP-OPDM, TN3 3.1, 70 MHz, 64-QAM, 30 MHz)	SG NR FR1 TDD 9.56 ± 9.6 %
11061	AAD	SG NR CP (CP-OPDM, TN3 3.1, 80 MHz, 64-QAM, 30 MHz)	SG NR FR1 TDD 9.53 ± 9.6 %
11062	AAD	SG NR CP (CP-OPDM, TN3 3.1, 90 MHz, 64-QAM, 30 MHz)	SG NR FR1 TDD 9.50 ± 9.6 %
11063	AAD	SG NR CP (CP-OPDM, TN3 3.1, 40 MHz, 64-QAM, 30 MHz)	SG NR FR1 TDD 9.54 ± 9.6 %
11064	AAD	SG NR CP (CP-OPDM, TN3 3.1, 30 MHz, 64-QAM, 30 MHz)	SG NR FR1 TDD 9.50 ± 9.6 %
11065	AAD	SG NR CP (CP-OPDM, TN3 3.1, 30 MHz, 64-QAM, 30 MHz)	SG NR FR1 TDD 9.53 ± 9.6 %
11066	AAD	SG NR CP (CP-OPDM, TN3 3.1, 70 MHz, 64-QAM, 30 MHz)	SG NR FR1 TDD 9.56 ± 9.6 %
11067	AAD	SG NR CP (CP-OPDM, TN3 3.1, 80 MHz, 64-QAM, 30 MHz)	SG NR FR1 TDD 9.53 ± 9.6 %
11068	AAD	SG NR CP (CP-OPDM, TN3 3.1, 90 MHz, 64-QAM, 30 MHz)	SG NR FR1 TDD 9.50 ± 9.6 %
11069	AAD	SG NR CP (CP-OPDM, TN3 3.1, 40 MHz, 64-QAM, 30 MHz)	SG NR FR1 TDD 9.54 ± 9.6 %
11070	AAD	SG NR CP (CP-OPDM, TN3 3.1, 30 MHz, 64-QAM, 30 MHz)	SG NR FR1 TDD 9.50 ± 9.6 %
11071	AAD	SG NR CP (CP-OPDM, TN3 3.1, 30 MHz, 64-QAM, 30 MHz)	SG NR FR1 TDD 9.53 ± 9.6 %
11072	AAD	SG NR CP (CP-OPDM, TN3 3.1, 70 MHz, 64-QAM, 30 MHz)	SG NR FR1 TDD 9.56 ± 9.6 %
11073	AAD	SG NR CP (CP-OPDM, TN3 3.1, 80 MHz, 64-QAM, 30 MHz)	SG NR FR1 TDD 9.53 ± 9.6 %
11074	AAD	SG NR CP (CP-OPDM, TN3 3.1, 90 MHz, 64-QAM, 30 MHz)	SG NR FR1 TDD 9.50 ± 9.6 %
11075	AAD	SG NR CP (CP-OPDM, TN3 3.1, 40 MHz, 64-QAM, 30 MHz)	SG NR FR1 TDD 9.54 ± 9.6 %
11076	AAD	SG NR CP (CP-OPDM, TN3 3.1, 30 MHz, 64-QAM, 30 MHz)	SG NR FR1 TDD 9.50 ± 9.6 %
11077	AAD	SG NR CP (CP-OPDM, TN3 3.1, 30 MHz, 64-QAM, 30 MHz)	SG NR FR1 TDD 9.53 ± 9.6 %
11078	AAD	SG NR CP (CP-OPDM, TN3 3.1, 70 MHz, 64-QAM, 30 MHz)	SG NR FR1 TDD 9.56 ± 9.6 %
11079	AAD	SG NR CP (CP-OPDM, TN3 3.1, 80 MHz, 64-QAM, 30 MHz)	SG NR FR1 TDD 9.53 ± 9.6 %
11080	AAD	SG NR CP (CP-OPDM, TN3 3.1, 90 MHz, 64-QAM, 30 MHz)	SG NR FR1 TDD 9.50 ± 9.6 %
11081	AAD	SG NR CP (CP-OPDM, TN3 3.1, 40 MHz, 64-QAM, 30 MHz)	SG NR FR1 TDD 9.54 ± 9.6 %
11082	AAD	SG NR CP (CP-OPDM, TN3 3.1, 30 MHz, 64-QAM, 30 MHz)	SG NR FR1 TDD 9.50 ± 9.6 %
11083	AAD	SG NR CP (CP-OPDM, TN3 3.1, 30 MHz, 64-QAM, 30 MHz)	SG NR FR1 TDD 9.53 ± 9.6 %
11084	AAD	SG NR CP (CP-OPDM, TN3 3.1, 70 MHz, 64-QAM, 30 MHz)	SG NR FR1 TDD 9.56 ± 9.6 %
11085	AAD	SG NR CP (CP-OPDM, TN3 3.1, 80 MHz, 64-QAM, 30 MHz)	SG NR FR1 TDD 9.53 ± 9.6 %
11086	AAD	SG NR CP (CP-OPDM, TN3 3.1, 90 MHz, 64-QAM, 30 MHz)	SG NR FR1 TDD 9.50 ± 9.6 %
11087	AAD	SG NR CP (CP-OPDM, TN3 3.1, 40 MHz, 64-QAM, 30 MHz)	SG NR FR1 TDD 9.54 ± 9.6 %
11088	AAD	SG NR CP (CP-OPDM, TN3 3.1, 30 MHz, 64-QAM, 30 MHz)	SG NR FR1 TDD 9.50 ± 9.6 %
11089	AAD	SG NR CP (CP-OPDM, TN3 3.1, 30 MHz, 64-QAM, 30 MHz)	SG NR FR1 TDD 9.53 ± 9.6 %
11090	AAD	SG NR CP (CP-OPDM, TN3 3.1, 70 MHz, 64-QAM, 30 MHz)	SG NR FR1 TDD 9.56 ± 9.6 %
11091	AAD	SG NR CP (CP-OPDM, TN3 3.1, 80 MHz, 64-QAM, 30 MHz)	SG NR FR1 TDD 9.53 ± 9.6 %
11092	AAD	SG NR CP (CP-OPDM, TN3 3.1, 90 MHz, 64-QAM, 30 MHz)	SG NR FR1 TDD 9.50 ± 9.6 %
11093	AAD	SG NR CP (CP-OPDM, TN3 3.1, 40 MHz, 64-QAM, 30 MHz)	SG NR FR1 TDD 9.54 ± 9.6 %
11094	AAD	SG NR CP (CP-OPDM, TN3 3.1, 30 MHz, 64-QAM, 30 MHz)	SG NR FR1 TDD 9.50 ± 9.6 %
11095	AAD	SG NR CP (CP-OPDM, TN3 3.1, 30 MHz, 64-QAM, 30 MHz)	SG NR FR1 TDD 9.53 ± 9.6 %
11096	AAD	SG NR CP (CP-OPDM, TN3 3.1, 70 MHz, 64-QAM, 30 MHz)	SG NR FR1 TDD 9.56 ± 9.6 %
11097	AAD	SG NR CP (CP-OPDM, TN3 3.1, 80 MHz, 64-QAM, 30 MHz)	SG NR FR1 TDD 9.53 ± 9.6 %
11098	AAD	SG NR CP (CP-OPDM, TN3 3.1, 90 MHz, 64-QAM, 30 MHz)	SG NR FR1 TDD 9.50 ± 9.6 %
11099	AAD	SG NR CP (CP-OPDM, TN3 3.1, 40 MHz, 64-QAM, 30 MHz)	SG NR FR1 TDD 9.54 ± 9.6 %
11100	AAD	SG NR CP (CP-OPDM, TN3 3.1, 30 MHz, 64-QAM, 30 MHz)	SG NR FR1 TDD 9.50 ± 9.6 %
11101	AAD	SG NR CP (CP-OPDM, TN3 3.1, 30 MHz, 64-QAM, 30 MHz)	SG NR FR1 TDD 9.53 ± 9.6 %
11102	AAD	SG NR CP (CP-OPDM, TN3 3.1, 70 MHz, 64-QAM, 30 MHz)	SG NR FR1 TDD 9.56 ± 9.6 %
11103	AAD	SG NR CP (CP-OPDM, TN3 3.1, 80 MHz, 64-QAM, 30 MHz)	SG NR FR1 TDD 9.53 ± 9.6 %
11104	AAD	SG NR CP (CP-OPDM, TN3 3.1, 90 MHz, 64-QAM, 30 MHz)	SG NR FR1 TDD 9.50 ± 9.6 %
11105	AAD	SG NR CP (CP-OPDM, TN3 3.1, 40 MHz, 64-QAM, 30 MHz)	SG NR FR1 TDD 9.54 ± 9.6 %
11106	AAD	SG NR CP (CP-OPDM, TN3 3.1, 30 MHz, 64-QAM, 30 MHz)	SG NR FR1 TDD 9.50 ± 9.6 %
11107	AAD	SG NR CP (CP-OPDM, TN3 3.1, 30 MHz, 64-QAM, 30 MHz)	SG NR FR1 TDD 9.53 ± 9.6 %
11108	AAD	SG NR CP (CP-OPDM, TN3 3.1, 70 MHz, 64-QAM, 30 MHz)	SG NR FR1 TDD 9.56 ± 9.6 %
11109	AAD	SG NR CP (CP-OPDM, TN3 3.1, 80 MHz, 64-QAM, 30 MHz)	SG NR FR1 TDD 9.53 ± 9.6 %
11110	AAD	SG NR CP (CP-OPDM, TN3 3.1, 90 MHz, 64-QAM, 30 MHz)	SG NR FR1 TDD 9.50 ± 9.6 %
11111	AAD	SG NR CP (CP-OPDM, TN3 3.1, 40 MHz, 64-QAM, 30 MHz)	SG NR FR1 TDD 9.54 ± 9.6 %
11112	AAD	SG NR CP (CP-OPDM, TN3 3.1, 30 MHz, 64-QAM, 30 MHz)	SG NR FR1 TDD 9.50 ± 9.6 %
11113	AAD	SG NR CP (CP-OPDM, TN3 3.1, 30 MHz, 64-QAM, 30 MHz)	SG NR FR1 TDD 9.53 ± 9.6 %
11114	AAD	SG NR CP (CP-OPDM, TN3 3.1, 70 MHz, 64-QAM, 30 MHz)	SG NR FR1 TDD 9.56 ± 9.6 %
11115	AAD	SG NR CP (CP-OPDM, TN3 3.1, 80 MHz, 64-QAM, 30 MHz)	SG NR FR1 TDD 9.53 ± 9.6 %
11116	AAD	SG NR CP (CP-OPDM, TN3 3.1, 90 MHz, 64-QAM, 30 MHz)	SG NR FR1 TDD 9.50 ± 9.6 %
11117	AAD	SG NR CP (CP-OPDM, TN3 3.1, 40 MHz, 64-QAM, 30 MHz)	SG NR FR1 TDD 9.54 ± 9.6 %
11118	AAD	SG NR CP (CP-OPDM, TN3 3.1, 30 MHz, 64-QAM, 30 MHz)	SG NR FR1 TDD 9.50 ± 9.6 %
11119	AAD	SG NR CP (CP-OPDM, TN3 3.1, 30 MHz, 64-QAM, 30 MHz)	SG NR FR1 TDD 9.53 ± 9.6 %
11120	AAD	SG NR CP (CP-OPDM, TN3 3.1, 70 MHz, 64-QAM, 30 MHz)	SG NR FR1 TDD 9.56 ± 9.6 %
11121	AAD	SG NR CP (CP-OPDM, TN3 3.1, 80 MHz, 64-QAM, 30 MHz)	SG NR FR1 TDD 9.53 ± 9.6 %
11122	AAD	SG NR CP (CP-OPDM, TN3 3.1, 90 MHz, 64-QAM, 30 MHz)	SG NR FR1 TDD 9.50 ± 9.6 %
11123	AAD	SG NR CP (CP-OPDM, TN3 3.1, 40 MHz, 64-QAM, 30 MHz)	SG NR FR1 TDD 9.54 ± 9.6 %
11124	AAD	SG NR CP (CP-OPDM, TN3 3.1, 30 MHz, 64-QAM, 30 MHz)	SG NR FR1 TDD 9.50 ± 9.6 %
11125	AAD	SG NR CP (CP-OPDM, TN3 3.1, 30 MHz, 64-QAM, 30 MHz)	SG NR FR1 TDD 9.53 ± 9.6 %
11126	AAD	SG NR CP (CP-OPDM, TN3 3.1, 70 MHz, 64-QAM, 30 MHz)	SG NR FR1 TDD 9.56 ± 9.6 %
11127	AAD	SG NR CP (CP-OPDM, TN3 3.1, 80 MHz, 64-QAM, 30 MHz)	SG NR FR1 TDD 9.53 ± 9.6 %
11128	AAD	SG NR CP (CP-OPDM, TN3 3.1, 90 MHz, 64-QAM, 30 MHz)	SG NR FR1 TDD 9.50 ± 9.6 %
11129	AAD	SG NR CP (CP-OPDM, TN3 3.1, 40 MHz, 64-QAM, 30 MHz)	SG NR FR1 TDD 9.54 ± 9.6 %
11130	AAD	SG NR CP (CP-OPDM, TN3 3.1, 30 MHz, 64-QAM, 30 MHz)	SG NR FR1 TDD 9.50 ± 9.6 %
11131	AAD	SG NR CP (CP-OPDM, TN3 3.1, 30 MHz, 64-QAM, 30 MHz)	SG NR FR1 TDD 9.53 ± 9.6 %
11132	AAD	SG NR CP (CP-OPDM, TN3 3.1, 70 MHz, 64-QAM, 30 MHz)	SG NR FR1 TDD 9.56 ± 9.6 %
11133	AAD	SG NR CP (CP-OPDM, TN3 3.1, 80 MHz, 64-QAM, 30 MHz)	SG NR FR1 TDD 9.53 ± 9.6 %
11134	AAD	SG NR CP (CP-OPDM, TN3 3.1, 90 MHz, 64-QAM, 30 MHz)	SG NR FR1 TDD 9.50 ± 9.6 %
11135	AAD	SG NR CP (CP-OPDM, TN3 3.1, 40 MHz, 64-QAM, 30 MHz)	SG NR FR1 TDD 9.54 ± 9.6 %
11136			

4 Impedance and return loss

Dipole CLA150 SN 4025				
Head Liquid				
Date of Measurement	Return Loss(dB)	Δ %	Impedance (Ω)	$\Delta\Omega$
2021/4/26	-31.4	/	47.8	/
Dipole D450V3 SN 1103				
Head Liquid				
Date of Measurement	Return Loss(dB)	Δ %	Impedance (Ω)	$\Delta\Omega$
2021/4/21	-23	/	57.1	/



Unless otherwise agreed in writing, this document is issued by the Company subject to its General Conditions of Service printed overleaf, available on request or accessible at <http://www.sgs.com/en/Terms-and-Conditions.aspx> and, for electronic format documents, subject to Terms and Conditions for Electronic Documents at <http://www.sgs.com/en/Terms-and-Conditions/Terms-e-Documents.aspx>. Attention is drawn to the limitation of liability, indemnification and jurisdiction issues defined therein. Any holder of this document is deemed to have read, understood and accepted the Terms and Conditions of the document and to have agreed to follow the Client's instructions, if any. The Company's sole responsibility is to its Client and this document does not exonerate parties to a transaction from exercising all their rights and obligations under the transaction documents. This document cannot be reproduced except in full, without prior written approval of the Company. Any unauthorized alteration, forgery or falsification of the content or expiration date of this document will render it void and null and any such use will be prosecuted to the fullest extent of the law. The results shown in this test report refer only to the sample(s) tested and such sample(s) are retained for 30 days only.

Results shown in this test report refer only to the sample(s) tested and such sample(s) are retained for 30 days only.
Attention: To check the authenticity of testing/inspection report & certificate, please contact us at telephone: (86-755) 8307 1443,
or email: CN.Doccheck@sgs.com
No.10, Weijue Road, Innovation Park, Kunshan, Jiangsu, China 215300 t(86-512)6735888 f(86-512)67370818 www.sgs.com
中国·江苏·昆山市留学生创业园佳业路10号 邮编 215300 t(86-512)6735888 f(86-512)67370818 sgs.china@sgs.com