

## SAR PROBE CALIBRATION (ET3DV6, SN 1679)

**Model No. : SH-03B**

**FCC ID : APYHRO00113**

The following procedures are recommended for DUT measurements at 150 MHz to 3 GHz to minimize probe calibration and tissue dielectric parameter discrepancies.

a) In general, DUT SAR measurements below 300 MHz should be within +/- 50 MHz of the probe calibration frequency.

SEE ALSO ITEM c).

b) At 300 MHz to 3 GHz, DUT measurements should be within +/- 100 MHz of the probe calibration frequency.

SEE ALSO ITEM c).

c) Measurements exceeding 50 % of these intervals, I.E.,

+/- 25 MHz, DUT  $f < 300$  MHz, OR

+/- 50 MHz, DUT  $f \geq 300$  MHz,

**SHALL APPLY THE FOLLOWING additional steps:**

1) When the actual tissue dielectric parameters used for probe calibration are available (careful about some probe manuf. list only nominal or range on calib. cert.), the differences for relative permittivity and conductivity between probe calibration and routine measurements should each be less than or equal to 5 % while also satisfying the required +/- 5 % tolerances in target dielectric parameters.

<Head 900 MHz>

The test frequencies are properly matched as this is a cellular band. The probe calibration for permittivity and conductivity is within +/-5%, were the probe calibrated centre frequency at **900MHz** has permittivity and conductivity of **41.5** and **0.97** respectively. At the probe extreme frequencies the following are true: at 800 MHz the permittivity and conductivity are 39.4 and 0.86 respectively. At 1000 MHz the permittivity and conductivity are 43.6 and 1.03 respectively.

The probe was calibrated at these parameters in order to cover the frequency range 800 MHz to 1000 MHz.

The screenshot shows a 'Conversion' dialog box with the following fields and values:

Parameter	X	Y	Z
Name:	900 (Head)		
Conversion factor:	6.29	6.29	6.29
Alpha:	0.38	0.38	0.38
Delta:	2.35	2.35	2.35
Frequency range:	800	to	1000 MHz
Permittivity range:	39.4	to	43.6
Conductivity range:	0.86	to	1.03 S/m
Calibrated for:	900	MHz	
Calibrated for:	41.5		
Calibrated for:	0.97	S/m	

Buttons: OK, Cancel

## <Body 900 MHz>

The test frequencies are properly matched as this is a cellular band. The probe calibration for permittivity and conductivity is within +/-5%, were the probe calibrated centre frequency at **900MHz** has permittivity and conductivity of **55.0** and **1.05** respectively. At the probe extreme frequencies the following are true: at 800 MHz the permittivity and conductivity are 52.3 and 0.92 respectively. At 1000 MHz the permittivity and conductivity are 57.8 and 1.10 respectively.

The probe was calibrated at these parameters in order to cover the frequency range 800 MHz to 1000 MHz.

The screenshot shows a 'Conversion' dialog box with the following fields and values:

Parameter	X	Y	Z
Name:	900 (Body)		
Conversion factor:	6.22	6.22	6.22
Alpha:	0.3	0.3	0.3
Delta:	2.97	2.97	2.97
Frequency range:	800	to	1000 MHz
Permittivity range:	52.3	to	57.8
Conductivity range:	0.92	to	1.1 S/m
Calibrated for:	900		MHz
Calibrated for:	55		
Calibrated for:	1.05		S/m

Buttons: OK, Cancel

## <Head 1810 MHz>

The test frequencies are properly matched as this is a cellular band. The probe calibration for permittivity and conductivity is within +/-5%, were the probe calibrated centre frequency at **1810MHz** has permittivity and conductivity of **40.0** and **1.40** respectively. At the probe extreme frequencies the following are true: at 1710 MHz the permittivity and conductivity are 38.0 and 1.29 respectively. At 1910 MHz the permittivity and conductivity are 42.0 and 1.47 respectively.

The probe was calibrated at these parameters in order to cover the frequency range 1710 MHz to 1910 MHz.

The screenshot shows a 'Conversion' dialog box with the following fields and values:

Parameter	X	Y	Z
Name	1810 (Head)		
Conversion factor	5.31	5.31	5.31
Alpha	0.57	0.57	0.57
Delta	2.41	2.41	2.41
Frequency range	1710	to	1910
Permittivity range	38	to	42
Conductivity range	1.29	to	1.47
Calibrated for	1810	MHz	
Calibrated for	40		
Calibrated for	1.4	S/m	

Buttons: OK, Cancel

## <Body 1810 MHz>

The test frequencies are properly matched as this is a cellular band. The probe calibration for permittivity and conductivity is within +/-5%, were the probe calibrated centre frequency at **1810MHz** has permittivity and conductivity of **53.3** and **1.52** respectively. At the probe extreme frequencies the following are true: at 1710 MHz the permittivity and conductivity are 50.6 and 1.38 respectively. At 1910 MHz the permittivity and conductivity are 56.0 and 1.60 respectively.

The probe was calibrated at these parameters in order to cover the frequency range 1710 MHz to 1910 MHz.

	X:	Y:	Z:	
Name:	1810 (Body)			OK
Conversion factor:	4.86	4.86	4.86	Cancel
Alpha:	0.6	0.6	0.6	
Delta:	2.4	2.4	2.4	
Frequency range:	1710	to	1910	MHz
Calibrated for:	1810			MHz
Permittivity range:	50.6	to	56	
Calibrated for:	53.3			
Conductivity range:	1.38	to	1.6	S/m
Calibrated for:	1.52			S/m

The target permittivity and conductivity at 835 MHz is 41.5 and 0.90 and 1900 MHz is 40.0 and 1.40 respectively which is within the calibrated range of the probe parameter. The following parameters are declared in the probe calibration certificate.

f [MHz]	Validity [MHz] <sup>©</sup>	TSL	Permittivity	Conductivity	Alpha	Depth	ConvF Uncertainty
900	± 50 / ± 100	Head	41.5 ± 5%	0.97 ± 5%	0.38	2.35	6.29 ± 11.0% (k=2)
1450	± 50 / ± 100	Head	40.5 ± 5%	1.20 ± 5%	0.38	3.45	5.37 ± 11.0% (k=2)
1810	± 50 / ± 100	Head	40.0 ± 5%	1.40 ± 5%	0.57	2.41	5.31 ± 11.0% (k=2)
1950	± 50 / ± 100	Head	40.0 ± 5%	1.40 ± 5%	0.70	2.15	5.02 ± 11.0% (k=2)
2450	± 50 / ± 100	Head	39.2 ± 5%	1.80 ± 5%	0.99	1.65	4.64 ± 11.0% (k=2)
900	± 50 / ± 100	Body	55.0 ± 5%	1.05 ± 5%	0.30	2.97	6.22 ± 11.0% (k=2)
1450	± 50 / ± 100	Body	54.0 ± 5%	1.30 ± 5%	0.52	2.54	5.07 ± 11.0% (k=2)
1810	± 50 / ± 100	Body	53.3 ± 5%	1.52 ± 5%	0.60	2.40	4.86 ± 11.0% (k=2)
1950	± 50 / ± 100	Body	53.3 ± 5%	1.52 ± 5%	0.70	2.30	4.76 ± 11.0% (k=2)
2450	± 50 / ± 100	Body	52.7 ± 5%	1.95 ± 5%	0.99	1.61	4.05 ± 11.0% (k=2)

<sup>©</sup> The validity of ± 100 MHz only applies for DASY v4.4 and higher (see Page 2). The uncertainty is the RSS of the ConvF uncertainty at calibration frequency and the uncertainty for the indicated frequency band.

2) When nominal tissue dielectric parameters are PROVIDED in the probe calibration data, the tissue dielectric parameters measured for routine measurements should be less than the target relative permittivity and higher than the target conductivity values, to minimize SAR underestimations. Otherwise, a thorough analysis of the effective frequency interval supported by the probe calibration and dielectric medium should be included in the SAR report to substantiate the test results – SEE ITEM d). Alternatively, the measured 1-g SAR may be compensated with respect to +5 % tolerances in relative permittivity and -5 % tolerances in conductivity, computed according to valid SAR sensitivity data, to reduce SAR underestimation and maintain conservativeness.

d) When thorough analysis is required for the additional steps, the following SHALL ALSO BE ADDRESSED.

These other items can contribute to additional SAR differences, especially when the probe calibration, tissue dielectric parameters and device test frequencies are misaligned.

1) The probe conversion factor and its frequency response, with respect to the tissue dielectric media used during probe calibration and routine measurements, should be examined to determine if the effective frequency interval is adequate for the intended measurements to satisfy protocol requirements.

2) Measurements within the required frequency interval should satisfy an expanded probe calibration uncertainty ( $k=2$ ) less than or equal to 15 % for all measurement conditions.

3) When SAR is reported within 10 % of the SAR limit, differences in field conditions and effects of output power levels on signal modulation between probe calibration and routine measurements should be examined to determine probe calibration validity.

4) Probe isotropy should also be assessed by rotating the probe in 15 degree increments at the peak SAR location of the zoom scan and accounted for in the measurement uncertainty.



The measured SAR values in the report are all below 10% of the SAR limit.

The measurement within the required frequency interval satisfy an expanded probe calibration uncertainty ( $k=2$ )  $\leq$  15% for all measurement conditions. Please refer to SAR report for probe and dipole calibration certificates produce by the system manufacturer.

As you can see we used the conductivity and permittivity parameters which are within +/- 5 % of the target values.



<WCDMA 850 MHz Head>

Liquid		Parameters	Target	Measured	Deviation [%]
Medium	Freq. [MHz]				
Head	825.0	Permittivity	41.6	42.28	+1.63
		Conductivity	0.90	0.884	-1.78
	835.0	Permittivity	41.5	42.18	+1.64
		Conductivity	0.90	0.893	-0.78
	845.0	Permittivity	41.5	42.10	+1.45
		Conductivity	0.91	0.902	-0.88

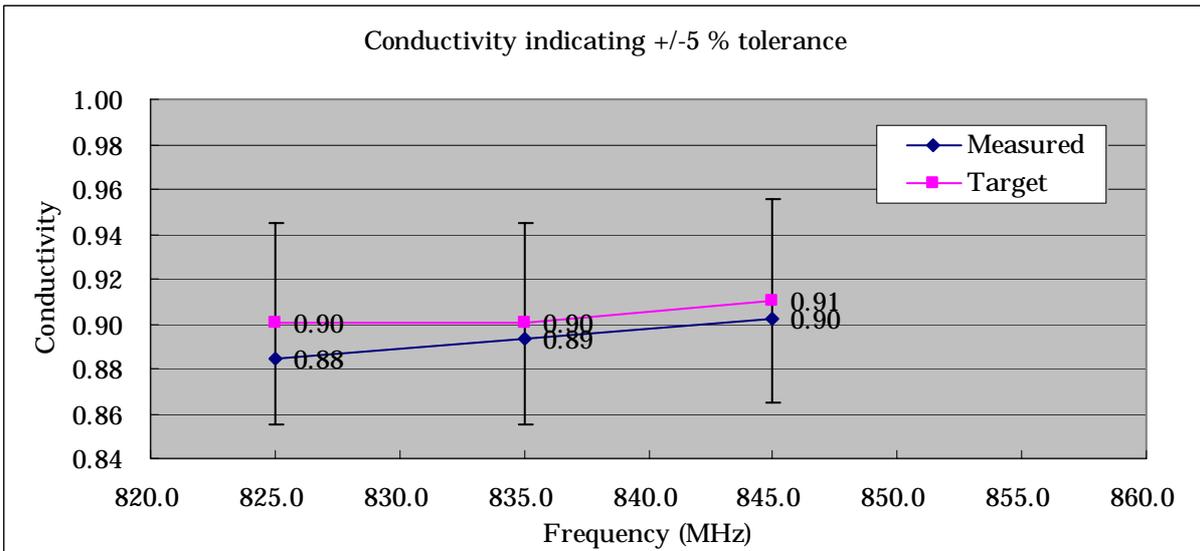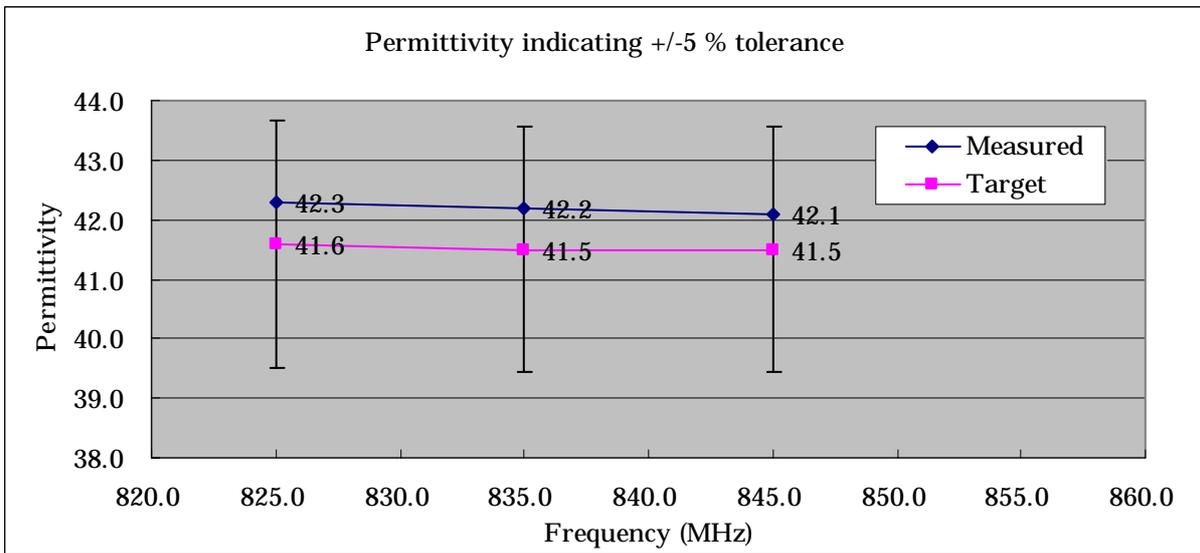



<WCDMA 850 MHz Body>

Liquid		Parameters	Target	Measured	Deviation [%]
Medium	Freq. [MHz]				
Body	825.0	Permittivity	55.2	54.49	-1.29
		Conductivity	0.97	0.931	-4.02
	835.0	Permittivity	55.2	54.39	-1.47
		Conductivity	0.97	0.941	-2.99
	845.0	Permittivity	55.2	54.28	-1.67
		Conductivity	0.98	0.952	-2.86

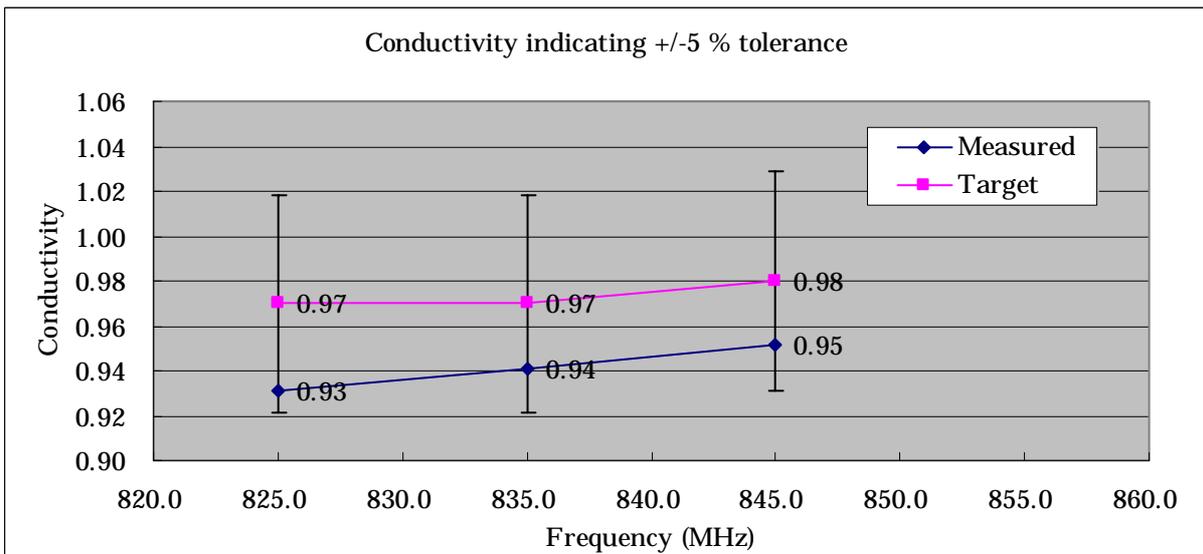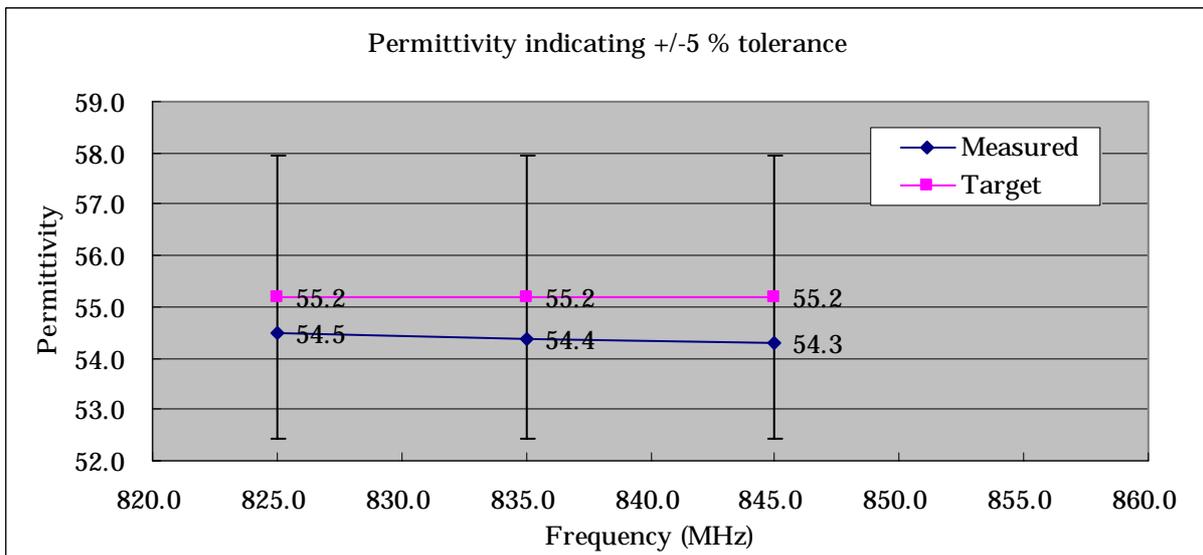

<PCS 1900 MHz Head>

Liquid		Parameters	Target	Measured	Deviation [%]
Medium	Freq. [MHz]				
Head	1850.0	Permittivity	40.0	39.72	-0.70
		Conductivity	1.40	1.364	-2.57
	1880.0	Permittivity	40.0	39.56	-1.10
		Conductivity	1.40	1.394	-0.43
	1910.0	Permittivity	40.0	39.45	-1.37
		Conductivity	1.40	1.427	+1.93

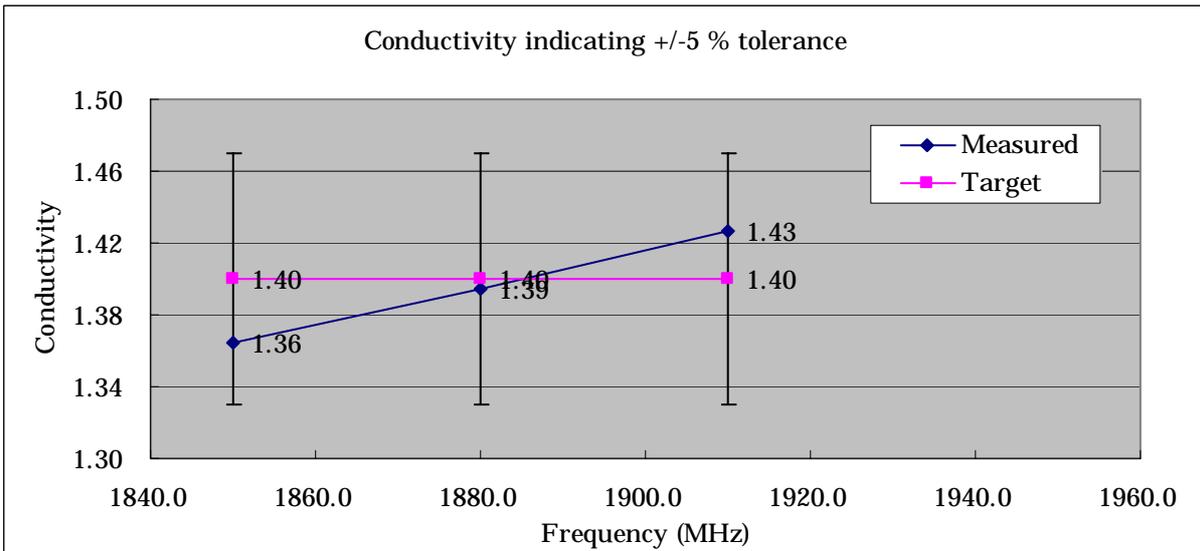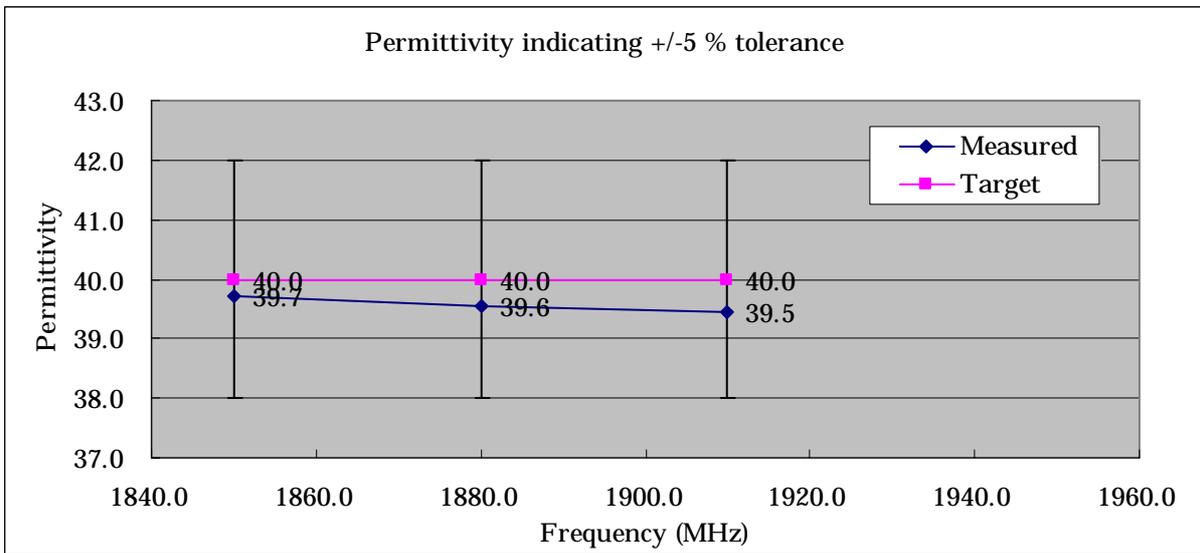

<PCS 1900 MHz Body>

Liquid		Parameters	Target	Measured	Deviation [%]
Medium	Freq. [MHz]				
Body	1850.0	Permittivity	53.3	52.57	-1.37
		Conductivity	1.52	1.512	-0.53
	1880.0	Permittivity	53.3	52.44	-1.61
		Conductivity	1.52	1.544	+1.58
	1910.0	Permittivity	53.3	52.31	-1.86
		Conductivity	1.52	1.580	+3.95

