



Attachment 1 – System Validation Plots

Test Laboratory: JAPAN QUALITY ASSURANCE ORGANIZATION

System Validation (Head 1900 MHz)

DUT: Dipole 1900 MHz; Type: D1900V2; Serial: 5d112

Communication System: CW; Frequency: 1900 MHz; Duty Cycle: 1:1

Medium: HSL1900 Medium parameters used: $f = 1900$ MHz; $\sigma = 1.42$ mho/m; $\epsilon_r = 40$; $\rho = 1000$ kg/m³

Phantom section: Flat Section

Measurement Standard: DAS4 (High Precision Assessment)

DASY4 Configuration:

- Probe: ET3DV6 - SN1679; ConvF(5.32, 5.32, 5.32); Calibrated: 2009/12/14
- Sensor-Surface: 4mm (Mechanical And Optical Surface Detection)
- Electronics: DAE3 Sn508; Calibrated: 2009/11/09
- Phantom: SAM 1200; Type: QD 000 P40 CA; Serial: 1200
- Measurement SW: DAS4, V4.7 Build 80; Postprocessing SW: SEMCAD, V1.8 Build 184

Antenna Input Power 250 mW/Area Scan (5x5x1): Measurement grid: dx=20mm, dy=20mm

Maximum value of SAR (measured) = 11.1 mW/g


Antenna Input Power 250 mW/Zoom Scan (5x5x7)/Cube 0: Measurement grid: dx=8mm, dy=8mm,

dz=5mm

Reference Value = 94.0 V/m; Power Drift = -0.009 dB

Peak SAR (extrapolated) = 16.8 W/kg

SAR(1 g) = 9.82 mW/g; SAR(10 g) = 5.12 mW/g

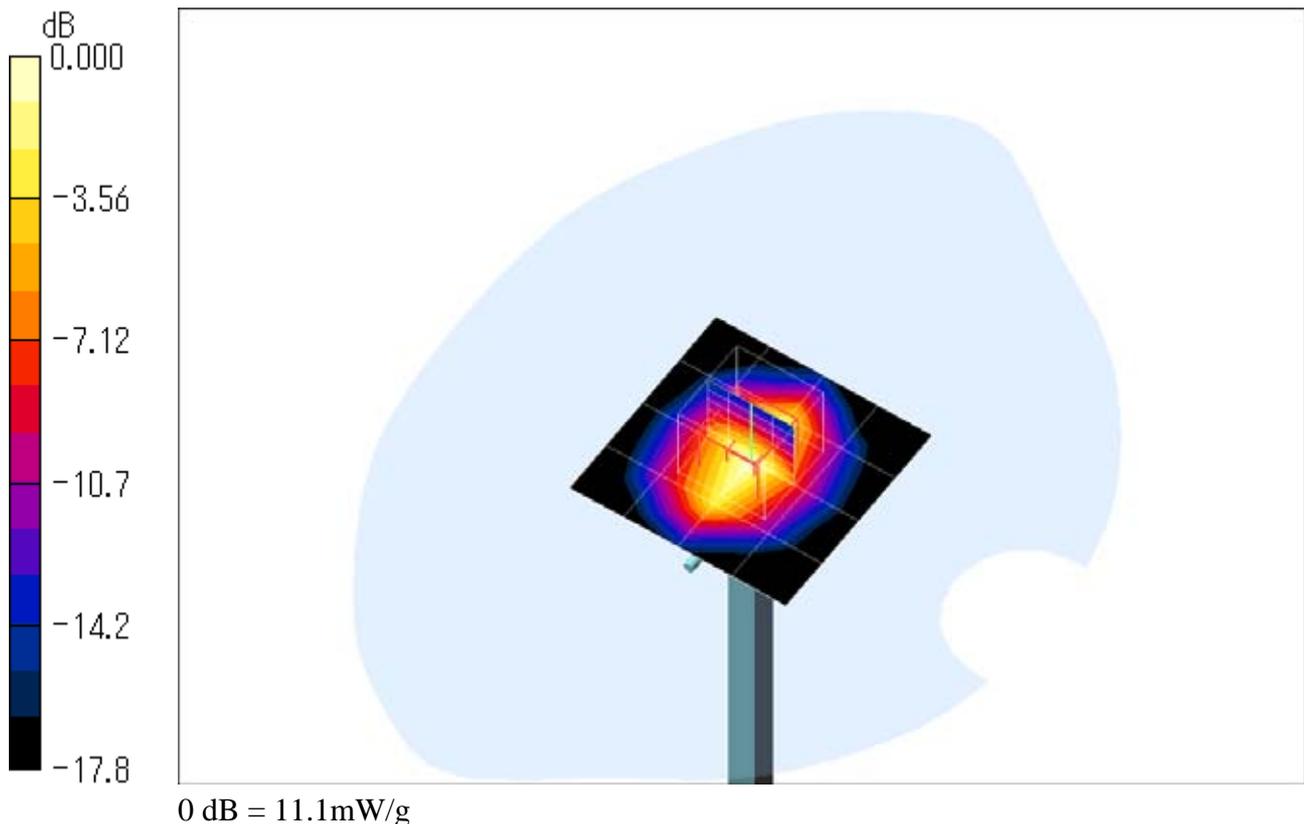

Test Laboratory: JAPAN QUALITY ASSURANCE ORGANIZATION

System Validation (Body 1900 MHz)

DUT: Dipole 1900 MHz; Type: D1900V2; Serial: 5d112

Communication System: CW; Frequency: 1900 MHz; Duty Cycle: 1:1

Medium: M1900 Medium parameters used: $f = 1900$ MHz; $\sigma = 1.58$ mho/m; $\epsilon_r = 52.7$; $\rho = 1000$ kg/m³

Phantom section: Flat Section

Measurement Standard: DASY4 (High Precision Assessment)

DASY4 Configuration:

- Probe: ET3DV6 - SN1679; ConvF(4.74, 4.74, 4.74); Calibrated: 2009/12/14
- Sensor-Surface: 4mm (Mechanical And Optical Surface Detection)
- Electronics: DAE3 Sn508; Calibrated: 2009/11/09
- Phantom: SAM 1200; Type: QD 000 P40 CA; Serial: 1200
- Measurement SW: DASY4, V4.7 Build 80; Postprocessing SW: SEMCAD, V1.8 Build 184

Antenna Input Power 250 mW/Area Scan (5x5x1): Measurement grid: dx=20mm, dy=20mm

Maximum value of SAR (measured) = 11.1 mW/g


Antenna Input Power 250 mW/Zoom Scan (5x5x7)/Cube 0: Measurement grid: dx=8mm, dy=8mm, dz=5mm

Reference Value = 92.5 V/m; Power Drift = 0.000 dB

Peak SAR (extrapolated) = 15.4 W/kg

SAR(1 g) = 9.79 mW/g; SAR(10 g) = 5.22 mW/g

Maximum value of SAR (measured) = 11.2 mW/g

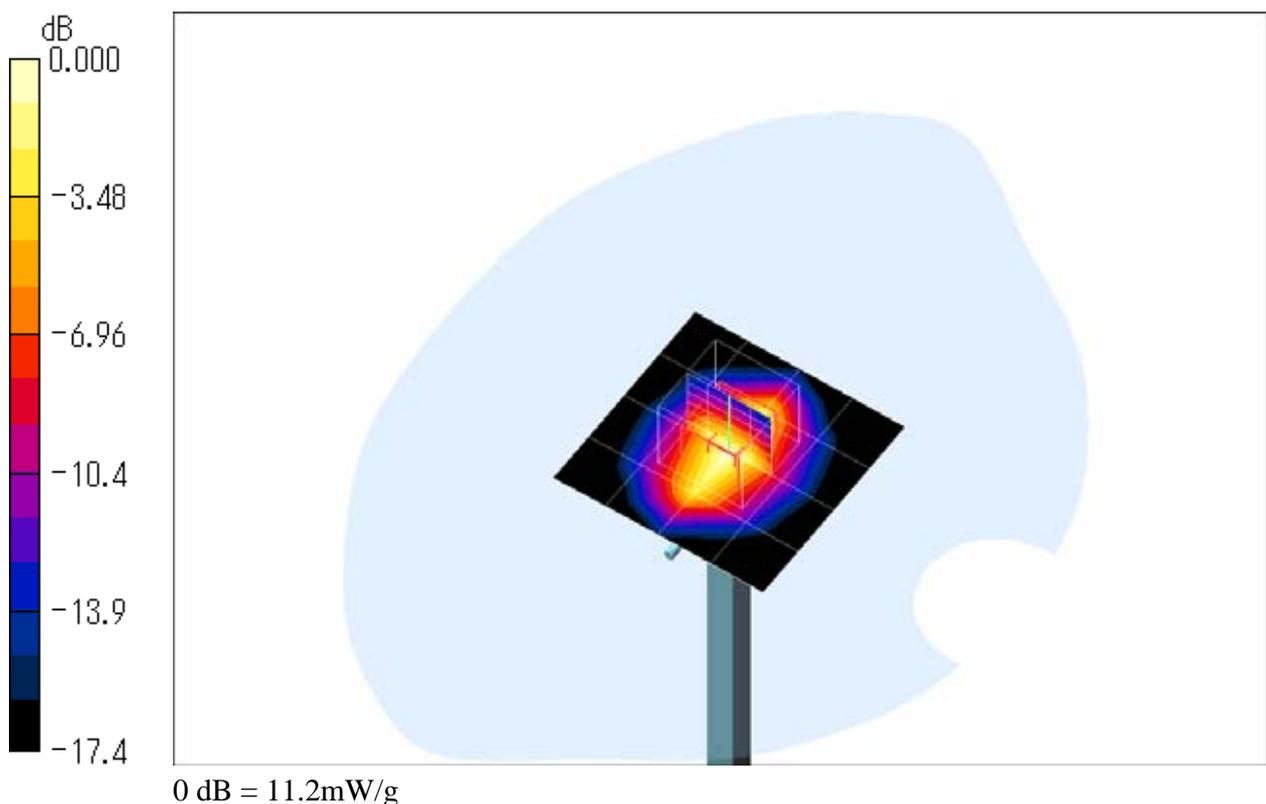



Attachment 2 – SAR Test Plots

Test Laboratory: JAPAN QUALITY ASSURANCE ORGANIZATION

Left Head, Cheek/Touch 512ch (1850.2MHz)

DUT: Cellular Phone; Type: 842SH; Serial: 004401/11/268181/8

Communication System: GSM 1900; Frequency: 1850.2 MHz; Duty Cycle: 1:8.3

Medium: HSL1900 Medium parameters used: $f = 1850.2 \text{ MHz}$; $\sigma = 1.37 \text{ mho/m}$; $\epsilon_r = 40.1$; $\rho = 1000 \text{ kg/m}^3$

Phantom section: Left Section

Measurement Standard: DASy4 (High Precision Assessment)

DASy4 Configuration:

- Probe: ET3DV6 - SN1679; ConvF(5.32, 5.32, 5.32); Calibrated: 2009/12/14
- Sensor-Surface: 4mm (Mechanical And Optical Surface Detection)
- Electronics: DAE3 Sn508; Calibrated: 2009/11/09
- Phantom: SAM 1200; Type: QD 000 P40 CA; Serial: 1200
- Measurement SW: DASy4, V4.7 Build 80; Postprocessing SW: SEMCAD, V1.8 Build 184

Cheek/Touch Position/Area Scan (11x6x1): Measurement grid: $dx=15\text{mm}$, $dy=15\text{mm}$


Maximum value of SAR (measured) = 0.343 mW/g

Cheek/Touch Position/Zoom Scan (5x5x7)/Cube 0: Measurement grid: $dx=8\text{mm}$, $dy=8\text{mm}$, $dz=5\text{mm}$

Reference Value = 12.9 V/m; Power Drift = -0.032 dB

Peak SAR (extrapolated) = 0.440 W/kg

SAR(1 g) = 0.317 mW/g; SAR(10 g) = 0.200 mW/g

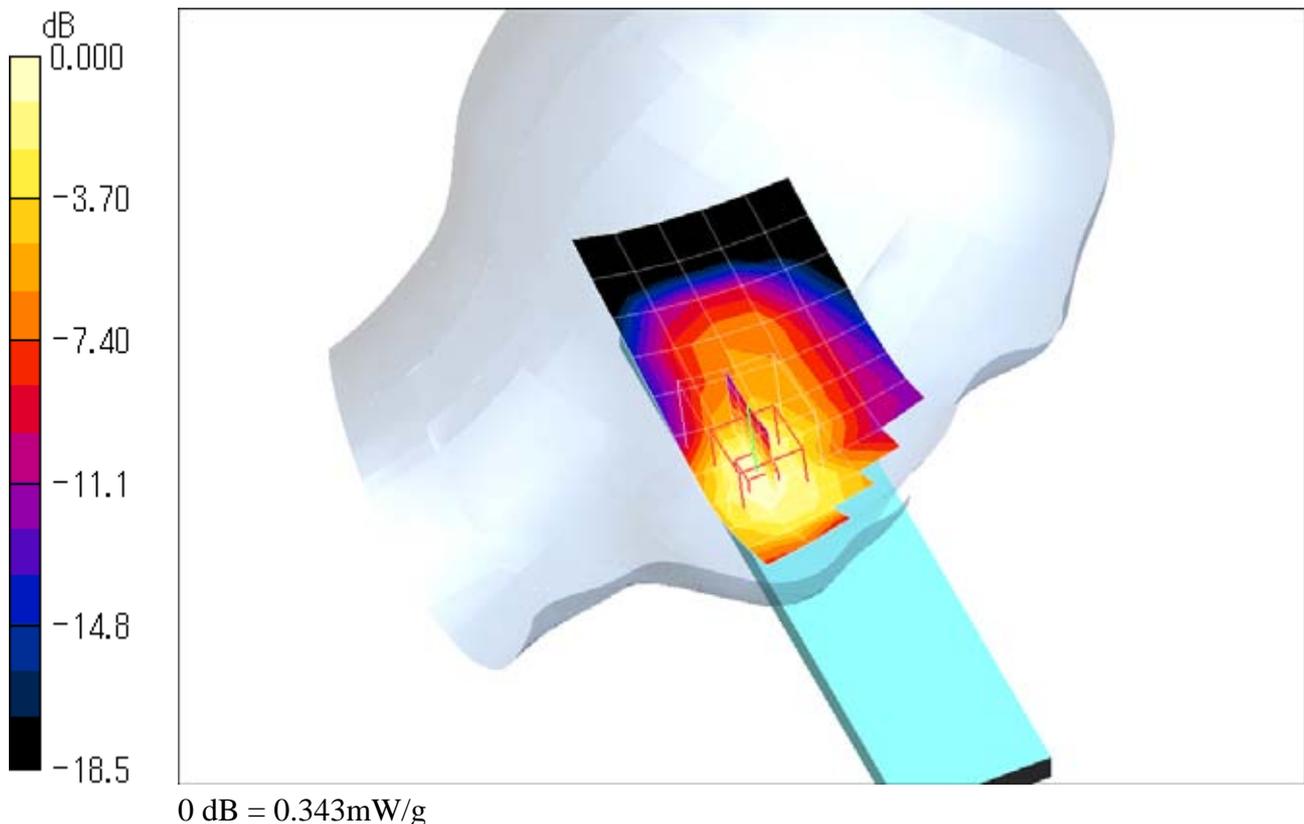

Test Laboratory: JAPAN QUALITY ASSURANCE ORGANIZATION

Left Head, Cheek/Touch 661ch (1880.0MHz)

DUT: Cellular Phone; Type: 842SH; Serial: 004401/11/268181/8

Communication System: GSM 1900; Frequency: 1880 MHz; Duty Cycle: 1:8.3

Medium: HSL1900 Medium parameters used: $f = 1880 \text{ MHz}$; $\sigma = 1.4 \text{ mho/m}$; $\epsilon_r = 39.9$; $\rho = 1000 \text{ kg/m}^3$

Phantom section: Left Section

Measurement Standard: DAS4 (High Precision Assessment)

DASY4 Configuration:

- Probe: ET3DV6 - SN1679; ConvF(5.32, 5.32, 5.32); Calibrated: 2009/12/14
- Sensor-Surface: 4mm (Mechanical And Optical Surface Detection)
- Electronics: DAE3 Sn508; Calibrated: 2009/11/09
- Phantom: SAM 1200; Type: QD 000 P40 CA; Serial: 1200
- Measurement SW: DAS4, V4.7 Build 80; Postprocessing SW: SEMCAD, V1.8 Build 184

Cheek/Touch Position/Area Scan (11x6x1): Measurement grid: $dx=15\text{mm}$, $dy=15\text{mm}$

Maximum value of SAR (measured) = 0.397 mW/g


Cheek/Touch Position/Zoom Scan (5x5x7)/Cube 0: Measurement grid: $dx=8\text{mm}$, $dy=8\text{mm}$, $dz=5\text{mm}$

Reference Value = 13.1 V/m; Power Drift = -0.086 dB

Peak SAR (extrapolated) = 0.517 W/kg

SAR(1 g) = 0.367 mW/g; SAR(10 g) = 0.228 mW/g

Maximum value of SAR (measured) = 0.394 mW/g

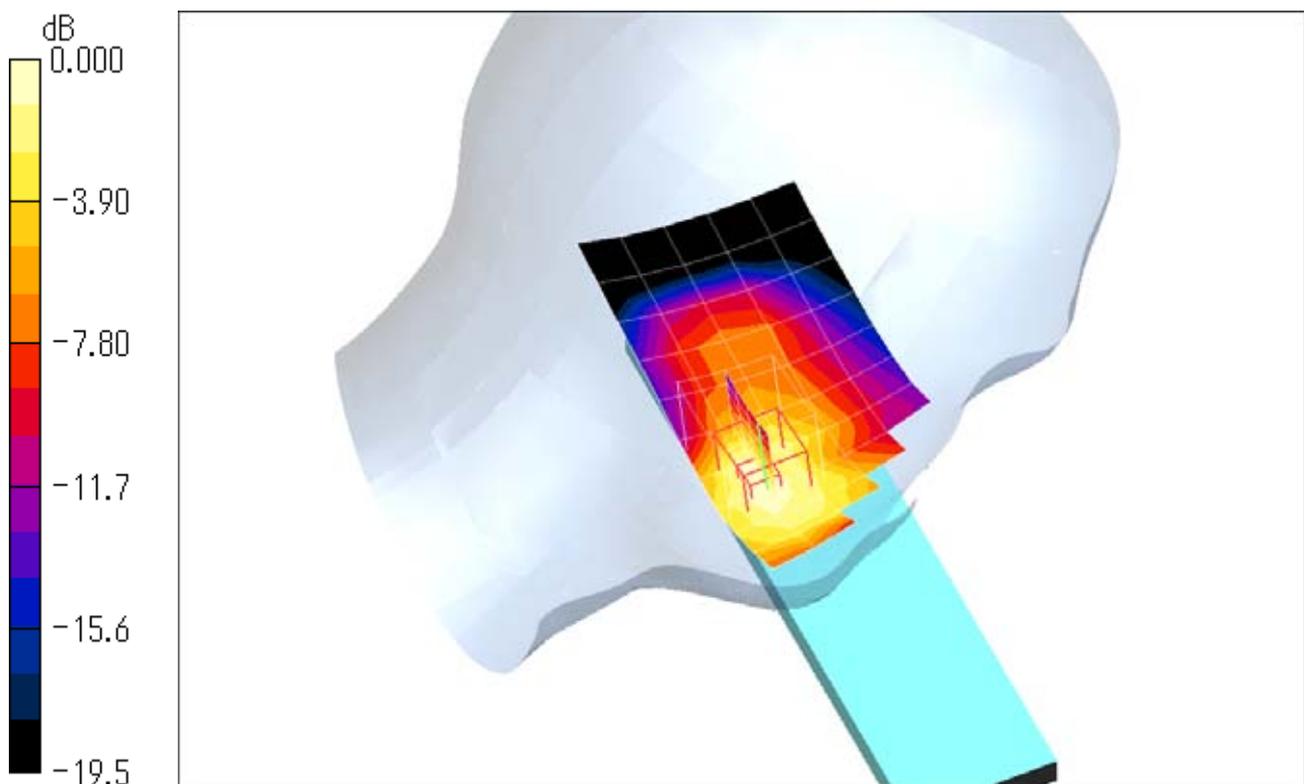

0 dB = 0.394mW/g

Test Laboratory: JAPAN QUALITY ASSURANCE ORGANIZATION

Left Head, Cheek/Touch 810ch (1909.8MHz)

DUT: Cellular Phone; Type: 842SH; Serial: 004401/11/268181/8

Communication System: GSM 1900; Frequency: 1909.8 MHz; Duty Cycle: 1:8.3

Medium: HSL1900 Medium parameters used: $f = 1909.8$ MHz; $\sigma = 1.43$ mho/m; $\epsilon_r = 39.8$; $\rho = 1000$ kg/m³

Phantom section: Left Section

Measurement Standard: DASY4 (High Precision Assessment)

DASY4 Configuration:

- Probe: ET3DV6 - SN1679; ConvF(5.32, 5.32, 5.32); Calibrated: 2009/12/14
- Sensor-Surface: 4mm (Mechanical And Optical Surface Detection)
- Electronics: DAE3 Sn508; Calibrated: 2009/11/09
- Phantom: SAM 1200; Type: QD 000 P40 CA; Serial: 1200
- Measurement SW: DASY4, V4.7 Build 80; Postprocessing SW: SEMCAD, V1.8 Build 184

Cheek/Touch Position/Area Scan (11x6x1): Measurement grid: dx=15mm, dy=15mm

Maximum value of SAR (measured) = 0.389 mW/g


Cheek/Touch Position/Zoom Scan (5x5x7)/Cube 0: Measurement grid: dx=8mm, dy=8mm, dz=5mm

Reference Value = 14.0 V/m; Power Drift = -0.007 dB

Peak SAR (extrapolated) = 0.530 W/kg

SAR(1 g) = 0.376 mW/g; SAR(10 g) = 0.235 mW/g

Maximum value of SAR (measured) = 0.412 mW/g

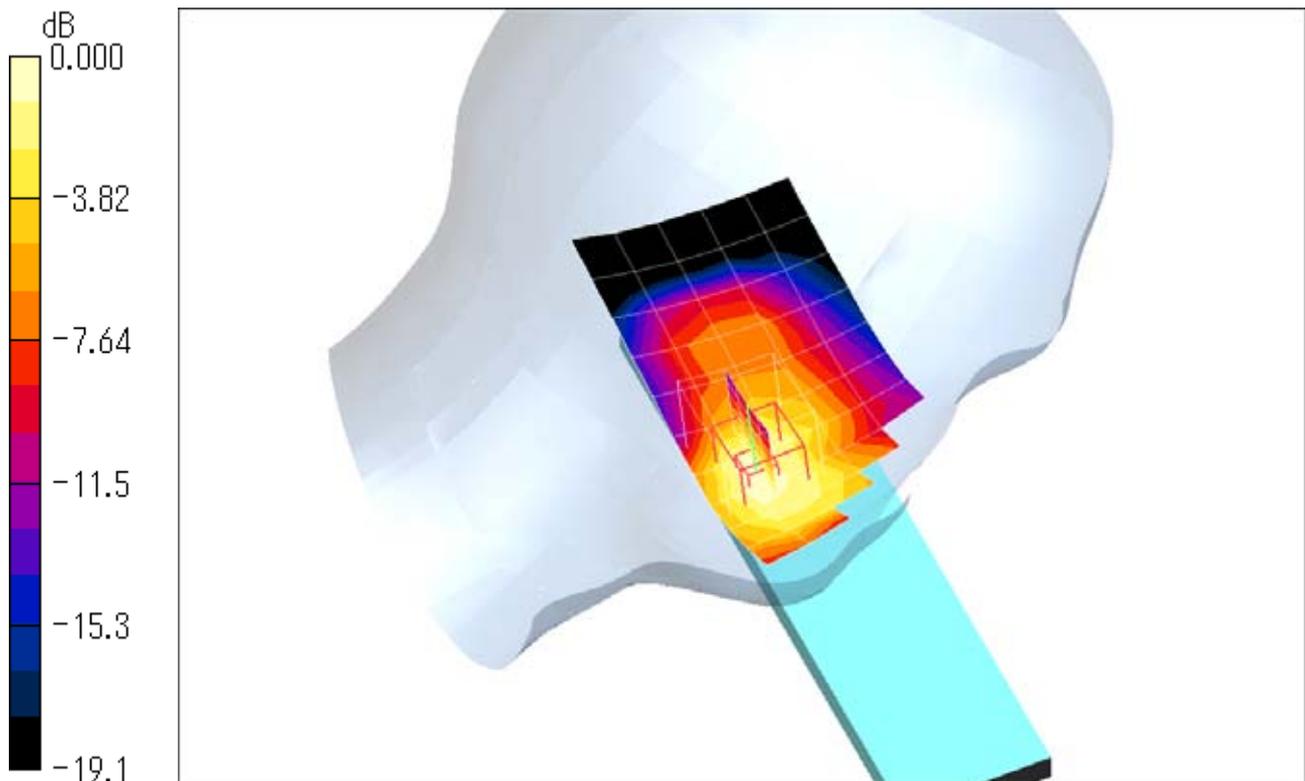

0 dB = 0.412mW/g

Test Laboratory: JAPAN QUALITY ASSURANCE ORGANIZATION

Left Head, Cheek/Touch 810ch (1909.8MHz)**DUT: Cellular Phone; Type: 842SH; Serial: 004401/11/268181/8**

Communication System: GSM 1900; Frequency: 1909.8 MHz; Duty Cycle: 1:8.3


Medium: HSL1900 Medium parameters used: $f = 1909.8$ MHz; $\sigma = 1.43$ mho/m; $\epsilon_r = 39.8$; $\rho = 1000$ kg/m³

Phantom section: Left Section

Measurement Standard: DAS4 (High Precision Assessment)

DASY4 Configuration:

- Probe: ET3DV6 - SN1679; ConvF(5.32, 5.32, 5.32); Calibrated: 2009/12/14
- Sensor-Surface: 4mm (Mechanical And Optical Surface Detection)
- Electronics: DAE3 Sn508; Calibrated: 2009/11/09
- Phantom: SAM 1200; Type: QD 000 P40 CA; Serial: 1200
- Measurement SW: DAS4, V4.7 Build 80; Postprocessing SW: SEMCAD, V1.8 Build 184

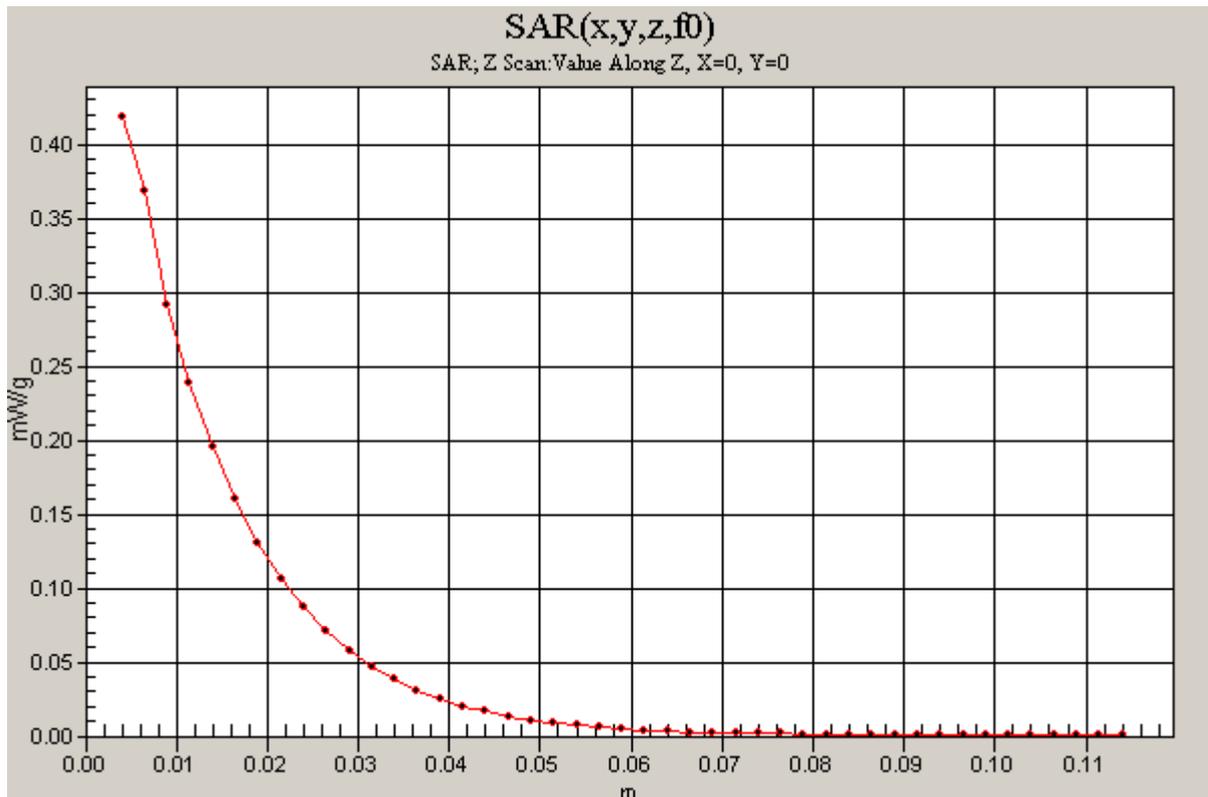Cheek/Touch Position/Z Scan (1x1x45): Measurement grid: dx=20mm, dy=20mm, dz=2.5mm
Maximum value of SAR (measured) = 0.418 mW/g

Test Laboratory: JAPAN QUALITY ASSURANCE ORGANIZATION

Left Head, Ear/Tilt 661ch (1880.0MHz)

DUT: Cellular Phone; Type: 842SH; Serial: 004401/11/268181/8

Communication System: GSM 1900; Frequency: 1880 MHz; Duty Cycle: 1:8.3

Medium: HSL1900 Medium parameters used: $f = 1880$ MHz; $\sigma = 1.4$ mho/m; $\epsilon_r = 39.9$; $\rho = 1000$ kg/m³

Phantom section: Left Section

Measurement Standard: DASY4 (High Precision Assessment)

DASY4 Configuration:

- Probe: ET3DV6 - SN1679; ConvF(5.32, 5.32, 5.32); Calibrated: 2009/12/14
- Sensor-Surface: 4mm (Mechanical And Optical Surface Detection)
- Electronics: DAE3 Sn508; Calibrated: 2009/11/09
- Phantom: SAM 1200; Type: QD 000 P40 CA; Serial: 1200
- Measurement SW: DASY4, V4.7 Build 80; Postprocessing SW: SEMCAD, V1.8 Build 184

Ear/Tilt Position/Area Scan (11x6x1): Measurement grid: dx=15mm, dy=15mm

Maximum value of SAR (measured) = 0.172 mW/g


Ear/Tilt Position/Zoom Scan (5x5x7)/Cube 0: Measurement grid: dx=8mm, dy=8mm, dz=5mm

Reference Value = 4.45 V/m; Power Drift = 0.022 dB

Peak SAR (extrapolated) = 0.229 W/kg

SAR(1 g) = 0.166 mW/g; SAR(10 g) = 0.107 mW/g

Maximum value of SAR (measured) = 0.176 mW/g

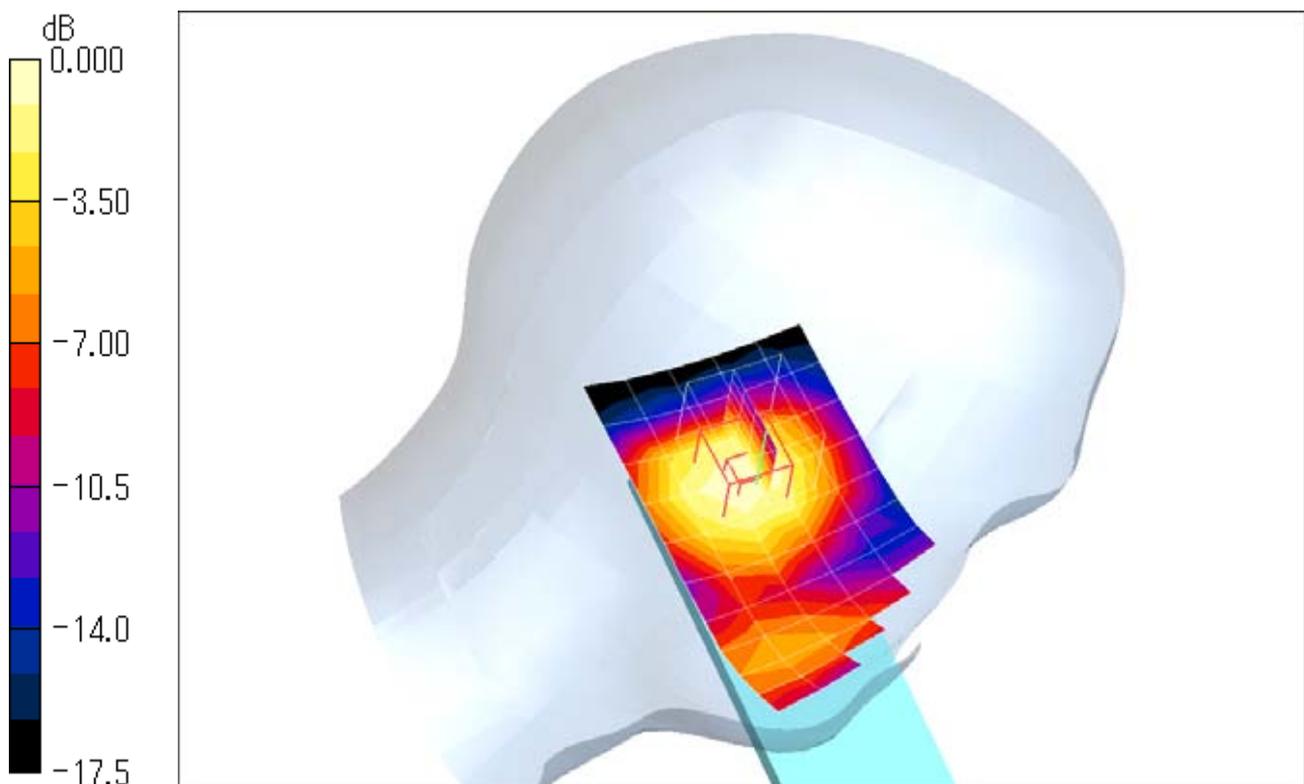

0 dB = 0.176mW/g

Test Laboratory: JAPAN QUALITY ASSURANCE ORGANIZATION

Right Head, Cheek/Touch 661ch (1880.0MHz)

DUT: Cellular Phone; Type: 842SH; Serial: 004401/11/268181/8

Communication System: GSM 1900; Frequency: 1880 MHz; Duty Cycle: 1:8.3

Medium: HSL1900 Medium parameters used: $f = 1880 \text{ MHz}$; $\sigma = 1.4 \text{ mho/m}$; $\epsilon_r = 39.9$; $\rho = 1000 \text{ kg/m}^3$

Phantom section: Right Section

Measurement Standard: DAS4 (High Precision Assessment)

DASY4 Configuration:

- Probe: ET3DV6 - SN1679; ConvF(5.32, 5.32, 5.32); Calibrated: 2009/12/14
- Sensor-Surface: 4mm (Mechanical And Optical Surface Detection)
- Electronics: DAE3 Sn508; Calibrated: 2009/11/09
- Phantom: SAM 1200; Type: QD 000 P40 CA; Serial: 1200
- Measurement SW: DAS4, V4.7 Build 80; Postprocessing SW: SEMCAD, V1.8 Build 184

Cheek/Touch Position/Area Scan (11x6x1): Measurement grid: $dx=15\text{mm}$, $dy=15\text{mm}$

Maximum value of SAR (measured) = 0.391 mW/g


Cheek/Touch Position/Zoom Scan (5x5x7)/Cube 0: Measurement grid: $dx=8\text{mm}$, $dy=8\text{mm}$, $dz=5\text{mm}$

Reference Value = 15.4 V/m; Power Drift = -0.064 dB

Peak SAR (extrapolated) = 0.455 W/kg

SAR(1 g) = 0.359 mW/g; SAR(10 g) = 0.238 mW/g

Maximum value of SAR (measured) = 0.381 mW/g

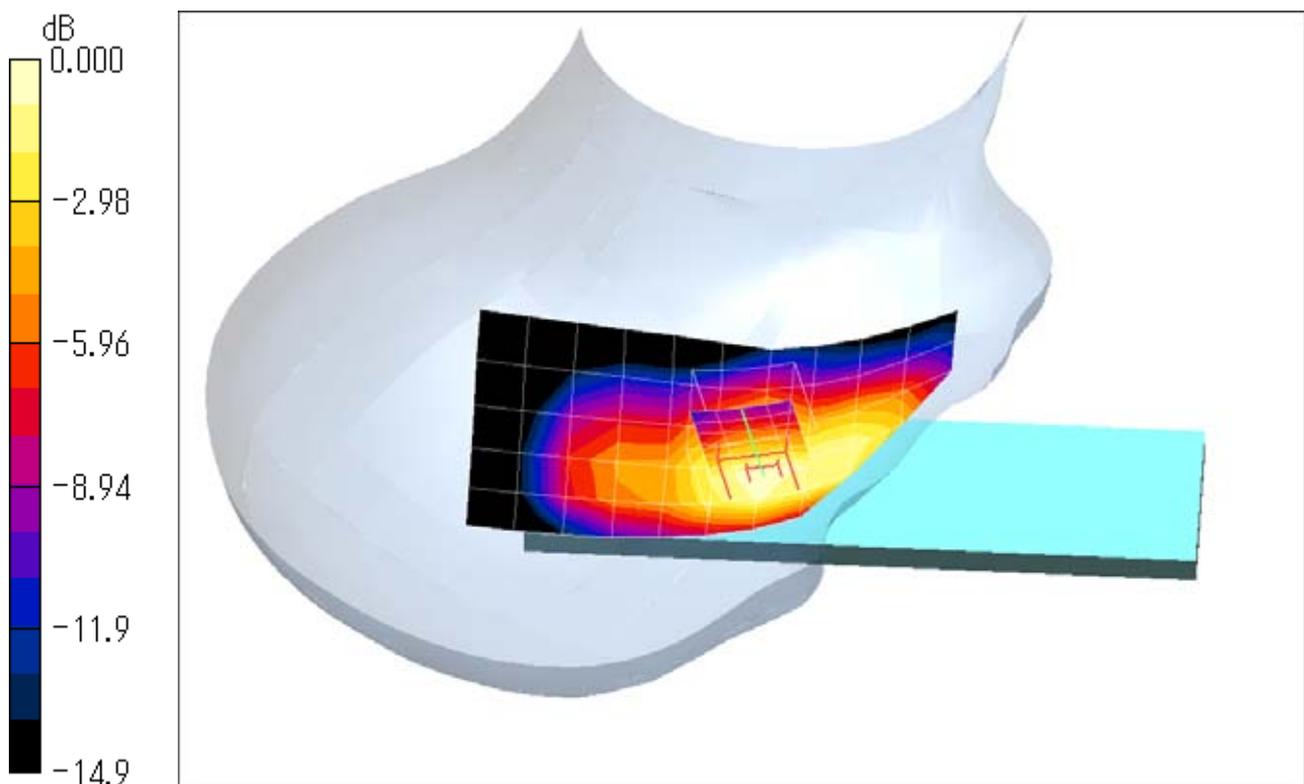

0 dB = 0.381mW/g

Test Laboratory: JAPAN QUALITY ASSURANCE ORGANIZATION

Right Head, Ear/Tilt 661ch (1880.0MHz)

DUT: Cellular Phone; Type: 842SH; Serial: 004401/11/268181/8

Communication System: GSM 1900; Frequency: 1880 MHz; Duty Cycle: 1:8.3

Medium: HSL1900 Medium parameters used: $f = 1880 \text{ MHz}$; $\sigma = 1.4 \text{ mho/m}$; $\epsilon_r = 39.9$; $\rho = 1000 \text{ kg/m}^3$

Phantom section: Right Section

Measurement Standard: DASY4 (High Precision Assessment)

DASY4 Configuration:

- Probe: ET3DV6 - SN1679; ConvF(5.32, 5.32, 5.32); Calibrated: 2009/12/14
- Sensor-Surface: 4mm (Mechanical And Optical Surface Detection)
- Electronics: DAE3 Sn508; Calibrated: 2009/11/09
- Phantom: SAM 1200; Type: QD 000 P40 CA; Serial: 1200
- Measurement SW: DASY4, V4.7 Build 80; Postprocessing SW: SEMCAD, V1.8 Build 184

Ear/Tilt Position/Area Scan (11x6x1): Measurement grid: $dx=15\text{mm}$, $dy=15\text{mm}$

Maximum value of SAR (measured) = 0.183 mW/g


Ear/Tilt Position/Zoom Scan (5x5x7)/Cube 0: Measurement grid: $dx=8\text{mm}$, $dy=8\text{mm}$, $dz=5\text{mm}$

Reference Value = 4.85 V/m; Power Drift = 0.013 dB

Peak SAR (extrapolated) = 0.250 W/kg

SAR(1 g) = 0.189 mW/g; SAR(10 g) = 0.122 mW/g

Maximum value of SAR (measured) = 0.205 mW/g

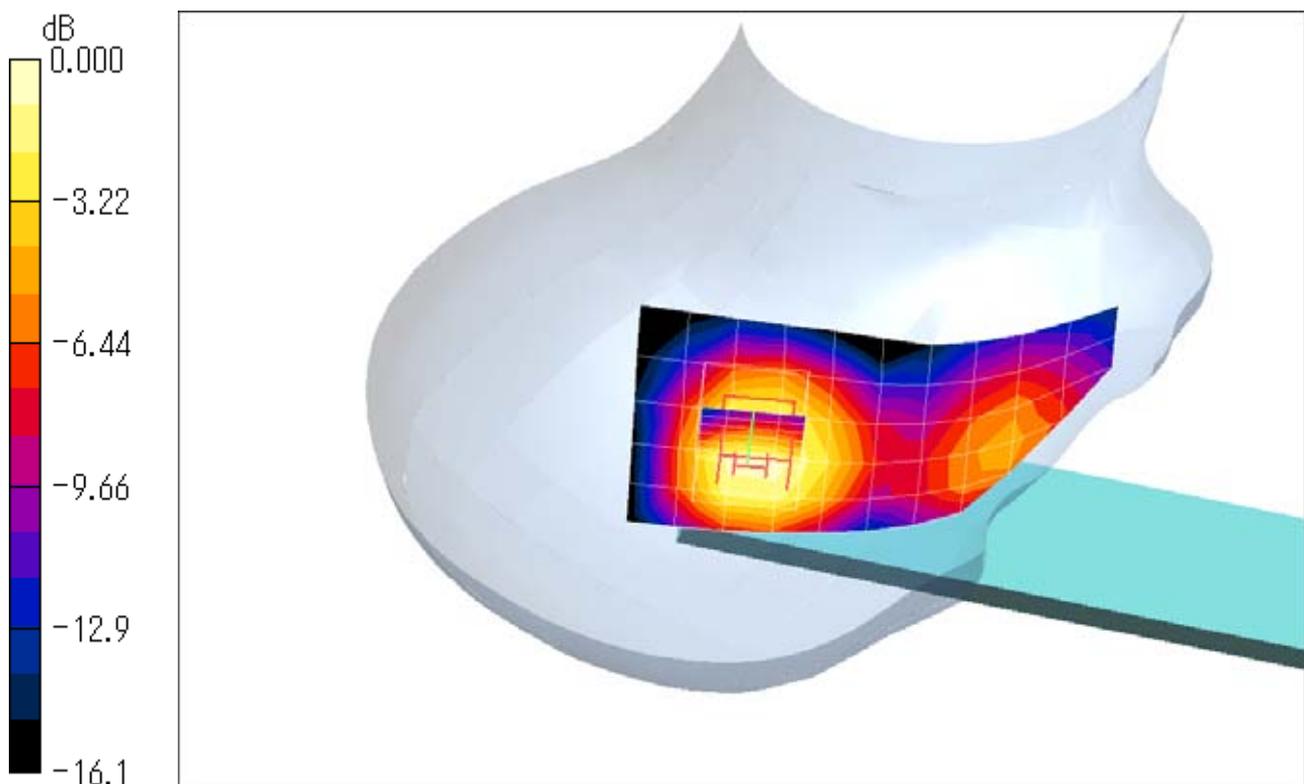

0 dB = 0.205mW/g

Test Laboratory: JAPAN QUALITY ASSURANCE ORGANIZATION

Body-worn Rear 661ch (1880.0MHz)**DUT: Cellular Phone; Type: 842SH; Serial: 004401/11/268181/8**

Communication System: GSM 1900; Frequency: 1880 MHz; Duty Cycle: 1:8.3

Medium: M1900 Medium parameters used: $f = 1880$ MHz; $\sigma = 1.56$ mho/m; $\epsilon_r = 52.7$; $\rho = 1000$ kg/m³

Phantom section: Flat Section

Measurement Standard: DAS4 (High Precision Assessment)

DASY4 Configuration:

- Probe: ET3DV6 - SN1679; ConvF(4.74, 4.74, 4.74); Calibrated: 2009/12/14
- Sensor-Surface: 4mm (Mechanical And Optical Surface Detection)
- Electronics: DAE3 Sn508; Calibrated: 2009/11/09
- Phantom: SAM 1200; Type: QD 000 P40 CA; Serial: 1200
- Measurement SW: DAS4, V4.7 Build 80; Postprocessing SW: SEMCAD, V1.8 Build 184

Body-worn/Area Scan (6x10x1): Measurement grid: dx=15mm, dy=15mm

Maximum value of SAR (measured) = 0.190 mW/g


Body-worn/Zoom Scan (5x5x7)/Cube 0: Measurement grid: dx=8mm, dy=8mm, dz=5mm

Reference Value = 4.88 V/m; Power Drift = 0.008 dB

Peak SAR (extrapolated) = 0.290 W/kg

SAR(1 g) = 0.193 mW/g; SAR(10 g) = 0.117 mW/g

Maximum value of SAR (measured) = 0.211 mW/g

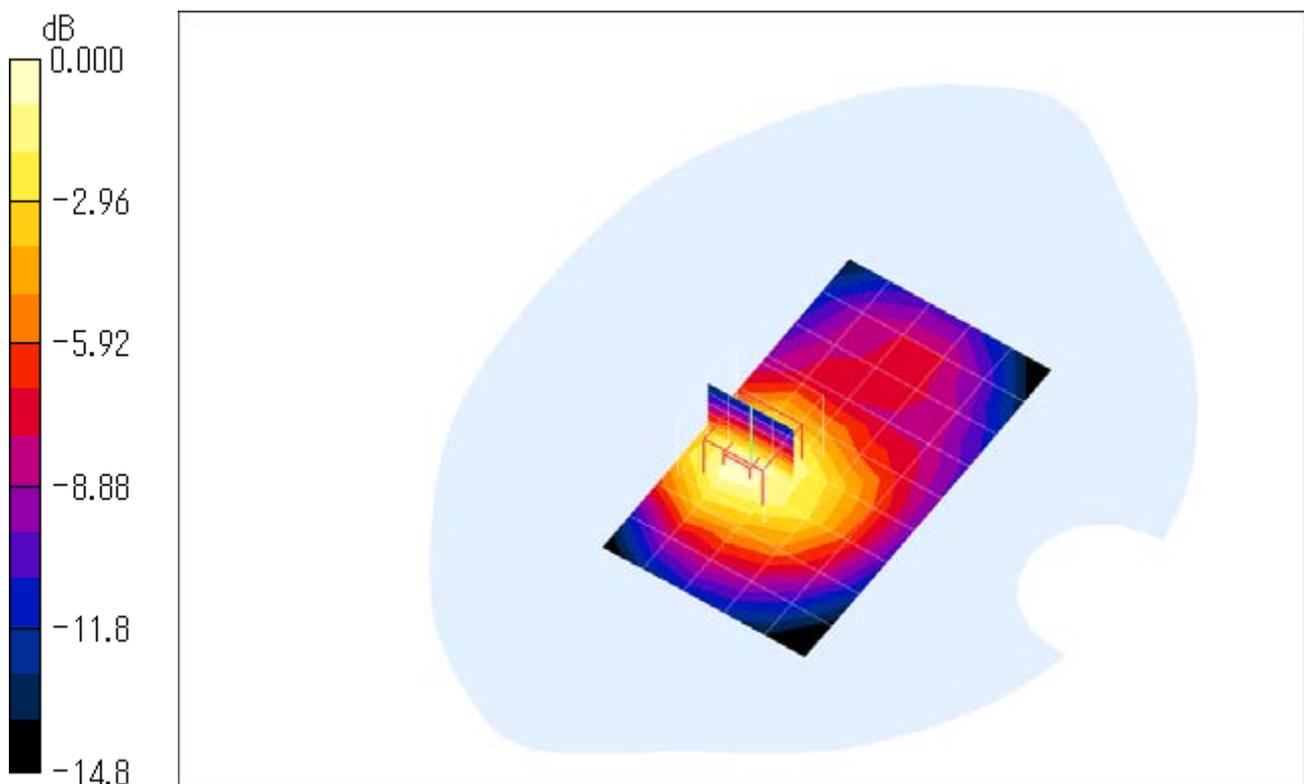

0 dB = 0.211mW/g

Test Laboratory: JAPAN QUALITY ASSURANCE ORGANIZATION

Body-worn Rear 661ch (1880.0MHz) : GPRS Class 10 (1slot)**DUT: Cellular Phone; Type: 842SH; Serial: 004401/11/268181/8**

Communication System: GSM 1900; Frequency: 1880 MHz; Duty Cycle: 1:8.3

Medium: M1900 Medium parameters used: $f = 1880$ MHz; $\sigma = 1.56$ mho/m; $\epsilon_r = 52.7$; $\rho = 1000$ kg/m³

Phantom section: Flat Section

Measurement Standard: DAS4 (High Precision Assessment)

DASY4 Configuration:

- Probe: ET3DV6 - SN1679; ConvF(4.74, 4.74, 4.74); Calibrated: 2009/12/14
- Sensor-Surface: 4mm (Mechanical And Optical Surface Detection)
- Electronics: DAE3 Sn508; Calibrated: 2009/11/09
- Phantom: SAM 1200; Type: QD 000 P40 CA; Serial: 1200
- Measurement SW: DAS4, V4.7 Build 80; Postprocessing SW: SEMCAD, V1.8 Build 184

Body-worn/Area Scan (6x10x1): Measurement grid: dx=15mm, dy=15mm

Maximum value of SAR (measured) = 0.183 mW/g


Body-worn/Zoom Scan (5x5x7)/Cube 0: Measurement grid: dx=8mm, dy=8mm, dz=5mm

Reference Value = 4.58 V/m; Power Drift = 0.030 dB

Peak SAR (extrapolated) = 0.268 W/kg

SAR(1 g) = 0.179 mW/g; SAR(10 g) = 0.110 mW/g

Maximum value of SAR (measured) = 0.194 mW/g

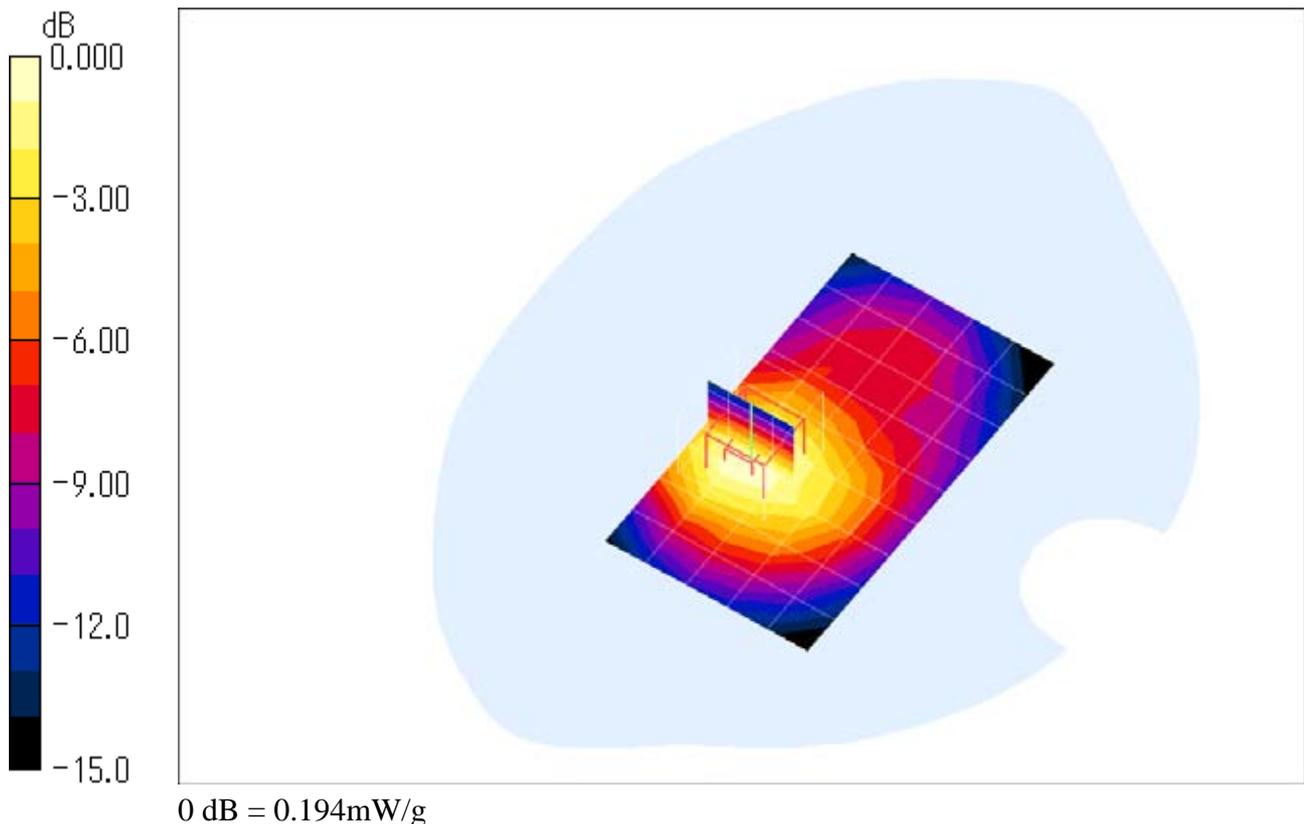

Test Laboratory: JAPAN QUALITY ASSURANCE ORGANIZATION

Body-worn Rear 512ch (1850.2MHz) : GPRS Class 10 (2slots)

DUT: Cellular Phone; Type: 842SH; Serial: 004401/11/268181/8

Communication System: GSM 1900; Frequency: 1850.2 MHz; Duty Cycle: 1:4.15

Medium: M1900 Medium parameters used: $f = 1850.2 \text{ MHz}$; $\sigma = 1.52 \text{ mho/m}$; $\epsilon_r = 52.8$; $\rho = 1000 \text{ kg/m}^3$

Phantom section: Flat Section

Measurement Standard: DAS4 (High Precision Assessment)

DASY4 Configuration:

- Probe: ET3DV6 - SN1679; ConvF(4.74, 4.74, 4.74); Calibrated: 2009/12/14
- Sensor-Surface: 4mm (Mechanical And Optical Surface Detection)
- Electronics: DAE3 Sn508; Calibrated: 2009/11/09
- Phantom: SAM 1200; Type: QD 000 P40 CA; Serial: 1200
- Measurement SW: DAS4, V4.7 Build 80; Postprocessing SW: SEMCAD, V1.8 Build 184

Body-worn/Area Scan (6x10x1): Measurement grid: $dx=15\text{mm}$, $dy=15\text{mm}$

Maximum value of SAR (measured) = 0.394 mW/g


Body-worn/Zoom Scan (5x5x7)/Cube 0: Measurement grid: $dx=8\text{mm}$, $dy=8\text{mm}$, $dz=5\text{mm}$

Reference Value = 6.40 V/m; Power Drift = -0.029 dB

Peak SAR (extrapolated) = 0.570 W/kg

SAR(1 g) = 0.384 mW/g; SAR(10 g) = 0.235 mW/g

Maximum value of SAR (measured) = 0.421 mW/g

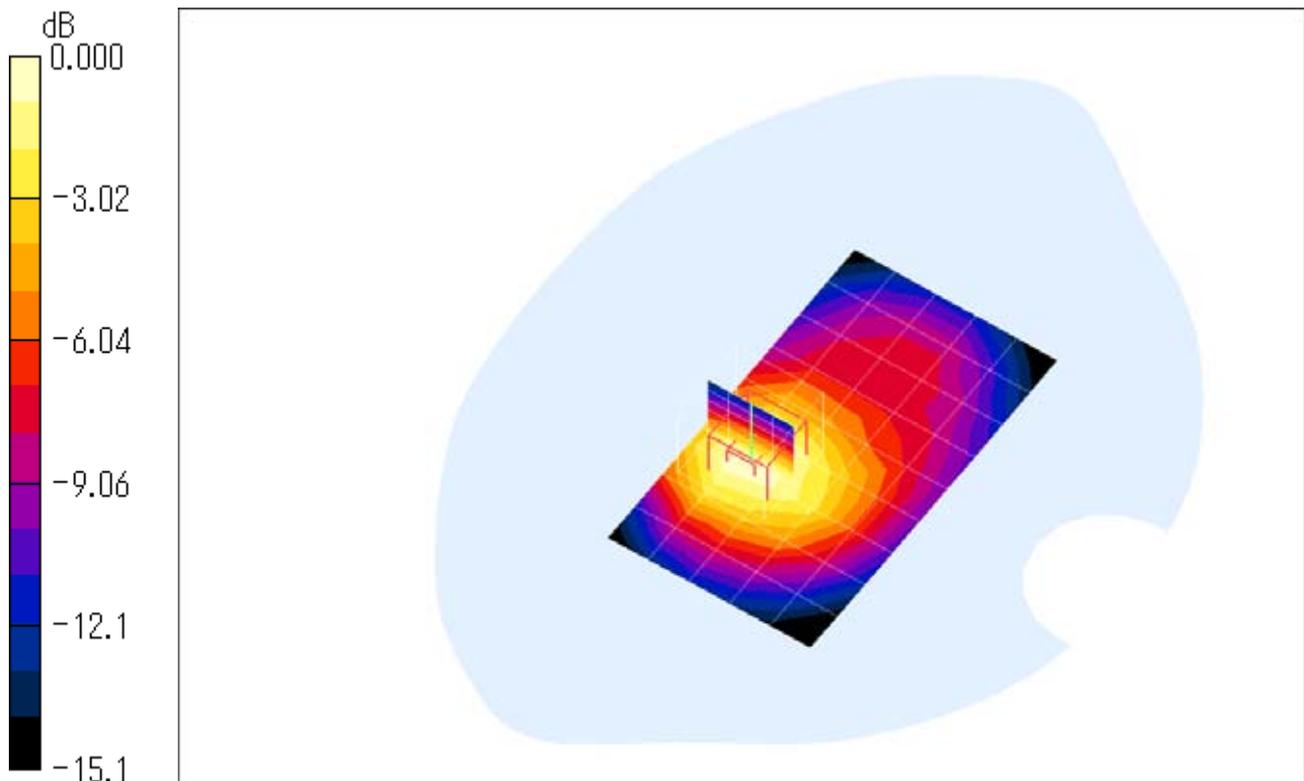

Test Laboratory: JAPAN QUALITY ASSURANCE ORGANIZATION

Body-worn Rear 661ch (1880.0MHz) : GPRS Class 10 (2slots)**DUT: Cellular Phone; Type: 842SH; Serial: 004401/11/268181/8**

Communication System: GSM 1900; Frequency: 1880 MHz; Duty Cycle: 1:4.15

Medium: M1900 Medium parameters used: $f = 1880$ MHz; $\sigma = 1.56$ mho/m; $\epsilon_r = 52.7$; $\rho = 1000$ kg/m³

Phantom section: Flat Section

Measurement Standard: DAS4 (High Precision Assessment)

DASY4 Configuration:

- Probe: ET3DV6 - SN1679; ConvF(4.74, 4.74, 4.74); Calibrated: 2009/12/14
- Sensor-Surface: 4mm (Mechanical And Optical Surface Detection)
- Electronics: DAE3 Sn508; Calibrated: 2009/11/09
- Phantom: SAM 1200; Type: QD 000 P40 CA; Serial: 1200
- Measurement SW: DAS4, V4.7 Build 80; Postprocessing SW: SEMCAD, V1.8 Build 184

Body-worn/Area Scan (6x10x1): Measurement grid: dx=15mm, dy=15mm

Maximum value of SAR (measured) = 0.370 mW/g


Body-worn/Zoom Scan (5x5x7)/Cube 0: Measurement grid: dx=8mm, dy=8mm, dz=5mm

Reference Value = 6.28 V/m; Power Drift = 0.085 dB

Peak SAR (extrapolated) = 0.534 W/kg

SAR(1 g) = 0.354 mW/g; SAR(10 g) = 0.214 mW/g

Maximum value of SAR (measured) = 0.388 mW/g

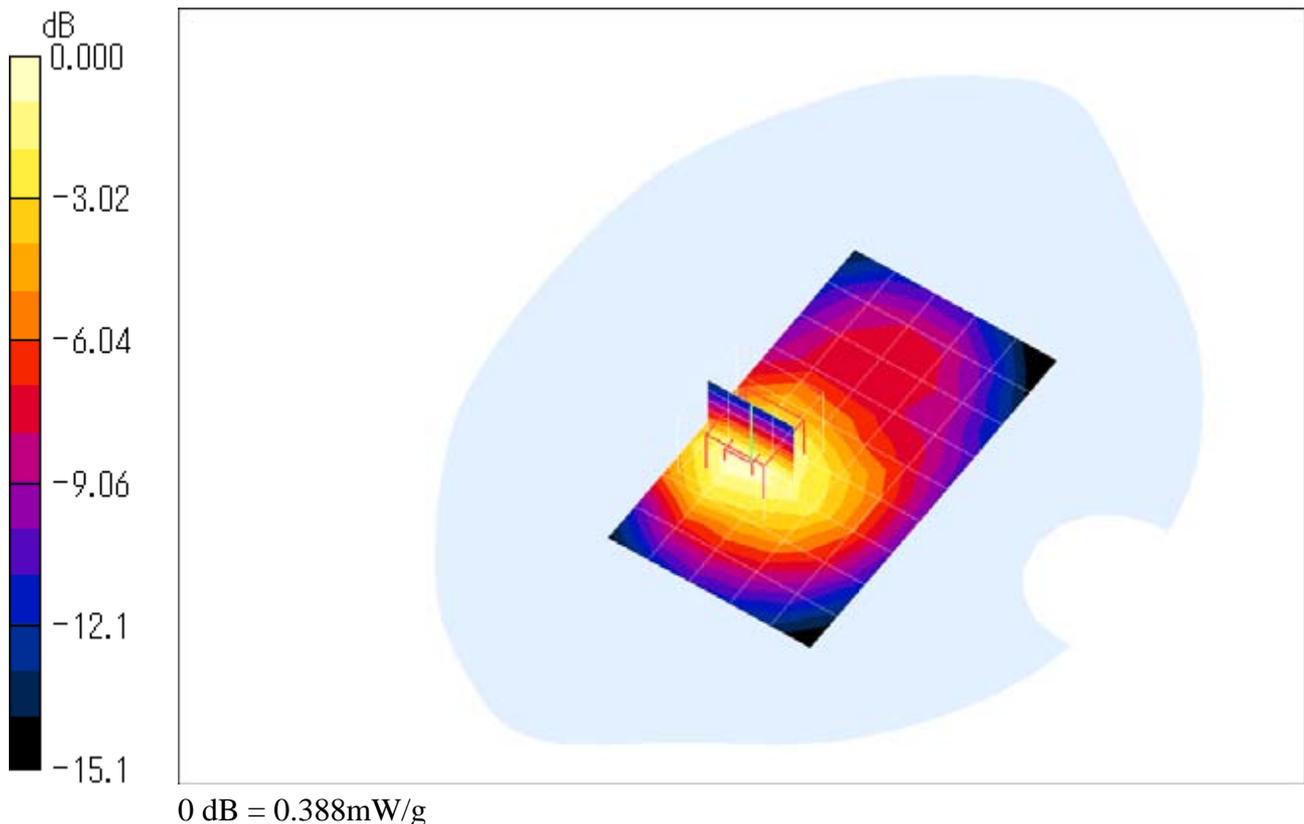

Test Laboratory: JAPAN QUALITY ASSURANCE ORGANIZATION

Body-worn Rear 810ch (1909.8MHz) : GPRS Class 10 (2slots)**DUT: Cellular Phone; Type: 842SH; Serial: 004401/11/268181/8**

Communication System: GSM 1900; Frequency: 1909.8 MHz; Duty Cycle: 1:4.15

Medium: M1900 Medium parameters used: $f = 1909.8 \text{ MHz}$; $\sigma = 1.59 \text{ mho/m}$; $\epsilon_r = 52.7$; $\rho = 1000 \text{ kg/m}^3$

Phantom section: Flat Section

Measurement Standard: DAS4 (High Precision Assessment)

DASY4 Configuration:

- Probe: ET3DV6 - SN1679; ConvF(4.74, 4.74, 4.74); Calibrated: 2009/12/14
- Sensor-Surface: 4mm (Mechanical And Optical Surface Detection)
- Electronics: DAE3 Sn508; Calibrated: 2009/11/09
- Phantom: SAM 1200; Type: QD 000 P40 CA; Serial: 1200
- Measurement SW: DAS4, V4.7 Build 80; Postprocessing SW: SEMCAD, V1.8 Build 184

Body-worn/Area Scan (6x10x1): Measurement grid: $dx=15\text{mm}$, $dy=15\text{mm}$

Maximum value of SAR (measured) = 0.420 mW/g


Body-worn/Zoom Scan (5x5x7)/Cube 0: Measurement grid: $dx=8\text{mm}$, $dy=8\text{mm}$, $dz=5\text{mm}$

Reference Value = 7.19 V/m; Power Drift = -0.079 dB

Peak SAR (extrapolated) = 0.641 W/kg

SAR(1 g) = 0.416 mW/g; SAR(10 g) = 0.248 mW/g

Maximum value of SAR (measured) = 0.456 mW/g

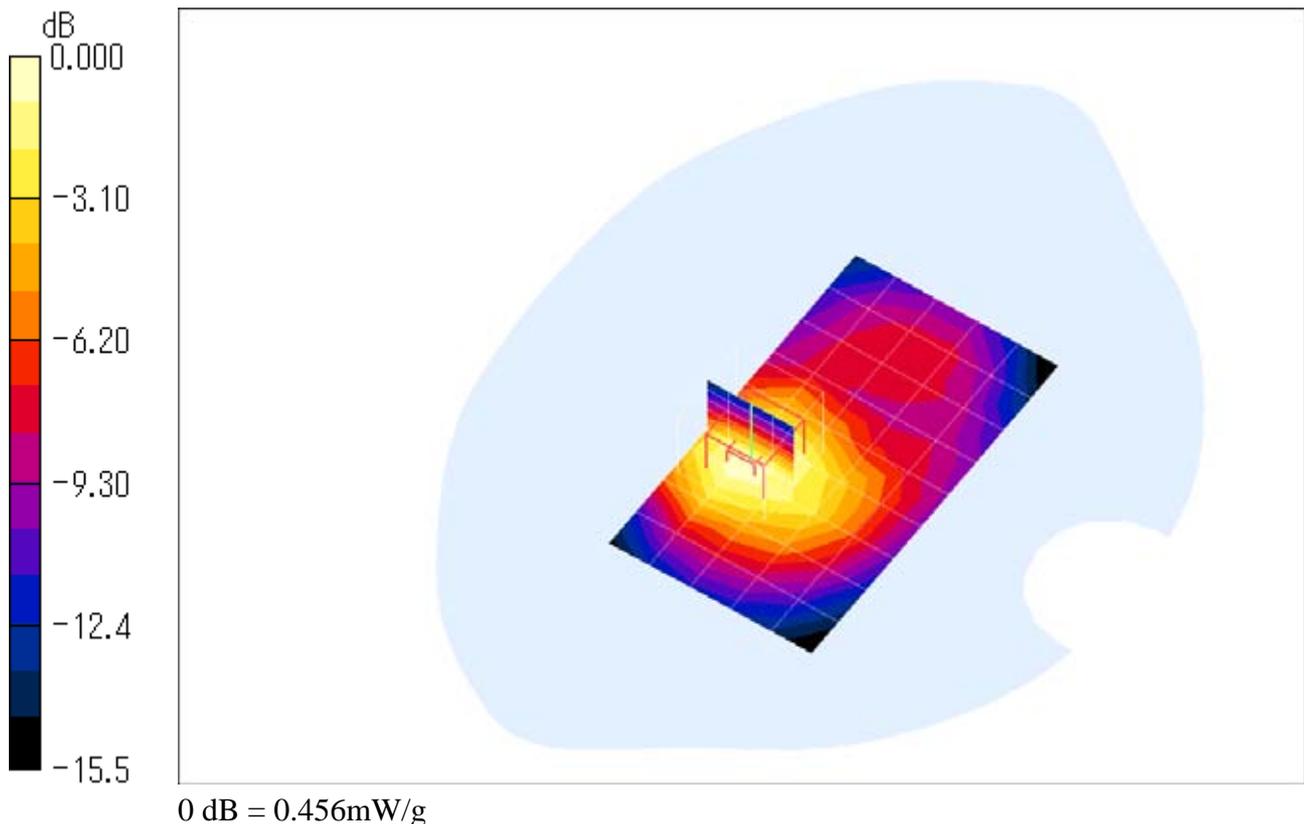

Test Laboratory: JAPAN QUALITY ASSURANCE ORGANIZATION

Body-worn Rear 810ch (1909.8MHz) : GPRS Class 10 (2slots)**DUT: Cellular Phone; Type: 842SH; Serial: 004401/11/268181/8**

Communication System: GSM 1900; Frequency: 1909.8 MHz; Duty Cycle: 1:4.15

Medium: M1900 Medium parameters used: $f = 1909.8 \text{ MHz}$; $\sigma = 1.59 \text{ mho/m}$; $\epsilon_r = 52.7$; $\rho = 1000 \text{ kg/m}^3$

Phantom section: Flat Section


Measurement Standard: DAS4 (High Precision Assessment)

DASY4 Configuration:

- Probe: ET3DV6 - SN1679; ConvF(4.74, 4.74, 4.74); Calibrated: 2009/12/14
- Sensor-Surface: 4mm (Mechanical And Optical Surface Detection)
- Electronics: DAE3 Sn508; Calibrated: 2009/11/09
- Phantom: SAM 1200; Type: QD 000 P40 CA; Serial: 1200
- Measurement SW: DAS4, V4.7 Build 80; Postprocessing SW: SEMCAD, V1.8 Build 184

Body-worn/Z Scan (1x1x45): Measurement grid: $dx=20\text{mm}$, $dy=20\text{mm}$, $dz=2.5\text{mm}$

Maximum value of SAR (measured) = 0.458 mW/g

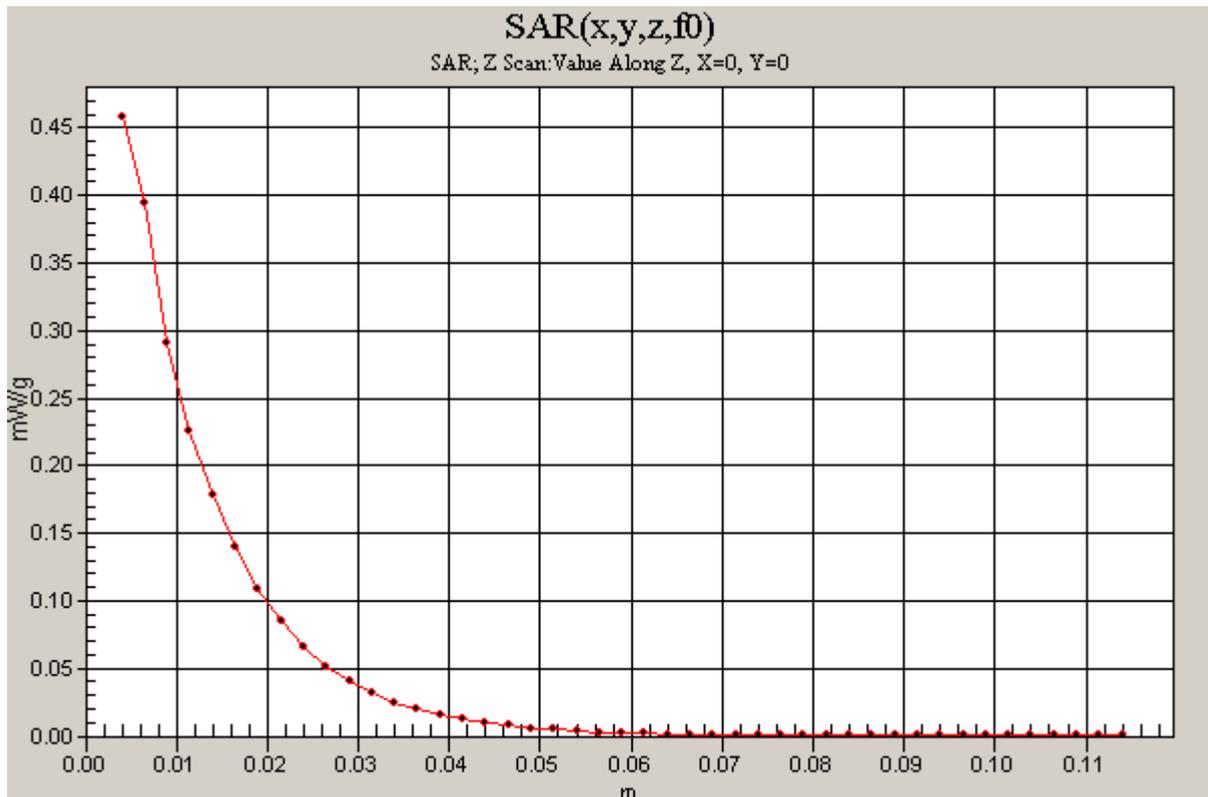

Test Laboratory: JAPAN QUALITY ASSURANCE ORGANIZATION

Body-worn Front 661ch (1880.0MHz) : GPRS Class 10 (2slots)**DUT: Cellular Phone; Type: 842SH; Serial: 004401/11/268181/8**

Communication System: GSM 1900; Frequency: 1880 MHz; Duty Cycle: 1:4.15

Medium: M1900 Medium parameters used: $f = 1880 \text{ MHz}$; $\sigma = 1.56 \text{ mho/m}$; $\epsilon_r = 52.7$; $\rho = 1000 \text{ kg/m}^3$

Phantom section: Flat Section

Measurement Standard: DASY4 (High Precision Assessment)

DASY4 Configuration:

- Probe: ET3DV6 - SN1679; ConvF(4.74, 4.74, 4.74); Calibrated: 2009/12/14
- Sensor-Surface: 4mm (Mechanical And Optical Surface Detection)
- Electronics: DAE3 Sn508; Calibrated: 2009/11/09
- Phantom: SAM 1200; Type: QD 000 P40 CA; Serial: 1200
- Measurement SW: DASY4, V4.7 Build 80; Postprocessing SW: SEMCAD, V1.8 Build 184

Body-worn/Area Scan (6x10x1): Measurement grid: $dx=15\text{mm}$, $dy=15\text{mm}$

Maximum value of SAR (measured) = 0.282 mW/g


Body-worn/Zoom Scan (5x5x7)/Cube 0: Measurement grid: $dx=8\text{mm}$, $dy=8\text{mm}$, $dz=5\text{mm}$

Reference Value = 8.71 V/m; Power Drift = 0.042 dB

Peak SAR (extrapolated) = 0.380 W/kg

SAR(1 g) = 0.282 mW/g; SAR(10 g) = 0.184 mW/g

Maximum value of SAR (measured) = 0.306 mW/g

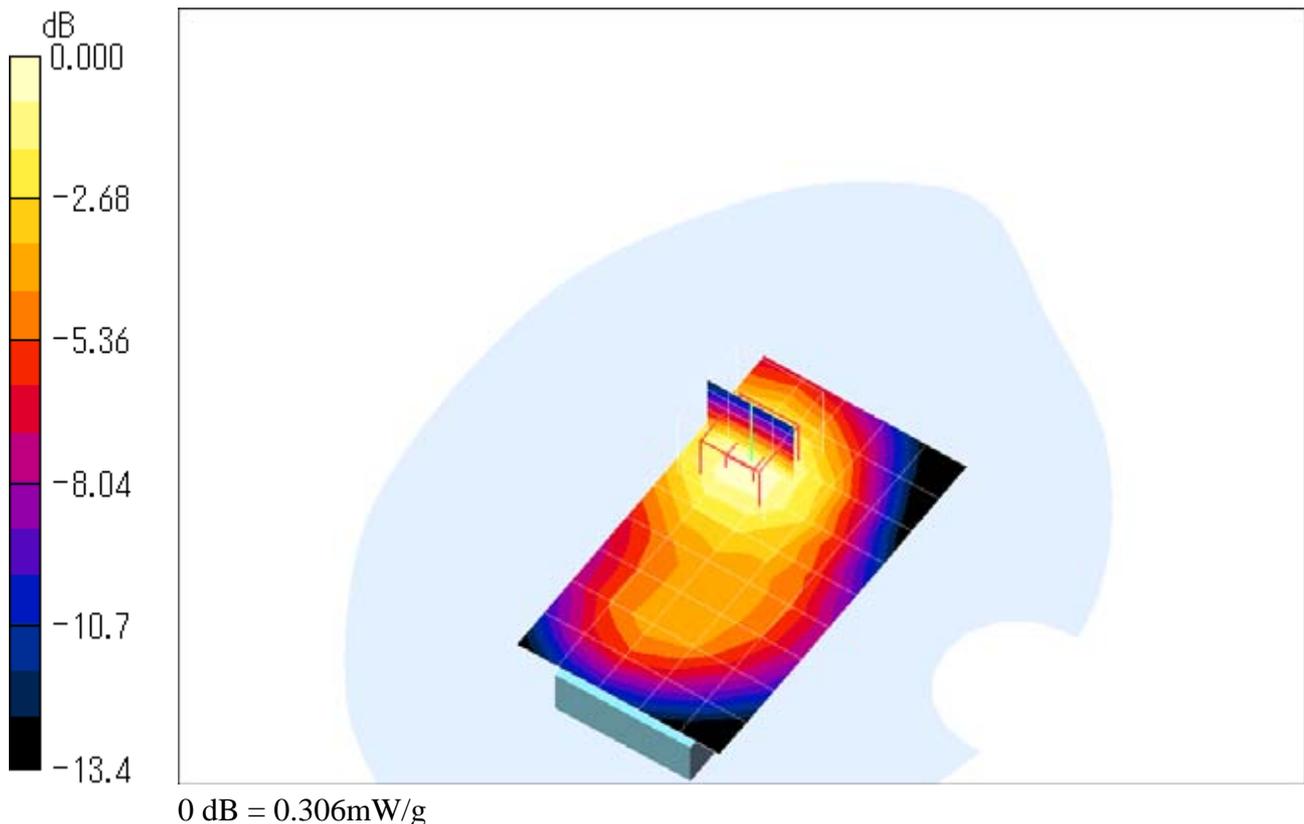



Attachment 3 – Dosimetric E-Field Probe – ET3DV6, S/N: 1679 Calibration Data



Accredited by the Swiss Accreditation Service (SAS)
The Swiss Accreditation Service is one of the signatories to the EA
Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: SCS 108

Client JQA (PTT)

Certificate No: ET3-1679_Dec09

CALIBRATION CERTIFICATE

Object ET3DV6 - SN:1679

Calibration procedure(s) QA CAL-01.v6, QA CAL-23.v3 and QA CAL-25.v2
Calibration procedure for dosimetric E-field probes

Calibration date: December 14, 2009

This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI).
The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility: environment temperature $(22 \pm 3)^\circ\text{C}$ and humidity $< 70\%$.

Calibration Equipment used (M&TE critical for calibration)

| Primary Standards | ID # | Cal Date (Certificate No.) | Scheduled Calibration |
|----------------------------|-----------------|--------------------------------|-----------------------|
| Power meter E4419B | GB41293874 | 1-Apr-09 (No. 217-01030) | Apr-10 |
| Power sensor E4412A | MY41495277 | 1-Apr-09 (No. 217-01030) | Apr-10 |
| Power sensor E4412A | MY41498087 | 1-Apr-09 (No. 217-01030) | Apr-10 |
| Reference 3 dB Attenuator | SN: S5054 (3c) | 31-Mar-09 (No. 217-01026) | Mar-10 |
| Reference 20 dB Attenuator | SN: S5086 (20b) | 31-Mar-09 (No. 217-01028) | Mar-10 |
| Reference 30 dB Attenuator | SN: S5129 (30b) | 31-Mar-09 (No. 217-01027) | Mar-10 |
| Reference Probe ES3DV2 | SN: 3013 | 2-Jan-09 (No. ES3-3013_Jan09) | Jan-10 |
| DAE4 | SN: 660 | 29-Sep-09 (No. DAE4-660_Sep09) | Sep-10 |

| Secondary Standards | ID # | Check Date (in house) | Scheduled Check |
|---------------------------|--------------|-----------------------------------|------------------------|
| RF generator HP 8648C | US3642U01700 | 4-Aug-99 (in house check Oct-09) | In house check: Oct-11 |
| Network Analyzer HP 8753E | US37390585 | 18-Oct-01 (in house check Oct-09) | In house check: Oct10 |

Calibrated by: Jeton Kastrati Laboratory Technician

Signature

Approved by: Katja Pokovic Technical Manager

Signature

Issued: December 16, 2009

This calibration certificate shall not be reproduced except in full without written approval of the laboratory.



Accredited by the Swiss Accreditation Service (SAS)
The Swiss Accreditation Service is one of the signatories to the EA
Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: **SCS 108**

Glossary:

| | |
|--------------------------|---|
| TSL | tissue simulating liquid |
| NORM _{x,y,z} | sensitivity in free space |
| ConvF | sensitivity in TSL / NORM _{x,y,z} |
| DCP | diode compression point |
| CF | crest factor (1/duty_cycle) of the RF signal |
| A, B, C | modulation dependent linearization parameters |
| Polarization φ | φ rotation around probe axis |
| Polarization ϑ | ϑ rotation around an axis that is in the plane normal to probe axis (at measurement center), i.e., $\vartheta = 0$ is normal to probe axis |

Calibration is Performed According to the Following Standards:

- IEEE Std 1528-2003, "IEEE Recommended Practice for Determining the Peak Spatial-Averaged Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques", December 2003
- IEC 62209-1, "Procedure to measure the Specific Absorption Rate (SAR) for hand-held devices used in close proximity to the ear (frequency range of 300 MHz to 3 GHz)", February 2005

Methods Applied and Interpretation of Parameters:

- NORM_{x,y,z}**: Assessed for E-field polarization $\vartheta = 0$ ($f \leq 900$ MHz in TEM-cell; $f > 1800$ MHz: R22 waveguide). NORM_{x,y,z} are only intermediate values, i.e., the uncertainties of NORM_{x,y,z} does not effect the E^2 -field uncertainty inside TSL (see below *ConvF*).
- NORM(f)_{x,y,z}** = NORM_{x,y,z} * *frequency_response* (see Frequency Response Chart). This linearization is implemented in DASY4 software versions later than 4.2. The uncertainty of the frequency response is included in the stated uncertainty of *ConvF*.
- DCP_{x,y,z}**: DCP are numerical linearization parameters assessed based on the data of power sweep with CW signal (no uncertainty required). DCP does not depend on frequency nor media.
- A_{x,y,z}; B_{x,y,z}; C_{x,y,z}; VR_{x,y,z}**: A, B, C are numerical linearization parameters assessed based on the data of power sweep for specific modulation signal. The parameters do not depend on frequency nor media. VR is the maximum calibration range expressed in RMS voltage across the diode.
- ConvF and Boundary Effect Parameters**: Assessed in flat phantom using E-field (or Temperature Transfer Standard for $f \leq 800$ MHz) and inside waveguide using analytical field distributions based on power measurements for $f > 800$ MHz. The same setups are used for assessment of the parameters applied for boundary compensation (alpha, depth) of which typical uncertainty values are given. These parameters are used in DASY4 software to improve probe accuracy close to the boundary. The sensitivity in TSL corresponds to NORM_{x,y,z} * *ConvF* whereby the uncertainty corresponds to that given for *ConvF*. A frequency dependent *ConvF* is used in DASY version 4.4 and higher which allows extending the validity from ± 50 MHz to ± 100 MHz.
- Spherical isotropy (3D deviation from isotropy)**: in a field of low gradients realized using a flat phantom exposed by a patch antenna.
- Sensor Offset**: The sensor offset corresponds to the offset of virtual measurement center from the probe tip (on probe axis). No tolerance required.

Probe ET3DV6

SN:1679

| | |
|------------------|-------------------|
| Manufactured: | May 7, 2002 |
| Last calibrated: | December 15, 2008 |
| Recalibrated: | December 14, 2009 |

Calibrated for DASYS Systems

(Note: non-compatible with DASYS2 system!)

DASY - Parameters of Probe: ET3DV6 SN:1679

Basic Calibration Parameters

| | Sensor X | Sensor Y | Sensor Z | Unc (k=2) |
|---|----------|----------|----------|-----------|
| Norm ($\mu\text{V}/(\text{V}/\text{m})^2$) ^A | 1.94 | 1.89 | 1.92 | ± 10.1% |
| DCP (mV) ^B | 93.0 | 92.4 | 92.6 | |

Modulation Calibration Parameters

| UID | Communication System Name | PAR | | A dB | B dBuV | C | VR mV | Unc ^E (k=2) |
|-------|---------------------------|------|---|---------|-----------|------|----------|---------------------------|
| 10000 | CW | 0.00 | X | 0.00 | 0.00 | 1.00 | 300 | ± 1.5% |
| | | | Y | 0.00 | 0.00 | 1.00 | 300 | |
| | | | Z | 0.00 | 0.00 | 1.00 | 300 | |

The reported uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor k=2, which for a normal distribution corresponds to a coverage probability of approximately 95%.

^A The uncertainties of NormX,Y,Z do not affect the E²-field uncertainty inside TSL (see Pages 5 and 6).

^B Numerical linearization parameter: uncertainty not required.

^E Uncertainty is determined using the maximum deviation from linear response applying recatangular distribution and is expressed for the square of the field value.

DASY - Parameters of Probe: ET3DV6 SN:1679

Calibration Parameter Determined in Head Tissue Simulating Media

| f [MHz] | Validity [MHz] ^c | Permittivity | Conductivity | ConvF X | ConvF Y | ConvF Z | Alpha | Depth Unc (k=2) |
|---------|-----------------------------|--------------|--------------|---------|---------|---------|-------|-----------------|
| 835 | ± 50 / ± 100 | 41.9 ± 5% | 0.89 ± 5% | 6.63 | 6.63 | 6.63 | 0.47 | 2.03 ± 11.0% |
| 900 | ± 50 / ± 100 | 41.5 ± 5% | 0.97 ± 5% | 6.43 | 6.43 | 6.43 | 0.37 | 2.38 ± 11.0% |
| 1450 | ± 50 / ± 100 | 40.5 ± 5% | 1.20 ± 5% | 5.56 | 5.56 | 5.56 | 0.39 | 3.25 ± 11.0% |
| 1750 | ± 50 / ± 100 | 40.1 ± 5% | 1.37 ± 5% | 5.63 | 5.63 | 5.63 | 0.49 | 2.94 ± 11.0% |
| 1900 | ± 50 / ± 100 | 40.0 ± 5% | 1.40 ± 5% | 5.32 | 5.32 | 5.32 | 0.48 | 2.89 ± 11.0% |
| 1950 | ± 50 / ± 100 | 40.0 ± 5% | 1.40 ± 5% | 5.15 | 5.15 | 5.15 | 0.54 | 2.68 ± 11.0% |
| 2450 | ± 50 / ± 100 | 39.2 ± 5% | 1.80 ± 5% | 4.62 | 4.62 | 4.62 | 0.99 | 1.82 ± 11.0% |

^c The validity of ± 100 MHz only applies for DASY v4.4 and higher (see Page 2). The uncertainty is the RSS of the ConvF uncertainty at calibration frequency and the uncertainty for the indicated frequency band.

DASY - Parameters of Probe: ET3DV6 SN:1679


Calibration Parameter Determined in Body Tissue Simulating Media

| f [MHz] | Validity [MHz] ^C | Permittivity | Conductivity | ConvF X | ConvF Y | ConvF Z | Alpha | Depth Unc (k=2) |
|---------|-----------------------------|--------------|--------------|---------|---------|---------|-------|-----------------|
| 835 | ± 50 / ± 100 | 55.2 ± 5% | 0.97 ± 5% | 6.31 | 6.31 | 6.31 | 0.23 | 3.78 ± 11.0% |
| 900 | ± 50 / ± 100 | 55.0 ± 5% | 1.05 ± 5% | 6.15 | 6.15 | 6.15 | 0.28 | 3.48 ± 11.0% |
| 1450 | ± 50 / ± 100 | 54.0 ± 5% | 1.30 ± 5% | 5.36 | 5.36 | 5.36 | 0.50 | 2.53 ± 11.0% |
| 1750 | ± 50 / ± 100 | 53.4 ± 5% | 1.49 ± 5% | 5.08 | 5.08 | 5.08 | 0.71 | 2.98 ± 11.0% |
| 1900 | ± 50 / ± 100 | 53.3 ± 5% | 1.52 ± 5% | 4.74 | 4.74 | 4.74 | 0.97 | 2.36 ± 11.0% |
| 1950 | ± 50 / ± 100 | 53.3 ± 5% | 1.52 ± 5% | 4.84 | 4.84 | 4.84 | 0.99 | 2.31 ± 11.0% |
| 2450 | ± 50 / ± 100 | 52.7 ± 5% | 1.95 ± 5% | 4.21 | 4.21 | 4.21 | 0.99 | 1.74 ± 11.0% |

^C The validity of ± 100 MHz only applies for DASY v4.4 and higher (see Page 2). The uncertainty is the RSS of the ConvF uncertainty at calibration frequency and the uncertainty for the indicated frequency band.



Frequency Response of E-Field

(TEM-Cell:ifi110 EXX, Waveguide: R22)

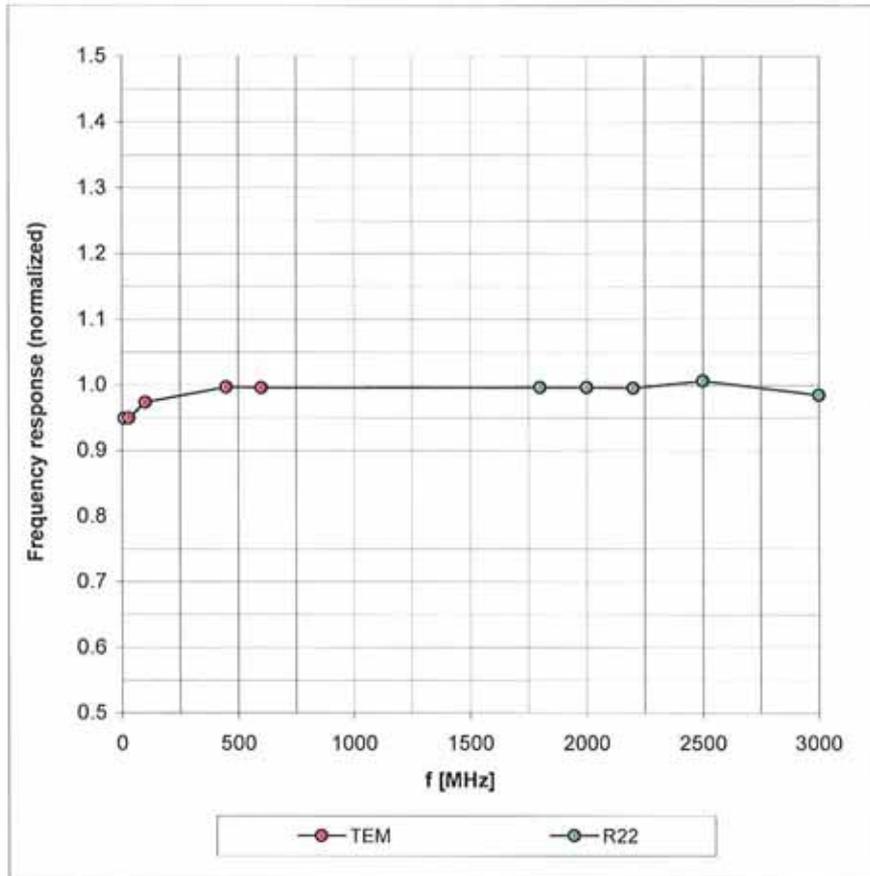



Uncertainty of Frequency Response of E-field: $\pm 6.3\%$ (k=2)

Receiving Pattern (ϕ), $\vartheta = 0^\circ$

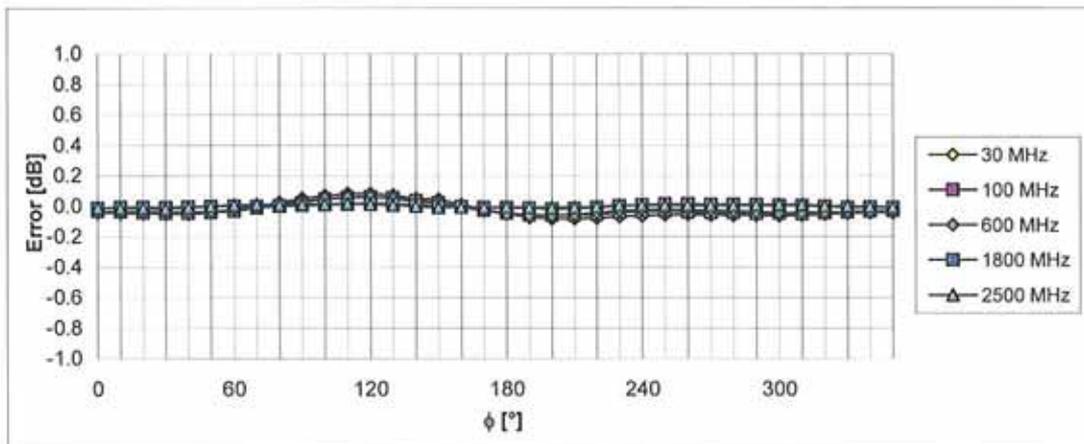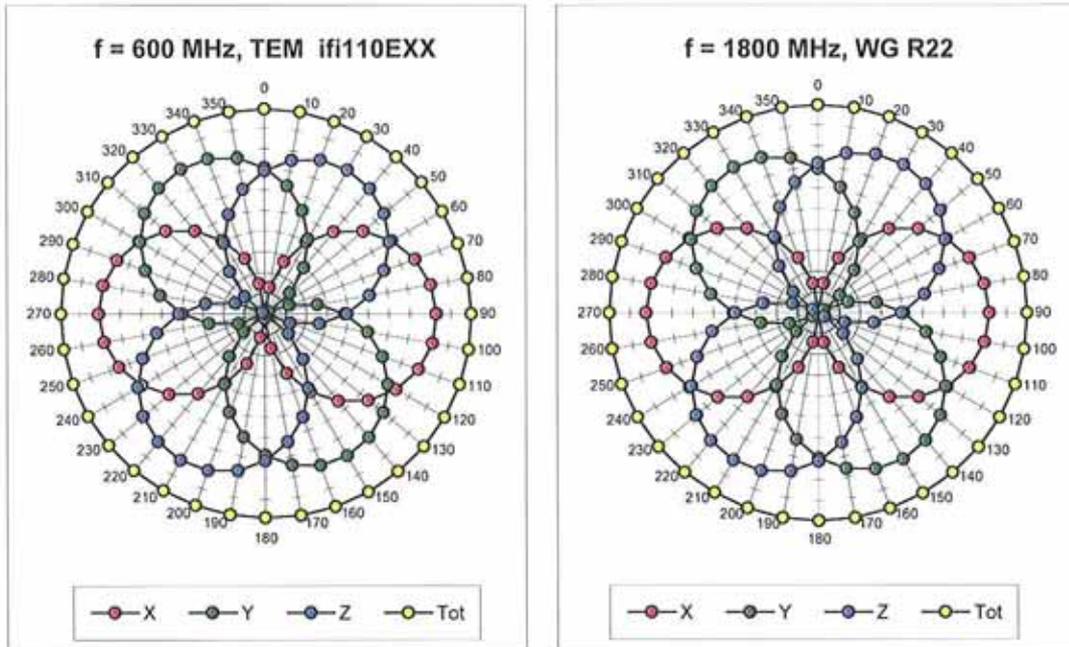



Uncertainty of Axial Isotropy Assessment: $\pm 0.5\%$ (k=2)

Dynamic Range $f(SAR_{head})$ (Waveguide R22, $f = 1800$ MHz)

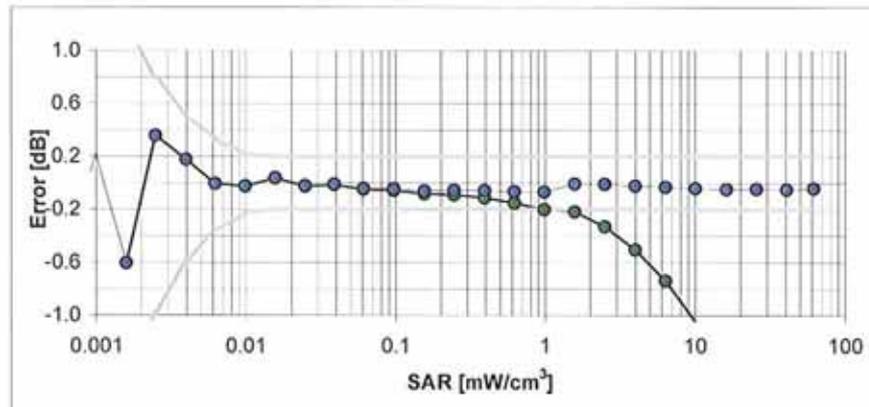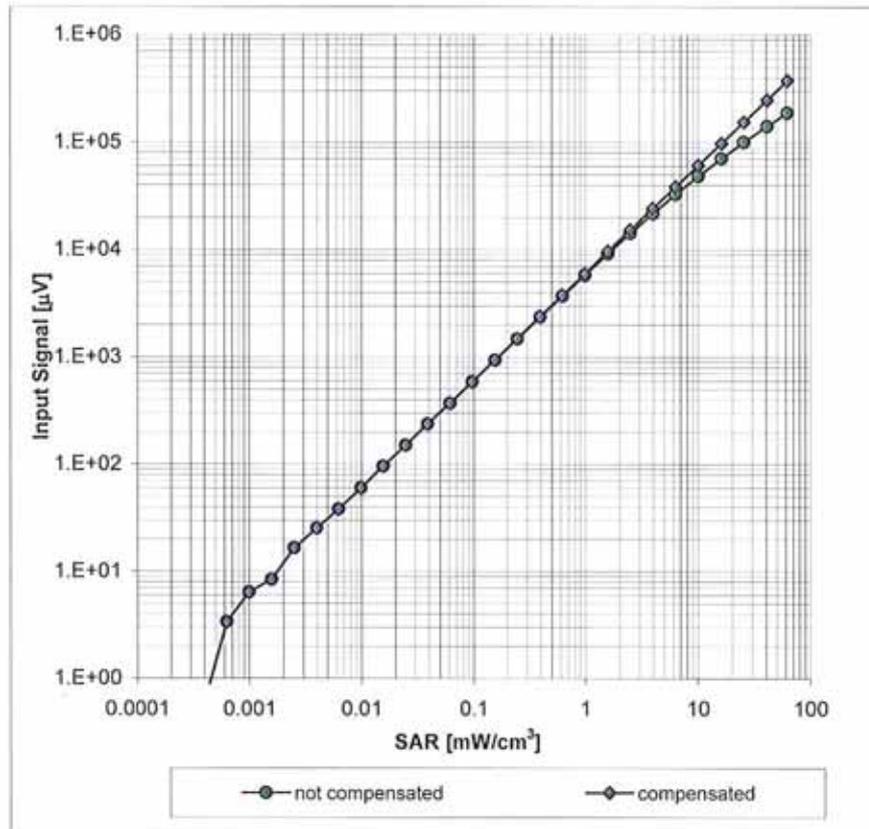


Uncertainty of Linearity Assessment: $\pm 0.6\%$ ($k=2$)

Conversion Factor Assessment

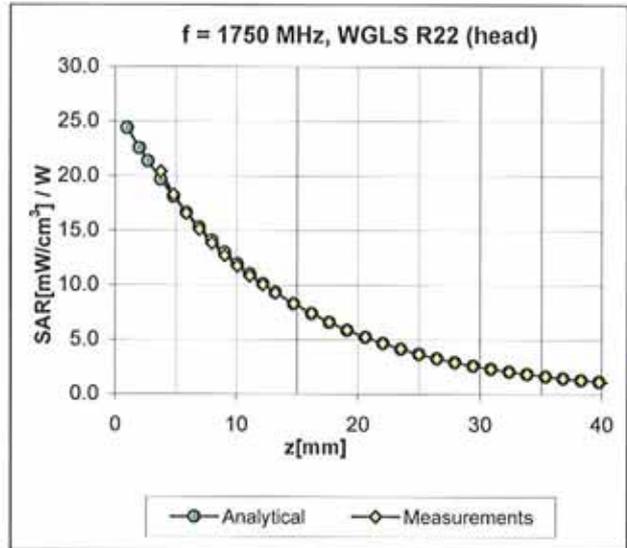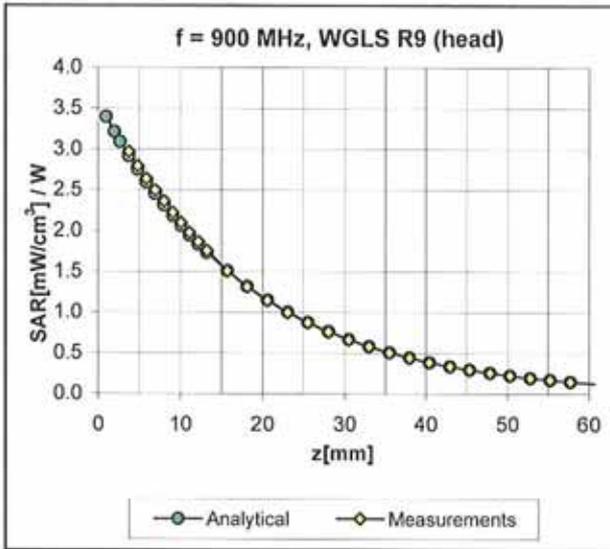

Deviation from Isotropy in HSL

Error (ϕ , θ), f = 900 MHz

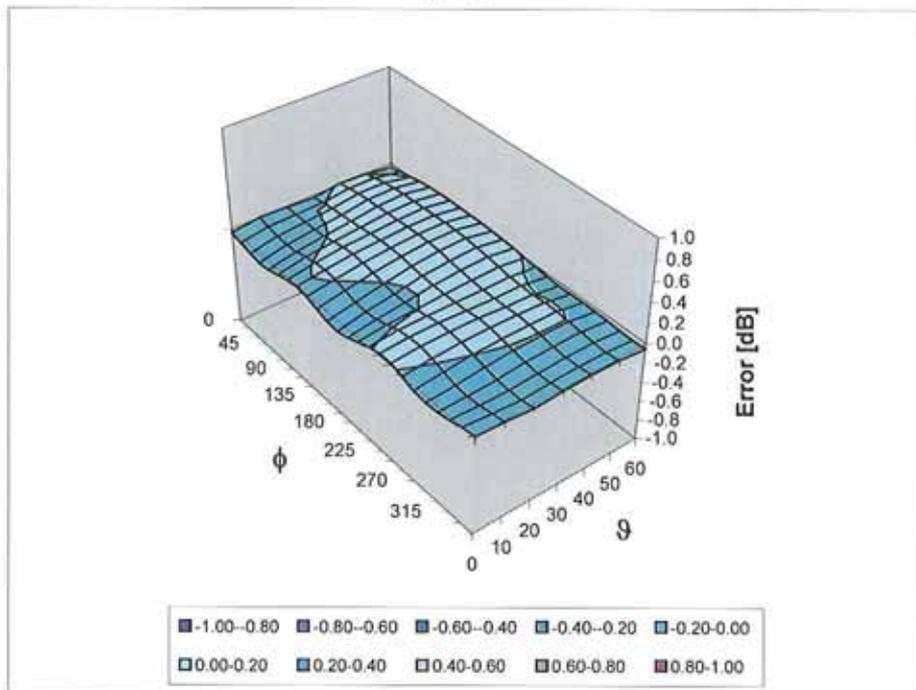

Uncertainty of Spherical Isotropy Assessment: $\pm 2.6\%$ (k=2)

Other Probe Parameters

| | |
|---|----------------|
| Sensor Arrangement | Triangular |
| Connector Angle (°) | Not applicable |
| Mechanical Surface Detection Mode | enabled |
| Optical Surface Detection Mode | enabled |
| Probe Overall Length | 337 mm |
| Probe Body Diameter | 10 mm |
| Tip Length | 10 mm |
| Tip Diameter | 6.8 mm |
| Probe Tip to Sensor X Calibration Point | 2.7 mm |
| Probe Tip to Sensor Y Calibration Point | 2.7 mm |
| Probe Tip to Sensor Z Calibration Point | 2.7 mm |
| Recommended Measurement Distance from Surface | 4 mm |



Attachment 4 – System Validation Dipole – D1900V2, S/N: 5d112 Calibration Data



Accredited by the Swiss Accreditation Service (SAS)
The Swiss Accreditation Service is one of the signatories to the EA
Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: **SCS 108**

Client **JQA (PTT)**

Certificate No: **D1900V2-5d112_Jul09**

CALIBRATION CERTIFICATE

Object: **D1900V2 - SN: 5d112**

Calibration procedure(s): **QA CAL-05.v7
Calibration procedure for dipole validation kits**

Calibration date: **July 14, 2009**

Condition of the calibrated item: **In Tolerance**

This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI).
The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility: environment temperature (22 ± 3)°C and humidity < 70%.

Calibration Equipment used (M&TE critical for calibration)

| Primary Standards | ID # | Cal Date (Calibrated by, Certificate No.) | Scheduled Calibration |
|-----------------------------|--------------------|---|------------------------|
| Power meter EPM-442A | GB37480704 | 08-Oct-08 (No. 217-00898) | Oct-09 |
| Power sensor HP 8481A | US37292783 | 08-Oct-08 (No. 217-00898) | Oct-09 |
| Reference 20 dB Attenuator | SN: 5086 (20g) | 31-Mar-09 (No. 217-01025) | Mar-10 |
| Type-N mismatch combination | SN: 5047.2 / 06327 | 31-Mar-09 (No. 217-01029) | Mar-10 |
| Reference Probe ES3DV2 | SN: 3025 | 30-Apr-09 (No. ES3-3025_Apr09) | Apr-10 |
| DAE4 | SN: 601 | 07-Mar-09 (No. DAE4-601_Mar09) | Mar-10 |
| Secondary Standards | ID # | Check Date (in house) | Scheduled Check |
| Power sensor HP 8481A | MY41092317 | 18-Oct-02 (in house check Oct-07) | In house check: Oct-09 |
| RF generator R&S SMT-06 | 100005 | 4-Aug-99 (in house check Oct-07) | In house check: Oct-09 |
| Network Analyzer HP 8753E | US37390585 S4206 | 18-Oct-01 (in house check Oct-08) | In house check: Oct-09 |

Calibrated by: **Name: Mike Meili, Function: Laboratory Technician, Signature: [Handwritten Signature]**

Approved by: **Name: Katja Pokovic, Function: Technical Manager, Signature: [Handwritten Signature]**

Issued: July 14, 2009

This calibration certificate shall not be reproduced except in full without written approval of the laboratory.



Accredited by the Swiss Accreditation Service (SAS)
The Swiss Accreditation Service is one of the signatories to the EA
Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: **SCS 108**

Glossary:

| | |
|-------|---------------------------------|
| TSL | tissue simulating liquid |
| ConvF | sensitivity in TSL / NORM x,y,z |
| N/A | not applicable or not measured |

Calibration is Performed According to the Following Standards:

- IEEE Std 1528-2003, "IEEE Recommended Practice for Determining the Peak Spatial-Averaged Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques", December 2003
- CENELEC EN 50361, "Basic standard for the measurement of Specific Absorption Rate related to human exposure to electromagnetic fields from mobile phones (300 MHz - 3 GHz), July 2001
- Federal Communications Commission Office of Engineering & Technology (FCC OET), "Evaluating Compliance with FCC Guidelines for Human Exposure to Radiofrequency Electromagnetic Fields; Additional Information for Evaluating Compliance of Mobile and Portable Devices with FCC Limits for Human Exposure to Radiofrequency Emissions", Supplement C (Edition 01-01) to Bulletin 65

Additional Documentation:

- DASY4/5 System Handbook

Methods Applied and Interpretation of Parameters:

- Measurement Conditions:** Further details are available from the Validation Report at the end of the certificate. All figures stated in the certificate are valid at the frequency indicated.
- Antenna Parameters with TSL:** The dipole is mounted with the spacer to position its feed point exactly below the center marking of the flat phantom section, with the arms oriented parallel to the body axis.
- Feed Point Impedance and Return Loss:** These parameters are measured with the dipole positioned under the liquid filled phantom. The impedance stated is transformed from the measurement at the SMA connector to the feed point. The Return Loss ensures low reflected power. No uncertainty required.
- Electrical Delay:** One-way delay between the SMA connector and the antenna feed point. No uncertainty required.
- SAR measured:** SAR measured at the stated antenna input power.
- SAR normalized:** SAR as measured, normalized to an input power of 1 W at the antenna connector.
- SAR for nominal TSL parameters:** The measured TSL parameters are used to calculate the nominal SAR result.

Measurement Conditions

DASY system configuration, as far as not given on page 1.

| | | |
|------------------------------|---------------------------|-------------|
| DASY Version | DASY5 | V5.0 |
| Extrapolation | Advanced Extrapolation | |
| Phantom | Modular Flat Phantom V5.0 | |
| Distance Dipole Center - TSL | 10 mm | with Spacer |
| Zoom Scan Resolution | dx, dy, dz = 5 mm | |
| Frequency | 1900 MHz \pm 1 MHz | |

Head TSL parameters

The following parameters and calculations were applied.

| | Temperature | Permittivity | Conductivity |
|----------------------------------|---------------------|----------------|----------------------|
| Nominal Head TSL parameters | 22.0 °C | 40.0 | 1.40 mho/m |
| Measured Head TSL parameters | (22.0 \pm 0.2) °C | 40.9 \pm 6 % | 1.43 mho/m \pm 6 % |
| Head TSL temperature during test | (22.0 \pm 0.2) °C | ---- | ---- |

SAR result with Head TSL

| SAR averaged over 1 cm ³ (1 g) of Head TSL | condition | |
|---|--------------------|--|
| SAR measured | 250 mW input power | 10.5 mW / g |
| SAR normalized | normalized to 1W | 42.0 mW / g |
| SAR for nominal Head TSL parameters ¹ | normalized to 1W | 41.7 mW / g \pm 17.0 % (k=2) |

| SAR averaged over 10 cm ³ (10 g) of Head TSL | Condition | |
|---|--------------------|--|
| SAR measured | 250 mW input power | 5.49 mW / g |
| SAR normalized | normalized to 1W | 22.0 mW / g |
| SAR for nominal Head TSL parameters ¹ | normalized to 1W | 21.9 mW / g \pm 16.5 % (k=2) |

¹ Correction to nominal TSL parameters according to d), chapter "SAR Sensitivities"

Body TSL parameters

The following parameters and calculations were applied.

| | Temperature | Permittivity | Conductivity |
|----------------------------------|-----------------|--------------|------------------|
| Nominal Body TSL parameters | 22.0 °C | 53.3 | 1.52 mho/m |
| Measured Body TSL parameters | (22.0 ± 0.2) °C | 53.5 ± 6 % | 1.55 mho/m ± 6 % |
| Body TSL temperature during test | (21.1 ± 0.2) °C | ---- | ---- |

SAR result with Body TSL

| SAR averaged over 1 cm ³ (1 g) of Body TSL | Condition | |
|---|--------------------|-----------------------------------|
| SAR measured | 250 mW input power | 10.6 mW / g |
| SAR normalized | normalized to 1W | 42.4 mW / g |
| SAR for nominal Body TSL parameters ² | normalized to 1W | 42.0 mW / g ± 17.0 % (k=2) |

| SAR averaged over 10 cm ³ (10 g) of Body TSL | condition | |
|---|--------------------|-----------------------------------|
| SAR measured | 250 mW input power | 5.60 mW / g |
| SAR normalized | normalized to 1W | 22.4 mW / g |
| SAR for nominal Body TSL parameters ² | normalized to 1W | 22.3 mW / g ± 16.5 % (k=2) |

² Correction to nominal TSL parameters according to d), chapter "SAR Sensitivities"

Appendix

Antenna Parameters with Head TSL

| | |
|--------------------------------------|-------------------------------|
| Impedance, transformed to feed point | 51.9 Ω + 7.6 $j\Omega$ |
| Return Loss | - 22.3 dB |

Antenna Parameters with Body TSL

| | |
|--------------------------------------|-------------------------------|
| Impedance, transformed to feed point | 46.6 Ω + 7.9 $j\Omega$ |
| Return Loss | - 21.0 dB |

General Antenna Parameters and Design

| | |
|----------------------------------|----------|
| Electrical Delay (one direction) | 1.204 ns |
|----------------------------------|----------|

After long term use with 100W radiated power, only a slight warming of the dipole near the feedpoint can be measured.

The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals.

No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feedpoint may be damaged.

Additional EUT Data

| | |
|-----------------|----------------|
| Manufactured by | SPEAG |
| Manufactured on | March 28, 2008 |

DASY5 Validation Report for Head TSL

Date/Time: 07.07.2009 16:04:52

Test Laboratory: SPEAG, Zurich, Switzerland

DUT: Dipole 1900 MHz; Type: D1900V2; Serial: D1900V2 - SN:5d112

Communication System: CW; Frequency: 1900 MHz; Duty Cycle: 1:1

Medium: HSL U11 BB

Medium parameters used: $f = 1900$ MHz; $\sigma = 1.43$ mho/m; $\epsilon_r = 40.9$; $\rho = 1000$ kg/m³

Phantom section: Flat Section

Measurement Standard: DASY5 (IEEE/IEC)

DASY5 Configuration:

- Probe: ES3DV2 - SN3025; ConvF(4.88, 4.88, 4.88); Calibrated: 30.04.2009
- Sensor-Surface: 3mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn601; Calibrated: 07.03.2009
- Phantom: Flat Phantom 5.0 (front); Type: QD000P50AA; Serial: 1001
- Measurement SW: DASY5, V5.0 Build 120; SEMCAD X Version 13.4 Build 45

**Pin = 250 mW; dip = 10 mm, scan at 3.0 mm/Zoom Scan (dist=3.0 mm, probe 0deg)
(7x7x7)/Cube 0:**


Measurement grid: dx=5mm, dy=5mm, dz=5mm

Reference Value = 98.2 V/m; Power Drift = 0.042 dB

Peak SAR (extrapolated) = 19.2 W/kg

SAR(1 g) = 10.5 mW/g; SAR(10 g) = 5.49 mW/g

Maximum value of SAR (measured) = 12.9 mW/g

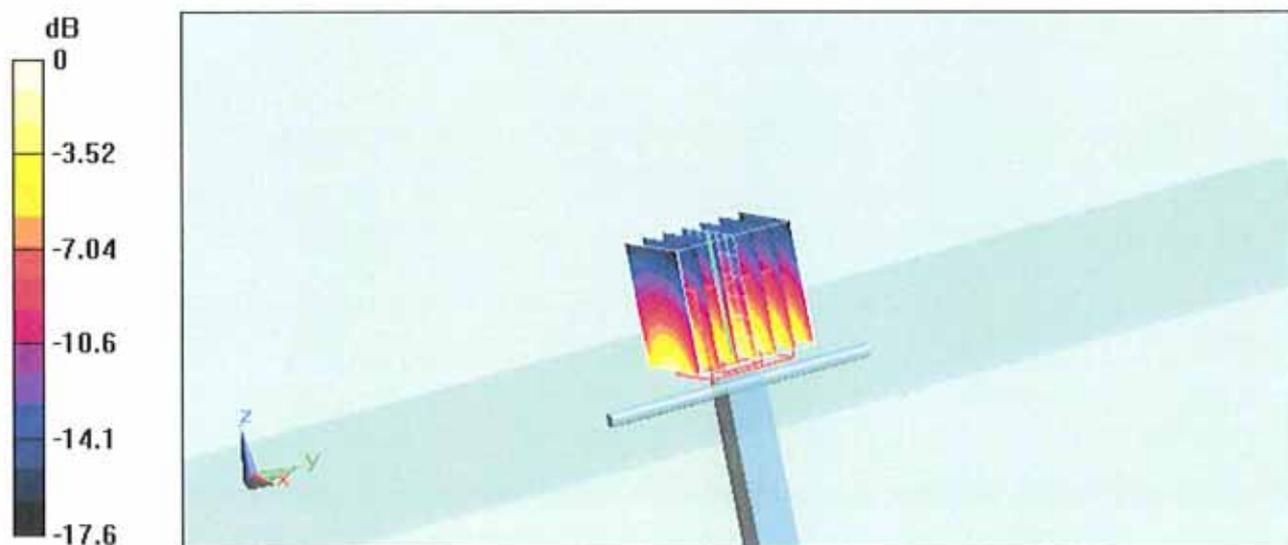

0 dB = 12.9mW/g

Impedance Measurement Plot for Head TSL

7 Jul 2009 11:07:19

CH1 S11 1 U FS


2: 51.881 Ω 7.6348 Ω 639.53 μH

1 900.000 000 MHz

*
De1
Cor

avg
16

↑

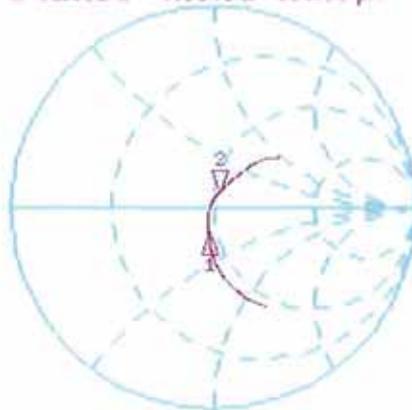

CH1 Markers

1: 46.078 Ω
-12.771 Ω
1.80000 GHz


CH2 S11 LOG 5 dB/REF -20 dB

2: -22.272 dB 1 900.000 000 MHz

Cor

avg
16

↑

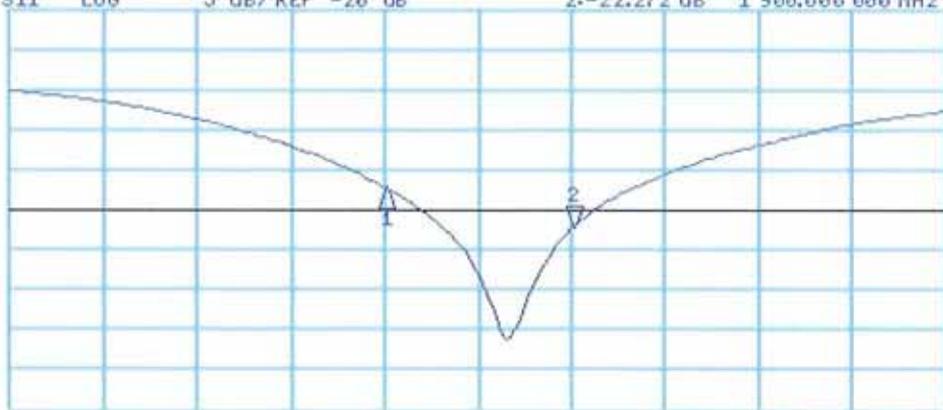

CH2 Markers

1: -17.214 dB
1.80000 GHz

START 1 600.000 000 MHz

STOP 2 100.000 000 MHz

DASY5 Validation Report for Body TSL

Date/Time: 14.07.2009 17:05:18

Test Laboratory: SPEAG, Zurich, Switzerland

DUT: Dipole 1900 MHz; Type: D1900V2; Serial: D1900V2 - SN:5d112

Communication System: CW; Frequency: 1900 MHz; Duty Cycle: 1:1

Medium: MSL U10 BB

Medium parameters used: $f = 1900$ MHz; $\sigma = 1.55$ mho/m; $\epsilon_r = 53.6$; $\rho = 1000$ kg/m³

Phantom section: Flat Section

Measurement Standard: DASY5 (IEEE/IEC)

DASY5 Configuration:

- Probe: ES3DV2 - SN3025; ConvF(4.46, 4.46, 4.46); Calibrated: 30.04.2009
- Sensor-Surface: 3mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn601; Calibrated: 07.03.2009
- Phantom: Flat Phantom 5.0 (back); Type: QD000P50AA; Serial: 1002
- Measurement SW: DASY5, V5.0 Build 120; SEMCAD X Version 13.4 Build 45

**Pin = 250 mW; dip = 10 mm, scan at 3.0mm/Zoom Scan (dist=3.0mm, probe 0deg)
(7x7x7)/Cube 0:**


Measurement grid: dx=5mm, dy=5mm, dz=5mm

Reference Value = 97.1 V/m; Power Drift = -0.00971 dB

Peak SAR (extrapolated) = 18.8 W/kg

SAR(1 g) = 10.6 mW/g; SAR(10 g) = 5.6 mW/g

Maximum value of SAR (measured) = 13.5 mW/g

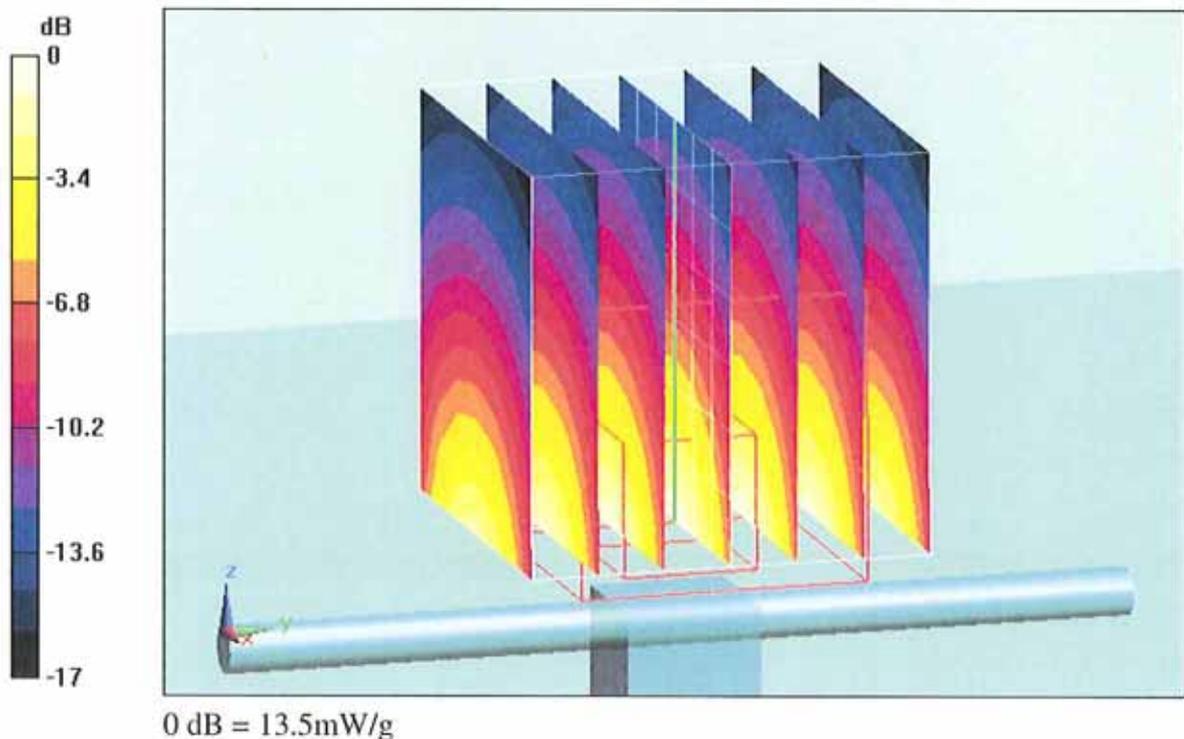


Impedance Measurement Plot for Body TSL

14 Jul 2009 11:52:04

[CH1] S11 1 U FS 1: 46.635 Ω 7.9199 Ω 663.42 μH 1 900.000 000 MHz

De 1
Ca

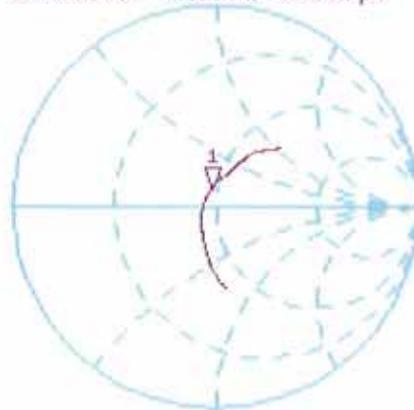

avg
16


↑

CH2 S11 LOG 5 dB/REF -20 dB 1: -21.034 dB 1 900.000 000 MHz

De 1
Ca

avg
16

↑

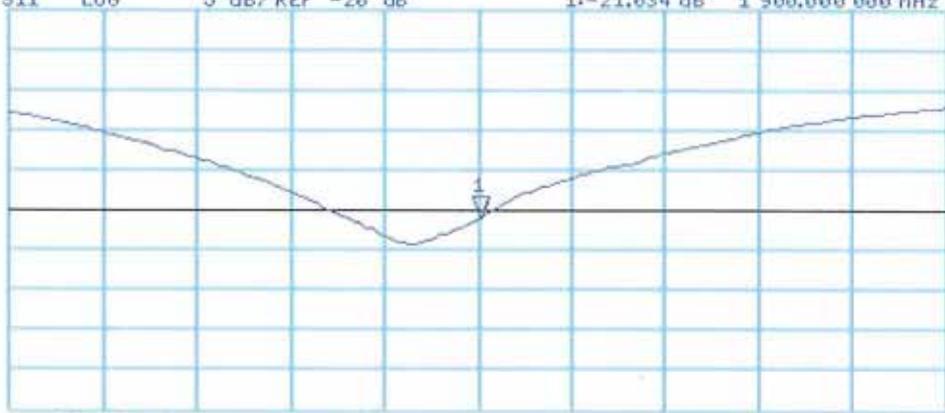

CENTER 1 900.000 000 MHz

SPAN 400.000 000 MHz