

2.17 WLAN 5000MHZ BODY SAR TEST RESULTS AND COURSE AREA SCANS – 2D

SYSTEM / SOFTWARE:	SARA-C / v6.08.11	INPUT POWER DRIFT:	0 dB
DATE / TIME:	08/10/2013-12:35:40	DUT BATTERY MODEL/NO:	n/a
AMBIENT TEMPERATURE:	23.30°C	LIQUID SIMULANT:	5000Body
DEVICE UNDER TEST:	SHL23	RELATIVE PERMITTIVITY:	48.71
RELATIVE HUMIDITY:	54.70%	CONDUCTIVITY:	5.538
PHANTOM S/NO:	IXB-2HF	LIQUID TEMPERATURE:	22.80°C
PHANTOM ROTATION:	N/A	MAX SAR Y-AXIS LOCATION:	-41.50mm
DUT POSITION:	10mm-Front Facing	MAX SAR Z-AXIS LOCATION:	-46.20mm
ANTENNA CONFIGURATION:	N/A	MAX E FIELD:	2.752
TEST FREQUENCY:	5520.0MHz	SAR 1g:	0.039 W/kg
TYPE OF MODULATION:	WLAN(DSSS)	SAR 10g:	N/A
MODN. DUTY CYCLE:	100%	SAR START:	0.056 W/kg
INPUT POWER LEVEL:	16dBm	SAR END:	0.056 W/kg
PROBE BATTERY LAST CHANGED:	08/10/2013	SAR DRIFT DURING SCAN:	0.000 %

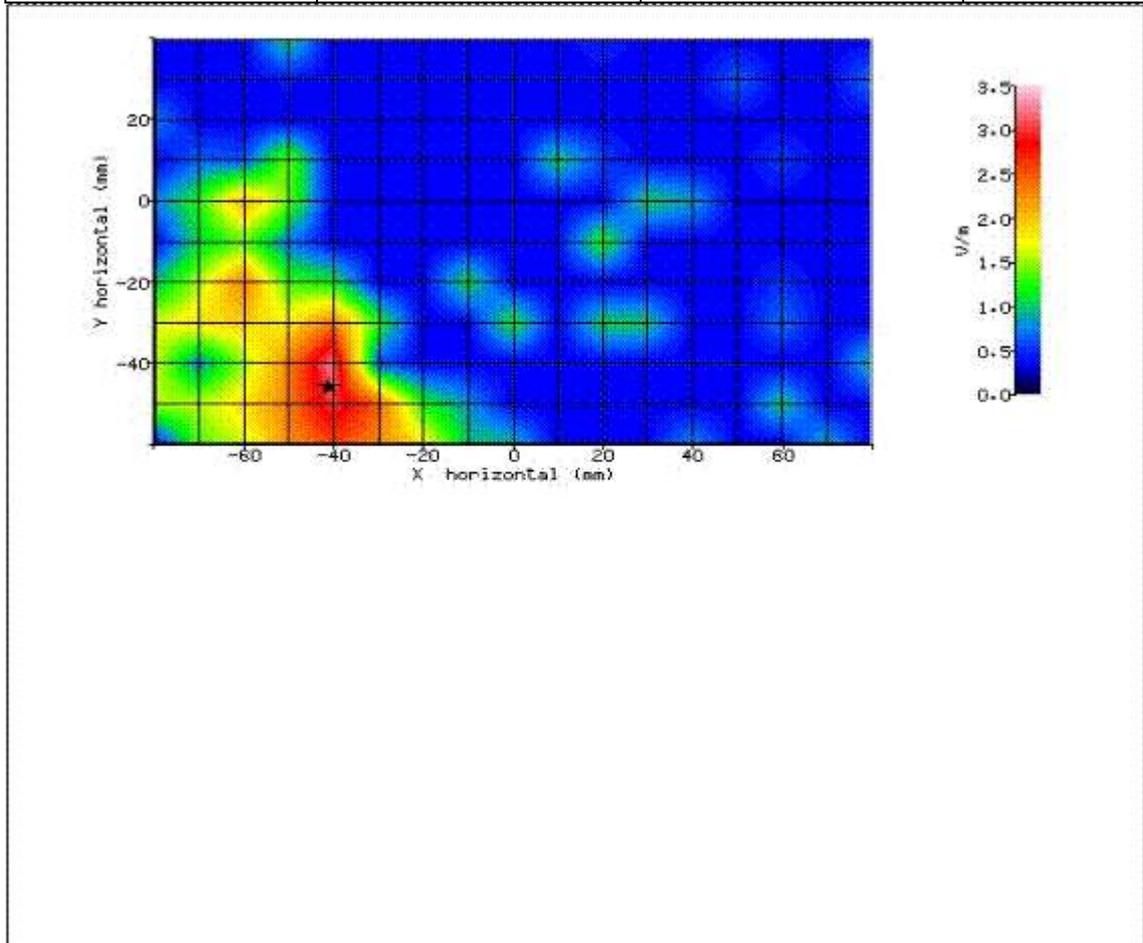


Figure 70: SAR Head Testing Results for the SHL23 Mobile Handset at 5520.0MHz. (NUA)

SYSTEM / SOFTWARE:	SARA-C / v6.08.11	INPUT POWER DRIFT:	0 dB
DATE / TIME:	08/10/2013-12:49:02	DUT BATTERY MODEL/NO:	n/a
AMBIENT TEMPERATURE:	23.30°C	LIQUID SIMULANT:	5000Body
DEVICE UNDER TEST:	SHL23	RELATIVE PERMITTIVITY:	48.71
RELATIVE HUMIDITY:	54.70%	CONDUCTIVITY:	5.538
PHANTOM S/NO:	IXB-2HF	LIQUID TEMPERATURE:	22.80°C
PHANTOM ROTATION:	N/A	MAX SAR X-AXIS LOCATION:	-38.90mm
DUT POSITION:	10mm-Rear Facing	MAX SAR Y-AXIS LOCATION:	34.30mm
ANTENNA CONFIGURATION:	N/A	MAX E FIELD:	7.075
TEST FREQUENCY:	5520.0MHz	SAR 1g:	0.291 W/kg
TYPE OF MODULATION:	WLAN(DSSS)	SAR 10g:	N/A
MODN. DUTY CYCLE:	100%	SAR START:	0.466 W/kg
INPUT POWER LEVEL:	16dBm	SAR END:	0.471 W/kg
PROBE BATTERY LAST CHANGED:	08/10/2013	SAR DRIFT DURING SCAN:	1.000 %

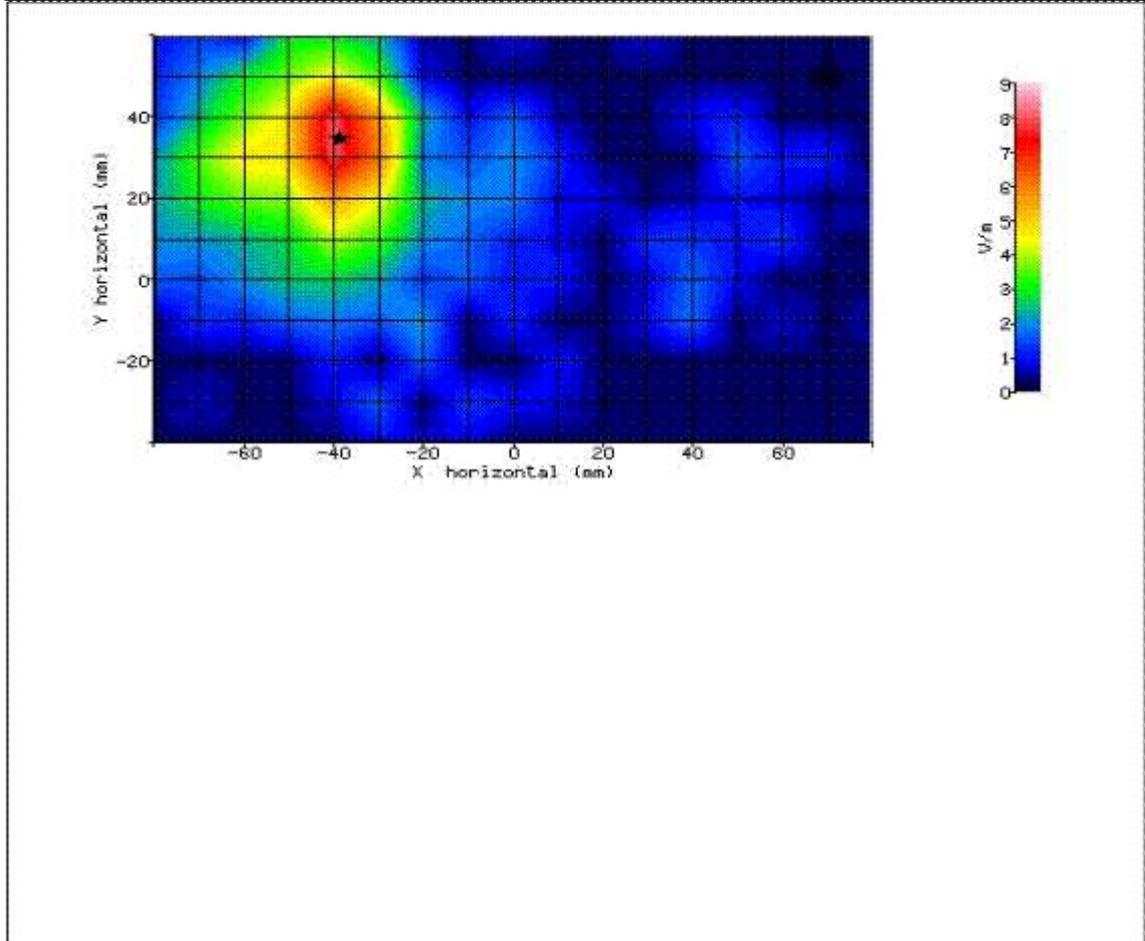


Figure 71: SAR Body Testing Results for the SHL23 Mobile Handset at 5520.0MHz. (NUA)

SYSTEM / SOFTWARE:	SARA-C / v6.08.11	INPUT POWER DRIFT:	0 dB
DATE / TIME:	08/10/2013-13:01:55	DUT BATTERY MODEL/NO:	n/a
AMBIENT TEMPERATURE:	23.30°C	LIQUID SIMULANT:	5000Body
DEVICE UNDER TEST:	SHL23	RELATIVE PERMITTIVITY:	48.71
RELATIVE HUMIDITY:	54.70%	CONDUCTIVITY:	5.538
PHANTOM S/NO:	IXB-2HF	LIQUID TEMPERATURE:	22.80°C
PHANTOM ROTATION:	N/A	MAX SAR X-AXIS LOCATION:	-41.40mm
DUT POSITION:	10mm-Right Edge	MAX SAR Y-AXIS LOCATION:	-7.50mm
ANTENNA CONFIGURATION:	N/A	MAX E FIELD:	6.229
TEST FREQUENCY:	5520.0MHz	SAR 1g:	0.219 W/kg
TYPE OF MODULATION:	WLAN(DSSS)	SAR 10g:	N/A
MODN. DUTY CYCLE:	100%	SAR START:	0.341 W/kg
INPUT POWER LEVEL:	16dBm	SAR END:	0.342 W/kg
PROBE BATTERY LAST CHANGED:	08/10/2013	SAR DRIFT DURING SCAN:	0.300 %

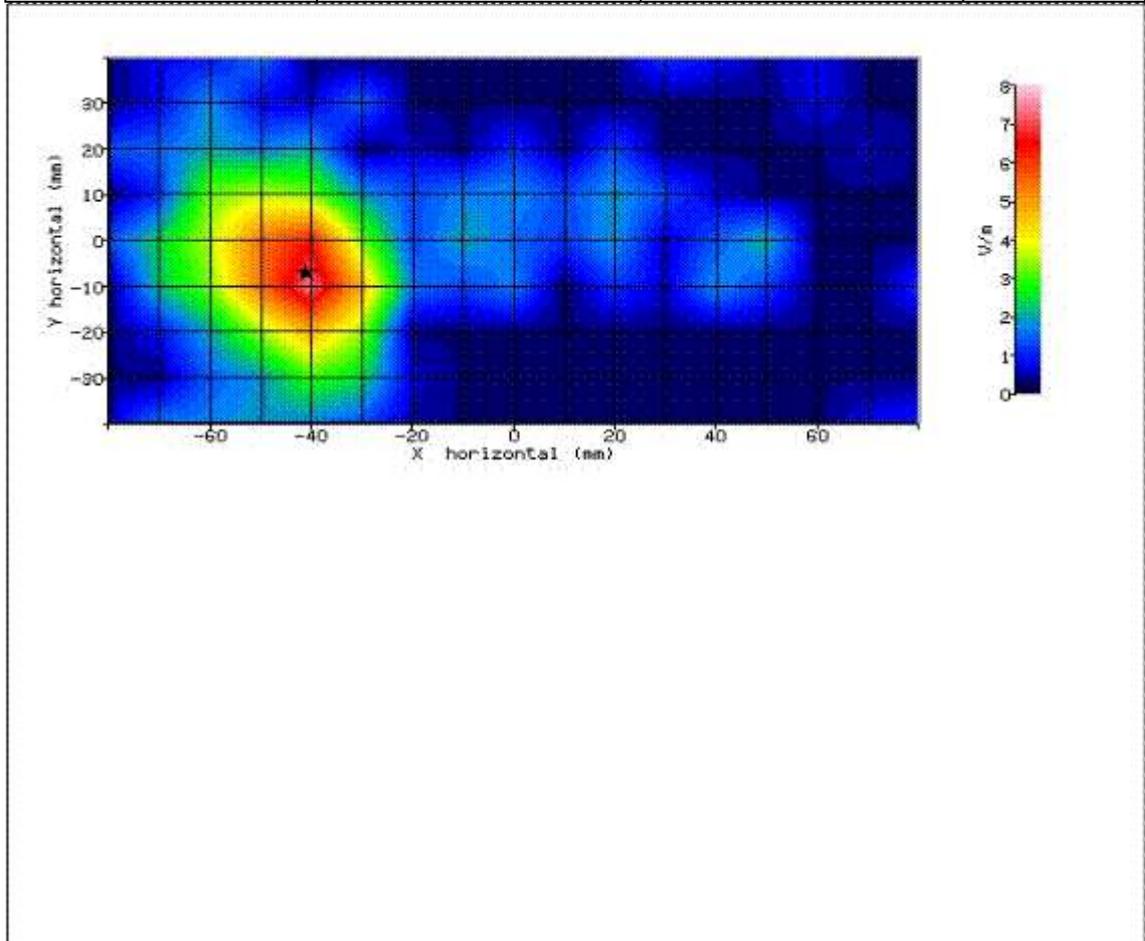


Figure 72: SAR Body Testing Results for the SHL23 Mobile Handset at 5520.0MHz. (NUA)

SYSTEM / SOFTWARE:	SARA-C / v6.08.11	INPUT POWER DRIFT:	0 dB
DATE / TIME:	08/10/2013-13:15:35	DUT BATTERY MODEL/NO:	n/a
AMBIENT TEMPERATURE:	23.30°C	LIQUID SIMULANT:	5000Body
DEVICE UNDER TEST:	SHL23	RELATIVE PERMITTIVITY:	48.71
RELATIVE HUMIDITY:	54.70%	CONDUCTIVITY:	5.538
PHANTOM S/NO:	IXB-2HF	LIQUID TEMPERATURE:	22.80°C
PHANTOM ROTATION:	N/A	MAX SAR X-AXIS LOCATION:	17.90mm
DUT POSITION:	10mm-Top Edge	MAX SAR Y-AXIS LOCATION:	-6.80mm
ANTENNA CONFIGURATION:	N/A	MAX E FIELD:	1.989
TEST FREQUENCY:	5520.0MHz	SAR 1g:	0.016 W/kg
TYPE OF MODULATION:	WLAN(DSSS)	SAR 10g:	N/A
MODN. DUTY CYCLE:	100%	SAR START:	0.032 W/kg
INPUT POWER LEVEL:	16dBm	SAR END:	0.032 W/kg
PROBE BATTERY LAST CHANGED:	08/10/2013	SAR DRIFT DURING SCAN:	0.000 %

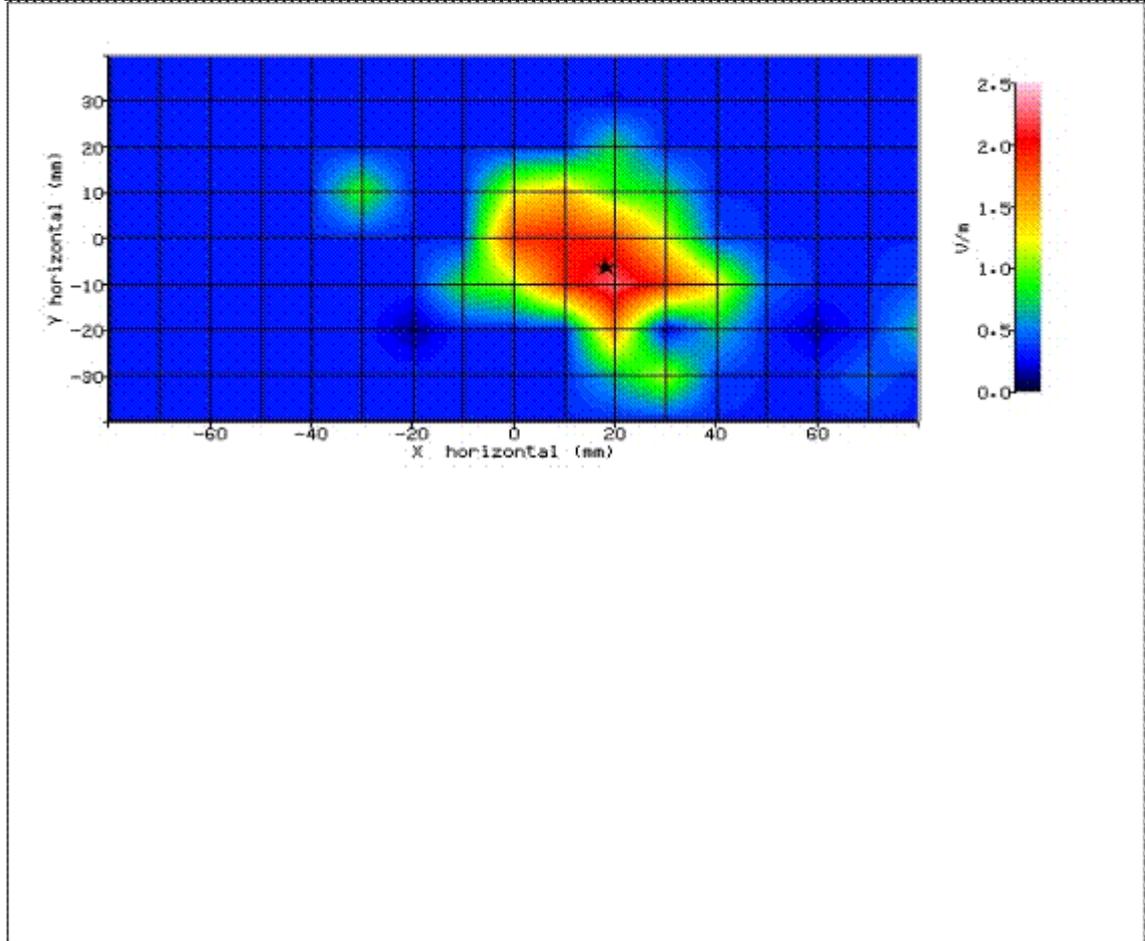


Figure 73: SAR Body Testing Results for the SHL23 Mobile Handset at 5520.0MHz. (NUA)



Product Service

SECTION 3

TEST EQUIPMENT USED



3.1 TEST EQUIPMENT USED

The following test equipment was used at TÜV SÜD Product Service:

Instrument Description	Manufacturer	Model Type	TE Number	Cal Period (months)	Calibration Due Date
Signal Generator	Hewlett Packard	ESG4000A	38	12	23-May-2014
Radiocommunications Tester	Rohde & Schwarz	CMU 200	39	12	21-Dec-2013
10MHz - 2.5GHz, 3W, Amplifier	Vectawave Technology	VTL5400	51	-	TU
Directional Coupler	Krytar	1850	58	-	TU
Power Sensor	Rohde & Schwarz	NRV-Z1	60	12	14-Jun-2014
Signal Generator	Hewlett Packard	ESG4000A	61	12	22-May-2014
Thermometer	Digitron	T208	64	12	16-Jan-2014
Amplifier (5GHz)	IndexSar Ltd	5GHz	157	-	TU
Attenuator (Step, 11dB, 1W)	Hewlett Packard	8494H	425	-	TU
Directional Coupler	Hewlett Packard	11692D	452	-	TU
Attenuator (20dB, 10W)	Weinschel	37-20-34	482	12	11-Oct-2013
Attenuator (20dB, 20W)	Narda	766F-20	483	12	13-Jun-2014
Spectrum Analyser	Agilent Technologies	E7405A	1410	12	27-Sep-2014
Validation Amplifier (10MHz - 2.5GHz)	IndexSar Ltd	VBM2500-3	2415	-	TU
Hygrometer	Rotronic	I-1000	2784	12	3-Apr-2014
GSM Test Set	Rohde & Schwarz	CMU 200	2809	12	18-Jun-2014
Power Sensor	Rohde & Schwarz	NRV- Z5	2878	12	14-Jun-2014
Antenna (Omnidirectional)	Katherin Scala Division	OG-890/1990/DC	2905	-	TU
Power Meter	Rohde & Schwarz	NRVD	2979	12	25-May-2014
Dual Channel Power Meter	Rohde & Schwarz	NRVD	3259	12	14-Jun-2014
Signal Generator: 10MHz to 20GHz	Rohde & Schwarz	SMR20	3475	12	1-Feb-2014
Power Sensor	Rohde & Schwarz	NRV-Z1	3563	12	23-May-2014
Meter & T/C	R.S Components	Meter 615-8206 & Type K T/C	3612	12	8-Jul-2014
SAR 1800 MHz dipole	Speag	D1800V2	3855	-	O/P Mon
SAR 900 MHz dipole	Speag	D900V2	3856	-	O/P Mon
SAR 835 MHz dipole	Speag	D835V2	3857	-	O/P Mon
Part of SARAC System	IndexSar Ltd	Robot Controller	4076	-	TU
Part of SARAC System	IndexSar Ltd	Cartesian Leg Extension	4078	-	TU
Cartesian 4-axis Robot	IndexSar Ltd	SARAC	4079	-	TU
Part of SARAC System	IndexSar Ltd	Wooden Bench	4081	-	TU
Wideband Radio Communication Tester	Rohde & Schwarz	CMW 500	4144	12	17-Jul-2014
Head Phantom	IndexSar Ltd	IXB-040 Inverted SAM phantom	4254	-	TU
Flat Phantom	IndexSar Ltd	IXB-2HF 800-6000MHz	4255	-	TU
Flat Phantom	IndexSar Ltd	IXB-2HF 800-6000MHz	4256	-	TU
Spacer used to raise body phantom	IndexSar Ltd	Body Phantom Spacer	4260	-	TU
Part of SARAC System	IndexSar Ltd	Wooden Bench	4266	-	TU
Part of SARAC System	IndexSar Ltd	Robot Controller	4267	-	TU
Part of SARAC System	IndexSar Ltd	Cartesian Leg Extension	4268	-	TU
Cartesian 4-axis Robot	IndexSar Ltd	SARAC	4269	-	TU



Product Service

Instrument Description	Manufacturer	Model Type	TE Number	Cal Period (months)	Calibration Due Date
Digital thermo Hygrometer	Radio Spares	1260	4300	12	22-Mar-2014
SAR 5GHz Di-pole	Speag	D5GHzV2	4309	-	TU
Immersible SAR Probe	IndexSar Ltd	IXP-025	4310	24	28-Nov-2013
Immersible SAR Probe	IndexSar Ltd	IXP-021	4311	24	24-Oct-2014
Immersible SAR Probe	IndexSar Ltd	IPX-050	4313	24	7-Mar-2015
Immersible SAR Probe	IndexSar Ltd	IPX-020	4317	24	24-Apr-2015
Immersible SAR Probe	IndexSar Ltd	IPX-020	4318	24	24-Apr-2015
835MHz Head Fluid	TUV SUD Product Service	Batch 19	N/A	1	31-Oct-2013
835MHz Body Fluid	TUV SUD Product Service	Batch 13	N/A	1	31-Oct-2013
1900MHz Head Fluid	TUV SUD Product Service	Batch 8	N/A	1	31-Oct-2013
1900MHz Body Fluid	TUV SUD Product Service	Batch 4	N/A	1	31-Oct-2013
2450MHz Head Fluid	TUV SUD Product Service	Batch 10	N/A	1	31-Oct-2013
2450MHz Body Fluid	TUV SUD Product Service	Batch 7	N/A	1	31-Oct-2013
5200MHz Head Fluid	TUV SUD Product Service	Batch 3	N/A	1	31-Oct-2013
5200MHz Body Fluid	TUV SUD Product Service	Batch 2	N/A	1	31-Oct-2013

TU – Traceability Unscheduled



3.2 TEST SOFTWARE

The following software was used to control the TÜV SÜD Product Service SARAC System.

Instrument	Version Number	Date
SARA-C system	v.6.08.11	06 June 2013
IFA-10 Probe amplifier	Version 2	-



3.3 DIELECTRIC PROPERTIES OF SIMULANT LIQUIDS

The fluid properties of the simulant fluids used during routine SAR evaluation meet the dielectric properties required KDB 865665.

IEEE 1528 Recipes

Frequency (MHz)	300			450			835			900			1450			1800					1900		1950	2000	2100		2450			3000
Recipe#	1	1	3	1			1	2	3	1	1	2	2	3	1	2	4	1	1	2	2	3	2	2	3	2				
Ingredients (% by weight)																														
1, 2-Propanediol						64.81																								
Bactericide	0.19	0.19	0.50	0.10	0.10		0.50																				0.50			
Diacetin			48.90				49.20																				49.45			
DGBE								45.41	47.00	13.84	44.92			44.94	13.84	45.00	50.00	50.00	7.99	7.99							7.99			
HEC	0.98	0.96		1.00	1.00																									
NaCl	5.95	3.95	1.70	1.45	1.48	0.79	1.10	0.67	0.36	0.35	0.18	0.64	0.18	0.35											0.16	0.16		0.16		
Sucrose	55.32	56.32		57.00	56.50																									
Triton X-100											30.45			30.45										19.97	19.97			19.97		
Water	37.56	38.56	48.90	40.45	40.92	34.40	49.20	53.80	52.64	55.36	54.90	49.43	54.90	55.36	55.00	50.00	50.00	50.00	71.88	71.88	49.75	71.88					71.88			
Measured dielectric parameters																														
ϵ_r	46.00	43.40	44.30	41.60	41.20	41.80	42.70	40.9	39.3	41.00	40.40	39.20	39.90	41.00	40.10	37.00	36.80	41.10	40.30	39.20	37.90									
σ (S/m)	0.86	0.85	0.90	0.90	0.98	0.97	0.99	1.21	1.39	1.38	1.40	1.40	1.42	1.38	1.41	1.40	1.51	1.55	1.88	1.82	2.46									
Temp (°C)	22	22	20	22	22	22	20	22	22	21	22	20	21	21	20	22	22	20	20	20	20									
Target dielectric parameters (Table 2)																														
ϵ_r	45.30	43.50	41.5	41.50	40.50					40.00								39.80	39.20	38.50										
σ (S/m)	0.87	0.87	0.9	0.97	1.20					1.40								1.49	1.80	2.40										

NOTE – Multiple columns for any single frequency are optional recipe #, reference: 1 (Kanda et al. [B185]), 2 (Vigneras [B143]), 3 (Peyman and Gabriel [B119]), 4 (Fukunaga et al [B50])

The dielectric properties of the tissue simulant liquids used for the SAR testing at TÜV SÜD Product Service are as follows:-

Fluid Type and Frequency	Relative Permittivity ϵ_R (ϵ') Target	Relative Permittivity ϵ_R (ϵ') Measured	Conductivity σ Target	Conductivity σ Measured
835MHz Head	41.5	42.69	0.90	0.913
835MHz Body	55.0	56.99	0.97	1.015
1900MHz Head	40.0	40.08	1.40	1.447
1900MHz Body	53.3	53.64	1.52	1.497
2450 MHz Head	39.2	37.68	1.8	1.813
2450MHz Body	52.7	51.57	1.95	1.962
5200MHz Head	36.0	35.35	4.66	4.556
5200MHz Body	49.0	49.57	5.30	5.091
5500MHz Head	35.6	34.52	4.96	4.896
5500MHz Body	48.6	48.71	5.65	5.538



Product Service

3.4 TEST CONDITIONS

3.4.1 Test Laboratory Conditions

Ambient temperature: Within +15°C to +35°C.

The actual temperature during the testing ranged from 22.5°C to 69.3°C.

The actual humidity during the testing ranged from 22.8% to 68.6% RH.

3.4.2 Test Fluid Temperature Range

Frequency	Body / Head Fluid	Min Temperature °C	Max Temperature °C
835MHz	Head	22.8	22.8
835MHz	Body	22.6	22.6
1900MHz	Head	22.8	22.8
1900MHz	Body	22.4	22.4
2450MHz	Head	22.6	22.6
2450MHz	Body	22.7	22.7
5200MHz	Head	22.9	22.9
5200MHz	Body	22.8	22.8
5500MHz	Head	23.0	23.0
5500MHz	Body	22.8	22.8

3.4.3 SAR Drift

The SAR Drift was within acceptable limits during scans. The maximum SAR Drift, drift due to the handset electronics, was recorded as 8.2% (1.085 dB) for all of the testing. The measurement uncertainty budget for this assessment includes the maximum SAR Drift figures for Head and/or Body as applicable.



3.5 MEASUREMENT UNCERTAINTY

Head SAR Measurements.

Source of Uncertainty	Description	Tolerance / Uncertainty ± %	Probability distribution	Div	C_i (1g)	Standard Uncertainty ± % (1g)	V_i or V_{eff}
<i>Measurement System</i>							
Probe calibration	7.2.1	8.73	N	1	1	8.73	∞
Isotropy	7.2.1.2	3.18	R	1.73	1	1.84	∞
Probe angle >30deg	additional	12.00	R	1.73	1	6.93	∞
Boundary effect	7.2.1.5	0.49	R	1.73	1	0.28	∞
Linearity	7.2.1.3	1.00	R	1.73	1	0.58	∞
Detection limits	7.2.1.4	0.00	R	1.73	1	0.00	∞
Readout electronics	7.2.1.6	0.30	N	1	1	0.30	∞
Response time	7.2.1.7	0.00	R	1.73	1	0.00	∞
Integration time (equiv.)	7.2.1.8	1.38	R	1.73	1	0.80	∞
RF ambient conditions	7.2.3.6	3.00	R	1.73	1	1.73	∞
Probe positioner mech. restrictions	7.2.2.1	5.35	R	1.73	1	3.09	∞
Probe positioning with respect to phantom shell	7.2.2.3	5.00	R	1.73	1	2.89	∞
Post-processing	7.2.4	7.00	R	1.73	1	4.04	∞
<i>Test sample related</i>							
Test sample positioning	7.2.2.4	1.50	R	1.73	1	0.87	∞
Device holder uncertainty	7.2.2.4.2	1.73	R	1.73	1	1.00	∞
Drift of output power	7.2.3.4	8.2	R	1.73	1	4.73	∞
<i>Phantom and set-up</i>							
Phantom uncertainty (shape and thickness tolerances)	7.2.2.2	2.01	R	1.73	1	1.16	∞
Liquid conductivity (target)	7.2.3.3	5.00	R	1.73	0.64	1.85	∞
Liquid conductivity (meas.)	7.2.3.3	5.00	N	1	0.64	3.20	∞
Liquid permittivity (target)	7.2.3.4	5.00	R	1.73	0.6	1.73	∞
Liquid permittivity (meas.)	7.2.3.4	3.00	N	1	0.6	1.80	∞
Combined standard uncertainty			RSS			11.27	
Expanded uncertainty (95% confidence interval)			K=2			22.53	



Body SAR Measurements.

Source of Uncertainty	Description	Tolerance / Uncertainty ± %	Probability distribution	Div	c_i (1g)	Standard Uncertainty ± % (1g)	V_i or V_{eff}
<i>Measurement System</i>							
Probe calibration	7.2.1	8.73	N	1	1	8.73	∞
Isotropy	7.2.1.2	3.18	R	1.73	1	1.84	∞
Boundary effect	7.2.1.5	0.49	R	1.73	1	0.28	∞
Linearity	7.2.1.3	1.00	R	1.73	1	0.58	∞
Detection limits	7.2.1.4	0.00	R	1.73	1	0.00	∞
Readout electronics	7.2.1.6	0.30	N	1	1	0.30	∞
Response time	7.2.1.7	0.00	R	1.73	1	0.00	∞
Integration time (equiv.)	7.2.1.8	1.38	R	1.73	1	0.80	∞
RF ambient conditions	7.2.3.6	3.00	R	1.73	1	1.73	∞
Probe positioner mech. restrictions	7.2.2.1	0.60	R	1.73	1	0.35	∞
Probe positioning with respect to phantom shell	7.2.2.3	2.00	R	1.73	1	1.15	∞
Post-processing	7.2.4	7.00	R	1.73	1	4.04	∞
<i>Test sample related</i>							
Test sample positioning	7.2.2.4	1.50	R	1.73	1	0.87	∞
Device holder uncertainty	7.2.2.4.2	1.73	R	1.73	1	1.00	∞
Drift of output power	7.2.3.4	5.2	R	1.73	1	3.00	∞
<i>Phantom and set-up</i>							
Phantom uncertainty (shape and thickness tolerances)	7.2.2.2	2.01	R	1.73	1	1.16	∞
Liquid conductivity (target)	7.2.3.3	5.00	R	1.73	0.64	1.85	∞
Liquid conductivity (meas.)	7.2.3.3	5.00	N	1	0.64	3.20	∞
Liquid permittivity (target)	7.2.3.4	5.00	R	1.73	0.6	1.73	∞
Liquid permittivity (meas.)	7.2.3.4	3.00	N	1	0.6	1.80	∞
Combined standard uncertainty			RSS			10.42	
Expanded uncertainty (95% confidence interval)			K=2			20.84	



SECTION 4

ACCREDITATION, DISCLAIMERS AND COPYRIGHT



4.1 ACCREDITATION, DISCLAIMERS AND COPYRIGHT



This report relates only to the actual item/items tested.

Our UKAS Accreditation does not cover opinions and interpretations and any expressed are outside the scope of our UKAS Accreditation.

Results of tests not covered by our UKAS Accreditation Schedule are marked NUA (Not UKAS Accredited).

This report must not be reproduced, except in its entirety, without the written permission of TÜV SÜD Product Service

© 2013 TÜV SÜD Product Service



Product Service

ANNEX A

PROBE CALIBRATION REPORT



Product Service



NATIONAL PHYSICAL LABORATORY

Teddington Middlesex UK TW11 0LW Telephone +44 20 8977 3222

Certificate of Calibration

SAR PROBE

IndexSAR

Model: IXP-050

Serial number: 0170

This certificate provides traceability of measurement to recognised national standards, and to the units of measurement realised at the National Physical Laboratory or other recognised national standards laboratories. This certificate may not be reproduced other than in full, unless permission for the publication of an approved extract has been obtained in writing from the Managing Director. It does not of itself impute to the subject of calibration any attributes beyond those shown by the data contained herein.

FOR: Indexsar Ltd.
Oakfield House
Cudworth Lane
Newdigate
Surrey
RH5 5BG

DESCRIPTION: An IndexSAR isotropic electric field probe for determining specific absorption rates (SAR) in dielectric liquids. The probe has three orthogonal sensors, and the output voltage of the sensors is converted to an optical signal by a meter unit containing an analogue to digital (AD) converter. Probe readings are obtained using software via the RS232 port. The probe was calibrated with IndexSAR amplifier model IXA-010 S/N 036 belonging to NPL.

IDENTIFICATION: The probe is marked with the manufacturer's serial number 0170

MEASUREMENTS COMPLETED ON: 1 March 2012

The reported uncertainty is based on a coverage factor $k = 2$, providing a level of confidence of approximately 95%

Reference : 2012020074-1

Date of Issue : 1 March 2012

Checked by : BGL

Page 1 of 7

Signed : B. Loader (Authorised Signatory)

Name : Mr B G Loader on behalf of NPLML



NATIONAL PHYSICAL LABORATORY

Continuation Sheet

MEASUREMENT PROCEDURE

For frequencies at or above 835 MHz, the calibration method is based on establishing a calculable specific absorption rate (SAR) using a matched waveguide cell [1]. The cell has a feed-section and a liquid-filled section separated by a matching window that is designed to minimise reflections at the interface. A TE_{01} mode is launched into the waveguide by means of a N-type-to-waveguide adapter. The power delivered to the liquid is calculated from the forward power and reflection coefficient measured at the input to the cell. At the centre of the cross-section of the waveguide cell, the volume specific absorption rate (SAR^V) in the liquid as a function of distance from the window is given by

$$SAR^V = \frac{4(P_w)}{ab\delta} e^{-2Z/\delta} \quad (1)$$

where

- a = the larger cross-sectional dimension of the waveguide.
- b = the smaller cross-sectional dimension of the waveguide.
- δ = the skin depth for the liquid in the waveguide.
- Z = the distance of the probe's sensors from the liquid to matching window boundary.
- P_w = the power delivered to the liquid.

For frequencies below 835 MHz, the SAR in the liquid is established by measuring the rate of temperature rise in the liquid at the calibration point. In this case the SAR in the liquid is related to the temperature rise by

$$SAR = c \frac{dT}{dt} \quad (2)$$

where c is the specific heat of the liquid.

Liquids having the properties specified by SAR measurement standards [2, 3, 4] were used for the calibration. The value of δ for the liquid was obtained by measuring the electric field (E) at a number of distances from the matching window. The calibration was for continuous wave (CW) signals, and the axis of the probe was parallel to the direction of propagation of the incident field i.e. end-on to the incident radiation. The probe was rotated about its axis in 15-degree steps, and the ratio of the calibration factors for the three probe sensors X, Y, & Z were optimized to give the best axial isotropy.

Reference : 2012020074-1

Page 2 of 7

Date of Issue : 1 March 2012

Checked by : *BAU*



NATIONAL PHYSICAL LABORATORY

Continuation Sheet

The probe was calibrated with the linearisation and air-correction factors enabled. Comparing the measured values of E^2 in the liquid to those calculated for the waveguide cell allows the ratio, $ConvF$, of sensitivity for $(E^2_{LIQUID}) / (E^2_{AIR})$ to be determined, as required by the probe software.

The linear response of the probe to continuous wave signals was tested at 1800 MHz over the range 0.12 W/kg to 100 W/kg in accordance with [3].

The spherical isotropy of the probe was tested in head liquid at 900 MHz, in accordance with [3, 5, 6], for probe axial rotation (θ) through 360° and source polarisation (ϕ) rotation through 90° in 15° increments.

ENVIRONMENT

Measurements were made in a temperature-controlled laboratory at $22 \pm 1^\circ\text{C}$. The temperature of the liquid used was measured at the beginning and end of each measurement.

UNCERTAINTIES

The estimated uncertainty in calibration for SAR (W kg^{-1}) is $\pm 10\%$. The reported uncertainty is based on a standard uncertainty multiplied by a coverage factor $k=2$, providing a level of confidence of approximately 95%.

This uncertainty is valid when the probe is used in a liquid with the same dielectric properties as those used for the calibration. No estimate is made for the long-term stability of the device calibrated or of the fluids used in the calibration.

When using the probe for SAR testing, additional uncertainties should be added to account for the spherical isotropy of the probe, proximity effects, linearity, and response to pulsed fields. There will be additional uncertainty if the probe is used in liquids having significantly different electrical properties to those used for the calibration. The electrical properties of the liquids will be related to temperature.

RESULTS

Tables 1 and 2 give the results for calibration in liquid.

These calibration factors are only correct when the values for sensitivity in free-space, diode compression and sensor offset from the tip of the probe, as set in the probe software, are the same as those given in Table 1 and 2.

Reference : 2012020074-1

Page 3 of 7

Date of Issue : 1 March 2012

Checked by : *Blel*



NATIONAL PHYSICAL LABORATORY

Continuation Sheet

Table 3 contains the values of the boundary correction factors $f(0)$ and d .

Table 4 gives the probe linearity and spherical isotropy.

REFERENCES:

- [1] Pokovic, KT, T.Schmid and N.Kuster, "Robust set-up for Precise Calibration of E-field probes in Tissue Simulating Liquids at Mobile Phone Frequencies", Proceedings ICECOM 1997, pp 120 – 124, Dubrovnik, Croatia Oct 12-17, 1997.
- [2] British Standard BS EN 503361:2001. "Basic standard for the measurement of specific absorption rate related to human exposure to electromagnetic fields from mobile phones (300 MHz – 3 GHz)".
- [3] IEEE Standard 1528-2003 "Recommended Practice for Determining the Peak Spatial-Averaged Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques".
- [4] Federal Communications Commission, FCC OET Bulletin 65, Supplement C, June 2001, "Evaluating Compliance with FCC Guidelines for Human Exposure to Radiofrequency Electromagnetic Fields Additional Information for Evaluating Compliance of Mobile and Portable Devices with FCC Limits for Human Exposure to Radiofrequency Emissions", David L. Means, Kwok W. Chan.
- [5] IEC Standard 62209-1 Ed 1. (2005), "Human Exposure to Radio Frequency Fields from Handheld and Body-Mounted Wireless Communication Devices - Human models, Instrumentation, and Procedures -- Part 1: Procedure to determine the specific absorption rate (SAR) for hand-held devices used in close proximity to the ear (frequency range of 300 MHz to 3 GHz)".
- [6] IEC Standard 62209-2 Ed 1. (2010), "Human exposure to radio frequency fields from hand-held and body-mounted wireless communication devices - Human models, instrumentation, and procedures - Part 2: Procedure to determine the specific absorption rate (SAR) for wireless communication devices used in close proximity to the human body (frequency range of 30 MHz to 6 GHz)".

Reference : 2012020074-1

Page 4 of 7

Date of Issue : 1 March 2012

Checked by : *PLC*



NATIONAL PHYSICAL LABORATORY

Continuation Sheet

Table 1
Sensitivity in Head Simulating Liquids.
SAR probe: IXP-050
S/N 0170

Probe settings for calibration						
Sensitivity in free-space ⁽¹⁾		Diode Compression ⁽²⁾		Sensor offset from tip of probe ⁽²⁾		
Lin X = 524.99 (V/m) ² /(V*200)		DCP _X = 20 (V*200)		2.7 mm		
Lin Y = 453.82 (V/m) ² /(V*200)		DCP _Y = 20 (V*200)				
Lin Z = 484.81 (V/m) ² /(V*200)		DCP _Z = 20 (V*200)				
Sensitivity in Head Simulating Liquid.						
Calibration frequency	Liquid Phantom ⁽³⁾		Calibration Factors for E^2_{Liquid} / E^2_{Air}			Axial Isotropy
(MHz)	ϵ' ⁽¹⁾	σ ⁽¹⁾ (Sm ⁻¹)	ConvF _X	ConvF _Y	ConvF _Z	(dB)
450	41.8	0.88	0.180	0.177	0.187	±0.01
835	40.2	0.93	0.240	0.215	0.228	±0.01
900	39.8	0.97	0.242	0.217	0.228	±0.01
1800	40.0	1.41	0.277	0.299	0.295	±0.05
1900	39.2	1.39	0.308	0.335	0.292	±0.01
2100	40.5	1.46	0.319	0.350	0.331	±0.02
2450	39.1	1.80	0.308	0.342	0.325	±0.02
2600	38.6	1.95	0.323	0.360	0.344	±0.02

Reference : 2012020074-1

Page 5 of 7

Date of Issue : 1 March 2012

Checked by : *BCel.*



NATIONAL PHYSICAL LABORATORY

Continuation Sheet

Table 2
Sensitivity in Body Simulating Liquids.
SAR probe: IXP-050
S/N 0170

Probe settings for calibration						
Sensitivity in free-space ⁽¹⁾		Diode Compression ⁽²⁾		Sensor offset from tip of probe ⁽²⁾		
Lin X = 524.99 (V/m) ² /(V*200)		DCP _x = 20 (V*200)		2.7 mm		
Lin Y = 453.82 (V/m) ² /(V*200)		DCP _y = 20 (V*200)				
Lin Z = 484.81 (V/m) ² /(V*200)		DCP _z = 20 (V*200)				
Sensitivity in Body Simulating Liquid.						
Calibration frequency (MHz)	Liquid Phantom ⁽³⁾		Calibration Factors for $E^2_{\text{Liquid}} / E^2_{\text{Air}}$			Axial Isotropy (dB)
	ϵ' ⁽³⁾	σ ⁽³⁾ (Sm ⁻¹)	ConvF _x	ConvF _y	ConvF _z	
450	55.6	0.98	0.194	0.187	0.200	±0.03
835	56.1	1.02	0.225	0.231	0.233	±0.01
900	55.8	1.05	0.234	0.242	0.243	±0.01
1800	52.3	1.51	0.305	0.320	0.321	±0.02
1900	52.0	1.59	0.319	0.337	0.338	±0.03
2100	51.5	1.63	0.341	0.375	0.365	±0.01
2450	50.5	1.96	0.342	0.383	0.367	±0.02
2600	50.2	2.12	0.355	0.399	0.382	±0.02

Notes.⁽¹⁾ Measured at 900 MHz⁽²⁾ The manufacturer supplied these figures.⁽³⁾ Measured at a temperature of 22 ± 1 °C.

Reference : 2012020074-1

Date of Issue : 1 March 2012

Checked by : *Blal*

Page 6 of 7



NATIONAL PHYSICAL LABORATORY

Continuation Sheet

Table 3
Boundary Correction Factors
SAR probe: IXP-050
S/N 0170

Frequency (MHz)	Head Simulating Liquid		Body Simulating Liquid	
	$f(0)$	d	$f(0)$	d
450	4.99	0.77	1.17	1.27
835	0.49	2.51	2.71	0.92
900	1.14	1.24	0.98	1.47
1800	0.64	1.73	0.59	1.90
1900	0.76	1.55	0.63	1.80
2100	0.71	1.71	0.69	1.72
2450	1.10	1.30	0.99	1.39
2600	0.77	1.50	0.78	1.55

Table 4
Linearity and Spherical Isotropy
SAR probe: IXP-050
S/N 0170

Parameter	Frequency	Range	Maximum deviation
Linearity	1800 MHz	0.12 – 100 W/kg	± 0.10 dB
Spherical isotropy in head liquid	900 MHz	$\theta = 0$ to 360° , $\varphi = 0$ to 90°	± 0.9 dB

Reference : 2012020074-1

Page 7 of 7

Date of Issue : 1 March 2012

Checked by : *Blcl.*



Product Service



NATIONAL PHYSICAL LABORATORY

Teddington Middlesex UK TW11 0LW Telephone +44 20 8977 3222

Certificate of Calibration

SAR PROBE

IndexSAR

Model: IXP-025

Serial number: G0006

This certificate provides traceability of measurement to recognised national standards, and to the units of measurement realised at the National Physical Laboratory or other recognised national standards laboratories. This certificate may not be reproduced other than in full, unless permission for the publication of an approved extract has been obtained in writing from the Managing Director. It does not of itself impinge to the subject of calibration any attributes beyond those shown by the data contained herein.

FOR: Indexsar Ltd.
Oakfield House
Cudworth Lane
Newdigate
Surrey
RH5 5BG

DESCRIPTION: An IndexSAR isotropic electric field probe for determining specific absorption rates (SAR) in dielectric liquids. The probe has three orthogonal sensors, and the output voltage of the sensors is converted to an optical signal by a meter unit containing an analogue to digital (AD) converter. Probe readings are obtained using software via the RS232 port. The probe was calibrated with IndexSAR amplifier model IXA-010 S/N 036 belonging to NPL.

IDENTIFICATION: The probe is marked with the manufacturer's serial number G0006

MEASUREMENTS COMPLETED ON: 28 November 2011

The reported uncertainty is based on a coverage factor $k = 2$, providing a level of confidence of approximately 95%

Reference : 2011110089-1

Page 1 of 6

Date of Issue : 6 December 2011

Signed : *B. Loader* (Authorised Signatory)Checked by : *BGL*

Name : Mr B G Loader on behalf of NPLML



NATIONAL PHYSICAL LABORATORY

Continuation Sheet

MEASUREMENT PROCEDURE

For frequencies at or above 835 MHz, the calibration method is based on establishing a calculable specific absorption rate (SAR) using a matched waveguide cell [1]. The cell has a feed-section and a liquid-filled section separated by a matching window that is designed to minimise reflections at the interface. A TE_{01} mode is launched into the waveguide by means of a N-type-to-waveguide adapter. The power delivered to the liquid is calculated from the forward power and reflection coefficient measured at the input to the cell. At the centre of the cross-section of the waveguide cell, the volume specific absorption rate (SAR^V) in the liquid as a function of distance from the window is given by

$$SAR^V = \frac{4(P_w)}{ab\delta} e^{-2Z/\delta} \quad (1)$$

where

a = the larger cross-sectional dimension of the waveguide.

b = the smaller cross-sectional dimension of the waveguide.

δ = the skin depth for the liquid in the waveguide.

Z = the distance of the probe's sensors from the liquid to matching window boundary.

P_w = the power delivered to the liquid.

For frequencies below 835 MHz, the SAR in the liquid is established by measuring the rate of temperature rise in the liquid at the calibration point. In this case the SAR in the liquid is related to the temperature rise by

$$SAR = c \frac{dT}{dt} \quad (2)$$

where c is the specific heat of the liquid.

Liquids having the properties specified by SAR measurement standards [2, 3, 4] were used for the calibration. The value of δ for the liquid was obtained by measuring the electric field (E) at a number of distances from the matching window. The calibration was for continuous wave (CW) signals, and the axis of the probe was parallel to the direction of propagation of the incident field i.e. end-on to the incident radiation. The probe was rotated about its axis in 15-degree steps, and the ratio of the calibration factors for the three probe sensors X, Y, & Z were optimized to give the best axial isotropy.

Reference : 2011110089-1

Page 2 of 6

Date of Issue : 6 December 2011

Checked by : *BGL*



NATIONAL PHYSICAL LABORATORY

Continuation Sheet

The probe was calibrated with the linearisation and air-correction factors enabled. Comparing the measured values of E^2 in the liquid to those calculated for the waveguide cell allows the ratio, $ConvF$, of sensitivity for $(E^2_{LIQUID}) / (E^2_{AIR})$ to be determined, as required by the probe software.

ENVIRONMENT

Measurements were made in a temperature-controlled laboratory at $22 \pm 1^\circ\text{C}$. The temperature of the liquid used was measured at the beginning and end of each measurement.

UNCERTAINTIES

The estimated uncertainty in calibration for SAR (W kg^{-1}) is $\pm 10\%$. The reported uncertainty is based on a standard uncertainty multiplied by a coverage factor $k = 2$, providing a level of confidence of approximately 95%.

This uncertainty is valid when the probe is used in a liquid with the same dielectric properties as those used for the calibration. No estimate is made for the long-term stability of the device calibrated or of the fluids used in the calibration.

When using the probe for SAR testing, additional uncertainties should be added to account for the spherical isotropy of the probe, proximity effects, linearity, and response to pulsed fields. There will be additional uncertainty if the probe is used in liquids having significantly different electrical properties to those used for the calibration. The electrical properties of the liquids will be related to temperature.

RESULTS

Tables 1 and 2 give the results for calibration in liquid.

These calibration factors are only correct when the values for sensitivity in free-space, diode compression and sensor offset from the tip of the probe, as set in the probe software, are the same as those given in Table 1 and 2.

Table 3 contains the values of the boundary correction factors $f(\theta)$ and d .

Reference : 2011110089-1

Page 3 of 6

Date of Issue : 6 December 2011

Checked by : *BGL*



NATIONAL PHYSICAL LABORATORY

Continuation Sheet

REFERENCES:

- [1] Pokovic, KT, T.Schmid and N.Kuster, "Robust set-up for Precise Calibration of E-field probes in Tissue Simulating Liquids at Mobile Phone Frequencies", Proceedings ICECOM 1997, pp 120 – 124, Dubrovnik, Croatia Oct 12-17, 1997.
- [2] British Standard BS EN 503361:2001. "Basic standard for the measurement of specific absorption rate related to human exposure to electromagnetic fields from mobile phones (300 MHz – 3 GHz)".
- [3] IEEE Standard 1528-2003 "Recommended Practice for Determining the Peak Spatial-Averaged Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques".
- [4] Federal Communications Commission, FCC OET Bulletin 65, Supplement C, June 2001, "Evaluating Compliance with FCC Guidelines for Human Exposure to Radiofrequency Electromagnetic Fields Additional Information for Evaluating Compliance of Mobile and Portable Devices with FCC Limits for Human Exposure to Radiofrequency Emissions", David L. Means, Kwok W. Chan.

Reference : 2011110089-1

Page 4 of 6

Date of Issue : 6 December 2011

Checked by : *BGL*



NATIONAL PHYSICAL LABORATORY

Continuation Sheet

Table 1
Sensitivity in Head Simulating Liquids.
SAR probe: IXP-025
S/N G0006

Probe settings for calibration						
Sensitivity in free-space ⁽¹⁾		Diode Compression ⁽²⁾		Sensor offset from tip of probe ⁽²⁾		
Lin X = 4181.03 (V/m) ² /(V*200)		DCP _x = 20 (V*200)		1.39 mm		
Lin Y = 4634.25 (V/m) ² /(V*200)		DCP _y = 20 (V*200)				
Lin Z = 3860.61 (V/m) ² /(V*200)		DCP _z = 20 (V*200)				
Sensitivity in Head Simulating Liquid.						
Calibration frequency	Liquid Phantom ⁽³⁾		Calibration Factors for E ² _{Liquid} / E ² _{Air}			Axial Isotropy
(MHz)	ε' ⁽³⁾	σ ⁽³⁾ (Sm ⁻¹)	ConvF _x	ConvF _y	ConvF _z	(dB)
5200	35.16	4.89	0.343	0.335	0.162	±0.09
5800	33.78	5.57	0.405	0.413	0.200	±0.07

Reference : 2011110089-1

Page 5 of 6

Date of Issue : 6 December 2011

Checked by : *Bled*



NATIONAL PHYSICAL LABORATORY

Continuation Sheet

Table 2
Sensitivity in Body Simulating Liquids.
SAR probe: IXP-025
S/N G0006

Probe settings for calibration						
Sensitivity in free-space ⁽¹⁾		Diode Compression ⁽²⁾		Sensor offset from tip of probe ⁽²⁾		
Lin X = 4181.03 (V/m) ² /(V*200)		DCP _x = 20 (V*200)		1.39 mm		
Lin Y = 4634.25 (V/m) ² /(V*200)		DCP _y = 20 (V*200)				
Lin Z = 3860.61 (V/m) ² /(V*200)		DCP _z = 20 (V*200)				
Sensitivity in Body Simulating Liquid.						
Calibration frequency	Liquid Phantom ⁽³⁾		Calibration Factors for E^2_{Liquid} / E^2_{Air}			Axial Isotropy
(MHz)	ϵ' ⁽³⁾	σ ⁽³⁾ (Sm ⁻¹)	$ConvF_x$	$ConvF_y$	$ConvF_z$	(dB)
5200	50.52	5.38	0.439	0.436	0.214	±0.04
5800	48.91	6.24	0.473	0.494	0.235	±0.06

Notes.

- ⁽¹⁾ Measured at 900 MHz
- ⁽²⁾ The manufacturer supplied these figures.
- ⁽³⁾ Measured at a temperature of 22 ± 1 °C.

Table 3
Boundary Correction Factors
SAR probe: IXP-025
S/N G0006

Frequency	Head Simulating Liquid		Body Simulating Liquid	
(MHz)	$f(0)$	d	$f(0)$	d
5200	0.247	1.332	0.281	1.630
5800	0.627	0.992	0.235	2.036

Reference : 2011110089-1

Page 6 of 6

Date of Issue : 6 December 2011

Checked by : *Bld*



Product Service




IMMERSIBLE SAR PROBE

CALIBRATION REPORT

Part Number: IXP-020

S/N L0011

October 2011

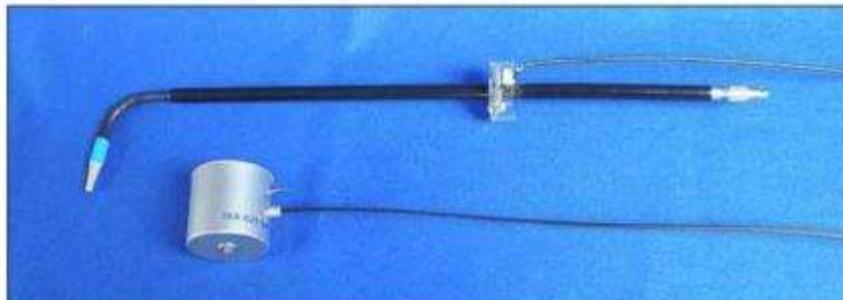

Indexsar Limited
Oakfield House
Cudworth Lane
Newdigate
Surrey RH5 5BG
Tel: +44 (0) 1306 632 870
Fax: +44 (0) 1306 631 834
e-mail: enquiries@indexsar.com

Reproduction of this report is authorized by Indexsar Ltd provided the report is reproduced in its entirety



Product Service



Indexsar Limited
 Oakfield House
 Cudworth Lane
 Newdigate
 Surrey RH5 5BG
 Tel: +44 (0) 1306 632 870
 Fax: +44 (0) 1306 631 834
 e-mail: enquiries@indexsar.com

Calibration Certificate 1110/L0011
Date of Issue: 11th October 2011
Immersible SAR Probe

Type:	IXP-020
Manufacturer:	IndexSAR, UK
Serial Number:	L0011
Place of Calibration:	IndexSAR, UK
Date of Receipt of Probe:	N/A
Calibration Dates:	7 th April — 18 th May 2011
Customer:	TUV

IndexSAR Ltd hereby declares that the IXP-020 Probe named above has been calibrated for conformity to the IEEE 1528 and BSEN 62209-1 standards using the methods described in this calibration document. Where applicable, the standards used in the calibration process are traceable to the UK's National Physical Laboratory.

Calibrated by: *A. Brinklow* Technical Manager

Approved by: *[Signature]* Director

Please keep this certificate with the calibration document. When the probe is sent for a calibration check, please include the calibration document.



INTRODUCTION

This Report presents measured calibration data for a particular Indexsar SAR probe (S/N L0011) only and describes the procedures used for characterisation and calibration.

Indexsar probes are characterised using procedures that, where applicable, follow the recommendations of BSEN 622009-1 [Ref 1] & IEEE [Ref 2] standards. The procedures incorporate techniques for probe linearisation, isotropy assessment and determination of liquid factors (conversion factors). Calibrations are determined by comparing probe readings with analytical computations in canonical test geometries (waveguides) using normalised power inputs.

Each step of the calibration procedure and the equipment used is described in the sections below.

CALIBRATION PROCEDURE

1. Objectives

The calibration process comprises two stages:-

- 1) Determination of the channel sensitivity factors which optimise the probe's overall spherical isotropy in 900MHz brain fluid
- 2) At each frequency of interest, application of these channel sensitivity factors to model the exponential decay of SAR in a waveguide fluid cell, and hence derive the liquid conversion factors at that frequency

2. Probe output

The probe channel output signals are linearised in the manner set out in Refs [1] and [2]. The following equation is utilized for each channel:

$$U_{in} = U_{op} + U_{op}^2 / DCP \quad (1)$$

where U_{in} is the linearised signal, U_{op} is the raw output signal in mV and DCP is the diode compression potential, also in mV.

DCP is determined from fitting equation (1) to measurements of U_{in} versus source feed power over the full dynamic range of the probe. The DCP is a characteristic of the Schottky diodes used as the sensors. For the IXP-020 probes with CW signals the DCP values are typically 100mV.

In turn, measurements of E-field are determined using the following equation:

$$E_{liq}^2 \text{ (V/m)} = U_{inx} * Air Factor_x * Liq Factor_x + U_{iny} * Air Factor_y * Liq Factor_y + U_{inz} * Air Factor_z * Liq Factor_z \quad (3)$$



Here, "Air Factor" represents each channel's sensitivity, while "Liq Factor" represents the enhancement in signal level when the probe is immersed in tissue-simulant liquids at each frequency of interest.

3. Selecting channel sensitivity factors to optimise isotropic response

After manufacture, the first stage of the calibration process is to balance the three channels' Air Factor values, thereby optimising the probe's overall response to incoming signals of any polarisation position angle ("spherical isotropy"). The setup for measuring the probe's spherical isotropy is shown in Figure 1.

A box phantom containing 900MHz head fluid is irradiated by a vertically-polarised, tuned dipole, mounted at the side of the phantom on the robot's seventh axis. The dipole is connected to a signal generator and amplifier via a directional coupler and power meter. The absolute power level is not important as long as it is stable, with stability being monitored using the coupler and power meter.

During calibration, the spherical response is generated by changing the orientation of the probe sensors with respect to the dipole, keeping the long shaft of the probe vertical and the probe sensors at the same position in space.

Initially, the short shaft of the probe is positioned parallel to the phantom wall with its sensors at the same vertical height as the centre of the source dipole and the line joining sensors to dipole perpendicular to the phantom wall (see Figure 1). In this position, the probe is said to be at a position angle of -90 degrees. During the scan, the probe is rotated from -90 to +90 degrees in 10 degree steps, and at each position angle, the dipole polarisation changes from 0 to 360 degrees in 20 degree steps. The short shaft of the probe thereby starts moving increasingly end-on to the dipole, and after perpendicularity, it carries on until facing in the opposite direction from its starting position, all the time with the centroid of the sensors occupying the same position in space.

At each position, an Indexsar 'Fast' amplifier samples the probe channels 500 times per second for 0.4 s. The raw U_{op} data from each sample are packed into 10 bytes and transmitted back to the PC controller via an optical cable. U_{inx} , U_{iny} and U_{inz} are derived from the raw U_{op} values and written to an Excel template.

Once a full set of data has been collected, the Air Factors are adjusted using a special Excel Solver routine to equalise the output from each channel and hence minimise the spherical isotropy. This automated approach to optimisation removes the effect of human bias.



4. Determination of Conversion ("Liquid") Factors at each frequency of interest

A lookup table of conversion factors for a probe allows a SAR value to be derived at the measured frequencies, and for either brain or body fluid-simulant.

The method by which the conversion factors are assessed is based on the comparison between measured and analytical rates of decay of SAR with perpendicular distance from a dielectric window. This way, not only can the conversion factors for that frequency/fluid combination be determined, but an allowance can also be made for the scale and range of boundary layer effects.

The theoretical relationship between the SAR at the cross-sectional centre of the lossy waveguide as a function of the longitudinal distance (z) from the dielectric separator is given by Equation 4:

$$SAR(z) = \frac{4(P_f - P_b)}{\rho ab \delta} e^{-2z/\delta} \quad (4)$$

Here, the density ρ is conventionally assumed to be 1000 kg/m^3 , ab is the cross-sectional area of the waveguide, and P_f and P_b are the forward and reflected power inside the lossless section of the waveguide, respectively. The penetration depth δ (which is the reciprocal of the waveguide-mode attenuation coefficient) is a property of the lossy liquid and is given by Equation (5).

$$\delta = \left[\text{Re} \left\{ \sqrt{(\pi/a)^2 + j\omega\mu_0 (\sigma + j\omega\epsilon_0 \epsilon_r)} \right\} \right]^{-1} \quad (5)$$

where σ is the conductivity of the tissue-simulant liquid in S/m, ϵ_r is its relative permittivity, and ω is the radial frequency (rad/s). Values for σ and ϵ_r are obtained prior to each waveguide test using an Indexsar DiLine measurement kit, which uses the TEM method as recommended in [2]. σ and ϵ_r are both temperature- and fluid-dependent, so are best measured using a sample of the tissue-simulant fluid immediately prior to the actual calibration.

Wherever possible, all DiLine and calibration measurements should be made in the open laboratory at $22 \pm 2.0^\circ\text{C}$; if this is not possible, the values of σ and ϵ_r should reflect the actual temperature. Values employed for calibration are listed in the tables below.

Dedicated waveguides have been designed to accommodate the geometry of an L-shaped probe as it traces out the decay profile. Traditional straight probes measure the decay rate of a vertical-travelling signal above a horizontal dielectric window; for the L-shaped probes, the geometry has had to be changed, and the waveguide now lies horizontally and instead of being open at the end, is capped with a metal plate (see Figure 4). A slot is cut in



the top ("b") face through which tissue simulant fluid can be poured, and through which the probe can enter the guide and be offered up to the now vertical waveguide window.

During calibration, the probe is moved carefully until the flat face of the tip is just touching the cross-sectional centre of the dielectric window. 200 samples are then taken and written to an Excel template file before moving the probe into the liquid away from the waveguide window. This cycle is repeated 150 times. The spatial separation between readings is determined from practical considerations of the expected SAR decay rate, and range from 0.2mm steps at low frequency, through 0.1mm at 2450MHz, down to 0.05mm at 5GHz.

Once the data collection is complete, a Solver routine is run which optimises the measured-theoretical fit by varying the conversion factor, and the boundary correction size and range.

By ensuring the waveguide cap is at least three penetration depths, reflections are negligible. The power absorbed in the liquid is therefore determined solely from the waveguide forward and reflected power.

Different waveguides are used for 835/900MHz, 1800/1900MHz, 2100/2450/2600MHz and 5200/5800MHz measurements. Table A.1 of [1] can be used for designing calibration waveguides with a return loss greater than 20 dB at the most important frequencies used for personal wireless communications, and better than 15dB for frequencies greater than 5GHz. Values for the penetration depth for these specific fixtures and tissue-simulating mixtures are also listed in Table A.1.

For 450 MHz calibrations, a slightly different technique must be used — the equatorial response of the probe-under-test is compared with the equivalent response of a probe whose 450MHz characteristics have already been determined by NPL. The conversion factor of the probe-under-test can then be deduced.

According to [1], this calibration technique provides excellent accuracy, with standard uncertainty of less than 3.6% depending on the frequency and medium. The calibration itself is reduced to power measurements traceable to a standard calibration procedure. The practical limitation to the frequency band of 800 to 5800 MHz because of the waveguide size is not severe in the context of compliance testing.

CALIBRATION FACTORS MEASURED FOR PROBE S/N L0011

The probe was calibrated at 835, 900, 1800, 1900, 2100 and 2450 MHz in liquid samples representing brain liquid at these frequencies.

The calibration was for CW signals only, and the horizontal axis of the probe was parallel to the direction of propagation of the incident field i.e. end-on to the incident radiation.



The reference point for the calibration is in the centre of the probe's cross-section at a distance of 2.7 mm from the probe tip in the direction of the probe amplifier. A value of 2.7 mm should be used for the tip to sensor offset distance in the software. The distance of 2.7mm for assembled probes has been confirmed by taking X-ray images of the probe tips (see Figure 9).

It is important that the diode compression point and air factors used in the software are the same as those quoted in the results tables, as these are used to convert the diode output voltages to a SAR value.

CALIBRATION EQUIPMENT

The Table on page 16 indicates the calibration status of all test equipment used during probe calibration.

MEASUREMENT UNCERTAINTIES


A complete measurement uncertainty analysis for the SARA2 measurement system has been published in Reference [3]. Table 10 from that document is re-created below, and lists the uncertainty factors associated just with the calibration of probes.

Source of uncertainty	Uncertainty value \pm %	Probability distribution	Divisor	c_i	Standard uncertainty $u_i \pm$ %	v_i or v_{eff}
Incident or forward power	5.743	N	1.00	1	5.743	∞
Reflected power	5.773	N	1.00	1	5.773	∞
Liquid conductivity	1.120	N	1.00	1	1.120	∞
Liquid permittivity	1.085	N	1.00	1	1.085	∞
Field homogeneity	0.002	R	1.73	1	0.001	∞
Probe positioning: ± 0.05 mm	0.55	R	1.73	1	0.318	
Influence on Probe pos. $11\%/mm$						
Field probe linearity	4.7	R	1.73	1	2.714	∞
Combined standard uncertainty		RSS			8.729	

At the 95% confidence level, therefore, the expanded uncertainty is 17.1%



SUMMARY OF CAL FACTORS FOR PROBE IXP-020 S/N L0011

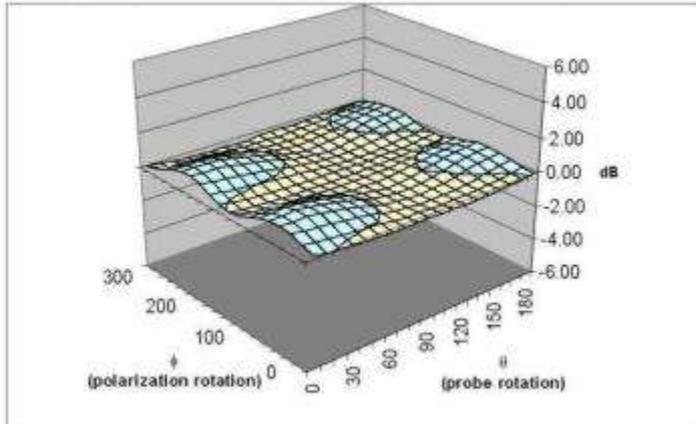

Surface Isotropy diagram of IXP-020 Probe S/N L0011 at 900MHz (axial isotropy +/-0.03dB, spherical isotropy +/-0.58dB, other subsets listed below)

Measured Isotropy at 900MHz	Probe orientation range relative to dipole	(+/-) dB
Spherical Isotropy	±90°	0.58
	±60°	0.54
	±30°	0.32
	±20°	0.22
Axial Isotropy	0°	0.03

Channel Sensitivities				
	X	Y	Z	
Air Factors	69.36	84.92	85.72	(V/m) ² /mV
CW DCPs	100	100	100	mV

SAR Conversion Factors/ Boundary Corrections				
Freq (MHz)	SAR Conv Factor	Boundary Correction f(0)	Boundary Correction d(mm)	Notes
835	0.265	1.9	1.1	1,2
900	0.273	2.0	1.0	1,2
1800	0.327	1.3	1.3	1,2
1900	0.331	0.9	1.5	1,2
2100	0.350	1.0	1.5	1,2
2450	0.359	0.8	1.6	1,2
Notes				
1)	Calibrations done at 22°C +/-2°C			
2)	Waveguide calibration			

Probe tip radius: 0 mm
 X Ch. Angle to red dot: 0°



PROBE SPECIFICATIONS

Indexsar probe L0011, along with its calibration, is compared with BSEN 62209-1 and IEEE standards recommendations (Refs [1] and [2]) in the Tables below. A listing of relevant specifications is contained in the tables below:

Dimensions	S/N L0011	BSEN [1]	IEEE [2]
Vertical shaft (mm)	510		
Horizontal shaft (mm)	90		
Tip length (mm)	10		
Body diameter (mm)	12		
Tip diameter (mm)	5.2	8	8
Distance from probe tip to dipole centers (mm)	2.7		

Dynamic range	S/N L0011	BSEN [1]	IEEE [2]
Minimum (W/kg)	0.01	<0.02	0.01
Maximum (W/kg) N.B. only measured to > 100 W/kg on representative probes	>100	>100	100

Isotropy (measured at 900MHz)		S/N L0011	BSEN [1]	IEEE [2]
Spherical	Probe at $\pm 90^\circ$	0.58	1.0	0.50
	Probe at $\pm 60^\circ$	0.54		
	Probe at $\pm 30^\circ$	0.32		
	Probe at $\pm 20^\circ$	0.22		
Axial	Probe at 0°	0.03	0.5	0.25

Construction	Each probe contains three orthogonal dipole sensors arranged on a triangular prism core, protected against static charges by built-in shielding, and covered at the tip by PEEK cylindrical enclosure material. Outer case materials are PEEK and heat-shrink sleeving.
Chemical resistance	Tested to be resistant to TWEEN and sugar/salt-based simulant liquids but probes should be removed, cleaned and dried when not in use. NOT recommended for use with glycol or soluble oil-based liquids.



Product Service

REFERENCES

- [1] BSEN 62209-1:2006. Human exposure to radio frequency fields from hand-held and body-mounted wireless communication devices — Human models, instrumentation, and procedures — Part 1: Procedure to determine the specific absorption rate (SAR) for hand-held devices used in close proximity to the ear (frequency range of 300 MHz to 3 GHz)
- [2] IEEE 1528, 2003 Recommended Practice for Determining the Peak Spatial-Average Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques
- [3] Indexsar Report IXS-0300, October 2007. Measurement uncertainties for the SARA2 system assessed against the recommendations of BS EN 62209-1:2006

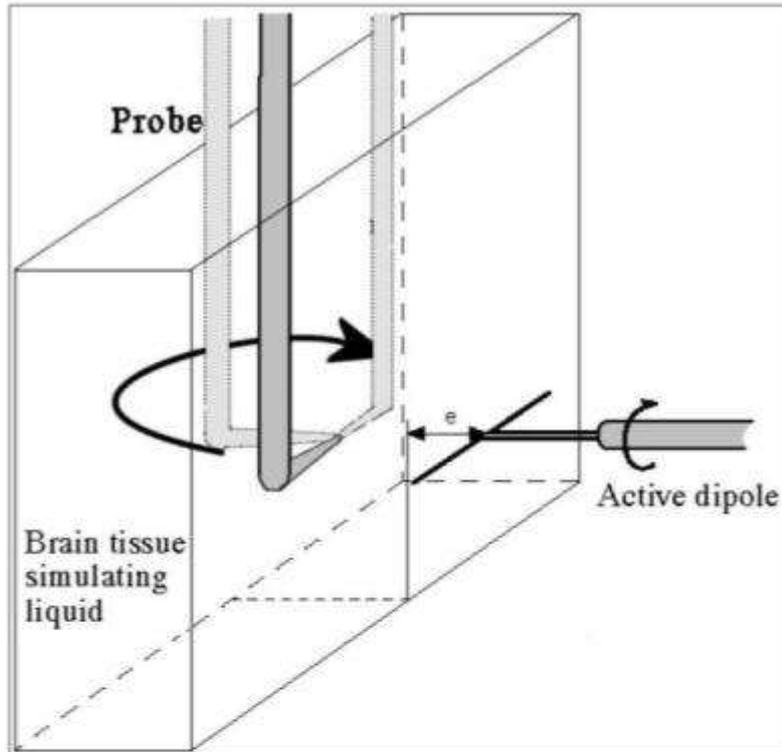


Figure 1. Spherical isotropy jig showing probe, dipole and box filled with simulated brain liquid (see Ref [2], Section A.5.2.1)

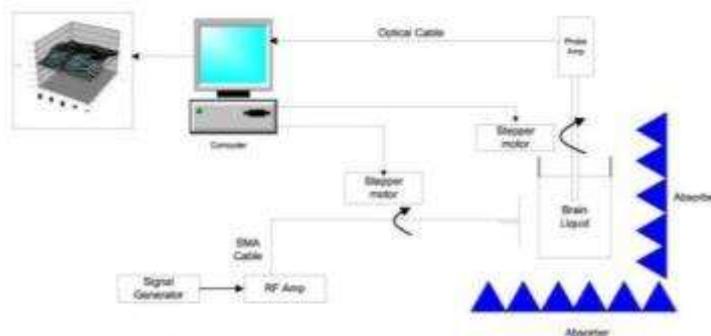


Figure 2. Schematic diagram of the test geometry used for isotropy determination

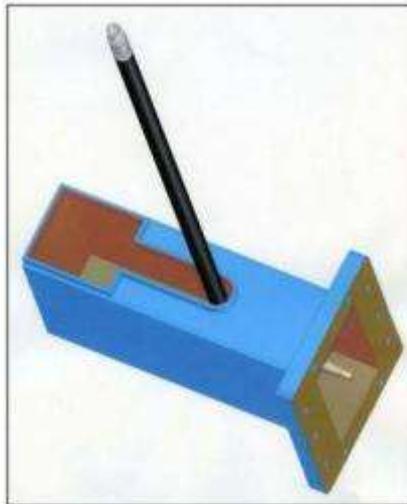


Figure 4. Schematic showing the innovative design of slot in the waveguide termination

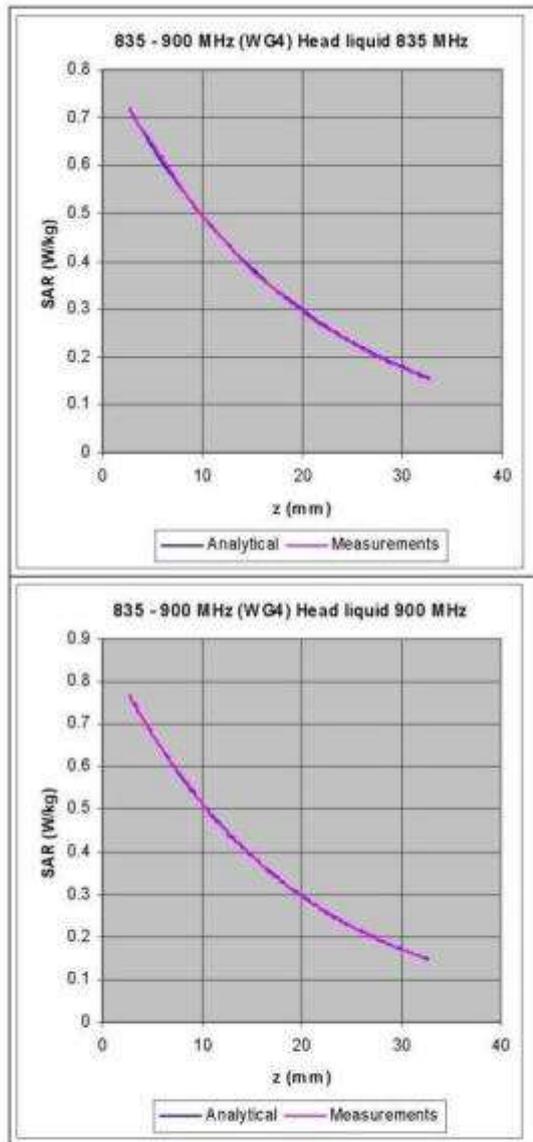
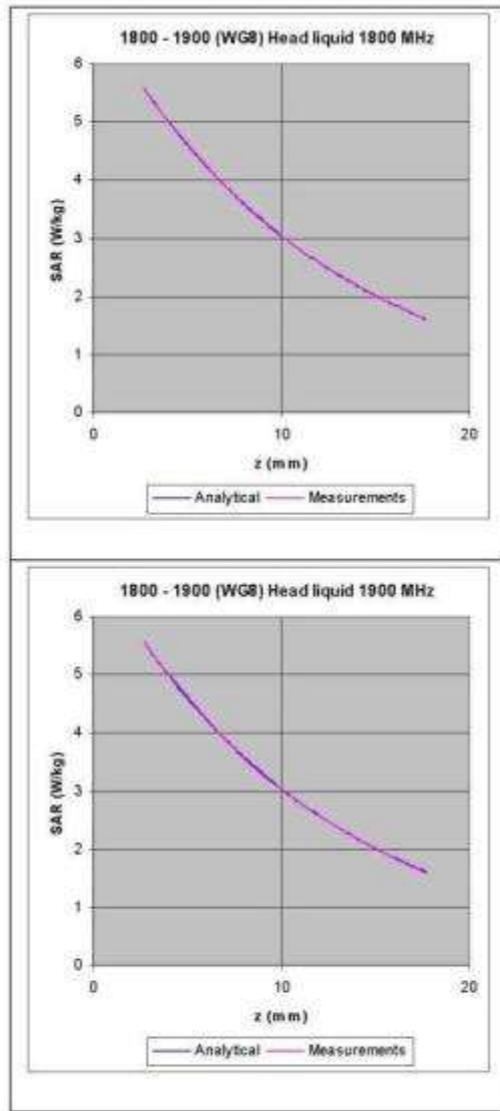


Figure 6. The measured SAR decay function along the centreline of the WG4 waveguide with conversion factors adjusted to fit to the theoretical function for the particular dimension, frequency, power and liquid properties employed.



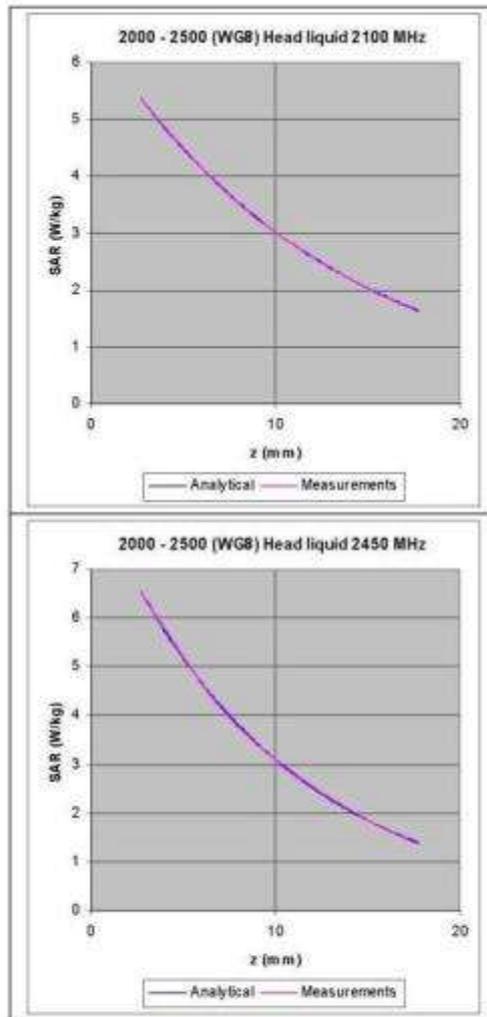


Figure 7. The measured SAR decay function along the centreline of the R22 waveguide with conversion factors adjusted to fit to the theoretical function for the particular dimension, frequency, power and liquid properties employed.

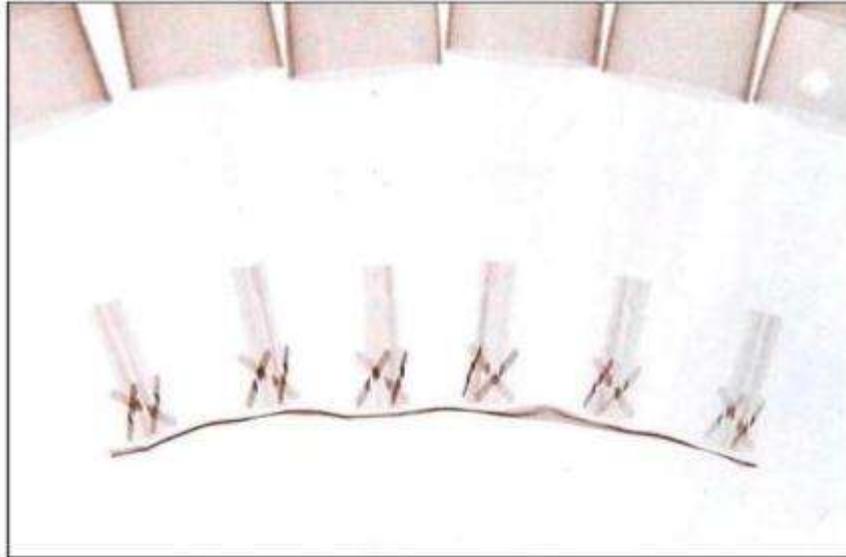


Figure 9: X-ray positive image of 5mm probes

Table indicating the dielectric parameters of the liquids used for calibrations at each frequency

Liquid used	Relative permittivity (measured)	Conductivity (S/m) (measured)
835 MHz BRAIN	42.80	0.91
900 MHz BRAIN	40.47	0.95
1800 MHz BRAIN	40.01	1.42
1900 MHz BRAIN	40.08	1.42
2100 MHz BRAIN	41.98	1.38
2450 MHz BRAIN	40.68	1.77

Table of test equipment calibration status

Instrument description	Supplier / Manufacturer	Model	Serial No.	Last calibration date	Calibration due date
Power sensor	Rohde & Schwarz	NRP-Z23	100169	14/09/2010	14/9/2012
Dielectric property measurement	Index sar	DILine (sensor lengths: 160mm, 80mm and 60mm)	N/A	(absolute) – checked against NPL values using reference liquids	N/A
Vector network analyser	Anritsu	MS6423B	003102	17/01/2011	17/01/2012
SMA autocalibration module	Anritsu	36581KKF/1	001902	17/01/2011	17/01/2012



Product Service




IMMERSIBLE SAR PROBE

CALIBRATION REPORT

Part Number: IXP-021

S/N LG0018

October 2012

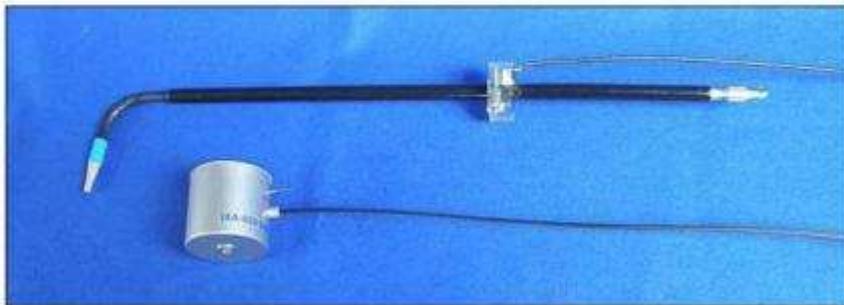

**Indexsar Limited
Oakfield House
Cudworth Lane
Newdigate
Surrey RH5 5BG**

Tel: +44 (0) 1306 632 870

Fax: +44 (0) 1306 631 834

e-mail: enquiries@indexsar.com

Reproduction of this report is authorized by Indexsar Ltd provided the report is reproduced in its entirety



Product Service



Indexsar Limited
Oakfield House
Cudworth Lane
Newdigate
Surrey RH5 5BG
 Tel: +44 (0) 1306 632 870
 Fax: +44 (0) 1306 631 834
 e-mail: enquiries@indexsar.com

Calibration Certificate 1210/LG0018
Date of Issue: 24th October 2012
Immersible SAR Probe

Type:	IXP-021
Manufacturer:	IndexSAR, UK
Serial Number:	LG0018
Place of Calibration:	IndexSAR, UK
Date of Receipt of Probe:	N/A
Customer:	TUV Sud

IndexSAR Ltd hereby declares that the IXP-021 Probe named above has been calibrated for conformity to the IEEE 1528 and BSEN 62209-1 standards using the methods described in this calibration document. Where applicable, the standards used in the calibration process are traceable to the UK's National Physical Laboratory.

Calibrated by: *A. Brinklow* Technical Manager

Approved by: *[Signature]* Director

Please keep this certificate with the calibration document. When the probe is sent for a calibration check, please include the calibration document.



INTRODUCTION

This Report presents measured calibration data for a particular Indexsar SAR probe (S/N LG0018) only and describes the procedures used for characterisation and calibration.

Indexsar probes are characterised using procedures that, where applicable, follow the recommendations of BSEN 622009-1 [Ref 1] & IEEE [Ref 2] standards. The procedures incorporate techniques for probe linearisation, isotropy assessment and determination of liquid factors (conversion factors). Calibrations are determined by comparing probe readings with analytical computations in canonical test geometries (waveguides) using normalised power inputs.

Each step of the calibration procedure and the equipment used is described in the sections below.

CALIBRATION PROCEDURE

1. Objectives

The calibration process comprises two stages:-

- 1) Determination of the channel sensitivity factors which optimise the probe's overall rotational isotropy in brain fluid
- 2) At each frequency of interest, application of these channel sensitivity factors to model the exponential decay of SAR in a waveguide fluid cell, and hence derive the liquid conversion factors at that frequency

2. Probe output

The probe channel output signals are linearised in the manner set out in Refs [1] and [2]. The following equation is utilized for each channel:

$$U_{lin} = U_{op} + U_{op}^2 / DCP \quad (1)$$

where U_{lin} is the linearised signal, U_{op} is the raw output signal in mV and DCP is the diode compression potential, also in mV.

DCP is determined from fitting equation (1) to measurements of U_{lin} versus source feed power over the full dynamic range of the probe. The DCP is a characteristic of the Schottky diodes used as the sensors. For the IXP-021 probes with CW signals the DCP values are typically 100mV.

In turn, measurements of E-field are determined using the following equation:

$$E_{liq}^2 (V/m) = U_{linx} * Air Factor_x * Liq Factor_x + U_{liny} * Air Factor_y * Liq Factor_y + U_{linz} * Air Factor_z * Liq Factor_z \quad (3)$$



Here, "Air Factor" represents each channel's sensitivity, while "Liq Factor" represents the enhancement in signal level when the probe is immersed in tissue-simulant liquids at each frequency of interest.

3. Selecting channel sensitivity factors to optimise isotropic response

After manufacture, the first stage of the calibration process is to balance the three channels' Air Factor values, thereby optimising the probe's overall response to incoming signals of any polarisation position angle ("rotational isotropy"). The setup for measuring the probe's rotational isotropy for frequencies below 3GHz is shown in Figure 1, while above 3GHz, the probe is clamped with the short shaft hanging down vertically in the mouth of a waveguide mounted on a turntable, Figure 2.

A box phantom containing head fluid is irradiated by a vertically-polarised, tuned dipole, mounted at the side of the phantom on the robot's seventh axis. The dipole is connected to a signal generator and amplifier via a directional coupler and power meter. The absolute power level is not important as long as it is stable, with stability being monitored using the coupler and power meter.

During calibration, the spherical response is generated by changing the orientation of the probe sensors with respect to the dipole, keeping the long shaft of the probe vertical and the probe sensors at the same position in space.

Initially, the short shaft of the probe is positioned parallel to the phantom wall with its sensors at the same vertical height as the centre of the source dipole and the line joining sensors to dipole perpendicular to the phantom wall (see Figure 1). In this position, the probe is said to be at a position angle of -90 degrees. During the scan, the probe is rotated from -90 to +90 degrees in 10 degree steps, and at each position angle, the dipole polarisation changes from 0 to 360 degrees in 20 degree steps. The short shaft of the probe thereby starts moving increasingly end-on to the dipole, and after perpendicularity, it carries on until facing in the opposite direction from its starting position, all the time with the centroid of the sensors occupying the same position in space. When the short shaft is exactly end-on to the dipole, rotating the dipole generates the rotational isotropy figure.

At each position, an Indexsar 'Fast' amplifier samples the probe channels 500 times per second for 0.4 s. The raw U_{olp} data from each sample are packed into 10 bytes and transmitted back to the PC controller via an optical cable. U_{linx} , U_{liny} and U_{linz} are derived from the raw U_{olp} values and written to an Excel template.

Once a full set of data has been collected, the Air Factors are adjusted using a special Excel Solver routine to equalise the output from each channel and hence minimise the rotational isotropy. This automated approach to optimisation removes the effect of human bias.

The process is repeated for each frequency of interest.



4. Determination of Conversion (“Liquid”) Factors at each frequency of interest

A lookup table of conversion factors for a probe allows a SAR value to be derived at the measured frequencies, and for either brain or body fluid-simulant.

The method by which the conversion factors are assessed is based on the comparison between measured and analytical rates of decay of SAR with perpendicular distance from a dielectric window. This way, not only can the conversion factors for that frequency/fluid combination be determined, but an allowance can also be made for the scale and range of boundary layer effects.

The theoretical relationship between the SAR at the cross-sectional centre of the lossy waveguide as a function of the longitudinal distance (*z*) from the dielectric separator is given by Equation 4:

$$SAR(z) = \frac{4(P_f - P_r)}{\rho ab \delta} e^{-2z/\delta} \tag{4}$$

Here, the density ρ is conventionally assumed to be 1000 kg/m³, ab is the cross-sectional area of the waveguide, and P_f and P_r are the forward and reflected power inside the lossless section of the waveguide, respectively. The penetration depth δ (which is the reciprocal of the waveguide-mode attenuation coefficient) is a property of the lossy liquid and is given by Equation (5).

$$\delta = \left[\text{Re} \left\{ \sqrt{(\pi/a)^2 + j\omega\mu_0 (\sigma + j\omega\epsilon_0 \epsilon_r)} \right\} \right]^{-1} \tag{5}$$

where σ is the conductivity of the tissue-simulant liquid in S/m, ϵ_r is its relative permittivity, and ω is the radial frequency (rad/s). Values for σ and ϵ_r are obtained prior to each waveguide test using an Indexsar DiLine measurement kit, which uses the TEM method as recommended in [2]. σ and ϵ_r are both temperature- and fluid-dependent, so are best measured using a sample of the tissue-simulant fluid immediately prior to the actual calibration.

Wherever possible, all DiLine and calibration measurements should be made in the open laboratory at 22 ± 2.0°C; if this is not possible, the values of σ and ϵ_r should reflect the actual temperature. Values employed for calibration are listed in the tables below.

Dedicated waveguides have been designed to accommodate the geometry of an L-shaped probe as it traces out the decay profile. Traditional straight probes measure the decay rate of a vertical-travelling signal above a horizontal dielectric window; for the L-shaped probes below 3GHz, the geometry has had to be changed, and the waveguide now lies horizontally



and instead of being open at the end, is capped with a metal plate (see Figure 4). A slot is cut in the top ("b") face through which tissue simulant fluid can be poured, and through which the probe can enter the guide and be offered up to the now vertical waveguide window. Above 3GHz, where the short shaft is longer than the height of the fluid-filled waveguide cell, the probe is oriented as shown in Figure 2.

During calibration, the probe is moved carefully until the flat face of the tip is just touching the cross-sectional centre of the dielectric window. 200 samples are then taken and written to an Excel template file before moving the probe into the liquid away from the waveguide window. This cycle is repeated 150 times. The spatial separation between readings is determined from practical considerations of the expected SAR decay rate, and range from 0.2mm steps at low frequency, through 0.1mm at 2450MHz, down to 0.05mm at 5GHz.

Once the data collection is complete, a Solver routine is run which optimises the measured-theoretical fit by varying the conversion factor, and the boundary correction size and range.

By ensuring the waveguide cap is at least three penetration depths, reflections are negligible. The power absorbed in the liquid is therefore determined solely from the waveguide forward and reflected power.

Different waveguides are used for 835/900MHz, 1800/1900MHz, 2100/2450/2600MHz and 5200/5800MHz measurements. Table A.1 of [1] can be used for designing calibration waveguides with a return loss greater than 20 dB at the most important frequencies used for personal wireless communications, and better than 15dB for frequencies greater than 5GHz. Values for the penetration depth for these specific fixtures and tissue-simulating mixtures are also listed in Table A.1.

For 450 MHz calibrations, a slightly different technique must be used — the equatorial response of the probe-under-test is compared with the equivalent response of a probe whose 450MHz characteristics have already been determined by NPL. The conversion factor of the probe-under-test can then be deduced.

According to [1], this calibration technique provides excellent accuracy, with standard uncertainty of less than 3.6% depending on the frequency and medium. The calibration itself is reduced to power measurements traceable to a standard calibration procedure. The practical limitation to the frequency band of 800 to 5800 MHz because of the waveguide size is not severe in the context of compliance testing.

CALIBRATION FACTORS MEASURED FOR PROBE S/N LG0018

The probe was calibrated at 5200 and 5800 MHz in liquid samples representing brain and muscle tissue at these frequencies.



The calibration was for CW signals only, and the horizontal axis of the probe was parallel to the direction of propagation of the incident field i.e. end-on to the incident radiation.

The reference point for the calibration is in the centre of the probe's cross-section at a distance of 2.7 mm from the probe tip in the direction of the probe amplifier. A value of 2.7 mm should be used for the tip to sensor offset distance in the software. The distance of 2.7mm for assembled probes has been confirmed by taking X-ray images of the probe tips (see Figure 9).

It is important that the diode compression point and air factors used in the software are the same as those quoted in the results tables, as these are used to convert the diode output voltages to a SAR value.

CALIBRATION EQUIPMENT

The Table on page 16 indicates the calibration status of all test equipment used during probe calibration.

MEASUREMENT UNCERTAINTIES

A complete measurement uncertainty analysis for the SARA-C measurement system has been published in Reference [3]. Table 17 from that document is re-created below, and lists the uncertainty factors associated just with the calibration of probes.

Source of uncertainty	Uncertainty value ± %	Probability distribution	Divisor	c _i	Standard uncertainty u _i ± %	v _i of V _{ref}
Forward power	3.92	N	1.00	1	3.92	=
Reflected power	4.09	N	1.00	1	4.09	=
Liquid conductivity	1.308	N	1.00	1	1.31	=
Liquid permittivity	1.271	N	1.00	1	1.27	=
Field homogeneity	3.0	R	1.73	1	1.73	=
Probe positioning	0.22	R	1.73	1	0.13	=
Field probe linearity	0.2	R	1.73	1	0.12	=
Combined standard uncertainty		RSS			6.20	

At the 95% confidence level, therefore, the expanded uncertainty is ±12.4%

SUMMARY OF CAL FACTORS FOR PROBE IXP-021 S/N LG0018

SAR Calibration Factors / Boundary Corrections*								
Freq (MHz)	Tissue Type	Air Factor X ((V/m) ² :mV)	Air Factor Y ((V/m) ² :mV)	Air Factor Z ((V/m) ² :mV)	Rotational Isotropy (± dB)	SAR Conv Factor	Boundary Correction f(θ)	Boundary Correction d(mm)
5200	Head	285.66	352.95	321.39	0.07	0.784	0.675	0.891
5500		287.11	350.55	322.34	-	0.851	0.635	1.084
5800		288.55	348.15	323.30	0.04	0.919	0.594	1.277
5200	Body	287.52	347.12	325.35	0.02	1.029	0.541	1.790
5500		288.25	347.27	326.48	-	1.039	0.515	1.705
5800		284.98	347.41	327.61	0.02	1.049	0.489	1.619

* Data for 5500MHz are interpolated from measured data at 5200 and 5800MHz



PROBE SPECIFICATIONS

Indexsar probe LG0018, along with its calibration, is compared with BSEN 62209-1 and IEEE standards recommendations (Refs [1] and [2]) in the Tables below. A listing of relevant specifications is contained in the tables below:

Dimensions	S/N LG0018	BSEN [1]	IEEE [2]
Vertical shaft (mm)	510		
Horizontal shaft (mm)	90		
Tip length (mm)	10		
Body diameter (mm)	12		
Tip diameter (mm)	5.2	8	8
Distance from probe tip to dipole centers (mm)	2.7		

Dynamic range	S/N LG0018	BSEN [1]	IEEE [2]
Minimum (W/kg)	0.01	<0.02	0.01
Maximum (W/kg) N.B. only measured to > 100 W/kg on representative probes	>100	>100	100

Rotational Isotropy	S/N LG0018	BSEN [1]	IEEE [2]
5200 Head	0.07	0.5	0.25
5800 Head	0.04		
5200 Body	0.02		
5800 Body	0.02		

Construction	Each probe contains three orthogonal dipole sensors arranged on a triangular prism core, protected against static charges by built-in shielding, and covered at the tip by PEEK cylindrical enclosure material. Outer case materials are PEEK and heat-shrink sleeving.
Chemical resistance	Tested to be resistant to TWEEN and sugar/salt-based simulant liquids but probes should be removed, cleaned and dried when not in use. NOT recommended for use with glycol or soluble oil-based liquids.

REFERENCES

[1] BSEN 62209-1:2006. Human exposure to radio frequency fields from hand-held and body-mounted wireless communication devices — Human models, instrumentation, and procedures — Part 1: Procedure to determine the specific absorption rate (SAR) for hand-held devices used in close proximity to the ear (frequency range of 300 MHz to 3 GHz)

[2] IEEE 1528, 2003 Recommended Practice for Determining the Peak Spatial-Average Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques

[3] SARA-C SAR Testing System: Measurement Uncertainty, v1.0.3. 13 October 2011.

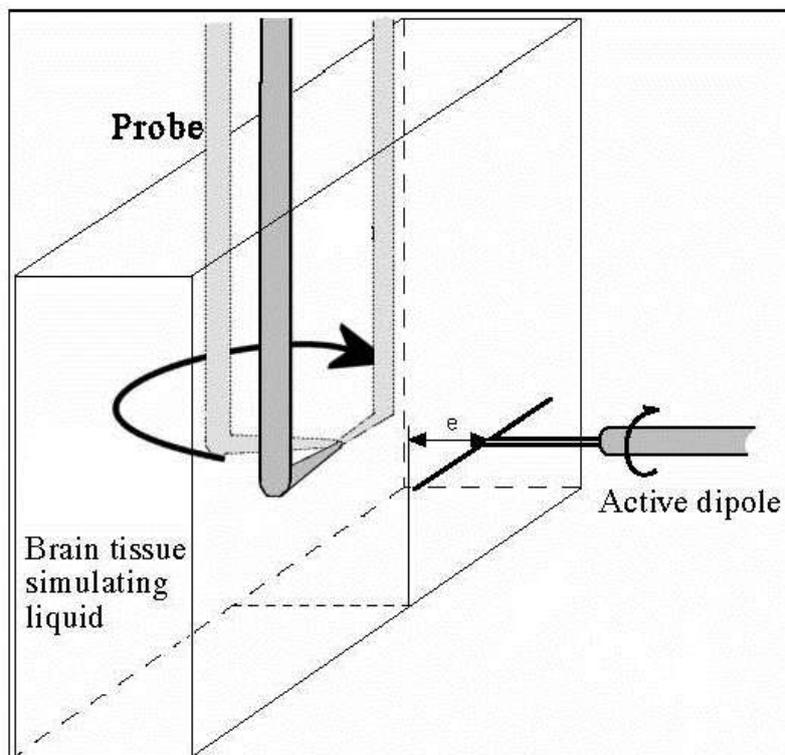


Figure 1. Spherical isotropy jig showing probe, dipole and box filled with simulated brain liquid (see Ref [2], Section A.5.2.1)

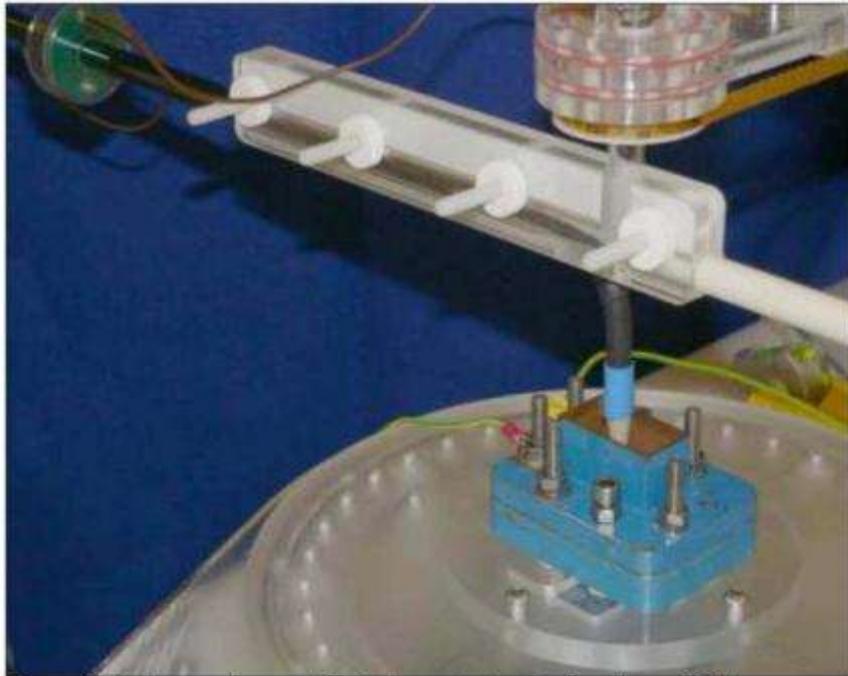


Figure 2 Test geometry used for isotropy determination above 3GHz

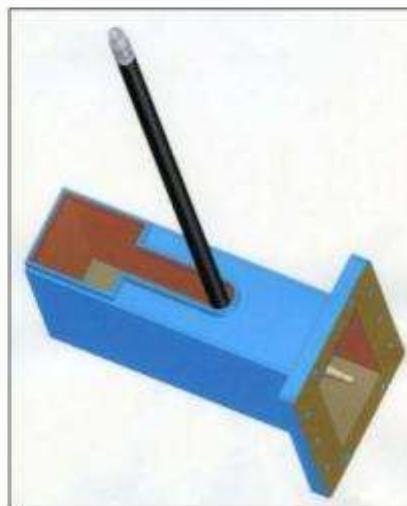


Figure 4. Schematic showing the innovative design of slot in the waveguide termination

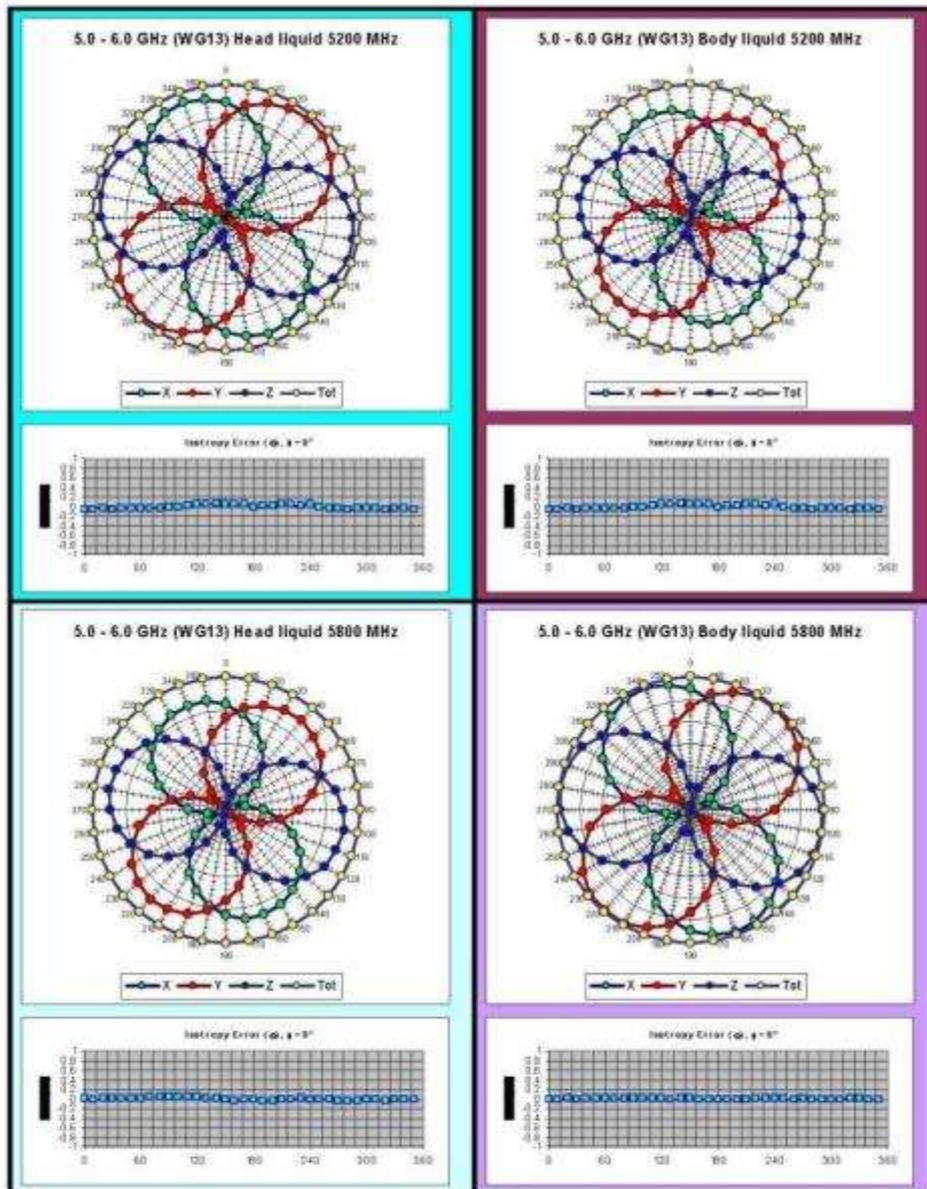


Figure 6. Rotational isotropy measurements inside a WG13 waveguide.

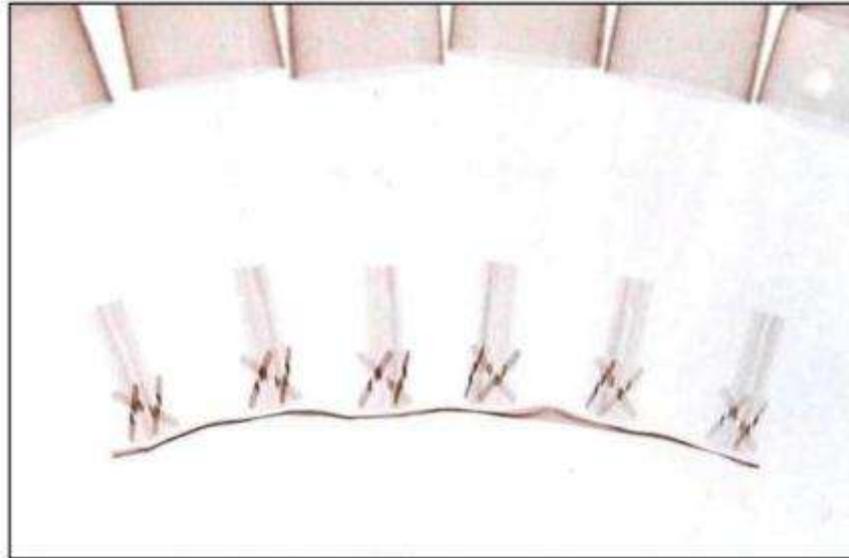


Figure 9: X-ray positive image of 5mm probes

Table indicating the dielectric parameters of the liquids used for calibrations at each frequency

Liquid used	Relative permittivity (measured)	Conductivity (S/m) (measured)
5200 MHz HEAD	36.24	4.53
5800 MHz HEAD	35.17	4.99
5200 MHz BODY	50.89	4.93
5800 MHz BODY	48.67	6.02

Table of test equipment calibration status as at time of probe calibration

Instrument description	Supplier / Manufacturer	Model	Serial No.	Calibration due date
Power sensor	Rohde & Schwarz	NRP-Z23	100063	08/09/2014
Dielectric property measurement	Indexsar	DiLine (sensor lengths: 160mm, 80mm and 60mm)	N/A	N/A
Vector network analyser	Anritsu	MS6423B	003102	16/01/2013
SMA autocalibration module	Anritsu	36581KKF/1	001902	16/01/2013



Product Service

ANNEX B

DIPOLE CALIBRATION REPORTS



Product Service

**Calibration Laboratory of
Schmid & Partner
Engineering AG**
Zeughausstrasse 43, 8004 Zurich, Switzerland



S Schweizerischer Kalibrierdienst
C Service suisse d'étalonnage
S Servizio svizzero di taratura
S Swiss Calibration Service

Accredited by the Swiss Accreditation Service (SAS)
The Swiss Accreditation Service is one of the signatories to the EA
Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: **SCS 108**

Client **TÜV Product Service Ltd**

Certificate No: **D1900V2-546_Mar11**

CALIBRATION CERTIFICATE

Object: **D1900V2 - SN: 546**

Calibration procedure(s): **QA CAL-05.v8
Calibration procedure for dipole validation kits**

Calibration date: **March 21, 2011**

This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI).
The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility; environment temperature (22 ± 3)°C and humidity < 70%.

Calibration Equipment used (M&TE critical for calibration)

Primary Standards	ID #	Cal Date (Certificate No.)	Scheduled Calibration
Power meter EPM-442A	GB37480704	06-Oct-10 (No. 217-01266)	Oct-11
Power sensor HP 8481A	US37292783	06-Oct-10 (No. 217-01268)	Oct-11
Reference 20 dB Attenuator	SN: 5086 (20g)	30-Mar-10 (No. 217-01159)	Mar-11
Type-N mismatch combination	SN: 5047.2 / 06327	30-Mar-10 (No. 217-01162)	Mar-11
Reference Probe ES3DV3	SN: 3205	30-Apr-10 (No. ES3-3205_Apr10)	Apr-11
DAE4	SN: 601	10-Jun-10 (No. DAE4-601_Jun10)	Jun-11
Secondary Standards	ID #	Check Date (in house)	Scheduled Check
Power sensor HP 8481A	MY41092317	18-Oct-02 (in house check Oct-09)	In house check: Oct-11
RF generator R&S SMT-06	100005	4-Aug-99 (in house check Oct-09)	In house check: Oct-11
Network Analyzer HP 8753E	US37390585 S4206	18-Oct-01 (in house check Oct-10)	In house check: Oct-11

Calibrated by: **Jeton Kastrati** (Name), **Laboratory Technician** (Function), [Signature]

Approved by: **Katja Pokovic** (Name), **Technical Manager** (Function), [Signature]

Issued: March 21, 2011

This calibration certificate shall not be reproduced except in full without written approval of the laboratory.



Product Service

Calibration Laboratory of
Schmid & Partner
Engineering AG
Zeughausstrasse 43, 8004 Zurich, Switzerland



S Schweizerischer Kalibrierdienst
C Service suisse d'étalonnage
S Servizio svizzero di taratura
S Swiss Calibration Service

Accredited by the Swiss Accreditation Service (SAS)
The Swiss Accreditation Service is one of the signatories to the EA
Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: **SCS 108****Glossary:**

TSL	tissue simulating liquid
ConvF	sensitivity in TSL / NORM x,y,z
N/A	not applicable or not measured

Calibration is Performed According to the Following Standards:

- IEEE Std 1528-2003, "IEEE Recommended Practice for Determining the Peak Spatial-Averaged Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques", December 2003
- IEC 62209-1, "Procedure to measure the Specific Absorption Rate (SAR) for hand-held devices used in close proximity to the ear (frequency range of 300 MHz to 3 GHz)", February 2005
- Federal Communications Commission Office of Engineering & Technology (FCC OET), "Evaluating Compliance with FCC Guidelines for Human Exposure to Radiofrequency Electromagnetic Fields; Additional Information for Evaluating Compliance of Mobile and Portable Devices with FCC Limits for Human Exposure to Radiofrequency Emissions", Supplement C (Edition 01-01) to Bulletin 65

Additional Documentation:

- DASY4/5 System Handbook

Methods Applied and Interpretation of Parameters:

- Measurement Conditions:** Further details are available from the Validation Report at the end of the certificate. All figures stated in the certificate are valid at the frequency indicated.
- Antenna Parameters with TSL:** The dipole is mounted with the spacer to position its feed point exactly below the center marking of the flat phantom section, with the arms oriented parallel to the body axis.
- Feed Point Impedance and Return Loss:** These parameters are measured with the dipole positioned under the liquid filled phantom. The impedance stated is transformed from the measurement at the SMA connector to the feed point. The Return Loss ensures low reflected power. No uncertainty required.
- Electrical Delay:** One-way delay between the SMA connector and the antenna feed point. No uncertainty required.
- SAR measured:** SAR measured at the stated antenna input power.
- SAR normalized:** SAR as measured, normalized to an input power of 1 W at the antenna connector.
- SAR for nominal TSL parameters:** The measured TSL parameters are used to calculate the nominal SAR result.



Measurement Conditions

DASY system configuration, as far as not given on page 1.

DASY Version	DASY5	V52.6.2
Extrapolation	Advanced Extrapolation	
Phantom	Modular Flat Phantom V5.0	
Distance Dipole Center - TSL	10 mm	with Spacer
Zoom Scan Resolution	dx, dy, dz = 5 mm	
Frequency	1900 MHz \pm 1 MHz	

Head TSL parameters

The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Head TSL parameters	22.0 °C	40.0	1.40 mho/m
Measured Head TSL parameters	(22.0 \pm 0.2) °C	39.3 \pm 6 %	1.40 mho/m \pm 6 %
Head TSL temperature during test	(21.5 \pm 0.2) °C	----	----

SAR result with Head TSL

SAR averaged over 1 cm ³ (1 g) of Head TSL	Condition	
SAR measured	250 mW input power	10.1 mW / g
SAR normalized	normalized to 1W	40.4 mW / g
SAR for nominal Head TSL parameters	normalized to 1W	41.3 mW /g \pm 17.0 % (k=2)

SAR averaged over 10 cm ³ (10 g) of Head TSL	condition	
SAR measured	250 mW input power	5.25 mW / g
SAR normalized	normalized to 1W	21.0 mW / g
SAR for nominal Head TSL parameters	normalized to 1W	21.0 mW /g \pm 16.5 % (k=2)

**Body TSL parameters**

The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Body TSL parameters	22.0 °C	53.3	1.52 mho/m
Measured Body TSL parameters	(22.0 ± 0.2) °C	52.1 ± 6 %	1.51 mho/m ± 6 %
Body TSL temperature during test	(21.5 ± 0.2) °C	----	----

SAR result with Body TSL

SAR averaged over 1 cm ³ (1 g) of Body TSL	Condition	
SAR measured	250 mW input power	9.96 mW / g
SAR normalized	normalized to 1W	39.8 mW / g
SAR for nominal Body TSL parameters	normalized to 1W	39.8 mW / g ± 17.0 % (k=2)

SAR averaged over 10 cm ³ (10 g) of Body TSL	condition	
SAR measured	250 mW input power	5.20 mW / g
SAR normalized	normalized to 1W	20.8 mW / g
SAR for nominal Body TSL parameters	normalized to 1W	20.8 mW / g ± 16.5 % (k=2)



Product Service

Appendix

Antenna Parameters with Head TSL

Impedance, transformed to feed point	50.9 Ω + 3.9 j Ω
Return Loss	- 26.1 dB

Antenna Parameters with Body TSL

Impedance, transformed to feed point	45.8 Ω + 4.1 j Ω
Return Loss	- 24.3 dB

General Antenna Parameters and Design

Electrical Delay (one direction)	1.204 ns
----------------------------------	----------

After long term use with 100W radiated power, only a slight warming of the dipole near the feedpoint can be measured.

The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals.

No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feedpoint may be damaged.

Additional EUT Data

Manufactured by	SPEAG
Manufactured on	November 15, 2001



DASY5 Validation Report for Head TSL

Date/Time: 21.03.2011 15:38:43

Test Laboratory: SPEAG, Zurich, Switzerland

DUT: Dipole 1900 MHz; Type: D1900V2; Serial: D1900V2 - SN:546

Communication System: CW; Frequency: 1900 MHz; Duty Cycle: 1:1

Medium: HSL U12 BB

Medium parameters used: $f = 1900$ MHz; $\sigma = 1.4$ mho/m; $\epsilon_r = 39.4$; $\rho = 1000$ kg/m³

Phantom section: Flat Section

Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2007)

DASY5 Configuration:

- Probe: ES3DV3 - SN3205; ConvF(5.09, 5.09, 5.09); Calibrated: 30.04.2010
- Sensor-Surface: 3mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn601; Calibrated: 10.06.2010
- Phantom: Flat Phantom 5.0 (front); Type: QD000P50AA; Serial: 1001
- Measurement SW: DASY52, V52.6.2 Build (424)
- Postprocessing SW: SEMCAD X, V14.4.2 Build (2829)

Pin=250 mW /d=10mm, dist=3.0mm (ES-Probe)/Zoom Scan (7x7x7) /Cube 0: Measurement


grid: dx=5mm, dy=5mm, dz=5mm

Reference Value = 96.820 V/m; Power Drift = 0.04 dB

Peak SAR (extrapolated) = 18.710 W/kg

SAR(1 g) = 10.1 mW/g; SAR(10 g) = 5.25 mW/g


Maximum value of SAR (measured) = 12.512 mW/g

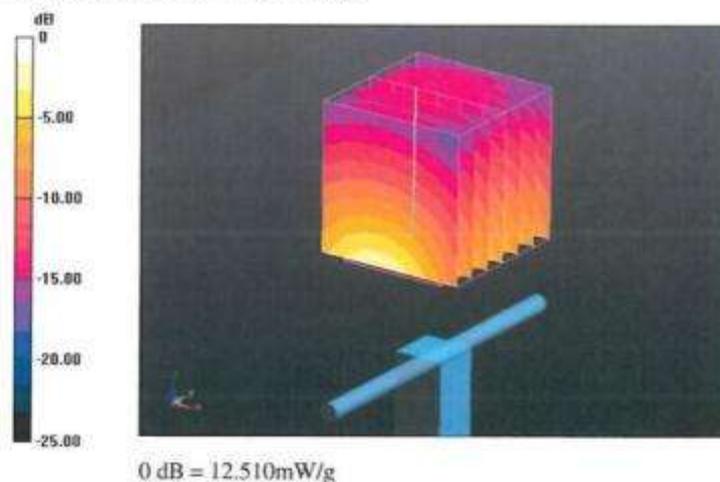



Product Service

Impedance Measurement Plot for Head TSL

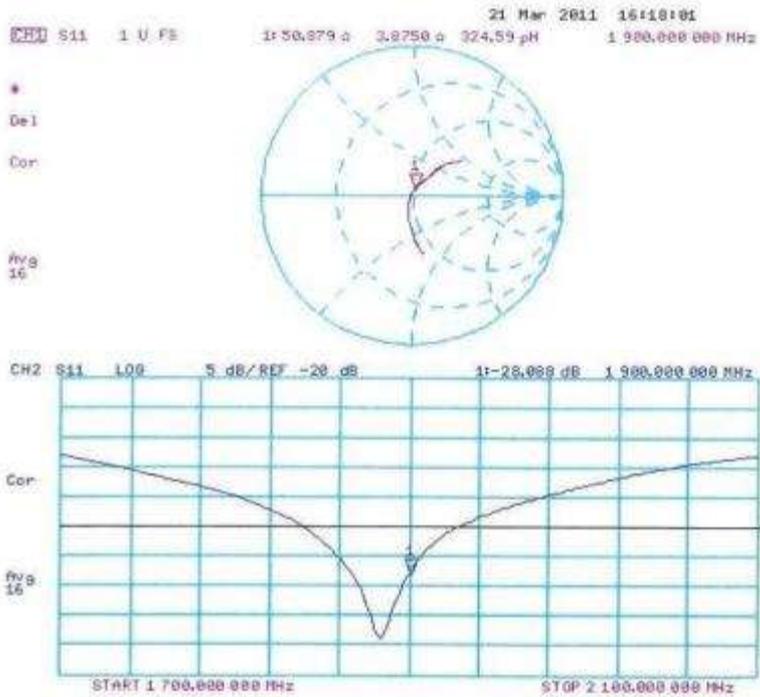



DASY5 Validation Report for Body TSL

Date/Time: 21.03.2011 13:11:15

Test Laboratory: SPEAG, Zurich, Switzerland

DUT: Dipole 1900 MHz; Type: D1900V2; Serial: D1900V2 - SN:546

Communication System: CW; Frequency: 1900 MHz; Duty Cycle: 1:1

Medium: MSL U12 BB

Medium parameters used: $f = 1900$ MHz; $\sigma = 1.51$ mho/m; $\epsilon_r = 52.2$; $\rho = 1000$ kg/m³

Phantom section: Flat Section

Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2007)

DASY5 Configuration:

- Probe: ES3DV3 - SN3205; ConvF(4.59, 4.59, 4.59); Calibrated: 30.04.2010
- Sensor-Surface: 3mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn601; Calibrated: 10.06.2010
- Phantom: Flat Phantom 5.0 (back); Type: QD000P50AA; Serial: 1002
- Measurement SW: DASY52, V52.6.2 Build (424)
- Postprocessing SW: SEMCAD X, V14.4.2 Build (2829)


Pin=250 mW /d=10mm, dist=3.0mm (ES-Probe)/Zoom Scan (7x7x7) /Cube 0: Measurement grid: dx=5mm, dy=5mm, dz=5mm

Reference Value = 96.768 V/m; Power Drift = 0.01 dB

Peak SAR (extrapolated) = 17.207 W/kg

SAR(1 g) = 9.96 mW/g; SAR(10 g) = 5.2 mW/g


Maximum value of SAR (measured) = 12.620 mW/g

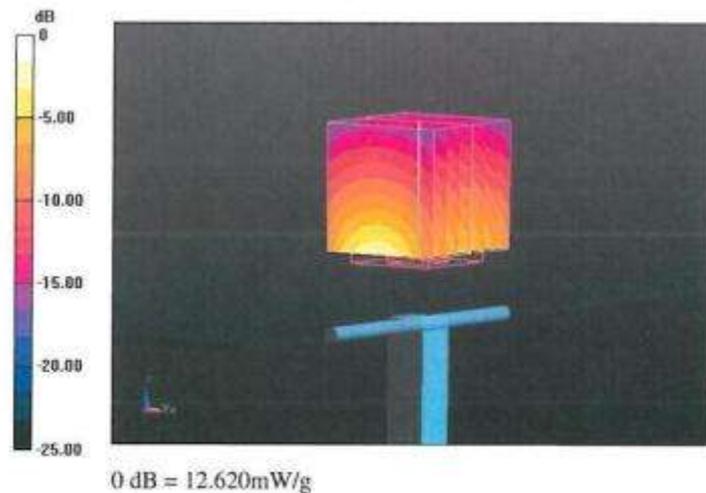



Product Service

Impedance Measurement Plot for Body TSL

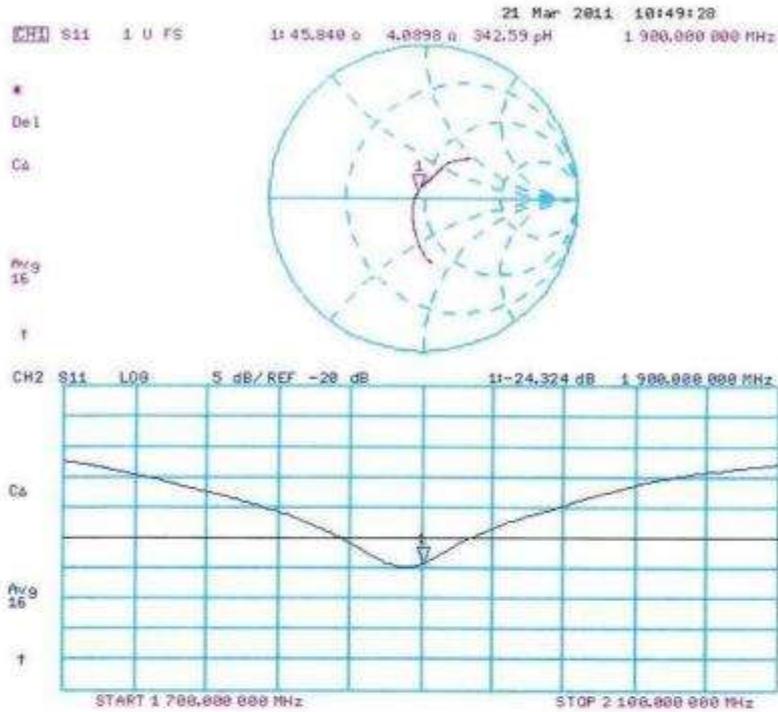



Product Service

**Calibration Laboratory of
Schmid & Partner
Engineering AG**
Zeughausstrasse 43, 8004 Zurich, Switzerland



S Schweizerischer Kalibrierdienst
C Service suisse d'étalonnage
S Servizio svizzero di taratura
S Swiss Calibration Service

Accredited by the Swiss Accreditation Service (SAS)
The Swiss Accreditation Service is one of the signatories to the EA
Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: **SCS 108**

Client **TÜV Product Service Ltd**

Certificate No.: **D2450V2-715_Mar11**

CALIBRATION CERTIFICATE

Object	D2450V2 - SN: 715		
Calibration procedure(s)	QA CAL-05.v8 Calibration procedure for dipole validation kits		
Calibration date:	March 22, 2011		
<p>This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI). The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.</p> <p>All calibrations have been conducted in the closed laboratory facility; environment temperature (22 ± 3)°C and humidity < 70%.</p> <p>Calibration Equipment used (M&TE critical for calibration)</p>			
Primary Standards	ID #	Cal Date (Certificate No.)	Scheduled Calibration
Power meter EPM-442A	GB37480704	06-Oct-10 (No. 217-01266)	Oct-11
Power sensor HP 8481A	US37292783	06-Oct-10 (No. 217-01266)	Oct-11
Reference 20 dB Attenuator	SN: 5086 (20g)	30-Mar-10 (No. 217-01158)	Mar-11
Type-N mismatch combination	SN: 5047.2 / 06327	30-Mar-10 (No. 217-01162)	Mar-11
Reference Probe ES30V3	SN: 3205	30-Apr-10 (No. ES3-3205_Apr10)	Apr-11
DAE4	SN: 601	10-Jun-10 (No. DAE4-601_Jun10)	Jun-11
Secondary Standards	ID #	Check Date (in house)	Scheduled Check
Power sensor HP 8481A	MY41092317	16-Oct-02 (in house check Oct-09)	In house check: Oct-11
RF generator R&S SMT-06	100005	4-Aug-99 (in house check Oct-09)	In house check: Oct-11
Network Analyzer HP 8753E	US37390585 S4206	16-Oct-01 (in house check Oct-10)	In house check: Oct-11
Calibrated by:	Name Dimce Iliev	Function Laboratory Technician	Signature
Approved by:	Name Katja Pokovic	Function Technical Manager	Signature
			Issued: March 22, 2011
This calibration certificate shall not be reproduced except in full without written approval of the laboratory.			



Product Service

**Calibration Laboratory of
Schmid & Partner
Engineering AG**
Zeughausstrasse 43, 8004 Zurich, Switzerland



S Schweizerischer Kalibrierdienst
C Service suisse d'étalonnage
S Servizio svizzero di taratura
S Swiss Calibration Service

Accredited by the Swiss Accreditation Service (SAS)

The Swiss Accreditation Service is one of the signatories to the EA
Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: **SCS 108**

Glossary:

TSL	tissue simulating liquid
ConvF	sensitivity in TSL / NORM x,y,z
N/A	not applicable or not measured

Calibration is Performed According to the Following Standards:

- IEEE Std 1528-2003, "IEEE Recommended Practice for Determining the Peak Spatial-Averaged Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques", December 2003
- IEC 62209-1, "Procedure to measure the Specific Absorption Rate (SAR) for hand-held devices used in close proximity to the ear (frequency range of 300 MHz to 3 GHz)", February 2005
- Federal Communications Commission Office of Engineering & Technology (FCC OET), "Evaluating Compliance with FCC Guidelines for Human Exposure to Radiofrequency Electromagnetic Fields; Additional Information for Evaluating Compliance of Mobile and Portable Devices with FCC Limits for Human Exposure to Radiofrequency Emissions", Supplement C (Edition 01-01) to Bulletin 65

Additional Documentation:

- DASY4/5 System Handbook

Methods Applied and Interpretation of Parameters:

- Measurement Conditions:** Further details are available from the Validation Report at the end of the certificate. All figures stated in the certificate are valid at the frequency indicated.
- Antenna Parameters with TSL:** The dipole is mounted with the spacer to position its feed point exactly below the center marking of the flat phantom section, with the arms oriented parallel to the body axis.
- Feed Point Impedance and Return Loss:** These parameters are measured with the dipole positioned under the liquid filled phantom. The impedance stated is transformed from the measurement at the SMA connector to the feed point. The Return Loss ensures low reflected power. No uncertainty required.
- Electrical Delay:** One-way delay between the SMA connector and the antenna feed point. No uncertainty required.
- SAR measured:** SAR measured at the stated antenna input power.
- SAR normalized:** SAR as measured, normalized to an input power of 1 W at the antenna connector.
- SAR for nominal TSL parameters:** The measured TSL parameters are used to calculate the nominal SAR result.



Measurement Conditions

DASY system configuration, as far as not given on page 1.

DASY Version	DASY5	V52.6.2
Extrapolation	Advanced Extrapolation	
Phantom	Modular Flat Phantom V5.0	
Distance Dipole Center - TSL	10 mm	with Spacer
Zoom Scan Resolution	dx, dy, dz = 5 mm	
Frequency	2450 MHz \pm 1 MHz	

Head TSL parameters

The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Head TSL parameters	22.0 °C	39.2	1.80 mho/m
Measured Head TSL parameters	(22.0 \pm 0.2) °C	38.7 \pm 6 %	1.72 mho/m \pm 6 %
Head TSL temperature during test	(21.3 \pm 0.2) °C	---	---

SAR result with Head TSL

SAR averaged over 1 cm ³ (1 g) of Head TSL	Condition	
SAR measured	250 mW input power	13.0 mW / g
SAR normalized	normalized to 1W	52.0 mW / g
SAR for nominal Head TSL parameters	normalized to 1W	52.9 mW / g \pm 17.0 % (k=2)

SAR averaged over 10 cm ³ (10 g) of Head TSL	condition	
SAR measured	250 mW input power	6.09 mW / g
SAR normalized	normalized to 1W	24.4 mW / g
SAR for nominal Head TSL parameters	normalized to 1W	24.5 mW / g \pm 16.5 % (k=2)



Product Service

Body TSL parameters

The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Body TSL parameters	22.0 °C	52.7	1.95 mho/m
Measured Body TSL parameters	(22.0 ± 0.2) °C	51.5 ± 6 %	1.92 mho/m ± 6 %
Body TSL temperature during test	(22.0 ± 0.2) °C	----	----

SAR result with Body TSL

SAR averaged over 1 cm ³ (1 g) of Body TSL	Condition	
SAR measured	250 mW input power	12.8 mW / g
SAR normalized	normalized to 1W	51.2 mW / g
SAR for nominal Body TSL parameters	normalized to 1W	51.3 mW / g ± 17.0 % (k=2)

SAR averaged over 10 cm ³ (10 g) of Body TSL	condition	
SAR measured	250 mW input power	5.95 mW / g
SAR normalized	normalized to 1W	23.8 mW / g
SAR for nominal Body TSL parameters	normalized to 1W	23.8 mW / g ± 16.5 % (k=2)



Appendix

Antenna Parameters with Head TSL

Impedance, transformed to feed point	53.4 Ω - 0.4 $\mu\Omega$
Return Loss	- 29.5 dB

Antenna Parameters with Body TSL

Impedance, transformed to feed point	49.2 Ω + 1.4 $\mu\Omega$
Return Loss	- 35.7 dB

General Antenna Parameters and Design

Electrical Delay (one direction)	1.156 ns
----------------------------------	----------

After long term use with 100W radiated power, only a slight warming of the dipole near the feedpoint can be measured.

The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals.

No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feedpoint may be damaged.

Additional EUT Data

Manufactured by	SPEAG
Manufactured on	July 05, 2002

**DASY5 Validation Report for Head TSL**

Date/Time: 22.03.2011 13:23:3

Test Laboratory: SPEAG, Zurich, Switzerland

DUT: Dipole 2450 MHz; Type: D2450V2; Serial: D2450V2 - SN:715

Communication System: CW; Frequency: 2450 MHz; Duty Cycle: 1:1

Medium: HSL U12 BB

Medium parameters used: $f = 2450$ MHz; $\sigma = 1.72$ mho/m; $\epsilon_r = 38.8$; $\rho = 1000$ kg/m³

Phantom section: Flat Section

Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2007)

DASY5 Configuration:

- Probe: ES3DV3 - SN3205; ConvF(4.53, 4.53, 4.53); Calibrated: 30.04.2010
- Sensor-Surface: 3mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn601; Calibrated: 10.06.2010
- Phantom: Flat Phantom 5.0 (front); Type: QD000P50AA; Serial: 1001
- Measurement SW: DASY52, V52.6.2 Build (424)
- Postprocessing SW: SEMCAD X, V14.4.4 Build (2829)

Pin=250 mW /d=10mm, dist=3.0mm (ES-Probe)/Zoom Scan (7x7x7) /Cube 0: Measurement


grid: dx=5mm, dy=5mm, dz=5mm

Reference Value = 102.1 V/m; Power Drift = 0.05 dB

Peak SAR (extrapolated) = 26.631 W/kg


SAR(1 g) = 13 mW/g; SAR(10 g) = 6.09 mW/g

Maximum value of SAR (measured) = 16.606 mW/g

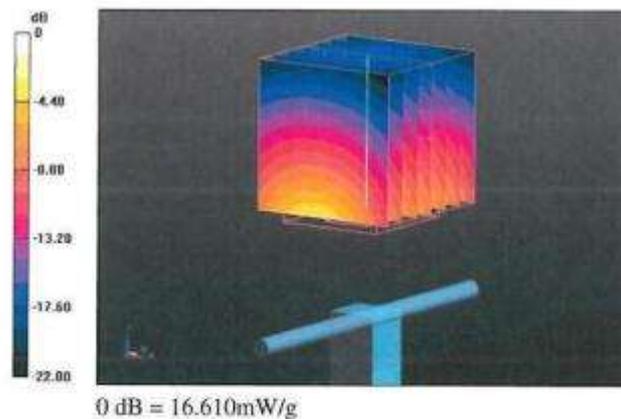



Impedance Measurement Plot for Head TSL

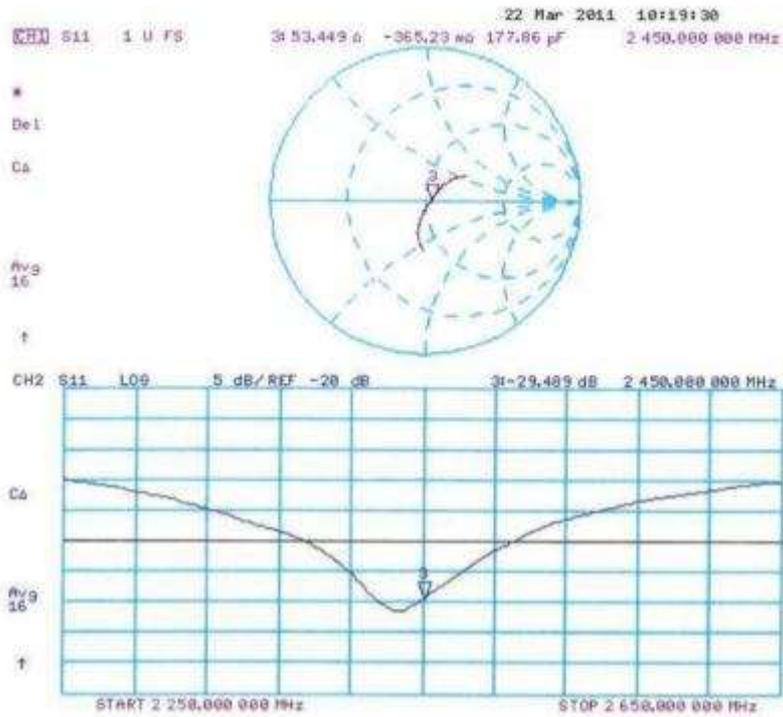

**DASY5 Validation Report for Body TSL**

Date/Time: 21.03.2011 13:50:01

Test Laboratory: SPEAG, Zurich, Switzerland

DUT: Dipole 2450 MHz; Type: D2450V2; Serial: D2450V2 - SN:715

Communication System: CW; Frequency: 2450 MHz; Duty Cycle: 1:1

Medium: MSL U12 BB

Medium parameters used: $f = 2450$ MHz; $\sigma = 1.92$ mho/m; $\epsilon_r = 51.5$; $\rho = 1000$ kg/m³

Phantom section: Flat Section

Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2007)

DASY5 Configuration:

- Probe: ES3DV3 - SN3205; ConvF(4.31, 4.31, 4.31); Calibrated: 30.04.2010
- Sensor-Surface: 3mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn601; Calibrated: 10.06.2010
- Phantom: Flat Phantom 5.0 (back); Type: QD000P50AA; Serial: 1002
- Measurement SW: DASY52, V52.6.2 Build (424)
- Postprocessing SW: SEMCAD X, V14.4.4 Build (2829)

Pin=250 mW /d=10mm, dist=3.0mm (ES-Probe)/Zoom Scan (7x7x7) /Cube 0: Measurement


grid: dx=5mm, dy=5mm, dz=5mm

Reference Value = 96.265 V/m; Power Drift = 0.0074 dB

Peak SAR (extrapolated) = 26.996 W/kg

SAR(1 g) = 12.8 mW/g; SAR(10 g) = 5.95 mW/g

Maximum value of SAR (measured) = 16.835 mW/g

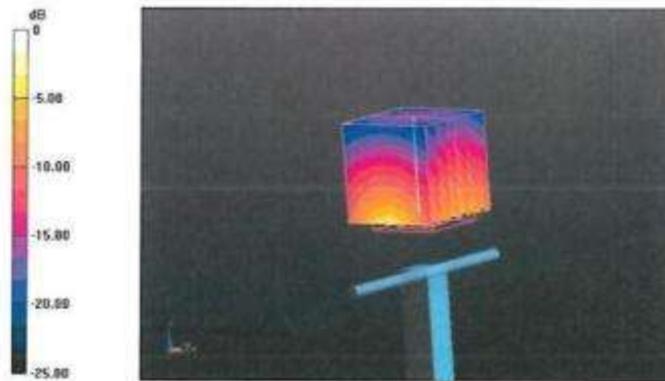


0 dB = 16.840mW/g



Product Service

Impedance Measurement Plot for Body TSL

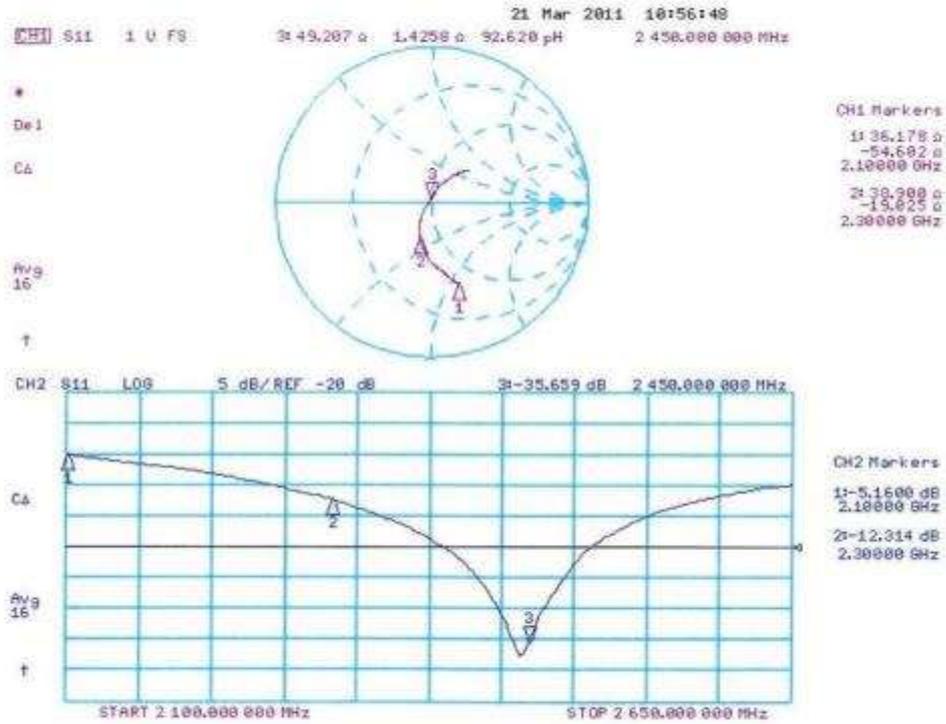



Product Service

**Calibration Laboratory of
Schmid & Partner
Engineering AG**
Zeughausstrasse 43, 8004 Zurich, Switzerland



S Schweizerischer Kalibrierdienst
C Service suisse d'étalonnage
S Servizio svizzero di taratura
S Swiss Calibration Service

Accredited by the Swiss Accreditation Service (SAS)
The Swiss Accreditation Service is one of the signatories to the EA
Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: **SCS 108**

Client **TÜV Product Service Ltd**

Certificate No: **D5GHzV2-1100_Mar11**

CALIBRATION CERTIFICATE

Object: **D5GHzV2 - SN: 1100**

Calibration procedure(s): **QA CAL-22.v1
Calibration procedure for dipole validation kits between 3-6 GHz**

Calibration date: **March 14, 2011**

This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI).
The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility: environment temperature (22 ± 3)°C and humidity < 70%.

Calibration Equipment used (M&TE critical for calibration)

Primary Standards	ID #	Cal Date (Certificate No.)	Scheduled Calibration
Power meter EPM-442A	GB37480704	08-Oct-10 (No. 217-01266)	Oct-11
Power sensor HP 8461A	US37292783	08-Oct-10 (No. 217-01266)	Oct-11
Reference 20 dB Attenuator	SN: 5086 (20g)	30-Mar-10 (No. 217-01158)	Mar-11
Type-N mismatch combination	SN: 5047.2 / 06327	30-Mar-10 (No. 217-01162)	Mar-11
Reference Probe EX3DV4	SN: 3503	04-Mar-11 (No. EX3-3503_Mar11)	Mar-12
DAE4	SN: 601	10-Jun-10 (No. DAE4-601_Jun10)	Jun-11
Secondary Standards	ID #	Check Date (in house)	Scheduled Check
Power sensor HP 8481A	MY41092317	18-Oct-02 (in house check Oct-09)	in house check: Oct-11
RF generator R&S SMT-06	100005	4-Aug-99 (in house check Oct-09)	in house check: Oct-11
Network Analyzer HP 8753E	US37390585 S4206	18-Oct-01 (in house check Oct-10)	in house check: Oct-11

	Name	Function	Signature
Calibrated by:	Dimce Iliev	Laboratory Technician	
Approved by:	Katja Pokovic	Technical Manager	

Issued: March 16, 2011

This calibration certificate shall not be reproduced except in full without written approval of the laboratory.



Product Service

**Calibration Laboratory of
Schmid & Partner
Engineering AG**
Zeughausstrasse 43, 8004 Zurich, Switzerland



S Schweizerischer Kalibrierdienst
C Service suisse d'étalonnage
S Servizio svizzero di taratura
S Swiss Calibration Service

Accredited by the Swiss Accreditation Service (SAS)
The Swiss Accreditation Service is one of the signatories to the EA
Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: **SCS 108****Glossary:**

TSL	tissue simulating liquid
ConvF	sensitivity in TSL / NORM x,y,z
N/A	not applicable or not measured

Calibration is Performed According to the Following Standards:

- IEC 62209-2, "Evaluation of Human Exposure to Radio Frequency Fields from Handheld and Body-Mounted Wireless Communication Devices in the Frequency Range of 30 MHz to 6 GHz: Human models, Instrumentation, and Procedures"; Part 2: "Procedure to determine the Specific Absorption Rate (SAR) for including accessories and multiple transmitters", March 2010
- Federal Communications Commission Office of Engineering & Technology (FCC OET), "Evaluating Compliance with FCC Guidelines for Human Exposure to Radiofrequency Electromagnetic Fields; Additional Information for Evaluating Compliance of Mobile and Portable Devices with FCC Limits for Human Exposure to Radiofrequency Emissions", Supplement C (Edition 01-01) to Bulletin 65

Additional Documentation:

- DASY4/5 System Handbook

Methods Applied and Interpretation of Parameters:

- Measurement Conditions:** Further details are available from the Validation Report at the end of the certificate. All figures stated in the certificate are valid at the frequency indicated.
- Antenna Parameters with TSL:** The dipole is mounted with the spacer to position its feed point exactly below the center marking of the flat phantom section, with the arms oriented parallel to the body axis.
- Feed Point Impedance and Return Loss:** These parameters are measured with the dipole positioned under the liquid filled phantom. The impedance stated is transformed from the measurement at the SMA connector to the feed point. The Return Loss ensures low reflected power. No uncertainty required.
- Electrical Delay:** One-way delay between the SMA connector and the antenna feed point. No uncertainty required.
- SAR measured:** SAR measured at the stated antenna input power.
- SAR normalized:** SAR as measured, normalized to an input power of 1 W at the antenna connector.
- SAR for nominal TSL parameters:** The measured TSL parameters are used to calculate the nominal SAR result.



Measurement Conditions

DASY system configuration, as far as not given on page 1.

DASY Version	DASY5	V52.6.2
Extrapolation	Advanced Extrapolation	
Phantom	Modular Flat Phantom V5.0	
Distance Dipole Center - TSL	10 mm	with Spacer
Area Scan resolution	dx, dy = 10 mm	
Zoom Scan Resolution	dx, dy = 4.0 mm, dz = 1.4 mm	
Frequency	5200 MHz ± 1 MHz 5500 MHz ± 1 MHz 5800 MHz ± 1 MHz	

Head TSL parameters at 5200 MHz

The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Head TSL parameters	22.0 °C	36.0	4.66 mho/m
Measured Head TSL parameters	(22.0 ± 0.2) °C	36.4 ± 6 %	4.51 mho/m ± 6 %
Head TSL temperature during test	(22.0 ± 0.2) °C	----	----

SAR result with Head TSL at 5200 MHz

SAR averaged over 1 cm ³ (1 g) of Head TSL	condition	
SAR measured	100 mW input power	8.31 mW / g
SAR normalized	normalized to 1W	83.1 mW / g
SAR for nominal Head TSL parameters	normalized to 1W	83.2 mW / g ± 19.9 % (k=2)

SAR averaged over 10 cm ³ (10 g) of Head TSL	condition	
SAR measured	100 mW input power	2.36 mW / g
SAR normalized	normalized to 1W	23.6 mW / g
SAR for nominal Head TSL parameters	normalized to 1W	23.6 mW / g ± 19.5 % (k=2)



Head TSL parameters at 5500 MHz

The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Head TSL parameters	22.0 °C	35.6	4.96 mho/m
Measured Head TSL parameters	(22.0 ± 0.2) °C	35.9 ± 6 %	4.80 mho/m ± 6 %
Head TSL temperature during test	(22.0 ± 0.2) °C	----	----

SAR result with Head TSL at 5500 MHz

SAR averaged over 1 cm ³ (1 g) of Head TSL	condition	
SAR measured	100 mW input power	8.98 mW / g
SAR normalized	normalized to 1W	89.8 mW / g
SAR for nominal Head TSL parameters	normalized to 1W	89.8 mW / g ± 19.9 % (k=2)

SAR averaged over 10 cm ³ (10 g) of Head TSL	condition	
SAR measured	100 mW input power	2.54 mW / g
SAR normalized	normalized to 1W	25.4 mW / g
SAR for nominal Head TSL parameters	normalized to 1W	25.4 mW / g ± 19.5 % (k=2)

Head TSL parameters at 5800 MHz

The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Head TSL parameters	22.0 °C	35.3	5.27 mho/m
Measured Head TSL parameters	(22.0 ± 0.2) °C	35.5 ± 6 %	5.10 mho/m ± 6 %
Head TSL temperature during test	(22.0 ± 0.2) °C	----	----

SAR result with Head TSL at 5800 MHz

SAR averaged over 1 cm ³ (1 g) of Head TSL	condition	
SAR measured	100 mW input power	8.39 mW / g
SAR normalized	normalized to 1W	83.9 mW / g
SAR for nominal Head TSL parameters	normalized to 1W	83.9 mW / g ± 19.9 % (k=2)

SAR averaged over 10 cm ³ (10 g) of Head TSL	condition	
SAR measured	100 mW input power	2.37 mW / g
SAR normalized	normalized to 1W	23.7 mW / g
SAR for nominal Head TSL parameters	normalized to 1W	23.7 mW / g ± 19.5 % (k=2)



Body TSL parameters at 5200 MHz

The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Body TSL parameters	22.0 °C	49.0	5.30 mho/m
Measured Body TSL parameters	(22.0 ± 0.2) °C	48.4 ± 6 %	5.48 mho/m ± 6 %
Body TSL temperature during test	(21.0 ± 0.2) °C	----	----

SAR result with Body TSL at 5200 MHz

SAR averaged over 1 cm ³ (1 g) of Body TSL	condition	
SAR measured	100 mW input power	7.70 mW / g
SAR normalized	normalized to 1W	77.0 mW / g
SAR for nominal Body TSL parameters	normalized to 1W	76.8 mW / g ± 19.9 % (k=2)

SAR averaged over 10 cm ³ (10 g) of Body TSL	condition	
SAR measured	100 mW input power	2.14 mW / g
SAR normalized	normalized to 1W	21.4 mW / g
SAR for nominal Body TSL parameters	normalized to 1W	21.4 mW / g ± 19.5 % (k=2)

Body TSL parameters at 5500 MHz

The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Body TSL parameters	22.0 °C	48.6	5.65 mho/m
Measured Body TSL parameters	(22.0 ± 0.2) °C	47.8 ± 6 %	5.85 mho/m ± 6 %
Body TSL temperature during test	(21.0 ± 0.2) °C	----	----

SAR result with Body TSL at 5500 MHz

SAR averaged over 1 cm ³ (1 g) of Body TSL	condition	
SAR measured	100 mW input power	8.22 mW / g
SAR normalized	normalized to 1W	82.2 mW / g
SAR for nominal Body TSL parameters	normalized to 1W	82.0 mW / g ± 19.9 % (k=2)

SAR averaged over 10 cm ³ (10 g) of Body TSL	condition	
SAR measured	100 mW input power	2.27 mW / g
SAR normalized	normalized to 1W	22.7 mW / g
SAR for nominal Body TSL parameters	normalized to 1W	22.7 mW / g ± 19.5 % (k=2)



Product Service

Body TSL parameters at 5800 MHz

The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Body TSL parameters	22.0 °C	48.2	6.00 mho/m
Measured Body TSL parameters	(22.0 ± 0.2) °C	47.1 ± 6 %	6.22 mho/m ± 6 %
Body TSL temperature during test	(21.0 ± 0.2) °C	---	---

SAR result with Body TSL at 5800 MHz

SAR averaged over 1 cm ² (1 g) of Body TSL	condition	
SAR measured	100 mW input power	7.61 mW / g
SAR normalized	normalized to 1W	76.1 mW / g
SAR for nominal Body TSL parameters	normalized to 1W	75.6 mW / g ± 19.9 % (k=2)

SAR averaged over 10 cm ² (10 g) of Body TSL	condition	
SAR measured	100 mW input power	2.10 mW / g
SAR normalized	normalized to 1W	21.0 mW / g
SAR for nominal Body TSL parameters	normalized to 1W	20.9 mW / g ± 19.5 % (k=2)



Appendix

Antenna Parameters with Head TSL at 5200 MHz

Impedance, transformed to feed point	52.5 Ω - 7.5 j Ω
Return Loss	-22.3 dB

Antenna Parameters with Head TSL at 5500 MHz

Impedance, transformed to feed point	48.9 Ω - 1.7 j Ω
Return Loss	-33.8 dB

Antenna Parameters with Head TSL at 5800 MHz

Impedance, transformed to feed point	51.7 Ω + 4.3 j Ω
Return Loss	-26.9 dB

Antenna Parameters with Body TSL at 5200 MHz

Impedance, transformed to feed point	53.0 Ω - 6.6 j Ω
Return Loss	-23.1 dB

Antenna Parameters with Body TSL at 5500 MHz

Impedance, transformed to feed point	49.4 Ω - 1.4 j Ω
Return Loss	-36.4 dB

Antenna Parameters with Body TSL at 5800 MHz

Impedance, transformed to feed point	52.2 Ω + 3.8 j Ω
Return Loss	-27.3 dB



Product Service

General Antenna Parameters and Design

Electrical Delay (one direction)	1.207 ns
----------------------------------	----------

After long term use with 40 W radiated power, only a slight warming of the dipole near the feedpoint can be measured.

The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals.

No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feedpoint may be damaged.

Additional EUT Data

Manufactured by	SPEAG
Manufactured on	September 24, 2010

**DASY5 Validation Report for Head TSL**

Date/Time: 11.03.2011 14:54:17

Test Laboratory: SPEAG, Zurich, Switzerland

DUT: Dipole 5GHz; Type: D5GHz; Serial: D5GHzV2 - SN:1100

Communication System: CW; Frequency: 5200 MHz, Frequency: 5500 MHz, Frequency: 5800 MHz; Duty Cycle: 1:1

Medium: HSL 5000

Medium parameters used: $f = 5200$ MHz; $\sigma = 4.51$ mho/m; $\epsilon_r = 36.4$; $\rho = 1000$ kg/m³,Medium parameters used: $f = 5500$ MHz; $\sigma = 4.8$ mho/m; $\epsilon_r = 35.9$; $\rho = 1000$ kg/m³,Medium parameters used: $f = 5800$ MHz; $\sigma = 5.1$ mho/m; $\epsilon_r = 35.5$; $\rho = 1000$ kg/m³

Phantom section: Flat Section

Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2007)

DASY5 Configuration:

- Probe: EX3DV4 - SN3503; ConvF(5.41, 5.41, 5.41), ConvF(4.91, 4.91, 4.91), ConvF(4.81, 4.81, 4.81); Calibrated: 04.03.2011
- Sensor-Surface: 1.4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn601; Calibrated: 10.06.2010
- Phantom: Flat Phantom 5.0 (front); Type: QD000P50AA; Serial: 1001
- Measurement SW: DASY52, V52.6.2 Build (424)
- Postprocessing SW: SEMCAD X, V14.4.4 Build (2829)

Pin=100mW, f=5200 MHz/Zoom Scan (4x4x1.4mm), dist=1.4mm (8x8x7)/Cube 0:

Measurement grid: dx=4mm, dy=4mm, dz=1.4mm

Reference Value = 60.701 V/m; Power Drift = 0.06 dB

Peak SAR (extrapolated) = 31.049 W/kg

SAR(1 g) = 8.31 mW/g; SAR(10 g) = 2.36 mW/g

Maximum value of SAR (measured) = 18.802 mW/g

Pin=100mW, f=5500 MHz/Zoom Scan (4x4x1.4mm), dist=1.4mm (8x8x7)/Cube 0:

Measurement grid: dx=4mm, dy=4mm, dz=1.4mm

Reference Value = 60.450 V/m; Power Drift = 0.07 dB

Peak SAR (extrapolated) = 35.828 W/kg

SAR(1 g) = 8.98 mW/g; SAR(10 g) = 2.54 mW/g

Maximum value of SAR (measured) = 21.257 mW/g

Pin=100mW, f=5800 MHz/Zoom Scan (4x4x1.4mm), dist=1.4mm (8x8x7)/Cube 0:

Measurement grid: dx=4mm, dy=4mm, dz=1.4mm

Reference Value = 57.226 V/m; Power Drift = 0.04 dB


Peak SAR (extrapolated) = 35.431 W/kg

SAR(1 g) = 8.39 mW/g; SAR(10 g) = 2.37 mW/g

Maximum value of SAR (measured) = 20.329 mW/g




Product Service

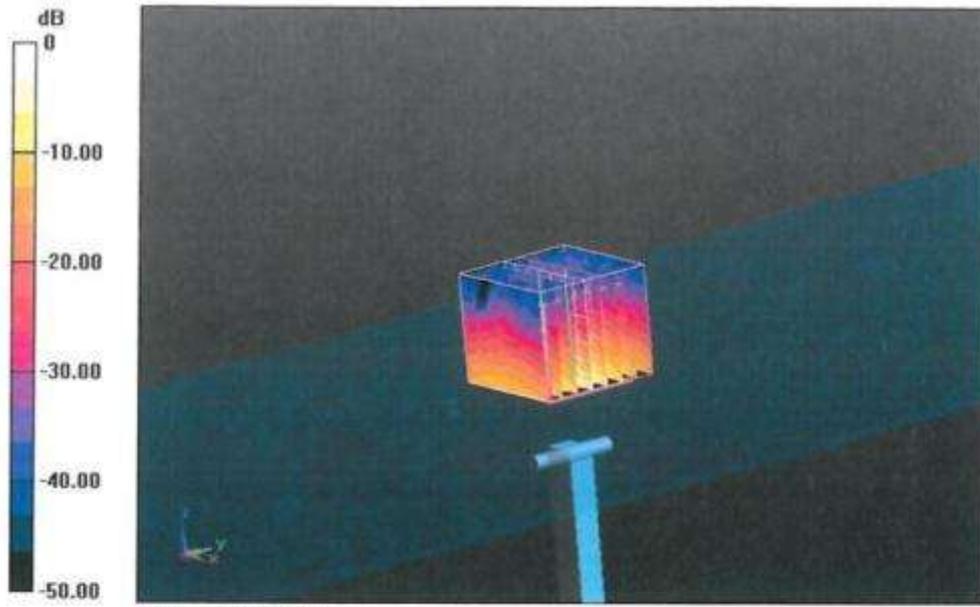

0 dB = 20.330mW/g



Impedance Measurement Plot for Head TSL

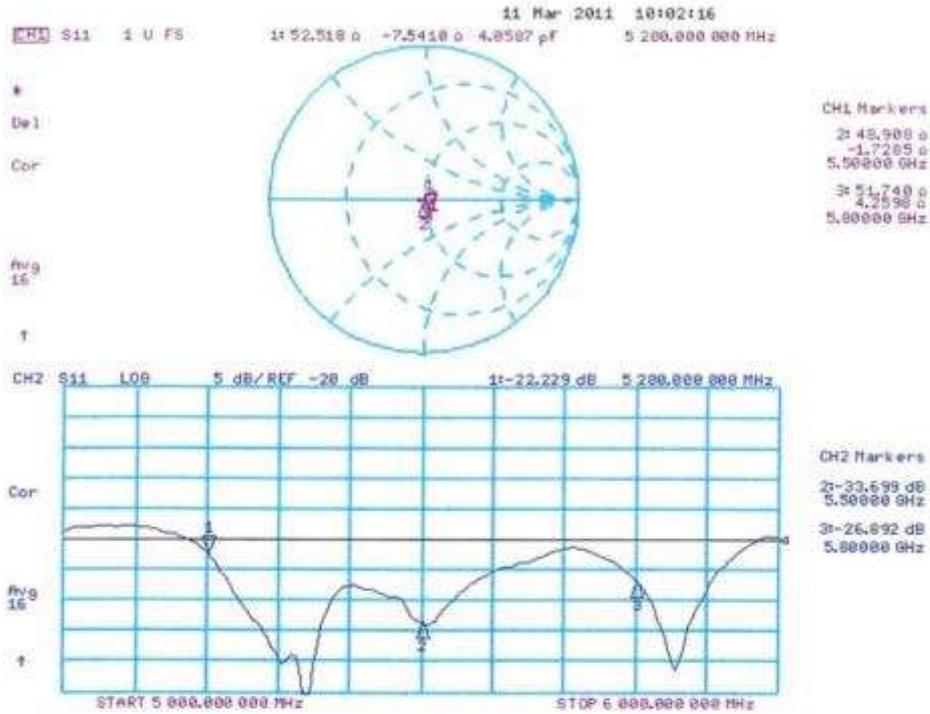

**DASY5 Validation Report for Body TSL**

Date/Time: 14.03.2011 15:25:41

Test Laboratory: SPEAG, Zurich, Switzerland

DUT: Dipole 5GHz; Type: D5GHz; Serial: D5GHzV2 - SN:1100

Communication System: CW; Frequency: 5200 MHz, Frequency: 5500 MHz, Frequency: 5800 MHz; Duty Cycle: 1:1

Medium: MSL 5000 MHz

Medium parameters used: $f = 5200$ MHz; $\sigma = 5.54$ mho/m; $\epsilon_r = 48.3$; $\rho = 1000$ kg/m³,Medium parameters used: $f = 5500$ MHz; $\sigma = 5.92$ mho/m; $\epsilon_r = 47.7$; $\rho = 1000$ kg/m³,Medium parameters used: $f = 5800$ MHz; $\sigma = 6.3$ mho/m; $\epsilon_r = 47$; $\rho = 1000$ kg/m³

Phantom section: Flat Section

Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2007)

DASY5 Configuration:

- Probe: EX3DV4 - SN3503; ConvF(4.91, 4.91, 4.91), ConvF(4.43, 4.43, 4.43), ConvF(4.38, 4.38, 4.38); Calibrated: 04.03.2011
- Sensor-Surface: 1.4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn601; Calibrated: 10.06.2010
- Phantom: Flat Phantom 5.0 (back); Type: QD000P50AA; Serial: 1002
- Measurement SW: DASY52, V52.6.2 Build (424)
- Postprocessing SW: SEMCAD X, V14.4.4 Build (2829)

Pin=100mW, f=5200 MHz/Zoom Scan (4x4x1.4mm), dist=1.4mm (8x8x7)/Cube 0:

Measurement grid: dx=4mm, dy=4mm, dz=1.4mm

Reference Value = 58.462 V/m; Power Drift = -0.0014 dB

Peak SAR (extrapolated) = 30.321 W/kg

SAR(1 g) = 7.7 mW/g; SAR(10 g) = 2.14 mW/g

Maximum value of SAR (measured) = 17.819 mW/g

Pin=100mW, f=5500 MHz/Zoom Scan (4x4x1.4mm), dist=1.4mm (8x8x7)/Cube 0:

Measurement grid: dx=4mm, dy=4mm, dz=1.4mm

Reference Value = 58.851 V/m; Power Drift = -0.03 dB

Peak SAR (extrapolated) = 35.000 W/kg

SAR(1 g) = 8.22 mW/g; SAR(10 g) = 2.27 mW/g

Maximum value of SAR (measured) = 19.554 mW/g

Pin=100mW, f=5800 MHz/Zoom Scan (4x4x1.4mm), dist=1.4mm (8x8x7)/Cube 0:

Measurement grid: dx=4mm, dy=4mm, dz=1.4mm

Reference Value = 55.021 V/m; Power Drift = -0.03 dB


Peak SAR (extrapolated) = 35.337 W/kg

SAR(1 g) = 7.61 mW/g; SAR(10 g) = 2.1 mW/g

Maximum value of SAR (measured) = 18.772 mW/g



Product Service

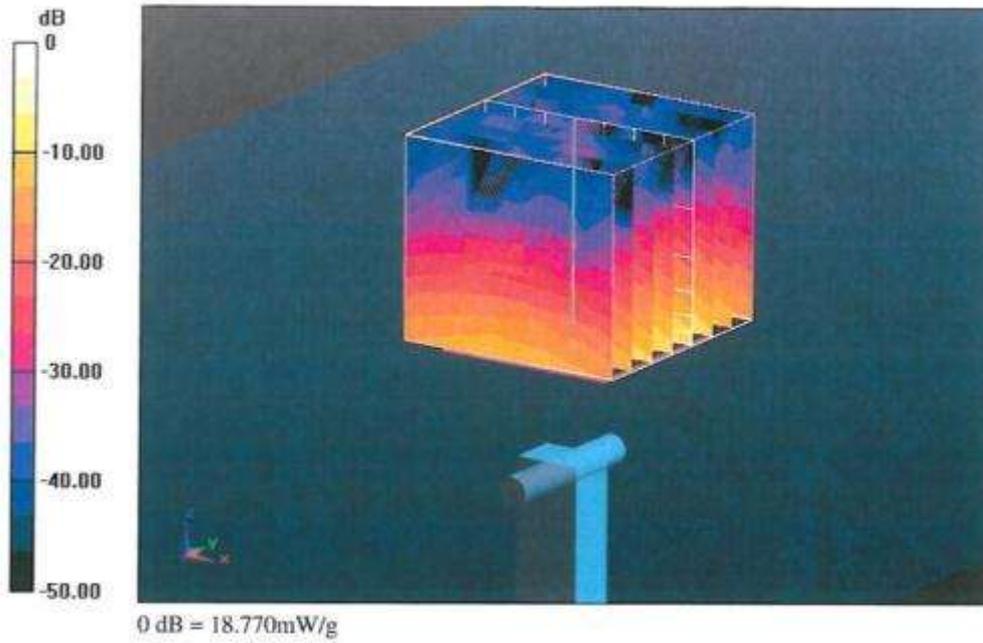



Product Service

Impedance Measurement Plot for Body TSL

