



kit, which uses the TEM method as recommended in [2].  $\sigma$  and  $\epsilon_r$  are both temperature- and fluid-dependent, so are best measured using a sample of the tissue-simulant fluid immediately prior to the actual calibration.

Wherever possible, all DiLine and calibration measurements should be made in the open laboratory at  $22 \pm 2.0^\circ\text{C}$ ; if this is not possible, the values of  $\sigma$  and  $\epsilon_r$  should reflect the actual temperature. Values employed for calibration are listed in the tables below.

By ensuring the liquid height in the waveguide is at least three penetration depths, reflections at the upper surface of the liquid are negligible. The power absorbed in the liquid is therefore determined solely from the waveguide forward and reflected power.

Different waveguides are used for 700MHz, 835/900MHz, 1450MHz, 1800/1900MHz, 2100/2450/2600MHz and 5200/5800MHz measurements. Table A.1 of [1] can be used for designing calibration waveguides with a return loss greater than 20 dB at the most important frequencies used for personal wireless communications, and better than 15dB for frequencies greater than 5GHz. Values for the penetration depth for these specific fixtures and tissue-simulating mixtures are also listed in Table A.1.

According to [1], this calibration technique provides excellent accuracy, with standard uncertainty of less than 3.6% depending on the frequency and medium. The calibration itself is reduced to power measurements traceable to a standard calibration procedure. The practical limitation to the frequency band of 800 to 5800 MHz because of the waveguide size is not severe in the context of compliance testing.

Prior to the actual calibration run, the probe must be lowered 0.01mm at a time until it is just touching the cross-sectional centre of the dielectric window, at which point live SAR readings will stop increasing. During calibration, 200 samples are taken and written to an Excel template file before moving the probe vertically upwards by one step. This cycle is repeated 150 times. The vertical separation between readings is determined from practical considerations of the expected SAR decay rate, and range from 0.2mm steps at low frequency, through 0.1mm at 2450MHz, down to 0.05mm at 5GHz.

Once the data collection is complete, a Solver routine is run which optimises the measured-theoretical fit by varying the conversion factor, and the boundary correction size and range.

For calibrations at 450MHz, where waveguide calibrations become unfeasible, a full 3D SAR scan over a tuned dipole is performed, and the conversion factor adjusted to make the measured 1g and 10g volume-averaged SAR values agree with published targets.



**CALIBRATION FACTORS MEASURED FOR PROBE S/N G0014**

The probe was calibrated at 5.2, 5.5 and 5.8GHz in liquid samples representing brain and body liquid at these frequencies.

The calibration was for CW signals only, and the axis of the probe was parallel to the direction of propagation of the incident field i.e. end-on to the incident radiation. The axial isotropy of the probe was measured by rotating the probe about its axis in 10 degree steps through 360 degrees in this orientation.

The reference point for the calibration is in the centre of the probe's cross-section at a distance of 1.39 mm from the probe tip in the direction of the probe amplifier. A value of 1.39 mm should be used for the tip to sensor offset distance in the software. The distance of 1.39mm for assembled probes has been confirmed by taking X-ray images of the probe tips (see Figure 4).

It is important that the diode compression point and air factors used in the software are the same as those quoted in the results tables, as these are used to convert the diode output voltages to a SAR value.

**CALIBRATION EQUIPMENT**

The table on page 20 indicates the calibration status of all test equipment used during probe calibration.

**MEASUREMENT UNCERTAINTIES**

A complete measurement uncertainty analysis for the SARA-C measurement system has been published in Reference [6]. Table 17 from that document is re-created below, and lists the uncertainty factors associated just with the calibration of probes.

| Source of uncertainty         | Uncertainty value $\pm$ % | Probability distribution | Divisor | $c_i$ | Standard uncertainty $u_i \pm$ % | $v_i$ or $v_{eff}$ |
|-------------------------------|---------------------------|--------------------------|---------|-------|----------------------------------|--------------------|
| Forward power                 | 3.92                      | N                        | 1.00    | 1     | 3.92                             | $\infty$           |
| Reflected power               | 4.09                      | N                        | 1.00    | 1     | 4.09                             | $\infty$           |
| Liquid conductivity           | 1.308                     | N                        | 1.00    | 1     | 1.31                             | $\infty$           |
| Liquid permittivity           | 1.271                     | N                        | 1.00    | 1     | 1.27                             | $\infty$           |
| Field homogeneity             | 3.0                       | R                        | 1.73    | 1     | 1.73                             | $\infty$           |
| Probe positioning             | 0.22                      | R                        | 1.73    | 1     | 0.13                             | $\infty$           |
| Field probe linearity         | 0.2                       | R                        | 1.73    | 1     | 0.12                             | $\infty$           |
| Combined standard uncertainty |                           | RSS                      |         |       | 6.20                             |                    |

At the 95% confidence level, therefore, the expanded uncertainty is  $\pm 12.4\%$



**SUMMARY OF CAL FACTORS FOR PROBE IXP-025 S/N G0014**

| Relative Channel Sensitivities<br>(to optimise Axial Isotropy) |        |        |        |                        |
|--|--------|--------|--------|------------------------|
|  | X      | Y      | Z      |                        |
| <b>Air Factors*</b>  | 343.22 | 245.00 | 371.78 | (V/m) <sup>2</sup> /mV |
| <b>DCPs</b>  | 100    | 100    | 100    | mV                     |

| Measured Isotropy | (+/-)<br>dB |
|-------------------|-------------|
| Axial Isotropy    | 0.07        |

| Physical Information       |      |
|----------------------------|------|
| Sensor offset (mm)         | 1.39 |
| Elbow – Tip dimension (mm) | 0.0  |

| SAR Conversion Factors/ Boundary Corrections |                                  |                          |                           |                 |                          |                           |       |
|--|----------------------------------|--------------------------|---------------------------|-----------------|--------------------------|---------------------------|-------|
| Frequency*<br>(MHz)                          | Head Fluid                       |                          |                           | Body Fluid      |                          |                           | Notes |
|  | SAR Conv Factor                  | Boundary Correction f(θ) | Boundary Correction d(mm) | SAR Conv Factor | Boundary Correction f(θ) | Boundary Correction d(mm) |       |
| <b>5200</b>                                  | 0.56                             | 0.65                     | 0.8                       | 0.59            | 0.67                     | 0.8                       | 1,2   |
| <b>5500</b>                                  | 0.54                             | 0.63                     | 0.8                       | 0.63            | 0.72                     | 0.8                       | 1,2   |
| <b>5800</b>                                  | 0.55                             | 1.24                     | 0.6                       | 0.67            | 0.82                     | 0.7                       | 1,2   |
| Notes  |                                  |                          |                           |                 |                          |                           |       |
| 1)   | Calibrations done at 22°C +/-2°C |                          |                           |                 |                          |                           |       |
| 2)   | Waveguide calibration            |                          |                           |                 |                          |                           |       |
| 3)   | By interpolation                 |                          |                           |                 |                          |                           |       |

\*The valid frequency of SARA-C probe calibrations are ±100MHz (F<300MHz) and ±200MHz (F>300MHz).



## PROBE SPECIFICATIONS

Indexsar probe G0014, along with its calibration, is compared with BSEN 62209-1 and IEEE standards recommendations (Refs [1] and [2]) in the Tables below. A listing of relevant specifications is contained in the tables below:

| <b>Dimensions</b>                              | S/N G0014 | BSEN [1] | IEEE [2] |
|--|-----------|----------|----------|
| Overall length (mm)                            | 350       |          |          |
| Tip length (mm)                                | 10        |          |          |
| Body diameter (mm)                             | 12        |          |          |
| Tip diameter (mm)                              | 2.55      | 8        | 8        |
| Distance from probe tip to dipole centers (mm) | 1.39      |          |          |

| <b>Typical Dynamic range</b>   | S/N G0014 | BSEN [1] | IEEE [2] |
|--|-----------|----------|----------|
| Minimum (W/kg)   | 0.01      | <0.02    | 0.01     |
| Maximum (W/kg)<br>N.B. only measured to > 100 W/kg<br>on representative probes | >100      | >100     | 100      |

| <b>Isotropy (measured at 5200MHz)</b>               | S/N G0014 | BSEN [1] | IEEE [2] |
|---|-----------|----------|----------|
| Axial rotation with probe normal to source (+/- dB) | <0.07     | 0.5      | 0.25     |

|                            |  |
|----------------------------|--|
| <b>Construction</b>        | Each probe contains three orthogonal dipole sensors arranged on a triangular prism core, protected against static charges by built-in shielding, and covered at the tip by PEEK cylindrical enclosure material. No adhesives are used in the immersed section. Outer case materials are PEEK and heat-shrink sleeving. |
| <b>Chemical resistance</b> | Tested to be resistant to TWEEN20 and sugar/salt-based simulant liquids but probes should be removed, cleaned and dried when not in use.<br><br>NOT recommended for use with glycol or soluble oil-based liquids.  |

**REFERENCES**

References are either specific (identified by date of publication, edition number, version number, etc.) or non-specific.

For a specific reference, subsequent revisions do not apply.

For a non-specific reference, the latest version applies.

- [1] IEC 62209-1.  
Human exposure to radio frequency fields from hand-held and body-mounted wireless communication devices — Human models, instrumentation, and procedures — Part 1: Procedure to determine the specific absorption rate (SAR) for hand-held devices used in close proximity to the ear (frequency range of 300 MHz to 3 GHz)
- [2] IEEE 1528  
Recommended Practice for Determining the Peak Spatial-Average Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques
- [3] IEC 62209-2  
Human exposure to radio frequency fields from hand-held and body-mounted wireless communication devices – Human models, instrumentation, and procedures – Part 2: Procedure to determine the specific absorption rate (SAR) for wireless communication devices used in close proximity to the human body (frequency range of 30 MHz to 6 GHz)
- [4] FCC OET65  
Evaluating Compliance with FCC Guidelines for Human Exposure to Radiofrequency Electromagnetic Fields
- [5] Indexsar Report IXS-0300, October 2007.  
Measurement uncertainties for the SARA2 system assessed against the recommendations of BS EN 62209-1:2006
- [6] SARA-C SAR Testing System: Measurement Uncertainty, v1.0.3. October 2011.

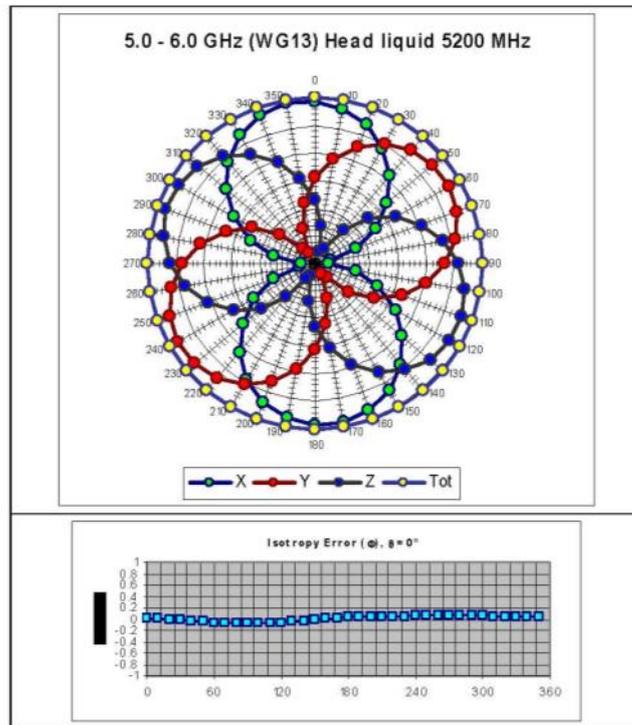


Figure 1. The axial isotropy of probe S/N G0014 obtained by rotating the probe in a liquid-filled waveguide at 5200 MHz. (NB Axial Isotropy is largely independent of frequency)

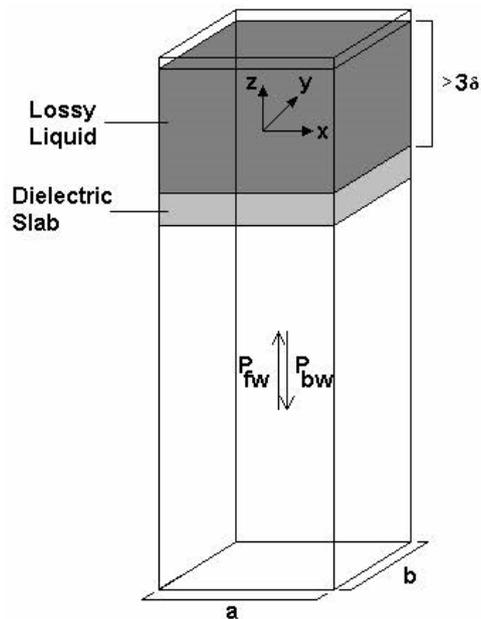


Figure 2. Geometry used for waveguide calibration (after Ref [2]. Section A.3.2.2)

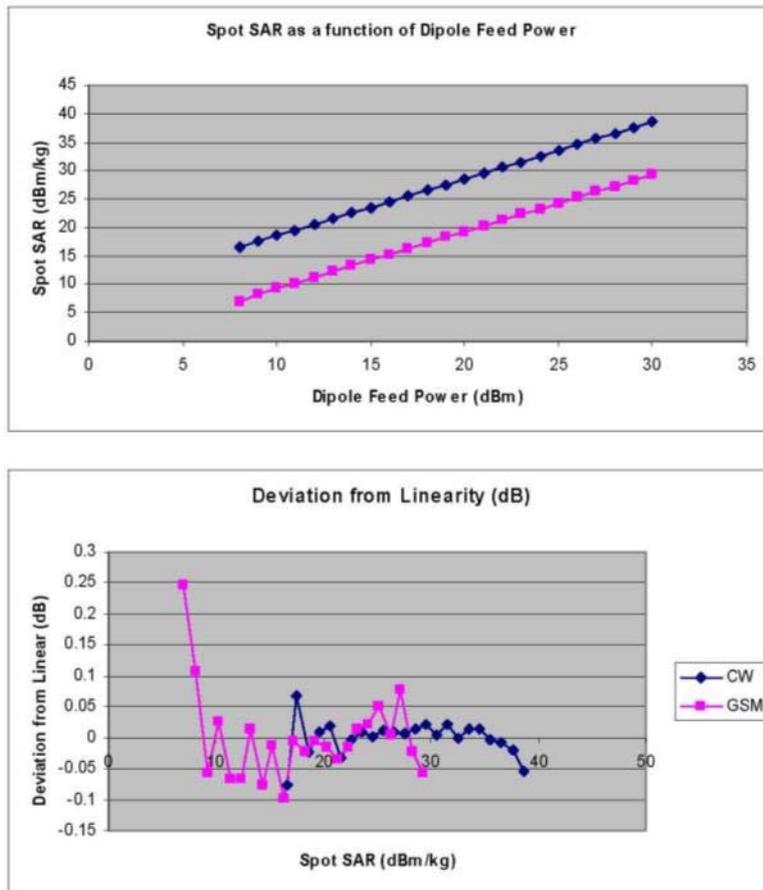


Figure 3 : The typical linearity response of IXP-025 probes to both CW (blue) and GSM (pink) modulation in close proximity to a source dipole. The top diagram shows the SAR reading as a function of dipole feed power, with GSM modulation being approx a factor of 8 (ie 9dB) lower than CW. The lower diagram shows the departure from linearity of the same two datasets.

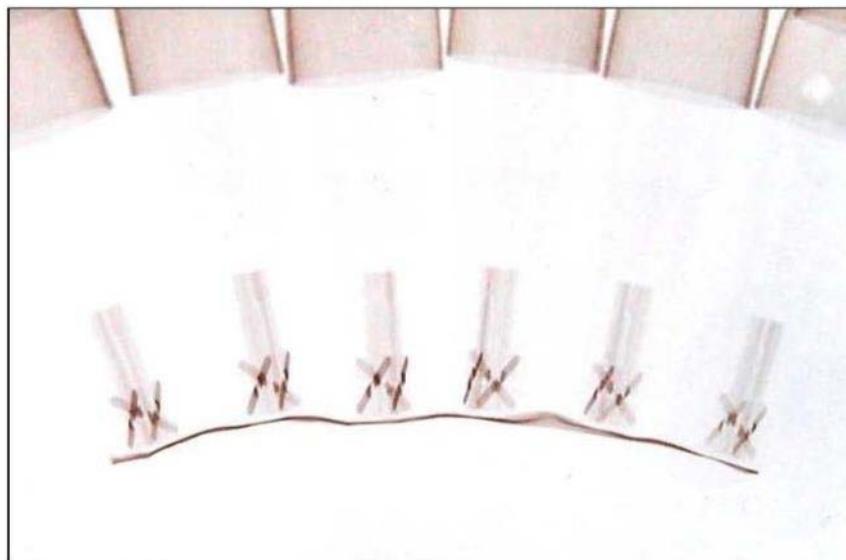


Figure 4 : X-ray positive image of 5mm probes. 2.5mm probes are similar



Table indicating the dielectric parameters of the liquids used for calibrations at each frequency

| Frequency (MHz) | Fluid Type | Measured              |                    | Target                |                    | % Deviation           |              | Verdict               |              |
|-----------------|------------|-----------------------|--------------------|-----------------------|--------------------|-----------------------|--------------|-----------------------|--------------|
|                 |            | Relative Permittivity | Conductivity (S/m) | Relative Permittivity | Conductivity (S/m) | Relative Permittivity | Conductivity | Relative Permittivity | Conductivity |
| 5200            | Head       | 37.01                 | 4.82               | 36.0                  | 4.66               | 2.8                   | 3.3          | Pass                  | Pass         |
| 5500            |            | 36.34                 | 5.12               | 35.7                  | 4.97               | 1.9                   | 3.0          | Pass                  | Pass         |
| 5800            |            | 35.61                 | 5.47               | 35.3                  | 5.27               | 0.9                   | 3.7          | Pass                  | Pass         |
| 5200            | Body       | 49.19                 | 5.30               | 49.0                  | 5.30               | 0.4                   | -0.1         | Pass                  | Pass         |
| 5500            |            | 48.38                 | 5.62               | 48.6                  | 5.65               | -0.5                  | -0.5         | Pass                  | Pass         |
| 5800            |            | 47.41                 | 6.06               | 48.2                  | 6.00               | -1.6                  | 1.1          | Pass                  | Pass         |

Table of test equipment calibration status at time of calibration

| Instrument description          | Supplier / Manufacturer | Model   | Serial No. | Last calibration date   | Cal certificate number | See Annex | Calibration due date |
|---------------------------------|-------------------------|---|------------|---|------------------------|-----------|----------------------|
| Power sensor                    | Rohde & Schwarz         | NRP-Z23                                       | 100063     | 14/08/2013  | 10-300287035           | 1         | 14/08/2015           |
| Dielectric property measurement | Indexsar                | DILine (sensor lengths: 160mm, 80mm and 60mm) | N/A        | (absolute) – checked against NPL values using reference liquids | N/A                    |           | N/A                  |
| Vector network analyser         | Anritsu                 | MS6423B                                       | 003102     | 21/01/2014  | RMA20021769            | 2         | 21/01/2015           |
| SMA autocalibration module      | Anritsu                 | 36581KKF/1                                    | 001902     | 21/01/2014  | RMA20021769            | 2         | 21/01/2015           |



Product Service

Annex 1

Calibration Certificate of NRP-Z23 power sensor

|   |   |   |
|---|---|---|
|   |   | <b>Calibration Certificate</b><br>Certificate Number 10-300287035 |
| <b>Kalibrierschein</b>  |   | <b>Zertifikatsnummer</b>  |
| <b>Unit Data</b>  |   |   |
| Item<br>Gegenstand  | Average power sensor  |   |
| Manufacturer<br>Hersteller  | ROHDE & SCHWARZ   |   |
| Type<br>Typ   | NRP-Z23   |   |
| Material Number<br>Materialnummer   | 1137.8002.02  | Serial Number<br>Seriennummer 100063                              |
| Asset Number<br>Inventarnummer  |   |   |
| <b>Order Data</b>   |   |   |
| Customer<br>Auftraggeber  | IndexSAR Ltd  |   |
|   | Oakfield House,<br>RH5 5BG Newdigate<br>GB  |   |
| Order Number<br>Bestellnummer   |   |   |
| Date of Receipt<br>Eingangsdatum  | 2013-08-08  |   |
| <b>Performance</b>  |   |   |
| Place and Date of Calibration<br>Ort und Datum der Kalibrierung   | Memmingen, 2013-08-14   |   |
| Scope of Calibration<br>Umfang der Kalibrierung   | Standard Calibration  |   |
| Statement of Compliance<br>(Incoming)<br>Konformitätsaussage<br>(Anlieferung)   | Measurement results within specifications   |   |
| Statement of Compliance<br>(Outgoing)<br>Konformitätsaussage<br>(Auslieferung)  | Measurement results within specifications   |   |
| Extent of Calibration Documents<br>Umfang des Kalibrierdokuments  | 2 Pages Calibration Certificate<br>17 Pages Outgoing Results<br>17 Pages Incoming Results |   |
| This calibration certificate documents, that the named item is tested and measured against defined specifications. Measurement results are located usually in the corresponding interval with a probability of approx. 95% (coverage factor k = 2). Calibration is performed with test equipment and standards directly or indirectly traceable by means of approved calibration techniques to the PTB/DKD or other national / international standards, which realize the physical units of measurement according to the International System of Units (SI). In all cases where no standards are available, measurements are referenced to standards of the R&S laboratories. Principles and methods of calibration correspond with EN ISO/IEC 17025. The applied quality system is certified to EN ISO 9001. This calibration certificate may not be reproduced other than in full. Calibration certificates without signatures are not valid. The user is obliged to have the object recalibrated at appropriate intervals.   |   |   |
| Dieser Kalibrierschein dokumentiert, dass der genannte Gegenstand nach festgelegten Vorgaben geprüft und gemessen wurde. Die Messwerte lagen im Regelfall mit einer Wahrscheinlichkeit von annähernd 95% im zugeordneten Wertesintervall (Erweiterte Messunsicherheit mit k = 2). Die Kalibrierung erfolgte mit Messmitteln und Normalen, die direkt oder indirekt durch Ableitung mittels anerkannter Kalibriertechniken rückgeführt sind auf Normale der PTB/DKD oder anderer nationaler/internationaler Standards zur Darstellung der physikalischen Einheiten in Übereinstimmung mit dem internationalen Einheitensystem (SI). Wenn keine Normale existieren, erfolgt die Rückführung auf Bezugnormale der R&S-Laboratorien. Grundsätze und Verfahren der Kalibrierung entsprechen EN ISO/IEC 17025. Das angewandte Qualitätsmanagement-System ist zertifiziert nach EN ISO 9001. Dieser Kalibrierschein darf nur vollständig und unverändert weiterverbreitet werden. Kalibrierscheine ohne Signifizierungen sind ungültig. Für die Einhaltung einer angemessenen Frist zur Wiederholung der Kalibrierung ist der Benutzer verantwortlich. |   |   |
| <b>Rohde &amp; Schwarz GmbH &amp; Co. KG; Service Operations West</b>   |   |   |
| Date of Issue<br>Ausstellungsdatum  | Head of Laboratory<br>Laborleitung  | Person Responsible<br>Bearbeiter                                  |
| 2013-08-14  | <br>Courage   | <br>Ruprecht Schmid   |
|   |   | Page 1/2<br>ver0815RSM0606  |
| ROHDE & SCHWARZ GmbH & Co. KG · Mühlhofstraße 15 · D-81671 München, Federal Republic of Germany · Telefon (089) 41 29-0 · Telefax (089) 41 29-132 75<br>Geschäftsführung: Manfred Fleischmann (Vorsitzender), Christian Lecher, Gerhard Geier<br>Sitz München · Registeramt: HRA 18 270 · Persönlich haftender Gesellschafter: RUSEG Verwaltungs-GmbH · Sitz München · Registeramt: AG München HRB 7 834  |   |   |



Product Service

Material Number 1137.8002.02      Serial Number 100063      Certificate Number 10-300287035

Calibration Method      **NRVC-1109.0930.32**      Relative Humidity      **20%-60%**  
 Kalibrieranweisung           Relative Luftfeuchte  
 Ambient Temperature      **(23 <sup>+1</sup> <sub>-1</sub>) °C**  
 Umgebungstemperatur

| Working standards used (having a significant effect on the accuracy)<br>Verwendete Gebrauchsnormale (mit signifikantem Einfluss auf die Genauigkeit) |             |                               |   |                         |
|--|-------------|-------------------------------|---|-------------------------|
| Item<br>Gegenstand   | Type<br>Typ | Serial Number<br>Seriennummer | Calibration Certificate Number<br>Kalibrierscheinnummer | Cal. Due<br>Kalibr. bis |
| Dual Channel Powermeter  | NRVD        | 100862                        | 0114 D-K-15195-01-00 2013-08                            | 2014-11-30              |
| Dual Channel Power Meter   | NRVD        | 828583/0023                   | 0113 D-K-15195-01-00 2013-08                            | 2014-11-30              |
| Vector Network Analyzer  | ZVM         | 835228/0020                   | 0102-DKD-K-16101-2011-08                                | 2013-10-31              |
| Access Set for Lin. Measurement  | NRVC-B2     | 848997/0028                   | 0085 D-K-15195-01-00 2013-01                            | 2014-04-30              |
| Calibration Kit Type-N ;50 Ohm   | 85054B      | .2705A00160                   | 217-01723 [METAS]                                       | 2015-03-31              |
| Power Standard   | NRVC        | 836497/0005                   | 0082 D-K-15195-01-00 2013-01                            | 2014-04-30              |

Conformity statements take the measurement uncertainties into account.  
 Die Konformitätsaussagen berücksichtigen die Messunsicherheiten.

Notes  
 Anmerkungen

Installed options are included in calibration. Depending on installed options, numbers of pages of the record are not consecutive.



Product Service

**Annex 2**

Calibration certificate of MS4623 VNA and 36581KKF/1 auto-cal kit

| Certificate of Calibration   |  | Anritsu  |
|--|--|--|
|  |  | Discover What's Possible™  |
| Customer:<br>INDEXSAR LTD<br>INDEXSAR LTD_   | ANRITSU EMEA LIMITED<br>200 CAPABILITY GREEN<br>LUTON LU1 3LU<br>UNITED KINGDOM<br>Tel: +44 (0) 1582 433285<br>Fax: +44 (0) 1582 455575<br>Email: service_esc@eu.anritsu.com |  |
| OAKFIELD HOUSE<br>NEWDIGATE<br>SURREY RH5 5BG<br>UNITED KINGDOM  |  |  |
| <b>Date of Issue:</b> 21/01/2014   | <b>Certificate N°:</b> RMA20021769   |  |
| <b>Customer:</b> INDEXSAR LTD  | <b>Order N°:</b> Contract  |  |
| <b>Manufacturer:</b> Anritsu Company   |  |  |
| Model  | Serial Number  | Description  |
| MS4623B  | 003102   | VNA,10 MHZ-6 GHZ,ACTIVE  |
| 36581KKF/1   | 001902   | TESTED & CHARACTERIZED TO 6 GHZ  |
| <p>Anritsu EMEA Limited does hereby certify the above listed equipment complies to published or stated specifications at the measured parameters, and has been calibrated to the general requirements of ISO 17025 against instruments whose accuracies are traceable to National or International Standards, where such standards are applicable.</p>   |  |  |
| Within specification before calibration  | ( yes )  | <br>Murray Coleman<br>Head of Customer Services (EMEA) |
| Repair required before calibration   | ( no )   |  |
| Electrical Safety  | ( yes )  |  |
| Laser safety class   | ( )  |  |
| <p>Note: Original calibration results are attached and copies held on file at Anritsu EMEA Limited.<br/>                     The attached results relate only to the instrument under calibration.<br/>                     Anritsu EMEA Limited Quality system is certified to ISO9001:2000 (Cert. No. FQA 0353170).<br/>                     This Certificate comprises of:<br/>                     Certificate of Calibration<br/>                     Call Report<br/>                     25 Page(s) of test results</p> |  |  |



Product Service

## **ANNEX B**

### **DIPOLE CALIBRATION REPORTS**



Product Service

Test Equipment Number (TE): 4413

Calibration Class: A

## TUV SUD Product Service

### Internal Calibration Laboratory Report

Date of Calibration: 18/03/2014

Report Number: 26602

Calibration Expiry Date: 18/03/2017

Page 1 of 6

It is certified that the test(s) detailed in the above Calibration Report have been carried out to the requirement of the specification, unless otherwise stated above. The quality control arrangements adopted in respect of these tests have accorded with the conditions of our UKAS registration. The uncertainties are for an estimated confidence probability of not less than 95%.

**Manufacturer:** IndexSar Ltd**Item:** Dipoles**Model:** 700**Serial No:** 0279**Calibration Procedure, as per:** CP036/CAL

The results recorded, were taken after a warm up period of 1 Hour(s) in an ambient temperature of  $23.2^{\circ}\text{C} \pm 3^{\circ}\text{C}$  @ 29.3% RH  $\pm 10\%$  RH. The mains voltage was  $240\text{V} \pm 10\%$ .

**Calibration Engineer:** \_\_\_\_\_ 

N. R. Grigsby

**Approved Signatory:** \_\_\_\_\_ 

A. T. Pearce



## CALIBRATION LABORATORY REPORT

TUV SUD Product ServiceCalibration Classification and Key to Results

**(X) Class A:** All results measured, lie within the specification limits, even when extended by their measurement uncertainties. The instrument therefore complies with the specification.

**( ) Class B:** Some/all results measured, lie INSIDE the specification limits, by a margin less than their measurement uncertainties. It is therefore not possible to state compliance of these results. However, these results indicate that compliance is more probable than non-compliance. (\*\*\*)

**( ) Class C:** Some/all results measured, lie OUTSIDE the specification limits, by a margin less than their measurement uncertainties. It is therefore not possible to state compliance of these results. However, these results indicate that non-compliance is more probable than compliance. (\*\*)

**( ) Class D:** Some/all results measured, lie OUTSIDE the specification limits, by a margin greater than their measurement uncertainties. Those results therefore, do not comply with the specification. (\*)

**( ) Class R:** The instrument was repaired prior to calibration. Refer to enclosed repair report for details.

Test Equipment Used On This Calibration

| Make & Model                                    | Description                           | Calibration Due | TE ID  |
|---|---------------------------------------|-----------------|--------|
| Rohde & Schwarz: NRV-Z1                         | Power Sensor                          | 14/06/2014      | TE0060 |
| Hewlett Packard: ESG4000A                       | Signal Generator                      | 22/05/2014      | TE0061 |
| Narda: 766F-20                                  | Attenuator (20dB, 20W)                | 13/06/2014      | TE0483 |
| Hewlett Packard: 8753D                          | Network Analyser                      | 23/04/2014      | TE1149 |
| Hewlett Packard: 85054A                         | 'N' Calibration Kit                   | 24/12/2014      | TE1309 |
| IndexSar Ltd: 7401 (VDC0830-20)                 | Bi-directional Coupler                |                 | TE2414 |
| IndexSar Ltd: VBM2500-3                         | Validation Amplifier (10MHz - 2.5GHz) |                 | TE2415 |
| Rotronic: I-1000                                | Hygromer                              | 03/04/2014      | TE2784 |
| Rohde & Schwarz: NRV- Z5                        | Power Sensor                          | 14/06/2014      | TE2878 |
| Rohde & Schwarz: NRVD                           | Dual Channel Power Meter              | 14/06/2014      | TE3259 |
| R.S Components: Meter 615-8206 & Type K T/C     | Meter & T/C                           | 08/07/2014      | TE3612 |
| IndexSar Ltd: SARAC                             | Cartesian 4-axis Robot                |                 | TE4079 |
| IndexSar Ltd: White Benchtop                    | Part of SARAC System                  |                 | TE4080 |
| IndexSar Ltd: Wooden Bench                      | Part of SARAC System                  |                 | TE4081 |
| IndexSar Ltd: IPX-050                           | Immersible SAR Probe                  | 07/03/2015      | TE4313 |
| IndexSar Ltd: IXB-2HF 700- 6000MHz Flat Phantom | TE4400                                |                 |        |



**CALIBRATION LABORATORY REPORT**

**Dipole impedance and return loss**

The dipoles are designed to have low return loss ONLY when presented against a lossy-phantom at the specified distance. A Vector Network Analyser (VNA) was used to perform a return loss measurement on the specific dipole when in the measurement-location against the box phantom. The distance was as specified in the standard i.e. 15mm from the liquid (for 700MHz).

The impedance was measured at the SMA-connector with the network analyser. The following parameters were measured against Head fluid:



|                            |                          |
|----------------------------|--------------------------|
| Dipole impedance at 700MHz | $Re\{Z\} = 52.35 \Omega$ |
| Return loss at 700MHz      | $Im\{Z\} = -3.65 \Omega$ |
|                            | <b>-27.29 dB</b>         |

Standards [1][2][3][4] call for dipoles to have a return loss better than 20dB

The measurements repeated against Body fluid:





**CALIBRATION LABORATORY REPORT**

|                              |                  |
|------------------------------|------------------|
| Dipole impedance at 700MHz   | Re{Z} = 51.215 Ω |
| <b>Return loss at 700MHz</b> | Im{Z} = -7.51 Ω  |
|                              | <b>-22.58 dB</b> |

Standards [1][2][3][4] call for dipoles to have a return loss better than 20dB

**SAR Validation Measurement in Brain Fluid**


SAR validation checks have been performed using the 700MHz dipole and the box-phantom located on the SARA-C phantom support base on the SARA-C robot system. Tests were then conducted at a feed power level of approx. 0.25W. The actual power level was recorded and used to normalise the results obtained to the standard input power conditions of 1W (forward power). The ambient temperature was 23.2°C and the relative humidity was 29.3% during the measurements.

The phantom was filled with 700MHz brain liquid using a recipe from [1], which has the following electrical parameters (measured using an Indexsar DiLine kit) at 700MHz at the measurement temperature:

|                       |                  |
|-----------------------|------------------|
| Relative Permittivity | <b>42.6</b>      |
| Conductivity          | <b>0.896 S/m</b> |
| Fluid Temperature     | 22.6 °C          |

The SARA-C software version v6.08.11 was used with Indexsar IXP\_050 probe Serial Number 204 previously calibrated using waveguides.

The 3D measurement made using the dipole at the bottom of the phantom box is shown below:

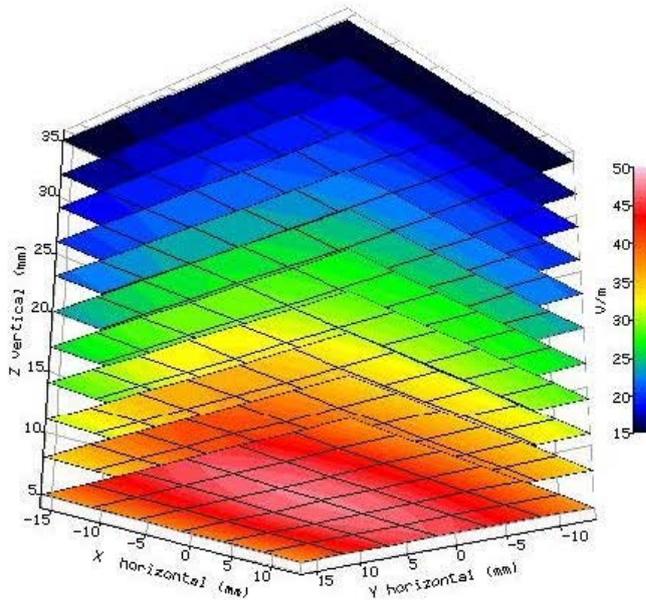



**CALIBRATION LABORATORY REPORT**

The validation results normalised to an input power of 1W (forward power) were:

|                | Measured SAR values (W/kg) (250mW input power) | Measured SAR values (W/kg) (Normalised to 1W feed power) and % Variance from target Value. |            | Target SAR values (W/kg) derived from system validation (Normalised to 1W feed power) |
|----------------|--|--|------------|---|
|                |  | Measured   | % Variance |   |
| <b>1g SAR</b>  | 1.94   | 7.72   | 0.64       | 7.67  |
| <b>10g SAR</b> | 1.30   | 5.16   | 0.97       | 5.11  |

All validation measurements are with ± 10% of Target values as required in standards [1][2][3][4]

**SAR Measurement in Body Fluid**


SAR validation checks have been performed using the 700MHz dipole and the box-phantom located on the SARA-C phantom support base on the SARA-C robot system. Tests were then conducted at a feed power level of approx. 0.25W. The actual power level was recorded and used to normalise the results obtained to the standard input power conditions of 1W (forward power). The ambient temperature was 23.3°C and the relative humidity was 30.9% during the measurements.

The phantom was filled with 700MHz body liquid using a recipe from [1][4], which has the following electrical parameters (measured using an Indxsar DiLine kit) at 700MHz at the measurement temperature:

Relative Permittivity           **55.4**  
 Conductivity                   **0.988 S/m**  
 Fluid Temperature           **22.7 °C**

The SARA-C software version v6.08.11 was used with Indxsar IXP\_050 probe Serial Number 204 previously calibrated using waveguides.

The 3D measurement made using the dipole at the bottom of the phantom box is shown below:

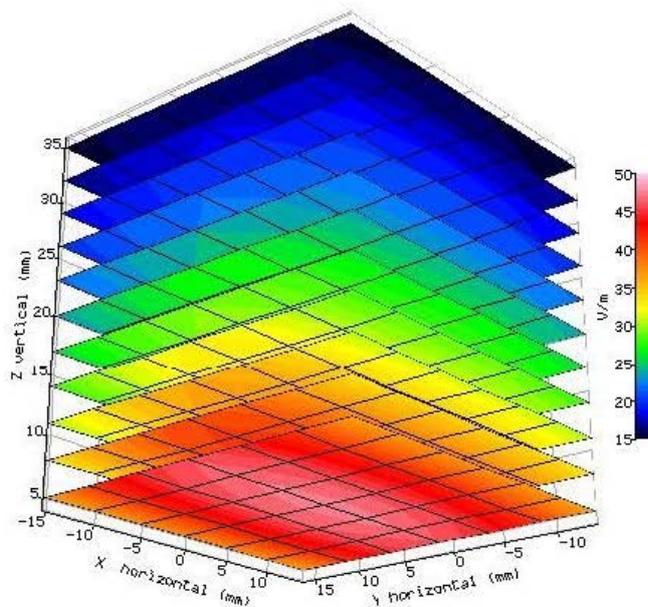



**CALIBRATION LABORATORY REPORT**

The validation results normalised to an input power of 1W (forward power) were:

|                | Measured SAR values (W/kg) (250mW input power) | Measured SAR values (W/kg) (Normalised to 1W feed power) and % Variance from target Value. |            | Target SAR values (W/kg) derived from system validation (Normalised to 1W feed power) |
|----------------|--|--|------------|---|
|                |  | Measured   | % Variance |   |
| <b>1g SAR</b>  | 2.061  | 8.20   | 6.97**     | 7.67*   |
| <b>10g SAR</b> | 1.40   | 5.57   | 8.91**     | 5.11*   |

\* In the specifications, SAR validation target values are only define for standardised measurements in brain fluid. Using the target values (W/kg) derived from system validation with brain fluid the validation measurements are within ± 10% of Target values.

\*\*Variance against target values (W/kg) derived from system validation with brain fluid.

**References**

[1] IEEE Std 1528-2013. IEEE recommended practice for determining the peak spatial-average specific absorption rate (SAR) in the human body due to wireless communications devices: Measurement Techniques – Description.

[2]BS EN 62209-1:2006 Human exposure to radio frequency fields from hand-held and body-mounted wireless communication devices — Human models, instrumentation, and procedures — Part 1: Procedure to determine the specific absorption rate (SAR) for hand-held devices used in close proximity to the ear (frequency range of 300 MHz to 3 GHz).

[3]BS EN 62209-2:2010 Human exposure to radio frequency fields from hand-held and body-mounted wireless communication devices — Human models, instrumentation, and procedures — Part 2: Procedure to determine the specific absorption rate (SAR) for hand-held devices used in close proximity to the human body (frequency range of 300 MHz to 6 GHz) (IEC 62209-2:2010)

[4] FCC KDB 865664 D01 SAR Measurement 100MHz to 6GHz V01r03



Product Service

**Calibration Laboratory of  
Schmid & Partner  
Engineering AG**  
Zeughausstrasse 43, 8004 Zurich, Switzerland



**S** Schweizerischer Kalibrierdienst  
**C** Service suisse d'étalonnage  
**S** Servizio svizzero di taratura  
**S** Swiss Calibration Service

Accredited by the Swiss Accreditation Service (SAS)  
The Swiss Accreditation Service is one of the signatories to the EA  
Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: **SCS 0108**

Client **TÜV SÜD UK**

Certificate No: **D835V2-447\_Nov15**

**CALIBRATION CERTIFICATE**

| Object   | D835V2 - SN: 447   |                                   |                        |                   |      |                            |                       |                      |            |                           |        |                       |            |                           |        |                       |            |                           |        |                            |                |                           |        |                             |                    |                           |        |                        |          |                                |        |      |         |                                |        |                     |      |                       |                 |                         |        |                                   |                        |                           |                  |                                   |                        |
|--|--|-----------------------------------|------------------------|-------------------|------|----------------------------|-----------------------|----------------------|------------|---------------------------|--------|-----------------------|------------|---------------------------|--------|-----------------------|------------|---------------------------|--------|----------------------------|----------------|---------------------------|--------|-----------------------------|--------------------|---------------------------|--------|------------------------|----------|--------------------------------|--------|------|---------|--------------------------------|--------|---------------------|------|-----------------------|-----------------|-------------------------|--------|-----------------------------------|------------------------|---------------------------|------------------|-----------------------------------|------------------------|
| Calibration procedure(s)   | QA CAL-05.v9<br>Calibration procedure for dipole validation kits above 700 MHz |                                   |                        |                   |      |                            |                       |                      |            |                           |        |                       |            |                           |        |                       |            |                           |        |                            |                |                           |        |                             |                    |                           |        |                        |          |                                |        |      |         |                                |        |                     |      |                       |                 |                         |        |                                   |                        |                           |                  |                                   |                        |
| Calibration date:  | November 12, 2015  |                                   |                        |                   |      |                            |                       |                      |            |                           |        |                       |            |                           |        |                       |            |                           |        |                            |                |                           |        |                             |                    |                           |        |                        |          |                                |        |      |         |                                |        |                     |      |                       |                 |                         |        |                                   |                        |                           |                  |                                   |                        |
| <p>This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI).<br/>The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.</p> <p>All calibrations have been conducted in the closed laboratory facility: environment temperature (22 ± 3)°C and humidity &lt; 70%.</p> <p>Calibration Equipment used (M&amp;TE critical for calibration)</p> <table border="1"> <thead> <tr> <th>Primary Standards</th> <th>ID #</th> <th>Cal Date (Certificate No.)</th> <th>Scheduled Calibration</th> </tr> </thead> <tbody> <tr> <td>Power meter EPM-442A</td> <td>GB37480704</td> <td>07-Oct-15 (No. 217-02222)</td> <td>Oct-16</td> </tr> <tr> <td>Power sensor HP 8481A</td> <td>US37292783</td> <td>07-Oct-15 (No. 217-02222)</td> <td>Oct-16</td> </tr> <tr> <td>Power sensor HP 8481A</td> <td>MY41092317</td> <td>07-Oct-15 (No. 217-02223)</td> <td>Oct-16</td> </tr> <tr> <td>Reference 20 dB Attenuator</td> <td>SN: 5058 (20k)</td> <td>01-Apr-15 (No. 217-02131)</td> <td>Mar-16</td> </tr> <tr> <td>Type-N mismatch combination</td> <td>SN: 5047.2 / 06327</td> <td>01-Apr-15 (No. 217-02134)</td> <td>Mar-16</td> </tr> <tr> <td>Reference Probe EX3DV4</td> <td>SN: 7349</td> <td>30-Dec-14 (No. EX3-7349_Dec14)</td> <td>Dec-15</td> </tr> <tr> <td>DAE4</td> <td>SN: 601</td> <td>17-Aug-15 (No. DAE4-601_Aug15)</td> <td>Aug-16</td> </tr> </tbody> </table><br><table border="1"> <thead> <tr> <th>Secondary Standards</th> <th>ID #</th> <th>Check Date (in house)</th> <th>Scheduled Check</th> </tr> </thead> <tbody> <tr> <td>RF generator R&amp;S SMT-06</td> <td>100972</td> <td>15-Jun-15 (in house check Jun-15)</td> <td>In house check: Jun-16</td> </tr> <tr> <td>Network Analyzer HP 8753E</td> <td>US37390585 S4206</td> <td>18-Oct-01 (in house check Oct-15)</td> <td>In house check: Oct-16</td> </tr> </tbody> </table> |  |                                   |                        | Primary Standards | ID # | Cal Date (Certificate No.) | Scheduled Calibration | Power meter EPM-442A | GB37480704 | 07-Oct-15 (No. 217-02222) | Oct-16 | Power sensor HP 8481A | US37292783 | 07-Oct-15 (No. 217-02222) | Oct-16 | Power sensor HP 8481A | MY41092317 | 07-Oct-15 (No. 217-02223) | Oct-16 | Reference 20 dB Attenuator | SN: 5058 (20k) | 01-Apr-15 (No. 217-02131) | Mar-16 | Type-N mismatch combination | SN: 5047.2 / 06327 | 01-Apr-15 (No. 217-02134) | Mar-16 | Reference Probe EX3DV4 | SN: 7349 | 30-Dec-14 (No. EX3-7349_Dec14) | Dec-15 | DAE4 | SN: 601 | 17-Aug-15 (No. DAE4-601_Aug15) | Aug-16 | Secondary Standards | ID # | Check Date (in house) | Scheduled Check | RF generator R&S SMT-06 | 100972 | 15-Jun-15 (in house check Jun-15) | In house check: Jun-16 | Network Analyzer HP 8753E | US37390585 S4206 | 18-Oct-01 (in house check Oct-15) | In house check: Oct-16 |
| Primary Standards  | ID #   | Cal Date (Certificate No.)        | Scheduled Calibration  |                   |      |                            |                       |                      |            |                           |        |                       |            |                           |        |                       |            |                           |        |                            |                |                           |        |                             |                    |                           |        |                        |          |                                |        |      |         |                                |        |                     |      |                       |                 |                         |        |                                   |                        |                           |                  |                                   |                        |
| Power meter EPM-442A   | GB37480704   | 07-Oct-15 (No. 217-02222)         | Oct-16                 |                   |      |                            |                       |                      |            |                           |        |                       |            |                           |        |                       |            |                           |        |                            |                |                           |        |                             |                    |                           |        |                        |          |                                |        |      |         |                                |        |                     |      |                       |                 |                         |        |                                   |                        |                           |                  |                                   |                        |
| Power sensor HP 8481A  | US37292783   | 07-Oct-15 (No. 217-02222)         | Oct-16                 |                   |      |                            |                       |                      |            |                           |        |                       |            |                           |        |                       |            |                           |        |                            |                |                           |        |                             |                    |                           |        |                        |          |                                |        |      |         |                                |        |                     |      |                       |                 |                         |        |                                   |                        |                           |                  |                                   |                        |
| Power sensor HP 8481A  | MY41092317   | 07-Oct-15 (No. 217-02223)         | Oct-16                 |                   |      |                            |                       |                      |            |                           |        |                       |            |                           |        |                       |            |                           |        |                            |                |                           |        |                             |                    |                           |        |                        |          |                                |        |      |         |                                |        |                     |      |                       |                 |                         |        |                                   |                        |                           |                  |                                   |                        |
| Reference 20 dB Attenuator   | SN: 5058 (20k)   | 01-Apr-15 (No. 217-02131)         | Mar-16                 |                   |      |                            |                       |                      |            |                           |        |                       |            |                           |        |                       |            |                           |        |                            |                |                           |        |                             |                    |                           |        |                        |          |                                |        |      |         |                                |        |                     |      |                       |                 |                         |        |                                   |                        |                           |                  |                                   |                        |
| Type-N mismatch combination  | SN: 5047.2 / 06327   | 01-Apr-15 (No. 217-02134)         | Mar-16                 |                   |      |                            |                       |                      |            |                           |        |                       |            |                           |        |                       |            |                           |        |                            |                |                           |        |                             |                    |                           |        |                        |          |                                |        |      |         |                                |        |                     |      |                       |                 |                         |        |                                   |                        |                           |                  |                                   |                        |
| Reference Probe EX3DV4   | SN: 7349   | 30-Dec-14 (No. EX3-7349_Dec14)    | Dec-15                 |                   |      |                            |                       |                      |            |                           |        |                       |            |                           |        |                       |            |                           |        |                            |                |                           |        |                             |                    |                           |        |                        |          |                                |        |      |         |                                |        |                     |      |                       |                 |                         |        |                                   |                        |                           |                  |                                   |                        |
| DAE4   | SN: 601  | 17-Aug-15 (No. DAE4-601_Aug15)    | Aug-16                 |                   |      |                            |                       |                      |            |                           |        |                       |            |                           |        |                       |            |                           |        |                            |                |                           |        |                             |                    |                           |        |                        |          |                                |        |      |         |                                |        |                     |      |                       |                 |                         |        |                                   |                        |                           |                  |                                   |                        |
| Secondary Standards  | ID #   | Check Date (in house)             | Scheduled Check        |                   |      |                            |                       |                      |            |                           |        |                       |            |                           |        |                       |            |                           |        |                            |                |                           |        |                             |                    |                           |        |                        |          |                                |        |      |         |                                |        |                     |      |                       |                 |                         |        |                                   |                        |                           |                  |                                   |                        |
| RF generator R&S SMT-06  | 100972   | 15-Jun-15 (in house check Jun-15) | In house check: Jun-16 |                   |      |                            |                       |                      |            |                           |        |                       |            |                           |        |                       |            |                           |        |                            |                |                           |        |                             |                    |                           |        |                        |          |                                |        |      |         |                                |        |                     |      |                       |                 |                         |        |                                   |                        |                           |                  |                                   |                        |
| Network Analyzer HP 8753E  | US37390585 S4206   | 18-Oct-01 (in house check Oct-15) | In house check: Oct-16 |                   |      |                            |                       |                      |            |                           |        |                       |            |                           |        |                       |            |                           |        |                            |                |                           |        |                             |                    |                           |        |                        |          |                                |        |      |         |                                |        |                     |      |                       |                 |                         |        |                                   |                        |                           |                  |                                   |                        |
| Calibrated by:   | Name<br>Jeton Kastrati   | Function<br>Laboratory Technician | Signature<br>          |                   |      |                            |                       |                      |            |                           |        |                       |            |                           |        |                       |            |                           |        |                            |                |                           |        |                             |                    |                           |        |                        |          |                                |        |      |         |                                |        |                     |      |                       |                 |                         |        |                                   |                        |                           |                  |                                   |                        |
| Approved by:   | Name<br>Katja Pokovic  | Function<br>Technical Manager     | Signature<br>          |                   |      |                            |                       |                      |            |                           |        |                       |            |                           |        |                       |            |                           |        |                            |                |                           |        |                             |                    |                           |        |                        |          |                                |        |      |         |                                |        |                     |      |                       |                 |                         |        |                                   |                        |                           |                  |                                   |                        |
| Issued: November 12, 2015  |  |                                   |                        |                   |      |                            |                       |                      |            |                           |        |                       |            |                           |        |                       |            |                           |        |                            |                |                           |        |                             |                    |                           |        |                        |          |                                |        |      |         |                                |        |                     |      |                       |                 |                         |        |                                   |                        |                           |                  |                                   |                        |
| This calibration certificate shall not be reproduced except in full without written approval of the laboratory.  |  |                                   |                        |                   |      |                            |                       |                      |            |                           |        |                       |            |                           |        |                       |            |                           |        |                            |                |                           |        |                             |                    |                           |        |                        |          |                                |        |      |         |                                |        |                     |      |                       |                 |                         |        |                                   |                        |                           |                  |                                   |                        |



Product Service

**Calibration Laboratory of  
Schmid & Partner  
Engineering AG**  
Zeughausstrasse 43, 8004 Zurich, Switzerland



**S** Schweizerischer Kalibrierdienst  
**C** Service suisse d'étalonnage  
**S** Servizio svizzero di taratura  
**S** Swiss Calibration Service

Accredited by the Swiss Accreditation Service (SAS)  
The Swiss Accreditation Service is one of the signatories to the EA  
Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: **SCS 0108**

**Glossary:**

TSL tissue simulating liquid  
ConvF sensitivity in TSL / NORM x,y,z  
N/A not applicable or not measured

**Calibration is Performed According to the Following Standards:**

- a) IEEE Std 1528-2013, "IEEE Recommended Practice for Determining the Peak Spatial-Averaged Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques", June 2013
- b) IEC 62209-1, "Procedure to measure the Specific Absorption Rate (SAR) for hand-held devices used in close proximity to the ear (frequency range of 300 MHz to 3 GHz)", February 2005
- c) IEC 62209-2, "Procedure to determine the Specific Absorption Rate (SAR) for wireless communication devices used in close proximity to the human body (frequency range of 30 MHz to 6 GHz)", March 2010
- d) KDB 865664, "SAR Measurement Requirements for 100 MHz to 6 GHz"

**Additional Documentation:**

- e) DASY4/5 System Handbook

**Methods Applied and Interpretation of Parameters:**

- *Measurement Conditions:* Further details are available from the Validation Report at the end of the certificate. All figures stated in the certificate are valid at the frequency indicated.
- *Antenna Parameters with TSL:* The dipole is mounted with the spacer to position its feed point exactly below the center marking of the flat phantom section, with the arms oriented parallel to the body axis.
- *Feed Point Impedance and Return Loss:* These parameters are measured with the dipole positioned under the liquid filled phantom. The impedance stated is transformed from the measurement at the SMA connector to the feed point. The Return Loss ensures low reflected power. No uncertainty required.
- *Electrical Delay:* One-way delay between the SMA connector and the antenna feed point. No uncertainty required.
- *SAR measured:* SAR measured at the stated antenna input power.
- *SAR normalized:* SAR as measured, normalized to an input power of 1 W at the antenna connector.
- *SAR for nominal TSL parameters:* The measured TSL parameters are used to calculate the nominal SAR result.

The reported uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor k=2, which for a normal distribution corresponds to a coverage probability of approximately 95%.



### Measurement Conditions

DASY system configuration, as far as not given on page 1.

|                              |                        |             |
|------------------------------|------------------------|-------------|
| DASY Version                 | DASY5                  | V52.8.8     |
| Extrapolation                | Advanced Extrapolation |             |
| Phantom                      | Modular Flat Phantom   |             |
| Distance Dipole Center - TSL | 15 mm                  | with Spacer |
| Zoom Scan Resolution         | dx, dy, dz = 5 mm      |             |
| Frequency                    | 835 MHz $\pm$ 1 MHz    |             |

### Head TSL parameters

The following parameters and calculations were applied.

|   | Temperature         | Permittivity   | Conductivity         |
|---|---------------------|----------------|----------------------|
| Nominal Head TSL parameters             | 22.0 °C             | 41.5           | 0.90 mho/m           |
| Measured Head TSL parameters            | (22.0 $\pm$ 0.2) °C | 42.6 $\pm$ 6 % | 0.92 mho/m $\pm$ 6 % |
| Head TSL temperature change during test | < 0.5 °C            | ----           | ----                 |

### SAR result with Head TSL

| SAR averaged over 1 cm <sup>3</sup> (1 g) of Head TSL | Condition          |                              |
|---|--------------------|------------------------------|
| SAR measured  | 250 mW input power | 2.34 W/kg                    |
| SAR for nominal Head TSL parameters                   | normalized to 1W   | 9.26 W/kg $\pm$ 17.0 % (k=2) |

| SAR averaged over 10 cm <sup>3</sup> (10 g) of Head TSL | condition          |                              |
|---|--------------------|------------------------------|
| SAR measured  | 250 mW input power | 1.52 W/kg                    |
| SAR for nominal Head TSL parameters                     | normalized to 1W   | 6.02 W/kg $\pm$ 16.5 % (k=2) |

### Body TSL parameters

The following parameters and calculations were applied.

|   | Temperature         | Permittivity   | Conductivity         |
|---|---------------------|----------------|----------------------|
| Nominal Body TSL parameters             | 22.0 °C             | 55.2           | 0.97 mho/m           |
| Measured Body TSL parameters            | (22.0 $\pm$ 0.2) °C | 55.6 $\pm$ 6 % | 0.99 mho/m $\pm$ 6 % |
| Body TSL temperature change during test | < 0.5 °C            | ----           | ----                 |

### SAR result with Body TSL

| SAR averaged over 1 cm <sup>3</sup> (1 g) of Body TSL | Condition          |                              |
|---|--------------------|------------------------------|
| SAR measured  | 250 mW input power | 2.40 W/kg                    |
| SAR for nominal Body TSL parameters                   | normalized to 1W   | 9.47 W/kg $\pm$ 17.0 % (k=2) |

| SAR averaged over 10 cm <sup>3</sup> (10 g) of Body TSL | condition          |                              |
|---|--------------------|------------------------------|
| SAR measured  | 250 mW input power | 1.57 W/kg                    |
| SAR for nominal Body TSL parameters                     | normalized to 1W   | 6.21 W/kg $\pm$ 16.5 % (k=2) |



**Appendix (Additional assessments outside the scope of SCS 0108)**

**Antenna Parameters with Head TSL**

|                                      |                 |
|--------------------------------------|-----------------|
| Impedance, transformed to feed point | 49.9 Ω - 7.0 jΩ |
| Return Loss                          | - 23.1 dB       |

**Antenna Parameters with Body TSL**

|                                      |                 |
|--------------------------------------|-----------------|
| Impedance, transformed to feed point | 46.0 Ω - 8.7 jΩ |
| Return Loss                          | - 20.0 dB       |

**General Antenna Parameters and Design**

|                                  |          |
|----------------------------------|----------|
| Electrical Delay (one direction) | 1.386 ns |
|----------------------------------|----------|

After long term use with 100W radiated power, only a slight warming of the dipole near the feedpoint can be measured.

The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals. On some of the dipoles, small end caps are added to the dipole arms in order to improve matching when loaded according to the position as explained in the "Measurement Conditions" paragraph. The SAR data are not affected by this change. The overall dipole length is still according to the Standard.

No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feedpoint may be damaged.

**Additional EUT Data**

|                 |                  |
|-----------------|------------------|
| Manufactured by | SPEAG            |
| Manufactured on | October 24, 2001 |



## DASY5 Validation Report for Head TSL

Date: 12.11.2015

Test Laboratory: SPEAG, Zurich, Switzerland

**DUT: Dipole 835 MHz; Type: D835V2; Serial: D835V2 - SN: 447**

Communication System: UID 0 - CW; Frequency: 835 MHz

Medium parameters used:  $f = 835 \text{ MHz}$ ;  $\sigma = 0.92 \text{ S/m}$ ;  $\epsilon_r = 42.6$ ;  $\rho = 1000 \text{ kg/m}^3$

Phantom section: Flat Section

Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2011)

DASY52 Configuration:

- Probe: EX3DV4 - SN7349; ConvF(9.77, 9.77, 9.77); Calibrated: 30.12.2014;
- Sensor-Surface: 1.4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn601; Calibrated: 17.08.2015
- Phantom: Flat Phantom 4.9L; Type: QD000P49AA; Serial: 1001
- DASY52 52.8.8(1222); SEMCAD X 14.6.10(7331)

### Dipole Calibration for Head Tissue/Pin=250 mW, d=15mm/Zoom Scan (7x7x7)/Cube 0:


Measurement grid:  $dx=5\text{mm}$ ,  $dy=5\text{mm}$ ,  $dz=5\text{mm}$

Reference Value = 61.13 V/m; Power Drift = 0.03 dB

Peak SAR (extrapolated) = 3.47 W/kg


**SAR(1 g) = 2.34 W/kg; SAR(10 g) = 1.52 W/kg**

Maximum value of SAR (measured) = 3.10 W/kg

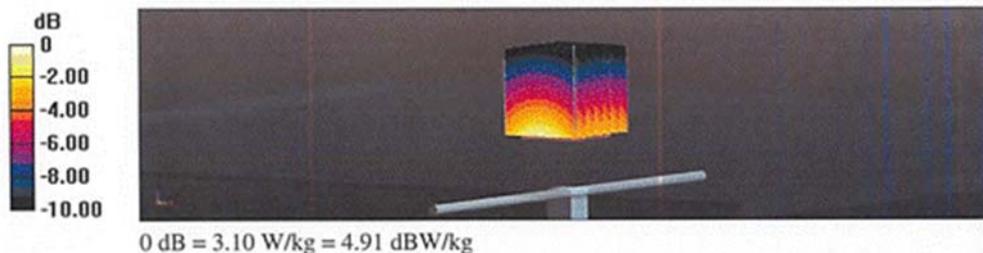



### Impedance Measurement Plot for Head TSL

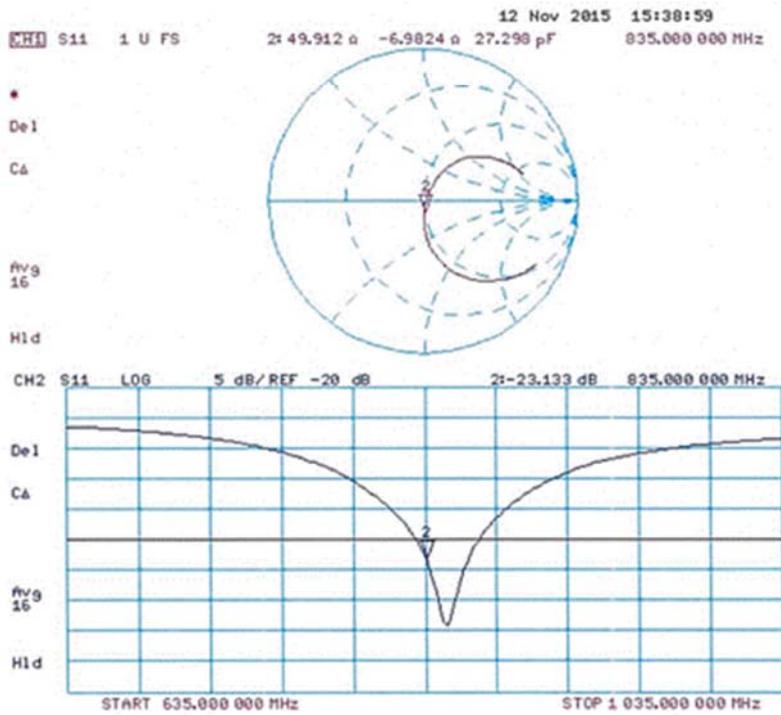



## DASY5 Validation Report for Body TSL

Date: 12.11.2015

Test Laboratory: SPEAG, Zurich, Switzerland

**DUT: Dipole 835 MHz; Type: D835V2; Serial: D835V2 - SN: 447**

Communication System: UID 0 - CW; Frequency: 835 MHz

Medium parameters used:  $f = 835$  MHz;  $\sigma = 0.99$  S/m;  $\epsilon_r = 55.6$ ;  $\rho = 1000$  kg/m<sup>3</sup>

Phantom section: Flat Section

Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2011)

DASY52 Configuration:

- Probe: EX3DV4 - SN7349; ConvF(9.72, 9.72, 9.72); Calibrated: 30.12.2014;
- Sensor-Surface: 1.4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn601; Calibrated: 17.08.2015
- Phantom: Flat Phantom 4.9L; Type: QD000P49AA; Serial: 1001
- DASY52 52.8.8(1222); SEMCAD X 14.6.10(7331)

### Dipole Calibration for Body Tissue/Pin=250 mW, d=15mm/Zoom Scan (7x7x7)/Cube 0:


Measurement grid: dx=5mm, dy=5mm, dz=5mm

Reference Value = 59.65 V/m; Power Drift = 0.02 dB

Peak SAR (extrapolated) = 3.57 W/kg


SAR(1 g) = 2.4 W/kg; SAR(10 g) = 1.57 W/kg

Maximum value of SAR (measured) = 3.17 W/kg

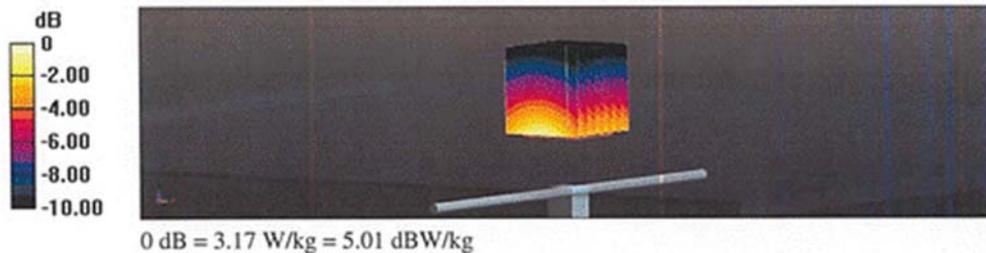



### Impedance Measurement Plot for Body TSL

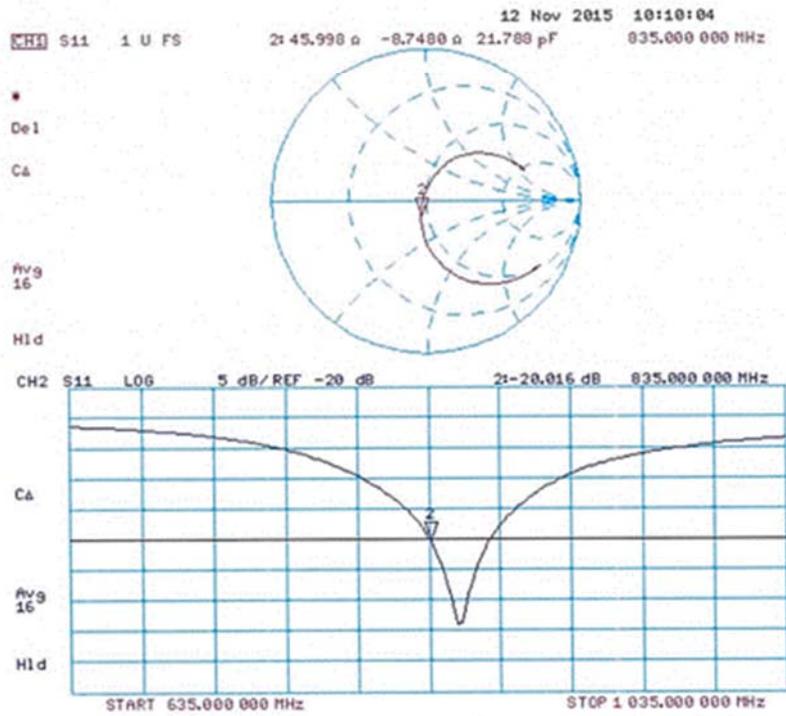



Product Service

**Calibration Laboratory of  
Schmid & Partner  
Engineering AG**  
Zeughausstrasse 43, 8004 Zurich, Switzerland



**S** Schweizerischer Kalibrierdienst  
**C** Service suisse d'étalonnage  
**S** Servizio svizzero di taratura  
**S** Swiss Calibration Service

Accredited by the Swiss Accreditation Service (SAS)  
The Swiss Accreditation Service is one of the signatories to the EA  
Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: **SCS 0108**

Client **TüV SÜD UK**

Certificate No: **D835V2-447\_Nov15**

**CALIBRATION CERTIFICATE**

| Object   | D835V2 - SN: 447   |                                   |                        |                   |      |                            |                       |                      |            |                           |        |                       |            |                           |        |                       |            |                           |        |                            |                |                           |        |                             |                    |                           |        |                        |          |                                |        |      |         |                                |        |                     |      |                       |                 |                         |        |                                   |                        |                           |                  |                                   |                        |
|--|--|-----------------------------------|------------------------|-------------------|------|----------------------------|-----------------------|----------------------|------------|---------------------------|--------|-----------------------|------------|---------------------------|--------|-----------------------|------------|---------------------------|--------|----------------------------|----------------|---------------------------|--------|-----------------------------|--------------------|---------------------------|--------|------------------------|----------|--------------------------------|--------|------|---------|--------------------------------|--------|---------------------|------|-----------------------|-----------------|-------------------------|--------|-----------------------------------|------------------------|---------------------------|------------------|-----------------------------------|------------------------|
| Calibration procedure(s)   | QA CAL-05.v9<br>Calibration procedure for dipole validation kits above 700 MHz |                                   |                        |                   |      |                            |                       |                      |            |                           |        |                       |            |                           |        |                       |            |                           |        |                            |                |                           |        |                             |                    |                           |        |                        |          |                                |        |      |         |                                |        |                     |      |                       |                 |                         |        |                                   |                        |                           |                  |                                   |                        |
| Calibration date:  | November 12, 2015  |                                   |                        |                   |      |                            |                       |                      |            |                           |        |                       |            |                           |        |                       |            |                           |        |                            |                |                           |        |                             |                    |                           |        |                        |          |                                |        |      |         |                                |        |                     |      |                       |                 |                         |        |                                   |                        |                           |                  |                                   |                        |
| <p>This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI).<br/>The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.</p> <p>All calibrations have been conducted in the closed laboratory facility: environment temperature (22 ± 3)°C and humidity &lt; 70%.</p> <p>Calibration Equipment used (M&amp;TE critical for calibration)</p> <table border="1"> <thead> <tr> <th>Primary Standards</th> <th>ID #</th> <th>Cal Date (Certificate No.)</th> <th>Scheduled Calibration</th> </tr> </thead> <tbody> <tr> <td>Power meter EPM-442A</td> <td>GB37480704</td> <td>07-Oct-15 (No. 217-02222)</td> <td>Oct-16</td> </tr> <tr> <td>Power sensor HP 8481A</td> <td>US37292783</td> <td>07-Oct-15 (No. 217-02222)</td> <td>Oct-16</td> </tr> <tr> <td>Power sensor HP 8481A</td> <td>MY41092317</td> <td>07-Oct-15 (No. 217-02223)</td> <td>Oct-16</td> </tr> <tr> <td>Reference 20 dB Attenuator</td> <td>SN: 5058 (20k)</td> <td>01-Apr-15 (No. 217-02131)</td> <td>Mar-16</td> </tr> <tr> <td>Type-N mismatch combination</td> <td>SN: 5047.2 / 06327</td> <td>01-Apr-15 (No. 217-02134)</td> <td>Mar-16</td> </tr> <tr> <td>Reference Probe EX3DV4</td> <td>SN: 7349</td> <td>30-Dec-14 (No. EX3-7349_Dec14)</td> <td>Dec-15</td> </tr> <tr> <td>DAE4</td> <td>SN: 601</td> <td>17-Aug-15 (No. DAE4-601_Aug15)</td> <td>Aug-16</td> </tr> </tbody> </table><br><table border="1"> <thead> <tr> <th>Secondary Standards</th> <th>ID #</th> <th>Check Date (in house)</th> <th>Scheduled Check</th> </tr> </thead> <tbody> <tr> <td>RF generator R&amp;S SMT-06</td> <td>100972</td> <td>15-Jun-15 (in house check Jun-15)</td> <td>In house check: Jun-16</td> </tr> <tr> <td>Network Analyzer HP 8753E</td> <td>US37390585 S4206</td> <td>18-Oct-01 (in house check Oct-15)</td> <td>In house check: Oct-16</td> </tr> </tbody> </table> |  |                                   |                        | Primary Standards | ID # | Cal Date (Certificate No.) | Scheduled Calibration | Power meter EPM-442A | GB37480704 | 07-Oct-15 (No. 217-02222) | Oct-16 | Power sensor HP 8481A | US37292783 | 07-Oct-15 (No. 217-02222) | Oct-16 | Power sensor HP 8481A | MY41092317 | 07-Oct-15 (No. 217-02223) | Oct-16 | Reference 20 dB Attenuator | SN: 5058 (20k) | 01-Apr-15 (No. 217-02131) | Mar-16 | Type-N mismatch combination | SN: 5047.2 / 06327 | 01-Apr-15 (No. 217-02134) | Mar-16 | Reference Probe EX3DV4 | SN: 7349 | 30-Dec-14 (No. EX3-7349_Dec14) | Dec-15 | DAE4 | SN: 601 | 17-Aug-15 (No. DAE4-601_Aug15) | Aug-16 | Secondary Standards | ID # | Check Date (in house) | Scheduled Check | RF generator R&S SMT-06 | 100972 | 15-Jun-15 (in house check Jun-15) | In house check: Jun-16 | Network Analyzer HP 8753E | US37390585 S4206 | 18-Oct-01 (in house check Oct-15) | In house check: Oct-16 |
| Primary Standards  | ID #   | Cal Date (Certificate No.)        | Scheduled Calibration  |                   |      |                            |                       |                      |            |                           |        |                       |            |                           |        |                       |            |                           |        |                            |                |                           |        |                             |                    |                           |        |                        |          |                                |        |      |         |                                |        |                     |      |                       |                 |                         |        |                                   |                        |                           |                  |                                   |                        |
| Power meter EPM-442A   | GB37480704   | 07-Oct-15 (No. 217-02222)         | Oct-16                 |                   |      |                            |                       |                      |            |                           |        |                       |            |                           |        |                       |            |                           |        |                            |                |                           |        |                             |                    |                           |        |                        |          |                                |        |      |         |                                |        |                     |      |                       |                 |                         |        |                                   |                        |                           |                  |                                   |                        |
| Power sensor HP 8481A  | US37292783   | 07-Oct-15 (No. 217-02222)         | Oct-16                 |                   |      |                            |                       |                      |            |                           |        |                       |            |                           |        |                       |            |                           |        |                            |                |                           |        |                             |                    |                           |        |                        |          |                                |        |      |         |                                |        |                     |      |                       |                 |                         |        |                                   |                        |                           |                  |                                   |                        |
| Power sensor HP 8481A  | MY41092317   | 07-Oct-15 (No. 217-02223)         | Oct-16                 |                   |      |                            |                       |                      |            |                           |        |                       |            |                           |        |                       |            |                           |        |                            |                |                           |        |                             |                    |                           |        |                        |          |                                |        |      |         |                                |        |                     |      |                       |                 |                         |        |                                   |                        |                           |                  |                                   |                        |
| Reference 20 dB Attenuator   | SN: 5058 (20k)   | 01-Apr-15 (No. 217-02131)         | Mar-16                 |                   |      |                            |                       |                      |            |                           |        |                       |            |                           |        |                       |            |                           |        |                            |                |                           |        |                             |                    |                           |        |                        |          |                                |        |      |         |                                |        |                     |      |                       |                 |                         |        |                                   |                        |                           |                  |                                   |                        |
| Type-N mismatch combination  | SN: 5047.2 / 06327   | 01-Apr-15 (No. 217-02134)         | Mar-16                 |                   |      |                            |                       |                      |            |                           |        |                       |            |                           |        |                       |            |                           |        |                            |                |                           |        |                             |                    |                           |        |                        |          |                                |        |      |         |                                |        |                     |      |                       |                 |                         |        |                                   |                        |                           |                  |                                   |                        |
| Reference Probe EX3DV4   | SN: 7349   | 30-Dec-14 (No. EX3-7349_Dec14)    | Dec-15                 |                   |      |                            |                       |                      |            |                           |        |                       |            |                           |        |                       |            |                           |        |                            |                |                           |        |                             |                    |                           |        |                        |          |                                |        |      |         |                                |        |                     |      |                       |                 |                         |        |                                   |                        |                           |                  |                                   |                        |
| DAE4   | SN: 601  | 17-Aug-15 (No. DAE4-601_Aug15)    | Aug-16                 |                   |      |                            |                       |                      |            |                           |        |                       |            |                           |        |                       |            |                           |        |                            |                |                           |        |                             |                    |                           |        |                        |          |                                |        |      |         |                                |        |                     |      |                       |                 |                         |        |                                   |                        |                           |                  |                                   |                        |
| Secondary Standards  | ID #   | Check Date (in house)             | Scheduled Check        |                   |      |                            |                       |                      |            |                           |        |                       |            |                           |        |                       |            |                           |        |                            |                |                           |        |                             |                    |                           |        |                        |          |                                |        |      |         |                                |        |                     |      |                       |                 |                         |        |                                   |                        |                           |                  |                                   |                        |
| RF generator R&S SMT-06  | 100972   | 15-Jun-15 (in house check Jun-15) | In house check: Jun-16 |                   |      |                            |                       |                      |            |                           |        |                       |            |                           |        |                       |            |                           |        |                            |                |                           |        |                             |                    |                           |        |                        |          |                                |        |      |         |                                |        |                     |      |                       |                 |                         |        |                                   |                        |                           |                  |                                   |                        |
| Network Analyzer HP 8753E  | US37390585 S4206   | 18-Oct-01 (in house check Oct-15) | In house check: Oct-16 |                   |      |                            |                       |                      |            |                           |        |                       |            |                           |        |                       |            |                           |        |                            |                |                           |        |                             |                    |                           |        |                        |          |                                |        |      |         |                                |        |                     |      |                       |                 |                         |        |                                   |                        |                           |                  |                                   |                        |
| Calibrated by:   | Name<br>Jeton Kastrati   | Function<br>Laboratory Technician | Signature<br>          |                   |      |                            |                       |                      |            |                           |        |                       |            |                           |        |                       |            |                           |        |                            |                |                           |        |                             |                    |                           |        |                        |          |                                |        |      |         |                                |        |                     |      |                       |                 |                         |        |                                   |                        |                           |                  |                                   |                        |
| Approved by:   | Name<br>Katja Pokovic  | Function<br>Technical Manager     | Signature<br>          |                   |      |                            |                       |                      |            |                           |        |                       |            |                           |        |                       |            |                           |        |                            |                |                           |        |                             |                    |                           |        |                        |          |                                |        |      |         |                                |        |                     |      |                       |                 |                         |        |                                   |                        |                           |                  |                                   |                        |
| Issued: November 12, 2015  |  |                                   |                        |                   |      |                            |                       |                      |            |                           |        |                       |            |                           |        |                       |            |                           |        |                            |                |                           |        |                             |                    |                           |        |                        |          |                                |        |      |         |                                |        |                     |      |                       |                 |                         |        |                                   |                        |                           |                  |                                   |                        |
| This calibration certificate shall not be reproduced except in full without written approval of the laboratory.  |  |                                   |                        |                   |      |                            |                       |                      |            |                           |        |                       |            |                           |        |                       |            |                           |        |                            |                |                           |        |                             |                    |                           |        |                        |          |                                |        |      |         |                                |        |                     |      |                       |                 |                         |        |                                   |                        |                           |                  |                                   |                        |



Product Service

**Calibration Laboratory of  
Schmid & Partner  
Engineering AG**  
Zeughausstrasse 43, 8004 Zurich, Switzerland



**S** Schweizerischer Kalibrierdienst  
**C** Service suisse d'étalonnage  
**S** Servizio svizzero di taratura  
**S** Swiss Calibration Service

Accredited by the Swiss Accreditation Service (SAS)  
The Swiss Accreditation Service is one of the signatories to the EA  
Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: **SCS 0108**

**Glossary:**

TSL tissue simulating liquid  
ConvF sensitivity in TSL / NORM x,y,z  
N/A not applicable or not measured

**Calibration is Performed According to the Following Standards:**

- a) IEEE Std 1528-2013, "IEEE Recommended Practice for Determining the Peak Spatial-Averaged Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques", June 2013
- b) IEC 62209-1, "Procedure to measure the Specific Absorption Rate (SAR) for hand-held devices used in close proximity to the ear (frequency range of 300 MHz to 3 GHz)", February 2005
- c) IEC 62209-2, "Procedure to determine the Specific Absorption Rate (SAR) for wireless communication devices used in close proximity to the human body (frequency range of 30 MHz to 6 GHz)", March 2010
- d) KDB 865664, "SAR Measurement Requirements for 100 MHz to 6 GHz"

**Additional Documentation:**

- e) DASY4/5 System Handbook

**Methods Applied and Interpretation of Parameters:**

- *Measurement Conditions:* Further details are available from the Validation Report at the end of the certificate. All figures stated in the certificate are valid at the frequency indicated.
- *Antenna Parameters with TSL:* The dipole is mounted with the spacer to position its feed point exactly below the center marking of the flat phantom section, with the arms oriented parallel to the body axis.
- *Feed Point Impedance and Return Loss:* These parameters are measured with the dipole positioned under the liquid filled phantom. The impedance stated is transformed from the measurement at the SMA connector to the feed point. The Return Loss ensures low reflected power. No uncertainty required.
- *Electrical Delay:* One-way delay between the SMA connector and the antenna feed point. No uncertainty required.
- *SAR measured:* SAR measured at the stated antenna input power.
- *SAR normalized:* SAR as measured, normalized to an input power of 1 W at the antenna connector.
- *SAR for nominal TSL parameters:* The measured TSL parameters are used to calculate the nominal SAR result.

The reported uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor k=2, which for a normal distribution corresponds to a coverage probability of approximately 95%.



### Measurement Conditions

DASY system configuration, as far as not given on page 1.

|                              |                        |             |
|------------------------------|------------------------|-------------|
| DASY Version                 | DASY5                  | V52.8.8     |
| Extrapolation                | Advanced Extrapolation |             |
| Phantom                      | Modular Flat Phantom   |             |
| Distance Dipole Center - TSL | 15 mm                  | with Spacer |
| Zoom Scan Resolution         | dx, dy, dz = 5 mm      |             |
| Frequency                    | 835 MHz $\pm$ 1 MHz    |             |

### Head TSL parameters

The following parameters and calculations were applied.

|   | Temperature         | Permittivity   | Conductivity         |
|---|---------------------|----------------|----------------------|
| Nominal Head TSL parameters             | 22.0 °C             | 41.5           | 0.90 mho/m           |
| Measured Head TSL parameters            | (22.0 $\pm$ 0.2) °C | 42.6 $\pm$ 6 % | 0.92 mho/m $\pm$ 6 % |
| Head TSL temperature change during test | < 0.5 °C            | ----           | ----                 |

### SAR result with Head TSL

| SAR averaged over 1 cm <sup>3</sup> (1 g) of Head TSL | Condition          |                              |
|---|--------------------|------------------------------|
| SAR measured  | 250 mW input power | 2.34 W/kg                    |
| SAR for nominal Head TSL parameters                   | normalized to 1W   | 9.26 W/kg $\pm$ 17.0 % (k=2) |

| SAR averaged over 10 cm <sup>3</sup> (10 g) of Head TSL | condition          |                              |
|---|--------------------|------------------------------|
| SAR measured  | 250 mW input power | 1.52 W/kg                    |
| SAR for nominal Head TSL parameters                     | normalized to 1W   | 6.02 W/kg $\pm$ 16.5 % (k=2) |

### Body TSL parameters

The following parameters and calculations were applied.

|   | Temperature         | Permittivity   | Conductivity         |
|---|---------------------|----------------|----------------------|
| Nominal Body TSL parameters             | 22.0 °C             | 55.2           | 0.97 mho/m           |
| Measured Body TSL parameters            | (22.0 $\pm$ 0.2) °C | 55.6 $\pm$ 6 % | 0.99 mho/m $\pm$ 6 % |
| Body TSL temperature change during test | < 0.5 °C            | ----           | ----                 |

### SAR result with Body TSL

| SAR averaged over 1 cm <sup>3</sup> (1 g) of Body TSL | Condition          |                              |
|---|--------------------|------------------------------|
| SAR measured  | 250 mW input power | 2.40 W/kg                    |
| SAR for nominal Body TSL parameters                   | normalized to 1W   | 9.47 W/kg $\pm$ 17.0 % (k=2) |

| SAR averaged over 10 cm <sup>3</sup> (10 g) of Body TSL | condition          |                              |
|---|--------------------|------------------------------|
| SAR measured  | 250 mW input power | 1.57 W/kg                    |
| SAR for nominal Body TSL parameters                     | normalized to 1W   | 6.21 W/kg $\pm$ 16.5 % (k=2) |



### Appendix (Additional assessments outside the scope of SCS 0108)

#### Antenna Parameters with Head TSL

|                                      |                               |
|--------------------------------------|-------------------------------|
| Impedance, transformed to feed point | 49.9 $\Omega$ - 7.0 $j\Omega$ |
| Return Loss                          | - 23.1 dB                     |

#### Antenna Parameters with Body TSL

|                                      |                               |
|--------------------------------------|-------------------------------|
| Impedance, transformed to feed point | 46.0 $\Omega$ - 8.7 $j\Omega$ |
| Return Loss                          | - 20.0 dB                     |

#### General Antenna Parameters and Design

|                                  |          |
|----------------------------------|----------|
| Electrical Delay (one direction) | 1.386 ns |
|----------------------------------|----------|

After long term use with 100W radiated power, only a slight warming of the dipole near the feedpoint can be measured.

The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals. On some of the dipoles, small end caps are added to the dipole arms in order to improve matching when loaded according to the position as explained in the "Measurement Conditions" paragraph. The SAR data are not affected by this change. The overall dipole length is still according to the Standard.

No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feedpoint may be damaged.

#### Additional EUT Data

|                 |                  |
|-----------------|------------------|
| Manufactured by | SPEAG            |
| Manufactured on | October 24, 2001 |



## DASY5 Validation Report for Head TSL

Date: 12.11.2015

Test Laboratory: SPEAG, Zurich, Switzerland

**DUT: Dipole 835 MHz; Type: D835V2; Serial: D835V2 - SN: 447**

Communication System: UID 0 - CW; Frequency: 835 MHz

Medium parameters used:  $f = 835 \text{ MHz}$ ;  $\sigma = 0.92 \text{ S/m}$ ;  $\epsilon_r = 42.6$ ;  $\rho = 1000 \text{ kg/m}^3$

Phantom section: Flat Section

Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2011)

DASY52 Configuration:

- Probe: EX3DV4 - SN7349; ConvF(9.77, 9.77, 9.77); Calibrated: 30.12.2014;
- Sensor-Surface: 1.4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn601; Calibrated: 17.08.2015
- Phantom: Flat Phantom 4.9L; Type: QD000P49AA; Serial: 1001
- DASY52 52.8.8(1222); SEMCAD X 14.6.10(7331)

### Dipole Calibration for Head Tissue/Pin=250 mW, d=15mm/Zoom Scan (7x7x7)/Cube 0:


Measurement grid: dx=5mm, dy=5mm, dz=5mm

Reference Value = 61.13 V/m; Power Drift = 0.03 dB

Peak SAR (extrapolated) = 3.47 W/kg


**SAR(1 g) = 2.34 W/kg; SAR(10 g) = 1.52 W/kg**

Maximum value of SAR (measured) = 3.10 W/kg

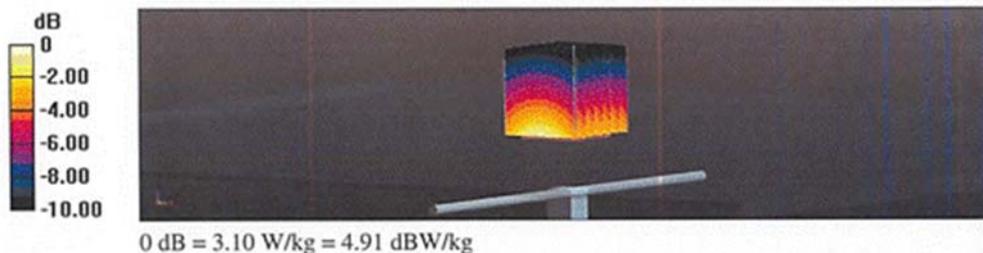



### Impedance Measurement Plot for Head TSL

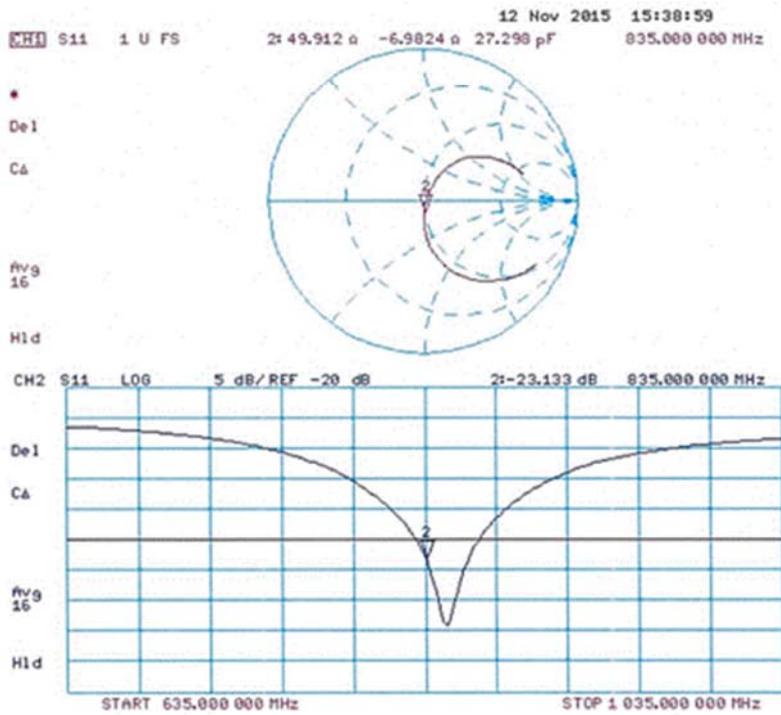



## DASY5 Validation Report for Body TSL

Date: 12.11.2015

Test Laboratory: SPEAG, Zurich, Switzerland

DUT: Dipole 835 MHz; Type: D835V2; Serial: D835V2 - SN: 447

Communication System: UID 0 - CW; Frequency: 835 MHz

Medium parameters used:  $f = 835$  MHz;  $\sigma = 0.99$  S/m;  $\epsilon_r = 55.6$ ;  $\rho = 1000$  kg/m<sup>3</sup>

Phantom section: Flat Section

Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2011)

DASY52 Configuration:

- Probe: EX3DV4 - SN7349; ConvF(9.72, 9.72, 9.72); Calibrated: 30.12.2014;
- Sensor-Surface: 1.4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn601; Calibrated: 17.08.2015
- Phantom: Flat Phantom 4.9L; Type: QD000P49AA; Serial: 1001
- DASY52 52.8.8(1222); SEMCAD X 14.6.10(7331)

### Dipole Calibration for Body Tissue/Pin=250 mW, d=15mm/Zoom Scan (7x7x7)/Cube 0:


Measurement grid: dx=5mm, dy=5mm, dz=5mm

Reference Value = 59.65 V/m; Power Drift = 0.02 dB

Peak SAR (extrapolated) = 3.57 W/kg


SAR(1 g) = 2.4 W/kg; SAR(10 g) = 1.57 W/kg

Maximum value of SAR (measured) = 3.17 W/kg

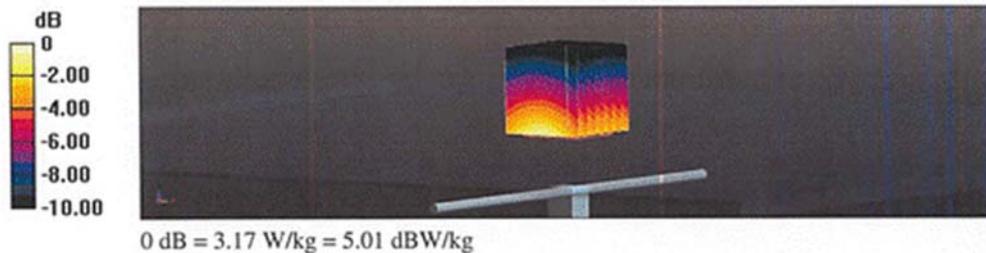



### Impedance Measurement Plot for Body TSL

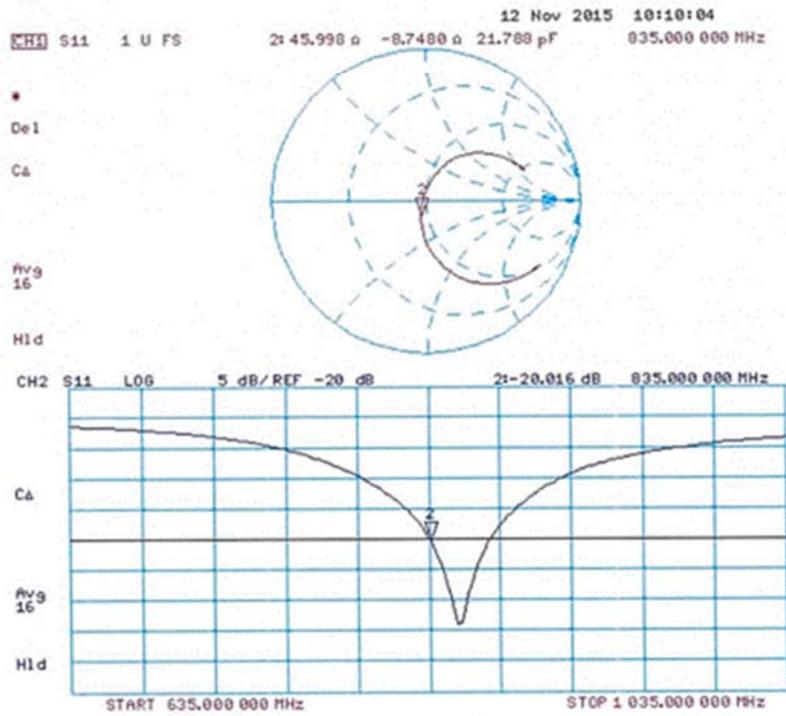



Product Service

**Calibration Laboratory of  
Schmid & Partner  
Engineering AG**  
Zeughausstrasse 43, 8004 Zurich, Switzerland



**S** Schweizerischer Kalibrierdienst  
**C** Service suisse d'étalonnage  
**S** Servizio svizzero di taratura  
**S** Swiss Calibration Service

Accredited by the Swiss Accreditation Service (SAS)  
The Swiss Accreditation Service is one of the signatories to the EA  
Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: **SCS 0108**

Client **TÜV SÜD UK**

Certificate No: **D1900V2-546\_Nov15**

**CALIBRATION CERTIFICATE**

| Object   | D1900V2 - SN: 546  |                                   |                        |                   |      |                            |                       |                      |            |                           |        |                       |            |                           |        |                       |            |                           |        |                            |                |                           |        |                             |                    |                           |        |                        |          |                                |        |      |         |                                |        |                     |      |                       |                 |                         |        |                                   |                        |                           |                  |                                   |                        |
|--|--|-----------------------------------|------------------------|-------------------|------|----------------------------|-----------------------|----------------------|------------|---------------------------|--------|-----------------------|------------|---------------------------|--------|-----------------------|------------|---------------------------|--------|----------------------------|----------------|---------------------------|--------|-----------------------------|--------------------|---------------------------|--------|------------------------|----------|--------------------------------|--------|------|---------|--------------------------------|--------|---------------------|------|-----------------------|-----------------|-------------------------|--------|-----------------------------------|------------------------|---------------------------|------------------|-----------------------------------|------------------------|
| Calibration procedure(s)   | QA CAL-05.v9<br>Calibration procedure for dipole validation kits above 700 MHz |                                   |                        |                   |      |                            |                       |                      |            |                           |        |                       |            |                           |        |                       |            |                           |        |                            |                |                           |        |                             |                    |                           |        |                        |          |                                |        |      |         |                                |        |                     |      |                       |                 |                         |        |                                   |                        |                           |                  |                                   |                        |
| Calibration date:  | November 17, 2015  |                                   |                        |                   |      |                            |                       |                      |            |                           |        |                       |            |                           |        |                       |            |                           |        |                            |                |                           |        |                             |                    |                           |        |                        |          |                                |        |      |         |                                |        |                     |      |                       |                 |                         |        |                                   |                        |                           |                  |                                   |                        |
| <p>This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI).<br/>The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.</p> <p>All calibrations have been conducted in the closed laboratory facility: environment temperature (22 ± 3)°C and humidity &lt; 70%.</p> <p>Calibration Equipment used (M&amp;TE critical for calibration)</p> <table border="1"> <thead> <tr> <th>Primary Standards</th> <th>ID #</th> <th>Cal Date (Certificate No.)</th> <th>Scheduled Calibration</th> </tr> </thead> <tbody> <tr> <td>Power meter EPM-442A</td> <td>GB37480704</td> <td>07-Oct-15 (No. 217-02222)</td> <td>Oct-16</td> </tr> <tr> <td>Power sensor HP 8481A</td> <td>US37292783</td> <td>07-Oct-15 (No. 217-02222)</td> <td>Oct-16</td> </tr> <tr> <td>Power sensor HP 8481A</td> <td>MY41092317</td> <td>07-Oct-15 (No. 217-02223)</td> <td>Oct-16</td> </tr> <tr> <td>Reference 20 dB Attenuator</td> <td>SN: 5058 (20k)</td> <td>01-Apr-15 (No. 217-02131)</td> <td>Mar-16</td> </tr> <tr> <td>Type-N mismatch combination</td> <td>SN: 5047.2 / 06327</td> <td>01-Apr-15 (No. 217-02134)</td> <td>Mar-16</td> </tr> <tr> <td>Reference Probe EX3DV4</td> <td>SN: 7349</td> <td>30-Dec-14 (No. EX3-7349_Dec14)</td> <td>Dec-15</td> </tr> <tr> <td>DAE4</td> <td>SN: 601</td> <td>17-Aug-15 (No. DAE4-601_Aug15)</td> <td>Aug-16</td> </tr> </tbody> </table><br><table border="1"> <thead> <tr> <th>Secondary Standards</th> <th>ID #</th> <th>Check Date (in house)</th> <th>Scheduled Check</th> </tr> </thead> <tbody> <tr> <td>RF generator R&amp;S SMT-06</td> <td>100972</td> <td>15-Jun-15 (in house check Jun-15)</td> <td>In house check: Jun-18</td> </tr> <tr> <td>Network Analyzer HP 8753E</td> <td>US37390585 S4206</td> <td>18-Oct-01 (in house check Oct-15)</td> <td>In house check: Oct-16</td> </tr> </tbody> </table> |  |                                   |                        | Primary Standards | ID # | Cal Date (Certificate No.) | Scheduled Calibration | Power meter EPM-442A | GB37480704 | 07-Oct-15 (No. 217-02222) | Oct-16 | Power sensor HP 8481A | US37292783 | 07-Oct-15 (No. 217-02222) | Oct-16 | Power sensor HP 8481A | MY41092317 | 07-Oct-15 (No. 217-02223) | Oct-16 | Reference 20 dB Attenuator | SN: 5058 (20k) | 01-Apr-15 (No. 217-02131) | Mar-16 | Type-N mismatch combination | SN: 5047.2 / 06327 | 01-Apr-15 (No. 217-02134) | Mar-16 | Reference Probe EX3DV4 | SN: 7349 | 30-Dec-14 (No. EX3-7349_Dec14) | Dec-15 | DAE4 | SN: 601 | 17-Aug-15 (No. DAE4-601_Aug15) | Aug-16 | Secondary Standards | ID # | Check Date (in house) | Scheduled Check | RF generator R&S SMT-06 | 100972 | 15-Jun-15 (in house check Jun-15) | In house check: Jun-18 | Network Analyzer HP 8753E | US37390585 S4206 | 18-Oct-01 (in house check Oct-15) | In house check: Oct-16 |
| Primary Standards  | ID #   | Cal Date (Certificate No.)        | Scheduled Calibration  |                   |      |                            |                       |                      |            |                           |        |                       |            |                           |        |                       |            |                           |        |                            |                |                           |        |                             |                    |                           |        |                        |          |                                |        |      |         |                                |        |                     |      |                       |                 |                         |        |                                   |                        |                           |                  |                                   |                        |
| Power meter EPM-442A   | GB37480704   | 07-Oct-15 (No. 217-02222)         | Oct-16                 |                   |      |                            |                       |                      |            |                           |        |                       |            |                           |        |                       |            |                           |        |                            |                |                           |        |                             |                    |                           |        |                        |          |                                |        |      |         |                                |        |                     |      |                       |                 |                         |        |                                   |                        |                           |                  |                                   |                        |
| Power sensor HP 8481A  | US37292783   | 07-Oct-15 (No. 217-02222)         | Oct-16                 |                   |      |                            |                       |                      |            |                           |        |                       |            |                           |        |                       |            |                           |        |                            |                |                           |        |                             |                    |                           |        |                        |          |                                |        |      |         |                                |        |                     |      |                       |                 |                         |        |                                   |                        |                           |                  |                                   |                        |
| Power sensor HP 8481A  | MY41092317   | 07-Oct-15 (No. 217-02223)         | Oct-16                 |                   |      |                            |                       |                      |            |                           |        |                       |            |                           |        |                       |            |                           |        |                            |                |                           |        |                             |                    |                           |        |                        |          |                                |        |      |         |                                |        |                     |      |                       |                 |                         |        |                                   |                        |                           |                  |                                   |                        |
| Reference 20 dB Attenuator   | SN: 5058 (20k)   | 01-Apr-15 (No. 217-02131)         | Mar-16                 |                   |      |                            |                       |                      |            |                           |        |                       |            |                           |        |                       |            |                           |        |                            |                |                           |        |                             |                    |                           |        |                        |          |                                |        |      |         |                                |        |                     |      |                       |                 |                         |        |                                   |                        |                           |                  |                                   |                        |
| Type-N mismatch combination  | SN: 5047.2 / 06327   | 01-Apr-15 (No. 217-02134)         | Mar-16                 |                   |      |                            |                       |                      |            |                           |        |                       |            |                           |        |                       |            |                           |        |                            |                |                           |        |                             |                    |                           |        |                        |          |                                |        |      |         |                                |        |                     |      |                       |                 |                         |        |                                   |                        |                           |                  |                                   |                        |
| Reference Probe EX3DV4   | SN: 7349   | 30-Dec-14 (No. EX3-7349_Dec14)    | Dec-15                 |                   |      |                            |                       |                      |            |                           |        |                       |            |                           |        |                       |            |                           |        |                            |                |                           |        |                             |                    |                           |        |                        |          |                                |        |      |         |                                |        |                     |      |                       |                 |                         |        |                                   |                        |                           |                  |                                   |                        |
| DAE4   | SN: 601  | 17-Aug-15 (No. DAE4-601_Aug15)    | Aug-16                 |                   |      |                            |                       |                      |            |                           |        |                       |            |                           |        |                       |            |                           |        |                            |                |                           |        |                             |                    |                           |        |                        |          |                                |        |      |         |                                |        |                     |      |                       |                 |                         |        |                                   |                        |                           |                  |                                   |                        |
| Secondary Standards  | ID #   | Check Date (in house)             | Scheduled Check        |                   |      |                            |                       |                      |            |                           |        |                       |            |                           |        |                       |            |                           |        |                            |                |                           |        |                             |                    |                           |        |                        |          |                                |        |      |         |                                |        |                     |      |                       |                 |                         |        |                                   |                        |                           |                  |                                   |                        |
| RF generator R&S SMT-06  | 100972   | 15-Jun-15 (in house check Jun-15) | In house check: Jun-18 |                   |      |                            |                       |                      |            |                           |        |                       |            |                           |        |                       |            |                           |        |                            |                |                           |        |                             |                    |                           |        |                        |          |                                |        |      |         |                                |        |                     |      |                       |                 |                         |        |                                   |                        |                           |                  |                                   |                        |
| Network Analyzer HP 8753E  | US37390585 S4206   | 18-Oct-01 (in house check Oct-15) | In house check: Oct-16 |                   |      |                            |                       |                      |            |                           |        |                       |            |                           |        |                       |            |                           |        |                            |                |                           |        |                             |                    |                           |        |                        |          |                                |        |      |         |                                |        |                     |      |                       |                 |                         |        |                                   |                        |                           |                  |                                   |                        |
| Calibrated by:   | Name<br>Jeton Kastrati   | Function<br>Laboratory Technician | Signature<br>          |                   |      |                            |                       |                      |            |                           |        |                       |            |                           |        |                       |            |                           |        |                            |                |                           |        |                             |                    |                           |        |                        |          |                                |        |      |         |                                |        |                     |      |                       |                 |                         |        |                                   |                        |                           |                  |                                   |                        |
| Approved by:   | Name<br>Katja Pokovic  | Function<br>Technical Manager     | Signature<br>          |                   |      |                            |                       |                      |            |                           |        |                       |            |                           |        |                       |            |                           |        |                            |                |                           |        |                             |                    |                           |        |                        |          |                                |        |      |         |                                |        |                     |      |                       |                 |                         |        |                                   |                        |                           |                  |                                   |                        |
| Issued: November 17, 2015  |  |                                   |                        |                   |      |                            |                       |                      |            |                           |        |                       |            |                           |        |                       |            |                           |        |                            |                |                           |        |                             |                    |                           |        |                        |          |                                |        |      |         |                                |        |                     |      |                       |                 |                         |        |                                   |                        |                           |                  |                                   |                        |
| This calibration certificate shall not be reproduced except in full without written approval of the laboratory.  |  |                                   |                        |                   |      |                            |                       |                      |            |                           |        |                       |            |                           |        |                       |            |                           |        |                            |                |                           |        |                             |                    |                           |        |                        |          |                                |        |      |         |                                |        |                     |      |                       |                 |                         |        |                                   |                        |                           |                  |                                   |                        |



Product Service

**Calibration Laboratory of  
Schmid & Partner  
Engineering AG**  
Zeughausstrasse 43, 8004 Zurich, Switzerland



**S** Schweizerischer Kalibrierdienst  
**C** Service suisse d'étalonnage  
**S** Servizio svizzero di taratura  
**S** Swiss Calibration Service

Accredited by the Swiss Accreditation Service (SAS)  
The Swiss Accreditation Service is one of the signatories to the EA  
Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: SCS 0108

**Glossary:**

|       |                                 |
|-------|---------------------------------|
| TSL   | tissue simulating liquid        |
| ConvF | sensitivity in TSL / NORM x,y,z |
| N/A   | not applicable or not measured  |

**Calibration is Performed According to the Following Standards:**

- IEEE Std 1528-2013, "IEEE Recommended Practice for Determining the Peak Spatial-Averaged Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques", June 2013
- IEC 62209-1, "Procedure to measure the Specific Absorption Rate (SAR) for hand-held devices used in close proximity to the ear (frequency range of 300 MHz to 3 GHz)", February 2005
- IEC 62209-2, "Procedure to determine the Specific Absorption Rate (SAR) for wireless communication devices used in close proximity to the human body (frequency range of 30 MHz to 6 GHz)", March 2010
- KDB 865664, "SAR Measurement Requirements for 100 MHz to 6 GHz"

**Additional Documentation:**

- DASY4/5 System Handbook

**Methods Applied and Interpretation of Parameters:**

- Measurement Conditions:** Further details are available from the Validation Report at the end of the certificate. All figures stated in the certificate are valid at the frequency indicated.
- Antenna Parameters with TSL:** The dipole is mounted with the spacer to position its feed point exactly below the center marking of the flat phantom section, with the arms oriented parallel to the body axis.
- Feed Point Impedance and Return Loss:** These parameters are measured with the dipole positioned under the liquid filled phantom. The impedance stated is transformed from the measurement at the SMA connector to the feed point. The Return Loss ensures low reflected power. No uncertainty required.
- Electrical Delay:** One-way delay between the SMA connector and the antenna feed point. No uncertainty required.
- SAR measured:** SAR measured at the stated antenna input power.
- SAR normalized:** SAR as measured, normalized to an input power of 1 W at the antenna connector.
- SAR for nominal TSL parameters:** The measured TSL parameters are used to calculate the nominal SAR result.

The reported uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor  $k=2$ , which for a normal distribution corresponds to a coverage probability of approximately 95%.



**Measurement Conditions**

DASY system configuration, as far as not given on page 1.

|                              |                        |             |
|------------------------------|------------------------|-------------|
| DASY Version                 | DASY5                  | V52.8.8     |
| Extrapolation                | Advanced Extrapolation |             |
| Phantom                      | Modular Flat Phantom   |             |
| Distance Dipole Center - TSL | 10 mm                  | with Spacer |
| Zoom Scan Resolution         | dx, dy, dz = 5 mm      |             |
| Frequency                    | 1900 MHz ± 1 MHz       |             |

**Head TSL parameters**

The following parameters and calculations were applied.

|   | Temperature     | Permittivity | Conductivity     |
|---|-----------------|--------------|------------------|
| Nominal Head TSL parameters             | 22.0 °C         | 40.0         | 1.40 mho/m       |
| Measured Head TSL parameters            | (22.0 ± 0.2) °C | 39.4 ± 6 %   | 1.39 mho/m ± 6 % |
| Head TSL temperature change during test | < 0.5 °C        | ----         | ----             |

**SAR result with Head TSL**

| SAR averaged over 1 cm <sup>3</sup> (1 g) of Head TSL | Condition          |                          |
|---|--------------------|--------------------------|
| SAR measured  | 250 mW input power | 9.93 W/kg                |
| SAR for nominal Head TSL parameters                   | normalized to 1W   | 39.8 W/kg ± 17.0 % (k=2) |

| SAR averaged over 10 cm <sup>3</sup> (10 g) of Head TSL | condition          |                          |
|---|--------------------|--------------------------|
| SAR measured  | 250 mW input power | 5.19 W/kg                |
| SAR for nominal Head TSL parameters                     | normalized to 1W   | 20.8 W/kg ± 16.5 % (k=2) |

**Body TSL parameters**

The following parameters and calculations were applied.

|   | Temperature     | Permittivity | Conductivity     |
|---|-----------------|--------------|------------------|
| Nominal Body TSL parameters             | 22.0 °C         | 53.3         | 1.52 mho/m       |
| Measured Body TSL parameters            | (22.0 ± 0.2) °C | 52.2 ± 6 %   | 1.52 mho/m ± 6 % |
| Body TSL temperature change during test | < 0.5 °C        | ----         | ----             |

**SAR result with Body TSL**

| SAR averaged over 1 cm <sup>3</sup> (1 g) of Body TSL | Condition          |                          |
|---|--------------------|--------------------------|
| SAR measured  | 250 mW input power | 10.1 W/kg                |
| SAR for nominal Body TSL parameters                   | normalized to 1W   | 40.2 W/kg ± 17.0 % (k=2) |

| SAR averaged over 10 cm <sup>3</sup> (10 g) of Body TSL | condition          |                          |
|---|--------------------|--------------------------|
| SAR measured  | 250 mW input power | 5.31 W/kg                |
| SAR for nominal Body TSL parameters                     | normalized to 1W   | 21.2 W/kg ± 16.5 % (k=2) |



### Appendix (Additional assessments outside the scope of SCS 0108)

#### Antenna Parameters with Head TSL

|                                      |                                |
|--------------------------------------|--------------------------------|
| Impedance, transformed to feed point | 50.7 $\Omega$ + 3.2 j $\Omega$ |
| Return Loss                          | - 29.9 dB                      |

#### Antenna Parameters with Body TSL

|                                      |                                |
|--------------------------------------|--------------------------------|
| Impedance, transformed to feed point | 46.4 $\Omega$ + 4.4 j $\Omega$ |
| Return Loss                          | - 24.6 dB                      |

#### General Antenna Parameters and Design

|                                  |          |
|----------------------------------|----------|
| Electrical Delay (one direction) | 1.204 ns |
|----------------------------------|----------|

After long term use with 100W radiated power, only a slight warming of the dipole near the feedpoint can be measured.

The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals. On some of the dipoles, small end caps are added to the dipole arms in order to improve matching when loaded according to the position as explained in the "Measurement Conditions" paragraph. The SAR data are not affected by this change. The overall dipole length is still according to the Standard.

No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feedpoint may be damaged.

#### Additional EUT Data

|                 |                   |
|-----------------|-------------------|
| Manufactured by | SPEAG             |
| Manufactured on | November 15, 2001 |



## DASY5 Validation Report for Head TSL

Date: 10.11.2015

Test Laboratory: SPEAG, Zurich, Switzerland

**DUT: Dipole 1900 MHz; Type: D1900V2; Serial: D1900V2 - SN: 546**

Communication System: UID 0 - CW; Frequency: 1900 MHz

Medium parameters used:  $f = 1900$  MHz;  $\sigma = 1.39$  S/m;  $\epsilon_r = 39.4$ ;  $\rho = 1000$  kg/m<sup>3</sup>

Phantom section: Flat Section

Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2011)

DASY52 Configuration:

- Probe: EX3DV4 - SN7349; ConvF(8.14, 8.14, 8.14); Calibrated: 30.12.2014;
- Sensor-Surface: 1.4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn601; Calibrated: 17.08.2015
- Phantom: Flat Phantom 5.0 (front); Type: QD000P50AA; Serial: 1001
- DASY52 52.8.8(1222); SEMCAD X 14.6.10(7331)

### Dipole Calibration for Head Tissue/Pin=250 mW, d=10mm/Zoom Scan (7x7x7)/Cube 0:


Measurement grid: dx=5mm, dy=5mm, dz=5mm

Reference Value = 108.9 V/m; Power Drift = 0.01 dB

Peak SAR (extrapolated) = 18.7 W/kg


SAR(1 g) = 9.93 W/kg; SAR(10 g) = 5.19 W/kg

Maximum value of SAR (measured) = 15.6 W/kg

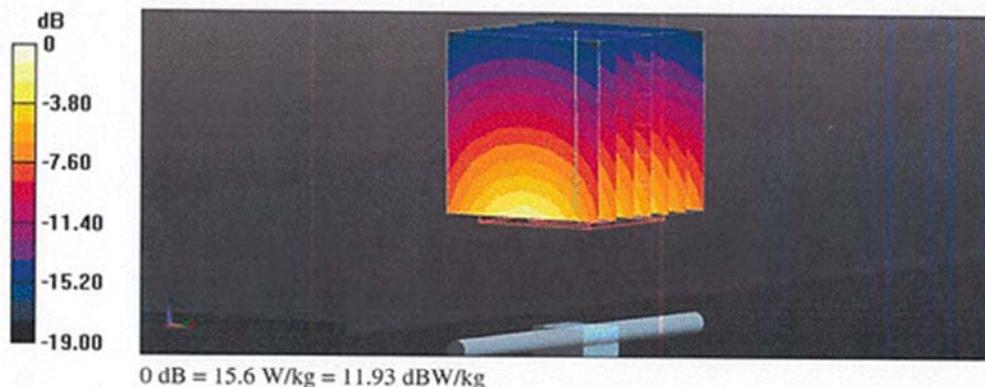



### Impedance Measurement Plot for Head TSL

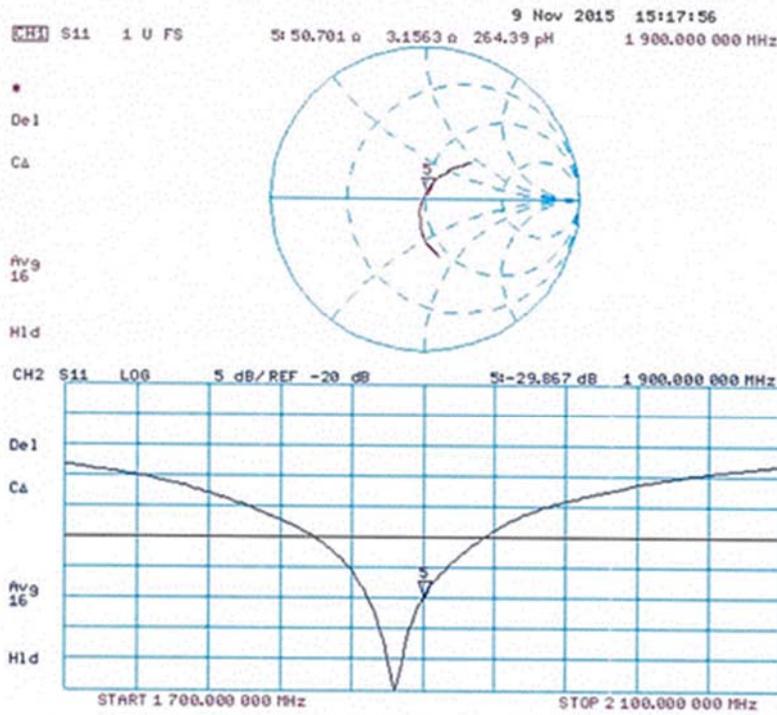



**DASY5 Validation Report for Body TSL**

Date: 17.11.2015

Test Laboratory: SPEAG, Zurich, Switzerland

**DUT: Dipole 1900 MHz; Type: D1900V2; Serial: D1900V2 - SN: 546**


Communication System: UID 0 - CW; Frequency: 1900 MHz  
 Medium parameters used:  $f = 1900 \text{ MHz}$ ;  $\sigma = 1.52 \text{ S/m}$ ;  $\epsilon_r = 52.2$ ;  $\rho = 1000 \text{ kg/m}^3$   
 Phantom section: Flat Section  
 Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2011)

**DASY52 Configuration:**

- Probe: EX3DV4 - SN7349; ConvF(7.9, 7.9, 7.9); Calibrated: 30.12.2014;
- Sensor-Surface: 1.4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn601; Calibrated: 17.08.2015
- Phantom: Flat Phantom 5.0 (back); Type: QD000P50AA; Serial: 1002
- DASY52 52.8.8(1222); SEMCAD X 14.6.10(7331)

**Dipole Calibration for Body Tissue/Pin=250 mW, d=10mm/Zoom Scan (7x7x7)/Cube 0:**


Measurement grid:  $dx=5\text{mm}$ ,  $dy=5\text{mm}$ ,  $dz=5\text{mm}$   
 Reference Value = 104.5 V/m; Power Drift = 0.00 dB  
 Peak SAR (extrapolated) = 18.1 W/kg  
**SAR(1 g) = 10.1 W/kg; SAR(10 g) = 5.31 W/kg**  
 Maximum value of SAR (measured) = 15.4 W/kg

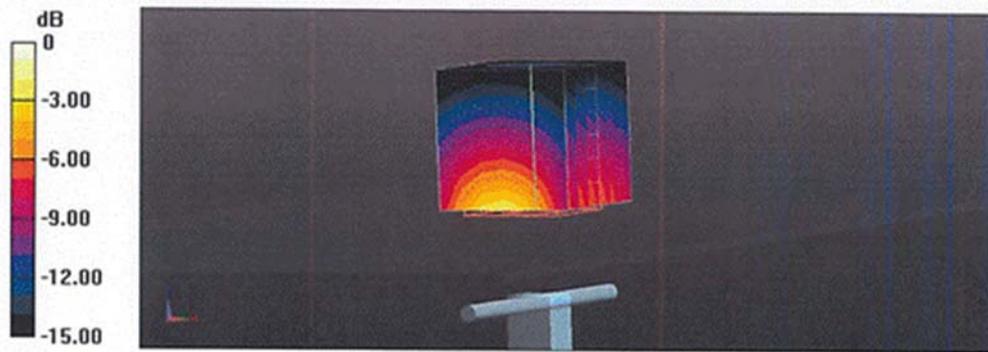

0 dB = 15.4 W/kg = 11.88 dBW/kg



### Impedance Measurement Plot for Body TSL

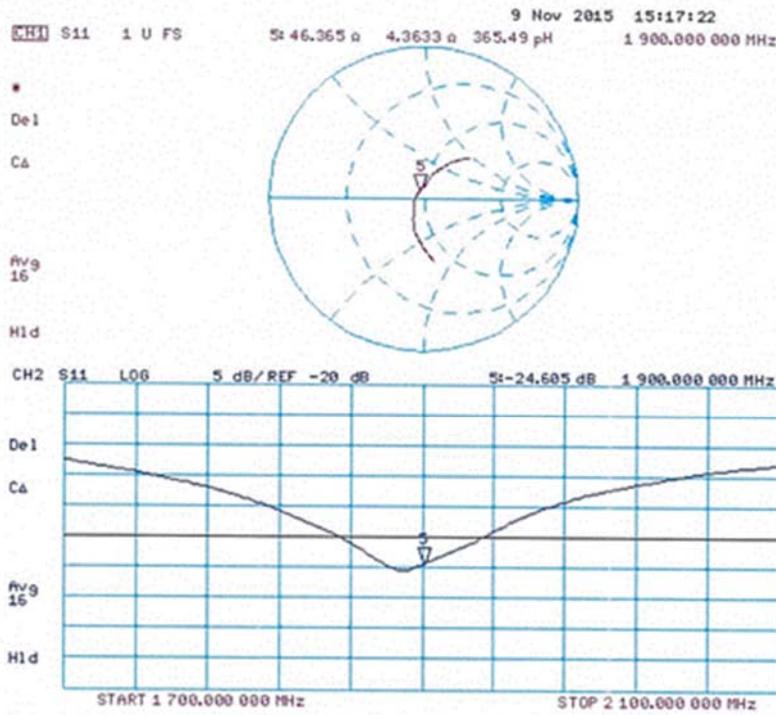



Product Service

**Calibration Laboratory of  
Schmid & Partner  
Engineering AG**  
Zeughausstrasse 43, 8004 Zurich, Switzerland



**S** Schweizerischer Kalibrierdienst  
**C** Service suisse d'étalonnage  
**S** Servizio svizzero di taratura  
**S** Swiss Calibration Service

Accredited by the Swiss Accreditation Service (SAS)  
The Swiss Accreditation Service is one of the signatories to the EA  
Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: **SCS 0108**

Client **TÜV SÜD UK**

Certificate No: **D2450V2-715\_Nov15**

**CALIBRATION CERTIFICATE**

|  |  |                                   |                                |
|--|--|-----------------------------------|--------------------------------|
| Object   | D2450V2 - SN: 715  |                                   |                                |
| Calibration procedure(s)   | QA CAL-05.v9<br>Calibration procedure for dipole validation kits above 700 MHz |                                   |                                |
| Calibration date:  | November 10, 2015  |                                   |                                |
| <p>This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI).<br/>The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.</p> <p>All calibrations have been conducted in the closed laboratory facility: environment temperature (22 ± 3)°C and humidity &lt; 70%.</p> <p>Calibration Equipment used (M&amp;TE critical for calibration)</p> |  |                                   |                                |
| <b>Primary Standards</b>   | <b>ID #</b>  | <b>Cal Date (Certificate No.)</b> | <b>Scheduled Calibration</b>   |
| Power meter EPM-442A   | GB37480704   | 07-Oct-15 (No. 217-02222)         | Oct-16                         |
| Power sensor HP 8481A  | US37292783   | 07-Oct-15 (No. 217-02222)         | Oct-16                         |
| Power sensor HP 8481A  | MY41092317   | 07-Oct-15 (No. 217-02223)         | Oct-16                         |
| Reference 20 dB Attenuator   | SN: 5058 (20k)   | 01-Apr-15 (No. 217-02131)         | Mar-16                         |
| Type-N mismatch combination  | SN: 5047.2 / 06327   | 01-Apr-15 (No. 217-02134)         | Mar-16                         |
| Reference Probe EX3DV4   | SN: 7349   | 30-Dec-14 (No. EX3-7349_Dec14)    | Dec-15                         |
| DAE4   | SN: 601  | 17-Aug-15 (No. DAE4-601_Aug15)    | Aug-16                         |
| <b>Secondary Standards</b>   | <b>ID #</b>  | <b>Check Date (in house)</b>      | <b>Scheduled Check</b>         |
| RF generator R&S SMT-06  | 100972   | 15-Jun-15 (in house check Jun-15) | In house check: Jun-18         |
| Network Analyzer HP 8753E  | US37390585 S4206   | 18-Oct-01 (in house check Oct-15) | In house check: Oct-16         |
| Calibrated by:   | Name<br>Michael Weber  | Function<br>Laboratory Technician | Signature<br><i>M. Weber</i>   |
| Approved by:   | Name<br>Katja Pokovic  | Function<br>Technical Manager     | Signature<br><i>K. Pokovic</i> |
|  |  |                                   | Issued: November 11, 2015      |
| This calibration certificate shall not be reproduced except in full without written approval of the laboratory.  |  |                                   |                                |

Certificate No: D2450V2-715\_Nov15

Page 1 of 8



Product Service

**Calibration Laboratory of  
Schmid & Partner  
Engineering AG**  
Zeughausstrasse 43, 8004 Zurich, Switzerland



**S** Schweizerischer Kalibrierdienst  
**C** Service suisse d'étalonnage  
**S** Servizio svizzero di taratura  
**S** Swiss Calibration Service

Accredited by the Swiss Accreditation Service (SAS)  
The Swiss Accreditation Service is one of the signatories to the EA  
Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: SCS 0108

**Glossary:**

TSL tissue simulating liquid  
ConvF sensitivity in TSL / NORM x,y,z  
N/A not applicable or not measured

**Calibration is Performed According to the Following Standards:**

- a) IEEE Std 1528-2013, "IEEE Recommended Practice for Determining the Peak Spatial-Averaged Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques", June 2013
- b) IEC 62209-1, "Procedure to measure the Specific Absorption Rate (SAR) for hand-held devices used in close proximity to the ear (frequency range of 300 MHz to 3 GHz)", February 2005
- c) IEC 62209-2, "Procedure to determine the Specific Absorption Rate (SAR) for wireless communication devices used in close proximity to the human body (frequency range of 30 MHz to 6 GHz)", March 2010
- d) KDB 865664, "SAR Measurement Requirements for 100 MHz to 6 GHz"

**Additional Documentation:**

- e) DASY4/5 System Handbook

**Methods Applied and Interpretation of Parameters:**

- *Measurement Conditions:* Further details are available from the Validation Report at the end of the certificate. All figures stated in the certificate are valid at the frequency indicated.
- *Antenna Parameters with TSL:* The dipole is mounted with the spacer to position its feed point exactly below the center marking of the flat phantom section, with the arms oriented parallel to the body axis.
- *Feed Point Impedance and Return Loss:* These parameters are measured with the dipole positioned under the liquid filled phantom. The impedance stated is transformed from the measurement at the SMA connector to the feed point. The Return Loss ensures low reflected power. No uncertainty required.
- *Electrical Delay:* One-way delay between the SMA connector and the antenna feed point. No uncertainty required.
- *SAR measured:* SAR measured at the stated antenna input power.
- *SAR normalized:* SAR as measured, normalized to an input power of 1 W at the antenna connector.
- *SAR for nominal TSL parameters:* The measured TSL parameters are used to calculate the nominal SAR result.

The reported uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor  $k=2$ , which for a normal distribution corresponds to a coverage probability of approximately 95%.



**Measurement Conditions**

DASY system configuration, as far as not given on page 1.

|                              |                        |             |
|------------------------------|------------------------|-------------|
| DASY Version                 | DASY5                  | V52.8.8     |
| Extrapolation                | Advanced Extrapolation |             |
| Phantom                      | Modular Flat Phantom   |             |
| Distance Dipole Center - TSL | 10 mm                  | with Spacer |
| Zoom Scan Resolution         | dx, dy, dz = 5 mm      |             |
| Frequency                    | 2450 MHz ± 1 MHz       |             |

**Head TSL parameters**

The following parameters and calculations were applied.

|   | Temperature     | Permittivity | Conductivity     |
|---|-----------------|--------------|------------------|
| Nominal Head TSL parameters             | 22.0 °C         | 39.2         | 1.80 mho/m       |
| Measured Head TSL parameters            | (22.0 ± 0.2) °C | 38.2 ± 6 %   | 1.87 mho/m ± 6 % |
| Head TSL temperature change during test | < 0.5 °C        | ----         | ----             |

**SAR result with Head TSL**

| SAR averaged over 1 cm <sup>3</sup> (1 g) of Head TSL | Condition          |                          |
|---|--------------------|--------------------------|
| SAR measured  | 250 mW input power | 13.7 W/kg                |
| SAR for nominal Head TSL parameters                   | normalized to 1W   | 53.5 W/kg ± 17.0 % (k=2) |

| SAR averaged over 10 cm <sup>3</sup> (10 g) of Head TSL | condition          |                          |
|---|--------------------|--------------------------|
| SAR measured  | 250 mW input power | 6.34 W/kg                |
| SAR for nominal Head TSL parameters                     | normalized to 1W   | 25.0 W/kg ± 16.5 % (k=2) |

**Body TSL parameters**

The following parameters and calculations were applied.

|   | Temperature     | Permittivity | Conductivity     |
|---|-----------------|--------------|------------------|
| Nominal Body TSL parameters             | 22.0 °C         | 52.7         | 1.95 mho/m       |
| Measured Body TSL parameters            | (22.0 ± 0.2) °C | 52.7 ± 6 %   | 2.02 mho/m ± 6 % |
| Body TSL temperature change during test | < 0.5 °C        | ----         | ----             |

**SAR result with Body TSL**

| SAR averaged over 1 cm <sup>3</sup> (1 g) of Body TSL | Condition          |                          |
|---|--------------------|--------------------------|
| SAR measured  | 250 mW input power | 13.6 W/kg                |
| SAR for nominal Body TSL parameters                   | normalized to 1W   | 53.5 W/kg ± 17.0 % (k=2) |

| SAR averaged over 10 cm <sup>3</sup> (10 g) of Body TSL | condition          |                          |
|---|--------------------|--------------------------|
| SAR measured  | 250 mW input power | 6.38 W/kg                |
| SAR for nominal Body TSL parameters                     | normalized to 1W   | 25.3 W/kg ± 16.5 % (k=2) |



**Appendix (Additional assessments outside the scope of SCS 0108)**

**Antenna Parameters with Head TSL**

|                                      |                                |
|--------------------------------------|--------------------------------|
| Impedance, transformed to feed point | 53.7 $\Omega$ + 2.7 j $\Omega$ |
| Return Loss                          | - 27.1 dB                      |

**Antenna Parameters with Body TSL**

|                                      |                                |
|--------------------------------------|--------------------------------|
| Impedance, transformed to feed point | 50.1 $\Omega$ + 5.5 j $\Omega$ |
| Return Loss                          | - 25.2 dB                      |

**General Antenna Parameters and Design**

|                                  |          |
|----------------------------------|----------|
| Electrical Delay (one direction) | 1.156 ns |
|----------------------------------|----------|

After long term use with 100W radiated power, only a slight warming of the dipole near the feedpoint can be measured.

The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals. On some of the dipoles, small end caps are added to the dipole arms in order to improve matching when loaded according to the position as explained in the "Measurement Conditions" paragraph. The SAR data are not affected by this change. The overall dipole length is still according to the Standard.

No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feedpoint may be damaged.

**Additional EUT Data**

|                 |               |
|-----------------|---------------|
| Manufactured by | SPEAG         |
| Manufactured on | July 05, 2002 |



**DASY5 Validation Report for Head TSL**

Date: 10.11.2015

Test Laboratory: SPEAG, Zurich, Switzerland

**DUT: Dipole 2450 MHz ; Type: D2450V2; Serial: D2450V2 - SN: 715**

Communication System: UID 0 - CW; Frequency: 2450 MHz

Medium parameters used:  $f = 2450$  MHz;  $\sigma = 1.87$  S/m;  $\epsilon_r = 38.2$ ;  $\rho = 1000$  kg/m<sup>3</sup>

Phantom section: Flat Section

Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2011)

DASY52 Configuration:

- Probe: EX3DV4 - SN7349; ConvF(7.67, 7.67, 7.67); Calibrated: 30.12.2014;
- Sensor-Surface: 1.4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn601; Calibrated: 17.08.2015
- Phantom: Flat Phantom 5.0 (front); Type: QD000P50AA; Serial: 1001
- DASY52 52.8.8(1222); SEMCAD X 14.6.10(7331)

**Dipole Calibration for Head Tissue/Pin=250 mW, d=10mm/Zoom Scan (7x7x7)/Cube 0:**


Measurement grid: dx=5mm, dy=5mm, dz=5mm

Reference Value = 116.3 V/m; Power Drift = 0.01 dB

Peak SAR (extrapolated) = 28.7 W/kg


**SAR(1 g) = 13.7 W/kg; SAR(10 g) = 6.34 W/kg**

Maximum value of SAR (measured) = 23.3 W/kg

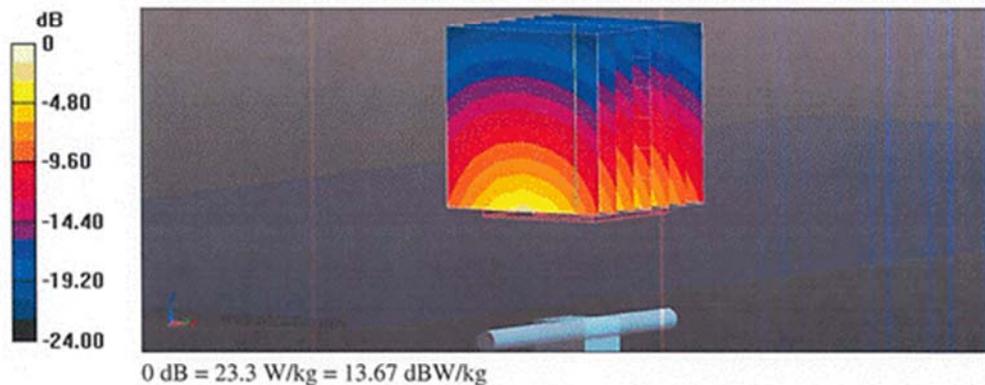



### Impedance Measurement Plot for Head TSL

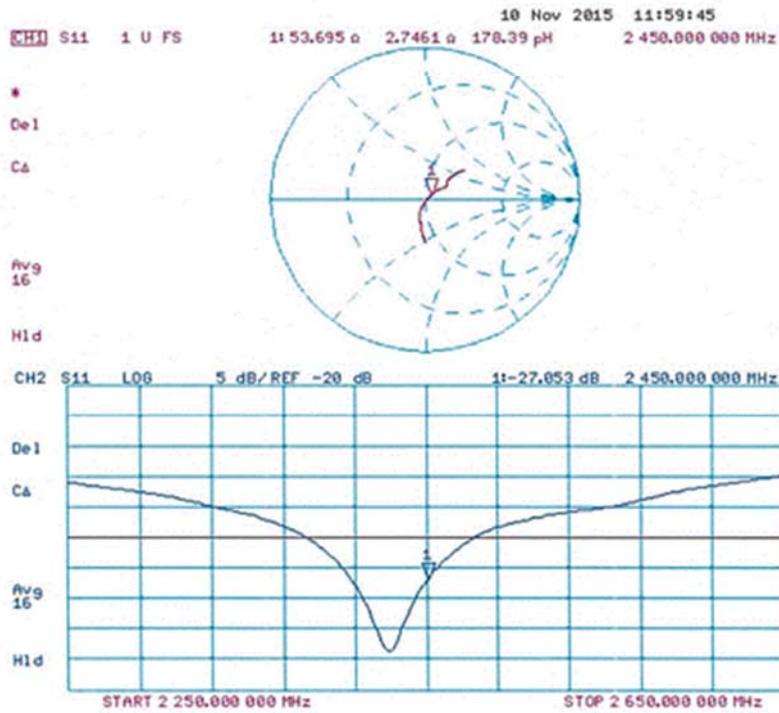



## DASY5 Validation Report for Body TSL

Date: 10.11.2015

Test Laboratory: SPEAG, Zurich, Switzerland

**DUT: Dipole 2450 MHz; Type: D2450V2; Serial: D2450V2 - SN: 715**

Communication System: UID 0 - CW; Frequency: 2450 MHz

Medium parameters used:  $f = 2450$  MHz;  $\sigma = 2.02$  S/m;  $\epsilon_r = 52.7$ ;  $\rho = 1000$  kg/m<sup>3</sup>

Phantom section: Flat Section

Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2011)

DASY52 Configuration:

- Probe: EX3DV4 - SN7349; ConvF(7.53, 7.53, 7.53); Calibrated: 30.12.2014;
- Sensor-Surface: 1.4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn601; Calibrated: 17.08.2015
- Phantom: Flat Phantom 5.0 (back); Type: QD000P50AA; Serial: 1002
- DASY52 52.8.8(1222); SEMCAD X 14.6.10(7331)

### Dipole Calibration for Body Tissue/Pin=250 mW, d=10mm/Zoom Scan (7x7x7)/Cube 0:


Measurement grid: dx=5mm, dy=5mm, dz=5mm

Reference Value = 109.5 V/m; Power Drift = 0.01 dB

Peak SAR (extrapolated) = 27.2 W/kg

SAR(1 g) = 13.6 W/kg; SAR(10 g) = 6.38 W/kg

Maximum value of SAR (measured) = 22.2 W/kg

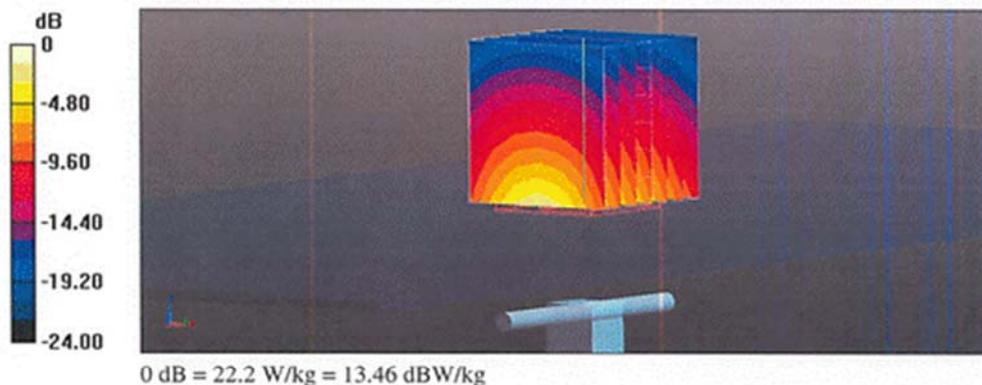



### Impedance Measurement Plot for Body TSL

