



Tel: +86-10-62304633-2711

E-mail: emf@caict.ac.cn

http://www.caict.ac.cn

### Appendix (Additional assessments outside the scope of CNAS L0570)

### Antenna Parameters with Head TSL at 4500 MHz

Impedance, transformed to feed point	47.1Ω - 4.03jΩ
Return Loss	- 25.8dB

### Antenna Parameters with Head TSL at 4700 MHz

Impedance, transformed to feed point	55.3Ω - 1.24jΩ
Return Loss	- 25.7dB

### General Antenna Parameters and Design

Electrical Delay (one direction)	1.015 ns
----------------------------------	----------

After long term use with 100W radiated power, only a slight warming of the dipole near the feed-point can be measured.

The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals. On some of the dipoles, small end caps are added to the dipole arms in order to improve matching when loaded according to the position as explained in the "Measurement Conditions" paragraph. The SAR data are not affected by this change. The overall dipole length is still according to the Standard. No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feed-point may be damaged.

### Additional EUT Data

Manufactured by	SPEAG
-----------------	-------

Certificate No: Z22-60455



Date: 2022-10-20

Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China

Tel: +86-10-62304633-2711

E-mail: emf@caict.ac.cn

http://www.caict.ac.cn

### **DASY5 Validation Report for Head TSL**

Test Laboratory: CTTL, Beijing, China

DUT: Dipole 4600 MHz; Type: D4600V2; Serial: D4600V2 - SN: 1033

Communication System: UID 0, CW; Frequency: 4500 MHz; Frequency: 4700 MHz Medium parameters used: f = 4500 MHz;  $\sigma = 3.87$  S/m;  $\epsilon_r = 36.69$ ;  $\rho = 1000$  kg/m<sup>3</sup> Medium parameters used: f = 4700 MHz;  $\sigma = 4.113$  S/m;  $\epsilon_r = 36.186$ ;  $\rho = 1000$  kg/m<sup>3</sup>

Phantom section: Right Section

Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2007)

DASY5 Configuration:

Certificate No: Z22-60455

- Probe: EX3DV4 SN7464; ConvF(6.53, 6.53, 6.53) @ 4500 MHz;
   ConvF(6.4, 6.4, 6.4) @ 4700 MHz; Calibrated: 2022-01-26
- Sensor-Surface: 1.4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn1556; Calibrated: 2022-01-12
- Phantom: MFP\_V5.1C (20deg probe tilt); Type: QD 000 P51 Cx; Serial: 1062
- DASY52 52.10.4(1535); SEMCAD X 14.6.14(7501)

Dipole Calibration /Pin=100mW, d=10mm, f=4500 MHz/Zoom Scan,

dist=1.4mm (8x8x7)/Cube 0: Measurement grid: dx=4mm, dy=4mm, dz=1.4mm

Reference Value = 61.33 V/m; Power Drift = 0.02 dB

Peak SAR (extrapolated) = 20.4 W/kg

SAR(1 g) = 6.78 W/kg; SAR(10 g) = 2.25 W/kg

Smallest distance from peaks to all points 3 dB below = 7.9 mm

Ratio of SAR at M2 to SAR at M1 = 72.7%

Maximum value of SAR (measured) = 13.8 W/kg

Dipole Calibration /Pin=100mW, d=10mm, f=4700 MHz/Zoom Scan,

dist=1.4mm (8x8x7)/Cube 0: Measurement grid: dx=4mm, dy=4mm, dz=1.4mm

Reference Value = 59.59 V/m; Power Drift = 0.00 dB

Peak SAR (extrapolated) = 20.8 W/kg

SAR(1 g) = 6.61 W/kg; SAR(10 g) = 2.17 W/kg

Smallest distance from peaks to all points 3 dB below = 8 mm

Ratio of SAR at M2 to SAR at M1 = 70.9%

Maximum value of SAR (measured) = 13.8 W/kg

Page 5 of 7



# S D e a g CALIBRATION LABORATORY




Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China

Tel: +86-10-62304633-2711

E-mail: emf@caict.ac.cn

http://www.caict.ac.cn

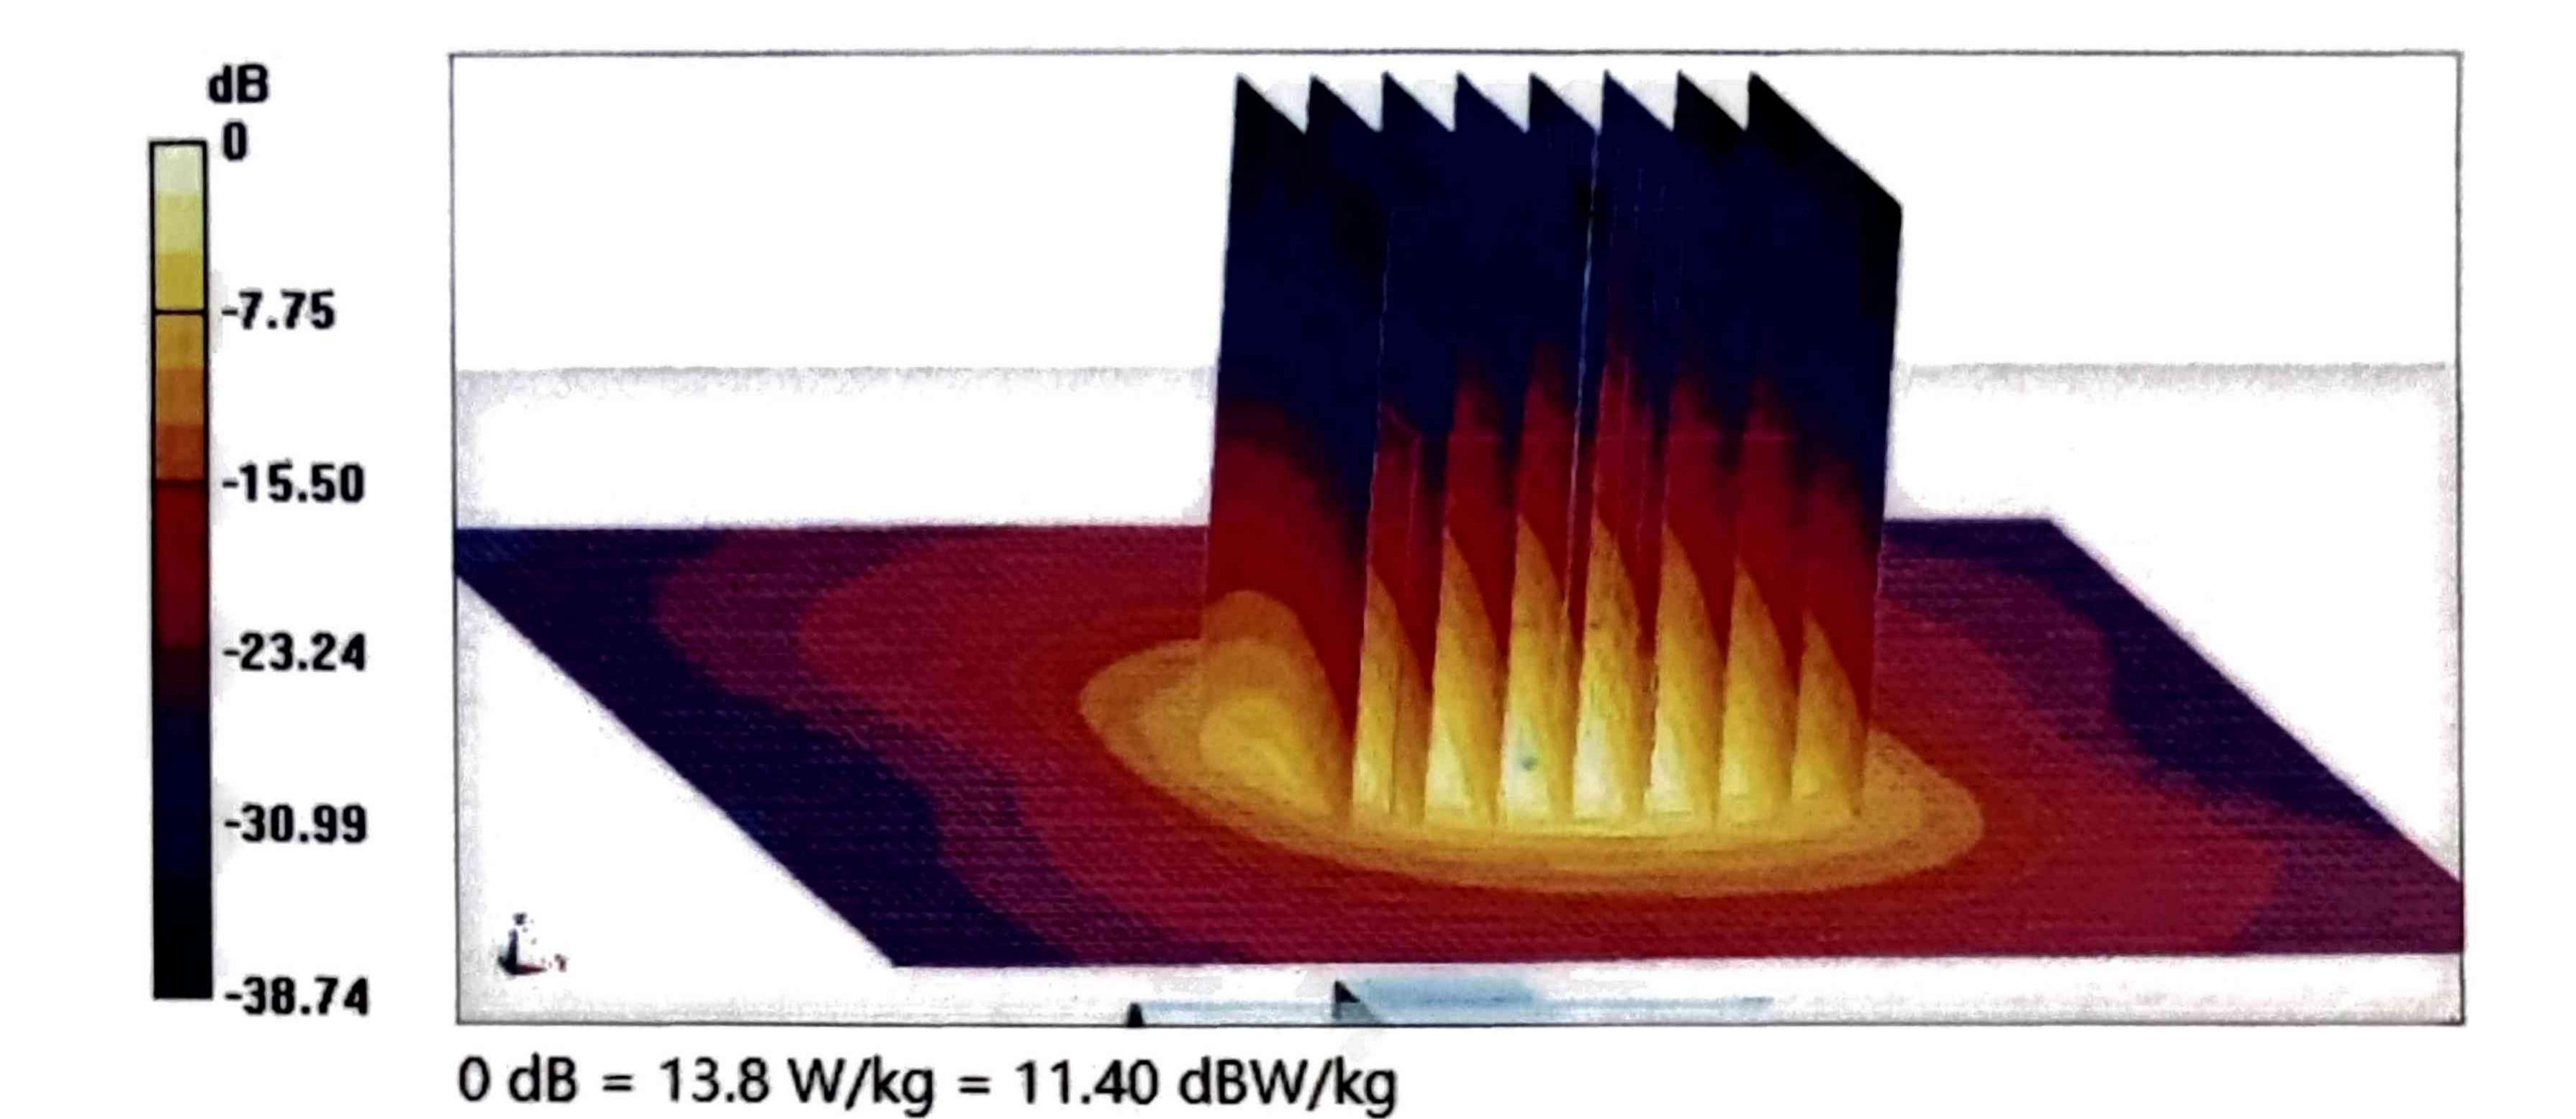

Certificate No: Z22-60455




Tel: +86-10-62304633-2711

B-mail: emf@caict.ac.cn

http://www.caict.ac.cn

### Impedance Measurement Plot for Head TSL

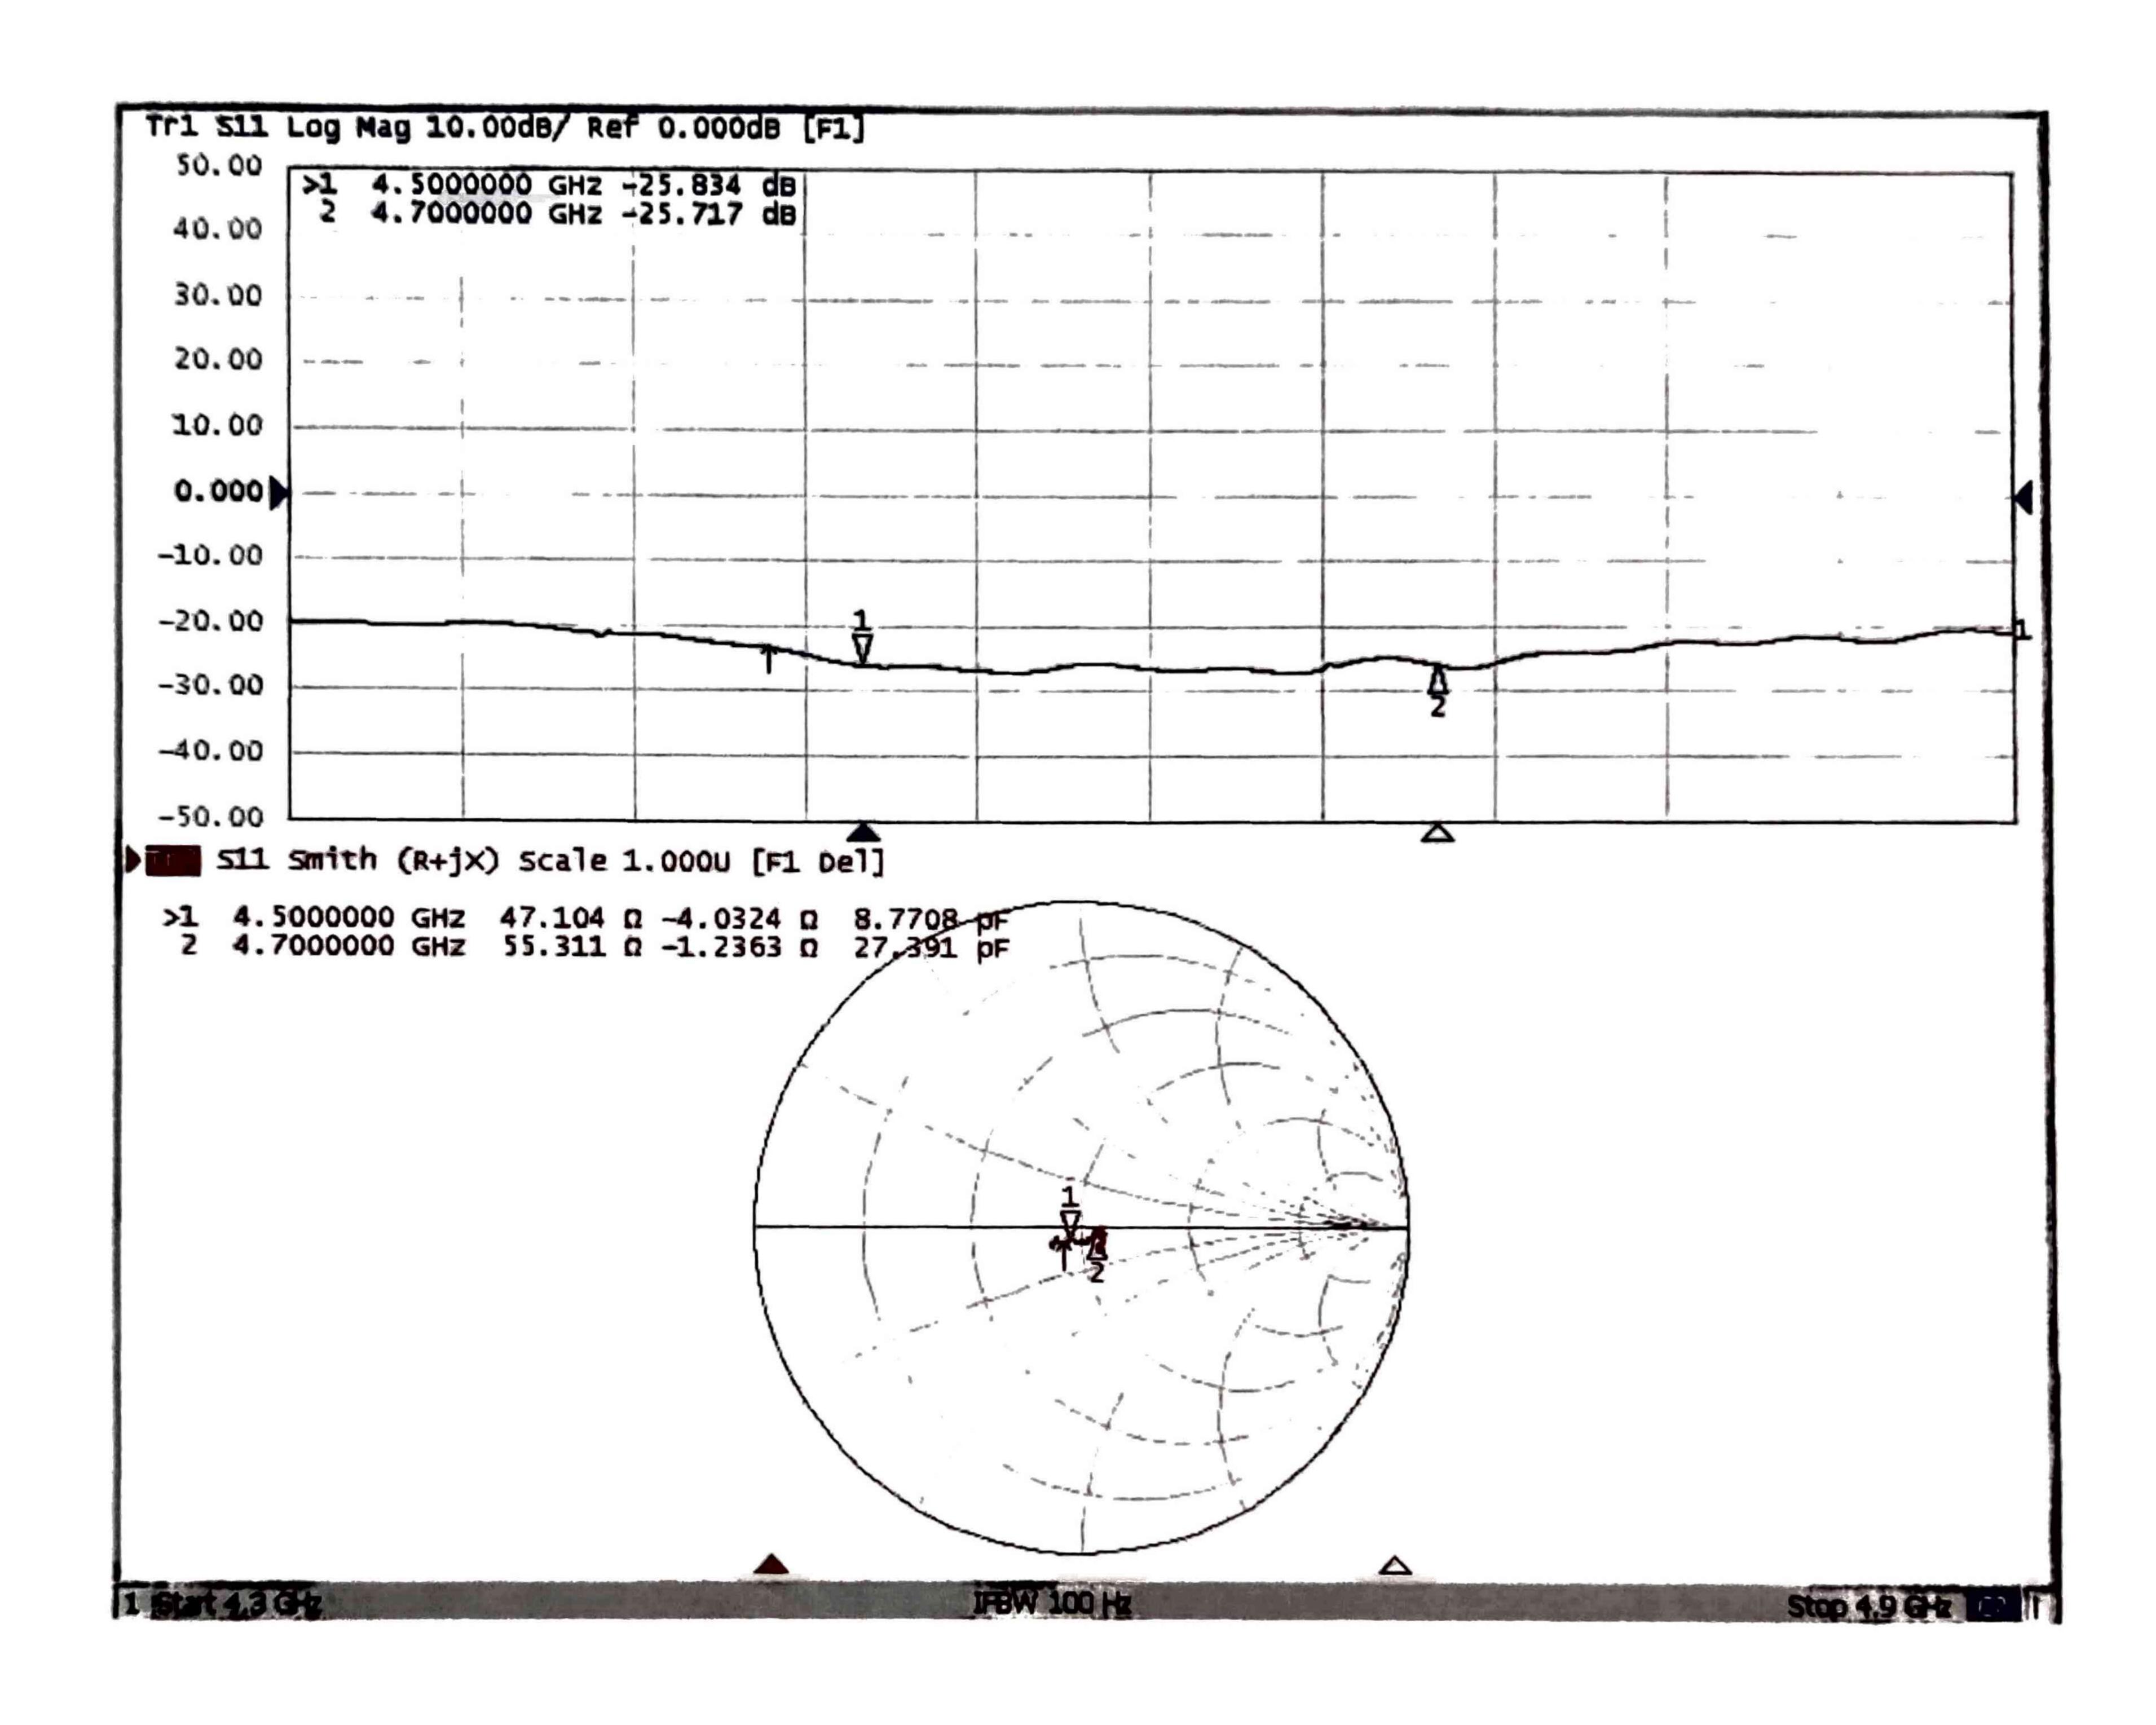







Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191

Tel: +86-10-62304633-2117

E-mail: emf@caict.ac.cn

http://www.caict.ac.cn

Client

SRTC

Certificate No:

Z22-60456

## CALIBRATION CERTIFICATE

Object

D4900V2 - SN: 1025

Calibration Procedure(s)

FF-Z11-003-01

Calibration Procedures for dipole validation kits

Calibration date:

October 21, 2022

This calibration Certificate documents the traceability to national standards, which realize the physical units of measurements (SI). The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility: environment temperature (22±3)℃ and humidity<70%.

Calibration Equipment used (M&TE critical for calibration)

Primary Standards	ID#	Cal Date (Calibrated by, Certificate No.)	Scheduled Calibration
Power Meter NRP2	106276	10-May-22 (CTTL, No.J22X03103)	May-23
Power sensor NRP6A	101369	10-May-22 (CTTL, No.J22X03103)	May-23
Reference Probe EX3DV4	SN 7464	26-Jan-22(SPEAG,No.EX3-7464_Jan22)	Jan-23
DAE4	SN 1556	12-Jan-22(CTTL-SPEAG,No.Z22-60007)	Jan-23
Secondary Standards	ID#	Cal Date (Calibrated by, Certificate No.)	Scheduled Calibration
Signal Generator E4438C	MY49071430	13-Jan-22 (CTTL, No.J22X00409)	Jan-23
Network Analyzer E5071C	MY46110673	14-Jan-22 (CTTL, No.J22X00406)	Jan-23

Name Function

Calibrated by: Zhao Jing SAR Test Engineer

Reviewed by:

Lin Hao

SAR Test Engineer

Approved by:

Qi Dianyuan


SAR Project Leader

Issued: October 31, 2022

Signature

This calibration certificate shall not be reproduced except in full without written approval of the laboratory.

Certificate No: Z22-60456

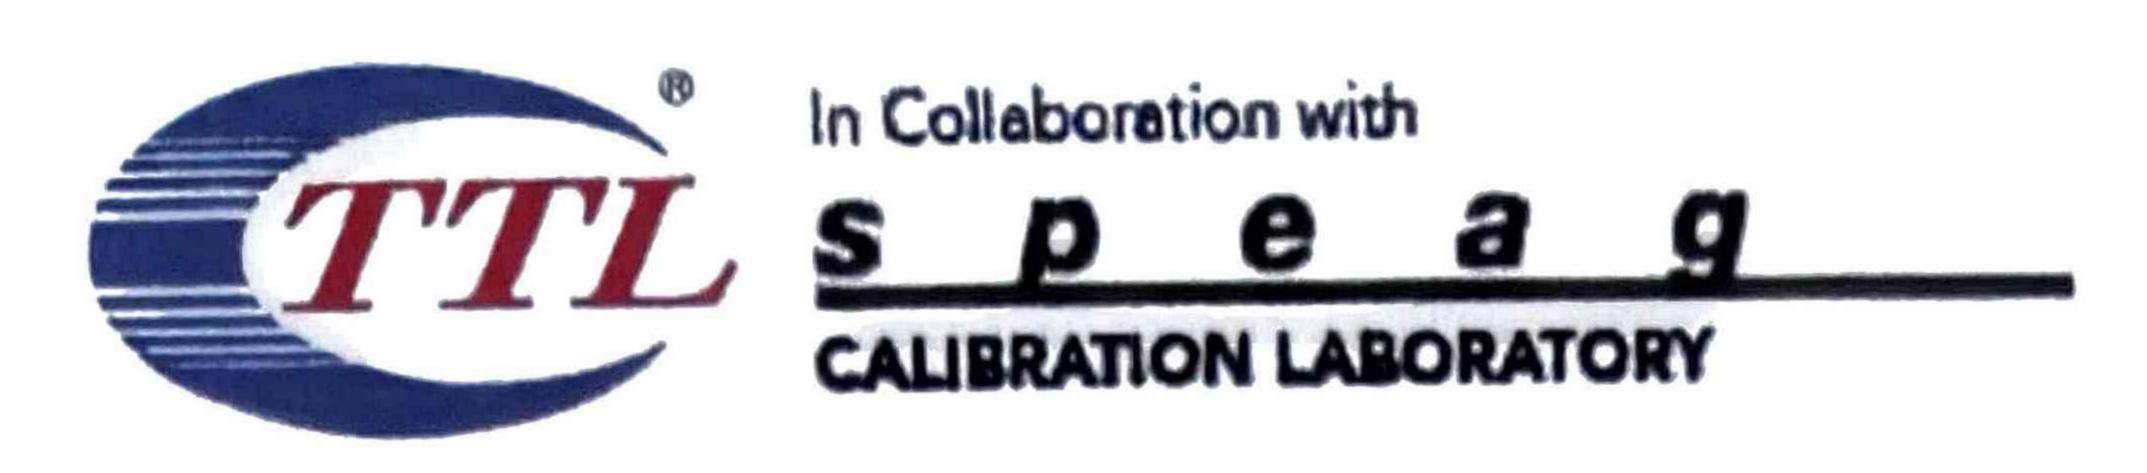



Tel: +86-10-62304633-2711

B-mail: emf@caict.ac.cn

http://www.caict.ac.cn

Glossary:

TSL tissue sim

tissue simulating liquid

ConvF

sensitivity in TSL / NORMx,y,z

N/A not applicable or not measured

## Calibration is Performed According to the Following Standards:

a) IEC/IEEE 62209-1528, "Measurement Procedure for The Assessment of Specific Absorption Rate of Human Exposure to Radio Frequency Fields from Hand-held and Body-mounted Wireless Communication Devices- Part 1528: Human Models, Instrumentation and Procedures (Frequency range of 4 MHz to 10 GHz)", October 2020

b) KDB 865664, "SAR Measurement Requirements for 100 MHz to 6 GHz"

### Additional Documentation:


c) DASY4/5 System Handbook

### Methods Applied and Interpretation of Parameters:

- Measurement Conditions: Further details are available from the Validation Report at the end
  of the certificate. All figures stated in the certificate are valid at the frequency indicated.
- Antenna Parameters with TSL: The dipole is mounted with the spacer to position its feed
  point exactly below the center marking of the flat phantom section, with the arms oriented
  parallel to the body axis.
- Feed Point Impedance and Return Loss: These parameters are measured with the dipole
  positioned under the liquid filled phantom. The impedance stated is transformed from the
  measurement at the SMA connector to the feed point. The Return Loss ensures low
  reflected power. No uncertainty required.
- Electrical Delay: One-way delay between the SMA connector and the antenna feed point.
   No uncertainty required.
- SAR measured: SAR measured at the stated antenna input power.
- SAR normalized: SAR as measured, normalized to an input power of 1 W at the antenna connector.
- SAR for nominal TSL parameters: The measured TSL parameters are used to calculate the nominal SAR result.

The reported uncertainty of measurement is stated as the standard uncertainty of Measurement multiplied by the coverage factor k=2, which for a normal distribution Corresponds to a coverage probability of approximately 95%.

Certificate No: Z22-60456 Page 2 of 6

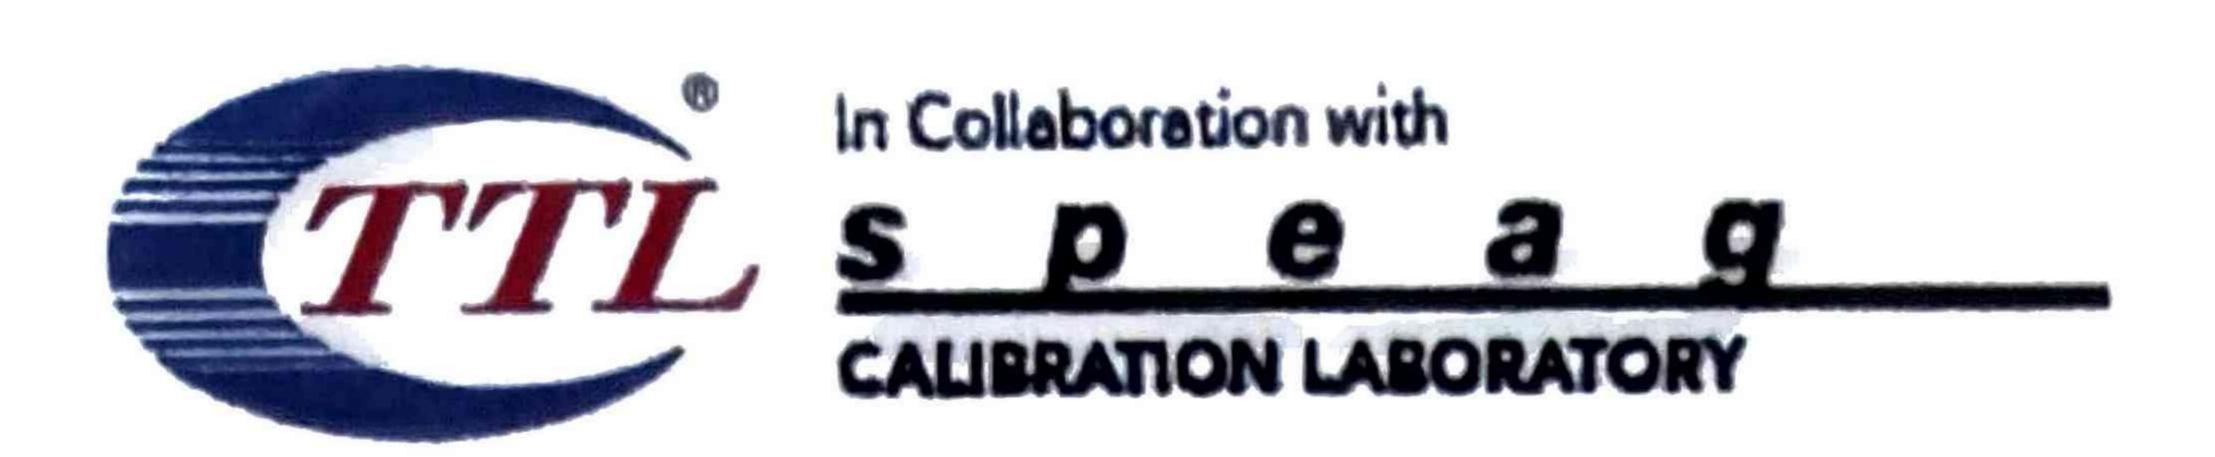



Tel: +86-10-62304633-2711

B-mail: emf@caict.ac.cn

http://www.caict.ac.cn

### Measurement Conditions

DASY system configuration, as far as not given on page 1.

DASY system configuration, as far as not given on page 1.			
DASY Version	DASY52	52.10.4	
Extrapolation	Advanced Extrapolation		
Phantom	Triple Flat Phantom 5.1C		
Distance Dipole Center - TSL	10 mm	with Spacer	
Zoom Scan Resolution	dx, dy = 4 mm, dz = 1.4 mm	Graded Ratio = 1.4 (Z direction)	
Frequency	4900 MHz ± 1 MHz		

## Head TSL parameters at 4900 MHz


The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Head TSL parameters	22.0 ℃	36.3	4.35 mho/m
Measured Head TSL parameters	(22.0 ± 0.2) ℃	36.8 ±6 %	4.37 mho/m ±6 %
Head TSL temperature change during test	<1.0 ℃		

### SAR result with Head TSL at 4900 MHz

ticout with ficure to at 4000 mile			
SAR averaged over 1 $cm^3$ (1 g) of Head TSL	Condition		
SAR measured	100 mW input power	6.95 W/kg	
SAR for nominal Head TSL parameters	normalized to 1W	69.7 W/kg ± 24.4 % (k=2)	
SAR averaged over 10 cm <sup>3</sup> (10 g) of Head TSL	Condition		
SAR measured	100 mW input power	2.19 W/kg	
SAR for nominal Head TSL parameters	normalized to 1W	22.0 W/kg ±24.2 % (k=2)	

Certificate No: Z22-60456

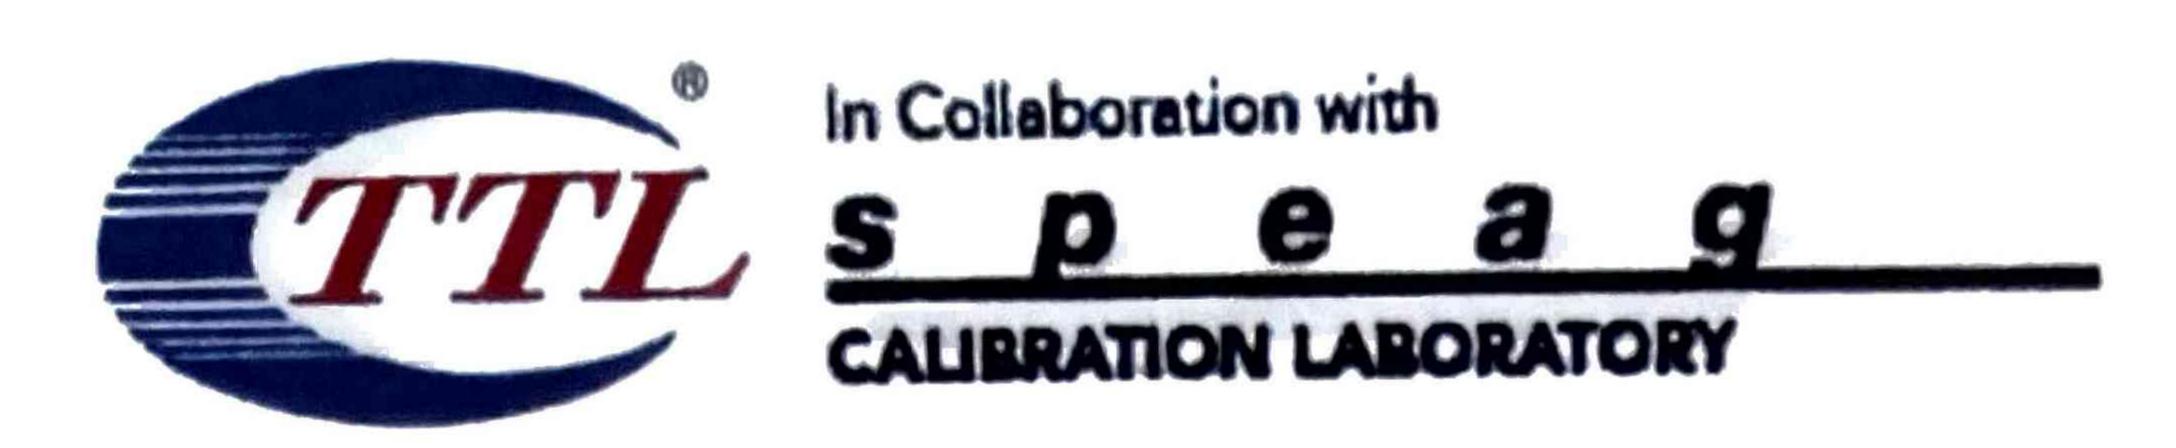



Tel: +86-10-62304633-2711

E-mail: emf@caict.ac.cn http://www.caict.ac.cn

## Appendix (Additional assessments outside the scope of CNAS L0570)

### Antenna Parameters with Head TSL at 4900MHz

Impedance, transformed to feed point	51.2Ω- 4.95jΩ
Return Loss	- 26.0dB

### General Antenna Parameters and Design

Electrical Delay (one direction)	0.998 ns


After long term use with 100W radiated power, only a slight warming of the dipole near the feed-point can be measured.

The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals. On some of the dipoles, small end caps are added to the dipole arms in order to improve matching when loaded according to the position as explained in the "Measurement Conditions" paragraph. The SAR data are not affected by this change. The overall dipole length is still according to the Standard. No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feed-point may be damaged.

### **Additional EUT Data**

Manufactured by	SPEAG

Certificate No: Z22-60456 Page 4 of 6

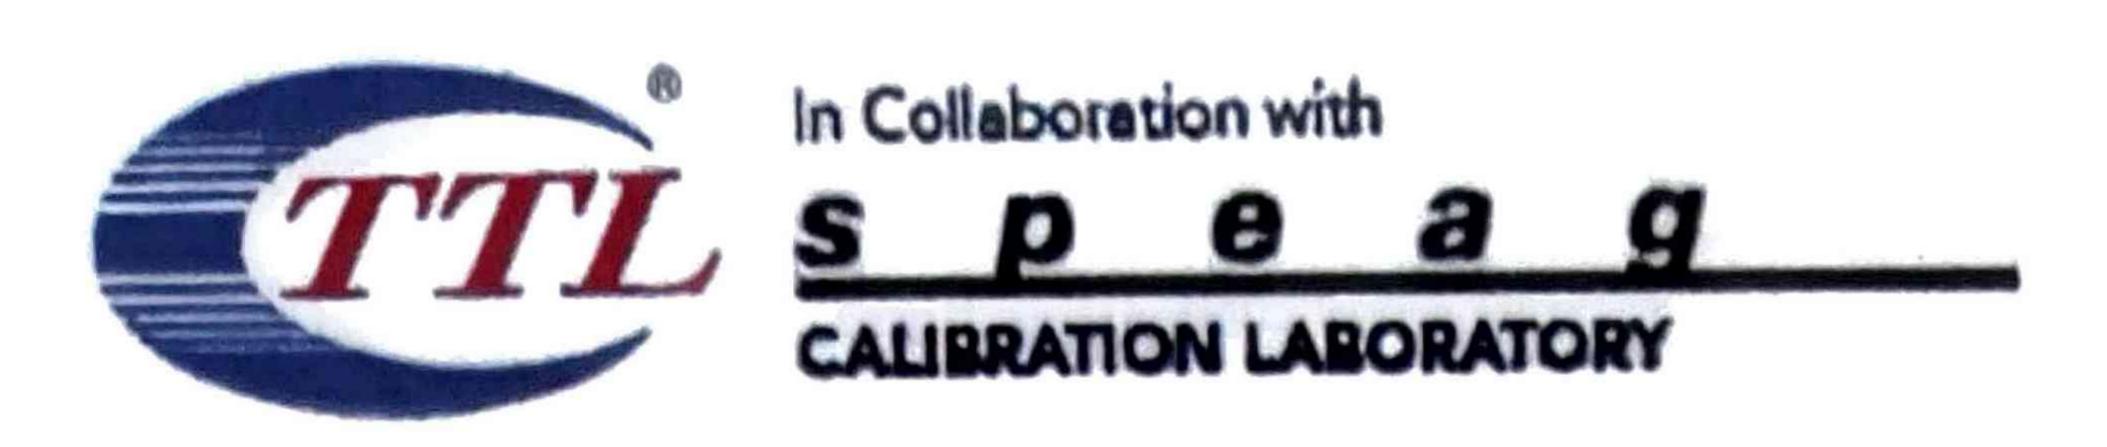



Date: 2022-10-21

Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China

Tel: +86-10-62304633-2711

E-mail: emf@caict.ac.cn http://www.caict.ac.cn

### DASY5 Validation Report for Head TSL

Test Laboratory: CTTL, Beijing, China

DUT: Dipole 4900 MHz; Type: D4900V2; Serial: D4900V2 - SN: 1025

Communication System: UID 0, CW; Frequency: 4900 MHz

Medium parameters used: f = 4900 MHz;  $\sigma = 4.372$  S/m;  $\varepsilon_r = 36.81$ ;  $\rho = 1000$  kg/m<sup>3</sup>

Phantom section: Right Section

Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2007)

DASY5 Configuration:

- Probe: EX3DV4 SN7464; ConvF(6, 6, 6) @ 4900 MHz; Calibrated:
   2022-01-26
- Sensor-Surface: 1.4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn1556; Calibrated: 2022-01-12
- Phantom: MFP\_V5.1C (20deg probe tilt); Type: QD 000 P51 Cx; Serial:
   1062
- DASY52 52.10.4(1535); SEMCAD X 14.6.14(7501)

Dipole Calibration /Pin=100mW, d=10mm, f=4900 MHz/Zoom Scan,

dist=1.4mm (8x8x7)/Cube 0: Measurement grid: dx=4mm, dy=4mm, dz=1.4mm

Reference Value = 64.57 V/m; Power Drift = -0.01 dB


Peak SAR (extrapolated) = 23.9 W/kg

SAR(1 g) = 6.95 W/kg; SAR(10 g) = 2.19 W/kg

Smallest distance from peaks to all points 3 dB below = 8 mm


Ratio of SAR at M2 to SAR at M1 = 68.5%

Maximum value of SAR (measured) = 15.3 W/kg

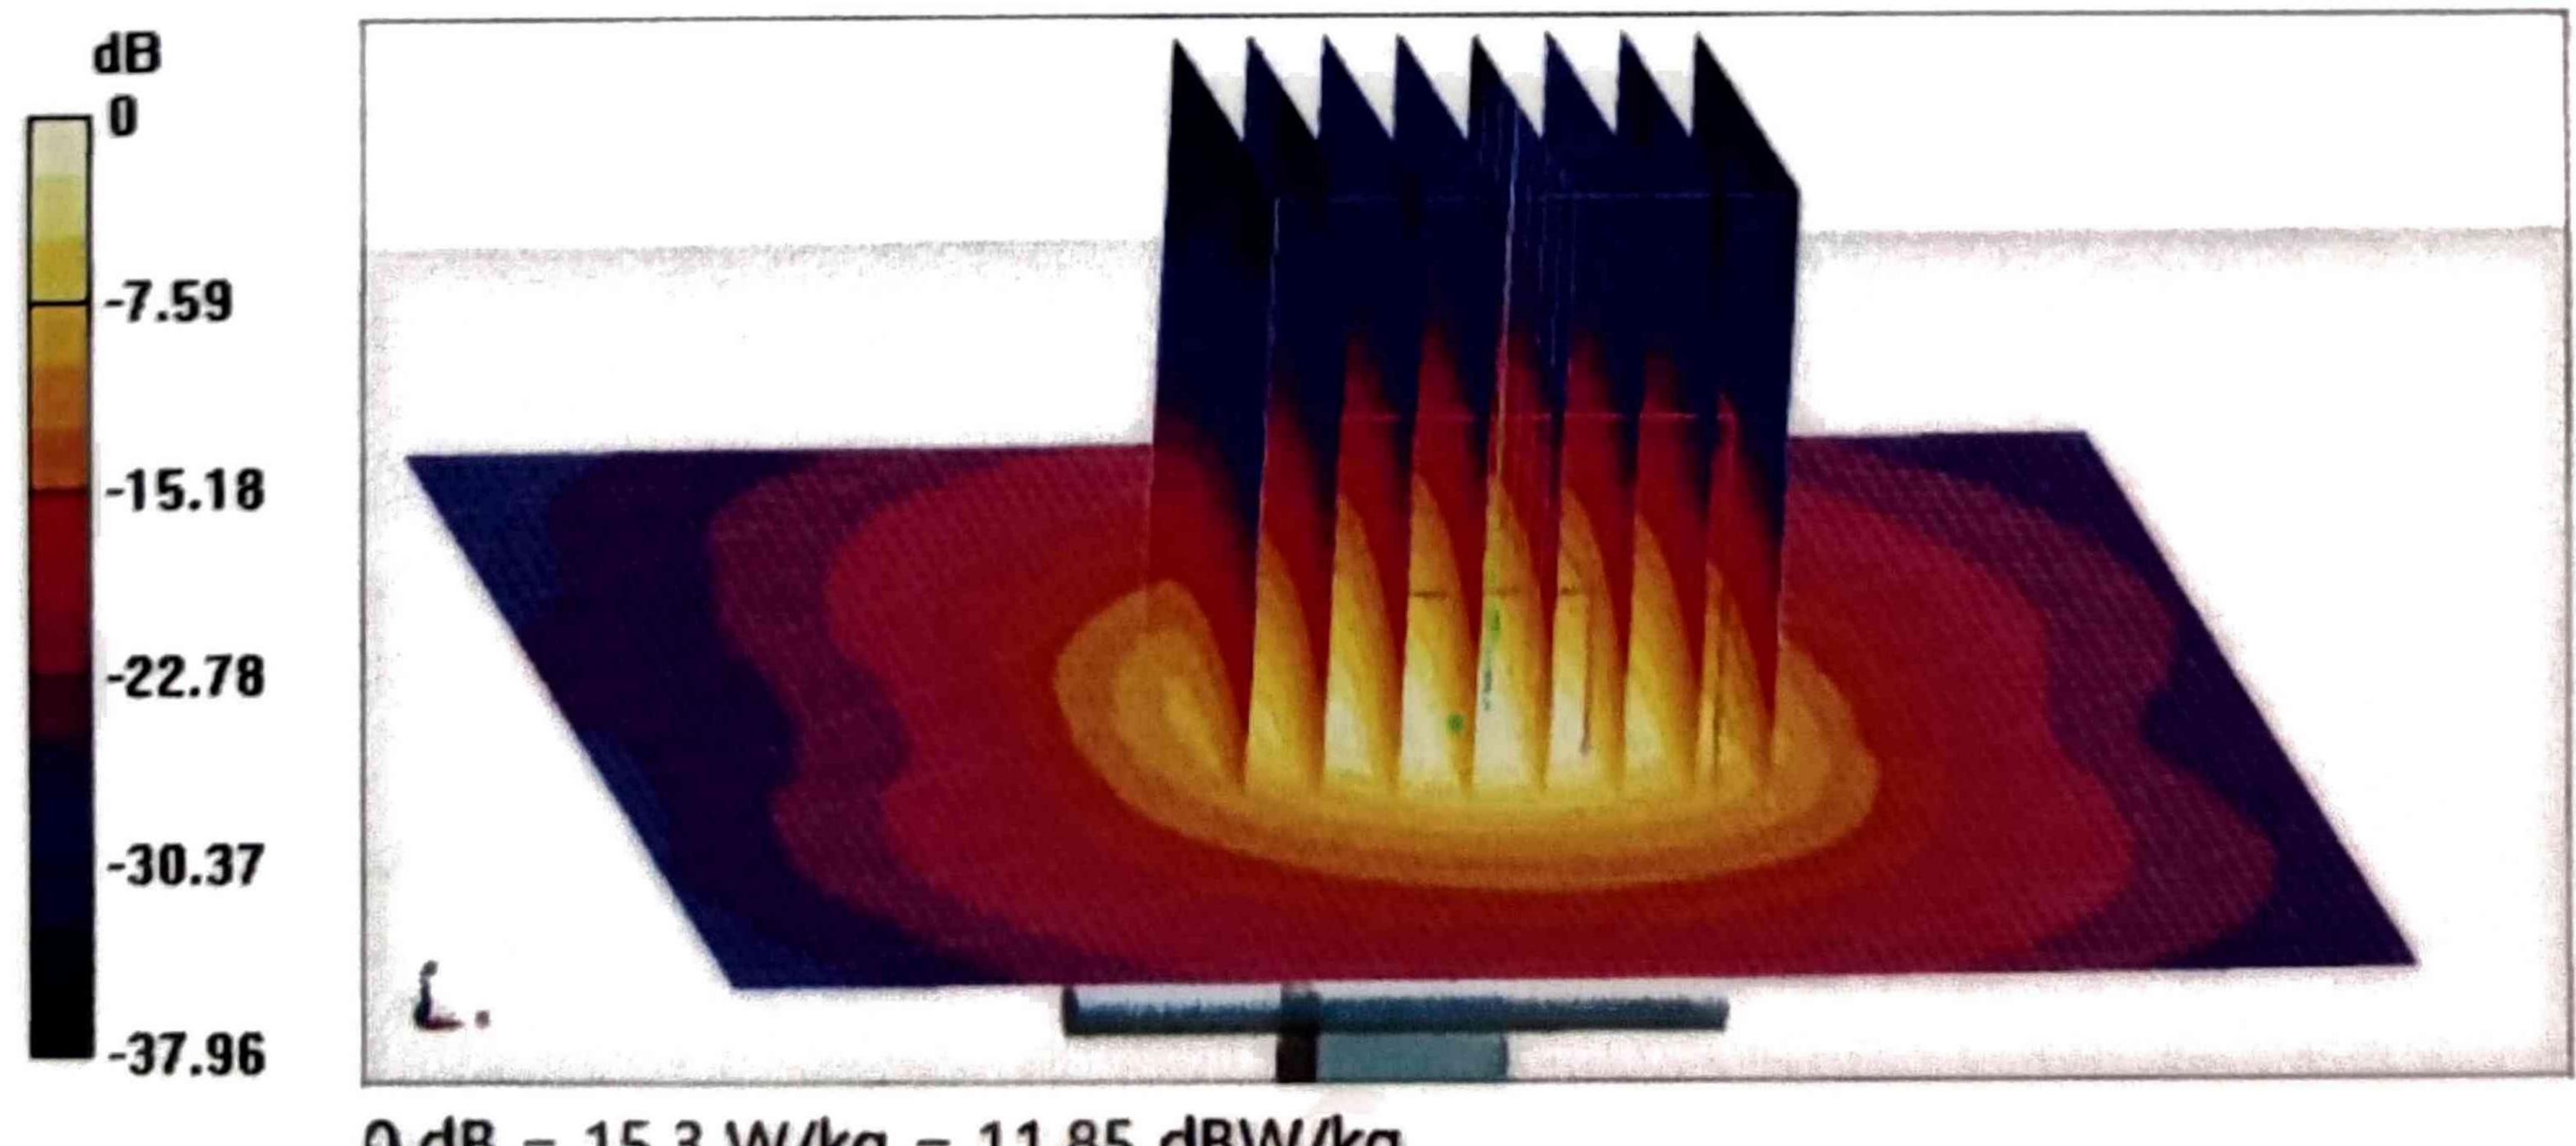

0 dB = 15.3 W/kg = 11.85 dBW/kg

Certificate No: Z22-60456 Page 5 of 6

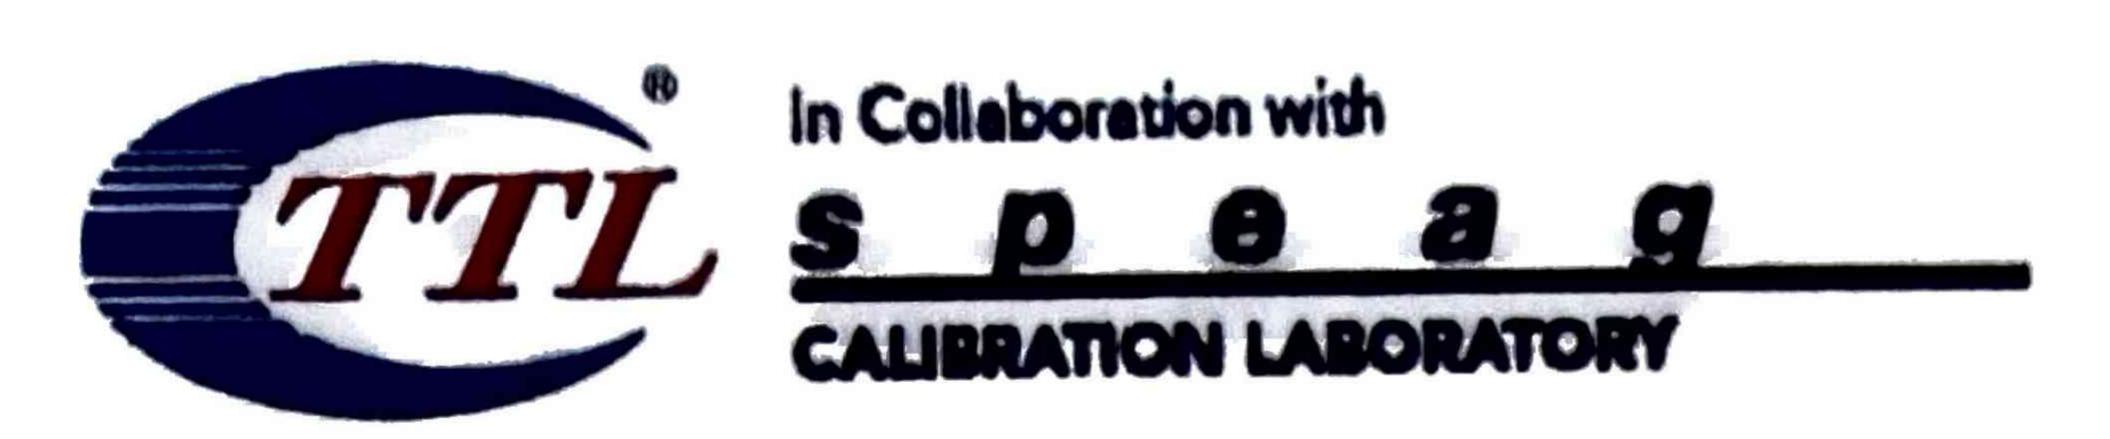





Tel: +86-10-62304633-2711

E-mail: emf@caict.ac.cn http://www.caict.ac.cn

### Impedance Measurement Plot for Head TSL

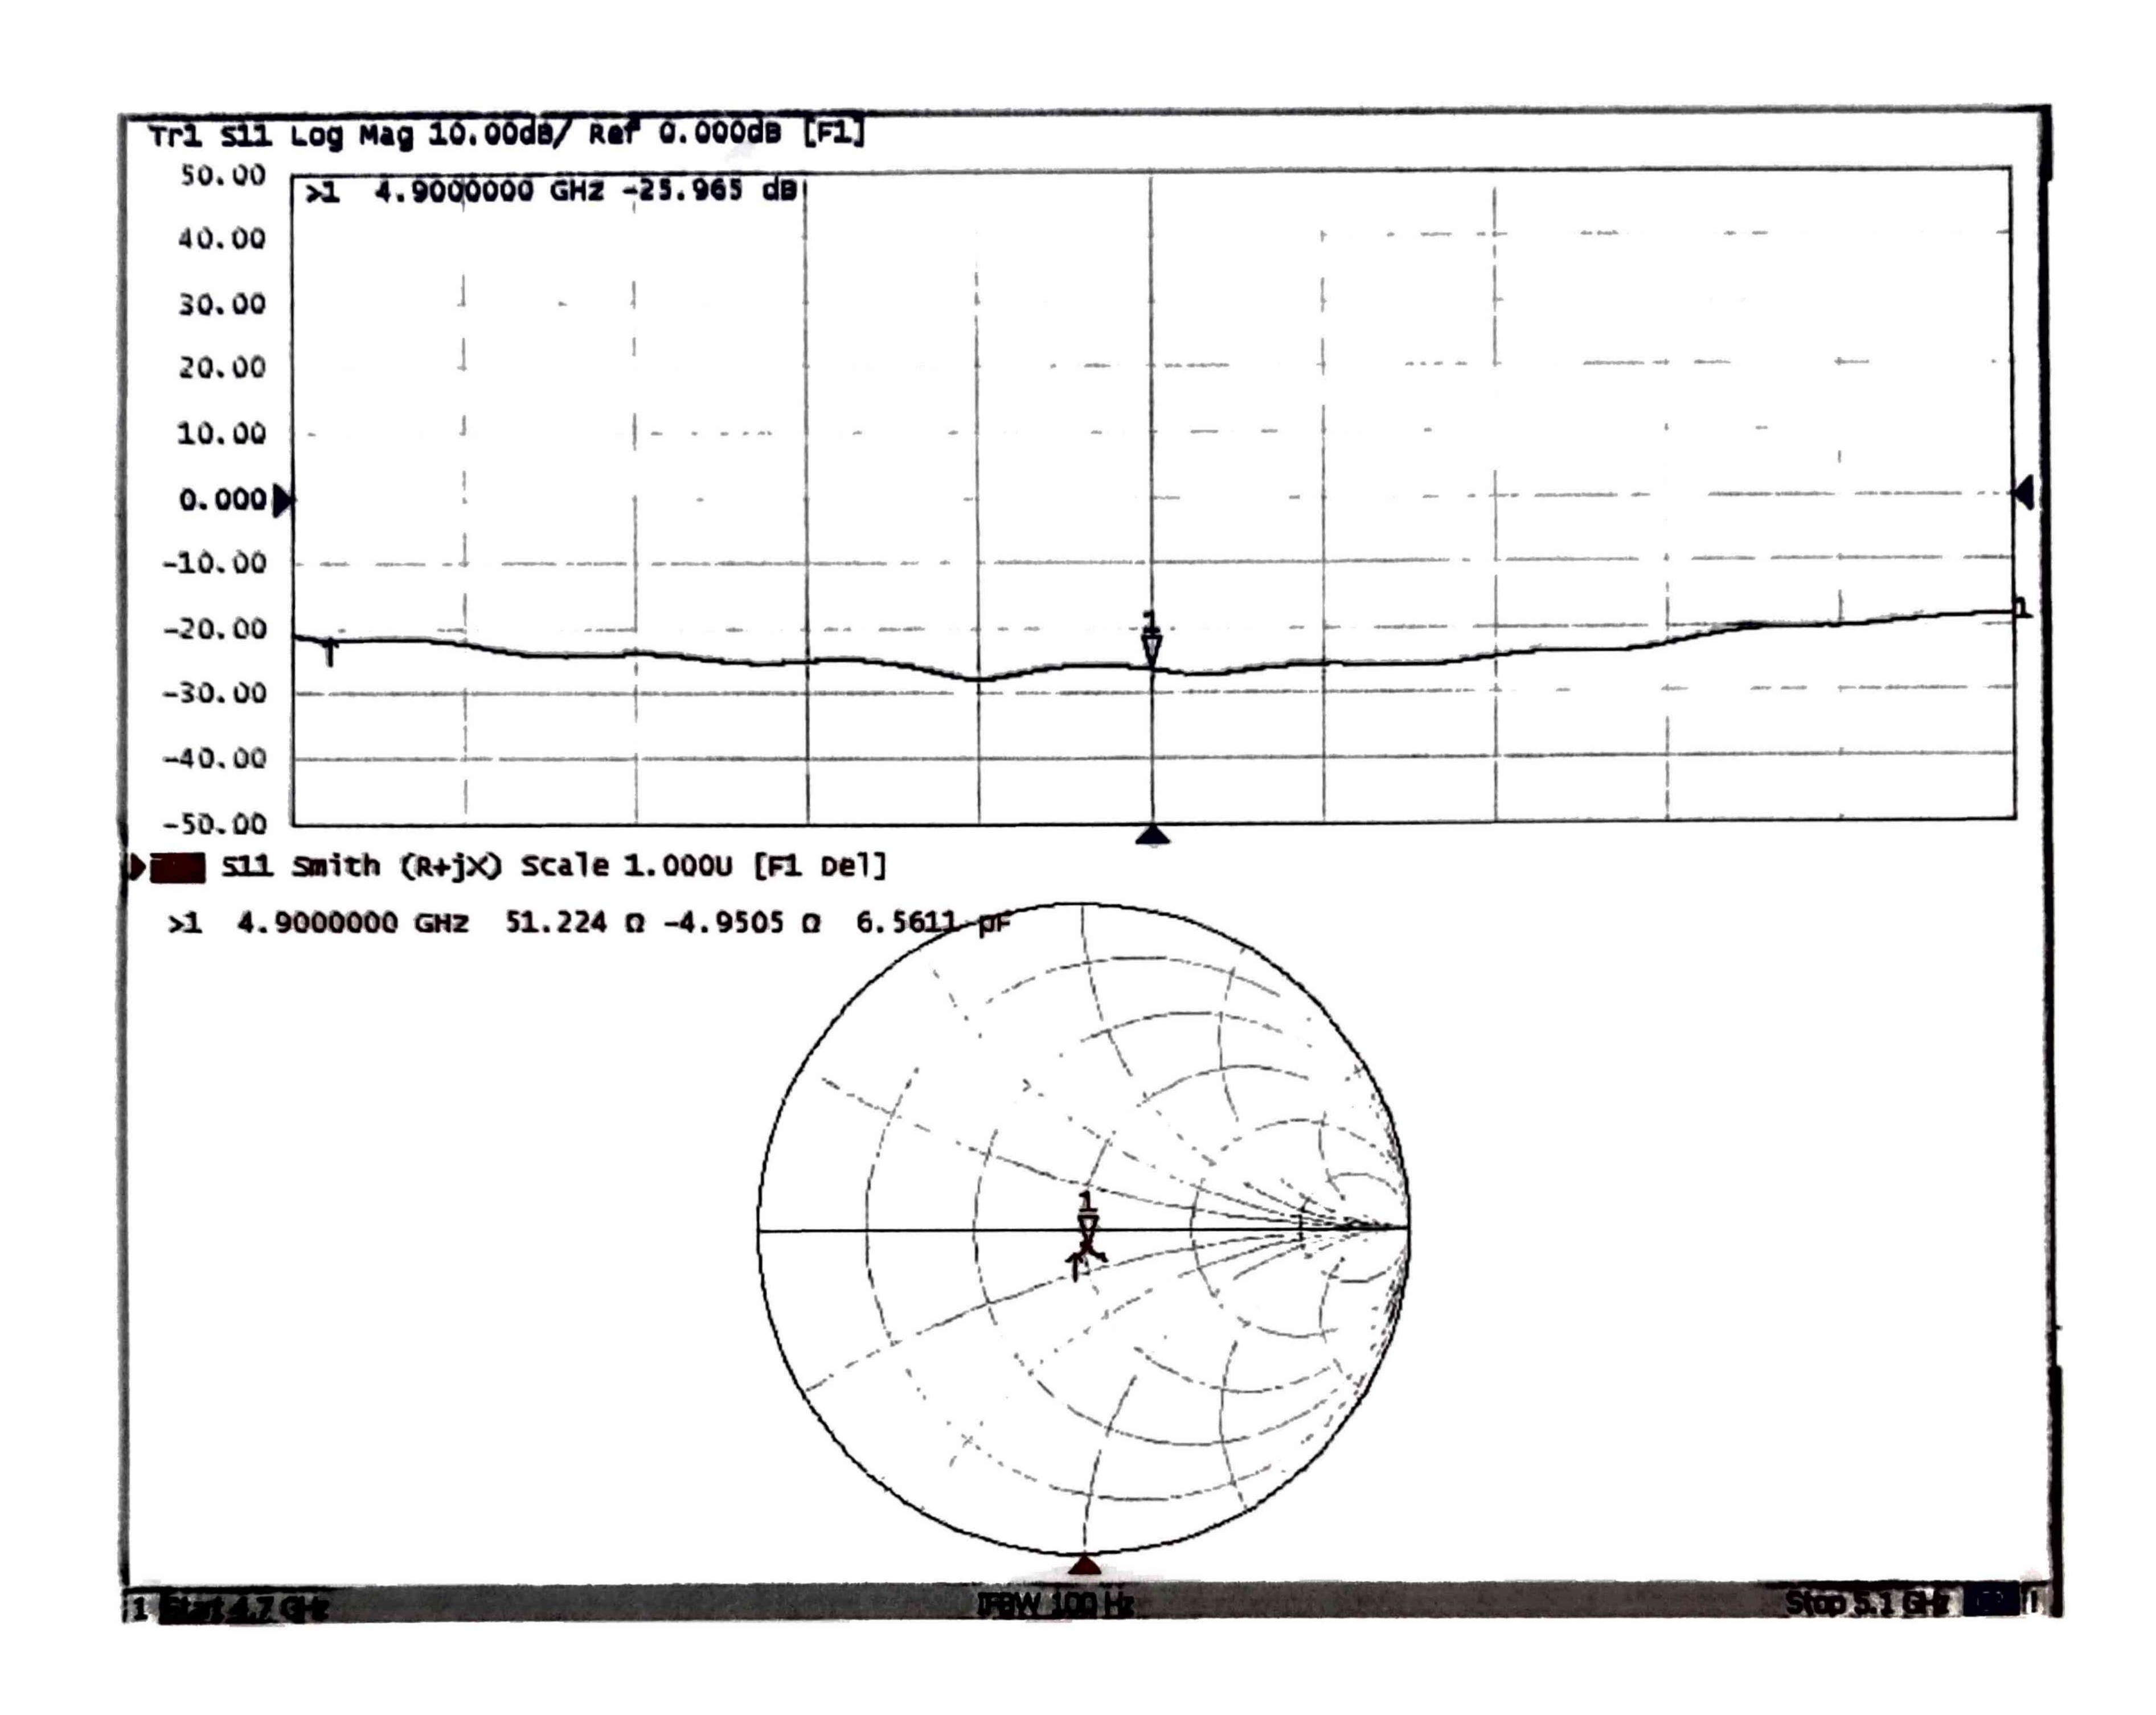







Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191 Tel: +86-10-62302117

E-mail: emf@caict.ac.cn

http://www.caict.ac.ca

Client

SRTC

Certificate No:

23J02Z80090

### **CALIBRATION CERTIFICATE**

Object D5GHzV2 - SN: 1079

Calibration Procedure(s)

FF-Z11-003-01

Calibration Procedures for dipole validation kits

Calibration date:

October 17, 2023

This calibration Certificate documents the traceability to national standards, which realize the physical units of measurements (SI). The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility: environment temperature (22±3)\*C and humidity<70%.

Calibration Equipment used (M&TE critical for calibration)

Primary Standards	ID#	Cal Date (Calibrated by, Certificate No.)	Scheduled Calibration
Power Meter NRP2	106276	15-May-23 (CTTL, No.J23X04183)	May-24
Power sensor NRP6A	101369	15-May-23 (CTTL, No.J23X04183)	May-24
Reference Probe EX3DV4	SN 3617	31-Mar-23(CTTL-SPEAG,No.Z23-60161)	Mar-24
DAE4	SN 1556	11-Jan-23(CTTL-SPEAG,No.Z23-60034)	Jan-24
Secondary Standards	ID#	Cal Date (Calibrated by, Certificate No.)	Scheduled Calibration
Signal Generator E4438C	MY49071430	05-Jan-23 (CTTL, No. J23X00107)	Jan-24
Network Analyzer E5071C	MY46110673	10-Jan-23 (CTTL, No. J23X00104)	Jan-24

Name Fun

Function

J M

Reviewed by:

Callbrated by:

Lin Hao

Zhao Jing

SAR Test Engineer

SAR Test Engineer

Approved by:

Qi Dianyuan

SAR Project Leader

in Charte

Issued: October 31, 2023

This calibration certificate shall not be reproduced except in full without written approval of the laboratory.

Certificate No: 23J02Z80090

Page 1 of 10



Add No.52 HuaYuanHei Road, Haidian District, Beijing, 100191, Ulima Fel: #86-10-62302117 B-mail: zmif@caict.ac.cn http://www.caict.ac.cn

Glossary:

TSL tissue simulating liquid

ConvF sensitivity in TSL / NORMx,y,z N/A not applicable or not measured

Calibration is Performed According to the Following Standards:

a) IEC/IEEE 62209-1528, "Measurement Procedure for The Assessment of Specific Absorption Rate of Human Exposure to Radio Frequency Fields from Hand-held and Body-mounted Wireless Communication Devices- Part 1528: Human Models, Instrumentation and Procedures (Frequency range of 4 MHz to 10 GHz)", October 2020

b) KDB 865664, "SAR Measurement Requirements for 100 MHz to 6 GHz"

### Additional Documentation:


c) DASY4/5 System Handbook

### Methods Applied and Interpretation of Parameters:

- Measurement Conditions: Further details are available from the Validation Report at the end
  of the certificate. All figures stated in the certificate are valid at the frequency indicated.
- Antenna Parameters with TSL: The dipole is mounted with the spacer to position its feed
  point exactly below the center marking of the flat phantom section, with the arms oriented
  parallel to the body axis.
- Feed Point Impedance and Return Loss: These parameters are measured with the dipole
  positioned under the liquid filled phantom. The Impedance stated is transformed from the
  measurement at the SMA connector to the feed point. The Return Loss ensures low
  reflected power. No uncertainty required.
- Electrical Delay: One-way delay between the SMA connector and the antenna feed point.
   No uncertainty required.
- SAR measured: SAR measured at the stated antenna input power.
- SAR normalized: SAR as measured, normalized to an input power of 1 W at the antenna connector.
- SAR for nominal TSL parameters: The measured TSL parameters are used to calculate the nominal SAR result.

The reported uncertainty of measurement is stated as the standard uncertainty of Measurement multiplied by the coverage factor k=2, which for a normal distribution Corresponds to a coverage probability of approximately 95%.

Certificate No: 23J02Z80090 Page 2 of 10





Tel: +86-10-62302117

E-mail: emf@caict.ac.cn

http://www.caict.ac.cn

### **Measurement Conditions**

ASY system configuration, as far as	not given on page 1.	W
DASY Version	DASY52	52,10,4
Extrapolation	Advanced Extrapolation	
Phantom	Triple Flat Phantom 5.1C	
Distance Dipole Center - TSL	10 mm	with Spacer
Zoom Scan Resolution	dx, dy = 4 mm, dz = 1.4 mm	Graded Ratio = 1.4 (Z direction)
Frequency	5200 MHz ± 1 MHz 5300 MHz ± 1 MHz 5500 MHz ± 1 MHz 5600 MHz ± 1 MHz 5800 MHz ± 1 MHz	

Head TSL parameters at 5200MHz


The following parameters and calculations were applied.

PW-1.	Temperature	Permittivity	Conductivity
Nominal Head TSL parameters	22.0 °C	36.0	4.66 mho/m
Measured Head TSL parameters	(22.0 ± 0.2) °C	36.3 ± 6 %	4.67 mho/m ± 6 %
Head TSL temperature change during test	<1.0 °C	-	-

### SAR result with Head TSL at 5200MHz

Certificate No: 23J02Z80090

SAR averaged over 1 cm <sup>3</sup> (1 g) of Head TSL	Condition	
SAR measured	250 mW input power	7.83 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	78.4 W/kg ± 24.4 % (k=2)
SAR averaged over 10 cm <sup>3</sup> (10 g) of Head TSL	Condition	
SAR measured	250 mW input power	2.20 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	22.1 W/kg ± 24.2 % (k=2)





E-mail: emf@caict.ac.en http://www.caict.ac.en

Head TSL parameters at 5300MHz

The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Head TSL parameters	22.0 °C	35.9	4.76 mho/m
Measured Head TSL parameters	(22.0 ± 0.2) °C	36.1 ± 6 %	4.79 mho/m ± 6 %
Head TSL temperature change during test	<1.0 °C	-	-

### SAR result with Head TSL at 5300MHz


SAR averaged over 1 cm <sup>3</sup> (1 g) of Head TSL	Condition	
SAR measured	100 mW input power	7.96 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	79,7 W/kg ± 24.4 % (k=2)
SAR averaged over 10 cm <sup>3</sup> (10 g) of Head TSL	Condition	
SAR measured	100 mW input power	2.25 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	22.5 W/kg ± 24.2 % (k=2)

Head TSL parameters at 5500MHz

	Temperature	Permittivity	Conductivity
Nominal Head TSL parameters	22.0 °C	35.6	4.96 mho/m
Measured Head TSL parameters	(22,0 ± 0,2) °C	35.8 ± 6 %	5.00 mho/m ± 6 %
Head TSL temperature change during test	<1.0 °C	-	_

### SAR result with Head TSL at 5500MHz

SAR averaged over 1 cm <sup>3</sup> (1 g) of Head TSL	Condition	
SAR measured	100 mW input power	8.27 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	82.8 W/kg ± 24.4 % (k=2)
SAR averaged over 10 cm <sup>3</sup> (10 g) of Head TSL	Condition	
SAR measured	100 mW input power	2.31 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	23.1 W/kg ± 24.2 % (k=2)





Tel: +86-10-62302117

E-mail: emf@caict.ac.cn http://www.naict.ac.cn

### Head TSL parameters at 5600MHz

The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Head TSL parameters	22.0 °C	35.5	5.07 mho/m
Measured Head TSL parameters	(22.0 ± 0.2) °C	35.6 ± 6 %	5.11 mho/m ± 6 %
Head TSL temperature change during test	<1.0 °C	-	_

### SAR result with Head TSL at 5600MHz

SAR averaged over 1 cm <sup>3</sup> (1 g) of Head TSL	Condition	
SAR measured	100 mW input power	8.13 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	81.4 W/kg ± 24.4 % (k=2)
SAR averaged over 10 cm <sup>3</sup> (10 g) of Head TSL	Condition	
SAR measured	100 mW input power	2.29 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	22.9 W/kg ± 24.2 % (k=2)

### Head TSL parameters at 5800MHz The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Head TSL parameters	22.0 °C	35,3	5.27 mho/m
Measured Head TSL parameters	(22.0 ± 0.2) °C	35.3 ± 6 %	5.31 mho/m ± 6 %
Head TSL temperature change during test	<1.0 °C	_	_

### SAR result with Head TSL at 5800MHz

Condition	
100 mW input power	7.88 W/kg
normalized to 1W	78.8 W/kg ± 24.4 % (k=2)
Condition	
100 mW input power	2.20 W/kg
normalized to 1W	22.0 W/kg ± 24.2 % (k=2
	100 mW input power normalized to 1W Condition 100 mW input power

Certificate No: 23J02Z80090 Page 5 of 10



Add: No.52 HuaYuanBei Road, Hardian District, Beijing, 100191, China. Tel: +56-10-62307117 E-mail: emfigicarctac.cn http://www.catct.ac.cn

### Appendix (Additional assessments outside the scope of CNAS L0570)

### Antenna Parameters with Head TSL at 5200MHz

Impedance, transformed to feed point	50.5Ω- 9.26jΩ
Return Loss	- 20.7dB

### Antenna Parameters with Head TSL at 5300MHz

Impedance, transformed to feed point	50.0Ω- 5.75 Ω	
Return Loss	- 24.8dB	

### Antenna Parameters with Head TSL at 5500MHz

Impedance, transformed to feed point	54.4Ω-4.97jΩ
Return Loss	+23.9dB


### Antenna Parameters with Head TSL at 5600MHz

Impedance, transformed to feed point	57.2Ω- 3.24jΩ
Return Loss	-22.6dB

### Antenna Parameters with Head TSL at 5800MHz

Impedance, transformed to feed point	56.9Ω-5.03jΩ
Return Loss	- 22.0dB

Certificate No: 23J02Z80090





Tel: +86-10-62302117

H-mail: emflécaict.sc.cn

http://www.caict.ac.cn

### General Antenna Parameters and Design

1	Electrical Delay (one direction)	1.110 ns
-		

After long term use with 100W radiated power, only a slight warming of the dipole near the feed-point can be measured.


The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals. On some of the dipoles, small end caps are added to the dipole arms in order to improve matching when loaded according to the position as explained in the "Measurement Conditions" paragraph. The SAR data are not affected by this change. The overall dipole length is still according to the Standard.

No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feed-point may be damaged.

### Additional EUT Data

Manufactured by SPEAG
-----------------------

Certificate No: 23J02Z80090 Page 7 of 10





Date: 2023-10-17

Add, No.52 HorYoutHel Road, Haidam District, Berjing, 190171, China Tel: 486-10-62302117

Formail: emf(a)entet ac en http://www.ordet.ac.co.

### DASY5 Validation Report for Head TSL

Test Laboratory: CTTL, Beijing, China

DUT: Dipole 5GHz; Type: D5GHzV2; Serial: D5GHzV2 - SN: 1079

Communication System: CW; Frequency: 5200 MHz, Frequency: 5300 MHz,

Frequency: 5500 MHz, Frequency: 5600 MHz, Frequency: 5800 MHz

Medium parameters used: f = 5200 MHz;  $\sigma = 4.67 \text{ S/m}$ ;  $\epsilon_r = 36.33$ ;  $\rho = 1000 \text{ kg/m}^3$ 

Medium parameters used: f = 5300 MHz;  $\sigma = 4.785 \text{ S/m}$ ;  $\epsilon_f = 36.13$ ;  $\rho = 1000 \text{ kg/m}^3$ 

Medium parameters used: f = 5500 MHz; a = 4.996 S/m; E = 35.76; p = 1000 kg/m

Medium parameters used: f = 5600 MHz; a = 5.11 S/m;  $\epsilon_f = 35.61$ ;  $\rho = 1000 \text{ kg/m}^3$ 

Medium parameters used: f = 5800 MHz, a = 5.308 S/m,  $\epsilon_f = 35.34$ ;  $\rho = 1000 \text{ kg/m}^3$ 

Phantom section: Right Section

Measurement Standard: DASY5 (IEEE/IEC/ANSI C63 19-2007)

DASY5 Configuration:

- Probe: EX3DV4 SN3617; ConvF(5.5, 5.5, 5.5) @ 5200 MHz; ConvF(5.5, 5.5, 5.5) @ 5300 MHz; ConvF(5.01, 5.01, 5.01) @ 5500 MHz; ConvF(5.01, 5.01, 5.01) @ 5800 MHz; ConvF(5.01, 5.01, 5.01) @ 5800 MHz; Calibrated: 2023-03-31
- Sensor-Surface: 1.4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn1556; Calibrated: 2023-01-11
- Phantom: MFP\_V5.1C (20deg probe tilt): Type: QD 000 P51 Cx; Serial: 1062
- DASY52 52.10.4(1535); SEMCAD X 14.6.14(7501)

Dipole Calibration /Pin=100mW, d=10mm, f=5200 MHz/Zoom Scan,

dist=1.4mm (8x8x7)/Cube 0: Measurement grid. dx=4mm, dy=4mm, dz=1.4mm

Reference Value = 57.18 V/m; Power Drift = -0.08 dB

Peak SAR (extrapolated) = 31.6 W/kg

SAR(1 g) = 7.83 W/kg; SAR(10 g) = 2.2 W/kg

Smallest distance from peaks to all points 3 dB below = 7.2 mm

Ratio of SAR at M2 to SAR at M1 = 65.3%

Maximum value of SAR (measured) = 18.5 W/kg

Dipole Calibration /Pin=100mW, d=10mm, f=5300 MHz/Zoom Scan,

dist=1.4mm (8x8x7)/Cube 0: Measurement grid: dx=4mm, dy=4mm, dz=1.4mm

Reference Value = 57.14 V/m; Power Drift = -0.06 dB

Peak SAR (extrapolated) = 33.1 W/kg


SAR(1 g) = 7.96 W/kg; SAR(10 g) = 2.25 W/kg


Smallest distance from peaks to all points 3 dB below = 7.2 mm

Ratio of SAR at M2 to SAR at M1 = 64.4%

Maximum value of SAR (measured) = 19.1 W/kg

Certificate No. 23J02Z80090 Page x of 10





Tel: -86-10-62302117

E-mail: emf@cnict.sc.cn

http://www.caict.ac.cn

Dipole Calibration /Pin=100mW, d=10mm, f=5500 MHz/Zoom Scan,

dist=1.4mm (8x8x7)/Cube 0: Measurement grid: dx=4mm, dy=4mm, dz=1.4mm

Reference Value = 58.01 V/m; Power Drift = -0.06 dB

Peak SAR (extrapolated) = 36.1 W/kg

SAR(1 g) = 8.27 W/kg; SAR(10 g) = 2.31 W/kg

Smallest distance from peaks to all points 3 dB below = 7.4 mm

Ratio of SAR at M2 to SAR at M1 = 62.9%

Maximum value of SAR (measured) = 20.0 W/kg

Dipole Calibration /Pin=100mW, d=10mm, f=5600 MHz/Zoom Scan,

dist=1.4mm (8x8x7)/Cube 0: Measurement grid: dx=4mm, dy=4mm, dz=1.4mm

Reference Value = 56.92 V/m; Power Drift = -0.03 dB

Peak SAR (extrapolated) = 36.4 W/kg

SAR(1 g) = 8.13 W/kg; SAR(10 g) = 2.29 W/kg

Smallest distance from peaks to all points 3 dB below = 7.2 mm

Ratio of SAR at M2 to SAR at M1 = 62%

Maximum value of SAR (measured) = 19.8 W/kg

Dipole Calibration /Pin=100mW, d=10mm, f=5800 MHz/Zoom Scan,

dist=1.4mm (8x8x7)/Cube 0: Measurement grid: dx=4mm, dy=4mm, dz=1.4mm

Reference Value = 55.83 V/m; Power Drift = -0.04 dB


Peak SAR (extrapolated) = 37.1 W/kg

SAR(1 g) = 7.88 W/kg; SAR(10 g) = 2.2 W/kg

Smallest distance from peaks to all points 3 dB below = 7.4 mm

Ratio of SAR at M2 to SAR at M1 = 60.6%

Maximum value of SAR (measured) = 19.6 W/kg

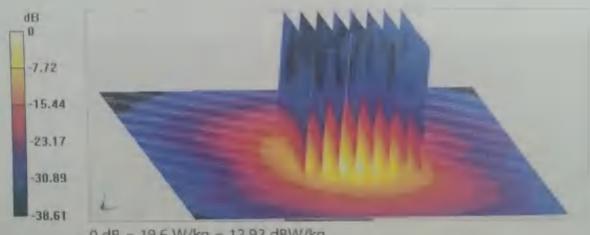

0 dB = 19.6 W/kg = 12.92 dBW/kg

Page 9 of 10 Certificate No: 23J02Z80090




Tel +86-10-62302117

E-mail: emil@carct.ac.cn

http://www.caict.no.co

### Impedance Measurement Plot for Head TSL

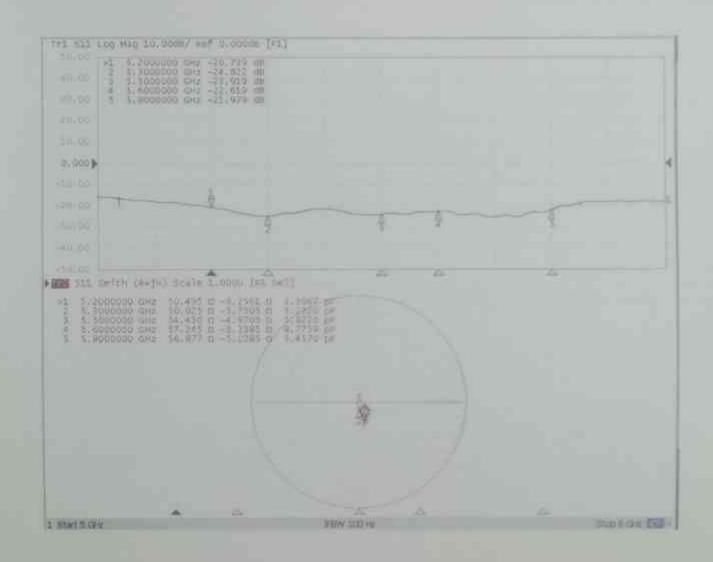

### Calibration Laboratory of Schmid & Partner Engineering AG Zeughausstrasse 43, 8004 Zurich, Switzerland





Schweizerischer Kalibrierdienst Service suisse d'étalonnage Servizio svizzero di taratura Swiss Calibration Service

Accreditation No.: SCS 0108

Accredited by the Swiss Accreditation Service (SAS)

The Swiss Accreditation Service is one of the signatories to the EA

Multilateral Agreement for the recognition of calibration certificates

Client

SRTC (Auden)

Certificate No: D6.5GHzV2-1055\_Nov22

### CALIBRATION CERTIFICATE

Object

D6.5GHzV2 - SN:1055

Calibration procedure(s)

QA CAL-22.v6

Calibration Procedure for SAR Validation Sources between 3-10 GHz

Califoration date:

November 29, 2022

This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (Si). The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility; environment temperature (22 ± 3)°C and humidity < 70%.

Calibration Equipment used (M&TE critical for calibration)

Primary Standards	ID #	Cal Date (Certificate No.)	Scheduled Calibration
Power meter NRP	SN: 104776	09-Apr-21 (No. 217-03291/03292)	Apr-22
Power sensor NRP-Z91	SN: 103244	09-Apr-21 (No. 217-03291)	Apr-22
Power sensor NRP-Z91	SN: 103245	09-Apr-21 (No. 217-03292)	Apr-2-3
Power sensor R&S NRP33T	SN: 100967	08-Apr-21 (No. 217-03290)	Apa della
Reference 20 dB Altenuator	SN: BH9394 (20k)	09-Apr-21 (No. 217-03343)	Acristi
Type-N mismatch combination	SN: 310962 / 06327	09-Apr-21 (No. 217-03544)	Acc. 22
Reference Probe EX3DV4	SN: 7405	30-Dec-20 (No. EX3-7405_Dec-20)	D 21
DAE4	SN: 908	24-Jun-21 (No. DAE4-509 Jun-31)	June
Secondary Standards	ID#	Check Date (in hours)	- I will yield
RF generator Anapico APSIN20G	SN: 609	28-Mar-17 (in house check land-18)	bridge them Par El-
Network Analyzer Fl&S ZVL13	SN: 101093	10-May-12 (in finuse chiesi Dec-19)	brown down Trees

Calibrated by:

Name Leif Klysner Function Laboratory Technician

Approved by:

Niels Kuster

Quality Manager

Issued November 29, 2022

Signifiance

This calibration certificate shall not be reproduced except in full without written approval of the laboratory.

### Calibration Laboratory of

Schmid & Partner
Engineering AG
Zoughausstrasse 43, 5004 Zurich, Switzerland





S Schweizerischer Kallbrierdienst
C Service sulsse d'étalonnage
Servizio svizzero di tereture
S Swiss Dalibration Service

Accreditation No.: SCS 0108

Accordance by the Swiss Accordance Service (SAS)

The Swiss Accordination Service is one of the signatories to the EA

Multilateral Agreement for the recognition of calibration certificates

Glossary:

TSL

N/A

tissue simulating liquid

ConvF

sensitivity in TSL / NORM x,y,z not applicable or not measured

Calibration is Performed According to the Following Standards:

a) IEC/IEEE 62209-1528, "Measurement Procedure For The Assessment Of Specific Absorption Rate Of Human Exposure To Radio Frequency Fields From Hand-Held And Body-Worn Wireless Communication Devices - Part 1528; Human Models, Instrumentation And Procedures (Frequency Range Of 4 MHz To 10 GHz)", October 2020.

### Additional Documentation:

b) DASY System Handbook

### Methods Applied and Interpretation of Parameters:

- Measurement Conditions: Further details are available from the Validation Report at the end of the certificate. All figures stated in the certificate are valid at the frequency indicated.
- Antenna Parameters with TSL: The dipole is mounted with the spacer to position its feed point
  exactly below the center marking of the flat phantom section, with the arms oriented parallel to the
  body axis.
- Feed Point Impedance and Return Loss: These parameters are measured with the dipole positioned under the liquid filled phantom. The impedance stated is transformed from the measurement at the SMA connector to the feed point. The Return Loss ensures low reflected power. No uncertainty required.
- SAR measured: SAR measured at the stated antenna input power.
- SAR normalized: SAR as measured, normalized to an input power of 1 W at the antenna connector.
- SAR for nominal TSL parameters: The measured TSL parameters are used to calculate the nominal SAR result.
- The absorbed power density (APD): The absorbed power density is evaluated according to Samaras T, Christ A. Kuster N, "Compliance assessment of the epithelial or absorbed power density above 6 GHz using SAR measurement systems", Bioelectromagnetics, 2021 (submitted). The additional evaluation uncertainty of 0.55 dB (rectangular distribution) is considered.

The reported uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor k=2, which for a normal distribution corresponds to a coverage probability of approximately 95%.

### **Measurement Conditions**

DASY system configuration, as far as not given on page 1.

DASY Version	DASY6	V16.0
Extrapolation	Advanced Extrapolation	
Phantom	Modular Flat Phantom	
Distance Dipole Center - TSL	5 mm	with Spacer
Zoom Scan Resolution	dx, dy = 3.4 mm, dz = 1.4 mm	Graded Ratio = 1.4 (Z direction)
Frequency	6500 MHz ± 1 MHz	

Head TSL parameters

The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Head TSL parameters	22.0 °C	34.5	6.07 mho/m
Measured Head TSL parameters	(22.0 ± 0.2) °C	34.3 ± 6 %	6.13 mho/m ± 6 %
Head TSL temperature change during test	< 0.5 °C	****	

### SAR result with Head TSL

SAR averaged over 1 cm <sup>3</sup> (1 g) of Head TSL	Condition	
SAR measured	100 mW input power	28.8 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	287 W/kg ± 24.7 % (k=2)

SAR averaged over 10 cm <sup>3</sup> (10 g) of Head TSL	condition	
SAR measured	100 mW input power	5.32 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	53.2 W/kg ± 24.4 % (k=2)

### Appendix

### Antenna Parameters with Head TSL

Impedance, transformed to feed point	51.1 Ω - 2.2 jΩ	
Return Loss	- 32.3 dB	

### APD (Absorbed Power Density)

APD averaged over 1 cm <sup>2</sup>	Condition		
APD measured	100 mW input power	287 W/m <sup>2</sup>	
APD measured	normalized to 1W	2870 W/m <sup>2</sup> ± 29.2 % (k=2)	

APD averaged over 4 cm <sup>2</sup>	condition	
APD measured	100 mW input power	130 W/m <sup>2</sup>
APD measured	normalized to 1W	1300 W/m <sup>2</sup> ± 28.9 % (k=2)

<sup>\*</sup>The reported APD values have been derived using psSAR8g.

### General Antenna Parameters and Design

After long term use with 100W radiated power, only a slight warming of the dipole near the feedpoint can be measured.

The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals. On some of the dipoles, small end caps are added to the dipole arms in order to improve matching when loaded according to the position as explained in the "Measurement Conditions" paragraph. The SAR data are not affected by this change. The overall dipole length is still according to the Standard.

No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feedpoint may be damaged.

### Additional EUT Data

Manufactured by	SPEAG	

### **DASY6 Validation Report for Head TSL**

Measurement Report for D6.5GHz-1055, UID 0 -, Channel 6500 (6500.0MHz)

Device un	nder Test	<b>Properties</b>
-----------	-----------	-------------------

Name, Manufacturer	Dimensions [mm]	IMEI	DUT Type
D6.5GHz	16.0 x 6.0 x 300.0	SN: 1055	- Ост туре

### **Exposure Conditions**

Phantom Section, TSL	Position, Test Distance [mm]	Band	Group, UID	Frequency [MHz]	Conversion Factor	TSL Cond. [S/m]	TSL Permittivity
Flat, HSL	5.00	Band	CW,	6500	5.75	6.13	34.3

### **Hardware Setup**

Phantom	TSL	Probe, Calibration Date	DAE, Calibration Date
MFP V8.0 Center - 1182	HBBL600-10000V6	EX3DV4 - SN7405, 2020-12-30	DAE4 Sn908, 2021-06-24

### Scan Setup

		micasai ciliciit ucsaits	
	Zoom Scan		Zoom Scan
Grid Extents [mm]	22.0 x 22.0 x 22.0	Date	2021-11-29, 10:54
Grid Steps [mm]	3.4 x 3.4 x 1.4	psSAR1g [W/Kg]	28.8
Sensor Surface [mm]	1.4	psSAR10g [W/Kg]	5.32
Graded Grid	Yes	Power Drift [dB]	-0.01
Grading Ratio	1.4	Power Scaling	Disabled
MAIA	N/A	Scaling Factor [dB]	
Surface Detection	VMS + 6p	TSL Correction	No correction
Scan Method	Measured	M2/M1 [%]	50.3
		Dist 3dB Peak [mm]	4.8



### Impedance Measurement Plot for Head TSL

