

## APPENDIX D: PROBE CALIBRATION

PCTESTÔ SAR REPORT	POTEST	FCC CERTIFICATION	<b>(2)</b>	Reviewed by: Quality Manager
SAR Filename: SAR.240309236.AZ4	Test Dates: March 22-24, 2004	Phone Type: Dual-Mode PTT Phone (iDEN/ISM)	FCC ID: AZ489FT5831	Page D-1 of D-22



## APPENDIX D: PROBE CALIBRATION

PCTESTÔ SAR REPORT	PCTEST	FCC CERTIFICATION	<b>©</b>	Reviewed by: Quality Manager
SAR Filename: SAR.240309236.AZ4	Test Dates: March 22-24, 2004	Phone Type: Dual-Mode PTT Phone (iDEN/ISM)	FCC ID: AZ489FT5831	Page D-1 of D-22



### Calibration Laboratory of Schmid & Partner Engineering AG Zeughausstrasse 43, 8004 Zurich, Switzerland

Client

PC Test

Object(s)	ES3DV2 - SN	3022	
Calbration procedure(s)	OA CAL-01 va Calibration pro	) icedure for dosimetric E-field prob	<b>P5</b>
Calibration date:	September 23	. 2003	
Condition of the calibrated item	In Tolerance (	according to the specific calibration	document)
17025 international standard.		used in the calibration procedures and conformity of ry facility: environment temperature 22 +/- 2 degrees	04-03-176-46-0-1-1-1-1000-174-0-1-1-1-4-0-4-1-1-1-1-1-1-1-1-1-1-1-1-
Calibration Equipment used (M&TE			o to to and initially a 1070.
Model Type	iD#	Cal Date (Calibrated by, Certificate No.)	Scheduled Calibration
CONTRACTOR DESCRIPTION OF THE PROPERTY OF THE	ID# GB41293874	Cal Date (Calibrated by, Certificate No.) 2-Apr-03 (METAS, No 252-0250)	Scheduled Calibration Apr-04
Power meter EPM E44198 Power sensor E4412A			
Power meter EPM E44198 Power sensor E4412A Reference 20 dB Attenuator	GB41293874 MY41495277 SN: 5086 (20b)	2-Apr-03 (METAS, No 252-0250)	Apr-04
Power meter EPM E44198 Power sensor E4412A Reference 20 dB Attenuator Fluke Process Calibrator Type 702	GB41293874 MY41495277 SN: 5086 (20b) SN: 6295803	2-Apr-03 (METAS, No 252-0250) 2-Apr-03 (METAS, No 252-0250) 3-Apr-03 (METAS No. 251-0340 8-Sep-03 (Sintrel SCS No. E-030020)	Apr-04 Apr-04
Power meter EPM E44198 Power sensor E4412A Reference 20 dB Attenuator Fluke Process Calibrator Type 702 Power sensor HP 8481A	GB41293874 MY41495277 SN: 5086 (20b) SN: 6295803 MY41092180	2-Apr-03 (METAS, No 252-0250) 2-Apr-03 (METAS, No 252-0250) 3-Apr-03 (METAS No. 251-0340 8-Sep-03 (Sintrel SCS No. E-030020) 18-Sep-02 (Agillorit, No. 20020918)	Apr-04 Apr-04 Apr-04 Sep-04 In house check: Oct 03
Power meter EPM E44198 Power sensor E4412A Reference 20 dB Attenuator Fluke Process Calibrator Type 702 Power sensor HP 6481A RF generator HP 8984C	GB41293874 MY41495277 SN: 5086 (20b) SN: 6295803	2-Apr-03 (METAS, No 252-0250) 2-Apr-03 (METAS, No 252-0250) 3-Apr-03 (METAS No. 251-0340 8-Sep-03 (Sintrel SCS No. E-030020)	Apr-04 Apr-04 Apr-04 Sep-04
Model Type Power meter EPM E44198 Power sensor E4412A Reference 20 dB Attenuator Fluke Process Calibrator Type 702 Power sensor HP 8481A RF generator HP 8584C Network Analyzer HP 8753E	GB41293874 MY41495277 SN: 5086 (20b) SN: 6295803 MY41092180 US3642U01700	2-Apr-03 (METAS, No 252-0250) 2-Apr-03 (METAS, No 252-0250) 3-Apr-03 (METAS No. 251-0340 8-Sep-03 (Sintrel SCS No. E-030020) 18-Sep-02 (Agilent, No. 20020918) 4-Aug-99 (SPEAG, in house check Aug-02) 18-Oct-01 (Agilent, No. 24BR1033101)	Apr-04 Apr-04 Apr-04 Sep-04 In house check: Oct 03 In house check: Aug-05 In house check: Oct 03
Power meter EPM E44198 Power sensor E4412A Reference 20 dB Attenuator Fluke Process Calibrator Type 702 Power sensor HP 6481A RF generator HP 8984C	GB41293874 MY41495277 SN: 5086 (20b) SN: 6295803 MY41092180 US3642UD1700 US37390585	2-Apr-03 (METAS, No 252-0250) 2-Apr-03 (METAS, No 252-0250) 3-Apr-03 (METAS No. 251-0340 8-Sep-03 (Sintrel SCS No. E-030020) 18-Sep-02 (Agilant, No. 20020918) 4-Aug-99 (SPEAG, in house check Aug-02)	Apr-04 Apr-04 Apr-04 Sep-04 In house check: Oct 03 In house check: Aug-05
Power meter EPM E44198 Power sensor E4412A Reference 20 dB Attenuator Fluke Process Calibrator Type 702 Power sensor HP 6481A RF generator HP 8584C Network Analyzer HP 8753E Calibrated by:	GB41293874 MY41495277 SN: 5086 (20b) SN: 6295803 MY41092180 US3642U01700 US37390585	2-Apr-03 (METAS, No 252-0250) 2-Apr-03 (METAS, No 252-0250) 3-Apr-03 (METAS No. 251-0340 8-Sep-03 (Sintrel SCS No. E-030020) 18-Sep-02 (Agilent, No. 20020918) 4-Aug-99 (SPEAG, in house check Aug-02) 18-Oct-01 (Agilent, No. 24BR1033101) Function	Apr-04 Apr-04 Apr-04 Sep-04 In house check: Oct 03 In house check: Aug-05 In house check: Oct 03
Power meter EPM E44198 Power sensor E4412A Reference 20 dB Attenuator Fluke Process Calibrator Type 702 Power sensor HP 6481A RF generator HP 8584C Network Analyzer HP 8753E	GB41293874 MY41495277 SN: 5086 (20b) SN: 6295803 MY41092180 US3642U01700 US37390585 Name	2-Apr-03 (METAS, No 252-0250) 2-Apr-03 (METAS, No 252-0250) 3-Apr-03 (METAS No. 251-0340 8-Sep-03 (Sintrel SCS No. E-030020) 18-Sep-02 (Agilent, No. 20020918) 4-Aug-99 (SPEAG, in house check Aug-02) 18-Oct-01 (Agilent, No. 24BR1033101)  Function Laboratory Director	Apr-04 Apr-04 Apr-04 Sep-04 In house check: Oct 03 In house check: Aug-05 In house check: Oct 03
Power meter EPM E44198 Power sensor E4412A Reference 20 dB Attenuator Fluke Process Calibrator Type 702 Power sensor HP 6481A RF generator HP 8584C Network Analyzer HP 8753E Calibrated by:	GB41293874 MY41495277 SN: 5086 (20b) SN: 6295803 MY41092180 US3642U01700 US37390585 Name	2-Apr-03 (METAS, No 252-0250) 2-Apr-03 (METAS, No 252-0250) 3-Apr-03 (METAS No. 251-0340 8-Sep-03 (Sintrel SCS No. E-030020) 18-Sep-02 (Agilent, No. 20020918) 4-Aug-99 (SPEAG, in house check Aug-02) 18-Oct-01 (Agilent, No. 24BR1033101)  Function Laboratory Director	Apr-04 Apr-04 Apr-04 Sep-04 In house check: Oct 03 In house check: Aug-05 In house check: Oct 03

PCTESTÔ SAR REPORT	APCTEST	FCC CERTIFICATION	<b>©</b>	Reviewed by: Quality Manager
SAR Filename: SAR.240309236.AZ4	Test Dates: March 22-24, 2004	Phone Type: Dual-Mode PTT Phone (iDEN/ISM)	FCC ID: AZ489FT5831	Page D-2 of D-22



s p e a g

Zeughausstrasse 43, 8004 Zurich, Switzerland Phone +41 1 245 9700, Fax +41 1 245 9779 info@speag.com, http://www.speag.com

# Probe ES3DV2

SN:3022

Manufactured: Last calibration:

April 15, 2003

September 23, 2003

Calibrated for DASY Systems

(Note: non-compatible with DASY2 system!)

PCTESTÔ SAR REPORT	POTERT	FCC CERTIFICATION	<b>(4)</b>	Reviewed by: Quality Manager
SAR Filename:	Test Dates:	Phone Type:	FCC ID:	Page D-3 of D-22
SAR.240309236.AZ4	March 22-24, 2004	Dual-Mode PTT Phone (iDEN/ISM)	AZ489FT5831	1 age D-3 of D-22



ES3DV2 SN:3022 September 23, 2003

## DASY - Parameters of Probe: ES3DV2 SN:3022

### Sensitivity in Free Space

### Diode Compression

NormX	1.00 μV/(V/m) <sup>2</sup>	DCP X	95	mV
NormY	1.04 $\mu V/(V/m)^2$	DCP Y	95	mV
NormZ	0.98 μV/(V/m) <sup>2</sup>	DCP Z	95	mV

## Sensitivity in Tissue Simulating Liquid

Head	900 MHz	$\epsilon_r = 41.5 \pm 5\%$	$\sigma = 0.97 \pm 5\% \text{ mho/m}$
Valid for f=800-100	00 MHz with Head	Tissue Simulating Liquid	according to EN 50361, P1528-200X

ConvF X	6.1 ± 9.5% (k=2)	Boundary	effect:
ConvF Y	6.1 ± 9.5% (k=2)	Alpha	0.32
ConvF Z	6.1 ± 9.5% (k=2)	Depth	1.65

Head	1800 MHz	$\varepsilon_{\rm r}$ = 40.0 ± 5%	a = 1.40 ± 5% mho/m
Valid for f=17	710-1910 MHz with Head T	issue Simulating Liquid ac	cording to EN 50361, P1528-200X

ConvF X	5.0 ± 9.5% (k=2)	Boundary	effect:
ConvF Y	5.0 ± 9.5% (k=2)	Alpha	0.25
ConvF Z	5.0 ± 9.5% (k=2)	Depth	2.30

## **Boundary Effect**

Head	900 MHz	Typical SAR gradient: 5 % per mm

Probe Tip to Boundary		1 mm	2 mm
SAR <sub>be</sub> [%]	Without Correction Algorithm	5.5	2.5
SAR <sub>be</sub> [%]	With Correction Algorithm	0.1	0.4


### Head 1800 MHz Typical SAR gradient: 10 % per mm

Probe Tip t	Probe Tip to Boundary  SAR <sub>be</sub> [%] Without Correction Algorithm  SAR <sub>be</sub> [%] With Correction Algorithm	1 mm	2 mm	
SAR <sub>be</sub> [%]	Without Correction Algorithm	7.1	4.4	
SAR <sub>be</sub> [%]	With Correction Algorithm	0.0	0.1	

### Sensor Offset


Probe Tip to Sensor Center 2.0 mm

PCTESTÔ SAR REPORT	PCTEST	FCC CERTIFICATION	<b>(4)</b>	Reviewed by: Quality Manager
SAR Filename:	Test Dates:	Phone Type:	FCC ID:	Page D-4 of D-22
SAR.240309236.AZ4	March 22-24, 2004	Dual-Mode PTT Phone (iDEN/ISM)	AZ489FT5831	1 age D-4 01 D-22






## Receiving Pattern ( $\phi$ , $\theta$ = 0°

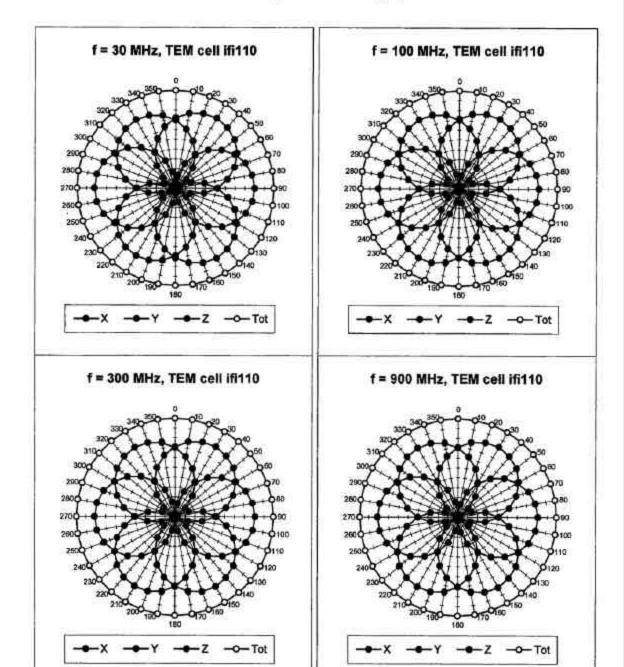


PCTESTÔ SAR REPORT	POTEST	FCC CERTIFICATION	<b>(4)</b>	Reviewed by: Quality Manager
SAR Filename:	Test Dates:	Phone Type:	FCC ID:	Page D-5 of D-22
SAR.240309236.AZ4	March 22-24, 2004	Dual-Mode PTT Phone (iDEN/ISM)	AZ489FT5831	Page D-5 of D-22




### September 23, 2003

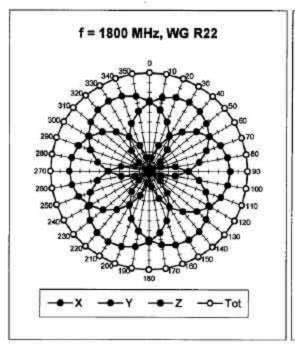

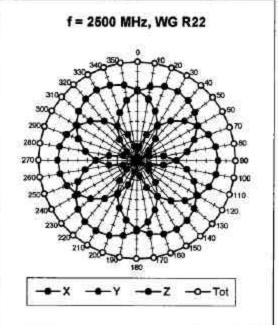

## Isotropy Error ( $\phi$ ), $\theta$ = 0°

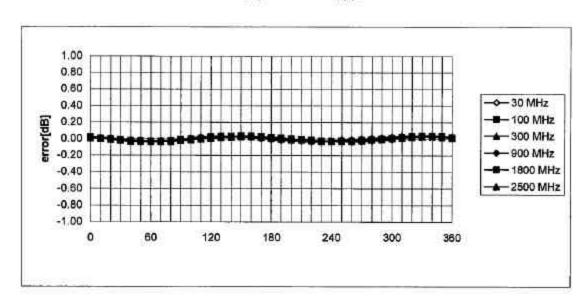


PCTESTÔ SAR REPORT	-V-CTEBT	FCC CERTIFICATION	<b>&amp;</b>	Reviewed by: Quality Manager
SAR Filename:	Test Dates:	Phone Type:	FCC ID:	Page D-6 of D-22
SAR.240309236.AZ4	March 22-24, 2004	Dual-Mode PTT Phone (iDEN/ISM)	AZ489FT5831	1 age D-0 01 D-22



## Frequency Response of E-Field


(TEM-Cell:ifi110, Waveguide R22)

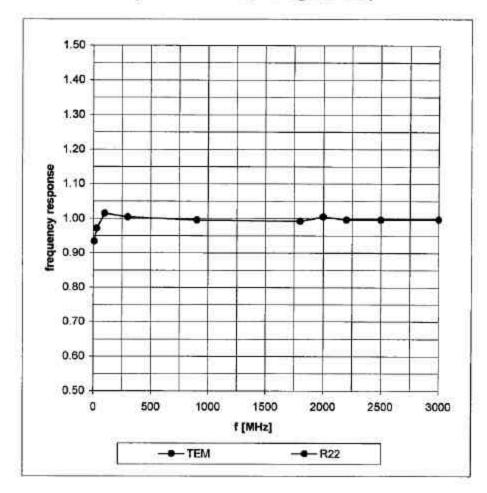


PCTESTÔ SAR REPORT	POTEST	FCC CERTIFICATION	<b>(3)</b>	Reviewed by: Quality Manager
SAR Filename:	Test Dates:	Phone Type:	FCC ID:	Page D-7 of D-22
SAR.240309236.AZ4	March 22-24, 2004	Dual-Mode PTT Phone (iDEN/ISM)	AZ489FT5831	1 age D-7 of D-22



## **Conversion Factor Assessment**

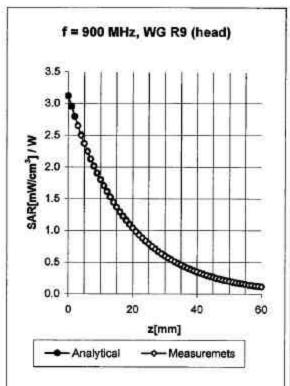

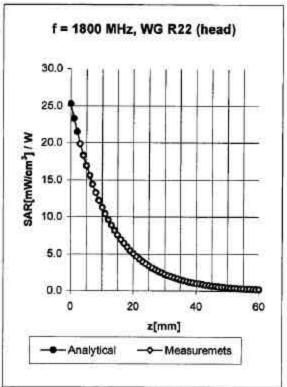

Head 900 MHz  $\epsilon_r = 41.5 \pm 5\%$   $\sigma = 0.97 \pm 5\%$  mho/m

Valid for f=800-1000 MHz with Head Tissue Simulating Liquid according to EN 50361, P1528-200X

ConvF X 6.1 ± 9.5% (k=2) Boundary effect:

ConvF Y 6.1 ± 9.5% (k=2) Alpha 0.32

ConvF Z 6.1 ± 9.5% (k=2) Depth 1.65

Head 1800 MHz  $\epsilon_r = 40.0 \pm 5\%$   $\sigma = 1.40 \pm 5\%$  mho/m

Valid for f=1710-1910 MHz with Head Tissue Simulating Liquid according to EN 50361, P1528-200X

ConvF X 5.0 ± 9.5% (k=2) Boundary effect:

ConvF Y 5.0 ± 9.5% (k=2) Alpha 0.25


ConvF Z 5.0 ± 9.5% (k=2) Depth 2.30


PCTESTÔ SAR REPORT	PCTEST	FCC CERTIFICATION	<b>©</b>	Reviewed by: Quality Manager
SAR Filename: SAR.240309236.AZ4	<b>Test Dates:</b> March 22-24, 2004	Phone Type: Dual-Mode PTT Phone (iDEN/ISM)	FCC ID: AZ489FT5831	Page D-8 of D-22



## Dynamic Range f(SAR<sub>brain</sub>)

(Waveguide R22)

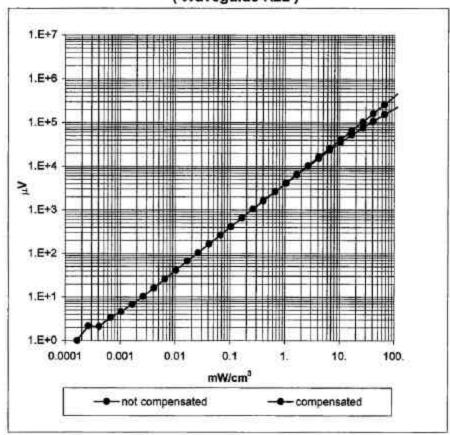


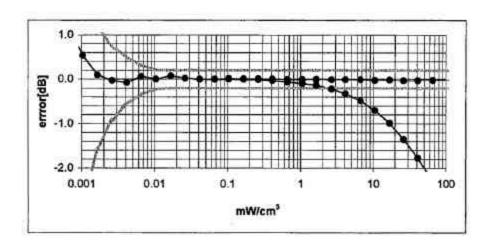


PCTESTÔ SAR REPORT	-V-CTEBT	FCC CERTIFICATION	<b>&amp;</b>	Reviewed by: Quality Manager
SAR Filename:	Test Dates:	Phone Type:	FCC ID:	Page D-9 of D-22
SAR.240309236.AZ4	March 22-24, 2004	Dual-Mode PTT Phone (iDEN/ISM)	AZ489FT5831	1 age D-7 01 D-22



## **Conversion Factor Assessment**

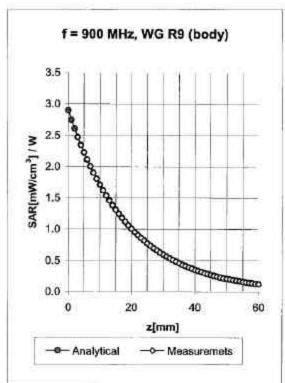

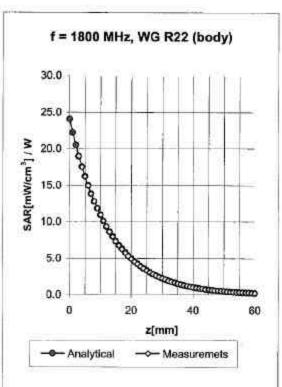

Body 900 MHz

Er = 55.0 ± 5%

 $\sigma = 1.05 \pm 5\% \, \text{mho/m}$ 

Valid for f=800-1000 MHz with Body Tissue Simulating Liquid according to OET 65 Suppl. C

ConvF X

6.0 ± 9.5% (k=2)

Boundary effect:

ConvF Y

6.0 ± 9.5% (k=2)

Alpha

0.38

ConvF Z

6.0 ± 9.5% (k=2)

Depth

1.47

Body

1800 MHz

E. = 53.3 ± 5%

 $\sigma = 1.52 \pm 5\% \text{ mho/m}$ 

Valid for f=1710-1910 MHz with Body Tissue Simulating Liquid according to OET 65 Suppl. C

ConvF X

4.5 ± 9.5% (k=2)

Boundary effect:

ConvF Y

4.5 ± 9.5% (k=2)

Alpha

0.22

ConvF Z

4.5 ± 9.5% (k=2)


Depth


3.42

PCTESTÔ SAR REPORT	POTEST	FCC CERTIFICATION	<b>©</b>	Reviewed by: Quality Manager
SAR Filename: SAR.240309236.AZ4	<b>Test Dates:</b> March 22-24, 2004	Phone Type: Dual-Mode PTT Phone (iDEN/ISM)	FCC ID: AZ489FT5831	Page D-10 of D-22



## **Conversion Factor Assessment**

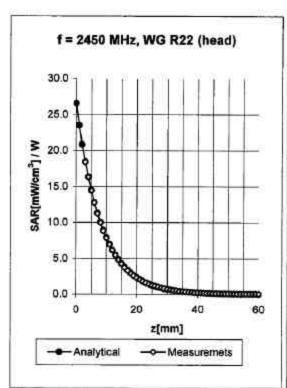

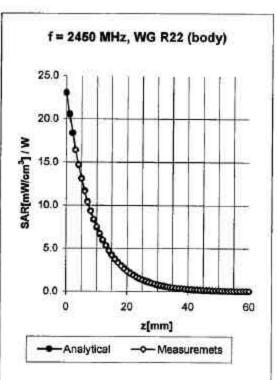

Head 2450 MHz

Er = 39.2 ± 5%

σ = 1.80 ± 5% mho/m

Valid for f=2400-2500 MHz with Head Tissue Simulating Liquid according to EN 50361, P1528-200X

ConvF X 4.5 ± 9.5% (k=2)

Boundary effect:

ConvF Y

4.5 ± 9.5% (k=2)

Alpha

ConvF Z

4.5 ± 9.5% (k=2)

Depth 1.56

Body

2450 MHz

Er = 52.7 ± 5%

σ = 1.95 ± 5% mho/m

Valid for f=2400-2500 MHz with Body Tissue Simulating Liquid according to OET 65 Suppl. C

ConvF X

4.2 ± 9.5% (k=2)

Boundary effect:

ConvF Y

4.2 ± 9.5% (k=2)

Alpha

ConvF Z

4.2 ± 9.5% (k=2)

Depth


1.65


0.42

PCTESTÔ SAR REPORT	POTEST	FCC CERTIFICATION	<b>©</b>	Reviewed by: Quality Manager
SAR Filename:	<b>Test Dates:</b>	Phone Type:	FCC ID:	Page D-11 of D-22
SAR.240309236.AZ4	March 22-24, 2004	Dual-Mode PTT Phone (iDEN/ISM)	AZ489FT5831	



### Conversion Factor Assessment

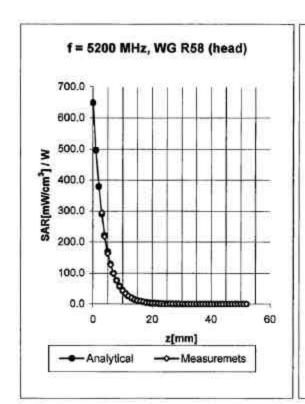

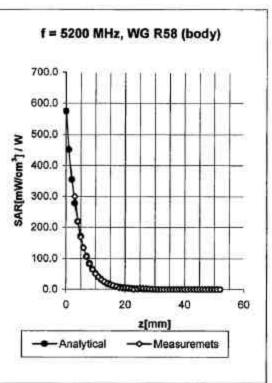

Head 5200 MHz

 $\varepsilon_r = 36.0 \pm 5\%$ 

 $\sigma = 4.66 \pm 5\% \text{ mho/m}$ 

Valid for f=4940-5460 MHz with Head Tissue Simulating Liquid according to OET65-SuppC

ConvF X 2.60 ± 16.6% (k=2)

Boundary effect:

ConvF Y 2.60 ± 16.6% (k=2)

Alpha 0.93

ConvF Z 2.60 ± 16.6% (k=2)

Depth 1.50

Body

5200 MHz

ε, = 49.0 ± 5%

 $\sigma = 5.30 \pm 5\% \text{ mho/m}$ 

Valid for f=4940-5460 MHz with Body Tissue Simulating Liquid according to OET65-SuppC

ConvF X

1.80 ± 16.6% (k=2)

Boundary effect:

ConvF Y

1.80 ± 16.6% (k=2)

Alpha

1.05

ConvF Z

1.80 ± 16.6% (k=2)


Depth


1.60

PCTESTÔ SAR REPORT	PCTEST	FCC CERTIFICATION	<b>©</b>	Reviewed by: Quality Manager
SAR Filename:	<b>Test Dates:</b>	Phone Type:	FCC ID:	Page D-12 of D-22
SAR.240309236.AZ4	March 22-24, 2004	Dual-Mode PTT Phone (iDEN/ISM)	AZ489FT5831	



## **Conversion Factor Assessment**

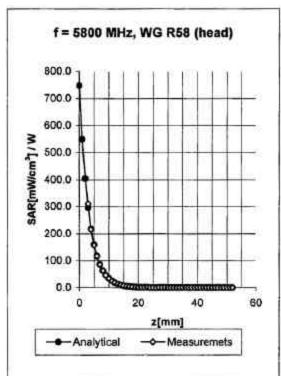

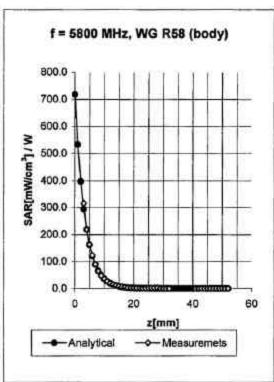

Head 5800 MHz  $\epsilon_r = 35.3 \pm 5\%$   $\sigma = 5.27 \pm 5\%$  mho/m

Valid for f=5510-6090 MHz with Head Tissue Simulating Liquid according to OET65-SuppC

ConvF X 2.15 ± 16.6% (k=2) Boundary effect:

ConvF Y 2.15 ± 16.6% (k=2) Alpha 1.04

ConvF Z 2.15 ± 16.6% (k=2) Depth 1.50


Valid for f=5510-6090 MHz with Body Tissue Simulating Liquid according to OET65-SuppC

ConvF X 1.57 ± 16.6% (k=2) Boundary effect:

ConvF Y 1.57 ± 16.6% (k=2) Alpha 1.15

ConvF Z 1.57 ± 16.6% (k=2) Depth 1.70


PCTESTÔ SAR REPORT	POTEST	FCC CERTIFICATION	<b>©</b>	Reviewed by: Quality Manager
SAR Filename:	Test Dates:	Phone Type:	FCC ID:	Page D-13 of D-22
SAR.240309236.AZ4	March 22-24, 2004	Dual-Mode PTT Phone (iDEN/ISM)	AZ489FT5831	1 age D-13 01 D-22





## Deviation from Isotropy in HSL

Error (θφ ), f = 900 MHz

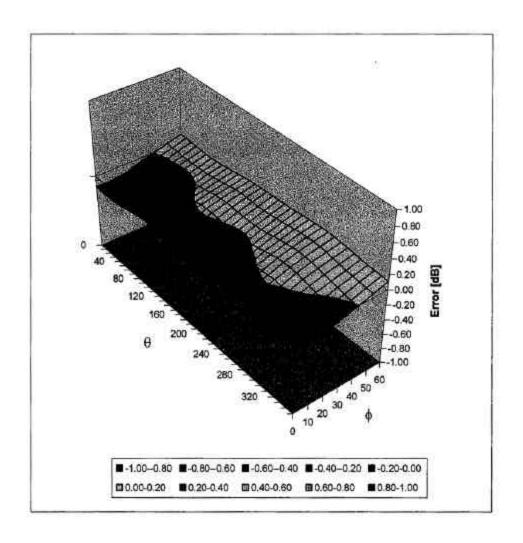

PCTESTÔ SAR REPORT	POTEST	FCC CERTIFICATION	<b>&amp;</b>	Reviewed by: Quality Manager
SAR Filename:	Test Dates:	Phone Type:	FCC ID:	Page D-14 of D-22
SAR.240309236.AZ4	March 22-24, 2004	Dual-Mode PTT Phone (iDEN/ISM)	AZ489FT5831	1 age D-14 01 D-22

s p e a g

Zeughausstrasse 43, 8004 Zurich, Switzerland Phone +41 1 245 9700, Fax +41 1 245 9779 info@speag.com, http://www.speag.com


### **Additional Conversion Factors**

for Dosimetric E-Field Probe

Type:	ES3DV2
Serial Number:	3022
Place of Assessment:	Zurich
Date of Assessment:	December 3, 2003
Probe Calibration Date:	September 23, 2003

Schmid & Partner Engineering AG hereby certifies that conversion factor(s) of this probe have been evaluated on the date indicated above. The assessment was performed using the FDTD numerical code SEMCAD of Schmid & Partner Engineering AG. Since the evaluation is coupled with measured conversion factors, it has to be recalculated yearly, i.e., following the re-calibration schedule of the probe. The uncertainty of the numerical assessment is based on the extrapolation from measured value at 900 MHz or at 1800 MHz.

Assessed by:



PCTESTÔ SAR REPORT	PCTEST	FCC CERTIFICATION	<b>(4)</b>	Reviewed by: Quality Manager
SAR Filename:	Test Dates:	Phone Type:	FCC ID:	Page D-15 of D-22
SAR.240309236.AZ4	March 22-24, 2004	Dual-Mode PTT Phone (iDEN/ISM)	AZ489FT5831	1 age D-13 01 D-22



## Dosimetric E-Field Probe ES3DV2 SN:3022

Conversion factor (± standard deviation)

1950 MHz	ConvF	$4.7 \pm 9.5\%$	$\Box = 40.0 \pm 5\%$ $\Box = 1.40 \pm 5\%$ mho/m (head tissue)
1950 MHz	ConvF	4. 3± 9.5%	$\Box = 53.3 \pm 5\%$ $\Box = 1.52 \pm 5\%$ mho/m (body tissue)

PCTESTÔ SAR REPORT	PCTERT	FCC CERTIFICATION	<b>©</b>	Reviewed by: Quality Manager
SAR Filename:	Test Dates:	Phone Type:	FCC ID:	Page D-16 of D-22
SAR.240309236.AZ4	March 22-24, 2004	Dual-Mode PTT Phone (iDEN/ISM)	AZ489FT5831	1 age D-10 01 D-22



speag

Zeughausstrasse 43, 8004 Zurich, Switzerland Phone +41 1 245 9700, Fax +41 1 245 9779 info@speag.com, http://www.speag.com

## **Additional Conversion Factors**

for Dosimetric E-Field Probe

Type: ES3DV2

Serial Number: 3022

Place of Assessment: Zurich

Date of Assessment: October 3, 2003

Probe Calibration Date: September 23, 2003

Schmid & Partner Engineering AG hereby certifies that conversion factor(s) of this probe have been evaluated on the date indicated above. The assessment was performed using the FDTD numerical code SEMCAD of Schmid & Partner Engineering AG. Since the evaluation is coupled with measured conversion factors, it has to be recalculated yearly, i.e., following the re-calibration schedule of the probe. The uncertainty of the numerical assessment is based on the extrapolation from measured value at 900 MHz or at 1800 MHz.

Assessed by:

Total S	-	200	w		85
2122	1	× .	Mos	64	H.H
1	AL.	اع مراط	and,	,	800
0	TOTAL STREET	SE HELL			2574

PCTESTÔ SAR REPORT	POTEST	FCC CERTIFICATION	<b>&amp;</b>	Reviewed by: Quality Manager
SAR Filename:	Test Dates:	Phone Type:	FCC ID:	Page D-17 of D-22
SAR.240309236.AZ4	March 22-24, 2004	Dual-Mode PTT Phone (iDEN/ISM)	AZ489FT5831	1 age D-17 01 D-22



Zeughausstrasse 43, 8004 Zurich, Switzerland Phone +41 1 245 9700, Fax +41 1 245 9779 info@speag.com, http://www.speag.com

## Dosimetric E-Field Probe ES3DV2 SN:3022

Conversion factor (± standard deviation)

150 MHz	ConvF	8.5 ± 8%	$\epsilon_r = 52.3 \pm 5\%$ $\sigma = 0.76 \pm 5\% \text{ mho/m}$ (head tissue)
150 MHz	ConvF	8.0 ± 8%	$\epsilon_r = 61.9 \pm 5\%$ $\sigma = 0.80 \pm 5\%$ mho/m (body tissue)
450 MHz	ConvF	$7.1\pm8\%$	$\epsilon_r = 43.5 \pm 5\%$ $\sigma = 0.87 \pm 5\% \text{ mho/m}$ (head tissue)
450 MHz	ConvF	7.2 ± 8%	$\epsilon_r = 56.7 \pm 5\%$ $\sigma = 0.94 \pm 5\% \text{ mho/m}$ (body tissue)

PCTESTÔ SAR REPORT	POTEST	FCC CERTIFICATION	<b>©</b>	Reviewed by: Quality Manager
SAR Filename:	Test Dates:	Phone Type:	FCC ID:	Page D-18 of D-22
SAR.240309236.AZ4	March 22-24, 2004	Dual-Mode PTT Phone (iDEN/ISM)	AZ489FT5831	1 age D-10 01 D-22



s p e a g

Zeughausstrasse 43, 8004 Zurich, Switzerland Phone +41 1 245 9700, Fax +41 1 245 9779 info@speag.com, http://www.speag.com

## **Additional Conversion Factors**

for Dosimetric E-Field Probe

Type:	ES3DV2
Serial Number:	3022
Place of Assessment:	Zurich
Date of Assessment:	November 28, 2003
Probe Calibration Date:	September 23, 2003

Schmid & Partner Engineering AG hereby certifies that conversion factor(s) of this probe have been evaluated on the date indicated above. The assessment was performed using the FDTD numerical code SEMCAD of Schmid & Partner Engineering AG. Since the evaluation is coupled with measured conversion factors, it has to be recalculated yearly, i.e., following the re-calibration schedule of the probe. The uncertainty of the numerical assessment is based on the extrapolation from measured value at 900 MHz or at 1800 MHz.

Assessed by:

	17.2 21.1
	Martin
d by:	
u by.	

PCTESTÔ SAR REPORT	POTEST	FCC CERTIFICATION	<b>©</b>	Reviewed by: Quality Manager
SAR Filename: SAR.240309236.AZ4	Test Dates: March 22-24, 2004	Phone Type: Dual-Mode PTT Phone (iDEN/ISM)	FCC ID: AZ489FT5831	Page D-19 of D-22



### Dosimetric E-Field Probe ES3DV2 SN:3022

Conversion factor (± standard deviation)

1600 MHz ConvF  $5.2 \pm 8\%$   $\Box = 40.3 \pm 5\%$   $\Box = 1.29 \pm 5\%$  mho/m (head tissue)

 $\Box = 1.40 \pm 5\% \text{ mho/m}$ (body tissue)

PCTESTÔ SAR REPORT	ACTEST	FCC CERTIFICATION	<b>&amp;</b>	Reviewed by: Quality Manager
SAR Filename:	Test Dates:	Phone Type:	FCC ID:	Page D-20 of D-22
SAR.240309236.AZ4	March 22-24, 2004	Dual-Mode PTT Phone (iDEN/ISM)	AZ489FT5831	1 age D-20 01 D-22



s p e a g

Zeughausstrasse 43, 8004 Zurich, Switzerland Phone +41 1 245 9700, Fax +41 1 245 9779 info@speag.com, http://www.speag.com

## **Additional Conversion Factors**

for Dosimetric E-Field Probe

Type:	ES3DV2	
Serial Number:	3022	
Place of Assessment:	Zurich	
Date of Assessment:	December 9, 2003	
Probe Calibration Date:	September 23, 2003	

Schmid & Partner Engineering AG hereby certifies that conversion factor(s) of this probe have been evaluated on the date indicated above. The assessment was performed using the FDTD numerical code SEMCAD of Schmid & Partner Engineering AG. Since the evaluation is coupled with measured conversion factors, it has to be recalculated yearly, i.e., following the re-calibration schedule of the probe. The uncertainty of the numerical assessment is based on the extrapolation from measured value at 900 MHz or at 1800 MHz.

Assessed by:



PCTESTÔ SAR REPORT	POTEST	FCC CERTIFICATION		Reviewed by: Quality Manager
SAR Filename: SAR.240309236.AZ4	<b>Test Dates:</b> March 22-24, 2004	Phone Type: Dual-Mode PTT Phone (iDEN/ISM)	FCC ID: AZ489FT5831	Page D-21 of D-22



## Dosimetric E-Field Probe ES3DV2 SN:3022

Conversion factor (± standard deviation)

2140 MHz ConvF 4.5 ± 8%

= 39.8 ± 5% = 1.49 ± 5% mho/m (brain tissue)

PCTESTÔ SAR REPORT	ACTEST	FCC CERTIFICATION	<b>©</b>	Reviewed by: Quality Manager
SAR Filename:	Test Dates:	Phone Type:	FCC ID:	Page D-22 of D-22
SAR.240309236.AZ4	March 22-24, 2004	Dual-Mode PTT Phone (iDEN/ISM)	AZ489FT5831	1 age D-22 01 D-22