

Exhibit 7. Measurement Procedures -- 47 CFR. 2.947

7.1 RF Power – Pursuant to 47 CFR 2.947(c)

Method of Conducted Output Power Measurement: Adaptation of TIA/EIA-603-B clause 2.2.1 for Pulsed Measurements

The RF output power is not adjustable by the user. The output power is controlled by the radio in response to the received signal strength or by or special radio service software. To obtain RF output power reading, the radio was programmed to utilize the maximum and minimum output power setting. To correct the average reading power meter, a setting of the duty cycle on the RF power meter was set to 16.667% for herein reported 6:1 TDM test signals.

A special DC/RF test fixture was utilized to interface with the radio test RF connector while simultaneously supplying the nominal operating voltage of 4.0V. The radio RF connector is utilized in all factory tuning and testing procedures, and provides a 50 ohm connection to the transmitter path while disconnecting the radio antenna. All conducted measurements were performed via this test port.

NOTE: This DC/RF test fixture is not offered for sale.

Method of Measurement for Effective Radiated Power: TIA/EIA-603-B 2.2.17.2

The ERP characteristic was measured while a radio was set to transmit a test mode CW signal at the maximum rated output power (+/- 5%) and was vertically mounted on a non-conducting platform/turtable in a RF Anechoic Chamber. The power received at an antenna located at the end of the chamber was recorded on a spectrum analyzer for a complete 360-degree rotation. The same procedure was repeated for 800 and 900 MHz sleeve reference dipole. The CW RF output power of the radio product was measured by a conducted means to determine the necessary input power for the reference dipole (after compensation for interface, cable, and antenna losses). The maximum power levels measured were compared to determine the antenna gain of the radio antenna in reference to the standard dipole. This relative antenna gain was used to scale the maximum RF conducted output power and determine the maximum herein reported ERP.

7.2 Emission Mask-- Pursuant to 47 CFR 2.947(b)

Method of Measurement: Per TIA/EIA-603-B clause 2.2.11

- (1) Set the radio for measurement of RF output power using the power test procedure in the service manual which employs a pseudo random data sequence per part 2.1049(h), and attach it to a spectrum analyzer through a 10 dB attenuator. The analyzer is to be set for peak detection with a video bandwidth of 3 times the resolution bandwidth setting, a span of 100 kHz, and a sweep period of 20 seconds.
- (2) Using a 30 kHz resolution bandwidth to assure that essentially all of the transmitted energy is measured, obtain a "rainbow" curve and adjust the analyzer setting so that the crest of the curve lies at the 0 dB reference location. This is portrayed as trace 1 on the analyzer display.
- (3) Reduce the resolution bandwidth to 300 Hz to characterize the transmitter emission on-channel and adjacent channels spectral performance characteristic. This is portrayed as trace 2 on the analyzer display of Figures 6-7 to 6-12.
- (4) Overlay the applicable emission mask on the analyzer display as trace 3.
- (5) Compare traces 2 and 3 to ensure that trace 2 never exceeds trace 3.

7.3 Radiated Spurious Emissions -- Pursuant to 47 CFR 2.947(b)

Test Sites:

Open Area Test Site (OATS) of the Motorola EMC Lab, 8000 W. Sunrise Blvd., Plantation, Florida 33322 which is accredited to ISO/IEC 25 from the American Association for Laboratory Accreditation (FCC Registration: 91932 /Industry Canada: IC3697). The radiated emission testing was performed for minimum and maximum power levels in transmit mode.

Method of Measurement: TIA/EIA-603-B clause 2.2.12

The equipment is placed on the turntable and placed in normal operation transmit mode of operation.

A broad-band receiving antenna located 3 meters from the transmitter receives any signal radiated from the transmitter and its operational accessories. The antenna is adjustable in height and can be rotated for horizontal or vertical polarization. A spectrum analyzer covering the necessary frequency range is used to detect and measure any radiation received by the antenna.

The transmitter's modulated pseudo random digital signal is monitored and adjusted to obtain peak reading of received signals wherever they occur in the spectrum by:

- (1) Rotating the transmitter under test.
- (2) Adjusting the antenna height.

The testing procedure is repeated for both horizontal and vertical polarization of the receiving antenna. Relative signal strength is indicated on the spectrum analyzer connected to this antenna. The spectrum analyzer resolution bandwidth was set to 10 kHz for emissions below 1 GHz, and 1 MHz for higher frequency emissions. To obtain actual radiated signal strength for each spurious and harmonic frequency observed, a standard signal generator with calibrated output is connected to an antenna adjusted to in the range from 30 MHz to that harmonic frequency. This antenna is substituted for the transmitter under test. The signal generator output level is adjusted until a reading identical to that obtained with the actual transmitter is observed on the spectrum analyzer. Signal strength is then derived from the generator and appropriate cable losses due to set up. Measured emissions for both maximum and minimum transmit power levels are recorded in tables in Exhibit 6.

7.4 Emission Chart 902 MHz to 928 MHz ISM Band --- pursuant to 47 CFR 15.247(c)

- (1) Connect DUT to spectrum analyzer through 10 dB, 2W, RF power attenuator
- (2) Set up the spectrum analyzer as follows for measurement:
 - (a) Center frequency 902.525 MHz
 - (b) Span = 100KHz
 - (c) Sweep = Auto
 - (d) Ref Level = 30 dBm
 - (e) Trace = Max Hold (Positive peak detector)
- (3) Initiate transmission at 902.525 MHz and measure power
- (4) Change spectrum analyzer frequency to center frequency 901.95 MHz and measure power.
- (5) Repeat steps 2 and 3 for 927.475 MHz
- (6) Repeat step four for center frequency 928.05 MHz.

The comparison between on channel power in a 100 KHz BW and outside band edge 100 KHz BW power at both band edges demonstrates compliance with 47 CFR, part 15.247(c)

7.5 Frequency Stability -- Pursuant to 47 CFR 2.947(c)

Measuring the frequency accuracy of the iDEN time division multiplexed (TDM) transmitter needs special procedures for 3 reasons. First is the short (15 ms.) nature of its TDM pulses, which preclude the use of an ordinary CW type digital frequency counter. Second, software in the radio prevents the radio from transmitting its TDM pulses unless it is receiving a signal on the trunking system control channel. Third, to maintain the very high stability (greater than that required by part 90 rules) needed for system operation, the radio transmitter frequency is controlled by an automatic frequency control loop in the radio's receiver which locks onto the system forward control channel produced by a compatible FCC certified part 90 base station. This process results in electronic adjustments of the synthesizer section of the radio, which is used for both transmission and reception.

As a result, unlike traditional transceivers which do not frequency lock to a remote base station reference frequency, the transmitter frequency accuracy is essentially independent of the voltage and temperature induced variations of the subject transceiver's frequency reference oscillator. Rather, the transceiver frequency stability is that of the remote base station, but degraded by any inaccuracy in the transceiver frequency locking process.

By locking onto a base station meeting the requirements of 47 CFR 90.213, which is necessary for the transceiver to function, the transceiver transmitter inherits the inherent 1.5 PPM or better stability of the compatible base station. To assure attainment of the frequency accuracy requirement (1.5 PPM accuracy requirement for the 800MHz band and the 1.5PPM accuracy requirement for the 900MHz band) of part 90.213 for this transceiver, the frequency error is measured when locked to a base station simulator.

Frequency Error vs. temperature

The radio product sample tested used a frequency of 860.9875/820.9875 MHz (800MHz Band) and 938.48125/899.48125 MHz (900MHz band). A Power Supply was controlled to provide a continuous 4.0VDC to the unit tested. The sensor leads from the power supply were attached to the input of the DC/RF test fixture in which the radio was placed. A Temperature Chamber was used to control a temperature range of -30 degree Celsius to +60 degree Celsius.

At each set point, a soak time of 15 minutes was used to ensure thermal penetration of the unit tested before each measurement of frequency error was taken. A soak time of 45 minutes was used at -30 degree Celsius to ensure thermal penetration of the unit tested because of the variance from the starting temperature of +25 degree Celsius. Soak cycles of 20 minutes each thereafter were used because of the fact that the set points were incremented at 10 degree (Celsius) steps.

The measurement was taken by placing the unit tested into a phone call to the Motorola R2660C. The iDEN 3:1 Call Test on the Motorola R2660C was controlled to facilitate the call. Once the call had been established, a Hewlett Packard Model 89441A gathered measurements of the frequency error and recorded it to a data file.

After having taken measurement at a specific set point in the temperature range previously specified, the iDEN 3:1 Call test on the Motorola R2660C was terminated. The Temperature Chamber would proceed to its next increment and repeat the test execution process at the end of that particular soak cycle. The process was continued until measurements were made at each of the specified temperatures in the temperature range previously mentioned.

Frequency Error vs. voltage

The unit tested used a frequency of 860.9875/820.9875 MHz (800MHz Band) and 938.48125/899.48125 MHz (900MHz band). A Power Supply was controlled to provide a voltage range of 3.55VDC to 4.2VDC to the unit tested. The sensor leads from the power supply were attached to the input of the battery eliminator of the unit tested.

The measurements were taken by placing the unit tested into a phone call to the Motorola R2660C. The iDEN 3:1 Call Test on the Motorola R2660C was controlled to facilitate the call. Once the call had been established, a Hewlett Packard Model 89441A took measurement of the frequency error and recorded it to a data file.

After having taken a frequency error measurement at 4.2VDC, the Power Supply's output was reduced by an increment of 0.1VDC. The measurement process was repeated until Frequency Error measurements were made in 0.1VDC steps of each of the specified voltages in the range previously mentioned.

ISM Band: Frequency Error measurement in 902 MHz to 928 MHz ISM band

The unit was tested at a transmitter output frequency of 915.525 MHz. A power supply with the capability of toggling between 4.0 V and 3.55 V was used to provide battery voltage to the unit being tested. The units RF output was attached to a spectrum analyzer capable of making an occupied bandwidth measurement with high frequency accuracy.

The measurements were made by soaking the unit tested in an idle mode for the length of time necessary to stabilize transmitter temperature, at least 40 min per temperature. At the end the temperature soak the transmitter was enabled in the ISM band. Frequency deviation from 915.525 MHz was recorded after the transmitter had produced full output power for 10 seconds (as determined manually).

During operation of the transmitter at -30C, 20C, and 50C an attempt was made to determine frequency error caused by changing the supply voltage from 4.0 VDC (nominal) to 3.55 VDC (minimum). The voltage was toggled from nominal to minimum to nominal repeatedly while monitoring frequency.

Method of Measurement: Proprietary

Since the transmitter frequency is locked to the frequency of the compatible base station via the receiver in this transceiver, frequency accuracy data was measured with the transceiver locked onto a base station transmitter emulated by a Motorola R2660C Service Monitor as shown in Figure 7-1. This was done using the Quad-16QAM time division multiple access (TDMA) characteristic of the transceiver wherein it was placed into a TDMA mode of transmission as normally used to make a call to a landline phone.

During the test the transceiver was receiving a very high accuracy forward control channel frequency signal from the compatible base station emulator and TDMA transmitting a signal on the reverse control channel at a frequency 45 MHz lower in the 800MHz band, (39 MHz lower in the 900MHz band) corresponding to the normally assigned frequency separation. A Hewlett Packard model 89441A signal analyzer was used to measure the centroid frequency of the emission. The frequency of the transceiver was measured as operating voltage or temperature was varied, and compared to the frequency of the assigned channel.

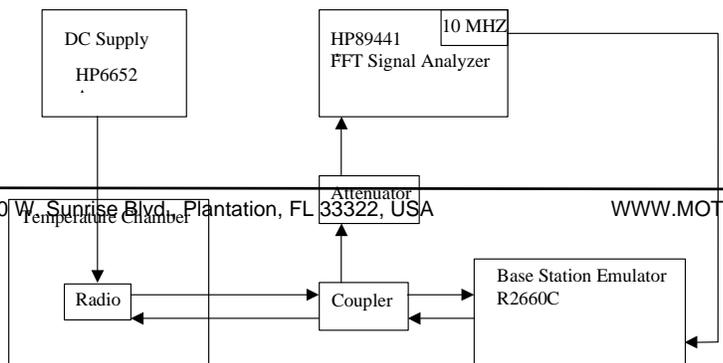


Figure 7-1: Transmit Frequency Measurement Setup

7.6 Power Line Conducted Spurious Output Voltage Pursuant 47 CFR 15.107

Test Site:

Open Area Test Site (OATS) of the Timco Eng. Lab, 849 N.W. State Road 45, Newberry, Florida 32669 which is accredited to ISO/IEC 25 from the American Association for Laboratory Accreditation (FCC Registration: 95517 /Industry Canada: 2056-A).

Method of Measurement: TIA/TEA-603-B clause 2.1.3

Connect the receiver to the power line through a line stabilization network. A spectrum analyzer of nominal 50 Ω impedance to one terminal (“neutral”) of the line stabilization network. The spectrum analyzer is then tuned to search for spurious outputs from 150 kHz to 30 MHz pursuant 47 CFR 15.107. All spurious voltages are recorded. Six highest local maxima are noted, measured with a “Quasi-peak” and “Average” detectors, and then tabulated.

7.7 Carrier Separation between Hopsets

The carriers within a 900 ISM Band hopset are separated by 500 kHz, and the 20 dB bandwidth of a 900 ISM Band carrier is 25.6 kHz.

The test is setup as shown in Figure 7-2. The spectrum analyzer is setup to capture two adjacent carriers. Transmission in the 900 ISM Band mode is initiated until relevant data is captured.




Figure 7-2. Test bench for ISM Band multi-channel measurements.

7.8 Hopping Bandwidth between Hopsets

The aggregate of all 10 hopsets result in an overall carrier separation of 50 kHz with a 20 dB bandwidth of 25.6 kHz.

- Step 1. Connect the DUT to the spectrum analyzer as in Figure 7-3.
- Step 2. Set up the spectrum analyzer as required to measure the 20 dB bandwidth
 - Span = 100 kHz
 - RBW = 300 kHz
 - Sweep = Auto
 - Ref. Level = 30 dBm
 - Trace = Max Hold (RMS Detector used)

Occupied Bandwidth
 Step 3. Initiate Transmission until relevant data captured.

- Step 4. Set up the spectrum analyzer as required to capture two adjacent carriers.
 - Span = 150 kHz
 - RBW = 300 Hz
 - Sweep = Auto
 - Ref. Level = 30 dBm
 - Trace = Max Hold
 - Use Markers
- Step 5. Initiate Transmission until relevant data captured.

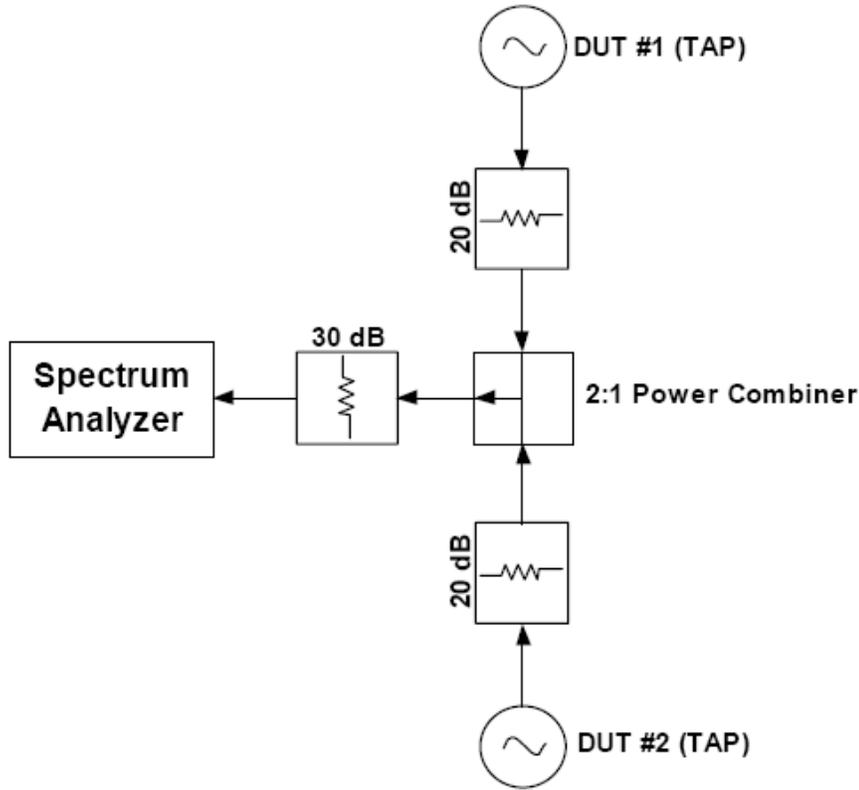


Figure 7-3. Test setup for multi-channel measurements.

7.9 Average Time of Occupancy

- Step 1. Set up the spectrum analyzer (or oscilloscope) as required to capture a single transmitted burst (or a continuous stream of bursts at the same frequency).
- Step 2. Initiate Transmission until relevant data captured.
- Step 3. Measure the duration of the 85.625 ms burst.
- Step 4. Describe worst case scenario (continuous transmission).

7.10 Equal Distribution of Hopping Frequencies for Continuous Transmission

Through ISM Band subscriber test-mode software, a frequency counting algorithm was implemented and used to keep count of how many times a particular frequency was used during a continuous transmission with a DUT. From this data, the frequency distribution can be calculated.

7.11 Equal Distribution of Hopping Frequencies for Discontinuous Transmission

Through ISM Band subscriber test-mode software, a frequency counting algorithm was implemented and used to keep count of how many times a particular frequency was used during a transmission with a DUT. The algorithm used the probability density function for 800/900 Band dispatch call lengths based on actual user data (refer to Figure 7-4) to model multiple ISM Band transmission times with the same call length distribution. The frequency distribution was calculated from the data generated.

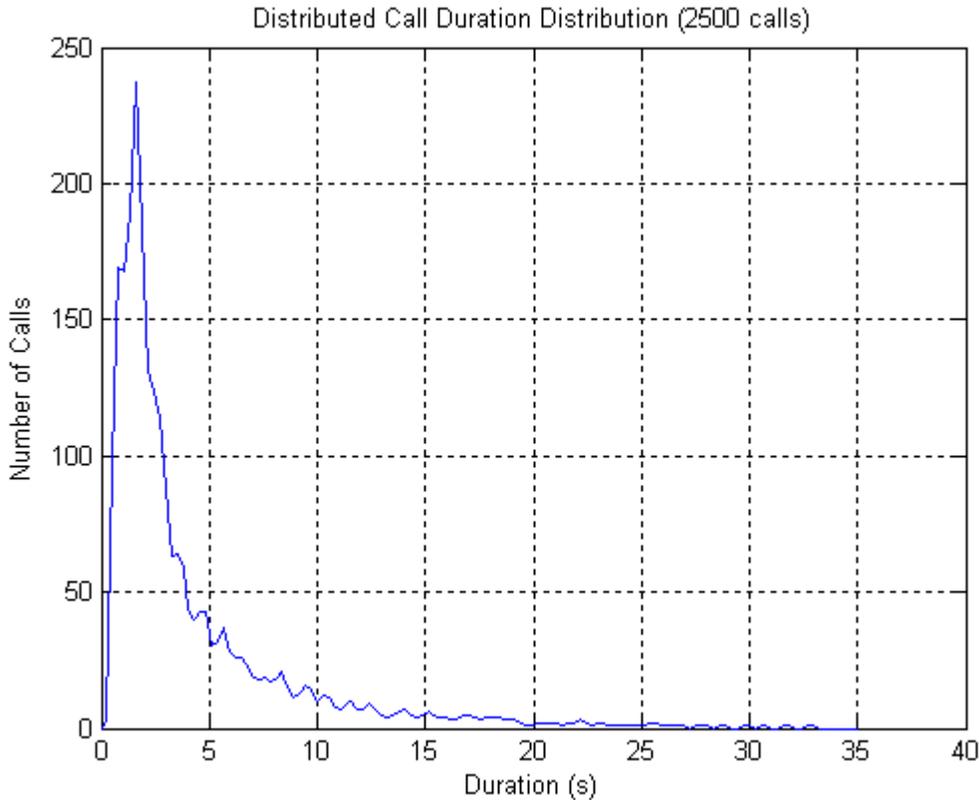


Figure 7-4. Call-length Probability Distribution Function

7.12 Measurement Equipment List ---- 47 CFR 2.947(d)

1. Spectrum Analyzer
 - H.P. 8566B
 - H.P. 8563E
 - Rhode & Schwarz ESI26
2. Vector Signal Analyzer
 - H.P. 89441A
3. Communications System Analyzer
 - Motorola R2660C MIRS Digital Communication System Analyzer
4. Oscilloscope
 - HP 54616B, Oscilloscope
 - Tektronix, Model TCP202, Current Probe
5. RF Signal Generator
 - H.P. 8656A
 - Rhode and Schwarz SMP22

- H.P. E4420A
- 6. Power Meter
 - H.P. 437B Power Meter
 - H.P. 8482A Power Sensor
- 7. Multimeter
 - Keithley 2001 Multimeter
- 8. Power Supply
 - Motorola Lithium Ion Battery, Kit #: NTN 5705A
 - DC Power Supply, H.P., Model: 6652A
 - DC Power Supply, H.P., Model: 6632A
 - DC Power Supply, H.P., Model: 6032A
 - Battery Charger, Model: NNTN4680A
 - DC/RF Test Fixture, 22000uF shunt capacitor / series .2 ohm resistor
- 9. RF Load
 - Weinschel Engineering, Model: 9305-30, 20 Watt, 30 dB Attenuator
 - Weinschel Engineering, Model: 9305-10, 20 Watt, 10 dB Attenuator
 - Narda, Model: MOD766-30, 20 Watt, 30 dB Attenuator
- 10. Filter
 - Trilithic, Model: X5HX1612-0-75-AA, High Pass Filter
 - Trilithic, Model: R9H1-1G4/8G-28A, High Pass Filter
- 11. Amplifier
 - MITEQ AFS5-00101800-25-UJLN, 1-18GHz, 25dB Gain Amplifier
 - PST 10W Amplifier
- 12. Antenna
 - Watkins - Johnson, 0.5 GHz - 12.4 GHz, Model WJ-48010
 - Watkins - Johnson, Model: AR122
 - A.H. Systems Inc., Model: SAS-200/571, 700MHz - 18GHz, Double Ridge Guide Horn
 - EMCO, Model: 3141, 20MHz – 1GHz, Biconilog
 - Schaffner-Chase EMC Ltd., Bilog Antenna, Model CBL6112B
 - Watkins-Johnson L.P. antenna AR7-17A
 - Sleeved-Dipole
- 13. Temperature Chamber
 - Thermotron, Model: S-8.0C
- 14. LISN
 - EMCO, Model: 3810/2NM, Line Impedance Stabilization Network
- 15. Antenna Positioning Mast / Turntable
 - Sunol Sciences Corp., Model: FM 2011, Turntable
 - Sunol Sciences Corp., Model: TLT95, Antenna Positioning Mast
 - Sunol Sciences Corp., Model: SC98V, System controller
 - Scientific Atlanta Antenna Analyzer System 2083A
- 16. Computers
 - Dell, Laptop Computer
 - Hitachi MX 166 computer, Hyperlink Terminal
 - Dell Precision 420 Computer
- 17. Programming Cable
 - RS232 Data Cable
- 18. Table
 - PVC Table
- 19. RF Tray
 - OATS RF Tray, Model 2000
- 20. Test Site
 - OATS, Ground plane
 - 60' Tapered Anechoic Chamber, Emerson & Cummings 1203