



MOTOROLA

**FCC ID: AZ489FT5848
DECLARATION OF COMPLIANCE HAC ASSESSMENT**

**Government & Enterprise Mobility Solutions
EME Test Laboratory
8000 West Sunrise Blvd
Fort Lauderdale, FL. 33322**

Date of Report: March 01, 2006
Report Revision: Rev. O
Report ID: FCC HAC rpt_i580_Rev O_060301SR3525

Responsible Engineer: Stephen C. Whalen
Date/s Tested: 2/24/2006, 2/25/2006
Manufacturer/Location: Motorola - Plantation
Sector/Group/Div.: iDEN Subscriber
Date submitted for test: 12/2/05
DUT Description: i580; iDEN1: 1:3 TDMA; 16 QAM 0.6W
806-825; 896-902 MHz
Test TX mode(s): 1:3
Max. Power output: iDEN - 0.640W; Pulse Averaged; Factory tuned
Nominal Power: iDEN - 0.600W; Pulse Averaged; Factory tuned
TX Frequency Bands: iDEN - 806-825, 896-902MHz
Signaling type: TDMA: iDEN
Model(s) Tested: H83XAH6RR4AN
Model(s) Certified: H83XAH6RR4AN
Serial Number(s): 364AFW00HP
Rule Part(s): 20.19



Approved Applicable Accessories:

Antenna(s):
8575868A01 - 806-928MHz ¼ wave antenna
Gain - 806-825MHz extended 2.15dBd, retracted -1.16 dBd, 896-902MHz extended 2.15dBd, retracted -1.22dBd
Battery(ies):
SNN5765A High Performance Li Ion, Battery Cover NNTN2332A
SNN5744A Slim Li Ion, Battery Cover NNTN2331A

**Max E-Field emission = 72.4 V/m @ 813.5125MHz
Max H-Field emission = 0.148 A/m @ 806.0125MHz
M Category = M3**

Based on the information and the testing results provided herein, the undersigned certifies that when used as stated in the operating instructions supplied, said product complies with the ANSI-PC63.19-2001 reference standard. This report shall not be reproduced without written approval from an officially designated representative of the Motorola EME Laboratory.

The results and statements contained in this report pertain only to the device(s) evaluated.

Al Wieczorek; Motorola iDEN Subscriber Division

Approval Date:

Certification Date:

CONTENTS

1.0 Introduction and Overview..... 3
 2.0 Near Field Compliance Criteria (Per PC63.19-2001 rd 3.6) 3
 3.0 Description of Device Under Test (DUT)..... 3
 4.0 Test Equipment List 3
 5.0 Description of Measurement System..... 4
 6.0 Measurement System Verification 4
 6.1 System Verification Test Results..... 5
 7.0 DUT Setup and Test Procedure..... 5
 8.0 Environmental Test Conditions..... 6
 9.0 Test Results Summary..... 6
 10.0 Probe Modulation Factor Measurement 7
 11.0 Uncertainty Budget..... 9
 12.0 Conclusion..... 10

APPENDICES

A System Verification Results 11
 B Measurement Results..... 20
 C Probe Calibration Certificates 39
 D Details of Automated Scanning Method and Computations 57

REVISION HISTORY

Date	Revision	Comments
3/01/06	O	Initial release

1.0 Introduction and Overview

This report details the utilization, test setup, test equipment, and test results of the Hearing Aid Compatibility (HAC) measurements performed at the Government & Enterprise Mobility Solutions (GEMS) EME Laboratory for the model number H83XAH6RR4AN of FCC ID: AZ489FT5848. Measurements were performed to ensure compliance to the PC63.19-2001 rd 3.6 standard. This report demonstrates compliance for near field emissions only and not for the T-coil performance compliance.

The test results presented herein clearly demonstrate compliance FCC 47 CFR section 20.19 and with the latest version of PC63.19-2001 rd 3.6 and only reflect the performance of the stated model herein.

2.0 Near Field Compliance Criteria (Per PC63.19-2001 rd 3.6)

Near Field M-Rating	AWF	Target Parameters	
		E-Field Emissions Peak V/m	H-Field Emissions Peak V/m
M3	iDEN = 0	63.1 - 112.2	0.19 - 0.34
M4	iDEN = 0	< 63.1	< 0.19

3.0 Description of Device Under Test (DUT)

FCC ID: AZ489FT5848 is a digital multi-service data capable device that employs time division multiplexing transmission technology with a duty cycle ranging from 16.67% to 33.33% using 16-QAM modulation for voice or circuit data transmission. This device may be used while held against the head in voice mode. FCC ID: AZ489FT5848 is capable of operating in the 806-825 MHz and 896-902MHz bands. The rated power is 0.6 watts pulse averaged.

The maximum output is 0.640 watts pulse average as defined by the upper limit of the production line final test station. The DUT was tuned to be within 5% of the maximum rated power.

4.0 Test Equipment List

Equipment Type	Model Number	Serial Number	Calibration Due Date
HP Power Meter (HP)	E4419B	MY20330364	1/31/2007
HP Power Sensor (HP)	8482B	3318A05259	3/28/2006
HP Power Sensor (HP)	8482B	3318A06774	3/22/2006
AMP (ComTech PST)	AR88258-10	N1R1A00-1015	CNR
Signal Generator (Agilent)	E4421B	US40051446	12/29/2007
Signal Generator (Agilent)	E4438C	MY42082269	1/31/2008
Directional Coupler (NARDA)	3020A	40295	7/18/2006
H-Field probe	H3DV6	6166	7/7/2006
E-Field probe	ER3DV6	2350	7/7/2006
SPEAG	DASY4	Version 4.5	NA
Data Acquisition Electronics (DAE)	DAE3V1	363	3/24/2006
Spectrum Analyzer (Advantest)	R3265A	45060026	CNR
Adjustable Attenuator (Weinschel)	940-114-33	9073	2/14/2007


5.0 Descriptions of Measurement System

The laboratory utilizes a Dosimetric Assessment System (DASY4™) measurement system Version 4.5 manufactured by Schmid & Partner Engineering AG (SPEAG™), of Zurich Switzerland. The test system consists of a Stäubli RX90L robot, DAE3V1, ER3DV6 E-Field probe, H3DV6 H-field probe, as well as the integrated HAC extension. Please reference the SPEAG user manual and application notes for detailed probe, robot, and HAC calibration and computational procedures. Section 4.0 presents relevant test equipment information. Appendices C present the applicable calibration certificates. Additional details concerning the test system measurement methods and calculations are provided in Appendix D.

The DASY4™ system is operated per the instructions in the DASY4™ Users Manual. The complete manual is available directly from SPEAG™. All measurement equipment used to assess HAC compliance was calibrated as indicated in section 4.0

6.0 Measurement System Verification

The HAC measurements were conducted with E and H field probes model/serial numbers ER3DV6/SN2350 and H3DV6/SN6166. An un-modulated CW signal was used for system verification following the guidelines specified in the referenced standard. Note that the 1 cm probe to dipole separation is measured from the top surface of the dipole to the calibration reference point of the probe. The DASY4 output files of the system verification test results are included in Appendix A. The photos below depict the validation setup using a planar dipole per ANSI PC63.19 section 4.2.2.1.4. Section 6.1 summarizes the system performance check results.

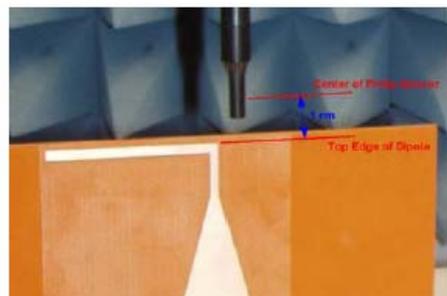

6.1 System Verification Test Results

In accordance with C63.19-2005 clause 4.2.2.1 setup verification measurement results listed and compared with expected values in the following tables using an un-modulated signal (CW) from a commercially available signal generator to drive the reference dipole. Plots of the field distributions observed while scanning the dipole are shown in Appendix A.

C63.19 clause 4.2.2.1.2 recommends additional test cases, one of which is to compare results from an 80% amplitude modulated (AM) signal with the CW results. The results obtained are also listed below.

E-Field CW

Frequency (MHz)	Input Power (W)	E-Field Results (V/m)	PC63.19 Target (V/m)	% Deviation w/ drift
813.5	0.1	202.2	206.6	-2.72%
898.5	0.1	201.9	200.0	0.65%

E-Field AM 80% Modulation

Frequency (MHz)	E-Field Results (V/m)	PC63.19 Target (V/m)	% Deviation w/ drift
813.5	192.7	206.6	-7.24%
898.5	200.5	200.0	0.29%

H-Field CW

Frequency (MHz)	Input Power (W)	H-Field Results (A/m)	PC63.19 Target (A/m)	% Deviation w/ drift
813.5	0.1	0.4687	0.4973	-4.92%
898.5	0.1	0.4746	0.4989	-5.25%

H-Field AM 80% Modulation

Frequency (MHz)	H-Field Results (A/m)	PC63.19 Target (A/m)	% Deviation w/ drift
813.5	0.4579	0.4973	-7.94%
898.5	0.4636	0.4989	-6.94%


An additional recommend test case is the emulated or real test signal. Unfortunately no calibrated test set or signal generator emulating the iDEN protocol is commercially available that has the capability to accurately reproduce the quad 16-QAM signal. Alternatively the results for iDEN modulation were obtained using the device under test as a signal source to drive the antenna via an antenna adapter and an attenuator to produce field strengths similar to that of the device under test. That data is provided in Section 10 where it is compared to CW modulation during the measurement of the probe modulation response, per the alternate procedure given in C63.19-2005 Annex C.3.1.

7.0 DUT Setup and Test Procedure

The automated test procedure guidelines presented in PC63.19-2001 section 4.3.1.2.2 were followed in order to demonstrate HAC compliance. The photos below depict the DUT test setup. The reference grid depicts the alignment with the center of the acoustic output used for coupling to hearing aid devices. The test results using embedded test mode software with an unlighted display are presented in section 9.0.



DUT test setup with 10mm spacing

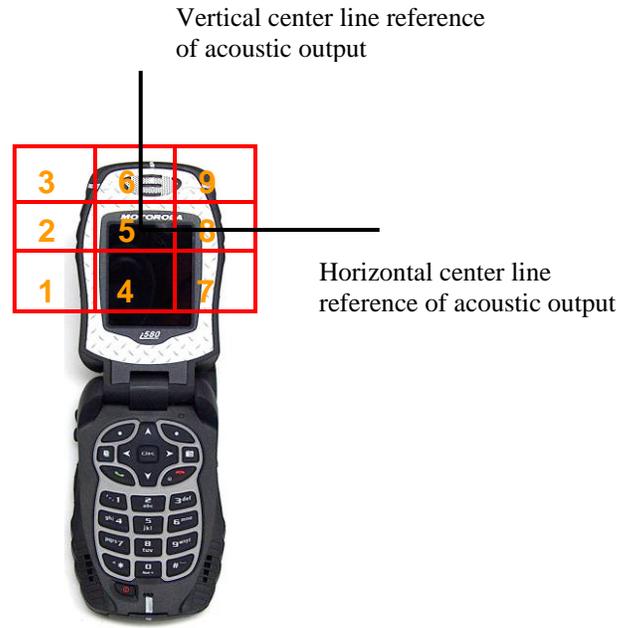

WD with reference grid (Not to scale)

8.0 Environmental Test Conditions

The table below presents the range and average environmental conditions during the HAC tests reported herein:

	Target	Measured
Ambient Temperature	23 °C +/- 5 °C	Avg.:22.2 °C Range: 22.0-22.4 °C
Relative Humidity	0 - 80 %	Avg.:51.4 % Range: 49.5-53.9 %

The EME Lab RF environment uses a Spectrum Analyzer to monitor for extraneous large signal RF contaminants that could possibly affect the test results. If such unwanted signals are discovered the HAC scans are repeated. Per the pretest procedures in PC63.19-2001 rd 3.6 section 4.3.1.1 footnote 13, interference from reflective objects was found not to exceed -20dB.

9.0 Test Results Summary

The values listed in the following tables were calculated by the applicable Probe Modulation Factor (PMF) determined in section 10 for the frequency band in which the handset transmitted during the scan.

iDEN 800MHz Band

Freq. (MHz)	Battery	Rated Max Power (W)	E/H Field	Measured Field (V/m or A/m)	Appendix B Data (pg)	Excluded Cells	M-Rating
813.5125	SNN5744 A	0.640	E	72.4	21	1,2,4	M-3
813.5125	SNN5765 A	0.640	E	71.4	23	1,2,4	M-3
806.0125	SNN5744 A	0.640	E	70.7	24	1,2,4	M-3
824.9875	SNN5744 A	0.640	E	67.3	25	1,2,4	M-3
813.5125	SNN5744 A	0.640	H	0.136	26	1,4,7	M-4
813.5125	SNN5765 A	0.640	H	0.136	27	1,4,7	M-4
806.0125	SNN5765 A	0.640	H	0.148	28	1,4,7	M-4
824.9875	SNN5765 A	0.640	H	0.140	30	1,4,7	M-4

iDEN 900MHz Band


Freq. (MHz)	Battery	Rated Max Power (W)	E/H Field	Measured Field (V/m or A/m)	Appendix B Data (pg)	Excluded Cells	M-Rating
898.5187	SNN5744 A	0.640	E	45.8	31	1,4,7	M-4
898.5187	SNN5765 A	0.640	E	47.2	32	1,4,7	M-4
896.0187	SNN5765 A	0.640	E	46.3	33	1,2,4	M-4
900.9812	SNN5765 A	0.640	E	47.8	34	1,4,7	M-4
898.5187	SNN5744 A	0.640	H	0.108	35	1,4,7	M-4
898.5187	SNN5765 A	0.640	H	0.108	36	1,4,7	M-4
896.0187	SNN5765 A	0.640	H	0.112	37	1,4,7	M-4
900.9812	SNN5765 A	0.640	H	0.111	38	1,4,7	M-4

Probe rotations were done at the highest measured locations for each data page. The highest results for both the E and H field probes are included in appendix B following the HAC results.


10.0 Probe Modulation Factor Measurement

- A. Per C63.19 rd 3.6 alternate measurement procedure steps 1, 2 and 3 the phone was set into a test mode at within 5% of maximum output power. The phone was connected to the reference dipole antenna through an attenuator to assure the E-field probe reading on the field strength measurement system was in the range corresponding to a C63.19 category rating of M2, as


illustrated below. The crest factor of the DASY measurement system was set equal to the TDM multiplex factor (3) and the probe reading recorded as noted in the following PMF Data Table.

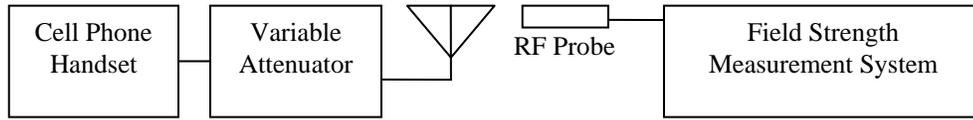


- B. The phone was then connected to a spectrum analyzer as illustrated below. Similar to C63.19 rd 3.6 Figure C-1 step 5, the analyzer was set for zero span (with a time span of 2.5ms. and amplitude scale of 1 dB/div to clearly show the peak amplitude and frequency of the digital modulation symbols that occur at a 4 kHz rate).

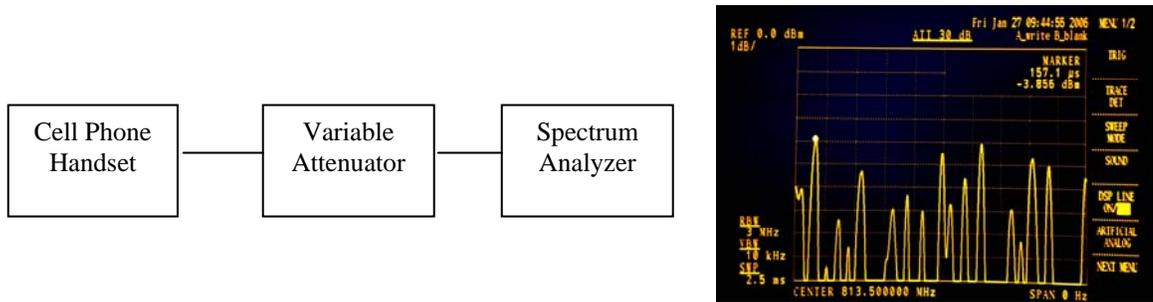

- C. Per C63.19 rd 3.6 step 4 an un-modulated signal from a signal generator operating at the same frequency as the phone was amplified and applied to the spectrum analyzer in lieu of the phone and attenuator, as illustrated below. Per C63.19 rd 3.6 Figure C-1 step 6 the peak amplitude of the signal generator was set equal to the peak amplitude observed with the phone signal.



- D. Per C63.19 rd step 6 the signal applied to the spectrum analyzer was then applied to the reference dipole as shown in Figure 5. The crest factor of the DASY measurement system was set to unity and the probe reading was recorded as noted in the following PMF Data Table.

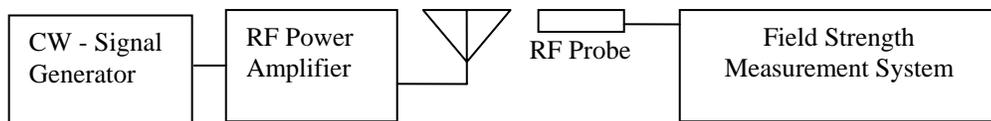

- E. Per C63.19 rd 3.6, step 7 the square root of the ratio of the reading in D above divided by the reading in B above is calculated as the probe modulation factor and listed in the following PMF Data Table.
- F. The above procedure was repeated using an H-field RF probe.

Probe Modulation Factor (PMF) Data

Probe Model / SN	Frequency (MHz)	Source	E/H Field	Measured Field (V/m or A/m)	PMF
ER3DV6 / 2350	813.5	Sig Gen	E	133.1	1.82
ER3DV6 / 2350	813.5	Handset	E	40.19	
ER3DV6 / 2350	898.5	Sig Gen	E	139.3	1.79
ER3DV6 / 2350	898.5	Handset	E	43.59	
H3DV6 / 6166	813.5	Sig Gen	H	0.3396	1.81
H3DV6 / 6166	813.5	Handset	H	0.1033	
H3DV6 / 6166	898.5	Sig Gen	H	0.3147	1.78
H3DV6 / 6166	898.5	Handset	H	0.09953	

11.0 Uncertainty Budget

Motorola Uncertainty Budget for E-Field HAC Testing

Error	Value (R=1)	Distribution	Div	Std Unc	Unc^2	Source
RF Reflections	5.6%	R	1.73	3.2%	0.10%	From Reflection Test 050628.xls
Probe Calibration	5.1%	N	1.00	5.1%	0.26%	SPEAG DASYS Chapter 28 Hearing Aid Extension (Draft)
Isotropy	3.6%	R	1.73	2.1%	0.04%	From averaged results from IDEN HAC Tests i730, 850, 855, 450, 560 formatted.xls
Frequency Response						
Linearity	4.7%	R	1.73	2.7%	0.07%	SPEAG DASYS Chapter 28 Hearing Aid Extension (Draft)
Boundary Effects	2.4%	R	1.73	1.4%	0.02%	SPEAG DASYS Chapter 28 Hearing Aid Extension (Draft)
Sensor Displacement	16.5%	R	1.73	9.5%	0.91%	SPEAG DASYS Chapter 28 Hearing Aid Extension (Draft)
Probe Positioning accuracy	2.7%	R	1.73	1.6%	0.02%	SPEAG DASYS Chapter 28 Hearing Aid Extension (Draft)
Probe Positioner	1.2%	R	1.73	0.7%	0.00%	SPEAG DASYS Chapter 28 Hearing Aid Extension (Draft)
Extrapolation/Interpolation	1.0%	R	1.73	0.6%	0.00%	SPEAG DASYS Chapter 28 Hearing Aid Extension (Draft)
System Detection Limit	1.0%	R	1.73	0.6%	0.00%	SPEAG DASYS Chapter 28 Hearing Aid Extension (Draft)
Readout Electronics	0.3%	N	1.00	0.3%	0.00%	SPEAG DASYS Chapter 28 Hearing Aid Extension (Draft)
Integration Time	2.6%	R	1.73	1.5%	0.02%	SPEAG DASYS Chapter 28 Hearing Aid Extension (Draft)
Response Time	0.8%	R	1.73	0.5%	0.00%	SPEAG DASYS Chapter 28 Hearing Aid Extension (Draft)
RF Ambient Conditions	3.0%	R	1.73	1.7%	0.03%	SPEAG DASYS Chapter 28 Hearing Aid Extension (Draft)
Vertical Device Positioning	4.7%	R	1.73	2.7%	0.07%	SPEAG DASYS Chapter 28 Hearing Aid Extension (Draft)
Lateral Device Positioning	1.0%	R	1.73	0.6%	0.00%	SPEAG DASYS Chapter 28 Hearing Aid Extension (Draft)
Device Holder	1.4%	N	1.00	1.4%	0.02%	SPEAG DASYS Chapter 28 Hearing Aid Extension (Draft)
Power Drift	2.9%	R	1.73	1.7%	0.03%	SPEAG DASYS Chapter 28 Hearing Aid Extension (Draft)
				Comb Std. Uncertainty	12.7%	
				Exp Uncertainty	25.5%	

Motorola Uncertainty Budget for H-Field HAC Testing

Error	Value (R=1)	Distribution	Div	Std Unc	Unc^2	Source
RF Reflections	5.6%	R	1.73	3.2%	0.10%	From Reflection Test 050628.xls
Probe Calibration	5.1%	N	1.00	5.1%	0.26%	SPEAG DASY Chapter 28 Hearing Aid Extention (Draft)
Isotropy	3.6%	R	1.73	2.1%	0.04%	From averaged results from iDEN HAC Tests i730, 850, 855, 450, 560 formatted.xls
Frequency Response						
Linearity	4.7%	R	1.73	2.7%	0.07%	SPEAG DASY Chapter 28 Hearing Aid Extention (Draft)
Boundary Effects	2.4%	R	1.73	1.4%	0.02%	SPEAG DASY Chapter 28 Hearing Aid Extention (Draft)
Sensor Displacement	2.4%	R	1.73	1.4%	0.02%	SPEAG DASY Chapter 28 Hearing Aid Extention (Draft)
Probe Positioning accuracy	3.1%	R	1.73	1.8%	0.03%	SPEAG DASY Chapter 28 Hearing Aid Extention (Draft)
Probe Positioner	0.9%	R	1.73	0.5%	0.00%	SPEAG DASY Chapter 28 Hearing Aid Extention (Draft)
Extrapolation/Interpolation	1.0%	R	1.73	0.6%	0.00%	SPEAG DASY Chapter 28 Hearing Aid Extention (Draft)
System Detection Limit	1.0%	R	1.73	0.6%	0.00%	SPEAG DASY Chapter 28 Hearing Aid Extention (Draft)
Readout Electronics	0.3%	N	1.00	0.3%	0.00%	SPEAG DASY Chapter 28 Hearing Aid Extention (Draft)
Integration Time	2.6%	R	1.73	1.5%	0.02%	SPEAG DASY Chapter 28 Hearing Aid Extention (Draft)
Response Time	0.8%	R	1.73	0.5%	0.00%	SPEAG DASY Chapter 28 Hearing Aid Extention (Draft)
RF Ambient Conditions	3.0%	R	1.73	1.7%	0.03%	SPEAG DASY Chapter 28 Hearing Aid Extention (Draft)
Vertical Device Positioning	3.1%	R	1.73	1.8%	0.03%	SPEAG DASY Chapter 28 Hearing Aid Extention (Draft)
Lateral Device Positioning	0.6%	R	1.73	0.3%	0.00%	SPEAG DASY Chapter 28 Hearing Aid Extention (Draft)
Device Holder	1.4%	N	1.00	1.4%	0.02%	SPEAG DASY Chapter 28 Hearing Aid Extention (Draft)
Power Drift	2.9%	R	1.73	1.7%	0.03%	SPEAG DASY Chapter 28 Hearing Aid Extention (Draft)
				Comb Std. Uncertain	8.4%	
				Exp Uncertainty	16.7%	

12.0 Conclusion

The highest Operational Maximum Calculated E and H field emissions results found for FCC ID: AZ489FT5848, model H83XAH6RR4AN are presented below. In accordance with FCC rule 47 CFR 2.1033(d) these test results clearly demonstrate compliance with FCC 47 CFR section 20.19 and with PC63.19-2001 rd 3.6.

Max E Field emission = 72.4 V/m @ 813.5125MHz
Max H Field emission = 0.148 A/m @ 806.0125MHz
M Category = M3

APPENDIX A
System Verification Results

Motorola GEMS EME Laboratory
GEMS-3; DUT: 813.5 MHz HAC Dipole-Date/Time: 2/24/2006 8:52:58 PM

Run#: MeC-SYSP-HAC Val 813.5 E-field 060224-01
Model# / Serial#: MFRL Planer / 002
TX Freq. / Start Power: 813.5 (MHz) / 100 (mW)


Target: 206.6 V/m
Calculated: 202.2 V/m
Drift: 0.0263 dB
Percent from Target (+/-): 2.72 %
(Including Drift)

Comments: CW

Probe: ER3DV6 - SN2350, Calibrated: 7/7/2005, ConvF(1, 1, 1)
Duty Cycle: 1:1, Medium: Air, Medium parameters used: $\sigma = 0$ mho/m, $\epsilon_r = 1$; $\rho = 1000$ kg/m³
Electronics: DAE3 Sn363, Calibrated: 5/24/2005

813.5 MHz Validation/Generic Scan (61x121x1): Measurement grid: dx=5mm, dy=15mm, dz=20mm
Maximum value of Total (interpolated) = 209.7 V/m

813.5 MHz Validation/Generic Scan 2 (41x41x1): Measurement grid: dx=5mm, dy=5mm, dz=20mm
Maximum value of Total (interpolated) = 202.2 V/m

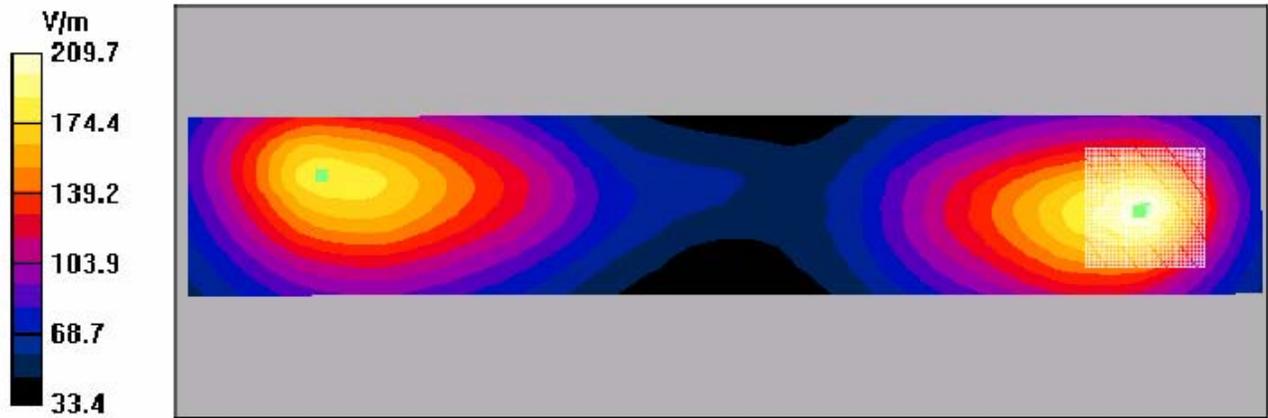

Motorola GEMS EME Laboratory
GEMS-3; DUT: 813.5 MHz HAC Dipole-Date/Time: 2/24/2006 8:58:36 PM

Run#: MeC-SYSP-HAC Val 813.5 AM E-field 060224-02
Model# / Serial#: MFRL Planer / 002
TX Freq. / Start Power: 813.5 (MHz) / 100 (mW)


Target: 206.6 V/m
Calculated: 192.7 V/m
Drift: 0.0241 dB
Percent from Target (+/-): 7.24 %
(Including Drift)

Comments: With 80% AM Modulation On

Probe: ER3DV6 - SN2350, Calibrated: 7/7/2005, ConvF(1, 1, 1)
Duty Cycle: 1:1, Medium: Air, Medium parameters used: $\sigma = 0$ mho/m, $\epsilon_r = 1$; $\rho = 1000$ kg/m³
Electronics: DAE3 Sn363, Calibrated: 5/24/2005

813.5 MHz Validation/Generic Scan (61x121x1): Measurement grid: dx=5mm, dy=15mm, dz=20mm
Maximum value of Total (interpolated) = 200.1 V/m

813.5 MHz Validation/Generic Scan 2 (41x41x1): Measurement grid: dx=5mm, dy=5mm, dz=20mm
Maximum value of Total (interpolated) = 192.7 V/m

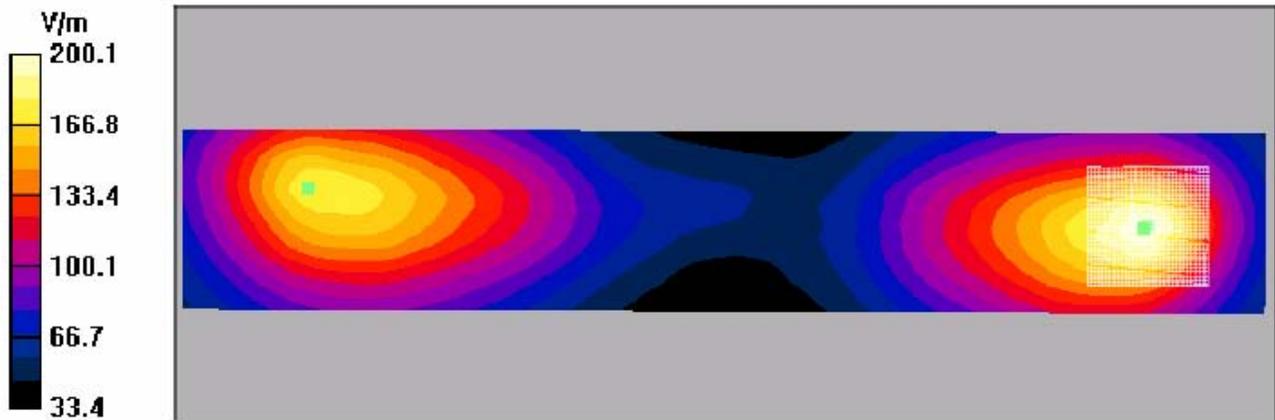

Motorola GEMS EME Laboratory
GEMS-3; DUT: 898.5 MHz HAC Dipole-Date/Time: 2/24/2006 9:30:33 PM

Run#: MeC-SYSP-HAC Val 898.5 E-field 060224-03
Model# / Serial#: MFRL Planer / 004
TX Freq. / Start Power: 898.5 (MHz) / 100 (mW)


Target: 200.0 V/m
Calculated: 201.9 V/m
Drift: 0.013 dB
Percent from Target (+/-): 0.65 %
(Including Drift)

Comments: CW

Probe: ER3DV6 - SN2350, Calibrated: 7/7/2005, ConvF(1, 1, 1)
Duty Cycle: 1:1, Medium: Air, Medium parameters used: $\sigma = 0$ mho/m, $\epsilon_r = 1$; $\rho = 1000$ kg/m³
Electronics: DAE3 Sn363, Calibrated: 5/24/2005

898.5 MHz Validation/Generic Scan (61x121x1): Measurement grid: dx=5mm, dy=15mm, dz=20mm
Maximum value of Total (interpolated) = 195.2 V/m

898.5 MHz Validation/Generic Scan 2 (41x41x1): Measurement grid: dx=5mm, dy=5mm, dz=20mm
Maximum value of Total (interpolated) = 201.9 V/m

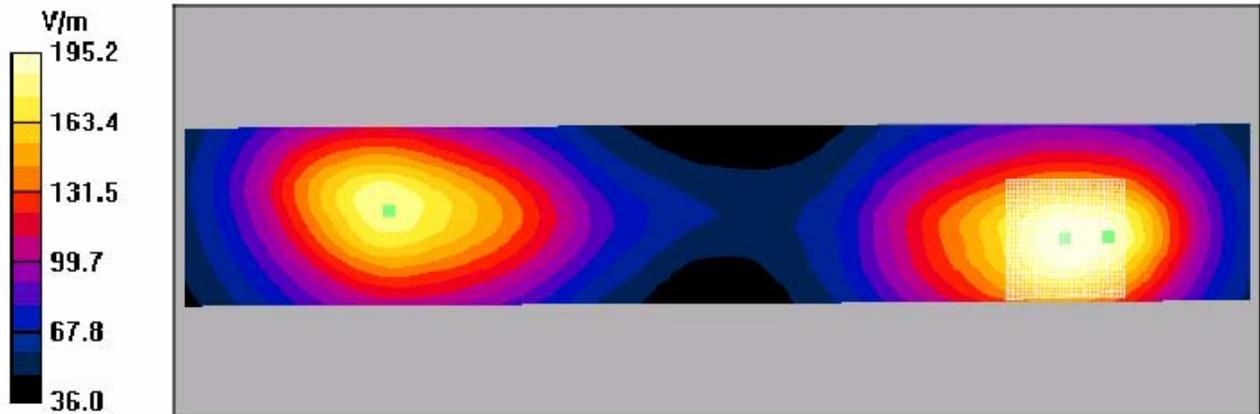

Motorola GEMS EME Laboratory
GEMS-3; DUT: 898.5 MHz HAC Dipole-Date/Time: 2/24/2006 9:41:48 PM


Run#: MeC-SYSP-HAC Val 898.5 AM E-field 060224-04
Model# / Serial#: MFRL Planer / 004
TX Freq. / Start Power: 898.5 (MHz) / 100 (mW)

Target: 200.0 V/m
Calculated: 200.5 V/m
Drift: -0.00165 dB
Percent from Target (+/-): 0.29 %
(Including Drift)

Comments: With 80% AM Modulation On
Probe: ER3DV6 - SN2350, Calibrated: 7/7/2005, ConvF(1, 1, 1)
Duty Cycle: 1:1, Medium: Air, Medium parameters used: $\sigma = 0$ mho/m, $\epsilon_r = 1$; $\rho = 1000$ kg/m³
Electronics: DAE3 Sn363, Calibrated: 5/24/2005

898.5 MHz Validation/Generic Scan (61x121x1): Measurement grid: dx=5mm, dy=15mm, dz=20mm
Maximum value of Total (interpolated) = 201.3 V/m

898.5 MHz Validation/Generic Scan 2 (41x41x1): Measurement grid: dx=5mm, dy=5mm, dz=20mm
Maximum value of Total (interpolated) = 200.5 V/m

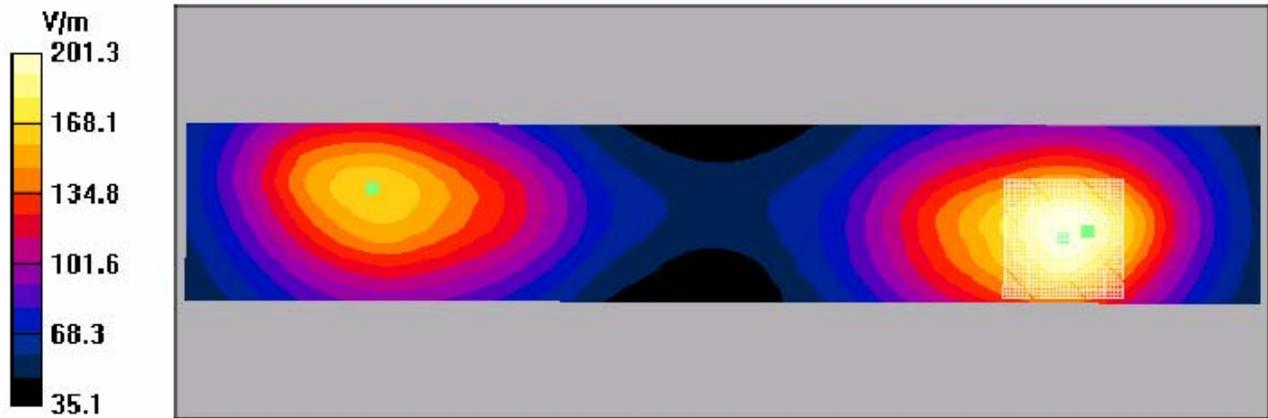

Motorola GEMS EME Laboratory
GEMS-3; DUT: 813.5 MHz HAC Dipole-Date/Time: 2/24/2006 10:38:25 PM

Run#: MeC-SYSP-HAC Val 813.5 H-field 060224-07
Model# / Serial#: MFRL Planer / 002
TX Freq. / Start Power: 813.5 (MHz) / 100 (mW)


Target: 0.4973 A/m
Calculated: 0.4687 A/m
Drift: -0.0382 dB
Percent from Target (+/-): -4.92 %
(Including Drift)

Comments: CW

Probe: H3DV6 - SN6166, Calibrated: 7/7/2005,
Duty Cycle: 1:1, Medium: Air, Medium parameters used: $\sigma = 0$ mho/m, $\epsilon_r = 1$; $\rho = 1$ kg/m³
Electronics: DAE3 Sn363, Calibrated: 5/24/2005

813.5 MHz Validation/Generic Scan (61x121x1): Measurement grid: dx=5mm, dy=15mm, dz=20mm
Maximum value of Total (interpolated) = 0.465 A/m

813.5 MHz Validation/Generic Scan 2 (41x41x1): Measurement grid: dx=5mm, dy=5mm, dz=20mm
Maximum value of Total (interpolated) = 0.469 A/m

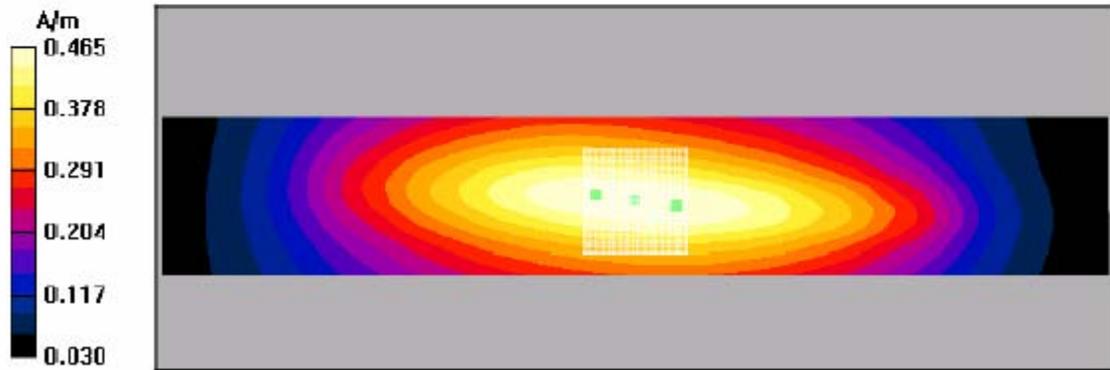

Motorola GEMS EME Laboratory
GEMS-3; DUT: 813.5 MHz HAC Dipole-Date/Time: 2/24/2006 10:44:24 PM

Run#: MeC-SYSP-HAC Val 813.5 AM H-field 060224-08
Model# / Serial#: MFRL Planer / 002
TX Freq. / Start Power: 813.5 (MHz) / 100 (mW)


Target: 0.4973 A/m
Calculated: 0.4579 A/m
Drift: 0.000993 dB
Percent from Target (+/-): 7.94 %
(Including Drift)

Comments: With 80% AM Modulation On

Probe: H3DV6 - SN6166, Calibrated: 7/7/2005,
Duty Cycle: 1:1, Medium: Air, Medium parameters used: $\sigma = 0$ mho/m, $\epsilon_r = 1$; $\rho = 1$ kg/m³
Electronics: DAE3 Sn363, Calibrated: 5/24/2005

813.5 MHz Validation/Generic Scan (61x121x1): Measurement grid: dx=5mm, dy=15mm, dz=20mm
Maximum value of Total (interpolated) = 0.456 A/m

813.5 MHz Validation/Generic Scan 2 (41x41x1): Measurement grid: dx=5mm, dy=5mm, dz=20mm
Maximum value of Total (interpolated) = 0.458 A/m

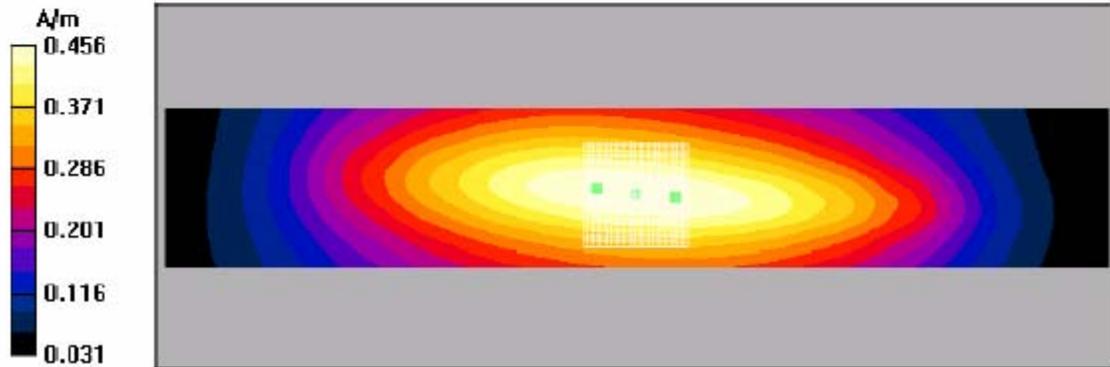

Motorola GEMS EME Laboratory
GEMS-3; DUT: 898.5 MHz HAC Dipole-Date/Time: 2/24/2006 10:13:14 PM

Run#: MeC-SYSP-HAC Val 898.5 H-field 060224-05
Model# / Serial#: MFRL Planer / 004
TX Freq. / Start Power: 898.5 (MHz) / 100 (mW)


Target: 0.4989 A/m
Calculated: 0.4746 A/m
Drift: 0.0173 dB
Percent from Target (+/-): 5.25 %
(Including Drift)

Comments: CW

Probe: H3DV6 - SN6166, Calibrated: 7/7/2005,
Duty Cycle: 1:1, Medium: Air, Medium parameters used: $\sigma = 0$ mho/m, $\epsilon_r = 1$; $\rho = 1$ kg/m³
Electronics: DAE3 Sn363, Calibrated: 5/24/2005

898.5 MHz Validation/Generic Scan (61x121x1): Measurement grid: dx=5mm, dy=15mm, dz=20mm
Maximum value of Total (interpolated) = 0.470 A/m

898.5 MHz Validation/Generic Scan 2 (41x41x1): Measurement grid: dx=5mm, dy=5mm, dz=20mm
Maximum value of Total (interpolated) = 0.475 A/m

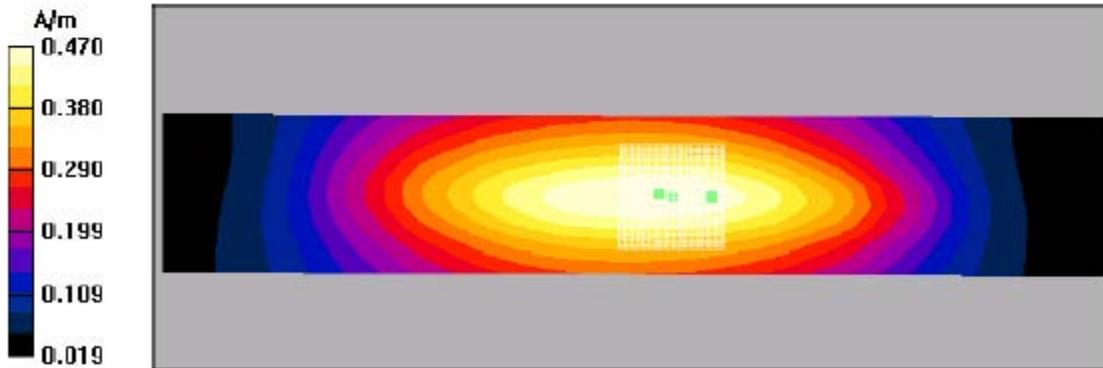

Motorola GEMS EME Laboratory
GEMS-3; DUT: 898.5 MHz HAC Dipole-Date/Time: 2/24/2006 10:18:55 PM

Run#: MeC-SYSP-HAC Val 898.5 AM H-field 060224-06
Model# / Serial#: MFRL Planer / 004
TX Freq. / Start Power: 898.5 (MHz) / 100 (mW)


Target: 0.4989 A/m
Calculated: 0.4636 A/m
Drift: -0.00630 dB
Percent from Target (+/-): 6.94 %
(Including Drift)

Comments: With 80% AM Modulation On

Probe: H3DV6 - SN6166, Calibrated: 7/7/2005,
Duty Cycle: 1:1, Medium: Air, Medium parameters used: $\sigma = 0$ mho/m, $\epsilon_r = 1$; $\rho = 1$ kg/m³
Electronics: DAE3 Sn363, Calibrated: 5/24/2005

898.5 MHz Validation/Generic Scan (61x121x1): Measurement grid: dx=5mm, dy=15mm, dz=20mm
Maximum value of Total (interpolated) = 0.459 A/m

898.5 MHz Validation/Generic Scan 2 (41x41x1): Measurement grid: dx=5mm, dy=5mm, dz=20mm
Maximum value of Total (interpolated) = 0.464 A/m

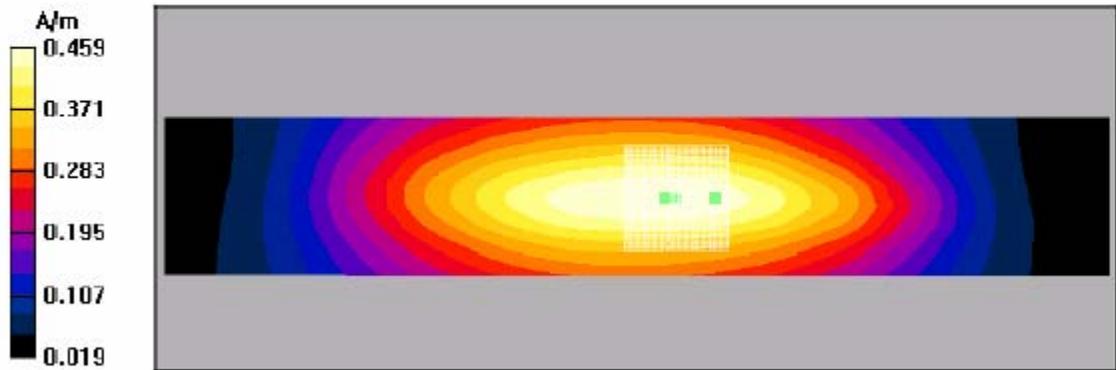

Appendix B
Measurement Results

Motorola GEMS EME Laboratory
GEMS-3; DUT: i580 H83XAH6RR4AN-Date/Time: 2/25/2006 1:59:07 PM

Run#: MeC-i580 Radio 813 E-field 060225-09
 Model# / Serial#: H83XAH6RR4AN / 364AGA0361
 TX Freq.: 813.5125 (MHz)
 Antenna: 8575868A01
 Battery# / Battery Cover#: SNN5744A / NNTN2344A

Comments:


Probe: ER3DV6 - SN2350, Calibrated: 7/7/2005, ConvF(1, 1, 1)
 Duty Cycle: 1:3, Medium: Air, Medium parameters used: $\sigma = 0$ mho/m, $\epsilon_r = 1$; $\rho = 1000$ kg/m³
 Electronics: DAE3 Sn363, Calibrated: 5/24/2005

813.5125 w/SNN5744A Battery/Hearing Aid Compatibility Test (101x101x1): Measurement
 grid: dx=5mm, dy=5mm
 Maximum value of peak Total field = 72.4 V/m
 Probe Modulation Factor = 1.82
 Reference Value = 34.5 V/m; Power Drift = 0.0352 dB
Hearing Aid Near-Field Category: M3 (AWF 0 dB)

E-Field V/m
(Time averaged)

Grid 3 56.0	Grid 6 56.2	Grid 9 52.4
Grid 2 73.6	Grid 5 70.8	Grid 8 63.8
Grid 1 84.7	Grid 4 79.9	Grid 7 72.4

 Excluded sub grids
 Max remaining grid

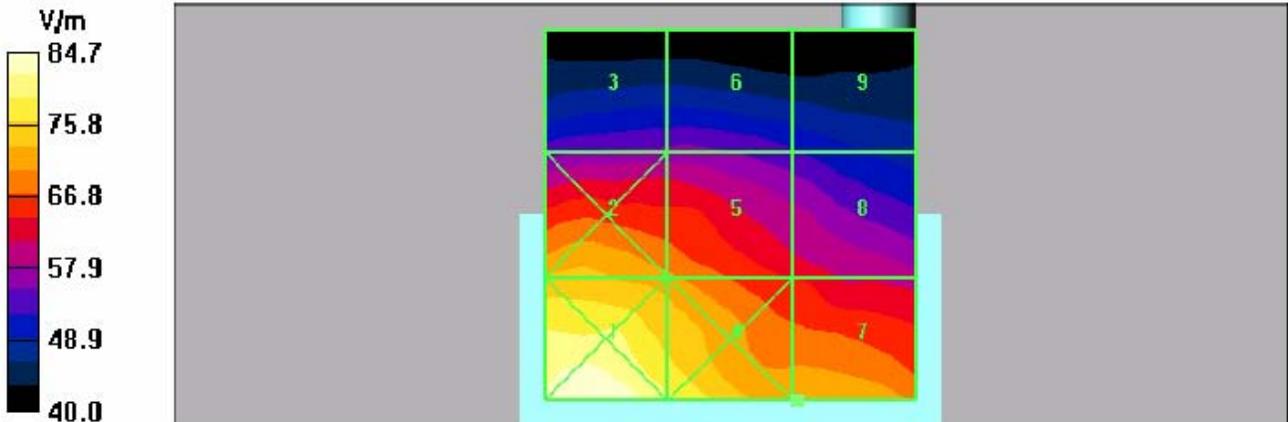


Motorola GEMS EME Laboratory
GEMS-3; DUT: i580 H83XAH6RR4AN-Date/Time: 2/25/2006 1:59:07 PM

Run#: MeC-i580 Radio 813 E-field 060225-09
Model# / Serial#: H83XAH6RR4AN / 364AGA0361
TX Freq.: 813.5125 (MHz)
Antenna: 8575868A01
Battery# / Battery Cover#: SNN5744A / NNTN2344A

Comments:

Probe: ER3DV6 - SN2350, Calibrated: 7/7/2005, ConvF(1, 1, 1)
Duty Cycle: 1:3, Medium: Air, Medium parameters used: $\sigma = 0$ mho/m, $\epsilon_r = 1$; $\rho = 1000$ kg/m³
Electronics: DAE3 Sn363, Calibrated: 5/24/2005

813.5125 w/SNN5744A Battery/Hearing Aid Compatibility Test (101x101x1): Measurement grid: dx=5mm, dy=5mm
Maximum value of peak Total field = 72.4 V/m
Probe Modulation Factor = 1.82
Reference Value = 34.5 V/m; Power Drift = 0.0352 dB
Hearing Aid Near-Field Category: M3 (AWF 0 dB)

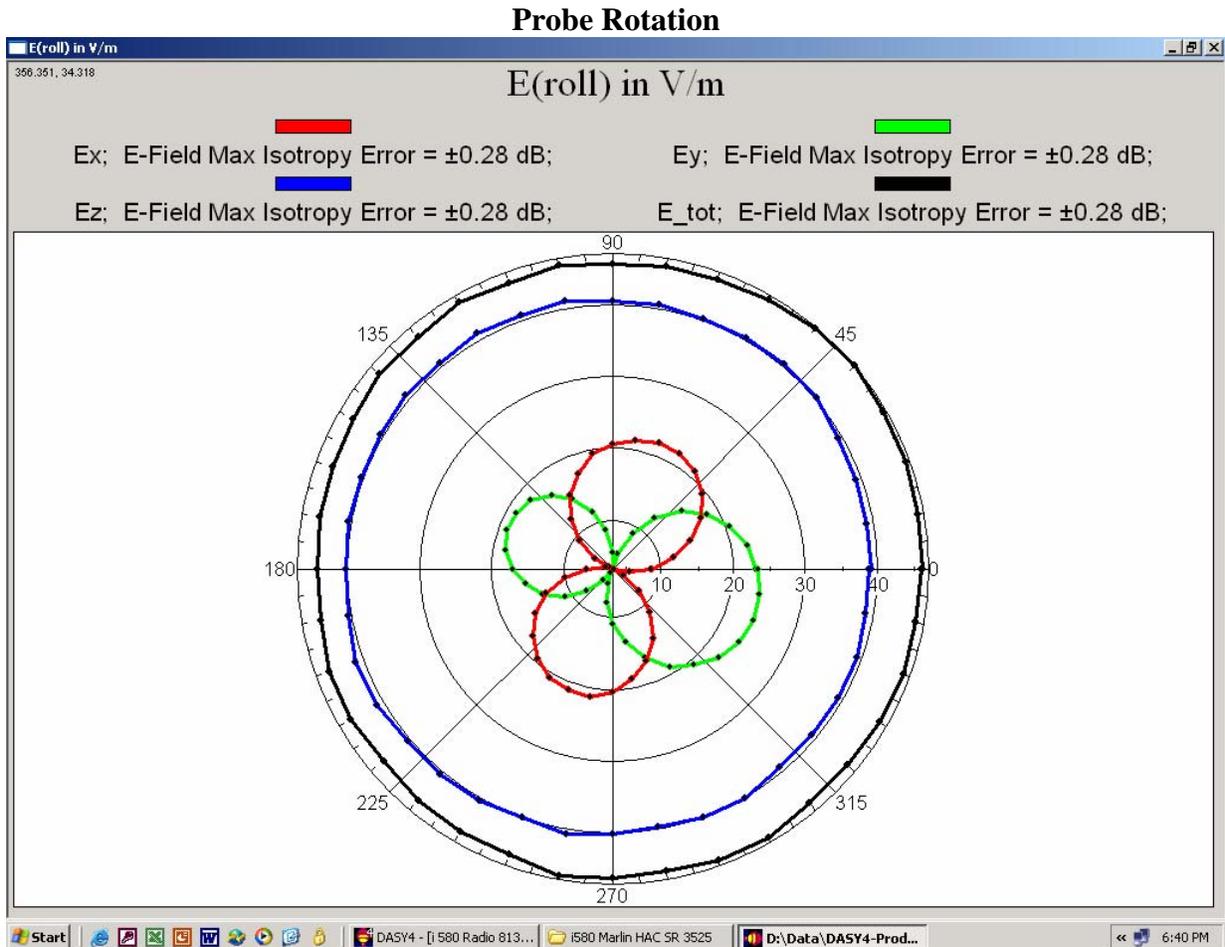

Motorola GEMS EME Laboratory
GEMS-3; DUT: i580 H83XAH6RR4AN-Date/Time: 2/25/2006 2:20:54 PM

Run#: MeC-i580 Radio 813 E-field 060225-10
 Model# / Serial#: H83XAH6RR4AN / 364AGA0361
 TX Freq.: 813.5125 (MHz)
 Antenna: 8575868A01
 Battery# / Battery Cover#: SNN5765A / NNTN2345A

Comments:



Probe: ER3DV6 - SN2350, Calibrated: 7/7/2005, ConvF(1, 1, 1)
 Duty Cycle: 1:3, Medium: Air, Medium parameters used: $\sigma = 0$ mho/m, $\epsilon_r = 1$; $\rho = 1000$ kg/m³
 Electronics: DAE3 Sn363, Calibrated: 5/24/2005

813.5125 w/SNN5765A Battery/Hearing Aid Compatibility Test (101x101x1): Measurement grid: dx=5mm, dy=5mm
 Maximum value of peak Total field = 71.4 V/m
 Probe Modulation Factor = 1.82
 Reference Value = 34.7 V/m; Power Drift = -0.059 dB
Hearing Aid Near-Field Category: M3 (AWF 0 dB)

E-Field V/m
(Time averaged)

Grid 3 56.6	Grid 6 56.6	Grid 9 52.9
Grid 2 73.0	Grid 5 70.9	Grid 8 63.7
Grid 1 80.7	Grid 4 77.8	Grid 7 71.4

 Excluded sub grids
 Max remaining grid

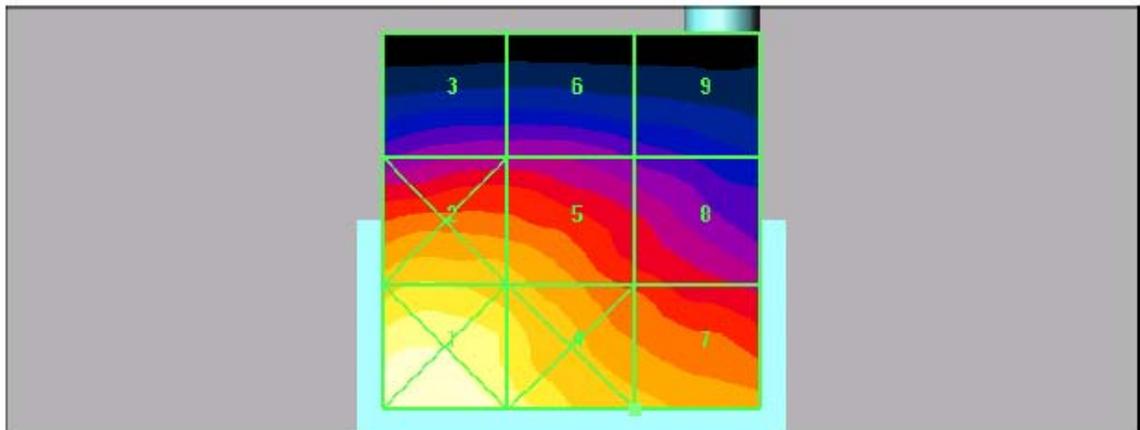

Motorola GEMS EME Laboratory
 GEMS-3; DUT: i580 H83XAH6RR4AN-Date/Time: 2/25/2006 2:37:52 PM

Run#: MeC-i580 Radio 806 E-field 060225-11
 Model# / Serial#: H83XAH6RR4AN / 364AGA0361
 TX Freq.: 806.0125 (MHz)
 Antenna: 8575868A01
 Battery# / Battery Cover#: SNN5744A / NNTN2344A

Comments:



Probe: ER3DV6 - SN2350, Calibrated: 7/7/2005, ConvF(1, 1, 1)
 Duty Cycle: 1:3, Medium: Air, Medium parameters used: $\sigma = 0$ mho/m, $\epsilon_r = 1$; $\rho = 1000$ kg/m³
 Electronics: DAE3 Sn363, Calibrated: 5/24/2005

806.0125 w/SNN5744A Battery/Hearing Aid Compatibility Test (101x101x1): Measurement grid: dx=5mm, dy=5mm
 Maximum value of peak Total field = 70.7 V/m
 Probe Modulation Factor = 1.82
 Reference Value = 35.3 V/m; Power Drift = -0.112 dB
Hearing Aid Near-Field Category: M3 (AWF 0 dB)

E-Field V/m
(Time averaged)

Grid 3 56.2	Grid 6 56.8	Grid 9 52.7
Grid 2 72.5	Grid 5 70.7	Grid 8 62.6
Grid 1 80.3	Grid 4 75.1	Grid 7 67.7

 Excluded sub grids
 Max remaining grid

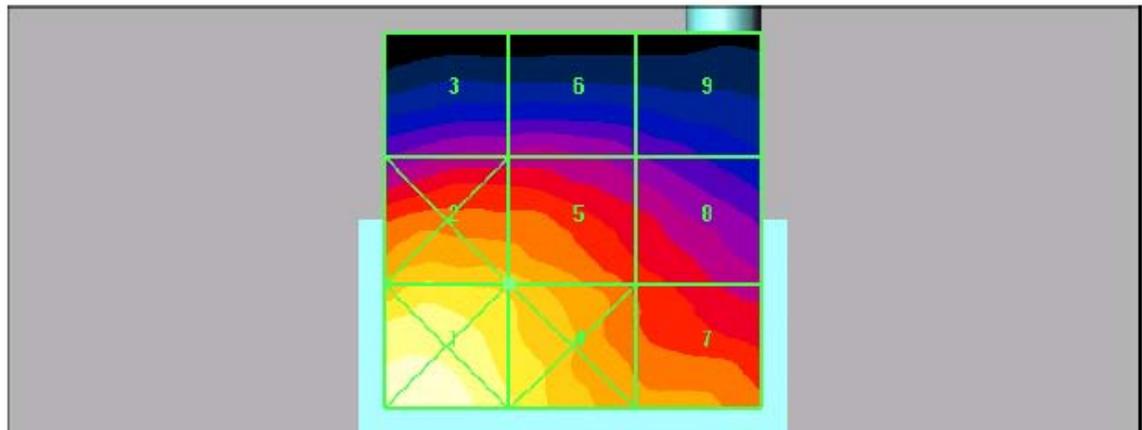

Motorola GEMS EME Laboratory
GEMS-3; DUT: i580 H83XAH6RR4AN-Date/Time: 2/25/2006 2:54:33 PM

Run#: MeC-i580 Radio 824 E-field 060225-12
 Model# / Serial#: H83XAH6RR4AN / 364AGA0361
 TX Freq.: 824.9875 (MHz)
 Antenna: 8575868A01
 Battery# / Battery Cover#: SNN5744A / NNTN2344A

Comments:


Probe: ER3DV6 - SN2350, Calibrated: 7/7/2005, ConvF(1, 1, 1)
 Duty Cycle: 1:3, Medium: Air, Medium parameters used: $\sigma = 0$ mho/m, $\epsilon_r = 1$; $\rho = 1000$ kg/m³
 Electronics: DAE3 Sn363, Calibrated: 5/24/2005

824.9875 w/SNN5744A Battery/Hearing Aid Compatibility Test (101x101x1): Measurement grid: dx=5mm, dy=5mm
 Maximum value of peak Total field = 67.3 V/m
 Probe Modulation Factor = 1.82
 Reference Value = 33.7 V/m; Power Drift = -0.120 dB
Hearing Aid Near-Field Category: M3 (AWF 0 dB)

E-Field V/m
(Time averaged)

Grid 3 52.4	Grid 6 52.1	Grid 9 48.1
Grid 2 69.3	Grid 5 67.2	Grid 8 61.6
Grid 1 79.1	Grid 4 73.5	Grid 7 67.3

 Excluded sub grids
 Max remaining grid

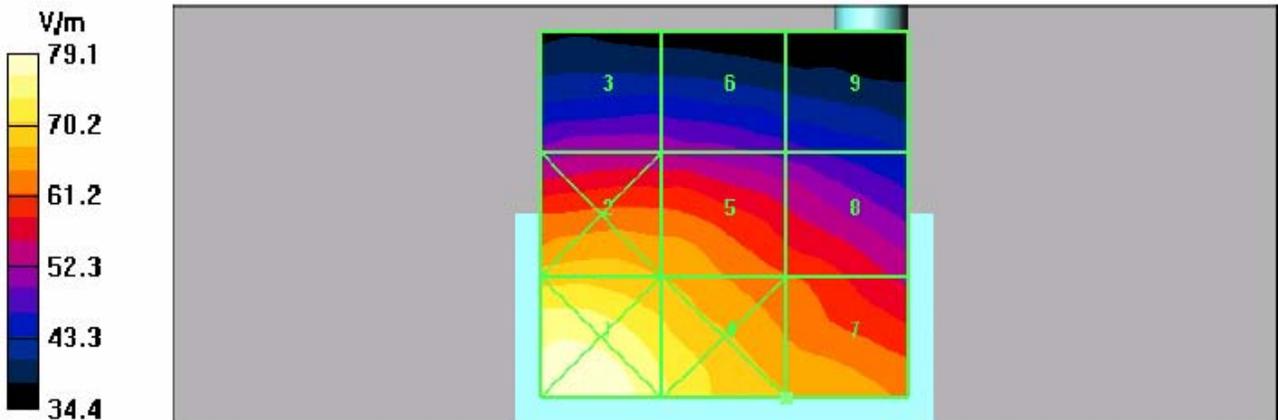

Motorola GEMS EME Laboratory
 GEMS-3; DUT: i580 H83XAH6RR4AN-Date/Time: 2/25/2006 4:33:01 PM

Run#: MeC-i580 Radio 813 H-field 060225-17
 Model# / Serial#: H83XAH6RR4AN / 364AGA0361
 TX Freq.: 813.5125 (MHz)
 Antenna: 8575868A01
 Battery# / Battery Cover#: SNN5744A / NNTN2344A

Comments:

Probe: H3DV6 - SN6166, Calibrated: 7/7/2005,
 Duty Cycle: 1:3, Medium: Air, Medium parameters used: $\sigma = 0$ mho/m, $\epsilon_r = 1$; $\rho = 1$ kg/m³
 Electronics: DAE3 Sn363, Calibrated: 5/24/2005

813.5125 w/SNN5744A Battery/Hearing Aid Compatibility Test (101x101x1): Measurement


grid: dx=5mm, dy=5mm
 Maximum value of peak Total field = 0.136 A/m
 Probe Modulation Factor = 1.81
 Reference Value = 0.067 A/m; Power Drift = -0.025 dB

Hearing Aid Near-Field Category: M4 (AWF 0 dB)

H-Field A/m
(Time averaged)

Grid 3 0.111	Grid 6 0.110	Grid 9 0.109
Grid 2 0.136	Grid 5 0.132	Grid 8 0.134
Grid 1 0.168	Grid 4 0.160	Grid 7 0.166

Excluded sub grids
 Max remaining grid

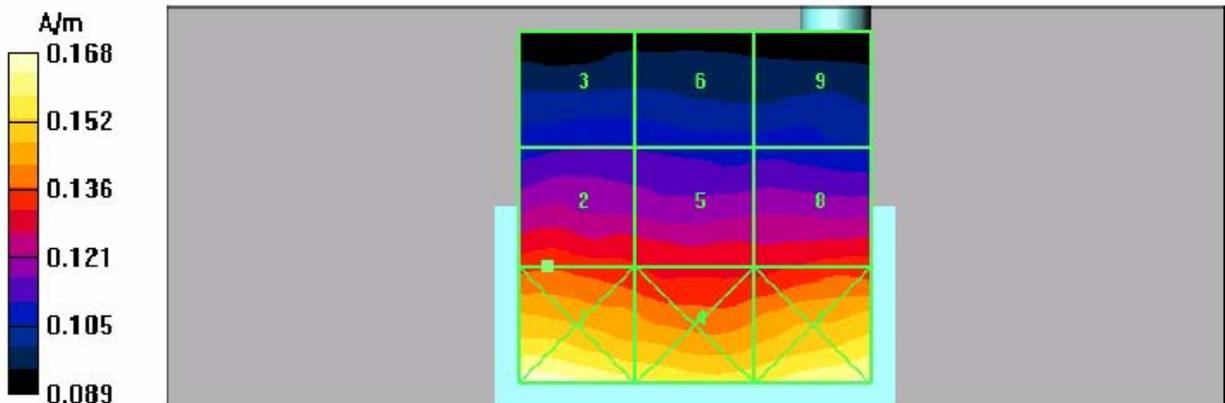

Motorola GEMS EME Laboratory
GEMS-3; DUT: i580 H83XAH6RR4AN-Date/Time: 2/25/2006 4:49:01 PM

Run#: MeC-i580 Radio 813 H-field 060225-18
 Model# / Serial#: H83XAH6RR4AN / 364AGA0361
 TX Freq.: 813.5125 (MHz)
 Antenna: 8575868A01
 Battery# / Battery Cover#: SNN5765A / NNTN2345A

Comments:


Probe: H3DV6 - SN6166, Calibrated: 7/7/2005,
 Duty Cycle: 1:3, Medium: Air, Medium parameters used: $\sigma = 0$ mho/m, $\epsilon_r = 1$; $\rho = 1$ kg/m³
 Electronics: DAE3 Sn363, Calibrated: 5/24/2005

813.5125 w/SNN5765A Battery/Hearing Aid Compatibility Test (101x101x1): Measurement grid: dx=5mm, dy=5mm
 Maximum value of peak Total field = 0.136 A/m
 Probe Modulation Factor = 1.81
 Reference Value = 0.067 A/m; Power Drift = 0.004 dB
Hearing Aid Near-Field Category: M4 (AWF 0 dB)

H-Field A/m
(Time averaged)

Grid 3 0.110	Grid 6 0.110	Grid 9 0.108
Grid 2 0.136	Grid 5 0.131	Grid 8 0.134
Grid 1 0.169	Grid 4 0.160	Grid 7 0.169

 Excluded sub grids
 Max remaining grid

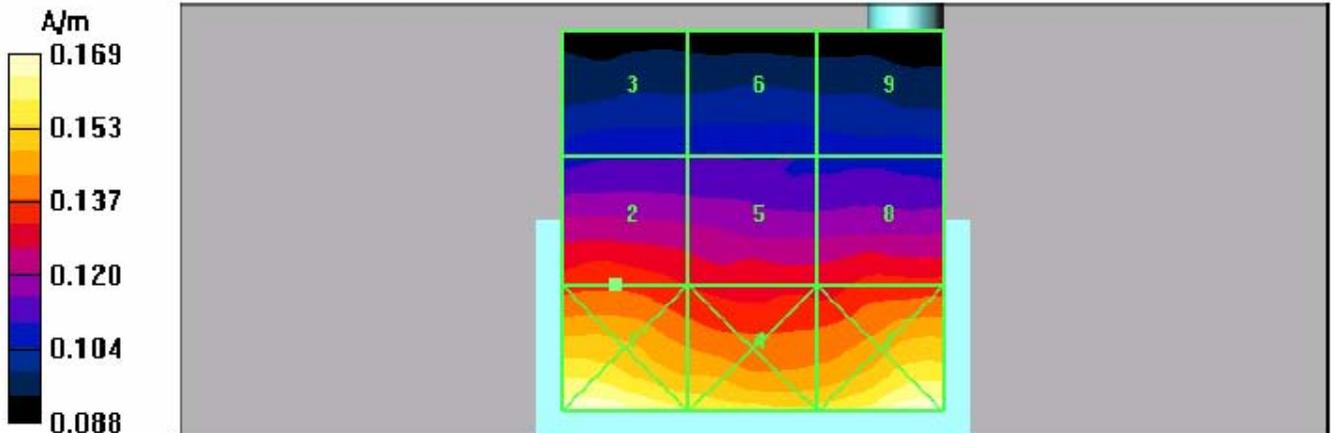

Motorola GEMS EME Laboratory
GEMS-3; DUT: i580 H83XAH6RR4AN-Date/Time: 2/25/2006 5:06:38 PM

Run#: MeC-i580 Radio 806 H-field 060225-19
 Model# / Serial#: H83XAH6RR4AN / 364AGA0361
 TX Freq.: 806.0125 (MHz)
 Antenna: 8575868A01
 Battery# / Battery Cover#: SNN5765A / NNTN2345A

Comments:


Probe: H3DV6 - SN6166, Calibrated: 7/7/2005,
 Duty Cycle: 1:3, Medium: Air, Medium parameters used: $\sigma = 0$ mho/m, $\epsilon_r = 1$; $\rho = 1$ kg/m³
 Electronics: DAE3 Sn363, Calibrated: 5/24/2005

806.0125 w/SNN5765A Battery/Hearing Aid Compatibility Test (101x101x1): Measurement grid: dx=5mm, dy=5mm
 Maximum value of peak Total field = 0.148 A/m
 Probe Modulation Factor = 1.81
 Reference Value = 0.073 A/m; Power Drift = -0.062 dB
Hearing Aid Near-Field Category: M4 (AWF 0 dB)

H-Field A/m
(Time averaged)

Grid 3 0.118	Grid 6 0.120	Grid 9 0.121
Grid 2 0.147	Grid 5 0.144	Grid 8 0.148
Grid 1 0.181	Grid 4 0.173	Grid 7 0.182

 Excluded sub grids
 Max remaining grid

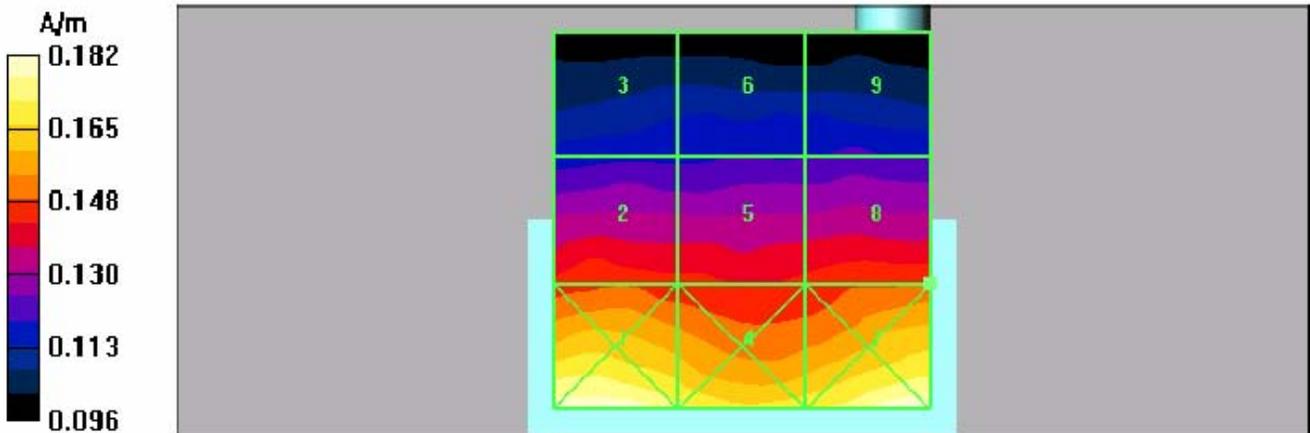


Motorola GEMS EME Laboratory
GEMS-3; DUT: i580 H83XAH6RR4AN-Date/Time: 2/25/2006 5:06:38 PM

Run#: MeC-i580 Radio 806 H-field 060225-19
Model# / Serial#: H83XAH6RR4AN / 364AGA0361
TX Freq.: 806.0125 (MHz)
Antenna: 8575868A01
Battery# / Battery Cover#: SNN5765A / NNTN2345A

Comments:

Probe: H3DV6 - SN6166, Calibrated: 7/7/2005,
Duty Cycle: 1:3, Medium: Air, Medium parameters used: $\sigma = 0$ mho/m, $\epsilon_r = 1$; $\rho = 1$ kg/m³
Electronics: DAE3 Sn363, Calibrated: 5/24/2005

806.0125 w/SNN5765A Battery/Hearing Aid Compatibility Test (101x101x1): Measurement
grid: dx=5mm, dy=5mm
Maximum value of peak Total field = 0.148 A/m
Probe Modulation Factor = 1.81
Reference Value = 0.073 A/m; Power Drift = -0.062 dB
Hearing Aid Near-Field Category: M4 (AWF 0 dB)

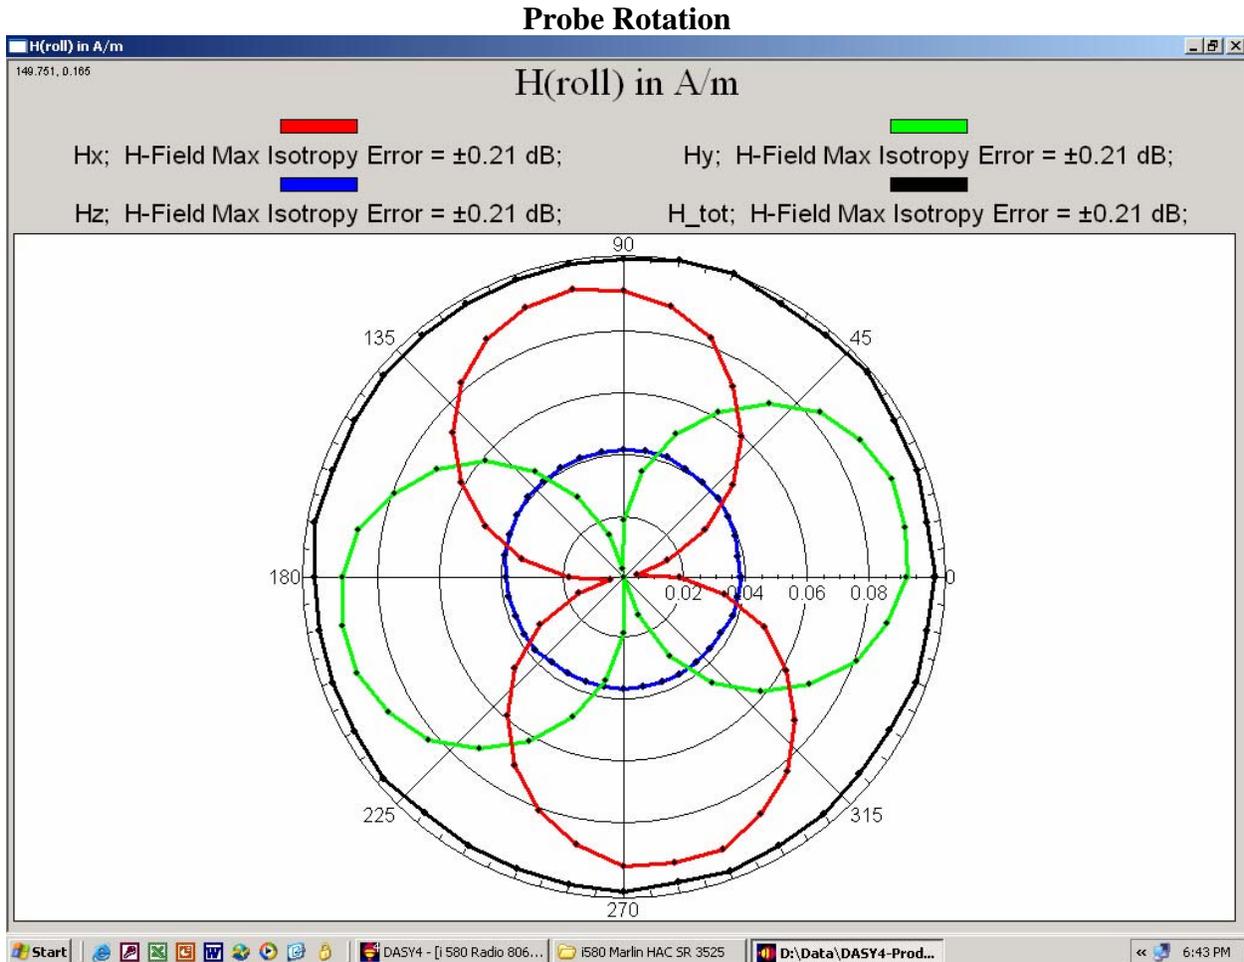

Motorola GEMS EME Laboratory
 GEMS-3; DUT: i580 H83XAH6RR4AN-Date/Time: 2/25/2006 5:23:18 PM

Run#: MeC-i580 Radio 824 H-field 060225-20
 Model# / Serial#: H83XAH6RR4AN / 364AGA0361
 TX Freq.: 824.9875 (MHz)
 Antenna: 8575868A01
 Battery# / Battery Cover#: SNN5765A / NNTN2345A

Comments:


Probe: H3DV6 - SN6166, Calibrated: 7/7/2005,
 Duty Cycle: 1:3, Medium: Air, Medium parameters used: $\sigma = 0$ mho/m, $\epsilon_r = 1$; $\rho = 1$ kg/m³
 Electronics: DAE3 Sn363, Calibrated: 5/24/2005

824.9875 w/SNN5765A Battery/Hearing Aid Compatibility Test (101x101x1): Measurement grid: dx=5mm, dy=5mm
 Maximum value of peak Total field = 0.140 A/m
 Probe Modulation Factor = 1.81
 Reference Value = 0.066 A/m; Power Drift = -0.039 dB
Hearing Aid Near-Field Category: M4 (AWF 0 dB)

H-Field A/m
(Time averaged)

Grid 3 0.111	Grid 6 0.109	Grid 9 0.107
Grid 2 0.140	Grid 5 0.133	Grid 8 0.133
Grid 1 0.176	Grid 4 0.166	Grid 7 0.170

 Excluded sub grids
 Max remaining grid

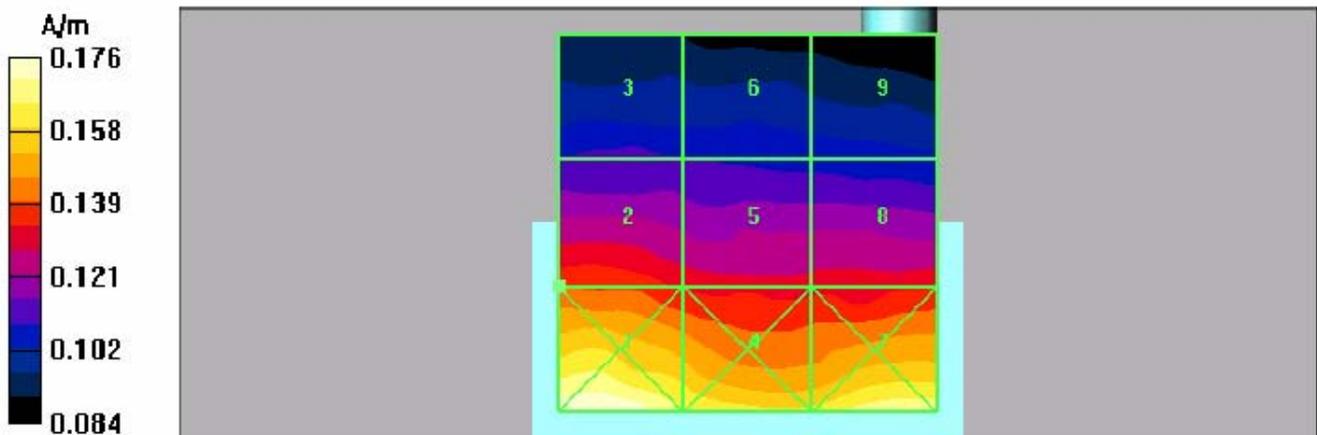

Motorola GEMS EME Laboratory
GEMS-3; DUT: i580 H83XAH6RR4AN-Date/Time: 2/25/2006 3:15:04 PM

Run#: MeC-i580 Radio 898 E-field 060225-13
 Model# / Serial#: H83XAH6RR4AN / 364AGA0361
 TX Freq.: 898.5187 (MHz)
 Antenna: 8575868A01
 Battery# / Battery Cover#: SNN5744A / NNTN2344A

Comments:



Probe: ER3DV6 - SN2350, Calibrated: 7/7/2005, ConvF(1, 1, 1)
 Duty Cycle: 1:3, Medium: Air, Medium parameters used: $\sigma = 0$ mho/m, $\epsilon_r = 1$; $\rho = 1000$ kg/m³
 Electronics: DAE3 Sn363, Calibrated: 5/24/2005

898.5187 w/SNN5744A Battery/Hearing Aid Compatibility Test (101x101x1): Measurement grid: dx=5mm, dy=5mm
 Maximum value of peak Total field = 45.8 V/m
 Probe Modulation Factor = 1.79
 Reference Value = 21.6 V/m; Power Drift = -0.109 dB
Hearing Aid Near-Field Category: M4 (AWF 0 dB)

E-Field V/m
(Time averaged)

Grid 3 34.8	Grid 6 35.0	Grid 9 34.2
Grid 2 45.8	Grid 5 44.1	Grid 8 39.5
Grid 1 56.3	Grid 4 53.6	Grid 7 47.3

 Excluded sub grids
 Max remaining grid

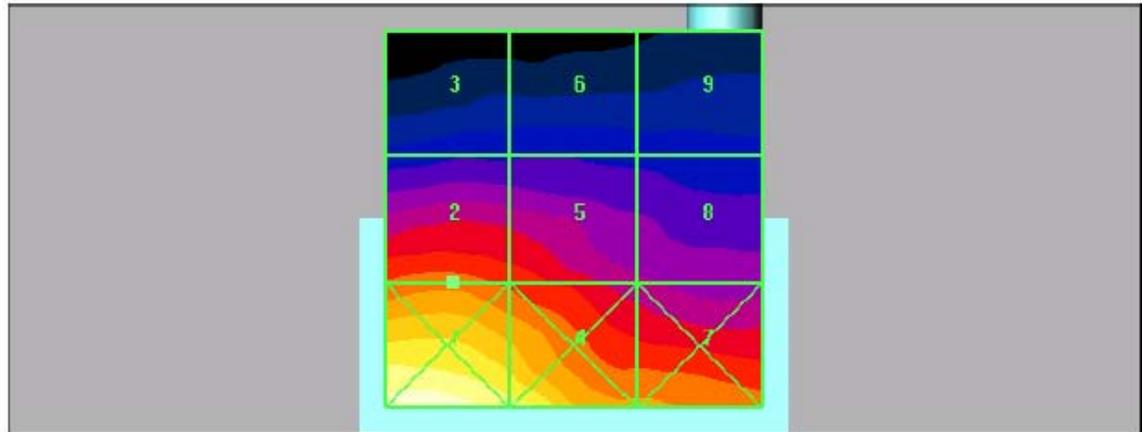

Motorola GEMS EME Laboratory
 GEMS-3; DUT: i580 H83XAH6RR4AN-Date/Time: 2/25/2006 3:31:23 PM

Run#: MeC-i580 Radio 898 E-field 060225-14
 Model# / Serial#: H83XAH6RR4AN / 364AGA0361
 TX Freq.: 898.5187 (MHz)
 Antenna: 8575868A01
 Battery# / Battery Cover#: SNN5765A / NNTN2345A

Comments:

Probe: ER3DV6 - SN2350, Calibrated: 7/7/2005, ConvF(1, 1, 1)
 Duty Cycle: 1:3, Medium: Air, Medium parameters used: $\sigma = 0$ mho/m, $\epsilon_r = 1$; $\rho = 1000$ kg/m³
 Electronics: DAE3 Sn363, Calibrated: 5/24/2005

898.5187 w/SNN5765A Battery/Hearing Aid Compatibility Test (101x101x1): Measurement grid: dx=5mm, dy=5mm


Maximum value of peak Total field = 47.2 V/m
 Probe Modulation Factor = 1.79
 Reference Value = 21.9 V/m; Power Drift = -0.053 dB

Hearing Aid Near-Field Category: M4 (AWF 0 dB)

E-Field V/m
(Time averaged)

Grid 3 36.5	Grid 6 36.1	Grid 9 34.3
Grid 2 47.2	Grid 5 44.7	Grid 8 40.1
Grid 1 56.7	Grid 4 54.8	Grid 7 48.1

 Excluded sub grids
 Max remaining grid

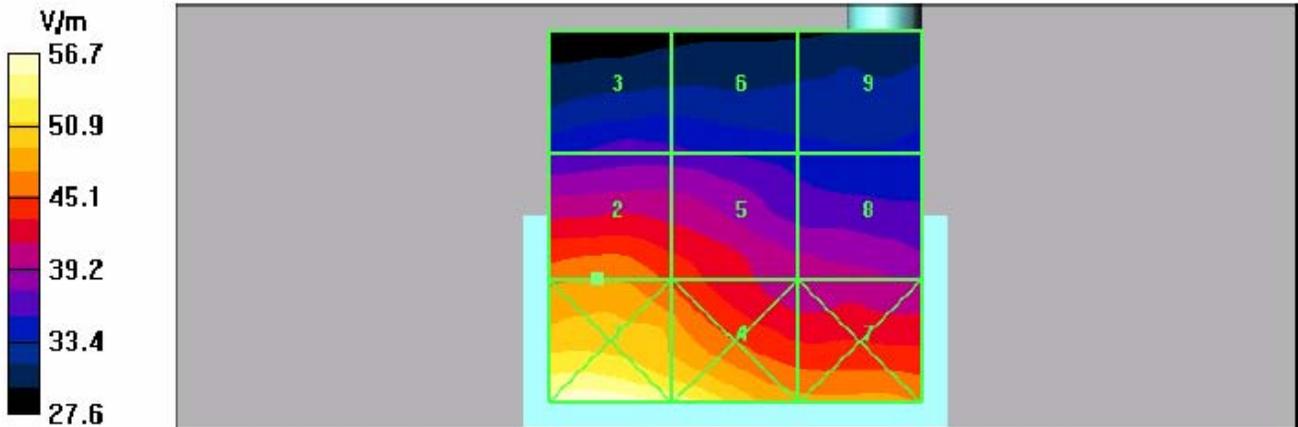

Motorola GEMS EME Laboratory
GEMS-3; DUT: i580 H83XAH6RR4AN-Date/Time: 2/25/2006 3:54:33 PM

Run#: MeC-i580 Radio 896 E-field 060225-15
 Model# / Serial#: H83XAH6RR4AN / 364AGA0361
 TX Freq.: 896.0187 (MHz)
 Antenna: 8575868A01
 Battery# / Battery Cover#: SNN5765A / NNTN2345A

Comments:

Probe: ER3DV6 - SN2350, Calibrated: 7/7/2005, ConvF(1, 1, 1)
 Duty Cycle: 1:3, Medium: Air, Medium parameters used: $\sigma = 0$ mho/m, $\epsilon_r = 1$; $\rho = 1000$ kg/m³
 Electronics: DAE3 Sn363, Calibrated: 5/24/2005

896.0187 w/SNN5765A Battery/Hearing Aid Compatibility Test (101x101x1): Measurement



grid: dx=5mm, dy=5mm
 Maximum value of peak Total field = 46.3 V/m
 Probe Modulation Factor = 1.79
 Reference Value = 21.7 V/m; Power Drift = -0.103 dB

Hearing Aid Near-Field Category: M4 (AWF 0 dB)

E-Field V/m
(Time averaged)

Grid 3 36	Grid 6 36.1	Grid 9 34.7
Grid 2 46.6	Grid 5 43.9	Grid 8 39.7
Grid 1 54.9	Grid 4 50.5	Grid 7 46.3

 Excluded sub grids
 Max remaining grid

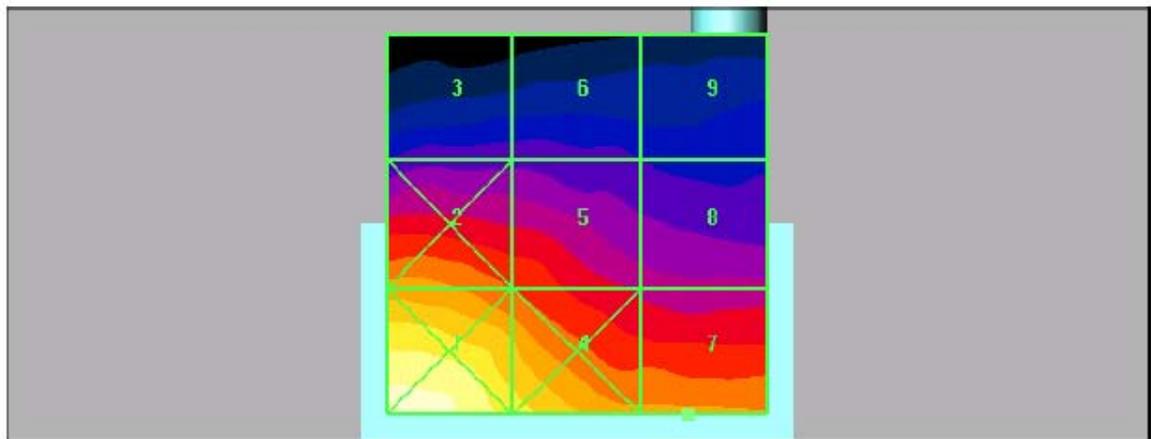

Motorola GEMS EME Laboratory
GEMS-3; DUT: i580 H83XAH6RR4AN-Date/Time: 2/25/2006 4:13:40 PM

Run#: MeC-i580 Radio 900 E-field 060225-16
 Model# / Serial#: H83XAH6RR4AN / 364AGA0361
 TX Freq.: 900.9812 (MHz)
 Antenna: 8575868A01
 Battery# / Battery Cover#: SNN5765A / NNTN2345A

Comments:


Probe: ER3DV6 - SN2350, Calibrated: 7/7/2005, ConvF(1, 1, 1)
 Duty Cycle: 1:3, Medium: Air, Medium parameters used: $\sigma = 0$ mho/m, $\epsilon_r = 1$; $\rho = 1000$ kg/m³
 Electronics: DAE3 Sn363, Calibrated: 5/24/2005

900.9812 w/SNN5765A Battery/Hearing Aid Compatibility Test (101x101x1): Measurement grid: dx=5mm, dy=5mm
 Maximum value of peak Total field = 47.8 V/m
 Probe Modulation Factor = 1.79
 Reference Value = 21.8 V/m; Power Drift = -0.117 dB
Hearing Aid Near-Field Category: M4 (AWF 0 dB)

E-Field V/m
(Time averaged)

Grid 3 36.1	Grid 6 36.0	Grid 9 35.1
Grid 2 47.8	Grid 5 45.7	Grid 8 40.6
Grid 1 57.8	Grid 4 55.7	Grid 7 48.0

 Excluded sub grids
 Max remaining grid

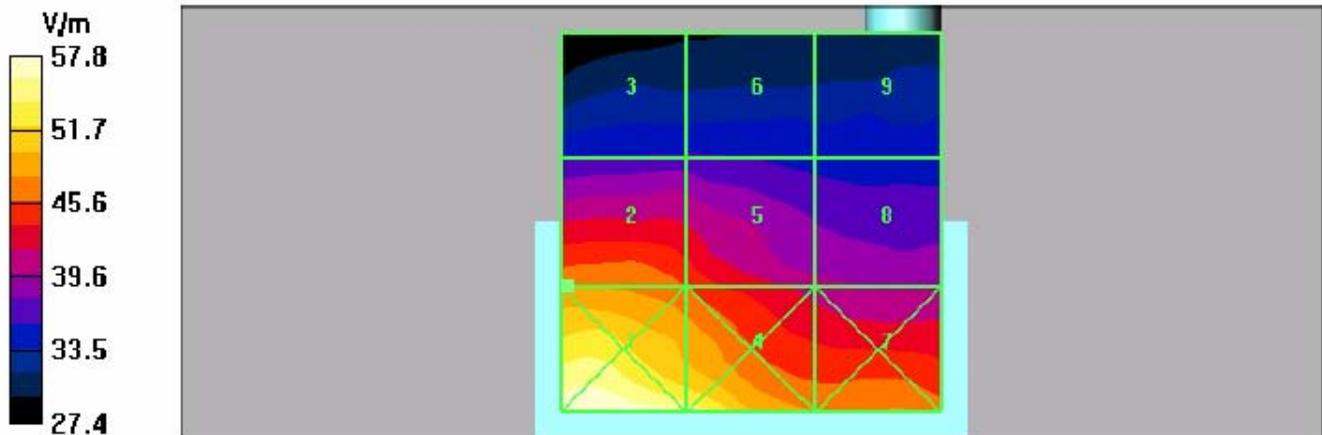

Motorola GEMS EME Laboratory
GEMS-3; DUT: i580 H83XAH6RR4AN-Date/Time: 2/25/2006 5:39:08 PM

Run#: MeC-i580 Radio 898 H-field 060225-21
 Model# / Serial#: H83XAH6RR4AN / 364AGA0361
 TX Freq.: 898.5187 (MHz)
 Antenna: 8575868A01
 Battery# / Battery Cover#: SNN5744A / NNTN2344A

Comments:

Probe: H3DV6 - SN6166, Calibrated: 7/7/2005,
 Duty Cycle: 1:3, Medium: Air, Medium parameters used: $\sigma = 0$ mho/m, $\epsilon_r = 1$; $\rho = 1$ kg/m³
 Electronics: DAE3 Sn363, Calibrated: 5/24/2005

898.5187 w/SNN5744A Battery/Hearing Aid Compatibility Test (101x101x1): Measurement grid: dx=5mm, dy=5mm

Maximum value of peak Total field = 0.108 A/m

Probe Modulation Factor = 1.78


Reference Value = 0.054 A/m; Power Drift = -0.079 dB

Hearing Aid Near-Field Category: M4 (AWF 0 dB)

H-Field A/m
(Time averaged)

Grid 3 0.092	Grid 6 0.090	Grid 9 0.087
Grid 2 0.108	Grid 5 0.103	Grid 8 0.107
Grid 1 0.130	Grid 4 0.124	Grid 7 0.135

- Excluded sub grids
- Max remaining grid

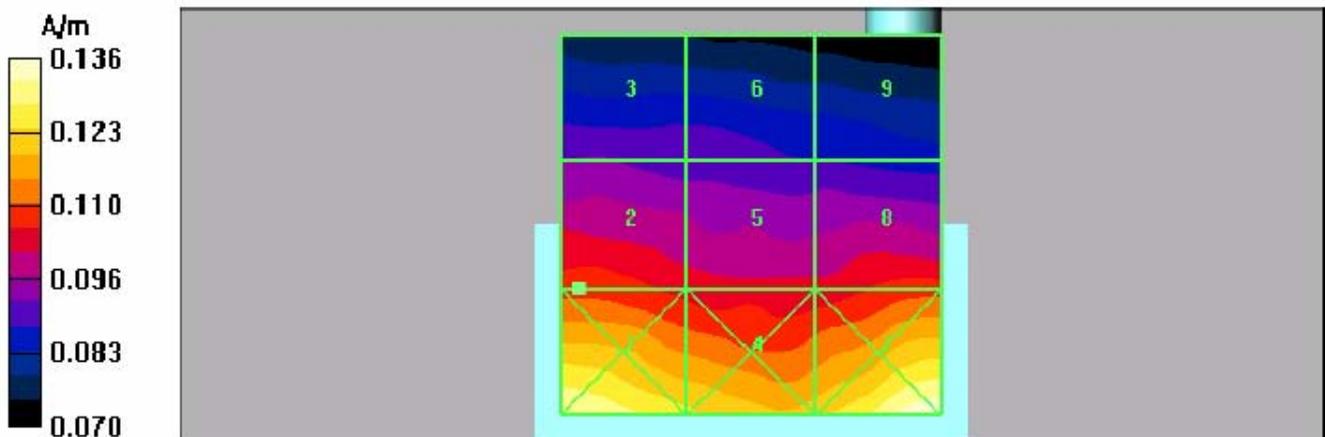

Motorola GEMS EME Laboratory
GEMS-3; DUT: i580 H83XAH6RR4AN-Date/Time: 2/25/2006 5:56:45 PM

Run#: MeC-i580 Radio 898 H-field 060225-22
 Model# / Serial#: H83XAH6RR4AN / 364AGA0361
 TX Freq.: 898.5187 (MHz)
 Antenna: 8575868A01
 Battery# / Battery Cover#: SNN5765A / NNTN2345A

Comments:

Probe: H3DV6 - SN6166, Calibrated: 7/7/2005,
 Duty Cycle: 1:3, Medium: Air, Medium parameters used: $\sigma = 0$ mho/m, $\epsilon_r = 1$; $\rho = 1$ kg/m³
 Electronics: DAE3 Sn363, Calibrated: 5/24/2005

898.5187 w/SNN5765A Battery/Hearing Aid Compatibility Test (101x101x1): Measurement grid: dx=5mm, dy=5mm


Maximum value of peak Total field = 0.108 A/m
 Probe Modulation Factor = 1.78
 Reference Value = 0.053 A/m; Power Drift = 0.079 dB

Hearing Aid Near-Field Category: M4 (AWF 0 dB)

H-Field A/m
(Time averaged)

Grid 3 0.090	Grid 6 0.090	Grid 9 0.088
Grid 2 0.108	Grid 5 0.105	Grid 8 0.106
Grid 1 0.129	Grid 4 0.123	Grid 7 0.132

 Excluded sub grids
 Max remaining grid

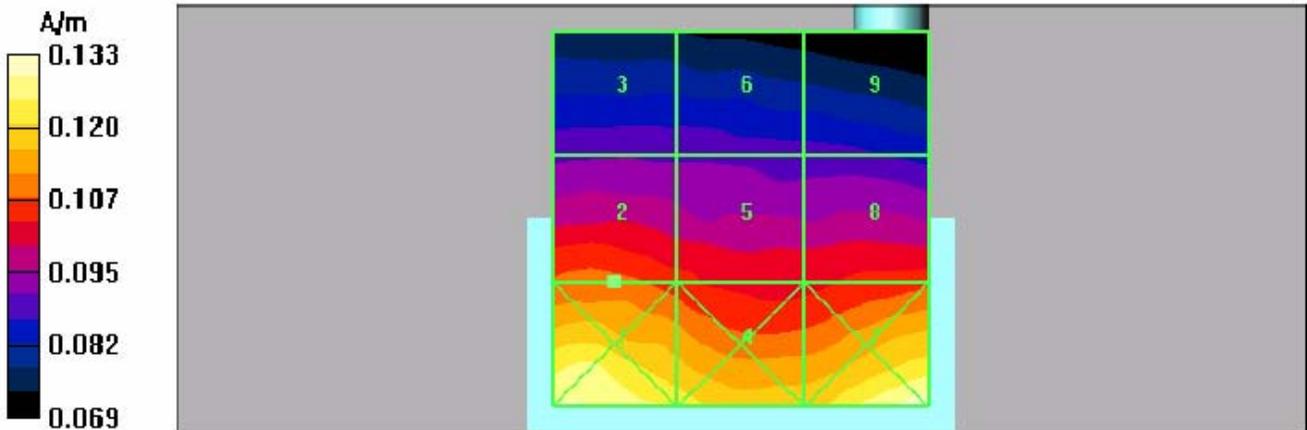

Motorola GEMS EME Laboratory
 GEMS-3; DUT: i580 H83XAH6RR4AN-Date/Time: 2/25/2006 6:13:58 PM

Run#: MeC-i580 Radio 896 H-field 060225-23
 Model# / Serial#: H83XAH6RR4AN / 364AGA0361
 TX Freq.: 896.0187 (MHz)
 Antenna: 8575868A01
 Battery# / Battery Cover#: SNN5765A / NNTN2345A

Comments:

Probe: H3DV6 - SN6166, Calibrated: 7/7/2005,
 Duty Cycle: 1:3, Medium: Air, Medium parameters used: $\sigma = 0$ mho/m, $\epsilon_r = 1$; $\rho = 1$ kg/m³
 Electronics: DAE3 Sn363, Calibrated: 5/24/2005

896.0187 w/SNN5765A Battery/Hearing Aid Compatibility Test (101x101x1): Measurement grid: dx=5mm, dy=5mm



Maximum value of peak Total field = 0.112 A/m
 Probe Modulation Factor = 1.78
 Reference Value = 0.055 A/m; Power Drift = -0.321 dB

Hearing Aid Near-Field Category: M4 (AWF 0 dB)

**H-Field A/m
 (Time averaged)**

Grid 3 0.090	Grid 6 0.090	Grid 9 0.087
Grid 2 0.112	Grid 5 0.107	Grid 8 0.108
Grid 1 0.131	Grid 4 0.125	Grid 7 0.135

 Excluded sub grids
 Max remaining grid

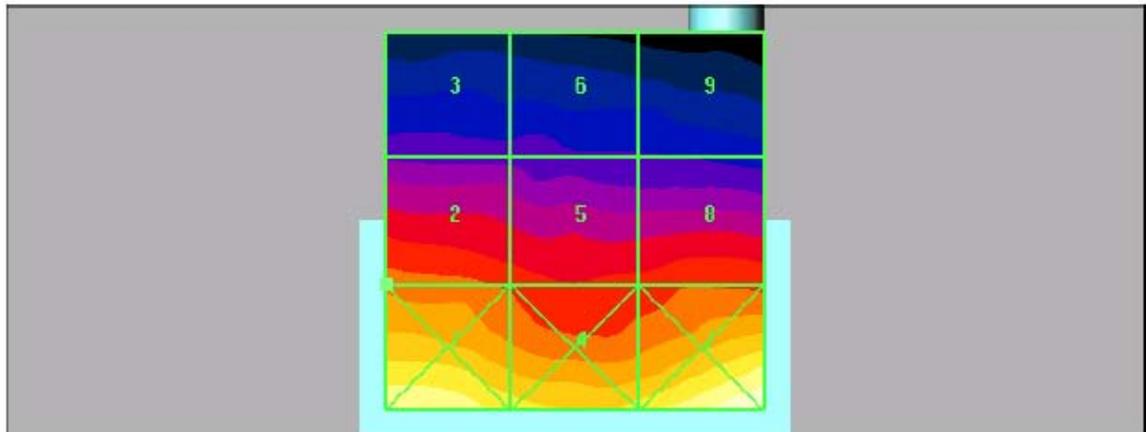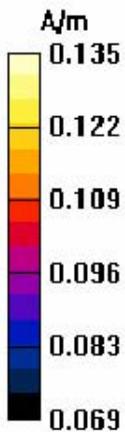

Motorola GEMS EME Laboratory
GEMS-3; DUT: i580 H83XAH6RR4AN-Date/Time: 2/25/2006 6:30:35 PM

Run#: MeC-i580 Radio 900 H-field 060225-24
 Model# / Serial#: H83XAH6RR4AN / 364AGA0361
 TX Freq.: 900.9812 (MHz)
 Antenna: 8575868A01
 Battery# / Battery Cover#: SNN5765A / NNTN2345A

Comments:


Probe: H3DV6 - SN6166, Calibrated: 7/7/2005,
 Duty Cycle: 1:3, Medium: Air, Medium parameters used: $\sigma = 0$ mho/m, $\epsilon_r = 1$; $\rho = 1$ kg/m³
 Electronics: DAE3 Sn363, Calibrated: 5/24/2005

900.9812 w/SNN5765A Battery/Hearing Aid Compatibility Test (101x101x1): Measurement grid: dx=5mm, dy=5mm
 Maximum value of peak Total field = 0.111 A/m
 Probe Modulation Factor = 1.78
 Reference Value = 0.054 A/m; Power Drift = 0.036 dB
Hearing Aid Near-Field Category: M4 (AWF 0 dB)

H-Field A/m
(Time averaged)

Grid 3 0.093	Grid 6 0.092	Grid 9 0.092
Grid 2 0.108	Grid 5 0.105	Grid 8 0.111
Grid 1 0.131	Grid 4 0.126	Grid 7 0.14

 Excluded sub grids
 Max remaining grid

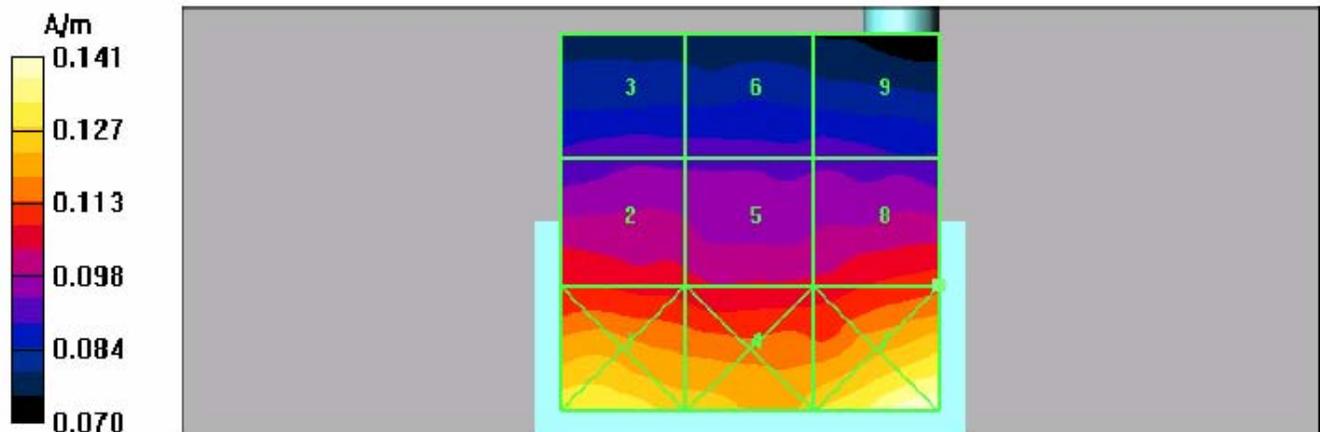

Appendix C
Probe Calibration Certificates

**Calibration Laboratory of
Schmid & Partner
Engineering AG**
Zeughausstrasse 43, 8004 Zurich, Switzerland



S Schweizerischer Kalibrierdienst
C Service suisse d'étalonnage
S Servizio svizzero di taratura
S Swiss Calibration Service

Accredited by the Swiss Federal Office of Metrology and Accreditation
The Swiss Accreditation Service is one of the signatories to the EA
Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: **SCS 108**

Client **Motorola**

Certificate No: **ER3-2350_Jul05**

CALIBRATION CERTIFICATE

Object **ER3DV6 - SN:2350**

Calibration procedure(s) **QA CAL-02.v4
Calibration procedure for E-field probes optimized for close near field
evaluations in air**

Calibration date: **July 7, 2005**

Condition of the calibrated item **In Tolerance**

This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI).
The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility: environment temperature (22 ± 3)°C and humidity < 70%.

Calibration Equipment used (M&TE critical for calibration)

Primary Standards	ID #	Cal Date (Calibrated by, Certificate No.)	Scheduled Calibration
Power meter E4419B	GB41293874	3-May-05 (METAS, No. 251-00466)	May-06
Power sensor E4412A	MY41495277	3-May-05 (METAS, No. 251-00466)	May-06
Power sensor E4412A	MY41498087	3-May-05 (METAS, No. 251-00466)	May-06
Reference 3 dB Attenuator	SN: S5054 (3c)	10-Aug-04 (METAS, No. 251-00403)	Aug-05
Reference 20 dB Attenuator	SN: S5086 (20b)	3-May-05 (METAS, No. 251-00467)	May-06
Reference 30 dB Attenuator	SN: S5129 (30b)	10-Aug-04 (METAS, No. 251-00404)	Aug-05
Reference Probe ER3DV6	SN: 2328	6-Oct-04 (SPEAG, No. ER3-2328_Oct04)	Oct-05
DAE4	SN: 617	19-Jan-05 (SPEAG, No. DAE4-617_Jan05)	Jan-06

Secondary Standards	ID #	Check Date (in house)	Scheduled Check
RF generator HP 8648C	US3642U01700	4-Aug-99 (SPEAG, in house check Dec-03)	In house check: Dec-05
Network Analyzer HP 8753E	US37390585	18-Oct-01 (SPEAG, in house check Nov-04)	In house check: Nov 05

	Name	Function	Signature
Calibrated by:	Katja Pokovic	Technical Manager	
Approved by:	Niels Kuster	Quality Manager	

Issued: July 22, 2005

This calibration certificate shall not be reproduced except in full without written approval of the laboratory.

Calibration Laboratory of
Schmid & Partner
Engineering AG
Zeughausstrasse 43, 8004 Zurich, Switzerland



S Schweizerischer Kalibrierdienst
C Service suisse d'étalonnage
S Servizio svizzero di taratura
S Swiss Calibration Service

Accredited by the Swiss Federal Office of Metrology and Accreditation
The Swiss Accreditation Service is one of the signatories to the EA
Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: **SCS 108**

Glossary:

NORM _{x,y,z}	sensitivity in free space
DCP	diode compression point
Polarization φ	φ rotation around probe axis
Polarization ϑ	ϑ rotation around an axis that is in the plane normal to probe axis (at measurement center), i.e., $\vartheta = 0$ is normal to probe axis
Connector Angle	information used in DASY system to align probe sensor X to the robot coordinate system

Calibration is Performed According to the Following Standards:

- a) IEEE Std 1309-1996, "IEEE Standard for calibration of electromagnetic field sensors and probes, excluding antennas, from 9 kHz to 40 GHz", 1996.

Methods Applied and Interpretation of Parameters:

- *NORM_{x,y,z}*: Assessed for E-field polarization $\vartheta = 0$ for XY sensors and $\vartheta = 90$ for Z sensor ($f \leq 900$ MHz in TEM-cell; $f > 1800$ MHz: R22 waveguide).
- *NORM(f)_{x,y,z}* = *NORM_{x,y,z}* * *frequency_response* (see Frequency Response Chart).
- *DCP_{x,y,z}*: DCP are numerical linearization parameters assessed based on the data of power sweep (no uncertainty required). DCP does not depend on frequency.
- *Spherical isotropy (3D deviation from isotropy)*: in a locally homogeneous field realized using an open waveguide setup.
- *Sensor Offset*: The sensor offset corresponds to the offset of virtual measurement center from the probe tip (on probe axis). No tolerance required.
- *Connector Angle*: The angle is assessed using the information gained by determining the *NORM_x* (no uncertainty required).

ER3DV6 SN:2350

July 7, 2005

Probe ER3DV6

SN:2350

Manufactured:	March 8, 2005
Calibrated:	July 7, 2005

Calibrated for DASY Systems

(Note: non-compatible with DASY2 system!)

ER3DV6 SN:2350

July 7, 2005

DASY - Parameters of Probe: ER3DV6 SN:2350

Sensitivity in Free Space [$\mu\text{V}/(\text{V}/\text{m})^2$]		Diode Compression ^A	
NormX	1.77 ± 10.1 % (k=2)	DCP X	94 mV
NormY	1.61 ± 10.1 % (k=2)	DCP Y	94 mV
NormZ	1.57 ± 10.1 % (k=2)	DCP Z	96 mV

Frequency Correction

X	0.0
Y	0.0
Z	0.0

Sensor Offset (Probe Tip to Sensor Center)

X	2.5 mm
Y	2.5 mm
Z	2.5 mm


Connector Angle 261 °

The reported uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor k=2, which for a normal distribution corresponds to a coverage probability of approximately 95%.

^A numerical linearization parameter: uncertainty not required



Frequency Response of E-Field

(TEM-Cell:ifi110 EXX, Waveguide R22)


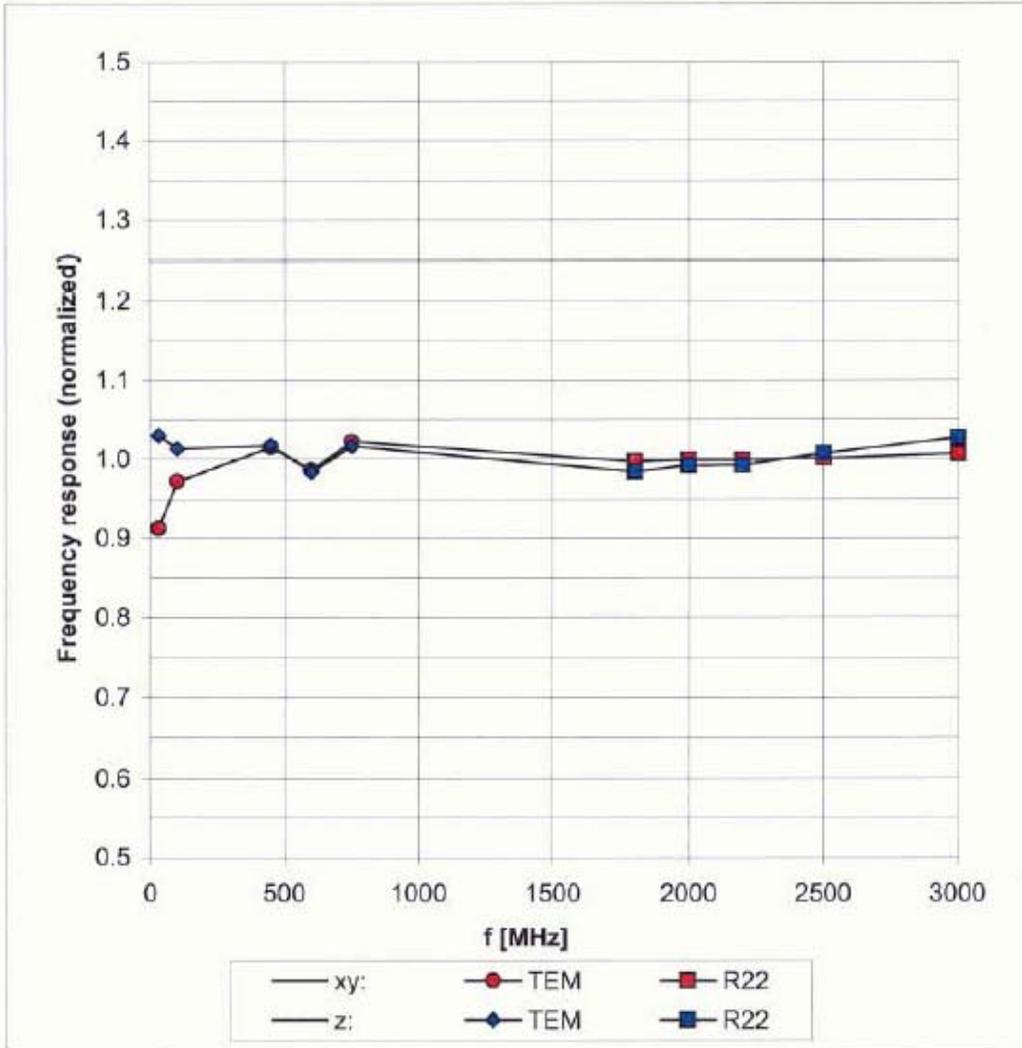


Uncertainty of Frequency Response of E-field: $\pm 6.3\%$ ($k=2$)


Receiving Pattern (ϕ), $\vartheta = 0^\circ$

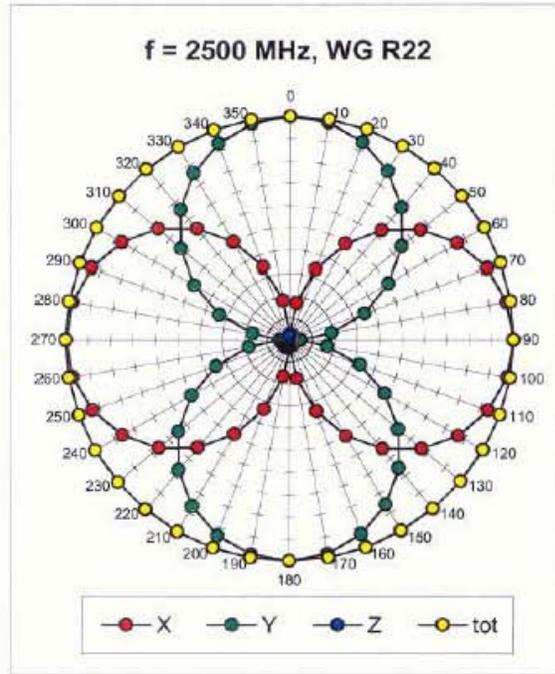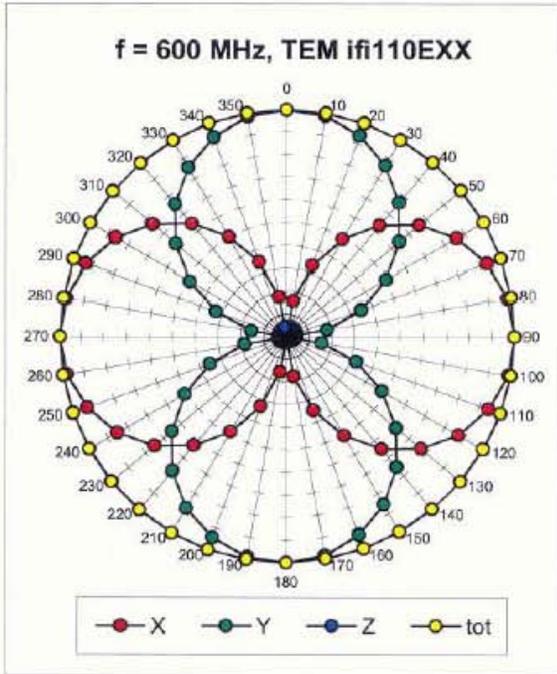

Receiving Pattern (ϕ), $\vartheta = 90^\circ$

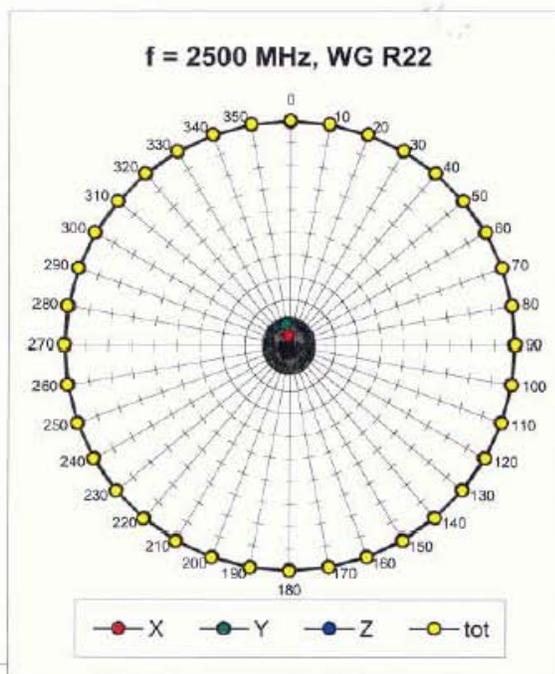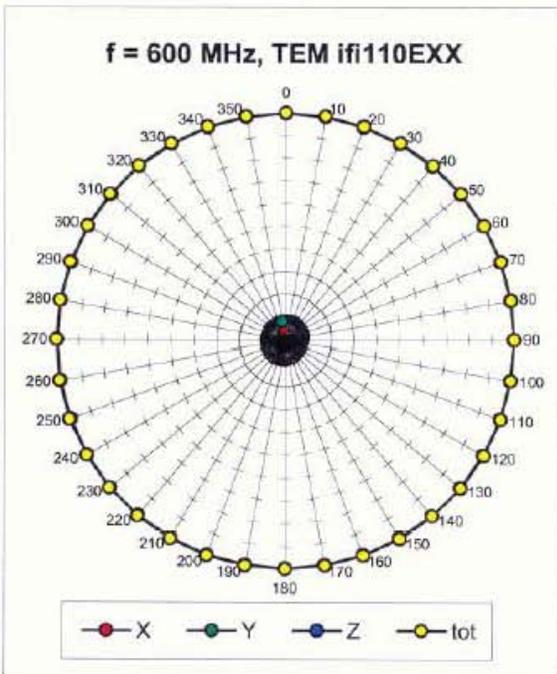


Receiving Pattern (ϕ), $\vartheta = 0^\circ$

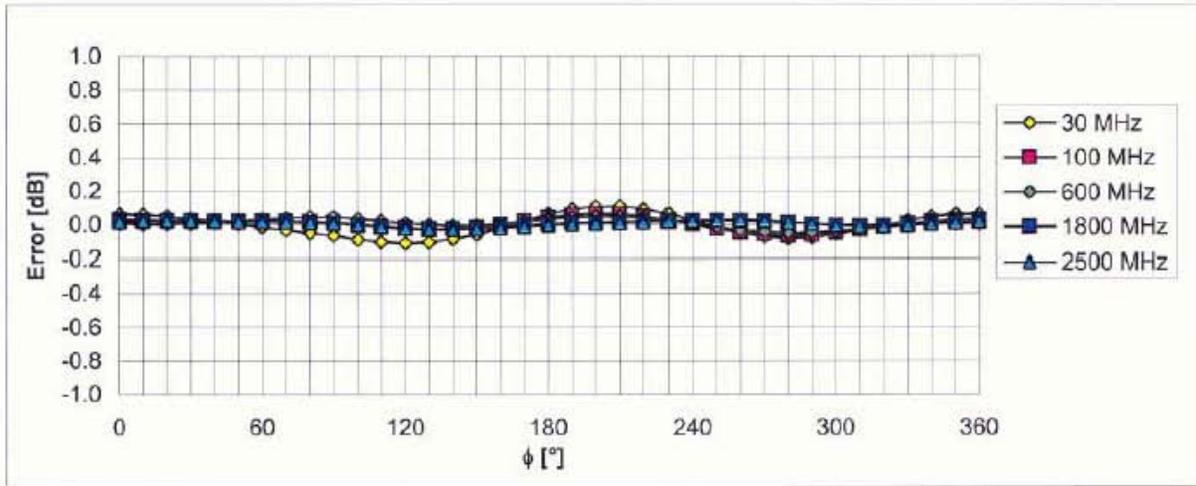



Uncertainty of Axial Isotropy Assessment: $\pm 0.5\%$ ($k=2$)

Receiving Pattern (ϕ), $\vartheta = 90^\circ$

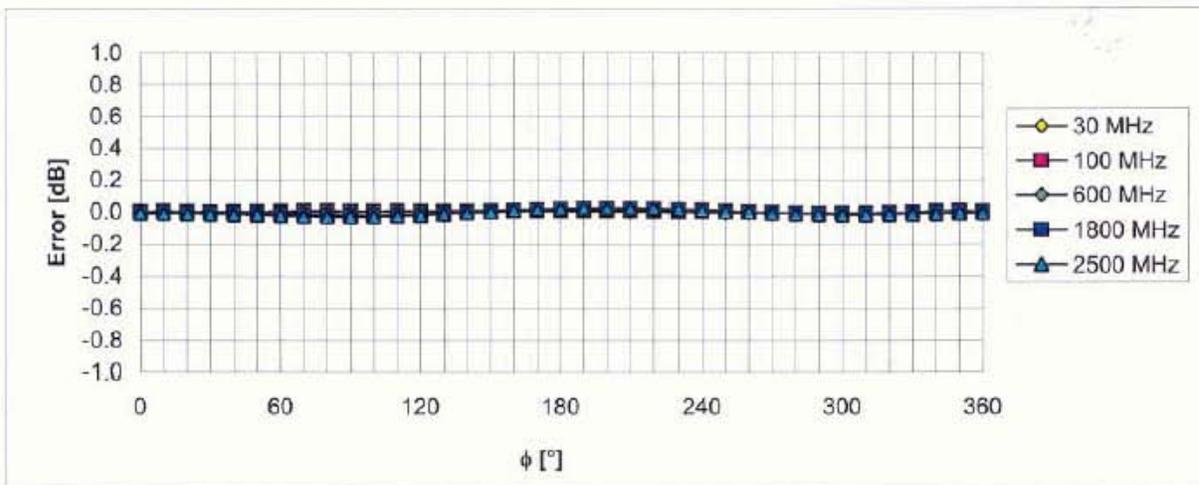


Uncertainty of Axial Isotropy Assessment: $\pm 0.5\%$ ($k=2$)

Dynamic Range f(E-field) (Waveguide R22, f = 1800 MHz)

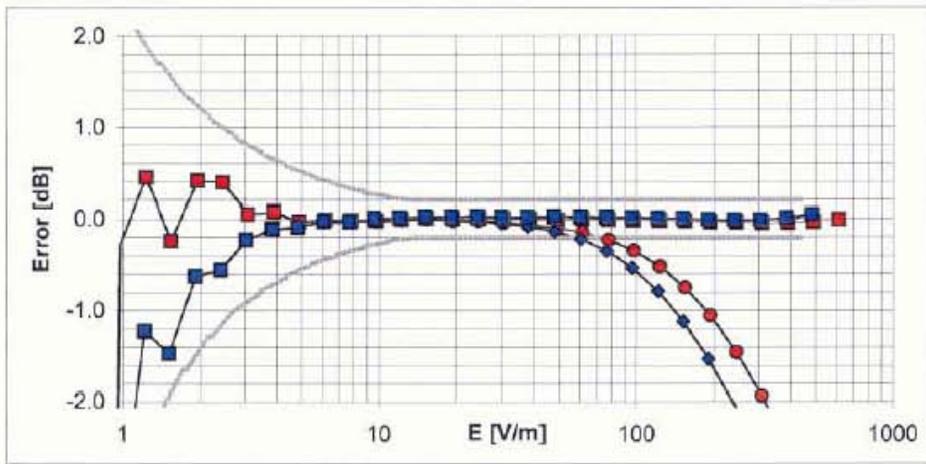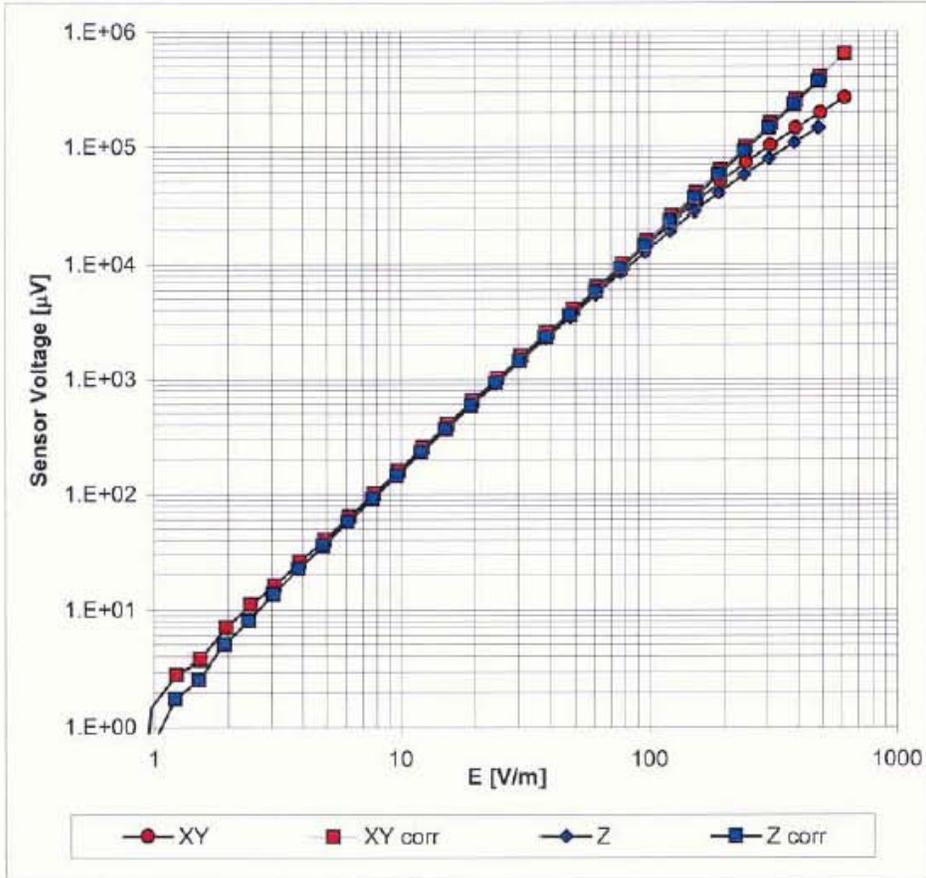

Uncertainty of Linearity Assessment: $\pm 0.6\%$ ($k=2$)

Deviation from Isotropy in Air Error (ϕ, ϑ), $f = 900$ MHz

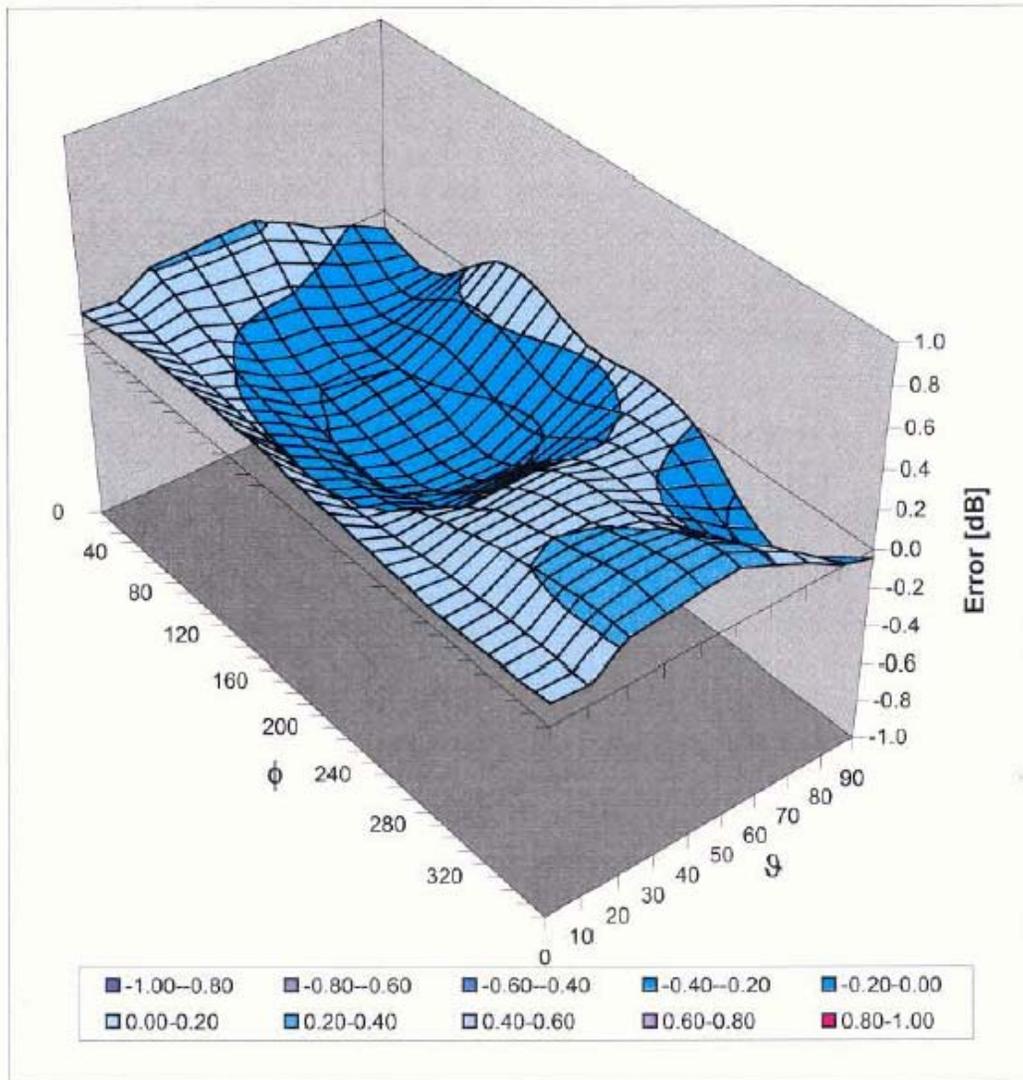

Uncertainty of Spherical Isotropy Assessment: $\pm 2.6\%$ ($k=2$)

**Calibration Laboratory of
Schmid & Partner
Engineering AG**
Zeughausstrasse 43, 8004 Zurich, Switzerland



S Schweizerischer Kalibrierdienst
C Service suisse d'étalonnage
S Servizio svizzero di taratura
S Swiss Calibration Service

Accredited by the Swiss Federal Office of Metrology and Accreditation
The Swiss Accreditation Service is one of the signatories to the EA
Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: **SCS 108**

Client **Motorola**

Certificate No: **H3-6166_Jul05**

CALIBRATION CERTIFICATE

Object **H3DV6 - SN:6166**

Calibration procedure(s) **QA CAL-03.v4
Calibration procedure for H-field probes optimized for close near field
evaluations in air**

Calibration date: **July 7, 2005**

Condition of the calibrated item **In Tolerance**

This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI).
The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility: environment temperature (22 ± 3)°C and humidity < 70%.

Calibration Equipment used (M&TE critical for calibration)

Primary Standards	ID #	Cal Date (Calibrated by, Certificate No.)	Scheduled Calibration
Power meter E4419B	GB41293874	3-May-05 (METAS, No. 251-00466)	May-06
Power sensor E4412A	MY41495277	3-May-05 (METAS, No. 251-00466)	May-06
Power sensor E4412A	MY41498087	3-May-05 (METAS, No. 251-00466)	May-06
Reference 3 dB Attenuator	SN: S5054 (3c)	10-Aug-04 (METAS, No. 251-00403)	Aug-05
Reference 20 dB Attenuator	SN: S5086 (20b)	3-May-05 (METAS, No. 251-00467)	May-06
Reference 30 dB Attenuator	SN: S5129 (30b)	10-Aug-04 (METAS, No. 251-00404)	Aug-05
Reference Probe H3DV6	SN: 6182	6-Oct-04 (SPEAG, No. H3-6182_Oct04)	Oct-05
DAE4	SN: 617	19-Jan-05 (SPEAG, No. DAE4-617_Jan05)	Jan-06

Secondary Standards	ID #	Check Date (in house)	Scheduled Check
RF generator HP 8648C	US3642U01700	4-Aug-99 (SPEAG, in house check Dec-03)	In house check: Dec-05
Network Analyzer HP 8753E	US37390585	18-Oct-01 (SPEAG, in house check Nov-04)	In house check: Nov 05

	Name	Function	Signature
Calibrated by:	Katja Pokovic	Technical Manager	
Approved by:	Niels Kuster	Quality Manager	

Issued: July 22, 2005

This calibration certificate shall not be reproduced except in full without written approval of the laboratory.

**Calibration Laboratory of
Schmid & Partner
Engineering AG**
Zeughausstrasse 43, 8004 Zurich, Switzerland



S Schweizerischer Kalibrierdienst
C Service suisse d'étalonnage
S Servizio svizzero di taratura
S Swiss Calibration Service

Accredited by the Swiss Federal Office of Metrology and Accreditation
The Swiss Accreditation Service is one of the signatories to the EA
Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: **SCS 108**

Glossary:

NORM _{x,y,z}	sensitivity in free space
DCP	diode compression point
Polarization φ	φ rotation around probe axis
Polarization ϑ	ϑ rotation around an axis that is in the plane normal to probe axis (at measurement center), i.e., $\vartheta = 0$ is normal to probe axis
Connector Angle	information used in DASY system to align probe sensor X to the robot coordinate system

Calibration is Performed According to the Following Standards:

- a) IEEE Std 1309-1996, " IEEE Standard for calibration of electromagnetic field sensors and probes, excluding antennas, from 9 kHz to 40 GHz", 1996.

Methods Applied and Interpretation of Parameters:

- X, Y, Z_{a0a1a2} : Assessed for E-field polarization $\vartheta = 90$ for XY sensors and $\vartheta = 0$ for Z sensor ($f \leq 900$ MHz in TEM-cell; $f > 1800$ MHz: R22 waveguide).
- $X, Y, Z(f)_{a0a1a2} = X, Y, Z_{a0a1a2} * frequency_response$ (see Frequency Response Chart).
- $DCP_{x,y,z}$: DCP are numerical linearization parameters assessed based on the data of power sweep (no uncertainty required). DCP does not depend on frequency.
- *Spherical isotropy (3D deviation from isotropy)*: in a locally homogeneous field realized using an open waveguide setup.
- *Sensor Offset*: The sensor offset corresponds to the offset of virtual measurement center from the probe tip (on probe axis). No tolerance required.
- *Connector Angle*: The angle is assessed using the information gained by determining the X_{a0a1a2} (no uncertainty required).

H3DV6 SN:6166

July 7, 2005

Probe H3DV6

SN:6166

Manufactured:	May 19, 2005
Calibrated:	July 7, 2005

Calibrated for DASY Systems

(Note: non-compatible with DASY2 system!)

H3DV6 SN:6166

July 7, 2005

DASY - Parameters of Probe: H3DV6 SN:6166

Sensitivity in Free Space [A/m / $\sqrt{\mu\text{V}}$]

	a0	a1	a2
X	2.535E-03	5.193E-5	-8.930E-6 ± 5.1 % (k=2)
Y	2.538E-03	5.837E-7	9.973E-6 ± 5.1 % (k=2)
Z	2.997E-03	-5.464E-5	3.814E-5 ± 5.1 % (k=2)

Diode Compression¹

DCP X	86 mV
DCP Y	86 mV
DCP Z	86 mV

Sensor Offset (Probe Tip to Sensor Center)

X	3.0 mm
Y	3.0 mm
Z	3.0 mm


Connector Angle 186 °

The reported uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor k=2, which for a normal distribution corresponds to a coverage probability of approximately 95%.

¹ numerical linearization parameter; uncertainty not required



Frequency Response of H-Field

(TEM-Cell:ifi110, Waveguide R22)


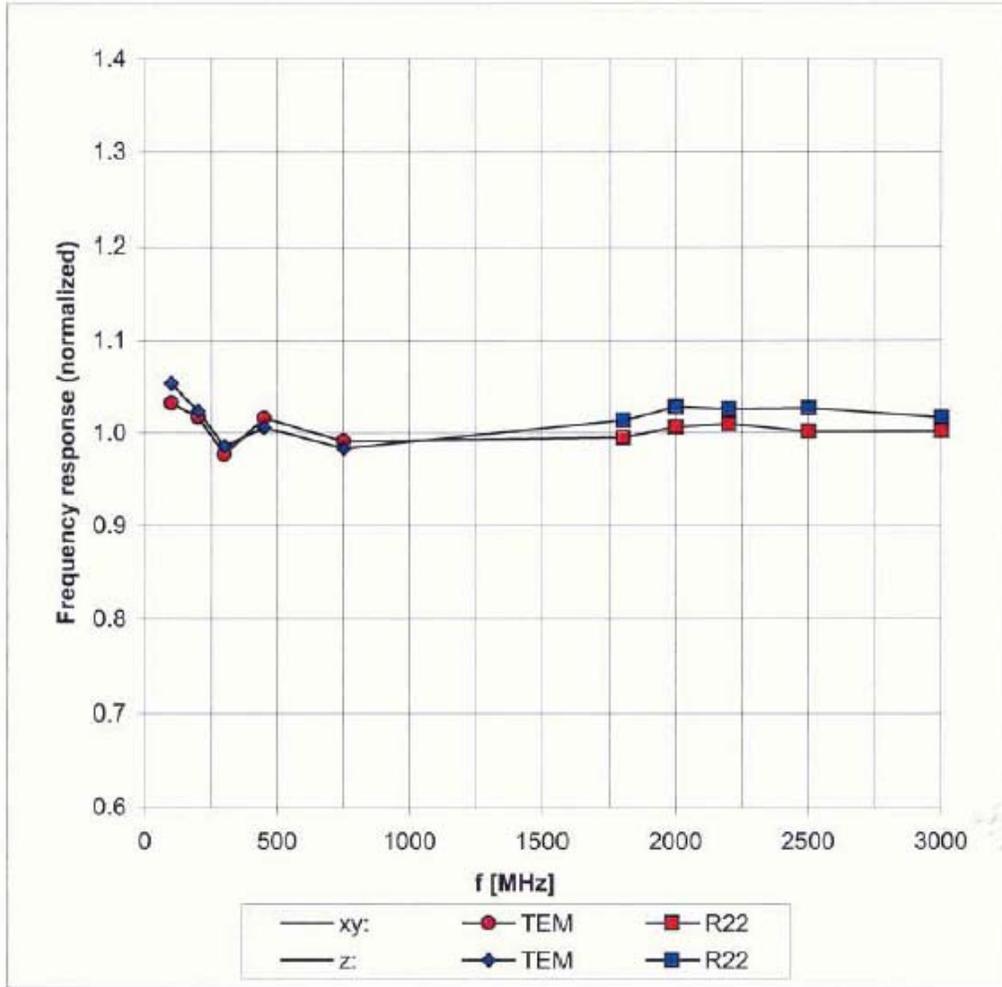


Uncertainty of Frequency Response of E-field: $\pm 6.3\%$ (k=2)


Receiving Pattern (ϕ), $\vartheta = 90^\circ$

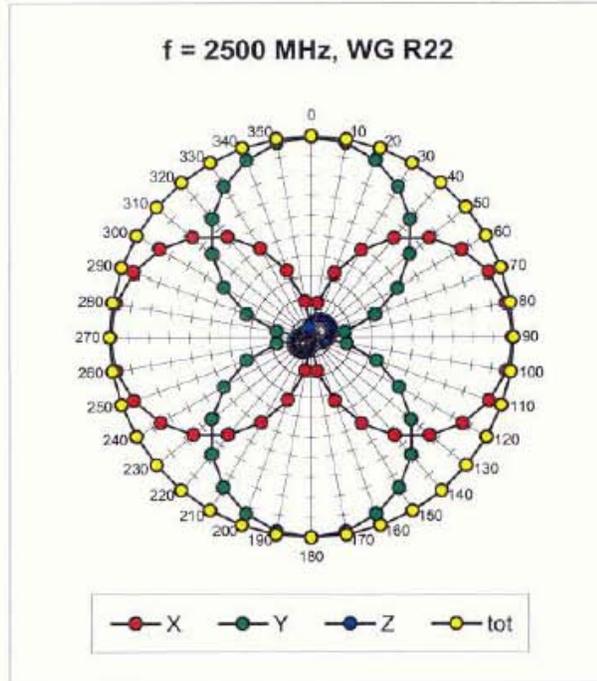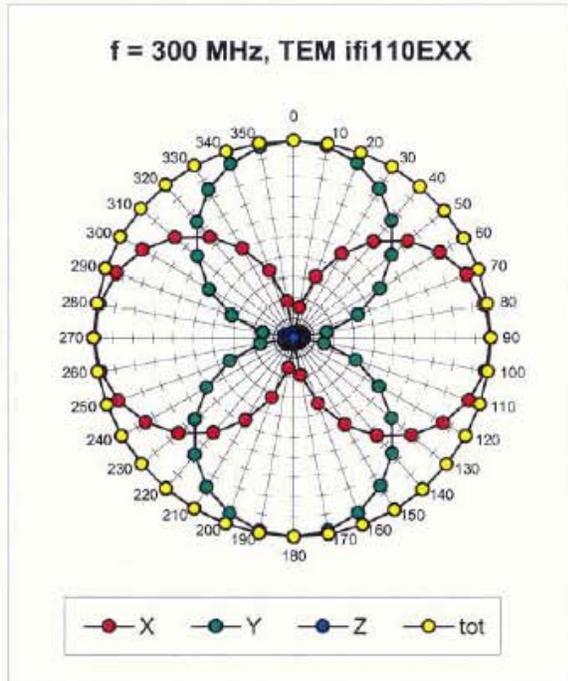

Receiving Pattern (ϕ), $\vartheta = 0^\circ$

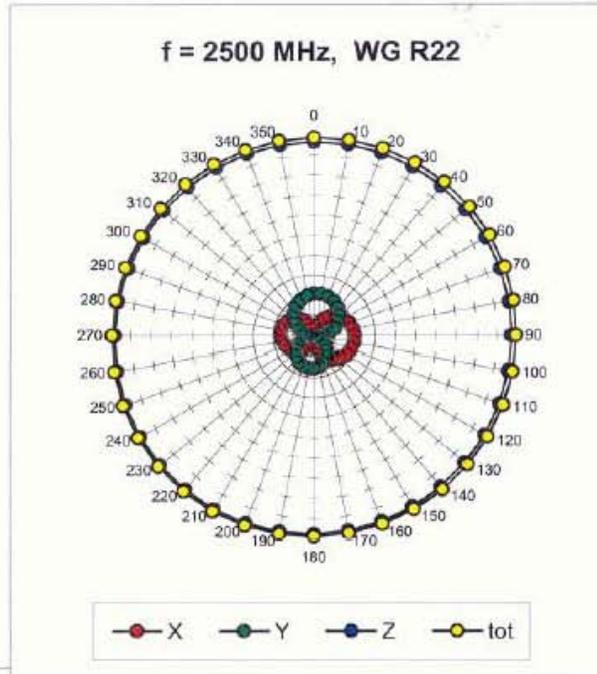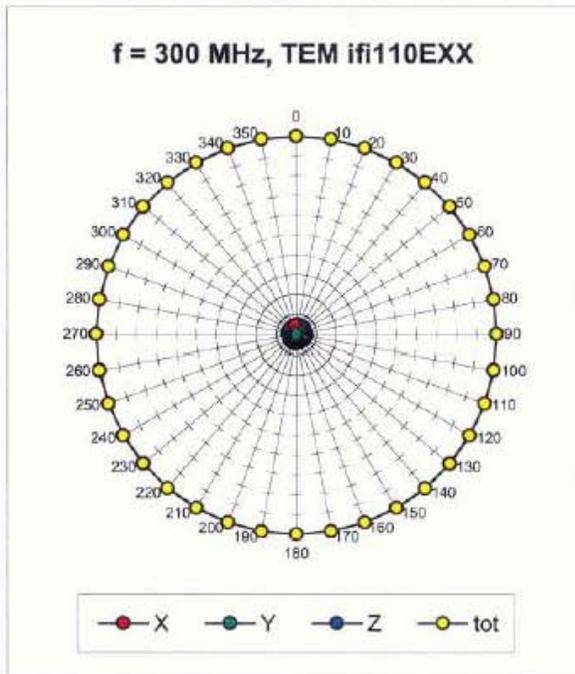


Receiving Pattern (ϕ), $\vartheta = 90^\circ$

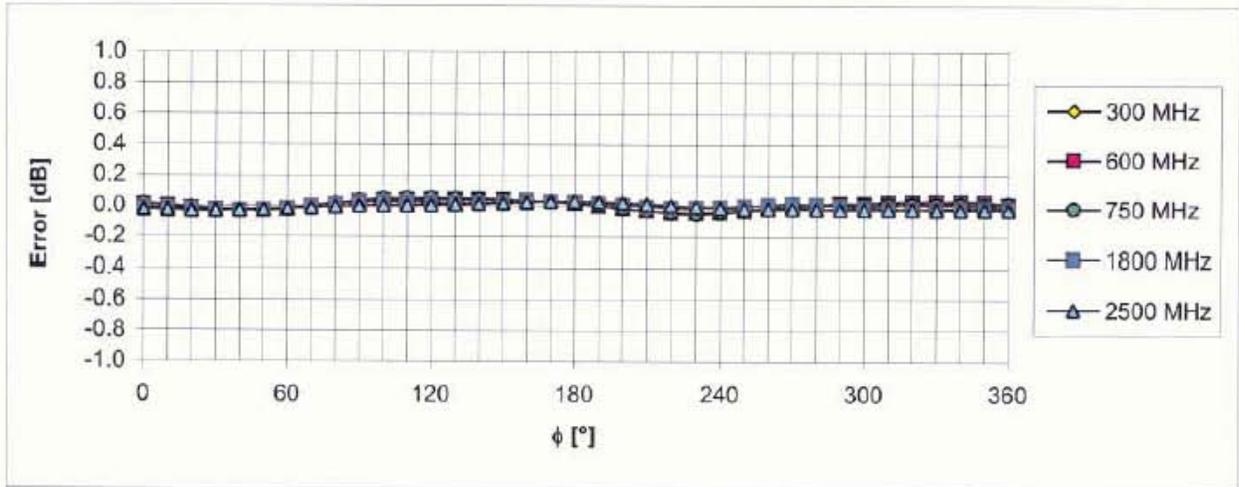



Uncertainty of Axial Isotropy Assessment: $\pm 0.5\%$ (k=2)

Receiving Pattern (ϕ), $\vartheta = 0^\circ$

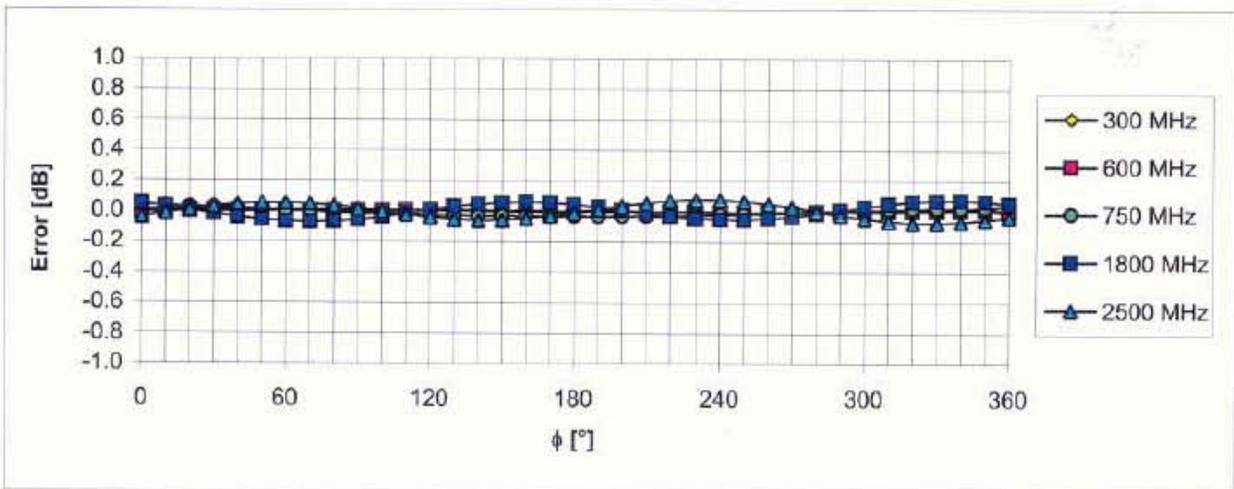

Uncertainty of Axial Isotropy Assessment: $\pm 0.5\%$ (k=2)

Dynamic Range f(H-field) (Waveguide R22, f = 1800 MHz)

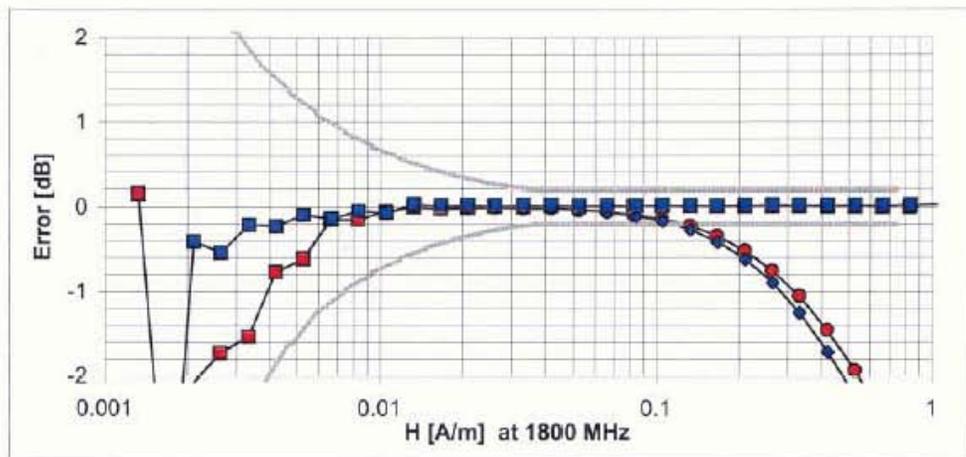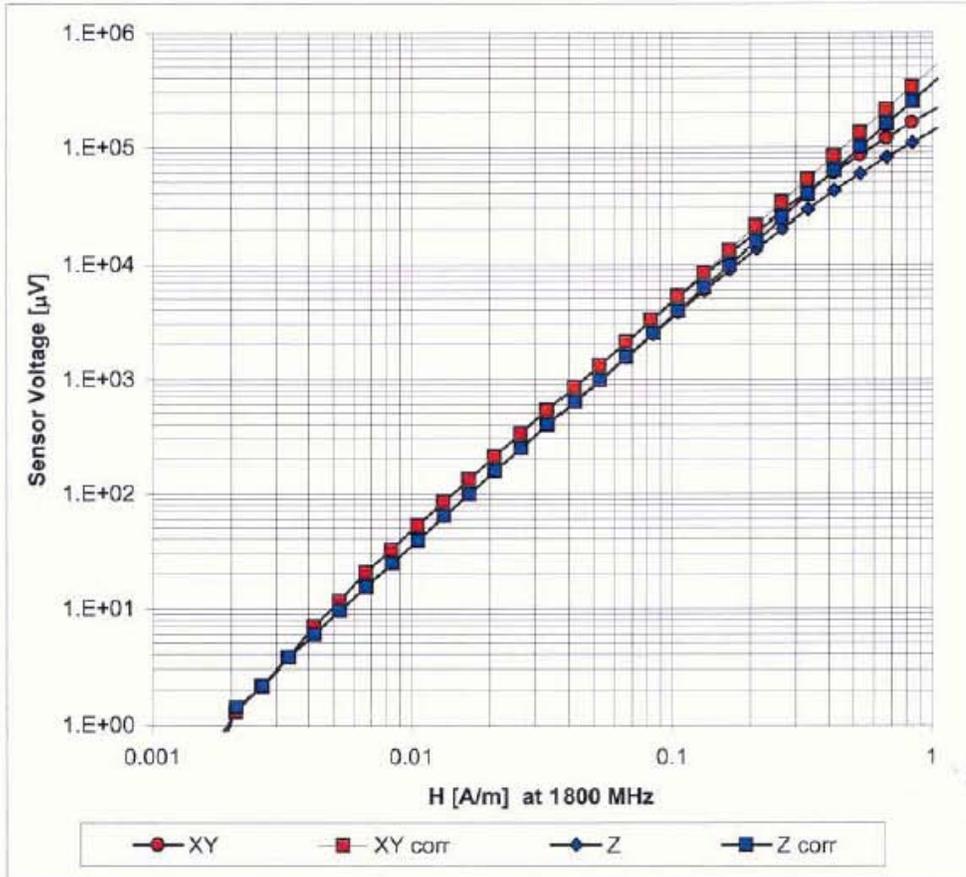

Uncertainty of Linearity Assessment: $\pm 0.6\%$ ($k=2$)


Appendix D

Details of Automated Scanning Method and Computations (Inserts from DASY 4 User Manual)

Chapter 11

System Description and Setup

11.1 System Description

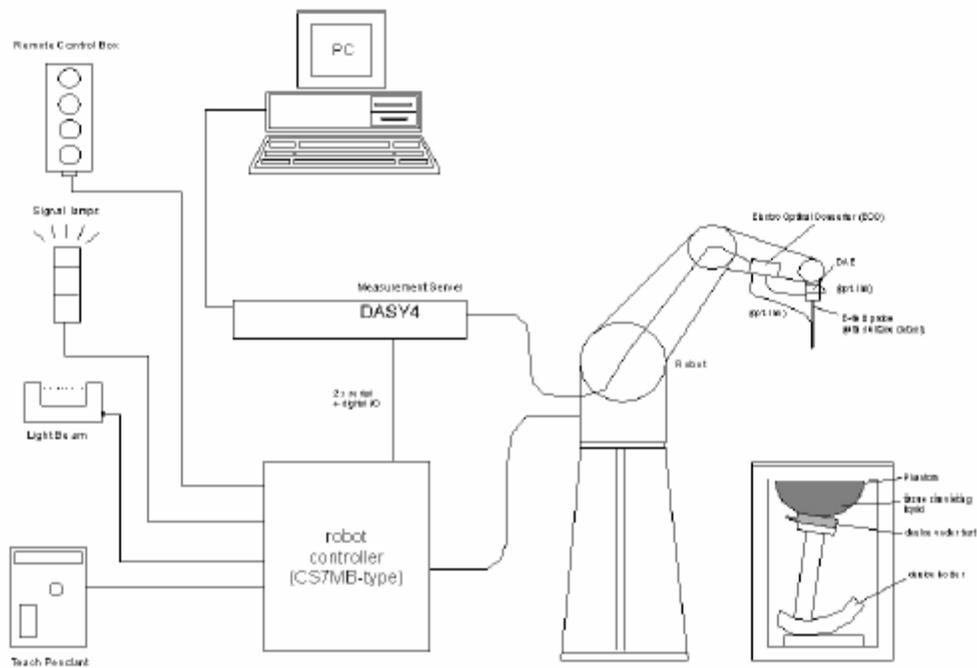

The DASy4 system for performing compliance tests consists of the following items:

- A standard high precision 6-axis robot (Stäubli RX family) with controller, teach pendant and software. An arm extension for accommodating the data acquisition electronics (DAE).
- A dosimetric probe, i.e., an isotropic E-field probe optimized and calibrated for usage in tissue simulating liquid. The probe is equipped with an optical surface detector system.
- A data acquisition electronics (DAE) which performs the signal amplification, signal multiplexing, AD-conversion, offset measurements, mechanical surface detection, collision detection, etc. The unit is battery powered with standard or rechargeable batteries. The signal is optically transmitted to the EOC.

- The Electro-optical converter (EOC) performs the conversion between optical and electrical of the signals for the digital communication to the DAE and for the analog signal from the optical surface detection. The EOC is connected to the measurement server.
- The function of the measurement server is to perform the time critical tasks such as signal filtering, control of the robot operation and fast movement interrupts.
- A probe alignment unit which improves the (absolute) accuracy of the probe positioning.
- A computer operating Windows 2000 or Windows XP.
- DASY4 software.
- Remote control with teach pendant and additional circuitry for robot safety such as warning lamps, etc.
- The SAM twin phantom enabling testing left-hand and right-hand usage.
- The device holder for handheld mobile phones.
- Tissue simulating liquid mixed according to the given recipes.
- Validation dipole kits allowing to validate the proper functioning of the system.


OPTIONS

- Isotropic E-field probe optimized and calibrated for E-field measurements in free space.
- Isotropic H-field probe optimized and calibrated for H-field measurements in any non-magnetic media.
- Flat Phantom (only for body-mounted transceivers operating below 800 MHz).

ADDITIONAL UTILITIES FOR SAR-MEASUREMENTS NOT PROVIDED BY SPEAG

- System to operate the device in a defined mode. For compliance testing, no cable should be attached. This is usually accomplished with tester communication with an air link or by special device software.
- System to measure the dielectric properties of the tissue simulating liquids. For the time being we recommend the usage of the HP 85070 dielectric probe kit. An alternative is the slotted coaxial line method. Both methods require a network analyzer.
- Signal generator, amplifier, power meter (precision <0.1dB), coupler and cable in order to perform the system check. A power level of larger than 14dBm is required (preferably 20-25 dBm).
- Utilities to prepare tissue simulating solution
 - Stirrer (magneto-stirrer with heating plate is recommended)
 - Balance (1 g accuracy, 500 to 2'000 g range)
 - Glass flask 3 l to 10 l for mixing liquid

11.2 System Setup

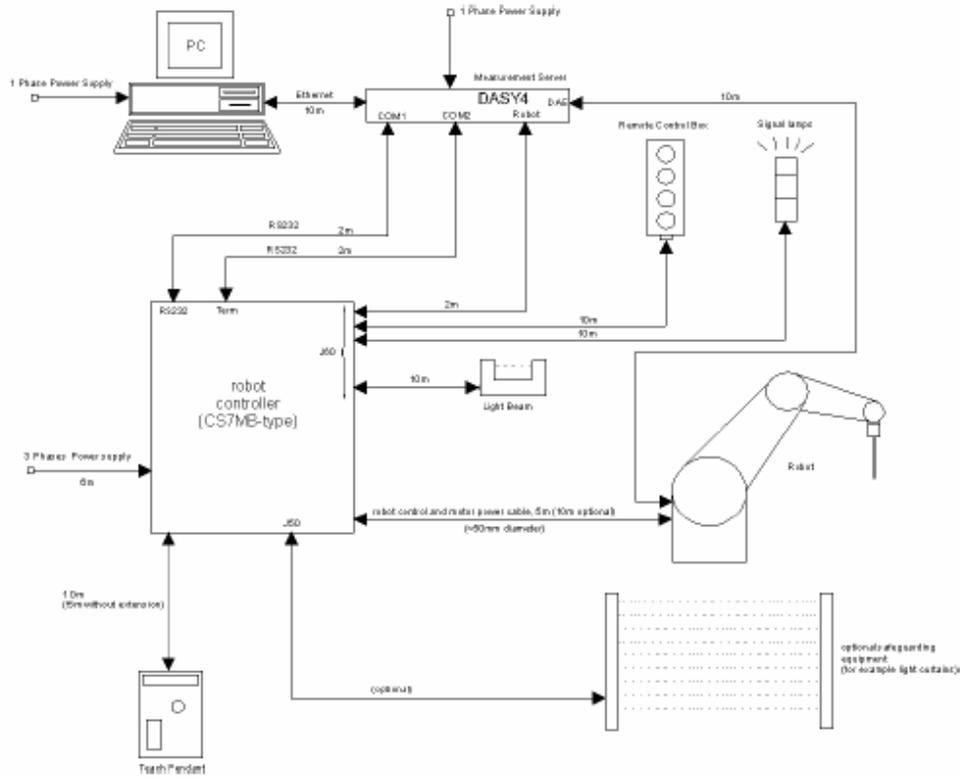

11.3 Requirements for the Room

- Approximately constant room temperature is recommended (because of the sensitivity of the liquid parameters). The floor should be easy to clean (liquid in phantom), stable, flat and vibration free.
- The circuit breaker for the 3-phase power for the robot depends on the power net voltage. For 3 phases 400 V (Europe) 4 Amp are needed and for 3 phases 208 V (USA, Asia) 10 Amp.

11.4 RF-Absorber in Operating Room or Laboratory

For dosimetric measurements, no RF-absorbers are needed. If you perform free space measurements other than only in the immediate near-field, moveable absorbers are useful to avoid reflections from the walls, robot etc. Shielding and absorbers might be necessary to avoid interference with other devices (e.g., sensitive measurement systems, base stations).

11.5 Wiring for Power Connection in USA

An open ended 4 wire cable for power connection with the following configuration is delivered with the DASY system:


- 3 phases Δ 208 V
- Ground (Safety Ground)

Customer needs to organize a wall-mounted plug and a corresponding connector for the installation

11.6 Wiring for Power Connection in Europe


A standard CEE 16 Amp plug connector is delivered (3-phase + safety ground).

11.7 Dimensions of DASY4 Compact Version

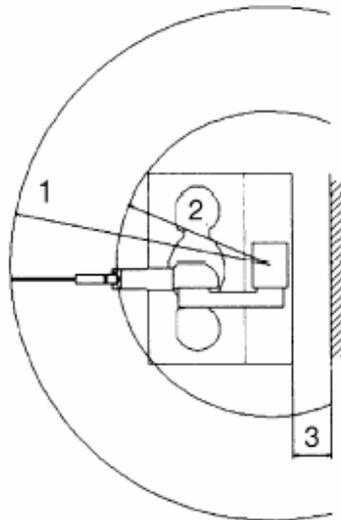

TOP VIEW

1. Range for horizontal aligned probes (e.g., free space measurements): 1350 mm
2. Range for vertical aligned probes (max distance to phantom): 800mm
3. Minimum distance from wall or absorber: 200 mm

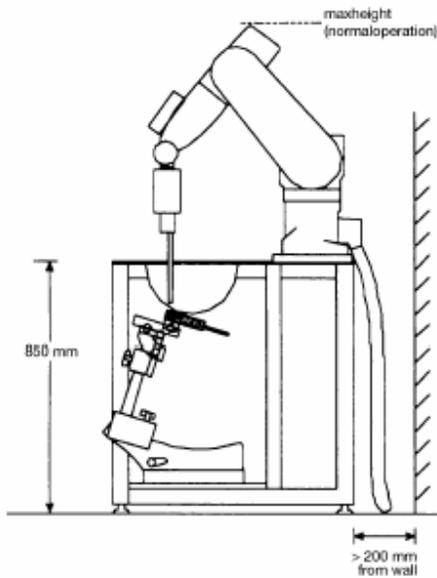


SIDE VIEW

1. Minimum free height: approx. 1700 mm
2. Height of table: 850 mm

TYPICAL SHIPPING DIMENSIONS


From robot company or SPEAG:	47x68x72cm 55 kg, 90x80x100cm 140 kg
From Schmid & Partner Engineering AG:	3 to 4 Euro - Palettes (120x80x100cm) total 400 kg

11.8 Dimensions of DASY4 Professional Version

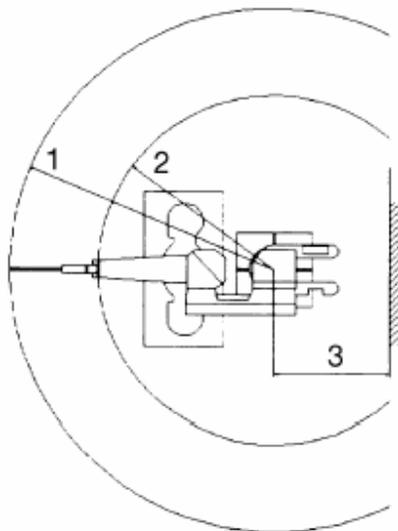

TOP VIEW

1. Range for horizontal aligned probes (e.g., free space measurements):
RX90L: 1590 mm, RX90: 1390 mm
2. Range for vertical aligned probes (max. distance to phantom):
RX90L: 1100 mm, RX90: 900 mm
3. Minimum distance from wall or absorber:
750 mm

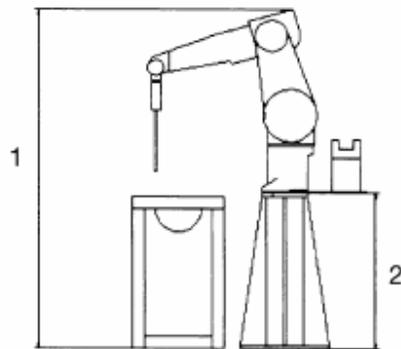

SIDE VIEW

- 1. Minimum free height: approx. 1900 mm
- 2. Height of robot socket: 850 mm

TYPICAL SHIPPING DIMENSIONS

From robot company or SPEAG:	85x65x121cm 140 kg, 90x80x100cm 140 kg
From Schmid & Partner Engineering AG:	3 to 4 Euro - Palettes (120x80x100cm) total 400 kg

Chapter 19

Data Storage and Evaluation

19.1 Data Storage

The DASY4 software stores the assessed data from the data acquisition electronics as raw data (in microvolt readings from the probe sensors), together with all the necessary software parameters for the data evaluation (probe calibration data, liquid parameters and device frequency and modulation data) in measurement files with the extension **.DA4**. The postprocessing software evaluates the desired unit and format for output each time the data is visualized or exported. This allows verification of the complete software setup even after the measurement and allows correction of erroneous parameter settings. For example, if a measurement has been performed with an incorrect crest factor parameter in the device setup, the parameter can be corrected afterwards and the data can be reevaluated.

To avoid unintentional parameter changes or data manipulations, the parameters in measured files are locked. In the administrator access mode of the software, the parameters can be unlocked (see Section **6.9 Unlocking a Setup**). After changing the parameters, the measured scans can be reevaluated in the postprocessing engine.

The measured data can be visualized or exported in different units or formats, depending on the selected probe type (e.g., [V/m], [A/m] or [mW/g]). Some of these units are not available in certain situations or give meaningless results, e.g., a SAR-output in a lossless media will always be zero. Raw data can also be exported to perform the evaluation with other software packages.

19.2 Data Evaluation

The DASY4 postprocessing software (SEMCAD) automatically executes the following procedures to calculate the field units from the microvolt readings at the probe connector. The parameters used in the evaluation are stored in the configuration modules of the software:

Probe parameters:	- Sensitivity	$Norm_i, a_{i0}, a_{i1}, a_{i2}$
	- Conversion factor	$ConvF_i$
	- Diode compression point	dcp_i
Device parameters:	- Frequency	f
	- Crest factor	cf
Media parameters:	- Conductivity	σ
	- Density	ρ

These parameters must be set correctly in the software. They can be found in the component documents or they can be imported into the software from the configuration files issued for the DASY components. In the direct measuring mode of the multimeter option, the parameters of the actual system setup are used. In the scan visualization and export modes, the parameters stored in the corresponding document files are used.

The first step of the evaluation is a linearization of the filtered input signal to account for the compression characteristics of the detector diode. The compensation depends on the input signal, the diode type and the DC-transmission factor from the diode to the evaluation electronics. If the exciting field is pulsed, the crest factor of the signal must be known to correctly compensate for peak power. The formula for each channel can be given as:

$$V_i = U_i + U_i^2 \cdot \frac{cf}{dcp_i} \tag{19.1}$$

- with V_i = compensated signal of channel i (i = x, y, z)
- U_i = input signal of channel i (i = x, y, z)
- cf = crest factor of exciting field (DASY parameter)
- dcp_i = diode compression point (DASY parameter)

From the compensated input signals the primary field data for each channel can be evaluated:

$$\text{E - fieldprobes : } E_i = \sqrt{\frac{V_i}{Norm_i \cdot ConvF}}$$

$$\text{H - fieldprobes : } H_i = \sqrt{V_i} \cdot \frac{a_{i0} + a_{i1}f + a_{i2}f^2}{f}$$

- with V_i = compensated signal of channel i (i = x, y, z)
- $Norm_i$ = sensor sensitivity of channel i (i = x, y, z)
- $ConvF$ = sensitivity enhancement in solution
- a_{ij} = sensor sensitivity factors for H-field probes
- f = carrier frequency [GHz]
- E_i = electric field strength of channel i in V/m
- H_i = magnetic field strength of channel i in A/m

The RSS value of the field components gives the total field strength (Hermitian magnitude):

$$E_{tot} = \sqrt{E_x^2 + E_y^2 + E_z^2} \tag{19.2}$$

The primary field data are used to calculate the derived field units.

$$SAR = E_{tot}^2 \cdot \frac{\sigma}{\rho \cdot 1'000} \tag{19.3}$$

- with SAR = local specific absorption rate in mW/g
- E_{tot} = total field strength in V/m
- σ = conductivity in [mho/m] or [Siemens/m]
- ρ = equivalent tissue density in g/cm³

Note that the density is set to 1, to account for actual head tissue density rather than the density of the tissue simulating liquid.

The power flow density is calculated assuming the excitation field to be a free space field.

$$P_{pwe} = \frac{E_{tot}^2}{3770} \quad \text{or} \quad P_{pwe} = H_{tot}^2 \cdot 37.7 \quad (19.4)$$

with P_{pwe} = equivalent power density of a plane wave in mW/cm²
 E_{tot} = total electric field strength in V/m
 H_{tot} = total magnetic field strength in A/m