



**DECLARATION OF COMPLIANCE SAR ASSESSMENT PCII Report Part 2 of 2**

**Motorola Solutions Inc**  
**EME Test Laboratory**  
 Motorola Solutions Malaysia Sdn Bhd (Innoplex) (455657-H)  
 Plot 2A, Medan Bayan Lepas,  
 Mukim 12 SWD, 11900 Bayan Lepas Penang, Malaysia.

**Date of Report:** 10/23/2017  
**Report Revision:** A

**Responsible Engineer:** Veeramani Veerapan  
**Report Author:** Veeramani Veerapan  
**Date/s Tested:** 07/13/2017- 08/11/2017  
**Manufacturer:** Motorola Solutions Inc.  
**DUT Description:** Handheld Portable - Frequency bands; LMR 136-174 MHz, 380-520 MHz, 764-776 MHz, 794-824 MHz & 851-869 MHz; Bluetooth 2.402-2.480 GHz; WLAN 2.400-2.483.5 GHz  
**Test TX mode(s):** CW (PTT), Bluetooth, and WLAN 802.11b/g/n  
**Max. Power output:** 6.6 W (VHF), 5.7 W (UHF), 2.99 W (700 MHz band), 3.6 W (800 MHz band), 10 mW (Bluetooth), 63.1 mW (802.11b), 25.1 mW (802.11g/n)  
**Nominal Power:** 6.0 W (VHF), 5.0 W (UHF), 2.5 W (700 MHz band), 3.0 W (800 MHz band), 10 mW (Bluetooth), 47.1 mW (802.11b), 19.95 mW (802.11g), 19.63 mW (802.11n)  
**Tx Frequency Bands:** LMR 136-174 MHz, 380-520 MHz, 764-805 MHz, 806-870 MHz; Bluetooth 2402-2480 MHz; WLAN 2400-2483.5 MHz  
**Signaling type:** FM, TDMA, FHSS (Bluetooth), 802.11b/g/n (WLAN)  
**Model(s) Tested:** H91TGD9PW5AN (PNUW1012C), H91TGD9PW7AN (PNUW1014C)  
**Model(s) Certified:** H91TGD9PW5AN (PNUW1012C), H91TGD9PW7AN (PNUW1014C)  
**Serial Number(s):** 579TTME968, 579TTME969, 579TTME980  
**Classification:** Occupational/Controlled  
**FCC ID:** AZ489FT7061; 150.8-173.4 MHz, 406.1-512 MHz, 764-775 MHz, 794-824 MHz, 851-869 MHz  
 This report contains results that are immaterial for FCC equipment approval, which are clearly identified.  
**IC** 109U-89FT7061; This report contains results that are immaterial for ISED equipment approval, which are clearly identified.  
**ISED Test Site Registration:** 109AK  
**FCC Test Firm Registration Number:** 823256

The test results clearly demonstrate compliance with FCC Occupational/Controlled RF Exposure limits of 8 W/kg averaged over 1 gram per the requirements of FCC 47 CFR § 2.1093.

Based on the information and the testing results provided herein, the undersigned certifies that when used as stated in the operating instructions supplied, said product complies with the national and international reference standards and guidelines listed in section 4.0 of this report. This report shall not be reproduced without written approval from an officially designated representative of the Motorola Solutions Inc EME Laboratory. I attest to the accuracy of the data and assume full responsibility for the completeness of these measurements. This reporting format is consistent with the suggested guidelines of the TIA TSB-150 December 2004. The results and statements contained in this report pertain only to the device(s) evaluated.

*Tiong*  
**Tiong Nguk Ing**  
**Deputy Technical Manager**  
**Approval Date:** 10/23/2017

## Appendix C Dipole Calibration Certificates

**Calibration Laboratory of  
Schmid & Partner  
Engineering AG**  
Zeughausstrasse 43, 8004 Zurich, Switzerland



**S** Schweizerischer Kalibrierdienst  
**C** Service suisse d'étalonnage  
**S** Servizio svizzero di taratura  
**S** Swiss Calibration Service

Accredited by the Swiss Accreditation Service (SAS)  
The Swiss Accreditation Service is one of the signatories to the EA  
Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: **SCS 0108**

Client **Motorola Solutions MY**

Certificate No: **CLA150-4010\_Nov16**

**CALIBRATION CERTIFICATE**

Object: **CLA150 - SN: 4010**

Calibration procedure(s): **QA CAL-15.v8  
Calibration procedure for system validation sources below 700 MHz**

Calibration date: **November 08, 2016**

This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI).  
The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility: environment temperature (22 ± 3)°C and humidity < 70%.

Calibration Equipment used (M&TE critical for calibration)

Primary Standards	ID #	Cal Date (Certificate No.)	Scheduled Calibration
Power meter NRP	SN: 104778	06-Apr-16 (No. 217-02288/02289)	Apr-17
Power sensor NRP-Z91	SN: 103244	06-Apr-16 (No. 217-02288)	Apr-17
Power sensor NRP-Z91	SN: 103245	06-Apr-16 (No. 217-02289)	Apr-17
Reference 30 dB Attenuator	SN: 5129 (30b)	05-Apr-16 (No. 217-02294)	Apr-17
Type-N mismatch combination	SN: 5047.2 / 06327	05-Apr-16 (No. 217-02295)	Apr-17
Reference Probe EX3DV4 DAE4	SN: 3877 SN: 654	31-Dec-15 (No. EX3-3877_Dec15) 12-Aug-16 (No. DAE4-654_Aug16)	Dec-16 Aug-17
Secondary Standards	ID #	Check Date (in house)	Scheduled Check
Power meter E4419B	SN: 0B411293874	06-Apr-16 (No. 217-02285/02284)	In house check: Jun-18
Power sensor E4412A	SN: MY41498087	06-Apr-16 (No. 217-02285)	In house check: Jun-18
Power sensor E4412A	SN: 000110210	06-Apr-16 (No. 217-02284)	In house check: Jun-18
RF generator HP 8648C	SN: US3642U01700	04-Aug-99 (in house check Jun-16)	In house check: Jun-18
Network Analyzer HP 8753E	SN: US37390585	18-Oct-01 (in house check Oct-16)	In house check: Oct-17

	Name	Function	Signature
Calibrated by:	Jeton Kastali	Laboratory Technician	
Approved by:	Katja Pokovic	Technical Manager	

issued: November 9, 2016

This calibration certificate shall not be reproduced except in full without written approval of the laboratory.

**Calibration Laboratory of  
Schmid & Partner  
Engineering AG**  
Zeughausstrasse 43, 8004 Zurich, Switzerland



**S** Schweizerischer Kalibrierdienst  
**C** Service suisse d'étalonnage  
**S** Servizio svizzero di taratura  
**S** Swiss Calibration Service

Accredited by the Swiss Accreditation Service (SAS)  
The Swiss Accreditation Service is one of the signatories to the EA  
Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: **SCS 0108**

**Glossary:**

TSL tissue simulating liquid  
ConvF sensitivity in TSL / NORM x,y,z  
N/A not applicable or not measured

**Calibration is Performed According to the Following Standards:**

- a) IEEE Std 1528-2013, "IEEE Recommended Practice for Determining the Peak Spatial-Averaged Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques", June 2013
- b) IEC 62209-1, "Procedure to measure the Specific Absorption Rate (SAR) for hand-held devices used in close proximity to the ear (frequency range of 300 MHz to 3 GHz)", February 2005
- c) IEC 62209-2, "Procedure to determine the Specific Absorption Rate (SAR) for wireless communication devices used in close proximity to the human body (frequency range of 30 MHz to 6 GHz)", March 2010
- d) KDB 865864, "SAR Measurement Requirements for 100 MHz to 6 GHz"

**Additional Documentation:**

- e) DASY4/5 System Handbook

**Methods Applied and Interpretation of Parameters:**

- *Measurement Conditions:* Further details are available from the Validation Report at the end of the certificate. All figures stated in the certificate are valid at the frequency indicated.
- *Antenna Parameters with TSL:* The source is mounted in a touch configuration below the center marking of the flat phantom.
- *Return Loss:* This parameter is measured with the source positioned under the liquid filled phantom (as described in the measurement condition clause). The Return Loss ensures low reflected power. No uncertainty required.
- *SAR measured:* SAR measured at the stated antenna input power.
- *SAR normalized:* SAR as measured, normalized to an input power of 1 W at the antenna connector.
- *SAR for nominal TSL parameters:* The measured TSL parameters are used to calculate the nominal SAR result.

The reported uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor k=2, which for a normal distribution corresponds to a coverage probability of approximately 95%.

**Measurement Conditions**

DASY system configuration, as far as not given on page 1.

DASY Version	DASY5	V52.8.8
Extrapolation	Advanced Extrapolation	
Phantom	ELI4 Flat Phantom	Shell thickness: $2 \pm 0.2$ mm
EUT Positioning	Touch Position	
Zoom Scan Resolution	$dx, dy = 4.0$ mm, $dz = 1.4$ mm	Graded Ratio = 1.4 (Z direction)
Frequency	150 MHz $\pm 1$ MHz	

**Head TSL parameters**

The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Head TSL parameters	22.0 °C	52.3	0.76 mho/m
Measured Head TSL parameters	$(22.0 \pm 0.2)$ °C	$50.1 \pm 6 \%$	$0.75$ mho/m $\pm 6 \%$
Head TSL temperature change during test	< 0.5 °C	---	---

**SAR result with Head TSL**

SAR averaged over 1 cm <sup>3</sup> (1 g) of Head TSL	Condition	
SAR measured	1 W input power	3.69 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	<b>3.69 W/kg <math>\pm 18.4 \%</math> (k=2)</b>

SAR averaged over 10 cm <sup>3</sup> (10 g) of Head TSL	condition	
SAR measured	1 W input power	2.45 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	<b>2.46 W/kg <math>\pm 18.0 \%</math> (k=2)</b>

**Body TSL parameters**

The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Body TSL parameters	22.0 °C	61.9	0.80 mho/m
Measured Body TSL parameters	$(22.0 \pm 0.2)$ °C	$61.4 \pm 6 \%$	$0.82$ mho/m $\pm 6 \%$
Body TSL temperature change during test	< 0.5 °C	----	----

**SAR result with Body TSL**

SAR averaged over 1 cm <sup>3</sup> (1 g) of Body TSL	Condition	
SAR measured	1 W input power	3.86 W/kg
SAR for nominal Body TSL parameters	normalized to 1W	<b>3.78 W/kg <math>\pm 18.4 \%</math> (k=2)</b>

SAR averaged over 10 cm <sup>3</sup> (10 g) of Body TSL	condition	
SAR measured	1 W input power	2.56 W/kg
SAR for nominal Body TSL parameters	normalized to 1W	<b>2.51 W/kg <math>\pm 18.0 \%</math> (k=2)</b>

**Appendix (Additional assessments outside the scope of SCS 0108)**

**Antenna Parameters with Head TSL**

Impedance, transformed to feed point	45.9 $\Omega$ - 4.5 $j\Omega$
Return Loss	- 24.1 dB

**Antenna Parameters with Body TSL**

Impedance, transformed to feed point	50.9 $\Omega$ - 6.6 $j\Omega$
Return Loss	- 23.7 dB

**Additional EUT Data**

Manufactured by	SPEAG
Manufactured on	April 15, 2014

**DASY5 Validation Report for Head TSL**

Date: 07.11.2016

Test Laboratory: SPEAG, Zurich, Switzerland

**DUT: CLA-150; Type: CLA-150; Serial: 4010**

Communication System: UID 0 - CW; Frequency: 150 MHz  
 Medium parameters used:  $f = 150 \text{ MHz}$ ;  $\sigma = 0.75 \text{ S/m}$ ;  $\epsilon_r = 50.1$ ;  $\rho = 1000 \text{ kg/m}^3$   
 Phantom section: Flat Section  
 Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2011)

DASY52 Configuration:


- Probe: EX3DV4 - SN3877; ConvF(12.02, 12.02, 12.02); Calibrated: 31.12.2015;
- Sensor-Surface: 1.4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn654; Calibrated: 12.08.2016
- Phantom: ELI v4.0; Type: QDOVA001BB; Serial: TP:1003
- DASY52 52.8.8(1258); SEMCAD X 14.6.10(7372)

**CLA Calibration for HSL-LF Tissue/CLA150, touch configuration, Pin=1W/Area Scan (81x81x1):**

Interpolated grid:  $dx=1.500 \text{ mm}$ ,  $dy=1.500 \text{ mm}$   
 Maximum value of SAR (interpolated) = 5.16 W/kg


**CLA Calibration for HSL-LF Tissue/CLA150, touch configuration, Pin=1W/Zoom Scan, dist=1.4mm (8x10x7)/Cube 0:**

Measurement grid:  $dx=4\text{mm}$ ,  $dy=4\text{mm}$ ,  $dz=1.4\text{mm}$   
 Reference Value = 82.42 V/m; Power Drift = -0.02 dB  
 Peak SAR (extrapolated) = 6.93 W/kg  
**SAR(1 g) = 3.69 W/kg; SAR(10 g) = 2.45 W/kg**  
 Maximum value of SAR (measured) = 5.16 W/kg

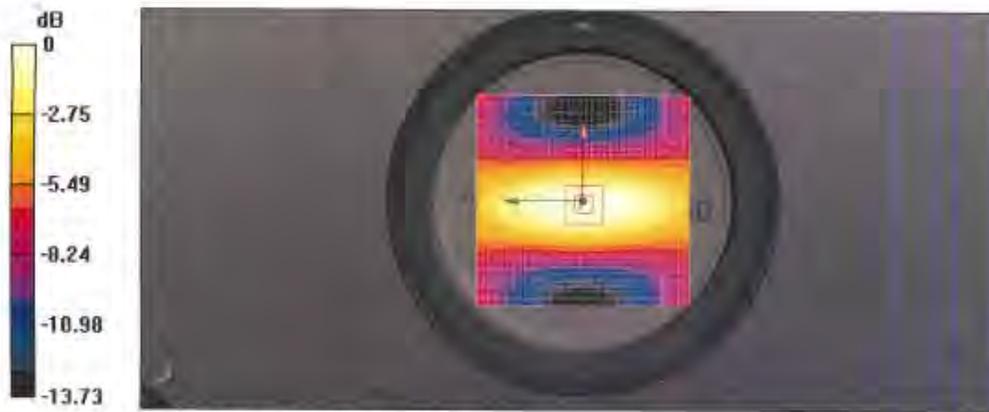

0 dB = 5.16 W/kg = 7.13 dBW/kg

### Impedance Measurement Plot for Head TSL

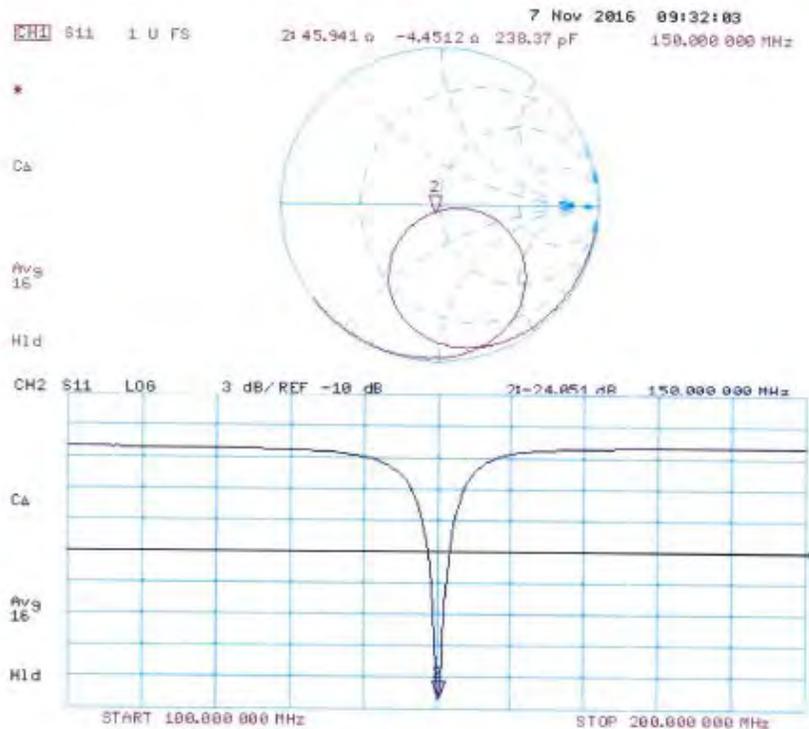

**DASY5 Validation Report for Body TSL**

Date: 08.11.2016

Test Laboratory: SPEAG, Zurich, Switzerland

**DUT: CLA-150; Type: CLA-150; Serial: 4010**

Communication System: UID 0 - CW; Frequency: 150 MHz  
 Medium parameters used:  $f = 150 \text{ MHz}$ ;  $\sigma = 0.82 \text{ S/m}$ ;  $\epsilon_r = 61.4$ ;  $\rho = 1000 \text{ kg/m}^3$   
 Phantom section: Flat Section  
 Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2011)

**DASY52 Configuration:**


- Probe: EX3DV4 - SN3877; ConvF(11.44, 11.44, 11.44); Calibrated: 31.12.2015;
- Sensor-Surface: 1.4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn654; Calibrated: 12.08.2016
- Phantom: ELI v4.0; Type: QDOVA001BB; Serial: TP:1003
- DASY52 52.8.8(1258); SEMCAD X 14.6.10(7372)

**CLA Calibration for MSL-LF Tissue/CLA150, touch configuration, Pin=1W/Area Scan (81x81x1):**

Interpolated grid:  $dx=1.500 \text{ mm}$ ,  $dy=1.500 \text{ mm}$   
 Maximum value of SAR (interpolated) = 5.45 W/kg


**CLA Calibration for MSL-LF Tissue/CLA150, touch configuration, Pin=1W/Zoom Scan,**

**dist=1.4mm (8x10x7)/Cube 0:** Measurement grid:  $dx=4\text{mm}$ ,  $dy=4\text{mm}$ ,  $dz=1.4\text{mm}$   
 Reference Value = 80.49 V/m; Power Drift = -0.09 dB  
 Peak SAR (extrapolated) = 7.18 W/kg  
**SAR(1 g) = 3.86 W/kg; SAR(10 g) = 2.56 W/kg**  
 Maximum value of SAR (measured) = 5.38 W/kg

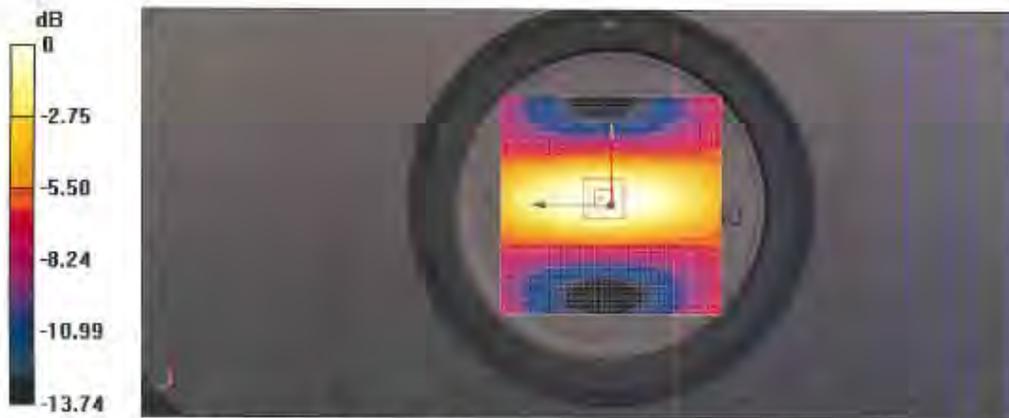

0 dB = 5.45 W/kg = 7.36 dBW/kg

### Impedance Measurement Plot for Body TSL

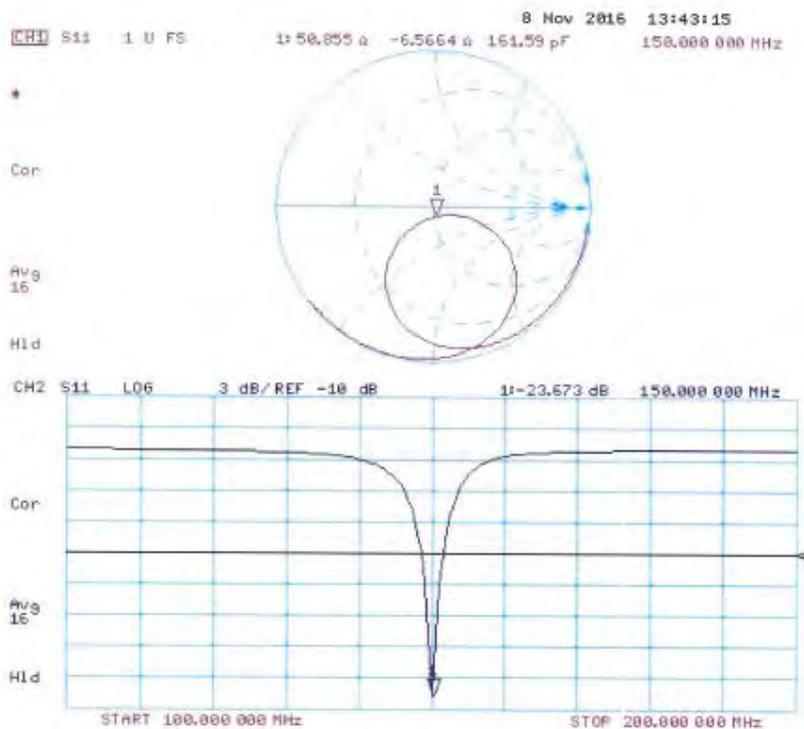

**Calibration Laboratory of  
Schmid & Partner  
Engineering AG**  
Zeughausstrasse 43, 8004 Zurich, Switzerland



**S** Schweizerischer Kalibrierdienst  
**S** Service suisse d'étalonnage  
**S** Servizio svizzero di taratura  
**S** Swiss Calibration Service

Accredited by the Swiss Accreditation Service (SAS)  
The Swiss Accreditation Service is one of the signatories to the EA  
Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: **SCS 0108**

Client: **Motorola EME**

Certificate No: **D450V3-1077\_Nov15**

**CALIBRATION CERTIFICATE**

Object: **D450V3 - SN: 1077**

Calibration procedure(s): **QA CAL-15.v8  
Calibration procedure for dipole validation kits below 700 MHz**

Calibration date: **November 25, 2015**

This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI).  
The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility: environment temperature (22 ± 3)°C and humidity < 70%.

Calibration Equipment used (M&TE critical for calibration)

Primary Standards	ID #	Cal Date (Certificate No.)	Scheduled Calibration
Power meter E4419B	GB41293674	01-Apr-15 (No. 217-02128)	Mar-16
Power sensor E4412A	MY41498087	01-Apr-15 (No. 217-02128)	Mar-16
Reference 3 dB Attenuator	SN: S5054 (3c)	01-Apr-15 (No. 217-02128)	Mar-16
Reference 20 dB Attenuator	SN: S5058 (20k)	01-Apr-15 (No. 217-02131)	Mar-16
Type-N mismatch combination	SN: 5047.2 / 06327	01-Apr-15 (No. 217-02134)	Mar-16
Reference Probe ET3DV6	SN: 1507	30-Dec-14 (No. ET3-1507_Dec14)	Dec-15
DAE4	SN: 654	08-Jul-15 (No. DAE4-654_Jul15)	Jul-16

Secondary Standards	ID #	Check Date (in house)	Scheduled Check
RF generator HP 8648C	US3642U01700	04-Aug-99 (in house check Apr-13)	in house check: Apr-16
Network Analyzer HP 8753E	US37390585 S4206	16-Oct-01 (in house check Oct-15)	in house check: Oct-16

Calibrated by: **Leif Klysnar** (Name), **Laboratory Technician** (Function), *[Signature]* (Signature)

Approved by: **Katja Pokovic** (Name), **Technical Manager** (Function), *[Signature]* (Signature)

Issued: November 25, 2015

This calibration certificate shall not be reproduced except in full without written approval of the laboratory.

**Calibration Laboratory of  
Schmid & Partner  
Engineering AG**  
Zeughausstrasse 43, 8004 Zurich, Switzerland



**S** Schweizerischer Kalibrierdienst  
**C** Service suisse d'étalonnage  
**S** Servizio svizzero di taratura  
**S** Swiss Calibration Service

Accredited by the Swiss Accreditation Service (SAS)  
The Swiss Accreditation Service is one of the signatories to the EA  
Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: **SCS 0108**

**Glossary:**

TSL tissue simulating liquid  
ConvF sensitivity in TSL / NORM x,y,z  
N/A not applicable or not measured

**Calibration is Performed According to the Following Standards:**

- a) IEEE Std 1528-2013, "IEEE Recommended Practice for Determining the Peak Spatial-Averaged Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques", June 2013
- b) IEC 62209-1, "Procedure to measure the Specific Absorption Rate (SAR) for hand-held devices used in close proximity to the ear (frequency range of 300 MHz to 3 GHz)", February 2005
- c) IEC 62209-2, "Procedure to determine the Specific Absorption Rate (SAR) for wireless communication devices used in close proximity to the human body (frequency range of 30 MHz to 6 GHz)", March 2010
- d) KDB 865664, "SAR Measurement Requirements for 100 MHz to 6 GHz"

**Additional Documentation:**

- e) DASY4/5 System Handbook

**Methods Applied and Interpretation of Parameters:**

- *Measurement Conditions:* Further details are available from the Validation Report at the end of the certificate. All figures stated in the certificate are valid at the frequency indicated.
- *Antenna Parameters with TSL:* The dipole is mounted with the spacer to position its feed point exactly below the center marking of the flat phantom section, with the arms oriented parallel to the body axis.
- *Feed Point Impedance and Return Loss:* These parameters are measured with the dipole positioned under the liquid filled phantom. The impedance stated is transformed from the measurement at the SMA connector to the feed point. The Return Loss ensures low reflected power. No uncertainty required.
- *Electrical Delay:* One-way delay between the SMA connector and the antenna feed point. No uncertainty required.
- *SAR measured:* SAR measured at the stated antenna input power.
- *SAR normalized:* SAR as measured, normalized to an input power of 1 W at the antenna connector.
- *SAR for nominal TSL parameters:* The measured TSL parameters are used to calculate the nominal SAR result.

The reported uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor k=2, which for a normal distribution corresponds to a coverage probability of approximately 95%.

**Measurement Conditions**

DASY system configuration, as far as not given on page 1.

DASY Version	DASY5	V52.8.8
Extrapolation	Advanced Extrapolation	
Phantom	EL14 Flat Phantom	Shell thickness: 2 ± 0.2 mm
Distance Dipole Center - TSL	15 mm	with Spacer
Zoom Scan Resolution	dx, dy, dz = 5 mm	
Frequency	450 MHz ± 1 MHz	

**Head TSL parameters**

The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Head TSL parameters	22.0 °C	43.5	0.87 mho/m
Measured Head TSL parameters	(22.0 ± 0.2) °C	44.0 ± 6 %	0.89 mho/m ± 6 %
Head TSL temperature change during test	< 0.5 °C	---	---

**SAR result with Head TSL**

SAR averaged over 1 cm <sup>3</sup> (1 g) of Head TSL	Condition	
SAR measured	250 mW input power	1.16 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	4.57 W/kg ± 18.1 % (k=2)

SAR averaged over 10 cm <sup>3</sup> (10 g) of Head TSL	condition	
SAR measured	250 mW input power	0.777 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	3.07 W/kg ± 17.6 % (k=2)

**Body TSL parameters**

The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Body TSL parameters	22.0 °C	56.7	0.94 mho/m
Measured Body TSL parameters	(22.0 ± 0.2) °C	56.3 ± 6 %	0.95 mho/m ± 6 %
Body TSL temperature change during test	< 0.5 °C	---	---

**SAR result with Body TSL**

SAR averaged over 1 cm <sup>3</sup> (1 g) of Body TSL	Condition	
SAR measured	250 mW input power	1.14 W/kg
SAR for nominal Body TSL parameters	normalized to 1W	4.52 W/kg ± 18.1 % (k=2)

SAR averaged over 10 cm <sup>3</sup> (10 g) of Body TSL	condition	
SAR measured	250 mW input power	0.749 W/kg
SAR for nominal Body TSL parameters	normalized to 1W	2.97 W/kg ± 17.6 % (k=2)

**Appendix (Additional assessments outside the scope of SCS 0108)**

**Antenna Parameters with Head TSL**

Impedance, transformed to feed point	58.1 Ω - 2.3 jΩ
Return Loss	- 22.1 dB

**Antenna Parameters with Body TSL**

Impedance, transformed to feed point	55.0 Ω - 6.8 jΩ
Return Loss	- 21.9 dB

**General Antenna Parameters and Design**

Electrical Delay (one direction)	1.349 ns
----------------------------------	----------

After long term use with 100W radiated power, only a slight warming of the dipole near the feedpoint can be measured.

The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals. On some of the dipoles, small end caps are added to the dipole arms in order to improve matching when loaded according to the position as explained in the "Measurement Conditions" paragraph. The SAR data are not affected by this change. The overall dipole length is still according to the Standard.

No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feedpoint may be damaged.

**Additional EUT Data**

Manufactured by	SPEAG
Manufactured on	June 24, 2010

**DASY5 Validation Report for Head TSL**

Date: 25.11.2015

Test Laboratory: SPEAG, Zurich, Switzerland

**DUT: Dipole 450 MHz; Type: D450V3; Serial: D450V3 - SN: 1077**


Communication System: UID 0 - CW; Frequency: 450 MHz  
 Medium parameters used:  $f = 450 \text{ MHz}$ ;  $\sigma = 0.89 \text{ S/m}$ ;  $\epsilon_r = 44$ ;  $\rho = 1000 \text{ kg/m}^3$   
 Phantom section: Flat Section  
 Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2011)

**DASY52 Configuration:**

- Probe: ET3DV6 - SN1507; ConvF(6.58, 6.58, 6.58); Calibrated: 30.12.2014;
- Sensor-Surface: 4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn654; Calibrated: 08.07.2015
- Phantom: ELI v4.0; Type: QDOVA001BB; Serial: TP:1003
- DASY52 52.8.8(1222); SEMCAD X 14.6.10(7331)


**Dipole Calibration for Head Tissue/d=15mm, Pin=250mW/Zoom Scan (7x7x7)/Cube 0:**

Measurement grid:  $dx=5\text{mm}$ ,  $dy=5\text{mm}$ ,  $dz=5\text{mm}$   
 Reference Value = 39.43 V/m; Power Drift = -0.04 dB  
 Peak SAR (extrapolated) = 1.67 W/kg  
**SAR(1 g) = 1.16 W/kg; SAR(10 g) = 0.777 W/kg**  
 Maximum value of SAR (measured) = 1.25 W/kg

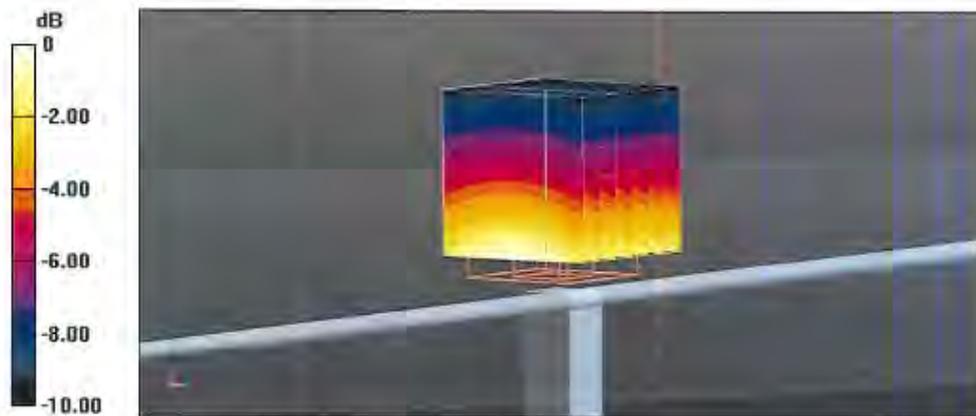

0 dB = 1.25 W/kg = 0.97 dBW/kg

### Impedance Measurement Plot for Head TSL

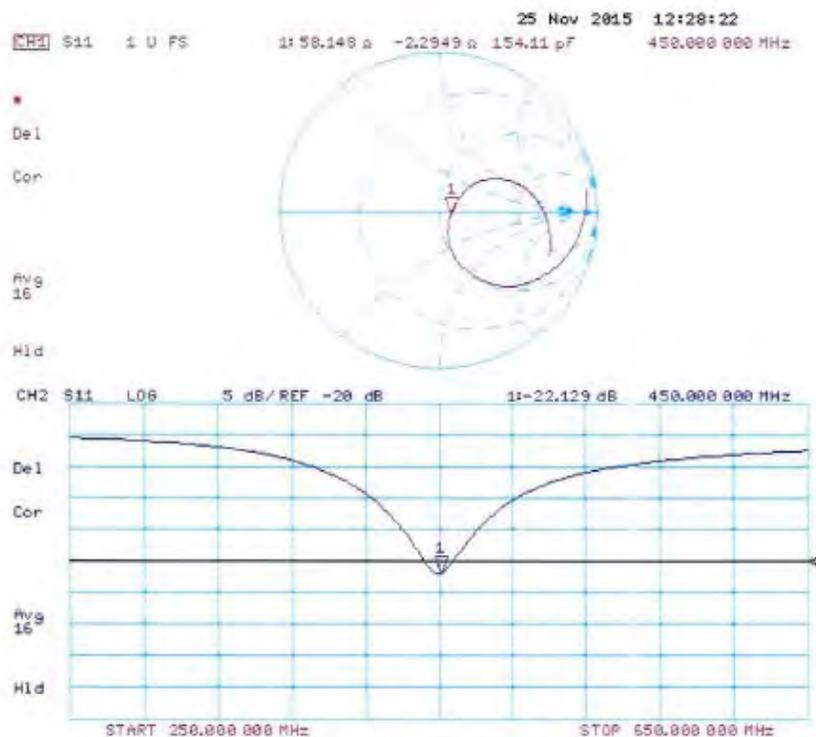

**DASY5 Validation Report for Body TSL**

Date: 25.11.2015

Test Laboratory: SPEAG, Zurich, Switzerland

**DUT: Dipole 450 MHz; Type: D450V3; Serial: D450V3 - SN: 1077**


Communication System: UID 0 - CW; Frequency: 450 MHz  
Medium parameters used:  $f = 450 \text{ MHz}$ ;  $\sigma = 0.95 \text{ S/m}$ ;  $\epsilon_r = 56.3$ ;  $\rho = 1000 \text{ kg/m}^3$   
Phantom section: Flat Section  
Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2011)

**DASY52 Configuration:**


- Probe: ET3DV6 - SN1507; ConvF(7.05, 7.05, 7.05); Calibrated: 30.12.2014;
- Sensor-Surface: 4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn654; Calibrated: 08.07.2015
- Phantom: ELI v4.0; Type: QDOVA001BB; Serial: TP:1003
- DASY52 52.8.8(1222); SEMCAD X 14.6.10(7331)

**Dipole Calibration for Body Tissue/d=15mm, Pin=250mW/Zoom Scan (7x7x7)/Cube 0:**

Measurement grid:  $dx=5\text{mm}$ ,  $dy=5\text{mm}$ ,  $dz=5\text{mm}$   
Reference Value = 36.74 V/m; Power Drift = -0.04 dB  
Peak SAR (extrapolated) = 1.80 W/kg  
**SAR(1 g) = 1.14 W/kg; SAR(10 g) = 0.749 W/kg**  
Maximum value of SAR (measured) = 1.22 W/kg

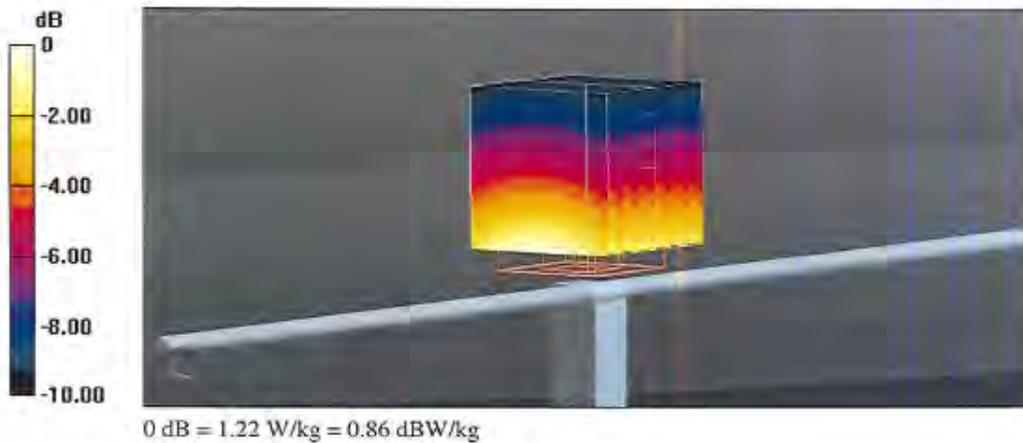

### Impedance Measurement Plot for Body TSL

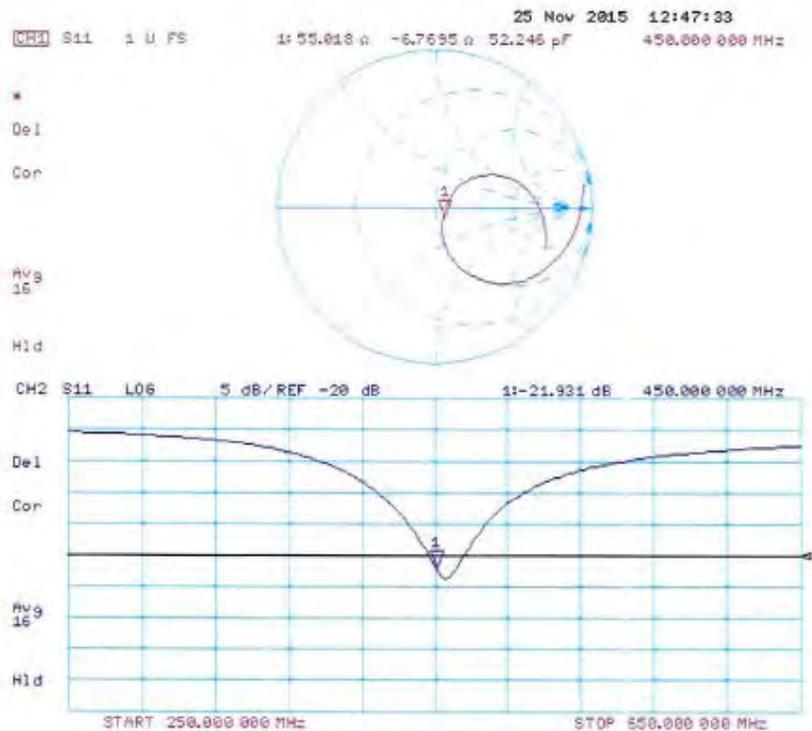

**Calibration Laboratory of  
Schmid & Partner  
Engineering AG**  
Zeughausstrasse 43, 8004 Zurich, Switzerland



**S** Schweizerischer Kalibrierdienst  
**S** Service suisse d'étalonnage  
**C** Servizio svizzero di taratura  
**S** Swiss Calibration Service

Accredited by the Swiss Accreditation Service (SAS)  
The Swiss Accreditation Service is one of the signatories to the EA  
Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: **SCS 0108**

Client: **Motorola EME**

Certificate No: **D750V3-1098\_Nov15**

**CALIBRATION CERTIFICATE**

Object: **D750V3 - SN: 1098**

Calibration procedure(s): **QA CAL-05.v9  
Calibration procedure for dipole validation kits above 700 MHz**

Calibration date: **November 24, 2015**

This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI).  
The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility: environment temperature (22 ± 3)°C and humidity < 70%.

Calibration Equipment used (M&TE critical for calibration)

Primary Standards	ID #	Cal Date (Certificate No.)	Scheduled Calibration
Power meter EPM-442A	GB37480704	07-Oct-15 (No. 217-02222)	Oct-15
Power sensor HP 8481A	US37292783	07-Oct-15 (No. 217-02222)	Oct-15
Power sensor HP 8481A	MY41092317	07-Oct-15 (No. 217-02223)	Oct-15
Reference 20 dB Attenuator	SN: 5058 (20k)	01-Apr-15 (No. 217-02131)	Mar-16
Type-N mismatch combination	SN: 5047.2 / 06327	01-Apr-15 (No. 217-02134)	Mar-16
Reference Probe EX3DV4	SN: 7349	30-Dec-14 (No. EX3-7349_Dec14)	Dec-15
DAE4	SN: 601	17-Aug-15 (No. DAE4-601_Aug15)	Aug-16
Secondary Standards	ID #	Check Date (in house)	Scheduled Check
RF generator R&S SMT-06	100972	15-Jun-15 (in house check Jun-15)	In house check: Jun-16
Network Analyzer HP 8753E	US37390685 S4206	18-Oct-01 (in house check Oct-15)	In house check: Oct-16

Calibrated by:	Name <b>Claudio Leubler</b>	Function <b>Laboratory Technician</b>	Signature 
Approved by:	Name <b>Katja Pokovic</b>	Technical Manager	

Issued: November 24, 2015

This calibration certificate shall not be reproduced except in full without written approval of the laboratory.

**Calibration Laboratory of**  
**Schmid & Partner**  
**Engineering AG**  
 Zeughausstrasse 43, 8004 Zurich, Switzerland



**S** Schweizerischer Kalibrierdienst  
**C** Service suisse d'étalonnage  
**S** Servizio svizzero di taratura  
**S** Swiss Calibration Service

Accredited by the Swiss Accreditation Service (SAS)  
 The Swiss Accreditation Service is one of the signatories to the EA  
 Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: **SCS 0108**

**Glossary:**

TSL tissue simulating liquid  
 ConvF sensitivity in TSL / NORM x,y,z  
 N/A not applicable or not measured

**Calibration is Performed According to the Following Standards:**

- a) IEEE Std 1528-2013, "IEEE Recommended Practice for Determining the Peak Spatial-Averaged Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques", June 2013
- b) IEC 62209-1, "Procedure to measure the Specific Absorption Rate (SAR) for hand-held devices used in close proximity to the ear (frequency range of 300 MHz to 3 GHz)", February 2005
- c) IEC 62209-2, "Procedure to determine the Specific Absorption Rate (SAR) for wireless communication devices used in close proximity to the human body (frequency range of 30 MHz to 6 GHz)", March 2010
- d) KDB 865664, "SAR Measurement Requirements for 100 MHz to 6 GHz"

**Additional Documentation:**

- e) DASy4/5 System Handbook

**Methods Applied and Interpretation of Parameters:**

- *Measurement Conditions:* Further details are available from the Validation Report at the end of the certificate. All figures stated in the certificate are valid at the frequency indicated.
- *Antenna Parameters with TSL:* The dipole is mounted with the spacer to position its feed point exactly below the center marking of the flat phantom section, with the arms oriented parallel to the body axis.
- *Feed Point Impedance and Return Loss:* These parameters are measured with the dipole positioned under the liquid filled phantom. The impedance stated is transformed from the measurement at the SMA connector to the feed point. The Return Loss ensures low reflected power. No uncertainty required.
- *Electrical Delay:* One-way delay between the SMA connector and the antenna feed point. No uncertainty required.
- *SAR measured:* SAR measured at the stated antenna input power.
- *SAR normalized:* SAR as measured, normalized to an input power of 1 W at the antenna connector.
- *SAR for nominal TSL parameters:* The measured TSL parameters are used to calculate the nominal SAR result.

The reported uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor k=2, which for a normal distribution corresponds to a coverage probability of approximately 95%.

**Measurement Conditions**

DASY system configuration, as far as not given on page 1.

DASY Version	DASY5	V52.8.8
Extrapolation	Advanced Extrapolation	
Phantom	Modular Flat Phantom	
Distance Dipole Center - TSL	15 mm	with Spacer
Zoom Scan Resolution	dx, dy, dz = 5 mm	
Frequency	750 MHz ± 1 MHz	

**Head TSL parameters**

The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Head TSL parameters	22.0 °C	41.9	0.89 mho/m
Measured Head TSL parameters	(22.0 ± 0.2) °C	42.8 ± 6 %	0.90 mho/m ± 5 %
Head TSL temperature change during test	< 0.5 °C	---	---

**SAR result with Head TSL**

SAR averaged over 1 cm <sup>3</sup> (1 g) of Head TSL	Condition	
SAR measured	250 mW input power	2.06 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	<b>8.21 W/kg ± 17.0 % (k=2)</b>

SAR averaged over 10 cm <sup>3</sup> (10 g) of Head TSL	condition	
SAR measured	250 mW input power	1.35 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	<b>5.38 W/kg ± 16.5 % (k=2)</b>

**Body TSL parameters**

The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Body TSL parameters	22.0 °C	55.5	0.96 mho/m
Measured Body TSL parameters	(22.0 ± 0.2) °C	55.9 ± 6 %	0.97 mho/m ± 6 %
Body TSL temperature change during test	< 0.5 °C	---	---

**SAR result with Body TSL**

SAR averaged over 1 cm <sup>3</sup> (1 g) of Body TSL	Condition	
SAR measured	250 mW input power	2.23 W/kg
SAR for nominal Body TSL parameters	normalized to 1W	<b>8.86 W/kg ± 17.0 % (k=2)</b>

SAR averaged over 10 cm <sup>3</sup> (10 g) of Body TSL	condition	
SAR measured	250 mW input power	1.48 W/kg
SAR for nominal Body TSL parameters	normalized to 1W	<b>5.89 W/kg ± 16.5 % (k=2)</b>

**Appendix (Additional assessments outside the scope of SCS 0108)**

**Antenna Parameters with Head TSL**

Impedance, transformed to feed point	53.0 Ω - 2.8 jΩ
Return Loss	- 28.0 dB

**Antenna Parameters with Body TSL**

Impedance, transformed to feed point	49.3 Ω - 4.5 jΩ
Return Loss	- 26.7 dB

**General Antenna Parameters and Design**

Electrical Delay (one direction)	1.031 ns
----------------------------------	----------

After long term use with 100W radiated power, only a slight warming of the dipole near the feedpoint can be measured.

The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals. On some of the dipoles, small end caps are added to the dipole arms in order to improve matching when loaded according to the position as explained in the "Measurement Conditions" paragraph. The SAR data are not affected by this change. The overall dipole length is still according to the Standard.

No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feedpoint may be damaged.

**Additional EUT Data**

Manufactured by	SPEAG
Manufactured on	July 05, 2013

**DASY5 Validation Report for Head TSL**

Date: 24.11.2015

Test Laboratory: SPEAG, Zurich, Switzerland

**DUT: Dipole 750 MHz; Type: D750V3; Serial: D750V3 - SN: 1098**


Communication System: UID 0 - CW; Frequency: 750 MHz  
Medium parameters used:  $f = 750$  MHz;  $\sigma = 0.9$  S/m;  $\epsilon_r = 42.8$ ;  $\rho = 1000$  kg/m<sup>3</sup>  
Phantom section: Flat Section  
Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2011)

DASY52 Configuration:


- Probe: EX3DV4 - SN7349; ConvF(10.1, 10.1, 10.1); Calibrated: 30.12.2014;
- Sensor-Surface: 1.4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn601; Calibrated: 17.08.2015
- Phantom: Flat Phantom 4.9L; Type: QD000P49AA; Serial: 1001
- DASY52 52.8.8(1222); SEMCAD X 14.6.10(7331)

**Dipole Calibration for Head Tissue/Pin=250 mW, d=15mm/Zoom Scan (7x7x7)/Cube 0:**

Measurement grid: dx=5mm, dy=5mm, dz=5mm  
Reference Value = 58.25 V/m; Power Drift = 0.04 dB  
Peak SAR (extrapolated) = 3.11 W/kg  
**SAR(1 g) = 2.06 W/kg; SAR(10 g) = 1.35 W/kg**  
Maximum value of SAR (measured) = 2.77 W/kg

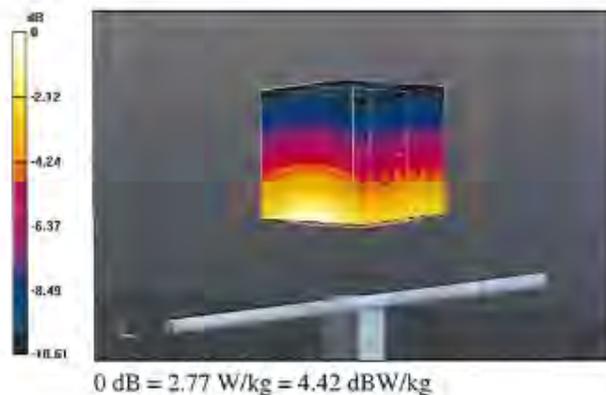

### Impedance Measurement Plot for Head TSL

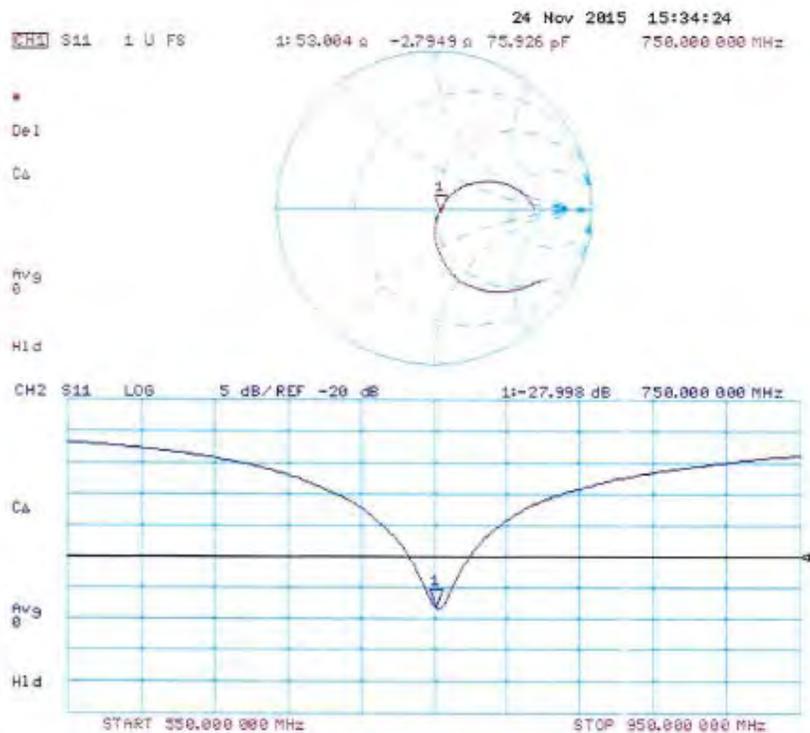

**DASY5 Validation Report for Body TSL**

Date: 24.11.2015

Test Laboratory: SPEAG, Zurich, Switzerland

**DUT: Dipole 750 MHz; Type: D750V3; Serial: D750V3 - SN: 1098**


Communication System: UID 0 - CW; Frequency: 750 MHz  
 Medium parameters used:  $f = 750$  MHz;  $\sigma = 0.97$  S/m;  $\epsilon_r = 55.9$ ;  $\rho = 1000$  kg/m<sup>3</sup>  
 Phantom section: Flat Section  
 Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2011)

**DASY52 Configuration:**


- Probe: EX3DV4 - SN7349; ConvF(9.61, 9.61, 9.61); Calibrated: 30.12.2014;
- Sensor-Surface: 1.4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn601; Calibrated: 17.08.2015
- Phantom: Flat Phantom 4.9L; Type: QD000P49AA; Serial: 1001
- DASY52 52.8.8(1222); SEMCAD X 14.6.10(7331)

**Dipole Calibration for Body Tissue/Pin=250 mW, d=15mm/Zoom Scan (7x7x7)/Cube 0:**

Measurement grid: dx=5mm, dy=5mm, dz=5mm  
 Reference Value = 57.88 V/m; Power Drift = 0.00 dB  
 Peak SAR (extrapolated) = 3.27 W/kg  
**SAR(1 g) = 2.23 W/kg; SAR(10 g) = 1.48 W/kg**  
 Maximum value of SAR (measured) = 2.92 W/kg

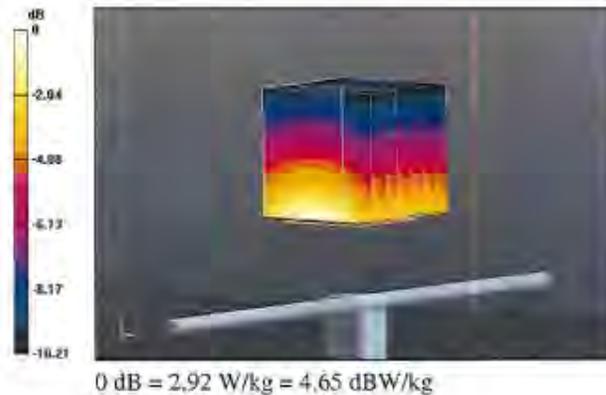

### Impedance Measurement Plot for Body TSL

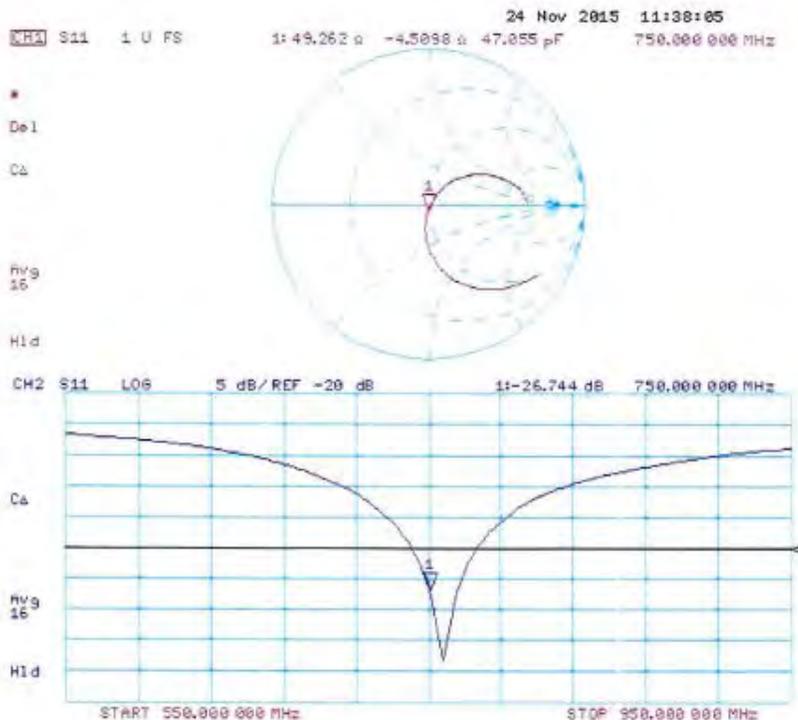

**Calibration Laboratory of  
Schmid & Partner  
Engineering AG**  
Zaughausstrasse 43, 8004 Zurich, Switzerland



**S** Schweizerischer Kalibrierdienst  
**C** Service suisse d'étalonnage  
**S** Servizio svizzero di taratura  
**S** Swiss Calibration Service

Accredited by the Swiss Accreditation Service (SAS)  
The Swiss Accreditation Service is one of the signatories to the EA  
Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: **SCS 0108**

Client: **Motorola Solutions MY**

Certificate No: **D900V2-1d026\_Jan17**

**CALIBRATION CERTIFICATE**

Object: **D900V2 - SN:1d026**

Calibration procedure(s): **QA CAL-05.v9  
Calibration procedure for dipole validation kits above 700 MHz**

Calibration date: **January 18, 2017**

This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI).  
The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility: environment temperature (22 ± 3)°C and humidity < 70%.

Calibration Equipment used (M&E critical for calibration)

Primary Standards	ID #	Cal Date (Certificate No.)	Scheduled Calibration
Power meter NRP	SN: 104778	06-Apr-16 (No. 217-02288/02289)	Apr-17
Power sensor NRP-Z91	SN: 103244	06-Apr-16 (No. 217-02288)	Apr-17
Power sensor NRP-Z91	SN: 103245	06-Apr-16 (No. 217-02289)	Apr-17
Reference 20 dB Attenuator	SN: 5058 (20k)	05-Apr-16 (No. 217-02292)	Apr-17
Type-N mismatch combination	SN: 5047.2 / 06327	05-Apr-16 (No. 217-02295)	Apr-17
Reference Probe EX3DV4	SN: 7349	31-Dec-16 (No. EX3-7349_Dec16)	Dec-17
D4E4	SN: 601	04-Jan-17 (No. DAE4-601_Jan17)	Jan-18
Secondary Standards	ID #	Check Date (in house)	Scheduled Check
Power meter EPM-442A	SN: GB37480704	07-Oct-15 (in house check Oct-16)	In house check: Oct-18
Power sensor HP 8481A	SN: US37292783	07-Oct-15 (in house check Oct-16)	In house check: Oct-18
Power sensor HP 8481A	SN: MY41D92317	07-Oct-15 (in house check Oct-16)	In house check: Oct-18
RF generator R&S SMT-06	SN: 100972	15-Jun-15 (in house check Oct-16)	In house check: Oct-18
Network Analyzer HP 8753E	SN: US37390585	18-Oct-01 (in house check Oct-16)	In house check: Oct-17

Calibrated by:	Name: Johannes Kuricka	Function: Laboratory Technician	Signature:
Approved by:	Name: Katja Pokovic	Function: Technical Manager	Signature:

Issued: January 20, 2017

This calibration certificate shall not be reproduced except in full without written approval of the laboratory.

**Calibration Laboratory of  
Schmid & Partner  
Engineering AG**  
Zeughausstrasse 43, 8004 Zurich, Switzerland



**S** Schweizerischer Kalibrierdienst  
**S** Service suisse d'étalonnage  
**C** Servizio svizzero di taratura  
**S** Swiss Calibration Service

Accredited by the Swiss Accreditation Service (SAS)  
The Swiss Accreditation Service is one of the signatories to the EA  
Multilateral Agreement for the recognition of calibration certificates.

Accreditation No.: **SCS 0108**

**Glossary:**

TSL tissue simulating liquid  
ConvF sensitivity in TSL / NORM x,y,z  
N/A not applicable or not measured

**Calibration is Performed According to the Following Standards:**

- a) IEEE Std 1528-2013, "IEEE Recommended Practice for Determining the Peak Spatial-Averaged Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques", June 2013
- b) IEC 62209-1, "Procedure to measure the Specific Absorption Rate (SAR) for hand-held devices used in close proximity to the ear (frequency range of 300 MHz to 3 GHz)", February 2005
- c) IEC 62209-2, "Procedure to determine the Specific Absorption Rate (SAR) for wireless communication devices used in close proximity to the human body (frequency range of 30 MHz to 6 GHz)", March 2010
- d) KDB 865664, "SAR Measurement Requirements for 100 MHz to 6 GHz"

**Additional Documentation:**

- e) DASY4/5 System Handbook

**Methods Applied and Interpretation of Parameters:**

- *Measurement Conditions:* Further details are available from the Validation Report at the end of the certificate. All figures stated in the certificate are valid at the frequency indicated.
- *Antenna Parameters with TSL:* The dipole is mounted with the spacer to position its feed point exactly below the center marking of the flat phantom section, with the arms oriented parallel to the body axis.
- *Feed Point Impedance and Return Loss:* These parameters are measured with the dipole positioned under the liquid filled phantom. The impedance stated is transformed from the measurement at the SMA connector to the feed point. The Return Loss ensures low reflected power. No uncertainty required.
- *Electrical Delay:* One-way delay between the SMA connector and the antenna feed point. No uncertainty required.
- *SAR measured:* SAR measured at the stated antenna input power.
- *SAR normalized:* SAR as measured, normalized to an input power of 1 W at the antenna connector.
- *SAR for nominal TSL parameters:* The measured TSL parameters are used to calculate the nominal SAR result.

The reported uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor k=2, which for a normal distribution corresponds to a coverage probability of approximately 95%.

**Measurement Conditions**

DASY system configuration, as far as not given on page 1.

DASY Version	DASY5	V52.8.8
Extrapolation	Advanced Extrapolation	
Phantom	Modular Flat Phantom	
Distance Dipole Center - TSL	15 mm	with Spacer
Zoom Scan Resolution	dx, dy, dz = 5 mm	
Frequency	900 MHz ± 1 MHz	

**Head TSL parameters**

The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Head TSL parameters	22.0 °C	41.5	0.97 mho/m
Measured Head TSL parameters	(22.0 ± 0.2) °C	41.2 ± 6 %	0.94 mho/m ± 6 %
Head TSL temperature change during test	< 0.5 °C	---	---

**SAR result with Head TSL**

SAR averaged over 1 cm <sup>3</sup> (1 g) of Head TSL	Condition	
SAR measured	250 mW input power	2.66 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	10.9 W/kg ± 17.0 % (k=2)

SAR averaged over 10 cm <sup>3</sup> (10 g) of Head TSL	condition	
SAR measured	250 mW input power	1.70 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	6.92 W/kg ± 16.5 % (k=2)

**Body TSL parameters**

The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Body TSL parameters	22.0 °C	55.0	1.05 mho/m
Measured Body TSL parameters	(22.0 ± 0.2) °C	53.8 ± 6 %	1.02 mho/m ± 6 %
Body TSL temperature change during test	< 0.5 °C	---	---

**SAR result with Body TSL**

SAR averaged over 1 cm <sup>3</sup> (1 g) of Body TSL	Condition	
SAR measured	250 mW input power	2.71 W/kg
SAR for nominal Body TSL parameters	normalized to 1W	11.0 W/kg ± 17.0 % (k=2)

SAR averaged over 10 cm <sup>3</sup> (10 g) of Body TSL	condition	
SAR measured	250 mW input power	1.75 W/kg
SAR for nominal Body TSL parameters	normalized to 1W	7.10 W/kg ± 16.5 % (k=2)

**Appendix (Additional assessments outside the scope of SCS 0108)**

**Antenna Parameters with Head TSL**

Impedance, transformed to feed point	50.6 Ω - 0.2 jΩ
Return Loss	- 43.5 dB

**Antenna Parameters with Body TSL**

Impedance, transformed to feed point	46.7 Ω - 2.3 jΩ
Return Loss	- 27.5 dB

**General Antenna Parameters and Design**

Electrical Delay (one direction)	1.395 ns
----------------------------------	----------

After long term use with 100W radiated power, only a slight warming of the dipole near the feedpoint can be measured.

The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals. On some of the dipoles, small end caps are added to the dipole arms in order to improve matching when loaded according to the position as explained in the "Measurement Conditions" paragraph. The SAR data are not affected by this change. The overall dipole length is still according to the Standard.

No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feedpoint may be damaged.

**Additional EUT Data**

Manufactured by	SPEAG
Manufactured on	February 08, 2005

**DASY5 Validation Report for Head TSL**

Date: 16.01.2017

Test Laboratory: SPEAG, Zurich, Switzerland

**DUT: Dipole 900 MHz; Type: D900V2; Serial: D900V2 - SN:1d026**


Communication System: UID 0 - CW; Frequency: 900 MHz  
 Medium parameters used:  $f = 900 \text{ MHz}$ ;  $\sigma = 0.94 \text{ S/m}$ ;  $\epsilon_r = 41.2$ ;  $\rho = 1000 \text{ kg/m}^3$   
 Phantom section: Flat Section  
 Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2011)

**DASY52 Configuration:**


- Probe: EX3DV4 - SN7349; ConvF(9.7, 9.7, 9.7); Calibrated: 31.12.2016;
- Sensor-Surface: 1.4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn601; Calibrated: 04.01.2017
- Phantom: Flat Phantom 4.9 (front); Type: QD 00L P49 AA; Serial: 1001
- DASY52 52.8.8(1258); SEMCAD X 14.6.10(7372)

**Dipole Calibration for Head Tissue/Pin=250 mW, d=15mm/Zoom Scan (7x7x7)/Cube 0:**

Measurement grid:  $dx=5\text{mm}$ ,  $dy=5\text{mm}$ ,  $dz=5\text{mm}$   
 Reference Value = 64.94 V/m; Power Drift = 0.01 dB  
 Peak SAR (extrapolated) = 4.18 W/kg  
**SAR(1 g) = 2.66 W/kg; SAR(10 g) = 1.7 W/kg**  
 Maximum value of SAR (measured) = 3.63 W/kg

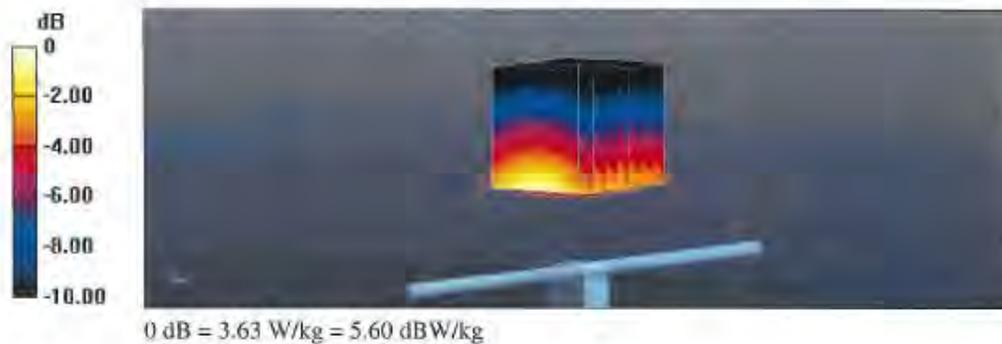

### Impedance Measurement Plot for Head TSL

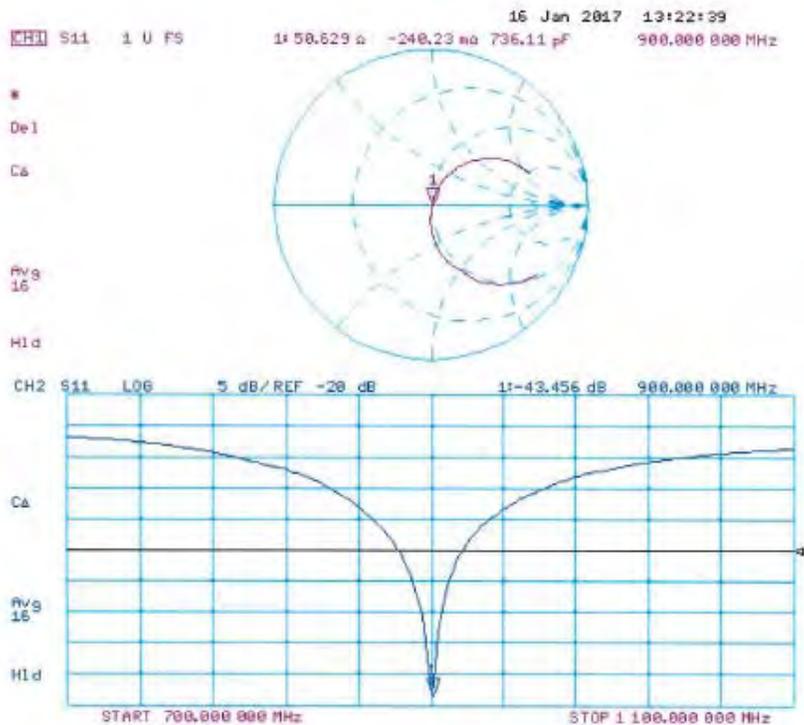

**DASY5 Validation Report for Body TSL**

Date: 18.01.2017

Test Laboratory: SPEAG, Zurich, Switzerland

**DUT: Dipole 900 MHz; Type: D900V2; Serial: D900V2 - SN:1d026**


Communication System: UID 0 - CW; Frequency: 900 MHz  
 Medium parameters used:  $f = 900 \text{ MHz}$ ;  $\sigma = 1.02 \text{ S/m}$ ;  $\epsilon_r = 53.8$ ;  $\rho = 1000 \text{ kg/m}^3$   
 Phantom section: Flat Section  
 Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2011)

**DASY52 Configuration:**


- Probe: EX3DV4 - SN7349; ConvF(9.64, 9.64, 9.64); Calibrated: 31.12.2016;
- Sensor-Surface: 1.4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn601; Calibrated: 04.01.2017
- Phantom: Flat Phantom 4.9 (Back); Type: QD 00R P49 AA; Serial: 1005
- DASY52 52.8.8(1258); SEMCAD X 14.6.10(7372)

**Dipole Calibration for Body Tissue/Pin=250 mW, d=15mm/Zoom Scan (7x7x7)/Cube 0:**

Measurement grid:  $dx=5\text{mm}$ ,  $dy=5\text{mm}$ ,  $dz=5\text{mm}$   
 Reference Value = 62.82 V/m; Power Drift = -0.01 dB  
 Peak SAR (extrapolated) = 4.11 W/kg  
**SAR(1 g) = 2.71 W/kg; SAR(10 g) = 1.75 W/kg**  
 Maximum value of SAR (measured) = 3.63 W/kg

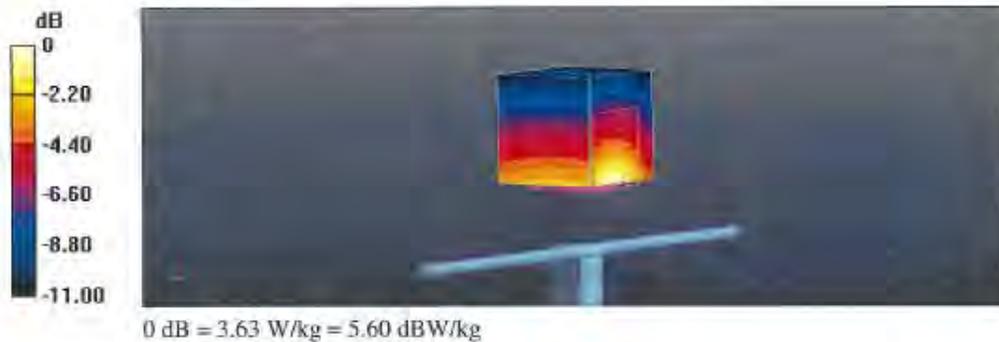

### Impedance Measurement Plot for Body TSL

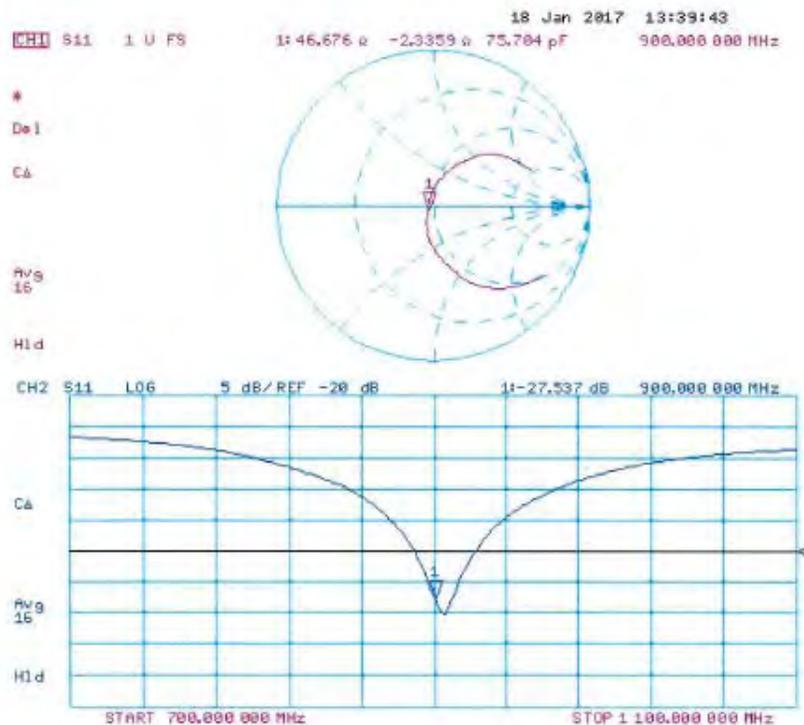

## Dipole Data

As stated in KDB 865664, for dipole exceeded annual calibration, the test laboratory must ensure that the required supporting information and documentation are included in report to qualify for extended calibration interval.

The table below includes dipole impedance and return loss measurement data measured by Motorola Solutions' EME lab. The results meet requirements stated in KDB 865664.

Dipole D450V3 (SN 1077)	Head			Body		
	Impedance		Return Loss	Impedance		Return Loss
Date Measured	real $\Omega$	imag $j\Omega$	dB	real $\Omega$	imag $j\Omega$	dB
06/28/2016	58.87	-2.93	-22.48	50.59	-6.61	-22.25
12/01/2016	59.08	-2.93	-22.65	51.05	-7.45	-22.63

Dipole D750V3 (SN 1098)	Head			Body		
	Impedance		Return Loss	Impedance		Return Loss
Date Measured	real $\Omega$	imag $j\Omega$	dB	real $\Omega$	imag $j\Omega$	dB
06/24/2016	47.61	-2.13	-28.03	49.37	-2.23	-26.10
10/30/2016	48.81	-2.69	-27.25	47.99	-1.98	-30.77

## **APPENDIX D**

### **System Verification Check Scans**

**Motorola Solutions, Inc. EME Laboratory**  
Date/Time: 7/12/2017 7:23:09 AM

Robot#: DASY5-PG-2 | Run#: ZR-SYSP-750B-170712-04  
 Dipole Model# D750V3  
 Phantom#: ELI4 1090  
 Tissue Temp: 21.1 (C)  
 Serial#: 1098  
 Test Freq: 750.0000 (MHz)  
 Start Power: 250 (mW)  
 Rotation (1D): 0.035 dB  
 Adjusted SAR (1W): 8.76 mW/g (1g)

Comments:

Duty Cycle: 1:1, Medium parameters used:  $f = 750 \text{ MHz}$ ;  $\sigma = 0.92 \text{ S/m}$ ;  $\epsilon_r = 56.2$ ;  $\rho = 1000 \text{ kg/m}^3$   
 Probe: ES3DV3 - SN3122, , Frequency: 750 MHz, ConvF(6.34, 6.34, 6.34); Calibrated: 3/10/2017  
 Electronics: DAE4 Sn850, Calibrated: 2/28/2017

**Below 2 GHz-Rev.2/System Performance Check/Dipole Area Scan 2 (41x131x1):**



Interpolated grid:  $dx=1.500 \text{ mm}$ ,  $dy=1.500 \text{ mm}$   
 Reference Value = 53.56 V/m; Power Drift = -0.10 dB  
 Fast SAR: SAR(1 g) = 2.19 W/kg; SAR(10 g) = 1.45 W/kg (SAR corrected for target medium)  
 Maximum value of SAR (interpolated) = 2.43 W/kg

**Below 2 GHz-Rev.2/System Performance Check/0-Degree Cube (5x5x7)/Cube 0:**

Measurement grid:  $dx=7.5\text{mm}$ ,  $dy=7.5\text{mm}$ ,  $dz=5\text{mm}$   
 Reference Value = 53.56 V/m; Power Drift = -0.10 dB  
 Peak SAR (extrapolated) = 3.03 W/kg  
 SAR(1 g) = 2.18 W/kg; SAR(10 g) = 1.46 W/kg (SAR corrected for target medium)  
 Maximum value of SAR (measured) = 2.43 W/kg

**Below 2 GHz-Rev.2/System Performance Check/Z-Axis Retraction (1x1x17): Measurement**

grid:  $dx=20\text{mm}$ ,  $dy=20\text{mm}$ ,  $dz=10\text{mm}$   
 Maximum value of SAR (measured) = 2.44 W/kg

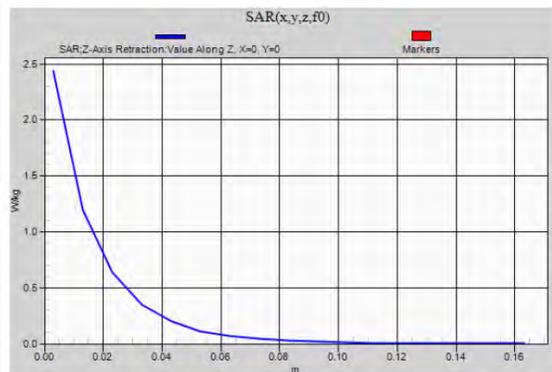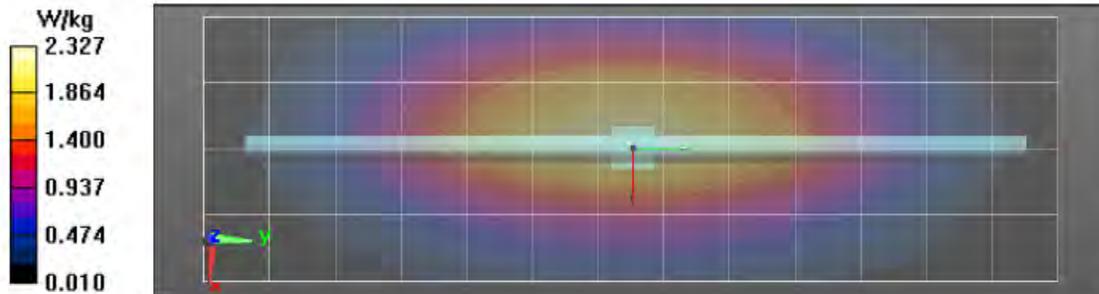

**Motorola Solutions, Inc. EME Laboratory**  
Date/Time: 7/15/2017 11:01:25 AM

Robot#: DASY5-PG-2 | Run#: ZR-SYSP-450B-170715-06  
 Dipole Model#: D450V3  
 Phantom#: ELI4 1103  
 Tissue Temp: 21.5 (C)  
 Serial#: 1077  
 Test Freq: 450.0000 (MHz)  
 Start Power: 250 (mW)  
 Rotation (1D): 0.041 dB  
 Adjusted SAR (1W): 4.64 mW/g (1g)

Comments:

Duty Cycle: 1:1, Medium parameters used:  $f = 450$  MHz;  $\sigma = 0.95$  S/m;  $\epsilon_r = 56.3$ ;  $\rho = 1000$  kg/m<sup>3</sup>  
 Probe: ES3DV3 - SN3122, , Frequency: 450 MHz, ConvF(7.1, 7.1, 7.1); Calibrated: 3/10/2017  
 Electronics: DAE4 Sn850, Calibrated: 2/28/2017



**Below 2 GHz-Rev.2/System Performance Check/Dipole Area Scan 2 (41x201x1):**

Interpolated grid: dx=1.500 mm, dy=1.500 mm  
 Reference Value = 38.27 V/m; Power Drift = -0.08 dB  
 Fast SAR: SAR(1 g) = 1.19 W/kg; SAR(10 g) = 0.826 W/kg (SAR corrected for target medium)  
 Maximum value of SAR (interpolated) = 1.37 W/kg

**Below 2 GHz-Rev.2/System Performance Check/0-Degree Cube (5x5x7)/Cube 0:**

Measurement grid: dx=7.5mm, dy=7.5mm, dz=5mm  
 Reference Value = 38.27 V/m; Power Drift = -0.08 dB  
 Peak SAR (extrapolated) = 1.86 W/kg  
 SAR(1 g) = 1.16 W/kg; SAR(10 g) = 0.770 W/kg (SAR corrected for target medium)  
 Maximum value of SAR (measured) = 1.36 W/kg

**Below 2 GHz-Rev.2/System Performance Check/Z-Axis Retraction (1x1x17):** Measurement grid: dx=20mm, dy=20mm, dz=10mm

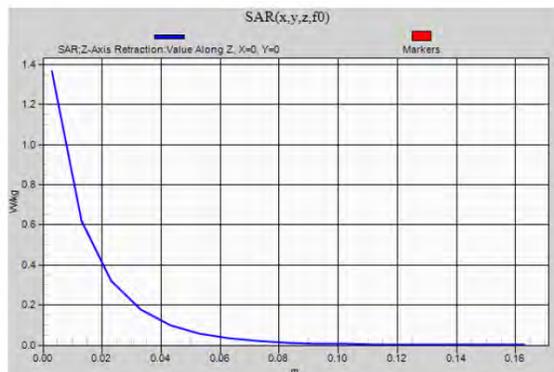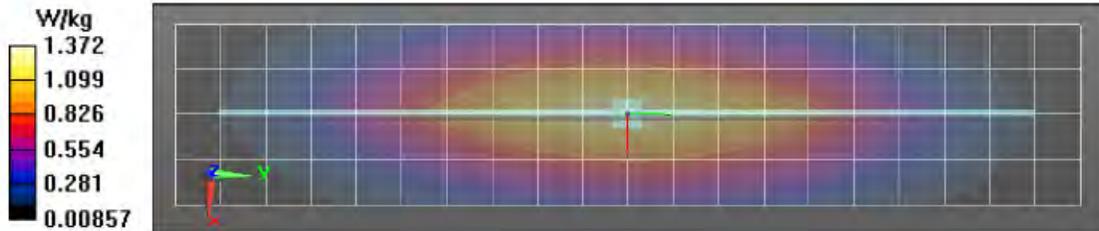

**Motorola Solutions, Inc. EME Laboratory**

Date/Time: 7/17/2017 7:23:57 PM

Robot#: DASY5-PG-2 | Run#: ZR-SYSP-150B-170717-12  
 Dipole Model#: CLA 150  
 Phantom#: ELI4 1011  
 Tissue Temp: 21.1 (C)  
 Serial#: 4010  
 Test Freq: 150.0000 (MHz)  
 Start Power: 1000 (mW)  
 Rotation (1D): 0.055 dB  
 Adjusted SAR (1W): 3.96 mW/g (1g)

Comments:

Duty Cycle: 1:1, Medium parameters used:  $f = 150$  MHz;  $\sigma = 0.77$  S/m;  $\epsilon_r = 59.3$ ;  $\rho = 1000$  kg/m<sup>3</sup>  
 Probe: ES3DV3 - SN3122, Frequency: 150 MHz, ConvF(6.91, 6.91, 6.91); Calibrated: 3/10/2017  
 Electronics: DAE4 Sn850, Calibrated: 2/28/2017

**Below 2 GHz-Rev.2/System Performance Check/Dipole Area Scan 2 (81x81x1):**



Interpolated grid: dx=1.500 mm, dy=1.500 mm  
 Reference Value = 77.19 V/m; Power Drift = 0.01 dB  
 Fast SAR: SAR(1 g) = 4.2 W/kg; SAR(10 g) = 3.01 W/kg (SAR corrected for target medium)  
 Maximum value of SAR (interpolated) = 4.61 W/kg

**Below 2 GHz-Rev.2/System Performance Check/0-Degree Cube (5x6x7)/Cube 0:**

Measurement grid: dx=7.5mm, dy=7.5mm, dz=5mm  
 Reference Value = 77.19 V/m; Power Drift = 0.01 dB  
 Peak SAR (extrapolated) = 6.51 W/kg  
 SAR(1 g) = 3.96 W/kg; SAR(10 g) = 2.59 W/kg (SAR corrected for target medium)  
 Maximum value of SAR (measured) = 4.54 W/kg

**Below 2 GHz-Rev.2/System Performance Check/Z-Axis Retraction (1x1x17): Measurement**

grid: dx=20mm, dy=20mm, dz=10mm  
 Maximum value of SAR (measured) = 4.57 W/kg

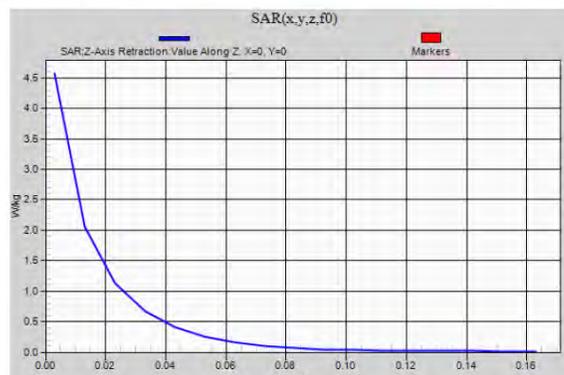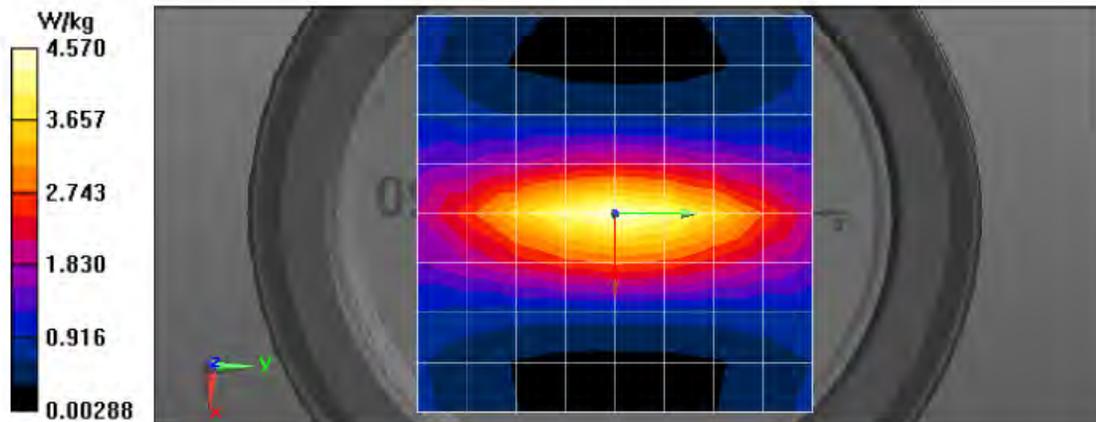

**Motorola Solutions, Inc. EME Laboratory**  
Date/Time: 7/18/2017 10:37:23 AM

Robot#: DASY5-PG-2 | Run#: FD-SYSP-750H-170718-11  
 Dipole Model#: D750V3  
 Phantom#: ELI4 1037  
 Tissue Temp: 21.7 (C)  
 Serial#: 1098  
 Test Freq: 750.0000 (MHz)  
 Start Power: 250 (mW)  
 Rotation (1D): 0.040 dB  
 Adjusted SAR (1W): 8.40 mW/g (1g)

**Comments:**

Duty Cycle: 1:1, Medium parameters used:  $f = 750$  MHz;  $\sigma = 0.85$  S/m;  $\epsilon_r = 43.2$ ;  $\rho = 1000$  kg/m<sup>3</sup>  
 Probe: ES3DV3 - SN3122, , Frequency: 750 MHz, ConvF(6.62, 6.62, 6.62); Calibrated: 3/10/2017  
 Electronics: DAE4 Sn850, Calibrated: 2/28/2017

**Below 2 GHz-Rev.2/System Performance Check/Dipole Area Scan 2 (41x141x1):**



Interpolated grid: dx=1.500 mm, dy=1.500 mm  
 Reference Value = 53.76 V/m; Power Drift = -0.02 dB  
 Fast SAR: SAR(1 g) = 2.1 W/kg; SAR(10 g) = 1.39 W/kg (SAR corrected for target medium)  
 Maximum value of SAR (interpolated) = 2.33 W/kg

**Below 2 GHz-Rev.2/System Performance Check/0-Degree Cube (5x5x7)/Cube 0:**

Measurement grid: dx=7.5mm, dy=7.5mm, dz=5mm  
 Reference Value = 53.76 V/m; Power Drift = -0.02 dB  
 Peak SAR (extrapolated) = 3.02 W/kg  
 SAR(1 g) = 2.1 W/kg; SAR(10 g) = 1.38 W/kg (SAR corrected for target medium)  
 Maximum value of SAR (measured) = 2.35 W/kg

**Below 2 GHz-Rev.2/System Performance Check/Z-Axis Retraction (1x1x17): Measurement**

grid: dx=20mm, dy=20mm, dz=10mm  
 Maximum value of SAR (measured) = 2.36 W/kg

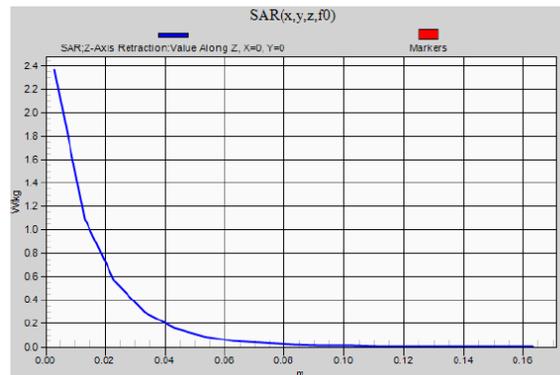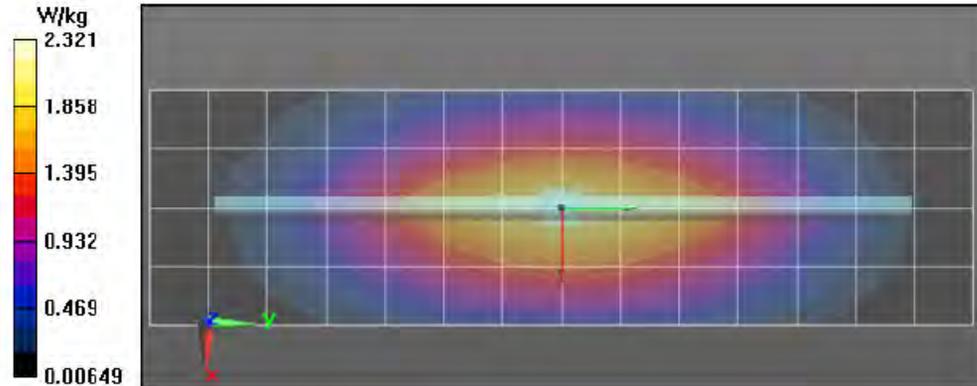

**Motorola Solutions, Inc. EME Laboratory**  
Date/Time: 8/3/2017 3:34:09 AM

Robot#: DASY5-PG-2 | Run#: ZR(AN)-SYSP-450H-170803-03  
 Dipole Model#: D450V3  
 Phantom#: ELI4 1109  
 Tissue Temp: 21.0 (C)  
 Serial#: 1077  
 Test Freq: 450.0000 (MHz)  
 Start Power: 250 (mW)  
 Rotation (1D): 0.21 dB  
 Adjusted SAR (1W): 4.68 mW/g (1g)

Comments:

Duty Cycle: 1:1, Medium parameters used:  $f = 450$  MHz;  $\sigma = 0.88$  S/m;  $\epsilon_r = 43.7$ ;  $\rho = 1000$  kg/m<sup>3</sup>  
 Probe: ES3DV3 - SN3122, Frequency: 450 MHz, ConvF(7, 7, 7); Calibrated: 3/10/2017  
 Electronics: DAE4 Sn850, Calibrated: 2/28/2017



**Below 2 GHz-Rev.2/System Performance Check/Dipole Area Scan 2 (41x201x1):**

Interpolated grid: dx=1.500 mm, dy=1.500 mm  
 Reference Value = 39.90 V/m; Power Drift = -0.03 dB  
 Fast SAR: SAR(1 g) = 1.2 W/kg; SAR(10 g) = 0.831 W/kg (SAR corrected for target medium)  
 Maximum value of SAR (interpolated) = 1.37 W/kg

**Below 2 GHz-Rev.2/System Performance Check/0-Degree Cube (5x5x7)/Cube 0:**

Measurement grid: dx=7.5mm, dy=7.5mm, dz=5mm  
 Reference Value = 39.90 V/m; Power Drift = -0.03 dB  
 Peak SAR (extrapolated) = 1.90 W/kg  
 SAR(1 g) = 1.17 W/kg; SAR(10 g) = 0.770 W/kg (SAR corrected for target medium)  
 Maximum value of SAR (measured) = 1.38 W/kg

**Below 2 GHz-Rev.2/System Performance Check/Z-Axis Retraction (1x1x17):** Measurement grid: dx=20mm, dy=20mm, dz=10mm

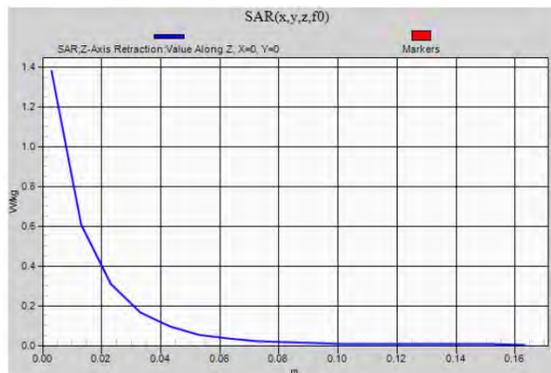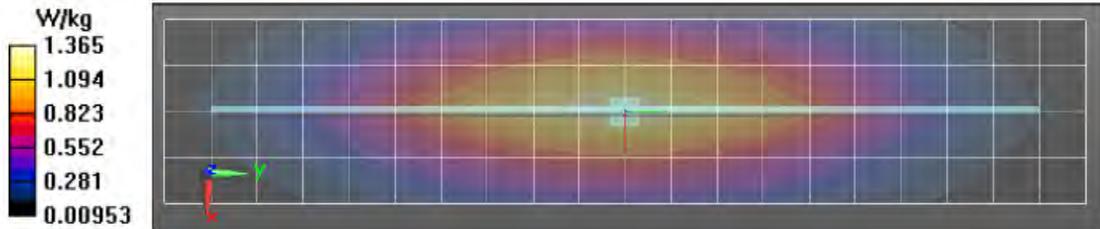

**Motorola Solutions, Inc. EME Laboratory**

Date/Time: 8/3/2017 4:16:15 PM

Robot#: DASY5-PG-2 | Run#: FD(HR-SYSP-150H-170803-10  
 Dipole Model# CLA150  
 Phantom#: ELI4 1022  
 Tissue Temp: 20.4 (C)  
 Serial#: 4010  
 Test Freq: 150.0000 (MHz)  
 Start Power: 1000 (mW)  
 Rotation (1D): 0.031 dB  
 Adjusted SAR (1W): 3.64mW/g (1g)

Comments:

Duty Cycle: 1:1, Medium parameters used:  $f = 150$  MHz;  $\sigma = 0.74$  S/m;  $\epsilon_r = 52.5$ ;  $\rho = 1000$  kg/m<sup>3</sup>  
 Probe: ES3DV3 - SN3122, Frequency: 150 MHz, ConvF(7.36, 7.36, 7.36); Calibrated: 3/10/2017  
 Electronics: DAE4 Sn850, Calibrated: 2/28/2017

**Below 2 GHz-Rev.2/System Performance Check/Dipole Area Scan 2 (81x81x1):**



Interpolated grid: dx=1.500 mm, dy=1.500 mm  
 Reference Value = 75.05 V/m; Power Drift = -0.05 dB  
 Fast SAR: SAR(1 g) = 3.89 W/kg; SAR(10 g) = 2.79 W/kg (SAR corrected for target medium)  
 Maximum value of SAR (interpolated) = 4.23 W/kg

**Below 2 GHz-Rev.2/System Performance Check/0-Degree Cube (5x5x7)/Cube 0:**

Measurement grid: dx=7.5mm, dy=7.5mm, dz=5mm  
 Reference Value = 75.05 V/m; Power Drift = -0.05 dB  
 Peak SAR (extrapolated) = 6.11 W/kg  
 SAR(1 g) = 3.64 W/kg; SAR(10 g) = 2.36 W/kg (SAR corrected for target medium)  
 Maximum value of SAR (measured) = 4.18 W/kg

**Below 2 GHz-Rev.2/System Performance Check/Z-Axis Retraction (1x1x17):** Measurement

grid: dx=20mm, dy=20mm, dz=10mm

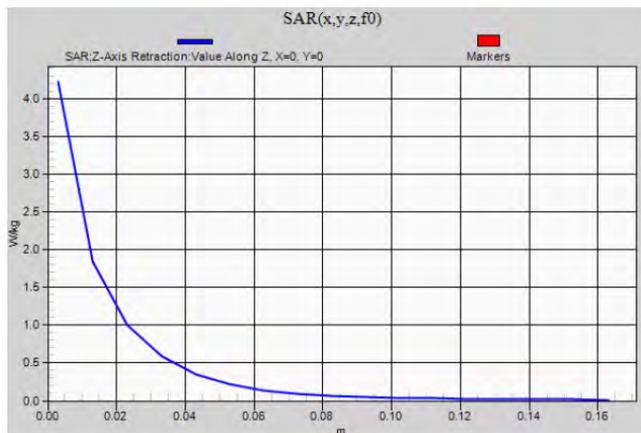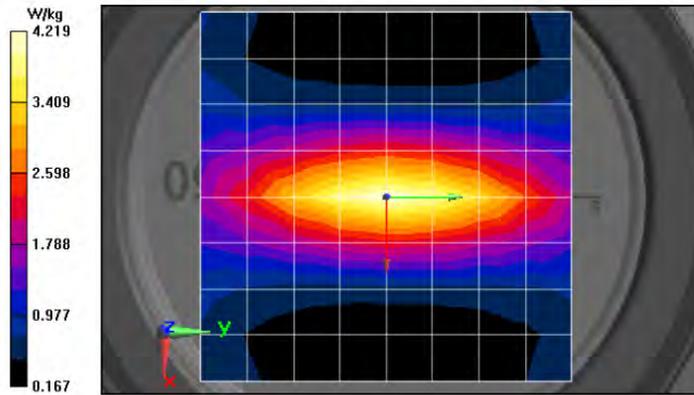

**Motorola Solutions, Inc. EME Laboratory**  
Date/Time: 8/7/2017 9:16:50 PM

Robot#: DASY5-PG-2 | Run#: TLC(HR)-SYSP-450B-170807-05  
 Dipole Model# D450V3  
 Phantom#: ELI4 1103  
 Tissue Temp: 20.8 (C)  
 Serial#: 1077  
 Test Freq: 450.0000 (MHz)  
 Start Power: 250 (mW)  
 Rotation (1D): 0.023dB  
 Adjusted SAR (1W): 4.64mW/g (1g)

Comments:

Duty Cycle: 1:1, Medium parameters used:  $f = 450$  MHz;  $\sigma = 0.93$  S/m;  $\epsilon_r = 56.1$ ;  $\rho = 1000$  kg/m<sup>3</sup>  
 Probe: ES3DV3 - SN3122, , Frequency: 450 MHz, ConvF(7.1, 7.1, 7.1); Calibrated: 3/10/2017  
 Electronics: DAE4 Sn850, Calibrated: 2/28/2017

**Below 2 GHz-Rev.2/System Performance Check/Dipole Area Scan 2 (41x201x1):**



Interpolated grid: dx=1.500 mm, dy=1.500 mm  
 Reference Value = 38.19 V/m; Power Drift = -0.02 dB  
 Fast SAR: SAR(1 g) = 1.19 W/kg; SAR(10 g) = 0.823 W/kg (SAR corrected for target medium)  
 Maximum value of SAR (interpolated) = 1.35 W/kg

**Below 2 GHz-Rev.2/System Performance Check/0-Degree Cube (5x5x7)/Cube 0:**

Measurement grid: dx=7.5mm, dy=7.5mm, dz=5mm  
 Reference Value = 38.19 V/m; Power Drift = -0.02 dB  
 Peak SAR (extrapolated) = 1.84 W/kg  
 SAR(1 g) = 1.16 W/kg; SAR(10 g) = 0.774 W/kg (SAR corrected for target medium)

**Below 2 GHz-Rev.2/System Performance Check/Z-Axis Retraction (1x1x17): Measurement**

grid: dx=20mm, dy=20mm, dz=10mm

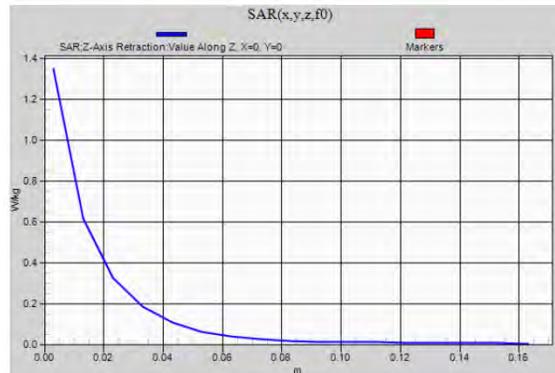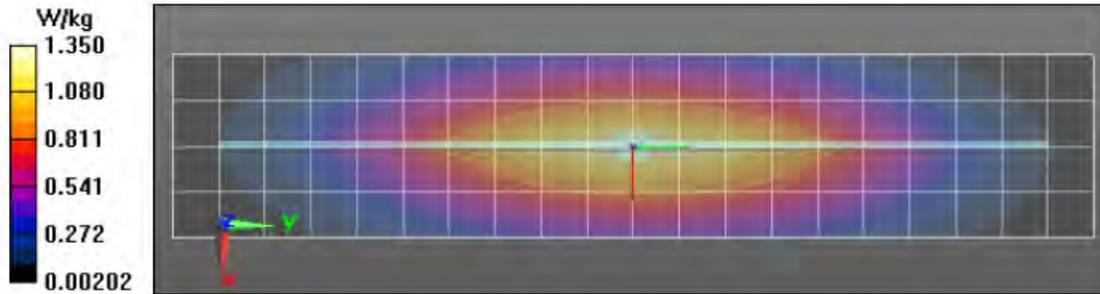

**Motorola Solutions, Inc. EME Laboratory**  
Date/Time: 8/10/2017 9:59:35 PM

Robot#: DASY5-PG-2 | Run#: FD(HR)-SYSP-900H-170810-01  
 Dipole Model#: 1d026  
 Phantom#: ELI4 1037  
 Tissue Temp: 21.0 (C)  
 Serial#: 1d026  
 Test Freq: 900.0000 (MHz)  
 Start Power: 250 (mW)  
 Rotation (1D): 0.017dB  
 Adjusted SAR (1W): 10.36mW/g (1g)

Comments:

Duty Cycle: 1:1, Medium parameters used:  $f = 900 \text{ MHz}$ ;  $\sigma = 0.99 \text{ S/m}$ ;  $\epsilon_r = 40.8$ ;  $\rho = 1000 \text{ kg/m}^3$   
 Probe: ES3DV3 - SN3122, Frequency: 900 MHz, ConvF(6.36, 6.36, 6.36); Calibrated: 3/10/2017  
 Electronics: DAE4 Sn850, Calibrated: 2/28/2017



**Below 2 GHz-Rev.2/System Performance Check/Dipole Area Scan 2 (41x131x1):**

Interpolated grid:  $dx=1.500 \text{ mm}$ ,  $dy=1.500 \text{ mm}$   
 Reference Value = 57.49 V/m; Power Drift = -0.01 dB  
 Fast SAR: SAR(1 g) = 2.63 W/kg; SAR(10 g) = 1.72 W/kg (SAR corrected for target medium)  
 Maximum value of SAR (interpolated) = 3.12 W/kg

**Below 2 GHz-Rev.2/System Performance Check/0-Degree Cube (5x5x7)/Cube 0:**

Measurement grid:  $dx=7.5\text{mm}$ ,  $dy=7.5\text{mm}$ ,  $dz=5\text{mm}$   
 Reference Value = 57.49 V/m; Power Drift = -0.01 dB  
 Peak SAR (extrapolated) = 4.06 W/kg  
 SAR(1 g) = 2.59 W/kg; SAR(10 g) = 1.66 W/kg (SAR corrected for target medium)  
 Maximum value of SAR (measured) = 3.12 W/kg

**Below 2 GHz-Rev.2/System Performance Check/Z-Axis Retraction (1x1x17):** Measurement grid:  $dx=20\text{mm}$ ,  $dy=20\text{mm}$ ,  $dz=10\text{mm}$

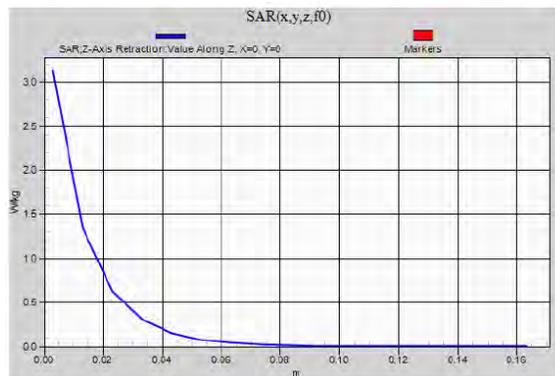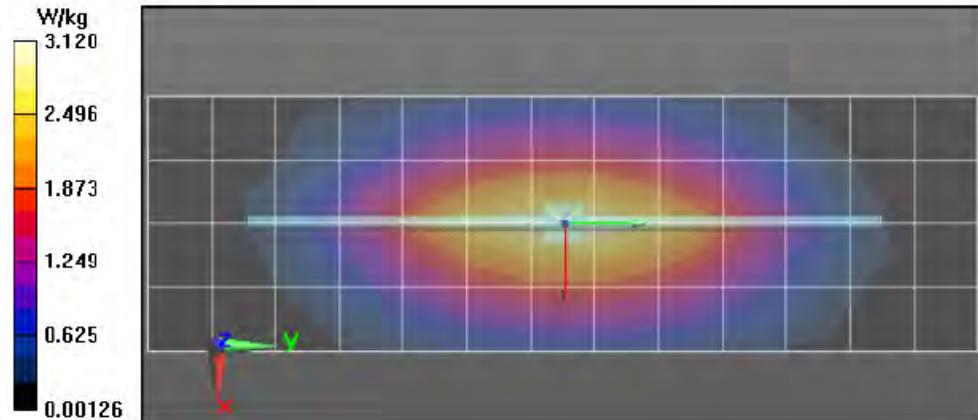

**APPENDIX E**  
**DUT Scans - (Shortened Scan and Highest SAR configurations)**

## Shortened Scan of Highest SAR configuration

Motorola Solutions, Inc. EME Laboratory

Date/Time: 8/11/2017 10:49:12 AM

Robot#: DASY5-PG-2 | Run#: ZR(AN)-FACE-170811-01#  
 Model#: H91TGD9PW7AN (PNUW1014C)  
 Phantom#: ELI4 1037  
 Tissue Temp: 20.6 (C)  
 Serial#: 579TTME980  
 Antenna: NAR6595A  
 Test Freq: 808.5000 (MHz)  
 Battery: NNTN7038B  
 Carry Acc: None; Radio at back  
 Audio Acc: None  
 Start Power: 3.60 (W)

Comments: Shorten scan


Duty Cycle: 1:1, Medium parameters used:  $f = 809 \text{ MHz}$ ;  $\sigma = 0.9 \text{ S/m}$ ;  $\epsilon_r = 42$ ;  $\rho = 1000 \text{ kg/m}^3$   
 Probe: ES3DV3 - SN3122, Frequency: 808.5 MHz, ConvF(6.62, 6.62, 6.62); Calibrated: 3/10/2017  
 Electronics: DAE4 Sn850, Calibrated: 2/28/2017

**Below 2 GHz-Rev.2/Face Scan/1-Area Scan (81x191x1):** Interpolated grid:  $dx=1.500 \text{ mm}$ ,  $dy=1.500 \text{ mm}$   
 Reference Value = 74.30 V/m; Power Drift = -0.27 dB  
 Fast SAR: SAR(1 g) = 6.61 W/kg; SAR(10 g) = 4.64 W/kg (SAR corrected for target medium)  
 Maximum value of SAR (interpolated) = 7.46 W/kg

**Below 2 GHz-Rev.2/Face Scan/2-Volume Scan 2D (41x41x1):** Interpolated grid:  $dx=0.7500 \text{ mm}$ ,  $dy=0.7500 \text{ mm}$ ,  $dz=1.000 \text{ mm}$   
 Reference Value = 74.30 V/m; Power Drift = -0.36 dB  
 Fast SAR: SAR(1 g) = 6.42 W/kg; SAR(10 g) = 4.6 W/kg (SAR corrected for target medium)  
 Maximum value of SAR (interpolated) = 7.17 W/kg

**Below 2 GHz-Rev.2/Face Scan/3-Zoom Scan (5x5x7)/Cube 0:** Measurement grid:  $dx=7.5 \text{ mm}$ ,  $dy=7.5 \text{ mm}$ ,  $dz=5 \text{ mm}$   
 Reference Value = 96.37 V/m; Power Drift = -0.12 dB  
 Peak SAR (extrapolated) = 9.16 W/kg  
 SAR(1 g) = 7.05 W/kg; SAR(10 g) = 5.22 W/kg (SAR corrected for target medium)  
 Maximum value of SAR (measured) = 7.80 W/kg

**Below 2 GHz-Rev.2/Face Scan/4-Z-Axis Scan (1x1x17):** Measurement grid:  $dx=20 \text{ mm}$ ,  $dy=20 \text{ mm}$ ,  $dz=10 \text{ mm}$   
 Maximum value of SAR (measured) = 7.05 W/kg

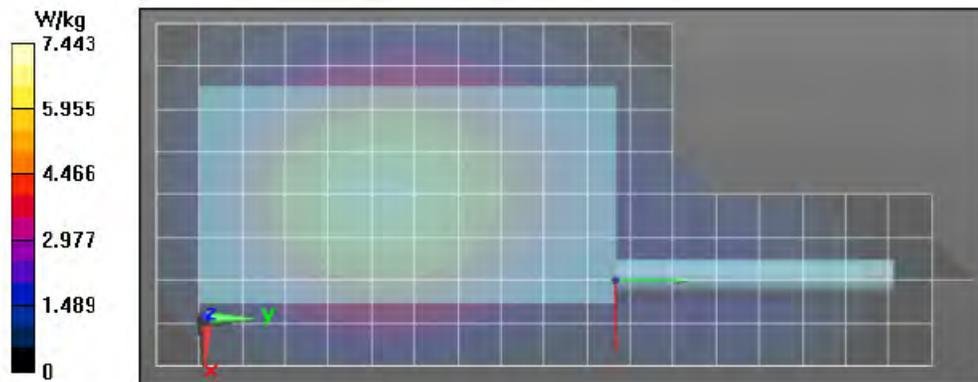

Shortened scan reflects highest SAR producing configuration and is compared to the full scan.

Scan Description	Referenced Table	Test Time (min.)	SAR 1g (W/kg)
Shorten scan (zoom)	19	8	3.62
Full scan (area & zoom)	18	25	3.42

## Highest Body SAR Configuration Results Table – 17; VHF

**Motorola Solutions, Inc. EME Laboratory**  
Date/Time: 7/17/2017 10:31:40 PM

Robot#: DASY5-PG-2 | Run#: ZR-AB-170717-15  
 Model#: H91TGD9PW5AN (PNUW1012C)  
 Phantom#: ELI4 1011  
 Tissue Temp: 20.9 (C)  
 Serial#: 579TTME968  
 Antenna: PMAT4001A  
 Test Freq: 139.7000 (MHz)  
 Battery: NNTN7573A  
 Carry Acc: HLN6875A  
 Audio Acc: None  
 Start Power: 6.52 (W)


**Comments:**

Duty Cycle: 1:1, Medium parameters used:  $f = 140$  MHz;  $\sigma = 0.76$  S/m;  $\epsilon_r = 59.5$ ;  $\rho = 1000$  kg/m<sup>3</sup>  
 Probe: ES3DV3 - SN3122, , Frequency: 139.7 MHz, ConvF(6.91, 6.91, 6.91); Calibrated: 3/10/2017  
 Electronics: DAE4 Sn850, Calibrated: 2/28/2017

**Below 2 GHz-Rev.2/Ab Scan/1-Area Scan (81x301x1):** Interpolated grid: dx=1.500 mm, dy=1.500 mm  
 Reference Value = 58.64 V/m; Power Drift = -0.41 dB  
**Fast SAR: SAR(1 g) = 12.2 W/kg; SAR(10 g) = 7.44 W/kg** (SAR corrected for target medium)  
 Maximum value of SAR (interpolated) = 15.7 W/kg

**Below 2 GHz-Rev.2/Ab Scan/3-Zoom Scan (6x6x7)/Cube 0:** Measurement grid: dx=7.5mm, dy=7.5mm, dz=5mm  
 Reference Value = 58.64 V/m; Power Drift = -0.45 dB  
 Peak SAR (extrapolated) = 49.3 W/kg  
**SAR(1 g) = 12.3 W/kg; SAR(10 g) = 5.13 W/kg** (SAR corrected for target medium)  
 Maximum value of SAR (measured) = 14.0 W/kg

**Below 2 GHz-Rev.2/Ab Scan/4-Z-Axis Scan (1x1x17):** Measurement grid: dx=20mm, dy=20mm, dz=10mm  
 Maximum value of SAR (measured) = 18.1 W/kg

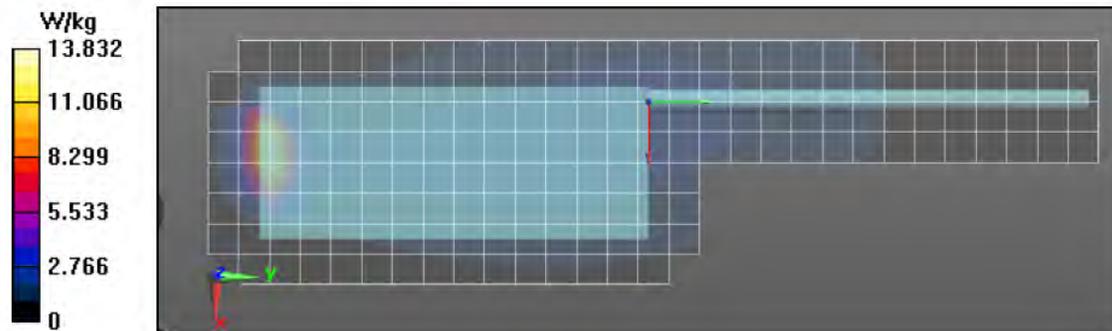

### Table – 17; VHF

**Motorola Solutions, Inc. EME Laboratory**  
Date/Time: 7/17/2017 9:38:47 PM

Robot#: DASY5-PG-2 | Run#: ZR-AB-170717-14  
 Model#: H91TGD9PW5AN (PNUW1012C)  
 Phantom#: ELI4 1011  
 Tissue Temp: 21.0 (C)  
 Serial#: 579TTME968  
 Antenna: NAR6594A  
 Test Freq: 156.4500 (MHz)  
 Battery: NNTN7573A  
 Carry Acc: HLN6875A  
 Audio Acc: None  
 Start Power: 6.53 (W)


Comments:

Duty Cycle: 1:1, Medium parameters used:  $f = 156 \text{ MHz}$ ;  $\sigma = 0.77 \text{ S/m}$ ;  $\epsilon_r = 59.2$ ;  $\rho = 1000 \text{ kg/m}^3$   
 Probe: ES3DV3 - SN3122, , Frequency: 156.45 MHz, ConvF(6.91, 6.91, 6.91); Calibrated: 3/10/2017  
 Electronics: DAE4 Sn850, Calibrated: 2/28/2017

**Below 2 GHz-Rev.2/Ab Scan/1-Area Scan (81x301x1):** Interpolated grid:  $dx=1.500 \text{ mm}$ ,  $dy=1.500 \text{ mm}$   
 Reference Value = 41.38 V/m; Power Drift = -0.32 dB  
 Fast SAR: SAR(1 g) = 5.61 W/kg; SAR(10 g) = 3.47 W/kg (SAR corrected for target medium)  
 Maximum value of SAR (interpolated) = 7.65 W/kg

**Below 2 GHz-Rev.2/Ab Scan/3-Zoom Scan (6x6x7)/Cube 0:** Measurement grid:  $dx=7.5\text{mm}$ ,  
 $dy=7.5\text{mm}$ ,  $dz=5\text{mm}$   
 Reference Value = 41.38 V/m; Power Drift = -0.36 dB  
 Peak SAR (extrapolated) = 29.1 W/kg  
 SAR(1 g) = 6.5 W/kg; SAR(10 g) = 2.53 W/kg (SAR corrected for target medium)  
 Maximum value of SAR (measured) = 7.94 W/kg

**Below 2 GHz-Rev.2/Ab Scan/4-Z-Axis Scan (1x1x17):** Measurement grid:  $dx=20\text{mm}$ ,  $dy=20\text{mm}$ ,  
 $dz=10\text{mm}$   
 Maximum value of SAR (measured) = 9.46 W/kg

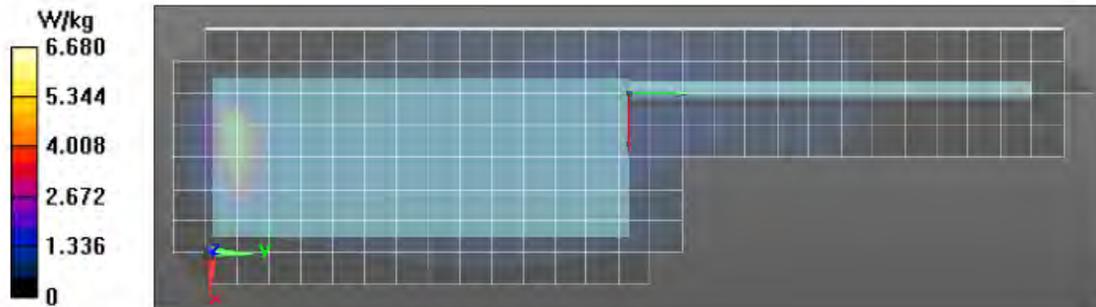

### Table – 17; UHF1

**Motorola Solutions, Inc. EME Laboratory**  
Date/Time: 8/7/2017 11:09:55 PM

Robot#: DASY5-PG-2 | Run#: TLC(HR)-AB-170807-07  
 Model#: H91TGD9PW5AN (PNUW1012C)  
 Phantom#: ELI4 1103  
 Tissue Temp: 20.7 (C)  
 Serial#: 579TTME969  
 Antenna: FAF5259A  
 Test Freq: 406.1250 (MHz)  
 Battery: NNTN7038B  
 Carry Acc: NTN8266B  
 Audio Acc: NNTN8575A  
 Start Power: 5.70 (W)


Comments:

Duty Cycle: 1:1, Medium parameters used:  $f = 406$  MHz;  $\sigma = 0.89$  S/m;  $\epsilon_r = 56.7$ ;  $\rho = 1000$  kg/m<sup>3</sup>  
 Probe: ES3DV3 - SN3122, , Frequency: 406.012 MHz, ConvF(7.1, 7.1, 7.1); Calibrated: 3/10/2017  
 Electronics: DAE4 Sn850, Calibrated: 2/28/2017

**Below 2 GHz-Rev.2/Ab Scan/1-Area Scan (81x181x1):** Interpolated grid: dx=1.500 mm, dy=1.500 mm  
 Reference Value = 114.3 V/m; Power Drift = -0.23 dB  
 Fast SAR: SAR(1 g) = 15.2 W/kg; SAR(10 g) = 10.8 W/kg (SAR corrected for target medium)  
 Maximum value of SAR (interpolated) = 16.7 W/kg

**Below 2 GHz-Rev.2/Ab Scan/3-Zoom Scan (6x8x7)/Cube 0:** Measurement grid: dx=7.5mm, dy=7.5mm, dz=5mm  
 Reference Value = 114.3 V/m; Power Drift = -0.33 dB  
 Peak SAR (extrapolated) = 21.8 W/kg  
 SAR(1 g) = 14.7 W/kg; SAR(10 g) = 10.4 W/kg (SAR corrected for target medium)  
 Maximum value of SAR (measured) = 16.4 W/kg

**Below 2 GHz-Rev.2/Ab Scan/4-Z-Axis Scan (1x1x17):** Measurement grid: dx=20mm, dy=20mm, dz=10mm

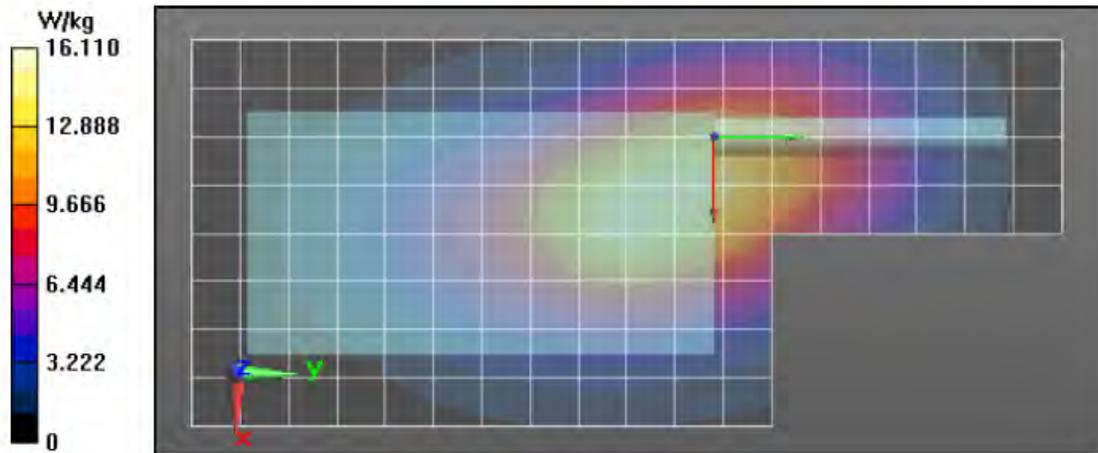

### Table – 17; UHF2

#### Motorola Solutions, Inc. EME Laboratory

Date/Time: 7/15/2017 6:21:00 PM

Robot#: DASY5-PG-2 | Run#: ZR-AB-170715-11  
 Model#: H91TGD9PW5AN (PNUW1012C)  
 Phantom#: ELI4 1103  
 Tissue Temp: 21.0 (C)  
 Serial#: 579TTME968  
 Antenna: FAF5260A  
 Test Freq: 450.0000 (MHz)  
 Battery: PMNN4403B  
 Carry Acc: NTN8266B  
 Audio Acc: None  
 Start Power: 5.70 (W)


Comments:

Duty Cycle: 1:1, Medium parameters used:  $f = 450 \text{ MHz}$ ;  $\sigma = 0.95 \text{ S/m}$ ;  $\epsilon_r = 56.3$ ;  $\rho = 1000 \text{ kg/m}^3$   
 Probe: ES3DV3 - SN3122, , Frequency: 450 MHz, ConvF(7.1, 7.1, 7.1); Calibrated: 3/10/2017  
 Electronics: DAE4 Sn850, Calibrated: 2/28/2017

**Below 2 GHz-Rev.2/Ab Scan/1-Area Scan (81x181x1):** Interpolated grid:  $dx=1.500 \text{ mm}$ ,  $dy=1.500 \text{ mm}$   
 Reference Value = 108.6 V/m; Power Drift = -0.20 dB  
 Fast SAR: SAR(1 g) = 12.5 W/kg; SAR(10 g) = 9 W/kg (SAR corrected for target medium)  
 Maximum value of SAR (interpolated) = 14.1 W/kg

**Below 2 GHz-Rev.2/Ab Scan/3-Zoom Scan (7x9x7)/Cube 0:** Measurement grid:  $dx=7.5\text{mm}$ ,  
 $dy=7.5\text{mm}$ ,  $dz=5\text{mm}$   
 Reference Value = 108.6 V/m; Power Drift = -0.29 dB  
 Peak SAR (extrapolated) = 19.3 W/kg  
 SAR(1 g) = 12.6 W/kg; SAR(10 g) = 8.83 W/kg (SAR corrected for target medium)  
 Maximum value of SAR (measured) = 14.6 W/kg

**Below 2 GHz-Rev.2/Ab Scan/4-Z-Axis Scan (1x1x17):** Measurement grid:  $dx=20\text{mm}$ ,  $dy=20\text{mm}$ ,  
 $dz=10\text{mm}$   
 Maximum value of SAR (measured) = 14.3 W/kg

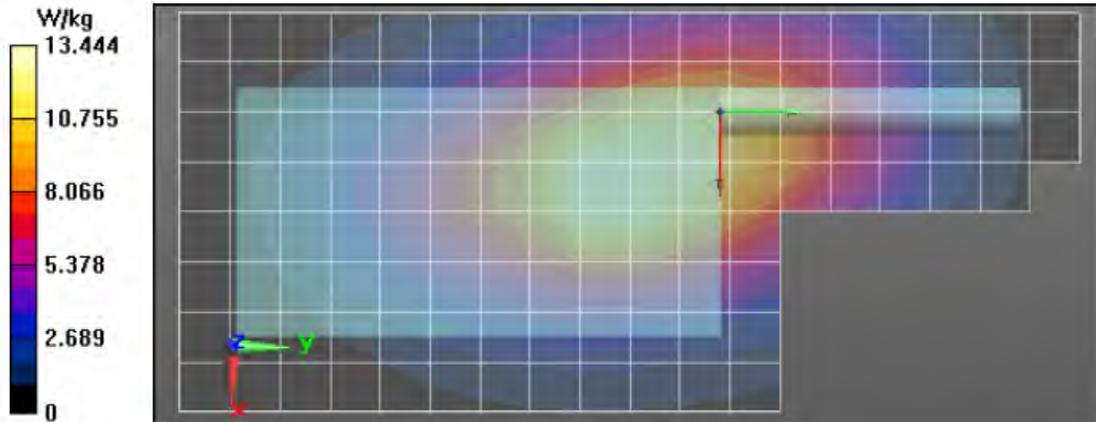

### Table – 17; 7/800 MHz

**Motorola Solutions, Inc. EME Laboratory**  
 Date/Time: 7/13/2017 1:08:14 AM

Robot#: DASY5-PG-2 | Run#: FD-AB-170713-01#  
 Model#: H91TGD9PW5AN (PNUW1012C)  
 Phantom#: ELI4 1090  
 Tissue Temp: 21.4 (C)  
 Serial#: 579TTME968  
 Antenna: NAR6595A  
 Test Freq: 808.5000 (MHz)  
 Battery: PMNN4403B  
 Carry Acc: NTN8266B  
 Audio Acc: NMN6274A  
 Start Power: 3.60 (W)


Comments:

Duty Cycle: 1:1, Medium parameters used:  $f = 809 \text{ MHz}$ ;  $\sigma = 0.98 \text{ S/m}$ ;  $\epsilon_r = 55.7$ ;  $\rho = 1000 \text{ kg/m}^3$   
 Probe: ES3DV3 - SN3122, Frequency: 808.5 MHz, ConvF(6.34, 6.34, 6.34); Calibrated: 3/10/2017  
 Electronics: DAE4 Sn850, Calibrated: 2/28/2017

**Below 2 GHz-Rev.2/Ab Scan/1-Area Scan (81x191x1):** Interpolated grid:  $dx=1.500 \text{ mm}$ ,  $dy=1.500 \text{ mm}$   
 Reference Value = 92.08 V/m; Power Drift = -0.72 dB  
 Fast SAR: SAR(1 g) = 12 W/kg; SAR(10 g) = 7.93 W/kg (SAR corrected for target medium)  
 Maximum value of SAR (interpolated) = 14.3 W/kg

**Below 2 GHz-Rev.2/Ab Scan/3-Zoom Scan (6x8x7)/Cube 0:** Measurement grid:  $dx=7.5\text{mm}$ ,  
 $dy=7.5\text{mm}$ ,  $dz=5\text{mm}$   
 Reference Value = 92.08 V/m; Power Drift = -1.08 dB  
 Peak SAR (extrapolated) = 18.5 W/kg  
 SAR(1 g) = 10.9 W/kg; SAR(10 g) = 7.59 W/kg (SAR corrected for target medium)  
 Maximum value of SAR (measured) = 13.1 W/kg

**Below 2 GHz-Rev.2/Ab Scan/4-Z-Axis Scan (1x1x17):** Measurement grid:  $dx=20\text{mm}$ ,  $dy=20\text{mm}$ ,  
 $dz=10\text{mm}$   
 Maximum value of SAR (measured) = 12.3 W/kg

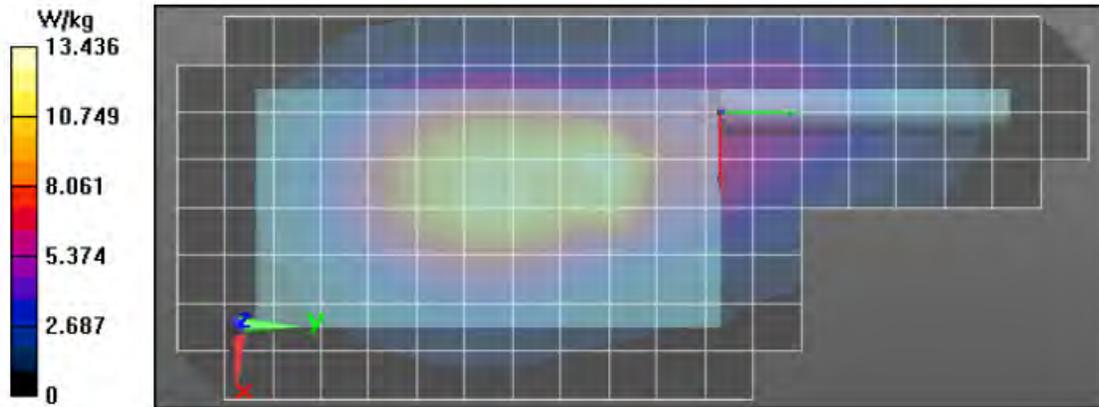

## Highest Face SAR Configuration Results Table – 18; VHF

**Motorola Solutions, Inc. EME Laboratory**  
Date/Time: 8/3/2017 5:03:02 PM

Robot#: DASY5-PG-2 | Run#: FD(HR)-FACE-170803-11  
 Model#: H91TGD9PW7AN (PNUW1014C)  
 Phantom#: ELI4 1050  
 Tissue Temp: 20.5 (C)  
 Serial#: 579TTME980  
 Antenna: PMAT4001A  
 Test Freq: 143.4000 (MHz)  
 Battery: NNTN8092A  
 Carry Acc: None; Radio at back  
 Audio Acc: None  
 Start Power: 6.60 (W)


**Comments:**

Duty Cycle: 1:1, Medium parameters used:  $f = 143 \text{ MHz}$ ;  $\sigma = 0.74 \text{ S/m}$ ;  $\epsilon_r = 52.8$ ;  $\rho = 1000 \text{ kg/m}^3$   
 Probe: ES3DV3 - SN3122, . Frequency: 143.4 MHz. ConvF(7.36, 7.36, 7.36); Calibrated: 3/10/2017  
 Electronics: DAE4 Sn850, Calibrated: 2/28/2017

**Below 2 GHz-Rev.2/Face Scan/1-Area Scan (81x281x1):** Interpolated grid:  $dx=1.500 \text{ mm}$ ,  $dy=1.500 \text{ mm}$   
 Reference Value = 60.23 V/m; Power Drift = -0.17 dB  
**Fast SAR: SAR(1 g) = 2.5 W/kg; SAR(10 g) = 1.94 W/kg** (SAR corrected for target medium)  
 Maximum value of SAR (interpolated) = 2.70 W/kg

**Below 2 GHz-Rev.2/Face Scan/3-Zoom Scan (5x5x7)/Cube 0:** Measurement grid:  $dx=7.5\text{mm}$ ,  $dy=7.5\text{mm}$ ,  $dz=5\text{mm}$   
 Reference Value = 60.23 V/m; Power Drift = -0.16 dB  
 Peak SAR (extrapolated) = 3.40 W/kg  
**SAR(1 g) = 2.45 W/kg; SAR(10 g) = 1.89 W/kg** (SAR corrected for target medium)

**Below 2 GHz-Rev.2/Face Scan/4-Z-Axis Scan (1x1x17):** Measurement grid:  $dx=20\text{mm}$ ,  $dy=20\text{mm}$ ,  $dz=10\text{mm}$

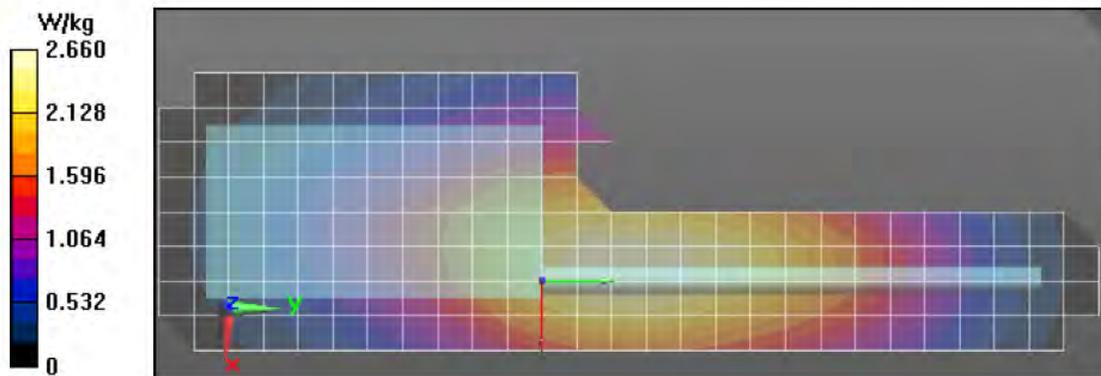

### Table – 18; VHF

**Motorola Solutions, Inc. EME Laboratory**  
Date/Time: 8/3/2017 10:44:47 PM

Robot#: DASY5-PG-2 | Run#: TLC(AN)-FACE-170803-12  
 Model#: H91TGD9PW7AN (PNUW1014C)  
 Phantom#: ELI4 1022  
 Tissue Temp: 20.0 (C)  
 Serial#: 579TTME980  
 Antenna: NAR6594A  
 Test Freq: 173.4000 (MHz)  
 Battery: NNTN8092A  
 Carry Acc: None; Radio at back  
 Audio Acc: None  
 Start Power: 6.60 (W)


**Comments:**

Duty Cycle: 1:1, Medium parameters used:  $f = 173 \text{ MHz}$ ;  $\sigma = 0.76 \text{ S/m}$ ;  $\epsilon_r = 51.5$ ;  $\rho = 1000 \text{ kg/m}^3$   
 Probe: ES3DV3 - SN3122, Frequency: 173.4 MHz, ConvF(7.36, 7.36, 7.36); Calibrated: 3/10/2017  
 Electronics: DAE4 Sn850, Calibrated: 2/28/2017

**Below 2 GHz-Rev.2/Face Scan/1-Area Scan (81x281x1):** Interpolated grid:  $dx=1.500 \text{ mm}$ ,  $dy=1.500 \text{ mm}$   
 Reference Value = 47.04 V/m; Power Drift = -0.26 dB  
 Fast SAR: SAR(1 g) = 1.52 W/kg; SAR(10 g) = 1.16 W/kg (SAR corrected for target medium)  
 Maximum value of SAR (interpolated) = 1.64 W/kg

**Below 2 GHz-Rev.2/Face Scan/3-Zoom Scan (5x6x7)/Cube 0:** Measurement grid:  $dx=7.5\text{mm}$ ,  $dy=7.5\text{mm}$ ,  $dz=5\text{mm}$   
 Reference Value = 47.04 V/m; Power Drift = -0.30 dB  
 Peak SAR (extrapolated) = 2.01 W/kg  
 SAR(1 g) = 1.44 W/kg; SAR(10 g) = 1.11 W/kg (SAR corrected for target medium)  
 Maximum value of SAR (measured) = 1.57 W/kg

**Below 2 GHz-Rev.2/Face Scan/4-Z-Axis Scan (1x1x17):** Measurement grid:  $dx=20\text{mm}$ ,  $dy=20\text{mm}$ ,  $dz=10\text{mm}$   
 Maximum value of SAR (measured) = 1.56 W/kg

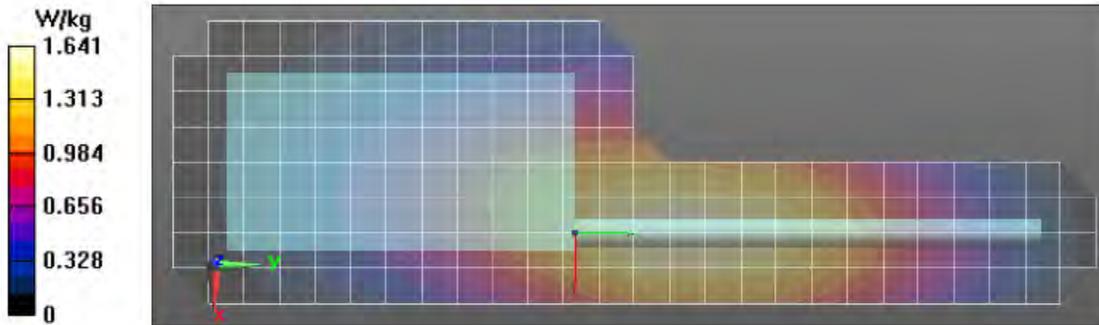

### Table – 18; UHF1

Motorola Solutions, Inc. EME Laboratory  
Date/Time: 8/3/2017 2:44:44 PM

Robot#: DASY5-PG-2 | Run#: FD(HR)-FACE-170803-09  
 Model#: H91TGD9PW7AN (PNUW1014C)  
 Phantom#: ELI4 1109  
 Tissue Temp: 20.7 (C)  
 Serial#: 579TTME980  
 Antenna: FAF5259A  
 Test Freq: 406.1250 (MHz)  
 Battery: NNIN7038B  
 Carry Acc: None; Radio at back  
 Audio Acc: None  
 Start Power: 5.67 (W)


Comments:

Duty Cycle: 1:1. Medium parameters used:  $f = 406 \text{ MHz}$ ;  $\sigma = 0.84 \text{ S/m}$ ;  $\epsilon_r = 44.6$ ;  $\rho = 1000 \text{ kg/m}^3$   
 Probe: ES3DV3 - SN3122, , Frequency: 406.125 MHz, ConvF(7, 7, 7); Calibrated: 3/10/2017  
 Electronics: DAE4 Sn850, Calibrated: 2/28/2017

**Below 2 GHz-Rev.2/Face Scan/1-Area Scan (71x181x1):** Interpolated grid:  $dx=1.500 \text{ mm}$ ,  $dy=1.500 \text{ mm}$   
 Reference Value = 100.9 V/m; Power Drift = -0.20 dB  
 Fast SAR: SAR(1 g) = 9.05 W/kg; SAR(10 g) = 6.64 W/kg (SAR corrected for target medium)  
 Maximum value of SAR (interpolated) = 9.78 W/kg

**Below 2 GHz-Rev.2/Face Scan/3-Zoom Scan (5x5x7)/Cube 0:** Measurement grid:  $dx=7.5\text{mm}$ ,  $dy=7.5\text{mm}$ ,  $dz=5\text{mm}$   
 Reference Value = 100.9 V/m; Power Drift = -0.23 dB  
 Peak SAR (extrapolated) = 11.9 W/kg  
 SAR(1 g) = 8.77 W/kg; SAR(10 g) = 6.51 W/kg (SAR corrected for target medium)  
 Maximum value of SAR (measured) = 9.52 W/kg

**Below 2 GHz-Rev.2/Face Scan/4-Z-Axis Scan (1x1x17):** Measurement grid:  $dx=20\text{mm}$ ,  $dy=20\text{mm}$ ,  $dz=10\text{mm}$   
 Maximum value of SAR (measured) = 9.45 W/kg

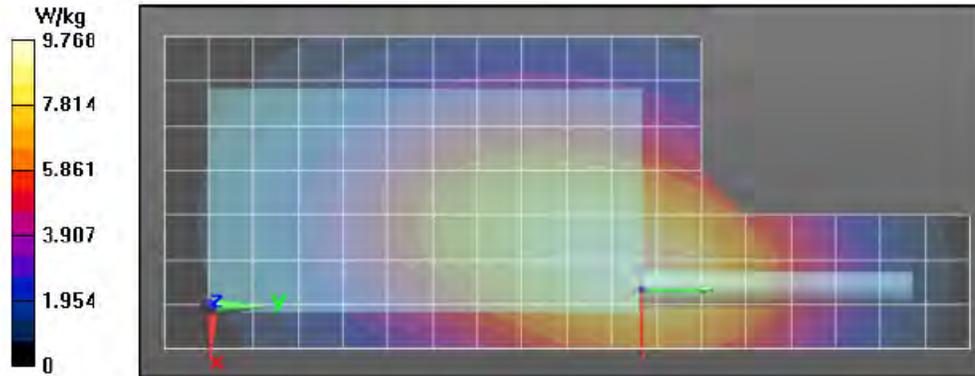

### Table – 18; UHF2

**Motorola Solutions, Inc. EME Laboratory**  
Date/Time: 8/3/2017 1:55:23 PM

Robot#: DASY5-PG-2 | Run#: FD(HR)-FACE-170803-08  
 Model#: H91TGD9PW7AN (PNUW1014C)  
 Phantom#: ELI4 1109  
 Tissue Temp: 20.9 (C)  
 Serial#: 579TTME980  
 Antenna: FAF5260A  
 Test Freq: 481.0000 (MHz)  
 Battery: NNTN7038B  
 Carry Acc: None; Radio at back  
 Audio Acc: None  
 Start Power: 5.66 (W)


**Comments:**

Duty Cycle: 1:1, Medium parameters used:  $f = 481 \text{ MHz}$ ;  $\sigma = 0.9 \text{ S/m}$ ;  $\epsilon_r = 43$ ;  $\rho = 1000 \text{ kg/m}^3$   
 Probe: ES3DV3 - SN3122, Frequency: 481 MHz, ConvF(7, 7, 7); Calibrated: 3/10/2017  
 Electronics: DAE4 Sn850, Calibrated: 2/28/2017

**Below 2 GHz-Rev.2/Face Scan/1-Area Scan (81x181x1):** Interpolated grid:  $dx=1.500 \text{ mm}$ ,  $dy=1.500 \text{ mm}$   
 Reference Value = 86.33 V/m; Power Drift = -0.19 dB  
 Fast SAR: SAR(1 g) = 6.84 W/kg; SAR(10 g) = 5.02 W/kg (SAR corrected for target medium)  
 Maximum value of SAR (interpolated) = 7.64 W/kg

**Below 2 GHz-Rev.2/Face Scan/3-Zoom Scan (5x5x7)/Cube 0:** Measurement grid:  $dx=7.5\text{mm}$ ,  $dy=7.5\text{mm}$ ,  $dz=5\text{mm}$   
 Reference Value = 86.33 V/m; Power Drift = -0.22 dB  
 Peak SAR (extrapolated) = 9.32 W/kg  
 SAR(1 g) = 6.72 W/kg; SAR(10 g) = 5.02 W/kg (SAR corrected for target medium)  
 Maximum value of SAR (measured) = 7.49 W/kg

**Below 2 GHz-Rev.2/Face Scan/4-Z-Axis Scan (1x1x17):** Measurement grid:  $dx=20\text{mm}$ ,  $dy=20\text{mm}$ ,  $dz=10\text{mm}$

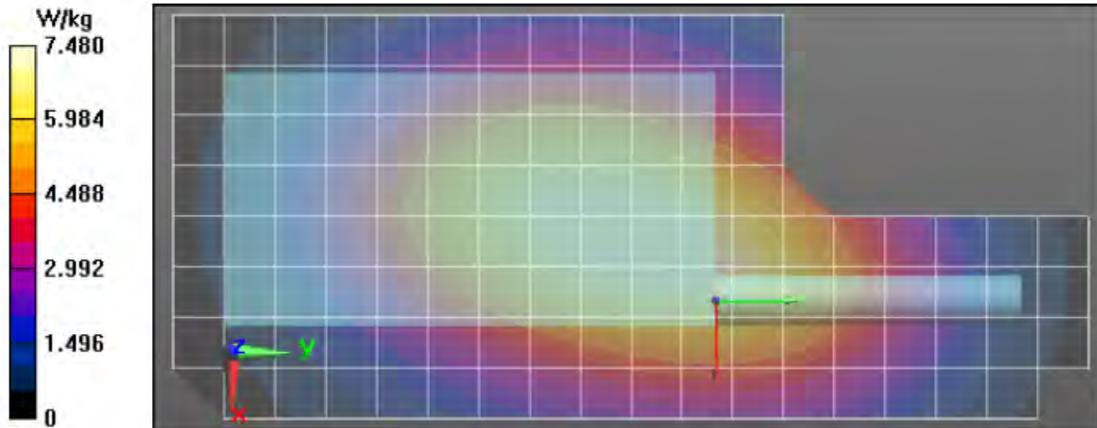

### Table – 18; 7/800 MHz

**Motorola Solutions, Inc. EME Laboratory**  
Date/Time: 7/19/2017 12:58:21 AM

Robot#: DASY5-PG-2 | Run#: ZR-FACE-170719-01#  
 Model#: H91TGD9PW7AN (PNUW1014C)  
 Phantom#: ELI4 1037  
 Tissue Temp: 20.8 (C)  
 Serial#: 579TTME980  
 Antenna: NAR6595A  
 Test Freq: 808.5000 (MHz)  
 Battery: NNTN7038B  
 Carry Acc: None; Radio at back  
 Audio Acc: None  
 Start Power: 3.60 (W)


**Comments:**

Duty Cycle: 1:1, Medium parameters used:  $f = 809 \text{ MHz}$ ;  $\sigma = 0.91 \text{ S/m}$ ;  $\epsilon_r = 42.3$ ;  $\rho = 1000 \text{ kg/m}^3$   
 Probe: ES3DV3 - SN3122, , Frequency: 808.5 MHz, ConvF(6.62, 6.62, 6.62); Calibrated: 3/10/2017  
 Electronics: DAE4 Sn850, Calibrated: 2/28/2017

**Below 2 GHz-Rev.2/Face Scan/1-Area Scan (81x201x1):** Interpolated grid:  $dx=1.500 \text{ mm}$ ,  $dy=1.500 \text{ mm}$   
 Reference Value = 66.52 V/m; Power Drift = -0.28 dB  
 Fast SAR: SAR(1 g) = 6.37 W/kg; SAR(10 g) = 4.49 W/kg (SAR corrected for target medium)  
 Maximum value of SAR (interpolated) = 7.21 W/kg

**Below 2 GHz-Rev.2/Face Scan/3-Zoom Scan (5x5x7)/Cube 0:** Measurement grid:  $dx=7.5\text{mm}$ ,  $dy=7.5\text{mm}$ ,  $dz=5\text{mm}$   
 Reference Value = 66.52 V/m; Power Drift = -0.43 dB  
 Peak SAR (extrapolated) = 8.06 W/kg  
 SAR(1 g) = 6.19 W/kg; SAR(10 g) = 4.61 W/kg (SAR corrected for target medium)  
 Maximum value of SAR (measured) = 6.87 W/kg

**Below 2 GHz-Rev.2/Face Scan/4-Z-Axis Scan (1x1x17):** Measurement grid:  $dx=20\text{mm}$ ,  $dy=20\text{mm}$ ,  $dz=10\text{mm}$   
 Maximum value of SAR (measured) = 6.74 W/kg

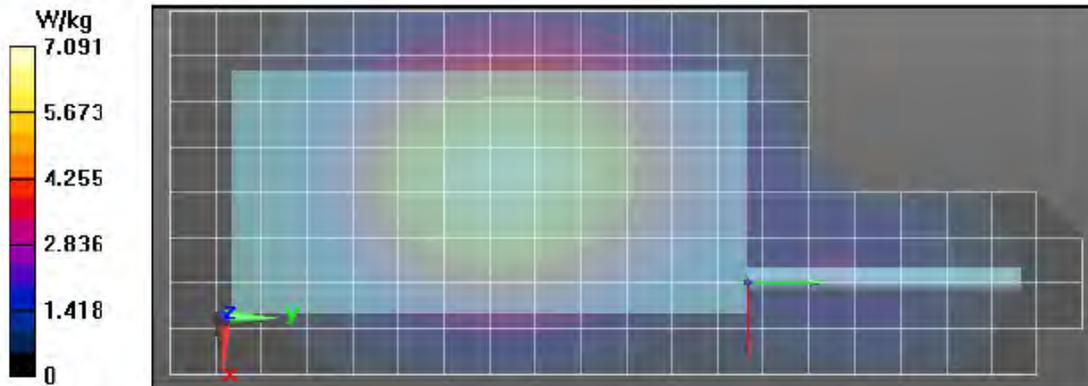

**APPENDIX F**  
**DUT Test Position Photos**

**1.0 Highest SAR Test Position per body location**

**1.1 Body**

DUT with antenna FAF5259A with offered battery NNTN7038B and belt clip NTN8266B against the phantom with an audio accessory NNTN8575A attached. Same position used for other applicable offered antennas, batteries, and audio accessory.



Antenna kit #	Separation Distances (mm)		
	@ bottom surface of the DUT	@ antenna's base	@ antenna's tip
FAF5259A	8	26	33

**1.2 Face**

Back of DUT with antenna FAF5259A and battery NNTN7038B separated 2.5cm from the phantom without an audio accessory attached. Same position used for other applicable offered antennas and batteries.



Antenna kit #	Separation Distances (mm)		
	@ bottom surface of the DUT	@ antenna's base	@ antenna's tip
FAF5259A	21	33	36