



CERTIFICATE 2518.05

DECLARATION OF COMPLIANCE SAR ASSESSMENT Part 2 of 4

Motorola Solutions Inc.
EME Test Laboratory
 Motorola Solutions Malaysia Sdn Bhd (Innoplex)
 Plot 2A, Medan Bayan Lepas,
 Mukim 12 SWD 11900 Bayan Lepas Penang, Malaysia.

Date of Report: 06/14/2016
Report Revision: C

Responsible Engineer: Saw Sun Hock, Veeramani Veerapan
Report Author: Saw Sun Hock, Veeramani Veerapan
Date/s Tested: 3/30/2016 - 5/21/2016
Manufacturer: Motorola Solutions Inc.
DUT Description: Handheld Portable – APX6000 and APX6000XE refresh 7/800MHz 764-870 MHz

Test TX mode(s): CW (PTT), Bluetooth, and WLAN 802.11b/g/n
Max. Power output: 2.95 W (764-805 MHz), 3.6 W (806-824 MHz), 10 mW (Bluetooth), 1.98 mW (Bluetooth LE), 63.1 mW (802.11b), 25.1 mW (802.11g), 15.5 mW (802.11n)
Nominal Power: 2.35 W (764-805 MHz), 3.0 W (806-824 MHz), 8 mW (Bluetooth), 1.5 mW (Bluetooth LE), 31.6 mW (802.11b), 12.5 mW (802.11g), 12.5 mW (802.11n)
Tx Frequency Bands: LMR 764-805 MHz, 806-870 MHz ; Bluetooth 2402-2480 MHz; WLAN 2412-2462 MHz
Signaling type: FM, TDMA, FHSS (Bluetooth), 802.11b/g/n (WLAN)
Model(s) Tested: H98UCD9PW5BN (PMUF1877A)
Model(s) Certified: H98UCD9PW5BN (PMUF1865A), H98UCD9PW5BN (PMUF1877A), H98UCH9PW7BN (PMUF1867A), H98UCH9PW7BN (PMUF1879A)
Serial Number(s): 756TSD0541, 756TSD0544
Classification: Occupational/Controlled
FCC ID: AZ489FT7086; LMR 764-775 MHz, 794-824 MHz, 851-869 MHz, Bluetooth 2.402-2.480 GHz, WLAN 802.11 b/g/n 2.412-2.462 GHz
 This report contains results that are immaterial for FCC equipment approval, which are clearly identified.
IC: 109U-89FT7086; This report contains results that are immaterial for IC equipment approval, which are clearly identified.

The test results clearly demonstrate compliance with FCC Occupational/Controlled RF Exposure limits of 8 W/kg averaged over 1 gram per the requirements of OET Bulletin 65. The 10 grams result is not applicable to FCC filing. The test results clearly demonstrate compliance with ICNIRP (1998) Guidelines for limiting exposure in time-varying electric, magnetic, and electromagnetic fields (up to 300 GHz), Health Physics 74, 494-522 RF Exposure limits of 10 W/kg averaged over 10grams of contiguous tissue.

Based on the information and the testing results provided herein, the undersigned certifies that when used as stated in the operating instructions supplied, said product complies with the national and international reference standards and guidelines listed in section 4.0 of this report. This report shall not be reproduced without written approval from an officially designated representative of the Motorola Solutions Inc EME Laboratory. I attest to the accuracy of the data and assume full responsibility for the completeness of these measurements. This reporting format is consistent with the suggested guidelines of the TIA TSB-150 December 2004. The results and statements contained in this report pertain only to the device(s) evaluated.

Tiong
Tiong Nguk Ing
Deputy Technical Manager
Approval Date: 06/14/2016

Certification Date: 5/27/2016
Certification No.: L1160578P

Appendix B

Probe Calibration Certificates

**Calibration Laboratory of
Schmid & Partner
Engineering AG**
Zeughausstrasse 43, 8004 Zurich, Switzerland



S Schweizerischer Kalibrierdienst
C Service suisse d'étalonnage
S Servizio svizzero di taratura
Swiss Calibration Service

Accredited by the Swiss Accreditation Service (SAS)
The Swiss Accreditation Service is one of the signatories to the EA
Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: **SCS 0108**

Client **Motorola Solutions MY**

Certificate No: **ES3-3122_Jun15**

CALIBRATION CERTIFICATE

Object: **ES3DV3 - SN:3122**

Calibration procedure(s): **QA CAL-01.v9, QA CAL-12.v9, QA CAL-23.v5, QA CAL-25.v6**
Calibration procedure for dosimetric E-field probes

Calibration date: **June 19, 2015**

This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI).
The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility; environment temperature (22 ± 3)°C and humidity = 70%.

Calibration Equipment used (M&TE critical for calibration)

Primary Standards	ID	Cal Date (Certificate No.)	Scheduled Calibration
Power meter E4419B	GB41293874	01-Apr-15 (No. 217-02128)	Mar-16
Power sensor E4412A	MY41498087	01-Apr-15 (No. 217-02128)	Mar-16
Reference 3 dB Attenuator	SN: S5054 (3c)	01-Apr-15 (No. 217-02129)	Mar-16
Reference 20 dB Attenuator	SN: S5277 (20x)	01-Apr-15 (No. 217-02132)	Mar-16
Reference 30 dB Attenuator	SN: S5129 (30b)	01-Apr-15 (No. 217-02133)	Mar-16
Reference Probe ES3DV2	SN: 3013	30-Dec-14 (No. ES3-3013_Dec14)	Dec-15
DAE4	SN: 660	14-Jan-15 (No. DAE4-660_Jan15)	Jan-16
Secondary Standards	ID	Check Date (in house)	Scheduled Check
RF generator HP 8648C	US3642U01700	4-Aug-99 (in house check Apr-13)	In house check: Apr-16
Network Analyzer HP 8753E	US37390585	18-Oct-01 (in house check Oct-14)	In house check: Oct-15

	Name	Function	Signature
Calibrated by:	Jeton Kasriel	Laboratory Technician	
Approved by:	Kolja Pokovic	Technical Manager	

Issued: June 20, 2015

This calibration certificate shall not be reproduced except in full without written approval of the laboratory.

**Calibration Laboratory of
Schmid & Partner
Engineering AG**
Zeughausstrasse 43, 8004 Zurich, Switzerland



SCS Schweizerischer Kalibrierdienst
Service suisse d'étalonnage
Servizio svizzero di taratura
Swiss Calibration Service

Accredited by the Swiss Accreditation Service (SAS)
The Swiss Accreditation Service is one of the signatories to the EA
Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: **SCS 0108**

Glossary:

TSL	tissue simulating liquid
NORM _{x,y,z}	sensitivity in free space
ConvF	sensitivity in TSL / NORM _{x,y,z}
DCP	diode compression point
CF	crest factor (1/duty_cycle) of the RF signal
A, B, C, D	modulation dependent linearization parameters
Polarization φ	φ rotation around probe axis
Polarization θ	θ rotation around an axis that is in the plane normal to probe axis (at measurement center), i.e., θ = 0 is normal to probe axis
Connector Angle	information used in DASY system to align probe-sensor X to the robot coordinate system

Calibration is Performed According to the Following Standards:

- a) IEEE Std 1528-2013, "IEEE Recommended Practice for Determining the Peak Spatial-Averaged Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques", June 2013
- b) IEC 62209-1, "Procedure to measure the Specific Absorption Rate (SAR) for hand-held devices used in close proximity to the ear (frequency range of 300 MHz to 3 GHz)", February 2005

Methods Applied and Interpretation of Parameters:

- **NORM_{x,y,z}**: Assessed for E-field polarization θ = 0 (f ≤ 900 MHz in TEM-cell; f > 1800 MHz: R22 waveguide). NORM_{x,y,z} are only intermediate values, i.e., the uncertainties of NORM_{x,y,z} does not affect the E²-field uncertainty inside TSL (see below ConvF).
- **NORM(f)_{x,y,z} = NORM_{x,y,z} * frequency_response** (see Frequency Response Chart). This linearization is implemented in DASY4 software versions later than 4.2. The uncertainty of the frequency response is included in the stated uncertainty of ConvF.
- **DCP_{x,y,z}**: DCP are numerical linearization parameters assessed based on the data of power sweep with CW signal (no uncertainty required). DCP does not depend on frequency nor media.
- **PAR**: PAR is the Peak to Average Ratio that is not calibrated but determined based on the signal characteristics.
- **A_{x,y,z}; B_{x,y,z}; C_{x,y,z}; D_{x,y,z}; VR_{x,y,z}; A, B, C, D** are numerical linearization parameters assessed based on the data of power sweep for specific modulation signal. The parameters do not depend on frequency nor media. VR is the maximum calibration range expressed in RMS voltage across the diode.
- **ConvF and Boundary Effect Parameters**: Assessed in flat phantom using E-field (or Temperature Transfer Standard for f ≤ 800 MHz) and inside waveguide using analytical field distributions based on power measurements for f > 800 MHz. The same setups are used for assessment of the parameters applied for boundary compensation (alpha, depth) of which typical uncertainty values are given. These parameters are used in DASY4 software to improve probe accuracy close to the boundary. The sensitivity in TSL corresponds to NORM_{x,y,z} * ConvF whereby the uncertainty corresponds to that given for ConvF. A frequency dependent ConvF is used in DASY version 4.4 and higher which allows extending the validity from ± 50 MHz to ± 100 MHz.
- **Spherical isotropy (3D deviation from isotropy)**: in a field of low gradients realized using a flat phantom exposed by a patch antenna.
- **Sensor Offset**: The sensor offset corresponds to the offset of virtual measurement center from the probe tip (on probe axis). No tolerance required.
- **Connector Angle**: The angle is assessed using the information gained by determining the NORM_x (no uncertainty required).

ES3DV3 - SN:3122

June 19, 2015

Probe ES3DV3

SN:3122

Manufactured: July 11, 2006
Calibrated: June 19, 2015

Calibrated for DASY/EASY Systems
(Note: non-compatible with DASY2 system!)

ES3DV3- SN:3122

June 19, 2015

DASY/EASY - Parameters of Probe: ES3DV3 - SN:3122

Basic Calibration Parameters

	Sensor X	Sensor Y	Sensor Z	Unc (k=2)
Norm $(\mu V/(V/m)^2)^A$	1.34	1.22	1.42	$\pm 10.1 \%$
DICP (mV) ^B	102.6	103.7	101.0	

Modulation Calibration Parameters

UID	Communication System Name		A dB	B dB $\sqrt{\mu V}$	C	D dB	VR mV	Unc ^C (k=2)
0	CW	X	0.0	0.0	1.0	0.00	209.7	$\pm 7.0 \%$
		Y	0.0	0.0	1.0		202.5	
		Z	0.0	0.0	1.0		200.4	
10021-DAB	GSM-FDD (TDMA, GMSK)	X	27.30	99.6	27.9	9.39	147.3	$\pm 2.5 \%$
		Y	27.71	99.5	27.9		147.9	
		Z	26.04	99.6	28.1		137.2	
10023-DAB	GPRS-FDD (TDMA, GMSK, TN 0)	X	27.85	100.0	28.2	9.57	143.3	$\pm 2.5 \%$
		Y	26.86	99.4	28.1		145.7	
		Z	25.87	99.3	28.0		131.5	
10024-DAB	GPRS-FDD (TDMA, GMSK, TN 0-1)	X	38.48	99.1	25.1	6.56	119.9	$\pm 1.9 \%$
		Y	41.84	99.6	25.1		149.5	
		Z	29.41	94.8	23.8		137.4	
10025-DAB	EDGE-FDD (TDMA, 8PSK, TN 0)	X	13.71	94.1	35.8	12.82	94.9	$\pm 2.7 \%$
		Y	15.75	99.6	38.3		92.3	
		Z	12.29	91.8	34.8		87.0	
10026-DAB	EDGE-FDD (TDMA, 8PSK, TN 0-1)	X	15.93	94.8	32.6	9.55	121.3	$\pm 2.5 \%$
		Y	19.12	99.6	34.3		147.2	
		Z	19.09	99.8	34.3		135.4	
10027-DAB	GPRS-FDD (TDMA, GMSK, TN 0-1-2)	X	57.99	99.7	23.3	4.90	132.9	$\pm 1.9 \%$
		Y	54.04	99.8	23.8		131.2	
		Z	59.21	99.7	23.1		122.7	
10028-DAB	GPRS-FDD (TDMA, GMSK, TN 0-1-2-3)	X	62.80	99.8	22.5	3.55	139.9	$\pm 2.2 \%$
		Y	62.85	99.6	22.4		138.5	
		Z	84.57	99.8	21.8		129.1	
10029-DAB	EDGE-FDD (TDMA, 8PSK, TN 0-1-2)	X	18.17	94.0	30.7	7.78	137.1	$\pm 2.7 \%$
		Y	19.76	99.6	33.0		134.5	
		Z	15.07	93.3	30.5		125.4	
10039-CAB	CDMA2000 (1xRTT, RC1)	X	4.90	68.8	18.9	4.57	144.7	$\pm 1.2 \%$
		Y	4.88	67.3	19.3		145.2	
		Z	4.65	65.0	18.3		136.8	
10058-DAB	EDGE-FDD (TDMA, 8PSK, TN 0-1-2-3)	X	14.14	91.7	29.2	6.52	142.1	$\pm 1.9 \%$
		Y	18.83	98.5	31.7		141.2	
		Z	11.43	87.2	27.3		131.6	
10081-CAB	CDMA2000 (1xRTT, RC3)	X	3.96	65.9	18.2	3.97	138.0	$\pm 0.7 \%$
		Y	3.99	66.5	18.8		138.7	
		Z	3.77	65.0	17.6		131.9	

Certificate No: ES3-3122_Jun15

Page 4 of 12

ES3DV3- SN.3122

June 19, 2010

10080-DAB	GPRS-FDD (TDMA, GMSK, TN 0-4)	X	42.71	99.9	25.1	6.56	147.2	±1.9 %
		Y	39.29	99.6	25.2		119.4	
		Z	40.45	99.7	25.0		135.9	
10089-DAB	EDGE-FDD (TDMA, 8PSK, TN 0-4)	X	10.62	86.0	29.5	9.55	98.1	±3.0 %
		Y	15.63	97.2	34.3		96.6	
		Z	10.00	85.3	29.3		91.4	
10290-AAB	CDMA2000, RC1, SO55, Full Rate	X	4.46	67.1	18.6	3.91	143.1	±0.9 %
		Y	4.40	67.5	19.0		143.6	
		Z	4.15	66.0	17.9		134.7	
10291-AAB	CDMA2000, RC3, SO55, Full Rate	X	3.63	66.2	18.1	3.46	137.6	±0.7 %
		Y	3.65	66.6	18.7		138.2	
		Z	3.40	65.0	17.3		130.5	
10292-AAB	CDMA2000, RC3, SO32, Full Rate	X	3.58	66.3	18.2	3.39	137.6	±0.7 %
		Y	3.63	67.1	18.8		137.8	
		Z	3.39	65.3	17.5		130.2	
10293-AAB	CDMA2000, RC3, SO3, Full Rate	X	3.68	66.4	18.3	3.50	137.4	±0.7 %
		Y	3.67	66.8	18.7		138.4	
		Z	3.43	65.0	17.3		130.3	
10295-AAB	CDMA2000, RC1, SO3, 1/8th Rate 25 fr.	X	14.16	89.1	34.0	12.49	103.9	±2.2 %
		Y	19.23	99.6	38.9		102.8	
		Z	14.30	90.6	35.0		94.2	
10403-AAB	CDMA2000 (1xEV-DO, Rev. 0)	X	4.62	66.7	17.9	3.76	127.8	±0.7 %
		Y	4.64	67.4	18.4		127.7	
		Z	4.57	66.9	17.8		142.5	
10404-AAB	CDMA2000 (1xEV-DO, Rev. A)	X	4.75	67.7	18.4	3.77	149.9	±0.7 %
		Y	4.74	68.3	18.9		149.9	
		Z	4.41	66.6	17.7		140.6	
10406-AAB	CDMA2000, RC3, SO32, SCH0, Full Rate	X	6.18	67.6	19.1	5.22	132.8	±1.2 %
		Y	6.23	68.4	19.6		132.7	
		Z	6.19	68.1	19.1		148.3	

The reported uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor $k=2$, which for a normal distribution corresponds to a coverage probability of approximately 95%.

^a The uncertainties of Norm X, Y, Z do not affect the E²-field uncertainty inside TSL (see Pages 6 and 7).
^b Numerical linearization parameter: uncertainty not required.
^c Uncertainty is determined using the max. deviation from linear response applying rectangular distribution and is expressed for the square of the field value.

ES3DV3-SN:3122

June 19, 2015

DASY/EASY - Parameters of Probe: ES3DV3 - SN:3122

Calibration Parameter Determined in Head Tissue Simulating Media

f (MHz) ^c	Relative Permittivity ^f	Conductivity (S/m) ^e	ConvF X	ConvF Y	ConvF Z	Alpha ^d	Depth ^g (mm)	Unct. (k=2)
150	52.3	0.76	7.00	7.00	7.00	0.08	1.20	± 13.3 %
300	45.3	0.87	6.79	6.79	6.79	0.15	1.20	± 13.3 %
450	43.5	0.87	6.79	6.79	6.79	0.21	1.30	± 13.3 %
750	41.9	0.89	6.39	6.39	6.39	0.33	1.75	± 12.0 %
900	41.5	0.97	6.02	6.02	6.02	0.46	1.51	± 12.0 %
1810	40.0	1.40	5.07	5.07	5.07	0.59	1.40	± 12.0 %
1900	40.0	1.40	5.02	5.02	5.02	0.80	1.16	± 12.0 %
2450	39.2	1.80	4.46	4.46	4.46	0.80	1.31	± 12.0 %

^c Frequency validity above 300 MHz or ± 100 MHz only applies for DASY v4.4 and higher (see Page 2), else it is restricted to ± 50 MHz. The uncertainty is the RSS of the ConvF uncertainty at calibration frequency and the uncertainty for the indicated frequency band. Frequency validity below 300 MHz is ± 10, 25, 40, 50 and 70 MHz for ConvF assessments at 30, 50, 126, 150 and 220 MHz respectively. Above 5 GHz frequency validity can be extended to ± 110 MHz.

^f At frequencies below 3 GHz, the validity of tissue parameters (ϵ and σ) can be relaxed to ± 10% if liquid compensation formula is applied to measured SAR values. At frequencies above 3 GHz, the validity of tissue parameters (ϵ and σ) is restricted to ± 5%. The uncertainty is the RSS of the ConvF uncertainty for indicated target tissue parameters.

^g Alpha/Depth are determined during calibration. BPCAG warrants that the remaining deviation due to the boundary effect after compensation is always less than ± 1% for frequencies below 3 GHz and below ± 2% for frequencies between 3-6 GHz at any distance larger than half the probe tip diameter from the boundary.

ES3DV3- SN:3122

June 18, 2015

DASY/EASY - Parameters of Probe: ES3DV3 - SN:3122

Calibration Parameter Determined in Body Tissue Simulating Media

f (MHz) ^E	Relative Permittivity ^F	Conductivity (S/m) ^F	ConvF X	ConvF Y	ConvF Z	Alpha ^G	Depth ^G (mm)	Unct. (k=2)
150	61.9	0.80	6.58	6.58	6.58	0.06	1.20	± 13.3 %
300	58.2	0.92	6.71	6.71	6.71	0.12	1.30	± 13.3 %
450	56.7	0.94	6.78	6.78	6.78	0.15	1.30	± 13.3 %
750	55.5	0.96	6.06	6.06	6.06	0.55	1.38	± 12.0 %
900	55.0	1.05	5.88	5.88	5.88	0.46	1.45	± 12.0 %
1810	53.3	1.52	4.74	4.74	4.74	0.38	1.85	± 12.0 %
1900	53.3	1.52	4.63	4.63	4.63	0.43	1.76	± 12.0 %
2450	52.7	1.95	4.28	4.28	4.28	0.60	1.20	± 12.0 %

^E Frequency validity above 300 MHz of ± 100 MHz only applies for DASY v4.4 and higher (see Page 2), else it is restricted to ± 50 MHz. The uncertainty is the RSS of the ConvF uncertainty at calibration frequency and the uncertainty for the indicated frequency band. Frequency validity below 300 MHz is ± 10, 25, 40, 50 and 70 MHz for ConvF assessments at 30, 60, 120, 150 and 220 MHz respectively. Above 5 GHz frequency validity can be extended to ± 110 MHz.


^F At frequencies below 3 GHz, the validity of tissue parameters (ε and σ) can be relaxed to ± 10% if liquid compensation formula is applied to measured SAR values. At frequencies above 3 GHz, the validity of tissue parameters (ε and σ) is restricted to ± 5%. The uncertainty is the RSS of the ConvF uncertainty for indicated target tissue parameters.

^G Alpha/Depth are determined during calibration. SPEAG warrants that the remaining deviation due to the boundary effect after compensation is always less than ± 1% for frequencies below 3 GHz and below ± 2% for frequencies between 3-6 GHz at any distance larger than half the probe tip diameter from the boundary.

ES3DV3- SN:3122

June 19, 2015

Frequency Response of E-Field (TEM-Cell:ift110 EXX, Waveguide: R22)


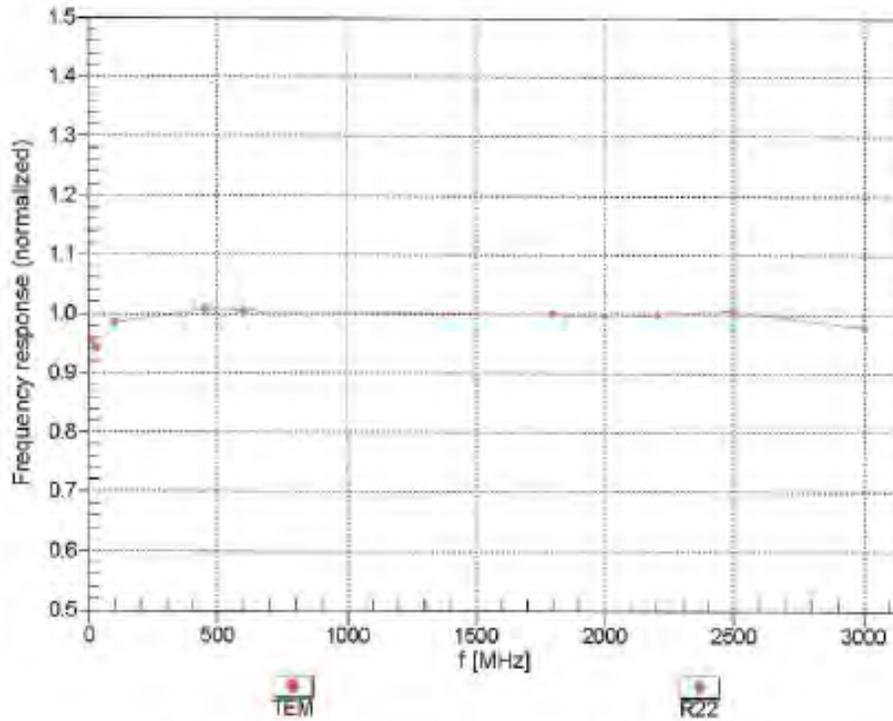


Uncertainty of Frequency Response of E-field: $\pm 6.3\%$ (k=2)

Receiving Pattern (ϕ), $\theta = 0^\circ$

f=600 MHz,TEM

f=1800 MHz,R22

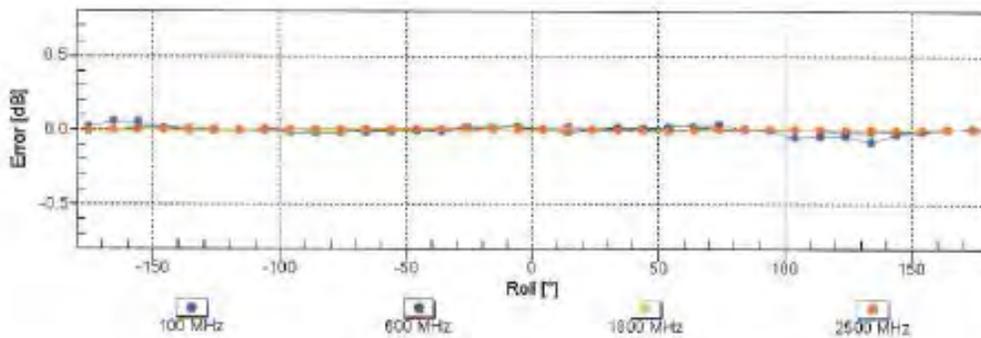
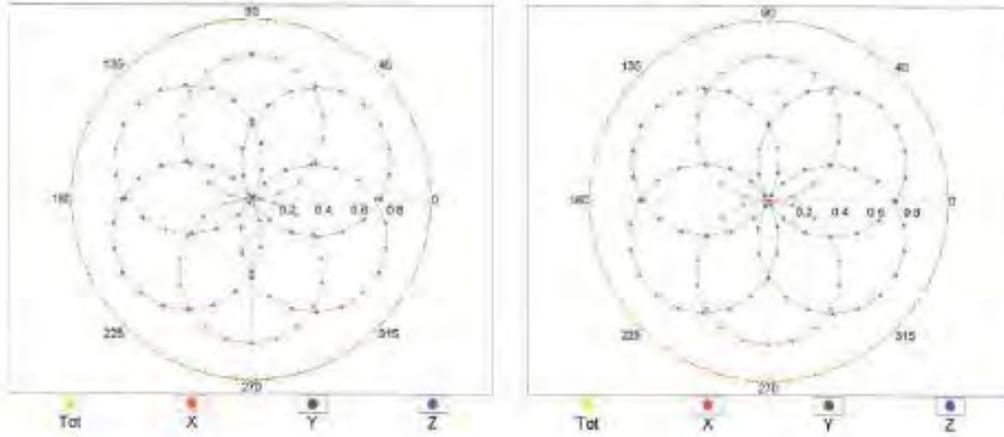


Uncertainty of Axial Isotropy Assessment: $\pm 0.5\%$ ($k=2$)

ES3DV3- SN:3122


June 19, 2015

Dynamic Range $f(\text{SAR}_{\text{head}})$ (TEM cell, $f_{\text{eval}} = 1900 \text{ MHz}$)

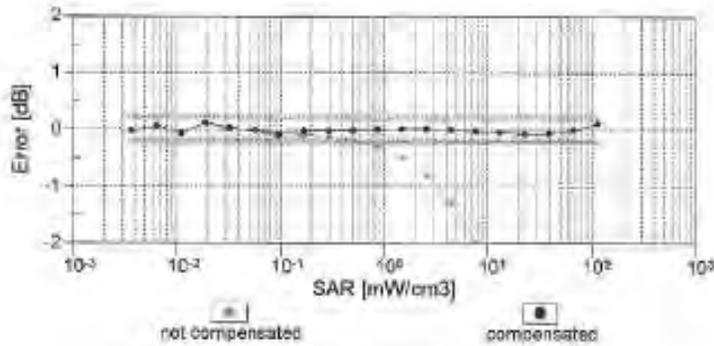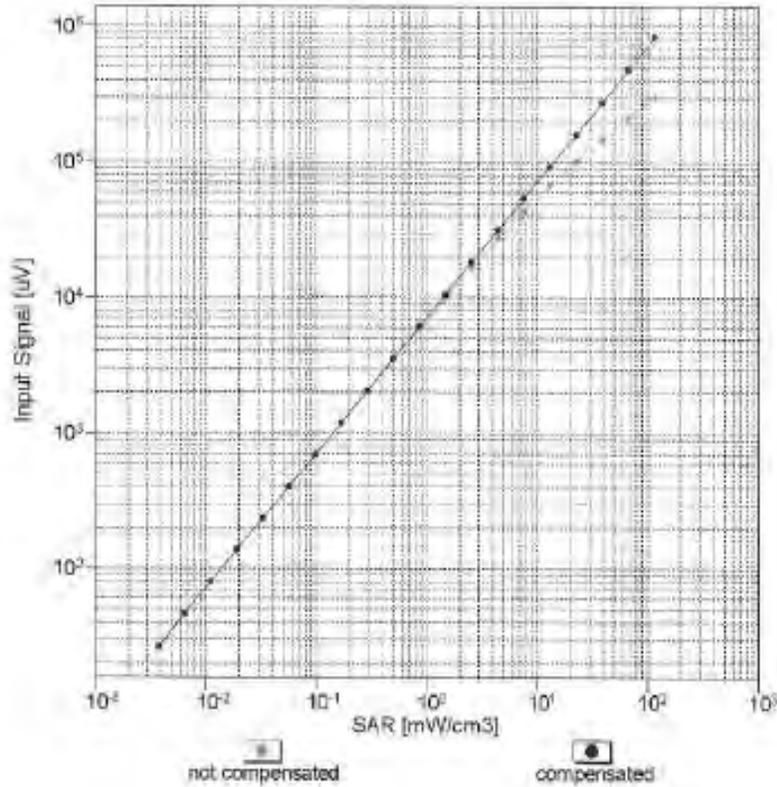


Uncertainty of Linearity Assessment: $\pm 0.6\%$ ($k=2$)

Conversion Factor Assessment

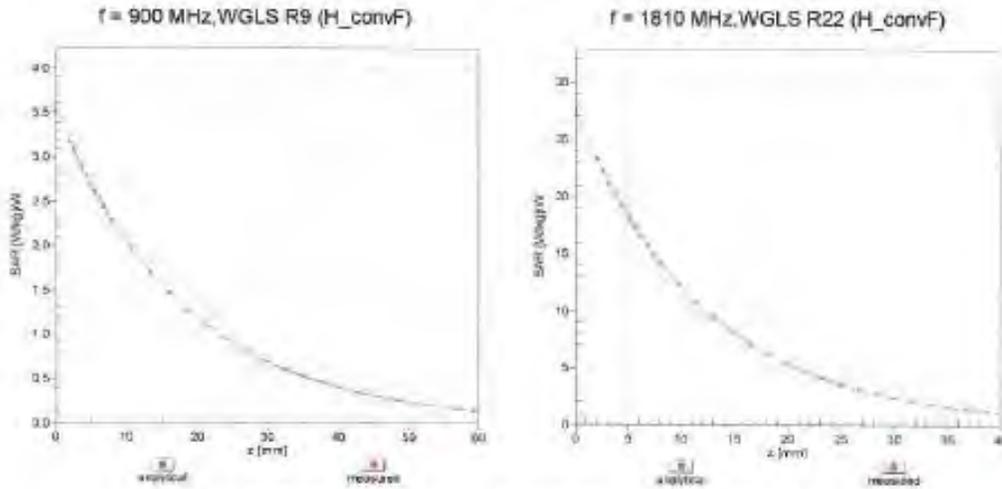

Deviation from Isotropy in Liquid Error (ϕ, θ), f = 900 MHz

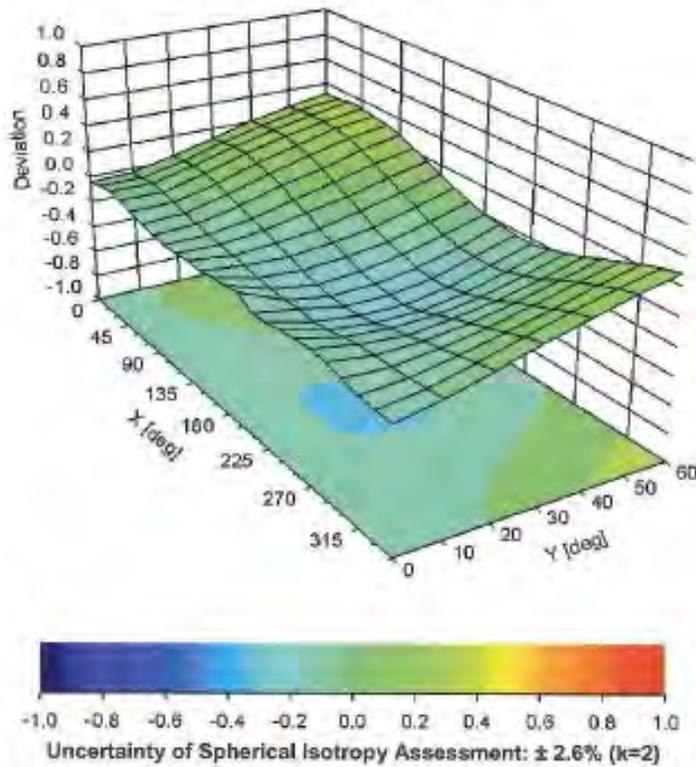

ES3DV5- SN:3122

June 19, 2015

DASY/EASY - Parameters of Probe: ES3DV3 - SN:3122

Other Probe Parameters

Sensor Arrangement	Triangular
Connector Angle (°)	24.1
Mechanical Surface Detection Mode	enabled
Optical Surface Detection Mode	disabled
Probe Overall Length	337 mm
Probe Body Diameter	10 mm
Tip Length	10 mm
Tip Diameter	4 mm
Probe Tip to Sensor X Calibration Point	2 mm
Probe Tip to Sensor Y Calibration Point	2 mm
Probe Tip to Sensor Z Calibration Point	2 mm
Recommended Measurement Distance from Surface	3 mm

**Calibration Laboratory of
Schmid & Partner
Engineering AG**
Zaughausstrasse 43, 8004 Zurich, Switzerland



S Schweizerischer Kalibrierdienst
C Service suisse d'étalonnage
S Servizio svizzero di tarature
S Swiss Calibration Service

Accredited by the Swiss Accreditation Service (SA5)
The Swiss Accreditation Service is one of the signatories to the EA
Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: **SCS 0108**

Client: **Motorola Solutions MY**

Certificate No: **EX3-7364_Jun15**

CALIBRATION CERTIFICATE

Object: **EX3DV4 - SN:7364**

Calibration procedure(s): **QA CAL-01.v9, QA CAL-12.v9, QA CAL-14.v4, QA CAL-23.v5,
QA CAL-25.v8
Calibration procedure for dosimetric E-field probes**

Calibration date: **June 23, 2015**

This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI).
The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility: environment temperature (22 ± 3)°C and humidity < 70%.

Calibration Equipment used (M&IE critical for calibration):

Primary Standards	ID	Cal Date (Certificate No.)	Scheduled Calibration
Power meter E4419B	GB41293874	01-Apr-15 (No. 217-02128)	Mar-16
Power sensor E4412A	MY41488087	01-Apr-15 (No. 217-02128)	Mar-16
Reference 3 dB Attenuator	SN: S5054 (3c)	01-Apr-15 (No. 217-02129)	Mar-16
Reference 20 dB Attenuator	SN: S5277 (20x)	01-Apr-15 (No. 217-02132)	Mar-16
Reference 30 dB Attenuator	SN: S5129 (30b)	01-Apr-15 (No. 217-02133)	Mar-16
Reference Probe ES3DVZ	SN: 3013	30-Dec-14 (No. ES3-3013_Dec14)	Dec-15
DAE4	SN: 660	14-Jan-15 (No. DAE4-660_Jan15)	Jan-16
Secondary Standards	ID	Check Date (in house)	Scheduled Check
RF generator HP 8648C	US3642U01700	4-Aug-09 (in house check Apr-15)	In house check: Apr-16
Network Analyzer HP 8753E	US37390585	18-Oct-01 (in house check Oct-14)	In house check: Oct-15

Calibrated by:	Name Claudio Leuter	Function Laboratory Technician	Signature
Approved by:	Name Katja Pokovic	Function Technical Manager	

Issued: June 24, 2015

This calibration certificate shall not be reproduced except in full without written approval of the laboratory.

**Calibration Laboratory of
Schmid & Partner
Engineering AG**
Zaughausstrasse 43, 8004 Zurich, Switzerland



S Schweizerischer Kalibrierdienst
S Service suisse d'étalonnage
S Servizio svizzero di taratura
S Swiss Calibration Service

Accredited by the Swiss Accreditation Service (SAS)

Accreditation No.: **SCS 0108**

The Swiss Accreditation Service is one of the signatories to the EA
Multilateral Agreement for the recognition of calibration certificates

Glossary:

TSL	tissue simulating liquid
NORM _{x,y,z}	sensitivity in free space
ConvF	sensitivity in TSL / NORM _{x,y,z}
DCP	diode compression point
CF	crest factor (1/duty_cycle) of the RF signal
A, B, C, D	modulation dependent linearization parameters
Polarization φ	φ rotation around probe axis
Polarization θ	θ rotation around an axis that is in the plane normal to probe axis (at measurement center) i.e., $\theta = 0$ is normal to probe axis
Connector Angle	information used in DASY system to align probe sensor X to the robot coordinate system

Calibration is Performed According to the Following Standards:

- a) IEEE Std 1528-2013, "IEEE Recommended Practice for Determining the Peak Spatial-Averaged Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques", June 2013
- b) IEC 62209-1, "Procedure to measure the Specific Absorption Rate (SAR) for hand-held devices used in close proximity to the ear (frequency range of 300 MHz to 3 GHz)", February 2005

Methods Applied and Interpretation of Parameters:

- **NORM_{x,y,z}**: Assessed for E-field polarization $\theta = 0$ ($f < 900$ MHz in TEM-cell; $f > 1800$ MHz: R22 waveguide). NORM_{x,y,z} are only intermediate values, i.e., the uncertainties of NORM_{x,y,z} does not affect the E²-field uncertainty inside TSL (see below ConvF).
- **NORM(f)_{x,y,z} = NORM_{x,y,z} * frequency_response** (see Frequency Response Chart). This linearization is implemented in DASY4 software versions later than 4.2. The uncertainty of the frequency response is included in the stated uncertainty of ConvF.
- **DCP_{x,y,z}**: DCP are numerical linearization parameters assessed based on the data of power sweep with CW signal (no uncertainty required). DCP does not depend on frequency nor media.
- **PAR**: PAR is the Peak to Average Ratio that is not calibrated but determined based on the signal characteristics.
- **A_{x,y,z}; B_{x,y,z}; C_{x,y,z}; D_{x,y,z}; VR_{x,y,z}; A, B, C, D** are numerical linearization parameters assessed based on the data of power sweep for specific modulation signal. The parameters do not depend on frequency nor media. VR is the maximum calibration range expressed in RMS voltage across the diode.
- **ConvF and Boundary Effect Parameters**: Assessed in flat phantom using E-field (or Temperature Transfer Standard for $f \leq 800$ MHz) and inside waveguide using analytical field distributions based on power measurements for $f > 800$ MHz. The same setups are used for assessment of the parameters applied for boundary compensation (alpha, depth) of which typical uncertainty values are given. These parameters are used in DASY4 software to improve probe accuracy close to the boundary. The sensitivity in TSL corresponds to NORM_{x,y,z} * ConvF whereby the uncertainty corresponds to that given for ConvF. A frequency dependent ConvF is used in DASY version 4.4 and higher which allows extending the validity from ± 50 MHz to ± 100 MHz.
- **Spherical isotropy (3D deviation from isotropy)**: in a field of low gradients realized using a flat phantom exposed by a patch antenna.
- **Sensor Offset**: The sensor offset corresponds to the offset of virtual measurement center from the probe lip (on probe axis). No tolerance required.
- **Connector Angle**: The angle is assessed using the information gained by determining the NORM_x (no uncertainty required).

EX3DV4 – SN:7364

June 23, 2015

Probe EX3DV4

SN:7364

Manufactured: February 5, 2015
Calibrated: June 23, 2015

Calibrated for DASY/EASY Systems
(Note: non-compatible with DASY2 systems)

EX3DV4- SN:7364

June 23, 2015

DASY/EASY - Parameters of Probe: EX3DV4 - SN:7364

Basic Calibration Parameters

	Sensor X	Sensor Y	Sensor Z	Unc. (k=2)
Norm ($\mu\text{V}/(\text{V}/\text{m})^2$) ^A	0.48	0.46	0.59	$\pm 10.1\%$
DCP (mV) ^B	97.7	96.3	97.3	

Modulation Calibration Parameters

UID	Communication System Name		A dB	B dB $\sqrt{\mu\text{V}}$	C	D dB	VR mV	Unc. (k=2)
0	CW	X	0.0	0.0	1.0	0.00	115.0	$\pm 3.5\%$
		Y	0.0	0.0	1.0		110.5	
		Z	0.0	0.0	1.0		124.6	
10011-CAB	UMTS-FDD (WCDMA)	X	3.42	67.2	18.6	2.91	122.6	$\pm 0.5\%$
		Y	3.14	64.8	18.9		117.5	
		Z	3.46	67.3	18.5		135.3	
10012-CAB	IEEE 802.11b WiFi 2.4 GHz (DSSS, 1 Mbps)	X	2.86	68.1	18.5	1.87	122.4	$\pm 0.5\%$
		Y	2.39	63.9	15.8		117.3	
		Z	3.01	69.0	18.8		135.0	
10013-CAB	IEEE 802.11g WiFi 2.4 GHz (DSSS-OFDM, 6 Mbps)	X	10.47	68.7	22.2	9.46	115.4	$\pm 2.7\%$
		Y	10.30	68.1	21.6		107.3	
		Z	10.58	69.3	22.6		126.2	
10059-CAB	IEEE 802.11b WiFi 2.4 GHz (DSSS, 2 Mbps)	X	3.03	69.0	19.0	2.12	120.5	$\pm 0.5\%$
		Y	2.58	65.1	16.6		115.0	
		Z	2.93	68.2	18.4		133.3	
10060-CAB	IEEE 802.11b WiFi 2.4 GHz (DSSS, 5.5 Mbps)	X	3.74	77.3	22.8	2.83	148.9	$\pm 0.5\%$
		Y	2.75	70.3	19.2		141.7	
		Z	3.40	75.1	21.8		118.6	
10061-CAB	IEEE 802.11b WiFi 2.4 GHz (DSSS, 11 Mbps)	X	3.83	73.4	21.4	3.60	145.6	$\pm 0.7\%$
		Y	3.06	68.2	18.5		139.1	
		Z	3.96	74.0	21.7		117.9	
10062-CAB	IEEE 802.11a/b WiFi 5 GHz (OFDM, 6 Mbps)	X	10.17	66.5	21.5	8.68	116.8	$\pm 2.5\%$
		Y	9.91	67.6	20.8		107.4	
		Z	10.99	69.3	22.0		132.5	
10063-CAB	IEEE 802.11a/b WiFi 5 GHz (OFDM, 9 Mbps)	X	10.01	68.4	21.4	8.63	116.3	$\pm 2.5\%$
		Y	9.65	67.7	20.9		108.8	
		Z	10.24	69.2	22.0		131.7	
10064-CAB	IEEE 802.11a/b WiFi 5 GHz (OFDM, 12 Mbps)	X	10.46	68.7	21.9	9.09	117.4	$\pm 2.7\%$
		Y	10.34	68.2	21.3		110.7	
		Z	10.69	69.6	22.5		132.1	
10065-CAB	IEEE 802.11a/b WiFi 5 GHz (OFDM, 18 Mbps)	X	10.10	68.4	21.7	9.00	113.5	$\pm 2.5\%$
		Y	10.01	68.0	21.2		107.5	
		Z	10.29	69.2	22.2		127.8	
10066-CAB	IEEE 802.11a/b WiFi 5 GHz (OFDM, 24 Mbps)	X	10.32	68.7	22.1	9.38	113.2	$\pm 2.5\%$
		Y	10.20	68.1	21.6		106.0	
		Z	10.49	69.4	22.6		125.8	

EX3DV4-SN:7364

June 23, 2015

10067-CAB	IEEE 802.11a/n WiFi 5 GHz (OFDM, 36 Mbps)	X	10.83	69.1	22.8	10.12	111.9	±3.0 %
		Y	10.70	68.6	22.3		105.5	
		Z	11.04	70.0	23.5		125.5	
10068-CAB	IEEE 802.11a/n WiFi 5 GHz (OFDM, 48 Mbps)	X	10.64	69.0	22.9	10.24	108.5	±3.3 %
		Y	11.07	70.0	23.2		145.3	
		Z	10.83	69.9	23.5		121.7	
10069-CAB	IEEE 802.11a/n WiFi 5 GHz (OFDM, 54 Mbps)	X	10.95	69.2	23.2	10.56	109.6	±3.5 %
		Y	11.38	70.3	23.6		148.1	
		Z	11.13	70.1	23.8		122.0	
10071-CAB	IEEE 802.11g WiFi 2.4 GHz (DSSS/OFDM, 9 Mbps)	X	10.46	68.7	22.4	9.83	110.6	±2.5 %
		Y	10.36	68.2	21.9		105.8	
		Z	10.71	69.6	23.1		124.2	
10072-CAB	IEEE 802.11g WiFi 2.4 GHz (DSSS/OFDM, 12 Mbps)	X	10.01	68.4	22.2	9.62	106.7	±3.0 %
		Y	10.38	69.2	22.4		144.1	
		Z	10.18	69.1	22.7		119.4	
10073-CAB	IEEE 802.11g WiFi 2.4 GHz (DSSS/OFDM, 18 Mbps)	X	10.78	70.9	23.9	9.94	149.7	±3.0 %
		Y	10.27	69.1	22.6		139.1	
		Z	10.17	69.3	23.1		115.9	
10074-CAB	IEEE 802.11g WiFi 2.4 GHz (DSSS/OFDM, 24 Mbps)	X	10.82	71.0	24.2	10.30	144.0	±3.3 %
		Y	10.30	69.2	22.9		131.6	
		Z	10.22	69.5	23.4		111.6	
10075-CAB	IEEE 802.11g WiFi 2.4 GHz (DSSS/OFDM, 36 Mbps)	X	10.91	71.3	24.8	10.77	138.9	±3.3 %
		Y	10.34	69.2	23.3		129.4	
		Z	10.31	69.7	23.9		108.0	
10076-CAB	IEEE 802.11g WiFi 2.4 GHz (DSSS/OFDM, 48 Mbps)	X	10.84	71.1	24.9	10.94	134.9	±3.3 %
		Y	10.25	69.0	23.3		125.9	
		Z	10.28	69.7	24.1		106.3	
10077-CAB	IEEE 802.11g WiFi 2.4 GHz (DSSS/OFDM, 54 Mbps)	X	10.61	71.1	24.9	11.00	133.2	±3.5 %
		Y	10.23	69.1	23.4		124.7	
		Z	11.06	72.3	25.8		148.3	
10097-CAB	UMTS-FDD (HSDPA)	X	4.84	66.4	18.3	3.98	129.4	±0.7 %
		Y	4.47	65.1	17.4		126.4	
		Z	4.82	67.2	18.8		144.7	
10096-CAB	UMTS-FDD (HSUPA, Subtest 2)	X	4.66	66.5	18.4	3.98	130.1	±0.7 %
		Y	4.50	65.3	17.5		126.7	
		Z	4.78	67.0	18.7		145.5	
10100-CAB	LTE-FDD (SC-FDMA, 100% RB, 20 MHz, QPSK)	X	6.58	67.6	19.7	5.67	136.1	±1.4 %
		Y	6.37	66.4	18.8		131.7	
		Z	6.14	66.0	18.9		107.5	
10101-CAB	LTE-FDD (SC-FDMA, 100% RB, 20 MHz, 16-QAM)	X	7.69	67.9	20.1	6.42	146.1	±1.7 %
		Y	7.50	67.0	19.4		140.3	
		Z	7.24	66.6	19.5		115.2	
10102-CAB	LTE-FDD (SC-FDMA, 100% RB, 20 MHz, 64-QAM)	X	8.00	68.2	20.4	6.60	148.5	±1.7 %
		Y	7.78	67.2	19.6		141.8	
		Z	7.54	66.9	19.7		117.4	

EX3DV4-- SN:7364

June 23, 2015

10108-CAC	LTE-FDD (SC-FDMA, 100% RB, 10 MHz, QPSK)	X	6.41	67.0	19.5	5.80	133.0	±1.2 %
		Y	6.24	66.1	18.8		128.4	
		Z	6.04	65.7	18.9		106.2	
10109-CAC	LTE-FDD (SC-FDMA, 100% RB, 10 MHz, 16-QAM)	X	7.40	67.6	20.0	6.43	141.0	±1.7 %
		Y	7.23	66.7	19.3		135.5	
		Z	6.98	66.3	19.4		111.0	
10110-CAC	LTE-FDD (SC-FDMA, 100% RB, 5 MHz, QPSK)	X	6.05	66.5	19.2	5.75	129.1	±1.4 %
		Y	5.89	65.5	18.5		124.3	
		Z	6.26	67.4	19.9		145.9	
10111-CAC	LTE-FDD (SC-FDMA, 100% RB, 5 MHz, 16-QAM)	X	7.12	67.4	20.0	6.44	136.5	±1.4 %
		Y	6.94	66.5	19.2		130.6	
		Z	6.69	66.0	19.3		107.3	
10112-CAC	LTE-FDD (SC-FDMA, 100% RB, 10 MHz, 64-QAM)	X	7.64	67.8	20.2	6.59	142.4	±1.7 %
		Y	7.46	66.9	19.5		136.7	
		Z	7.21	66.5	19.6		111.3	
10113-CAC	LTE-FDD (SC-FDMA, 100% RB, 5 MHz, 64-QAM)	X	7.32	67.5	20.1	6.62	137.7	±1.7 %
		Y	7.15	66.6	19.4		131.4	
		Z	6.92	66.2	19.4		108.9	
10114-CAB	IEEE 802.11n (HT Greenfield, 13.5 Mbps, BPSK)	X	10.23	68.5	21.0	8.10	124.2	±2.5 %
		Y	10.04	67.9	20.5		117.0	
		Z	10.56	69.5	21.7		142.7	
10115-CAB	IEEE 802.11n (HT Greenfield, 81 Mbps, 16-QAM)	X	10.80	69.1	21.5	8.46	128.6	±2.5 %
		Y	10.61	68.5	21.0		120.9	
		Z	11.08	70.0	22.1		145.6	
10116-CAB	IEEE 802.11n (HT Greenfield, 135 Mbps, 64-QAM)	X	10.31	68.7	21.1	8.15	125.0	±2.5 %
		Y	10.13	68.1	20.8		118.2	
		Z	10.59	69.6	21.7		142.4	
10117-CAB	IEEE 802.11n (HT Mixed, 13.5 Mbps, BPSK)	X	10.27	68.8	21.1	8.07	125.9	±2.5 %
		Y	10.08	68.0	20.5		119.0	
		Z	10.52	69.4	21.6		142.8	
10118-CAB	IEEE 802.11n (HT Mixed, 81 Mbps, 16-QAM)	X	10.91	69.2	21.7	8.59	128.3	±2.5 %
		Y	10.70	68.6	21.1		121.2	
		Z	11.21	70.2	22.3		146.3	
10119-CAB	IEEE 802.11n (HT Mixed, 135 Mbps, 64-QAM)	X	10.27	68.6	21.1	8.13	125.1	±2.5 %
		Y	10.10	68.0	20.6		118.1	
		Z	10.57	69.6	21.7		142.8	
10140-CAB	LTE-FDD (SC-FDMA, 100% RB, 15 MHz, 16-QAM)	X	7.93	68.3	20.4	6.49	147.7	±1.7 %
		Y	7.73	67.4	19.6		142.8	
		Z	7.42	66.8	19.6		116.6	
10141-CAB	LTE-FDD (SC-FDMA, 100% RB, 15 MHz, 64-QAM)	X	8.04	68.2	20.3	6.53	149.1	±1.7 %
		Y	7.84	67.4	19.6		143.2	
		Z	7.56	66.9	19.7		117.6	
10142-CAC	LTE-FDD (SC-FDMA, 100% RB, 3 MHz, QPSK)	X	5.83	66.2	19.1	5.73	125.7	±1.2 %
		Y	5.68	65.2	18.4		121.2	
		Z	6.04	67.0	19.6		142.9	

EX3DV4- SN:7364

June 23, 2015

10143-CAC	LTE-FDD (SC-FDMA, 100% RB, 3 MHz, 16-QAM)	X	6.82	67.3	19.9	6.35	131.4	±1.4 %
		Y	6.65	66.3	19.1		126.5	
		Z	7.04	68.1	20.4		148.1	
10144-CAC	LTE-FDD (SC-FDMA, 100% RB, 3 MHz, 64-QAM)	X	7.15	67.5	20.1	6.65	132.6	±1.4 %
		Y	6.96	66.6	19.4		127.2	
		Z	7.36	68.4	20.7		149.1	
10145-CAC	LTE-FDD (SC-FDMA, 100% RB, 1.4 MHz, QPSK)	X	5.54	65.9	19.0	5.76	120.5	±1.2 %
		Y	5.42	65.1	18.3		116.1	
		Z	5.76	66.9	19.6		135.7	
10146-CAC	LTE-FDD (SC-FDMA, 100% RB, 1.4 MHz, 16-QAM)	X	6.48	67.3	19.9	6.41	124.0	±1.4 %
		Y	6.28	66.2	19.1		119.2	
		Z	6.70	68.1	20.4		140.0	
10147-CAC	LTE-FDD (SC-FDMA, 100% RB, 1.4 MHz, 64-QAM)	X	6.74	67.4	20.1	6.72	124.3	±1.7 %
		Y	6.55	66.4	19.4		119.3	
		Z	6.97	68.3	20.7		140.2	
10149-CAB	LTE-FDD (SC-FDMA, 50% RB, 20 MHz, 16-QAM)	X	7.35	67.4	19.9	6.42	138.2	±1.4 %
		Y	7.17	66.5	19.2		133.3	
		Z	6.97	66.3	19.4		109.6	
10150-CAB	LTE-FDD (SC-FDMA, 50% RB, 20 MHz, 64-QAM)	X	7.61	67.7	20.1	6.60	140.5	±1.4 %
		Y	7.45	66.9	19.5		135.0	
		Z	7.22	66.5	19.6		112.4	
10154-CAC	LTE-FDD (SC-FDMA, 50% RB, 10 MHz, QPSK)	X	6.03	66.4	19.2	5.75	127.0	±1.4 %
		Y	5.85	65.3	18.4		122.3	
		Z	6.24	67.3	19.8		145.2	
10155-CAC	LTE-FDD (SC-FDMA, 50% RB, 10 MHz, 16-QAM)	X	7.06	67.2	19.8	6.43	134.1	±1.4 %
		Y	6.91	66.4	19.2		128.7	
		Z	6.69	66.1	19.3		107.1	
10156-CAC	LTE-FDD (SC-FDMA, 50% RB, 5 MHz, QPSK)	X	5.76	66.0	19.1	5.79	123.3	±1.2 %
		Y	5.63	65.1	18.3		118.7	
		Z	5.97	67.0	19.7		139.3	
10157-CAC	LTE-FDD (SC-FDMA, 50% RB, 5 MHz, 16-QAM)	X	6.80	67.2	19.9	6.49	128.7	±1.4 %
		Y	6.62	66.3	19.2		123.2	
		Z	6.99	68.0	20.4		144.9	
10158-CAC	LTE-FDD (SC-FDMA, 50% RB, 10 MHz, 64-QAM)	X	7.30	67.4	20.0	6.62	134.5	±1.4 %
		Y	7.12	66.5	19.3		129.0	
		Z	6.91	66.3	19.5		107.5	
10159-CAC	LTE-FDD (SC-FDMA, 50% RB, 5 MHz, 64-QAM)	X	6.91	67.4	20.0	6.56	129.3	±1.4 %
		Y	6.69	66.3	19.2		123.1	
		Z	7.12	68.2	20.5		145.9	
10160-CAB	LTE-FDD (SC-FDMA, 50% RB, 15 MHz, QPSK)	X	6.54	67.1	19.6	5.82	132.9	±1.4 %
		Y	6.29	65.9	18.7		126.6	
		Z	6.71	67.9	20.0		149.3	
10161-CAB	LTE-FDD (SC-FDMA, 50% RB, 15 MHz, 16-QAM)	X	7.41	67.6	20.0	6.43	139.7	±1.7 %
		Y	7.22	66.6	19.3		133.2	
		Z	6.97	66.2	19.3		110.0	

EX3DV4- SN.7364

June 23, 2015

10162-CAB	LTE-FDD (SC-FDMA, 50% RB, 15 MHz, 64-QAM)	X	7.66	67.9	20.2	6.58	141.5	±1.7 %
		Y	7.48	67.0	19.5		134.6	
		Z	7.18	66.4	19.5		112.1	
10165-CAC	LTE-FDD (SC-FDMA, 50% RB, 1.4 MHz, QPSK)	X	4.96	65.8	18.8	5.46	115.4	±0.8 %
		Y	4.78	64.5	17.9		110.2	
		Z	5.13	66.5	19.3		130.4	
10167-CAC	LTE-FDD (SC-FDMA, 50% RB, 1.4 MHz, 16-QAM)	X	5.82	66.9	19.6	6.21	117.4	±1.2 %
		Y	5.60	65.7	18.8		109.9	
		Z	6.07	67.9	20.3		132.7	
10168-CAC	LTE-FDD (SC-FDMA, 50% RB, 1.4 MHz, 64-QAM)	X	6.28	67.1	20.0	6.79	117.2	±1.4 %
		Y	6.06	66.0	19.2		111.0	
		Z	6.49	67.9	20.6		132.0	
10169-CAB	LTE-FDD (SC-FDMA, 1 RB, 20 MHz, QPSK)	X	4.78	65.9	19.1	5.73	109.6	±1.2 %
		Y	4.92	66.1	19.0		145.5	
		Z	4.94	66.5	19.6		123.2	
10170-CAB	LTE-FDD (SC-FDMA, 1 RB, 20 MHz, 16-QAM)	X	5.36	66.3	19.7	6.52	107.4	±1.4 %
		Y	5.59	67.0	19.8		142.7	
		Z	5.61	67.4	20.4		121.7	
10171-AAB	LTE-FDD (SC-FDMA, 1 RB, 20 MHz, 64-QAM)	X	5.38	66.5	19.7	6.49	107.3	±1.4 %
		Y	5.55	67.1	19.8		144.6	
		Z	5.64	67.6	20.4		121.5	
10175-CAC	LTE-FDD (SC-FDMA, 1 RB, 10 MHz, QPSK)	X	4.71	65.4	18.6	5.72	107.7	±1.2 %
		Y	4.91	66.0	18.9		144.8	
		Z	4.91	66.3	19.4		122.3	
10176-CAC	LTE-FDD (SC-FDMA, 1 RB, 10 MHz, 16-QAM)	X	5.78	68.1	20.6	6.52	149.6	±1.4 %
		Y	5.57	66.9	19.7		142.9	
		Z	5.66	67.6	20.5		121.7	
10177-CAF	LTE-FDD (SC-FDMA, 1 RB, 5 MHz, QPSK)	X	5.05	67.1	19.7	5.73	150.0	±1.2 %
		Y	4.91	66.0	18.9		144.6	
		Z	4.93	66.5	19.5		122.4	
10178-CAC	LTE-FDD (SC-FDMA, 1 RB, 5 MHz, 16-QAM)	X	5.80	68.2	20.7	6.52	149.3	±1.4 %
		Y	5.59	67.0	19.8		142.5	
		Z	5.63	67.5	20.4		121.7	
10179-CAC	LTE-FDD (SC-FDMA, 1 RB, 10 MHz, 64-QAM)	X	5.80	68.3	20.7	6.50	149.2	±1.4 %
		Y	5.62	67.2	19.8		144.9	
		Z	5.61	67.5	20.4		121.4	
10180-CAC	LTE-FDD (SC-FDMA, 1 RB, 5 MHz, 64-QAM)	X	5.80	68.3	20.7	6.50	148.6	±1.4 %
		Y	5.60	67.1	19.8		144.4	
		Z	5.63	67.5	20.4		121.6	
10181-CAB	LTE-FDD (SC-FDMA, 1 RB, 15 MHz, QPSK)	X	5.04	67.0	19.7	5.72	149.4	±1.2 %
		Y	4.94	66.2	19.1		145.6	
		Z	4.92	66.4	19.5		122.1	
10182-CAB	LTE-FDD (SC-FDMA, 1 RB, 15 MHz, 16-QAM)	X	5.79	68.2	20.7	6.52	148.9	±1.4 %
		Y	5.57	66.9	19.7		142.2	
		Z	5.63	67.5	20.5		121.0	

Certificate No: EX3-7364_Jun15

Page 5 of 18

EX3DV4- SN:7364

June 23, 2015

10183-AAA	LTE-FDD (SC-FDMA, 1 RB, 15 MHz, 64-QAM)	X	5.81	68.4	20.8	6.50	148.4	±1.4 %
		Y	5.62	67.2	19.9		144.3	
		Z	5.62	67.5	20.4		121.1	
10184-CAC	LTE-FDD (SC-FDMA, 1 RB, 3 MHz, QPSK)	X	5.06	67.1	19.8	5.73	149.2	±1.2 %
		Y	4.91	66.0	18.9		144.9	
		Z	4.94	66.5	19.5		122.0	
10185-CAC	LTE-FDD (SC-FDMA, 1 RB, 3 MHz, 16-QAM)	X	5.77	68.1	20.6	6.51	148.4	±1.4 %
		Y	5.57	66.9	19.8		142.5	
		Z	5.62	67.5	20.4		121.5	
10186-AAC	LTE-FDD (SC-FDMA, 1 RB, 3 MHz, 64-QAM)	X	5.81	68.4	20.8	6.50	148.0	±1.7 %
		Y	5.63	67.3	19.9		144.7	
		Z	5.60	67.5	20.3		121.0	
10187-CAC	LTE-FDD (SC-FDMA, 1 RB, 1.4 MHz, QPSK)	X	5.07	67.1	19.8	5.73	149.3	±1.2 %
		Y	4.94	66.2	19.0		145.6	
		Z	4.91	66.3	19.4		122.3	
10188-CAC	LTE-FDD (SC-FDMA, 1 RB, 1.4 MHz, 16-QAM)	X	5.79	68.2	20.7	6.52	148.1	±1.7 %
		Y	5.57	66.9	19.7		142.5	
		Z	5.61	67.4	20.4		121.2	
10189-AAC	LTE-FDD (SC-FDMA, 1 RB, 1.4 MHz, 64-QAM)	X	5.83	68.5	20.8	6.50	148.1	±1.4 %
		Y	5.60	67.1	19.8		144.5	
		Z	5.64	67.6	20.4		121.5	
10193-CAB	IEEE 802.11n (HT Greenfield, 6.5 Mbps, BPSK)	X	9.64	67.7	20.6	8.09	112.5	±2.2 %
		Y	9.63	67.5	20.3		109.6	
		Z	10.04	68.9	21.4		132.4	
10194-CAB	IEEE 802.11n (HT Greenfield, 39 Mbps, 16-QAM)	X	9.78	68.0	20.9	8.12	116.1	±2.2 %
		Y	9.67	67.5	20.4		110.9	
		Z	10.06	68.9	21.5		131.8	
10195-CAB	IEEE 802.11n (HT Greenfield, 65 Mbps, 64-QAM)	X	9.93	68.3	21.0	8.21	117.1	±2.5 %
		Y	9.81	67.7	20.5		112.3	
		Z	10.19	69.1	21.5		134.2	
10196-CAB	IEEE 802.11n (HT Mixed, 6.5 Mbps, BPSK)	X	9.73	68.0	20.8	8.10	116.3	±2.2 %
		Y	9.62	67.5	20.3		111.7	
		Z	10.01	68.9	21.4		132.6	
10197-CAB	IEEE 802.11n (HT Mixed, 39 Mbps, 16-QAM)	X	9.77	68.0	20.8	8.13	116.4	±2.2 %
		Y	9.75	67.7	20.5		111.4	
		Z	10.10	69.0	21.5		132.9	
10198-CAB	IEEE 802.11n (HT Mixed, 65 Mbps, 64-QAM)	X	9.96	68.2	21.0	8.27	117.4	±2.5 %
		Y	9.88	67.8	20.6		112.8	
		Z	10.29	69.3	21.7		135.1	
10219-CAB	IEEE 802.11n (HT Mixed, 7.2 Mbps, BPSK)	X	9.62	67.9	20.8	8.03	116.5	±2.2 %
		Y	9.53	67.4	20.3		111.0	
		Z	9.94	68.9	21.4		132.9	
10220-CAB	IEEE 802.11n (HT Mixed, 43.3 Mbps, 16-QAM)	X	9.81	68.1	20.9	8.13	117.2	±2.2 %
		Y	9.70	67.6	20.4		111.6	
		Z	10.10	69.0	21.5		134.0	

EX3DV4- SN:7364

June 23, 2015

10221-CAB	IEEE 802.11n (HT Mixed, 72.2 Mbps, 64-QAM)	X	9.97	68.2	21.0	8.27	118.3	±2.5 %
		Y	9.89	67.8	20.6		112.7	
		Z	10.29	69.2	21.7		135.4	
10222-CAB	IEEE 802.11n (HT Mixed, 15 Mbps, BPSK)	X	10.14	68.4	20.9	8.06	122.8	±2.5 %
		Y	10.02	67.9	20.5		116.9	
		Z	10.48	69.4	21.6		140.6	
10223-CAB	IEEE 802.11n (HT Mixed, 90 Mbps, 16-QAM)	X	10.72	69.0	21.4	8.48	126.2	±2.5 %
		Y	10.54	68.3	20.9		119.3	
		Z	11.04	69.9	22.1		143.9	
10224-CAB	IEEE 802.11n (HT Mixed, 150 Mbps, 64-QAM)	X	10.13	68.4	20.9	8.08	123.4	±2.5 %
		Y	10.01	68.0	20.5		115.7	
		Z	10.44	69.3	21.5		140.3	
10225-CAB	UMTS-FDD (HSPA+)	X	7.19	67.5	19.6	5.97	143.8	±1.4 %
		Y	7.05	66.7	19.0		138.4	
		Z	6.78	66.2	19.0		112.5	
10274-CAB	UMTS-FDD (HSUPA, Subtest 5, 3GPP Rel8.10)	X	6.03	66.9	18.8	4.87	136.9	±1.2 %
		Y	5.89	66.1	18.1		131.5	
		Z	5.76	66.1	18.5		109.1	
10275-CAB	UMTS-FDD (HSUPA, Subtest 5, 3GPP Rel8.4)	X	4.32	65.7	18.0	3.96	119.3	±0.9 %
		Y	4.16	64.5	17.1		112.7	
		Z	4.57	66.9	18.7		136.2	
10297-AAA	LTE-FDD (SC-FDMA, 50% RB, 20 MHz, QPSK)	X	6.29	66.6	19.2	5.81	126.9	±1.4 %
		Y	6.12	65.6	18.5		120.7	
		Z	6.52	67.5	19.8		142.9	
10298-AAB	LTE-FDD (SC-FDMA, 50% RB, 3 MHz, QPSK)	X	5.62	66.1	19.1	5.72	120.8	±1.2 %
		Y	5.44	65.0	18.3		115.1	
		Z	5.80	66.9	19.6		136.0	
10299-AAB	LTE-FDD (SC-FDMA, 50% RB, 3 MHz, 16-QAM)	X	6.55	67.1	19.8	6.39	125.4	±1.4 %
		Y	6.35	66.1	19.0		119.2	
		Z	6.82	68.2	20.5		140.5	
10300-AAB	LTE-FDD (SC-FDMA, 50% RB, 3 MHz, 64-QAM)	X	6.73	67.3	20.0	6.60	125.1	±1.4 %
		Y	6.53	66.3	19.2		118.8	
		Z	6.99	68.2	20.6		140.9	
10311-AAA	LTE-FDD (SC-FDMA, 100% RB, 15 MHz, QPSK)	X	6.94	67.4	19.7	6.06	135.3	±1.4 %
		Y	6.75	66.4	19.0		129.1	
		Z	6.55	66.2	19.2		106.3	
10315-AAB	IEEE 802.11b WiFi 2.4 GHz (DSSS, 1 Mbps, 96pc duty cycle)	X	2.71	67.3	17.7	1.71	120.4	±0.5 %
		Y	2.36	64.0	15.7		114.8	
		Z	2.97	68.9	18.7		133.5	
10316-AAB	IEEE 802.11g WiFi 2.4 GHz (ERP-OFDM, 6 Mbps, 96pc duty cycle)	X	9.89	68.1	21.1	8.36	116.2	±2.5 %
		Y	9.75	67.5	20.5		108.9	
		Z	10.15	69.0	21.6		131.4	
10317-AAB	IEEE 802.11a WiFi 5 GHz (OFDM, 6 Mbps, 96pc duty cycle)	X	9.89	68.1	21.1	8.36	116.7	±2.5 %
		Y	9.76	67.6	20.6		110.0	
		Z	10.16	69.0	21.7		132.3	

EX3DV4- SN 7364

June 23, 2015

10415-AAA	IEEE 802.11b WiFi 2.4 GHz (DSSS, 1 Mbps, 99pc duty cycle)	X	2.58	66.6	17.4	1.54	122.6	±0.5 %
		Y	2.36	64.2	15.8		117.2	
		Z	2.79	68.0	18.2		136.1	
10416-AAA	IEEE 802.11g WiFi 2.4 GHz (ERP-OFDM, 6 Mbps, 99pc duty cycle)	X	9.83	68.1	21.0	8.23	117.6	±2.2 %
		Y	9.72	67.6	20.5		110.8	
		Z	10.12	69.0	21.6		132.8	
10417-AAA	IEEE 802.11a/n WiFi 5 GHz (OFDM, 6 Mbps, 99pc duty cycle)	X	9.82	68.1	20.9	8.23	117.7	±2.2 %
		Y	9.76	67.7	20.5		111.5	
		Z	10.11	69.0	21.6		133.6	
10418-AAA	IEEE 802.11g WiFi 2.4 GHz (DSSS-OFDM, 6 Mbps, 99pc duty cycle, Long preamble)	X	9.89	68.0	20.9	8.14	118.8	±2.2 %
		Y	9.59	67.5	20.4		110.3	
		Z	9.85	68.8	21.4		131.4	
10419-AAA	IEEE 802.11g WiFi 2.4 GHz (DSSS-OFDM, 6 Mbps, 99pc duty cycle, Short preamble)	X	9.78	68.1	20.9	8.19	117.3	±2.2 %
		Y	9.70	67.6	20.5		111.1	
		Z	10.04	68.9	21.5		132.4	
10422-AAA	IEEE 802.11n (HT Greenfield, 7.2 Mbps, BPSK)	X	10.03	68.4	21.1	8.32	119.6	±2.5 %
		Y	9.90	67.7	20.6		112.6	
		Z	10.29	69.2	21.7		133.6	
10423-AAA	IEEE 802.11n (HT Greenfield, 43.3 Mbps, 16-QAM)	X	10.19	68.5	21.3	8.47	120.0	±2.5 %
		Y	10.08	68.0	20.8		112.9	
		Z	10.43	69.3	21.8		134.2	
10424-AAA	IEEE 802.11n (HT Greenfield, 72.2 Mbps, 64-QAM)	X	10.08	68.4	21.2	8.40	119.6	±2.5 %
		Y	9.96	67.8	20.7		112.6	
		Z	10.33	69.2	21.8		133.7	
10425-AAA	IEEE 802.11n (HT Greenfield, 15 Mbps, BPSK)	X	10.62	68.9	21.4	8.41	126.1	±2.7 %
		Y	10.42	68.2	20.8		117.7	
		Z	10.92	69.6	22.0		142.2	
10426-AAA	IEEE 802.11n (HT Greenfield, 90 Mbps, 16-QAM)	X	10.68	69.0	21.5	8.45	126.5	±2.7 %
		Y	10.43	68.2	20.8		118.2	
		Z	10.95	69.8	22.0		142.5	
10427-AAA	IEEE 802.11n (HT Greenfield, 150 Mbps, 64-QAM)	X	10.65	69.0	21.4	8.41	126.9	±2.7 %
		Y	10.40	68.2	20.8		118.2	
		Z	10.92	69.8	22.0		142.7	
10434-AAA	W-CDMA (BS Test Model 1, 64 DPCH)	X	9.04	67.7	21.1	8.60	103.3	±2.7 %
		Y	8.68	69.3	21.7		143.5	
		Z	8.37	68.8	21.8		116.7	

The reported uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor $k=2$, which for a normal distribution corresponds to a coverage probability of approximately 95%.

* The uncertainties of Norm(X, Y, Z) do not affect the E²-field uncertainty inside TSI. (see Pages 12 and 16).

** Numerical linearization parameter: uncertainty not required.

† Uncertainty is determined using the max. deviation from linear response applying rectangular distribution and is expressed for the square of the field value.

EX3DV4- SN:7364

June 23, 2015

DASY/EASY - Parameters of Probe: EX3DV4 - SN:7364

Calibration Parameter Determined in Head Tissue Simulating Media

f (MHz) ^c	Relative Permittivity ^e	Conductivity (S/m) ^f	ConvF X	ConvF Y	ConvF Z	Alpha ^g	Depth ^h (mm)	Unct. (k=2)
150	52.3	0.76	12.95	12.95	12.95	0.00	1.00	± 13.3 %
300	45.3	0.87	11.95	11.95	11.95	0.10	1.10	± 13.3 %
450	43.5	0.87	10.72	10.72	10.72	0.15	1.10	± 13.3 %
750	41.9	0.89	10.01	10.01	10.01	0.29	1.08	± 12.0 %
900	41.5	0.97	9.26	9.26	9.26	0.24	1.23	± 12.0 %
1810	40.0	1.40	7.93	7.93	7.93	0.33	0.80	± 12.0 %
1900	40.0	1.40	7.93	7.93	7.93	0.35	0.80	± 12.0 %
2450	39.2	1.80	7.18	7.18	7.18	0.27	0.98	± 12.0 %
2600	39.0	1.96	6.93	6.93	6.93	0.34	0.93	± 12.0 %
5200	36.0	4.66	5.22	5.22	5.22	0.35	1.80	± 13.1 %
5300	35.9	4.76	5.00	5.00	5.00	0.35	1.80	± 13.1 %
5500	35.6	4.96	4.75	4.75	4.75	0.40	1.80	± 13.1 %
5600	35.5	5.07	4.64	4.64	4.64	0.40	1.80	± 13.1 %
5800	35.3	5.27	4.52	4.52	4.52	0.40	1.80	± 13.1 %

^c Frequency validity above 300 MHz of ± 100 MHz only applies for DASY with and higher (see Page 2), else it is restricted to ± 50 MHz. The uncertainty is the RSS of the ConvF uncertainty at calibration frequency and the uncertainty for the indicated frequency band. Frequency validity below 300 MHz is ± 10, 25, 40, 50 and 70 MHz for ConvF assessments at 30, 64, 128, 150 and 220 MHz respectively. Above 5 GHz frequency validity can be extended to ± 110 MHz.

^e At frequencies below 3 GHz, the validity of tissue parameters (ε and σ) can be relaxed to ± 10% if equal compensation formula is applied to measured SAR values. At frequencies above 3 GHz, the validity of tissue parameters (ε and σ) is restricted to ± 5%. The uncertainty is the RSS of the ConvF uncertainty for indicated target tissue parameters.

^g Alpha/Depth are determined during calibration. SPEAG warrants that the remaining deviation due to the boundary effect after compensation is always less than ± 1% for frequencies below 3 GHz and below ± 2% for frequencies between 3-5 GHz at any distance larger than half the probe diameter from the boundary.

EX3DV4 - SN 7364

June 23, 2015

DASY/EASY - Parameters of Probe: EX3DV4 - SN:7364

Calibration Parameter Determined in Body Tissue Simulating Media

f (MHz) ^c	Relative Permittivity ^e	Conductivity (S/m) ^f	ConvF X	ConvF Y	ConvF Z	Alpha ^g	Depth ^h (mm)	Unct. (k=2)
150	61.9	0.80	12.28	12.28	12.28	0.00	1.00	± 13.3 %
300	58.2	0.92	11.24	11.24	11.24	0.08	1.10	± 13.3 %
450	56.7	0.94	11.02	11.02	11.02	0.08	1.10	± 13.3 %
750	55.5	0.96	9.42	9.42	9.42	0.27	1.06	± 12.0 %
900	55.0	1.05	9.20	9.20	9.20	0.27	1.22	± 12.0 %
1810	53.3	1.52	7.75	7.75	7.75	0.43	0.85	± 12.0 %
1900	53.3	1.52	7.57	7.57	7.57	0.47	0.80	± 12.0 %
2450	52.7	1.95	7.33	7.33	7.33	0.35	0.90	± 12.0 %
2600	52.5	2.16	7.17	7.17	7.17	0.31	0.95	± 12.0 %
5200	49.0	5.30	4.52	4.52	4.52	0.45	1.80	± 13.1 %
5300	48.9	5.42	4.29	4.29	4.29	0.45	1.80	± 13.1 %
5500	48.6	5.65	3.92	3.92	3.92	0.50	1.90	± 13.1 %
5600	48.5	5.77	3.74	3.74	3.74	0.50	1.80	± 13.1 %
5800	48.2	6.00	4.06	4.06	4.06	0.50	1.80	± 13.1 %

^c Frequency validity above 300 MHz of ± 100 MHz only applies for DASY v4.4 and higher (see Page 2); else it is restricted to ± 50 MHz. The uncertainty is the RSS of the ConvF uncertainty at calibration frequency and the uncertainty for the indicated frequency band. Frequency validity below 300 MHz is ± 10, 25, 40, 50 and 70 MHz for ConvF assessments at 30, 64, 138, 150 and 220 MHz respectively. Above 5 GHz frequency validity can be extended to ± 110 MHz.


^e At frequencies below 3 GHz, the validity of tissue parameters (ε and σ) can be related to ± 10% if liquid compensation formula is applied to measured SAR values. At frequencies above 3 GHz, the validity of tissue parameters (ε and σ) is restricted to ± 5%. The uncertainty is the RSS of the ConvF uncertainty for indicated target tissue parameters.

^g Alpha/Depth are determined during calibration. SPEAG warrants that the remaining deviation due to the boundary effect after compensation is always less than ± 1% for frequencies below 3 GHz and below ± 2% for frequencies between 3-6 GHz at any distance larger than half the (probe) diameter from the boundary.

EX3DV4- SN:7364

June 23, 2015

Frequency Response of E-Field (TEM-Cell: IF110 EXX, Waveguide: R22)

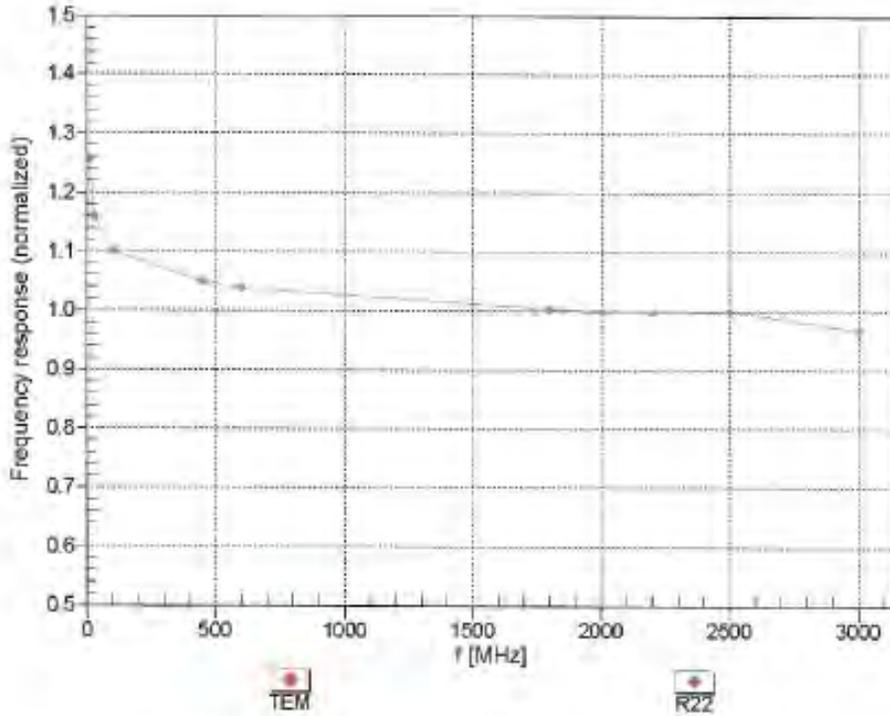

Uncertainty of Frequency Response of E-field: $\pm 6.3\%$ (k=2)



EX3DV4-SN:7364

June 23, 2015

Receiving Pattern (ϕ), $\theta = 0^\circ$

f=600 MHz,TEM

f=1800 MHz,R22

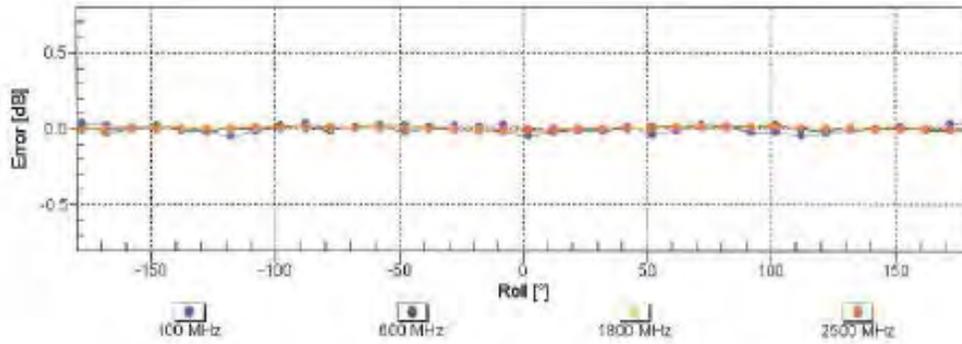
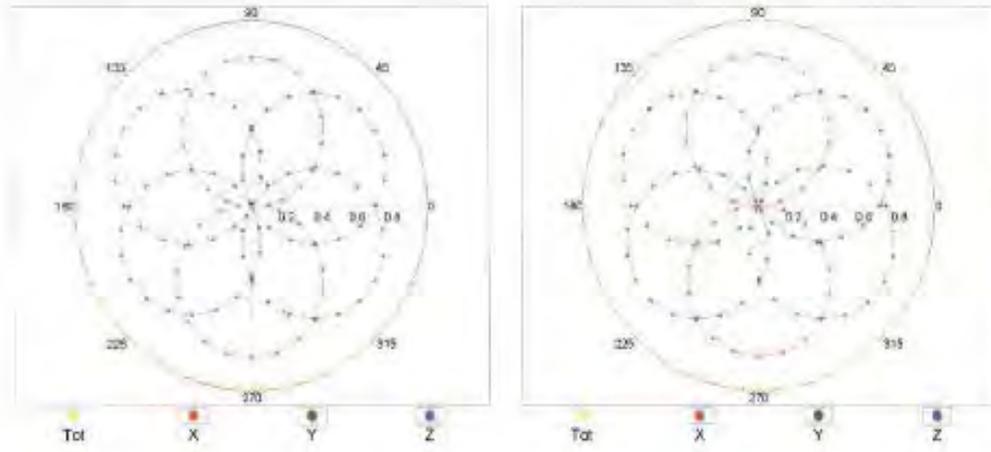


Uncertainty of Axial Isotropy Assessment: $\pm 0.5\%$ (k=2)

EX3DV4- SN:7364

June 23, 2015

Dynamic Range f(SAR_{head}) (TEM cell , f_{eval}= 1900 MHz)

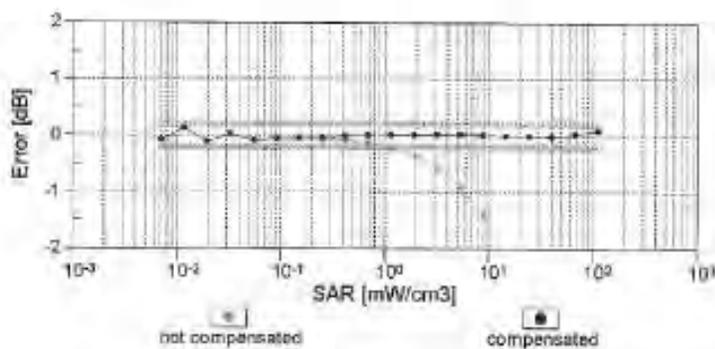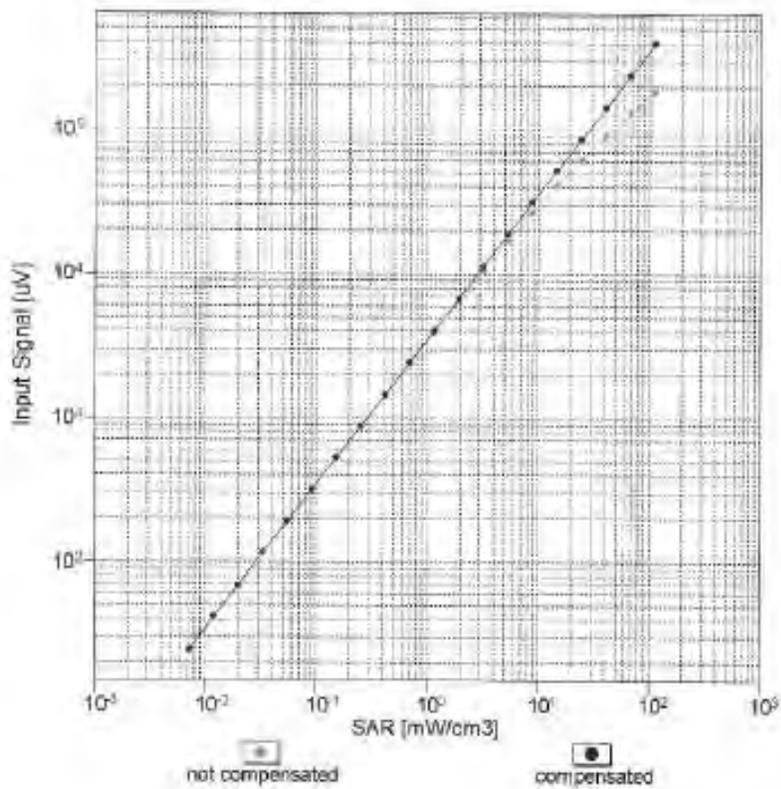


Uncertainty of Linearity Assessment: ± 0.6% (k=2)


EX3DV4- SN-7364

June 23, 2015

Conversion Factor Assessment

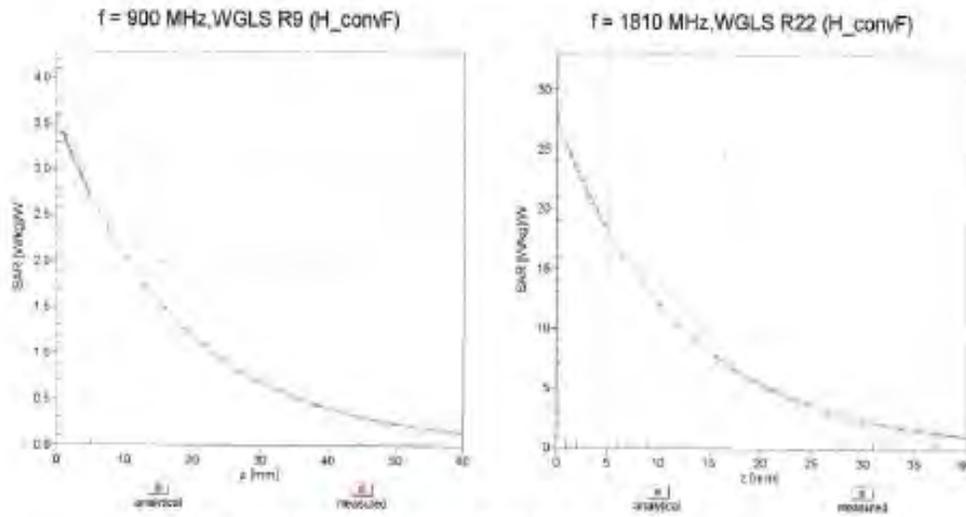

Deviation from Isotropy in Liquid Error (ϕ, θ), f = 900 MHz

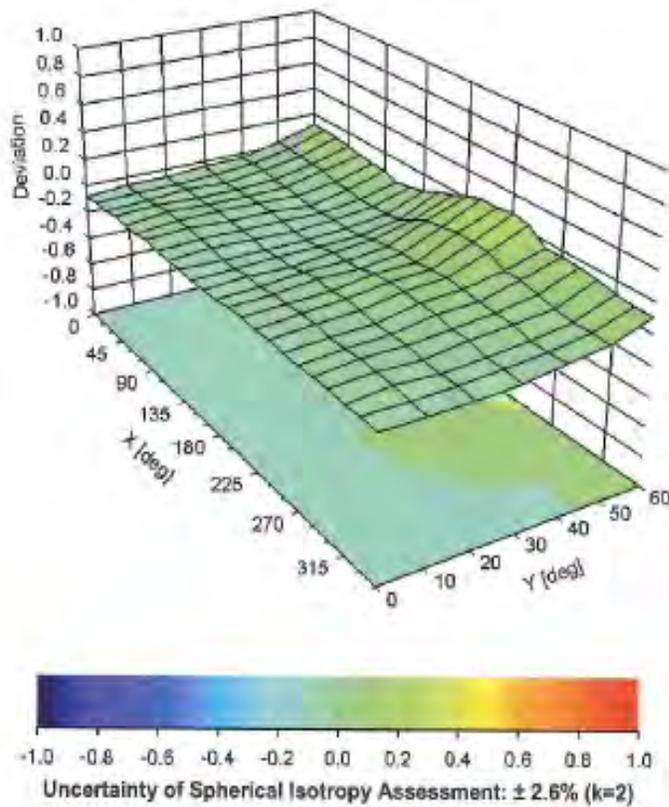

EX3DV4-SN:7364

June 23, 2015

DASY/EASY - Parameters of Probe: EX3DV4 - SN:7364

Other Probe Parameters

Sensor Arrangement	Triangular
Connector Angle (°)	132.1
Mechanical Surface Detection Mode	enabled
Optical Surface Detection Mode	disabled
Probe Overall Length	337 mm
Probe Body Diameter	10 mm
Tip Length	9 mm
Tip Diameter	2.5 mm
Probe Tip to Sensor X Calibration Point	1 mm
Probe Tip to Sensor Y Calibration Point	1 mm
Probe Tip to Sensor Z Calibration Point	1 mm
Recommended Measurement Distance from Surface	1.4 mm

**Calibration Laboratory of
Schmid & Partner
Engineering AG**
Zeughausstrasse 43, 8004 Zurich, Switzerland



S Schweizerischer Kalibrierdienst
C Service suisse d'étalonnage
S Servizio svizzero di taratura
S Swiss Calibration Service

Accredited by the Swiss Accreditation Service (SAS)
The Swiss Accreditation Service is one of the signatories to the EA
Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: **SCS 0108**

Client **Motorola Solutions MY**

Certificate No: **ES3-3196_Nov15**

CALIBRATION CERTIFICATE

Object **ES3DV3 - SN:3196**

Calibration procedure(s) **QA CAL-01.v9, QA CAL-12.v9, QA CAL-23.v5, QA CAL-25.v6
Calibration procedure for dosimetric E-field probes**

Calibration date: **November 17, 2015**

This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI).
The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility: environment temperature (22 ± 3)°C and humidity < 70%.

Calibration Equipment used (M&TE critical for calibration)

Primary Standards	ID	Cal Date (Certificate No.)	Scheduled Calibration
Power meter E4419B	GB41293874	01-Apr-15 (No. 217-02128)	Mar-16
Power sensor E4412A	MY41498087	01-Apr-15 (No. 217-02128)	Mar-16
Reference 3 dB Attenuator	SN: S5054 (3c)	01-Apr-15 (No. 217-02129)	Mar-16
Reference 20 dB Attenuator	SN: S5277 (20x)	01-Apr-15 (No. 217-02132)	Mar-16
Reference 30 dB Attenuator	SN: S5129 (30b)	01-Apr-15 (No. 217-02133)	Mar-16
Reference Probe ES3DV2	SN: 3013	30-Dec-14 (No. ES3-3013_Dec14)	Dec-15
DAE4	SN: 660	14-Jan-15 (No. DAE4-660_Jan15)	Jan-16
Secondary Standards	ID	Check Date (in house)	Scheduled Check
RF generator HP 8648C	US3642U01700	4-Aug-99 (in house check Apr-13)	In house check: Apr-16
Network Analyzer HP 8753E	US37390585	18-Oct-01 (in house check Oct-15)	In house check: Oct-16

Calibrated by:	Name Claudio Leubler	Function Laboratory Technician	Signature
Approved by:	Name Katja Pokovic	Function Technical Manager	

Issued: November 17, 2015

This calibration certificate shall not be reproduced except in full without written approval of the laboratory.

Calibration Laboratory of
Schmid & Partner
 Engineering AG
 Zeughausstrasse 43, 8004 Zurich, Switzerland



S Schweizerischer Kalibrierdienst
C Service suisse d'étalonnage
S Servizio svizzero di taratura
S Swiss Calibration Service

Accredited by the Swiss Accreditation Service (SAS)

The Swiss Accreditation Service is one of the signatories to the EA
 Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: **SCS 0108**

Glossary:

TSL	tissue simulating liquid
NORM _{x,y,z}	sensitivity in free space
ConvF	sensitivity in TSL / NORM _{x,y,z}
DCP	diode compression point
CF	crest factor (1/duty_cycle) of the RF signal
A, B, C, D	modulation dependent linearization parameters
Polarization φ	φ rotation around probe axis
Polarization ϑ	ϑ rotation around an axis that is in the plane normal to probe axis (at measurement center), i.e., $\vartheta = 0$ is normal to probe axis
Connector Angle	information used in DASY system to align probe sensor X to the robot coordinate system

Calibration is Performed According to the Following Standards:

- IEEE Std 1528-2013, "IEEE Recommended Practice for Determining the Peak Spatial-Averaged Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques", June 2013
- IEC 62209-1, "Procedure to measure the Specific Absorption Rate (SAR) for hand-held devices used in close proximity to the ear (frequency range of 300 MHz to 3 GHz)", February 2005
- IEC 62209-2, "Procedure to determine the Specific Absorption Rate (SAR) for wireless communication devices used in close proximity to the human body (frequency range of 30 MHz to 6 GHz)", March 2010
- KDB 865664, "SAR Measurement Requirements for 100 MHz to 6 GHz"

Methods Applied and Interpretation of Parameters:

- NORM_{x,y,z}**: Assessed for E-field polarization $\vartheta = 0$ ($f \leq 900$ MHz in TEM-cell; $f > 1800$ MHz: R22 waveguide). NORM_{x,y,z} are only intermediate values, i.e., the uncertainties of NORM_{x,y,z} does not affect the E²-field uncertainty inside TSL (see below ConvF).
- NORM(f)_{x,y,z} = NORM_{x,y,z} * frequency_response** (see Frequency Response Chart). This linearization is implemented in DASY4 software versions later than 4.2. The uncertainty of the frequency response is included in the stated uncertainty of ConvF.
- DCP_{x,y,z}**: DCP are numerical linearization parameters assessed based on the data of power sweep with CW signal (no uncertainty required). DCP does not depend on frequency nor media.
- PAR**: PAR is the Peak to Average Ratio that is not calibrated but determined based on the signal characteristics
- A_{x,y,z}; B_{x,y,z}; C_{x,y,z}; D_{x,y,z}; VR_{x,y,z}**: A, B, C, D are numerical linearization parameters assessed based on the data of power sweep for specific modulation signal. The parameters do not depend on frequency nor media. VR is the maximum calibration range expressed in RMS voltage across the diode.
- ConvF and Boundary Effect Parameters**: Assessed in flat phantom using E-field (or Temperature Transfer Standard for $f \leq 800$ MHz) and inside waveguide using analytical field distributions based on power measurements for $f > 800$ MHz. The same setups are used for assessment of the parameters applied for boundary compensation (alpha, depth) of which typical uncertainty values are given. These parameters are used in DASY4 software to improve probe accuracy close to the boundary. The sensitivity in TSL corresponds to NORM_{x,y,z} * ConvF whereby the uncertainty corresponds to that given for ConvF. A frequency dependent ConvF is used in DASY version 4.4 and higher which allows extending the validity from ± 50 MHz to ± 100 MHz.
- Spherical isotropy (3D deviation from isotropy)**: in a field of low gradients realized using a flat phantom exposed by a patch antenna.
- Sensor Offset**: The sensor offset corresponds to the offset of virtual measurement center from the probe tip (on probe axis). No tolerance required.
- Connector Angle**: The angle is assessed using the information gained by determining the NORM_x (no uncertainty required).

ES3DV3 – SN:3196

November 17, 2015

Probe ES3DV3

SN:3196

Manufactured: June 16, 2008
Calibrated: November 17, 2015

Calibrated for DASY/EASY Systems
(Note: non-compatible with DASY2 system!)

ES3DV3- SN:3196

November 17, 2015

DASY/EASY - Parameters of Probe: ES3DV3 - SN:3196

Basic Calibration Parameters

	Sensor X	Sensor Y	Sensor Z	Unc (k=2)
Norm ($\mu V/(V/m)^2$) ^A	1.27	1.29	1.33	$\pm 10.1\%$
DCP (mV) ^B	104.9	104.0	102.6	

Modulation Calibration Parameters

UID	Communication System Name		A dB	B dB $\sqrt{\mu V}$	C	D dB	VR mV	Unc ^E (k=2)
0	CW	X	0.0	0.0	1.0	0.00	213.4	$\pm 3.3\%$
		Y	0.0	0.0	1.0		214.3	
		Z	0.0	0.0	1.0		218.9	
10012-CAB	IEEE 802.11b WiFi 2.4 GHz (DSSS, 1 Mbps)	X	2.95	69.6	19.1	1.87	148.8	$\pm 0.7\%$
		Y	3.00	69.4	18.9		147.7	
		Z	2.76	68.0	18.4		132.0	
10013-CAB	IEEE 802.11g WiFi 2.4 GHz (DSSS-OFDM, 6 Mbps)	X	11.06	71.2	23.8	9.46	143.4	$\pm 3.3\%$
		Y	10.98	70.6	23.3		145.2	
		Z	10.86	70.5	23.4		124.5	
10059-CAB	IEEE 802.11b WiFi 2.4 GHz (DSSS, 2 Mbps)	X	3.25	70.7	19.7	2.12	147.8	$\pm 0.7\%$
		Y	3.55	72.1	20.2		147.4	
		Z	3.08	69.5	19.2		131.0	
10071-CAB	IEEE 802.11g WiFi 2.4 GHz (DSSS/OFDM, 9 Mbps)	X	11.24	71.6	24.3	9.83	140.4	$\pm 2.7\%$
		Y	11.13	70.9	23.7		141.2	
		Z	11.61	72.5	24.9		149.5	
10114-CAB	IEEE 802.11n (HT Greenfield, 13.5 Mbps, BPSK)	X	10.05	68.9	21.4	8.10	127.0	$\pm 2.2\%$
		Y	9.87	68.3	21.0		126.0	
		Z	10.23	69.4	21.7		134.0	
10117-CAB	IEEE 802.11n (HT Mixed, 13.5 Mbps, BPSK)	X	10.01	68.8	21.3	8.07	127.5	$\pm 2.2\%$
		Y	9.87	68.3	20.9		127.2	
		Z	10.21	69.3	21.7		134.9	
10193-CAB	IEEE 802.11n (HT Greenfield, 6.5 Mbps, BPSK)	X	10.02	69.6	21.9	8.09	147.9	$\pm 2.5\%$
		Y	9.96	69.2	21.5		149.5	
		Z	9.84	69.0	21.6		129.1	
10196-CAB	IEEE 802.11n (HT Mixed, 6.5 Mbps, BPSK)	X	10.00	69.6	21.9	8.10	147.4	$\pm 2.2\%$
		Y	9.92	69.1	21.5		147.7	
		Z	9.82	69.0	21.6		128.8	
10219-CAB	IEEE 802.11n (HT Mixed, 7.2 Mbps, BPSK)	X	9.88	69.5	21.8	8.03	146.9	$\pm 2.5\%$
		Y	9.78	68.9	21.4		146.3	
		Z	9.73	69.0	21.6		127.8	
10222-CAB	IEEE 802.11n (HT Mixed, 15 Mbps, BPSK)	X	10.00	68.8	21.3	8.06	127.3	$\pm 2.2\%$
		Y	9.80	68.2	20.9		126.3	
		Z	10.17	69.2	21.6		134.7	

ES3DV3- SN:3196

November 17, 2015

10422-AAA	IEEE 802.11n (HT Greenfield, 7.2 Mbps, BPSK)	X	10.28	69.9	22.2	8.32	149.2	±2.5 %
		Y	10.19	69.4	21.8		149.0	
		Z	10.09	69.3	21.9		129.5	
10425-AAA	IEEE 802.11n (HT Greenfield, 15 Mbps, BPSK)	X	10.45	69.3	21.8	8.41	129.4	±2.5 %
		Y	10.27	68.7	21.3		128.2	
		Z	10.65	69.8	22.1		135.7	

The reported uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor $k=2$, which for a normal distribution corresponds to a coverage probability of approximately 95%.

^A The uncertainties of Norm X,Y,Z do not affect the E^2 -field uncertainty inside TSL (see Pages 6 and 7).
^B Numerical linearization parameter: uncertainty not required.
^E Uncertainty is determined using the max. deviation from linear response applying rectangular distribution and is expressed for the square of the field value.

ES3DV3- SN:3196

November 17, 2015

DASY/EASY - Parameters of Probe: ES3DV3 - SN:3196

Calibration Parameter Determined in Head Tissue Simulating Media

f (MHz) ^C	Relative Permittivity ^F	Conductivity (S/m) ^F	ConvF X	ConvF Y	ConvF Z	Alpha ^G	Depth ^G (mm)	Unc (k=2)
150	52.3	0.76	7.31	7.31	7.31	0.06	1.25	± 13.3 %
300	45.3	0.87	7.34	7.34	7.34	0.14	1.60	± 13.3 %
450	43.5	0.87	6.83	6.83	6.83	0.22	1.80	± 13.3 %
750	41.9	0.89	6.46	6.46	6.46	0.40	1.64	± 12.0 %
900	41.5	0.97	6.13	6.13	6.13	0.56	1.38	± 12.0 %
2450	39.2	1.80	4.54	4.54	4.54	0.68	1.36	± 12.0 %

^C Frequency validity above 300 MHz of ± 100 MHz only applies for DASY v4.4 and higher (see Page 2), else it is restricted to ± 50 MHz. The uncertainty is the RSS of the ConvF uncertainty at calibration frequency and the uncertainty for the indicated frequency band. Frequency validity below 300 MHz is ± 10, 25, 40, 50 and 70 MHz for ConvF assessments at 30, 64, 128, 150 and 220 MHz respectively. Above 5 GHz frequency validity can be extended to ± 110 MHz.

^F At frequencies below 3 GHz, the validity of tissue parameters (ϵ and σ) can be relaxed to ± 10% if liquid compensation formula is applied to measured SAR values. At frequencies above 3 GHz, the validity of tissue parameters (ϵ and σ) is restricted to ± 5%. The uncertainty is the RSS of the ConvF uncertainty for indicated target tissue parameters.

^G Alpha/Depth are determined during calibration. SPEAG warrants that the remaining deviation due to the boundary effect after compensation is always less than ± 1% for frequencies below 3 GHz and below ± 2% for frequencies between 3-6 GHz at any distance larger than half the probe tip diameter from the boundary.

ES3DV3- SN:3196

November 17, 2015

DASY/EASY - Parameters of Probe: ES3DV3 - SN:3196

Calibration Parameter Determined in Body Tissue Simulating Media

f (MHz) ^C	Relative Permittivity ^F	Conductivity (S/m) ^F	ConvF X	ConvF Y	ConvF Z	Alpha ^G	Depth (mm) ^G	Unc (k=2)
150	61.9	0.80	6.94	6.94	6.94	0.06	1.25	± 13.3 %
300	58.2	0.92	6.94	6.94	6.94	0.10	1.60	± 13.3 %
450	56.7	0.94	7.06	7.06	7.06	0.13	1.60	± 13.3 %
750	55.5	0.96	6.36	6.36	6.36	0.42	1.59	± 12.0 %
900	55.0	1.05	6.10	6.10	6.10	0.39	1.80	± 12.0 %
2450	52.7	1.95	4.43	4.43	4.43	0.71	1.28	± 12.0 %

^C Frequency validity above 300 MHz of ± 100 MHz only applies for DASY v4.4 and higher (see Page 2), else it is restricted to ± 50 MHz. The uncertainty is the RSS of the ConvF uncertainty at calibration frequency and the uncertainty for the indicated frequency band. Frequency validity below 300 MHz is ± 10, 25, 40, 50 and 70 MHz for ConvF assessments at 30, 64, 128, 150 and 220 MHz respectively. Above 5 GHz frequency validity can be extended to ± 110 MHz.


^F At frequencies below 3 GHz, the validity of tissue parameters (ϵ and σ) can be relaxed to ± 10% if liquid compensation formula is applied to measured SAR values. At frequencies above 3 GHz, the validity of tissue parameters (ϵ and σ) is restricted to ± 5%. The uncertainty is the RSS of the ConvF uncertainty for indicated target tissue parameters.

^G Alpha/Depth are determined during calibration. SPEAG warrants that the remaining deviation due to the boundary effect after compensation is always less than ± 1% for frequencies below 3 GHz and below ± 2% for frequencies between 3-6 GHz at any distance larger than half the probe tip diameter from the boundary.

ES3DV3- SN:3196

November 17, 2015

Frequency Response of E-Field (TEM-Cell:ifi110 EXX, Waveguide: R22)


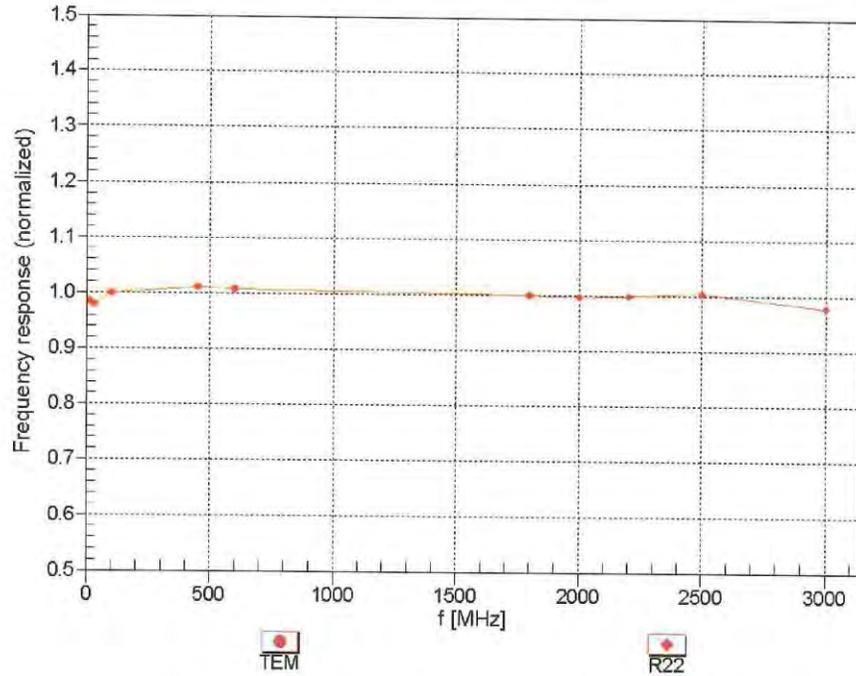


Uncertainty of Frequency Response of E-field: $\pm 6.3\%$ (k=2)

ES3DV3- SN:3196

November 17, 2015

Receiving Pattern (ϕ), $\theta = 0^\circ$

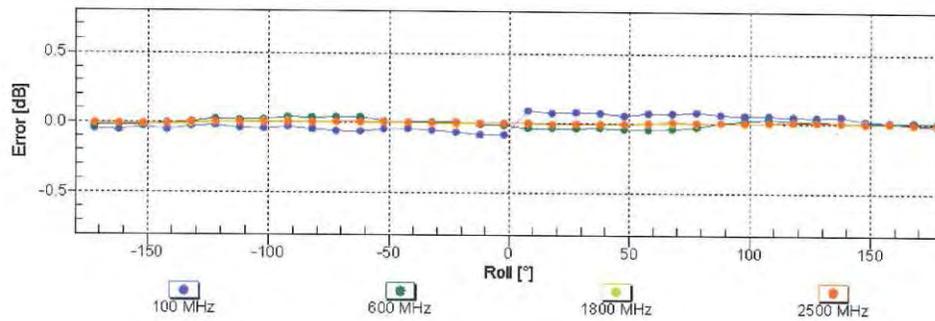
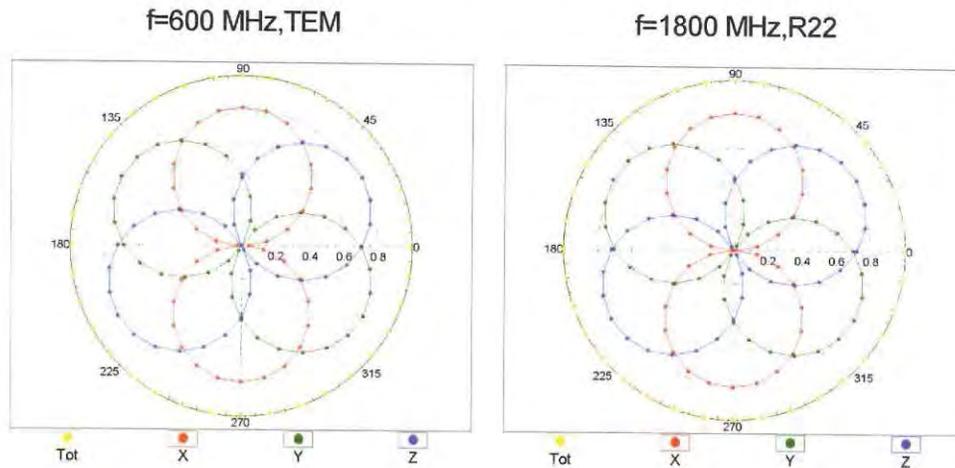


Uncertainty of Axial Isotropy Assessment: $\pm 0.5\%$ ($k=2$)

ES3DV3- SN:3196

November 17, 2015

Dynamic Range $f(SAR_{head})$ (TEM cell, $f_{eval} = 1900$ MHz)

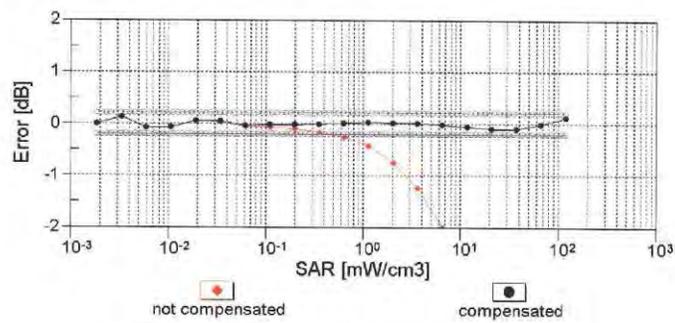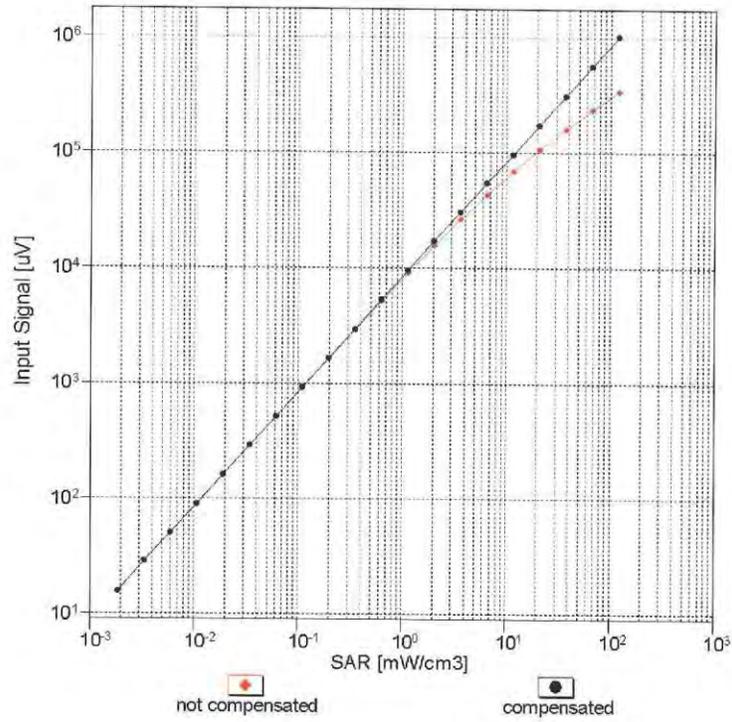


Uncertainty of Linearity Assessment: $\pm 0.6\%$ (k=2)


ES3DV3- SN:3196

November 17, 2015

Conversion Factor Assessment

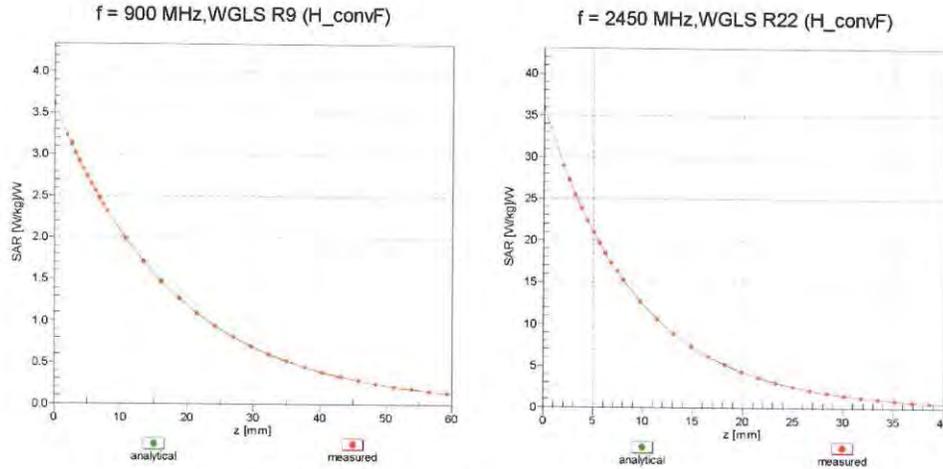

Deviation from Isotropy in Liquid Error (ϕ, θ), f = 900 MHz

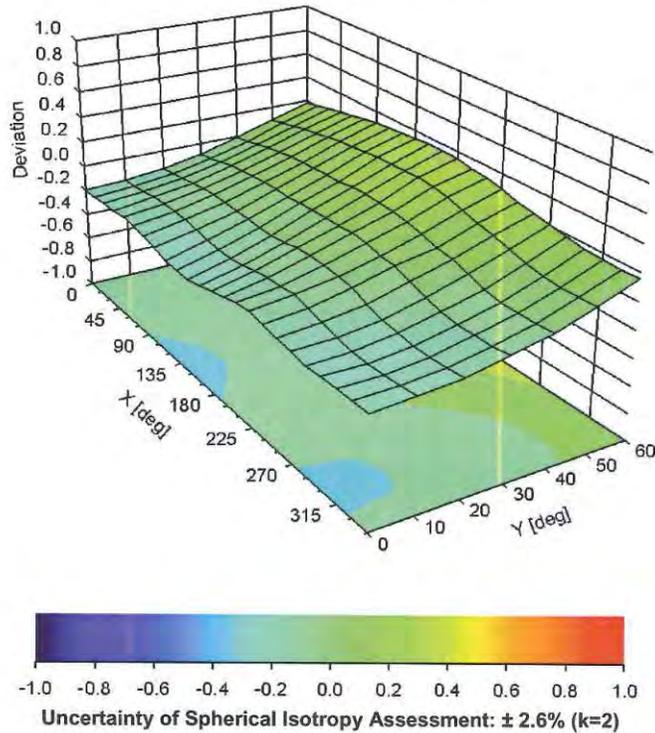

ES3DV3- SN:3196

November 17, 2015

DASY/EASY - Parameters of Probe: ES3DV3 - SN:3196

Other Probe Parameters

Sensor Arrangement	Triangular
Connector Angle (°)	7.9
Mechanical Surface Detection Mode	enabled
Optical Surface Detection Mode	disabled
Probe Overall Length	337 mm
Probe Body Diameter	10 mm
Tip Length	10 mm
Tip Diameter	4 mm
Probe Tip to Sensor X Calibration Point	2 mm
Probe Tip to Sensor Y Calibration Point	2 mm
Probe Tip to Sensor Z Calibration Point	2 mm
Recommended Measurement Distance from Surface	3 mm

**Calibration Laboratory of
Schmid & Partner
Engineering AG**
Zeughausstrasse 43, 8004 Zurich, Switzerland



S Schweizerischer Kalibrierdienst
C Service suisse d'étalonnage
S Servizio svizzero di taratura
S Swiss Calibration Service

Accredited by the Swiss Accreditation Service (SAS)
The Swiss Accreditation Service is one of the signatories to the EA
Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: **SCS 0108**

Client **Motorola EME**

Certificate No: **EX3-3735_Jul15**

CALIBRATION CERTIFICATE

Object **EX3DV4 - SN:3735**

Calibration procedure(s) **QA CAL-01.v9, QA CAL-12.v9, QA CAL-14.v4, QA CAL-23.v5,
QA CAL-25.v6
Calibration procedure for dosimetric E-field probes**

Calibration date: **July 16, 2015**

This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI).
The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility: environment temperature (22 ± 3)°C and humidity < 70%.

Calibration Equipment used (M&TE critical for calibration)

Primary Standards	ID	Cal Date (Certificate No.)	Scheduled Calibration
Power meter E4419B	GB41293874	01-Apr-15 (No. 217-02128)	Mar-16
Power sensor E4412A	MY41498087	01-Apr-15 (No. 217-02128)	Mar-16
Reference 3 dB Attenuator	SN: S5054 (3c)	01-Apr-15 (No. 217-02129)	Mar-16
Reference 20 dB Attenuator	SN: S5277 (20x)	01-Apr-15 (No. 217-02132)	Mar-16
Reference 30 dB Attenuator	SN: S5129 (30b)	01-Apr-15 (No. 217-02133)	Mar-16
Reference Probe ES3DV2	SN: 3013	30-Dec-14 (No. ES3-3013_Dec14)	Dec-15
DAE4	SN: 660	14-Jan-15 (No. DAE4-660_Jan15)	Jan-16
Secondary Standards	ID	Check Date (in house)	Scheduled Check
RF generator HP 8648C	US3642U01700	4-Aug-99 (in house check Apr-13)	In house check: Apr-16
Network Analyzer HP 8753E	US37390585	18-Oct-01 (in house check Oct-14)	In house check: Oct-15

Calibrated by:	Name Claudio Leubler	Function Laboratory Technician	Signature
Approved by:	Name Katja Pokovic	Function Technical Manager	Signature

Issued: July 18, 2015

This calibration certificate shall not be reproduced except in full without written approval of the laboratory.

Validation Laboratory of
 Schmid & Partner
 Engineering AG
 Zeughausstrasse 43, 8004 Zurich, Switzerland



S Schweizerischer Kalibrierdienst
 C Service suisse d'étalonnage
 S Servizio svizzero di taratura
 S Swiss Calibration Service

Accredited by the Swiss Accreditation Service (SAS)

Accreditation No.: SCS 0108

The Swiss Accreditation Service is one of the signatories to the EA
 Multilateral Agreement for the recognition of calibration certificates

Glossary:

TSL	tissue simulating liquid
NORM _{x,y,z}	sensitivity in free space
ConvF	sensitivity in TSL / NORM _{x,y,z}
DCP	diode compression point
CF	crest factor (1/duty_cycle) of the RF signal
A, B, C, D	modulation dependent linearization parameters
Polarization φ	φ rotation around probe axis
Polarization θ	θ rotation around an axis that is in the plane normal to probe axis (at measurement center), i.e., $\theta = 0$ is normal to probe axis
Connector Angle	information used in DASY system to align probe sensor X to the robot coordinate system

Calibration is Performed According to the Following Standards:

- a) IEEE Std 1528-2013, "IEEE Recommended Practice for Determining the Peak Spatial-Averaged Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques", June 2013
- b) IEC 62209-1, "Procedure to measure the Specific Absorption Rate (SAR) for hand-held devices used in close proximity to the ear (frequency range of 300 MHz to 3 GHz)", February 2005
- c) IEC 62209-2, "Procedure to determine the Specific Absorption Rate (SAR) for wireless communication devices used in close proximity to the human body (frequency range of 30 MHz to 6 GHz)", March 2010
- d) KDB 865664, "SAR Measurement Requirements for 100 MHz to 6 GHz"

Methods Applied and Interpretation of Parameters:

- **NORM_{x,y,z}:** Assessed for E-field polarization $\theta = 0$ ($f \leq 900$ MHz in TEM-cell; $f > 1800$ MHz: R22 waveguide). NORM_{x,y,z} are only intermediate values, i.e., the uncertainties of NORM_{x,y,z} does not affect the E²-field uncertainty inside TSL (see below ConvF).
- **NORM(f)_{x,y,z} = NORM_{x,y,z} * frequency_response** (see Frequency Response Chart). This linearization is implemented in DASY4 software versions later than 4.2. The uncertainty of the frequency response is included in the stated uncertainty of ConvF.
- **DCP_{x,y,z}:** DCP are numerical linearization parameters assessed based on the data of power sweep with CW signal (no uncertainty required). DCP does not depend on frequency nor media.
- **PAR:** PAR is the Peak to Average Ratio that is not calibrated but determined based on the signal characteristics
- **A_{x,y,z}; B_{x,y,z}; C_{x,y,z}; D_{x,y,z}; VR_{x,y,z}:** A, B, C, D are numerical linearization parameters assessed based on the data of power sweep for specific modulation signal. The parameters do not depend on frequency nor media. VR is the maximum calibration range expressed in RMS voltage across the diode.
- **ConvF and Boundary Effect Parameters:** Assessed in flat phantom using E-field (or Temperature Transfer Standard for $f \leq 800$ MHz) and inside waveguide using analytical field distributions based on power measurements for $f > 800$ MHz. The same setups are used for assessment of the parameters applied for boundary compensation (alpha, depth) of which typical uncertainty values are given. These parameters are used in DASY4 software to improve probe accuracy close to the boundary. The sensitivity in TSL corresponds to NORM_{x,y,z} * ConvF whereby the uncertainty corresponds to that given for ConvF. A frequency dependent ConvF is used in DASY version 4.4 and higher which allows extending the validity from ± 50 MHz to ± 100 MHz.
- **Spherical isotropy (3D deviation from isotropy):** in a field of low gradients realized using a flat phantom exposed by a patch antenna.
- **Sensor Offset:** The sensor offset corresponds to the offset of virtual measurement center from the probe tip (on probe axis). No tolerance required.
- **Connector Angle:** The angle is assessed using the information gained by determining the NORM_x (no uncertainty required).

EX3DV4 – SN:3735

July 16, 2015

Probe EX3DV4

SN:3735

Manufactured: February 15, 2010
Calibrated: July 16, 2015

Calibrated for DASY/EASY Systems
(Note: non-compatible with DASY2 system!)

EX3DV4- SN:3735

July 16, 2015

DASY/EASY - Parameters of Probe: EX3DV4 - SN:3735

Basic Calibration Parameters

	Sensor X	Sensor Y	Sensor Z	Unc (k=2)
Norm ($\mu\text{V}/(\text{V}/\text{m})^2$) ^A	0.38	0.40	0.47	$\pm 10.1\%$
DCP (mV) ^B	111.5	99.9	102.9	

Modulation Calibration Parameters

UID	Communication System Name		A dB	B dB $\sqrt{\mu\text{V}}$	C	D dB	VR mV	Unc ^E (k=2)
0	CW	X	0.0	0.0	1.0	0.00	188.7	$\pm 2.5\%$
		Y	0.0	0.0	1.0		193.7	
		Z	0.0	0.0	1.0		146.8	
10012-CAB	IEEE 802.11b WiFi 2.4 GHz (DSSS, 1 Mbps)	X	5.18	80.8	24.1	1.87	147.5	$\pm 1.2\%$
		Y	2.46	64.5	15.7		149.6	
		Z	3.46	71.5	19.9		114.9	
10013-CAB	IEEE 802.11g WiFi 2.4 GHz (DSSS-OFDM, 6 Mbps)	X	10.67	70.2	22.8	9.46	136.0	$\pm 2.7\%$
		Y	10.60	69.5	22.3		139.4	
		Z	10.27	68.4	21.8		106.6	
10059-CAB	IEEE 802.11b WiFi 2.4 GHz (DSSS, 2 Mbps)	X	5.95	83.5	25.3	2.12	144.6	$\pm 0.7\%$
		Y	2.73	66.2	16.7		149.3	
		Z	3.70	72.4	20.3		115.3	
10060-CAB	IEEE 802.11b WiFi 2.4 GHz (DSSS, 5.5 Mbps)	X	10.99	98.9	30.6	2.83	128.2	$\pm 0.9\%$
		Y	3.35	73.2	20.2		131.9	
		Z	8.60	90.5	27.1		145.6	
10061-CAB	IEEE 802.11b WiFi 2.4 GHz (DSSS, 11 Mbps)	X	14.67	99.7	30.9	3.60	127.5	$\pm 0.7\%$
		Y	3.91	72.2	20.1		132.3	
		Z	7.03	82.6	24.6		145.7	
10062-CAB	IEEE 802.11a/h WiFi 5 GHz (OFDM, 6 Mbps)	X	10.36	69.9	22.2	8.68	138.1	$\pm 2.2\%$
		Y	10.32	69.3	21.7		142.9	
		Z	9.97	68.3	21.3		109.6	
10063-CAB	IEEE 802.11a/h WiFi 5 GHz (OFDM, 9 Mbps)	X	10.25	69.9	22.1	8.63	137.4	$\pm 2.2\%$
		Y	10.21	69.2	21.6		144.7	
		Z	9.86	68.2	21.2		110.0	
10064-CAB	IEEE 802.11a/h WiFi 5 GHz (OFDM, 12 Mbps)	X	10.66	70.2	22.5	9.09	138.1	$\pm 2.5\%$
		Y	10.63	69.6	22.1		145.8	
		Z	10.30	68.6	21.7		110.5	
10065-CAB	IEEE 802.11a/h WiFi 5 GHz (OFDM, 18 Mbps)	X	10.37	70.1	22.5	9.00	134.2	$\pm 2.5\%$
		Y	10.34	69.5	22.0		141.7	
		Z	10.01	68.4	21.6		107.6	
10066-CAB	IEEE 802.11a/h WiFi 5 GHz (OFDM, 24 Mbps)	X	10.60	70.4	22.9	9.38	132.9	$\pm 2.7\%$
		Y	10.54	69.6	22.3		139.7	
		Z	10.27	68.7	22.0		107.1	
10067-CAB	IEEE 802.11a/h WiFi 5 GHz (OFDM, 36 Mbps)	X	11.10	70.9	23.6	10.12	131.6	$\pm 3.0\%$
		Y	11.05	70.1	23.1		137.5	
		Z	10.85	69.4	22.8		107.0	

Certificate No: EX3-3735_Jul15

Page 4 of 14

EX3DV4- SN:3735

July 16, 2015

10068-CAB	IEEE 802.11a/h WiFi 5 GHz (OFDM, 48 Mbps)	X	10.92	70.8	23.7	10.24	126.8	±3.0 %
		Y	10.85	69.9	23.1		133.2	
		Z	10.70	69.3	22.9		104.2	
10069-CAB	IEEE 802.11a/h WiFi 5 GHz (OFDM, 54 Mbps)	X	11.22	71.0	24.1	10.56	128.7	±3.0 %
		Y	10.52	68.4	22.4		93.7	
		Z	11.02	69.5	23.2		105.9	
10071-CAB	IEEE 802.11g WiFi 2.4 GHz (DSSS/OFDM, 9 Mbps)	X	10.74	70.4	23.2	9.83	131.2	±3.0 %
		Y	10.68	69.5	22.6		138.2	
		Z	10.47	68.8	22.4		105.9	
10072-CAB	IEEE 802.11g WiFi 2.4 GHz (DSSS/OFDM, 12 Mbps)	X	10.25	70.0	22.9	9.62	125.4	±2.5 %
		Y	10.19	69.2	22.3		132.4	
		Z	10.04	68.6	22.2		102.3	
10073-CAB	IEEE 802.11g WiFi 2.4 GHz (DSSS/OFDM, 18 Mbps)	X	10.25	70.1	23.2	9.94	121.4	±2.7 %
		Y	10.13	69.1	22.5		127.7	
		Z	10.14	68.9	22.6		99.9	
10074-CAB	IEEE 802.11g WiFi 2.4 GHz (DSSS/OFDM, 24 Mbps)	X	10.32	70.3	23.6	10.30	117.5	±2.7 %
		Y	10.15	69.1	22.7		123.1	
		Z	10.23	69.1	23.0		97.2	
10075-CAB	IEEE 802.11g WiFi 2.4 GHz (DSSS/OFDM, 36 Mbps)	X	10.42	70.5	24.0	10.77	114.3	±3.0 %
		Y	10.20	69.1	23.1		120.4	
		Z	10.38	69.5	23.5		94.8	
10076-CAB	IEEE 802.11g WiFi 2.4 GHz (DSSS/OFDM, 48 Mbps)	X	10.33	70.3	24.1	10.94	111.7	±3.0 %
		Y	10.14	69.0	23.2		117.2	
		Z	10.35	69.4	23.6		93.0	
10077-CAB	IEEE 802.11g WiFi 2.4 GHz (DSSS/OFDM, 54 Mbps)	X	10.33	70.4	24.2	11.00	110.5	±3.0 %
		Y	10.11	69.0	23.2		116.2	
		Z	10.34	69.5	23.7		92.3	
10114-CAB	IEEE 802.11n (HT Greenfield, 13.5 Mbps, BPSK)	X	10.48	69.9	21.7	8.10	148.6	±2.2 %
		Y	9.69	67.5	20.2		106.5	
		Z	10.01	68.3	20.8		116.5	
10115-CAB	IEEE 802.11n (HT Greenfield, 81 Mbps, 16-QAM)	X	10.02	68.1	20.9	8.46	101.0	±2.2 %
		Y	10.17	68.0	20.7		108.3	
		Z	10.55	68.9	21.3		119.8	
10116-CAB	IEEE 802.11n (HT Greenfield, 135 Mbps, 64-QAM)	X	9.59	67.7	20.5	8.15	99.3	±1.9 %
		Y	9.79	67.8	20.4		106.1	
		Z	10.06	68.4	20.9		117.0	
10117-CAB	IEEE 802.11n (HT Mixed, 13.5 Mbps, BPSK)	X	9.58	67.7	20.5	8.07	100.1	±1.9 %
		Y	9.75	67.7	20.3		106.6	
		Z	10.02	68.3	20.8		118.1	
10118-CAB	IEEE 802.11n (HT Mixed, 81 Mbps, 16-QAM)	X	10.17	68.3	21.0	8.59	101.6	±2.2 %
		Y	10.31	68.2	20.9		107.8	
		Z	10.67	69.0	21.5		120.4	
10119-CAB	IEEE 802.11n (HT Mixed, 135 Mbps, 64-QAM)	X	9.62	67.9	20.6	8.13	99.3	±1.9 %
		Y	9.73	67.6	20.3		105.5	
		Z	10.05	68.4	20.9		117.5	

EX3DV4- SN:3735

July 16, 2015

10193-CAB	IEEE 802.11n (HT Greenfield, 6.5 Mbps, BPSK)	X	10.06	69.8	21.7	8.09	142.7	±2.2 %
		Y	10.03	69.1	21.2		148.7	
		Z	9.66	68.1	20.9		112.6	
10194-CAB	IEEE 802.11n (HT Greenfield, 39 Mbps, 16-QAM)	X	10.10	69.8	21.7	8.12	142.3	±1.9 %
		Y	10.05	69.1	21.3		147.4	
		Z	9.68	68.1	20.9		113.1	
10195-CAB	IEEE 802.11n (HT Greenfield, 65 Mbps, 64-QAM)	X	10.24	70.0	21.9	8.21	142.8	±2.2 %
		Y	10.17	69.3	21.4		147.7	
		Z	9.75	68.1	20.9		113.5	
10196-CAB	IEEE 802.11n (HT Mixed, 6.5 Mbps, BPSK)	X	10.08	69.8	21.8	8.10	140.8	±1.9 %
		Y	9.94	68.9	21.1		147.5	
		Z	9.63	68.1	20.8		112.6	
10197-CAB	IEEE 802.11n (HT Mixed, 39 Mbps, 16-QAM)	X	10.12	69.8	21.8	8.13	141.6	±1.9 %
		Y	10.09	69.2	21.3		147.6	
		Z	9.65	68.0	20.8		112.5	
10198-CAB	IEEE 802.11n (HT Mixed, 65 Mbps, 64-QAM)	X	10.24	69.9	21.9	8.28	141.7	±1.9 %
		Y	10.22	69.3	21.5		146.6	
		Z	9.84	68.3	21.0		113.2	
10219-CAB	IEEE 802.11n (HT Mixed, 7.2 Mbps, BPSK)	X	9.96	69.7	21.7	8.03	140.1	±1.9 %
		Y	9.89	69.0	21.2		146.3	
		Z	9.47	67.8	20.7		111.3	
10220-CAB	IEEE 802.11n (HT Mixed, 43.3 Mbps, 16-QAM)	X	10.10	69.8	21.8	8.13	141.4	±1.9 %
		Y	10.08	69.2	21.3		147.4	
		Z	9.66	68.0	20.8		112.4	
10221-CAB	IEEE 802.11n (HT Mixed, 72.2 Mbps, 64-QAM)	X	10.28	70.0	21.9	8.27	142.2	±1.9 %
		Y	10.25	69.4	21.5		147.3	
		Z	9.81	68.1	20.9		112.9	
10222-CAB	IEEE 802.11n (HT Mixed, 15 Mbps, BPSK)	X	10.48	70.0	21.8	8.06	148.5	±1.9 %
		Y	9.73	67.8	20.4		104.7	
		Z	9.97	68.3	20.8		116.9	
10223-CAB	IEEE 802.11n (HT Mixed, 90 Mbps, 16-QAM)	X	10.05	68.2	21.0	8.48	101.5	±2.2 %
		Y	10.21	68.1	20.8		106.6	
		Z	10.54	68.8	21.3		119.6	
10224-CAB	IEEE 802.11n (HT Mixed, 150 Mbps, 64-QAM)	X	9.58	67.9	20.6	8.08	99.7	±1.9 %
		Y	9.74	67.8	20.5		104.7	
		Z	9.99	68.4	20.9		117.2	
10315-AAB	IEEE 802.11b WiFi 2.4 GHz (DSSS, 1 Mbps, 96pc duty cycle)	X	6.51	66.2	26.4	1.71	147.6	±0.7 %
		Y	3.20	69.8	18.4		108.5	
		Z	3.53	72.5	20.4		118.2	
10316-AAB	IEEE 802.11g WiFi 2.4 GHz (ERP-OFDM, 6 Mbps, 96pc duty cycle)	X	10.19	69.8	21.9	8.36	138.7	±2.2 %
		Y	10.18	69.3	21.6		143.5	
		Z	9.78	68.1	21.0		111.6	
10317-AAB	IEEE 802.11a WiFi 5 GHz (OFDM, 6 Mbps, 96pc duty cycle)	X	10.21	69.9	22.0	8.36	140.4	±2.2 %
		Y	10.21	69.3	21.5		148.0	
		Z	9.78	68.1	21.0		112.0	

EX3DV4- SN:3735

July 16, 2015

10415-AAA	IEEE 802.11b WiFi 2.4 GHz (DSSS, 1 Mbps, 99pc duty cycle)	X	9.26	93.6	29.0	1.54	145.9	±0.9 %
		Y	3.29	70.6	18.7		109.4	
		Z	3.36	72.0	20.2		120.1	
10416-AAA	IEEE 802.11g WiFi 2.4 GHz (ERP-OFDM, 6 Mbps, 99pc duty cycle)	X	10.14	69.9	21.9	8.23	139.7	±1.9 %
		Y	10.08	69.2	21.4		145.0	
		Z	9.69	68.0	20.9		111.6	
10417-AAA	IEEE 802.11a/h WiFi 5 GHz (OFDM, 6 Mbps, 99pc duty cycle)	X	10.17	69.9	21.9	8.23	140.9	±1.9 %
		Y	10.10	69.2	21.4		148.2	
		Z	9.66	68.0	20.9		111.9	
10418-AAA	IEEE 802.11g WiFi 2.4 GHz (DSSS-OFDM, 6 Mbps, 99pc duty cycle, Long preamble)	X	9.99	69.7	21.7	8.14	139.4	±1.9 %
		Y	9.98	69.2	21.3		146.6	
		Z	9.56	67.9	20.8		111.1	
10419-AAA	IEEE 802.11g WiFi 2.4 GHz (DSSS-OFDM, 6 Mbps, 99pc duty cycle, Short preamble)	X	10.09	69.8	21.9	8.19	139.7	±1.9 %
		Y	10.02	69.1	21.3		145.1	
		Z	9.66	68.1	20.9		111.7	
10422-AAA	IEEE 802.11n (HT Greenfield, 7.2 Mbps, BPSK)	X	10.29	69.9	21.9	8.32	141.8	±1.9 %
		Y	10.27	69.4	21.6		146.7	
		Z	9.85	68.2	21.0		113.2	
10423-AAA	IEEE 802.11n (HT Greenfield, 43.3 Mbps, 16-QAM)	X	10.47	70.1	22.1	8.47	142.0	±2.2 %
		Y	10.40	69.4	21.6		149.4	
		Z	10.02	68.3	21.2		113.4	
10424-AAA	IEEE 802.11n (HT Greenfield, 72.2 Mbps, 64-QAM)	X	10.38	70.1	22.1	8.40	141.4	±2.2 %
		Y	10.30	69.3	21.5		148.5	
		Z	9.98	68.4	21.2		114.1	
10425-AAA	IEEE 802.11n (HT Greenfield, 15 Mbps, BPSK)	X	10.86	70.3	22.1	8.41	149.7	±2.2 %
		Y	10.10	68.0	20.7		105.9	
		Z	10.48	68.8	21.3		120.6	
10426-AAA	IEEE 802.11n (HT Greenfield, 90 Mbps, 16-QAM)	X	9.97	68.1	21.0	8.45	100.1	±1.9 %
		Y	10.14	68.1	20.8		106.2	
		Z	10.47	68.8	21.3		119.7	
10427-AAA	IEEE 802.11n (HT Greenfield, 150 Mbps, 64-QAM)	X	9.96	68.1	20.9	8.41	100.3	±2.2 %
		Y	10.11	68.0	20.7		106.4	
		Z	10.46	68.8	21.3		120.5	

The reported uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor $k=2$, which for a normal distribution corresponds to a coverage probability of approximately 95%.

^A The uncertainties of Norm X,Y,Z do not affect the E^2 -field uncertainty inside TSL (see Pages 8 and 9).

^B Numerical linearization parameter: uncertainty not required.

^E Uncertainty is determined using the max. deviation from linear response applying rectangular distribution and is expressed for the square of the field value.

EX3DV4- SN:3735

July 16, 2015

DASY/EASY - Parameters of Probe: EX3DV4 - SN:3735

Calibration Parameter Determined in Head Tissue Simulating Media

f (MHz) ^C	Relative Permittivity ^F	Conductivity (S/m) ^F	ConvF X	ConvF Y	ConvF Z	Alpha ^G	Depth ^G (mm)	Unc (k=2)
150	52.3	0.76	11.17	11.17	11.17	0.00	1.00	± 13.3 %
220	49.0	0.81	10.50	10.50	10.50	0.00	1.00	± 13.3 %
2450	39.2	1.80	6.85	6.85	6.85	0.40	0.85	± 12.0 %
4950	36.3	4.40	5.26	5.26	5.26	0.35	1.80	± 13.1 %
5200	36.0	4.66	5.01	5.01	5.01	0.35	1.80	± 13.1 %
5300	35.9	4.76	4.73	4.73	4.73	0.35	1.80	± 13.1 %
5500	35.6	4.96	4.49	4.49	4.49	0.40	1.80	± 13.1 %
5600	35.5	5.07	4.29	4.29	4.29	0.40	1.80	± 13.1 %
5800	35.3	5.27	4.42	4.42	4.42	0.40	1.80	± 13.1 %

^C Frequency validity above 300 MHz of ± 100 MHz only applies for DASY v4.4 and higher (see Page 2), else it is restricted to ± 50 MHz. The uncertainty is the RSS of the ConvF uncertainty at calibration frequency and the uncertainty for the indicated frequency band. Frequency validity below 300 MHz is ± 10, 25, 40, 50 and 70 MHz for ConvF assessments at 30, 64, 128, 150 and 220 MHz respectively. Above 5 GHz frequency validity can be extended to ± 110 MHz.

^F At frequencies below 3 GHz, the validity of tissue parameters (ϵ and σ) can be relaxed to ± 10% if liquid compensation formula is applied to measured SAR values. At frequencies above 3 GHz, the validity of tissue parameters (ϵ and σ) is restricted to ± 5%. The uncertainty is the RSS of the ConvF uncertainty for indicated target tissue parameters.

^G Alpha/Depth are determined during calibration. SPEAG warrants that the remaining deviation due to the boundary effect after compensation is always less than ± 1% for frequencies below 3 GHz and below ± 2% for frequencies between 3-6 GHz at any distance larger than half the probe tip diameter from the boundary.

EX3DV4- SN:3735

July 16, 2015

DASY/EASY - Parameters of Probe: EX3DV4 - SN:3735

Calibration Parameter Determined in Body Tissue Simulating Media

f (MHz) ^C	Relative Permittivity ^F	Conductivity (S/m) ^F	ConvF X	ConvF Y	ConvF Z	Alpha ^G	Depth (mm) ^G	Unc (k=2)
150	61.9	0.80	10.63	10.63	10.63	0.00	1.00	± 13.3 %
220	60.2	0.86	9.94	9.94	9.94	0.00	1.00	± 13.3 %
2450	52.7	1.95	6.96	6.96	6.96	0.26	0.95	± 12.0 %
4950	49.4	5.01	4.57	4.57	4.57	0.40	1.90	± 13.1 %
5200	49.0	5.30	4.28	4.28	4.28	0.45	1.90	± 13.1 %
5300	48.9	5.42	4.10	4.10	4.10	0.45	1.90	± 13.1 %
5500	48.6	5.65	3.79	3.79	3.79	0.50	1.90	± 13.1 %
5600	48.5	5.77	3.70	3.70	3.70	0.50	1.90	± 13.1 %
5800	48.2	6.00	3.84	3.84	3.84	0.50	1.90	± 13.1 %

^C Frequency validity above 300 MHz of ± 100 MHz only applies for DASY v4.4 and higher (see Page 2), else it is restricted to ± 50 MHz. The uncertainty is the RSS of the ConvF uncertainty at calibration frequency and the uncertainty for the indicated frequency band. Frequency validity below 300 MHz is ± 10, 25, 40, 50 and 70 MHz for ConvF assessments at 30, 64, 128, 150 and 220 MHz respectively. Above 5 GHz frequency validity can be extended to ± 110 MHz.


^F At frequencies below 3 GHz, the validity of tissue parameters (ϵ and σ) can be relaxed to ± 10% if liquid compensation formula is applied to measured SAR values. At frequencies above 3 GHz, the validity of tissue parameters (ϵ and σ) is restricted to ± 5%. The uncertainty is the RSS of the ConvF uncertainty for indicated target tissue parameters.

^G Alpha/Depth are determined during calibration. SPEAG warrants that the remaining deviation due to the boundary effect after compensation is always less than ± 1% for frequencies below 3 GHz and below ± 2% for frequencies between 3-6 GHz at any distance larger than half the probe tip diameter from the boundary.

EX3DV4- SN:3735

July 16, 2015

Frequency Response of E-Field (TEM-Cell:ifi110 EXX, Waveguide: R22)


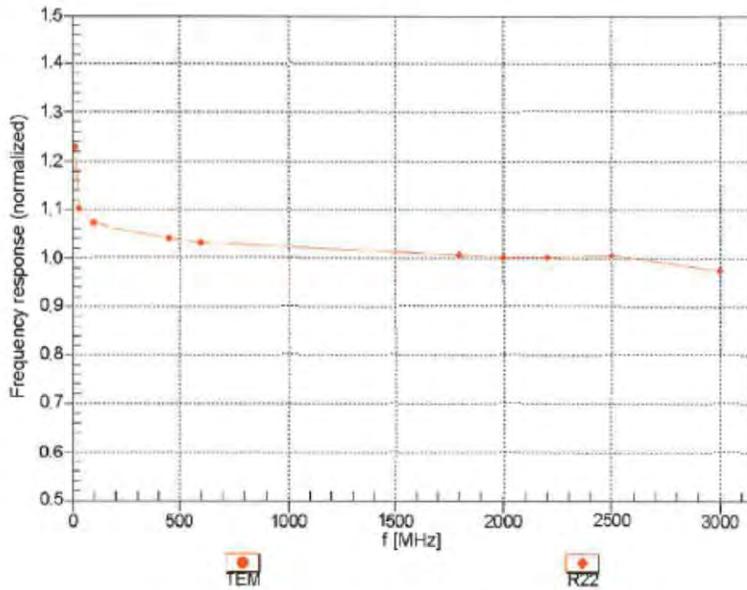


Uncertainty of Frequency Response of E-field: $\pm 6.3\%$ (k=2)

EX3DV4-- SN:3735



July 16, 2015

Receiving Pattern (ϕ), $\theta = 0^\circ$

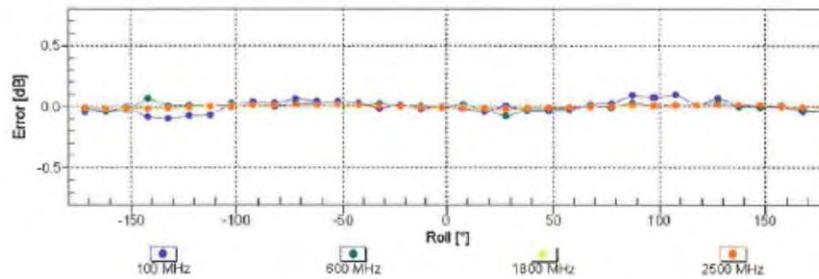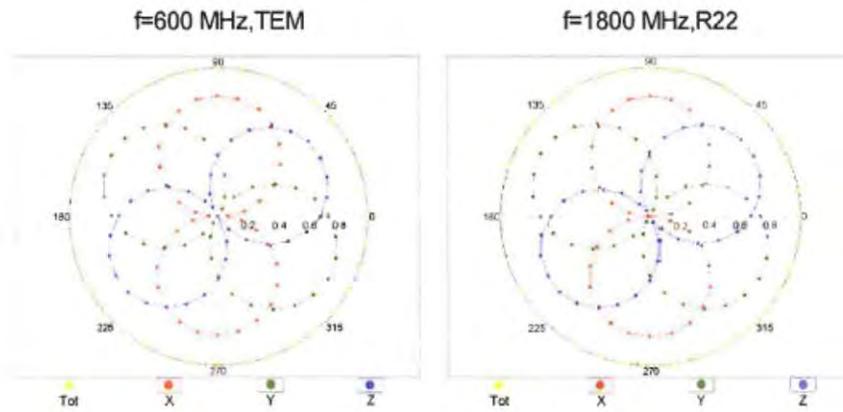


Uncertainty of Axial Isotropy Assessment: $\pm 0.5\%$ (k=2)

Dynamic Range f(SAR_{head}) (TEM cell, f_{eval} = 1900 MHz)

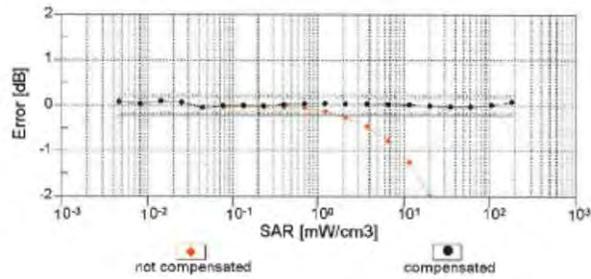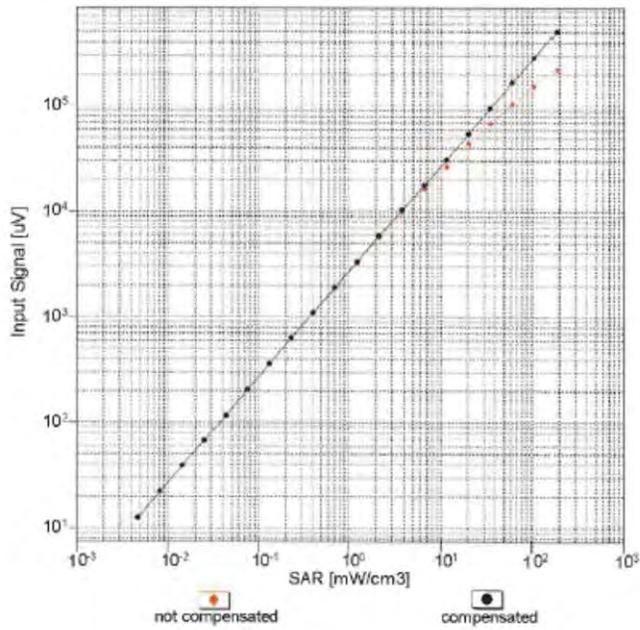



Uncertainty of Linearity Assessment: ± 0.6% (k=2)

Conversion Factor Assessment

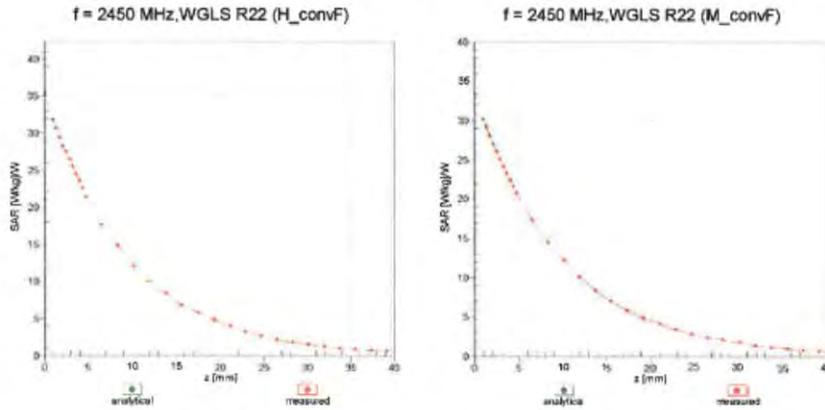

Deviation from Isotropy in Liquid

Error (ϕ, θ), f = 900 MHz

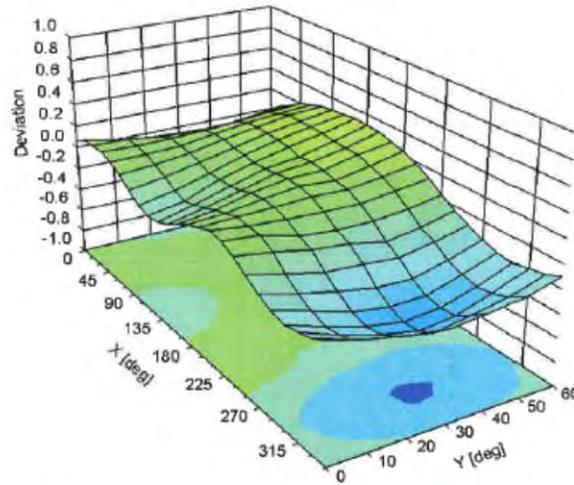

EX3DV4- SN:3735

July 16, 2015

DASY/EASY - Parameters of Probe: EX3DV4 - SN:3735

Other Probe Parameters

Sensor Arrangement	Triangular
Connector Angle (°)	-2.2
Mechanical Surface Detection Mode	enabled
Optical Surface Detection Mode	disabled
Probe Overall Length	337 mm
Probe Body Diameter	10 mm
Tip Length	9 mm
Tip Diameter	2.5 mm
Probe Tip to Sensor X Calibration Point	1 mm
Probe Tip to Sensor Y Calibration Point	1 mm
Probe Tip to Sensor Z Calibration Point	1 mm
Recommended Measurement Distance from Surface	1.4 mm

Appendix C Dipole Calibration Certificates

**Calibration Laboratory of
Schmid & Partner
Engineering AG**
Zeughausstrasse 43, 8004 Zurich, Switzerland



S Schweizerischer Kalibrierdienst
C Service suisse d'étalonnage
S Servizio svizzero di taratura
S Swiss Calibration Service

Accredited by the Swiss Accreditation Service (SAS)
The Swiss Accreditation Service is one of the signatories to the EA
Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: **SCS 0108**

Client **Motorola Solutions MY**

Certificate No: **D835V2-4d029_Mar15**

CALIBRATION CERTIFICATE																																															
Object	D835V2 - SN:4d029																																														
Calibration procedure(s)	QA CAL-05.v9 Calibration procedure for dipole validation kits above 700 MHz																																														
Calibration date:	March 20, 2015																																														
<p>This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI). The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.</p> <p>All calibrations have been conducted in the closed laboratory facility: environment temperature (22 ± 3)°C and humidity < 70%.</p> <p>Calibration Equipment used (M&TE critical for calibration)</p> <table border="1"> <thead> <tr> <th>Primary Standards</th> <th>ID #</th> <th>Cal Date (Certificate No.)</th> <th>Scheduled Calibration</th> </tr> </thead> <tbody> <tr> <td>Power meter EPM-442A</td> <td>GB37480704</td> <td>07-Oct-14 (No. 217-02020)</td> <td>Oct-15</td> </tr> <tr> <td>Power sensor HP 8481A</td> <td>US37292783</td> <td>07-Oct-14 (No. 217-02020)</td> <td>Oct-15</td> </tr> <tr> <td>Power sensor HP 8481A</td> <td>MY41092317</td> <td>07-Oct-14 (No. 217-02021)</td> <td>Oct-15</td> </tr> <tr> <td>Reference 20 dB Attenuator</td> <td>SN: 5058 (20k)</td> <td>03-Apr-14 (No. 217-01918)</td> <td>Apr-15</td> </tr> <tr> <td>Type-N mismatch combination</td> <td>SN: 5047.2 / 06327</td> <td>03-Apr-14 (No. 217-01921)</td> <td>Apr-15</td> </tr> <tr> <td>Reference Probe ES3DV3</td> <td>SN: 3205</td> <td>30-Dec-14 (No. ES3-3205_Dec14)</td> <td>Dec-15</td> </tr> <tr> <td>DAE4</td> <td>SN: 601</td> <td>18-Aug-14 (No. DAE4-601_Aug14)</td> <td>Aug-15</td> </tr> </tbody> </table> <table border="1"> <thead> <tr> <th>Secondary Standards</th> <th>ID #</th> <th>Check Date (in house)</th> <th>Scheduled Check</th> </tr> </thead> <tbody> <tr> <td>RF generator R&S SMT-06</td> <td>100005</td> <td>04-Aug-99 (in house check Oct-13)</td> <td>In house check: Oct-16</td> </tr> <tr> <td>Network Analyzer HP 8753E</td> <td>US37390585 S4206</td> <td>18-Oct-01 (in house check Oct-14)</td> <td>In house check: Oct-15</td> </tr> </tbody> </table>				Primary Standards	ID #	Cal Date (Certificate No.)	Scheduled Calibration	Power meter EPM-442A	GB37480704	07-Oct-14 (No. 217-02020)	Oct-15	Power sensor HP 8481A	US37292783	07-Oct-14 (No. 217-02020)	Oct-15	Power sensor HP 8481A	MY41092317	07-Oct-14 (No. 217-02021)	Oct-15	Reference 20 dB Attenuator	SN: 5058 (20k)	03-Apr-14 (No. 217-01918)	Apr-15	Type-N mismatch combination	SN: 5047.2 / 06327	03-Apr-14 (No. 217-01921)	Apr-15	Reference Probe ES3DV3	SN: 3205	30-Dec-14 (No. ES3-3205_Dec14)	Dec-15	DAE4	SN: 601	18-Aug-14 (No. DAE4-601_Aug14)	Aug-15	Secondary Standards	ID #	Check Date (in house)	Scheduled Check	RF generator R&S SMT-06	100005	04-Aug-99 (in house check Oct-13)	In house check: Oct-16	Network Analyzer HP 8753E	US37390585 S4206	18-Oct-01 (in house check Oct-14)	In house check: Oct-15
Primary Standards	ID #	Cal Date (Certificate No.)	Scheduled Calibration																																												
Power meter EPM-442A	GB37480704	07-Oct-14 (No. 217-02020)	Oct-15																																												
Power sensor HP 8481A	US37292783	07-Oct-14 (No. 217-02020)	Oct-15																																												
Power sensor HP 8481A	MY41092317	07-Oct-14 (No. 217-02021)	Oct-15																																												
Reference 20 dB Attenuator	SN: 5058 (20k)	03-Apr-14 (No. 217-01918)	Apr-15																																												
Type-N mismatch combination	SN: 5047.2 / 06327	03-Apr-14 (No. 217-01921)	Apr-15																																												
Reference Probe ES3DV3	SN: 3205	30-Dec-14 (No. ES3-3205_Dec14)	Dec-15																																												
DAE4	SN: 601	18-Aug-14 (No. DAE4-601_Aug14)	Aug-15																																												
Secondary Standards	ID #	Check Date (in house)	Scheduled Check																																												
RF generator R&S SMT-06	100005	04-Aug-99 (in house check Oct-13)	In house check: Oct-16																																												
Network Analyzer HP 8753E	US37390585 S4206	18-Oct-01 (in house check Oct-14)	In house check: Oct-15																																												
Calibrated by:	Name Israe Elnaouq	Function Laboratory Technician	Signature 																																												
Approved by:	Katja Pokovic	Technical Manager																																													
			Issued: March 20, 2015																																												
This calibration certificate shall not be reproduced except in full without written approval of the laboratory.																																															

**Calibration Laboratory of
Schmid & Partner
Engineering AG**
Zeughausstrasse 43, 8004 Zurich, Switzerland



S Schweizerischer Kalibrierdienst
C Service suisse d'étalonnage
S Servizio svizzero di taratura
S Swiss Calibration Service

Accredited by the Swiss Accreditation Service (SAS)
The Swiss Accreditation Service is one of the signatories to the EA
Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: **SCS 0108**

Glossary:

TSL tissue simulating liquid
ConvF sensitivity in TSL / NORM x,y,z
N/A not applicable or not measured

Calibration is Performed According to the Following Standards:

- a) IEEE Std 1528-2013, "IEEE Recommended Practice for Determining the Peak Spatial-Averaged Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques", June 2013
- b) IEC 62209-1, "Procedure to measure the Specific Absorption Rate (SAR) for hand-held devices used in close proximity to the ear (frequency range of 300 MHz to 3 GHz)", February 2005
- c) KDB 865664, "SAR Measurement Requirements for 100 MHz to 6 GHz"

Additional Documentation:

- d) DASY4/5 System Handbook

Methods Applied and Interpretation of Parameters:

- *Measurement Conditions:* Further details are available from the Validation Report at the end of the certificate. All figures stated in the certificate are valid at the frequency indicated.
- *Antenna Parameters with TSL:* The dipole is mounted with the spacer to position its feed point exactly below the center marking of the flat phantom section, with the arms oriented parallel to the body axis.
- *Feed Point Impedance and Return Loss:* These parameters are measured with the dipole positioned under the liquid filled phantom. The impedance stated is transformed from the measurement at the SMA connector to the feed point. The Return Loss ensures low reflected power. No uncertainty required.
- *Electrical Delay:* One-way delay between the SMA connector and the antenna feed point. No uncertainty required.
- *SAR measured:* SAR measured at the stated antenna input power.
- *SAR normalized:* SAR as measured, normalized to an input power of 1 W at the antenna connector.
- *SAR for nominal TSL parameters:* The measured TSL parameters are used to calculate the nominal SAR result.

The reported uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor k=2, which for a normal distribution corresponds to a coverage probability of approximately 95%.

Measurement Conditions

DASY system configuration, as far as not given on page 1.

DASY Version	DASY5	V52.8.8
Extrapolation	Advanced Extrapolation	
Phantom	Modular Flat Phantom	
Distance Dipole Center - TSL	15 mm	with Spacer
Zoom Scan Resolution	dx, dy, dz = 5 mm	
Frequency	835 MHz ± 1 MHz	

Head TSL parameters

The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Head TSL parameters	22.0 °C	41.5	0.90 mho/m
Measured Head TSL parameters	(22.0 ± 0.2) °C	40.6 ± 6 %	0.92 mho/m ± 6 %
Head TSL temperature change during test	< 0.5 °C	----	----

SAR result with Head TSL

SAR averaged over 1 cm ³ (1 g) of Head TSL	Condition	
SAR measured	250 mW input power	2.37 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	9.28 W/kg ± 17.0 % (k=2)

SAR averaged over 10 cm ³ (10 g) of Head TSL	condition	
SAR measured	250 mW input power	1.54 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	6.06 W/kg ± 16.5 % (k=2)

Body TSL parameters

The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Body TSL parameters	22.0 °C	55.2	0.97 mho/m
Measured Body TSL parameters	(22.0 ± 0.2) °C	54.6 ± 6 %	1.02 mho/m ± 6 %
Body TSL temperature change during test	< 0.5 °C	----	----

SAR result with Body TSL

SAR averaged over 1 cm ³ (1 g) of Body TSL	Condition	
SAR measured	250 mW input power	2.38 W/kg
SAR for nominal Body TSL parameters	normalized to 1W	9.15 W/kg ± 17.0 % (k=2)

SAR averaged over 10 cm ³ (10 g) of Body TSL	condition	
SAR measured	250 mW input power	1.55 W/kg
SAR for nominal Body TSL parameters	normalized to 1W	6.01 W/kg ± 16.5 % (k=2)

Appendix (Additional assessments outside the scope of SCS 0108)

Antenna Parameters with Head TSL

Impedance, transformed to feed point	51.6 Ω - 2.3 j Ω
Return Loss	- 31.3 dB

Antenna Parameters with Body TSL

Impedance, transformed to feed point	48.3 Ω - 3.4 j Ω
Return Loss	- 28.1 dB

General Antenna Parameters and Design

Electrical Delay (one direction)	1.388 ns
----------------------------------	----------

After long term use with 100W radiated power, only a slight warming of the dipole near the feedpoint can be measured.

The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals. On some of the dipoles, small end caps are added to the dipole arms in order to improve matching when loaded according to the position as explained in the "Measurement Conditions" paragraph. The SAR data are not affected by this change. The overall dipole length is still according to the Standard.

No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feedpoint may be damaged.

Additional EUT Data

Manufactured by	SPEAG
Manufactured on	December 17, 2004

DASY5 Validation Report for Head TSL

Date: 19.03.2015

Test Laboratory: SPEAG, Zurich, Switzerland

DUT: Dipole 835 MHz; Type: D835V2; Serial: D835V2 - SN:4d029

Communication System: UID 0 - CW; Frequency: 835 MHz

Medium parameters used: $f = 835 \text{ MHz}$; $\sigma = 0.92 \text{ S/m}$; $\epsilon_r = 40.6$; $\rho = 1000 \text{ kg/m}^3$

Phantom section: Flat Section

Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2011)

DASY52 Configuration:

- Probe: ES3DV3 - SN3205; ConvF(6.2, 6.2, 6.2); Calibrated: 30.12.2014;
- Sensor-Surface: 3mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn601; Calibrated: 18.08.2014
- Phantom: Flat Phantom 4.9L; Type: QD000P49AA; Serial: 1001
- DASY52 52.8.8(1222); SEMCAD X 14.6.10(7331)

Dipole Calibration for Head Tissue/Pin=250 mW, d=15mm/Zoom Scan (7x7x7)/Cube 0:


Measurement grid: $dx=5\text{mm}$, $dy=5\text{mm}$, $dz=5\text{mm}$

Reference Value = 56.74 V/m; Power Drift = 0.01 dB


Peak SAR (extrapolated) = 3.54 W/kg

SAR(1 g) = 2.37 W/kg; SAR(10 g) = 1.54 W/kg

Maximum value of SAR (measured) = 2.77 W/kg

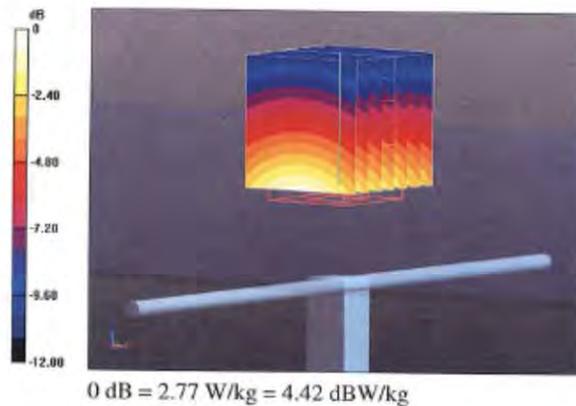

Impedance Measurement Plot for Head TSL

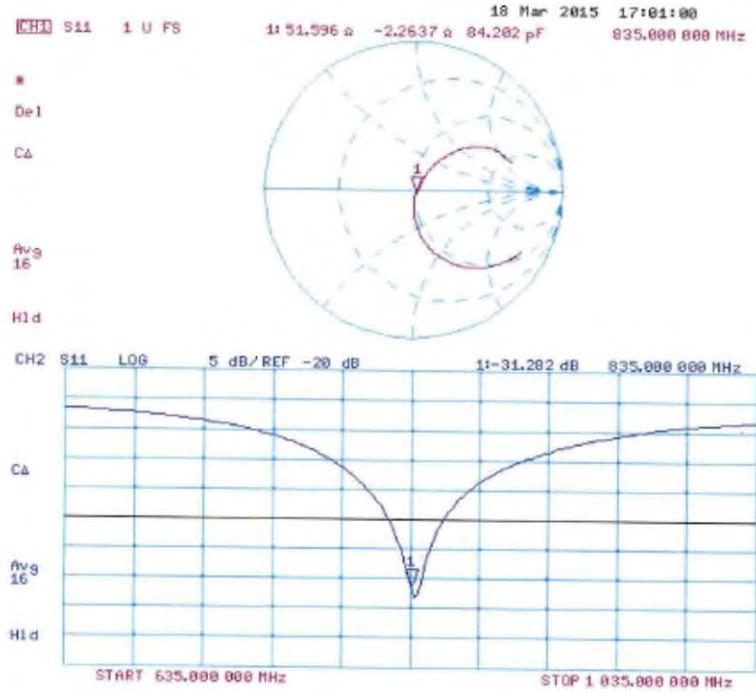

DASY5 Validation Report for Body TSL

Date: 20.03.2015

Test Laboratory: SPEAG, Zurich, Switzerland

DUT: Dipole 835 MHz; Type: D835V2; Serial: D835V2 - SN:4d029

Communication System: UID 0 - CW; Frequency: 835 MHz

Medium parameters used: $f = 835 \text{ MHz}$; $\sigma = 1.02 \text{ S/m}$; $\epsilon_r = 54.6$; $\rho = 1000 \text{ kg/m}^3$

Phantom section: Flat Section

Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2011)

DASY52 Configuration:

- Probe: ES3DV3 - SN3205; ConvF(6.17, 6.17, 6.17); Calibrated: 30.12.2014;
- Sensor-Surface: 3mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn601; Calibrated: 18.08.2014
- Phantom: Flat Phantom 4.9L; Type: QD000P49AA; Serial: 1001
- DASY52 52.8.8(1222); SEMCAD X 14.6.10(7331)

Dipole Calibration for Body Tissue/Pin=250 mW, d=15mm/Zoom Scan (7x7x7)/Cube 0:


Measurement grid: $dx=5\text{mm}$, $dy=5\text{mm}$, $dz=5\text{mm}$

Reference Value = 54.10 V/m; Power Drift = -0.01 dB


Peak SAR (extrapolated) = 3.50 W/kg

SAR(1 g) = 2.38 W/kg; SAR(10 g) = 1.55 W/kg

Maximum value of SAR (measured) = 2.78 W/kg

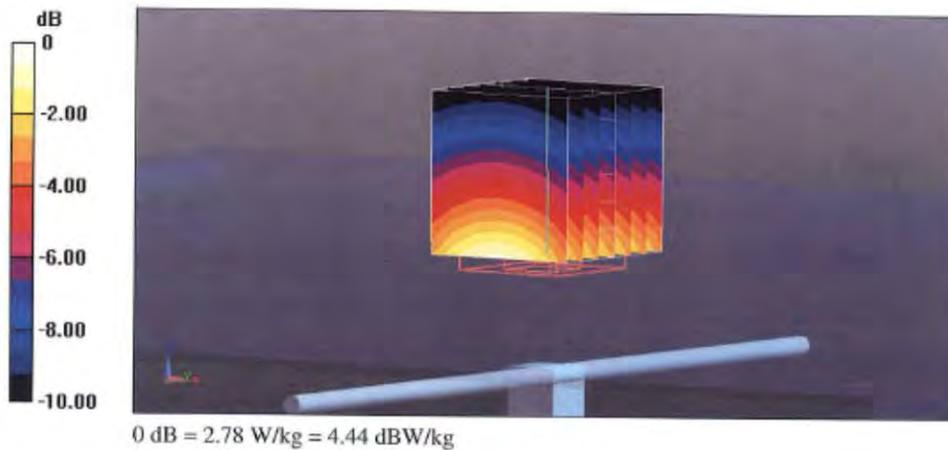

Impedance Measurement Plot for Body TSL

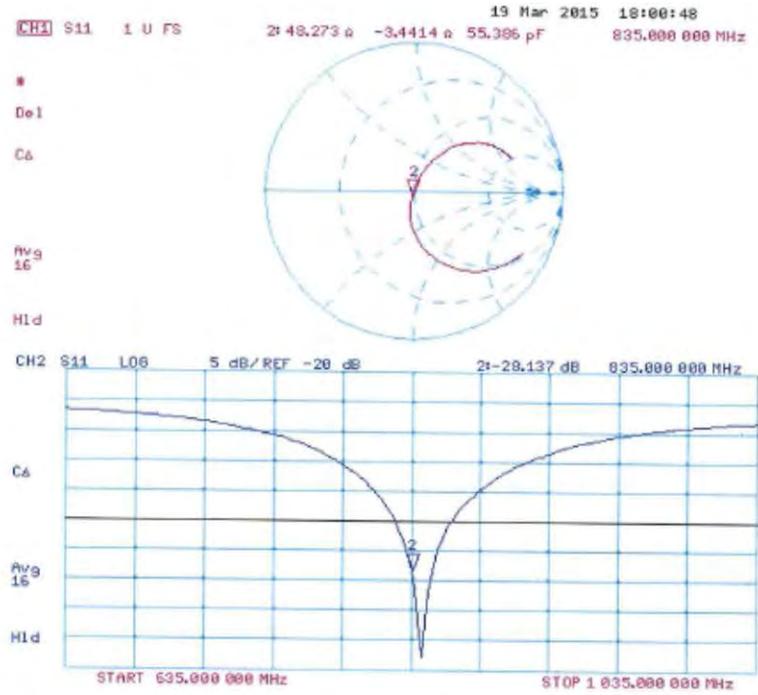

**Calibration Laboratory of
Schmid & Partner
Engineering AG**
Zeughausstrasse 43, 8004 Zurich, Switzerland



S Schweizerischer Kalibrierdienst
C Service suisse d'étalonnage
S Servizio svizzero di taratura
S Swiss Calibration Service

Accredited by the Swiss Accreditation Service (SAS)
The Swiss Accreditation Service is one of the signatories to the EA
Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: **SCS 0108**

Client **Motorola Solutions MY**

Certificate No: **D2450V2-781_Mar15**

CALIBRATION CERTIFICATE

Object **D2450V2 - SN:781**

Calibration procedure(s) **QA CAL-05.v9
Calibration procedure for dipole validation kits above 700 MHz**

Calibration date: **March 20, 2015**

This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI).
The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility, environment temperature (22 ± 3)°C and humidity < 70%.

Calibration Equipment used (M&TE critical for calibration)

Primary Standards	ID #	Cal Date (Certificate No.)	Scheduled Calibration
Power meter EPM-442A	GB37480704	07-Oct-14 (No. 217-02020)	Oct-15
Power sensor HP 8481A	US37292783	07-Oct-14 (No. 217-02020)	Oct-15
Power sensor HP 8481A	MY41092317	07-Oct-14 (No. 217-02021)	Oct-15
Reference 20 dB Attenuator	SN: 5058 (20k)	03-Apr-14 (No. 217-01918)	Apr-15
Type-N mismatch combination	SN: 5047.2 / 06327	03-Apr-14 (No. 217-01921)	Apr-15
Reference Probe ES3DV3	SN: 3205	30-Dec-14 (No. ES3-3205_Dec14)	Dec-15
DAE4	SN: 601	18-Aug-14 (No. DAE4-601_Aug14)	Aug-15

Secondary Standards	ID #	Check Date (in house)	Scheduled Check
RF generator R&S SMT-06	100005	04-Aug-09 (in house check Oct-13)	In house check: Oct-16
Network Analyzer HP 8753E	US37390585 S4206	18-Oct-01 (in house check Oct-14)	In house check: Oct-15

Calibrated by:	Name Israa Elnaouq	Function Laboratory Technician	Signature
Approved by:	Name Katja Pokovic	Technical Manager	

Issued: March 20, 2015

This calibration certificate shall not be reproduced except in full without written approval of the laboratory.

**Calibration Laboratory of
Schmid & Partner
Engineering AG**
Zougheustrasse 43, 8004 Zurich, Switzerland



S Schweizerischer Kalibrierdienst
S Service suisse d'étalonnage
C Servizio svizzero di taratura
S Swiss Calibration Service

Accredited by the Swiss Accreditation Service (SAS)
The Swiss Accreditation Service is one of the signatories to the EA
Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: **SCS 0108**

Glossary:

TSL tissue simulating liquid
ConvF sensitivity in TSL / NORM x,y,z
N/A not applicable or not measured

Calibration is Performed According to the Following Standards:

- a) IEEE Std 1528-2013, "IEEE Recommended Practice for Determining the Peak Spatial-Averaged Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques", June 2013
- b) IEC 62209-1, "Procedure to measure the Specific Absorption Rate (SAR) for hand-held devices used in close proximity to the ear (frequency range of 300 MHz to 3 GHz)", February 2005
- c) KDB 865664, "SAR Measurement Requirements for 100 MHz to 6 GHz"

Additional Documentation:

- d) DASY4/5 System Handbook

Methods Applied and Interpretation of Parameters:

- *Measurement Conditions:* Further details are available from the Validation Report at the end of the certificate. All figures stated in the certificate are valid at the frequency indicated.
- *Antenna Parameters with TSL:* The dipole is mounted with the spacer to position its feed point exactly below the center marking of the flat phantom section, with the arms oriented parallel to the body axis.
- *Feed Point Impedance and Return Loss:* These parameters are measured with the dipole positioned under the liquid filled phantom. The impedance stated is transformed from the measurement at the SMA connector to the feed point. The Return Loss ensures low reflected power. No uncertainty required.
- *Electrical Delay:* One-way delay between the SMA connector and the antenna feed point. No uncertainty required.
- *SAR measured:* SAR measured at the stated antenna input power.
- *SAR normalized:* SAR as measured, normalized to an input power of 1 W at the antenna connector.
- *SAR for nominal TSL parameters:* The measured TSL parameters are used to calculate the nominal SAR result.

The reported uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor k=2, which for a normal distribution corresponds to a coverage probability of approximately 95%.

Measurement Conditions

DASY system configuration, as far as not given on page 1.

DASY Version	DASY5	V52.8.8
Extrapolation	Advanced Extrapolation	
Phantom	Modular Flat Phantom	
Distance Dipole Center - TSL	10 mm	with Spacer
Zoom Scan Resolution	dx, dy, dz = 5 mm	
Frequency	2450 MHz ± 1 MHz	

Head TSL parameters

The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Head TSL parameters	22.0 °C	39.2	1.80 mho/m
Measured Head TSL parameters	(22.0 ± 0.2) °C	37.8 ± 6 %	1.83 mho/m ± 6 %
Head TSL temperature change during test	< 0.5 °C	---	---

SAR result with Head TSL

SAR averaged over 1 cm ³ (1 g) of Head TSL	Condition	
SAR measured	250 mW input power	13.3 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	52.3 W/kg ± 17.0 % (k=2)

SAR averaged over 10 cm ³ (10 g) of Head TSL	condition	
SAR measured	250 mW input power	6.16 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	24.4 W/kg ± 16.5 % (k=2)

Body TSL parameters

The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Body TSL parameters	22.0 °C	52.7	1.95 mho/m
Measured Body TSL parameters	(22.0 ± 0.2) °C	50.8 ± 6 %	2.02 mho/m ± 6 %
Body TSL temperature change during test	< 0.5 °C	---	---

SAR result with Body TSL

SAR averaged over 1 cm ³ (1 g) of Body TSL	Condition	
SAR measured	250 mW input power	13.3 W/kg
SAR for nominal Body TSL parameters	normalized to 1W	51.9 W/kg ± 17.0 % (k=2)

SAR averaged over 10 cm ³ (10 g) of Body TSL	condition	
SAR measured	250 mW input power	6.15 W/kg
SAR for nominal Body TSL parameters	normalized to 1W	24.2 W/kg ± 16.5 % (k=2)

Appendix (Additional assessments outside the scope of SCS 0108)

Antenna Parameters with Head TSL

Impedance, transformed to feed point	53.9 Ω + 1.2 jΩ
Return Loss	- 28.2 dB

Antenna Parameters with Body TSL

Impedance, transformed to feed point	49.9 Ω + 3.2 jΩ
Return Loss	- 30.0 dB

General Antenna Parameters and Design

Electrical Delay (one direction)	1.155 ns
----------------------------------	----------

After long term use with 100W radiated power, only a slight warming of the dipole near the feedpoint can be measured.

The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals. On some of the dipoles, small end caps are added to the dipole arms in order to improve matching when loaded according to the position as explained in the "Measurement Conditions" paragraph. The SAR data are not affected by this change. The overall dipole length is still according to the Standard.

No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feedpoint may be damaged.

Additional EUT Data

Manufactured by	SPEAG
Manufactured on	May 06, 2005

DASY5 Validation Report for Head TSL

Date: 20.03.2015

Test Laboratory: SPEAG, Zurich, Switzerland

DUT: Dipole 2450 MHz; Type: D2450V2; Serial: D2450V2 - SN:781

Communication System: UID 0 - CW; Frequency: 2450 MHz

Medium parameters used: $f = 2450 \text{ MHz}$; $\sigma = 1.83 \text{ S/m}$; $\epsilon_r = 37.8$; $\rho = 1000 \text{ kg/m}^3$

Phantom section: Flat Section

Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2011)

DASY52 Configuration:

- Probe: ES3DV3 - SN3205; ConvF(4.54, 4.54, 4.54); Calibrated: 30.12.2014;
- Sensor-Surface: 3mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn601; Calibrated: 18.08.2014
- Phantom: Flat Phantom 5.0 (front); Type: QD000P50AA; Serial: 1001
- DASY52 52.8.8(1222); SEMCAD X 14.6.10(7331)

Dipole Calibration for Head Tissue/Pin=250 mW, d=10mm/Zoom Scan (7x7x7)/Cube 0:

Measurement grid: $dx=5\text{mm}$, $dy=5\text{mm}$, $dz=5\text{mm}$

Reference Value = 101.2 V/m; Power Drift = 0.01 dB

Peak SAR (extrapolated) = 27.9 W/kg


SAR(1 g) = 13.3 W/kg; SAR(10 g) = 6.16 W/kg

Maximum value of SAR (measured) = 17.4 W/kg



0 dB = 17.4 W/kg = 12.41 dBW/kg

Impedance Measurement Plot for Head TSL

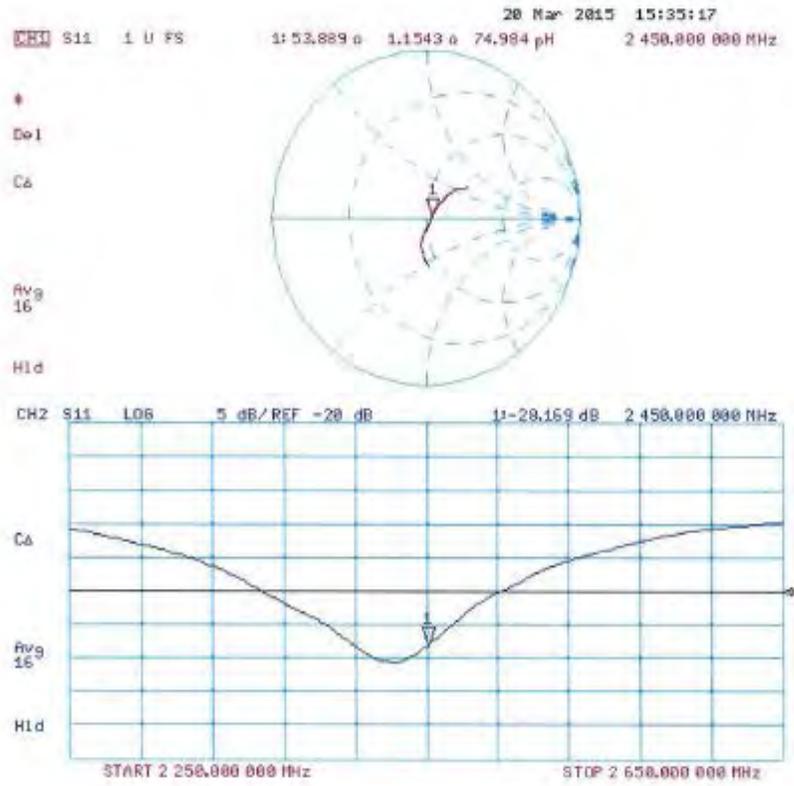

DASY5 Validation Report for Body TSL

Date: 19.03.2015

Test Laboratory: SPEAG, Zurich, Switzerland

DUT: Dipole 2450 MHz; Type: D2450V2; Serial: D2450V2 - SN:781

Communication System: UID 0 - CW; Frequency: 2450 MHz

Medium parameters used: $f = 2450$ MHz; $\sigma = 2.02$ S/m; $\epsilon_r = 50.8$; $\rho = 1000$ kg/m³

Phantom section: Flat Section

Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2011)

DASY52 Configuration:

- Probe: ES3DV3 - SN3205; ConvF(4.32, 4.32, 4.32); Calibrated: 30.12.2014;
- Sensor-Surface: 3mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn601; Calibrated: 18.08.2014
- Phantom: Flat Phantom 5.0 (back); Type: QD000P50AA; Serial: 1002
- DASY52 52.8.8(1222); SEMCAD X 14.6.10(7331)

Dipole Calibration for Body Tissue/Pin=250 mW, d=10mm/Zoom Scan (7x7x7)/Cube 0:

Measurement grid: dx=5mm, dy=5mm, dz=5mm

Reference Value = 95.66 V/m; Power Drift = 0.03 dB

Peak SAR (extrapolated) = 28.0 W/kg


SAR(1 g) = 13.3 W/kg; SAR(10 g) = 6.15 W/kg

Maximum value of SAR (measured) = 17.4 W/kg



0 dB = 17.4 W/kg = 12.41 dBW/kg

Impedance Measurement Plot for Body TSL

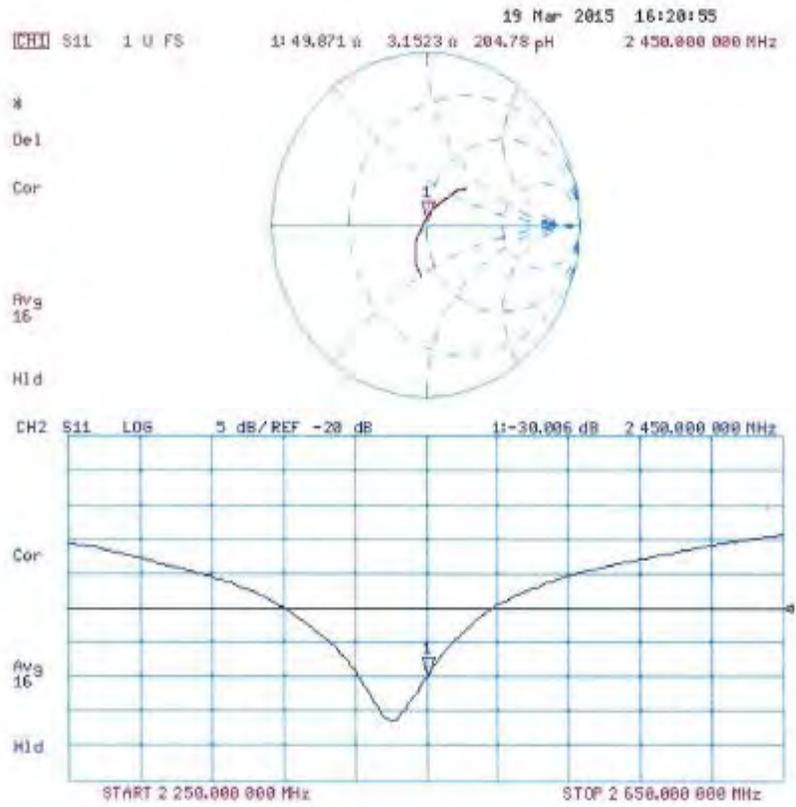

Dipole Data

As stated in KDB 865664, only dipoles exceed annual calibration interval required to provide supporting information and measurement to qualify for extended calibration interval.

The table below includes dipole impedance and return loss measurement data measured by Motorola Solutions' EME lab. The results meet requirements stated in KDB 865664.

Dipole D835V2 (SN 4D029)	Head			Body		
	Impedance		Return Loss	Impedance		Return Loss
	real Ω	imag $j\Omega$	dB	real Ω	imag $j\Omega$	dB
04/16/2015	51.23	-2.35	-31.79	48.03	-2.55	-28.29
02/16/2016	49.98	-3.64	-28.84	46.39	-3.09	-26.26

Dipole D2450V2 (SN 781)	Head			Body		
	Impedance		Return Loss	Impedance		Return Loss
	real Ω	imag $j\Omega$	dB	real Ω	imag $j\Omega$	dB
04/14/2015	53.04	3.88	-26.54	49.66	3.79	-28.55
02/15/2016	53.32	3.21	-27.02	50.38	4.72	-30.76