

APPENDIX

11. Photographs of Test Setup



Fig.1 Photograph of the SAR measurement system

Photograph of the Tissue Simulant Fluid Liquid Depth

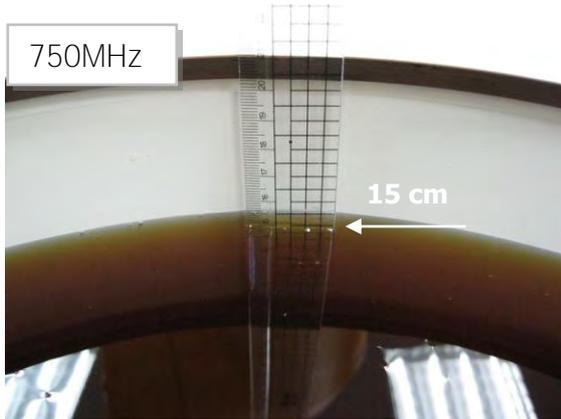


Fig.2.1

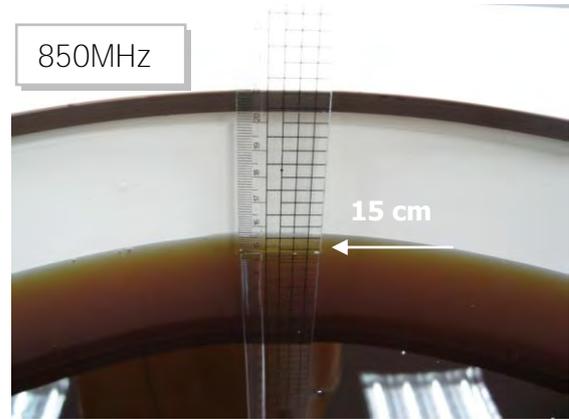


Fig.2.2

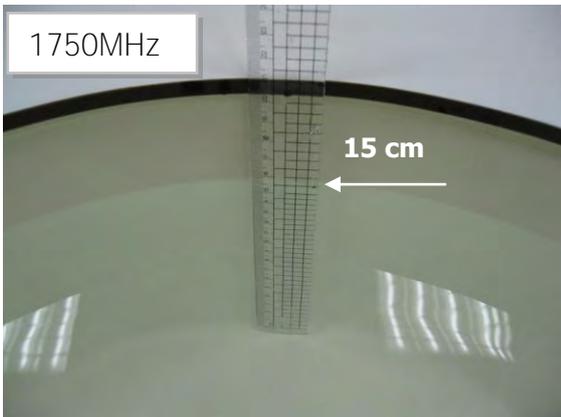


Fig.2.3

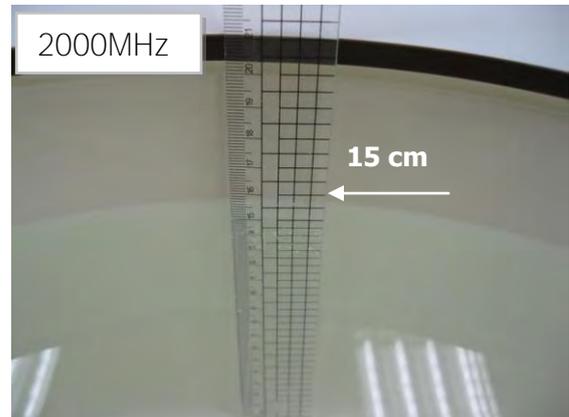


Fig.2.4

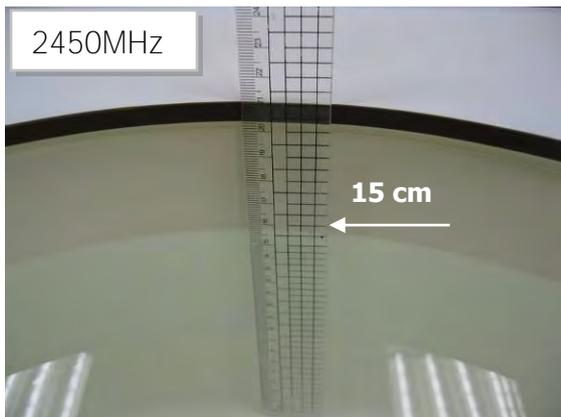


Fig.2.5

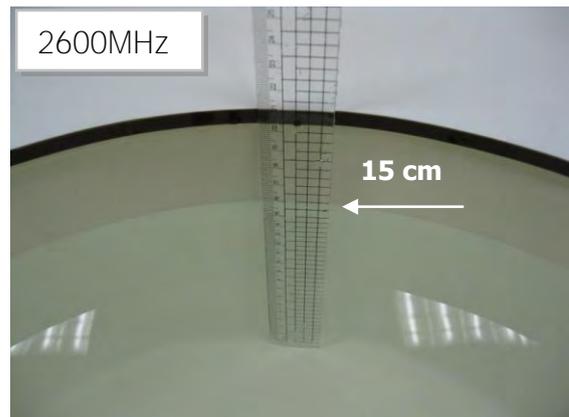


Fig.2.6

Photograph of the Tissue Simulant Fluid Liquid Depth

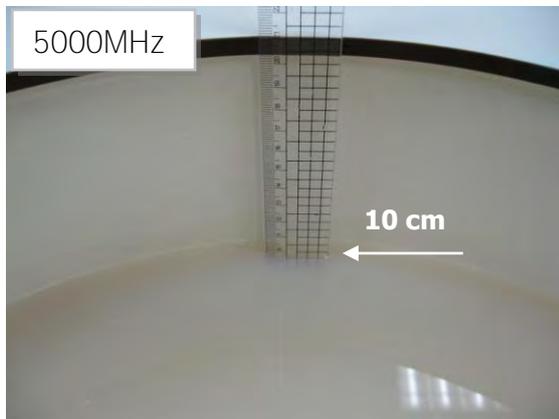


Fig.2.7

Body - distance between flat phantom and EUT is 0 mm

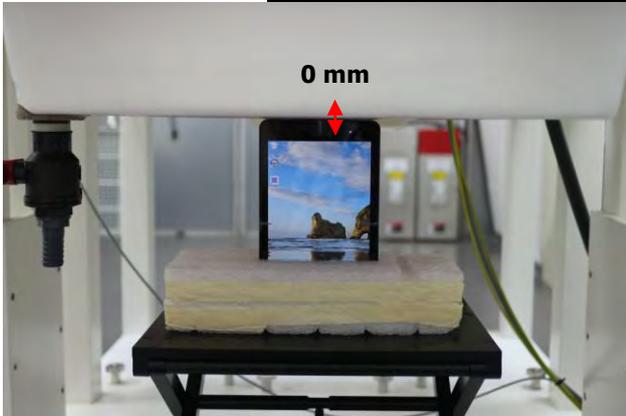


Fig.3 EUT Top side to flat phantom

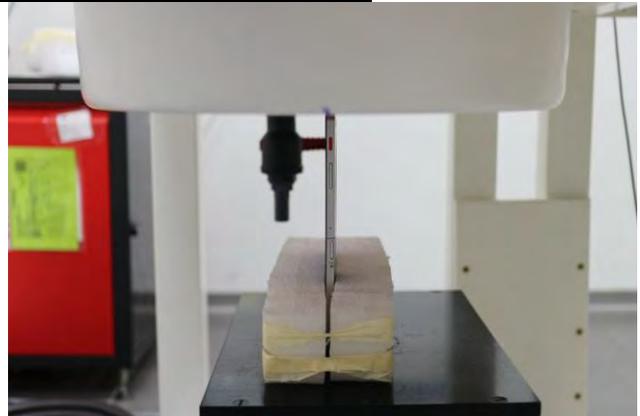


Fig.4 EUT Back side to flat phantom

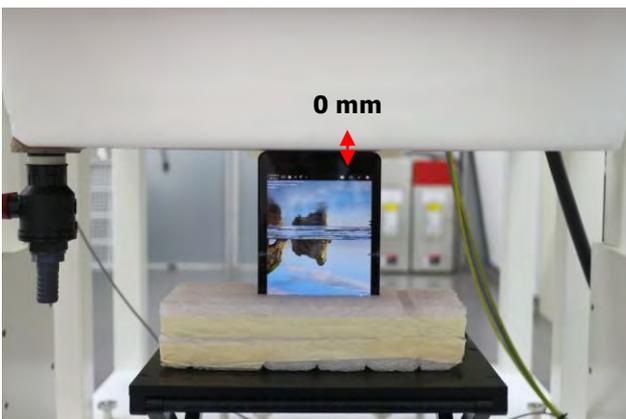
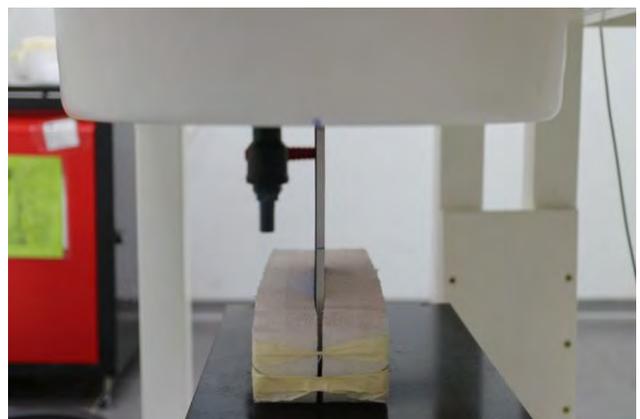


Fig.5 EUT Bottom side to flat phantom



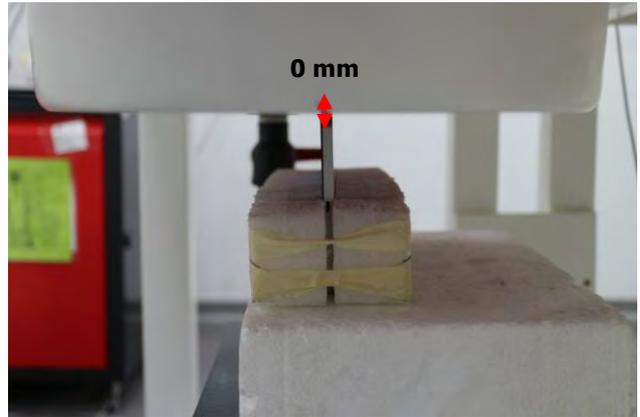


Fig.6 EUT Right side to flat phantom

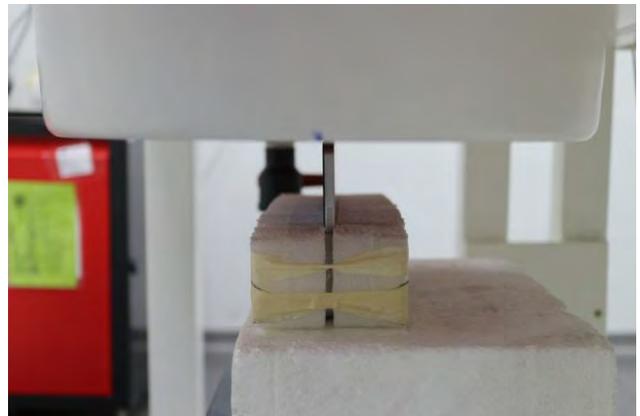
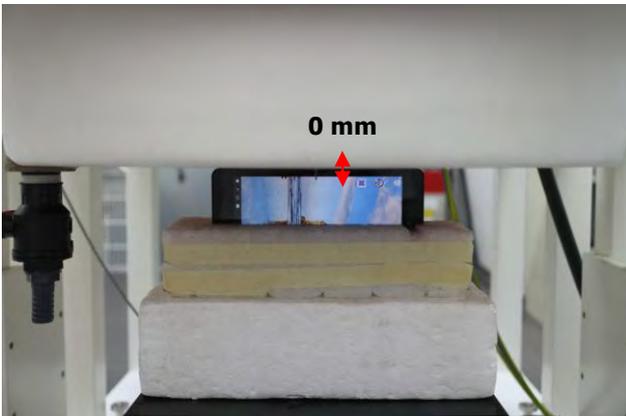


Fig.7 EUT Left side to flat phantom

Body - distance between flat phantom and EUT is 5 mm

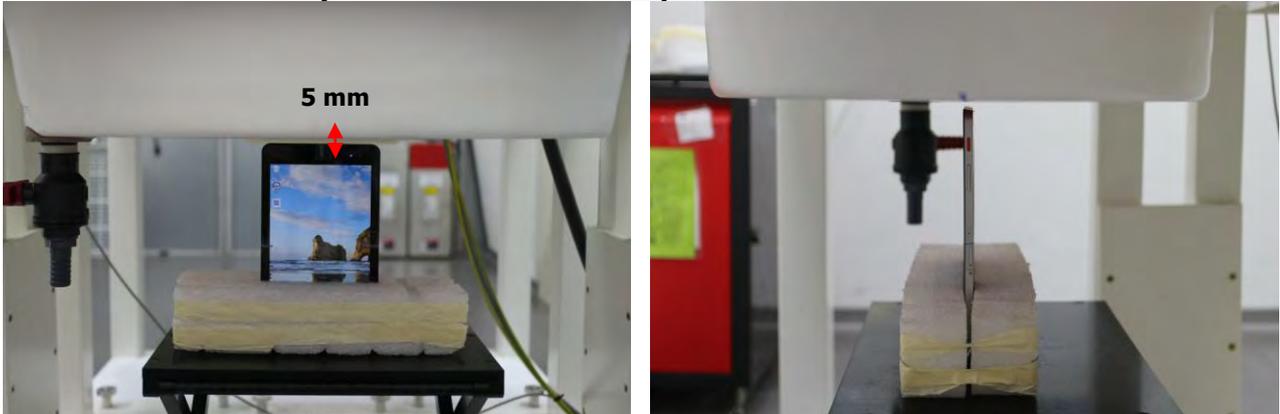


Fig.8 EUT Top side to flat phantom

Body - distance between flat phantom and EUT is 10 mm



Fig.9 EUT Back side to flat phantom

12. Photographs of the EUT

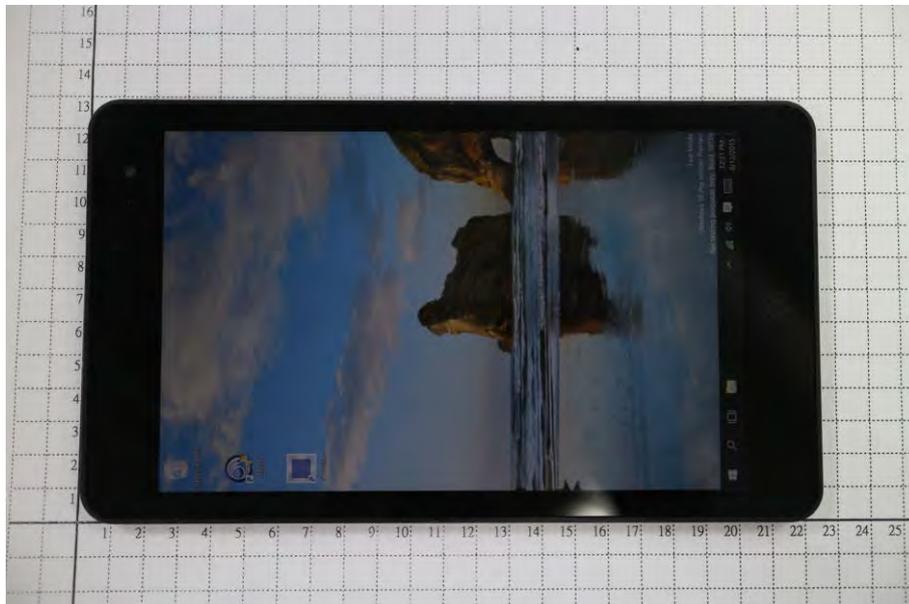


Fig.10 Front view of EUT

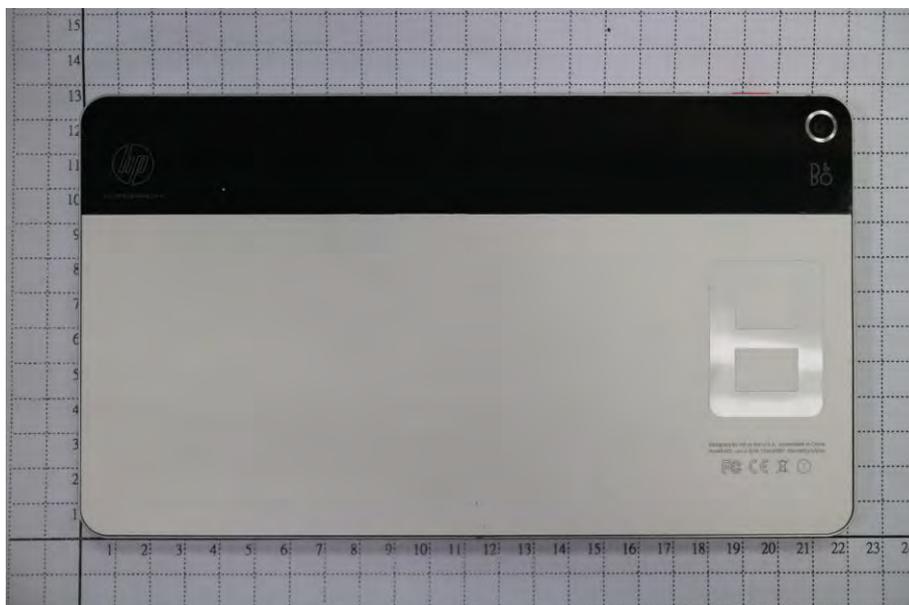


Fig.11 Back view of EUT

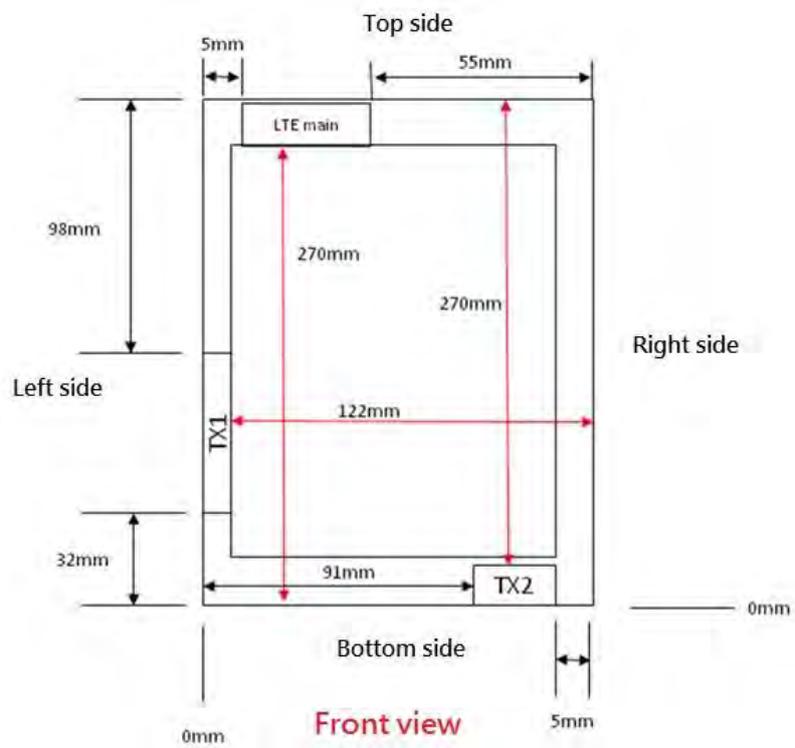


Fig.12 Antenna position of EUT (Front view)

- End of Report -