

APPENDIX A: VERIFICATION PLOTS

ELEMENT

DUT: Dipole 2450.000 MHz; Type: D2450V2 - SN750

Communication System: UID: 0, CW; Frequency: 2450.000 MHz
Medium: 2450 Head; Medium parameters used:
 $f = 2450.000$ MHz; $\text{cond} = 1.80$ S/m; $\text{perm} = 38.0$; $\text{density} = 1000$ kg/m³
Phantom Section: Flat; Space: 10 mm

Test Date: 07/28/2025; Ambient Temp: 23.5°C; Tissue Temp: 20.9°C

Probe: EX3DV4 - SN7360; ConvF:(7.14,7.04,8.0); Calibrated: 2025-03-07
Sensor-Surface: 1.4mm (VMS + 6p)
Electronics: DAE4 Sn534; Calibrated: 2025-03-11
Phantom: Twin-SAM V8.0; Serial: 2034
Measurement SW: DASY Module SAR V16.4.0.5005

2450.0 MHz System Verification at 20.0 dBm (100 mW)


Area Scan (40.0 x 80.0): Measurement grid: $dx=10.0$ mm, $dy=10.0$ mm

Zoom Scan (30.0 x 30.0 x 31.2): Measurement grid: $dx=5.0$ mm, $dy=5.0$ mm, $dz=1.5$ mm; Graded Ratio: 1.5

Peak SAR (extrapolated) = 11.7 W/kg

SAR(1 g) = 5.75 W/kg

Deviation (1 g) = 7.88%

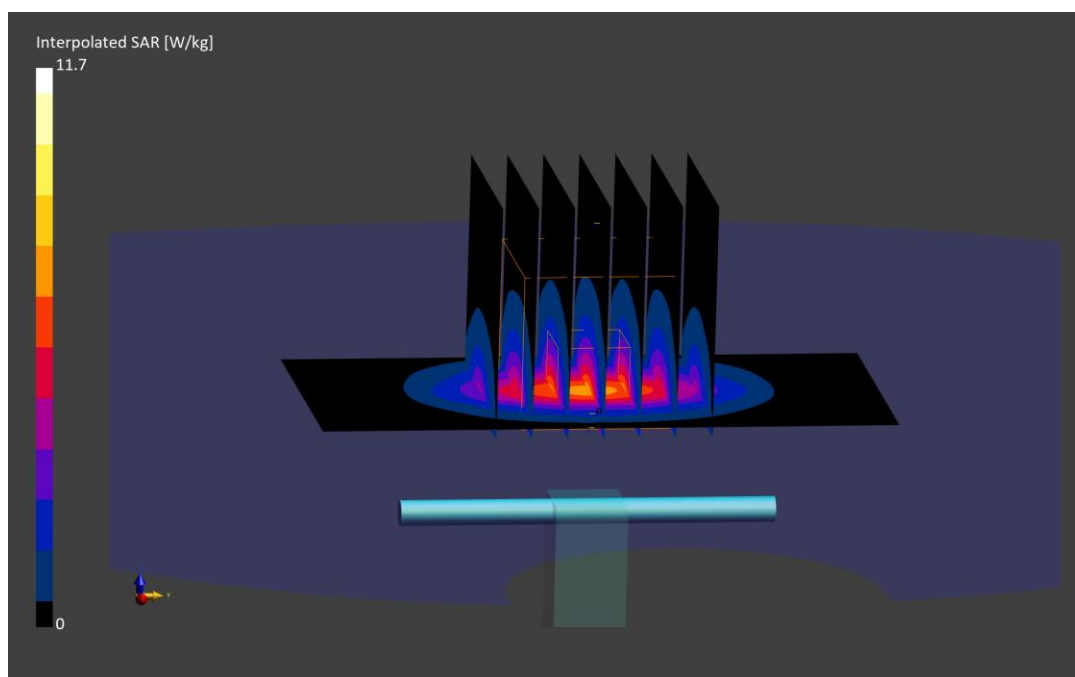

ELEMENT

DUT: Dipole 2450.000 MHz; Type: D2450V2 - SN750

Communication System: UID: 0, CW; Frequency: 2450.000 MHz

Medium: 2450 Head; Medium parameters used:

$f = 2450.000$ MHz; $\text{cond} = 1.81$ S/m; $\text{perm} = 38.1$; $\text{density} = 1000$ kg/m³

Phantom Section: Flat; Space: 10 mm

Test Date: 08/06/2025; Ambient Temp: 24.0°C; Tissue Temp: 22.3°C

Probe: EX3DV4 - SN7552; ConvF:(6.69,7.41,7.22); Calibrated: 2025-05-14

Sensor-Surface: 1.4mm (VMS + 6p)

Electronics: DAE4 Sn1676; Calibrated: 2025-05-13

Phantom: Twin-SAM V8.0; Serial: 1944

Measurement SW: DASY Module SAR V16.4.0.5005

2450.0 MHz System Verification at 20.0 dBm (100 mW)


Area Scan (40.0 x 80.0): Measurement grid: $dx=10.0$ mm, $dy=10.0$ mm

Zoom Scan (30.0 x 30.0 x 31.2): Measurement grid: $dx=5.0$ mm, $dy=5.0$ mm, $dz=1.5$ mm; Graded Ratio: 1.5

Peak SAR (extrapolated) = 10.3 W/kg

SAR(1 g) = 5.03 W/kg

Deviation (1 g) = -5.63%

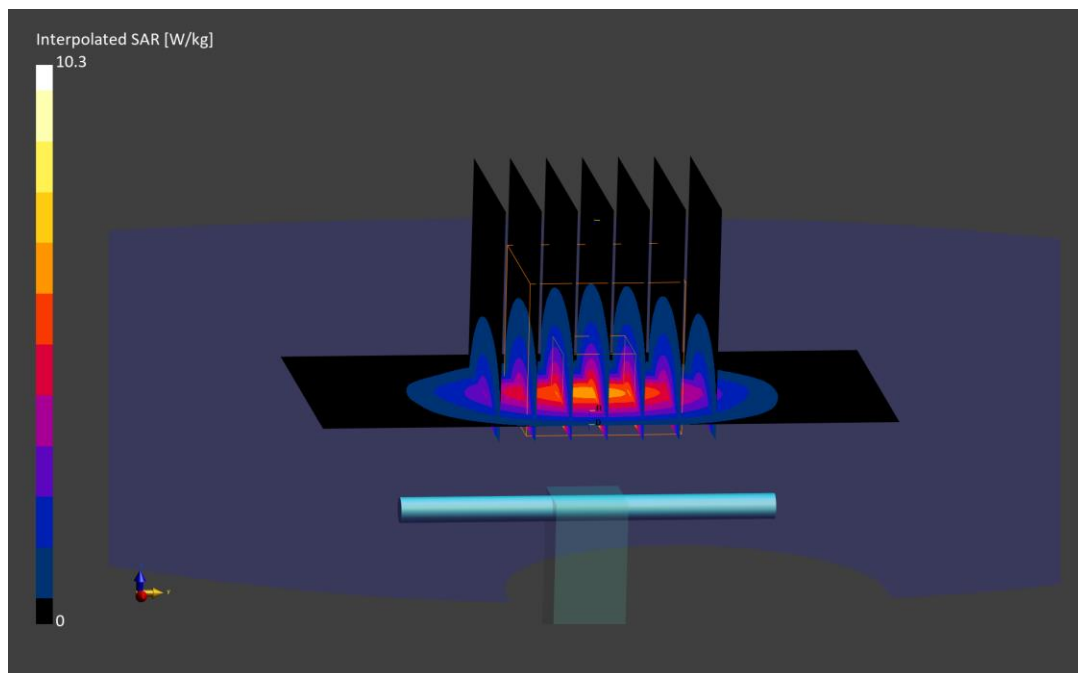

ELEMENT

DUT: Dipole 2600.000 MHz; Type: D2600V2 - SN1042

Communication System: UID: 0, CW; Frequency: 2600.000 MHz
Medium: 2450 Head; Medium parameters used:
 $f = 2600.000$ MHz; $\text{cond} = 1.92$ S/m; $\text{perm} = 37.7$; $\text{density} = 1000$ kg/m³
Phantom Section: Flat; Space: 10 mm

Test Date: 07/28/2025; Ambient Temp: 23.5°C; Tissue Temp: 20.9°C

Probe: EX3DV4 - SN7360; ConvF:(6.89,6.79,7.72); Calibrated: 2025-03-07
Sensor-Surface: 1.4mm (VMS + 6p)
Electronics: DAE4 Sn534; Calibrated: 2025-03-11
Phantom: Twin-SAM V8.0; Serial: 2034
Measurement SW: DASY Module SAR V16.4.0.5005

2600.0 MHz System Verification at 20.0 dBm (100 mW)


Area Scan (40.0 x 80.0): Measurement grid: $dx=10.0$ mm, $dy=10.0$ mm

Zoom Scan (30.0 x 30.0 x 31.2): Measurement grid: $dx=5.0$ mm, $dy=5.0$ mm, $dz=1.5$ mm; Graded Ratio: 1.5

Peak SAR (extrapolated) = 11.8 W/kg

SAR(1 g) = 5.61 W/kg

Deviation (1 g) = 2.19%

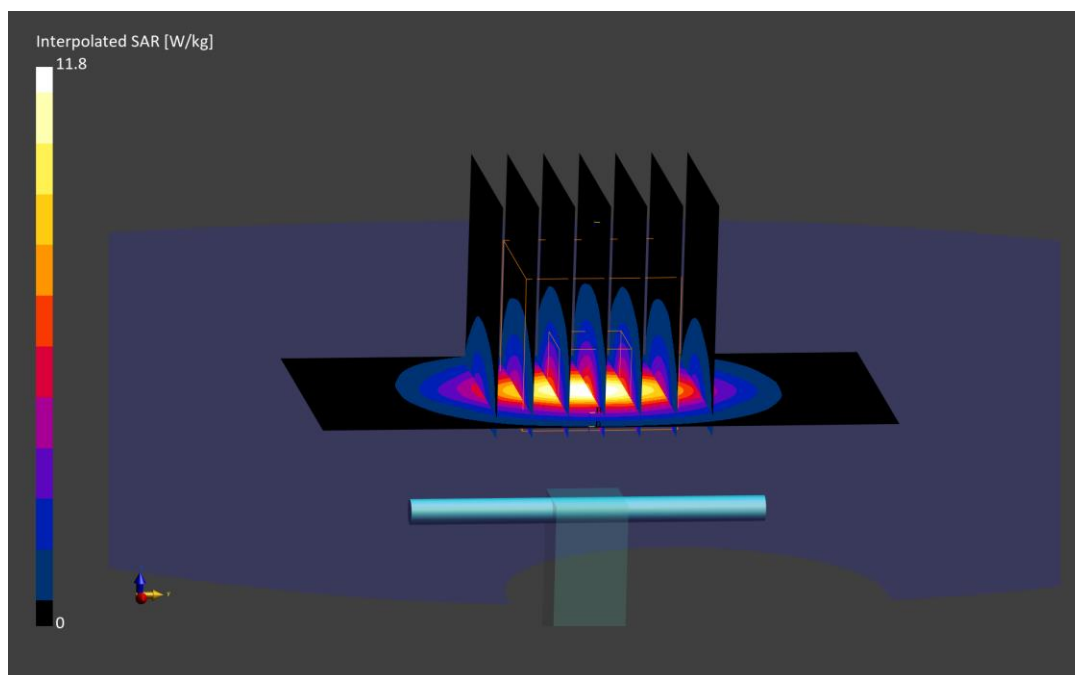

ELEMENT

DUT: Dipole 2600.000 MHz; Type: D2600V2 - SN1042

Communication System: UID: 0, CW; Frequency: 2600.000 MHz
Medium: 2450 Head; Medium parameters used:
 $f = 2600.000$ MHz; $\text{cond} = 1.93$ S/m; $\text{perm} = 37.9$; $\text{density} = 1000$ kg/m³
Phantom Section: Flat; Space: 10 mm

Test Date: 08/06/2025; Ambient Temp: 24.0°C; Tissue Temp: 22.3°C

Probe: EX3DV4 - SN7552; ConvF:(6.68,7.41,7.21); Calibrated: 2025-05-14
Sensor-Surface: 1.4mm (VMS + 6p)
Electronics: DAE4 Sn1676; Calibrated: 2025-05-13
Phantom: Twin-SAM V8.0; Serial: 1944
Measurement SW: DASY Module SAR V16.4.0.5005

2600.0 MHz System Verification at 20.0 dBm (100 mW)

Area Scan (40.0 x 80.0): Measurement grid: $dx=10.0$ mm, $dy=10.0$ mm

Zoom Scan (30.0 x 30.0 x 31.2): Measurement grid: $dx=5.0$ mm, $dy=5.0$ mm, $dz=1.5$ mm; Graded Ratio: 1.5

Peak SAR (extrapolated) = 12.1 W/kg

SAR(1 g) = 5.81 W/kg

Deviation (1 g) = 5.83%

