



Accredited by the Swiss Accreditation Service (SAS)  
The Swiss Accreditation Service is one of the signatories to the EA  
Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: **SCS 0108**

Client **Element**

Certificate No: **D2450V2-855\_Nov22**

## CALIBRATION CERTIFICATE

Object **D2450V2 - SN:855**

Calibration procedure(s) **QA CAL-05.v11**  
**Calibration Procedure for SAR Validation Sources between 0.7-3 GHz**

Calibration date: **November 15, 2022**

✓ **ATM**

**12/16/22**

✓ **YW 12/13/2023**

✓ **YW 11/19/2024**

This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI).  
The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility: environment temperature ( $22 \pm 3$ )°C and humidity < 70%.

Calibration Equipment used (M&TE critical for calibration)

| Primary Standards               | ID #               | Cal Date (Certificate No.)        | Scheduled Calibration  |
|---------------------------------|--------------------|-----------------------------------|------------------------|
| Power meter NRP                 | SN: 104778         | 04-Apr-22 (No. 217-03525/03524)   | Apr-23                 |
| Power sensor NRP-Z91            | SN: 103244         | 04-Apr-22 (No. 217-03524)         | Apr-23                 |
| Power sensor NRP-Z91            | SN: 103245         | 04-Apr-22 (No. 217-03525)         | Apr-23                 |
| Reference 20 dB Attenuator      | SN: BH9394 (20k)   | 04-Apr-22 (No. 217-03527)         | Apr-23                 |
| Type-N mismatch combination     | SN: 310982 / 06327 | 04-Apr-22 (No. 217-03528)         | Apr-23                 |
| Reference Probe EX3DV4          | SN: 7349           | 31-Dec-21 (No. EX3-7349_Dec21)    | Dec-22                 |
| DAE4                            | SN: 601            | 31-Aug-22 (No. DAE4-601_Aug22)    | Aug-23                 |
| Secondary Standards             | ID #               | Check Date (in house)             | Scheduled Check        |
| Power meter E4419B              | SN: GB39512475     | 30-Oct-14 (in house check Oct-22) | In house check: Oct-24 |
| Power sensor HP 8481A           | SN: US37292783     | 07-Oct-15 (in house check Oct-22) | In house check: Oct-24 |
| Power sensor HP 8481A           | SN: MY41093315     | 07-Oct-15 (in house check Oct-22) | In house check: Oct-24 |
| RF generator R&S SMT-06         | SN: 100972         | 15-Jun-15 (in house check Oct-22) | In house check: Oct-24 |
| Network Analyzer Agilent E8358A | SN: US41080477     | 31-Mar-14 (in house check Oct-22) | In house check: Oct-24 |

Calibrated by: **Jeton Kastrati** **Laboratory Technician**

Signature

Approved by: **Sven Kühn** **Technical Manager**

Signature

Issued: November 16, 2022

This calibration certificate shall not be reproduced except in full without written approval of the laboratory.



Accredited by the Swiss Accreditation Service (SAS)

The Swiss Accreditation Service is one of the signatories to the EA  
Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: **SCS 0108**

**Glossary:**

|       |                                 |
|-------|---------------------------------|
| TSL   | tissue simulating liquid        |
| ConvF | sensitivity in TSL / NORM x,y,z |
| N/A   | not applicable or not measured  |

**Calibration is Performed According to the Following Standards:**

- a) IEC/IEEE 62209-1528, "Measurement Procedure For The Assessment Of Specific Absorption Rate Of Human Exposure To Radio Frequency Fields From Hand-Held And Body-Worn Wireless Communication Devices - Part 1528: Human Models, Instrumentation And Procedures (Frequency Range of 4 MHz to 10 GHz)", October 2020.
- b) KDB 865664, "SAR Measurement Requirements for 100 MHz to 6 GHz"

**Additional Documentation:**

- c) DASY System Handbook

**Methods Applied and Interpretation of Parameters:**

- *Measurement Conditions:* Further details are available from the Validation Report at the end of the certificate. All figures stated in the certificate are valid at the frequency indicated.
- *Antenna Parameters with TSL:* The source is mounted in a touch configuration below the center marking of the flat phantom.
- *Return Loss:* This parameter is measured with the source positioned under the liquid filled phantom (as described in the measurement condition clause). The Return Loss ensures low reflected power. No uncertainty required.
- *SAR measured:* SAR measured at the stated antenna input power.
- *SAR normalized:* SAR as measured, normalized to an input power of 1 W at the antenna connector.
- *SAR for nominal TSL parameters:* The measured TSL parameters are used to calculate the nominal SAR result.

The reported uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor  $k=2$ , which for a normal distribution corresponds to a coverage probability of approximately 95%.

## Measurement Conditions

DASY system configuration, as far as not given on page 1.

|                              |                        |             |
|------------------------------|------------------------|-------------|
| DASY Version                 | DASY52                 | V52.10.4    |
| Extrapolation                | Advanced Extrapolation |             |
| Phantom                      | Modular Flat Phantom   |             |
| Distance Dipole Center - TSL | 10 mm                  | with Spacer |
| Zoom Scan Resolution         | dx, dy, dz = 5 mm      |             |
| Frequency                    | 2450 MHz $\pm$ 1 MHz   |             |

## Head TSL parameters

The following parameters and calculations were applied.

|                                         | Temperature         | Permittivity   | Conductivity         |
|-----------------------------------------|---------------------|----------------|----------------------|
| Nominal Head TSL parameters             | 22.0 °C             | 39.2           | 1.80 mho/m           |
| Measured Head TSL parameters            | (22.0 $\pm$ 0.2) °C | 38.4 $\pm$ 6 % | 1.87 mho/m $\pm$ 6 % |
| Head TSL temperature change during test | < 0.5 °C            | ----           | ----                 |

## SAR result with Head TSL

|                                                       |                    |                              |
|-------------------------------------------------------|--------------------|------------------------------|
| SAR averaged over 1 cm <sup>3</sup> (1 g) of Head TSL | Condition          |                              |
| SAR measured                                          | 250 mW input power | 13.4 W/kg                    |
| SAR for nominal Head TSL parameters                   | normalized to 1W   | 52.4 W/kg $\pm$ 17.0 % (k=2) |

|                                                         |                    |                              |
|---------------------------------------------------------|--------------------|------------------------------|
| SAR averaged over 10 cm <sup>3</sup> (10 g) of Head TSL | condition          |                              |
| SAR measured                                            | 250 mW input power | 6.24 W/kg                    |
| SAR for nominal Head TSL parameters                     | normalized to 1W   | 24.6 W/kg $\pm$ 16.5 % (k=2) |

## Body TSL parameters

The following parameters and calculations were applied.

|                                         | Temperature         | Permittivity   | Conductivity         |
|-----------------------------------------|---------------------|----------------|----------------------|
| Nominal Body TSL parameters             | 22.0 °C             | 52.7           | 1.95 mho/m           |
| Measured Body TSL parameters            | (22.0 $\pm$ 0.2) °C | 51.7 $\pm$ 6 % | 2.01 mho/m $\pm$ 6 % |
| Body TSL temperature change during test | < 0.5 °C            | ----           | ----                 |

## SAR result with Body TSL

|                                                       |                    |                              |
|-------------------------------------------------------|--------------------|------------------------------|
| SAR averaged over 1 cm <sup>3</sup> (1 g) of Body TSL | Condition          |                              |
| SAR measured                                          | 250 mW input power | 12.8 W/kg                    |
| SAR for nominal Body TSL parameters                   | normalized to 1W   | 50.2 W/kg $\pm$ 17.0 % (k=2) |

|                                                         |                    |                              |
|---------------------------------------------------------|--------------------|------------------------------|
| SAR averaged over 10 cm <sup>3</sup> (10 g) of Body TSL | condition          |                              |
| SAR measured                                            | 250 mW input power | 6.03 W/kg                    |
| SAR for nominal Body TSL parameters                     | normalized to 1W   | 23.8 W/kg $\pm$ 16.5 % (k=2) |

## Appendix (Additional assessments outside the scope of SCS 0108)

### Antenna Parameters with Head TSL

|                                      |                             |
|--------------------------------------|-----------------------------|
| Impedance, transformed to feed point | $52.5 \Omega + 6.3 j\Omega$ |
| Return Loss                          | - 23.6 dB                   |

### Antenna Parameters with Body TSL

|                                      |                             |
|--------------------------------------|-----------------------------|
| Impedance, transformed to feed point | $48.9 \Omega + 7.9 j\Omega$ |
| Return Loss                          | - 21.9 dB                   |

### General Antenna Parameters and Design

|                                  |          |
|----------------------------------|----------|
| Electrical Delay (one direction) | 1.157 ns |
|----------------------------------|----------|

After long term use with 100W radiated power, only a slight warming of the dipole near the feedpoint can be measured.

The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals. On some of the dipoles, small end caps are added to the dipole arms in order to improve matching when loaded according to the position as explained in the "Measurement Conditions" paragraph. The SAR data are not affected by this change. The overall dipole length is still according to the Standard.

No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feedpoint may be damaged.

### Additional EUT Data

|                 |       |
|-----------------|-------|
| Manufactured by | SPEAG |
|-----------------|-------|

## DASY5 Validation Report for Head TSL

Date: 15.11.2022

Test Laboratory: SPEAG, Zurich, Switzerland

**DUT: Dipole 2450 MHz; Type: D2450V2; Serial: D2450V2 - SN:855**

Communication System: UID 0 - CW; Frequency: 2450 MHz

Medium parameters used:  $f = 2450$  MHz;  $\sigma = 1.87$  S/m;  $\epsilon_r = 38.4$ ;  $\rho = 1000$  kg/m<sup>3</sup>

Phantom section: Flat Section

Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2011)

DASY52 Configuration:

- Probe: EX3DV4 - SN7349; ConvF(7.96, 7.96, 7.96) @ 2450 MHz; Calibrated: 31.12.2021
- Sensor-Surface: 1.4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn601; Calibrated: 31.08.2022
- Phantom: Flat Phantom 5.0 (front); Type: QD 000 P50 AA; Serial: 1001
- DASY52 52.10.4(1535); SEMCAD X 14.6.14(7501)

### Dipole Calibration for Head Tissue/Pin=250 mW, d=10mm/Zoom Scan (7x7x7)/Cube 0:

Measurement grid: dx=5mm, dy=5mm, dz=5mm

Reference Value = 116.1 V/m; Power Drift = 0.01 dB


Peak SAR (extrapolated) = 26.2 W/kg

**SAR(1 g) = 13.4 W/kg; SAR(10 g) = 6.24 W/kg**

Smallest distance from peaks to all points 3 dB below = 9 mm


Ratio of SAR at M2 to SAR at M1 = 51.1%

Maximum value of SAR (measured) = 22.0 W/kg

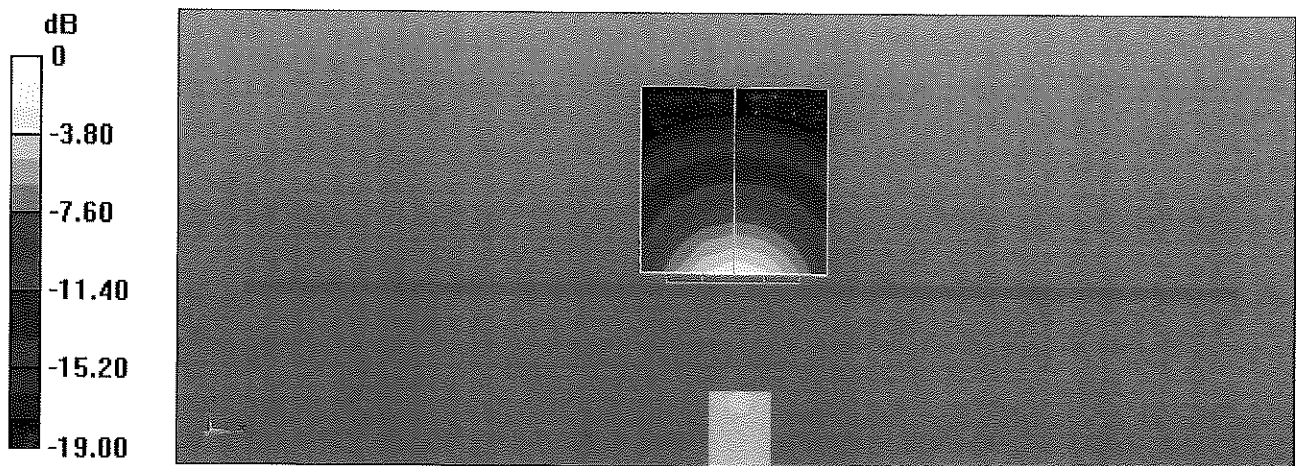

0 dB = 22.0 W/kg = 13.42 dBW/kg

# Impedance Measurement Plot for Head TSL

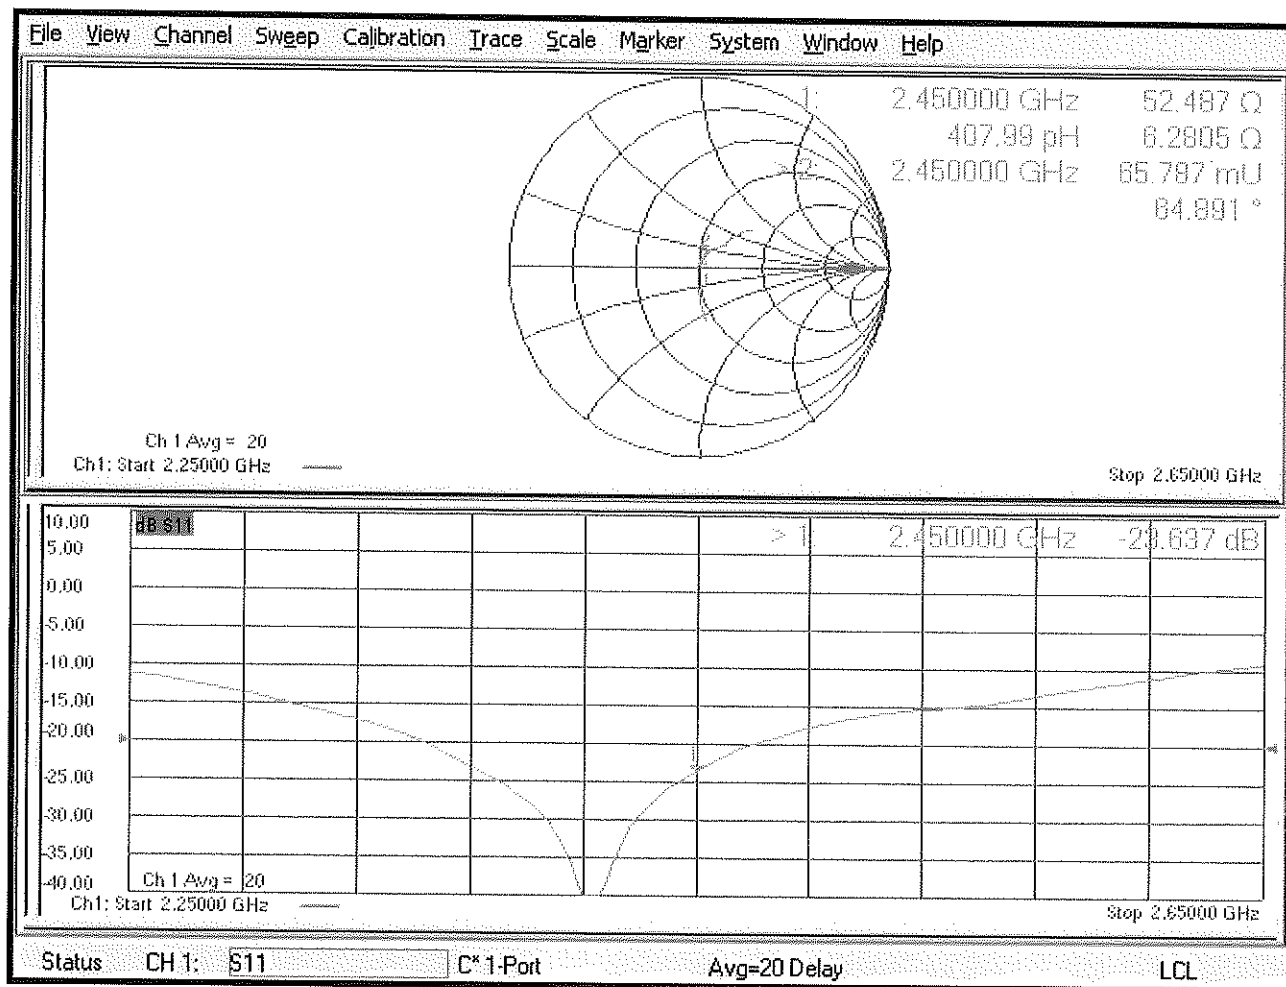

## DASY5 Validation Report for Body TSL

Date: 15.11.2022

Test Laboratory: SPEAG, Zurich, Switzerland

**DUT: Dipole 2450 MHz; Type: D2450V2; Serial: D2450V2 - SN:855**

Communication System: UID 0 - CW; Frequency: 2450 MHz

Medium parameters used:  $f = 2450$  MHz;  $\sigma = 2.01$  S/m;  $\epsilon_r = 51.7$ ;  $\rho = 1000$  kg/m<sup>3</sup>

Phantom section: Flat Section

Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2011)

DASY52 Configuration:

- Probe: EX3DV4 - SN7349; ConvF(8.12, 8.12, 8.12) @ 2450 MHz; Calibrated: 31.12.2021
- Sensor-Surface: 1.4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn601; Calibrated: 31.08.2022
- Phantom: Flat Phantom 5.0 (back); Type: QD 000 P50 AA; Serial: 1002
- DASY52 52.10.4(1535); SEMCAD X 14.6.14(7501)

### Dipole Calibration for Body Tissue/ $P_{in}=250$ mW, $d=10$ mm 2/Zoom Scan (7x7x7)/Cube 0:

Measurement grid:  $dx=5$ mm,  $dy=5$ mm,  $dz=5$ mm

Reference Value = 108.4 V/m; Power Drift = -0.04 dB


Peak SAR (extrapolated) = 24.1 W/kg

**SAR(1 g) = 12.8 W/kg; SAR(10 g) = 6.03 W/kg**

Smallest distance from peaks to all points 3 dB below = 8.9 mm


Ratio of SAR at M2 to SAR at M1 = 53.7%

Maximum value of SAR (measured) = 20.4 W/kg

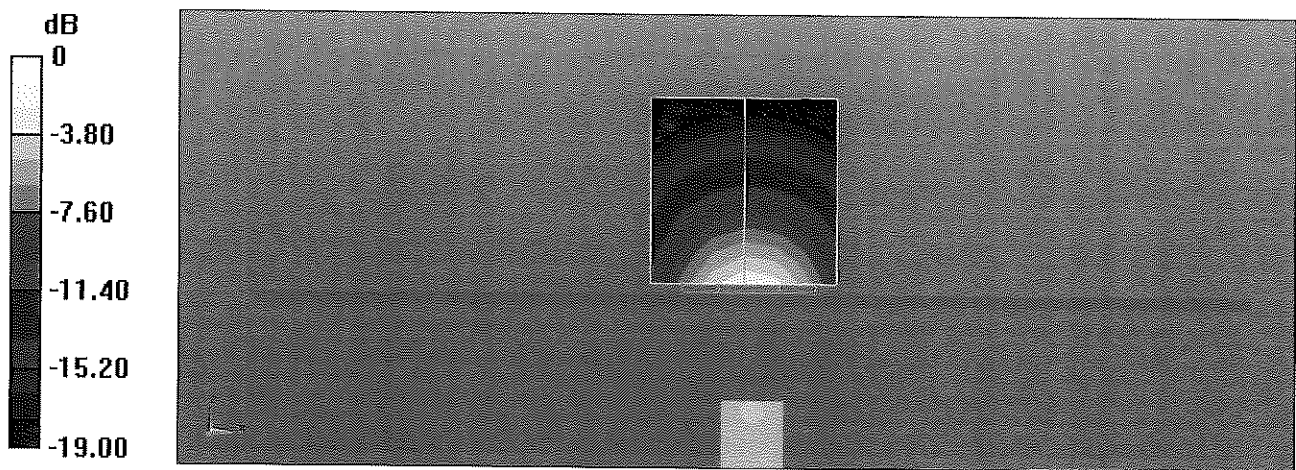

0 dB = 20.4 W/kg = 13.10 dBW/kg

## Impedance Measurement Plot for Body TSL

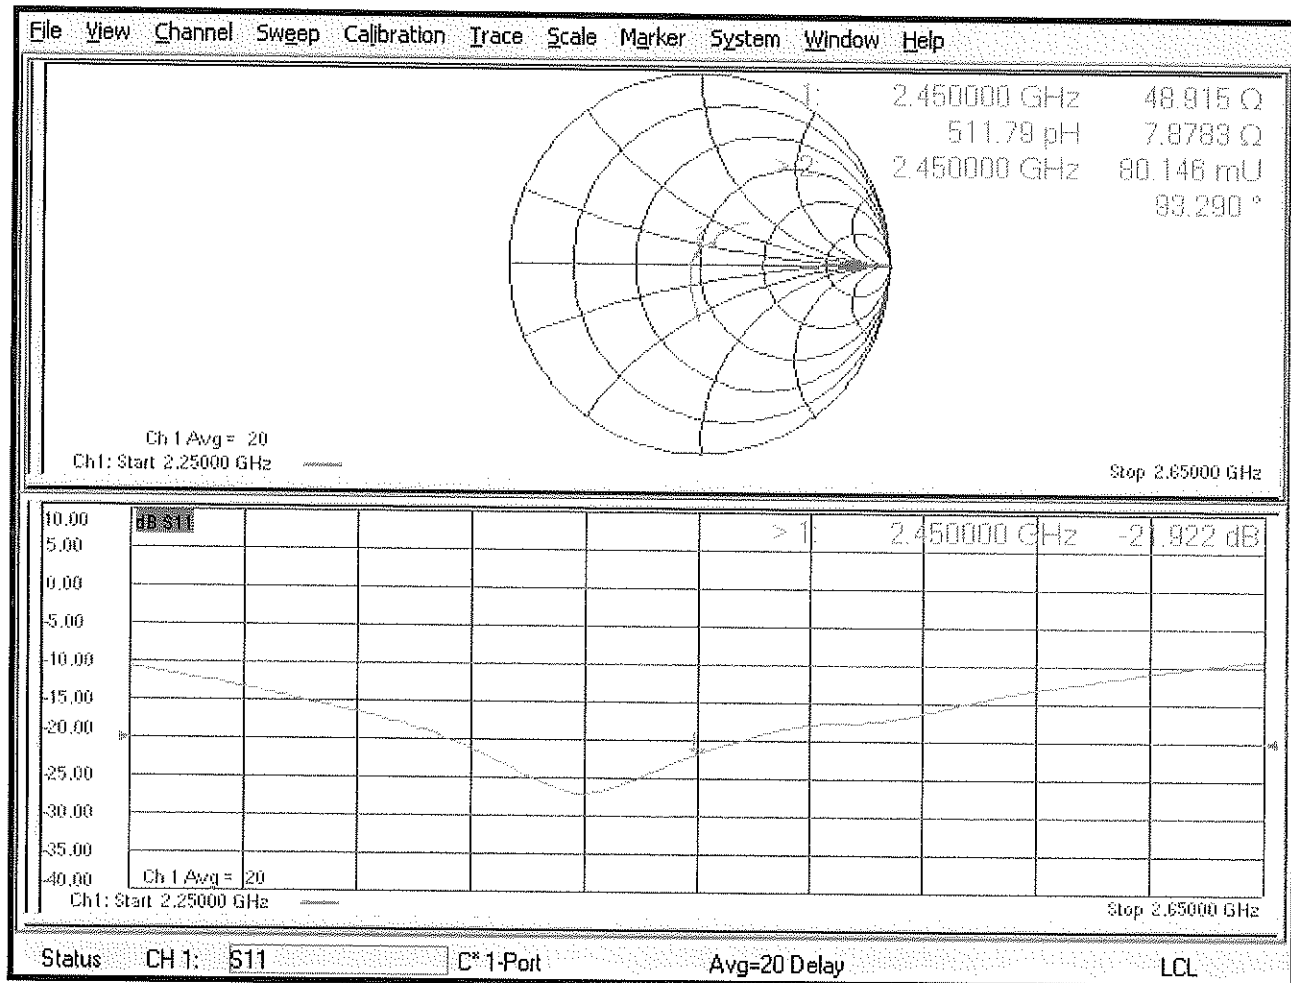

## Certification of Calibration

Object: D2450V2 – SN: 855

Calibration procedure(s): Procedure for Calibration Extension for SAR Dipoles.

Extension Calibration date: November 15, 2023

Description: SAR Validation Dipole at 2450 MHz.

### Calibration Equipment used:

| Manufacturer       | Model         | Description                         | Cal Date   | Cal Interval | Cal Due    | Serial Number |
|--------------------|---------------|-------------------------------------|------------|--------------|------------|---------------|
| Agilent            | 8753ES        | S-Parameter Vector Network Analyzer | 6/2/2023   | Annual       | 6/12/2024  | MY40003841    |
| Agilent            | E4438C        | ESG Vector Signal Generator         | 4/25/2023  | Annual       | 4/25/2024  | US41460739    |
| Amplifier Research | 15S1G6        | Amplifier                           | CBT        | N/A          | CBT        | 343972        |
| Rohde & Schwarz    | NRX           | Power Meter                         | 1/11/2023  | Annual       | 1/11/2024  | 102583        |
| Rohde & Schwarz    | NRP-Z81       | Wide Band Power Sensor              | 1/19/2023  | Annual       | 1/19/2024  | 106563        |
| Rohde & Schwarz    | NRP-Z81       | Wide Band Power Sensor              | 1/11/2023  | Annual       | 1/11/2024  | 106564        |
| Traceable          | 4040 90080-06 | Therm./ Clock/ Humidity Monitor     | 5/11/2022  | Biennial     | 5/11/2024  | 221514974     |
| Control Company    | 4353          | Ultra Long Stem Thermometer         | 10/24/2023 | Annual       | 10/24/2024 | 200645916     |
| Agilent            | 85033E        | 3.5mm Standard Calibration Kit      | 7/18/2023  | Annual       | 7/18/2024  | MY53402352    |
| Mini-Circuits      | VL6-6000+     | Low Pass Filter DC to 6000 MHz      | CBT        | N/A          | CBT        | N/A           |
| Narda              | 4772-3        | Attenuator (3dB)                    | CBT        | N/A          | CBT        | 9406          |
| Mini-Circuits      | ZHDC-16-63-S+ | 50-6000MHz Bidirectional Coupler    | CBT        | N/A          | CBT        | N/A           |
| Pasternack         | NC-100        | Torque Wrench                       | 12/5/2022  | Biennial     | 12/5/2024  | N/A           |
| SPEAG              | DAK-3.5       | Dielectric Assessment Kit           | 5/9/2023   | Annual       | 5/9/2024   | 1070          |
| SPEAG              | EX3DV4        | SAR Probe                           | 11/9/2023  | Annual       | 11/9/2024  | 7639          |
| SPEAG              | DAE4          | Dasy Data Acquisition Electronics   | 11/14/2023 | Annual       | 11/14/2024 | 1403          |

Measurement Uncertainty =  $\pm 23\%$  (k=2)

|                | Name            | Function                   | Signature                                                                             |
|----------------|-----------------|----------------------------|---------------------------------------------------------------------------------------|
| Calibrated By: | Arturo Oliveros | Compliance Engineer        |  |
| Approved By:   | Greg Snyder     | Executive VP of Operations |  |

# DIPOLE CALIBRATION EXTENSION



Per KDB 865664 D01, calibration intervals of up to three years may be considered for reference dipoles when it is demonstrated that the SAR target, impedance and return loss of a dipole have remained stable according to the following requirements:

1. The measured SAR does not deviate more than 10% from the target on the calibration certificate.
2. The return-loss does not deviate more than 20% from the previous measurement and meets the required 20dB minimum return-loss requirement.
3. The measurement of real or imaginary parts of impedance does not deviate more than 5Ω from the previous measurement.

The following dipole was checked to pass the above 3 requirements to have 2-year calibration period from the calibration date:

| Calibration Date | Extension Date | Certificate Electrical Delay (ns) | Certificate SAR Target Head (1g) W/kg @ 20.0 dBm | Measured Head SAR (1g) W/kg @ 20.0 dBm | Deviation 1g (%) | Certificate SAR Target Head (10g) W/kg @ 20.0 dBm | Measured Head SAR (10g) W/kg @ 20.0 dBm | Deviation 10g (%) | Certificate Impedance Head (Ohm) Real | Measured Impedance Head (Ohm) Real | Difference (Ohm) Real | Certificate Impedance Head (Ohm) Imaginary | Measured Impedance Head (Ohm) Imaginary | Difference (Ohm) Imaginary | Certificate Return Loss Head (dB) | Measured Return Loss Head (dB) | Deviation (%) |
|------------------|----------------|-----------------------------------|--------------------------------------------------|----------------------------------------|------------------|---------------------------------------------------|-----------------------------------------|-------------------|---------------------------------------|------------------------------------|-----------------------|--------------------------------------------|-----------------------------------------|----------------------------|-----------------------------------|--------------------------------|---------------|
| 11/15/2022       | 11/15/2023     | 1.157                             | 5.24                                             | 5.13                                   | -2.10%           | 2.46                                              | 2.38                                    | -3.25%            | 52.5                                  | 53.9                               | 1.4                   | 6.3                                        | 2.9                                     | 3.4                        | -23.6                             | -25.4                          | -7.70%        |

Impedance & Return-Loss Measurement Plot for Head TSL

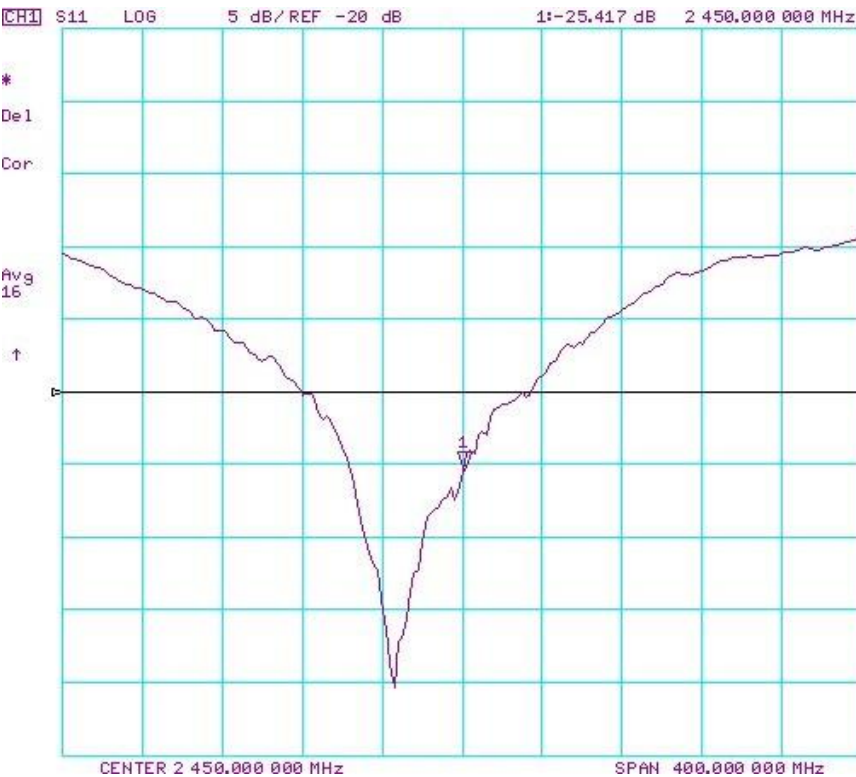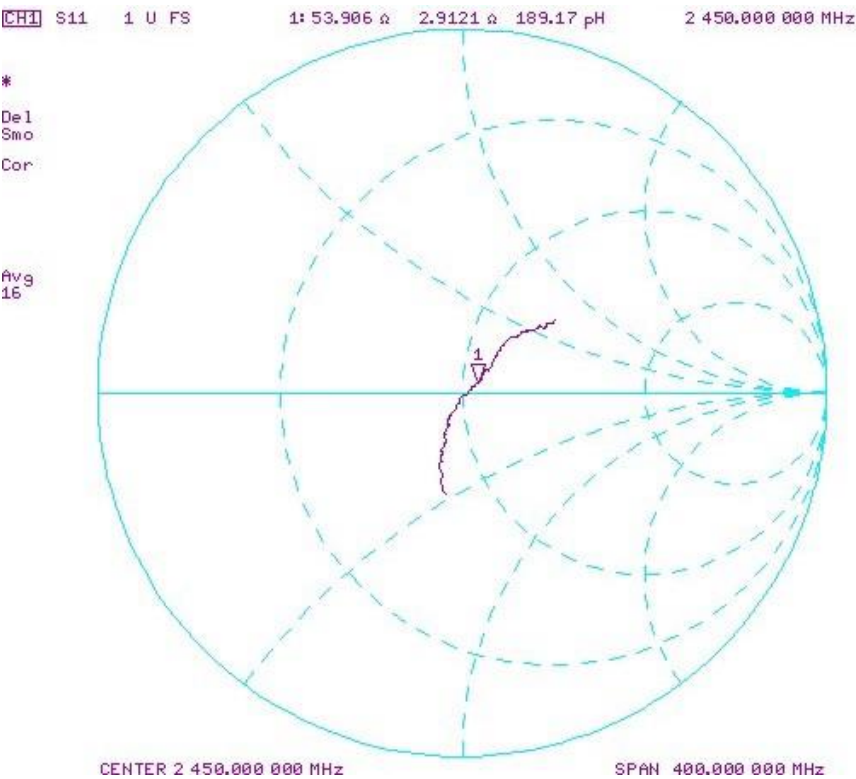

## Certification of Calibration

Object: D2450V2 – SN: 855

Calibration procedure(s): Procedure for Calibration Extension for SAR Dipoles.



Extension Calibration date: November 15, 2024

Description: SAR Validation Dipole at 2450 MHz.

### Calibration Equipment used:

| Manufacturer       | Model         | Description                       | Cal Date  | Cal Interval | Cal Due   | Serial Number |
|--------------------|---------------|-----------------------------------|-----------|--------------|-----------|---------------|
| Hewlett Packard    | 8753E         | RF Vector Network Analyzer        | 5/21/2024 | Annual       | 5/21/2025 | US38161081    |
| Agilent            | E4438C        | ESG Vector Signal Generator       | 5/19/2024 | Annual       | 5/19/2025 | US41460739    |
| Amplifier Research | 15S1G6        | Amplifier                         | CBT       | N/A          | CBT       | 343972        |
| Anritsu            | ML2496A       | Power Meter                       | 7/15/2024 | Annual       | 7/15/2025 | 1138001       |
| Anritsu            | MA2411B       | Pulse Power Sensor                | 7/10/2024 | Annual       | 7/10/2025 | 1126066       |
| Anritsu            | MA2411B       | Pulse Power Sensor                | 7/1/2024  | Annual       | 7/1/2025  | 1911105       |
| Traceable          | 4040 90080-06 | Therm./ Clock/ Humidity Monitor   | 1/15/2024 | Annual       | 1/15/2025 | 160574418     |
| Control Company    | 4352          | Ultra Long Stem Thermometer       | 1/15/2024 | Annual       | 1/15/2025 | 160508097     |
| Agilent            | 85033E        | 3.5mm Standard Calibration Kit    | 7/31/2024 | Annual       | 7/31/2025 | MY53402352    |
| Mini-Circuits      | VLF-6000+     | Low Pass Filter DC to 6000 MHz    | CBT       | N/A          | CBT       | N/A           |
| Narda              | 4772-3        | Attenuator (3dB)                  | CBT       | N/A          | CBT       | 9406          |
| Mini-Circuits      | ZHDC-16-63-S+ | 50-6000MHz Bidirectional Coupler  | CBT       | N/A          | CBT       | N/A           |
| Pasternack         | NC-100        | Torque Wrench                     | 12/5/2022 | Biennial     | 12/5/2024 | N/A           |
| SPEAG              | DAK-3.5       | Dielectric Assessment Kit         | 5/14/2024 | Annual       | 5/14/2025 | 1070          |
| SPEAG              | EX3DV4        | SAR Probe                         | 9/9/2024  | Annual       | 9/9/2025  | 7639          |
| SPEAG              | DAE4          | Dasy Data Acquisition Electronics | 9/4/2024  | Annual       | 9/4/2025  | 1403          |

Measurement Uncertainty =  $\pm 23\%$  (k=2)

|                | Name            | Function                   | Signature                                                                             |
|----------------|-----------------|----------------------------|---------------------------------------------------------------------------------------|
| Calibrated By: | Arturo Oliveros | Compliance Engineer        |  |
| Approved By:   | Greg Snyder     | Executive VP of Operations |  |

# DIPOLE CALIBRATION EXTENSION

Per KDB 865664 D01, calibration intervals of up to three years may be considered for reference dipoles when it is demonstrated that the SAR target, impedance and return loss of a dipole have remained stable according to the following requirements:

1. The measured SAR does not deviate more than 10% from the target on the calibration certificate.
2. The return-loss does not deviate more than 20% from the previous measurement and meets the required 20dB minimum return-loss requirement.
3. The measurement of real or imaginary parts of impedance does not deviate more than 5Ω from the previous measurement.


The following dipole was checked to pass the above 3 requirements to have 3-year calibration period from the calibration date:

| Calibration Date | Extension Date | Certificate Electrical Delay (ns) | Certificate SAR Target Head (1g) W/kg @ 20.0 dBm | Measured Head SAR (1g) W/kg @ 20.0 dBm | Deviation 1g (%) | Certificate SAR Target Head (10g) W/kg @ 20.0 dBm | Measured Head SAR (10g) W/kg @ 20.0 dBm | Deviation 10g (%) | Certificate Impedance Head (Ohm) Real | Measured Impedance Head (Ohm) Real | Difference (Ohm) Real | Certificate Impedance Head (Ohm) Imaginary | Measured Impedance Head (Ohm) Imaginary | Difference (Ohm) Imaginary | Certificate Return Loss Head (dB) | Measured Return Loss Head (dB) | Deviation (%) |
|------------------|----------------|-----------------------------------|--------------------------------------------------|----------------------------------------|------------------|---------------------------------------------------|-----------------------------------------|-------------------|---------------------------------------|------------------------------------|-----------------------|--------------------------------------------|-----------------------------------------|----------------------------|-----------------------------------|--------------------------------|---------------|
| 11/15/2022       | 11/15/2024     | 1.157                             | 5.24                                             | 5.31                                   | 1.34%            | 2.46                                              | 2.49                                    | 1.22%             | 52.5                                  | 50.2                               | 2.3                   | 6.3                                        | 3.5                                     | 2.8                        | -23.6                             | -27.1                          | -14.80%       |

Impedance & Return-Loss Measurement Plot for Head TSL


[CH1] S11 1 U FS 1: 50.164  $\Omega$  3.4980  $\Omega$  227.24 pF 2 450.000 000 MHz

\*  
De1  
Cor  
  
↑

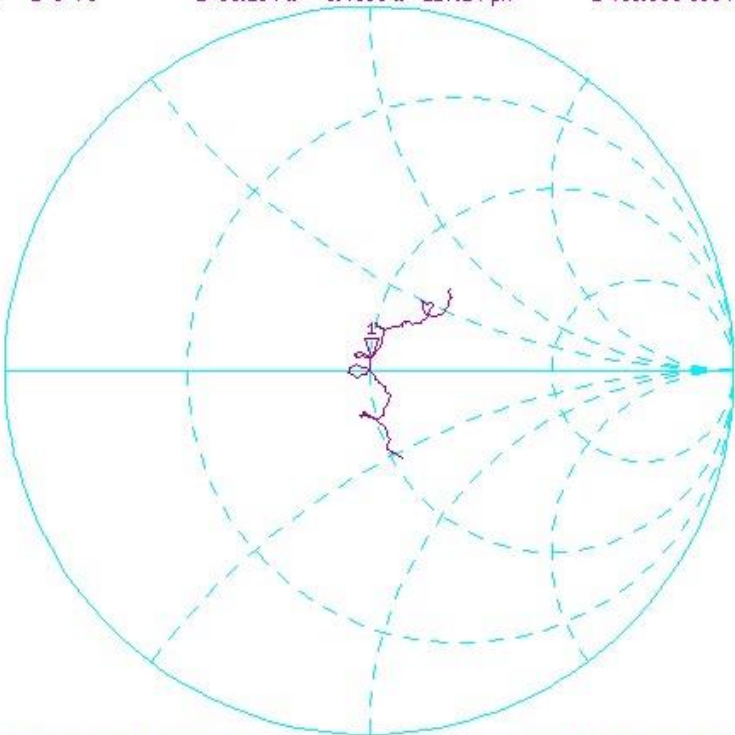

[CH1] S11 LOG 5 dB/REF -20 dB 1:-27.092 dB 2 450.000 000 MHz  
CENTER 2 450.000 000 MHz SPAN 400.000 000 MHz

\*  
De1  
Cor  
  
↑

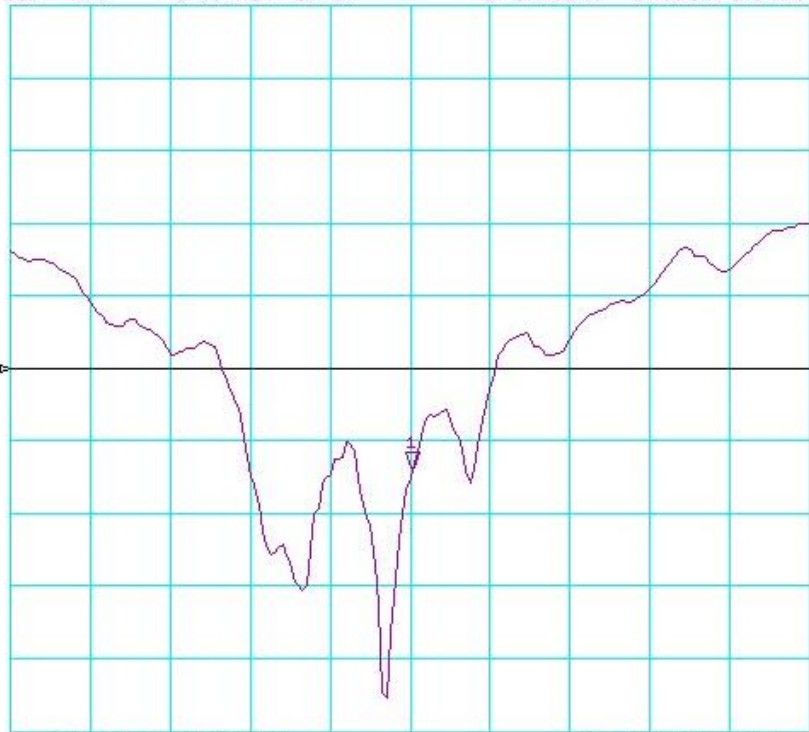

Object:

D2450V2 – SN: 855

Date Issued:

11/15/2024



Accredited by the Swiss Accreditation Service (SAS)  
 The Swiss Accreditation Service is one of the signatories to the EA  
 Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: **SCS 0108**

Client

**Element**  
**Morgan Hill, USA**

Certificate No.

**D2600V2-1042\_May25**

## CALIBRATION CERTIFICATE

Object **D2600V2 - SN: 1042**

Calibration procedure(s) **QA CAL-05.v12**  
**Calibration Procedure for SAR Validation Sources between 0.7 - 3 GHz**

Calibration date **May 7, 2025**

This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI).  
 The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility: environment temperature  $(22 \pm 3)^\circ\text{C}$  and humidity  $< 70\%$ .

Calibration Equipment used (M&TE critical for calibration)

| Primary Standards           | ID         | Cal Date (Certificate No.)             | Scheduled Cal |
|-----------------------------|------------|----------------------------------------|---------------|
| Power Sensor R&S NRP-33T    | SN: 100967 | 26-Mar-25 (No. 217-04290)              | Mar-26        |
| Power Sensor R&S NRP18A     | SN: 101859 | 06-Feb-25 (No. 4030A315009541)         | Feb-26        |
| Spectrum Analyzer R&S FSV40 | SN: 101832 | 29-Jan-25 (No. 4030A315009658)         | Jan-26        |
| 3.5mm mismatch combination  | SN: 1152   | 24-Mar-25 (No. 217-04293)              | Mar-26        |
| OCP DAK-12                  | SN: 1016   | 24-Sept-24 (No. OCP-DAK12-1016_Sep24)  | Sep-25        |
| OCP DAK-3.5                 | SN: 1249   | 23-Sept-24 (No. OCP-DAK3.5-1249_Sep24) | Sep-25        |
| Reference Probe EX3DV4      | SN: 7349   | 10-Jan-25 (No. EX3-7349_Jan25)         | Jan-26        |
| DAE4ip                      | SN: 1836   | 17-Apr-25 (No. DAE4ip-1836_Apr25)      | Apr-26        |

| Secondary Standards          | ID         | Check Date (in house)                      | Scheduled Check |
|------------------------------|------------|--------------------------------------------|-----------------|
| ACAD Setup 1                 | SN: 1000   | 28-May-24 (No. 675-ACAD_Source_Box-240528) | May-25          |
| Signal Generator R&S SMB100A | SN: 182081 | 28-May-24 (No. 675-CAL16-S4588-240528)     | May-25          |
| Mismatch; SMA                | SN: 1102   | 22-May-24 (No. 675-Mismatch_SMA-240522)    | May-25          |

|               | Name         | Function              | Signature |
|---------------|--------------|-----------------------|-----------|
| Calibrated by | Leif Klysner | Laboratory Technician |           |
| Approved by   | Sven Kühn    | Technical Manager     |           |

Issued: May 7, 2025

This calibration certificate shall not be reproduced except in full without written approval of the laboratory.



Accredited by the Swiss Accreditation Service (SAS)  
The Swiss Accreditation Service is one of the signatories to the EA  
Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: **SCS 0108**

## Glossary

TSL tissue simulating liquid  
ConvF sensitivity in TSL / NORM x,y,z  
N/A not applicable or not measured

## Calibration is Performed According to the Following Standards

- IEC/IEEE 62209-1528, "Measurement Procedure For The Assessment Of Specific Absorption Rate Of Human Exposure To Radio Frequency Fields From Hand-Held And Body-Worn Wireless Communication Devices - Part 1528: Human Models, Instrumentation And Procedures (Frequency Range of 4 MHz to 10 GHz)", October 2020.
- KDB 865664, "SAR Measurement Requirements for 100 MHz to 6 GHz"

## Additional Documentation

- DASY System Handbook

## Methods Applied and Interpretation of Parameters

- *Measurement Conditions*: Further details are available from the Validation Report at the end of the certificate. All figures stated in the certificate are valid at the frequency indicated.
- *Antenna Parameters with TSL*: The dipole is mounted with the spacer to position its feed point exactly below the center marking of the flat phantom section, with the arms oriented parallel to the body axis.
- *Feed Point Impedance and Return Loss*: These parameters are measured with the dipole positioned under the liquid filled phantom. The impedance stated is transformed from the measurement at the SMA connector to the feed point. The Return Loss ensures low reflected power. No uncertainty required.
- *Electrical Delay*: One-way delay between the SMA connector and the antenna feed point. No uncertainty required.
- *SAR measured*: SAR measured at the stated antenna input power.
- *SAR normalized*: SAR as measured, normalized to an input power of 1 W at the antenna connector.
- *SAR for nominal TSL parameters*: The measured TSL parameters are used to calculate the nominal SAR result.

The reported uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor  $k=2$ , which for a normal distribution corresponds to a coverage probability of approximately 95%.

## Measurement Conditions

DASY system configuration, as far as not given on page 1.

|                                     |                          |                                     |
|-------------------------------------|--------------------------|-------------------------------------|
| <b>DASY Version</b>                 | DASY8 Module SAR         | 16.4.0                              |
| <b>Extrapolation</b>                | Advanced Extrapolation   |                                     |
| <b>Phantom</b>                      | Modular Flat Phantom     |                                     |
| <b>Distance Dipole Center - TSL</b> | 10 mm                    | with spacer                         |
| <b>Zoom Scan Resolution</b>         | dx, dy = 5mm, dz = 1.5mm | Graded Ratio = 1.5 mm (Z direction) |
| <b>Frequency</b>                    | 2600MHz $\pm$ 1MHz       |                                     |

## HSL parameters at 2600 MHz

The following parameters and calculations were applied.

|                                           | Temperature        | Permittivity  | Conductivity        |
|-------------------------------------------|--------------------|---------------|---------------------|
| <b>Nominal HSL parameters</b>             | 22.0 °C            | 39.0          | 1.96 mho/m          |
| <b>Measured HSL parameters</b>            | (22.0 $\pm$ 0.2)°C | 37.3 $\pm$ 6% | 2.00 mho/m $\pm$ 6% |
| <b>HSL temperature change during test</b> | < 0.5 °C           |               |                     |

## SAR result with HSL at 2600 MHz

| <b>SAR averaged over 1 cm<sup>3</sup> (1 g) of HSL</b> | Condition          |                               |
|--------------------------------------------------------|--------------------|-------------------------------|
| SAR for nominal HSL parameters                         | 24 dBm input power | 13.8 W/kg                     |
| SAR for nominal HSL parameters                         | normalized to 1W   | 54.9 W/kg $\pm$ 17.0% (k = 2) |

| <b>SAR averaged over 10 cm<sup>3</sup> (10 g) of HSL</b> | Condition          |                               |
|----------------------------------------------------------|--------------------|-------------------------------|
| SAR for nominal HSL parameters                           | 24 dBm input power | 6.16 W/kg                     |
| SAR for nominal HSL parameters                           | normalized to 1W   | 24.5 W/kg $\pm$ 16.5% (k = 2) |

**MSL parameters at 2600 MHz**

The following parameters and calculations were applied.

|                                    | Temperature   | Permittivity | Conductivity   |
|------------------------------------|---------------|--------------|----------------|
| Nominal MSL parameters             | 22.0 °C       | 52.5         | 2.16 mho/m     |
| Measured MSL parameters            | (22.0 ±0.2)°C | 51.6 ±6%     | 2.20 mho/m ±6% |
| MSL temperature change during test | < 0.5 °C      |              |                |

**SAR result with MSL at 2600 MHz**

| SAR averaged over 1 cm <sup>3</sup> (1 g) of MSL | Condition          |                          |
|--------------------------------------------------|--------------------|--------------------------|
| SAR for nominal MSL parameters                   | 24 dBm input power | 13.4 W/kg                |
| SAR for nominal MSL parameters                   | normalized to 1W   | 53.3 W/kg ±17.0% (k = 2) |

| SAR averaged over 10 cm <sup>3</sup> (10 g) of MSL | Condition          |                          |
|----------------------------------------------------|--------------------|--------------------------|
| SAR for nominal MSL parameters                     | 24 dBm input power | 6.03 W/kg                |
| SAR for nominal MSL parameters                     | normalized to 1W   | 24.0 W/kg ±16.5% (k = 2) |

**Appendix (Additional assessments outside the scope of SCS 0108)****Antenna Parameters with HSL at 2600 MHz**

|             |                                |
|-------------|--------------------------------|
| Impedance   | 48.1 $\Omega$ – 9.3 j $\Omega$ |
| Return Loss | -20.4 dB                       |

**Antenna Parameters with MSL at 2600 MHz**

|             |                                |
|-------------|--------------------------------|
| Impedance   | 44.3 $\Omega$ – 7.4 j $\Omega$ |
| Return Loss | -20.1 dB                       |

**General Antenna Parameters and Design**

|                                  |         |
|----------------------------------|---------|
| Electrical Delay (one direction) | 1.15 ns |
|----------------------------------|---------|

After long term use with 100W radiated power, only a slight warming of the dipole near the feedpoint can be measured. The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals. On some of the dipoles, small end caps are added to the dipole arms in order to improve matching when loaded according to the position as explained in the "Measurement Conditions" paragraph. The SAR data are not affected by this change. The overall dipole length is still according to the Standard. No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feedpoint may be damaged.

**Additional EUT Data**

|                 |       |
|-----------------|-------|
| Manufactured by | SPEAG |
|-----------------|-------|

System Performance Check Report

Summary

| Dipole           | Frequency [MHz] | TSL | Power [dBm] |
|------------------|-----------------|-----|-------------|
| D2600V2 - SN1042 | 2600            | HSL | 24          |

Exposure Conditions

| Phantom Section, TSL | Test Distance [mm] | Band | Group, UID | Frequency [MHz], Channel Number | Conversion Factor | TSL Conductivity [S/m] | TSL Permittivity |
|----------------------|--------------------|------|------------|---------------------------------|-------------------|------------------------|------------------|
| Flat                 | 10                 |      | CW, 0--    | 2600, 0                         | 7.26              | 2.00                   | 37.3             |

Hardware Setup

| Phantom         | TSL, Measured Date | Probe, Calibration Date     | DAE, Calibration Date     |
|-----------------|--------------------|-----------------------------|---------------------------|
| MFP V8.0 Center | HSL, 2025-05-07    | EX3DV4 - SN7349, 2025-01-10 | DAE4lp Sn1836, 2025-04-17 |

Scans Setup

|                     | Zoom Scan       |
|---------------------|-----------------|
| Grid Extents [mm]   | 30 x 30 x 30    |
| Grid Steps [mm]     | 5.0 x 5.0 x 1.5 |
| Sensor Surface [mm] | 1.4             |
| Graded Grid         | Yes             |
| Grading Ratio       | 1.5             |
| MAIA                | N/A             |
| Surface Detection   | VMS + 6p        |
| Scan Method         | Measured        |


Measurement Results

|                     | Zoom Scan           |
|---------------------|---------------------|
| Date                | 2025-05-07          |
| psSAR1g [W/Kg]      | 13.8                |
| psSAR10g [W/Kg]     | 6.16                |
| Power Drift [dB]    | 0.01                |
| Power Scaling       | Disabled            |
| Scaling Factor [dB] |                     |
| TSL Correction      | Positive / Negative |



0 dB = 30.3 W/Kg

## Impedance Measurement Plot for HSL

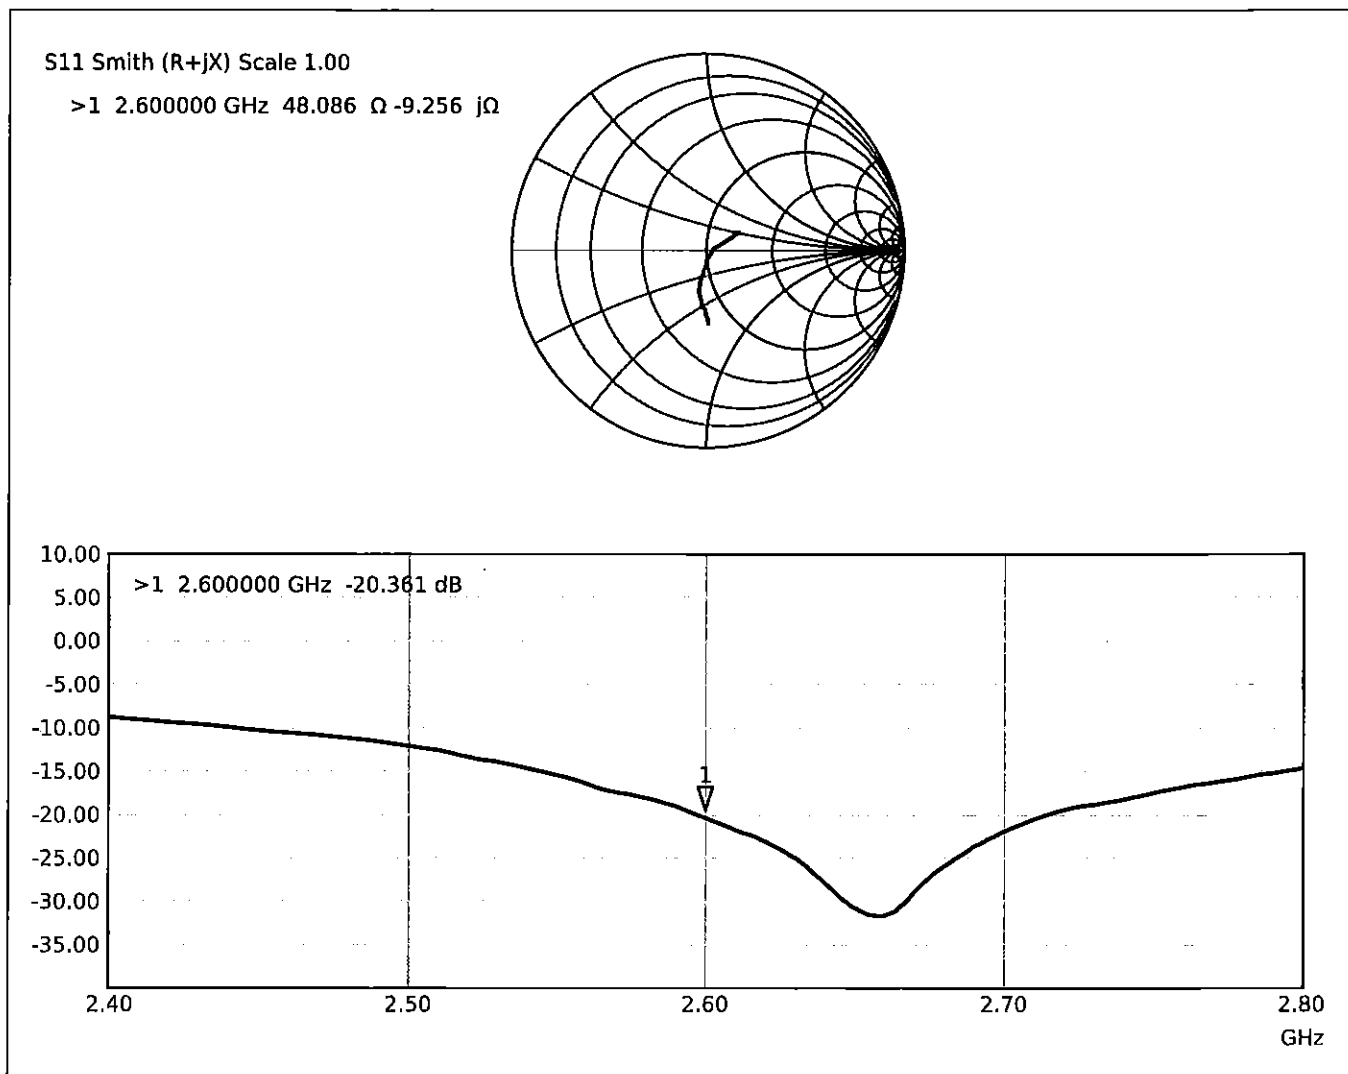

## System Performance Check Report

## Summary

| Dipole           | Frequency [MHz] | TSL | Power [d8m] |
|------------------|-----------------|-----|-------------|
| D2600V2 - SN1042 | 2600            | MSL | 24          |

## Exposure Conditions

| Phantom Section, TSL | Test Distance [mm] | Band | Group, UID | Frequency [MHz], Channel Number | Conversion Factor | TSL Conductivity [S/m] | TSL Permittivity |
|----------------------|--------------------|------|------------|---------------------------------|-------------------|------------------------|------------------|
| Flat                 | 10                 |      | CW, 0--    | 2600, 0                         | 7.19              | 2.20                   | 51.6             |

## Hardware Setup


| Phantom         | TSL, Measured Date | Probe, Calibration Date     | DAE, Calibration Date     |
|-----------------|--------------------|-----------------------------|---------------------------|
| MFP V8.0 Center | MSL, 2025-05-06    | EX3DV4 - SN7349, 2025-01-10 | DAE4lp Sn1836, 2025-04-17 |

## Scans Setup

|                     | Zoom Scan       |
|---------------------|-----------------|
| Grid Extents [mm]   | 30 x 30 x 30    |
| Grid Steps [mm]     | 5.0 x 5.0 x 1.5 |
| Sensor Surface [mm] | 1.4             |
| Graded Grid         | Yes             |
| Grading Ratio       | 1.5             |
| MAIA                | N/A             |
| Surface Detection   | VMS + 6p        |
| Scan Method         | Measured        |


## Measurement Results

|                     | Zoom Scan           |
|---------------------|---------------------|
| Date                | 2025-05-06          |
| psSAR1g [W/Kg]      | 13.4                |
| psSAR10g [W/Kg]     | 6.03                |
| Power Drift [dB]    | -0.01               |
| Power Scaling       | Disabled            |
| Scaling Factor [dB] |                     |
| TSL Correction      | Positive / Negative |

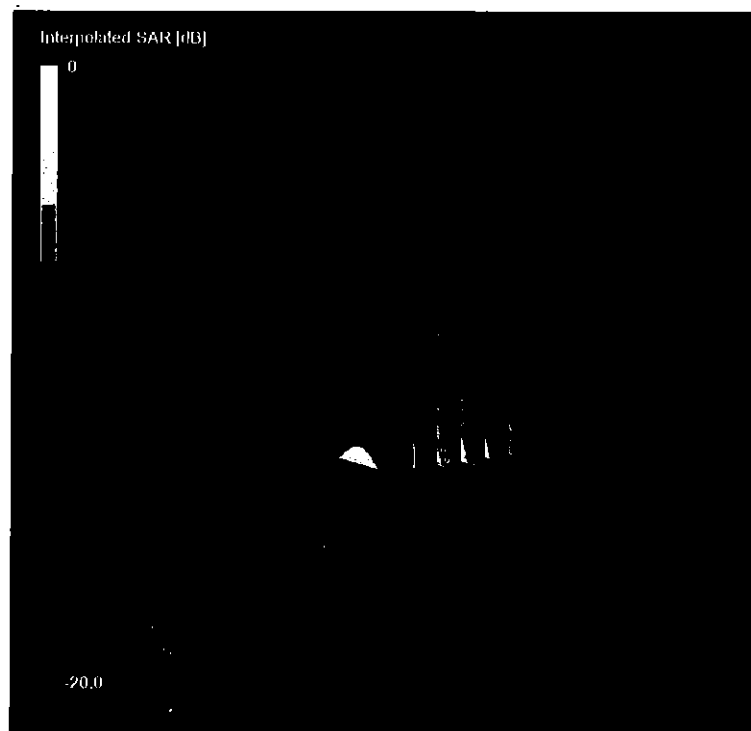

0 dB = 27.7 W/Kg

## Impedance Measurement Plot for MSL

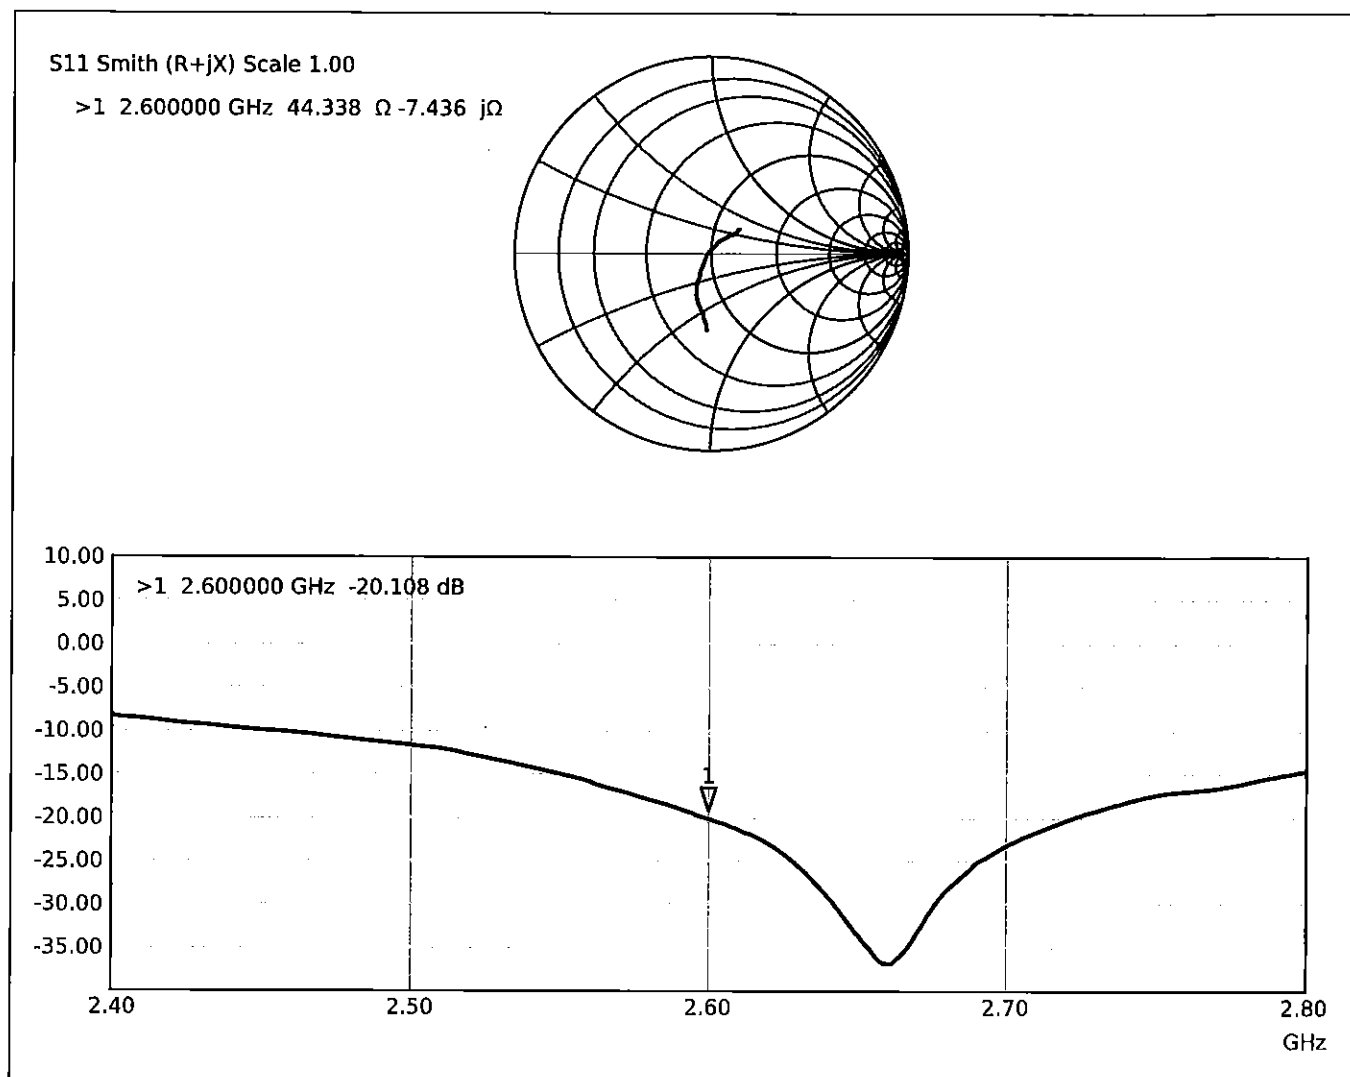



Accredited by the Swiss Accreditation Service (SAS)  
 The Swiss Accreditation Service is one of the signatories to the EA  
 Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: **SCS 0108**

Client **Element**

Certificate No: **D2600V2-1068\_Nov22**

## CALIBRATION CERTIFICATE

Object **D2600V2 - SN:1068**

Calibration procedure(s) **QA CAL-05.v11**  
**Calibration Procedure for SAR Validation Sources between 0.7-3 GHz**

Calibration date: **November 15, 2022**

✓  
 ATM

12/6/22

✓ YW 12/28/2023

✓ YW 11/19/2024

This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI).  
 The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility: environment temperature  $(22 \pm 3)^\circ\text{C}$  and humidity  $< 70\%$ .

Calibration Equipment used (M&TE critical for calibration)

| Primary Standards           | ID #               | Cal Date (Certificate No.)      | Scheduled Calibration |
|-----------------------------|--------------------|---------------------------------|-----------------------|
| Power meter NRP             | SN: 104778         | 04-Apr-22 (No. 217-03525/03524) | Apr-23                |
| Power sensor NRP-Z91        | SN: 103244         | 04-Apr-22 (No. 217-03524)       | Apr-23                |
| Power sensor NRP-Z91        | SN: 103245         | 04-Apr-22 (No. 217-03525)       | Apr-23                |
| Reference 20 dB Attenuator  | SN: BH9394 (20k)   | 04-Apr-22 (No. 217-03527)       | Apr-23                |
| Type-N mismatch combination | SN: 310982 / 06327 | 04-Apr-22 (No. 217-03528)       | Apr-23                |
| Reference Probe EX3DV4      | SN: 7349           | 31-Dec-21 (No. EX3-7349_Dec21)  | Dec-22                |
| DAE4                        | SN: 601            | 31-Aug-22 (No. DAE4-601_Aug22)  | Aug-23                |

| Secondary Standards             | ID #           | Check Date (in house)             | Scheduled Check        |
|---------------------------------|----------------|-----------------------------------|------------------------|
| Power meter E4419B              | SN: GB39512475 | 30-Oct-14 (in house check Oct-22) | In house check: Oct-24 |
| Power sensor HP 8481A           | SN: US37292783 | 07-Oct-15 (in house check Oct-22) | In house check: Oct-24 |
| Power sensor HP 8481A           | SN: MY41093315 | 07-Oct-15 (in house check Oct-22) | In house check: Oct-24 |
| RF generator R&S SMT-06         | SN: 100972     | 15-Jun-15 (in house check Oct-22) | In house check: Oct-24 |
| Network Analyzer Agilent E8358A | SN: US41080477 | 31-Mar-14 (in house check Oct-22) | In house check: Oct-24 |

Calibrated by: **Jeton Kastrati** **Laboratory Technician**

Approved by: **Sven Kühn** **Technical Manager**

Signature

*[Signature]*

*[Signature]*

Issued: November 16, 2022

This calibration certificate shall not be reproduced except in full without written approval of the laboratory.



Accredited by the Swiss Accreditation Service (SAS)

Accreditation No.: **SCS 0108**

The Swiss Accreditation Service is one of the signatories to the EA  
Multilateral Agreement for the recognition of calibration certificates

**Glossary:**

|       |                                 |
|-------|---------------------------------|
| TSL   | tissue simulating liquid        |
| ConvF | sensitivity in TSL / NORM x,y,z |
| N/A   | not applicable or not measured  |

**Calibration is Performed According to the Following Standards:**

- a) IEC/IEEE 62209-1528, "Measurement Procedure For The Assessment Of Specific Absorption Rate Of Human Exposure To Radio Frequency Fields From Hand-Held And Body-Worn Wireless Communication Devices - Part 1528: Human Models, Instrumentation And Procedures (Frequency Range of 4 MHz to 10 GHz)", October 2020.
- b) KDB 865664, "SAR Measurement Requirements for 100 MHz to 6 GHz"

**Additional Documentation:**

- c) DASY System Handbook

**Methods Applied and Interpretation of Parameters:**

- *Measurement Conditions:* Further details are available from the Validation Report at the end of the certificate. All figures stated in the certificate are valid at the frequency indicated.
- *Antenna Parameters with TSL:* The source is mounted in a touch configuration below the center marking of the flat phantom.
- *Return Loss:* This parameter is measured with the source positioned under the liquid filled phantom (as described in the measurement condition clause). The Return Loss ensures low reflected power. No uncertainty required.
- *SAR measured:* SAR measured at the stated antenna input power.
- *SAR normalized:* SAR as measured, normalized to an input power of 1 W at the antenna connector.
- *SAR for nominal TSL parameters:* The measured TSL parameters are used to calculate the nominal SAR result.

The reported uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor  $k=2$ , which for a normal distribution corresponds to a coverage probability of approximately 95%.

## Measurement Conditions

DASY system configuration, as far as not given on page 1.

|                              |                        |             |
|------------------------------|------------------------|-------------|
| DASY Version                 | DASY52                 | V52.10.4    |
| Extrapolation                | Advanced Extrapolation |             |
| Phantom                      | Modular Flat Phantom   |             |
| Distance Dipole Center - TSL | 10 mm                  | with Spacer |
| Zoom Scan Resolution         | dx, dy, dz = 5 mm      |             |
| Frequency                    | 2600 MHz $\pm$ 1 MHz   |             |

## Head TSL parameters

The following parameters and calculations were applied.

|                                         | Temperature         | Permittivity   | Conductivity         |
|-----------------------------------------|---------------------|----------------|----------------------|
| Nominal Head TSL parameters             | 22.0 °C             | 39.0           | 1.96 mho/m           |
| Measured Head TSL parameters            | (22.0 $\pm$ 0.2) °C | 37.8 $\pm$ 6 % | 2.03 mho/m $\pm$ 6 % |
| Head TSL temperature change during test | < 0.5 °C            | ----           | ----                 |

## SAR result with Head TSL

|                                                       |                    |                              |
|-------------------------------------------------------|--------------------|------------------------------|
| SAR averaged over 1 cm <sup>3</sup> (1 g) of Head TSL | Condition          |                              |
| SAR measured                                          | 250 mW input power | 14.4 W/kg                    |
| SAR for nominal Head TSL parameters                   | normalized to 1W   | 56.5 W/kg $\pm$ 17.0 % (k=2) |

|                                                         |                    |                              |
|---------------------------------------------------------|--------------------|------------------------------|
| SAR averaged over 10 cm <sup>3</sup> (10 g) of Head TSL | condition          |                              |
| SAR measured                                            | 250 mW input power | 6.43 W/kg                    |
| SAR for nominal Head TSL parameters                     | normalized to 1W   | 25.4 W/kg $\pm$ 16.5 % (k=2) |

## Body TSL parameters

The following parameters and calculations were applied.

|                                         | Temperature         | Permittivity   | Conductivity         |
|-----------------------------------------|---------------------|----------------|----------------------|
| Nominal Body TSL parameters             | 22.0 °C             | 52.5           | 2.16 mho/m           |
| Measured Body TSL parameters            | (22.0 $\pm$ 0.2) °C | 51.3 $\pm$ 6 % | 2.19 mho/m $\pm$ 6 % |
| Body TSL temperature change during test | < 0.5 °C            | ----           | ----                 |

## SAR result with Body TSL

|                                                       |                    |                              |
|-------------------------------------------------------|--------------------|------------------------------|
| SAR averaged over 1 cm <sup>3</sup> (1 g) of Body TSL | Condition          |                              |
| SAR measured                                          | 250 mW input power | 13.6 W/kg                    |
| SAR for nominal Body TSL parameters                   | normalized to 1W   | 53.9 W/kg $\pm$ 17.0 % (k=2) |

|                                                         |                    |                              |
|---------------------------------------------------------|--------------------|------------------------------|
| SAR averaged over 10 cm <sup>3</sup> (10 g) of Body TSL | condition          |                              |
| SAR measured                                            | 250 mW input power | 6.07 W/kg                    |
| SAR for nominal Body TSL parameters                     | normalized to 1W   | 24.1 W/kg $\pm$ 16.5 % (k=2) |

## Appendix (Additional assessments outside the scope of SCS 0108)

### Antenna Parameters with Head TSL

|                                      |                                |
|--------------------------------------|--------------------------------|
| Impedance, transformed to feed point | 47.8 $\Omega$ - 5.9 j $\Omega$ |
| Return Loss                          | - 23.9 dB                      |

### Antenna Parameters with Body TSL

|                                      |                                |
|--------------------------------------|--------------------------------|
| Impedance, transformed to feed point | 44.5 $\Omega$ - 5.0 j $\Omega$ |
| Return Loss                          | - 22.1 dB                      |

### General Antenna Parameters and Design

|                                  |          |
|----------------------------------|----------|
| Electrical Delay (one direction) | 1.148 ns |
|----------------------------------|----------|

After long term use with 100W radiated power, only a slight warming of the dipole near the feedpoint can be measured.

The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals. On some of the dipoles, small end caps are added to the dipole arms in order to improve matching when loaded according to the position as explained in the "Measurement Conditions" paragraph. The SAR data are not affected by this change. The overall dipole length is still according to the Standard.

No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feedpoint may be damaged.

### Additional EUT Data

|                 |       |
|-----------------|-------|
| Manufactured by | SPEAG |
|-----------------|-------|

## DASY5 Validation Report for Head TSL

Date: 15.11.2022

Test Laboratory: SPEAG, Zurich, Switzerland

**DUT: Dipole 2600 MHz; Type: D2600V2; Serial: D2600V2 - SN:1068**

Communication System: UID 0 - CW; Frequency: 2600 MHz

Medium parameters used:  $f = 2600$  MHz;  $\sigma = 2.03$  S/m;  $\epsilon_r = 37.8$ ;  $\rho = 1000$  kg/m<sup>3</sup>

Phantom section: Flat Section

Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2011)

DASY52 Configuration:

- Probe: EX3DV4 - SN7349; ConvF(7.84, 7.84, 7.84) @ 2600 MHz; Calibrated: 31.12.2021
- Sensor-Surface: 1.4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn601; Calibrated: 31.08.2022
- Phantom: Flat Phantom 5.0 (front); Type: QD 000 P50 AA; Serial: 1001
- DASY52 52.10.4(1535); SEMCAD X 14.6.14(7501)

### Dipole Calibration for Head Tissue/Pin=250 mW, d=10mm/Zoom Scan (7x7x7)/Cube 0:

Measurement grid: dx=5mm, dy=5mm, dz=5mm

Reference Value = 118.5 V/m; Power Drift = 0.01 dB


Peak SAR (extrapolated) = 29.2 W/kg

**SAR(1 g) = 14.4 W/kg; SAR(10 g) = 6.43 W/kg**

Smallest distance from peaks to all points 3 dB below = 9 mm


Ratio of SAR at M2 to SAR at M1 = 49.4%

Maximum value of SAR (measured) = 24.5 W/kg

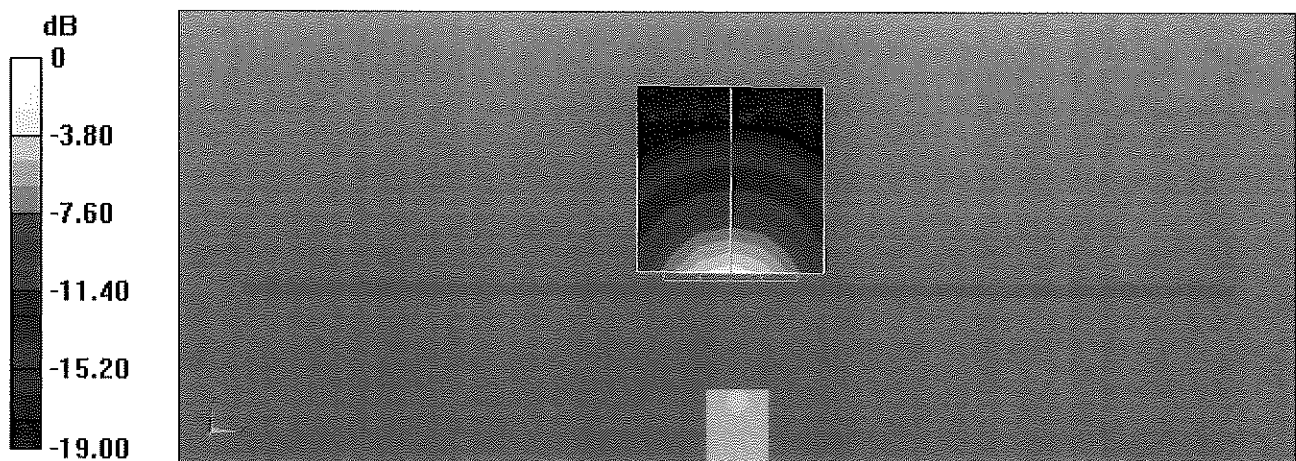

0 dB = 24.5 W/kg = 13.88 dBW/kg

# Impedance Measurement Plot for Head TSL

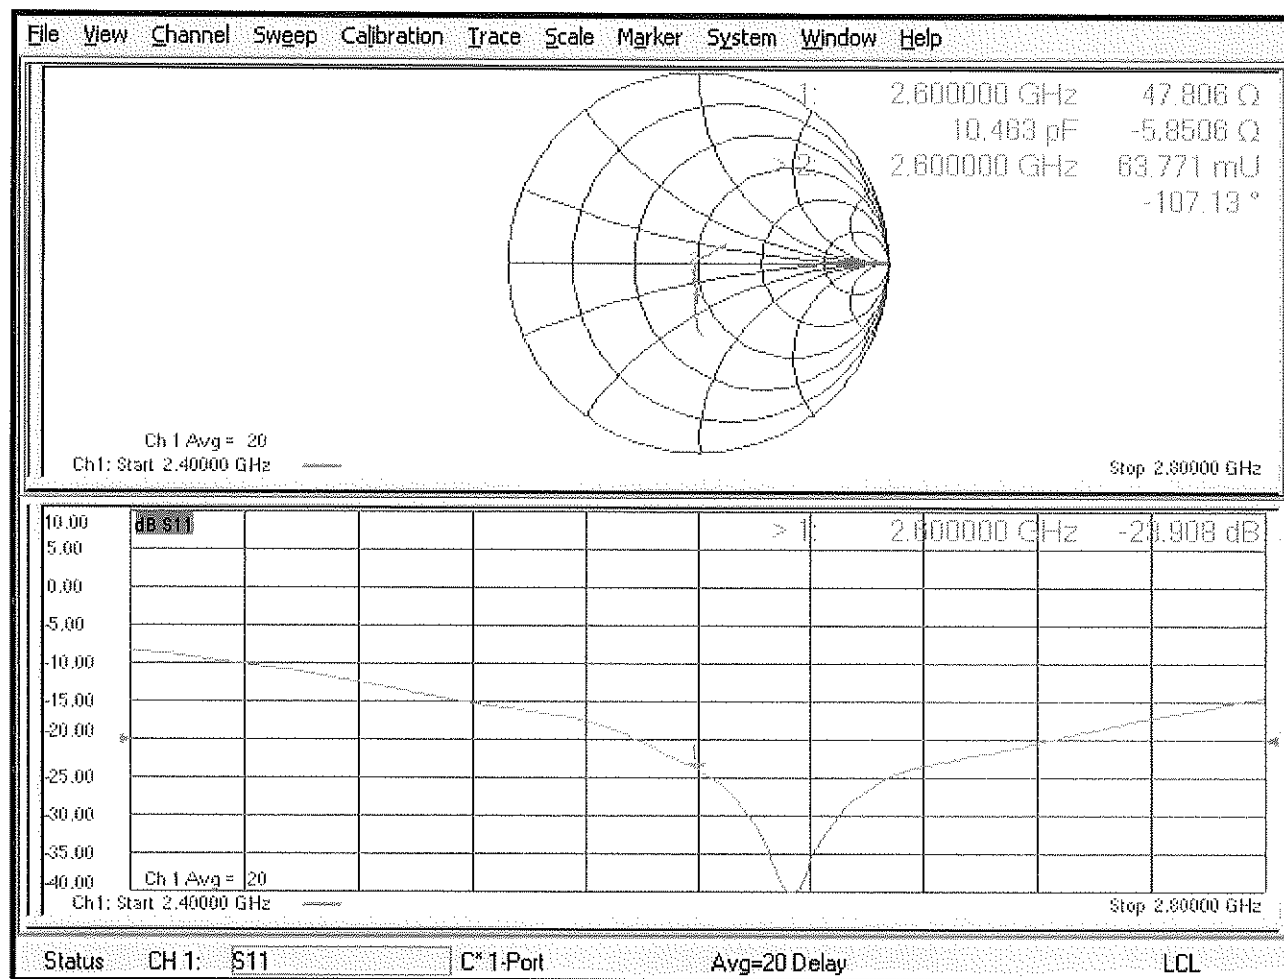

## DASY5 Validation Report for Body TSL

Date: 15.11.2022

Test Laboratory: SPEAG, Zurich, Switzerland

**DUT: Dipole 2600 MHz; Type: D2600V2; Serial: D2600V2 - SN:1068**

Communication System: UID 0 - CW; Frequency: 2600 MHz

Medium parameters used:  $f = 2600$  MHz;  $\sigma = 2.19$  S/m;  $\epsilon_r = 51.3$ ;  $\rho = 1000$  kg/m<sup>3</sup>

Phantom section: Flat Section

Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2011)

DASY52 Configuration:

- Probe: EX3DV4 - SN7349; ConvF(7.91, 7.91, 7.91) @ 2600 MHz; Calibrated: 31.12.2021
- Sensor-Surface: 1.4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn601; Calibrated: 31.08.2022
- Phantom: Flat Phantom 5.0 (back); Type: QD 000 P50 AA; Serial: 1002
- DASY52 52.10.4(1535); SEMCAD X 14.6.14(7501)

### Dipole Calibration for Body Tissue/Pin=250 mW, d=10mm/Zoom Scan (7x7x7)/Cube 0:

Measurement grid: dx=5mm, dy=5mm, dz=5mm

Reference Value = 107.9 V/m; Power Drift = -0.05 dB


Peak SAR (extrapolated) = 27.0 W/kg

**SAR(1 g) = 13.6 W/kg; SAR(10 g) = 6.07 W/kg**

Smallest distance from peaks to all points 3 dB below = 8.5 mm


Ratio of SAR at M2 to SAR at M1 = 51.2%

Maximum value of SAR (measured) = 22.5 W/kg

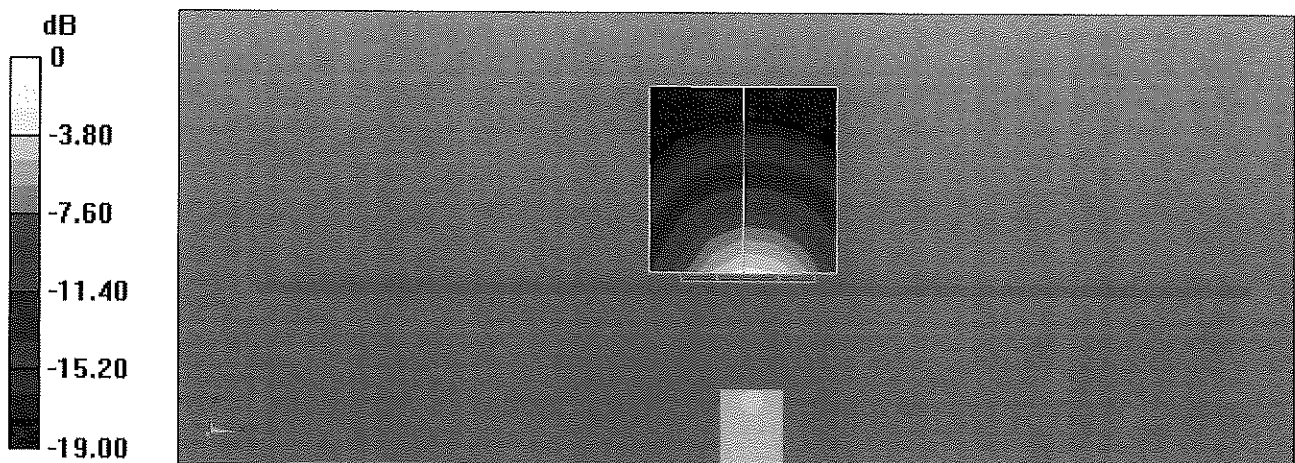

0 dB = 22.5 W/kg = 13.51 dBW/kg

## Impedance Measurement Plot for Body TSL

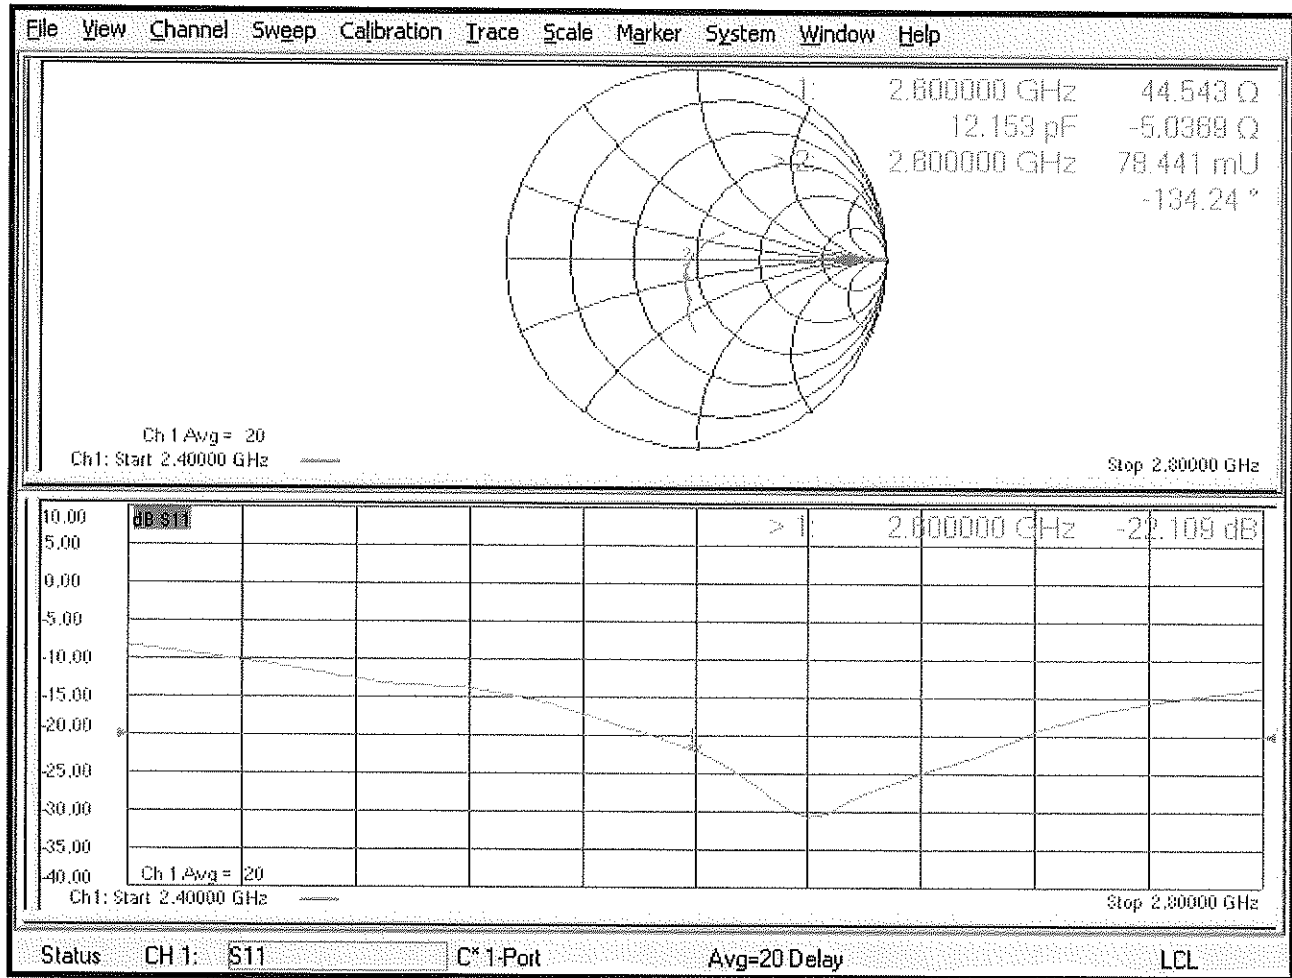

## Certification of Verification

Object: D2600V2 – SN: 1068

Calibration procedure(s): Procedure for Calibration Extension for SAR Dipoles.

Calibration Date: November 15, 2022


Extension Calibration date: November 15, 2023

Description: SAR Validation Dipole at 2600 MHz.

### Calibration Equipment used:

| Manufacturer       | Model         | Description                         | Cal Date   | Cal Interval | Cal Due    | Serial Number |
|--------------------|---------------|-------------------------------------|------------|--------------|------------|---------------|
| Agilent            | 8753ES        | S-Parameter Vector Network Analyzer | 6/2/2023   | Annual       | 6/12/2024  | MY40003841    |
| Agilent            | E4438C        | ESG Vector Signal Generator         | 4/25/2023  | Annual       | 4/25/2024  | US41460739    |
| Amplifier Research | 15S1G6        | Amplifier                           | CBT        | N/A          | CBT        | 343972        |
| Rohde & Schwarz    | NRX           | Power Meter                         | 1/11/2023  | Annual       | 1/11/2024  | 102583        |
| Rohde & Schwarz    | NRP-Z81       | Wide Band Power Sensor              | 1/19/2023  | Annual       | 1/19/2024  | 106563        |
| Rohde & Schwarz    | NRP-Z81       | Wide Band Power Sensor              | 1/11/2023  | Annual       | 1/11/2024  | 106564        |
| Traceable          | 4040 90080-06 | Therm./ Clock/ Humidity Monitor     | 5/11/2022  | Biennial     | 5/11/2024  | 221514974     |
| Control Company    | 4353          | Ultra Long Stem Thermometer         | 10/24/2023 | Annual       | 10/24/2024 | 200645916     |
| Agilent            | 85033E        | 3.5mm Standard Calibration Kit      | 7/18/2023  | Annual       | 7/18/2024  | MY53402352    |
| Mini-Circuits      | VLF-6000+     | Low Pass Filter DC to 6000 MHz      | CBT        | N/A          | CBT        | N/A           |
| Narda              | 4772-3        | Attenuator (3dB)                    | CBT        | N/A          | CBT        | 9406          |
| Mini-Circuits      | ZHDC-16-63-S+ | 50-6000MHz Bidirectional Coupler    | CBT        | N/A          | CBT        | N/A           |
| Pasternack         | NC-100        | Torque Wrench                       | 12/5/2022  | Biennial     | 12/5/2024  | N/A           |
| SPEAG              | DAK-3.5       | Dielectric Assessment Kit           | 5/9/2023   | Annual       | 5/9/2024   | 1070          |
| SPEAG              | EX3DV4        | SAR Probe                           | 11/9/2023  | Annual       | 11/9/2024  | 7639          |
| SPEAG              | DAE4          | Dasy Data Acquisition Electronics   | 11/14/2023 | Annual       | 11/14/2024 | 1403          |

Measurement Uncertainty =  $\pm 23\%$  (k=2)

|                | Name            | Function                   | Signature                                                                             |
|----------------|-----------------|----------------------------|---------------------------------------------------------------------------------------|
| Calibrated By: | Arturo Oliveros | Compliance Engineer        |  |
| Approved By:   | Greg Snyder     | Executive VP of Operations |  |

# DIPOLE CALIBRATION EXTENSION


Per KDB 865664 D01, calibration intervals of up to three years may be considered for reference dipoles when it is demonstrated that the SAR target, impedance and return loss of a dipole have remained stable according to the following requirements:

1. The measured SAR does not deviate more than 10% from the target on the calibration certificate.
2. The return-loss does not deviate more than 20% from the previous measurement and meets the required 20dB minimum return-loss requirement.
3. The measurement of real or imaginary parts of impedance does not deviate more than 5Ω from the previous measurement.

The following dipole was checked to pass the above 3 requirements to have 2-year calibration period from the calibration date:

| Calibration Date | Extension Date | Certificate Electrical Delay (ns) | Certificate SAR Target Head (1g) W/kg @ 20.0 dBm | Measured Head SAR (1g) W/kg @ 20.0 dBm | Deviation 1g (%) | Certificate SAR Target Head (10g) W/kg @ 20.0 dBm | Measured Head SAR (10g) W/kg @ 20.0 dBm | Deviation 10g (%) | Certificate Impedance Head (Ohm) Real | Measured Impedance Head (Ohm) Real | Difference (Ohm) Real | Certificate Impedance Head (Ohm) Imaginary | Measured Impedance Head (Ohm) Imaginary | Difference (Ohm) Imaginary | Certificate Return Loss Head (dB) | Measured Return Loss Head (dB) | Deviation (%) |
|------------------|----------------|-----------------------------------|--------------------------------------------------|----------------------------------------|------------------|---------------------------------------------------|-----------------------------------------|-------------------|---------------------------------------|------------------------------------|-----------------------|--------------------------------------------|-----------------------------------------|----------------------------|-----------------------------------|--------------------------------|---------------|
| 11/15/2022       | 11/15/2023     | 1.148                             | 5.65                                             | 5.2                                    | -7.96%           | 2.54                                              | 2.35                                    | -7.48%            | 47.8                                  | 50.8                               | 3                     | -5.9                                       | -8.7                                    | 2.8                        | -23.9                             | -21.2                          | 11.20%        |

Impedance & Return-Loss Measurement Plot for Head TSL

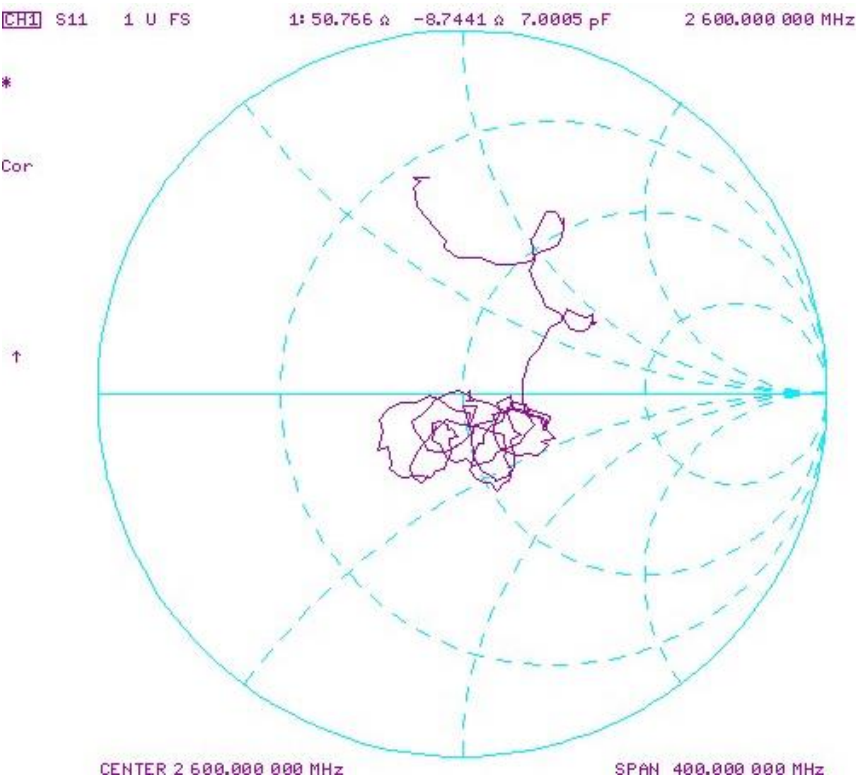

## Certification of Calibration

Object: D2600V2 – SN: 1068

Calibration procedure(s): Procedure for Calibration Extension for SAR Dipoles.


Extension Calibration date: November 15, 2024

Description: SAR Validation Dipole at 2600 MHz.

### Calibration Equipment used:

| Manufacturer       | Model         | Description                       | Cal Date  | Cal Interval | Cal Due   | Serial Number |
|--------------------|---------------|-----------------------------------|-----------|--------------|-----------|---------------|
| Hewlett Packard    | 8753E         | RF Vector Network Analyzer        | 5/21/2024 | Annual       | 5/21/2025 | US38161081    |
| Agilent            | E4438C        | ESG Vector Signal Generator       | 5/19/2024 | Annual       | 5/19/2025 | US41460739    |
| Amplifier Research | 15S1G6        | Amplifier                         | CBT       | N/A          | CBT       | 343972        |
| Anritsu            | ML2496A       | Power Meter                       | 7/15/2024 | Annual       | 7/15/2025 | 1138001       |
| Anritsu            | MA2411B       | Pulse Power Sensor                | 7/10/2024 | Annual       | 7/10/2025 | 1126066       |
| Anritsu            | MA2411B       | Pulse Power Sensor                | 7/1/2024  | Annual       | 7/1/2025  | 1911105       |
| Traceable          | 4040 90080-06 | Therm./ Clock/ Humidity Monitor   | 1/15/2024 | Annual       | 1/15/2025 | 160574418     |
| Control Company    | 4352          | Ultra Long Stem Thermometer       | 1/15/2024 | Annual       | 1/15/2025 | 160508097     |
| Agilent            | 85033E        | 3.5mm Standard Calibration Kit    | 7/31/2024 | Annual       | 7/31/2025 | MY53402352    |
| Mini-Circuits      | VLF-6000+     | Low Pass Filter DC to 6000 MHz    | CBT       | N/A          | CBT       | N/A           |
| Narda              | 4772-3        | Attenuator (3dB)                  | CBT       | N/A          | CBT       | 9406          |
| Mini-Circuits      | ZHDC-16-63-S+ | 50-6000MHz Bidirectional Coupler  | CBT       | N/A          | CBT       | N/A           |
| Pasternack         | NC-100        | Torque Wrench                     | 12/5/2022 | Biennial     | 12/5/2024 | N/A           |
| SPEAG              | DAK-3.5       | Dielectric Assessment Kit         | 5/14/2024 | Annual       | 5/14/2025 | 1070          |
| SPEAG              | EX3DV4        | SAR Probe                         | 9/9/2024  | Annual       | 9/9/2025  | 7639          |
| SPEAG              | DAE4          | Dasy Data Acquisition Electronics | 9/4/2024  | Annual       | 9/4/2025  | 1403          |

Measurement Uncertainty =  $\pm 23\%$  (k=2)

|                | Name            | Function                   | Signature                                                                             |
|----------------|-----------------|----------------------------|---------------------------------------------------------------------------------------|
| Calibrated By: | Arturo Oliveros | Compliance Engineer        |  |
| Approved By:   | Greg Snyder     | Executive VP of Operations |  |

# DIPOLE CALIBRATION EXTENSION



Per KDB 865664 D01, calibration intervals of up to three years may be considered for reference dipoles when it is demonstrated that the SAR target, impedance and return loss of a dipole have remained stable according to the following requirements:

1. The measured SAR does not deviate more than 10% from the target on the calibration certificate.
2. The return-loss does not deviate more than 20% from the previous measurement and meets the required 20dB minimum return-loss requirement.
3. The measurement of real or imaginary parts of impedance does not deviate more than 5Ω from the previous measurement.

The following dipole was checked to pass the above 3 requirements to have 3-year calibration period from the calibration date:

| Calibration Date | Extension Date | Certificate Electrical Delay (ns) | Certificate SAR Target Head (1g) W/kg @ 20.0 dBm | Measured Head SAR (1g) W/kg @ 20.0 dBm | Deviation 1g (%) | Certificate SAR Target Head (10g) W/kg @ 20.0 dBm | Measured Head SAR (10g) W/kg @ 20.0 dBm | Deviation 10g (%) | Certificate Impedance Head (Ohm) Real | Measured Impedance Head (Ohm) Real | Difference (Ohm) Real | Certificate Impedance Head (Ohm) Imaginary | Measured Impedance Head (Ohm) Imaginary | Difference (Ohm) Imaginary | Certificate Return Loss Head (dB) | Measured Return Loss Head (dB) | Deviation (%) |
|------------------|----------------|-----------------------------------|--------------------------------------------------|----------------------------------------|------------------|---------------------------------------------------|-----------------------------------------|-------------------|---------------------------------------|------------------------------------|-----------------------|--------------------------------------------|-----------------------------------------|----------------------------|-----------------------------------|--------------------------------|---------------|
| 11/15/2022       | 11/15/2024     | 1.148                             | 5.65                                             | 5.62                                   | -0.53%           | 2.54                                              | 2.55                                    | 0.39%             | 47.8                                  | 49.2                               | 1.4                   | -5.9                                       | -5.7                                    | 0.2                        | -23.9                             | -24.7                          | -3.50%        |

Impedance & Return-Loss Measurement Plot for Head TSL

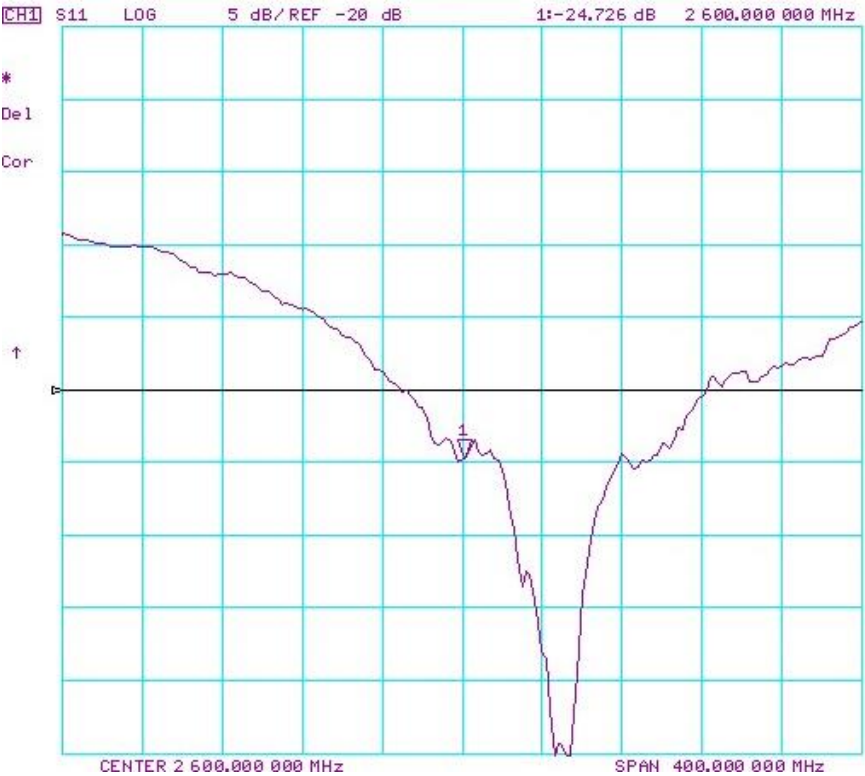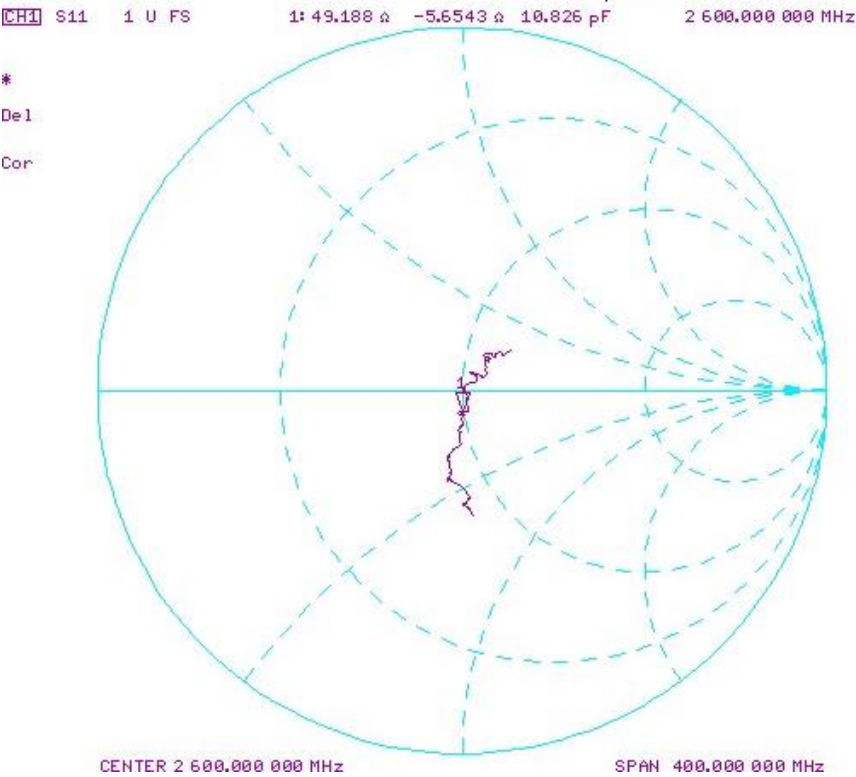



Accredited by the Swiss Accreditation Service (SAS)

The Swiss Accreditation Service is one of the signatories to the EA  
Multilateral Agreement for the recognition of calibration certificates

Client **Element**  
**Morgan Hill, USA**

Certificate No. **D2600V2-1069\_Sep23**

## CALIBRATION CERTIFICATE

Object **D2600V2 - SN:1069**

Calibration procedure(s) **QA CAL-05.v12**  
**Calibration Procedure for SAR Validation Sources between 0.7-3 GHz**

Calibration date: **September 12, 2023**

This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI).  
The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility: environment temperature ( $22 \pm 3$ )°C and humidity < 70%.

Calibration Equipment used (M&TE critical for calibration)

| Primary Standards           | ID #               | Cal Date (Certificate No.)      | Scheduled Calibration |
|-----------------------------|--------------------|---------------------------------|-----------------------|
| Power meter NRP2            | SN: 104778         | 30-Mar-23 (No. 217-03804/03805) | Mar-24                |
| Power sensor NRP-Z91        | SN: 103244         | 30-Mar-23 (No. 217-03804)       | Mar-24                |
| Power sensor NRP-Z91        | SN: 103245         | 30-Mar-23 (No. 217-03805)       | Mar-24                |
| Reference 20 dB Attenuator  | SN: BH9394 (20k)   | 30-Mar-23 (No. 217-03809)       | Mar-24                |
| Type-N mismatch combination | SN: 310982 / 06327 | 30-Mar-23 (No. 217-03810)       | Mar-24                |
| Reference Probe EX3DV4      | SN: 7349           | 10-Jan-23 (No. EX3-7349_Jan23)  | Jan-24                |
| DAE4                        | SN: 601            | 19-Dec-22 (No. DAE4-601_Dec22)  | Dec-23                |

| Secondary Standards             | ID #           | Check Date (in house)             | Scheduled Check        |
|---------------------------------|----------------|-----------------------------------|------------------------|
| Power meter E4419B              | SN: GB39512475 | 30-Oct-14 (in house check Oct-22) | In house check: Oct-24 |
| Power sensor HP 8481A           | SN: US37292783 | 07-Oct-15 (in house check Oct-22) | In house check: Oct-24 |
| Power sensor HP 8481A           | SN: MY41093315 | 07-Oct-15 (in house check Oct-22) | In house check: Oct-24 |
| RF generator R&S SMT-06         | SN: 100972     | 15-Jun-15 (in house check Oct-22) | In house check: Oct-24 |
| Network Analyzer Agilent E8358A | SN: US41080477 | 31-Mar-14 (in house check Oct-22) | In house check: Oct-24 |

Calibrated by: **Krešimir Franjić** **Laboratory Technician**

Approved by: **Sven Kühn** **Technical Manager**

Issued: September 14, 2023

This calibration certificate shall not be reproduced except in full without written approval of the laboratory.



Accredited by the Swiss Accreditation Service (SAS)

Accreditation No.: **SCS 0108**

The Swiss Accreditation Service is one of the signatories to the EA  
Multilateral Agreement for the recognition of calibration certificates

### Glossary:

|       |                                 |
|-------|---------------------------------|
| TSL   | tissue simulating liquid        |
| ConvF | sensitivity in TSL / NORM x,y,z |
| N/A   | not applicable or not measured  |

### Calibration is Performed According to the Following Standards:

- IEC/IEEE 62209-1528, "Measurement Procedure For The Assessment Of Specific Absorption Rate Of Human Exposure To Radio Frequency Fields From Hand-Held And Body-Worn Wireless Communication Devices - Part 1528: Human Models, Instrumentation And Procedures (Frequency Range of 4 MHz to 10 GHz)", October 2020.
- KDB 865664, "SAR Measurement Requirements for 100 MHz to 6 GHz"

### Additional Documentation:

- DASY System Handbook

### Methods Applied and Interpretation of Parameters:

- Measurement Conditions:* Further details are available from the Validation Report at the end of the certificate. All figures stated in the certificate are valid at the frequency indicated.
- Antenna Parameters with TSL:* The source is mounted in a touch configuration below the center marking of the flat phantom.
- Return Loss:* This parameter is measured with the source positioned under the liquid filled phantom (as described in the measurement condition clause). The Return Loss ensures low reflected power. No uncertainty required.
- SAR measured:* SAR measured at the stated antenna input power.
- SAR normalized:* SAR as measured, normalized to an input power of 1 W at the antenna connector.
- SAR for nominal TSL parameters:* The measured TSL parameters are used to calculate the nominal SAR result.

The reported uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor  $k=2$ , which for a normal distribution corresponds to a coverage probability of approximately 95%.

## Measurement Conditions

DASY system configuration, as far as not given on page 1.

|                              |                        |             |
|------------------------------|------------------------|-------------|
| DASY Version                 | DASY52                 | V52.10.4    |
| Extrapolation                | Advanced Extrapolation |             |
| Phantom                      | Modular Flat Phantom   |             |
| Distance Dipole Center - TSL | 10 mm                  | with Spacer |
| Zoom Scan Resolution         | dx, dy, dz = 5 mm      |             |
| Frequency                    | 2600 MHz $\pm$ 1 MHz   |             |

## Head TSL parameters

The following parameters and calculations were applied.

|                                         | Temperature         | Permittivity   | Conductivity         |
|-----------------------------------------|---------------------|----------------|----------------------|
| Nominal Head TSL parameters             | 22.0 °C             | 39.0           | 1.96 mho/m           |
| Measured Head TSL parameters            | (22.0 $\pm$ 0.2) °C | 37.2 $\pm$ 6 % | 1.99 mho/m $\pm$ 6 % |
| Head TSL temperature change during test | < 0.5 °C            | ---            | ---                  |

## SAR result with Head TSL

|                                                       |                    |                              |
|-------------------------------------------------------|--------------------|------------------------------|
| SAR averaged over 1 cm <sup>3</sup> (1 g) of Head TSL | Condition          |                              |
| SAR measured                                          | 250 mW input power | 14.3 W/kg                    |
| SAR for nominal Head TSL parameters                   | normalized to 1W   | 56.2 W/kg $\pm$ 17.0 % (k=2) |

|                                                         |                    |                              |
|---------------------------------------------------------|--------------------|------------------------------|
| SAR averaged over 10 cm <sup>3</sup> (10 g) of Head TSL | condition          |                              |
| SAR measured                                            | 250 mW input power | 6.45 W/kg                    |
| SAR for nominal Head TSL parameters                     | normalized to 1W   | 25.5 W/kg $\pm$ 16.5 % (k=2) |

## Body TSL parameters

The following parameters and calculations were applied.

|                                         | Temperature         | Permittivity   | Conductivity         |
|-----------------------------------------|---------------------|----------------|----------------------|
| Nominal Body TSL parameters             | 22.0 °C             | 52.5           | 2.16 mho/m           |
| Measured Body TSL parameters            | (22.0 $\pm$ 0.2) °C | 52.2 $\pm$ 6 % | 2.20 mho/m $\pm$ 6 % |
| Body TSL temperature change during test | < 0.5 °C            | ---            | ---                  |

## SAR result with Body TSL

|                                                       |                    |                              |
|-------------------------------------------------------|--------------------|------------------------------|
| SAR averaged over 1 cm <sup>3</sup> (1 g) of Body TSL | Condition          |                              |
| SAR measured                                          | 250 mW input power | 13.5 W/kg                    |
| SAR for nominal Body TSL parameters                   | normalized to 1W   | 53.3 W/kg $\pm$ 17.0 % (k=2) |

|                                                         |                    |                              |
|---------------------------------------------------------|--------------------|------------------------------|
| SAR averaged over 10 cm <sup>3</sup> (10 g) of Body TSL | condition          |                              |
| SAR measured                                            | 250 mW input power | 6.10 W/kg                    |
| SAR for nominal Body TSL parameters                     | normalized to 1W   | 24.3 W/kg $\pm$ 16.5 % (k=2) |

## Appendix (Additional assessments outside the scope of SCS 0108)

### Antenna Parameters with Head TSL

|                                      |                                |
|--------------------------------------|--------------------------------|
| Impedance, transformed to feed point | 48.5 $\Omega$ - 5.0 j $\Omega$ |
| Return Loss                          | - 25.6 dB                      |

### Antenna Parameters with Body TSL

|                                      |                                |
|--------------------------------------|--------------------------------|
| Impedance, transformed to feed point | 46.2 $\Omega$ - 5.5 j $\Omega$ |
| Return Loss                          | - 23.2 dB                      |

### General Antenna Parameters and Design

|                                  |          |
|----------------------------------|----------|
| Electrical Delay (one direction) | 1.152 ns |
|----------------------------------|----------|

After long term use with 100W radiated power, only a slight warming of the dipole near the feedpoint can be measured.

The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals. On some of the dipoles, small end caps are added to the dipole arms in order to improve matching when loaded according to the position as explained in the "Measurement Conditions" paragraph. The SAR data are not affected by this change. The overall dipole length is still according to the Standard.

No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feedpoint may be damaged.

### Additional EUT Data

|                 |       |
|-----------------|-------|
| Manufactured by | SPEAG |
|-----------------|-------|

## DASY5 Validation Report for Head TSL

Date: 12.09.2023

Test Laboratory: SPEAG, Zurich, Switzerland

**DUT: Dipole 2600 MHz; Type: D2600V2; Serial: D2600V2 - SN:1069**

Communication System: UID 0 - CW; Frequency: 2600 MHz

Medium parameters used:  $f = 2600$  MHz;  $\sigma = 1.99$  S/m;  $\epsilon_r = 37.2$ ;  $\rho = 1000$  kg/m<sup>3</sup>

Phantom section: Flat Section

Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2011)

DASY52 Configuration:

- Probe: EX3DV4 - SN7349; ConvF(7.68, 7.68, 7.68) @ 2600 MHz; Calibrated: 10.01.2023
- Sensor-Surface: 1.4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn601; Calibrated: 19.12.2022
- Phantom: Flat Phantom 5.0 (front); Type: QD 000 P50 AA; Serial: 1001
- DASY52 52.10.4(1535); SEMCAD X 14.6.14(7501)

### Dipole Calibration for Head Tissue/Pin=250 mW, d=10mm/Zoom Scan (7x7x7)/Cube 0:

Measurement grid: dx=5mm, dy=5mm, dz=5mm

Reference Value = 120.2 V/m; Power Drift = 0.01 dB



Peak SAR (extrapolated) = 27.8 W/kg

**SAR(1 g) = 14.3 W/kg; SAR(10 g) = 6.45 W/kg**

Smallest distance from peaks to all points 3 dB below = 9 mm


Ratio of SAR at M2 to SAR at M1 = 51.5%

Maximum value of SAR (measured) = 23.5 W/kg

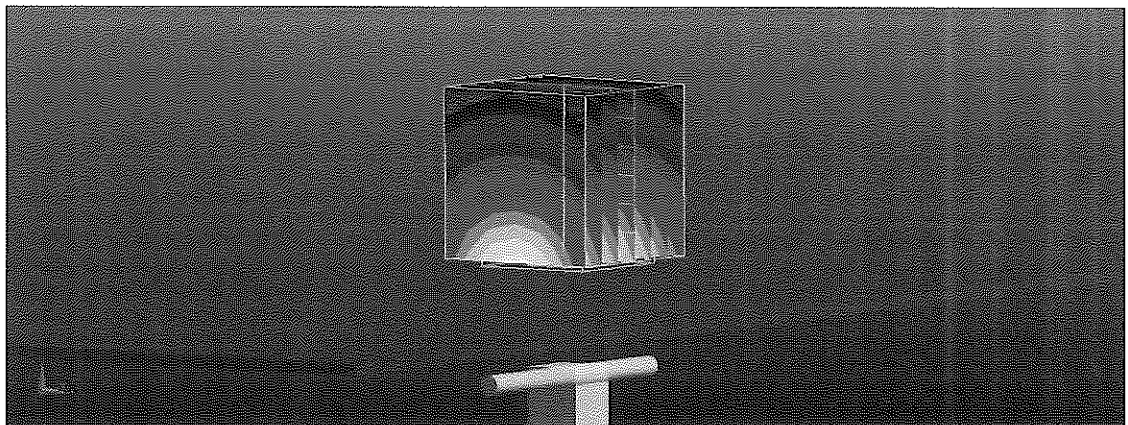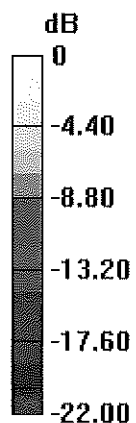

0 dB = 23.5 W/kg = 13.71 dBW/kg

## Impedance Measurement Plot for Head TSL

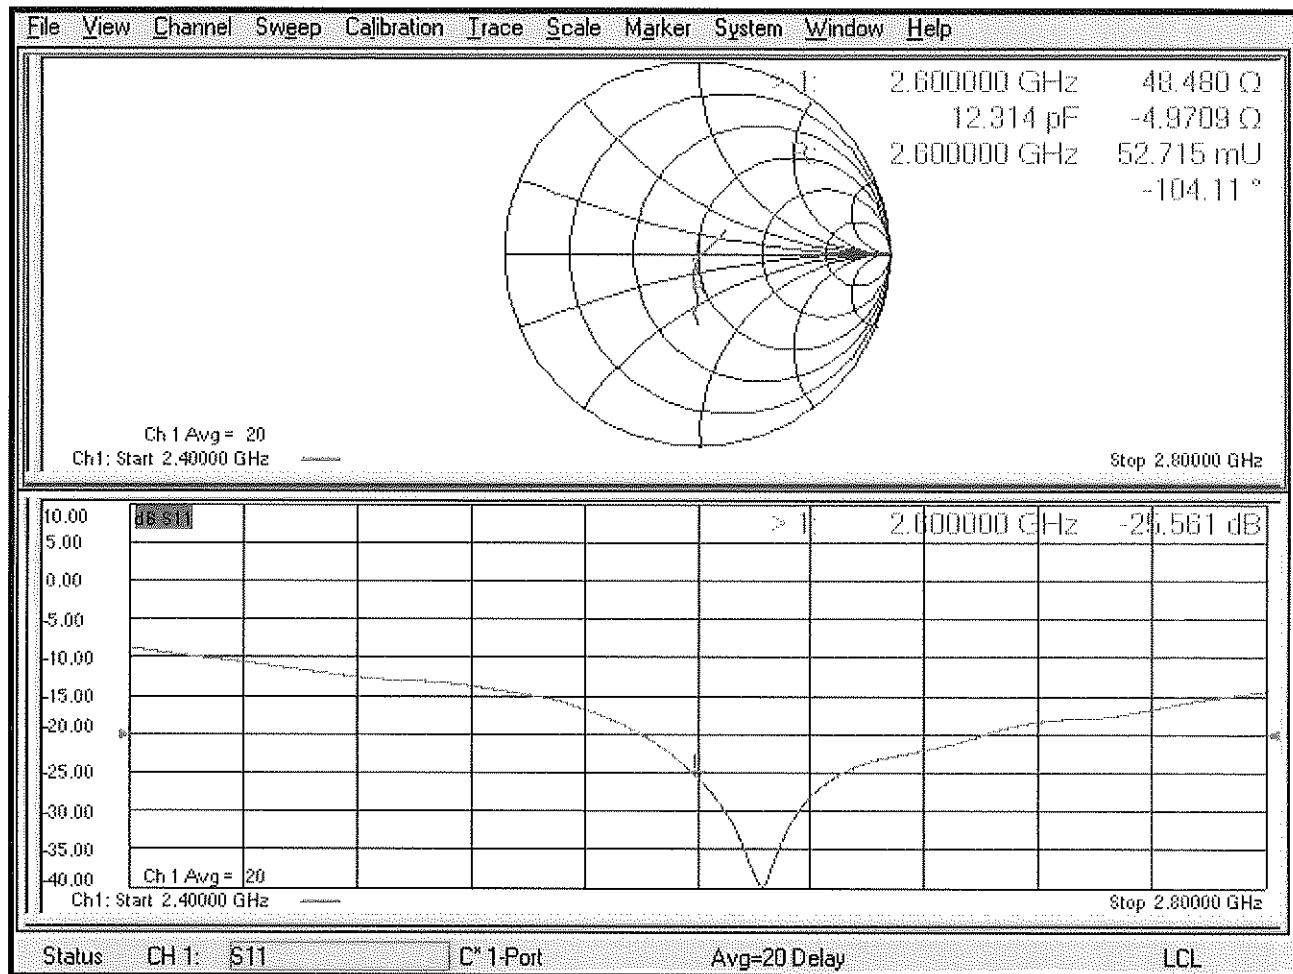

## DASY5 Validation Report for Body TSL

Date: 06.09.2023

Test Laboratory: SPEAG, Zurich, Switzerland

**DUT: Dipole 2600 MHz; Type: D2600V2; Serial: D2600V2 - SN:1069**

Communication System: UID 0 - CW; Frequency: 2600 MHz

Medium parameters used:  $f = 2600$  MHz;  $\sigma = 2.2$  S/m;  $\epsilon_r = 52.2$ ;  $\rho = 1000$  kg/m<sup>3</sup>

Phantom section: Flat Section

Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2011)

DASY52 Configuration:

- Probe: EX3DV4 - SN7349; ConvF(7.83, 7.83, 7.83) @ 2600 MHz; Calibrated: 10.01.2023
- Sensor-Surface: 1.4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn601; Calibrated: 19.12.2022
- Phantom: Flat Phantom 5.0 (back); Type: QD 000 P50 AA; Serial: 1002
- DASY52 52.10.4(1535); SEMCAD X 14.6.14(7501)

### Dipole Calibration for Body Tissue/Pin=250 mW, d=10mm/Zoom Scan (7x7x7)/Cube 0:

Measurement grid: dx=5mm, dy=5mm, dz=5mm

Reference Value = 106.7 V/m; Power Drift = -0.09 dB


Peak SAR (extrapolated) = 25.9 W/kg

**SAR(1 g) = 13.5 W/kg; SAR(10 g) = 6.10 W/kg**

Smallest distance from peaks to all points 3 dB below = 8.5 mm


Ratio of SAR at M2 to SAR at M1 = 53.3%

Maximum value of SAR (measured) = 21.7 W/kg

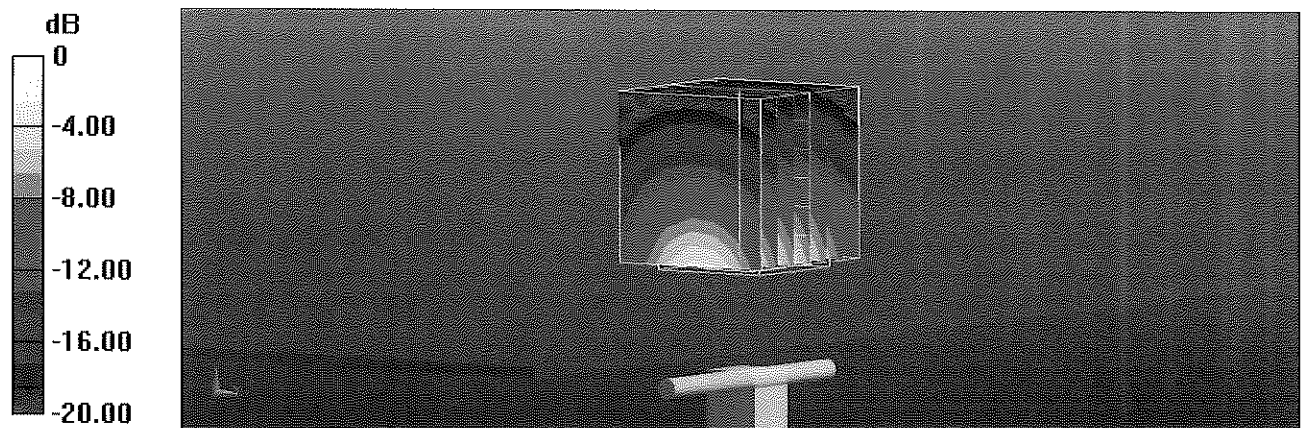

0 dB = 21.7 W/kg = 13.37 dBW/kg

# Impedance Measurement Plot for Body TSL

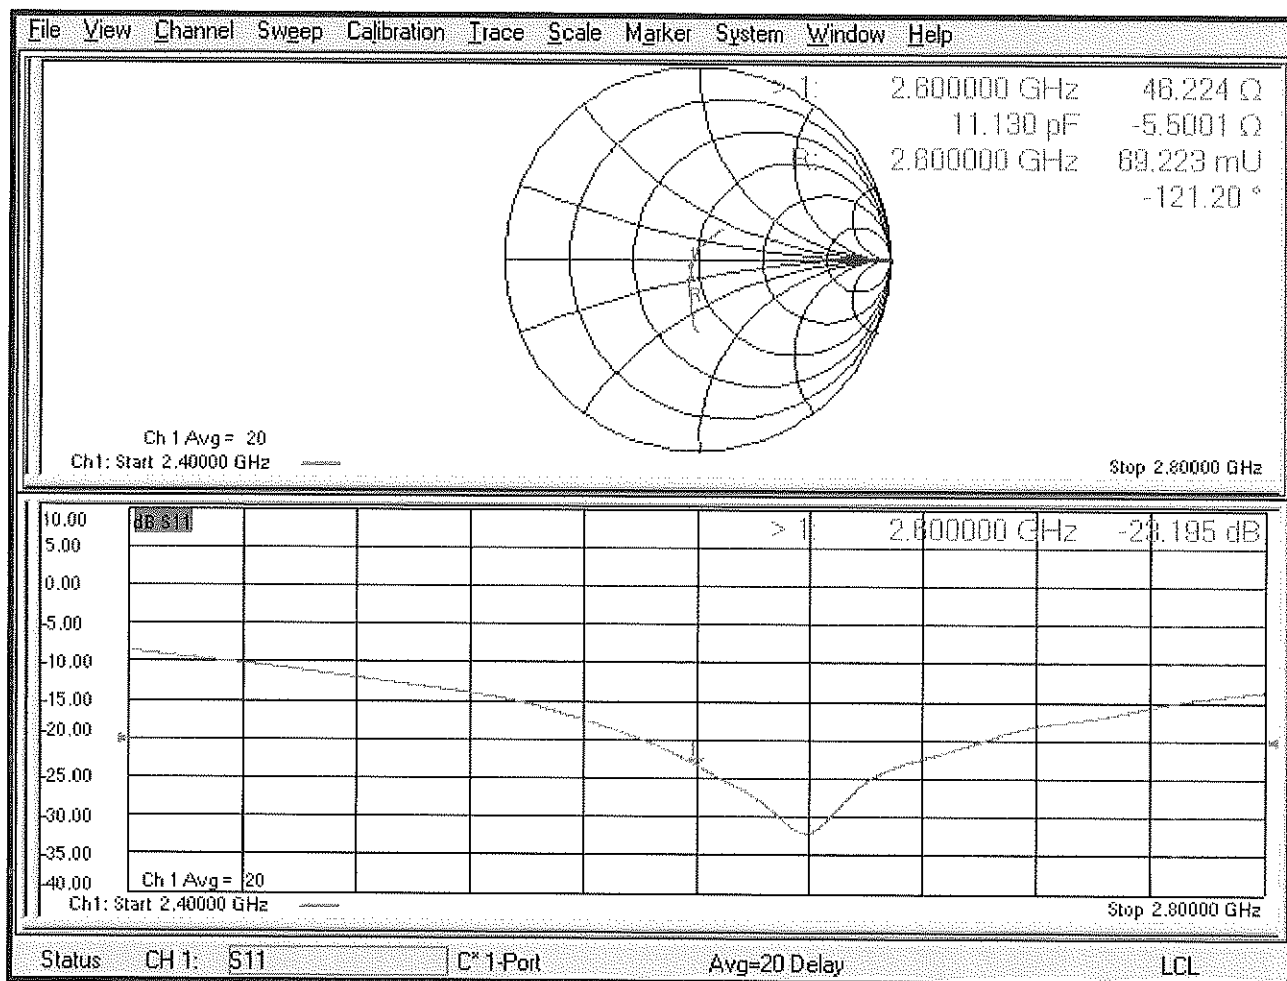

## Certification of Calibration

Object: D2600V2 – SN: 1069

Calibration procedure(s): Procedure for Calibration Extension for SAR Dipoles.


Extension Calibration date: September 12, 2024

Description: SAR Validation Dipole at 2600 MHz.

### Calibration Equipment used:

| Manufacturer       | Model         | Description                       | Cal Date  | Cal Interval | Cal Due   | Serial Number |
|--------------------|---------------|-----------------------------------|-----------|--------------|-----------|---------------|
| Hewlett Packard    | 8753E         | RF Vector Network Analyzer        | 5/21/2024 | Annual       | 5/21/2025 | US38161081    |
| Agilent            | E4438C        | ESG Vector Signal Generator       | 5/19/2024 | Annual       | 5/19/2025 | US41460739    |
| Amplifier Research | 1551G6        | Amplifier                         | CBT       | N/A          | CBT       | 343972        |
| Anritsu            | ML2496A       | Power Meter                       | 7/15/2024 | Annual       | 7/15/2025 | 1138001       |
| Anritsu            | MA2411B       | Pulse Power Sensor                | 7/10/2024 | Annual       | 7/10/2025 | 1126066       |
| Anritsu            | MA2411B       | Pulse Power Sensor                | 7/1/2024  | Annual       | 7/1/2025  | 1911105       |
| Traceable          | 4040 90080-06 | Therm./ Clock/ Humidity Monitor   | 1/15/2024 | Annual       | 1/15/2025 | 160574418     |
| Control Company    | 4352          | Ultra Long Stem Thermometer       | 1/15/2024 | Annual       | 1/15/2025 | 160508097     |
| Agilent            | 85033E        | 3.5mm Standard Calibration Kit    | 7/31/2024 | Annual       | 7/31/2025 | MY53402352    |
| Mini-Circuits      | VLF-6000+     | Low Pass Filter DC to 6000 MHz    | CBT       | N/A          | CBT       | N/A           |
| Narda              | 4772-3        | Attenuator (3dB)                  | CBT       | N/A          | CBT       | 9406          |
| Mini-Circuits      | ZHDC-16-63-S+ | 50-6000MHz Bidirectional Coupler  | CBT       | N/A          | CBT       | N/A           |
| Pasternack         | NC-100        | Torque Wrench                     | 12/5/2022 | Biennial     | 12/5/2024 | N/A           |
| SPEAG              | DAK-3.5       | Dielectric Assessment Kit         | 5/14/2024 | Annual       | 5/14/2025 | 1070          |
| SPEAG              | EX3DV4        | SAR Probe                         | 5/13/2024 | Annual       | 5/13/2025 | 7552          |
| SPEAG              | DAE4          | Dasy Data Acquisition Electronics | 5/8/2024  | Annual       | 5/8/2025  | 1676          |

Measurement Uncertainty =  $\pm 23\%$  (k=2)

|                | Name            | Function                   | Signature                                                                             |
|----------------|-----------------|----------------------------|---------------------------------------------------------------------------------------|
| Calibrated By: | Arturo Oliveros | Compliance Engineer        |  |
| Approved By:   | Greg Snyder     | Executive VP of Operations |  |

# DIPOLE CALIBRATION EXTENSION

Per KDB 865664 D01, calibration intervals of up to three years may be considered for reference dipoles when it is demonstrated that the SAR target, impedance and return loss of a dipole have remained stable according to the following requirements:


1. The measured SAR does not deviate more than 10% from the target on the calibration certificate.
2. The return-loss does not deviate more than 20% from the previous measurement and meets the required 20dB minimum return-loss requirement.
3. The measurement of real or imaginary parts of impedance does not deviate more than 5Ω from the previous measurement.

The following dipole was checked to pass the above 3 requirements to have 2-year calibration period from the calibration date:

| Calibration Date | Extension Date | Certificate Electrical Delay (ns) | Certificate SAR Target Head (1g) W/kg @ 20.0 dBm | Measured Head SAR (1g) W/kg @ 20.0 dBm | Deviation 1g (%) | Certificate SAR Target Head (10g) W/kg @ 20.0 dBm | Measured Head SAR (10g) W/kg @ 20.0 dBm | Deviation 10g (%) | Certificate Impedance Head (Ohm) Real | Measured Impedance Head (Ohm) Real | Difference (Ohm) Real | Certificate Impedance Head (Ohm) Imaginary | Measured Impedance Head (Ohm) Imaginary | Difference (Ohm) Imaginary | Certificate Return Loss Head (dB) | Measured Return Loss Head (dB) | Deviation (%) |
|------------------|----------------|-----------------------------------|--------------------------------------------------|----------------------------------------|------------------|---------------------------------------------------|-----------------------------------------|-------------------|---------------------------------------|------------------------------------|-----------------------|--------------------------------------------|-----------------------------------------|----------------------------|-----------------------------------|--------------------------------|---------------|
| 9/12/2023        | 9/12/2024      | 1.152                             | 5.62                                             | 5.56                                   | -1.07%           | 2.55                                              | 2.42                                    | -5.10%            | 48.5                                  | 53.2                               | 4.7                   | -5                                         | -2.2                                    | 2.8                        | -25.6                             | -23.9                          | 6.50%         |

Impedance & Return-Loss Measurement Plot for Head TSL

[CH1] S11 1 U FS 1: 53.184  $\Omega$  -2.1660  $\Omega$  28.261 pF 2 600.000 000 MHz

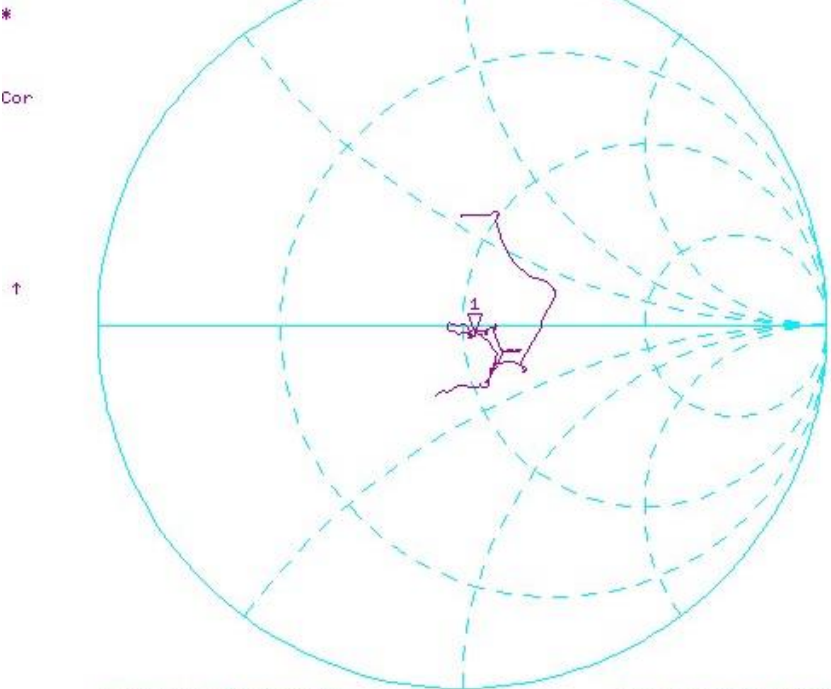

[CH1] S11 CENTER 2 600.000 000 MHz L06 5 dB/ REF -20 dB 1:-23.935 dB SPAN 400.000 000 MHz 2 600.000 000 MHz



**Calibration Laboratory of****Schmid & Partner  
Engineering AG**

Zeughausstrasse 43, 8004 Zurich, Switzerland

**S** Schweizerischer Kalibrierdienst  
**C** Service suisse d'étalonnage  
**S** Servizio svizzero di taratura  
**S** Swiss Calibration Service

Accredited by the Swiss Accreditation Service (SAS)

**The Swiss Accreditation Service is one of the signatories to the EA  
Multilateral Agreement for the recognition of calibration certificates**Accreditation No.: **SCS 0108**

Client

**Element**

Morgan Hill, USA

Certificate No.

**D5GHzV2-1066\_Nov24****CALIBRATION CERTIFICATE**

Object

D5GHzV2 - SN: 1066

✓ yw 11/19/24

Calibration procedure(s)

QA CAL-22.v7

Calibration Procedure for SAR Validation Sources between 3 - 10 GHz

Calibration date

November 8, 2024

This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI).  
The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility: environment temperature  $(22 \pm 3)^\circ\text{C}$  and humidity  $< 70\%$ .

Calibration Equipment used (M&TE critical for calibration)

| Primary Standards                          | ID         | Cal Date (Certificate No.)            | Scheduled Cal |
|--------------------------------------------|------------|---------------------------------------|---------------|
| Power Sensor R&S NRP-33T                   | SN: 100967 | 28-Mar-24 (No. 217-04038)             | Mar-25        |
| Power Sensor R&S NRP18A                    | SN: 101859 | 22-Jul-24 (No. 4030A315008547)        | Jul-25        |
| Spectrum Analyzer R&S FSV40                | SN: 101832 | 25-Jan-24 (No. 4030-315007551)        | Jan-25        |
| Mismatch; Short [S4188] Attenuator [S4423] | SN: 1152   | 28-Mar-24 (No. 217-04050)             | Mar-25        |
| OCP DAK-12                                 | SN: 1016   | 24-Sep-24 (No. OCP-DAK12-1016_Sep24)  | Sep-25        |
| OCP DAK-3.5                                | SN: 1249   | 23-Sep-24 (No. OCP-DAK3.5-1249_Sep24) | Sep-25        |
| Reference Probe EX3DV4                     | SN: 7349   | 03-Jun-24 (No. EX3-7349_Jun24)        | Jun-25        |
| DAE4ip                                     | SN: 1836   | 28-Oct-24 (No. DAE4ip-1836_Oct24)     | Oct-25        |

| Secondary Standards          | ID         | Check Date (in house)                      | Scheduled Check |
|------------------------------|------------|--------------------------------------------|-----------------|
| ACAD Source Box              | SN: 1000   | 28-May-24 (No. 675-ACAD_Source_Box-240528) | May-25          |
| Signal Generator R&S SMB100A | SN: 182081 | 28-May-24 (No. 675-CAL16-S4588-240528)     | May-25          |
| Mismatch; SMA                | SN: 1102   | 22-May-24 (No. 675-Mismatch_SMA-240522)    | May-25          |

|                                                                                                                 | Name       | Function              | Signature |
|-----------------------------------------------------------------------------------------------------------------|------------|-----------------------|-----------|
| Calibrated by                                                                                                   | Paulo Pina | Laboratory Technician |           |
| Approved by                                                                                                     | Sven Kühn  | Technical Manager     |           |
| Issued: November 12, 2024                                                                                       |            |                       |           |
| This calibration certificate shall not be reproduced except in full without written approval of the laboratory. |            |                       |           |



Accredited by the Swiss Accreditation Service (SAS)  
The Swiss Accreditation Service is one of the signatories to the EA  
Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: **SCS 0108**

## Glossary

|       |                                 |
|-------|---------------------------------|
| TSL   | tissue simulating liquid        |
| ConvF | sensitivity in TSL / NORM x,y,z |
| N/A   | not applicable or not measured  |

## Calibration is Performed According to the Following Standards

- IEC/IEEE 62209-1528, "Measurement Procedure For The Assessment Of Specific Absorption Rate Of Human Exposure To Radio Frequency Fields From Hand-Held And Body-Worn Wireless Communication Devices - Part 1528: Human Models, Instrumentation And Procedures (Frequency Range of 4 MHz to 10 GHz)", October 2020.
- KDB 865664, "SAR Measurement Requirements for 100 MHz to 6 GHz"

## Additional Documentation

- DASY System Handbook

## Methods Applied and Interpretation of Parameters

- *Measurement Conditions:* Further details are available from the Validation Report at the end of the certificate. All figures stated in the certificate are valid at the frequency indicated.
- *Antenna Parameters with TSL:* The dipole is mounted with the spacer to position its feed point exactly below the center marking of the flat phantom section, with the arms oriented parallel to the body axis.
- *Feed Point Impedance and Return Loss:* These parameters are measured with the dipole positioned under the liquid filled phantom. The impedance stated is transformed from the measurement at the SMA connector to the feed point. The Return Loss ensures low reflected power. No uncertainty required.
- *Electrical Delay:* One-way delay between the SMA connector and the antenna feed point. No uncertainty required.
- *SAR measured:* SAR measured at the stated antenna input power.
- *SAR normalized:* SAR as measured, normalized to an input power of 1 W at the antenna connector.
- *SAR for nominal TSL parameters:* The measured TSL parameters are used to calculate the nominal SAR result.

The reported uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor  $k=2$ , which for a normal distribution corresponds to a coverage probability of approximately 95%.

## Measurement Conditions

DASY system configuration, as far as not given on page 1.

|                              |                                                                                      |                                     |
|------------------------------|--------------------------------------------------------------------------------------|-------------------------------------|
| DASY Version                 | DASY8 Module SAR                                                                     | 16.4.0                              |
| Extrapolation                | Advanced Extrapolation                                                               |                                     |
| Phantom                      | Modular Flat Phantom                                                                 |                                     |
| Distance Dipole Center - TSL | 10 mm                                                                                | with spacer                         |
| Zoom Scan Resolution         | dx, dy = 4mm, dz = 1.4mm                                                             | Graded Ratio = 1.4 mm (Z direction) |
| Frequency                    | 5250MHz $\pm$ 1MHz<br>5600MHz $\pm$ 1MHz<br>5750MHz $\pm$ 1MHz<br>5850MHz $\pm$ 1MHz |                                     |

## Head TSL parameters at 5250 MHz

The following parameters and calculations were applied.

|                                         | Temperature        | Permittivity  | Conductivity        |
|-----------------------------------------|--------------------|---------------|---------------------|
| Nominal Head TSL parameters             | 22.0 °C            | 35.9          | 4.71 mho/m          |
| Measured Head TSL parameters            | (22.0 $\pm$ 0.2)°C | 35.8 $\pm$ 6% | 4.58 mho/m $\pm$ 6% |
| Head TSL temperature change during test | < 0.5 °C           |               |                     |

## SAR result with Head TSL at 5250 MHz

| SAR averaged over 1 cm <sup>3</sup> (1 g) of Head TSL | Condition          |                               |
|-------------------------------------------------------|--------------------|-------------------------------|
| SAR for nominal Head TSL parameters                   | 20 dBm input power | 7.79 W/kg                     |
| SAR for nominal Head TSL parameters                   | normalized to 1W   | 77.9 W/kg $\pm$ 19.9% (k = 2) |

| SAR averaged over 10 cm <sup>3</sup> (10 g) of Head TSL | Condition          |                               |
|---------------------------------------------------------|--------------------|-------------------------------|
| SAR for nominal Head TSL parameters                     | 20 dBm input power | 2.25 W/kg                     |
| SAR for nominal Head TSL parameters                     | normalized to 1W   | 22.5 W/kg $\pm$ 19.5% (k = 2) |

**Head TSL parameters at 5600 MHz**

The following parameters and calculations were applied.

|                                         | Temperature   | Permittivity | Conductivity   |
|-----------------------------------------|---------------|--------------|----------------|
| Nominal Head TSL parameters             | 22.0 °C       | 35.5         | 5.07 mho/m     |
| Measured Head TSL parameters            | (22.0 ±0.2)°C | 35.2 ±6%     | 4.96 mho/m ±6% |
| Head TSL temperature change during test | < 0.5 °C      |              |                |

**SAR result with Head TSL at 5600 MHz**

| SAR averaged over 1 cm <sup>3</sup> (1 g) of Head TSL | Condition          |                          |
|-------------------------------------------------------|--------------------|--------------------------|
| SAR for nominal Head TSL parameters                   | 20 dBm input power | 8.18 W/kg                |
| SAR for nominal Head TSL parameters                   | normalized to 1W   | 81.8 W/kg ±19.9% (k = 2) |

| SAR averaged over 10 cm <sup>3</sup> (10 g) of Head TSL | Condition          |                          |
|---------------------------------------------------------|--------------------|--------------------------|
| SAR for nominal Head TSL parameters                     | 20 dBm input power | 2.37 W/kg                |
| SAR for nominal Head TSL parameters                     | normalized to 1W   | 23.7 W/kg ±19.5% (k = 2) |

**Head TSL parameters at 5750 MHz**

The following parameters and calculations were applied.

|                                         | Temperature   | Permittivity | Conductivity   |
|-----------------------------------------|---------------|--------------|----------------|
| Nominal Head TSL parameters             | 22.0 °C       | 35.4         | 5.22 mho/m     |
| Measured Head TSL parameters            | (22.0 ±0.2)°C | 35.0 ±6%     | 5.12 mho/m ±6% |
| Head TSL temperature change during test | < 0.5 °C      |              |                |

**SAR result with Head TSL at 5750 MHz**

| SAR averaged over 1 cm <sup>3</sup> (1 g) of Head TSL | Condition          |                          |
|-------------------------------------------------------|--------------------|--------------------------|
| SAR for nominal Head TSL parameters                   | 20 dBm input power | 8.07 W/kg                |
| SAR for nominal Head TSL parameters                   | normalized to 1W   | 80.7 W/kg ±19.9% (k = 2) |

| SAR averaged over 10 cm <sup>3</sup> (10 g) of Head TSL | Condition          |                          |
|---------------------------------------------------------|--------------------|--------------------------|
| SAR for nominal Head TSL parameters                     | 20 dBm input power | 2.32 W/kg                |
| SAR for nominal Head TSL parameters                     | normalized to 1W   | 23.2 W/kg ±19.5% (k = 2) |

**Head TSL parameters at 5850 MHz**

The following parameters and calculations were applied.

|                                         | Temperature   | Permittivity | Conductivity   |
|-----------------------------------------|---------------|--------------|----------------|
| Nominal Head TSL parameters             | 22.0 °C       | 35.2         | 5.32 mho/m     |
| Measured Head TSL parameters            | (22.0 ±0.2)°C | 34.9 ±6%     | 5.21 mho/m ±6% |
| Head TSL temperature change during test | < 0.5 °C      |              |                |

**SAR result with Head TSL at 5850 MHz**

| SAR averaged over 1 cm <sup>3</sup> (1 g) of Head TSL | Condition          |                          |
|-------------------------------------------------------|--------------------|--------------------------|
| SAR for nominal Head TSL parameters                   | 20 dBm input power | 7.74 W/kg                |
| SAR for nominal Head TSL parameters                   | normalized to 1W   | 77.4 W/kg ±19.9% (k = 2) |

| SAR averaged over 10 cm <sup>3</sup> (10 g) of Head TSL | Condition          |                          |
|---------------------------------------------------------|--------------------|--------------------------|
| SAR for nominal Head TSL parameters                     | 20 dBm input power | 2.22 W/kg                |
| SAR for nominal Head TSL parameters                     | normalized to 1W   | 22.2 W/kg ±19.5% (k = 2) |

**Appendix (Additional assessments outside the scope of SCS 0108)****Antenna Parameters with Head TSL at 5250 MHz**

|             |                                |
|-------------|--------------------------------|
| Impedance   | 48.2 $\Omega$ – 2.3 j $\Omega$ |
| Return Loss | -30.6 dB                       |

**Antenna Parameters with Head TSL at 5600 MHz**

|             |                                |
|-------------|--------------------------------|
| Impedance   | 57.0 $\Omega$ – 0.7 j $\Omega$ |
| Return Loss | -23.7 dB                       |

**Antenna Parameters with Head TSL at 5750 MHz**

|             |                                |
|-------------|--------------------------------|
| Impedance   | 55.3 $\Omega$ + 1.1 j $\Omega$ |
| Return Loss | -25.8 dB                       |

**Antenna Parameters with Head TSL at 5850 MHz**

|             |                                |
|-------------|--------------------------------|
| Impedance   | 55.7 $\Omega$ – 3.6 j $\Omega$ |
| Return Loss | -23.9 dB                       |

**General Antenna Parameters and Design**

|                                  |          |
|----------------------------------|----------|
| Electrical Delay (one direction) | 1.195 ns |
|----------------------------------|----------|

After long term use with 100W radiated power, only a slight warming of the dipole near the feedpoint can be measured. The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals. On some of the dipoles, small end caps are added to the dipole arms in order to improve matching when loaded according to the position as explained in the "Measurement Conditions" paragraph. The SAR data are not affected by this change. The overall dipole length is still according to the Standard. No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feedpoint may be damaged.

**Additional EUT Data**

|                 |       |
|-----------------|-------|
| Manufactured by | SPEAG |
|-----------------|-------|

## System Performance Check Report

## Summary

| Dipole           | Frequency [MHz] | TSL | Power [dBm] |
|------------------|-----------------|-----|-------------|
| D5GHzV2 - SN1066 | 5250            | HSL | 20          |

## Exposure Conditions

| Phantom Section, TSL | Test Distance [mm] | Band | Group, UID | Frequency [MHz], Channel Number | Conversion Factor | TSL Conductivity [S/m] | TSL Permittivity |
|----------------------|--------------------|------|------------|---------------------------------|-------------------|------------------------|------------------|
| Flat                 | 10                 |      | CW, 0--    | 5250, 0                         | 5.39              | 4.58                   | 35.8             |

## Hardware Setup


| Phantom       | TSL, Measured Date | Probe, Calibration Date     | DAE, Calibration Date     |
|---------------|--------------------|-----------------------------|---------------------------|
| MFP V8.0 Left | HSL, 2024-11-08    | EX3DV4 - SN7349, 2024-06-03 | DAE4lp Sn1836, 2024-10-28 |

## Scans Setup

|                     | Zoom Scan       |
|---------------------|-----------------|
| Grid Extents [mm]   | 22 x 22 x 22    |
| Grid Steps [mm]     | 4.0 x 4.0 x 1.4 |
| Sensor Surface [mm] | 1.4             |
| Graded Grid         | Yes             |
| Grading Ratio       | 1.4             |
| MAIA                | N/A             |
| Surface Detection   | All points      |
| Scan Method         | Measured        |

## Measurement Results

|                     | Zoom Scan           |
|---------------------|---------------------|
| Date                | 2024-11-08          |
| psSAR1g [W/Kg]      | 7.79                |
| psSAR10g [W/Kg]     | 2.25                |
| Power Drift [dB]    | 0.03                |
| Power Scaling       | Disabled            |
| Scaling Factor [dB] |                     |
| TSL Correction      | Positive / Negative |

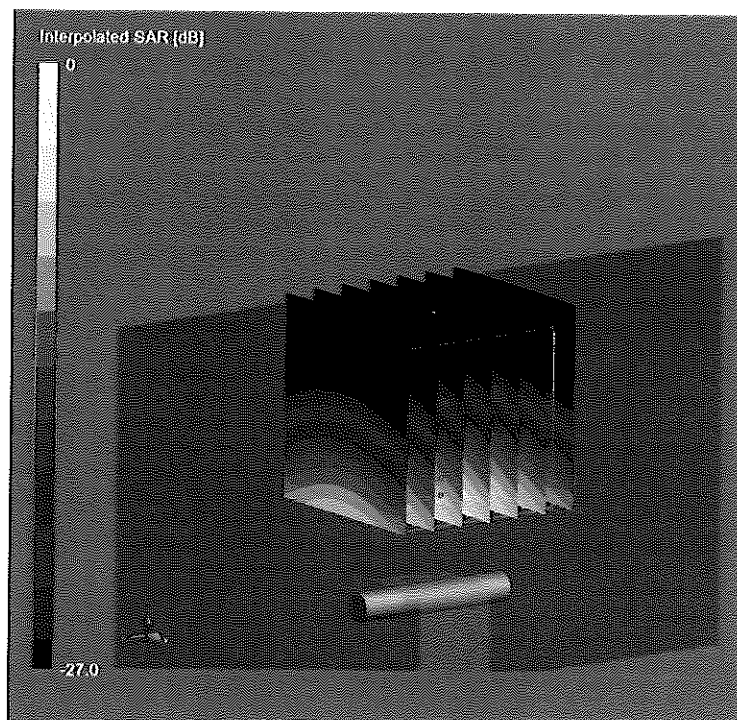

0 dB = 30.9 W/Kg

## System Performance Check Report

## Summary

| Dipole            | Frequency [MHz] | TSL | Power [dBm] |
|-------------------|-----------------|-----|-------------|
| D5GHzV2 -- SN1066 | 5600            | HSL | 20          |

## Exposure Conditions

| Phantom Section, TSL | Test Distance [mm] | Band    | Group, UID | Frequency [MHz], Channel Number | Conversion Factor | TSL Conductivity [S/m] | TSL Permittivity |
|----------------------|--------------------|---------|------------|---------------------------------|-------------------|------------------------|------------------|
| Flat                 | 10                 | CW, 0-- |            | 5600, 0                         | 4.93              | 4.96                   | 35.2             |

## Hardware Setup


| Phantom       | TSL, Measured Date | Probe, Calibration Date      | DAE, Calibration Date     |
|---------------|--------------------|------------------------------|---------------------------|
| MFP V8.0 Left | HSL, 2024-11-08    | EX3DV4 -- SN7349, 2024-06-03 | DAE4lp Sn1836, 2024-10-28 |

## Scans Setup

|                     | Zoom Scan       |
|---------------------|-----------------|
| Grid Extents [mm]   | 22 x 22 x 22    |
| Grid Steps [mm]     | 4.0 x 4.0 x 1.4 |
| Sensor Surface [mm] | 1.4             |
| Graded Grid         | Yes             |
| Grading Ratio       | 1.4             |
| MAIA                | N/A             |
| Surface Detection   | All points      |
| Scan Method         | Measured        |

## Measurement Results

|                     | Zoom Scan           |
|---------------------|---------------------|
| Date                | 2024-11-08          |
| psSAR1g [W/Kg]      | 8.18                |
| psSAR10g [W/Kg]     | 2.37                |
| Power Drift [dB]    | -0.09               |
| Power Scaling       | Disabled            |
| Scaling Factor [dB] |                     |
| TSL Correction      | Positive / Negative |

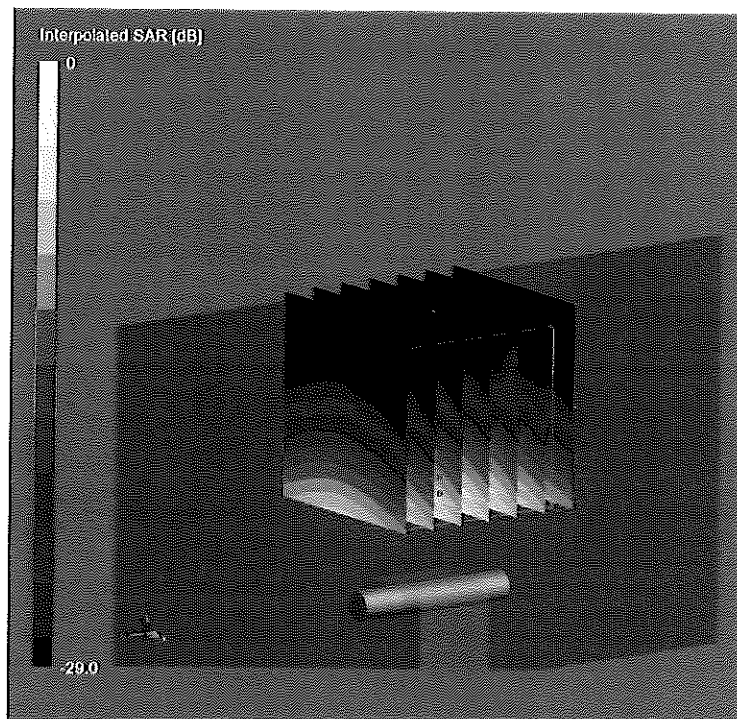

0 dB = 35.1 W/Kg

System Performance Check Report

Summary

| Dipole           | Frequency [MHz] | TSL | Power [d8m] |
|------------------|-----------------|-----|-------------|
| D5GHzV2 - SN1066 | 5750            | HSL | 20          |

Exposure Conditions

| Phantom Section, TSL | Test Distance [mm] | Band    | Group, UID | Frequency [MHz], Channel Number | Conversion Factor | TSL Conductivity [S/m] | TSL Permittivity |
|----------------------|--------------------|---------|------------|---------------------------------|-------------------|------------------------|------------------|
| Flat                 | 10                 | CW, 0-- | 5750, 0    |                                 | 4.93              | 5.12                   | 35.0             |

Hardware Setup


| Phantom       | TSL, Measured Date | Probe, Calibration Date     | DAE, Calibration Date     |
|---------------|--------------------|-----------------------------|---------------------------|
| MFP V8.0 Left | HSL, 2024-11-08    | EX3DV4 - SN7349, 2024-06-03 | DAE4lp Sn1836, 2024-10-28 |

Scans Setup

|                     | Zoom Scan       |
|---------------------|-----------------|
| Grid Extents [mm]   | 22 x 22 x 22    |
| Grid Steps [mm]     | 4.0 x 4.0 x 1.4 |
| Sensor Surface [mm] | 1.4             |
| Graded Grid         | Yes             |
| Grading Ratio       | 1.4             |
| MAIA                | N/A             |
| Surface Detection   | All points      |
| Scan Method         | Measured        |

Measurement Results

|                     | Zoom Scan           |
|---------------------|---------------------|
| Date                | 2024-11-08          |
| psSAR1g [W/Kg]      | 8.07                |
| psSAR10g [W/Kg]     | 2.32                |
| Power Drift [dB]    | 0.00                |
| Power Scaling       | Disabled            |
| Scaling Factor [dB] |                     |
| TSL Correction      | Positive / Negative |

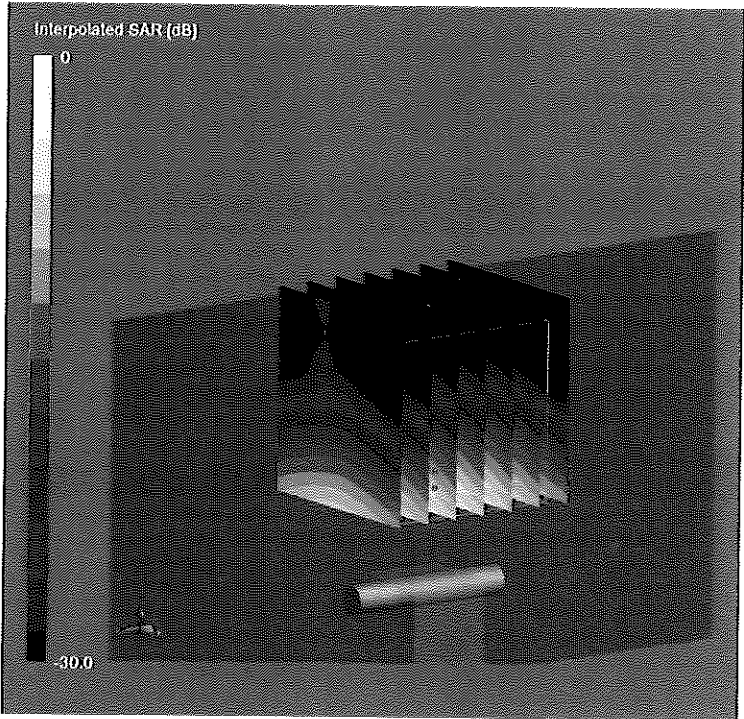

0 dB = 35.6 W/Kg

System Performance Check Report

Summary

| Dipole           | Frequency [MHz] | TSL | Power [dBm] |
|------------------|-----------------|-----|-------------|
| D5GHzV2 - SN1066 | 5850            | HSL | 20          |

Exposure Conditions

| Phantom Section, TSL | Test Distance [mm] | Band | Group, UID | Frequency [MHz], Channel Number | Conversion Factor | TSL Conductivity [S/m] | TSL Permittivity |
|----------------------|--------------------|------|------------|---------------------------------|-------------------|------------------------|------------------|
| Flat                 | 10                 |      | CW, 0--    | 5850, 0                         | 4.96              | 5.21                   | 34.9             |

Hardware Setup


| Phantom       | TSL, Measured Date | Probe, Calibration Date     | DAE, Calibration Date     |
|---------------|--------------------|-----------------------------|---------------------------|
| MFP V8.0 Left | HSL, 2024-11-08    | EX3DV4 - SN7349, 2024-06-03 | DAE4lp Sn1836, 2024-10-28 |

Scans Setup

|                     | Zoom Scan       |
|---------------------|-----------------|
| Grid Extents [mm]   | 22 x 22 x 22    |
| Grid Steps [mm]     | 4.0 x 4.0 x 1.4 |
| Sensor Surface [mm] | 1.4             |
| Graded Grid         | Yes             |
| Grading Ratio       | 1.4             |
| MAIA                | N/A             |
| Surface Detection   | All points      |
| Scan Method         | Measured        |

Measurement Results

|                     | Zoom Scan           |
|---------------------|---------------------|
| Date                | 2024-11-08          |
| psSAR1g [W/Kg]      | 7.74                |
| psSAR10g [W/Kg]     | 2.22                |
| Power Drift [dB]    | -0.09               |
| Power Scaling       | Disabled            |
| Scaling Factor [dB] |                     |
| TSL Correction      | Positive / Negative |

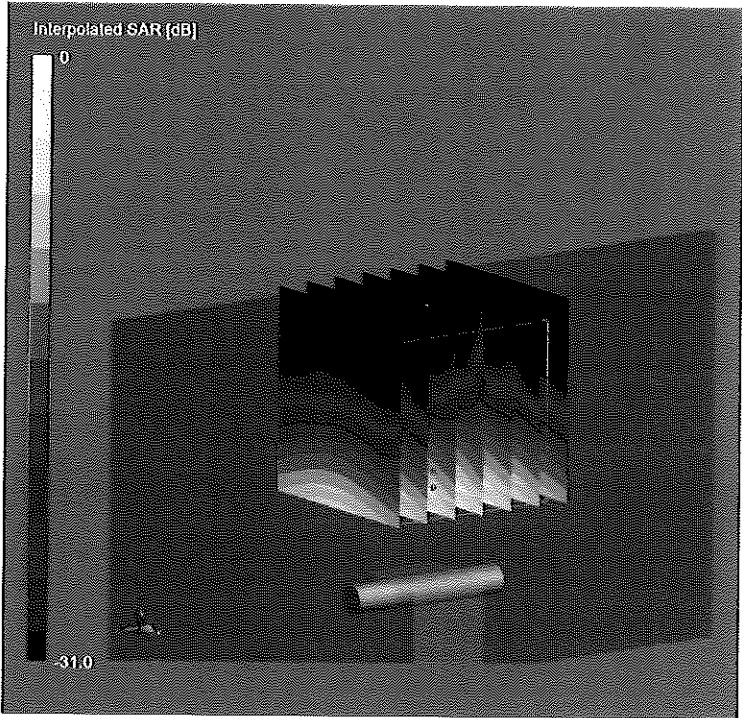

0 dB = 35.0 W/Kg

## Impedance Measurement Plot for Head TSL

