

Client C&C Taiwan (Auden)

## CALIBRATION CERTIFICATE

Object(s) D5GH2V2 - SN 1004

Calibration procedure(s) QA CAL-05 v2  
Calibration procedure for dipole validation kits

Calibration date: October 5, 2003



Condition of the calibrated item In Tolerance (according to the specific calibration document)

This calibration statement documents traceability of M&TE used in the calibration procedures and conformity of the procedures with the ISO/IEC 17025 international standard.

All calibrations have been conducted in the closed laboratory facility: environment temperature 22 +/- 2 degrees Celsius and humidity < 75%.

Calibration Equipment used (M&TE critical for calibration)

| Model Type                        | ID #           | Cal Date (Calibrated by, Certificate No.) | Scheduled Calibration  |
|-----------------------------------|----------------|-------------------------------------------|------------------------|
| Power meter EPM E4419B            | GB41293874     | 2-Apr-03 (METAS, No 252-0250)             | Apr-04                 |
| Power sensor E4412A               | MY41495277     | 2-Apr-03 (METAS, No 252-0250)             | Apr-04                 |
| Reference 20 dB Attenuator        | SN: 5086 (20b) | 3-Apr-03 (METAS No. 251-0340)             | Apr-04                 |
| Fluke Process Calibrator Type 702 | SN: 6295803    | 8-Sep-03 (Sintrel SCS No. E-030020)       | Sep-04                 |
| Power sensor HP 8481A             | MY41082180     | 18-Sep-02 (Agilent, No. 20020918)         | In house check: Oct 03 |
| RF generator R&S SMT06            | 100058         | 23-May-01 (SPEAG, in house check May-03)  | In house check: May-05 |
| Network Analyzer HP 8753E         | US37390685     | 18-Oct-01 (Agilent, No. 24BR1033101)      | In house check: Oct 03 |

|                | Name          | Function            | Signature                                                                             |
|----------------|---------------|---------------------|---------------------------------------------------------------------------------------|
| Calibrated by: | Katia Pokorny | Laboratory Director |  |
| Approved by:   | Heidi Kuster  | Quality Manager     |  |

Date issued: October 6, 2003

This calibration certificate is issued as an intermediate solution until the accreditation process (based on ISO/IEC 17025 International Standard) for Calibration Laboratory of Schmid & Partner Engineering AG is completed.

# DASY

## Dipole Validation Kit

Type: D5GHzV2

Serial: 1004

Manufactured: July 8, 2003

Calibrated: October 5, 2003

## 1. Measurement Conditions

The measurements were performed in the flat section of the SAM twin phantom filled with head simulating solution of the following electrical parameters:

|                        |            |      |
|------------------------|------------|------|
| Frequency:             | 5200 MHz   |      |
| Relative Dielectricity | 36.3       | ± 5% |
| Conductivity           | 4.57 mho/m | ± 5% |
| Frequency:             | 5800 MHz   |      |
| Relative Dielectricity | 35.4       | ± 5% |
| Conductivity           | 5.20 mho/m | ± 5% |

The DASY3 System with a dosimetric E-field probe ES3DV3 - SN:3025 was used for the measurements. The dipole was mounted on the small tripod so that the dipole feedpoint was positioned below the center marking of the flat phantom section and the dipole was oriented parallel to the body axis (the long side of the phantom). The standard measuring distance was 10mm from dipole center to the solution surface. Lossless spacer was used during measurements for accurate distance positioning.

The coarse grid with a grid spacing of 10mm was aligned with the dipole. Special 8x8x8 fine cube was chosen for cube integration ( $dx=dy=4.3\text{mm}$ ,  $dz=3\text{mm}$ ). Distance between probe sensors and phantom surface was set to 3.0 mm. The dipole input power (forward power) was  $250\text{mW} \pm 3\%$ . The results are normalized to 1W input power.

## 2. SAR Measurement with DASY System

Standard SAR-measurements were performed according to the measurement conditions described in section 1. The results (see figures supplied) have been normalized to a dipole input power of 1W (forward power). The resulting averaged SAR-values measured at 5200 MHz (Head Tissue) with the dosimetric probe ES3DV3 SN:3025 and applying the advanced extrapolation are:

|                                                  |                                       |
|--------------------------------------------------|---------------------------------------|
| averaged over $1\text{ cm}^3$ (1 g) of tissue:   | $86.0\text{ mW/g} \pm 32.0\% (k=2)^1$ |
| averaged over $10\text{ cm}^3$ (10 g) of tissue: | $23.8\text{ mW/g} \pm 31.7\% (k=2)^1$ |

The resulting averaged SAR-values measured at 5800 MHz (Head Tissue) with the dosimetric probe ES3DV3 SN:3025 and applying the advanced extrapolation are:

|                                                  |                                       |
|--------------------------------------------------|---------------------------------------|
| averaged over $1\text{ cm}^3$ (1 g) of tissue:   | $88.8\text{ mW/g} \pm 32.0\% (k=2)^2$ |
| averaged over $10\text{ cm}^3$ (10 g) of tissue: | $24.4\text{ mW/g} \pm 31.7\% (k=2)^2$ |

<sup>1</sup> Target dipole values determined by FDTD (feedpoint impedance set to 50 Ohm). The values are SAR<sub>1g</sub>=76.5 mW/g, SAR<sub>10g</sub>=21.6 mW/g and SAR<sub>peak</sub>=310.3 mW/g.

<sup>2</sup> Target dipole values determined by FDTD (feedpoint impedance set to 50 Ohm). The values are SAR<sub>1g</sub>=78.0 mW/g, SAR<sub>10g</sub>=21.9 mW/g and SAR<sub>peak</sub>=340.9 mW/g.

### 3. Dipole Transformation Parameters

The impedance was measured at the SMA-connector with a network analyzer and numerically transformed to the dipole feedpoint (please refer to the graphics attached to this document). The transformation parameters from the SMA-connector to the dipole feedpoint are:

|                      |          |                                       |
|----------------------|----------|---------------------------------------|
| Electrical delay:    | 1.153 ns | (one direction)                       |
| Transmission factor: | 0.954    | (voltage transmission, one direction) |

### 4. Measurement Conditions

The measurements were performed in the flat section of the SAM twin phantom filled with body simulating solution of the following electrical parameters:

|                        |            |      |
|------------------------|------------|------|
| Frequency:             | 5200 MHz   |      |
| Relative Dielectricity | 49.7       | ± 5% |
| Conductivity           | 5.18 mho/m | ± 5% |
| Frequency:             | 5800 MHz   |      |
| Relative Dielectricity | 48.5       | ± 5% |
| Conductivity           | 6.01 mho/m | ± 5% |

The DASY3 System with a dosimetric E-field probe ES3DV3 - SN:3025 was used for the measurements. The dipole was mounted on the small tripod so that the dipole feedpoint was positioned below the center marking of the flat phantom section and the dipole was oriented parallel to the body axis (the long side of the phantom). The standard measuring distance was 10mm from dipole center to the solution surface. Lossless spacer was used during measurements for accurate distance positioning.

The coarse grid with a grid spacing of 10mm was aligned with the dipole. The 8x8x8 fine cube was chosen for cube integration (dx=dy=4.3mm, dz=3mm). Distance between probe sensors and phantom surface was set to 3.0 mm. The dipole input power (forward power) was 250mW ± 3 %. The results are normalized to 1W input power.

## **5. SAR Measurement with DASY System**

Standard SAR-measurements were performed according to the measurement conditions described in section 4. The results (see figures supplied) have been normalized to a dipole input power of 1W (forward power). The resulting averaged SAR-values measured at **5200 MHz (Body Tissue)** with the dosimetric probe ES3DV3 SN:3025 and applying the advanced extrapolation are:

averaged over 1 cm<sup>3</sup> (1 g) of tissue: **84.0 mW/g  $\pm$  32.0 % (k=2)<sup>3</sup>**

averaged over 10 cm<sup>3</sup> (10 g) of tissue: **23.4 mW/g  $\pm$  31.7 % (k=2)<sup>3</sup>**

The resulting averaged SAR-values measured at **5800 MHz (Body Tissue)** with the dosimetric probe ES3DV3 SN:3025 and applying the advanced extrapolation are:

averaged over 1 cm<sup>3</sup> (1 g) of tissue: **80.0 mW/g  $\pm$  32.0 % (k=2)<sup>4</sup>**

averaged over 10 cm<sup>3</sup> (10 g) of tissue: **22.4 mW/g  $\pm$  31.7 % (k=2)<sup>4</sup>**

## **6. Handling**

Do not apply excessive force to the dipole arms, because they might bend. Bending of the dipole arms stresses the soldered connections near the feedpoint leading to a damage of the dipole.

## **7. Design**

The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals.

Small end caps have been added to the dipole arms in order to increase frequency bandwidth at the position as explained in Sections 1 and 4.

## **8. Power Test**

After long term use with 40W radiated power, only a slight warming of the dipole near the feedpoint can be measured.

<sup>3</sup> Target dipole values determined by FDTD (feedpoint impedance set to 50 Ohm). The values are SAR\_1g=71.8 mW/g, SAR\_10g=20.1 mW/g and SAR\_peak=284.7 mW/g.

<sup>4</sup> Target dipole values determined by FDTD (feedpoint impedance set to 50 Ohm). The values are SAR\_1g=74.1 mW/g, SAR\_10g=20.5 mW/g and SAR\_peak=324.7 mW/g.

## SPEAG Calibration Laboratory

**DUT: Dipole 5GHz; Type: D5GHz; Serial: D5GHzV2 - SN:1004**

Communication System: CW-5GHz; Frequency: 5200 MHz; Duty Cycle: 1:1

Medium: HSL5800 ( $\sigma = 4.57$  mho/m,  $\epsilon_r = 36.34$ ,  $\rho = 1000$  kg/m<sup>3</sup>)

Phantom section: Flat Section

## DASY4 Configuration:

- Probe: ES3DV3 - SN3025-Y2003; ConvF(2.65, 2.65, 2.65); Calibrated: 9/19/2003
- Sensor-Surface: 3mm (Mechanical Surface Detection)
- Electronics: DAE3 Sn410; Calibrated: 4/22/2003
- Phantom: SAM 12b; Type: SAM 4.0; Serial: TP:1197
- Measurement SW: DASY4, V4.1 Build 47; Postprocessing SW: SEMCAD, V1.8 Build 60

d=10mm, Pin=250mW, f=5200 MHz/Area Scan (91x91x1): Measurement grid: dx=10mm, dy=10mm

Reference Value = 91.5 V/m

Power Drift = -0.001 dB

Maximum value of SAR = 33.2 mW/g

d=10mm, Pin=250mW, f=5200 MHz/Zoom Scan (8x8x8), dist=3mm (7x7x8)/Cube 0: Measurement grid: dx=4.3mm, dy=4.3mm, dz=3mm


Peak SAR (extrapolated) = 98.6 W/kg

SAR(1 g) = 21.5 mW/g; SAR(10 g) = 5.94 mW/g

Reference Value = 91.5 V/m

Power Drift = -0.001 dB

Maximum value of SAR = 30.2 mW/g

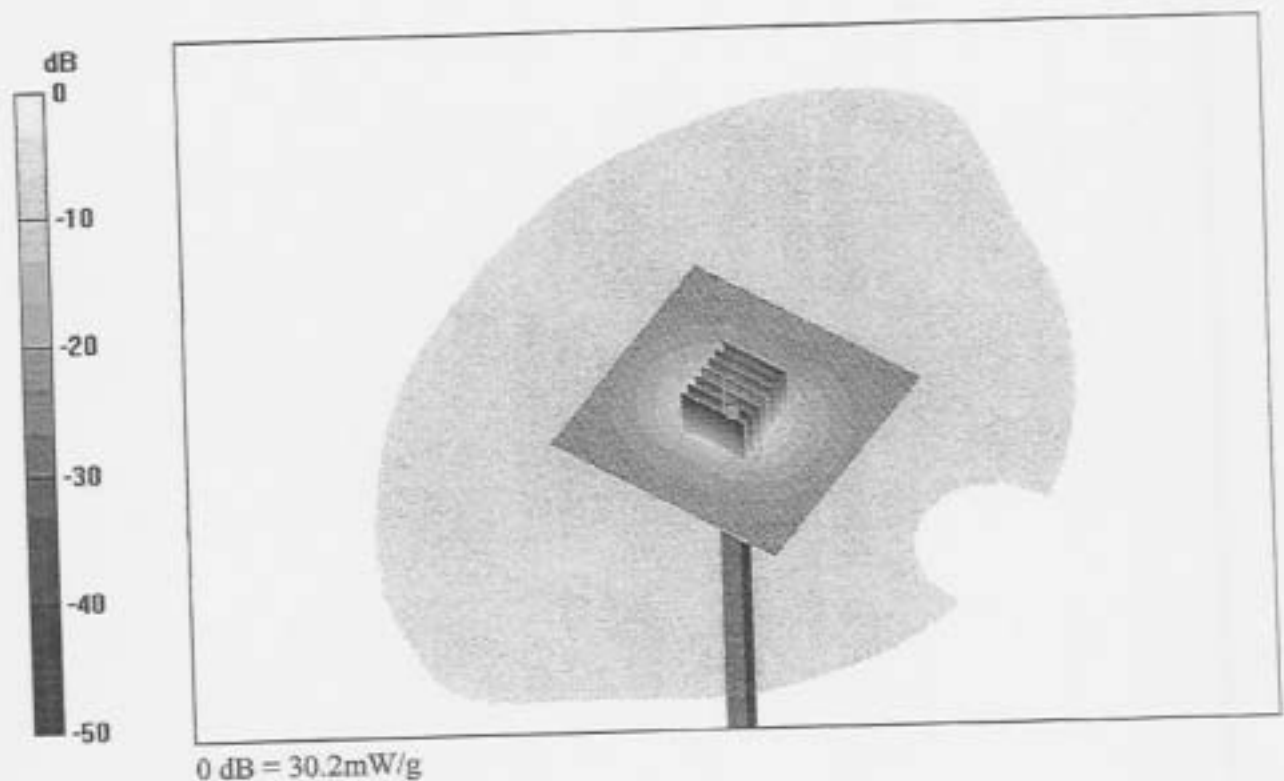

SPEAG Calibration Laboratory

**DUT: Dipole 5GHz; Type: D5GHz; Serial: D5GHzV2 - SN:1004**

Communication System: CW-5GHz; Frequency: 5800 MHz; Duty Cycle: 1:1

Medium: HSL5800 ( $\sigma = 5.2 \text{ mho/m}$ ,  $\epsilon_r = 35.39$ ,  $\rho = 1000 \text{ kg/m}^3$ )

Phantom section: Flat Section

DASY4 Configuration:

- Probe: ES3DV3 - SN3025-Y2003; ConvF(2.3, 2.3, 2.3); Calibrated: 9/19/2003
- Sensor-Surface: 3mm (Mechanical Surface Detection)
- Electronics: DAE3 Sn410; Calibrated: 4/22/2003
- Phantom: SAM 12b; Type: SAM 4.0; Serial: TP:1197
- Measurement SW: DASY4, V4.1 Build 47; Postprocessing SW: SEMCAD, V1.8 Build 60

**d=10mm, Pin=250mW, f=5800 MHz/Area Scan (91x91x1):** Measurement grid: dx=10mm, dy=10mm

Reference Value = 84.8 V/m

Power Drift = -0.0 dB

Maximum value of SAR = 33.1 mW/g

**d=10mm, Pin=250mW, f=5800 MHz/Zoom Scan (8x8x8), dist=3mm (7x7x8)/Cube 0:** Measurement grid: dx=4.3mm, dy=4.3mm, dz=3mm


Peak SAR (extrapolated) = 114.0 W/kg

SAR(1 g) = 22.2 mW/g; SAR(10 g) = 6.1 mW/g

Reference Value = 84.8 V/m

Power Drift = -0.0 dB


Maximum value of SAR = 30 mW/g

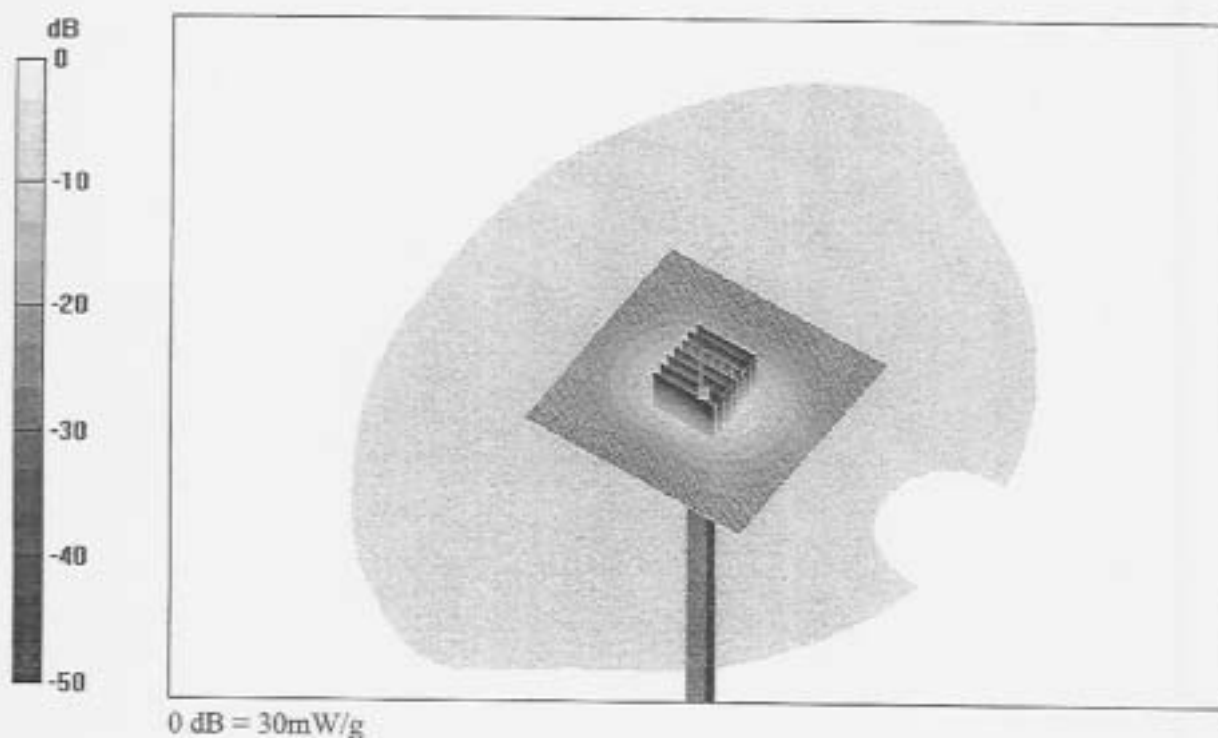

1004  
Head

4 Oct 2003 12:58:01  
CH1 S11 1 U FS 2149.600 a -9.4551 a 3.2371 pF 5 200.000 000 MHz

De1  
Cor

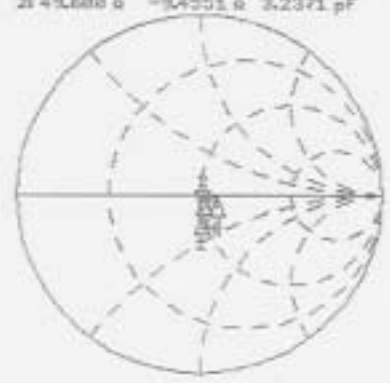


CH1 Markers

1: 40.547 a  
-11.793 a  
5.10000 GHz  
3: 51.215 a  
-1.6916 a  
5.50000 GHz  
4: 50.904 a  
-2.6157 a  
5.50000 GHz

CH2 S11 L06 5 dB/REF -20 dB 20-20.481 dB 5 200.000 000 MHz

Sec  
Cor  
Avg  
16  
†

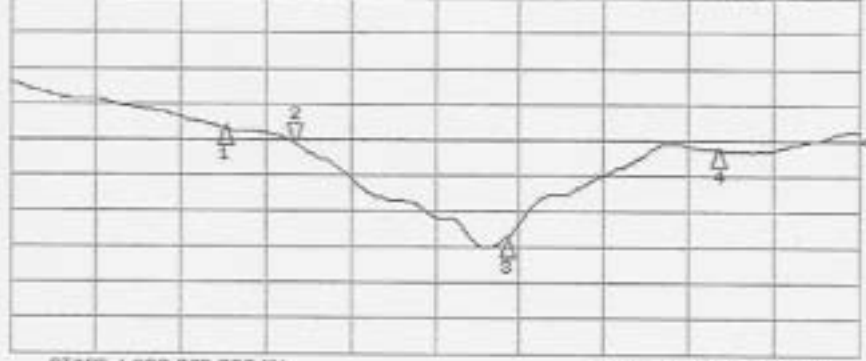

CH2 Markers

1: -18.463 dB  
5.10000 GHz  
3: -33.833 dB  
5.50000 GHz  
4: -21.414 dB  
5.60000 GHz

START 4 000.000 000 MHz

STOP 5 000.000 000 MHz

SPEAG Calibration Laboratory

**DUT: Dipole 5GHz; Type: D5GHz; Serial: D5GHzV2 - SN:1004**

Communication System: CW-5GHz; Frequency: 5200 MHz; Duty Cycle: 1:1

Medium: MSL5800 ( $\sigma = 5.18 \text{ mho/m}$ ,  $\epsilon_r = 49.73$ ,  $\rho = 1000 \text{ kg/m}^3$ )

Phantom section: Flat Section

DASY4 Configuration:

- Probe: ES3DV3 - SN3025-Y2003; ConvF(1.93, 1.93, 1.93); Calibrated: 9/19/2003
- Sensor-Surface: 3mm (Mechanical Surface Detection)
- Electronics: DAE3 Sn410; Calibrated: 4/22/2003
- Phantom: SAM 12b; Type: SAM 4.0; Serial: TP:1197
- Measurement SW: DASY4, V4.1 Build 47; Postprocessing SW: SEMCAD, V1.8 Build 60

**d=10mm, Pin=250mW, f=5200 MHz/Area Scan (91x91x1):** Measurement grid: dx=10mm, dy=10mm

Reference Value = 86.6 V/m

Power Drift = -0.0 dB

Maximum value of SAR = 33.4 mW/g

**d=10mm, Pin=250mW, f=5200 MHz/Zoom Scan (8x8x8), dist=3mm (7x7x8)/Cube 0:** Measurement grid: dx=4.3mm, dy=4.3mm, dz=3mm


Peak SAR (extrapolated) = 80.6 W/kg

SAR(1 g) = 21 mW/g; SAR(10 g) = 5.84 mW/g

Reference Value = 86.6 V/m

Power Drift = -0.0 dB

Maximum value of SAR = 31 mW/g

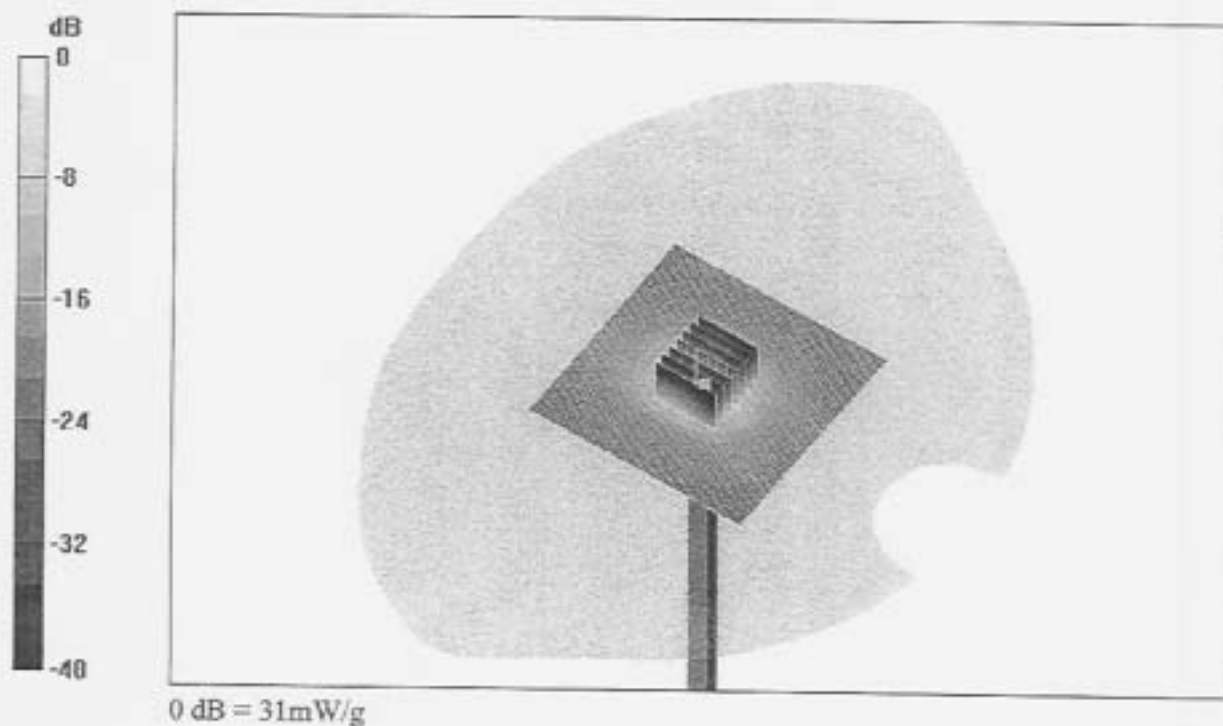

SPEAG Calibration Laboratory

**DUT: Dipole 5GHz; Type: D5GHz; Serial: D5GHzV2 - SN:1004**

Communication System: CW-5GHz; Frequency: 5800 MHz; Duty Cycle: 1:1

Medium: MSL5800 ( $\sigma = 6.01$  mho/m,  $\epsilon_r = 48.51$ ,  $\rho = 1000$  kg/m<sup>3</sup>)

Phantom section: Flat Section

DASY4 Configuration:

- Probe: ES3DV3 - SN3025-Y2003; ConvF(1.65, 1.65, 1.65); Calibrated: 9/19/2003
- Sensor-Surface: 3mm (Mechanical Surface Detection)
- Electronics: DAE3 Sn410; Calibrated: 4/22/2003
- Phantom: SAM 12b; Type: SAM 4.0; Serial: TP:1197
- Measurement SW: DASY4, V4.1 Build 47; Postprocessing SW: SEMCAD, V1.8 Build 60

**d=10mm, Pin=250mW, f=5800 MHz/Area Scan (91x91x1):** Measurement grid: dx=10mm, dy=10mm

Reference Value = 82 V/m

Power Drift = -0.0008 dB

Maximum value of SAR = 31.6 mW/g

**d=10mm, Pin=250mW, f=5800 MHz/Zoom Scan (8x8x8), dist=3mm (7x7x8)/Cube 0:** Measurement grid: dx=4.3mm, dy=4.3mm, dz=3mm


Peak SAR (extrapolated) = 80.3 W/kg

SAR(1 g) = 20 mW/g; SAR(10 g) = 5.61 mW/g

Reference Value = 82 V/m

Power Drift = -0.0008 dB

Maximum value of SAR = 29.1 mW/g

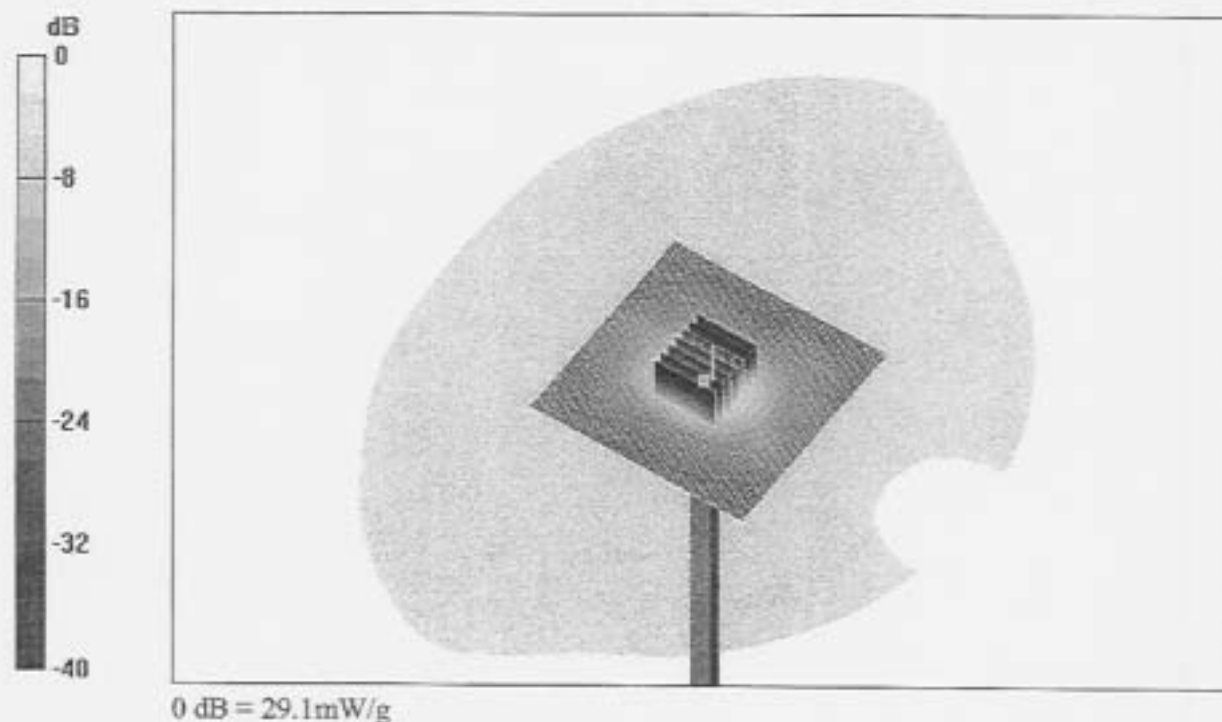

1004  
Body

5 Oct 2003 12:29:16  
CH1 S11 1 U FS 2148.492 a -8.7637 a 3.4925 pF 5.200.000 000 MHz

Del

Cor



CH1 Markers

1: 48.424 a  
-10.598 a  
5.10000 GHz  
3: 51.492 a  
-445.22 a0  
5.50000 GHz  
4: 60.572 a  
-324.22 a0  
5.80000 GHz

†

CH2 S11 LOS 5 dB/REF -20 dB 20-21.167 dB 5.200.000 000 MHz


Seo

Cor

avg

16

†

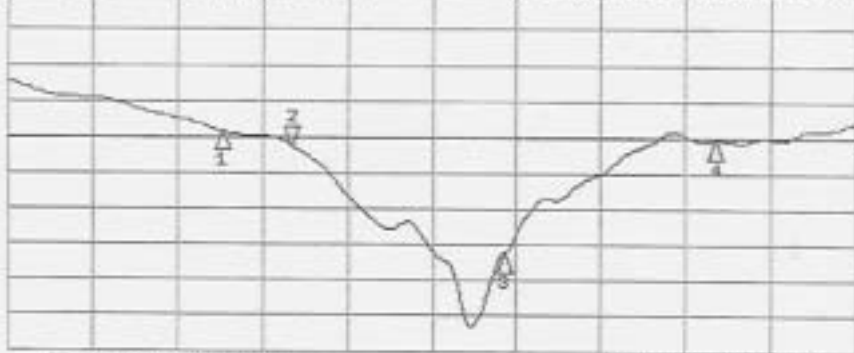

START 4.800.000 000 MHz

STOP 6.000.000 000 MHz

CH2 Markers

1: -19.201 dB  
5.10000 GHz  
3: -26.359 dB  
5.50000 GHz  
4: -28.392 dB  
5.80000 GHz