

Pictures for the Report

Dosimetric Assessment of the Portable Device Clear-Com BP1G9 (FCC ID: BYMBP1G9) (IC: 1860A-BP1G9)

According to the FCC Requirements

June 05, 2014

IMST GmbH

Carl-Friedrich-Gauß-Str. 2 - 4
D-47475 Kamp-Lintfort

Customer

HM Electronics, Inc.
14110 Stowe Drive, Poway
CA 92064
USA

The test results only relate to the items tested.

This report shall not be reproduced except in full without the written approval of the testing laboratory.

Subject of Investigation



Fig. 1: Pictures of the device under test.

7.9 Pictures of the Device under Test

Figure 7 - 8 show the device under test.



Fig. 7: Front view of the device under test.



Fig. 8: Back view of the device under test.

7.10 Test Positions for the Device under Test

Figure 9- 14 show the test positions for the SAR measurements.



Fig. 9: Body worn configuration for Clear-Com BP1G9, position 1, front side towards the phantom, 0 mm distance.



Fig. 10: Body worn configuration for Clear-Com BP1G9, position 2, back side towards the phantom, 0 mm distance.



Fig. 11: Body worn configuration for Clear-Com BP1G9, position 3, top edge towards the phantom, 0 mm distance.

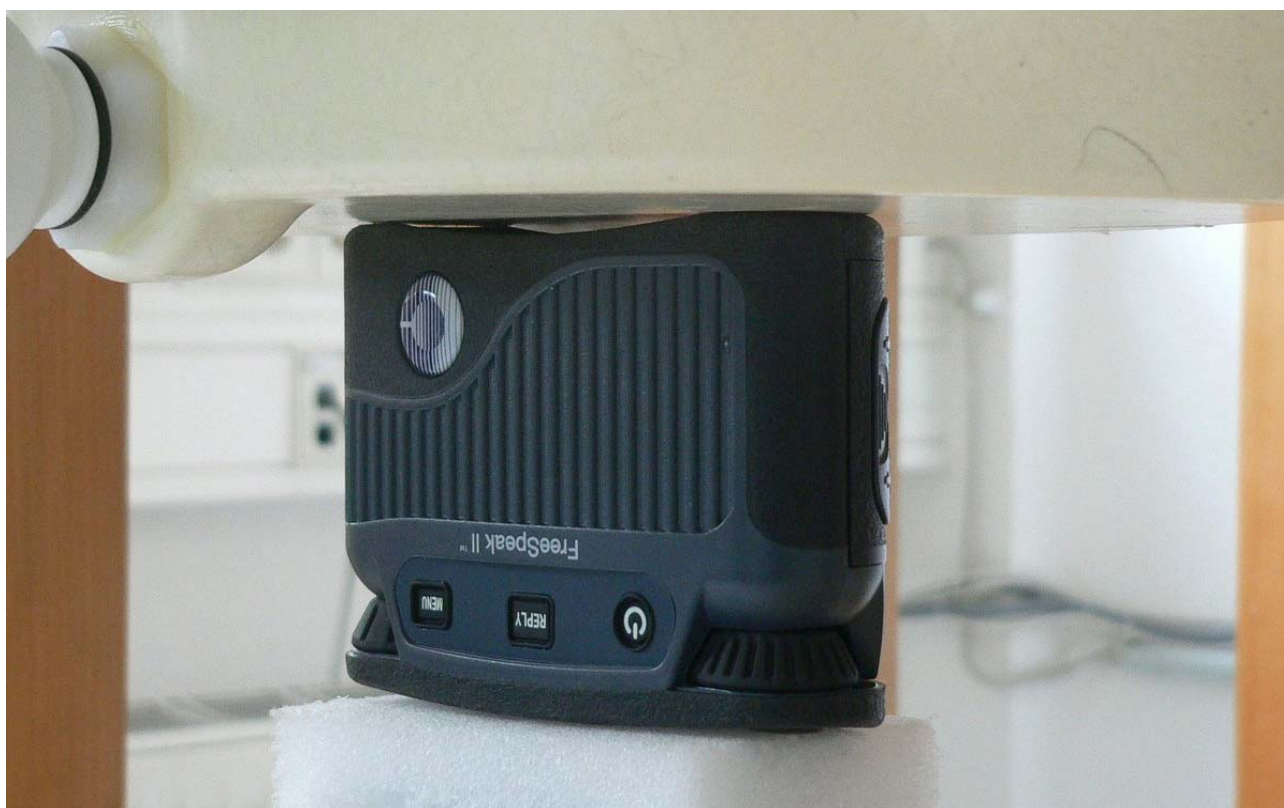


Fig. 12: Body worn configuration for Clear-Com BP1G9, position 4, bottom edge towards the phantom, 0 mm distance.



Fig. 13: Body worn configuration for Clear-Com BP1G9, position 5, left edge towards the phantom, 0 mm distance.



Fig. 14: Body worn configuration for Clear-Com BP1G9, position 6, right edge towards the phantom, 0 mm distance.