

Part 15.231, ANSI C63.4 , RSS 210

This is a list of all test equipment used.

Test Equipment list for Honeywell OATS & Conducted Line:

Equipment	Mfg	Model	Cal Date	Cal Due
Spectrum Analyzer	Rohde & Schwarz	FSEA20	10/19/11	10/19/12
Antenna ('Biconilog')	ETS (EMCO)Lindgren	3149	08/22/11	08/22/12
Surge Suppressor	Agilent (HP)	HP11947A	05/12/11	05/12/12
LISN	Com-Power	LI-115	10/20/11	10/20/12

PLEASE SEE PAGE 2-7 FOR TEST EQUIPMENT TRACEABILITY

If you need any additional information from Honeywell please contact:

Greg Barbato RF Engineer
(Acting for Ken Eskildsen)
Phone (Direct): (516) 577-5863
Email: greg.barbato@honeywell.com

Certificate of Calibration

Issue Date: 10/19/2011



General Calibration, Inc.
2 Mars Court, Boonton, New Jersey 07005
Phone (973) 299-2950 Fax (973) 299-0595

Certificate #: MR-19809
Work Order #: MR504
Customer #: 001464

Performed By:

GENERAL CALIBRATION, INC.

Location of Calibration:

HONEYWELL SECURITY (001464)

2 MARS COURT
BOONTON, NJ 07005

2 CORPORATE CENTER DRIVE
MELVILLE, NY 11747

Equipment Information:

Job No.: 018674
Manufacturer: R&S
Description: SPECTRUM ANALYZER
Department: ALARMNET
Temp./RH: 22 C / 45 %
Cal. Interval: 12 MONTHS
Cal Date: 10/19/2011

Purchase Order: 5247582

Asset Tag No.: 10503
Model Number: FSEA20
Serial Number: DE31589
Inspected By: MR1
Job Title: METROLOGIST
Calibration Result: PASSED
Cal. Due Date: 10/19/2012

Calibration Notes:

Condition: Found In Tolerance and Left In Tolerance

Procedures #GCP: RS FSEA20

Standards Used To Calibrate Equipment

Company	I.D.	Description	Cal. Due Date
GENERAL CALIBRATION	1001	ATTENUATOR	10/26/2011
GENERAL CALIBRATION	332	FREQUENCY COUNTER	04/20/2012
GENERAL CALIBRATION	446	SYNTHESIZED SWEEPER	01/05/2012
GENERAL CALIBRATION	690	POWER METER	04/26/2012
GENERAL CALIBRATION	774	POWER SENSOR	07/08/2012
GENERAL CALIBRATION	967	FUNCTION GENERATOR	10/05/2012

This is to certify that General Calibration, Inc. is A2LA accredited and that its calibration system is in compliance with ISO/IEC 17025-2005, ANSI NCSL Z540-1, ANSI NCSL Z540-3, and ISO 9001:2008. The test limits stated in the report correspond to the published specifications of the equipment, at the points tested. Calibration of standards, reference standards and Intermediate standards in this calibration have been certified traceable to the SI Units of measurement. Any accredited calibration under our A2LA scope of accreditation is denoted with A2LA accredited symbol on the calibration certificate. If the certificate includes any unaccredited items calibrated, they are clearly marked as unaccredited calibration.

Best Uncertainties represent expanded uncertainties expressed at approximately the 95% confidence level using a coverage factor of k=2. The results documented in this certificate relate only to the item(s) calibrated or tested.

Approved By _____

Richard D. Miller
General Calibration, Inc. - Q. A. Manager



ETS-LINDGREN™

An ESCO Technologies Company

1301 Arrow Point Drive
Cedar Park, Texas 78613
(512) 531-6498

Cert I.D.: 86798

Certificate of Calibration Conformance

Page 1 of 5

The instrument identified below has been individually calibrated in compliance with the following standard(s):

SAE, ARP-958 - 2003, Electromagnetic Interference Measurement Antennas; Standard Calibration Method, Society of Automotive Engineers, Aerospace Recommended Practice. Fixed height, three antenna rotation, 1 meter separation. 3 meter separation performed per Annex C. Vertical calibration performed per above listed methodology.

Environment: Laboratory MTE is maintained in a temperature controlled environment with ambient conditions from 18 to 28 C, relative humidity less than 90%. The instrument under test has been calibrated on an open air test site (OATS) with environment temperature conditions ranging from 0 to 40 C which has no known influences on measurement quality.

Manufacturer:	ETS-Lindgren	Operating Range:	80 MHz - 6 GHz
Model Number:	3149.	Instrument Type:	Biconilog (Type 5)
Serial Number/ ID:	00045682	Date Code:	
Tracking Number:	S 000023192	Alternate ID:	11242
Date Completed:	22-Aug-11	Customer:	HONEYWELL (NY)
Test Type:	3 meter, Horizontal and Vertical		
Calibration Uncertainty:	01m	26 - 1000 MHz, +/-0.9 dB; 1000 - 2000 MHz, +/-0.8 dB; 2000 - 6000 MHz, +/-1.2 dB	
k=2, (95% Confidence Level)	03m	26 - 1000 MHz, +/-0.9 dB; 1000 - 2000 MHz, +/-0.8 dB; 2000 - 6000 MHz, +/-1.3 dB	
	10m	26 - 1000 MHz, +/-1.0 dB; 1000 - 2000 MHz, +/-1.4 dB; 2000 - 6000 MHz, +/-2.3 dB	

Test Remarks: Calibrated down to 26 MHz. per customer request.

Calibration Traceability: All Measuring and Test Equipment (M/TE) identified below are traceable to the SI units through the National Institute for Standards and Technology (NIST). Calibration Laboratory and Quality System controls are compliant with ISO/IEC 17025-2005 and ANSI/NC SL Z540-1-1994.

Standards and Equipment Used:

Make / Model / Name / S/N / Recall Date

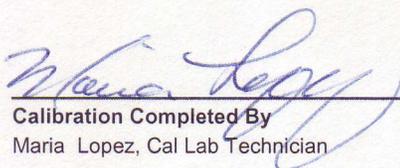
Anritsu	MS4623A	Network Analyzer	992201	18-Mar-12
---------	---------	------------------	--------	-----------

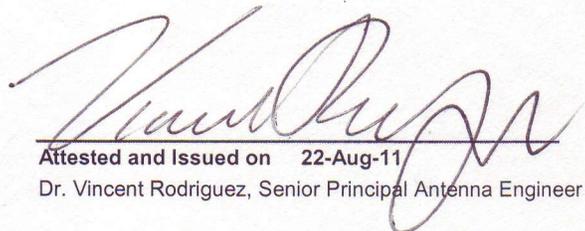
Condition of Instrument Upon Receipt:

In Tolerance to Internal Quality Standards

On Release:


In Tolerance to Internal Quality Standards


 Calibration Completed By
 Maria Lopez, Cal Lab Technician


 Attested and Issued on 22-Aug-11
 Dr. Vincent Rodriguez, Senior Principal Antenna Engineer

Certificate of Calibration

Issue Date: 5/11/2011



General Calibration, Inc.
2 Mars Court, Boonton, New Jersey 07005
Phone (973) 299-2950 Fax (973) 299-0595

Certificate #: MR-18671
Purchase Order: 5247582
Work Order #: MR450
Customer #: 001464

Performed By:

GENERAL CALIBRATION, INC.
2 MARS COURT

BOONTON, NJ 07005

Location of Calibration:

HONEYWELL SECURITY (001464)
2 CORPORATE CENTER DRIVE

MELVILLE, NY 11747

Equipment Information

Job No.: 096188
Manufacturer: HP
Description: TRANSIENT LIMITER
Department:
Temp./RH: 22 C / 45 %
Cal. Interval: 12 MONTHS
Cal Date: 05/11/2011

Asset Tag No.: 10131
Model Number: 11947A
Serial Number: 3107A02782
Inspected By: MR1
Job Title: METROLOGIST
Calibration Result: PASSED
Cal. Due Date: 05/11/2012

Calibration Notes

Condition: Found In Tolerance and Left In Tolerance

Procedures #GCP: HP 11947A

Standards Used To Calibrate Equipment

Company	I.D.	Description	Cal. Due Date
GENERAL CALIBRATION	1031	SYNTHESIZED SWEEPER, 26GHZ	04/06/2012
GENERAL CALIBRATION	503	SPECTRUM ANALYZER	04/12/2012
GENERAL CALIBRATION	688	LEVEL GENERATOR	03/14/2012

The above instrument has been checked and calibrated against the above working standard(s) which are traceable to the NIST. The test limits stated in the report correspond to the published specifications of the equipment, at the points tested. Also, the collective uncertainties of measurement standards do not exceed 25% of the tolerance of the characteristics being calibrated, where possible. The metrology procedures utilized conform to and satisfy the requirements set forth in ANSI/NCSS Z540-1-1994, 10 CFR part 21, ISO 9001-2008, ISO 10012-2003, and MIL-STD 45662A.

Approved By _____

General Calibration, Inc. - Q. A. Manager

Certificate of Calibration

Issue Date: 10/20/2011



General Calibration, Inc.
2 Mars Court, Boonton, New Jersey 07005
Phone (973) 299-2950 Fax (973) 299-0595

Certificate #: MR-19821
Work Order #: MR504
Customer #: 001464

Performed By:

GENERAL CALIBRATION, INC.

Location of Calibration:

HONEYWELL SECURITY (001464)

2 MARS COURT
BOONTON, NJ 07005

2 CORPORATE CENTER DRIVE
MELVILLE, NY 11747

Equipment Information:

Job No.: 076905
Manufacturer: COM-POWER
Description: LISN
Department: DAVID KALMUS
Temp./RH: 22 C / 45 %
Cal. Interval: 12 MONTHS
Cal Date: 10/20/2011

Purchase Order: 5247582
Asset Tag No.: 11262
Model Number: LI-115
Serial Number: 241050
Inspected By: MR1
Job Title: METROLOGIST
Calibration Result: PASSED
Cal. Due Date: 10/20/2012

Calibration Notes:

Condition: Found In Tolerance and Left In Tolerance

Procedures #GCP: COM-POWER LI-115

Standards Used To Calibrate Equipment

Company	I.D.	Description	Cal. Due Date
GENERAL CALIBRATION	418	DIGITAL MULTIMETER	01/03/2012
GENERAL CALIBRATION	700	DIGITAL MULTIMETER	02/10/2012

This is to certify that General Calibration, Inc. is A2LA accredited and that its calibration system is in compliance with ISO/IEC17025-2005, ANSI NCSL Z540-1, ANSI NCSL Z540-3, and ISO 9001:2008. The test limits stated in the report correspond to the published specifications of the equipment, at the points tested. Calibration of standards, reference standards and Intermediate standards in this calibration have been certified traceable to the SI Units of measurement. Any accredited calibration under our A2LA scope of accreditation is denoted with A2LA accredited symbol on the calibration certificate. If the certificate includes any unaccredited items calibrated, they are clearly marked as unaccredited calibration.

Best Uncertainties represent expanded uncertainties expressed at approximately the 95% confidence level using a coverage factor of k=2. The results documented in this certificate relate only to the item(s) calibrated or tested.

Approved By

General Calibration, Inc. - Q. A. Manager