

Appendix A SAR Plots



SAR Test Report

Operator : Y. Chen
Validation Date : 15-Mar-2004
Measurement Date : 15-Mar-2004
Starting Time : 15-Mar-2004 03:59:46 PM
End Time : 15-Mar-2004 04:04:44 PM
Scanning Time : 298 secs

Product Data
Device Name : HP Sapphire
Serial No. : J311500PV033
Type : Other
Model : Sapphire
Frequency : 2412.00 MHz
Max. Transmit Pwr : 0.05 W
Drift Time : 0 min(s)
Length : 200
Width : 180
Depth : 10
Antenna Type : Internal
Power Drift-Start : 0.48
Power Drift-Finish : 0.42
Power Drift : 0.06

Phantom Data
Name : APREL-Uni
Type : Uni-Phantom
Size : 280 x 280 x 200
Serial No. : Stuart
Location : Center
Description : Uni1

Tissue Data
Type : Body
Serial No. : Valiation
Frequency : 2450 MHz
Calibration Date : 15-Mar-2004
Temperature : 24 °C
Ambient Temp. : 24 °C
Humidity : 50 RH%
Epsilon : 50 F/m
Sigma : 1.79 S/m
Density : 1000 kg/cu. m

Probe Data
Name : Probe-212
Model : E020
Type : E-Field Triangle
Serial No. : 212
Calibration Date : 05-Mar-2004
Frequency : 2450 MHz
Duty Cycle Factor : 1
Conversion Factor : 1.7
Probe Sensitivity : 0.78 0.78 0.75 $\mu\text{V}/(\text{V}/\text{sq. m})$
Compression Point : 93
Offset : 1.56




Measurement Data

Crest Factor : 1
Scan Type : Complete
Set-up Date : 15-Mar-2004
Set-up Time : 3:59:32 PM

Other Data

DUT Position : Touch
Separation : 0
Channel : Low - 2412

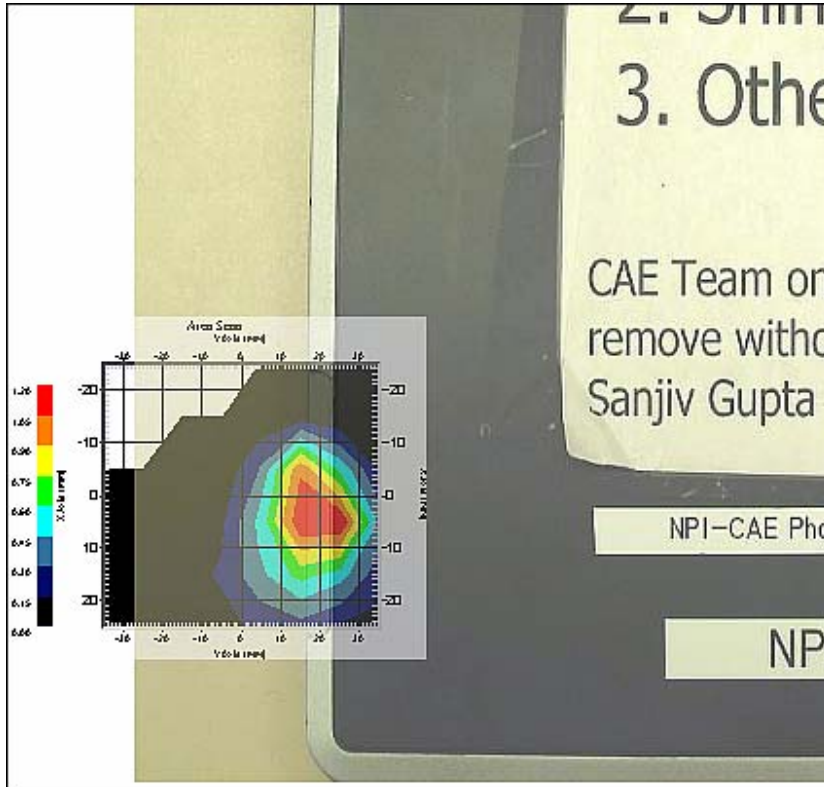


1 gram SAR value : 0.90.05 W/kg
Area Scan Peak SAR : 1.19
Zoom Scan Peak SAR : 2.53

Exposure Assessment Measurement Uncertainty

Source of Uncertainty	Tolerance Value	Probability Distribution	Divisor	c_i^1 (1-g)	c_i^1 (10-g)	Standard Uncertainty (1-g)	Standard Uncertainty (10-g)
Measurement System							
Probe Calibration	3.5	normal	1	1	1	3.5	3.5
Axial Isotropy	3.7	rectangular	$\sqrt{3}$	$(1-cp)_2^{1/}$	$(1-cp)_2^{1/}$	1.5	1.5
Hemispherical Isotropy	10.9	rectangular	$\sqrt{3}$	$\sqrt{cp}$	$\sqrt{cp}$	4.4	4.4
Boundary Effect	1.0	rectangular	$\sqrt{3}$	1	1	0.6	0.6
Linearity	4.7	rectangular	$\sqrt{3}$	1	1	2.7	2.7
Detection Limit	1.0	rectangular	$\sqrt{3}$	1	1	0.6	0.6
Readout Electronics	1.0	normal	1	1	1	1.0	1.0
Response Time	0.8	rectangular	$\sqrt{3}$	1	1	0.5	0.5
Integration Time	1.7	rectangular	$\sqrt{3}$	1	1	1.0	1.0
RF Ambient Condition	3.0	rectangular	$\sqrt{3}$	1	1	1.7	1.7
Probe Positioner Mech.	0.4	rectangular	$\sqrt{3}$	1	1	0.2	0.2
Restriction							
Probe Positioning with respect to Phantom Shell	2.9	rectangular	$\sqrt{3}$	1	1	2.1	2.1
Extrapolation and Integration	3.7	rectangular	$\sqrt{3}$	1	1	2.1	2.1
Test Sample Positioning	4.0	normal	1	1	1	4.0	4.0
Device Holder Uncertainty	2.0	normal	1	1	1	2.0	2.0
Drift of Output Power	0.1	rectangular	$\sqrt{3}$	1	1	0.0	0.0
Phantom and Setup							
Phantom Uncertainty(shape & thickness tolerance)	3.4	rectangular	$\sqrt{3}$	1	1	2.0	2.0
Liquid Conductivity(target)	13.0	rectangular	$\sqrt{3}$	0.7	0.5	5.3	3.8
Liquid Conductivity(meas.)	0.2	rectangular	$\sqrt{3}$	0.7	0.5	0.1	0.1
Liquid Permittivity(target)	2.0	rectangular	$\sqrt{3}$	0.6	0.5	0.8	0.6
Liquid Permittivity(meas.)	5.0	rectangular	$\sqrt{3}$	0.6	0.5	1.7	1.4
Combined Uncertainty		RSS				10.3	9.5
Combined Uncertainty (coverage factor=2)		Normal(k=2)				20.6	19.1



Z-Axis Scan

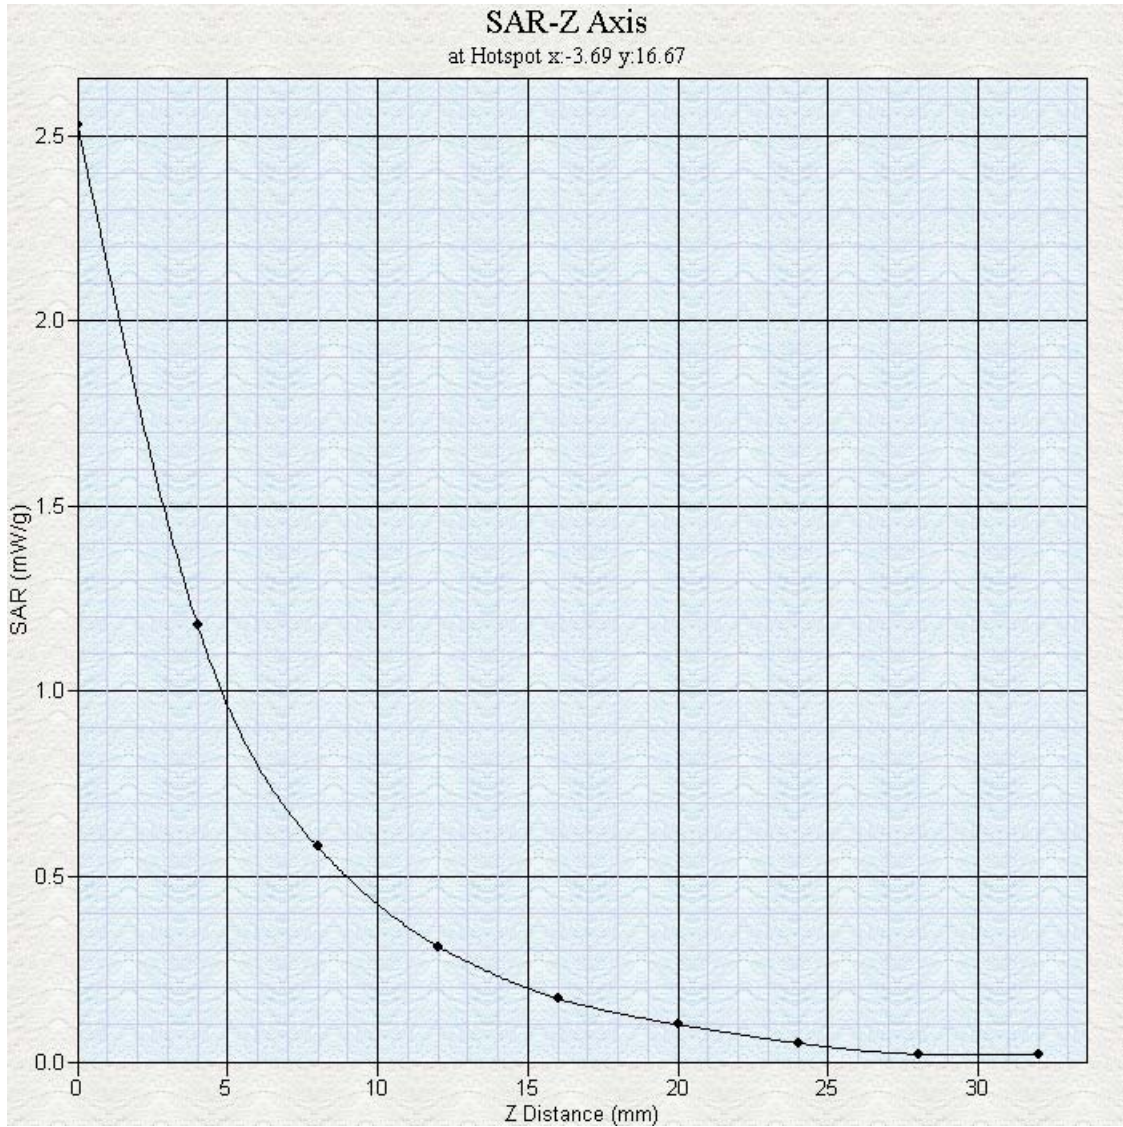

Project number: ITLB-Dell-5008
FCC ID: ID:CNTPP3006

51 Spectrum Way
Nepean, Ontario
Canada K2R 1E6
© 2004 APREL Laboratories

AL-065



This report shall not be reproduced, except in full, without written approval of APREL Laboratories

Page 27 of 64

Tel: (613) 820-2730
Fax: (613) 820-4161
Info@aprel.com
www.aprel.com

SAR Test Report

Operator : Y. Chen
 Validation Date : 15-Mar-2004
 Measurement Date : 15-Mar-2004
 Starting Time : 15-Mar-2004 04:14:09 PM
 End Time : 15-Mar-2004 04:19:09 PM
 Scanning Time : 300 secs

Product Data
 Device Name : HP Sapphire
 Serial No. : J311500PV033
 Type : Other
 Model : Sapphire
 Frequency : 2437.00 MHz
 Max. Transmit Pwr : 0.05 W
 Drift Time : 0 min(s)
 Length : 200
 Width : 180
 Depth : 10
 Antenna Type : Internal
 Power Drift-Start : 3.20
 Power Drift-Finish : 3.29
 Power Drift : 0.09

Phantom Data
 Name : APREL-Uni
 Type : Uni-Phantom
 Size : 280 x 280 x 200
 Serial No. : Stuart
 Location : Center
 Description : Uni1

Tissue Data
 Type : Body
 Serial No. : Valiation
 Frequency : 2450 MHz
 Calibration Date : 15-Mar-2004
 Temperature : 24 °C
 Ambient Temp. : 24 °C
 Humidity : 50 RH%
 Epsilon : 50 F/m
 Sigma : 1.79 S/m
 Density : 1000 kg/cu. m


Probe Data
 Name : Probe-212
 Model : E020
 Type : E-Field Triangle
 Serial No. : 212
 Calibration Date : 05-Mar-2004
 Frequency : 2450 MHz
 Duty Cycle Factor : 1
 Conversion Factor : 1.7
 Probe Sensitivity : 0.78 0.78 0.75 $\mu\text{V}/(\text{V}/\text{sq. m})$
 Compression Point : 93
 Offset : 1.56

Measurement Data

Crest Factor : 1
Scan Type : Complete
Set-up Date : 15-Mar-2004
Set-up Time : 3:51:42 PM

Other Data

DUT Position : LCD Top
Separation : 0
Channel : Mid - 2437

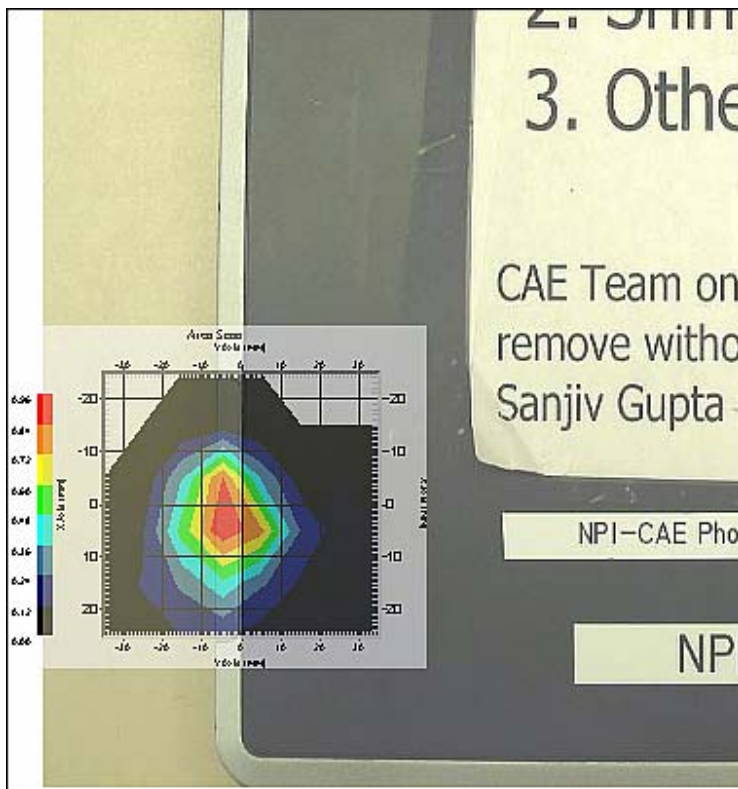


1 gram SAR value : 0.86 W/kg
Area Scan Peak SAR : 0.94
Zoom Scan Peak SAR : 2.21

Exposure Assessment Measurement Uncertainty

Source of Uncertainty	Tolerance Value	Probability Distribution	Divisor	c_i^1 (1-g)	c_i^1 (10-g)	Standard Uncertainty (1-g)	Standard Uncertainty (10-g)
Measurement System							
Probe Calibration	3.5	normal	1	1	1	3.5	3.5
Axial Isotropy	3.7	rectangular	$\sqrt{3}$	$(1-cp)_2^{1/}$	$(1-cp)_2^{1/}$	1.5	1.5
Hemispherical Isotropy	10.9	rectangular	$\sqrt{3}$	$\sqrt{cp}$	$\sqrt{cp}$	4.4	4.4
Boundary Effect	1.0	rectangular	$\sqrt{3}$	1	1	0.6	0.6
Linearity	4.7	rectangular	$\sqrt{3}$	1	1	2.7	2.7
Detection Limit	1.0	rectangular	$\sqrt{3}$	1	1	0.6	0.6
Readout Electronics	1.0	normal	1	1	1	1.0	1.0
Response Time	0.8	rectangular	$\sqrt{3}$	1	1	0.5	0.5
Integration Time	1.7	rectangular	$\sqrt{3}$	1	1	1.0	1.0
RF Ambient Condition	3.0	rectangular	$\sqrt{3}$	1	1	1.7	1.7
Probe Positioner Mech.	0.4	rectangular	$\sqrt{3}$	1	1	0.2	0.2
Restriction							
Probe Positioning with respect to Phantom Shell	2.9	rectangular	$\sqrt{3}$	1	1	2.1	2.1
Extrapolation and Integration	3.7	rectangular	$\sqrt{3}$	1	1	2.1	2.1
Test Sample Positioning	4.0	normal	1	1	1	4.0	4.0
Device Holder Uncertainty	2.0	normal	1	1	1	2.0	2.0
Drift of Output Power	0.1	rectangular	$\sqrt{3}$	1	1	0.1	0.1
Phantom and Setup							
Phantom Uncertainty(shape & thickness tolerance)	3.4	rectangular	$\sqrt{3}$	1	1	2.0	2.0
Liquid Conductivity(target)	13.0	rectangular	$\sqrt{3}$	0.7	0.5	5.3	3.8
Liquid Conductivity(meas.)	0.2	rectangular	$\sqrt{3}$	0.7	0.5	0.1	0.1
Liquid Permittivity(target)	2.0	rectangular	$\sqrt{3}$	0.6	0.5	0.8	0.6
Liquid Permittivity(meas.)	5.0	rectangular	$\sqrt{3}$	0.6	0.5	1.7	1.4
Combined Uncertainty		RSS				10.3	9.5
Combined Uncertainty (coverage factor=2)		Normal(k=2)				20.6	19.1



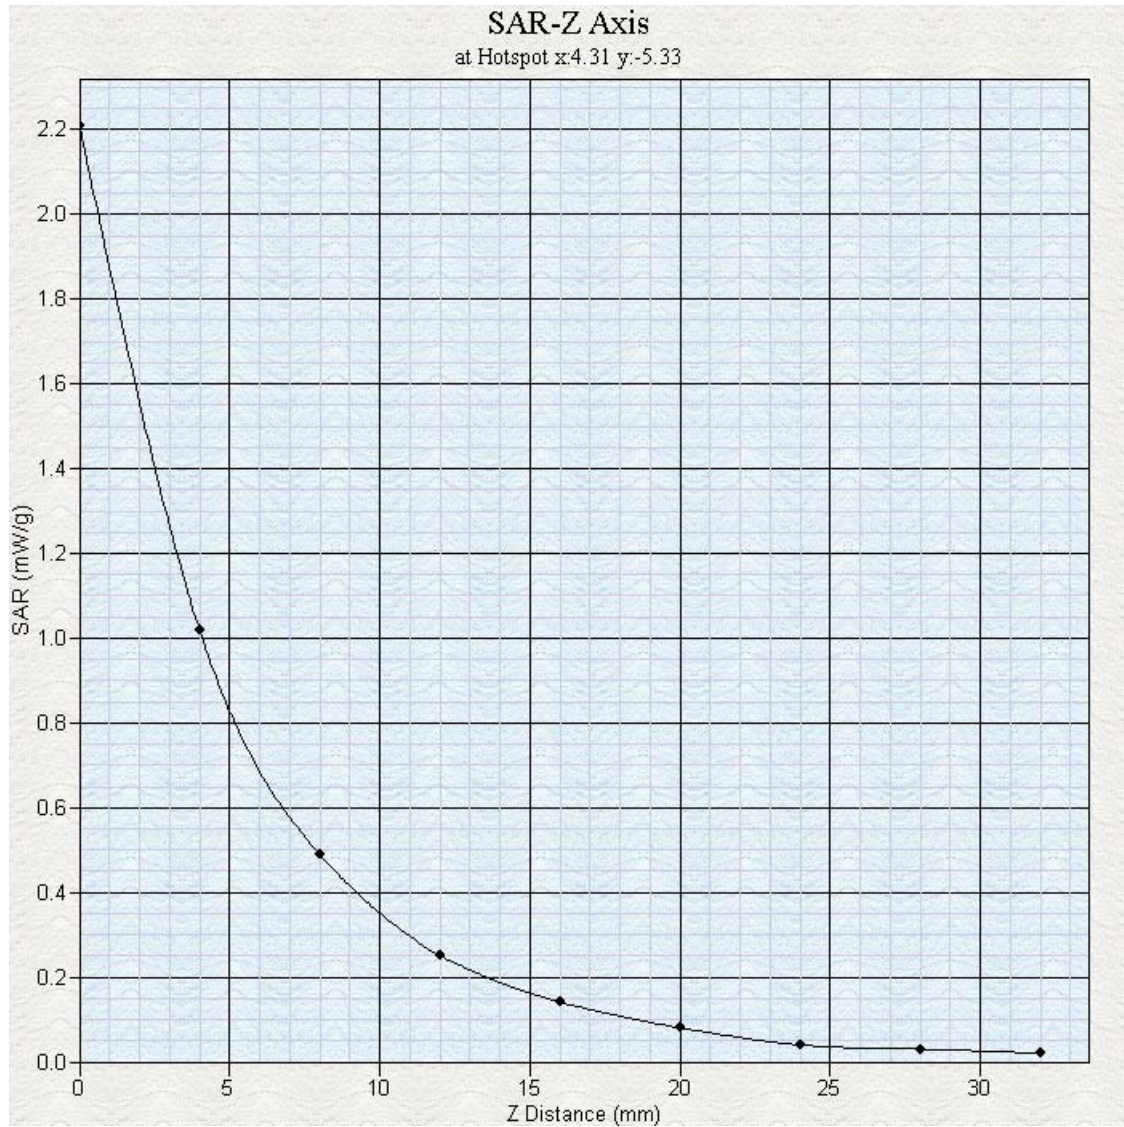

Project number: ITLB-Dell-5008
FCC ID: ID:CNTPP3006

Page 31 of 64

51 Spectrum Way
Nepean, Ontario
Canada K2R 1E6
© 2004 APREL Laboratories



Tel: (613) 820-2730
Fax: (613) 820-4161
Info@aprel.com
www.aprel.com

AL-065

This report shall not be reproduced, except in full, without written approval of APREL Laboratories

SAR Test Report

Operator : Y. Chen
Validation Date : 15-Mar-2004
Measurement Date : 15-Mar-2004
Starting Time : 15-Mar-2004 04:22:29 PM
End Time : 15-Mar-2004 04:27:30 PM
Scanning Time : 301 secs

Product Data

Device Name : HP Sapphire
Serial No. : J311500PV033
Type : Other
Model : Sapphire
Frequency : 2462.00 MHz
Max. Transmit Pwr : 0.05 W
Drift Time : 0 min(s)
Length : 200
Width : 180
Depth : 10
Antenna Type : Internal
Power Drift-Start : 2.93
Power Drift-Finish : 2.74
Power Drift : 0.19

Phantom Data

Name : APREL-Uni
Type : Uni-Phantom
Size : 280 x 280 x 200
Serial No. : Stuart
Location : Center
Description : Uni1

Tissue Data

Type : Body
Serial No. : Valiation
Frequency : 2450 MHz
Calibration Date : 15-Mar-2004
Temperature : 24 °C
Ambient Temp. : 24 °C
Humidity : 50 RH%
Epsilon : 50 F/m
Sigma : 1.79 S/m
Density : 1000 kg/cu. m

Probe Data


Name : Probe-212
Model : E020
Type : E-Field Triangle
Serial No. : 212
Calibration Date : 05-Mar-2004
Frequency : 2450 MHz
Duty Cycle Factor : 1
Conversion Factor : 1.7
Probe Sensitivity : 0.78 0.78 0.75 $\mu\text{V}/(\text{V}/\text{sq. m})$
Compression Point : 93
Offset : 1.56

Measurement Data

Crest Factor : 1
Scan Type : Complete
Set-up Date : 15-Mar-2004
Set-up Time : 3:51:42 PM

Other Data

DUT Position : LCD Top
Separation : 0
Channel : High - 2462

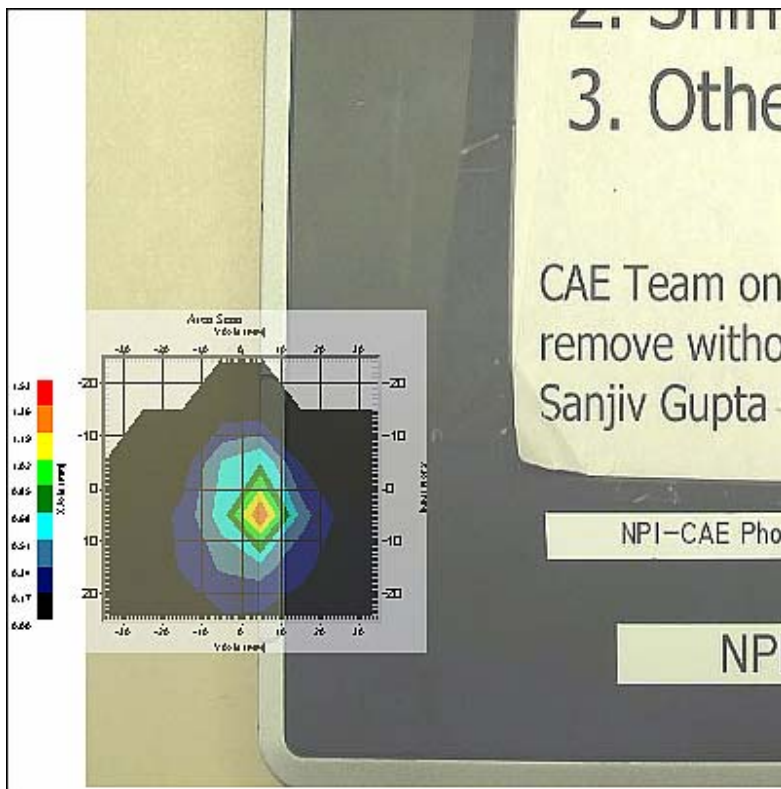


1 gram SAR value : 0.79 W/kg
Area Scan Peak SAR : 1.36
Zoom Scan Peak SAR : 2.24

Exposure Assessment Measurement Uncertainty

Source of Uncertainty	Tolerance Value	Probability Distribution	Divisor	c_i^1 (1-g)	c_i^1 (10-g)	Standard Uncertainty (1-g)	Standard Uncertainty (10-g)
Measurement System							
Probe Calibration	3.5	normal	1	1	1	3.5	3.5
Axial Isotropy	3.7	rectangular	$\sqrt{3}$	$(1-cp)^{1/2}$	$(1-cp)^{1/2}$	1.5	1.5
Hemispherical Isotropy	10.9	rectangular	$\sqrt{3}$	$\sqrt{cp}$	$\sqrt{cp}$	4.4	4.4
Boundary Effect	1.0	rectangular	$\sqrt{3}$	1	1	0.6	0.6
Linearity	4.7	rectangular	$\sqrt{3}$	1	1	2.7	2.7
Detection Limit	1.0	rectangular	$\sqrt{3}$	1	1	0.6	0.6
Readout Electronics	1.0	normal	1	1	1	1.0	1.0
Response Time	0.8	rectangular	$\sqrt{3}$	1	1	0.5	0.5
Integration Time	1.7	rectangular	$\sqrt{3}$	1	1	1.0	1.0
RF Ambient Condition	3.0	rectangular	$\sqrt{3}$	1	1	1.7	1.7
Probe Positioner Mech.	0.4	rectangular	$\sqrt{3}$	1	1	0.2	0.2
Restriction							
Probe Positioning with respect to Phantom Shell	2.9	rectangular	$\sqrt{3}$	1	1	2.1	2.1
Extrapolation and Integration	3.7	rectangular	$\sqrt{3}$	1	1	2.1	2.1
Test Sample Positioning	4.0	normal	1	1	1	4.0	4.0
Device Holder Uncertainty	2.0	normal	1	1	1	2.0	2.0
Drift of Output Power	0.2	rectangular	$\sqrt{3}$	1	1	0.1	0.1
Phantom and Setup							
Phantom Uncertainty(shape & thickness tolerance)	3.4	rectangular	$\sqrt{3}$	1	1	2.0	2.0
Liquid Conductivity(target)	13.0	rectangular	$\sqrt{3}$	0.7	0.5	5.3	3.8
Liquid Conductivity(meas.)	0.2	rectangular	$\sqrt{3}$	0.7	0.5	0.1	0.1
Liquid Permittivity(target)	2.0	rectangular	$\sqrt{3}$	0.6	0.5	0.8	0.6
Liquid Permittivity(meas.)	5.0	rectangular	$\sqrt{3}$	0.6	0.5	1.7	1.4
Combined Uncertainty		RSS				10.3	9.5
Combined Uncertainty (coverage factor=2)		Normal(k=2)				20.6	19.1



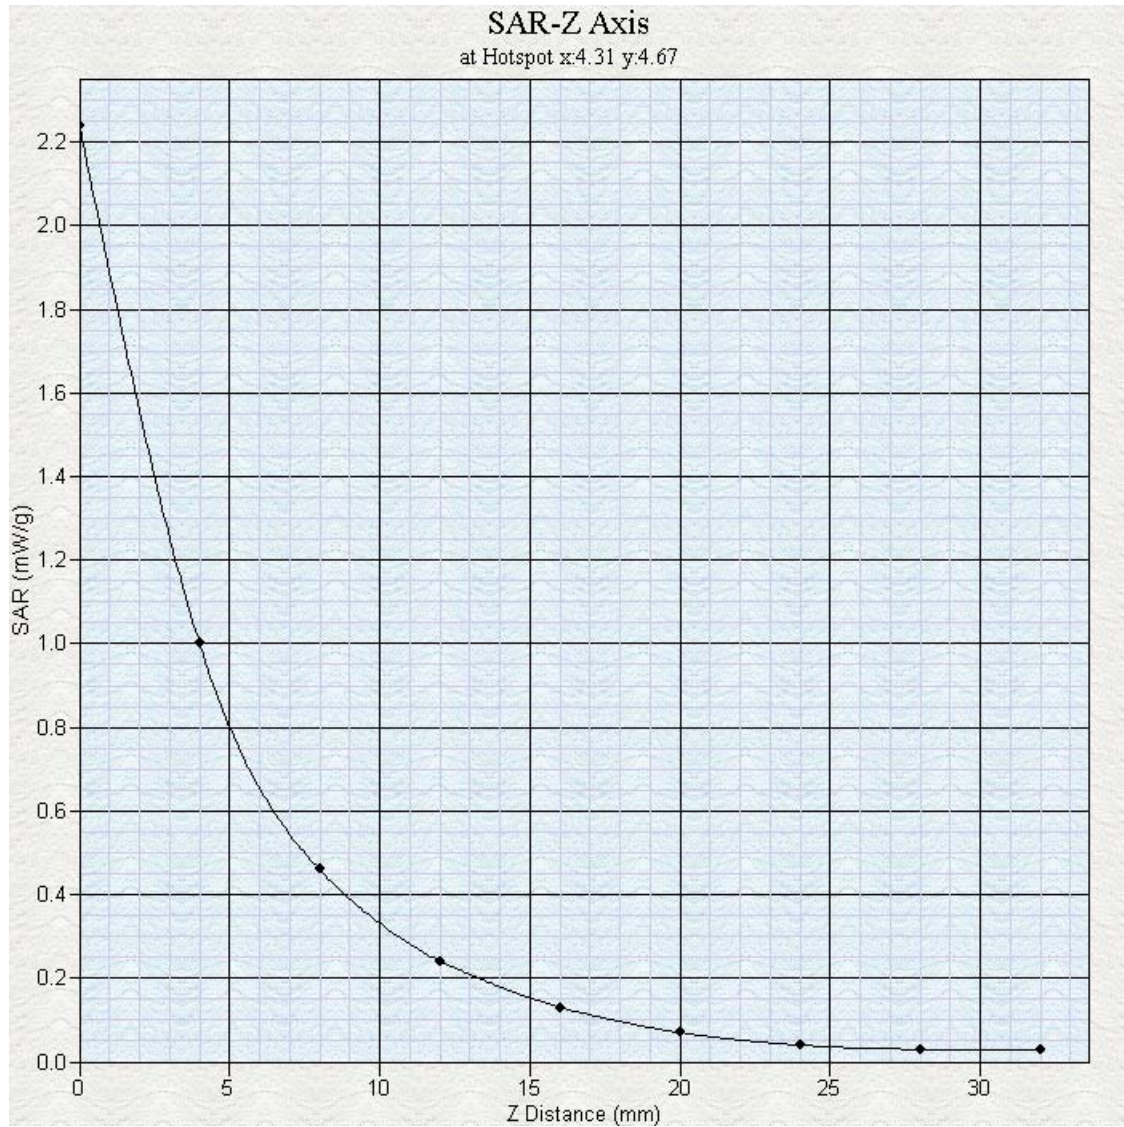

SAR Test Report

Operator : Y. Chen
 Validation Date : 15-Mar-2004
 Measurement Date : 15-Mar-2004
 Starting Time : 15-Mar-2004 04:47:42 PM
 End Time : 15-Mar-2004 04:52:39 PM
 Scanning Time : 297 secs

Product Data
 Device Name : HP Sapphire
 Serial No. : J311500PV033
 Type : Other
 Model : Sapphire
 Frequency : 2462.00 MHz
 Max. Transmit Pwr : 0.05 W
 Drift Time : 0 min(s)
 Length : 200
 Width : 180
 Depth : 10
 Antenna Type : Internal
 Power Drift-Start : 0.33
 Power Drift-Finish : 0.39
 Power Drift : 0.06

Phantom Data
 Name : APREL-Uni
 Type : Uni-Phantom
 Size : 280 x 280 x 200
 Serial No. : Stuart
 Location : Center
 Description : Uni1

Tissue Data
 Type : Body
 Serial No. : Valiation
 Frequency : 2450 MHz
 Calibration Date : 15-Mar-2004
 Temperature : 24 °C
 Ambient Temp. : 24 °C
 Humidity : 50 RH%
 Epsilon : 50 F/m
 Sigma : 1.79 S/m
 Density : 1000 kg/cu. m


Probe Data
 Name : Probe-212
 Model : E020
 Type : E-Field Triangle
 Serial No. : 212
 Calibration Date : 05-Mar-2004
 Frequency : 2450 MHz
 Duty Cycle Factor: 1
 Conversion Factor: 1.7
 Probe Sensitivity: 0.78 0.78 0.75 $\mu\text{V}/(\text{V}/\text{sq. m})$
 Compression Point: 93
 Offset : 1.56

Measurement Data

Crest Factor : 1
Scan Type : Complete
Set-up Date : 15-Mar-2004
Set-up Time : 3:51:42 PM

Other Data

DUT Position : LCD Top
Separation : 0
Channel : High - 2462

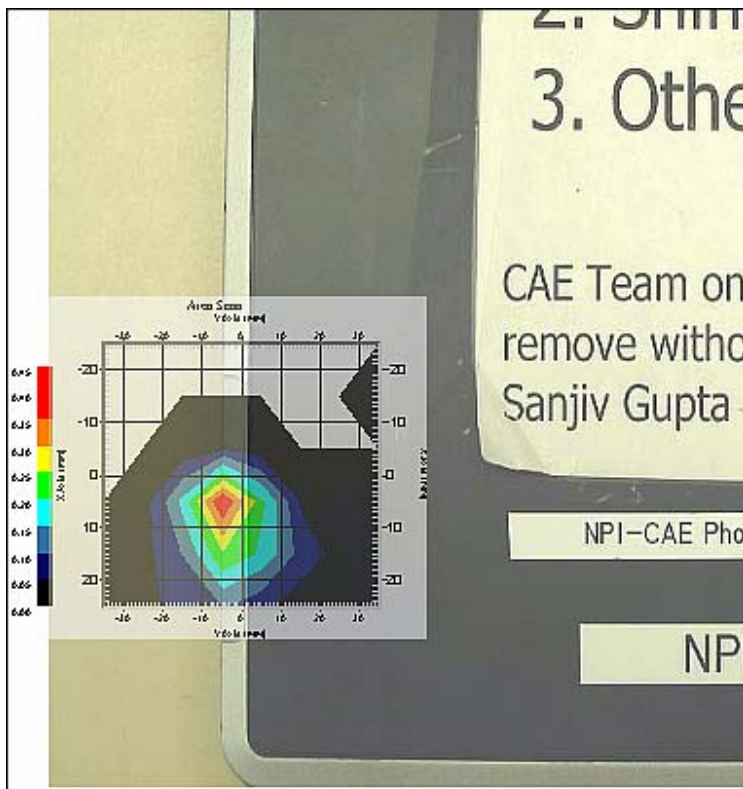


1 gram SAR value : 0.26 W/kg
Area Scan Peak SAR : 0.40
Zoom Scan Peak SAR : 0.75

Exposure Assessment Measurement Uncertainty

Source of Uncertainty	Tolerance Value	Probability Distribution	Divisor	c_i^1 (1-g)	c_i^1 (10-g)	Standard Uncertainty (1-g)	Standard Uncertainty (10-g)
Measurement System							
Probe Calibration	3.5	normal	1	1	1	3.5	3.5
Axial Isotropy	3.7	rectangular	$\sqrt{3}$	$(1-cp)_2^{1/}$	$(1-cp)_2^{1/}$	1.5	1.5
Hemispherical Isotropy	10.9	rectangular	$\sqrt{3}$	$\sqrt{cp}$	$\sqrt{cp}$	4.4	4.4
Boundary Effect	1.0	rectangular	$\sqrt{3}$	1	1	0.6	0.6
Linearity	4.7	rectangular	$\sqrt{3}$	1	1	2.7	2.7
Detection Limit	1.0	rectangular	$\sqrt{3}$	1	1	0.6	0.6
Readout Electronics	1.0	normal	1	1	1	1.0	1.0
Response Time	0.8	rectangular	$\sqrt{3}$	1	1	0.5	0.5
Integration Time	1.7	rectangular	$\sqrt{3}$	1	1	1.0	1.0
RF Ambient Condition	3.0	rectangular	$\sqrt{3}$	1	1	1.7	1.7
Probe Positioner Mech.	0.4	rectangular	$\sqrt{3}$	1	1	0.2	0.2
Restriction							
Probe Positioning with respect to Phantom Shell	2.9	rectangular	$\sqrt{3}$	1	1	2.1	2.1
Extrapolation and Integration	3.7	rectangular	$\sqrt{3}$	1	1	2.1	2.1
Test Sample Positioning	4.0	normal	1	1	1	4.0	4.0
Device Holder Uncertainty	2.0	normal	1	1	1	2.0	2.0
Drift of Output Power	0.1	rectangular	$\sqrt{3}$	1	1	0.0	0.0
Phantom and Setup							
Phantom Uncertainty(shape & thickness tolerance)	3.4	rectangular	$\sqrt{3}$	1	1	2.0	2.0
Liquid Conductivity(target)	13.0	rectangular	$\sqrt{3}$	0.7	0.5	5.3	3.8
Liquid Conductivity(meas.)	0.2	rectangular	$\sqrt{3}$	0.7	0.5	0.1	0.1
Liquid Permittivity(target)	2.0	rectangular	$\sqrt{3}$	0.6	0.5	0.8	0.6
Liquid Permittivity(meas.)	5.0	rectangular	$\sqrt{3}$	0.6	0.5	1.7	1.4
Combined Uncertainty		RSS				10.3	9.5
Combined Uncertainty (coverage factor=2)		Normal(k=2)				20.6	19.1



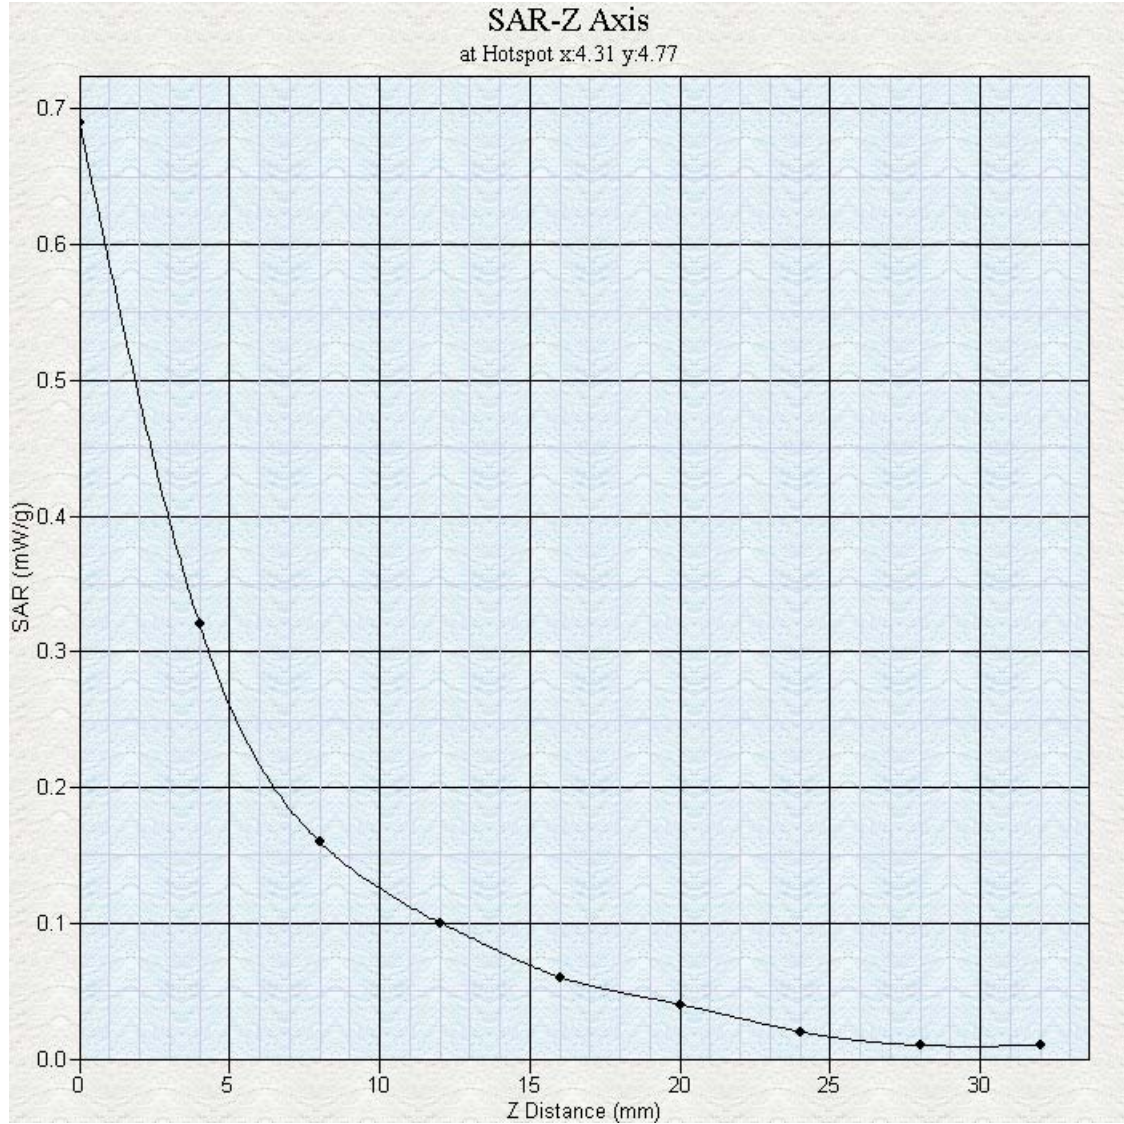

SAR Test Report

Operator : Y. Chen
 Validation Date : 16-Mar-2004
 Measurement Date : 16-Mar-2004
 Starting Time : 16-Mar-2004 04:20:12 PM
 End Time : 16-Mar-2004 04:25:10 PM
 Scanning Time : 298 secs

Product Data

Device Name : HP Sapphire
 Serial No. : J311500PV033
 Type : Other
 Model : Sapphire
 Frequency : 2412.00 MHz
 Max. Transmit Pwr : 0.05 W
 Drift Time : 0 min(s)
 Length : 200
 Width : 180
 Depth : 10
 Antenna Type : Internal
 Power Drift-Start : 0.89
 Power Drift-Finish : 0.80
 Power Drift : 0.09

Phantom Data

Name : APREL-Uni
 Type : Uni-Phantom
 Size : 280 x 280 x 200
 Serial No. : Stuart
 Location : Center
 Description : Uni1

Tissue Data

Type : Body
 Serial No. : Valiation
 Frequency : 2450 MHz
 Calibration Date : 15-Mar-2004
 Temperature : 24 °C
 Ambient Temp. : 24 °C
 Humidity : 50 RH%
 Epsilon : 50 F/m
 Sigma : 1.79 S/m
 Density : 1000 kg/cu. m

Probe Data


Name : Probe-212
 Model : E020
 Type : E-Field Triangle
 Serial No. : 212
 Calibration Date : 05-Mar-2004
 Frequency : 2450 MHz
 Duty Cycle Factor : 1
 Conversion Factor : 1.7
 Probe Sensitivity : 0.78 0.78 0.75 $\mu\text{V}/(\text{V}/\text{sq. m})$
 Compression Point : 93
 Offset : 1.56

Measurement Data

Crest Factor : 1
Scan Type : Complete
Set-up Date : 16-Mar-2004
Set-up Time : 9:42:00 AM

Other Data


DUT Position : Touch
Separation : 0
Channel : Low - 2412

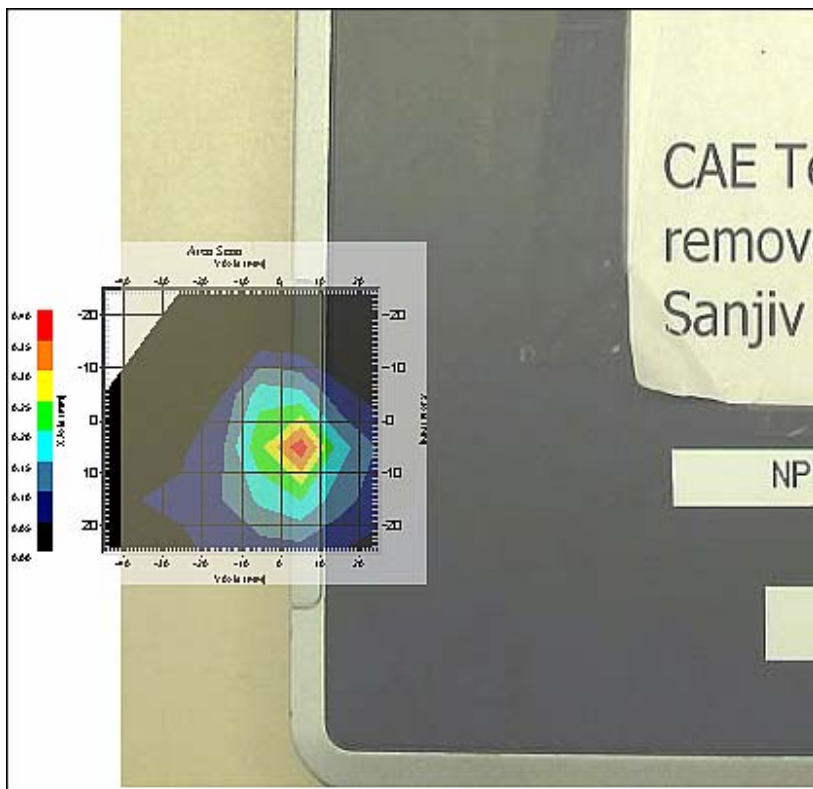

1 gram SAR value : 0.27 W/kg
Area Scan Peak SAR : 0.38
Zoom Scan Peak SAR : 0.69

Exposure Assessment Measurement Uncertainty

Source of Uncertainty	Tolerance Value	Probability Distribution	Divisor	c_i^1 (1-g)	c_i^1 (10-g)	Standard Uncertainty (1-g)	Standard Uncertainty (10-g)
Measurement System							
Probe Calibration	3.5	normal	1	1	1	3.5	3.5
Axial Isotropy	3.7	rectangular	$\sqrt{3}$	$(1-cp)_2^{1/}$	$(1-cp)_2^{1/}$	1.5	1.5
Hemispherical Isotropy	10.9	rectangular	$\sqrt{3}$	$\sqrt{cp}$	$\sqrt{cp}$	4.4	4.4
Boundary Effect	1.0	rectangular	$\sqrt{3}$	1	1	0.6	0.6
Linearity	4.7	rectangular	$\sqrt{3}$	1	1	2.7	2.7
Detection Limit	1.0	rectangular	$\sqrt{3}$	1	1	0.6	0.6
Readout Electronics	1.0	normal	1	1	1	1.0	1.0
Response Time	0.8	rectangular	$\sqrt{3}$	1	1	0.5	0.5
Integration Time	1.7	rectangular	$\sqrt{3}$	1	1	1.0	1.0
RF Ambient Condition	3.0	rectangular	$\sqrt{3}$	1	1	1.7	1.7
Probe Positioner Mech.	0.4	rectangular	$\sqrt{3}$	1	1	0.2	0.2
Restriction							
Probe Positioning with respect to Phantom Shell	2.9	rectangular	$\sqrt{3}$	1	1	2.1	2.1
Extrapolation and Integration	3.7	rectangular	$\sqrt{3}$	1	1	2.1	2.1
Test Sample Positioning	4.0	normal	1	1	1	4.0	4.0
Device Holder Uncertainty	2.0	normal	1	1	1	2.0	2.0
Drift of Output Power	0.1	rectangular	$\sqrt{3}$	1	1	0.1	0.1
Phantom and Setup							
Phantom Uncertainty(shape & thickness tolerance)	3.4	rectangular	$\sqrt{3}$	1	1	2.0	2.0
Liquid Conductivity(target)	13.0	rectangular	$\sqrt{3}$	0.7	0.5	5.3	3.8
Liquid Conductivity(meas.)	0.2	rectangular	$\sqrt{3}$	0.7	0.5	0.1	0.1
Liquid Permittivity(target)	2.0	rectangular	$\sqrt{3}$	0.6	0.5	0.8	0.6
Liquid Permittivity(meas.)	5.0	rectangular	$\sqrt{3}$	0.6	0.5	1.7	1.4
Combined Uncertainty		RSS				10.3	9.5
Combined Uncertainty (coverage factor=2)		Normal(k=2)				20.6	19.1

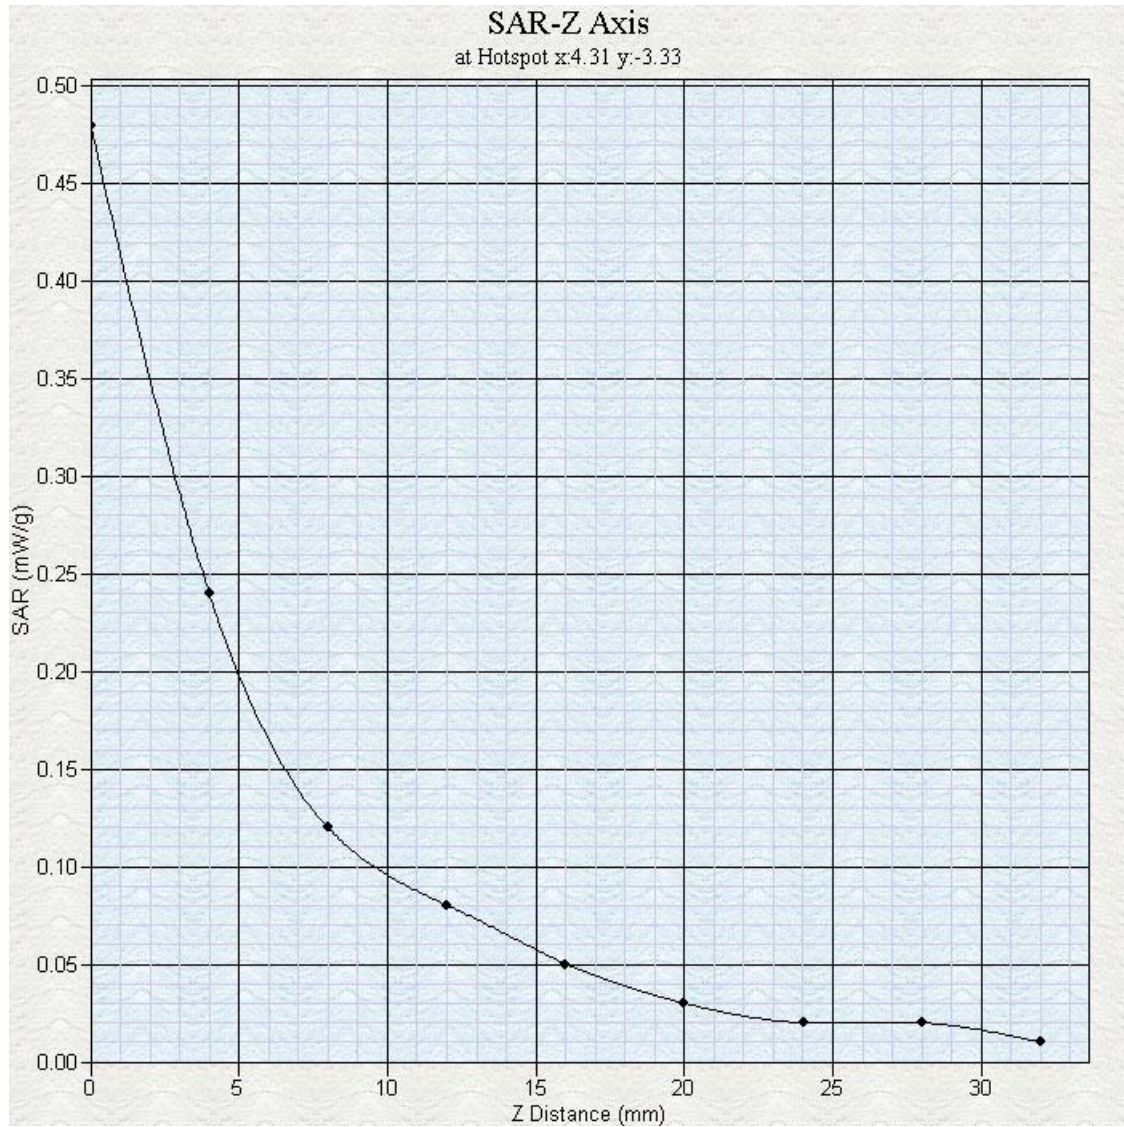

SAR Test Report

Operator : Y. Chen
 Validation Date : 16-Mar-2004
 Measurement Date : 16-Mar-2004
 Starting Time : 16-Mar-2004 04:37:34 PM
 End Time : 16-Mar-2004 04:42:32 PM
 Scanning Time : 298 secs

Product Data
 Device Name : HP Sapphire
 Serial No. : J311500PV033
 Type : Other
 Model : Sapphire
 Frequency : 2437.00 MHz
 Max. Transmit Pwr : 0.05 W
 Drift Time : 0 min(s)
 Length : 200
 Width : 180
 Depth : 10
 Antenna Type : Internal
 Power Drift-Start : 0.73
 Power Drift-Finish : 0.70
 Power Drift : 0.03

Phantom Data
 Name : APREL-Uni
 Type : Uni-Phantom
 Size : 280 x 280 x 200
 Serial No. : Stuart
 Location : Center
 Description : Uni1

Tissue Data
 Type : Body
 Serial No. : Valiation
 Frequency : 2450 MHz
 Calibration Date : 15-Mar-2004
 Temperature : 24 °C
 Ambient Temp. : 24 °C
 Humidity : 50 RH%
 Epsilon : 50 F/m
 Sigma : 1.79 S/m
 Density : 1000 kg/cu. m


Probe Data
 Name : Probe-212
 Model : E020
 Type : E-Field Triangle
 Serial No. : 212
 Calibration Date : 05-Mar-2004
 Frequency : 2450 MHz
 Duty Cycle Factor: 1
 Conversion Factor: 1.7
 Probe Sensitivity: 0.78 0.78 0.75 $\mu\text{V}/(\text{V}/\text{sq. m})$
 Compression Point: 93
 Offset : 1.56

Measurement Data

Crest Factor : 1
Scan Type : Complete
Set-up Date : 16-Mar-2004
Set-up Time : 9:42:00 AM

Other Data

DUT Position : Touch
Separation : 0
Channel : Mid - 2437

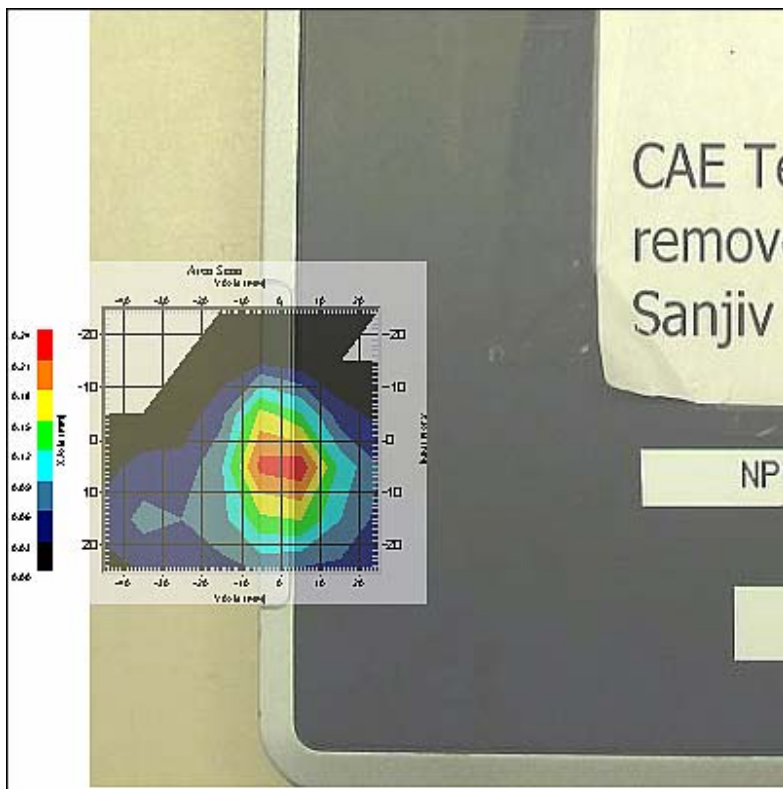


1 gram SAR value : 0.20 W/kg
Area Scan Peak SAR : 0.23
Zoom Scan Peak SAR : 0.48

Exposure Assessment Measurement Uncertainty

Source of Uncertainty	Tolerance Value	Probability Distribution	Divisor	c_i^1 (1-g)	c_i^1 (10-g)	Standard Uncertainty (1-g)	Standard Uncertainty (10-g)
Measurement System							
Probe Calibration	3.5	normal	1	1	1	3.5	3.5
Axial Isotropy	3.7	rectangular	$\sqrt{3}$	$(1-cp)_2^{1/}$	$(1-cp)_2^{1/}$	1.5	1.5
Hemispherical Isotropy	10.9	rectangular	$\sqrt{3}$	$\sqrt{cp}$	$\sqrt{cp}$	4.4	4.4
Boundary Effect	1.0	rectangular	$\sqrt{3}$	1	1	0.6	0.6
Linearity	4.7	rectangular	$\sqrt{3}$	1	1	2.7	2.7
Detection Limit	1.0	rectangular	$\sqrt{3}$	1	1	0.6	0.6
Readout Electronics	1.0	normal	1	1	1	1.0	1.0
Response Time	0.8	rectangular	$\sqrt{3}$	1	1	0.5	0.5
Integration Time	1.7	rectangular	$\sqrt{3}$	1	1	1.0	1.0
RF Ambient Condition	3.0	rectangular	$\sqrt{3}$	1	1	1.7	1.7
Probe Positioner Mech.	0.4	rectangular	$\sqrt{3}$	1	1	0.2	0.2
Restriction							
Probe Positioning with respect to Phantom Shell	2.9	rectangular	$\sqrt{3}$	1	1	2.1	2.1
Extrapolation and Integration	3.7	rectangular	$\sqrt{3}$	1	1	2.1	2.1
Test Sample Positioning	4.0	normal	1	1	1	4.0	4.0
Device Holder Uncertainty	2.0	normal	1	1	1	2.0	2.0
Drift of Output Power	0.0	rectangular	$\sqrt{3}$	1	1	0.0	0.0
Phantom and Setup							
Phantom Uncertainty(shape & thickness tolerance)	3.4	rectangular	$\sqrt{3}$	1	1	2.0	2.0
Liquid Conductivity(target)	13.0	rectangular	$\sqrt{3}$	0.7	0.5	5.3	3.8
Liquid Conductivity(meas.)	0.2	rectangular	$\sqrt{3}$	0.7	0.5	0.1	0.1
Liquid Permittivity(target)	2.0	rectangular	$\sqrt{3}$	0.6	0.5	0.8	0.6
Liquid Permittivity(meas.)	5.0	rectangular	$\sqrt{3}$	0.6	0.5	1.7	1.4
Combined Uncertainty		RSS				10.3	9.5
Combined Uncertainty (coverage factor=2)		Normal(k=2)				20.6	19.1



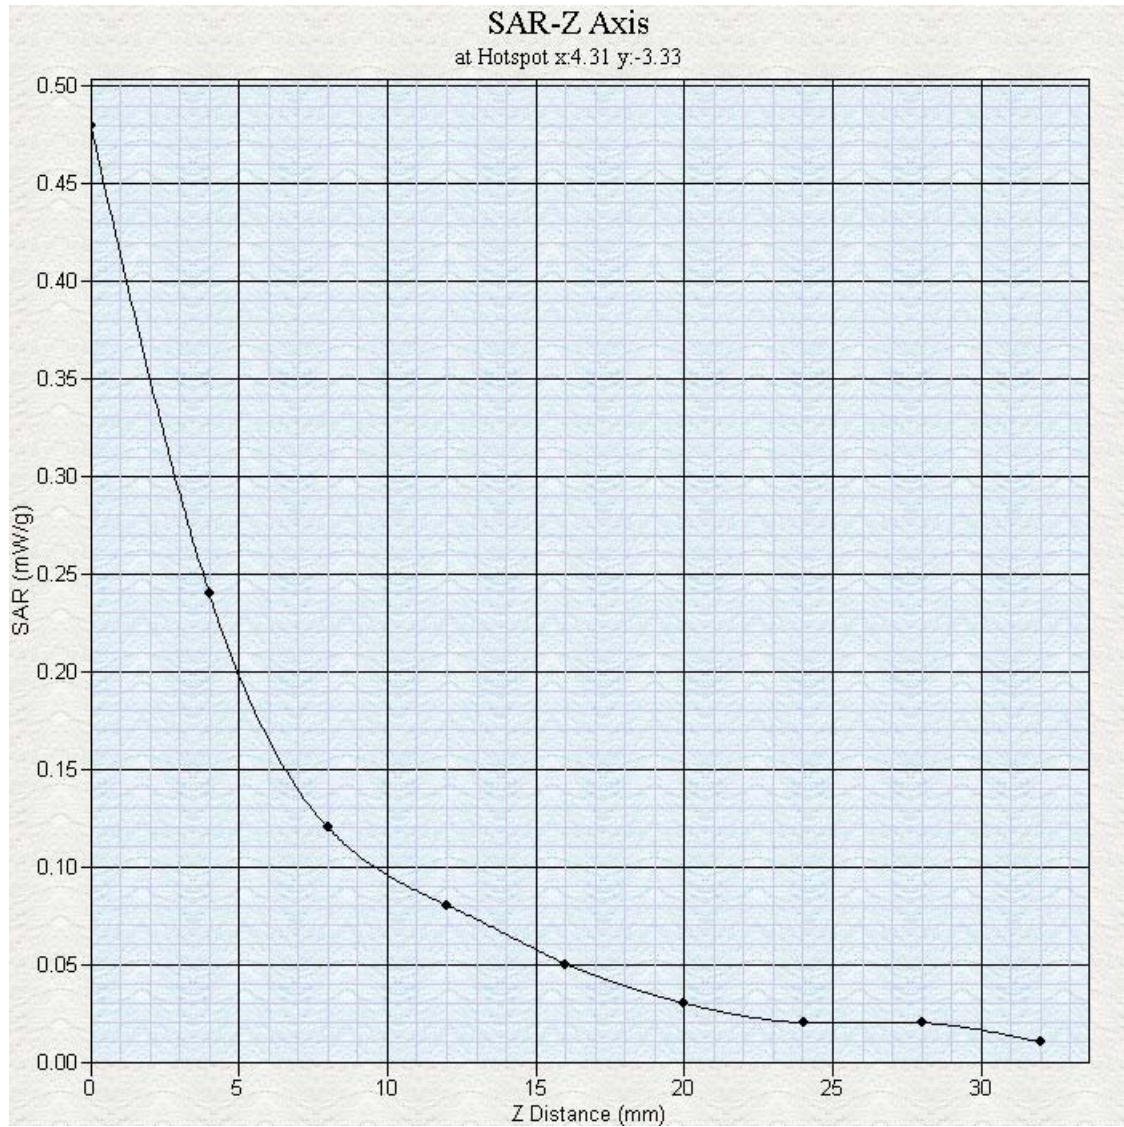

SAR Test Report

Operator : Y. Chen
 Validation Date : 16-Mar-2004
 Measurement Date : 16-Mar-2004
 Starting Time : 16-Mar-2004 01:55:34 PM
 End Time : 16-Mar-2004 02:00:31 PM
 Scanning Time : 297 secs

Product Data
 Device Name : HP Sapphire
 Serial No. : J311500PV033
 Type : Other
 Model : Sapphire
 Frequency : 2462.00 MHz
 Max. Transmit Pwr : 0.05 W
 Drift Time : 0 min(s)
 Length : 200
 Width : 180
 Depth : 10
 Antenna Type : Internal
 Power Drift-Start : 0.90
 Power Drift-Finish : 0.90
 Power Drift : 0.00

Phantom Data
 Name : APREL-Uni
 Type : Uni-Phantom
 Size : 280 x 280 x 200
 Serial No. : Stuart
 Location : Center
 Description : Uni1

Tissue Data
 Type : Body
 Serial No. : Valiation
 Frequency : 2450 MHz
 Calibration Date : 15-Mar-2004
 Temperature : 24 °C
 Ambient Temp. : 24 °C
 Humidity : 50 RH%
 Epsilon : 50 F/m
 Sigma : 1.79 S/m
 Density : 1000 kg/cu. m


Probe Data
 Name : Probe-212
 Model : E020
 Type : E-Field Triangle
 Serial No. : 212
 Calibration Date : 05-Mar-2004
 Frequency : 2450 MHz
 Duty Cycle Factor : 1
 Conversion Factor : 1.7
 Probe Sensitivity : 0.78 0.78 0.75 $\mu\text{V}/(\text{V}/\text{sq. m})$
 Compression Point : 93
 Offset : 1.56

Measurement Data

Crest Factor : 1
Scan Type : Complete
Set-up Date : 16-Mar-2004
Set-up Time : 9:42:00 AM

Other Data


DUT Position : Touch
Separation : 0
Channel : High - 2462

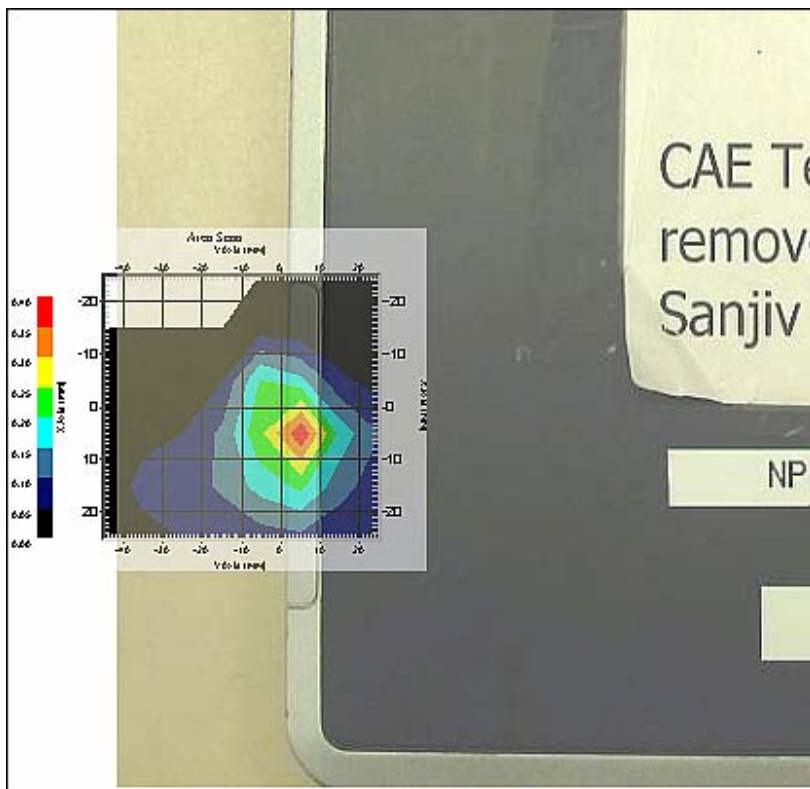

1 gram SAR value : 0.27 W/kg
Area Scan Peak SAR : 0.39
Zoom Scan Peak SAR : 0.69

Exposure Assessment Measurement Uncertainty

Source of Uncertainty	Tolerance Value	Probability Distribution	Divisor	c_i^1 (1-g)	c_i^1 (10-g)	Standard Uncertainty (1-g)	Standard Uncertainty (10-g)
Measurement System							
Probe Calibration	3.5	normal	1	1	1	3.5	3.5
Axial Isotropy	3.7	rectangular	$\sqrt{3}$	$(1-cp)_2^{1/}$	$(1-cp)_2^{1/}$	1.5	1.5
Hemispherical Isotropy	10.9	rectangular	$\sqrt{3}$	$\sqrt{cp}$	$\sqrt{cp}$	4.4	4.4
Boundary Effect	1.0	rectangular	$\sqrt{3}$	1	1	0.6	0.6
Linearity	4.7	rectangular	$\sqrt{3}$	1	1	2.7	2.7
Detection Limit	1.0	rectangular	$\sqrt{3}$	1	1	0.6	0.6
Readout Electronics	1.0	normal	1	1	1	1.0	1.0
Response Time	0.8	rectangular	$\sqrt{3}$	1	1	0.5	0.5
Integration Time	1.7	rectangular	$\sqrt{3}$	1	1	1.0	1.0
RF Ambient Condition	3.0	rectangular	$\sqrt{3}$	1	1	1.7	1.7
Probe Positioner Mech.	0.4	rectangular	$\sqrt{3}$	1	1	0.2	0.2
Restriction							
Probe Positioning with respect to Phantom Shell	2.9	rectangular	$\sqrt{3}$	1	1	2.1	2.1
Extrapolation and Integration	3.7	rectangular	$\sqrt{3}$	1	1	2.1	2.1
Test Sample Positioning	4.0	normal	1	1	1	4.0	4.0
Device Holder Uncertainty	2.0	normal	1	1	1	2.0	2.0
Drift of Output Power	0.0	rectangular	$\sqrt{3}$	1	1	0.0	0.0
Phantom and Setup							
Phantom Uncertainty(shape & thickness tolerance)	3.4	rectangular	$\sqrt{3}$	1	1	2.0	2.0
Liquid Conductivity(target)	13.0	rectangular	$\sqrt{3}$	0.7	0.5	5.3	3.8
Liquid Conductivity(meas.)	0.2	rectangular	$\sqrt{3}$	0.7	0.5	0.1	0.1
Liquid Permittivity(target)	2.0	rectangular	$\sqrt{3}$	0.6	0.5	0.8	0.6
Liquid Permittivity(meas.)	5.0	rectangular	$\sqrt{3}$	0.6	0.5	1.7	1.4
Combined Uncertainty		RSS				10.3	9.5
Combined Uncertainty (coverage factor=2)		Normal(k=2)				20.6	19.1

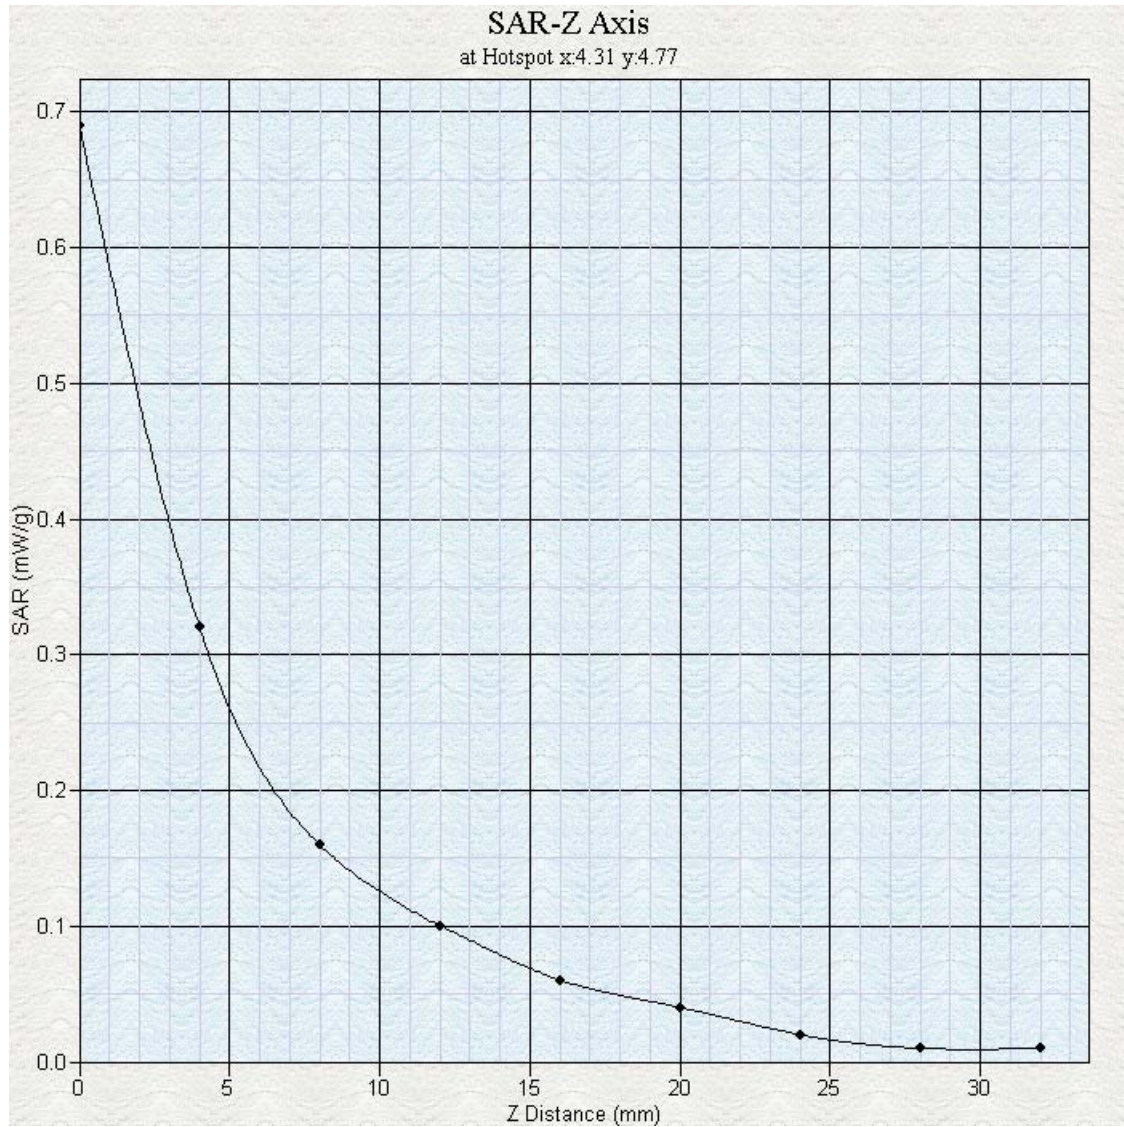

Appendix B
Probe Calibration Certificate

Project number: ITLB-Dell-5008
FCC ID: ID:CNTPP3006

51 Spectrum Way
Nepean, Ontario
Canada K2R 1E6
© 2004 APREL Laboratories

AL-065



Page 52 of 64

Tel: (613) 820-2730
Fax: (613) 820-4161
Info@aprel.com
www.aprel.com

This report shall not be reproduced, except in full, without written approval of APREL Laboratories

NCL CALIBRATION LABORATORIES

Calibration File No.: CP-339

Client.: APREL

C E R T I F I C A T E O F C A L I B R A T I O N

It is certified that the equipment identified below has been calibrated in the
NCL CALIBRATION LABORATORIES by qualified personnel following recognized
procedures and using transfer standards traceable to NRC/NIST.

Equipment: Miniature Isotropic RF Probe 2450 MHz

Manufacturer: APREL Laboratories

Model No.: E-020

Serial No.: 212

BODY Calibration

Calibration Procedure: SSI/DRB-TP-D01-032-E020

Project No: Internal

Calibrated: 3rd November 2003

Released on: 4th November 2003

This Calibration Certificate is Incomplete Unless Accompanied with the Calibration
Results Summary

Released By: _____

NCL CALIBRATION LABORATORIES

51 SPECTRUM WAY
NEPEAN, ONTARIO
CANADA K2R 1E6

Division of APREL Lab.
TEL: (613) 820-4988
FAX: (613) 820-4161



Introduction

This Calibration Report reproduces the results of the calibration performed in line with the SSI/DRB-TP-D01-032-E020 E-Field Probe Calibration Procedure. The results contained within this report are for APREL E-Field Probe E-020 209.

References

SSI/DRB-TP-D01-032-E020 E-Field Probe Calibration Procedure
IEEE 1528 "Recommended Practice for Determining the Peak Spatial-Average Specific Absorption Rate (SAR) in the Human Body Due to Wireless Communications Devices: Experimental Techniques"
SSI-TP-011 Tissue Calibration Procedure

Conditions

Probe 209 was a new probe taken from stock prior to calibration.

Ambient Temperature of the Laboratory: 22 °C +/- 0.5°C
Temperature of the Tissue: 21 °C +/- 0.5°C

Calibration Results Summary

Probe Type:	E-Field Probe E-020
Serial Number:	212
Frequency:	2450 MHz
Sensor Offset:	1.56 mm
Sensor Length:	2.5 mm
Tip Enclosure:	Ertalyte*
Tip Diameter:	5 mm
Tip Length:	60 mm
Total Length:	290 mm

*Resistive to recommended tissue recipes per IEEE-1528

Sensitivity in Air

Channel X:	$0.78 \mu\text{V}/(\text{V}/\text{m})^2$
Channel Y:	$0.78 \mu\text{V}/(\text{V}/\text{m})^2$
Channel Z:	$0.75 \mu\text{V}/(\text{V}/\text{m})^2$
Diode Compression Point:	93 mV

Sensitivity in Body Tissue

Frequency: 2450 MHz

Epsilon: 50.6 (+/-5%) **Sigma:** 1.98 S/m (+/-10%)

ConvF

Channel X: 1.70

Channel Y: 1.70

Channel Z: 1.70

Tissue sensitivity values were calculated using the load impedance of the APREL Laboratories Daq-Paq.


Boundary Effect:

Uncertainty resulting from the boundary effect is less than 2% for the distance between the tip of the probe and the tissue boundary, when less than 2.4mm.



Spatial Resolution:

The measured probe tip diameter is 5 mm (+/- 0.01 mm) and therefore meets the requirements of SSI/DRB-TP-D01-032 for spatial resolution.

Receiving Pattern 2450 MHz (Air)

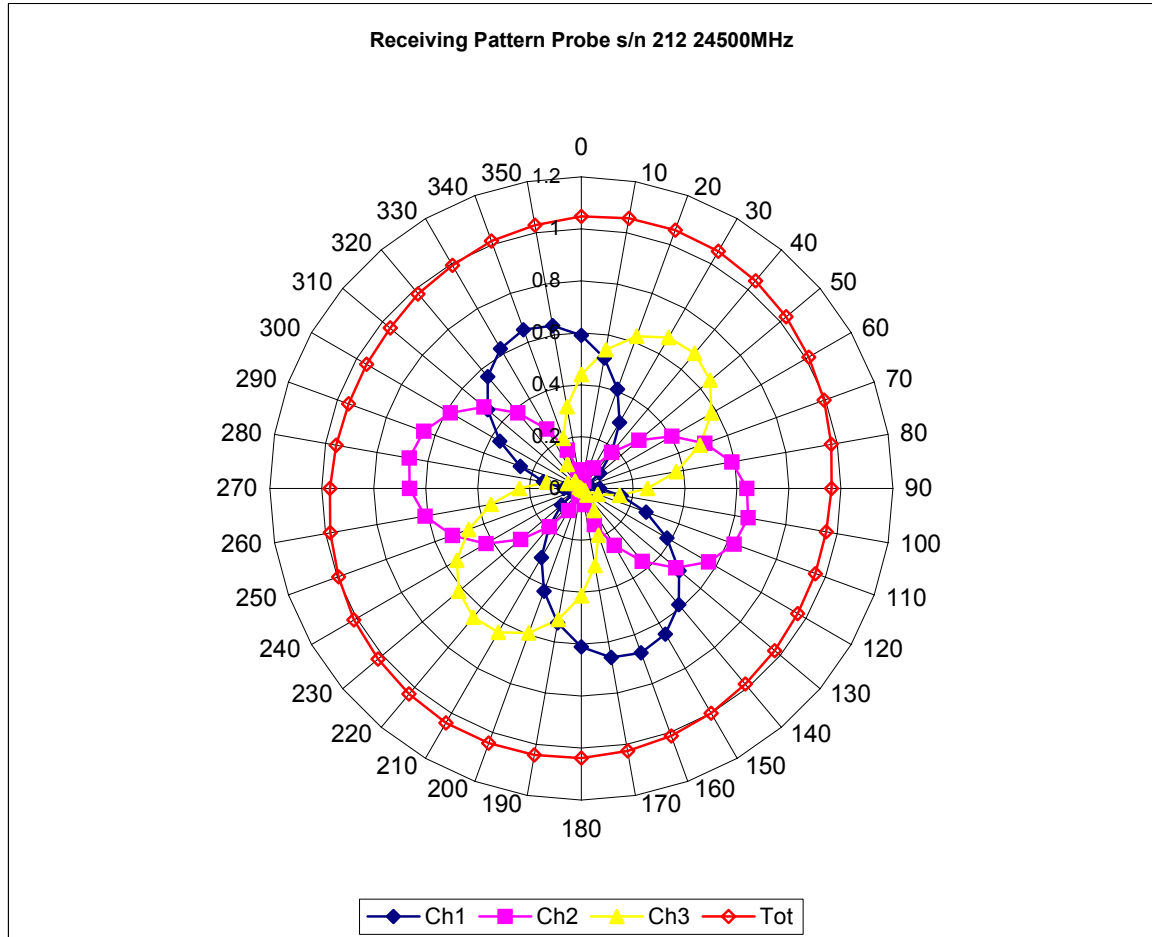


Isotropy Error 2450 MHz (Air)

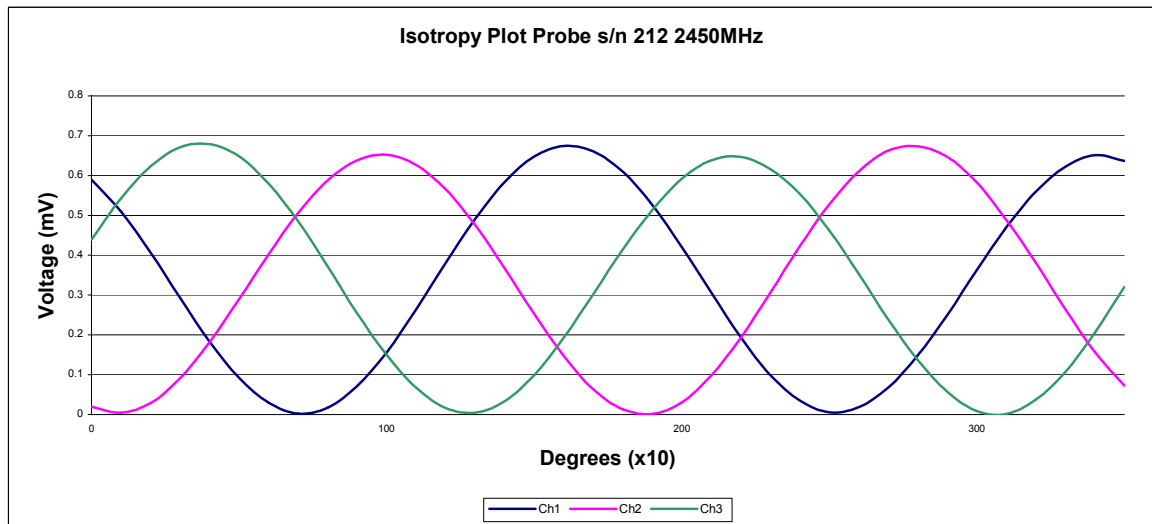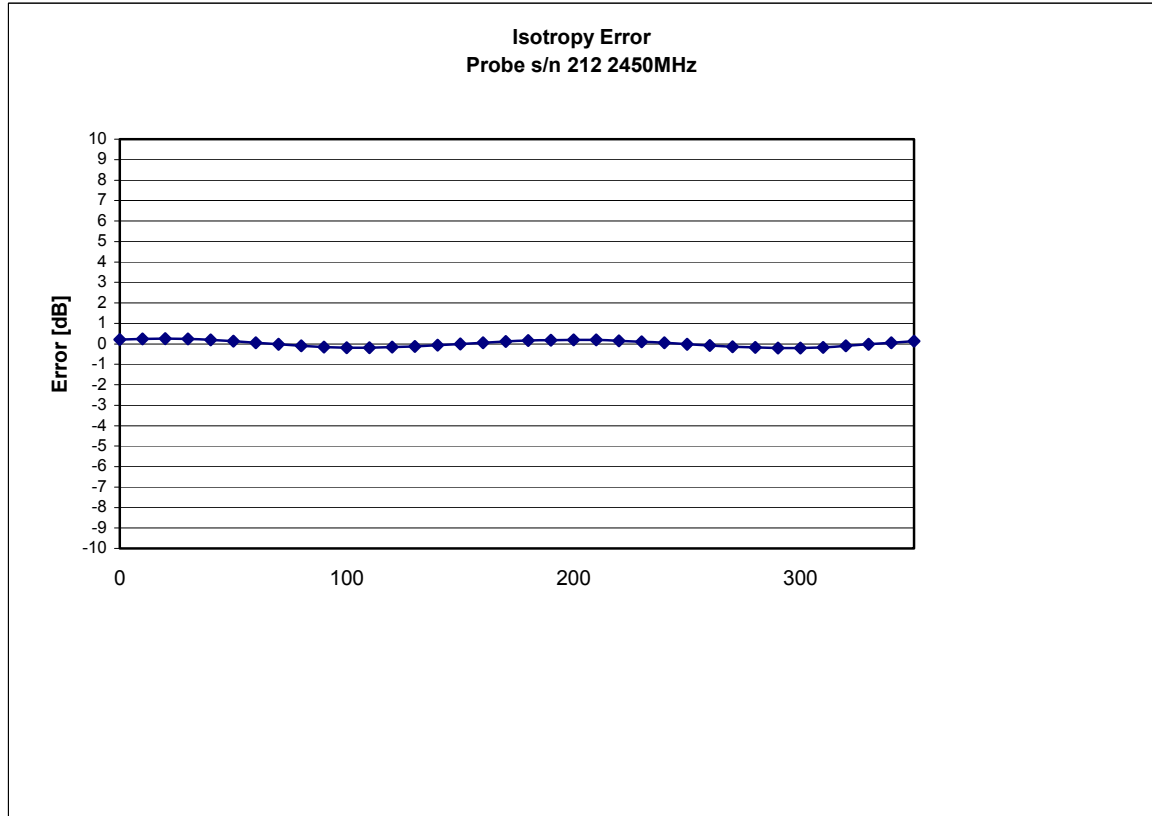

Isotropy:


0.10 dB

Dynamic Range

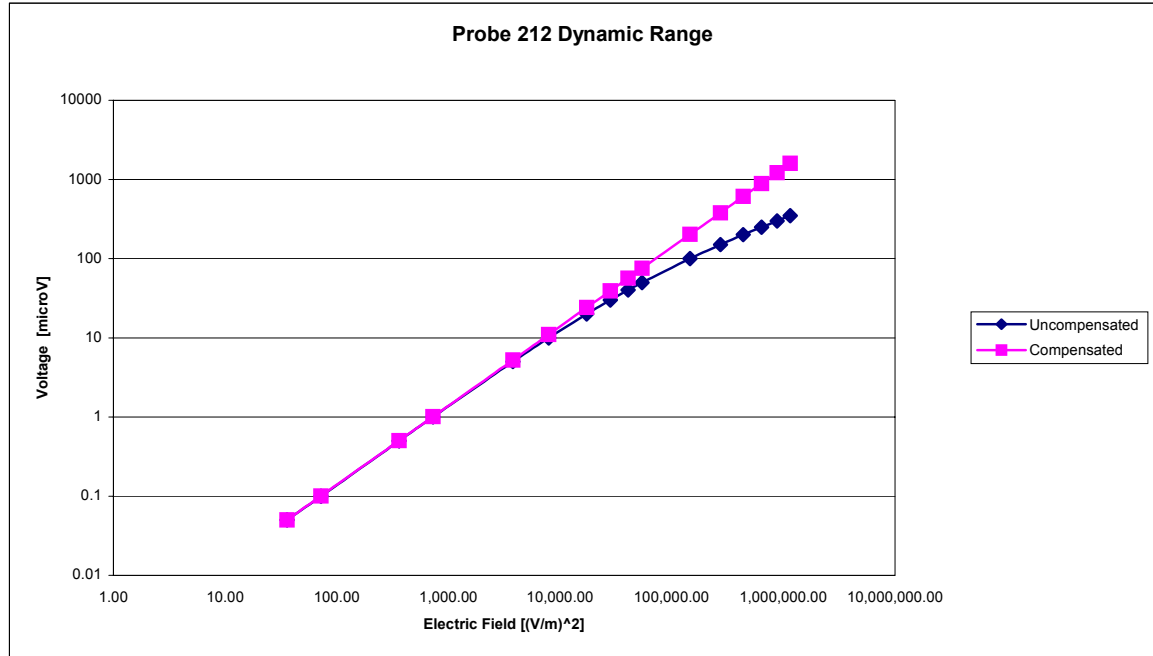

Video Bandwidth

Probe Frequency Characteristics

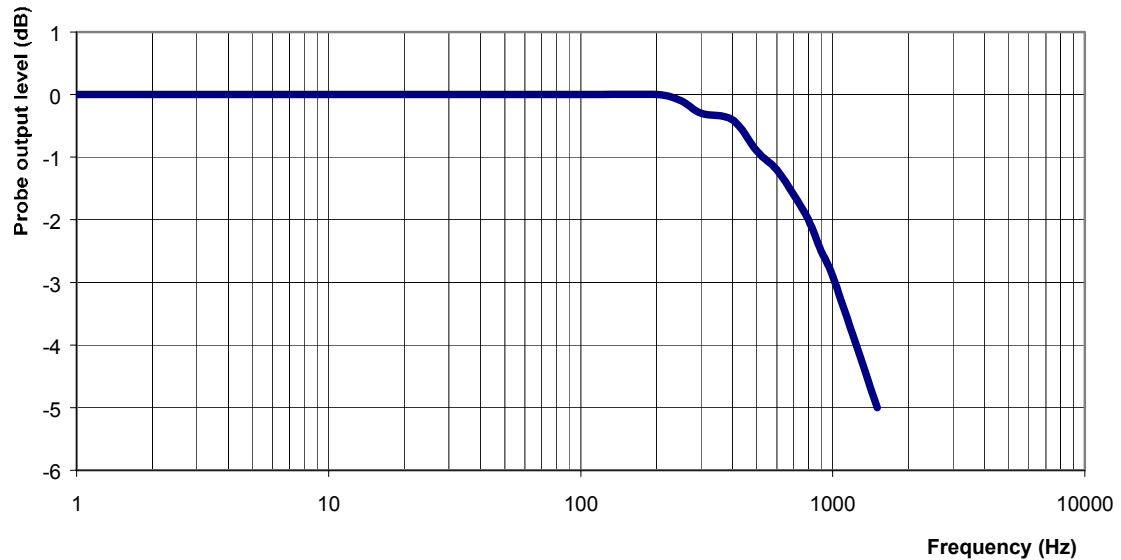

Video Bandwidth at 500 Hz 1 dB
Video Bandwidth at 1.02 KHz: 3 dB

Conversion Factor Uncertainty Assessment

Frequency: 2450MHz

Epsilon: 50.6 (+/-5%)

Sigma: 1.98 S/m (+/-10%)

ConvF

Channel X: 1.70 7%(K=2)

Channel Y: 1.70 7%(K=2)

Channel Z: 1.70 7%(K=2)

To minimize the uncertainty calculation all tissue sensitivity values were calculated using a load impedance of 5 MΩ.

Boundary Effect:

For a distance of 2.4mm the evaluated uncertainty (increase in the probe sensitivity) is less than 2%.

Test Equipment

The test equipment used during Probe Calibration, manufacturer, model number and, current calibration status are listed and located on the main APREL server R:\NCL\Calibration Equipment\Instrument List May 2003.

Appendix C Dipole Calibration Certificate

Project number: ITLB-Dell-5008
FCC ID: ID:CNTPP3006

51 Spectrum Way
Nepean, Ontario
Canada K2R 1E6
© 2004 APREL Laboratories

AL-065



Page 63 of 64

Tel: (613) 820-2730
Fax: (613) 820-4161
Info@aprel.com
www.aprel.com

This report shall not be reproduced, except in full, without written approval of APREL Laboratories

NCL CALIBRATION LABORATORIES

Calibration File No: DC-0265

Project Number: Internal

C E R T I F I C A T E O F C A L I B R A T I O N

It is certified that the equipment identified below has been calibrated in the
NCL CALIBRATION LABORATORIES by qualified personnel following recognized
procedures and using transfer standards traceable to NRC/NIST.

APREL Validation Dipole

Manufacturer: APREL Laboratories

Part number: D-2450-S-1

Frequency: 2.45 GHz

Serial No: ALCD-10

Customer: APREL

Calibrated: 14 November 2003

Released on: 15 November 2003

Released By: _____

NCL CALIBRATION LABORATORIES

51 SPECTRUM WAY
NEPEAN, ONTARIO
CANADA K2R 1E6

Division of APREL Lab.
TEL: (613) 820-4988
FAX: (613) 820-4161



Calibration Results Summary

The following results relate the Calibrated Dipole and should be used as a quick reference for the user.

Mechanical Dimensions


Length: 51.7 mm
Height: 30.8 mm

Electrical Specification

SWR: 1.181U
Return Loss: -21.4 dB
Impedance: 46.175

System Validation Results

Frequency	1 Gram	10 Gram	Peak
2.45 GHz	52.45	22.91	102.91

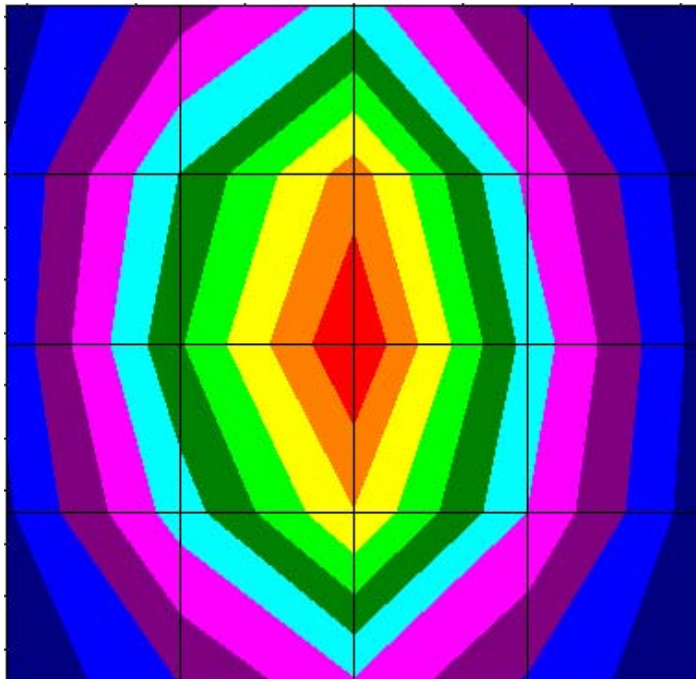

Introduction

This Calibration Report has been produced in line with the SSI Dipole Calibration Procedure SSI-TP-018. The results contained within this report are for Validation Dipole ALCD-10 at 2.45 GHz. The calibration routine consisted of a three-step process. Step 0.05 Was a mechanical verification of the dipole to ensure that it meets the IEEE mechanical specification. Step 2 was an Electrical Calibration for the Validation Dipole, where the SWR, Impedance, and the Return loss were assessed. Step 3 involved a System Validation using the ALIDX-500, along with the APREL Reference E-010 130 MHz to 26 GHz E-Field Probe Serial Number 163.

References

SSI-TP-018 Dipole Calibration Procedure
SSI-TP-016 Tissue Calibration Procedure
IEEE 1528 *DRAFT* "Recommended Practice for Determining the Peak Spatial-Average Specific Absorption Rate (SAR) in the Human Body Due to Wireless Communications Devices: Experimental Techniques"

Conditions

Dipole ALCD-10 was a new Dipole taken from stock prior to calibration.

Ambient Temperature of the Laboratory: 24 °C +/- 0.5°C
Temperature of the Tissue: 20 °C +/- 0.5°C

Dipole Calibration Results**Mechanical Verification**

IEEE Length	IEEE Height	Measured Length	Measured Height
51.5 mm	30.4 mm	51.7 mm	30.8 mm

Tissue Validation

Head Tissue 2450 MHz	Measured
Dielectric constant, ϵ_r	39.2
Conductivity, σ [S / m]	1.82
Tissue Conversion Factor,	4.61

Electrical Calibration


Test	Result	IEEE Value
S11 R/L	-21.4	-21 dB
SWR	1.181U	-
Impedance	46.175 Ω	

The Following Graphs are the results as displayed on the Vector Network Analyzer.

S11 Parameter Return Loss

S11 FORWARD REFLECTION

LOG MAGNITUDE REF=0.000 dB 10.000 dB/DIV

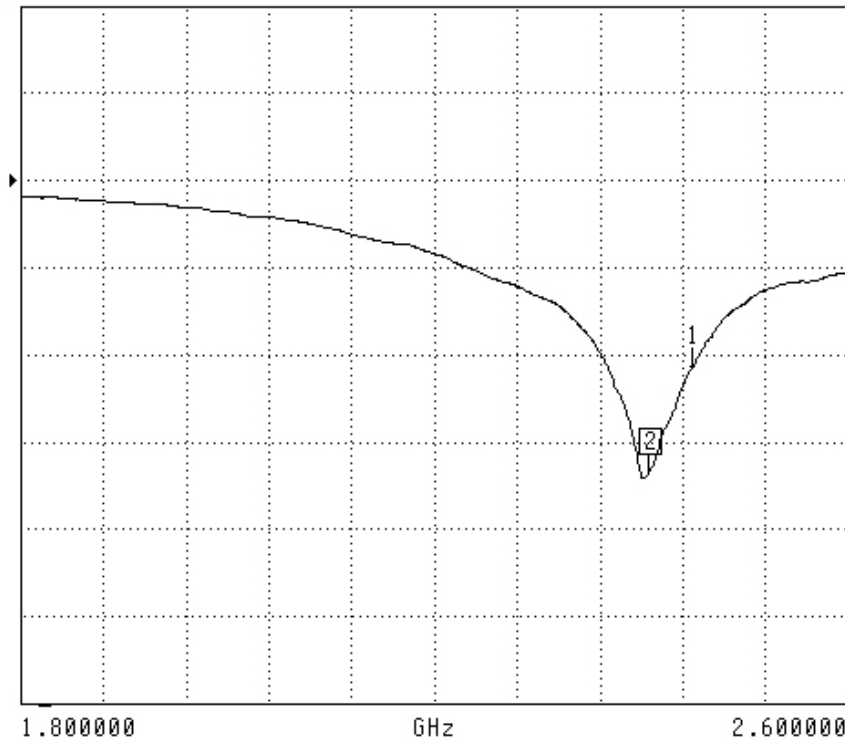

CH 1 - S11
REFERENCE PLANE
5.1160 mm

MARKER 2
2.408000 GHz
-33.566 dB


MARKER TO MAX
▶ MARKER TO MIN

1 2.450000 GHz
-21.377 dB

MARKER READOUT
FUNCTIONS

SWR

S11 FORWARD REFLECTION

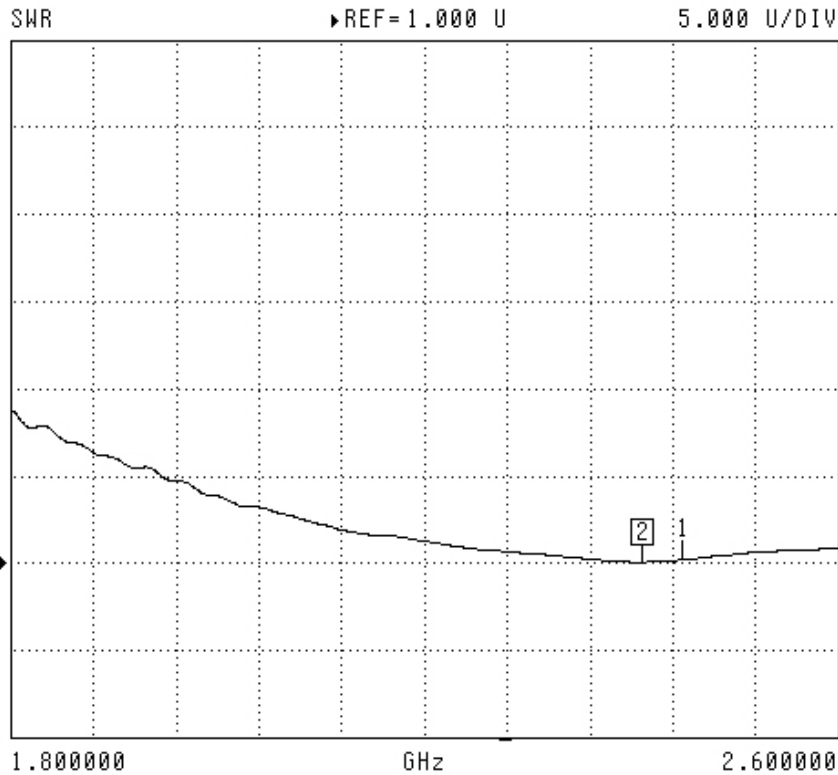

CH 1 - S11
REFERENCE PLANE
5.1160 mm

MARKER 2
2.411000 GHz
1.049 U


MARKER TO MAX
▶ MARKER TO MIN

1 2.450000 GHz
1.181 U

MARKER READOUT
FUNCTIONS

Smith Chart Dipole Impedance

S11 FORWARD REFLECTION
IMPEDANCE

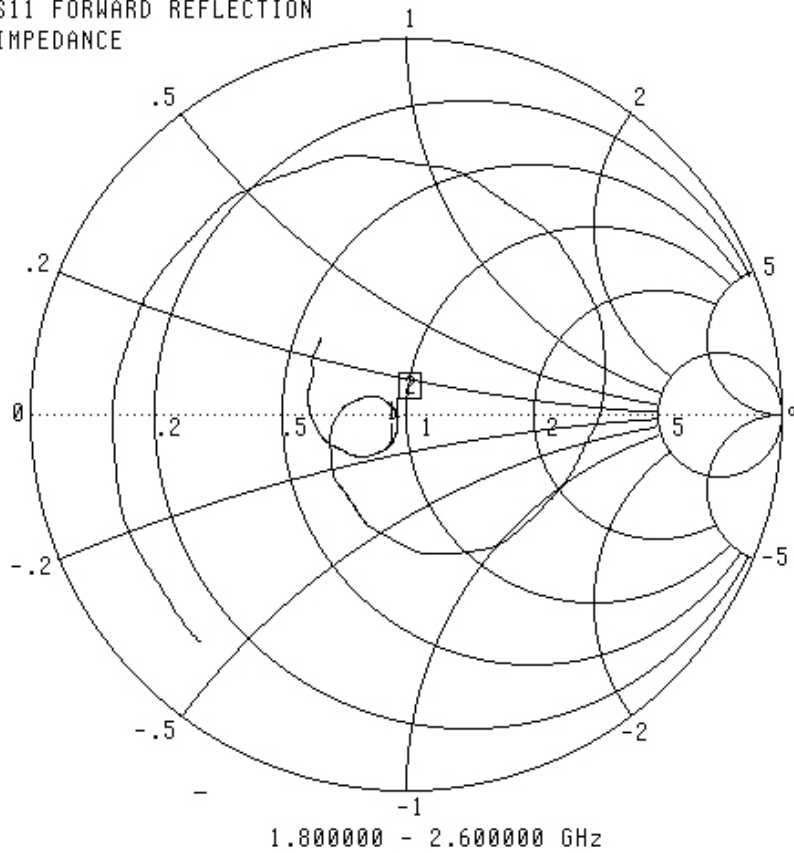

CH 1 - S11
REFERENCE PLANE
5.1160 mm

MARKER 2
2.411000 GHz
48.080 Ω
-1.171 jΩ


MARKER TO MAX
▶ MARKER TO MIN
1 2.450000 GHz
46.175 Ω
-7.199 jΩ

MARKER READOUT
FUNCTIONS

System Validation Results Using the Electrically Calibrated Dipole

Frequency	1 Gram	10 Gram	Peak Above Feed Point
2.45 GHz	52.45	22.91	102.91

The following Graphic Plot is the splined measurement result for the course scan.

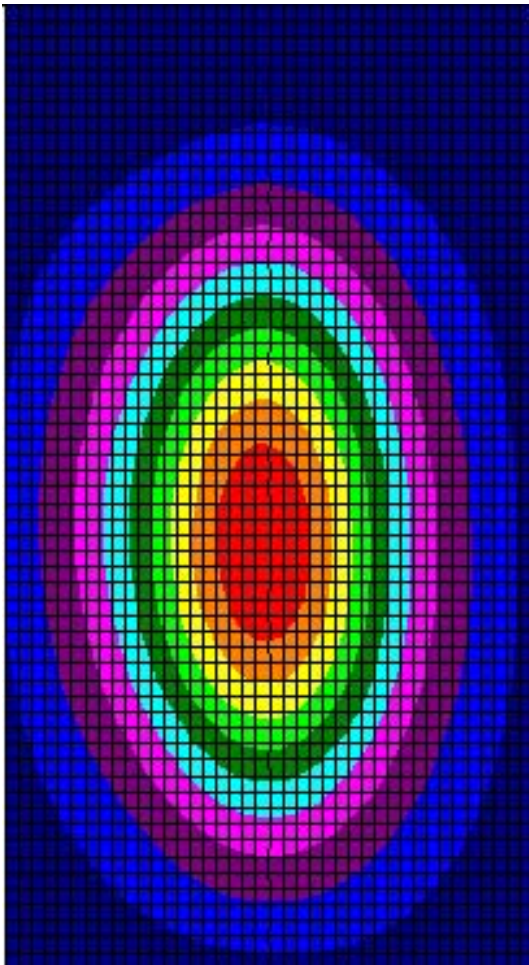

Test Equipment

The test equipment used during Probe Calibration, manufacturer, model number and, current calibration status are listed and located on the main APREL server
R:\NCL\Calibration Equipment\Instrument List May 2003

