



### Zimmer CAS 20-8011-000-03 Internal Photos



Top View



Bottom View




Right Side View



Left Side View

Four devices are always packaged together in a box as shown in the picture below. The packaging is sealed and sterilized. The product is used for orthopaedic surgeries. Because the content must be kept sterile, it can only be opened during a surgery, inside the sterile field of the operating room. The devices are disposable, so they are only used once. Because of these reasons, the necessary markings are located on the outer box, where the medical personnel can access it before using the product.

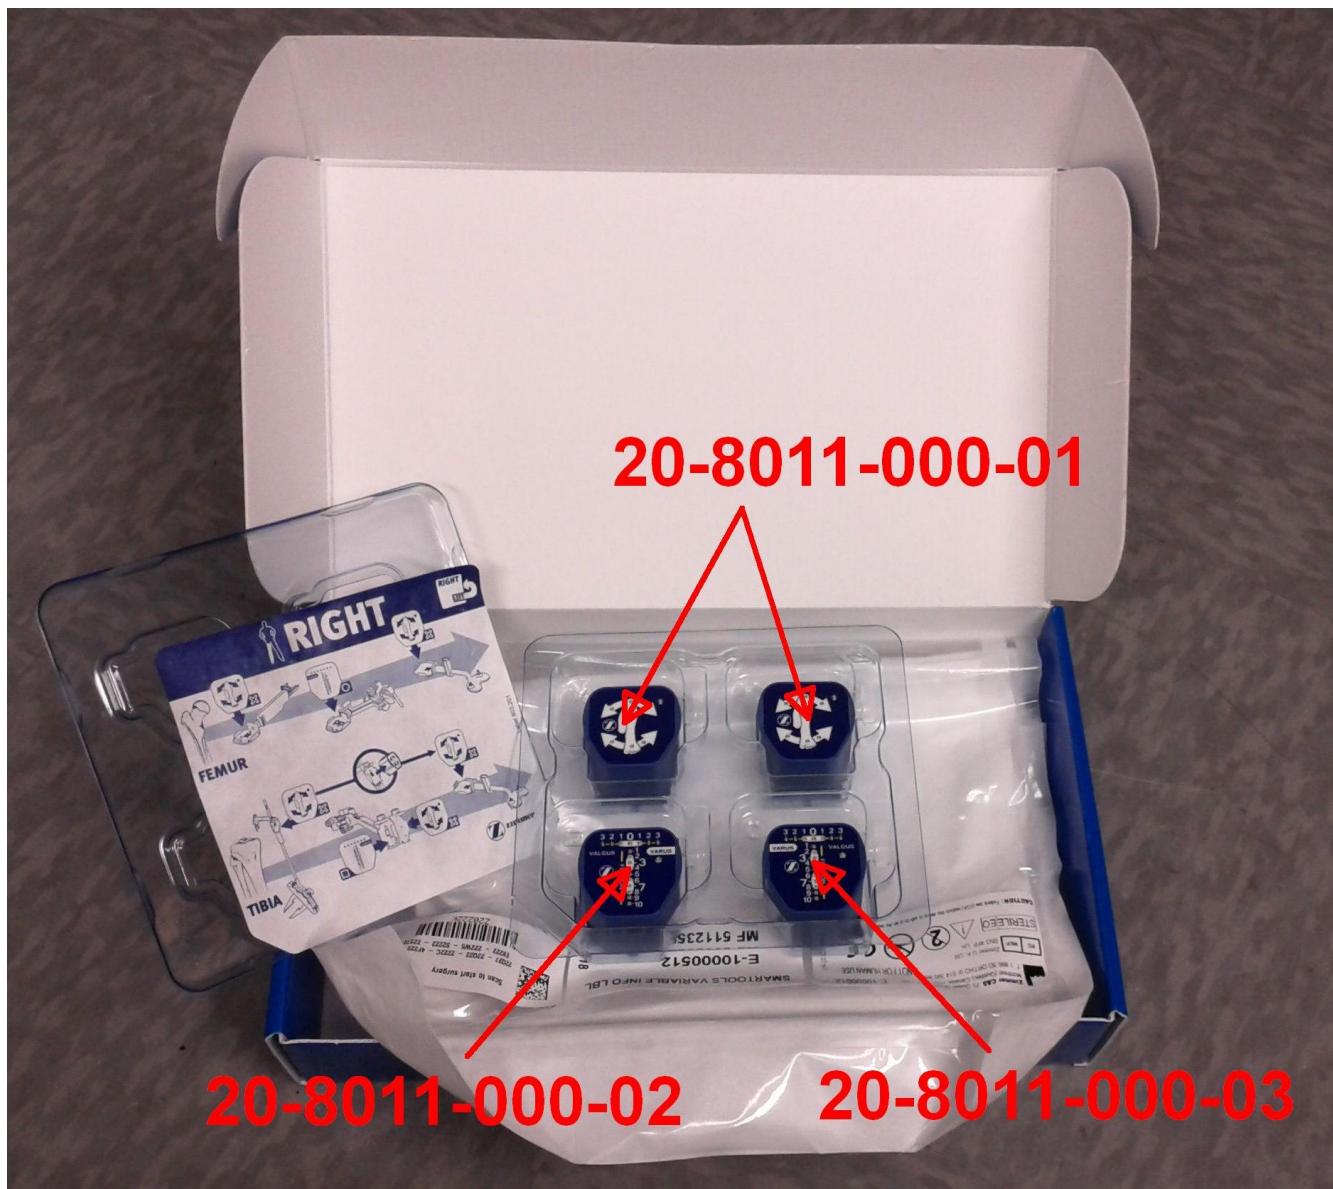

Devices inside the packaging