

Guidant Corporation MN

Zoom 2920

July 29, 2004

Report No. GDMN0003

Report Prepared By:



www.nwemc.com
1-888-EMI-CERT

Test Report



22975 NW Evergreen Parkway
Suite 400
Hillsboro, Oregon 97124

Certificate of Test
Issue Date: July 29, 2004
Guidant Corporation MN
Model: Zoom 2920

Emissions			
Specification	Test Method	Pass	Fail
FCC 15.209:2003	ANSI C63.4:2001 Fundamental Field Strength	☒	☐
FCC 15.209:2003	ANSI C63.4:2001 Radiated Spurious Emissions	☒	☐
FCC 15.207:2003	ANSI C63.4:2001 Conducted Emissions	☒	☐

Modifications made to the product

See the Modifications section of this report

Approved By:

Don Fecteau, IS Manager

This report must not be used to claim product certification, approval, or endorsement by NVLAP, NIST, or any agency of the federal government of the United States of America.

Product compliance is the responsibility of the client, therefore the tests and equipment modes of operation represented in this report were agreed upon by the client, prior to testing. This Report may only be duplicated in its entirety. The results of this test pertain only to the sample(s) tested, the specific description is noted in each of the individual sections of the test report supporting this certificate of test.

Revision Number	Description	Date	Page Number
00	None		

FCC: Accredited by NVLAP for performance of FCC radio, digital, and ISM device testing. Our Open Area Test Sites, certification chambers, and conducted measurement facilities, have been fully described in reports filed with the FCC and accepted by the FCC in letters maintained in our files. Northwest EMC has been accredited by ANSI to ISO / IEC Guide 65 as a product certifier. We have been designated by the FCC as a Telecommunications Certification Body (TCB). This allows Northwest EMC to certify transmitters to FCC specifications in accordance with 47 CFR 2.960 and 2.962.



NVLAP: Northwest EMC, Inc. is recognized under the United States Department of Commerce, National Institute of Standards and Technology, National Voluntary Laboratory Accreditation Program for satisfactory compliance with the requirements of ISO/IEC 17025 for Testing Laboratories. The NVLAP accreditation encompasses Electromagnetic Compatibility Testing in accordance with the European Union EMC Directive 89/336/EEC, ANSI C63.4, MIL-STD 461E, DO-160D and SAE J1113. Additionally, Northwest EMC is accredited by NVLAP to perform radio testing in accordance with the European Union R&TTE Directive 1999/5/EEC, the requirements of FCC, and the RSS radio standards for Industry Canada. Accreditation has been granted to Northwest EMC, Inc. under Certificate Numbers: 200629-0, 200630-0, and 200676-0.



Industry Canada: Accredited by NVLAP for performance of Industry Canada RSS and ICES testing. Our Open Area Test Sites and certification chambers comply with RSS 212, Issue 1 (Provisional) and have been filed with Industry Canada and accepted. Northwest EMC has been accredited by ANSI to ISO / IEC Guide 65 as a product certifier. We have been designated by NIST and recognized by Industry Canada as a Certification Body (CB) per the APEC Mutual Recognition Arrangement (MRA). This allows Northwest EMC to certify transmitters to Industry Canada technical requirements.



CAB: Designated by NIST and validated by the European Commission as a Conformity Assessment Body (CAB) to conduct tests and approve products to the EMC directive and transmitters to the R&TTE directive, as described in the U.S. - EU Mutual Recognition Agreement



TÜV Product Service: Included in TÜV Product Service Group's Listing of Recognized Laboratories. It qualifies in connection with the TÜV Certification after Recognition of Agent's Testing Program for the product categories and/or standards shown in TÜV's current Listing of CARAT Laboratories available from TÜV. A certificate was issued to represent that this laboratory continues to meet TÜV's CARAT Program requirements. Certificate No. USA0401C



TÜV Rheinland: Authorized to carryout EMC tests by order and under supervision of TÜV Rheinland. This authorization is based on "Conditions for EMC-Subcontractors" of November 1992.



NEMKO: Assessed and accredited by NEMKO (Norwegian testing and certification body) for European emissions and immunity testing. As a result of NEMKO's laboratory assessment, they will accept test results from Northwest EMC, Inc. for product certification (Authorization No. ELA 119).



Technology International: Assessed in accordance with ISO Guide 25 defining the general international requirements for the competence of calibration and testing laboratories and with ITI assessment criteria LACO196. Based upon that assessment Interference Technology International, Ltd., has granted approval for specifications implementing the EU Directive on EMC (89/336/EEC and amendments). The scope of the approval was provided on a Schedule of Assessment supplied with the certificate and is available upon request.



Australia/New Zealand: The National Association of Testing Authorities (NATA), Australia has been appointed by the ACA as an accreditation body to accredit test laboratories and competent bodies for EMC standards. Accredited test reports or assessments by competent bodies must carry the NATA logo. Test reports made by an overseas laboratory that has been accredited for the relevant standards by an overseas accreditation body that has a Mutual Recognition Agreement (MRA) with NATA are also accepted as technical grounds for product conformity. The report should be endorsed with the respective logo of the accreditation body. (NVLAP)



VCCI: Accepted as an Associate Member to the VCCI, Acceptance No. 564. Conducted and radiated measurement facilities have been registered in accordance with Regulations for Voluntary Control Measures, Article 8. (*Registration Nos. - Evergreen: C-1071 and R-1025, Trails End: C-1877 and R-1760, Sultan: R-871, C-1784 and R-1761*)



BSMI: Northwest EMC has been designated by NIST and validated by C-Taipei (BSMI) as a CAB to conduct tests as described in the APEC Mutual Recognition Agreement. License No.SL2-IN-E-1017.



GOST: Northwest EMC, Inc. has been assessed and accredited by the Russian Certification bodies Certinform VNIINMASH, CERTINFO, SAMTES, and Federal CHEC, to perform EMC and Hygienic testing for Information Technology Products. As a result of their laboratory assessment, they will accept test results from Northwest EMC, Inc. for product certification



SCOPE

For details on the Scopes of our Accreditations, please visit:

<http://www.nwemc.com/scope.asp>

What is measurement uncertainty?

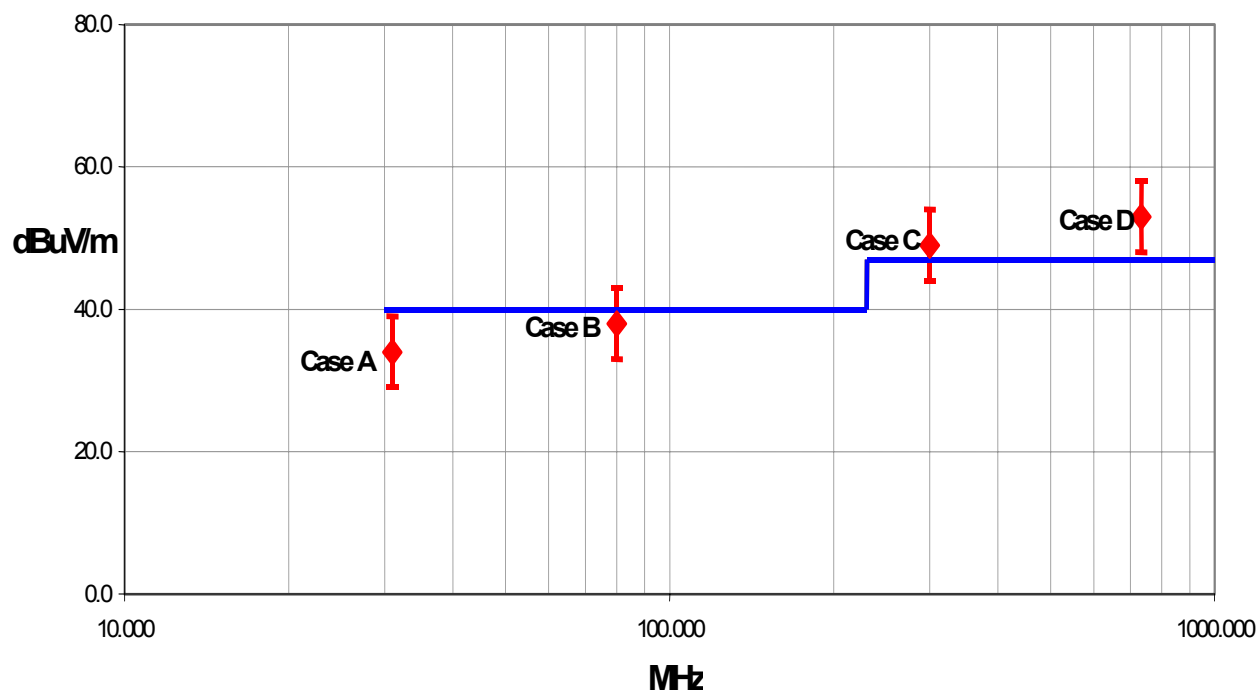
When a measurement is made, the result will be different from the true or theoretically correct value. The difference is the result of tolerances in the measurement system that cannot be completely eliminated. To the extent that technology allows us, it has been our aim to minimize this error. The following statement of measurement uncertainty is used to reflect the accuracy of the measured result as compared with its “true” value. In the case of transient tests (ESD, EFT, Surge, Voltage Dips and Interruptions), the test equipment has been demonstrated by calibration to provide at least a 95% confidence that it complies with the test specification requirements.

The following documents were the basis for determining the uncertainty levels of our measurements:

- “ISO Guide to the Expression of Uncertainty in Measurements”, October 1993
- “NIS81: The Treatment of Uncertainty in EMC Measurements”, May 1994
- “IEC CISPR 16-3 A1 f1 Ed.1: Radio-interference measurements and statistical techniques”, December 2000

How might measurement uncertainty be applied to test results?

If the diamond marks the measured value for the test and the vertical bars bracket the range of + and – measurement uncertainty, then test results can be interpreted from the diagram below.

**Test Result Scenarios:**

Case A: Product complies.

Case B: Product conditionally complies. It is not possible to say with 95% confidence that the product complies.

Case C: Product conditionally does not comply. It is not possible to say with 95% confidence that the product does not comply.

Case D: Product does not comply.

Radiated Emissions ≤ 1 GHz

Value (dB)

Test Distance	Probability Distribution	Biconical Antenna		Log Periodic Antenna		Dipole Antenna	
		3m	10m	3m	10m	3m	10m
Combined standard uncertainty $u_c(y)$	normal	+ 1.86 - 1.88	+ 1.82 - 1.87	+ 2.23 - 1.41	+ 1.29 - 1.26	+ 1.31 - 1.27	+ 1.25 - 1.25
Expanded uncertainty U (level of confidence $\approx 95\%$)	normal (k=2)	+ 3.72 - 3.77	+ 3.64 - 3.73	+ 4.46 - 2.81	+ 2.59 - 2.52	+ 2.61 - 2.55	+ 2.49 - 2.49

Radiated Emissions > 1 GHz

Value (dB)

Test Distance	Probability Distribution	Without High Pass Filter		With High Pass Filter	
		3m	10m	3m	10m
Combined standard uncertainty $u_c(y)$	normal	+ 1.29 - 1.25	+ 1.29 - 1.25	+ 1.38 - 1.35	+ 1.38 - 1.35
Expanded uncertainty U (level of confidence $\approx 95\%$)	normal (k=2)	+ 2.57 - 2.51	+ 2.57 - 2.51	+ 2.76 - 2.70	+ 2.76 - 2.70

Conducted Emissions

Test Distance	Probability Distribution	Value (+/- dB)	
		3m	10m
Combined standard uncertainty $u_c(y)$	normal	1.48	1.48
Expanded uncertainty U (level of confidence $\approx 95\%$)	normal (k = 2)	2.97	2.97

Radiated Immunity

Test Distance	Probability Distribution	Value (+/- dB)	
		3m	10m
Combined standard uncertainty $u_c(y)$	normal	1.05	1.05
Expanded uncertainty U (level of confidence $\approx 95\%$)	normal (k = 2)	2.11	2.11

Conducted Immunity

Test Distance	Probability Distribution	Value (+/- dB)	
		3m	10m
Combined standard uncertainty $u_c(y)$	normal	1.05	1.05
Expanded uncertainty U (level of confidence $\approx 95\%$)	normal (k = 2)	2.10	2.10

Legend

$u_c(y)$ = square root of the sum of squares of the individual standard uncertainties

U = combined standard uncertainty multiplied by the coverage factor: k . This defines an interval about the measured result that will encompass the true value with a confidence level of approximately 95%. If a higher level of confidence is required, then $k=3$ (CL of 99.7%) can be used. Please note that with a coverage factor of one, $u_c(y)$ yields a confidence level of only 68%.

**California****Orange County Facility**

41 Tesla Ave.
Irvine, CA 92618
(888) 364-2378
FAX (503) 844-3826

**Oregon****Evergreen Facility**

22975 NW Evergreen Pkwy.,
Suite 400
Hillsboro, OR 97124
(503) 844-4066
FAX (503) 844-3826

**Oregon****Trails End Facility**

30475 NE Trails End Lane
Newberg, OR 97132
(503) 844-4066
FAX (503) 537-0735

**Washington****Sultan Facility**

14128 339th Ave. SE
Sultan, WA 98294
(888) 364-2378
FAX (360) 793-2536

Party Requesting the Test

Company Name:	Guidant Corporation MN
Address:	4100 Hamline Avenue North
City, State, Zip:	Saint Paul, MN 55112-5798
Test Requested By:	Yogi Shah
Model:	Zoom 2920
First Date of Test:	07-15-04
Last Date of Test:	07-28-04
Receipt Date of Samples:	06-30-04
Equipment Design Stage:	Production
Equipment Condition:	No visual damage.

Information Provided by the Party Requesting the Test

Clocks/Oscillators:	41 kHz, 40MHz, 33.3MHz, 100MHz, 66.6MHz, 4.1MHz, 41.667MHz, 6MHz, 32.768kHz, 14.318MHz, 16.67MHz, 24MHz, 25MHz, 48MHz, 16MHz, 10MHz, 210.38MHz, 833.52MHz, 13MHz
I/O Ports:	Telemetry Wand

Functional Description of the EUT (Equipment Under Test):

The ZOOM® LATITUDE™ Programming System, which includes the Model 2920 Programmer/Recorder/Monitor (PRM), is a portable cardiac rhythm management system designed to be used with certain models of Guidant implantable pulse generators. It is a telemetry system operating under 15.209 using the telemetry. The Model 2920 PRM is designed to be used only with the Model 6577 Sterilizable Telemetry Wand. The Model 2920 is provided with only one available antenna to meet the unique antenna requirements of 47 CFR 15.203.

Client Justification for EUT Selection:

The product is a representative production sample.

Client Justification for Test Selection:

Tests required to meet the FCC requirements for approval.

Equipment modifications					
Item	Test	Date	Modification	Note	Disposition of EUT
1	Conducted Emissions	07/15/2004	No EMI suppression devices were added or modified during this test.	Same configuration as delivered.	EUT remained at Northwest EMC.
2	Radiated Emissions	07/28/2004	No EMI suppression devices were added or modified during this test.	Same configuration as in previous test.	EUT remained at Northwest EMC.

Justification

The individuals and/or the organization requesting the test provided the modes, configurations and settings available to evaluate. All of the EUT parameters listed below were investigated. This includes, but may not be limited to, CPU speeds, video resolution settings, operational modes, and input voltages.

Operating Modes Investigated:

Typical operating mode

Power Input Settings Investigated:

120 VAC, 60 Hz

Software\Firmware Applied During Test

Exercise Software	Product 2909 System Software Quick Start	Version	Version 4.1 Version 1.38
Description			
The system was tested using standard operating production software to exercise the functions of the device during the testing.			

EUT and Peripherals in Test Setup Boundary

Description	Manufacturer	Model/Part Number	Serial Number
Programmer	Guidant	2920	022394
Pulse Generator	Guidant	Vitality AVT	106433
Pulse Generator	Guidant	Renewal TR	100088
Pulse Generator	Guidant	Insignia I Plus	104568
Loop Sensor	Guidant	6577	none

Cables

Cable Type	Shield	Length (m)	Ferrite	Connection 1	Connection 2
AC Power	No	2.3	No	Programmer	AC Mains
Loop Sensor	PA	3.0	PA	Loop Sensor	Programmer
Vitality Patient Leads	PA	0.5	PA	Vitality AVT	Termination
Renewal Patient Leads	PA	0.5	PA	Renewal TR	Termination
Insignia Patient Leads	PA	0.1	PA	Insignia I Plus	Termination
PA = Cable is permanently attached to the device. Shielding and/or presence of ferrite may be unknown.					

Measurement Equipment

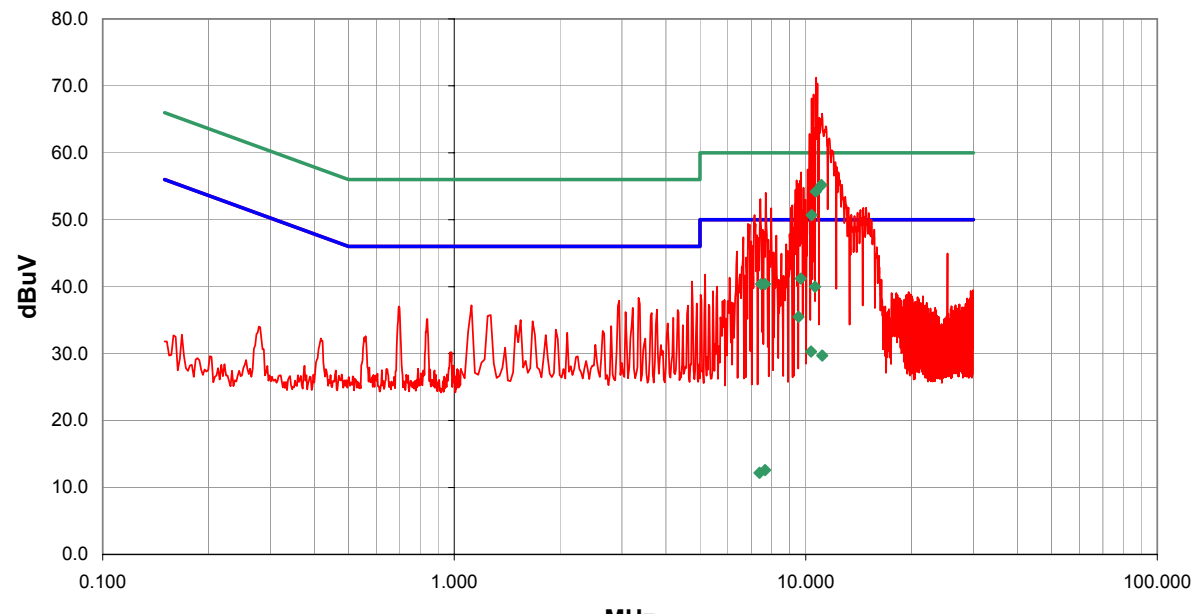
Description	Manufacturer	Model	Identifier	Last Cal	Interval
LISN	Solar	9252-50-24-BNC	LIA	12/16/2003	13 mo
LISN	Solar	9252-50-R-24-BNC	LIQ	12/17/2003	13 mo
Spectrum Analyzer	Hewlett Packard	8593E	AAP	03/22/2004	13 mo
Receiver	Schaffner	SCR 3101	ARC	04/28/2003	24 mo

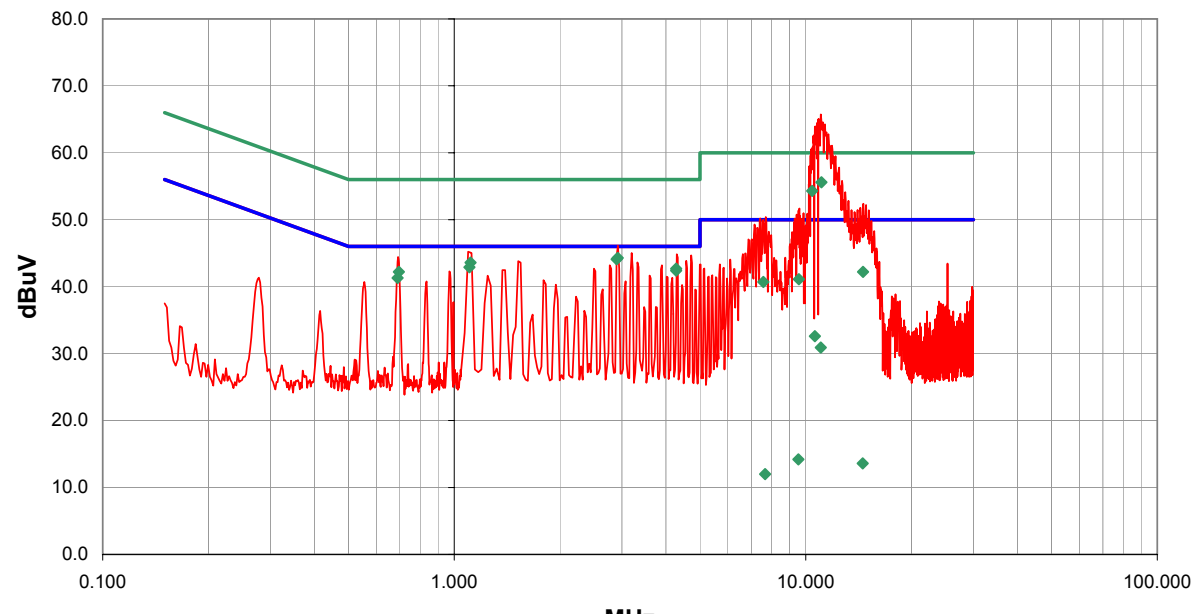
Test Description

Using the mode of operation and configuration noted within this report, conducted emissions tests were performed. The frequency range investigated (scanned), is also noted in this report. Conducted power line measurements are made, unless otherwise specified, over the frequency range from 150 kHz to 30 MHz to determine the line-to-ground radio-noise voltage that is conducted from the EUT power-input terminals that are directly (or indirectly via separate transformer or power supplies) connected to a public power network. Equipment is tested with power cords that are normally used or that have electrical or shielding characteristics that are the same as those cords normally used. Typically those measurements are made using a LISN (Line Impedance Stabilization Network), the 50 Ω measuring port is terminated by a 50 Ω EMI meter or a 50 Ω resistive load. All 50 Ω measuring ports of the LISN are terminated by 50 Ω .

Measurement Bandwidths			
Frequency Range (MHz)	Peak Data (kHz)	Quasi-Peak Data (kHz)	Average Data (kHz)
0.01 – 0.15	1.0	0.2	0.2
0.15 – 30.0	10.0	9.0	9.0
30.0 - 1000	100.0	120.0	120.0
Above 1000	1000.0	N/A	1000.0
<i>Measurements were made using the bandwidths and detectors specified. No video filter was used.</i>			

Completed by:

NORTHWEST EMC		CONDUCTED EMISSIONS DATA SHEET				REV dtd. 13 05/06/2004				
EUT: Zoom 2920		Work Order: GDMN0009								
Serial Number: 022394		Date: 07/15/04								
Customer: Guidant Corporation MN		Temperature: 75F								
Attendees: Holli Pheil		Humidity: 46%								
Cust. Ref. No.:		Barometric Pressure: 30								
Tested by: Jeremiah Darden		Power: 120VAC/60Hz		Job Site: OC10						
TEST SPECIFICATIONS										
Specification: FCC Part 15.207		Year: 2003								
Method: ANSI C63.4		Year: 2001								
SAMPLE CALCULATIONS										
Radiated Emissions: Field Strength = Measured Level + Antenna Factor + Cable Factor - Amplifier Gain + Distance Adjustment Factor + External Attenuation										
Conducted Emissions: Adjusted Level = Measured Level + Transducer Factor + Cable Attenuation Factor + External Attenuator										
COMMENTS										
System fully cabled and functional										
EUT OPERATING MODES										
Standard Operating Mode - Telemetry Wand Operating										
DEVIATIONS FROM TEST STANDARD										
No deviations.										
RESULTS										
Pass		Line L1		Run # 40						
Other										
		 Tested By:								
										
Freq (MHz)	Amplitude (dBuV)			Transducer (dB)	Cable (dB)	External Attenuation (dB)	Detector (blank equal peaks [PK] from scan)	Adjusted dBuV	Spec. Limit dBuV	Compared to Spec. (dB)
11.085	34.3			0.0	0.9	20.0	QP	55.2	60.0	-4.8
10.681	33.3			0.0	0.9	20.0	QP	54.2	60.0	-5.8
10.399	29.8			0.0	0.9	20.0	QP	50.7	60.0	-9.3
10.625	19.1			0.0	0.9	20.0	AV	40.0	50.0	-10.0
9.538	14.6			0.0	0.9	20.0	AV	35.5	50.0	-14.5
9.676	20.3			0.0	0.9	20.0	QP	41.2	60.0	-18.8
7.651	19.6			0.0	0.8	20.0	QP	40.4	60.0	-19.6
7.464	19.6			0.0	0.8	20.0	QP	40.4	60.0	-19.6
10.353	9.4			0.0	0.9	20.0	AV	30.3	50.0	-19.7
11.143	8.8			0.0	0.9	20.0	AV	29.7	50.0	-20.3
7.664	-8.2			0.0	0.8	20.0	AV	12.6	50.0	-37.4
7.384	-8.6			0.0	0.8	20.0	AV	12.2	50.0	-37.8

NORTHWEST EMC		CONDUCTED EMISSIONS DATA SHEET				REV d4.13 05/06/2004				
EUT: Zoom 2920		Work Order: GDMN0009								
Serial Number: 022394		Date: 07/15/04								
Customer: Guidant Corporation MN		Temperature: 75F								
Attendees: Holli Pheil		Humidity: 46%								
Cust. Ref. No.:		Barometric Pressure: 30								
Tested by: Jeremiah Darden		Power: 120VAC/60Hz		Job Site: OC10						
TEST SPECIFICATIONS										
Specification: FCC Part 15.207		Year: 2003								
Method: ANSI C63.4		Year: 2001								
SAMPLE CALCULATIONS										
Radiated Emissions: Field Strength = Measured Level + Antenna Factor + Cable Factor - Amplifier Gain + Distance Adjustment Factor + External Attenuation										
Conducted Emissions: Adjusted Level = Measured Level + Transducer Factor + Cable Attenuation Factor + External Attenuator										
COMMENTS										
System fully cabled and functional										
EUT OPERATING MODES										
Standard Operating Mode - Telemetry Wand Operating										
DEVIATIONS FROM TEST STANDARD										
No deviations.										
RESULTS		Line		Run #						
Pass		L2		41						
Other										
		 Tested By:								
										
Freq (MHz)	Amplitude (dBuV)			Transducer (dB)	Cable (dB)	External Attenuation (dB)	Detector (blank equal peaks [PK] from scan)	Adjusted dBuV	Spec. Limit dBuV	Compared to Spec. (dB)
2.898	23.6			0.0	0.5	20.0	AV	44.1	46.0	-1.9
1.104	22.6			0.0	0.3	20.0	AV	42.9	46.0	-3.1
4.278	21.8			0.0	0.6	20.0	AV	42.4	46.0	-3.6
11.085	34.7			0.0	0.9	20.0	QP	55.6	60.0	-4.4
0.690	21.3			0.0	0.0	20.0	AV	41.3	46.0	-4.7
10.423	33.4			0.0	0.9	20.0	QP	54.3	60.0	-5.7
2.918	23.8			0.0	0.5	20.0	QP	44.3	56.0	-11.7
1.113	23.3			0.0	0.3	20.0	QP	43.6	56.0	-12.4
4.280	22.1			0.0	0.6	20.0	QP	42.7	56.0	-13.3
0.696	22.2			0.0	0.0	20.0	QP	42.2	56.0	-13.8
10.611	11.7			0.0	0.9	20.0	AV	32.6	50.0	-17.4
14.548	21.1			0.0	1.1	20.0	QP	42.2	60.0	-17.8
9.557	20.2			0.0	0.9	20.0	QP	41.1	60.0	-18.9
11.035	10.0			0.0	0.9	20.0	AV	30.9	50.0	-19.1
7.574	19.9			0.0	0.8	20.0	QP	40.7	60.0	-19.3
9.534	-6.7			0.0	0.9	20.0	AV	14.2	50.0	-35.8
14.529	-7.5			0.0	1.1	20.0	AV	13.6	50.0	-36.4
7.663	-8.8			0.0	0.8	20.0	AV	12.0	50.0	-38.0



Justification

The individuals and/or the organization requesting the test provided the modes, configurations and settings available to evaluate. While scanning the radiated emissions, all of the EUT parameters listed below were investigated. This includes, but may not be limited to, antennas, tuned transmit frequency ranges, operating modes, and data rates.

Channels in Specified Band Investigated:

Single

Operating Modes Investigated:

Typical

Data Rates Investigated:

Maximum

Output Power Setting(s) Investigated:

Maximum

Power Input Settings Investigated:

120 VAC, 60 Hz.

Frequency Range Investigated

Start Frequency	10 kHz	Stop Frequency	30 MHz
------------------------	--------	-----------------------	--------

Software\Firmware Applied During Test

Exercise Software	Product 2909 System Software Quick Start	Version	Version 4.1 Version 1.38
Description			
The system was tested using standard operating production software to exercise the functions of the device during the testing.			

EUT and Peripherals

Description	Manufacturer	Model/Part Number	Serial Number
Programmer	Guidant	2920	022394
Pulse Generator	Guidant	Vitality AVT	106433
Pulse Generator	Guidant	Renewal TR	100088
Pulse Generator	Guidant	Insignia I Plus	104568
Loop Sensor	Guidant	6577	none

Field Strength of Fundamental and Spurious Radiated Emissions

Cables

Cable Type	Shield	Length (m)	Ferrite	Connection 1	Connection 2
AC Power	No	2.3	No	Programmer	AC Mains
Loop Sensor	PA	3.0	PA	Loop Sensor	Programmer
Vitality Patient Leads	PA	0.5	PA	Vitality AVT	Termination
Renewal Patient Leads	PA	0.5	PA	Renewal TR	Termination
Insignia Patient Leads	PA	0.1	PA	Insignia I Plus	Termination
PA = Cable is permanently attached to the device. Shielding and/or presence of ferrite may be unknown.					

Measurement Equipment

Description	Manufacturer	Model	Identifier	Last Cal	Interval
Quasi-Peak Adapter	Hewlett-Packard	85650A	AQD	02/10/2004	13 mo
Spectrum Analyzer	Hewlett-Packard	8568B	AAI	02/10/2004	13 mo
Antenna, Loop	EMCO	6502	AOA	01/08/2002	36 mo

Test Description


Requirement: No portion of the transmitted carrier, including sidebands and modulation products may lie within any of the restricted bands of 15.205. In addition, no spurious emission level may be higher than the level of the fundamental frequency. All emissions must meet the specification limits of 15.209. Emissions in the 9 kHz – 90 kHz and 110 – 490 kHz range are measured using an average detector for comparison to the limit. Peak emission limiting specified in 15.35 also applies for average measurements, with the limit for peak emissions 20 dB higher than the average limit.

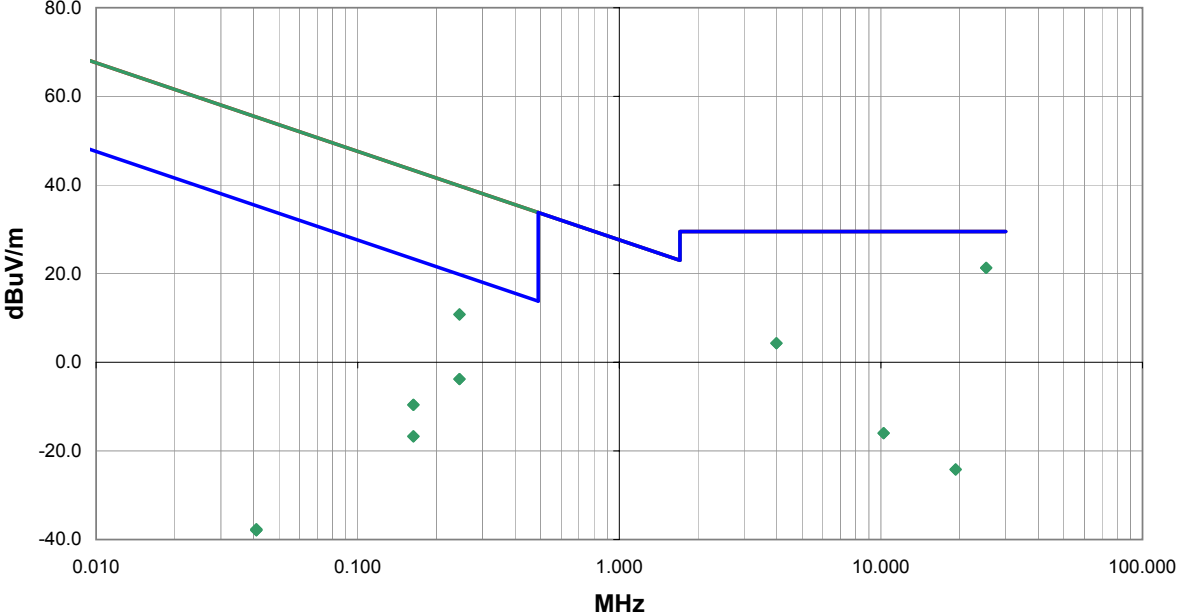
The level of any unwanted emissions from an intentional radiator operating under these general provisions shall not exceed the level of the fundamental emission. For intentional radiators which operate under the provisions of other sections within this part and which are required to reduce their unwanted emissions to the limits specified in this table, the limits in this table are based on the frequency of the unwanted emission and not the fundamental frequency. However, the level of any unwanted emissions shall not exceed the level of the fundamental frequency. Please note, the 3-meter average data demonstrates compliance with this requirement.

Configuration: The EUT was configured for typical operation, transmitting continuously with modulation at its single operating frequency. Emissions were maximized by rotating the turntable and varying the height of the measurement antenna. The position of the loop sensor, loop sensor cables, and pulse generators were also varied in three orthogonal axis (per ANSI C63.4: 2001) to maximize the level of emissions.

The emissions from the EUT were found compliant with all the requirements of FCC 15C.

Completed by:



NORTHWEST EMC										REV d14.13 05/06/2004			
RADIATED EMISSIONS DATA SHEET													
EUT: Zoom 2920					Work Order: GDMN0009								
Serial Number: 022394					Date: 07/28/04								
Customer: Guidant Corporation MN					Temperature: 73F								
Attendees: none					Humidity: 50%								
Cust. Ref. No.:					Barometric Pressure: 29.92								
Tested by: Jeremiah Darden					Power: 120VAC/60Hz					Job Site: OC08			
TEST SPECIFICATIONS													
Specification: FCC 15.209					Year: 2003								
Method: ANSI C63.4					Year: 2001								
SAMPLE CALCULATIONS													
Radiated Emissions: Field Strength = Measured Level + Antenna Factor + Cable Factor - Amplifier Gain + Distance Adjustment Factor + External Attenuation													
Conducted Emissions: Adjusted Level = Measured Level + Transducer Factor + Cable Attenuation Factor + External Attenuator													
COMMENTS													
System fully cabled and functional													
EUT OPERATING MODES													
Standard Operating Mode - Telemetry Wand Operating - 41 kHz Fundamental													
DEVIATIONS FROM TEST STANDARD													
No deviations.													
RESULTS										Run #			
Pass										5			
Other													
										 Tested By:			
													
Freq (MHz)	Amplitude (dBuV)	Factor (dB)	Azimuth (degrees)	Height (meters)	Distance (meters)	External Attenuation (dB)	Polarity	Detector	Distance Adjustment (dB)	Adjusted dBuV/m	Spec. Limit dBuV/m	Compared to Spec. (dB)	
25.255	21.6	8.7	320.0	1.8	3.0	0.0	Loop	QP	9.0	21.3	29.5	-8.2	
25.255	19.6	8.7	320.0	1.8	5.0	0.0	Loop	QP	7.0	21.3	29.5	-8.2	
0.245	35.7	10.3	180.0	1.8	3.0	0.0	Loop	AV	35.2	10.8	19.8	-9.0	
0.245	31.8	10.3	181.0	1.8	5.0	0.0	Loop	AV	31.3	10.8	19.8	-9.0	
3.988	16.5	10.3	360.0	1.8	3.0	0.0	Loop	QP	22.5	4.3	29.5	-25.2	
3.988	11.5	10.3	360.0	1.8	5.0	0.0	Loop	QP	17.5	4.3	29.5	-25.2	
0.163	36.1	10.4	184.0	1.8	5.0	0.0	Loop	AV	56.1	-9.6	23.3	-32.9	
0.163	43.1	10.4	183.0	1.8	3.0	0.0	Loop	AV	63.1	-9.6	23.4	-33.0	
0.245	40.4	10.3	181.0	1.8	5.0	0.0	Loop	PK	54.5	-3.8	39.8	-43.6	
0.245	47.2	10.3	180.0	1.8	3.0	0.0	Loop	PK	61.3	-3.8	39.8	-43.6	
10.236	19.6	10.4	0.0	1.8	3.0	0.0	Loop	QP	46.0	-16.0	29.5	-45.5	
10.236	9.4	10.4	360.0	1.8	5.0	0.0	Loop	QP	35.8	-16.0	29.5	-45.5	
19.304	19.5	9.9	-1.0	1.8	3.0	0.0	Loop	QP	53.6	-24.2	29.5	-53.7	
19.304	7.6	9.9	360.0	1.8	5.0	0.0	Loop	QP	41.7	-24.2	29.5	-53.7	
0.163	45.0	10.4	184.0	1.8	5.0	0.0	Loop	PK	72.1	-16.7	43.3	-60.0	
0.163	54.0	10.4	183.0	1.8	3.0	0.0	Loop	PK	81.1	-16.7	43.4	-60.1	
0.041	32.9	11.8	83.0	1.8	5.0	0.0	Loop	AV	82.6	-37.9	35.3	-73.2	
0.041	43.2	11.8	82.0	1.8	3.0	0.0	Loop	AV	92.9	-37.9	35.3	-73.2	
0.041	40.3	11.8	83.0	1.7	5.0	0.0	Loop	PK	89.8	-37.7	55.3	-93.0	
0.041	51.5	11.8	82.0	1.8	3.0	0.0	Loop	PK	101.0	-37.7	55.3	-93.0	

Distance Adjustment Factor for Radiated Emissions below 30 MHz

Method: Per 47 CFR 15.31(f)(2), the data was extrapolated based upon a the measured fall-off (at each frequency / polarity).

EUT: 2920

S/N: 30265

Date: 7/28/2004

Job Number: GDMN0003

[illegible]

