

NORTHWEST EMC

Boston Scientific Corporation

Model 3300

Listen Before Talk (LBT) per:

EN 301 839 V2.1.1:2016

FCC 95I:2016

RSS-243:2010

Korea Radio Law

Japan Specified low-power radio equipment Item 8 of Article 2-1

MICS Radio

Report # BSTN0663.22 Rev. 1



NVLAP Lab Code: 200881-0

This report must not be used to claim product certification, approval, or endorsement by NVLAP, NIST, or any agency of the federal government of the United States of America. This Report may only be duplicated in its entirety

CERTIFICATE OF TEST

Last Date of Test: August 25, 2016
Boston Scientific Corporation
Model: 3300

Radio Equipment Testing Standards

Specification	Method
EN 301 839 V2.1.1:2016	EN 301 839 V2.1.1:2016
FCC 951:2016	
RSS-243:2010	
Korean Radio Law	KN 301 839 V2.1.1:2016
Japan Specified low-power radio equipment Item 8 of Article 2-1	EN 301 839-1 V1.3.1:2009

Results (10 Channel)

Method Clause	Test Description	Applied	Results	Comments
5.3.7.1.3	LBT Threshold Power Level	Yes	Pass	
5.3.7.1.4	Monitoring System Bandwidth	Yes	Pass	
5.3.7.1.5	Monitoring System Scan Cycle Time	Yes	Pass	
5.3.7.1.5	Minimum Channel Monitoring Period	Yes	Pass	
5.3.7.1.6	Channel Access Based on Ambient Levels	Yes	Pass	
5.3.7.1.7	Discontinuation of a MICS Session	Yes	Pass	
5.3.7.1.8	Use of Pre-Scanned Alternative Channels	Yes	Pass	
5.3.8	Receiver Blocking	Yes	Pass	

Results (2 Channel)

Method Clause	Test Description	Applied	Results	Comments
5.3.7.1.3	LBT Threshold Power Level	Yes	Pass	
5.3.7.1.4	Monitoring System Bandwidth	Yes	Pass	
5.3.7.1.5	Monitoring System Scan Cycle Time	Yes	Pass	
5.3.7.1.5	Minimum Channel Monitoring Period	Yes	Pass	
5.3.7.1.6	Channel Access Based on Ambient Levels	Yes	Pass	
5.3.7.1.7	Discontinuation of a MICS Session	Yes	Pass	
5.3.7.1.8	Use of Pre-Scanned Alternative Channels	Yes	N/A	Not required. The EUT does not use Pre-Scanned Alternate Channels.
5.3.8	Receiver Blocking	Yes	Pass	

Deviations from Test Standards

None

Approved By:



Dean Ghizzone, General Manager

Product compliance is the responsibility of the client; therefore, the tests and equipment modes of operation represented in this report were agreed upon by the client, prior to testing. The results of this test pertain only to the sample(s) tested. The specific description is noted in each of the individual sections of the test report supporting this certificate of test. This report reflects only those tests from the referenced standards shown in the certificate of test. It does not include inspection or verification of labels, identification, marking or user information.

REVISION HISTORY

Revision Number	Description	Date	Page Number
00	None		
01	Corrected the EN 301 839 Specification on the data sheets	4/26/2017	15, 21, 27, 33, 39, 48, 57, 65, 73, 78, 83, 88, 93, 98

ACCREDITATIONS AND AUTHORIZATIONS

United States

FCC - Designated by the FCC as a Telecommunications Certification Body (TCB). Certification chambers, Open Area Test Sites, and conducted measurement facilities are listed with the FCC.

A2LA - Accredited by A2LA to ISO / IEC 17065 as a product certifier. This allows Northwest EMC to certify transmitters to FCC and IC specifications.

NVLAP - Each laboratory is accredited by NVLAP to ISO 17025

Canada

ISED - Recognized by Innovation, Science and Economic Development Canada as a Certification Body (CB). Certification chambers and Open Area Test Sites are filed with ISED.

European Union

European Commission – Validated by the European Commission as a Notified Body under the R&TTE Directive.

Australia/New Zealand

ACMA - Recognized by ACMA as a CAB for the acceptance of test data.

Korea

MSIP / RRA - Recognized by KCC's RRA as a CAB for the acceptance of test data.

Japan

VCCI - Associate Member of the VCCI. Conducted and radiated measurement facilities are registered.

Taiwan

BSMI – Recognized by BSMI as a CAB for the acceptance of test data.

NCC - Recognized by NCC as a CAB for the acceptance of test data.

Singapore

IDA – Recognized by IDA as a CAB for the acceptance of test data.

Israel

MOC – Recognized by MOC as a CAB for the acceptance of test data.

Hong Kong

OFCA – Recognized by OFCA as a CAB for the acceptance of test data.

Vietnam

MIC – Recognized by MIC as a CAB for the acceptance of test data.

SCOPE

For details on the Scopes of our Accreditations, please visit:

<http://www.nwemc.com/accreditations/>
<http://gsi.nist.gov/global/docs/cabs/designations.html>

MEASUREMENT UNCERTAINTY

Measurement Uncertainty

When a measurement is made, the result will be different from the true or theoretically correct value. The difference is the result of tolerances in the measurement system that cannot be completely eliminated. To the extent that technology allows us, it has been our aim to minimize this error. Measurement uncertainty is a statistical expression of measurement error qualified by a probability distribution.

A measurement uncertainty estimation has been performed for each test per our internal quality document WP 342. The estimation is used to compare the measured result with its "true" or theoretically correct value. The expanded measurement uncertainty (K=2) for each test is on each data sheet. Our measurement data meets or exceeds the measurement uncertainty requirements of the applicable specification; therefore, the test data can be compared directly to the specification limit to determine compliance. The calculations for estimating measurement uncertainty are based upon ETSI TR 100 028 (or CISPR 16-4-2 as applicable), and are available upon request.



The following table represents the Measurement Uncertainty (MU) budgets for each of the tests that may be contained in this report.

Test	+ MU	- MU
Frequency Accuracy (Hz)	0.0007%	-0.0007%
Amplitude Accuracy (dB)	1.2 dB	-1.2 dB
Conducted Power (dB)	0.3 dB	-0.3 dB
Radiated Power via Substitution (dB)	0.7 dB	-0.7 dB
Temperature (degrees C)	0.7°C	-0.7°C
Humidity (% RH)	2.5% RH	-2.5% RH
Voltage (AC)	1.0%	-1.0%
Voltage (DC)	0.7%	-0.7%
Field Strength (dB)	5.2 dB	-5.2 dB
AC Powerline Conducted Emissions (dB)	2.4 dB	-2.4 dB

FACILITIES



California Labs OC01-13 41 Tesla Irvine, CA 92618 (949) 861-8918	Minnesota Labs MN01-08, MN10 9349 W Broadway Ave. Brooklyn Park, MN 55445 (612)-638-5136	New York Labs NY01-04 4939 Jordan Rd. Elbridge, NY 13060 (315) 554-8214	Oregon Labs EV01-12 22975 NW Evergreen Pkwy Hillsboro, OR 97124 (503) 844-4066	Texas Labs TX01-09 3801 E Plano Pkwy Plano, TX 75074 (469) 304-5255	Washington Labs NC01-05 19201 120 th Ave NE Bothell, WA 98011 (425)984-6600
NVLAP					
NVLAP Lab Code: 200676-0	NVLAP Lab Code: 200881-0	NVLAP Lab Code: 200761-0	NVLAP Lab Code: 200630-0	NVLAP Lab Code:201049-0	NVLAP Lab Code: 200629-0
Innovation, Science and Economic Development Canada					
2834B-1, 2834B-3	2834E-1	N/A	2834D-1, 2834D-2	2834G-1	2834F-1
BSMI					
SL2-IN-E-1154R	SL2-IN-E-1152R	N/A	SL2-IN-E-1017	SL2-IN-E-1158R	SL2-IN-E-1153R
VCCI					
A-0029	A-0109	N/A	A-0108	A-0201	A-0110
Recognized Phase I CAB for ACMA, BSMI, IDA, KCC/RRR, MIC, MOC, NCC, OFCA					
US0158	US0175	N/A	US0017	US0191	US0157

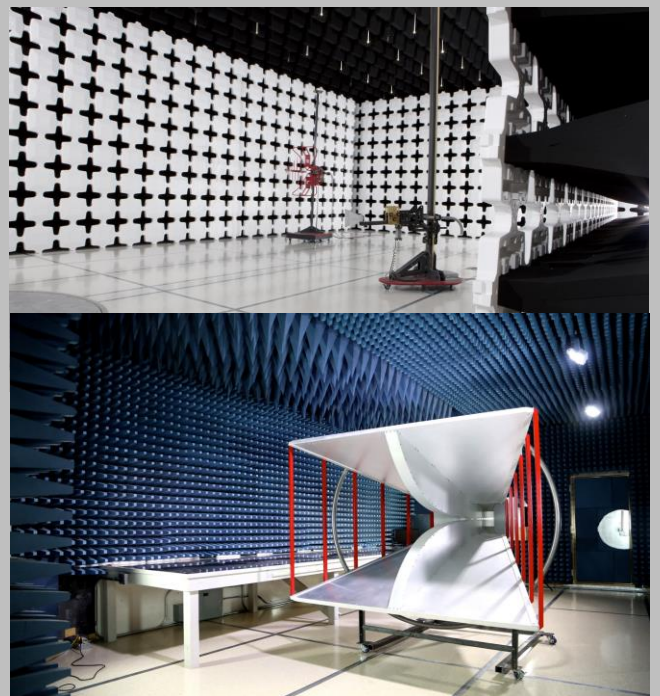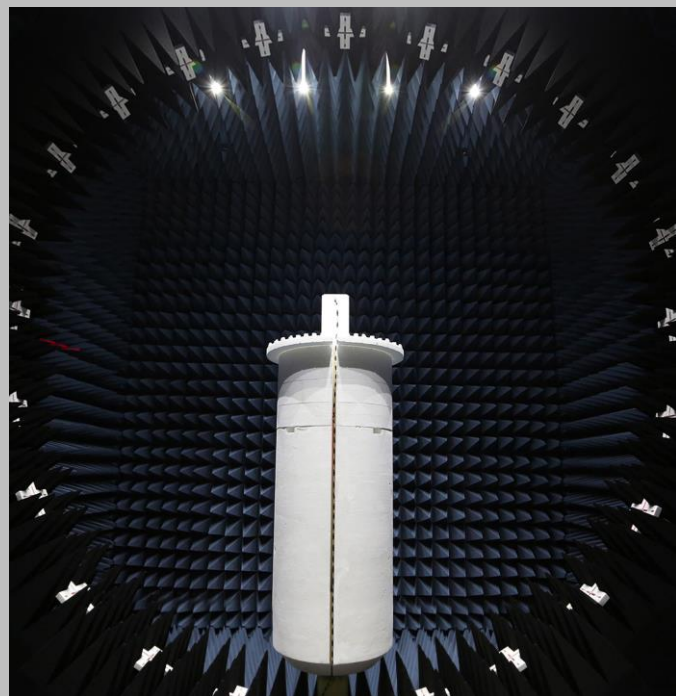

PRODUCT DESCRIPTION

Client and Equipment Under Test (EUT) Information

Company Name:	Boston Scientific Corporation
Address:	4100 Hamline Avenue North
City, State, Zip:	St. Paul, MN 55112-5798
Test Requested By:	Pete Musto
Model:	Model 3300
First Date of Test:	August 8, 2016
Last Date of Test:	August 25, 2016
Receipt Date of Samples:	July 14, 2016
Equipment Design Stage:	Production
Equipment Condition:	No Damage

Information Provided by the Party Requesting the Test

Functional Description of the EUT:

The Boston Scientific Model 3300 Latitude Programmer (PRM) is a device that is used to interrogate and program Boston Scientific PGs and defibrillators. PG specific software applications are loaded into the PRM and communicate with the implanted device. The telemetry communications allow the physician the ability to program the PG or query the PG for historical data or operating parameters. The PRM allows other external instruments or equipment to be connected, including printers, network connections, external display monitors, USB data storage devices, and cellular adapters. The PRM also provides a Pacing Systems Analyzer for implant lead evaluation and diagnostics.

Testing Objective:

To demonstrate compliance of the MICS radio to Article 3.2 of the R&TTE Directive, FCC Authorization to FCC 95I, CB authorization to RSS-243, authorization to Korean Radio Law and Japan Specified low-power radio equipment Item 8 of Article 2-1.

CONFIGURATIONS

Configuration BSTN0663- 7

Software/Firmware Running during test	
Description	Version
PRM Application - 3869	0.03.13

EUT			
Description	Manufacturer	Model/Part Number	Serial Number
Latitude Vision Programmer	Boston Scientific Corporation	3300	058

Peripherals in test setup boundary			
Description	Manufacturer	Model/Part Number	Serial Number
AC/DC Adapter	GlobTek, Inc	GTM41133-9016-1.0-T3A	None
USB Memory Feature Key	Boston Scientific Corporation	None	043
USB Memory MTI	Kingston	DTSE9 G2	None
Keyboard	Lenovo	KU-0989	1S54Y94890909725E
Implant	Boston Scientific Corporation	Ingenio 2 U226-100-0	299107

Cables					
Cable Type	Shield	Length (m)	Ferrite	Connection 1	Connection 2
AC Cable	Yes	2.5m	No	AC/DC Adapter	AC Mains
DC Cable	No	2m	Yes	AC/DC Adapter	Programmer
USB Cable (Keyboard)	Yes	1.8m	No	Keyboard	Programmer

CONFIGURATIONS

Configuration BSTN0663- 8

Software/Firmware Running during test	
Description	Version
MTI	2.0-7

EUT			
Description	Manufacturer	Model/Part Number	Serial Number
Latitude Vision Programmer	Boston Scientific Corporation	3300	058

Peripherals in test setup boundary			
Description	Manufacturer	Model/Part Number	Serial Number
AC/DC Adapter	GlobTek, Inc	GTM41133-9016-1.0-T3A	None
USB Memory Feature Key	Boston Scientific Corporation	None	043
USB Memory MTI	Kingston	DTSE9 G2	None
Keyboard	Lenovo	KU-0989	1S54Y94890909725E
Implant	Boston Scientific Corporation	Ingenio 2 U226-100-0	299107

Cables					
Cable Type	Shield	Length (m)	Ferrite	Connection 1	Connection 2
AC Cable	Yes	2.5m	No	AC/DC Adapter	AC Mains
DC Cable	No	2m	Yes	AC/DC Adapter	Programmer
USB Cable (Keyboard)	Yes	1.8m	No	Keyboard	Programmer

CONFIGURATIONS

Configuration BSTN0663- 10

Software/Firmware Running during test	
Description	Version
MTI	2.0-7

EUT			
Description	Manufacturer	Model/Part Number	Serial Number
Latitude Vision Programmer	Boston Scientific Corporation	3300	058

Peripherals in test setup boundary			
Description	Manufacturer	Model/Part Number	Serial Number
AC/DC Adapter	GlobTek, Inc	GTM41133-9016-1.0-T3A	None
USB Memory Feature Key	Boston Scientific Corporation	None	043
USB Memory MTI	Kingston	DTSE9 G2	None
Keyboard	Lenovo	KU-0989	1S54Y94890909725E
Implant	Boston Scientific Corporation	Emblem A209	100588

Cables					
Cable Type	Shield	Length (m)	Ferrite	Connection 1	Connection 2
AC Cable	Yes	2.5m	No	AC/DC Adapter	AC Mains
DC Cable	No	2m	Yes	AC/DC Adapter	Programmer
USB Cable (Keyboard)	Yes	1.8m	No	Keyboard	Programmer

CONFIGURATIONS

Configuration BSTN0663- 11

Software/Firmware Running during test	
Description	Version
PRM Application - 3869	0.04.02

EUT			
Description	Manufacturer	Model/Part Number	Serial Number
Latitude Vision Programmer	Boston Scientific Corporation	3300	058

Peripherals in test setup boundary			
Description	Manufacturer	Model/Part Number	Serial Number
AC/DC Adapter	GlobTek, Inc	GTM41133-9016-1.0-T3A	None
USB Memory Feature Key	Boston Scientific Corporation	None	043
USB Memory MTI	Kingston	DTSE9 G2	None
Keyboard	Lenovo	KU-0989	1S54Y94890909725E
Implant	Boston Scientific Corporation	Ingenio 2 U226-100-0	299107

Cables					
Cable Type	Shield	Length (m)	Ferrite	Connection 1	Connection 2
AC Cable	Yes	2.5m	No	AC/DC Adapter	AC Mains
DC Cable	No	2m	Yes	AC/DC Adapter	Programmer
USB Cable (Keyboard)	Yes	1.8m	No	Keyboard	Programmer

CONFIGURATIONS

Configuration BSTN0663- 12

Software/Firmware Running during test	
Description	Version
MTI	2.0-11

EUT			
Description	Manufacturer	Model/Part Number	Serial Number
Latitude Vision Programmer	Boston Scientific Corporation	3300	058

Peripherals in test setup boundary			
Description	Manufacturer	Model/Part Number	Serial Number
AC/DC Adapter	GlobTek, Inc	GTM41133-9016-1.0-T3A	None
USB Memory Feature Key	Boston Scientific Corporation	None	043
USB Memory MTI	Kingston	DTSE9 G2	None
Keyboard	Lenovo	KU-0989	1S54Y94890909725E
Implant	Boston Scientific Corporation	Emblem A209	100588

Cables					
Cable Type	Shield	Length (m)	Ferrite	Connection 1	Connection 2
AC Cable	Yes	2.5m	No	AC/DC Adapter	AC Mains
DC Cable	No	2m	Yes	AC/DC Adapter	Programmer
USB Cable (Keyboard)	Yes	1.8m	No	Keyboard	Programmer

MODIFICATIONS

Equipment Modifications

Item	Date	Test	Modification	Note	Disposition of EUT
1	8/8/2016	Use of a Pre-Scanned Alternative Channel	Tested as delivered to Test Station.	No EMI suppression devices were added or modified during this test.	EUT remained at Northwest EMC following the test.
2	8/16/2016	LBT Threshold Power Level	Tested as delivered to Test Station.	No EMI suppression devices were added or modified during this test.	EUT remained at Northwest EMC following the test.
3	8/16/2016	Monitoring System Bandwidth	Tested as delivered to Test Station.	No EMI suppression devices were added or modified during this test.	EUT remained at Northwest EMC following the test.
4	8/16/2016	Monitoring System Scan Cycle Time	Tested as delivered to Test Station.	No EMI suppression devices were added or modified during this test.	EUT remained at Northwest EMC following the test.
5	8/16/2016	Channel Access Based on Ambient Levels	Tested as delivered to Test Station.	No EMI suppression devices were added or modified during this test.	EUT remained at Northwest EMC following the test.
6	8/16/2016	Discontinuation of a MICS Session	Tested as delivered to Test Station.	No EMI suppression devices were added or modified during this test.	EUT remained at Northwest EMC following the test.
7	8/16/2016	Receiver Blocking	Tested as delivered to Test Station.	No EMI suppression devices were added or modified during this test.	EUT remained at Northwest EMC following the test.
8	8/25/2016	Minimum Channel Monitoring Period	Tested as delivered to Test Station.	No EMI suppression devices were added or modified during this test.	Scheduled testing was completed.

LBT THRESHOLD POWER LEVEL, 10 CHANNEL

Testing was performed using the mode(s) of operation and configuration(s) noted within the report. The individuals and/or the organization requesting the test provided the modes, configurations and settings used to complete the evaluation. The actual test parameters are specified in the test data, this includes items such as investigated frequency range (scanned) and test levels. The testing methods and performance specifications, as well as the test site used for the evaluation are indicated in the test data.

TEST EQUIPMENT

Description	Manufacturer	Model	ID	Last Cal.	Cal. Due
Probe - Near Field Set	ETS Lindgren	7405	IPO	NCR	NCR
Directional Coupler	Fairview Microwave	SMC4039-10	RGS	NCR	NCR
Power Divider/Combiner	Fairview Microwave Inc (SM electronics)	MP8451-2	IAD	NCR	NCR
Power Divider/Combiner	Fairview Microwave Inc (SM electronics)	MP8451-2	IAC	NCR	NCR
Generator - Signal	Agilent	N5182A	TIF	8/12/2014	8/12/2017
Generator - Signal	Agilent	E4422B	TGQ	3/17/2015	3/17/2018
Cable	ESM Cable Corp.	TTBJ141 KMKM-72	MNU	9/18/2015	9/18/2016
Block - DC	Fairview Microwave	SD3379	AMI	9/18/2015	9/18/2016
Analyzer - Spectrum Analyzer	Agilent	E4440A	AAX	3/24/2016	3/24/2017


TEST DESCRIPTION

A near-field probe was placed near the transmitter. A low-loss coaxial cable was used to connect the near-field probe to the spectrum analyzer. The EUT was configured according to the following block diagram:


The signal generator was set to multitone operation to cause equal interference across the entire band. The amplitude of the multitone signals (out of operation region) were set to the LBT threshold of $10 \cdot \log(\text{Bandwidth}) - 150 + \text{Antenna Gain} + 3 \text{ dB}$.

The spectrum analyzer was set to measure the transmit band of 402-405 MHz. The multitone signal of the intended frequency (F_c) was set to the LBT threshold - 6 dB, and raised by 1 dB increments until the EUT choose a different channel to start a session. Screen captures were provided to show the EUT behavior at the different LBT threshold levels.

The signal generator amplitude at F_c was then measured and recorded with the spectrum analyzer.

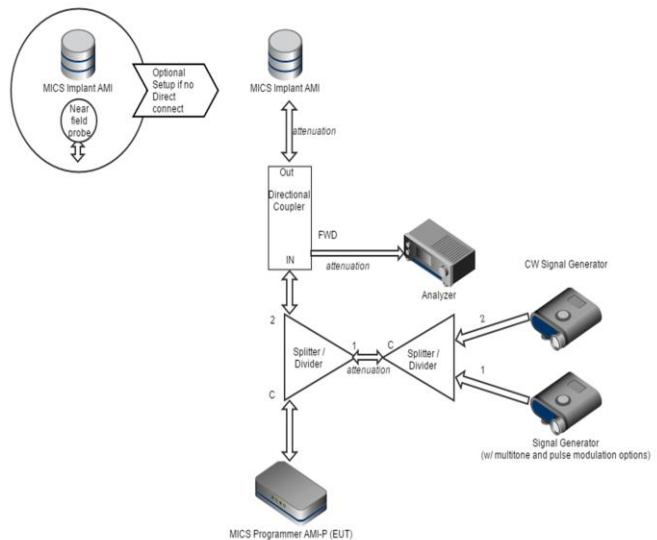


LBT THRESHOLD POWER LEVEL, 10 CHANNEL


EUT: Model 3300		Work Order: BSTN0663	
Serial Number: 058		Date: 08/08/16	
Customer: Boston Scientific Corporation		Temperature: 23.2 °C	
Attendees: Pete Musto		Humidity: 53.6% RH	
Project: Laramie Vision		Barometric Pres.: 1019 mbar	
Tested by: Dustin Sparks	Power: 220VAC/60Hz	Job Site: MN02	
TEST SPECIFICATIONS		Test Method	
EN 301 839 V2.1.1:2016		EN 301 839 V2.1.1:2016	
COMMENTS			
EUT emissions bandwidth is 300000 Hz, 2.7 dBi antenna gain. Antenna port B, PRM Application 3869 v. 0.03.13			
DEVIATIONS FROM TEST STANDARD			
None			
Configuration #	7	Signature 	
		Value (dBm)	Limit (dBm)
LBT Threshold - 6dB		N/A	N/A
LBT Threshold + 2dB		N/A	N/A
LBT Threshold + 3dB		-93.5	<= 92.5
			Result
			N/A
			N/A
			Pass

LBT THRESHOLD POWER LEVEL, 10 CHANNEL

LBT Threshold - 6dB						
				Value (dBm)	Limit (dBm)	Result
				N/A	N/A	N/A

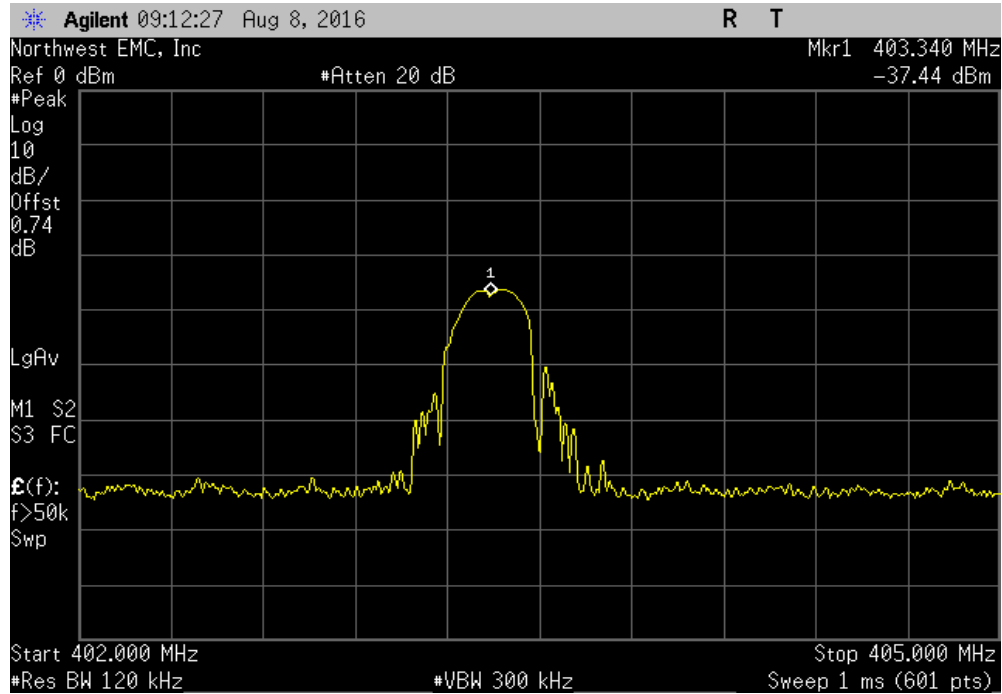


LBT Threshold + 2dB						
				Value (dBm)	Limit (dBm)	Result
				N/A	N/A	N/A

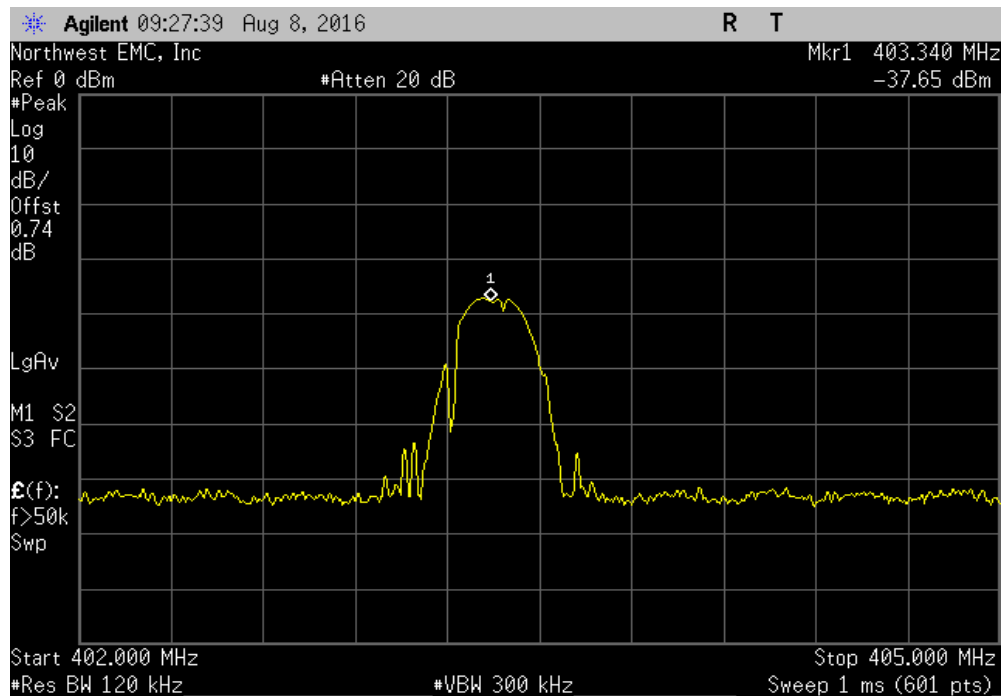


LBT THRESHOLD POWER LEVEL, 10 CHANNEL



LBT Threshold + 3dB						
				Value (dBm)	Limit (dBm)	Result
				-93.5	<= 92.5	Pass

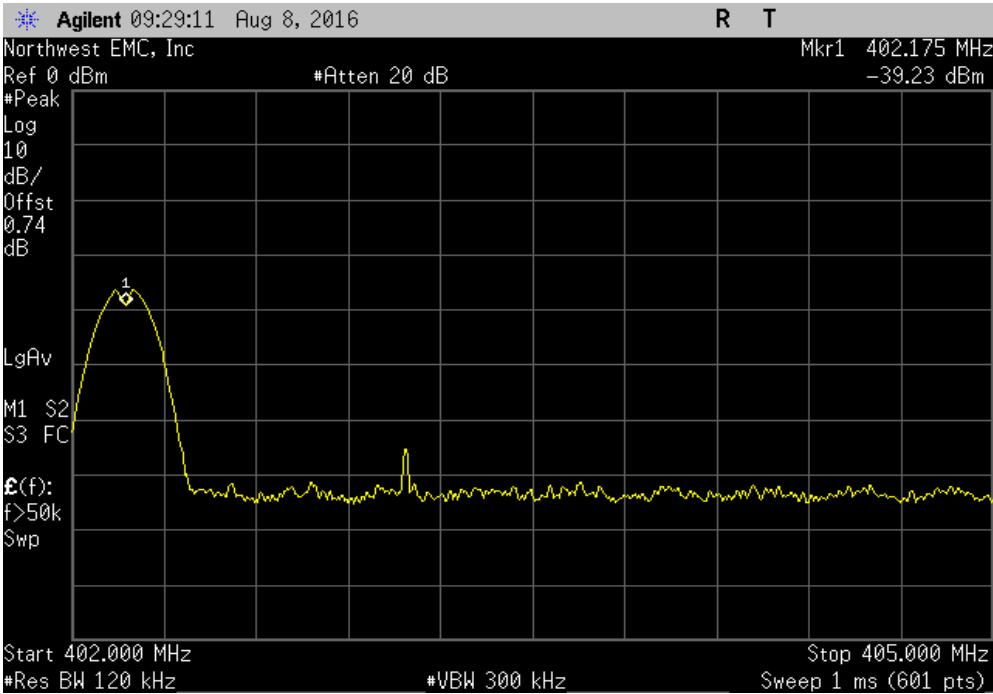

LBT THRESHOLD POWER LEVEL, 10 CHANNEL

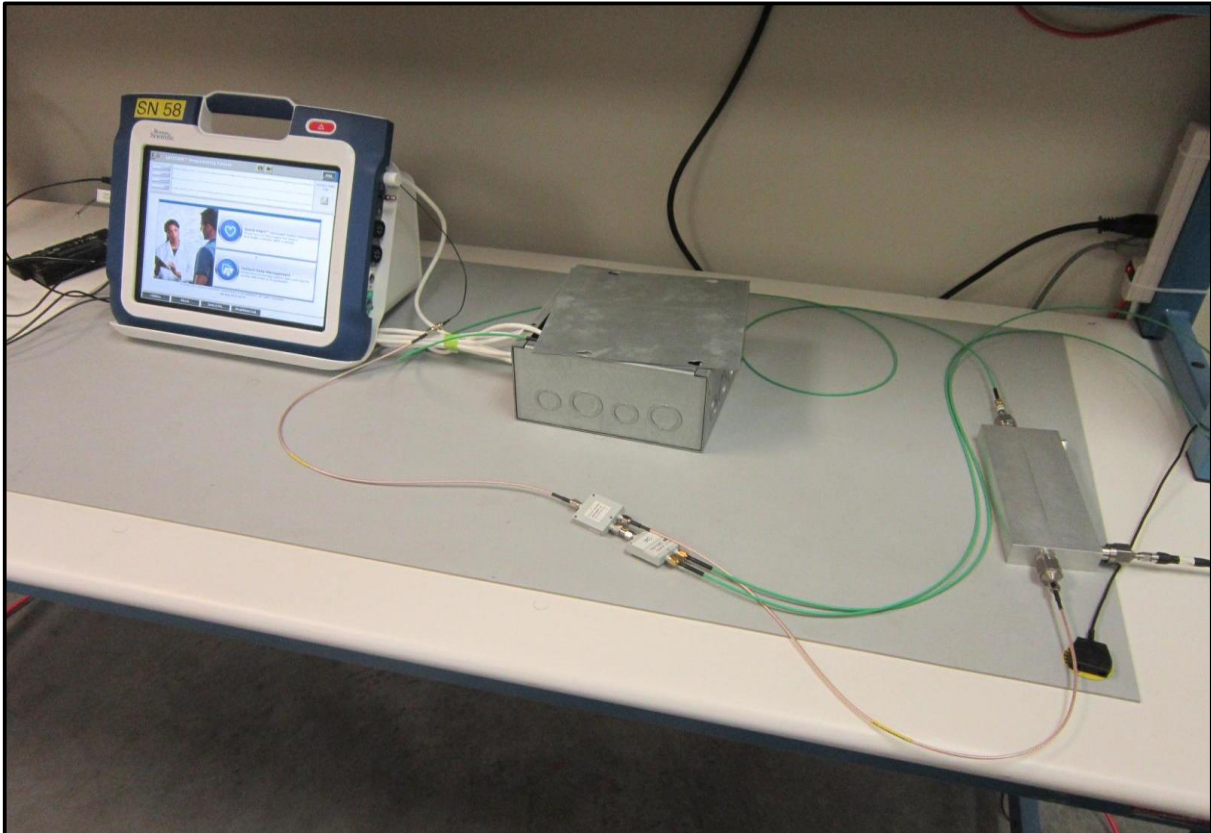

LBT THRESHOLD POWER LEVEL, 10 CHANNEL

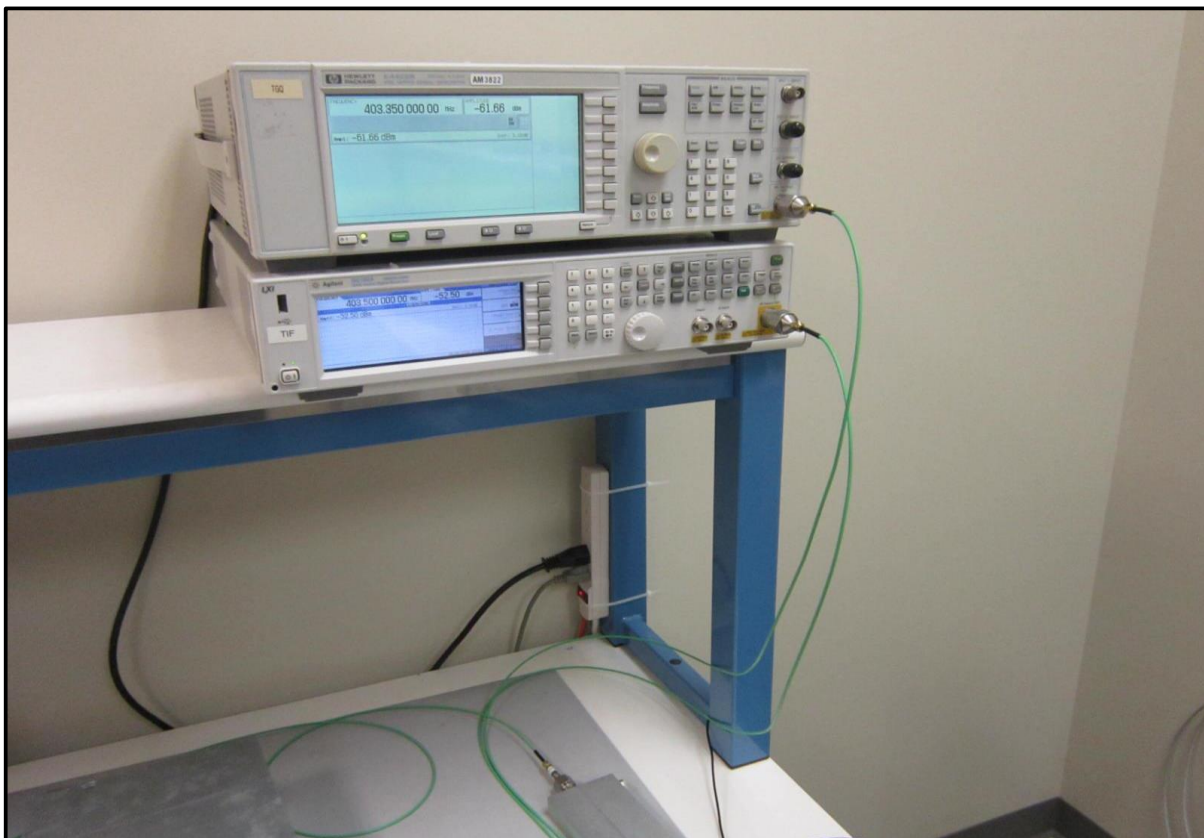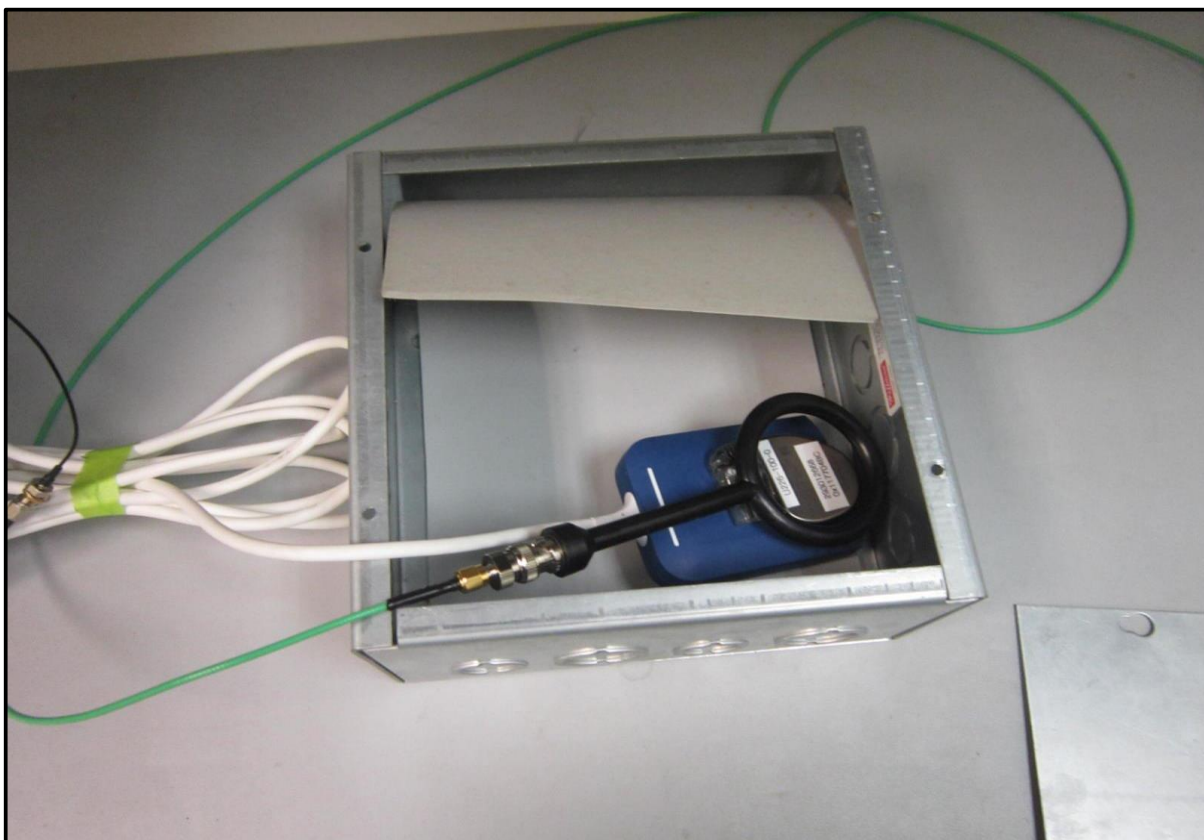

LBT THRESHOLD POWER LEVEL, 2 CHANNEL

Testing was performed using the mode(s) of operation and configuration(s) noted within the report. The individuals and/or the organization requesting the test provided the modes, configurations and settings used to complete the evaluation. The actual test parameters are specified in the test data, this includes items such as investigated frequency range (scanned) and test levels. The testing methods and performance specifications, as well as the test site used for the evaluation are indicated in the test data.

TEST EQUIPMENT

Description	Manufacturer	Model	ID	Last Cal.	Cal. Due
Probe - Near Field Set	ETS Lindgren	7405	IPO	NCR	NCR
Power Divider/Combiner	Fairview Microwave Inc (SM electronics)	MP8451-2	IAD	NCR	NCR
Power Divider/Combiner	Fairview Microwave Inc (SM electronics)	MP8451-2	IAC	NCR	NCR
Directional Coupler	Fairview Microwave	SMC4039-10	RGS	NCR	NCR
Generator - Signal	Agilent	N5182A	TIF	8/12/2014	8/12/2017
Generator - Signal	Agilent	N5183A	TIK	10/17/2014	10/17/2017
Cable	ESM Cable Corp.	TTBJ141 KMKM-72	MNU	9/18/2015	9/18/2016
Attenuator	S.M. Electronics	SA26B-20	RFW	2/26/2016	2/26/2017
Block - DC	Fairview Microwave	SD3379	AMI	9/18/2015	9/18/2016
Analyzer - Spectrum Analyzer	Agilent	E4440A	AAX	3/24/2016	3/24/2017


TEST DESCRIPTION

The measurement was made using a direct connection between the RF output of the EUT and a spectrum analyzer. The EUT was configured according to the following block diagram:


The signal generator was set to multitone operation to cause equal interference across the entire band. The amplitude of the multitone signals (out of operation region) were set to the LBT threshold of $10 \cdot \log(\text{Bandwidth}) - 150 + \text{Antenna Gain} + 3 \text{ dB}$.

The spectrum analyzer was set to measure the transmit band of 402-405 MHz. The multitone signal of the intended frequency (F_c) was set to the LBT threshold - 6 dB, and raised by 1 dB increments until the EUT choose a different channel to start a session. Screen captures were provided to show the EUT behavior at the different LBT threshold levels.

The signal generator amplitude at F_c was then measured and recorded with the spectrum analyzer.

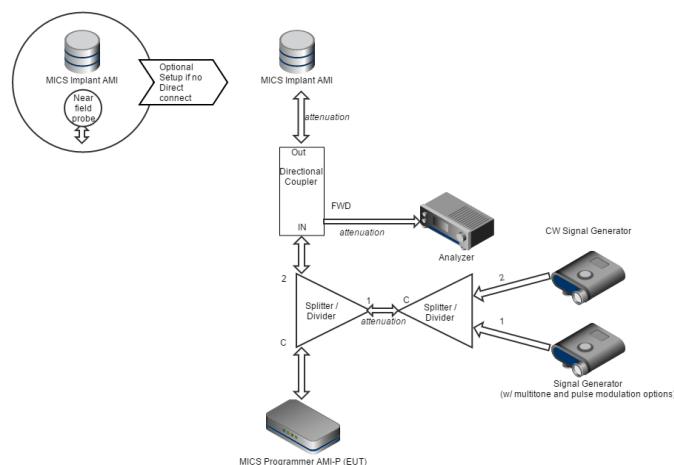


LBT THRESHOLD POWER LEVEL, 2 CHANNEL


EUT: Model 3300		Work Order: BSTN0663	
Serial Number: 058		Date: 08/16/16	
Customer: Boston Scientific Corporation		Temperature: 23.6 °C	
Attendees: Pete Musto		Humidity: 59.1% RH	
Project: Laramie Vision		Barometric Pres.: 1019 mbar	
Tested by: Dustin Sparks	Power: 110VAC/60Hz	Job Site: MN08	
TEST SPECIFICATIONS		Test Method	
EN 301 839 V2.1.1:2016		EN 301 839 V2.1.1:2016	
COMMENTS			
EUT bandwidth is 300000 Hz with an antenna gain of -5 dBi.			
DEVIATIONS FROM TEST STANDARD			
None			
Configuration #	10	Signature 	
		Value (dBm)	Limit (dBm)
LBT Threshold -6dB		N/A	N/A
LBT Threshold +2dB		N/A	N/A
LBT Threshold +3dB		-101.2	<= -100.2
			Result
			N/A
			N/A
			Pass

LBT THRESHOLD POWER LEVEL, 2 CHANNEL

LBT Threshold -6dB						
				Value (dBm)	Limit (dBm)	Result
				N/A	N/A	N/A

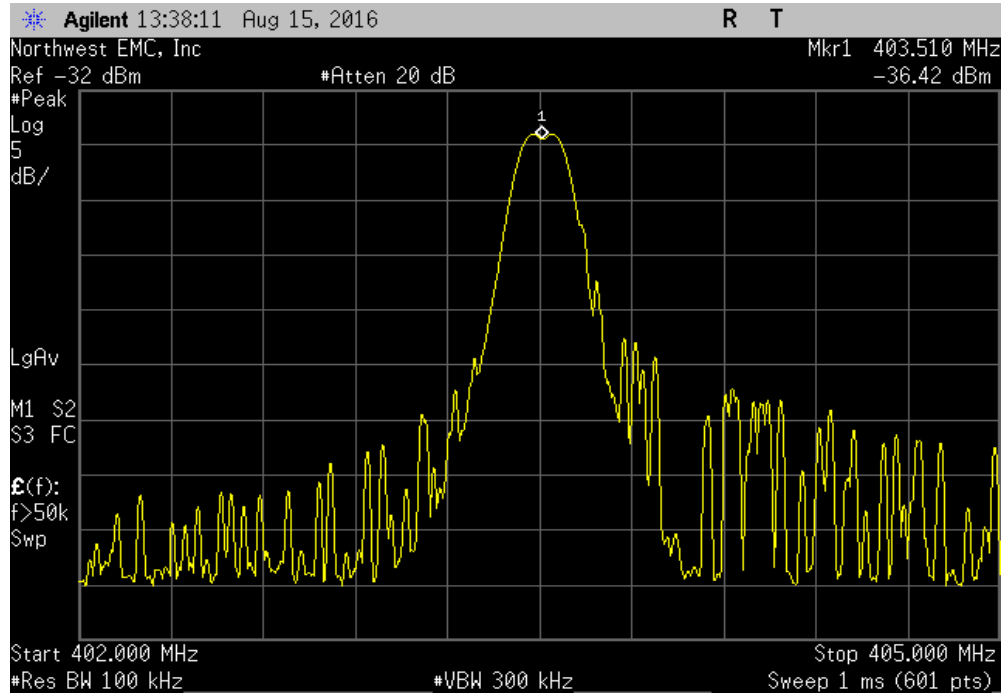


LBT Threshold +2dB						
				Value (dBm)	Limit (dBm)	Result
				N/A	N/A	N/A

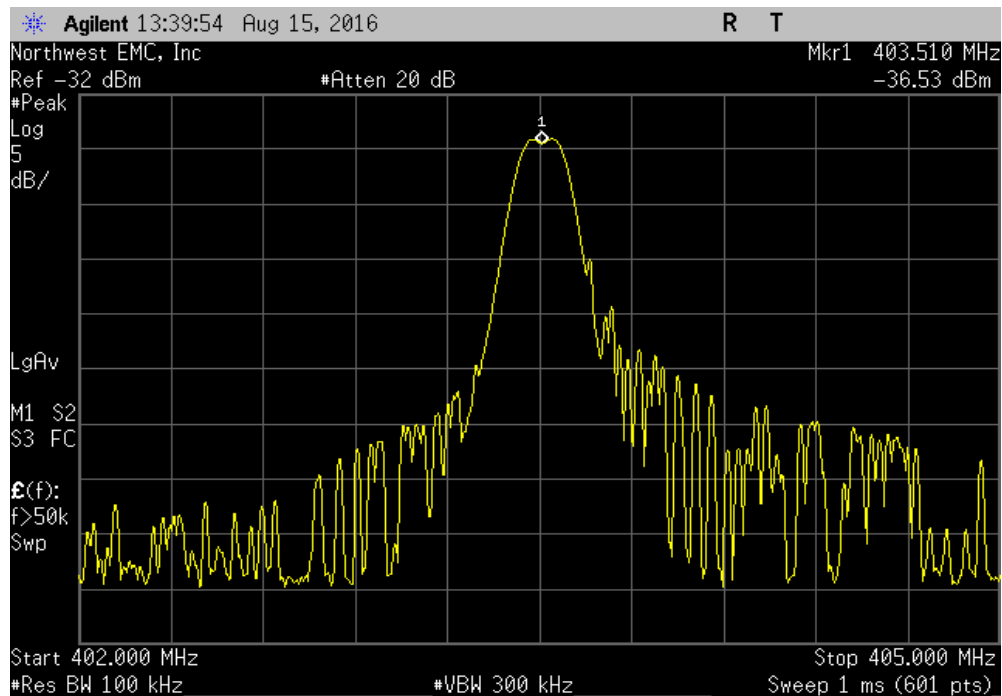


LBT THRESHOLD POWER LEVEL, 2 CHANNEL

LBT Threshold +3dB						
				Value (dBm)	Limit (dBm)	Result
				-101.2	<= -100.2	Pass

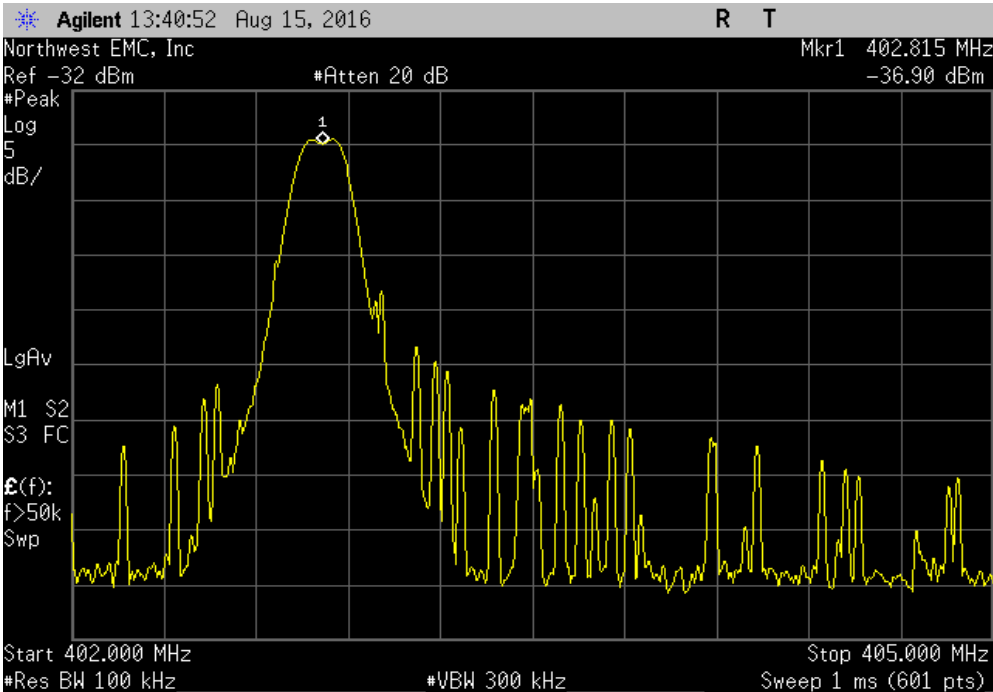

LBT THRESHOLD POWER LEVEL, 2 CHANNEL

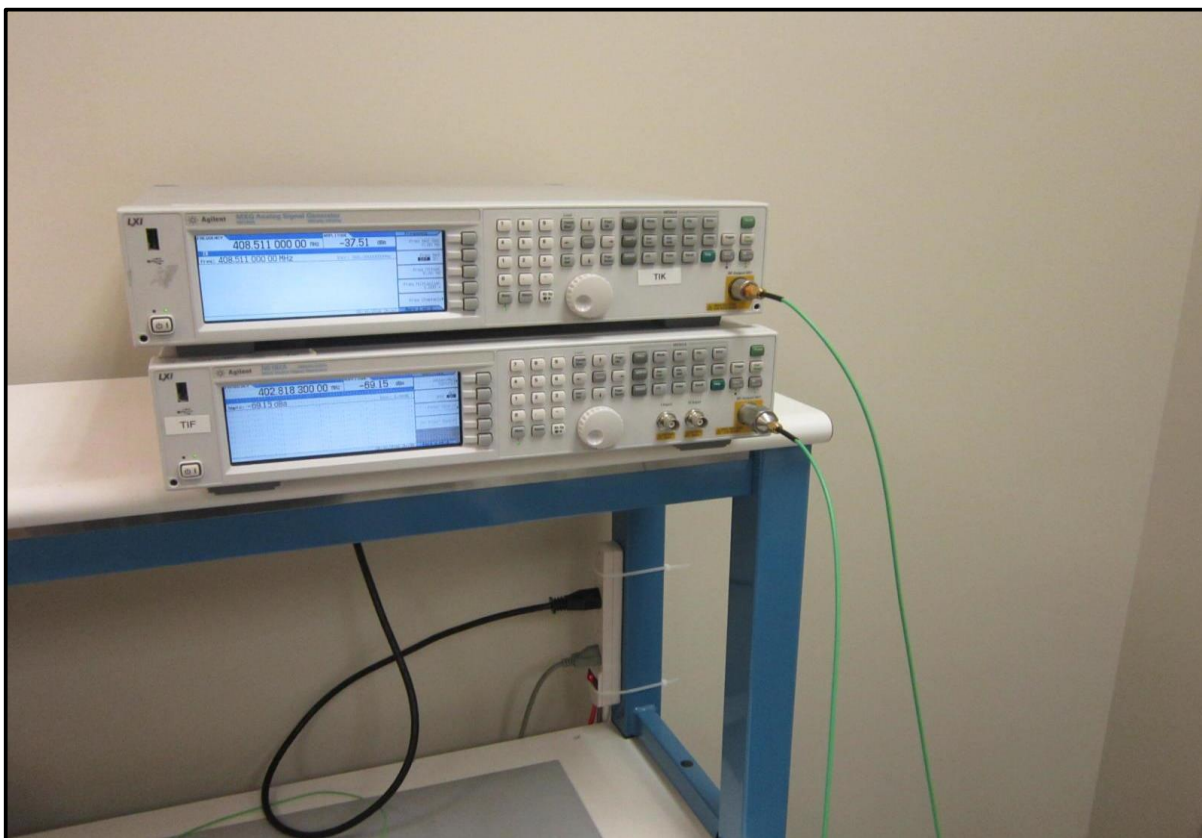

LBT THRESHOLD POWER LEVEL, 2 CHANNEL



NORTHWEST EMC

Testing was performed using the mode(s) of operation and configuration(s) noted within the report. The individuals and/or the organization requesting the test provided the modes, configurations and settings used to complete the evaluation. The actual test parameters are specified in the test data, this includes items such as investigated frequency range (scanned) and test levels. The testing methods and performance specifications, as well as the test site used for the evaluation are indicated in the test data.

TEST EQUIPMENT

TEST EQUIPMENT					
Description	Manufacturer	Model	ID	Last Cal.	Cal. Due
Probe - Near Field Set	ETS Lindgren	7405	IPO	NCR	NCR
Directional Coupler	Fairview Microwave	SMC4039-10	RGS	NCR	NCR
Power Divider/Combiner	Fairview Microwave Inc (SM electronics)	MP8451-2	IAD	NCR	NCR
Power Divider/Combiner	Fairview Microwave Inc (SM electronics)	MP8451-2	IAC	NCR	NCR
ESD Gun	Teseq	NSG 437	IGQ	6/3/2016	12/3/2016
Cable	ESM Cable Corp.	TTBJ141 KMKM-72	MNU	9/18/2015	9/18/2016
Block - DC	Fairview Microwave	SD3379	AMI	9/18/2015	9/18/2016
Analyzer - Spectrum Analyzer	Agilent	E4440A	AAX	3/24/2016	3/24/2017

TEST DESCRIPTION


A near-field probe was placed near the transmitter. A low-loss coaxial cable was used to connect the near-field probe to the spectrum analyzer. The EUT was configured according to the following block diagram:

The signal generator was set to multitone operation to cause equal interference across the entire band. The amplitude of the multitone signals (out of operation region) were set to the LBT threshold of $10 \cdot \text{LOG}(\text{Bandwidth}) - 150 + \text{Antenna Gain} + 3 \text{ dB}$.

The spectrum analyzer was set to measure the transmit band of 402-405 MHz. The multitone signal of the intended frequency (F_c) was set to a level above the LBT threshold, and lowered by 1 dB increments until the EUT chooses the intended frequency (F_c) to start a session on.

The blocking frequency at F_c was then lowered to $F_c - \text{Bandwidth} / 2$. The amplitude was then raised until the EUT chooses a channel other than F_c . This was repeated with the blocking frequency raised to $F_c + \text{Bandwidth} / 2$.

The signal generator amplitude at F_c was measured at

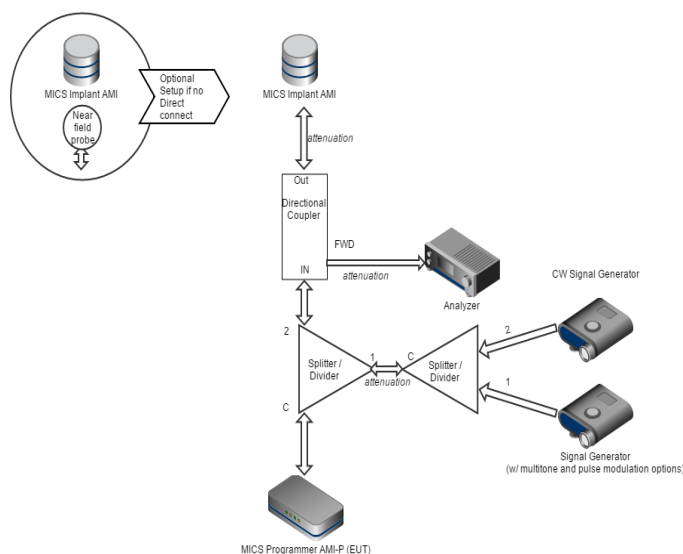


MONITORING SYSTEM BANDWIDTH, 10 CHANNEL


EUT: Model 3300		Work Order: BSTN0663	
Serial Number: 58		Date: 08/08/16	
Customer: Boston Scientific Corporation		Temperature: 23.2 °C	
Attendees: Pete Musto		Humidity: 53.7% RH	
Project: Laramie Vision		Barometric Pres.: 1019 mbar	
Tested by: Dustin Sparks	Power: 220VAC/60Hz	Job Site: MN02	
TEST SPECIFICATIONS		Test Method	
EN 301 839 V2.1.1:2016		EN 301 839 V2.1.1:2016	
COMMENTS			
EUT emissions bandwidth is 300000 Hz, 2.7 dBi antenna gain. Antenna port B, PRM Application 3869 v. 0.03.13			
DEVIATIONS FROM TEST STANDARD			
None			
Configuration #	7	Signature 	
		Measured Value (dBm)	Limit < (dB)
(Pa) = Fc		-90.53	N/A
(Pb) = Fc - Emissions BW/2		-86.53	20
(Pc) = Fc + Emissions BW/2		-87.53	20
			Result
			N/A
			Pass
			Pass

MONITORING SYSTEM BANDWIDTH, 10 CHANNEL

(Pa) = Fc						
Measured				Limit		
Value (dBm)				< (dB)	Result	
-90.53				N/A	N/A	

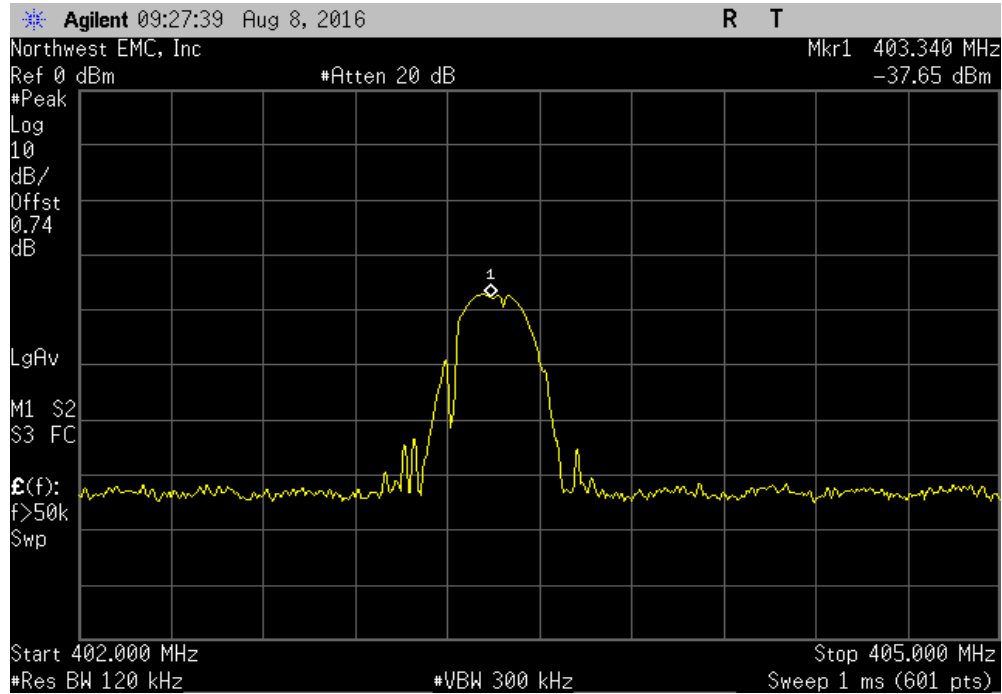


(Pb) = Fc - Emissions BW/2						
Measured				Limit		
Value (dBm)				< (dB)	Result	
-86.53				-4	20	
					Pass	

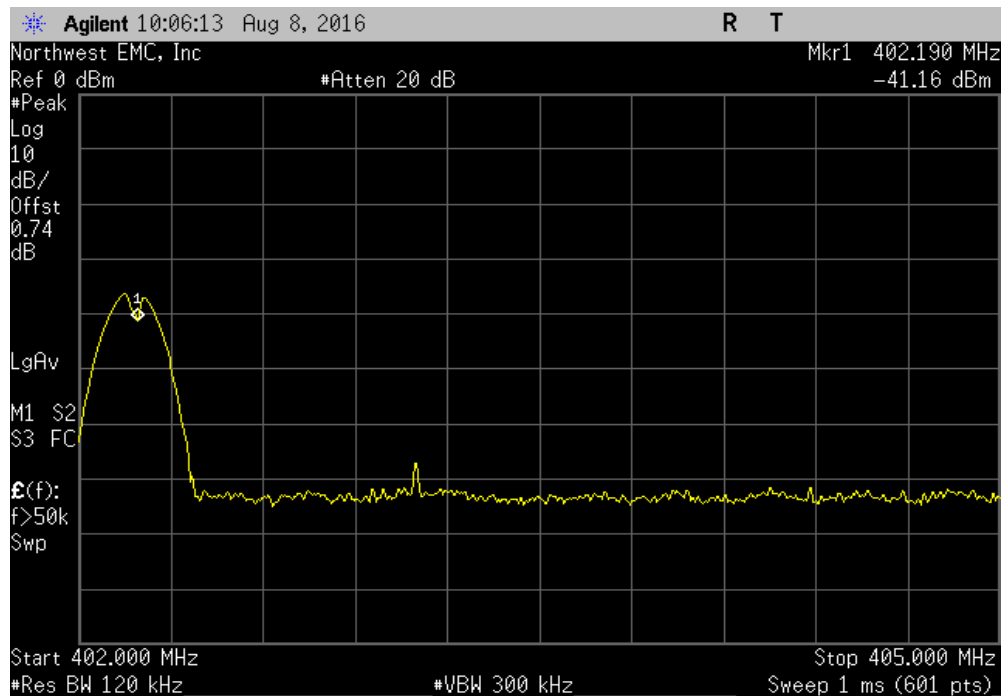

MONITORING SYSTEM BANDWIDTH, 10 CHANNEL


(Pc) = Fc + Emissions BW/2						
Measured			Limit		Result	
Value (dBm)	Value (dB)		< (dB)			
-87.53	-3		20		Pass	

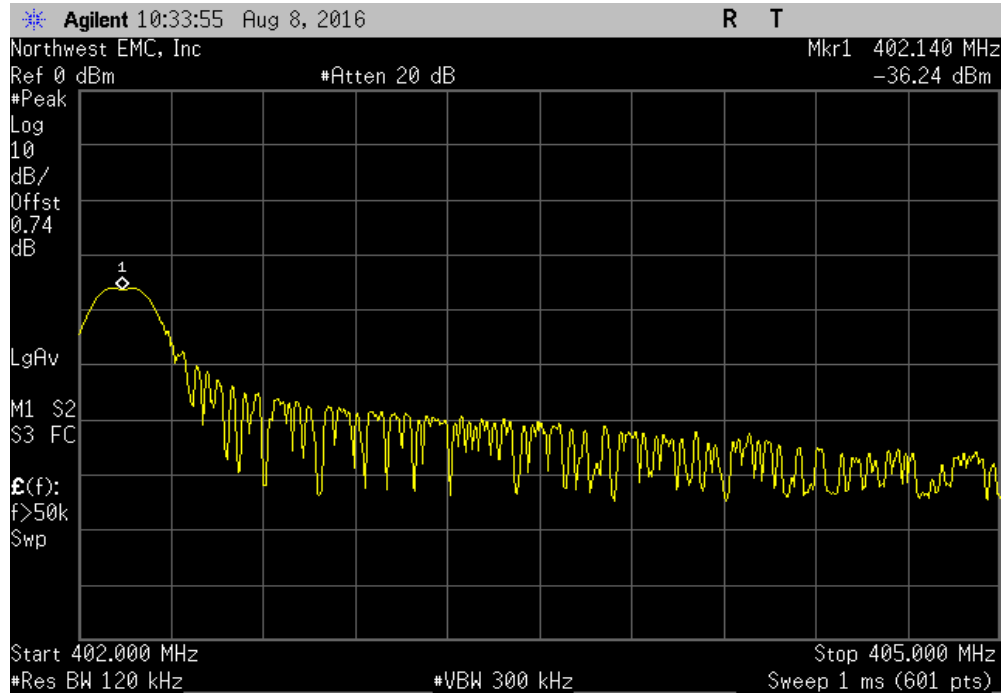



MONITORING SYSTEM BANDWIDTH, 10 CHANNEL

**NORTHWEST
EMC**

XMit 2016.05.06

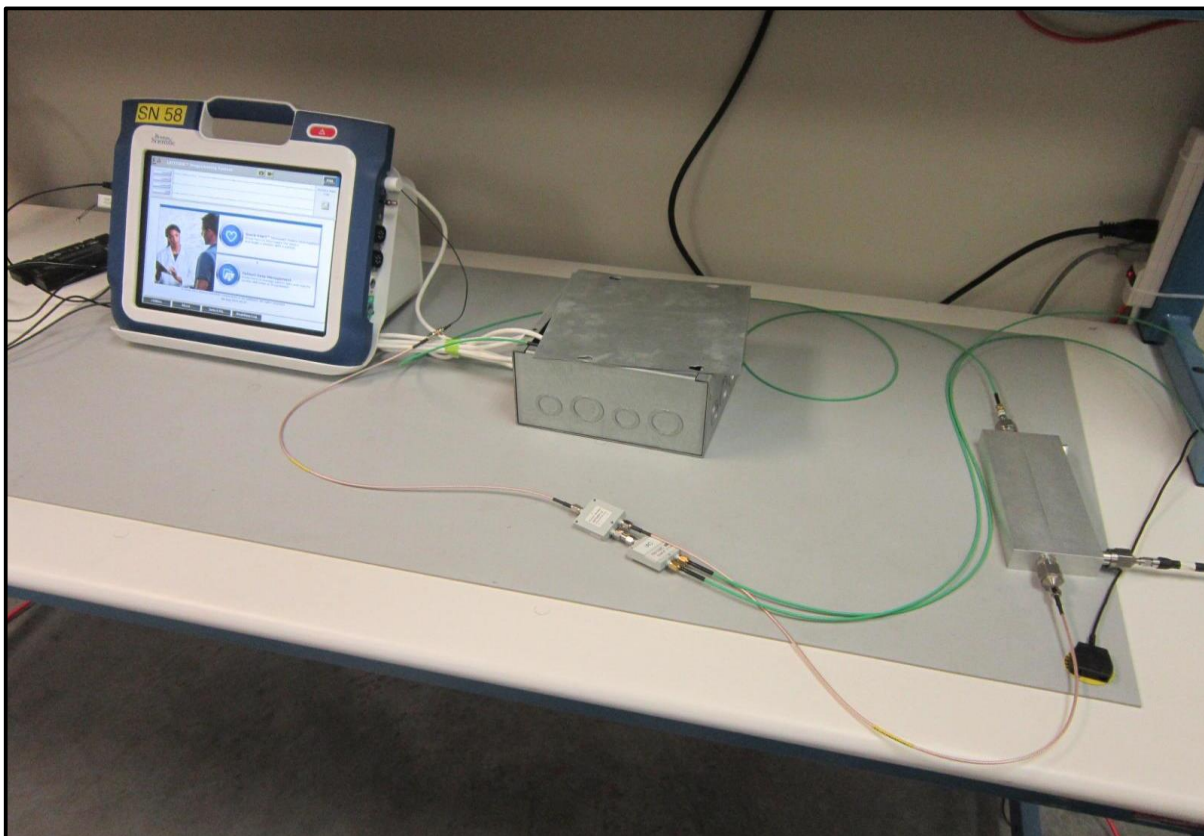

MONITORING SYSTEM BANDWIDTH, 10 CHANNEL

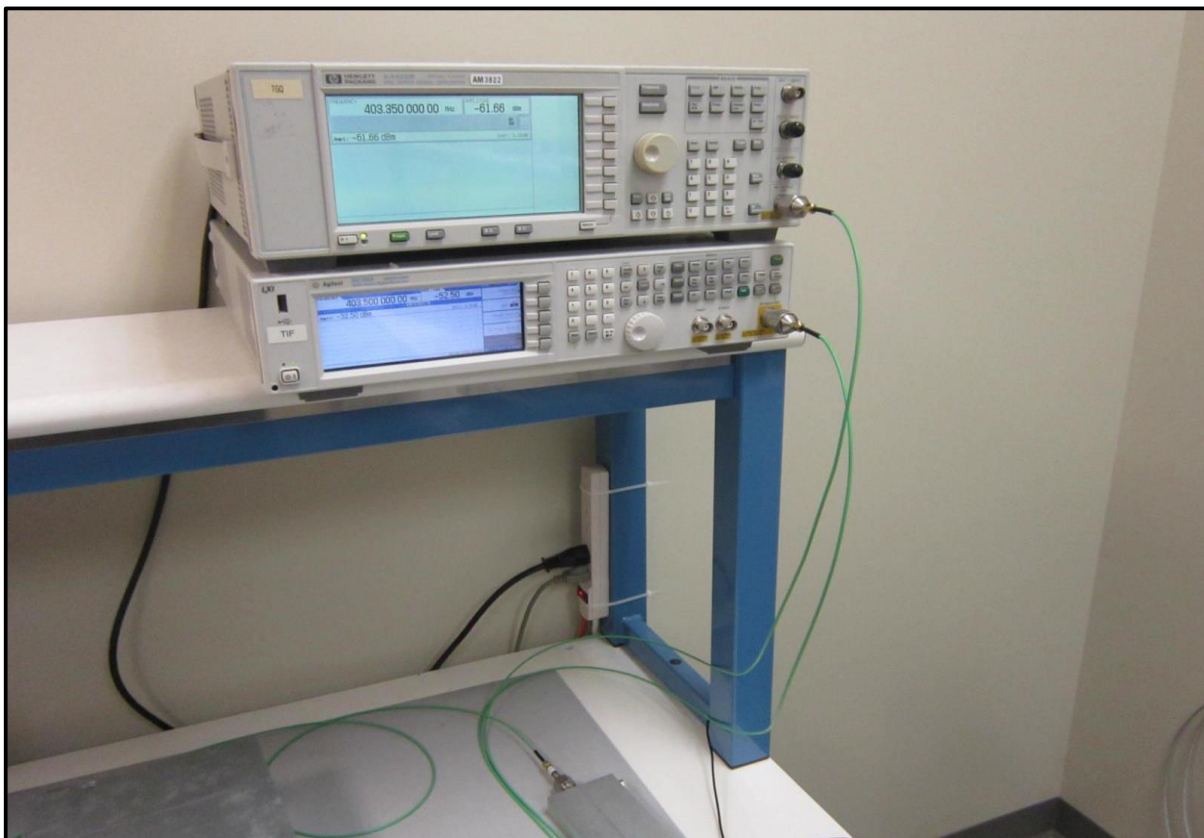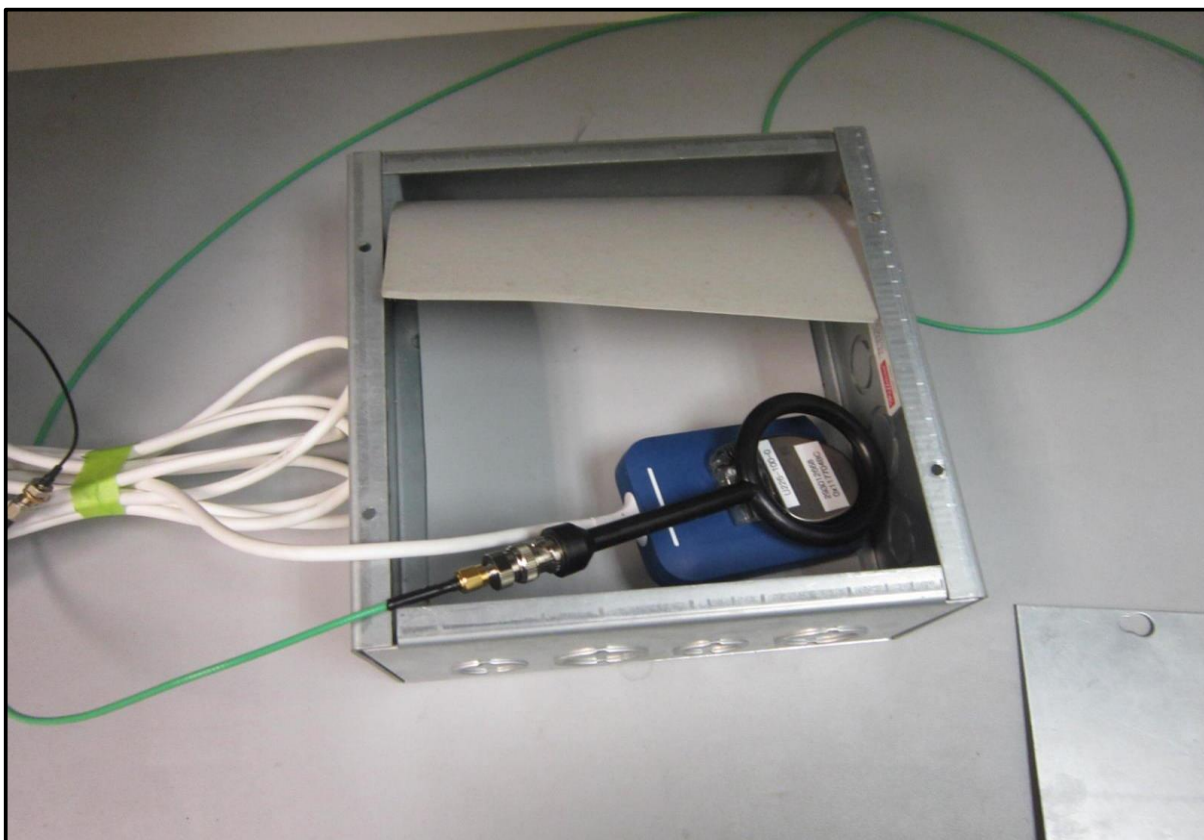

MONITORING SYSTEM BANDWIDTH, 2 CHANNEL

Testing was performed using the mode(s) of operation and configuration(s) noted within the report. The individuals and/or the organization requesting the test provided the modes, configurations and settings used to complete the evaluation. The actual test parameters are specified in the test data, this includes items such as investigated frequency range (scanned) and test levels. The testing methods and performance specifications, as well as the test site used for the evaluation are indicated in the test data.

TEST EQUIPMENT

Description	Manufacturer	Model	ID	Last Cal.	Cal. Due
Probe - Near Field Set	ETS Lindgren	7405	IPO	NCR	NCR
Directional Coupler	Fairview Microwave	SMC4039-10	RGS	NCR	NCR
Power Divider/Combiner	Fairview Microwave Inc (SM electronics)	MP8451-2	IAD	NCR	NCR
Power Divider/Combiner	Fairview Microwave Inc (SM electronics)	MP8451-2	IAC	NCR	NCR
Generator - Signal	Agilent	N5183A	TIK	10/17/2014	10/17/2017
Generator - Signal	Agilent	N5182A	TIF	8/12/2014	8/12/2017
Cable	ESM Cable Corp.	TTBJ141 KMKM-72	MNU	9/18/2015	9/18/2016
Attenuator	S.M. Electronics	SA26B-20	RFW	2/26/2016	2/26/2017
Block - DC	Fairview Microwave	SD3379	AMI	9/18/2015	9/18/2016
Analyzer - Spectrum Analyzer	Agilent	E4440A	AAX	3/24/2016	3/24/2017

TEST DESCRIPTION


The measurement was made using a direct connection between the RF output of the EUT and a spectrum analyzer. The EUT was configured according to the following block diagram:

The signal generator was set to multitone operation to cause equal interference across the entire band. The amplitude of the multitone signals (out of operation region) were set to the LBT threshold of $10 \cdot \log(\text{Bandwidth}) - 150 + \text{Antenna Gain} + 3 \text{ dB}$.

The spectrum analyzer was set to measure the transmit band of 402-405 MHz. The multitone signal of the intended frequency (F_c) was set to a level above the LBT threshold, and lowered by 1 dB increments until the EUT chooses the intended frequency (F_c) to start a session on.

The blocking frequency at F_c was then lowered to $F_c - \text{Bandwidth} / 2$. The amplitude was then raised until the EUT chooses a channel other than F_c . This was repeated with the blocking frequency raised to $F_c + \text{Bandwidth} / 2$.

The signal generator amplitude at F_c was measured at each point.

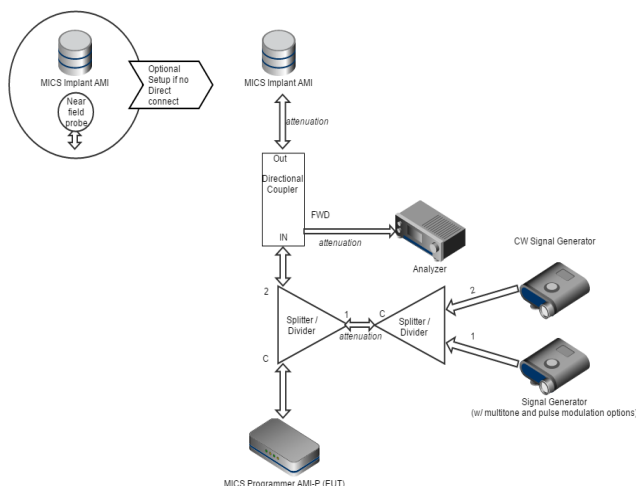


MONITORING SYSTEM BANDWIDTH, 2 CHANNEL


EUT: Model 3300		Work Order: BSTN0663	
Serial Number: 058		Date: 08/16/16	
Customer: Boston Scientific Corporation		Temperature: 23.6 °C	
Attendees: Pete Musto		Humidity: 59.8% RH	
Project: Laramie Vision		Barometric Pres.: 1019 mbar	
Tested by: Dustin Sparks	Power: 110VAC/60Hz	Job Site: MN08	
TEST SPECIFICATIONS		Test Method	
EN 301 839 V2.1.1:2016		EN 301 839 V2.1.1:2016	
COMMENTS			
EUT bandwidth is 300000 Hz with an antenna gain of -5 dBi.			
DEVIATIONS FROM TEST STANDARD			
None			
Configuration #	10	Signature 	
		Measured Value (dBm)	Value (dB)
(Pa) = Fc		-70.15	N/A
(Pb) = Fc - Emissions BW/2		-57.15	13
(Pc) = Fc + Emissions BW/2		-56.15	14
			Limit (dB)
			<= 20
			<= 20
			Result
			N/A
			Pass
			Pass

MONITORING SYSTEM BANDWIDTH, 2 CHANNEL

(Pa) = Fc						
	Measured Value (dBm)		Value (dB)	Limit (dB)	Result	
	-70.15		N/A	N/A	N/A	

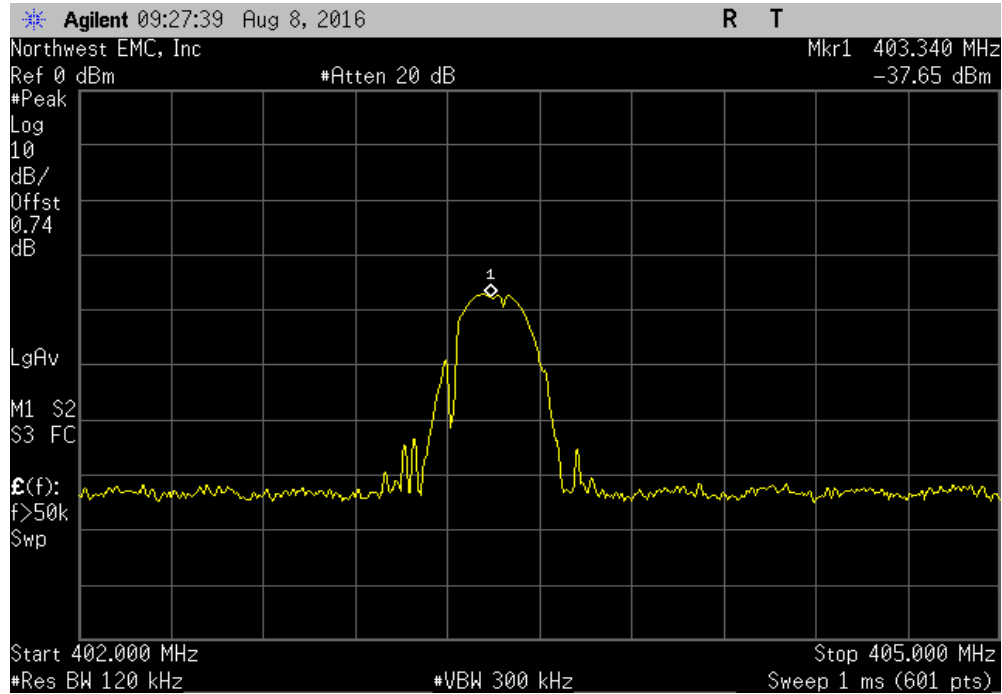


(Pb) = Fc - Emissions BW/2						
	Measured Value (dBm)		Value (dB)	Limit (dB)	Result	
	-57.15		13	<= 20	Pass	

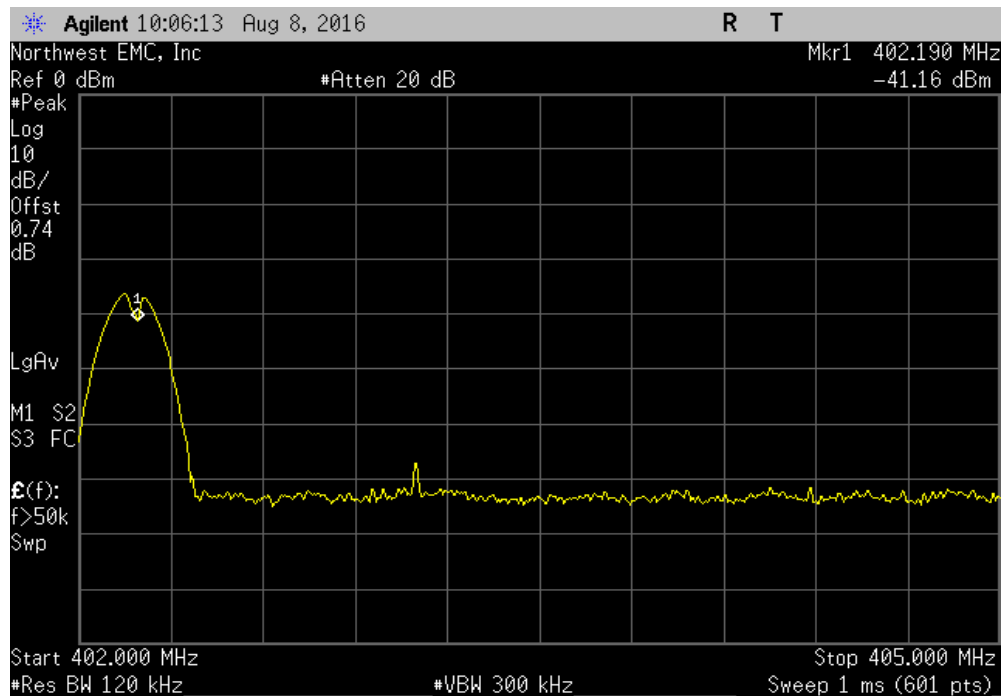


MONITORING SYSTEM BANDWIDTH, 2 CHANNEL

(Pc) = Fc + Emissions BW/2						
	Measured Value (dBm)		Value (dB)		Limit (dB)	Result
	-56.15		14		<= 20	Pass

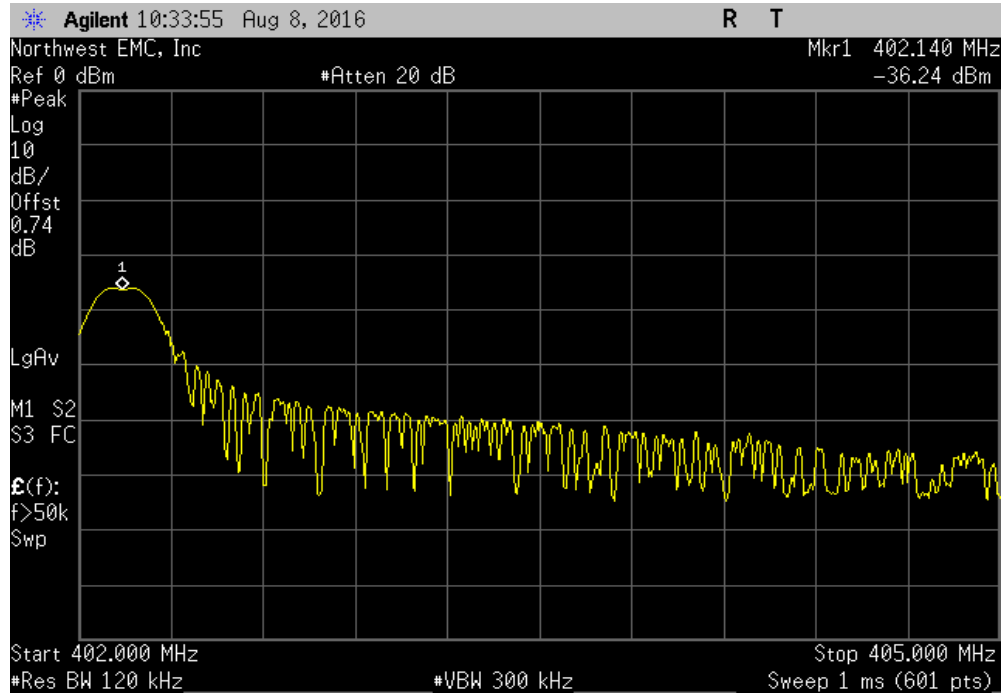

MONITORING SYSTEM BANDWIDTH, 2 CHANNEL

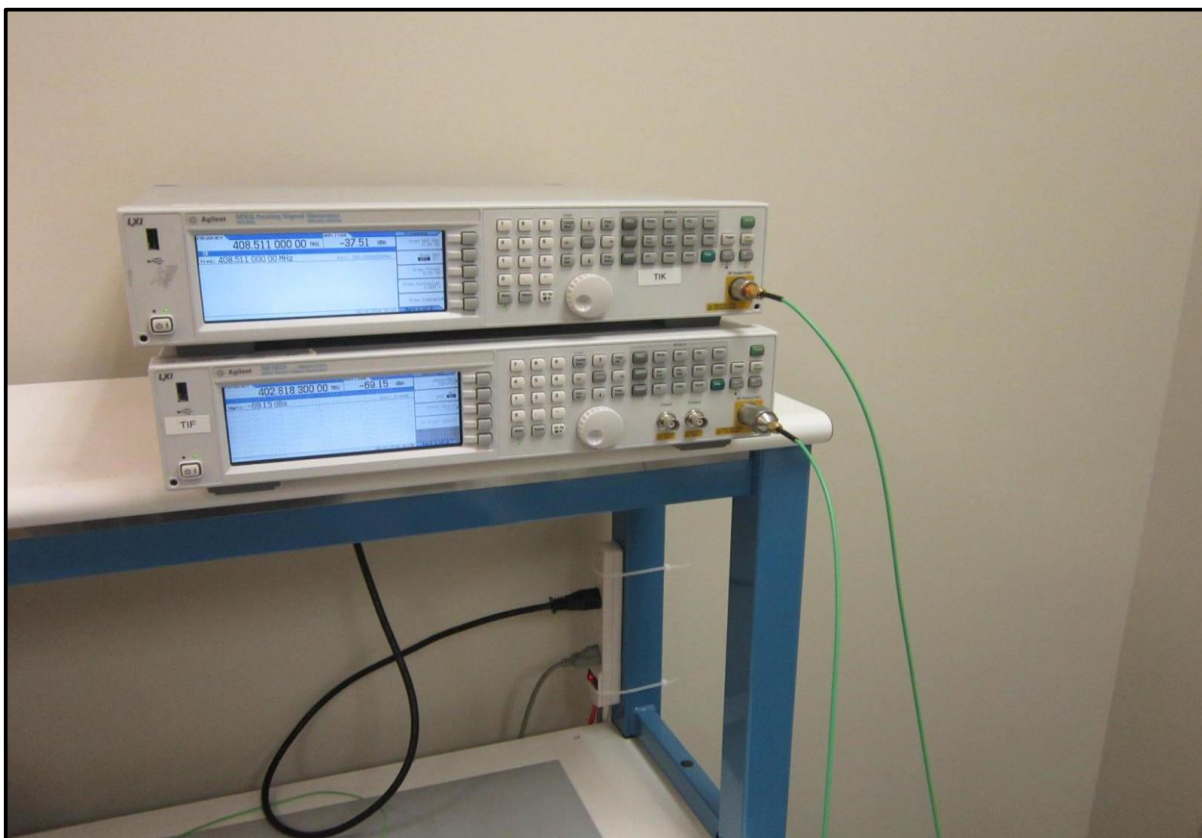

MONITORING SYSTEM BANDWIDTH, 2 CHANNEL



NORTHWEST EMC

Testing was performed using the mode(s) of operation and configuration(s) noted within the report. The individuals and/or the organization requesting the test provided the modes, configurations and settings used to complete the evaluation. The actual test parameters are specified in the test data, this includes items such as investigated frequency range (scanned) and test levels. The testing methods and performance specifications, as well as the test site used for the evaluation are indicated in the test data.

TEST EQUIPMENT


Description	Manufacturer	Model	ID	Last Cal.	Cal. Due
Directional Coupler	Fairview Microwave	SMC4039-10	RGS	NCR	NCR
Probe - Near Field Set	ETS Lindgren	7405	IPO	NCR	NCR
Power Divider/Combiner	Fairview Microwave Inc (SM electronics)	MP8451-2	IAD	NCR	NCR
Power Divider/Combiner	Fairview Microwave Inc (SM electronics)	MP8451-2	IAC	NCR	NCR
Generator - Signal	Agilent	E4422B	TGQ	3/17/2015	3/17/2018
Generator - Signal	Agilent	N5182A	TIF	8/12/2014	8/12/2017
Cable	ESM Cable Corp.	TTBJ141 KMKM-72	MNU	9/18/2015	9/18/2016
Block - DC	Fairview Microwave	SD3379	AMI	9/18/2015	9/18/2016
Analyzer - Spectrum Analyzer	Agilent	E4440A	AAX	3/24/2016	3/24/2017

TEST DESCRIPTION

A near-field probe was placed near the transmitter. A low-loss coaxial cable was used to connect the near-field probe to the spectrum analyzer. The EUT was configured according to the following block diagram:

The signal generator was set to multitone operation to cause equal interference across the entire band. The spectrum analyzer was set to zero span with a sweep time equal to 10 seconds.

The CW signal on the intended frequency (F_c) was removed. At the same time, the EUT was set to seek a session with the implantable device. The delay between F_c becoming available and the EUT establishing a session was measured.

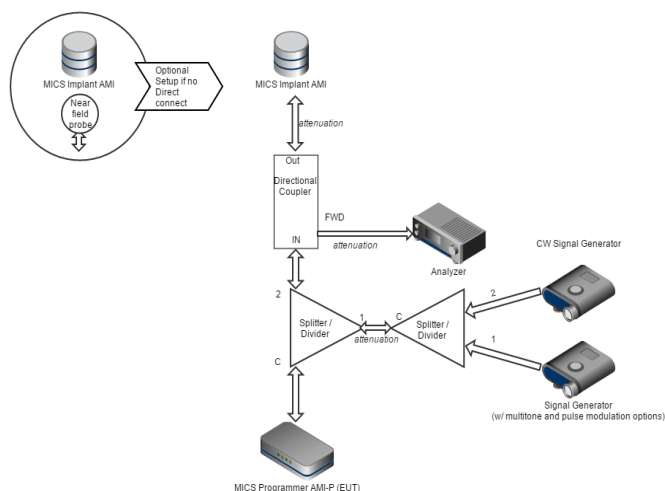

MONITORING SYSTEM SCAN CYCLE TIME, 10 CHANNEL




XMR 2016.05.06


EUT: Model 3300		Work Order: BSTN0663	
Serial Number: 058		Date: 08/08/16	
Customer: Boston Scientific Corporation		Temperature: 23.3 °C	
Attendees: Pete Musto		Humidity: 54.3% RH	
Project: Laramie Vision		Barometric Pres.: 1018 mbar	
Tested by: Dustin Sparks		Power: 220VAC/60Hz	
		Job Site: MN02	
TEST SPECIFICATIONS			
EN 301 839 V2.1.1:2016		Test Method	
EN 301 839 V2.1.1:2016		EN 301 839 V2.1.1:2016	
COMMENTS			
EUT emissions bandwidth is 300000 Hz, 2.7 dBi antenna gain. Antenna port B, MT1 v. 2.0-7			
DEVIATIONS FROM TEST STANDARD			
None			
Configuration #	8	Signature 	
		Value (s)	Limit (s)
Sample 1		2.109	<= 5
Sample 2		2.181	<= 5
Sample 3		2.509	<= 5
Sample 4		2.441	<= 5
Sample 5		2.401	<= 5
Sample 6		2.249	<= 5
Sample 7		2.381	<= 5
Sample 8		2.145	<= 5
Sample 9		2.365	<= 5
Sample 10		2.349	<= 5
			Result
			Pass
			Pass
			Pass
			Pass
			Pass
			Pass
			Pass
			Pass
			Pass
			Pass

MONITORING SYSTEM SCAN CYCLE TIME, 10 CHANNEL

Sample 1						
				Value (s)	Limit (s)	Result
				2.109	<= 5	Pass

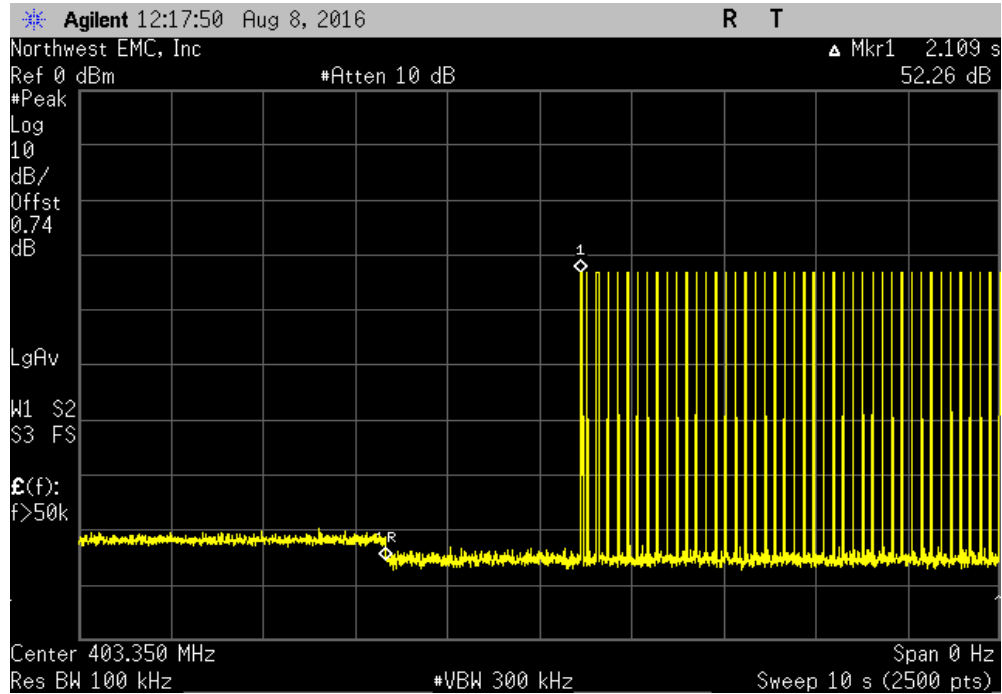


Sample 2						
				Value (s)	Limit (s)	Result
				2.181	<= 5	Pass

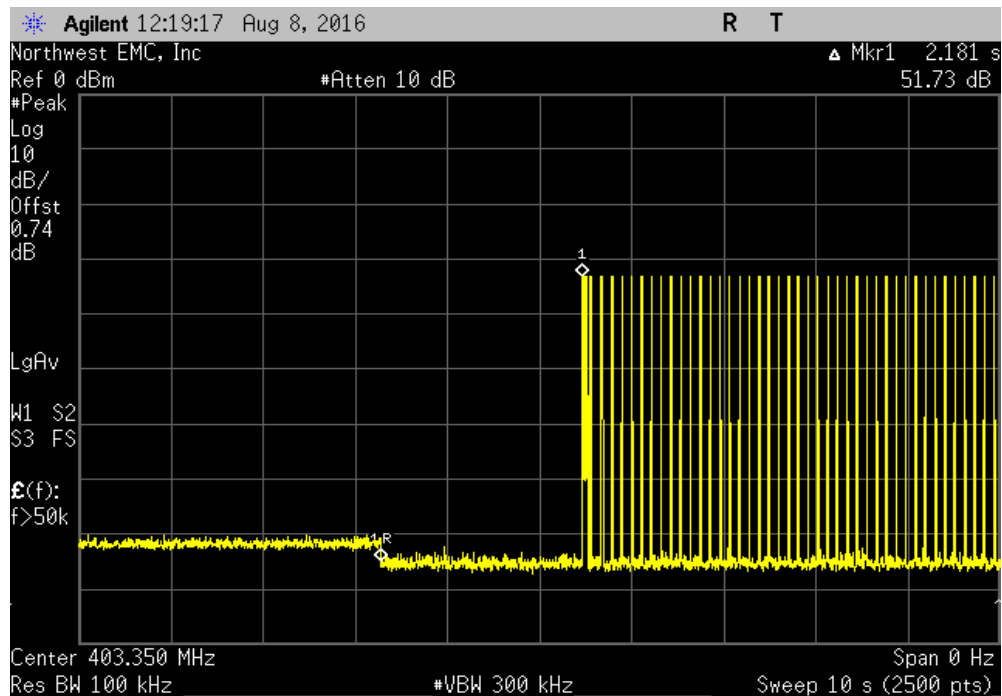


MONITORING SYSTEM SCAN CYCLE TIME, 10 CHANNEL

Sample 3						
				Value (s)	Limit (s)	Result
				2.509	<= 5	Pass

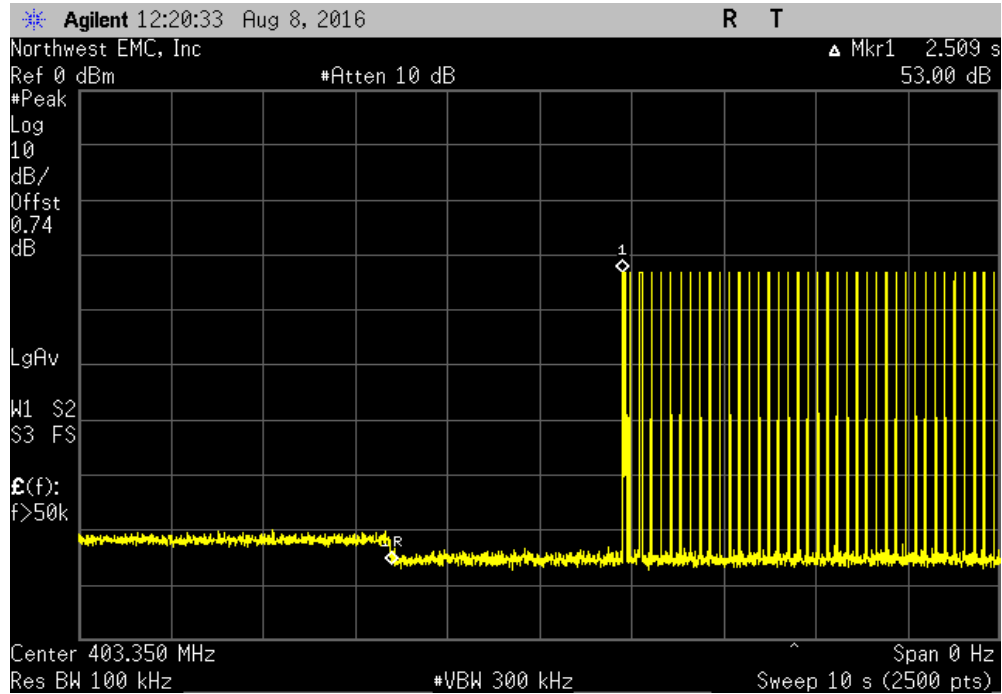


Sample 4						
				Value (s)	Limit (s)	Result
				2.441	<= 5	Pass

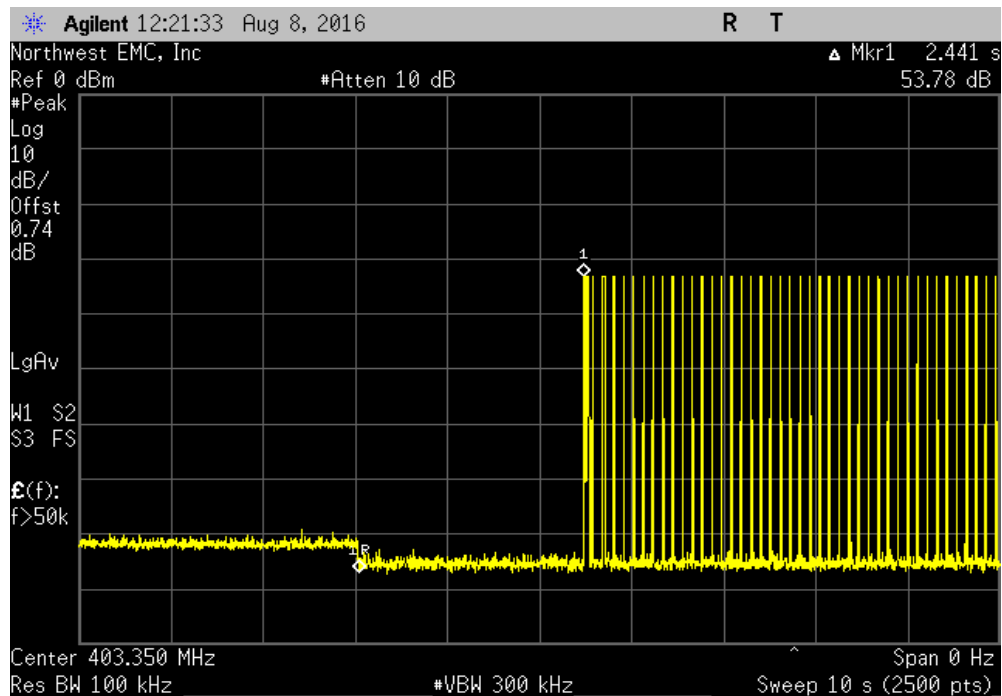


MONITORING SYSTEM SCAN CYCLE TIME, 10 CHANNEL

Sample 5						
				Value (s)	Limit (s)	Result
				2.401	<= 5	Pass

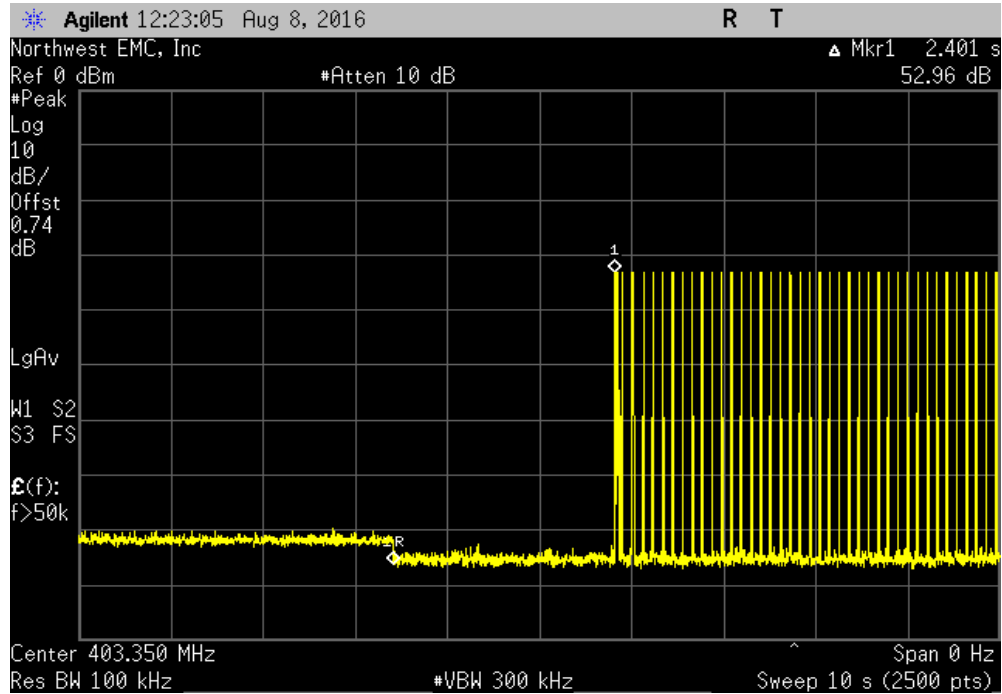


Sample 6						
				Value (s)	Limit (s)	Result
				2.249	<= 5	Pass

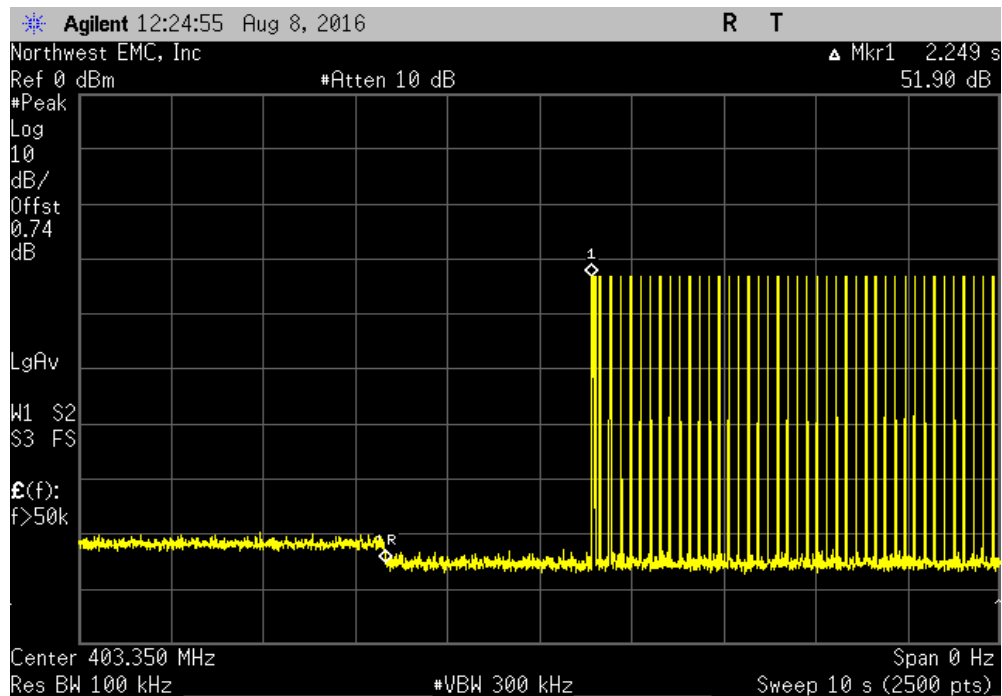


MONITORING SYSTEM SCAN CYCLE TIME, 10 CHANNEL

Sample 7						
				Value (s)	Limit (s)	Result
				2.381	<= 5	Pass

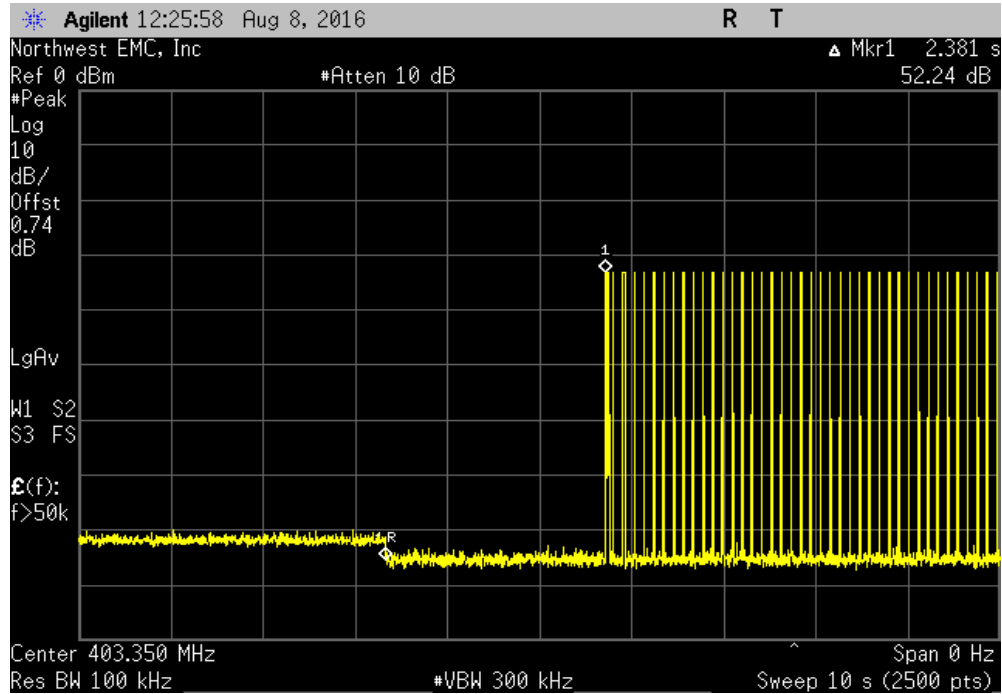


Sample 8						
				Value (s)	Limit (s)	Result
				2.145	<= 5	Pass

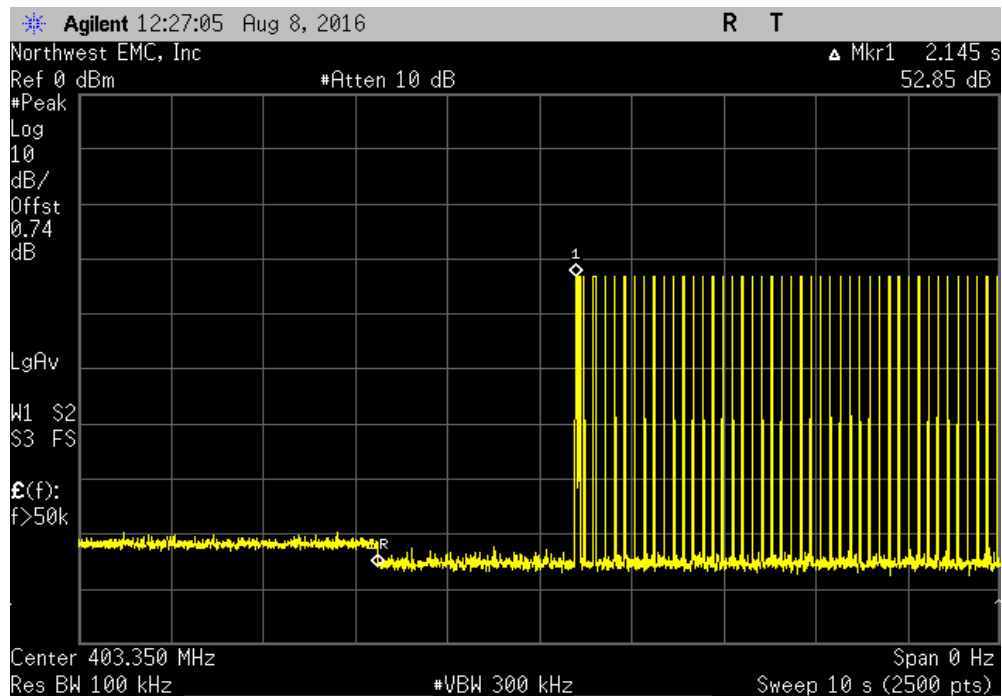


MONITORING SYSTEM SCAN CYCLE TIME, 10 CHANNEL

Sample 9						
				Value (s)	Limit (s)	Result
				2.365	<= 5	Pass

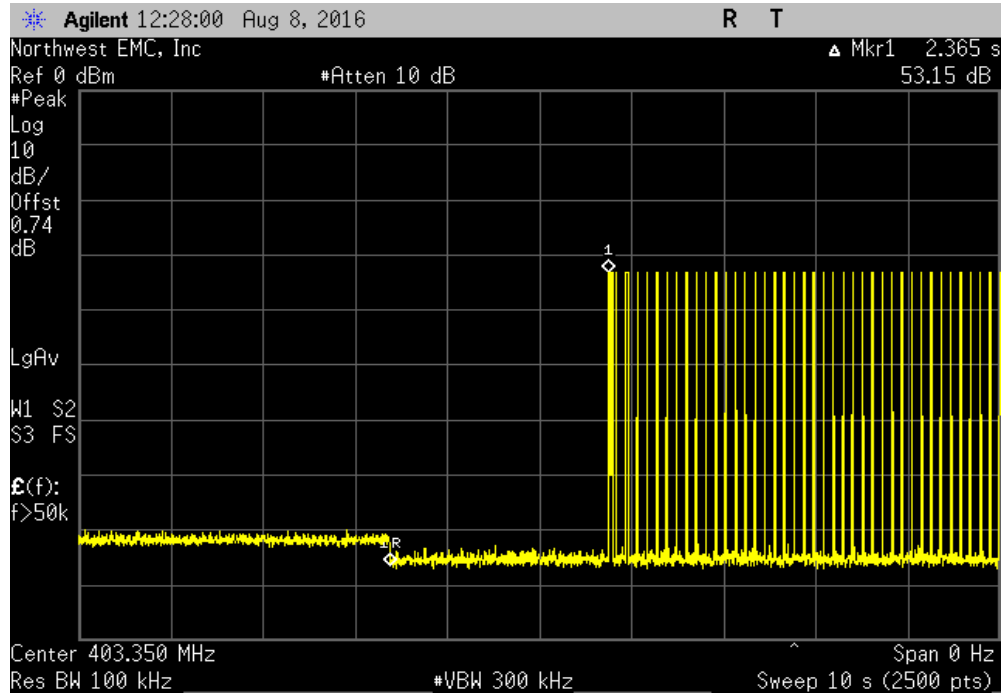



Sample 10						
				Value (s)	Limit (s)	Result
				2.349	<= 5	Pass

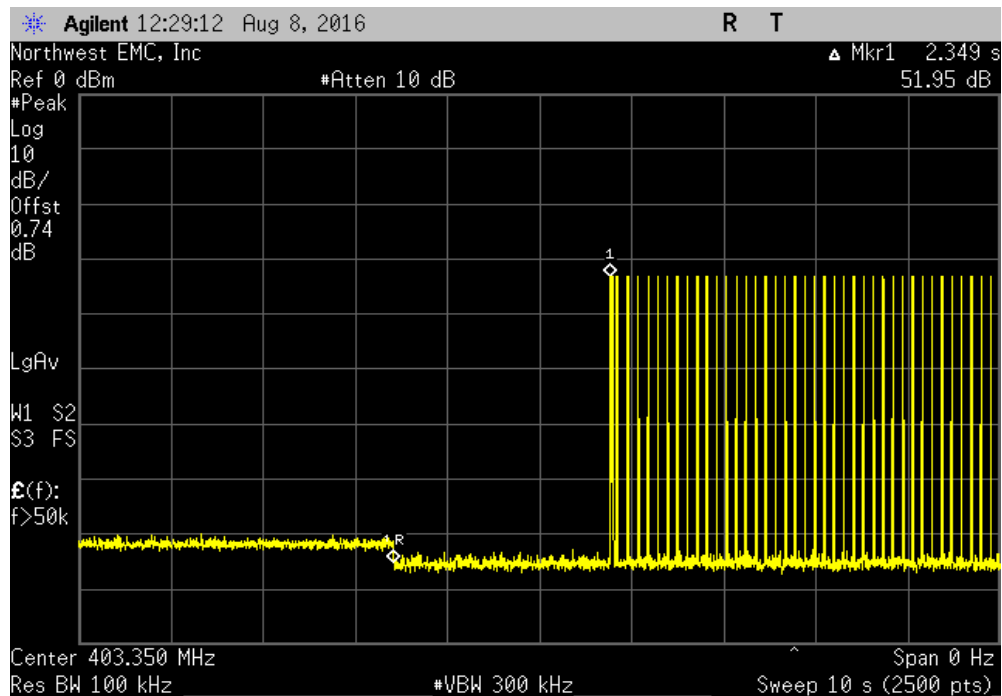



MONITORING SYSTEM SCAN CYCLE TIME, 10 CHANNEL

**NORTHWEST
EMC**

XMit 2016.05.06

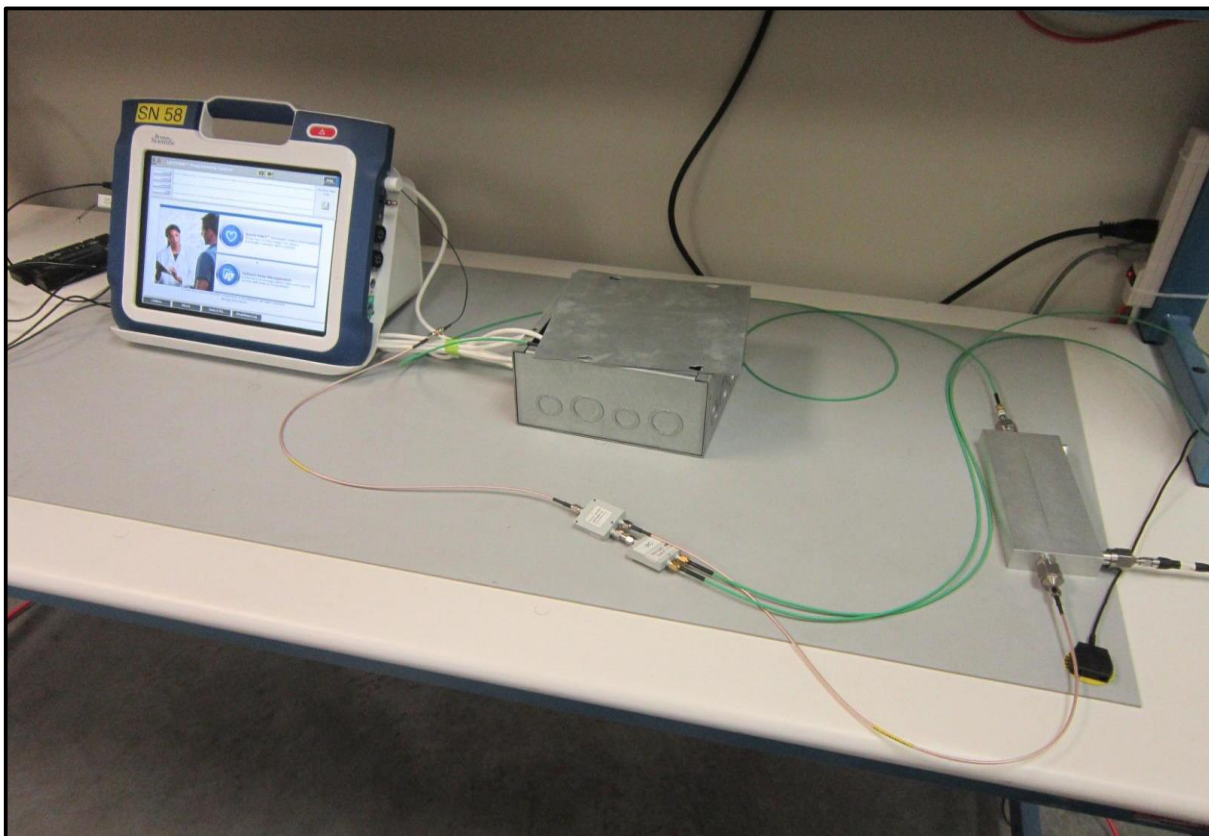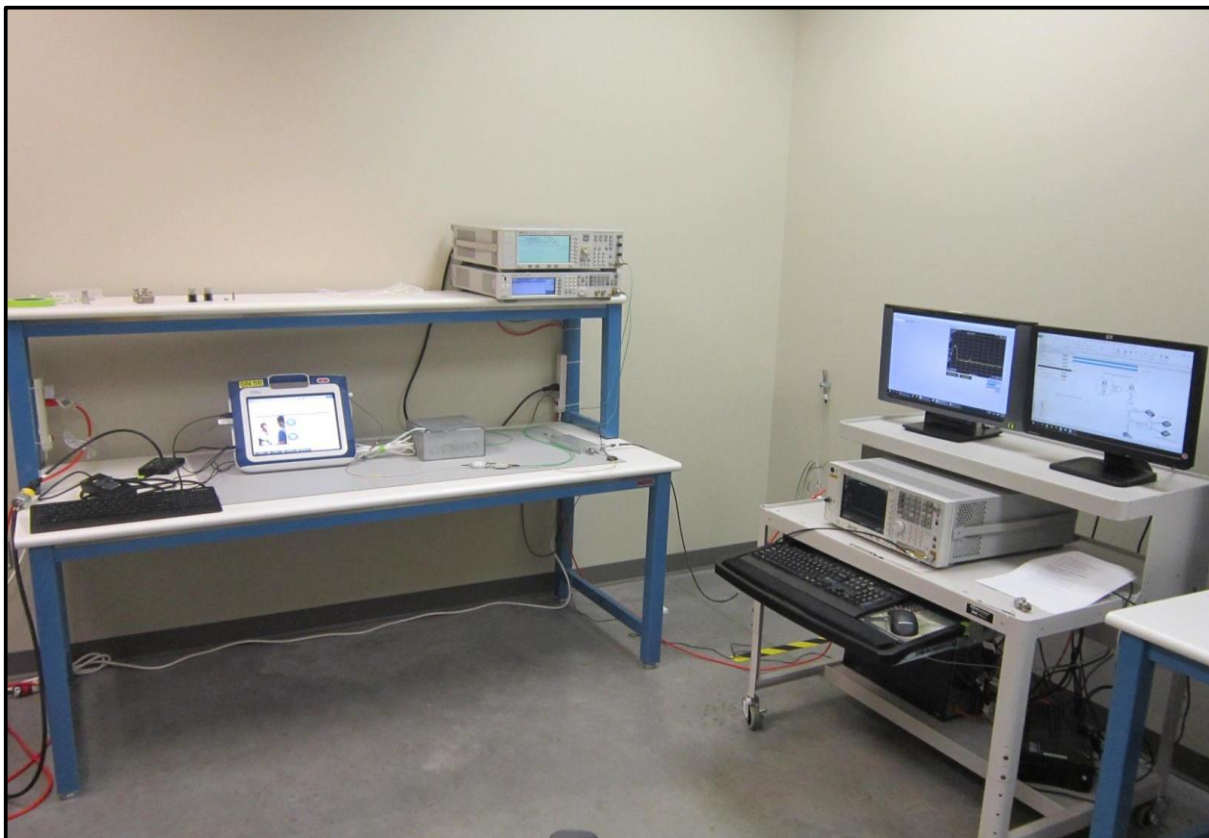

MONITORING SYSTEM SCAN CYCLE TIME, 10 CHANNEL

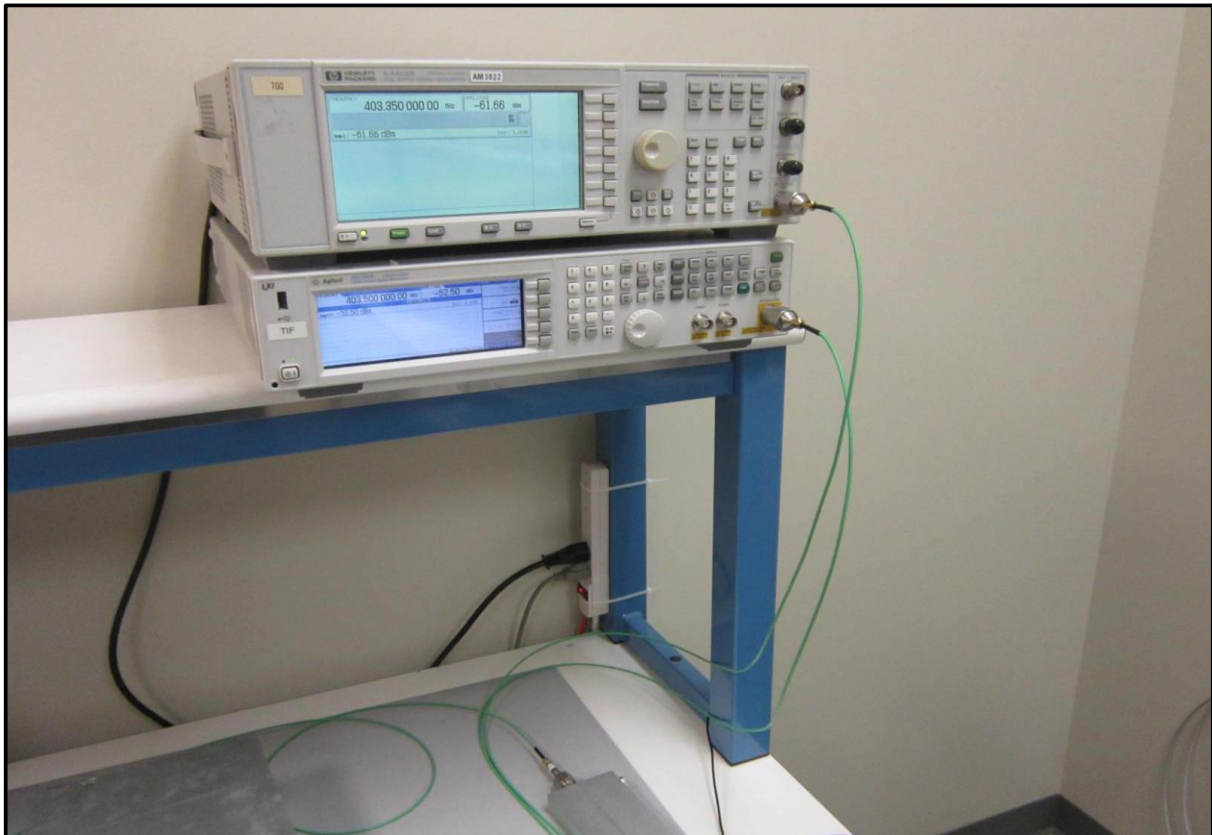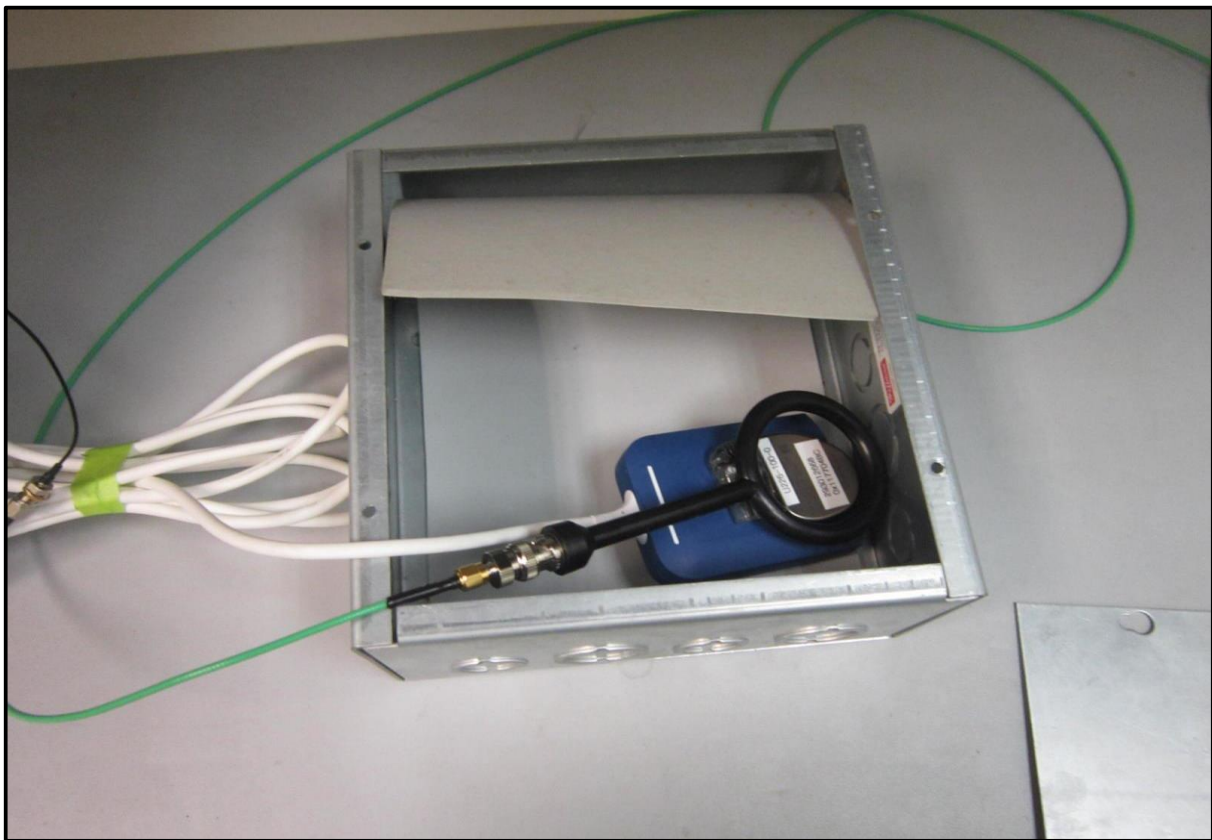

MONITORING SYSTEM SCAN CYCLE TIME, 2 CHANNEL

Testing was performed using the mode(s) of operation and configuration(s) noted within the report. The individuals and/or the organization requesting the test provided the modes, configurations and settings used to complete the evaluation. The actual test parameters are specified in the test data, this includes items such as investigated frequency range (scanned) and test levels. The testing methods and performance specifications, as well as the test site used for the evaluation are indicated in the test data.

TEST EQUIPMENT


Description	Manufacturer	Model	ID	Last Cal.	Cal. Due
Probe - Near Field Set	ETS Lindgren	7405	IPO	NCR	NCR
Directional Coupler	Fairview Microwave	SMC4039-10	RGS	NCR	NCR
Power Divider/Combiner	Fairview Microwave Inc (SM electronics)	MP8451-2	IAD	NCR	NCR
Power Divider/Combiner	Fairview Microwave Inc (SM electronics)	MP8451-2	IAC	NCR	NCR
Generator - Signal	Agilent	N5183A	TIK	10/17/2014	10/17/2017
Generator - Signal	Agilent	N5182A	TIF	8/12/2014	8/12/2017
Cable	ESM Cable Corp.	TTBJ141 KMKM-72	MNU	9/18/2015	9/18/2016
Attenuator	S.M. Electronics	SA26B-20	RFW	2/26/2016	2/26/2017
Block - DC	Fairview Microwave	SD3379	AMI	9/18/2015	9/18/2016
Analyzer - Spectrum Analyzer	Agilent	E4440A	AAX	3/24/2016	3/24/2017

TEST DESCRIPTION

The measurement was made using a direct connection between the RF output of the EUT and a spectrum analyzer. The EUT was configured according to the following block diagram:

The signal generator was set to multitone operation to cause equal interference across the entire band. The spectrum analyzer was set to zero span with a sweep time equal to 10 seconds.


The CW signal on the intended frequency (F_c) was removed. At the same time, the EUT was set to seek a session with the implantable device. The delay between F_c becoming available and the EUT establishing a session was measured.

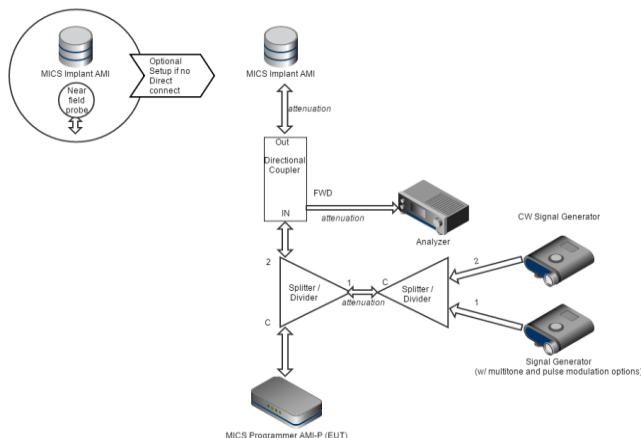

MONITORING SYSTEM SCAN CYCLE TIME, 2 CHANNEL




XMR 2016.05.06


EUT: Model 3300		Work Order: BSTN0663	
Serial Number: 058		Date: 08/16/16	
Customer: Boston Scientific Corporation		Temperature: 23.6 °C	
Attendees: Pete Musto		Humidity: 59.7% RH	
Project: Laramie Vision		Barometric Pres.: 1019 mbar	
Tested by: Dustin Sparks	Power: 110VAC/60Hz	Job Site: MN08	
TEST SPECIFICATIONS		Test Method	
EN 301 839 V2.1.1:2016		EN 301 839 V2.1.1:2016	
COMMENTS			
EUT bandwidth is 300000 Hz with an antenna gain of -5 dBi. Communications session was initiated at ~2 seconds into each 10 second single sweep.			
DEVIATIONS FROM TEST STANDARD			
None			
Configuration #	10	Signature 	
		Value (seconds)	Limit (seconds) Result
Sample 1		2.013	<= 5 Pass
Sample 2		1.565	<= 5 Pass
Sample 3		1.397	<= 5 Pass
Sample 4		1.969	<= 5 Pass
Sample 5		1.857	<= 5 Pass
Sample 6		1.144	<= 5 Pass
Sample 7		1.809	<= 5 Pass
Sample 8		1.649	<= 5 Pass
Sample 9		1.989	<= 5 Pass
Sample 10		1.733	<= 5 Pass

MONITORING SYSTEM SCAN CYCLE TIME, 2 CHANNEL

Sample 1						
				Value (seconds)	Limit (seconds)	Result
				2.013	<= 5	Pass

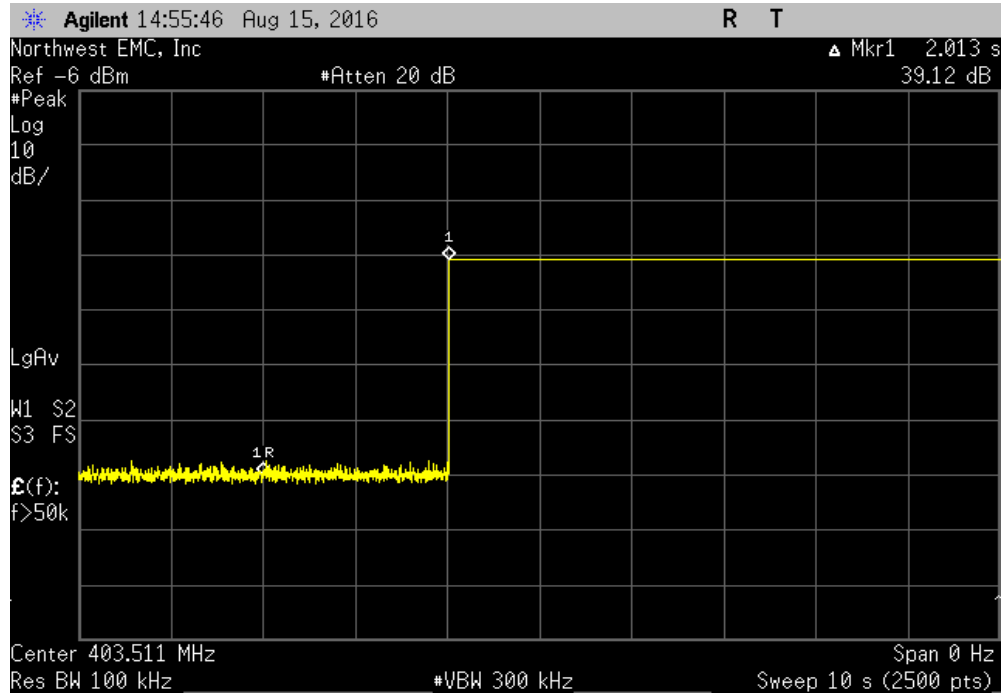


Sample 2						
				Value (seconds)	Limit (seconds)	Result
				1.565	<= 5	Pass

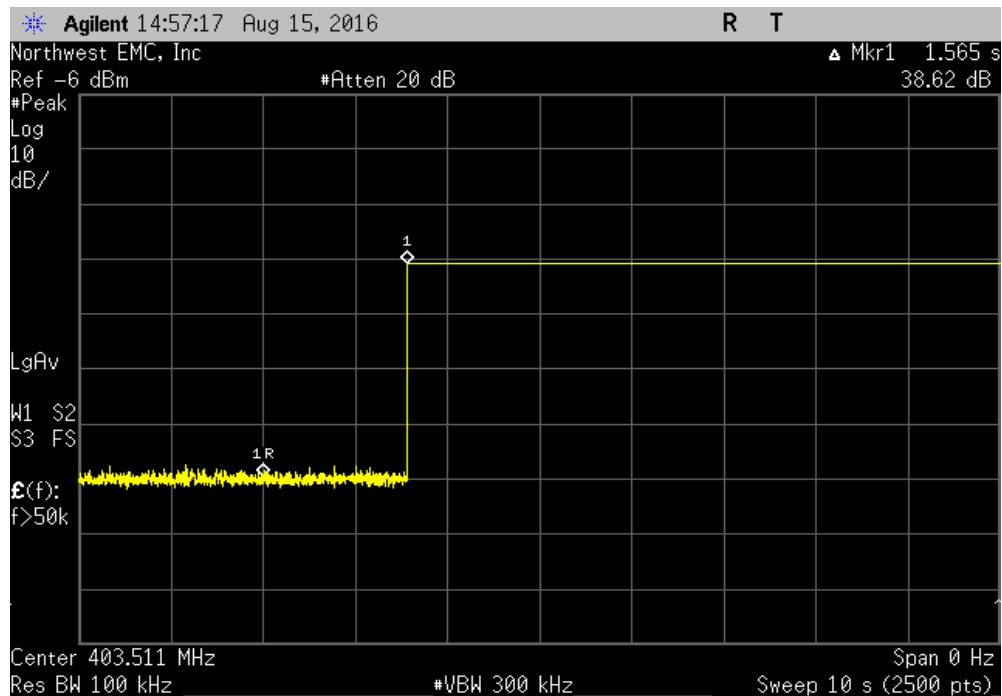


MONITORING SYSTEM SCAN CYCLE TIME, 2 CHANNEL

Sample 3					Value (seconds)	Limit (seconds)	Result
					1.397	<= 5	Pass

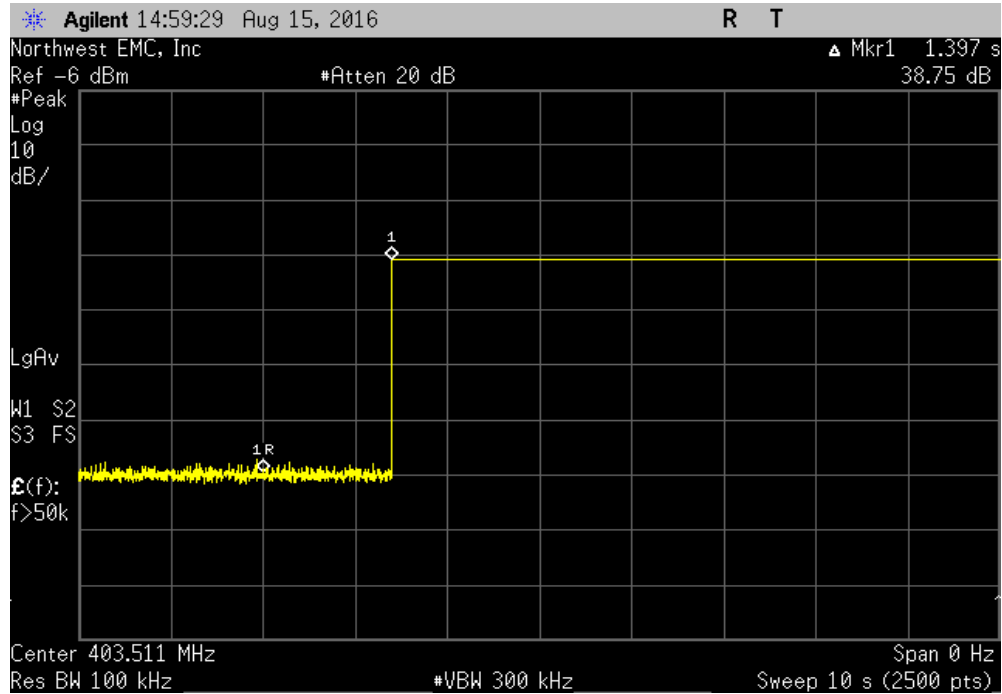


Sample 4					Value (seconds)	Limit (seconds)	Result
					1.969	<= 5	Pass

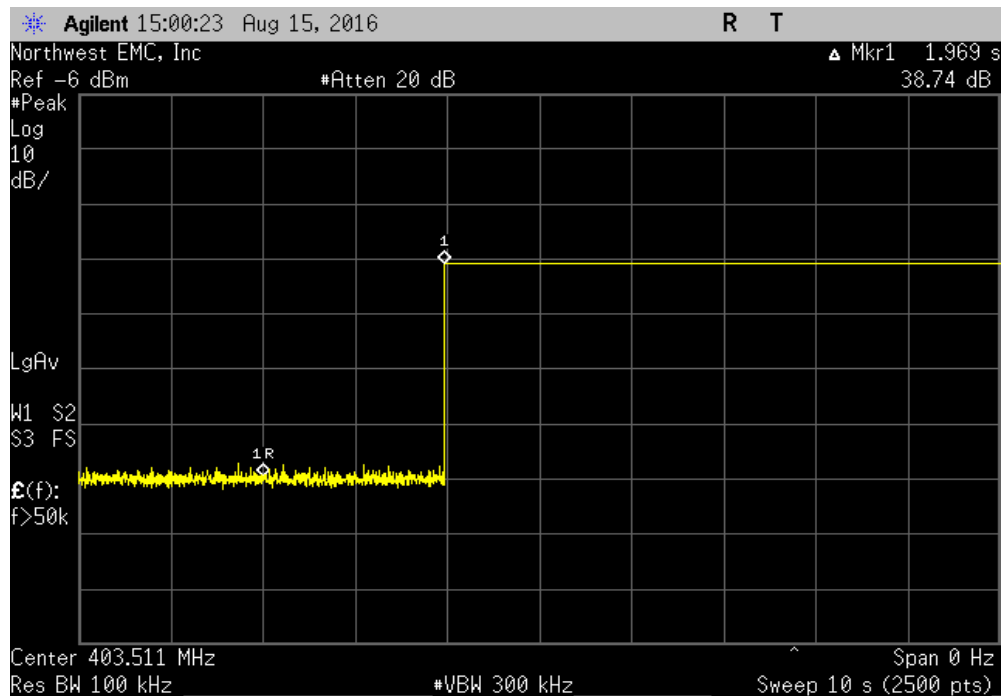


MONITORING SYSTEM SCAN CYCLE TIME, 2 CHANNEL

Sample 5						
				Value (seconds)	Limit (seconds)	Result
				1.857	<= 5	Pass

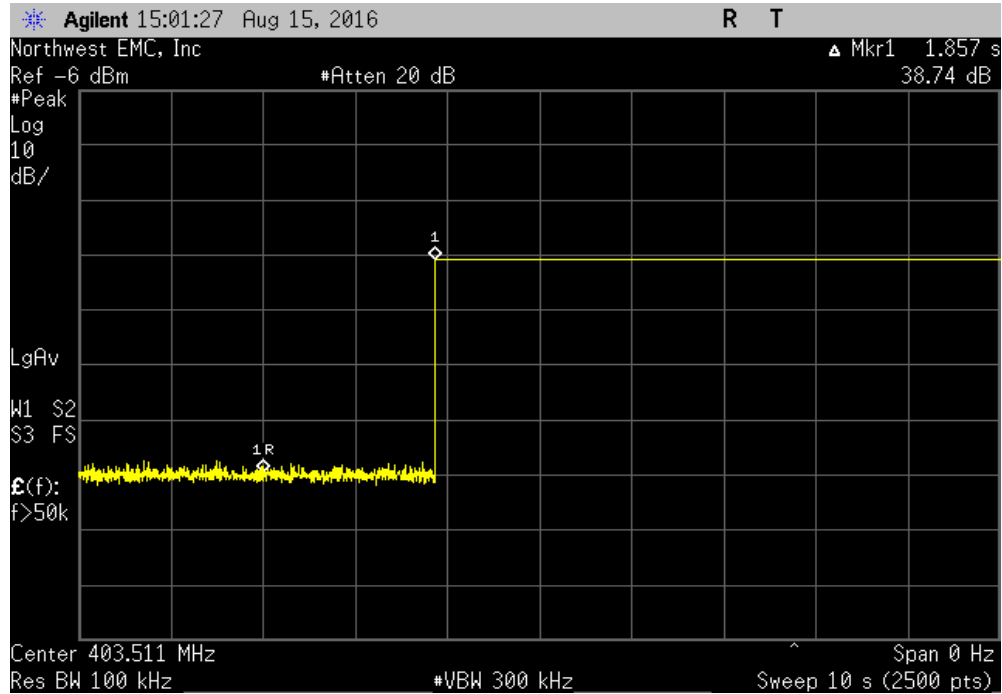


Sample 6						
				Value (seconds)	Limit (seconds)	Result
				1.144	<= 5	Pass

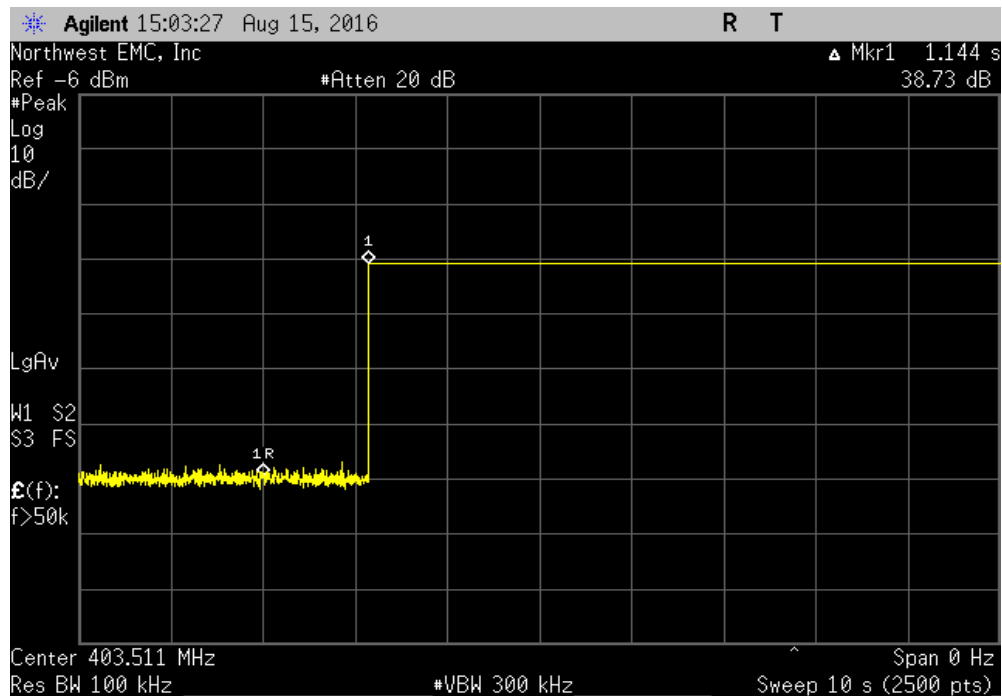


MONITORING SYSTEM SCAN CYCLE TIME, 2 CHANNEL

Sample 7						
				Value (seconds)	Limit (seconds)	Result
				1.809	<= 5	Pass

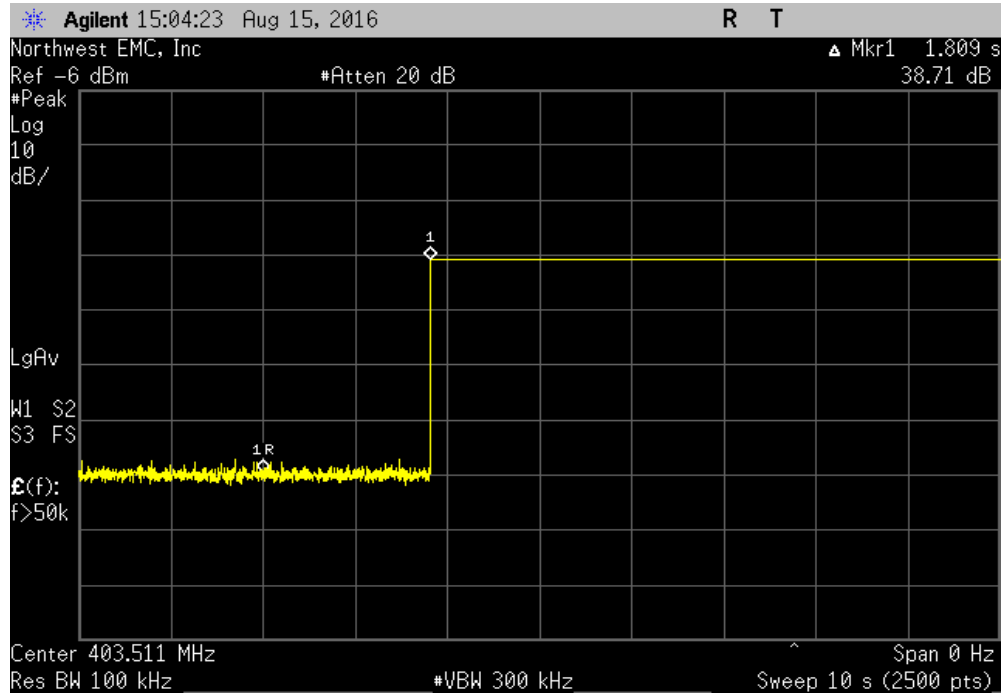


Sample 8						
				Value (seconds)	Limit (seconds)	Result
				1.649	<= 5	Pass

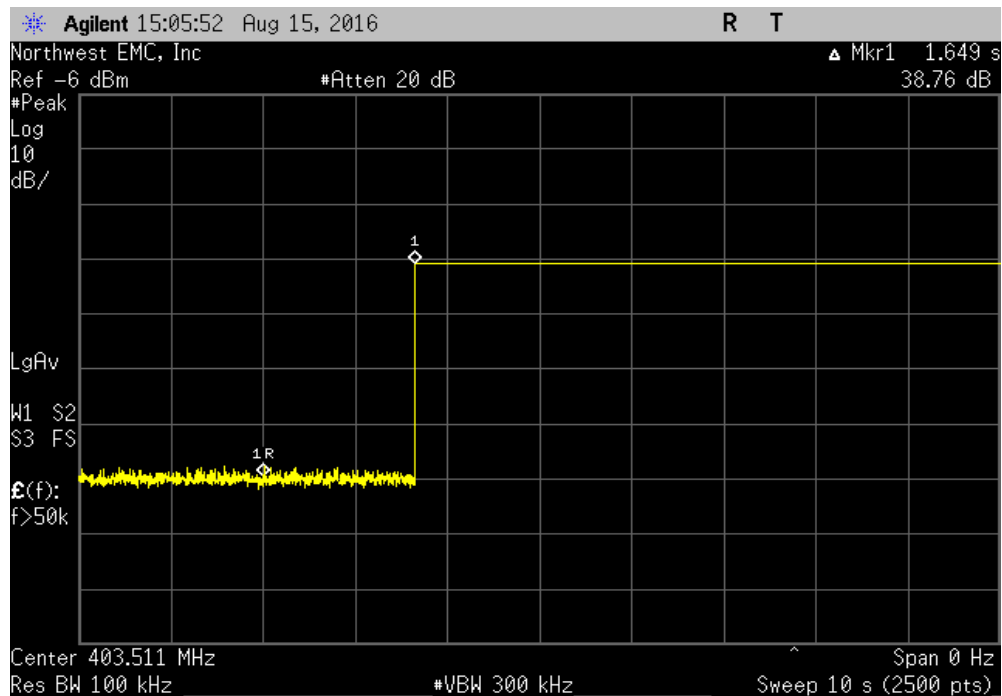


MONITORING SYSTEM SCAN CYCLE TIME, 2 CHANNEL

Sample 9						
				Value (seconds)	Limit (seconds)	Result
				1.989	<= 5	Pass

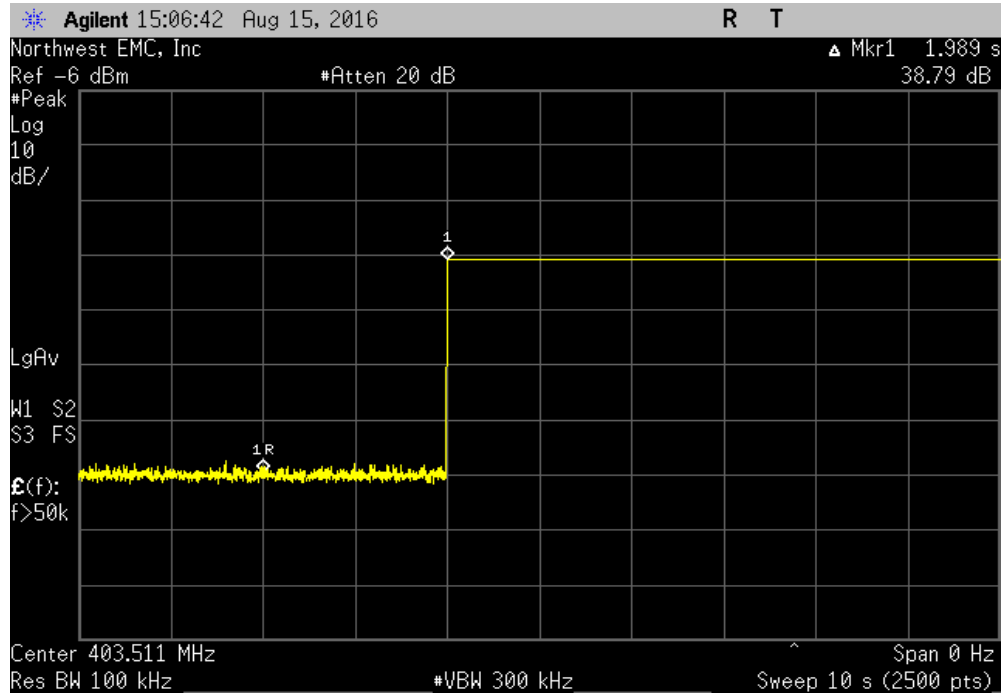


Sample 10						
				Value (seconds)	Limit (seconds)	Result
				1.733	<= 5	Pass

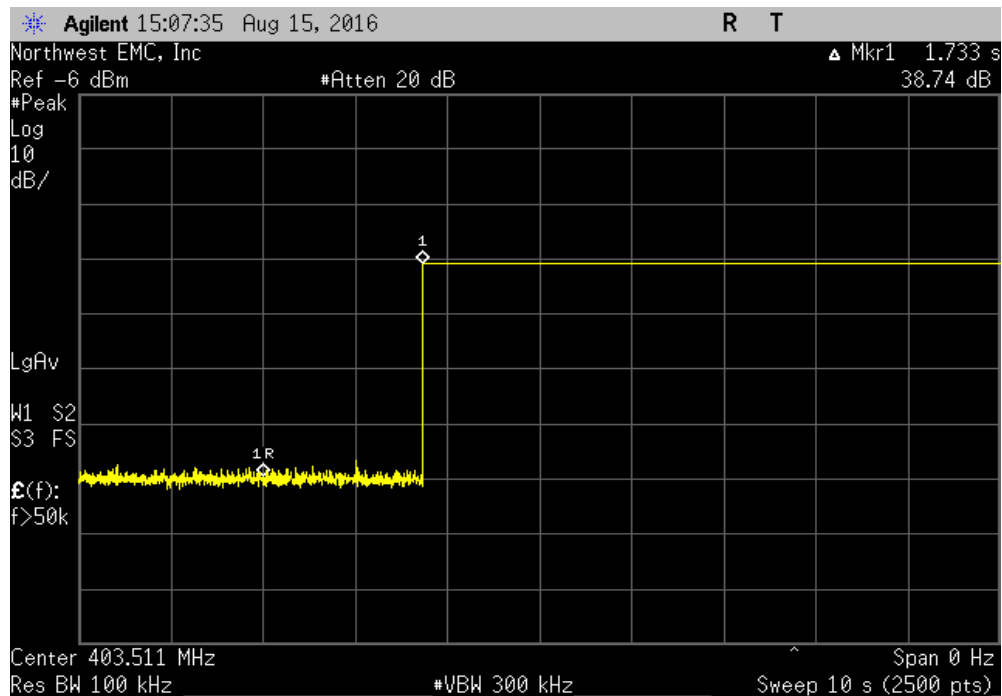

MONITORING SYSTEM SCAN CYCLE TIME, 2 CHANNEL

**NORTHWEST
EMC**

XMit 2016.05.06

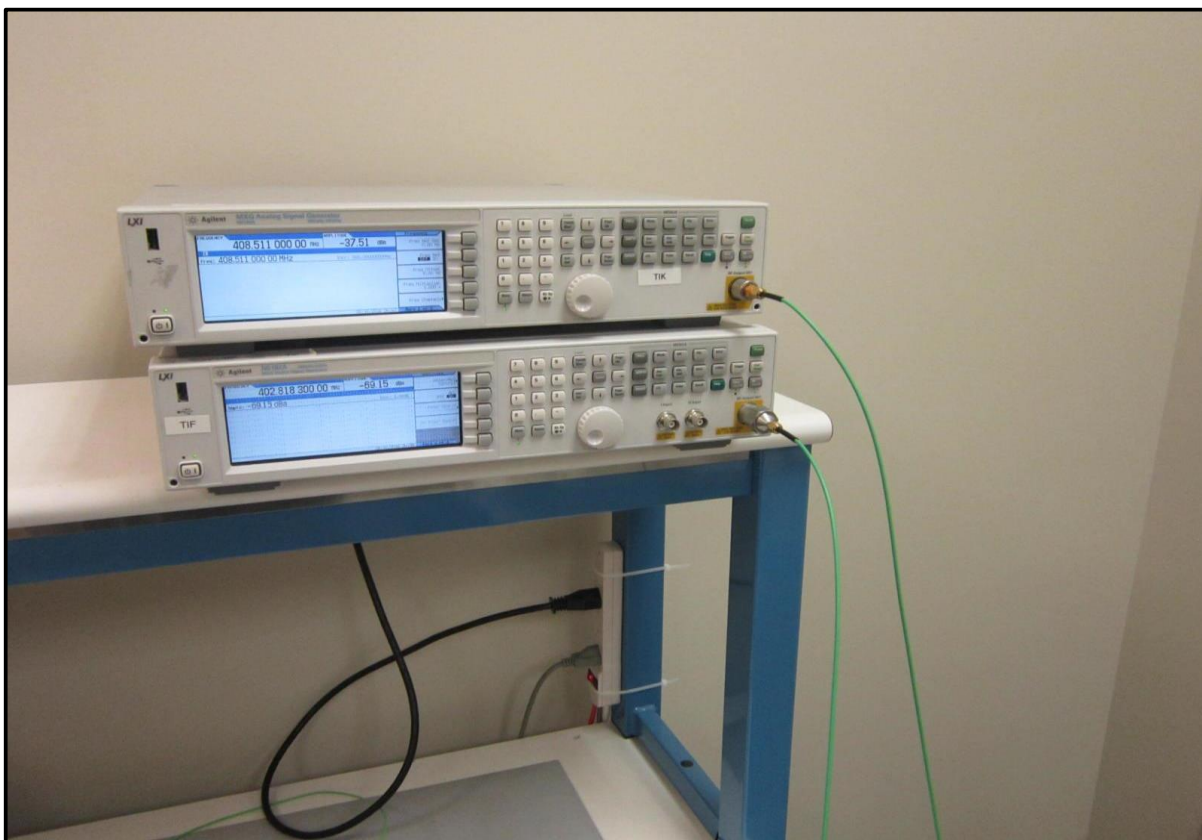

MONITORING SYSTEM SCAN CYCLE TIME, 2 CHANNEL

**NORTHWEST
EMC**

XMit 2016.05.06



MINIMUM CHANNEL MONITORING PERIOD, 10 CHANNEL

Testing was performed using the mode(s) of operation and configuration(s) noted within the report. The individuals and/or the organization requesting the test provided the modes, configurations and settings used to complete the evaluation. The actual test parameters are specified in the test data, this includes items such as investigated frequency range (scanned) and test levels. The testing methods and performance specifications, as well as the test site used for the evaluation are indicated in the test data.

TEST EQUIPMENT


Description	Manufacturer	Model	ID	Last Cal.	Cal. Due
Block - DC	Fairview Microwave	SD3379	AMI	9/18/2015	9/18/2016
Probe - Near Field Set	ETS Lindgren	7405	IPO	NCR	NCR
Generator - Signal	Agilent	N5182A	TIF	8/12/2014	8/12/2017
Generator - Signal	Agilent	E4422B	TGQ	3/17/2015	3/17/2018
Power Divider/Combiner	Fairview Microwave Inc (SM electronics)	MP8451-2	IAD	NCR	NCR
Power Divider/Combiner	Fairview Microwave Inc (SM electronics)	MP8451-2	IAC	NCR	NCR
Directional Coupler	Fairview Microwave	SMC4039-10	RGS	NCR	NCR
Attenuator	S.M. Electronics	SA26B-20	RFW	2/26/2016	2/26/2017
Analyzer - Spectrum Analyzer	Agilent	E4440A	AAX	3/24/2016	3/24/2017

TEST DESCRIPTION

The measurement was made using a direct connection between the RF output of the EUT and a spectrum analyzer. The EUT was configured according to the following block diagram:

The signal generator was set to multitone operation to cause equal interference across the entire band, except one channel (Fc) was left available. The multitone operation (out of operation region) was also set to Pulse modulation with a Period of 10 mS, and a Pulse Width of 0.1 mS. The spectrum analyzer was set to measure the transmit band of 402-405 MHz.

The EUT was set to seek a session with the implantable device. The EUT was verified to connect on the available channel with multiple screen captures.

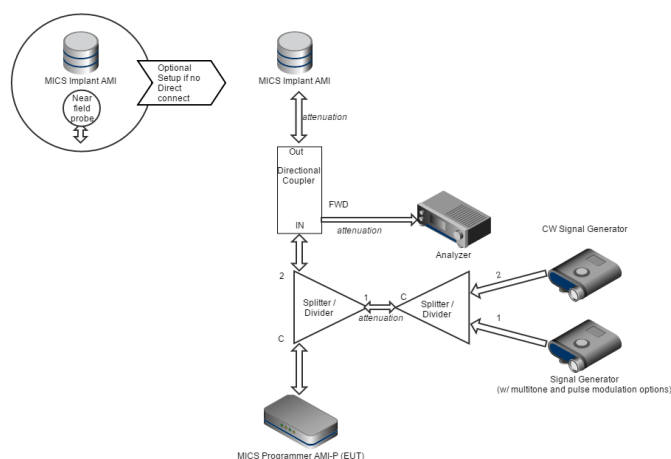


MINIMUM CHANNEL MONITORING PERIOD, 10 CHANNEL


EUT: Model 3300		Work Order: BSTN0663	
Serial Number: 058		Date: 08/25/16	
Customer: Boston Scientific Corporation		Temperature: 22.1 °C	
Attendees: Pete Musto		Humidity: 51.8% RH	
Project: Laramie Vision		Barometric Pres.: 1020 mbar	
Tested by: Trevor Buls	Power: 220VAC/60Hz	Job Site: MN08	
TEST SPECIFICATIONS		Test Method	
EN 301 839 V2.1.1:2016		EN 301 839 V2.1.1:2016	
COMMENTS			
EUT bandwidth is 300000 Hz with an antenna gain of 2.7 dBi.			
DEVIATIONS FROM TEST STANDARD			
None			
Configuration #	11	Signature <i>Trevor Buls</i>	
		Transmits On Fc	Limit Result
Sample 1		Yes	Pass
Sample 2		Yes	Pass
Sample 3		Yes	Pass
Sample 4		Yes	Pass
Sample 5		Yes	Pass
Sample 6		Yes	Pass
Sample 7		Yes	Pass
Sample 8		Yes	Pass
Sample 9		Yes	Pass
Sample 10		Yes	Pass

MINIMUM CHANNEL MONITORING PERIOD, 10 CHANNEL

Sample 1						
				Transmits	Limit	Result
				On Fc		
				Yes	Yes	Pass

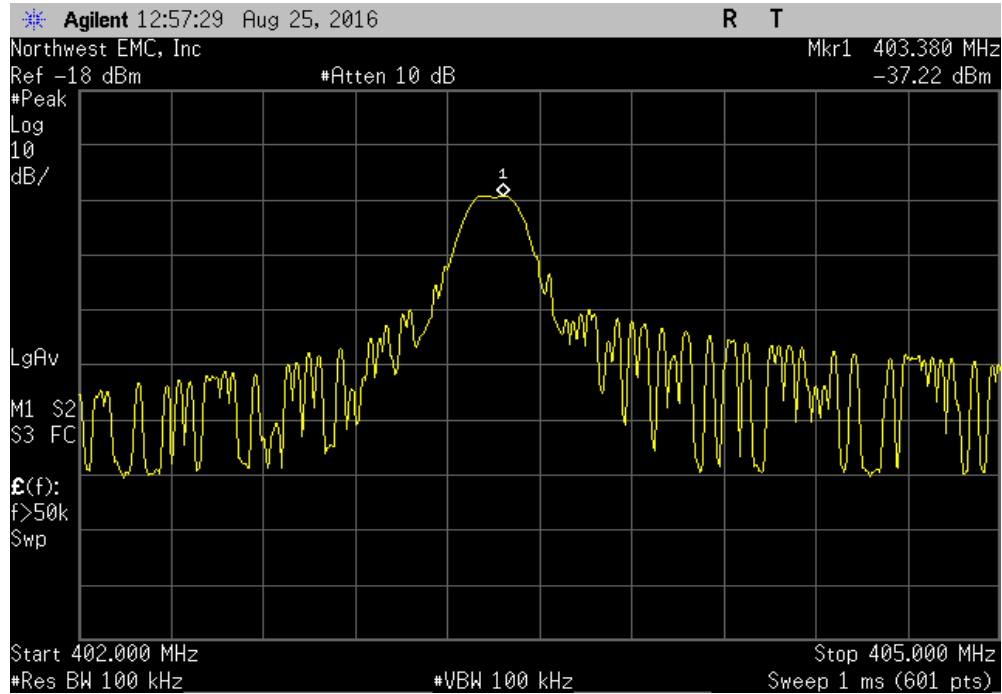


Sample 2						
				Transmits	Limit	Result
				On Fc		
				Yes	Yes	Pass

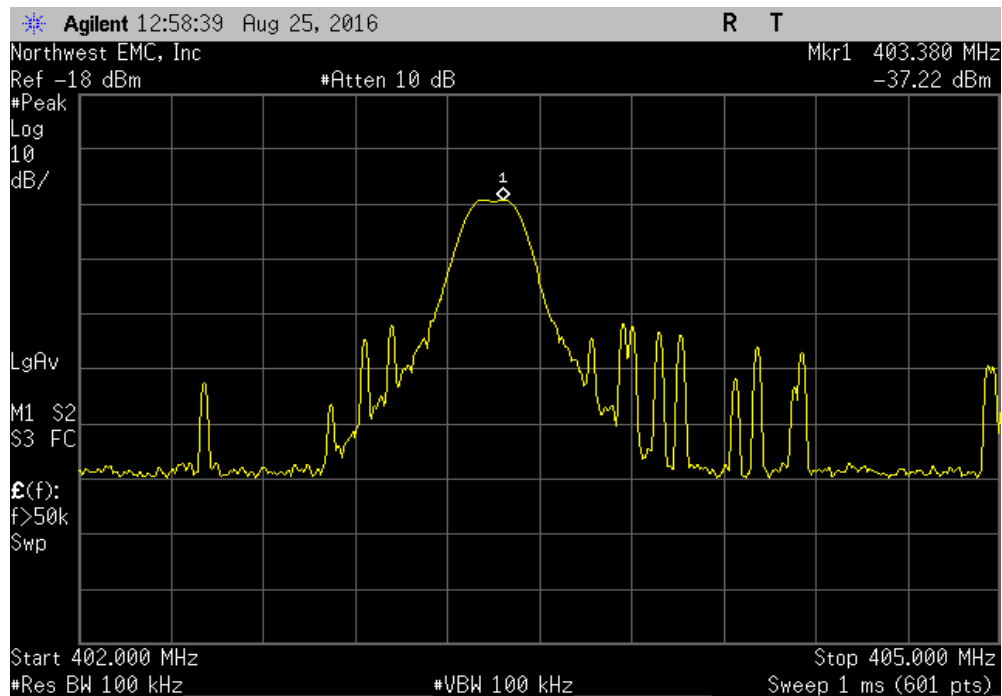


MINIMUM CHANNEL MONITORING PERIOD, 10 CHANNEL

Sample 3						
				Transmits	Limit	Result
				On Fc	Yes	Pass

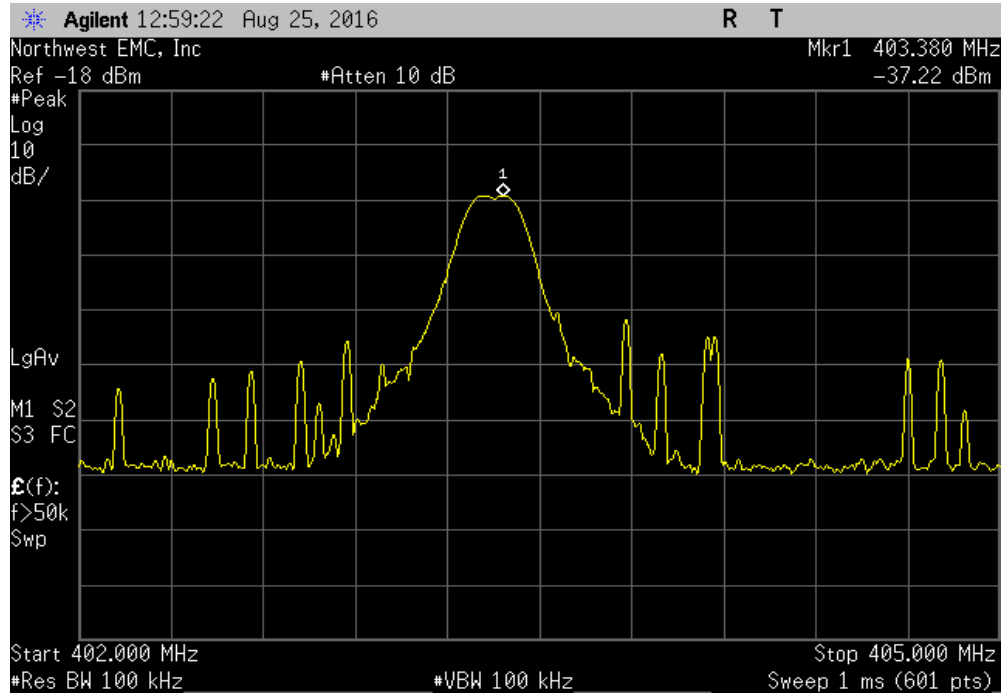


Sample 4						
				Transmits	Limit	Result
				On Fc	Yes	Pass

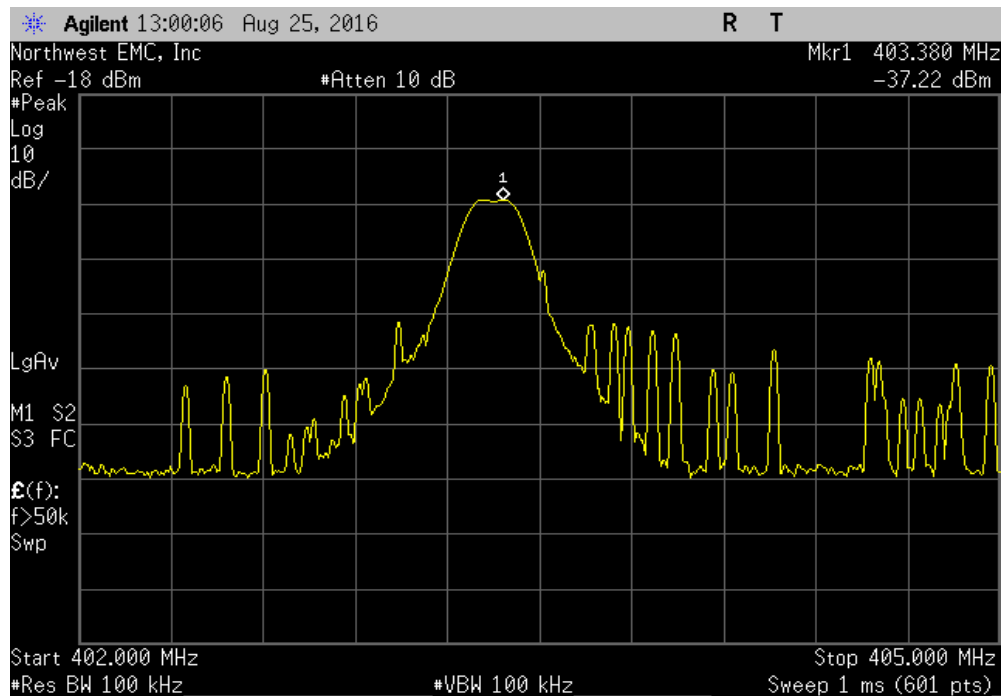


MINIMUM CHANNEL MONITORING PERIOD, 10 CHANNEL

Sample 5						
				Transmits	Limit	Result
				On Fc		
				Yes	Yes	Pass

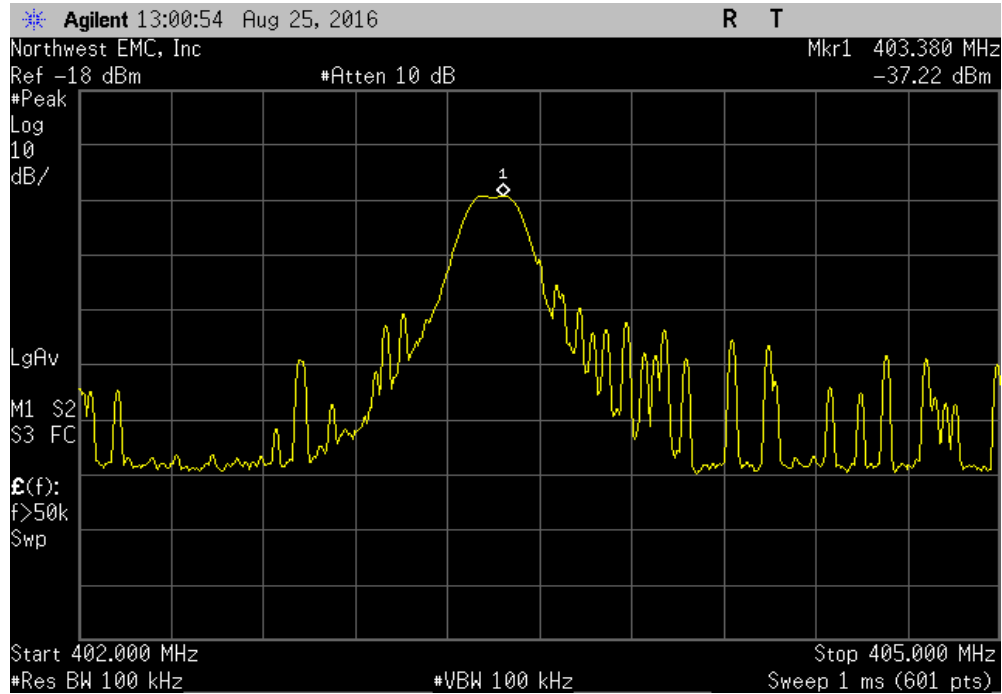


Sample 6						
				Transmits	Limit	Result
				On Fc		
				Yes	Yes	Pass

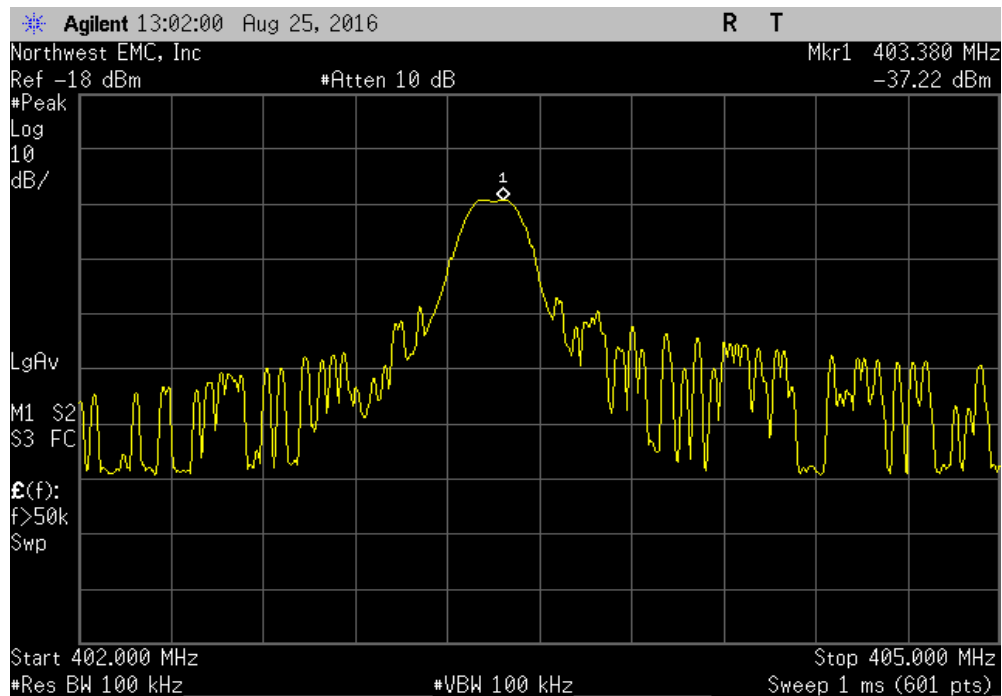


MINIMUM CHANNEL MONITORING PERIOD, 10 CHANNEL

Sample 7						
				Transmits	Limit	Result
				On Fc	Yes	Pass

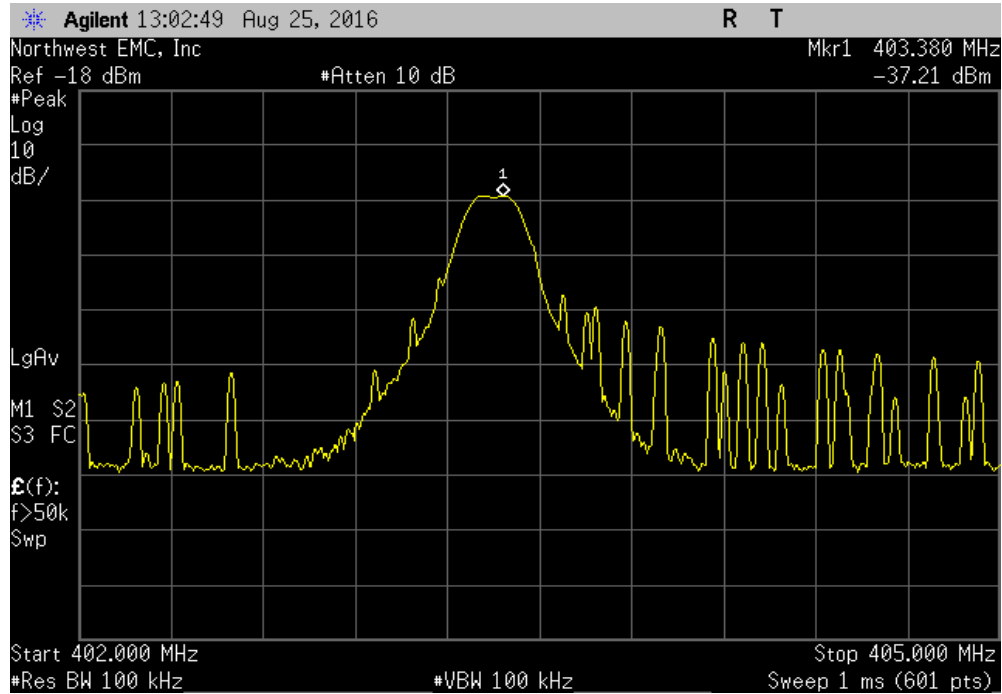


Sample 8						
				Transmits	Limit	Result
				On Fc	Yes	Pass

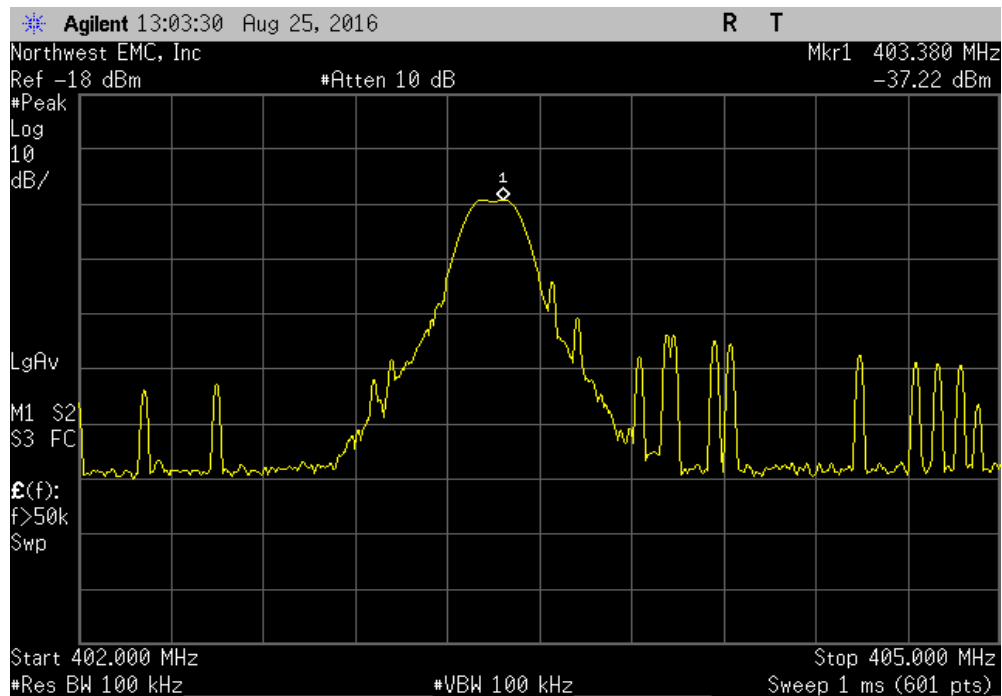


MINIMUM CHANNEL MONITORING PERIOD, 10 CHANNEL



Sample 9					Transmits		
					On Fc	Limit	Result
					Yes	Yes	Pass

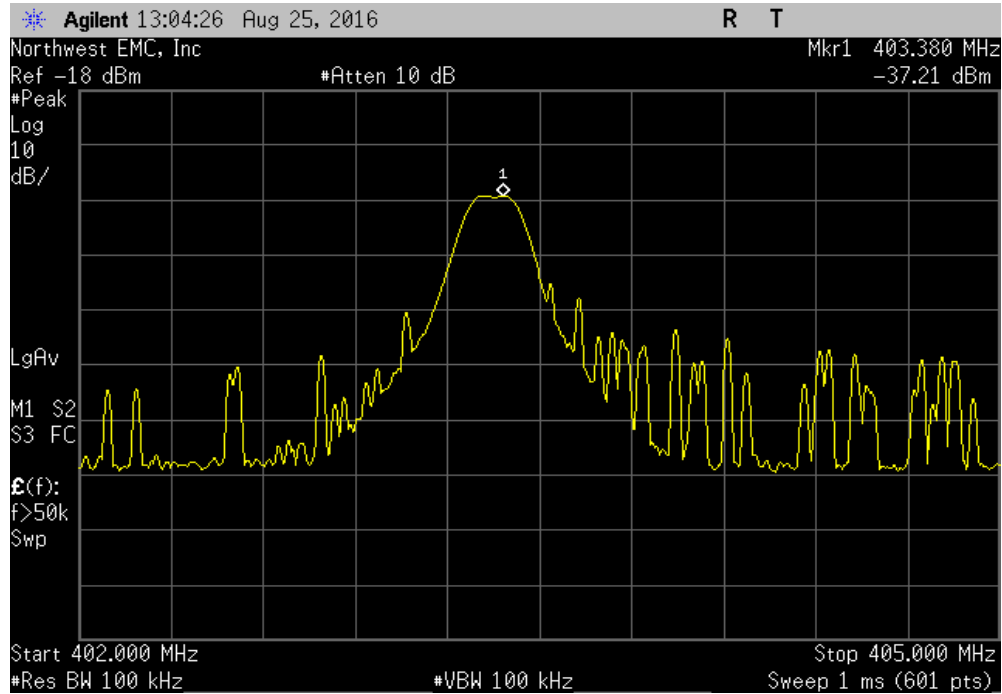

Sample 10					Transmits		
					On Fc	Limit	Result
					Yes	Yes	Pass

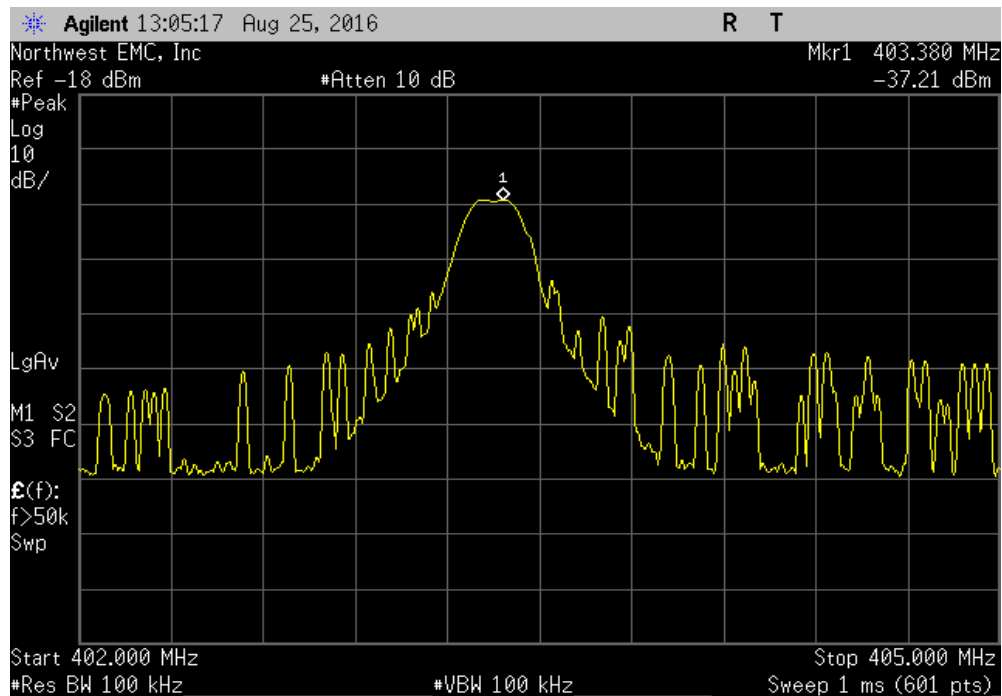

MINIMUM CHANNEL MONITORING PERIOD, 10 CHANNEL

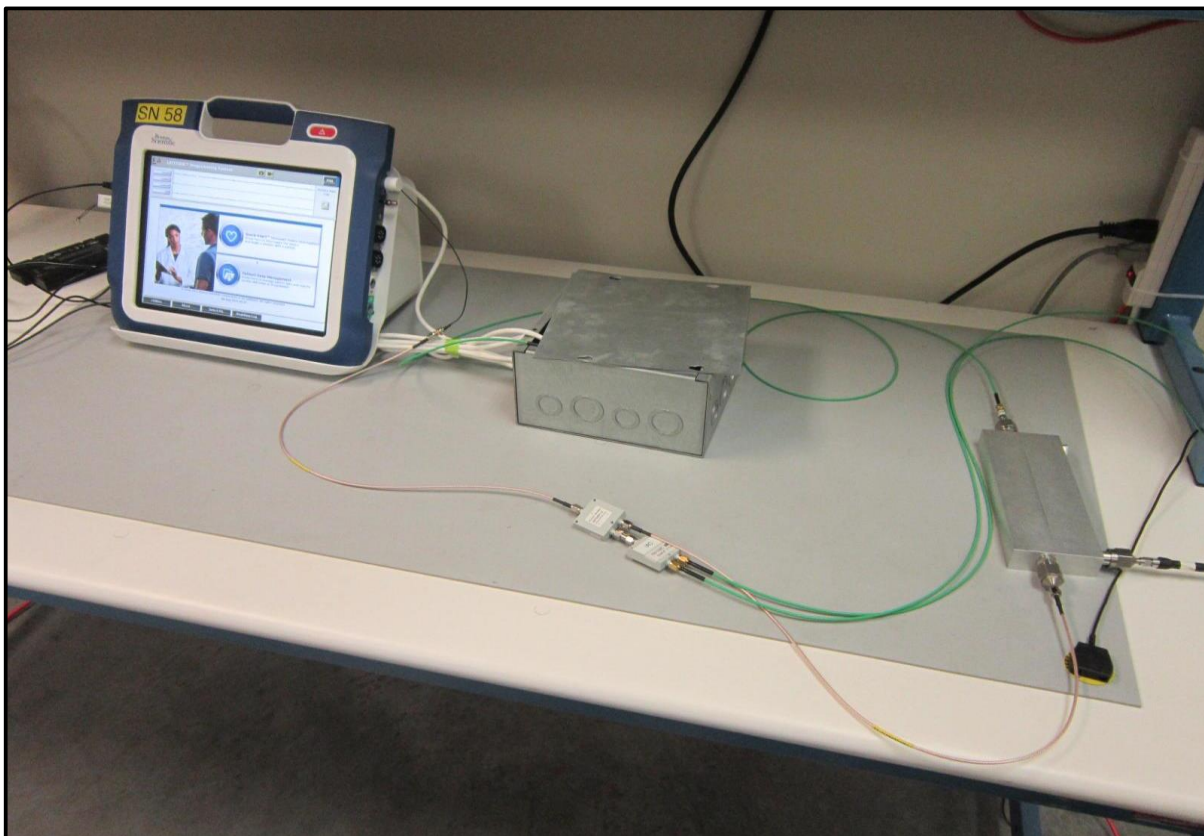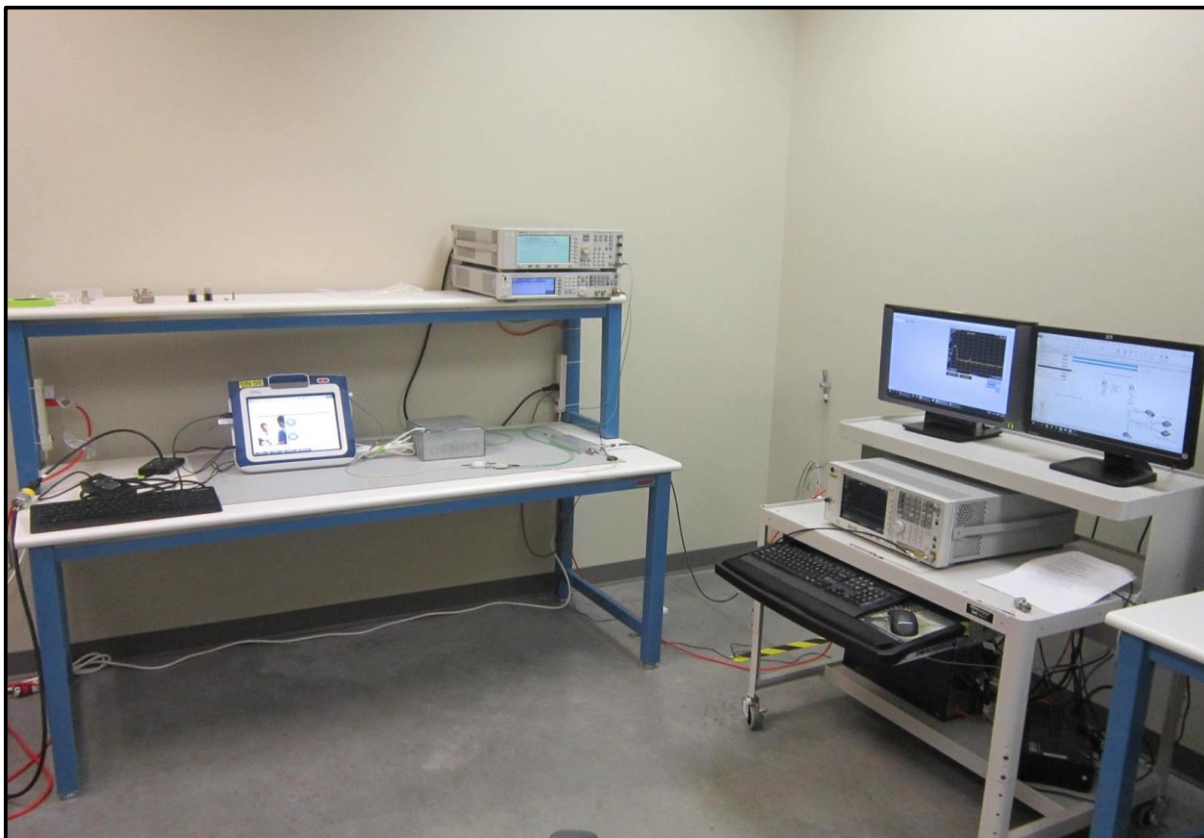

MINIMUM CHANNEL MONITORING PERIOD, 2 CHANNEL

Testing was performed using the mode(s) of operation and configuration(s) noted within the report. The individuals and/or the organization requesting the test provided the modes, configurations and settings used to complete the evaluation. The actual test parameters are specified in the test data, this includes items such as investigated frequency range (scanned) and test levels. The testing methods and performance specifications, as well as the test site used for the evaluation are indicated in the test data.

TEST EQUIPMENT


Description	Manufacturer	Model	ID	Last Cal.	Cal. Due
Block - DC	Fairview Microwave	SD3379	AMI	9/18/2015	9/18/2016
Probe - Near Field Set	ETS Lindgren	7405	IPO	NCR	NCR
Generator - Signal	Agilent	N5182A	TIF	8/12/2014	8/12/2017
Generator - Signal	Agilent	E4422B	TGQ	3/17/2015	3/17/2018
Power Divider/Combiner	Fairview Microwave Inc (SM electronics)	MP8451-2	IAD	NCR	NCR
Power Divider/Combiner	Fairview Microwave Inc (SM electronics)	MP8451-2	IAC	NCR	NCR
Directional Coupler	Fairview Microwave	SMC4039-10	RGS	NCR	NCR
Attenuator	S.M. Electronics	SA26B-20	RFW	2/26/2016	2/26/2017
Analyzer - Spectrum Analyzer	Agilent	E4440A	AAX	3/24/2016	3/24/2017

TEST DESCRIPTION

The measurement was made using a direct connection between the RF output of the EUT and a spectrum analyzer. The EUT was configured according to the following block diagram:

The signal generator was set to multitone operation to cause equal interference across the entire band, except one channel (Fc) was left available. The multitone operation (out of operation region) was also set to Pulse modulation with a Period of 10 mS, and a Pulse Width of 0.1 mS. The spectrum analyzer was set to measure the transmit band of 402-405 MHz.

The EUT was set to seek a session with the implantable device. The EUT was verified to connect on the available channel with multiple screen captures.

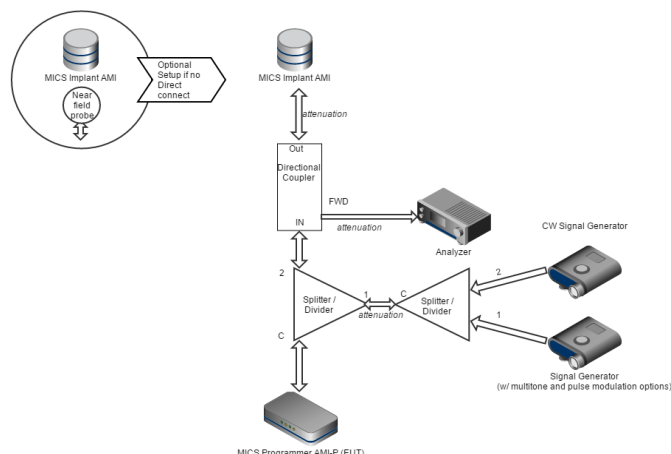

MINIMUM CHANNEL MONITORING PERIOD, 2 CHANNEL




XMR 2016.05.06


EUT: Model 3300		Work Order: BSTN0663	
Serial Number: 058		Date: 08/25/16	
Customer: Boston Scientific Corporation		Temperature: 22.1 °C	
Attendees: Pete Musto		Humidity: 51.8% RH	
Project: Laramie Vision		Barometric Pres.: 1020 mbar	
Tested by: Trevor Buls	Power: 220VAC/60Hz	Job Site: MN08	
TEST SPECIFICATIONS		Test Method	
EN 301 839 V2.1.1:2016		EN 301 839 V2.1.1:2016	
COMMENTS			
EUT bandwidth is 300000 Hz with an antenna gain of -5 dBi.			
DEVIATIONS FROM TEST STANDARD			
None			
Configuration #	12	Signature <i>Trevor Buls</i>	
		Transmits On Fc	Limit Result
Sample 1		Yes	Pass
Sample 2		Yes	Pass
Sample 3		Yes	Pass
Sample 4		Yes	Pass
Sample 5		Yes	Pass
Sample 6		Yes	Pass
Sample 7		Yes	Pass
Sample 8		Yes	Pass
Sample 9		Yes	Pass
Sample 10		Yes	Pass

MINIMUM CHANNEL MONITORING PERIOD, 2 CHANNEL

Sample 1						
				Transmits	Limit	Result
				On Fc		
				Yes	Yes	Pass

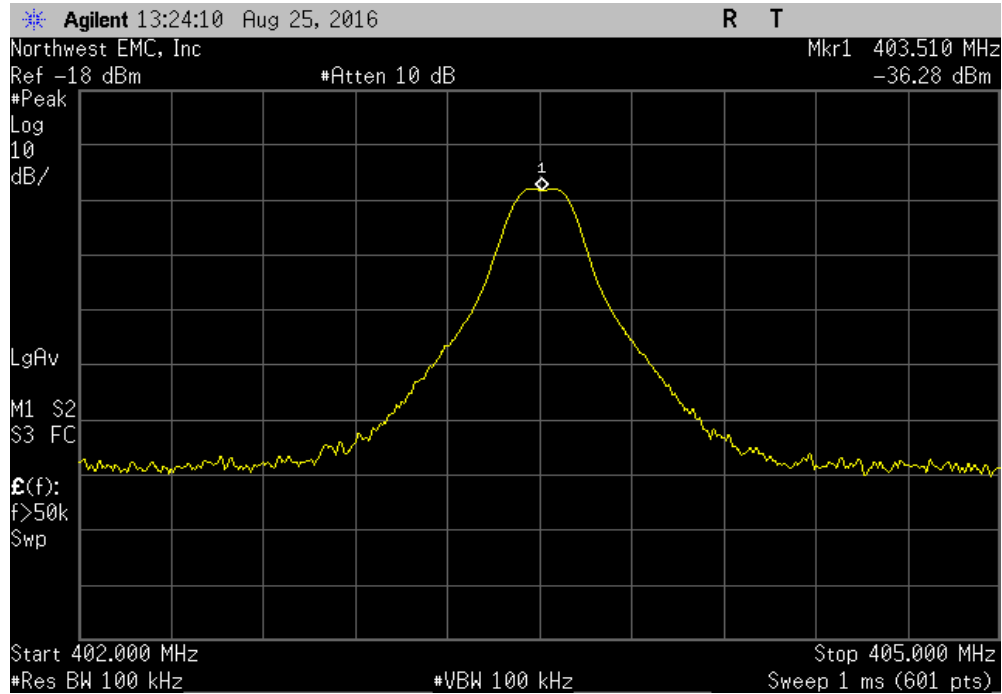


Sample 2						
				Transmits	Limit	Result
				On Fc		
				Yes	Yes	Pass

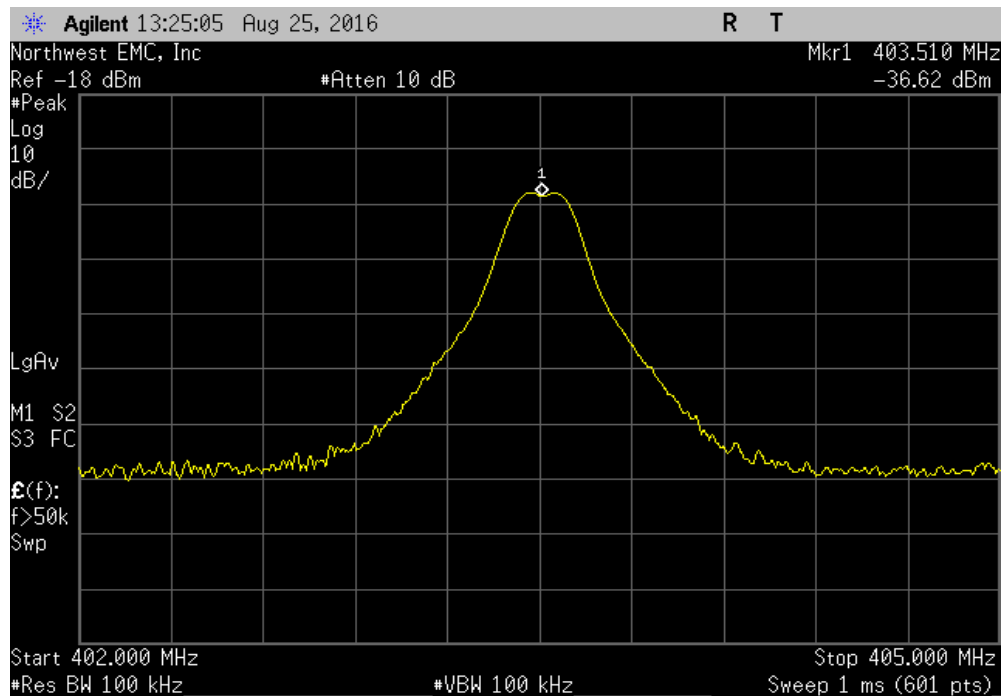


MINIMUM CHANNEL MONITORING PERIOD, 2 CHANNEL

Sample 3						
				Transmits	Limit	Result
				On Fc	Yes	Pass

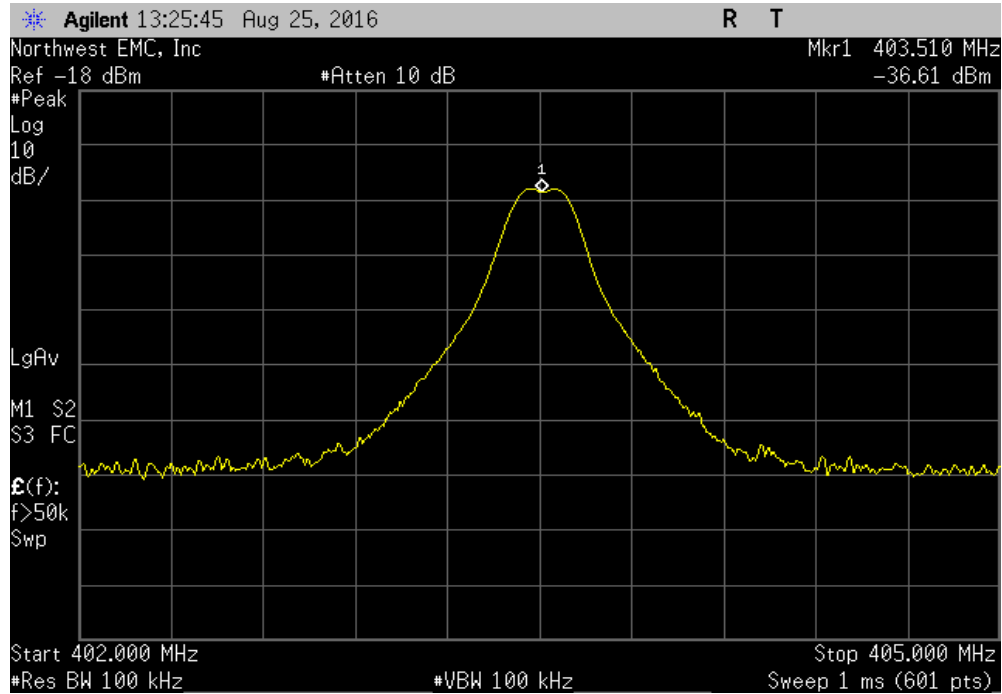


Sample 4						
				Transmits	Limit	Result
				On Fc	Yes	Pass

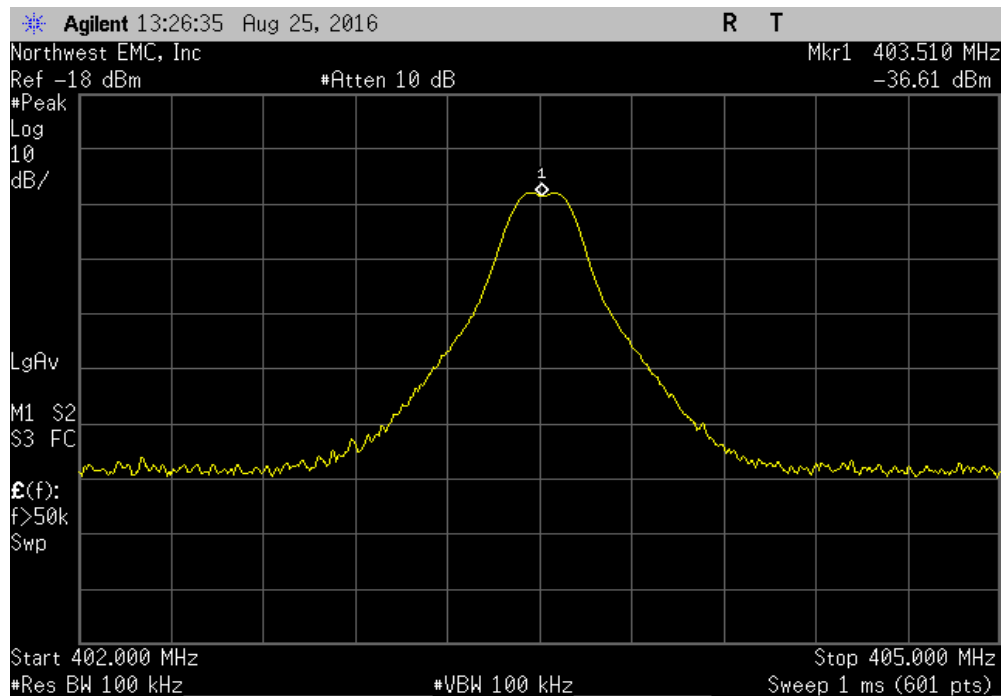


MINIMUM CHANNEL MONITORING PERIOD, 2 CHANNEL

Sample 5						
				Transmits On Fc	Limit	Result
				Yes	Yes	Pass

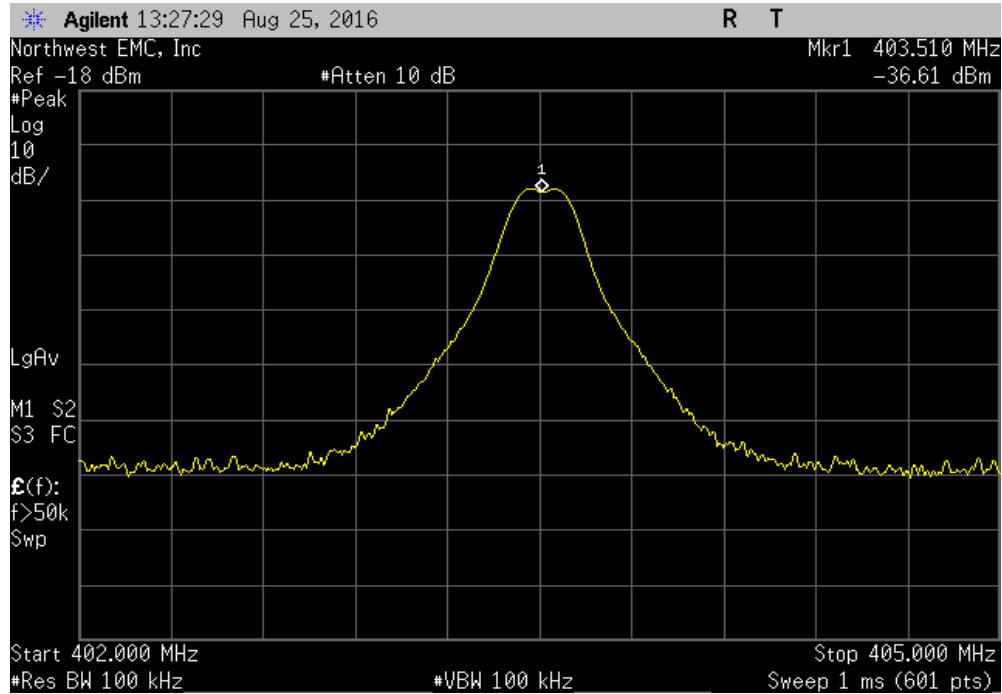


Sample 6						
				Transmits On Fc	Limit	Result
				Yes	Yes	Pass

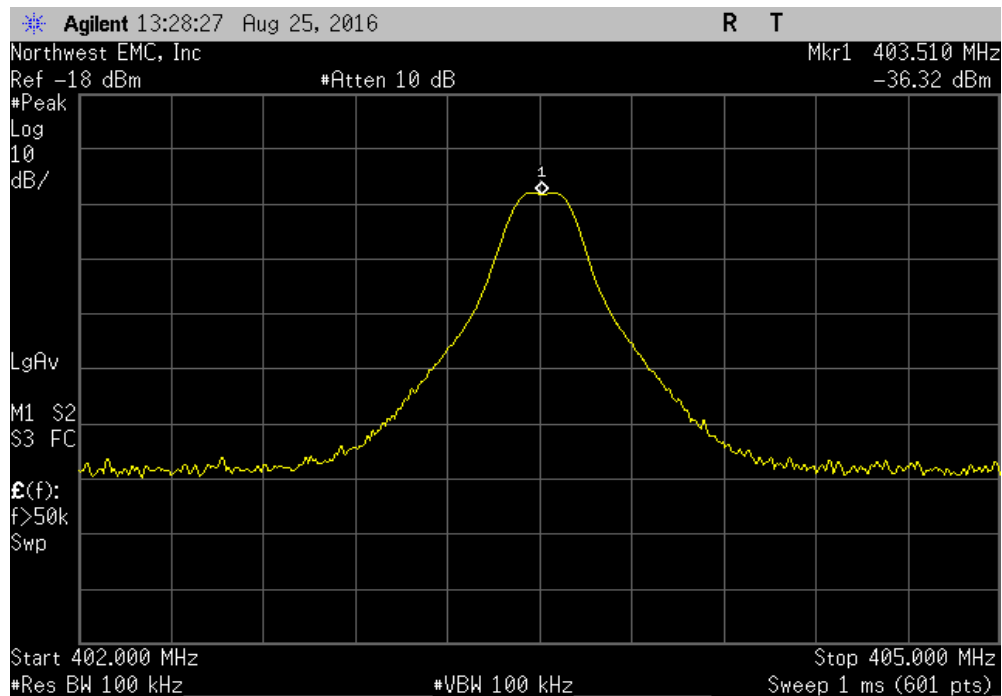


MINIMUM CHANNEL MONITORING PERIOD, 2 CHANNEL

Sample 7						
				Transmits On Fc	Limit	Result
				Yes	Yes	Pass

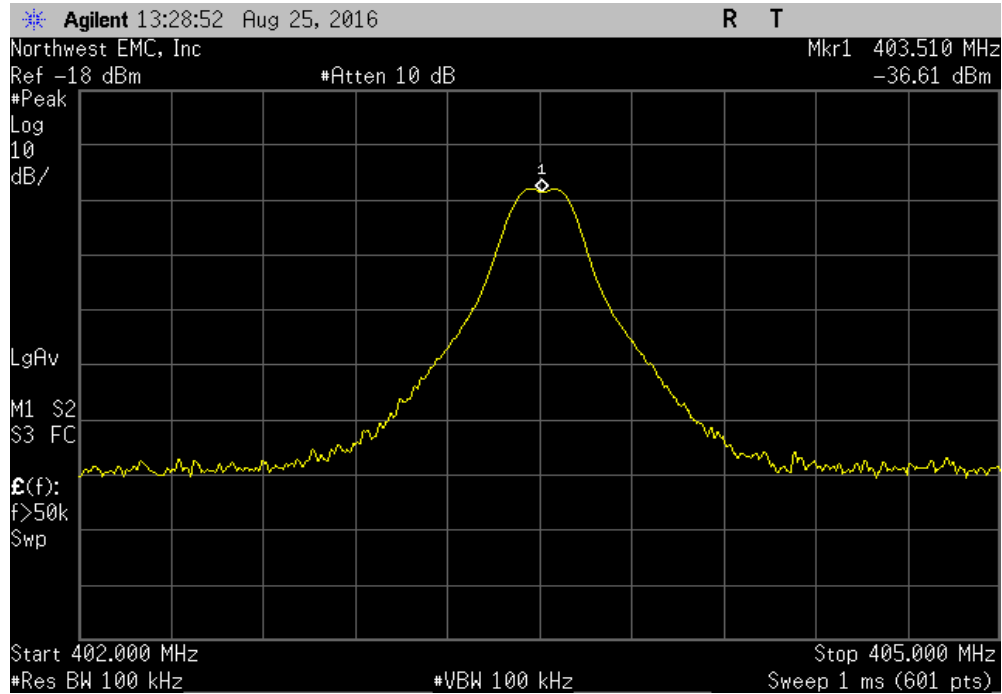


Sample 8						
				Transmits On Fc	Limit	Result
				Yes	Yes	Pass

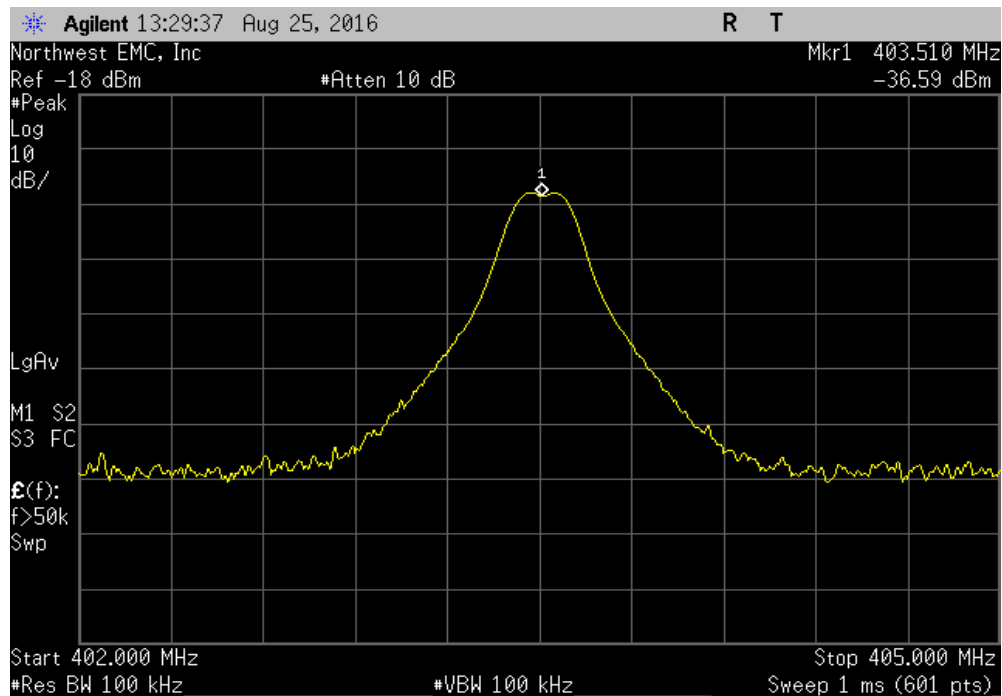


MINIMUM CHANNEL MONITORING PERIOD, 2 CHANNEL



Sample 9						
				Transmits	Limit	Result
				On Fc	Yes	Pass

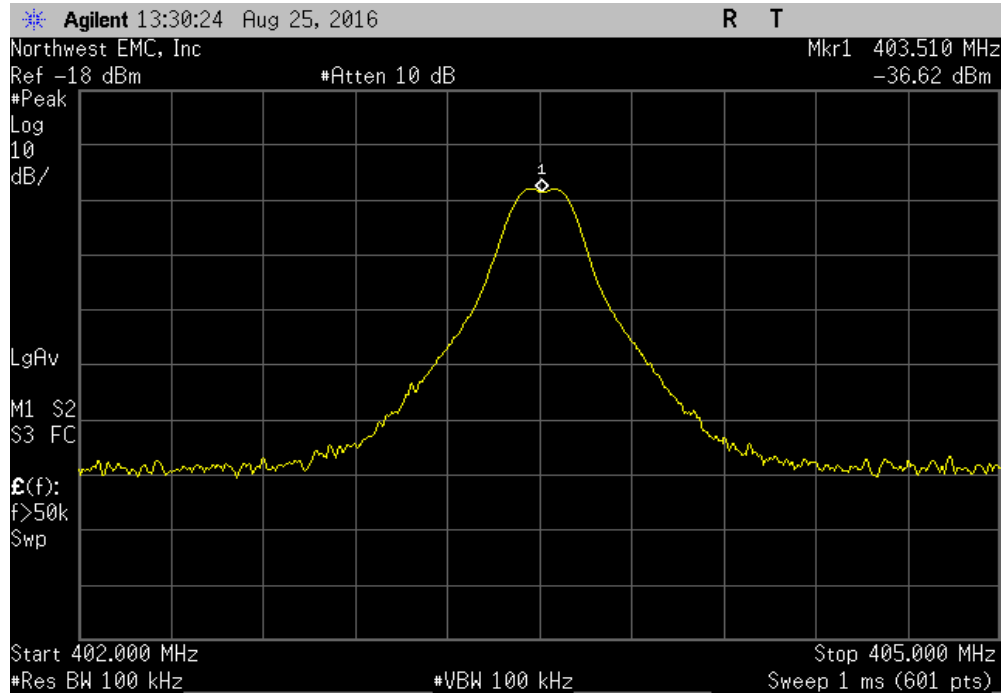

Sample 10						
				Transmits	Limit	Result
				On Fc	Yes	Pass

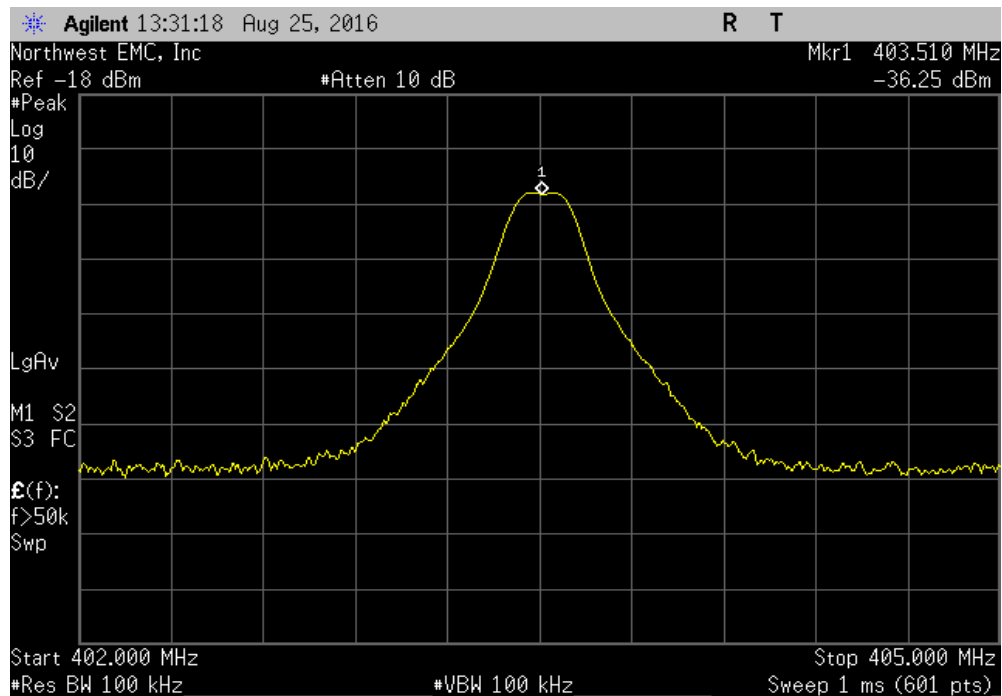

MINIMUM CHANNEL MONITORING PERIOD, 2 CHANNEL

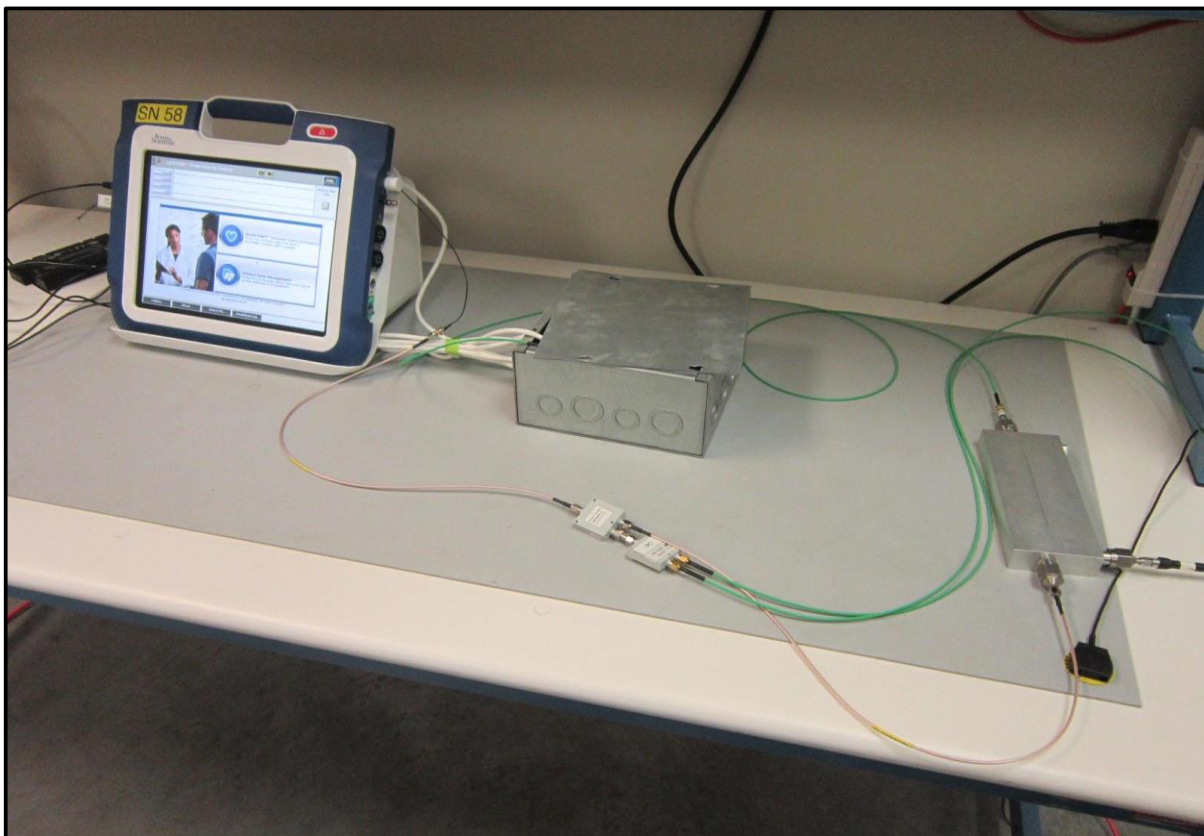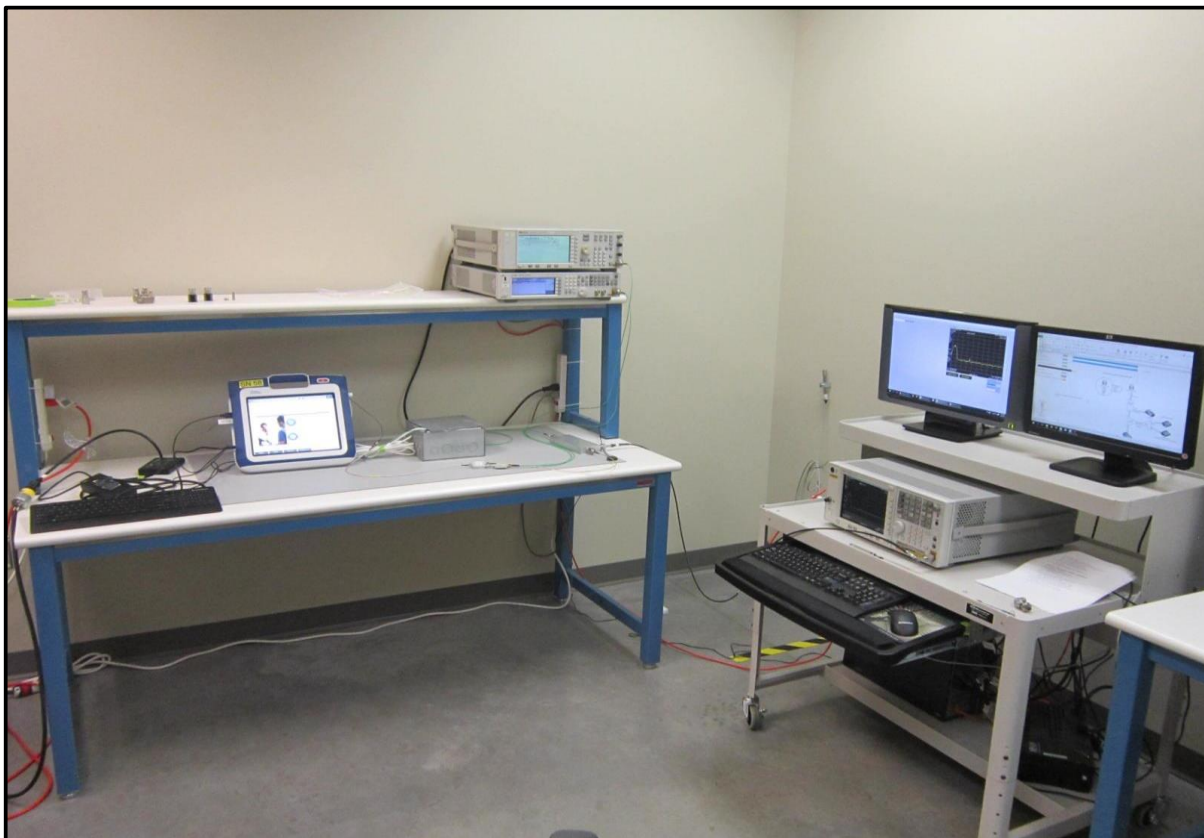

CHANNEL ACCESS BASED ON AMBIENT LEVELS, 10 CHANNEL

Testing was performed using the mode(s) of operation and configuration(s) noted within the report. The individuals and/or the organization requesting the test provided the modes, configurations and settings used to complete the evaluation. The actual test parameters are specified in the test data, this includes items such as investigated frequency range (scanned) and test levels. The testing methods and performance specifications, as well as the test site used for the evaluation are indicated in the test data.

TEST EQUIPMENT

Description	Manufacturer	Model	ID	Last Cal.	Cal. Due
Probe - Near Field Set	ETS Lindgren	7405	IPO	NCR	NCR
Directional Coupler	Fairview Microwave	SMC4039-10	RGS	NCR	NCR
Power Divider/Combiner	Fairview Microwave Inc (SM electronics)	MP8451-2	IAD	NCR	NCR
Power Divider/Combiner	Fairview Microwave Inc (SM electronics)	MP8451-2	IAC	NCR	NCR
Generator - Signal	Agilent	N5182A	TIF	8/12/2014	8/12/2017
Generator - Signal	Agilent	E4422B	TGQ	3/17/2015	3/17/2018
Cable	ESM Cable Corp.	TTBJ141 KMKM-72	MNU	9/18/2015	9/18/2016
Block - DC	Fairview Microwave	SD3379	AMI	9/18/2015	9/18/2016
Analyzer - Spectrum Analyzer	Agilent	E4440A	AAX	3/24/2016	3/24/2017


TEST DESCRIPTION

A near-field probe was placed near the transmitter. A low-loss coaxial cable was used to connect the near-field probe to the spectrum analyzer. The EUT was configured according to the following block diagram:

The signal generator was set to multitone operation to cause equal interference across the entire band. The amplitude of the multitone signals (out of operation region) were set to the LBT threshold of $10 \cdot \text{LOG}(\text{Bandwidth}) - 150 + \text{Antenna Gain} + 10 \text{ dB}$.

The intended frequency (F_c) was set to the LBT threshold - 3 dB. A least interfered channel (LIC) was set to the LBT threshold + 3 dB. The EUT was verified to transmit on F_c . The amplitude of F_c was then raised to the LBT threshold + 6 dB. The EUT was verified to transmit on LIC.

The spectrum analyzer was set to measure the transmit band of 402-405 MHz. Screen captures were provided to show the EUT behavior at the different LBT threshold levels.

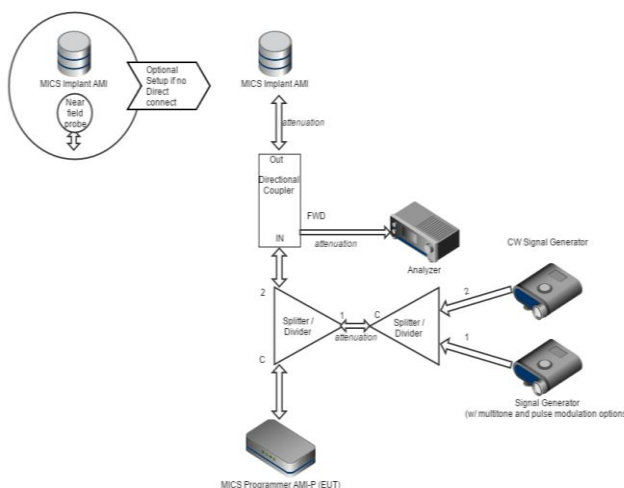


CHANNEL ACCESS BASED ON AMBIENT LEVELS, 10 CHANNEL


EUT: Model 3300		Work Order: BSTN0663	
Serial Number: 058		Date: 08/08/16	
Customer: Boston Scientific Corporation		Temperature: 23.3 °C	
Attendees: Pete Musto		Humidity: 54.2% RH	
Project: Laramie Vision		Barometric Pres.: 1018 mbar	
Tested by: Dustin Sparks	Power: 220VAC/60Hz	Job Site: MN02	
TEST SPECIFICATIONS		Test Method	
EN 301 839 V2.1.1:2016		EN 301 839 V2.1.1:2016	
COMMENTS			
EUT emissions bandwidth is 300000 Hz, 2.7 dBi antenna gain. Antenna port B, PRM application 3869 0.03.13			
DEVIATIONS FROM TEST STANDARD			
None			
Configuration #	7	Signature 	
		Transmit on Fc	Transmit on LIC
Fc LBT Threshold -3dB		Yes	No
Fc LBT Threshold +6dB		No	Yes
		Limit (Tx on LIC?)	Result
		No	Pass
		Yes	Pass

CHANNEL ACCESS BASED ON AMBIENT LEVELS, 10 CHANNEL

Fc LBT Threshold -3dB						
			Transmit on Fc	Transmit on LIC	Limit (Tx on LIC?)	Result
			Yes	No	No	Pass

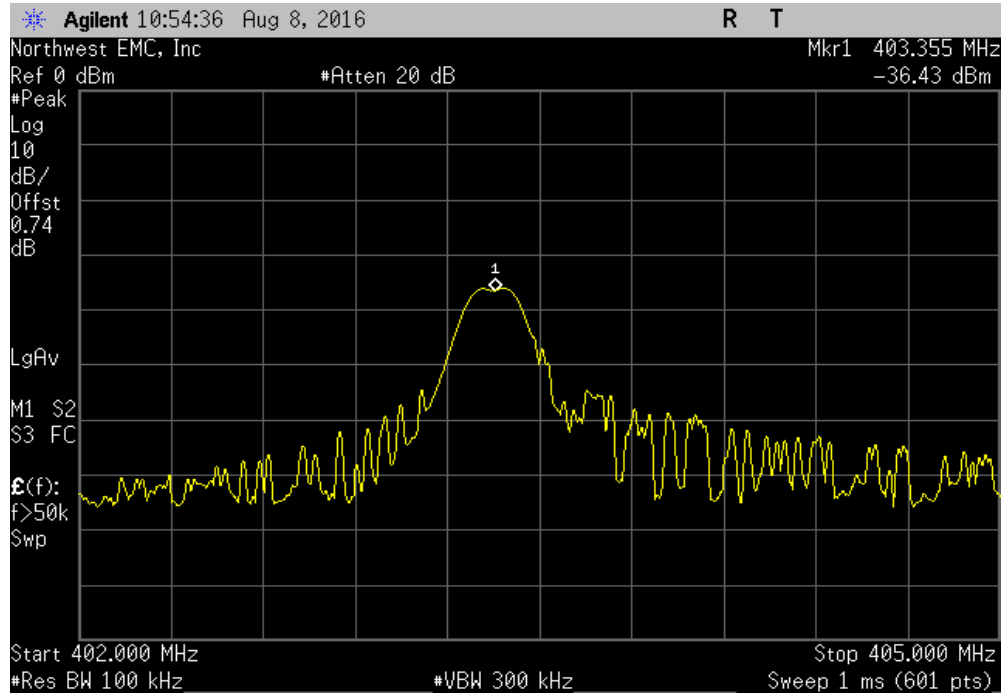



Fc LBT Threshold +6dB						
			Transmit on Fc	Transmit on LIC	Limit (Tx on LIC?)	Result
			No	Yes	Yes	Pass

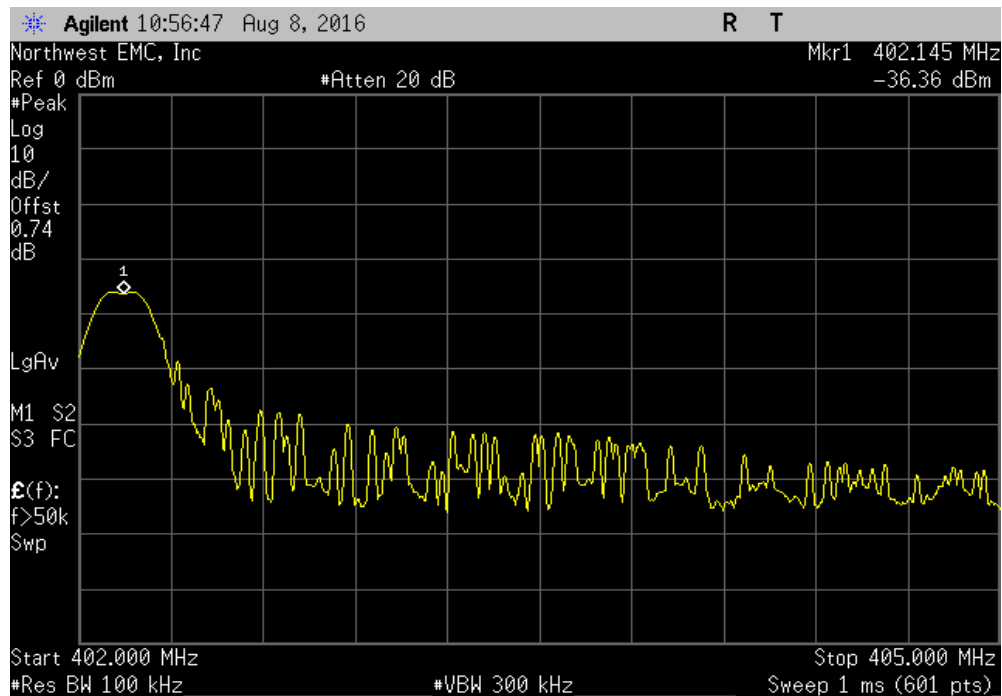

CHANNEL ACCESS BASED ON AMBIENT LEVELS, 10 CHANNEL

**NORTHWEST
EMC**

XMit 2016.05.06

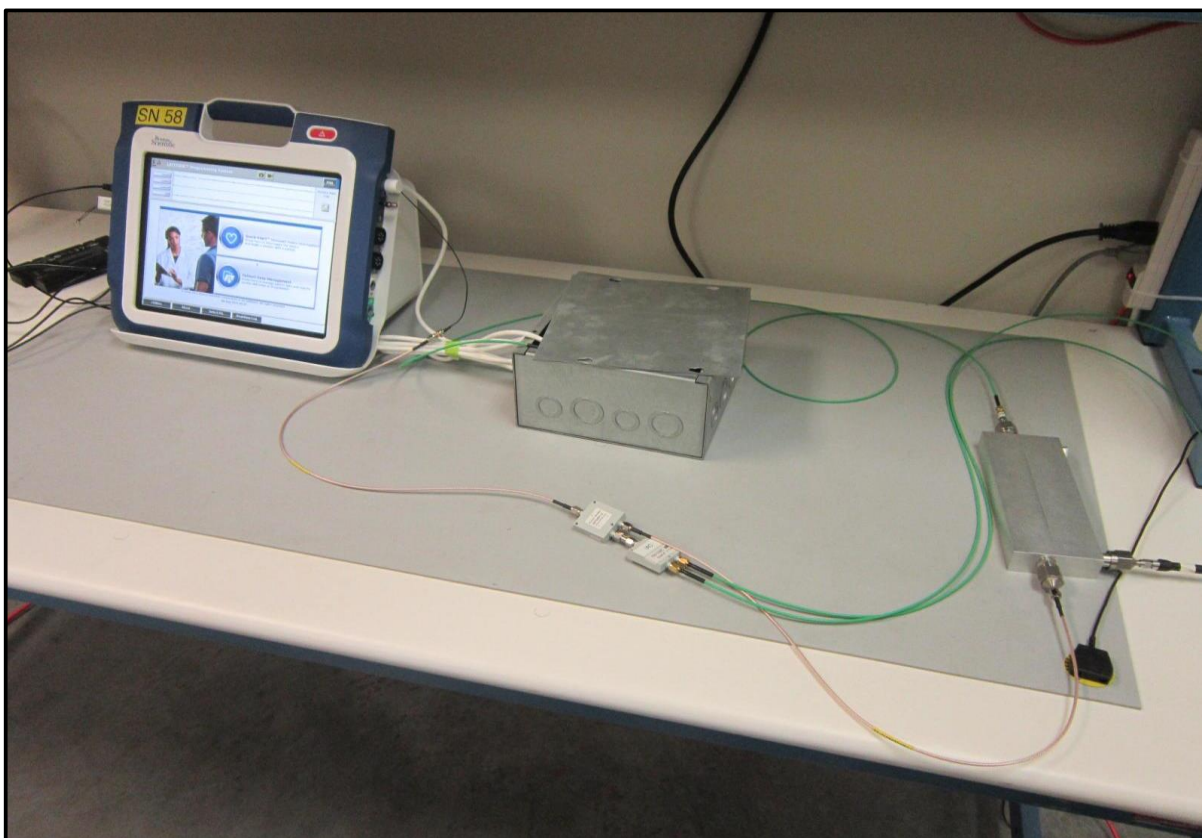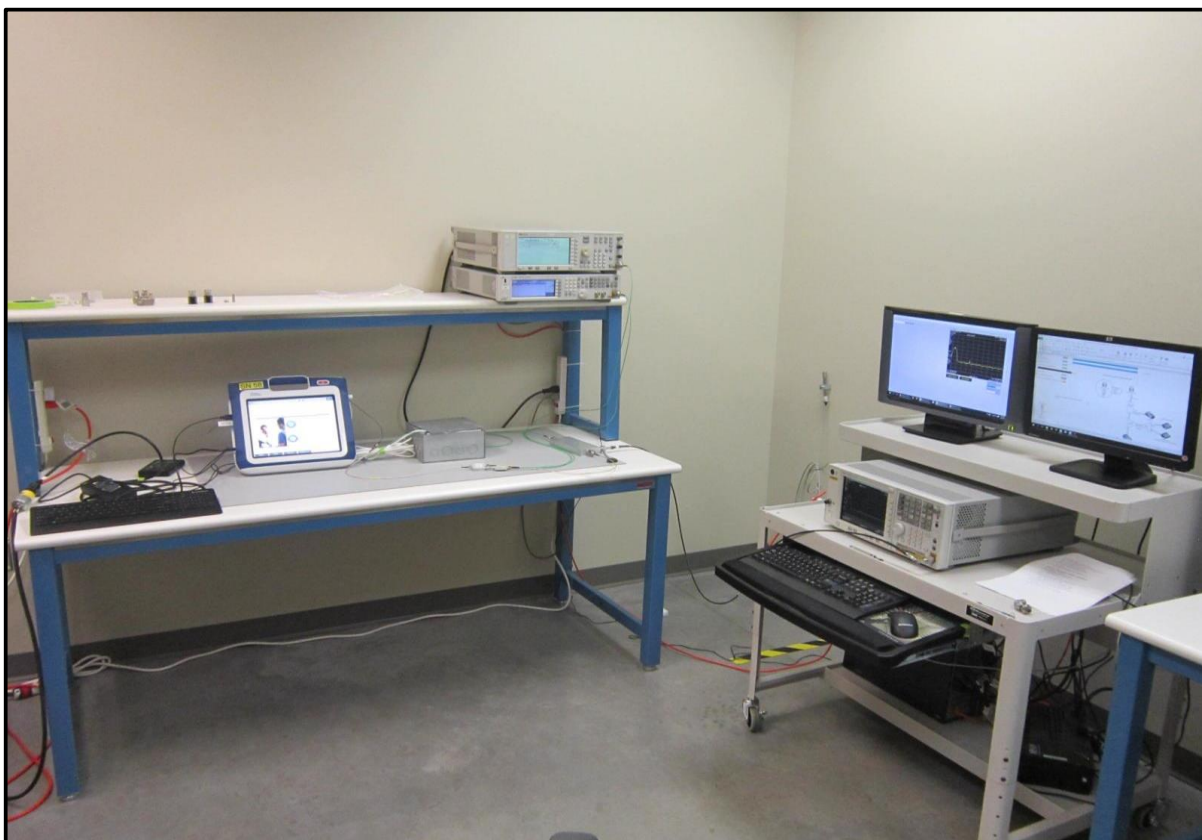

CHANNEL ACCESS BASED ON AMBIENT LEVELS, 10 CHANNEL

