

Validation Data (835MHz Brain)

Dipole 835 MHz

SAM I Phantom; Flat Section; Position: (90°,90°); Frequency: 835 MHz

Probe: ET3DV6 - SN1798; ConvF(6.60,6.60,6.60); Crest factor: 1.0; Brain 835 MHz: $\sigma = 0.88$

mho/m $\epsilon_r = 42.7$ $\rho = 1.00$ g/cm³

Cubes (2): SAR (1g): 9.69 mW/g ± 0.25 dB, SAR (10g): 6.19 mW/g ± 0.25 dB

Coarse: Dx = 20.0, Dy = 20.0, Dz = 10.0

Powerdrift: 0.05 dB

Comment:


835MHz Brain Dipole Validation (D835V2/ S.N: 441)

Antenna Input Power: 30 dBm (1 W)

HCT Co., Ltd. Brain Tissue Simulating Liquid

Liquid Temperature: 21.7 °C

Date Tested : January 26, 2004

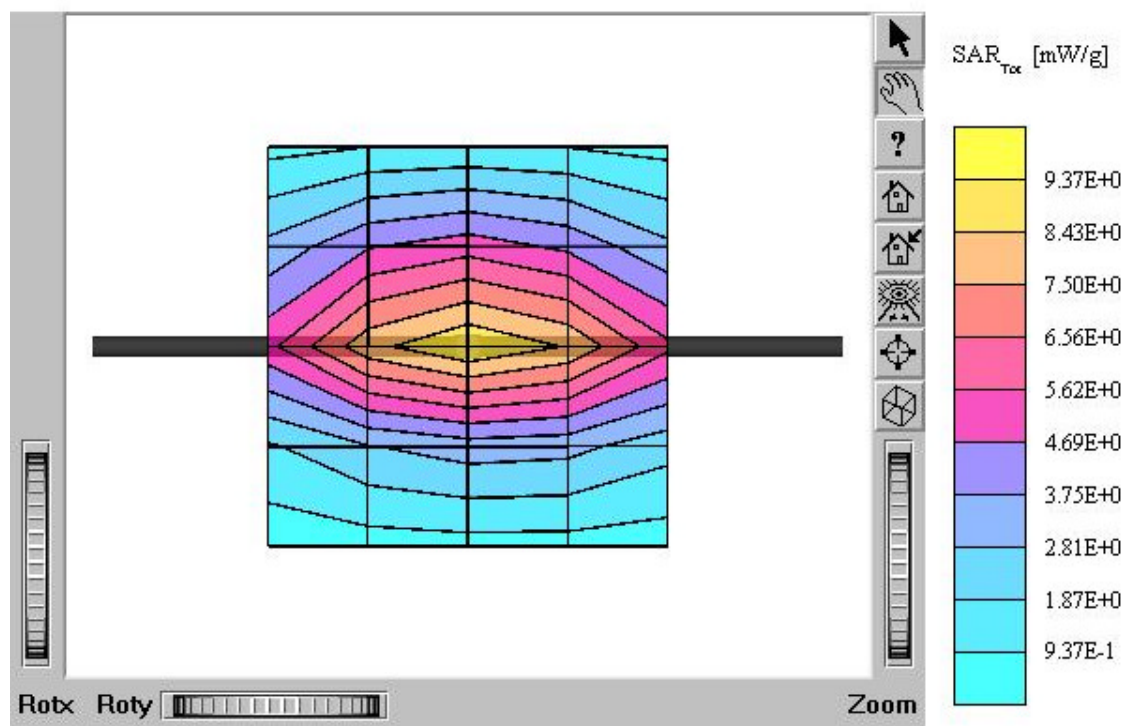

Dipole 835 MHz

SAM I Phantom; Flat Section; Position: (90°,90°); Frequency: 835 MHz

Probe: ET3DV6 - SN1798; ConvF(6.60,6.60,6.60); Crest factor: 1.0; Brain 835 MHz: $\sigma = 0.88$

mho/m $\epsilon_r = 42.7$ $\rho = 1.00$ g/cm³

Cubes (2): SAR (1g): 9.69 mW/g ± 0.25 dB, SAR (10g): 6.19 mW/g ± 0.25 dB

Cube 5x5x7: Dx = 8.0, Dy = 8.0, Dz = 5.0

Comment:


835MHz Brain Dipole Validation (D835V2/ S.N: 441)

Antenna Input Power: 30 dBm (1 W)

HCT Co., Ltd. Brain Tissue Simulating Liquid

Liquid Temperature: 21.7 °C

Date Tested : January 26, 2004

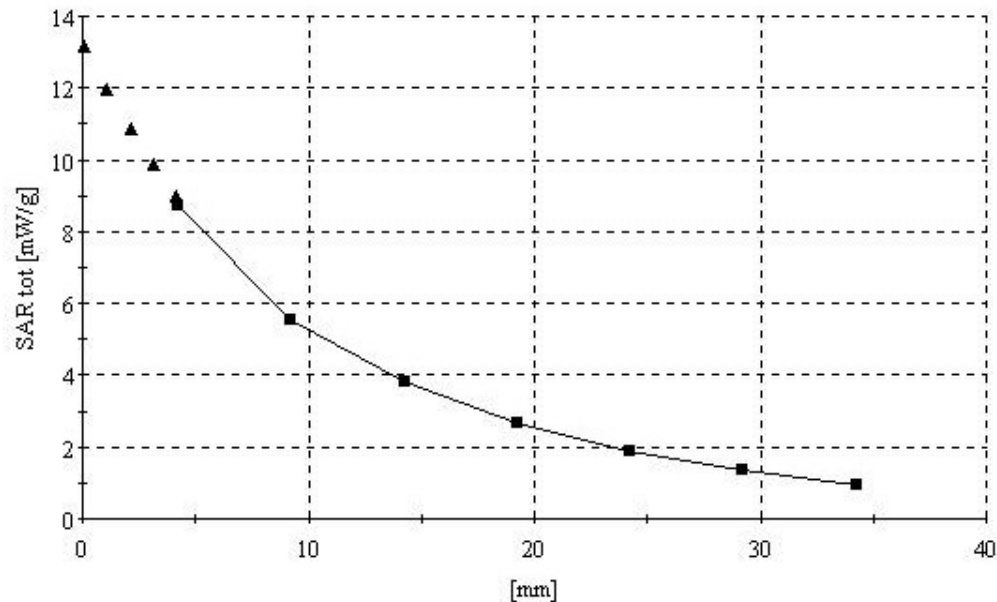

! Dielectric Parameter (835MHz Brain)

Title : XC-101**SubTitle : 835 MHz Brain****January 26, 2004 08:42 AM**

Frequency	e'	e''
800.000000 MHz	43.5392	19.0869
805.000000 MHz	43.4474	19.0257
810.000000 MHz	43.3069	18.9792
815.000000 MHz	43.1951	18.9900
820.000000 MHz	43.0363	18.9238
825.000000 MHz	42.8711	18.9031
830.000000 MHz	42.7729	18.8694
835.000000 MHz	42.7053	18.9012
840.000000 MHz	42.5862	18.8954
845.000000 MHz	42.5373	18.8386
850.000000 MHz	42.4911	18.8956
855.000000 MHz	42.4700	18.8932
860.000000 MHz	42.4589	18.8878
865.000000 MHz	42.5159	18.9031
870.000000 MHz	42.4886	18.9429
875.000000 MHz	42.5012	19.0110
880.000000 MHz	42.5365	19.0512
885.000000 MHz	42.5441	19.0488
890.000000 MHz	42.4985	19.0022
895.000000 MHz	42.5045	19.0402
900.000000 MHz	42.4409	18.9798

! Dielectric Parameter (835MHz Muscle)**Title : XC-101****SubTitle : 835 MHz Body****January 26, 2004 09:10 AM**

Frequency	e'	e''
800.000000 MHz	54.3167	21.5319
805.000000 MHz	54.3625	21.4885
810.000000 MHz	54.2580	21.4985
815.000000 MHz	54.2712	21.4553
820.000000 MHz	54.2122	21.4438
825.000000 MHz	54.1628	21.4402
830.000000 MHz	54.1542	21.4384
835.000000 MHz	54.1050	21.4293
840.000000 MHz	54.0874	21.3535
845.000000 MHz	54.0269	21.3381
850.000000 MHz	53.9734	21.3094
855.000000 MHz	53.9008	21.2556
860.000000 MHz	53.8589	21.2235
865.000000 MHz	53.7957	21.2750
870.000000 MHz	53.7602	21.1979
875.000000 MHz	53.6819	21.1750
880.000000 MHz	53.5831	21.1925
885.000000 MHz	53.5127	21.1833
890.000000 MHz	53.4664	21.1652
895.000000 MHz	53.3679	21.1046
900.000000 MHz	53.3605	21.1139

Calibration Laboratory of
Schmid & Partner
Engineering AG
Zeughausstrasse 43, 8004 Zurich, Switzerland

Client **Hyundai (Dymstec)**

CALIBRATION CERTIFICATE

Object(s) **D835V2 - SN:441**

Calibration procedure(s) **QA CAL-05.v2
Calibration procedure for dipole validation kits**

Calibration date: **October 3, 2003**

Condition of the calibrated item **In Tolerance (according to the specific calibration document)**

This calibration statement documents traceability of M&TE used in the calibration procedures and conformity of the procedures with the ISO/IEC 17025 international standard.

All calibrations have been conducted in the closed laboratory facility: environment temperature 22 +/- 2 degrees Celsius and humidity < 75%.

Calibration Equipment used (M&TE critical for calibration)

Model Type	ID #	Cal Date (Calibrated by, Certificate No.)	Scheduled Calibration
Power sensor HP 8481A	MY41092317	18-Oct-02 (Agilent, No. 20021018)	Oct-04
Power sensor HP 8481A	US37292783	30-Oct-02 (METAS, No. 252-0236)	Oct-03
Power meter EPM E442	GB37480704	30-Oct-02 (METAS, No. 252-0236)	Oct-03
RF generator R&S SML-03	100698	27-Mar-2002 (R&S, No. 20-92389)	In house check: Mar-05
Network Analyzer HP 8753E	US37390585	18-Oct-01 (Agilent, No. 24BR1033101)	In house check: Oct 03

	Name	Function	Signature
Calibrated by:	Judith Mueller	Technician	

Approved by:	Katja Pokovic	Laboratory Director	
--------------	---------------	---------------------	---

Date issued: October 10, 2003

This calibration certificate is issued as an intermediate solution until the accreditation process (based on ISO/IEC 17025 International Standard) for Calibration Laboratory of Schmid & Partner Engineering AG is completed.

Schmid & Partner Engineering AG

s p e a g

Zeughausstrasse 43, 8004 Zurich, Switzerland
Phone +41 1 245 9700, Fax +41 1 245 9779
info@speag.com, <http://www.speag.com>

DASY

Dipole Validation Kit

Type: D835V2

Serial: 441

Manufactured: March 9, 2001
Calibrated: October 3, 2003

1. Measurement Conditions

The measurements were performed in the flat section of the SAM twin phantom filled with **head simulating solution** of the following electrical parameters at 835 MHz:

Relative Dielectricity	43.0	$\pm 5\%$
Conductivity	0.90 mho/m	$\pm 5\%$

The DASY4 System with a dosimetric E-field probe ET3DV6 (SN:1507, Conversion factor 6.7 at 835 MHz) was used for the measurements.

The dipole was mounted on the small tripod so that the dipole feedpoint was positioned below the center marking of the flat phantom section and the dipole was oriented parallel to the body axis (the long side of the phantom). The standard measuring distance was 15mm from dipole center to the solution surface. The included distance spacer was used during measurements for accurate distance positioning.

The coarse grid with a grid spacing of 15mm was aligned with the dipole. The 7x7x7 fine cube was chosen for cube integration.

The dipole input power (forward power) was $250 \text{ mW} \pm 3\%$. The results are normalized to 1W input power.

2. SAR Measurement with DASY4 System

Standard SAR-measurements were performed according to the measurement conditions described in section 1. The results (see figure supplied) have been normalized to a dipole input power of 1W (forward power). The resulting averaged SAR-values measured with the dosimetric probe ET3DV6 SN:1507 and applying the advanced extrapolation are:

averaged over 1 cm^3 (1 g) of tissue: **9.24 mW/g** $\pm 16.8\%$ ($k=2$)¹

averaged over 10 cm^3 (10 g) of tissue: **6.08 mW/g** $\pm 16.2\%$ ($k=2$)¹

¹ validation uncertainty

3. Dipole Impedance and Return Loss

The impedance was measured at the SMA-connector with a network analyzer and numerically transformed to the dipole feedpoint. The transformation parameters from the SMA-connector to the dipole feedpoint are:

Electrical delay: 1.377 ns (one direction)
Transmission factor: 0.983 (voltage transmission, one direction)

The dipole was positioned at the flat phantom sections according to section 1 and the distance spacer was in place during impedance measurements.

Feedpoint impedance at 835 MHz: $\text{Re}\{Z\} = 52.0 \Omega$
 $\text{Im}\{Z\} = -6.1 \Omega$
Return Loss at 835 MHz -24.1 dB

4. Handling

Do not apply excessive force to the dipole arms, because they might bend. Bending of the dipole arms stresses the soldered connections near the feedpoint leading to a damage of the dipole.

5. Design

The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals.

6. Power Test

After long term use with 100W radiated power, only a slight warming of the dipole near the feedpoint can be measured.

Test Laboratory: SPEAG, Zurich, Switzerland

DUT: Dipole 835 MHz; Type: D835V2; Serial: D835V2 - SN441

Communication System: CW-835; Frequency: 835 MHz; Duty Cycle: 1:1

Medium: HSL 835 MHz ($\sigma = 0.9$ mho/m, $\epsilon_r = 43$, $\rho = 1000$ kg/m³)

Phantom section: Flat Section

Measurement Standard: DASY4 (High Precision Assessment)

DASY4 Configuration:

- Probe: ET3DV6 - SN1507; ConvF(6.7, 6.7, 6.7); Calibrated: 1/18/2003
- Sensor-Surface: 4mm (Mechanical Surface Detection)
- Electronics: DAE3 - SN411; Calibrated: 1/16/2003
- Phantom: SAM with CRP - TP1006; Type: SAM 4.0; Serial: TP:1006
- Measurement SW: DASY4, V4.1 Build 47; Postprocessing SW: SEMCAD, V1.8 Build 60

Pin = 250 mW; d = 15 mm/Area Scan (81x81x1): Measurement grid: dx=15mm, dy=15mm

Reference Value = 54.7 V/m

Power Drift = 0.003 dB

Maximum value of SAR = 2.48 mW/g

Pin = 250 mW; d = 15 mm/Zoom Scan (7x7x7)/Cube 0: Measurement grid: dx=5mm, dy=5mm, dz=5mm

Peak SAR (extrapolated) = 3.45 W/kg

SAR(1 g) = 2.31 mW/g; SAR(10 g) = 1.52 mW/g

Reference Value = 54.7 V/m

Power Drift = 0.003 dB

Maximum value of SAR = 2.5 mW/g

