

System Check_Head_2450MHz

DUT: D2450V2-SN:1040

Communication System: ; Frequency: 2450.0

Medium: HSL. Medium parameters used: $f= 2450.0$ MHz; $\sigma= 1.74$ S/m; $\epsilon_r = 39.2$

Ambient Temperature: 23.3°C; Liquid Temperature: 22.7°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7764; ConvF(8.25, 8.25, 8.25); Calibrated: 2022-09-30
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1279; Calibrated: 2022-10-26
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2074
- Measurement Software: cDASY6 V6.6.0.13926


Area Scan (40.0 mm x 96.0 mm): Measurement Grid: 12.0 mm x 12.0 mm

SAR (1g) = 2.42 W/kg; SAR (10g) = 1.02 W/kg;

Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm): Measurement Grid: 5.0 mm x 5.0 mm x 5.0 mm

Power Drift = -0.05 dB

SAR (1g) = 2.47 W/kg; SAR (10g) = 1.13 W/kg;

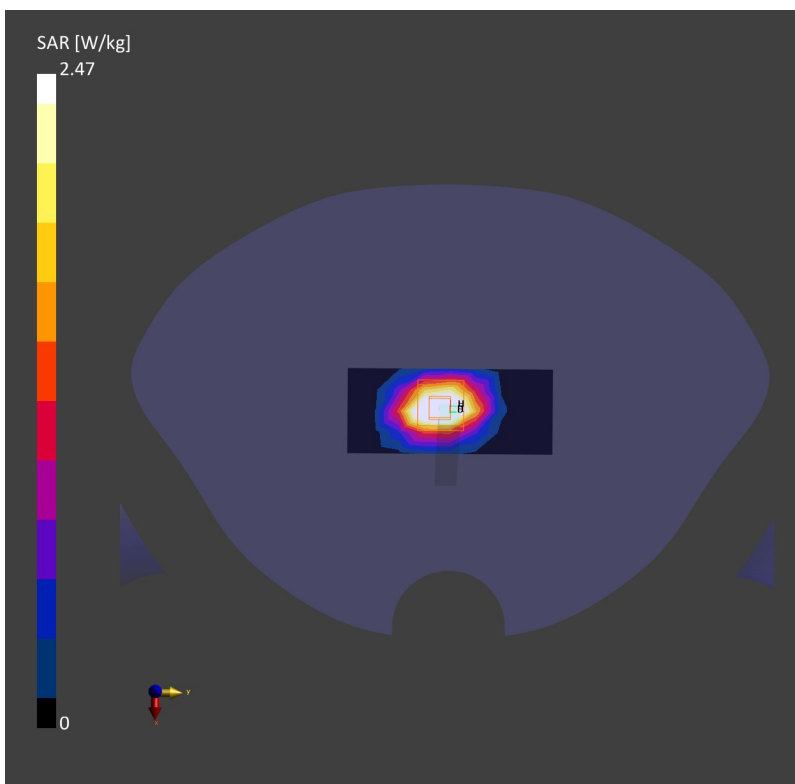

System Check_Head_5250MHz

DUT: D5GHzV2-SN:1341

Communication System: ; Frequency: 5250.0

Medium: HSL. Medium parameters used: $f= 5250.0$ MHz; $\sigma= 4.58$ S/m; $\epsilon_r = 35.7$

Ambient Temperature: 23.2°C; Liquid Temperature: 22.9°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7764; ConvF(5.65, 5.65, 5.65); Calibrated: 2022-09-30
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1279; Calibrated: 2022-10-26
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2074
- Measurement Software: cDASY6 V6.6.0.13926


Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 3.64 W/kg; SAR (10g) = 1.07 W/kg;

Zoom Scan (24.0 mm x 24.0 mm x 22.0 mm): Measurement Grid: 4.0 mm x 4.0 mm x 1.4 mm

Power Drift = 0.01 dB

SAR(1 g) = 4.03 W/kg; SAR(10 g) = 1.16 W/kg;

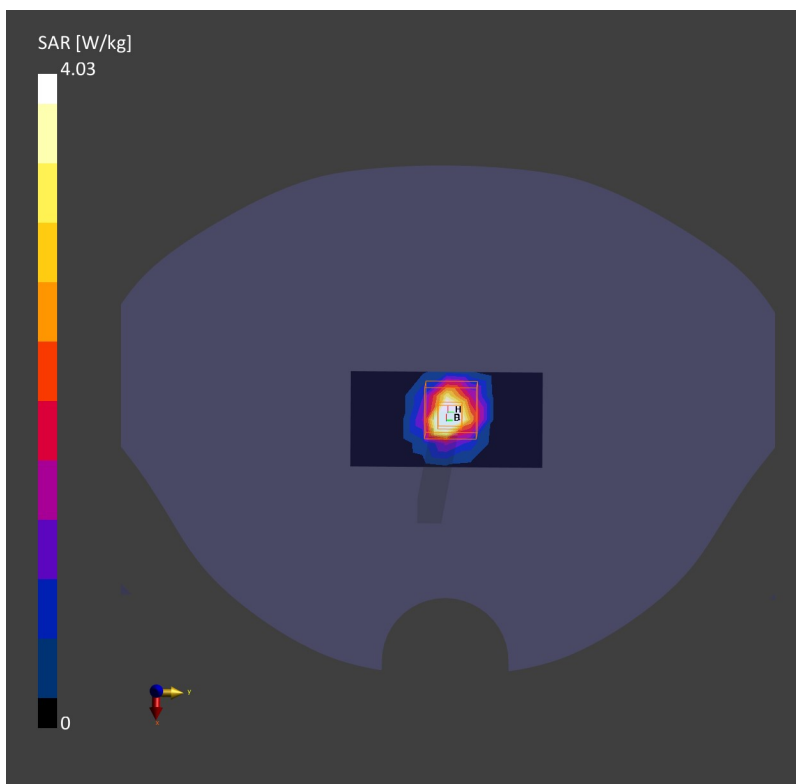

System Check_Head_5600MHz

DUT: D5GHzV2-SN:1341

Communication System: ; Frequency: 5600.0

Medium: HSL. Medium parameters used: $f= 5600.0$ MHz; $\sigma= 4.96$ S/m; $\epsilon_r = 35.0$

Ambient Temperature: 23.4°C; Liquid Temperature: 22.8°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7764; ConvF(4.9, 4.9, 4.9); Calibrated: 2022-09-30
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1279; Calibrated: 2022-10-26
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2074
- Measurement Software: cDASY6 V6.6.0.13926


Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 3.45 W/kg; SAR (10g) = 1.05 W/kg;

Zoom Scan (24.0 mm x 24.0 mm x 22.0 mm): Measurement Grid: 4.0 mm x 4.0 mm x 1.4 mm

Power Drift = 0.01 dB

SAR(1 g) = 3.95 W/kg; SAR(10 g) = 1.12 W/kg;

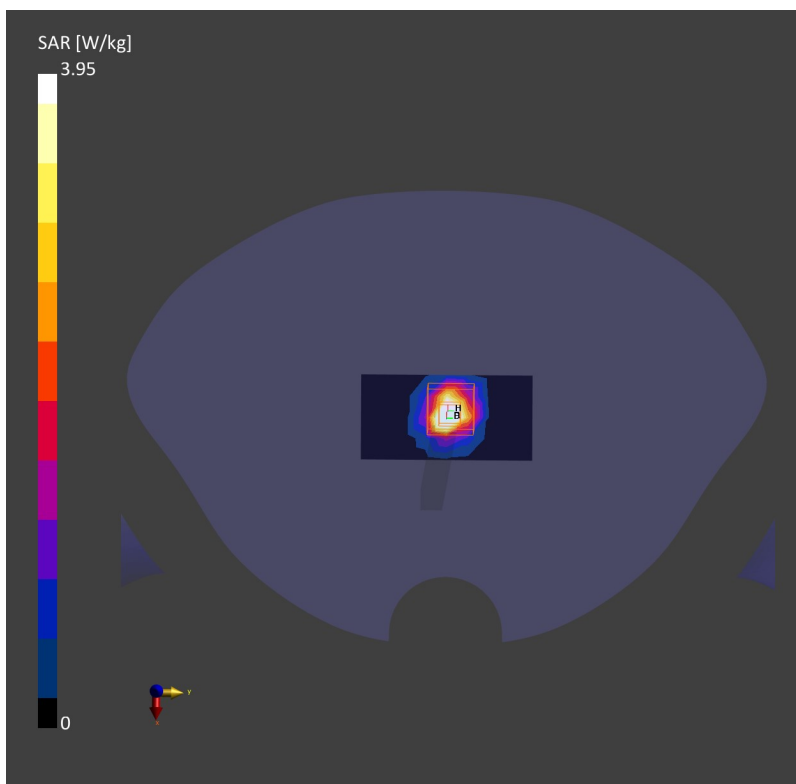

System Check_Head_5750MHz

DUT: D5GHzV2-SN:1341

Communication System: ; Frequency: 5750.0

Medium: HSL. Medium parameters used: $f= 5750.0$ MHz; $\sigma= 5.12$ S/m; $\epsilon_r = 34.8$

Ambient Temperature: 23.4°C; Liquid Temperature: 22.9°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7764; ConvF(5.1, 5.1, 5.1); Calibrated: 2022-09-30
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1279; Calibrated: 2022-10-26
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2074
- Measurement Software: cDASY6 V6.6.0.13926


Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 3.40 W/kg; SAR (10g) = 1.06 W/kg;

Zoom Scan (24.0 mm x 24.0 mm x 22.0 mm): Measurement Grid: 4.0 mm x 4.0 mm x 1.4 mm

Power Drift = -0.03 dB

SAR(1 g) = 3.95 W/kg; SAR(10 g) = 1.13 W/kg;

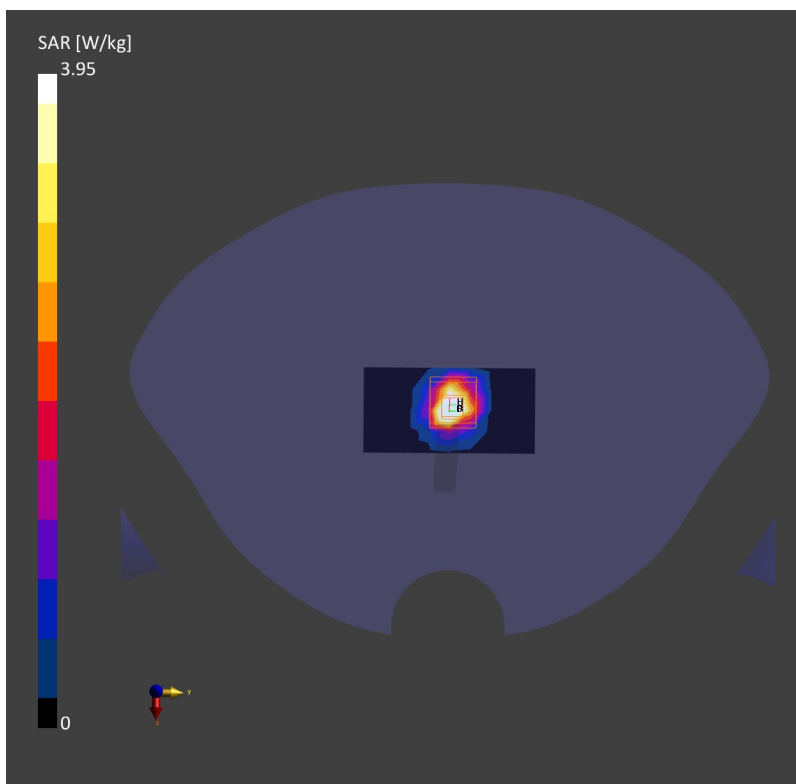

System Check_Head_2450MHz

DUT: D2450V2-SN:1040

Communication System: ; Frequency: 2450.0

Medium: HSL. Medium parameters used: $f= 2450.0$ MHz; $\sigma= 1.74$ S/m; $\epsilon_r = 39.2$

Ambient Temperature: 23.3°C; Liquid Temperature: 22.6°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7764; ConvF(8.25, 8.25, 8.25); Calibrated: 2022-09-30
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1279; Calibrated: 2022-10-26
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2074
- Measurement Software: cDASY6 V6.6.0.13926


Area Scan (40.0 mm x 96.0 mm): Measurement Grid: 12.0 mm x 12.0 mm

SAR (1g) = 2.47 W/kg; SAR (10g) = 1.06 W/kg;

Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm): Measurement Grid: 5.0 mm x 5.0 mm x 5.0 mm

Power Drift = 0.05 dB

SAR (1g) = 2.52 W/kg; SAR (10g) = 1.18 W/kg;

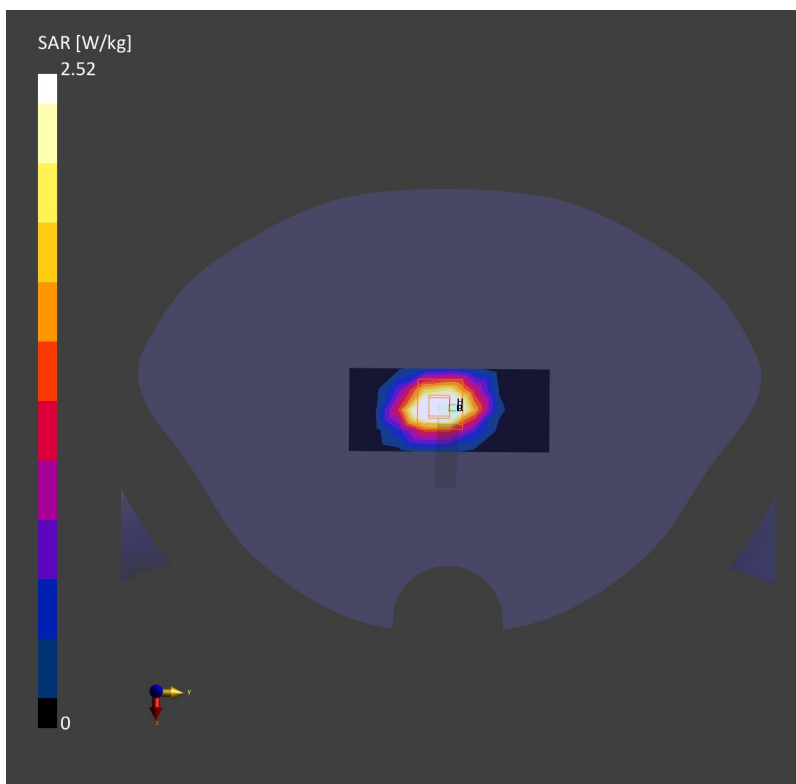

System Check_Head_5250MHz

DUT: D5GHzV2-SN:1341

Communication System: ; Frequency: 5250.0

Medium: HSL. Medium parameters used: $f= 5250.0$ MHz; $\sigma= 4.58$ S/m; $\epsilon_r = 35.7$

Ambient Temperature: 23.2°C; Liquid Temperature: 22.9°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7764; ConvF(5.65, 5.65, 5.65); Calibrated: 2022-09-30
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1279; Calibrated: 2022-10-26
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2074
- Measurement Software: cDASY6 V6.6.0.13926


Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 3.66 W/kg; SAR (10g) = 1.05 W/kg;

Zoom Scan (24.0 mm x 24.0 mm x 22.0 mm): Measurement Grid: 4.0 mm x 4.0 mm x 1.4 mm

Power Drift = 0.01 dB

SAR(1 g) = 3.98 W/kg; SAR(10 g) = 1.12 W/kg;

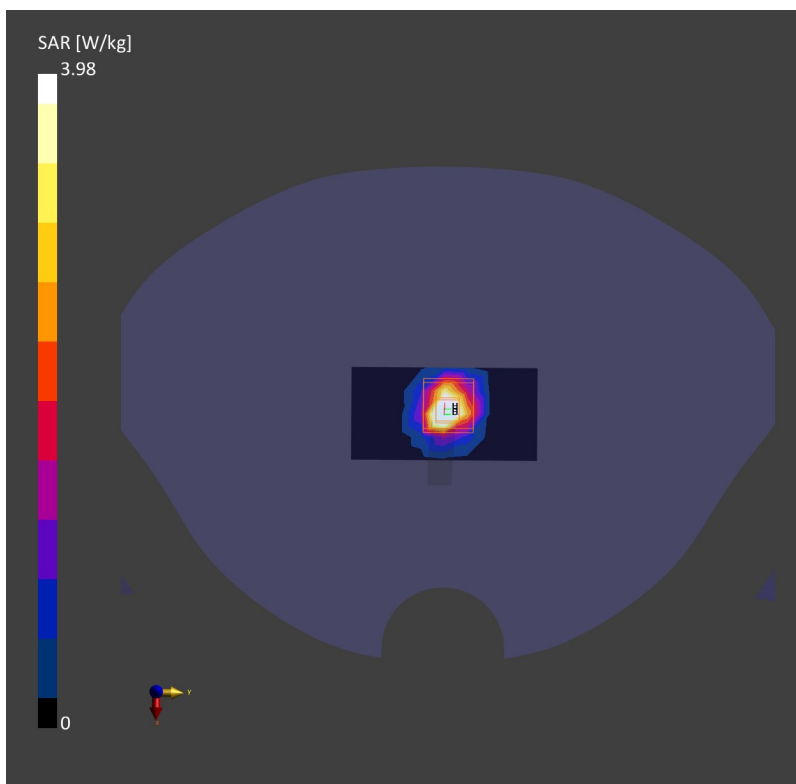

System Check_Head_5600MHz

DUT: D5GHzV2-SN:1341

Communication System: ; Frequency: 5600.0

Medium: HSL. Medium parameters used: $f= 5600.0$ MHz; $\sigma= 4.95$ S/m; $\epsilon_r = 35.1$

Ambient Temperature: 23.4°C; Liquid Temperature: 22.8°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7764; ConvF(4.9, 4.9, 4.9); Calibrated: 2022-09-30
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1279; Calibrated: 2022-10-26
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2074
- Measurement Software: cDASY6 V6.6.0.13926


Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 3.53 W/kg; SAR (10g) = 1.08 W/kg;

Zoom Scan (24.0 mm x 24.0 mm x 22.0 mm): Measurement Grid: 4.0 mm x 4.0 mm x 1.4 mm

Power Drift = 0.01 dB

SAR(1 g) = 4.02 W/kg; SAR(10 g) = 1.16 W/kg;

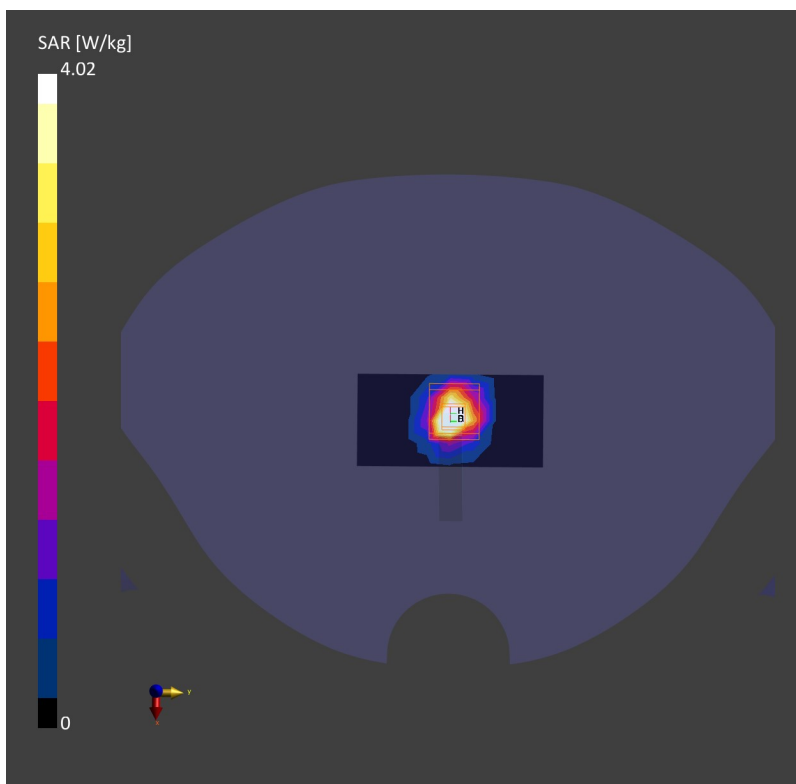

System Check_Head_5750MHz

DUT: D5GHzV2-SN:1341

Communication System: ; Frequency: 5750.0

Medium: HSL. Medium parameters used: $f= 5750.0$ MHz; $\sigma= 5.11$ S/m; $\epsilon_r = 34.9$

Ambient Temperature: 23.3°C; Liquid Temperature: 22.8°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7764; ConvF(5.1, 5.1, 5.1); Calibrated: 2022-09-30
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1279; Calibrated: 2022-10-26
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2074
- Measurement Software: cDASY6 V6.6.0.13926

Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 3.53 W/kg; SAR (10g) = 1.02 W/kg;

Zoom Scan (24.0 mm x 24.0 mm x 22.0 mm): Measurement Grid: 4.0 mm x 4.0 mm x 1.4 mm

Power Drift = -0.06 dB

SAR(1 g) = 3.92 W/kg; SAR(10 g) = 1.10 W/kg;

