

System Check_Head_750MHz

DUT: D750V3-SN:1087

Communication System: ; Frequency: 750.0

Medium: HSL. Medium parameters used: $f = 750.0$ MHz; $\sigma = 0.890$ S/m; $\epsilon_r = 42.2$

Ambient Temperature: 23.3°C; Liquid Temperature: 22.6°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7630; ConvF(10.35, 10.35, 10.35); Calibrated: 2022-03-04
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1305; Calibrated: 2022-04-27
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2022
- Measurement Software: cDASY6 V6.6.0.13926


Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 15.0 mm x 15.0 mm

SAR (1g) = 0.402 W/kg; SAR (10g) = 0.254 W/kg;

Zoom Scan (32.0 mm x 32.0 mm x 30.0 mm): Measurement Grid: 8.0 mm x 8.0 mm x 5.0 mm

Power Drift = -0.03 dB

SAR (1g) = 0.411 W/kg; SAR (10g) = 0.265 W/kg;

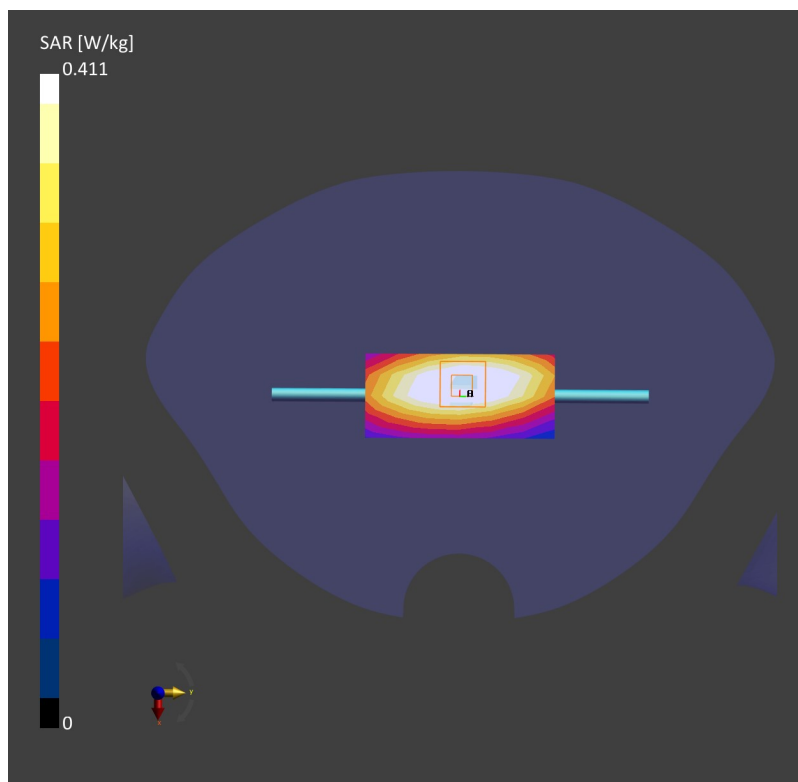

System Check_Head_835MHz

DUT: D835V2-SN:4d091

Communication System: ; Frequency: 835.0

Medium: HSL. Medium parameters used: $f = 835.0$ MHz; $\sigma = 0.912$ S/m; $\epsilon_r = 41.9$

Ambient Temperature: 23.1°C; Liquid Temperature: 22.8°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7630; ConvF(10.05, 10.05, 10.05); Calibrated: 2022-03-04
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1305; Calibrated: 2022-04-27
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2022
- Measurement Software: cDASY6 V6.6.0.13926


Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 15.0 mm x 15.0 mm

SAR (1g) = 0.469 W/kg; SAR (10g) = 0.299 W/kg;

Zoom Scan (32.0 mm x 32.0 mm x 30.0 mm): Measurement Grid: 8.0 mm x 8.0 mm x 5.0 mm

Power Drift = 0.06 dB

SAR (1g) = 0.474 W/kg; SAR (10g) = 0.317 W/kg;

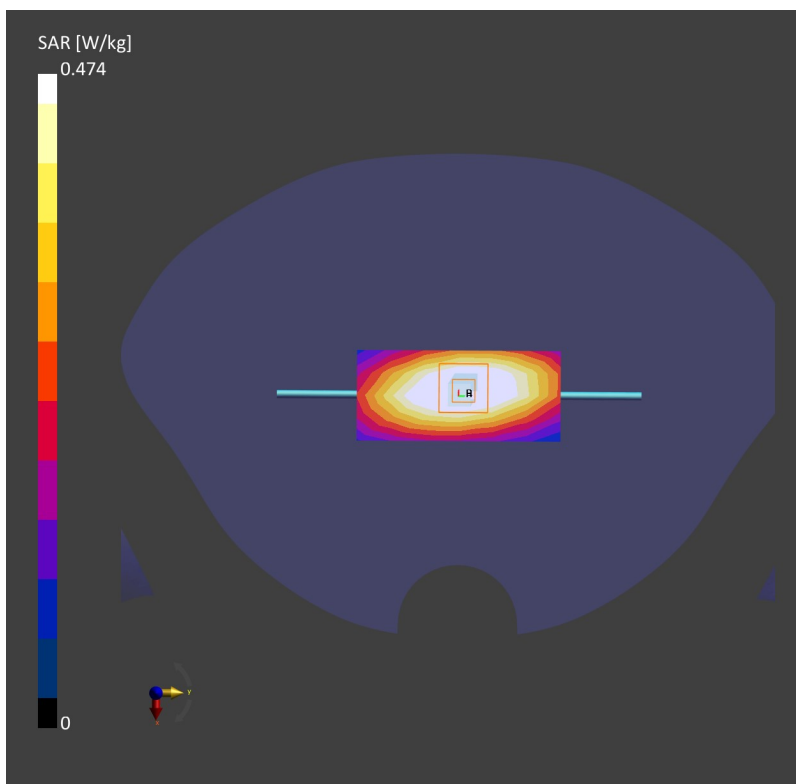

System Check_Head_1750MHz

DUT: D1750V2-SN:1090

Communication System: ; Frequency: 1750.0

Medium: HSL. Medium parameters used: $f = 1750.0$ MHz; $\sigma = 1.32$ S/m; $\epsilon_r = 40.2$

Ambient Temperature: 23.2°C; Liquid Temperature: 22.8°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7630; ConvF(8.97, 8.97, 8.97); Calibrated: 2022-03-04
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1305; Calibrated: 2022-04-27
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2022
- Measurement Software: cDASY6 V6.6.0.13926


Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 15.0 mm x 15.0 mm

SAR (1g) = 1.62 W/kg; SAR (10g) = 0.941 W/kg;

Zoom Scan (32.0 mm x 32.0 mm x 30.0 mm): Measurement Grid: 8.0 mm x 8.0 mm x 5.0 mm

Power Drift = 0.01 dB

SAR (1g) = 1.77 W/kg; SAR (10g) = 0.958 W/kg;

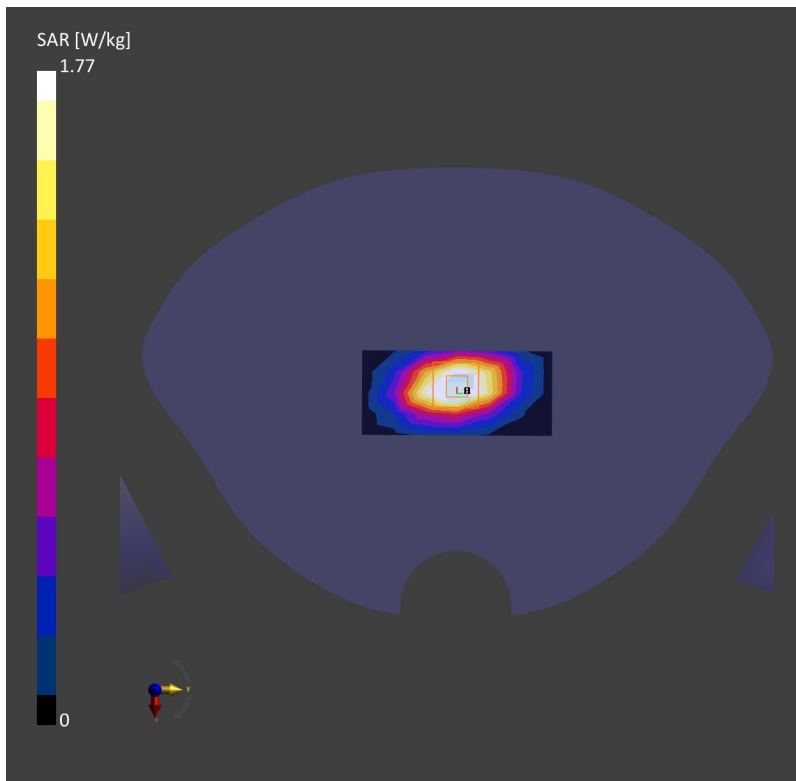

System Check_Head_1900MHz

DUT: D1900V2-SN:5d182

Communication System: ; Frequency: 1900.0

Medium: HSL. Medium parameters used: $f = 1900.0$ MHz; $\sigma = 1.40$ S/m; $\epsilon_r = 40.2$

Ambient Temperature: 23.3°C; Liquid Temperature: 22.7°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7630; ConvF(8.51, 8.51, 8.51); Calibrated: 2022-03-04
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1305; Calibrated: 2022-04-27
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2022
- Measurement Software: cDASY6 V6.6.0.13926


Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 15.0 mm x 15.0 mm

SAR (1g) = 1.90 W/kg; SAR (10g) = 1.01 W/kg;

Zoom Scan (32.0 mm x 32.0 mm x 30.0 mm): Measurement Grid: 8.0 mm x 8.0 mm x 5.0 mm

Power Drift = -0.01 dB

SAR (1g) = 1.93 W/kg; SAR (10g) = 1.02 W/kg;

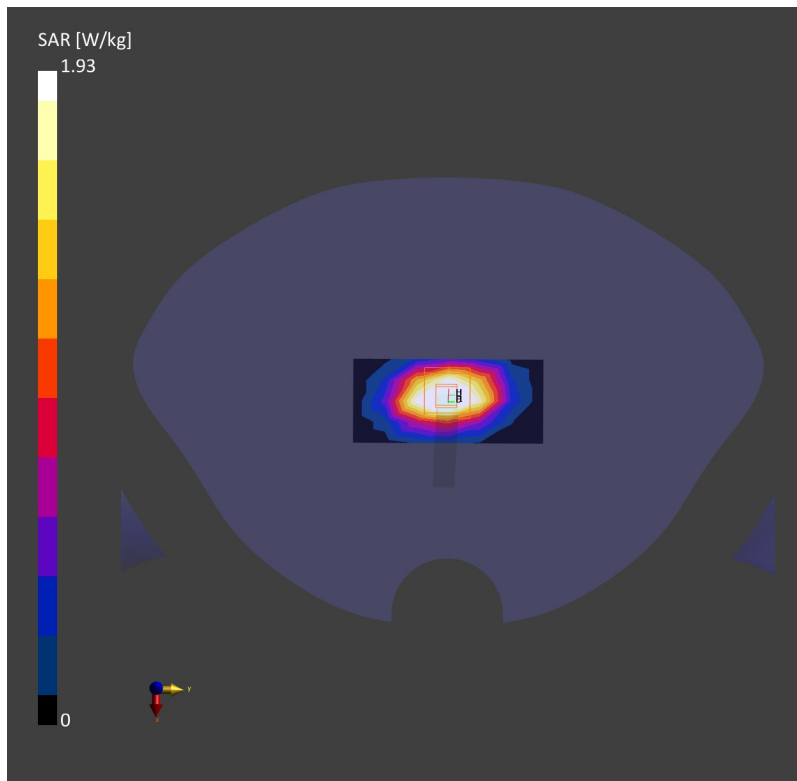

System Check_Head_2300MHz

DUT: D2300V2-SN:1055

Communication System: ; Frequency: 2300.0

Medium: HSL. Medium parameters used: $f = 2300.0$ MHz; $\sigma = 1.65$ S/m; $\epsilon_r = 39.6$

Ambient Temperature: 23.2°C; Liquid Temperature: 22.7°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7630; ConvF(8.37, 8.37, 8.37); Calibrated: 2022-03-04
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1305; Calibrated: 2022-04-27
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2022
- Measurement Software: cDASY6 V6.6.0.13926


Area Scan (40.0 mm x 96.0 mm): Measurement Grid: 12.0 mm x 12.0 mm

SAR (1g) = 2.12 W/kg; SAR (10g) = 0.984 W/kg;

Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm): Measurement Grid: 5.0 mm x 5.0 mm x 5.0 mm

Power Drift = 0.06 dB

SAR (1g) = 2.33 W/kg; SAR (10g) = 1.14 W/kg;

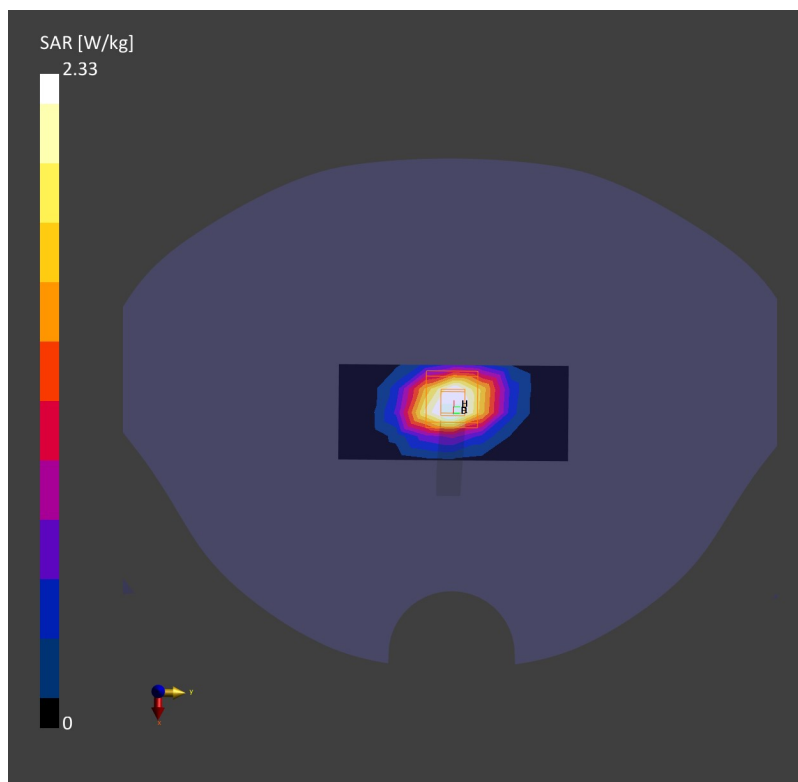

System Check_Head_2600MHz

DUT: D2600V2-SN:1061

Communication System: ; Frequency: 2600.0

Medium: HSL. Medium parameters used: $f = 2600.0$ MHz; $\sigma = 2.01$ S/m; $\epsilon_r = 40.5$

Ambient Temperature: 23.4°C; Liquid Temperature: 22.6°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7630; ConvF(7.82, 7.82, 7.82); Calibrated: 2022-03-04
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1305; Calibrated: 2022-04-27
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2022
- Measurement Software: cDASY6 V6.6.0.13926


Area Scan (40.0 mm x 96.0 mm): Measurement Grid: 12.0 mm x 12.0 mm

SAR (1g) = 2.62 W/kg; SAR (10g) = 1.15 W/kg;

Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm): Measurement Grid: 5.0 mm x 5.0 mm x 5.0 mm

Power Drift = 0.01 dB

SAR(1 g) = 2.69 W/kg; SAR(10 g) = 1.19 W/kg;

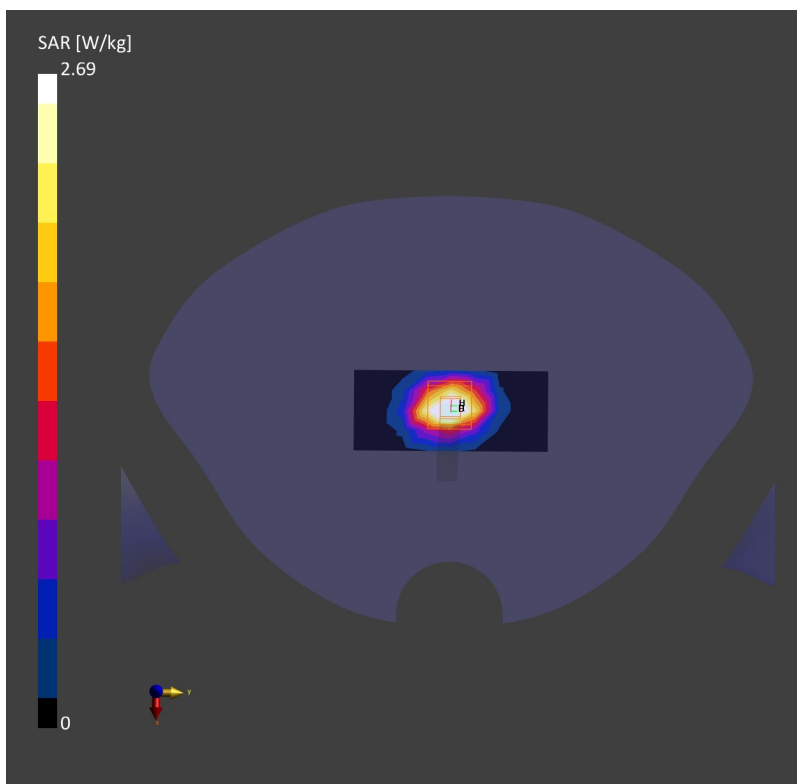

System Check_Head_3500MHz

DUT: D3500V2-SN:1037

Communication System: ; Frequency: 3500.0

Medium: HSL. Medium parameters used: $f = 3500.0$ MHz; $\sigma = 2.81$ S/m; $\epsilon_r = 38.7$

Ambient Temperature: 23.3°C; Liquid Temperature: 22.6°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7630; ConvF(7.34, 7.34, 7.34); Calibrated: 2022-03-04
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1305; Calibrated: 2022-04-27
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2022
- Measurement Software: cDASY6 V6.6.0.13926


Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 3.11 W/kg; SAR (10g) = 1.21 W/kg;

Zoom Scan (24.0 mm x 24.0 mm x 22.0 mm): Measurement Grid: 4.0 mm x 4.0 mm x 1.4 mm

Power Drift = 0.01 dB

SAR(1 g) = 3.29 W/kg; SAR(10 g) = 1.27 W/kg;

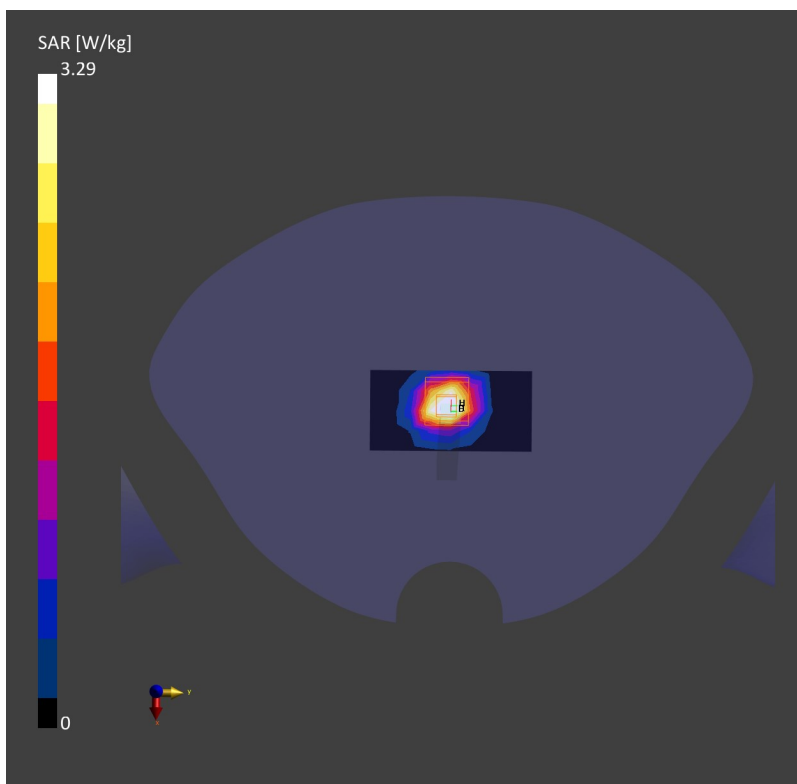

System Check_Head_3700MHz

DUT: D3700V2-SN:1008

Communication System: ; Frequency: 3700.0

Medium: HSL. Medium parameters used: $f = 3700.0$ MHz; $\sigma = 2.99$ S/m; $\epsilon_r = 38.3$

Ambient Temperature: 23.2°C; Liquid Temperature: 22.9°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7630; ConvF(7.33, 7.33, 7.33); Calibrated: 2022-03-04
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1305; Calibrated: 2022-04-27
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2022
- Measurement Software: cDASY6 V6.6.0.13926


Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 2.98 W/kg; SAR (10g) = 1.10 W/kg;

Zoom Scan (24.0 mm x 24.0 mm x 22.0 mm): Measurement Grid: 4.0 mm x 4.0 mm x 1.4 mm

Power Drift = -0.02 dB

SAR(1 g) = 3.23 W/kg; SAR(10 g) = 1.16 W/kg;

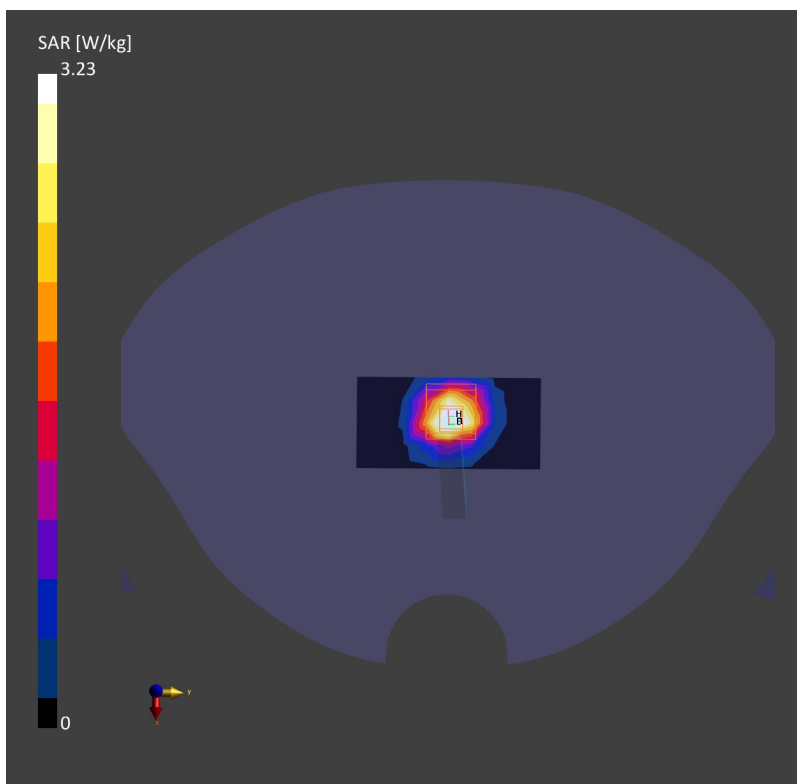

System Check_Head_3900MHz

DUT: D3900V2-SN:1048

Communication System: ; Frequency: 3900.0

Medium: HSL. Medium parameters used: $f = 3900.0$ MHz; $\sigma = 3.28$ S/m; $\epsilon_r = 37.6$

Ambient Temperature: 23.2°C; Liquid Temperature: 22.8°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7764; ConvF(6.66, 6.66, 6.66); Calibrated: 2022-09-30
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1279; Calibrated: 2022-10-26
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2022
- Measurement Software: cDASY6 V6.6.0.13926


Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 3.22 W/kg; SAR (10g) = 1.13 W/kg;

Zoom Scan (24.0 mm x 24.0 mm x 22.0 mm): Measurement Grid: 4.0 mm x 4.0 mm x 1.4 mm

Power Drift = -0.04 dB

SAR(1 g) = 3.45 W/kg; SAR(10 g) = 1.18 W/kg;

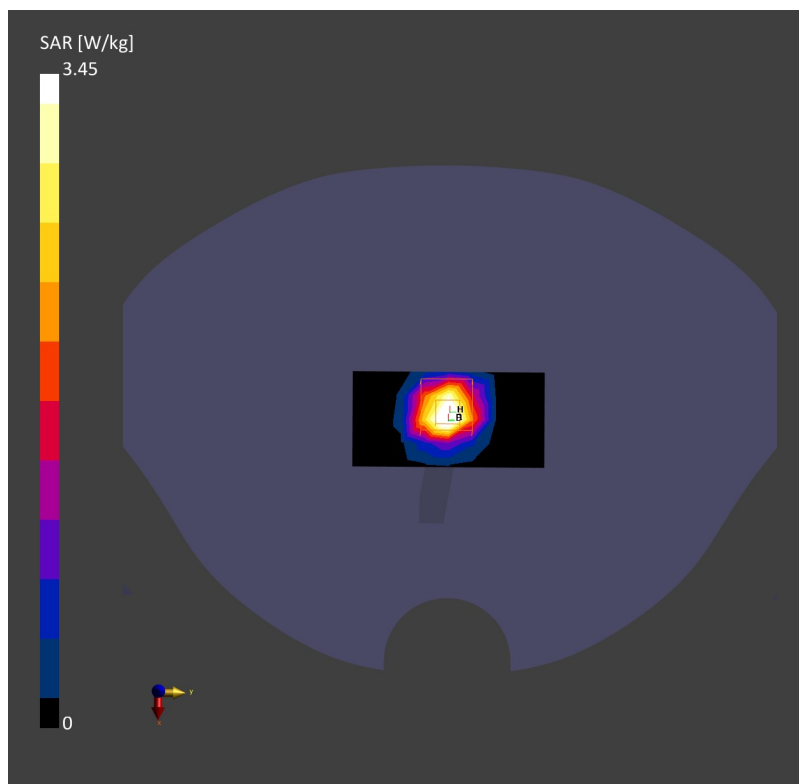

System Check_Head_750MHz

DUT: D750V3-SN:1087

Communication System: ; Frequency: 750.0

Medium: HSL. Medium parameters used: $f = 750.0$ MHz; $\sigma = 0.888$ S/m; $\epsilon_r = 42.2$

Ambient Temperature: 23.3°C; Liquid Temperature: 22.6°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7630; ConvF(10.35, 10.35, 10.35); Calibrated: 2022-03-04
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1305; Calibrated: 2022-04-27
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2022
- Measurement Software: cDASY6 V6.6.0.13926


Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 15.0 mm x 15.0 mm

SAR (1g) = 0.397 W/kg; SAR (10g) = 0.263 W/kg;

Zoom Scan (32.0 mm x 32.0 mm x 30.0 mm): Measurement Grid: 8.0 mm x 8.0 mm x 5.0 mm

Power Drift = -0.01 dB

SAR (1g) = 0.406 W/kg; SAR (10g) = 0.277 W/kg;

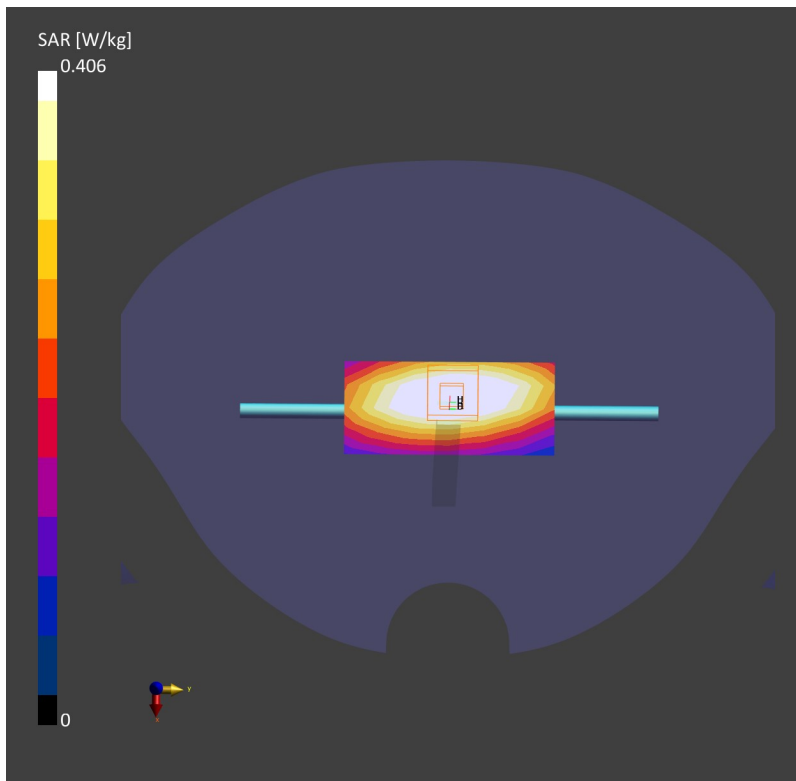

System Check_Head_835MHz

DUT: D835V2-SN:4d091

Communication System: ; Frequency: 835.0

Medium: HSL. Medium parameters used: $f = 835.0$ MHz; $\sigma = 0.911$ S/m; $\epsilon_r = 41.9$

Ambient Temperature: 23.1°C; Liquid Temperature: 22.6°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7630; ConvF(10.05, 10.05, 10.05); Calibrated: 2022-03-04
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1305; Calibrated: 2022-04-27
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2022
- Measurement Software: cDASY6 V6.6.0.13926


Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 15.0 mm x 15.0 mm

SAR (1g) = 0.461 W/kg; SAR (10g) = 0.284 W/kg;

Zoom Scan (32.0 mm x 32.0 mm x 30.0 mm): Measurement Grid: 8.0 mm x 8.0 mm x 5.0 mm

Power Drift = 0.04 dB

SAR (1g) = 0.466 W/kg; SAR (10g) = 0.302 W/kg;

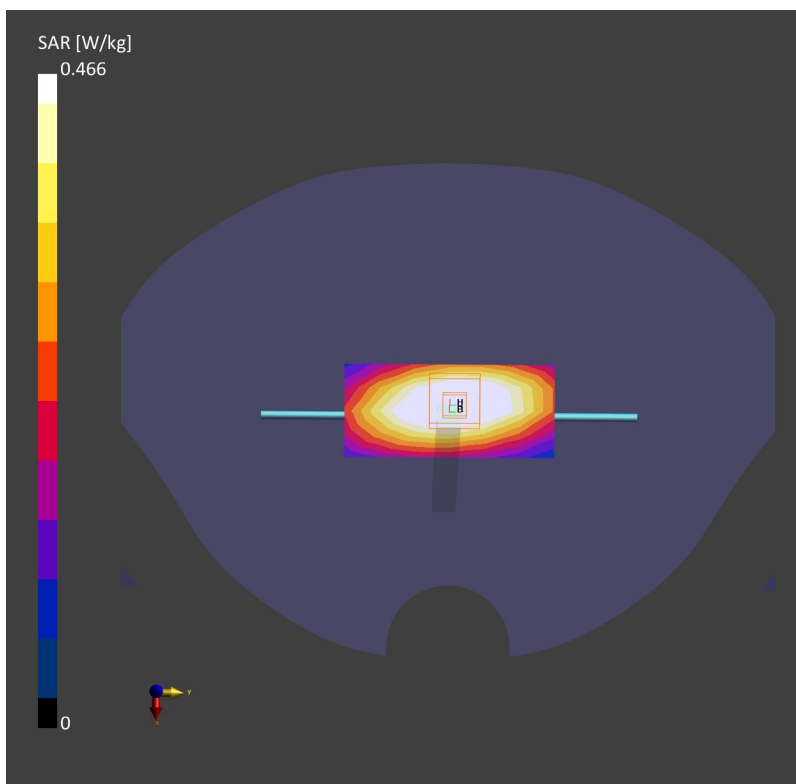

System Check_Head_1750MHz

DUT: D1750V2-SN:1090

Communication System: ; Frequency: 1750.0

Medium: HSL. Medium parameters used: $f = 1750.0$ MHz; $\sigma = 1.32$ S/m; $\epsilon_r = 40.2$

Ambient Temperature: 23.2°C; Liquid Temperature: 22.9°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7630; ConvF(8.97, 8.97, 8.97); Calibrated: 2022-03-04
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1305; Calibrated: 2022-04-27
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2022
- Measurement Software: cDASY6 V6.6.0.13926


Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 15.0 mm x 15.0 mm

SAR (1g) = 1.64 W/kg; SAR (10g) = 0.946 W/kg;

Zoom Scan (32.0 mm x 32.0 mm x 30.0 mm): Measurement Grid: 8.0 mm x 8.0 mm x 5.0 mm

Power Drift = 0.01 dB

SAR (1g) = 1.79 W/kg; SAR (10g) = 0.963 W/kg;

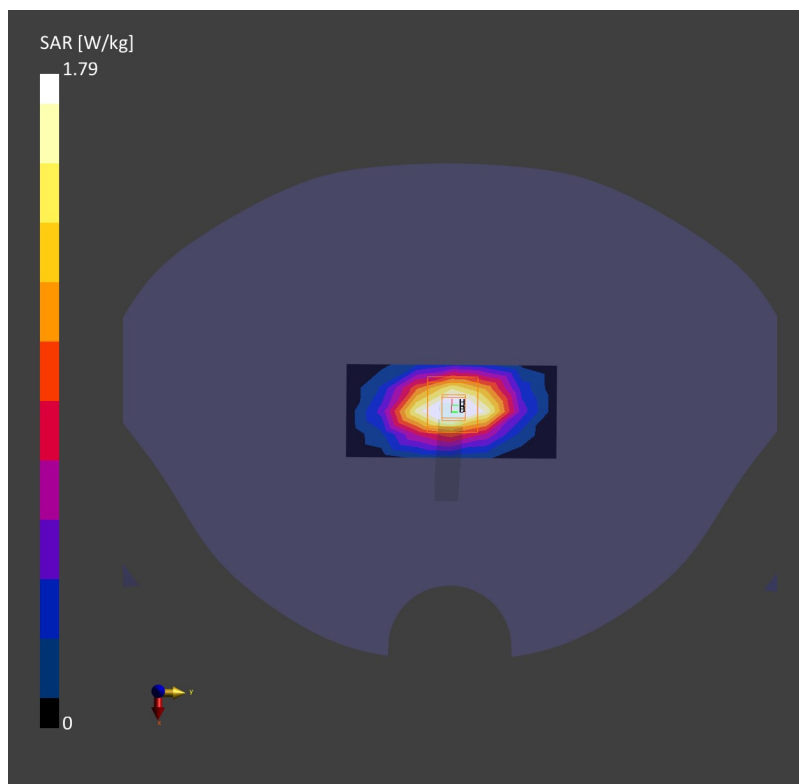

System Check_Head_1900MHz

DUT: D1900V2-SN:5d182

Communication System: ; Frequency: 1900.0

Medium: HSL. Medium parameters used: $f = 1900.0$ MHz; $\sigma = 1.41$ S/m; $\epsilon_r = 40.2$

Ambient Temperature: 23.2°C; Liquid Temperature: 22.7°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7630; ConvF(8.51, 8.51, 8.51); Calibrated: 2022-03-04
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1305; Calibrated: 2022-04-27
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2022
- Measurement Software: cDASY6 V6.6.0.13926


Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 15.0 mm x 15.0 mm

SAR (1g) = 1.94 W/kg; SAR (10g) = 1.03 W/kg;

Zoom Scan (32.0 mm x 32.0 mm x 30.0 mm): Measurement Grid: 8.0 mm x 8.0 mm x 5.0 mm

Power Drift = -0.03 dB

SAR (1g) = 1.98 W/kg; SAR (10g) = 1.05 W/kg;

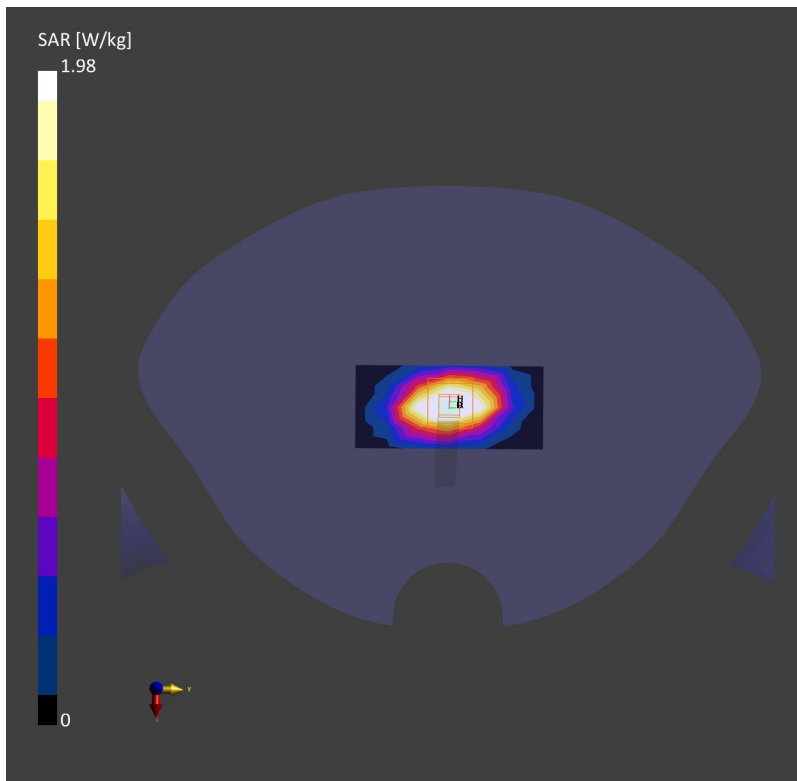

System Check_Head_2300MHz

DUT: D2300V2-SN:1055

Communication System: ; Frequency: 2300.0

Medium: HSL. Medium parameters used: $f = 2300.0$ MHz; $\sigma = 1.65$ S/m; $\epsilon_r = 39.6$

Ambient Temperature: 23.3°C; Liquid Temperature: 22.7°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7630; ConvF(8.37, 8.37, 8.37); Calibrated: 2022-03-04
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1305; Calibrated: 2022-04-27
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2022
- Measurement Software: cDASY6 V6.6.0.13926


Area Scan (40.0 mm x 96.0 mm): Measurement Grid: 12.0 mm x 12.0 mm

SAR (1g) = 2.16 W/kg; SAR (10g) = 1.04 W/kg;

Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm): Measurement Grid: 5.0 mm x 5.0 mm x 5.0 mm

Power Drift = 0.06 dB

SAR (1g) = 2.37 W/kg; SAR (10g) = 1.17 W/kg;

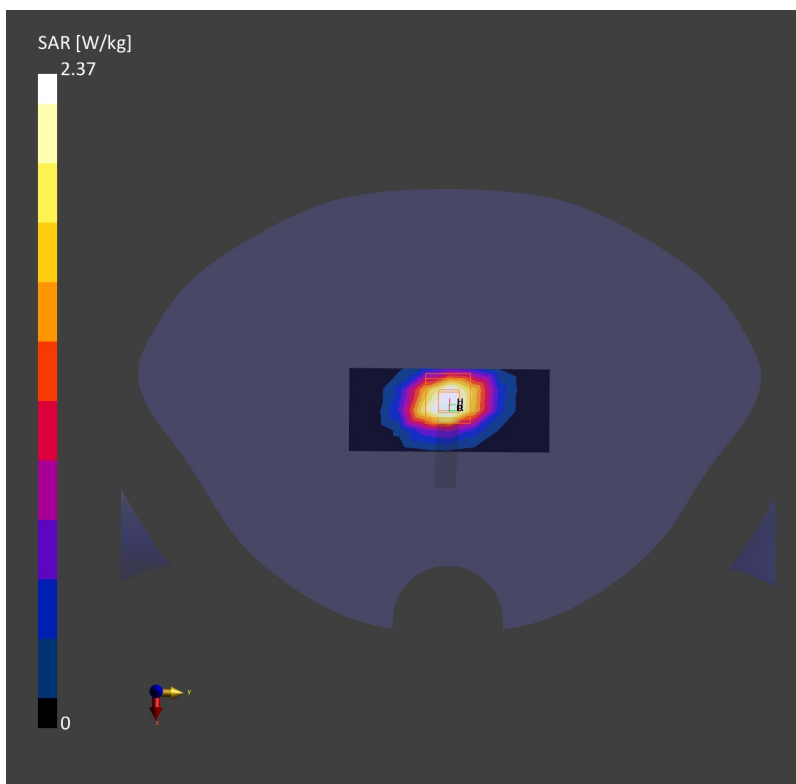

System Check_Head_2600MHz

DUT: D2600V2-SN:1061

Communication System: ; Frequency: 2600.0

Medium: HSL. Medium parameters used: $f = 2600.0$ MHz; $\sigma = 1.93$ S/m; $\epsilon_r = 38.2$

Ambient Temperature: 23.3°C; Liquid Temperature: 22.6°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7630; ConvF(7.82, 7.82, 7.82); Calibrated: 2022-03-04
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1305; Calibrated: 2022-04-27
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2022
- Measurement Software: cDASY6 V6.6.0.13926


Area Scan (40.0 mm x 96.0 mm): Measurement Grid: 12.0 mm x 12.0 mm

SAR (1g) = 2.59 W/kg; SAR (10g) = 1.13 W/kg;

Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm): Measurement Grid: 5.0 mm x 5.0 mm x 5.0 mm

Power Drift = 0.01 dB

SAR (1g) = 2.66 W/kg; SAR(10 g) = 1.17 W/kg;

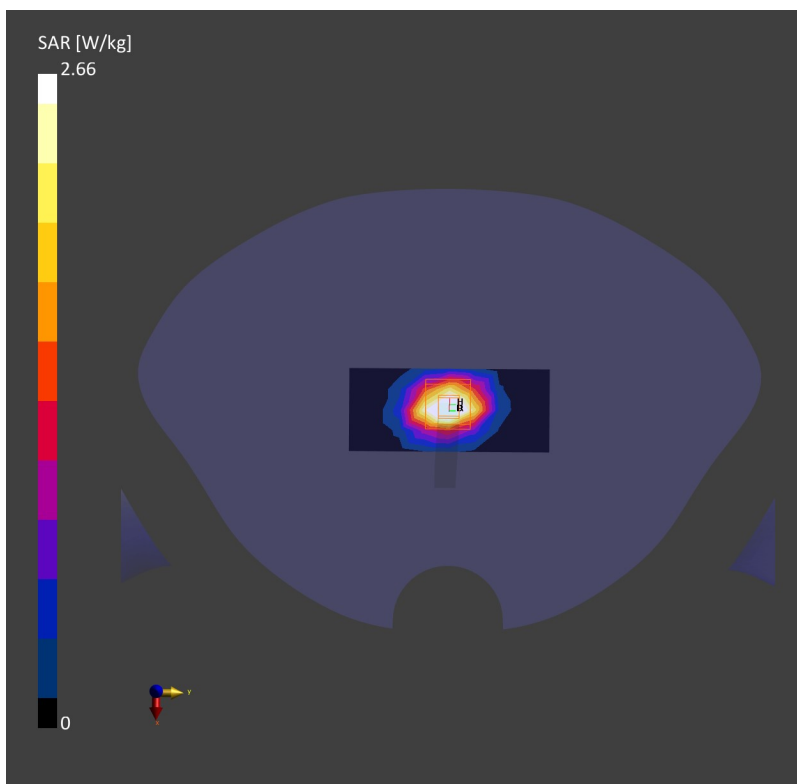

System Check_Head_3500MHz

DUT: D3500V2-SN:1037

Communication System: ; Frequency: 3500.0

Medium: HSL. Medium parameters used: $f = 3500.0$ MHz; $\sigma = 2.81$ S/m; $\epsilon_r = 38.7$

Ambient Temperature: 23.3°C; Liquid Temperature: 22.6°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7630; ConvF(7.34, 7.34, 7.34); Calibrated: 2022-03-04
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1305; Calibrated: 2022-04-27
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2022
- Measurement Software: cDASY6 V6.6.0.13926


Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 3.17 W/kg; SAR (10g) = 1.26 W/kg;

Zoom Scan (24.0 mm x 24.0 mm x 22.0 mm): Measurement Grid: 4.0 mm x 4.0 mm x 1.4 mm

Power Drift = 0.04 dB

SAR (1g) = 3.35 W/kg; SAR(10 g) = 1.32 W/kg;

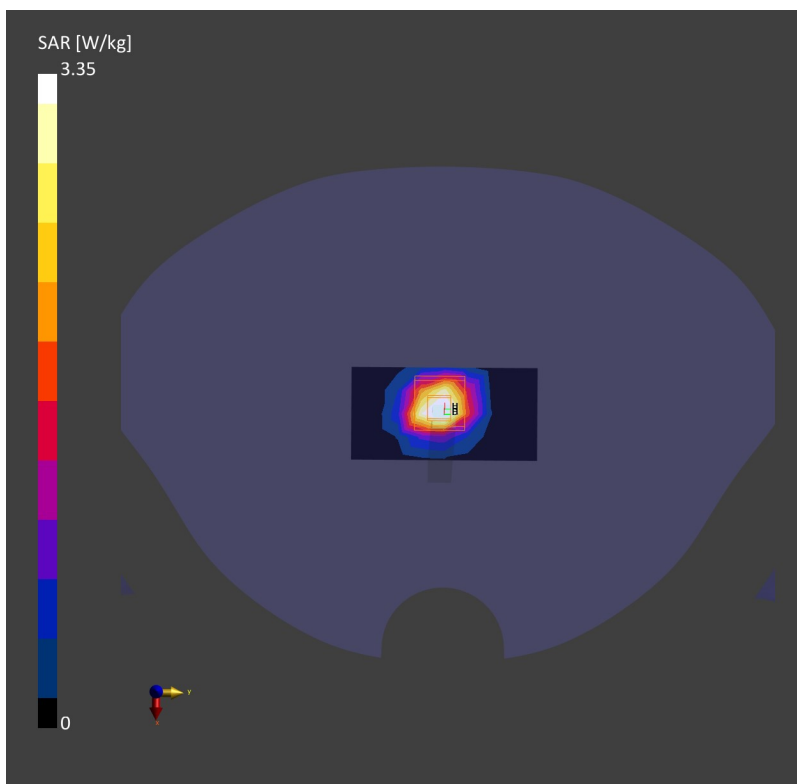

System Check_Head_3700MHz

DUT: D3700V2-SN:1008

Communication System: ; Frequency: 3700.0

Medium: HSL. Medium parameters used: $f = 3700.0$ MHz; $\sigma = 2.99$ S/m; $\epsilon_r = 38.4$

Ambient Temperature: 23.2°C; Liquid Temperature: 22.7°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7630; ConvF(7.33, 7.33, 7.33); Calibrated: 2022-03-04
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1305; Calibrated: 2022-04-27
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2022
- Measurement Software: cDASY6 V6.6.0.13926


Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 3.07 W/kg; SAR (10g) = 1.16 W/kg;

Zoom Scan (24.0 mm x 24.0 mm x 22.0 mm): Measurement Grid: 4.0 mm x 4.0 mm x 1.4 mm

Power Drift = -0.05 dB

SAR (1g) = 3.34 W/kg; SAR(10 g) = 1.22 W/kg;

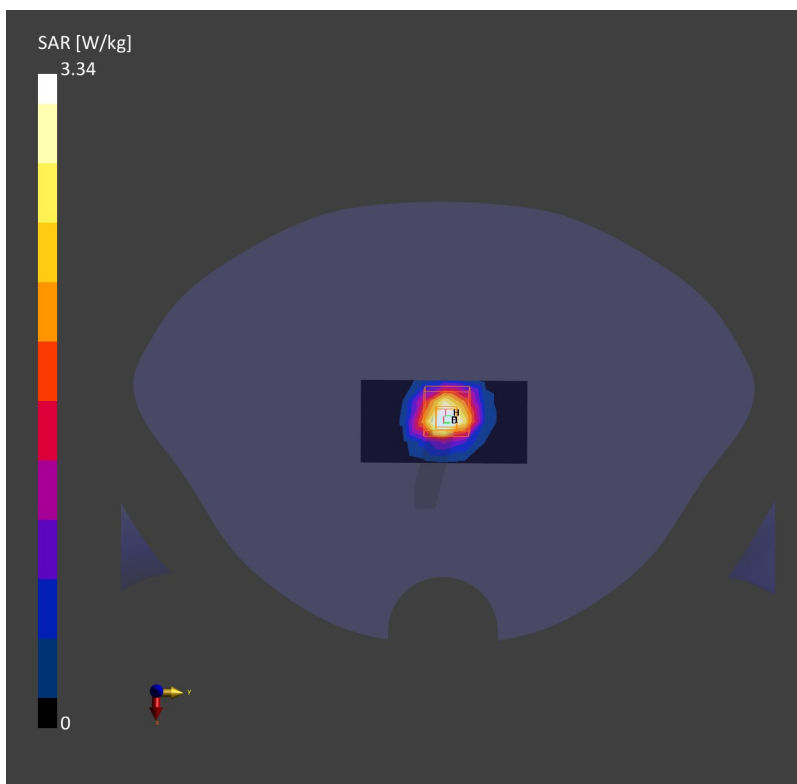

System Check_Head_3900MHz

DUT: D3900V2-SN:1048

Communication System: ; Frequency: 3900.0

Medium: HSL. Medium parameters used: $f = 3900.0$ MHz; $\sigma = 3.31$ S/m; $\epsilon_r = 38.8$

Ambient Temperature: 23.2°C; Liquid Temperature: 22.7°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7764; ConvF(6.66, 6.66, 6.66); Calibrated: 2022-09-30
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1279; Calibrated: 2022-10-26
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2022
- Measurement Software: cDASY6 V6.6.0.13926


Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 3.17 W/kg; SAR (10g) = 1.14 W/kg;

Zoom Scan (24.0 mm x 24.0 mm x 22.0 mm): Measurement Grid: 4.0 mm x 4.0 mm x 1.4 mm

Power Drift = 0.04 dB

SAR (1g) = 3.36 W/kg; SAR(10 g) = 1.20 W/kg;

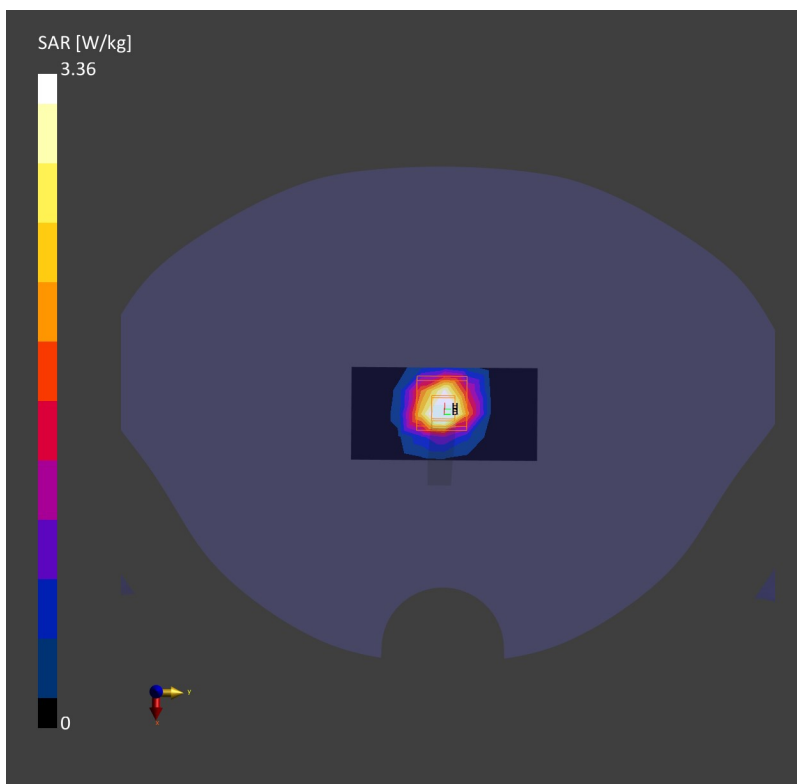

System Check_Head_2450MHz

DUT: D2450V2-SN:1040

Communication System: ; Frequency: 2450.0

Medium: HSL. Medium parameters used: $f = 2450.0$ MHz; $\sigma = 1.74$ S/m; $\epsilon_r = 39.2$

Ambient Temperature: 23.2°C; Liquid Temperature: 22.8°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7764; ConvF(8.25, 8.25, 8.25); Calibrated: 2022-09-30
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1279; Calibrated: 2022-10-26
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2022
- Measurement Software: cDASY6 V6.6.0.13926


Area Scan (40.0 mm x 96.0 mm): Measurement Grid: 12.0 mm x 12.0 mm

SAR (1g) = 2.74 W/kg; SAR (10g) = 1.26 W/kg;

Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm): Measurement Grid: 5.0 mm x 5.0 mm x 5.0 mm

Power Drift = 0.05 dB

SAR (1g) = 2.77 W/kg; SAR (10g) = 1.28 W/kg;

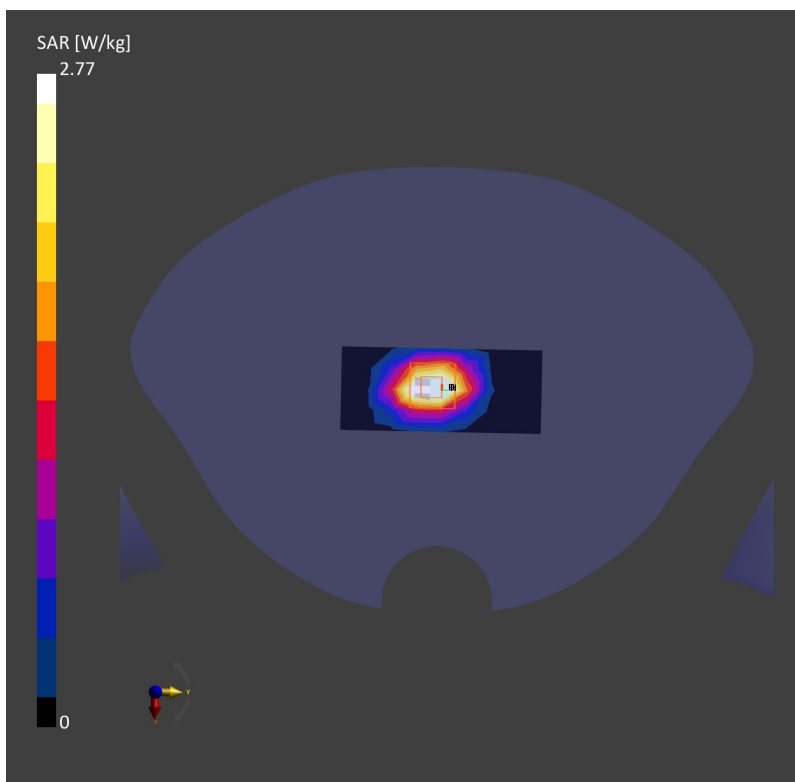

System Check_Head_5250MHz

DUT: D5GHzV2-SN:1341

Communication System: ; Frequency: 5250.0

Medium: HSL. Medium parameters used: $f= 5250.0$ MHz; $\sigma= 4.58$ S/m; $\epsilon_r = 35.7$

Ambient Temperature: 23.2°C; Liquid Temperature: 22.9°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7764; ConvF(5.65, 5.65, 5.65); Calibrated: 2022-09-30
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1279; Calibrated: 2022-10-26
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2022
- Measurement Software: cDASY6 V6.6.0.13926


Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 3.75 W/kg; SAR (10g) = 1.13 W/kg;

Zoom Scan (24.0 mm x 24.0 mm x 22.0 mm): Measurement Grid: 4.0 mm x 4.0 mm x 1.4 mm

Power Drift = 0.09 dB

SAR (1g) = 4.13 W/kg; SAR (10g) = 1.22 W/kg;

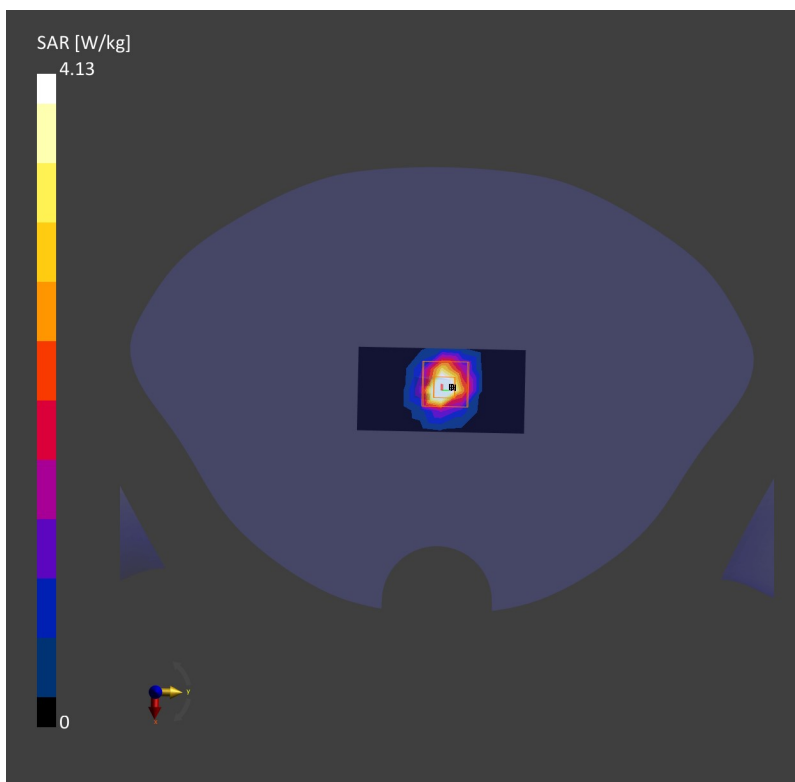

System Check_Head_5600MHz

DUT: D5GHzV2-SN:1341

Communication System: ; Frequency: 5600.0

Medium: HSL. Medium parameters used: $f = 5600.0$ MHz; $\sigma = 4.96$ S/m; $\epsilon_r = 35.0$

Ambient Temperature: 23.1°C; Liquid Temperature: 22.7°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7764; ConvF(4.9, 4.9, 4.9); Calibrated: 2022-09-30
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1279; Calibrated: 2022-10-26
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2022
- Measurement Software: cDASY6 V6.6.0.13926


Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 3.54 W/kg; SAR (10g) = 1.13 W/kg;

Zoom Scan (24.0 mm x 24.0 mm x 22.0 mm): Measurement Grid: 4.0 mm x 4.0 mm x 1.4 mm

Power Drift = 0.05 dB

SAR (1g) = 4.06 W/kg; SAR (10g) = 1.24 W/kg;

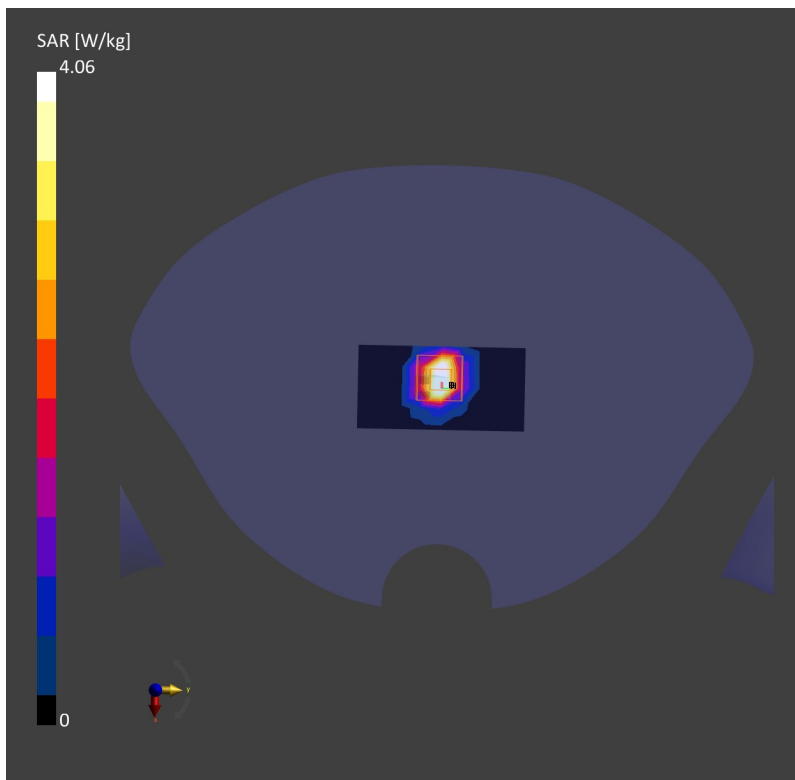

System Check_Head_5750MHz

DUT: D5GHzV2-SN:1341

Communication System: ; Frequency: 5750.0

Medium: HSL. Medium parameters used: $f = 5750.0$ MHz; $\sigma = 5.12$ S/m; $\epsilon_r = 34.8$

Ambient Temperature: 23.3°C; Liquid Temperature: 22.6°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7764; ConvF(5.1, 5.1, 5.1); Calibrated: 2022-09-30
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1279; Calibrated: 2022-10-26
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2022
- Measurement Software: cDASY6 V6.6.0.13926

Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 3.58 W/kg; SAR (10g) = 1.08 W/kg;

Zoom Scan (24.0 mm x 24.0 mm x 22.0 mm): Measurement Grid: 4.0 mm x 4.0 mm x 1.4 mm

Power Drift = 0.05 dB

SAR (1g) = 3.85 W/kg; SAR (10g) = 1.21 W/kg;

