

Appendix C**Tissue Parameters**

SAR measurements were made within 24 hours of the measurement of liquid parameters.

850MHz Body Liquid:**Recipe:**

The following recipe is provided in percentage by weight.

49.8%	water
41.3%	DGBE
8.9%	salt

Date	Freq. (MHz)	Rel. Perm.	Condy (S/m)
03/18/2009	835	54.42	0.981

1900MHz Body Liquid:**Recipe:**

The following recipe is provided in percentage by weight.

69.17%	water
30.29%	DGBE
0.54%	salt

Date	Freq. (MHz)	Rel. Perm.	Condy (S/m)
03/18/09	1880	52.97	1.507
03/18/09	1900	52.65	1.518

2450MHz Body Liquid:**Recipe:**

73.3%	water
12.88%	DGBE
12.88%	triton X-100
0.94%	salt

Date	Freq. (MHz)	Rel. Perm.	Condy (S/m)
03/18/2009	2441	49.33	1.958
03/18/2009	2450	49.25	1.984

Appendix C**Test Equipment**

Instrument description	Supplier / Manufacturer	Model	Serial No.	Calibration (date)	Calibration Due (date)
Bench top Robot	Mitsubishi supplied by IndexSAR	RV-E2	EA1030108	N/A	N/A
SAM Phantom	Upright shell phantom made by Antennessa digitized and mounted by IndexSAR	SAM	03FT26	04/03	N/A
Flat Phantom	IndexSAR	HeadBox_1	N/A	N/A	N/A
Software	IndexSAR	SARA2 v0.420	N/A	N/A	N/A
850 MHz Body Tissue Simulant	Cetecom Inc.	850 Body	N/A	03/18/2009	N/A
1900 MHz Body Tissue Simulant	Cetecom Inc.	1900 Body	N/A	03/18/2009	N/A
2450 MHz Body Tissue Simulant	Cetecom Inc.	2450 Body	N/A	03/18/2009	N/A
835 MHz Dipole	IndexSAR – IEEE 1528 design	IXD-835	081	02/13/2009	02/13/2011
1900 MHz Dipole	IndexSAR – IEEE 1528 design	IXDA-188	016	02/13/2009	02/13/2011
2450 MHz Dipole	IndexSAR – IEEE 1528 design	IXD-245	228	02/13/2009	02/13/2011
Directional coupler	Werlatone	C6529	11249	N/A	N/A
RF Amplifier	Vectawave	VTL5400	N/A	N/A	N/A
SAR Probe	IndexSAR	IXP-030	S/N M0024	02/05/2009	02/05/2010
Dielectric Measurement Kit	IndexSAR	Di-Line	N/A	N/A	N/A

Appendix C

Equipment Calibration/Performance Documents:

Attached:

SAR Probe Calibration Report M0024

835 MHz Dipole Calibration Report 081

1880 MHz Dipole Calibration Report 016

2450 MHz Dipole Calibration Report 228




IMMERSIBLE SAR PROBE

CALIBRATION REPORT

Part Number: IXP – 030

S/N M0024

February 2009

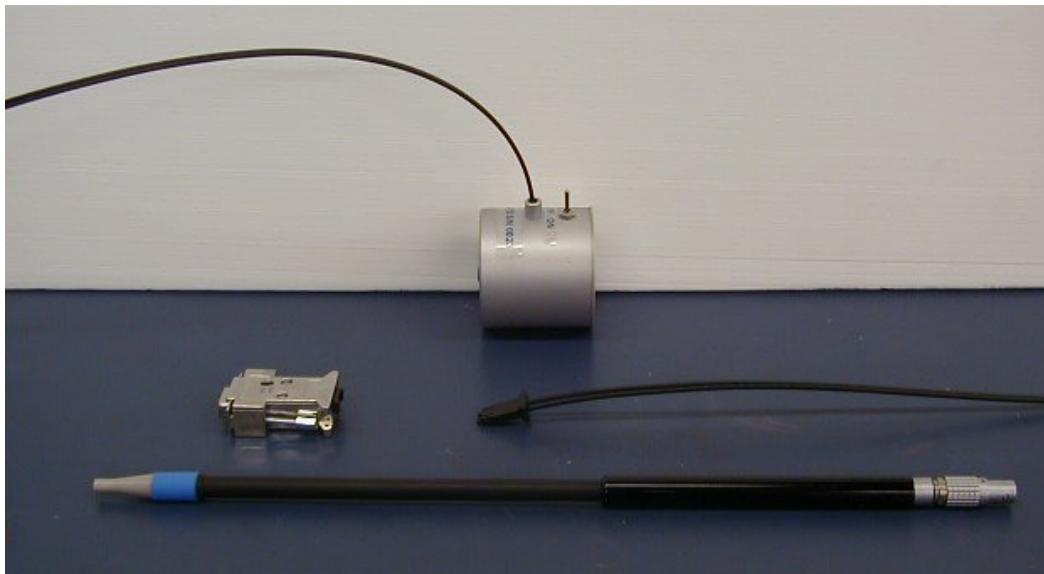

Indexsar Limited
Oakfield House
Cudworth Lane
Newdigate
Surrey RH5 5BG
Tel: +44 (0) 1306 632 870
Fax: +44 (0) 1306 631 834
e-mail: enquiries@indexsar.com

Reproduction of this report is authorized by Indexsar Ltd provided the report is reproduced in its entirety



Indexsar Limited
Oakfield House
Cudworth Lane
Newdigate
Surrey RH5 5BG
Tel: +44 (0) 1306 632 870
Fax: +44 (0) 1306 631 834
e-mail: enquiries@indexsar.com

Calibration Certificate 0902/M0024
Date of Issue: 5th February 2008
Immersible SAR Probe

Type:	IXP-030
Manufacturer:	IndexSAR, UK
Serial Number:	M0024
Place of Calibration:	IndexSAR, UK
Date of Receipt of Probe:	14 th January 2009
Calibration Dates:	21 st January — 4 th February 2009
Customer:	Cetecom

IndexSAR Ltd hereby declares that the IXP-030 Probe named above has been calibrated for conformity to the IEEE 1528 and BSEN 62209-1 standards using the methods described in this calibration document. Where applicable, the standards used in the calibration process are traceable to the UK's National Physical Laboratory.

Calibrated by:	 A. Brinklow	Technical Manager
Approved by:	 M.J. Maini	Director

Please keep this certificate with the calibration document. When the probe is sent for a calibration check, please include the calibration document.

INTRODUCTION

This Report presents measured calibration data for a particular Indexsar SAR probe (S/N M0024) only and describes the procedures used for characterisation and calibration.

Indexsar probes are characterised using procedures that, where applicable, follow the recommendations of BSEN 622009-1 [Ref 1] & IEEE [Ref 2] standards. The procedures incorporate techniques for probe linearisation, isotropy assessment and determination of liquid factors (conversion factors). Calibrations are determined by comparing probe readings with analytical computations in canonical test geometries (waveguides) using normalised power inputs.

Each step of the calibration procedure and the equipment used is described in the sections below.

CALIBRATION PROCEDURE

1. Objectives

The calibration process comprises four stages

- 1) Determination of the channel sensitivity factors which optimise the probe's overall rotational isotropy in 2450MHz brain fluid
- 2) Determination of the channel sensitivity factors and angular offset of the X channel which together optimise the probe's spherical isotropy in 2450MHz brain fluid
- 3) Numerical combination of the two sets of channel sensitivity factors to give both acceptable rotational isotropy and acceptable spherical isotropy values
- 4) At each frequency of interest, application of these channel sensitivity factors to model the exponential decay of SAR in a waveguide fluid cell, and hence derive the liquid conversion factors at that frequency

2. Probe output

The probe channel output signals are linearised in the manner set out in Refs [1] and [2]. The following equation is utilized for each channel:

$$U_{lin} = U_{o/p} + U_{o/p}^2 / DCP \quad (1)$$

where U_{lin} is the linearised signal, $U_{o/p}$ is the raw output signal in mV and DCP is the diode compression potential in similar voltage units.

DCP is determined from fitting equation (1) to measurements of U_{lin} versus source feed power over the full dynamic range of the probe. The DCP is a characteristic of the Schottky diodes used as the sensors. For the IXP-030 probes with CW signals the DCP values are typically 100mV.

Conventionally, when used in conjunction with the SARA2 test jig, all measured voltages and voltage-derived values are quoted in units of V*200

eg a DCP value of 100mV corresponds to 20 in V*200 units. Conversely, in the SARA C and HACSAR measurement systems, unmodified mV values are used throughout. As a consequence, the cal factors for this probe are listed in two tables, one for SARA2 and one for SARA C / HACSAR.

In turn, measurements of E-field are determined using the following equation (where output voltages are also in units of mV):

$$\begin{aligned} E_{liq}^2 \text{ (V/m)} = & U_{linx} * \text{Air Factor}_x * \text{Liq Factor}_x \\ & + U_{liny} * \text{Air Factor}_y * \text{Liq Factor}_y \\ & + U_{linz} * \text{Air Factor}_z * \text{Liq Factor}_z \end{aligned} \quad (2)$$

Here, “Air Factor” represents each channel’s sensitivity, while “Liq Factor” represents the enhancement in signal level when the probe is immersed in tissue-simulant liquids at each frequency of interest.

3. Selecting channel sensitivity factors to optimise isotropic response

After manufacture, the first stage of the calibration process is to balance the three channels’ Air Factor values, thereby optimising the probe’s overall axial response (“rotational isotropy”).

To do this, a 2450MHz waveguide containing head-fluid simulant is selected. Like all waveguides used during probe calibration, this particular waveguide contains two distinct sections: an air-filled launcher section, and a liquid cell section, separated by a dielectric matching window designed to minimise reflections at the air-liquid interface.

The waveguide stands in an upright position and the liquid cell section is filled with 2450MHz brain fluid to within 10 mm of the open end. The depth of liquid ensures there is negligible radiation from the waveguide open top and that the probe calibration is not influenced by reflections from nearby objects.

During the measurement, a TE_{01} mode is launched into the waveguide by means of an N-type-to-waveguide adapter. The probe is then lowered vertically into the liquid until the tip is exactly 10mm above the centre of the dielectric window. This particular separation ensures that the probe is operating in a part of the waveguide where boundary corrections are not necessary.

Care must also be taken that the probe tip is centred while rotating.

The exact power applied to the input of the waveguide during this stage of the probe calibration is immaterial since only relative values are of interest while the probe rotates. However, the power must be sufficiently above the noise floor and free from drift.

The dedicated Indexsar calibration software rotates the probe in 10 degree steps about its axis, and at each position, an Indexsar ‘Fast’ amplifier samples the probe channels 500 times per second for 0.4 s. The raw $U_{o/p}$ data from each sample are packed into 10 bytes and transmitted back to the PC

controller via an optical cable. U_{linx} , U_{liny} and U_{linz} are derived from the raw $U_{o/p}$ values and written to an Excel template.

Once data have been collected from a full probe rotation, the Air Factors are adjusted using a special Excel Solver routine to equalise the output from each channel and hence minimise the rotational isotropy. This automated approach to optimisation removes the effect of human bias.

Figure 6 represents the output from each diode sensor as a function of probe rotation angle.

4. Measurement of Spherical Isotropy

The setup for measuring the probe's spherical isotropy is shown in Figure 2.

A box phantom containing 2450MHz head fluid is irradiated by a vertically-polarised, tuned dipole, mounted to the side of the phantom on the robot's seventh axis. During calibration, the spherical response is generated by rotating the probe about its axis in 20 degree steps and changing the dipole polarisation in 10 degree steps.

By using the VPM technique discussed below, an allowance can also be made for the effect of E-field gradient across the probe's spatial extent. This permits values for the probe's effective tip radius and X-channel angular offset to be modelled until the overall spherical isotropy figure is optimised.

The dipole is connected to a signal generator and amplifier via a directional coupler and power meter. As with the determination of rotational isotropy, the absolute power level is not important as long as it is stable.

The probe is positioned within the fluid so that its sensors are at the same vertical height as the centre of the source dipole. The line joining probe to dipole should be perpendicular to the phantom wall, while the horizontal separation between the two should be small enough for VPM corrections to be applicable, without encroaching near the boundary layer of the phantom wall. VPM corrections require a knowledge of the fluid skin depth. This is measured during the calibration by recording the E-field strength while systematically moving the probe away from the dipole in 2mm steps over a 20mm range.

The directionality of the orthogonally-arranged sensors can be checked by analysing the data using dedicated Indexsar software, which displays the data in 3D format, a representative image of which is shown in Figure 3. The left-hand side of this diagram shows the individual channel outputs after linearisation (see above). The program uses these data to balance the channel outputs and then applies an optimisation process, which makes fine adjustments to the channel factors for optimum isotropic response.

5. Determination of Conversion (“Liquid”) Factors at each frequency of interest

A lookup table of conversion factors for a probe allows a SAR value to be derived at the measured frequencies, and for either brain or body fluid-simulant.

The method by which the conversion factors are assessed is based on the comparison between measured and analytical rates of decay of SAR with height above a dielectric window. This way, not only can the conversion factors for that frequency/fluid combination be determined, but an allowance can also be made for the scale and range of boundary layer effects.

The theoretical relationship between the SAR at the cross-sectional centre of the lossy waveguide as a function of the longitudinal distance (z) from the dielectric separator is given by Equation 3:

$$SAR(z) = \frac{4(P_f - P_b)}{\rho ab\delta} e^{-2z/\delta} \quad (3)$$

Here, the density ρ is conventionally assumed to be 1000 kg/m³, ab is the cross-sectional area of the waveguide, and P_f and P_b are the forward and reflected power inside the lossless section of the waveguide, respectively. The penetration depth δ (which is the reciprocal of the waveguide-mode attenuation coefficient) is a property of the lossy liquid and is given by Equation (4).

$$\delta = \left[\text{Re} \left\{ \sqrt{(\pi/a)^2 + j\omega\mu_o(\sigma + j\omega\epsilon_o\epsilon_r)} \right\} \right]^{-1} \quad (4)$$

where σ is the conductivity of the tissue-simulant liquid in S/m, ϵ_r is its relative permittivity, and ω is the radial frequency (rad/s). Values for σ and ϵ_r are obtained prior to each waveguide test using an Indexsar DiLine measurement kit, which uses the TEM method as recommended in [2]. σ and ϵ_r are both temperature- and fluid-dependent, so are best measured using a sample of the tissue-simulant fluid immediately prior to the actual calibration.

Wherever possible, all DiLine and calibration measurements should be made in the open laboratory at 22 \pm 2.0°C; if this is not possible, the values of σ and ϵ_r should reflect the actual temperature. Values employed for calibration are listed in the tables below.

By ensuring the liquid height in the waveguide is at least three penetration depths, reflections at the upper surface of the liquid are negligible. The power absorbed in the liquid is therefore determined solely from the waveguide forward and reflected power.

Different waveguides are used for 835/900MHz, 1800/1900MHz, 2100/2450MHz and 5000/6000MHz measurements. Table A.1 of [1] can be used for designing calibration waveguides with a return loss greater than 20

dB at the most important frequencies used for personal wireless communications, and better than 15dB for frequencies greater than 5GHz. Values for the penetration depth for these specific fixtures and tissue-simulating mixtures are also listed in the aforementioned Table A.1.

According to [1], this calibration technique provides excellent accuracy, with standard uncertainty of less than 3.6% depending on the frequency and medium. The calibration itself is reduced to power measurements traceable to a standard calibration procedure. The practical limitation to the frequency band of 800 to 5800 MHz because of the waveguide size is not severe in the context of compliance testing.

During calibration, the probe is lowered carefully until it is just touching the cross-sectional centre of the dielectric window. 200 samples are then taken and written to an Excel template file before moving the probe vertically upwards. This cycle is repeated 150 times. The vertical separation between readings is determined from practical considerations of the expected SAR decay rate, and range from 0.2mm steps at low frequency, through 0.1mm at 2450MHz, down to 0.05mm at 5GHz.

Once the data collection is complete, a Solver routine is run which optimises the measured-theoretical fit by varying the conversion factor, and the boundary correction size and range.

For 450 MHz calibrations, a slightly different technique must be used — the equatorial response of the probe-under-test is compared with the equivalent response of a probe whose 450MHz characteristics have already been determined by NPL. The conversion factor of the probe-under-test can then be deduced.

VPM (Virtual Probe Miniaturisation)

SAR probes with 3 diode-sensors in an orthogonal arrangement are designed to display an isotropic response when exposed to a uniform field. However, the probes are ordinarily used for measurements in non-uniform fields and isotropy is not assured when the field gradients are significant compared to the dimensions of the tip containing the three orthogonally-arranged dipole sensors.

It becomes increasingly important to assess the effects of field gradients on SAR probe readings when higher frequencies are being used. For Indexsar IXP-050 probes, which are of 5mm tip diameter, field gradient effects are minor at GSM frequencies, but are major above 5GHz. Smaller probes are less affected by field gradients and so probes, which are significantly less than 5mm diameter, would be better for applications above 5GHz.

The IndexSAR report IXS0223 [4] describes theoretical and experimental studies to evaluate the issues associated with the use of probes at arbitrary angles to surfaces and field directions. Based upon these studies, the procedures and uncertainty analyses referred to in [2] are addressed for the full range of probe presentation angles.

In addition, generalized procedures for correcting for the finite size of immersible SAR probes are developed. Use of these procedures enables application of schemes for virtual probe miniaturization (VPM) – allowing probes of a specific size to be used where physically-smaller probes would otherwise be required.

Given the typical dimensions of 3-channel SAR probes presently available, use of the VPM technique extends the satisfactory measurement range to higher frequencies.

CALIBRATION FACTORS MEASURED FOR PROBE S/N M0024

The probe was calibrated at 835, 900, 1800, 1900, 2100 and 2450 MHz in liquid samples representing brain and body liquid at these frequencies. In addition, calibration measurements in brain liquid were performed every 100MHz from 5100 MHz to 5800 MHz inclusive.

The calibration was for CW signals only, and the axis of the probe was parallel to the direction of propagation of the incident field i.e. end-on to the incident radiation. The axial isotropy of the probe was measured by rotating the probe about its axis in 10 degree steps through 360 degrees in this orientation.

The reference point for the calibration is in the centre of the probe's cross-section at a distance of 1.7 mm from the probe tip in the direction of the probe amplifier. A value of 1.7 mm should be used for the tip to sensor offset distance in the software. The distance of 1.7mm for assembled probes has been confirmed by taking X-ray images of the probe tips (eg see Figure 10).

It is important that the diode compression point and air factors used in the software are the same as those quoted in the results tables, as these are used to convert the diode output voltages to a SAR value.

CALIBRATION EQUIPMENT

The table on page 25 indicates the calibration status of all test equipment used during probe calibration.

MEASUREMENT UNCERTAINTIES

A complete measurement uncertainty analysis for the SARA2 measurement system has been published in Reference [3]. Table 10 from that document is re-created below, and lists the uncertainty factors associated just with the calibration of probes.

Source of uncertainty	Uncertainty value $\pm \%$	Probability distribution	Divisor	c_i	Standard uncertainty $u_i \pm \%$	v_i or v_{eff}
Incident or forward power	5.743	N	1.00	1	5.743	∞
Refelected power	5.773	N	1.00	1	5.773	∞
Liquid conductivity	1.120	N	1.00	1	1.120	∞
Liquid permittivity	1.085	N	1.00	1	1.085	∞
Field homogeneity	0.002	R	1.73	1	0.001	∞
Probe positioning: +/-0.05mm	0.55	R	1.73	1	0.318	
Influence on Probe pos: 11%/mm						
Field probe linearity	4.7	R	1.73	1	2.714	∞
Combined standard uncertainty		RSS			8.729	

At the 95% confidence level, therefore, the expanded uncertainty is 17.1%

SUMMARY OF CALIBRATION FACTORS
 (for use with SARA C & HACSAR)

	X	Y	Z	Units
Air Factors	514.6	452.4	473.1	(V/m) ² /mV
CW DCPS	100	100	100	mV

Freq (MHz)	Head			Body		
	SAR Conv Factor	Bound Corrn. – f(0)	Bound Corrn. – d(mm)	SAR Conv Factor	Bound Corrn. – f(0)	Bound Corrn. – d(mm)
835	0.391	2.0	0.7	0.395	1.9	0.7
900	0.385	1.5	0.8	0.395	2.0	0.7
1800	0.449	2.3	0.6	0.456	2.8	0.6
1900	0.449	2.6	0.6	0.476	2.7	0.6
2100	0.465	1.7	0.7	0.487	1.8	0.7
2450	0.470	1.4	0.8	0.487	1.9	0.7
5100	0.523	0.7	1.3	0.475	0.7	1.2
5200	0.465	0.9	1.1	0.550	0.7	1.2
5300	0.472	0.7	1.5	0.550	0.7	1.2
5400	±0.544	0.6	1.8	±0.450	0.7	1.2
5500	±0.458	0.7	1.6	±0.600	0.8	1.2
5600	0.461	0.7	1.6	0.540	0.8	1.2
5700	0.497	0.7	1.5	0.540	0.8	1.2
5800	0.501	0.7	1.7	0.550	0.8	1.2

Miscellaneous	
Sensor offset	1.7 mm
X Ch. Angle to red dot	-21.5°

Measured Isotropy at 900MHz	(+/-) dB
Spherical Isotropy	0.64
Axial Isotropy	0.05

‡ Note: These values may be anomalous due to some waveguide characteristic – a smoothed response between 5200MHz and 5800MHz may be more appropriate.

SUMMARY OF CALIBRATION FACTORS
(for use with SARA 2)

	X	Y	Z	Units
Air Factors	2573	2262	2365	$(V/m)^2/(V^*200)$
CW DCPS	20	20	20	V^*200

Freq (MHz)	Head			Body		
	SAR Conv Factor	Bound Corrn. – f(0)	Bound Corrn. – d(mm)	SAR Conv Factor	Bound Corrn. – f(0)	Bound Corrn. – d(mm)
835	0.391	2.0	0.7	0.395	1.9	0.7
900	0.385	1.5	0.8	0.395	2.0	0.7
1800	0.449	2.3	0.6	0.456	2.8	0.6
1900	0.449	2.6	0.6	0.476	2.7	0.6
2100	0.465	1.7	0.7	0.487	1.8	0.7
2450	0.470	1.4	0.8	0.487	1.9	0.7
5100	0.523	0.7	1.3	0.475	0.7	1.2
5200	0.465	0.9	1.1	0.550	0.7	1.2
5300	0.472	0.7	1.5	0.550	0.7	1.2
5400	±0.544	0.6	1.8	±0.450	0.7	1.2
5500	±0.458	0.7	1.6	±0.600	0.8	1.2
5600	0.461	0.7	1.6	0.540	0.8	1.2
5700	0.497	0.7	1.5	0.540	0.8	1.2
5800	0.501	0.7	1.7	0.550	0.8	1.2

Miscellaneous	
Tip radius	1.0 mm
X Ch. Angle to red dot	-21.5°

Measured Isotropy at 900MHz	(+/-) dB
Spherical Isotropy	0.64
Axial Isotropy	0.05

‡ Note: These values may be anomalous due to some waveguide characteristic – a smoothed response between 5200MHz and 5800MHz may be more appropriate.

PROBE SPECIFICATIONS

Indexsar probe M0024, along with its calibration, is compared with BSEN 62209-1 and IEEE standards recommendations (Refs [1] and [2]) in the Tables below. A listing of relevant specifications is contained in the tables below:

Dimensions	S/N M0024	BSEN [1]	IEEE [2]
Overall length (mm)	350		
Tip length (mm)	10		
Body diameter (mm)	12		
Tip diameter (mm)	3.1	8	8
Distance from probe tip to dipole centers (mm)	1.7		

Dynamic range	S/N M0024	BSEN [1]	IEEE [2]
Minimum (W/kg)	0.01	<0.02	0.01
Maximum (W/kg)	>100	>100	100
N.B. only measured to > 100 W/kg on representative probes			

Isotropy (measured at 900MHz)	S/N M0024	BSEN [1]	IEEE [2]
Axial rotation with probe normal to source (+/- dB)	0.05 (See table above)	0.5	0.25
Spherical isotropy covering all orientations to source (+/- dB)	0.64	1.0	0.50

Construction	Each probe contains three orthogonal dipole sensors arranged on a triangular prism core, protected against static charges by built-in shielding, and covered at the tip by PEEK cylindrical enclosure material. Outer case materials are PEEK and adhesive-lined heat-shrink sleeving.
Chemical resistance	Tested to be resistant to TWEEN20 and sugar/salt-based simulant liquids, but probes should be removed, cleaned and dried when not in use. NOT recommended for use with glycol or soluble oil-based liquids.

REFERENCES

- [1] BSEN 62209-1:2006. Human exposure to radio frequency fields from hand-held and body-mounted wireless communication devices — Human models, instrumentation, and procedures — Part 1: Procedure to determine the specific absorption rate (SAR) for hand-held devices used in close proximity to the ear (frequency range of 300 MHz to 3 GHz)
- [2] IEEE 1528, 2003 Recommended Practice for Determining the Peak Spatial-Average Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques
- [3] Indexsar Report IXS-0300, October 2007. Measurement uncertainties for the SARA2 system assessed against the recommendations of BS EN 62209-1:2006
- [4] Indexsar Report IXS-0223, May 2003. Compensating for the finite size of SAR probes used in electric field gradients

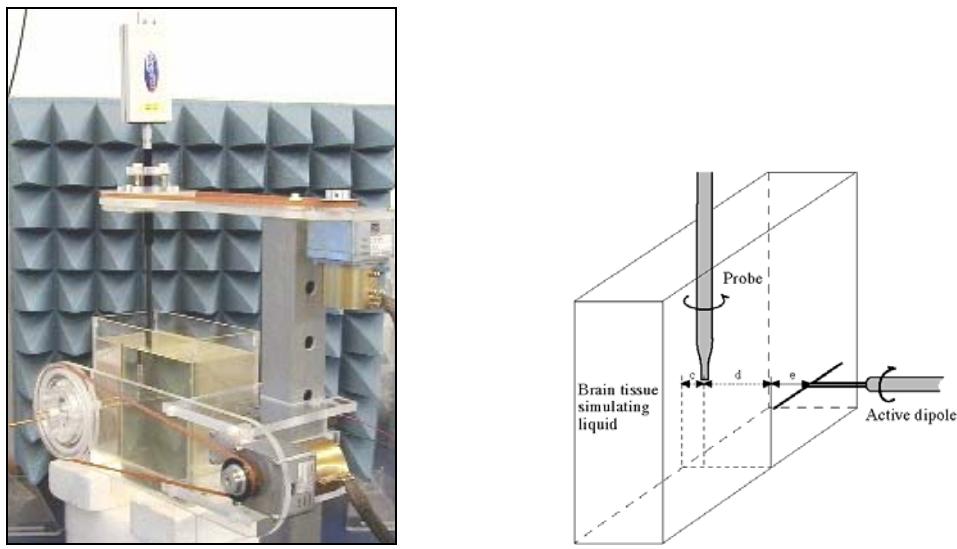


Figure 1. Spherical isotropy jig showing probe, dipole and box filled with simulated brain liquid (see Ref [2], Section A.5.2.1)

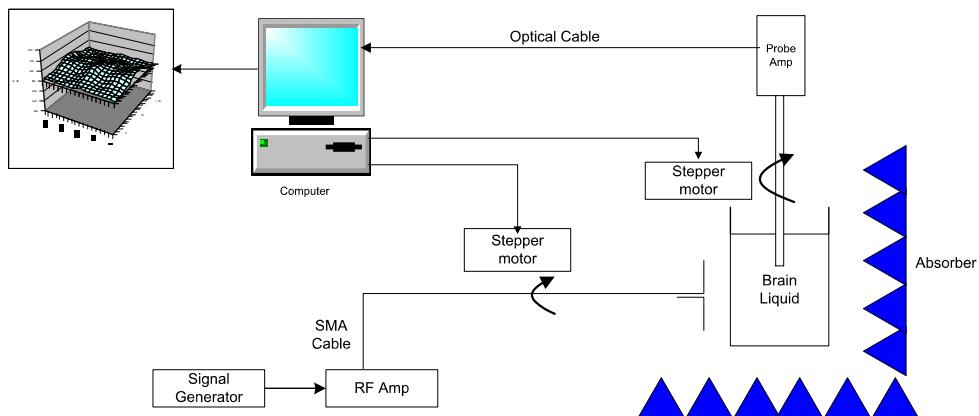


Figure 2 Schematic diagram of the test geometry used for isotropy determination

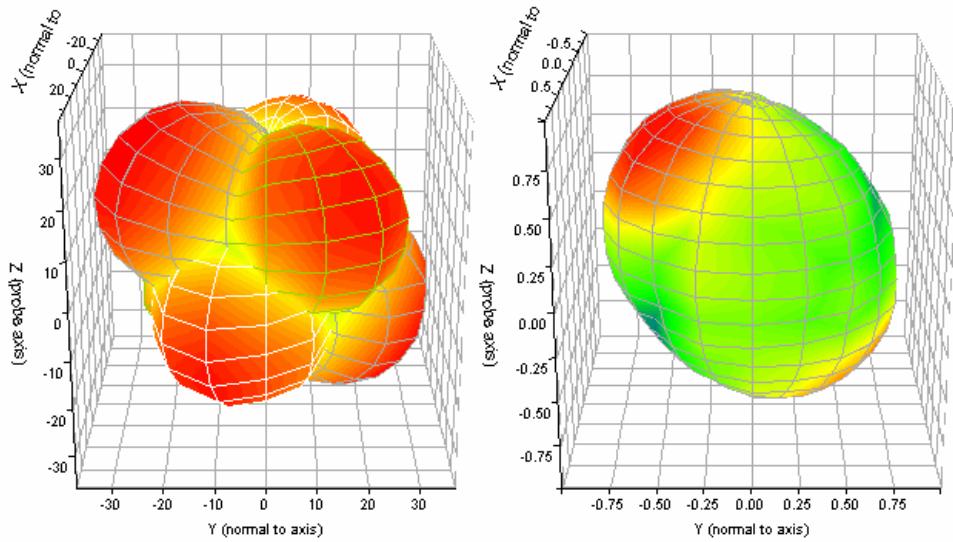


Figure 3 Graphical representation of probe M0024's response to fields applied from each direction. The diagram on the left shows the individual response characteristics of each of the three channels and the diagram on the right shows the resulting probe sensitivity sensitivity in each direction. The colour range in the figure images the lowest values as blue and the maximum values as red. For probe S/N M0024, this range is (+/-) 0.64dB.

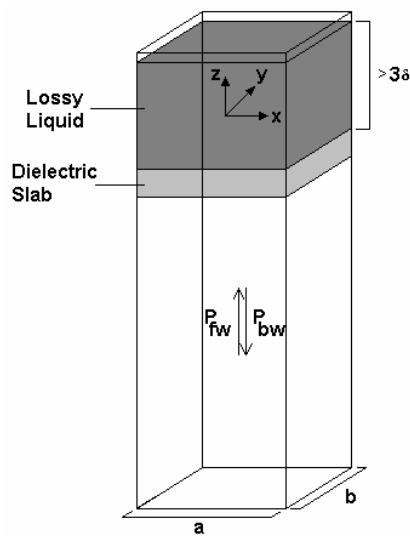


Figure 4 Geometry used for waveguide calibration (after Ref [2]. Section A.3.2.2)

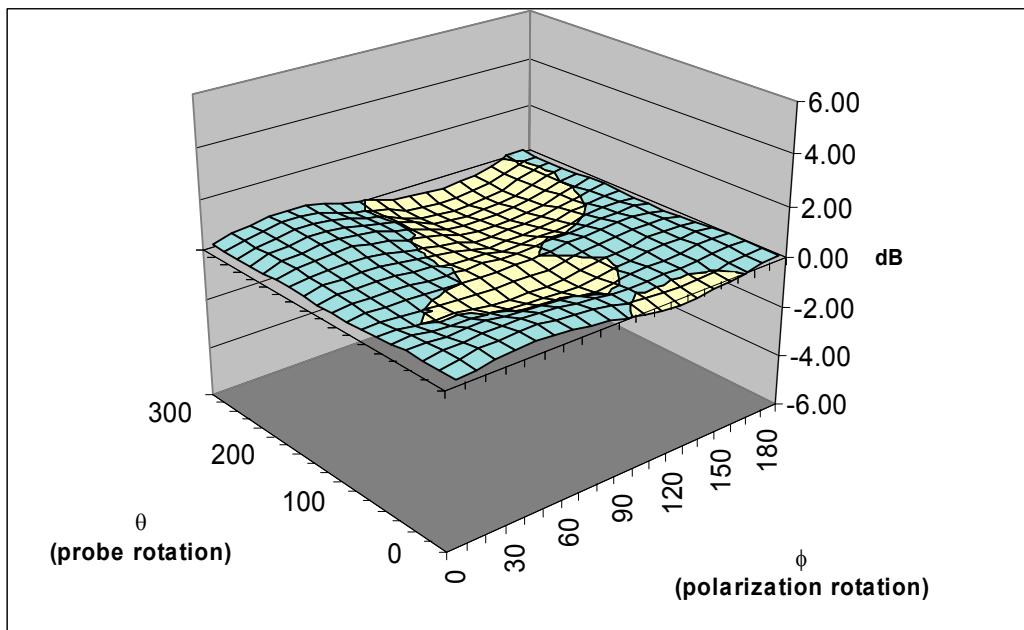


Figure 5 Surface Isotropy diagram of IXP-030 Probe S/N M0024 at 2450MHz after VPM (rotational isotropy axial +/-0.05dB, spherical isotropy +/-0.64dB)

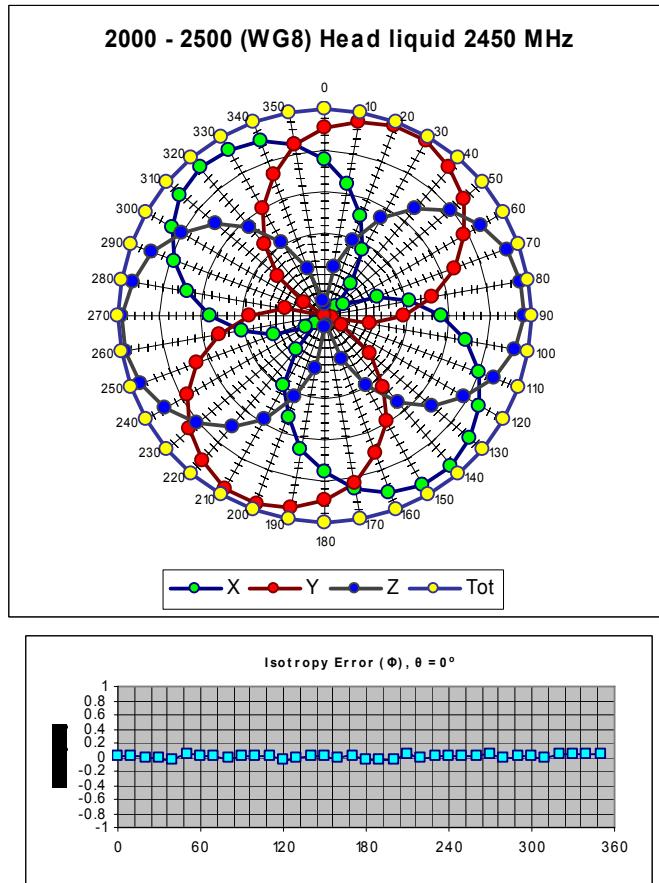


Figure 6. The rotational isotropy of probe S/N M0024 obtained by rotating the probe in a liquid-filled waveguide at 2450 MHz.

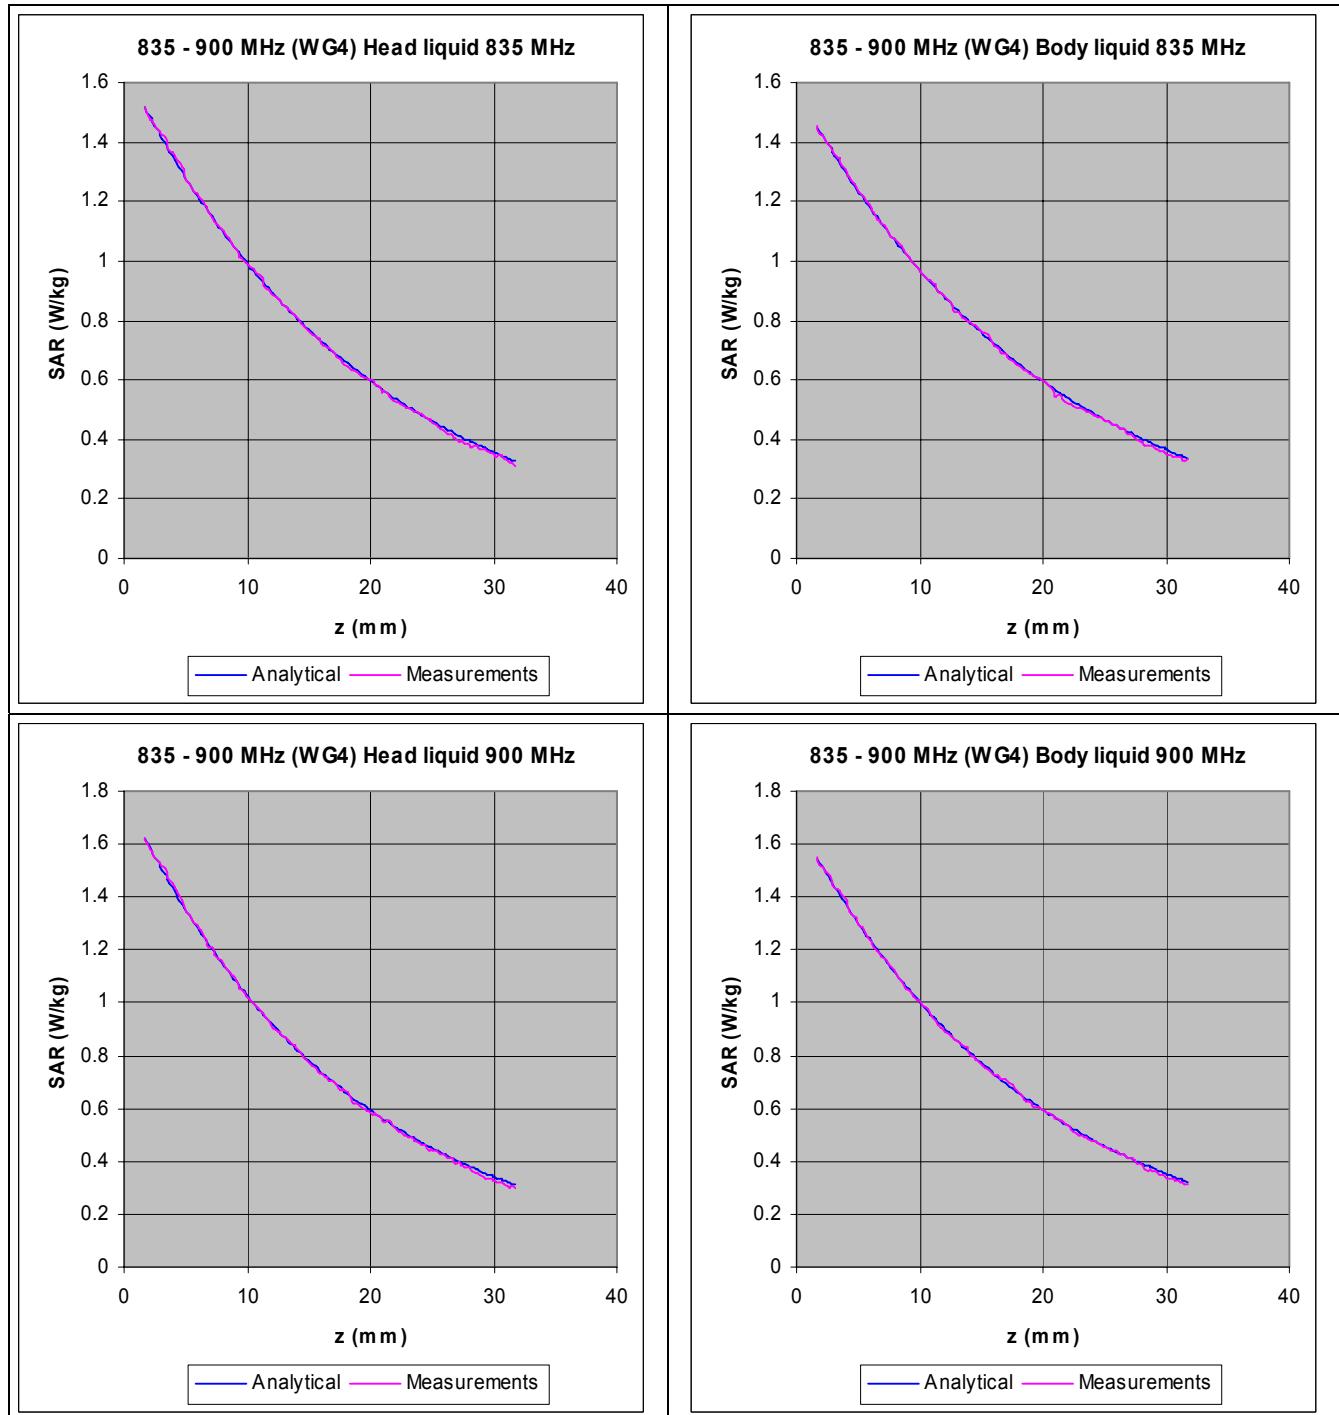
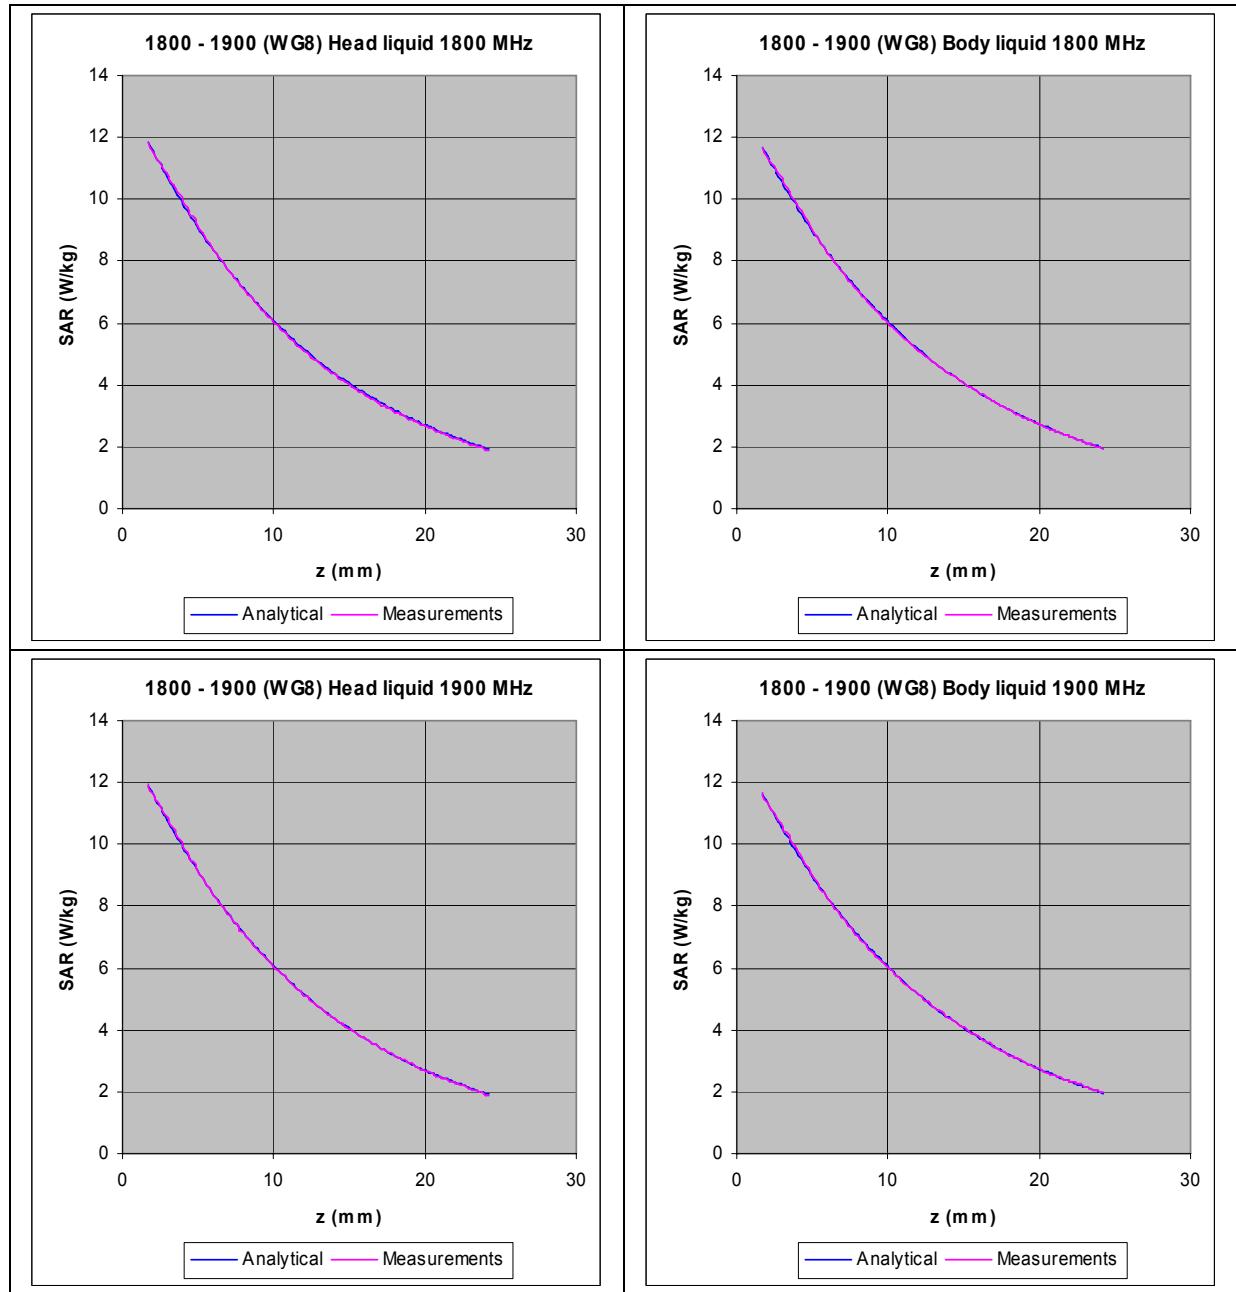


Figure 7. The measured SAR decay function along the centreline of the WG4 waveguide with conversion factors adjusted to fit to the theoretical function for the particular dimension, frequency, power and liquid properties employed.



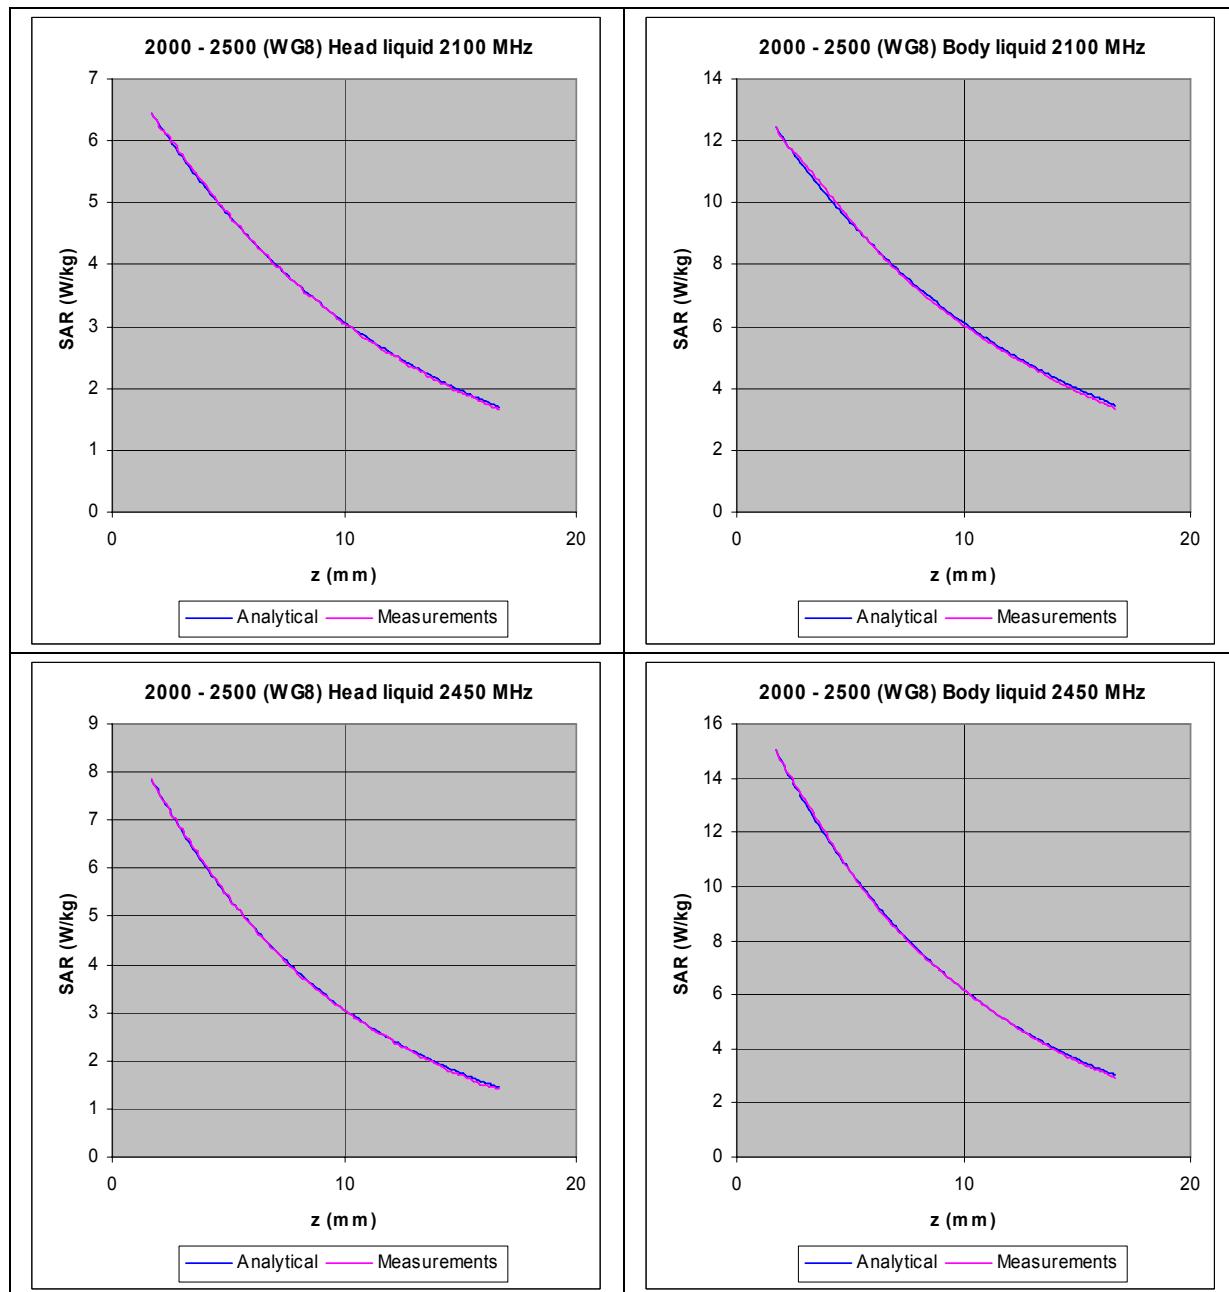
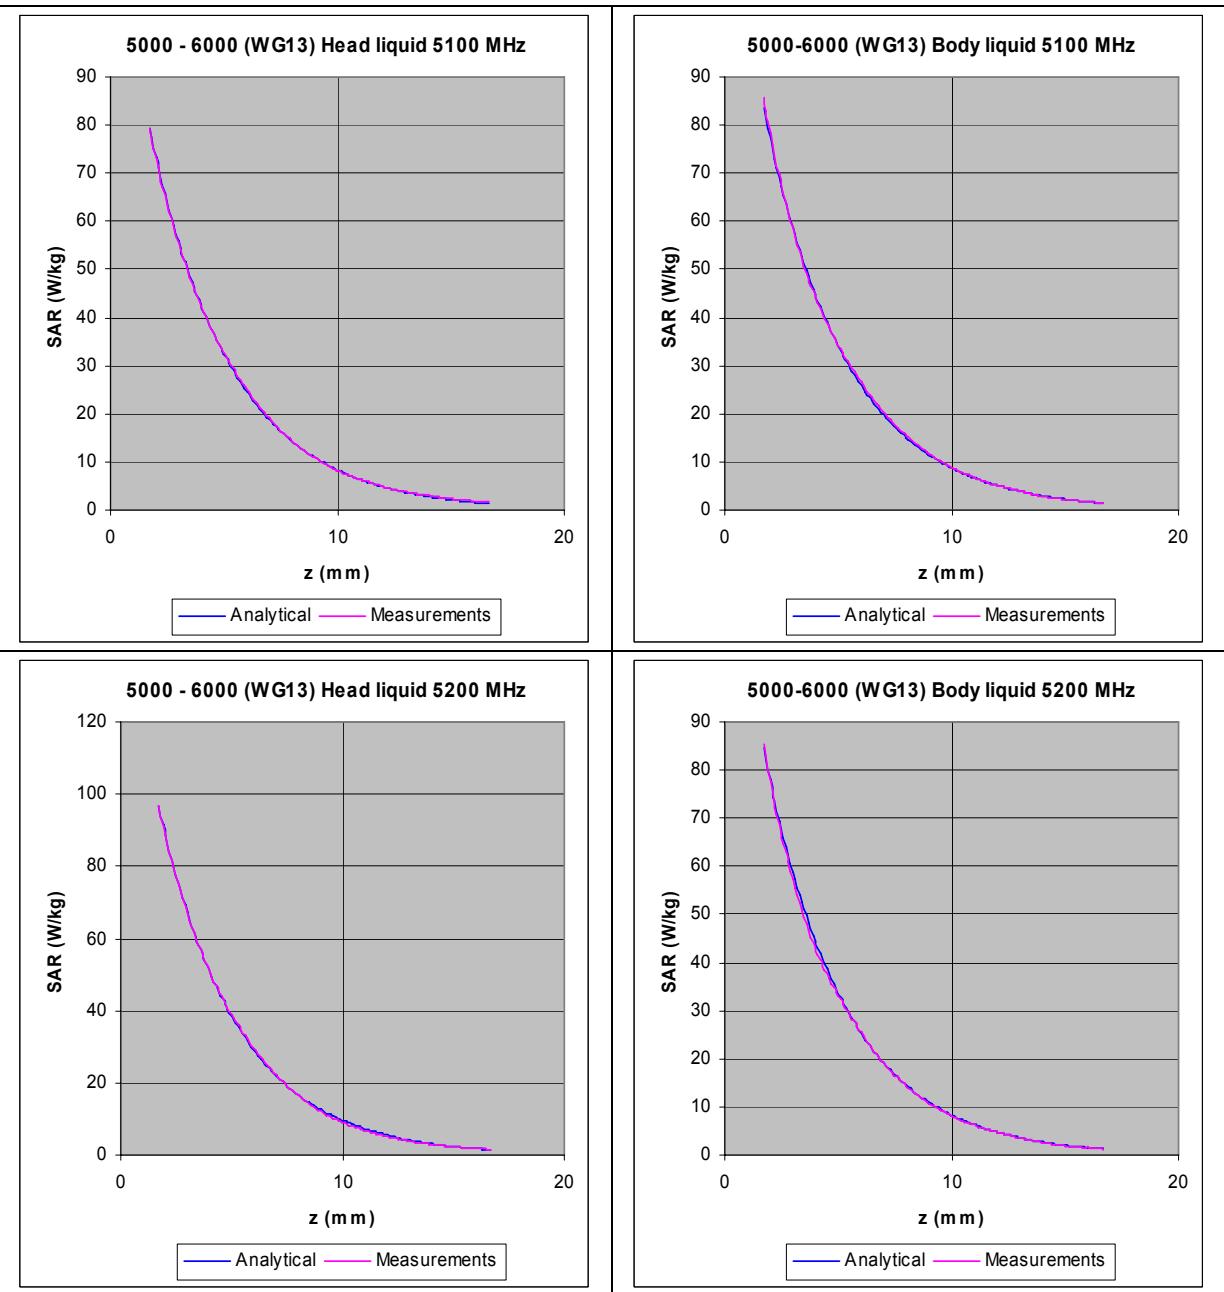
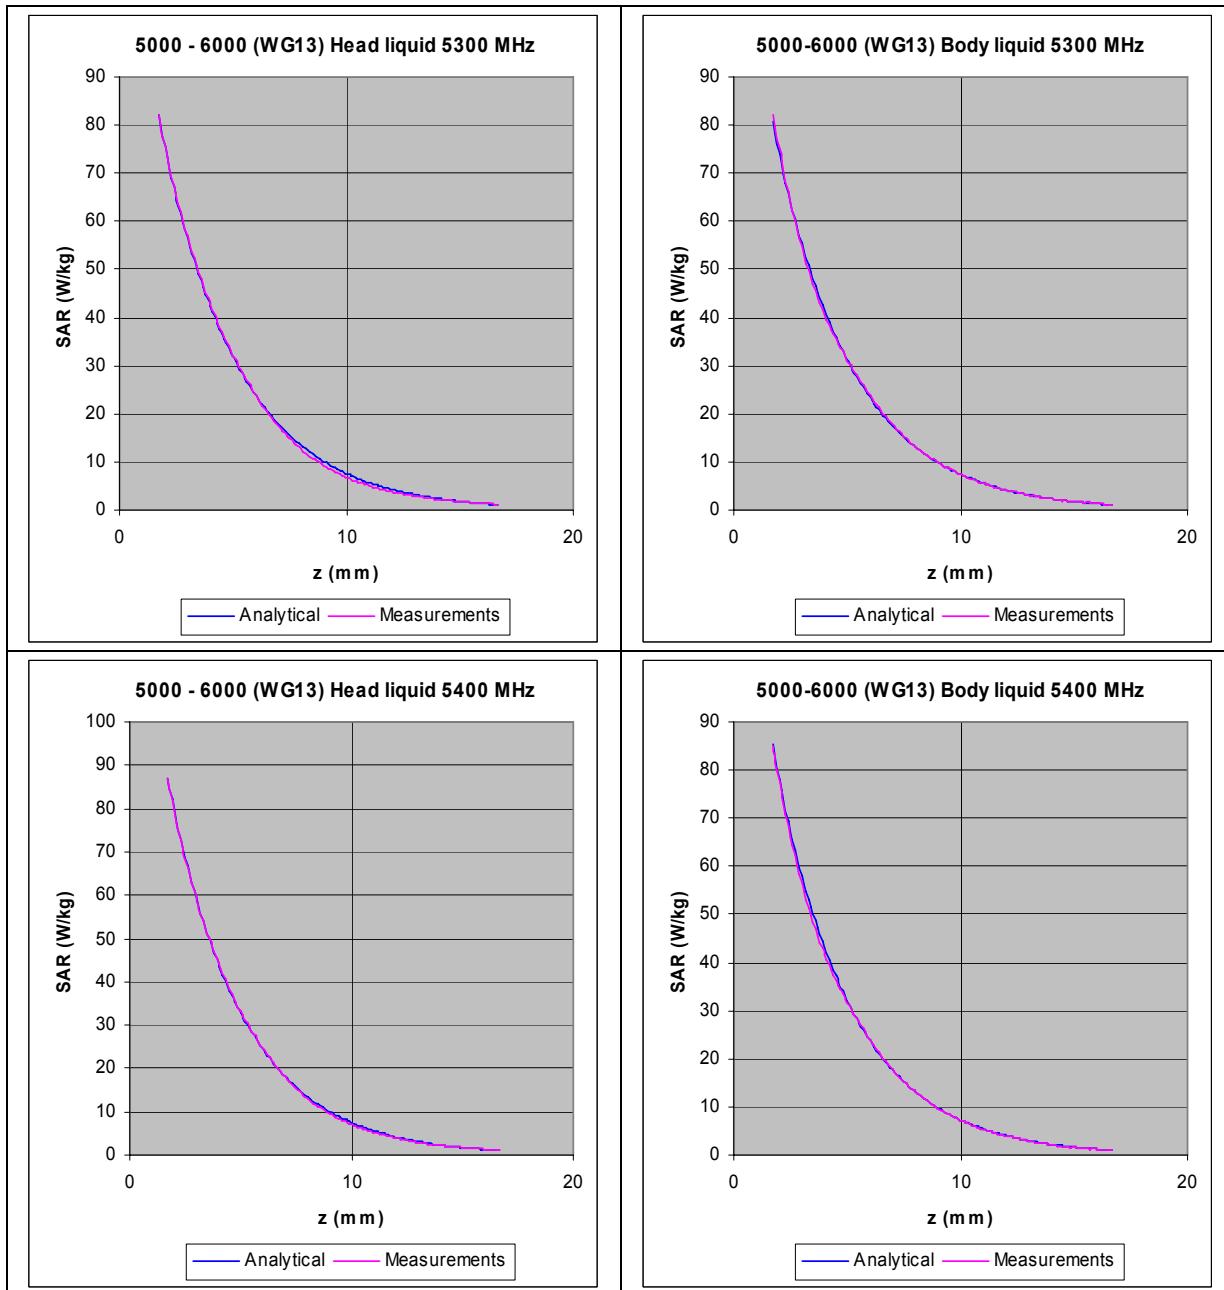
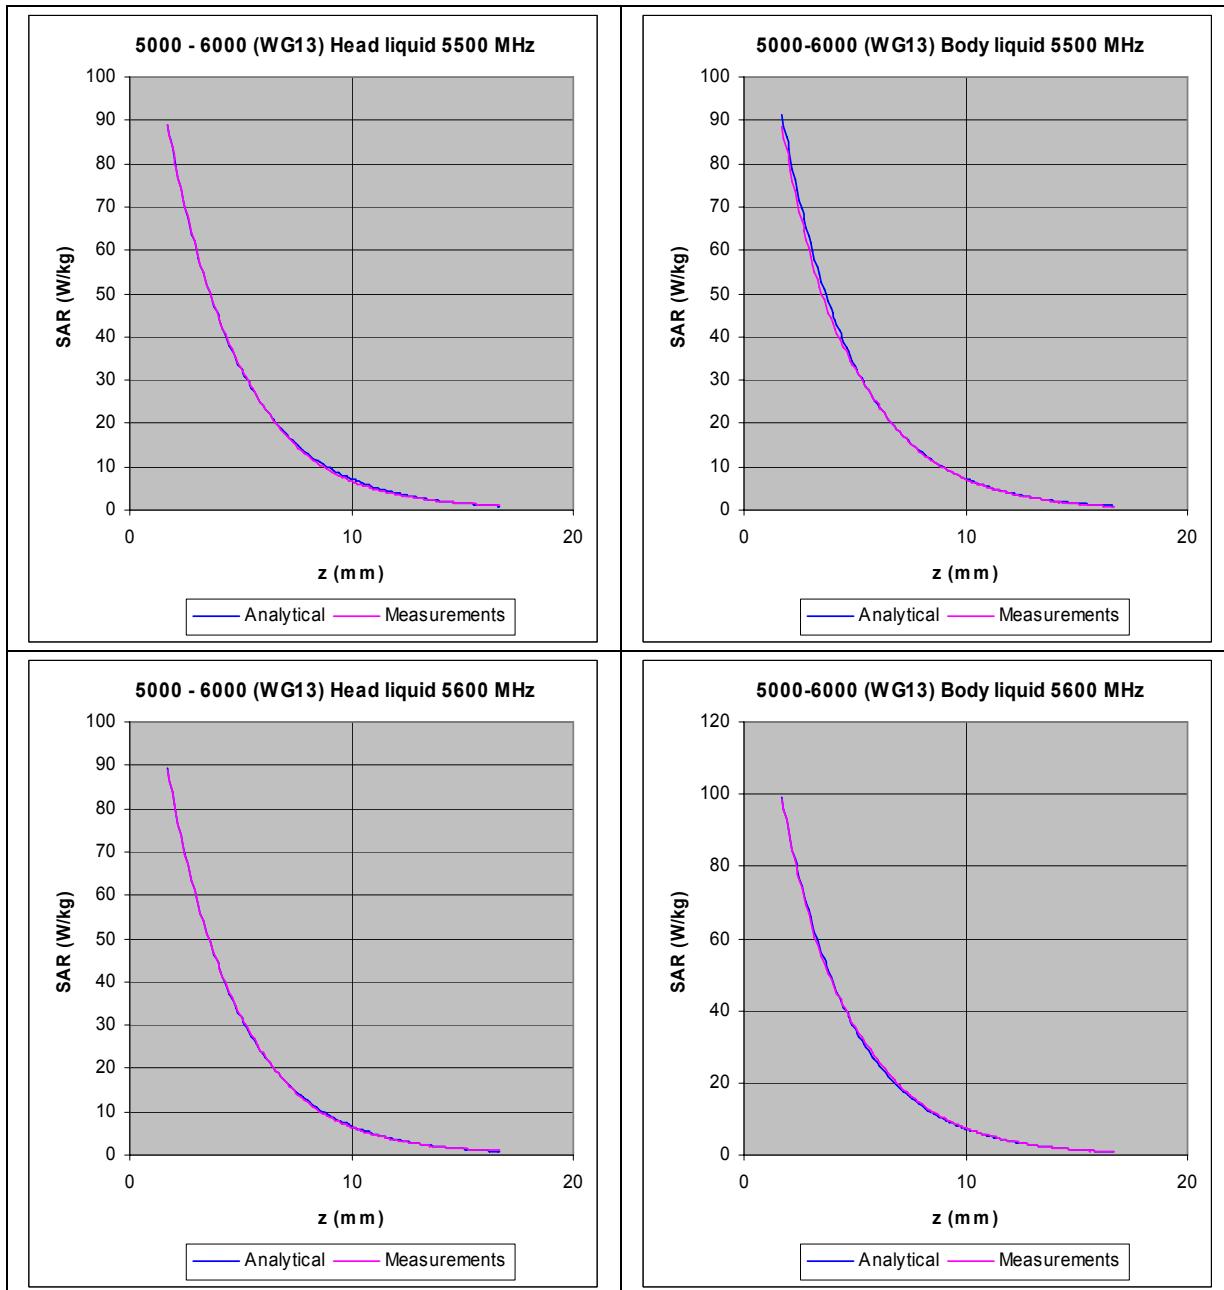


Figure 8. The measured SAR decay function along the centreline of the WG8 waveguide with conversion factors adjusted to fit to the theoretical function for the particular dimension, frequency, power and liquid properties employed.







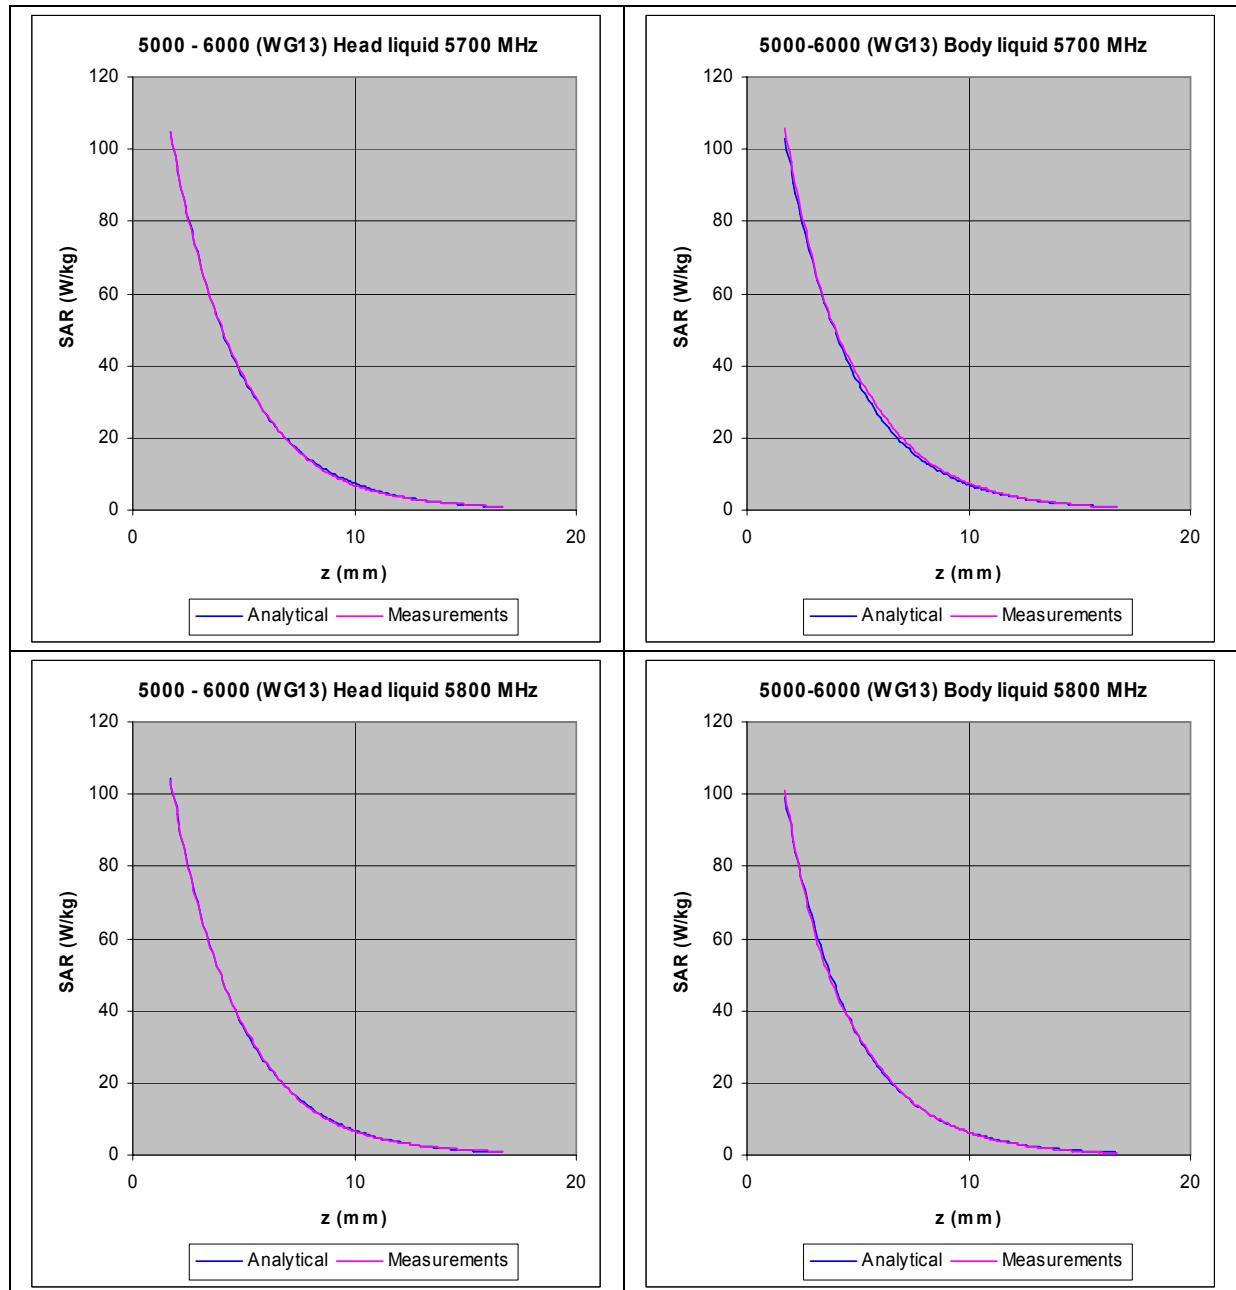


Figure 9 The measured SAR decay function along the centreline of the WG13 waveguide with conversion factors adjusted to fit to the theoretical function for the particular dimension, frequency, power and liquid properties employed.

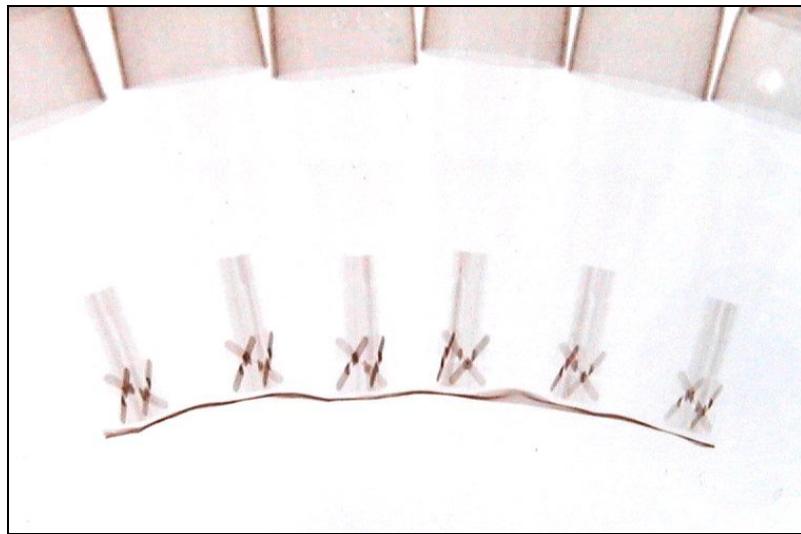


Figure 10: X-ray positive image of 5mm probes

Table indicating the dielectric parameters of the liquids used for calibrations at each frequency

Frequency (MHz)	BRAIN		BODY	
	Relative permittivity (measured)	Conductivity (S/m) (measured)	Relative permittivity (measured)	Conductivity (S/m) (measured)
835	41.50	0.90	55.93	0.99
900	40.88	0.96	55.32	1.05
1800	39.77	1.38	53.14	1.56
1900	39.98	1.39	54.12	1.57
2100	39.29	1.51	53.65	1.68
2450	37.86	1.88	52.55	2.09
5100	34.25	4.35	45.89	5.00
5200	33.97	4.45	45.53	5.13
5300	33.70	4.56	45.24	5.26
5400	33.44	4.68	44.99	5.41
5500	33.15	4.79	44.677	5.55
5600	32.86	4.90	44.35	5.70
5700	32.61	5.00	44.08	5.84
5800	32.32	5.11	43.72	5.98

Note: Alternative dielectric measurement techniques give different property values for 5-6GHz liquids. Based on waveguide fits to analytical decay curves, DiLine conductivity values listed above were reduced by 10% from the reported value.

Table of test equipment calibration status

Instrument description	Supplier / Manufacturer	Model	Serial No.	Last calibration date	Calibration due date
Power sensor	Rohde & Schwarz	NRP-Z23	100063	16/06/2008	16/6/2010
Dielectric property measurement	Indexsar	DiLine (sensor lengths: 160mm, 80mm and 60mm)	N/A	(absolute) – checked against NPL values using reference liquids	N/A
Vector network analyser	Anritsu	MS6423B	003102	18/12/2008	18/12/2010
SMA autocalibration module	Anritsu	36581KKF/1	001902	18/12/2008	18/12/2010




Report No. SN081_0902
13th February 2009

**INDEXSAR
835 MHz Validation Dipole
Type IXD-835 S/N 081**

Performance measurements

Dr Tony Brinklow

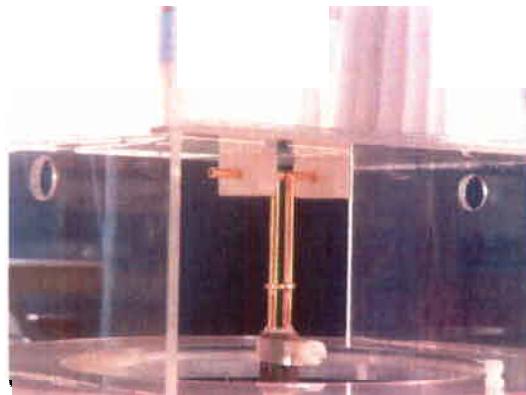

**Indexsar, Oakfield House, Cudworth Lane,
Newdigate, Surrey RH5 5BG, UK.
Tel: +44 (0) 1306 632 870 Fax: +44 (0) 1306 631 834
E-mail: enquiries@indexsar.com**

1. Measurement Conditions

Measurements were performed using a box-shaped phantom made of PMMA with dimensions designed to meet the accuracy criteria for reasonably-sized phantoms that do not have liquid capacities substantially in excess of the volume of liquid required to fill the Indexsar upright SAM phantoms used for SAR testing of handsets against the ear. The wall thickness was 2mm.

An Anritsu MS4623B vector network analyser was used for the return loss measurements. The dipole was placed in a special holder made of low-permittivity, low-loss materials. This holder enables the dipole to be positioned accurately in the centre of the wall of the Indexsar box-phantom used for flat-surface testing and validation checks.

The validation dipoles are supplied with special spacers made from a low-permittivity, low-loss foam material. These spacers are fitted to the dipole arms to ensure that, when the dipole is offered up to the phantom surface, the spacing between the dipole and the liquid surface is accurately aligned according to the guidance in the relevant standards documentation [1]. The spacers are rectangular with a central hole equal to the dipole arm diameter and dimensioned so that the longer side can be used to ensure a spacing of 15mm from the liquid in the phantom (for tests at 1000MHz and below) and the shorter side can be used for tests at 1000MHz and above to ensure a spacing of 10mm from the liquid in the phantom. The spacers are made on a CNC milling machine with an accuracy of 1/40th mm but they may suffer wear and tear and need to be replaced periodically. The material used is Rohacell, which has a relative permittivity of approx. 1.05 and a negligible loss tangent.

The apparatus supplied by Indexsar for dipole validation tests thus includes:


Balanced dipoles for each frequency required are dimensioned according to the guidelines given in IEEE 1528 [1]. The dipoles are made from semi-rigid 50 Ohm co-ax, which is joined by soldering and is gold-plated subsequently. The constructed dipoles are easily deformed, if mis-handled, and periodic checks need to be made of their symmetry.

Rohacell foam spacers designed for presenting the dipoles to 2mm thick PMMA box phantoms. These components also suffer wear and tear and should be replaced when the central hole is a loose-fit on the dipole arms or if the edges are too worn to ensure accurate alignment. The standard spacers are dimensioned for use with 2mm wall thickness (additional spacers are available for 4mm wall thickness).

2. Dipole impedance and return loss

The dipoles are designed to have low return loss ONLY when presented against a lossy-phantom at the specified distance. A Vector Network Analyser (VNA) was used to perform a return loss measurement on the specific dipole when in the measurement-location against the box phantom. The distance was as specified in the standard i.e. 15mm from the liquid (for 835MHz). The Indexsar foam spacers (described above) were used to ensure this condition during measurement.


The impedance was measured at the SMA-connector with the network analyser. The following parameters were measured against Head fluid:

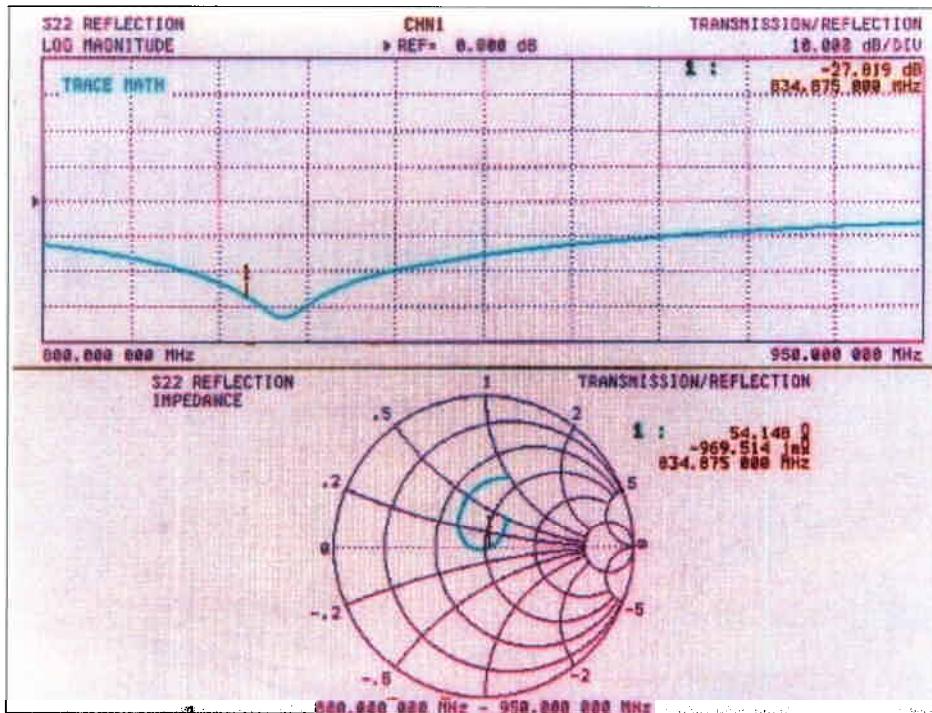

Dipole impedance at 835 MHz $\text{Re}\{Z\} = 54.1 \Omega$
 $\text{Im}\{Z\} = -0.9 \Omega$

Return loss at 835MHz **-27.8 dB**

The measurements were also repeated against 835MHz Body fluid:

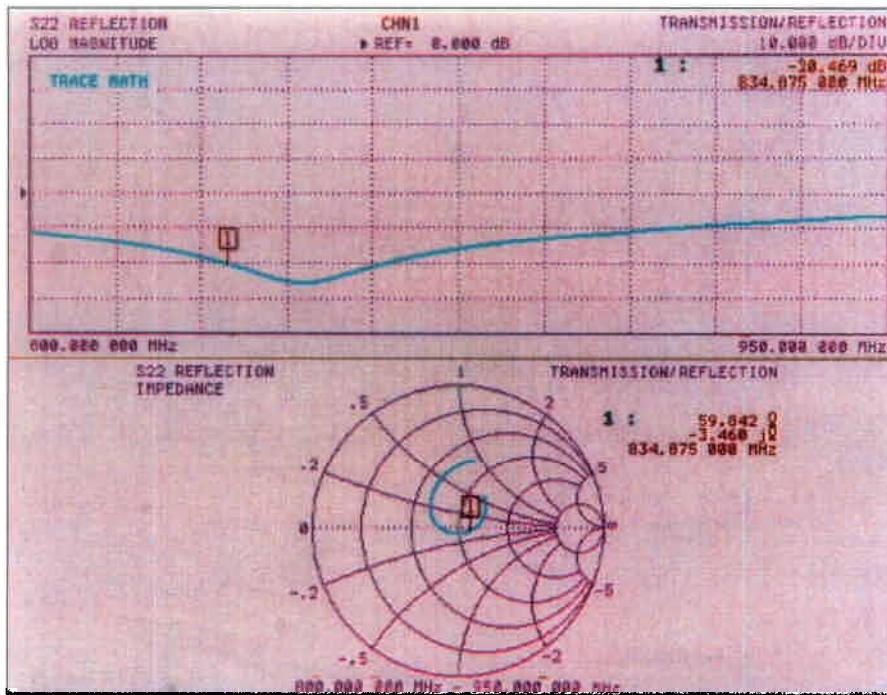

Dipole impedance at 835 MHz $\text{Re}\{Z\} = 59.8 \Omega$
 $\text{Im}\{Z\} = -3.5 \Omega$

Return loss at 835MHz -20.5 dB

3. SAR Validation Measurement in Brain Fluid

SAR validation checks have been performed using the dipole and the box-phantom located on the SARA2 phantom support base on the SARA2 robot system. Tests were then conducted at a feed power level of approx. 0.25W. The actual power level was recorded and used to normalise the results obtained to the standard input power conditions of 1W (forward power). A correction factor was also applied to account for transmission loss arising from the dipole's reflection coefficient.

The ambient temperature was 21°C +/- 1°C and the relative humidity was around 35% during the measurements.

The phantom was filled with a 835MHz brain liquid using a recipe from [1], which has the following electrical parameters (measured using an Indexsar DiLine kit) at 835MHz at the measurement temperature:


Relative Permittivity	40.85	(Target: 41.5)
Conductivity	0.90 S/m	(Target: 0.90 S/m)

SAR specification EN62209-2(2007) [ref 2], in which the validation method is described, specifies how to adjust measured 1g & 10g volume-averaged SAR values to take into account the difference between the fluid's actual, and target, electrical properties. The correction factors for this combination of properties at 835MHz equals:

1g: -0.1%
10g: -0.03%

The SARA2 software version 2.54 VPM was used with Indexsar IXP_050 probe Serial Number 0127 previously calibrated using waveguides.

The 3D measurement made using the dipole at the bottom of the phantom box is shown below:

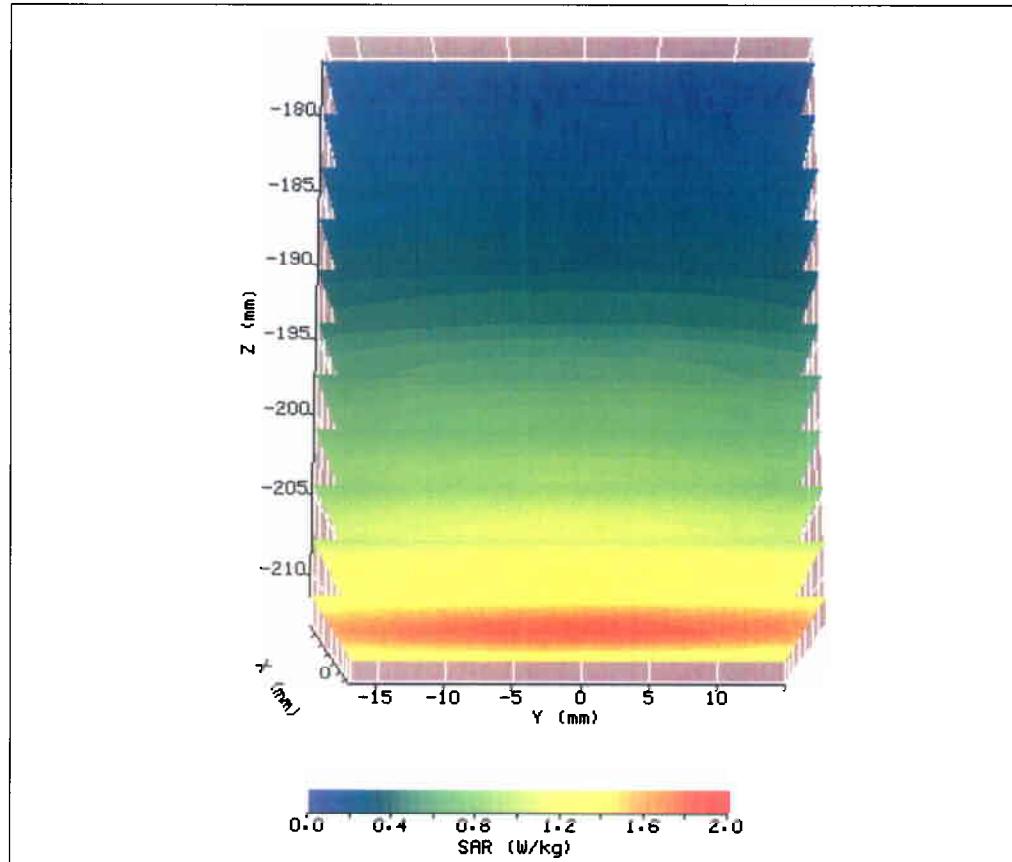

SAR measurement standard 62209-1 [ref 2] tabulates the volume-averaged 1g and 10g SAR values over a range of frequencies up to 3000MHz. The following values are listed for 835MHz:

SAR values (W/kg) (Normalised to 1W feed power)	
1g SAR	9.5
10g SAR	6.2

The validation results, also normalised to an input power of 1W (forward power) were:

	Measured SAR values (W/kg) (Normalised to 1W feed power)	% Deviation from Standard
1g SAR	9.44	-0.7%
10g SAR	6.24	+0.6%

4. SAR Measurement in Body Fluid

SAR validation checks are only defined in the standard against brain simulant fluid. Nonetheless, it is possible to measure the effective volume-averaged SAR values against body fluid, simply to provide a reference value.

The ambient temperature was 21°C +/- 1°C and the relative humidity was around 32% during the measurements.

The phantom was filled with a 835MHz body liquid using a recipe from [1], which has the following electrical parameters (measured using an Indexsar DiLine kit) at 835MHz at the measurement temperature:


Relative Permittivity	55.91	(Target: 55.2)
Conductivity	0.99 S/m	(Target: 0.97 S/m)

The correction factors for this combination of properties at 835MHz equals:

1g: -1.1%
10g: -0.9%

The SARA2 software version 2.54 VPM was used with Indexsar IXP_050 probe Serial Number 0127 previously calibrated using waveguides.

The 3D measurement made using the dipole at the bottom of the phantom box is shown below:

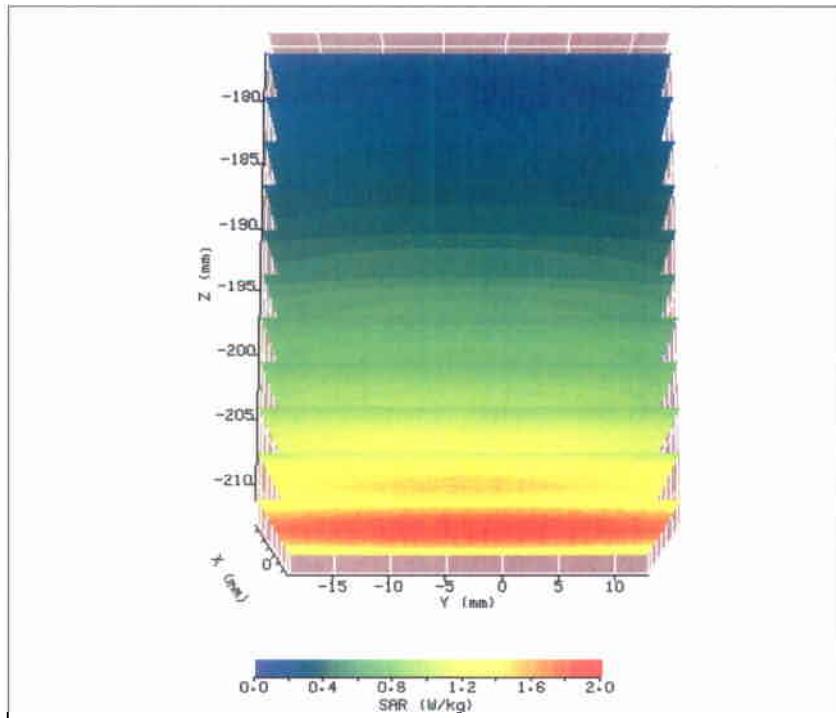

The validation results, also normalised to an input power of 1W (forward power) were:

	Measured SAR values (W/kg) (Normalised to 1W feed power)	% Deviation from Standard
1g SAR	9.78	N/A
10g SAR	6.48	N/A

5. Dipole handling

The dipoles are made from standard, copper-sheathed coaxial cable. In assembly, the sections are joined using ordinary soft-soldering. This is necessary to avoid excessive heat input in manufacture, which would destroy the polythene dielectric used for the cable. The consequence of the construction material and the assembly technique is that the dipoles are fragile and can be deformed by rough handling. Conversely, they can be straightened quite easily as described in this report.

If a dipole is suspected of being deformed, a normal workshop lathe can be used as an alignment jig to restore the symmetry. To do this, the dipole is first placed in the headstock of the lathe (centred on the plastic or brass spacers) and the headstock is rotated by hand (do NOT use the motor). A marker (lathe tool or similar) is brought up close to the end of one dipole arm and then the headstock is rotated by 0.5 rev. to check the opposing arm. If they are not balanced, judicious deformation of the arms can be used to restore the symmetry.

If a dipole has a failed solder joint, the dipole can be fixed down in such a way that the arms are co-linear and the joint re-soldered with a reasonably-powerful electrical soldering iron. Do not use gas soldering irons. After such a repair, electrical tests must be performed as described below.

Please note that, because of their construction, the dipoles are short-circuited for DC signals.

6. Tuning the dipole

The dipole dimensions are based on calculations that assumed specific liquid dielectric properties. If the liquid dielectric properties are somewhat different, the dipole tuning will also vary. A pragmatic way of accounting for variations in liquid properties is to 'tune' the dipole (by applying minor variations to its effective length). For this purpose, Indexsar can supply short brass tube lengths to extend the length of the dipole and thus 'tune' the dipole. It cannot be made shorter without removing a bit from the arm. An alternative way to tune the dipole is to use copper shielding tape to extend the effective length of the dipole. Do both arms equally.

It should be possible to tune a dipole as described, whilst in place in the measurement position as long as the user has access to a VNA for determining the return loss.

7. References

- [1] IEEE Std 1528-2003. IEEE recommended practice for determining the peak spatial-average specific absorption rate (SAR) in the human body due to wireless communications devices: Measurement Techniques – Description.
- [2] BS EN 62209-1:2006 Human exposure to radio frequency fields from hand-held and body-mounted wireless communication devices — Human models, instrumentation, and procedures — Part 1: Procedure to determine the specific absorption rate (SAR) for hand-held devices used in close proximity to the ear (frequency range of 300 MHz to 3 GHz)
- [3] BS EN 62209-2:2007 Human Exposure to Radio Frequency Fields from Handheld and Body-Mounted Wireless Communication Devices - Human models, Instrumentation, and Procedures - Part 2: Procedure to determine the specific absorption rate (SAR) for mobile wireless communication devices used in close proximity to the human body (frequency range of 30 MHz to 6 GHz)



Report No. SN016_0902
13th February 2009

**INDEXSAR
1880 MHz Validation Dipole
Type IXDA-188 S/N 016**

Performance measurements

Dr Tony Brinklow



**Indexsar, Oakfield House, Cudworth Lane,
Newdigate, Surrey RH5 5BG. UK.
Tel: +44 (0) 1306 632 870 Fax: +44 (0) 1306 631 834
E-mail: enquiries@indexsar.com**

1. Measurement Conditions

Measurements were performed using a box-shaped phantom made of PMMA with dimensions designed to meet the accuracy criteria for reasonably-sized phantoms that do not have liquid capacities substantially in excess of the volume of liquid required to fill the Indexsar upright SAM phantoms used for SAR testing of handsets against the ear. The wall thickness was 2mm.

An Anritsu MS4623B vector network analyser was used for the return loss measurements. The dipole was placed in a special holder made of low-permittivity, low-loss materials. This holder enables the dipole to be positioned accurately in the centre of the wall of the Indexsar box-phantom used for flat-surface testing and validation checks.

The validation dipoles are supplied with special spacers made from a low-permittivity, low-loss foam material. These spacers are fitted to the dipole arms to ensure that, when the dipole is offered up to the phantom surface, the spacing between the dipole and the liquid surface is accurately aligned according to the guidance in the relevant standards documentation [1]. The spacers are rectangular with a central hole equal to the dipole arm diameter and dimensioned so that the longer side can be used to ensure a spacing of 15mm from the liquid in the phantom (for tests at 1000MHz and below) and the shorter side can be used for tests at 1000MHz and above to ensure a spacing of 10mm from the liquid in the phantom. The spacers are made on a CNC milling machine with an accuracy of 1/40th mm but they may suffer wear and tear and need to be replaced periodically. The material used is Rohacell, which has a relative permittivity of approx. 1.05 and a negligible loss tangent.

The apparatus supplied by Indexsar for dipole validation tests thus includes:

Balanced dipoles for each frequency required are dimensioned according to the guidelines given in IEEE 1528 [1]. The dipoles are made from semi-rigid 50 Ohm co-ax, which is joined by soldering and is gold-plated subsequently. The constructed dipoles are easily deformed, if mis-handled, and periodic checks need to be made of their symmetry.


Rohacell foam spacers designed for presenting the dipoles to 2mm thick PMMA box phantoms. These components also suffer wear and tear and should be replaced when the central hole is a loose-fit on the dipole arms or if the edges are too worn to ensure accurate alignment. The standard spacers are dimensioned for use with 2mm wall thickness (additional spacers are available for 4mm wall thickness).

2. Dipole impedance and return loss

The customer advised that although the dipole-under-test was designed as an 1880MHz air dipole (model IXDA-188), in practice it is used as a SAR dipole. Consequently, this report concentrates on the dipole's 1900MHz performance relative to the 1900MHz reference values.

The dipoles are designed to have low return loss ONLY when presented against a lossy-phantom at the specified distance. A Vector Network Analyser (VNA) was used to perform a return loss measurement on the specific dipole when in the measurement-location against the box phantom. The distance was as specified in the standard i.e. 10mm from the liquid (for 1900MHz). The Indexsar foam spacers (described above) were used to ensure this condition during measurement.


The impedance was measured at the SMA-connector with the network analyser. The following parameters were measured against Head fluid:

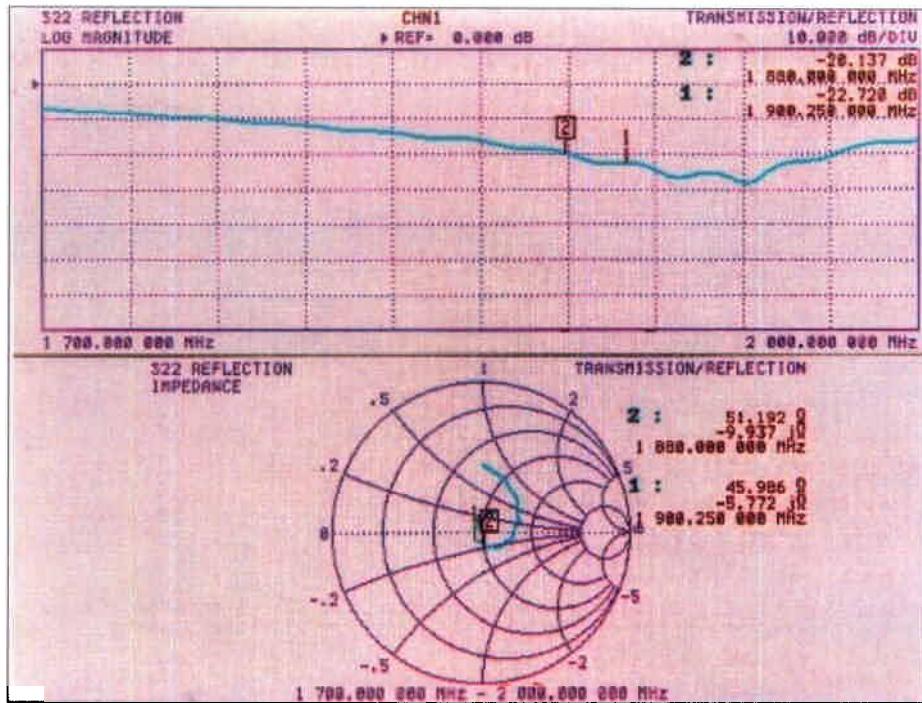

Dipole impedance at 1900 MHz $\text{Re}\{Z\} = 46.0 \Omega$
 $\text{Im}\{Z\} = -5.8 \Omega$

Return loss at 1900MHz **-22.7 dB**

The measurements were also repeated against 1900MHz Body fluid:

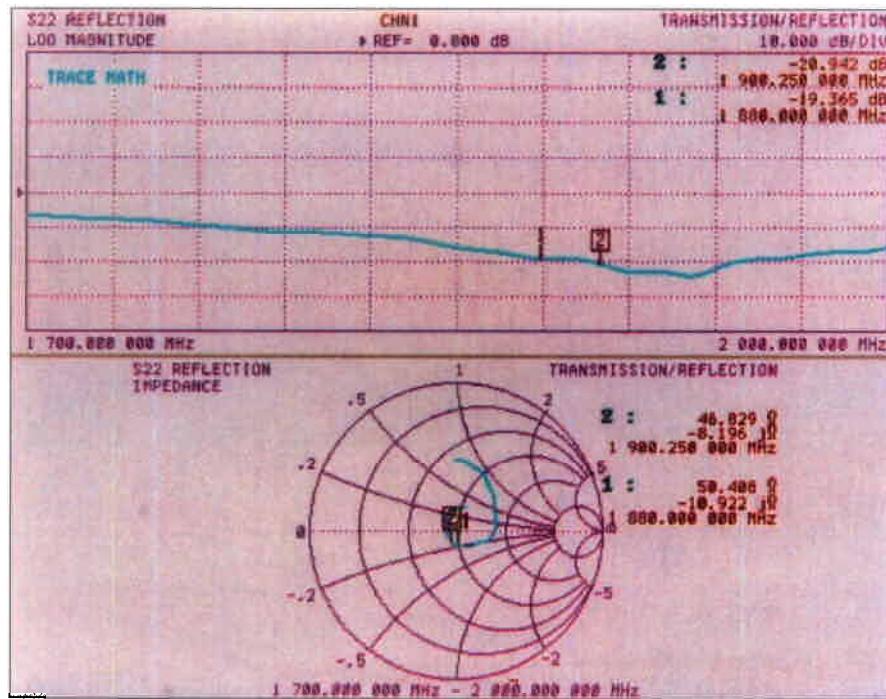

Dipole impedance at 1900 MHz $\text{Re}\{Z\} = 46.8 \Omega$
 $\text{Im}\{Z\} = -8.2 \Omega$

Return loss at 1900MHz **-20.9 dB**

3. SAR Validation Measurement in Brain Fluid

SAR validation checks have been performed using the dipole and the box-phantom located on the SARA2 phantom support base on the SARA2 robot system. Tests were then conducted at a feed power level of approx. 0.25W. The actual power level was recorded and used to normalise the results obtained to the standard input power conditions of 1W (forward power). A correction factor was also applied to account for transmission loss arising from the dipole's reflection coefficient.

The ambient temperature was $21^\circ\text{C} \pm 1^\circ\text{C}$ and the relative humidity was around 35% during the measurements.

The phantom was filled with a 1900MHz brain liquid using a recipe from [1], which has the following electrical parameters (measured using an Indexsar DiLine kit) at 1900MHz at the measurement temperature:

Relative Permittivity	39.10	(Target: 40.0)
Conductivity	1.52 S/m	(Target: 1.40 S/m)


SAR specification EN62209-2(2007) [ref 2], in which the validation method is described, specifies how to adjust measured 1g & 10g volume-averaged SAR values to take into account the difference between the fluid's actual and target electrical properties. The correction factors for this combination of properties at 1900MHz equals:

1g: -5.3%

10g: -3.4%

The SARA2 software version 2.54 VPM was used with Indexsar IXP_050 probe Serial Number 0127 previously calibrated using waveguides.

The 3D measurement made using the dipole at the bottom of the phantom box is shown below:

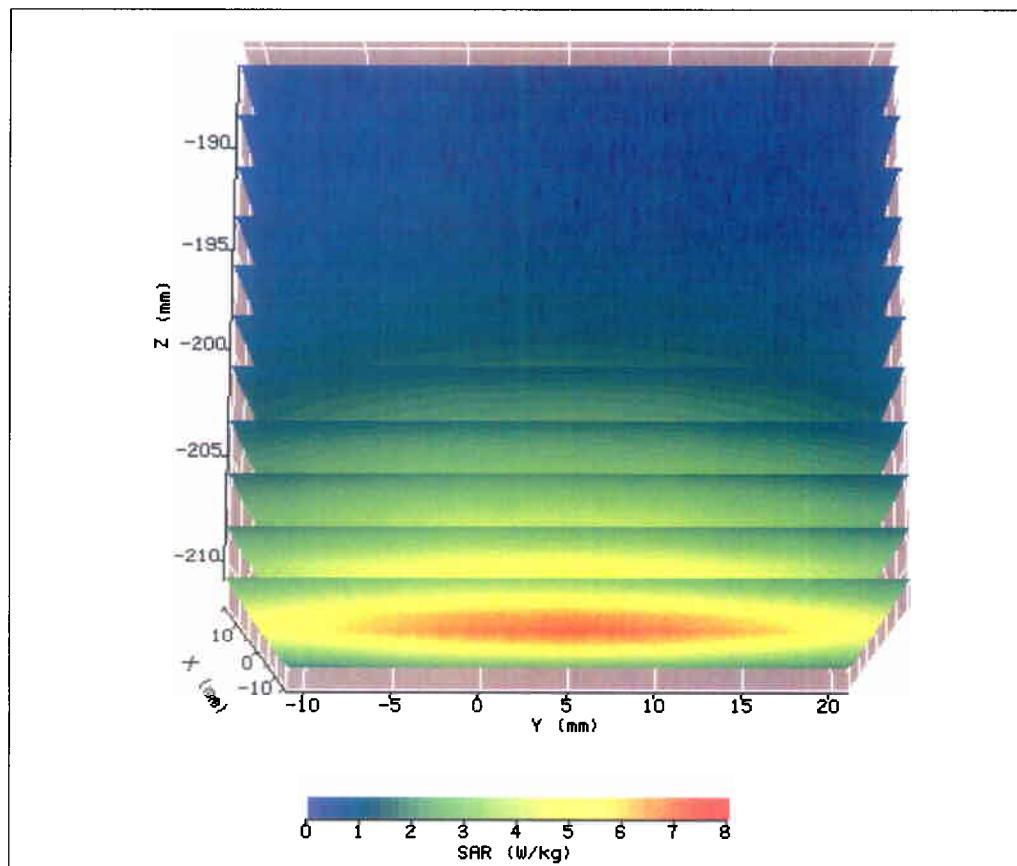

SAR measurement standard 62209-1 [ref 2] tabulates the volume-averaged 1g and 10g SAR values over a range of frequencies up to 3000MHz. The following values are listed for 1900MHz:

	Target SAR values (W/kg) (Normalised to 1W feed power)
1g SAR	39.7
10g SAR	20.5

The validation results, also normalised to an input power of 1W (forward power) were:

	Measured SAR values (W/kg) (Normalised to 1W feed power)	% Deviation from Standard
1g SAR	38.3	-3.6%
10g SAR	20.2	-1.6%

4. SAR Measurement in Body Fluid

SAR validation checks are only defined in the standard against brain simulant fluid. Nonetheless, it is possible to measure the effective volume-averaged SAR values against body fluid, simply to provide a reference value.

The ambient temperature was 21°C +/- 1°C and the relative humidity was around 32% during the measurements.

The phantom was filled with a 1900MHz body liquid using a recipe from [1], which has the following electrical parameters (measured using an Indexsar DiLine kit) at 1900MHz at the measurement temperature:


Relative Permittivity 54.05 (Target: 53.3)
 Conductivity 1.55 S/m (Target: 1.52 S/m)

The correction factors for this combination of properties at 1900MHz equals:

1g: -0.9%
 10g: -0.6%

The SARA2 software version 2.54 VPM was used with Indexsar IXP_050 probe Serial Number 0127 previously calibrated using waveguides.

The 3D measurement made using the dipole at the bottom of the phantom box is shown below:

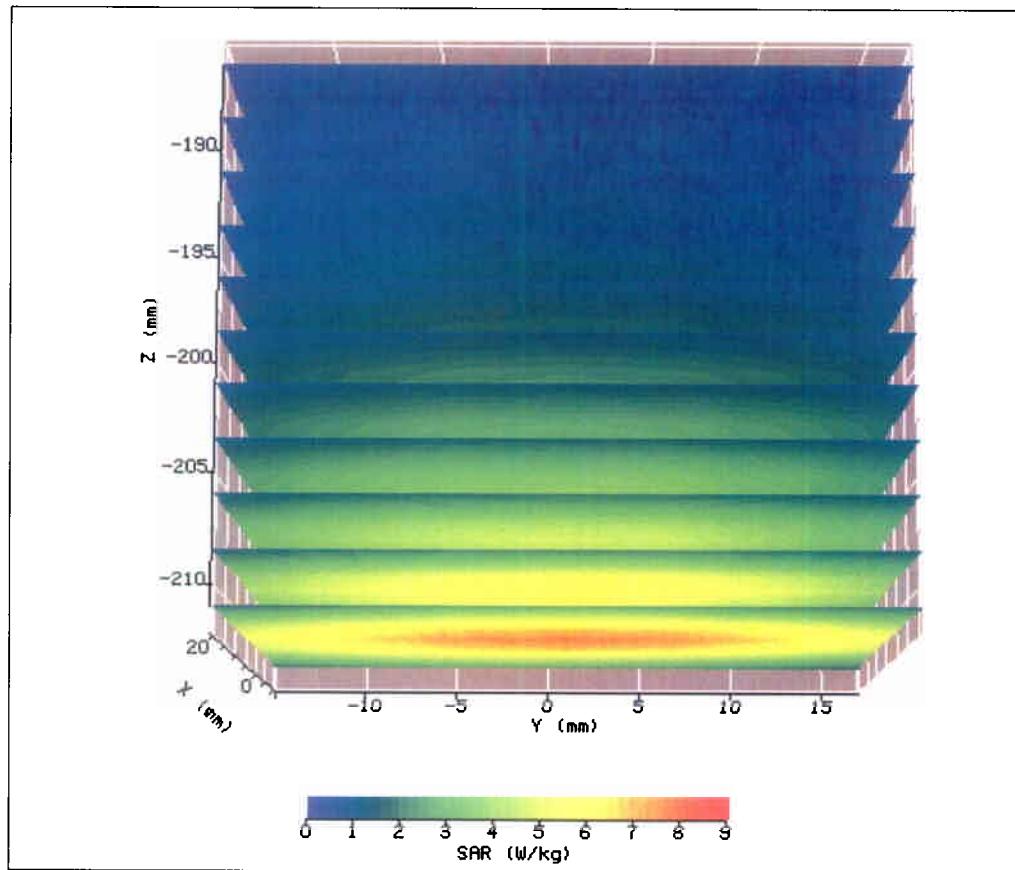

The validation results, also normalised to an input power of 1W (forward power) were:

	Measured SAR values (W/kg) (Normalised to 1W feed power)	% Deviation from Standard
1g SAR	40.35	N/A
10g SAR	21.76	N/A

5. Dipole handling

The dipoles are made from standard, copper-sheathed coaxial cable. In assembly, the sections are joined using ordinary soft-soldering. This is necessary to avoid excessive heat input in manufacture, which would destroy the polythene dielectric used for the cable. The consequence of the construction material and the assembly technique is that the dipoles are fragile and can be deformed by rough handling. Conversely, they can be straightened quite easily as described in this report.

If a dipole is suspected of being deformed, a normal workshop lathe can be used as an alignment jig to restore the symmetry. To do this, the dipole is first placed

in the headstock of the lathe (centred on the plastic or brass spacers) and the headstock is rotated by hand (do NOT use the motor). A marker (lathe tool or similar) is brought up close to the end of one dipole arm and then the headstock is rotated by 0.5 rev. to check the opposing arm. If they are not balanced, judicious deformation of the arms can be used to restore the symmetry.

If a dipole has a failed solder joint, the dipole can be fixed down in such a way that the arms are co-linear and the joint re-soldered with a reasonably-powerful electrical soldering iron. Do not use gas soldering irons. After such a repair, electrical tests must be performed as described below.

Please note that, because of their construction, the dipoles are short-circuited for DC signals.

6. Tuning the dipole

The dipole dimensions are based on calculations that assumed specific liquid dielectric properties. If the liquid dielectric properties are somewhat different, the dipole tuning will also vary. A pragmatic way of accounting for variations in liquid properties is to 'tune' the dipole (by applying minor variations to its effective length). For this purpose, Indexsar can supply short brass tube lengths to extend the length of the dipole and thus 'tune' the dipole. It cannot be made shorter without removing a bit from the arm. An alternative way to tune the dipole is to use copper shielding tape to extend the effective length of the dipole. Do both arms equally.

It should be possible to tune a dipole as described, whilst in place in the measurement position as long as the user has access to a VNA for determining the return loss.

7. References

- [1] IEEE Std 1528-2003. IEEE recommended practice for determining the peak spatial-average specific absorption rate (SAR) in the human body due to wireless communications devices: Measurement Techniques – Description.
- [2] BS EN 62209-1:2006 Human exposure to radio frequency fields from hand-held and body-mounted wireless communication devices — Human models, instrumentation, and procedures — Part 1: Procedure to determine the specific absorption rate (SAR) for hand-held devices used in close proximity to the ear (frequency range of 300 MHz to 3 GHz)
- [3] BS EN 62209-2:2007 Human Exposure to Radio Frequency Fields from Handheld and Body-Mounted Wireless Communication Devices - Human models, Instrumentation, and Procedures - Part 2: Procedure to determine the specific absorption rate (SAR) for mobile wireless communication devices used in close proximity to the human body (frequency range of 30 MHz to 6 GHz)




Report No. SN228_0902
13th February 2009

INDEXSAR
2450 MHz Validation Dipole
Type IXD-245 S/N 228

Performance measurements

Dr Tony Brinklow

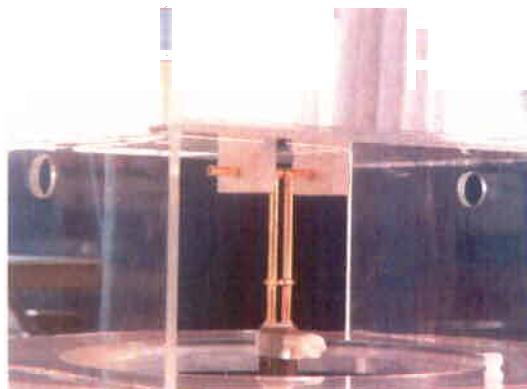

**Indexsar, Oakfield House, Cudworth Lane,
Newdigate, Surrey RH5 5BG. UK.**
Tel: +44 (0) 1306 632 870 Fax: +44 (0) 1306 631 834
E-mail: enquiries@indexsar.com

1. Measurement Conditions

Measurements were performed using a box-shaped phantom made of PMMA with dimensions designed to meet the accuracy criteria for reasonably-sized phantoms that do not have liquid capacities substantially in excess of the volume of liquid required to fill the Indexsar upright SAM phantoms used for SAR testing of handsets against the ear. The wall thickness was 2mm.

An Anritsu MS4623B vector network analyser was used for the return loss measurements. The dipole was placed in a special holder made of low-permittivity, low-loss materials. This holder enables the dipole to be positioned accurately in the centre of the wall of the Indexsar box-phantom used for flat-surface testing and validation checks.

The validation dipoles are supplied with special spacers made from a low-permittivity, low-loss foam material. These spacers are fitted to the dipole arms to ensure that, when the dipole is offered up to the phantom surface, the spacing between the dipole and the liquid surface is accurately aligned according to the guidance in the relevant standards documentation [1]. The spacers are rectangular with a central hole equal to the dipole arm diameter and dimensioned so that the longer side can be used to ensure a spacing of 15mm from the liquid in the phantom (for tests at 1000MHz and below) and the shorter side can be used for tests at 1000MHz and above to ensure a spacing of 10mm from the liquid in the phantom. The spacers are made on a CNC milling machine with an accuracy of 1/40th mm but they may suffer wear and tear and need to be replaced periodically. The material used is Rohacell, which has a relative permittivity of approx. 1.05 and a negligible loss tangent.

The apparatus supplied by Indexsar for dipole validation tests thus includes:


Balanced dipoles for each frequency required are dimensioned according to the guidelines given in IEEE 1528 [1]. The dipoles are made from semi-rigid 50 Ohm co-ax, which is joined by soldering and is gold-plated subsequently. The constructed dipoles are easily deformed, if mis-handled, and periodic checks need to be made of their symmetry.

Rohacell foam spacers designed for presenting the dipoles to 2mm thick PMMA box phantoms. These components also suffer wear and tear and should be replaced when the central hole is a loose-fit on the dipole arms or if the edges are too worn to ensure accurate alignment. The standard spacers are dimensioned for use with 2mm wall thickness (additional spacers are available for 4mm wall thickness).

2. Dipole impedance and return loss

The dipoles are designed to have low return loss ONLY when presented against a lossy-phantom at the specified distance. A Vector Network Analyser (VNA) was used to perform a return loss measurement on the specific dipole when in the measurement-location against the box phantom. The distance was as specified in the standard i.e. 10mm from the liquid (for 2450MHz). The Indexsar foam spacers (described above) were used to ensure this condition during measurement.


The impedance was measured at the SMA-connector with the network analyser. The following parameters were measured against Head fluid:

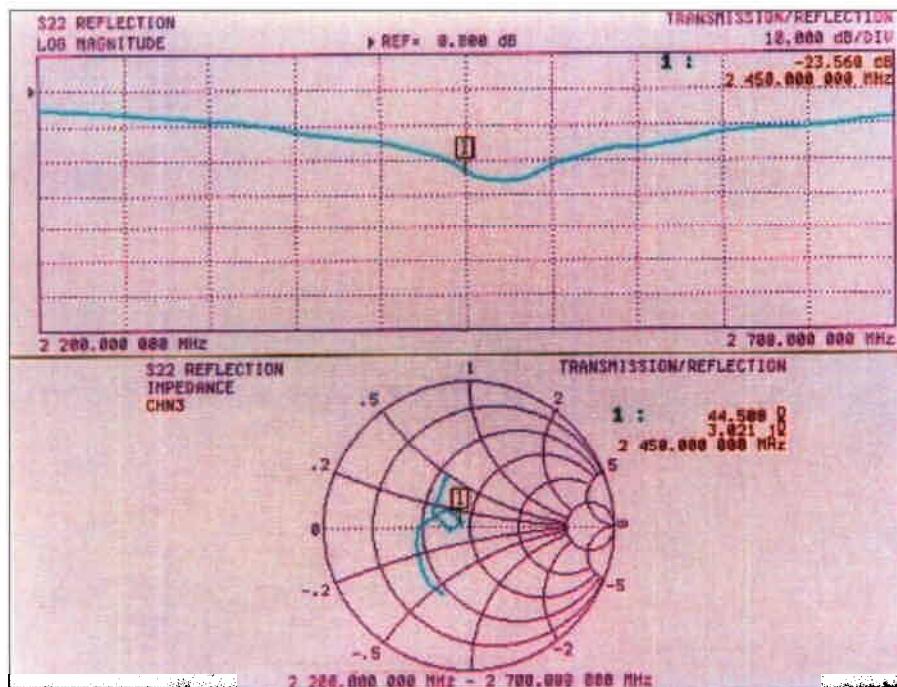

Dipole impedance at 2450 MHz $\text{Re}\{Z\} = 44.5 \Omega$
 $\text{Im}\{Z\} = 3.0 \Omega$

Return loss at 2450MHz -23.6 dB

The measurements were also repeated against 2450MHz Body fluid:

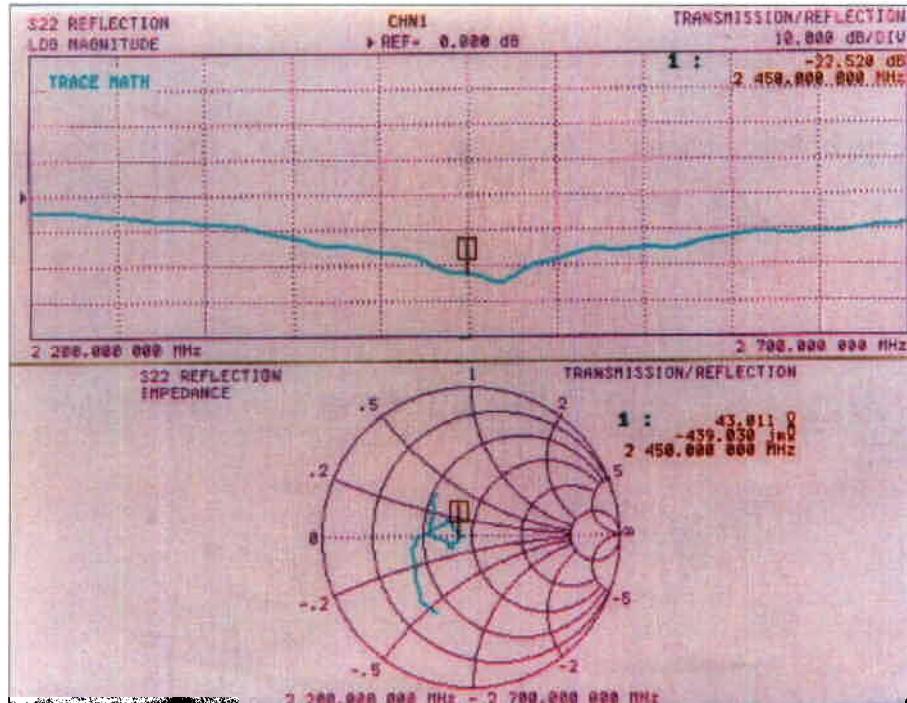

Dipole impedance at 2450 MHz $\text{Re}\{Z\} = 43.0 \Omega$
 $\text{Im}\{Z\} = -0.4 \Omega$

Return loss at 2450MHz -22.5 dB

3. SAR Validation Measurement in Brain Fluid

SAR validation checks have been performed using the dipole and the box-phantom located on the SARA2 phantom support base on the SARA2 robot system. Tests were then conducted at a feed power level of approx. 0.25W. The actual power level was recorded and used to normalise the results obtained to the standard input power conditions of 1W (forward power). A correction factor was also applied to account for transmission loss arising from the dipole's reflection coefficient.

The ambient temperature was 21°C +/- 1°C and the relative humidity was around 35% during the measurements.

The phantom was filled with a 2450MHz brain liquid using a recipe from [1], which has the following electrical parameters (measured using an Indexsar DiLine kit) at 2450MHz at the measurement temperature:


Relative Permittivity	37.96	(Target: 39.2)
Conductivity	1.86 S/m	(Target: 1.80 S/m)

SAR specification EN62209-2(2007) [ref 2], in which the validation method is described, specifies how to adjust measured 1g & 10g volume-averaged SAR values to take into account the difference between the fluid's actual and target electrical properties. The correction factors for this combination of properties at 2450MHz equals:

1g: -2.3%
10g: -1.3%

The SARA2 software version 2.54 VPM was used with Indexsar IXP_050 probe Serial Number 0127 previously calibrated using waveguides.

The 3D measurement made using the dipole at the bottom of the phantom box is shown below:

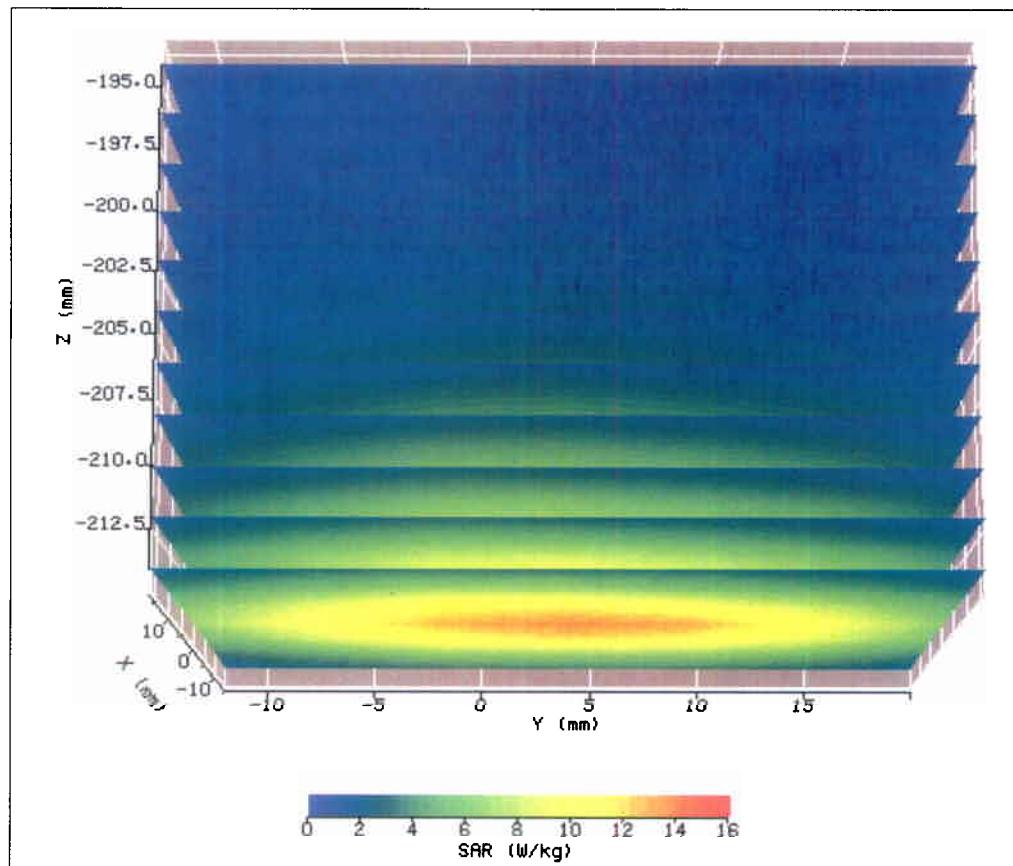

SAR measurement standard 62209-1 [ref 2] tabulates the volume-averaged 1g and 10g SAR values over a range of frequencies up to 3000MHz. The following values are listed for 2450MHz:

SAR values (W/kg) (Normalised to 1W feed power)	
1g SAR	52.4
10g SAR	24.0

The validation results, also normalised to an input power of 1W (forward power) were:

	Measured SAR values (W/kg) (Normalised to 1W feed power)	% Deviation from Standard
1g SAR	52.3	-0.3%
10g SAR	24.1	+0.5%

4. SAR Measurement in Body Fluid

SAR validation checks are only defined in the standard against brain simulant fluid. Nonetheless, it is possible to measure the effective volume-averaged SAR values against body fluid, simply to provide a reference value.

The ambient temperature was 21°C +/- 1°C and the relative humidity was around 32% during the measurements.

The phantom was filled with a 2450MHz body liquid using a recipe from [1], which has the following electrical parameters (measured using an Indexsar DiLine kit) at 2450MHz at the measurement temperature:


Relative Permittivity **52.55** (Target: 52.7)
Conductivity **2.10 S/m** (Target: 1.95 S/m)

The correction factors for this combination of properties at 2450MHz equals:

1g: -3.6%
10g: -2.0%

The SARA2 software version 2.54 VPM was used with Indexsar IXP_050 probe Serial Number 0127 previously calibrated using waveguides.

The 3D measurement made using the dipole at the bottom of the phantom box is shown below:

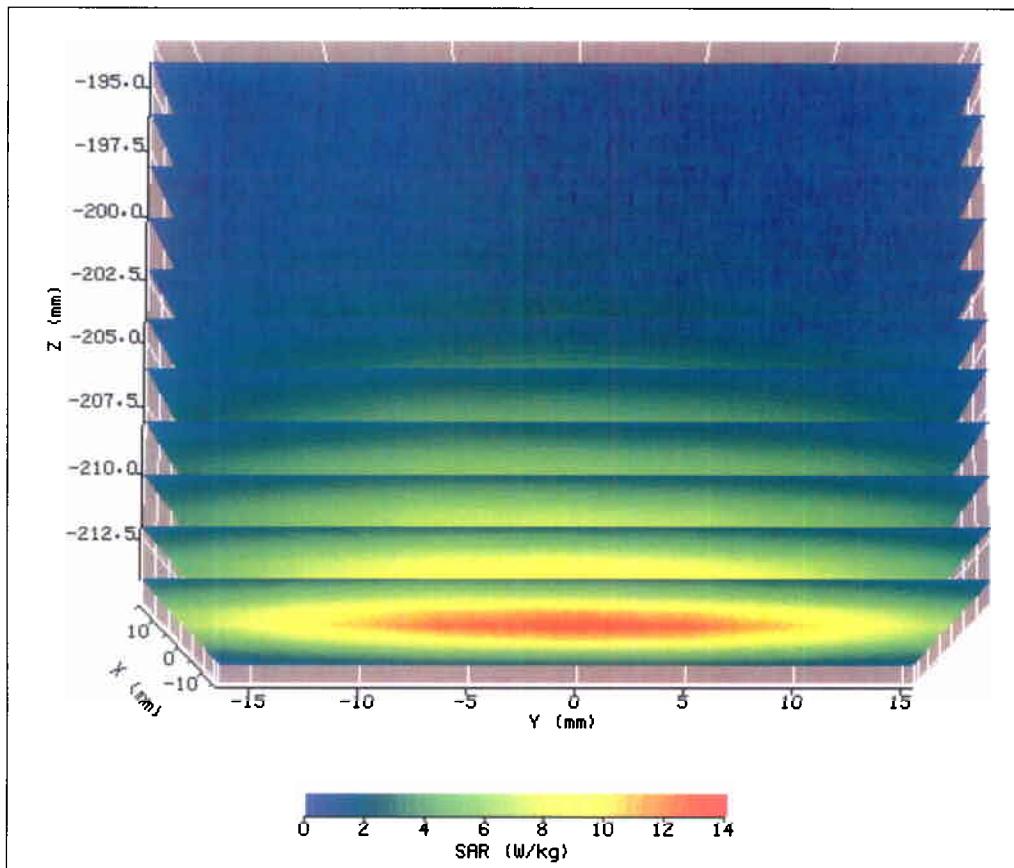

The validation results, also normalised to an input power of 1W (forward power) were:

	Measured SAR values (W/kg) (Normalised to 1W feed power)	% Deviation from Standard
1g SAR	50.17	N/A
10g SAR	23.50	N/A

5. Dipole handling

The dipoles are made from standard, copper-sheathed coaxial cable. In assembly, the sections are joined using ordinary soft-soldering. This is necessary to avoid excessive heat input in manufacture, which would destroy the polythene dielectric used for the cable. The consequence of the construction material and the assembly technique is that the dipoles are fragile and can be deformed by rough handling. Conversely, they can be straightened quite easily as described in this report.

If a dipole is suspected of being deformed, a normal workshop lathe can be used as an alignment jig to restore the symmetry. To do this, the dipole is first placed in the headstock of the lathe (centred on the plastic or brass spacers) and the headstock is rotated by hand (do NOT use the motor). A marker (lathe tool or

similar) is brought up close to the end of one dipole arm and then the headstock is rotated by 0.5 rev. to check the opposing arm. If they are not balanced, judicious deformation of the arms can be used to restore the symmetry.

If a dipole has a failed solder joint, the dipole can be fixed down in such a way that the arms are co-linear and the joint re-soldered with a reasonably-powerful electrical soldering iron. Do not use gas soldering irons. After such a repair, electrical tests must be performed as described below.

Please note that, because of their construction, the dipoles are short-circuited for DC signals.

6. Tuning the dipole

The dipole dimensions are based on calculations that assumed specific liquid dielectric properties. If the liquid dielectric properties are somewhat different, the dipole tuning will also vary. A pragmatic way of accounting for variations in liquid properties is to 'tune' the dipole (by applying minor variations to its effective length). For this purpose, Indexsar can supply short brass tube lengths to extend the length of the dipole and thus 'tune' the dipole. It cannot be made shorter without removing a bit from the arm. An alternative way to tune the dipole is to use copper shielding tape to extend the effective length of the dipole. Do both arms equally.

It should be possible to tune a dipole as described, whilst in place in the measurement position as long as the user has access to a VNA for determining the return loss.

7. References

- [1] IEEE Std 1528-2003. IEEE recommended practice for determining the peak spatial-average specific absorption rate (SAR) in the human body due to wireless communications devices: Measurement Techniques – Description.
- [2] BS EN 62209-1:2006 Human exposure to radio frequency fields from hand-held and body-mounted wireless communication devices — Human models, instrumentation, and procedures — Part 1: Procedure to determine the specific absorption rate (SAR) for hand-held devices used in close proximity to the ear (frequency range of 300 MHz to 3 GHz)
- [3] BS EN 62209-2:2007 Human Exposure to Radio Frequency Fields from Handheld and Body-Mounted Wireless Communication Devices - Human models, Instrumentation, and Procedures - Part 2: Procedure to determine the specific absorption rate (SAR) for mobile wireless communication devices used in close proximity to the human body (frequency range of 30 MHz to 6 GHz)