


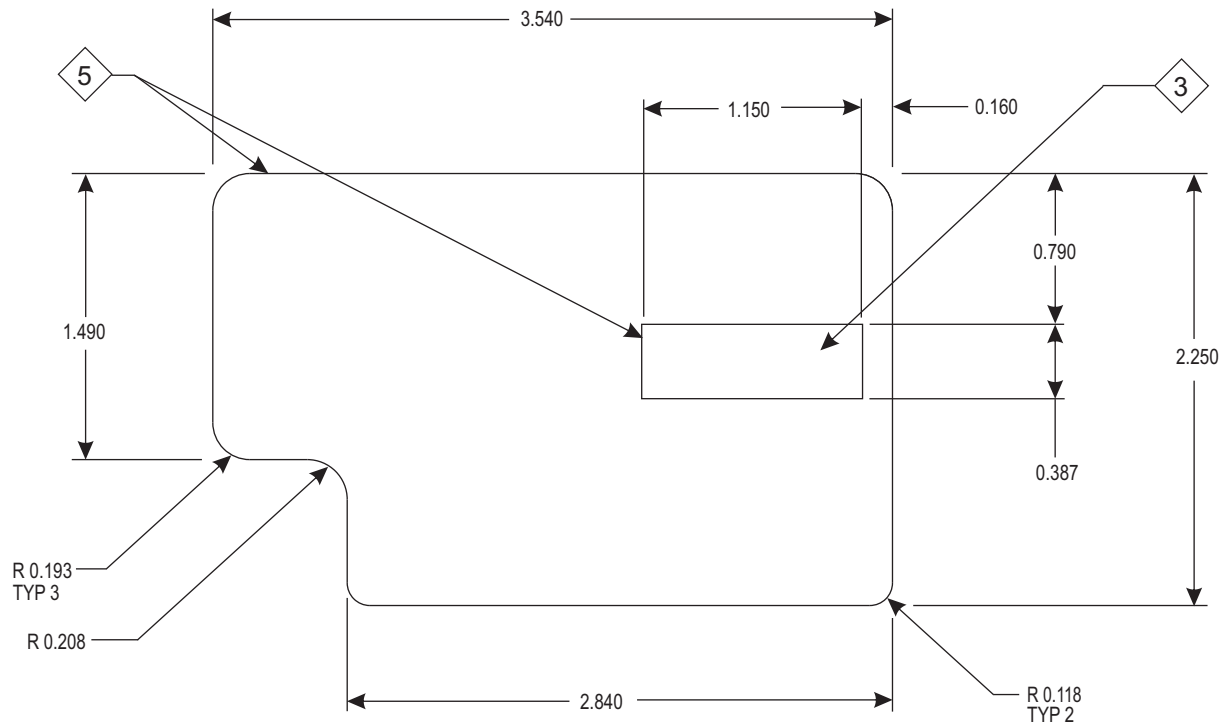

Notes:

1. Material: 0.010 Clear Polycarbonate
Coating: Selective velvet texture over label except Clear Window area.
Adhesive: MIS-01-022-04
Finish: Laminate white barrier layer for opacity (General Formulations PPS2W-STC-OL/53# or equivalent).
Final Thickness: 0.015 ± 0.002 inches
2. Text Copy: Mortara Black per MIS-01-021-05.
Background: Mortara White per MIS-01-021-03.
3. Clear window to be free of adhesive, ink, and texture.
4. The label shall be a "UL" recognized marking and labeling system, for use on various metals, painted surfaces, and plastic, to indicate conformance to this requirement, the supplier shall identify conformance with appropriate markings on direct packaging.
5. Lines depicting label borders are for reference only and should not appear on finished copy.

Dimensions in Inches

Tolerance: +/-0.010 unless otherwise noted.

"ELECTRONIC ORIGINAL" Any Changes To This Document Done Manually Void The Data Base Original.		CONFIDENTIAL This print and the design therein represented are the property of Mortara Instrument, Incorporated, and may not be used in any manner detrimental to its interest. This print has been issued with the understanding that it will not be reproduced, that no disclosure of its contents will be made to others, that it will not be used for manufacture for others, and will be returned upon request.		Mortara INSTRUMENT 7865 N. 86th STREET, MILWAUKEE, WI 53224 TEL. 414-354-1600	
DRAWN BY: GRZinda		DATE: 02/12/09		TITLE: LABEL WAM NAMEPLATE	
DOCUMENTATION CHECKED BY:		DATE:		LATEST DOCUMENT CHANGE:	
ENGINEERING APPROVED BY:		DATE:		DR: 1	
MANUFACTURING APPROVED BY:		DATE:		ECO: XXXX	
Q.A. APPROVED BY:		DATE:		DATE: 02/27/09	
OTHER:		DATE:		BY: GRZinda	
		SCALE: NTS		PART NUMBER:	
		PAGE 1 OF 2		9042 - 069 - 02	
				REV: A1	



Mortara INSTRUMENT
Milwaukee, WI U.S.A.

Wireless Acquisition Module

This device complies with part 15 of the FCC rules.
Operation is subject to the following two conditions:
(1) this device may not cause harmful interference,
and (2) this device must accept any interference
received, including interference that may cause
undesired operation.

FCC ID: HJR-WAM2500 IC: 3758B-WAM2500


MODEL: WAM

SN

REF

MEDICAL EQUIPMENT

IPX1



UL60601-1, IEC60601-1
CAN/CSA C22.2 No. 601.1
IEC60601-2-25

PAGE:	SCALE :	PART NUMBER:	REV:
2 of 2	NTS	9042 - 069 - 02	A1