

Contents

10.APPENDIX.....	50
10.1 Photographs of Test Setup.....	50
10.2. Photographs of the EUT	52

10.APPENDIX

10.1 Photographs of Test Setup

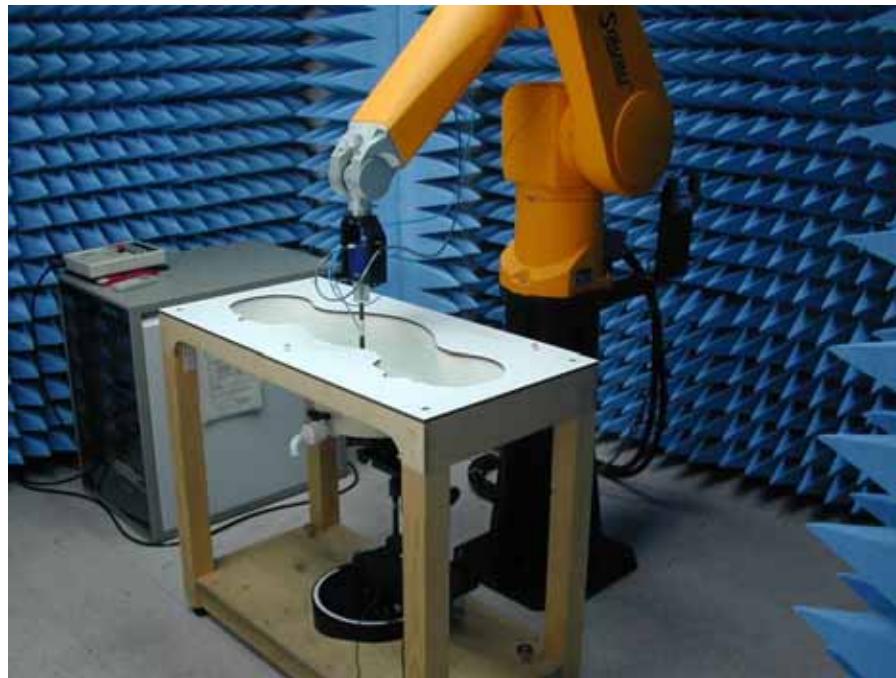


Fig.1 Photograph of the SAR measurement System

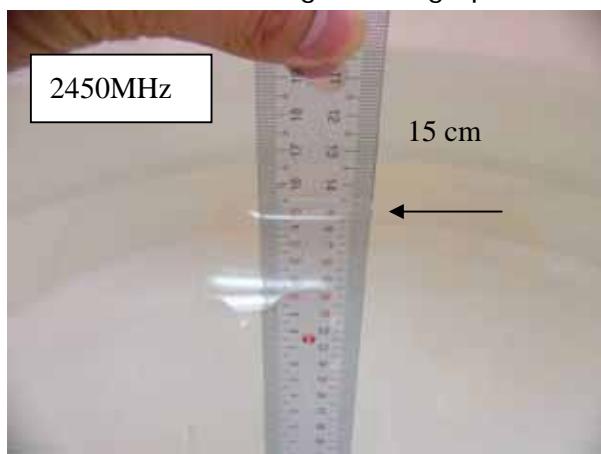


Fig.2 Photograph of the Tissue Simulant Fluid
liquid depth 15cm for Flat (Body)



Fig.7 Body worn- EUT front to flat phantom and distance between flat phantom and mobile phone is 1.5 cm

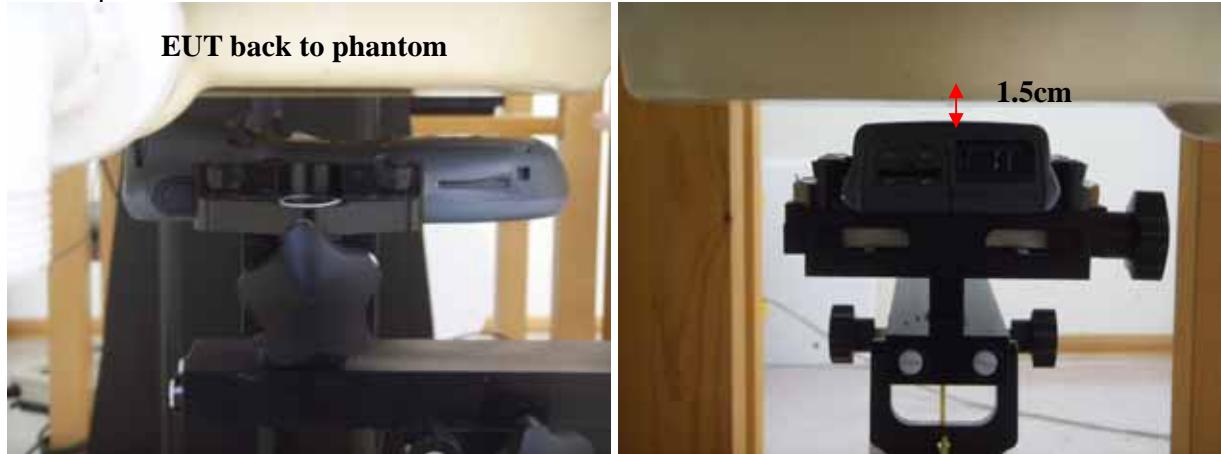


Fig.8 Body worn- EUT back to flat phantom and distance between flat phantom and mobile phone is 1.5 cm

10.2. Photographs of the EUT



Fig.9 Front view of device



Fig.10 Back view of device



Fig.11 Right side view of device



Fig.12 Left side view of device



Fig.13 Front view of Battery



Fig.14 Back view of Battery



Fig.15 Charger

End of Report