

Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China
Tel: +86-10-62304633-2117
E-mail: emf@caict.ac.cn <http://www.caict.ac.cn>

DASY/EASY – Parameters of Probe: EX3DV4 – SN:3767

Calibration Parameter Determined in Head Tissue Simulating Media

f [MHz] ^C	Relative Permittivity ^F	Conductivity (S/m) ^F	ConvF X	ConvF Y	ConvF Z	Alpha ^G	Depth ^G (mm)	Unct. (k=2)
750	41.9	0.89	9.84	9.84	9.84	0.16	1.29	± 12.7%
835	41.5	0.90	9.50	9.50	9.50	0.16	1.37	± 12.7%
900	41.5	0.97	9.44	9.44	9.44	0.17	1.32	± 12.7%
1450	40.5	1.20	8.55	8.55	8.55	0.22	1.02	± 12.7%
1750	40.1	1.37	8.30	8.30	8.30	0.25	1.05	± 12.7%
1900	40.0	1.40	8.05	8.05	8.05	0.25	1.04	± 12.7%
2000	40.0	1.40	8.07	8.07	8.07	0.23	1.10	± 12.7%
2300	39.5	1.67	7.85	7.85	7.85	0.65	0.66	± 12.7%
2450	39.2	1.80	7.60	7.60	7.60	0.64	0.68	± 12.7%
2600	39.0	1.96	7.44	7.44	7.44	0.65	0.68	± 12.7%
3300	38.2	2.71	7.12	7.12	7.12	0.53	0.84	± 13.9%
3500	37.9	2.91	6.92	6.92	6.92	0.47	0.97	± 13.9%
3700	37.7	3.12	6.72	6.72	6.72	0.43	1.04	± 13.9%
3900	37.5	3.32	6.62	6.62	6.62	0.35	1.35	± 13.9%
4100	37.2	3.53	6.52	6.52	6.52	0.40	1.15	± 13.9%
4400	36.9	3.84	6.32	6.32	6.32	0.40	1.25	± 13.9%
4600	36.7	4.04	6.26	6.26	6.26	0.35	1.40	± 13.9%
4800	36.4	4.25	6.25	6.25	6.25	0.40	1.40	± 13.9%
4950	36.3	4.40	5.90	5.90	5.90	0.45	1.25	± 13.9%
5200	36.0	4.66	5.50	5.50	5.50	0.40	1.45	± 13.9%
5300	35.9	4.76	5.32	5.32	5.32	0.40	1.45	± 13.9%
5500	35.6	4.96	4.93	4.93	4.93	0.45	1.40	± 13.9%
5600	35.5	5.07	4.85	4.85	4.85	0.45	1.40	± 13.9%
5800	35.3	5.27	4.91	4.91	4.91	0.50	1.30	± 13.9%

^C Frequency validity above 300 MHz of ±100MHz only applies for DASY v4.4 and higher (Page 2), else it is restricted to ±50MHz. The uncertainty is the RSS of ConvF uncertainty at calibration frequency and the uncertainty for the indicated frequency band. Frequency validity below 300 MHz is ± 10, 25, 40, 50 and 70 MHz for ConvF assessments at 30, 64, 128, 150 and 220 MHz respectively. Above 5 GHz frequency validity can be extended to ± 110 MHz.

^F At frequency up to 6 GHz, the validity of tissue parameters (ϵ and σ) can be relaxed to ±10% if liquid compensation formula is applied to measured SAR values. The uncertainty is the RSS of the ConvF uncertainty for indicated target tissue parameters.

^G Alpha/Depth are determined during calibration. SPEAG warrants that the remaining deviation due to the boundary effect after compensation is always less than ± 1% for frequencies below 3 GHz and below ± 2% for the frequencies between 3-6 GHz at any distance larger than half the probe tip diameter from the boundary.

Certificate No: 24J02Z000483

Page 4 of 9




In Collaboration with
s p e a g
CALIBRATION LABORATORY




Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China
Tel: +86-10-62304633-2117
E-mail: emf@caict.ac.cn <http://www.caict.ac.cn>

Frequency Response of E-Field (TEM-Cell: ifi110 EXX, Waveguide: R22)

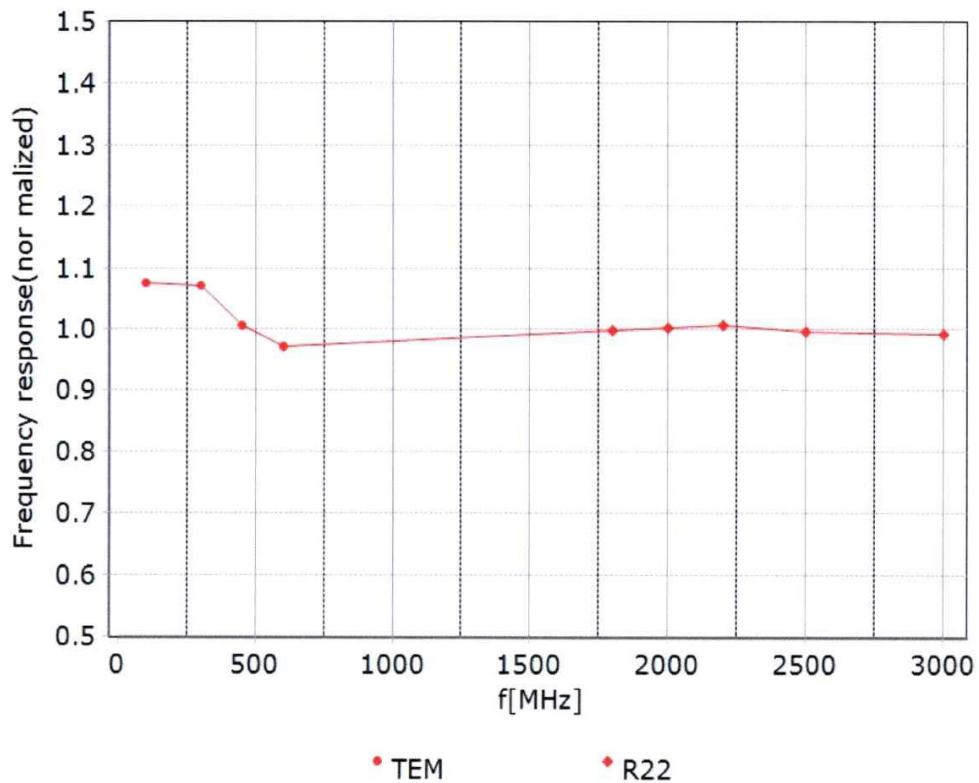


Uncertainty of Frequency Response of E-field: $\pm 7.4\%$ ($k=2$)

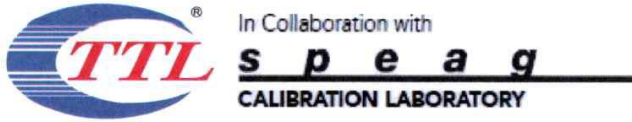



Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China
 Tel: +86-10-62304633-2117
 E-mail: emf@caict.ac.cn <http://www.caict.ac.cn>

Receiving Pattern (Φ), $\theta=0^\circ$


f=600 MHz, TEM

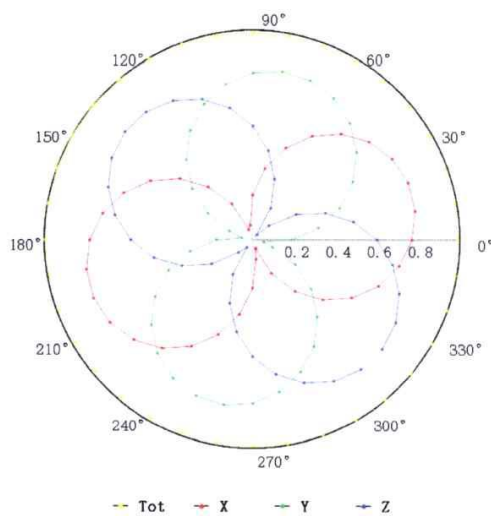

f=1800 MHz, R22

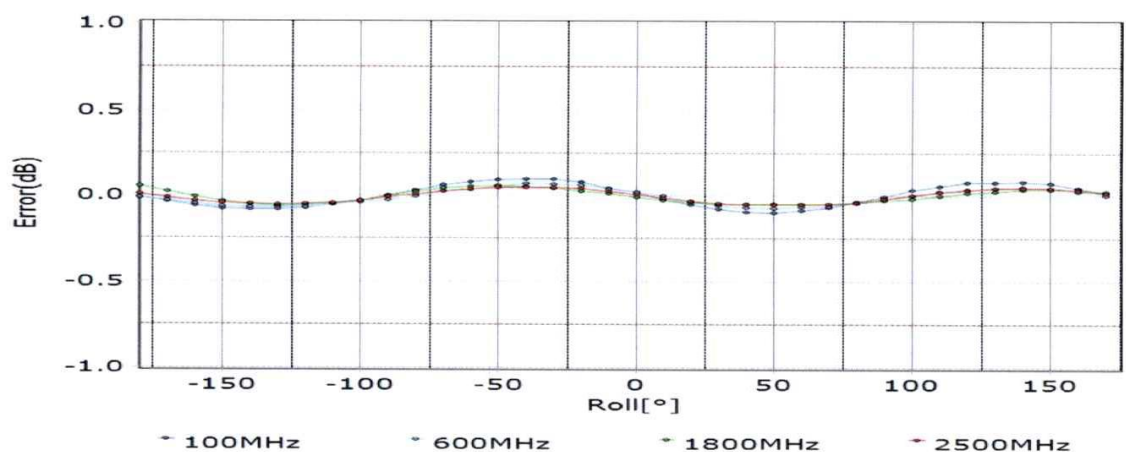
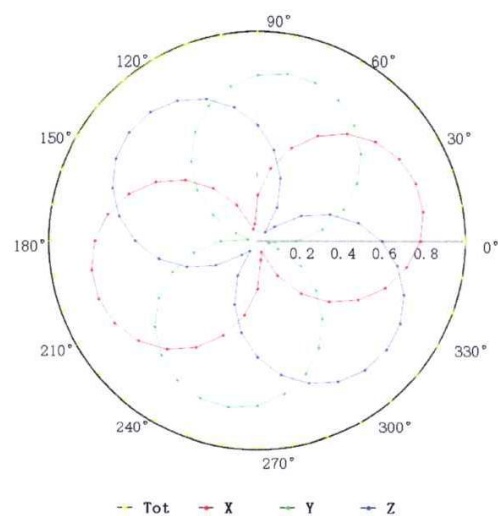


Uncertainty of Axial Isotropy Assessment: $\pm 1.2\%$ ($k=2$)

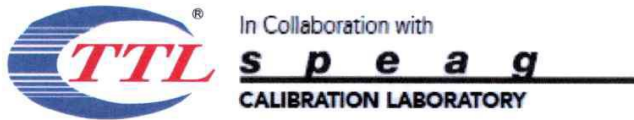


Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China
 Tel: +86-10-62304633-2117
 E-mail: emf@caict.ac.cn <http://www.caict.ac.cn>

Dynamic Range f(SAR_{head}) (TEM cell, f = 900 MHz)

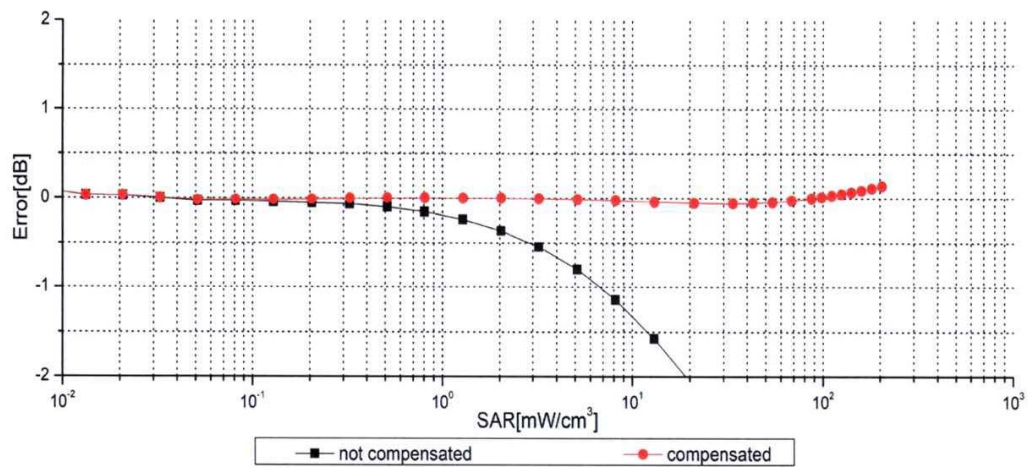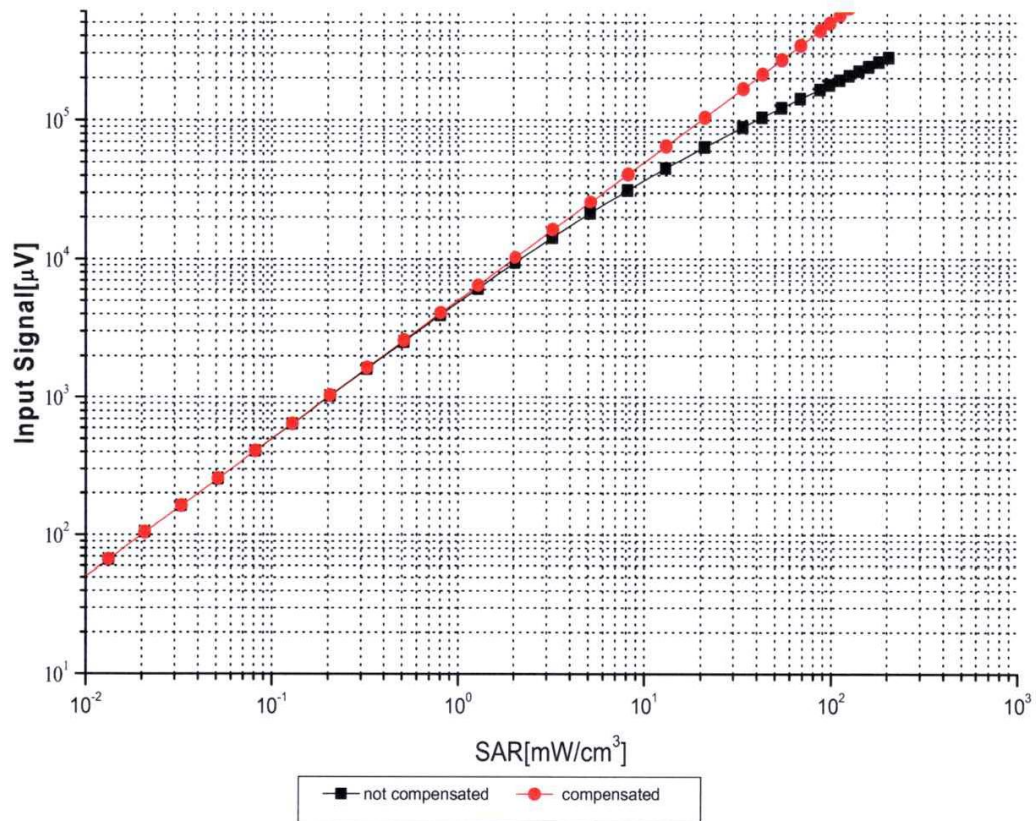

Uncertainty of Linearity Assessment: $\pm 0.9\%$ ($k=2$)





Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China
 Tel: +86-10-62304633-2117
 E-mail: emf@caict.ac.cn <http://www.caict.ac.cn>


Conversion Factor Assessment

f=750 MHz,WGLS R9(H_convF)


f=1750 MHz,WGLS R22(H_convF)

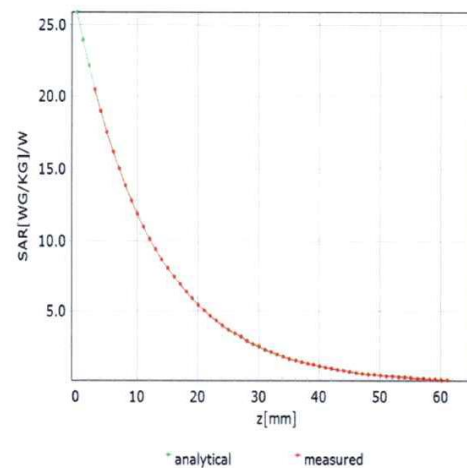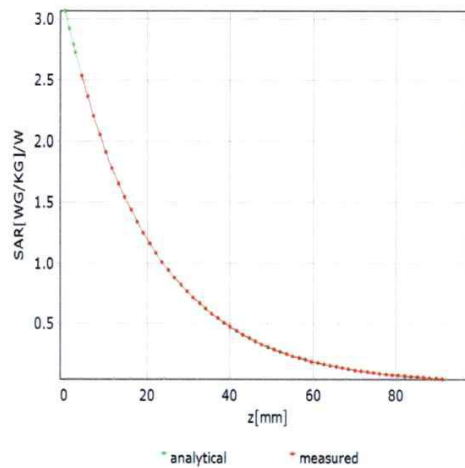

Deviation from Isotropy in Liquid

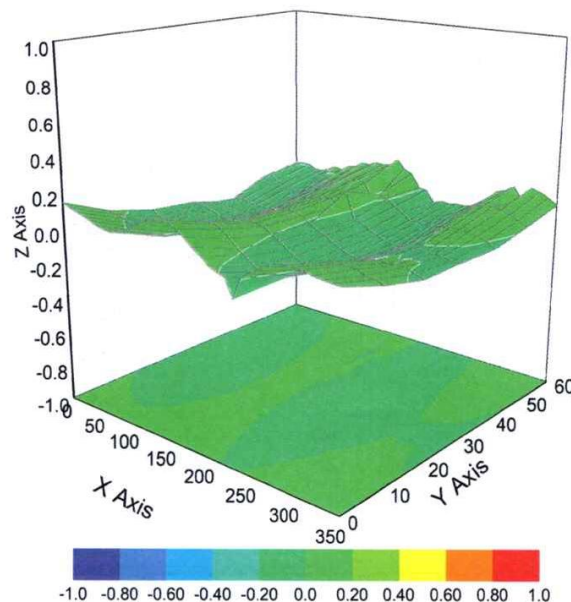

Uncertainty of Spherical Isotropy Assessment: $\pm 3.2\%$ ($k=2$)



Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China
Tel: +86-10-62304633-2117
E-mail: emf@caict.ac.cn <http://www.caict.ac.cn>

DASY/EASY – Parameters of Probe: EX3DV4 – SN:3767

Other Probe Parameters

Sensor Arrangement	Triangular
Connector Angle (°)	151.2
Mechanical Surface Detection Mode	enabled
Optical Surface Detection Mode	disable
Probe Overall Length	337mm
Probe Body Diameter	10mm
Tip Length	9mm
Tip Diameter	2.5mm
Probe Tip to Sensor X Calibration Point	1mm
Probe Tip to Sensor Y Calibration Point	1mm
Probe Tip to Sensor Z Calibration Point	1mm
Recommended Measurement Distance from Surface	1.4mm