

TEST REPORT

Report Number: 3109551-002b

June 12, 2007

Product Designation: M/N: 200-17RF, FCC ID: HNB200-17RF

Standard: 47 CFR Part 15, Subpart C (15.231 - Periodic operation in the band
40.66-40.70 MHz and above 70 MHz)

Tested by:

Intertek Testing Services NA Inc.
1950 Evergreen Blvd., Suite 100
Duluth, GA 30096

Client:

American Medical Alert Corp
3636 33rd Street
Long Island City, NY 11106
Contact: John Collins
Phone: 800.286.2622
Fax: 516.536.5276

Tests performed by:



Richard C. Bianco
EMC Project Engineer

Report reviewed by:



David J. Schramm
EMC Department Manager

All services undertaken are subject to the following general policy: This report is for the exclusive use of Intertek's Client and is provided pursuant to the agreement between Intertek and its Client. Intertek's responsibility and liability are limited to the terms and conditions of the agreement. Intertek assumes no liability to any party, other than to the Client in accordance with the agreement, for any loss, expense or damage occasioned by the use of this report. Only the Client is authorized to copy or distribute this report and then only in its entirety. Any use of the Intertek name or one of its marks for the sale or advertisement of the tested material, product or service must first be approved in writing by Intertek. The observations and test results in this report are relevant only to the sample tested. This report by itself does not imply that the material, product, or service is or has ever been under an Intertek certification program. This report must not be used to claim product endorsement by A2LA, NIST, or any agency of the US Government.

1.0 Introduction and Conclusion

The tests indicated in section 2.0 were performed on the product constructed as described in section 3.0. The remaining test sections are the verbatim text from the actual data sheets used during the investigation. These test sections include the test name, the specified test Method, a list of the actual Test Equipment Used, documentation Photos, Results and raw Data. No additions, deviations, or exclusions have been made from the standard(s) unless specifically noted.

Based on the results of our investigation, we have concluded the product tested complies with the requirements of the standard(s) indicated. The results obtained in this test report pertain only to the item(s) tested.

2.0 Test Summary

Section	Test Full Name	Test Date	Result
4.0	System setup including cable interconnection details, support equipment and simplified block diagram. (System Setup)		
5.0	Overview of EUT (Low Power Transmitters) (FCC 15C - EUT Overview)	12/12/2006	
6.0	Restrictions (FCC 15C - 15.231(a))	12/12/2006	
7.0	Duty Cycle Determination (FCC 15A - 15.35(c))	12/12/2006	PASS
8.0	Radiated Emissions (FCC 15C - 15.231(b))	12/12/2006	PASS
9.0	Bandwidth Requirements (FCC 15C - 15.231(c))	12/12/2006	PASS

3.0 Description of Equipment Under Test

Equipment Under Test			
Description	Manufacturer	Model Number	Serial Number
433MHz Smoke Alarm	American Medical Alert Inc.	200-17RF	NA

EUT receive date:	12/11/2006
EUT receive condition:	Good

Description of EUT provided by Client:

The Transmitter is designed for use in a smoke detector.

Description of EUT exercising:

The EUT was placed in a continuous transmit mode during the emissions portion of the testing and in a normal operating state during the duty cycle measurements.

4.0 System setup including cable interconnection details, support equipment and simplified block diagram. (System Setup)

Method:

Record the details of EUT cabling, document the support equipment, and show the interconnections in a block diagram.

Drawing:



Block Diagram

4.0 System setup including cable interconnection details, support equipment and simplified block diagram. (System Setup)

Data:

EUT Cabling						
ID	Description	Length	Shielding	Ferrites	Connection	
					From	To
	None					

Support Equipment			
Description	Manufacturer	Model Number	Serial Number
None			

5.0 Overview of EUT (Low Power Transmitters) (FCC 15C - EUT Overview)**Method:**

Complete the overview spreadsheet.

Related Submittal(s) Grants: This report is for use with an application for certification of a low power transmitter. One transmitter is included in the application.

Data:

Applicant	American Medical Alert Incorporated
	3636 33rd St.
	Long Island City, NY 11106
Trade Name & Model No.	200-17RF
FCC Identifier	HNB200-17RF
Use of product	Smoke Alarm Transmitter
Transmitter activation	☐ Manual and automatically deactivate within 5 seconds of being released
	☒ Periodic transmissions
Frequency Range (MHz)	433
Antenna Type (15.203)	Intergrated - permanently attached
Manufacturer name & address	American Medical Alert Incorporated
	3636 33rd St.
	Long Island City, NY 11106
Related Submittals and Grants:	This report is for use with an application for certification of a low power transmitter. One transmitter is included in the application.
Additions, deviations and exclusions from standards	None

6.0 Restrictions (FCC 15C - 15.231(a))

Method:

15.231(a) The provisions of this section are restricted to periodic operation within the band 40.66-40.70 MHz and above 70 MHz. Except as shown in paragraph (e) of this section, the intentional radiator is restricted to the transmission of a control signal such as those used with alarm systems, door openers, remote switches, etc. Continuous transmissions, voice, video and the radio control of toys are not permitted. Data is permitted to be sent with a control signal. The following conditions shall be met to comply with the provisions for this periodic operation:


- (1) A manually operated transmitter shall employ a switch that will automatically deactivate the transmitter within not more than 5 seconds of being released.
- (2) A transmitter activated automatically shall cease transmission within 5 seconds after activation.
- (3) Periodic transmissions at regular predetermined intervals are not permitted. However, polling or supervision transmissions, including data, to determine system integrity of transmitters used in security or safety applications are allowed if the total duration of transmissions does not exceed more than two seconds per hour for each transmitter. There is no limit on the number of individual transmissions, provided the total transmission time does not exceed two seconds per hour.
- (4) Intentional radiators which are employed for radio control purposes during emergencies involving fire, security, and safety of life, when activated to signal an alarm, may operate during the pendency of the alarm condition
- (5) Transmission of set-up information for security systems may exceed the transmission duration limits in paragraphs (a)(1) and (a)(2) of this section, provided such transmissions are under the control of a professional installer and do not exceed ten seconds after a manually operated switch is released or a transmitter is activated automatically. Such set-up information may include data.

6.0 Restrictions (FCC 15C - 15.231(a))

Drawing:



Delta 1 [T1] RBW 100 kHz RF Att 10 dB
 Ref Lvl -46.66 dB VBW 300 kHz
 90 dBμV 1.202365 s SWT 5 s Unit dBμV

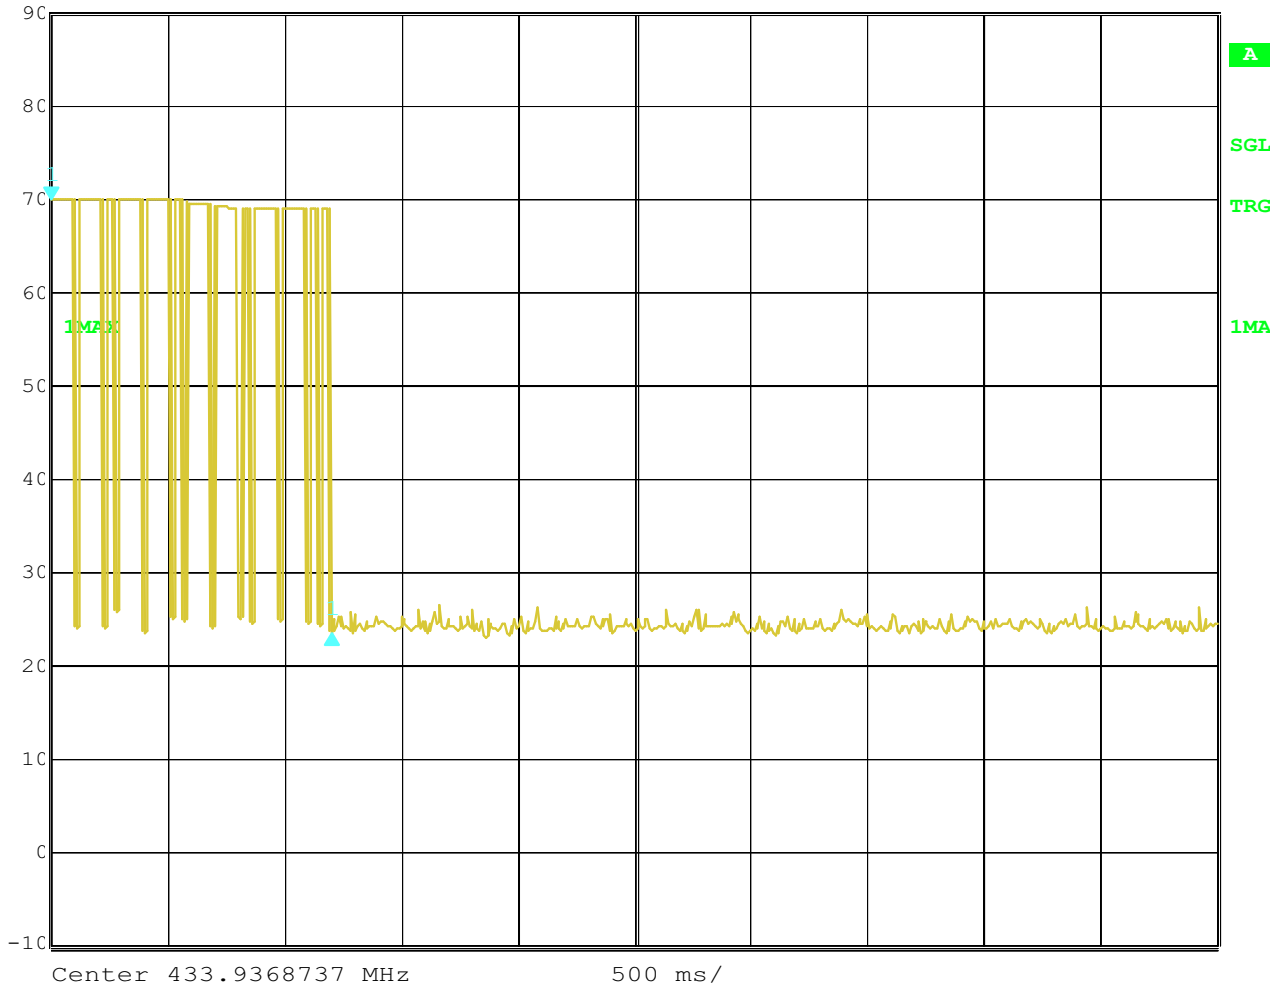

Date: 29.DEC.2006 10:11:56

Deactivation within 5 seconds

6.0 Restrictions (FCC 15C - 15.231(a))

Data:

15.231(a)	Response	Requirement
Frequency Range (Mhz, max)	433	40.66-40.70 MHz and > 70MHz
Frequency Range (MHz, min)	433	40.66-40.70 MHz and > 70MHz
Transmit only control signal?	Yes	Only control signal allowed
Continuous transmission?	No	No
Voice transmission?	No	No
Video transmission?	No	No
Radio control of toy?	No	No

15.231(a)(1)		
Manually operated?	No	
Deactivates within 5 seconds?	N/A	Yes
Show plot (10 second sweep)	N/A	

15.231(a)(2)		
Automatically operated?	Yes	
Deactivates within 5 seconds?	Yes	Yes
Show plot (10 second sweep)	Yes	

15.231(a)(3)		
Periodically transmits at predetermined intervals?	No	No
Polling signals?	No	Allowed, with restrictions
Polling rate and timing	No	< 2 seconds per hour

15.231(a)(4)		
For Emergency Use?	Yes	Allowed

15.231(a)(5)		
Exceed 15.231(a)(1) or (a)(2) requirements?	No	Allowed for professional install

7.0 Duty Cycle Determination (FCC 15A - 15.35(c))

Method:

(c) Unless otherwise specified, e.g. §15.255(b), when the radiated emission limits are expressed in terms of the average value of the emission, and pulsed operation is employed, the measurement field strength shall be determined by averaging over one complete pulse train, including blanking intervals, as long as the pulse train does not exceed 0.1 seconds. As an alternative (provided the transmitter operates for longer than 0.1 seconds) or in cases where the pulse train exceeds 0.1 seconds, the measured field strength shall be determined from the average absolute voltage during a 0.1 second interval during which the field strength is at its maximum value. The exact method of calculating the average field strength shall be submitted with any application for certification or shall be retained in the measurement data file for equipment subject to notification or verification.

Determine the period of the pulse train, T, in mSec and record the results. T is defined as the time from the beginning of one pulse train to the beginning of the next pulse train.

Count the number of different types of pulses, N and record the results.

For each of the different types of pulses, count the number of occurrences within one pulse train.


Use the Duty Cycle Correction Factor, DCCF, from the results table and use it to adjust the field strength measurements recorded for radiated emissions.

Test Equipment Used:

Description:	Manufacturer:	Model:	Asset Number:	Cal Date:	Cal Due:
Cable E05 (Formerly HS 1500 N-N)	Huber-Suhner	Sucoflex 104PEA	E05	05/11/2006	05/11/2007
Spectrum Analyzer, 20 Hz to 40 GHz	Rohde & Schwarz	FSEK30	200062	01/12/2006	01/12/2007


Results: The sample tested was found to Comply.

Plot:

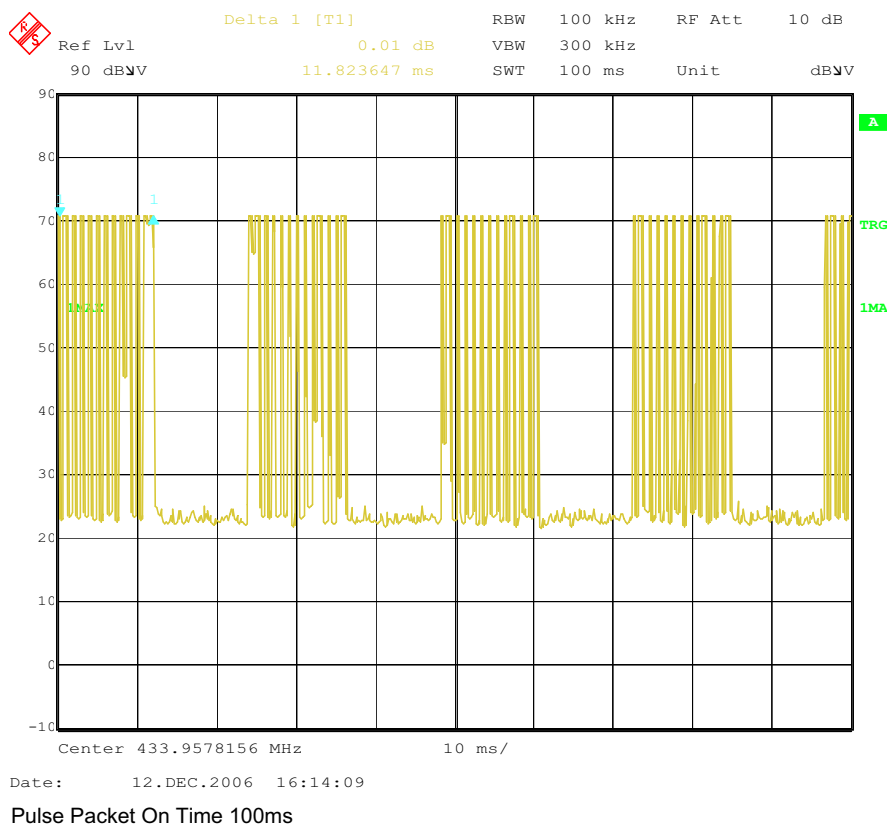

7.0 Duty Cycle Determination (FCC 15A - 15.35(c))

Plot:

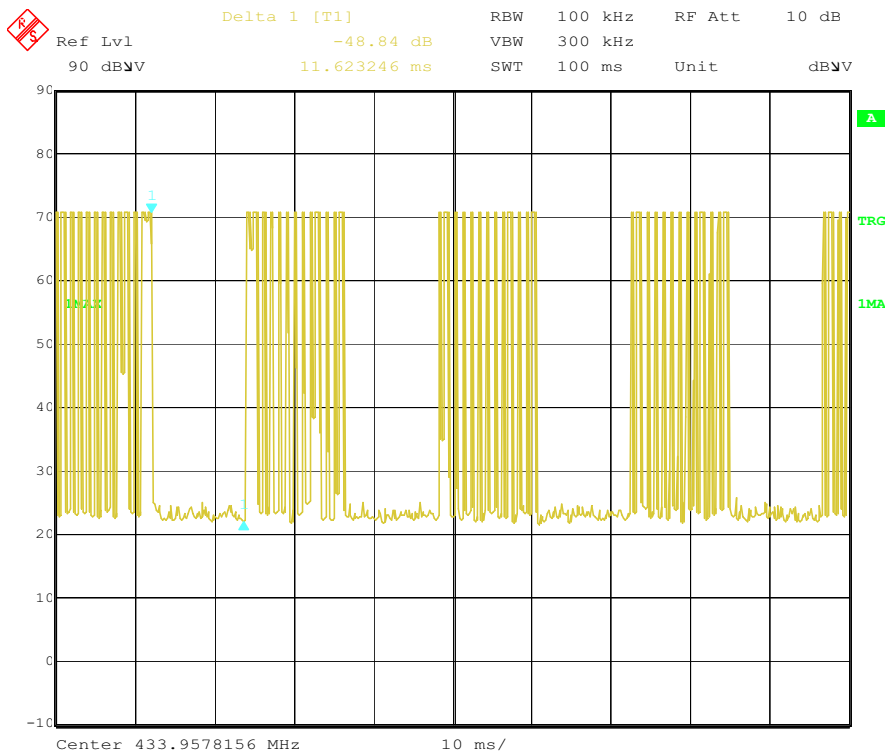


Date: 12.DEC.2006 16:14:50

Pulse Packet Off Time 100ms

7.0 Duty Cycle Determination (FCC 15A - 15.35(c))

Plot:

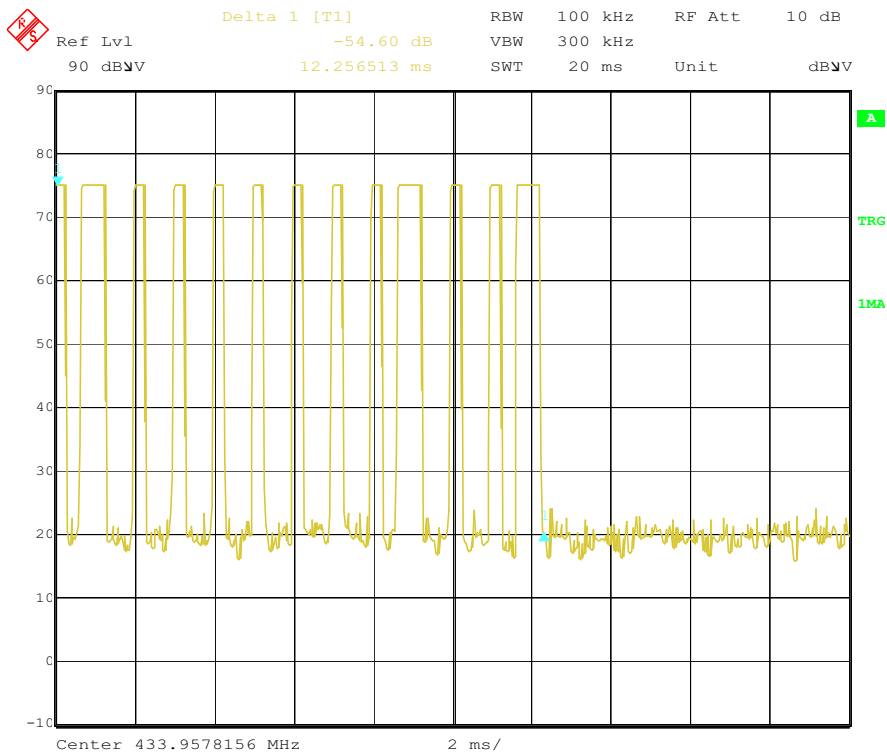


Date: 12.DEC.2006 16:16:50

Single Pulse On Time 20ms

7.0 Duty Cycle Determination (FCC 15A - 15.35(c))

Plot:

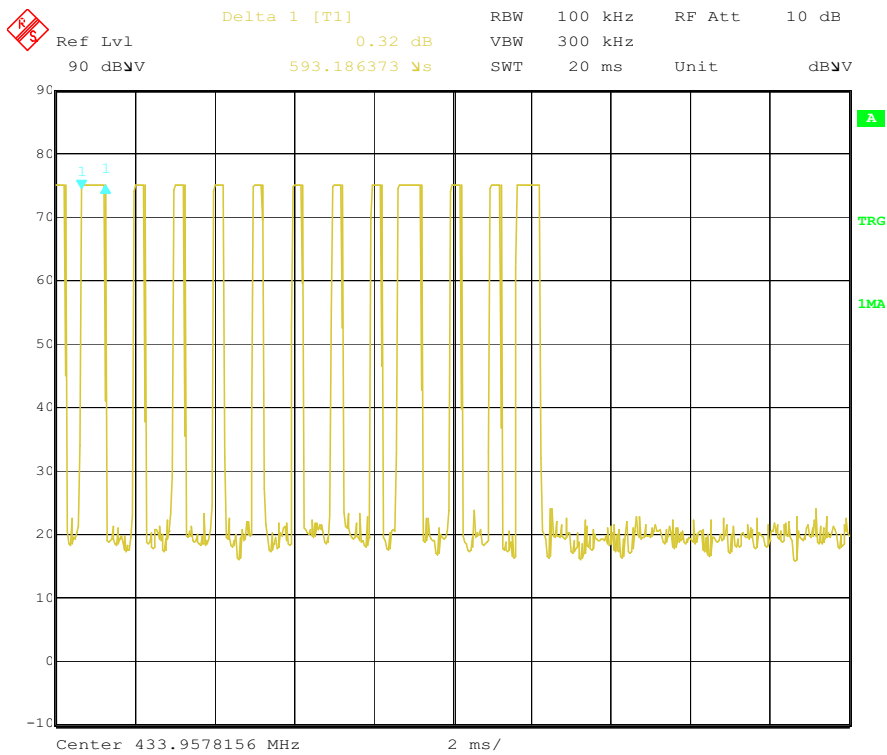


Date: 12.DEC.2006 16:18:41

Large Pulse On Time

7.0 Duty Cycle Determination (FCC 15A - 15.35(c))

Plot:

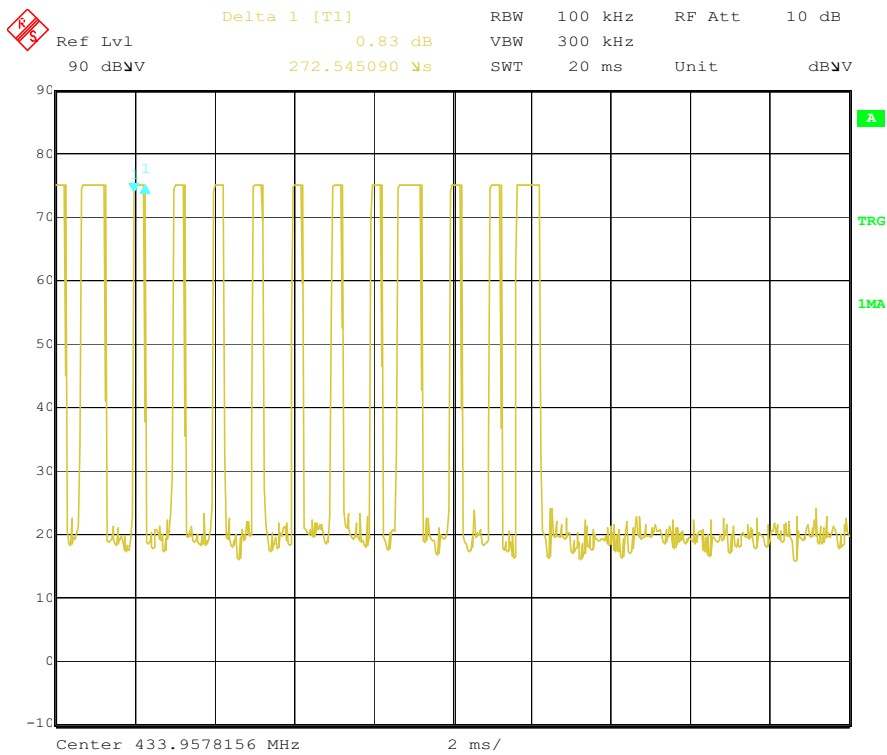

Date: 12.DEC.2006 16:19:29

Small Pulse On Time

7.0 Duty Cycle Determination (FCC 15A - 15.35(c))

Data:

Duration of Pulse Train, T (mSec):	100
Averaging Interval, A_I (mSec):	100
Number of different Pulses, N:	56

	Number (#P _x)	Pulse Width, mSec (PW _x)	Product (#P _x)*(PW _x)
Pulse Width 1	13	0.593	7.709
Pulse Width 2	43	0.273	11.739
Pulse Width 3			
Pulse Width 4			
Pulse Width 5			
Pulse Width 6			
Pulse Width 7			
Pulse Width 8			
Pulse Width 9			
Pulse Width 10			

Duty Cycle:	0.19448
Duty Cycle Correction Factor, dB:	-14.2

$$T_{on} = (PW_1 * \#P_1) + (PW_2 * \#P_2) + \dots + (PW_n * \#P_n)$$

$$DutyCycle = T_{on} \div A_I$$

$$DCCF = 20 * \log_{10}(DutyCycle)$$

8.0 Radiated Emissions (FCC 15C - 15.231(b))

Method:

(b) In addition to the provisions of §15.205, the field strength of emissions from intentional radiators operated under this section shall not exceed the limits specified in FCC Part 15.231(b).

Intentional radiators operating under the provisions of this section shall demonstrate compliance with the limits on the field strength of emissions, as shown in the above table, based on the average value of the measured emissions. As an alternative, compliance with the limits in the above table may be based on the use of measurement instrumentation with a CISPR quasi-peak detector. The specific method of measurement employed shall be specified in the application for equipment authorization. If average emission measurements are employed, the provisions in §15.35 for averaging pulsed emissions and for limiting peak emissions apply. Further, compliance with the provisions of §15.205 shall be demonstrated using the measurement instrumentation specified in that section.

The limits on the field strength of the spurious emissions in the above table are based on the fundamental frequency of the intentional radiator. Spurious emissions shall be attenuated to the average (or, alternatively, CISPR quasi-peak) limits shown in this table or to the general limits shown in §15.209, whichever limit permits a higher field strength.

For radiated emission measurements, the EUT is attached to a styro-foam block and placed on a non-conductive table whose top is 80cm above the ground plane. If the EUT is handheld, the signal shall be maximized through rotation and placement in the three orthogonal axes.

During the test the EUT is rotated and the antenna height and polarization are varied during the search for maximum signal level. The antenna height is varied from 1 to 4 meters.

Radiated emissions are taken at 3 meters unless the signal level is too low for measurement at that distance. If necessary, a pre-amplifier is used and/or the test is conducted at a closer distance. All readings are extrapolated back to the equivalent 3-meter reading using inverse scaling with distance.

Radiated emission measurements were performed from 30 MHz to 10 times the highest frequency generated in the EUT.

Analyzer resolution is:

- 100 kHz or greater for frequencies 1000 MHz and below,
- 1 MHz for frequencies above 1000 MHz.

The Peak value of the Field Strength was measured. The Average value was obtained from the Peak by subtracting the Duty Cycle Correction Factor.

Test Equipment Used:

Description:	Manufacturer:	Model:	Asset Number:	Cal Date:	Cal Due:
Antenna, Bilog (20MHz to 2GHz)	Chase	CBL6112B	211386	08/29/2006	08/29/2007
Attenuator, 10 dB	Weinschel Corp	2	200009	07/18/2006	07/18/2007
Cable E01 (Formerly PE7000N-N2 or N2)	Pasternack	RG214/U	E01	05/11/2006	05/11/2007
Cable E05 (Formerly HS 1500 N-N)	Huber-Suhner	Sucoflex 104PEA	E05	05/11/2006	05/11/2007
Cable E11 (Formerly HS 7000 N-SMA)	Huber-Suhner	Sucoflex 104PEA	E11 211266	05/11/2006	05/11/2007
Cable E20 (Formerly Cable 8)	United Microwave Pro	Micropore 190 577	E20	05/12/2006	05/12/2007
Cable, 18 GHz, N, 394 inches	Megaphase	G919-NKNK-394	MP3	05/11/2006	05/11/2007
Coaxial Cable, 6ft, N(Male) to N(Male)	Mini-Circuits	CBL-6FT-NMNM	TT1	05/11/2006	05/11/2007
EMI Receiver	Hewlett Packard	8546A	211388	08/04/2006	08/04/2007
EMI Receiver, Preselector section	Hewlett Packard	85460A	211389	08/04/2006	08/04/2007
Excel spreadsheet for radiated emissions	Software	Excel - RE Worksh	SW004	08/01/2006	08/01/2007
Preamplifier, 10 MHz to 2000 MHz, 27 dB gain	Mini-Circuits	ZKL-2	200074	01/24/2006	01/24/2007
Preamplifier, 1-26 GHz	Hewlett Packard	8449B	213191	05/04/2006	05/04/2007
Spectrum Analyzer, 20 Hz to 40 GHz	Rohde & Schwarz	FSEK30	200062	01/12/2006	01/12/2007
Tile software profile for radiated and conducted emissions testing.	Software	Tile - Emissions	SW006	06/25/2006	06/25/2007

Results: The sample tested was found to Comply.

8.0 Radiated Emissions (FCC 15C - 15.231(b))**Photo:**


Rear View

8.0 Radiated Emissions (FCC 15C - 15.231(b))**Photo:**

Front View

8.0 Radiated Emissions (FCC 15C - 15.231(b))


Plot:

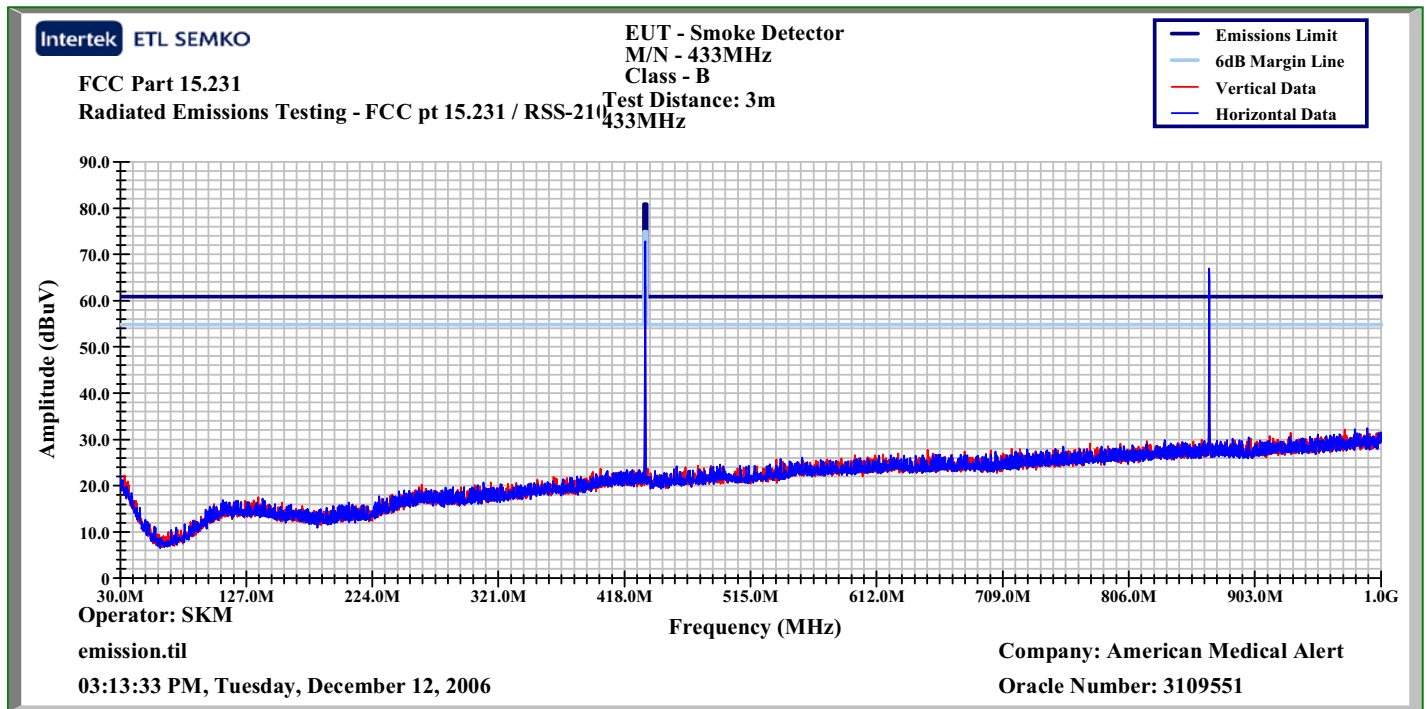

30-1000MHz

8.0 Radiated Emissions (FCC 15C - 15.231(b))

Plot:

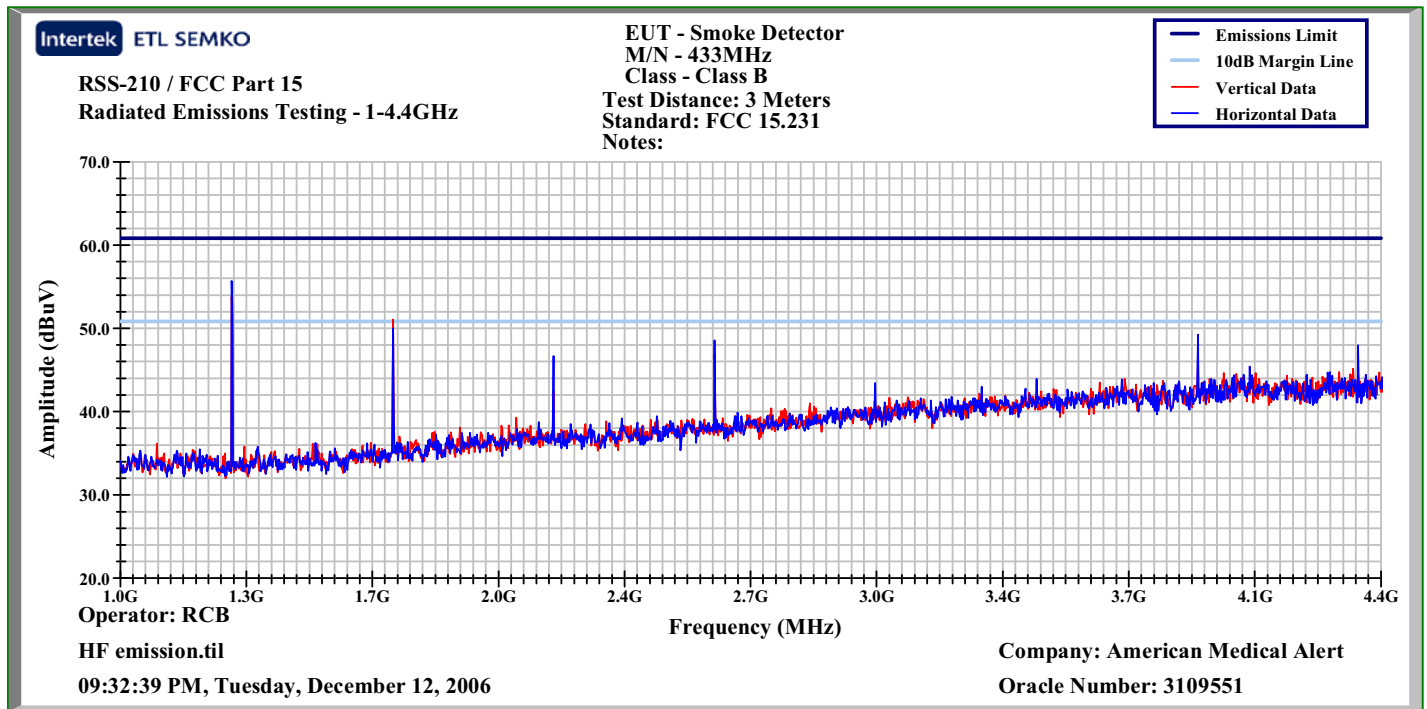

1000-5000MHz

8.0 Radiated Emissions (FCC 15C - 15.231(b))

Data:

Frequency Range (MHz): 30-1000

Test Distance (m): 3m

Input power: Battery

Modifications for compliance (y/n): No

A	B	C	D	E	F	G	H	I	J	K
Ant. Pol. (V/H)	Frequency MHz	Reading dB(uV)	Antenna Factor dB(1/m)	Cable Loss dB	Pre-amp Factor dB	Duty Cycle Factor dB	Net dB(uV/m)	3m Limit dB(uV/m)	Margin dB	Axis / Detector
V	433.900	82.8	17.0	3.8	27.9	0.0	75.7	100.8	-25.1	X/P
V	433.900	82.8	17.0	3.8	27.9	14.2	61.5	80.8	-19.3	X/A
H	433.900	74.6	17.2	3.8	27.9	0.0	67.7	100.8	-33.1	X/P
H	433.900	74.6	17.2	3.8	27.9	14.2	53.5	80.8	-27.3	X/A
V	433.900	82.8	17.0	3.8	27.9	0.0	75.7	100.8	-25.1	Y/P
V	433.900	82.8	17.0	3.8	27.9	14.2	61.5	80.8	-19.3	Y/A
H	433.900	74.6	17.2	3.8	27.9	0.0	67.7	100.8	-33.1	Y/P
H	433.900	74.6	17.2	3.8	27.9	14.2	53.5	80.8	-27.3	Y/A
V	433.900	69.2	17.0	3.8	27.9	0.0	62.1	100.8	-38.7	Z/P
V	433.900	69.2	17.0	3.8	27.9	14.2	47.9	80.8	-32.9	Z/A
H	433.900	81.7	17.2	3.8	27.9	0.0	74.8	100.8	-26.0	Z/P
H	433.900	81.7	17.2	3.8	27.9	14.2	60.6	80.8	-20.2	Z/A
V	867.811	64.5	20.7	5.2	27.7	0.0	62.7	80.8	-18.1	X/P
V	867.811	64.5	20.7	5.2	27.7	14.2	48.5	60.8	-12.3	X/A
H	867.811	65.0	21.4	5.2	27.7	0.0	64.0	80.8	-16.8	X/P
H	867.811	65.0	21.4	5.2	27.7	14.2	49.8	60.8	-11.0	X/A
V	867.811	64.5	20.7	5.2	27.7	0.0	62.8	80.8	-18.1	Y/P
V	867.811	64.5	20.7	5.2	27.7	14.2	48.6	60.8	-12.3	Y/A
H	867.811	65.0	21.4	5.2	27.7	0.0	64.0	80.8	-16.9	Y/P
H	867.811	65.0	21.4	5.2	27.7	14.2	49.8	60.8	-11.1	Y/A
V	867.811	58.4	20.7	5.2	27.7	0.0	56.6	80.8	-24.2	Z/P
V	867.811	58.4	20.7	5.2	27.7	14.2	42.4	60.8	-18.4	Z/A
H	867.811	67.1	21.4	5.2	27.7	0.0	66.1	80.8	-14.7	Z/P
H	867.811	67.1	21.4	5.2	27.7	14.2	51.9	60.8	-8.9	Z/A
Calculations		H=C+D+E-F-G			J=H-I					

Tabular Data - 30-1000MHz

8.0 Radiated Emissions (FCC 15C - 15.231(b))

Data:

Frequency Range (MHz): 1000-5000

Test Distance (m): 3m

Input power: Battery

Modifications for compliance (y/n): No

A	B	C	D	E	F	G	H	I	J	K
Ant. Pol. (V/H)	Frequency MHz	Reading dB(uV)	Antenna Factor dB(1/m)	Cable Loss dB	Pre-amp Factor dB	Duty Cycle	Net dB(uV/m)	3m Limit dB(uV/m)	Margin dB	Axis / Detector
V	1301.720	63.5	24.3	6.2	37.2	0.0	56.8	80.8	-24.0	X/P
V	1301.720	63.5	24.3	6.2	37.2	14.4	42.4	60.8	-18.4	X/A
H	1301.720	66.7	24.5	6.2	37.2	0.0	60.2	80.8	-20.6	X/P
H	1301.720	66.7	24.5	6.2	37.2	14.4	45.8	60.8	-15.0	X/A
V	1301.720	63.5	24.3	6.2	37.2	0.0	56.8	80.8	-24.0	Y/P
V	1301.720	63.5	24.3	6.2	37.2	14.4	42.4	60.8	-18.4	Y/P
H	1301.720	66.7	24.5	6.2	37.2	0.0	60.3	80.8	-20.5	Y/P
H	1301.720	66.7	24.5	6.2	37.2	14.4	45.9	60.8	-14.9	Y/P
V	1301.720	60.4	24.3	6.2	37.2	0.0	53.7	80.8	-27.1	Z/P
V	1301.720	60.4	24.3	6.2	37.2	14.4	39.3	60.8	-21.5	Z/A
H	1301.720	67.6	24.5	6.2	37.2	0.0	61.2	80.8	-19.6	Z/P
H	1301.720	67.6	24.5	6.2	37.2	14.4	46.8	60.8	-14.0	Z/A
V	1735.634	59.3	25.1	6.2	36.2	0.0	54.4	80.8	-26.4	X/P
V	1735.634	59.3	25.1	6.2	36.2	14.4	40.0	60.8	-20.8	X/A
H	1735.634	54.7	25.3	6.2	36.2	0.0	50.0	80.8	-30.8	X/P
H	1735.634	54.7	25.3	6.2	36.2	14.4	35.6	60.8	-25.2	X/A
V	1735.634	59.3	25.1	6.2	36.2	0.0	54.4	80.8	-26.4	Y/P
V	1735.634	59.3	25.1	6.2	36.2	14.4	40.0	60.8	-20.8	Y/P
H	1735.634	54.7	25.3	6.2	36.2	0.0	50.0	80.8	-30.8	Y/P
H	1735.634	54.7	25.3	6.2	36.2	14.4	35.6	60.8	-25.2	Y/P
V	1735.634	53.0	25.1	6.2	36.2	0.0	48.1	80.8	-32.7	Z/P
V	1735.634	53.0	25.1	6.2	36.2	14.4	33.7	60.8	-27.1	Z/A
H	1735.634	60.4	25.3	6.2	36.2	0.0	55.6	80.8	-25.2	Z/P
H	1735.634	60.4	25.3	6.2	36.2	14.4	41.2	60.8	-19.6	Z/A
V	2169.542	48.4	27.2	8.7	35.8	0.0	48.5	80.8	-32.3	X/P
V	2169.542	48.4	27.2	8.7	35.8	14.4	34.1	60.8	-26.7	X/A
H	2169.542	46.6	27.4	8.7	35.8	0.0	46.9	80.8	-33.9	X/P
H	2169.542	46.6	27.4	8.7	35.8	14.4	32.5	60.8	-28.3	X/A
V	2169.542	48.4	27.2	8.7	35.8	0.0	48.5	80.8	-32.3	Y/P
V	2169.542	48.4	27.2	8.7	35.8	14.4	34.1	60.8	-26.7	Y/P
H	2169.542	46.6	27.4	8.7	35.8	0.0	46.9	80.8	-33.9	Y/P
H	2169.542	46.6	27.4	8.7	35.8	14.4	32.5	60.8	-28.3	Y/P
V	2169.542	46.7	27.2	8.7	35.8	0.0	46.8	80.8	-34.0	Z/P
V	2169.542	46.7	27.2	8.7	35.8	14.4	32.4	60.8	-28.4	Z/A
H	2169.542	53.4	27.4	8.7	35.8	0.0	53.7	80.8	-27.1	Z/P
H	2169.542	53.4	27.4	8.7	35.8	14.4	39.3	60.8	-21.5	Z/A
V	2603.458	46.0	28.2	8.7	35.7	0.0	47.3	80.8	-33.5	X/P
V	2603.458	46.0	28.2	8.7	35.7	14.4	32.9	60.8	-27.9	X/A
H	2603.458	49.6	28.4	8.7	35.7	0.0	51.1	80.8	-29.7	X/P
H	2603.458	49.6	28.4	8.7	35.7	14.4	36.7	60.8	-24.1	X/A
V	2603.458	46.0	28.2	8.7	35.7	0.0	47.2	80.8	-33.6	Y/P
V	2603.458	46.0	28.2	8.7	35.7	14.4	32.8	60.8	-28.0	Y/P
H	2603.458	49.6	28.4	8.7	35.7	0.0	51.0	80.8	-29.8	Y/P
H	2603.458	49.6	28.4	8.7	35.7	14.4	36.6	60.8	-24.2	Y/P
V	2603.458	48.6	28.2	8.7	35.7	0.0	49.8	80.8	-31.0	Z/P
V	2603.458	48.6	28.2	8.7	35.7	14.4	35.4	60.8	-25.4	Z/A
H	2603.458	53.7	28.4	8.7	35.7	0.0	55.1	80.8	-25.7	Z/P
H	2603.458	53.7	28.4	8.7	35.7	14.4	40.7	60.8	-20.1	Z/A
V	3037.375	44.8	29.9	10.9	35.7	0.0	49.9	80.8	-30.9	X/P
V	3037.375	44.8	29.9	10.9	35.7	14.4	35.5	60.8	-25.3	X/A
H	3037.375	44.5	30.0	10.9	35.7	0.0	49.8	80.8	-31.0	X/P
H	3037.375	44.5	30.0	10.9	35.7	14.4	35.4	60.8	-25.4	X/A
V	3037.375	44.8	29.9	10.9	35.7	0.0	49.9	80.8	-30.9	Y/P
V	3037.375	44.8	29.9	10.9	35.7	14.4	35.5	60.8	-25.3	Y/P
H	3037.375	44.5	30.0	10.9	35.7	0.0	49.7	80.8	-31.1	Y/P
H	3037.375	44.5	30.0	10.9	35.7	14.4	35.3	60.8	-25.5	Y/P
V	3037.375	44.0	29.9	10.9	35.7	0.0	49.1	80.8	-31.7	Z/P
V	3037.375	44.0	29.9	10.9	35.7	14.4	34.7	60.8	-26.1	Z/A
H	3037.375	46.9	30.0	10.9	35.7	0.0	52.1	80.8	-28.7	Z/P
H	3037.375	46.9	30.0	10.9	35.7	14.4	37.7	60.8	-23.1	Z/A
V	3905.194	43.5	31.0	10.9	35.6	0.0	49.8	80.8	-31.0	X/P
V	3905.194	43.5	31.0	10.9	35.6	14.4	35.4	60.8	-25.4	X/A
H	3905.194	44.2	31.2	10.9	35.6	0.0	50.8	80.8	-30.0	X/P
H	3905.194	44.2	31.2	10.9	35.6	14.4	36.4	60.8	-24.4	X/A
V	3905.194	43.5	31.0	10.9	35.6	0.0	49.8	80.8	-31.0	Y/P
V	3905.194	43.5	31.0	10.9	35.6	14.4	35.4	60.8	-25.4	Y/P

Tabular Data - 1000-5000MHz

9.0 Bandwidth Requirements (FCC 15C - 15.231(c))

Method:

The bandwidth of the emission shall be no wider than 0.25% of the center frequency for devices operating above 70 MHz and below 900 MHz. For devices operating above 900 MHz, the emission shall be no wider than 0.5% of the center frequency. Bandwidth is determined at the points 20 dB down from the modulated carrier.


- Center Frequency is set to the fundamental of transmitter.
- Resolution Bandwidth is set to approximately 1% of the emission bandwidth.
- Video Bandwidth is set greater than or equal to the Resolution Bandwidth.

Test Equipment Used:

Description:	Manufacturer:	Model:	Asset Number:	Cal Date:	Cal Due:
Cable E05 (Formerly HS 1500 N-N)	Huber-Suhner	Sucoflex 104PEA	E05	05/11/2006	05/11/2007
Spectrum Analyzer, 20 Hz to 40 GHz	Rohde & Schwarz	FSEK30	200062	01/12/2006	01/12/2007

Results: The sample tested was found to Comply.

Plot:

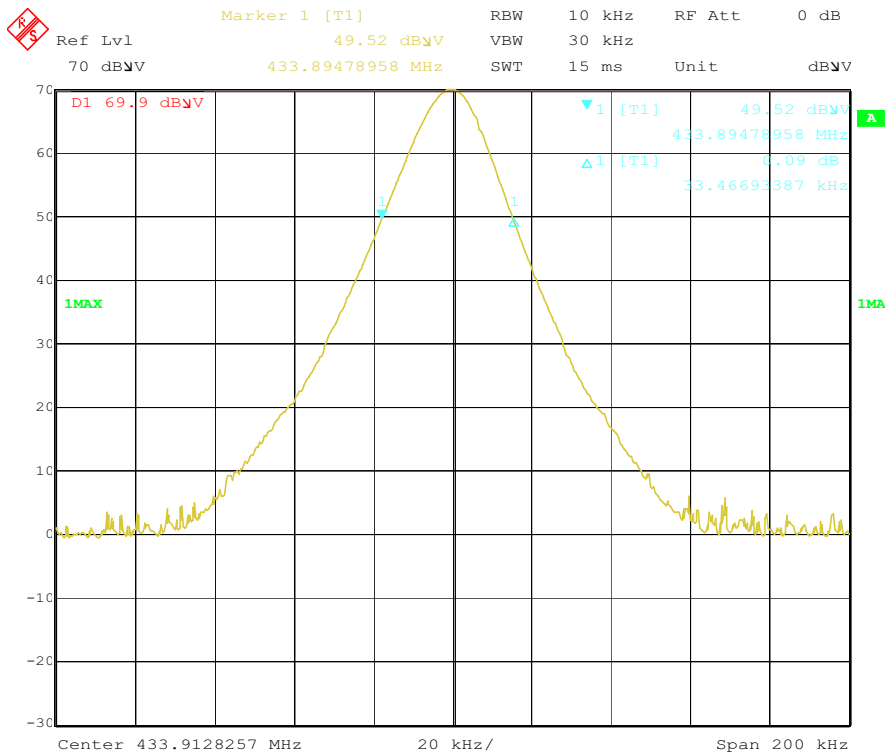

Date: 19.DEC.2006 22:00:17

Occupied Bandwidth

9.0 Bandwidth Requirements (FCC 15C - 15.231(c))**Data:**

Fundamental Frequency MHz	Measured Bandwidth MHz	Bandwidth Limit MHz
433	0.02346	1.0825

Suggested Instrument Settings	
RBW (kHz):	10
VBW (kHz):	30
Span (MHz):	1.080
Sweep time (s):	>1