

System Check_Head_835MHz

DUT: D835V2-SN:4d162

Communication System: ; Frequency: 835.0

Medium: HSL. Medium parameters used: $f = 835.0$ MHz; $\sigma = 0.930$ S/m; $\epsilon_r = 40.9$

Ambient Temperature: 23.2°C; Liquid Temperature: 22.7°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7706; ConvF(10.57,10.57, 10.57); Calibrated: 2022-01-20
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1649; Calibrated: 2022-03-30
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2074; Section: Flat
- Measurement Software: cDASY6 V6.6.0.13926


Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 15.0 mm x 15.0 mm

SAR (1g) = 0.486 W/kg; SAR (10g) = 0.311 W/kg;

Zoom Scan (32.0 mm x 32.0 mm x 30.0 mm): Measurement Grid: 8.0 mm x 8.0 mm x 5.0 mm

Power Drift = 0.02 dB

SAR (1g) = 0.502 W/kg; SAR (10g) = 0.328 W/kg;

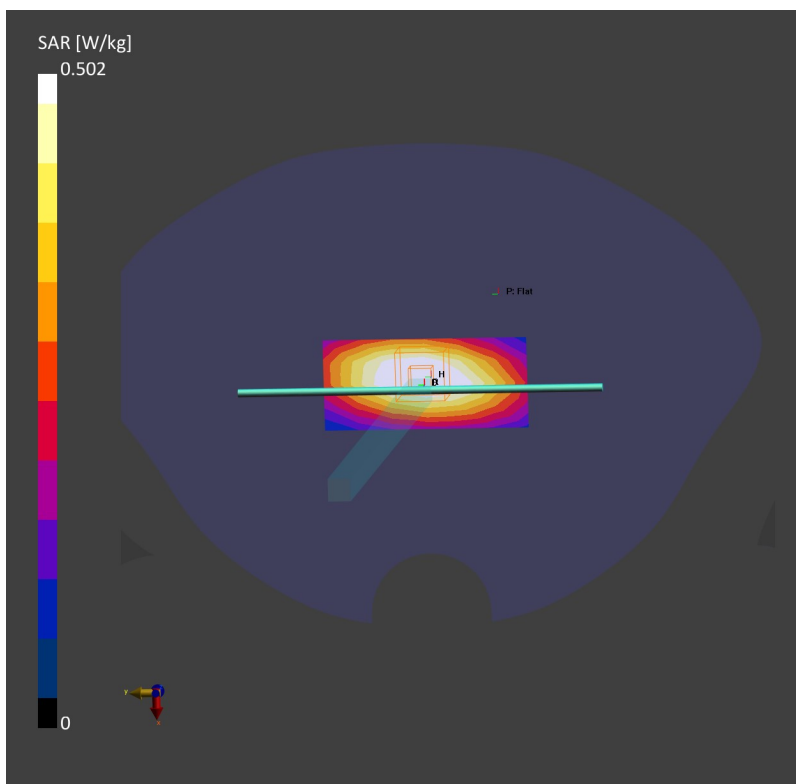

System Check_Head_1900MHz

DUT: D1900V2-SN:5d182

Communication System: ; Frequency: 1900.0

Medium: HSL. Medium parameters used: $f = 1900.0$ MHz; $\sigma = 1.40$ S/m; $\epsilon_r = 41.4$

Ambient Temperature: 23.2°C; Liquid Temperature: 22.6°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7706; ConvF(8.8, 8.8, 8.8); Calibrated: 2022-01-20
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1649; Calibrated: 2022-03-30
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2074; Section: Flat
- Measurement Software: cDASY6 V6.6.0.13926


Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 15.0 mm x 15.0 mm

SAR (1g) = 1.89 W/kg; SAR (10g) = 0.941 W/kg;

Zoom Scan (32.0 mm x 32.0 mm x 30.0 mm): Measurement Grid: 8.0 mm x 8.0 mm x 5.0 mm

Power Drift = 0.03 dB

SAR (1g) = 1.93 W/kg; SAR (10g) = 0.980 W/kg;

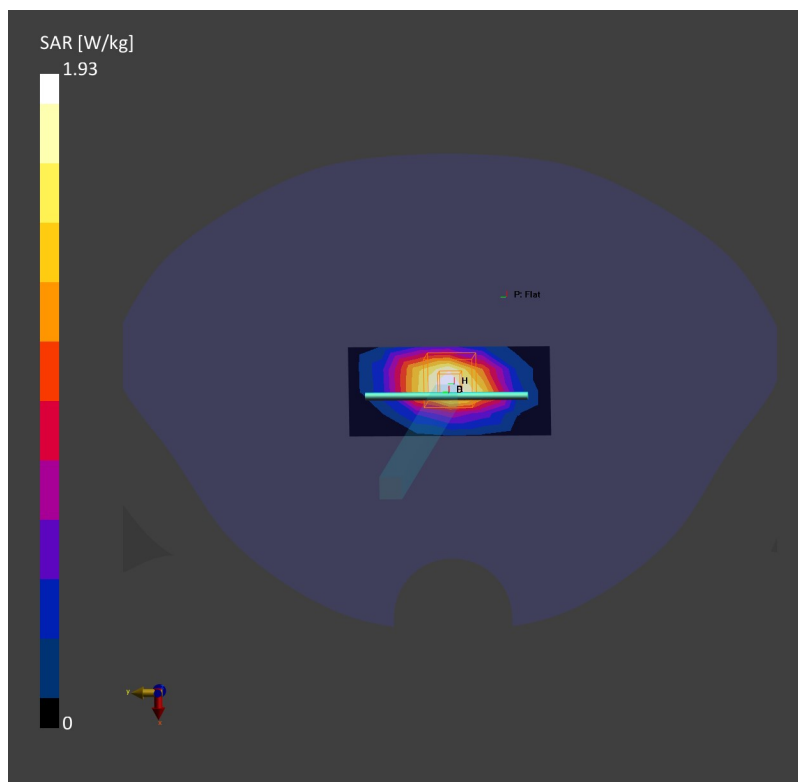

System Check_Head_2450MHz

DUT: D2450V2-SN:924

Communication System: ; Frequency: 2450.0

Medium: HSL. Medium parameters used: $f = 2450.0$ MHz; $\sigma = 1.81$ S/m; $\epsilon_r = 38.6$

Ambient Temperature: 23.4°C; Liquid Temperature: 22.9°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7706; ConvF(8.29, 8.29, 8.29); Calibrated: 2022-01-20
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1649; Calibrated: 2022-03-30
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2074; Section: Flat
- Measurement Software: cDASY6 V6.6.0.13926


Area Scan (40.0 mm x 96.0 mm): Measurement Grid: 12.0 mm x 12.0 mm

SAR (1g) = 2.36 W/kg; SAR (10g) = 1.14 W/kg;

Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm): Measurement Grid: 5.0 mm x 5.0 mm x 5.0 mm

Power Drift = -0.01 dB

SAR (1g) = 2.44 W/kg; SAR (10g) = 1.15 W/kg;

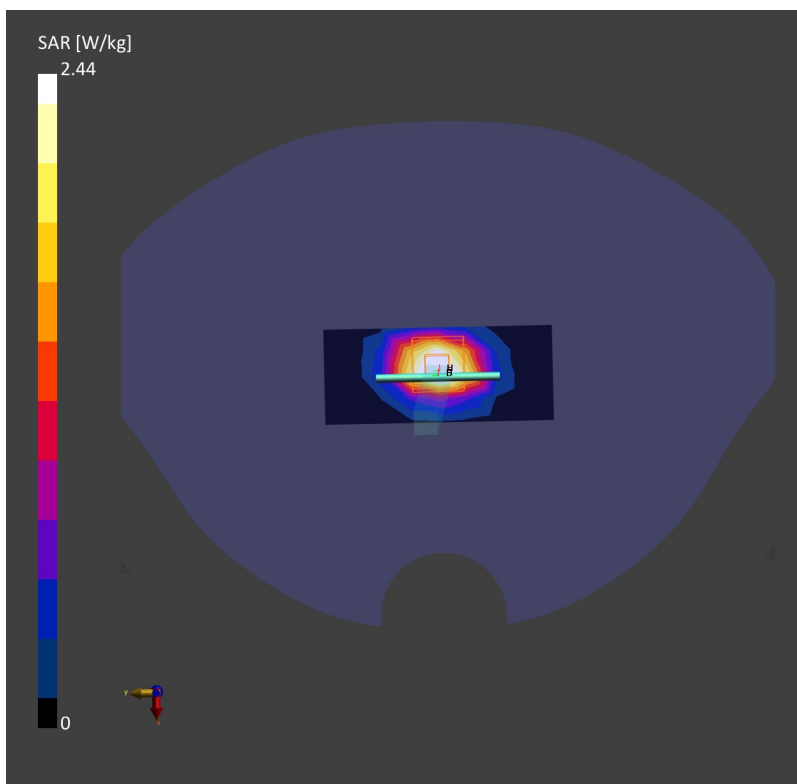

System Check_Head_2600MHz

DUT: D2600V2-SN:1061

Communication System: ; Frequency: 2600.0

Medium: HSL. Medium parameters used: $f = 2600.0$ MHz; $\sigma = 1.92$ S/m; $\epsilon_r = 38.3$

Ambient Temperature: 23.1°C; Liquid Temperature: 22.8°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7706; ConvF(8.02, 8.02, 8.02); Calibrated: 2022-01-20
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1649; Calibrated: 2022-03-30
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2074; Section: Flat
- Measurement Software: cDASY6 V6.6.0.13926


Area Scan (40.0 mm x 96.0 mm): Measurement Grid: 12.0 mm x 12.0 mm

SAR (1g) = 2.55 W/kg; SAR (10g) = 1.21 W/kg;

Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm): Measurement Grid: 5.0 mm x 5.0 mm x 5.0 mm

Power Drift = -0.05 dB

SAR (1g) = 2.72 W/kg; SAR (10g) = 1.26 W/kg;

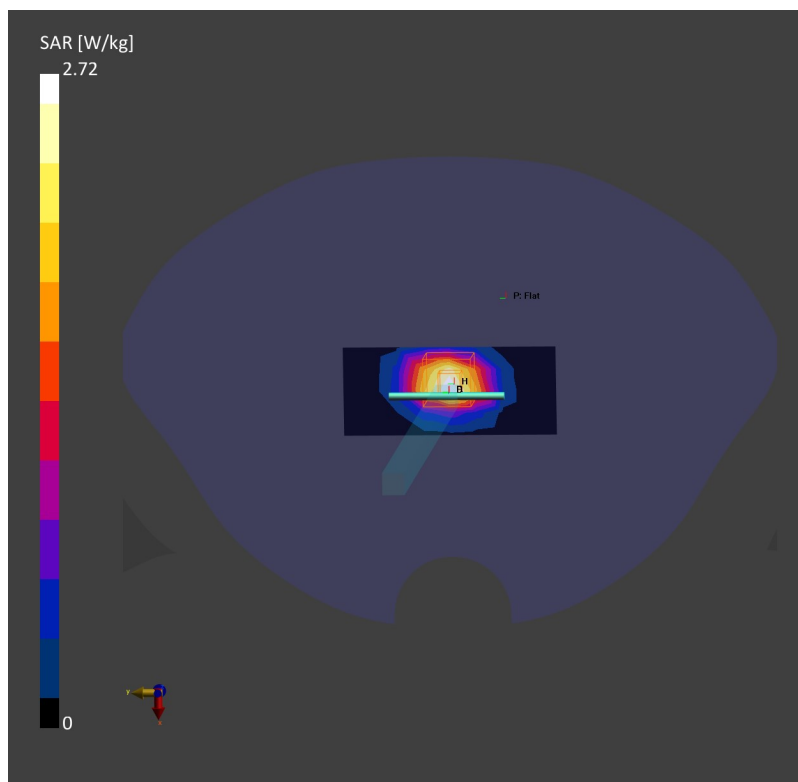

System Check_Head_5250MHz

DUT: D5GHzV2-SN:1113

Communication System: ; Frequency: 5250.0

Medium: HSL. Medium parameters used: $f = 5250.0$ MHz; $\sigma = 4.60$ S/m; $\epsilon_r = 35.9$

Ambient Temperature: 23.1°C; Liquid Temperature: 22.7°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7706; ConvF(6.07, 6.07, 6.07); Calibrated: 2022-01-20
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1649; Calibrated: 2022-03-30
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2074; Section: Flat
- Measurement Software: cDASY6 V6.6.0.13926


Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 3.68 W/kg; SAR (10g) = 1.01 W/kg;

Zoom Scan (24.0 mm x 24.0 mm x 22.0 mm): Measurement Grid: 4.0 mm x 4.0 mm x 1.4 mm

Power Drift = 0.11 dB

SAR (1g) = 3.81 W/kg; SAR (10g) = 1.12 W/kg;

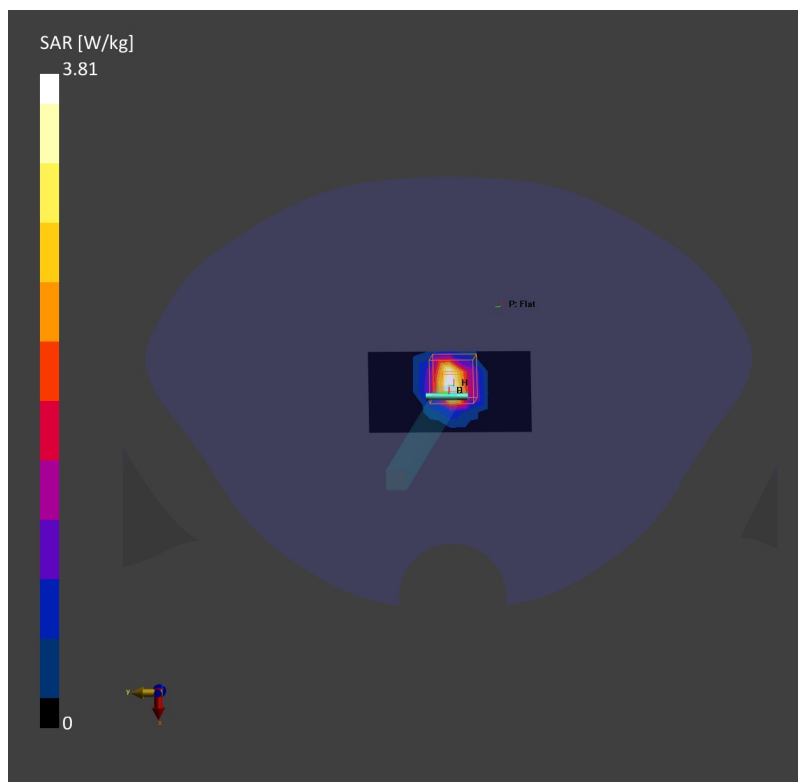

System Check_Head_5600MHz

DUT: D5GHzV2-SN:1113

Communication System: ; Frequency: 5600.0

Medium: HSL. Medium parameters used: $f = 5600.0$ MHz; $\sigma = 4.99$ S/m; $\epsilon_r = 35.4$

Ambient Temperature: 23.3°C; Liquid Temperature: 22.8°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7706; ConvF(5.3, 5.3, 5.3); Calibrated: 2022-01-20
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1649; Calibrated: 2022-03-30
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2074; Section: Flat
- Measurement Software: cDASY6 V6.6.0.13926


Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 3.62 W/kg; SAR (10g) = 1.05 W/kg;

Zoom Scan (24.0 mm x 24.0 mm x 22.0 mm): Measurement Grid: 4.0 mm x 4.0 mm x 1.4 mm

Power Drift = -0.05 dB

SAR (1g) = 3.91 W/kg; SAR (10g) = 1.13 W/kg;

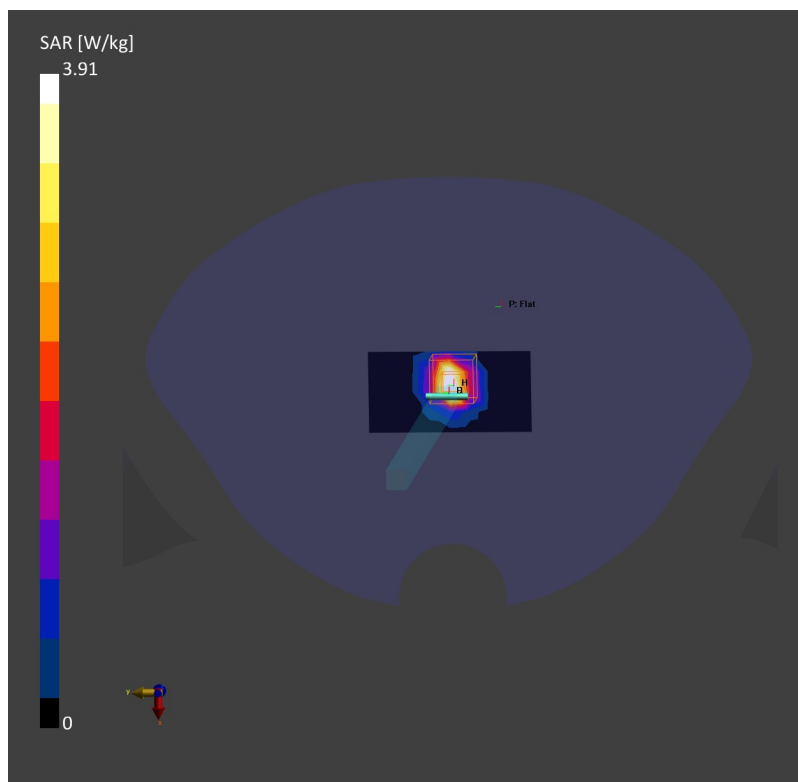

System Check_Head_5750MHz

DUT: D5GHzV2-SN:1113

Communication System: ; Frequency: 5750.0

Medium: HSL. Medium parameters used: $f = 5750.0$ MHz; $\sigma = 5.16$ S/m; $\epsilon_r = 35.2$

Ambient Temperature: 23.4°C; Liquid Temperature: 22.6°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7706; ConvF(5.49, 5.49, 5.49); Calibrated: 2022-01-20
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1649; Calibrated: 2022-03-30
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2074; Section: Flat
- Measurement Software: cDASY6 V6.6.0.13926

Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 3.76 W/kg; SAR (10g) = 0.978 W/kg;

Zoom Scan (24.0 mm x 24.0 mm x 22.0 mm): Measurement Grid: 4.0 mm x 4.0 mm x 1.4 mm

Power Drift = 0.08 dB

SAR (1g) = 3.95 W/kg; SAR (10g) = 1.10 W/kg;

