

Date: 2025/2/23

## System Check\_1750MHz

### D1750V2-SN:1137

Communication System: CW; Frequency: 1750.0 MHz; Duty Cycle: 1:1  
Medium: HSL Medium parameters used:  $f=1750.0$  MHz;  $\sigma=1.34$  S/m;  $\epsilon_r=41.9$   
Ambient Temperature: 23.6°C; Liquid Temperature: 22.5°C

#### DASY6 Configuration:

- Probe: EX3DV4 - SN3819; ConvF(7.94, 7.08, 7.5); Calibrated: 2024/8/22
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1386; Calibrated: 2024/8/30
- Phantom: Twin-SAM V5.0 (30deg probe tilt); Serial: 1670; Section: Flat
- Measurement Software: cDASY6 V16.0.0.116
- UID: CW, 0--

**Area Scan (40.0 mm x 120.0 mm):** Measurement Grid: 5.0 mm x 15.0 mm SAR (1g)  
= 8.85 W/kg; SAR (10g) = 4.80 W/kg;


**Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm):** Measurement Grid: 6.0 mm x 6.0mm x 1.5 mm

Power Drift = 0.01 dB

SAR (1g) = 8.76 W/kg; SAR (10g) = 4.71 W/kg

Smallest distance from peaks to all points 3 dB below = 9.9 mm

Ratio of SAR at M2 to SAR at M1 = 83.1 %

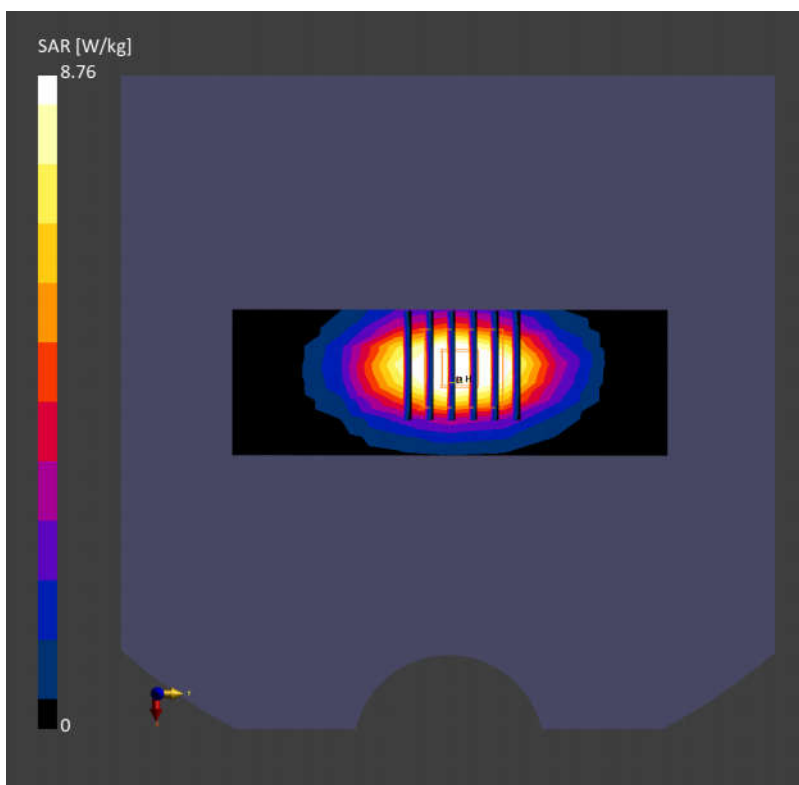

Date: 2025/2/23

## System Check\_1900MHz

### D1900V2-SN:5d118

Communication System: CW; Frequency: 1900.0 MHz; Duty Cycle: 1:1  
Medium: HSL Medium parameters used:  $f=1900.0$  MHz;  $\sigma=1.44$  S/m;  $\epsilon_r=41.7$   
Ambient Temperature: 23.2°C; Liquid Temperature: 22.3°C

#### DASY6 Configuration:

- Probe: EX3DV4 - SN3819; ConvF(7.95, 7.09, 7.51); Calibrated: 2024/8/22
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1386; Calibrated: 2024/8/30
- Phantom: Twin-SAM V5.0 (30deg probe tilt); Serial: 1670; Section: Flat
- Measurement Software: cDASY6 V16.0.0.116
- UID: CW, 0--

**Area Scan (40.0 mm x 120.0 mm):** Measurement Grid: 5.0 mm x 15.0 mm SAR (1g)  
= 9.93 W/kg; SAR (10g) = 5.22 W/kg;


**Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm):** Measurement Grid: 6.0 mm x 6.0mm x 1.5 mm

Power Drift = -0.01 dB

SAR (1g) = 9.83 W/kg; SAR (10g) = 5.11 W/kg

Smallest distance from peaks to all points 3 dB below = 9.7 mm

Ratio of SAR at M2 to SAR at M1 = 82.2 %

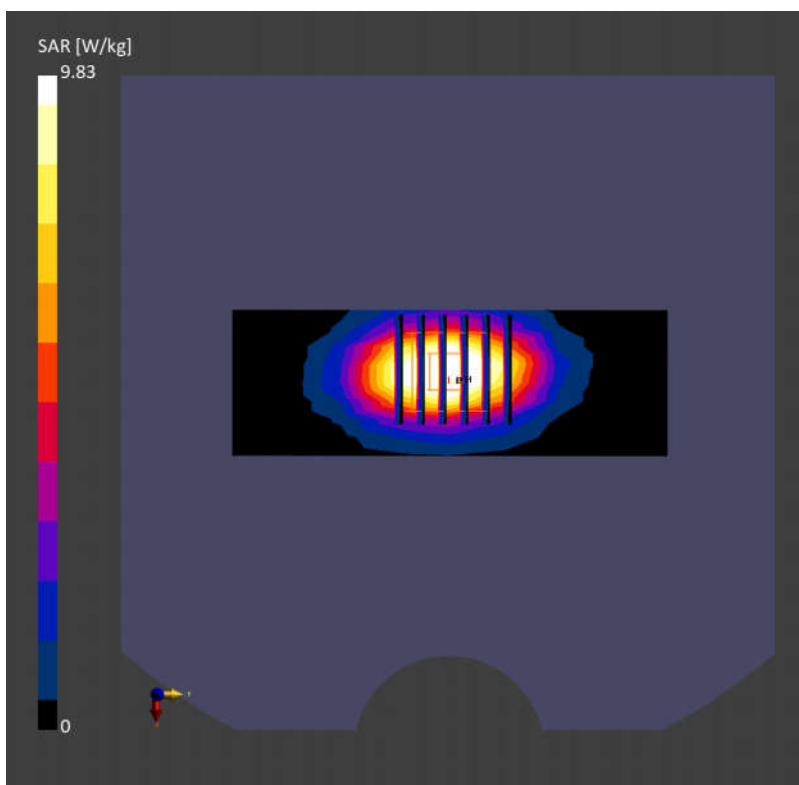

Date: 2025/2/23

## System Check\_2600MHz

### D2600V2-SN:1008

Communication System: CW; Frequency: 2600.0 MHz; Duty Cycle: 1:1  
Medium: HSL Medium parameters used:  $f = 2600.0$  MHz;  $\sigma = 1.94$  S/m;  $\epsilon_r = 40.7$   
Ambient Temperature: 23.3°C; Liquid Temperature: 22.4°C

#### DASY6 Configuration:

- Probe: EX3DV4 - SN3819; ConvF(7.68, 6.85, 7.26); Calibrated: 2024/8/22
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1386; Calibrated: 2024/8/30
- Phantom: Twin-SAM V5.0 (30deg probe tilt); Serial: 1670; Section: Flat
- Measurement Software: cDASY6 V16.0.0.116
- UID: CW, 0--

**Area Scan (40.0 mm x 80.0 mm):** Measurement Grid: 5.0 mm x 10.0 mm SAR (1g)  
= 13.5 W/kg; SAR (10g) = 6.16 W/kg;


**Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm):** Measurement Grid: 5.0 mm x 5.0mm x 1.5 mm

Power Drift = -0.00 dB

SAR (1g) = 13.1 W/kg; SAR (10g) = 6.30 W/kg

Smallest distance from peaks to all points 3 dB below = 9.0 mm

Ratio of SAR at M2 to SAR at M1 = 77.5 %

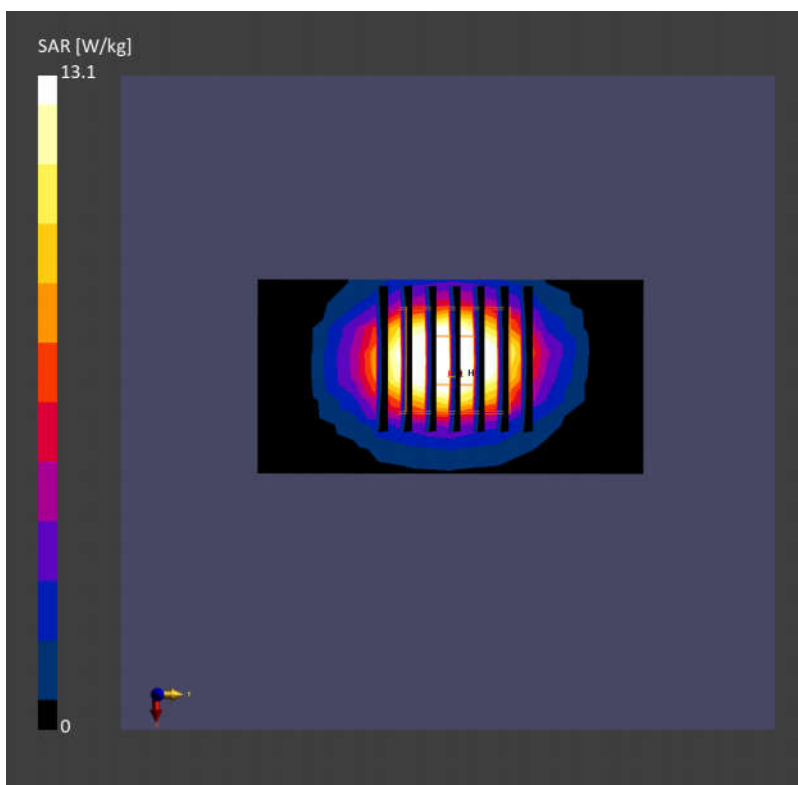

Date: 2025/2/23

**System Check\_3700MHz****D3700V2-SN:1037**

Communication System: CW; Frequency: 3700.0 MHz; Duty Cycle: 1:1  
Medium: HSL Medium parameters used:  $f = 3700.0$  MHz;  $\sigma = 3.10$  S/m;  $\epsilon_r = 38.9$   
Ambient Temperature: 23.5°C; Liquid Temperature: 22.6°C

## DASY6 Configuration:

- Probe: EX3DV4 - SN3819; ConvF(6.92, 6.17, 6.53); Calibrated: 2024/8/22
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1386; Calibrated: 2024/8/30
- Phantom: Twin-SAM V5.0 (30deg probe tilt); Serial: 1670; Section: Flat
- Measurement Software: cDASY6 V16.0.0.116
- UID: CW, 0--

**Area Scan (40.0 mm x 80.0 mm):** Measurement Grid: 5.0 mm x 10.0 mm SAR (1g)  
= 6.69 W/kg; SAR (10g) = 2.52 W/kg;

**Zoom Scan (28.0 mm x 28.0 mm x 28.0 mm):** Measurement Grid: 5.0 mm x 5.0mm x 1.4 mm

Power Drift = 0.00 dB

SAR (1g) = 6.71 W/kg; SAR (10g) = 2.45 W/kg

Smallest distance from peaks to all points 3 dB below = 8.0 mm

Ratio of SAR at M2 to SAR at M1 = 74.8 %

