

Date: 2025-01-07

System Check_Head_750MHz**DUT: D750V3 - SN1087**

Communication System: CW; Frequency: 750.000 MHz; Duty Cycle: 1:1

Medium: Head Simulating Liquid Medium parameters used: $f = 750.000$ MHz; $\sigma = 0.889$ S/m; $\epsilon_r = 42.3$

Ambient Temperature: 23.3°C; Liquid Temperature: 22.6°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7774; ConvF(8.12, 8.81, 8.04); Calibrated: 2024-06-27
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1358; Calibrated: 2024-05-23
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2022; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=50mW/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 0.405 W/kg; SAR (10g) = 0.274 W/kg;


Pin=50mW/Zoom Scan (32.0 mm x 32.0 mm x 30.0 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm

Power Drift = 0.01 dB

SAR (1g) = 0.418 W/kg; SAR (10g) = 0.285 W/kg

Smallest distance from peaks to all points 3 dB below = 16.1 mm

Ratio of SAR at M2 to SAR at M1 = 88.2 %

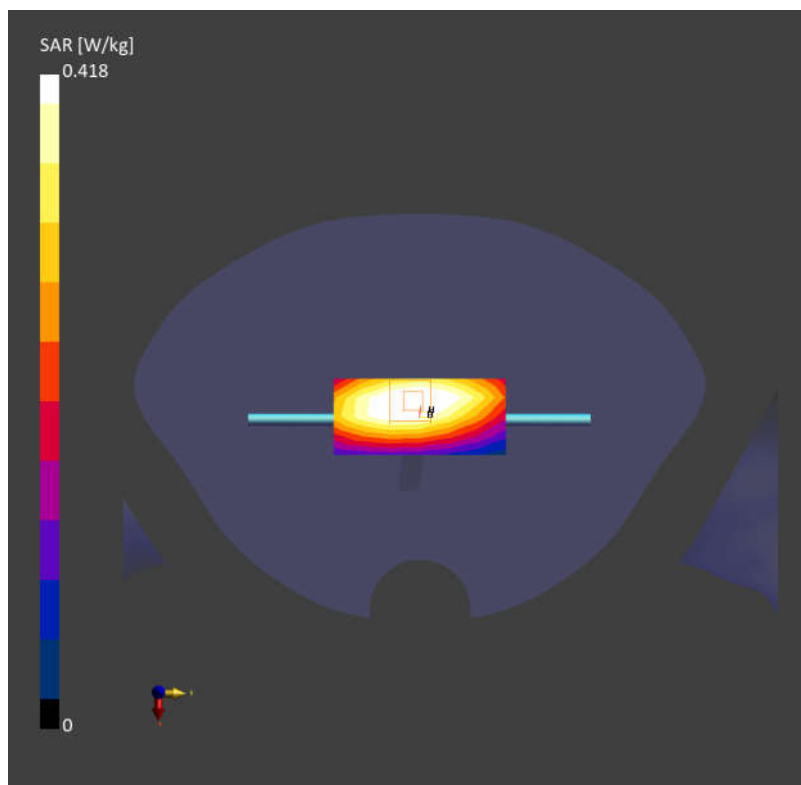

Date: 2025-01-09

System Check_Head_2600MHz**DUT: D2600V2 - SN1112**

Communication System: CW; Frequency: 2600.000 MHz; Duty Cycle: 1:1

Medium: Head Simulating Liquid Medium parameters used: $f = 2600.000$ MHz; $\sigma = 1.89$ S/m; $\epsilon_r = 39.2$

Ambient Temperature: 23.3°C; Liquid Temperature: 22.8°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7774; ConvF(6.16, 6.71, 6.3); Calibrated: 2024-06-27
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1358; Calibrated: 2024-05-23
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2022; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=50mW/Area Scan (40.0 mm x 96.0 mm): Measurement Grid: 10.0 mm x 12.0 mm

SAR (1g) = 2.33 W/kg; SAR (10g) = 1.10 W/kg;


Pin=50mW/Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.5 mm

Power Drift = -0.01 dB

SAR (1g) = 2.61 W/kg; SAR (10g) = 1.22 W/kg

Smallest distance from peaks to all points 3 dB below = 9.0 mm

Ratio of SAR at M2 to SAR at M1 = 82.4 %

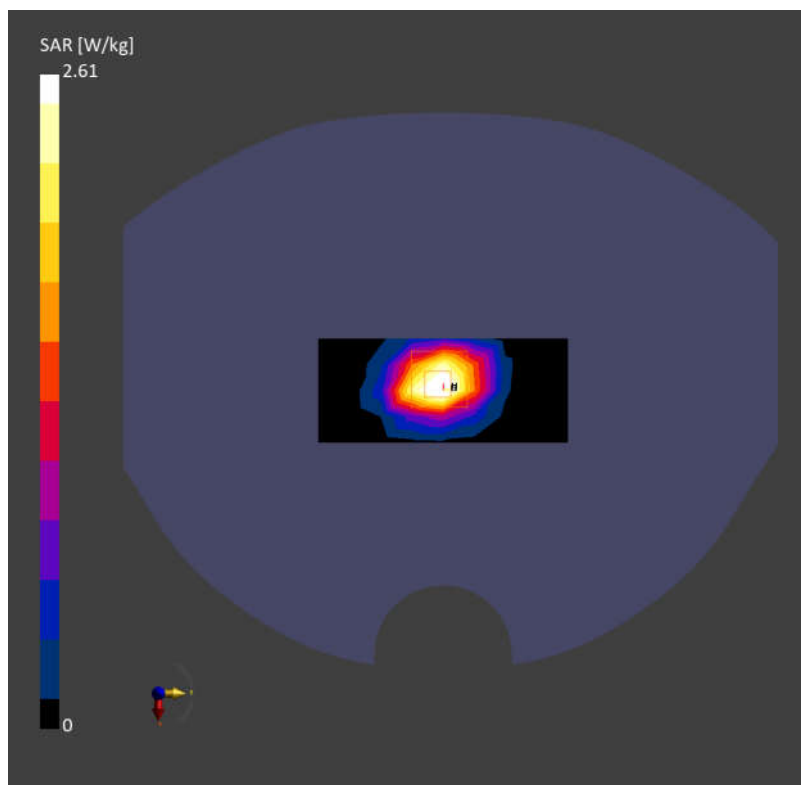

Date: 2025-01-11

System Check_Head_3900MHz**DUT: D3900V2 - SN1048**

Communication System: CW; Frequency: 3900.000 MHz; Duty Cycle: 1:1

Medium: Head Simulating Liquid Medium parameters used: $f = 3900.000$ MHz; $\sigma = 3.21$ S/m; $\epsilon_r = 38.0$

Ambient Temperature: 23.2°C; Liquid Temperature: 22.8°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7774; ConvF(5.5, 6.03, 5.62); Calibrated: 2024-06-27
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1358; Calibrated: 2024-05-23
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2022; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=50mW/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 3.37 W/kg; SAR (10g) = 1.20 W/kg;


Pin=50mW/Zoom Scan (24.0 mm x 24.0 mm x 22.0 mm): Measurement Grid: 4.0 mm x 4.0mm x 1.4 mm

Power Drift = 0.01 dB

SAR (1g) = 3.46 W/kg; SAR (10g) = 1.27 W/kg

Smallest distance from peaks to all points 3 dB below = 8.1 mm

Ratio of SAR at M2 to SAR at M1 = 75.8 %

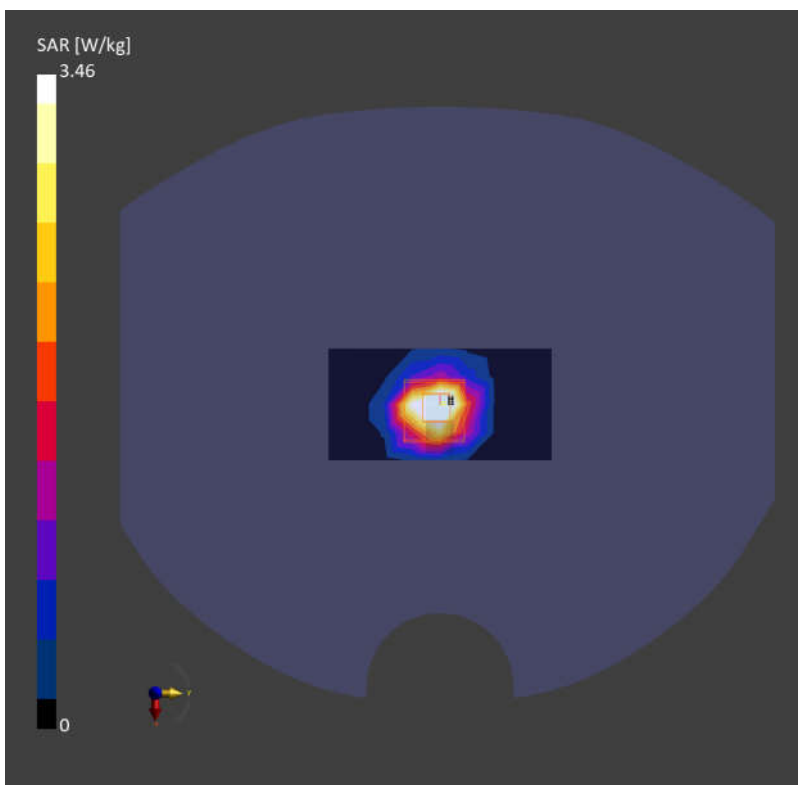

Date: 2025-01-13

System Check_Head_750MHz**DUT: D750V3 - SN1087**

Communication System: CW; Frequency: 750.000 MHz; Duty Cycle: 1:1

Medium: Head Simulating Liquid Medium parameters used: $f = 750.000$ MHz; $\sigma = 0.925$ S/m; $\epsilon_r = 42.4$

Ambient Temperature: 23.3°C; Liquid Temperature: 22.9°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7774; ConvF(8.12, 8.81, 8.04); Calibrated: 2024-06-27
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1358; Calibrated: 2024-05-23
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2022; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=50mW/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 0.422 W/kg; SAR (10g) = 0.286 W/kg;


Pin=50mW/Zoom Scan (32.0 mm x 32.0 mm x 30.0 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm

Power Drift = 0.01 dB

SAR (1g) = 0.436 W/kg; SAR (10g) = 0.298 W/kg

Smallest distance from peaks to all points 3 dB below = 16.8 mm

Ratio of SAR at M2 to SAR at M1 = 87.9 %

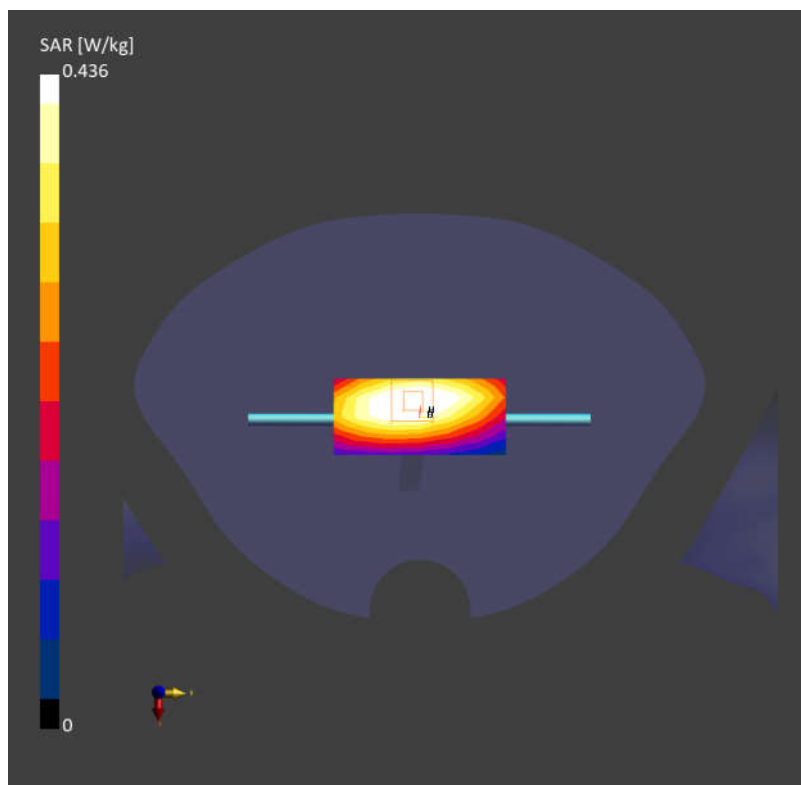

Date: 2025-01-15

System Check_Head_2600MHz**DUT: D2600V2 - SN1112**

Communication System: CW; Frequency: 2600.000 MHz; Duty Cycle: 1:1

Medium: Head Simulating Liquid Medium parameters used: $f = 2600.000$ MHz; $\sigma = 1.93$ S/m; $\epsilon_r = 39.0$

Ambient Temperature: 23.3°C; Liquid Temperature: 22.7°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7774; ConvF(6.16, 6.71, 6.3); Calibrated: 2024-06-27
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1358; Calibrated: 2024-05-23
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2022; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=50mW/Area Scan (40.0 mm x 96.0 mm): Measurement Grid: 10.0 mm x 12.0 mm

SAR (1g) = 2.42 W/kg; SAR (10g) = 1.14 W/kg;


Pin=50mW/Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.5 mm

Power Drift = -0.01 dB

SAR (1g) = 2.70 W/kg; SAR (10g) = 1.26 W/kg

Smallest distance from peaks to all points 3 dB below = 9.0 mm

Ratio of SAR at M2 to SAR at M1 = 82.2 %

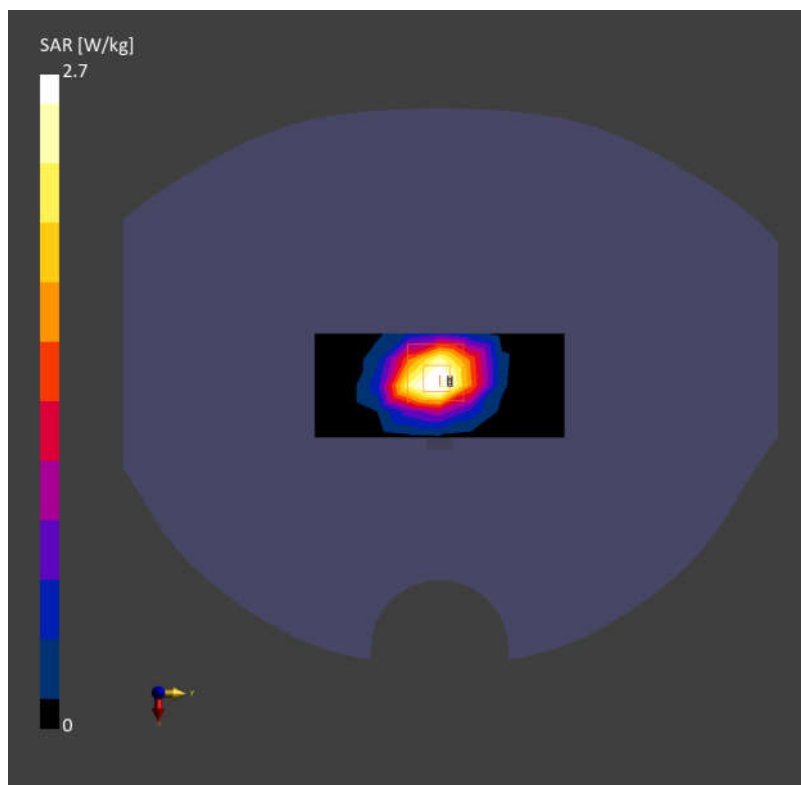

Date: 2025-01-17

System Check_Head_3900MHz**DUT: D3900V2 - SN1048**

Communication System: CW; Frequency: 3900.000 MHz; Duty Cycle: 1:1

Medium: Head Simulating Liquid Medium parameters used: $f = 3900.000$ MHz; $\sigma = 3.18$ S/m; $\epsilon_r = 38.4$

Ambient Temperature: 23.2°C; Liquid Temperature: 22.8°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7774; ConvF(5.5, 6.03, 5.62); Calibrated: 2024-06-27
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1358; Calibrated: 2024-05-23
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2022; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=50mW/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 3.32 W/kg; SAR (10g) = 1.19 W/kg;


Pin=50mW/Zoom Scan (24.0 mm x 24.0 mm x 22.0 mm): Measurement Grid: 4.0 mm x 4.0mm x 1.4 mm

Power Drift = 0.01 dB

SAR (1g) = 3.35 W/kg; SAR (10g) = 1.23 W/kg

Smallest distance from peaks to all points 3 dB below = 8.1 mm

Ratio of SAR at M2 to SAR at M1 = 76.1 %

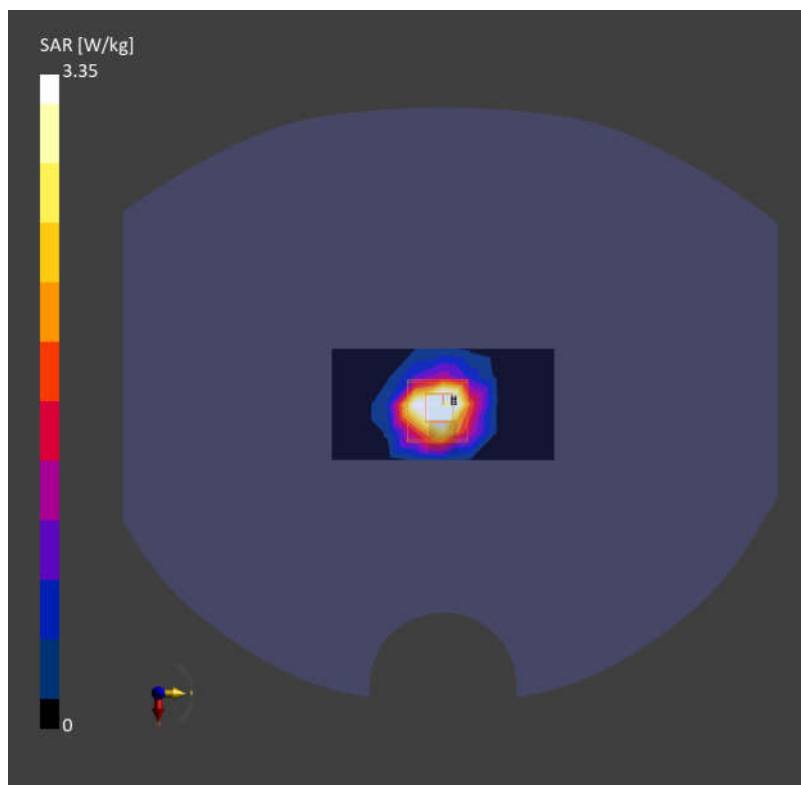

Date: 2025-01-19

System Check_Head_835MHz**DUT: D835V2 - SN4d298**

Communication System: CW; Frequency: 835.000 MHz; Duty Cycle: 1:1

Medium: Head Simulating Liquid Medium parameters used: $f = 835.000$ MHz; $\sigma = 0.918$ S/m; $\epsilon_r = 41.5$

Ambient Temperature: 23.1°C; Liquid Temperature: 22.7°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7774; ConvF(7.76, 8.53, 7.85); Calibrated: 2024-06-27
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1358; Calibrated: 2024-05-23
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2022; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=50mW/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 0.454 W/kg; SAR (10g) = 0.303 W/kg;


Pin=50mW/Zoom Scan (32.0 mm x 32.0 mm x 30.0 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm

Power Drift = -0.01 dB

SAR (1g) = 0.463 W/kg; SAR (10g) = 0.317 W/kg

Smallest distance from peaks to all points 3 dB below = 16.1 mm

Ratio of SAR at M2 to SAR at M1 = 89.3 %

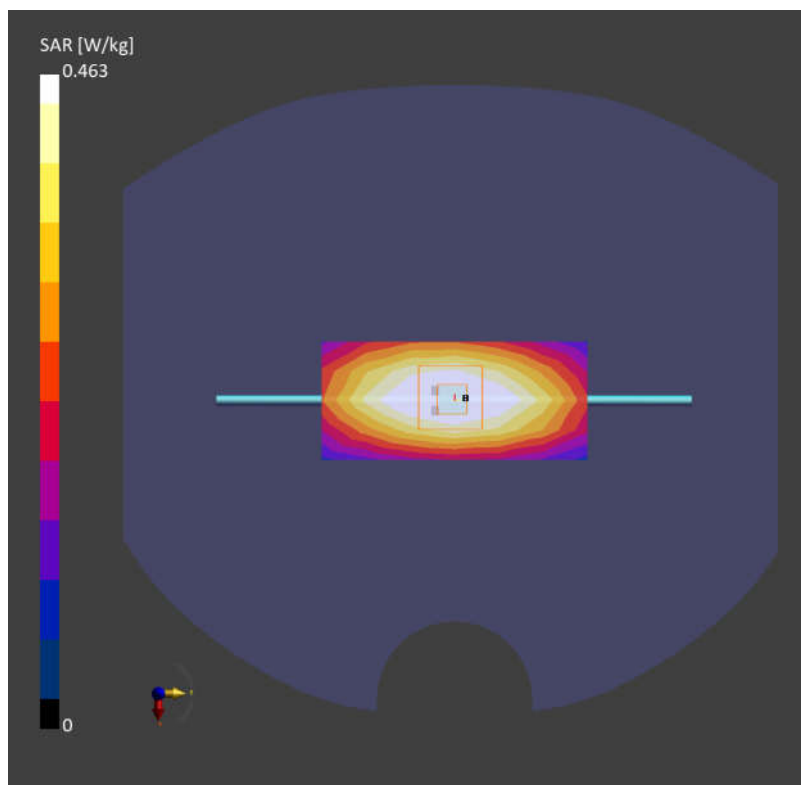

Date: 2025-01-20

SystemCheck_Head_1900MHz**DUT: D1900V2 - SN5d118**

Communication System: CW; Frequency: 1900.000 MHz; Duty Cycle: 1:1

Medium: Head Simulating Liquid Medium parameters used: $f = 1900.000$ MHz; $\sigma = 1.45$ S/m; $\epsilon_r = 39.9$

Ambient Temperature: 23.2°C; Liquid Temperature: 22.8°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7774; ConvF(6.48, 7.12, 6.7); Calibrated: 2024-06-27
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1358; Calibrated: 2024-05-23
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2022; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=50mW/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 1.76 W/kg; SAR (10g) = 0.928 W/kg;


Pin=50mW/Zoom Scan (32.0 mm x 32.0 mm x 30.0 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm

Power Drift = 0.07 dB

SAR (1g) = 1.92 W/kg; SAR (10g) = 0.977 W/kg

Smallest distance from peaks to all points 3 dB below = 9.6 mm

Ratio of SAR at M2 to SAR at M1 = 78.7 %

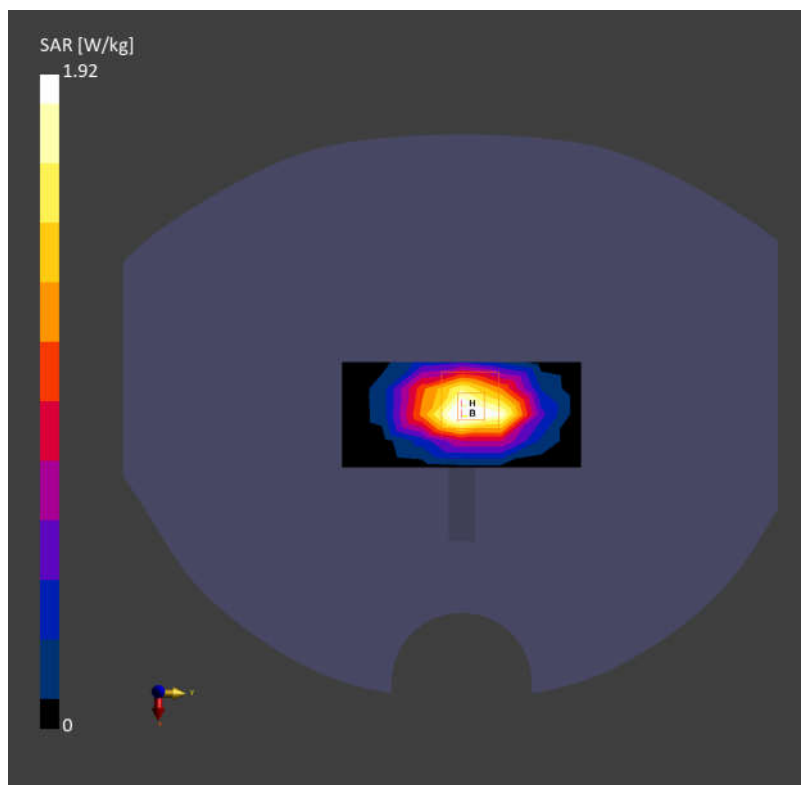

Date: 2025-01-21

System Check_Head_3500MHz**DUT: D3500V2 - SN1037**

Communication System: CW; Frequency: 3500.000 MHz; Duty Cycle: 1:1

Medium: Head Simulating Liquid Medium parameters used: $f = 3500.000$ MHz; $\sigma = 2.87$ S/m; $\epsilon_r = 38.5$

Ambient Temperature: 23.1°C; Liquid Temperature: 22.6°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7774; ConvF(5.49, 6.05, 5.64); Calibrated: 2024-06-27
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1358; Calibrated: 2024-05-23
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2022; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=50mW/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 3.08 W/kg; SAR (10g) = 1.20 W/kg;


Pin=50mW/Zoom Scan (24.0 mm x 24.0 mm x 22.0 mm): Measurement Grid: 4.0 mm x 4.0mm x 1.4 mm

Power Drift = -0.00 dB

SAR (1g) = 3.32 W/kg; SAR (10g) = 1.33 W/kg

Smallest distance from peaks to all points 3 dB below = 8.1 mm

Ratio of SAR at M2 to SAR at M1 = 79.0 %

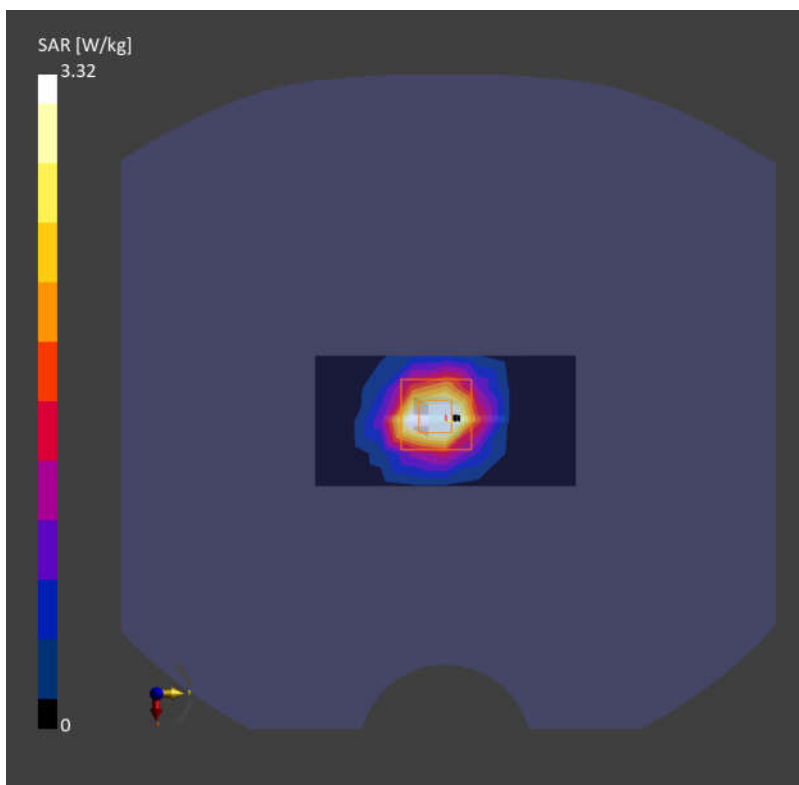

Date: 2025-01-22

System Check_Head_2450MHz**DUT: D2450V2 - SN1095**

Communication System: CW; Frequency: 2450.000 MHz; Duty Cycle: 1:1

Medium: Head Simulating Liquid Medium parameters used: $f = 2450.000$ MHz; $\sigma = 1.75$ S/m; $\epsilon_r = 39.5$

Ambient Temperature: 23.2°C; Liquid Temperature: 22.8°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7774; ConvF(6.08, 6.63, 6.23); Calibrated: 2024-06-27
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1358; Calibrated: 2024-05-23
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2022; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=50mW/Area Scan (40.0 mm x 96.0 mm): Measurement Grid: 10.0 mm x 12.0 mm

SAR (1g) = 2.83 W/kg; SAR (10g) = 1.34 W/kg;


Pin=50mW/Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.5 mm

Power Drift = 0.00 dB

SAR (1g) = 2.72 W/kg; SAR (10g) = 1.27 W/kg

Smallest distance from peaks to all points 3 dB below = 9.0 mm

Ratio of SAR at M2 to SAR at M1 = 83.6 %

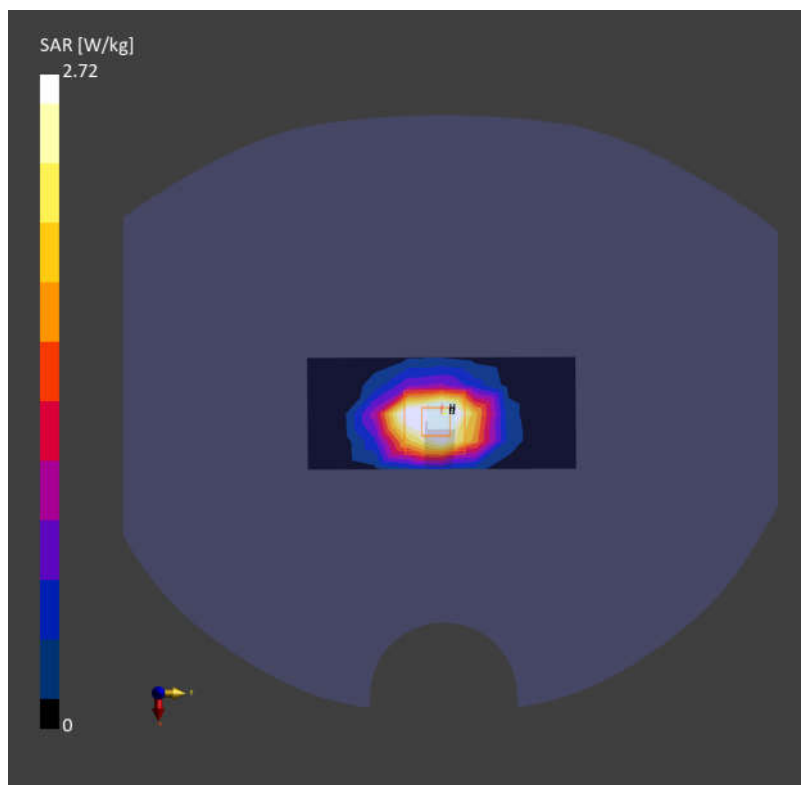

Date: 2025-01-23

System Check_Head_5250MHz**DUT: D5GHzV2 - SN1113**

Communication System: CW; Frequency: 5250.000 MHz; Duty Cycle: 1:1

Medium: Head Simulating Liquid Medium parameters used: $f = 5250.000$ MHz; $\sigma = 4.56$ S/m; $\epsilon_r = 35.0$

Ambient Temperature: 23.2°C; Liquid Temperature: 22.8°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7774; ConvF(4.32, 4.72, 4.38); Calibrated: 2024-06-27
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1358; Calibrated: 2024-05-23
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2022; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=50mW/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 3.64 W/kg; SAR (10g) = 1.11 W/kg;


Pin=50mW/Zoom Scan (22.0 mm x 22.0 mm x 22.0 mm): Measurement Grid: 4.0 mm x 4.0 mm
mm x 1.4 mm

Power Drift = -0.01 dB

SAR (1g) = 3.86 W/kg; SAR (10g) = 1.16 W/kg

Smallest distance from peaks to all points 3 dB below = 7.2 mm

Ratio of SAR at M2 to SAR at M1 = 65.4 %

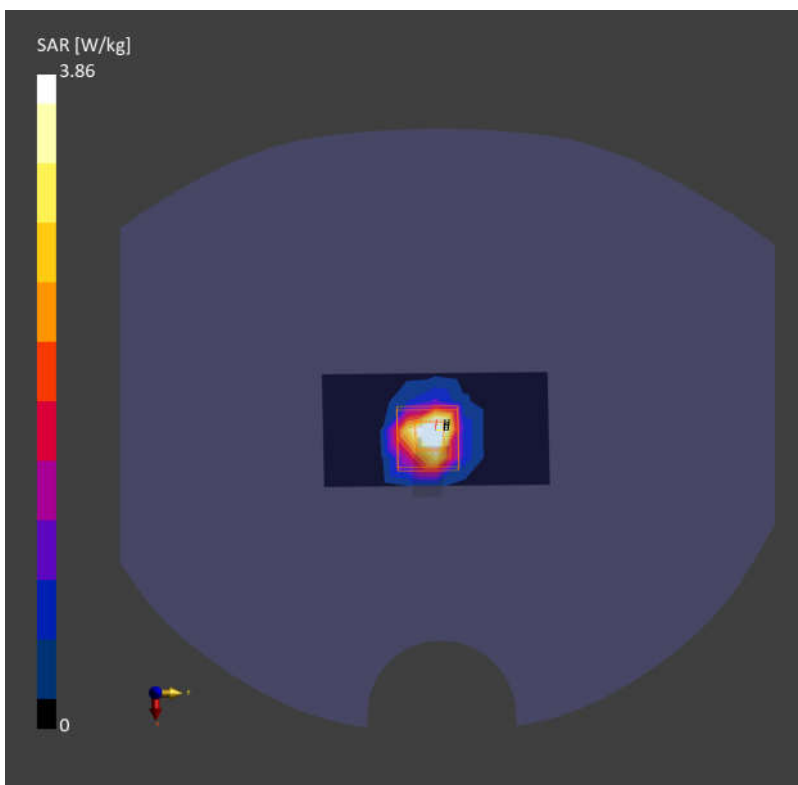

Date: 2025-01-24

System Check_Head_5600MHz**DUT: D5GHzV2 - SN1113**

Communication System: CW; Frequency: 5600.000 MHz; Duty Cycle: 1:1

Medium: Head Simulating Liquid Medium parameters used: $f = 5600.000$ MHz; $\sigma = 4.95$ S/m; $\epsilon_r = 34.4$

Ambient Temperature: 23.3°C; Liquid Temperature: 22.7°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7774; ConvF(3.87, 4.18, 3.91); Calibrated: 2024-06-27
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1358; Calibrated: 2024-05-23
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2022; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=50mW/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 3.58 W/kg; SAR (10g) = 1.07 W/kg;


Pin=50mW/Zoom Scan (22.0 mm x 22.0 mm x 22.0 mm): Measurement Grid: 4.0 mm x 4.0 mm x 1.4 mm

Power Drift = 0.02 dB

SAR (1g) = 3.96 W/kg; SAR (10g) = 1.13 W/kg

Smallest distance from peaks to all points 3 dB below = 7.2 mm

Ratio of SAR at M2 to SAR at M1 = 61.9 %

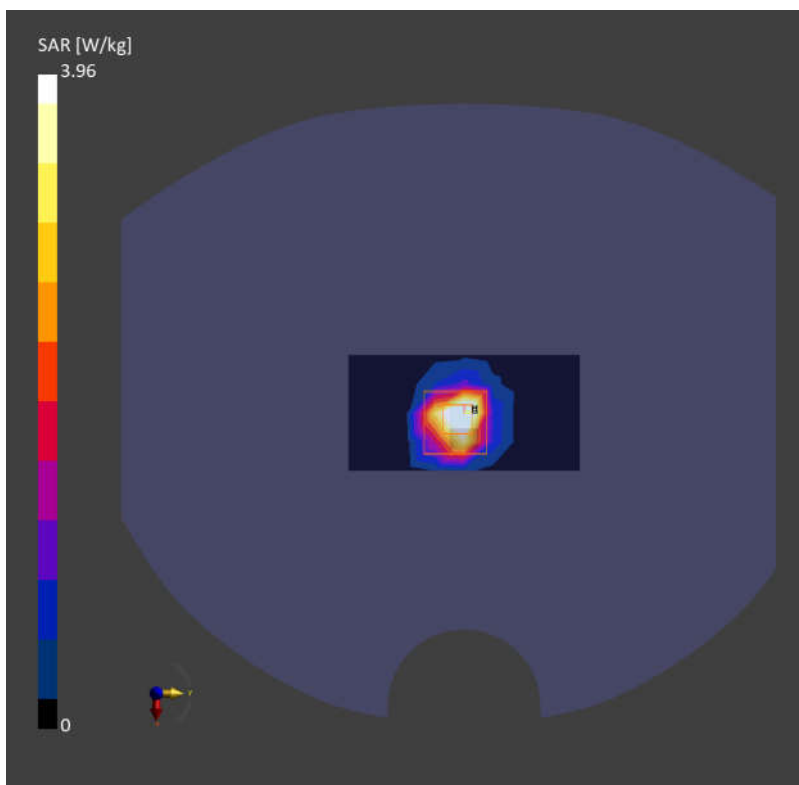

Date: 2025-01-25

System Check_Head_5750MHz**DUT: D5GHzV2 - SN1113**

Communication System: CW; Frequency: 5750.000 MHz; Duty Cycle: 1:1

Medium: Head Simulating Liquid Medium parameters used: $f = 5750.000$ MHz; $\sigma = 5.08$ S/m; $\epsilon_r = 34.3$

Ambient Temperature: 23.2°C; Liquid Temperature: 22.6°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7774; ConvF(3.91, 4.24, 3.96); Calibrated: 2024-06-27
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1358; Calibrated: 2024-05-23
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2022; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=50mW/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 3.31 W/kg; SAR (10g) = 1.00 W/kg;


Pin=50mW/Zoom Scan (22.0 mm x 22.0 mm x 22.0 mm): Measurement Grid: 4.0 mm x 4.0 mm x 1.4 mm

Power Drift = 0.03 dB

SAR (1g) = 3.84 W/kg; SAR (10g) = 1.09 W/kg

Smallest distance from peaks to all points 3 dB below = 7.2 mm

Ratio of SAR at M2 to SAR at M1 = 58.2 %

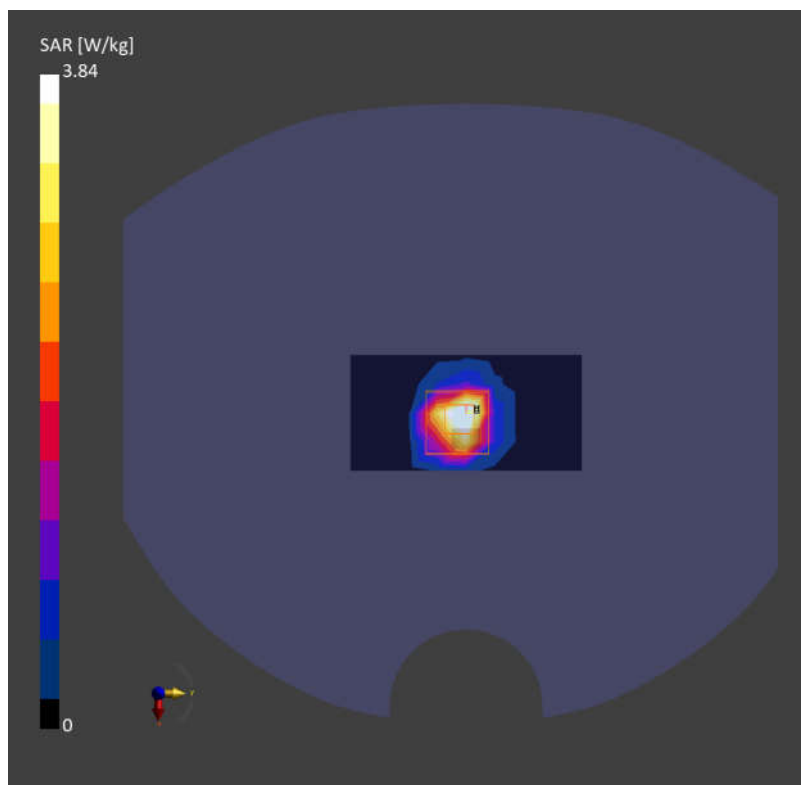

Date: 2025-01-14

System Check_Head_3700MHz**DUT: D3700V2 - SN1008**

Communication System: CW; Frequency: 3700.000 MHz; Duty Cycle: 1:1

Medium: Head Simulating Liquid Medium parameters used: $f = 3700.000$ MHz; $\sigma = 2.99$ S/m; $\epsilon_r = 38.4$

Ambient Temperature: 23.3°C; Liquid Temperature: 22.8°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7774; ConvF(5.18, 5.67, 5.29); Calibrated: 2024-06-27
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1358; Calibrated: 2024-05-23
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2022; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=50mW/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 3.29 W/kg; SAR (10g) = 1.21 W/kg;


Pin=50mW/Zoom Scan (24.0 mm x 24.0 mm x 22.0 mm): Measurement Grid: 4.0 mm x 4.0mm x 1.4 mm

Power Drift = -0.01 dB

SAR (1g) = 3.54 W/kg; SAR (10g) = 1.31 W/kg

Smallest distance from peaks to all points 3 dB below = 8.1 mm

Ratio of SAR at M2 to SAR at M1 = 77.2 %

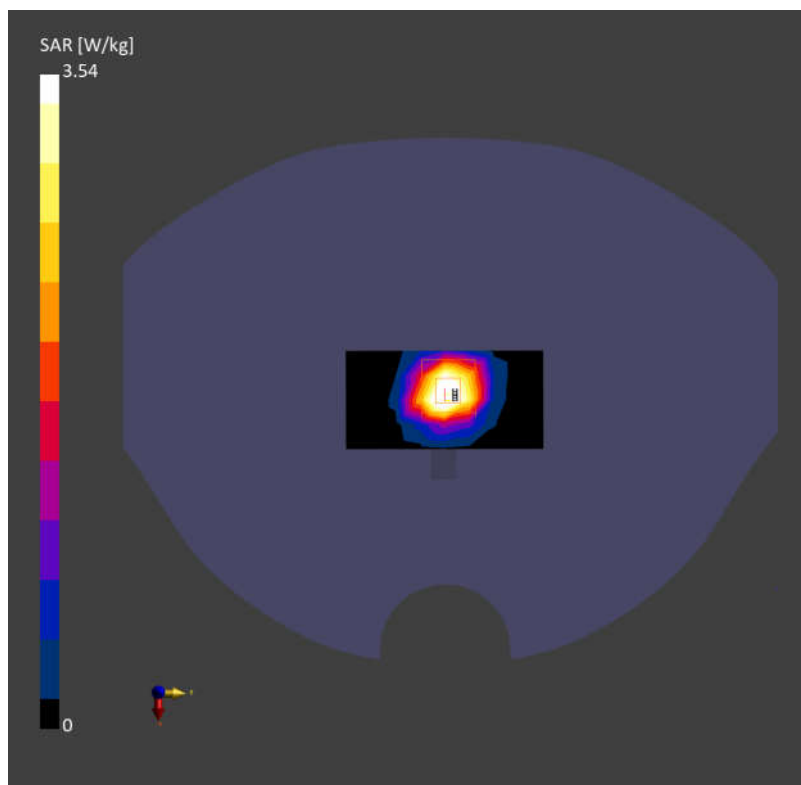

Date: 2025-01-10

System Check_Head_13MHz**DUT: CLA13 - SN:1023**

Communication System: ; Frequency: 13.000

Medium: HSL. Medium parameters used: $f=13.000$ MHz; $\sigma=0.757$ S/m; $\epsilon_r=53.7$

Ambient Temperature: 23.3°C; Liquid Temperature: 22.8°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7706; ConvF(16.1, 16.1, 16.1); Calibrated: 2024-01-24
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1649; Calibrated: 2024-07-03
- Phantom: ELI V8.0 (20deg probe tilt); Serial: 2135
- Measurement Software: 16.4.0.5005

Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 15.0 mm x 15.0 mm

SAR (1g) = 0.160 W/kg; SAR (10g) = 0.093 W/kg;

Zoom Scan (32.0 mm x 32.0 mm x 30.0 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm;


Graded Ratio:1.4

Power Drift = 0.01 dB

SAR (1g) = 0.143 W/kg; SAR (10g) = 0.081 W/kg;

Smallest distance from peaks to all points 3dB below is 15.9 mm

Ratio of SAR at M2 to SAR at M1 = 72.8 %

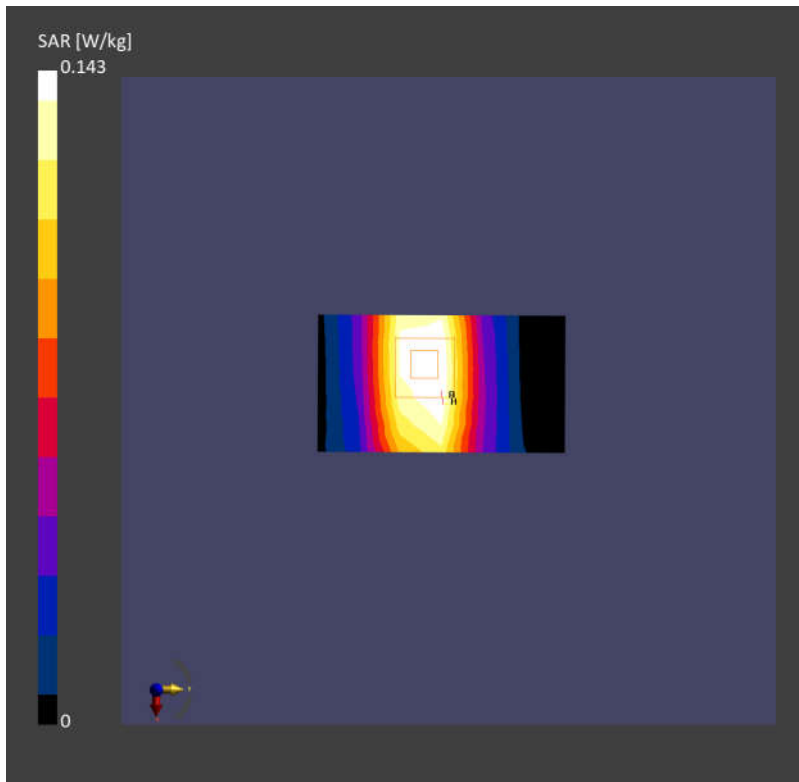

Date: 2025-02-15

System Check_Head_2600MHz**DUT: D2600V2 - SN1112**

Communication System: CW; Frequency: 2600.000 MHz; Duty Cycle: 1:1

Medium: Head Simulating Liquid Medium parameters used: $f = 2600.000$ MHz; $\sigma = 1.91$ S/m; $\epsilon_r = 39.2$

Ambient Temperature: 23.2°C; Liquid Temperature: 22.6°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7774; ConvF(6.16, 6.71, 6.3); Calibrated: 2024-06-27
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1358; Calibrated: 2024-05-23
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2022; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=50mW/Area Scan (40.0 mm x 96.0 mm): Measurement Grid: 10.0 mm x 12.0 mm
SAR (1g) = 2.66 W/kg; SAR (10g) = 1.19 W/kg;

Pin=50mW/Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.5 mm
Power Drift = -0.01 dB
SAR (1g) = 2.70 W/kg; SAR (10g) = 1.26 W/kg
Smallest distance from peaks to all points 3 dB below = 8.0 mm
Ratio of SAR at M2 to SAR at M1 = 79.4 %

