

Appendix 4

Probe Calibration Certificate

Schmid & Partner Engineering AG

Zeughausstrasse 43, 8004 Zurich, Switzerland, Phone +41 1 245 97 00, Fax +41 1 245 97 79

Calibration Certificate

Dosimetric E-Field Probe

Type:

ET3DV6

Serial Number:

1508

Place of Calibration:

Zurich

Date of Calibration:

October 25, 2001

Calibration Interval:

12 months

Schmid & Partner Engineering AG hereby certifies, that this device has been calibrated on the date indicated above. The calibration was performed in accordance with specifications and procedures of Schmid & Partner Engineering AG.

Wherever applicable, the standards used in the calibration process are traceable to international standards. In all other cases the standards of the Laboratory for EMF and Microwave Electronics at the Swiss Federal Institute of Technology (ETH) in Zurich, Switzerland have been applied.

Calibrated by:

N. Edlösser Meriana

Approved by:

Alain Katz

Probe ET3DV6

SN:1508

Manufactured:	October 24, 1999
Remade:	October 11, 2001
Recalibrated:	October 25, 2001

Calibrated for System DASY3

DASY3 - Parameters of Probe: ET3DV6 SN:1508

Sensitivity in Free Space

NormX	1.62 $\mu\text{V}/(\text{V}/\text{m})^2$
NormY	1.51 $\mu\text{V}/(\text{V}/\text{m})^2$
NormZ	1.49 $\mu\text{V}/(\text{V}/\text{m})^2$

Diode Compression

DCP X	97 mV
DCP Y	97 mV
DCP Z	97 mV

Sensitivity in Tissue Simulating Liquid


Head	450 MHz	$\epsilon_r = 40.4 \pm 5\%$	$s = 0.87 \pm 5\% \text{ mho/m}$
ConvF X	6.82	extrapolated	Boundary effect:
ConvF Y	6.82	extrapolated	Alpha 0.25
ConvF Z	6.82	extrapolated	Depth 2.86
Head	900 MHz	$\epsilon_r = 41.5 \pm 5\%$	$s = 0.97 \pm 5\% \text{ mho/m}$
Head	835 MHz	$\epsilon_r = 41.5 \pm 5\%$	$s = 0.90 \pm 5\% \text{ mho/m}$
ConvF X	6.35	$\pm 9.5\% (k=2)$	Boundary effect:
ConvF Y	6.35	$\pm 9.5\% (k=2)$	Alpha 0.35
ConvF Z	6.35	$\pm 9.5\% (k=2)$	Depth 2.68
Head	1500 MHz	$\epsilon_r = 40.4 \pm 5\%$	$s = 1.23 \pm 5\% \text{ mho/m}$
ConvF X	5.72	interpolated	Boundary effect:
ConvF Y	5.72	interpolated	Alpha 0.47
ConvF Z	5.72	interpolated	Depth 2.43
Head	1800 MHz	$\epsilon_r = 40.0 \pm 5\%$	$s = 1.40 \pm 5\% \text{ mho/m}$
Head	1900 MHz	$\epsilon_r = 40.0 \pm 5\%$	$s = 1.40 \pm 5\% \text{ mho/m}$
ConvF X	5.41	$\pm 9.5\% (k=2)$	Boundary effect:
ConvF Y	5.41	$\pm 9.5\% (k=2)$	Alpha 0.53
ConvF Z	5.41	$\pm 9.5\% (k=2)$	Depth 2.31

Sensor Offset


Probe Tip to Sensor Center	2.7	mm
Optical Surface Detection	1.4 ± 0.2	mm

Receiving Pattern (ϕ), $\theta = 0^\circ$


f = 30 MHz, TEM cell if110

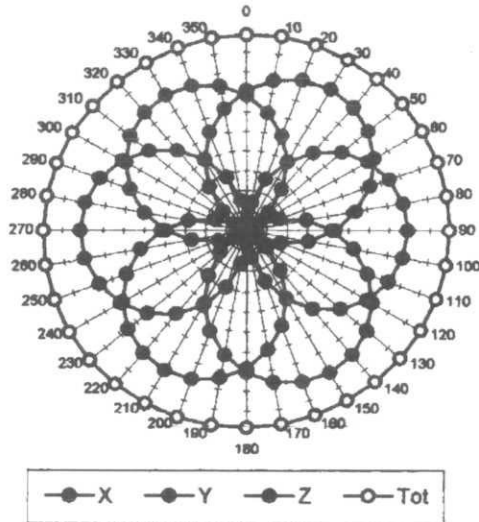


f = 100 MHz, TEM cell if110


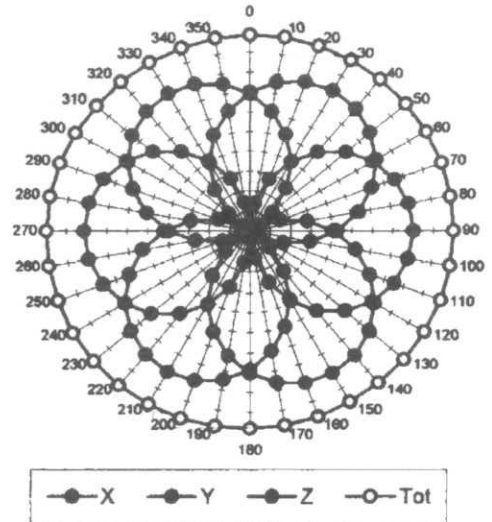


f = 300 MHz, TEM cell if110

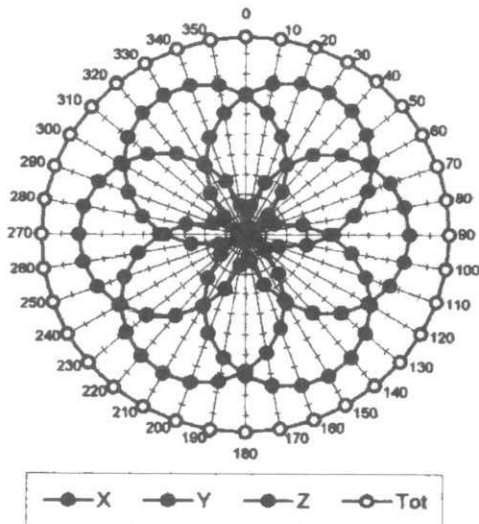


f = 900 MHz, TEM cell if110

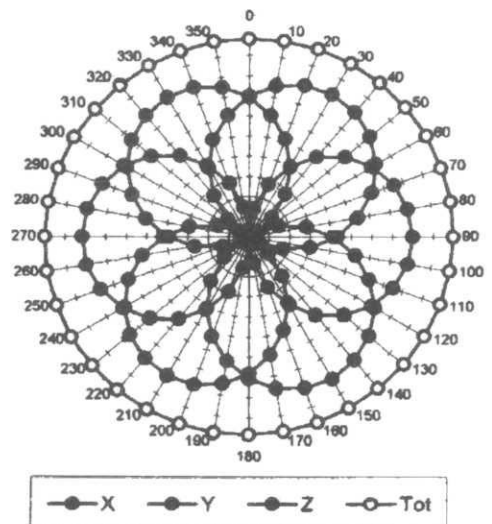

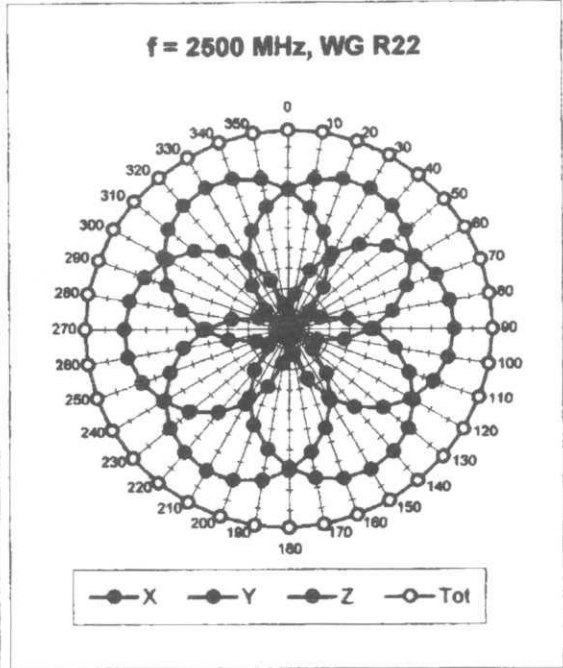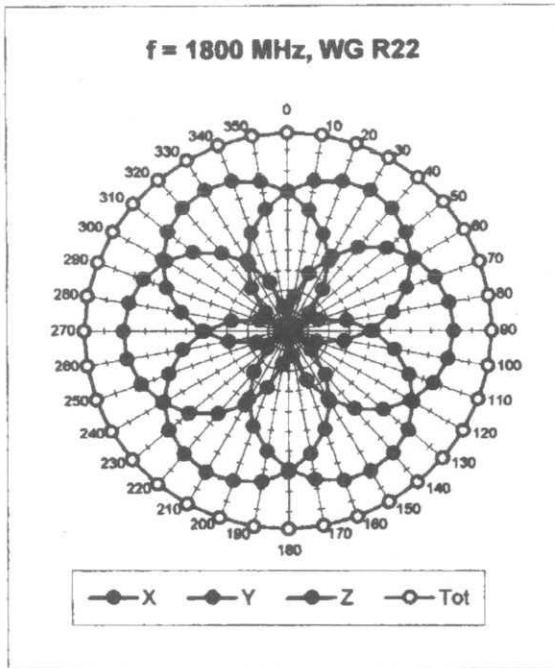


Isotropy Error (ϕ), $\theta = 0^\circ$


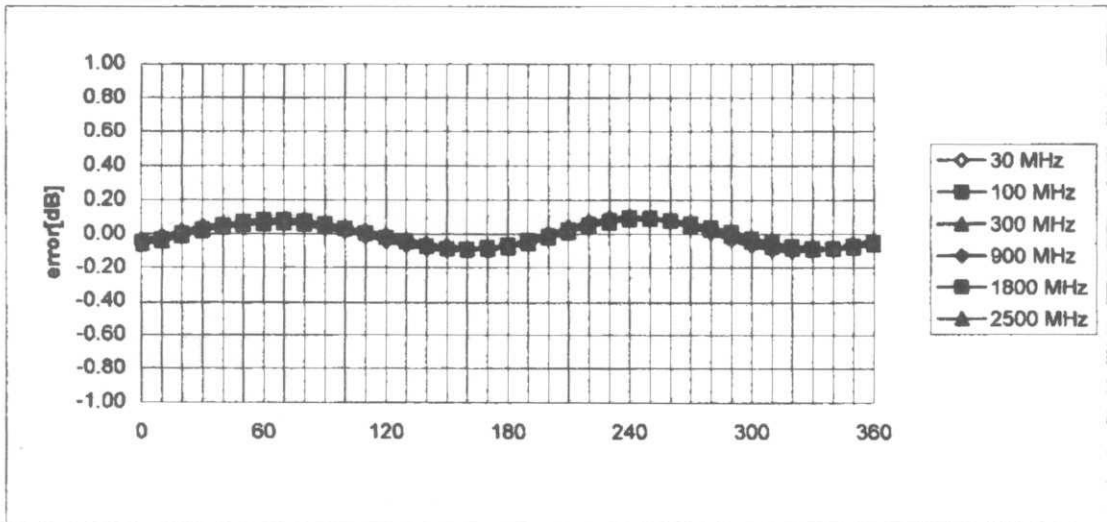


Frequency Response of E-Field


(TEM-Cell:ifi110, Waveguide R22)

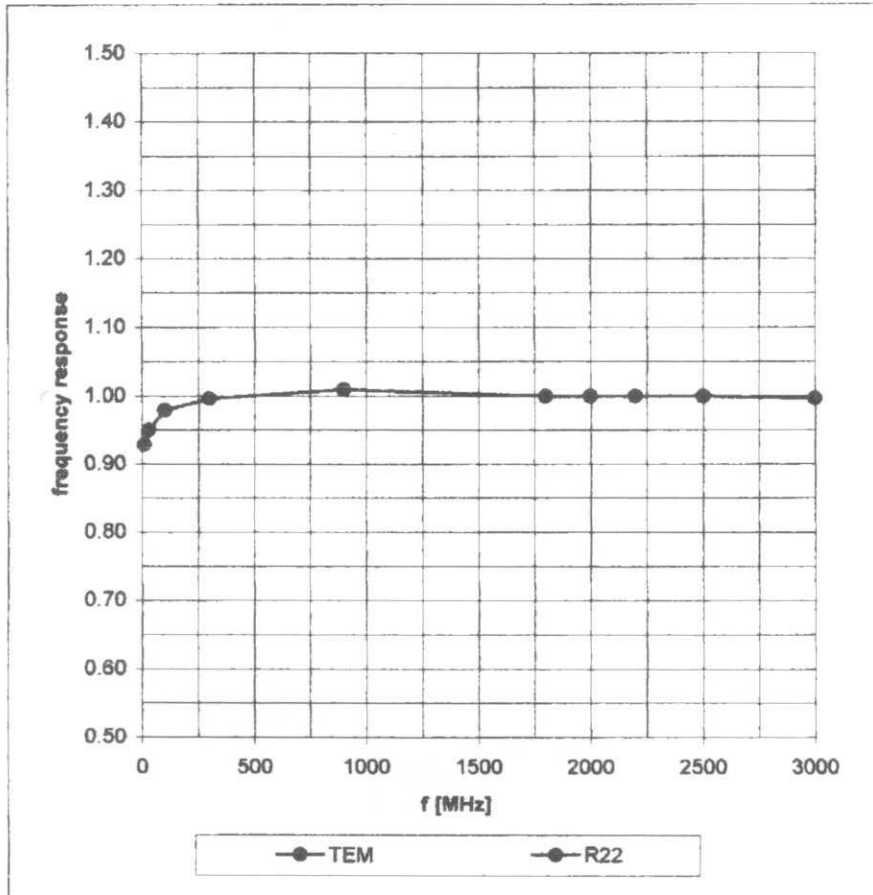

Dynamic Range $f(\text{SAR}_{\text{brain}})$ (Waveguide R22)

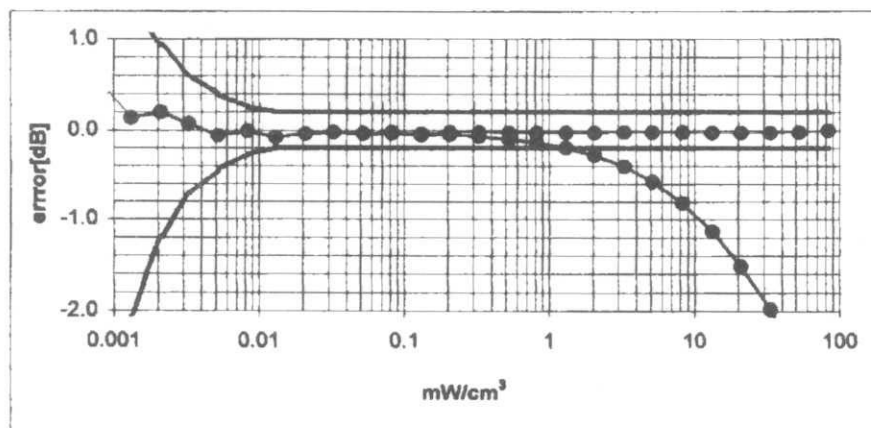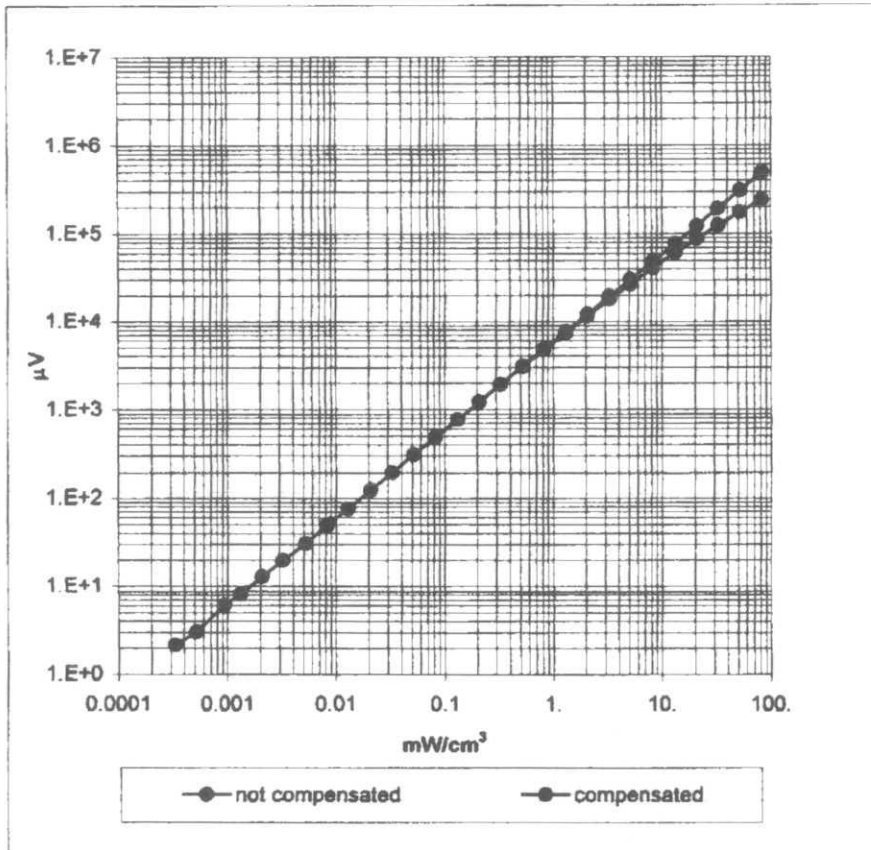

Conversion Factor Assessment

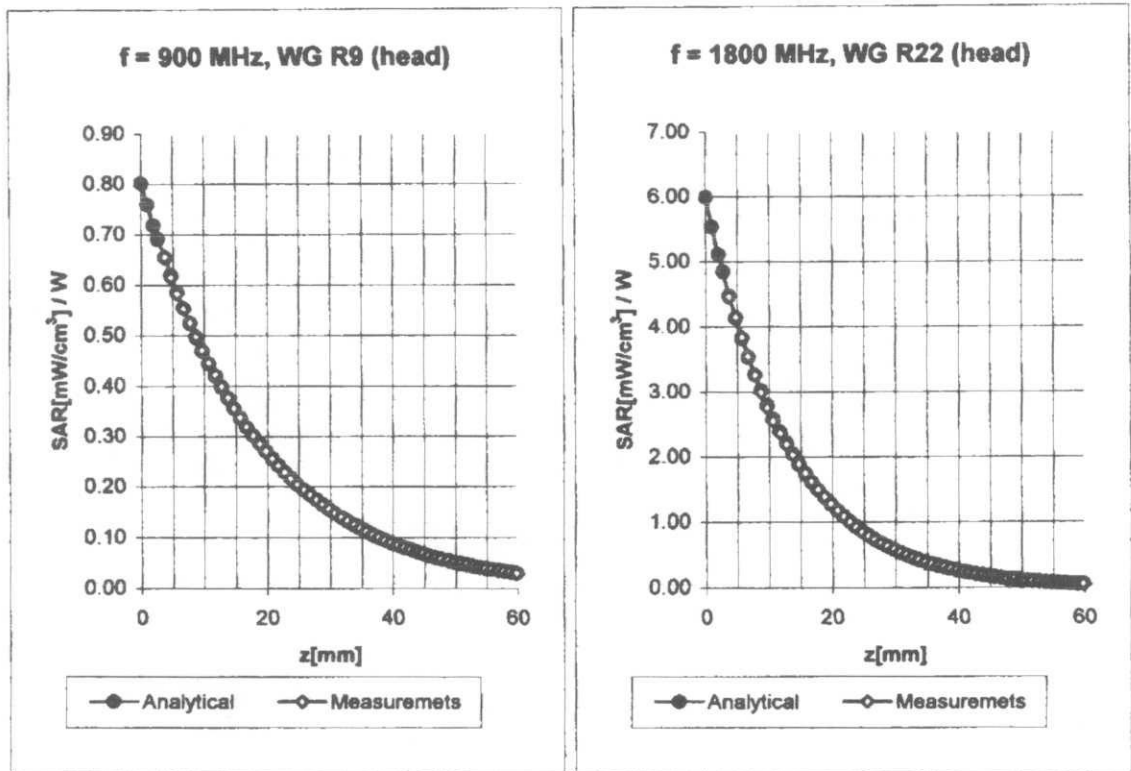

Head 800 - 1000 MHz

$\epsilon_r = 39.0 - 43.5$

$\sigma = 0.80 - 1.10$ mho/m

ConvF X **6.35** $\pm 9.5\%$ (k=2)

ConvF Y **6.35** $\pm 9.5\%$ (k=2)

ConvF Z **6.35** $\pm 9.5\%$ (k=2)

Boundary effect:

Alpha **0.35**

Depth **2.68**

Head 1700 - 1910 MHz

$\epsilon_r = 39.5 - 41.0$

$\sigma = 1.20 - 1.55$ mho/m

ConvF X **5.41** $\pm 9.5\%$ (k=2)

ConvF Y **5.41** $\pm 9.5\%$ (k=2)

ConvF Z **5.41** $\pm 9.5\%$ (k=2)


Boundary effect:

Alpha **0.53**

Depth **2.31**

Deviation from Isotropy in HSL

Error (θ, ϕ), $f = 900$ MHz

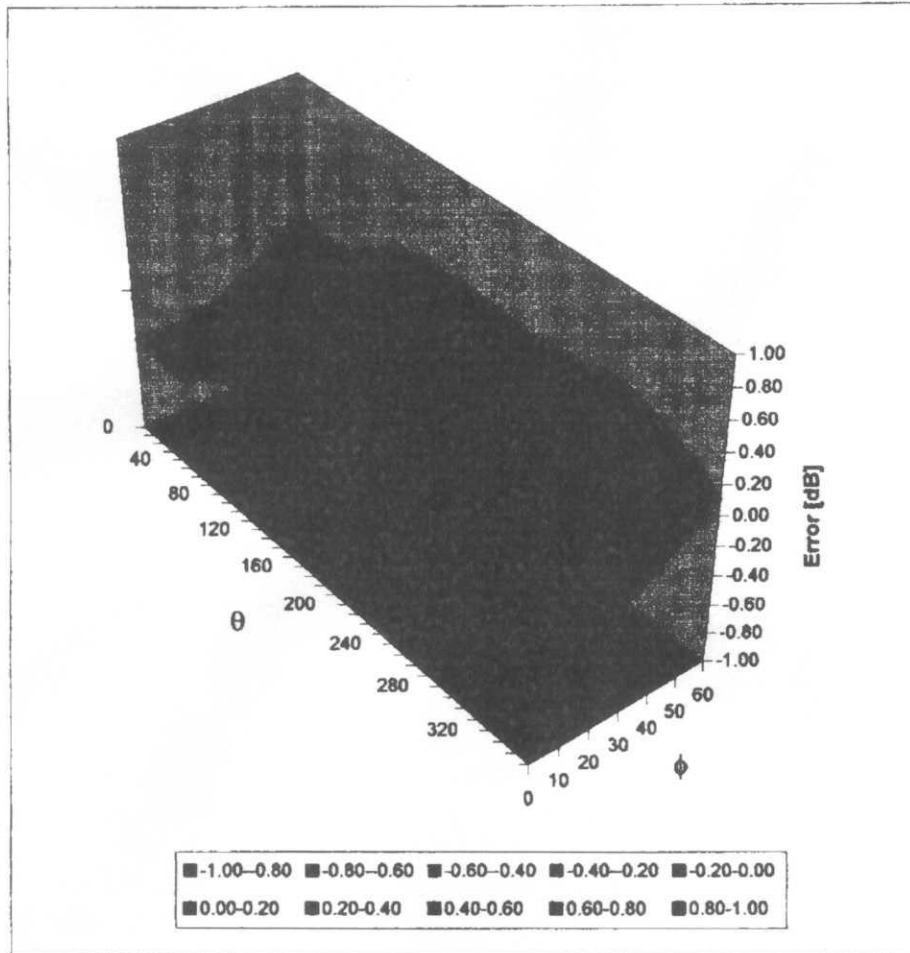


Additional Conversion Factors for Dosimetric E-Field Probe

Type:	ET3DV6
Serial Number:	1508
Place of Assessment:	Zurich
Date of Assessment:	November 14, 2001
Probe Calibration Date:	October 25, 2001

Schmid & Partner Engineering AG hereby certifies that conversion factor(s) of this probe have been evaluated on the date indicated above. The assessment was performed using the FDTD numerical code SEMCAD of Schmid & Partner Engineering AG. Since the evaluation is coupled with measured conversion factors, it has to be recalculated yearly, i.e., following the re-calibration schedule of the probe. The uncertainty of the numerical assessment is based on the extrapolation from measured value at 900 MHz or at 1800 MHz.

Assessed by:



Dosimetric E-Field Probe ET3DV6 SN:1508

Conversion factor (\pm standard deviation)

835 MHz	ConvF	6.5 \pm 8%	$\epsilon_r = 41.5$ $\sigma = 0.90$ mho/m (head tissue)
1950 MHz	ConvF	5.1 \pm 8%	$\epsilon_r = 40.0$ $\sigma = 1.40$ mho/m (head tissue)
835 MHz	ConvF	6.2 \pm 8%	$\epsilon_r = 55.2$ $\sigma = 0.97$ mho/m (body tissue)
900 MHz	ConvF	6.1 \pm 8%	$\epsilon_r = 55.0$ $\sigma = 1.05$ mho/m (body tissue)
1800 MHz	ConvF	5.0 \pm 8%	$\epsilon_r = 53.3$ $\sigma = 1.52$ mho/m (body tissue)
1950 MHz	ConvF	4.7 \pm 8%	$\epsilon_r = 53.3$ $\sigma = 1.52$ mho/m (body tissue)

Appendix 5

Photographs of the device under test



Figure 7. Front of the Phone (Antenna Fixed)



Figure 8. Distance of the Antenna (Fixed) to the Base of the Flat Phantom



Figure 9. Distance of the Antenna (Fixed) to the Base of the Flat Phantom

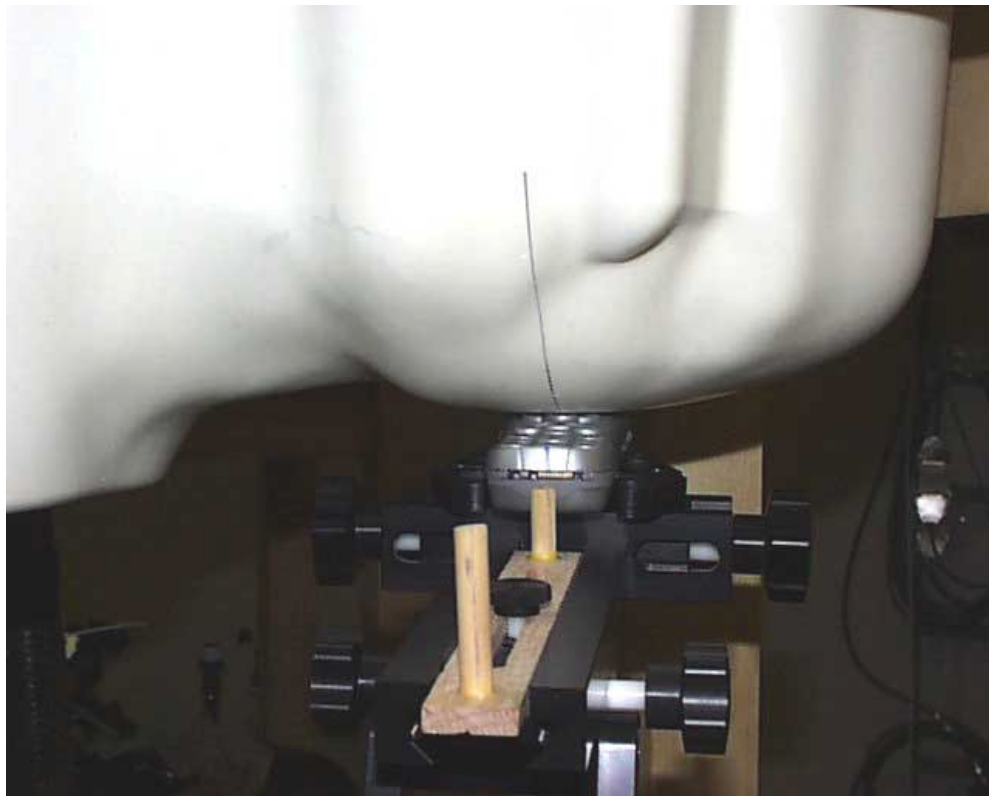


Figure 10. Front View of Phone Placed Against Head with Antenna Fixed



Figure 11. Back View of Phone Placed Against Head with Antenna Fixed



Figure 12. Front View of Phone Placed Against the Head (15° Tilt Position) with Antenna Fixed



Figure 13. Back View of Phone Placed Against the Head (15° Tilt Position) with Antenna Fixed

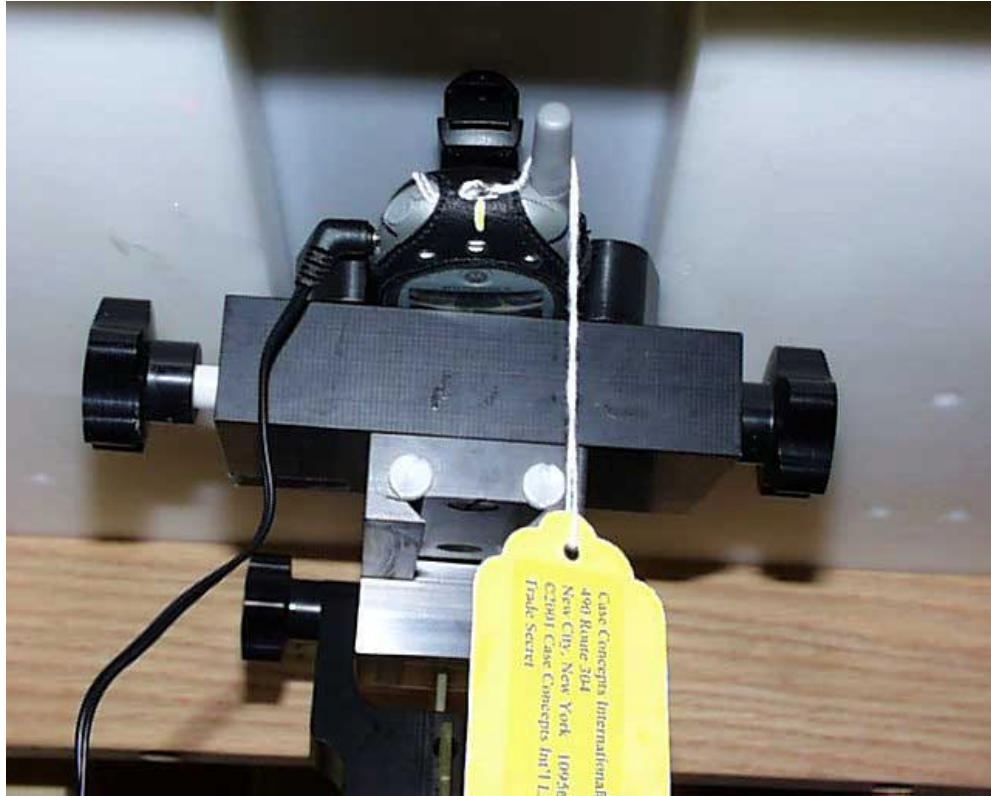


Figure 14. Phone with leather pouch with universal belt clip Placed under a Flat Phantom with Headset (Antenna Fixed)

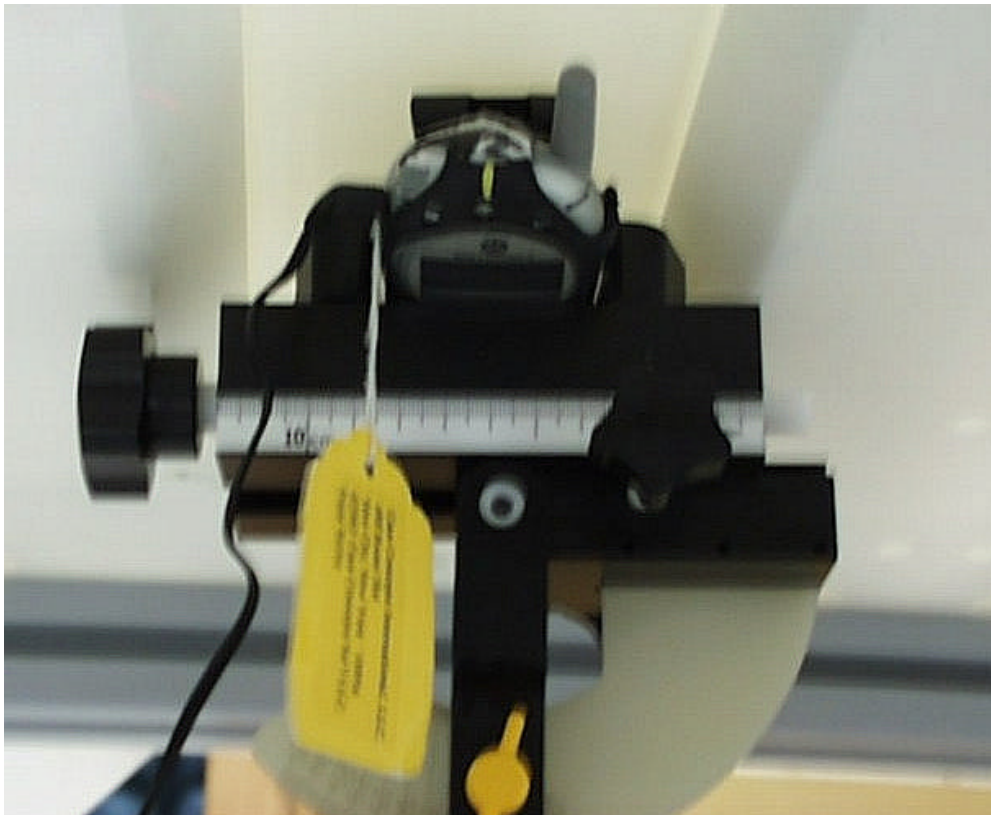


Figure 15. Phone with leather pouch with wishbone Placed under a Flat Phantom with Headset (Antenna Fixed)