

Schmid & Partner Engineering AG

Zeughausstrasse 43, 8004 Zurich, Switzerland, Phone +41 1 245 97 00, Fax +41 1 245 97 79

Calibration Certificate

1800 MHz System Validation Dipole

Type:

D1800V2

Serial Number:

258

Place of Calibration:

Zurich

Date of Calibration:

September 24, 2002

Calibration Interval:

24 months

Schmid & Partner Engineering AG hereby certifies, that this device has been calibrated on the date indicated above. The calibration was performed in accordance with specifications and procedures of Schmid & Partner Engineering AG.

Wherever applicable, the standards used in the calibration process are traceable to international standards. In all other cases the standards of the Laboratory for EMF and Microwave Electronics at the Swiss Federal Institute of Technology (ETH) in Zurich, Switzerland have been applied.

Calibrated by:

D. Vetter

Approved by:

Thomas Kofler

DASY

Dipole Validation Kit

Type: D1800V2

Serial: 258

Manufactured: November 20, 1999

Calibrated: September 24, 2002

1. Measurement Conditions

The measurements were performed in the flat section of the new generic twin phantom filled with head simulating glycol solution of the following electrical parameters at 1800 MHz:

Relative Dielectricity	40.3	± 5%
Conductivity	1.36 mho/m	± 5%

The DASY System with a dosimetric E-field probe ET3DV6 (SN:1507, Conversion factor 5.3 at 1800 MHz) was used for the measurements.

The dipole was mounted on the small tripod so that the dipole feedpoint was positioned below the center marking of the flat phantom section and the dipole was oriented parallel to the body axis (the long side of the phantom). The standard measuring distance was 10mm from dipole center to the solution surface. The included distance holder was used during measurements for accurate distance positioning.

The coarse grid with a grid spacing of 20mm was aligned with the dipole. The 5x5x7 fine cube was chosen for cube integration. Probe isotropy errors were cancelled by measuring the SAR with normal and 90° turned probe orientations and averaging.

The dipole input power (forward power) was 250mW ± 3 %. The results are normalized to 1W input power.

2.1. SAR Measurement with DASY3 System

Standard SAR-measurements were performed according to the measurement conditions described in section 1. The results (see figure supplied) have been normalized to a dipole input power of 1W (forward power). The resulting averaged SAR-values measured with the dosimetric probe ET3DV6 SN:1507 and applying the worst-case extrapolation are:

averaged over 1 cm ³ (1 g) of tissue:	38.6 mW/g
averaged over 10 cm ³ (10 g) of tissue:	20.4 mW/g

2.2 SAR Measurement with DASY4 System

Standard SAR-measurements were performed according to the measurement conditions described in section 1. The results (see figure supplied) have been normalized to a dipole input power of 1W (forward power). The resulting averaged SAR-values measured with the dosimetric probe ET3DV6 SN:1507 and applying the advanced extrapolation are:

averaged over 1 cm ³ (1 g) of tissue:	35.5 mW/g
averaged over 10 cm ³ (10 g) of tissue:	19.2 mW/g

3. Dipole Impedance and Return Loss

The impedance was measured at the SMA-connector with a network analyzer and numerically transformed to the dipole feedpoint. The transformation parameters from the SMA-connector to the dipole feedpoint are:

Electrical delay:	1.199 ns	(one direction)
Transmission factor:	0.980	(voltage transmission, one direction)

The dipole was positioned at the flat phantom sections according to section 1 and the distance holder was in place during impedance measurements.

Feedpoint impedance at 1800 MHz:	$\text{Re}\{Z\} = 52.0 \Omega$
----------------------------------	--------------------------------

	$\text{Im}\{Z\} = 5.9 \Omega$
--	-------------------------------

Return Loss at 1800 MHz	-24.2 dB
-------------------------	----------

4. Modification

Small end caps (3 mm in length) made of Teflon have been added to the dipole arms by the Client.

5. Handling

Do not apply excessive force to the dipole arms, because they might bend. Bending of the dipole arms stresses the soldered connections near the feedpoint leading to a damage of the dipole.

6. Design

The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals.

7. Power Test



After long term use with 40W radiated power, only a slight warming of the dipole near the feedpoint can be measured.

09/24/02

Validation Dipole D1800V2 SN:258, d = 10 mm

Frequency: 1800 MHz; Antenna Input Power: 250 [mW]
SAM Phantom, Flat Section; Grid Spacing: Dx = 20.0, Dy = 20.0, Dz = 10.0
Probe: ET3DV6 - SN1507; ConvF(5.30,5.30,5.30) at 1800 MHz; IEEE1528 1800 MHz: $\sigma = 1.36 \text{ mho/m}$, $\epsilon_r = 40.3$, $\rho = 1.00 \text{ g/cm}^3$
Cubes (2): Peak: 17.7 mW/g $\pm 0.03 \text{ dB}$, SAR (1g): 9.64 mW/g $\pm 0.00 \text{ dB}$, SAR (10g): 5.11 mW/g $\pm 0.03 \text{ dB}$, (Worst-case extrapolation)
Penetration depth: 8.5 (8.1, 9.3) [mm]
Powerdrift: -0.01 dB

SAR_{10g} [mW/g]

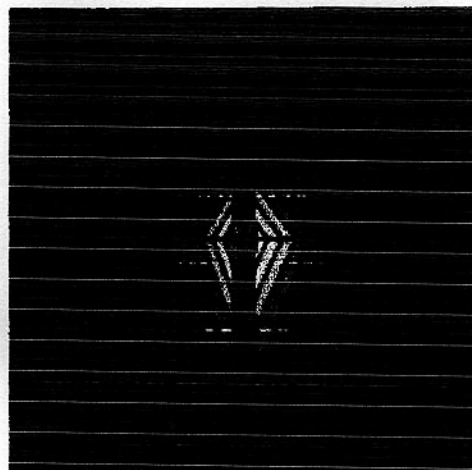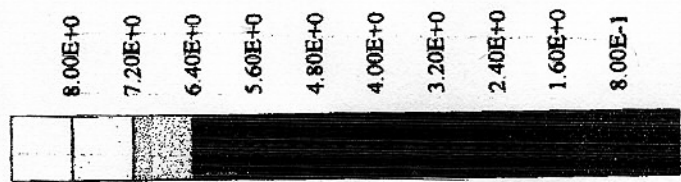

09/24/02

Validation Dipole D1800V2 SN:258, d = 10 mm

Frequency: 1800 MHz; Antenna Input Power: 250 [mW]

SAM Phantom; Flat Section; Grid Spacing: Dx = 20.0, Dy = 20.0, Dz = 10.0



Probe: ET3DV6 - SN1507; ConvF(5.30, 5.30, 5.30) at 1800 MHz; IEEE1528 1800 MHz: $\sigma = 1.36$ mho/m $\epsilon_r = 40.3$ $\rho = 1.00$ g/cm³

Cubes (2): Peak: 15.4 mW/g ± 0.03 dB, SAR (1g): 8.87 mW/g ± 0.00 dB, SAR (10g): 4.81 mW/g ± 0.03 dB, (Advanced extrapolation)

Penetration depth: 9.2 (9.1, 9.5) [mm]

Powerdrift: -0.01 dB

SAR_{10g} [mW/g]

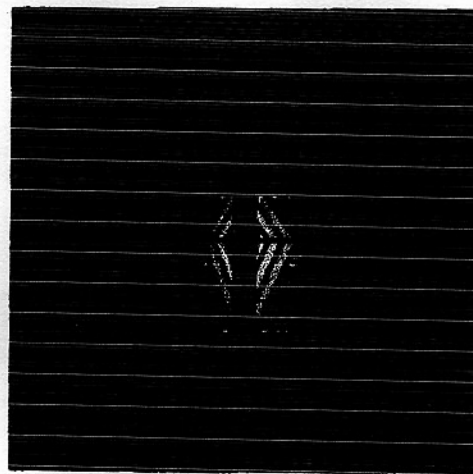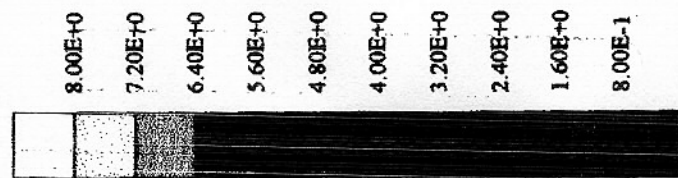

CH1 S11 1 U FS

1: 52.045 Ω 5.9453 Ω 525.68 pH

24 Sep 2002 09:51:33

1 800.000 000 MHz

258

De1


PRm

Cor

Avg

16


↑

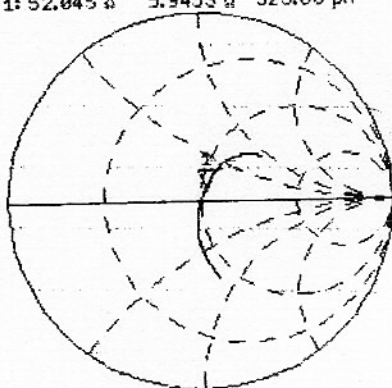

CH2 S11 LOG 5 dB/REF -5 dB 1:-24.224 dB 1 800.000 000 MHz

PRm
Cor

↑

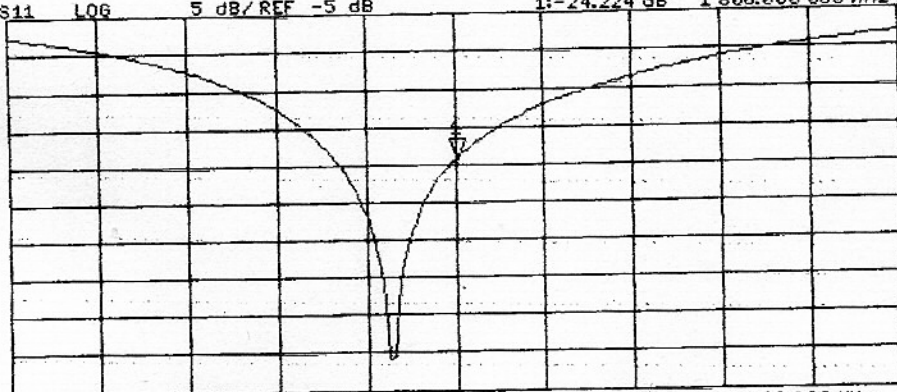

START 1.600.000 000 MHz

STOP 2 000.000 000 MHz