

Appendix C: System Check Plots

RF SAFETY LABORATORY

System Verification

Verification Conditions

Verification Source	Power [dBm]	Phantom Section	Test Distance [mm]	Signal, UID	Frequency [MHz]	ConvF (x, y, z)
D750V3 – SN1235	17.0	Flat	15	CW, 0	750.000	9.2, 9.0,9.65

Test Setup


Test Date	Ambient Temp [°C]	TSL Temp [°C]	Measurement SW	Phantom	TSL Type	Cond. [S/m]	Perm.	Probe, Cal. Date	DAE, Cal. Date
2025-08-08	22.3	21.3	16.4.0.5005	Twin-SAM V8.0 – 2165	Head Simulating Liquid	0.883	43.7	EX3DV4 – SN7836, 2024-09-12	DAE4ip Sn1839, 2024-09-04

Scans Setup

	Area Scan	Zoom Scan
Grid Extents [mm]	40.0 x 90.0	30.0 x 30.0 x 31.2
Grid Steps [mm]	10.0 x 15.0	6.0 x 6.0 x 1.5
Sensor Surface [mm]	3.0	1.4
Grading Ratio	N/A	1.5

Measurement Results

	SAR [W/kg] or APD [W/m²]	Deviation [%]
psSAR1g	0.432	-0.81
psSAR10g	0.286	0.29
Peak SAR (Extrapolated)	0.638	1.03
psAPD (4.0 cm², sq)	N/A	N/A

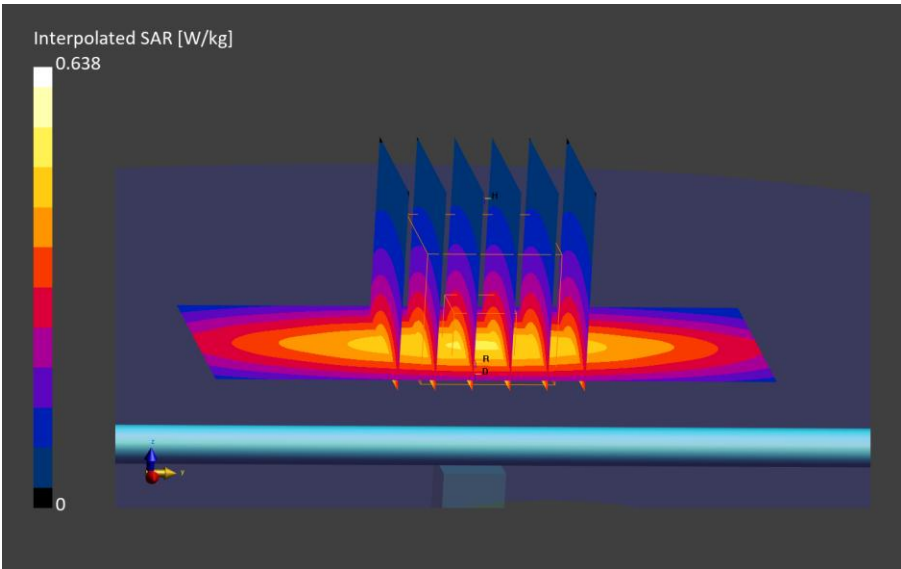

RF SAFETY LABORATORY

System Verification

Verification Conditions

Verification Source	Power [dBm]	Phantom Section	Test Distance [mm]	Signal, UID	Frequency [MHz]	ConvF (x, y, z)
D1750V2 – SN1205	17.0	Flat	10	CW, 0	1750.000	7.52, 7.93,7.47

Test Setup


Test Date	Ambient Temp [°C]	TSL Temp [°C]	Measurement SW	Phantom	TSL Type	Cond. [S/m]	Perm.	Probe, Cal. Date	DAE, Cal. Date
2025-08-11	22.7	22.5	16.4.0.5005	Twin-SAM V8.0 – 2159	Head Simulating Liquid	1.36	40.1	EX3DV4 – SN7859, 2025-05-05	DAE4ip Sn1905, 2025-04-25

Scans Setup

	Area Scan	Zoom Scan
Grid Extents [mm]	40.0 x 90.0	30.0 x 30.0 x 31.2
Grid Steps [mm]	10.0 x 15.0	6.0 x 6.0 x 1.5
Sensor Surface [mm]	3.0	1.4
Grading Ratio	N/A	1.5

Measurement Results

	SAR [W/kg] or APD [W/m²]	Deviation [%]
psSAR1g	1.73	-5.43
psSAR10g	0.934	-2.94
Peak SAR (Extrapolated)	2.96	-9
psAPD (4.0 cm², sq)	N/A	N/A

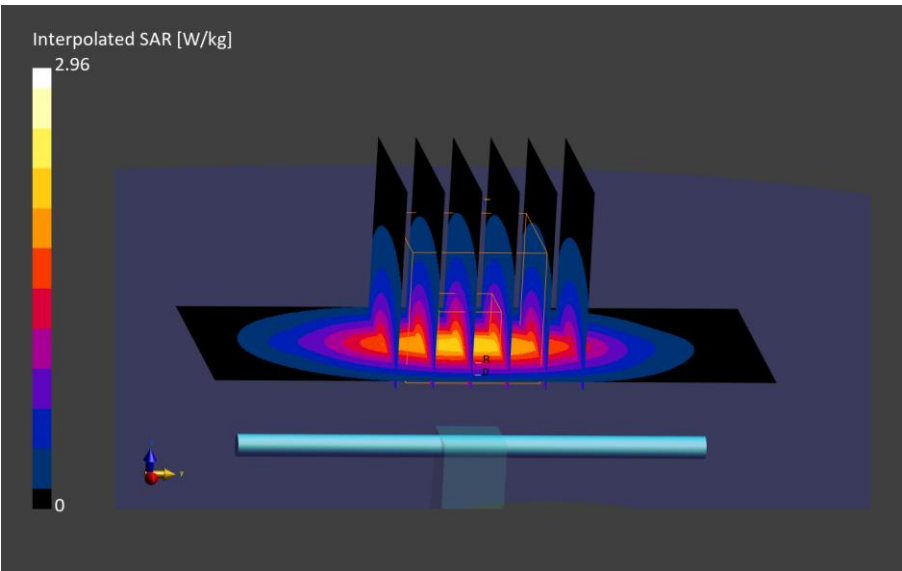

RF SAFETY LABORATORY

System Verification

Verification Conditions

Verification Source	Power [dBm]	Phantom Section	Test Distance [mm]	Signal, UID	Frequency [MHz]	ConvF (x, y, z)
D1900V2 – SN5d252	17.0	Flat	10	CW, 0	1900.000	7.26, 7.65, 7.22

Test Setup


Test Date	Ambient Temp [°C]	TSL Temp [°C]	Measurement SW	Phantom	TSL Type	Cond. [S/m]	Perm.	Probe, Cal. Date	DAE, Cal. Date
2025-08-07	22.5	22	16.4.0.5005	Twin-SAM V8.0 – 2159	Head Simulating Liquid	1.44	39.5	EX3DV4 – SN7859, 2025-05-05	DAE4ip Sn1905, 2025-04-25

Scans Setup

	Area Scan	Zoom Scan
Grid Extents [mm]	40.0 x 90.0	30.0 x 30.0 x 31.2
Grid Steps [mm]	10.0 x 15.0	6.0 x 6.0 x 1.5
Sensor Surface [mm]	3.0	1.4
Grading Ratio	N/A	1.5

Measurement Results

	SAR [W/kg] or APD [W/m²]	Deviation [%]
psSAR1g	1.93	-3.24
psSAR10g	1.02	-3.09
Peak SAR (Extrapolated)	3.40	-5.91
psAPD (4.0 cm², sq)	N/A	N/A

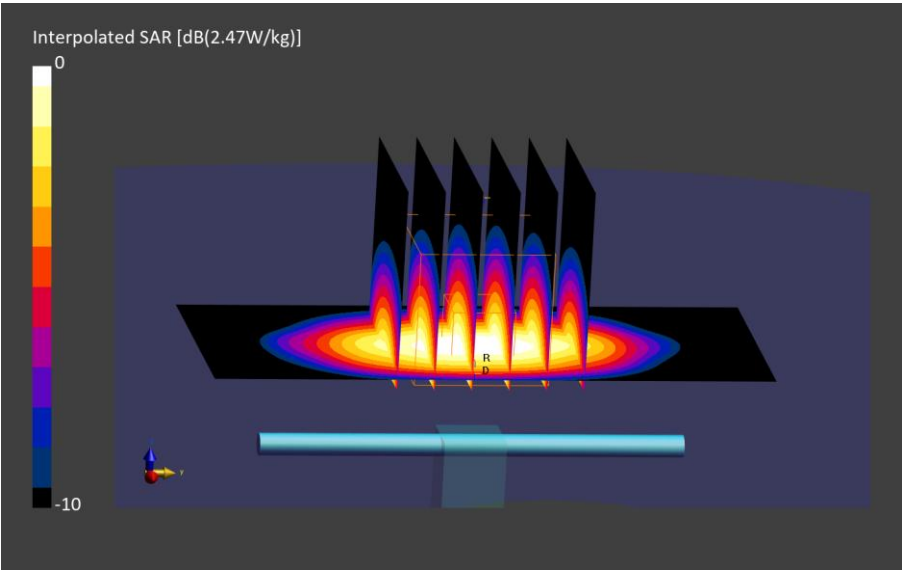

RF SAFETY LABORATORY

System Verification

Verification Conditions

Verification Source	Power [dBm]	Phantom Section	Test Distance [mm]	Signal, UID	Frequency [MHz]	ConvF (x, y, z)
D2450V2 – SN1112	17.0	Flat	10	CW, 0	2450.000	7.02, 6.86, 7.36

Test Setup


Test Date	Ambient Temp [°C]	TSL Temp [°C]	Measurement SW	Phantom	TSL Type	Cond. [S/m]	Perm.	Probe, Cal. Date	DAE, Cal. Date
2025-08-06	22.5	22.3	16.4.0.5005	Twin-SAM V8.0 – 2165	Head Simulating Liquid	1.79	40.8	EX3DV4 – SN7836, 2024-09-12	DAE4ip Sn1839, 2024-09-04

Scans Setup

	Area Scan	Zoom Scan
Grid Extents [mm]	40.0 x 80.0	30.0 x 30.0 x 31.2
Grid Steps [mm]	10.0 x 10.0	5.0 x 5.0 x 1.5
Sensor Surface [mm]	3.0	1.4
Grading Ratio	N/A	1.5

Measurement Results

	SAR [W/kg] or APD [W/m²]	Deviation [%]
psSAR1g	2.49	-1.81
psSAR10g	1.17	-1.5
Peak SAR (Extrapolated)	4.85	-7.13
psAPD (4.0 cm², sq)	N/A	N/A

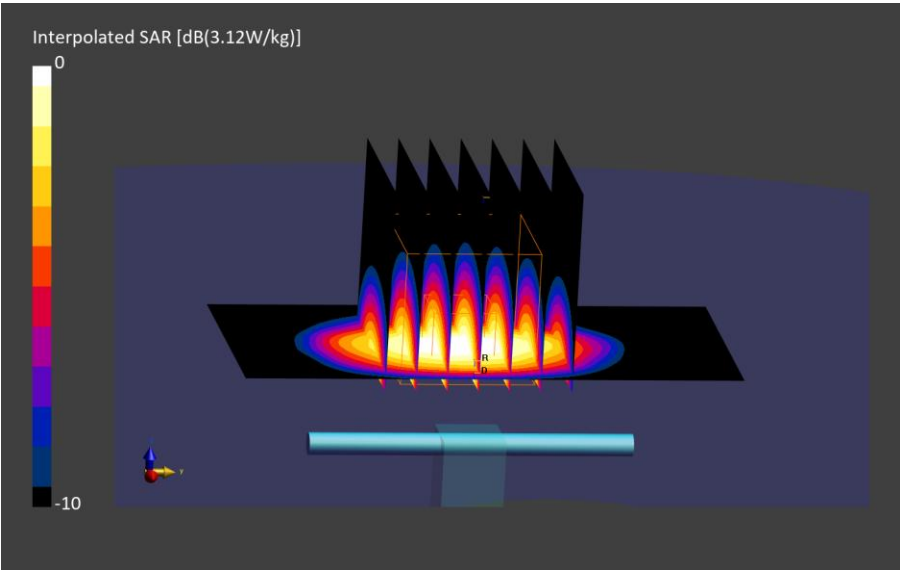

RF SAFETY LABORATORY

System Verification

Verification Conditions

Verification Source	Power [dBm]	Phantom Section	Test Distance [mm]	Signal, UID	Frequency [MHz]	ConvF (x, y, z)
D5GHzV2 – SN1396	17.0	Flat	10	CW, 0	5250.000	5.28, 5.16, 5.54

Test Setup

Test Date	Ambient Temp [°C]	TSL Temp [°C]	Measurement SW	Phantom	TSL Type	Cond. [S/m]	Perm.	Probe, Cal. Date	DAE, Cal. Date
2025-08-07	22.7	22.1	16.4.0.5005	Twin-SAM V8.0 – 2165	Head Simulating Liquid	4.66	35.9	EX3DV4 – SN7836, 2024-09-12	DAE4ip Sn1839, 2024-09-04

Scans Setup

	Area Scan	Zoom Scan
Grid Extents [mm]	40.0 x 80.0	24.0 x 28.0 x 22.9
Grid Steps [mm]	10.0 x 10.0	4.0 x 4.0 x 1.4
Sensor Surface [mm]	3.0	1.4
Grading Ratio	N/A	1.4

Measurement Results

	SAR [W/kg] or APD [W/m²]	Deviation [%]
psSAR1g	3.77	-3.44
psSAR10g	1.07	-4.69
Peak SAR (Extrapolated)	15.2	-2.23
psAPD (4.0 cm², sq)	N/A	N/A



RF SAFETY LABORATORY

System Verification

Verification Conditions

Verification Source	Power [dBm]	Phantom Section	Test Distance [mm]	Signal, UID	Frequency [MHz]	ConvF (x, y, z)
D5GHzV2 – SN1396	17.0	Flat	10	CW, 0	5750.000	4.98, 4.87,5.22

Test Setup

Test Date	Ambient Temp [°C]	TSL Temp [°C]	Measurement SW	Phantom	TSL Type	Cond. [S/m]	Perm.	Probe, Cal. Date	DAE, Cal. Date
2025-08-07	22.7	22.1	16.4.0.5005	Twin-SAM V8.0 – 2165	Head Simulating Liquid	5.24	35.0	EX3DV4 – SN7836, 2024-09-12	DAE4ip Sn1839, 2024-09-04

Scans Setup

	Area Scan	Zoom Scan
Grid Extents [mm]	40.0 x 80.0	24.0 x 28.0 x 22.9
Grid Steps [mm]	10.0 x 10.0	4.0 x 4.0 x 1.4
Sensor Surface [mm]	3.0	1.4
Grading Ratio	N/A	1.4

Measurement Results

	SAR [W/kg] or APD [W/m²]	Deviation [%]
psSAR1g	3.74	-6.84
psSAR10g	1.06	-7.24
Peak SAR (Extrapolated)	16.8	0.63
psAPD (4.0 cm², sq)	N/A	N/A

