

SAR Plots

- Verification Plots
- SAR Test Plots

DT&C Co., Ltd.

DUT: Dipole 1900 MHz; Type: D1900V2; Serial: D1900V2 - SN:5d176

Communication System: CW (0); Frequency: 1900 MHz; Duty Cycle: 1:1
Medium parameters used: $f = 1900$ MHz; $\sigma = 1.432$ S/m; $\epsilon_r = 40.573$; $\rho = 1000$ kg/m³
Phantom section: Flat Section

DASY5 Configuration:

Probe: ES3DV3 - SN3328; ConvF(5.19, 5.19, 5.19); Calibrated: 3/18/2016; ; Electronics: DAE4 Sn1391
Phantom: SAM with CRP_2016_07_22_middle; Type: QD000P40CD; Serial: TP:1786
Measurement SW: DASY52, Version 52.8 (8); SEMCAD X Version 14.6.10 (7331)

Test Date: 2016-12-17; Ambient Temp: 20.8; Tissue Temp: 21.3

1900 MHz System Verification


Area Scan (5x7x1): Measurement grid: dx=15mm, dy=15mm

Zoom Scan (5x5x7)/Cube 0: Measurement grid: dx=8mm, dy=8mm, dz=5mm

Power Drift = -0.04 dB

Peak SAR (extrapolated) = 19.1 W/kg

SAR(1 g) = 10.6 W/kg; SAR(10 g) = 5.63 W/kg

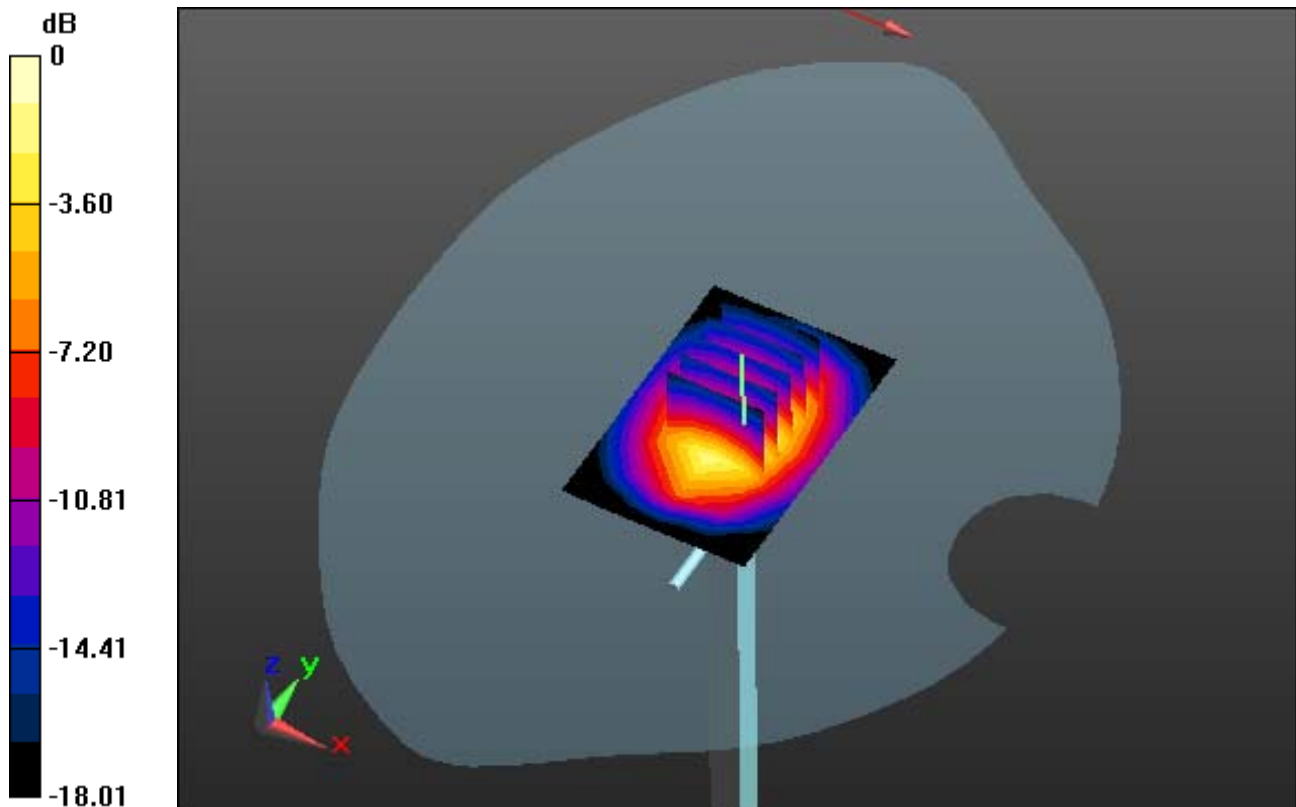

0 dB = 13.3 W/kg

DT&C Co., Ltd.

DUT: Dipole 1900 MHz; Type: D1900V2; Serial: D1900V2 - SN:5d176

Communication System: CW (0); Frequency: 1900 MHz; Duty Cycle: 1:1
Medium parameters used: $f = 1900$ MHz; $\sigma = 1.432$ S/m; $\epsilon_r = 40.573$; $\rho = 1000$ kg/m³
Phantom section: Flat Section

DASY5 Configuration:

Probe: ES3DV3 - SN3328; ConvF(5.19, 5.19, 5.19); Calibrated: 3/18/2016; ; Electronics: DAE4 Sn1391
Phantom: SAM with CRP_2016_07_22_middle; Type: QD000P40CD; Serial: TP:1786
Measurement SW: DASY52, Version 52.8 (8); SEMCAD X Version 14.6.10 (7331)

Test Date: 2016-12-17; Ambient Temp: 20.8; Tissue Temp: 21.3

1900 MHz System Verification


Area Scan (5x7x1): Measurement grid: dx=15mm, dy=15mm

Zoom Scan (5x5x7)/Cube 0: Measurement grid: dx=8mm, dy=8mm, dz=5mm

Power Drift = -0.04 dB

Peak SAR (extrapolated) = 19.1 W/kg

SAR(1 g) = 10.6 W/kg; SAR(10 g) = 5.63 W/kg

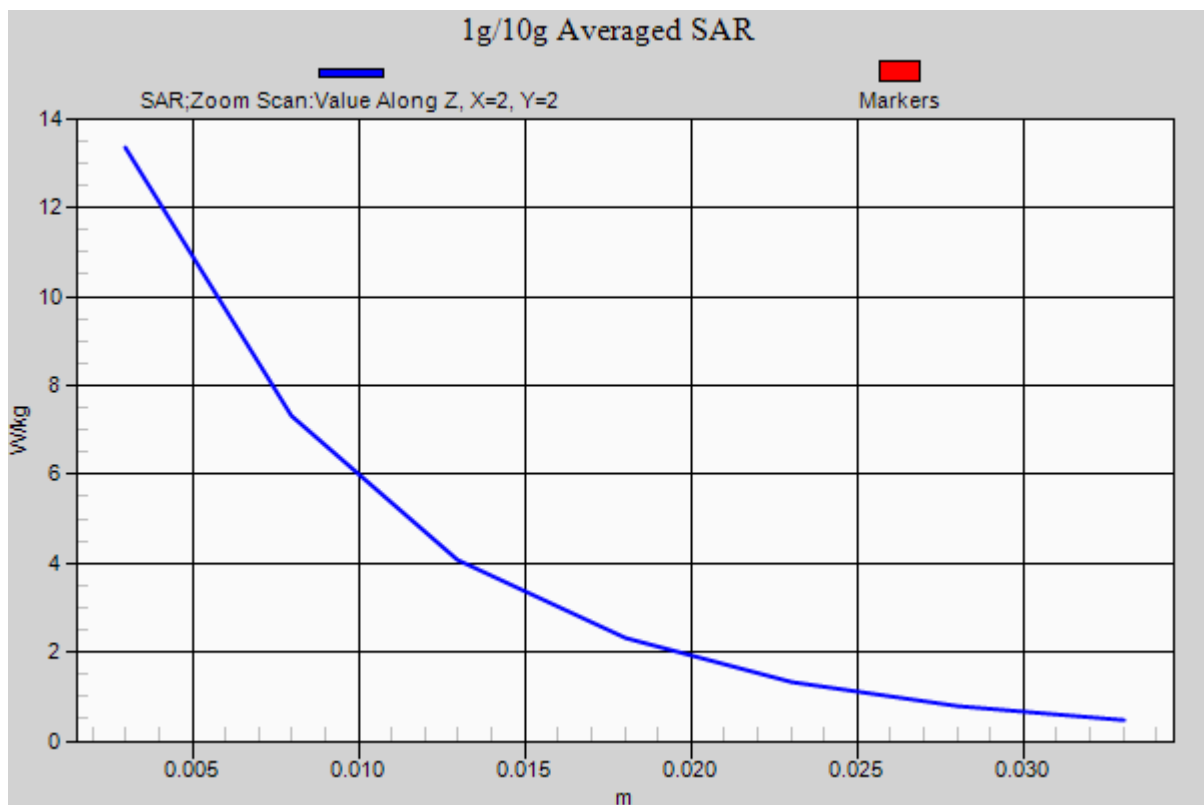

DT&C Co., Ltd.

DUT: Dipole 1900 MHz; Type: D1900V2; Serial: D1900V2 - SN:5d176

Communication System: CW (0); Frequency: 1900 MHz; Duty Cycle: 1:1
Medium parameters used: $f = 1900$ MHz; $\sigma = 1.568$ S/m; $\epsilon_r = 51.656$; $\rho = 1000$ kg/m³
Phantom section: Flat Section

DASY5 Configuration:

Probe: ES3DV3 - SN3328; ConvF(4.73, 4.73, 4.73); Calibrated: 3/18/2016; ; Electronics: DAE4 Sn1391
Phantom: SAM with CRP_2016_07_22_middle; Type: QD000P40CD; Serial: TP:1786
Measurement SW: DASY52, Version 52.8 (8); SEMCAD X Version 14.6.10 (7331)

Test Date: 2016-12-17; Ambient Temp: 20.8; Tissue Temp: 21.1

1900 MHz System Verification


Area Scan (5x7x1): Measurement grid: dx=15mm, dy=15mm

Zoom Scan (5x5x7)/Cube 0: Measurement grid: dx=8mm, dy=8mm, dz=5mm

Power Drift = -0.05 dB

Peak SAR (extrapolated) = 19.9 W/kg

SAR(1 g) = 10.2 W/kg; SAR(10 g) = 5.36 W/kg

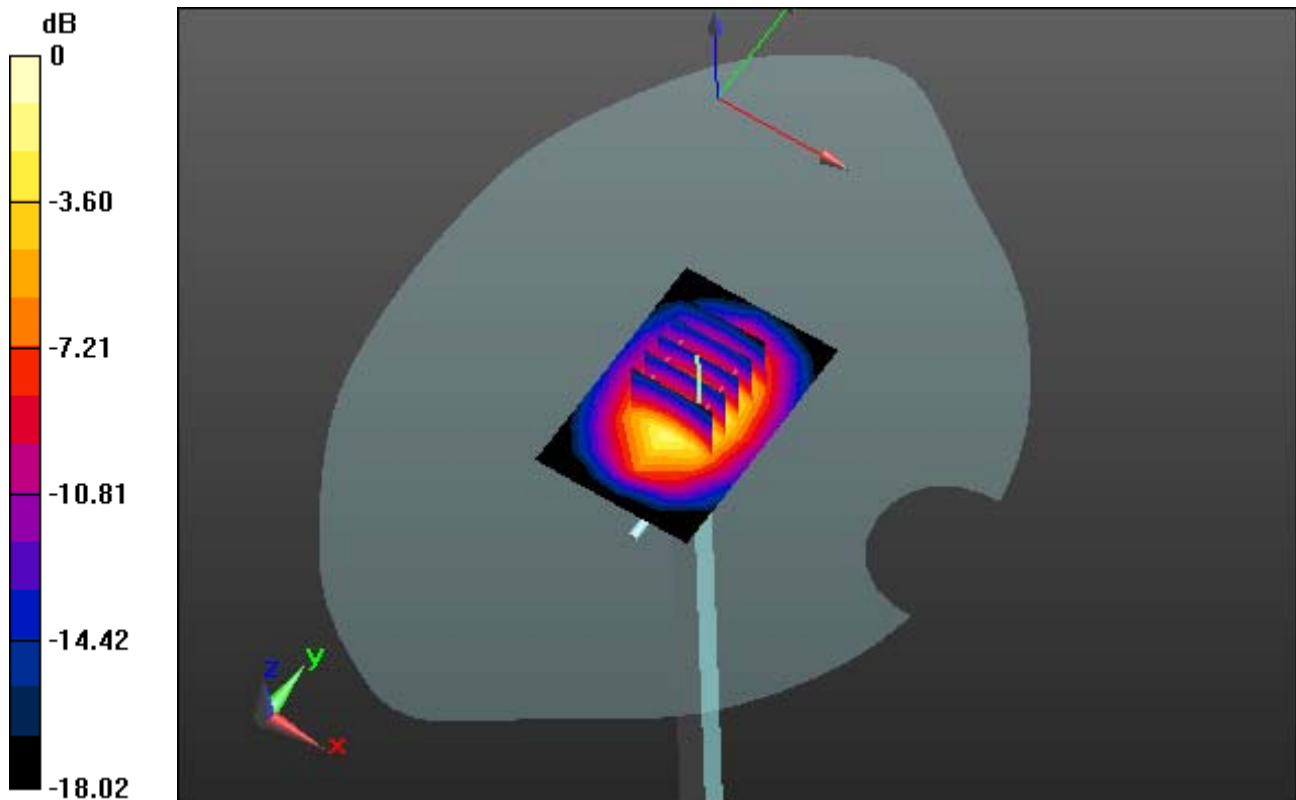

0 dB = 14.2 W/kg

DT&C Co., Ltd.

DUT: Dipole 1900 MHz; Type: D1900V2; Serial: D1900V2 - SN:5d176

Communication System: CW (0); Frequency: 1900 MHz; Duty Cycle: 1:1
Medium parameters used: $f = 1900$ MHz; $\sigma = 1.568$ S/m; $\epsilon_r = 51.656$; $\rho = 1000$ kg/m³
Phantom section: Flat Section

DASY5 Configuration:

Probe: ES3DV3 - SN3328; ConvF(4.73, 4.73, 4.73); Calibrated: 3/18/2016; ; Electronics: DAE4 Sn1391
Phantom: SAM with CRP_2016_07_22_middle; Type: QD000P40CD; Serial: TP:1786
Measurement SW: DASY52, Version 52.8 (8); SEMCAD X Version 14.6.10 (7331)

Test Date: 2016-12-17; Ambient Temp: 20.8; Tissue Temp: 21.1

1900 MHz System Verification


Area Scan (5x7x1): Measurement grid: dx=15mm, dy=15mm

Zoom Scan (5x5x7)/Cube 0: Measurement grid: dx=8mm, dy=8mm, dz=5mm

Power Drift = -0.05 dB

Peak SAR (extrapolated) = 19.9 W/kg

SAR(1 g) = 10.2 W/kg; SAR(10 g) = 5.36 W/kg

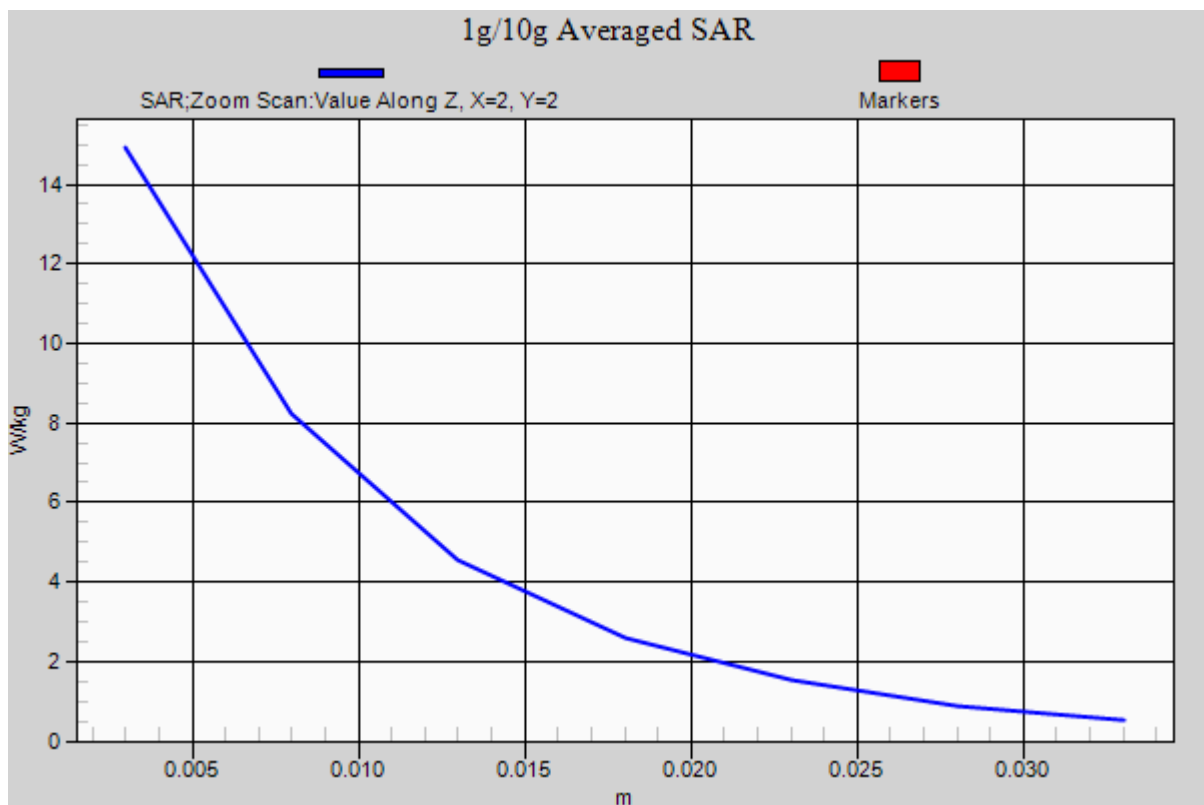

DT&C Co., Ltd.

DUT: Dipole 2450 MHz; Type: D2450V2; Serial: D2450V2 - SN:920

Communication System: CW (0); Frequency: 2450 MHz; Duty Cycle: 1:1
Medium parameters used: $f = 2450$ MHz; $\sigma = 1.824$ S/m; $\epsilon_r = 39.108$; $\rho = 1000$ kg/m³
Phantom section: Flat Section

DASY5 Configuration:

Probe: ES3DV3 - SN3328; ConvF(4.68, 4.68, 4.68); Calibrated: 3/18/2016; ; Electronics: DAE4 Sn1391
Phantom: SAM with CRP_2016_07_22_middle; Type: QD000P40CD; Serial: TP:1786
Measurement SW: DASY52, Version 52.8 (8); SEMCAD X Version 14.6.10 (7331)

Test Date: 2016-12-19; Ambient Temp: 20.4; Tissue Temp: 21.3

2450 MHz System Verification


Area Scan (7x10x1): Measurement grid: dx=10mm, dy=10mm

Zoom Scan (7x7x7)/Cube 0: Measurement grid: dx=5mm, dy=5mm, dz=5mm

Power Drift = -0.12 dB

Peak SAR (extrapolated) = 27.7 W/kg

SAR(1 g) = 13.3 W/kg; SAR(10 g) = 6.19 W/kg

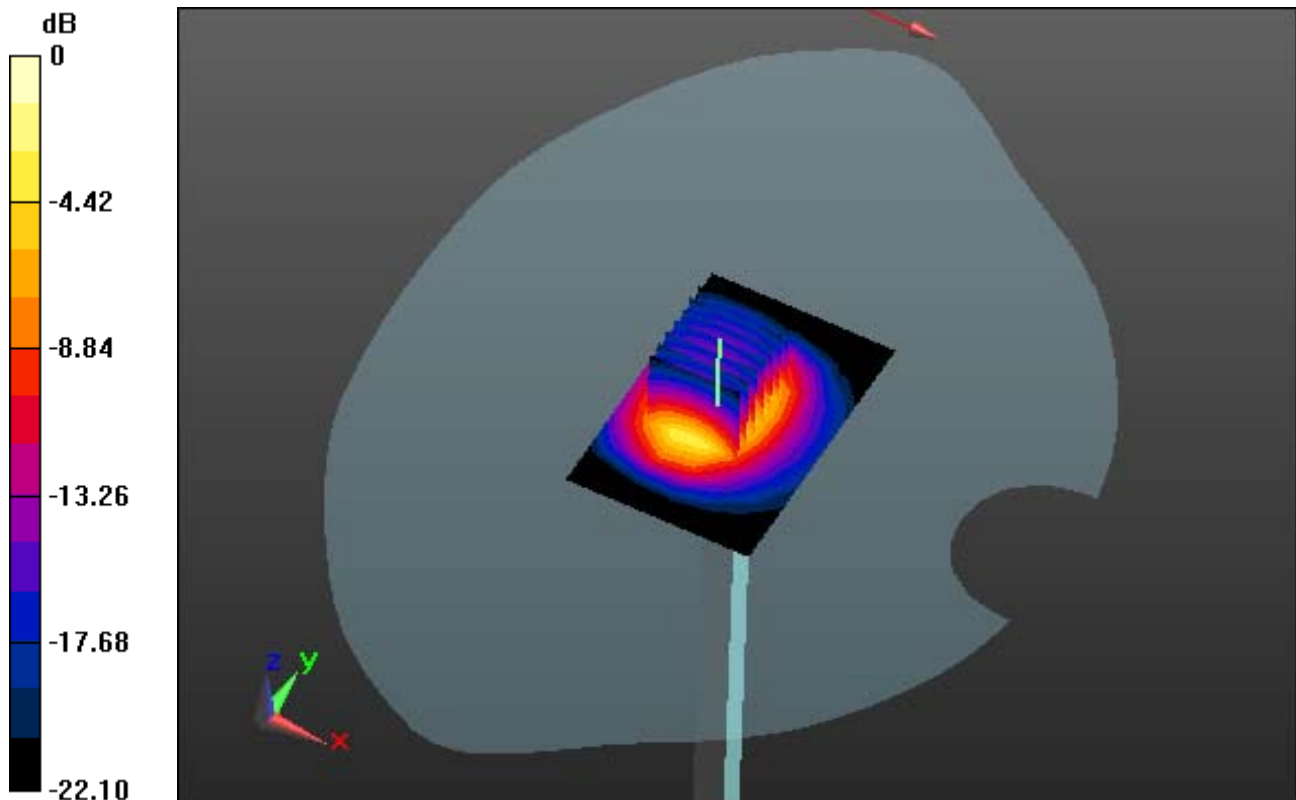

0 dB = 17.7 W/kg

DT&C Co., Ltd.

DUT: Dipole 2450 MHz; Type: D2450V2; Serial: D2450V2 - SN:920

Communication System: CW (0); Frequency: 2450 MHz; Duty Cycle: 1:1
Medium parameters used: $f = 2450$ MHz; $\sigma = 1.824$ S/m; $\epsilon_r = 39.108$; $\rho = 1000$ kg/m³
Phantom section: Flat Section

DASY5 Configuration:

Probe: ES3DV3 - SN3328; ConvF(4.68, 4.68, 4.68); Calibrated: 3/18/2016; ; Electronics: DAE4 Sn1391
Phantom: SAM with CRP_2016_07_22_middle; Type: QD000P40CD; Serial: TP:1786
Measurement SW: DASY52, Version 52.8 (8); SEMCAD X Version 14.6.10 (7331)

Test Date: 2016-12-19; Ambient Temp: 20.4; Tissue Temp: 21.3

2450 MHz System Verification


Area Scan (7x10x1): Measurement grid: dx=10mm, dy=10mm

Zoom Scan (7x7x7)/Cube 0: Measurement grid: dx=5mm, dy=5mm, dz=5mm

Power Drift = -0.12 dB

Peak SAR (extrapolated) = 27.7 W/kg

SAR(1 g) = 13.3 W/kg; SAR(10 g) = 6.19 W/kg

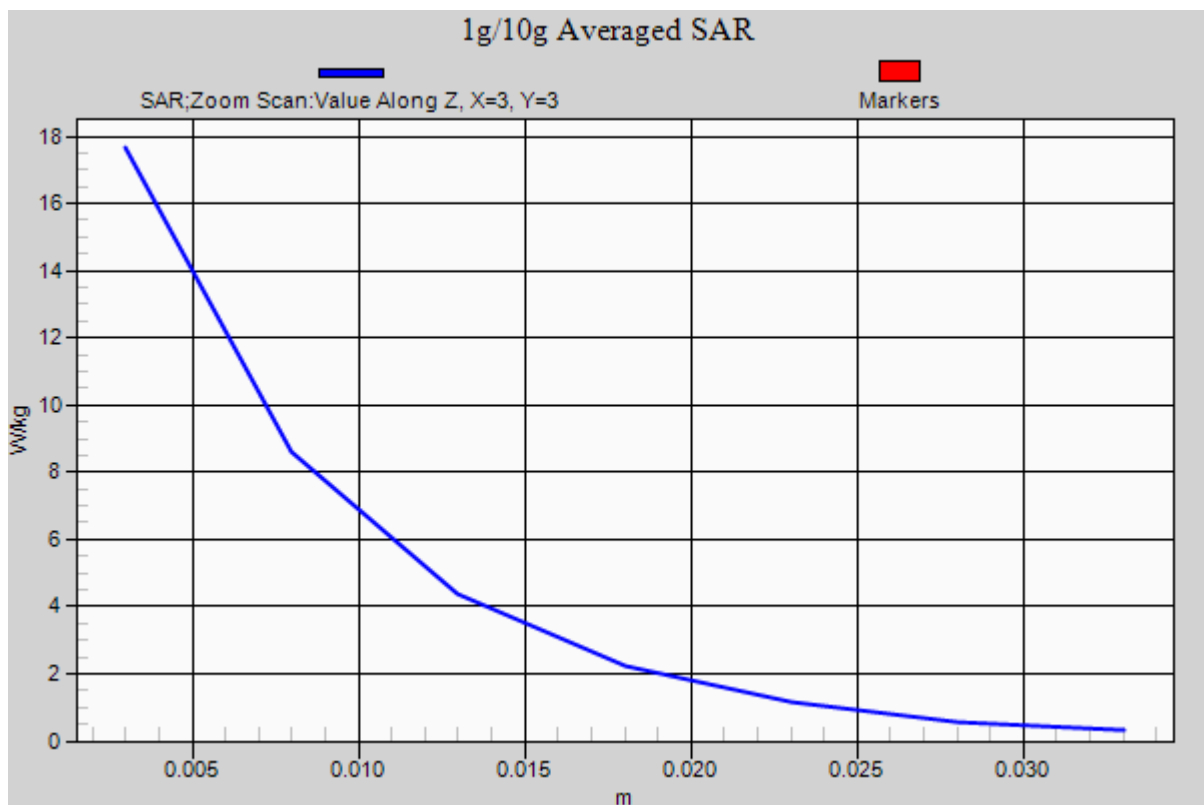

DT&C Co., Ltd.

DUT: Dipole 2450 MHz; Type: D2450V2; Serial: D2450V2 - SN:920

Communication System: CW; Frequency: 2450 MHz; Duty Cycle: 1:1
Medium parameters used: $f = 2450$ MHz; $\sigma = 1.935$ S/m; $\epsilon_r = 51.081$; $\rho = 1000$ kg/m³
Phantom section: Flat Section

DASY5 Configuration:

Probe: ES3DV3 - SN3328; ConvF(4.4, 4.4, 4.4); Calibrated: 3/18/2016; ; Electronics: DAE4 Sn1391
Phantom: SAM with CRP_2016_07_22_middle; Type: QD000P40CD; Serial: TP:1786
Measurement SW: DASY52, Version 52.8 (8); SEMCAD X Version 14.6.10 (7331)

Test Date: 2016-12-19; Ambient Temp: 20.4; Tissue Temp: 21.0

2450 MHz System Verification


Area Scan (7x10x1): Measurement grid: dx=10mm, dy=10mm

Zoom Scan (7x7x7)/Cube 0: Measurement grid: dx=5mm, dy=5mm, dz=5mm

Power Drift = 0.02 dB

Peak SAR (extrapolated) = 23.3 W/kg

SAR(1 g) = 11.9 W/kg; SAR(10 g) = 5.63 W/kg

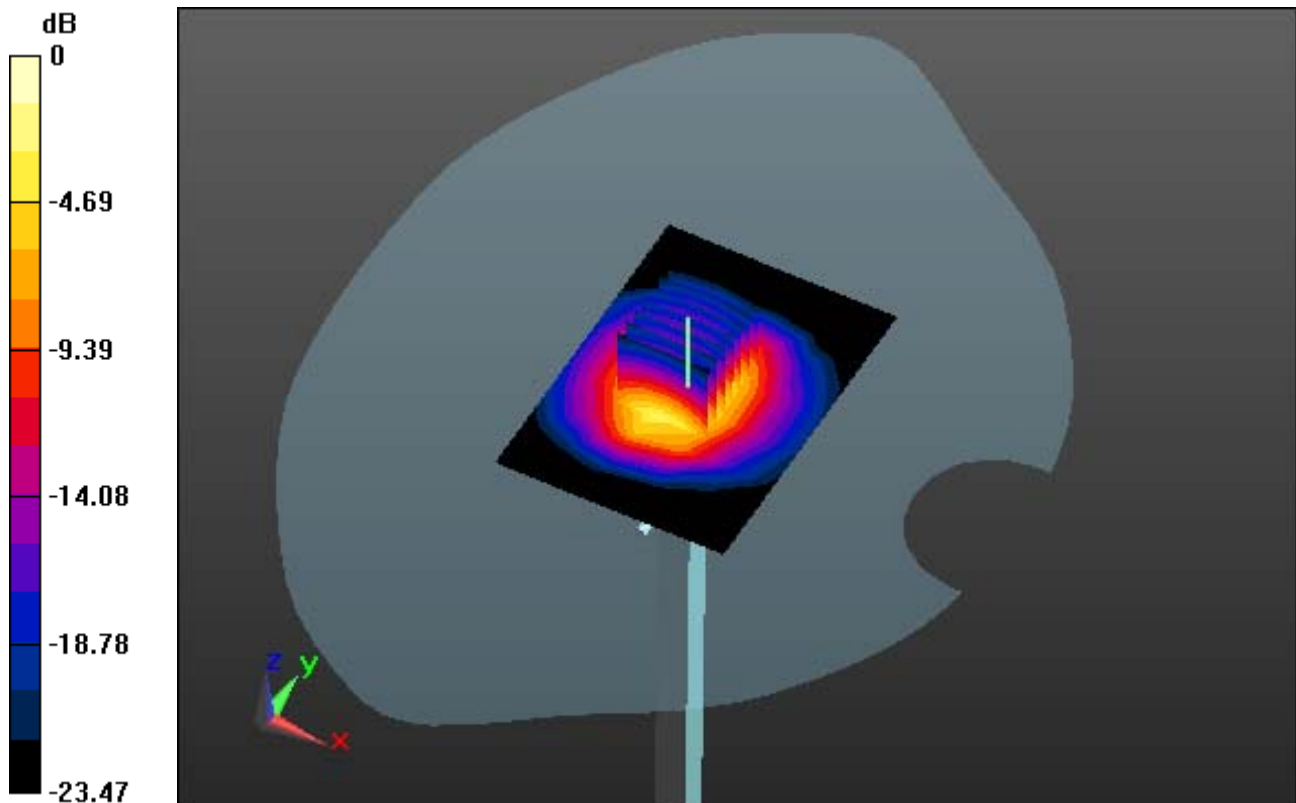

0 dB = 16.4 W/kg

DT&C Co., Ltd.

DUT: Dipole 2450 MHz; Type: D2450V2; Serial: D2450V2 - SN:920

Communication System: CW; Frequency: 2450 MHz; Duty Cycle: 1:1

Medium parameters used: $f = 2450$ MHz; $\sigma = 1.935$ S/m; $\epsilon_r = 51.081$; $\rho = 1000$ kg/m³

Phantom section: Flat Section

DASY5 Configuration:

Probe: ES3DV3 - SN3328; ConvF(4.4, 4.4, 4.4); Calibrated: 3/18/2016; ; Electronics: DAE4 Sn1391

Phantom: SAM with CRP_2016_07_22_middle; Type: QD000P40CD; Serial: TP:1786

Measurement SW: DASY52, Version 52.8 (8); SEMCAD X Version 14.6.10 (7331)

Test Date: 2016-12-19; Ambient Temp: 20.4; Tissue Temp: 21.0

2450 MHz System Verification


Area Scan (7x10x1): Measurement grid: dx=10mm, dy=10mm

Zoom Scan (7x7x7)/Cube 0: Measurement grid: dx=5mm, dy=5mm, dz=5mm

Power Drift = 0.02 dB

Peak SAR (extrapolated) = 23.3 W/kg

SAR(1 g) = 11.9 W/kg; SAR(10 g) = 5.63 W/kg

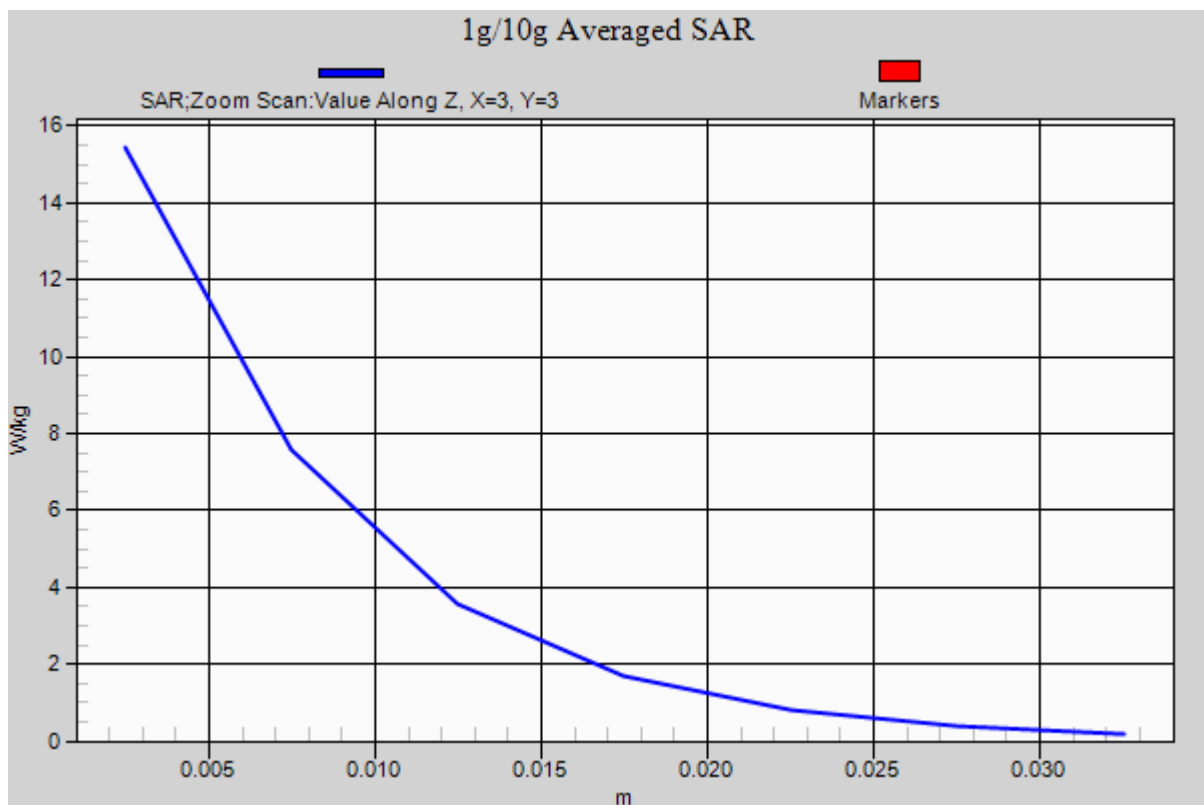

DT&C Co., Ltd.

DUT: YKDA25; Type: Bar

Communication System: PCS 1900 (0); Frequency: 1880 MHz; Duty Cycle: 1:8.3
Medium parameters used: $f = 1880$ MHz; $\sigma = 1.413$ S/m; $\epsilon_r = 40.652$; $\rho = 1000$ kg/m³
Phantom section: Left Section

DASY5 Configuration:

Probe: ES3DV3 - SN3328; ConvF(5.19, 5.19, 5.19); Calibrated: 3/18/2016; Electronics: DAE4 Sn1391
Phantom: SAM with CRP_2016_07_22_middle; Type: QD000P40CD; Serial: TP:1786
Measurement SW: DASY52, Version 52.8 (8); SEMCAD X Version 14.6.10 (7331)

Test Date: 2016-12-17; Ambient Temp: 20.8; Tissue Temp: 21.3

Left Touch, PCS1900 Ch. 661, Ant Internal, Standard Battery


Area Scan (9x13x1): Measurement grid: dx=15mm, dy=15mm

Zoom Scan (5x5x7)/Cube 0: Measurement grid: dx=8mm, dy=8mm, dz=5mm

Power Drift = 0.16 dB

Peak SAR (extrapolated) = 0.491 W/kg

SAR(1 g) = 0.317 W/kg; SAR(10 g) = 0.195 W/kg

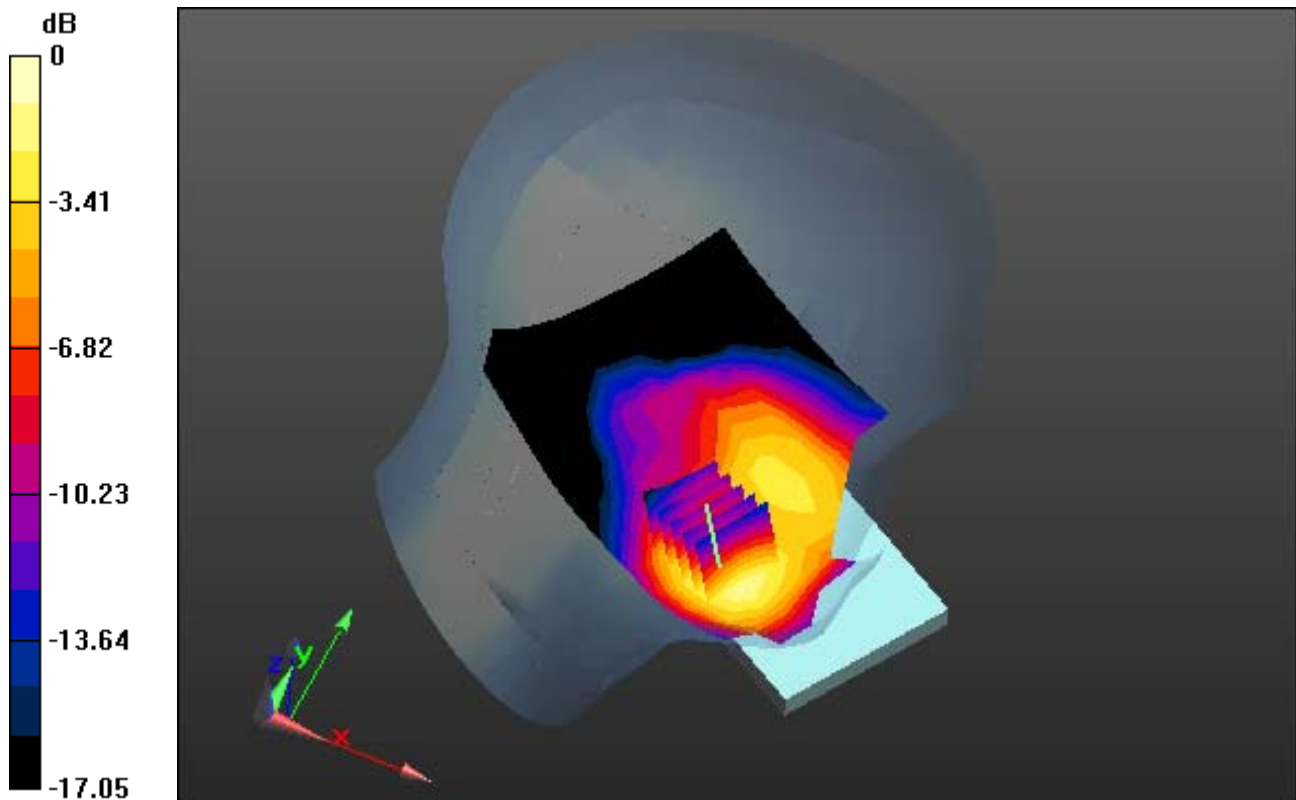

0 dB = 0.378 W/kg

DT&C Co., Ltd.

DUT: YKDA25; Type: Bar

Communication System: PCS 1900 (0); Frequency: 1880 MHz; Duty Cycle: 1:8.3
Medium parameters used: $f = 1880$ MHz; $\sigma = 1.413$ S/m; $\epsilon_r = 40.652$; $\rho = 1000$ kg/m³
Phantom section: Left Section

DASY5 Configuration:

Probe: ES3DV3 - SN3328; ConvF(5.19, 5.19, 5.19); Calibrated: 3/18/2016; Electronics: DAE4 Sn1391
Phantom: SAM with CRP_2016_07_22_middle; Type: QD000P40CD; Serial: TP:1786
Measurement SW: DASY52, Version 52.8 (8); SEMCAD X Version 14.6.10 (7331)

Test Date: 2016-12-17; Ambient Temp: 20.8; Tissue Temp: 21.3

Left Touch, PCS1900 Ch. 661, Ant Internal, Standard Battery

With Enlarge Plot image


Area Scan (9x13x1): Measurement grid: dx=15mm, dy=15mm

Zoom Scan (5x5x7)/Cube 0: Measurement grid: dx=8mm, dy=8mm, dz=5mm

Power Drift = 0.16 dB

Peak SAR (extrapolated) = 0.491 W/kg

SAR(1 g) = 0.317 W/kg; SAR(10 g) = 0.195 W/kg

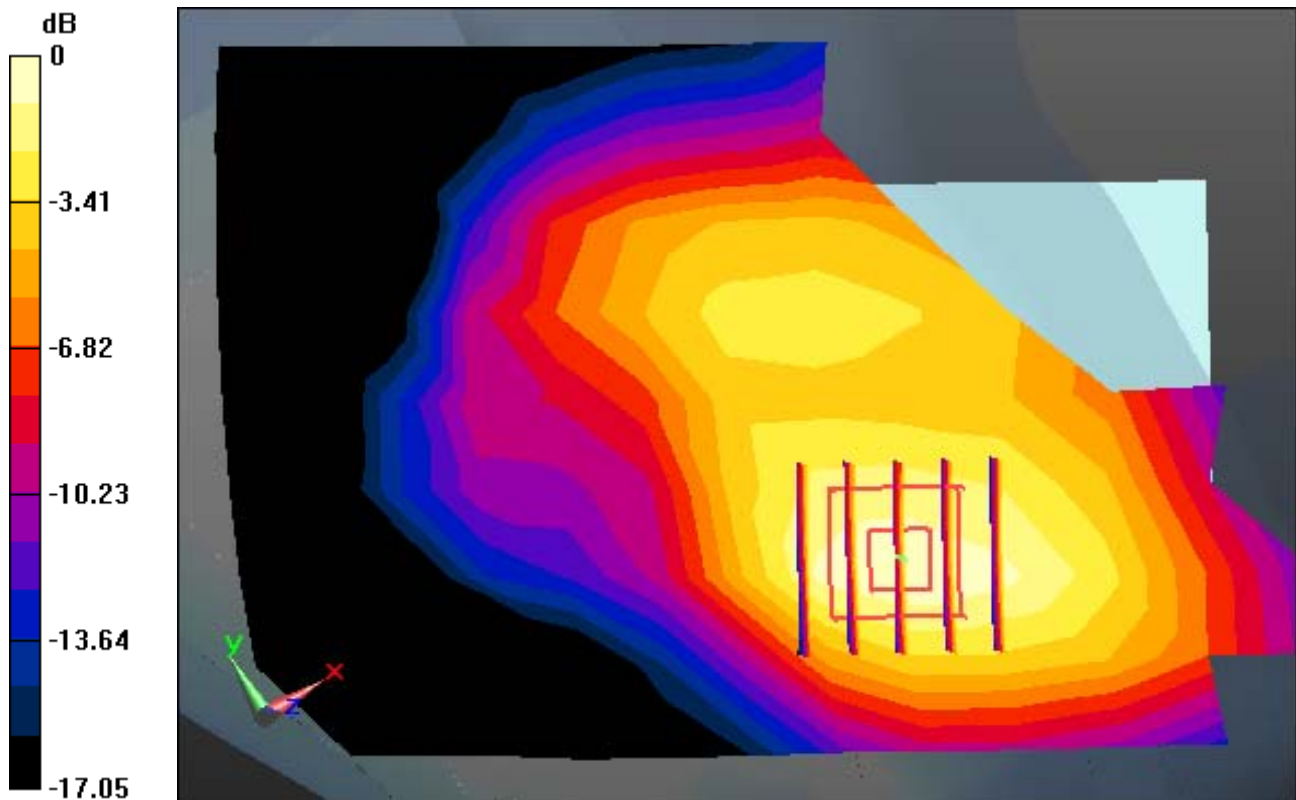

0 dB = 0.378 W/kg

A1

DT&C Co., Ltd.

DUT: YKDA25; Type: Bar

Communication System: PCS 1900 (0); Frequency: 1880 MHz; Duty Cycle: 1:8.3
Medium parameters used: $f = 1880$ MHz; $\sigma = 1.413$ S/m; $\epsilon_r = 40.652$; $\rho = 1000$ kg/m³
Phantom section: Left Section

DASY5 Configuration:

Probe: ES3DV3 - SN3328; ConvF(5.19, 5.19, 5.19); Calibrated: 3/18/2016; Electronics: DAE4 Sn1391
Phantom: SAM with CRP_2016_07_22_middle; Type: QD000P40CD; Serial: TP:1786
Measurement SW: DASY52, Version 52.8 (8); SEMCAD X Version 14.6.10 (7331)

Test Date: 2016-12-17; Ambient Temp: 20.8; Tissue Temp: 21.3

Left Touch, PCS1900 Ch. 661, Ant Internal, Standard Battery


Area Scan (9x13x1): Measurement grid: dx=15mm, dy=15mm

Zoom Scan (5x5x7)/Cube 0: Measurement grid: dx=8mm, dy=8mm, dz=5mm

Power Drift = 0.16 dB

Peak SAR (extrapolated) = 0.491 W/kg

SAR(1 g) = 0.317 W/kg; SAR(10 g) = 0.195 W/kg

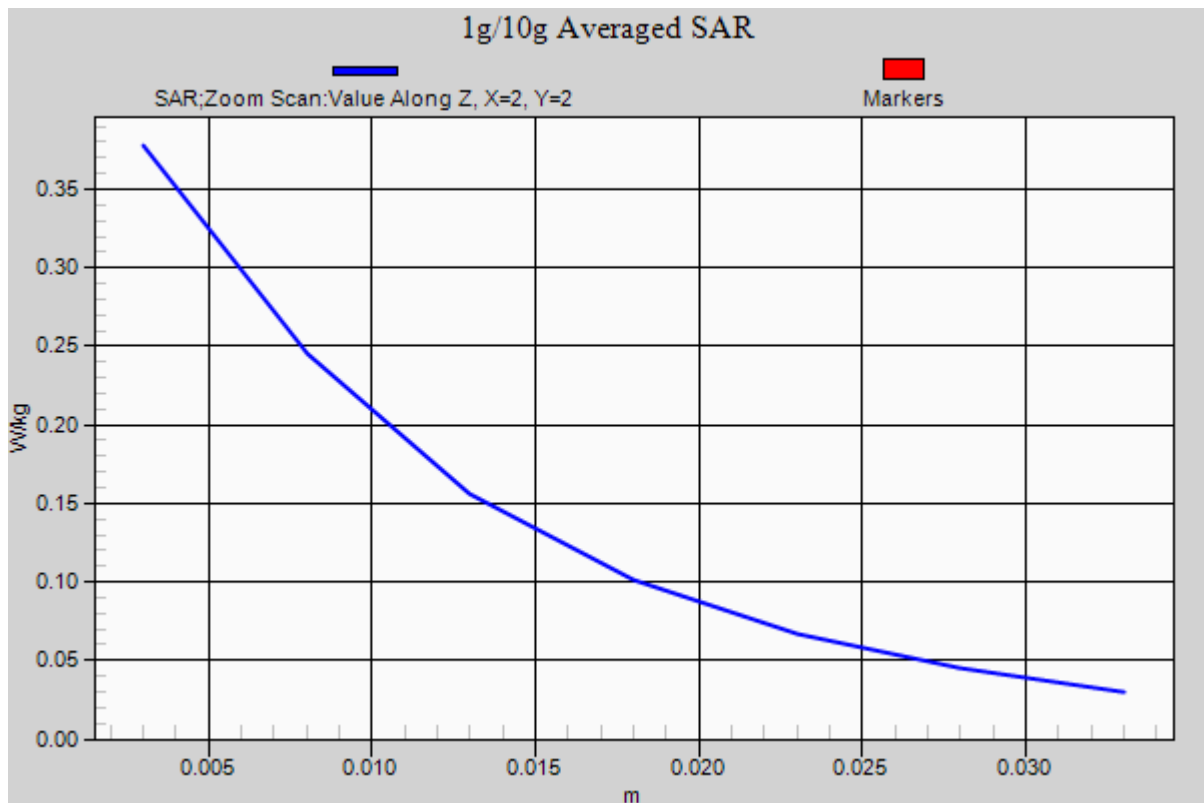

DT&C Co., Ltd.

DUT: YKDA25; Type: Bar

Communication System: PCS1900_Class 10 (0); Frequency: 1880 MHz; Duty Cycle: 1:4.15

Medium parameters used: $f = 1880 \text{ MHz}$; $\sigma = 1.413 \text{ S/m}$; $\epsilon_r = 40.652$; $\rho = 1000 \text{ kg/m}^3$

Phantom section: Left Section

DASY5 Configuration:

Probe: ES3DV3 - SN3328; ConvF(5.19, 5.19, 5.19); Calibrated: 3/18/2016; Electronics: DAE4 Sn1391

Phantom: SAM with CRP_2016_07_22_middle; Type: QD000P40CD; Serial: TP:1786

Measurement SW: DASY52, Version 52.8 (8); SEMCAD X Version 14.6.10 (7331)

Test Date: 2016-12-17; Ambient Temp: 20.8; Tissue Temp: 21.3

Left Touch, PCS1900 GPRS 2Tx Ch. 661, Ant Internal, Standard Battery


Area Scan (9x13x1): Measurement grid: $dx=15\text{mm}$, $dy=15\text{mm}$

Zoom Scan (5x5x7)/Cube 0: Measurement grid: $dx=8\text{mm}$, $dy=8\text{mm}$, $dz=5\text{mm}$

Power Drift = 0.15 dB

Peak SAR (extrapolated) = 0.969 W/kg

SAR(1 g) = 0.453 W/kg; SAR(10 g) = 0.278 W/kg

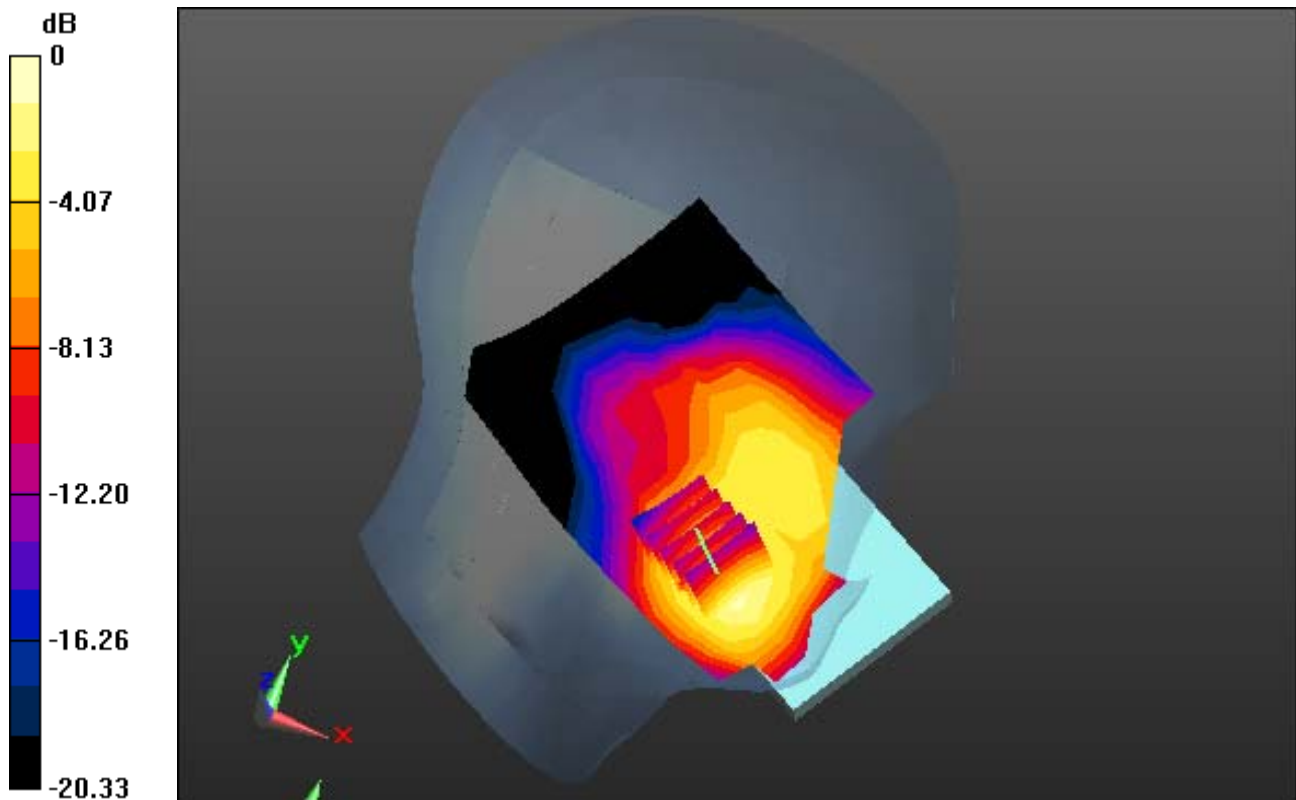

0 dB = 0.544 W/kg

DT&C Co., Ltd.

DUT: YKDA25; Type: Bar

Communication System: PCS1900_Class 10 (0); Frequency: 1880 MHz; Duty Cycle: 1:4.15

Medium parameters used: $f = 1880$ MHz; $\sigma = 1.413$ S/m; $\epsilon_r = 40.652$; $\rho = 1000$ kg/m³

Phantom section: Left Section

DASY5 Configuration:

Probe: ES3DV3 - SN3328; ConvF(5.19, 5.19, 5.19); Calibrated: 3/18/2016; Electronics: DAE4 Sn1391

Phantom: SAM with CRP_2016_07_22_middle; Type: QD000P40CD; Serial: TP:1786

Measurement SW: DASY52, Version 52.8 (8); SEMCAD X Version 14.6.10 (7331)

Test Date: 2016-12-17; Ambient Temp: 20.8; Tissue Temp: 21.3

Left Touch, PCS1900 GPRS 2Tx Ch. 661, Ant Internal, Standard Battery

With Enlarge Plot image


Area Scan (9x13x1): Measurement grid: dx=15mm, dy=15mm

Zoom Scan (5x5x7)/Cube 0: Measurement grid: dx=8mm, dy=8mm, dz=5mm

Power Drift = 0.15 dB

Peak SAR (extrapolated) = 0.969 W/kg

SAR(1 g) = 0.453 W/kg; SAR(10 g) = 0.278 W/kg

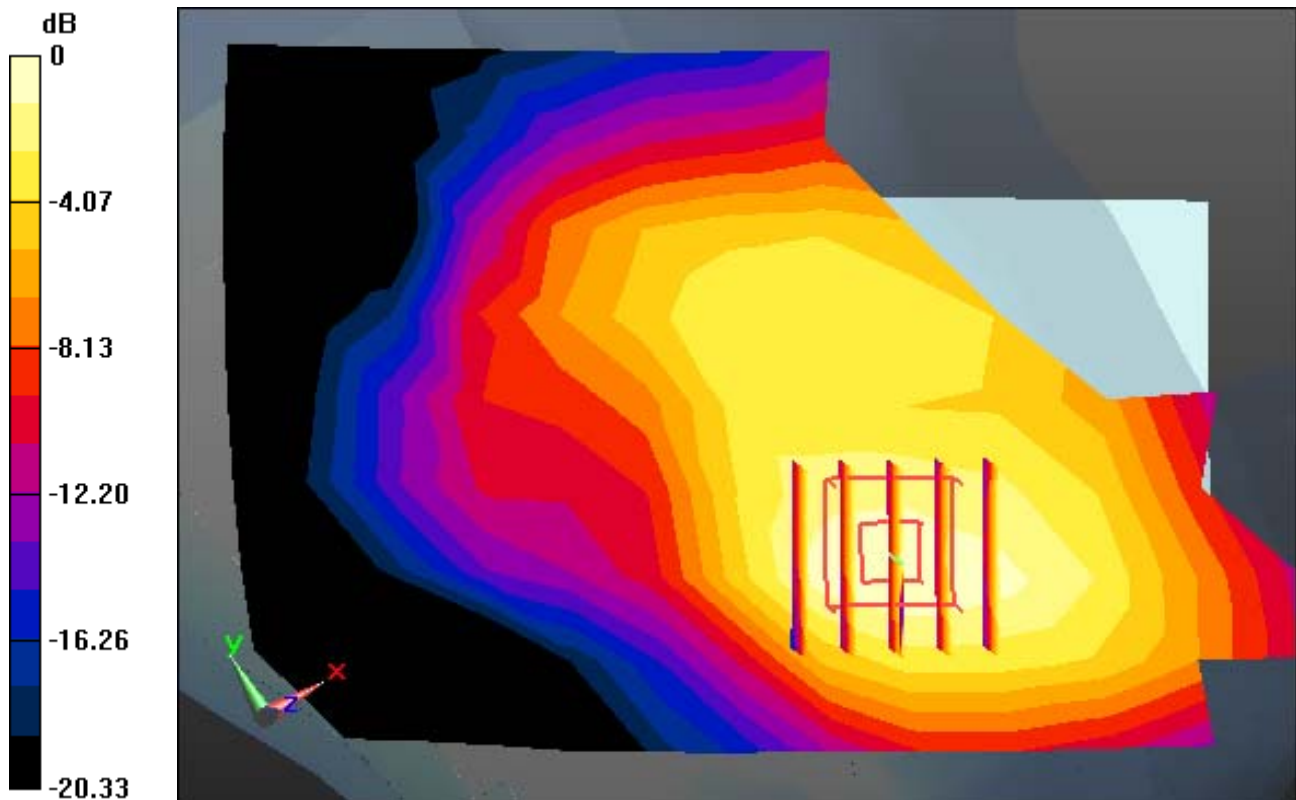

0 dB = 0.544 W/kg

A2

DT&C Co., Ltd.

DUT: YKDA25; Type: Bar

Communication System: PCS1900_Class 10 (0); Frequency: 1880 MHz; Duty Cycle: 1:4.15

Medium parameters used: $f = 1880$ MHz; $\sigma = 1.413$ S/m; $\epsilon_r = 40.652$; $\rho = 1000$ kg/m³

Phantom section: Left Section

DASY5 Configuration:

Probe: ES3DV3 - SN3328; ConvF(5.19, 5.19, 5.19); Calibrated: 3/18/2016; Electronics: DAE4 Sn1391

Phantom: SAM with CRP_2016_07_22_middle; Type: QD000P40CD; Serial: TP:1786

Measurement SW: DASY52, Version 52.8 (8); SEMCAD X Version 14.6.10 (7331)

Test Date: 2016-12-17; Ambient Temp: 20.8; Tissue Temp: 21.3

Left Touch, PCS1900 GPRS 2Tx Ch. 661, Ant Internal, Standard Battery


Area Scan (9x13x1): Measurement grid: dx=15mm, dy=15mm

Zoom Scan (5x5x7)/Cube 0: Measurement grid: dx=8mm, dy=8mm, dz=5mm

Power Drift = 0.15 dB

Peak SAR (extrapolated) = 0.969 W/kg

SAR(1 g) = 0.453 W/kg; SAR(10 g) = 0.278 W/kg

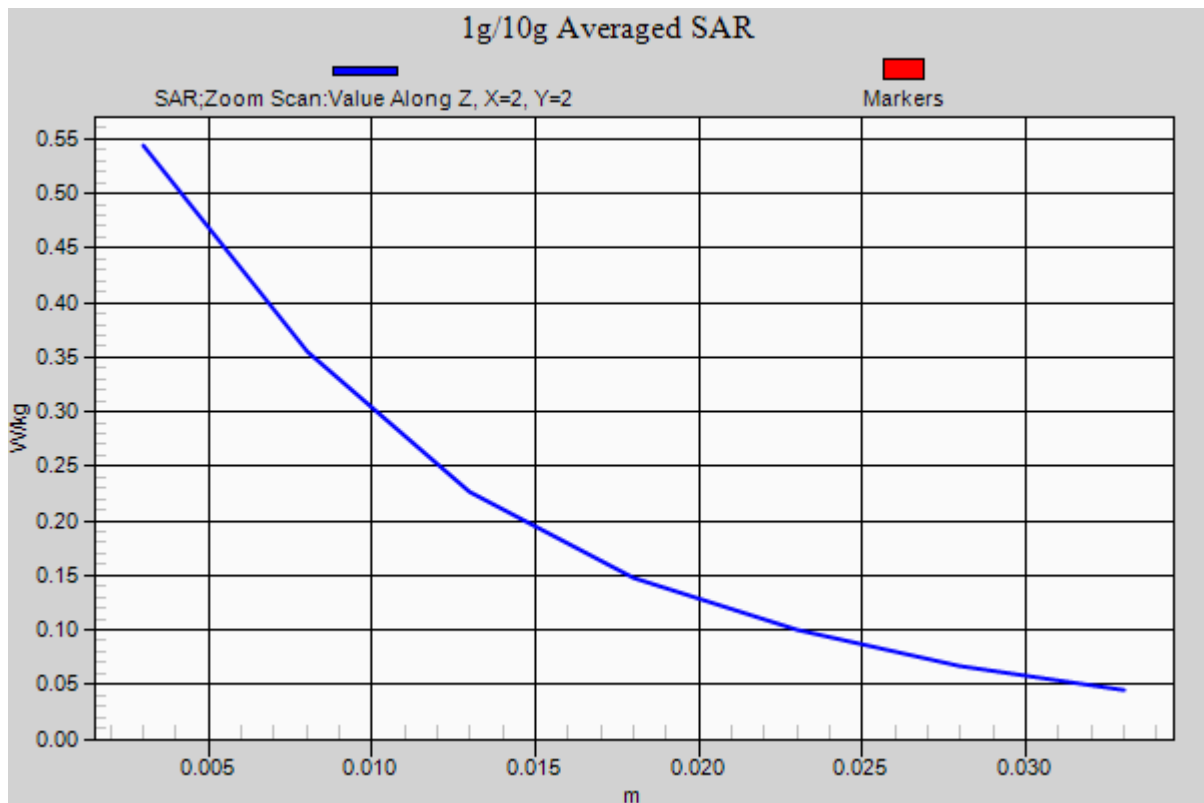

DT&C Co., Ltd.

DUT: YKDA25; Type: Bar

Communication System: W-LAN (0); Frequency: 2412 MHz; Duty Cycle: 1:1
Medium parameters used: $f = 2412 \text{ MHz}$; $\sigma = 1.782 \text{ S/m}$; $\epsilon_r = 39.221$; $\rho = 1000 \text{ kg/m}^3$
Phantom section: Right Section

DASY5 Configuration:

Probe: ES3DV3 - SN3328; ConvF(4.68, 4.68, 4.68); Calibrated: 3/18/2016; Electronics: DAE4 Sn1391
Phantom: SAM with CRP_2016_07_22_middle; Type: QD000P40CD; Serial: TP:1786
Measurement SW: DASY52, Version 52.8 (8); SEMCAD X Version 14.6.10 (7331)

Test Date: 2016-12-19; Ambient Temp: 20.4; Tissue Temp: 21.3

Right Touch, W-LAN(802.11b) Ch. 1, Ant Internal, Standard Battery


Area Scan (11x16x1): Measurement grid: $dx=12\text{mm}$, $dy=12\text{mm}$

Zoom Scan (7x7x7)/Cube 0: Measurement grid: $dx=5\text{mm}$, $dy=5\text{mm}$, $dz=5\text{mm}$

Power Drift = 0.10 dB

Peak SAR (extrapolated) = 0.879 W/kg

SAR(1 g) = 0.365 W/kg; SAR(10 g) = 0.165 W/kg

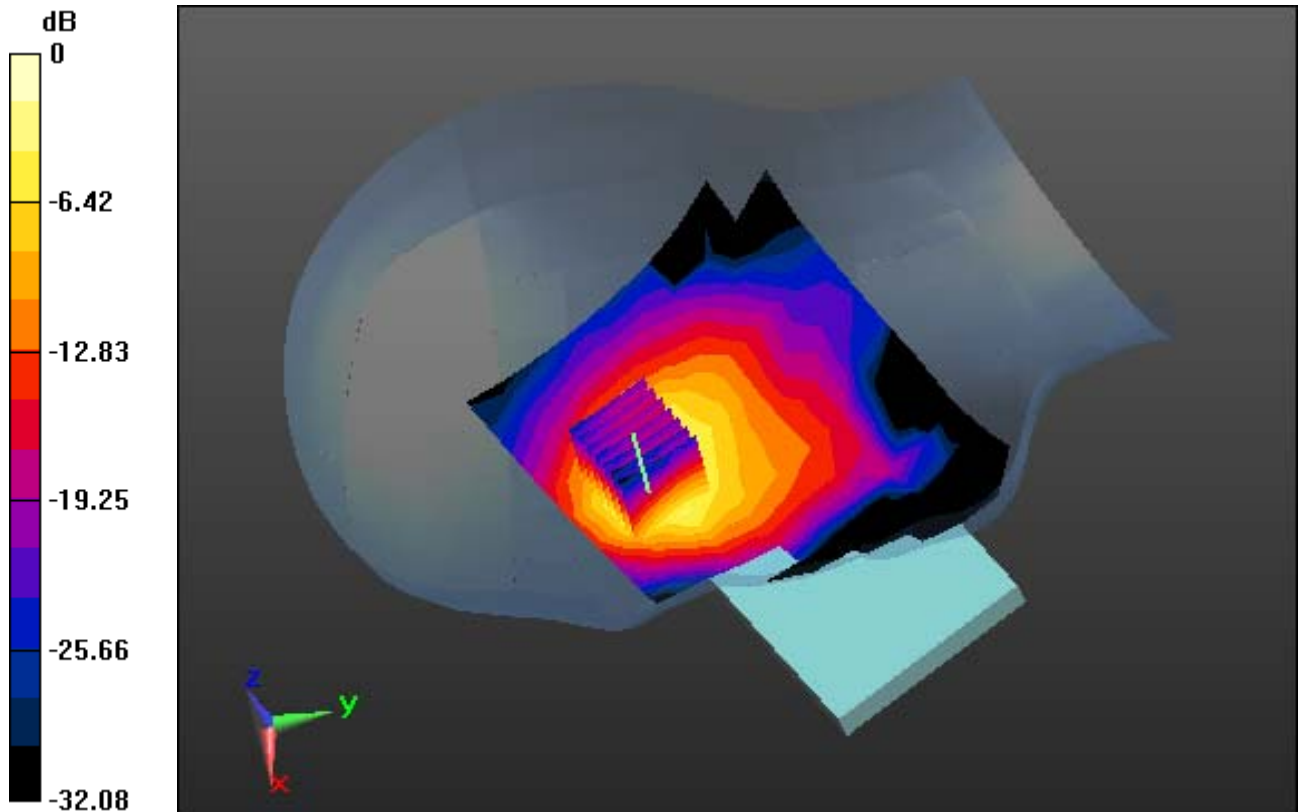

0 dB = 0.493 W/kg

DT&C Co., Ltd.

DUT: YKDA25; Type: Bar

Communication System: W-LAN (0); Frequency: 2412 MHz; Duty Cycle: 1:1
Medium parameters used: $f = 2412 \text{ MHz}$; $\sigma = 1.782 \text{ S/m}$; $\epsilon_r = 39.221$; $\rho = 1000 \text{ kg/m}^3$
Phantom section: Right Section

DASY5 Configuration:

Probe: ES3DV3 - SN3328; ConvF(4.68, 4.68, 4.68); Calibrated: 3/18/2016; Electronics: DAE4 Sn1391
Phantom: SAM with CRP_2016_07_22_middle; Type: QD000P40CD; Serial: TP:1786
Measurement SW: DASY52, Version 52.8 (8); SEMCAD X Version 14.6.10 (7331)

Test Date: 2016-12-19; Ambient Temp: 20.4; Tissue Temp: 21.3

Right Touch, W-LAN(802.11b) Ch. 1, Ant Internal, Standard Battery

With Enlarge Plot image


Area Scan (11x16x1): Measurement grid: $dx=12\text{mm}$, $dy=12\text{mm}$

Zoom Scan (7x7x7)/Cube 0: Measurement grid: $dx=5\text{mm}$, $dy=5\text{mm}$, $dz=5\text{mm}$

Power Drift = 0.10 dB

Peak SAR (extrapolated) = 0.879 W/kg

SAR(1 g) = 0.365 W/kg; SAR(10 g) = 0.165 W/kg

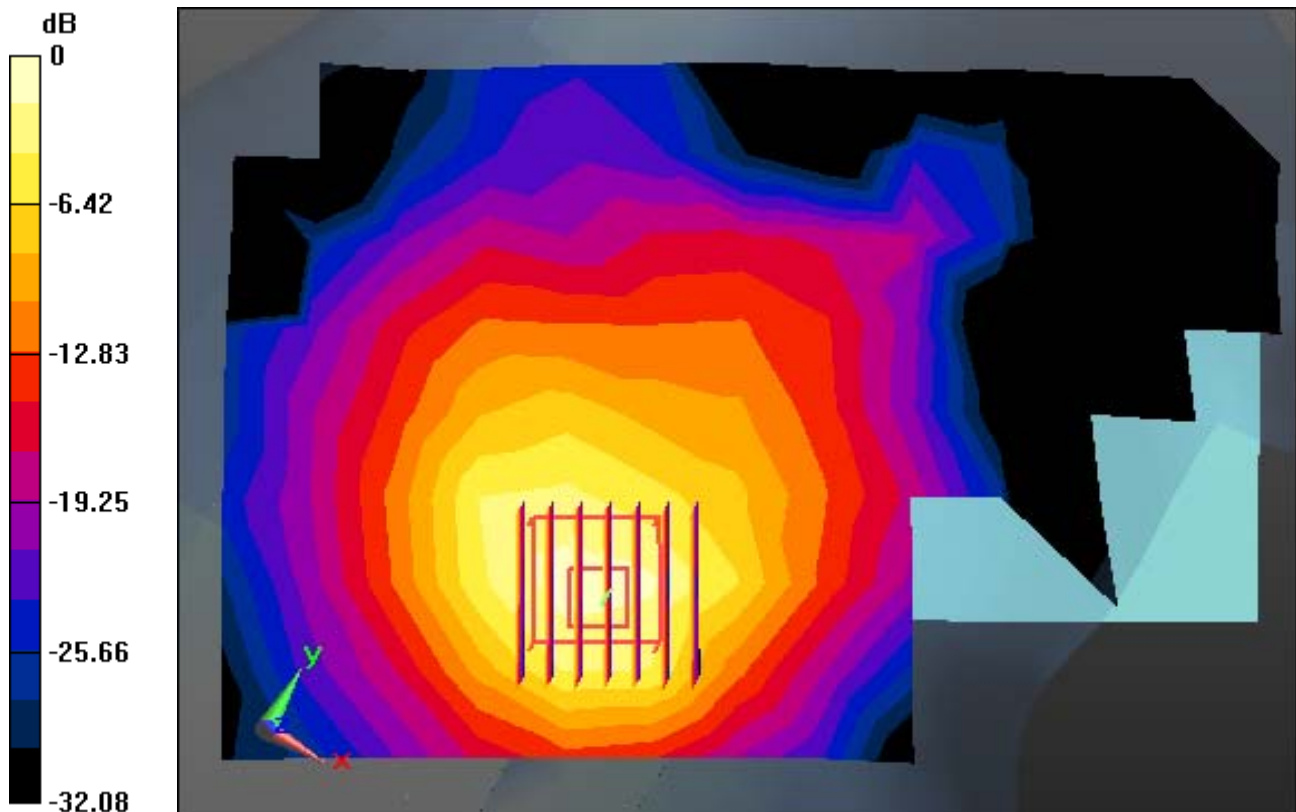

0 dB = 0.493 W/kg

DT&C Co., Ltd.

DUT: YKDA25; Type: Bar

Communication System: W-LAN (0); Frequency: 2412 MHz; Duty Cycle: 1:1
Medium parameters used: $f = 2412$ MHz; $\sigma = 1.782$ S/m; $\epsilon_r = 39.221$; $\rho = 1000$ kg/m³
Phantom section: Right Section

DASY5 Configuration:

Probe: ES3DV3 - SN3328; ConvF(4.68, 4.68, 4.68); Calibrated: 3/18/2016; Electronics: DAE4 Sn1391
Phantom: SAM with CRP_2016_07_22_middle; Type: QD000P40CD; Serial: TP:1786
Measurement SW: DASY52, Version 52.8 (8); SEMCAD X Version 14.6.10 (7331)

Test Date: 2016-12-19; Ambient Temp: 20.4; Tissue Temp: 21.3

Right Touch, W-LAN(802.11b) Ch. 1, Ant Internal, Standard Battery


Area Scan (11x16x1): Measurement grid: dx=12mm, dy=12mm

Zoom Scan (7x7x7)/Cube 0: Measurement grid: dx=5mm, dy=5mm, dz=5mm

Power Drift = 0.10 dB

Peak SAR (extrapolated) = 0.879 W/kg

SAR(1 g) = 0.365 W/kg; SAR(10 g) = 0.165 W/kg

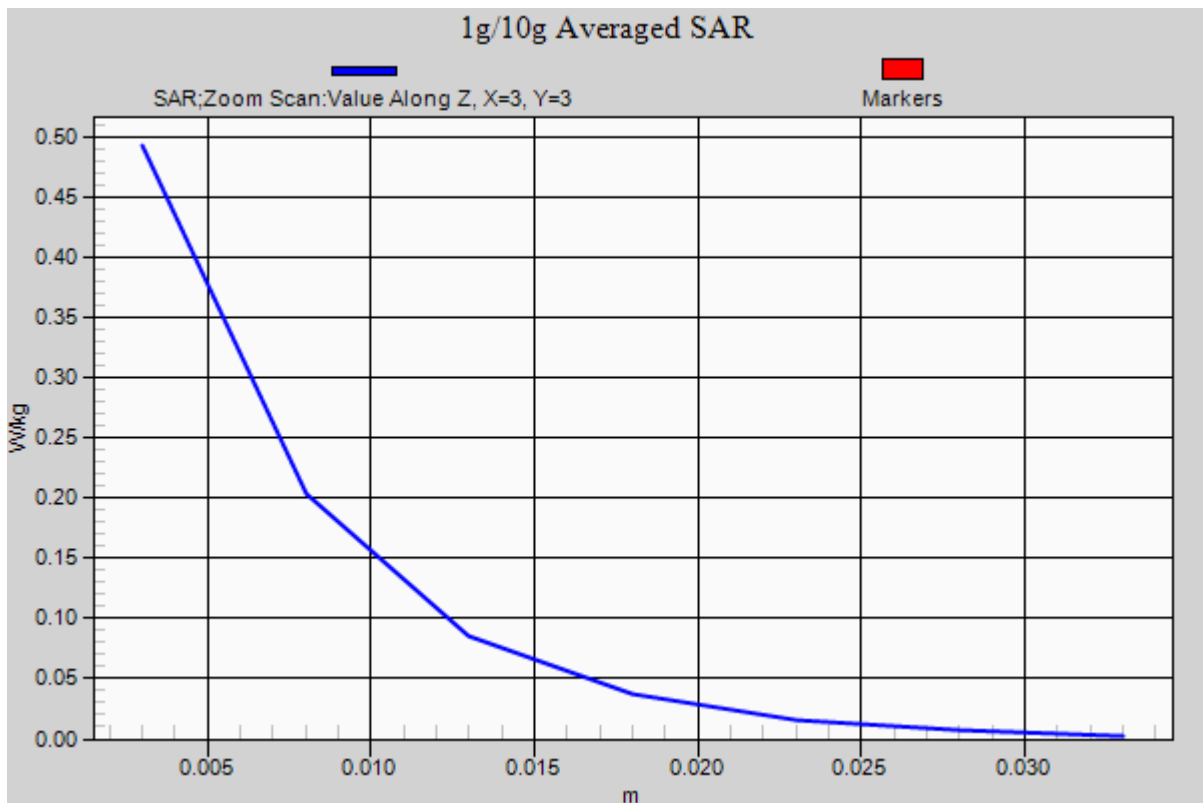

DT&C Co., Ltd.

DUT: YKDA25; Type: Bar

Communication System: PCS 1900 (0); Frequency: 1880 MHz; Duty Cycle: 1:8.3
Medium parameters used: $f = 1880$ MHz; $\sigma = 1.552$ S/m; $\epsilon_r = 51.696$; $\rho = 1000$ kg/m³
Phantom section: Flat Section

DASY5 Configuration:

Probe: ES3DV3 - SN3328; ConvF(4.73, 4.73, 4.73); Calibrated: 3/18/2016; Electronics: DAE4 Sn1391
Phantom: SAM with CRP_2016_07_22_middle; Type: QD000P40CD; Serial: TP:1786
Measurement SW: DASY52, Version 52.8 (8); SEMCAD X Version 14.6.10 (7331)

Test Date: 2016-12-17; Ambient Temp; 20.8; Tissue Temp: 21.1

1cm space from Body, Rear, PCS1900 Ch. 661, Ant Internal


Area Scan (9x13x1): Measurement grid: dx=15mm, dy=15mm

Zoom Scan (5x5x7)/Cube 0: Measurement grid: dx=8mm, dy=8mm, dz=5mm

Power Drift = 0.05 dB

Peak SAR (extrapolated) = 0.658 W/kg

SAR(1 g) = 0.410 W/kg; SAR(10 g) = 0.247 W/kg

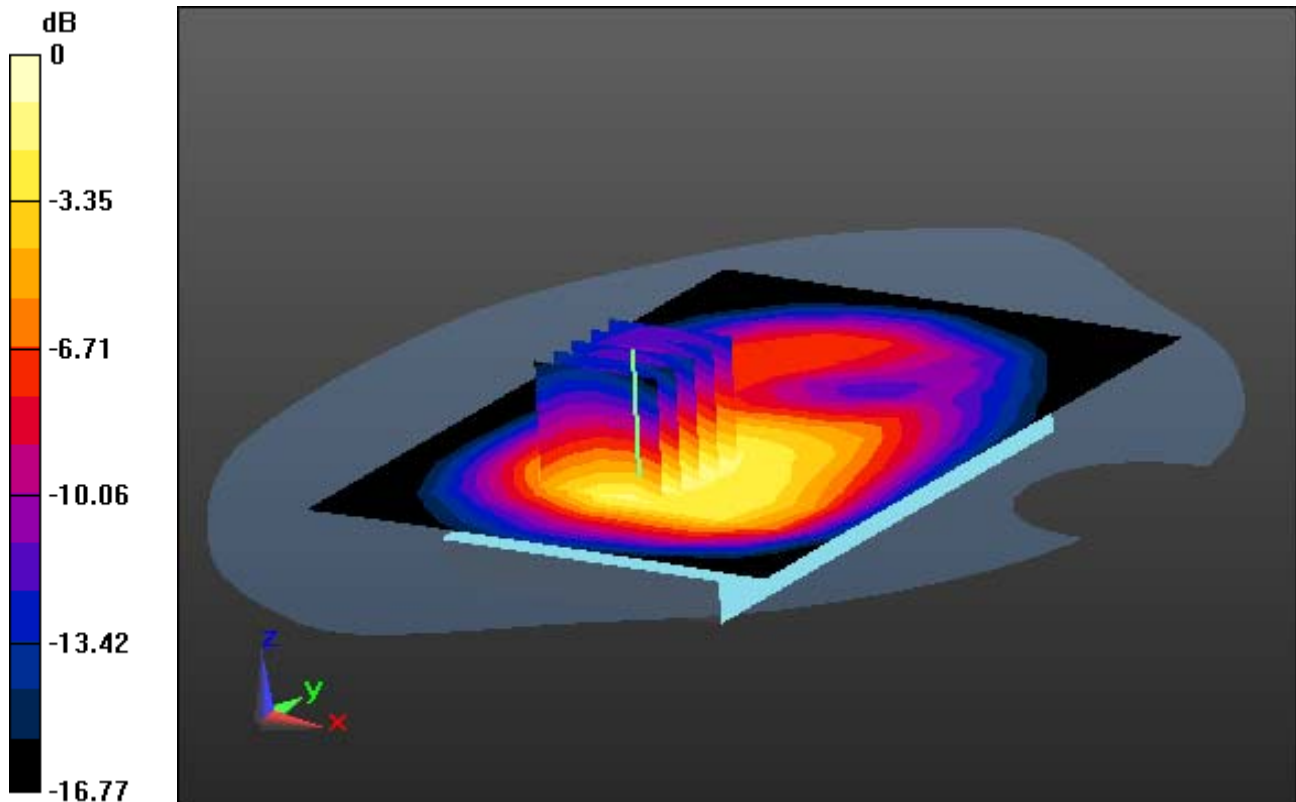

0 dB = 0.490 W/kg

DT&C Co., Ltd.

DUT: YKDA25; Type: Bar

Communication System: PCS 1900 (0); Frequency: 1880 MHz; Duty Cycle: 1:8.3
Medium parameters used: $f = 1880 \text{ MHz}$; $\sigma = 1.552 \text{ S/m}$; $\epsilon_r = 51.696$; $\rho = 1000 \text{ kg/m}^3$
Phantom section: Flat Section

DASY5 Configuration:

Probe: ES3DV3 - SN3328; ConvF(4.73, 4.73, 4.73); Calibrated: 3/18/2016; Electronics: DAE4 Sn1391
Phantom: SAM with CRP_2016_07_22_middle; Type: QD000P40CD; Serial: TP:1786
Measurement SW: DASY52, Version 52.8 (8); SEMCAD X Version 14.6.10 (7331)

Test Date: 2016-12-17; Ambient Temp; 20.8; Tissue Temp: 21.1

1cm space from Body, Rear, PCS1900 Ch. 661, Ant Internal

With Enlarge Plot image


Area Scan (9x13x1): Measurement grid: $dx=15\text{mm}$, $dy=15\text{mm}$

Zoom Scan (5x5x7)/Cube 0: Measurement grid: $dx=8\text{mm}$, $dy=8\text{mm}$, $dz=5\text{mm}$

Power Drift = 0.05 dB

Peak SAR (extrapolated) = 0.658 W/kg

SAR(1 g) = 0.410 W/kg; SAR(10 g) = 0.247 W/kg

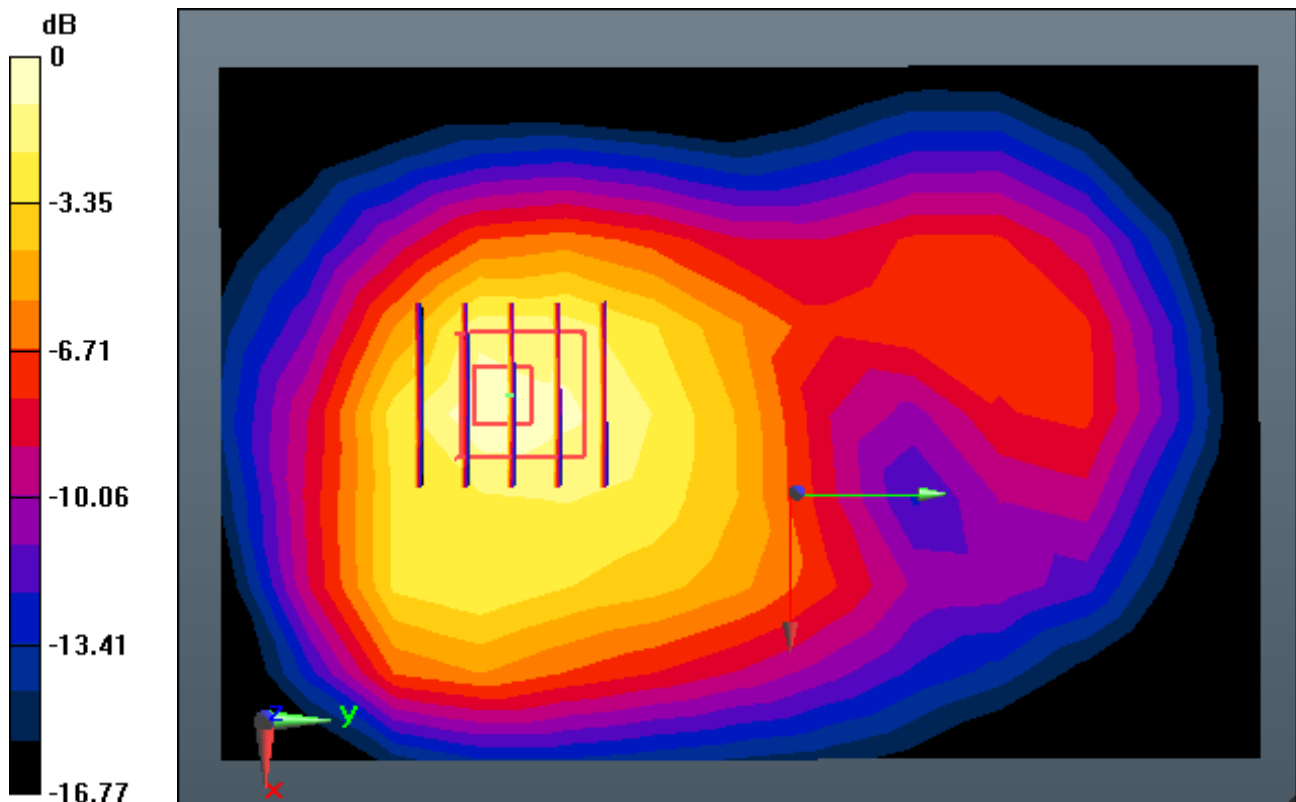

0 dB = 0.490 W/kg

DT&C Co., Ltd.

DUT: YKDA25; Type: Bar

Communication System: PCS 1900 (0); Frequency: 1880 MHz; Duty Cycle: 1:8.3
Medium parameters used: $f = 1880$ MHz; $\sigma = 1.552$ S/m; $\epsilon_r = 51.696$; $\rho = 1000$ kg/m³
Phantom section: Flat Section

DASY5 Configuration:

Probe: ES3DV3 - SN3328; ConvF(4.73, 4.73, 4.73); Calibrated: 3/18/2016; Electronics: DAE4 Sn1391
Phantom: SAM with CRP_2016_07_22_middle; Type: QD000P40CD; Serial: TP:1786
Measurement SW: DASY52, Version 52.8 (8); SEMCAD X Version 14.6.10 (7331)

Test Date: 2016-12-17; Ambient Temp; 20.8; Tissue Temp: 21.1

1cm space from Body, Rear, PCS1900 Ch. 661, Ant Internal


Area Scan (9x13x1): Measurement grid: dx=15mm, dy=15mm

Zoom Scan (5x5x7)/Cube 0: Measurement grid: dx=8mm, dy=8mm, dz=5mm

Power Drift = 0.05 dB

Peak SAR (extrapolated) = 0.658 W/kg

SAR(1 g) = 0.410 W/kg; SAR(10 g) = 0.247 W/kg

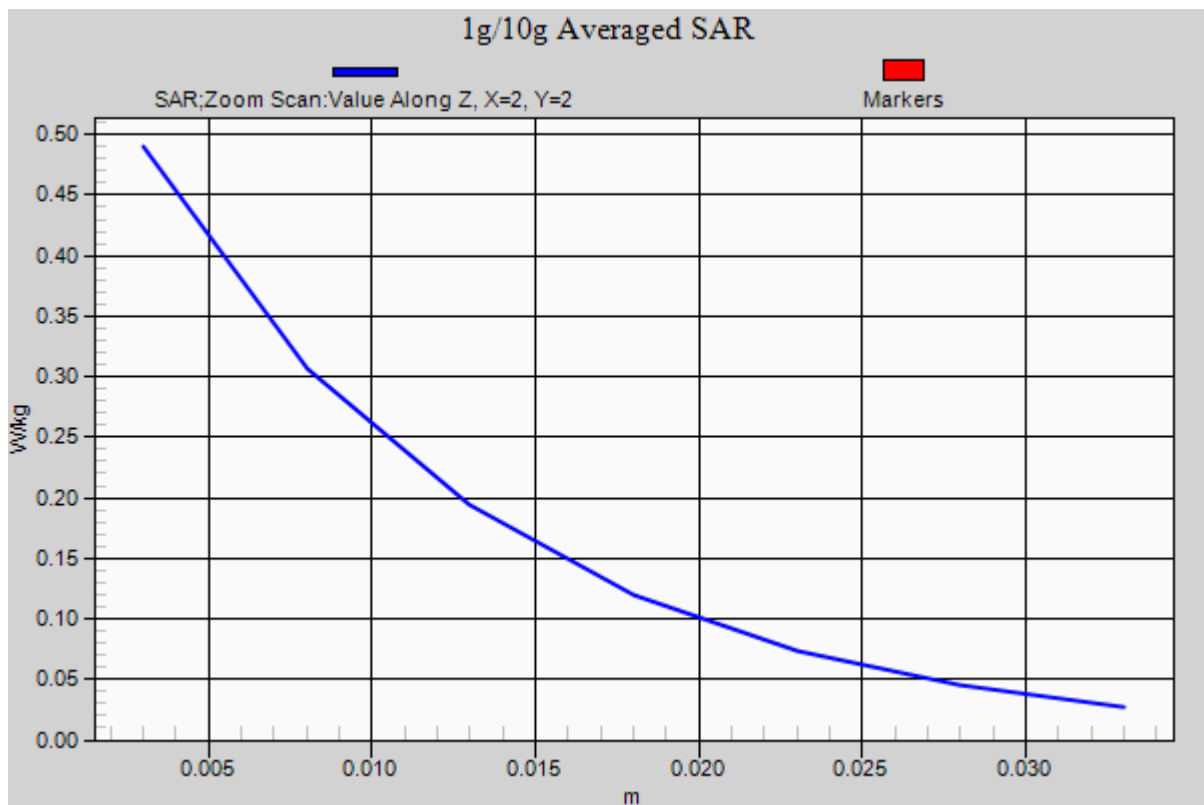

DT&C Co., Ltd.

DUT: YKDA25; Type: Bar

Communication System: PCS1900_Class 10 (0); Frequency: 1880 MHz; Duty Cycle: 1:4.15

Medium parameters used: $f = 1880$ MHz; $\sigma = 1.552$ S/m; $\epsilon_r = 51.696$; $\rho = 1000$ kg/m³

Phantom section: Flat Section

DASY5 Configuration:

Probe: ES3DV3 - SN3328; ConvF(4.73, 4.73, 4.73); Calibrated: 3/18/2016; Electronics: DAE4 Sn1391

Phantom: SAM with CRP_2016_07_22_middle; Type: QD000P40CD; Serial: TP:1786

Measurement SW: DASY52, Version 52.8 (8); SEMCAD X Version 14.6.10 (7331)

Test Date: 2016-12-17; Ambient Temp; 20.8; Tissue Temp: 21.1

1cm space from Body, Rear, PCS1900 GPRS 2Tx Ch. 661, Ant Internal


Area Scan (9x13x1): Measurement grid: dx=15mm, dy=15mm

Zoom Scan (5x5x7)/Cube 0: Measurement grid: dx=8mm, dy=8mm, dz=5mm

Power Drift = 0.09 dB

Peak SAR (extrapolated) = 0.952 W/kg

SAR(1 g) = 0.594 W/kg; SAR(10 g) = 0.358 W/kg

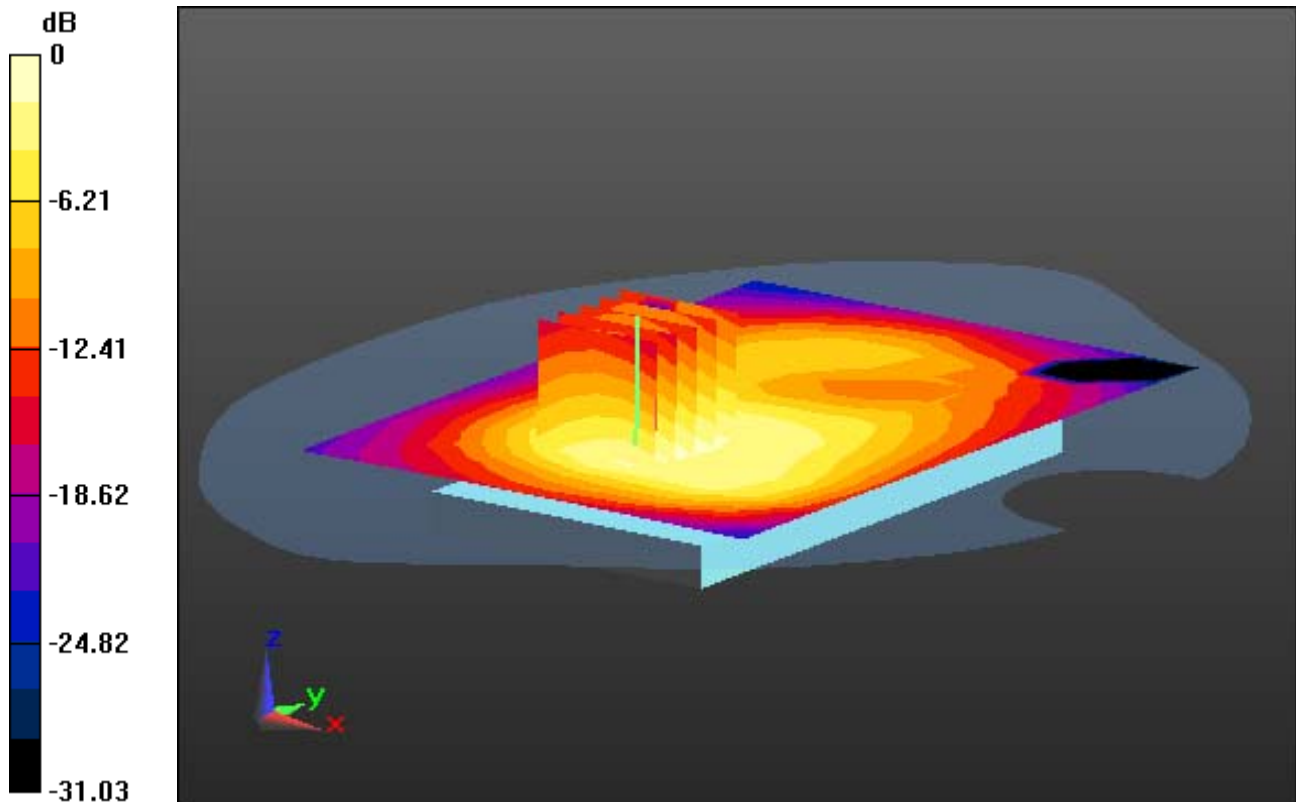

0 dB = 0.710 W/kg

DT&C Co., Ltd.

DUT: YKDA25; Type: Bar

Communication System: PCS1900_Class 10 (0); Frequency: 1880 MHz; Duty Cycle: 1:4.15

Medium parameters used: $f = 1880 \text{ MHz}$; $\sigma = 1.552 \text{ S/m}$; $\epsilon_r = 51.696$; $\rho = 1000 \text{ kg/m}^3$

Phantom section: Flat Section

DASY5 Configuration:

Probe: ES3DV3 - SN3328; ConvF(4.73, 4.73, 4.73); Calibrated: 3/18/2016; Electronics: DAE4 Sn1391

Phantom: SAM with CRP_2016_07_22_middle; Type: QD000P40CD; Serial: TP:1786

Measurement SW: DASY52, Version 52.8 (8); SEMCAD X Version 14.6.10 (7331)

Test Date: 2016-12-17; Ambient Temp; 20.8; Tissue Temp: 21.1

1cm space from Body, Rear, PCS1900 GPRS 2Tx Ch. 661, Ant Internal

With Enlarge Plot image


Area Scan (9x13x1): Measurement grid: $dx=15\text{mm}$, $dy=15\text{mm}$

Zoom Scan (5x5x7)/Cube 0: Measurement grid: $dx=8\text{mm}$, $dy=8\text{mm}$, $dz=5\text{mm}$

Power Drift = 0.09 dB

Peak SAR (extrapolated) = 0.952 W/kg

SAR(1 g) = 0.594 W/kg; SAR(10 g) = 0.358 W/kg

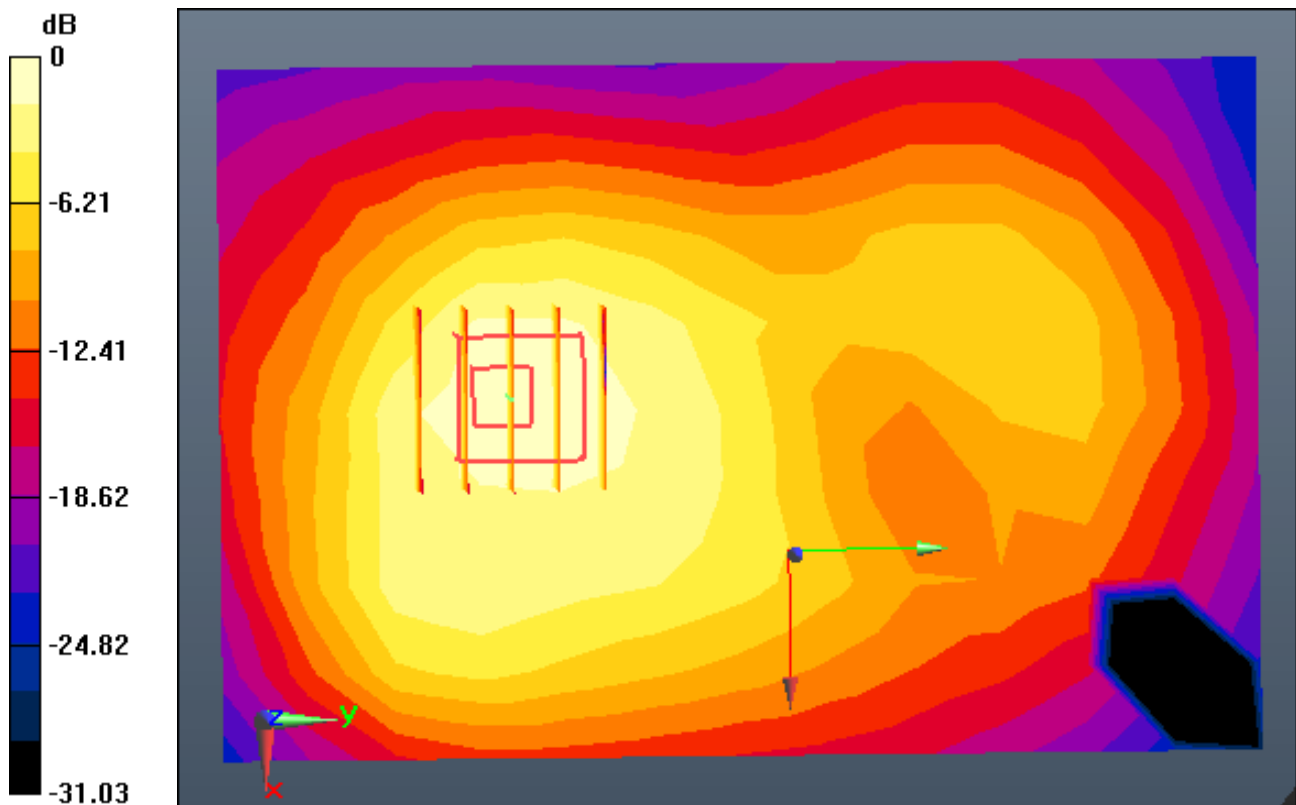

0 dB = 0.710 W/kg

DT&C Co., Ltd.

DUT: YKDA25; Type: Bar

Communication System: PCS1900_Class 10 (0); Frequency: 1880 MHz; Duty Cycle: 1:4.15

Medium parameters used: $f = 1880$ MHz; $\sigma = 1.552$ S/m; $\epsilon_r = 51.696$; $\rho = 1000$ kg/m³

Phantom section: Flat Section

DASY5 Configuration:

Probe: ES3DV3 - SN3328; ConvF(4.73, 4.73, 4.73); Calibrated: 3/18/2016; Electronics: DAE4 Sn1391

Phantom: SAM with CRP_2016_07_22_middle; Type: QD000P40CD; Serial: TP:1786

Measurement SW: DASY52, Version 52.8 (8); SEMCAD X Version 14.6.10 (7331)

Test Date: 2016-12-17; Ambient Temp; 20.8; Tissue Temp: 21.1

1cm space from Body, Rear, PCS1900 GPRS 2Tx Ch. 661, Ant Internal


Area Scan (9x13x1): Measurement grid: dx=15mm, dy=15mm

Zoom Scan (5x5x7)/Cube 0: Measurement grid: dx=8mm, dy=8mm, dz=5mm

Power Drift = 0.09 dB

Peak SAR (extrapolated) = 0.952 W/kg

SAR(1 g) = 0.594 W/kg; SAR(10 g) = 0.358 W/kg

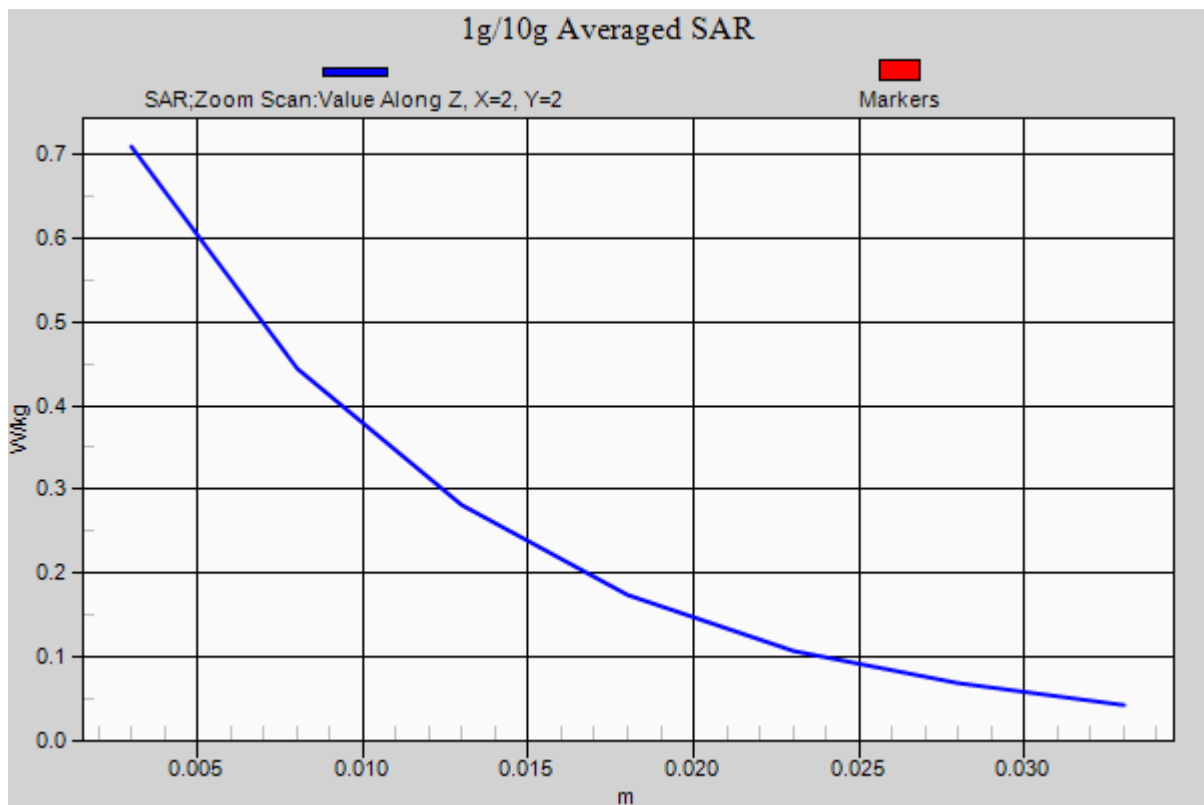

DT&C Co., Ltd.

DUT: YKDA25; Type: Bar

Communication System: W-LAN (0); Frequency: 2412 MHz; Duty Cycle: 1:1
Medium parameters used: $f = 2412$ MHz; $\sigma = 1.89$ S/m; $\epsilon_r = 51.136$; $\rho = 1000$ kg/m³
Phantom section: Flat Section

DASY5 Configuration:

Probe: ES3DV3 - SN3328; ConvF(4.4, 4.4, 4.4); Calibrated: 3/18/2016; Electronics: DAE4 Sn1391
Phantom: SAM with CRP_2016_07_22_middle; Type: QD000P40CD; Serial: TP:1786
Measurement SW: DASY52, Version 52.8 (8); SEMCAD X Version 14.6.10 (7331)

Test Date: 2016-12-19; Ambient Temp; 20.4; Tissue Temp: 21.0

1cm space from Body, Rear, W-LAN(802.11b) Ch. 1, Ant Internal


Area Scan (11x16x1): Measurement grid: dx=12mm, dy=12mm

Zoom Scan (7x7x7)/Cube 0: Measurement grid: dx=5mm, dy=5mm, dz=5mm

Power Drift = -0.05 dB

Peak SAR (extrapolated) = 0.421 W/kg

SAR(1 g) = 0.191 W/kg; SAR(10 g) = 0.093 W/kg

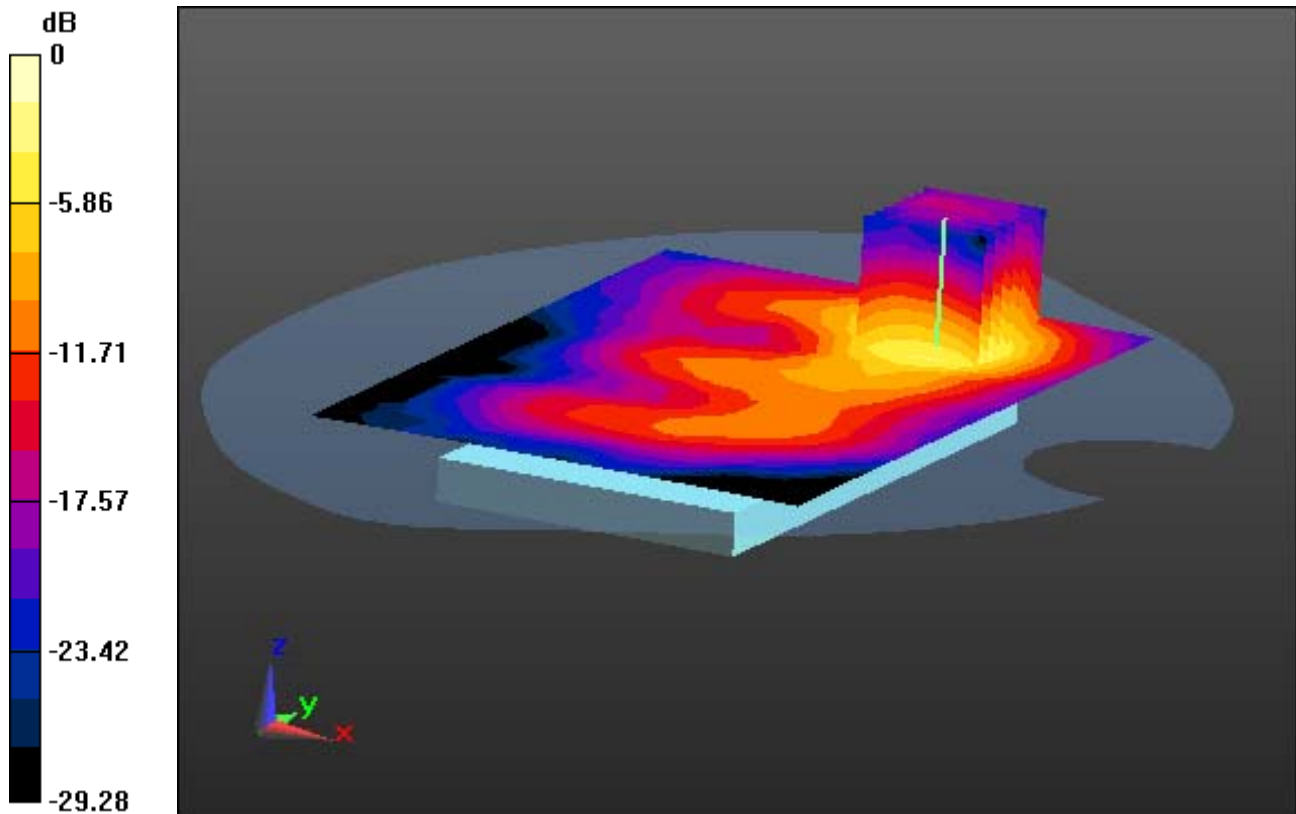

0 dB = 0.245 W/kg

DT&C Co., Ltd.

DUT: YKDA25; Type: Bar

Communication System: W-LAN (0); Frequency: 2412 MHz; Duty Cycle: 1:1
Medium parameters used: $f = 2412$ MHz; $\sigma = 1.89$ S/m; $\epsilon_r = 51.136$; $\rho = 1000$ kg/m³
Phantom section: Flat Section

DASY5 Configuration:

Probe: ES3DV3 - SN3328; ConvF(4.4, 4.4, 4.4); Calibrated: 3/18/2016; Electronics: DAE4 Sn1391
Phantom: SAM with CRP_2016_07_22_middle; Type: QD000P40CD; Serial: TP:1786
Measurement SW: DASY52, Version 52.8 (8); SEMCAD X Version 14.6.10 (7331)

Test Date: 2016-12-19; Ambient Temp; 20.4; Tissue Temp: 21.0

1cm space from Body, Rear, W-LAN(802.11b) Ch. 1, Ant Internal

With Enlarge Plot image


Area Scan (11x16x1): Measurement grid: dx=12mm, dy=12mm

Zoom Scan (7x7x7)/Cube 0: Measurement grid: dx=5mm, dy=5mm, dz=5mm

Power Drift = -0.05 dB

Peak SAR (extrapolated) = 0.421 W/kg

SAR(1 g) = 0.191 W/kg; SAR(10 g) = 0.093 W/kg

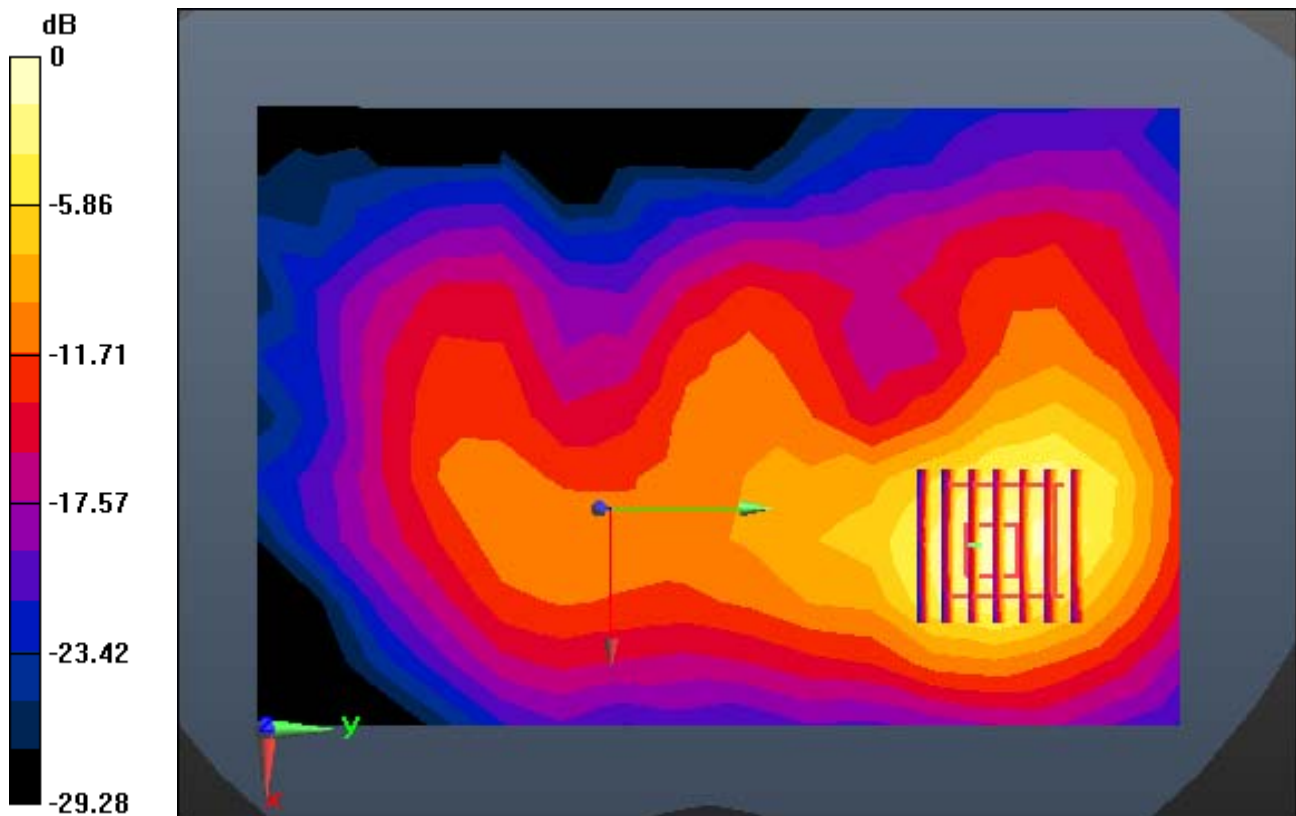

0 dB = 0.245 W/kg

DT&C Co., Ltd.

DUT: YKDA25; Type: Bar

Communication System: W-LAN (0); Frequency: 2412 MHz; Duty Cycle: 1:1
Medium parameters used: $f = 2412$ MHz; $\sigma = 1.89$ S/m; $\epsilon_r = 51.136$; $\rho = 1000$ kg/m³
Phantom section: Flat Section

DASY5 Configuration:

Probe: ES3DV3 - SN3328; ConvF(4.4, 4.4, 4.4); Calibrated: 3/18/2016; Electronics: DAE4 Sn1391
Phantom: SAM with CRP_2016_07_22_middle; Type: QD000P40CD; Serial: TP:1786
Measurement SW: DASY52, Version 52.8 (8); SEMCAD X Version 14.6.10 (7331)

Test Date: 2016-12-19; Ambient Temp; 20.4; Tissue Temp: 21.0

1cm space from Body, Rear, W-LAN(802.11b) Ch. 1, Ant Internal

Area Scan (11x16x1): Measurement grid: dx=12mm, dy=12mm

Zoom Scan (7x7x7)/Cube 0: Measurement grid: dx=5mm, dy=5mm, dz=5mm

Power Drift = -0.05 dB

Peak SAR (extrapolated) = 0.421 W/kg

SAR(1 g) = 0.191 W/kg; SAR(10 g) = 0.093 W/kg

