

## SAR TEST REPORT

<b>Applicant Name:</b> <b>JVC KENWOOD CORPORATION</b> 1-16-2 Hakusan Midori-ku Yokohama-shi Kanagawa 226-8525 Japan	<b>Date of Issue:</b> 05. 10, 2018 <b>Test Report No.:</b> HCT-SR-1802-FC001-R1 <b>Test Site:</b> HCT CO., LTD.
--	---

**FCC ID:****K44500000****Equipment Type:**  
**Model Name:****UHF DIGITAL TRANSCEIVER**  
**NX-P500-K****Testing has been carried out in accordance with:** 47CFR §2.1093  
ANSI/ IEEE C95.1 - 2005**Date of Test:**

02/08/2018, 02/19/2018

This device has been shown to be capable of compliance for localized specific absorption rate (SAR) for uncontrolled environment/general population exposure limits specified in FCC KDB procedures and had been tested in accordance with the measurement procedures specified in FCC KDB procedures.

I attest to the accuracy of data. All measurements reported herein were performed by me or were made under my supervision and are correct to the best of my knowledge and belief. I assume full responsibility for the completeness of these measurements and vouch for the qualifications of all persons taking them.

**Tested By**

**Bong-Kyun Park**  
Test Engineer / SAR Team  
Certification Division

**Reviewed By**

**Yun-jeang, Heo**  
Technical Manager / SAR Team  
Certification Division

This report only responds to the tested sample and may not be reproduced, except in full, without written approval of the HCT Co., Ltd.

**DOCUMENT HISTORY**

Rev.	DATE	DESCRIPTION
HCT-SR-1802-FC001	02. 26, 2018	First Approval Report
HCT-SR-1802-FC001-R1	05. 10, 2018	Device information was revised.

# Table of Contents

1. Attestation of Test Result of Device Under Test.....	4
3. Output Power Specifications.....	6
4. Manufacturer's Accessory List .....	7
5. INTRODUCTION .....	8
6. DESCRIPTION OF TEST EQUIPMENT .....	9
7. SAR MEASUREMENT PROCEDURE.....	12
8. DESCRIPTION OF TEST POSITION.....	14
9. ANSI/ IEEE C95.1 - 2005 RF EXPOSURE LIMITS .....	15
10. SYSTEM VERIFICATION.....	16
11. SAR TEST DATA SUMMARY .....	18
13. MEASUREMENT UNCERTAINTY .....	20
14. SAR TEST EQUIPMENT .....	21
15. CONCLUSION.....	22
16. REFERENCES .....	23
Attachment 1. – SAR Test Plots .....	25
Attachment 2. – Dipole Verification Plots.....	29
Attachment 3. – Probe Calibration Data.....	32
Attachment 4. – Dipole Calibration Data .....	44
Attachment 5. – SAR Tissue Characterization.....	53
Attachment 6. – SAR SYSTEM VALIDATION .....	54
Attachment 7. – SAR Test SETUP PHOTOGRAPHS	

## 1. Attestation of Test Result of Device Under Test

Test Laboratory	
Company Name:	HCT Co., LTD
Address	74, Seoicheon-ro 578beon-gil, Majang-myeon, Icheon-si, Gyeonggi-do, 17383, Rep. of Korea
Telephone	+82 31 645 6300
Fax.	+82 31 645 6401

Attestation of SAR test result	
Applicant Name:	JVC KENWOOD CORPORATION
FCC ID:	K44500000
Model:	NX-P500-K
EUT Type:	UHF DIGITAL TRANSCEIVER
Application Type:	Certification

The Highest Reported SAR					
Band	Tx. Frequency (MHz)	Equipment Class	Reported 1g SAR (W/kg)		
			Hand-held to Face	Body-Worn Belt clip	
UHF	450 ~ 470	TNF	0.92	1.32	50% PTT duty cycle
Simultaneous SAR per KDB 690783 D01v01r03			N/A		
Date(s) of Tests:	02/08/2018, 02/19/2018				

---

The tests documented in this report were performed in accordance with IEEE Standard 1528-2013 & IEEE 1528-2005 and the following published KDB procedures.

- FCC KDB Publication 447498 D01 General SAR Guidance v06
- FCC KDB Publication 865664 D01 SAR measurement 100 MHz to 6 GHz v01r04
- FCC KDB Publication 865664 D02 SAR Reporting v01r02
- FCC KDB Publication 643646 D01 SAR Test for PTT Radios v01r03

## 3. Output Power Specifications.

### 3.1 Nominal and Maximum Output Power Specifications

This device operates using the following maximum output power specifications. SAR values were scaled to the maximum allowed power to determine compliance per KDB publication 447498 D01v06.

### 3.2 Maximum Output Power

Band	Frequency	Power
UHF	450 MHz ~ 470 MHz	2.0 W

### 3.3 Output Average Conducted Power

UHF					
Model	Frequency (MHz)	Ch.	Ch. Type	Ch. Spacing	Conduction Power (dBm)
NX-P500-K	450.05	1	Analog	Narrow	32.695
	460.05	2	Analog	Narrow	32.775
	469.95	3	Analog	Narrow	32.575
	450.05	4	Analog	Wide	32.651
	460.05	5	Analog	Wide	32.769
	469.95	6	Analog	Wide	32.651
	450.05	7	Digital	Very Narrow	32.711
	460.05	8	Digital	Very Narrow	32.770
	469.95	9	Digital	Very Narrow	32.557
	450.05	10	Digital	Narrow	32.636
	460.05	11	Digital	Narrow	<b>32.776</b>
	469.95	12	Digital	Narrow	32.588

For FCC Band:

Per KDB 447498 D01v06 Page 7 section 6) pages 7-8, the number of channels are required to be tested is as follows.

$$F_{high} = 469.95 \text{ MHz}$$

$$F_c = 460.05 \text{ MHz}$$

$$F_{Low} = 450.05 \text{ MHz}$$

$$N_c = \text{Round} \{ [100(f_{high} - f_{low}) / f_c]^{0.5} \times (f_c / 100)^{0.2} \} = \text{Round} \{ [100(469.95 - 450.05) / 460.05]^{0.5} \times (460.05 / 100)^{0.2} \} = 3$$

Therefore, for the frequency band from 450.05 MHz to 469.95 MHz, 3 channels are required for testing.

## 4. Manufacturer's Accessory List

Part No.	Description	Accessory Type	Accessory
KNB-81L	Li-Ion Battery Pack (2200mAh)	Battery	1
KBH-14	Belt Clip	CARRYING ACCESSORIES	1
KBH-20	Belt Clip (Tested)		2
KBH-21	Belt Clip		3
KBH-22	Belt Clip Holster (Tested)		4
KMC-55	Speaker Microphone (Test)	Audio Accessory	1
KHS-37	Headset		2
EMC-14	Clip Microphone with Earphone		3
EMC-13	Clip Microphone with Earphone		4

\* Note: Battery Dimensions

No.	Battery Model	description	Size (mm)
1	KNB-81L	Li-Ion Battery Pack (2200 mAh)	57mm*34mm*10mm

### Body-Worn Test (Speaker Microphone)

Audio Accessory	Battery
	1
1	Yes
2	No
3	No
4	No

### Body-Worn Test (Belt Clip)

CARRYING Accessory	Battery
	1
1	No
2	Yes
3	No
4	Yes

\* Manufacturer's disclosed accessory listing information provided by Kenwood corporation.

\* Note: Audio Accessory KMC-55 was chosen for the testing body worn radio configuration.

## 5. INTRODUCTION

The FCC has adopted the guidelines for evaluating the environmental effects of radio frequency radiation in ET Docket 93-62 on Aug. 6, 1996 to protect the public and workers from the potential hazards of RF emissions due to FCC-regulated portable devices.

The safety limits used for the environmental evaluation measurements are based on the criteria published by the American National Standards Institute (ANSI) for localized specific absorption rate (SAR) in IEEE/ANSI C95.1-2005 Standard for Safety Levels with Respect to Human Exposure to Radio Frequency Electromagnetic Fields, 3 kHz to 300 GHz. 1992 by the Institute of Electrical and Electronics Engineers, Inc., New York 10017. The measurement procedure described in IEEE/ANSI C95.3-1992 Recommended Practice for the Measurement of Potentially Hazardous Electromagnetic Fields - RF and Microwave is used for guidance in measuring SAR due to the RF radiation exposure from the Equipment Under Test (EUT). These criteria for SAR evaluation are similar to those recommended by the National Council on Radiation Protection and Measurements (NCRP) in Biological Effects and Exposure Criteria for Radio frequency Electromagnetic Fields," NCRP Report No. 86 NCRP, 1986, Bethesda, MD 20814. SAR is a measure of the rate of energy absorption due to exposure to an RF transmitting source. SAR values have been related to threshold levels for potential biological hazards.

### SAR Definition

Specific Absorption Rate (SAR) is defined as the time derivative of the incremental electromagnetic energy ( $dW$ ) absorbed by (dissipated in) an incremental mass ( $dm$ ) contained in a volume element ( $dV$ ) of a given density ( $r$ ). It is also defined as the rate of RF energy absorption per unit mass at a point in an absorbing body.

$$SAR = \frac{d}{d t} \left( \frac{d U}{d m} \right)$$

Figure 1. SAR Mathematical Equation

*SAR is expressed in units of Watts per Kilogram (W/kg)*

$$SAR = \sigma E^2 / \rho$$

Where:

$\sigma$  = conductivity of the tissue-simulant material (S/m)

$\rho$  = mass density of the tissue-simulant material (kg/m<sup>3</sup>)

$E$  = Total RMS electric field strength (V/m)

NOTE: The primary factors that control rate of energy absorption were found to be the wavelength of the incident field in relations to the dimensions and geometry of the irradiated organism, the orientation of the organism in relation to the polarity of field vectors, the presence of reflecting surfaces, and whether conductive contact is made by the organism with a ground plane.

## 6. DESCRIPTION OF TEST EQUIPMENT

### 6.1 SAR MEASUREMENT SETUP

These measurements are performed using the DASY4 automated dosimetric assessment system. It is made by Schmid & Partner Engineering AG (SPEAG) in Zurich, Switzerland. It consists of high precision robotics system (Staubli), robot controller, Pentium III computer, near-field probe, probe alignment sensor, and the generic twin phantom containing the brain equivalent material. The robot is a six-axis industrial robot performing precise movements to position the probe to the location (points) of maximum electromagnetic field (EMF) (see Figure.2).

A cell controller system contains the power supply, robot controller, teach pendant (Joystick), and remote control, is used to drive the robot motors. The PC with Windows XP or Windows 7 is working with SAR Measurement system DASY4 & DASY5, A/D interface card, monitor, mouse, and keyboard. The Staubli Robot is connected to the cell controller to allow software manipulation of the robot. A data acquisition electronic (DAE) circuit performs the signal amplification, signal multiplexing, AD-conversion, offset measurements, mechanical surface detection, collision detection, etc. is connected to the Electro-optical coupler (EOC). The EOC performs the conversion from the optical into digital electric signal of the DAE and transfers data to the PC plug-in card.

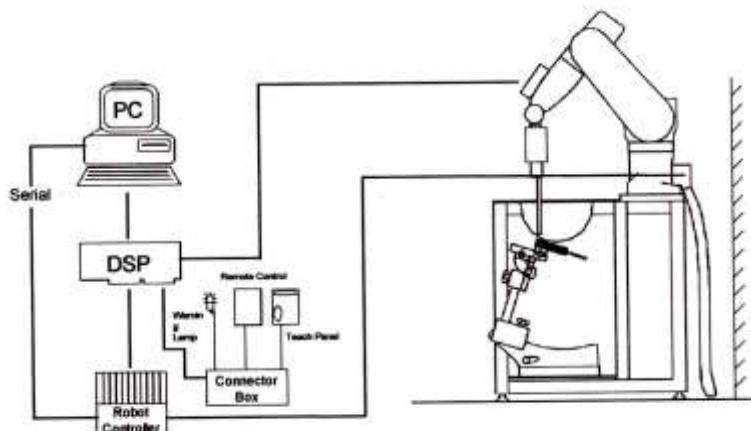


Figure 2. HCT SAR Lab. Test Measurement Set-up

The DAE consists of a highly sensitive electrometer-grade preamplifier with auto-zeroing, a channel and gain-switching multiplexer, a fast 16 bit AD-converter and a command decoder and control logic unit. Transmission to the PC-card is accomplished through an optical downlink for data and status information and an optical uplink for commands and clock lines. The mechanical probe mounting device includes two different sensor systems for frontal and sidewise probe contacts. They are also used for mechanical surface detection and probe collision detection. The robot uses its own controller with a built in VME-bus computer. The system is described in detail in.

## 6.2 Phantom

### • ELI Phantom

Phantom for compliance testing of handheld and body-mounted wireless devices in the frequency range of 30 MHz to 6 GHz. ELI is fully compatible with the IEC 62209-2 standard and all known tissue simulating liquids. ELI has been optimized regarding its performance and can be integrated into our standard phantom tables. A cover prevents evaporation of the liquid. Reference markings on the phantom allow installation of the complete setup, including all predefined phantom positions and measurement grids, by teaching three points. The phantom is compatible with all SPEAG diametric probes and dipoles.



Figure 6.1 ELI Phantom

Shell Thickness	2.0 ± 0.2mm
Filling Volume	approx. 30 liters
Dimensions	Major axis: 600 mm, Minor axis: 400 mm

## 6.3 Device Holder for Transmitters

### Device Holder – Mounting Device

In combination with the SAM Phantom, the Mounting Device enables the rotation of the mounted transmitter in spherical coordinates whereby the rotation points is the ear opening. The devices can be easily, accurately, and repeatable positioned according to the EN 50360:2001/A:2001 and FCC KDB specifications. The device holder can be locked at different phantom locations (left head, right head, flat phantom).

Note: A simulating human hand is not used due to the complex anatomical and geometrical structure of the hand that may produce infinite number of configurations. To produce the Worst-case condition (the hand absorbs antenna output power), the hand is omitted during the tests.



## 6.4 Validation Dipole

The reference dipole should have a return loss better than -20 dB (measured in the setup) at the resonant frequency to reduce the uncertainty in the power measurement.

System Validation Dipole	
<b>Description</b>	Symmetrical dipole with $\lambda/4$ balun. Enables measurement of feedpoint impedance with network analyzer (NWA). Matched for use near flat phantoms filled with tissue simulating liquids.
<b>Frequency</b>	450 MHz
<b>Return Loss</b>	> 20 dB at specified validation position
<b>Power Capability</b>	> 100 W (f < 1GHz), >40 W (f > 1 GHz)
<b>Dimension</b>	D450V2: dipole length : 272.0 mm ; overall height : 330.0 mm



## 6.5 Brain & Muscle Tissue Simulating Mixture Characterization

The brain and muscle mixtures consist of a viscous gel using hydrox-ethyl cellulose (HEC) gelling agent and saline solution (see Table 1). Preservation with a bactericide is added and visual inspection is made to make sure air bubbles are not trapped during the mixing process. The mixture is calibrated to obtain proper dielectric constant (permittivity) and conductivity of the desired tissue. The mixture characterizations used for the brain and muscle tissue simulating liquids are according to the data by C. Gabriel and G. Hartsgrove.

Frequency (MHz)	30	50	144	450	835	900		
Recipe source number	3	3	2	2	3	2	4	2
Ingredients (% by weight)								
Deionised water	48,30	48,30	53,53	55,12	48,30	48,53	56	50,36
Tween			44,70	43,31		49,51		48,39
Oxidised mineral oil						44		48,34
Diethylenglycol monohexylether								44
Triton X-100								
Diacetin	50,00	50,00			50,00			
DGBE								
NaCl	1,60	1,60	1,77	1,57	1,60	1,96		1,25
Additives and salt	0,10	0,10			0,10			1,35
Measured dielectric parameters								
$\epsilon_r'$	54,2	53,1	54,54	52,81	51,0	43,29	42,3	41,6
$\sigma$ (S/m)	0,75	0,75	0,76	0,76	0,77	0,88	0,84	0,90
Temp. (°C)			21	21		21	20	21
$\epsilon_{temp\_liquid}$ uncertainty (%)	0,8	0,1			0,1	0,1		0,04
$\sigma_{temp\_liquid}$ uncertainty (%)	2,8	2,8			2,6	4,2		1,6
Target values (from Table 1)								
$\epsilon_r'$	55,0	54,5		52,4		43,5	41,5	41,5
$\sigma$ (S/m)	0,75	0,75		0,76		0,87	0,90	0,97

Fig 4. Composition of the Tissue Equivalent Matter

## 7. SAR MEASUREMENT PROCEDURE

The evaluation was performed with the following procedure:

1. The SAR distribution at the exposed side of the head or body was measured at a distance no more than 5.0 mm from the inner surface of the shell. The area covered the entire dimension of the DUT's head and body area and the horizontal grid resolution was depending on the FCC KDB 865664 D01v01r04 table 4-1 & IEEE 1528-2013.
2. Based on step, the area of the maximum absorption was determined by sophisticated interpolations routines implemented in DASY software. When an Area Scan has measured all reachable point. DASY system computes the field maximal found in the scanned are, within a range of the maximum. SAR at this fixed point was measured and used as a reference value.
3. Around this point, a volume was assessed according to the measurement resolution and volume size requirements of FCC KDB 865664 D01v01r04 table 4-1 and IEEE 1528-2013. On the basis of this data set, the spatial peak SAR value was evaluated with the following procedure (reference from the DASY manual.)
  - a. The data at the surface were extrapolated, since the center of the dipoles is no more than 2.7 mm away from the tip of the probe (it is different from the probe type) and the distance between the surface and the lowest measuring point is 1.2 mm. The extrapolation was based on a least square algorithm. A polynomial of the fourth order was calculated through the points in z-axes. This polynomial was then used to evaluate the points between the surface and the probe tip.
  - b. The maximum interpolated value was searched with a straight-forward algorithm. Around this maximum the SAR values averaged over the spatial volumes (1 g or 10 g) were computed using the 3D-Spline interpolation algorithm. The 3D-spline is composed of three one-dimensional splines with the "Not a knot" condition (in x, y, and z directions. The volume was integrated with the trapezoidal algorithm. One thousand points (10 x 10 x 10) were interpolated to calculate the average.
  - c. All neighboring volumes were evaluated until no neighboring volume with a higher average value was found.
4. The SAR reference value, at the same location as step 2, was re-measured after the zoom scan. If the value changed by more than 5 %, the SAR evaluation and drift measurements were repeated.

Area scan and zoom scan resolution setting follow KDB 865664 D01v01r04 quoted below.

		$\leq 3$ GHz	$> 3$ GHz
Maximum distance from closest measurement point (geometric center of probe sensors) to phantom surface		$5 \pm 1$ mm	$\frac{1}{2} \delta \cdot \ln(2) \pm 0.5$ mm
Maximum probe angle from probe axis to phantom surface normal at the measurement location		$30^\circ \pm 1^\circ$	$20^\circ \pm 1^\circ$
		$\leq 2$ GHz: $\leq 15$ mm 2-3 GHz: $\leq 12$ mm	$3\text{-}4$ GHz: $\leq 12$ mm 4-6 GHz: $\leq 10$ mm
Maximum area scan Spatial resolution: $\Delta x_{\text{Area}}, \Delta y_{\text{Area}}$			When the x or y dimension of the test device, in the measurement plane orientation, is smaller than the above, the measurement resolution must be $\leq$ the corresponding x or y dimension of the test device with at least one measurement point on the test device.
Maximum zoom scan Spatial resolution: $\Delta x_{\text{zoom}}, \Delta y_{\text{zoom}}$		$\leq 2$ GHz: $\leq 8$ mm 2-3 GHz: $\leq 5$ mm*	$3\text{-}4$ GHz: $\leq 5$ mm* 4-6 GHz: $\leq 4$ mm*
Maximum zoom scan Spatial resolution normal to phantom surface	uniform grid: $\Delta z_{\text{zoom}}(n)$		$3\text{-}4$ GHz: $\leq 4$ mm 4-5 GHz: $\leq 3$ mm 5-6 GHz: $\leq 2$ mm
	graded grid	$\Delta z_{\text{zoom}}(1)$ : between 1 <sup>st</sup> two Points closest to phantom surface	$\leq 4$ mm
		$\Delta z_{\text{zoom}}(n>1)$ : between subsequent Points	$\leq 1.5 \cdot \Delta z_{\text{zoom}}(n-1)$
Minimum zoom scan volume	x, y, z	$\geq 30$ mm	$3\text{-}4$ GHz: $\geq 28$ mm 4-5 GHz: $\geq 25$ mm 5-6 GHz: $\geq 22$ mm

Note:  $\delta$  is the penetration depth of a plane-wave at normal incidence to the tissue medium; see draft standard IEEE P1528-2011 for details.

\* When zoom scan is required and the reported SAR from the area scan based 1-g SAR estimation procedures of KDB 447498 is  $\leq 1.4$  W/kg,  $\leq 8$  mm,  $\leq 7$  mm and  $\leq 5$  mm zoom scan resolution may be applied, respectively, for 2 GHz to 3 GHz, 3 GHz to 4 GHz and 4 GHz to 6 GHz.

## 8. DESCRIPTION OF TEST POSITION

### 8.1 Body Holster/Belt Clip Configurations

Body-worn operating configurations are tested with the belt-clips and holsters attached to the device and positioned against a flat phantom in a normal use configuration. A device with a headset output is tested with a headset connected to the device. Body dielectric parameters are used.

Accessories for Body-worn operation configurations are divided into two categories: those that do not contain metallic components and those that contain metallic components. When multiple accessories that do not contain metallic components are supplied with the device, the device is tested with only the accessory that dictates the closest spacing to the body. Then multiple accessories that contain metallic components are tested with each accessory. If multiple accessory share an identical metallic component (i.e. the same metallic belt-clip used with different holsters with no other metallic components) only the accessory that dictates the closest spacing to the body is tested.

Body-worn accessories may not always be supplied or available as options for some Devices intended to be authorized for body-worn use. In this case, a test configuration with a separation distance between the back of the device and the flat phantom is used.

Since this EUT does not supply any body worn accessory to the end user a distance of 0 cm from the EUT back surface to the liquid interface is configured for the generic test.


"See the Test SET-UP Photo"

Transmitters that are designed to operate in front of a person's face, as in push-to-talk configurations, are tested for SAR compliance with the front of the device positioned to face the flat phantom. For devices that are carried next to the body such as a shoulder, waist or chest-worn transmitters, SAR compliance is tested with the accessory(ies), Including headsets and microphones, attached to the device and positioned against a flat phantom in a normal use configuration.

In all cases SAR measurements are performed to investigate the worst-case positioning. Worst case positioning is then documented and used to perform Body SAR testing.

### 8.2 Hand-held to Face device

A typical example of a front-of-face device is a two-way radio that is held at a distance from the face of the user when transmitting. In these cases the device under test shall be positioned at the distance to the phantom surface that corresponds to the intended use as specified by the manufacturer in the user instructions. If the intended use is not specified, a separation distance of 25 mm<sup>5</sup> between the phantom surface and the device shall be used.

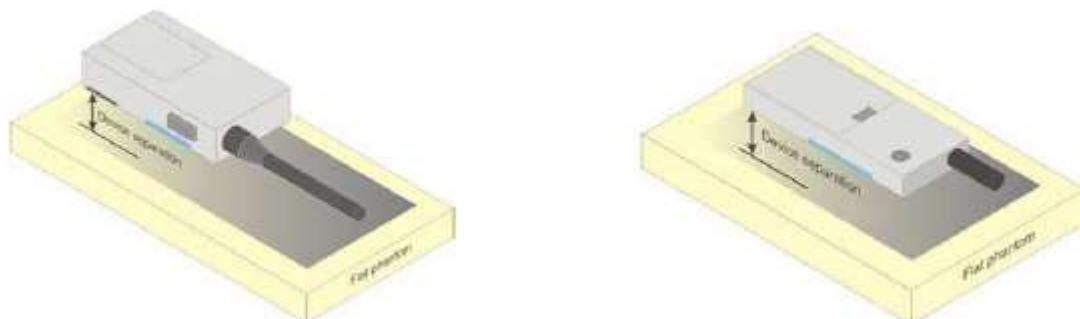

## 9. ANSI/ IEEE C95.1 - 2005 RF EXPOSURE LIMITS

HUMAN EXPOSURE	UNCONTROLLED ENVIRONMENT	CONTROLLED ENVIRONMENT
	General Population (W/kg) or (mW/g)	Occupational (W/kg) or (mW/g)
SPATIAL PEAK SAR * (Brain)	1.60	8.00
SPATIAL AVERAGE SAR ** (Whole Body)	0.08	0.40
SPATIAL PEAK SAR *** (Hands / Feet / Ankle / Wrist)	4.00	20.00

**Table 8.1 Safety Limits for Partial Body Exposure**

**NOTES:**

- \* The Spatial Peak value of the SAR averaged over any 1 g of tissue (defined as a tissue volume in the shape of a cube) and over the appropriate averaging time.
- \*\* The Spatial Average value of the SAR averaged over the whole-body.
- \*\*\* The Spatial Peak value of the SAR averaged over any 10 g of tissue (defined as a tissue volume in the shape of a cube) and over the appropriate averaging time.

**Uncontrolled Environments** are defined as locations where there is the exposure of individuals who have no knowledge or control of their exposure. The general population/uncontrolled exposure limits are applicable to situations in which the general public may be exposed or in which persons who are exposed as a consequence of their employment may not be made fully aware of the potential for exposure or cannot exercise control over their exposure. Members of the general public would come under this category when exposure is not employment-related; for example, in the case of a wireless transmitter that exposes persons in its vicinity.

**Controlled Environments** are defined as locations where there is exposure that may be incurred by persons who are aware of the potential for exposure, (i.e. as a result of employment or occupation). In general, occupational/controlled exposure limits are applicable to situations in which persons are exposed as a consequence of their employment, who have been made fully aware of the potential for exposure and can exercise control over their exposure. This exposure category is also applicable when the exposure is of a transient nature due to incidental passage through a location where the exposure levels may be higher than the general population/uncontrolled limits, but the exposed person is fully aware of the potential for exposure and can exercise control over his or her exposure by leaving the area or by some other appropriate means.

## 10. SYSTEM VERIFICATION

### 10.1 Tissue Verification

The Head /body simulating material is calibrated by HCT using the DAKS 3.5 to determine the conductivity and permittivity.

**Table for Head Tissue Verification**

Date of Tests	Tissue Temp. (°C)	Tissue Type	Freq. (MHz)	Measured Conductivity $\sigma$ (S/m)	Measured Dielectric Constant, $\epsilon$	Target Conductivity $\sigma$ (S/m)	Target Dielectric Constant, $\epsilon$	% dev $\sigma$	% dev $\epsilon$
02/08/2018	22.1	450H	430	0.831	44.945	0.870	43.740	-4.48%	2.75%
			450	0.849	44.414	0.870	43.500	-2.41%	2.10%
			500	0.888	43.076	0.874	43.240	1.60%	-0.38%

**Table for Body Tissue Verification**

Date of Tests	Tissue Temp. (°C)	Tissue Type	Freq. (MHz)	Measured Conductivity $\sigma$ (S/m)	Measured Dielectric Constant, $\epsilon$	Target Conductivity $\sigma$ (S/m)	Target Dielectric Constant, $\epsilon$	% dev $\sigma$	% dev $\epsilon$
02/19/2018	23.5	450B	430	0.935	56.051	0.937	56.900	-0.21%	-1.49%
			450	0.951	55.772	0.940	56.700	1.17%	-1.64%
			500	0.991	54.726	0.944	56.510	4.98%	-3.16%

## 10.2 System Verification

Prior to assessment, the system is verified to the  $\pm 10\%$  of the specifications at 450 MHz by using the system Verification kit. (Graphic Plots Attached)

### System Verification Results

Freq. [MHz]	Date	Probe (S/N)	Dipole (S/N)	Liquid	Amb. Temp.	Liquid Temp.	1 W Target SAR <sub>1g</sub> (SPEAG)	Measured SAR <sub>1g</sub>	1 W Normalized SAR <sub>1g</sub>	Deviation	Limit [%]
					[°C]	[°C]	[W/kg]	[W/kg]	[W/kg]	[%]	[%]
450	02/08/2018	3863	1007	Head	22.4	22.1	4.84	0.465	4.65	- 3.93	$\pm 10$
450	02/19/2018	3863	1007	Body	23.9	23.5	4.75	0.491	4.91	+ 3.37	$\pm 10$

## 10.3 System Verification Procedure

SAR measurement was prior to assessment, the system is verified to the  $\pm 10\%$  of the specifications at each frequency band by using the system Verification kit. (Graphic Plots Attached)

- Cabling the system, using the Verification kit equipments.
- Generate about 100 mW Input Level from the Signal generator to the Dipole Antenna.
- Dipole Antenna was placed below the Flat phantom.
- The measured one-gram SAR at the surface of the phantom above the dipole feed-point should be within 10 % of the target reference value.
- The results are normalized to 1 W input power.

NOTE:

SAR Verification was performed according to the FCC KDB 865664 D01v01r04.

## 11. SAR TEST DATA SUMMARY

### 11.1 Measurement Results (Hand-held to Face SAR)

Model Name	CH.	Battery	Frequency	Tune-Up Limit	Conducted Power	Power Drift	Separation Distance	Measured SAR	SAR 50% Duty	Reported SAR	Plot No.
			(MHz)	(dBm)	(dBm)	(dB)	(mm)	(mW/g)	(mW/g)	(mW/g)	
NX-P500-K	11	KNB-81L	460.05	33.0	32.776	-0.51	25	1.55	0.775	0.918	1
ANSI/ IEEE C95.1 - 2005 – Safety Limit Spatial Peak Controlled Exposure/ Occupational									8 W/kg (mW/g) Averaged over 1 gram		

### 11.2 Measurement Results (Body-worn Belt clip SAR)

Model Name	CH.	Battery	Carrying Accessory	Frequency	Tune-Up Limit	Conducted Power	Power Drift	Separation Distance	Measured SAR	SAR 50% Duty	Reported SAR	Plot No.
				(MHz)	(dBm)	(dBm)	(dB)	(mm)	(mW/g)	(mW/g)	(mW/g)	
NX-P500-K	11	KNB-81L	KBH-20	460.05	33.0	32.776	-0.37	0	2.31	1.155	1.324	2
	11	KNB-81L	KBH-22	460.05	33.0	32.776	-0.38	0	2.17	1.085	1.247	3
ANSI/ IEEE C95.1 - 2005 – Safety Limit Spatial Peak Controlled Exposure/ Occupational									8 W/kg (mW/g) Averaged over 1 gram			

## 11.3 SAR Test Notes

**General Notes:**

1. The test data reported are the worst-case SAR values according to test procedures specified in FCC KDB Procedure.
2. Batteries are fully charged at the beginning of the SAR measurements. A standard battery was used for all SAR measurements.
3. Liquid tissue depth was at least 15.0 cm for all frequencies.
4. The manufacturer has confirmed that the device(s) tested have the same physical, mechanical and thermal characteristics and are within operational tolerances expected for production units.
5. SAR results were scaled to the maximum allowed power to demonstrate compliance per FCC KDB 447498 D01v06.
6. Test signal call mode is Manual test cord.
7. The EUT was tested for face-held SAR with a 2.5 cm separation distance between the front of the EUT and the outer surface of the planer phantom
8. The Body-worn SAR evaluation was performed with the Balt-clip body-worn accessory attached to the DUT and touching the outer surface of the planar phantom.
9. The adjusted SAR value was calculated by first scaling the SAR value up by the drift. This value was then scaled up based on the difference of the upper end the tolerance (33.4 dBm) and the measured conducted power. The resultant value is then multiplied by 0.5 to give the SAR value at 50% duty cycle.
10. Measurement was reduced per KDB 643646 D01v01r03.
11. When the SAR for all antennas tested using the default battery is  $\leq 3.5$  W/kg, testing of all other required channels is not necessary.
12. When the SAR of an antenna tested on the highest output power using the default battery is  $> 3.5$  W/Kg and  $\leq 4.0$  W/Kg, testing of the immediately adjacent channel(s) is not necessary, but testing of other required channels may still be required.
13. When the SAR for all antennas tested using the default battery  $\leq 4.0$  W/kg, test additional batteries using the antenna and channel configuration that resulted in the highest SAR.
14. When the SAR of an antenna tested on the highest output power channel using the default battery is  $> 4.0$  W/kg and  $\leq 6.0$  W/kg, testing of the required immediately adjacent channel(s) is necessary. For the remaining channels that cannot be excluded, this rule may be applied recursively with respect to the highest output power channel among the remaining channels.
15. Based on the SAR measured in the body-worn test sequence with default audio accessory, if the SAR for the antenna, body-worn accessory and battery combination(s) applicable to an audio accessory is/are  $> 4.0$  W/kg and  $< 6.0$  W/kg, test that audio accessory using the highest body-worn SAR combination (antenna, battery and body-worn accessory) and channel configuration previously identified that is applicable to the audio accessory.
16. When the SAR of an antenna tested is  $> 6.0$  W/kg, test that battery and antenna combination with the default body-worn and audio accessory on the required immediately adjacent channels.
17. If the SAR measured  $> 7.0$  W/kg, test that battery, antenna, body-worn and audio accessory combination on all required channels.

## 13. MEASUREMENT UNCERTAINTY

### Measurement Uncertainty for DUT SAR test

<b>a</b>	<b>c</b>	<b>d</b>	<b>e</b>	<b>f</b>	<b>g</b>	<b><math>h = c \times f / e</math></b>	<b><math>i = c \times g / e</math></b>	<b><math>k</math></b>
<b>Source of uncertainty</b>	<b>Uncertainty ± %</b>	<b>Probability distribution</b>	<b>Div.</b>	<b><math>c_i</math></b>	<b><math>c_i</math></b>	<b>Standard Uncertainty</b>	<b>Standard Uncertainty</b>	<b><math>v_i</math> or <math>v_{eff}</math></b>
<b>Measurement system</b>								
Probe calibration	6.65	N	1	1	1	6.65	6.65	$\infty$
Axial isotropy	4.70	R	1.73	0.71	0.71	1.92	1.92	$\infty$
Hemispherical isotropy	9.60	R	1.73	0.71	0.71	3.92	3.92	$\infty$
Boundary effect	2.00	R	1.73	1	1	1.15	1.15	$\infty$
Linearity	4.70	R	1.73	1	1	2.71	2.71	$\infty$
Detection limits	1.00	R	1.73	1	1	0.58	0.58	$\infty$
Readout electronics	0.30	N	1	1	1	0.30	0.30	$\infty$
Response time	0.80	R	1.73	1	1	0.46	0.46	$\infty$
Integration time	2.60	R	1.73	1	1	1.50	1.50	$\infty$
RF ambient conditions - noise	3.00	R	1.73	1	1	1.73	1.73	$\infty$
RF ambient conditions - reflections	3.00	R	1.73	1	1	1.73	1.73	$\infty$
Probe positioner mechanical tolerance	0.80	R	1.73	1	1	0.46	0.46	$\infty$
Probe positioning with respect to phantom shell	6.70	R	1.73	1	1	3.87	3.87	$\infty$
Max. SAR Evaluation	4.00	R	1.73	1	1	2.31	2.31	$\infty$
<b>Test sample related</b>								
Test sample positioning	5.51	N	1	1	1	5.51	5.51	47
Device holder uncertainty	2.99	N	1	1	1	2.99	2.99	5
SAR drift measurement	5.00	R	1.73	1	1	2.89	2.89	$\infty$
SAR scaling	0.00	R	1.73	1	1	0.00	0.00	$\infty$
<b>Phantom and set-up</b>								
Phantom uncertainty (shape and thickness uncertainty)	7.60	R	1.73	1	1	4.39	4.39	$\infty$
Liquid conductivity (measured)	1.54	N	1	0.78	0.71	1.20	1.09	$\infty$
Liquid permittivity (measured)	1.17	N	1	0.23	0.26	0.22	0.25	$\infty$
Liquid conductivity (temperature uncert)	2.93	R	1.73	0.78	0.71	1.32	1.20	$\infty$
Liquid permittivity (temperature uncerta)	0.95	R	1.73	0.23	0.26	0.13	0.14	$\infty$
Liquid conductivity - deviation from targ	5.00	R	1.73	0.64	0.43	1.85	1.24	$\infty$
Liquid permittivity - deviation from targe	5.00	R	1.73	0.6	0.49	1.73	1.41	$\infty$
Combined standard uncertainty		RSS				13.34	13.21	$\infty$
<b>Expanded uncertainty (95% confidence interval)</b>		$k = 2$				<b>26.68</b>	<b>26.42</b>	

## 14. SAR TEST EQUIPMENT

Manufacturer	Type / Model	S/N	Calib. Date	Calib.Interval	Calib.Due
SPEAG	ELI Phantom	-	N/A	N/A	N/A
HP	SAR System Control PC	-	N/A	N/A	N/A
Staubli	Robot Controller CS8Cspeag-TX90	F10/5D1CA1/C/01	N/A	N/A	N/A
Staubli	Robot TX60 Lspeag	F10/5D1CA1/A/01	N/A	N/A	N/A
Staubli	Teach Pendant (Joystick)	D21142106	N/A	N/A	N/A
SPEAG	DAE4	1225	12/14/2017	Annual	12/14/2018
SPEAG	E-Field Probe EX3DV4	3863	05/31/2017	Annual	05/31/2018
SPEAG	D450V2	1007	07/18/2017	Annual	07/18/2018
Agilent	Power Meter N1911A	MY45101406	09/15/2017	Annual	09/15/2018
HP	Power Sensor N1921A	MY55220026	09/01/2017	Annual	09/01/2018
SPEAG	DAKS-3.5	1038	05/23/2017	Annual	05/23/2018
Agilent	Directional Bridge 86205A	3140A2914	05/10/2017	Annual	05/10/2018
HP	Signal Generator E4433B	US40052109	03/10/2017	Annual	03/10/2018
HP	11636B/Power Divider	58698	03/05/2017	Annual	03/05/2018
TESTO	175-H1/Thermometer	40331936309	02/06/2018	Annual	02/06/2019
EMPOWER	RF Power amplifier	1011	10/12/2017	Annual	10/12/2018
Agilent	Attenuator (3dB) 8491B	MY39270622	06/29/2017	Annual	06/29/2018
Agilent	Attenuator (20dB) 33340C	13311	05/10/2017	Annual	05/10/2018
HP	Notebook(DAKS)	-	N/A	N/A	N/A
HP	Dual Directional Coupler	16072	10/12/2017	Annual	10/12/2018
HP	Network Analyzer 8753ES	JP39240221	02/27/2017	Annual	02/27/2018
Aeroflex	Fixed Coaxial Attenuator (30dB)	CE6106	11/20/2017	Annual	11/20/2018

NOTE:

1. The E-field probe was calibrated by SPEAG, by the waveguide technique procedure. Dipole Verification measurement is performed by HCT Lab. before each test. The brain/body simulating material is calibrated by HCT using the DAKS 3.5 to determine the conductivity and permittivity (dielectric constant) of the brain/body-equivalent material.

## 15. CONCLUSION

The SAR measurement indicates that the EUT complies with the RF radiation exposure limits of the ANSI/IEEE C95.1- 2005.

These measurements are taken to simulate the RF effects exposure under worst-case conditions. Precise laboratory measures were taken to assure repeatability of the tests.

The SAR measurement indicates that the EUT complies with the RF radiation exposure limits of the FCC and Industry Canada. These measurements were taken to simulate the RF effects of RF exposure under worst-case conditions. Precise laboratory measures were taken to assure repeatability of the tests. The results and statements relate only to the item(s) tested.

## 16. REFERENCES

- [1] IEEE Standards Coordinating Committee 34 – IEEE Std. 1528-2013, IEEE Recommended Practice or Determining the Peak Spatial-Average Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices.
- [2] Federal Communications Commission, ET Docket 93-62, Guidelines for Evaluating the Environmental Effects of Radio frequency Radiation, Aug. 1996.
- [3] ANSI/IEEE C95.1 - 1991, American National Standard safety levels with respect to human exposure to radio frequency electromagnetic fields, 300 kHz to 100 GHz, New York: IEEE, Aug. 1992
- [4] ANSI/IEEE C 95.1 - 2005, American National Standard safety levels with respect to human exposure to radio frequency electromagnetic fields, 3 kHz to 300 GHz, New York: IEEE, 2006.
- [5] ANSI/IEEE C95.3 - 1991, IEEE Recommended Practice for the Measurement of Potentially Hazardous Electromagnetic Fields - RF and Microwave, New York: IEEE, 1992.
- [6] NCRP, National Council on Radiation Protection and Measurements, Biological Effects and Exposure Criteria for Radio Frequency Electromagnetic Fields, NCRP Report No. 86, 1986. Reprinted Feb. 1995.
- [7] T. Schmid, O. Egger, N. Kuster, Automated E-field scanning system for dosimetric assessments, IEEE Transaction on Microwave Theory and Techniques, vol. 44, Jan. 1996, pp. 105-113.
- [8] K. Pokovic, T. Schmid, N. Kuster, Robust setup for precise calibration of E-field probes in tissue simulating liquids at mobile communications frequencies, ICECOM97, Oct. 1997, pp. 120-124.
- [9] K. Pokovic, T. Schmid, and N. Kuster, E-field Probe with improved isotropy in brain simulating liquids, Proceedings of the ELMAR, Zadar, Croatia, June 23-25, 1996, pp. 172-175.
- [10] Schmid & Partner Engineering AG, Application Note: Data Storage and Evaluation, June 1998, p2.
- [11] V. Hombach, K. Meier, M. Burkhardt, E. Kuhn, N. Kuster, The Dependence of EM Energy Absorption upon Human Head Modeling at 900 MHz, IEEE Transaction on Microwave Theory and Techniques, vol. 44 no. 10, Oct. 1996, pp. 1865-1873.
- [12] N. Kuster and Q. Balzano, Energy absorption mechanism by biological bodies in the near field of dipole antennas above 300 MHz, IEEE Transaction on Vehicular Technology, vol. 41, no. 1, Feb. 1992, pp. 17-23.
- [13] G. Hartsgrove, A. Kraszewski, A. Surowiec, Simulated Biological Materials for Electromagnetic Radiation Absorption Studies, University of Ottawa, Bioelectromagnetics, Canada: 1987, pp. 29-36.
- [14] Q. Balzano, O. Garay, T. Manning Jr., Electromagnetic Energy Exposure of Simulated Users of Portable Cellular Telephones, IEEE Transactions on Vehicular Technology, vol. 44, no.3, Aug. 1995.
- [15] W. Gander, Computer mathematick, Birkhaeuser, Basel, 1992.
- [16] W.H. Press, S.A. Teukolsky, W.T. Vetterling, and B.P. Flannery, Numerical Receipes in C, The Art of Scientific Computing, Second edition, Cambridge University Press, 1992.
- [17] N. Kuster, R. Kastle, T. Schmid, Dosimetric evaluation of mobile communications equipment with known precision, IEEE Transaction on Communications, vol. E80-B, no. 5, May 1997, pp. 645-652.
- [18] CENELEC CLC/SC111B, European Prestandard (prENV 50166-2), Human Exposure to Electromagnetic Fields High-frequency: 10 kHz-300 GHz, Jan. 1995.
- [19] Prof. Dr. Niels Kuster, ETH, Eidgenössische Technische Hochschule Zürich, Dosimetric Evaluation of the Cellular Phone.
- [20] IEC 62209-1, Human exposure to radio frequency fields from hand-held and body-mounted wireless communication devices – Human models, instrumentation and procedures – Part 1:Procedure to determine the specific absorption rate (SAR) for hand-held devices used in close proximity to the ear (frequency range of 300 MHz to 3 GHz), Feb. 2005.

---

- [21] IEC 62209-2, Human exposure to radio frequency fields from hand-held and body-mounted wireless communication devices – Human models, instrumentation, and procedures – Part 2: Procedure to determine the specific absorption rate (SAR) for wireless communication devices used in close proximity to the human body (frequency range of 30 MHz to 6 GHz) Mar. 2010.
- [22] Industry Canada RSS-102 Radio Frequency Exposure Compliance of Radio communication Apparatus (All Frequency Band) Issue 5, March 2015.
- [23] Health Canada Safety Code 6 Limits of Human Exposure to Radio Frequency Electromagnetic Fields in the Frequency Range from 3 kHz – 300 GHz, 2009
- [24] FCC SAR Test procedures for 2G-3G Devices, Mobile Hotspot and UMPC Device KDB 941225 D01.
- [25] SAR Measurement Guidance for IEEE 802.11 transmitters, KDB 248227 D01v02r02
- [26] SAR Evaluation of Handsets with Multiple Transmitters and Antennas KDB 648474 D03, D04.
- [27] SAR Evaluation for Laptop, Notebook, Netbook and Tablet computers KDB 616217 D04.
- [28] SAR Measurement and Reporting Requirements for 100 MHz – 6 GHz, KDB 865664 D01, D02.
- [29] FCC General RF Exposure Guidance and SAR procedures for Dongles, KDB 447498 D01,D02.

## Attachment 1. – SAR Test Plots

Test Laboratory: HCT CO., LTD  
EUT Type: UHF DIGITAL TRANSCEIVER  
Liquid Temperature: 22.1 °C  
Ambient Temperature: 22.4 °C  
Test Date: 02/08/2018  
Plot No.: 1

**DUT: NX-P500-K**


Communication System: UID 0, UHF; Frequency: 460.05 MHz; Duty Cycle: 1:1  
Medium parameters used (interpolated):  $f = 460.05$  MHz;  $\sigma = 0.856$  S/m;  $\epsilon_r = 44.115$ ;  $\rho = 1000$  kg/m<sup>3</sup>  
Phantom section: Flat Section

DASY Configuration:

- Probe: EX3DV4 - SN3863; ConvF(11.04, 11.04, 11.04); Calibrated: 2017-05-31;
- Sensor-Surface: 1.4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn1225; Calibrated: 2017-12-14
- Phantom: ELI v4.0
- Measurement SW: DASY52, Version 52.8 (8);

**Hand-held to Face 11ch/Area Scan (6x14x1):** Measurement grid: dx=15mm, dy=15mm  
Maximum value of SAR (measured) = 2.09 W/kg

**Hand-held to Face 11ch/Zoom Scan (5x5x7)/Cube 0:** Measurement grid: dx=8mm, dy=8mm, dz=5mm  
Reference Value = 49.08 V/m; Power Drift = -0.51 dB  
Peak SAR (extrapolated) = 2.33 W/kg  
**SAR(1 g) = 1.55 W/kg; SAR(10 g) = 1.12 W/kg**  
Maximum value of SAR (measured) = 2.01 W/kg

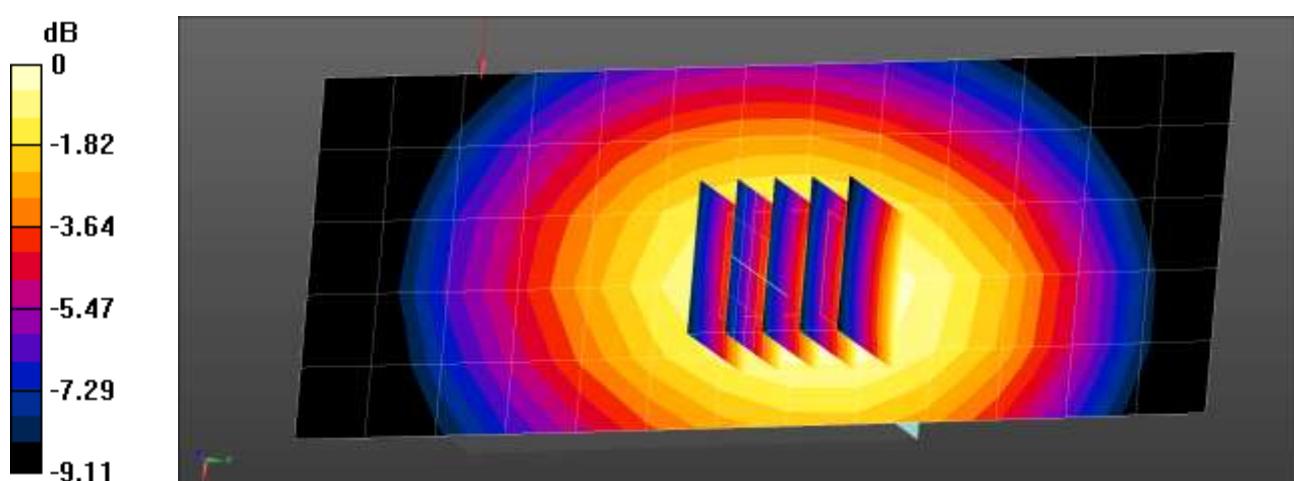

Test Laboratory: HCT CO., LTD  
EUT Type: UHF DIGITAL TRANSCEIVER  
Liquid Temperature: 23.5 °C  
Ambient Temperature: 23.9 °C  
Test Date: 02/19/2018  
Plot No.: 2

**DUT: NX-P500-K**

Communication System: UID 0, UHF; Frequency: 460.05 MHz; Duty Cycle: 1:1  
Medium parameters used (interpolated):  $f = 460.05$  MHz;  $\sigma = 0.961$  S/m;  $\epsilon_r = 55.324$ ;  $\rho = 1000$  kg/m<sup>3</sup>  
Phantom section: Flat Section

DASY Configuration:

- Probe: EX3DV4 - SN3863; ConvF(11.21, 11.21, 11.21); Calibrated: 2017-05-31;
- Sensor-Surface: 1.4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn1225; Calibrated: 2017-12-14
- Phantom: ELI v4.0
- Measurement SW: DASY52, Version 52.8 (8);

**Body-worn Belt clip KBH-20 11ch/Area Scan (6x14x1):** Measurement grid: dx=15mm, dy=15mm  
Maximum value of SAR (measured) = 2.99 W/kg


**Body-worn Belt clip KBH-20 11ch/Zoom Scan (5x5x7)/Cube 0:** Measurement grid: dx=8mm, dy=8mm, dz=5mm

Reference Value = 52.30 V/m; Power Drift = -0.37 dB

Peak SAR (extrapolated) = 3.57 W/kg

**SAR(1 g) = 2.31 W/kg; SAR(10 g) = 1.62 W/kg**

Maximum value of SAR (measured) = 3.07 W/kg

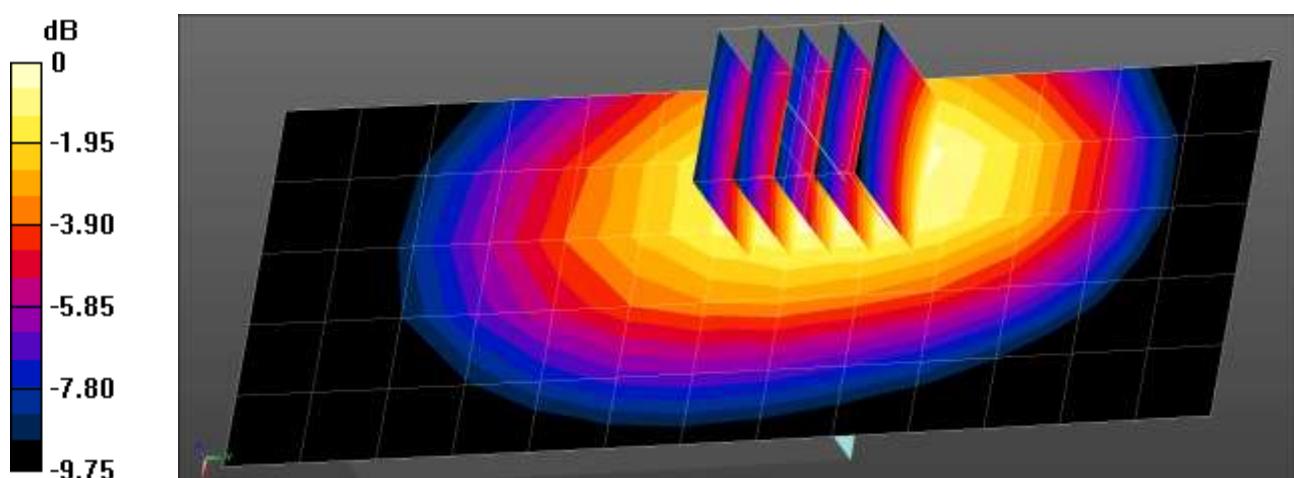

0 dB = 3.07 W/kg = 4.87 dBW/kg

Test Laboratory: HCT CO., LTD  
EUT Type: UHF DIGITAL TRANSCEIVER  
Liquid Temperature: 23.5 °C  
Ambient Temperature: 23.9 °C  
Test Date: 02/19/2018  
Plot No.: 3

**DUT: NX-P500-K**

Communication System: UID 0, UHF; Frequency: 460.05 MHz; Duty Cycle: 1:1  
Medium parameters used (interpolated):  $f = 460.05$  MHz;  $\sigma = 0.961$  S/m;  $\epsilon_r = 55.324$ ;  $\rho = 1000$  kg/m<sup>3</sup>  
Phantom section: Flat Section

DASY Configuration:

- Probe: EX3DV4 - SN3863; ConvF(11.21, 11.21, 11.21); Calibrated: 2017-05-31;
- Sensor-Surface: 1.4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn1225; Calibrated: 2017-12-14
- Phantom: ELI v4.0
- Measurement SW: DASY52, Version 52.8 (8);

**Body-worn Holster KBH-22 11ch/Area Scan (6x14x1):** Measurement grid: dx=15mm, dy=15mm  
Maximum value of SAR (measured) = 2.81 W/kg


**Body-worn Holster KBH-22 11ch/Zoom Scan (5x5x7)/Cube 0:** Measurement grid: dx=8mm, dy=8mm, dz=5mm

Reference Value = 51.96 V/m; Power Drift = -0.38 dB

Peak SAR (extrapolated) = 3.42 W/kg

**SAR(1 g) = 2.17 W/kg; SAR(10 g) = 1.53 W/kg**

Maximum value of SAR (measured) = 2.90 W/kg

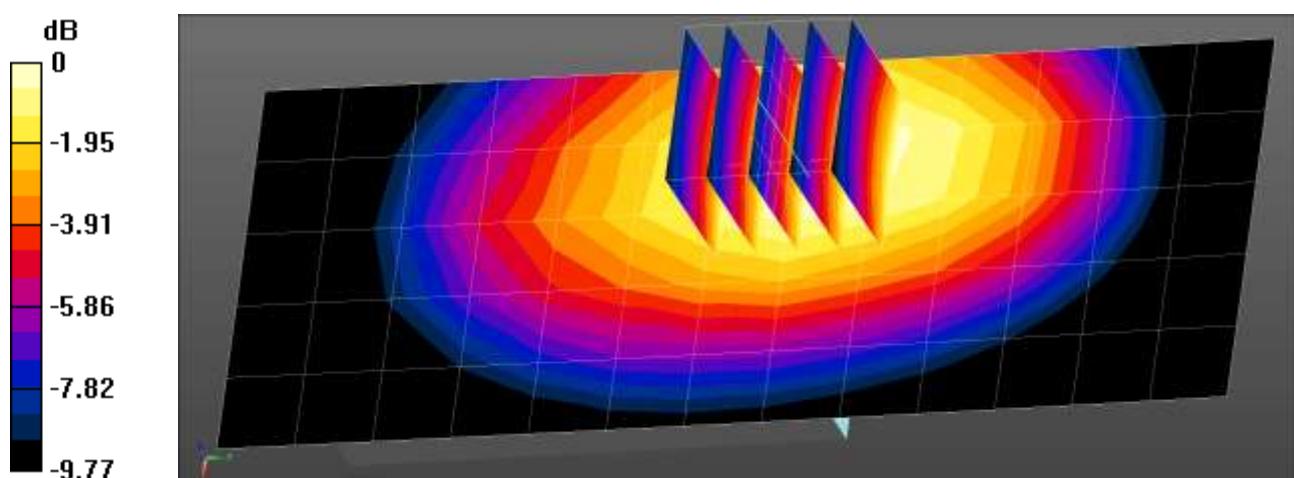

0 dB = 2.90 W/kg = 4.62 dBW/kg

## Attachment 2. – Dipole Verification Plots

## ■ Verification Data (450 MHz Head)

Test Laboratory: HCT CO., LTD

Input Power 100 mW (20 dBm)

Liquid Temp: 22.1 °C

Test Date: 02/08/2018

### **DUT: Dipole 450 MHz D450V2; Type: D450V2**

Communication System: UID 0, CW; Frequency: 450 MHz; Duty Cycle: 1:1

Medium parameters used:  $f = 450$  MHz;  $\sigma = 0.849$  S/m;  $\epsilon_r = 44.414$ ;  $\rho = 1000$  kg/m<sup>3</sup>

Phantom section: Flat Section

DASY Configuration:

- Probe: EX3DV4 - SN3863; ConvF(11.04, 11.04, 11.04); Calibrated: 2017-05-31;
- Sensor-Surface: 1.4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn1225; Calibrated: 2017-12-14
- Phantom: ELI v4.0
- Measurement SW: DASY52, Version 52.8 (8);

**Dipole/450 MHz Head Verification/Area Scan (7x18x1):** Measurement grid: dx=15mm, dy=15mm

Maximum value of SAR (measured) = 0.497 W/kg


**Dipole/450 MHz Head Verification/Zoom Scan (5x5x7)/Cube 0:** Measurement grid: dx=8mm, dy=8mm, dz=5mm

Reference Value = 24.35 V/m; Power Drift = -0.01 dB

Peak SAR (extrapolated) = 0.673 W/kg

**SAR(1 g) = 0.465 W/kg; SAR(10 g) = 0.316 W/kg**

Maximum value of SAR (measured) = 0.499 W/kg

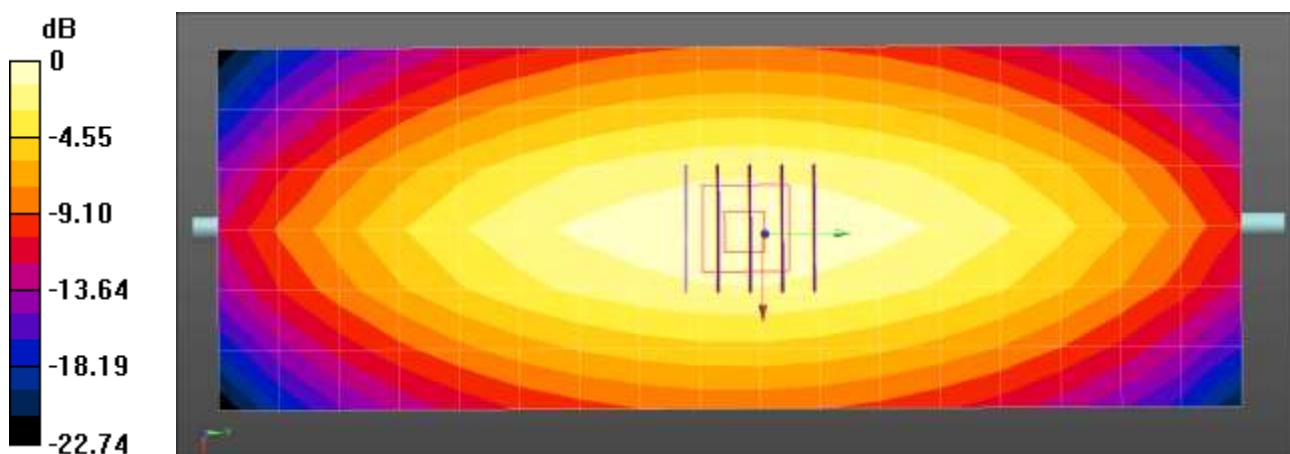

$$0 \text{ dB} = 0.497 \text{ W/kg} = -3.03 \text{ dBW/kg}$$

## ■ Verification Data (450 MHz Body)

Test Laboratory: HCT CO., LTD  
Input Power 100 mW (20 dBm)  
Liquid Temp: 23.5 °C  
Test Date: 02/19/2018

**DUT: Dipole 450 MHz D450V2; Type: D450V2**

Communication System: UID 0, CW; Frequency: 450 MHz; Duty Cycle: 1:1  
Medium parameters used:  $f = 450$  MHz;  $\sigma = 0.951$  S/m;  $\epsilon_r = 55.772$ ;  $\rho = 1000$  kg/m<sup>3</sup>  
Phantom section: Flat Section

DASY Configuration:

- Probe: EX3DV4 - SN3863; ConvF(11.21, 11.21, 11.21); Calibrated: 2017-05-31;
- Sensor-Surface: 1.4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn1225; Calibrated: 2017-12-14
- Phantom: ELI v4.0
- Measurement SW: DASY52, Version 52.8 (8);

**Dipole/450 MHz Body Verification/Area Scan (7x20x1):** Measurement grid: dx=15mm, dy=15mm  
Maximum value of SAR (measured) = 0.618 W/kg


**Dipole/450 MHz Body Verification/Zoom Scan (5x5x7)/Cube 0:** Measurement grid: dx=8mm, dy=8mm, dz=5mm

Reference Value = 25.73 V/m; Power Drift = -0.05 dB

Peak SAR (extrapolated) = 0.741 W/kg

**SAR(1 g) = 0.491 W/kg; SAR(10 g) = 0.329 W/kg**

Maximum value of SAR (measured) = 0.622 W/kg

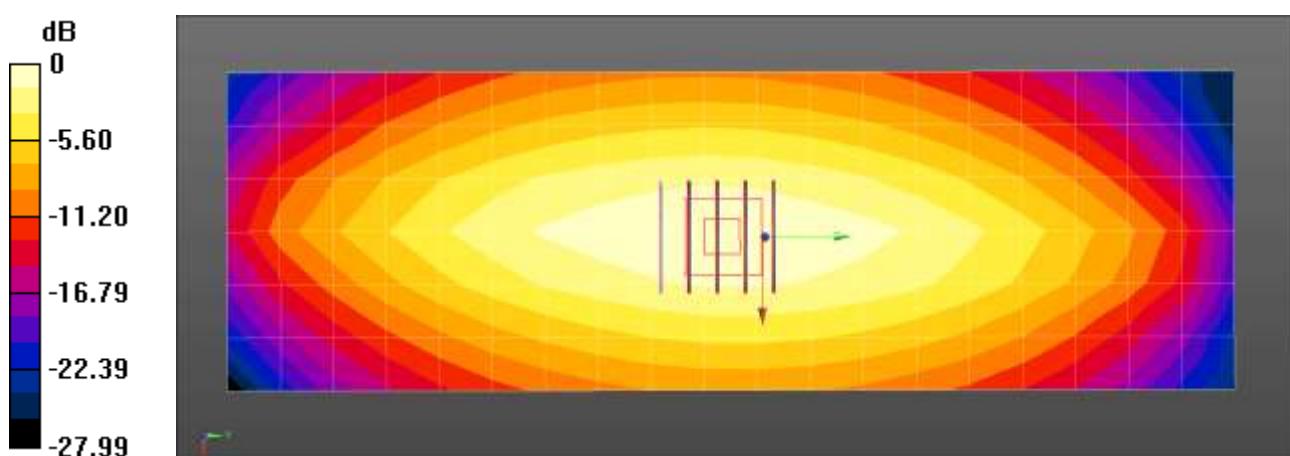

0 dB = 0.618 W/kg = -2.09 dBW/kg

## Attachment 3. – Probe Calibration Data

Calibration Laboratory of  
Schmid & Partner  
Engineering AG  
Zeughausstrasse 43, 8004 Zurich, Switzerland



S Schweizerischer Kalibrierdienst  
C Service suisse d'étalonnage  
S Servizio svizzero di taratura  
S Swiss Calibration Service

Accredited by the Swiss Accreditation Service (SAS)  
The Swiss Accreditation Service is one of the signatories to the EA  
Multilateral Agreement for the recognition of calibration certificates.

Accreditation No.: SCS 0108

Client: HCT (Dymstec)

Certificate No: EX3-3863\_May17

## CALIBRATION CERTIFICATE

Object: EX3DV4 - SN:3863

Calibration procedure(s): QA CAL-01.v9, QA CAL-12.v9, QA CAL-14.v4, QA CAL-23.v5,  
QA CAL-25.v6  
Calibration procedure for dosimetric E-field probes

Calibration date: May 31, 2017

This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI). The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility: environment temperature ( $22 \pm 3$ )°C and humidity < 70%.

Calibration Equipment used (M&amp;TE critical for calibration)

Primary Standards	ID	Cal Date (Certificate No.)	Scheduled Calibration
Power meter NRP	SN: 104778	04-Apr-17 (No. 217-02521/02522)	Apr-18
Power sensor NRP-Z91	SN: 103244	04-Apr-17 (No. 217-02521)	Apr-18
Power sensor NRP-Z91	SN: 103245	04-Apr-17 (No. 217-02525)	Apr-18
Reference 20 dB Attenuator	SN: SS277 (20x)	07-Apr-17 (No. 217-02528)	Apr-18
Reference Probe ES3DV2	SN: 3013	31-Dec-16 (No. ES3-3013_Dec16)	Dec-17
DAE4	SN: 660	7-Dec-16 (No. DAE4-660_Dec16)	Dec-17
Secondary Standards	ID	Check Date (in house)	Scheduled Check
Power meter E4419B	SN: GB41293874	06-Apr-16 (in house check Jun-16)	In house check: Jun-18
Power sensor E4412A	SN: MY41498087	06-Apr-16 (in house check Jun-16)	In house check: Jun-18
Power sensor E4412A	SN: 000110210	06-Apr-16 (in house check Jun-16)	In house check: Jun-18
RF generator HP 8648C	SN: US3642U01700	04-Aug-99 (in house check Jun-16)	In house check: Jun-18
Network Analyzer HP 8753E	SN: US37390585	18-Oct-01 (in house check Oct-16)	In house check: Oct-17

Calibrated by:	Name	Function	Signature
	Michael Weber	Laboratory Technician	
Approved by:	Kalja Pokovic	Technical Manager	

Issued: May 31, 2017

This calibration certificate shall not be reproduced except in full without written approval of the laboratory.

Certificate No: EX3-3863\_May17

Page 1 of 38

**Calibration Laboratory of**  
Schmid & Partner  
Engineering AG  
Zeughausstrasse 43, 8004 Zurich, Switzerland



**S** Schweizerischer Kalibrierdienst  
**C** Service suisse d'étalonnage  
**S** Servizio svizzero di taratura  
**S** Swiss Calibration Service

Accredited by the Swiss Accreditation Service (SAS).  
The Swiss Accreditation Service is one of the signatories to the EA  
Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: **SCS 0108**

#### Glossary:

TSL	tissue simulating liquid
NORM $x, y, z$	sensitivity in free space
ConvF	sensitivity in TSL / NORM $x, y, z$
DCP	diode compression point
CF	crest factor (1/duty_cycle) of the RF signal
A, B, C, D	modulation dependent linearization parameters
Polarization $\varphi$	$\varphi$ rotation around probe axis
Polarization $\theta$	$\theta$ rotation around an axis that is in the plane normal to probe axis (at measurement center), i.e., $\theta = 0$ is normal to probe axis
Connector Angle	information used in DASY system to align probe sensor X to the robot coordinate system

#### Calibration is Performed According to the Following Standards:

- IEEE Std 1528-2013, "IEEE Recommended Practice for Determining the Peak Spatial-Averaged Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques", June 2013
- IEC 62209-1, "Procedure to measure the Specific Absorption Rate (SAR) for hand-held devices used in close proximity to the ear (frequency range of 300 MHz to 3 GHz)", February 2005
- IEC 62209-2, "Procedure to determine the Specific Absorption Rate (SAR) for wireless communication devices used in close proximity to the human body (frequency range of 30 MHz to 6 GHz)", March 2010
- KDB 865664, "SAR Measurement Requirements for 100 MHz to 6 GHz"

#### Methods Applied and Interpretation of Parameters:

- $NORM $x, y, z$$ : Assessed for E-field polarization  $\theta = 0$  ( $f \leq 900$  MHz in TEM-cell;  $f > 1800$  MHz: R22 waveguide).  $NORM $x, y, z$$  are only intermediate values, i.e., the uncertainties of  $NORM $x, y, z$  does not affect the E'-field uncertainty inside TSL (see below ConvF).$
- $NORM(f)x, y, z = NORM $x, y, z * frequency_response$$  (see Frequency Response Chart). This linearization is implemented in DASY4 software versions later than 4.2. The uncertainty of the frequency response is included in the stated uncertainty of ConvF.
- $DCPx, y, z$ : DCP are numerical linearization parameters assessed based on the data of power sweep with CW signal (no uncertainty required). DCP does not depend on frequency nor media.
- $PAR$ : PAR is the Peak to Average Ratio that is not calibrated but determined based on the signal characteristics.
- $Ax, y, z; Bx, y, z; Cx, y, z; Dx, y, z; VRx, y, z$ : A, B, C, D are numerical linearization parameters assessed based on the data of power sweep for specific modulation signal. The parameters do not depend on frequency nor media. VR is the maximum calibration range expressed in RMS voltage across the diode.
- ConvF and Boundary Effect Parameters:** Assessed in flat phantom using E-field (or Temperature Transfer Standard for  $f \leq 800$  MHz) and inside waveguide using analytical field distributions based on power measurements for  $f > 800$  MHz. The same setups are used for assessment of the parameters applied for boundary compensation (alpha, depth) of which typical uncertainty values are given. These parameters are used in DASY4 software to improve probe accuracy close to the boundary. The sensitivity in TSL corresponds to  $NORM $x, y, z * ConvF$  whereby the uncertainty corresponds to that given for ConvF. A frequency dependent ConvF is used in DASY version 4.4 and higher which allows extending the validity from  $\pm 50$  MHz to  $\pm 100$  MHz.$
- Spherical Isotropy (3D deviation from isotropy):** in a field of low gradients realized using a flat phantom exposed by a patch antenna.
- Sensor Offset:** The sensor offset corresponds to the offset of virtual measurement center from the probe tip (on probe axis). No tolerance required.
- Connector Angle:** The angle is assessed using the information gained by determining the  $NORMx$  (no uncertainty required).

EX3DV4 – SN:3863

May 31, 2017

# Probe EX3DV4

## SN:3863

Manufactured: February 2, 2012  
Calibrated: May 31, 2017

Calibrated for DASY/EASY Systems  
(Note: non-compatible with DASY2 system!)

EX3DV4- SN:3863

May 31, 2017

**DASY/EASY - Parameters of Probe: EX3DV4 - SN:3863****Basic Calibration Parameters**

	Sensor X	Sensor Y	Sensor Z	Unc (k=2)
Norm ( $\mu$ V/(V/m)) <sup>A</sup>	0.34	0.33	0.44	$\pm 10.1\%$
DCP (mV) <sup>B</sup>	101.1	102.4	100.9	

**Modulation Calibration Parameters**

UID	Communication System Name		A dB	B dB $\sqrt{\mu$ V}	C	D dB	VR mV	Unc <sup>C</sup> (k=2)
0	CW	X	0.0	0.0	1.0	0.00	147.1	$\pm 3.3\%$
		Y	0.0	0.0	1.0		145.9	
		Z	0.0	0.0	1.0		138.9	

Note: For details on UID parameters see Appendix.

**Sensor Model Parameters**

	C1 fF	C2 fF	$\alpha$ V <sup>-1</sup>	T1 ms.V <sup>-2</sup>	T2 ms.V <sup>-1</sup>	T3 ms	T4 V <sup>-2</sup>	T5 V <sup>-1</sup>	T6
X	48.92	362.8	35.32	16.71	1.368	4.938	0.184	0.531	1.004
Y	21.91	161.9	35.16	6.73	0.877	4.912	0.044	0.199	0.999
Z	47.91	359.6	35.94	16.51	1.333	4.972	0.849	0.481	1.006

The reported uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor k=2, which for a normal distribution corresponds to a coverage probability of approximately 95%.

<sup>A</sup> The uncertainties of Norm X,Y,Z do not affect the E<sup>2</sup>-field uncertainty inside TSL (see Pages 5 and 6).<sup>B</sup> Numerical linearization parameter; uncertainty not required.<sup>C</sup> Uncertainty is determined using the max. deviation from linear response applying rectangular distribution and is expressed for the square of the field value.

EX3DV4- SN:3863

May 31, 2017

## DASY/EASY - Parameters of Probe: EX3DV4 - SN:3863

Calibration Parameter Determined in Head Tissue Simulating Media

f (MHz) <sup>c</sup>	Relative Permittivity <sup>f</sup>	Conductivity (S/m) <sup>f</sup>	ConvF X	ConvF Y	ConvF Z	Alpha <sup>g</sup>	Depth <sup>g</sup> (mm)	Unc (k=2)
150	52.3	0.76	12.83	12.83	12.83	0.00	1.00	± 13.3 %
300	45.3	0.87	11.88	11.88	11.88	0.08	1.20	± 13.3 %
450	43.5	0.87	11.04	11.04	11.04	0.13	1.25	± 13.3 %
750	41.9	0.89	10.75	10.75	10.75	0.51	0.87	± 12.0 %
835	41.5	0.90	10.44	10.44	10.44	0.54	0.83	± 12.0 %
900	41.5	0.97	10.33	10.33	10.33	0.50	0.80	± 12.0 %
1450	40.5	1.20	9.07	9.07	9.07	0.34	0.80	± 12.0 %
1750	40.1	1.37	8.63	8.63	8.63	0.36	0.83	± 12.0 %
1900	40.0	1.40	8.38	8.38	8.38	0.38	0.80	± 12.0 %
2300	39.5	1.67	8.11	8.11	8.11	0.35	0.80	± 12.0 %
2450	39.2	1.80	7.79	7.79	7.79	0.27	0.85	± 12.0 %
2600	39.0	1.96	7.62	7.62	7.62	0.38	0.85	± 12.0 %
5250	35.9	4.71	5.15	5.15	5.15	0.40	1.80	± 13.1 %
5600	35.5	5.07	4.91	4.91	4.91	0.40	1.80	± 13.1 %
5750	35.4	5.22	5.12	5.12	5.12	0.40	1.80	± 13.1 %

<sup>c</sup> Frequency validity above 300 MHz of ± 100 MHz only applies for DASY v4.4 and higher (see Page 2), else it is restricted to ± 50 MHz. The uncertainty is the RSS of the ConvF uncertainty at calibration frequency and the uncertainty for the indicated frequency band. Frequency validity below 300 MHz is ± 10, 25, 40, 50 and 70 MHz for ConvF assessments at 30, 64, 128, 150 and 220 MHz respectively. Above 5 GHz frequency validity can be extended to ± 110 MHz.

<sup>f</sup> At frequencies below 3 GHz, the validity of tissue parameters ( $\epsilon$  and  $\sigma$ ) can be relaxed to ± 10% if liquid compensation formula is applied to measured SAR values. At frequencies above 3 GHz, the validity of tissue parameters ( $\epsilon$  and  $\sigma$ ) is restricted to ± 5%. The uncertainty is the RSS of the ConvF uncertainty for indicated target tissue parameters.

<sup>g</sup> Alpha/Depth are determined during calibration. SPEAG warrants that the remaining deviation due to the boundary effect after compensation is always less than ± 1% for frequencies below 3 GHz and below ± 2% for frequencies between 3-6 GHz at any distance larger than half the probe tip diameter from the boundary.

EX3DV4- SN:3863

May 31, 2017

## DASY/EASY - Parameters of Probe: EX3DV4 - SN:3863

Calibration Parameter Determined in Body Tissue Simulating Media

f (MHz) <sup>c</sup>	Relative Permittivity <sup>e</sup>	Conductivity (S/m) <sup>f</sup>	ConvF X	ConvF Y	ConvF Z	Alpha <sup>g</sup>	Depth <sup>h</sup> (mm)	Unc (k=2)
150	61.9	0.80	12.34	12.34	12.34	0.00	1.00	± 13.3 %
300	58.2	0.92	11.41	11.41	11.41	0.04	1.25	± 13.3 %
450	56.7	0.94	11.21	11.21	11.21	0.08	1.25	± 13.3 %
750	55.5	0.96	10.26	10.26	10.26	0.40	0.97	± 12.0 %
835	55.2	0.97	9.90	9.90	9.90	0.36	0.98	± 12.0 %
1750	53.4	1.49	8.49	8.49	8.49	0.33	0.94	± 12.0 %
1900	53.3	1.52	8.14	8.14	8.14	0.34	0.93	± 12.0 %
2300	52.9	1.81	8.09	8.09	8.09	0.33	0.89	± 12.0 %
2450	52.7	1.95	7.93	7.93	7.93	0.37	0.85	± 12.0 %
2600	52.5	2.16	7.70	7.70	7.70	0.16	1.05	± 12.0 %
5250	48.9	5.36	4.80	4.80	4.80	0.40	1.90	± 13.1 %
5600	48.5	5.77	4.18	4.18	4.18	0.40	1.90	± 13.1 %
5750	48.3	5.94	4.48	4.48	4.48	0.45	1.90	± 13.1 %


<sup>c</sup> Frequency validity above 300 MHz of ± 100 MHz only applies for DASY v4.4 and higher (see Page 2), else it is restricted to ± 50 MHz. The uncertainty is the RSS of the ConvF uncertainty at calibration frequency and the uncertainty for the indicated frequency band. Frequency validity below 300 MHz is ± 10, 25, 40, 50 and 70 MHz for ConvF assessments at 30, 64, 128, 150 and 220 MHz respectively. Above 5 GHz frequency validity can be extended to ± 110 MHz.

<sup>e</sup> At frequencies below 3 GHz, the validity of tissue parameters (ε and σ) can be relaxed to ± 10% if liquid compensation formula is applied to measured SAR values. At frequencies above 3 GHz, the validity of tissue parameters (ε and σ) is restricted to ± 5%. The uncertainty is the RSS of the ConvF uncertainty for indicated target tissue parameters.

<sup>g</sup> Alpha/Depth are determined during calibration, SPEAG warrants that the remaining deviation due to the boundary effect after compensation is always less than ± 1% for frequencies below 3 GHz and below ± 2% for frequencies between 3-6 GHz at any distance larger than half the probe tip diameter from the boundary.

EX3DV4- SN:3863

May 31, 2017

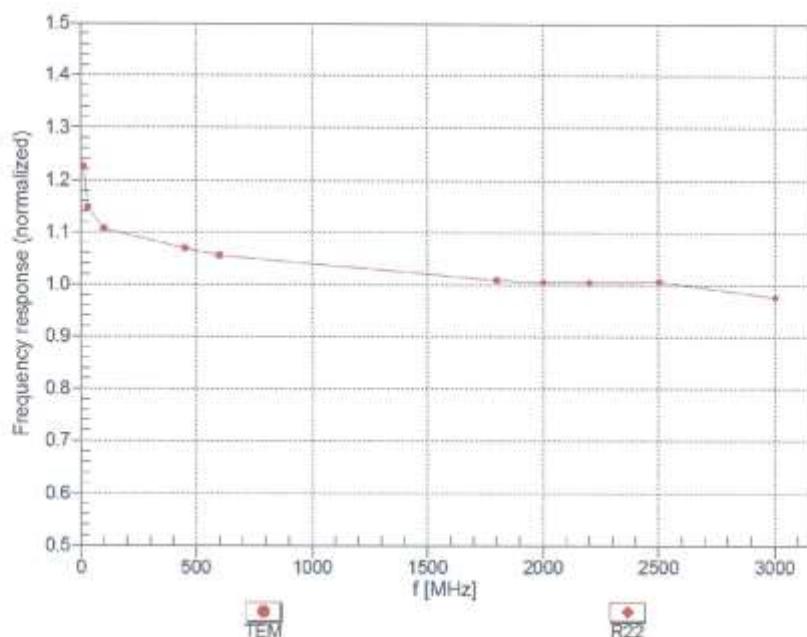
**Frequency Response of E-Field**  
(TEM-Cell:if110 EXX, Waveguide: R22)Uncertainty of Frequency Response of E-field:  $\pm 6.3\%$  ( $k=2$ )

EX3DV4- SN:3863



May 31, 2017

**Receiving Pattern ( $\phi$ ),  $\theta = 0^\circ$** 

f=600 MHz, TEM


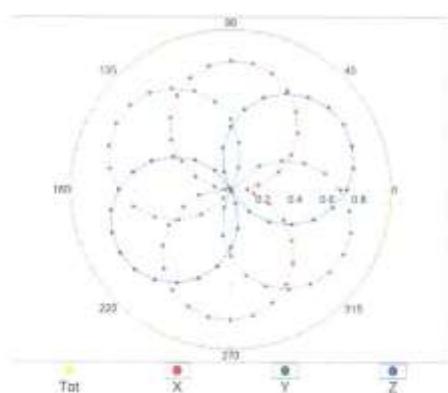


f=1800 MHz, R22

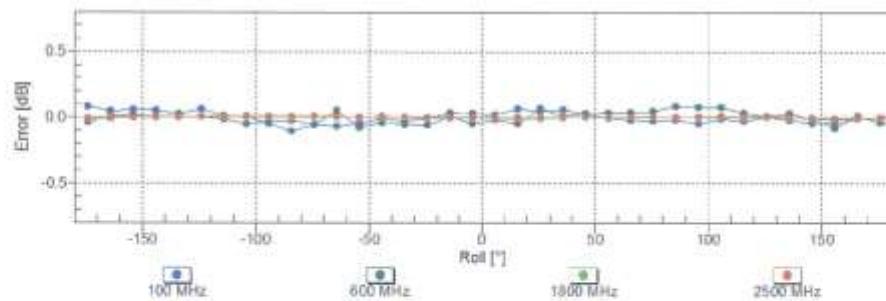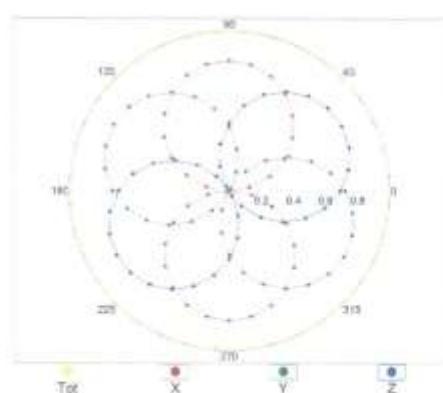Uncertainty of Axial Isotropy Assessment:  $\pm 0.5\%$  ( $k=2$ )

EX3DV4- SN3863


May 31, 2017

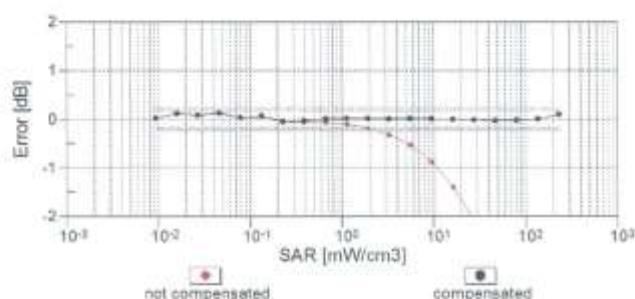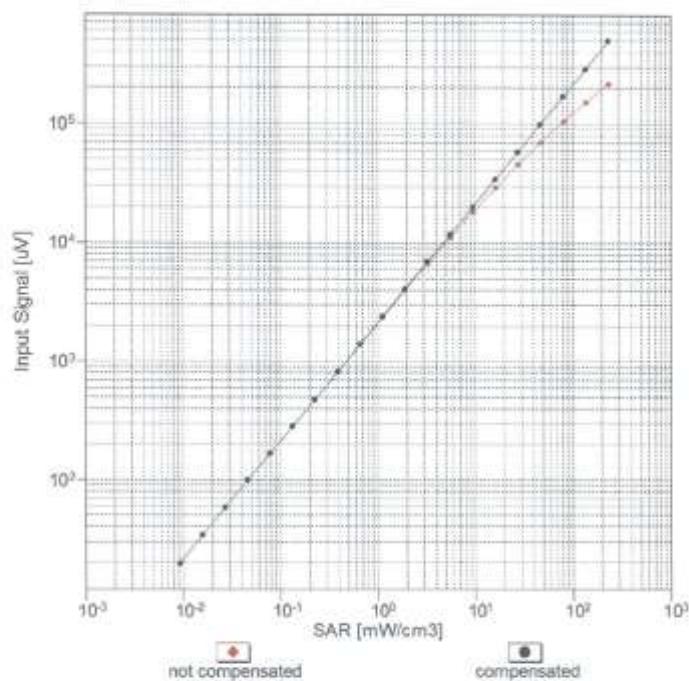**Dynamic Range f(SAR<sub>head</sub>)**  
(TEM cell , f<sub>oval</sub>= 1900 MHz)Uncertainty of Linearity Assessment:  $\pm 0.6\%$  ( $k=2$ )

EX3DV4- SN:3863


May 31, 2017

## Conversion Factor Assessment

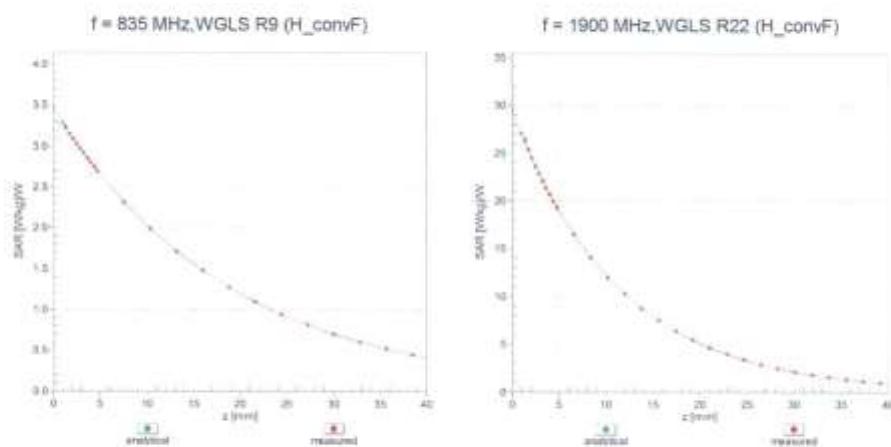

## Deviation from Isotropy in Liquid

Error ( $\phi, \theta$ ),  $f = 900$  MHz

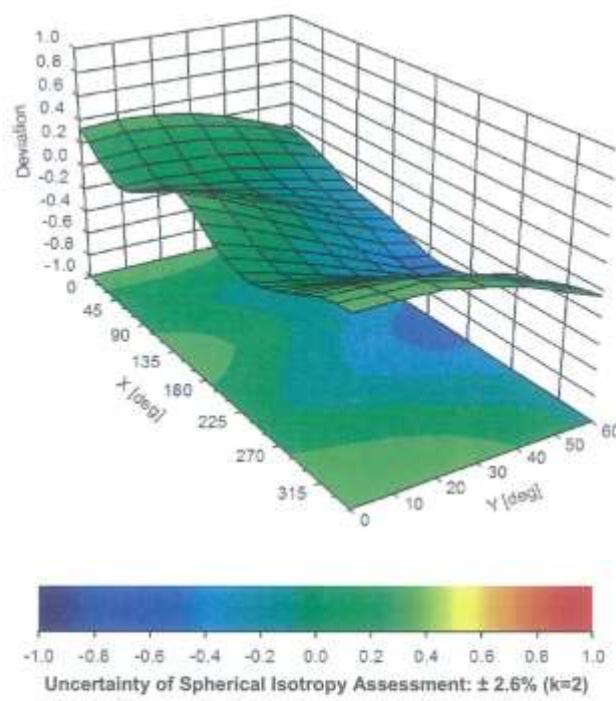

EX3DV4- SN:3863

May 31, 2017

**DASY/EASY - Parameters of Probe: EX3DV4 - SN:3863****Other Probe Parameters**

Sensor Arrangement	Triangular
Connector Angle (")	105.8
Mechanical Surface Detection Mode	enabled
Optical Surface Detection Mode	disabled
Probe Overall Length	337 mm
Probe Body Diameter	10 mm
Tip Length	9 mm
Tip Diameter	2.5 mm
Probe Tip to Sensor X Calibration Point	1 mm
Probe Tip to Sensor Y Calibration Point	1 mm
Probe Tip to Sensor Z Calibration Point	1 mm
Recommended Measurement Distance from Surface	1.4 mm

## Attachment 4. – Dipole Calibration Data

**Calibration Laboratory of**  
**Schmid & Partner**  
**Engineering AG**  
**Zeughausstrasse 43, 8004 Zurich, Switzerland**



**S** Schweizerischer Kalibrierdienst  
**C** Service suisse d'étalonnage  
**S** Servizio svizzero di taratura  
**S** Swiss Calibration Service

Accredited by the Swiss Accreditation Service (SAS)  
The Swiss Accreditation Service is one of the signatories to the EA  
Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: SCS 0108

Client **HCT (Dymstec)**

Certificate No: D450V2-1007\_Jul17

## CALIBRATION CERTIFICATE

Object **D450V2 - SN: 1007**

Calibration procedure(s) **QA CAL-15.v8**  
Calibration procedure for dipole validation kits below 700 MHz

Calibration date: **July 18, 2017**

This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI).  
The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility: environment temperature (22 ± 3)°C and humidity < 70%.

Calibration Equipment used (M&TE critical for calibration)

Primary Standards	ID #	Cal Date (Certificate No.)	Scheduled Calibration
Power meter NRP	SN: 104778	04-Apr-17 (No. 217-02521/02522)	Apr-18
Power sensor NRP-Z91	SN: 103244	04-Apr-17 (No. 217-02521)	Apr-18
Power sensor NRP-Z91	SN: 103245	04-Apr-17 (No. 217-02522)	Apr-18
Reference 20 dB Attenuator	SN: 5277 (20x)	07-Apr-17 (No. 217-02528)	Apr-18
Type-N mismatch combination	SN: 5047.2 / 06327	07-Apr-17 (No. 217-02529)	Apr-18
Reference Probe EX3DV4	SN: 3877	31-Dec-16 (No. EX3-3877_Dec16)	Dec-17
DAE4	SN: 654	12-Aug-16 (No. DAE4-654_Aug16)	Aug-17
Secondary Standards	ID #	Check Date (in house)	Scheduled Check
Power meter E4419B	SN: GB41293874	06-Apr-16 (No. 217-02285/02284)	In house check: Jun-18
Power sensor E4412A	SN: MY41498057	06-Apr-16 (No. 217-02285)	In house check: Jun-18
Power sensor E4412A	SN: 000110210	06-Apr-16 (No. 217-02284)	In house check: Jun-18
RF generator HP 8648C	SN: US3642UD1700	04-Aug-99 (in house check Jun-16)	In house check: Jun-18
Network Analyzer HP 8753E	SN: US37390585	18-Oct-01 (in house check Oct-16)	In house check: Oct-17

Calibrated by:	Name	Function	Signature
	Michael Weber	Laboratory Technician	
Approved by:	Katja Pokovic	Technical Manager	

Issued: July 18, 2017

This calibration certificate shall not be reproduced except in full without written approval of the laboratory.

**Calibration Laboratory of**  
Schmid & Partner  
Engineering AG  
Zeughausstrasse 43, 8004 Zurich, Switzerland



**S** Schweizerischer Kalibrierdienst  
**C** Service suisse d'étalonnage  
**S** Servizio svizzero di taratura  
**S** Swiss Calibration Service

Accredited by the Swiss Accreditation Service (SAS)  
The Swiss Accreditation Service is one of the signatories to the EA  
Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: **SCS 0108**

**Glossary:**

TSL	tissue simulating liquid
ConvF	sensitivity in TSL / NORM x,y,z
N/A	not applicable or not measured

**Calibration is Performed According to the Following Standards:**

- a) IEEE Std 1528-2013, "IEEE Recommended Practice for Determining the Peak Spatial-Averaged Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques", June 2013
- b) IEC 62209-1, "Measurement procedure for the assessment of Specific Absorption Rate (SAR) from hand-held and body-mounted devices used next to the ear (frequency range of 300 MHz to 6 GHz)", July 2016
- c) IEC 62209-2, "Procedure to determine the Specific Absorption Rate (SAR) for wireless communication devices used in close proximity to the human body (frequency range of 30 MHz to 6 GHz)", March 2010
- d) KDB 865664, "SAR Measurement Requirements for 100 MHz to 6 GHz"

**Additional Documentation:**

- e) DASY4/5 System Handbook

**Methods Applied and Interpretation of Parameters:**

- *Measurement Conditions:* Further details are available from the Validation Report at the end of the certificate. All figures stated in the certificate are valid at the frequency indicated.
- *Antenna Parameters with TSL:* The dipole is mounted with the spacer to position its feed point exactly below the center marking of the flat phantom section, with the arms oriented parallel to the body axis.
- *Feed Point Impedance and Return Loss:* These parameters are measured with the dipole positioned under the liquid filled phantom. The impedance stated is transformed from the measurement at the SMA connector to the feed point. The Return Loss ensures low reflected power. No uncertainty required.
- *Electrical Delay:* One-way delay between the SMA connector and the antenna feed point. No uncertainty required.
- *SAR measured:* SAR measured at the stated antenna input power.
- *SAR normalized:* SAR as measured, normalized to an input power of 1 W at the antenna connector.
- *SAR for nominal TSL parameters:* The measured TSL parameters are used to calculate the nominal SAR result.

The reported uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor k=2, which for a normal distribution corresponds to a coverage probability of approximately 95%.

**Measurement Conditions**

DASY system configuration, as far as not given on page 1:

DASY Version	DASY5	V52.10.0
Extrapolation	Advanced Extrapolation	
Phantom	Flat Phantom V4.4	Shell thickness: 6 ± 0.2 mm
Distance Dipole Center - TSL	15 mm	with Spacer
Zoom Scan Resolution	dx, dy, dz. = 5 mm	
Frequency	450 MHz ± 1 MHz	

**Head TSL parameters**

The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Head TSL parameters	22.0 °C	43.5	0.87 mho/m
Measured Head TSL parameters	(22.0 ± 0.2) °C	43.6 ± 6 %	0.87 mho/m ± 6 %
Head TSL temperature change during test	< 0.5 °C	---	---

**SAR result with Head TSL**

SAR averaged over 1 cm <sup>3</sup> (1 g) of Head TSL	Condition	
SAR measured	250 mW input power	1.21 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	4.84 W/kg ± 18.1 % (k=2)

SAR averaged over 10 cm <sup>3</sup> (10 g) of Head TSL	Condition	
SAR measured	250 mW input power	0.803 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	3.21 W/kg ± 17.6 % (k=2)

**Body TSL parameters**

The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Body TSL parameters	22.0 °C	56.7	0.94 mho/m
Measured Body TSL parameters	(22.0 ± 0.2) °C	56.2 ± 6 %	0.93 mho/m ± 6 %
Body TSL temperature change during test	< 0.5 °C	---	---

**SAR result with Body TSL**

SAR averaged over 1 cm <sup>3</sup> (1 g) of Body TSL	Condition	
SAR measured	250 mW input power	1.18 W/kg
SAR for nominal Body TSL parameters	normalized to 1W	4.75 W/kg ± 18.1 % (k=2)

SAR averaged over 10 cm <sup>3</sup> (10 g) of Body TSL	Condition	
SAR measured	250 mW input power	0.785 W/kg
SAR for nominal Body TSL parameters	normalized to 1W	3.16 W/kg ± 17.6 % (k=2)

**Appendix (Additional assessments outside the scope of SCS 0108)****Antenna Parameters with Head TSL**

Impedance, transformed to feed point	55.6 $\Omega$ - 8.8 $j\Omega$
Return Loss	- 20.1 dB

**Antenna Parameters with Body TSL**

Impedance, transformed to feed point	53.5 $\Omega$ - 9.1 $j\Omega$
Return Loss	- 20.5 dB

**General Antenna Parameters and Design**

Electrical Delay (one direction)	1.355 ns
----------------------------------	----------

After long term use with 100W radiated power, only a slight warming of the dipole near the feedpoint can be measured.

The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals. On some of the dipoles, small end caps are added to the dipole arms in order to improve matching when loaded according to the position as explained in the "Measurement Conditions" paragraph. The SAR data are not affected by this change. The overall dipole length is still according to the Standard.

No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feedpoint may be damaged.

**Additional EUT Data**

Manufactured by	SPEAG
Manufactured on	February 14, 2013

**DASY5 Validation Report for Head TSL**

Date: 18.07.2017

Test Laboratory: SPEAG, Zurich, Switzerland

**DUT: Dipole 450 MHz; Type: D450V2; Serial: D450V2 - SN: 1007**

Communication System: UID 0 - CW; Frequency: 450 MHz

Medium parameters used:  $f = 450$  MHz;  $\sigma = 0.87$  S/m;  $\epsilon_r = 43.6$ ;  $\rho = 1000$  kg/m<sup>3</sup>

Phantom section: Flat Section

Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2011)

DASY52 Configuration:

- Probe: EX3DV4 - SN3877; ConvF(10.5, 10.5, 10.5); Calibrated: 31.12.2016;
- Sensor-Surface: 1.4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn654; Calibrated: 12.08.2016
- Phantom: Flat Phantom 4.4 ; Type: Flat Phantom 4.4; Serial: 1002
- DASY52 52.10.0(1446); SEMCAD X 14.6.10(7417)

**Dipole Calibration for Head Tissue/d=15mm, Pin=250mW/Zoom Scan (7x7x7)/Cube 0:**


Measurement grid: dx=5mm, dy=5mm, dz=5mm

Reference Value = 43.54 V/m; Power Drift = -0.00 dB


Peak SAR (extrapolated) = 1.86 W/kg

SAR(1 g) = 1.21 W/kg; SAR(10 g) = 0.803 W/kg

Maximum value of SAR (measured) = 1.63 W/kg

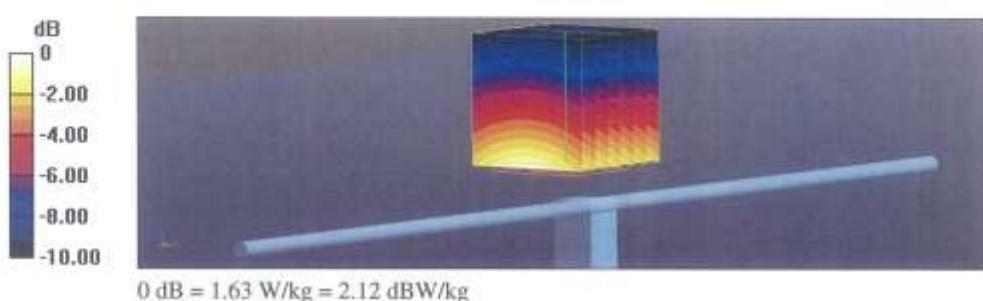

## Impedance Measurement Plot for Head TSL

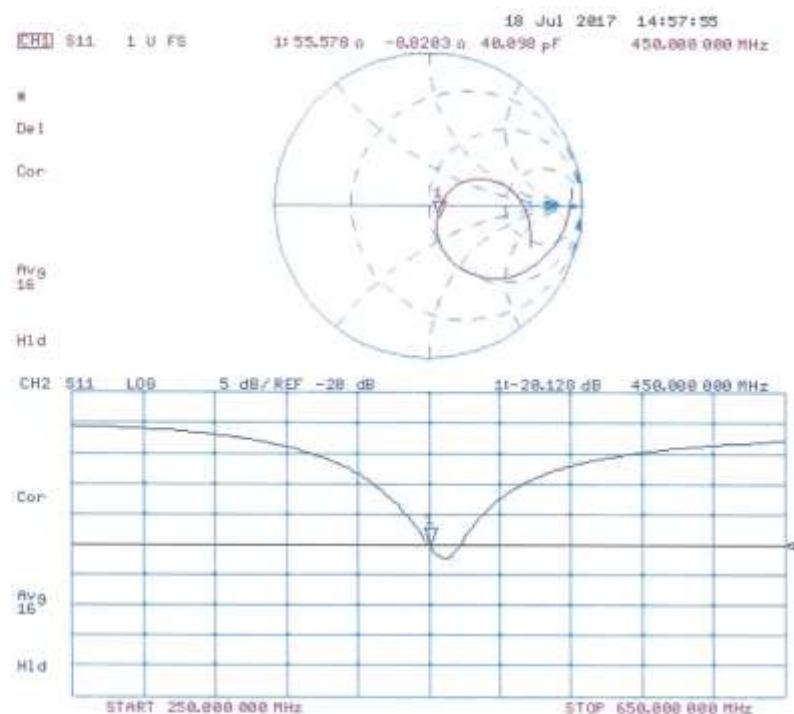

**DASY5 Validation Report for Body TSL**

Date: 18.07.2017

Test Laboratory: SPEAG, Zurich, Switzerland

**DUT: Dipole 450 MHz; Type: D450V2; Serial: D450V2 - SN: 1007**

Communication System: UID 0 - CW; Frequency: 450 MHz

Medium parameters used:  $f = 450$  MHz;  $\sigma = 0.93$  S/m;  $\epsilon_r = 56.2$ ;  $\rho = 1000$  kg/m<sup>3</sup>

Phantom section: Flat Section

Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2011)

DASY52 Configuration:

- Probe: EX3DV4 - SN3877; ConvF(10.7, 10.7, 10.7); Calibrated: 31.12.2016;
- Sensor-Surface: 1.4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn654; Calibrated: 12.08.2016
- Phantom: Flat Phantom 4.4 ; Type: Flat Phantom 4.4; Serial: 1002
- DASY52 52.10.0(1446); SEMCAD X 14.6.10(7417)

**Dipole Calibration for Body Tissue/d=15mm, Pin=250mW/Zoom Scan (7x7x7)/Cube 0:**


Measurement grid: dx=5mm, dy=5mm, dz=5mm

Reference Value = 41.32 V/m; Power Drift = -0.01 dB


Peak SAR (extrapolated) = 1.82 W/kg

SAR(1 g) = 1.18 W/kg; SAR(10 g) = 0.785 W/kg

Maximum value of SAR (measured) = 1.59 W/kg

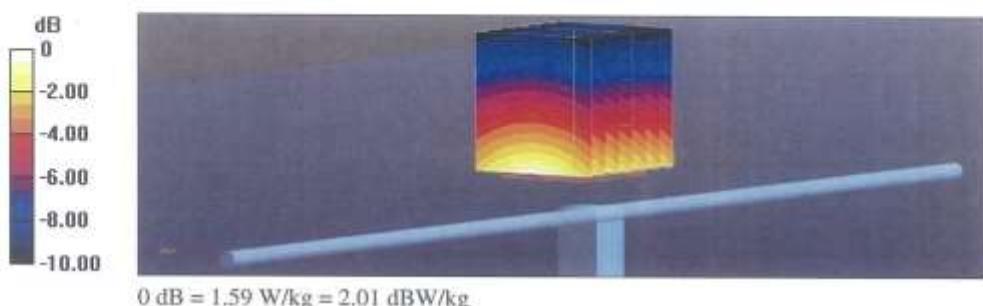

## Impedance Measurement Plot for Body TSL

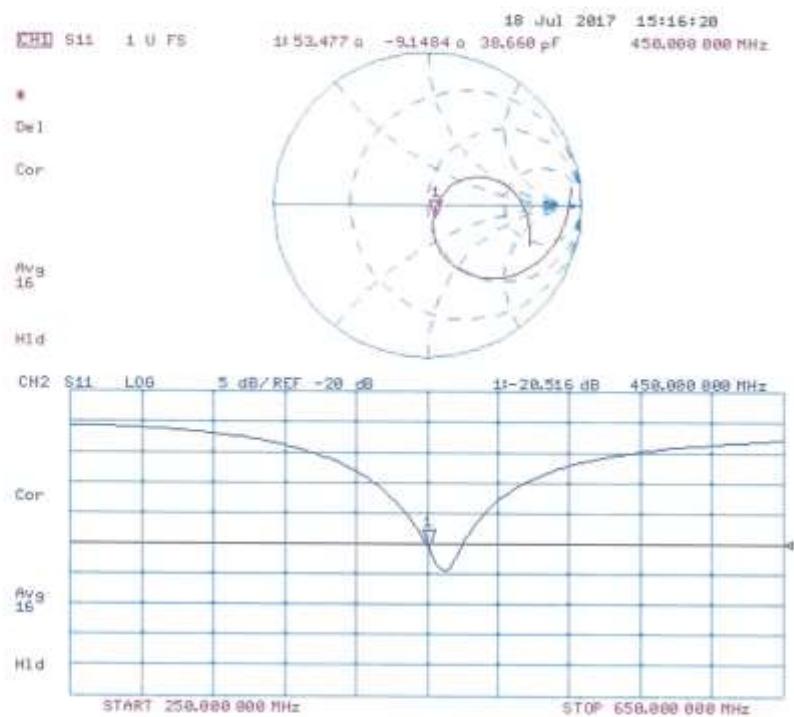

## Attachment 5. – SAR Tissue Characterization

The brain and muscle mixtures consist of a viscous gel using hydrox-ethyl cellulose (HEC) gelling agent and saline solution (see Table 3.1). Preservation with a bactericide is added and visual inspection is made to make sure air bubbles are not trapped during the mixing process. The mixture is calibrated to obtain proper dielectric constant (permittivity) and conductivity of the desired tissue. The mixture characterizations used for the brain and muscle tissue simulating liquids are according to the data by C. Gabriel and G. Hartsgrove.

Ingredients (% by weight)	Frequency (MHz)	
	450	
Tissue Type	Head	Body
Water	38.91 %	46.21 %
Salt (NaCl)	3.79 %	2.34 %
Sugar	56.93 %	51.17 %
HEC	0.25 %	0.18 %
Bactericide	0.12 %	0.08 %
Triton X-100	-	-
DGBE	-	-
Diethylene glycol hexyl ether	-	-

Salt: 99 % Pure Sodium Chloride      Sugar: 98 % Pure Sucrose  
Water: De-ionized, 16M resistivity      HEC: Hydroxyethyl Cellulose  
DGBE: 99 % Di(ethylene glycol) butyl ether,[2-(2-butoxyethoxy) ethanol]  
Triton X-100(ultra pure): Polyethylene glycol mono[4-(1,1,3,3-tetramethylbutyl)phenyl] ether

### Composition of the Tissue Equivalent Matter

## Attachment 6. – SAR SYSTEM VALIDATION

Per FCC KCB 865664 D02v01r02, SAR system validation status should be document to confirm measurement accuracy. The SAR systems (including SAR probes, system components and software versions) used for this device were validated against its performance specifications prior to the SAR measurements. Reference dipoles were used with the required tissue- equivalent media for system validation, according to the procedures outlined in IEEE 1528-2003 and FCC KDB 865664 D01v01r04. Since SAR probe calibrations are frequency dependent, each probe calibration point was validated at a frequency within the valid frequency range of the probe calibration point, using the system that normally operates with the probe for routine SAR measurements and according to the required tissue-equivalent media.

A tabulated summary of the system validation status including the validation date(s), measurement frequencies, SAR probes and tissue dielectric parameters has been included.

SAR System No.	Probe	Probe Type	Probe Calibration Point	Dipole	Date	Dielectric Parameters		CW Validation			Modulation Validation			
						Measured Permittivity	Measured Conductivity	Sensitivity	Probe Linearity	Probe Isotropy	MOD. Type	Duty Factor	PAR	
1	3863	EX3DV4	Head	450	1007	2017-08-16	43.6	0.86	PASS	PASS	PASS	N/A	N/A	N/A
1	3863	EX3DV4	Body	450	1007	2017-08-17	56.9	0.95	PASS	PASS	PASS	N/A	N/A	N/A

### SAR System Validation Summary

**Note:**

All measurement were performed using probes calibrated for CW signal only. Modulations in the table above represent test configurations for which the measurement system has been validated per FCC KDB Publication 865664 D01v01r04. SAR system were validated for modulated signals with a periodic duty cycle, such as GMSK, or with a high peak to average ratio (>5 dB), such as OFDM according to KDB 865664 D01v01r04.