



RF EXPOSURE LAB, LLC

2867 Progress Place, Suite 4D • Escondido, CA 92029 • U.S.A.

TEL (760) 737-3131 • FAX (760) 737-9131

<http://www.rfexposurelab.com>

CERTIFICATE OF COMPLIANCE SAR EVALUATION

LXE, Inc.
125 Technology Parkway
Norcross, GA 30092

Dates of Test: April 29-30, May 1, 2008
Test Report Number: SAR.20080409
Revision D

FCC ID:	KDZLXE4831P & KDZLXE001
IC Certificate:	1995B-4831 & 1995B-BT001
Model(s):	Host MX8 Containing Models 4831 & LMBA46NET2
Test Sample:	Production Unit
Serial No.:	MX8 Eng 1
Equipment Type:	Wireless Computer
Classification:	Portable Transmitter Next to Body
TX Frequency Range:	2412 – 2462 MHz, 5180 – 5240 MHz, 5260 – 5320 MHz, 5745 – 5805 MHz, 2402 – 2480 MHz
Frequency Tolerance:	± 25 ppm
Maximum RF Output:	2450 MHz (b) – 15.58 dBm, 2450 MHz (g) – 11.47 dBm, 5250 MHz – 12.93 dBm, 5800 MHz – 7.54 dBm Conducted
Signal Modulation:	DSSS, OFDM
Antenna Type (Length):	Left Antenna Part Number: SNE101898-E498 Right Antenna Part Number: SNE101899-E498
Battery:	LXE Part Number: 1613760001
Application Type:	Certification
FCC Rule Parts:	Part 15C
Industry Canada:	RSS-102

This wireless mobile and/or portable device has been shown to be compliant for localized specific absorption rate (SAR) for uncontrolled environment/general exposure limits specified in ANSI/IEEE Std. C95.1-1999 and had been tested in accordance with the measurement procedures specified in IEEE 1528-2003, OET Bulletin 65 Supp. C, RSS-102 and Safety Code 6 (See test report).

I attest to the accuracy of the data. All measurements were performed by myself or were made under my supervision and are correct to the best of my knowledge and belief. I assume full responsibility for the completeness of these measurements and vouch for the qualifications of all persons taking them.

RF Exposure Lab, LLC certifies that no party to this application has been denied FCC benefits pursuant to Section 5301 of the Anti-Drug Abuse Act of 1988, 21 U.S.C. 853(a).

Jay M. Moulton
Vice President



Certificate # 2387.01

Table of Contents

1.	Introduction	3
	SAR Definition [5].....	3
2.	SAR Measurement Setup	4
	Robotic System	4
	System Hardware	4
	System Description	4
	E-Field Probe	5
3.	Robot Specifications	7
4.	Probe and Dipole Calibration	8
5.	Phantom & Simulating Tissue Specifications.....	9
	SAM Phantom.....	9
	Brain & Muscle Simulating Mixture Characterization	9
	Device Holder	9
6.	Definition of Reference Points.....	10
	Ear Reference Point.....	10
	Device Reference Points	10
7.	Test Configuration Positions	11
	Positioning for Cheek/Touch [5].....	11
	Positioning for Ear / 15° Tilt [5].....	12
	Body Worn Configurations	13
8.	ANSI/IEEE C95.1 – 1999 RF Exposure Limits [2].....	14
	Uncontrolled Environment.....	14
	Controlled Environment	14
9.	Measurement Uncertainty	15
10.	System Validation	16
	Tissue Verification.....	16
	Test System Verification	16
11.	SAR Test Data Summary	17
	Procedures Used To Establish Test Signal.....	17
	Device Test Condition	17
	SAR Data Summary – 2450 MHz Body	19
	SAR Data Summary – 5200 MHz Body	20
	SAR Data Summary – 5800 MHz Body	21
	SAR Data Summary – 2450 MHz Bluetooth Body	22
12.1	Test Equipment List	23
13.1	Conclusion	24
14.1	References.....	25
	Appendix A – System Validation Plots and Data	26
	Appendix B – SAR Test Data Plots.....	40
	Appendix C – SAR Test Setup Photos	86
	Appendix D – Probe Calibration Data Sheets.....	92
	Appendix E – Dipole Calibration Data Sheets	133
	Appendix F – Phantom Calibration Data Sheets	156

1. Introduction

This measurement report shows compliance of the LXE, Inc. Model Host MX8 containing Model 4831 FCC ID: KDZLXE4831P and Model LMBA46NET2 FCC ID: KDZLXEBT001 with FCC Part 2, 1093, ET Docket 93-62 Rules for mobile and portable devices and IC Certificate: 1995B-4831 and IC Certificate: 1995B-BT001 with RSS102 & Safety Code 6. The FCC have adopted the guidelines for evaluating the environmental effects of radio frequency radiation in ET Docket 93-62 on August 6, 1996 to protect the public and workers from the potential hazards of RF emissions due to FCC regulated portable devices. [1], [6]

The testing of the WLAN was conducted April 29-30. The Bluetooth module was added after this testing was completed. The Bluetooth and the WLAN can transmit simultaneously. A question was posed to the FCC as to the requirement of having to conduct the Bluetooth measurement, and the FCC instructed that the measurement be conducted per KDB648474. The FCC response was documented in KDB802357. Therefore, the Bluetooth measurement was conducted on May 1 and the results were amended to the original report in this revision.

The test procedures, as described in ANSI C95.1 – 1999 Standard for Safety Levels with Respect to Human Exposure to Radio Frequency Electromagnetic Fields, 3 kHz to 300 GHz [2], ANSI C95.3 – 2002 Recommended Practice for the Measurement of Potentially Hazardous Electromagnetic Fields [3], FCC OET Bulletin 65 Supp. C – 2001 [4], IEEE Std.1528 – 2003 Recommended Practice [5], and Industry Canada Safety Code 6 Limits of Human Exposure to Radiofrequency Electromagnetic Fields in the Frequency Range from 3kHz to 300 GHz were employed.

SAR Definition [5]

Specific Absorption Rate is defined as the time derivative (rate) of the incremental energy (dW) absorbed by (dissipated in) an incremental mass (dm) contained in a volume element (dV) of a given density (ρ).

$$SAR = \frac{d}{dt} \left(\frac{dW}{dm} \right) = \frac{d}{dt} \left(\frac{dW}{\rho dV} \right)$$

SAR is expressed in units of watts per kilogram (W/kg). SAR can be related to the electric field at a point by

$$SAR = \frac{\sigma |E|^2}{\rho}$$

where:

σ = conductivity of the tissue (S/m)

ρ = mass density of the tissue (kg/m³)

E = rms electric field strength (V/m)

2. SAR Measurement Setup

Robotic System

The measurements are conducted utilizing the ALSAS-10-U automated dosimetric assessment system. The ALSAS-10-U is designed and manufactured by April Laboratories in Nepean, Ontario, Canada. The system utilizes a Robcomm 3 robot manufactured by ThermoCRS located in Michigan USA.

System Hardware

The system consists of a six axis articulated arm, controller for precise probe positioning (0.05 mm repeatability), a power supply, a teach pendant for teaching area scans, near field probe, an IBM Pentium 4™ 2.66 GHz PC with Windows XP Pro™, and custom software developed to enable communications between the robot controller software and the host operating system.

An amplifier is located on the articulated arm, which is isolated from the custom designed end effector and robot arm. The end effector provides the mechanical touch detection functionality and probe connection interface. The amplifier is functionally validated within the manufacturer's site and calibrated at NCL Calibration Laboratories. A Data Acquisition Card (DAC) is used to collect the signal as detected by the isotropic e-field probe. The DAC manufacturer calibrates the DAC to NIST standards. A formal validation is executed using all mechanical and electronic components to prove conformity of the measurement platform as a whole.

System Description

The ALSAS-10-U has been designed to measure devices within the compliance environment to meet all recognized standards. The system also conforms to standards, which are currently being developed by the scientific and manufacturing community.

The course scan resolution is defined by the operator and reflects the requirements of the standard to which the device is being tested. Precise measurements are made within the predefined course scan area and the values are logged.

The user predefines the sample rate for which the measurements are made so as to ensure that the full duty-cycle of a pulse modulation device is covered during the sample. The following algorithm is an example of the function used by the system for linearization of the output for the probe.

$$V_i = U_i + U_i^2 \bullet \frac{cf}{dcp_i}$$



The April E-Field probe is evaluated to establish the diode compression point.

A complex algorithm is then used to calculate the values within the measured points down to a resolution of 1mm. The data from this process is then used to provide the co-ordinates from which the cube scan is created for the determination of the 1 g and 10 g averages.

Cube scan averaging consists of a number of complex algorithms, which are used to calculate the one, and ten gram averages. The basis for the cube scan process is centered on the location where the maximum measured SAR value was found. When a secondary peak value is found which is within 60% of the initial peak value, the system will report this back to the operator who can then assess the need for further analysis of both the peak values prior to the one and ten-gram cube scan averaging process. The algorithm consists of 3D cubic Spline, and Lagrange extrapolation to the surface, which form the matrix for calculating the measurement output for the one and ten gram average values. The resolution for the physical scan integral is user defined with a final calculated resolution down to 1mm.

In-depth analysis for the differential of the physical scanning resolution for the cube scan analysis has been carried out, to identify the optimum setting for the probe positioning steps, and this has been determined at 8mm increments on the X, & Y planes. The reduction of the physical step increment increased the time taken for analysis but did not provide a better uncertainty or return on measured values.

The final output from the system provides data for the area scan measurements, physical and splined (1mm resolution) cube scan with physical and calculated values (1mm resolution).


The overall uncertainty for the methodology and algorithms the ALSAS-10-U used during the SAR calculation was evaluated using the data from IEEE 1528 f3 algorithm:

$$f_3(x, y, z) = A \frac{a^2}{\frac{a^2}{4} + x'^2 + y'^2} \left(e^{-\frac{2z}{a}} + \frac{a^2}{2(a + 2z)^2} \right)$$


The probe used during the measurement process has been assessed to provide values for diode compression. These values are calculated during the probe calibration exercise and are used in the mathematical calculations for the assessment of SAR.

E-Field Probe

The E-field probe used by RF Exposure Lab, LLC, has been fully calibrated and assessed for isotropic, and boundary effect. The probe utilizes a triangular sensor arrangement as detailed in the diagram below right.



Δ-BEAM

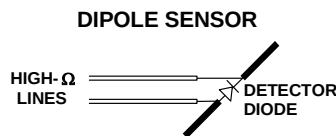

The SAR is assessed with the probe which moves at a default height of 5mm from the center of the diode, which is mounted to the sensor, to the phantom surface (Z height). The diagram above right shows how the center of the sensor is defined with the location of the diode placed at the center of the dipole. The 5mm default in the Z axis is the optimum height for assessing SAR where the boundary effect is at its least, with the probe located closest to the phantom surface (boundary).

The manufacturer specified precision of the robot is ± 0.05 mm and the precision of the APREL bottom detection device is ± 0.1 mm. These precisions are calibrated and tested in the manufacturing process of the bottom detection device. A constant distance is maintained because the surface of the phantom is dynamically detected for each point. The surface detection algorithm corrects the position of the robot so that the probe rests on the surface of the phantom. The probe is then moved to the measurement location 2.44 mm above the phantom surface resulting in the probe center location to be at 4.0 mm above the phantom surface. Therefore, the probe sensor will be at 4.0 mm above the phantom surface ± 0.1 mm for each SAR location for frequencies below 3 GHz. The probe is moved to the measurement location 1.44 mm above the phantom surface resulting in the probe center location to be at 2.0 mm above the phantom surface. Therefore, the probe sensor will be at 2.0 mm above the phantom surface ± 0.1 mm for each SAR location for frequencies above 3 GHz.

The probe boundary effect compensation cannot be disabled in the ALSAS-10U testing system. The probe tip will always be at least half a probe tip diameter from the phantom surface. For frequencies up to 3 GHz, the probe diameter is 5 mm. With the sensor offset set at 1.54 mm (default setting), the sensor to phantom gap will be 4.0 mm which is greater than half the probe tip diameter. For frequencies greater than 3 GHz, the probe diameter is 3 mm. With the sensor offset set at 0.56 mm (default setting), the sensor to phantom gap will be 3.0 mm which is greater than half the probe tip diameter.

The separation of the first 2 measurement points in the zoom scan is specified in the test setup software. For frequencies below 3 GHz, the user must specify a zoom scan resolution of less than 6 mm in the z-axis to have the first two measurements within 1 cm of the surface. The z-axis is set to 4 mm as shown on each of the data sheets in Appendix B. For frequencies above 3 GHz, the user must specify a zoom scan resolution of less than 3 mm in the z-axis to have the first two measurements within 5 mm of the surface. The z-axis is set to 2 mm as shown on each of the data sheets in Appendix B.

The zoom scan volume for devices ≤ 3 GHz with a cube scan of $5 \times 5 \times 8$ yields a volume of $32 \times 32 \times 28$ mm³. For devices > 3 GHz and < 4.5 GHz, the cube scan of $9 \times 9 \times 9$ yields a volume of $32 \times 32 \times 24$ mm³. For devices ≥ 4.5 GHz, the cube scan of $7 \times 7 \times 12$ yields a volume of $24 \times 24 \times 22$ mm³.

3. Robot Specifications

Specifications

Positioner:	ThermoCRS, Robot Model: Robocomm 3
Repeatability:	0.05 mm
No. of axis:	6

Data Acquisition Card (DAC) System

Cell Controller

Processor:	Pentium 4™
Clock Speed:	2.66 GHz
Operating System:	Windows XP Pro™

Data Converter

Features:	Signal Amplifier, End Effector, DAC
Software:	ALSAS 10-U Software

E-Field Probe

Model:	Various See Probe Calibration Sheet
Serial Number:	Various See Probe Calibration Sheet
Construction:	Triangular Core Touch Detection System
Frequency:	10MHz to 6GHz

Phantom

Phantom:	Uniphantom, Right Phantom, Left Phantom
----------	---



4. Probe and Dipole Calibration

See Appendix D and E.

5. Phantom & Simulating Tissue Specifications

SAM Phantom



The Aprel system utilizes three separate phantoms. Each phantom for SAR assessment testing is a low loss dielectric shell, with shape and dimensions derived from the anthropomorphic data of the 90th percentile adult male head dimensions as tabulated by the US Army. The SAM phantom shell is bisected along the mid sagittal plane into right and left halves. The perimeter sidewalls of each phantom half is extended to allow filling with liquid to a depth of 15 cm that is sufficient to minimize reflections from the upper surface [5]. See photos in Appendix C.

Brain & Muscle Simulating Mixture Characterization

The brain and muscle mixtures consist of a glycol based chemical and saline solution. The mixture is calibrated to obtain proper dielectric constant (permittivity) and conductivity of the desired tissue. The head tissue dielectric parameters recommended by the IEEE SCC-34/SC-2 have been incorporated in the following tables. Other head and body tissue parameters that have not been specified in P1528 are derived from the issue dielectric parameters computed from the 4-Cole-Cole equations.

Table 5.1 Typical Composition of Ingredients for Tissue

Ingredients		Simulating Tissue		
		2450 MHz Muscle	5200 MHz Muscle	5800 MHz Muscle
Mixing Percentage				
Water		73.20	58.85	59.00
Sugar		0.00	41.00	40.60
Salt		0.04	0.00	0.00
HEC		0.00	0.10	0.30
Bactericide		0.00	0.05	0.10
DGBE		26.70	0.00	0.00
Dielectric Constant	Target	52.70	48.96	48.25
Conductivity (S/m)	Target	1.95	5.35	5.96

Device Holder



In combination with the SAM phantom, the mounting device enables the rotation of the mounted transmitter in spherical coordinates whereby the rotation point is the ear opening. The devices can easily, accurately, and repeatably be positioned according to the FCC specifications. The device holder can be locked at different phantom locations (left head, right head, and uni-phantom).

6. Definition of Reference Points

Ear Reference Point

Figure 6.2 shows the front, back and side views of the SAM Phantom. The point “M” is the reference point for the center of the mouth, “LE” is the left ear reference point (ERP), and “RE” is the right ERP. The ERPs are 15mm posterior to the entrance to the ear canal (EEC) along the B-M line (Back-Mouth), as shown in Figure 6.1. The plane passing through the two ear canals and M is defined as the Reference Plane. The line N-F (Neck-Front) is perpendicular to the reference plane and passing through the RE (or LE) is called the Reference Pivoting Line (see Figure 6.1). Line B-M is perpendicular to the N-F line. Both N-F and B-M lines are marked on the external phantom shell to facilitate handset positioning [5].

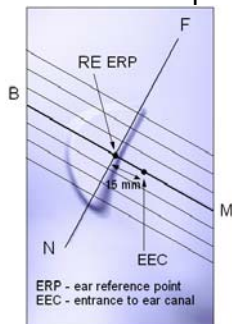


Figure 6.1 Close-up side view of ERP's



Figure 6.2 Front, back and side view of SAM

Device Reference Points

Two imaginary lines on the device need to be established: the vertical centerline and the horizontal line. The test device is placed in a normal operating position with the “test device reference point” located along the “vertical centerline” on the front of the device aligned to the “ear reference point” (See Fig. 6.3). The “test device reference point” is then located at the same level as the center of the ear reference point. The test device is positioned so that the “vertical centerline” is bisecting the front surface of the device at it’s top and bottom edges, positioning the “ear reference point” on the outer surface of both the left and right head phantoms on the ear reference point [5].

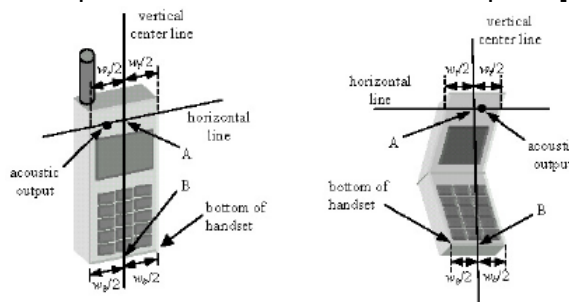


Figure 6.3 Handset Vertical Center & Horizontal Line Reference Points

7. Test Configuration Positions

Positioning for Cheek/Touch [5]

1. Position the device close to the surface of the phantom such that point A is on the (virtual) extension of the line passing through points RE and LE on the phantom (see Figure 7.1), such that the plane defined by the vertical center line and the horizontal line of the device is approximately parallel to the sagittal plane of the phantom.

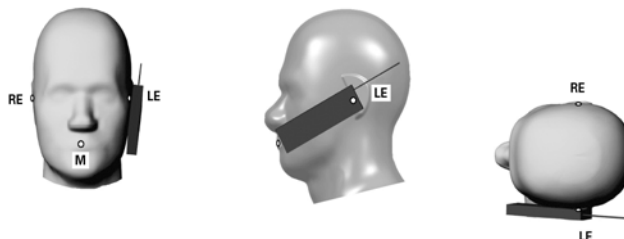


Figure 7.1 Front, Side and Top View of Cheek/Touch Position

2. Translate the device towards the phantom along the line passing through RE and LE until the device touches the ear.
3. While maintaining the device in this plane, rotate it around the LE-RE line until the vertical centerline is in the plane normal to MB-NF including the line MB (called the reference plane).
4. Rotate the device around the vertical centerline until the device (horizontal line) is symmetrical with respect to the line NF.
5. While maintaining the vertical centerline in the reference plane, keeping point A on the line passing through RE and LE and maintaining the device contact with the ear, rotate the device about the line NF until any point on the device is in contact with a phantom point below the ear (cheek). See Figure 7.2.




Figure 7.2 Side view w/ relevant markings

Positioning for Ear / 15° Tilt [5]

With the test device aligned in the Cheek/Touch Position”:

1. While maintaining the orientation of the device, retracted the device parallel to the reference plane far enough to enable a rotation of the device by 15 degrees.
2. Rotate the device around the horizontal line by 15 degrees.
3. While maintaining the orientation of the device, move the device parallel to the reference plane until any part of the device touches the head. (In this position, point A is located on the line RE-LE). The tilted position is obtained when the contact is on the pinna. If the contact is at any location other than the pinna, the angle of the device shall be reduced. The tilted position is obtained when any part of the device is in contact with the ear as well as a second part of the device is in contact with the head (see Figure 7.3).

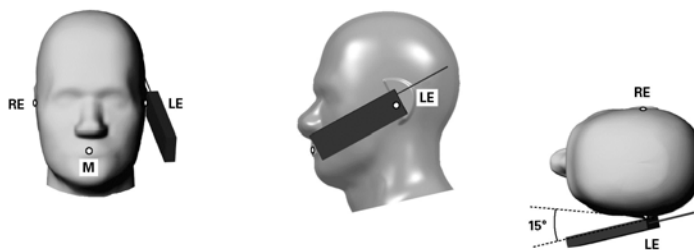


Figure 7.3 Front, Side and Top View of Ear/15° Tilt Position

Body Worn Configurations

Body-worn operating configurations are tested with the accessories attached to the device and positioned against a flat phantom in a normal use configuration. A device with a headset output is tested with a headset connected to the device. Body dielectric parameters are used.

Accessories for Body-worn operation configurations are divided into two categories: those that do not contain metallic components and those that do contain metallic components. When multiple accessories that do not contain metallic components are supplied with the device, the device is tested with only the accessory that dictates the closest spacing to the body. Then, when multiple accessories that contain metallic components are supplied with the device, the device is tested with each accessory that contains a unique metallic component. If multiple accessories share an identical metallic component (i.e. the same metallic belt-clip used with different holsters with no other metallic components) only the accessory that dictates the closest spacing to the body is tested.

Body-worn accessories may not always be supplied or available as options for some devices intended to be authorized for body-worn use. In this case, a test configuration where a separation distance between the back of the device and the flat phantom is used. All test position spacings are documented.

Transmitters that are designed to operate in front of a person's face, as in push-to-talk configurations, are tested for SAR compliance with the front of the device positioned to face the flat phantom. For devices that are carried next to the body such as a shoulder, waist or chest-worn transmitters, SAR compliance is tested with the accessory(ies), including headsets and microphones, attached to the device and positioned against a flat phantom in a normal use configuration.

In all cases SAR measurements are performed to investigate the worst-case positioning. Worst-case positioning is then documented and used to perform Body SAR testing.

In order for users to be aware of the body-worn operating requirements for meeting RF exposure compliance, operating instructions and cautions statements are included in the user's manual.

8. ANSI/IEEE C95.1 – 1999 RF Exposure Limits [2]

Uncontrolled Environment

Uncontrolled Environments are defined as locations where there is the exposure of individuals who have no knowledge or control of their exposure. The general population/uncontrolled exposure limits are applicable to situations in which the general public may be exposed or in which persons who are exposed as a consequence of their employment may not be made fully aware of the potential for exposure or cannot exercise control over their exposure. Members of the general public would come under this category when exposure is not employment-related; for example, in the case of a wireless transmitter that exposes persons in its vicinity.

Controlled Environment

Controlled Environments are defined as locations where there is exposure that may be incurred by persons who are aware of the potential for exposure, (i.e. as a result of employment or occupation). In general, occupational/controlled exposure limits are applicable to situations in which persons are exposed as a consequence of their employment, who have been made fully aware of the potential for exposure and can exercise control over their exposure. This exposure category is also applicable when the exposure is of a transient nature due to incidental passage through a location where the exposure levels may be higher than the general population/uncontrolled limits, but the exposed person is fully aware of the potential for exposure and can exercise control over his or her exposure by leaving the area or by some other appropriate means.

Table 8.1 Human Exposure Limits

	UNCONTROLLED ENVIRONMENT General Population (W/kg) or (mW/g)	CONTROLLED ENVIROMENT Professional Population (W/kg) or (mW/g)
SPATIAL PEAK SAR ¹ Brain	1.60	8.00
SPATIAL AVERAGE SAR ² Whole Body	0.08	0.40
SPATIAL PEAK SAR ³ Hands, Feet, Ankles, Wrists	4.00	20.00

¹ The Spatial Peak value of the SAR averaged over any 1 gram of tissue (defined as a tissue volume in the shape of a cube) and over the appropriate averaging time.

² The Spatial Average value of the SAR averaged over the whole body.

³ The Spatial Peak value of the SAR averaged over any 10 grams of tissue (defined as a tissue volume in the shape of a cube) and over the appropriate averaging time.

9. Measurement Uncertainty

Exposure Assessment Measurement Uncertainty

Source of Uncertainty	Tolerance Value	Probability Distribution	Divisor	c_i^1 (1-g)	c_i^1 (10-g)	Standard Uncertainty (1-g) %	Standard Uncertainty (10-g) %
Measurement System							
Probe Calibration	3.5	normal	1	1	1	3.5	3.5
Axial Isotropy	3.7	rectangular	•3	$(1-cp)^{1/2}$	$(1-cp)^{1/2}$	1.5	1.5
Hemispherical Isotropy	10.9	rectangular	•3	•cp	•cp	4.4	4.4
Boundary Effect	1.0	rectangular	•3	1	1	0.6	0.6
Linearity	4.7	rectangular	•3	1	1	2.7	2.7
Detection Limit	1.0	rectangular	•3	1	1	0.6	0.6
Readout Electronics	1.0	normal	1	1	1	1.0	1.0
Response Time	0.8	rectangular	•3	1	1	0.5	0.5
Integration Time	1.7	rectangular	•3	1	1	1.0	1.0
RF Ambient Condition	3.0	rectangular	•3	1	1	1.7	1.7
Probe Positioner Mech.	0.4	rectangular	•3	1	1	0.2	0.2
Restriction							
Probe Positioning with respect to Phantom Shell	2.9	rectangular	•3	1	1	1.7	1.7
Extrapolation and Integration	3.7	rectangular	•3	1	1	2.1	2.1
Test Sample Positioning	4.0	normal	1	1	1	4.0	4.0
Device Holder Uncertainty	2.0	normal	1	1	1	2.0	2.0
Drift of Output Power	4.2	rectangular	•3	1	1	2.4	2.4
Phantom and Setup							
Phantom Uncertainty(shape & thickness tolerance)	3.4	rectangular	•3	1	1	2.0	2.0
Liquid Conductivity(target)	5.0	rectangular	•3	0.7	0.5	2.0	1.4
Liquid Conductivity(meas.)	0.5	normal	1	0.7	0.5	0.4	0.3
Liquid Permittivity(target)	5.0	rectangular	•3	0.6	0.5	1.7	1.4
Liquid Permittivity(meas.)	1.0	normal	1	0.6	0.5	0.6	0.5
Combined Uncertainty		RSS				9.6	9.4
Combined Uncertainty (coverage factor=2)		Normal (k=2)				19.1	18.8

10. System Validation

Tissue Verification

Table 10.1 Measured Tissue Parameters

		2450 MHz Body		5250 MHz Body		5800 MHz Body	
Date(s)		April 29, 2008		April 30, 2008		May 1, 2008	
Liquid Temperature (°C)	20.0	Target	Measured	Target	Measured	Target	Measured
Dielectric Constant: ϵ		52.59	50.82	49.19	48.83	48.53	49.38
Conductivity: σ		1.92	1.87	5.40	5.31	5.95	5.84

		2450 MHz Body	
Date(s)		Dec. 15, 2008	
Liquid Temperature (°C)	20.0	Target	Measured
Dielectric Constant: ϵ		52.59	54.59
Conductivity: σ		1.92	1.95

See Appendix A for data printout.

Test System Verification

Prior to assessment, the system is verified to the $\pm 10\%$ of the specifications at the test frequency by using the system kit. Power is extrapolated to 1 watt. (Graphic Plots Attached)

Table 10.2 System Dipole Validation Target & Measured

	Test Frequency	Targeted SAR _{1g} (W/kg)	Measure SAR _{1g} (W/kg)	Deviation (%)
28-Apr-2008	2450 MHz	53.55	54.70	+ 2.15
30-Apr-2008	5250 MHz	62.98	64.46	+ 2.35
01-May-2008	5785 MHz	58.92	59.08	+ 0.27
15-Dec-2008	2450 MHz	53.55	53.79	+ 0.45

See Appendix A for data plots.

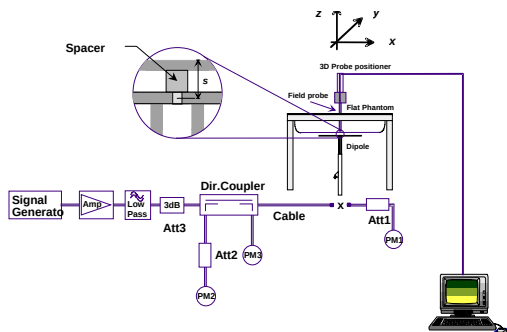


Figure 10.1 Dipole Validation Test Setup

11. SAR Test Data Summary

See Measurement Result Data Pages

See Appendix B for SAR Test Data Plots.
See Appendix C for SAR Test Setup Photos.

Procedures Used To Establish Test Signal

The device was placed into simulated transmit mode using the manufacturer's test codes. Such test signals offer a consistent means for testing SAR and are recommended for evaluating SAR. When test modes are not available or inappropriate for testing a device, the actual transmission is activated through a base station simulator or similar equipment. See data pages for actual procedure used in measurement.

Device Test Condition

The device is battery operated. Each SAR measurement was taken with a fully charged battery. In order to verify that the device was tested at full power, conducted output power measurements were performed before and after each SAR measurement to confirm the output power unless otherwise noted. If a conducted power deviation of more than 5% occurred, the test was repeated.

The testing was conducted on the back of the device due to the normal position of the device. The conducted power was measured before the start of testing. The power was not measured before and after each test due to the necessity of disassembling the device to take the measurement.

802.11b						802.11a 5.8 GHz				
Freq	Channel	Data Rate	Antenna	Power		Freq	Channel	Data Rate	Antenna	Power
2412	1	1	Main	15.46		5.745	149	6	Main	6.49
2437	6	1	Main	15.58		5.765	153	6	Main	6.43
2462	11	1	Main	15.30		5.785	157	6	Main	6.31
2412	1	1	Aux	14.62		5.805	161	6	Main	6.53
2437	6	1	Aux	14.35		5.745	149	6	Aux	7.54
2462	11	1	Aux	14.77		5.765	153	6	Aux	6.39
2437	6	2	Main	15.55		5.785	157	6	Aux	5.64
2437	6	5.5	Main	14.46		5.805	161	6	Aux	6.54
2437	6	11	Main	12.45		5.745	149	9	Main	4.96
						5.745	149	12	Main	5.57
802.11g						5.745	149	18	Main	5.89
Freq	Channel	Data Rate	Antenna	Power		5.745	149	24	Main	6.26
2412	1	6	Main	11.38		5.745	149	36	Main	6.06
2437	6	6	Main	11.22		5.745	149	48	Main	6.11
2462	11	6	Main	11.47		5.745	149	54	Main	6.23
2412	1	6	Aux	11.03						
2437	6	6	Aux	11.25						
2462	11	6	Aux	11.02						
2462	11	9	Main	10.44						
2462	11	12	Main	11.12						
2462	11	18	Main	10.76						
2462	11	24	Main	10.29						
2462	11	36	Main	8.96						
2462	11	48	Main	8.79						
2462	11	54	Main	9.98						
802.11a 5.2 GHz										
Freq	Channel	Data Rate	Antenna	Power						
5.18	36	6	Main	11.26						
5.20	40	6	Main	10.49						
5.22	44	6	Main	10.37						
5.24	48	6	Main	11.24						
5.18	36	6	Aux	11.97						
5.20	40	6	Aux	12.88						
5.22	44	6	Aux	12.79						
5.24	48	6	Aux	12.93						
5.24	48	9	Aux	11.68						
5.24	48	12	Aux	12.70						
5.24	48	18	Aux	12.61						
5.24	48	24	Aux	12.37						
5.24	48	36	Aux	7.57						
5.24	48	48	Aux	6.48						
5.24	48	54	Aux	5.99						

Conduct Power Measurements

SAR Data Summary – 2450 MHz Body

MEASUREMENT RESULTS								
Position	Band	Antenna	Frequency		Modulation	End Power	Battery	SAR (W/kg)
			MHz	Ch.		(dBm)		
Touch	b	Main	2412	1	DSSS	15.46	Standard	0.124
			2437	6	DSSS	15.58	Standard	0.117
			2462	11	DSSS	15.30	Standard	0.128
		Aux	2412	1	DSSS	14.62	Standard	0.234
			2437	6	DSSS	14.35	Standard	0.232
			2462	11	DSSS	14.77	Standard	0.276
	g	Main	2412	1	OFDM	11.38	Standard	0.096
			2437	6	OFDM	11.22	Standard	0.126
			2462	11	OFDM	11.47	Standard	0.148
		Aux	2412	1	OFDM	11.03	Standard	0.267
			2437	6	OFDM	11.25	Standard	0.117
			2462	11	OFDM	11.02	Standard	0.124

Muscle

1.6 W/kg (mW/g)

averaged over 1 gram

1. Battery is fully charged for all tests.

Power Measured

☒ Conducted

☐ ERP

☐ EIRP

2. SAR Measurement

Phantom Configuration

☐ Left Head

☒ Uniphantom

☐ Right Head

SAR Configuration

☐ Head

☒ Body

3. Test Signal Call Mode

☒ Test Code

☐ Base Station Simulator

4. Test Configuration

☐ With Belt Clip

☐ Without Belt Clip ☒ N/A



Jay M. Moulton
Vice President

SAR Data Summary – 5200 MHz Body

MEASUREMENT RESULTS								
Position	Band	Antenna	Frequency		Modulation	End Power	Battery	SAR (W/kg)
			MHz	Ch.		(dBm)		
Touch	A1	Main	5180	36	OFDM	11.26	Standard	0.138
			5240	48	OFDM	11.24	Standard	0.244
		Aux	5200	40	OFDM	12.88	Standard	0.221
			5240	48	OFDM	12.93	Standard	0.239
						Muscle 1.6 W/kg (mW/g) averaged over 1 gram		

- Battery is fully charged for all tests.
Power Measured ☒ Conducted ☐ ERP ☐ EIRP
- SAR Measurement
Phantom Configuration ☐ Left Head ☒ Uniphantom ☐ Right Head
SAR Configuration ☐ Head ☒ Body
- Test Signal Call Mode ☒ Test Code ☐ Base Station Simulator
- Test Configuration ☐ With Belt Clip ☐ Without Belt Clip ☒ N/A



Jay M. Moulton
Vice President

SAR Data Summary – 5800 MHz Body

MEASUREMENT RESULTS								
Position	Band	Antenna	Frequency		Modulation	End Power	Battery	SAR (W/kg)
			MHz	Ch.		(dBm)		
Touch	A3	Main	5745	149	OFDM	6.49	Standard	0.152
			5808	161	OFDM	6.53	Standard	0.119
		Aux	5745	149	OFDM	7.54	Standard	0.113
			5805	161	OFDM	6.54	Standard	0.149
						Muscle 1.6 W/kg (mW/g) averaged over 1 gram		

1. Battery is fully charged for all tests.

Power Measured

☒ Conducted

☐ ERP

☐ EIRP

2. SAR Measurement

Phantom Configuration

☐ Left Head

☒ Uniphantom

☐ Right Head

SAR Configuration

☐ Head

☒ Body

3. Test Signal Call Mode

☒ Test Code

☐ Base Station Simulator

4. Test Configuration

☐ With Belt Clip

☐ Without Belt Clip ☒ N/A



Jay M. Moulton
Vice President

SAR Data Summary – 2450 MHz Bluetooth Body

MEASUREMENT RESULTS

Position	Band	Simultaneous TX	Frequency		Modulation	End Power	Battery	Stand Alone SAR (W/kg)	Sum SAR (W/kg)
			MHz	Ch.		(dBm)			
Touch	BT	N.A.	-	-	OFDM	1.32	Standard	0.082	N.A.
	b	BT	2462	11	DSSS	14.77	Standard	0.276	0.358
	a1	BT	5240	48	OFDM	11.24	Standard	0.244	0.326
	a3	BT	5745	149	OFDM	6.49	Standard	0.152	0.234
Muscle 1.6 W/kg (mW/g) averaged over 1 gram									

1. Battery is fully charged for all tests.

Power Measured

☒ Conducted

☐ ERP

☐ EIRP

2. SAR Measurement

Phantom Configuration

☐ Left Head

☒ Uniphantom

☐ Right Head

SAR Configuration

☐ Head

☒ Body

3. Test Signal Call Mode

☒ Test Code

☐ Base Station Simulator

4. Test Configuration

☐ With Belt Clip

☐ Without Belt Clip ☒ N/A



Jay M. Moulton
Vice President

12.1 Test Equipment List

Table 12.1 Equipment Specifications

Type	Calibration Due Date	Serial Number
ThermoCRS Robot	N/A	RAF0338198
ThermoCRS Controller	N/A	RCF0338224
ThermoCRS Teach Pendant (Joystick)	N/A	STP0334405
IBM Computer, 2.66 MHz P4	N/A	8189D8U KCPR08N
Apriel E-Field Probe ALS-E020	12/03/2008	RFE-217
Apriel E-Field Probe ALS-E030	04/30/2008	AL-E3P1
Apriel Dummy Probe	N/A	023
Apriel Left Phantom	N/A	RFE-267
Apriel Right Phantom	N/A	RFE-268
Apriel UniPhantom	N/A	RFE-273
Apriel Validation Dipole ALS-D-450-S-2	04/30/2009	RFE-362
Apriel Validation Dipole ALS-D-835-S-2	02/22/2010	RFE-274
Apriel Validation Dipole ALS-D-1900-S-2	02/21/2010	RFE-277
Apriel Validation Dipole ALS-D-2450-S-2	02/20/2010	RFE-278
Apriel Validation Dipole ALS-D-BB-S-2	05/23/2009	5258-235-00801
Agilent (HP) 437B Power Meter	12/03/2008	3125U08837
Agilent (HP) 8481B Power Sensor	12/03/2008	3318A05384
Advantest R3261A Spectrum Analyzer	12/03/2008	31720068
Agilent (HP) 8350B Signal Generator	01/28/2009	2749A10226
Agilent (HP) 83525A RF Plug-In	01/28/2009	2647A01172
Agilent (HP) 8753C Vector Network Analyzer	01/28/2009	3135A01724
Agilent (HP) 85047A S-Parameter Test Set	01/28/2009	2904A00595
Apriel Dielectric Probe Assembly	N/A	0011
Brain Equivalent Matter (450 MHz)	N/A	N/A
Brain Equivalent Matter (835 MHz)	N/A	N/A
Brain Equivalent Matter (1900 MHz)	N/A	N/A
Brain Equivalent Matter (2450 MHz)	N/A	N/A
Muscle Equivalent Matter (450 MHz)	N/A	N/A
Muscle Equivalent Matter (835 MHz)	N/A	N/A
Muscle Equivalent Matter (1900 MHz)	N/A	N/A
Muscle Equivalent Matter (2450 MHz)	N/A	N/A
Muscle Equivalent Matter (5200 MHz)	N/A	N/A
Muscle Equivalent Matter (5800 MHz)	N/A	N/A

13.1 Conclusion

The SAR measurement indicates that the EUT complies with the RF radiation exposure limits of the FCC. These measurements are taken to simulate the RF effects exposure under worst-case conditions. Precise laboratory measures were taken to assure repeatability of the tests. The tested device complies with the requirements in respect to all parameters subject to the test. The test results and statements relate only to the item(s) tested.

Please note that the absorption and distribution of electromagnetic energy in the body is a very complex phenomena that depends on the mass, shape, and size of the body; the orientation of the body with respect to the field vectors; and, the electrical properties of both the body and the environment. Other variables that may play a substantial role in possible biological effects are those that characterize the environment (e.g. ambient temperature, air velocity, relative humidity, and body insulation) and those that characterize the individual (e.g. age, gender, activity level, debilitation, or disease). Because innumerable factors may interact to determine the specific biological outcome of an exposure to electromagnetic fields, any protection guide shall consider maximal amplification of biological effects as a result of field-body interactions, environmental conditions, and physiological variables. [3]

14.1 References

- [1] Federal Communications Commission, ET Docket 93-62, Guidelines for Evaluating the Environmental Effects of Radio Frequency Radiation, August 1996
- [2] ANSI/IEEE C95.1 – 1999, American National Standard Safety Levels with respect to Human Exposure to Radio Frequency Electromagnetic Fields, 300kHz to 100GHz, New York: IEEE, 1992.
- [3] ANSI/IEEE C95.3 – 2002, IEEE Recommended Practice for the Measurement of Potentially Hazardous Electromagnetic Fields – RF and Microwave, New York: IEEE, 1992.
- [4] Federal Communications Commission, OET Bulletin 65 (Edition 97-01), Supplement C (Edition 01-01), Evaluating Compliance with FCC Guidelines for Human Exposure to Radio Frequency Electromagnetic Fields, July 2001.
- [5] IEEE Standard 1528 – 2003, IEEE Recommended Practice for Determining the Peak-Spatial Average Specific Absorption Rate (SAR) in the Human Head from Wireless Communication Devices: Measurement Techniques, October 2003.
- [6] Industry Canada, RSS – 102e, Radio Frequency Exposure Compliance of Radiocommunication Apparatus (All Frequency Bands), November 2005.
- [7] Industry Canada, Safety Code 6, Limits of Human Exposure to Radiofrequency Electromagnetic Fields in the Frequency Range from 3kHz to 300 GHz, 1999.

Appendix A – System Validation Plots and Data

```
*****
Test Result for UIM Dielectric Parameter
Tue 29/Apr/2008 07:12:26
Freq Frequency(GHz)
FCC_eH      FCC Bulletin 65 Supplement C ( June 2001) Limits for Head Epsilon
FCC_sH      FCC Bulletin 65 Supplement C (June 2001) Limits for Head Sigma
FCC_eB      FCC Limits for Body Epsilon
FCC_sB      FCC Limits for Body Sigma
Test_e      Epsilon of UIM
Test_s      Sigma of UIM
*****
```

Freq	FCC_eB	FCC_sB	Test_e	Test_s
2.4200	52.74	1.92	50.99	1.85
2.4300	52.73	1.93	50.91	1.85
2.4400	52.71	1.94	50.87	1.86
2.4500	52.70	1.95	50.82	1.87
2.4600	52.69	1.96	50.80	1.89
2.4700	52.67	1.98	50.78	1.90
2.4800	52.66	1.99	50.76	1.91

```
*****
Test Result for UIM Dielectric Parameter
Wed 30/Apr/2007 07:08:34
Freq Frequency(GHz)
FCC_eH      FCC Bulletin 65 Supplement C ( June 2001) Limits for Head Epsilon
FCC_sH      FCC Bulletin 65 Supplement C (June 2001) Limits for Head Sigma
FCC_eB      FCC Limits for Body Epsilon
FCC_sB      FCC Limits for Body Sigma
Test_e      Epsilon of UIM
Test_s      Sigma of UIM
*****
```

Freq	FCC_eB	FCC_sB	Test_e	Test_s
5.2200	48.99	5.32	48.94	5.26
5.2300	48.97	5.33	48.88	5.28
5.2400	48.96	5.35	48.87	5.30
5.2500	48.95	5.36	48.83	5.31
5.2600	48.93	5.37	48.81	5.31
5.2700	48.92	5.38	48.79	5.33
5.2800	48.91	5.39	48.77	5.35

Test Result for UIM Dielectric Parameter

Thu 01/May/2008 07:07:46

Freq Frequency(GHz)

FCC_eH FCC Bulletin 65 Supplement C (June 2001) Limits for Head Epsilon

FCC_sH FCC Bulletin 65 Supplement C (June 2001) Limits for Head Sigma

FCC_eB FCC Limits for Body Epsilon

FCC_sB FCC Limits for Body Sigma

Test_e Epsilon of UIM

Test_s Sigma of UIM

Freq	FCC_eB	FCC_sB	Test_e	Test_s
5.7550	48.26	5.95	49.47	5.77
5.7650	48.25	5.96	49.45	5.80
5.7750	48.23	5.97	49.40	5.81
5.7850	48.22	5.98	49.38	5.84
5.7950	48.21	5.99	49.34	5.86
5.8050	48.19	6.01	49.31	5.87
5.8150	48.18	6.02	49.25	5.89

Test Result for UIM Dielectric Parameter

Mon 15/Dec/2008 10:18:42

Freq Frequency(GHz)

FCC_eH FCC Bulletin 65 Supplement C (June 2001) Limits for Head Epsilon

FCC_sH FCC Bulletin 65 Supplement C (June 2001) Limits for Head Sigma

FCC_eB FCC Limits for Body Epsilon

FCC_sB FCC Limits for Body Sigma

Test_e Epsilon of UIM

Test_s Sigma of UIM

Freq	FCC_eB	FCC_sB	Test_e	Test_s
2.4200	52.74	1.92	54.79	1.93
2.4300	52.73	1.93	54.76	1.94
2.4400	52.71	1.94	54.68	1.94
2.4500	52.70	1.95	54.59	1.95
2.4600	52.69	1.96	54.52	1.97
2.4700	52.67	1.98	54.44	1.98
2.4800	52.66	1.99	54.35	1.99

SAR Test Report

By Operator : Jay
Measurement Date : 29-Apr-2008
Starting Time : 29-Apr-2008 07:57:10 AM
End Time : 29-Apr-2008 08:09:53 AM
Scanning Time : 763 secs

Product Data

Device Name : Validation
Serial No. : 2450
Type : Dipole
Model : ALS-D-2450-S-2
Frequency : 2450.00 MHz
Max. Transmit Pwr : 0.1 W
Drift Time : 0 min(s)
Length : 51.5 mm
Width : 3.6 mm
Depth : 30.4 mm
Antenna Type : Internal
Orientation : Touch
Power Drift-Start : 6.131 W/kg
Power Drift-Finish: 6.206 W/kg
Power Drift (%) : 1.220

Phantom Data

Name : APREL-Uni
Type : Uni-Phantom
Size (mm) : 280 x 280 x 200
Serial No. : System Default
Location : Center
Description : Uni-Phantom

Tissue Data

Type : BODY
Serial No. : 2450
Frequency : 2450.00 MHz
Last Calib. Date : 29-Apr-2008
Temperature : 20.00 °C
Ambient Temp. : 24.00 °C
Humidity : 41.00 RH%
Epsilon : 50.82 F/m
Sigma : 1.87 S/m
Density : 1000.00 kg/cu. m

Probe Data


Name : RFEL 217
Model : E020
Type : E-Field Triangle
Serial No. : 217
Last Calib. Date : 03-Dec-2007
Frequency : 2450.00 MHz
Duty Cycle Factor: 1
Conversion Factor: 3.61
Probe Sensitivity: 1.20 1.20 1.20 $\mu\text{V}/(\text{V/m})^2$
Compression Point: 95.00 mV
Offset : 1.56 mm

Measurement Data

Crest Factor : 1
 Scan Type : Complete
 Tissue Temp. : 20.00 °C
 Ambient Temp. : 23.00 °C
 Set-up Date : 29-Apr-2008
 Set-up Time : 7:57:03 AM
 Area Scan : 5x5x1 : Measurement x=10mm, y=10mm, z=4mm
 Zoom Scan : 5x5x8 : Measurement x=8mm, y=8mm, z=4mm


Other Data

DUT Position : Touch
 Separation : 0
 Channel : Mid

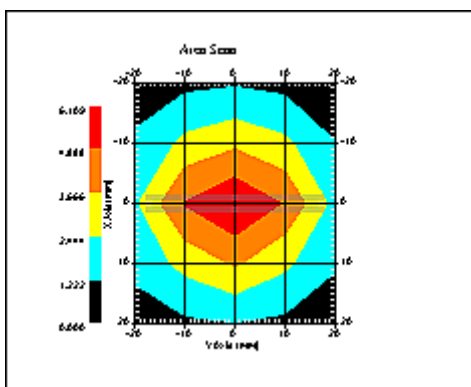

1 gram SAR value : 5.470 W/kg
 10 gram SAR value : 2.605 W/kg
 Area Scan Peak SAR : 6.109 W/kg
 Zoom Scan Peak SAR : 11.090 W/kg

SAR-Z Axis
at Hotspot x:0.28 y:-0.16

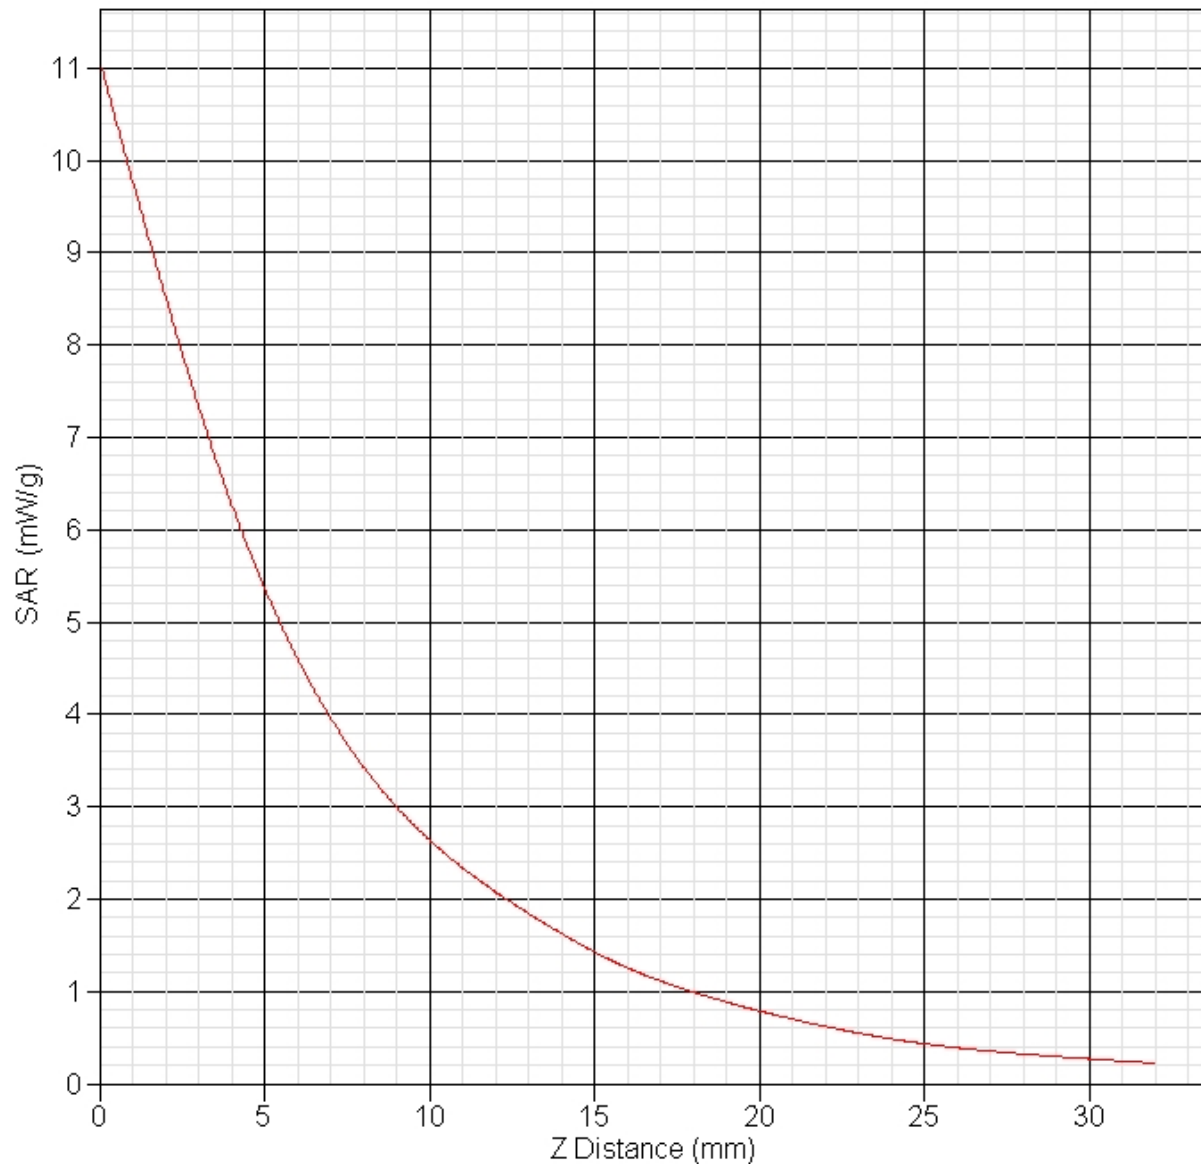

SAR Test Report

By Operator : Jay
Measurement Date : 30-Apr-2008
Starting Time : 30-Apr-2008 07:12:52 AM
End Time : 30-Apr-2008 07:35:57 AM
Scanning Time : 1385 secs

Product Data

Device Name : Validation
Serial No. : 5200
Type : Dipole
Model : ALS-D-BB-S-2
Frequency : 5200.00 MHz
Max. Transmit Pwr : 0.1 W
Drift Time : 0 min(s)
Length : 23.1 mm
Width : 3.6 mm
Depth : 20.7 mm
Antenna Type : Internal
Orientation : Touch
Power Drift-Start : 8.835 W/kg
Power Drift-Finish: 8.723 W/kg
Power Drift (%) : -1.265

Phantom Data

Name : APREL-Uni
Type : Uni-Phantom
Size (mm) : 280 x 280 x 200
Serial No. : System Default
Location : Center
Description : Uni-Phantom

Tissue Data

Type : BODY
Serial No. : 5200
Frequency : 5200.00 MHz
Last Calib. Date : 30-Apr-2008
Temperature : 20.00 °C
Ambient Temp. : 23.00 °C
Humidity : 50.00 RH%
Epsilon : 48.83 F/m
Sigma : 5.31 S/m
Density : 1000.00 kg/cu. m

Probe Data


Name : Probe AL-E3P1 - AL
Model : E-030
Type : E-Field Triangle
Serial No. : AL-E3P1
Last Calib. Date : 30-Apr-2007
Frequency : 5200.00 MHz
Duty Cycle Factor: 1
Conversion Factor: 13
Probe Sensitivity: 1.20 1.20 1.20 $\mu\text{V}/(\text{V/m})^2$
Compression Point: 95.00 mV
Offset : 0.56 mm

Measurement Data

Crest Factor : 1
 Scan Type : Complete
 Tissue Temp. : 20.00 °C
 Ambient Temp. : 23.00 °C
 Set-up Date : 30-Apr-2008
 Set-up Time : 9:00:47 AM
 Area Scan : 5x5x1 : Measurement x=10mm, y=10mm, z=2mm
 Zoom Scan : 7x7x10 : Measurement x=4mm, y=4mm, z=2.5mm


Other Data

DUT Position : Touch
 Separation : 10
 Channel : Mid

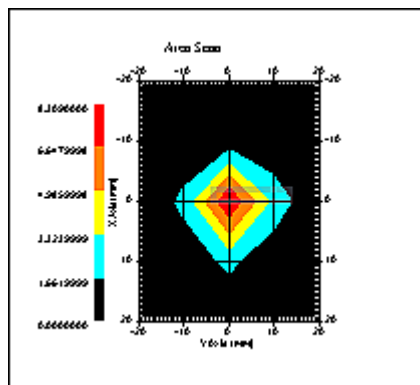

1 gram SAR value : 6.446 W/kg
 10 gram SAR value : 1.635 W/kg
 Area Scan Peak SAR : 8.309 W/kg
 Zoom Scan Peak SAR : 24.319 W/kg

SAR-Z Axis
at Hotspot x:0.29 y:-0.13

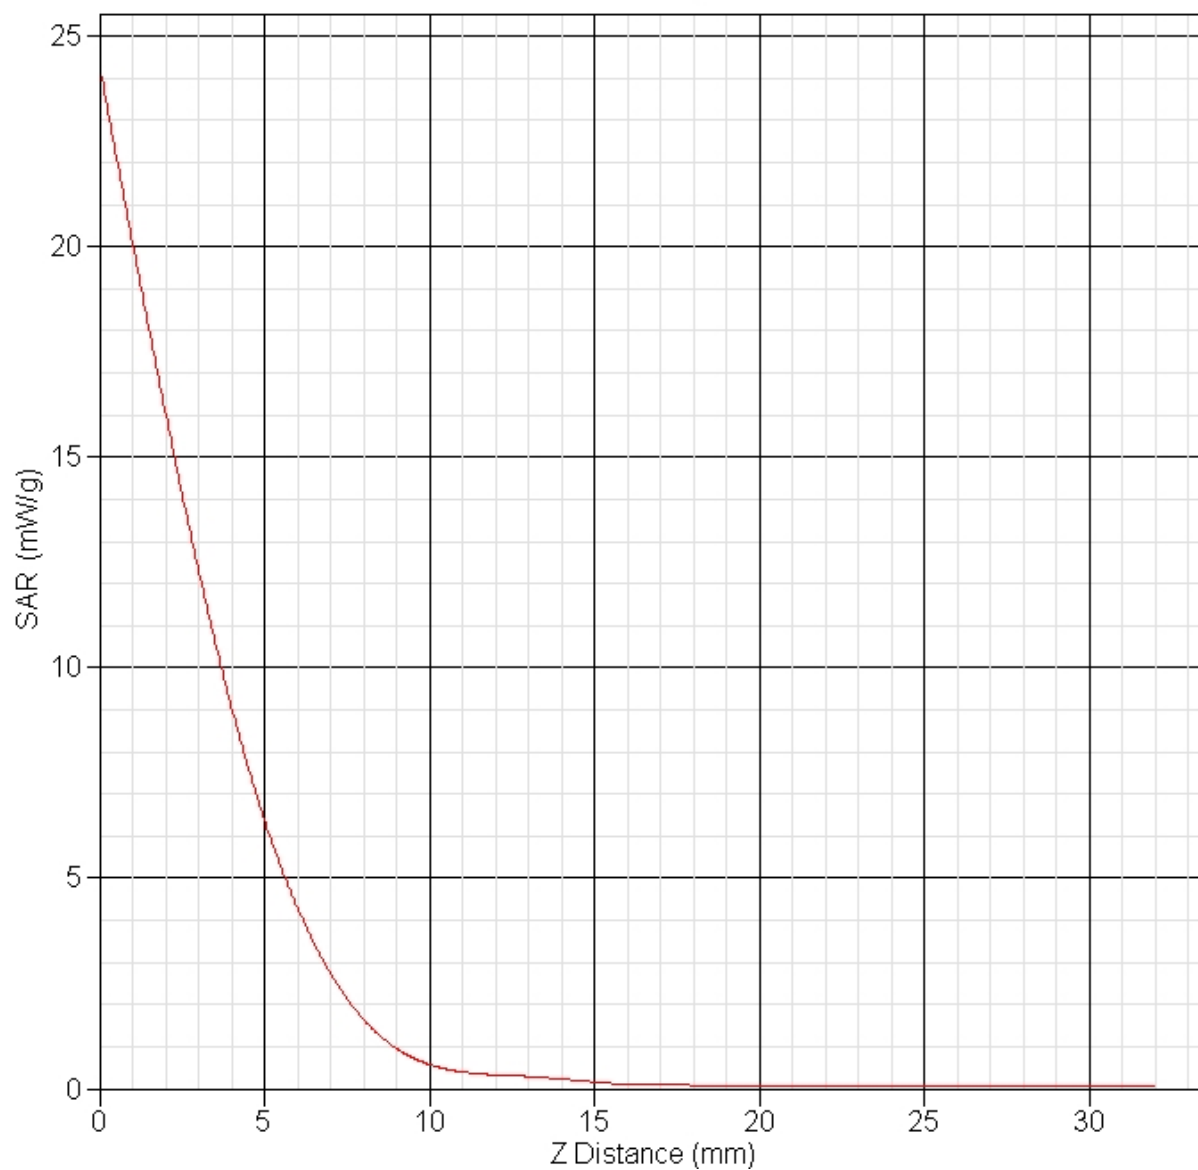

SAR Test Report

By Operator : Jay
Measurement Date : 01-May-2008
Starting Time : 01-May-2008 07:13:39 AM
End Time : 01-May-2008 07:36:30 AM
Scanning Time : 1371 secs

Product Data

Device Name : Validation
Serial No. : 5800
Type : Dipole
Model : ALS-D-BB-S-2
Frequency : 5800.00 MHz
Max. Transmit Pwr : 0.1 W
Drift Time : 0 min(s)
Length : 23.1 mm
Width : 3.6 mm
Depth : 20.7 mm
Antenna Type : Internal
Orientation : Touch
Power Drift-Start : 7.479 W/kg
Power Drift-Finish: 7.493 W/kg
Power Drift (%) : 0.189

Phantom Data

Name : APREL-Uni
Type : Uni-Phantom
Size (mm) : 280 x 280 x 200
Serial No. : System Default
Location : Center
Description : Uni-Phantom

Tissue Data

Type : BODY
Serial No. : 5800
Frequency : 5800.00 MHz
Last Calib. Date : 01-May-2008
Temperature : 20.00 °C
Ambient Temp. : 23.00 °C
Humidity : 50.00 RH%
Epsilon : 49.38 F/m
Sigma : 5.84 S/m
Density : 1000.00 kg/cu. m

Probe Data


Name : Probe AL-E3P1 - AL
Model : E-030
Type : E-Field Triangle
Serial No. : AL-E3P1
Last Calib. Date : 30-Apr-2007
Frequency : 5800.00 MHz
Duty Cycle Factor: 1
Conversion Factor: 14
Probe Sensitivity: 1.20 1.20 1.20 $\mu\text{V}/(\text{V/m})^2$
Compression Point: 95.00 mV
Offset : 0.56 mm

Measurement Data

Crest Factor : 1
 Scan Type : Complete
 Tissue Temp. : 20.00 °C
 Ambient Temp. : 23.00 °C
 Set-up Date : 01-May-2008
 Set-up Time : 4:10:18 PM
 Area Scan : 5x5x1 : Measurement x=10mm, y=10mm, z=2mm
 Zoom Scan : 7x7x10 : Measurement x=4mm, y=4mm, z=2.5mm


Other Data

DUT Position : Touch
 Separation : 10
 Channel : Mid

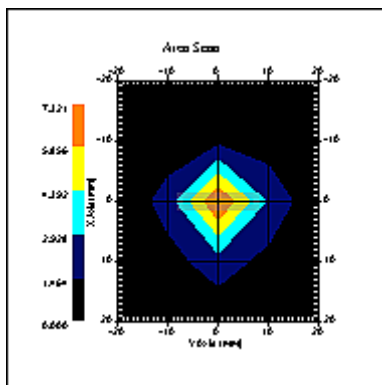

1 gram SAR value : 5.908 W/kg
 10 gram SAR value : 1.597 W/kg
 Area Scan Peak SAR : 7.321 W/kg
 Zoom Scan Peak SAR : 21.617 W/kg

SAR-Z Axis
at Hotspot x:0.32 y:-0.18

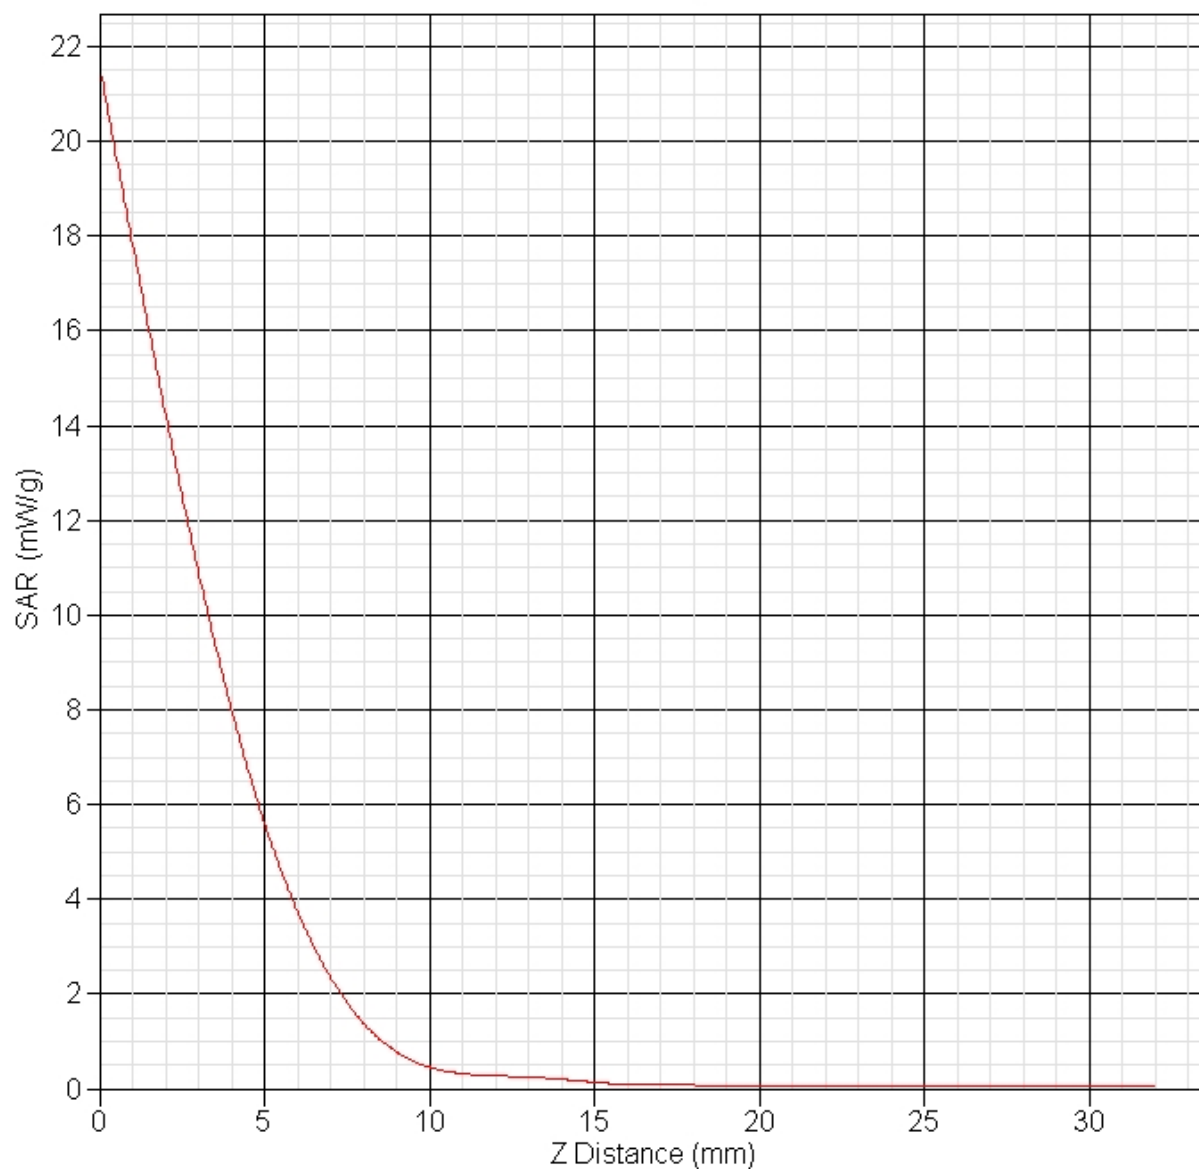

SAR Test Report

By Operator : Jay
Measurement Date : 15-Dec-2008
Starting Time : 15-Dec-2008 11:39:13 AM
End Time : 15-Dec-2008 11:52:07 AM
Scanning Time : 774 secs

Product Data

Device Name : Validation
Serial No. : 2450
Type : Dipole
Model : ALS-D-2450-S-2
Frequency : 2450.00 MHz
Max. Transmit Pwr : 0.1 W
Drift Time : 0 min(s)
Length : 51.5 mm
Width : 3.6 mm
Depth : 30.4 mm
Antenna Type : Internal
Orientation : Touch
Power Drift-Start : 6.215 W/kg
Power Drift-Finish: 6.280 W/kg
Power Drift (%) : 1.050

Phantom Data

Name : APREL-Uni
Type : Uni-Phantom
Size (mm) : 280 x 280 x 200
Serial No. : System Default
Location : Center
Description : Uni-Phantom

Tissue Data

Type : BODY
Serial No. : 2450
Frequency : 2450.00 MHz
Last Calib. Date : 15-Dec-2008
Temperature : 20.00 °C
Ambient Temp. : 23.00 °C
Humidity : 45.00 RH%
Epsilon : 54.59 F/m
Sigma : 1.95 S/m
Density : 1000.00 kg/cu. m

Probe Data


Name : Probe 215 - RFEL
Model : E020
Type : E-Field Triangle
Serial No. : 215
Last Calib. Date : 03-Nov-2008
Frequency : 2450.00 MHz
Duty Cycle Factor: 1
Conversion Factor: 4.5
Probe Sensitivity: 1.20 1.20 1.20 $\mu\text{V}/(\text{V/m})^2$
Compression Point: 95.00 mV
Offset : 1.56 mm

Measurement Data

Crest Factor : 1
 Scan Type : Complete
 Tissue Temp. : 20.00 °C
 Ambient Temp. : 23.00 °C
 Set-up Date : 15-Dec-2008
 Set-up Time : 7:40:13 AM
 Area Scan : 5x5x1 : Measurement x=10mm, y=10mm, z=4mm
 Zoom Scan : 5x5x8 : Measurement x=8mm, y=8mm, z=4mm


Other Data

DUT Position : Touch
 Separation : 10
 Channel : Mid

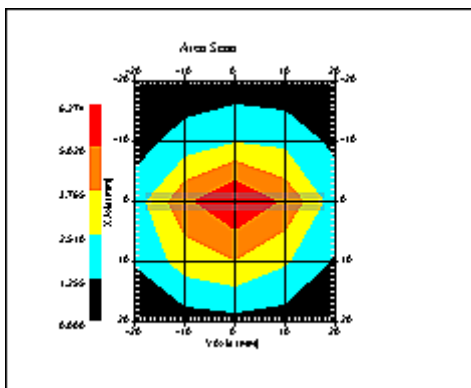

1 gram SAR value : 5.379 W/kg
 10 gram SAR value : 2.452 W/kg
 Area Scan Peak SAR : 6.274 W/kg
 Zoom Scan Peak SAR : 11.190 W/kg

SAR-Z Axis
at Hotspot x:0.24 y:-0.13

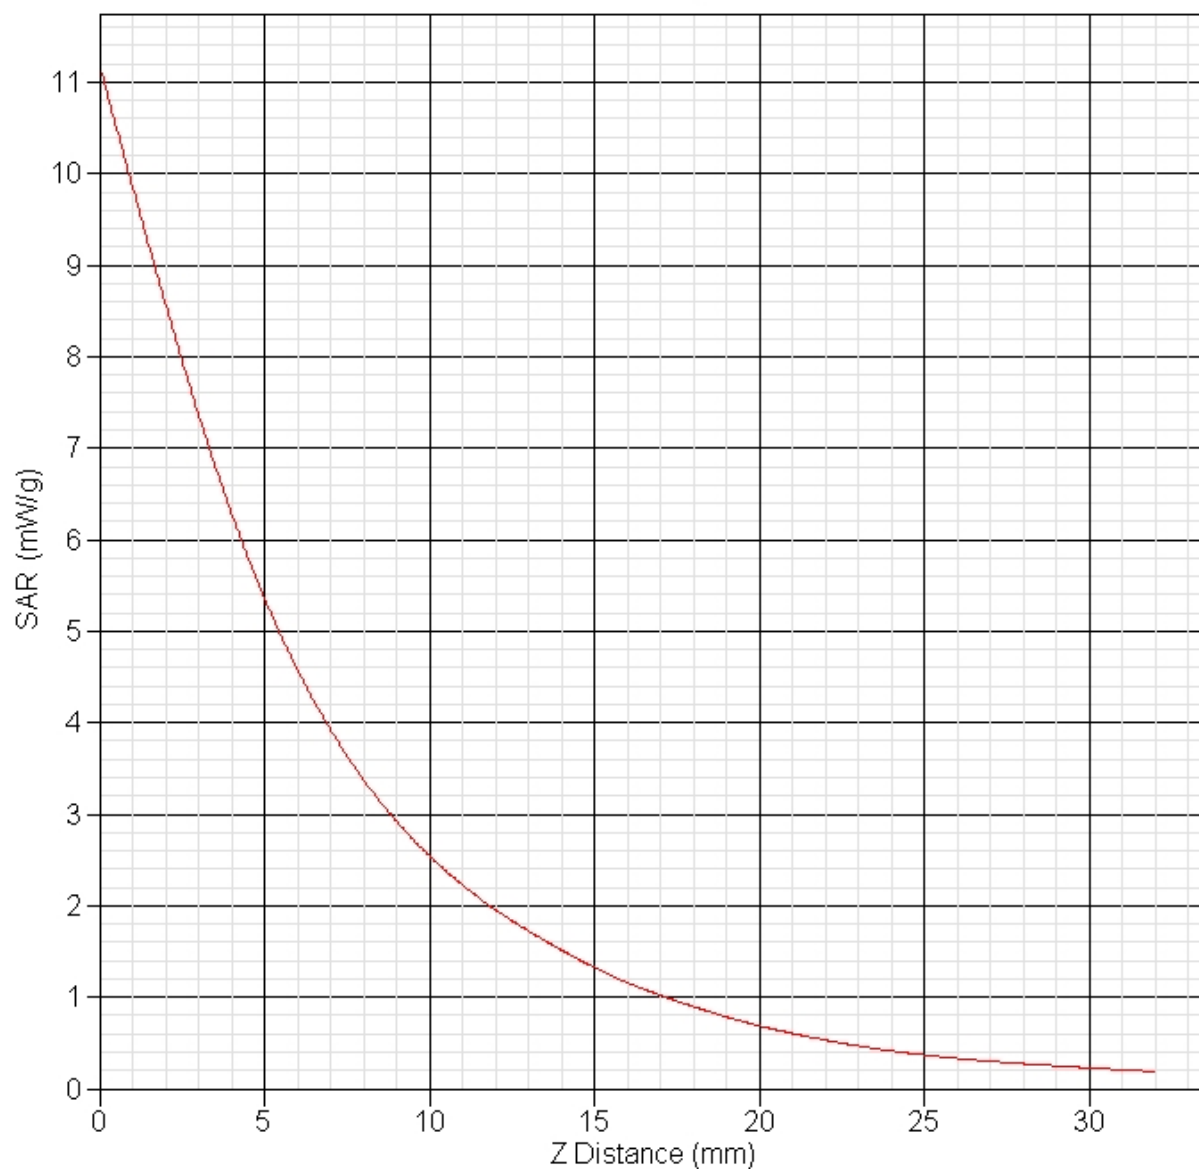

Appendix B – SAR Test Data Plots

SAR Test Report

By Operator : Jay
Measurement Date : 29-Apr-2008
Starting Time : 29-Apr-2008 11:18:02 AM
End Time : 29-Apr-2008 11:32:00 AM
Scanning Time : 838 secs

Product Data

Device Name : LXE
Serial No. : MX8 Eng 1
Type : Other
Model : MX8
Frequency : 2450.00 MHz
Max. Transmit Pwr : 0.03 W
Drift Time : 0 min(s)
Length : 188 mm
Width : 70 mm
Depth : 40 mm
Antenna Type : Internal
Orientation : Touch
Power Drift-Start : 0.116 W/kg
Power Drift-Finish: 0.120 W/kg
Power Drift (%) : 3.434

Phantom Data

Name : APREL-Uni
Type : Uni-Phantom
Size (mm) : 280 x 280 x 200
Serial No. : System Default
Location : Center
Description : Uni-Phantom

Tissue Data

Type : BODY
Serial No. : 2450
Frequency : 2450.00 MHz
Last Calib. Date : 29-Apr-2008
Temperature : 20.00 °C
Ambient Temp. : 24.00 °C
Humidity : 41.00 RH%
Epsilon : 50.82 F/m
Sigma : 1.87 S/m
Density : 1000.00 kg/cu. m

Probe Data


Name : RFEL 217
Model : E020
Type : E-Field Triangle
Serial No. : 217
Last Calib. Date : 03-Dec-2007
Frequency : 2450.00 MHz
Duty Cycle Factor: 1
Conversion Factor: 3.61
Probe Sensitivity: 1.20 1.20 1.20 $\mu\text{V}/(\text{V/m})^2$
Compression Point: 95.00 mV
Offset : 1.56 mm

Measurement Data

Crest Factor : 1
 Scan Type : Complete
 Tissue Temp. : 20.00 °C
 Ambient Temp. : 23.00 °C
 Set-up Date : 29-Apr-2008
 Set-up Time : 8:26:24 AM
 Area Scan : 7x5x1 : Measurement x=10mm, y=10mm, z=4mm
 Zoom Scan : 5x5x8 : Measurement x=8mm, y=8mm, z=4mm

Other Data

DUT Position : Touch
 Separation : 0
 Channel : Low

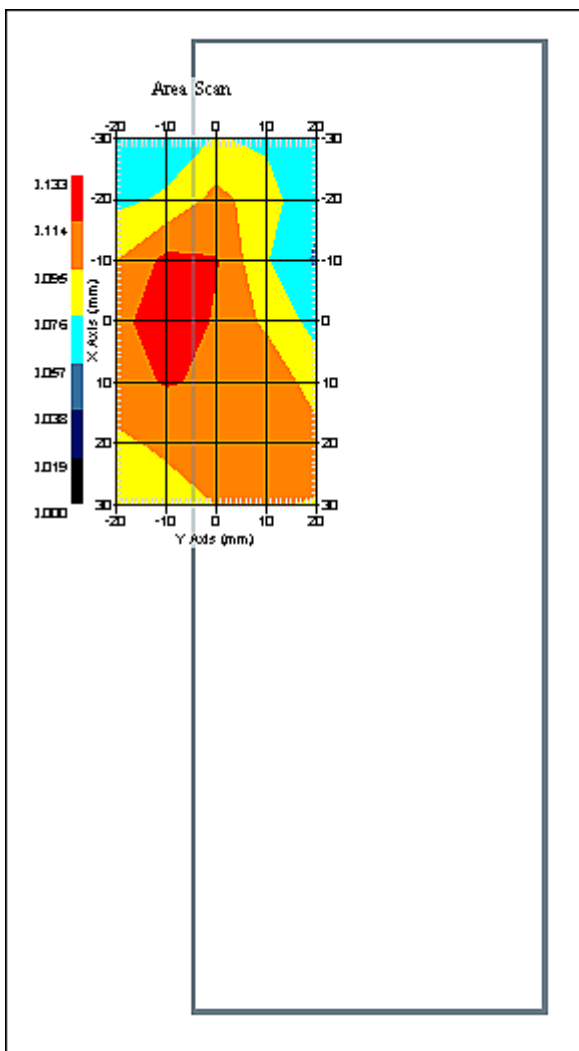

1 gram SAR value : 0.124 W/kg
 10 gram SAR value : 0.089 W/kg
 Area Scan Peak SAR : 0.132 W/kg
 Zoom Scan Peak SAR : 0.190 W/kg

SAR Test Report

By Operator : Jay
Measurement Date : 29-Apr-2008
Starting Time : 29-Apr-2008 11:34:14 AM
End Time : 29-Apr-2008 11:48:13 AM
Scanning Time : 839 secs

Product Data

Device Name : LXE
Serial No. : MX8 Eng 1
Type : Other
Model : MX8
Frequency : 2450.00 MHz
Max. Transmit Pwr : 0.03 W
Drift Time : 0 min(s)
Length : 188 mm
Width : 70 mm
Depth : 40 mm
Antenna Type : Internal
Orientation : Touch
Power Drift-Start : 0.120 W/kg
Power Drift-Finish: 0.115 W/kg
Power Drift (%) : -4.149

Phantom Data

Name : APREL-Uni
Type : Uni-Phantom
Size (mm) : 280 x 280 x 200
Serial No. : System Default
Location : Center
Description : Uni-Phantom

Tissue Data

Type : BODY
Serial No. : 2450
Frequency : 2450.00 MHz
Last Calib. Date : 29-Apr-2008
Temperature : 20.00 °C
Ambient Temp. : 24.00 °C
Humidity : 41.00 RH%
Epsilon : 50.82 F/m
Sigma : 1.87 S/m
Density : 1000.00 kg/cu. m

Probe Data


Name : RFEL 217
Model : E020
Type : E-Field Triangle
Serial No. : 217
Last Calib. Date : 03-Dec-2007
Frequency : 2450.00 MHz
Duty Cycle Factor: 1
Conversion Factor: 3.61
Probe Sensitivity: 1.20 1.20 1.20 $\mu\text{V}/(\text{V/m})^2$
Compression Point: 95.00 mV
Offset : 1.56 mm

Measurement Data

Crest Factor : 1
 Scan Type : Complete
 Tissue Temp. : 20.00 °C
 Ambient Temp. : 23.00 °C
 Set-up Date : 29-Apr-2008
 Set-up Time : 8:26:24 AM
 Area Scan : 7x5x1 : Measurement x=10mm, y=10mm, z=4mm
 Zoom Scan : 5x5x8 : Measurement x=8mm, y=8mm, z=4mm

Other Data

DUT Position : Touch
 Separation : 0
 Channel : Mid

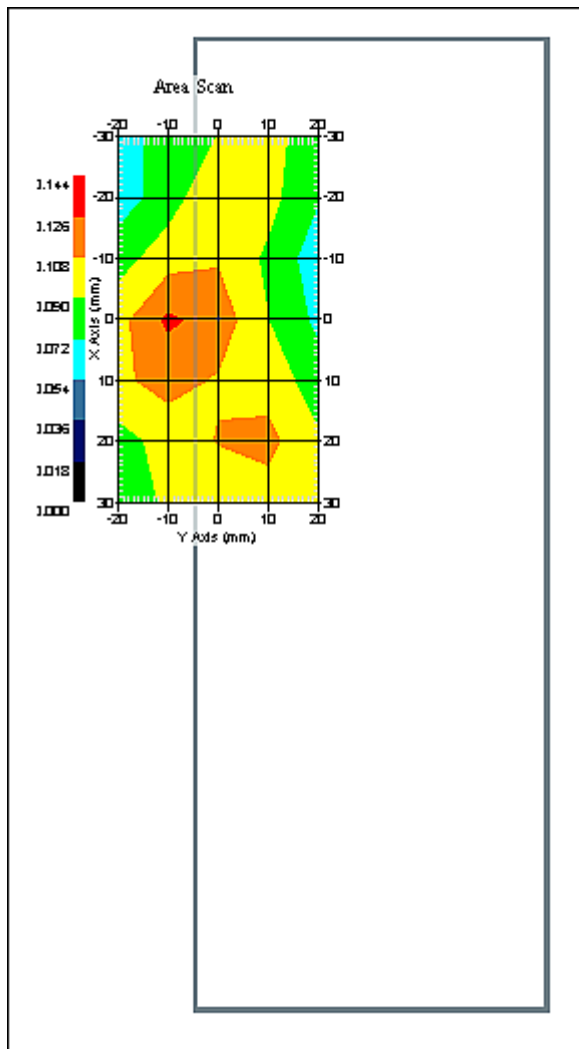

1 gram SAR value : 0.117 W/kg
 10 gram SAR value : 0.085 W/kg
 Area Scan Peak SAR : 0.129 W/kg
 Zoom Scan Peak SAR : 0.180 W/kg

SAR Test Report

By Operator : Jay
Measurement Date : 29-Apr-2008
Starting Time : 29-Apr-2008 12:01:03 PM
End Time : 29-Apr-2008 12:15:09 PM
Scanning Time : 846 secs

Product Data

Device Name : LXE
Serial No. : MX8 Eng 1
Type : Other
Model : MX8
Frequency : 2450.00 MHz
Max. Transmit Pwr : 0.03 W
Drift Time : 0 min(s)
Length : 188 mm
Width : 70 mm
Depth : 40 mm
Antenna Type : Internal
Orientation : Touch
Power Drift-Start : 0.124 W/kg
Power Drift-Finish: 0.120 W/kg
Power Drift (%) : -3.240

Phantom Data

Name : APREL-Uni
Type : Uni-Phantom
Size (mm) : 280 x 280 x 200
Serial No. : System Default
Location : Center
Description : Uni-Phantom

Tissue Data

Type : BODY
Serial No. : 2450
Frequency : 2450.00 MHz
Last Calib. Date : 29-Apr-2008
Temperature : 20.00 °C
Ambient Temp. : 24.00 °C
Humidity : 41.00 RH%
Epsilon : 50.82 F/m
Sigma : 1.87 S/m
Density : 1000.00 kg/cu. m

Probe Data


Name : RFEL 217
Model : E020
Type : E-Field Triangle
Serial No. : 217
Last Calib. Date : 03-Dec-2007
Frequency : 2450.00 MHz
Duty Cycle Factor: 1
Conversion Factor: 3.61
Probe Sensitivity: 1.20 1.20 1.20 $\mu\text{V}/(\text{V/m})^2$
Compression Point: 95.00 mV
Offset : 1.56 mm

Measurement Data

Crest Factor : 1
 Scan Type : Complete
 Tissue Temp. : 20.00 °C
 Ambient Temp. : 23.00 °C
 Set-up Date : 29-Apr-2008
 Set-up Time : 8:26:24 AM
 Area Scan : 7x5x1 : Measurement x=10mm, y=10mm, z=4mm
 Zoom Scan : 5x5x8 : Measurement x=8mm, y=8mm, z=4mm

Other Data

DUT Position : Touch
 Separation : 0
 Channel : High

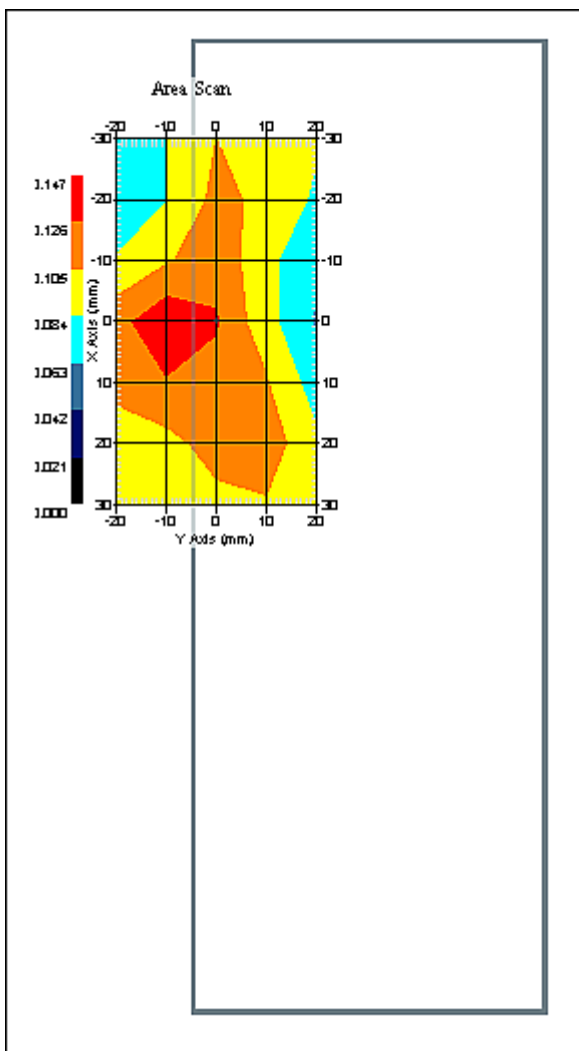

1 gram SAR value : 0.128 W/kg
 10 gram SAR value : 0.089 W/kg
 Area Scan Peak SAR : 0.144 W/kg
 Zoom Scan Peak SAR : 0.210 W/kg

SAR Test Report

By Operator : Jay
Measurement Date : 29-Apr-2008
Starting Time : 29-Apr-2008 02:19:06 PM
End Time : 29-Apr-2008 02:33:09 PM
Scanning Time : 843 secs

Product Data

Device Name : LXE
Serial No. : MX8 Eng 1
Type : Other
Model : MX8
Frequency : 2450.00 MHz
Max. Transmit Pwr : 0.03 W
Drift Time : 0 min(s)
Length : 188 mm
Width : 70 mm
Depth : 40 mm
Antenna Type : Internal
Orientation : Touch
Power Drift-Start : 0.249 W/kg
Power Drift-Finish: 0.243 W/kg
Power Drift (%) : -2.410

Phantom Data

Name : APREL-Uni
Type : Uni-Phantom
Size (mm) : 280 x 280 x 200
Serial No. : System Default
Location : Center
Description : Uni-Phantom

Tissue Data

Type : BODY
Serial No. : 2450
Frequency : 2450.00 MHz
Last Calib. Date : 29-Apr-2008
Temperature : 20.00 °C
Ambient Temp. : 24.00 °C
Humidity : 41.00 RH%
Epsilon : 50.82 F/m
Sigma : 1.87 S/m
Density : 1000.00 kg/cu. m

Probe Data


Name : RFEL 217
Model : E020
Type : E-Field Triangle
Serial No. : 217
Last Calib. Date : 03-Dec-2007
Frequency : 2450.00 MHz
Duty Cycle Factor: 1
Conversion Factor: 3.61
Probe Sensitivity: 1.20 1.20 1.20 $\mu\text{V}/(\text{V/m})^2$
Compression Point: 95.00 mV
Offset : 1.56 mm

Measurement Data

Crest Factor : 1
 Scan Type : Complete
 Tissue Temp. : 20.00 °C
 Ambient Temp. : 23.00 °C
 Set-up Date : 29-Apr-2008
 Set-up Time : 8:26:24 AM
 Area Scan : 7x5x1 : Measurement x=10mm, y=10mm, z=4mm
 Zoom Scan : 5x5x8 : Measurement x=8mm, y=8mm, z=4mm

Other Data

DUT Position : Touch
 Separation : 0
 Channel : Low

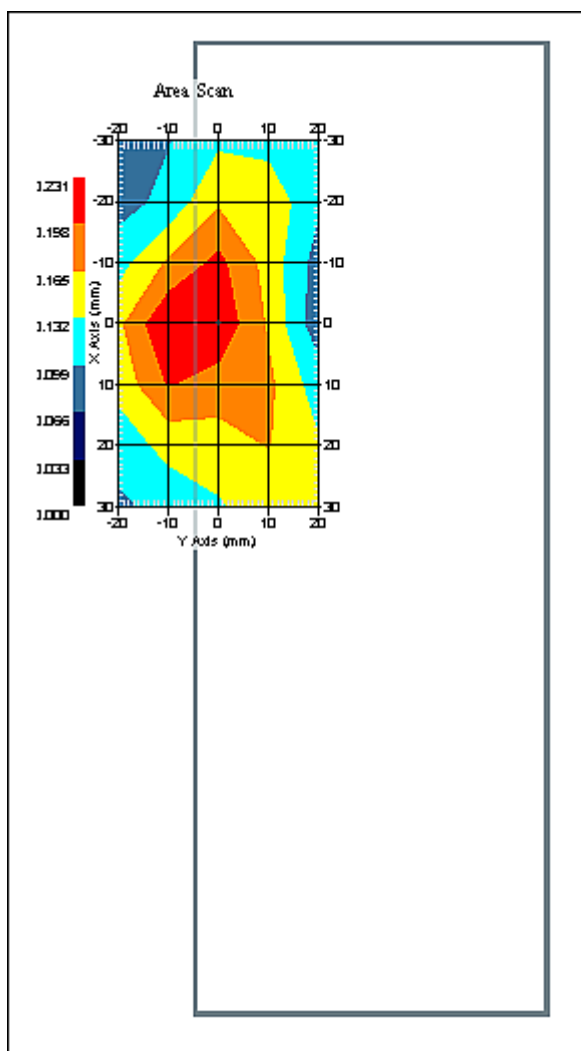

1 gram SAR value : 0.234 W/kg
 10 gram SAR value : 0.144 W/kg
 Area Scan Peak SAR : 0.230 W/kg
 Zoom Scan Peak SAR : 0.390 W/kg

SAR Test Report

By Operator : Jay
Measurement Date : 29-Apr-2008
Starting Time : 29-Apr-2008 02:44:27 PM
End Time : 29-Apr-2008 02:58:28 PM
Scanning Time : 841 secs

Product Data

Device Name : LXE
Serial No. : MX8 Eng 1
Type : Other
Model : MX8
Frequency : 2450.00 MHz
Max. Transmit Pwr : 0.03 W
Drift Time : 0 min(s)
Length : 188 mm
Width : 70 mm
Depth : 40 mm
Antenna Type : Internal
Orientation : Touch
Power Drift-Start : 0.228 W/kg
Power Drift-Finish: 0.221 W/kg
Power Drift (%) : -3.058

Phantom Data

Name : APREL-Uni
Type : Uni-Phantom
Size (mm) : 280 x 280 x 200
Serial No. : System Default
Location : Center
Description : Uni-Phantom

Tissue Data

Type : BODY
Serial No. : 2450
Frequency : 2450.00 MHz
Last Calib. Date : 29-Apr-2008
Temperature : 20.00 °C
Ambient Temp. : 24.00 °C
Humidity : 41.00 RH%
Epsilon : 50.82 F/m
Sigma : 1.87 S/m
Density : 1000.00 kg/cu. m

Probe Data


Name : RFEL 217
Model : E020
Type : E-Field Triangle
Serial No. : 217
Last Calib. Date : 03-Dec-2007
Frequency : 2450.00 MHz
Duty Cycle Factor: 1
Conversion Factor: 3.61
Probe Sensitivity: 1.20 1.20 1.20 $\mu\text{V}/(\text{V/m})^2$
Compression Point: 95.00 mV
Offset : 1.56 mm

Measurement Data

Crest Factor : 1
 Scan Type : Complete
 Tissue Temp. : 20.00 °C
 Ambient Temp. : 23.00 °C
 Set-up Date : 29-Apr-2008
 Set-up Time : 8:26:24 AM
 Area Scan : 7x5x1 : Measurement x=10mm, y=10mm, z=4mm
 Zoom Scan : 5x5x8 : Measurement x=8mm, y=8mm, z=4mm

Other Data

DUT Position : Touch
 Separation : 0
 Channel : Mid

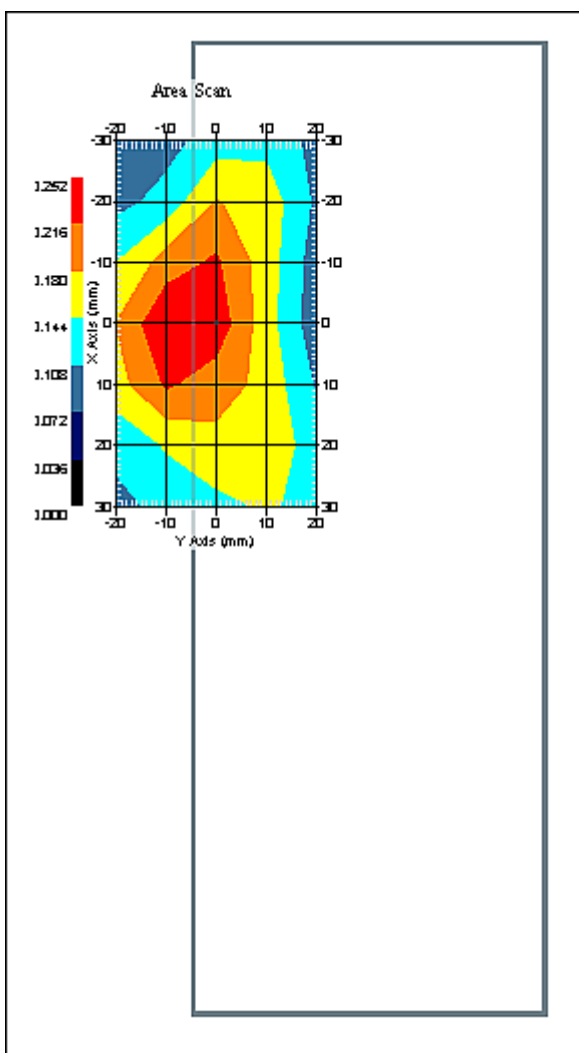

1 gram SAR value : 0.232 W/kg
 10 gram SAR value : 0.144 W/kg
 Area Scan Peak SAR : 0.252 W/kg
 Zoom Scan Peak SAR : 0.370 W/kg

SAR Test Report

By Operator : Jay
Measurement Date : 29-Apr-2008
Starting Time : 29-Apr-2008 03:01:33 PM
End Time : 29-Apr-2008 03:15:28 PM
Scanning Time : 835 secs

Product Data

Device Name : LXE
Serial No. : MX8 Eng 1
Type : Other
Model : MX8
Frequency : 2450.00 MHz
Max. Transmit Pwr : 0.03 W
Drift Time : 0 min(s)
Length : 188 mm
Width : 70 mm
Depth : 40 mm
Antenna Type : Internal
Orientation : Touch
Power Drift-Start : 0.271 W/kg
Power Drift-Finish: 0.262 W/kg
Power Drift (%) : -3.315

Phantom Data

Name : APREL-Uni
Type : Uni-Phantom
Size (mm) : 280 x 280 x 200
Serial No. : System Default
Location : Center
Description : Uni-Phantom

Tissue Data

Type : BODY
Serial No. : 2450
Frequency : 2450.00 MHz
Last Calib. Date : 29-Apr-2008
Temperature : 20.00 °C
Ambient Temp. : 24.00 °C
Humidity : 41.00 RH%
Epsilon : 50.82 F/m
Sigma : 1.87 S/m
Density : 1000.00 kg/cu. m

Probe Data


Name : RFEL 217
Model : E020
Type : E-Field Triangle
Serial No. : 217
Last Calib. Date : 03-Dec-2007
Frequency : 2450.00 MHz
Duty Cycle Factor: 1
Conversion Factor: 3.61
Probe Sensitivity: 1.20 1.20 1.20 $\mu\text{V}/(\text{V/m})^2$
Compression Point: 95.00 mV
Offset : 1.56 mm

Measurement Data

Crest Factor : 1
Scan Type : Complete
Tissue Temp. : 20.00 °C
Ambient Temp. : 23.00 °C
Set-up Date : 29-Apr-2008
Set-up Time : 8:26:24 AM
Area Scan : 7x5x1 : Measurement x=10mm, y=10mm, z=4mm
Zoom Scan : 5x5x8 : Measurement x=8mm, y=8mm, z=4mm


Other Data

DUT Position : Touch
Separation : 0
Channel : High

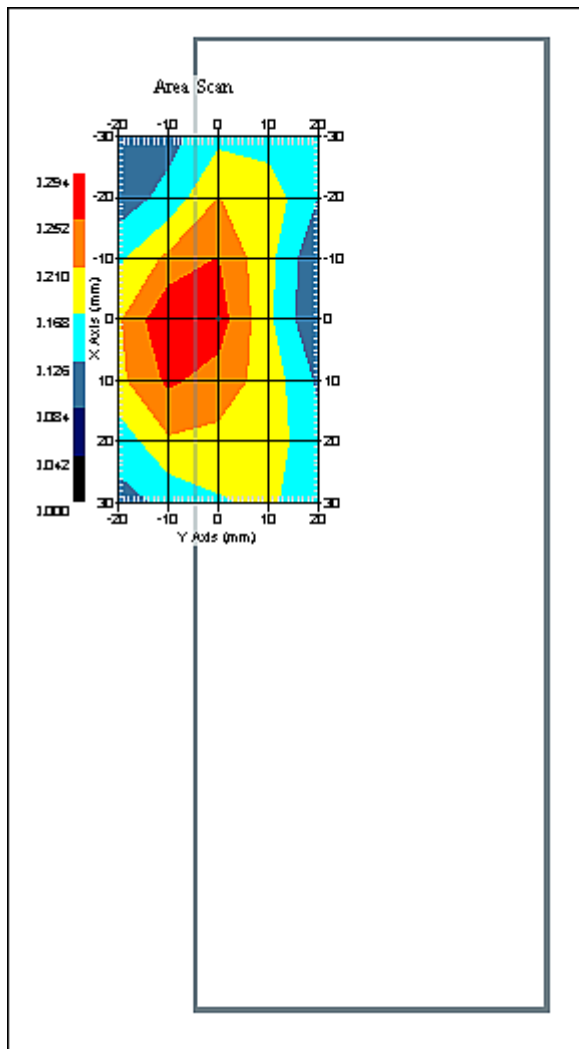

1 gram SAR value : 0.276 W/kg
10 gram SAR value : 0.169 W/kg
Area Scan Peak SAR : 0.291 W/kg
Zoom Scan Peak SAR : 0.460 W/kg

SAR-Z Axis
at Hotspot x:0.25 y:-10.13

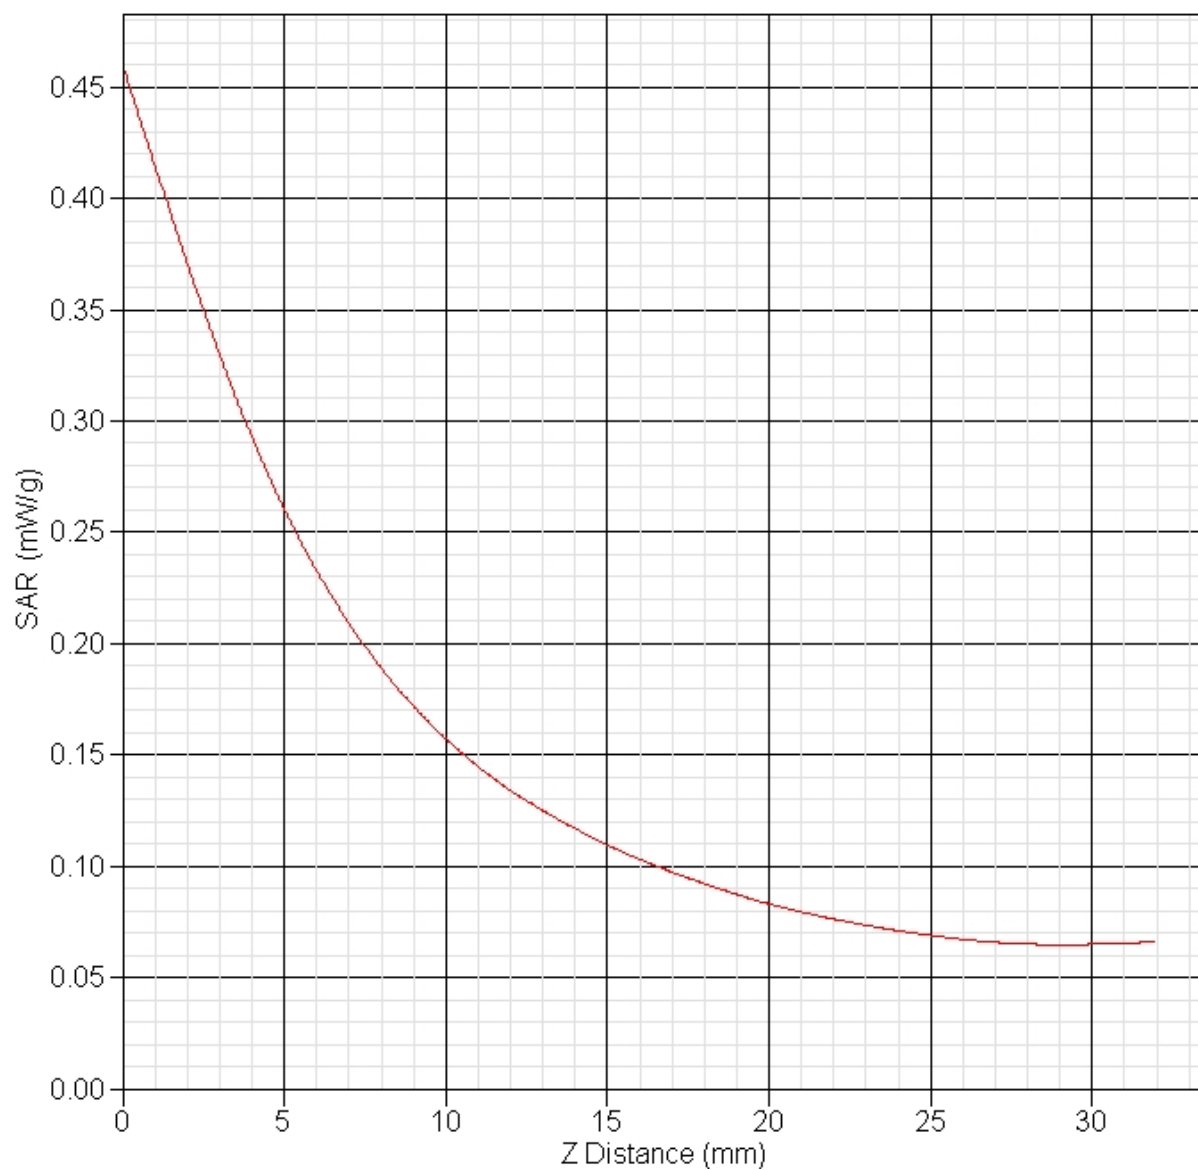

SAR Test Report

By Operator : Jay
Measurement Date : 29-Apr-2008
Starting Time : 29-Apr-2008 12:30:49 PM
End Time : 29-Apr-2008 12:44:53 PM
Scanning Time : 844 secs

Product Data

Device Name : LXE
Serial No. : MX8 Eng 1
Type : Other
Model : MX8
Frequency : 2450.00 MHz
Max. Transmit Pwr : 0.03 W
Drift Time : 0 min(s)
Length : 188 mm
Width : 70 mm
Depth : 40 mm
Antenna Type : Internal
Orientation : Touch
Power Drift-Start : 0.104 W/kg
Power Drift-Finish: 0.101 W/kg
Power Drift (%) : -2.844

Phantom Data

Name : APREL-Uni
Type : Uni-Phantom
Size (mm) : 280 x 280 x 200
Serial No. : System Default
Location : Center
Description : Uni-Phantom

Tissue Data

Type : BODY
Serial No. : 2450
Frequency : 2450.00 MHz
Last Calib. Date : 29-Apr-2008
Temperature : 20.00 °C
Ambient Temp. : 24.00 °C
Humidity : 41.00 RH%
Epsilon : 50.82 F/m
Sigma : 1.87 S/m
Density : 1000.00 kg/cu. m

Probe Data


Name : RFEL 217
Model : E020
Type : E-Field Triangle
Serial No. : 217
Last Calib. Date : 03-Dec-2007
Frequency : 2450.00 MHz
Duty Cycle Factor: 1
Conversion Factor: 3.61
Probe Sensitivity: 1.20 1.20 1.20 $\mu\text{V}/(\text{V/m})^2$
Compression Point: 95.00 mV
Offset : 1.56 mm

Measurement Data

Crest Factor : 1
 Scan Type : Complete
 Tissue Temp. : 20.00 °C
 Ambient Temp. : 23.00 °C
 Set-up Date : 29-Apr-2008
 Set-up Time : 8:26:24 AM
 Area Scan : 7x5x1 : Measurement x=10mm, y=10mm, z=4mm
 Zoom Scan : 5x5x8 : Measurement x=8mm, y=8mm, z=4mm

Other Data

DUT Position : Touch
 Separation : 0
 Channel : Low

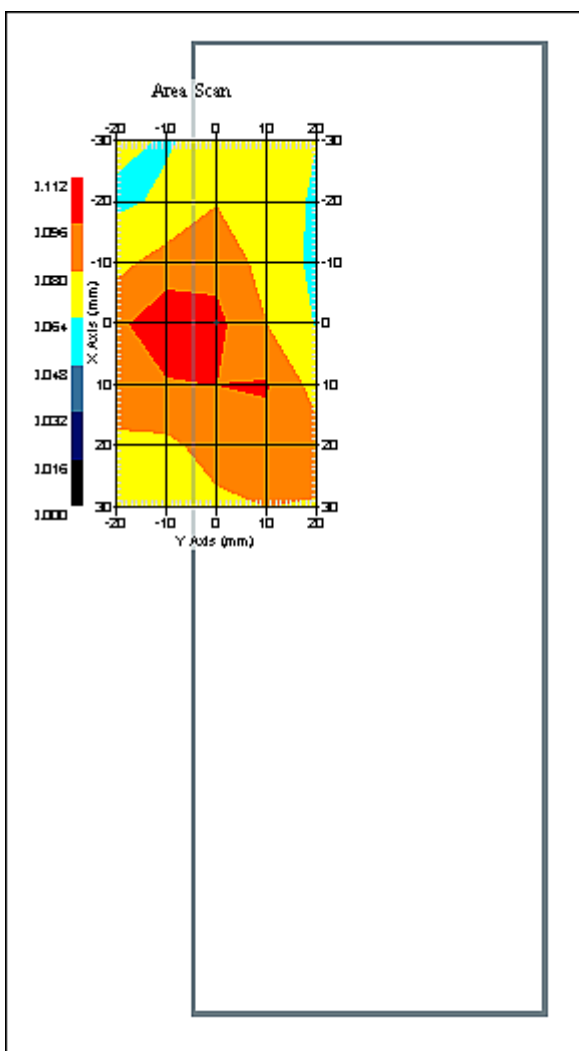

1 gram SAR value : 0.096 W/kg
 10 gram SAR value : 0.075 W/kg
 Area Scan Peak SAR : 0.109 W/kg
 Zoom Scan Peak SAR : 0.120 W/kg

SAR Test Report

By Operator : Jay
Measurement Date : 29-Apr-2008
Starting Time : 29-Apr-2008 01:15:45 PM
End Time : 29-Apr-2008 01:29:48 PM
Scanning Time : 843 secs

Product Data

Device Name : LXE
Serial No. : MX8 Eng 1
Type : Other
Model : MX8
Frequency : 2450.00 MHz
Max. Transmit Pwr : 0.03 W
Drift Time : 0 min(s)
Length : 188 mm
Width : 70 mm
Depth : 40 mm
Antenna Type : Internal
Orientation : Touch
Power Drift-Start : 0.124 W/kg
Power Drift-Finish: 0.123 W/kg
Power Drift (%) : -0.883

Phantom Data

Name : APREL-Uni
Type : Uni-Phantom
Size (mm) : 280 x 280 x 200
Serial No. : System Default
Location : Center
Description : Uni-Phantom

Tissue Data

Type : BODY
Serial No. : 2450
Frequency : 2450.00 MHz
Last Calib. Date : 29-Apr-2008
Temperature : 20.00 °C
Ambient Temp. : 24.00 °C
Humidity : 41.00 RH%
Epsilon : 50.82 F/m
Sigma : 1.87 S/m
Density : 1000.00 kg/cu. m

Probe Data


Name : RFEL 217
Model : E020
Type : E-Field Triangle
Serial No. : 217
Last Calib. Date : 03-Dec-2007
Frequency : 2450.00 MHz
Duty Cycle Factor: 1
Conversion Factor: 3.61
Probe Sensitivity: 1.20 1.20 1.20 $\mu\text{V}/(\text{V/m})^2$
Compression Point: 95.00 mV
Offset : 1.56 mm

Measurement Data

Crest Factor : 1
Scan Type : Complete
Tissue Temp. : 20.00 °C
Ambient Temp. : 23.00 °C
Set-up Date : 29-Apr-2008
Set-up Time : 8:26:24 AM
Area Scan : 7x5x1 : Measurement x=10mm, y=10mm, z=4mm
Zoom Scan : 5x5x8 : Measurement x=8mm, y=8mm, z=4mm

Other Data

DUT Position : Touch
Separation : 0
Channel : Mid

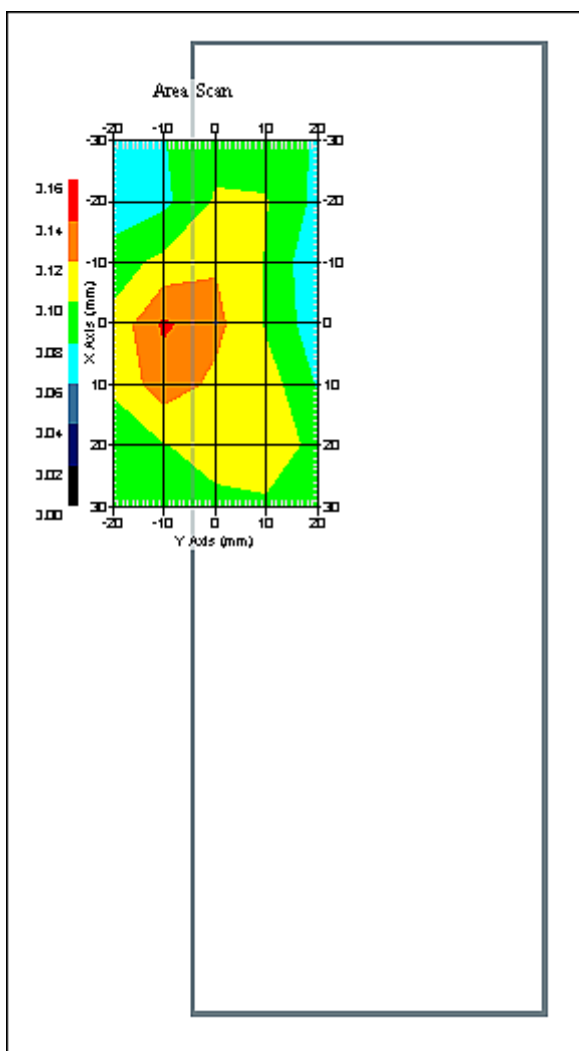

1 gram SAR value : 0.126 W/kg
10 gram SAR value : 0.088 W/kg
Area Scan Peak SAR : 0.143 W/kg
Zoom Scan Peak SAR : 0.200 W/kg

SAR Test Report

By Operator : Jay
Measurement Date : 29-Apr-2008
Starting Time : 29-Apr-2008 01:44:33 PM
End Time : 29-Apr-2008 01:58:26 PM
Scanning Time : 833 secs

Product Data

Device Name : LXE
Serial No. : MX8 Eng 1
Type : Other
Model : MX8
Frequency : 2450.00 MHz
Max. Transmit Pwr : 0.03 W
Drift Time : 0 min(s)
Length : 188 mm
Width : 70 mm
Depth : 40 mm
Antenna Type : Internal
Orientation : Touch
Power Drift-Start : 0.143 W/kg
Power Drift-Finish: 0.138 W/kg
Power Drift (%) : -3.464

Phantom Data

Name : APREL-Uni
Type : Uni-Phantom
Size (mm) : 280 x 280 x 200
Serial No. : System Default
Location : Center
Description : Uni-Phantom

Tissue Data

Type : BODY
Serial No. : 2450
Frequency : 2450.00 MHz
Last Calib. Date : 29-Apr-2008
Temperature : 20.00 °C
Ambient Temp. : 24.00 °C
Humidity : 41.00 RH%
Epsilon : 50.82 F/m
Sigma : 1.87 S/m
Density : 1000.00 kg/cu. m

Probe Data


Name : RFEL 217
Model : E020
Type : E-Field Triangle
Serial No. : 217
Last Calib. Date : 03-Dec-2007
Frequency : 2450.00 MHz
Duty Cycle Factor: 1
Conversion Factor: 3.61
Probe Sensitivity: 1.20 1.20 1.20 $\mu\text{V}/(\text{V/m})^2$
Compression Point: 95.00 mV
Offset : 1.56 mm

Measurement Data

Crest Factor : 1
Scan Type : Complete
Tissue Temp. : 20.00 °C
Ambient Temp. : 23.00 °C
Set-up Date : 29-Apr-2008
Set-up Time : 8:26:24 AM
Area Scan : 7x5x1 : Measurement x=10mm, y=10mm, z=4mm
Zoom Scan : 5x5x8 : Measurement x=8mm, y=8mm, z=4mm

Other Data

DUT Position : Touch
Separation : 0
Channel : High

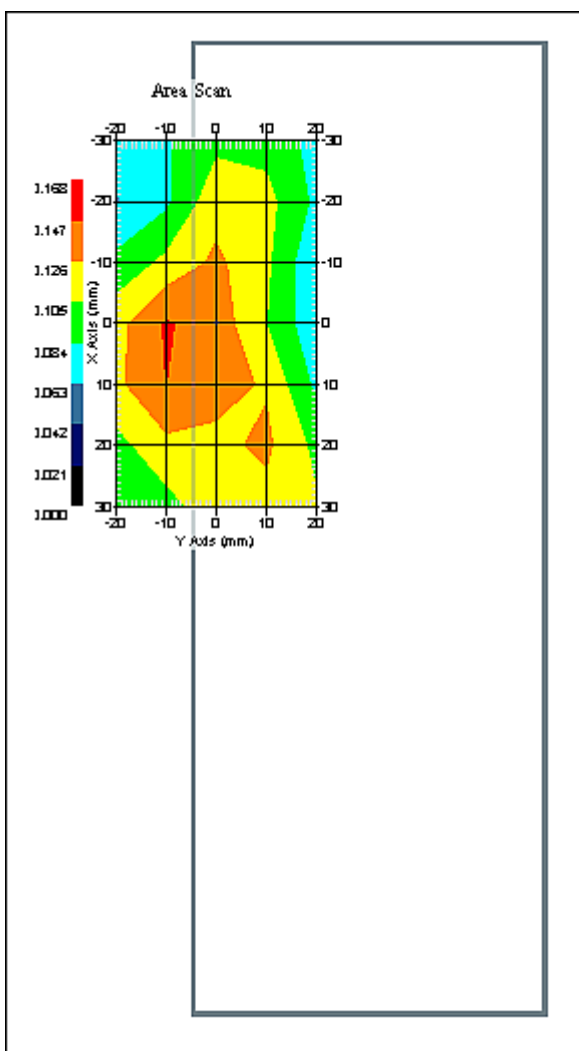

1 gram SAR value : 0.148 W/kg
10 gram SAR value : 0.102 W/kg
Area Scan Peak SAR : 0.149 W/kg
Zoom Scan Peak SAR : 0.190 W/kg

SAR Test Report

By Operator : Jay
Measurement Date : 29-Apr-2008
Starting Time : 29-Apr-2008 03:17:55 PM
End Time : 29-Apr-2008 03:31:51 PM
Scanning Time : 836 secs

Product Data

Device Name : LXE
Serial No. : MX8 Eng 1
Type : Other
Model : MX8
Frequency : 2450.00 MHz
Max. Transmit Pwr : 0.03 W
Drift Time : 0 min(s)
Length : 188 mm
Width : 70 mm
Depth : 40 mm
Antenna Type : Internal
Orientation : Touch
Power Drift-Start : 0.268 W/kg
Power Drift-Finish: 0.255 W/kg
Power Drift (%) : -4.821

Phantom Data

Name : APREL-Uni
Type : Uni-Phantom
Size (mm) : 280 x 280 x 200
Serial No. : System Default
Location : Center
Description : Uni-Phantom

Tissue Data

Type : BODY
Serial No. : 2450
Frequency : 2450.00 MHz
Last Calib. Date : 29-Apr-2008
Temperature : 20.00 °C
Ambient Temp. : 24.00 °C
Humidity : 41.00 RH%
Epsilon : 50.82 F/m
Sigma : 1.87 S/m
Density : 1000.00 kg/cu. m

Probe Data


Name : RFEL 217
Model : E020
Type : E-Field Triangle
Serial No. : 217
Last Calib. Date : 03-Dec-2007
Frequency : 2450.00 MHz
Duty Cycle Factor: 1
Conversion Factor: 3.61
Probe Sensitivity: 1.20 1.20 1.20 $\mu\text{V}/(\text{V/m})^2$
Compression Point: 95.00 mV
Offset : 1.56 mm

Measurement Data

Crest Factor : 1
 Scan Type : Complete
 Tissue Temp. : 20.00 °C
 Ambient Temp. : 23.00 °C
 Set-up Date : 29-Apr-2008
 Set-up Time : 8:26:24 AM
 Area Scan : 7x5x1 : Measurement x=10mm, y=10mm, z=4mm
 Zoom Scan : 5x5x8 : Measurement x=8mm, y=8mm, z=4mm

Other Data

DUT Position : Touch
 Separation : 0
 Channel : Low

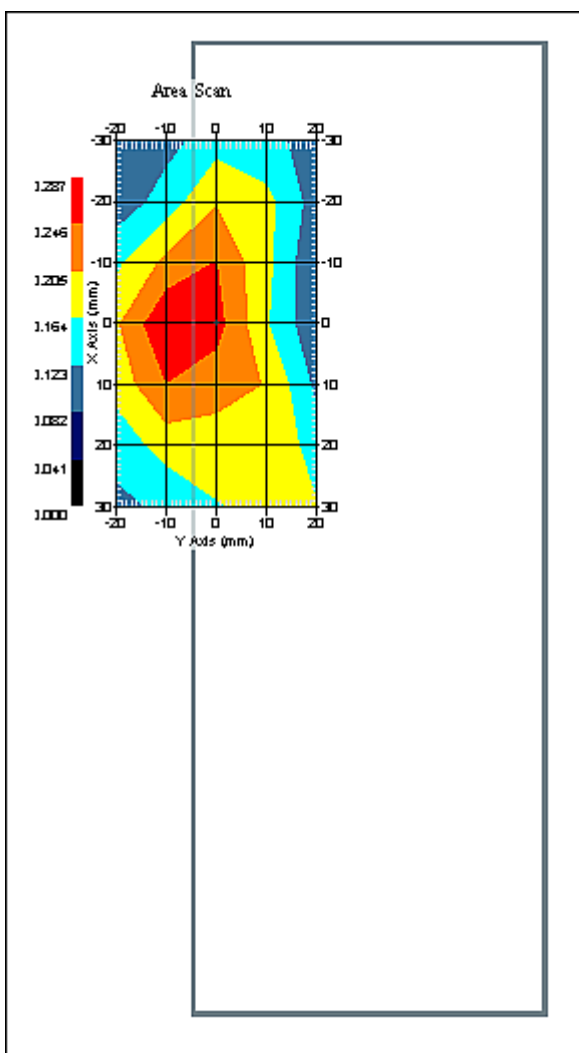

1 gram SAR value : 0.267 W/kg
 10 gram SAR value : 0.164 W/kg
 Area Scan Peak SAR : 0.286 W/kg
 Zoom Scan Peak SAR : 0.440 W/kg

SAR Test Report

By Operator : Jay
Measurement Date : 29-Apr-2008
Starting Time : 29-Apr-2008 03:36:31 PM
End Time : 29-Apr-2008 03:50:34 PM
Scanning Time : 843 secs

Product Data

Device Name : LXE
Serial No. : MX8 Eng 1
Type : Other
Model : MX8
Frequency : 2450.00 MHz
Max. Transmit Pwr : 0.03 W
Drift Time : 0 min(s)
Length : 188 mm
Width : 70 mm
Depth : 40 mm
Antenna Type : Internal
Orientation : Touch
Power Drift-Start : 0.114 W/kg
Power Drift-Finish: 0.110 W/kg
Power Drift (%) : -3.524

Phantom Data

Name : APREL-Uni
Type : Uni-Phantom
Size (mm) : 280 x 280 x 200
Serial No. : System Default
Location : Center
Description : Uni-Phantom

Tissue Data

Type : BODY
Serial No. : 2450
Frequency : 2450.00 MHz
Last Calib. Date : 29-Apr-2008
Temperature : 20.00 °C
Ambient Temp. : 24.00 °C
Humidity : 41.00 RH%
Epsilon : 50.82 F/m
Sigma : 1.87 S/m
Density : 1000.00 kg/cu. m

Probe Data


Name : RFEL 217
Model : E020
Type : E-Field Triangle
Serial No. : 217
Last Calib. Date : 03-Dec-2007
Frequency : 2450.00 MHz
Duty Cycle Factor: 1
Conversion Factor: 3.61
Probe Sensitivity: 1.20 1.20 1.20 $\mu\text{V}/(\text{V/m})^2$
Compression Point: 95.00 mV
Offset : 1.56 mm

Measurement Data

Crest Factor : 1
 Scan Type : Complete
 Tissue Temp. : 20.00 °C
 Ambient Temp. : 23.00 °C
 Set-up Date : 29-Apr-2008
 Set-up Time : 8:26:24 AM
 Area Scan : 7x5x1 : Measurement x=10mm, y=10mm, z=4mm
 Zoom Scan : 5x5x8 : Measurement x=8mm, y=8mm, z=4mm

Other Data

DUT Position : Touch
 Separation : 0
 Channel : Mid

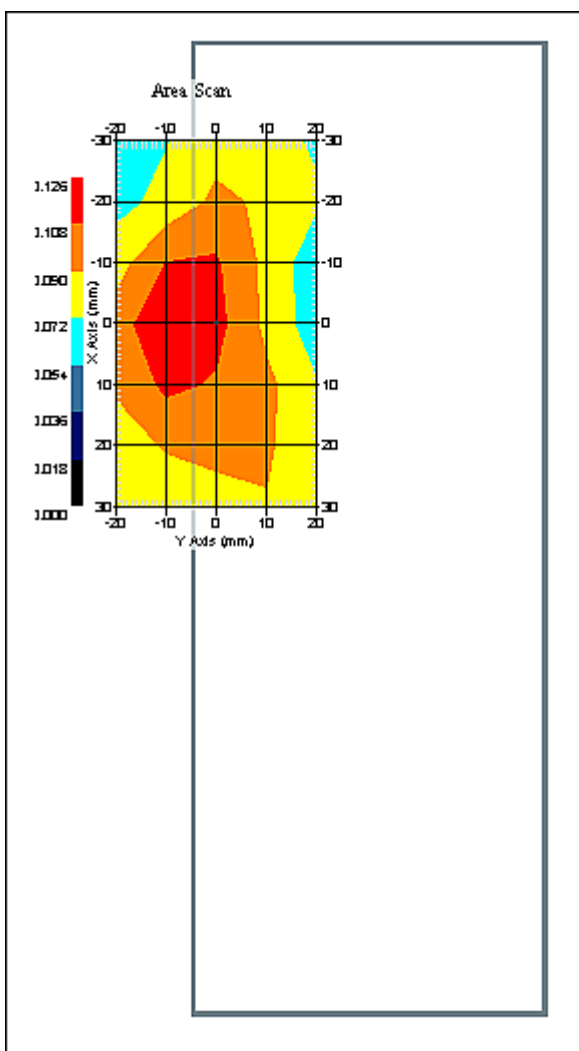

1 gram SAR value : 0.117 W/kg
 10 gram SAR value : 0.085 W/kg
 Area Scan Peak SAR : 0.125 W/kg
 Zoom Scan Peak SAR : 0.190 W/kg

SAR Test Report

By Operator : Jay
Measurement Date : 29-Apr-2008
Starting Time : 29-Apr-2008 03:56:39 PM
End Time : 29-Apr-2008 04:10:39 PM
Scanning Time : 840 secs

Product Data

Device Name : LXE
Serial No. : MX8 Eng 1
Type : Other
Model : MX8
Frequency : 2450.00 MHz
Max. Transmit Pwr : 0.03 W
Drift Time : 0 min(s)
Length : 188 mm
Width : 70 mm
Depth : 40 mm
Antenna Type : Internal
Orientation : Touch
Power Drift-Start : 0.111 W/kg
Power Drift-Finish: 0.112 W/kg
Power Drift (%) : 0.609

Phantom Data

Name : APREL-Uni
Type : Uni-Phantom
Size (mm) : 280 x 280 x 200
Serial No. : System Default
Location : Center
Description : Uni-Phantom

Tissue Data

Type : BODY
Serial No. : 2450
Frequency : 2450.00 MHz
Last Calib. Date : 29-Apr-2008
Temperature : 20.00 °C
Ambient Temp. : 24.00 °C
Humidity : 41.00 RH%
Epsilon : 50.82 F/m
Sigma : 1.87 S/m
Density : 1000.00 kg/cu. m

Probe Data


Name : RFEL 217
Model : E020
Type : E-Field Triangle
Serial No. : 217
Last Calib. Date : 03-Dec-2007
Frequency : 2450.00 MHz
Duty Cycle Factor: 1
Conversion Factor: 3.61
Probe Sensitivity: 1.20 1.20 1.20 $\mu\text{V}/(\text{V/m})^2$
Compression Point: 95.00 mV
Offset : 1.56 mm

Measurement Data

Crest Factor : 1
 Scan Type : Complete
 Tissue Temp. : 20.00 °C
 Ambient Temp. : 23.00 °C
 Set-up Date : 29-Apr-2008
 Set-up Time : 8:26:24 AM
 Area Scan : 7x5x1 : Measurement x=10mm, y=10mm, z=4mm
 Zoom Scan : 5x5x8 : Measurement x=8mm, y=8mm, z=4mm

Other Data

DUT Position : Touch
 Separation : 0
 Channel : High

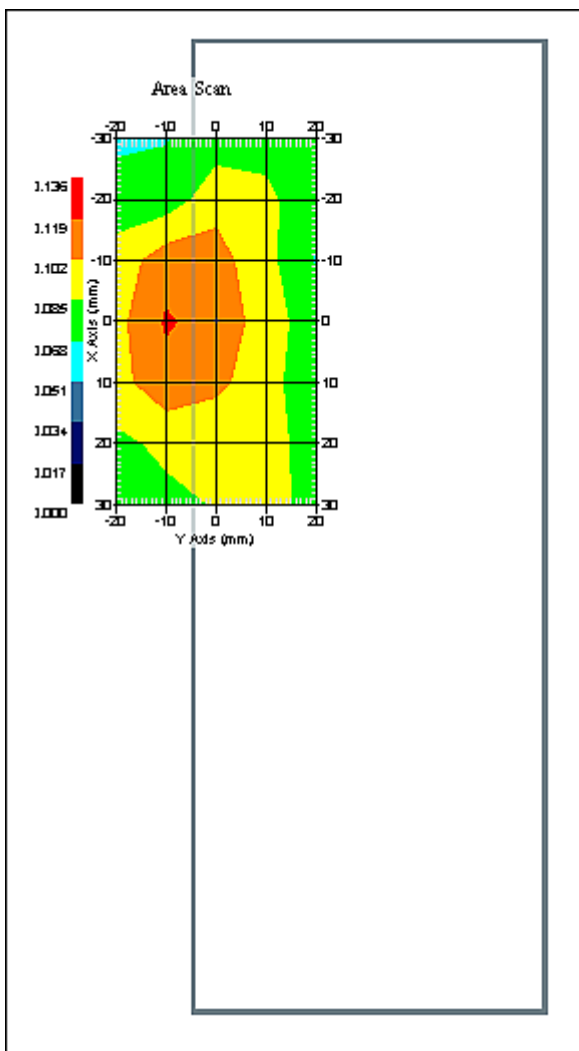

1 gram SAR value : 0.124 W/kg
 10 gram SAR value : 0.085 W/kg
 Area Scan Peak SAR : 0.121 W/kg
 Zoom Scan Peak SAR : 0.210 W/kg

SAR Test Report

By Operator : Jay
Measurement Date : 30-Apr-2008
Starting Time : 30-Apr-2008 04:38:47 PM
End Time : 30-Apr-2008 05:01:48 PM
Scanning Time : 1381 secs

Product Data

Device Name : LXE
Serial No. : MX8 Eng 1
Type : Other
Model : MX8
Frequency : 5200.00 MHz
Max. Transmit Pwr : 0.02 W
Drift Time : 0 min(s)
Length : 188 mm
Width : 70 mm
Depth : 40 mm
Antenna Type : Internal
Orientation : Touch
Power Drift-Start : 0.098 W/kg
Power Drift-Finish: 0.094 W/kg
Power Drift (%) : -4.050

Phantom Data

Name : APREL-Uni
Type : Uni-Phantom
Size (mm) : 280 x 280 x 200
Serial No. : System Default
Location : Center
Description : Uni-Phantom

Tissue Data

Type : BODY
Serial No. : 5200
Frequency : 5200.00 MHz
Last Calib. Date : 30-Apr-2008
Temperature : 20.00 °C
Ambient Temp. : 23.00 °C
Humidity : 50.00 RH%
Epsilon : 48.83 F/m
Sigma : 5.31 S/m
Density : 1000.00 kg/cu. m

Probe Data


Name : Probe AL-E3P1 - AL
Model : E-030
Type : E-Field Triangle
Serial No. : AL-E3P1
Last Calib. Date : 30-Apr-2007
Frequency : 5200.00 MHz
Duty Cycle Factor: 1
Conversion Factor: 13
Probe Sensitivity: 1.20 1.20 1.20 $\mu\text{V}/(\text{V/m})^2$
Compression Point: 95.00 mV
Offset : 0.56 mm

Measurement Data

Crest Factor : 1
 Scan Type : Complete
 Tissue Temp. : 20.00 °C
 Ambient Temp. : 23.00 °C
 Set-up Date : 30-Apr-2008
 Set-up Time : 3:01:32 PM
 Area Scan : 7x5x1 : Measurement x=10mm, y=10mm, z=2mm
 Zoom Scan : 7x7x10 : Measurement x=4mm, y=4mm, z=2.5mm

Other Data

DUT Position : Touch
 Separation : 0
 Channel : Low

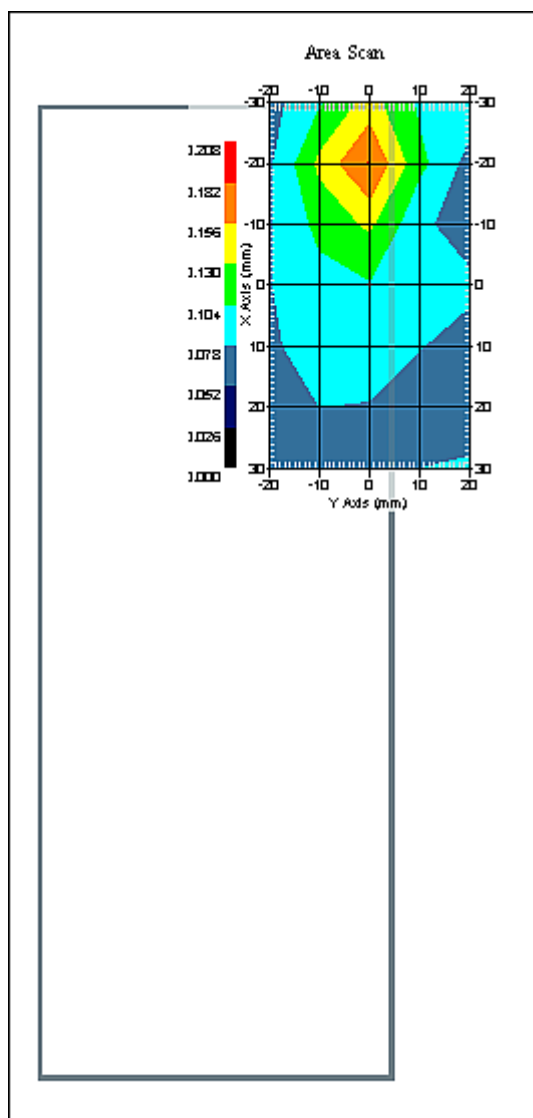

1 gram SAR value : 0.138 W/kg
 10 gram SAR value : 0.090 W/kg
 Area Scan Peak SAR : 0.184 W/kg
 Zoom Scan Peak SAR : 0.240 W/kg

SAR Test Report

By Operator : Jay
Measurement Date : 30-Apr-2008
Starting Time : 30-Apr-2008 04:11:27 PM
End Time : 30-Apr-2008 04:34:24 PM
Scanning Time : 1377 secs

Product Data

Device Name : LXE
Serial No. : MX8 Eng 1
Type : Other
Model : MX8
Frequency : 5200.00 MHz
Max. Transmit Pwr : 0.02 W
Drift Time : 0 min(s)
Length : 188 mm
Width : 70 mm
Depth : 40 mm
Antenna Type : Internal
Orientation : Touch
Power Drift-Start : 0.201 W/kg
Power Drift-Finish: 0.197 W/kg
Power Drift (%) : -1.948

Phantom Data

Name : APREL-Uni
Type : Uni-Phantom
Size (mm) : 280 x 280 x 200
Serial No. : System Default
Location : Center
Description : Uni-Phantom

Tissue Data

Type : BODY
Serial No. : 5200
Frequency : 5200.00 MHz
Last Calib. Date : 30-Apr-2008
Temperature : 20.00 °C
Ambient Temp. : 23.00 °C
Humidity : 50.00 RH%
Epsilon : 48.83 F/m
Sigma : 5.31 S/m
Density : 1000.00 kg/cu. m

Probe Data


Name : Probe AL-E3P1 - AL
Model : E-030
Type : E-Field Triangle
Serial No. : AL-E3P1
Last Calib. Date : 30-Apr-2007
Frequency : 5200.00 MHz
Duty Cycle Factor: 1
Conversion Factor: 13
Probe Sensitivity: 1.20 1.20 1.20 $\mu\text{V}/(\text{V/m})^2$
Compression Point: 95.00 mV
Offset : 0.56 mm

Measurement Data

Crest Factor : 1
 Scan Type : Complete
 Tissue Temp. : 20.00 °C
 Ambient Temp. : 23.00 °C
 Set-up Date : 30-Apr-2008
 Set-up Time : 3:01:32 PM
 Area Scan : 7x5x1 : Measurement x=10mm, y=10mm, z=2mm
 Zoom Scan : 7x7x10 : Measurement x=4mm, y=4mm, z=2.5mm


Other Data

DUT Position : Touch
 Separation : 0
 Channel : High

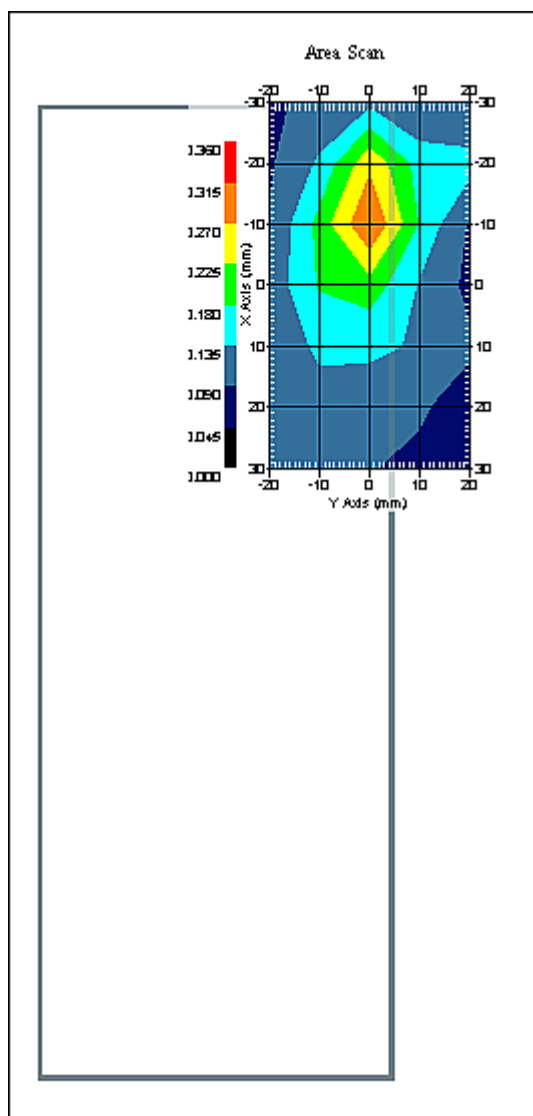

1 gram SAR value : 0.244 W/kg
 10 gram SAR value : 0.126 W/kg
 Area Scan Peak SAR : 0.316 W/kg
 Zoom Scan Peak SAR : 0.490 W/kg

SAR-Z Axis
at Hotspot x:-13.75 y:-0.17

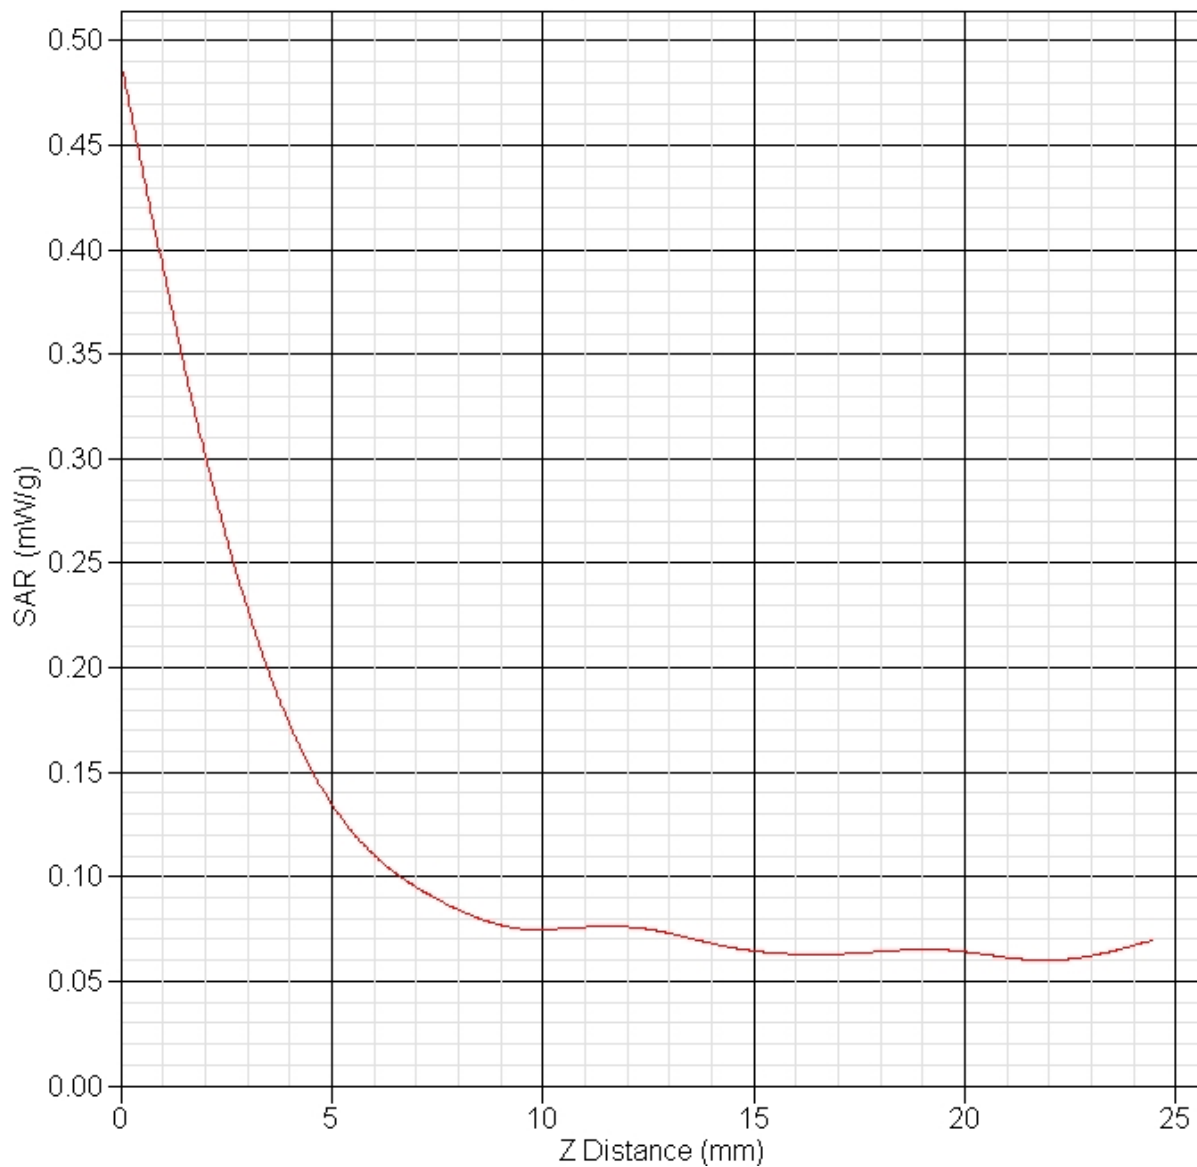

SAR Test Report

By Operator : Jay
Measurement Date : 30-Apr-2008
Starting Time : 30-Apr-2008 05:05:54 PM
End Time : 30-Apr-2008 05:28:44 PM
Scanning Time : 1370 secs

Product Data

Device Name : LXE
Serial No. : MX8 Eng 1
Type : Other
Model : MX8
Frequency : 5200.00 MHz
Max. Transmit Pwr : 0.02 W
Drift Time : 0 min(s)
Length : 188 mm
Width : 70 mm
Depth : 40 mm
Antenna Type : Internal
Orientation : Touch
Power Drift-Start : 0.104 W/kg
Power Drift-Finish: 0.101 W/kg
Power Drift (%) : -2.861

Phantom Data

Name : APREL-Uni
Type : Uni-Phantom
Size (mm) : 280 x 280 x 200
Serial No. : System Default
Location : Center
Description : Uni-Phantom

Tissue Data

Type : BODY
Serial No. : 5200
Frequency : 5200.00 MHz
Last Calib. Date : 30-Apr-2008
Temperature : 20.00 °C
Ambient Temp. : 23.00 °C
Humidity : 50.00 RH%
Epsilon : 48.83 F/m
Sigma : 5.31 S/m
Density : 1000.00 kg/cu. m

Probe Data


Name : Probe AL-E3P1 - AL
Model : E-030
Type : E-Field Triangle
Serial No. : AL-E3P1
Last Calib. Date : 30-Apr-2007
Frequency : 5200.00 MHz
Duty Cycle Factor: 1
Conversion Factor: 13
Probe Sensitivity: 1.20 1.20 1.20 $\mu\text{V}/(\text{V/m})^2$
Compression Point: 95.00 mV
Offset : 0.56 mm

Measurement Data

Crest Factor : 1
 Scan Type : Complete
 Tissue Temp. : 20.00 °C
 Ambient Temp. : 23.00 °C
 Set-up Date : 30-Apr-2008
 Set-up Time : 3:01:32 PM
 Area Scan : 7x5x1 : Measurement x=10mm, y=10mm, z=2mm
 Zoom Scan : 7x7x10 : Measurement x=4mm, y=4mm, z=2.5mm

Other Data

DUT Position : Touch
 Separation : 0
 Channel : Low

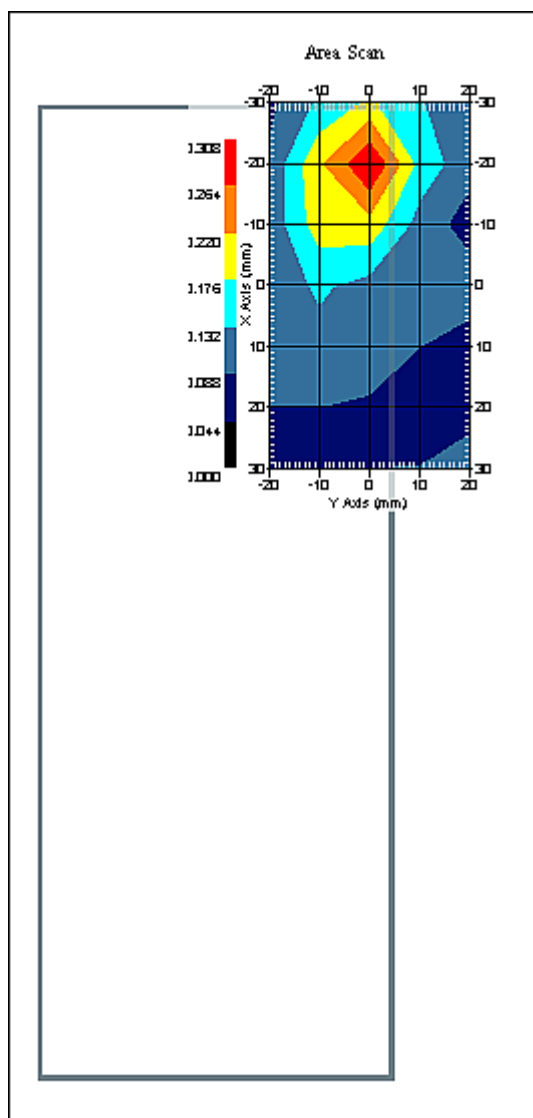

1 gram SAR value : 0.221 W/kg
 10 gram SAR value : 0.112 W/kg
 Area Scan Peak SAR : 0.308 W/kg
 Zoom Scan Peak SAR : 0.430 W/kg

SAR Test Report

By Operator : Jay
Measurement Date : 30-Apr-2008
Starting Time : 30-Apr-2008 05:33:45 PM
End Time : 30-Apr-2008 05:56:45 PM
Scanning Time : 1380 secs

Product Data

Device Name : LXE
Serial No. : MX8 Eng 1
Type : Other
Model : MX8
Frequency : 5200.00 MHz
Max. Transmit Pwr : 0.02 W
Drift Time : 0 min(s)
Length : 188 mm
Width : 70 mm
Depth : 40 mm
Antenna Type : Internal
Orientation : Touch
Power Drift-Start : 0.118 W/kg
Power Drift-Finish: 0.112 W/kg
Power Drift (%) : -4.866

Phantom Data

Name : APREL-Uni
Type : Uni-Phantom
Size (mm) : 280 x 280 x 200
Serial No. : System Default
Location : Center
Description : Uni-Phantom

Tissue Data

Type : BODY
Serial No. : 5200
Frequency : 5200.00 MHz
Last Calib. Date : 30-Apr-2008
Temperature : 20.00 °C
Ambient Temp. : 23.00 °C
Humidity : 50.00 RH%
Epsilon : 48.83 F/m
Sigma : 5.31 S/m
Density : 1000.00 kg/cu. m

Probe Data


Name : Probe AL-E3P1 - AL
Model : E-030
Type : E-Field Triangle
Serial No. : AL-E3P1
Last Calib. Date : 30-Apr-2007
Frequency : 5200.00 MHz
Duty Cycle Factor: 1
Conversion Factor: 13
Probe Sensitivity: 1.20 1.20 1.20 $\mu\text{V}/(\text{V/m})^2$
Compression Point: 95.00 mV
Offset : 0.56 mm

Measurement Data

Crest Factor : 1
 Scan Type : Complete
 Tissue Temp. : 20.00 °C
 Ambient Temp. : 23.00 °C
 Set-up Date : 30-Apr-2008
 Set-up Time : 3:01:32 PM
 Area Scan : 7x5x1 : Measurement x=10mm, y=10mm, z=2mm
 Zoom Scan : 7x7x10 : Measurement x=4mm, y=4mm, z=2.5mm

Other Data

DUT Position : Touch
 Separation : 0
 Channel : High

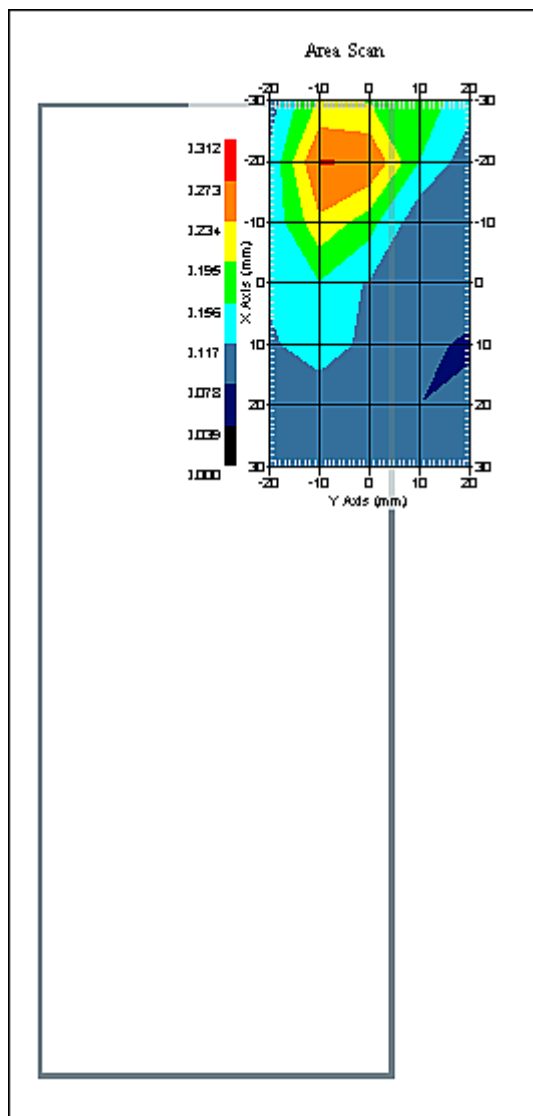

1 gram SAR value : 0.239 W/kg
 10 gram SAR value : 0.144 W/kg
 Area Scan Peak SAR : 0.276 W/kg
 Zoom Scan Peak SAR : 0.480 W/kg

SAR Test Report

By Operator : Jay
Measurement Date : 01-May-2008
Starting Time : 01-May-2008 10:29:46 AM
End Time : 01-May-2008 10:53:47 AM
Scanning Time : 1441 secs

Product Data

Device Name : LXE
Serial No. : MX8 Eng 1
Type : Other
Model : MX8
Frequency : 5800.00 MHz
Max. Transmit Pwr : 0.02 W
Drift Time : 0 min(s)
Length : 188 mm
Width : 70 mm
Depth : 40 mm
Antenna Type : Internal
Orientation : Touch
Power Drift-Start : 0.187 W/kg
Power Drift-Finish: 0.190 W/kg
Power Drift (%) : 1.677

Phantom Data

Name : APREL-Uni
Type : Uni-Phantom
Size (mm) : 280 x 280 x 200
Serial No. : System Default
Location : Center
Description : Uni-Phantom

Tissue Data

Type : BODY
Serial No. : 5800
Frequency : 5800.00 MHz
Last Calib. Date : 01-May-2008
Temperature : 20.00 °C
Ambient Temp. : 23.00 °C
Humidity : 50.00 RH%
Epsilon : 49.38 F/m
Sigma : 5.84 S/m
Density : 1000.00 kg/cu. m

Probe Data


Name : Probe AL-E3P1 - AL
Model : E-030
Type : E-Field Triangle
Serial No. : AL-E3P1
Last Calib. Date : 30-Apr-2007
Frequency : 5800.00 MHz
Duty Cycle Factor: 1
Conversion Factor: 12
Probe Sensitivity: 1.20 1.20 1.20 $\mu\text{V}/(\text{V/m})^2$
Compression Point: 95.00 mV
Offset : 1.06 mm

Measurement Data

Crest Factor : 1
 Scan Type : Complete
 Tissue Temp. : 20.00 °C
 Ambient Temp. : 23.00 °C
 Set-up Date : 01-May-2008
 Set-up Time : 7:38:29 AM
 Area Scan : 7x5x1 : Measurement x=10mm, y=10mm, z=2mm
 Zoom Scan : 7x7x10 : Measurement x=4mm, y=4mm, z=2.5mm


Other Data

DUT Position : Touch
 Separation : 0
 Channel : Low

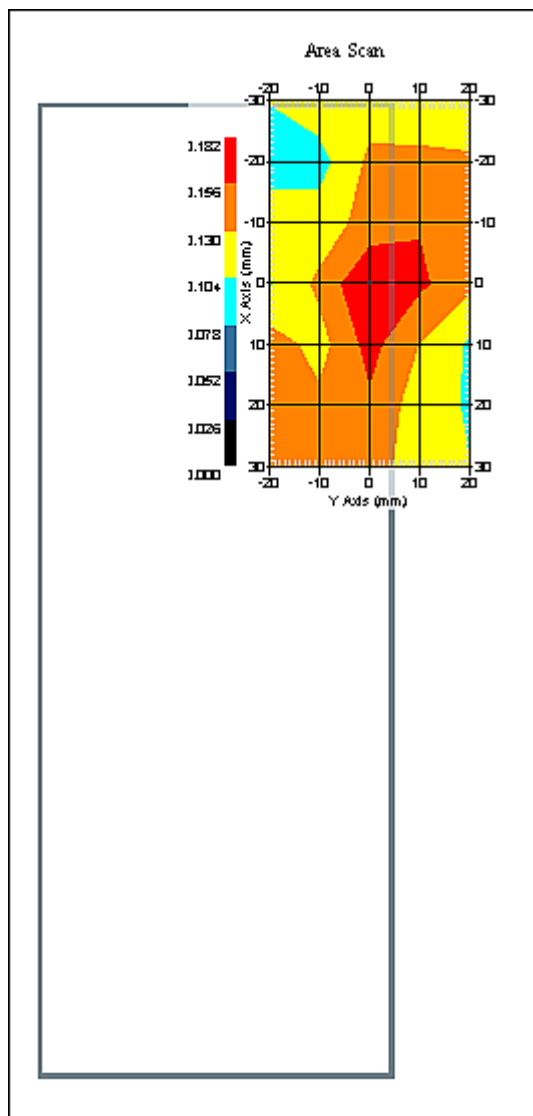

1 gram SAR value : 0.152 W/kg
 10 gram SAR value : 0.156 W/kg
 Area Scan Peak SAR : 0.181 W/kg
 Zoom Scan Peak SAR : 0.260 W/kg

SAR-Z Axis
at Hotspot x:-17.74 y:-2.12

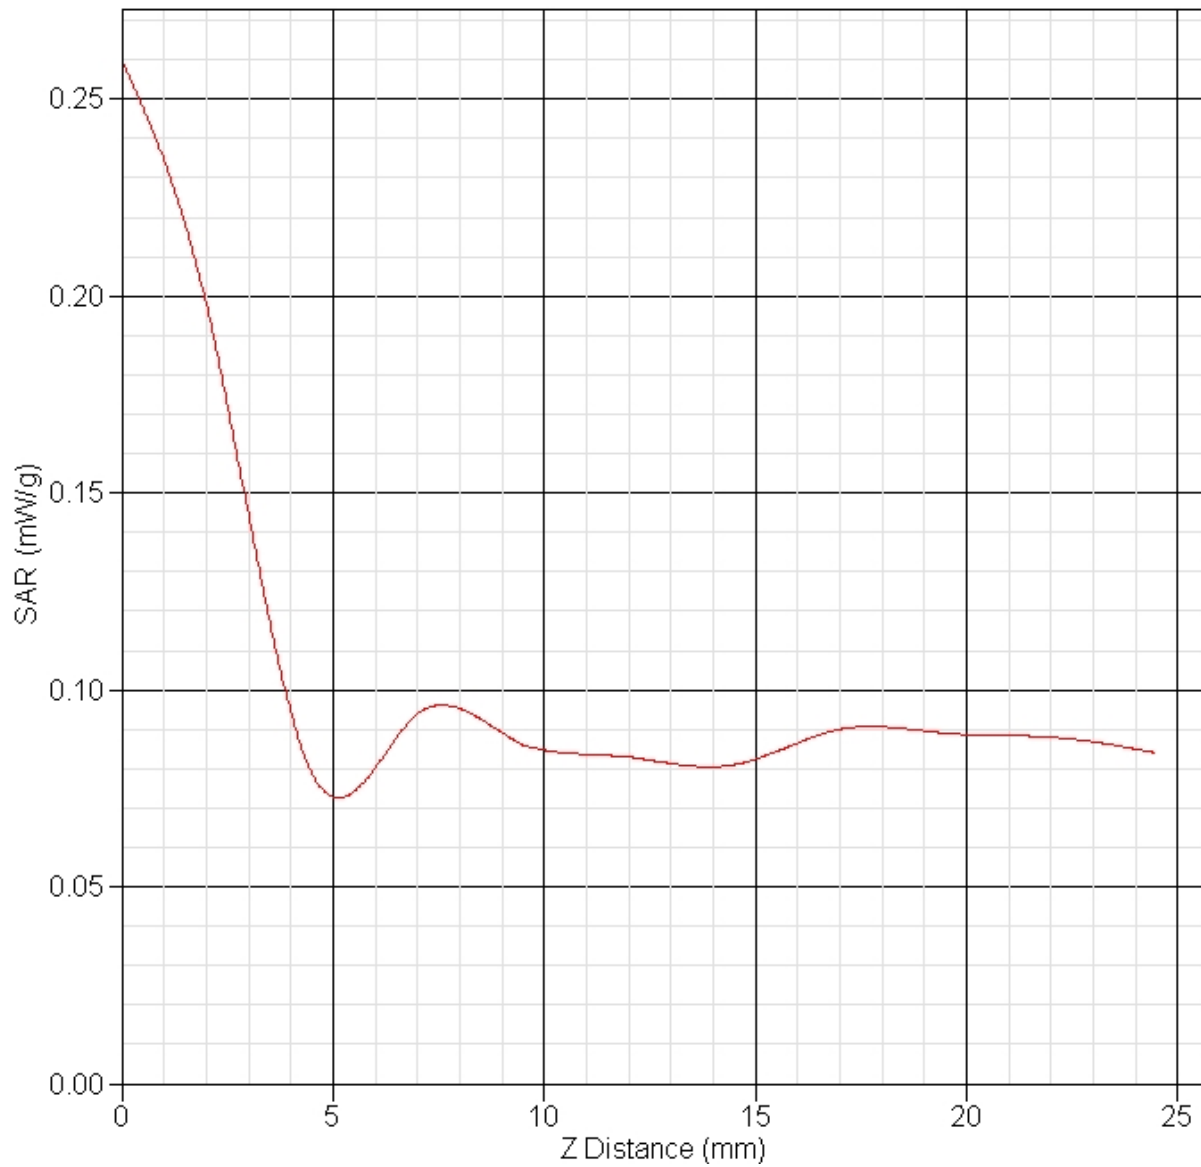

SAR Test Report

By Operator : Jay
Measurement Date : 01-May-2008
Starting Time : 01-May-2008 11:23:58 AM
End Time : 01-May-2008 11:47:53 AM
Scanning Time : 1435 secs

Product Data

Device Name : LXE
Serial No. : MX8 Eng 1
Type : Other
Model : MX8
Frequency : 5800.00 MHz
Max. Transmit Pwr : 0.02 W
Drift Time : 0 min(s)
Length : 188 mm
Width : 70 mm
Depth : 40 mm
Antenna Type : Internal
Orientation : Touch
Power Drift-Start : 0.134 W/kg
Power Drift-Finish: 0.135 W/kg
Power Drift (%) : 0.834

Phantom Data

Name : APREL-Uni
Type : Uni-Phantom
Size (mm) : 280 x 280 x 200
Serial No. : System Default
Location : Center
Description : Uni-Phantom

Tissue Data

Type : BODY
Serial No. : 5800
Frequency : 5800.00 MHz
Last Calib. Date : 01-May-2008
Temperature : 20.00 °C
Ambient Temp. : 23.00 °C
Humidity : 50.00 RH%
Epsilon : 49.38 F/m
Sigma : 5.84 S/m
Density : 1000.00 kg/cu. m

Probe Data


Name : Probe AL-E3P1 - AL
Model : E-030
Type : E-Field Triangle
Serial No. : AL-E3P1
Last Calib. Date : 30-Apr-2007
Frequency : 5800.00 MHz
Duty Cycle Factor: 1
Conversion Factor: 12
Probe Sensitivity: 1.20 1.20 1.20 $\mu\text{V}/(\text{V/m})^2$
Compression Point: 95.00 mV
Offset : 1.06 mm

Measurement Data

Crest Factor : 1
 Scan Type : Complete
 Tissue Temp. : 20.00 °C
 Ambient Temp. : 23.00 °C
 Set-up Date : 01-May-2008
 Set-up Time : 7:38:29 AM
 Area Scan : 7x5x1 : Measurement x=10mm, y=10mm, z=2mm
 Zoom Scan : 7x7x10 : Measurement x=4mm, y=4mm, z=2.5mm

Other Data

DUT Position : Touch
 Separation : 0
 Channel : High

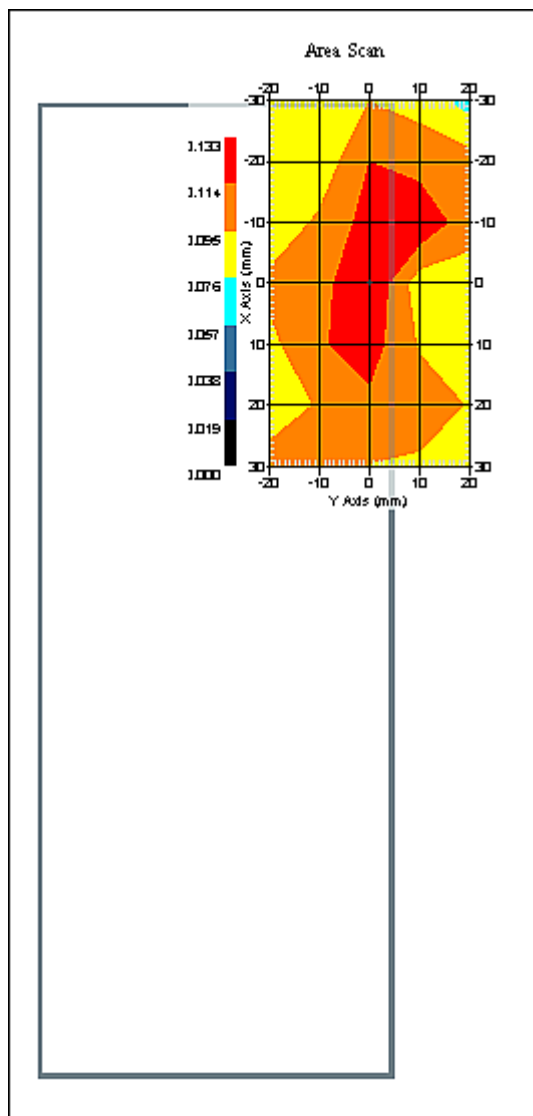

1 gram SAR value : 0.119 W/kg
 10 gram SAR value : 0.097 W/kg
 Area Scan Peak SAR : 0.133 W/kg
 Zoom Scan Peak SAR : 0.240 W/kg

SAR Test Report

By Operator : Jay
Measurement Date : 01-May-2008
Starting Time : 01-May-2008 11:54:43 AM
End Time : 01-May-2008 12:18:39 PM
Scanning Time : 1436 secs

Product Data

Device Name : LXE
Serial No. : MX8 Eng 1
Type : Other
Model : MX8
Frequency : 5800.00 MHz
Max. Transmit Pwr : 0.02 W
Drift Time : 0 min(s)
Length : 188 mm
Width : 70 mm
Depth : 40 mm
Antenna Type : Internal
Orientation : Touch
Power Drift-Start : 0.123 W/kg
Power Drift-Finish: 0.123 W/kg
Power Drift (%) : -0.376

Phantom Data

Name : APREL-Uni
Type : Uni-Phantom
Size (mm) : 280 x 280 x 200
Serial No. : System Default
Location : Center
Description : Uni-Phantom

Tissue Data

Type : BODY
Serial No. : 5800
Frequency : 5800.00 MHz
Last Calib. Date : 01-May-2008
Temperature : 20.00 °C
Ambient Temp. : 23.00 °C
Humidity : 50.00 RH%
Epsilon : 49.38 F/m
Sigma : 5.84 S/m
Density : 1000.00 kg/cu. m

Probe Data


Name : Probe AL-E3P1 - AL
Model : E-030
Type : E-Field Triangle
Serial No. : AL-E3P1
Last Calib. Date : 30-Apr-2007
Frequency : 5800.00 MHz
Duty Cycle Factor: 1
Conversion Factor: 12
Probe Sensitivity: 1.20 1.20 1.20 $\mu\text{V}/(\text{V/m})^2$
Compression Point: 95.00 mV
Offset : 1.06 mm

Measurement Data

Crest Factor : 1
 Scan Type : Complete
 Tissue Temp. : 20.00 °C
 Ambient Temp. : 23.00 °C
 Set-up Date : 01-May-2008
 Set-up Time : 7:38:29 AM
 Area Scan : 7x5x1 : Measurement x=10mm, y=10mm, z=2mm
 Zoom Scan : 7x7x10 : Measurement x=4mm, y=4mm, z=2.5mm

Other Data

DUT Position : Touch
 Separation : 0
 Channel : Low

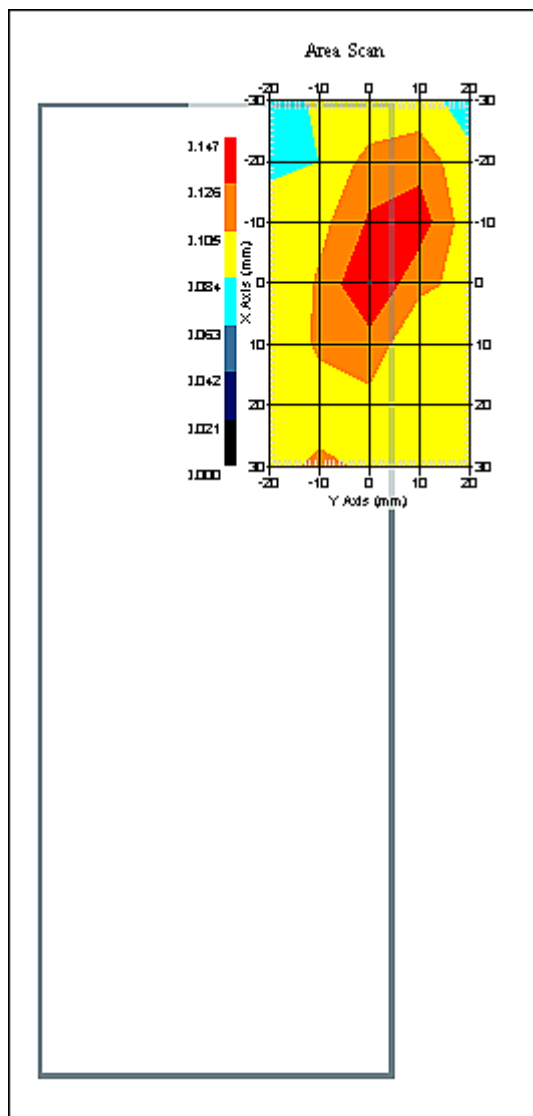

1 gram SAR value : 0.113 W/kg
 10 gram SAR value : 0.115 W/kg
 Area Scan Peak SAR : 0.147 W/kg
 Zoom Scan Peak SAR : 0.150 W/kg

SAR Test Report

By Operator : Jay
Measurement Date : 01-May-2008
Starting Time : 01-May-2008 01:23:47 PM
End Time : 01-May-2008 01:47:43 PM
Scanning Time : 1436 secs

Product Data

Device Name : LXE
Serial No. : MX8 Eng 1
Type : Other
Model : MX8
Frequency : 5800.00 MHz
Max. Transmit Pwr : 0.02 W
Drift Time : 0 min(s)
Length : 188 mm
Width : 70 mm
Depth : 40 mm
Antenna Type : Internal
Orientation : Touch
Power Drift-Start : 0.150 W/kg
Power Drift-Finish: 0.146 W/kg
Power Drift (%) : -2.676

Phantom Data

Name : APREL-Uni
Type : Uni-Phantom
Size (mm) : 280 x 280 x 200
Serial No. : System Default
Location : Center
Description : Uni-Phantom

Tissue Data

Type : BODY
Serial No. : 5800
Frequency : 5800.00 MHz
Last Calib. Date : 01-May-2008
Temperature : 20.00 °C
Ambient Temp. : 23.00 °C
Humidity : 50.00 RH%
Epsilon : 49.38 F/m
Sigma : 5.84 S/m
Density : 1000.00 kg/cu. m

Probe Data


Name : Probe AL-E3P1 - AL
Model : E-030
Type : E-Field Triangle
Serial No. : AL-E3P1
Last Calib. Date : 30-Apr-2007
Frequency : 5800.00 MHz
Duty Cycle Factor: 1
Conversion Factor: 12
Probe Sensitivity: 1.20 1.20 1.20 $\mu\text{V}/(\text{V/m})^2$
Compression Point: 95.00 mV
Offset : 1.06 mm

Measurement Data

Crest Factor : 1
 Scan Type : Complete
 Tissue Temp. : 20.00 °C
 Ambient Temp. : 23.00 °C
 Set-up Date : 01-May-2008
 Set-up Time : 7:38:29 AM
 Area Scan : 7x5x1 : Measurement x=10mm, y=10mm, z=2mm
 Zoom Scan : 7x7x10 : Measurement x=4mm, y=4mm, z=2.5mm

Other Data

DUT Position : Touch
 Separation : 0
 Channel : High

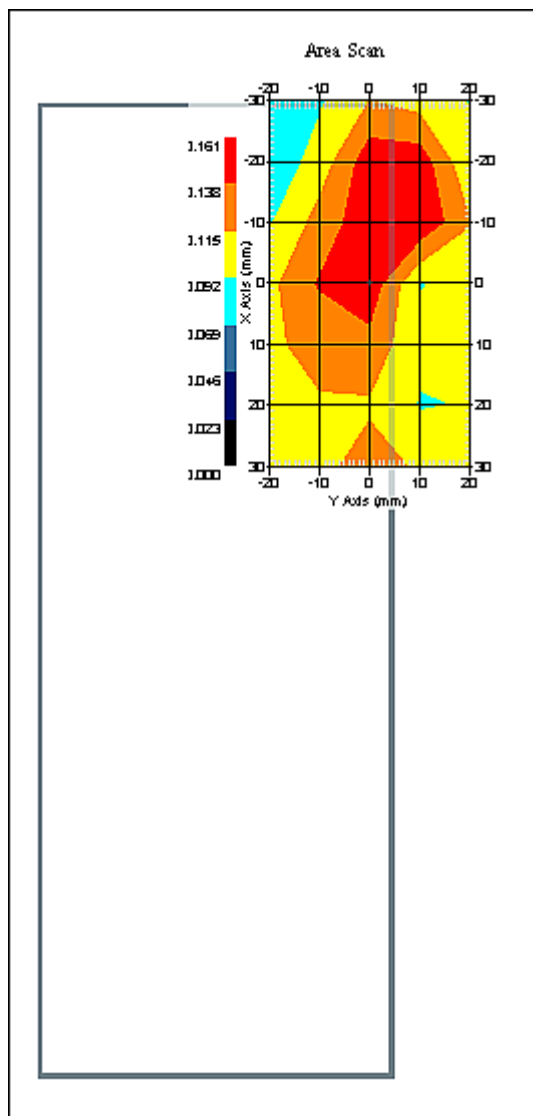

1 gram SAR value : 0.149 W/kg
 10 gram SAR value : 0.182 W/kg
 Area Scan Peak SAR : 0.158 W/kg
 Zoom Scan Peak SAR : 0.260 W/kg

SAR Test Report

By Operator : Jay
Measurement Date : 15-Dec-2008
Starting Time : 15-Dec-2008 04:29:26 PM
End Time : 15-Dec-2008 04:45:00 PM
Scanning Time : 934 secs

Product Data

Device Name : LXE
Serial No. : MX8 Eng 1
Type : Bluetooth
Model : MX8
Frequency : 2450.00 MHz
Max. Transmit Pwr : 0.005 W
Drift Time : 0 min(s)
Length : 188 mm
Width : 70 mm
Depth : 40 mm
Antenna Type : Internal
Orientation : Touch
Power Drift-Start : 0.111 W/kg
Power Drift-Finish: 0.111 W/kg
Power Drift (%) : 0.144

Phantom Data

Name : APREL-Uni
Type : Uni-Phantom
Size (mm) : 280 x 280 x 200
Serial No. : System Default
Location : Center
Description : Uni-Phantom

Tissue Data

Type : BODY
Serial No. : 2450
Frequency : 2450.00 MHz
Last Calib. Date : 15-Dec-2008
Temperature : 20.00 °C
Ambient Temp. : 23.00 °C
Humidity : 41.00 RH%
Epsilon : 54.59 F/m
Sigma : 1.95 S/m
Density : 1000.00 kg/cu. m

Probe Data


Name : Probe 215 - RFEL
Model : E020
Type : E-Field Triangle
Serial No. : 215
Last Calib. Date : 03-Nov-2008
Frequency : 2450.00 MHz
Duty Cycle Factor: 1
Conversion Factor: 4.5
Probe Sensitivity: 1.20 1.20 1.20 $\mu\text{V}/(\text{V/m})^2$
Compression Point: 95.00 mV
Offset : 1.56 mm

Measurement Data

Crest Factor : 1
 Scan Type : Complete
 Tissue Temp. : 20.00 °C
 Ambient Temp. : 23.00 °C
 Set-up Date : 15-Dec-2008
 Set-up Time : 7:25:03 AM
 Area Scan : 5x8x1 : Measurement x=10mm, y=10mm, z=4mm
 Zoom Scan : 5x5x8 : Measurement x=8mm, y=8mm, z=4mm


Other Data

DUT Position : Touch
 Separation : 0
 Channel : Mid

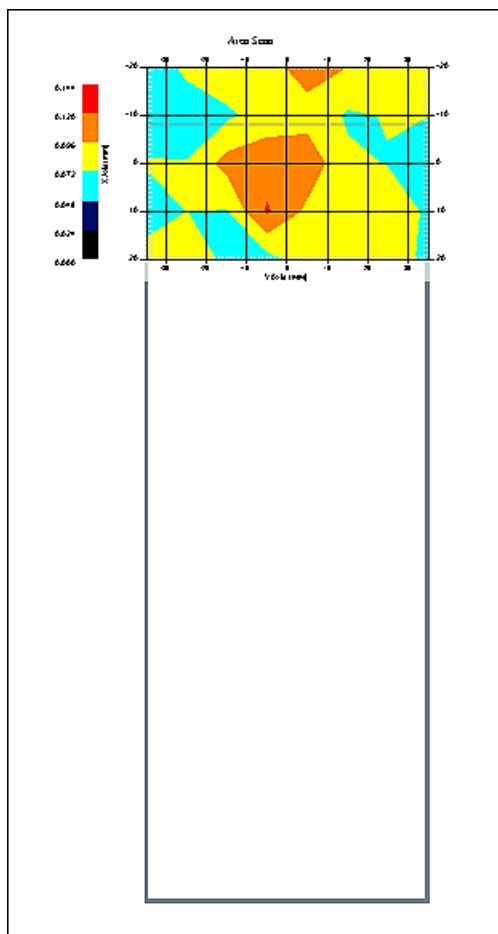


1 gram SAR value : 0.082 W/kg
 10 gram SAR value : 0.043 W/kg
 Area Scan Peak SAR : 0.102 W/kg
 Zoom Scan Peak SAR : 0.120 W/kg

Appendix C – SAR Test Setup Photos

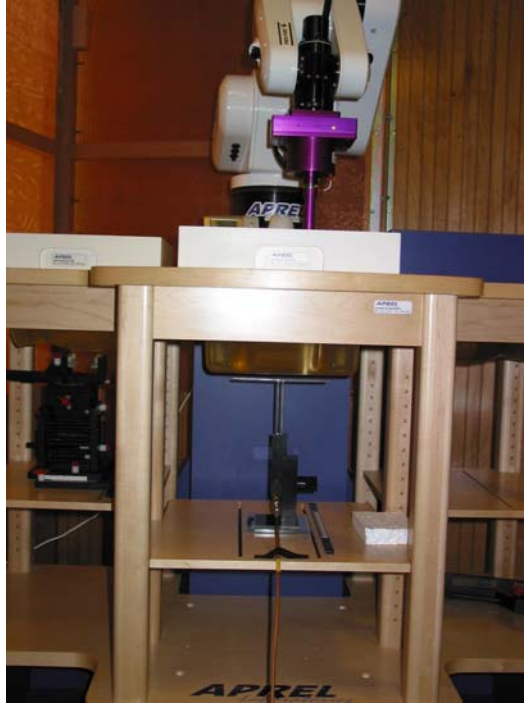

System Body Configuration

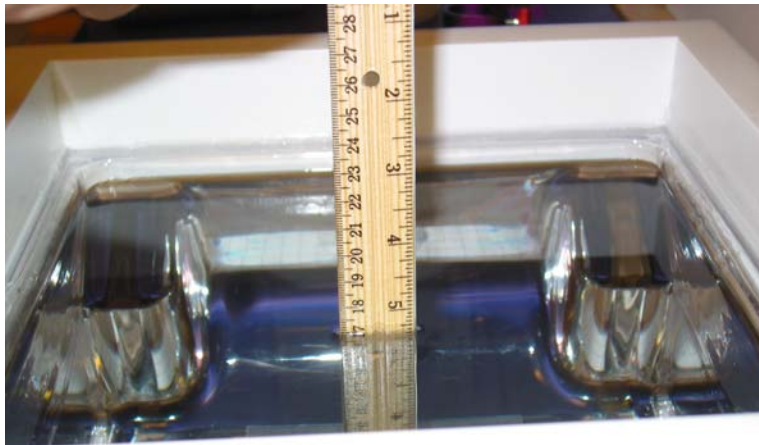


Body Tissue Depth




Back Of Unit Configuration




Front Of Device

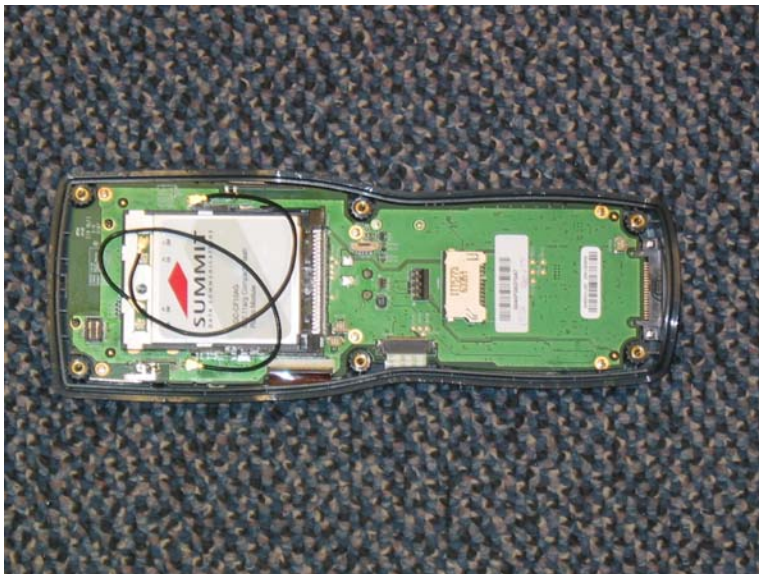


Back of Device with Cover Removed No Bluetooth

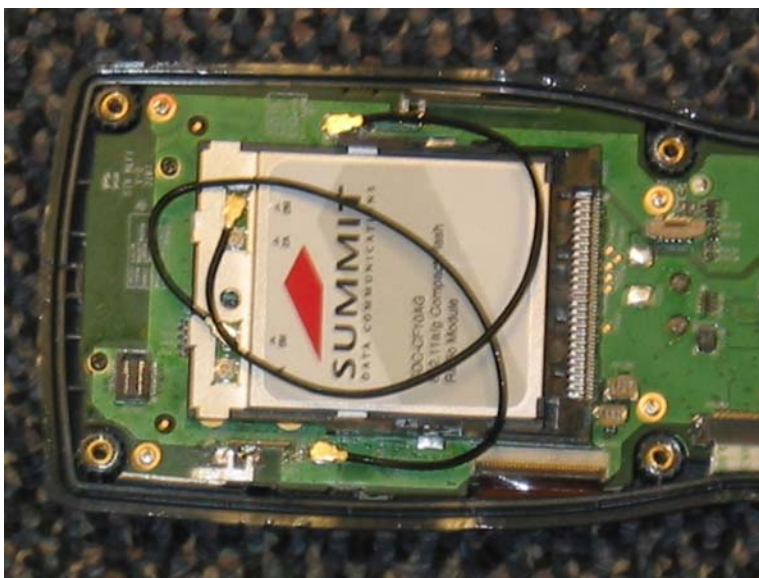

RF Module Installed

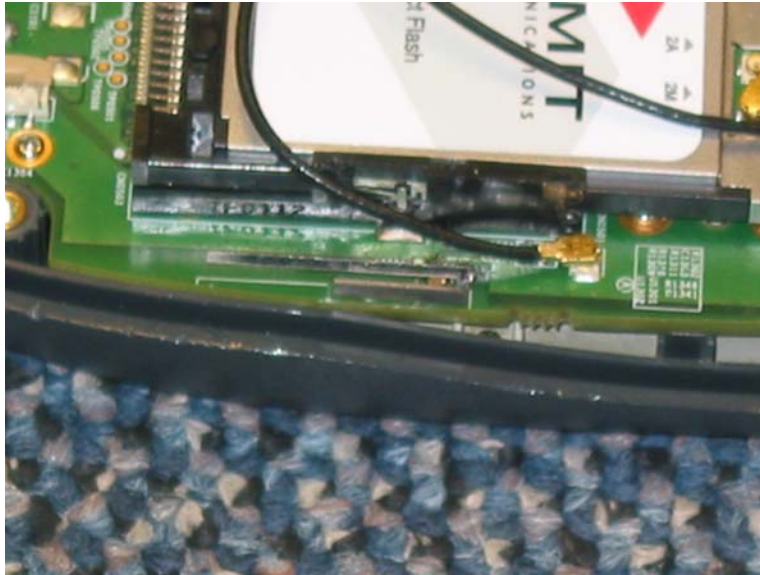

Right Antenna

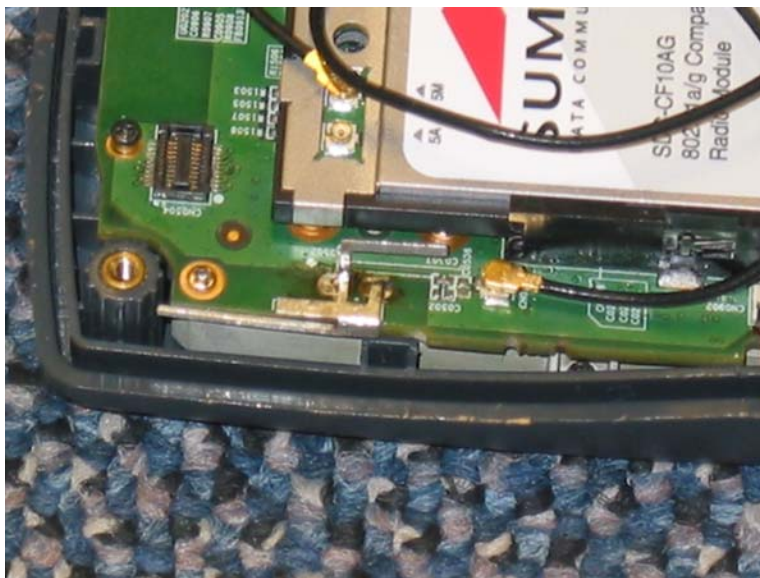

Left Antenna



Front of Battery



Back of Battery



Back of Device with Top Cover Removed With Bluetooth



Bluetooth Module Location

Appendix D – Probe Calibration Data Sheets

NCL CALIBRATION LABORATORIES

Calibration File No.: CP-844

Client.: RFEL

CERTIFICATE OF CALIBRATION

It is certified that the equipment identified below has been calibrated in the
NCL CALIBRATION LABORATORIES by qualified personnel following recognized
procedures and using transfer standards traceable to NRC/NIST.

Equipment: Miniature Isotropic RF Probe 2450 MHz

BODY Calibration

Manufacturer: APREL Laboratories

Model No.: E-020

Serial No.: 217

Calibration Procedure: SSI/DRB-TP-D01-032-E020-V2

Project No: RFEB-ALS-E-020-5318

Calibrated: 3rd December 2007
Released on: 3rd December 2007

This Calibration Certificate is Incomplete Unless Accompanied with the Calibration Results Summary
This calibration has been conducted in line with the SCC ISO-IEC 17025 Scope of Accreditation
Accredited Laboratory Number 48

Released By: _____

NCL CALIBRATION LABORATORIES

51 SPECTRUM WAY
NEPEAN, ONTARIO
CANADA K2R 1E6

Division of APREL Lab.
TEL: (613) 820-4988
FAX: (613) 820-4161

Introduction

This Calibration Report reproduces the results of the calibration performed in line with the SSI/DRB-TP-D01-032-E020-V2 E-Field Probe Calibration Procedure. The results contained within this report are for APREL E-Field Probe E-020 217.

References

SSI/DRB-TP-D01-032-E020-V2 E-Field Probe Calibration Procedure

IEEE 1528 "Recommended Practice for Determining the Peak Spatial-Average Specific Absorption Rate (SAR) in the Human Body Due to Wireless Communications Devices: Experimental Techniques"

SSI-TP-011 Tissue Calibration Procedure

IEC 62209 "Human exposure to radio frequency fields from hand-held and body-mounted wireless communication devices – Human models, instrumentation, and procedures –Part 1 & 2: Procedure to determine the Specific Absorption Rate (SAR) for hand-held devices used in close proximity of the ear (frequency range of 300 MHz to 3 GHz)"

IEEE 1309 Draft Standard for Calibration of Electromagnetic Field Sensors and Probes, Excluding Antennas, from 9kHz to 40GHz

Conditions


Probe 217 was a re-calibration.

Ambient Temperature of the Laboratory: 22 °C +/- 0.5°C

Temperature of the Tissue: 21 °C +/- 0.5°C

We the undersigned attest that to the best of our knowledge the calibration of this probe has been accurately conducted and that all information contained within this report has been reviewed for accuracy.



Stuart Nicol

Jesse Hones

Calibration Results Summary

Probe Type:	E-Field Probe E-020
Serial Number:	217
Frequency:	2450 MHz
Sensor Offset:	1.56 mm
Sensor Length:	2.5 mm
Tip Enclosure:	Ertalyte*
Tip Diameter:	<5 mm
Tip Length:	60 mm
Total Length:	290 mm

*Resistive to recommended tissue recipes per IEEE-1528

Sensitivity in Air

Channel X:	$1.2 \mu\text{V}/(\text{V}/\text{m})^2$
Channel Y:	$1.2 \mu\text{V}/(\text{V}/\text{m})^2$
Channel Z:	$1.2 \mu\text{V}/(\text{V}/\text{m})^2$
Diode Compression Point:	95 mV

Sensitivity in Body Tissue Measured

Frequency: 2450 MHz

Epsilon: 53.8 (+/-5%) **Sigma:** 1.99 S/m (+/-5%)

ConvF

Channel X: 3.61

Channel Y: 3.61

Channel Z: 3.61

Tissue sensitivity values were calculated using the load impedance of the APREL Laboratories Daq-Paq.


Boundary Effect:

Uncertainty resulting from the boundary effect is less than 2% for the distance between the tip of the probe and the tissue boundary, when less than 2.44mm.



Spatial Resolution:

The measured probe tip diameter is 5 mm (+/- 0.01 mm) and therefore meets the requirements of SSI/DRB-TP-D01-032 for spatial resolution.

Receiving Pattern 2450 MHz (Air)

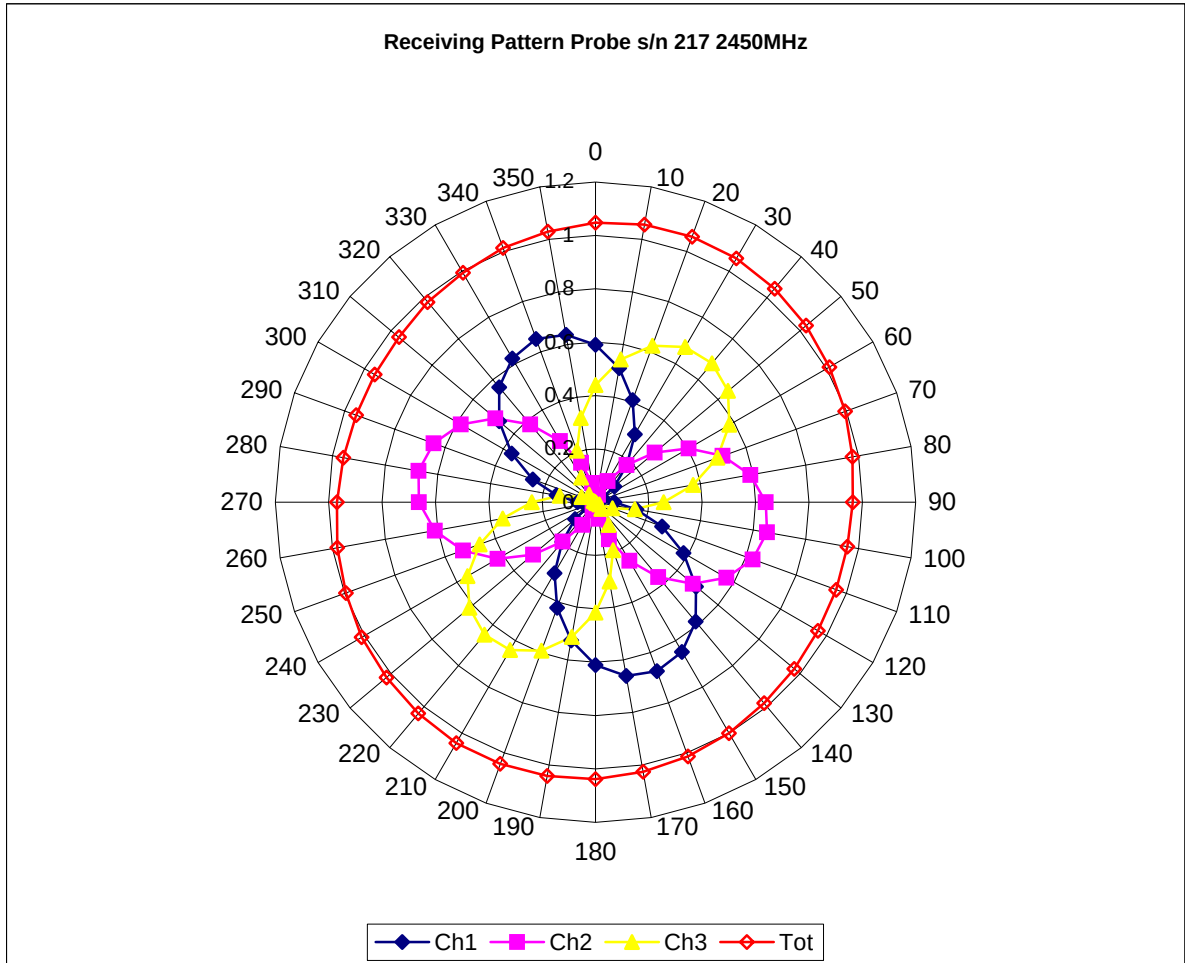


Isotropy Error 2450 MHz (Air)

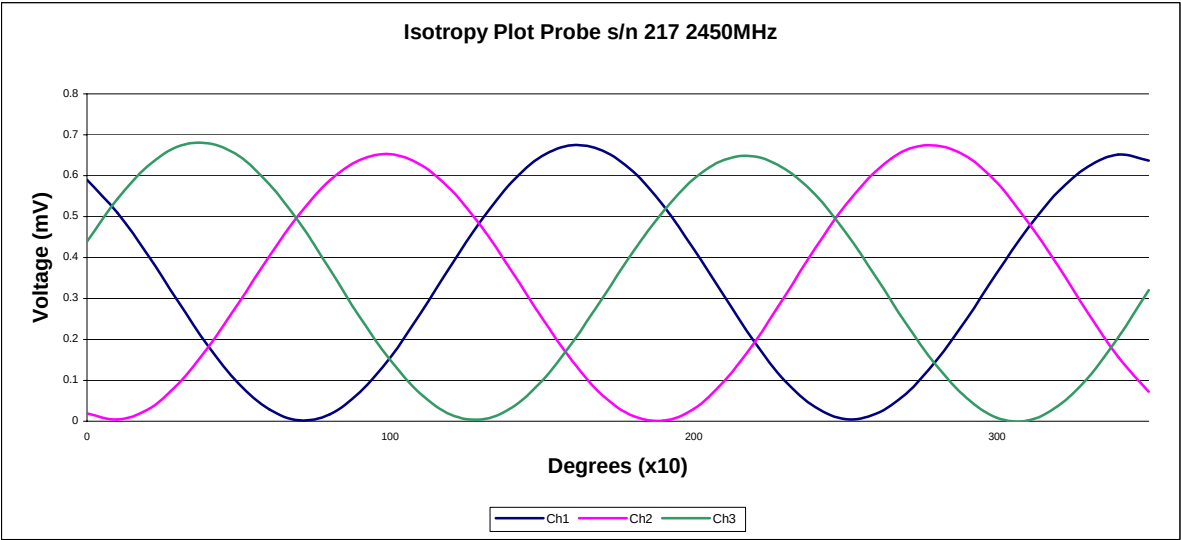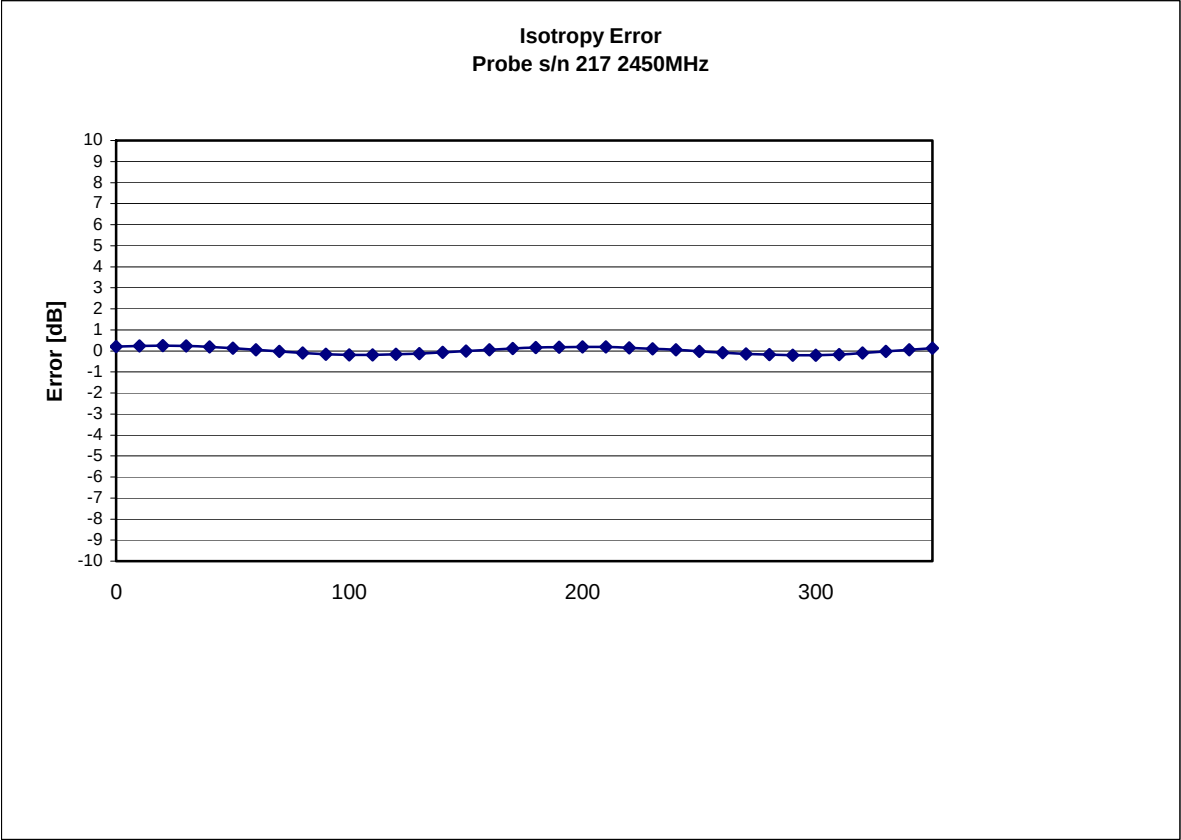


Isotropy Tissue:

0.10 dB

Dynamic Range

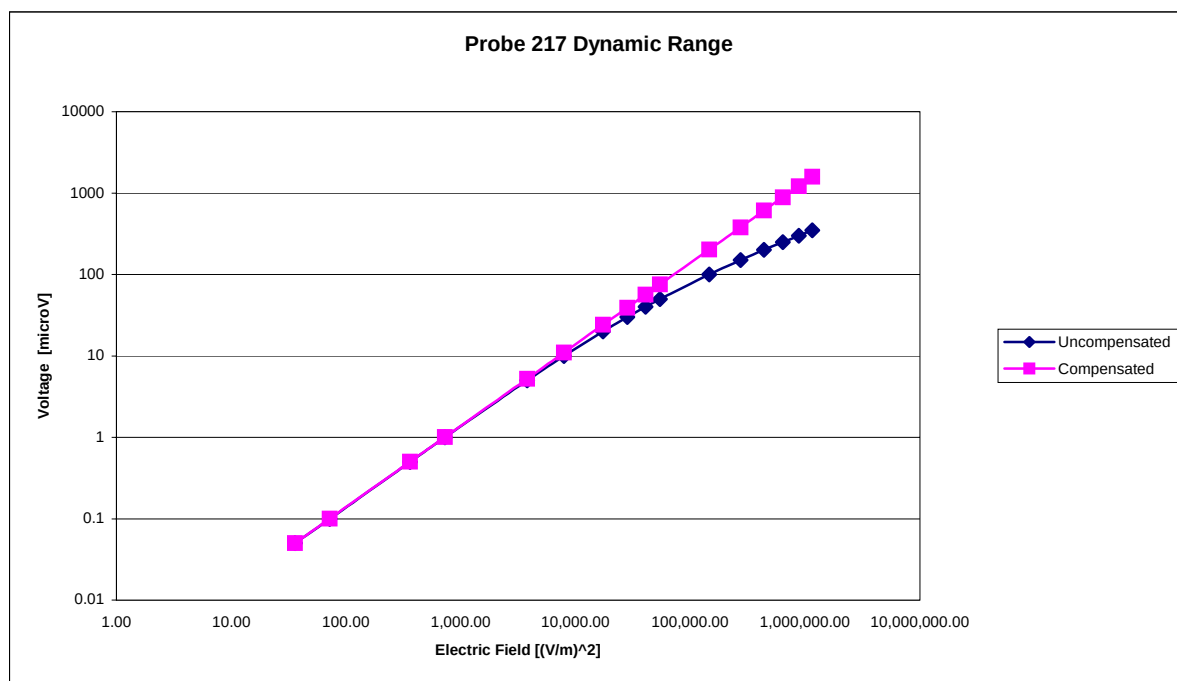

Video Bandwidth

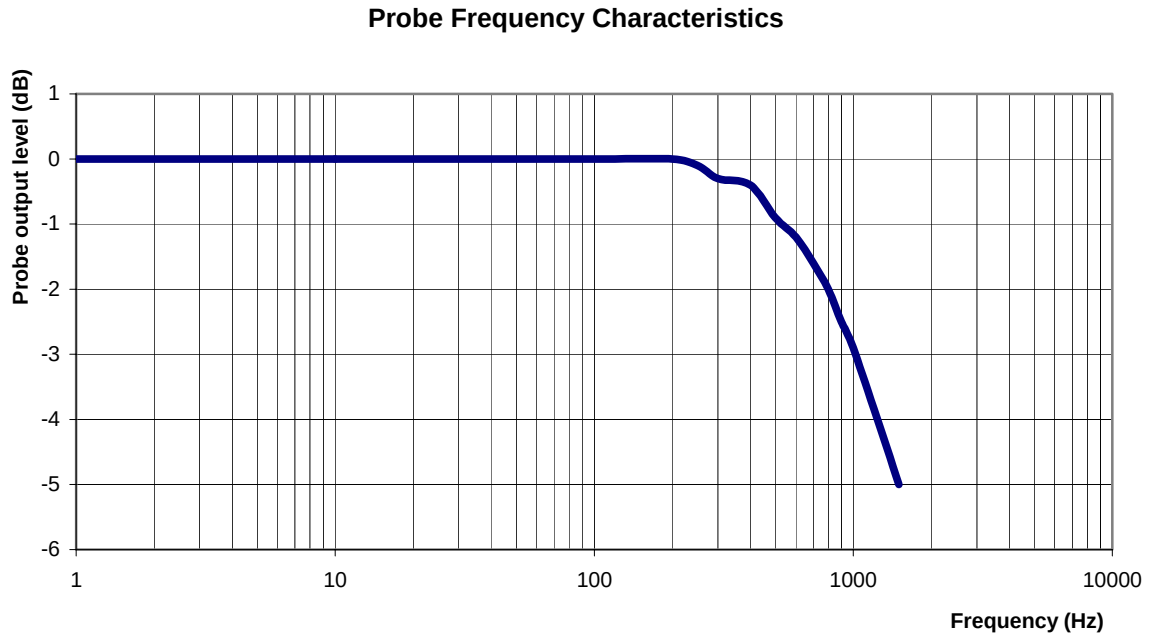

Video Bandwidth at 500 Hz	1 dB
Video Bandwidth at 1.02 KHz:	3 dB

Conversion Factor Uncertainty Assessment

Sensitivity in Body Tissue

Frequency: 2450 MHz

Epsilon: 53.8 (+/-5%)

Sigma: 1.99 S/m (+/-5%)

ConvF

Channel X: 3.61 7%(K=2)

Channel Y: 3.61 7%(K=2)

Channel Z: 3.61 7%(K=2)

To minimize the uncertainty calculation all tissue sensitivity values were calculated using a load impedance of 5 M Ω .

Boundary Effect:

For a distance of 2.5mm the evaluated uncertainty (increase in the probe sensitivity) is less than 2%.

Test Equipment

The test equipment used during Probe Calibration, manufacturer, model number and, current calibration status are listed and located on the main APREL server R:\NCL\Calibration Equipment\Instrument List May 2007.

NCL CALIBRATION LABORATORIES

Calibration File No.: CP-935

Client.: RFEL

CERTIFICATE OF CALIBRATION

It is certified that the equipment identified below has been calibrated in the
NCL CALIBRATION LABORATORIES by qualified personnel following recognized
procedures and using transfer standards traceable to NRC/NIST.

Equipment: Miniature Isotropic RF Probe 2450 MHz

BODY Calibration

Manufacturer: APREL Laboratories

Model No.: E-020

Serial No.: 215

Calibration Procedure: SSI/DRB-TP-D01-032-E020-V2

Project No: RFEL-00150-CAL-5367

Calibrated: 3rd November 2008
Released on: 3rd November 2008

This Calibration Certificate is Incomplete Unless Accompanied with the Calibration Results Summary
This calibration has been conducted in line with the SCC ISO-IEC 17025 Scope of Accreditation
Accredited Laboratory Number 48

Released By: _____

NCL CALIBRATION LABORATORIES

51 SPECTRUM WAY
NEPEAN, ONTARIO
CANADA K2R 1E6

Division of APREL Lab.
TEL: (613) 820-4988
FAX: (613) 820-4161

Introduction

This Calibration Report reproduces the results of the calibration performed in line with the SSI/DRB-TP-D01-032-E020-V2 E-Field Probe Calibration Procedure. The results contained within this report are for APREL E-Field Probe E-020 215.

References

SSI/DRB-TP-D01-032-E020-V2 E-Field Probe Calibration Procedure

IEEE 1528 "Recommended Practice for Determining the Peak Spatial-Average Specific Absorption Rate (SAR) in the Human Body Due to Wireless Communications Devices: Experimental Techniques"

IEEE 1309 "IEEE Standard for Calibration of Electromagnetic Field Sensors and Probes, Excluding Antennas, from 9 KHz to 40 GHz" 2005

SSI-TP-011 Tissue Calibration Procedure

IEC 62209 "Human exposure to radio frequency fields from handheld and body-mounted wireless communication devices –Human models, instrumentation and procedures Part 1 & 2: Procedure to determine the Specific Absorption Rate (SAR) for handheld devices used in close proximity of the ear (frequency range of 200MHz to 3GHz)"

Conditions


Probe 215 was a re-calibration.

Ambient Temperature of the Laboratory: 22 °C +/- 0.5°C

Temperature of the Tissue: 21 °C +/- 0.5°C

We the undersigned attest that to the best of our knowledge the calibration of this probe has been accurately conducted and that all information contained within this report has been reviewed for accuracy.



Stuart Nicol

Jesse Hones

Calibration Results Summary

Probe Type:	E-Field Probe E-020
Serial Number:	215
Frequency:	2450 MHz
Sensor Offset:	1.56 mm
Sensor Length:	2.5 mm
Tip Enclosure:	Ertalyte*
Tip Diameter:	<5 mm
Tip Length:	60 mm
Total Length:	290 mm

*Resistive to recommended tissue recipes per IEEE-1528

Sensitivity in Air

Channel X:	$1.2 \mu\text{V}/(\text{V}/\text{m})^2$
Channel Y:	$1.2 \mu\text{V}/(\text{V}/\text{m})^2$
Channel Z:	$1.2 \mu\text{V}/(\text{V}/\text{m})^2$
Diode Compression Point:	95 mV

Sensitivity in Body Tissue Measured

Frequency: 2450 MHz

Epsilon: 53.8 (+/-5%) **Sigma:** 1.99 S/m (+/-5%)

ConvF

Channel X: 4.5

Channel Y: 4.5

Channel Z: 4.5

Tissue sensitivity values were calculated using the load impedance of the APREL Laboratories Daq-Paq.


Boundary Effect:

Uncertainty resulting from the boundary effect is less than 2% for the distance between the tip of the probe and the tissue boundary, when less than 2.44mm.



Spatial Resolution:

The measured probe tip diameter is 5 mm (+/- 0.01 mm) and therefore meets the requirements of SSI/DRB-TP-D01-032 for spatial resolution.

Receiving Pattern 2450 MHz (Air)

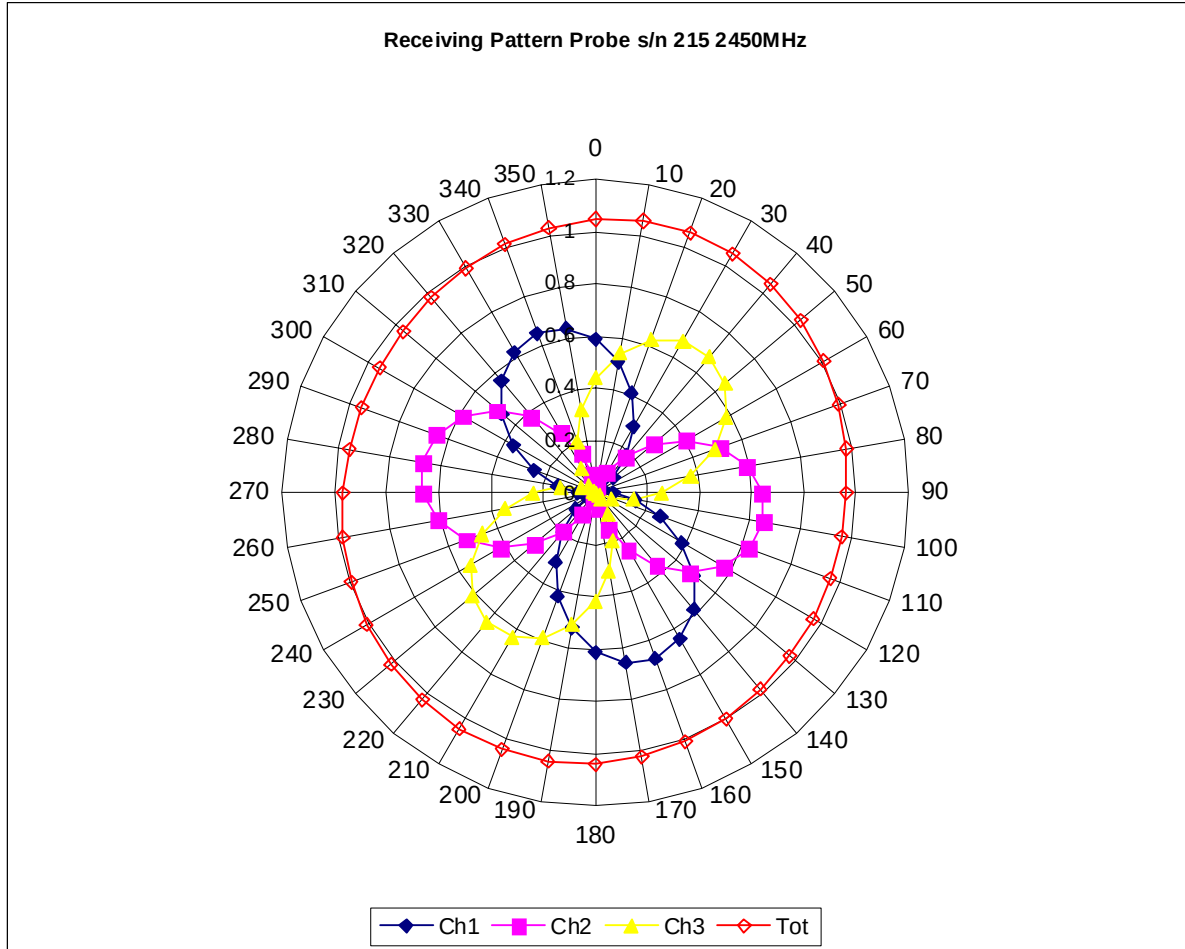


Isotropy Error 2450 MHz (Air)

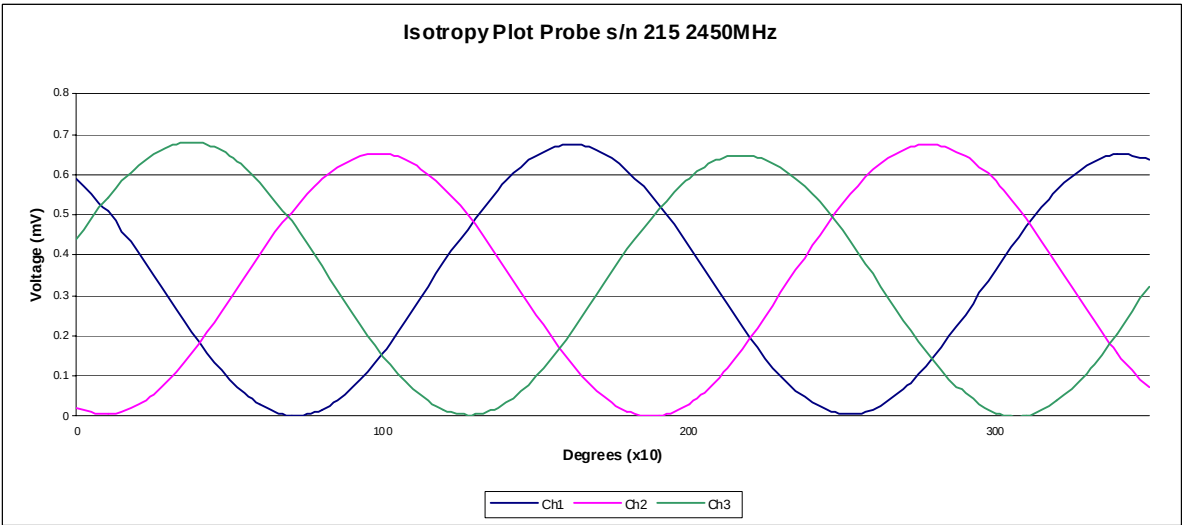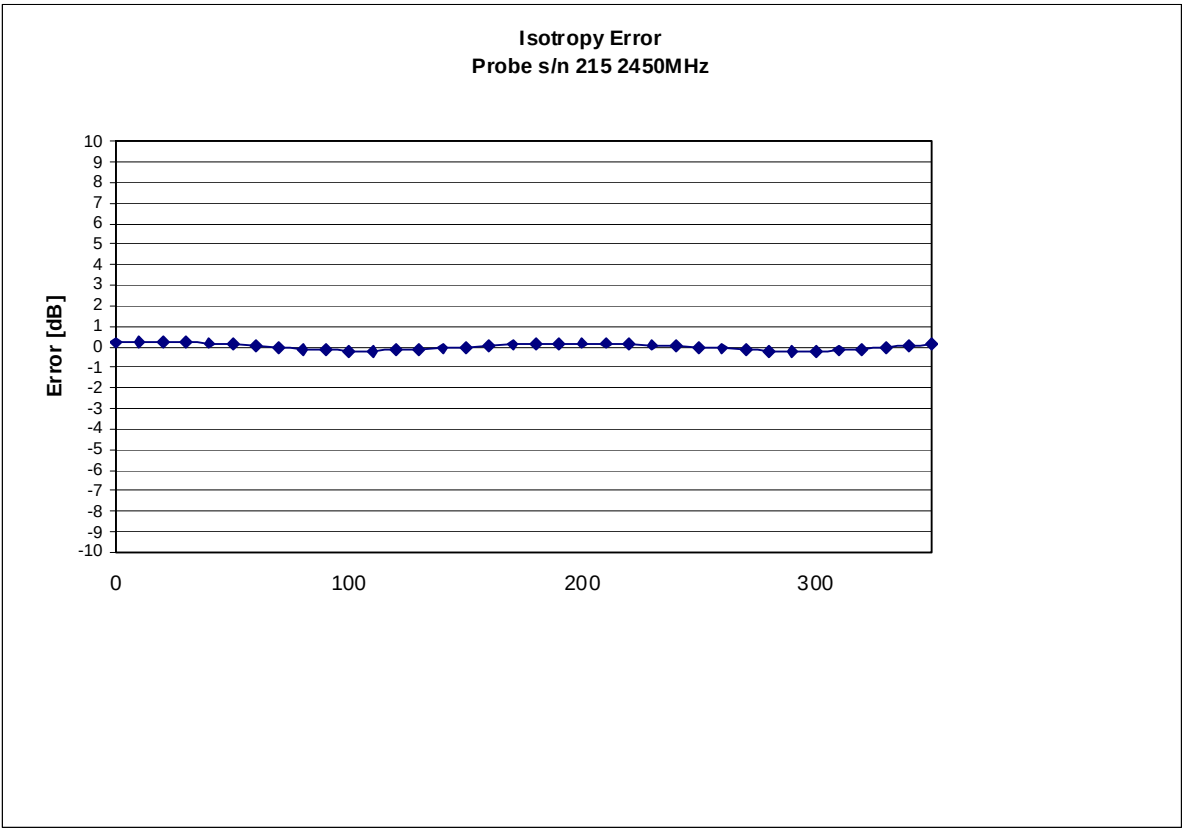


Isotropy Tissue:

0.10 dB

Dynamic Range

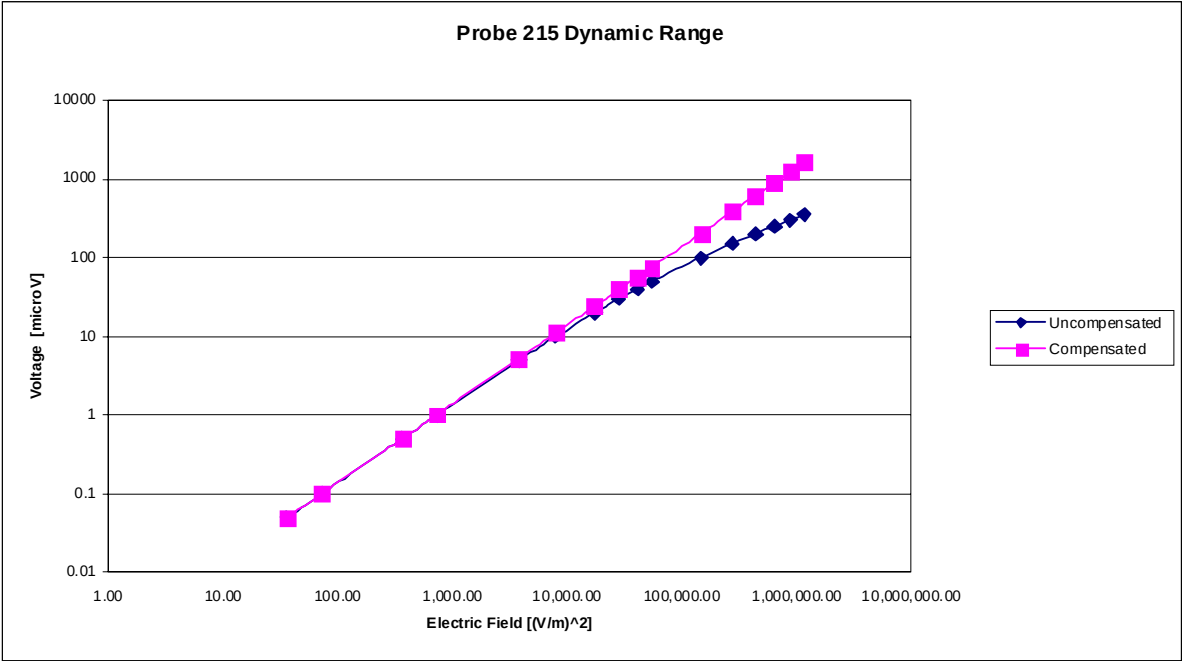

Video Bandwidth

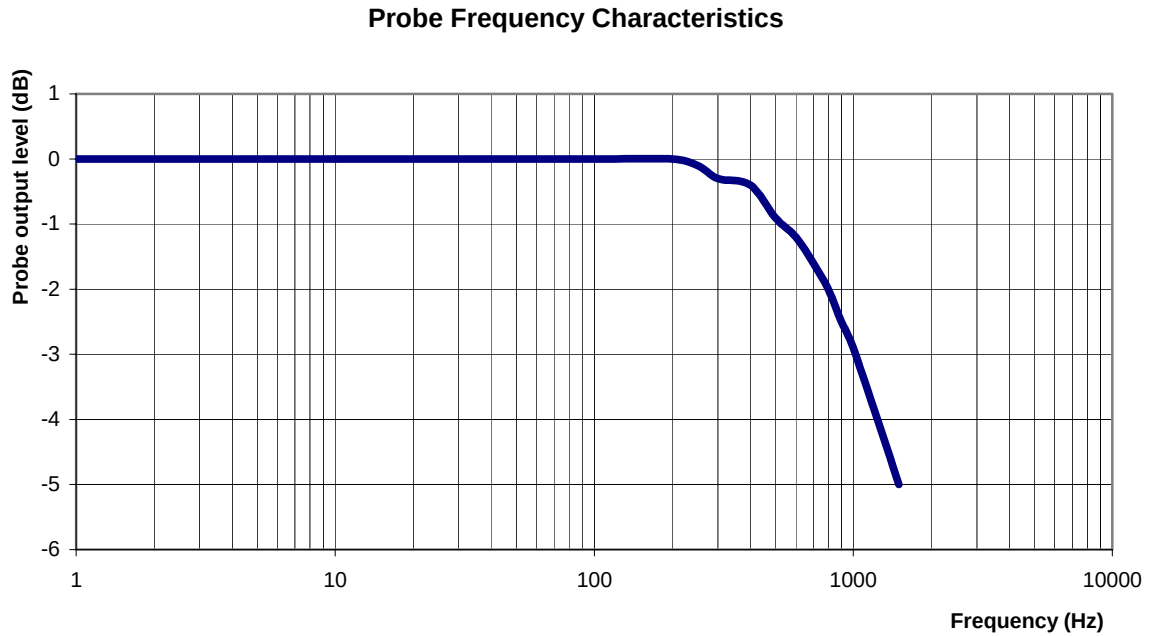

Video Bandwidth at 500 Hz	1 dB
Video Bandwidth at 1.02 KHz:	3 dB

Conversion Factor Uncertainty Assessment

Sensitivity in Body Tissue

Frequency: 2450 MHz

Epsilon: 53.8 (+/-5%)

Sigma: 1.99 S/m (+/-5%)

ConvF

Channel X: 4.5 7%(K=2)

Channel Y: 4.5 7%(K=2)

Channel Z: 4.5 7%(K=2)

To minimize the uncertainty calculation all tissue sensitivity values were calculated using a load impedance of 5 M Ω .

Boundary Effect:

For a distance of 2.5mm the evaluated uncertainty (increase in the probe sensitivity) is less than 2%.

Test Equipment

The test equipment used during Probe Calibration, manufacturer, model number and, current calibration status are listed and located on the main APREL server R:\NCL\Calibration Equipment\Instrument List May 2008.

NCL CALIBRATION LABORATORIES

Calibration File No.: CP-752

Client.: APREL

CERTIFICATE OF CALIBRATION

It is certified that the equipment identified below has been calibrated in the
NCL CALIBRATION LABORATORIES by qualified personnel following recognized
procedures and using transfer standards traceable to NRC/NIST.

Equipment: Miniature Isotropic RF Probe 5200 MHz

Manufacturer: APREL Laboratories

Model No.: E-030

Serial No.: AL-E3P1

Calibration in Body Tissue

Calibration Procedure: SSI/DRB-TP-D01-032-E020-V2


Project No: APLB-5200-PC-5264

Calibrated: 29th April 2007

Released on: 30th April 2007

This Calibration Certificate is Incomplete Unless Accompanied with the Calibration Results Summary

Released By: _____

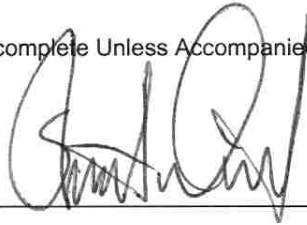

NCL CALIBRATION LABORATORIES

17 Bentley Avenue
NEPEAN, ONTARIO
CANADA K2E 6T7

Division of APREL Lab.
TEL: (613) 820-4988
FAX: (613) 820-4161

Introduction

This Calibration Report reproduces the results of the calibration performed in line with the SSI/DRB-TP-D01-032-E020-V2 E-Field Probe Calibration Procedure. The results contained within this report are for APREL E-Field Probe E-030 AL-E3P1.

References

SSI/DRB-TP-D01-032-E020-V2 E-Field Probe Calibration Procedure
IEEE 1528 "Recommended Practice for Determining the Peak Spatial-Average Specific Absorption Rate (SAR) in the Human Body Due to Wireless Communications Devices: Experimental Techniques"
SSI-TP-011 Tissue Calibration Procedure


Conditions

Probe AL-E3P1 was a new probe taken from stock prior to calibration.


Ambient Temperature of the Laboratory: 22 °C +/- 0.5°C

Temperature of the Tissue: 21 °C +/- 0.5°C

We the undersigned attest that to the best of our knowledge the calibration of this probe has been accurately conducted and that all information contained within this report has been reviewed for accuracy.



Stuart Nicol



Jesse Hones

Calibration Results Summary

Probe Type:	E-Field Probe E-030
Serial Number:	AL-E3P1
Frequency:	5200 MHz
Sensor Offset:	0.56 mm
Sensor Length:	2.5 mm
Tip Enclosure:	Ertalyte*
Tip Diameter:	<3 mm
Tip Length:	60 mm
Total Length:	290 mm

*Resistive to recommended tissue recipes per IEEE-1528

Sensitivity in Air

Channel X:	$1.2 \mu\text{V}/(\text{V}/\text{m})^2$
Channel Y:	$1.2 \mu\text{V}/(\text{V}/\text{m})^2$
Channel Z:	$1.2 \mu\text{V}/(\text{V}/\text{m})^2$
Diode Compression Point:	95 mV

Sensitivity in FCC Body Tissue

Frequency: 5200 MHz

Epsilon: 48.9 (+/-10%) **Sigma:** 5.35 S/m (+/-10%)

ConvF

Channel X: 13

Channel Y: 13

Channel Z: 13

Tissue sensitivity values were calculated using the load impedance of the APREL Laboratories Daq-Paq.


Boundary Effect:

Uncertainty resulting from the boundary effect is less than 2% for the distance between the tip of the probe and the tissue boundary, when less than 0.5mm.



Spatial Resolution:

The measured probe tip diameter is less than 3 mm (+/- 0.01 mm) and therefore meets the requirements of SSI/DRB-TP-D01-032 for spatial resolution.

Receiving Pattern 5200 MHz (Air)

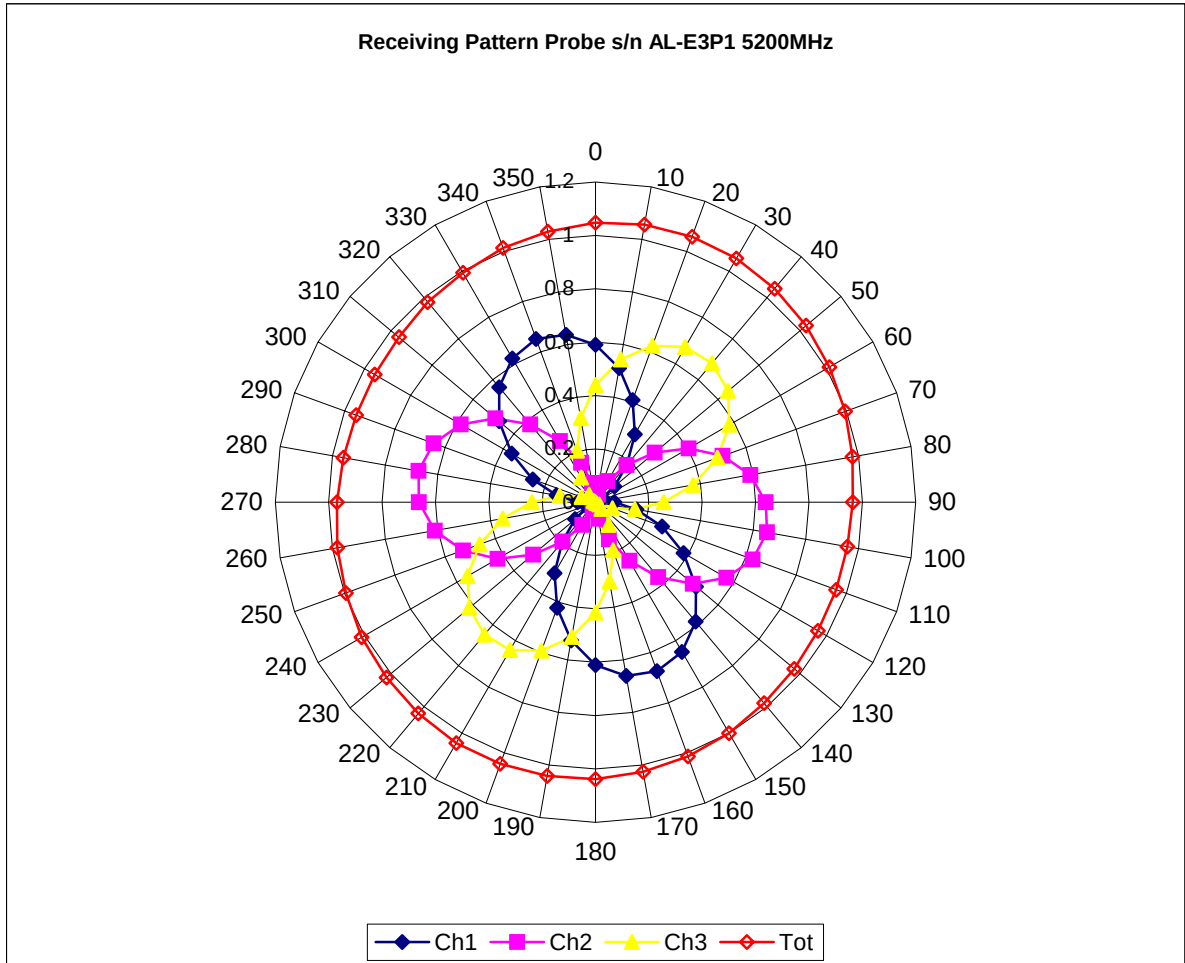


Isotropy Error 5200 MHz (Air)

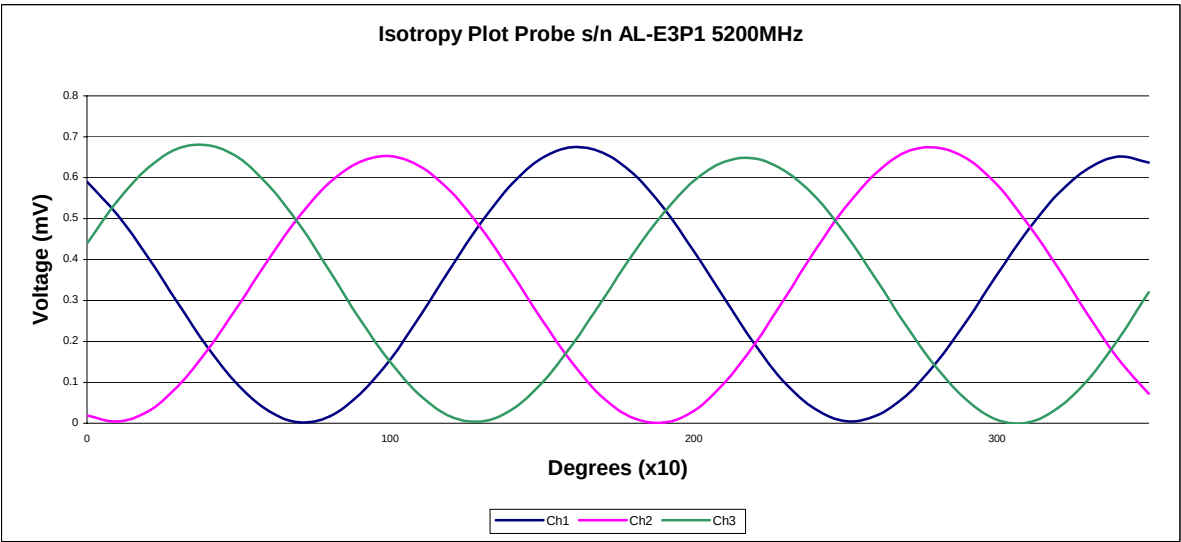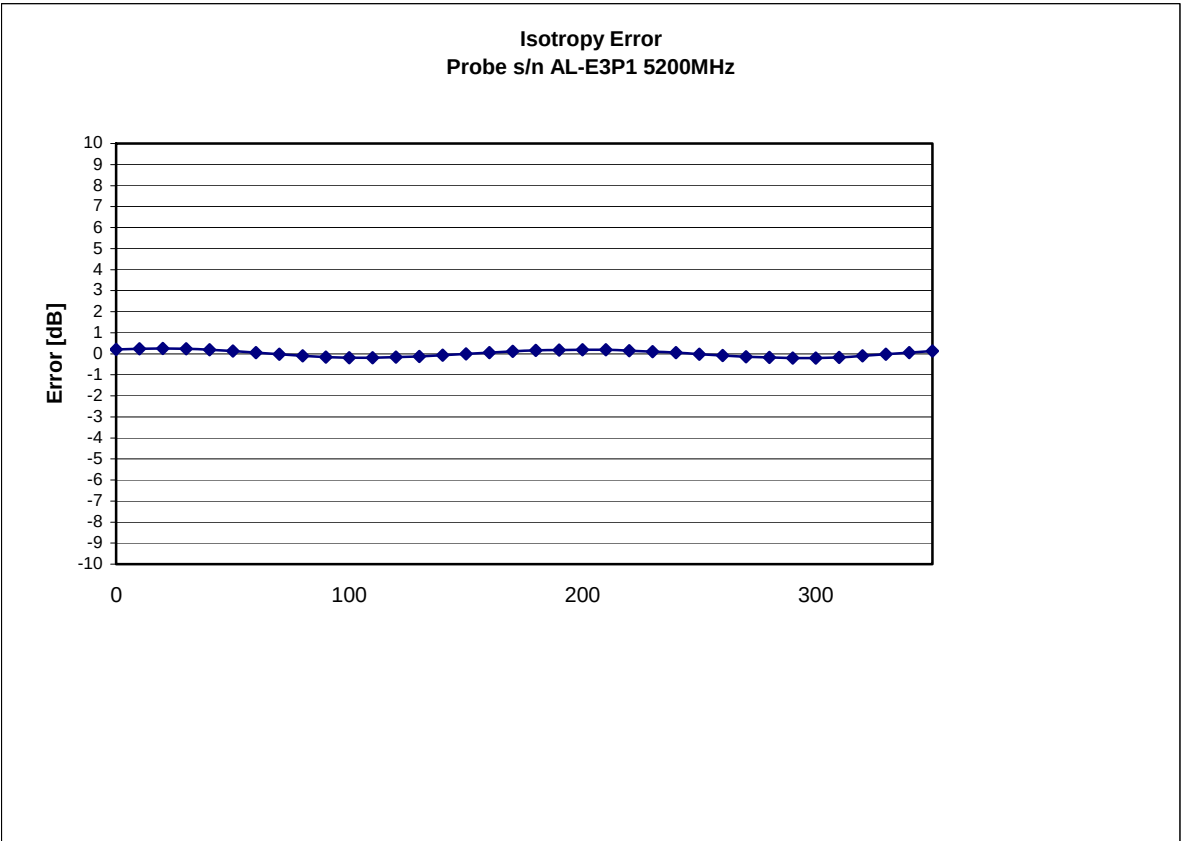


Isotropy in Tissue:

0.15 dB

Dynamic Range

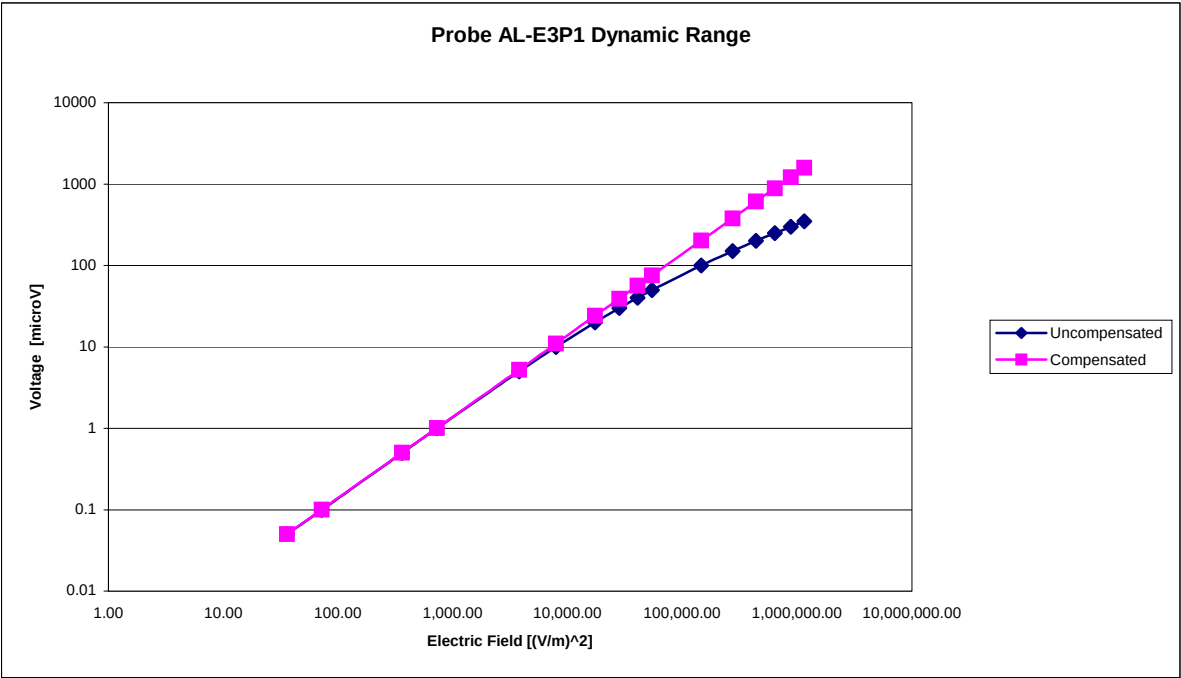

Video Bandwidth

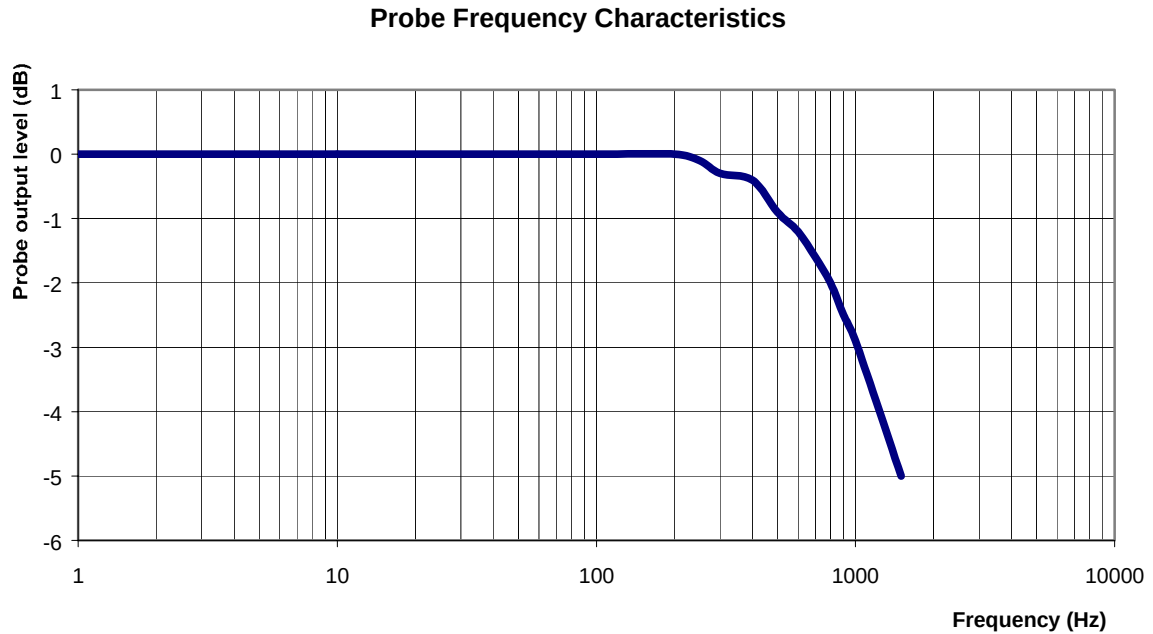

Video Bandwidth at 500 Hz 1 dB
Video Bandwidth at 1.02 KHz: 3 dB

Conversion Factor Uncertainty Assessment

Frequency: 5200 MHz

Epsilon: 48.9 (+/-10%)

Sigma: 5.35 S/m (+/-10%)

ConvF

Channel X: 13 7%(K=2)

Channel Y: 13 7%(K=2)

Channel Z: 13 7%(K=2)

To minimize the uncertainty calculation all tissue sensitivity values were calculated using a load impedance of 5 M Ω .

Boundary Effect:

For a distance of 0.5 mm the evaluated uncertainty (increase in the probe sensitivity) is less than 2%.

Test Equipment

The test equipment used during Probe Calibration, manufacturer, model number and, current calibration status are listed and located on the main APREL server R:\NCL\Calibration Equipment\Instrument List May 2006.

NCL CALIBRATION LABORATORIES

Calibration File No.: CP-754

Client.: APREL

CERTIFICATE OF CALIBRATION

It is certified that the equipment identified below has been calibrated in the
NCL CALIBRATION LABORATORIES by qualified personnel following recognized
procedures and using transfer standards traceable to NRC/NIST.

Equipment: Miniature Isotropic RF Probe 5800 MHz

Manufacturer: APREL Laboratories

Model No.: E-030

Serial No.: AL-E3P1

Calibration in Body Tissue


Calibration Procedure: SSI/DRB-TP-D01-032-E020-V2

Project No: APLB-5800-PC-5264

Calibrated: 30th April 2007
Released on: 30th April 2007

This Calibration Certificate is Incomplete Unless Accompanied with the Calibration Results Summary

Released By: _____

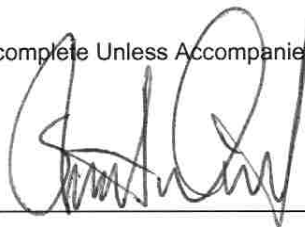

NCL CALIBRATION LABORATORIES

17 Bentley Avenue
NEPEAN, ONTARIO
CANADA K2E 6T7

Division of APREL Lab.
TEL: (613) 820-4988
FAX: (613) 820-4161

Introduction

This Calibration Report reproduces the results of the calibration performed in line with the SSI/DRB-TP-D01-032-E020-V2 E-Field Probe Calibration Procedure. The results contained within this report are for APREL E-Field Probe E-030 AL-E3P1.

References

SSI/DRB-TP-D01-032-E020-V2 E-Field Probe Calibration Procedure
IEEE 1528 "Recommended Practice for Determining the Peak Spatial-Average Specific Absorption Rate (SAR) in the Human Body Due to Wireless Communications Devices: Experimental Techniques"
SSI-TP-011 Tissue Calibration Procedure


Conditions


Probe AL-E3P1 was a new probe taken from stock prior to calibration.

Ambient Temperature of the Laboratory: 22 °C +/- 0.5°C

Temperature of the Tissue: 21 °C +/- 0.5°C

We the undersigned attest that to the best of our knowledge the calibration of this probe has been accurately conducted and that all information contained within this report has been reviewed for accuracy.



Stuart Nicol

Jesse Hones

Calibration Results Summary

Probe Type:	E-Field Probe E-030
Serial Number:	AL-E3P1
Frequency:	5800 MHz
Sensor Offset:	0.56 mm
Sensor Length:	2.5 mm
Tip Enclosure:	Ertalyte*
Tip Diameter:	<3 mm
Tip Length:	60 mm
Total Length:	290 mm

*Resistive to recommended tissue recipes per IEEE-1528

Sensitivity in Air

Channel X:	$1.2 \mu\text{V}/(\text{V}/\text{m})^2$
Channel Y:	$1.2 \mu\text{V}/(\text{V}/\text{m})^2$
Channel Z:	$1.2 \mu\text{V}/(\text{V}/\text{m})^2$
Diode Compression Point:	95 mV

Sensitivity in FCC Body Tissue

Frequency: 5800 MHz

Epsilon: 48.2 (+/-10%) **Sigma:** 6.0 S/m (+/-10%)

ConvF

Channel X: 14

Channel Y: 14

Channel Z: 14

Tissue sensitivity values were calculated using the load impedance of the APREL Laboratories Daq-Paq.


Boundary Effect:

Uncertainty resulting from the boundary effect is less than 2% for the distance between the tip of the probe and the tissue boundary, when less than 0.5mm.



Spatial Resolution:

The measured probe tip diameter is less than 3 mm (+/- 0.01 mm) and therefore meets the requirements of SSI/DRB-TP-D01-032 for spatial resolution.

Receiving Pattern 5800 MHz (Air)

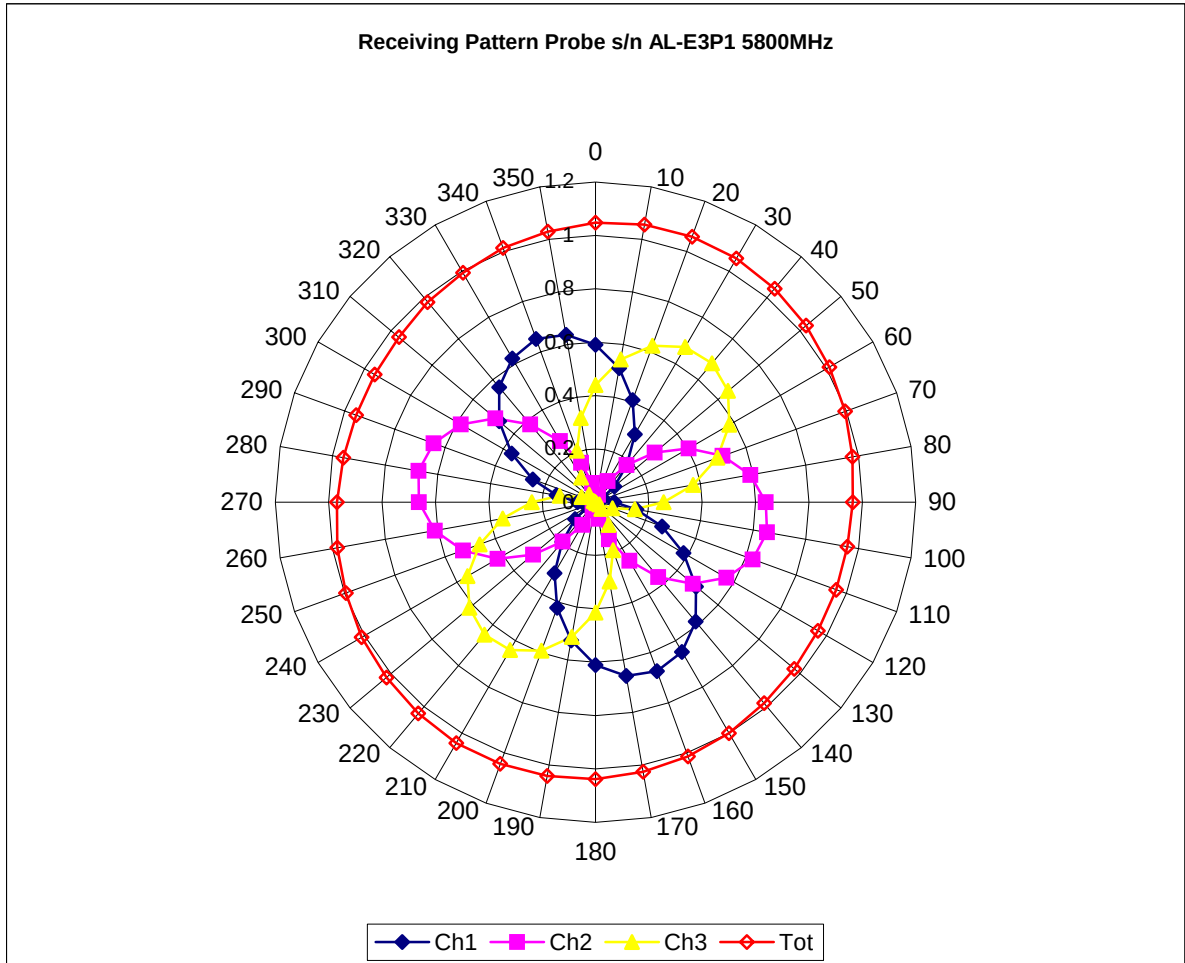


Isotropy Error 5800 MHz (Air)

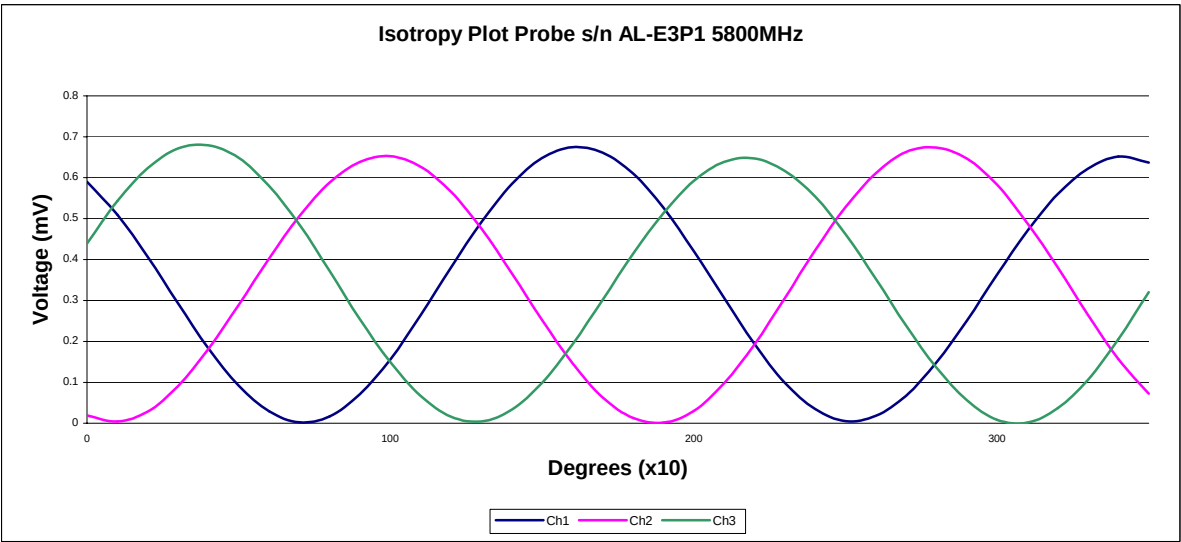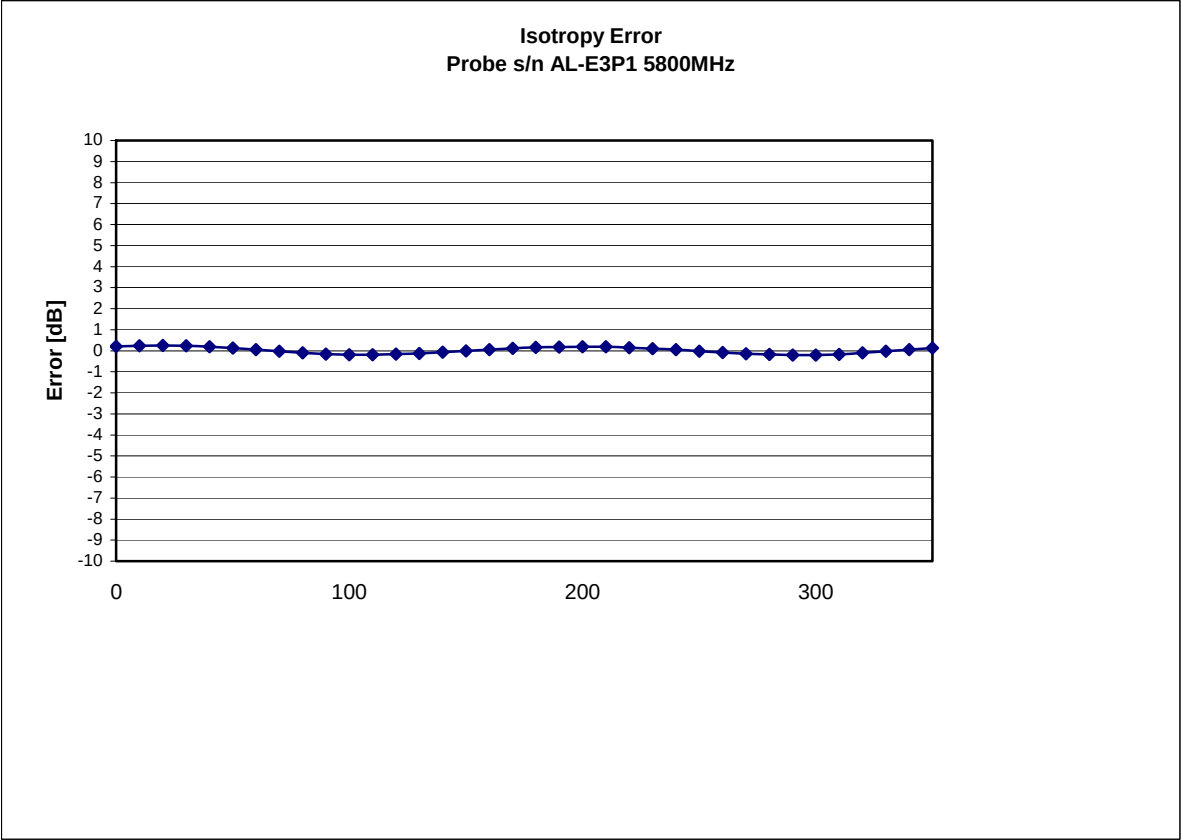


Isotropy in Tissue:

0.15 dB

Dynamic Range

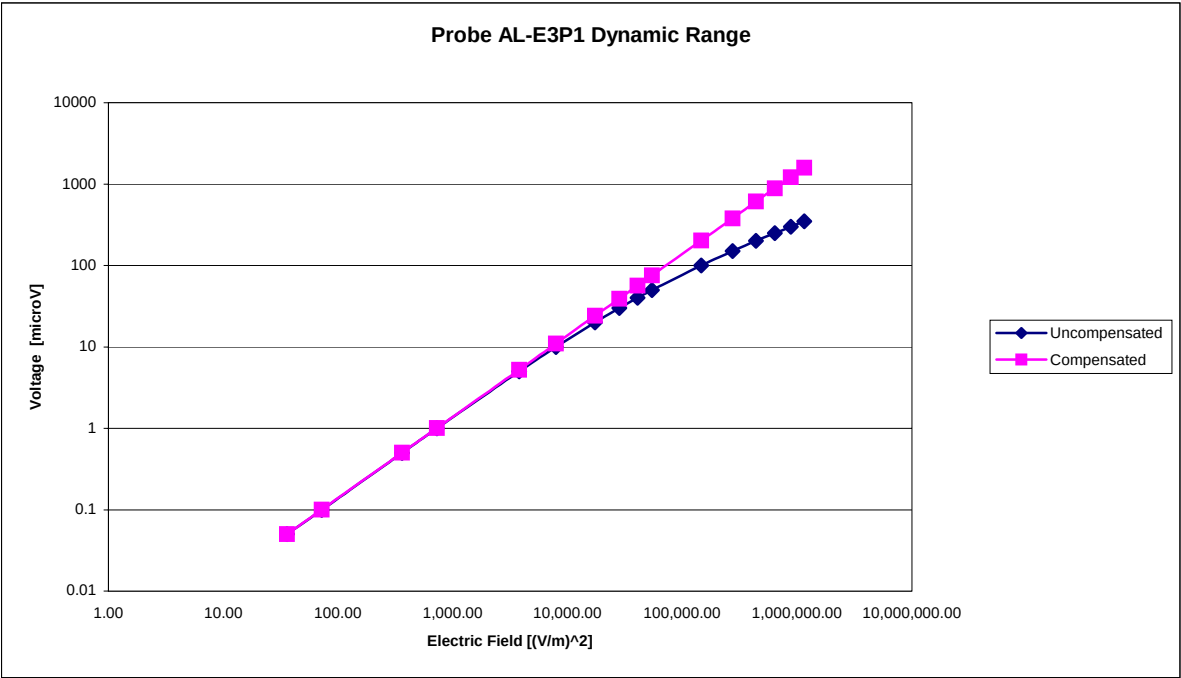

Video Bandwidth

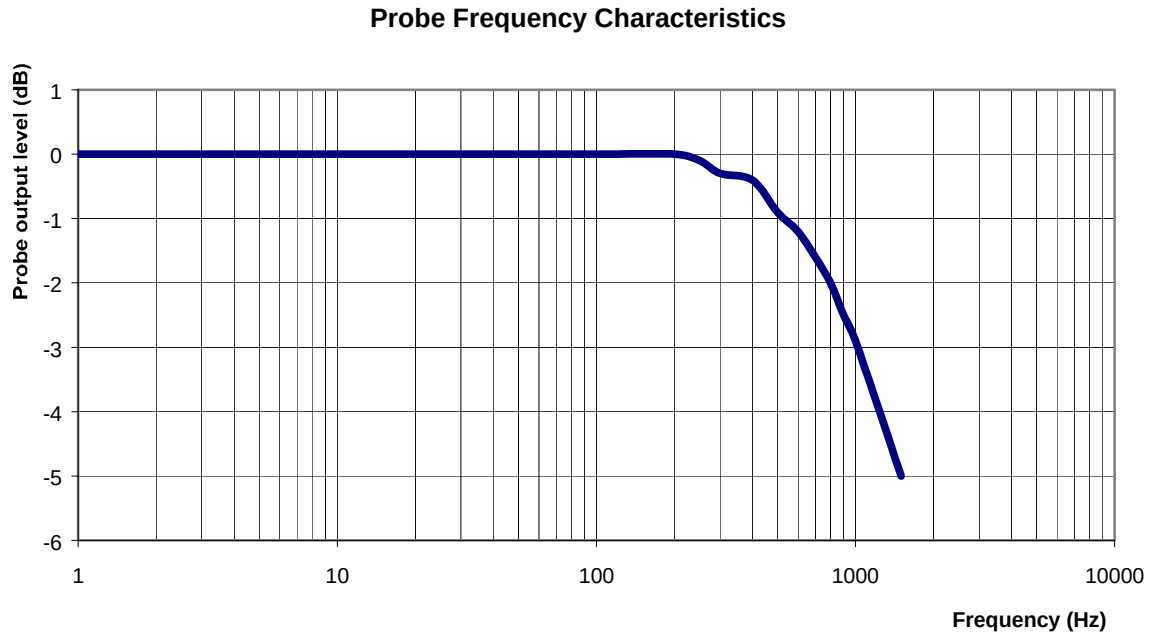

Video Bandwidth at 500 Hz 1 dB
Video Bandwidth at 1.02 KHz: 3 dB

Conversion Factor Uncertainty Assessment

Frequency:

5800 MHz

Epsilon: 48.4 (+/-10%)

Sigma: 6.0 S/m (+/-10%)

ConvF

Channel X: 14

7%(K=2)

Channel Y: 14

7%(K=2)

Channel Z: 14

7%(K=2)

To minimize the uncertainty calculation all tissue sensitivity values were calculated using a load impedance of 5 M Ω .

Boundary Effect:

For a distance of 0.5 mm the evaluated uncertainty (increase in the probe sensitivity) is less than 2%.

Test Equipment

The test equipment used during Probe Calibration, manufacturer, model number and, current calibration status are listed and located on the main APREL server R:\NCL\Calibration Equipment\Instrument List May 2006.

Appendix E – Dipole Calibration Data Sheets

RF Exposure Lab, LLC

Calibration File No: CAL.20080201

CERTIFICATE OF CALIBRATION

It is certified that the equipment identified below has been calibrated at RF Exposure Lab, LLC by qualified personnel following recognized procedures and using transfer standards traceable to NRC/NIST.

Validation Dipole

Manufacturer: APREL Laboratories

Part Number: ALS-D-2450-S-2

Frequency: 2.4 GHz

Serial No: RFE-278

Manufactured: 20 February 2004
Calibrated: 20 February 2008

Calibrated By: Signature on File
Jay Moulton – Technical Manager

Approved By: Signature on File
Tamara Moulton – Quality Manager

Measurement Uncertainty:

Repeatability:	2.3%
Tissue Uncertainty:	3.2%
Network Analyzer:	2.5%



RF EXPOSURE LAB, LLC

2867 Progress Place, Suite 4D
Escondido, CA 92029

Tel: (760) 737-3131
FAX: (760) 737-9131

Calibration Results Summary

The following results relate to the Calibrated Dipole and should be used as a quick reference for the user.

Mechanical Dimensions

Length: 51.5 mm
Height: 30.5 mm

Electrical Specifications

Head

SWR: 1.0953 U
Return Loss: -29.601 dB
Impedance: 53.854 Ω

System Validation Results

Frequency	1 Gram	10 Gram
2.45 GHz	52.880	24.500

Body

SWR: 1.1354 U
Return Loss: -31.173 dB
Impedance: 54.146 Ω

System Validation Results

Frequency	1 Gram	10 Gram
2.45 GHz	53.550	24.710

Head Measurement Conditions

The measurements were performed in the Uni-Phantom filled with head simulating liquid of the following electrical parameters at 2450 MHz:

Relative Dielectricity	39.37	$\pm 5\%$
Conductivity	1.78 mho/m	$\pm 5\%$

The APREL Laboratories ALSAS system with a dosimetric E-field probe E-020 (SN:217, Conversion factor 3.4 at 2450 MHz) was used for the measurements.

The dipole was mounted so that the dipole feed point was positioned below the center marking of the flat phantom and the dipole was oriented parallel to the body axis (the long side of the phantom). The standard measuring distance was 10mm from the dipole center to the solution surface.

The coarse grid with a grid spacing of 10mm was aligned with the dipole. The 5x5x8 fine cube was chosen for cube integration. The dipole input power (forward power) was 100mW $\pm 3\%$. The results are normalized to 1W input power.

The laboratories environmental conditions were as follows during the calibration sequence.

Ambient Temperature of the Laboratory:	24 °C ± 1.0 °C
Temperature of the Tissue:	20 °C ± 1.0 °C
Relative Humidity:	41%


SAR Measurement

Standard SAR measurements were performed according to the measurement conditions described above. The results have been normalized to a dipole input power of 1W (forward power). The resulting averaged SAR values measured with the dosimetric probe E-020 SN:217 and applying the advanced extrapolation are:

Averaged over 1 cm³ (1 g) of tissue: 52.880 mW/g $\pm$ 19.7% (k=2)¹

Averaged over 10 cm³ (10 g) of tissue: 24.500 mW/g $\pm$ 19.4% (k=2)¹

Area Scan

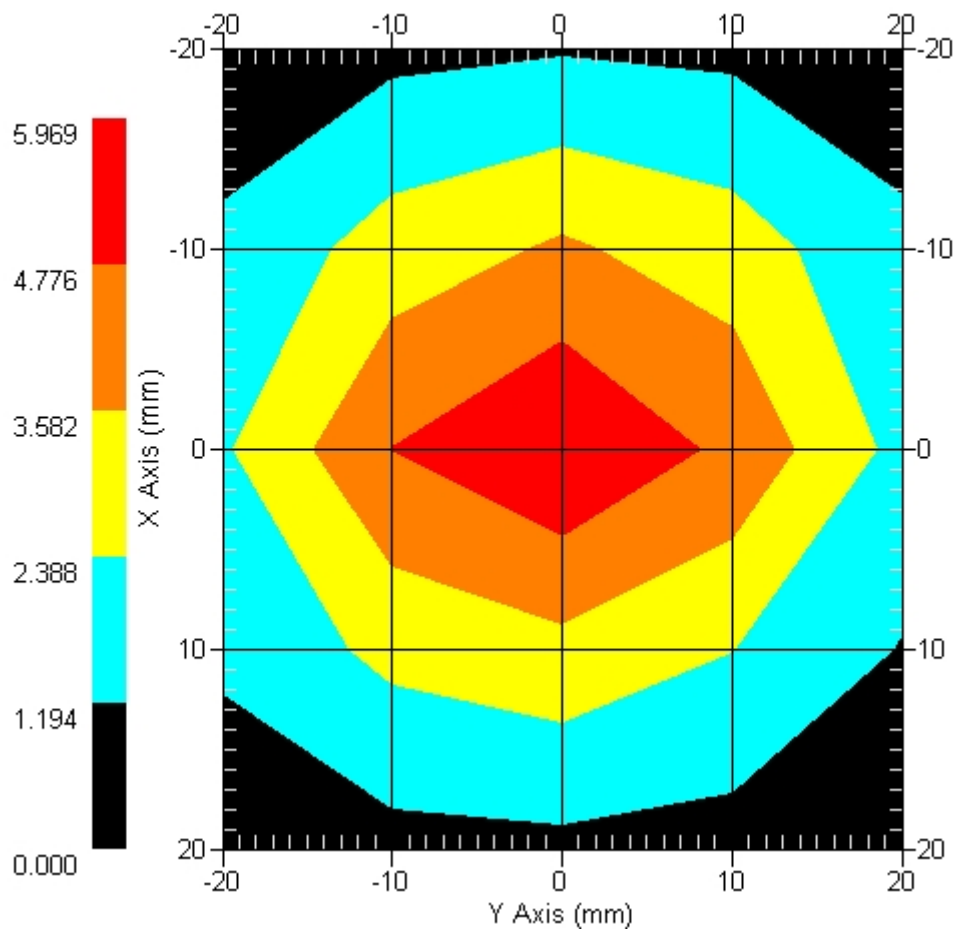

1 gram SAR value : 5.288 W/kg
 10 gram SAR value : 2.450 W/kg
 Area Scan Peak SAR : 5.969 W/kg
 Zoom Scan Peak SAR : 10.890 W/kg

¹ validation uncertainty


Dipole Impedance and Return Loss

The impedance was measured at the SMA connector with a network analyzer. The dipole was positioned at the flat phantom sections according to measurement conditions stated above during impedance measurements.


Test	Result
S11 R/L	-29.601 dB
SWR	1.0953 U
Impedance	53.854 Ω

The following graphs are the results as displayed on the Vector Network Analyzer.


S11 Parameter Return Loss

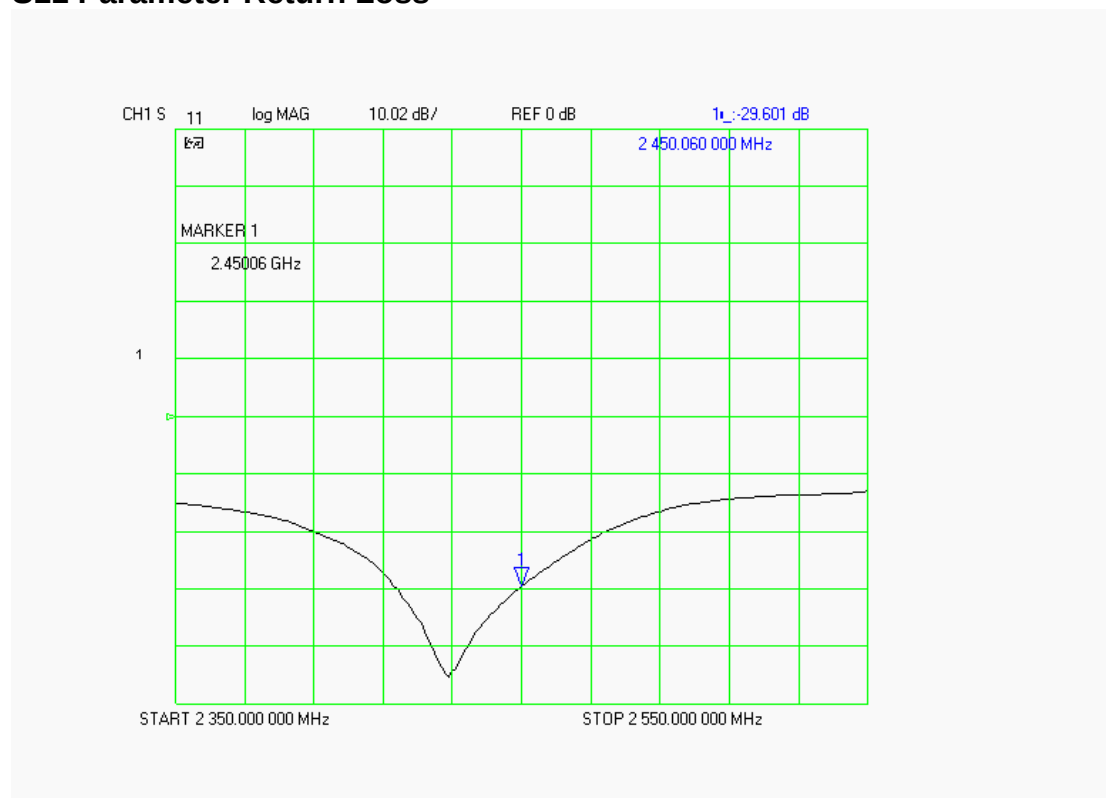

SWR

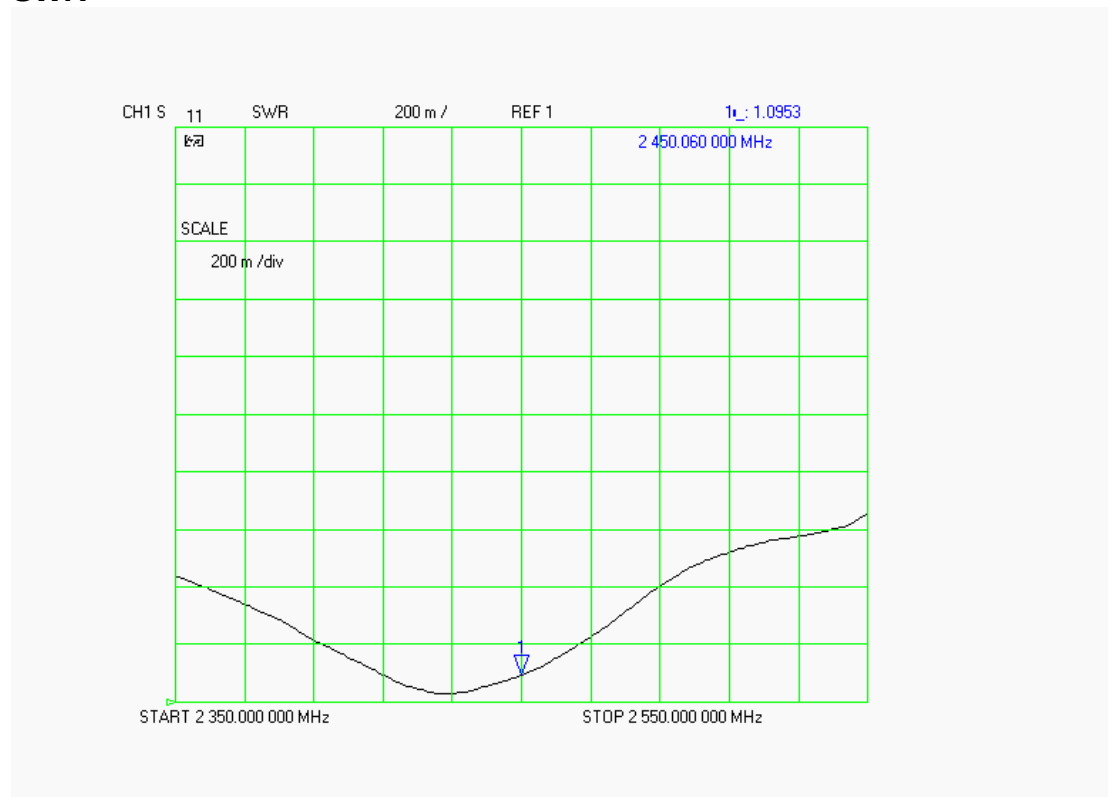

Smith Chart Dipole Impedance

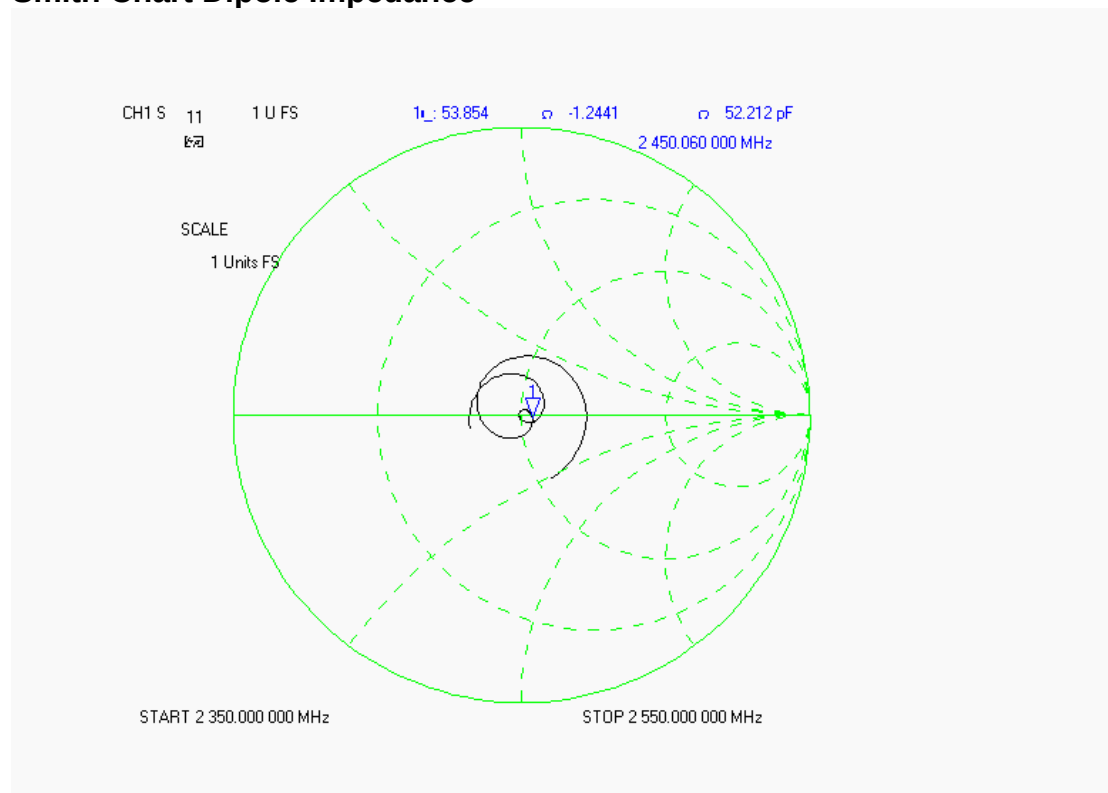

Body Measurement Conditions

The measurements were performed in the Uni-Phantom filled with body simulating liquid of the following electrical parameters at 2450 MHz:

Relative Dielectricity	52.59	$\pm 5\%$
Conductivity	1.92 mho/m	$\pm 5\%$

The APREL Laboratories ALSAS system with a dosimetric E-field probe E-020 (SN:217, Conversion factor 3.61 at 2450 MHz) was used for the measurements.

The dipole was mounted so that the dipole feed point was positioned below the center marking of the flat phantom and the dipole was oriented parallel to the body axis (the long side of the phantom). The standard measuring distance was 10mm from the dipole center to the solution surface.

The coarse grid with a grid spacing of 10mm was aligned with the dipole. The 5x5x8 fine cube was chosen for cube integration. The dipole input power (forward power) was 100mW $\pm 3\%$. The results are normalized to 1W input power.

The laboratories environmental conditions were as follows during the calibration sequence.

Ambient Temperature of the Laboratory:	24 °C ± 1.0 °C
Temperature of the Tissue:	20 °C ± 1.0 °C
Relative Humidity:	41%


SAR Measurement

Standard SAR measurements were performed according to the measurement conditions described above. The results have been normalized to a dipole input power of 1W (forward power). The resulting averaged SAR values measured with the dosimetric probe E-020 SN:217 and applying the advanced extrapolation are:

Averaged over 1 cm³ (1 g) of tissue: 53.550 mW/g $\pm$ 18.8% (k=2)¹

Averaged over 10 cm³ (10 g) of tissue: 24.710 mW/g $\pm$ 18.4% (k=2)¹

Area Scan

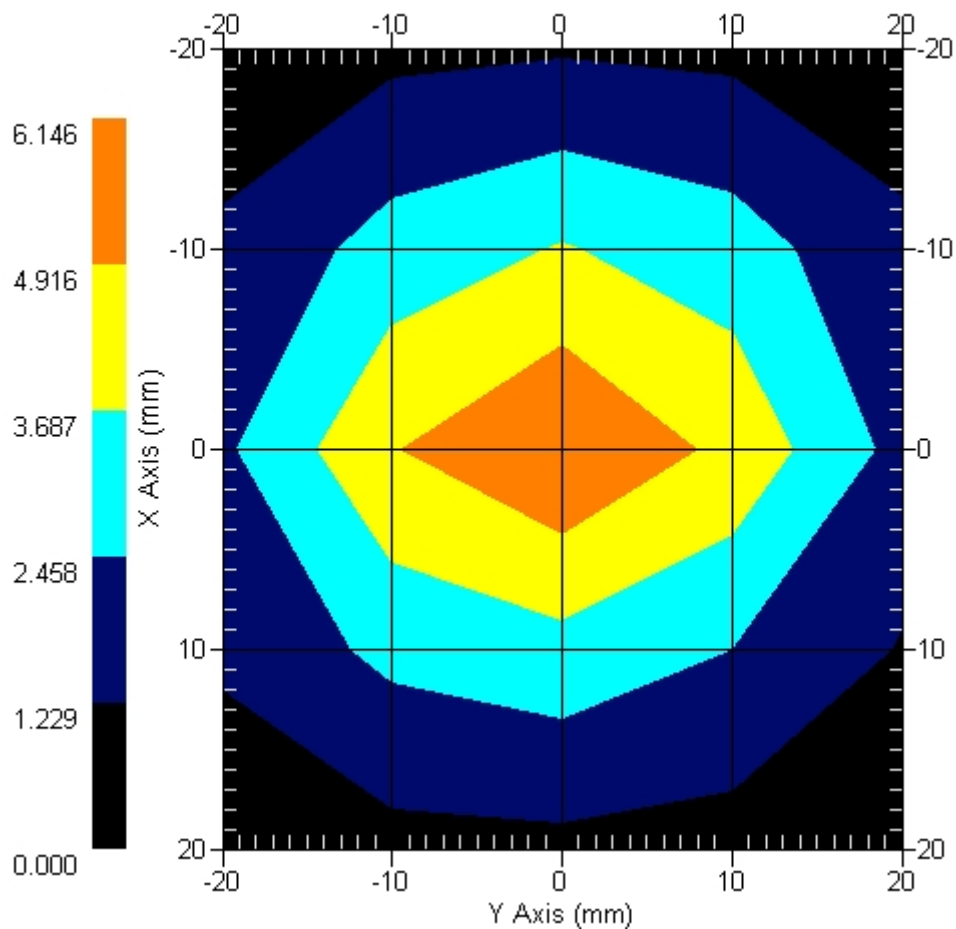

1 gram SAR value : 5.355 W/kg
 10 gram SAR value : 2.471 W/kg
 Area Scan Peak SAR : 6.146 W/kg
 Zoom Scan Peak SAR : 11.090 W/kg

¹ validation uncertainty


Dipole Impedance and Return Loss

The impedance was measured at the SMA connector with a network analyzer. The dipole was positioned at the flat phantom sections according to measurement conditions stated above during impedance measurements.


Test	Result
S11 R/L	-31.173 dB
SWR	1.1354 U
Impedance	54.146 Ω

The following graphs are the results as displayed on the Vector Network Analyzer.


S11 Parameter Return Loss

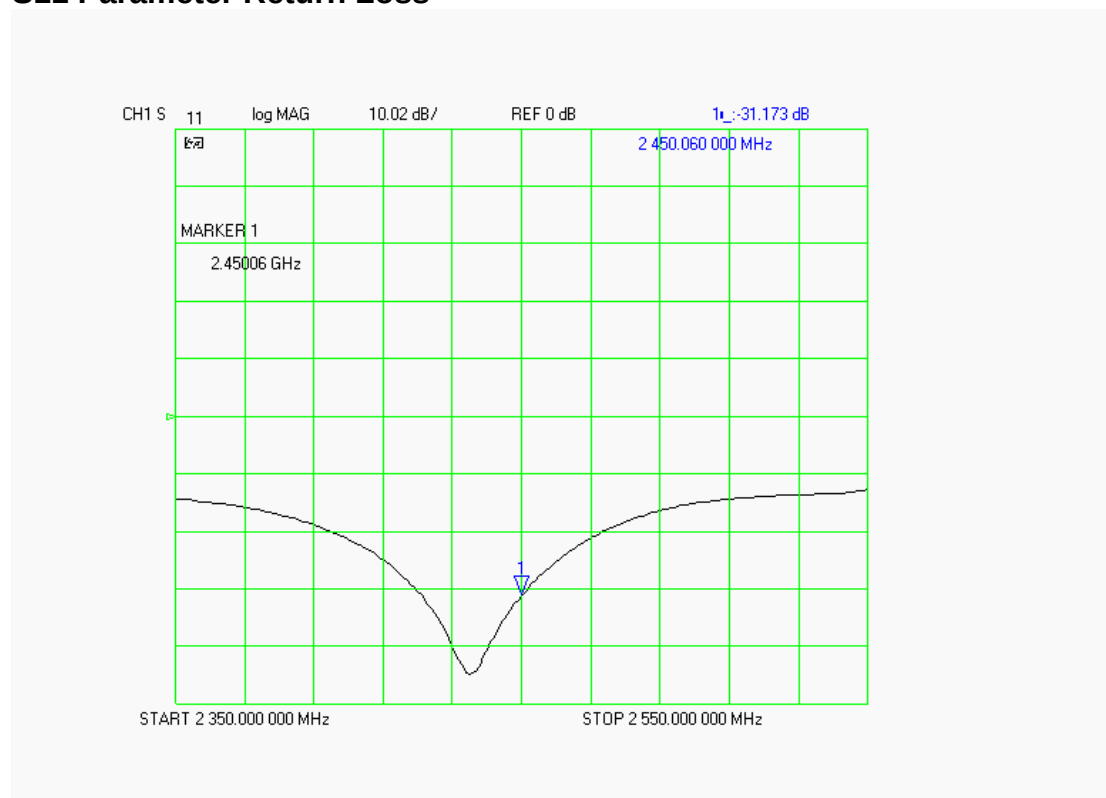

SWR

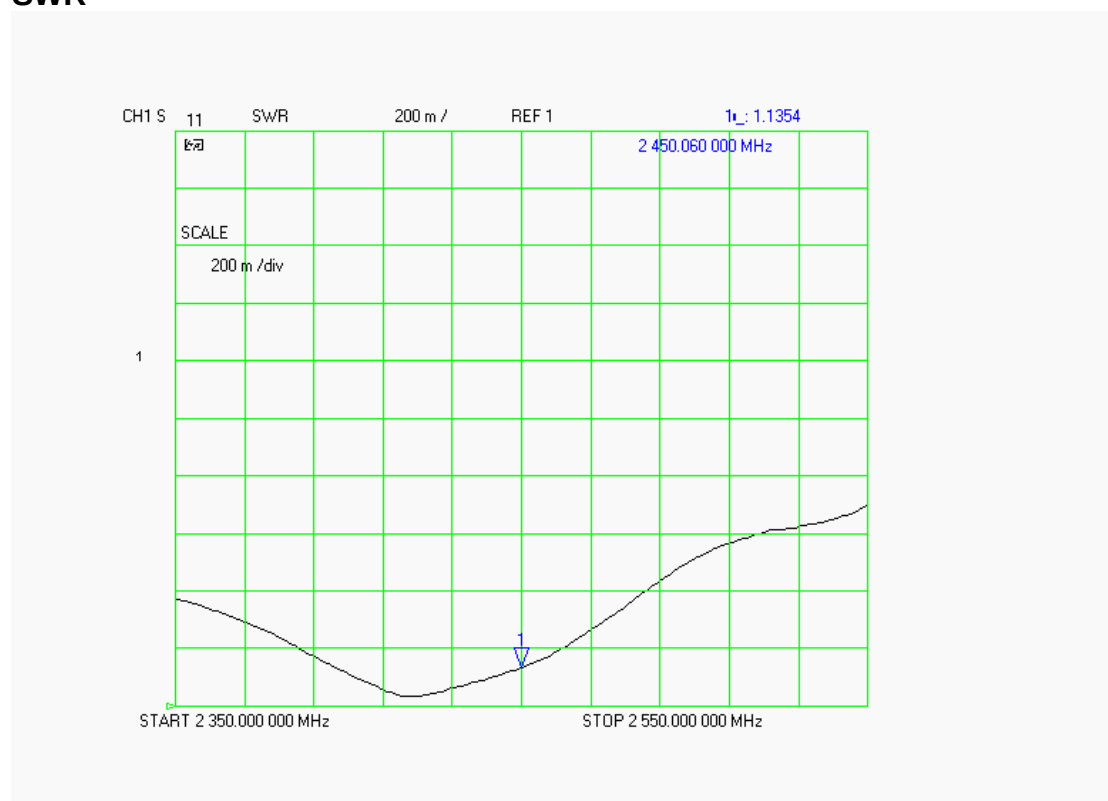

Smith Chart Dipole Impedance

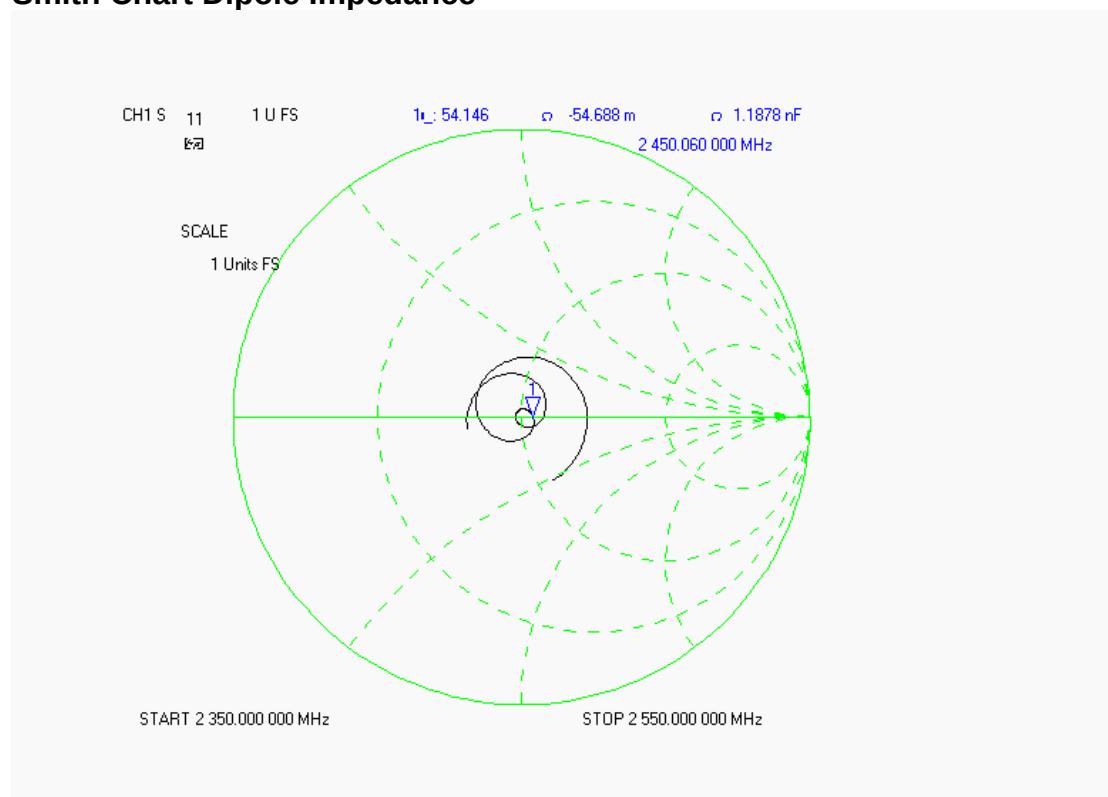

Test Equipment List

The test equipment used during Dipole Calibration, manufacturer, model number and, current calibration status are listed and located on the RF Exposure Lab, LLC system computer C:\Test Equipment\Calibration Equipment\Instrument List February 2008.

RF Exposure Lab, LLC

Calibration File No: CAL.20070501

CERTIFICATE OF CALIBRATION

It is certified that the equipment identified below has been calibrated at RF Exposure Lab, LLC by qualified personnel following recognized procedures and using transfer standards traceable to NRC/NIST.

Validation Dipole

Manufacturer: APREL Laboratories

Part Number: ALS-D-BB-S-2

Frequency: 5.2 GHz to 5.8 GHz

Serial No: 235-00801

Manufactured: 22 May 2005
Calibrated: 23 May 2007

Calibrated By: Signature on File
Jay Moulton – Technical Manager

Approved By: Signature on File
Tamara Moulton – Quality Manager

Measurement Uncertainty:

Repeatability:	2.3%
Tissue Uncertainty:	3.2%
Network Analyzer:	2.5%



RF EXPOSURE LAB, LLC

2867 Progress Place, Suite 4D
Escondido, CA 92029

Tel: (760) 737-3131
FAX: (760) 737-9131

Calibration Results Summary

The following results relate to the Calibrated Dipole and should be used as a quick reference for the user.

Mechanical Dimensions

Length: 23.3 mm
Height: 20.3 mm

Electrical Specifications

5.2 GHz Body

SWR: 1.8749 U
Return Loss: -17.057 dB
Impedance: 54.252 Ω

System Validation Results

Frequency	1 Gram	10 Gram
5.2 GHz	62.98	15.44

5.6 GHz Body

SWR: 1.2178 U
Return Loss: -18.513 dB
Impedance: 45.365 Ω

System Validation Results

Frequency	1 Gram	10 Gram
5.6 GHz	59.92	15.30

5.8 GHz Body

SWR: 1.8551 U
Return Loss: -10.237 dB
Impedance: 45.014 Ω

System Validation Results

Frequency	1 Gram	10 Gram
5.8 GHz	58.92	15.05

5.2 GHz Body Measurement Conditions

The measurements were performed in the Uni-Phantom filled with body simulating liquid of the following electrical parameters at 5.2 GHz:

Relative Dielectricity	49.19	$\pm 5\%$
Conductivity	5.40 mho/m	$\pm 5\%$

The APREL Laboratories ALSAS system with a dosimetric E-field probe E-030 (SN:AL-E3P1, Conversion factor 13.0 at 5.2 GHz) was used for the measurements.

The dipole was mounted so that the dipole feed point was positioned below the center marking of the flat phantom and the dipole was oriented parallel to the body axis (the long side of the phantom). The standard measuring distance was 10mm from the dipole center to the solution surface.

The coarse grid with a grid spacing of 10mm was aligned with the dipole. The 7x7x7 fine cube was chosen for cube integration. The dipole input power (forward power) was 100mW $\pm 3\%$. The results are normalized to 1W input power.

The laboratories environmental conditions were as follows during the calibration sequence.


Ambient Temperature of the Laboratory:	23 °C ± 1.0 °C
Temperature of the Tissue:	20 °C ± 1.0 °C
Relative Humidity:	52%

SAR Measurement

Standard SAR measurements were performed according to the measurement conditions described above. The results have been normalized to a dipole input power of 1W (forward power). The resulting averaged SAR values measured with the dosimetric probe E-030 SN:AL-E3P1 and applying the advanced extrapolation are:

Averaged over 1 cm³ (1 g) of tissue: 62.98 mW/g $\pm$ 19.1% (k=2)¹

Averaged over 10 cm³ (10 g) of tissue: 15.44 mW/g $\pm$ 18.8% (k=2)¹

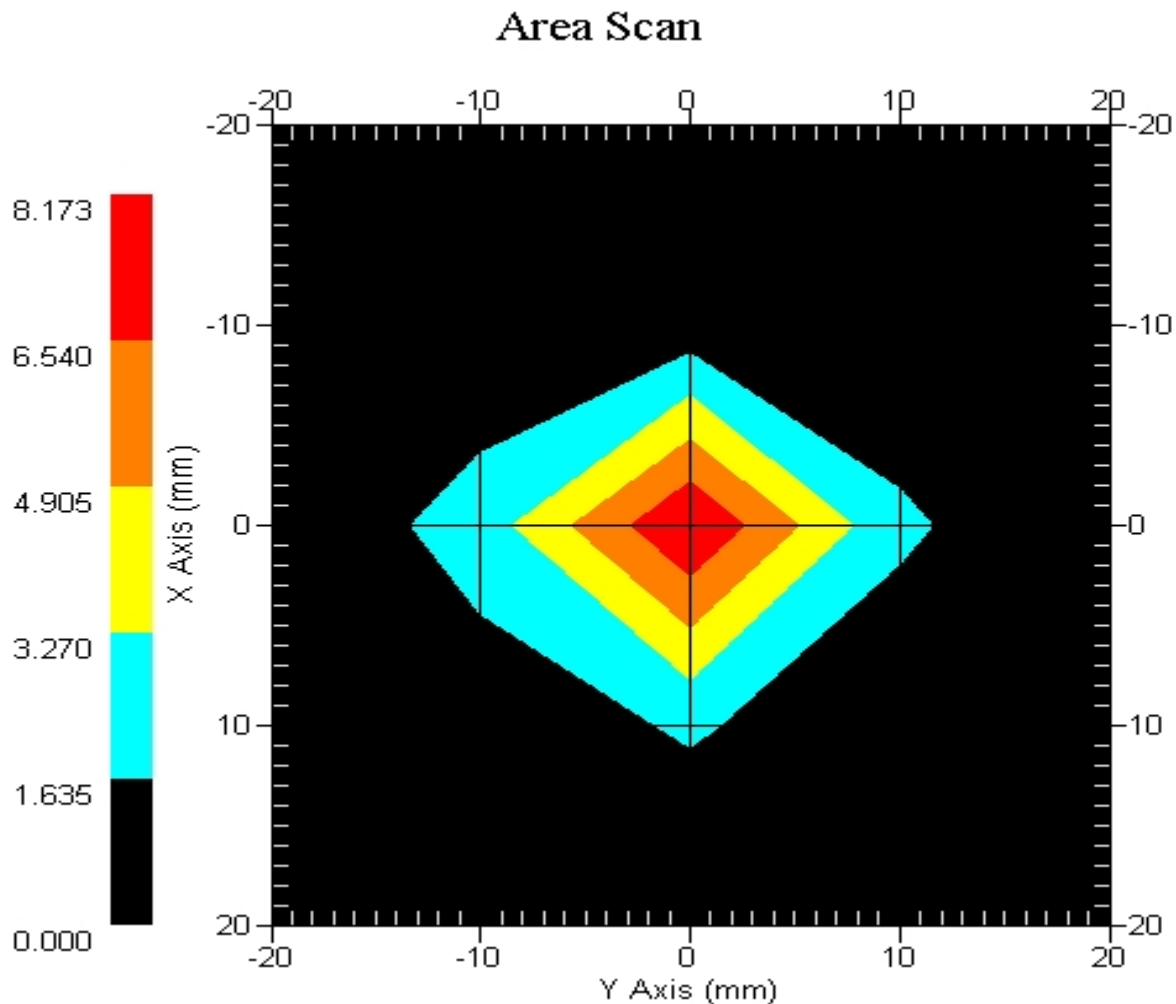

1 gram SAR value : 6.298 W/kg
 10 gram SAR value : 1.544 W/kg
 Area Scan Peak SAR : 8.173 W/kg
 Zoom Scan Peak SAR : 21.817 W/kg

¹ validation uncertainty

5.6 GHz Body Measurement Conditions

The measurements were performed in the Uni-Phantom filled with body simulating liquid of the following electrical parameters at 5.6 GHz:

Relative Dielectricity	48.22	$\pm 5\%$
Conductivity	5.68 mho/m	$\pm 5\%$

The APREL Laboratories ALSAS system with a dosimetric E-field probe E-030 (SN:AL-E3P1, Conversion factor 13.5 at 5.6 GHz) was used for the measurements.

The dipole was mounted so that the dipole feed point was positioned below the center marking of the flat phantom and the dipole was oriented parallel to the body axis (the long side of the phantom). The standard measuring distance was 10mm from the dipole center to the solution surface.

The coarse grid with a grid spacing of 10mm was aligned with the dipole. The 7x7x7 fine cube was chosen for cube integration. The dipole input power (forward power) was 100mW $\pm 3\%$. The results are normalized to 1W input power.

The laboratories environmental conditions were as follows during the calibration sequence.


Ambient Temperature of the Laboratory:	23 °C ± 1.0 °C
Temperature of the Tissue:	20 °C ± 1.0 °C
Relative Humidity:	52%

SAR Measurement

Standard SAR measurements were performed according to the measurement conditions described above. The results have been normalized to a dipole input power of 1W (forward power). The resulting averaged SAR values measured with the dosimetric probe E-030 SN:AL-E3P1 and applying the advanced extrapolation are:

Averaged over 1 cm³ (1 g) of tissue: 59.92 mW/g $\pm$ 19.1% (k=2)¹

Averaged over 10 cm³ (10 g) of tissue: 15.30 mW/g $\pm$ 18.8% (k=2)¹

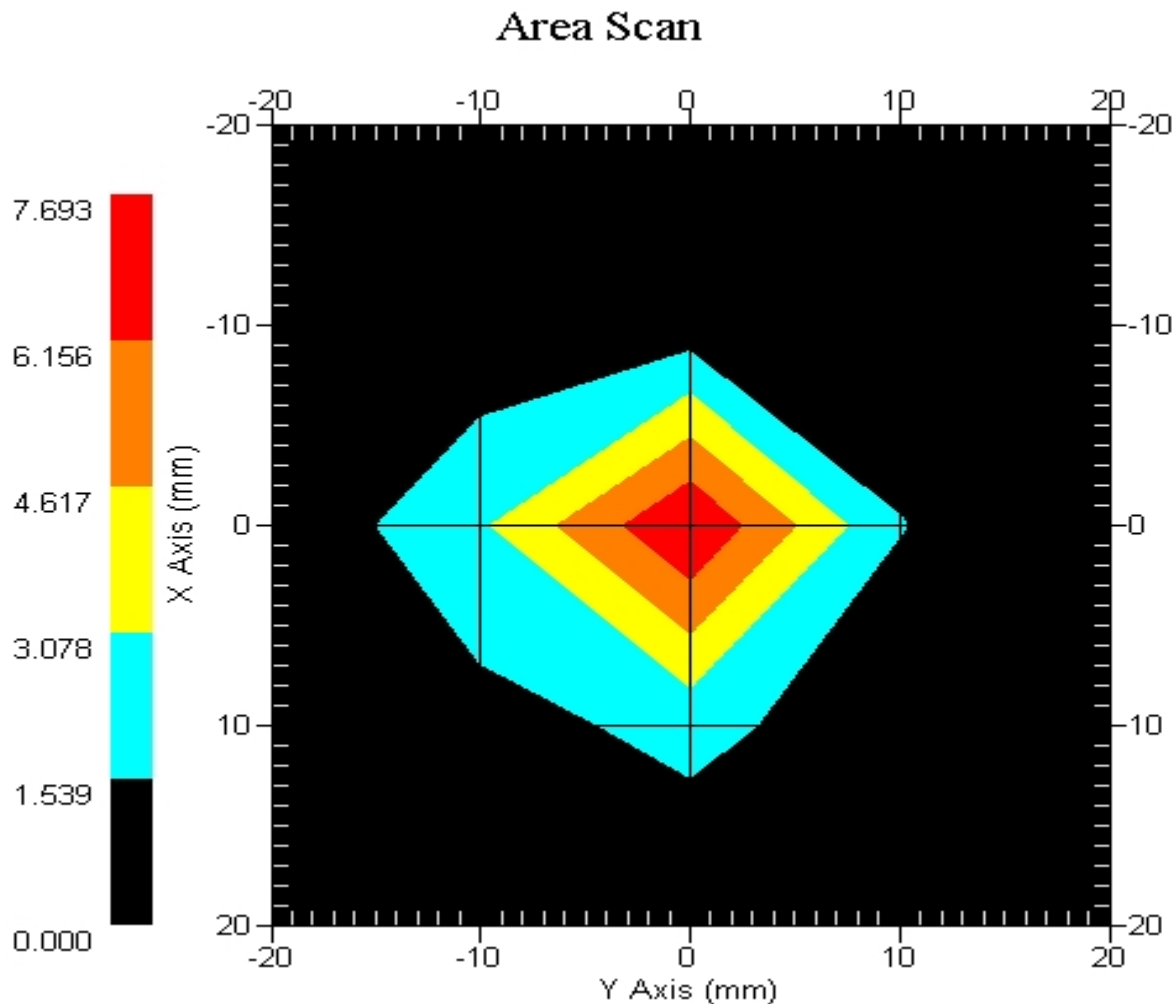

1 gram SAR value : 5.992 W/kg
 10 gram SAR value : 1.530 W/kg
 Area Scan Peak SAR : 7.693 W/kg
 Zoom Scan Peak SAR : 19.415 W/kg

¹ validation uncertainty

5.8 GHz Body Measurement Conditions

The measurements were performed in the Uni-Phantom filled with body simulating liquid of the following electrical parameters at 5.8 GHz:

Relative Dielectricity	48.53	$\pm 5\%$
Conductivity	5.95 mho/m	$\pm 5\%$

The APREL Laboratories ALSAS system with a dosimetric E-field probe E-030 (SN:AL-E3P1, Conversion factor 14.0 at 5.8 GHz) was used for the measurements.

The dipole was mounted so that the dipole feed point was positioned below the center marking of the flat phantom and the dipole was oriented parallel to the body axis (the long side of the phantom). The standard measuring distance was 10mm from the dipole center to the solution surface.

The coarse grid with a grid spacing of 10mm was aligned with the dipole. The 7x7x7 fine cube was chosen for cube integration. The dipole input power (forward power) was 100mW $\pm 3\%$. The results are normalized to 1W input power.

The laboratories environmental conditions were as follows during the calibration sequence.


Ambient Temperature of the Laboratory:	23 °C ± 1.0 °C
Temperature of the Tissue:	20 °C ± 1.0 °C
Relative Humidity:	52%

SAR Measurement

Standard SAR measurements were performed according to the measurement conditions described above. The results have been normalized to a dipole input power of 1W (forward power). The resulting averaged SAR values measured with the dosimetric probe E-030 SN:AL-E3P1 and applying the advanced extrapolation are:

Averaged over 1 cm³ (1 g) of tissue: 58.92 mW/g $\pm$ 19.1% (k=2)¹

Averaged over 10 cm³ (10 g) of tissue: 15.05 mW/g $\pm$ 18.8% (k=2)¹

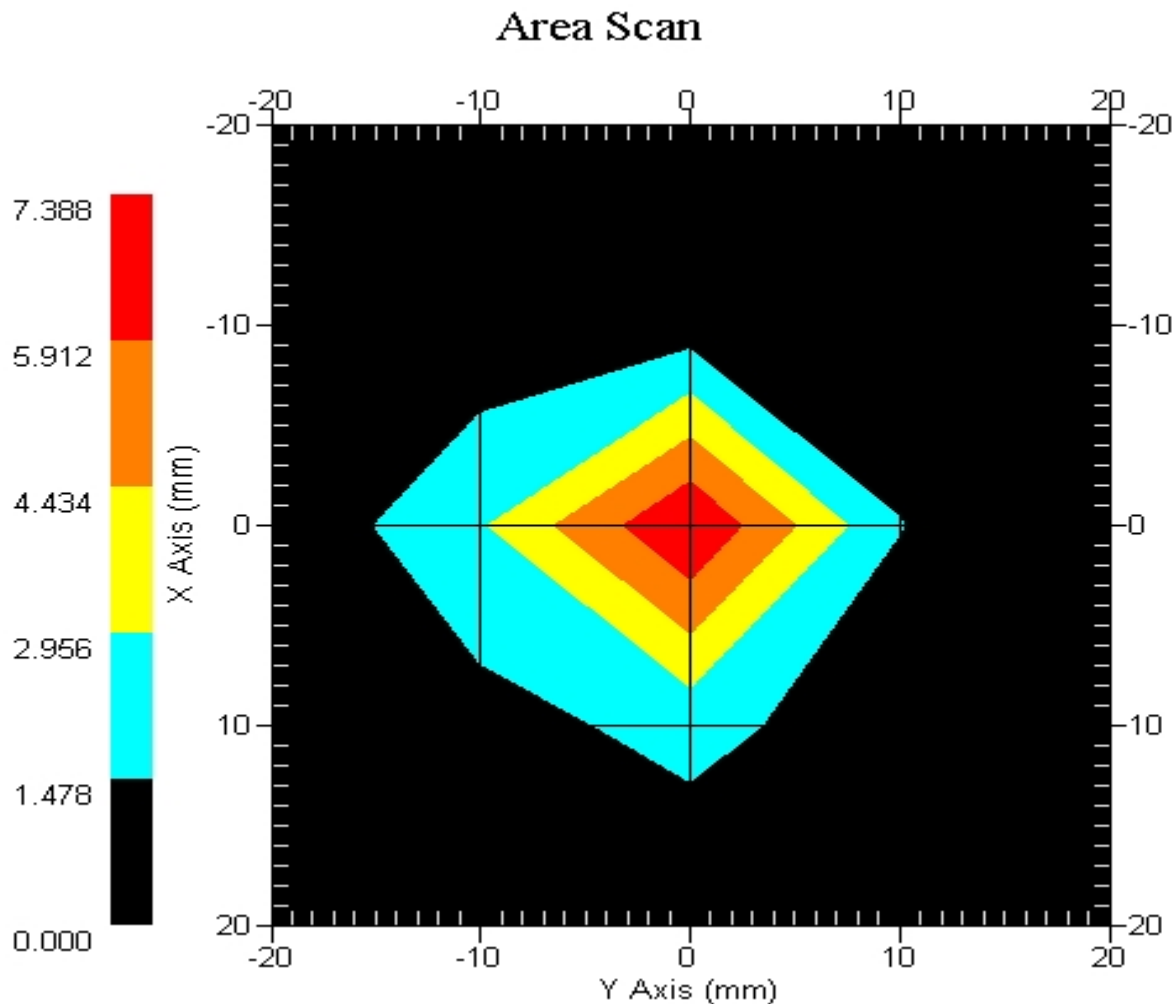

1 gram SAR value : 5.892 W/kg
 10 gram SAR value : 1.505 W/kg
 Area Scan Peak SAR : 7.388 W/kg
 Zoom Scan Peak SAR : 19.315 W/kg

¹ validation uncertainty


Dipole Impedance and Return Loss

The impedance was measured at the SMA connector with a network analyzer. The dipole was positioned at the flat phantom sections according to measurement conditions stated above during impedance measurements.


Test	Result – 5.2 GHz	Result – 5.6 GHz	Result – 5.8 GHz
S11 R/L	-17.057 dB	-18.513 dB	-10.237 dB
SWR	1.8749 U	1.2178 U	1.8551 U
Impedance	54.252 Ω	45.365 Ω	45.014 Ω

The following graphs are the results as displayed on the Vector Network Analyzer.


S11 Parameter Return Loss

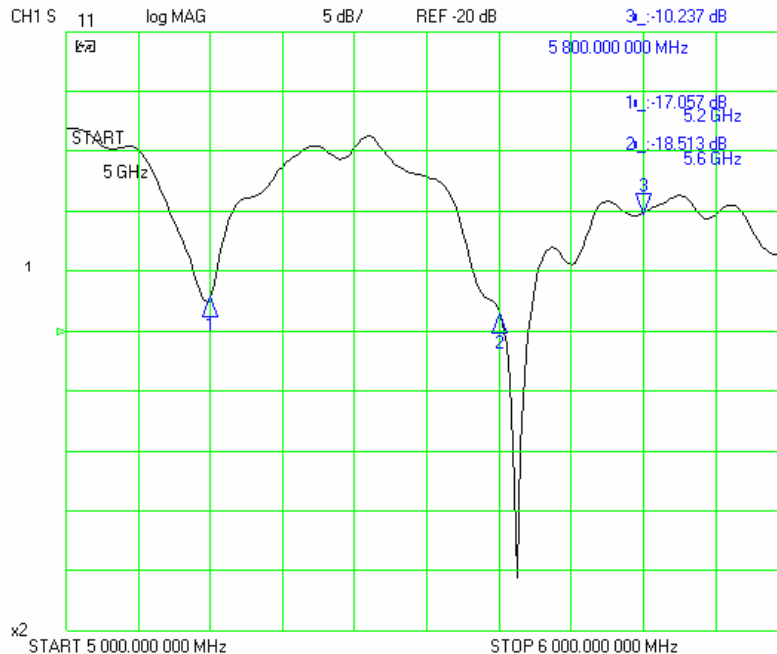

SWR

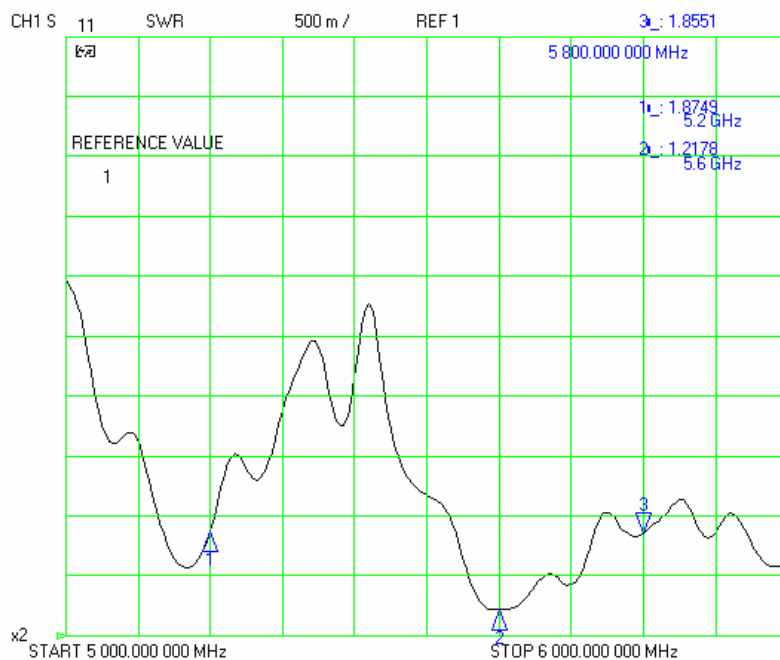

Smith Chart Dipole Impedance

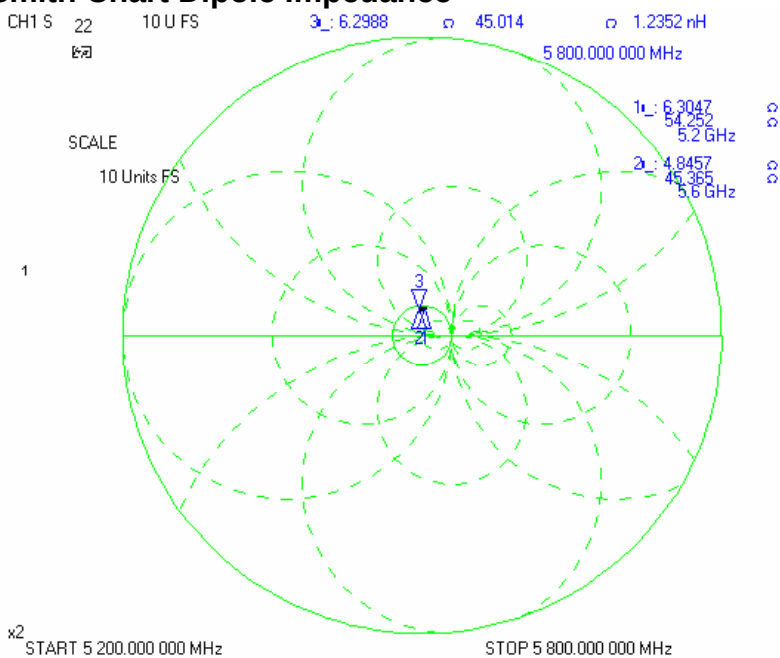

Test Equipment List

The test equipment used during Dipole Calibration, manufacturer, model number and, current calibration status are listed and located on the RF Exposure Lab, LLC system computer C:\Test Equipment\Calibration Equipment\Instrument List May 2007.

Appendix F – Phantom Calibration Data Sheets

NCL CALIBRATION LABORATORIES

Calibration File No.: RFE-273

CERTIFICATE OF CALIBRATION

It is certified that the equipment identified below has been calibrated in the
NCL CALIBRATION LABORATORIES by qualified personnel following recognized
procedures and using transfer standards traceable to National Standards.

Thickness of the UniPhantom is 2 mm $\pm$ 10%
Pinna thickness is 6 mm $\pm$ 10%

Resolution:	0.01 mm	Calibrated to:	0.0 mm
Stability:	OK	Accuracy:	< 0.1 mm

Calibrated By: Karen K. Feb 17/04.

NCL CALIBRATION LABORATORIES

51 SPECTRUM WAY
NEPEAN, ONTARIO
CANADA K2R 1E6

Division of APREL Lab.
TEL: (613) 820-4988
FAX: (613) 820-4161