



# RF EXPOSURE LAB, LLC

2867 Progress Place, Suite 4D • Escondido, CA 92029 • U.S.A.

TEL (760) 737-3131 • FAX (760) 737-9131

<http://www.rfexposurelab.com>

## CERTIFICATE OF COMPLIANCE SAR EVALUATION

LXE, Inc.  
125 Technology Parkway  
Norcross, GA 30092

Dates of Test: April 4 – 9, 2008  
Test Report Number: SAR.20080403

|                        |                                                                                                            |
|------------------------|------------------------------------------------------------------------------------------------------------|
| FCC ID:                | KDZLXE4831P                                                                                                |
| IC Certificate:        | 1995B-4831P                                                                                                |
| Model(s):              | MX7                                                                                                        |
| Summit WLAN:           | Model: SDC-CF10AG FCCID: TWG-SDCCF10AG                                                                     |
| Test Sample:           | Production Unit                                                                                            |
| Serial No.:            | MX708048360                                                                                                |
| Equipment Type:        | Wireless Computer                                                                                          |
| Classification:        | Portable Transmitter Next to Body                                                                          |
| TX Frequency Range:    | 2412 – 2462 MHz, 5180 – 5240 MHz, 5260 – 5320 MHz,<br>5745 – 5805 MHz                                      |
| Frequency Tolerance:   | ± 25 ppm                                                                                                   |
| Maximum RF Output:     | 2450 MHz (b) – 15.31 dBm, 2450 MHz (g) – 11.24 dBm,<br>5250 MHz – 12.90 dBm, 5800 MHz – 7.52 dBm Conducted |
| Signal Modulation:     | DSSS, OFDM                                                                                                 |
| Antenna Type (Length): | LXE Part Number: 161493-0001                                                                               |
| Battery:               | LXE Part Number: 159904-0001                                                                               |
| Application Type:      | Certification                                                                                              |
| FCC Rule Parts:        | Part 15C                                                                                                   |
| Industry Canada:       | RSS-102                                                                                                    |

This wireless mobile and/or portable device has been shown to be compliant for localized specific absorption rate (SAR) for uncontrolled environment/general exposure limits specified in ANSI/IEEE Std. C95.1-1999 and had been tested in accordance with the measurement procedures specified in IEEE 1528-2003, OET Bulletin 65 Supp. C, RSS-102 and Safety Code 6 (See test report).

I attest to the accuracy of the data. All measurements were performed by myself or were made under my supervision and are correct to the best of my knowledge and belief. I assume full responsibility for the completeness of these measurements and vouch for the qualifications of all persons taking them.

RF Exposure Lab, LLC certifies that no party to this application has been denied FCC benefits pursuant to Section 5301 of the Anti-Drug Abuse Act of 1988, 21 U.S.C. 853(a).

Jay M. Moulton  
Vice President



Certificate # 2387.01

## Table of Contents

|      |                                                          |     |
|------|----------------------------------------------------------|-----|
| 1.   | Introduction .....                                       | 3   |
|      | SAR Definition [5].....                                  | 3   |
| 2.   | SAR Measurement Setup .....                              | 4   |
|      | Robotic System .....                                     | 4   |
|      | System Hardware .....                                    | 4   |
|      | System Description .....                                 | 4   |
|      | E-Field Probe .....                                      | 5   |
| 3.   | Robot Specifications .....                               | 7   |
| 4.   | Probe and Dipole Calibration .....                       | 8   |
| 5.   | Phantom & Simulating Tissue Specifications.....          | 9   |
|      | SAM Phantom.....                                         | 9   |
|      | Brain & Muscle Simulating Mixture Characterization ..... | 9   |
|      | Device Holder .....                                      | 9   |
| 6.   | Definition of Reference Points.....                      | 10  |
|      | Ear Reference Point.....                                 | 10  |
|      | Device Reference Points .....                            | 10  |
| 7.   | Test Configuration Positions .....                       | 11  |
|      | Positioning for Cheek/Touch [5].....                     | 11  |
|      | Positioning for Ear / 15° Tilt [5].....                  | 12  |
|      | Body Worn Configurations .....                           | 13  |
| 8.   | ANSI/IEEE C95.1 – 1999 RF Exposure Limits [2].....       | 14  |
|      | Uncontrolled Environment.....                            | 14  |
|      | Controlled Environment .....                             | 14  |
| 9.   | Measurement Uncertainty .....                            | 15  |
| 10.  | System Validation .....                                  | 16  |
|      | Tissue Verification.....                                 | 16  |
|      | Test System Verification .....                           | 16  |
| 11.  | SAR Test Data Summary .....                              | 17  |
|      | Procedures Used To Establish Test Signal.....            | 17  |
|      | Device Test Condition .....                              | 17  |
|      | SAR Data Summary – 2450 MHz Body .....                   | 19  |
|      | SAR Data Summary – 5200 MHz Body .....                   | 20  |
|      | SAR Data Summary – 5800 MHz Body .....                   | 21  |
| 12.1 | Test Equipment List .....                                | 22  |
| 13.1 | Conclusion .....                                         | 23  |
| 14.1 | References.....                                          | 24  |
|      | Appendix A – System Validation Plots and Data .....      | 25  |
|      | Appendix B – SAR Test Data Plots.....                    | 36  |
|      | Appendix C – SAR Test Setup Photos .....                 | 80  |
|      | Appendix D – Probe Calibration Data Sheets.....          | 86  |
|      | Appendix E – Dipole Calibration Data Sheets .....        | 117 |
|      | Appendix F – Phantom Calibration Data Sheets .....       | 140 |

## 1. Introduction

This measurement report shows compliance of the LXE, Inc. Model MX7 FCC ID: KDZLXE4831P with FCC Part 2, 1093, ET Docket 93-62 Rules for mobile and portable devices and IC Certificate: 1995B-4831P with RSS102 & Safety Code 6. The FCC have adopted the guidelines for evaluating the environmental effects of radio frequency radiation in ET Docket 93-62 on August 6, 1996 to protect the public and workers from the potential hazards of RF emissions due to FCC regulated portable devices. [1], [6]

The test procedures, as described in ANSI C95.1 – 1999 Standard for Safety Levels with Respect to Human Exposure to Radio Frequency Electromagnetic Fields, 3 kHz to 300 GHz [2], ANSI C95.3 – 2002 Recommended Practice for the Measurement of Potentially Hazardous Electromagnetic Fields [3], FCC OET Bulletin 65 Supp. C – 2001 [4], IEEE Std.1528 – 2003 Recommended Practice [5], and Industry Canada Safety Code 6 Limits of Human Exposure to Radiofrequency Electromagnetic Fields in the Frequency Range from 3kHz to 300 GHz were employed.

## SAR Definition [5]

Specific Absorption Rate is defined as the time derivative (rate) of the incremental energy ( $dW$ ) absorbed by (dissipated in) an incremental mass ( $dm$ ) contained in a volume element ( $dV$ ) of a given density ( $\rho$ ).

$$SAR = \frac{d}{dt} \left( \frac{dW}{dm} \right) = \frac{d}{dt} \left( \frac{dW}{\rho dV} \right)$$

SAR is expressed in units of watts per kilogram (W/kg). SAR can be related to the electric field at a point by

$$SAR = \frac{\sigma |E|^2}{\rho}$$

where:

$\sigma$  = conductivity of the tissue (S/m)

$\rho$  = mass density of the tissue (kg/m<sup>3</sup>)

$E$  = rms electric field strength (V/m)

## 2. SAR Measurement Setup

### Robotic System

The measurements are conducted utilizing the ALSAS-10-U automated dosimetric assessment system. The ALSAS-10-U is designed and manufactured by Aprel Laboratories in Nepean, Ontario, Canada. The system utilizes a Robcomm 3 robot manufactured by ThermoCRS located in Michigan USA.

### System Hardware

The system consists of a six axis articulated arm, controller for precise probe positioning (0.05 mm repeatability), a power supply, a teach pendant for teaching area scans, near field probe, an IBM Pentium 4™ 2.66 GHz PC with Windows XP Pro™, and custom software developed to enable communications between the robot controller software and the host operating system.

An amplifier is located on the articulated arm, which is isolated from the custom designed end effector and robot arm. The end effector provides the mechanical touch detection functionality and probe connection interface. The amplifier is functionally validated within the manufacturer's site and calibrated at NCL Calibration Laboratories. A Data Acquisition Card (DAC) is used to collect the signal as detected by the isotropic e-field probe. The DAC manufacturer calibrates the DAC to NIST standards. A formal validation is executed using all mechanical and electronic components to prove conformity of the measurement platform as a whole.

### System Description

The ALSAS-10-U has been designed to measure devices within the compliance environment to meet all recognized standards. The system also conforms to standards, which are currently being developed by the scientific and manufacturing community.

The course scan resolution is defined by the operator and reflects the requirements of the standard to which the device is being tested. Precise measurements are made within the predefined course scan area and the values are logged.

The user predefines the sample rate for which the measurements are made so as to ensure that the full duty-cycle of a pulse modulation device is covered during the sample. The following algorithm is an example of the function used by the system for linearization of the output for the probe.

$$V_i = U_i + U_i^2 \bullet \frac{cf}{dcp_i}$$



The April E-Field probe is evaluated to establish the diode compression point.

A complex algorithm is then used to calculate the values within the measured points down to a resolution of 1mm. The data from this process is then used to provide the co-ordinates from which the cube scan is created for the determination of the 1 g and 10 g averages.

Cube scan averaging consists of a number of complex algorithms, which are used to calculate the one, and ten gram averages. The basis for the cube scan process is centered on the location where the maximum measured SAR value was found. When a secondary peak value is found which is within 60% of the initial peak value, the system will report this back to the operator who can then assess the need for further analysis of both the peak values prior to the one and ten-gram cube scan averaging process. The algorithm consists of 3D cubic Spline, and Lagrange extrapolation to the surface, which form the matrix for calculating the measurement output for the one and ten gram average values. The resolution for the physical scan integral is user defined with a final calculated resolution down to 1mm.

In-depth analysis for the differential of the physical scanning resolution for the cube scan analysis has been carried out, to identify the optimum setting for the probe positioning steps, and this has been determined at 8mm increments on the X, & Y planes. The reduction of the physical step increment increased the time taken for analysis but did not provide a better uncertainty or return on measured values.

The final output from the system provides data for the area scan measurements, physical and splined (1mm resolution) cube scan with physical and calculated values (1mm resolution).


The overall uncertainty for the methodology and algorithms the ALSAS-10-U used during the SAR calculation was evaluated using the data from IEEE 1528 f3 algorithm:

$$f_3(x, y, z) = A \frac{a^2}{\frac{a^2}{4} + x'^2 + y'^2} \left( e^{-\frac{2z}{a}} + \frac{a^2}{2(a + 2z)^2} \right)$$


The probe used during the measurement process has been assessed to provide values for diode compression. These values are calculated during the probe calibration exercise and are used in the mathematical calculations for the assessment of SAR.

## E-Field Probe

The E-field probe used by RF Exposure Lab, LLC, has been fully calibrated and assessed for isotropic, and boundary effect. The probe utilizes a triangular sensor arrangement as detailed in the diagram below right.



**Δ-BEAM**

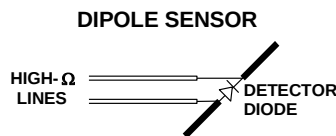

The SAR is assessed with the probe which moves at a default height of 5mm from the center of the diode, which is mounted to the sensor, to the phantom surface (Z height). The diagram above right shows how the center of the sensor is defined with the location of the diode placed at the center of the dipole. The 5mm default in the Z axis is the optimum height for assessing SAR where the boundary effect is at its least, with the probe located closest to the phantom surface (boundary).

The manufacturer specified precision of the robot is  $\pm 0.05$  mm and the precision of the APREL bottom detection device is  $\pm 0.1$  mm. These precisions are calibrated and tested in the manufacturing process of the bottom detection device. A constant distance is maintained because the surface of the phantom is dynamically detected for each point. The surface detection algorithm corrects the position of the robot so that the probe rests on the surface of the phantom. The probe is then moved to the measurement location 2.44 mm above the phantom surface resulting in the probe center location to be at 4.0 mm above the phantom surface. Therefore, the probe sensor will be at 4.0 mm above the phantom surface  $\pm 0.1$  mm for each SAR location for frequencies below 3 GHz. The probe is moved to the measurement location 1.44 mm above the phantom surface resulting in the probe center location to be at 2.0 mm above the phantom surface. Therefore, the probe sensor will be at 2.0 mm above the phantom surface  $\pm 0.1$  mm for each SAR location for frequencies above 3 GHz.

The probe boundary effect compensation cannot be disabled in the ALSAS-10U testing system. The probe tip will always be at least half a probe tip diameter from the phantom surface. For frequencies up to 3 GHz, the probe diameter is 5 mm. With the sensor offset set at 1.54 mm (default setting), the sensor to phantom gap will be 4.0 mm which is greater than half the probe tip diameter. For frequencies greater than 3 GHz, the probe diameter is 3 mm. With the sensor offset set at 0.56 mm (default setting), the sensor to phantom gap will be 3.0 mm which is greater than half the probe tip diameter.

The separation of the first 2 measurement points in the zoom scan is specified in the test setup software. For frequencies below 3 GHz, the user must specify a zoom scan resolution of less than 6 mm in the z-axis to have the first two measurements within 1 cm of the surface. The z-axis is set to 4 mm as shown on each of the data sheets in Appendix B. For frequencies above 3 GHz, the user must specify a zoom scan resolution of less than 3 mm in the z-axis to have the first two measurements within 5 mm of the surface. The z-axis is set to 2 mm as shown on each of the data sheets in Appendix B.

The zoom scan volume for devices  $\leq 3$  GHz with a cube scan of  $5 \times 5 \times 8$  yields a volume of  $32 \times 32 \times 28$  mm<sup>3</sup>. For devices  $> 3$  GHz and  $< 4.5$  GHz, the cube scan of  $9 \times 9 \times 9$  yields a volume of  $32 \times 32 \times 24$  mm<sup>3</sup>. For devices  $\geq 4.5$  GHz, the cube scan of  $7 \times 7 \times 12$  yields a volume of  $24 \times 24 \times 22$  mm<sup>3</sup>.

### 3. Robot Specifications

#### Specifications

|                |                                    |
|----------------|------------------------------------|
| Positioner:    | ThermoCRS, Robot Model: Robocomm 3 |
| Repeatability: | 0.05 mm                            |
| No. of axis:   | 6                                  |

#### Data Acquisition Card (DAC) System

##### Cell Controller

|                   |                 |
|-------------------|-----------------|
| Processor:        | Pentium 4™      |
| Clock Speed:      | 2.66 GHz        |
| Operating System: | Windows XP Pro™ |

##### Data Converter

|           |                                     |
|-----------|-------------------------------------|
| Features: | Signal Amplifier, End Effector, DAC |
| Software: | ALSAS 10-U Software                 |

##### E-Field Probe

|                |                                        |
|----------------|----------------------------------------|
| Model:         | Various See Probe Calibration Sheet    |
| Serial Number: | Various See Probe Calibration Sheet    |
| Construction:  | Triangular Core Touch Detection System |
| Frequency:     | 10MHz to 6GHz                          |

##### Phantom

|          |                                         |
|----------|-----------------------------------------|
| Phantom: | Uniphantom, Right Phantom, Left Phantom |
|----------|-----------------------------------------|



## **4. Probe and Dipole Calibration**

See Appendix D and E.

## 5. Phantom & Simulating Tissue Specifications

### SAM Phantom



The Aprel system utilizes three separate phantoms. Each phantom for SAR assessment testing is a low loss dielectric shell, with shape and dimensions derived from the anthropomorphic data of the 90<sup>th</sup> percentile adult male head dimensions as tabulated by the US Army. The SAM phantom shell is bisected along the mid sagittal plane into right and left halves. The perimeter sidewalls of each phantom half is extended to allow filling with liquid to a depth of 15 cm that is sufficient to minimize reflections from the upper surface [5]. See photos in Appendix C.

### Brain & Muscle Simulating Mixture Characterization

The brain and muscle mixtures consist of a glycol based chemical and saline solution. The mixture is calibrated to obtain proper dielectric constant (permittivity) and conductivity of the desired tissue. The head tissue dielectric parameters recommended by the IEEE SCC-34/SC-2 have been incorporated in the following tables. Other head and body tissue parameters that have not been specified in P1528 are derived from the issue dielectric parameters computed from the 4-Cole-Cole equations.

**Table 5.1 Typical Composition of Ingredients for Tissue**

| Ingredients         |        | Simulating Tissue |                 |                 |
|---------------------|--------|-------------------|-----------------|-----------------|
|                     |        | 2450 MHz Muscle   | 5200 MHz Muscle | 5800 MHz Muscle |
| Mixing Percentage   |        |                   |                 |                 |
| Water               |        | 73.20             | 58.85           | 59.00           |
| Sugar               |        | 0.00              | 41.00           | 40.60           |
| Salt                |        | 0.04              | 0.00            | 0.00            |
| HEC                 |        | 0.00              | 0.10            | 0.30            |
| Bactericide         |        | 0.00              | 0.05            | 0.10            |
| DGBE                |        | 26.70             | 0.00            | 0.00            |
| Dielectric Constant | Target | 52.70             | 48.96           | 48.25           |
| Conductivity (S/m)  | Target | 1.95              | 5.35            | 5.96            |

### Device Holder




In combination with the SAM phantom, the mounting device enables the rotation of the mounted transmitter in spherical coordinates whereby the rotation point is the ear opening. The devices can easily, accurately, and repeatably be positioned according to the FCC specifications. The device holder can be locked at different phantom locations (left head, right head, and uni-phantom).

## 6. Definition of Reference Points

### Ear Reference Point

Figure 6.2 shows the front, back and side views of the SAM Phantom. The point “M” is the reference point for the center of the mouth, “LE” is the left ear reference point (ERP), and “RE” is the right ERP. The ERPs are 15mm posterior to the entrance to the ear canal (EEC) along the B-M line (Back-Mouth), as shown in Figure 6.1. The plane passing through the two ear canals and M is defined as the Reference Plane. The line N-F (Neck-Front) is perpendicular to the reference plane and passing through the RE (or LE) is called the Reference Pivoting Line (see Figure 6.1). Line B-M is perpendicular to the N-F line. Both N-F and B-M lines are marked on the external phantom shell to facilitate handset positioning [5].

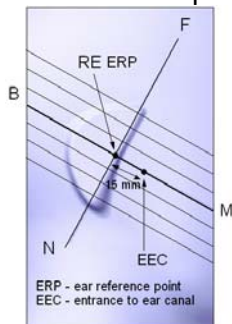


**Figure 6.1 Close-up side view of ERP's**



**Figure 6.2 Front, back and side view of SAM**

### Device Reference Points

Two imaginary lines on the device need to be established: the vertical centerline and the horizontal line. The test device is placed in a normal operating position with the “test device reference point” located along the “vertical centerline” on the front of the device aligned to the “ear reference point” (See Fig. 6.3). The “test device reference point” is then located at the same level as the center of the ear reference point. The test device is positioned so that the “vertical centerline” is bisecting the front surface of the device at it's top and bottom edges, positioning the “ear reference point” on the outer surface of both the left and right head phantoms on the ear reference point [5].

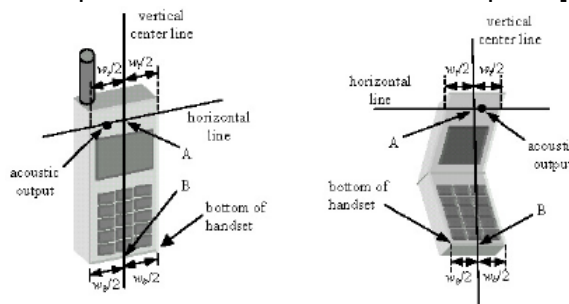


**Figure 6.3 Handset Vertical Center & Horizontal Line Reference Points**

## 7. Test Configuration Positions


### Positioning for Cheek/Touch [5]

1. Position the device close to the surface of the phantom such that point A is on the (virtual) extension of the line passing through points RE and LE on the phantom (see Figure 7.1), such that the plane defined by the vertical center line and the horizontal line of the device is approximately parallel to the sagittal plane of the phantom.

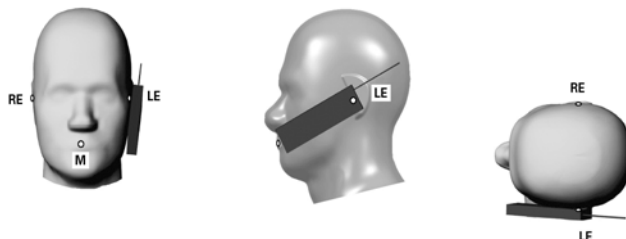

**Figure 7.1 Front, Side and Top View of Cheek/Touch Position**

2. Translate the device towards the phantom along the line passing through RE and LE until the device touches the ear.
3. While maintaining the device in this plane, rotate it around the LE-RE line until the vertical centerline is in the plane normal to MB-NF including the line MB (called the reference plane).
4. Rotate the device around the vertical centerline until the device (horizontal line) is symmetrical with respect to the line NF.
5. While maintaining the vertical centerline in the reference plane, keeping point A on the line passing through RE and LE and maintaining the device contact with the ear, rotate the device about the line NF until any point on the device is in contact with a phantom point below the ear (cheek). See Figure 7.2.




**Figure 7.2 Side view w/ relevant markings**

## Positioning for Ear / 15° Tilt [5]

With the test device aligned in the Cheek/Touch Position”:

1. While maintaining the orientation of the device, retracted the device parallel to the reference plane far enough to enable a rotation of the device by 15 degrees.
2. Rotate the device around the horizontal line by 15 degrees.
3. While maintaining the orientation of the device, move the device parallel to the reference plane until any part of the device touches the head. (In this position, point A is located on the line RE-LE). The tilted position is obtained when the contact is on the pinna. If the contact is at any location other than the pinna, the angle of the device shall be reduced. The tilted position is obtained when any part of the device is in contact with the ear as well as a second part of the device is in contact with the head (see Figure 7.3).

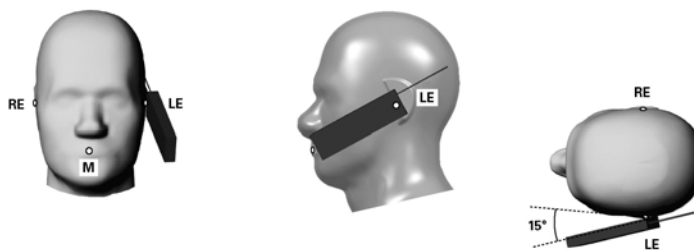

**Figure 7.3 Front, Side and Top View of Ear/15° Tilt Position**

## Body Worn Configurations

Body-worn operating configurations are tested with the accessories attached to the device and positioned against a flat phantom in a normal use configuration. A device with a headset output is tested with a headset connected to the device. Body dielectric parameters are used.

Accessories for Body-worn operation configurations are divided into two categories: those that do not contain metallic components and those that do contain metallic components. When multiple accessories that do not contain metallic components are supplied with the device, the device is tested with only the accessory that dictates the closest spacing to the body. Then, when multiple accessories that contain metallic components are supplied with the device, the device is tested with each accessory that contains a unique metallic component. If multiple accessories share an identical metallic component (i.e. the same metallic belt-clip used with different holsters with no other metallic components) only the accessory that dictates the closest spacing to the body is tested.

Body-worn accessories may not always be supplied or available as options for some devices intended to be authorized for body-worn use. In this case, a test configuration where a separation distance between the back of the device and the flat phantom is used. All test position spacings are documented.

Transmitters that are designed to operate in front of a person's face, as in push-to-talk configurations, are tested for SAR compliance with the front of the device positioned to face the flat phantom. For devices that are carried next to the body such as a shoulder, waist or chest-worn transmitters, SAR compliance is tested with the accessory(ies), including headsets and microphones, attached to the device and positioned against a flat phantom in a normal use configuration.

In all cases SAR measurements are performed to investigate the worst-case positioning. Worst-case positioning is then documented and used to perform Body SAR testing.

In order for users to be aware of the body-worn operating requirements for meeting RF exposure compliance, operating instructions and cautions statements are included in the user's manual.

## 8. ANSI/IEEE C95.1 – 1999 RF Exposure Limits [2]

### Uncontrolled Environment

Uncontrolled Environments are defined as locations where there is the exposure of individuals who have no knowledge or control of their exposure. The general population/uncontrolled exposure limits are applicable to situations in which the general public may be exposed or in which persons who are exposed as a consequence of their employment may not be made fully aware of the potential for exposure or cannot exercise control over their exposure. Members of the general public would come under this category when exposure is not employment-related; for example, in the case of a wireless transmitter that exposes persons in its vicinity.

### Controlled Environment

Controlled Environments are defined as locations where there is exposure that may be incurred by persons who are aware of the potential for exposure, (i.e. as a result of employment or occupation). In general, occupational/controlled exposure limits are applicable to situations in which persons are exposed as a consequence of their employment, who have been made fully aware of the potential for exposure and can exercise control over their exposure. This exposure category is also applicable when the exposure is of a transient nature due to incidental passage through a location where the exposure levels may be higher than the general population/uncontrolled limits, but the exposed person is fully aware of the potential for exposure and can exercise control over his or her exposure by leaving the area or by some other appropriate means.

**Table 8.1 Human Exposure Limits**

|                                                              | UNCONTROLLED ENVIRONMENT<br>General Population<br>(W/kg) or (mW/g) | CONTROLLED ENVIROMENT<br>Professional Population<br>(W/kg) or (mW/g) |
|--------------------------------------------------------------|--------------------------------------------------------------------|----------------------------------------------------------------------|
| SPATIAL PEAK SAR <sup>1</sup><br>Brain                       | 1.60                                                               | 8.00                                                                 |
| SPATIAL AVERAGE SAR <sup>2</sup><br>Whole Body               | 0.08                                                               | 0.40                                                                 |
| SPATIAL PEAK SAR <sup>3</sup><br>Hands, Feet, Ankles, Wrists | 4.00                                                               | 20.00                                                                |

<sup>1</sup> The Spatial Peak value of the SAR averaged over any 1 gram of tissue (defined as a tissue volume in the shape of a cube) and over the appropriate averaging time.

<sup>2</sup> The Spatial Average value of the SAR averaged over the whole body.

<sup>3</sup> The Spatial Peak value of the SAR averaged over any 10 grams of tissue (defined as a tissue volume in the shape of a cube) and over the appropriate averaging time.

## 9. Measurement Uncertainty

### Exposure Assessment Measurement Uncertainty

| Source of Uncertainty                            | Tolerance Value | Probability Distribution | Divisor | $c_i^1$<br>(1-g) | $c_i^1$<br>(10-g) | Standard Uncertainty<br>(1-g) % | Standard Uncertainty<br>(10-g) % |
|--------------------------------------------------|-----------------|--------------------------|---------|------------------|-------------------|---------------------------------|----------------------------------|
| Measurement System                               |                 |                          |         |                  |                   |                                 |                                  |
| Probe Calibration                                | 3.5             | normal                   | 1       | 1                | 1                 | 3.5                             | 3.5                              |
| Axial Isotropy                                   | 3.7             | rectangular              | •3      | $(1-cp)^{1/2}$   | $(1-cp)^{1/2}$    | 1.5                             | 1.5                              |
| Hemispherical Isotropy                           | 10.9            | rectangular              | •3      | •cp              | •cp               | 4.4                             | 4.4                              |
| Boundary Effect                                  | 1.0             | rectangular              | •3      | 1                | 1                 | 0.6                             | 0.6                              |
| Linearity                                        | 4.7             | rectangular              | •3      | 1                | 1                 | 2.7                             | 2.7                              |
| Detection Limit                                  | 1.0             | rectangular              | •3      | 1                | 1                 | 0.6                             | 0.6                              |
| Readout Electronics                              | 1.0             | normal                   | 1       | 1                | 1                 | 1.0                             | 1.0                              |
| Response Time                                    | 0.8             | rectangular              | •3      | 1                | 1                 | 0.5                             | 0.5                              |
| Integration Time                                 | 1.7             | rectangular              | •3      | 1                | 1                 | 1.0                             | 1.0                              |
| RF Ambient Condition                             | 3.0             | rectangular              | •3      | 1                | 1                 | 1.7                             | 1.7                              |
| Probe Positioner Mech.                           | 0.4             | rectangular              | •3      | 1                | 1                 | 0.2                             | 0.2                              |
| Restriction                                      |                 |                          |         |                  |                   |                                 |                                  |
| Probe Positioning with respect to Phantom Shell  | 2.9             | rectangular              | •3      | 1                | 1                 | 1.7                             | 1.7                              |
| Extrapolation and Integration                    | 3.7             | rectangular              | •3      | 1                | 1                 | 2.1                             | 2.1                              |
| Test Sample Positioning                          | 4.0             | normal                   | 1       | 1                | 1                 | 4.0                             | 4.0                              |
| Device Holder Uncertainty                        | 2.0             | normal                   | 1       | 1                | 1                 | 2.0                             | 2.0                              |
| Drift of Output Power                            | 4.2             | rectangular              | •3      | 1                | 1                 | 2.4                             | 2.4                              |
| Phantom and Setup                                |                 |                          |         |                  |                   |                                 |                                  |
| Phantom Uncertainty(shape & thickness tolerance) | 3.4             | rectangular              | •3      | 1                | 1                 | 2.0                             | 2.0                              |
| Liquid Conductivity(target)                      | 5.0             | rectangular              | •3      | 0.7              | 0.5               | 2.0                             | 1.4                              |
| Liquid Conductivity(meas.)                       | 0.5             | normal                   | 1       | 0.7              | 0.5               | 0.4                             | 0.3                              |
| Liquid Permittivity(target)                      | 5.0             | rectangular              | •3      | 0.6              | 0.5               | 1.7                             | 1.4                              |
| Liquid Permittivity(meas.)                       | 1.0             | normal                   | 1       | 0.6              | 0.5               | 0.6                             | 0.5                              |
| Combined Uncertainty                             |                 | RSS                      |         |                  |                   | 9.6                             | 9.4                              |
| Combined Uncertainty (coverage factor=2)         |                 | Normal (k=2)             |         |                  |                   | 19.1                            | 18.8                             |

## 10. System Validation

### Tissue Verification

**Table 10.1 Measured Tissue Parameters**

|                                 |      | 2450 MHz Body |          | 5250 MHz Body |          | 5800 MHz Body |          |
|---------------------------------|------|---------------|----------|---------------|----------|---------------|----------|
| Date(s)                         |      | Apr. 7, 2008  |          | Apr. 8, 2008  |          | Apr. 9, 2008  |          |
| Liquid Temperature (°C)         | 20.0 | Target        | Measured | Target        | Measured | Target        | Measured |
| Dielectric Constant: $\epsilon$ |      | 52.59         | 53.36    | 49.19         | 48.93    | 48.53         | 47.33    |
| Conductivity: $\sigma$          |      | 1.92          | 1.96     | 5.40          | 5.20     | 5.95          | 5.77     |

See Appendix A for data printout.


### Test System Verification

Prior to assessment, the system is verified to the  $\pm 10\%$  of the specifications at the test frequency by using the system kit. Power is extrapolated to 1 watt. (Graphic Plots Attached)

**Table 10.2 System Dipole Validation Target & Measured**

|             | Test Frequency | Targeted SAR <sub>1g</sub> (W/kg) | Measure SAR <sub>1g</sub> (W/kg) | Deviation (%) |
|-------------|----------------|-----------------------------------|----------------------------------|---------------|
| 07-Apr-2008 | 2450 MHz       | 53.55                             | 54.40                            | + 1.59        |
| 08-Apr-2008 | 5250 MHz       | 62.98                             | 62.27                            | - 1.13        |
| 09-Apr-2008 | 5785 MHz       | 58.92                             | 56.09                            | - 4.80        |

See Appendix A for data plots.

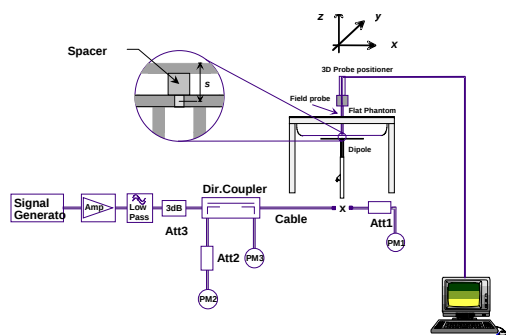

**Figure 10.1 Dipole Validation Test Setup**

## **11. SAR Test Data Summary**

### **See Measurement Result Data Pages**

See Appendix B for SAR Test Data Plots.  
See Appendix C for SAR Test Setup Photos.

### **Procedures Used To Establish Test Signal**

The device was placed into simulated transmit mode using the manufacturer's test codes. Such test signals offer a consistent means for testing SAR and are recommended for evaluating SAR. When test modes are not available or inappropriate for testing a device, the actual transmission is activated through a base station simulator or similar equipment. See data pages for actual procedure used in measurement.

### **Device Test Condition**

The device is battery operated. Each SAR measurement was taken with a fully charged battery. In order to verify that the device was tested at full power, conducted output power measurements were performed before and after each SAR measurement to confirm the output power unless otherwise noted. If a conducted power deviation of more than 5% occurred, the test was repeated.

The testing was conducted on the back of the device due to the normal position of the device. The conducted power was measured before the start of testing. The power was not measured before and after each test due to the necessity of disassembling the device to take the measurement.

| 802.11b         |         |           |         |       |  | 802.11a 5.8 GHz |         |           |         |       |
|-----------------|---------|-----------|---------|-------|--|-----------------|---------|-----------|---------|-------|
| Freq            | Channel | Data Rate | Antenna | Power |  | Freq            | Channel | Data Rate | Antenna | Power |
| 2412            | 1       | 1         | Main    | 15.31 |  | 5.745           | 149     | 6         | Main    | 6.48  |
| 2437            | 6       | 1         | Main    | 15.27 |  | 5.765           | 153     | 6         | Main    | 6.52  |
| 2462            | 11      | 1         | Main    | 14.56 |  | 5.785           | 157     | 6         | Main    | 6.05  |
| 2412            | 1       | 1         | Aux     | 14.85 |  | 5.805           | 161     | 6         | Main    | 6.63  |
| 2437            | 6       | 1         | Aux     | 14.90 |  | 5.745           | 149     | 6         | Aux     | 7.52  |
| 2462            | 11      | 1         | Aux     | 15.11 |  | 5.765           | 153     | 6         | Aux     | 6.20  |
| 2412            | 1       | 2         | Main    | 14.73 |  | 5.785           | 157     | 6         | Aux     | 5.51  |
| 2412            | 1       | 5.5       | Main    | 14.60 |  | 5.805           | 161     | 6         | Aux     | 6.42  |
| 2412            | 1       | 11        | Main    | 7.36  |  | 5.765           | 153     | 9         | Main    | 6.23  |
|                 |         |           |         |       |  | 5.765           | 153     | 12        | Main    | 5.57  |
| 802.11g         |         |           |         |       |  | 5.765           | 153     | 18        | Main    | 5.61  |
| Freq            | Channel | Data Rate | Antenna | Power |  | 5.765           | 153     | 24        | Main    | 5.49  |
| 2412            | 1       | 6         | Main    | 11.21 |  | 5.765           | 153     | 36        | Main    | 3.92  |
| 2437            | 6       | 6         | Main    | 11.20 |  | 5.765           | 153     | 48        | Main    | 2.67  |
| 2462            | 11      | 6         | Main    | 11.08 |  | 5.765           | 153     | 54        | Main    | 2.73  |
| 2412            | 1       | 6         | Aux     | 11.05 |  |                 |         |           |         |       |
| 2437            | 6       | 6         | Aux     | 11.12 |  |                 |         |           |         |       |
| 2462            | 11      | 6         | Aux     | 11.24 |  |                 |         |           |         |       |
| 2462            | 11      | 9         | Main    | 9.96  |  |                 |         |           |         |       |
| 2462            | 11      | 12        | Main    | 11.08 |  |                 |         |           |         |       |
| 2462            | 11      | 18        | Main    | 8.85  |  |                 |         |           |         |       |
| 2462            | 11      | 24        | Main    | 10.36 |  |                 |         |           |         |       |
| 2462            | 11      | 36        | Main    | 5.30  |  |                 |         |           |         |       |
| 2462            | 11      | 48        | Main    | 8.70  |  |                 |         |           |         |       |
| 2462            | 11      | 54        | Main    | 9.70  |  |                 |         |           |         |       |
|                 |         |           |         |       |  |                 |         |           |         |       |
| 802.11a 5.2 GHz |         |           |         |       |  |                 |         |           |         |       |
| Freq            | Channel | Data Rate | Antenna | Power |  |                 |         |           |         |       |
| 5.18            | 36      | 6         | Main    | 11.48 |  |                 |         |           |         |       |
| 5.20            | 40      | 6         | Main    | 10.44 |  |                 |         |           |         |       |
| 5.22            | 44      | 6         | Main    | 10.12 |  |                 |         |           |         |       |
| 5.24            | 48      | 6         | Main    | 11.24 |  |                 |         |           |         |       |
| 5.18            | 36      | 6         | Aux     | 12.87 |  |                 |         |           |         |       |
| 5.20            | 40      | 6         | Aux     | 12.80 |  |                 |         |           |         |       |
| 5.22            | 44      | 6         | Aux     | 12.83 |  |                 |         |           |         |       |
| 5.24            | 48      | 6         | Aux     | 12.90 |  |                 |         |           |         |       |
| 5.24            | 48      | 9         | Main    | 10.85 |  |                 |         |           |         |       |
| 5.24            | 48      | 12        | Main    | 12.27 |  |                 |         |           |         |       |
| 5.24            | 48      | 18        | Main    | 12.25 |  |                 |         |           |         |       |
| 5.24            | 48      | 24        | Main    | 11.81 |  |                 |         |           |         |       |
| 5.24            | 48      | 36        | Main    | 7.29  |  |                 |         |           |         |       |
| 5.24            | 48      | 48        | Main    | 4.78  |  |                 |         |           |         |       |
| 5.24            | 48      | 54        | Main    | 4.57  |  |                 |         |           |         |       |

## Conduct Power Measurements

## SAR Data Summary – 2450 MHz Body

| MEASUREMENT RESULTS |      |         |           |     |            |           |          |               |
|---------------------|------|---------|-----------|-----|------------|-----------|----------|---------------|
| Position            | Band | Antenna | Frequency |     | Modulation | End Power | Battery  | SAR<br>(W/kg) |
|                     |      |         | MHz       | Ch. |            | (dBm)     |          |               |
| Touch               | b    | Main    | 2412      | 1   | DSSS       | 15.31     | Standard | 0.147         |
|                     |      |         | 2437      | 6   | DSSS       | 15.27     | Standard | 0.130         |
|                     |      |         | 2462      | 11  | DSSS       | 14.56     | Standard | 0.103         |
|                     |      | Aux     | 2412      | 1   | DSSS       | 14.85     | Standard | 0.186         |
|                     |      |         | 2437      | 6   | DSSS       | 14.90     | Standard | 0.173         |
|                     |      |         | 2462      | 11  | DSSS       | 15.11     | Standard | 0.129         |
|                     | g    | Main    | 2412      | 1   | OFDM       | 11.21     | Standard | 0.101         |
|                     |      |         | 2437      | 6   | OFDM       | 11.20     | Standard | 0.090         |
|                     |      |         | 2462      | 11  | OFDM       | 11.08     | Standard | 0.080         |
|                     |      | Aux     | 2412      | 1   | OFDM       | 11.05     | Standard | 0.128         |
|                     |      |         | 2437      | 6   | OFDM       | 11.12     | Standard | 0.097         |
|                     |      |         | 2462      | 11  | OFDM       | 11.24     | Standard | 0.089         |

**Muscle**  
**1.6 W/kg (mW/g)**  
averaged over 1 gram

1. Battery is fully charged for all tests.

Power Measured

☒ Conducted

☐ ERP

☐ EIRP

2. SAR Measurement

Phantom Configuration

☐ Left Head

☒ Uniphantom

☐ Right Head

SAR Configuration

☐ Head

☒ Body

3. Test Signal Call Mode

☒ Test Code

☐ Base Station Simulator

4. Test Configuration

☐ With Belt Clip

☐ Without Belt Clip ☒ N/A



Jay M. Moulton  
Vice President

## SAR Data Summary – 5200 MHz Body

| MEASUREMENT RESULTS |       |         |           |     |            |                                                   |          |            |
|---------------------|-------|---------|-----------|-----|------------|---------------------------------------------------|----------|------------|
| Position            | Band  | Antenna | Frequency |     | Modulation | End Power                                         | Battery  | SAR (W/kg) |
|                     |       |         | MHz       | Ch. |            | (dBm)                                             |          |            |
| Touch               | Lower | Main    | 5180      | 36  | OFDM       | 11.48                                             | Standard | 0.225      |
|                     |       |         | 5240      | 48  | OFDM       | 11.24                                             | Standard | 0.225      |
|                     |       | Aux     | 5180      | 36  | OFDM       | 12.87                                             | Standard | 0.109      |
|                     |       |         | 5240      | 48  | OFDM       | 12.90                                             | Standard | 0.111      |
|                     |       |         |           |     |            | Muscle<br>1.6 W/kg (mW/g)<br>averaged over 1 gram |          |            |

- Battery is fully charged for all tests.  
Power Measured ☒ Conducted ☐ ERP ☐ EIRP
- SAR Measurement  
Phantom Configuration ☐ Left Head ☒ Uniphantom ☐ Right Head  
SAR Configuration ☐ Head ☒ Body
- Test Signal Call Mode ☒ Test Code ☐ Base Station Simulator
- Test Configuration ☐ With Belt Clip ☐ Without Belt Clip ☒ N/A



Jay M. Moulton  
Vice President

## SAR Data Summary – 5800 MHz Body

| MEASUREMENT RESULTS |      |         |           |     |            |                                                   |          |            |
|---------------------|------|---------|-----------|-----|------------|---------------------------------------------------|----------|------------|
| Position            | Band | Antenna | Frequency |     | Modulation | End Power                                         | Battery  | SAR (W/kg) |
|                     |      |         | MHz       | Ch. |            | (dBm)                                             |          |            |
| Touch               | A3   | Main    | 5745      | 149 | OFDM       | 6.48                                              | Standard | 0.132      |
|                     |      |         | 5805      | 161 | OFDM       | 6.63                                              | Standard | 0.120      |
|                     |      | Aux     | 5745      | 149 | OFDM       | 7.52                                              | Standard | 0.109      |
|                     |      |         | 5805      | 161 | OFDM       | 6.42                                              | Standard | 0.139      |
|                     |      |         |           |     |            | Muscle<br>1.6 W/kg (mW/g)<br>averaged over 1 gram |          |            |

- Battery is fully charged for all tests.  
Power Measured ☒ Conducted ☐ ERP ☐ EIRP
- SAR Measurement  
Phantom Configuration ☐ Left Head ☒ Uniphantom ☐ Right Head  
SAR Configuration ☐ Head ☒ Body
- Test Signal Call Mode ☒ Test Code ☐ Base Station Simulator
- Test Configuration ☐ With Belt Clip ☐ Without Belt Clip ☒ N/A



Jay M. Moulton  
Vice President

## 12.1 Test Equipment List

Table 12.1 Equipment Specifications

| Type                                       | Calibration Due Date | Serial Number   |
|--------------------------------------------|----------------------|-----------------|
| ThermoCRS Robot                            | N/A                  | RAF0338198      |
| ThermoCRS Controller                       | N/A                  | RCF0338224      |
| ThermoCRS Teach Pendant (Joystick)         | N/A                  | STP0334405      |
| IBM Computer, 2.66 MHz P4                  | N/A                  | 8189D8U KCPR08N |
| Aprel E-Field Probe ALS-E020               | 12/03/2008           | RFE-217         |
| Aprel E-Field Probe ALS-E030               | 04/29/2008           | AL-E3P1         |
| Aprel Dummy Probe                          | N/A                  | 023             |
| Aprel Left Phantom                         | N/A                  | RFE-267         |
| Aprel Right Phantom                        | N/A                  | RFE-268         |
| Aprel UniPhantom                           | N/A                  | RFE-273         |
| Aprel Validation Dipole ALS-D-450-S-2      | 04/30/2009           | RFE-362         |
| Aprel Validation Dipole ALS-D-835-S-2      | 02/22/2010           | RFE-274         |
| Aprel Validation Dipole ALS-D-1900-S-2     | 02/21/2010           | RFE-277         |
| Aprel Validation Dipole ALS-D-2450-S-2     | 02/20/2010           | RFE-278         |
| Aprel Validation Dipole ALS-D-BB-S-2       | 05/23/2009           | 5258-235-00801  |
| Agilent (HP) 437B Power Meter              | 12/03/2008           | 3125U08837      |
| Agilent (HP) 8481B Power Sensor            | 12/03/2008           | 3318A05384      |
| Advantest R3261A Spectrum Analyzer         | 12/03/2008           | 31720068        |
| Agilent (HP) 8350B Signal Generator        | 01/28/2009           | 2749A10226      |
| Agilent (HP) 83525A RF Plug-In             | 01/28/2009           | 2647A01172      |
| Agilent (HP) 8753C Vector Network Analyzer | 01/28/2009           | 3135A01724      |
| Agilent (HP) 85047A S-Parameter Test Set   | 01/28/2009           | 2904A00595      |
| Aprel Dielectric Probe Assembly            | N/A                  | 0011            |
| Brain Equivalent Matter (450 MHz)          | N/A                  | N/A             |
| Brain Equivalent Matter (835 MHz)          | N/A                  | N/A             |
| Brain Equivalent Matter (1900 MHz)         | N/A                  | N/A             |
| Brain Equivalent Matter (2450 MHz)         | N/A                  | N/A             |
| Muscle Equivalent Matter (450 MHz)         | N/A                  | N/A             |
| Muscle Equivalent Matter (835 MHz)         | N/A                  | N/A             |
| Muscle Equivalent Matter (1900 MHz)        | N/A                  | N/A             |
| Muscle Equivalent Matter (2450 MHz)        | N/A                  | N/A             |
| Muscle Equivalent Matter (5200 MHz)        | N/A                  | N/A             |
| Muscle Equivalent Matter (5800 MHz)        | N/A                  | N/A             |

## 13.1 Conclusion

The SAR measurement indicates that the EUT complies with the RF radiation exposure limits of the FCC. These measurements are taken to simulate the RF effects exposure under worst-case conditions. Precise laboratory measures were taken to assure repeatability of the tests. The tested device complies with the requirements in respect to all parameters subject to the test. The test results and statements relate only to the item(s) tested.

Please note that the absorption and distribution of electromagnetic energy in the body is a very complex phenomena that depends on the mass, shape, and size of the body; the orientation of the body with respect to the field vectors; and, the electrical properties of both the body and the environment. Other variables that may play a substantial role in possible biological effects are those that characterize the environment (e.g. ambient temperature, air velocity, relative humidity, and body insulation) and those that characterize the individual (e.g. age, gender, activity level, debilitation, or disease). Because innumerable factors may interact to determine the specific biological outcome of an exposure to electromagnetic fields, any protection guide shall consider maximal amplification of biological effects as a result of field-body interactions, environmental conditions, and physiological variables. [3]

## 14.1 References

- [1] Federal Communications Commission, ET Docket 93-62, Guidelines for Evaluating the Environmental Effects of Radio Frequency Radiation, August 1996
- [2] ANSI/IEEE C95.1 – 1999, American National Standard Safety Levels with respect to Human Exposure to Radio Frequency Electromagnetic Fields, 300kHz to 100GHz, New York: IEEE, 1992.
- [3] ANSI/IEEE C95.3 – 2002, IEEE Recommended Practice for the Measurement of Potentially Hazardous Electromagnetic Fields – RF and Microwave, New York: IEEE, 1992.
- [4] Federal Communications Commission, OET Bulletin 65 (Edition 97-01), Supplement C (Edition 01-01), Evaluating Compliance with FCC Guidelines for Human Exposure to Radio Frequency Electromagnetic Fields, July 2001.
- [5] IEEE Standard 1528 – 2003, IEEE Recommended Practice for Determining the Peak-Spatial Average Specific Absorption Rate (SAR) in the Human Head from Wireless Communication Devices: Measurement Techniques, October 2003.
- [6] Industry Canada, RSS – 102e, Radio Frequency Exposure Compliance of Radiocommunication Apparatus (All Frequency Bands), November 2005.
- [7] Industry Canada, Safety Code 6, Limits of Human Exposure to Radiofrequency Electromagnetic Fields in the Frequency Range from 3kHz to 300 GHz, 1999.

## Appendix A – System Validation Plots and Data

\*\*\*\*\*

Test Result for UIM Dielectric Parameter

Mon 07/Apr/2008 07:10:38

Freq Frequency(GHz)

FCC\_eH FCC Bulletin 65 Supplement C ( June 2001) Limits for Head Epsilon

FCC\_sH FCC Bulletin 65 Supplement C (June 2001) Limits for Head Sigma

FCC\_eB FCC Limits for Body Epsilon

FCC\_sB FCC Limits for Body Sigma

Test\_e Epsilon of UIM

Test\_s Sigma of UIM

\*\*\*\*\*

| Freq   | FCC_eB | FCC_sB | Test_e | Test_s |
|--------|--------|--------|--------|--------|
| 2.4200 | 52.74  | 1.92   | 53.42  | 1.91   |
| 2.4300 | 52.73  | 1.93   | 53.42  | 1.94   |
| 2.4400 | 52.71  | 1.94   | 53.38  | 1.95   |
| 2.4500 | 52.70  | 1.95   | 53.36  | 1.96   |
| 2.4600 | 52.69  | 1.96   | 53.28  | 1.98   |
| 2.4700 | 52.67  | 1.98   | 53.27  | 1.99   |
| 2.4800 | 52.66  | 1.99   | 53.19  | 2.00   |

\*\*\*\*\*

Test Result for UIM Dielectric Parameter

Tue 08/Apr/2008 07:05:58

Freq Frequency(GHz)

FCC\_eH FCC Bulletin 65 Supplement C ( June 2001) Limits for Head Epsilon

FCC\_sH FCC Bulletin 65 Supplement C (June 2001) Limits for Head Sigma

FCC\_eB FCC Limits for Body Epsilon

FCC\_sB FCC Limits for Body Sigma

Test\_e Epsilon of UIM

Test\_s Sigma of UIM

\*\*\*\*\*

| Freq   | FCC_eB | FCC_sB | Test_e | Test_s |
|--------|--------|--------|--------|--------|
| 5.2200 | 48.99  | 5.32   | 49.09  | 5.13   |
| 5.2300 | 48.97  | 5.33   | 49.03  | 5.14   |
| 5.2400 | 48.96  | 5.35   | 48.97  | 5.18   |
| 5.2500 | 48.95  | 5.36   | 48.93  | 5.20   |
| 5.2600 | 48.93  | 5.37   | 48.88  | 5.22   |
| 5.2700 | 48.92  | 5.38   | 48.87  | 5.25   |
| 5.2800 | 48.91  | 5.39   | 48.86  | 5.27   |

\*\*\*\*\*

## Test Result for UIM Dielectric Parameter

Wed 09/Apr/2008 07:07:41

Freq Frequency(GHz)

FCC\_eH FCC Bulletin 65 Supplement C ( June 2001) Limits for Head Epsilon

FCC\_sH FCC Bulletin 65 Supplement C (June 2001) Limits for Head Sigma

FCC\_eB FCC Limits for Body Epsilon

FCC\_sB FCC Limits for Body Sigma

Test\_e Epsilon of UIM

Test\_s Sigma of UIM

\*\*\*\*\*

| Freq   | FCC_eB | FCC_sB | Test_e | Test_s |
|--------|--------|--------|--------|--------|
| 5.7550 | 48.26  | 5.95   | 47.49  | 5.72   |
| 5.7650 | 48.25  | 5.96   | 47.41  | 5.74   |
| 5.7750 | 48.23  | 5.97   | 47.36  | 5.75   |
| 5.7850 | 48.22  | 5.98   | 47.33  | 5.77   |
| 5.7950 | 48.21  | 5.99   | 47.30  | 5.79   |
| 5.8050 | 48.19  | 6.01   | 47.27  | 5.80   |
| 5.8150 | 48.18  | 6.02   | 47.23  | 5.83   |

**SAR Test Report**

By Operator : Jay  
Measurement Date : 07-Apr-2008  
Starting Time : 07-Apr-2008 07:12:56 AM  
End Time : 07-Apr-2008 07:26:02 AM  
Scanning Time : 786 secs

**Product Data**

Device Name : Validation  
Serial No. : 2450  
Type : Dipole  
Model : ALS-D-2450-S-2  
Frequency : 2450.00 MHz  
Max. Transmit Pwr : 0.1 W  
Drift Time : 0 min(s)  
Length : 51.5 mm  
Width : 3.6 mm  
Depth : 30.4 mm  
Antenna Type : Internal  
Orientation : Touch  
Power Drift-Start : 6.381 W/kg  
Power Drift-Finish: 6.404 W/kg  
Power Drift (%) : 0.355

**Phantom Data**

Name : APREL-Uni  
Type : Uni-Phantom  
Size (mm) : 280 x 280 x 200  
Serial No. : System Default  
Location : Center  
Description : Uni-Phantom

**Tissue Data**

Type : BODY  
Serial No. : 2450  
Frequency : 2450.00 MHz  
Last Calib. Date : 07-Apr-2008  
Temperature : 20.00 °C  
Ambient Temp. : 23.00 °C  
Humidity : 45.00 RH%  
Epsilon : 53.36 F/m  
Sigma : 1.96 S/m  
Density : 1000.00 kg/cu. m

**Probe Data**


Name : Probe 217 - RFEL  
Model : E020  
Type : E-Field Triangle  
Serial No. : 217  
Last Calib. Date : 03-Dec-2007  
Frequency : 2450.00 MHz  
Duty Cycle Factor: 1  
Conversion Factor: 3.61  
Probe Sensitivity: 1.20 1.20 1.20  $\mu\text{V}/(\text{V/m})^2$   
Compression Point: 95.00 mV  
Offset : 1.56 mm

**Measurement Data**

Crest Factor : 1  
 Scan Type : Complete  
 Tissue Temp. : 20.00 °C  
 Ambient Temp. : 23.00 °C  
 Set-up Date : 07-Apr-2008  
 Set-up Time : 7:40:13 AM  
 Area Scan : 5x5x1 : Measurement x=10mm, y=10mm, z=4mm  
 Zoom Scan : 5x5x8 : Measurement x=8mm, y=8mm, z=4mm


**Other Data**

DUT Position : Touch  
 Separation : 10  
 Channel : Mid

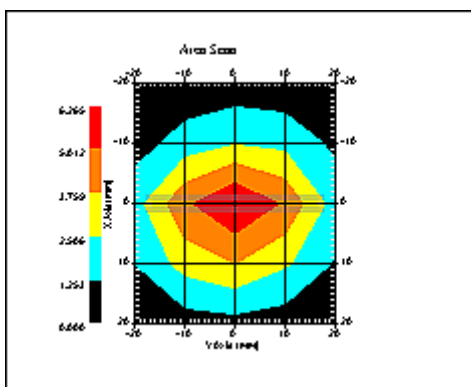

1 gram SAR value : 5.440 W/kg  
 10 gram SAR value : 2.476 W/kg  
 Area Scan Peak SAR : 6.265 W/kg  
 Zoom Scan Peak SAR : 11.190 W/kg

**SAR-Z Axis**  
at Hotspot x:0.24 y:-0.18

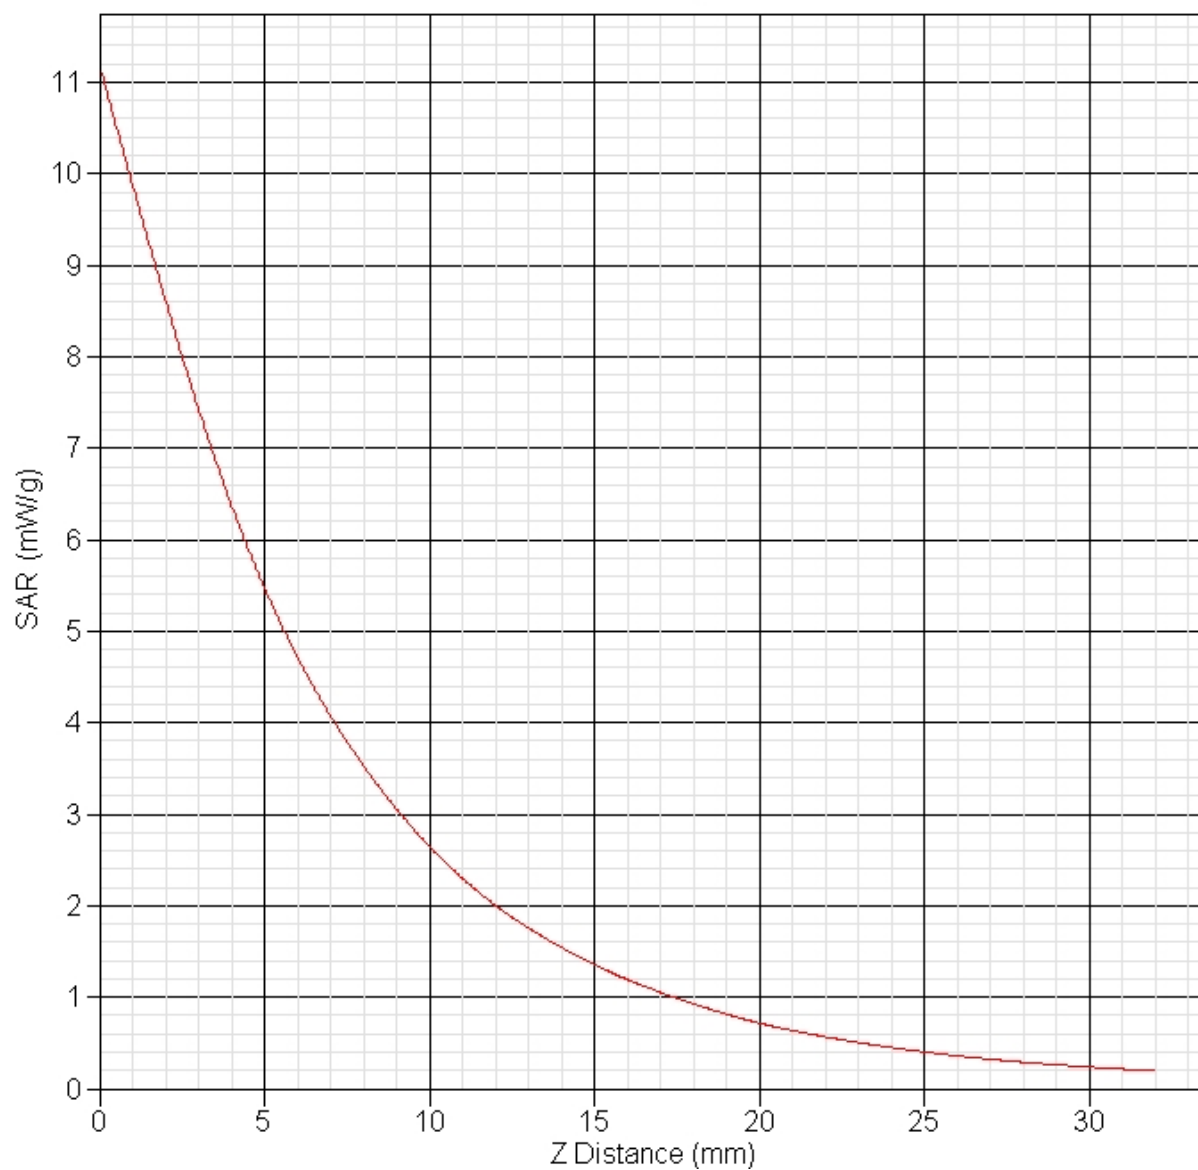

## SAR Test Report

By Operator : Jay  
Measurement Date : 08-Apr-2008  
Starting Time : 08-Apr-2008 07:09:43 AM  
End Time : 08-Apr-2008 07:32:59 AM  
Scanning Time : 1396 secs

### Product Data

Device Name : Validation  
Serial No. : 5200  
Type : Dipole  
Model : ALS-D-BB-S-2  
Frequency : 5200.00 MHz  
Max. Transmit Pwr : 0.1 W  
Drift Time : 0 min(s)  
Length : 23.1 mm  
Width : 3.6 mm  
Depth : 20.7 mm  
Antenna Type : Internal  
Orientation : Touch  
Power Drift-Start : 8.662 W/kg  
Power Drift-Finish: 8.729 W/kg  
Power Drift (%) : 0.776

### Phantom Data

Name : APREL-Uni  
Type : Uni-Phantom  
Size (mm) : 280 x 280 x 200  
Serial No. : System Default  
Location : Center  
Description : Uni-Phantom

### Tissue Data

Type : BODY  
Serial No. : 5200  
Frequency : 5200.00 MHz  
Last Calib. Date : 08-Apr-2008  
Temperature : 20.00 °C  
Ambient Temp. : 23.00 °C  
Humidity : 50.00 RH%  
Epsilon : 48.93 F/m  
Sigma : 5.20 S/m  
Density : 1000.00 kg/cu. m

### Probe Data


Name : Probe AL-E3P1 - AL  
Model : E-030  
Type : E-Field Triangle  
Serial No. : AL-E3P1  
Last Calib. Date : 30-Apr-2007  
Frequency : 5200.00 MHz  
Duty Cycle Factor: 1  
Conversion Factor: 13  
Probe Sensitivity: 1.20 1.20 1.20  $\mu\text{V}/(\text{V/m})^2$   
Compression Point: 95.00 mV  
Offset : 0.56 mm

**Measurement Data**

Crest Factor : 1  
 Scan Type : Complete  
 Tissue Temp. : 20.00 °C  
 Ambient Temp. : 23.00 °C  
 Set-up Date : 08-Apr-2008  
 Set-up Time : 9:00:47 AM  
 Area Scan : 5x5x1 : Measurement x=10mm, y=10mm, z=2mm  
 Zoom Scan : 7x7x10 : Measurement x=4mm, y=4mm, z=2.5mm


**Other Data**

DUT Position : Touch  
 Separation : 10  
 Channel : Mid

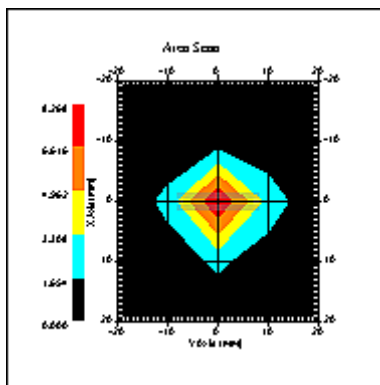

1 gram SAR value : 6.227 W/kg  
 10 gram SAR value : 1.583 W/kg  
 Area Scan Peak SAR : 8.268 W/kg  
 Zoom Scan Peak SAR : 23.318 W/kg

**SAR-Z Axis**  
at Hotspot x:0.41 y:-0.22

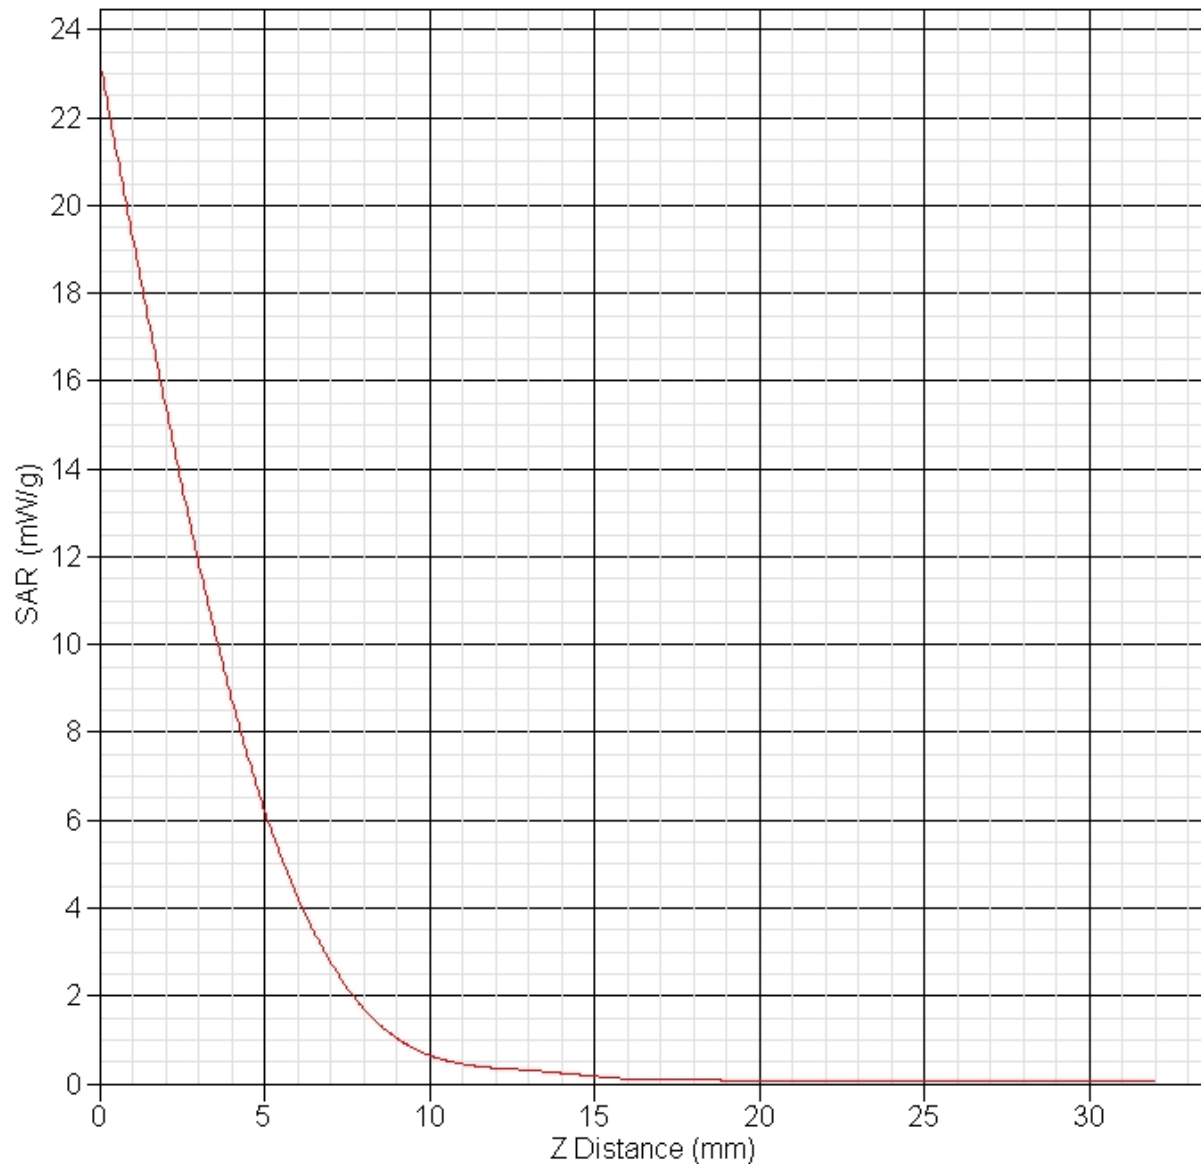

## SAR Test Report

By Operator : Jay  
Measurement Date : 08-Apr-2008  
Starting Time : 08-Apr-2008 07:10:24 AM  
End Time : 08-Apr-2008 07:33:11 AM  
Scanning Time : 1367 secs

### Product Data

Device Name : Validation  
Serial No. : 5800  
Type : Dipole  
Model : ALS-D-BB-S-2  
Frequency : 5800.00 MHz  
Max. Transmit Pwr : 0.1 W  
Drift Time : 0 min(s)  
Length : 23.1 mm  
Width : 3.6 mm  
Depth : 20.7 mm  
Antenna Type : Internal  
Orientation : Touch  
Power Drift-Start : 7.372 W/kg  
Power Drift-Finish: 7.416 W/kg  
Power Drift (%) : 0.599

### Phantom Data

Name : APREL-Uni  
Type : Uni-Phantom  
Size (mm) : 280 x 280 x 200  
Serial No. : System Default  
Location : Center  
Description : Uni-Phantom

### Tissue Data

Type : BODY  
Serial No. : 5800  
Frequency : 5800.00 MHz  
Last Calib. Date : 08-Apr-2008  
Temperature : 20.00 °C  
Ambient Temp. : 23.00 °C  
Humidity : 50.00 RH%  
Epsilon : 47.33 F/m  
Sigma : 5.77 S/m  
Density : 1000.00 kg/cu. m

### Probe Data


Name : Probe AL-E3P1 - AL  
Model : E-030  
Type : E-Field Triangle  
Serial No. : AL-E3P1  
Last Calib. Date : 30-Apr-2007  
Frequency : 5800.00 MHz  
Duty Cycle Factor: 1  
Conversion Factor: 14  
Probe Sensitivity: 1.20 1.20 1.20  $\mu\text{V}/(\text{V/m})^2$   
Compression Point: 95.00 mV  
Offset : 0.56 mm

**Measurement Data**

Crest Factor : 1  
 Scan Type : Complete  
 Tissue Temp. : 20.00 °C  
 Ambient Temp. : 23.00 °C  
 Set-up Date : 08-Apr-2008  
 Set-up Time : 4:10:18 PM  
 Area Scan : 5x5x1 : Measurement x=10mm, y=10mm, z=2mm  
 Zoom Scan : 7x7x10 : Measurement x=4mm, y=4mm, z=2.5mm


**Other Data**

DUT Position : Touch  
 Separation : 10  
 Channel : Mid

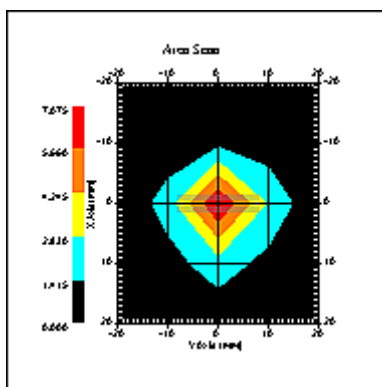

1 gram SAR value : 5.609 W/kg  
 10 gram SAR value : 1.551 W/kg  
 Area Scan Peak SAR : 7.075 W/kg  
 Zoom Scan Peak SAR : 20.116 W/kg

**SAR-Z Axis**  
at Hotspot x:0.31 y:-0.15

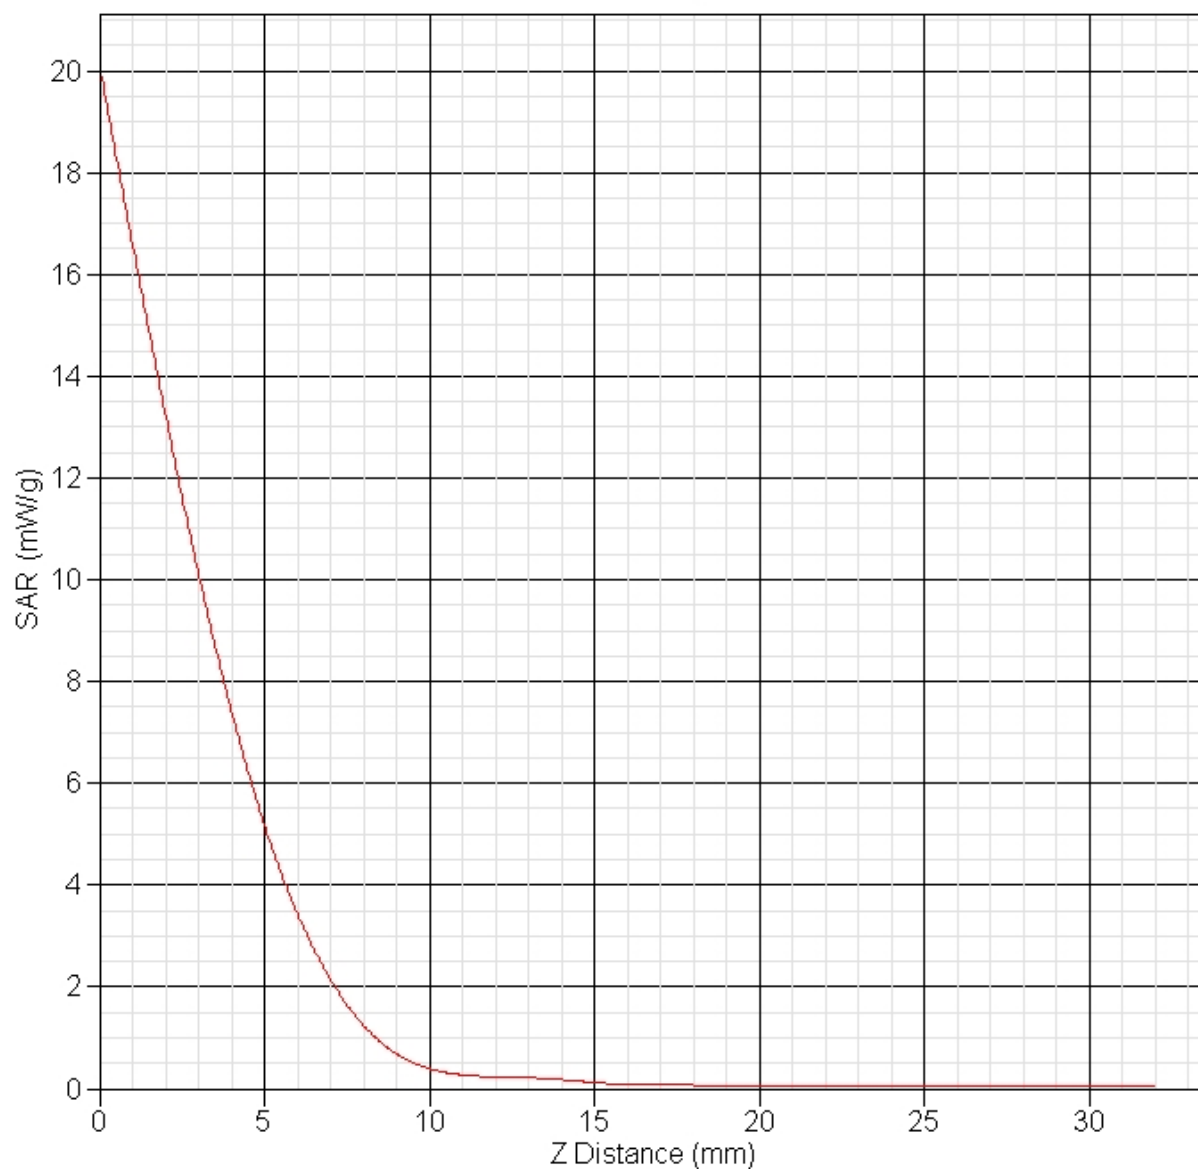

## Appendix B – SAR Test Data Plots

**SAR Test Report**

By Operator : Jay  
Measurement Date : 07-Apr-2008  
Starting Time : 07-Apr-2008 10:17:36 AM  
End Time : 07-Apr-2008 10:32:03 AM  
Scanning Time : 867 secs

**Product Data**

Device Name : LXE  
Serial No. : MX708048360  
Type : Other  
Model : MX7  
Frequency : 2450.00 MHz  
Max. Transmit Pwr : 0.03 W  
Drift Time : 0 min(s)  
Length : 224 mm  
Width : 88 mm  
Depth : 57 mm  
Antenna Type : Internal  
Orientation : Touch  
Power Drift-Start : 0.177 W/kg  
Power Drift-Finish: 0.169 W/kg  
Power Drift (%) : -4.328

**Phantom Data**

Name : APREL-Uni  
Type : Uni-Phantom  
Size (mm) : 280 x 280 x 200  
Serial No. : System Default  
Location : Center  
Description : Uni-Phantom

**Tissue Data**

Type : BODY  
Serial No. : 2450  
Frequency : 2450.00 MHz  
Last Calib. Date : 07-Apr-2008  
Temperature : 20.00 °C  
Ambient Temp. : 24.00 °C  
Humidity : 41.00 RH%  
Epsilon : 53.36 F/m  
Sigma : 1.96 S/m  
Density : 1000.00 kg/cu. m

**Probe Data**


Name : RFEL 217  
Model : E020  
Type : E-Field Triangle  
Serial No. : 217  
Last Calib. Date : 03-Dec-2007  
Frequency : 2450.00 MHz  
Duty Cycle Factor: 1  
Conversion Factor: 3.61  
Probe Sensitivity: 1.20 1.20 1.20  $\mu\text{V}/(\text{V/m})^2$   
Compression Point: 95.00 mV  
Offset : 1.56 mm

**Measurement Data**

Crest Factor : 1  
 Scan Type : Complete  
 Tissue Temp. : 20.00 °C  
 Ambient Temp. : 24.00 °C  
 Set-up Date : 07-Apr-2008  
 Set-up Time : 10:05:42 AM  
 Area Scan : 7x5x1 : Measurement x=10mm, y=10mm, z=4mm  
 Zoom Scan : 5x5x8 : Measurement x=8mm, y=8mm, z=4mm

**Other Data**

DUT Position : Touch  
 Separation : 0  
 Channel : Low

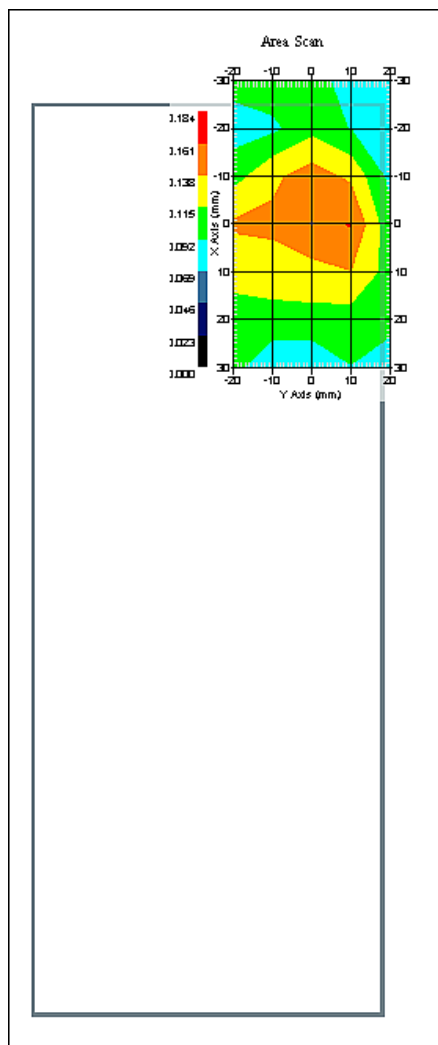

1 gram SAR value : 0.147 W/kg  
 10 gram SAR value : 0.109 W/kg  
 Area Scan Peak SAR : 0.163 W/kg  
 Zoom Scan Peak SAR : 0.180 W/kg

## SAR Test Report

By Operator : Jay  
Measurement Date : 07-Apr-2008  
Starting Time : 07-Apr-2008 10:34:20 AM  
End Time : 07-Apr-2008 10:48:50 AM  
Scanning Time : 870 secs

### Product Data

Device Name : LXE  
Serial No. : MX708048360  
Type : Other  
Model : MX7  
Frequency : 2450.00 MHz  
Max. Transmit Pwr : 0.03 W  
Drift Time : 0 min(s)  
Length : 224 mm  
Width : 88 mm  
Depth : 57 mm  
Antenna Type : Internal  
Orientation : Touch  
Power Drift-Start : 0.137 W/kg  
Power Drift-Finish: 0.133 W/kg  
Power Drift (%) : -2.985

### Phantom Data

Name : APREL-Uni  
Type : Uni-Phantom  
Size (mm) : 280 x 280 x 200  
Serial No. : System Default  
Location : Center  
Description : Uni-Phantom

### Tissue Data

Type : BODY  
Serial No. : 2450  
Frequency : 2450.00 MHz  
Last Calib. Date : 07-Apr-2008  
Temperature : 20.00 °C  
Ambient Temp. : 24.00 °C  
Humidity : 41.00 RH%  
Epsilon : 53.36 F/m  
Sigma : 1.96 S/m  
Density : 1000.00 kg/cu. m

### Probe Data


Name : RFEL 217  
Model : E020  
Type : E-Field Triangle  
Serial No. : 217  
Last Calib. Date : 03-Dec-2007  
Frequency : 2450.00 MHz  
Duty Cycle Factor: 1  
Conversion Factor: 3.61  
Probe Sensitivity: 1.20 1.20 1.20  $\mu\text{V}/(\text{V/m})^2$   
Compression Point: 95.00 mV  
Offset : 1.56 mm

## Measurement Data

Crest Factor : 1  
Scan Type : Complete  
Tissue Temp. : 20.00 °C  
Ambient Temp. : 24.00 °C  
Set-up Date : 07-Apr-2008  
Set-up Time : 10:05:42 AM  
Area Scan : 7x5x1 : Measurement x=10mm, y=10mm, z=4mm  
Zoom Scan : 5x5x8 : Measurement x=8mm, y=8mm, z=4mm

## Other Data

DUT Position : Touch  
Separation : 0  
Channel : Mid

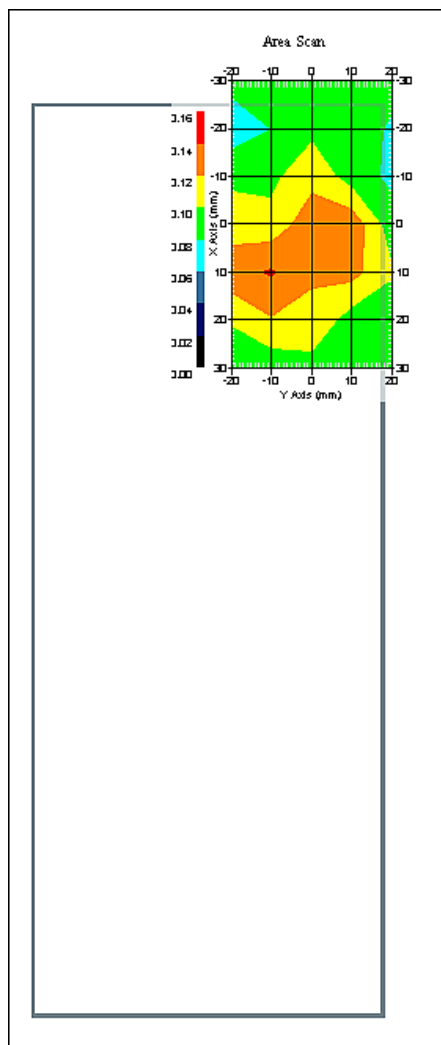

1 gram SAR value : 0.130 W/kg  
10 gram SAR value : 0.097 W/kg  
Area Scan Peak SAR : 0.142 W/kg  
Zoom Scan Peak SAR : 0.160 W/kg

## SAR Test Report

By Operator : Jay  
Measurement Date : 07-Apr-2008  
Starting Time : 07-Apr-2008 11:09:47 AM  
End Time : 07-Apr-2008 11:24:16 AM  
Scanning Time : 869 secs

### Product Data

Device Name : LXE  
Serial No. : MX708048360  
Type : Other  
Model : MX7  
Frequency : 2450.00 MHz  
Max. Transmit Pwr : 0.03 W  
Drift Time : 0 min(s)  
Length : 224 mm  
Width : 88 mm  
Depth : 57 mm  
Antenna Type : Internal  
Orientation : Touch  
Power Drift-Start : 0.104 W/kg  
Power Drift-Finish: 0.100 W/kg  
Power Drift (%) : -3.157

### Phantom Data

Name : APREL-Uni  
Type : Uni-Phantom  
Size (mm) : 280 x 280 x 200  
Serial No. : System Default  
Location : Center  
Description : Uni-Phantom

### Tissue Data

Type : BODY  
Serial No. : 2450  
Frequency : 2450.00 MHz  
Last Calib. Date : 07-Apr-2008  
Temperature : 20.00 °C  
Ambient Temp. : 24.00 °C  
Humidity : 41.00 RH%  
Epsilon : 53.36 F/m  
Sigma : 1.96 S/m  
Density : 1000.00 kg/cu. m

### Probe Data


Name : RFEL 217  
Model : E020  
Type : E-Field Triangle  
Serial No. : 217  
Last Calib. Date : 03-Dec-2007  
Frequency : 2450.00 MHz  
Duty Cycle Factor: 1  
Conversion Factor: 3.61  
Probe Sensitivity: 1.20 1.20 1.20  $\mu\text{V}/(\text{V/m})^2$   
Compression Point: 95.00 mV  
Offset : 1.56 mm

## Measurement Data

Crest Factor : 1  
Scan Type : Complete  
Tissue Temp. : 20.00 °C  
Ambient Temp. : 24.00 °C  
Set-up Date : 07-Apr-2008  
Set-up Time : 10:05:42 AM  
Area Scan : 7x5x1 : Measurement x=10mm, y=10mm, z=4mm  
Zoom Scan : 5x5x8 : Measurement x=8mm, y=8mm, z=4mm

## Other Data

DUT Position : Touch  
Separation : 0  
Channel : High

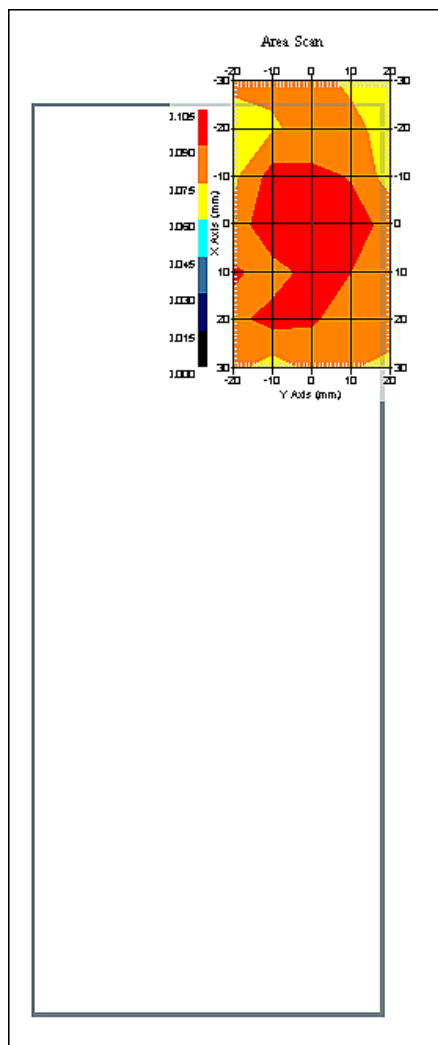

1 gram SAR value : 0.103 W/kg  
10 gram SAR value : 0.083 W/kg  
Area Scan Peak SAR : 0.103 W/kg  
Zoom Scan Peak SAR : 0.110 W/kg

## SAR Test Report

By Operator : Jay  
Measurement Date : 07-Apr-2008  
Starting Time : 07-Apr-2008 02:02:52 PM  
End Time : 07-Apr-2008 02:17:37 PM  
Scanning Time : 885 secs

### Product Data

Device Name : LXE  
Serial No. : MX708048360  
Type : Other  
Model : MX7  
Frequency : 2450.00 MHz  
Max. Transmit Pwr : 0.03 W  
Drift Time : 0 min(s)  
Length : 224 mm  
Width : 88 mm  
Depth : 57 mm  
Antenna Type : Internal  
Orientation : Touch  
Power Drift-Start : 0.212 W/kg  
Power Drift-Finish: 0.208 W/kg  
Power Drift (%) : -1.926

### Phantom Data

Name : APREL-Uni  
Type : Uni-Phantom  
Size (mm) : 280 x 280 x 200  
Serial No. : System Default  
Location : Center  
Description : Uni-Phantom

### Tissue Data

Type : BODY  
Serial No. : 2450  
Frequency : 2450.00 MHz  
Last Calib. Date : 07-Apr-2008  
Temperature : 20.00 °C  
Ambient Temp. : 24.00 °C  
Humidity : 41.00 RH%  
Epsilon : 53.36 F/m  
Sigma : 1.96 S/m  
Density : 1000.00 kg/cu. m

### Probe Data


Name : RFEL 217  
Model : E020  
Type : E-Field Triangle  
Serial No. : 217  
Last Calib. Date : 03-Dec-2007  
Frequency : 2450.00 MHz  
Duty Cycle Factor: 1  
Conversion Factor: 3.61  
Probe Sensitivity: 1.20 1.20 1.20  $\mu\text{V}/(\text{V/m})^2$   
Compression Point: 95.00 mV  
Offset : 1.56 mm

**Measurement Data**

Crest Factor : 1  
 Scan Type : Complete  
 Tissue Temp. : 20.00 °C  
 Ambient Temp. : 24.00 °C  
 Set-up Date : 07-Apr-2008  
 Set-up Time : 10:05:42 AM  
 Area Scan : 7x5x1 : Measurement x=10mm, y=10mm, z=4mm  
 Zoom Scan : 5x5x8 : Measurement x=8mm, y=8mm, z=4mm


**Other Data**

DUT Position : Touch  
 Separation : 0  
 Channel : Low

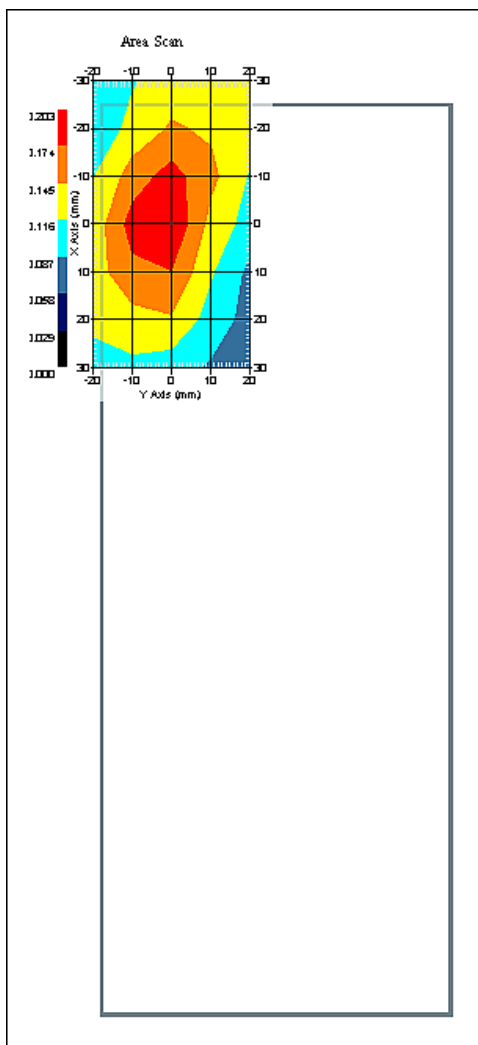

1 gram SAR value : 0.186 W/kg  
 10 gram SAR value : 0.124 W/kg  
 Area Scan Peak SAR : 0.201 W/kg  
 Zoom Scan Peak SAR : 0.290 W/kg

**SAR-Z Axis**  
at Hotspot x:0.25 y:-0.17

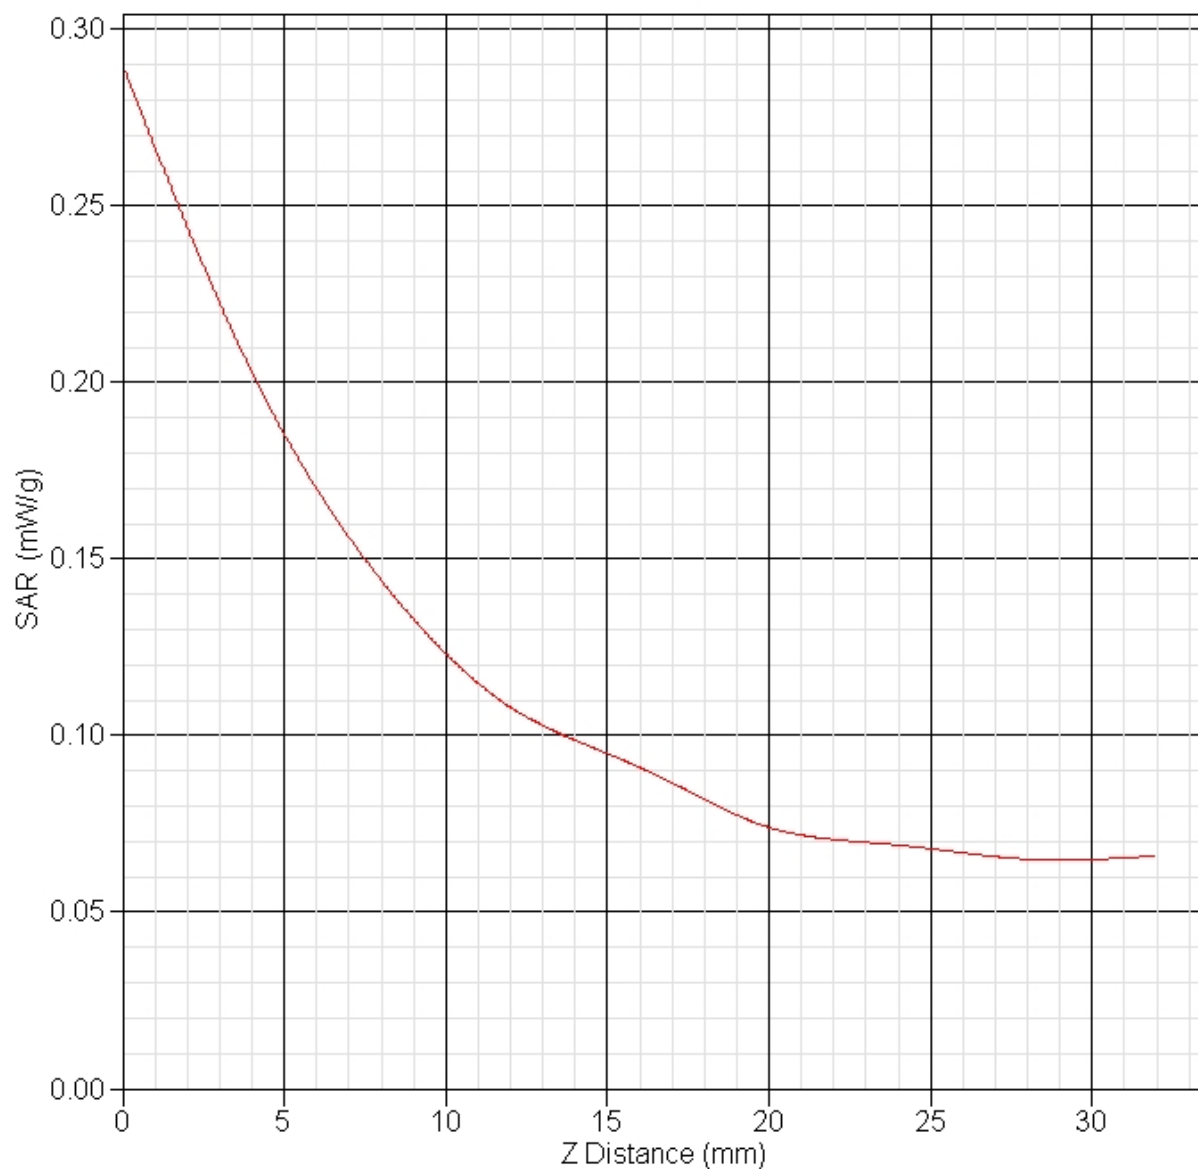

## SAR Test Report

By Operator : Jay  
Measurement Date : 07-Apr-2008  
Starting Time : 07-Apr-2008 02:23:47 PM  
End Time : 07-Apr-2008 02:38:23 PM  
Scanning Time : 876 secs

### Product Data

Device Name : LXE  
Serial No. : MX708048360  
Type : Other  
Model : MX7  
Frequency : 2450.00 MHz  
Max. Transmit Pwr : 0.03 W  
Drift Time : 0 min(s)  
Length : 224 mm  
Width : 88 mm  
Depth : 57 mm  
Antenna Type : Internal  
Orientation : Touch  
Power Drift-Start : 0.194 W/kg  
Power Drift-Finish: 0.185 W/kg  
Power Drift (%) : -4.321

### Phantom Data

Name : APREL-Uni  
Type : Uni-Phantom  
Size (mm) : 280 x 280 x 200  
Serial No. : System Default  
Location : Center  
Description : Uni-Phantom

### Tissue Data

Type : BODY  
Serial No. : 2450  
Frequency : 2450.00 MHz  
Last Calib. Date : 07-Apr-2008  
Temperature : 20.00 °C  
Ambient Temp. : 24.00 °C  
Humidity : 41.00 RH%  
Epsilon : 53.36 F/m  
Sigma : 1.96 S/m  
Density : 1000.00 kg/cu. m

### Probe Data


Name : RFEL 217  
Model : E020  
Type : E-Field Triangle  
Serial No. : 217  
Last Calib. Date : 03-Dec-2007  
Frequency : 2450.00 MHz  
Duty Cycle Factor: 1  
Conversion Factor: 3.61  
Probe Sensitivity: 1.20 1.20 1.20  $\mu\text{V}/(\text{V/m})^2$   
Compression Point: 95.00 mV  
Offset : 1.56 mm

**Measurement Data**

Crest Factor : 1  
 Scan Type : Complete  
 Tissue Temp. : 20.00 °C  
 Ambient Temp. : 24.00 °C  
 Set-up Date : 07-Apr-2008  
 Set-up Time : 10:05:42 AM  
 Area Scan : 7x5x1 : Measurement x=10mm, y=10mm, z=4mm  
 Zoom Scan : 5x5x8 : Measurement x=8mm, y=8mm, z=4mm

**Other Data**

DUT Position : Touch  
 Separation : 0  
 Channel : Mid

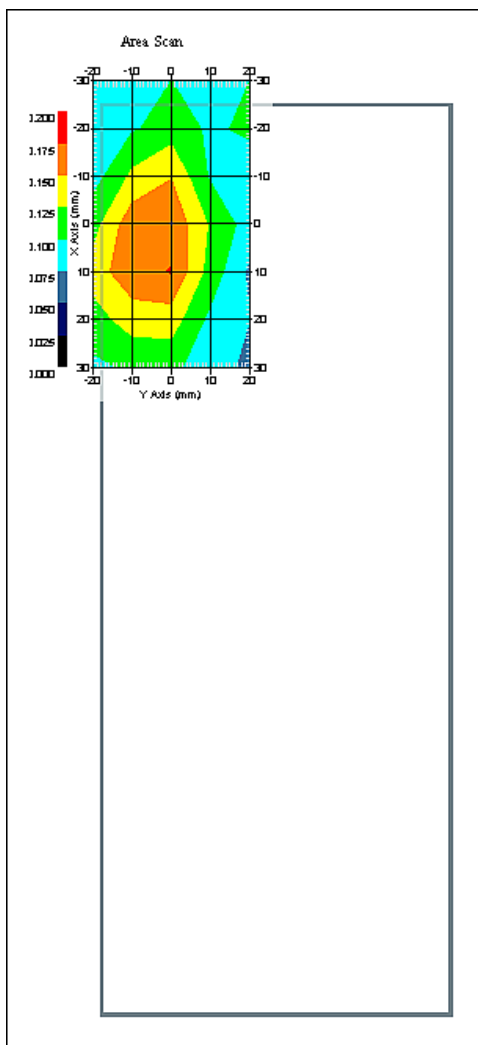

1 gram SAR value : 0.173 W/kg  
 10 gram SAR value : 0.116 W/kg  
 Area Scan Peak SAR : 0.176 W/kg  
 Zoom Scan Peak SAR : 0.270 W/kg

## SAR Test Report

By Operator : Jay  
Measurement Date : 07-Apr-2008  
Starting Time : 07-Apr-2008 02:40:14 PM  
End Time : 07-Apr-2008 02:54:54 PM  
Scanning Time : 880 secs

### Product Data

Device Name : LXE  
Serial No. : MX708048360  
Type : Other  
Model : MX7  
Frequency : 2450.00 MHz  
Max. Transmit Pwr : 0.03 W  
Drift Time : 0 min(s)  
Length : 224 mm  
Width : 88 mm  
Depth : 57 mm  
Antenna Type : Internal  
Orientation : Touch  
Power Drift-Start : 0.143 W/kg  
Power Drift-Finish: 0.140 W/kg  
Power Drift (%) : -2.796

### Phantom Data

Name : APREL-Uni  
Type : Uni-Phantom  
Size (mm) : 280 x 280 x 200  
Serial No. : System Default  
Location : Center  
Description : Uni-Phantom

### Tissue Data

Type : BODY  
Serial No. : 2450  
Frequency : 2450.00 MHz  
Last Calib. Date : 07-Apr-2008  
Temperature : 20.00 °C  
Ambient Temp. : 24.00 °C  
Humidity : 41.00 RH%  
Epsilon : 53.36 F/m  
Sigma : 1.96 S/m  
Density : 1000.00 kg/cu. m

### Probe Data


Name : RFEL 217  
Model : E020  
Type : E-Field Triangle  
Serial No. : 217  
Last Calib. Date : 03-Dec-2007  
Frequency : 2450.00 MHz  
Duty Cycle Factor: 1  
Conversion Factor: 3.61  
Probe Sensitivity: 1.20 1.20 1.20  $\mu\text{V}/(\text{V/m})^2$   
Compression Point: 95.00 mV  
Offset : 1.56 mm

## Measurement Data

Crest Factor : 1  
Scan Type : Complete  
Tissue Temp. : 20.00 °C  
Ambient Temp. : 24.00 °C  
Set-up Date : 07-Apr-2008  
Set-up Time : 10:05:42 AM  
Area Scan : 7x5x1 : Measurement x=10mm, y=10mm, z=4mm  
Zoom Scan : 5x5x8 : Measurement x=8mm, y=8mm, z=4mm

## Other Data

DUT Position : Touch  
Separation : 0  
Channel : High

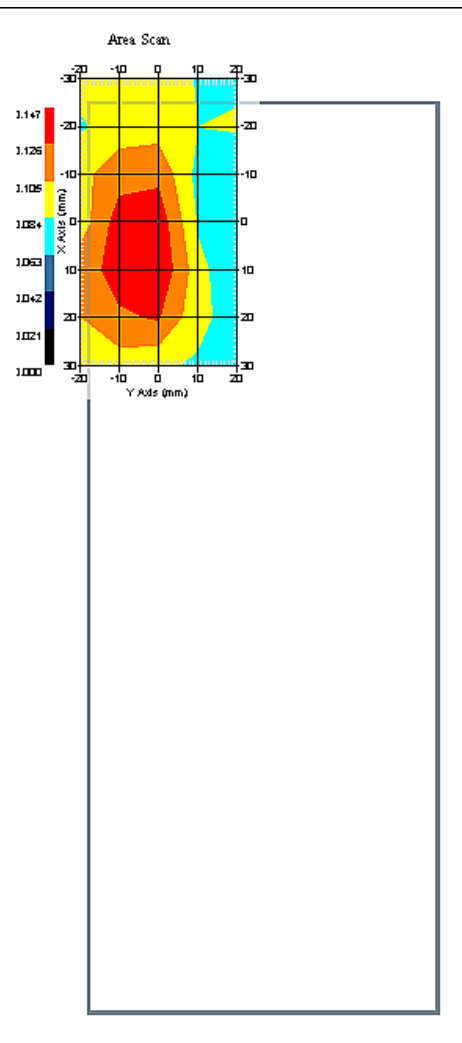

1 gram SAR value : 0.129 W/kg  
10 gram SAR value : 0.093 W/kg  
Area Scan Peak SAR : 0.146 W/kg  
Zoom Scan Peak SAR : 0.190 W/kg

## SAR Test Report

By Operator : Jay  
Measurement Date : 07-Apr-2008  
Starting Time : 07-Apr-2008 01:38:12 PM  
End Time : 07-Apr-2008 01:52:38 PM  
Scanning Time : 866 secs

### Product Data

Device Name : LXE  
Serial No. : MX708048360  
Type : Other  
Model : MX7  
Frequency : 2450.00 MHz  
Max. Transmit Pwr : 0.03 W  
Drift Time : 0 min(s)  
Length : 224 mm  
Width : 88 mm  
Depth : 57 mm  
Antenna Type : Internal  
Orientation : Touch  
Power Drift-Start : 0.096 W/kg  
Power Drift-Finish: 0.098 W/kg  
Power Drift (%) : 2.713

### Phantom Data

Name : APREL-Uni  
Type : Uni-Phantom  
Size (mm) : 280 x 280 x 200  
Serial No. : System Default  
Location : Center  
Description : Uni-Phantom

### Tissue Data

Type : BODY  
Serial No. : 2450  
Frequency : 2450.00 MHz  
Last Calib. Date : 07-Apr-2008  
Temperature : 20.00 °C  
Ambient Temp. : 24.00 °C  
Humidity : 41.00 RH%  
Epsilon : 53.36 F/m  
Sigma : 1.96 S/m  
Density : 1000.00 kg/cu. m

### Probe Data


Name : RFEL 217  
Model : E020  
Type : E-Field Triangle  
Serial No. : 217  
Last Calib. Date : 03-Dec-2007  
Frequency : 2450.00 MHz  
Duty Cycle Factor: 1  
Conversion Factor: 3.61  
Probe Sensitivity: 1.20 1.20 1.20  $\mu\text{V}/(\text{V/m})^2$   
Compression Point: 95.00 mV  
Offset : 1.56 mm

**Measurement Data**

Crest Factor : 1  
 Scan Type : Complete  
 Tissue Temp. : 20.00 °C  
 Ambient Temp. : 24.00 °C  
 Set-up Date : 07-Apr-2008  
 Set-up Time : 10:05:42 AM  
 Area Scan : 7x5x1 : Measurement x=10mm, y=10mm, z=4mm  
 Zoom Scan : 5x5x8 : Measurement x=8mm, y=8mm, z=4mm

**Other Data**

DUT Position : Touch  
 Separation : 0  
 Channel : Low

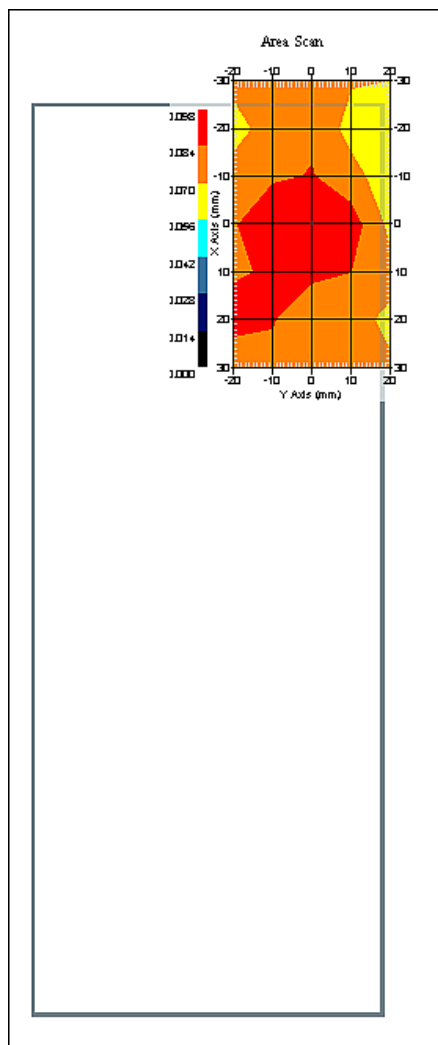

1 gram SAR value : 0.101 W/kg  
 10 gram SAR value : 0.078 W/kg  
 Area Scan Peak SAR : 0.098 W/kg  
 Zoom Scan Peak SAR : 0.040 W/kg

## SAR Test Report

By Operator : Jay  
Measurement Date : 07-Apr-2008  
Starting Time : 07-Apr-2008 01:21:41 PM  
End Time : 07-Apr-2008 01:36:16 PM  
Scanning Time : 875 secs

### Product Data

Device Name : LXE  
Serial No. : MX708048360  
Type : Other  
Model : MX7  
Frequency : 2450.00 MHz  
Max. Transmit Pwr : 0.03 W  
Drift Time : 0 min(s)  
Length : 224 mm  
Width : 88 mm  
Depth : 57 mm  
Antenna Type : Internal  
Orientation : Touch  
Power Drift-Start : 0.091 W/kg  
Power Drift-Finish: 0.087 W/kg  
Power Drift (%) : -4.623

### Phantom Data

Name : APREL-Uni  
Type : Uni-Phantom  
Size (mm) : 280 x 280 x 200  
Serial No. : System Default  
Location : Center  
Description : Uni-Phantom

### Tissue Data

Type : BODY  
Serial No. : 2450  
Frequency : 2450.00 MHz  
Last Calib. Date : 07-Apr-2008  
Temperature : 20.00 °C  
Ambient Temp. : 24.00 °C  
Humidity : 41.00 RH%  
Epsilon : 53.36 F/m  
Sigma : 1.96 S/m  
Density : 1000.00 kg/cu. m

### Probe Data


Name : RFEL 217  
Model : E020  
Type : E-Field Triangle  
Serial No. : 217  
Last Calib. Date : 03-Dec-2007  
Frequency : 2450.00 MHz  
Duty Cycle Factor: 1  
Conversion Factor: 3.61  
Probe Sensitivity: 1.20 1.20 1.20  $\mu\text{V}/(\text{V/m})^2$   
Compression Point: 95.00 mV  
Offset : 1.56 mm

**Measurement Data**

Crest Factor : 1  
 Scan Type : Complete  
 Tissue Temp. : 20.00 °C  
 Ambient Temp. : 24.00 °C  
 Set-up Date : 07-Apr-2008  
 Set-up Time : 10:05:42 AM  
 Area Scan : 7x5x1 : Measurement x=10mm, y=10mm, z=4mm  
 Zoom Scan : 5x5x8 : Measurement x=8mm, y=8mm, z=4mm

**Other Data**

DUT Position : Touch  
 Separation : 0  
 Channel : Mid

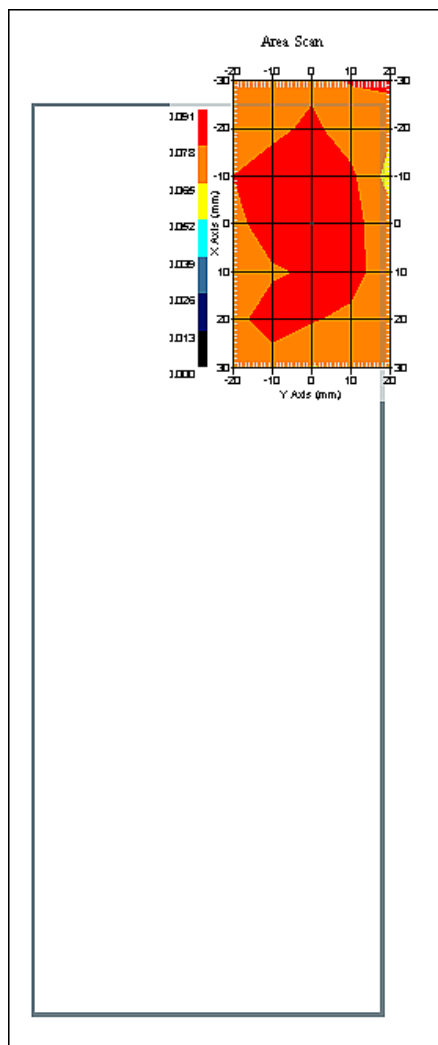

1 gram SAR value : 0.090 W/kg  
 10 gram SAR value : 0.073 W/kg  
 Area Scan Peak SAR : 0.090 W/kg  
 Zoom Scan Peak SAR : 0.020 W/kg

**SAR Test Report**

By Operator : Jay  
Measurement Date : 07-Apr-2008  
Starting Time : 07-Apr-2008 11:34:17 AM  
End Time : 07-Apr-2008 11:48:55 AM  
Scanning Time : 878 secs

**Product Data**

Device Name : LXE  
Serial No. : MX708048360  
Type : Other  
Model : MX7  
Frequency : 2450.00 MHz  
Max. Transmit Pwr : 0.03 W  
Drift Time : 0 min(s)  
Length : 224 mm  
Width : 88 mm  
Depth : 57 mm  
Antenna Type : Internal  
Orientation : Touch  
Power Drift-Start : 0.078 W/kg  
Power Drift-Finish: 0.075 W/kg  
Power Drift (%) : -3.906

**Phantom Data**

Name : APREL-Uni  
Type : Uni-Phantom  
Size (mm) : 280 x 280 x 200  
Serial No. : System Default  
Location : Center  
Description : Uni-Phantom

**Tissue Data**

Type : BODY  
Serial No. : 2450  
Frequency : 2450.00 MHz  
Last Calib. Date : 07-Apr-2008  
Temperature : 20.00 °C  
Ambient Temp. : 24.00 °C  
Humidity : 41.00 RH%  
Epsilon : 53.36 F/m  
Sigma : 1.96 S/m  
Density : 1000.00 kg/cu. m

**Probe Data**


Name : RFEL 217  
Model : E020  
Type : E-Field Triangle  
Serial No. : 217  
Last Calib. Date : 03-Dec-2007  
Frequency : 2450.00 MHz  
Duty Cycle Factor: 1  
Conversion Factor: 3.61  
Probe Sensitivity: 1.20 1.20 1.20  $\mu\text{V}/(\text{V/m})^2$   
Compression Point: 95.00 mV  
Offset : 1.56 mm

**Measurement Data**

Crest Factor : 1  
 Scan Type : Complete  
 Tissue Temp. : 20.00 °C  
 Ambient Temp. : 24.00 °C  
 Set-up Date : 07-Apr-2008  
 Set-up Time : 10:05:42 AM  
 Area Scan : 7x5x1 : Measurement x=10mm, y=10mm, z=4mm  
 Zoom Scan : 5x5x8 : Measurement x=8mm, y=8mm, z=4mm

**Other Data**

DUT Position : Touch  
 Separation : 0  
 Channel : High

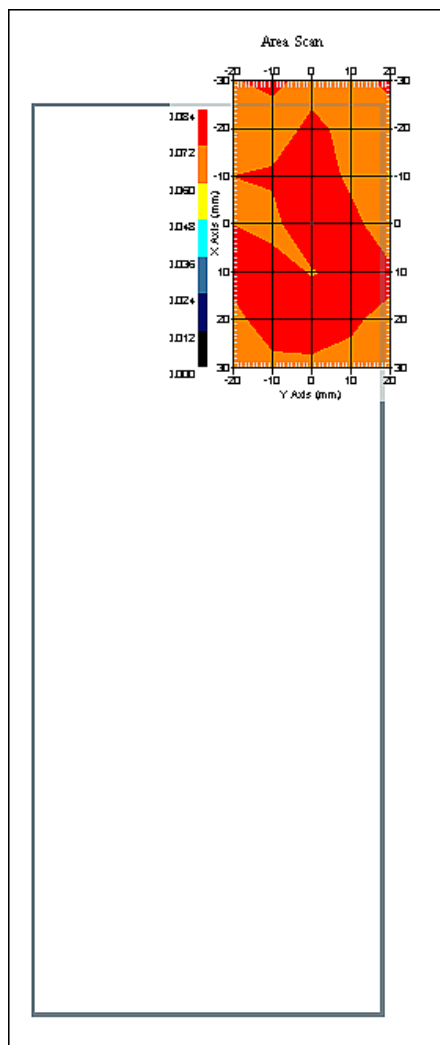

1 gram SAR value : 0.080 W/kg  
 10 gram SAR value : 0.057 W/kg  
 Area Scan Peak SAR : 0.084 W/kg  
 Zoom Scan Peak SAR : 0.130 W/kg

## SAR Test Report

By Operator : Jay  
Measurement Date : 07-Apr-2008  
Starting Time : 07-Apr-2008 03:29:05 PM  
End Time : 07-Apr-2008 03:43:30 PM  
Scanning Time : 865 secs

### Product Data

Device Name : LXE  
Serial No. : MX708048360  
Type : Other  
Model : MX7  
Frequency : 2450.00 MHz  
Max. Transmit Pwr : 0.03 W  
Drift Time : 0 min(s)  
Length : 224 mm  
Width : 88 mm  
Depth : 57 mm  
Antenna Type : Internal  
Orientation : Touch  
Power Drift-Start : 0.138 W/kg  
Power Drift-Finish: 0.133 W/kg  
Power Drift (%) : -3.719

### Phantom Data

Name : APREL-Uni  
Type : Uni-Phantom  
Size (mm) : 280 x 280 x 200  
Serial No. : System Default  
Location : Center  
Description : Uni-Phantom

### Tissue Data

Type : BODY  
Serial No. : 2450  
Frequency : 2450.00 MHz  
Last Calib. Date : 07-Apr-2008  
Temperature : 20.00 °C  
Ambient Temp. : 24.00 °C  
Humidity : 41.00 RH%  
Epsilon : 53.36 F/m  
Sigma : 1.96 S/m  
Density : 1000.00 kg/cu. m

### Probe Data


Name : RFEL 217  
Model : E020  
Type : E-Field Triangle  
Serial No. : 217  
Last Calib. Date : 03-Dec-2007  
Frequency : 2450.00 MHz  
Duty Cycle Factor: 1  
Conversion Factor: 3.61  
Probe Sensitivity: 1.20 1.20 1.20  $\mu\text{V}/(\text{V/m})^2$   
Compression Point: 95.00 mV  
Offset : 1.56 mm

**Measurement Data**

Crest Factor : 1  
 Scan Type : Complete  
 Tissue Temp. : 20.00 °C  
 Ambient Temp. : 24.00 °C  
 Set-up Date : 07-Apr-2008  
 Set-up Time : 10:05:42 AM  
 Area Scan : 7x5x1 : Measurement x=10mm, y=10mm, z=4mm  
 Zoom Scan : 5x5x8 : Measurement x=8mm, y=8mm, z=4mm

**Other Data**

DUT Position : Touch  
 Separation : 0  
 Channel : Low

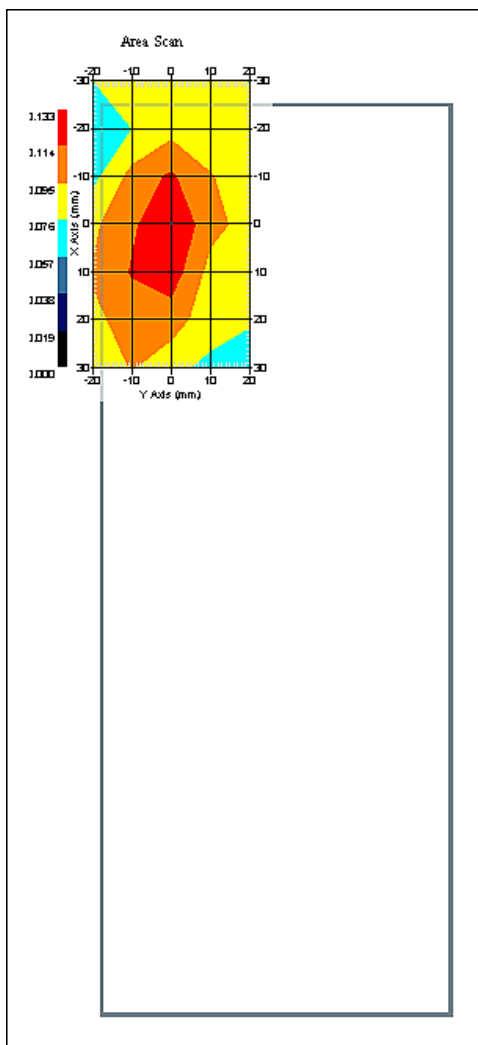

1 gram SAR value : 0.128 W/kg  
 10 gram SAR value : 0.092 W/kg  
 Area Scan Peak SAR : 0.133 W/kg  
 Zoom Scan Peak SAR : 0.180 W/kg

## SAR Test Report

By Operator : Jay  
Measurement Date : 07-Apr-2008  
Starting Time : 07-Apr-2008 03:12:59 PM  
End Time : 07-Apr-2008 03:27:32 PM  
Scanning Time : 873 secs

### Product Data

Device Name : LXE  
Serial No. : MX708048360  
Type : Other  
Model : MX7  
Frequency : 2450.00 MHz  
Max. Transmit Pwr : 0.03 W  
Drift Time : 0 min(s)  
Length : 224 mm  
Width : 88 mm  
Depth : 57 mm  
Antenna Type : Internal  
Orientation : Touch  
Power Drift-Start : 0.114 W/kg  
Power Drift-Finish: 0.111 W/kg  
Power Drift (%) : -2.495

### Phantom Data

Name : APREL-Uni  
Type : Uni-Phantom  
Size (mm) : 280 x 280 x 200  
Serial No. : System Default  
Location : Center  
Description : Uni-Phantom

### Tissue Data

Type : BODY  
Serial No. : 2450  
Frequency : 2450.00 MHz  
Last Calib. Date : 07-Apr-2008  
Temperature : 20.00 °C  
Ambient Temp. : 24.00 °C  
Humidity : 41.00 RH%  
Epsilon : 53.36 F/m  
Sigma : 1.96 S/m  
Density : 1000.00 kg/cu. m

### Probe Data


Name : RFEL 217  
Model : E020  
Type : E-Field Triangle  
Serial No. : 217  
Last Calib. Date : 03-Dec-2007  
Frequency : 2450.00 MHz  
Duty Cycle Factor: 1  
Conversion Factor: 3.61  
Probe Sensitivity: 1.20 1.20 1.20  $\mu\text{V}/(\text{V/m})^2$   
Compression Point: 95.00 mV  
Offset : 1.56 mm

**Measurement Data**

Crest Factor : 1  
 Scan Type : Complete  
 Tissue Temp. : 20.00 °C  
 Ambient Temp. : 24.00 °C  
 Set-up Date : 07-Apr-2008  
 Set-up Time : 10:05:42 AM  
 Area Scan : 7x5x1 : Measurement x=10mm, y=10mm, z=4mm  
 Zoom Scan : 5x5x8 : Measurement x=8mm, y=8mm, z=4mm

**Other Data**

DUT Position : Touch  
 Separation : 0  
 Channel : Mid

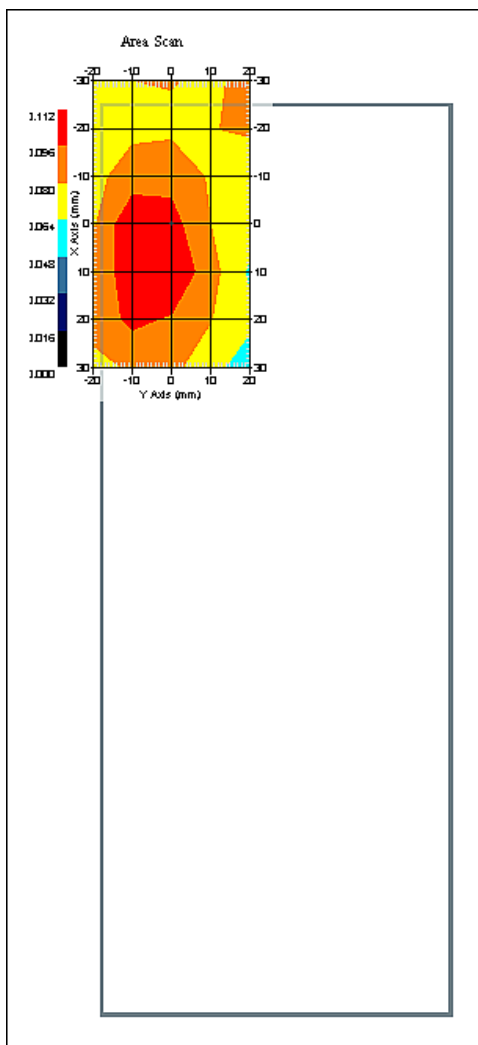

1 gram SAR value : 0.097 W/kg  
 10 gram SAR value : 0.076 W/kg  
 Area Scan Peak SAR : 0.111 W/kg  
 Zoom Scan Peak SAR : 0.130 W/kg

## SAR Test Report

By Operator : Jay  
Measurement Date : 07-Apr-2008  
Starting Time : 07-Apr-2008 02:56:47 PM  
End Time : 07-Apr-2008 03:11:26 PM  
Scanning Time : 879 secs

### Product Data

Device Name : LXE  
Serial No. : MX708048360  
Type : Other  
Model : MX7  
Frequency : 2450.00 MHz  
Max. Transmit Pwr : 0.03 W  
Drift Time : 0 min(s)  
Length : 224 mm  
Width : 88 mm  
Depth : 57 mm  
Antenna Type : Internal  
Orientation : Touch  
Power Drift-Start : 0.098 W/kg  
Power Drift-Finish: 0.100 W/kg  
Power Drift (%) : 1.802

### Phantom Data

Name : APREL-Uni  
Type : Uni-Phantom  
Size (mm) : 280 x 280 x 200  
Serial No. : System Default  
Location : Center  
Description : Uni-Phantom

### Tissue Data

Type : BODY  
Serial No. : 2450  
Frequency : 2450.00 MHz  
Last Calib. Date : 07-Apr-2008  
Temperature : 20.00 °C  
Ambient Temp. : 24.00 °C  
Humidity : 41.00 RH%  
Epsilon : 53.36 F/m  
Sigma : 1.96 S/m  
Density : 1000.00 kg/cu. m

### Probe Data


Name : RFEL 217  
Model : E020  
Type : E-Field Triangle  
Serial No. : 217  
Last Calib. Date : 03-Dec-2007  
Frequency : 2450.00 MHz  
Duty Cycle Factor: 1  
Conversion Factor: 3.61  
Probe Sensitivity: 1.20 1.20 1.20  $\mu\text{V}/(\text{V/m})^2$   
Compression Point: 95.00 mV  
Offset : 1.56 mm

**Measurement Data**

Crest Factor : 1  
 Scan Type : Complete  
 Tissue Temp. : 20.00 °C  
 Ambient Temp. : 24.00 °C  
 Set-up Date : 07-Apr-2008  
 Set-up Time : 10:05:42 AM  
 Area Scan : 7x5x1 : Measurement x=10mm, y=10mm, z=4mm  
 Zoom Scan : 5x5x8 : Measurement x=8mm, y=8mm, z=4mm

**Other Data**

DUT Position : Touch  
 Separation : 0  
 Channel : High

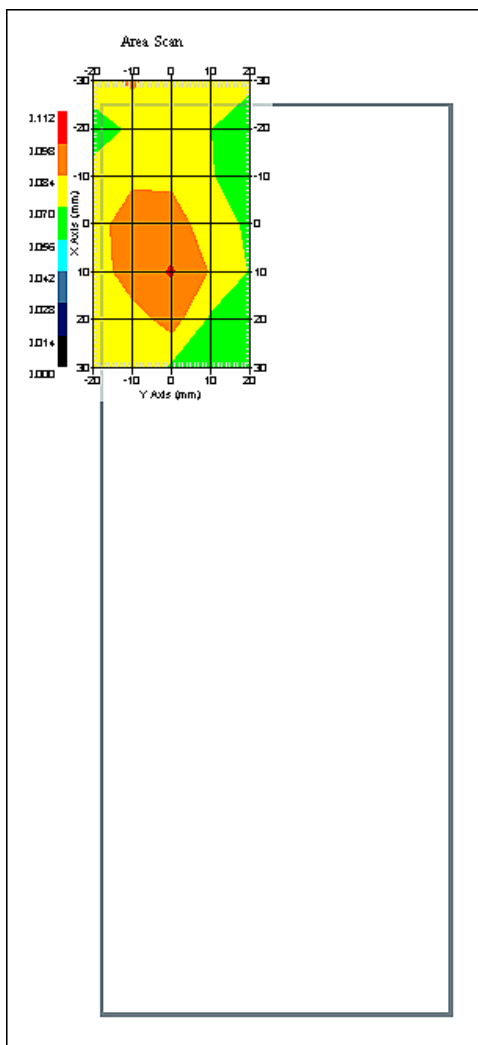

1 gram SAR value : 0.089 W/kg  
 10 gram SAR value : 0.070 W/kg  
 Area Scan Peak SAR : 0.099 W/kg  
 Zoom Scan Peak SAR : 0.140 W/kg

**SAR Test Report**

By Operator : Jay  
Measurement Date : 08-Apr-2008  
Starting Time : 08-Apr-2008 03:08:53 PM  
End Time : 08-Apr-2008 03:35:20 PM  
Scanning Time : 1587 secs

## Product Data

Device Name : LXE  
Serial No. : MX708048360  
Type : Other  
Model : MX7  
Frequency : 5200.00 MHz  
Max. Transmit Pwr : 0.02 W  
Drift Time : 0 min(s)  
Length : 224 mm  
Width : 88 mm  
Depth : 57 mm  
Antenna Type : Internal  
Orientation : Touch  
Power Drift-Start : 0.154 W/kg  
Power Drift-Finish: 0.149 W/kg  
Power Drift (%) : -3.785

## Phantom Data

Name : APREL-Uni  
Type : Uni-Phantom  
Size (mm) : 280 x 280 x 200  
Serial No. : System Default  
Location : Center  
Description : Uni-Phantom

## Tissue Data

Type : BODY  
Serial No. : 5200  
Frequency : 5200.00 MHz  
Last Calib. Date : 08-Apr-2008  
Temperature : 20.00 °C  
Ambient Temp. : 23.00 °C  
Humidity : 50.00 RH%  
Epsilon : 48.93 F/m  
Sigma : 5.20 S/m  
Density : 1000.00 kg/cu. m

## Probe Data


Name : Probe AL-E3P1 - AL  
Model : E-030  
Type : E-Field Triangle  
Serial No. : AL-E3P1  
Last Calib. Date : 30-Apr-2007  
Frequency : 5200.00 MHz  
Duty Cycle Factor: 1  
Conversion Factor: 13  
Probe Sensitivity: 1.20 1.20 1.20  $\mu\text{V}/(\text{V/m})^2$   
Compression Point: 95.00 mV  
Offset : 0.56 mm

## Measurement Data

Crest Factor : 1  
Scan Type : Complete  
Tissue Temp. : 20.00 °C  
Ambient Temp. : 23.00 °C  
Set-up Date : 08-Apr-2008  
Set-up Time : 12:18:46 PM  
Area Scan : 7x7x1 : Measurement x=10mm, y=10mm, z=2mm  
Zoom Scan : 7x7x10 : Measurement x=4mm, y=4mm, z=2.5mm

## Other Data

DUT Position : Touch  
Separation : 0  
Channel : Low

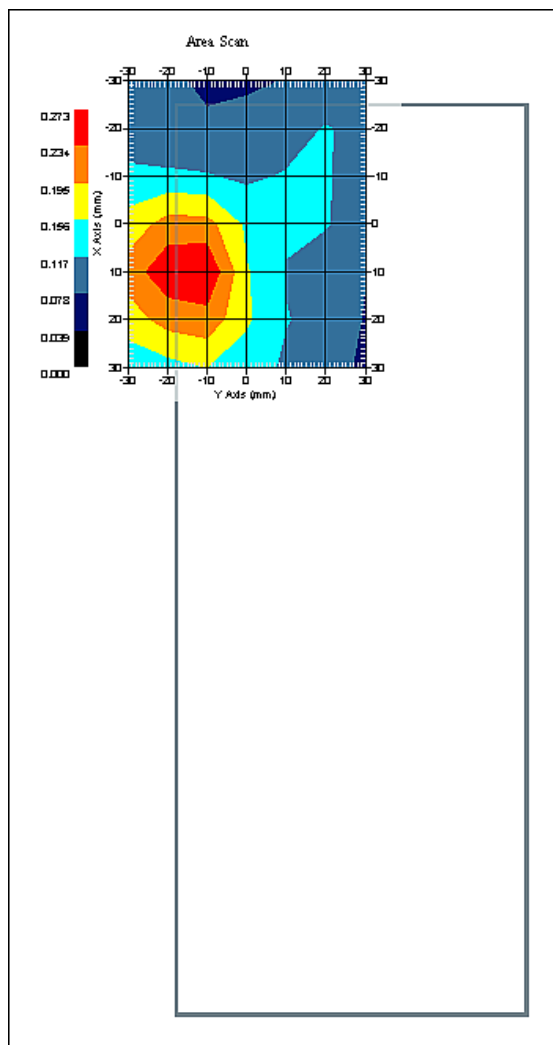

1 gram SAR value : 0.225 W/kg  
10 gram SAR value : 0.125 W/kg  
Area Scan Peak SAR : 0.270 W/kg  
Zoom Scan Peak SAR : 0.430 W/kg

## SAR Test Report

By Operator : Jay  
Measurement Date : 08-Apr-2008  
Starting Time : 08-Apr-2008 03:37:06 PM  
End Time : 08-Apr-2008 04:03:31 PM  
Scanning Time : 1585 secs

### Product Data

Device Name : LXE  
Serial No. : MX708048360  
Type : Other  
Model : MX7  
Frequency : 5200.00 MHz  
Max. Transmit Pwr : 0.02 W  
Drift Time : 0 min(s)  
Length : 224 mm  
Width : 88 mm  
Depth : 57 mm  
Antenna Type : Internal  
Orientation : Touch  
Power Drift-Start : 0.194 W/kg  
Power Drift-Finish: 0.187 W/kg  
Power Drift (%) : -3.867

### Phantom Data

Name : APREL-Uni  
Type : Uni-Phantom  
Size (mm) : 280 x 280 x 200  
Serial No. : System Default  
Location : Center  
Description : Uni-Phantom

### Tissue Data

Type : BODY  
Serial No. : 5200  
Frequency : 5200.00 MHz  
Last Calib. Date : 08-Apr-2008  
Temperature : 20.00 °C  
Ambient Temp. : 23.00 °C  
Humidity : 50.00 RH%  
Epsilon : 48.93 F/m  
Sigma : 5.20 S/m  
Density : 1000.00 kg/cu. m

### Probe Data


Name : Probe AL-E3P1 - AL  
Model : E-030  
Type : E-Field Triangle  
Serial No. : AL-E3P1  
Last Calib. Date : 30-Apr-2007  
Frequency : 5200.00 MHz  
Duty Cycle Factor: 1  
Conversion Factor: 13  
Probe Sensitivity: 1.20 1.20 1.20  $\mu\text{V}/(\text{V/m})^2$   
Compression Point: 95.00 mV  
Offset : 0.56 mm

**Measurement Data**

Crest Factor : 1  
 Scan Type : Complete  
 Tissue Temp. : 20.00 °C  
 Ambient Temp. : 23.00 °C  
 Set-up Date : 08-Apr-2008  
 Set-up Time : 12:18:46 PM  
 Area Scan : 7x7x1 : Measurement x=10mm, y=10mm, z=2mm  
 Zoom Scan : 7x7x10 : Measurement x=4mm, y=4mm, z=2.5mm


**Other Data**

DUT Position : Touch  
 Separation : 0  
 Channel : High

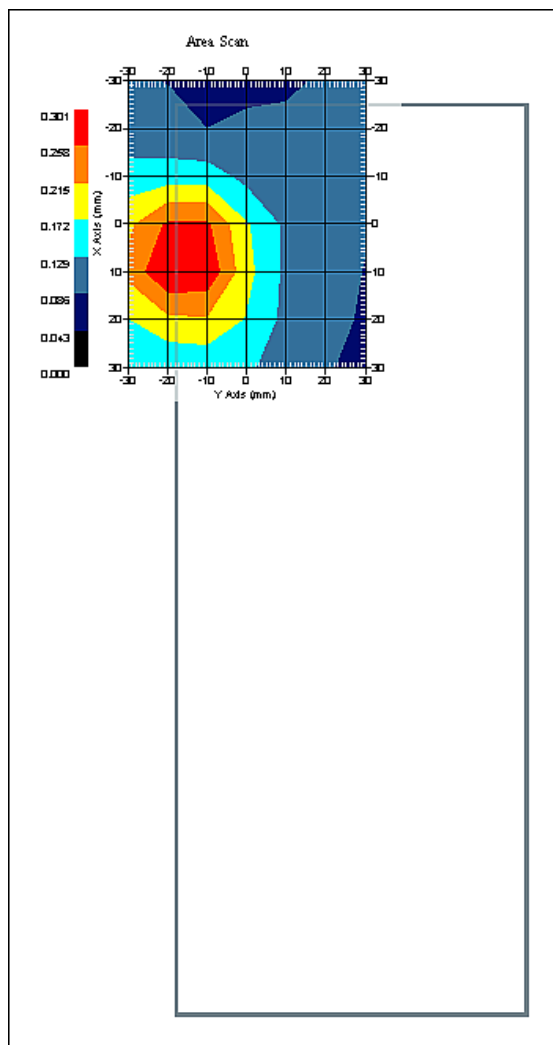

1 gram SAR value : 0.225 W/kg  
 10 gram SAR value : 0.134 W/kg  
 Area Scan Peak SAR : 0.299 W/kg  
 Zoom Scan Peak SAR : 0.500 W/kg

**SAR-Z Axis**  
at Hotspot x:6.22 y:-12.10

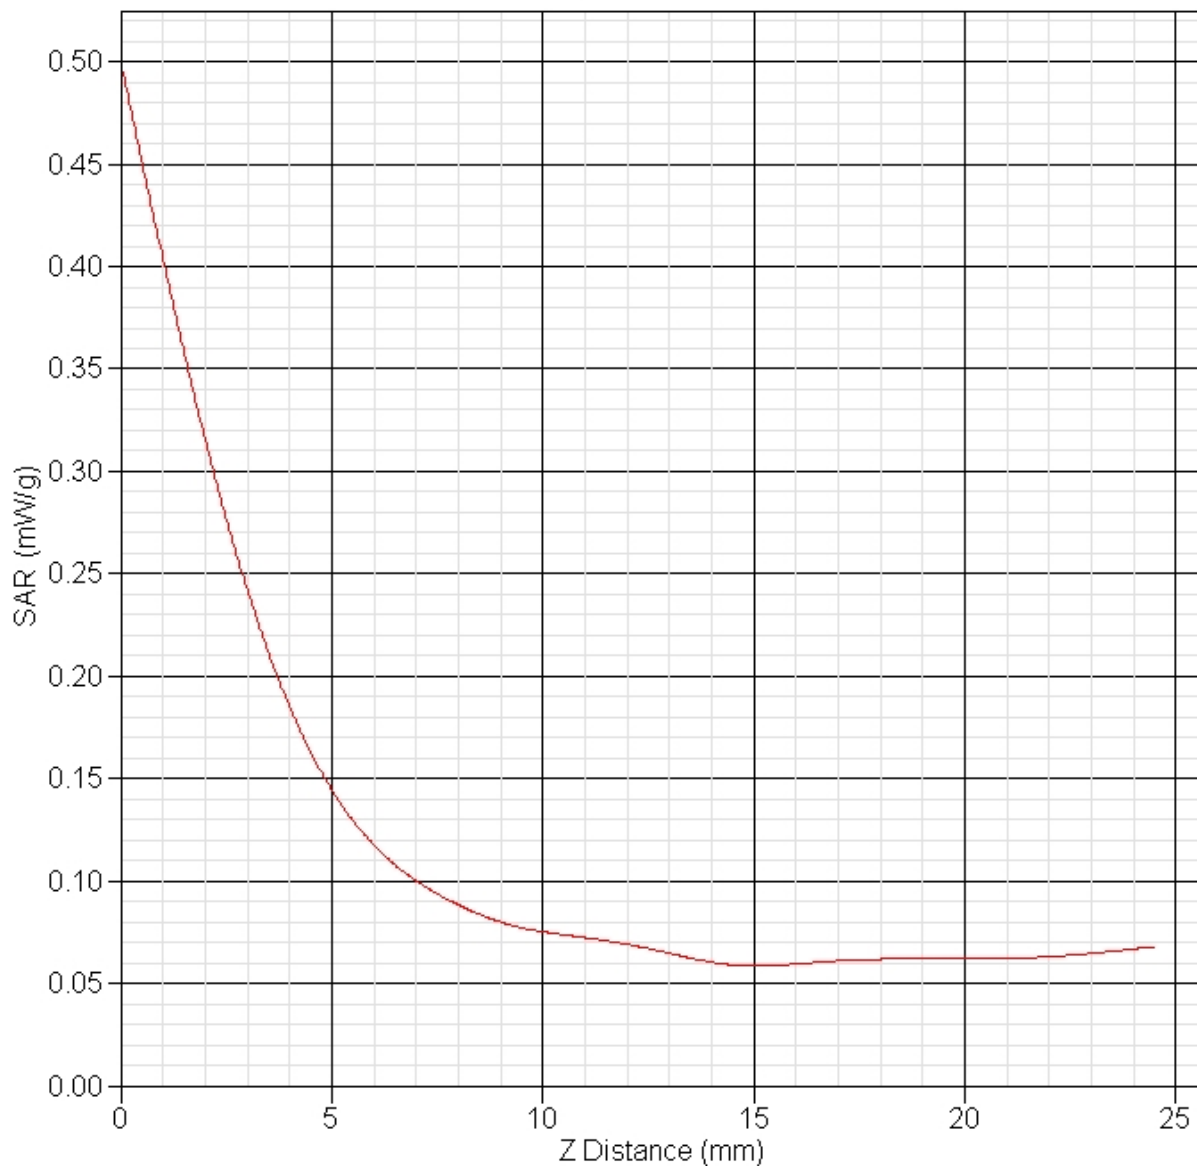

**SAR Test Report**

By Operator : Jay  
Measurement Date : 08-Apr-2008  
Starting Time : 08-Apr-2008 02:04:57 PM  
End Time : 08-Apr-2008 02:31:23 PM  
Scanning Time : 1586 secs

**Product Data**

Device Name : LXE  
Serial No. : MX708048360  
Type : Other  
Model : MX7  
Frequency : 5200.00 MHz  
Max. Transmit Pwr : 0.02 W  
Drift Time : 0 min(s)  
Length : 224 mm  
Width : 88 mm  
Depth : 57 mm  
Antenna Type : Internal  
Orientation : Touch  
Power Drift-Start : 0.098 W/kg  
Power Drift-Finish: 0.094 W/kg  
Power Drift (%) : -4.083

**Phantom Data**

Name : APREL-Uni  
Type : Uni-Phantom  
Size (mm) : 280 x 280 x 200  
Serial No. : System Default  
Location : Center  
Description : Uni-Phantom

**Tissue Data**

Type : BODY  
Serial No. : 5200  
Frequency : 5200.00 MHz  
Last Calib. Date : 08-Apr-2008  
Temperature : 20.00 °C  
Ambient Temp. : 23.00 °C  
Humidity : 50.00 RH%  
Epsilon : 48.93 F/m  
Sigma : 5.20 S/m  
Density : 1000.00 kg/cu. m

**Probe Data**


Name : Probe AL-E3P1 - AL  
Model : E-030  
Type : E-Field Triangle  
Serial No. : AL-E3P1  
Last Calib. Date : 30-Apr-2007  
Frequency : 5200.00 MHz  
Duty Cycle Factor: 1  
Conversion Factor: 13  
Probe Sensitivity: 1.20 1.20 1.20  $\mu\text{V}/(\text{V/m})^2$   
Compression Point: 95.00 mV  
Offset : 0.56 mm

**Measurement Data**

Crest Factor : 1  
 Scan Type : Complete  
 Tissue Temp. : 20.00 °C  
 Ambient Temp. : 23.00 °C  
 Set-up Date : 08-Apr-2008  
 Set-up Time : 12:18:46 PM  
 Area Scan : 7x7x1 : Measurement x=10mm, y=10mm, z=2mm  
 Zoom Scan : 7x7x10 : Measurement x=4mm, y=4mm, z=2.5mm

**Other Data**

DUT Position : Touch  
 Separation : 0  
 Channel : Low

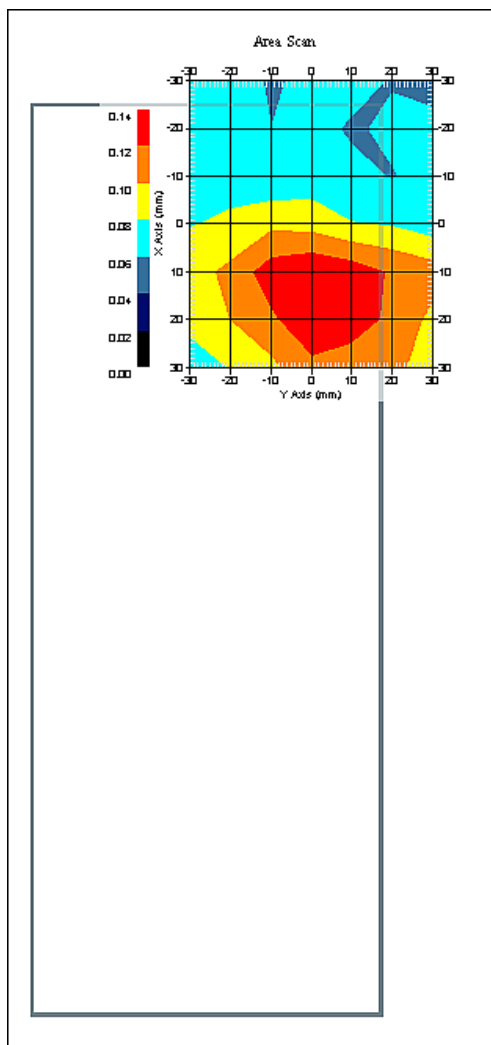

1 gram SAR value : 0.109 W/kg  
 10 gram SAR value : 0.078 W/kg  
 Area Scan Peak SAR : 0.139 W/kg  
 Zoom Scan Peak SAR : 0.180 W/kg

## SAR Test Report

By Operator : Jay  
Measurement Date : 08-Apr-2008  
Starting Time : 08-Apr-2008 02:33:56 PM  
End Time : 08-Apr-2008 03:00:17 PM  
Scanning Time : 1581 secs

### Product Data

Device Name : LXE  
Serial No. : MX708048360  
Type : Other  
Model : MX7  
Frequency : 5200.00 MHz  
Max. Transmit Pwr : 0.02 W  
Drift Time : 0 min(s)  
Length : 224 mm  
Width : 88 mm  
Depth : 57 mm  
Antenna Type : Internal  
Orientation : Touch  
Power Drift-Start : 0.125 W/kg  
Power Drift-Finish: 0.121 W/kg  
Power Drift (%) : -3.986

### Phantom Data

Name : APREL-Uni  
Type : Uni-Phantom  
Size (mm) : 280 x 280 x 200  
Serial No. : System Default  
Location : Center  
Description : Uni-Phantom

### Tissue Data

Type : BODY  
Serial No. : 5200  
Frequency : 5200.00 MHz  
Last Calib. Date : 08-Apr-2008  
Temperature : 20.00 °C  
Ambient Temp. : 23.00 °C  
Humidity : 50.00 RH%  
Epsilon : 48.93 F/m  
Sigma : 5.20 S/m  
Density : 1000.00 kg/cu. m

### Probe Data


Name : Probe AL-E3P1 - AL  
Model : E-030  
Type : E-Field Triangle  
Serial No. : AL-E3P1  
Last Calib. Date : 30-Apr-2007  
Frequency : 5200.00 MHz  
Duty Cycle Factor: 1  
Conversion Factor: 13  
Probe Sensitivity: 1.20 1.20 1.20  $\mu\text{V}/(\text{V/m})^2$   
Compression Point: 95.00 mV  
Offset : 0.56 mm

**Measurement Data**

Crest Factor : 1  
 Scan Type : Complete  
 Tissue Temp. : 20.00 °C  
 Ambient Temp. : 23.00 °C  
 Set-up Date : 08-Apr-2008  
 Set-up Time : 12:18:46 PM  
 Area Scan : 7x7x1 : Measurement x=10mm, y=10mm, z=2mm  
 Zoom Scan : 7x7x10 : Measurement x=4mm, y=4mm, z=2.5mm

**Other Data**

DUT Position : Touch  
 Separation : 0  
 Channel : High

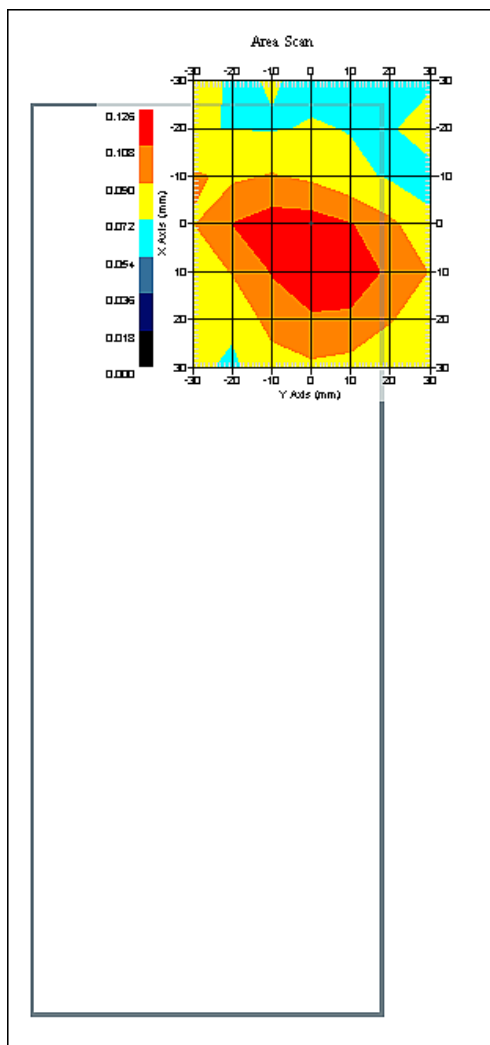

1 gram SAR value : 0.111 W/kg  
 10 gram SAR value : 0.078 W/kg  
 Area Scan Peak SAR : 0.125 W/kg  
 Zoom Scan Peak SAR : 0.150 W/kg

## SAR Test Report

By Operator : Jay  
Measurement Date : 09-Apr-2008  
Starting Time : 09-Apr-2008 11:12:03 AM  
End Time : 09-Apr-2008 11:38:56 AM  
Scanning Time : 1613 secs

### Product Data

Device Name : LXE  
Serial No. : MX708048360  
Type : Other  
Model : MX7  
Frequency : 5800.00 MHz  
Max. Transmit Pwr : 0.01 W  
Drift Time : 0 min(s)  
Length : 224 mm  
Width : 88 mm  
Depth : 57 mm  
Antenna Type : Internal  
Orientation : Touch  
Power Drift-Start : 0.122 W/kg  
Power Drift-Finish: 0.121 W/kg  
Power Drift (%) : -0.926

### Phantom Data

Name : APREL-Uni  
Type : Uni-Phantom  
Size (mm) : 280 x 280 x 200  
Serial No. : System Default  
Location : Center  
Description : Uni-Phantom

### Tissue Data

Type : BODY  
Serial No. : 5800  
Frequency : 5800.00 MHz  
Last Calib. Date : 09-Apr-2008  
Temperature : 20.00 °C  
Ambient Temp. : 23.00 °C  
Humidity : 50.00 RH%  
Epsilon : 47.33 F/m  
Sigma : 5.77 S/m  
Density : 1000.00 kg/cu. m

### Probe Data


Name : Probe AL-E3P1 - AL  
Model : E-030  
Type : E-Field Triangle  
Serial No. : AL-E3P1  
Last Calib. Date : 30-Apr-2007  
Frequency : 5800.00 MHz  
Duty Cycle Factor: 1  
Conversion Factor: 14  
Probe Sensitivity: 1.20 1.20 1.20  $\mu\text{V}/(\text{V/m})^2$   
Compression Point: 95.00 mV  
Offset : 0.56 mm

**Measurement Data**

Crest Factor : 1  
 Scan Type : Complete  
 Tissue Temp. : 20.00 °C  
 Ambient Temp. : 23.00 °C  
 Set-up Date : 09-Apr-2008  
 Set-up Time : 7:14:59 AM  
 Area Scan : 7x7x1 : Measurement x=10mm, y=10mm, z=2mm  
 Zoom Scan : 7x7x10 : Measurement x=4mm, y=4mm, z=2.5mm

**Other Data**

DUT Position : Touch  
 Separation : 0  
 Channel : Low

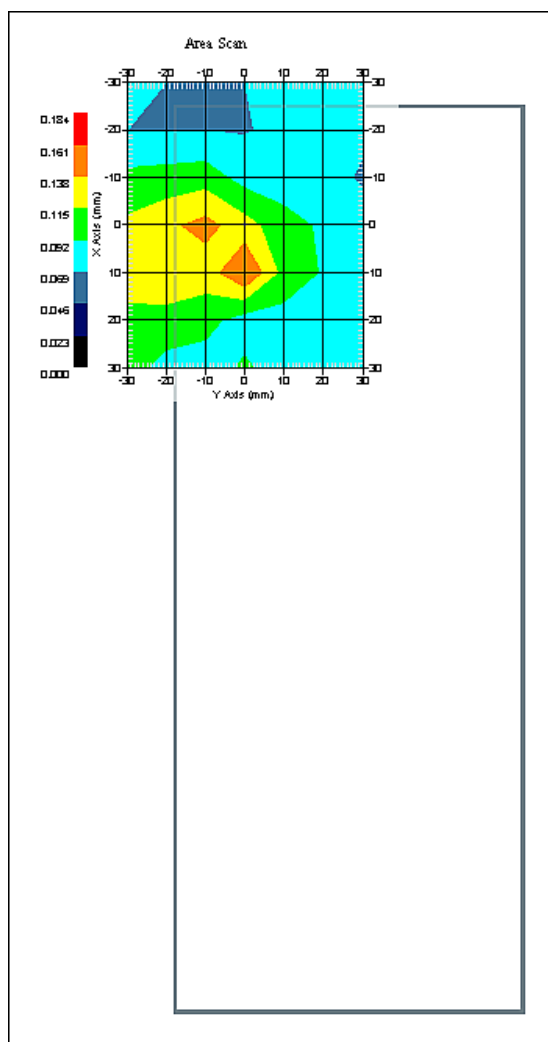

1 gram SAR value : 0.132 W/kg  
 10 gram SAR value : 0.142 W/kg  
 Area Scan Peak SAR : 0.162 W/kg  
 Zoom Scan Peak SAR : 0.160 W/kg

**SAR Test Report**

By Operator : Jay  
Measurement Date : 09-Apr-2008  
Starting Time : 09-Apr-2008 11:46:12 AM  
End Time : 09-Apr-2008 12:13:38 PM  
Scanning Time : 1646 secs

## Product Data

Device Name : LXE  
Serial No. : MX708048360  
Type : Other  
Model : MX7  
Frequency : 5800.00 MHz  
Max. Transmit Pwr : 0.01 W  
Drift Time : 0 min(s)  
Length : 224 mm  
Width : 88 mm  
Depth : 57 mm  
Antenna Type : Internal  
Orientation : Touch  
Power Drift-Start : 0.125 W/kg  
Power Drift-Finish: 0.121 W/kg  
Power Drift (%) : -3.856

## Phantom Data

Name : APREL-Uni  
Type : Uni-Phantom  
Size (mm) : 280 x 280 x 200  
Serial No. : System Default  
Location : Center  
Description : Uni-Phantom

## Tissue Data

Type : BODY  
Serial No. : 5800  
Frequency : 5800.00 MHz  
Last Calib. Date : 09-Apr-2008  
Temperature : 20.00 °C  
Ambient Temp. : 23.00 °C  
Humidity : 50.00 RH%  
Epsilon : 47.33 F/m  
Sigma : 5.77 S/m  
Density : 1000.00 kg/cu. m

## Probe Data


Name : Probe AL-E3P1 - AL  
Model : E-030  
Type : E-Field Triangle  
Serial No. : AL-E3P1  
Last Calib. Date : 30-Apr-2007  
Frequency : 5800.00 MHz  
Duty Cycle Factor: 1  
Conversion Factor: 14  
Probe Sensitivity: 1.20 1.20 1.20  $\mu\text{V}/(\text{V/m})^2$   
Compression Point: 95.00 mV  
Offset : 0.56 mm

**Measurement Data**

Crest Factor : 1  
 Scan Type : Complete  
 Tissue Temp. : 20.00 °C  
 Ambient Temp. : 23.00 °C  
 Set-up Date : 09-Apr-2008  
 Set-up Time : 7:14:59 AM  
 Area Scan : 7x7x1 : Measurement x=10mm, y=10mm, z=2mm  
 Zoom Scan : 7x7x10 : Measurement x=4mm, y=4mm, z=2.5mm

**Other Data**

DUT Position : Touch  
 Separation : 0  
 Channel : High

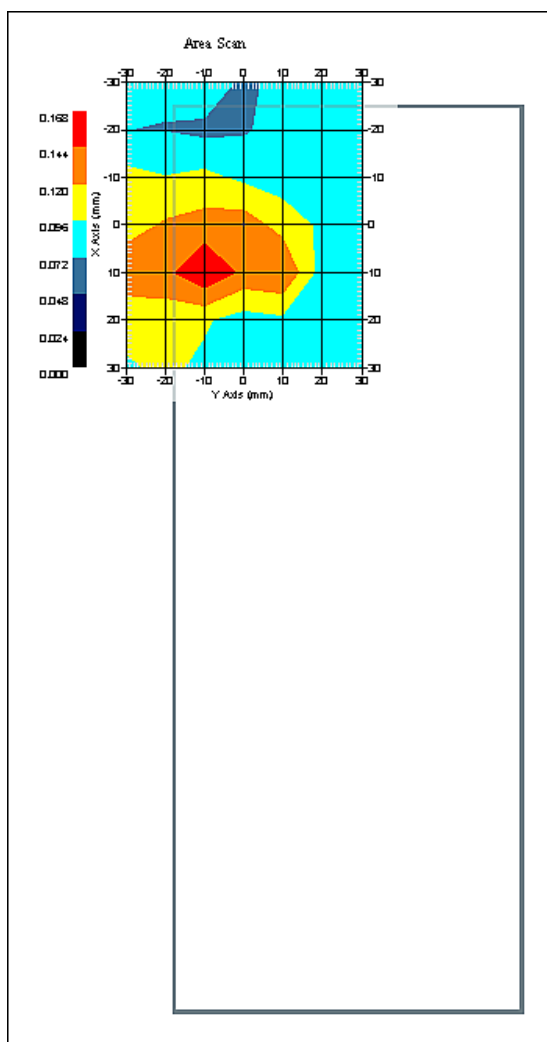

1 gram SAR value : 0.120 W/kg  
 10 gram SAR value : 0.112 W/kg  
 Area Scan Peak SAR : 0.168 W/kg  
 Zoom Scan Peak SAR : 0.160 W/kg

## SAR Test Report

By Operator : Jay  
Measurement Date : 09-Apr-2008  
Starting Time : 09-Apr-2008 10:00:52 AM  
End Time : 09-Apr-2008 10:27:44 AM  
Scanning Time : 1612 secs

### Product Data

Device Name : LXE  
Serial No. : MX708048360  
Type : Other  
Model : MX7  
Frequency : 5800.00 MHz  
Max. Transmit Pwr : 0.01 W  
Drift Time : 0 min(s)  
Length : 224 mm  
Width : 88 mm  
Depth : 57 mm  
Antenna Type : Internal  
Orientation : Touch  
Power Drift-Start : 0.115 W/kg  
Power Drift-Finish: 0.114 W/kg  
Power Drift (%) : -1.031

### Phantom Data

Name : APREL-Uni  
Type : Uni-Phantom  
Size (mm) : 280 x 280 x 200  
Serial No. : System Default  
Location : Center  
Description : Uni-Phantom

### Tissue Data

Type : BODY  
Serial No. : 5800  
Frequency : 5800.00 MHz  
Last Calib. Date : 09-Apr-2008  
Temperature : 20.00 °C  
Ambient Temp. : 23.00 °C  
Humidity : 50.00 RH%  
Epsilon : 47.33 F/m  
Sigma : 5.77 S/m  
Density : 1000.00 kg/cu. m

### Probe Data


Name : Probe AL-E3P1 - AL  
Model : E-030  
Type : E-Field Triangle  
Serial No. : AL-E3P1  
Last Calib. Date : 30-Apr-2007  
Frequency : 5800.00 MHz  
Duty Cycle Factor: 1  
Conversion Factor: 14  
Probe Sensitivity: 1.20 1.20 1.20  $\mu\text{V}/(\text{V/m})^2$   
Compression Point: 95.00 mV  
Offset : 0.56 mm

**Measurement Data**

Crest Factor : 1  
 Scan Type : Complete  
 Tissue Temp. : 20.00 °C  
 Ambient Temp. : 23.00 °C  
 Set-up Date : 09-Apr-2008  
 Set-up Time : 7:14:59 AM  
 Area Scan : 7x7x1 : Measurement x=10mm, y=10mm, z=2mm  
 Zoom Scan : 7x7x10 : Measurement x=4mm, y=4mm, z=2.5mm

**Other Data**

DUT Position : Touch  
 Separation : 0  
 Channel : Low

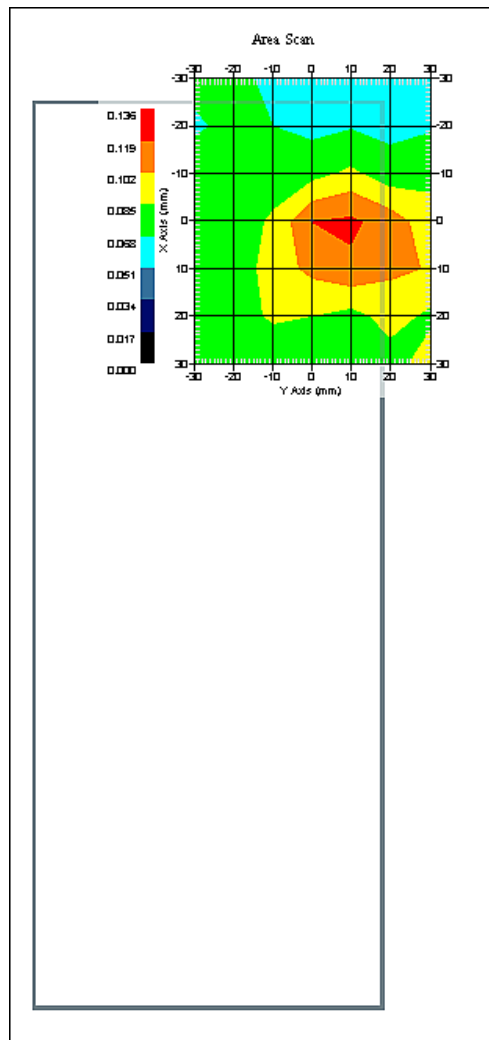

1 gram SAR value : 0.109 W/kg  
 10 gram SAR value : 0.078 W/kg  
 Area Scan Peak SAR : 0.122 W/kg  
 Zoom Scan Peak SAR : 0.200 W/kg

## SAR Test Report

By Operator : Jay  
Measurement Date : 09-Apr-2008  
Starting Time : 09-Apr-2008 10:29:45 AM  
End Time : 09-Apr-2008 10:56:43 AM  
Scanning Time : 1618 secs

### Product Data

Device Name : LXE  
Serial No. : MX708048360  
Type : Other  
Model : MX7  
Frequency : 5800.00 MHz  
Max. Transmit Pwr : 0.01 W  
Drift Time : 0 min(s)  
Length : 224 mm  
Width : 88 mm  
Depth : 57 mm  
Antenna Type : Internal  
Orientation : Touch  
Power Drift-Start : 0.137 W/kg  
Power Drift-Finish: 0.136 W/kg  
Power Drift (%) : -0.747

### Phantom Data

Name : APREL-Uni  
Type : Uni-Phantom  
Size (mm) : 280 x 280 x 200  
Serial No. : System Default  
Location : Center  
Description : Uni-Phantom

### Tissue Data

Type : BODY  
Serial No. : 5800  
Frequency : 5800.00 MHz  
Last Calib. Date : 09-Apr-2008  
Temperature : 20.00 °C  
Ambient Temp. : 23.00 °C  
Humidity : 50.00 RH%  
Epsilon : 47.33 F/m  
Sigma : 5.77 S/m  
Density : 1000.00 kg/cu. m

### Probe Data


Name : Probe AL-E3P1 - AL  
Model : E-030  
Type : E-Field Triangle  
Serial No. : AL-E3P1  
Last Calib. Date : 30-Apr-2007  
Frequency : 5800.00 MHz  
Duty Cycle Factor: 1  
Conversion Factor: 14  
Probe Sensitivity: 1.20 1.20 1.20  $\mu\text{V}/(\text{V/m})^2$   
Compression Point: 95.00 mV  
Offset : 0.56 mm

## Measurement Data

Crest Factor : 1  
Scan Type : Complete  
Tissue Temp. : 20.00 °C  
Ambient Temp. : 23.00 °C  
Set-up Date : 09-Apr-2008  
Set-up Time : 7:14:59 AM  
Area Scan : 7x7x1 : Measurement x=10mm, y=10mm, z=2mm  
Zoom Scan : 7x7x10 : Measurement x=4mm, y=4mm, z=2.5mm


## Other Data

DUT Position : Touch  
Separation : 0  
Channel : High

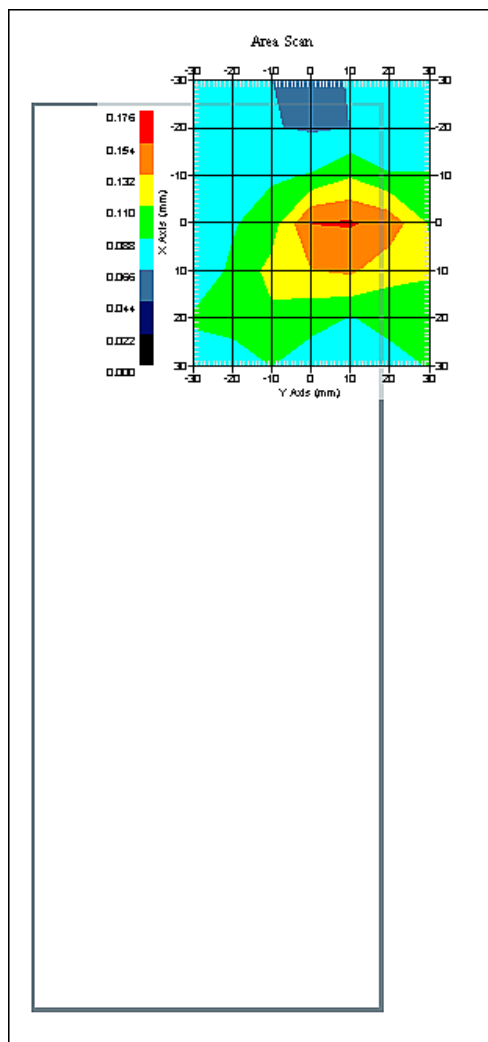


1 gram SAR value : 0.139 W/kg  
10 gram SAR value : 0.090 W/kg  
Area Scan Peak SAR : 0.156 W/kg  
Zoom Scan Peak SAR : 0.260 W/kg


**SAR-Z Axis**  
at Hotspot x:0.30 y:5.85

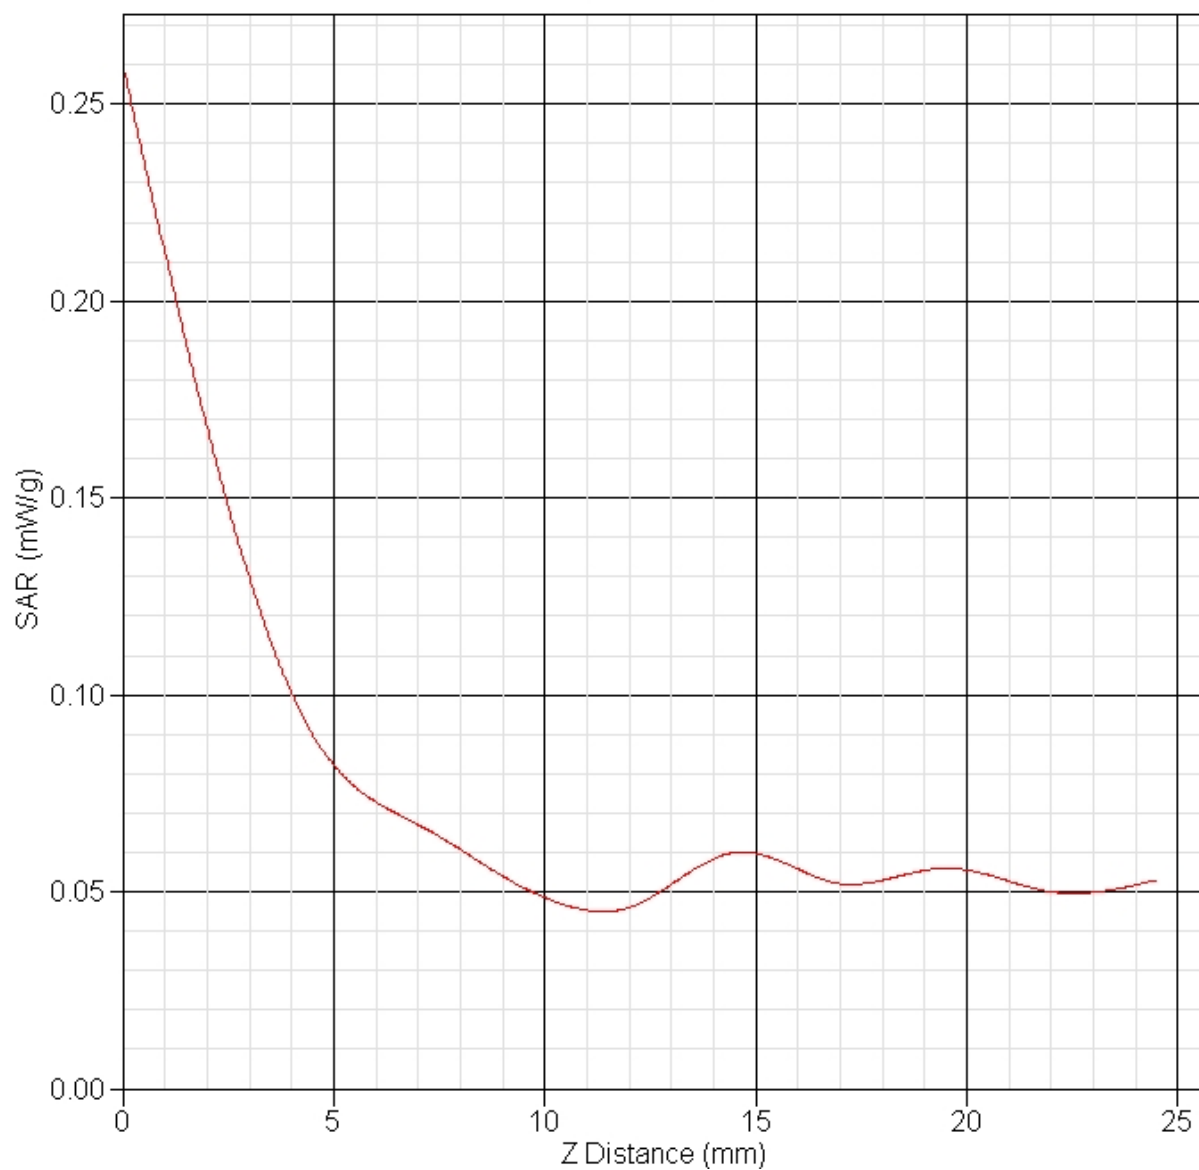


## Appendix C – SAR Test Setup Photos

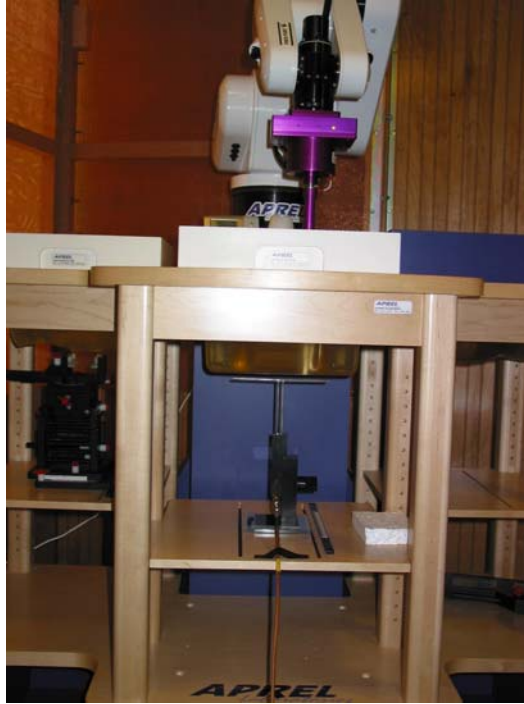

**System Body Configuration**

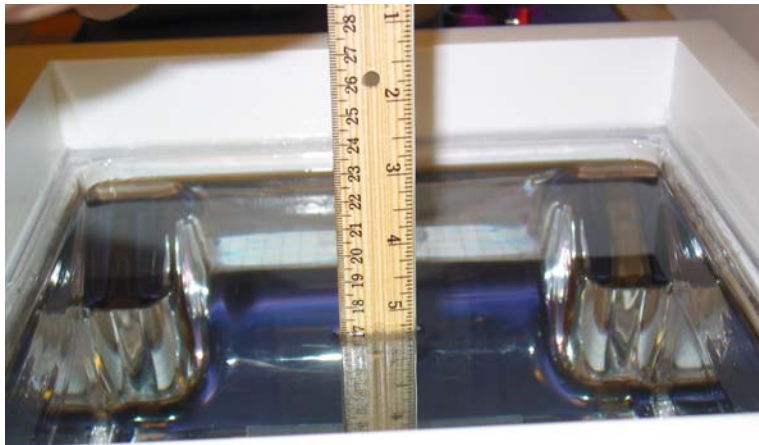

**Body Tissue Depth**

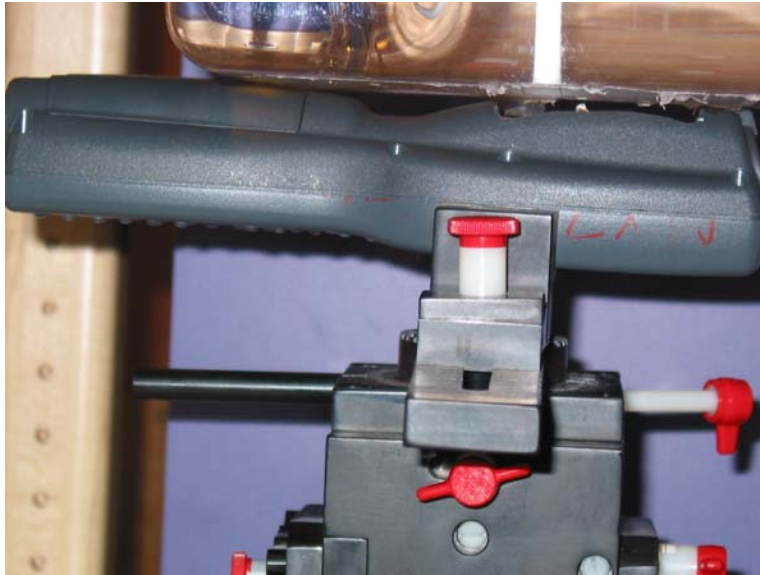

**Back Of Unit Configuration**




**Back Of Unit Configuration Close Up**



**Front of Device**



**Back of Device**

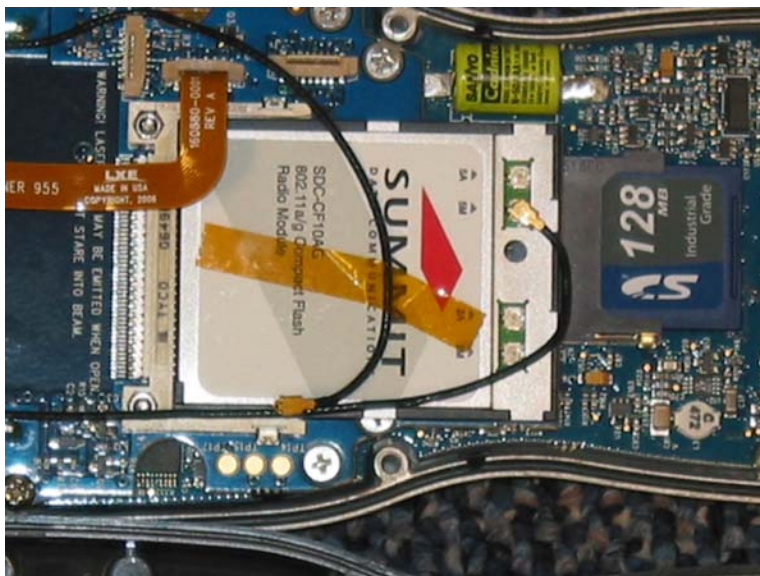


**Module Installed**




**Front of RF Module**



**Back of RF Module**

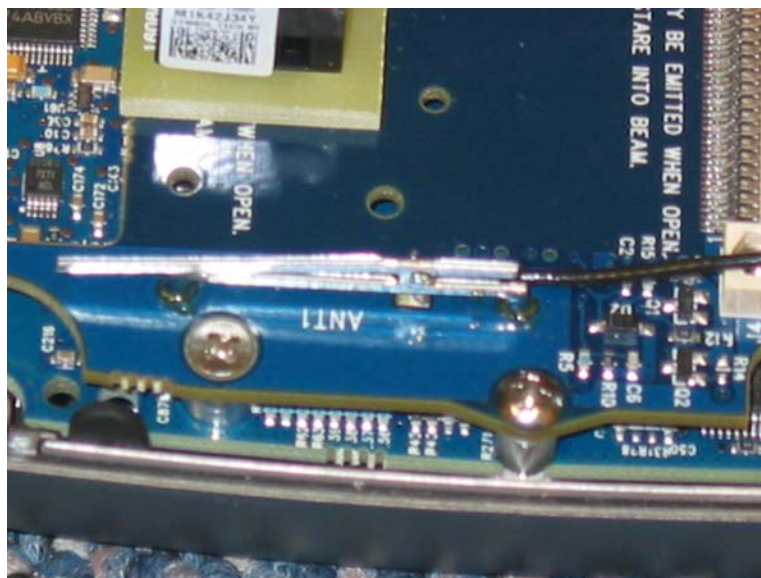

**Main Antenna**

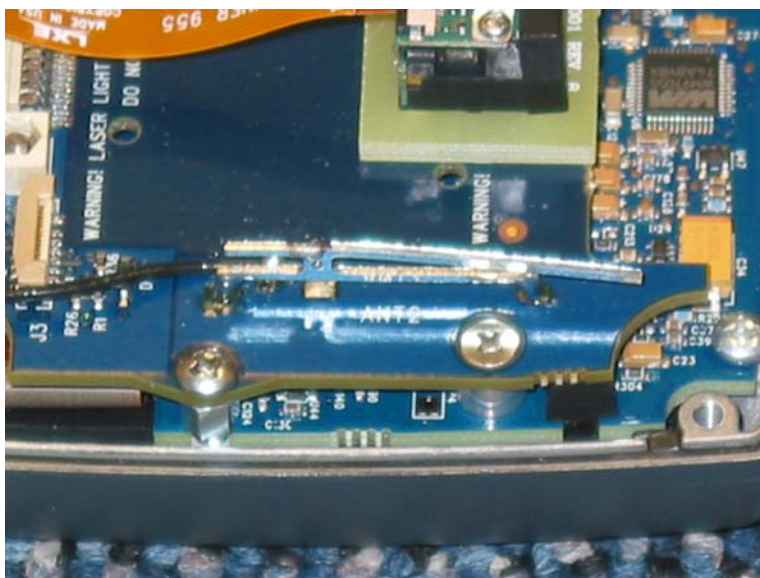

**Aux Antenna**

## Appendix D – Probe Calibration Data Sheets

# NCL CALIBRATION LABORATORIES

Calibration File No.: CP-844

Client.: RFEL

## CERTIFICATE OF CALIBRATION

It is certified that the equipment identified below has been calibrated in the  
**NCL CALIBRATION LABORATORIES** by qualified personnel following recognized  
procedures and using transfer standards traceable to NRC/NIST.

Equipment: Miniature Isotropic RF Probe 2450 MHz

BODY Calibration

Manufacturer: APREL Laboratories

Model No.: E-020

Serial No.: 217

Calibration Procedure: SSI/DRB-TP-D01-032-E020-V2

Project No: RFEB-ALS-E-020-5318

Calibrated: 3<sup>rd</sup> December 2007  
Released on: 3<sup>rd</sup> December 2007

This Calibration Certificate is Incomplete Unless Accompanied with the Calibration Results Summary  
This calibration has been conducted in line with the SCC ISO-IEC 17025 Scope of Accreditation  
Accredited Laboratory Number 48

Released By: \_\_\_\_\_

**NCL** CALIBRATION LABORATORIES

51 SPECTRUM WAY  
NEPEAN, ONTARIO  
CANADA K2R 1E6

Division of APREL Lab.  
TEL: (613) 820-4988  
FAX: (613) 820-4161

## Introduction

This Calibration Report reproduces the results of the calibration performed in line with the SSI/DRB-TP-D01-032-E020-V2 E-Field Probe Calibration Procedure. The results contained within this report are for APREL E-Field Probe E-020 217.

## References

SSI/DRB-TP-D01-032-E020-V2 E-Field Probe Calibration Procedure

IEEE 1528 "Recommended Practice for Determining the Peak Spatial-Average Specific Absorption Rate (SAR) in the Human Body Due to Wireless Communications Devices: Experimental Techniques"

SSI-TP-011 Tissue Calibration Procedure

IEC 62209 "Human exposure to radio frequency fields from hand-held and body-mounted wireless communication devices – Human models, instrumentation, and procedures –Part 1 & 2: Procedure to determine the Specific Absorption Rate (SAR) for hand-held devices used in close proximity of the ear (frequency range of 300 MHz to 3 GHz)"

IEEE 1309 Draft Standard for Calibration of Electromagnetic Field Sensors and Probes, Excluding Antennas, from 9kHz to 40GHz


## Conditions

Probe 217 was a re-calibration.

**Ambient Temperature of the Laboratory:** 22 °C +/- 0.5°C

**Temperature of the Tissue:** 21 °C +/- 0.5°C

**We the undersigned attest that to the best of our knowledge the calibration of this probe has been accurately conducted and that all information contained within this report has been reviewed for accuracy.**

  
-----  
**Stuart Nicol**  
-----  
**Jesse Hones**

## Calibration Results Summary

|                       |                     |
|-----------------------|---------------------|
| <b>Probe Type:</b>    | E-Field Probe E-020 |
| <b>Serial Number:</b> | 217                 |
| <b>Frequency:</b>     | 2450 MHz            |
| <b>Sensor Offset:</b> | 1.56 mm             |
| <b>Sensor Length:</b> | 2.5 mm              |
| <b>Tip Enclosure:</b> | Ertalyte*           |
| <b>Tip Diameter:</b>  | <5 mm               |
| <b>Tip Length:</b>    | 60 mm               |
| <b>Total Length:</b>  | 290 mm              |

\*Resistive to recommended tissue recipes per IEEE-1528

## Sensitivity in Air

|                                 |                                         |
|---------------------------------|-----------------------------------------|
| <b>Channel X:</b>               | $1.2 \mu\text{V}/(\text{V}/\text{m})^2$ |
| <b>Channel Y:</b>               | $1.2 \mu\text{V}/(\text{V}/\text{m})^2$ |
| <b>Channel Z:</b>               | $1.2 \mu\text{V}/(\text{V}/\text{m})^2$ |
| <b>Diode Compression Point:</b> | 95 mV                                   |

## **Sensitivity in Body Tissue Measured**

**Frequency:** 2450 MHz

**Epsilon:** 53.8 (+/-5%)      **Sigma:** 1.99 S/m (+/-5%)

### **ConvF**

**Channel X:** 3.61

**Channel Y:** 3.61

**Channel Z:** 3.61

Tissue sensitivity values were calculated using the load impedance of the APREL Laboratories Daq-Paq.


## **Boundary Effect:**

Uncertainty resulting from the boundary effect is less than 2% for the distance between the tip of the probe and the tissue boundary, when less than 2.44mm.



## **Spatial Resolution:**

The measured probe tip diameter is 5 mm (+/- 0.01 mm) and therefore meets the requirements of SSI/DRB-TP-D01-032 for spatial resolution.

## Receiving Pattern 2450 MHz (Air)

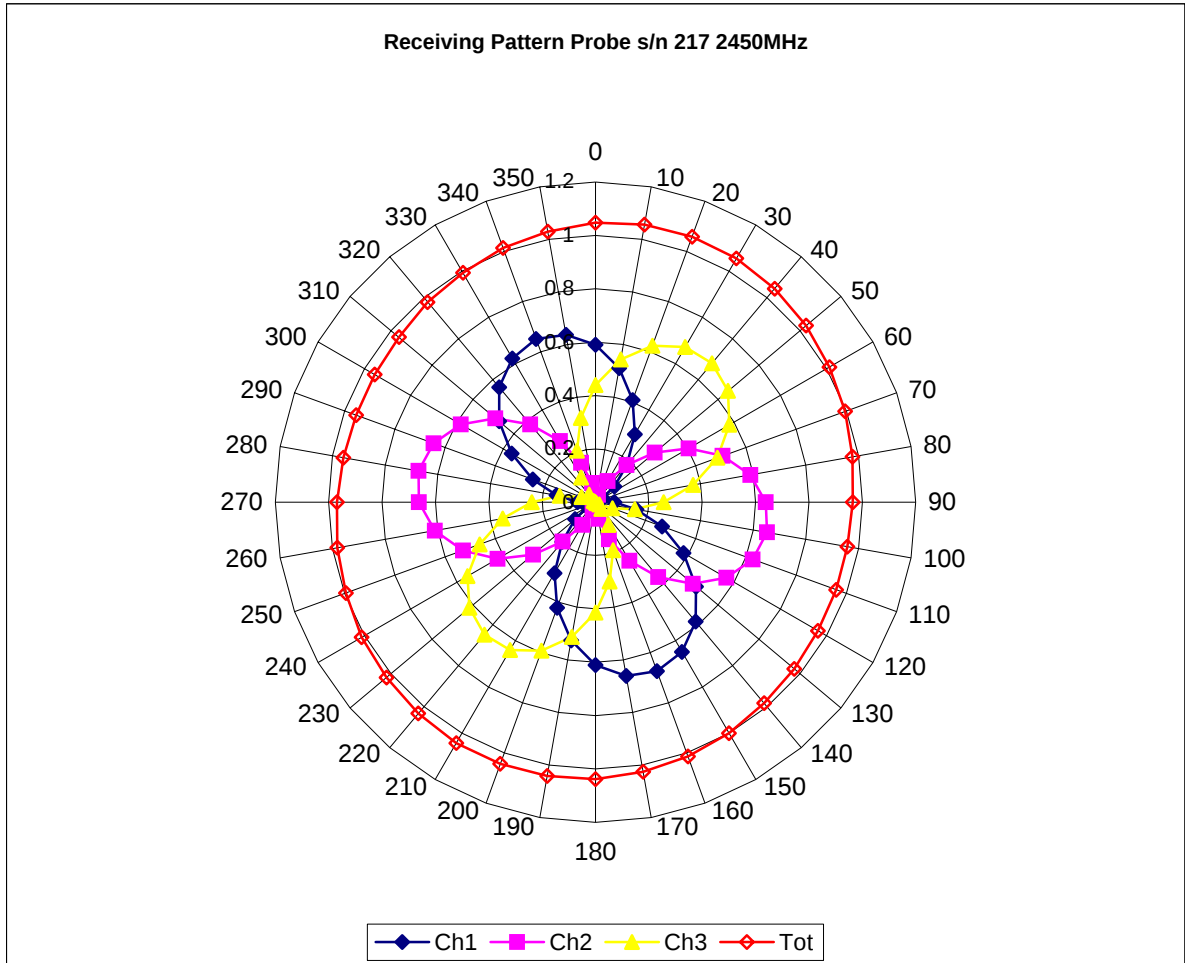


Isotropy Error 2450 MHz (Air)

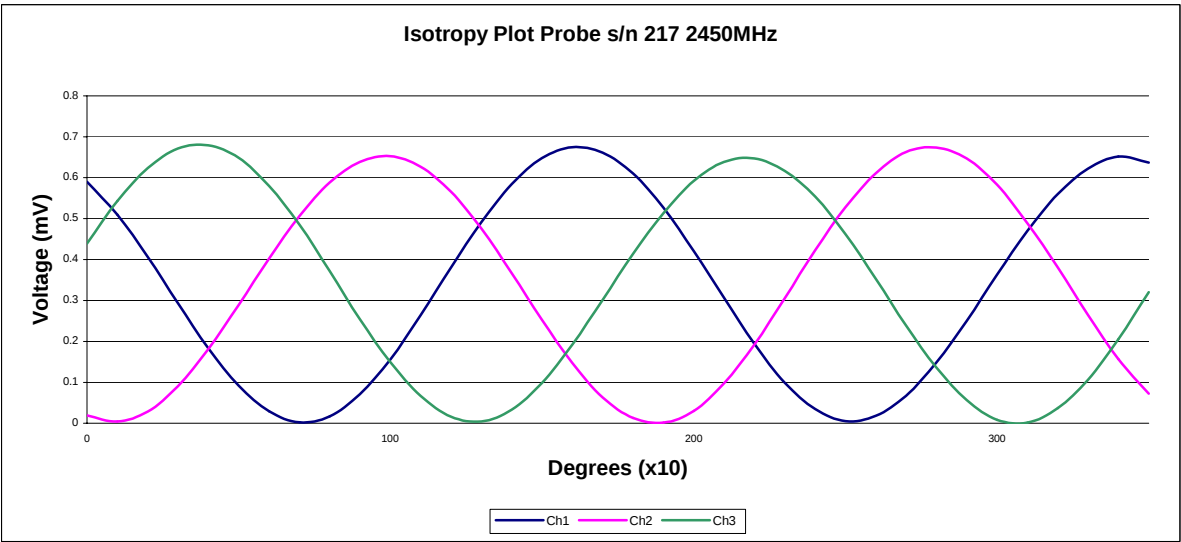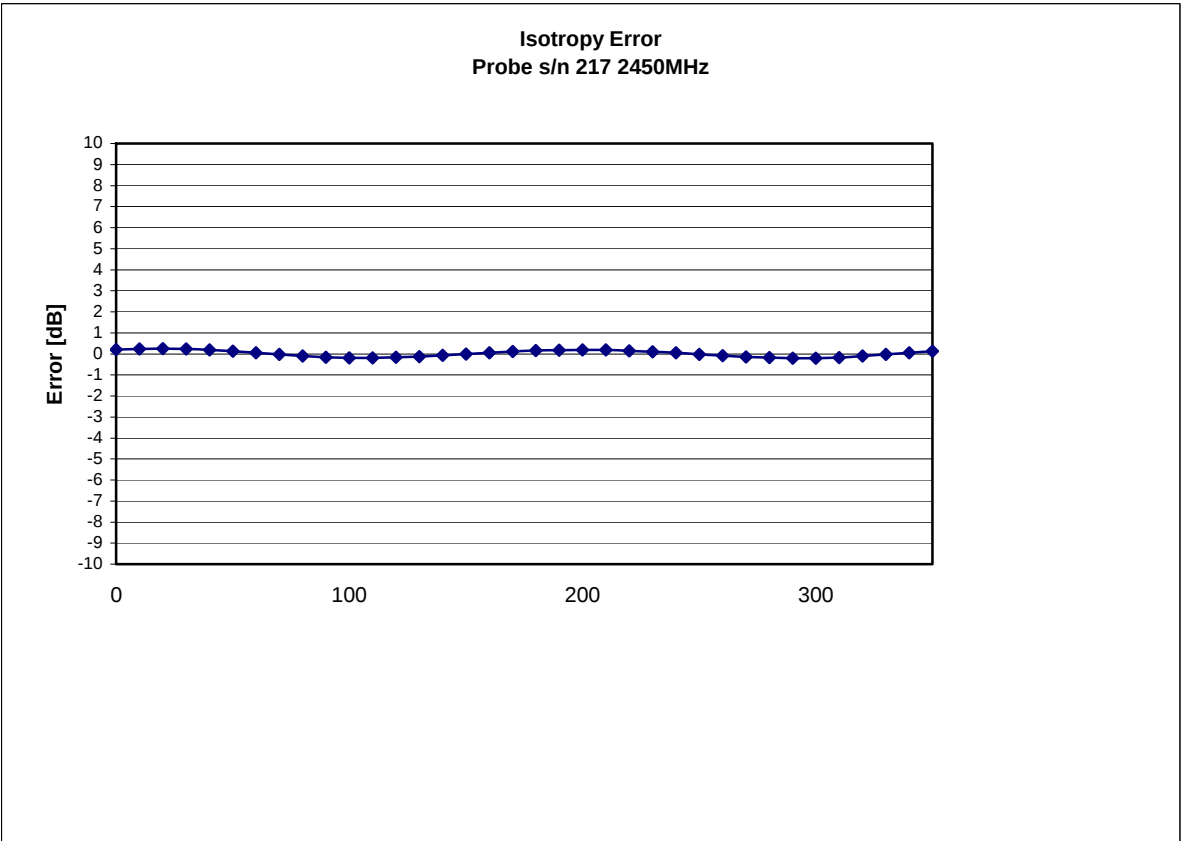


Isotropy Tissue:

0.10 dB

Dynamic Range

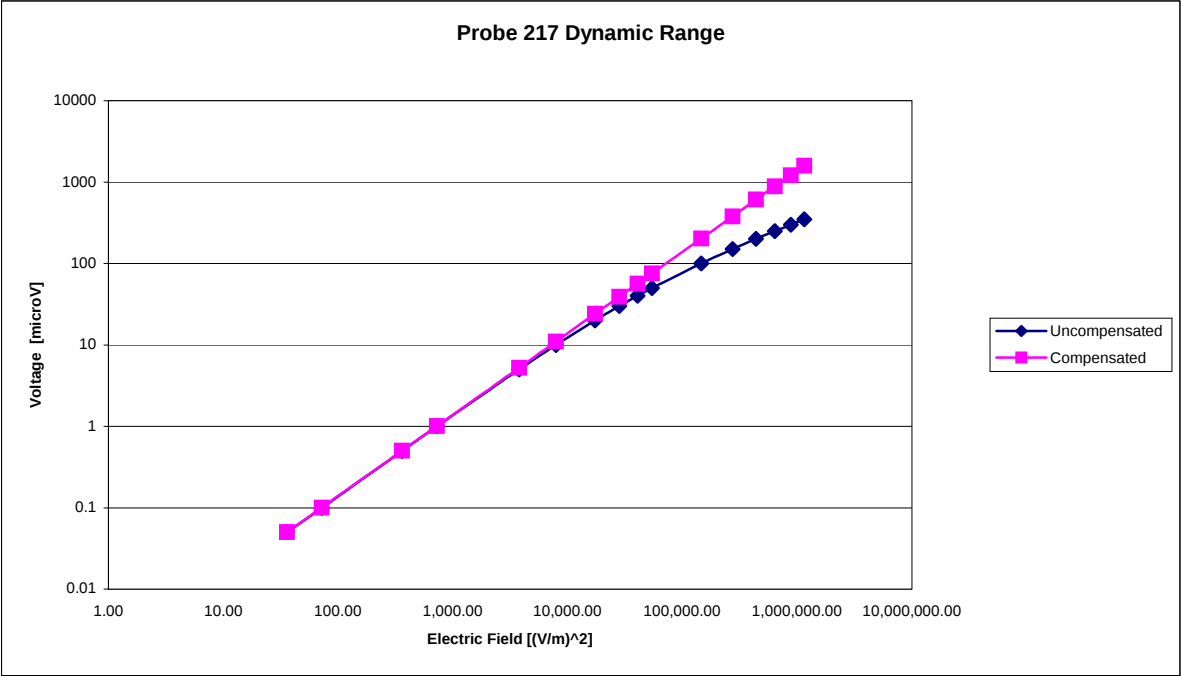

## Video Bandwidth

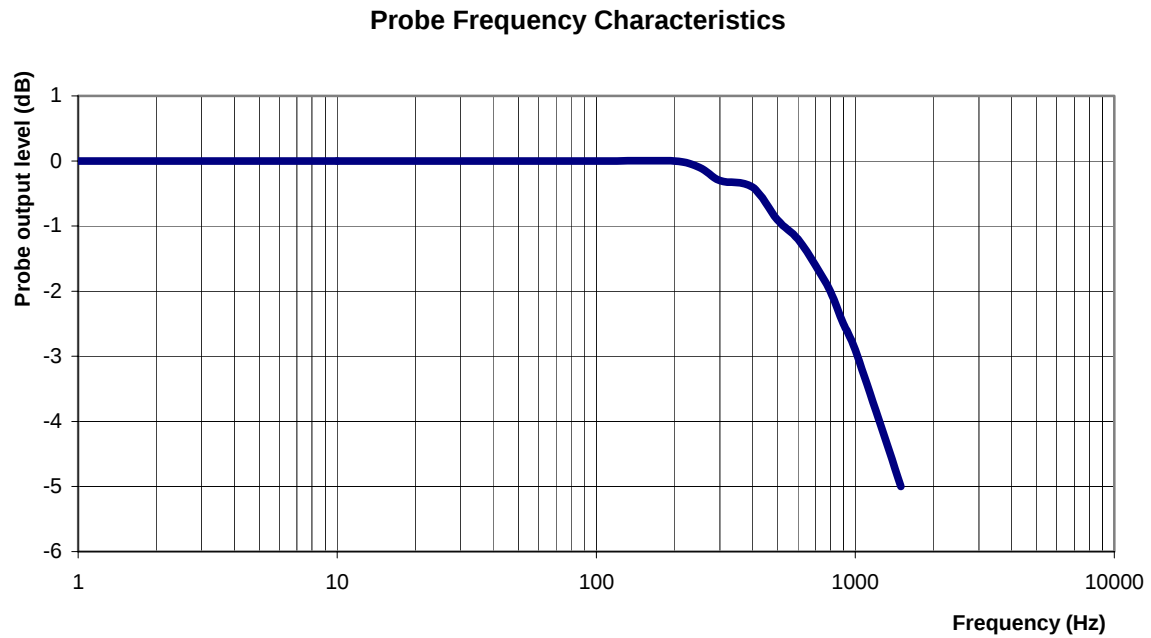

|                                     |             |
|-------------------------------------|-------------|
| <b>Video Bandwidth at 500 Hz</b>    | <b>1 dB</b> |
| <b>Video Bandwidth at 1.02 KHz:</b> | <b>3 dB</b> |

## **Conversion Factor Uncertainty Assessment**

### **Sensitivity in Body Tissue**

**Frequency:** 2450 MHz

**Epsilon:** 53.8 (+/-5%)

**Sigma:** 1.99 S/m (+/-5%)

#### **ConvF**

**Channel X:** 3.61 7%(K=2)

**Channel Y:** 3.61 7%(K=2)

**Channel Z:** 3.61 7%(K=2)

To minimize the uncertainty calculation all tissue sensitivity values were calculated using a load impedance of 5 M $\Omega$ .

#### **Boundary Effect:**

For a distance of 2.5mm the evaluated uncertainty (increase in the probe sensitivity) is less than 2%.

## **Test Equipment**

The test equipment used during Probe Calibration, manufacturer, model number and, current calibration status are listed and located on the main APREL server R:\NCL\Calibration Equipment\Instrument List May 2007.

# NCL CALIBRATION LABORATORIES

Calibration File No.: CP-752

Client.: APREL

## CERTIFICATE OF CALIBRATION

It is certified that the equipment identified below has been calibrated in the  
**NCL CALIBRATION LABORATORIES** by qualified personnel following recognized  
procedures and using transfer standards traceable to NRC/NIST.

Equipment: Miniature Isotropic RF Probe 5200 MHz

Manufacturer: APREL Laboratories

Model No.: E-030

Serial No.: AL-E3P1

Calibration in Body Tissue


Calibration Procedure: SSI/DRB-TP-D01-032-E020-V2

Project No: APLB-5200-PC-5264

Calibrated: 29<sup>th</sup> April 2007  
Released on: 30<sup>th</sup> April 2007

This Calibration Certificate is Incomplete Unless Accompanied with the Calibration Results Summary

Released By: \_\_\_\_\_

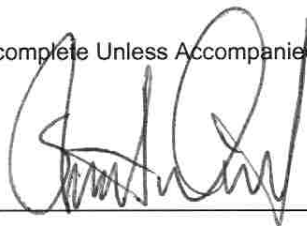

**NCL** CALIBRATION LABORATORIES

17 Bentley Avenue  
NEPEAN, ONTARIO  
CANADA K2E 6T7

Division of APREL Lab.  
TEL: (613) 820-4988  
FAX: (613) 820-4161

## Introduction

This Calibration Report reproduces the results of the calibration performed in line with the SSI/DRB-TP-D01-032-E020-V2 E-Field Probe Calibration Procedure. The results contained within this report are for APREL E-Field Probe E-030 AL-E3P1.

## References

SSI/DRB-TP-D01-032-E020-V2 E-Field Probe Calibration Procedure  
IEEE 1528 "Recommended Practice for Determining the Peak Spatial-Average Specific Absorption Rate (SAR) in the Human Body Due to Wireless Communications Devices: Experimental Techniques"  
SSI-TP-011 Tissue Calibration Procedure


## Conditions


Probe AL-E3P1 was a new probe taken from stock prior to calibration.

**Ambient Temperature of the Laboratory:** 22 °C +/- 0.5°C

**Temperature of the Tissue:** 21 °C +/- 0.5°C

**We the undersigned attest that to the best of our knowledge the calibration of this probe has been accurately conducted and that all information contained within this report has been reviewed for accuracy.**

  
-----  
**Stuart Nicol**

  
-----  
**Jesse Hones**

## Calibration Results Summary

|                       |                     |
|-----------------------|---------------------|
| <b>Probe Type:</b>    | E-Field Probe E-030 |
| <b>Serial Number:</b> | AL-E3P1             |
| <b>Frequency:</b>     | 5200 MHz            |
| <b>Sensor Offset:</b> | 0.56 mm             |
| <b>Sensor Length:</b> | 2.5 mm              |
| <b>Tip Enclosure:</b> | Ertalyte*           |
| <b>Tip Diameter:</b>  | <3 mm               |
| <b>Tip Length:</b>    | 60 mm               |
| <b>Total Length:</b>  | 290 mm              |

\*Resistive to recommended tissue recipes per IEEE-1528

## Sensitivity in Air

|                                 |                                         |
|---------------------------------|-----------------------------------------|
| <b>Channel X:</b>               | $1.2 \mu\text{V}/(\text{V}/\text{m})^2$ |
| <b>Channel Y:</b>               | $1.2 \mu\text{V}/(\text{V}/\text{m})^2$ |
| <b>Channel Z:</b>               | $1.2 \mu\text{V}/(\text{V}/\text{m})^2$ |
| <b>Diode Compression Point:</b> | 95 mV                                   |

## **Sensitivity in FCC Body Tissue**

**Frequency:** 5200 MHz

**Epsilon:** 48.9 (+/-10%)      **Sigma:** 5.35 S/m (+/-10%)

### **ConvF**

**Channel X:** 13

**Channel Y:** 13

**Channel Z:** 13

Tissue sensitivity values were calculated using the load impedance of the APREL Laboratories Daq-Paq.


## **Boundary Effect:**

Uncertainty resulting from the boundary effect is less than 2% for the distance between the tip of the probe and the tissue boundary, when less than 0.5mm.



## **Spatial Resolution:**

The measured probe tip diameter is less than 3 mm (+/- 0.01 mm) and therefore meets the requirements of SSI/DRB-TP-D01-032 for spatial resolution.

## Receiving Pattern 5200 MHz (Air)

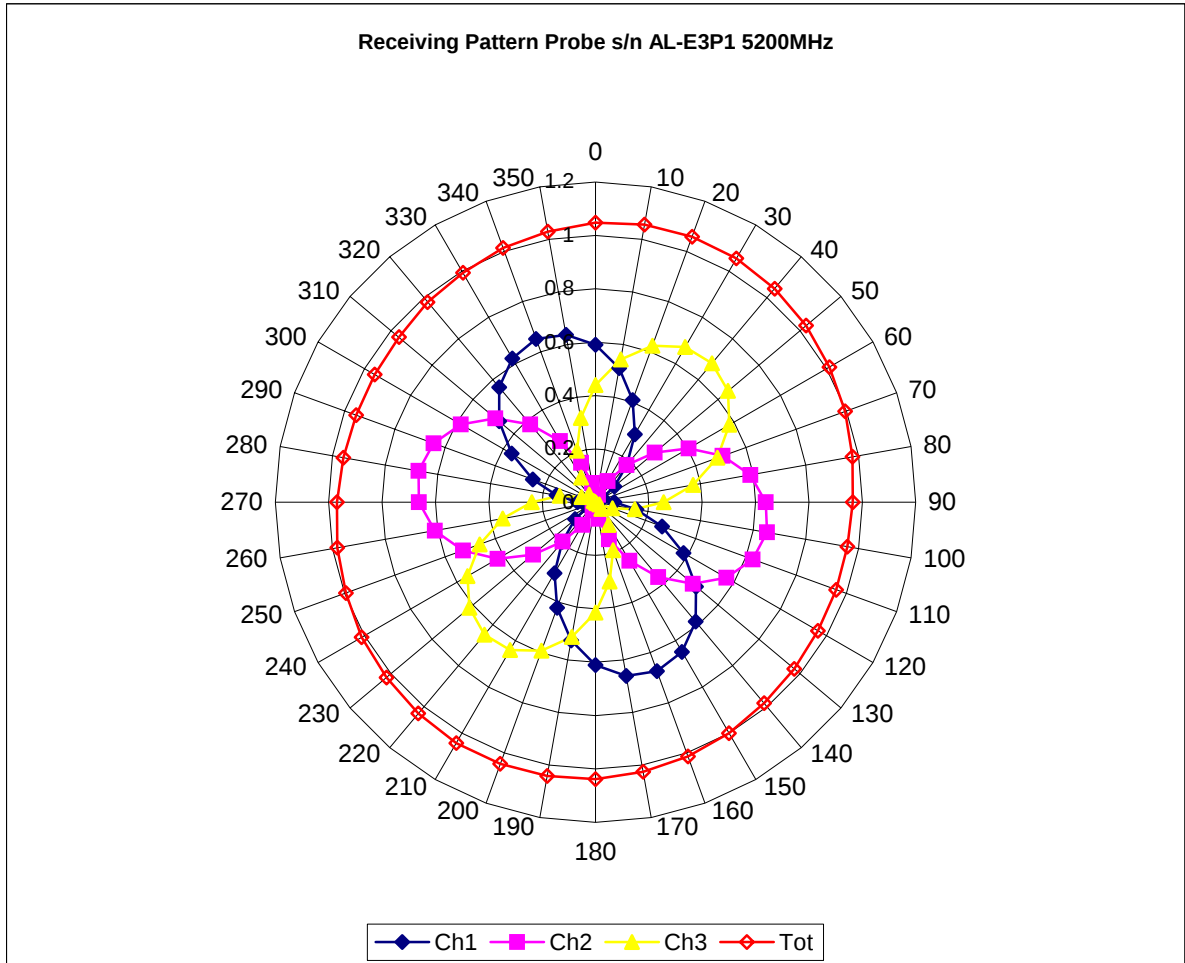


Isotropy Error 5200 MHz (Air)

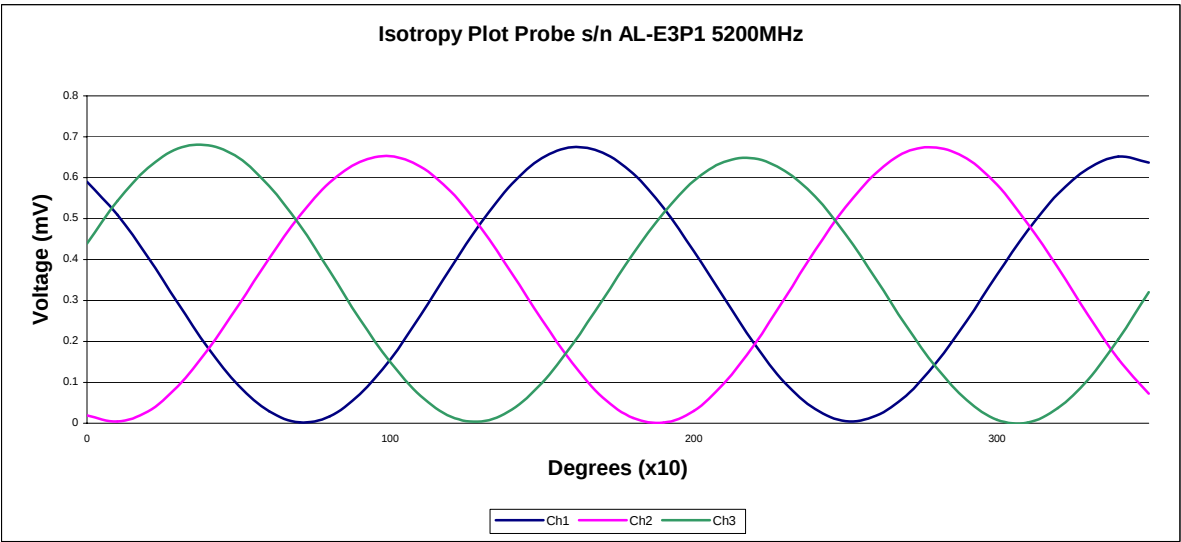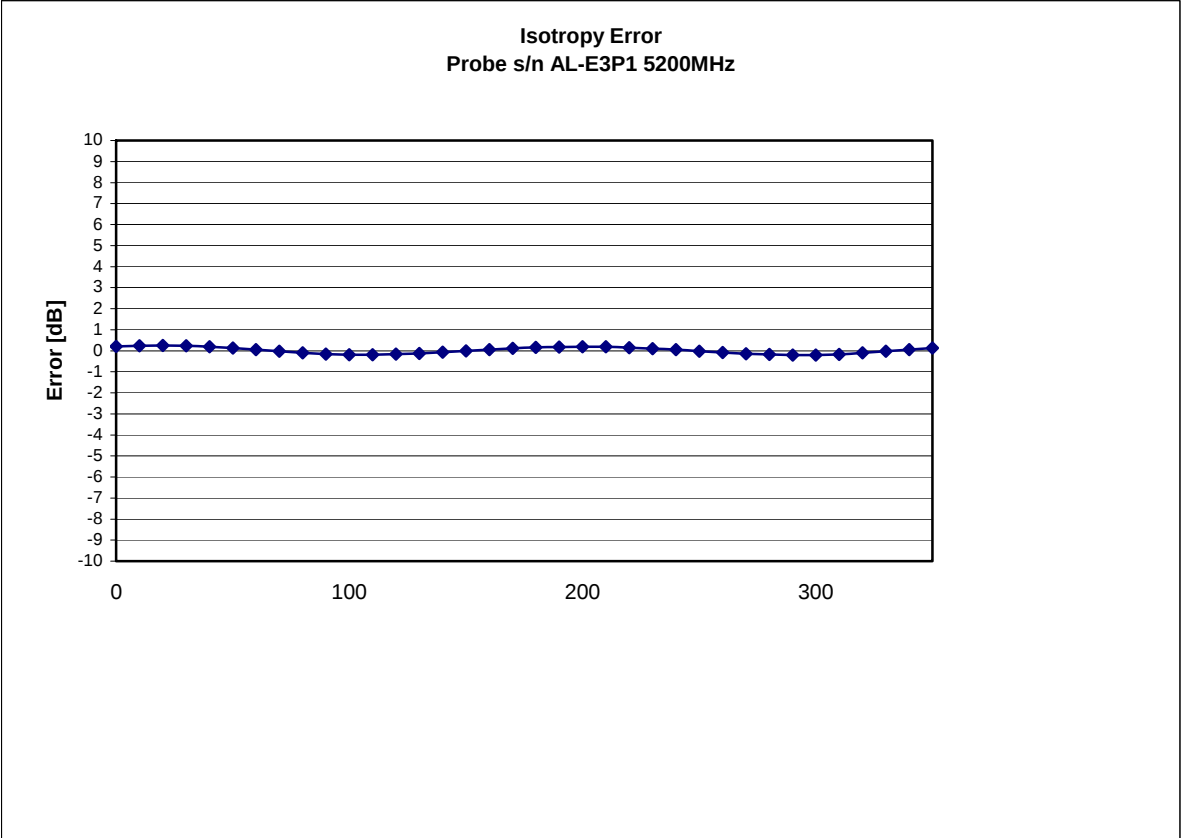


Isotropy in Tissue:

0.15 dB

Dynamic Range

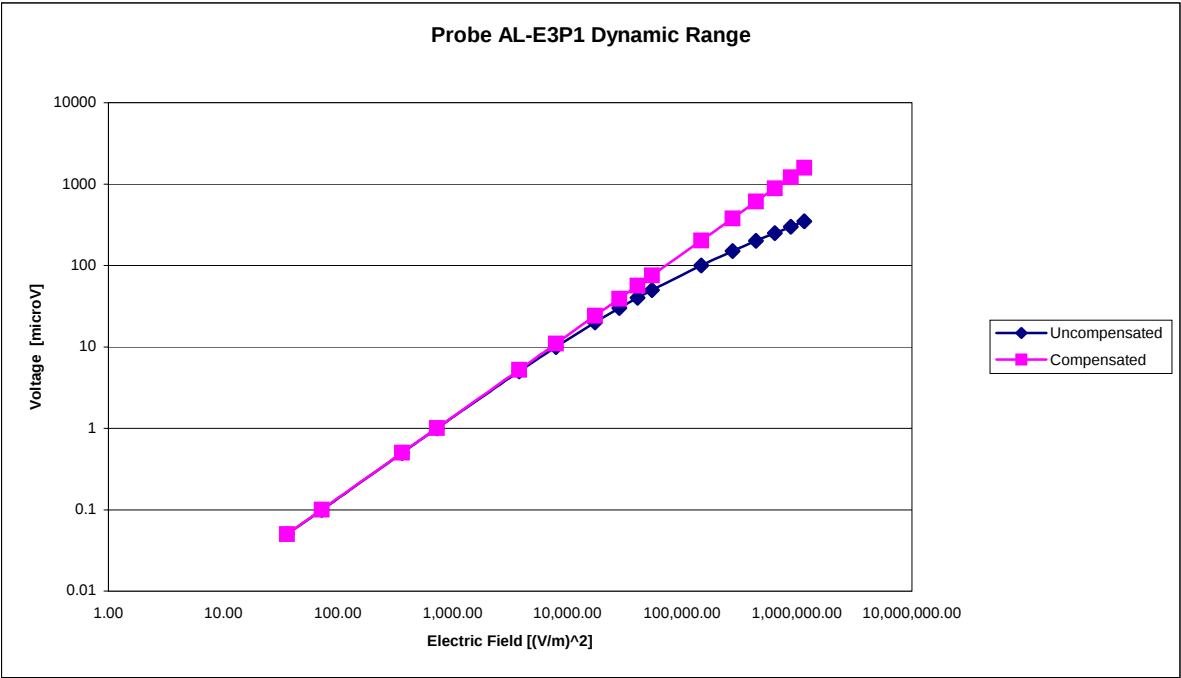

## Video Bandwidth

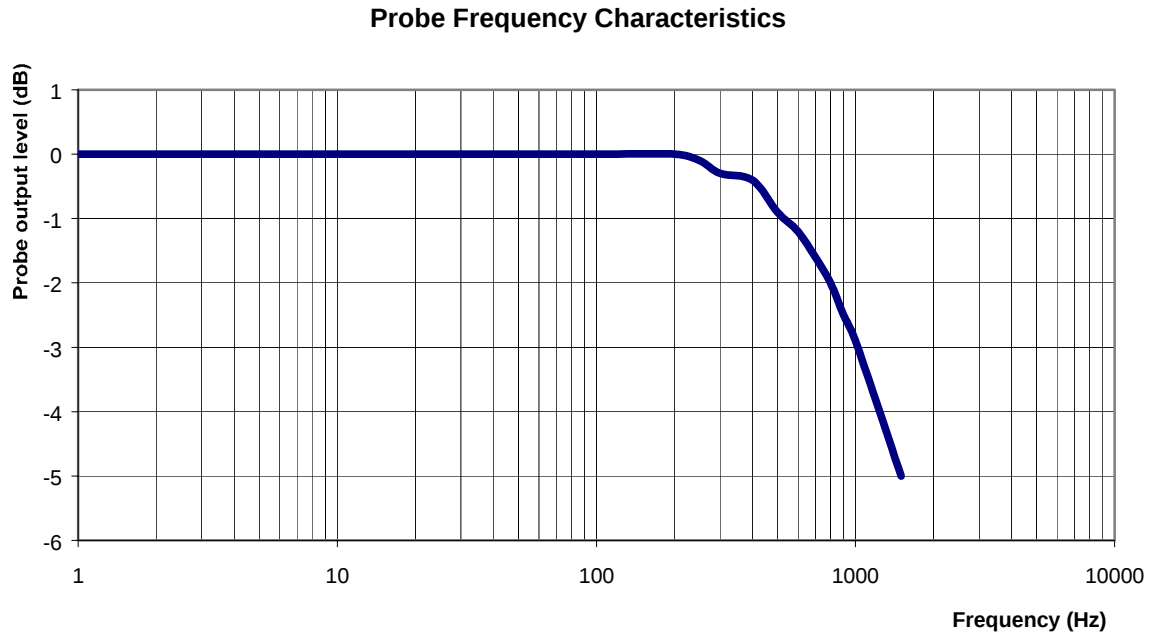

|                                     |             |
|-------------------------------------|-------------|
| <b>Video Bandwidth at 500 Hz</b>    | <b>1 dB</b> |
| <b>Video Bandwidth at 1.02 KHz:</b> | <b>3 dB</b> |

## **Conversion Factor Uncertainty Assessment**

**Frequency:** 5200 MHz

**Epsilon:** 48.9 (+/-10%)

**Sigma:** 5.35 S/m (+/-10%)

### **ConvF**

**Channel X:** 13 7%(K=2)

**Channel Y:** 13 7%(K=2)

**Channel Z:** 13 7%(K=2)

To minimize the uncertainty calculation all tissue sensitivity values were calculated using a load impedance of 5 M $\Omega$ .

### **Boundary Effect:**

For a distance of 0.5 mm the evaluated uncertainty (increase in the probe sensitivity) is less than 2%.

## **Test Equipment**

The test equipment used during Probe Calibration, manufacturer, model number and, current calibration status are listed and located on the main APREL server R:\NCL\Calibration Equipment\Instrument List May 2006.

# NCL CALIBRATION LABORATORIES

Calibration File No.: CP-754

Client.: APREL

## CERTIFICATE OF CALIBRATION

It is certified that the equipment identified below has been calibrated in the  
**NCL CALIBRATION LABORATORIES** by qualified personnel following recognized  
procedures and using transfer standards traceable to NRC/NIST.

Equipment: Miniature Isotropic RF Probe 5800 MHz

Manufacturer: APREL Laboratories

Model No.: E-030

Serial No.: AL-E3P1

Calibration in Body Tissue


Calibration Procedure: SSI/DRB-TP-D01-032-E020-V2

Project No: APLB-5800-PC-5264

Calibrated: 30<sup>th</sup> April 2007  
Released on: 30<sup>th</sup> April 2007

This Calibration Certificate is Incomplete Unless Accompanied with the Calibration Results Summary

Released By: \_\_\_\_\_

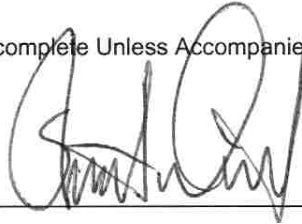

---

**NCL CALIBRATION LABORATORIES**

17 Bentley Avenue  
NEPEAN, ONTARIO  
CANADA K2E 6T7

Division of APREL Lab.  
TEL: (613) 820-4988  
FAX: (613) 820-4161

## Introduction

This Calibration Report reproduces the results of the calibration performed in line with the SSI/DRB-TP-D01-032-E020-V2 E-Field Probe Calibration Procedure. The results contained within this report are for APREL E-Field Probe E-030 AL-E3P1.

## References

SSI/DRB-TP-D01-032-E020-V2 E-Field Probe Calibration Procedure  
IEEE 1528 "Recommended Practice for Determining the Peak Spatial-Average Specific Absorption Rate (SAR) in the Human Body Due to Wireless Communications Devices: Experimental Techniques"  
SSI-TP-011 Tissue Calibration Procedure



## Conditions

Probe AL-E3P1 was a new probe taken from stock prior to calibration.

**Ambient Temperature of the Laboratory:** 22 °C +/- 0.5°C

**Temperature of the Tissue:** 21 °C +/- 0.5°C

We the undersigned attest that to the best of our knowledge the calibration of this probe has been accurately conducted and that all information contained within this report has been reviewed for accuracy.

  
-----  
**Stuart Nicol**  
-----  
**Jesse Hones**

## Calibration Results Summary

|                       |                     |
|-----------------------|---------------------|
| <b>Probe Type:</b>    | E-Field Probe E-030 |
| <b>Serial Number:</b> | AL-E3P1             |
| <b>Frequency:</b>     | 5800 MHz            |
| <b>Sensor Offset:</b> | 0.56 mm             |
| <b>Sensor Length:</b> | 2.5 mm              |
| <b>Tip Enclosure:</b> | Ertalyte*           |
| <b>Tip Diameter:</b>  | <3 mm               |
| <b>Tip Length:</b>    | 60 mm               |
| <b>Total Length:</b>  | 290 mm              |

\*Resistive to recommended tissue recipes per IEEE-1528

## Sensitivity in Air

|                                 |                                         |
|---------------------------------|-----------------------------------------|
| <b>Channel X:</b>               | $1.2 \mu\text{V}/(\text{V}/\text{m})^2$ |
| <b>Channel Y:</b>               | $1.2 \mu\text{V}/(\text{V}/\text{m})^2$ |
| <b>Channel Z:</b>               | $1.2 \mu\text{V}/(\text{V}/\text{m})^2$ |
| <b>Diode Compression Point:</b> | 95 mV                                   |

## **Sensitivity in FCC Body Tissue**

**Frequency:** 5800 MHz

**Epsilon:** 48.2 (+/-10%)      **Sigma:** 6.0 S/m (+/-10%)

### **ConvF**

**Channel X:** 14

**Channel Y:** 14

**Channel Z:** 14

Tissue sensitivity values were calculated using the load impedance of the APREL Laboratories Daq-Paq.


## **Boundary Effect:**

Uncertainty resulting from the boundary effect is less than 2% for the distance between the tip of the probe and the tissue boundary, when less than 0.5mm.



## **Spatial Resolution:**

The measured probe tip diameter is less than 3 mm (+/- 0.01 mm) and therefore meets the requirements of SSI/DRB-TP-D01-032 for spatial resolution.

## Receiving Pattern 5800 MHz (Air)

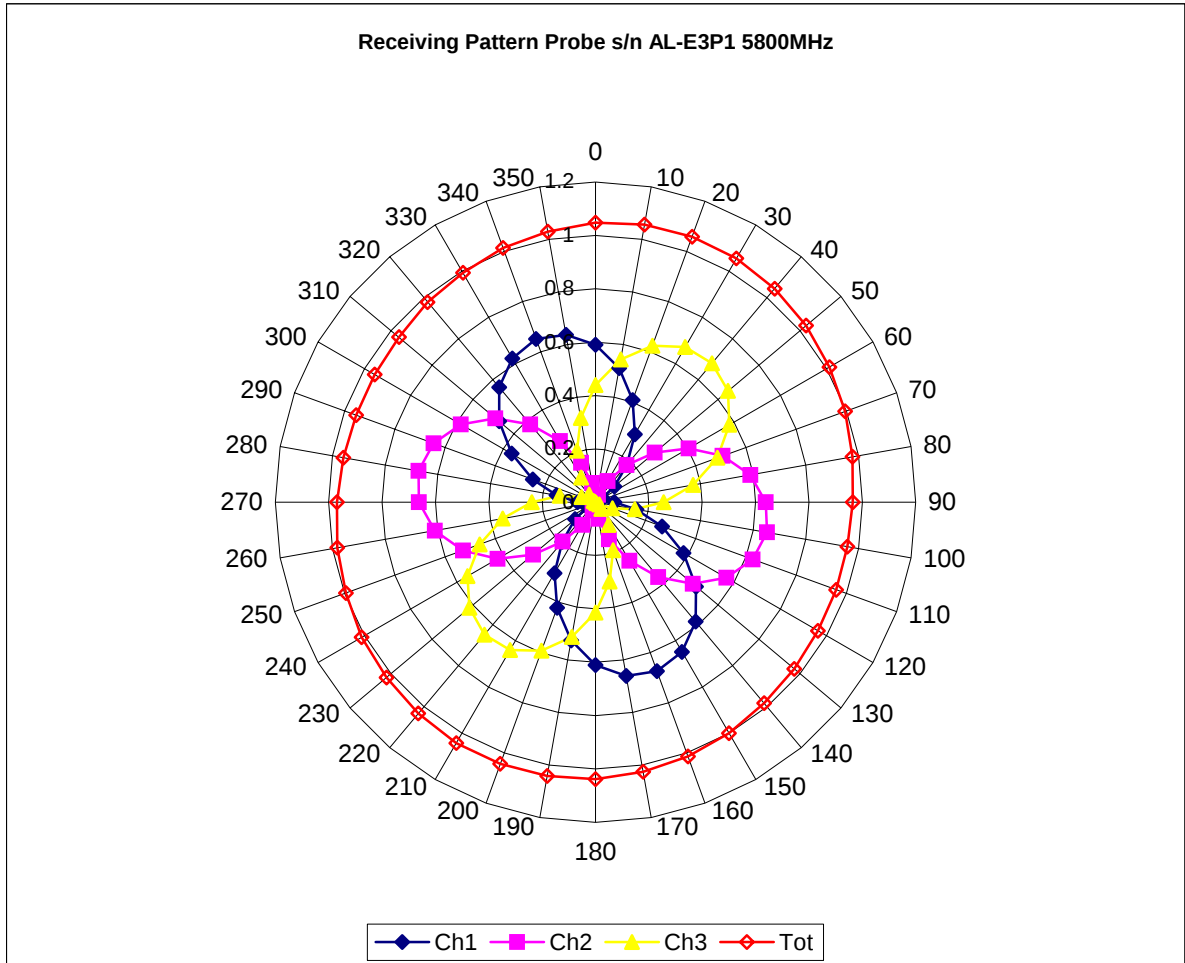


Isotropy Error 5800 MHz (Air)

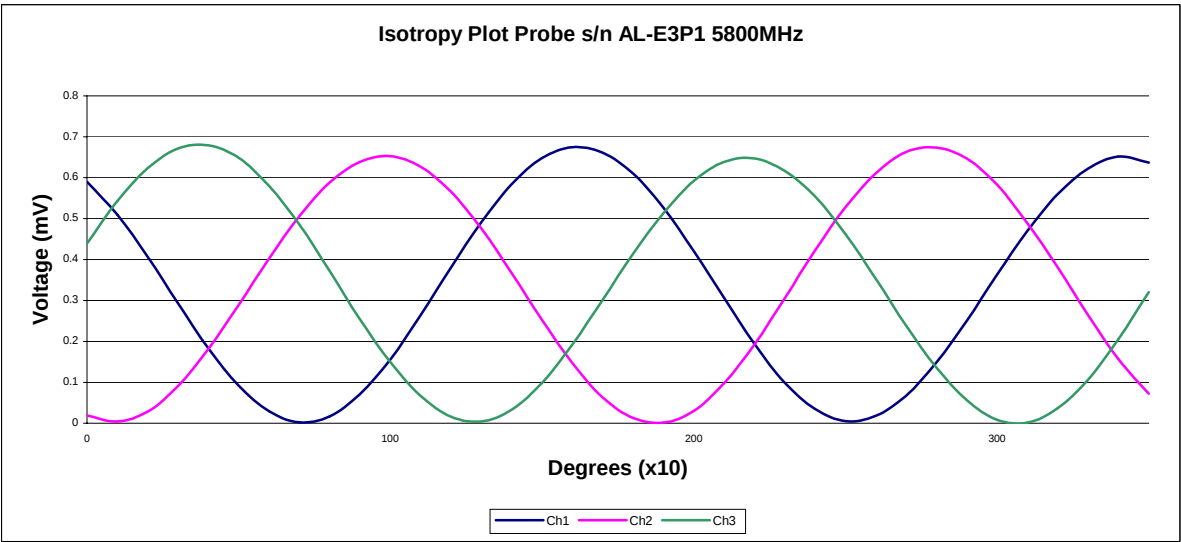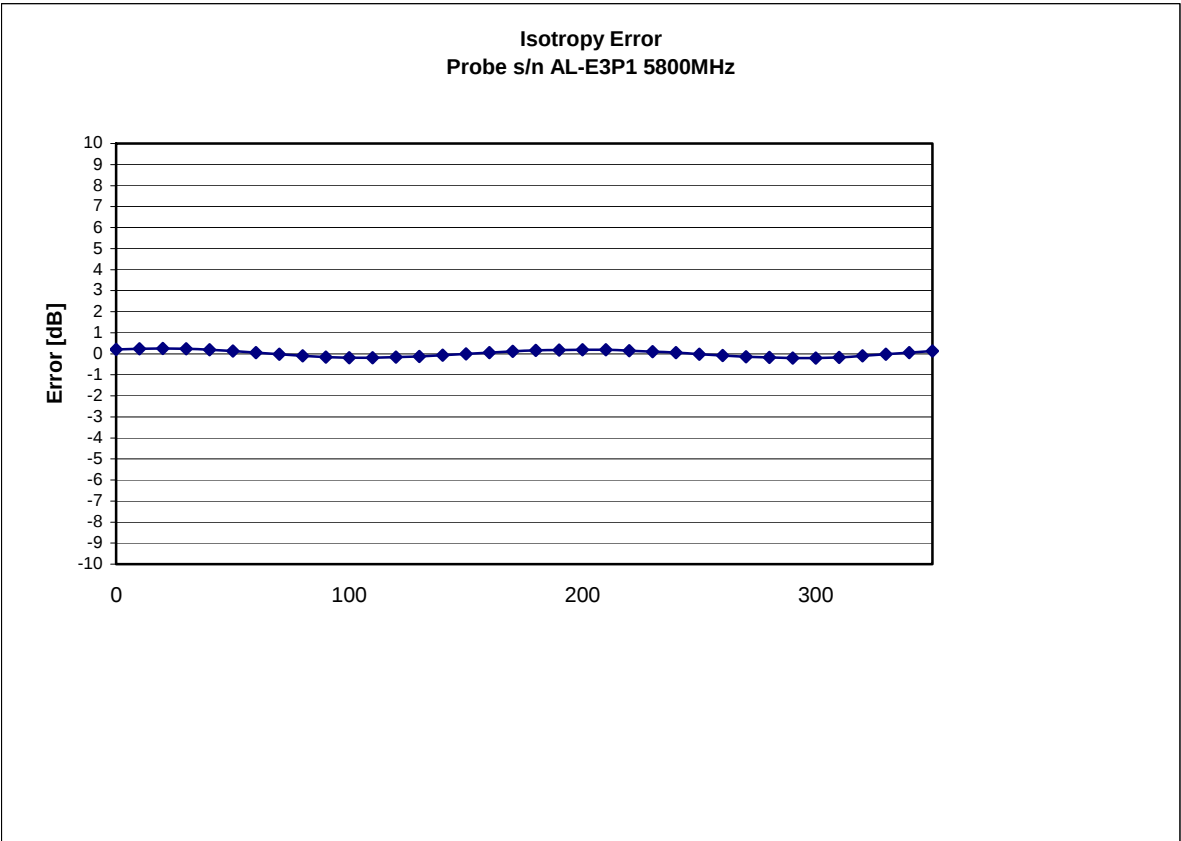


Isotropy in Tissue:

0.15 dB

Dynamic Range

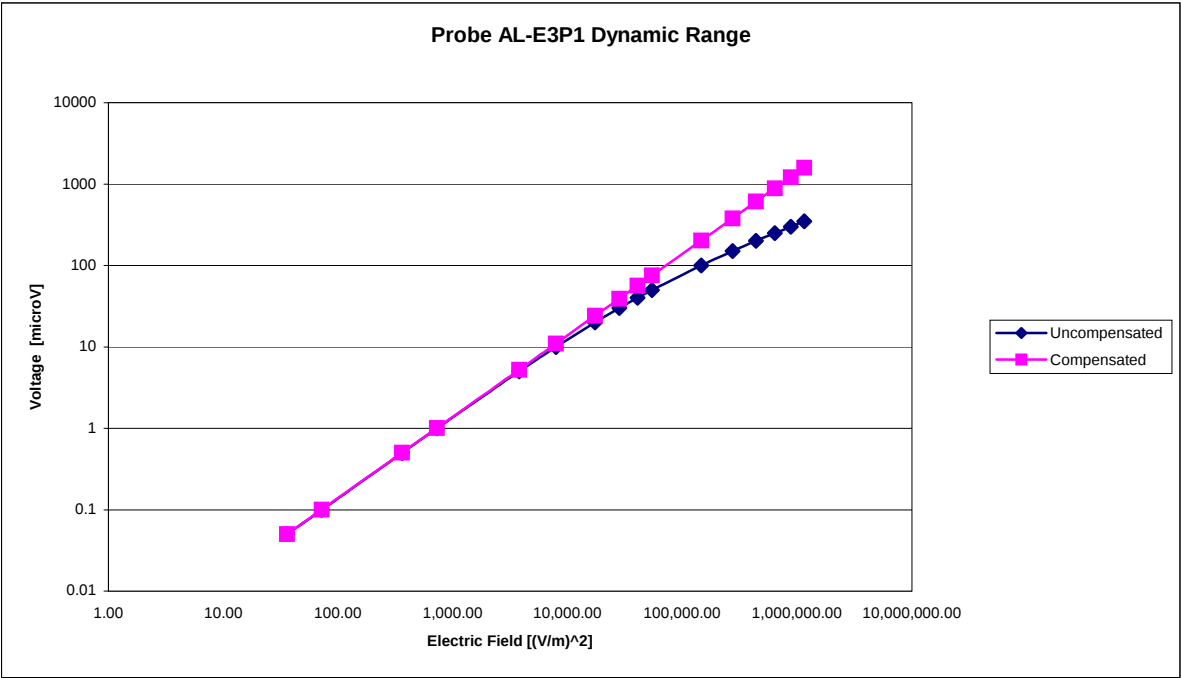

## Video Bandwidth

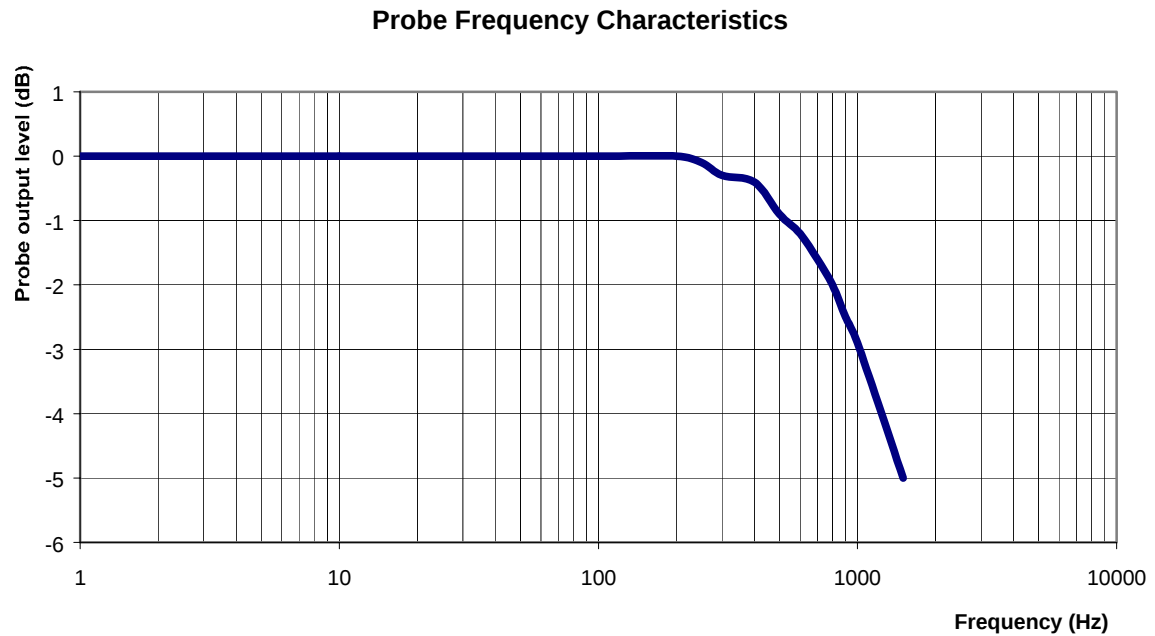

**Video Bandwidth at 500 Hz**                      1 dB  
**Video Bandwidth at 1.02 KHz:**                3 dB

## **Conversion Factor Uncertainty Assessment**

**Frequency:**

5800 MHz

**Epsilon:** 48.4 (+/-10%)

**Sigma:** 6.0 S/m (+/-10%)

**ConvF**

**Channel X:** 14

7%(K=2)

**Channel Y:** 14

7%(K=2)

**Channel Z:** 14

7%(K=2)

To minimize the uncertainty calculation all tissue sensitivity values were calculated using a load impedance of 5 M $\Omega$ .

### **Boundary Effect:**

For a distance of 0.5 mm the evaluated uncertainty (increase in the probe sensitivity) is less than 2%.

## **Test Equipment**

The test equipment used during Probe Calibration, manufacturer, model number and, current calibration status are listed and located on the main APREL server R:\NCL\Calibration Equipment\Instrument List May 2006.

## Appendix E – Dipole Calibration Data Sheets

## RF Exposure Lab, LLC

Calibration File No: CAL.20080201

### CERTIFICATE OF CALIBRATION

It is certified that the equipment identified below has been calibrated at RF Exposure Lab, LLC by qualified personnel following recognized procedures and using transfer standards traceable to NRC/NIST.

#### Validation Dipole

Manufacturer: APREL Laboratories

Part Number: ALS-D-2450-S-2

Frequency: 2.4 GHz

Serial No: RFE-278

Manufactured: 20 February 2004  
Calibrated: 20 February 2008

Calibrated By: Signature on File  
Jay Moulton – Technical Manager

Approved By: Signature on File  
Tamara Moulton – Quality Manager

Measurement Uncertainty:

|                     |      |
|---------------------|------|
| Repeatability:      | 23%  |
| Tissue Uncertainty: | 3.2% |
| Network Analyzer:   | 25%  |



## RF EXPOSURE LAB, LLC

2867 Progress Place, Suite 4D  
Escondido, CA 92029

Tel: (760) 737-3131  
FAX: (760) 737-9131

## Calibration Results Summary

The following results relate to the Calibrated Dipole and should be used as a quick reference for the user.

### Mechanical Dimensions

**Length:** 51.5 mm  
**Height:** 30.5 mm

### Electrical Specifications

#### Head

**SWR:** 1.0953 U  
**Return Loss:** -29.601 dB  
**Impedance:** 53.854  $\Omega$

### System Validation Results

| Frequency | 1 Gram | 10 Gram |
|-----------|--------|---------|
| 2.45 GHz  | 52.880 | 24.500  |

#### Body

**SWR:** 1.1354 U  
**Return Loss:** -31.173 dB  
**Impedance:** 54.146  $\Omega$

### System Validation Results

| Frequency | 1 Gram | 10 Gram |
|-----------|--------|---------|
| 2.45 GHz  | 53.550 | 24.710  |

## Head Measurement Conditions

The measurements were performed in the Uni-Phantom filled with head simulating liquid of the following electrical parameters at 2450 MHz:

|                        |            |           |
|------------------------|------------|-----------|
| Relative Dielectricity | 39.37      | $\pm 5\%$ |
| Conductivity           | 1.78 mho/m | $\pm 5\%$ |

The APREL Laboratories ALSAS system with a dosimetric E-field probe E-020 (SN:217, Conversion factor 3.4 at 2450 MHz) was used for the measurements.

The dipole was mounted so that the dipole feed point was positioned below the center marking of the flat phantom and the dipole was oriented parallel to the body axis (the long side of the phantom). The standard measuring distance was 10mm from the dipole center to the solution surface.

The coarse grid with a grid spacing of 10mm was aligned with the dipole. The 5x5x8 fine cube was chosen for cube integration. The dipole input power (forward power) was 100mW  $\pm 3\%$ . The results are normalized to 1W input power.

The laboratories environmental conditions were as follows during the calibration sequence.

|                                        |                    |
|----------------------------------------|--------------------|
| Ambient Temperature of the Laboratory: | 24 °C $\pm 1.0$ °C |
| Temperature of the Tissue:             | 20 °C $\pm 1.0$ °C |
| Relative Humidity:                     | 41%                |


## SAR Measurement

Standard SAR measurements were performed according to the measurement conditions described above. The results have been normalized to a dipole input power of 1W (forward power). The resulting averaged SAR values measured with the dosimetric probe E-020 SN:217 and applying the advanced extrapolation are:

Averaged over 1 cm<sup>3</sup> (1 g) of tissue: 52.880 mW/g  $\pm$  19.7% (k=2)<sup>1</sup>

Averaged over 10 cm<sup>3</sup> (10 g) of tissue: 24.500 mW/g  $\pm$  19.4% (k=2)<sup>1</sup>

### Area Scan

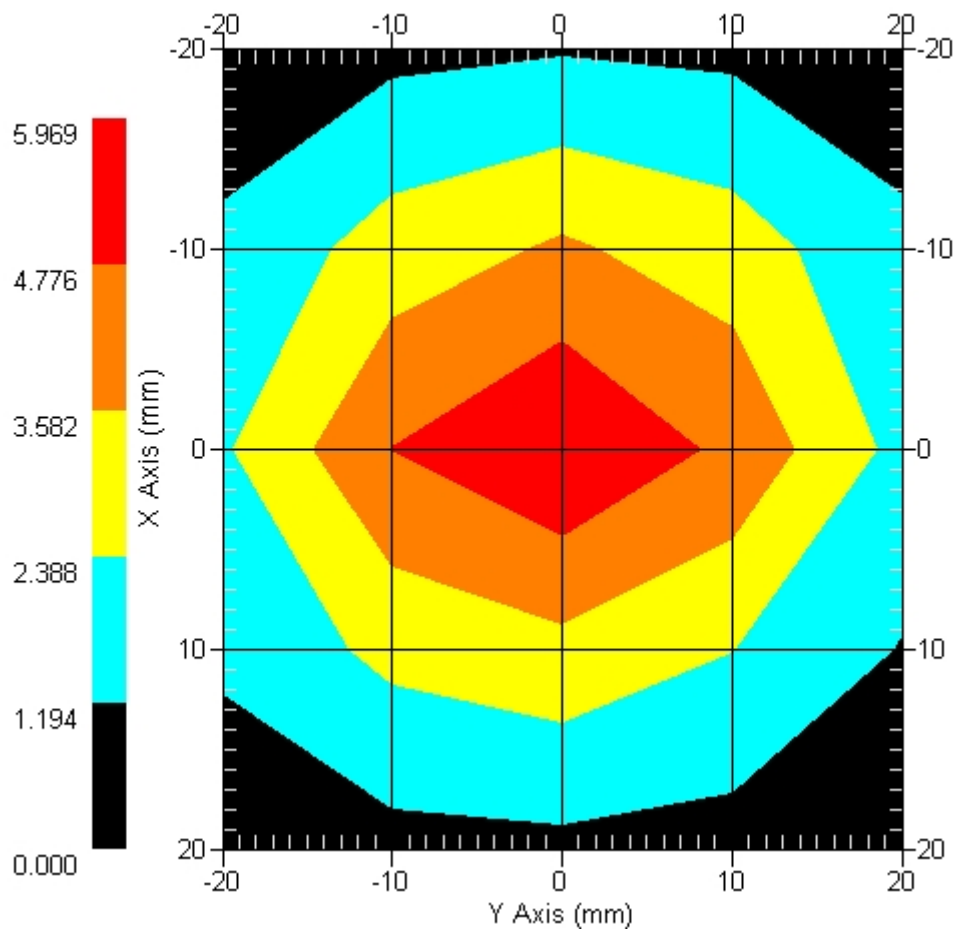

1 gram SAR value : 5.288 W/kg  
 10 gram SAR value : 2.450 W/kg  
 Area Scan Peak SAR : 5.969 W/kg  
 Zoom Scan Peak SAR : 10.890 W/kg

<sup>1</sup> validation uncertainty


## Dipole Impedance and Return Loss

The impedance was measured at the SMA connector with a network analyzer. The dipole was positioned at the flat phantom sections according to measurement conditions stated above during impedance measurements.


| Test      | Result          |
|-----------|-----------------|
| S11 R/L   | -29.601 dB      |
| SWR       | 1.0953 U        |
| Impedance | 53.854 $\Omega$ |

The following graphs are the results as displayed on the Vector Network Analyzer.


### S11 Parameter Return Loss

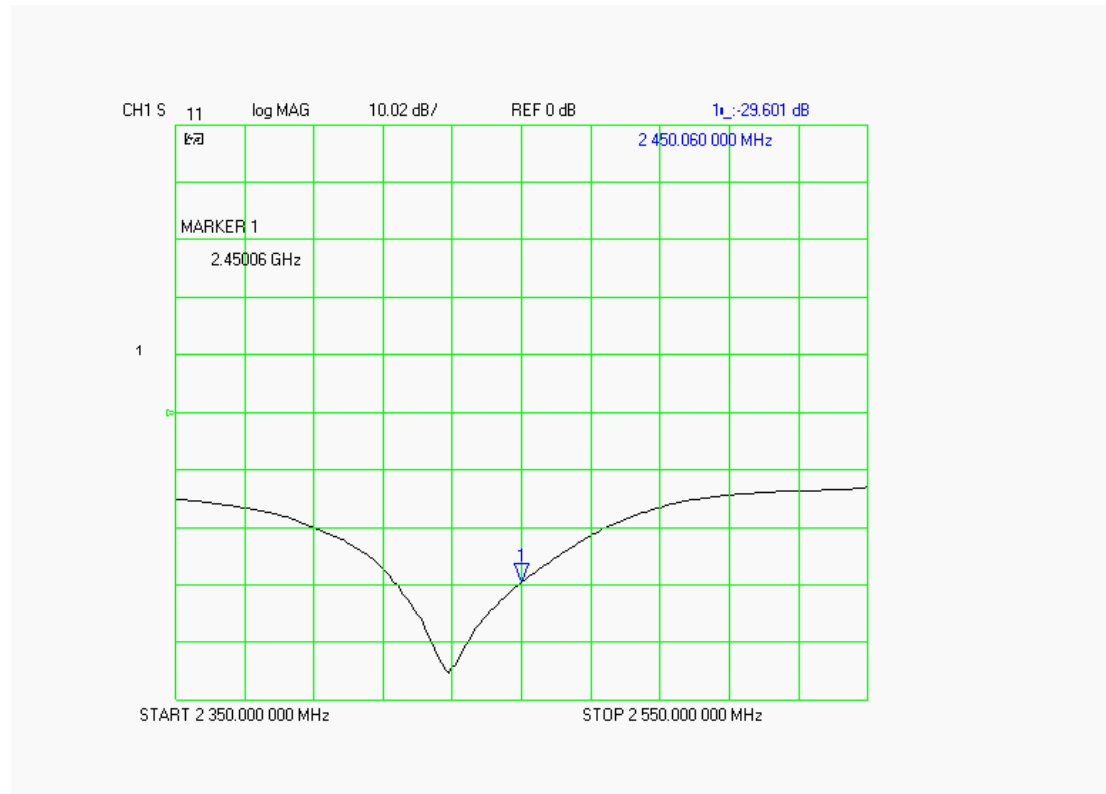

## SWR

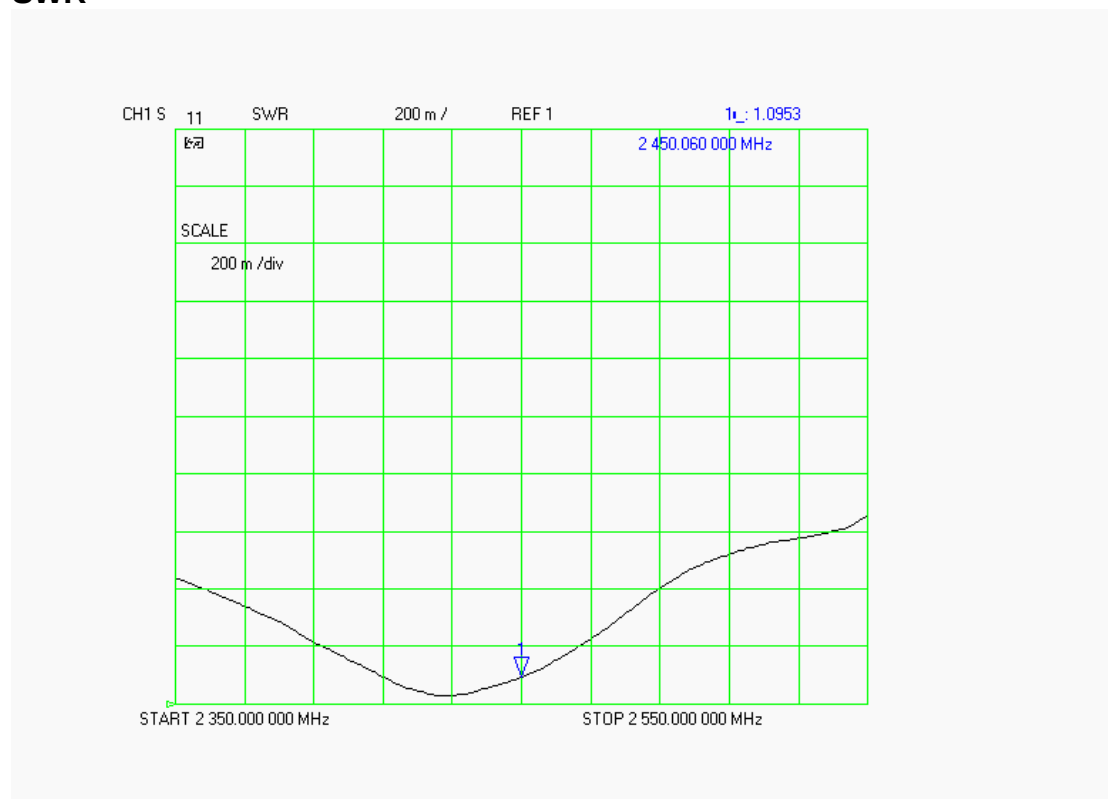

## Smith Chart Dipole Impedance

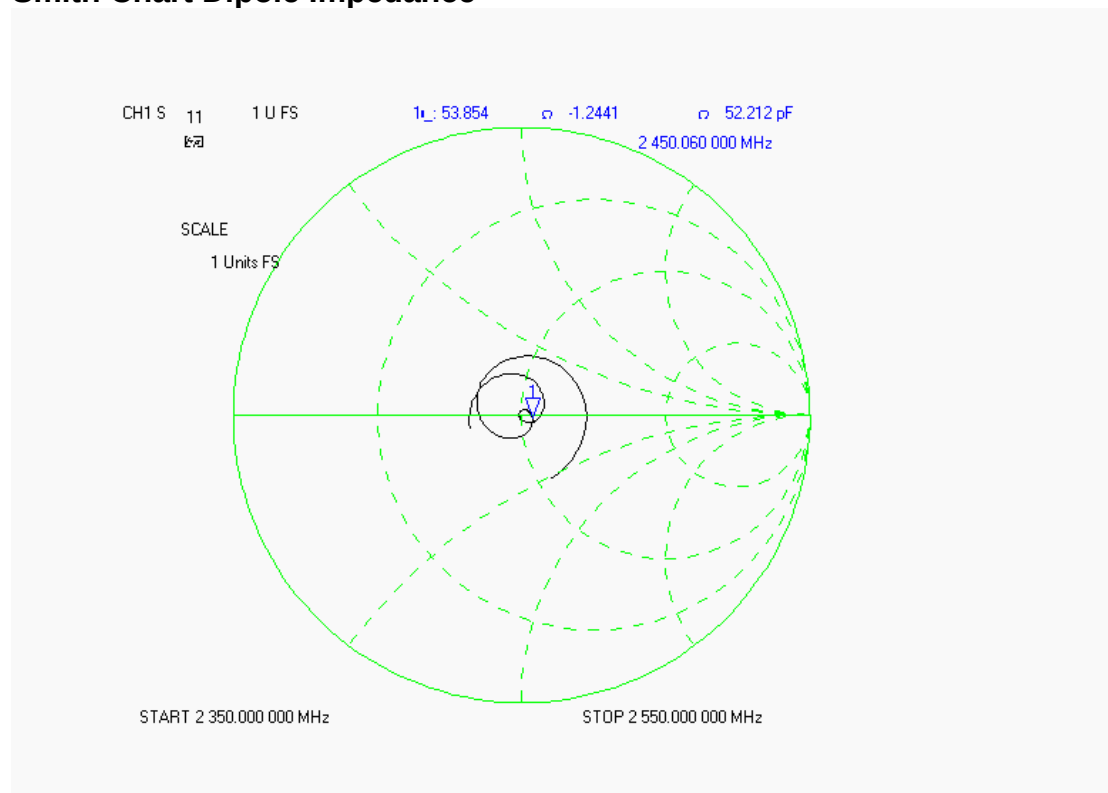

## Body Measurement Conditions

The measurements were performed in the Uni-Phantom filled with body simulating liquid of the following electrical parameters at 2450 MHz:

|                        |            |           |
|------------------------|------------|-----------|
| Relative Dielectricity | 52.59      | $\pm 5\%$ |
| Conductivity           | 1.92 mho/m | $\pm 5\%$ |

The APREL Laboratories ALSAS system with a dosimetric E-field probe E-020 (SN:217, Conversion factor 3.61 at 2450 MHz) was used for the measurements.

The dipole was mounted so that the dipole feed point was positioned below the center marking of the flat phantom and the dipole was oriented parallel to the body axis (the long side of the phantom). The standard measuring distance was 10mm from the dipole center to the solution surface.

The coarse grid with a grid spacing of 10mm was aligned with the dipole. The 5x5x8 fine cube was chosen for cube integration. The dipole input power (forward power) was 100mW  $\pm 3\%$ . The results are normalized to 1W input power.

The laboratories environmental conditions were as follows during the calibration sequence.

|                                        |                    |
|----------------------------------------|--------------------|
| Ambient Temperature of the Laboratory: | 24 °C $\pm 1.0$ °C |
| Temperature of the Tissue:             | 20 °C $\pm 1.0$ °C |
| Relative Humidity:                     | 41%                |


## SAR Measurement

Standard SAR measurements were performed according to the measurement conditions described above. The results have been normalized to a dipole input power of 1W (forward power). The resulting averaged SAR values measured with the dosimetric probe E-020 SN:217 and applying the advanced extrapolation are:

Averaged over 1 cm<sup>3</sup> (1 g) of tissue: 53.550 mW/g  $\pm$  18.8% (k=2)<sup>1</sup>

Averaged over 10 cm<sup>3</sup> (10 g) of tissue: 24.710 mW/g  $\pm$  18.4% (k=2)<sup>1</sup>

### Area Scan

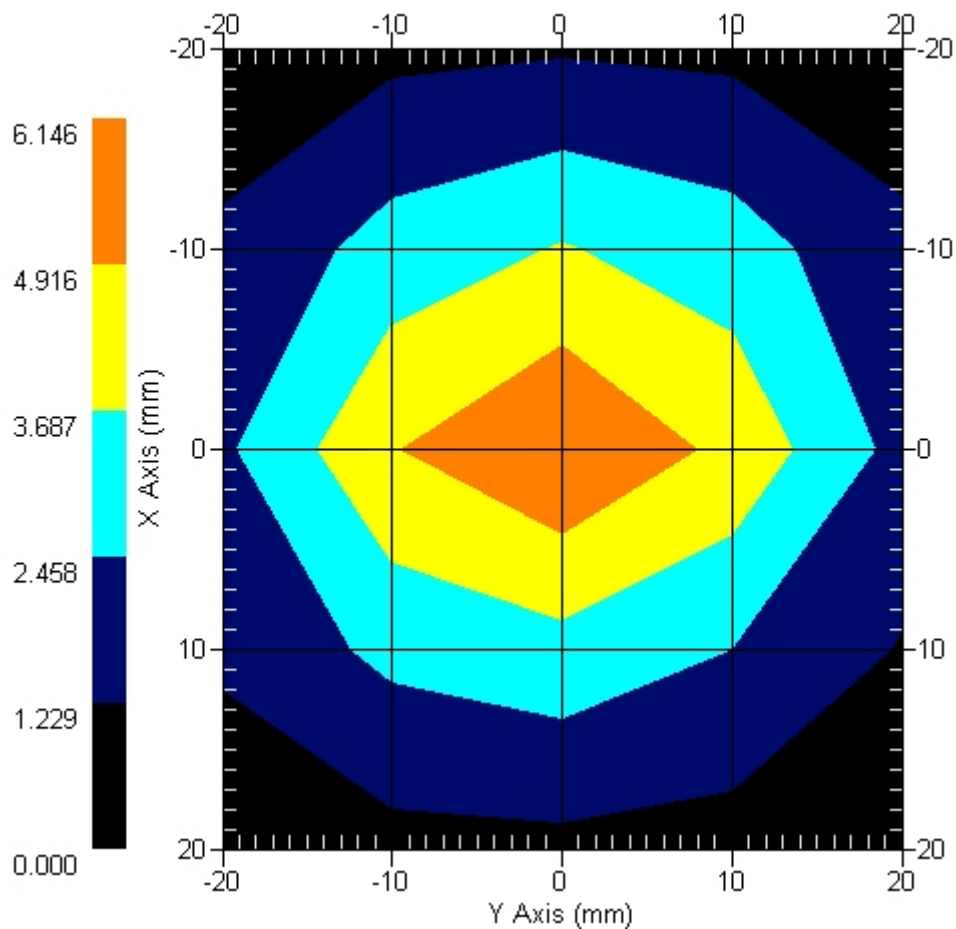

1 gram SAR value : 5.355 W/kg  
 10 gram SAR value : 2.471 W/kg  
 Area Scan Peak SAR : 6.146 W/kg  
 Zoom Scan Peak SAR : 11.090 W/kg

<sup>1</sup> validation uncertainty


## Dipole Impedance and Return Loss

The impedance was measured at the SMA connector with a network analyzer. The dipole was positioned at the flat phantom sections according to measurement conditions stated above during impedance measurements.


| Test      | Result          |
|-----------|-----------------|
| S11 R/L   | -31.173 dB      |
| SWR       | 1.1354 U        |
| Impedance | 54.146 $\Omega$ |

The following graphs are the results as displayed on the Vector Network Analyzer.


### S11 Parameter Return Loss

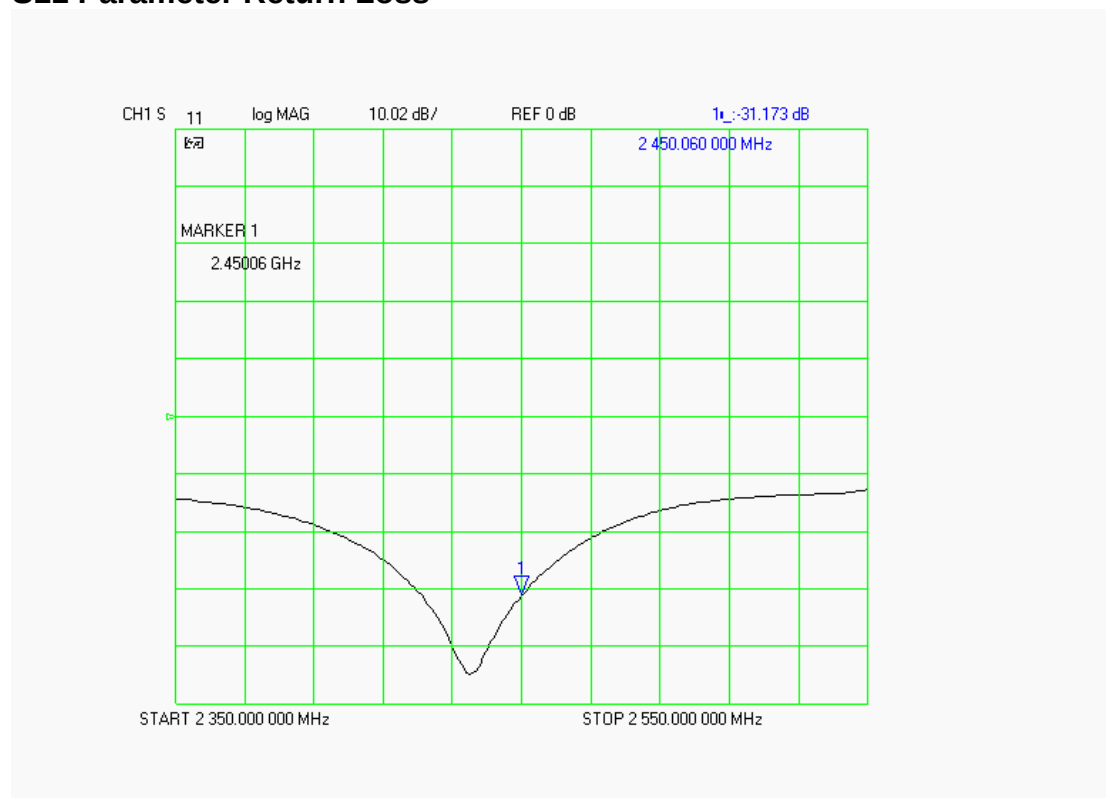

## SWR

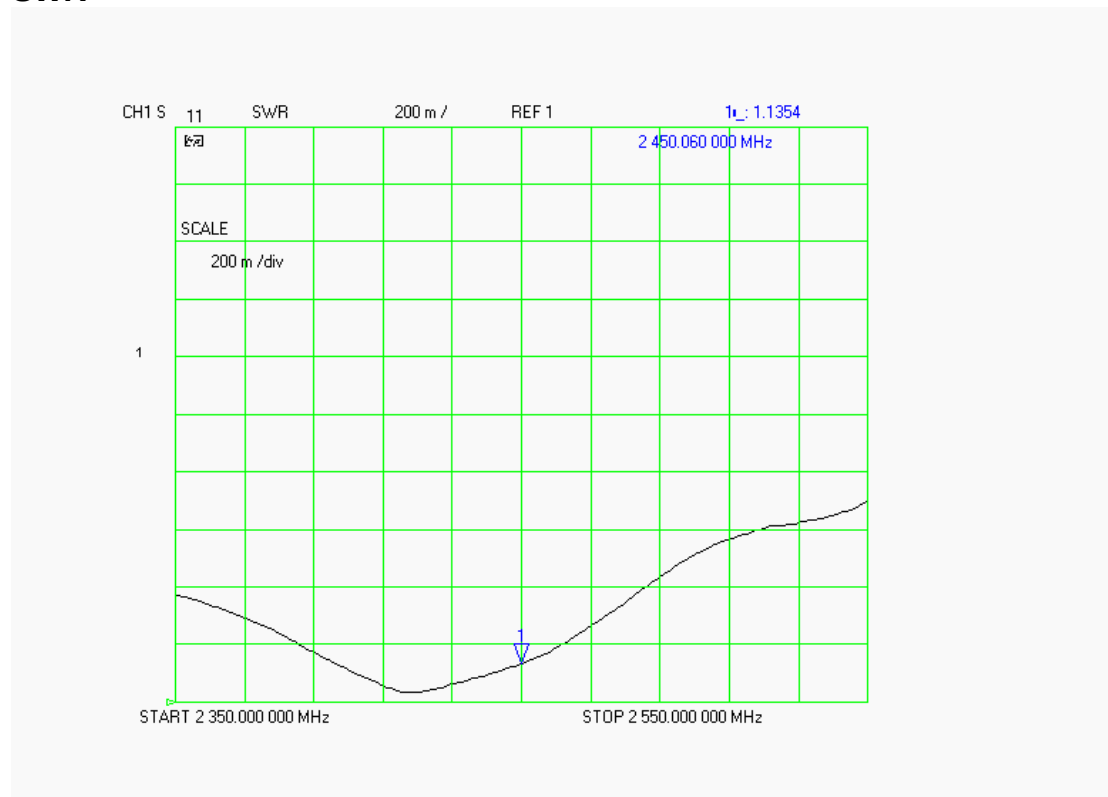

## Smith Chart Dipole Impedance

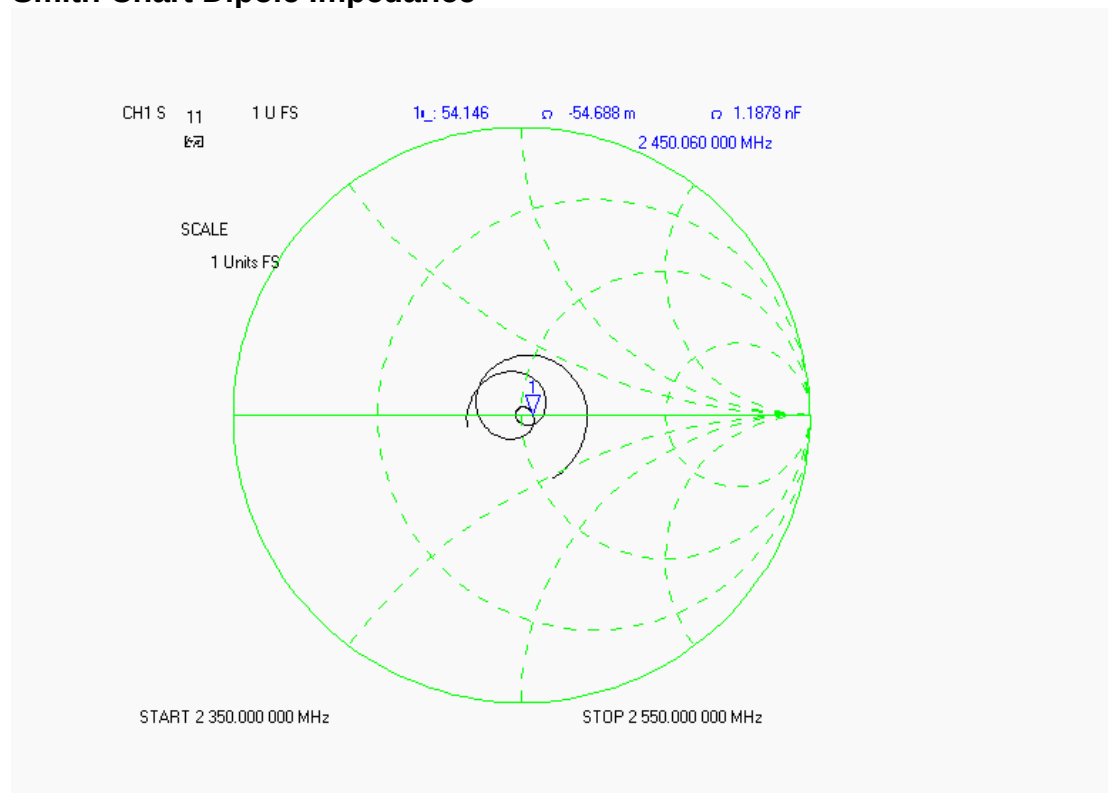

## Test Equipment List

The test equipment used during Dipole Calibration, manufacturer, model number and, current calibration status are listed and located on the RF Exposure Lab, LLC system computer C:\Test Equipment\Calibration Equipment\Instrument List February 2008.

## RF Exposure Lab, LLC

Calibration File No: CAL.20070501

### CERTIFICATE OF CALIBRATION

It is certified that the equipment identified below has been calibrated at RF Exposure Lab, LLC by qualified personnel following recognized procedures and using transfer standards traceable to NRC/NIST.

#### Validation Dipole

Manufacturer: APREL Laboratories

Part Number: ALS-D-BB-S-2

Frequency: 5.2 GHz to 5.8 GHz

Serial No: 235-00801

Manufactured: 22 May 2005  
Calibrated: 23 May 2007

Calibrated By: Signature on File  
Jay Moulton – Technical Manager

Approved By: Signature on File  
Tamara Moulton – Quality Manager

Measurement Uncertainty:

|                     |      |
|---------------------|------|
| Repeatability:      | 23%  |
| Tissue Uncertainty: | 3.2% |
| Network Analyzer:   | 25%  |



## RF EXPOSURE LAB, LLC

2867 Progress Place, Suite 4D  
Escondido, CA 92029

Tel: (760) 737-3131  
FAX: (760) 737-9131

## Calibration Results Summary

The following results relate to the Calibrated Dipole and should be used as a quick reference for the user.

### Mechanical Dimensions

**Length:** 23.3 mm  
**Height:** 20.3 mm

### Electrical Specifications

#### 5.2 GHz Body

**SWR:** 1.8749 U  
**Return Loss:** -17.057 dB  
**Impedance:** 54.252  $\Omega$

### System Validation Results

| Frequency | 1 Gram | 10 Gram |
|-----------|--------|---------|
| 5.2 GHz   | 62.98  | 15.44   |

#### 5.6 GHz Body

**SWR:** 1.2178 U  
**Return Loss:** -18.513 dB  
**Impedance:** 45.365  $\Omega$

### System Validation Results

| Frequency | 1 Gram | 10 Gram |
|-----------|--------|---------|
| 5.6 GHz   | 59.92  | 15.30   |

#### 5.8 GHz Body

**SWR:** 1.8551 U  
**Return Loss:** -10.237 dB  
**Impedance:** 45.014  $\Omega$

### System Validation Results

| Frequency | 1 Gram | 10 Gram |
|-----------|--------|---------|
| 5.8 GHz   | 58.92  | 15.05   |

## 5.2 GHz Body Measurement Conditions

The measurements were performed in the Uni-Phantom filled with body simulating liquid of the following electrical parameters at 5.2 GHz:

|                        |            |           |
|------------------------|------------|-----------|
| Relative Dielectricity | 49.19      | $\pm 5\%$ |
| Conductivity           | 5.40 mho/m | $\pm 5\%$ |

The APREL Laboratories ALSAS system with a dosimetric E-field probe E-030 (SN:AL-E3P1, Conversion factor 13.0 at 5.2 GHz) was used for the measurements.

The dipole was mounted so that the dipole feed point was positioned below the center marking of the flat phantom and the dipole was oriented parallel to the body axis (the long side of the phantom). The standard measuring distance was 10mm from the dipole center to the solution surface.

The coarse grid with a grid spacing of 10mm was aligned with the dipole. The 7x7x7 fine cube was chosen for cube integration. The dipole input power (forward power) was 100mW  $\pm 3\%$ . The results are normalized to 1W input power.

The laboratories environmental conditions were as follows during the calibration sequence.


|                                        |                    |
|----------------------------------------|--------------------|
| Ambient Temperature of the Laboratory: | 23 °C $\pm 1.0$ °C |
| Temperature of the Tissue:             | 20 °C $\pm 1.0$ °C |
| Relative Humidity:                     | 52%                |

## SAR Measurement

Standard SAR measurements were performed according to the measurement conditions described above. The results have been normalized to a dipole input power of 1W (forward power). The resulting averaged SAR values measured with the dosimetric probe E-030 SN:AL-E3P1 and applying the advanced extrapolation are:

Averaged over 1 cm<sup>3</sup> (1 g) of tissue: 62.98 mW/g  $\pm$  19.1% (k=2)<sup>1</sup>

Averaged over 10 cm<sup>3</sup> (10 g) of tissue: 15.44 mW/g  $\pm$  18.8% (k=2)<sup>1</sup>

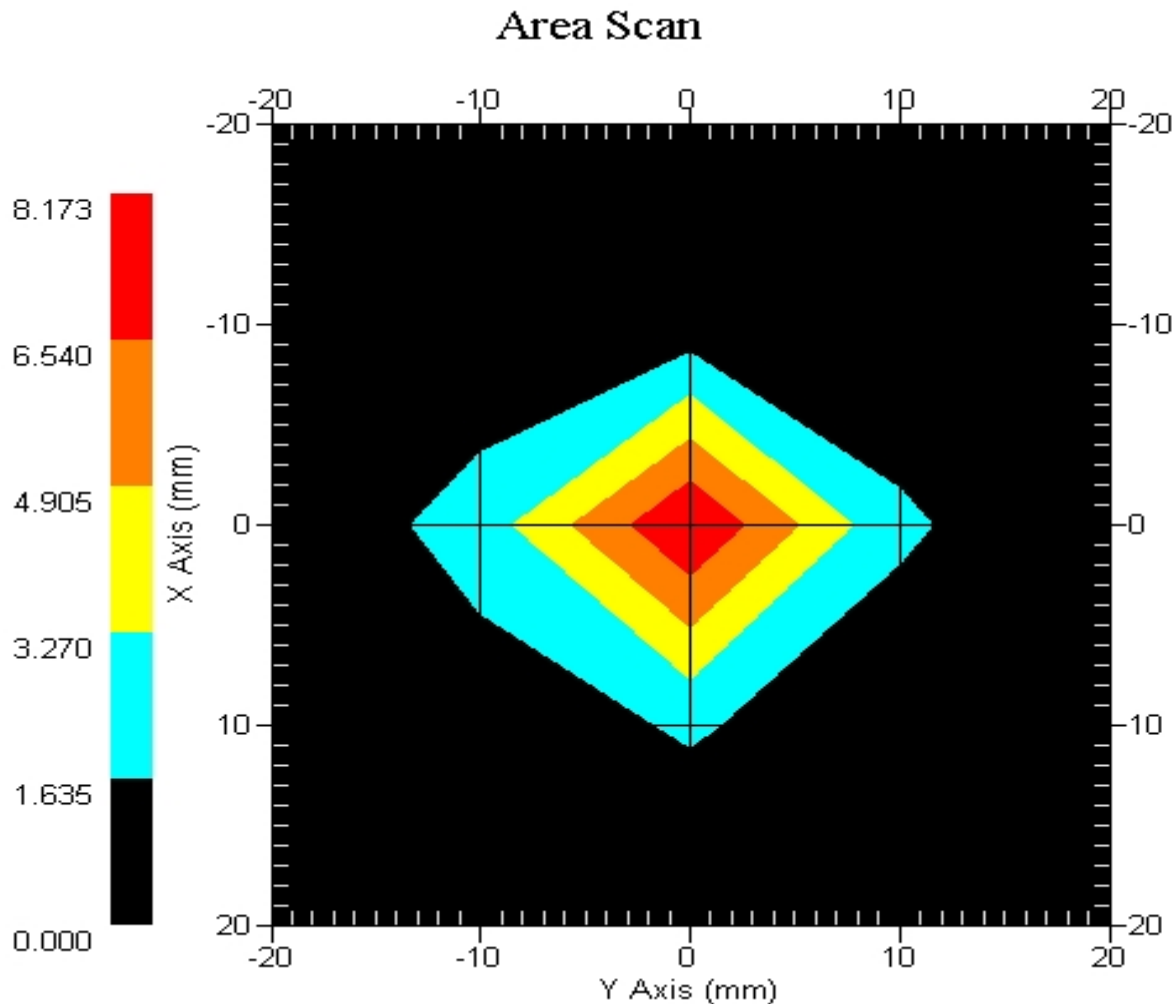

1 gram SAR value : 6.298 W/kg  
 10 gram SAR value : 1.544 W/kg  
 Area Scan Peak SAR : 8.173 W/kg  
 Zoom Scan Peak SAR : 21.817 W/kg

<sup>1</sup> validation uncertainty

## 5.6 GHz Body Measurement Conditions

The measurements were performed in the Uni-Phantom filled with body simulating liquid of the following electrical parameters at 5.6 GHz:

|                        |            |           |
|------------------------|------------|-----------|
| Relative Dielectricity | 48.22      | $\pm 5\%$ |
| Conductivity           | 5.68 mho/m | $\pm 5\%$ |

The APREL Laboratories ALSAS system with a dosimetric E-field probe E-030 (SN:AL-E3P1, Conversion factor 13.5 at 5.6 GHz) was used for the measurements.

The dipole was mounted so that the dipole feed point was positioned below the center marking of the flat phantom and the dipole was oriented parallel to the body axis (the long side of the phantom). The standard measuring distance was 10mm from the dipole center to the solution surface.

The coarse grid with a grid spacing of 10mm was aligned with the dipole. The 7x7x7 fine cube was chosen for cube integration. The dipole input power (forward power) was 100mW  $\pm 3\%$ . The results are normalized to 1W input power.

The laboratories environmental conditions were as follows during the calibration sequence.


|                                        |                    |
|----------------------------------------|--------------------|
| Ambient Temperature of the Laboratory: | 23 °C $\pm 1.0$ °C |
| Temperature of the Tissue:             | 20 °C $\pm 1.0$ °C |
| Relative Humidity:                     | 52%                |

## SAR Measurement

Standard SAR measurements were performed according to the measurement conditions described above. The results have been normalized to a dipole input power of 1W (forward power). The resulting averaged SAR values measured with the dosimetric probe E-030 SN:AL-E3P1 and applying the advanced extrapolation are:

Averaged over 1 cm<sup>3</sup> (1 g) of tissue: 59.92 mW/g  $\pm$  19.1% (k=2)<sup>1</sup>

Averaged over 10 cm<sup>3</sup> (10 g) of tissue: 15.30 mW/g  $\pm$  18.8% (k=2)<sup>1</sup>

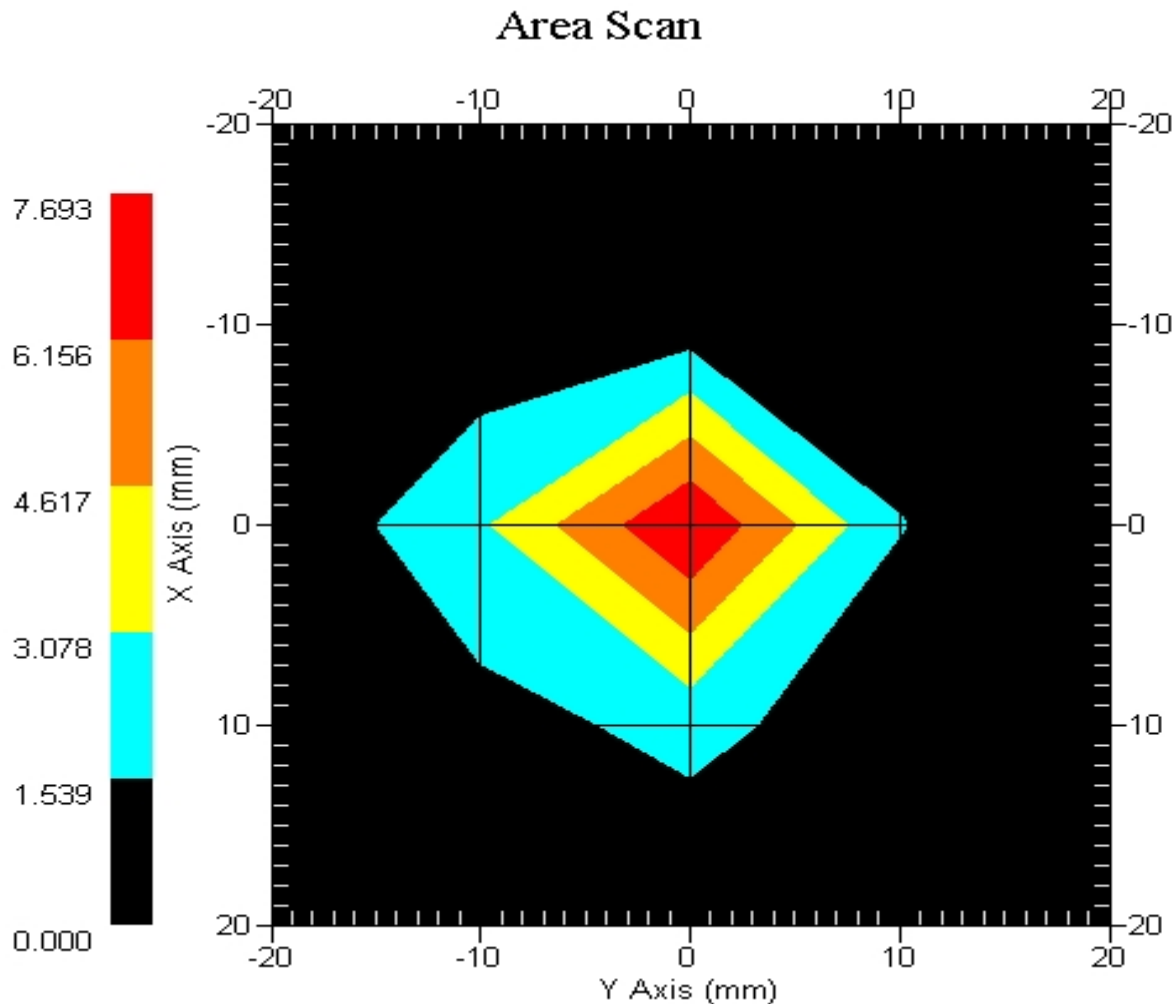

1 gram SAR value : 5.992 W/kg  
 10 gram SAR value : 1.530 W/kg  
 Area Scan Peak SAR : 7.693 W/kg  
 Zoom Scan Peak SAR : 19.415 W/kg

<sup>1</sup> validation uncertainty

## 5.8 GHz Body Measurement Conditions

The measurements were performed in the Uni-Phantom filled with body simulating liquid of the following electrical parameters at 5.8 GHz:

|                        |            |           |
|------------------------|------------|-----------|
| Relative Dielectricity | 48.53      | $\pm 5\%$ |
| Conductivity           | 5.95 mho/m | $\pm 5\%$ |

The APREL Laboratories ALSAS system with a dosimetric E-field probe E-030 (SN:AL-E3P1, Conversion factor 14.0 at 5.8 GHz) was used for the measurements.

The dipole was mounted so that the dipole feed point was positioned below the center marking of the flat phantom and the dipole was oriented parallel to the body axis (the long side of the phantom). The standard measuring distance was 10mm from the dipole center to the solution surface.

The coarse grid with a grid spacing of 10mm was aligned with the dipole. The 7x7x7 fine cube was chosen for cube integration. The dipole input power (forward power) was 100mW  $\pm 3\%$ . The results are normalized to 1W input power.

The laboratories environmental conditions were as follows during the calibration sequence.


|                                        |                    |
|----------------------------------------|--------------------|
| Ambient Temperature of the Laboratory: | 23 °C $\pm 1.0$ °C |
| Temperature of the Tissue:             | 20 °C $\pm 1.0$ °C |
| Relative Humidity:                     | 52%                |

## SAR Measurement

Standard SAR measurements were performed according to the measurement conditions described above. The results have been normalized to a dipole input power of 1W (forward power). The resulting averaged SAR values measured with the dosimetric probe E-030 SN:AL-E3P1 and applying the advanced extrapolation are:

Averaged over 1 cm<sup>3</sup> (1 g) of tissue: 58.92 mW/g  $\pm$  19.1% (k=2)<sup>1</sup>

Averaged over 10 cm<sup>3</sup> (10 g) of tissue: 15.05 mW/g  $\pm$  18.8% (k=2)<sup>1</sup>

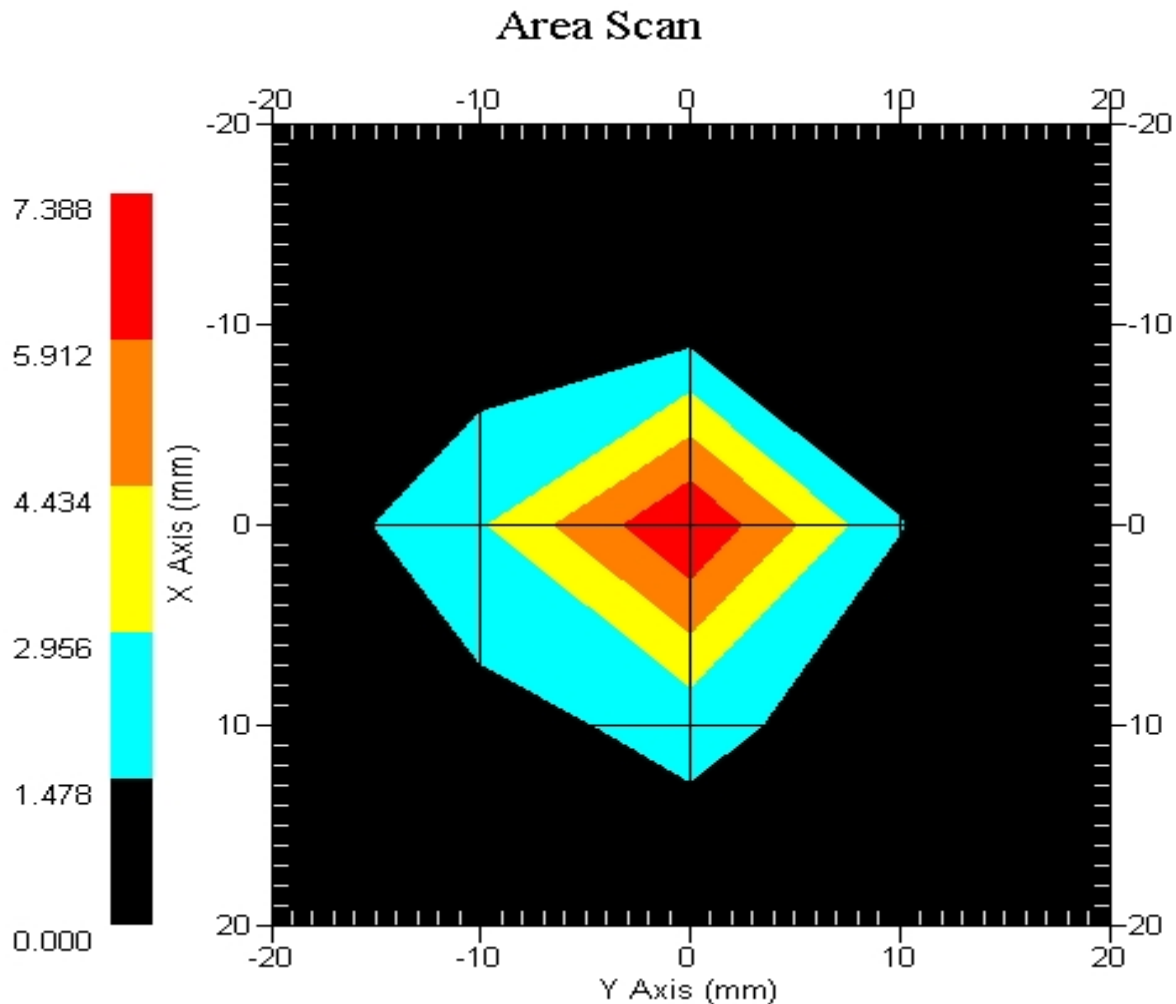

1 gram SAR value : 5.892 W/kg  
 10 gram SAR value : 1.505 W/kg  
 Area Scan Peak SAR : 7.388 W/kg  
 Zoom Scan Peak SAR : 19.315 W/kg

<sup>1</sup> validation uncertainty


## Dipole Impedance and Return Loss

The impedance was measured at the SMA connector with a network analyzer. The dipole was positioned at the flat phantom sections according to measurement conditions stated above during impedance measurements.


| Test      | Result – 5.2 GHz | Result – 5.6 GHz | Result – 5.8 GHz |
|-----------|------------------|------------------|------------------|
| S11 R/L   | -17.057 dB       | -18.513 dB       | -10.237 dB       |
| SWR       | 1.8749 U         | 1.2178 U         | 1.8551 U         |
| Impedance | 54.252 $\Omega$  | 45.365 $\Omega$  | 45.014 $\Omega$  |

The following graphs are the results as displayed on the Vector Network Analyzer.


### S11 Parameter Return Loss

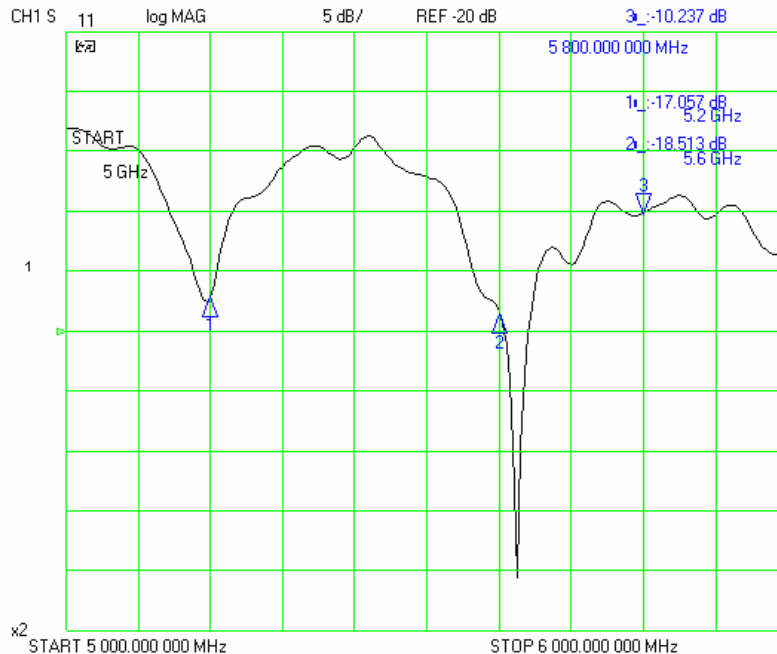

## SWR

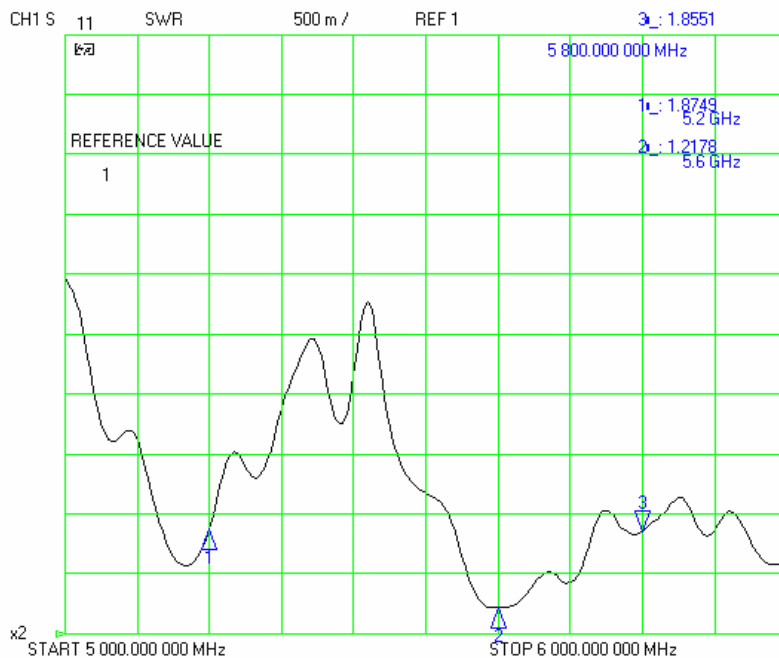

## Smith Chart Dipole Impedance

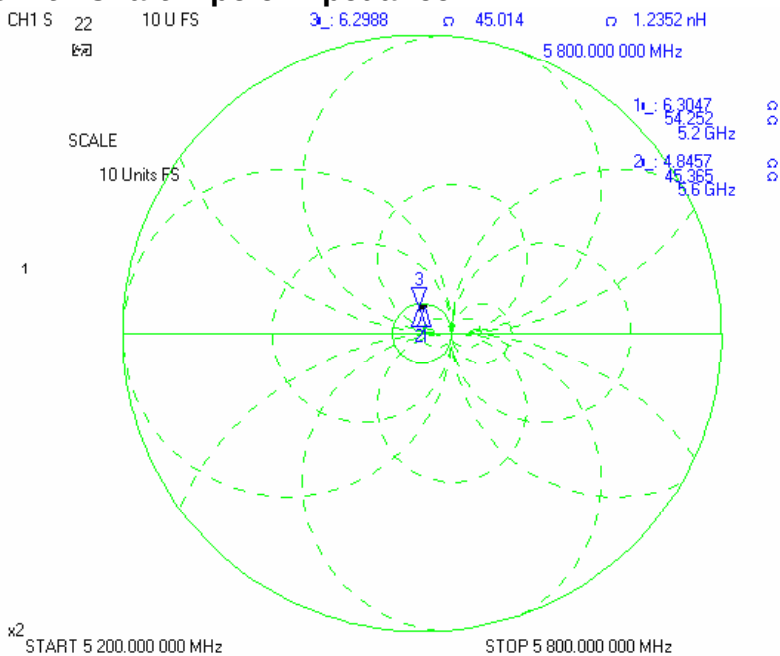

## Test Equipment List

The test equipment used during Dipole Calibration, manufacturer, model number and, current calibration status are listed and located on the RF Exposure Lab, LLC system computer C:\Test Equipment\Calibration Equipment\Instrument List May 2007.

## Appendix F – Phantom Calibration Data Sheets

## NCL CALIBRATION LABORATORIES

Calibration File No.: RFE-273

# CERTIFICATE OF CALIBRATION

It is certified that the equipment identified below has been calibrated in the  
**NCL CALIBRATION LABORATORIES** by qualified personnel following recognized  
procedures and using transfer standards traceable to National Standards.

Thickness of the UniPhantom is 2 mm  $\pm$  10%  
Pinna thickness is 6 mm  $\pm$  10%

|             |         |                |          |
|-------------|---------|----------------|----------|
| Resolution: | 0.01 mm | Calibrated to: | 0.0 mm   |
| Stability:  | OK      | Accuracy:      | < 0.1 mm |

Calibrated By: Karen K. Feb 17/04.

### **NCL** CALIBRATION LABORATORIES

51 SPECTRUM WAY  
NEPEAN, ONTARIO  
CANADA K2R 1E6

Division of APREL Lab.  
TEL: (613) 820-4988  
FAX: (613) 820-4161