

	Document <b>Appendix D for the BlackBerry® Smartphone Model RDU71CW/RDE71UW SAR Report Rev1</b>	Page <b>1(74)</b>
Author Data <b>Andrew Becker</b>	Dates of Test <b>Feb 7 – May 25, July 18, 2011</b>	Test Report No <b>RTS-3933-1105-11A RTS-2580-1106-03 Rev1</b> FCC ID: <b>L6ARDU70CW L6ARDE70UW</b> IC ID <b>2503A-RDU70CW 2503A-RDE70UW</b>

#### APPENDIX D: PROBE & DIPOLE CALIBRATION DATA

	Document <b>Appendix D for the BlackBerry® Smartphone Model RDU71CW/RDE71UW SAR Report Rev1</b>	Page <b>2(74)</b>
Author Data <b>Andrew Becker</b>	Dates of Test <b>Feb 7 – May 25, July 18, 2011</b>	Test Report No <b>RTS-3933-1105-11A RTS-2580-1106-03 Rev1</b> FCC ID: <b>L6ARDU70CW L6ARDE70UW</b> IC ID <b>2503A-RDU70CW 2503A-RDE70UW</b>

**Calibration Laboratory of**  
Schmid & Partner  
Engineering AG  
Zeughausstrasse 43, 8004 Zurich, Switzerland



**S** Schweizerischer Kalibrierdienst  
**C** Service suisse d'étalonnage  
**S** Servizio svizzero di taratura  
**S** Swiss Calibration Service

Accredited by the Swiss Accreditation Service (SAS)  
The Swiss Accreditation Service is one of the signatories to the EA  
Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: **SCS 108**

Client **RTS (RIM Testing Services)**

Certificate No: **ET3-1643\_Mar10**

## CALIBRATION CERTIFICATE

Object **ET3DV6 - SN:1643**

Calibration procedure(s) **QA CAL-01.v6, QA CAL-23.v3 and QA CAL-25.v2  
Calibration procedure for dosimetric E-field probes**

Calibration date: **March 9, 2010**

This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI). The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility: environment temperature  $(22 \pm 3)^\circ\text{C}$  and humidity  $< 70\%$ .

Calibration Equipment used (M&TE critical for calibration)

Primary Standards	ID #	Cal Date (Certificate No.)	Scheduled Calibration
Power meter E4419B	GB41293874	1-Apr-09 (No. 217-01030)	Apr-10
Power sensor E4412A	MY41495277	1-Apr-09 (No. 217-01030)	Apr-10
Power sensor E4412A	MY41498087	1-Apr-09 (No. 217-01030)	Apr-10
Reference 3 dB Attenuator	SN: S5054 (3c)	31-Mar-09 (No. 217-01026)	Mar-10
Reference 20 dB Attenuator	SN: S5086 (20b)	31-Mar-09 (No. 217-01028)	Mar-10
Reference 30 dB Attenuator	SN: S5129 (30b)	31-Mar-09 (No. 217-01027)	Mar-10
Reference Probe ES3DV2	SN: 3013	30-Dec-09 (No. ES3-3013_Dec09)	Dec-10
DAE4	SN: 660	29-Sep-09 (No. DAE4-660_Sep09)	Sep-10

Secondary Standards	ID #	Check Date (in house)	Scheduled Check
RF generator HP 8648C	US3642U01700	4-Aug-99 (in house check Oct-09)	In house check: Oct-11
Network Analyzer HP 8753E	US37390585	18-Oct-01 (in house check Oct-09)	In house check: Oct10

Calibrated by: **Jeton Kastrati** Function: **Laboratory Technician** Signature:

Approved by: **Katja Pokovic** Function: **Technical Manager** Signature:

Issued: March 10, 2010

This calibration certificate shall not be reproduced except in full without written approval of the laboratory.

Certificate No: **ET3-1643\_Mar10**

Page 1 of 11

	Document <b>Appendix D for the BlackBerry® Smartphone Model RDU71CW/RDE71UW SAR Report Rev1</b>	Page <b>3(74)</b>
Author Data <b>Andrew Becker</b>	Dates of Test <b>Feb 7 – May 25, July 18, 2011</b>	Test Report No <b>RTS-3933-1105-11A RTS-2580-1106-03 Rev1</b> FCC ID: <b>L6ARDU70CW L6ARDE70UW</b> IC ID <b>2503A-RDU70CW 2503A-RDE70UW</b>

**Calibration Laboratory of**  
Schmid & Partner  
Engineering AG  
Zeughausstrasse 43, 8004 Zurich, Switzerland



**S** Schweizerischer Kalibrierdienst  
**C** Service suisse d'étalonnage  
**S** Servizio svizzero di taratura  
**S** Swiss Calibration Service

Accredited by the Swiss Accreditation Service (SAS)  
The Swiss Accreditation Service is one of the signatories to the EA  
Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: **SCS 108**

### Glossary:

<b>TSL</b>	tissue simulating liquid
<b>NORM<sub>x,y,z</sub></b>	sensitivity in free space
<b>ConvF</b>	sensitivity in TSL / NORM <sub>x,y,z</sub>
<b>DCP</b>	diode compression point
<b>CF</b>	crest factor (1/duty_cycle) of the RF signal
<b>A, B, C</b>	modulation dependent linearization parameters
<b>Polarization <math>\varphi</math></b>	$\varphi$ rotation around probe axis
<b>Polarization <math>\theta</math></b>	$\theta$ rotation around an axis that is in the plane normal to probe axis (at measurement center), i.e., $\theta = 0$ is normal to probe axis

### Calibration is Performed According to the Following Standards:

- IEEE Std 1528-2003, "IEEE Recommended Practice for Determining the Peak Spatial-Averaged Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques", December 2003
- IEC 62209-1, "Procedure to measure the Specific Absorption Rate (SAR) for hand-held devices used in close proximity to the ear (frequency range of 300 MHz to 3 GHz)", February 2005

### Methods Applied and Interpretation of Parameters:

- NORM<sub>x,y,z</sub>**: Assessed for E-field polarization  $\theta = 0$  ( $f \leq 900$  MHz in TEM-cell;  $f > 1800$  MHz: R22 waveguide). NORM<sub>x,y,z</sub> are only intermediate values, i.e., the uncertainties of NORM<sub>x,y,z</sub> does not effect the E<sup>2</sup>-field uncertainty inside TSL (see below **ConvF**).
- NORM(f)<sub>x,y,z</sub>** = **NORM<sub>x,y,z</sub>** \* *frequency\_response* (see Frequency Response Chart). This linearization is implemented in DASY4 software versions later than 4.2. The uncertainty of the frequency response is included in the stated uncertainty of **ConvF**.
- DCPx,y,z**: DCP are numerical linearization parameters assessed based on the data of power sweep with CW signal (no uncertainty required). DCP does not depend on frequency nor media.
- A<sub>x,y,z</sub>; B<sub>x,y,z</sub>; C<sub>x,y,z</sub>**: **VRx,y,z**: **A, B, C** are numerical linearization parameters assessed based on the data of power sweep for specific modulation signal. The parameters do not depend on frequency nor media. VR is the maximum calibration range expressed in RMS voltage across the diode.
- ConvF and Boundary Effect Parameters**: Assessed in flat phantom using E-field (or Temperature Transfer Standard for  $f \leq 800$  MHz) and inside waveguide using analytical field distributions based on power measurements for  $f > 800$  MHz. The same setups are used for assessment of the parameters applied for boundary compensation (alpha, depth) of which typical uncertainty values are given. These parameters are used in DASY4 software to improve probe accuracy close to the boundary. The sensitivity in TSL corresponds to **NORM<sub>x,y,z</sub>** \* **ConvF** whereby the uncertainty corresponds to that given for **ConvF**. A frequency dependent **ConvF** is used in DASY version 4.4 and higher which allows extending the validity from  $\pm 50$  MHz to  $\pm 100$  MHz.
- Spherical Isotropy (3D deviation from Isotropy)**: in a field of low gradients realized using a flat phantom exposed by a patch antenna.
- Sensor Offset**: The sensor offset corresponds to the offset of virtual measurement center from the probe tip (on probe axis). No tolerance required.

 <p>Document  <b>Appendix D for the BlackBerry® Smartphone Model  RDU71CW/RDE71UW SAR Report Rev1</b></p>				Page <b>4(74)</b>
Author Data <b>Andrew Becker</b>	Dates of Test <b>Feb 7 – May 25, July 18,  2011</b>	Test Report No <b>RTS-3933-1105-11A  RTS-2580-1106-03 Rev1</b>	FCC ID: <b>L6ARDU70CW  L6ARDE70UW</b>	IC ID <b>2503A-RDU70CW  2503A-RDE70UW</b>

**ET3DV6 SN:1643**

**March 9, 2010**

# Probe ET3DV6

## SN:1643

Manufactured: November 7, 2001  
Last calibrated: March 10, 2009  
Recalibrated: March 9, 2010

**Calibrated for DASY Systems**

(Note: non-compatible with DASY2 system!)



Document

**Appendix D for the BlackBerry® Smartphone Model  
RDU71CW/RDE71UW SAR Report Rev1**Page  
**5(74)**

Author Data <b>Andrew Becker</b>	Dates of Test <b>Feb 7 – May 25, July 18, 2011</b>	Test Report No <b>RTS-3933-1105-11A RTS-2580-1106-03 Rev1</b>	FCC ID: <b>L6ARDU70CW L6ARDE70UW</b>	IC ID <b>2503A-RDU70CW 2503A-RDE70UW</b>
-------------------------------------	---	--	---	---

**ET3DV6 SN:1643****March 9, 2010****DASY - Parameters of Probe: ET3DV6 SN:1643****Basic Calibration Parameters**

	Sensor X	Sensor Y	Sensor Z	Unc (k=2)
Norm ( $\mu$ V/(V/m) <sup>2</sup> ) <sup>A</sup>	1.75	2.01	1.79	$\pm$ 10.1%
DCP (mV) <sup>B</sup>	93.2	91.0	90.9	

**Modulation Calibration Parameters**

UID	Communication System Name	PAR		A dB	B dBuV	C	VR mV	Unc <sup>E</sup> (k=2)
10000	CW	0.00	X Y Z	0.00 0.00 0.00	0.00 0.00 0.00	1.00 1.00 1.00	300.0 300.0 300.0	$\pm$ 1.5%

The reported uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor k=2, which for a normal distribution corresponds to a coverage probability of approximately 95%.

<sup>A</sup> The uncertainties of NormX,Y,Z do not affect the E-field uncertainty inside TSL (see Pages 5 and 6).<sup>B</sup> Numerical linearization parameter: uncertainty not required.<sup>E</sup> Uncertainty is determined using the maximum deviation from linear response applying rectangular distribution and is expressed for the square of the field value.



Document

**Appendix D for the BlackBerry® Smartphone Model  
RDU71CW/RDE71UW SAR Report Rev1**Page  
**6(74)**

Author Data <b>Andrew Becker</b>	Dates of Test <b>Feb 7 – May 25, July 18, 2011</b>	Test Report No <b>RTS-3933-1105-11A RTS-2580-1106-03 Rev1</b>	FCC ID: <b>L6ARDU70CW L6ARDE70UW</b>	IC ID <b>2503A-RDU70CW 2503A-RDE70UW</b>
-------------------------------------	---	--	---	---

**ET3DV6 SN:1643****March 9, 2010****DASY - Parameters of Probe: ET3DV6 SN:1643****Calibration Parameter Determined in Head Tissue Simulating Media**

<b>f [MHz]</b>	<b>Validity [MHz]<sup>c</sup></b>	<b>Permittivity</b>	<b>Conductivity</b>	<b>ConvF X</b>	<b>ConvF Y</b>	<b>ConvF Z</b>	<b>Alpha</b>	<b>Depth Unc (k=2)</b>
900	$\pm 50 / \pm 100$	$41.5 \pm 5\%$	$0.97 \pm 5\%$	6.01	6.01	6.01	0.42	$2.35 \pm 11.0\%$
1810	$\pm 50 / \pm 100$	$40.0 \pm 5\%$	$1.40 \pm 5\%$	4.99	4.99	4.99	0.62	$2.35 \pm 11.0\%$
1950	$\pm 50 / \pm 100$	$40.0 \pm 5\%$	$1.40 \pm 5\%$	4.74	4.74	4.74	0.79	$2.10 \pm 11.0\%$

<sup>c</sup> The validity of  $\pm 100$  MHz only applies for DASY v4.4 and higher (see Page 2). The uncertainty is the RSS of the ConvF uncertainty at calibration frequency and the uncertainty for the indicated frequency band.



Document

**Appendix D for the BlackBerry® Smartphone Model  
RDU71CW/RDE71UW SAR Report Rev1**Page  
7(74)

Author Data <b>Andrew Becker</b>	Dates of Test <b>Feb 7 – May 25, July 18, 2011</b>	Test Report No <b>RTS-3933-1105-11A RTS-2580-1106-03 Rev1</b>	FCC ID: <b>L6ARDU70CW L6ARDE70UW</b>	IC ID <b>2503A-RDU70CW 2503A-RDE70UW</b>
-------------------------------------	---	--	---	---

**ET3DV6 SN:1643****March 9, 2010****DASY - Parameters of Probe: ET3DV6 SN:1643****Calibration Parameter Determined in Body Tissue Simulating Media**

<b>f [MHz]</b>	<b>Validity [MHz]<sup>c</sup></b>	<b>Permittivity</b>	<b>Conductivity</b>	<b>ConvF X</b>	<b>ConvF Y</b>	<b>ConvF Z</b>	<b>Alpha</b>	<b>Depth Unc (k=2)</b>
900	$\pm 50 / \pm 100$	55.0 $\pm$ 5%	1.05 $\pm$ 5%	5.93	5.93	5.93	0.33	2.77 $\pm$ 11.0%
1810	$\pm 50 / \pm 100$	53.3 $\pm$ 5%	1.52 $\pm$ 5%	4.58	4.58	4.58	0.75	2.63 $\pm$ 11.0%
1950	$\pm 50 / \pm 100$	53.3 $\pm$ 5%	1.52 $\pm$ 5%	4.54	4.54	4.54	0.99	2.20 $\pm$ 11.0%

<sup>c</sup> The validity of  $\pm 100$  MHz only applies for DASY v4.4 and higher (see Page 2). The uncertainty is the RSS of the ConvF uncertainty at calibration frequency and the uncertainty for the indicated frequency band.


 <p>Document  <b>Appendix D for the BlackBerry® Smartphone Model  RDU71CW/RDE71UW SAR Report Rev1</b></p>				Page <b>8(74)</b>
Author Data <b>Andrew Becker</b>	Dates of Test <b>Feb 7 – May 25, July 18,  2011</b>	Test Report No <b>RTS-3933-1105-11A  RTS-2580-1106-03 Rev1</b>	FCC ID: <b>L6ARDU70CW  L6ARDE70UW</b>	IC ID <b>2503A-RDU70CW  2503A-RDE70UW</b>

**ET3DV6 SN:1643**

**March 9, 2010**

## **Frequency Response of E-Field**

**(TEM-Cell:ifi110 EXX, Waveguide: R22)**

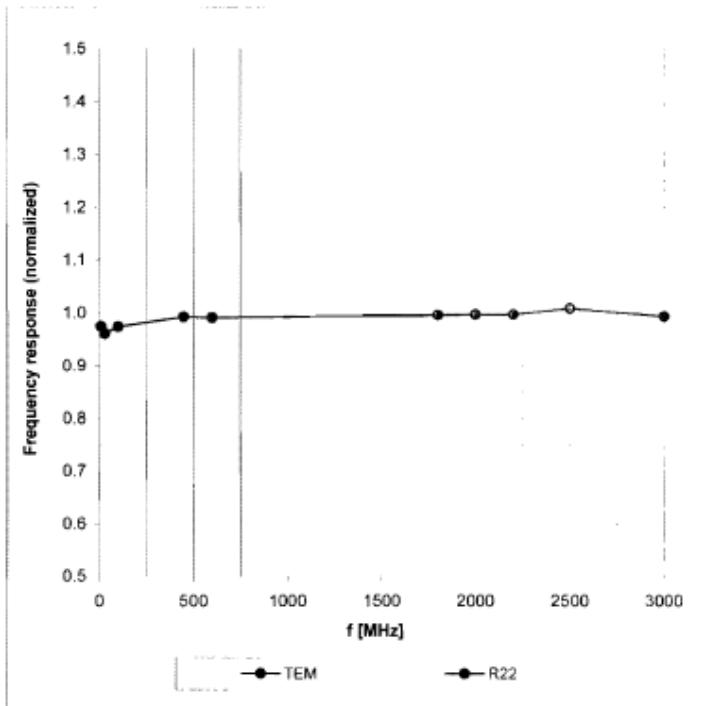



**Uncertainty of Frequency Response of E-field:  $\pm 6.3\%$  ( $k=2$ )**

Author Data <b>Andrew Becker</b>	Dates of Test <b>Feb 7 – May 25, July 18, 2011</b>	Test Report No <b>RTS-3933-1105-11A</b> <b>RTS-2580-1106-03 Rev1</b>	FCC ID: <b>L6ARDU70CW</b> <b>L6ARDE70UW</b>	IC ID <b>2503A-RDU70CW</b> <b>2503A-RDE70UW</b>
-------------------------------------	---	--	---	---

ET3DV6 SN:1643

March 9, 2010

### Receiving Pattern ( $\phi$ ), $\theta = 0^\circ$

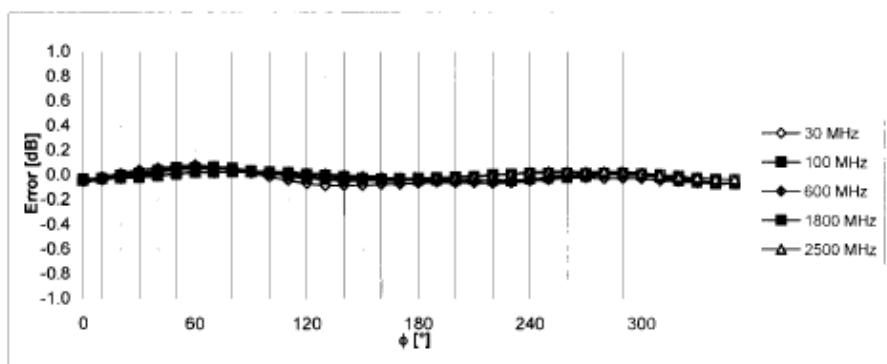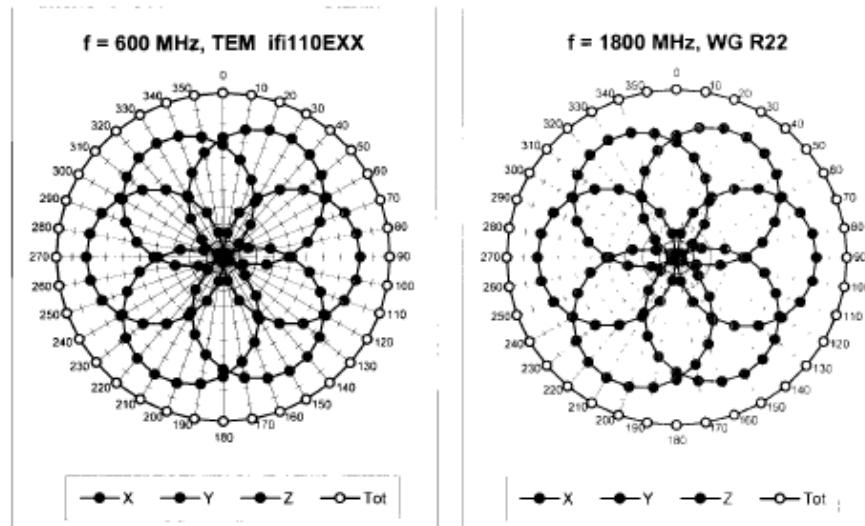

 Uncertainty of Axial Isotropy Assessment:  $\pm 0.5\%$  ( $k=2$ )

<b>RIM Testing Services</b>	Document <b>Appendix D for the BlackBerry® Smartphone Model RDU71CW/RDE71UW SAR Report Rev1</b>	Page <b>10(74)</b>
Author Data <b>Andrew Becker</b>	Dates of Test <b>Feb 7 – May 25, July 18, 2011</b>	Test Report No <b>RTS-3933-1105-11A RTS-2580-1106-03 Rev1</b> FCC ID: <b>L6ARDU70CW L6ARDE70UW</b> IC ID <b>2503A-RDU70CW 2503A-RDE70UW</b>

**ET3DV6 SN:1643**

**March 9, 2010**

**Dynamic Range  $f(\text{SAR}_{\text{head}})$**   
(Waveguide R22,  $f = 1800$  MHz)

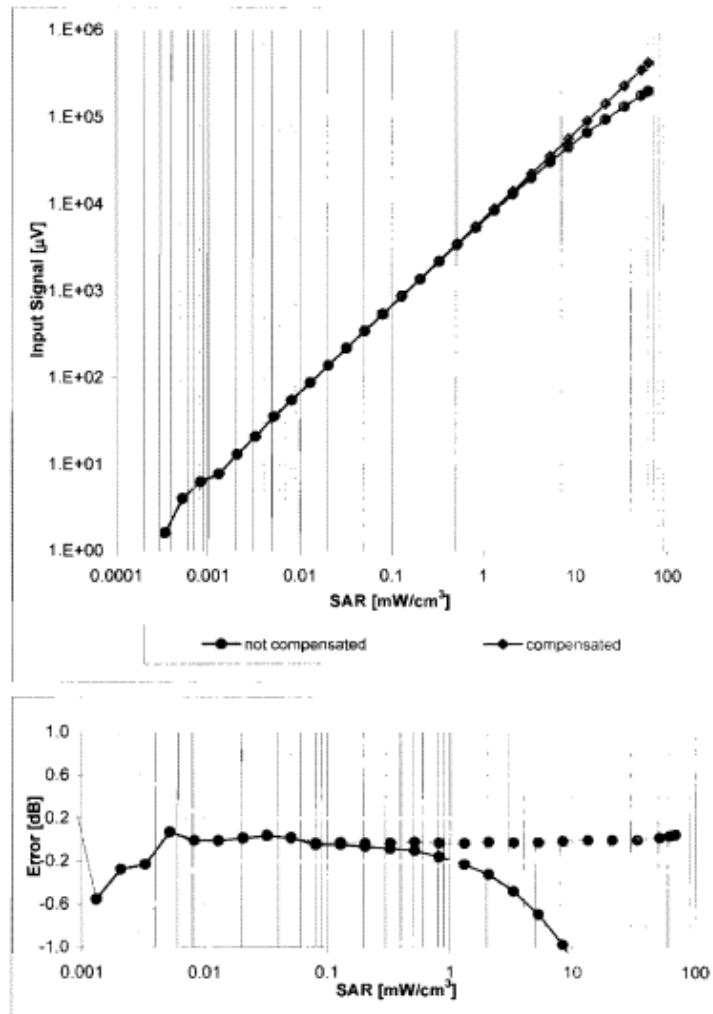


**Uncertainty of Linearity Assessment:  $\pm 0.6\%$  ( $k=2$ )**

Author Data <b>Andrew Becker</b>	Dates of Test <b>Feb 7 – May 25, July 18, 2011</b>	Test Report No <b>RTS-3933-1105-11A</b> <b>RTS-2580-1106-03 Rev1</b>	FCC ID: <b>L6ARDU70CW</b> <b>L6ARDE70UW</b>	IC ID <b>2503A-RDU70CW</b> <b>2503A-RDE70UW</b>
-------------------------------------	---	--	---	---


ET3DV6 SN:1643

March 9, 2010

## Conversion Factor Assessment

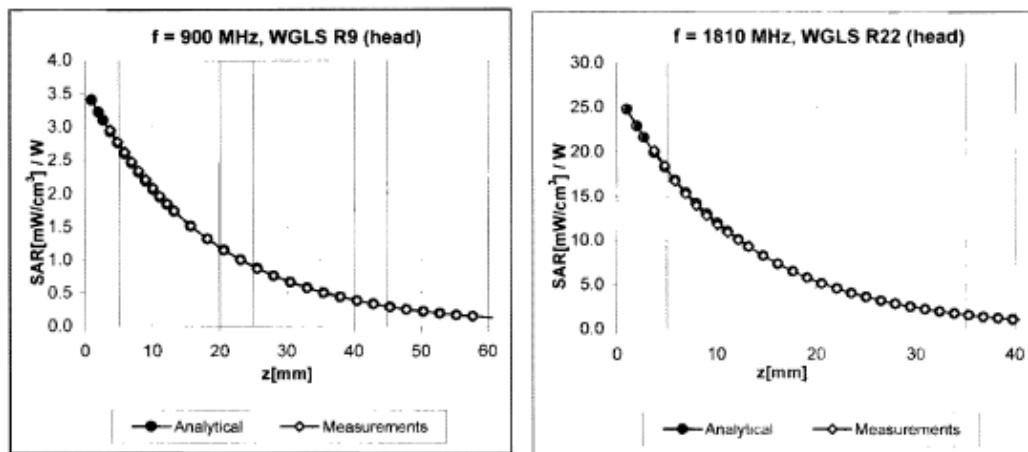

## Deviation from Isotropy in HSL

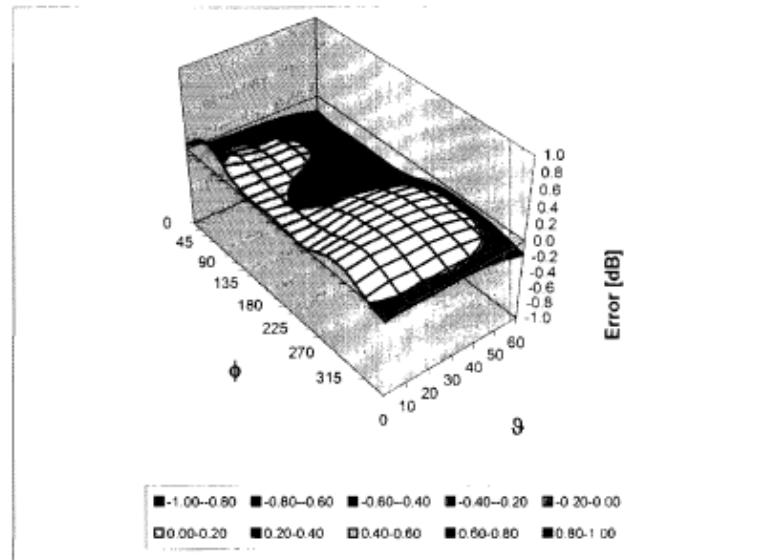Error ( $\phi, \theta$ ), f = 900 MHzUncertainty of Spherical Isotropy Assessment:  $\pm 2.6\%$  ( $k=2$ )



Document

**Appendix D for the BlackBerry® Smartphone Model  
RDU71CW/RDE71UW SAR Report Rev1**Page  
**12(74)**

Author Data <b>Andrew Becker</b>	Dates of Test <b>Feb 7 – May 25, July 18, 2011</b>	Test Report No <b>RTS-3933-1105-11A RTS-2580-1106-03 Rev1</b>	FCC ID: <b>L6ARDU70CW L6ARDE70UW</b>	IC ID <b>2503A-RDU70CW 2503A-RDE70UW</b>
-------------------------------------	---	--	---	---

**ET3DV6 SN:1643****March 9, 2010****Other Probe Parameters**

Sensor Arrangement	Triangular
Connector Angle (°)	Not applicable
Mechanical Surface Detection Mode	enabled
Optical Surface Detection Mode	enabled
Probe Overall Length	337 mm
Probe Body Diameter	10 mm
Tip Length	10 mm
Tip Diameter	6.8 mm
Probe Tip to Sensor X Calibration Point	2.7 mm
Probe Tip to Sensor Y Calibration Point	2.7 mm
Probe Tip to Sensor Z Calibration Point	2.7 mm
Recommended Measurement Distance from Surface	4 mm



Author Data <b>Andrew Becker</b>	Dates of Test <b>Feb 7 – May 25, July 18, 2011</b>	Test Report No <b>RTS-3933-1105-11A</b> <b>RTS-2580-1106-03 Rev1</b>	FCC ID: <b>L6ARDU70CW</b> <b>L6ARDE70UW</b>	IC ID <b>2503A-RDU70CW</b> <b>2503A-RDE70UW</b>
-------------------------------------	---	--	---	---

**Calibration Laboratory of**  
**Schmid & Partner**  
**Engineering AG**  
**Zeughausstrasse 43, 8004 Zurich, Switzerland**



**S** Schweizerischer Kalibrierdienst  
**C** Service suisse d'étalonnage  
**S** Servizio svizzero di taratura  
**S** Swiss Calibration Service

Accredited by the Swiss Accreditation Service (SAS)  
The Swiss Accreditation Service is one of the signatories to the EA  
Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: **SCS 108**

Client: **RTS (RIM Testing Services)**

Certificate No: **ET3-1644\_Nov10**

## CALIBRATION CERTIFICATE

Object	<b>ET3DV6 - SN:1644</b>
Calibration procedure(s)	<b>QA CAL-01.v6, QA CAL-23.v3 and QA CAL-25.v2</b> <b>Calibration procedure for dosimetric E-field probes</b>
Calibration date	<b>November 16, 2010</b>

This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI).  
The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility: environment temperature (22 ± 3)°C and humidity < 70%.

### Calibration Equipment used (M&TE critical for calibration)

Primary Standards	ID #	Cal Date (Certificate No.)	Scheduled Calibration
Power meter E44198	GB41293874	1-Apr-10 (No. 217-01138)	Apr-11
Power sensor E44128	MY41495277	1-Apr-10 (No. 217-01138)	Apr-11
Power sensor E4412A	MY41498867	1-Apr-10 (No. 217-01136)	Apr-11
Reference 3 dB Attenuator	SN: 55054 (3c)	30-Mar-10 (No. 217-01159)	Mar-11
Reference 20 dB Attenuator	SN: 55056 (20b)	30-Mar-10 (No. 217-01161)	Mar-11
Reference 30 dB Attenuator	SN: 55129 (30b)	30-Mar-10 (No. 217-01160)	Mar-11
Reference Probe E330V2	SN: 3013	30-Dec-09 (No. E33-3D13_Dec09)	Dec-10
DAE4	SN: 680	20-Apr-10 (No. DAE4-680_Apr10)	Apr-11

Secondary Standards	ID #	Check Date (in house)	Scheduled Check
RF generator HP 8645C	US3642U01700	4-Aug-09 (in house check Oct-09)	In house check: Oct-11
Network Analyzer HP 8753E	US37390585	18-Oct-09 (in house check Oct-10)	In house check: Oct-11

Calibrated by	Name	Function	Signature
	Jelena Kastell	Laboratory Technician	

Approved by	Name	Function	Signature
	Keija Pakkova	Technical Manager	

Issued: November 17, 2010

This calibration certificate shall not be reproduced except in full without written approval of the laboratory.

 <p>Document  <b>Appendix D for the BlackBerry® Smartphone Model  RDU71CW/RDE71UW SAR Report Rev1</b></p>				Page <b>14(74)</b>
Author Data <b>Andrew Becker</b>	Dates of Test <b>Feb 7 – May 25, July 18,  2011</b>	Test Report No <b>RTS-3933-1105-11A  RTS-2580-1106-03 Rev1</b>	FCC ID: <b>L6ARDU70CW  L6ARDE70UW</b>	IC ID <b>2503A-RDU70CW  2503A-RDE70UW</b>

**Calibration Laboratory of**  
**Schmid & Partner**  
**Engineering AG**  
**Zeughausstrasse 43, 8004 Zurich, Switzerland**



**S** Schweizerischer Kalibrierdienst  
**C** Service suisse d'étalonnage  
**S** Servizio svizzero di taratura  
**S** Swiss Calibration Service

Accredited by the Swiss Accreditation Service (SAS)  
The Swiss Accreditation Service is one of the signatories to the EA  
Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: **SCS 108**

#### Glossary:

TSL	tissue simulating liquid
NORM <sub>x,y,z</sub>	sensitivity in free space
ConvF	sensitivity in TSL / NORM <sub>x,y,z</sub>
DCP	diode compression point
CF	crest factor (1/duty_cycle) of the RF signal
A, B, C	modulation dependent linearization parameters
Polarization $\phi$	$\phi$ rotation around probe axis
Polarization $\theta$	$\theta$ rotation around an axis that is in the plane normal to probe axis (at measurement center), i.e., $\theta = 0$ is normal to probe axis

#### Calibration is Performed According to the Following Standards:

- IEEE Std 1528-2003, "IEEE Recommended Practice for Determining the Peak Spatial-Averaged Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques", December 2003
- IEC 62209-1, "Procedure to measure the Specific Absorption Rate (SAR) for hand-held devices used in close proximity to the ear (frequency range of 300 MHz to 3 GHz)", February 2005

#### Methods Applied and Interpretation of Parameters:

- $NORM_{x,y,z}$ : Assessed for E-field polarization  $\theta = 0$  ( $f \leq 900$  MHz in TEM-cell;  $f > 1800$  MHz: R22 waveguide).  $NORM_{x,y,z}$  are only intermediate values, i.e., the uncertainties of  $NORM_{x,y,z}$  does not effect the E<sup>2</sup>-field uncertainty inside TSL (see below ConvF).
- $NORM(f)x,y,z = NORM_{x,y,z} * \text{frequency\_response}$  (see Frequency Response Chart). This linearization is implemented in DASY4 software versions later than 4.2. The uncertainty of the frequency response is included in the stated uncertainty of ConvF.
- $DCPx,y,z$ : DCP are numerical linearization parameters assessed based on the data of power sweep with CW signal (no uncertainty required). DCP does not depend on frequency nor media.
- $Ax,y,z; Bx,y,z; Cx,y,z; VRx,y,z$ : A, B, C are numerical linearization parameters assessed based on the data of power sweep for specific modulation signal. The parameters do not depend on frequency nor media. VR is the maximum calibration range expressed in RMS voltage across the diode.
- ConvF and Boundary Effect Parameters:** Assessed in flat phantom using E-field (or Temperature Transfer Standard for  $f \leq 800$  MHz) and inside waveguide using analytical field distributions based on power measurements for  $f > 800$  MHz. The same setups are used for assessment of the parameters applied for boundary compensation (alpha, depth) of which typical uncertainty values are given. These parameters are used in DASY4 software to improve probe accuracy close to the boundary. The sensitivity in TSL corresponds to  $NORM_{x,y,z} * ConvF$  whereby the uncertainty corresponds to that given for ConvF. A frequency dependent ConvF is used in DASY version 4.4 and higher which allows extending the validity from  $\pm 50$  MHz to  $\pm 100$  MHz.
- Spherical Isotropy (3D deviation from isotropy):** in a field of low gradients realized using a flat phantom exposed by a patch antenna.
- Sensor Offset:** The sensor offset corresponds to the offset of virtual measurement center from the probe tip (on probe axis). No tolerance required.

	Document <b>Appendix D for the BlackBerry® Smartphone Model RDU71CW/RDE71UW SAR Report Rev1</b>	Page <b>15(74)</b>
Author Data <b>Andrew Becker</b>	Dates of Test <b>Feb 7 – May 25, July 18, 2011</b>	Test Report No <b>RTS-3933-1105-11A RTS-2580-1106-03 Rev1</b> FCC ID: <b>L6ARDU70CW L6ARDE70UW</b> IC ID <b>2503A-RDU70CW 2503A-RDE70UW</b>

**ET3DV6 SN:1644**

**November 16, 2010**

# Probe ET3DV6

## SN:1644

**Manufactured:** November 7, 2001  
**Last calibrated:** November 11, 2009  
**Recalibrated:** November 16, 2010

**Calibrated for DASY/EASY Systems**

(Note: non-compatible with DASY2 system!)



Document

**Appendix D for the BlackBerry® Smartphone Model  
RDU71CW/RDE71UW SAR Report Rev1**Page  
**16(74)**

Author Data <b>Andrew Becker</b>	Dates of Test <b>Feb 7 – May 25, July 18, 2011</b>	Test Report No <b>RTS-3933-1105-11A RTS-2580-1106-03 Rev1</b>	FCC ID: <b>L6ARDU70CW L6ARDE70UW</b>	IC ID <b>2503A-RDU70CW 2503A-RDE70UW</b>
-------------------------------------	---	--	---	---

ET3DV6 SN:1644

November 16, 2010

**DASY/EASY - Parameters of Probe: ET3DV6 SN:1644****Basic Calibration Parameters**

	Sensor X	Sensor Y	Sensor Z	Unc (k=2)
Norm ( $\mu$ V/(V/m) <sup>2</sup> ) <sup>a</sup>	1.83	1.95	2.01	$\pm 10.1\%$
DCP (mV) <sup>b</sup>	97.9	97.9	96.6	

**Modulation Calibration Parameters**

UID	Communication System Name	PAR		A dB	B dBuV	C	VR mV	Unc <sup>c</sup> (k=2)
10000	CW	0.00	X Y Z	0.00 0.00 0.00	0.00 0.00 0.00	1.00 1.00 1.00	143.5 146.8 146.4	$\pm 3.4\%$

The reported uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor k=2, which for a normal distribution corresponds to a coverage probability of approximately 95%.

<sup>a</sup> The uncertainties of Norm X, Y, Z do not affect the E<sup>2</sup>-field uncertainty inside TSL (see Pages 5 and 6)

<sup>b</sup> Numerical linearization parameter, uncertainty not required.

<sup>c</sup> Uncertainty is determined using the maximum deviation from linear response applying rectangular distribution and is expressed for the square of the field value.

	Document <b>Appendix D for the BlackBerry® Smartphone Model RDU71CW/RDE71UW SAR Report Rev1</b>	Page <b>17(74)</b>
Author Data <b>Andrew Becker</b>	Dates of Test <b>Feb 7 – May 25, July 18, 2011</b>	Test Report No <b>RTS-3933-1105-11A RTS-2580-1106-03 Rev1</b> FCC ID: <b>L6ARDU70CW L6ARDE70UW</b> IC ID <b>2503A-RDU70CW 2503A-RDE70UW</b>

ET3DV6 SN:1644

November 16, 2010

## DASY/EASY - Parameters of Probe: ET3DV6 SN:1644

### Calibration Parameter Determined in Head Tissue Simulating Media

f [MHz]	Validity [MHz] <sup>a</sup>	Permittivity	Conductivity	ConvF X	ConvF Y	ConvF Z	Alpha	Depth Unc (10^-2)
750	± 50 / ± 100	41.9 ± 5%	0.69 ± 5%	6.54	6.54	6.54	0.31	3.05 ± 11.0%
900	± 50 / ± 100	41.5 ± 5%	0.97 ± 5%	6.00	6.00	6.00	0.27	3.46 ± 11.0%
1810	± 50 / ± 100	40.0 ± 5%	1.40 ± 5%	5.09	5.09	5.09	0.40	2.50 ± 11.0%
2450	± 50 / ± 100	39.2 ± 5%	1.80 ± 5%	4.42	4.42	4.42	0.99	1.27 ± 11.0%

<sup>a</sup> The validity of ± 100 MHz only applies for DASY v4.4 and higher (see Page 2). The uncertainty is the RSS of the ConvF uncertainty at calibration frequency and the uncertainty for the indicated frequency band.

	Document <b>Appendix D for the BlackBerry® Smartphone Model RDU71CW/RDE71UW SAR Report Rev1</b>	Page <b>18(74)</b>
Author Data <b>Andrew Becker</b>	Dates of Test <b>Feb 7 – May 25, July 18, 2011</b>	Test Report No <b>RTS-3933-1105-11A RTS-2580-1106-03 Rev1</b>

**ET3DV6 SN:1644**

**November 16, 2010**

## **DASY/EASY - Parameters of Probe: ET3DV6 SN:1644**

### **Calibration Parameter Determined in Body Tissue Simulating Media**

<b>f [MHz]</b>	<b>Validity [MHz]<sup>a</sup></b>	<b>Permittivity</b>	<b>Conductivity</b>	<b>ConvF X</b>	<b>ConvF Y</b>	<b>ConvF Z</b>	<b>Alpha</b>	<b>Depth Unc (k=2)</b>
750	± 50 / ± 100	55.5 ± 5%	0.96 ± 5%	5.14	6.14	6.14	0.31	3.06 ± 11.0%
900	± 50 / ± 100	55.0 ± 5%	1.05 ± 5%	5.93	5.93	5.93	0.36	2.71 ± 11.0%
1810	± 50 / ± 100	53.3 ± 5%	1.52 ± 5%	4.59	4.59	4.59	0.32	2.60 ± 11.0%
2450	± 50 / ± 100	52.7 ± 5%	1.95 ± 5%	4.05	4.05	4.05	0.99	1.23 ± 11.0%

<sup>a</sup> The validity of ± 100 MHz only applies for DASY v4.4 and higher (see Page 2). The uncertainty is the RSS of the ConvF uncertainty at calibration frequency and the uncertainty for the indicated frequency band.


<b>RIM Testing Services</b>	Document <b>Appendix D for the BlackBerry® Smartphone Model RDU71CW/RDE71UW SAR Report Rev1</b>	Page <b>19(74)</b>
Author Data <b>Andrew Becker</b>	Dates of Test <b>Feb 7 – May 25, July 18, 2011</b>	Test Report No <b>RTS-3933-1105-11A RTS-2580-1106-03 Rev1</b> FCC ID: <b>L6ARDU70CW L6ARDE70UW</b> IC ID <b>2503A-RDU70CW 2503A-RDE70UW</b>

**ET3DV6 SN:1644**

**November 16, 2010**

### **Frequency Response of E-Field**

**(TEM-Cell: R110 EXX, Waveguide: R22)**

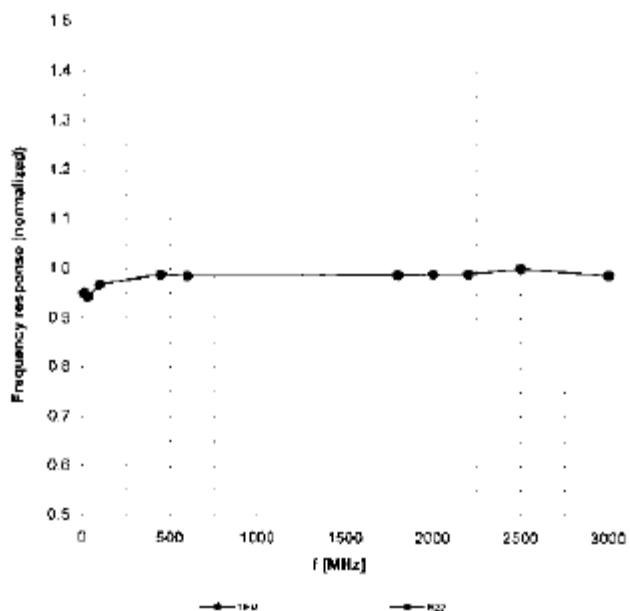

**Uncertainty of Frequency Response of E-field:  $\pm 6.3\%$  ( $k=2$ )**






Document

**Appendix D for the BlackBerry® Smartphone Model  
RDU71CW/RDE71UW SAR Report Rev1**Page  
**20(74)**

Author Data <b>Andrew Becker</b>	Dates of Test <b>Feb 7 – May 25, July 18, 2011</b>	Test Report No <b>RTS-3933-1105-11A</b> <b>RTS-2580-1106-03 Rev1</b>	FCC ID: <b>L6ARDU70CW</b> <b>L6ARDE70UW</b>	IC ID <b>2503A-RDU70CW</b> <b>2503A-RDE70UW</b>
-------------------------------------	---	--	---	---

ET3DV6 SN:1644

November 16, 2010

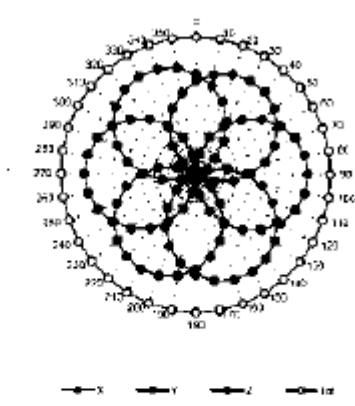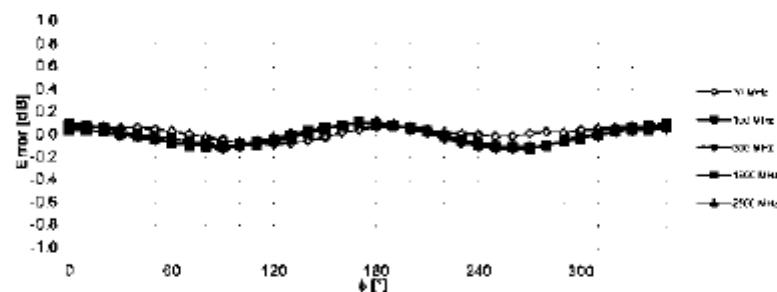
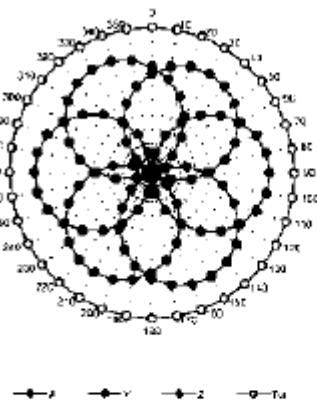
**Receiving Pattern ( $\phi$ ),  $\theta = 0^\circ$**  $f = 600 \text{ MHz, TEM i6110EXX}$  $f = 1800 \text{ MHz, WG R22}$ **Uncertainty of Axial Isotropy Assessment:  $\pm 0.5\%$  ( $k=2$ )**

Author Data <b>Andrew Becker</b>	Dates of Test <b>Feb 7 – May 25, July 18, 2011</b>	Test Report No <b>RTS-3933-1105-11A</b> <b>RTS-2580-1106-03 Rev1</b>	FCC ID: <b>L6ARDU70CW</b> <b>L6ARDE70UW</b>	IC ID <b>2503A-RDU70CW</b> <b>2503A-RDE70UW</b>
-------------------------------------	---	--	---	---

ET3DV6 SN:1644

November 16, 2010

### Dynamic Range $f(\text{SAR}_{\text{head}})$ (TEM cell, $f = 900 \text{ MHz}$ )

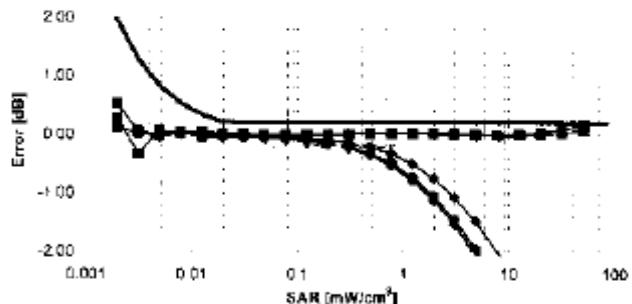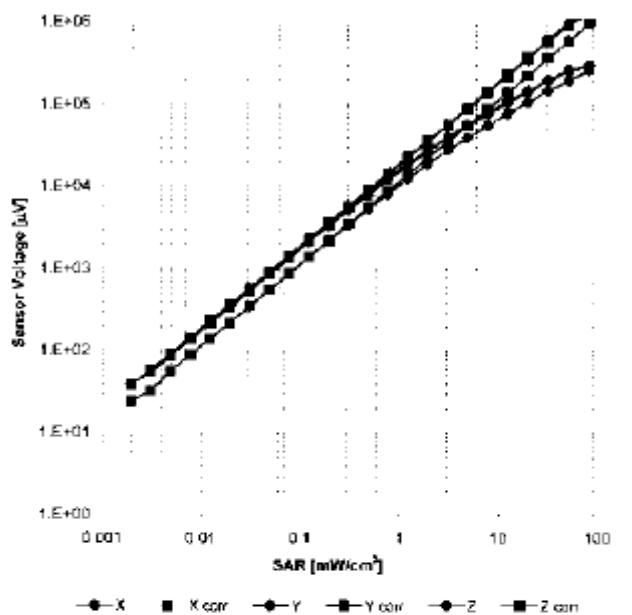

 Uncertainty of Linearity Assessment:  $\pm 0.6\%$  ( $k=2$ )

Author Data <b>Andrew Becker</b>	Dates of Test <b>Feb 7 – May 25, July 18, 2011</b>	Test Report No <b>RTS-3933-1105-11A</b> <b>RTS-2580-1106-03 Rev1</b>	FCC ID: <b>L6ARDU70CW</b> <b>L6ARDE70UW</b>	IC ID <b>2503A-RDU70CW</b> <b>2503A-RDE70UW</b>
-------------------------------------	---	--	---	---


ET3DV6 SN:1644

November 16, 2010

### Conversion Factor Assessment

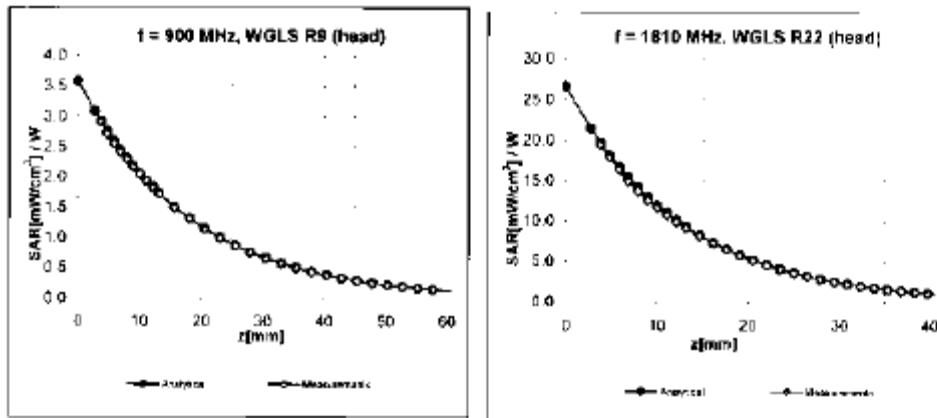

### Deviation from Isotropy in HSL

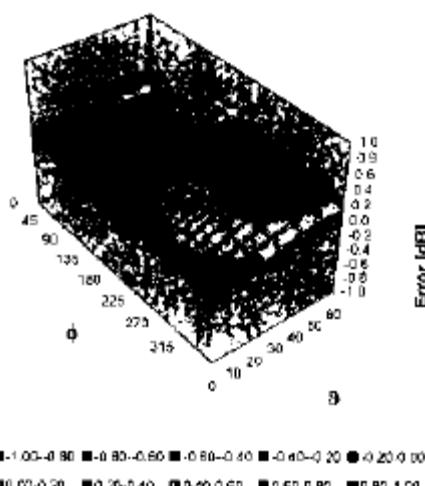Error ( $\phi, \theta$ ),  $f = 900$  MHz

■ -1.00--0.90 ■ 0.80--0.60 ■ -0.60--0.40 ■ -0.40--0.20 ■ 0.20--0.00

■ 0.00--0.20 ■ 0.20--0.40 ■ 0.40--0.60 ■ 0.60--0.80 ■ 0.80--1.00

Uncertainty of Spherical Isotropy Assessment:  $\pm 2.5\%$  ( $k=2$ )



Document

**Appendix D for the BlackBerry® Smartphone Model  
RDU71CW/RDE71UW SAR Report Rev1**Page  
**23(74)**

Author Data <b>Andrew Becker</b>	Dates of Test <b>Feb 7 – May 25, July 18, 2011</b>	Test Report No <b>RTS-3933-1105-11A RTS-2580-1106-03 Rev1</b>	FCC ID: <b>L6ARDU70CW L6ARDE70UW</b>	IC ID <b>2503A-RDU70CW 2503A-RDE70UW</b>
-------------------------------------	---	--	---	---

**ET3DV6 SN:1644****November 16, 2010****Other Probe Parameters**

Sensor Arrangement	Triangular
Connector Angle (°)	Not applicable
Mechanical Surface Detection Mode	enabled
Optical Surface Detection Mode	enabled
Probe Overall Length	337 mm
Probe Body Diameter	10 mm
Tip Length	10 mm
Tip Diameter	6.8 mm
Probe Tip to Sensor X Calibration Point	2.7 mm
Probe Tip to Sensor Y Calibration Point	2.7 mm
Probe Tip to Sensor Z Calibration Point	2.7 mm
Recommended Measurement Distance from Surface	3.7 mm



Author Data <b>Andrew Becker</b>	Dates of Test <b>Feb 7 – May 25, July 18, 2011</b>	Test Report No <b>RTS-3933-1105-11A</b> <b>RTS-2580-1106-03 Rev1</b>	FCC ID: <b>L6ARDU70CW</b> <b>L6ARDE70UW</b>	IC ID <b>2503A-RDU70CW</b> <b>2503A-RDE70UW</b>
-------------------------------------	---	--	---	---

**Calibration Laboratory of**  
**Schmid & Partner**  
**Engineering AG**  
**Zeughausstrasse 43, 8004 Zurich, Switzerland**



**S** Schweizerischer Kalibrierdienst  
**C** Service suisse d'étalonnage  
**S** Servizio svizzero di taratura  
**S** Swiss Calibration Service

Accredited by the Swiss Accreditation Service (SAS)  
The Swiss Accreditation Service is one of the signatories to the EA  
Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: **SCS 108**

Client **RTS (RIM Testing Services)**

Certificate No: **ES3-3225\_Jan11**

## **CALIBRATION CERTIFICATE**

Object **ES3DV3 - SN:3225**

Calibration procedure(s) **QA CAL-01.v7, QA CAL-23.v4 and QA CAL-25.v3**  
**Calibration procedure for dosimetric E-field probes**

Calibration date: **January 13, 2011**

This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI).  
The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility, environment temperature (22 ± 3)°C and humidity < 70%.

Calibration Equipment used (M&TE critical for calibration)

Primary Standards	ID #	Cal Date (Certificate No.)	Scheduled Calibration
Power meter E4419B	GB41293874	1-Apr-10 (No. 217-01136)	Apr-11
Power sensor E4412A	MY41495277	1-Apr-10 (No. 217-01136)	Apr-11
Power sensor E4412A	MY41498087	1-Apr-10 (No. 217-01136)	Apr-11
Reference 3 dB Attenuator	SN: S5054 (3c)	30-Mar-10 (No. 217-01159)	Mar-11
Reference 20 dB Attenuator	SN: S5086 (20b)	30-Mar-10 (No. 217-01161)	Mar-11
Reference 30 dB Attenuator	SN: S5129 (30b)	30-Mar-10 (No. 217-01160)	Mar-11
Reference Probe ES3DV2	SN: 3013	29-Dec-10 (No. ES3-3013_Dec10)	Dec-11
DAE4	SN: 680	20-Apr-10 (No. DAE4-680_Apr10)	Apr-11

Secondary Standards	ID #	Check Date (in house)	Scheduled Check
RF generator HP 8648C	US3642U01700	4-Aug-99 (in house check Oct-09)	In house check: Oct-11
Network Analyzer HP 8753E	US37390585	18-Oct-01 (in house check Oct-10)	In house check: Oct-11

Calibrated by:	Name	Function	Signature
	Jeton Kastrioti	Laboratory Technician	

Approved by:	Name	Function	Signature
	Katja Pokovic	Technical Manager	

Issued: January 15, 2011

This calibration certificate shall not be reproduced except in full without written approval of the laboratory.

 <p>Document  <b>Appendix D for the BlackBerry® Smartphone Model  RDU71CW/RDE71UW SAR Report Rev1</b></p>				Page <b>25(74)</b>
Author Data <b>Andrew Becker</b>	Dates of Test <b>Feb 7 – May 25, July 18, 2011</b>	Test Report No <b>RTS-3933-1105-11A</b> <b>RTS-2580-1106-03 Rev1</b>	FCC ID: <b>L6ARDU70CW</b> <b>L6ARDE70UW</b>	IC ID <b>2503A-RDU70CW</b> <b>2503A-RDE70UW</b>

**Calibration Laboratory of**  
**Schmid & Partner**  
**Engineering AG**  
**Zeughausstrasse 43, 8004 Zurich, Switzerland**



**S** Schweizerischer Kalibrierdienst  
**C** Service suisse d'étalonnage  
**S** Servizio svizzero di taratura  
**S** Swiss Calibration Service

Accredited by the Swiss Accreditation Service (SAS)  
The Swiss Accreditation Service is one of the signatories to the EA  
Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: **SCS 108**

### Glossary:

TSL	tissue simulating liquid
NORM <sub>x,y,z</sub>	sensitivity in free space
ConvF	sensitivity in TSL / NORM <sub>x,y,z</sub>
DCP	diode compression point
CF	crest factor (1/duty_cycle) of the RF signal
A, B, C	modulation dependent linearization parameters
Polarization $\phi$	$\phi$ rotation around probe axis
Polarization $\theta$	$\theta$ rotation around an axis that is in the plane normal to probe axis (at measurement center), i.e., $\theta = 0$ is normal to probe axis

### Calibration is Performed According to the Following Standards:

- IEEE Std 1528-2003, "IEEE Recommended Practice for Determining the Peak Spatial-Averaged Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques", December 2003
- IEC 62209-1, "Procedure to measure the Specific Absorption Rate (SAR) for hand-held devices used in close proximity to the ear (frequency range of 300 MHz to 3 GHz)", February 2005

### Methods Applied and Interpretation of Parameters:

- $NORM_{x,y,z}$ : Assessed for E-field polarization  $\theta = 0$  ( $f \leq 900$  MHz in TEM-cell;  $f > 1800$  MHz: R22 waveguide).  $NORM_{x,y,z}$  are only intermediate values, i.e., the uncertainties of  $NORM_{x,y,z}$  does not effect the  $E^2$ -field uncertainty inside TSL (see below  $ConvF$ ).
- $NORM(f)x,y,z = NORM_{x,y,z} * frequency\_response$  (see Frequency Response Chart). This linearization is implemented in DASY4 software versions later than 4.2. The uncertainty of the frequency response is included in the stated uncertainty of  $ConvF$ .
- $DCPx,y,z$ : DCP are numerical linearization parameters assessed based on the data of power sweep with CW signal (no uncertainty required). DCP does not depend on frequency nor media.
- $Ax,y,z$ ;  $Bx,y,z$ ;  $Cx,y,z$ ;  $VRx,y,z$ :  $A$ ,  $B$ ,  $C$  are numerical linearization parameters assessed based on the data of power sweep for specific modulation signal. The parameters do not depend on frequency nor media.  $VR$  is the maximum calibration range expressed in RMS voltage across the diode.
- ConvF and Boundary Effect Parameters*: Assessed in flat phantom using E-field (or Temperature Transfer Standard for  $f \leq 800$  MHz) and inside waveguide using analytical field distributions based on power measurements for  $f > 800$  MHz. The same setups are used for assessment of the parameters applied for boundary compensation (alpha, depth) of which typical uncertainty values are given. These parameters are used in DASY4 software to improve probe accuracy close to the boundary. The sensitivity in TSL corresponds to  $NORM_{x,y,z} * ConvF$  whereby the uncertainty corresponds to that given for  $ConvF$ . A frequency dependent  $ConvF$  is used in DASY version 4.4 and higher which allows extending the validity from  $\pm 50$  MHz to  $\pm 100$  MHz.
- Spherical isotropy (3D deviation from isotropy)*: in a field of low gradients realized using a flat phantom exposed by a patch antenna.
- Sensor Offset*: The sensor offset corresponds to the offset of virtual measurement center from the probe tip (on probe axis). No tolerance required.

 <p>Document  <b>Appendix D for the BlackBerry® Smartphone Model  RDU71CW/RDE71UW SAR Report Rev1</b></p>				Page <b>26(74)</b>
Author Data <b>Andrew Becker</b>	Dates of Test <b>Feb 7 – May 25, July 18,  2011</b>	Test Report No <b>RTS-3933-1105-11A  RTS-2580-1106-03 Rev1</b>	FCC ID: <b>L6ARDU70CW  L6ARDE70UW</b>	IC ID <b>2503A-RDU70CW  2503A-RDE70UW</b>

**ES3DV3 SN:3225**

**January 13, 2011**

# Probe ES3DV3

**SN:3225**

Manufactured: **September 1, 2009**  
Last calibrated: **December 11, 2009**  
Recalibrated: **January 13, 2011**

**Calibrated for DASY/EASY Systems**

(Note: non-compatible with DASY2 system!)



Document

**Appendix D for the BlackBerry® Smartphone Model  
RDU71CW/RDE71UW SAR Report Rev1**Page  
**27(74)**

Author Data <b>Andrew Becker</b>	Dates of Test <b>Feb 7 – May 25, July 18, 2011</b>	Test Report No <b>RTS-3933-1105-11A RTS-2580-1106-03 Rev1</b>	FCC ID: <b>L6ARDU70CW L6ARDE70UW</b>	IC ID <b>2503A-RDU70CW 2503A-RDE70UW</b>
-------------------------------------	---	--	---	---

ES3DV3 SN:3225

January 13, 2011

**DASY/EASY - Parameters of Probe: ES3DV3 SN:3225****Basic Calibration Parameters**

		Sensor X	Sensor Y	Sensor Z	Unc (k=2)
Norm ( $\mu$ V/(V/m) <sup>A</sup>		1.26	1.21	1.31	$\pm 10.1\%$
DCP (mV) <sup>B</sup>		102.1	100.8	99.1	

**Modulation Calibration Parameters**

UID	Communication System Name	PAR		A dB	B dBuV	C	VR mV	Unc <sup>C</sup> (k=2)
10000	CW	0.00	X Y Z	0.00 0.00 0.00	0.00 0.00 0.00	1.00 1.00 1.00	149.8 148.1 110.7	$\pm 2.6\%$

The reported uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor k=2, which for a normal distribution corresponds to a coverage probability of approximately 95%.

<sup>A</sup> The uncertainties of NormX,Y,Z do not affect the E<sup>2</sup>-field uncertainty inside TSL (see Pages 5 and 6).<sup>B</sup> Numerical linearization parameter, uncertainty not required.<sup>C</sup> Uncertainty is determined using the maximum deviation from linear response applying rectangular distribution and is expressed for the square of the field value.

	Document <b>Appendix D for the BlackBerry® Smartphone Model RDU71CW/RDE71UW SAR Report Rev1</b>	Page <b>28(74)</b>
Author Data <b>Andrew Becker</b>	Dates of Test <b>Feb 7 – May 25, July 18, 2011</b>	Test Report No <b>RTS-3933-1105-11A RTS-2580-1106-03 Rev1</b> FCC ID: <b>L6ARDU70CW L6ARDE70UW</b> IC ID <b>2503A-RDU70CW 2503A-RDE70UW</b>

ES3DV3 SN:3225

January 13, 2011

## DASY/EASY - Parameters of Probe: ES3DV3 SN:3225

### Calibration Parameter Determined in Head Tissue Simulating Media

f [MHz]	Validity [MHz] <sup>c</sup>	Permittivity	Conductivity	ConvF X	ConvF Y	ConvF Z	Alpha	Depth Unc (k=2)
750	± 50 / ± 100	41.9 ± 5%	0.89 ± 5%	6.47	6.47	6.47	0.89	1.08 ± 11.0%
900	± 50 / ± 100	41.5 ± 5%	0.97 ± 5%	6.11	6.11	6.11	0.81	1.10 ± 11.0%
1810	± 50 / ± 100	40.0 ± 5%	1.40 ± 5%	5.26	5.26	5.26	0.37	1.68 ± 11.0%
1950	± 50 / ± 100	40.0 ± 5%	1.40 ± 5%	4.98	4.98	4.98	0.48	1.51 ± 11.0%
2450	± 50 / ± 100	39.2 ± 5%	1.80 ± 5%	4.60	4.60	4.60	0.52	1.54 ± 11.0%
2600	± 50 / ± 100	39.0 ± 5%	1.96 ± 5%	4.52	4.52	4.52	0.53	1.58 ± 11.0%

<sup>c</sup> The validity of ± 100 MHz only applies for DASY v4.4 and higher (see Page 2). The uncertainty is the RSS of the ConvF uncertainty at calibration frequency and the uncertainty for the indicated frequency band.

 <p>Document  <b>Appendix D for the BlackBerry® Smartphone Model  RDU71CW/RDE71UW SAR Report Rev1</b></p>		Page <b>29(74)</b>	
Author Data <b>Andrew Becker</b>	Dates of Test <b>Feb 7 – May 25, July 18, 2011</b>	Test Report No <b>RTS-3933-1105-11A  RTS-2580-1106-03 Rev1</b>	FCC ID: <b>L6ARDU70CW  L6ARDE70UW</b> IC ID <b>2503A-RDU70CW  2503A-RDE70UW</b>

**ES3DV3 SN:3225**

**January 13, 2011**

## **DASY/EASY - Parameters of Probe: ES3DV3 SN:3225**

### **Calibration Parameter Determined in Body Tissue Simulating Media**

<b>f [MHz]</b>	<b>Validity [MHz]<sup>c</sup></b>	<b>Permittivity</b>	<b>Conductivity</b>	<b>ConvF X</b>	<b>ConvF Y</b>	<b>ConvF Z</b>	<b>Alpha</b>	<b>Depth Unc (k=2)</b>
750	± 50 / ± 100	55.5 ± 5%	0.96 ± 5%	6.30	6.30	6.30	0.76	1.17 ± 11.0%
900	± 50 / ± 100	55.0 ± 5%	1.05 ± 5%	6.12	6.12	6.12	0.72	1.20 ± 11.0%
1810	± 50 / ± 100	53.3 ± 5%	1.52 ± 5%	4.88	4.88	4.88	0.26	2.70 ± 11.0%
1950	± 50 / ± 100	53.3 ± 5%	1.52 ± 5%	4.89	4.89	4.89	0.33	2.28 ± 11.0%
2450	± 50 / ± 100	52.7 ± 5%	1.95 ± 5%	4.43	4.43	4.43	0.99	1.04 ± 11.0%
2600	± 50 / ± 100	52.5 ± 5%	2.16 ± 5%	4.29	4.29	4.29	0.99	1.05 ± 11.0%

<sup>c</sup> The validity of ± 100 MHz only applies for DASY v4.4 and higher (see Page 2). The uncertainty is the RSS of the ConvF uncertainty at calibration frequency and the uncertainty for the indicated frequency band.




Document

**Appendix D for the BlackBerry® Smartphone Model  
RDU71CW/RDE71UW SAR Report Rev1**Page  
**30(74)**

Author Data <b>Andrew Becker</b>	Dates of Test <b>Feb 7 – May 25, July 18, 2011</b>	Test Report No <b>RTS-3933-1105-11A</b> <b>RTS-2580-1106-03 Rev1</b>	FCC ID: <b>L6ARDU70CW</b> <b>L6ARDE70UW</b>	IC ID <b>2503A-RDU70CW</b> <b>2503A-RDE70UW</b>
-------------------------------------	---	--	---	---

**ES3DV3 SN:3225****January 13, 2011****Frequency Response of E-Field**

(TEM-Cell:ifi110 EXX, Waveguide: R22)


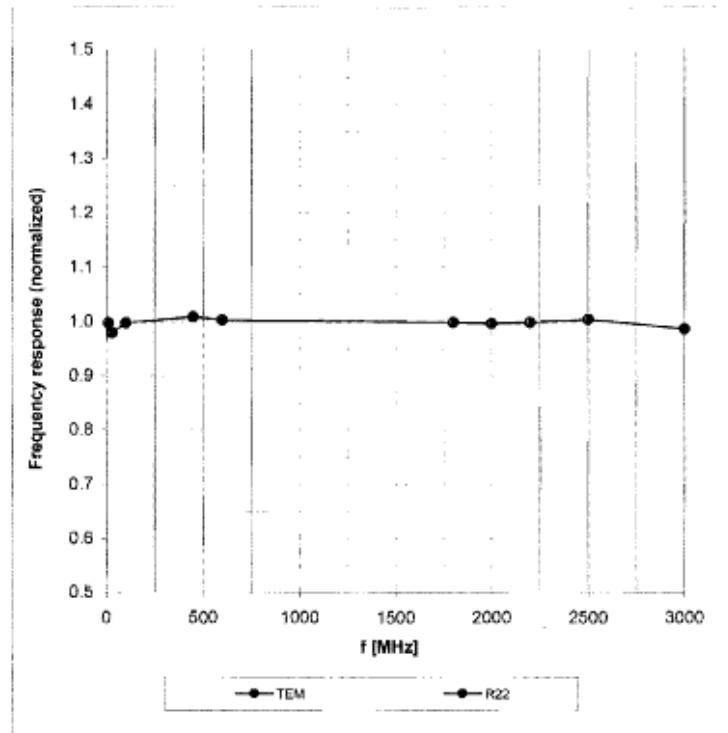
**Uncertainty of Frequency Response of E-field:  $\pm 6.3\% (k=2)$**

Author Data <b>Andrew Becker</b>	Dates of Test <b>Feb 7 – May 25, July 18, 2011</b>	Test Report No <b>RTS-3933-1105-11A</b> <b>RTS-2580-1106-03 Rev1</b>	FCC ID: <b>L6ARDU70CW</b> <b>L6ARDE70UW</b>	IC ID <b>2503A-RDU70CW</b> <b>2503A-RDE70UW</b>
-------------------------------------	---	--	---	---

ES3DV3 SN:3225

January 13, 2011

### Receiving Pattern ( $\phi$ ), $\theta = 0^\circ$

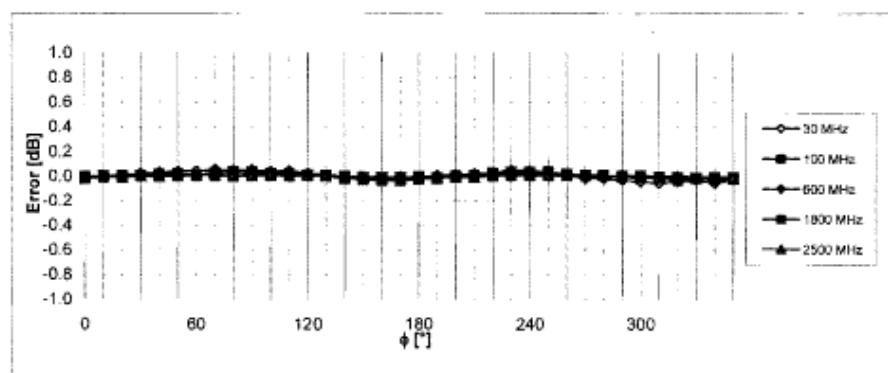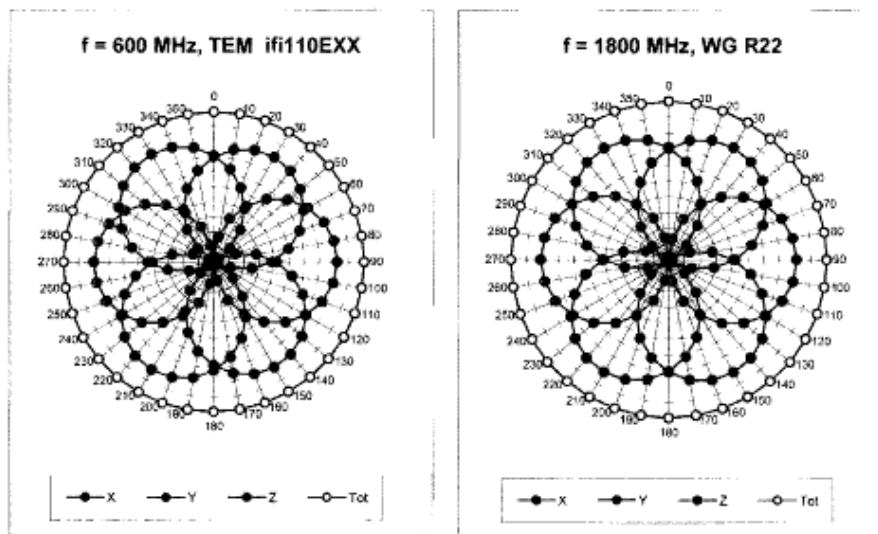
 Uncertainty of Axial Isotropy Assessment:  $\pm 0.5\%$  ( $k=2$ )



Author Data <b>Andrew Becker</b>	Dates of Test <b>Feb 7 – May 25, July 18, 2011</b>	Test Report No <b>RTS-3933-1105-11A</b> <b>RTS-2580-1106-03 Rev1</b>	FCC ID: <b>L6ARDU70CW</b> <b>L6ARDE70UW</b>	IC ID <b>2503A-RDU70CW</b> <b>2503A-RDE70UW</b>
-------------------------------------	---	--	---	---

ES3DV3 SN:3225

January 13, 2011

### Dynamic Range f(SAR<sub>head</sub>)

(TEM cell, f = 900 MHz)

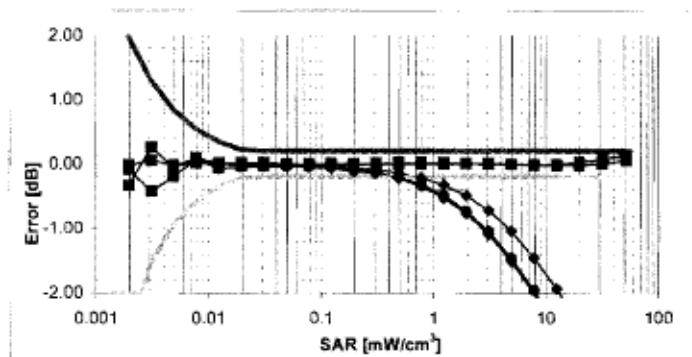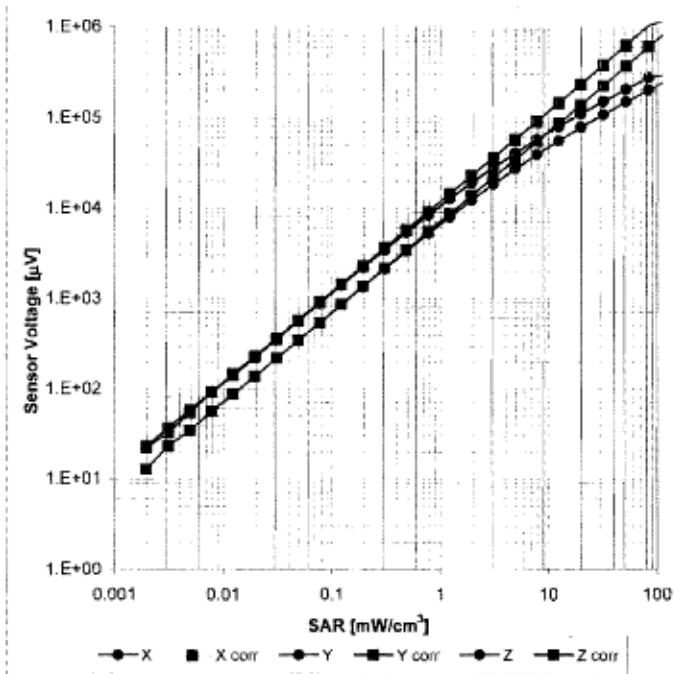


Uncertainty of Linearity Assessment: ± 0.6% (k=2)

 <p>Document  <b>Appendix D for the BlackBerry® Smartphone Model  RDU71CW/RDE71UW SAR Report Rev1</b></p>				Page <b>33(74)</b>
Author Data <b>Andrew Becker</b>	Dates of Test <b>Feb 7 – May 25, July 18, 2011</b>	Test Report No <b>RTS-3933-1105-11A</b> <b>RTS-2580-1106-03 Rev1</b>	FCC ID: <b>L6ARDU70CW</b> <b>L6ARDE70UW</b>	IC ID <b>2503A-RDU70CW</b> <b>2503A-RDE70UW</b>

**ES3DV3 SN:3225**


**January 13, 2011**

## Conversion Factor Assessment

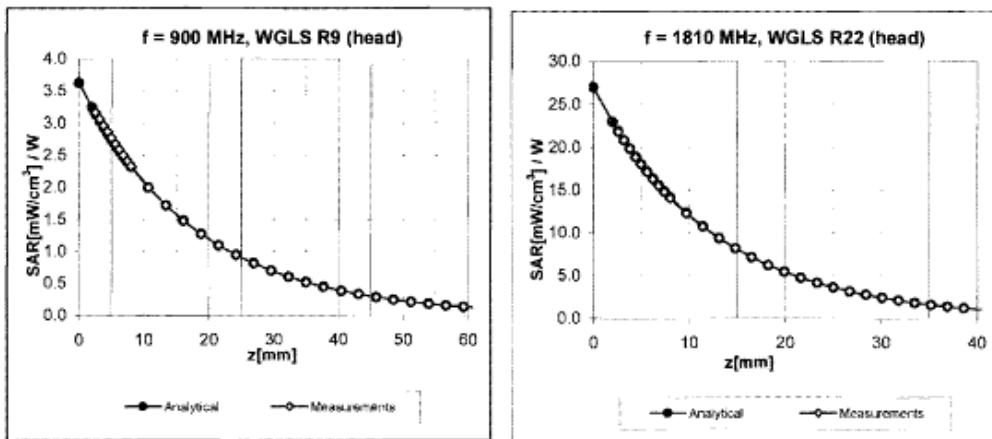

## Deviation from Isotropy in HSL

Error ( $\phi, \theta$ ),  $f = 900$  MHz

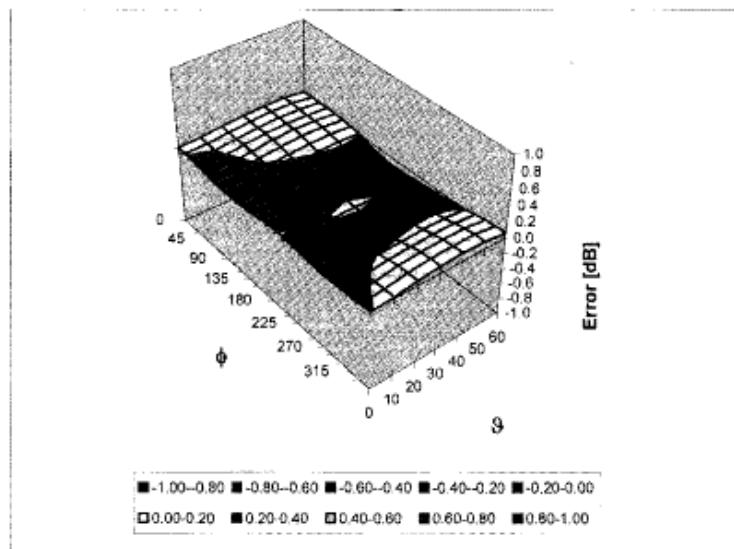

Uncertainty of Spherical Isotropy Assessment:  $\pm 2.6\%$  ( $k=2$ )



Document

**Appendix D for the BlackBerry® Smartphone Model  
RDU71CW/RDE71UW SAR Report Rev1**Page  
**34(74)**

Author Data <b>Andrew Becker</b>	Dates of Test <b>Feb 7 – May 25, July 18, 2011</b>	Test Report No <b>RTS-3933-1105-11A RTS-2580-1106-03 Rev1</b>	FCC ID: <b>L6ARDU70CW L6ARDE70UW</b>	IC ID <b>2503A-RDU70CW 2503A-RDE70UW</b>
-------------------------------------	---	--	---	---

**ES3DV3 SN:3225****January 13, 2011**

## Other Probe Parameters

Sensor Arrangement	Triangular
Connector Angle (°)	Not applicable
Mechanical Surface Detection Mode	enabled
Optical Surface Detection Mode	disabled
Probe Overall Length	337 mm
Probe Body Diameter	10 mm
Tip Length	10 mm
Tip Diameter	4 mm
Probe Tip to Sensor X Calibration Point	2 mm
Probe Tip to Sensor Y Calibration Point	2 mm
Probe Tip to Sensor Z Calibration Point	2 mm
Recommended Measurement Distance from Surface	3 mm

	Document <b>Appendix D for the BlackBerry® Smartphone Model RDU71CW/RDE71UW SAR Report Rev1</b>	Page <b>35(74)</b>
Author Data <b>Andrew Becker</b>	Dates of Test <b>Feb 7 – May 25, July 18, 2011</b>	Test Report No <b>RTS-3933-1105-11A RTS-2580-1106-03 Rev1</b> FCC ID: <b>L6ARDU70CW L6ARDE70UW</b> IC ID <b>2503A-RDU70CW 2503A-RDE70UW</b>

**Calibration Laboratory of**  
Schmid & Partner  
Engineering AG  
Zeughausstrasse 43, 8004 Zurich, Switzerland



**S** Schweizerischer Kalibrierdienst  
**C** Service suisse d'étalonnage  
**S** Servizio svizzero di taratura  
**S** Swiss Calibration Service

Accredited by the Swiss Accreditation Service (SAS)  
The Swiss Accreditation Service is one of the signatories to the EA  
Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: **SCS 108**

Client **RTS (RIM Testing Services)**

Certificate No: **EX3-3548\_Jan11**

## **CALIBRATION CERTIFICATE**

Object	<b>EX3DV4 - SN:3548</b>		
Calibration procedure(s)	<b>QA CAL-01.v7, QA CAL-14.v3, QA CAL-23.v4 and QA CAL-25.v3 Calibration procedure for dosimetric E-field probes</b>		
Calibration date:	<b>January 20, 2011</b>		
<p>This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI). The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.</p> <p>All calibrations have been conducted in the closed laboratory facility: environment temperature (22 ± 3)°C and humidity &lt; 70%.</p> <p>Calibration Equipment used (M&amp;TE critical for calibration)</p>			
Primary Standards	ID #	Cal Date (Certificate No.)	Scheduled Calibration
Power meter E4419B	GB41293874	1-Apr-10 (No. 217-01136)	Apr-11
Power sensor E4412A	MY41495277	1-Apr-10 (No. 217-01136)	Apr-11
Power sensor E4412A	MY41498087	1-Apr-10 (No. 217-01136)	Apr-11
Reference 3 dB Attenuator	SN: S5054 (3c)	30-Mar-10 (No. 217-01159)	Mar-11
Reference 20 dB Attenuator	SN: S5086 (20b)	30-Mar-10 (No. 217-01161)	Mar-11
Reference 30 dB Attenuator	SN: S5129 (30b)	30-Mar-10 (No. 217-01160)	Mar-11
Reference Probe ES3DV2	SN: 3013	29-Dec-10 (No. ES3-3013_Dec10)	Dec-11
DAE4	SN: 660	20-Apr-10 (No. DAE4-660_Apr10)	Apr-11
Secondary Standards	ID #	Check Date (in house)	Scheduled Check
RF generator HP 8648C	US3642U01700	4-Aug-99 (in house check Oct-09)	In house check: Oct-11
Network Analyzer HP 8753E	US37390585	18-Oct-01 (in house check Oct-10)	In house check: Oct-11
Calibrated by:	Name <b>Katja Pokovic</b>	Function <b>Technical Manager</b>	Signature 
Approved by:	Name <b>Niels Kuster</b>	Function <b>Quality Manager</b>	Signature 
Issued: January 20, 2011			
This calibration certificate shall not be reproduced except in full without written approval of the laboratory.			

Certificate No: **EX3-3548\_Jan11**

Page 1 of 11

This report shall NOT be reproduced except in full without the written consent of RIM Testing Services  
Copyright 2005-2011, RIM Testing Services, a division of Research In Motion Limited

 <p>Document  <b>Appendix D for the BlackBerry® Smartphone Model  RDU71CW/RDE71UW SAR Report Rev1</b></p>				Page <b>36(74)</b>
Author Data <b>Andrew Becker</b>	Dates of Test <b>Feb 7 – May 25, July 18, 2011</b>	Test Report No <b>RTS-3933-1105-11A  RTS-2580-1106-03 Rev1</b>	FCC ID: <b>L6ARDU70CW  L6ARDE70UW</b>	IC ID <b>2503A-RDU70CW  2503A-RDE70UW</b>

**Calibration Laboratory of**  
**Schmid & Partner**  
**Engineering AG**  
**Zeughausstrasse 43, 8004 Zurich, Switzerland**



**S** Schweizerischer Kalibrierdienst  
**C** Service suisse d'étalonnage  
**S** Servizio svizzero di taratura  
**S** Swiss Calibration Service

Accredited by the Swiss Accreditation Service (SAS)  
The Swiss Accreditation Service is one of the signatories to the EA  
Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: **SCS 108**

### Glossary:

TSL	tissue simulating liquid
NORM <sub>x,y,z</sub>	sensitivity in free space
ConvF	sensitivity in TSL / NORM <sub>x,y,z</sub>
DCP	diode compression point
CF	crest factor (1/duty_cycle) of the RF signal
A, B, C	modulation dependent linearization parameters
Polarization $\varphi$	$\varphi$ rotation around probe axis
Polarization $\theta$	$\theta$ rotation around an axis that is in the plane normal to probe axis (at measurement center), i.e., $\theta = 0$ is normal to probe axis

### Calibration is Performed According to the Following Standards:

- IEEE Std 1528-2003, "IEEE Recommended Practice for Determining the Peak Spatial-Averaged Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques", December 2003
- IEC 62209-1, "Procedure to measure the Specific Absorption Rate (SAR) for hand-held devices used in close proximity to the ear (frequency range of 300 MHz to 3 GHz)", February 2005

### Methods Applied and Interpretation of Parameters:

- NORM<sub>x,y,z</sub>**: Assessed for E-field polarization  $\theta = 0$  ( $f \leq 900$  MHz in TEM-cell;  $f > 1800$  MHz: R22 waveguide). NORM<sub>x,y,z</sub> are only intermediate values, i.e., the uncertainties of NORM<sub>x,y,z</sub> does not effect the E<sup>2</sup>-field uncertainty inside TSL (see below ConvF).
- NORM(f)<sub>x,y,z</sub> = NORM<sub>x,y,z</sub> \* frequency\_response** (see Frequency Response Chart). This linearization is implemented in DASY4 software versions later than 4.2. The uncertainty of the frequency response is included in the stated uncertainty of ConvF.
- DCPx,y,z**: DCP are numerical linearization parameters assessed based on the data of power sweep with CW signal (no uncertainty required). DCP does not depend on frequency nor media.
- A<sub>x,y,z</sub>; B<sub>x,y,z</sub>; C<sub>x,y,z</sub>; VR<sub>x,y,z</sub>**: A, B, C are numerical linearization parameters assessed based on the data of power sweep for specific modulation signal. The parameters do not depend on frequency nor media. VR is the maximum calibration range expressed in RMS voltage across the diode.
- ConvF and Boundary Effect Parameters**: Assessed in flat phantom using E-field (or Temperature Transfer Standard for  $f \leq 800$  MHz) and inside waveguide using analytical field distributions based on power measurements for  $f > 800$  MHz. The same setups are used for assessment of the parameters applied for boundary compensation (alpha, depth) of which typical uncertainty values are given. These parameters are used in DASY4 software to improve probe accuracy close to the boundary. The sensitivity in TSL corresponds to  $NORM<sub>x,y,z</sub> * ConvF$  whereby the uncertainty corresponds to that given for ConvF. A frequency dependent ConvF is used in DASY version 4.4 and higher which allows extending the validity from  $\pm 50$  MHz to  $\pm 100$  MHz.
- Spherical isotropy (3D deviation from isotropy)**: in a field of low gradients realized using a flat phantom exposed by a patch antenna.
- Sensor Offset**: The sensor offset corresponds to the offset of virtual measurement center from the probe tip (on probe axis). No tolerance required.

	Document <b>Appendix D for the BlackBerry® Smartphone Model RDU71CW/RDE71UW SAR Report Rev1</b>	Page <b>37(74)</b>
Author Data <b>Andrew Becker</b>	Dates of Test <b>Feb 7 – May 25, July 18, 2011</b>	Test Report No <b>RTS-3933-1105-11A RTS-2580-1106-03 Rev1</b> FCC ID: <b>L6ARDU70CW L6ARDE70UW</b> IC ID <b>2503A-RDU70CW 2503A-RDE70UW</b>

**EX3DV4 SN:3548**

**January 20, 2011**

# Probe EX3DV4

## SN:3548

Manufactured: November 16, 2004  
 Last calibrated: January 21, 2010  
 Recalibrated: January 20, 2011

**Calibrated for DASY/EASY Systems**

(Note: non-compatible with DASY2 system!)



Author Data <b>Andrew Becker</b>	Dates of Test <b>Feb 7 – May 25, July 18, 2011</b>	Test Report No <b>RTS-3933-1105-11A RTS-2580-1106-03 Rev1</b>	FCC ID: <b>L6ARDU70CW L6ARDE70UW</b>	IC ID <b>2503A-RDU70CW 2503A-RDE70UW</b>
-------------------------------------	---	--	---	---

**EX3DV4 SN:3548**

**January 20, 2011**

## **DASY/EASY - Parameters of Probe: EX3DV4 SN:3548**

### **Basic Calibration Parameters**

	<b>Sensor X</b>	<b>Sensor Y</b>	<b>Sensor Z</b>	<b>Unc (k=2)</b>
Norm ( $\mu$ V/(V/m)) <sup>2</sup> <sup>A</sup>	0.35	0.44	0.45	$\pm$ 10.1%
DCP (mV) <sup>B</sup>	101.4	100.4	99.2	

### **Modulation Calibration Parameters**

<b>UID</b>	<b>Communication System Name</b>	<b>PAR</b>		<b>A</b> <b>dB</b>	<b>B</b> <b>dBuV</b>	<b>C</b>	<b>VR</b> <b>mV</b>	<b>Unc<sup>E</sup></b> <b>(k=2)</b>
10000	CW	0.00	X Y Z	0.00 0.00 0.00	0.00 0.00 0.00	1.00 1.00 1.00	128.8 139.9 142.9	$\pm$ 2.9 %

The reported uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor k=2, which for a normal distribution corresponds to a coverage probability of approximately 95%.

<sup>A</sup> The uncertainties of NormX,Y,Z do not affect the E<sup>2</sup>-field uncertainty inside TSL (see Pages 5 and 6).

<sup>B</sup> Numerical linearization parameter: uncertainty not required.

<sup>E</sup> Uncertainty is determined using the maximum deviation from linear response applying rectangular distribution and is expressed for the square of the field value.

 Document	<b>Appendix D for the BlackBerry® Smartphone Model RDU71CW/RDE71UW SAR Report Rev1</b>					Page <b>39(74)</b>
	Author Data <b>Andrew Becker</b>	Dates of Test <b>Feb 7 – May 25, July 18, 2011</b>	Test Report No <b>RTS-3933-1105-11A</b> <b>RTS-2580-1106-03 Rev1</b>	FCC ID: <b>L6ARDU70CW</b> <b>L6ARDE70UW</b>	IC ID <b>2503A-RDU70CW</b> <b>2503A-RDE70UW</b>	

**EX3DV4 SN:3548**

**January 20, 2011**

## **DASY/EASY - Parameters of Probe: EX3DV4 SN:3548**

### **Calibration Parameter Determined in Head Tissue Simulating Media**

<b>f [MHz]</b>	<b>Validity [MHz]<sup>c</sup></b>	<b>Permittivity</b>	<b>Conductivity</b>	<b>ConvF X</b>	<b>ConvF Y</b>	<b>ConvF Z</b>	<b>Alpha</b>	<b>Depth Unc (k=2)</b>
2600	$\pm 50 / \pm 100$	$39.0 \pm 5\%$	$1.96 \pm 5\%$	7.08	7.08	7.08	0.23	$1.34 \pm 11.0\%$
5200	$\pm 50 / \pm 100$	$36.0 \pm 5\%$	$4.66 \pm 5\%$	5.01	5.01	5.01	0.40	$1.80 \pm 13.1\%$
5500	$\pm 50 / \pm 100$	$35.6 \pm 5\%$	$4.96 \pm 5\%$	4.63	4.63	4.63	0.50	$1.80 \pm 13.1\%$
5800	$\pm 50 / \pm 100$	$35.3 \pm 5\%$	$5.27 \pm 5\%$	4.42	4.42	4.42	0.50	$1.80 \pm 13.1\%$

<sup>c</sup> The validity of  $\pm 100$  MHz only applies for DASY v4.4 and higher (see Page 2). The uncertainty is the RSS of the ConvF uncertainty at calibration frequency and the uncertainty for the indicated frequency band.

	Document <b>Appendix D for the BlackBerry® Smartphone Model RDU71CW/RDE71UW SAR Report Rev1</b>	Page <b>40(74)</b>
Author Data <b>Andrew Becker</b>	Dates of Test <b>Feb 7 – May 25, July 18, 2011</b>	Test Report No <b>RTS-3933-1105-11A RTS-2580-1106-03 Rev1</b> FCC ID: <b>L6ARDU70CW L6ARDE70UW</b> IC ID <b>2503A-RDU70CW 2503A-RDE70UW</b>

**EX3DV4 SN:3548**

**January 20, 2011**

## **DASY/EASY - Parameters of Probe: EX3DV4 SN:3548**

### **Calibration Parameter Determined in Body Tissue Simulating Media**

<b>f [MHz]</b>	<b>Validity [MHz]<sup>c</sup></b>	<b>Permittivity</b>	<b>Conductivity</b>	<b>ConvF X</b>	<b>ConvF Y</b>	<b>ConvF Z</b>	<b>Alpha</b>	<b>Depth Unc (k=2)</b>
2600	$\pm 50 / \pm 100$	$52.5 \pm 5\%$	$2.16 \pm 5\%$	7.12	7.12	7.12	0.67	$0.71 \pm 11.0\%$
5200	$\pm 50 / \pm 100$	$49.0 \pm 5\%$	$5.30 \pm 5\%$	4.79	4.79	4.79	0.45	$1.90 \pm 13.1\%$
5500	$\pm 50 / \pm 100$	$48.6 \pm 5\%$	$5.65 \pm 5\%$	4.29	4.29	4.29	0.50	$1.90 \pm 13.1\%$
5800	$\pm 50 / \pm 100$	$48.2 \pm 5\%$	$6.00 \pm 5\%$	4.08	4.08	4.08	0.60	$1.90 \pm 13.1\%$

<sup>c</sup> The validity of  $\pm 100$  MHz only applies for DASY v4.4 and higher (see Page 2). The uncertainty is the RSS of the ConvF uncertainty at calibration frequency and the uncertainty for the indicated frequency band.


	Document <b>Appendix D for the BlackBerry® Smartphone Model RDU71CW/RDE71UW SAR Report Rev1</b>	Page <b>41(74)</b>
Author Data <b>Andrew Becker</b>	Dates of Test <b>Feb 7 – May 25, July 18, 2011</b>	Test Report No <b>RTS-3933-1105-11A RTS-2580-1106-03 Rev1</b> FCC ID: <b>L6ARDU70CW L6ARDE70UW</b> IC ID <b>2503A-RDU70CW 2503A-RDE70UW</b>

**EX3DV4 SN:3548**

**January 20, 2011**

## **Frequency Response of E-Field**

**(TEM-Cell:ifi110 EXX, Waveguide: R22)**



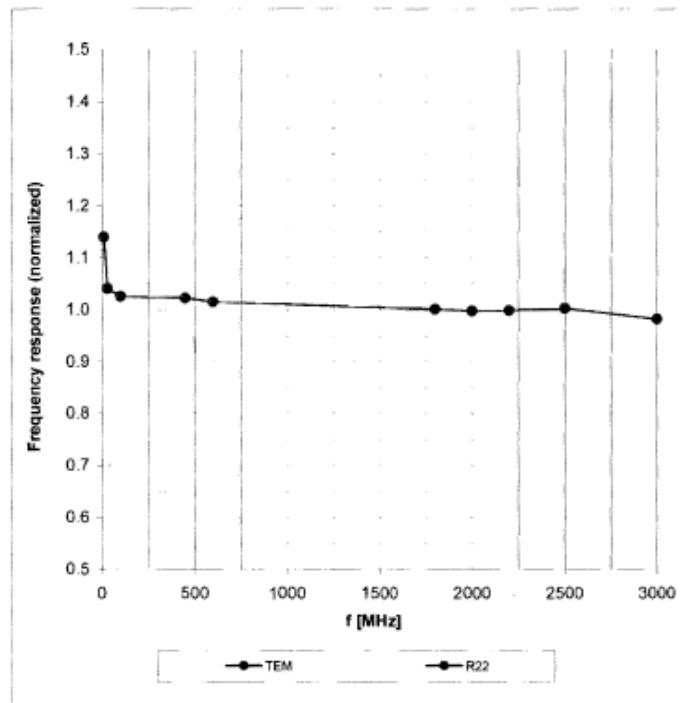


**Uncertainty of Frequency Response of E-field:  $\pm 6.3\%$  ( $k=2$ )**

Author Data <b>Andrew Becker</b>	Dates of Test <b>Feb 7 – May 25, July 18, 2011</b>	Test Report No <b>RTS-3933-1105-11A</b> <b>RTS-2580-1106-03 Rev1</b>	FCC ID: <b>L6ARDU70CW</b> <b>L6ARDE70UW</b>	IC ID <b>2503A-RDU70CW</b> <b>2503A-RDE70UW</b>
-------------------------------------	---	--	---	---

**EX3DV4 SN:3548****January 20, 2011**

### Receiving Pattern ( $\phi$ ), $\theta = 0^\circ$

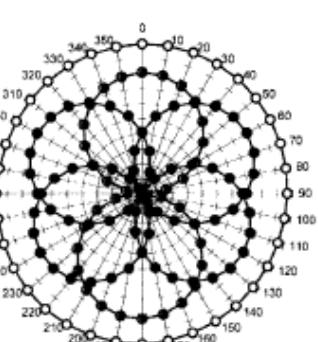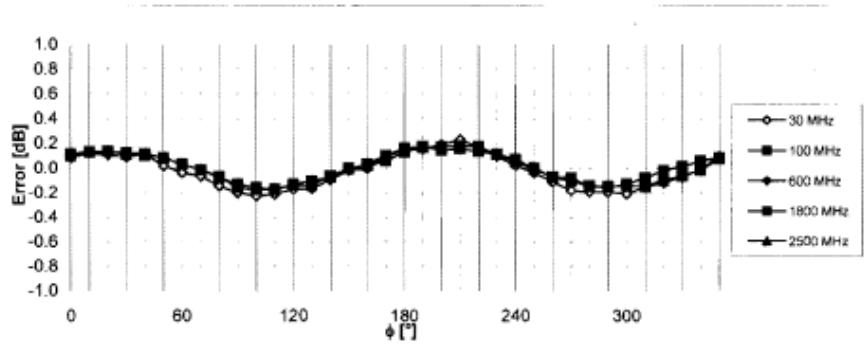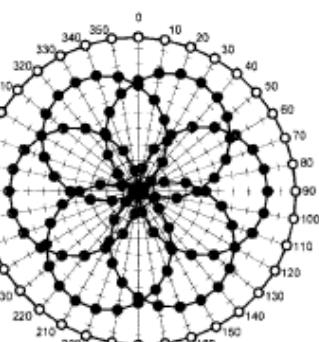**f = 600 MHz, TEM ifi110EXX****f = 1800 MHz, WG R22**
**Uncertainty of Axial Isotropy Assessment:  $\pm 0.5\%$  ( $k=2$ )**



Author Data <b>Andrew Becker</b>	Dates of Test <b>Feb 7 – May 25, July 18, 2011</b>	Test Report No <b>RTS-3933-1105-11A</b> <b>RTS-2580-1106-03 Rev1</b>	FCC ID: <b>L6ARDU70CW</b> <b>L6ARDE70UW</b>	IC ID <b>2503A-RDU70CW</b> <b>2503A-RDE70UW</b>
-------------------------------------	---	--	---	---

EX3DV4 SN:3548

January 20, 2011

### Dynamic Range f(SAR<sub>head</sub>)

(TEM cell, f = 900 MHz)

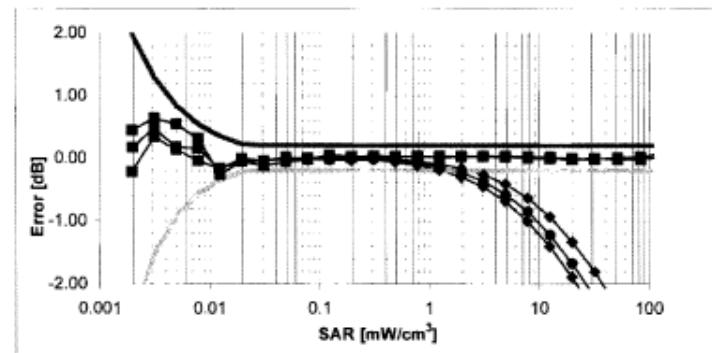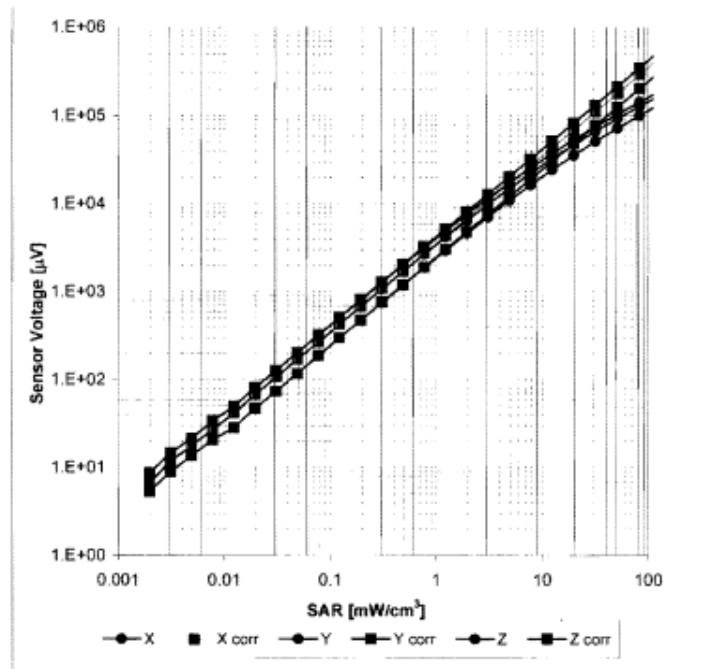
Uncertainty of Linearity Assessment:  $\pm 0.6\%$  (k=2)

Author Data <b>Andrew Becker</b>	Dates of Test <b>Feb 7 – May 25, July 18, 2011</b>	Test Report No <b>RTS-3933-1105-11A</b> <b>RTS-2580-1106-03 Rev1</b>	FCC ID: <b>L6ARDU70CW</b> <b>L6ARDE70UW</b>	IC ID <b>2503A-RDU70CW</b> <b>2503A-RDE70UW</b>
-------------------------------------	---	--	---	---


EX3DV4 SN:3548

January 20, 2011

## Conversion Factor Assessment

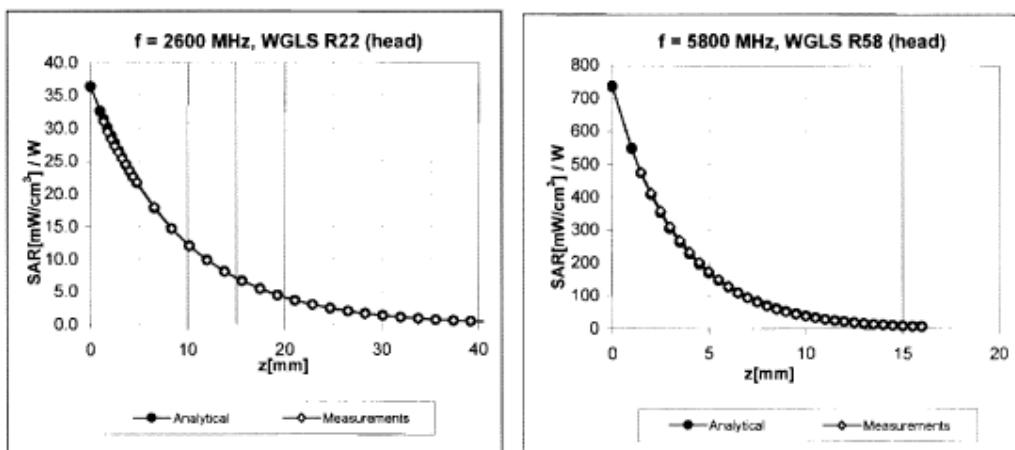

## Deviation from Isotropy in HSL

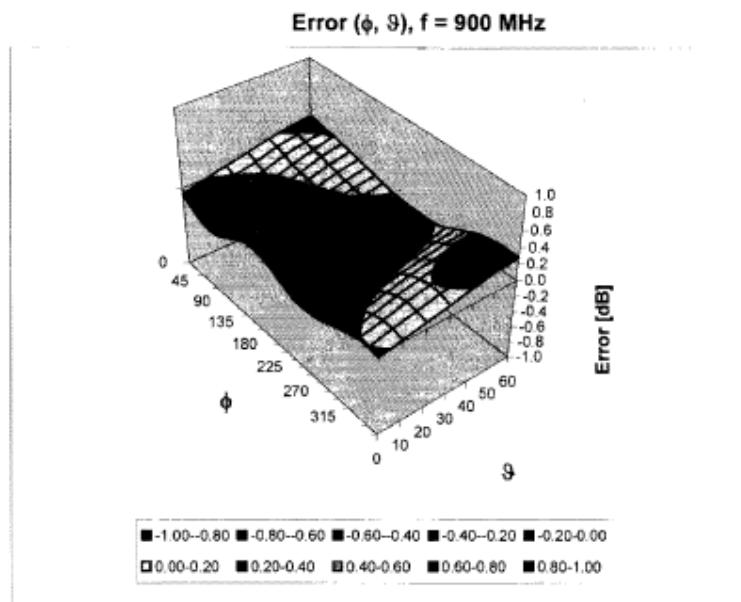

Uncertainty of Spherical Isotropy Assessment:  $\pm 2.6\%$  ( $k=2$ )



Document

**Appendix D for the BlackBerry® Smartphone Model  
RDU71CW/RDE71UW SAR Report Rev1**Page  
**45(74)**

Author Data <b>Andrew Becker</b>	Dates of Test <b>Feb 7 – May 25, July 18, 2011</b>	Test Report No <b>RTS-3933-1105-11A RTS-2580-1106-03 Rev1</b>	FCC ID: <b>L6ARDU70CW L6ARDE70UW</b>	IC ID <b>2503A-RDU70CW 2503A-RDE70UW</b>
-------------------------------------	---	--	---	---

**EX3DV4 SN:3548****January 20, 2011****Other Probe Parameters**

Sensor Arrangement	Triangular
Connector Angle (°)	Not applicable
Mechanical Surface Detection Mode	enabled
Optical Surface Detection Mode	disabled
Probe Overall Length	337 mm
Probe Body Diameter	10 mm
Tip Length	9 mm
Tip Diameter	2.5 mm
Probe Tip to Sensor X Calibration Point	1 mm
Probe Tip to Sensor Y Calibration Point	1 mm
Probe Tip to Sensor Z Calibration Point	1 mm
Recommended Measurement Distance from Surface	2 mm

	Document <b>Appendix D for the BlackBerry® Smartphone Model RDU71CW/RDE71UW SAR Report Rev1</b>	Page <b>46(74)</b>
Author Data <b>Andrew Becker</b>	Dates of Test <b>Feb 7 – May 25, July 18, 2011</b>	Test Report No <b>RTS-3933-1105-11A RTS-2580-1106-03 Rev1</b> FCC ID: <b>L6ARDU70CW L6ARDE70UW</b> IC ID <b>2503A-RDU70CW 2503A-RDE70UW</b>

**Calibration Laboratory of**  
Schmid & Partner  
Engineering AG  
Zeughausstrasse 43, 8004 Zurich, Switzerland



**S** Schweizerischer Kalibrierdienst  
**C** Service suisse d'étalonnage  
**S** Servizio svizzero di taratura  
**S** Swiss Calibration Service

Accredited by the Swiss Accreditation Service (SAS)  
The Swiss Accreditation Service is one of the signatories to the EA  
Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: **SCS 108**

Client **RTS (RIM Testing Services)**

Certificate No: **D835V2-446\_Jan11**

## **CALIBRATION CERTIFICATE**

Object **D835V2 - SN: 446**

Calibration procedure(s) **QA CAL-05.v8**  
**Calibration procedure for dipole validation kits**

Calibration date: **January 21, 2011**

This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI). The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility: environment temperature (22 ± 3)°C and humidity < 70%.

Calibration Equipment used (M&TE critical for calibration)

Primary Standards	ID #	Cal Date (Certificate No.)	Scheduled Calibration
Power meter EPM-442A	GB37480704	06-Oct-10 (No. 217-01266)	Oct-11
Power sensor HP 8481A	US37292783	06-Oct-10 (No. 217-01266)	Oct-11
Reference 20 dB Attenuator	SN: 5086 (20g)	30-Mar-10 (No. 217-01158)	Mar-11
Type-N mismatch combination	SN: 5047.2 / 06327	30-Mar-10 (No. 217-01162)	Mar-11
Reference Probe ES3DV3	SN: 3205	30-Apr-10 (No. ES3-3205_Apr10)	Apr-11
DAE4	SN: 601	10-Jun-10 (No. DAE4-601_Jun10)	Jun-11
Secondary Standards	ID #	Check Date (in house)	Scheduled Check
Power sensor HP 8481A	MY41092317	18-Oct-02 (in house check Oct-09)	In house check: Oct-11
RF generator R&S SMT-06	100005	4-Aug-99 (in house check Oct-09)	In house check: Oct-11
Network Analyzer HP 8753E	US37390585 S4206	18-Oct-01 (in house check Oct-10)	In house check: Oct-11

Calibrated by: Name **Dimce Iliev** Function **Laboratory Technician** Signature

Approved by: Name **Katja Pokovic** Function **Technical Manager** Signature

Issued: January 21, 2011

This calibration certificate shall not be reproduced except in full without written approval of the laboratory.

Certificate No: **D835V2-446\_Jan11**

Page 1 of 6

 <p>Document  <b>Appendix D for the BlackBerry® Smartphone Model  RDU71CW/RDE71UW SAR Report Rev1</b></p>				Page <b>47(74)</b>
Author Data <b>Andrew Becker</b>	Dates of Test <b>Feb 7 – May 25, July 18, 2011</b>	Test Report No <b>RTS-3933-1105-11A  RTS-2580-1106-03 Rev1</b>	FCC ID: <b>L6ARDU70CW  L6ARDE70UW</b>	IC ID <b>2503A-RDU70CW  2503A-RDE70UW</b>

**Calibration Laboratory of**  
**Schmid & Partner**  
**Engineering AG**  
**Zeughausstrasse 43, 8004 Zurich, Switzerland**



**S** Schweizerischer Kalibrierdienst  
**C** Service suisse d'étalementage  
**S** Servizio svizzero di taratura  
**S** Swiss Calibration Service

Accredited by the Swiss Accreditation Service (SAS)  
The Swiss Accreditation Service is one of the signatories to the EA  
Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: **SCS 108**

#### **Glossary:**

<b>TSL</b>	tissue simulating liquid
<b>ConvF</b>	sensitivity in TSL / NORM x,y,z
<b>N/A</b>	not applicable or not measured

#### **Calibration is Performed According to the Following Standards:**

- IEEE Std 1528-2003, "IEEE Recommended Practice for Determining the Peak Spatial-Averaged Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques", December 2003
- IEC 62209-1, "Procedure to measure the Specific Absorption Rate (SAR) for hand-held devices used in close proximity to the ear (frequency range of 300 MHz to 3 GHz)", February 2005
- Federal Communications Commission Office of Engineering & Technology (FCC OET), "Evaluating Compliance with FCC Guidelines for Human Exposure to Radiofrequency Electromagnetic Fields; Additional Information for Evaluating Compliance of Mobile and Portable Devices with FCC Limits for Human Exposure to Radiofrequency Emissions", Supplement C (Edition 01-01) to Bulletin 65

#### **Additional Documentation:**

- DASY4/5 System Handbook

#### **Methods Applied and Interpretation of Parameters:**

- Measurement Conditions:** Further details are available from the Validation Report at the end of the certificate. All figures stated in the certificate are valid at the frequency indicated.
- Antenna Parameters with TSL:** The dipole is mounted with the spacer to position its feed point exactly below the center marking of the flat phantom section, with the arms oriented parallel to the body axis.
- Feed Point Impedance and Return Loss:** These parameters are measured with the dipole positioned under the liquid filled phantom. The impedance stated is transformed from the measurement at the SMA connector to the feed point. The Return Loss ensures low reflected power. No uncertainty required.
- Electrical Delay:** One-way delay between the SMA connector and the antenna feed point. No uncertainty required.
- SAR measured:** SAR measured at the stated antenna input power.
- SAR normalized:** SAR as measured, normalized to an input power of 1 W at the antenna connector.
- SAR for nominal TSL parameters:** The measured TSL parameters are used to calculate the nominal SAR result.

	Document <b>Appendix D for the BlackBerry® Smartphone Model RDU71CW/RDE71UW SAR Report Rev1</b>	Page <b>48(74)</b>
Author Data <b>Andrew Becker</b>	Dates of Test <b>Feb 7 – May 25, July 18, 2011</b>	Test Report No <b>RTS-3933-1105-11A RTS-2580-1106-03 Rev1</b> FCC ID: <b>L6ARDU70CW L6ARDE70UW</b> IC ID <b>2503A-RDU70CW 2503A-RDE70UW</b>

### Measurement Conditions

DASY system configuration, as far as not given on page 1.

<b>DASY Version</b>	<b>DASY5</b>	<b>V52.6</b>
<b>Extrapolation</b>	<b>Advanced Extrapolation</b>	
<b>Phantom</b>	<b>Modular Flat Phantom V4.9</b>	
<b>Distance Dipole Center - TSL</b>	<b>15 mm</b>	<b>with Spacer</b>
<b>Zoom Scan Resolution</b>	<b>dx, dy, dz = 5 mm</b>	
<b>Frequency</b>	<b>835 MHz ± 1 MHz</b>	

### Head TSL parameters

The following parameters and calculations were applied.

	<b>Temperature</b>	<b>Permittivity</b>	<b>Conductivity</b>
<b>Nominal Head TSL parameters</b>	<b>22.0 °C</b>	<b>41.5</b>	<b>0.90 mho/m</b>
<b>Measured Head TSL parameters</b>	<b>(22.0 ± 0.2) °C</b>	<b>41.3 ± 6 %</b>	<b>0.89 mho/m ± 6 %</b>
<b>Head TSL temperature during test</b>	<b>(21.8 ± 0.2) °C</b>	<b>---</b>	<b>---</b>

### SAR result with Head TSL

<b>SAR averaged over 1 cm<sup>3</sup> (1 g) of Head TSL</b>	<b>Condition</b>	
SAR measured	250 mW input power	2.39 mW / g
SAR normalized	normalized to 1W	9.56 mW / g
SAR for nominal Head TSL parameters	normalized to 1W	<b>9.63 mW /g ± 17.0 % (k=2)</b>

<b>SAR averaged over 10 cm<sup>3</sup> (10 g) of Head TSL</b>	<b>Condition</b>	
SAR measured	250 mW input power	1.56 mW / g
SAR normalized	normalized to 1W	6.24 mW / g
SAR for nominal Head TSL parameters	normalized to 1W	<b>6.27 mW /g ± 16.5 % (k=2)</b>

	Document <b>Appendix D for the BlackBerry® Smartphone Model RDU71CW/RDE71UW SAR Report Rev1</b>	Page <b>49(74)</b>
Author Data <b>Andrew Becker</b>	Dates of Test <b>Feb 7 – May 25, July 18, 2011</b>	Test Report No <b>RTS-3933-1105-11A RTS-2580-1106-03 Rev1</b> FCC ID: <b>L6ARDU70CW L6ARDE70UW</b> IC ID <b>2503A-RDU70CW 2503A-RDE70UW</b>

## Appendix

### Antenna Parameters with Head TSL

Impedance, transformed to feed point	49.6 $\Omega$ - 7.7 $\mu\Omega$
Return Loss	- 22.2 dB

### General Antenna Parameters and Design

Electrical Delay (one direction)	1.386 ns
----------------------------------	----------

After long term use with 100W radiated power, only a slight warming of the dipole near the feedpoint can be measured.

The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals.

No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feedpoint may be damaged.

### Additional EUT Data

Manufactured by	SPEAG
Manufactured on	October 24, 2001

 <p>Document  <b>Appendix D for the BlackBerry® Smartphone Model  RDU71CW/RDE71UW SAR Report Rev1</b></p>				Page <b>50(74)</b>
Author Data <b>Andrew Becker</b>	Dates of Test <b>Feb 7 – May 25, July 18, 2011</b>	Test Report No <b>RTS-3933-1105-11A  RTS-2580-1106-03 Rev1</b>	FCC ID: <b>L6ARDU70CW  L6ARDE70UW</b>	IC ID <b>2503A-RDU70CW  2503A-RDE70UW</b>

## **DASY5 Validation Report for Head TSL**

Date/Time: 21.01.2011 10:18:05

Test Laboratory: SPEAG, Zurich, Switzerland

**DUT: Dipole 835 MHz; Type: D835V2; Serial: D835V2 - SN:446**

Communication System: CW; Frequency: 835 MHz; Duty Cycle: 1:1

Medium: HSL900

Medium parameters used:  $f = 835$  MHz;  $\sigma = 0.89$  mho/m;  $\epsilon_r = 41.2$ ;  $\rho = 1000$  kg/m<sup>3</sup>

Phantom section: Flat Section

Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2007)

DASY5 Configuration:

- Probe: ES3DV3 - SN3205; ConvF(6.03, 6.03, 6.03); Calibrated: 30.04.2010
- Sensor-Surface: 3mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn601; Calibrated: 10.06.2010
- Phantom: Flat Phantom 4.9L; Type: QD000P49AA; Serial: 1001
- Measurement SW: DASY52, V52.6.1 Build (408)
- Postprocessing SW: SEMCAD X, V14.4.2 Build (2595)


**Pin=250 mW /d=15mm, dist=3.0mm (ES-Probe)/Zoom Scan (7x7x7) /Cube 0:** Measurement grid: dx=5mm, dy=5mm, dz=5mm

Reference Value = 57.426 V/m; Power Drift = 0.04 dB

Peak SAR (extrapolated) = 3.600 W/kg


**SAR(1 g) = 2.39 mW/g; SAR(10 g) = 1.56 mW/g**

Maximum value of SAR (measured) = 2.790 mW/g

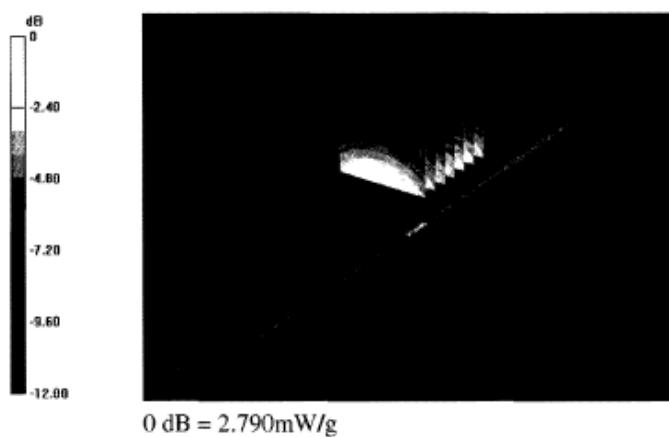

	Document <b>Appendix D for the BlackBerry® Smartphone Model RDU71CW/RDE71UW SAR Report Rev1</b>	Page <b>51(74)</b>
Author Data <b>Andrew Becker</b>	Dates of Test <b>Feb 7 – May 25, July 18, 2011</b>	Test Report No <b>RTS-3933-1105-11A RTS-2580-1106-03 Rev1</b> FCC ID: <b>L6ARDU70CW L6ARDE70UW</b> IC ID <b>2503A-RDU70CW 2503A-RDE70UW</b>

### Impedance Measurement Plot for Head TSL

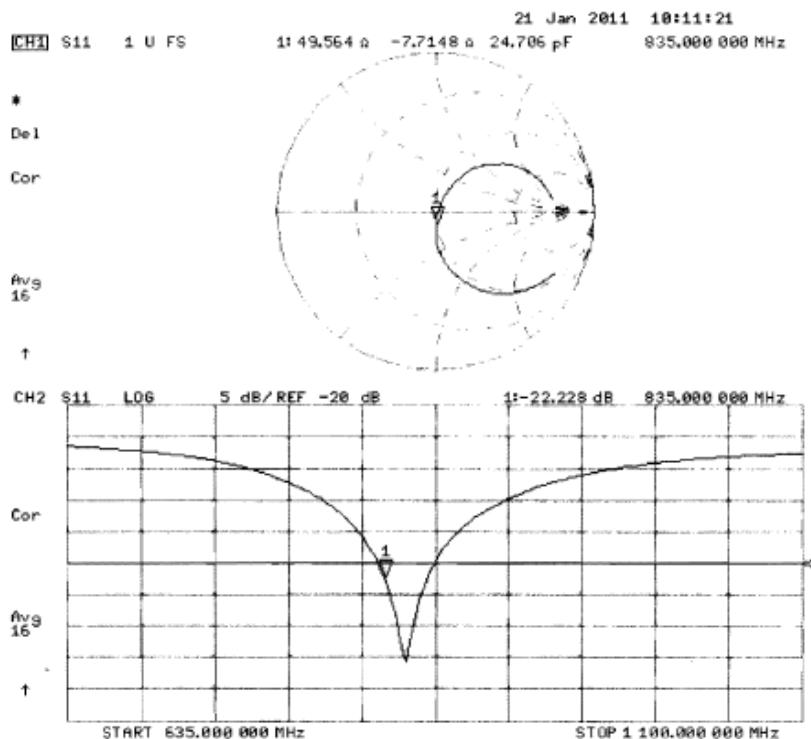



Author Data <b>Andrew Becker</b>	Dates of Test <b>Feb 7 – May 25, July 18, 2011</b>	Test Report No <b>RTS-3933-1105-11A</b> <b>RTS-2580-1106-03 Rev1</b>	FCC ID: <b>L6ARDU70CW</b> <b>L6ARDE70UW</b>	IC ID <b>2503A-RDU70CW</b> <b>2503A-RDE70UW</b>
-------------------------------------	---	--	---	---

**Calibration Laboratory of**  
**Schmid & Partner**  
**Engineering AG**  
**Zeughausstrasse 43, 8004 Zurich, Switzerland**



**S** Schweizerischer Kalibrierdienst  
**C** Service suisse d'étalonnage  
**S** Servizio svizzero di taratura  
**S** Swiss Calibration Service

Accredited by the Swiss Accreditation Service (SAS)  
The Swiss Accreditation Service is one of the signatories to the EA  
Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: **SCS 108**

Client **RTS (RIM Testing Services)**

Certificate No: **D1900V2-545\_Jan11**

## **CALIBRATION CERTIFICATE**

Object **D1900V2 - SN: 545**

Calibration procedure(s) **QA.CAL-05.v8**  
**Calibration procedure for dipole validation kits**

Calibration date: **January 13, 2011**

This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI).  
The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility: environment temperature  $(22 \pm 3)^\circ\text{C}$  and humidity  $< 70\%$ .

Calibration Equipment used (M&TE critical for calibration)

Primary Standards	ID #	Cal Date (Certificate No.)	Scheduled Calibration
Power meter EPM-442A	GB37480704	06-Oct-10 (No. 217-01266)	Oct-11
Power sensor HP 8481A	US37292783	06-Oct-10 (No. 217-01266)	Oct-11
Reference 20 dB Attenuator	SN: 5086 (20g)	30-Mar-10 (No. 217-01158)	Mar-11
Type-N mismatch combination	SN: 5047.2 / 06327	30-Mar-10 (No. 217-01162)	Mar-11
Reference Probe ES3DV3	SN: 3205	30-Apr-10 (No. ES3-3205_Apr10)	Apr-11
DAE4	SN: 601	10-Jun-10 (No. DAE4-601_Jun10)	Jun-11
Secondary Standards	ID #	Check Date (in house)	Scheduled Check
Power sensor HP 8481A	MY41092317	18-Oct-02 (in house check Oct-09)	In house check: Oct-11
RF generator R&S SMT-06	100005	4-Aug-99 (in house check Oct-09)	In house check: Oct-11
Network Analyzer HP 8753E	US37390585 S4206	18-Oct-01 (in house check Oct-10)	In house check: Oct-11

Calibrated by: Name **Dmitri Klev** Function **Laboratory Technician** Signature

Approved by: Name **Katja Pokovic** Function **Technical Manager** Signature

Issued: January 14, 2011

This calibration certificate shall not be reproduced except in full without written approval of the laboratory.

	Document <b>Appendix D for the BlackBerry® Smartphone Model RDU71CW/RDE71UW SAR Report Rev1</b>	Page <b>53(74)</b>
Author Data <b>Andrew Becker</b>	Dates of Test <b>Feb 7 – May 25, July 18, 2011</b>	Test Report No <b>RTS-3933-1105-11A RTS-2580-1106-03 Rev1</b> FCC ID: <b>L6ARDU70CW L6ARDE70UW</b> IC ID <b>2503A-RDU70CW 2503A-RDE70UW</b>

**Calibration Laboratory of**  
Schmid & Partner  
Engineering AG  
Zeughausstrasse 43, 8004 Zurich, Switzerland



**S** Schweizerischer Kalibrierdienst  
**C** Service suisse d'étalonnage  
**S** Servizio svizzero di taratura  
**S** Swiss Calibration Service

Accredited by the Swiss Accreditation Service (SAS)  
The Swiss Accreditation Service is one of the signatories to the EA  
Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: **SCS 108**

#### **Glossary:**

<b>TSL</b>	tissue simulating liquid
<b>ConvF</b>	sensitivity in TSL / NORM x,y,z
<b>N/A</b>	not applicable or not measured

#### **Calibration is Performed According to the Following Standards:**

- IEEE Std 1528-2003, "IEEE Recommended Practice for Determining the Peak Spatial-Averaged Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques", December 2003
- IEC 62209-1, "Procedure to measure the Specific Absorption Rate (SAR) for hand-held devices used in close proximity to the ear (frequency range of 300 MHz to 3 GHz)", February 2005
- Federal Communications Commission Office of Engineering & Technology (FCC OET), "Evaluating Compliance with FCC Guidelines for Human Exposure to Radiofrequency Electromagnetic Fields; Additional Information for Evaluating Compliance of Mobile and Portable Devices with FCC Limits for Human Exposure to Radiofrequency Emissions", Supplement C (Edition 01-01) to Bulletin 65

#### **Additional Documentation:**

- DASY4/5 System Handbook

#### **Methods Applied and Interpretation of Parameters:**

- Measurement Conditions:** Further details are available from the Validation Report at the end of the certificate. All figures stated in the certificate are valid at the frequency indicated.
- Antenna Parameters with TSL:** The dipole is mounted with the spacer to position its feed point exactly below the center marking of the flat phantom section, with the arms oriented parallel to the body axis.
- Feed Point Impedance and Return Loss:** These parameters are measured with the dipole positioned under the liquid filled phantom. The impedance stated is transformed from the measurement at the SMA connector to the feed point. The Return Loss ensures low reflected power. No uncertainty required.
- Electrical Delay:** One-way delay between the SMA connector and the antenna feed point. No uncertainty required.
- SAR measured:** SAR measured at the stated antenna input power.
- SAR normalized:** SAR as measured, normalized to an input power of 1 W at the antenna connector.
- SAR for nominal TSL parameters:** The measured TSL parameters are used to calculate the nominal SAR result.



Author Data <b>Andrew Becker</b>	Dates of Test <b>Feb 7 – May 25, July 18, 2011</b>	Test Report No <b>RTS-3933-1105-11A RTS-2580-1106-03 Rev1</b>	FCC ID: <b>L6ARDU70CW L6ARDE70UW</b>	IC ID <b>2503A-RDU70CW 2503A-RDE70UW</b>
-------------------------------------	---	--	---	---

### Measurement Conditions

DASY system configuration, as far as not given on page 1.

<b>DASY Version</b>	<b>DASY5</b>	<b>V52.6</b>
<b>Extrapolation</b>	<b>Advanced Extrapolation</b>	
<b>Phantom</b>	<b>Modular Flat Phantom V5.0</b>	
<b>Distance Dipole Center - TSL</b>	<b>10 mm</b>	<b>with Spacer</b>
<b>Zoom Scan Resolution</b>	<b>dx, dy, dz = 5 mm</b>	
<b>Frequency</b>	<b>1900 MHz ± 1 MHz</b>	

### Head TSL parameters

The following parameters and calculations were applied.

	<b>Temperature</b>	<b>Permittivity</b>	<b>Conductivity</b>
<b>Nominal Head TSL parameters</b>	22.0 °C	40.0	1.40 mho/m
<b>Measured Head TSL parameters</b>	(22.0 ± 0.2) °C	38.5 ± 6 %	1.43 mho/m ± 6 %
<b>Head TSL temperature during test</b>	(21.2 ± 0.2) °C	----	----

### SAR result with Head TSL

<b>SAR averaged over 1 cm<sup>3</sup> (1 g) of Head TSL</b>	<b>Condition</b>	
SAR measured	250 mW input power	10.2 mW / g
SAR normalized	normalized to 1W	40.8 mW / g
SAR for nominal Head TSL parameters	normalized to 1W	<b>40.0 mW /g ± 17.0 % (k=2)</b>

<b>SAR averaged over 10 cm<sup>3</sup> (10 g) of Head TSL</b>	<b>Condition</b>	
SAR measured	250 mW input power	5.26 mW / g
SAR normalized	normalized to 1W	21.0 mW / g
SAR for nominal Head TSL parameters	normalized to 1W	<b>20.8 mW /g ± 16.5 % (k=2)</b>

	Document <b>Appendix D for the BlackBerry® Smartphone Model RDU71CW/RDE71UW SAR Report Rev1</b>	Page <b>55(74)</b>
Author Data <b>Andrew Becker</b>	Dates of Test <b>Feb 7 – May 25, July 18, 2011</b>	Test Report No <b>RTS-3933-1105-11A RTS-2580-1106-03 Rev1</b> FCC ID: <b>L6ARDU70CW L6ARDE70UW</b> IC ID <b>2503A-RDU70CW 2503A-RDE70UW</b>

## Appendix

### Antenna Parameters with Head TSL

Impedance, transformed to feed point	50.8 $\Omega$ + 1.8 $j\Omega$
Return Loss	- 34.4 dB

### General Antenna Parameters and Design

Electrical Delay (one direction)	1.199 ns
----------------------------------	----------

After long term use with 100W radiated power, only a slight warming of the dipole near the feedpoint can be measured.

The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals.

No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feedpoint may be damaged.

### Additional EUT Data

Manufactured by	SPEAG
Manufactured on	November 15, 2001

 Document	<b>Appendix D for the BlackBerry® Smartphone Model RDU71CW/RDE71UW SAR Report Rev1</b>			Page <b>56(74)</b>
Author Data <b>Andrew Becker</b>	Dates of Test <b>Feb 7 – May 25, July 18, 2011</b>	Test Report No <b>RTS-3933-1105-11A RTS-2580-1106-03 Rev1</b>	FCC ID: <b>L6ARDU70CW L6ARDE70UW</b>	IC ID <b>2503A-RDU70CW 2503A-RDE70UW</b>

### **DASY5 Validation Report for Head TSL**

Date/Time: 13.01.2011 14:52:49

Test Laboratory: SPEAG, Zurich, Switzerland

**DUT: Dipole 1900 MHz; Type: D1900V2; Serial: D1900V2 - SN:545**

Communication System: CW; Frequency: 1900 MHz; Duty Cycle: 1:1

Medium: HSL U12 BB

Medium parameters used:  $f = 1900$  MHz;  $\sigma = 1.43$  mho/m;  $\epsilon_r = 38.6$ ;  $\rho = 1000$  kg/m<sup>3</sup>

Phantom section: Flat Section

Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2007)

DASY5 Configuration:

- Probe: ES3DV3 - SN3205; ConvF(5.09, 5.09, 5.09); Calibrated: 30.04.2010
- Sensor-Surface: 3mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn601; Calibrated: 10.06.2010
- Phantom: Flat Phantom 5.0 (front); Type: QD000P50AA; Serial: 1001
- Measurement SW: DASY52, V52.6.1 Build (408)
- Postprocessing SW: SEMCAD X, V14.4.2 Build (2595)


**Pin=250 mW /d=10mm, dist=3.0mm (ES-Probe)/Zoom Scan (7x7x7) /Cube 0:** Measurement grid: dx=5mm, dy=5mm, dz=5mm

Reference Value = 98.053 V/m; Power Drift = 0.03 dB

Peak SAR (extrapolated) = 18.648 W/kg


**SAR(1 g) = 10.2 mW/g; SAR(10 g) = 5.26 mW/g**

Maximum value of SAR (measured) = 12.743 mW/g

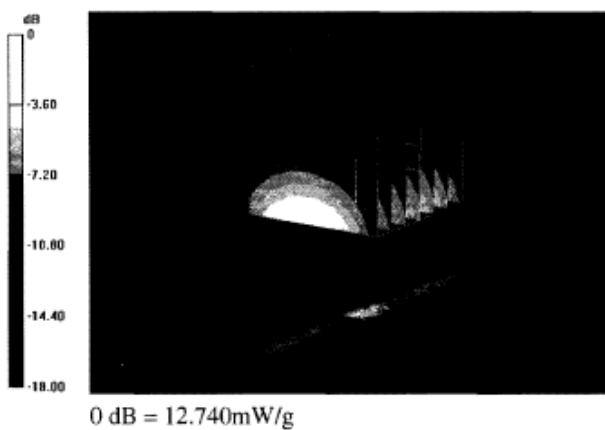

<b>RIM Testing Services</b>	Document <b>Appendix D for the BlackBerry® Smartphone Model RDU71CW/RDE71UW SAR Report Rev1</b>	Page <b>57(74)</b>
Author Data <b>Andrew Becker</b>	Dates of Test <b>Feb 7 – May 25, July 18, 2011</b>	Test Report No <b>RTS-3933-1105-11A RTS-2580-1106-03 Rev1</b> FCC ID: <b>L6ARDU70CW L6ARDE70UW</b> IC ID <b>2503A-RDU70CW 2503A-RDE70UW</b>

### Impedance Measurement Plot for Head TSL

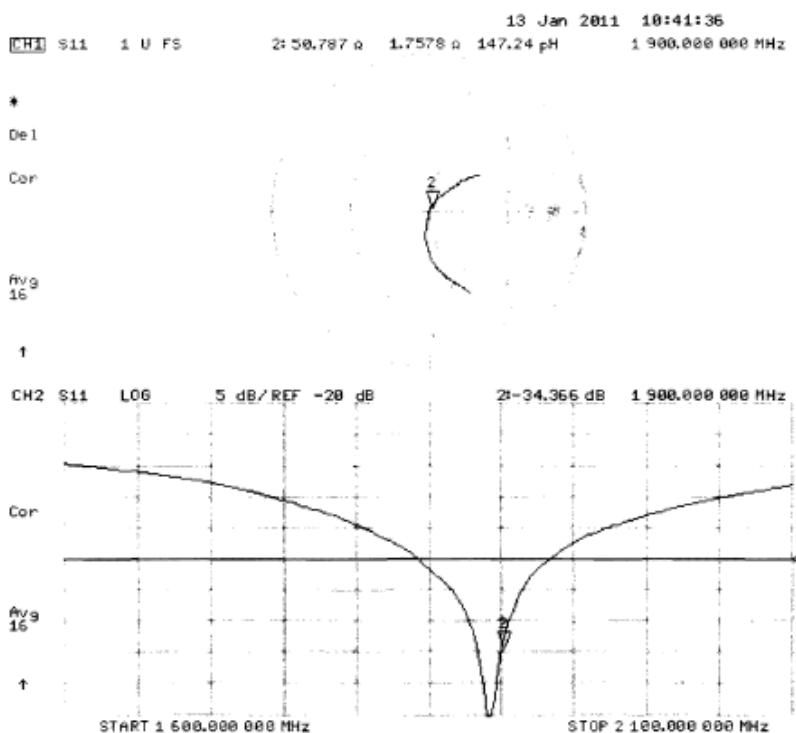

	Document <b>Appendix D for the BlackBerry® Smartphone Model RDU71CW/RDE71UW SAR Report Rev1</b>	Page <b>58(74)</b>
Author Data <b>Andrew Becker</b>	Dates of Test <b>Feb 7 – May 25, July 18, 2011</b>	Test Report No <b>RTS-3933-1105-11A RTS-2580-1106-03 Rev1</b> FCC ID: <b>L6ARDU70CW L6ARDE70UW</b> IC ID <b>2503A-RDU70CW 2503A-RDE70UW</b>

**Calibration Laboratory of**  
Schmid & Partner  
Engineering AG  
Zeughausstrasse 43, 8004 Zurich, Switzerland



**S** Schweizerischer Kalibrierdienst  
**C** Service suisse d'étalonnage  
**S** Servizio svizzero di taratura  
**S** Swiss Calibration Service

Accredited by the Swiss Accreditation Service (SAS)  
The Swiss Accreditation Service is one of the signatories to the EA  
Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: **SCS 108**

Client **RTS (RIM Testing Services)**

Certificate No: **D2450V2-747 Nov09**

## CALIBRATION CERTIFICATE

Object	<b>D2450V2 - SN: 747</b>		
Calibration procedure(s)	<b>QA CAL-05.v7</b> Calibration procedure for dipole validation kits		
Calibration date:	<b>November 11, 2009</b>		
<p>This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI). The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.</p> <p>All calibrations have been conducted in the closed laboratory facility: environment temperature <math>(22 \pm 3)^\circ\text{C}</math> and humidity <math>&lt; 70\%</math>.</p> <p>Calibration Equipment used (M&amp;TE critical for calibration)</p>			
Primary Standards	ID #	Cal Date (Certificate No.)	Scheduled Calibration
Power meter EPM-442A	GB37480704	06-Oct-09 (No. 217-01086)	Oct-10
Power sensor HP 8481A	US37292783	06-Oct-09 (No. 217-01086)	Oct-10
Reference 20 dB Attenuator	SN: 5086 (20g)	31-Mar-09 (No. 217-01025)	Mar-10
Type-N mismatch combination	SN: 5047.2 / 06327	31-Mar-09 (No. 217-01029)	Mar-10
Reference Probe ES3DV3	SN: 3205	26-Jun-09 (No. ES3-3205_Jun09)	Jun-10
DAE4	SN: 601	07-Mar-09 (No. DAE4-601_Mar09)	Mar-10
Secondary Standards	ID #	Check Date (in house)	Scheduled Check
Power sensor HP 8481A	MY41092317	18-Oct-02 (in house check Oct-09)	In house check: Oct-11
RF generator R&S SMT-06	100005	4-Aug-99 (in house check Oct-09)	In house check: Oct-11
Network Analyzer HP 8753E	US37390585 S4206	18-Oct-01 (in house check Oct-09)	In house check: Oct-10
Calibrated by:	Name <b>Mike Mell</b>	Function <b>Laboratory Technician</b>	Signature 
Approved by:	<b>Katja Pokovic</b>	<b>Technical Manager</b>	
Issued: November 16, 2009			
This calibration certificate shall not be reproduced except in full without written approval of the laboratory.			

 <p>Document  <b>Appendix D for the BlackBerry® Smartphone Model  RDU71CW/RDE71UW SAR Report Rev1</b></p>				Page <b>59(74)</b>
Author Data <b>Andrew Becker</b>	Dates of Test <b>Feb 7 – May 25, July 18, 2011</b>	Test Report No <b>RTS-3933-1105-11A  RTS-2580-1106-03 Rev1</b>	FCC ID: <b>L6ARDU70CW  L6ARDE70UW</b>	IC ID <b>2503A-RDU70CW  2503A-RDE70UW</b>

**Calibration Laboratory of**  
**Schmid & Partner**  
**Engineering AG**  
**Zeughausstrasse 43, 8004 Zurich, Switzerland**



**S** Schweizerischer Kalibrierdienst  
**C** Service suisse d'étalementage  
**S** Servizio svizzero di taratura  
**S** Swiss Calibration Service

Accredited by the Swiss Accreditation Service (SAS)  
The Swiss Accreditation Service is one of the signatories to the EA  
Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: **SCS 108**

#### **Glossary:**

<b>TSL</b>	tissue simulating liquid
<b>ConvF</b>	sensitivity in TSL / NORM x,y,z
<b>N/A</b>	not applicable or not measured

#### **Calibration is Performed According to the Following Standards:**

- IEEE Std 1528-2003, "IEEE Recommended Practice for Determining the Peak Spatial-Averaged Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques", December 2003
- IEC 62209-1, "Procedure to measure the Specific Absorption Rate (SAR) for hand-held devices used in close proximity to the ear (frequency range of 300 MHz to 3 GHz)", February 2005
- Federal Communications Commission Office of Engineering & Technology (FCC OET), "Evaluating Compliance with FCC Guidelines for Human Exposure to Radiofrequency Electromagnetic Fields; Additional Information for Evaluating Compliance of Mobile and Portable Devices with FCC Limits for Human Exposure to Radiofrequency Emissions", Supplement C (Edition 01-01) to Bulletin 65

#### **Additional Documentation:**

- DASY4/5 System Handbook

#### **Methods Applied and Interpretation of Parameters:**

- Measurement Conditions:** Further details are available from the Validation Report at the end of the certificate. All figures stated in the certificate are valid at the frequency indicated.
- Antenna Parameters with TSL:** The dipole is mounted with the spacer to position its feed point exactly below the center marking of the flat phantom section, with the arms oriented parallel to the body axis.
- Feed Point Impedance and Return Loss:** These parameters are measured with the dipole positioned under the liquid filled phantom. The impedance stated is transformed from the measurement at the SMA connector to the feed point. The Return Loss ensures low reflected power. No uncertainty required.
- Electrical Delay:** One-way delay between the SMA connector and the antenna feed point. No uncertainty required.
- SAR measured:** SAR measured at the stated antenna input power.
- SAR normalized:** SAR as measured, normalized to an input power of 1 W at the antenna connector.
- SAR for nominal TSL parameters:** The measured TSL parameters are used to calculate the nominal SAR result.



Document

**Appendix D for the BlackBerry® Smartphone Model  
RDU71CW/RDE71UW SAR Report Rev1**Page  
**60(74)**

Author Data <b>Andrew Becker</b>	Dates of Test <b>Feb 7 – May 25, July 18, 2011</b>	Test Report No <b>RTS-3933-1105-11A</b> <b>RTS-2580-1106-03 Rev1</b>	FCC ID: <b>L6ARDU70CW</b> <b>L6ARDE70UW</b>	IC ID <b>2503A-RDU70CW</b> <b>2503A-RDE70UW</b>
-------------------------------------	---	--	---	---

**Measurement Conditions**

DASY system configuration, as far as not given on page 1.

<b>DASY Version</b>	DASY5	V5.2
<b>Extrapolation</b>	Advanced Extrapolation	
<b>Phantom</b>	Modular Flat Phantom V4.9	
<b>Distance Dipole Center - TSL</b>	10 mm	with Spacer
<b>Zoom Scan Resolution</b>	dx, dy, dz = 5 mm	
<b>Frequency</b>	2450 MHz ± 1 MHz	

**Head TSL parameters**

The following parameters and calculations were applied.

	<b>Temperature</b>	<b>Permittivity</b>	<b>Conductivity</b>
<b>Nominal Head TSL parameters</b>	22.0 °C	39.2	1.80 mho/m
<b>Measured Head TSL parameters</b>	(22.0 ± 0.2) °C	39.1 ± 6 %	1.78 mho/m ± 6 %
<b>Head TSL temperature during test</b>	(21.3 ± 0.2) °C	---	---

**SAR result with Head TSL**

<b>SAR averaged over 1 cm<sup>3</sup> (1 g) of Head TSL</b>	<b>Condition</b>	
SAR measured	250 mW input power	13.3 mW / g
SAR normalized	normalized to 1W	53.2 mW / g
SAR for nominal Head TSL parameters	normalized to 1W	<b>53.4 mW /g ± 17.0 % (k=2)</b>

<b>SAR averaged over 10 cm<sup>3</sup> (10 g) of Head TSL</b>	<b>Condition</b>	
SAR measured	250 mW input power	6.23 mW / g
SAR normalized	normalized to 1W	24.9 mW / g
SAR for nominal Head TSL parameters	normalized to 1W	<b>24.9 mW /g ± 16.5 % (k=2)</b>

	Document <b>Appendix D for the BlackBerry® Smartphone Model RDU71CW/RDE71UW SAR Report Rev1</b>	Page <b>61(74)</b>
Author Data <b>Andrew Becker</b>	Dates of Test <b>Feb 7 – May 25, July 18, 2011</b>	Test Report No <b>RTS-3933-1105-11A RTS-2580-1106-03 Rev1</b> FCC ID: <b>L6ARDU70CW L6ARDE70UW</b> IC ID <b>2503A-RDU70CW 2503A-RDE70UW</b>

## Appendix

### Antenna Parameters with Head TSL

Impedance, transformed to feed point	51.9 $\Omega$ + 0.9 $\mu\Omega$
Return Loss	- 33.9 dB

### General Antenna Parameters and Design

Electrical Delay (one direction)	1.161 ns
----------------------------------	----------

After long term use with 100W radiated power, only a slight warming of the dipole near the feedpoint can be measured.

The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals.

No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feedpoint may be damaged.

### Additional EUT Data

Manufactured by	SPEAG
Manufactured on	December 01, 2003

 <p>Document  <b>Appendix D for the BlackBerry® Smartphone Model  RDU71CW/RDE71UW SAR Report Rev1</b></p>				Page <b>62(74)</b>
Author Data <b>Andrew Becker</b>	Dates of Test <b>Feb 7 – May 25, July 18, 2011</b>	Test Report No <b>RTS-3933-1105-11A  RTS-2580-1106-03 Rev1</b>	FCC ID: <b>L6ARDU70CW  L6ARDE70UW</b>	IC ID <b>2503A-RDU70CW  2503A-RDE70UW</b>

### **DASY5 Validation Report for Head TSL**

Date/Time: 11.11.2009 15:04:10

Test Laboratory: SPEAG, Zurich, Switzerland

**DUT: Dipole 2450 MHz; Type: D2450V2; Serial: D2450V2 - SN:747**

Communication System: CW; Frequency: 2450 MHz; Duty Cycle: 1:1

Medium: HSL U11 BB

Medium parameters used:  $f = 2450$  MHz;  $\sigma = 1.79$  mho/m;  $\epsilon_r = 39.2$ ;  $\rho = 1000$  kg/m<sup>3</sup>

Phantom section: Flat Section

Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2007)

DASY5 Configuration:

- Probe: ES3DV3 - SN3205; ConvF(4.53, 4.53, 4.53); Calibrated: 26.06.2009
- Sensor-Surface: 3mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn601; Calibrated: 07.03.2009
- Phantom: Flat Phantom 5.0 (front); Type: QD000P50AA; Serial: 1001
- Measurement SW: DASY5, V5.2 Build 157; SEMCAD X Version 14.0 Build 57

### **Head/d=10mm, Pin=250 mW, dist=3.0mm (ES-Probe)/Zoom Scan (7x7x7) (7x7x7)/Cube 0:**


Measurement grid: dx=5mm, dy=5mm, dz=5mm

Reference Value = 101.3 V/m; Power Drift = 0.067 dB

Peak SAR (extrapolated) = 27 W/kg

**SAR(1 g) = 13.3 mW/g; SAR(10 g) = 6.23 mW/g**

Maximum value of SAR (measured) = 17.1 mW/g

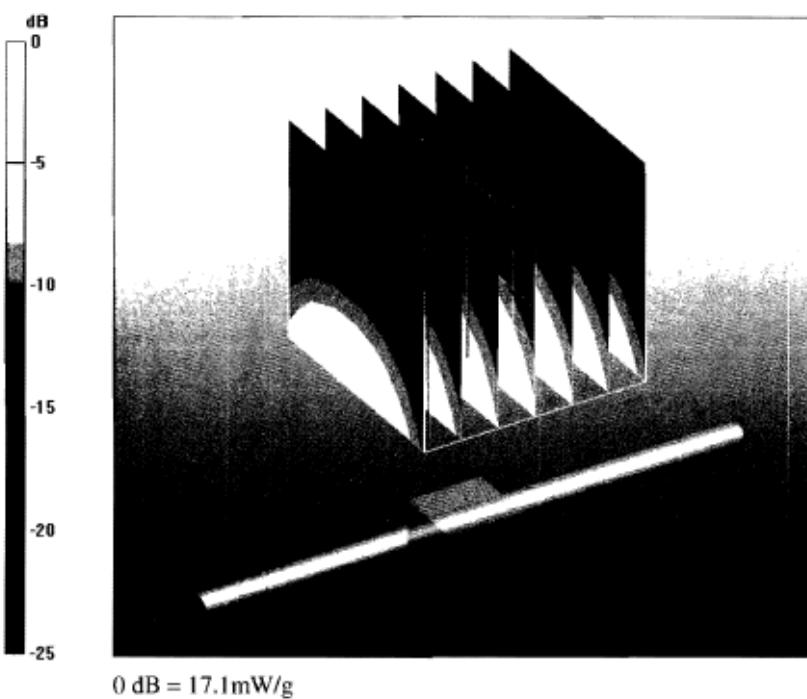




Document

**Appendix D for the BlackBerry® Smartphone Model  
RDU71CW/RDE71UW SAR Report Rev1**Page  
**63(74)**

Author Data <b>Andrew Becker</b>	Dates of Test <b>Feb 7 – May 25, July 18, 2011</b>	Test Report No <b>RTS-3933-1105-11A</b> <b>RTS-2580-1106-03 Rev1</b>	FCC ID: <b>L6ARDU70CW</b> <b>L6ARDE70UW</b>	IC ID <b>2503A-RDU70CW</b> <b>2503A-RDE70UW</b>
-------------------------------------	---	--	---	---

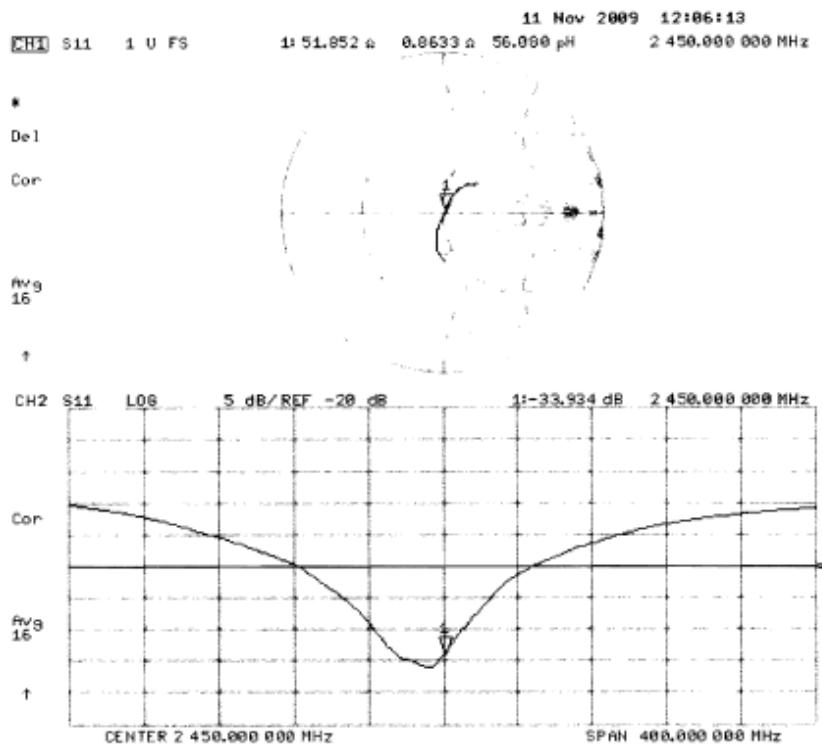**Impedance Measurement Plot for Head TSL**

	Document <b>Appendix D for the BlackBerry® Smartphone Model RDU71CW/RDE71UW SAR Report Rev1</b>	Page <b>64(74)</b>
Author Data <b>Andrew Becker</b>	Dates of Test <b>Feb 7 – May 25, July 18, 2011</b>	Test Report No <b>RTS-3933-1105-11A RTS-2580-1106-03 Rev1</b> FCC ID: <b>L6ARDU70CW L6ARDE70UW</b> IC ID <b>2503A-RDU70CW 2503A-RDE70UW</b>

**Calibration Laboratory of**  
Schmid & Partner  
Engineering AG  
Zeughausstrasse 43, 8004 Zurich, Switzerland



**S** Schweizerischer Kalibrierdienst  
**C** Service suisse d'étalonnage  
**S** Servizio svizzero di taratura  
**S** Swiss Calibration Service

Accredited by the Swiss Accreditation Service (SAS)  
The Swiss Accreditation Service is one of the signatories to the EA  
Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: **SCS 108**

Client **RTS (RIM Testing Services)**

Certificate No: **D5GHzV2-1033\_Nov09**

## CALIBRATION CERTIFICATE

Object	D5GHzV2 - SN: 1033
Calibration procedure(s)	QA CAL-22.v1 Calibration procedure for dipole validation kits between 3-6 GHz
Calibration date:	November 13, 2009

This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI). The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility: environment temperature  $(22 \pm 3)^\circ\text{C}$  and humidity  $< 70\%$ .

Calibration Equipment used (M&TE critical for calibration)

Primary Standards	ID #	Cal Date (Certificate No.)	Scheduled Calibration
Power meter EPM-442A	GB37480704	06-Oct-09 (No. 217-01086)	Oct-10
Power sensor HP 8481A	US37292783	06-Oct-09 (No. 217-01086)	Oct-10
Reference 20 dB Attenuator	SN: 5086 (20g)	31-Mar-09 (No. 217-01025)	Mar-10
Type-N mismatch combination	SN: 5047.2 / 06327	31-Mar-09 (No. 217-01029)	Mar-10
Reference Probe EX3DV4	SN: 3503	11-Mar-09 (No. EX3-3503_Mar09)	Mar-10
DAE4	SN: 601	07-Mar-09 (No. DAE4-601_Mar09)	Mar-10
Secondary Standards	ID #	Check Date (in house)	Scheduled Check
Power sensor HP 8481A	MY41092317	18-Oct-02 (in house check Oct-09)	In house check: Oct-11
RF generator R&S SMT-06	100005	4-Aug-99 (in house check Oct-09)	In house check: Oct-11
Network Analyzer HP 8753E	US37390585 S4206	18-Oct-01 (in house check Oct-09)	In house check: Oct-10

Calibrated by:	Name Jeton Kastrati	Function Laboratory Technician	Signature 
Approved by:	Katja Pokovic	Technical Manager	

Issued: November 16, 2009

This calibration certificate shall not be reproduced except in full without written approval of the laboratory.

	Document <b>Appendix D for the BlackBerry® Smartphone Model RDU71CW/RDE71UW SAR Report Rev1</b>	Page <b>65(74)</b>
Author Data <b>Andrew Becker</b>	Dates of Test <b>Feb 7 – May 25, July 18, 2011</b>	Test Report No <b>RTS-3933-1105-11A RTS-2580-1106-03 Rev1</b> FCC ID: <b>L6ARDU70CW L6ARDE70UW</b> IC ID <b>2503A-RDU70CW 2503A-RDE70UW</b>

**Calibration Laboratory of**  
Schmid & Partner  
Engineering AG  
Zeughausstrasse 43, 8004 Zurich, Switzerland



**S** Schweizerischer Kalibrierdienst  
**C** Service suisse d'étalonnage  
**S** Servizio svizzero di taratura  
**S** Swiss Calibration Service

Accredited by the Swiss Accreditation Service (SAS)  
The Swiss Accreditation Service is one of the signatories to the EA  
Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: **SCS 108**

#### **Glossary:**

<b>TSL</b>	tissue simulating liquid
<b>ConvF</b>	sensitivity in TSL / NORM x,y,z
<b>N/A</b>	not applicable or not measured

#### **Calibration is Performed According to the Following Standards:**

- IEC Std 62209 Part 2, "Evaluation of Human Exposure to Radio Frequency Fields from Handheld and Body-Mounted Wireless Communication Devices in the Frequency Range of 30 MHz to 6 GHz: Human models, Instrumentation, and Procedures"; Part 2: "Procedure to determine the Specific Absorption Rate (SAR) for including accessories and multiple transmitters", Draft Version 0.9, December 2004
- Federal Communications Commission Office of Engineering & Technology (FCC OET), "Evaluating Compliance with FCC Guidelines for Human Exposure to Radiofrequency Electromagnetic Fields; Additional Information for Evaluating Compliance of Mobile and Portable Devices with FCC Limits for Human Exposure to Radiofrequency Emissions", Supplement C (Edition 01-01) to Bulletin 65

#### **Additional Documentation:**

- DASY4/5 System Handbook

#### **Methods Applied and Interpretation of Parameters:**

- Measurement Conditions:** Further details are available from the Validation Report at the end of the certificate. All figures stated in the certificate are valid at the frequency indicated.
- Antenna Parameters with TSL:** The dipole is mounted with the spacer to position its feed point exactly below the center marking of the flat phantom section, with the arms oriented parallel to the body axis.
- Feed Point Impedance and Return Loss:** These parameters are measured with the dipole positioned under the liquid filled phantom. The impedance stated is transformed from the measurement at the SMA connector to the feed point. The Return Loss ensures low reflected power. No uncertainty required.
- Electrical Delay:** One-way delay between the SMA connector and the antenna feed point. No uncertainty required.
- SAR measured:** SAR measured at the stated antenna input power.
- SAR normalized:** SAR as measured, normalized to an input power of 1 W at the antenna connector.
- SAR for nominal TSL parameters:** The measured TSL parameters are used to calculate the nominal SAR result.

	Document <b>Appendix D for the BlackBerry® Smartphone Model RDU71CW/RDE71UW SAR Report Rev1</b>	Page <b>66(74)</b>
Author Data <b>Andrew Becker</b>	Dates of Test <b>Feb 7 – May 25, July 18, 2011</b>	Test Report No <b>RTS-3933-1105-11A RTS-2580-1106-03 Rev1</b> FCC ID: <b>L6ARDU70CW L6ARDE70UW</b> IC ID <b>2503A-RDU70CW 2503A-RDE70UW</b>

### Measurement Conditions

DASY system configuration, as far as not given on page 1.

<b>DASY Version</b>	DASY5	V5.2
<b>Extrapolation</b>	Advanced Extrapolation	
<b>Phantom</b>	Modular Flat Phantom V5.0	
<b>Distance Dipole Center - TSL</b>	10 mm	with Spacer
<b>Area Scan resolution</b>	dx, dy = 10 mm	
<b>Zoom Scan Resolution</b>	dx, dy = 4.0 mm, dz = 2.5 mm	
<b>Frequency</b>	5200 MHz ± 1 MHz 5500 MHz ± 1 MHz 5800 MHz ± 1 MHz	

### Head TSL parameters at 5200 MHz

The following parameters and calculations were applied.

	<b>Temperature</b>	<b>Permittivity</b>	<b>Conductivity</b>
<b>Nominal Head TSL parameters</b>	22.0 °C	36.0	4.66 mho/m
<b>Measured Head TSL parameters</b>	(22.0 ± 0.2) °C	35.4 ± 6 %	4.54 mho/m ± 6 %
<b>Head TSL temperature during test</b>	(22.5 ± 0.2) °C	---	---

### SAR result with Head TSL at 5200 MHz

<b>SAR averaged over 1 cm<sup>3</sup> (1 g) of Head TSL</b>	condition	
SAR measured	100 mW input power	7.75 mW / g
SAR normalized	normalized to 1W	77.5 mW / g
SAR for nominal Head TSL parameters	normalized to 1W	77.2 mW / g ± 19.9 % (k=2)

<b>SAR averaged over 10 cm<sup>3</sup> (10 g) of Head TSL</b>	condition	
SAR measured	100 mW input power	2.19 mW / g
SAR normalized	normalized to 1W	21.9 mW / g
SAR for nominal Head TSL parameters	normalized to 1W	21.8 mW / g ± 19.5 % (k=2)



Document

**Appendix D for the BlackBerry® Smartphone Model  
RDU71CW/RDE71UW SAR Report Rev1**

Page  
**67(74)**

Author Data <b>Andrew Becker</b>	Dates of Test <b>Feb 7 – May 25, July 18, 2011</b>	Test Report No <b>RTS-3933-1105-11A</b> <b>RTS-2580-1106-03 Rev1</b>	FCC ID: <b>L6ARDU70CW</b> <b>L6ARDE70UW</b>	IC ID <b>2503A-RDU70CW</b> <b>2503A-RDE70UW</b>
-------------------------------------	---	--	---	---

### Head TSL parameters at 5500 MHz

The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
<b>Nominal Head TSL parameters</b>	22.0 °C	35.6	4.96 mho/m
<b>Measured Head TSL parameters</b>	(22.0 ± 0.2) °C	35.6 ± 6 %	4.93 mho/m ± 6 %
<b>Head TSL temperature during test</b>	(22.5 ± 0.2) °C	—	—

### SAR result with Head TSL at 5500 MHz

<b>SAR averaged over 1 cm<sup>3</sup> (1 g) of Head TSL</b>	condition	
SAR measured	100 mW input power	8.29 mW / g
SAR normalized	normalized to 1W	82.9 mW / g
SAR for nominal Head TSL parameters	normalized to 1W	<b>82.9 mW / g ± 19.9 % (k=2)</b>

<b>SAR averaged over 10 cm<sup>3</sup> (10 g) of Head TSL</b>	condition	
SAR measured	100 mW input power	2.32 mW / g
SAR normalized	normalized to 1W	23.2 mW / g
SAR for nominal Head TSL parameters	normalized to 1W	<b>23.2 mW / g ± 19.5 % (k=2)</b>

### Head TSL parameters at 5800 MHz

The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
<b>Nominal Head TSL parameters</b>	22.0 °C	35.3	5.27 mho/m
<b>Measured Head TSL parameters</b>	(22.0 ± 0.2) °C	34.2 ± 6 %	5.10 mho/m ± 6 %
<b>Head TSL temperature during test</b>	(22.5 ± 0.2) °C	—	—

### SAR result with Head TSL at 5800 MHz

<b>SAR averaged over 1 cm<sup>3</sup> (1 g) of Head TSL</b>	condition	
SAR measured	100 mW input power	7.62 mW / g
SAR normalized	normalized to 1W	76.2 mW / g
SAR for nominal Head TSL parameters	normalized to 1W	<b>75.6 mW / g ± 19.9 % (k=2)</b>

<b>SAR averaged over 10 cm<sup>3</sup> (10 g) of Head TSL</b>	condition	
SAR measured	100 mW input power	2.15 mW / g
SAR normalized	normalized to 1W	21.5 mW / g
SAR for nominal Head TSL parameters	normalized to 1W	<b>21.3 mW / g ± 19.5 % (k=2)</b>



Document

**Appendix D for the BlackBerry® Smartphone Model  
RDU71CW/RDE71UW SAR Report Rev1**Page  
**68(74)**

Author Data <b>Andrew Becker</b>	Dates of Test <b>Feb 7 – May 25, July 18, 2011</b>	Test Report No <b>RTS-3933-1105-11A</b> <b>RTS-2580-1106-03 Rev1</b>	FCC ID: <b>L6ARDU70CW</b> <b>L6ARDE70UW</b>	IC ID <b>2503A-RDU70CW</b> <b>2503A-RDE70UW</b>
-------------------------------------	---	--	---	---

**Body TSL parameters at 5500 MHz**

The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
<b>Nominal Body TSL parameters</b>	22.0 °C	48.6	5.65 mho/m
<b>Measured Body TSL parameters</b>	(22.0 ± 0.2) °C	47.5 ± 6 %	5.86 mho/m ± 6 %
<b>Body TSL temperature during test</b>	(22.5 ± 0.2) °C	---	---

**SAR result with Body TSL at 5500 MHz**

SAR averaged over 1 cm <sup>3</sup> (1 g) of Body TSL	condition	
SAR measured	100 mW input power	8.22 mW / g
SAR normalized	normalized to 1W	82.2 mW / g
SAR for nominal Body TSL parameters	normalized to 1W	<b>81.9 mW / g ± 19.9 % (k=2)</b>

SAR averaged over 10 cm <sup>3</sup> (10 g) of Body TSL	condition	
SAR measured	100 mW input power	2.28 mW / g
SAR normalized	normalized to 1W	22.8 mW / g
SAR for nominal Body TSL parameters	normalized to 1W	<b>22.7 mW / g ± 19.5 % (k=2)</b>



Document

**Appendix D for the BlackBerry® Smartphone Model  
RDU71CW/RDE71UW SAR Report Rev1**Page  
**69(74)**

Author Data <b>Andrew Becker</b>	Dates of Test <b>Feb 7 – May 25, July 18, 2011</b>	Test Report No <b>RTS-3933-1105-11A RTS-2580-1106-03 Rev1</b>	FCC ID: <b>L6ARDU70CW L6ARDE70UW</b>	IC ID <b>2503A-RDU70CW 2503A-RDE70UW</b>
-------------------------------------	---	--	---	---

**Appendix****Antenna Parameters with Head TSL at 5200 MHz**

Impedance, transformed to feed point	<b>50.1 Ω - 9.2 jΩ</b>
Return Loss	<b>-20.7 dB</b>

**Antenna Parameters with Head TSL at 5500 MHz**

Impedance, transformed to feed point	<b>51.2 Ω - 4.2 jΩ</b>
Return Loss	<b>-27.3 dB</b>

**Antenna Parameters with Head TSL at 5800 MHz**

Impedance, transformed to feed point	<b>56.0 Ω - 2.6 jΩ</b>
Return Loss	<b>-24.2 dB</b>

**Antenna Parameters with Body TSL at 5500 MHz**

Impedance, transformed to feed point	<b>51.1 Ω - 3.0 jΩ</b>
Return Loss	<b>-29.9 dB</b>

**General Antenna Parameters and Design**

Electrical Delay (one direction)	<b>1.202 ns</b>
----------------------------------	-----------------

After long term use with 40 W radiated power, only a slight warming of the dipole near the feedpoint can be measured.

The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals.

No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feedpoint may be damaged.

**Additional EUT Data**

Manufactured by	<b>SPEAG</b>
Manufactured on	<b>July 09, 2004</b>

 <p>Document  <b>Appendix D for the BlackBerry® Smartphone Model  RDU71CW/RDE71UW SAR Report Rev1</b></p>				Page <b>70(74)</b>
Author Data <b>Andrew Becker</b>	Dates of Test <b>Feb 7 – May 25, July 18, 2011</b>	Test Report No <b>RTS-3933-1105-11A  RTS-2580-1106-03 Rev1</b>	FCC ID: <b>L6ARDU70CW  L6ARDE70UW</b>	IC ID <b>2503A-RDU70CW  2503A-RDE70UW</b>

## **DASY5 Validation Report for Head TSL**

Date/Time: 12.11.2009 13:12:49

Test Laboratory: SPEAG, Zurich, Switzerland

**DUT: Dipole 5GHz; Type: D5GHzV2; Serial: D5GHzV2 - SN:1033**

Communication System: CW; Frequency: 5200 MHz, Frequency: 5500 MHz, Frequency: 5800 MHz; Duty Cycle: 1:1

Medium: HSL 3-6 GHz

Medium parameters used:  $f = 5200$  MHz;  $\sigma = 4.53$  mho/m;  $\epsilon_r = 35.4$ ;  $\rho = 1000$  kg/m<sup>3</sup>, Medium parameters used:  $f = 5500$  MHz;  $\sigma = 4.81$  mho/m;  $\epsilon_r = 34.8$ ;  $\rho = 1000$  kg/m<sup>3</sup>, Medium parameters used:  $f = 5800$  MHz;  $\sigma = 5.08$  mho/m;  $\epsilon_r = 34.3$ ;  $\rho = 1000$  kg/m<sup>3</sup>

Phantom section: Flat Section

Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2007)

DASY5 Configuration:

- Probe: EX3DV4 - SN3503; ConvF(5.36, 5.36, 5.36), ConvF(4.85, 4.85, 4.85), ConvF(4.74, 4.74, 4.74); Calibrated: 11.03.2009
- Sensor-Surface: 2mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn601; Calibrated: 07.03.2009
- Phantom: Flat Phantom 5.0 (front); Type: QD000P50AA; Serial: 1001
- Measurement SW: DASY5, V5.2 Build 157; SEMCAD X Version 14.0 Build 57

### **Configuration D5GHzV2 Dipole (Head)/d=10mm, Pin=250mW, f=5200 MHz/Area Scan**

**(91x91x1):** Measurement grid: dx=10mm, dy=10mm

Maximum value of SAR (interpolated) = 15.4 mW/g

### **Configuration D5GHzV2 Dipole/d=10mm, Pin=250mW, f=5200 MHz/Zoom Scan**

**(4x4x2.5mm), dist=2mm (8x8x10)/Cube 0:** Measurement grid: dx=4mm, dy=4mm, dz=2.5mm

Reference Value = 64.7 V/m; Power Drift = 0.035 dB

Peak SAR (extrapolated) = 30 W/kg

**SAR(1 g) = 7.75 mW/g; SAR(10 g) = 2.19 mW/g**

Maximum value of SAR (measured) = 15.3 mW/g

### **Configuration D5GHzV2 Dipole/d=10mm, Pin=250mW, f=5500 MHz/Zoom Scan**

**(4x4x2.5mm), dist=2mm (8x8x10)/Cube 0:** Measurement grid: dx=4mm, dy=4mm, dz=2.5mm

Reference Value = 65.4 V/m; Power Drift = 0.057 dB

Peak SAR (extrapolated) = 33.8 W/kg

**SAR(1 g) = 8.29 mW/g; SAR(10 g) = 2.32 mW/g**

Maximum value of SAR (measured) = 16.5 mW/g

### **Configuration D5GHzV2 Dipole/d=10mm, Pin=250mW, f=5800 MHz/Zoom Scan**

**(4x4x2.5mm), dist=2mm (8x8x10)/Cube 0:** Measurement grid: dx=4mm, dy=4mm, dz=2.5mm

Reference Value = 61.7 V/m; Power Drift = 0.067 dB

Peak SAR (extrapolated) = 32.4 W/kg


**SAR(1 g) = 7.62 mW/g; SAR(10 g) = 2.15 mW/g**



Document


**Appendix D for the BlackBerry® Smartphone Model  
RDU71CW/RDE71UW SAR Report Rev1**Page  
**71(74)**

Author Data <b>Andrew Becker</b>	Dates of Test <b>Feb 7 – May 25, July 18, 2011</b>	Test Report No <b>RTS-3933-1105-11A</b> <b>RTS-2580-1106-03 Rev1</b>	FCC ID: <b>L6ARDU70CW</b> <b>L6ARDE70UW</b>	IC ID <b>2503A-RDU70CW</b> <b>2503A-RDE70UW</b>
-------------------------------------	---	--	---	---

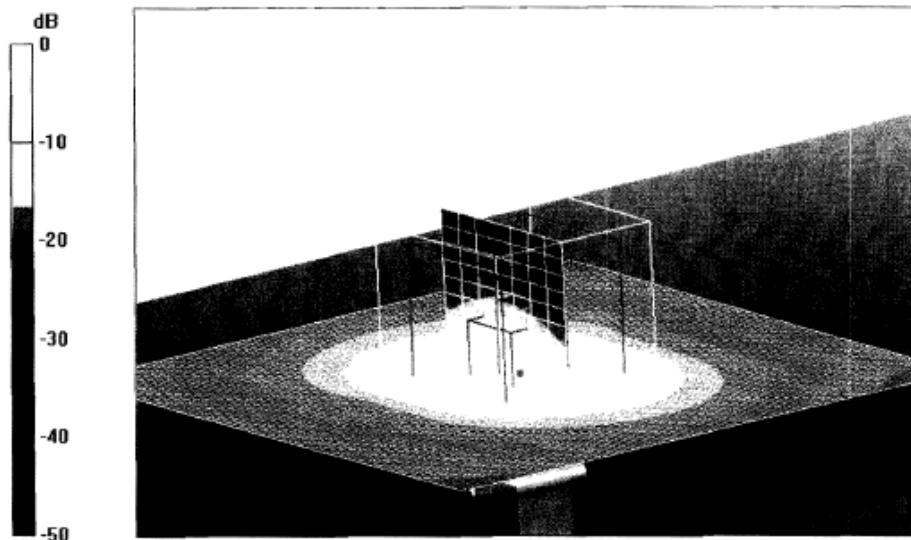

<b>RIM Testing Services</b>	Document <b>Appendix D for the BlackBerry® Smartphone Model RDU71CW/RDE71UW SAR Report Rev1</b>	Page <b>72(74)</b>
Author Data <b>Andrew Becker</b>	Dates of Test <b>Feb 7 – May 25, July 18, 2011</b>	Test Report No <b>RTS-3933-1105-11A RTS-2580-1106-03 Rev1</b> FCC ID: <b>L6ARDU70CW L6ARDE70UW</b> IC ID <b>2503A-RDU70CW 2503A-RDE70UW</b>

### Impedance Measurement Plot for Head TSL

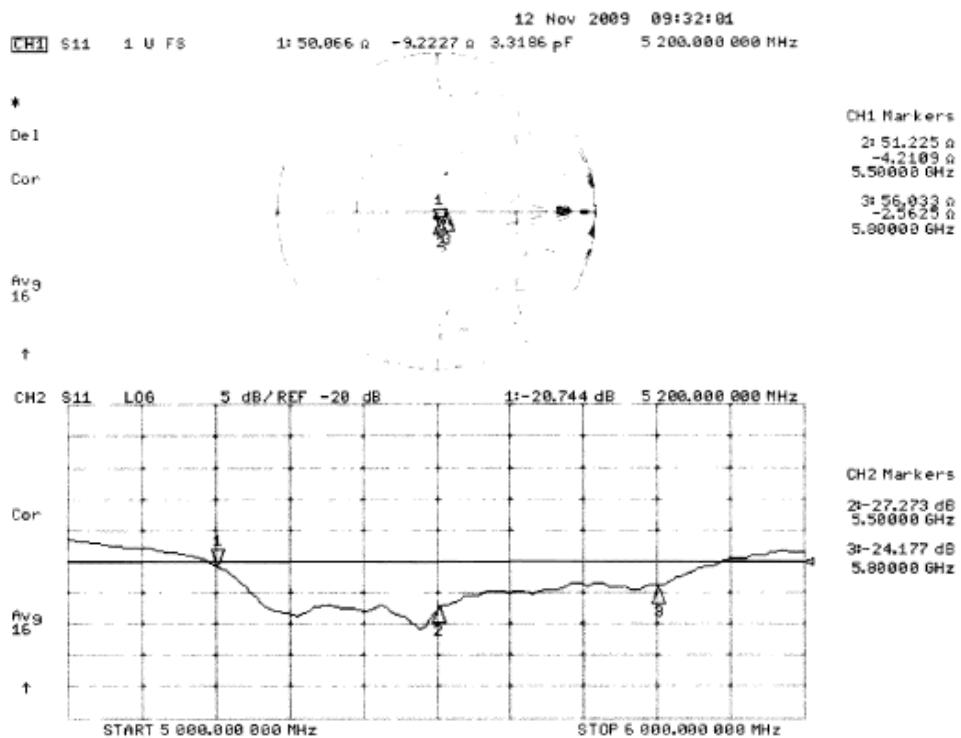

 Document <b>Appendix D for the BlackBerry® Smartphone Model RDU71CW/RDE71UW SAR Report Rev1</b>				Page <b>73(74)</b>
Author Data <b>Andrew Becker</b>	Dates of Test <b>Feb 7 – May 25, July 18, 2011</b>	Test Report No <b>RTS-3933-1105-11A RTS-2580-1106-03 Rev1</b>	FCC ID: <b>L6ARDU70CW L6ARDE70UW</b>	IC ID <b>2503A-RDU70CW 2503A-RDE70UW</b>

## DASY5 Validation Report for Body TSL

Date/Time: 13.11.2009 12:28:18

Test Laboratory: SPEAG, Zurich, Switzerland

**DUT: Dipole 5GHz; Type: D5GHzV2; Serial: D5GHzV2 - SN:1033**

Communication System: CW; Frequency: 5500 MHz; Duty Cycle: 1:1

Medium: MSL 3-6 GHz

Medium parameters used:  $f = 5500$  MHz;  $\sigma = 5.83$  mho/m;  $\epsilon_r = 47.6$ ;  $\rho = 1000$  kg/m<sup>3</sup>

Phantom section: Flat Section

Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2007)

DASY5 Configuration:

- Probe: EX3DV4 - SN3503; ConvF(4.37, 4.37, 4.37); Calibrated: 11.03.2009
- Sensor-Surface: 2mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn601; Calibrated: 07.03.2009
- Phantom: Flat Phantom 5.0 (back); Type: QD000P50AA; Serial: 1002
- Measurement SW: DASY5, V5.2 Build 157; SEMCAD X Version 14.0 Build 57

### Configuration D5GHzV2 Dipole/d=10mm, Pin=250mW, f=5500 MHz/Area Scan

(91x91x1): Measurement grid: dx=10mm, dy=10mm

Maximum value of SAR (interpolated) = 16.2 mW/g

### Configuration D5GHzV2 Dipole/d=10mm, Pin=250mW, f=5500 MHz/Zoom Scan


(4x4x2.5mm), dist=2mm (8x8x10)/Cube 0: Measurement grid: dx=4mm, dy=4mm, dz=2.5mm

Reference Value = 59.5 V/m; Power Drift = -0.044 dB

Peak SAR (extrapolated) = 33.3 W/kg

**SAR(1 g) = 8.22 mW/g; SAR(10 g) = 2.28 mW/g**

Maximum value of SAR (measured) = 16.4 mW/g

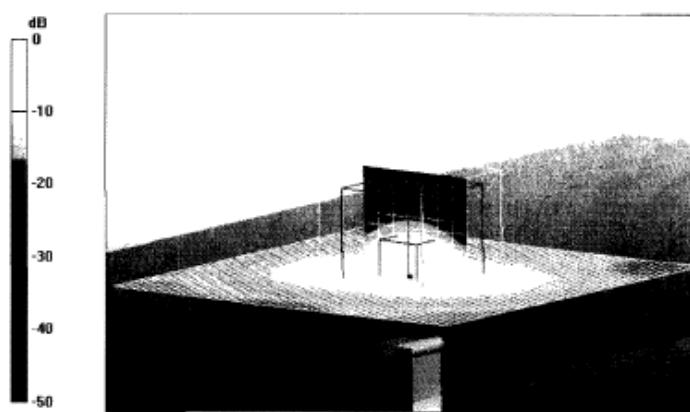

0 dB = 16.4 mW/g

Author Data <b>Andrew Becker</b>	Dates of Test <b>Feb 7 – May 25, July 18, 2011</b>	Test Report No <b>RTS-3933-1105-11A</b> <b>RTS-2580-1106-03 Rev1</b>	FCC ID: <b>L6ARDU70CW</b> <b>L6ARDE70UW</b>	IC ID <b>2503A-RDU70CW</b> <b>2503A-RDE70UW</b>
-------------------------------------	---	--	---	---

**Impedance Measurement Plot for Body TSL**
