



## **Accredited testing laboratory**

**DAR registration number: TTI-P-G 166/98**

**Federal Motor Transport Authority (KBA)  
DAR registration number: KBA-P 00070-97**

**Test report no. : 5-4113/02-1-3**  
**Type identification : BIRD (G4200D/001)**  
**Test specification : Draft IEEE Std 1528-200X**  
**FCC-ID : L82-BIRD**

## Table of Contents

|         |                                                              |    |
|---------|--------------------------------------------------------------|----|
| 1       | General Information .....                                    | 3  |
| 1.1     | Notes .....                                                  | 3  |
| 1.1.1   | Statement of Compliance.....                                 | 3  |
| 1.2     | Testing laboratory.....                                      | 4  |
| 1.3     | Details of applicant.....                                    | 4  |
| 1.4     | Application details.....                                     | 4  |
| 1.5     | Test item .....                                              | 5  |
| 1.5.1   | Test specification(s) .....                                  | 6  |
| 1.5.2   | RF exposure limits .....                                     | 6  |
| 2       | Technical test .....                                         | 7  |
| 2.1     | Summary of test results.....                                 | 7  |
| 2.2     | Test environment.....                                        | 7  |
| 2.3     | Measurement and test set-up .....                            | 7  |
| 2.4     | Measurement system.....                                      | 8  |
| 2.4.1   | System Description .....                                     | 8  |
| 2.4.2   | Test environment .....                                       | 9  |
| 2.4.3   | Probe description .....                                      | 9  |
| 2.4.4   | Phantom description.....                                     | 10 |
| 2.4.5   | Device holder description .....                              | 10 |
| 2.4.6   | Scanning procedure.....                                      | 11 |
| 2.4.7   | Spatial Peak SAR Evaluation.....                             | 12 |
| 2.4.8   | Data Storage and Evaluation.....                             | 13 |
| 2.4.9   | Test equipment utilized .....                                | 15 |
| 2.4.10  | Tissue dielectric properties .....                           | 16 |
| 2.4.11  | Tissue parameters.....                                       | 16 |
| 2.4.12  | Measurement uncertainties .....                              | 17 |
| 2.4.13  | System validation .....                                      | 18 |
| 2.4.14  | Validation procedure.....                                    | 18 |
| 2.5     | Test results (Body SAR) .....                                | 19 |
| 2.5.1   | Description of test positions during SAR evaluation.....     | 19 |
| 2.6     | Test results (power measurement) .....                       | 19 |
| Annex 1 | System performance verification .....                        | 20 |
| Annex 2 | Measurement results (printout from DASY <sup>TM</sup> )..... | 21 |
| Annex 3 | Photo documentation.....                                     | 28 |
| Annex 4 | Calibration parameters of E-field probe .....                | 40 |

## 1 General Information

### 1.1 Notes

The test results of this test report relate exclusively to the test item specified in 1.5. The CETECOM ICT Services GmbH does not assume responsibility for any conclusions and generalisations drawn from the test results with regard to other specimens or samples of the type of the equipment represented by the test item. The test report may only be reproduced or published in full. Reproduction or publication of extracts from the report requires the prior written approval of the CETECOM ICT Services GmbH.

#### 1.1.1 Statement of Compliance

The SAR values found for the BIRD portable phone with DECT technology are below the maximum recommended levels of 1.6 W/Kg as averaged over any 1 g tissue according the FCC rule §2.1093, the ANSI/IEEE C 95.1:1992 and the NCRP Report Number 86 for uncontrolled environment.

#### Test laboratory manager:

**October 9, 2002****Fabien Coulet**

Date

Name

Signature

---

#### Technical responsibility for area of testing:

**October 9, 2002****Bernd Rebmann**

Date

Name

Signature

---

## 1.2 Testing laboratory

CETECOM ICT Services GmbH  
Untertuerkheimer Straße 6-10,  
66117 Saarbruecken  
Germany  
Telephone: + 49 681 598 - 0  
Fax: + 49 681 598 - 8475

e-mail: [info@ict.cetecom.de](mailto:info@ict.cetecom.de)  
Internet: <http://www.cetecom-ict.de>

State of accreditation: The Test laboratory (area of testing) is accredited according to DIN EN ISO/IEC 17025. DAR registration number: TTI-P-G-166/98

Test location, if different from CETECOM ICT Services GmbH

Name:  
Street:  
Town:  
Country:  
Phone:  
Fax:

## 1.3 Details of applicant

Name: Siemens AG  
  
Street: Frankenstr. 2  
Town: 46395 Bocholt  
Country: Germany  
  
Contact: Uwe Alt  
Telephone: +49 (0) 2871 91-28 57

## 1.4 Application details

|                                 |                    |
|---------------------------------|--------------------|
| Date of receipt of application: | September 20, 2002 |
| Date of receipt of test item:   | September 23, 2002 |
| Start/Date of test:             | September 23, 2002 |
| End of test:                    | September 23, 2002 |

Person(s) present during the test:

## 1.5 Test item

|                                      |                                             |
|--------------------------------------|---------------------------------------------|
| Description of the test item:        | DECT                                        |
| Type identification:                 | BIRD (G4200D/001)                           |
| FCC-ID:                              | L82-BIRD                                    |
| Serial number:                       | S30852-S1415-R307-6                         |
| Manufacturer:                        |                                             |
| Name:                                | Siemens AG                                  |
| Street:                              | Frankenstr. 2                               |
| Town:                                | 46395 Bocholt                               |
| Country:                             | Germany                                     |
| additional information on the DUT:   |                                             |
| device type :                        | DECT (Digital Enhanced Cordless Telephone)  |
| device category :                    | portable device                             |
| test device production information : | production unit                             |
| exposure category :                  | general population / uncontrolled exposure  |
| device operating configurations :    |                                             |
| frequency range :                    | 2.407104 GHz to 2.469312 GHz                |
| operating mode :                     | DECT                                        |
|                                      | Digital modulated system according to FCC15 |
| maximum device rating :              | 234 mW (23.7 dBm)                           |
| antenna:                             | Integrated inverted F antenna               |
| battery type :                       | 2 rechargeable batteries (type AA)          |
| accessories :                        | ---                                         |
| Auxiliary equipment:                 | ---                                         |

### 1.5.1 Test specification(s)

Supplement C (Edition 01-01) to OET Bulletin 65 (Edition 97-01)

Draft IEEE Std 1528-200X: Version 6.4: July 2001

### 1.5.2 RF exposure limits

| Human Exposure                                  | Uncontrolled Environment<br>General Population | Controlled Environment<br>Occupational |
|-------------------------------------------------|------------------------------------------------|----------------------------------------|
| Spatial Peak SAR*<br>(Brain)                    | <b>1.60 mW/g</b>                               | 8.00 mW/g                              |
| Spatial Average SAR**<br>(Whole Body)           | 0.08 mW/g                                      | 0.40 mW/g                              |
| Spatial Peak SAR***<br>(Hands/Feet/Ankle/Wrist) | 4.00 mW/g                                      | 20.00 mW/g                             |

**Table 1: RF exposure limits**

The limit applied in this test report is shown in **bold** letters

**Notes:**

- \* The Spatial Peak value of the SAR averaged over any 1 gram of tissue (defined as a tissue volume in the shape of a cube) and over the appropriate averaging time
- \*\* The Spatial Average value of the SAR averaged over the whole body.
- \*\*\* The Spatial Peak value of the SAR averaged over any 10 grams of tissue (defined as a tissue volume in the shape of a cube) and over the appropriate averaging time.

**Uncontrolled Environments** are defined as locations where there is the exposure of individuals who have no knowledge or control of their exposure.

**Controlled Environments** are defined as locations where there is exposure that may be incurred by persons who are aware of the potential for exposure, (i.e. as a result of employment or occupation).

## 2 Technical test

### 2.1 Summary of test results

|                                                                                                          |                                     |
|----------------------------------------------------------------------------------------------------------|-------------------------------------|
| No deviations from the technical specification(s) were ascertained in the course of the tests performed. | <input checked="" type="checkbox"/> |
| The deviations as specified in 2.5 were ascertained in the course of the tests performed.                | <input type="checkbox"/>            |

### 2.2 Test environment

General Environment conditions in the test area are as follows :

Ambient temperature: 20°C – 24°C  
Tissue simulating liquid: 20°C – 24°C  
Humidity: 40% – 50%

Exact temperature values for each test are shown in the table(s) under 2.5. and/or on the measurement plots.

### 2.3 Measurement and test set-up


The measurement system is described in chapter 2.4.

The test setup for the system validation can be found in chapter 2.4.15.

A description of positioning and test signal control can be found in chapter 2.5 together with the test results.

## 2.4 Measurement system

### 2.4.1 System Description

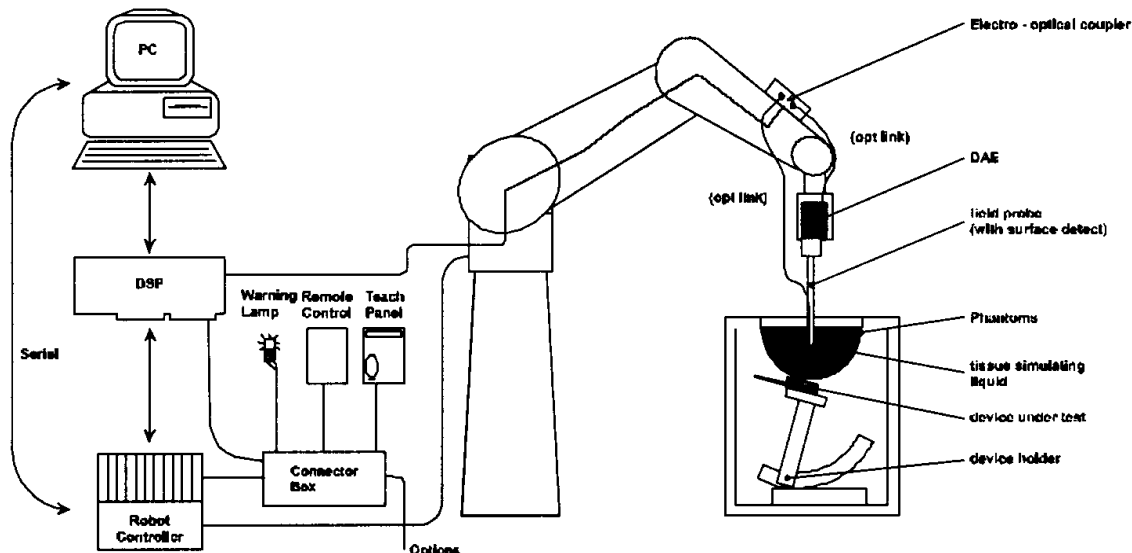

The DASY3 system for performing compliance tests consists of the following items:

- A standard high precision 6-axis robot (Stäubli RX family) with controller and software. An arm extension for accommodating the data acquisition electronics (DAE).
- A dosimetric probe, i.e. an isotropic E-field probe optimized and calibrated for usage in tissue simulating liquid. The probe is equipped with an optical surface detector system.
- A data acquisition electronic (DAE) which performs the signal amplification, signal multiplexing, AD-conversion, offset measurements, mechanical surface detection, collision detection, etc. The unit is battery powered with standard or rechargeable batteries. The signal is optically transmitted to the EOC.
- A unit to operate the optical surface detector which is connected to the EOC.
- The Electro-Optical Coupler (EOC) performs the conversion from the optical into a digital electric signal of the DAE. The EOC is connected to the PC plug-in card.
- The function of the PC plug-in card based on a DSP is to perform the time critical task such as signal filtering, surveillance of the robot operation fast movement interrupts.
- A computer operating Windows 95 or higher
- DASY3 software
- Remote control with teach panel and additional circuitry for robot safety such as warning lamps, etc.
- The generic twin phantom enabling the testing of left-hand and right-hand usage.
- The device holder for handheld mobile phones.
- Tissue simulating liquid mixed according to the given recipes.
- System validation dipoles allowing to validate the proper functioning of the system.



## 2.4.2 Test environment

The DASY3 measurement system is placed at the head end of a room with dimensions :  $5 \times 2.5 \times 3 \text{ m}^3$ , the SAM phantom is placed in a distance of 75 cm from the side walls and 1.1m from the rear wall. Above the test system a  $1.5 \times 1.5 \text{ m}^2$  array of pyramid absorbers is installed to reduce reflections from the ceiling.

Picture 1 of the photo documentation shows a complete view of the the test environment.

The system allows the measurement of SAR values larger than 0.005 mW/g.

## 2.4.3 Probe description


Isotropic E-Field Probe ET3DV6 for Dosimetric Measurements

| Technical data according to manufacturer information |                                                                                                                                                                                                                           |
|------------------------------------------------------|---------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|
| Construction                                         | Symmetrical design with triangular core<br>Built-in optical fiber for surface detection system<br>Built-in shielding against static charges<br>PEEK enclosure material (resistant to organic solvents, e.g., glycolether) |
| Calibration                                          | In air from 10 MHz to 2.5 GHz<br>In head tissue simulating liquid (HSL) at 900 (800-1000) MHz and 1.8 GHz (1700-1910 MHz)<br>(accuracy $\pm 9.5\%$ ; $k=2$ ) Calibration for other liquids and frequencies upon request   |
| Frequency                                            | 10 MHz to 3 GHz (dosimetry); Linearity: $\pm 0.2 \text{ dB}$ (30 MHz to 3 GHz)                                                                                                                                            |
| Directivity                                          | $\pm 0.2 \text{ dB}$ in HSL (rotation around probe axis)<br>$\pm 0.4 \text{ dB}$ in HSL (rotation normal to probe axis)                                                                                                   |
| Dynamic range                                        | $5 \mu\text{W/g}$ to $> 100 \text{ mW/g}$ ; Linearity: $\pm 0.2 \text{ dB}$                                                                                                                                               |
| Optical Surface Detection                            | $\pm 0.2 \text{ mm}$ repeatability in air and clear liquids over diffuse reflecting surfaces (ET3DV6 only)                                                                                                                |
| Dimensions                                           | Overall length: 330 mm<br>Tip length: 16 mm<br>Body diameter: 12 mm<br>Tip diameter: 6.8 mm<br>Distance from probe tip to dipole centers: 2.7 mm                                                                          |
| Application                                          | General dosimetry up to 3 GHz<br>Compliance tests of mobile phones<br>Fast automatic scanning in arbitrary phantoms (ET3DV6)                                                                                              |

#### 2.4.4 Phantom description

The used SAM Phantom meets the requirements specified in Edition 01-01 of Supplement C to OET Bulletin 65 for Specific Absorption Rate (SAR) measurements.

The phantom consists of a fibreglass shell integrated in a wooden table. It allows left-hand and right-hand head as well as body-worn measurements with a maximum liquid depth of 18 mm in head position and 22 mm in planar position (body measurements). The thickness of the Phantom shell is 2 mm +/- 0.1 mm.

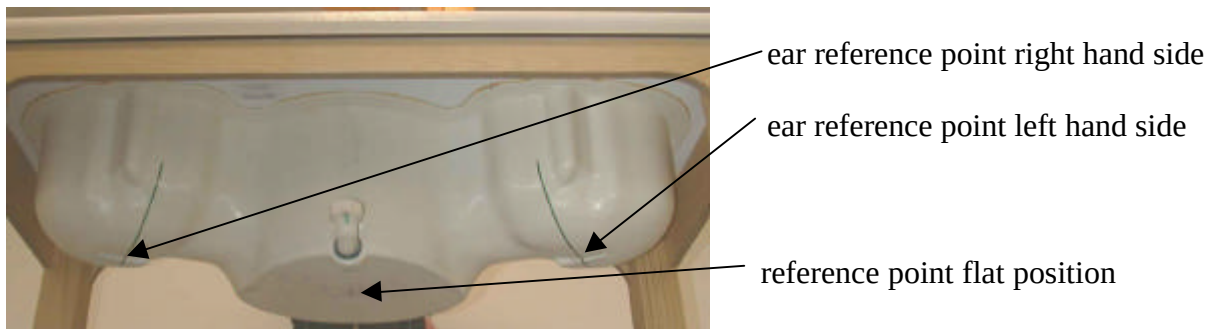

#### 2.4.5 Device holder description

The DASY3 device holder has two scales for device rotation (with respect to the body axis) and the device inclination (with respect to the line between the ear openings). The plane between the ear openings and the mouth tip has a rotation angle of 65°. The bottom plate contains three pair of bolts for locking the device holder. The device holder positions are adjusted to the standard measurement positions in the three sections. This device holder is used for standard mobile phones or PDA's only. If necessary an additional support of polystyrene material is used.



Larger DUT's (e.g. notebooks) cannot be tested using this device holder. Instead a support of bigger polystyrene cubes and thin polystyrene plates is used to position the DUT in all relevant positions to find and measure spots with maximum SAR values .

Therefore those devices are normally only tested at the flat part of the SAM.

## 2.4.6 Scanning procedure

The DASY3 installation includes predefined files with recommended procedures for measurements and validation. They are read-only document files and destined as fully defined but unmeasured masks. All test positions (head or body-worn) are tested with the same configuration of test steps differing only in the grid definition for the different test positions.

- The „reference“ and „drift“ measurements are located at the beginning and end of the batch process. They measure the field drift at one single point in the liquid over the complete procedure. The indicated drift is mainly the variation of the DUT's output power and should vary max. +/- 5 %.
- The „surface check“ measurement tests the optical surface detection system of the DASY3 system by repeatedly detecting the surface with the optical and mechanical surface detector and comparing the results. The output gives the detecting heights of both systems, the difference between the two systems and the standard deviation of the detection repeatability. Air bubbles or refraction in the liquid due to separation of the sugar-water mixture gives poor repeatability (above  $\pm 0.1\text{mm}$ ). To prevent wrong results tests are only executed when the liquid is free of air bubbles. The difference between the optical surface detection and the actual surface depends on the probe and is specified with each probe. (It does not depend on the surface reflectivity or the probe angle to the surface within  $\pm 30^\circ$ .)

The „coarse scan“ measures the SAR above the dipole on a parallel plane to the surface. It is used to locate the approximate location of the peak SAR with 2D spline interpolation. The robot performs a stepped movement along one grid axis while the local electrical field strength is measured by the probe. The standard scan uses large grid spacing for faster measurement. Standard grid spacing for head measurements is 15 mm in x- and y- dimension. If a finer graphic is needed, the grid spacing can be reduced. Grid spacing and orientation have no influence on the SAR result. For special applications where the standard scan method does not find the peak SAR within the grid, e.g. mobile phones with flip cover, the grid can be adapted in orientation.

Results of this coarse scan are shown in annex 2.

- A „cube 5x5x7 scan“ measures the field in a volume around the 2D peak SAR value acquired in the previous „coarse“ scan. This is a fine 5x5 grid where the robot additionally moves the probe in 7 steps along the z-axis away from the bottom of the Phantom. Grid spacing for the cube measurement is 8 mm in x and y-direction and 5 mm in z-direction. In this document, the evaluated peak 1g and 10g averaged SAR values are shown in the 2D-graphics in annex 2. Test results relevant for the specified standard (see chapter 1.7.) are shown in table form in chapter 2.5.

## 2.4.7 Spatial Peak SAR Evaluation

The spatial peak SAR - value for 1 and 10 g is evaluated after the Cube measurements have been done. The basis of the evaluation are the SAR values measured at the points of the fine cube grid consisting of 5 x 5 x 7 points. If any parameter is changed afterwards with 'File Modify' (for example crest factor or medium factors) a re-evaluation of the measurement is needed. This evaluation can be repeated by selecting 'Job Evaluation' on the selected scans. The algorithm that finds the maximal averaged volume is separated into three different stages.

- The data between the dipole center of the probe and the surface of the phantom are extrapolated. This data cannot be measured since the center of the dipole is 2.7 mm away from the tip of the probe and the distance between the surface and the lowest measuring point is about 1 mm (see probe calibration sheet). The extrapolated data from a cube measurement can be visualized by selecting 'Graph Evaluated'.
- The maximum interpolated value is searched with a straight-forward algorithm. Around this maximum the SAR - values averaged over the spatial volumes (1g or 10 g) are computed using the 3d-spline interpolation algorithm. If the volume cannot be evaluated (i.e., if a part of the grid was cut off by the boundary of the measurement area) the evaluation will be started on the corners of the bottom plane of the cube.
- All neighboring volumes are evaluated until no neighboring volume with a higher average value is found.

### Extrapolation

The extrapolation is based on a least square algorithm [W. Gander, Computermathematik, p.168-180]. Through the points in the first 3 cm along the z-axis, polynomials of order four are calculated. These polynomials are then used to evaluate the points between the surface and the probe tip. The points, calculated from the surface, have a distance of 1 mm from each other.

### Interpolation

The interpolation of the points is done with a 3d-Spline. The 3d-Spline is composed of three one-dimensional splines with the "Not a knot"-condition [W. Gander, Computermathematik, p.141-150] (x, y and z -direction) [Numerical Recipes in C, Second Edition, p.123ff ].

### Volume Averaging

At First the size of the cube is calculated. Then the volume is integrated with the trapezoidal algorithm. 8000 points (20x20x20) are interpolated to calculate the average.

### Advanced Extrapolation

The BIOEMC group of the ETH Zurich is currently investigating the boundary effects on E-field probes. As soon as the research is finished DASY3 will allow to compensate for these boundary effects. But until then we do not encourage to use the 'Advanced Extrapolation' option.

## 2.4.8 Data Storage and Evaluation

### 2.4.8.1 Data Storage

The DASY3 software stores the acquired data from the data acquisition electronics as raw data (in microvolt readings from the probe sensors), together with all necessary software parameters for the data evaluation (probe calibration data, liquid parameters and device frequency and modulation data) in measurement files with the extension ".DA3". The software evaluates the desired unit and format for output each time the data is visualized or exported. This allows verification of the complete software setup even after the measurement and allows correction of incorrect parameter settings. For example, if a measurement has been performed with a wrong crest factor parameter in the device setup, the parameter can be corrected afterwards and the data can be re-evaluated. To avoid unintentional parameter changes or data manipulations, the parameters in measured files are locked. In the administrator access mode of the software, the parameters can be unlocked by selecting the "modify"-switch in the "file"-pull down menu. After changing the parameters, the measured scans must be re-evaluated by selecting them and using the "evaluate"-option in the "scan"-pull down menu.

The measured data can be visualized or exported in different units or formats, depending on the selected probe type ([V/m], [A/m], [°C], [mW/g], [mW/cm<sup>2</sup>], [dBrel], etc.). Some of these units are not available in certain situations or show meaningless results, e.g., a SAR output in a lossless media will always be zero. Raw data can also be exported to perform the evaluation with other software packages.

### 2.4.8.2 Data Evaluation

The DASY3 software automatically executes the following procedures to calculate the field units from the microvolt readings at the probe connector. The parameters used in the evaluation are stored in the configuration modules of the software:

|                    |                           |                                                                         |
|--------------------|---------------------------|-------------------------------------------------------------------------|
| Probe parameters:  | - Sensitivity             | Norm <sub>i</sub> , a <sub>i0</sub> , a <sub>i1</sub> , a <sub>i2</sub> |
|                    | - Conversion factor       | ConvF <sub>i</sub>                                                      |
|                    | - Diode compression point | Dcpi                                                                    |
| Device parameters: | - Frequency               | f                                                                       |
|                    | - Crest factor            | cf                                                                      |
| Media parameters:  | - Conductivity            | s                                                                       |
|                    | - Density                 | r                                                                       |

These parameters must be set correctly in the software. They can be found in the component documents or they can be imported into the software from the configuration files issued for the DASY3 components. In the direct measuring mode of the multimeter option, the parameters of the actual system setup are used. In the scan visualization and export modes, the parameters stored in the corresponding document files are used.

The first step of the evaluation is a linearization of the filtered input signal to account for the compression characteristics of the detector diode. The compensation depends on the input signal, the diode type and the DC-transmission factor from the diode to the evaluation electronics.

If the exciting field is pulsed, the crest factor of the signal must be known to correctly compensate for peak power. The formula for each channel can be given as:

$$V_i = U_i + U_i^2 \cdot cf/dcp_i$$

with  $V_i$  = compensated signal of channel i (i = x, y, z)  
 $U_i$  = input signal of channel i (i = x, y, z)  
 $cf$  = crest factor of exciting field (DASY parameter)  
 $dcp_i$  = diode compression point (DASY parameter)

From the compensated input signals the primary field data for each channel can be evaluated:

E-field probes:  $E_i = (V_i / Norm_i \cdot ConvF)^{1/2}$

H-field probes:  $H_i = (V_i)^{1/2} \cdot (a_{i0} + a_{i1}f + a_{i2}f^2)/f$

with  $V_i$  = compensated signal of channel i (i = x, y, z)  
 $Norm_i$  = sensor sensitivity of channel i (i = x, y, z)  
[mV/(V/m)<sup>2</sup>] for E-field Probes  
 $ConvF$  = sensitivity enhancement in solution  
 $a_{ij}$  = sensor sensitivity factors for H-field probes  
 $f$  = carrier frequency [GHz]  
 $E_i$  = electric field strength of channel i in V/m  
 $H_i$  = magnetic field strength of channel i in A/m

The RSS value of the field components gives the total field strength (Hermitian magnitude):

$$E_{tot} = (E_x^2 + E_y^2 + E_z^2)^{1/2}$$

The primary field data are used to calculate the derived field units.

$$SAR = (E_{tot}^2 \cdot s) / (r \cdot 1000)$$

with  $SAR$  = local specific absorption rate in mW/g  
 $E_{tot}$  = total field strength in V/m  
 $s$  = conductivity in [mho/m] or [Siemens/m]  
 $r$  = equivalent tissue density in g/cm<sup>3</sup>

Note that the density is normally set to 1 (or 1.06), to account for actual brain density rather than the density of the simulation liquid. The power flow density is calculated assuming the excitation field to be a free space field.

$$P_{pwe} = E_{tot}^2 / 3770 \quad \text{or} \quad P_{pwe} = H_{tot}^2 \cdot 37.7$$

with  $P_{pwe}$  = equivalent power density of a plane wave in mW/cm<sup>2</sup>  
 $E_{tot}$  = total electric field strength in V/m  
 $H_{tot}$  = total magnetic field strength in A/m

## 2.4.9 Test equipment utilized

This table gives a complete overview of the SAR measurement equipment

Devices used during the test described in chapter 2.5. are marked ☒

|                                     | Manufacturer                    | Device                                                         | Type             | Serial number | Date of last calibration )* |
|-------------------------------------|---------------------------------|----------------------------------------------------------------|------------------|---------------|-----------------------------|
| <input checked="" type="checkbox"/> | Schmid & Partner Engineering AG | Dosimetric E-Field Probe                                       | ET3DV6           | 1558          | March 22, 2002              |
| <input type="checkbox"/>            | Schmid & Partner Engineering AG | Dosimetric E-Field Probe (spare)                               | ET3DV6           | 1559          | February 20, 2001           |
| <input type="checkbox"/>            | Schmid & Partner Engineering AG | 900 MHz System Validation Dipole                               | D900V2           | 102           | February 13, 2001           |
| <input type="checkbox"/>            | Schmid & Partner Engineering AG | 1800 MHz System Validation Dipole                              | D1800V2          | 287           | February 13, 2001           |
| <input type="checkbox"/>            | Schmid & Partner Engineering AG | 1900 MHz System Validation Dipole                              | D1900V2          | 5d009         | June 13, 2002               |
| <input checked="" type="checkbox"/> | Schmid & Partner Engineering AG | 2450 MHz System Validation Dipole                              | D2450V2          | 710           | July 15, 2002               |
| <input checked="" type="checkbox"/> | Schmid & Partner Engineering AG | Data acquisition electronics                                   | DAE3V1           | 413           | N/A                         |
| <input checked="" type="checkbox"/> | Schmid & Partner Engineering AG | Software                                                       | DASY 3 V3.1c     | ---           | N/A                         |
| <input checked="" type="checkbox"/> | Schmid & Partner Engineering AG | Phantom                                                        | SAM              | ---           | N/A                         |
| <input type="checkbox"/>            | Rohde & Schwarz                 | Universal Radio Communication Tester (used as controller only) | CMU 200          | U-972406/000  | August 30, 2001             |
|                                     |                                 |                                                                |                  |               |                             |
|                                     | Agilent                         | Network Analyser 300 kHz to 3 GHz                              | 8753C            | 2936A00872    | February 26, 2002           |
| <input type="checkbox"/>            | Agilent                         | Dielectric Probe Kit                                           | 85070C           | US99360146    | March 8, 2001               |
|                                     |                                 |                                                                |                  |               |                             |
| <input checked="" type="checkbox"/> | Agilent                         | Peak Power Analyzer                                            | 8990A            | 3128A00169    | August 6, 2002              |
| <input checked="" type="checkbox"/> | Agilent                         | Peak Power Sensor                                              | 84813A           | 3125A00111    | September 18, 2002          |
|                                     |                                 |                                                                |                  |               |                             |
| <input checked="" type="checkbox"/> | Rohde & Schwarz                 | Signal Generator                                               | SMPD             | 882.362/009   | January 11, 2002            |
| <input checked="" type="checkbox"/> | Amplifier Reasearch             | Amplifier                                                      | 25S1G4 (25 Watt) | 20452         | N/A                         |
| <input checked="" type="checkbox"/> | Agilent                         | Power Meter                                                    | 438A             | 2804U01006    | April 12, 2002              |
| <input checked="" type="checkbox"/> | Agilent                         | Power Meter Sensor                                             | 8482A            | 2703A03025    | April 22, 2002              |

)\* : Measurement devices are in a 1-year calibration cycle, validation dipoles are in a 2-year calibration cycle



## 2.4.10 Tissue dielectric properties

The following materials are used for producing the tissue-equivalent materials:

| Ingredients<br>(% of weight) | Frequency (MHz)              |       |                              |      |                              |       |                               |       |                               |       |                                          |      |
|------------------------------|------------------------------|-------|------------------------------|------|------------------------------|-------|-------------------------------|-------|-------------------------------|-------|------------------------------------------|------|
|                              | <input type="checkbox"/> 450 |       | <input type="checkbox"/> 835 |      | <input type="checkbox"/> 900 |       | <input type="checkbox"/> 1800 |       | <input type="checkbox"/> 1900 |       | <input checked="" type="checkbox"/> 2450 |      |
| Tissue Type                  | Head                         | Body  | Head                         | Body | Head                         | Body  | Head                          | Body  | Head                          | Body  | Head                                     | Body |
| Water                        | 38.56                        | 51.16 | 41.45                        | 52.4 | 41.05                        | 56.0  | 52.64                         | 69.91 | 52.64                         | 69.91 | 62.7                                     | 73.2 |
| Salt (NaCl)                  | 3.95                         | 1.49  | 1.45                         | 1.40 | 1.35                         | 0.76  | 0.36                          | 0.13  | 0.36                          | 0.13  | 0.5                                      | 0.04 |
| Sugar                        | 56.32                        | 46.78 | 56.0                         | 45.0 | 56.5                         | 41.76 | 0.0                           | 0.0   | 0.0                           | 0.0   | 0.0                                      | 0.0  |
| HEC                          | 0.98                         | 0.52  | 1.0                          | 1.0  | 1.0                          | 1.21  | 0.0                           | 0.0   | 0.0                           | 0.0   | 0.0                                      | 0.0  |
| Bactericide                  | 0.19                         | 0.05  | 0.1                          | 0.1  | 0.1                          | 0.27  | 0.0                           | 0.0   | 0.0                           | 0.0   | 0.0                                      | 0.0  |
| Triton X-100                 | 0.0                          | 0.0   | 0.0                          | 0.0  | 0.0                          | 0.0   | 0.0                           | 0.0   | 0.0                           | 0.0   | 36.8                                     | 0.0  |
| DGBE                         | 0.0                          | 0.0   | 0.0                          | 0.0  | 0.0                          | 0.0   | 47.0                          | 29.96 | 47.0                          | 29.96 | 0.0                                      | 26.7 |

**Table 2: Tissue dielectric properties**

Salt: 99+% Pure Sodium Chloride

Sugar: 98+% Pure Sucrose

Water: De-ionized, 16MΩ+ resistivity

HEC: Hydroxyethyl Cellulose

DGBE: 99+% Di(ethylene glycol) butyl ether, [2-(2-butoxyethoxy)ethanol]

Triton X-100(ultra pure): Polyethylene glycol mono [4-(1,1,3,3-tetramethylbutyl)phenyl]ether

## 2.4.11 Tissue parameters

| Used Target<br>Frequency<br>[GHz]        | Target<br>Head Tissue |                            | Target<br>Body Tissue |                            | Measured<br>Head Tissue |                            | Measured<br>Body Tissue |                            | Measured<br>Date |
|------------------------------------------|-----------------------|----------------------------|-----------------------|----------------------------|-------------------------|----------------------------|-------------------------|----------------------------|------------------|
|                                          | Permit-<br>tivity     | Conduc-<br>tivity<br>[S/m] | Permit-<br>tivity     | Conduc-<br>tivity<br>[S/m] | Permit-<br>tivity       | Conduc-<br>tivity<br>[S/m] | Permit-<br>tivity       | Conduc-<br>tivity<br>[S/m] |                  |
| <input type="checkbox"/> 450             | 44.0                  | 0.88                       | 56.7                  | 0.94                       | ---                     | ---                        | 60.6                    | 0.84                       | 2002-02-25       |
| <input type="checkbox"/> 835             | 41.5                  | 0.90                       | 55.2                  | 0.97                       | ---                     | ---                        | ---                     | ---                        | ---              |
| <input type="checkbox"/> 900             | 41.5                  | 0.97                       | 55.0                  | 1.05                       | 44.5                    | 0.95                       | 55.4                    | 0.98                       | 2002-08-22       |
| <input type="checkbox"/> 915             | 41.5                  | 0.98                       | 55.0                  | 1.06                       | ---                     | ---                        | ---                     | ---                        | ---              |
| <input type="checkbox"/> 1800            | 40.0                  | 1.38                       | 53.3                  | 1.52                       | 38.7                    | 1.40                       | 54.6                    | 1.31                       | 2002-08-22       |
| <input type="checkbox"/> 1900            | 40.0                  | 1.40                       | 53.3                  | 1.52                       | 38.3                    | 1.51                       | 55.8                    | 1.54                       | 2002-08-22       |
| <input checked="" type="checkbox"/> 2450 | 39.2                  | 1.80                       | 52.7                  | 1.95                       | 42.1                    | 1.88                       | 56.1                    | 2.01                       | 2002-09-05       |

**Table 3: Parameter of the tissue simulating liquid**

Note: The dielectric properties have been measured using the contact probe method at 22°C.



## 2.4.12 Measurement uncertainties

The overall combined measurement uncertainty of the measurement system is  $\pm 13,6\%$  ( $K=1$ ).

The breakdown of the individual uncertainties is as follows:

| Error Sources                | Uncertainty Value | Probability Distribution | Divisor    | $c_i$          | Standard Uncertainty | $v_i^2$ or $v_{eff}$ |
|------------------------------|-------------------|--------------------------|------------|----------------|----------------------|----------------------|
| <b>Measurement System</b>    |                   |                          |            |                |                      |                      |
| Probe calibration            | $\pm 4.4\%$       | Normal                   | 1          | 1              | $\pm 4.4\%$          | 8                    |
| Axial isotropy               | $\pm 4.7\%$       | Rectangular              | $\sqrt{3}$ | $(1-cp)^{1/2}$ | $\pm 1.9\%$          | 8                    |
| Spherical isotropy           | $\pm 9.6\%$       | Rectangular              | $\sqrt{3}$ | $(cp)^{1/2}$   | $\pm 3.9\%$          | 8                    |
| Spatial resolution           | $\pm 0.0\%$       | Rectangular              | $\sqrt{3}$ | 1              | $\pm 0.0\%$          | 8                    |
| Boundary effects             | $\pm 5.5\%$       | Rectangular              | $\sqrt{3}$ | 1              | $\pm 3.2\%$          | 8                    |
| Probe linearity              | $\pm 4.7\%$       | Rectangular              | $\sqrt{3}$ | 1              | $\pm 2.7\%$          | 8                    |
| Detection limit              | $\pm 1.0\%$       | Rectangular              | $\sqrt{3}$ | 1              | $\pm 0.6\%$          | 8                    |
| Readout electronics          | $\pm 1.0\%$       | Normal                   | 1          | 1              | $\pm 1.0\%$          | 8                    |
| Response time                | $\pm 0.8\%$       | Rectangular              | $\sqrt{3}$ | 1              | $\pm 0.5\%$          | 8                    |
| Integration time             | $\pm 1.4\%$       | Rectangular              | $\sqrt{3}$ | 1              | $\pm 0.8\%$          | 8                    |
| RF ambient conditions        | $\pm 3.0\%$       | Rectangular              | $\sqrt{3}$ | 1              | $\pm 1.7\%$          | 8                    |
| Mech. robot constructions    | $\pm 0.4\%$       | Rectangular              | $\sqrt{3}$ | 1              | $\pm 0.2\%$          | 8                    |
| Probe positioning            | $\pm 2.9\%$       | Rectangular              | $\sqrt{3}$ | 1              | $\pm 1.7\%$          | 8                    |
| Extrapolation & integration  | $\pm 3.9\%$       | Rectangular              | $\sqrt{3}$ | 1              | $\pm 2.3\%$          | 8                    |
| <b>Test Sample Related</b>   |                   |                          |            |                |                      |                      |
| Device holder                | $\pm 6.0\%$       | Normal                   | 0.89       | 1              | $\pm 6.7\%$          | 12                   |
| Device holder uncertainty    | $\pm 5.0\%$       | Normal                   | 0.84       | 1              | $\pm 5.9\%$          | 8                    |
| Power drift                  | $\pm 5.0\%$       | Rectangular              | $\sqrt{3}$ | 1              | $\pm 2.9\%$          | 8                    |
| <b>Phantom and Set-up</b>    |                   |                          |            |                |                      |                      |
| Phantom uncertainty          | $\pm 4.0\%$       | Rectangular              | $\sqrt{3}$ | 1              | $\pm 2.3\%$          | 8                    |
| Liquid conductivity (target) | $\pm 5.0\%$       | Rectangular              | $\sqrt{3}$ | 0.6            | $\pm 1.7\%$          | 8                    |
| Liquid conductivity (meas.)  | $\pm 10.0\%$      | Rectangular              | $\sqrt{3}$ | 0.6            | $\pm 3.5\%$          | 8                    |
| Liquid permittivity (target) | $\pm 5.0\%$       | Rectangular              | $\sqrt{3}$ | 0.6            | $\pm 1.7\%$          | 8                    |
| Liquid permittivity (meas.)  | $\pm 5.0\%$       | Rectangular              | $\sqrt{3}$ | 0.6            | $\pm 1.7\%$          | 8                    |
| <b>Combined Uncertainty</b>  |                   |                          |            |                | $\pm 13.6\%$         |                      |

**Table 4: Measurement uncertainties**

The measurement uncertainty budget suggested by IEEE Std 1528-200X and determined by Schmid & Partner Engineering AG. The expanded uncertainty ( $k=2$ ) is assessed to be  $\pm 27.2\%$

### 2.4.13 System validation

The system validation is used for verifying the accuracy of the complete measurement system and performance of the software. The system validation is performed with tissue equivalent material according to IEEE Std 1528-200X: 2001. The following table shows validation result(s) for the SAR test . Validation(s) valid for the tests performed for this test report are in bold letters (graphic plot(s) see annex 1).


| Validation Kit       | Frequency               | Target SAR <sub>1g</sub><br>(1000 mW)<br>(+/- 10%) | Target SAR <sub>10g</sub><br>(1000 mW)<br>(+/- 10%) | Measured SAR <sub>1g</sub> | Measured SAR <sub>10g</sub> | Measured date |
|----------------------|-------------------------|----------------------------------------------------|-----------------------------------------------------|----------------------------|-----------------------------|---------------|
| DV2 2450,<br>S/N:710 | 2450 MHz<br><b>head</b> | 57.6 mW/g                                          | 26.5 mW/g                                           | 54.4 mW/g                  | 25.6 mW/g                   | 2002-09-23    |

**Table 5: Results system validation**

### 2.4.14 Validation procedure

The validation is performed by using a validation dipole which is positioned parallel to the planar part of the SAM phantom at the reference point. The distance of the dipole to the SAM phantom is determined by a plexiglass distance holder. The dipole is connected to the the signal source consisting of signal generator and amplifier via an directional coupler , N-connector cable and adaption to SMA. It is fed with a power of 1000 mW. To adjust this power a power meter is used . The power sensor is connected to the cable before the validation to measure the power at this point and do adjustments at the signal generator. At the outputs of the directional coupler both return loss as well as forward power are controlled during the validation to make sure that emitted power at the dipole keeps being constant. This can also be checked by the power drift measurement after the test (result on plot).

Validation results have to be equal or near the values determined during dipole calibration (target SAR in table above) with the relevant liquids and test system.

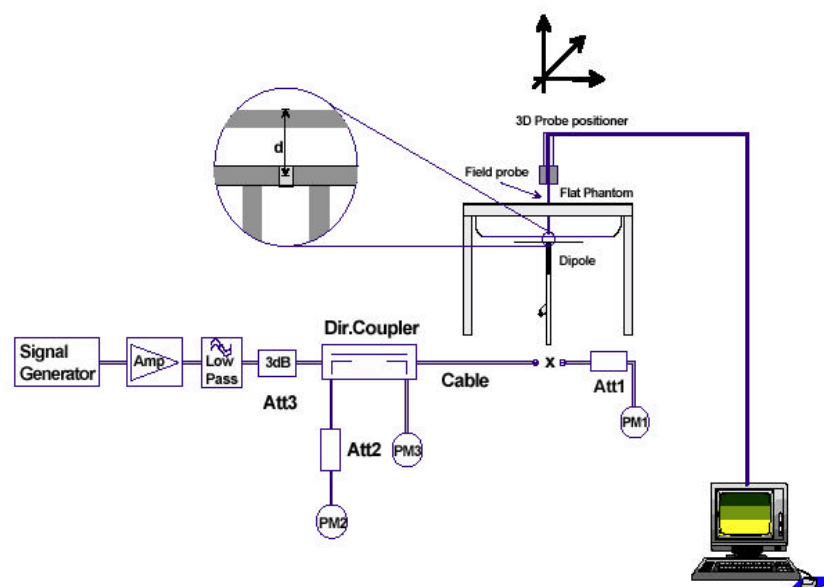

## 2.5 Test results (Body SAR)

| The table contains the measured SAR values averaged over a mass of 1 g |                        |                    |                     |          |                    |
|------------------------------------------------------------------------|------------------------|--------------------|---------------------|----------|--------------------|
| Channel/frequency                                                      | Position               | Left hand position | Right hand position | Limit    | Liquid temperature |
| 2441.664 MHz                                                           | cheek first peak       | 0.0100 W/kg        | 0.0085 W/kg         | 1.6 W/kg | 19.7 °C            |
| 2441.664 MHz                                                           | cheek second peak      | 0.0100 W/kg        | 0.0079 W/kg         | 1.6 W/kg | 19.7 °C            |
| 2441.664 MHz                                                           | tilted 15° first Peak  | 0.0071 W/kg        | 0.0067 W/kg         | 1.6 W/kg | 19.8 °C            |
| 2441.664 MHz                                                           | tilted 15° second Peak | 0.0033 W/kg        | 0.0026 W/kg         | 1.6 W/kg | 20.0 °C            |

**Table 6: Test results (Head SAR)**

Note: Upper and lower frequencies were not measured because the values at mid-band frequency do not exceeded 0.8 W/kg (1.60 W/kg reduced of 3dB)

### 2.5.1 Description of test positions during SAR evaluation

Test positions of the DECT handset are in accordance to the definitions given in IEEE Std. 1528-200X for testing of mobile phones. The device was tested in left and right head positions only as no body worn accessory is available.

The test was performed using head tissue simulating liquid for 2450 MHz.

The DECT handset was operating in standard configuration using the base station belonging to it and an integrated test software.


During the test a crest factor of 25 (typical for DECT) was used which resulted in very low SAR values which are near the noise floor of the measurement system.

## 2.6 Test results (power measurement)


| DECT 2.4 GHz        |                   |
|---------------------|-------------------|
| Channel / frequency | peak power (EIRP) |
| 2441.664 MHz        | 23.7 dBm          |


**Table 7: Test results (Head SAR)**

## Annex 1 System performance verification

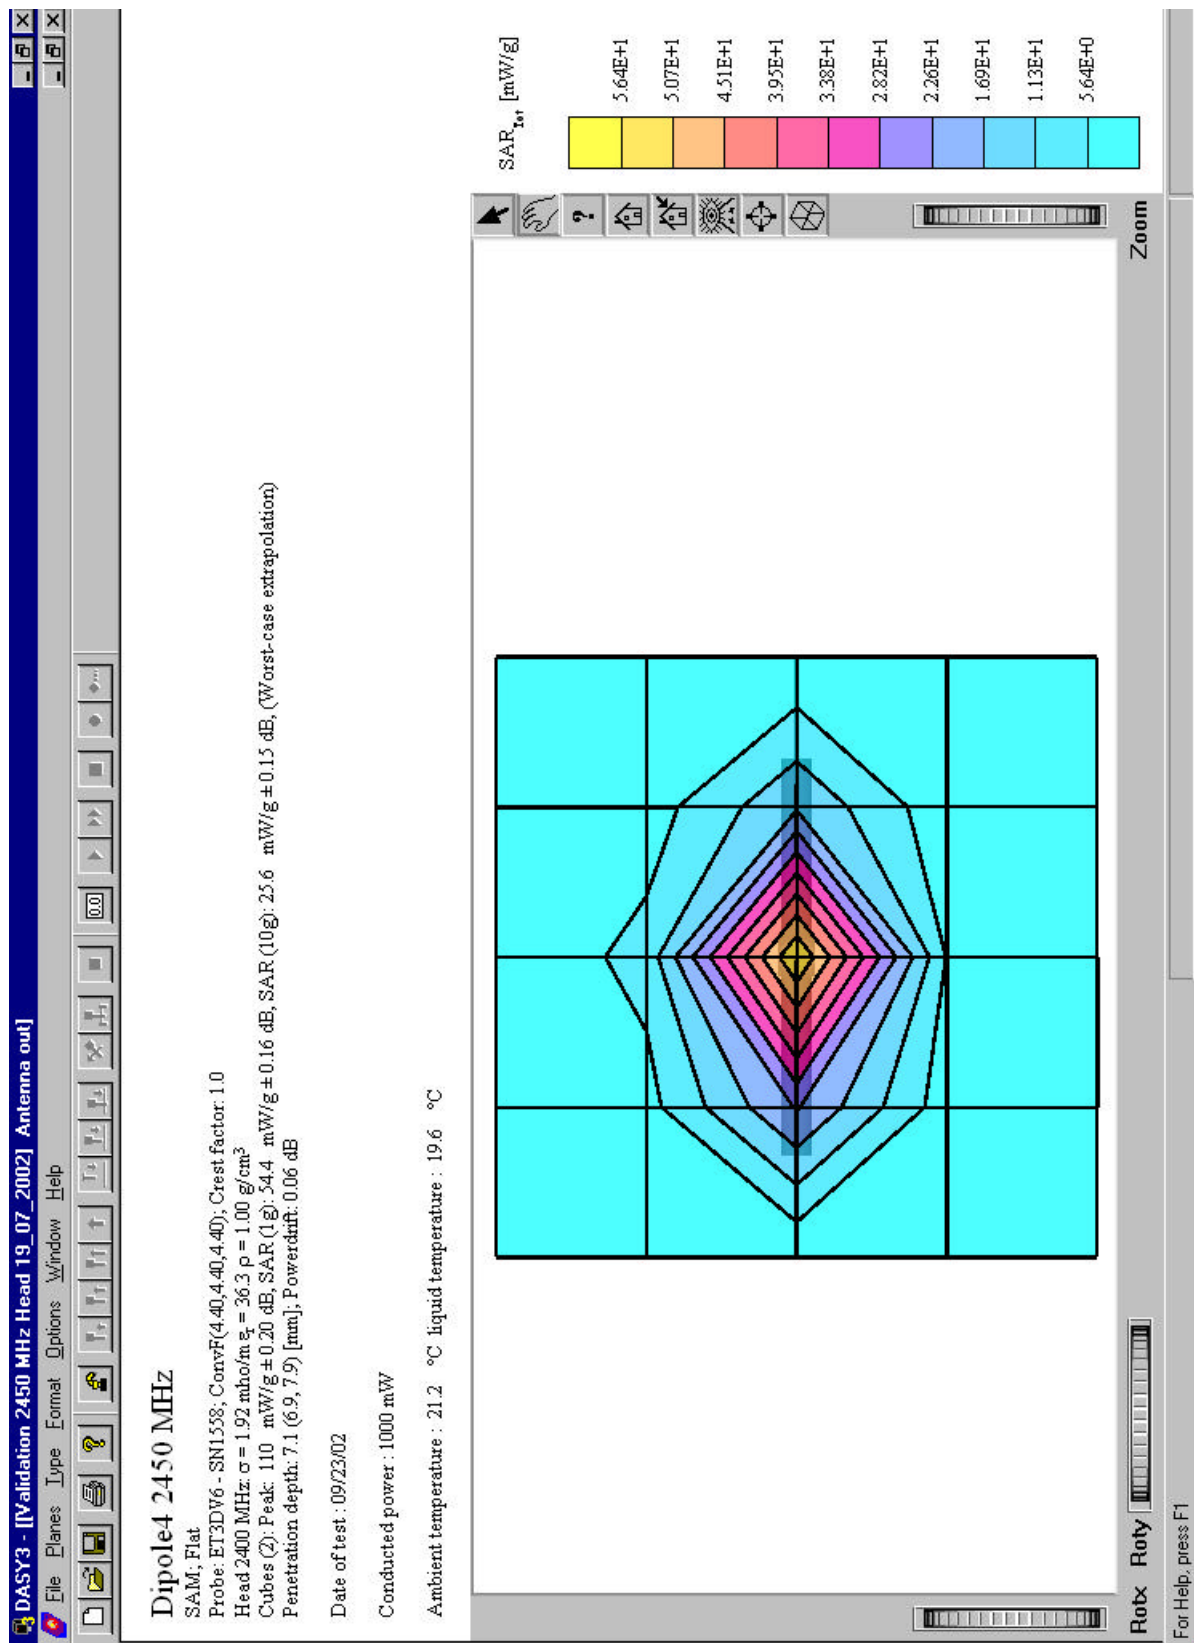



## Annex 2 Measurement results (printout from DASY™)

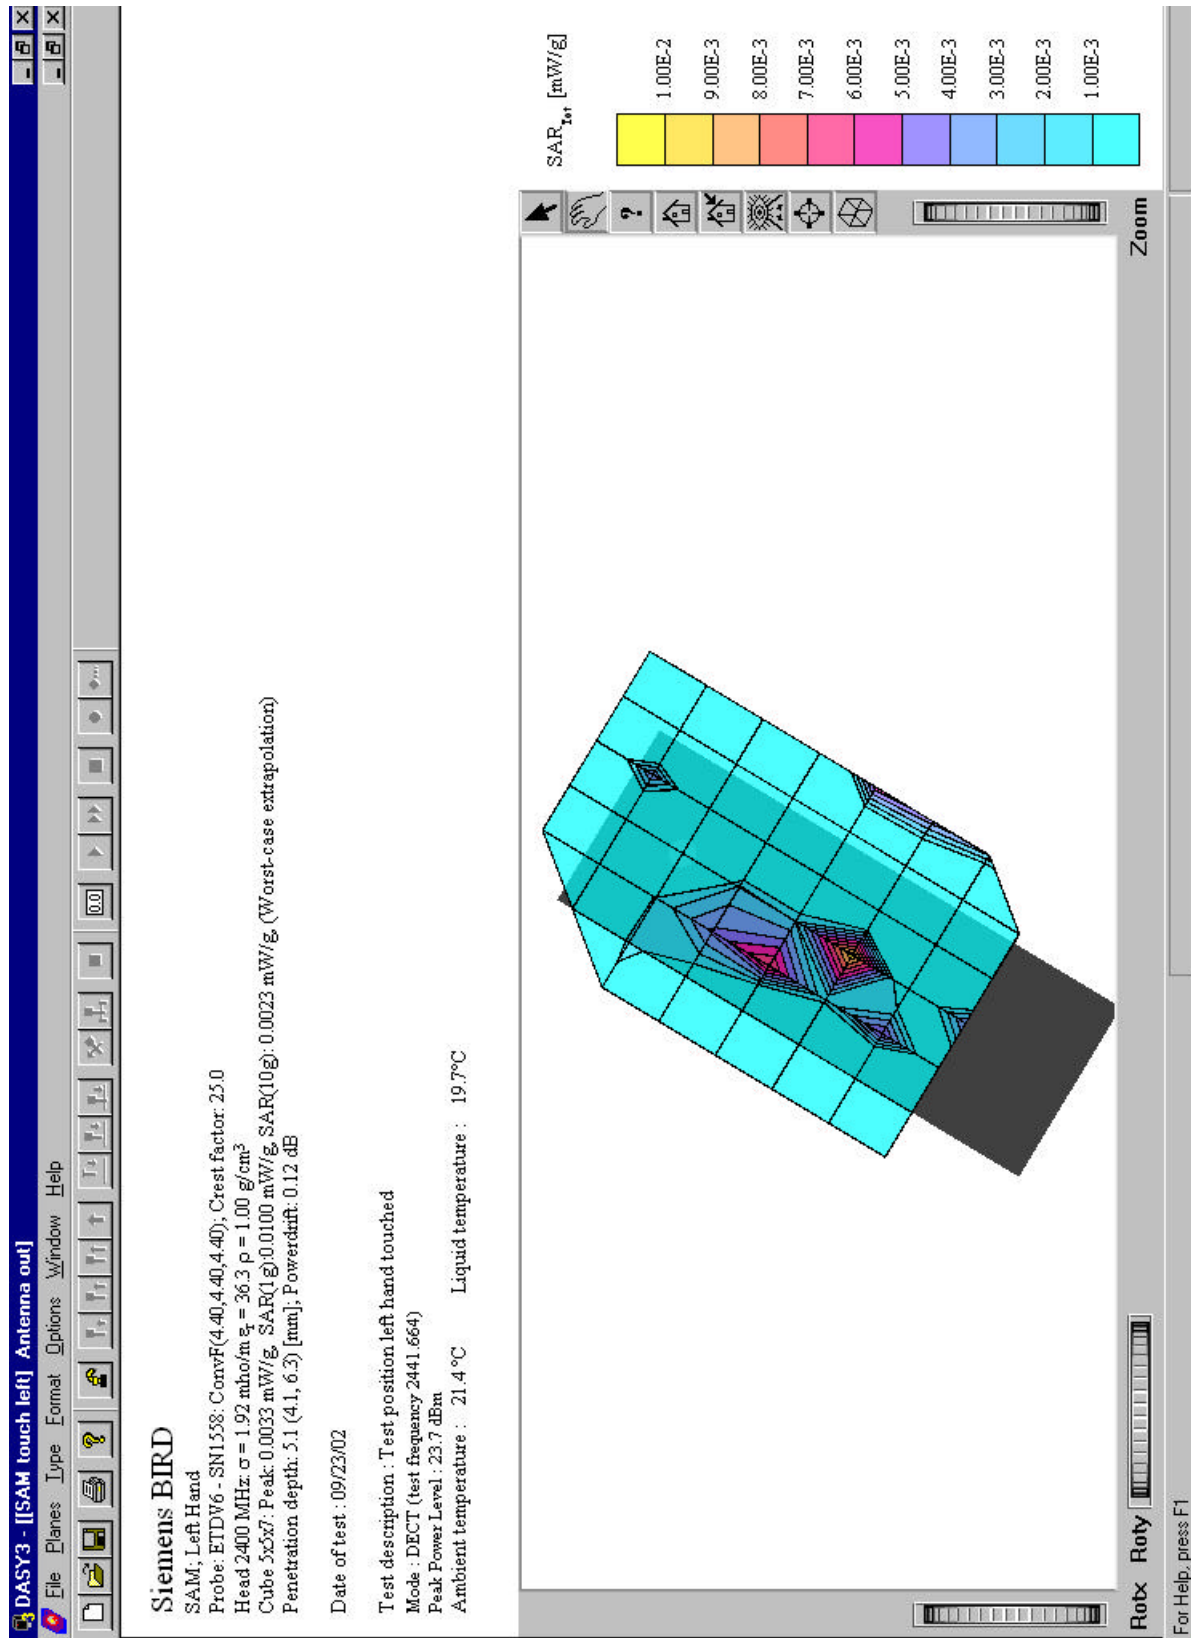

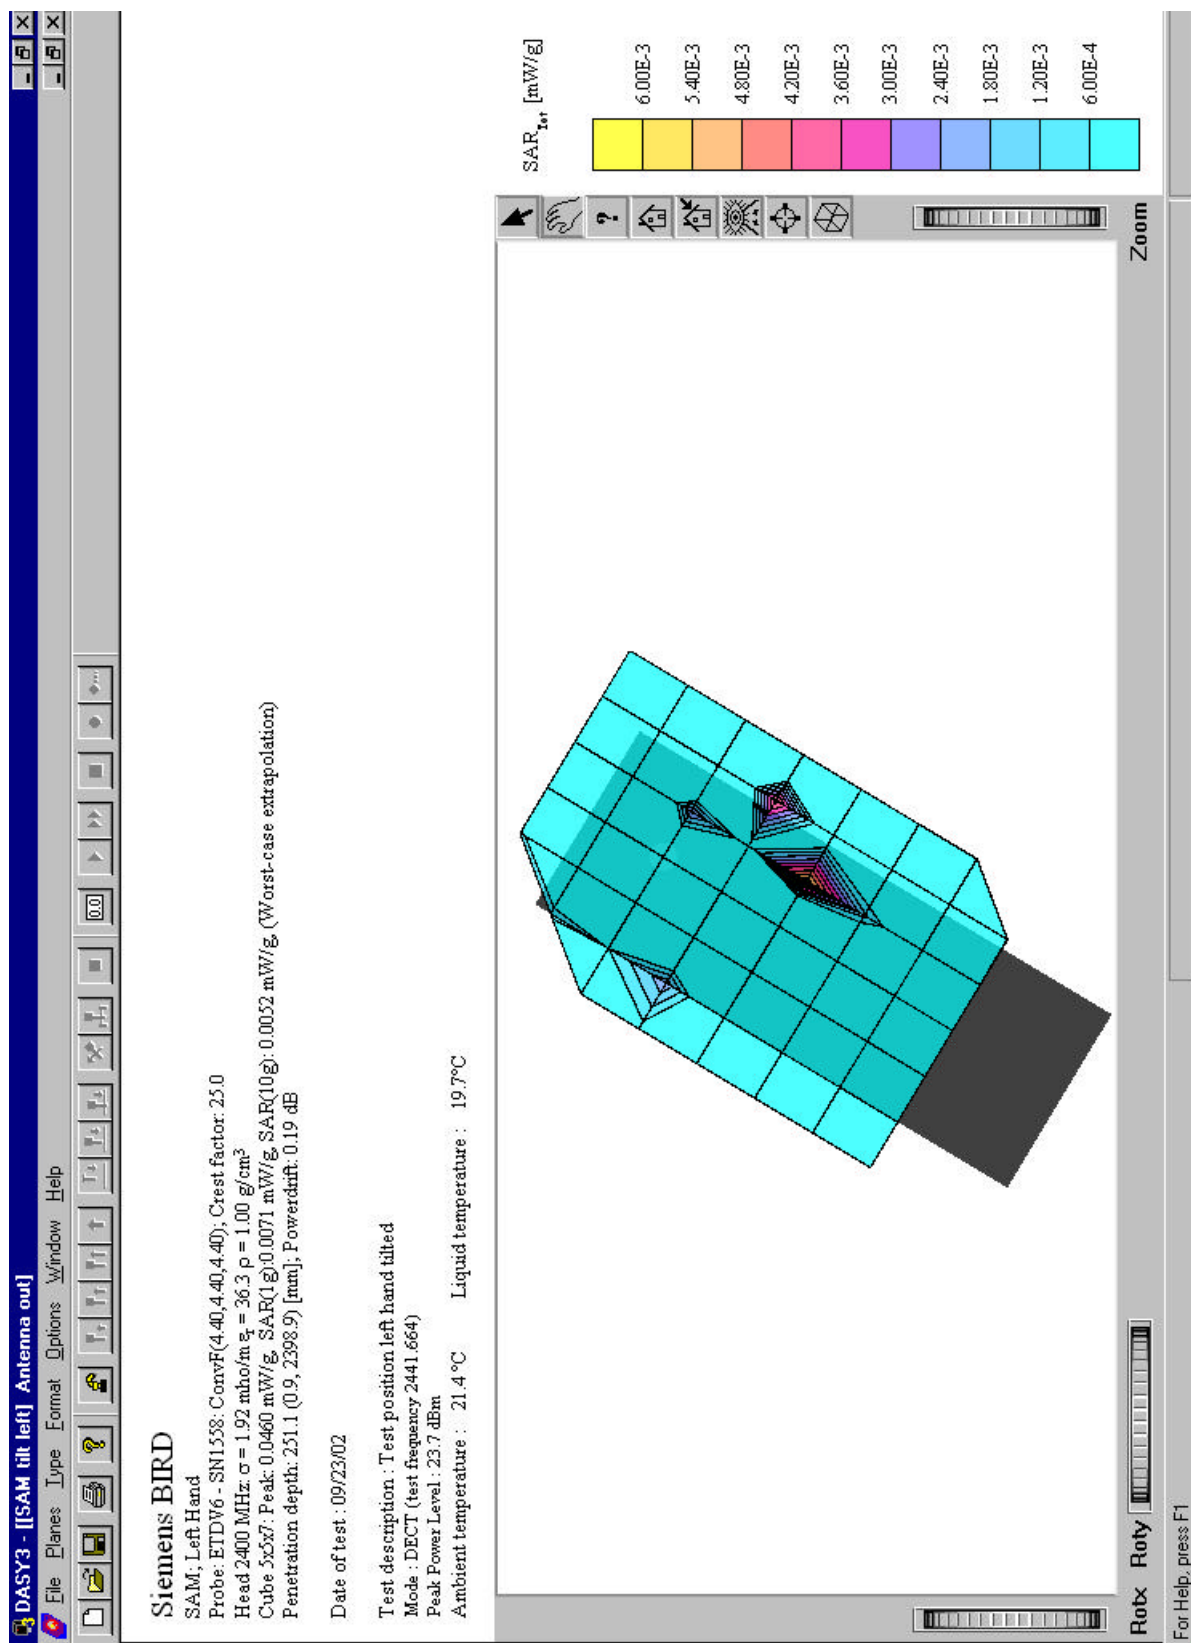





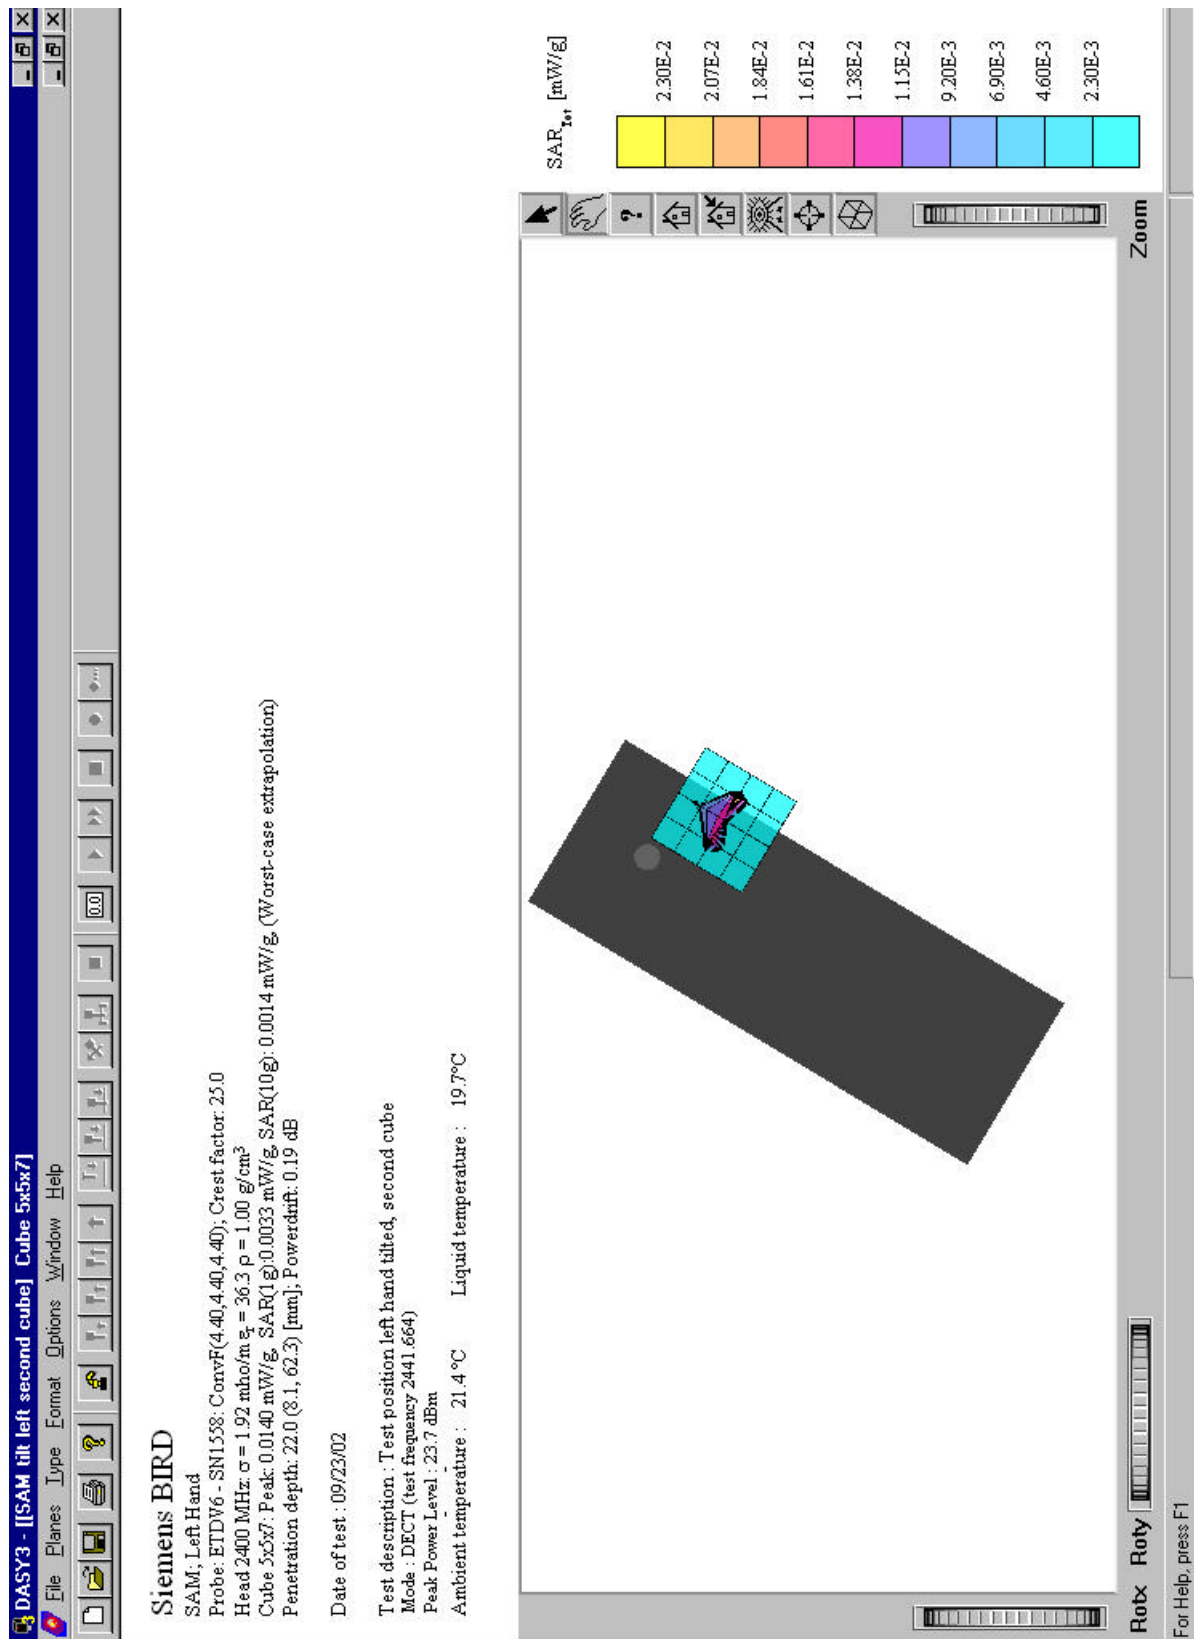


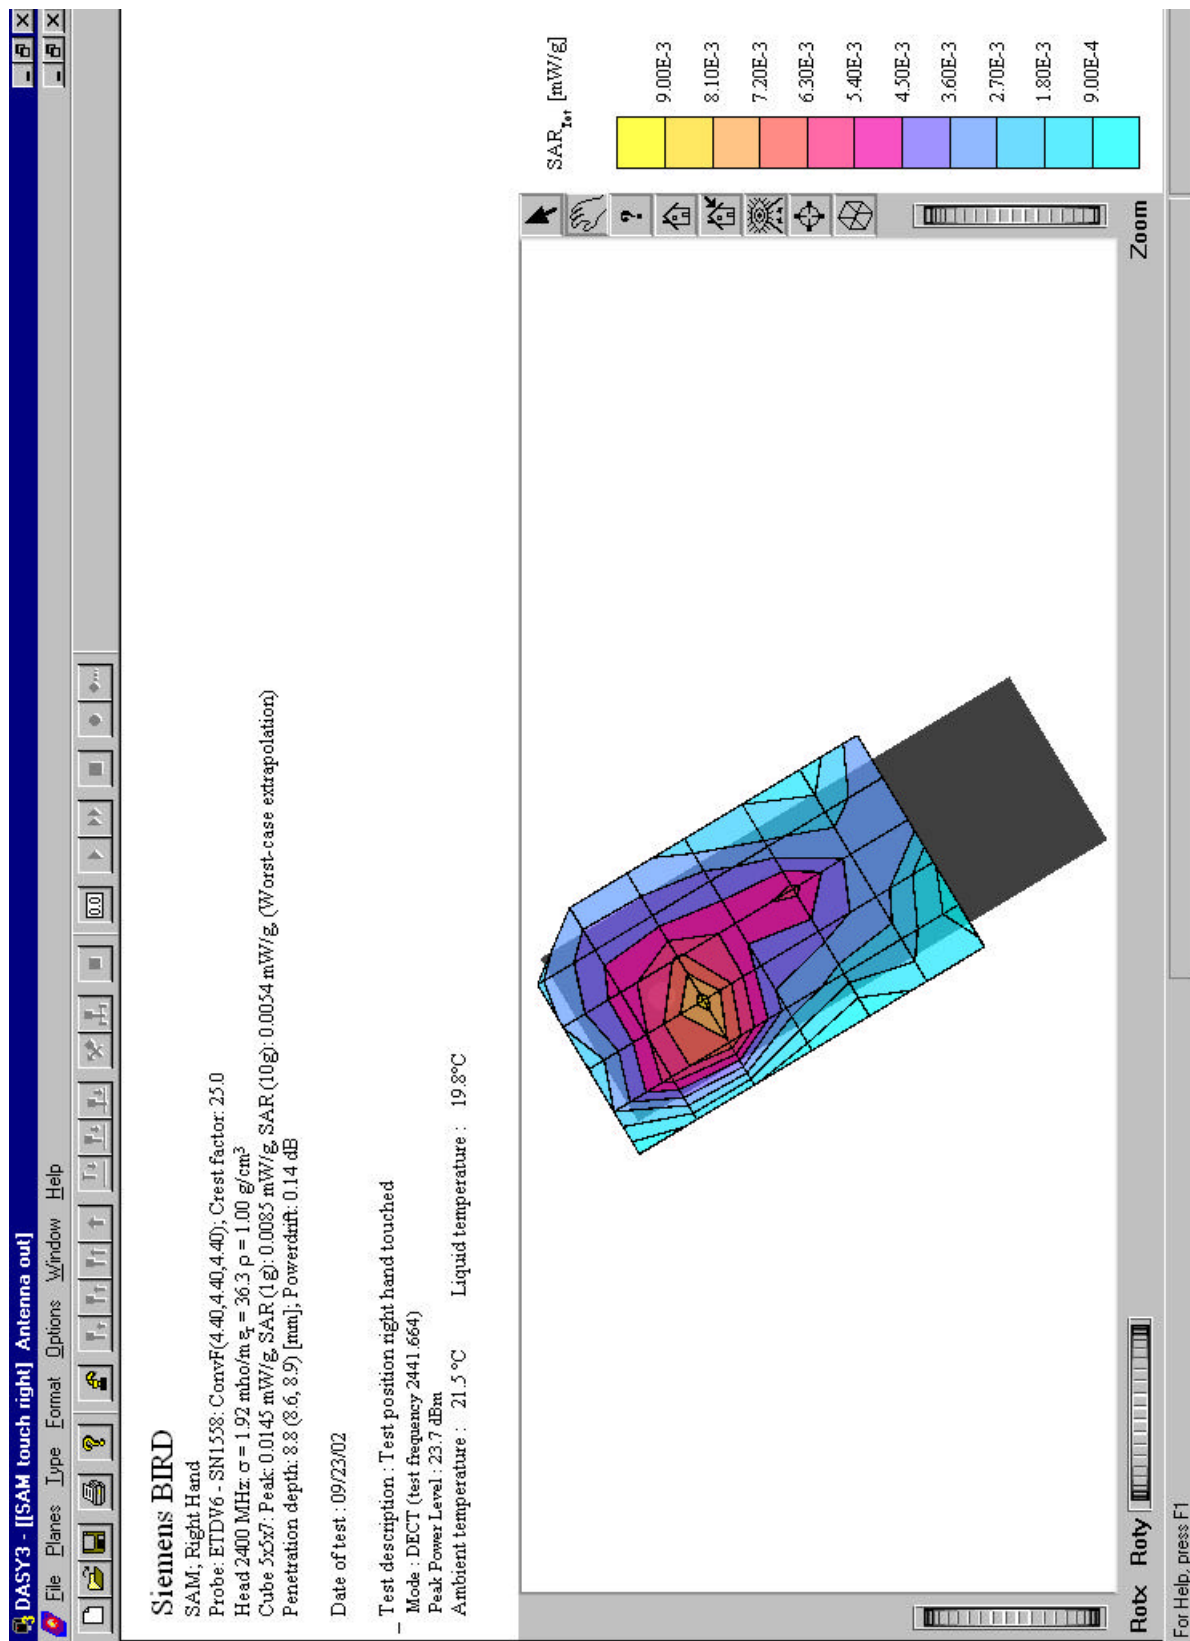



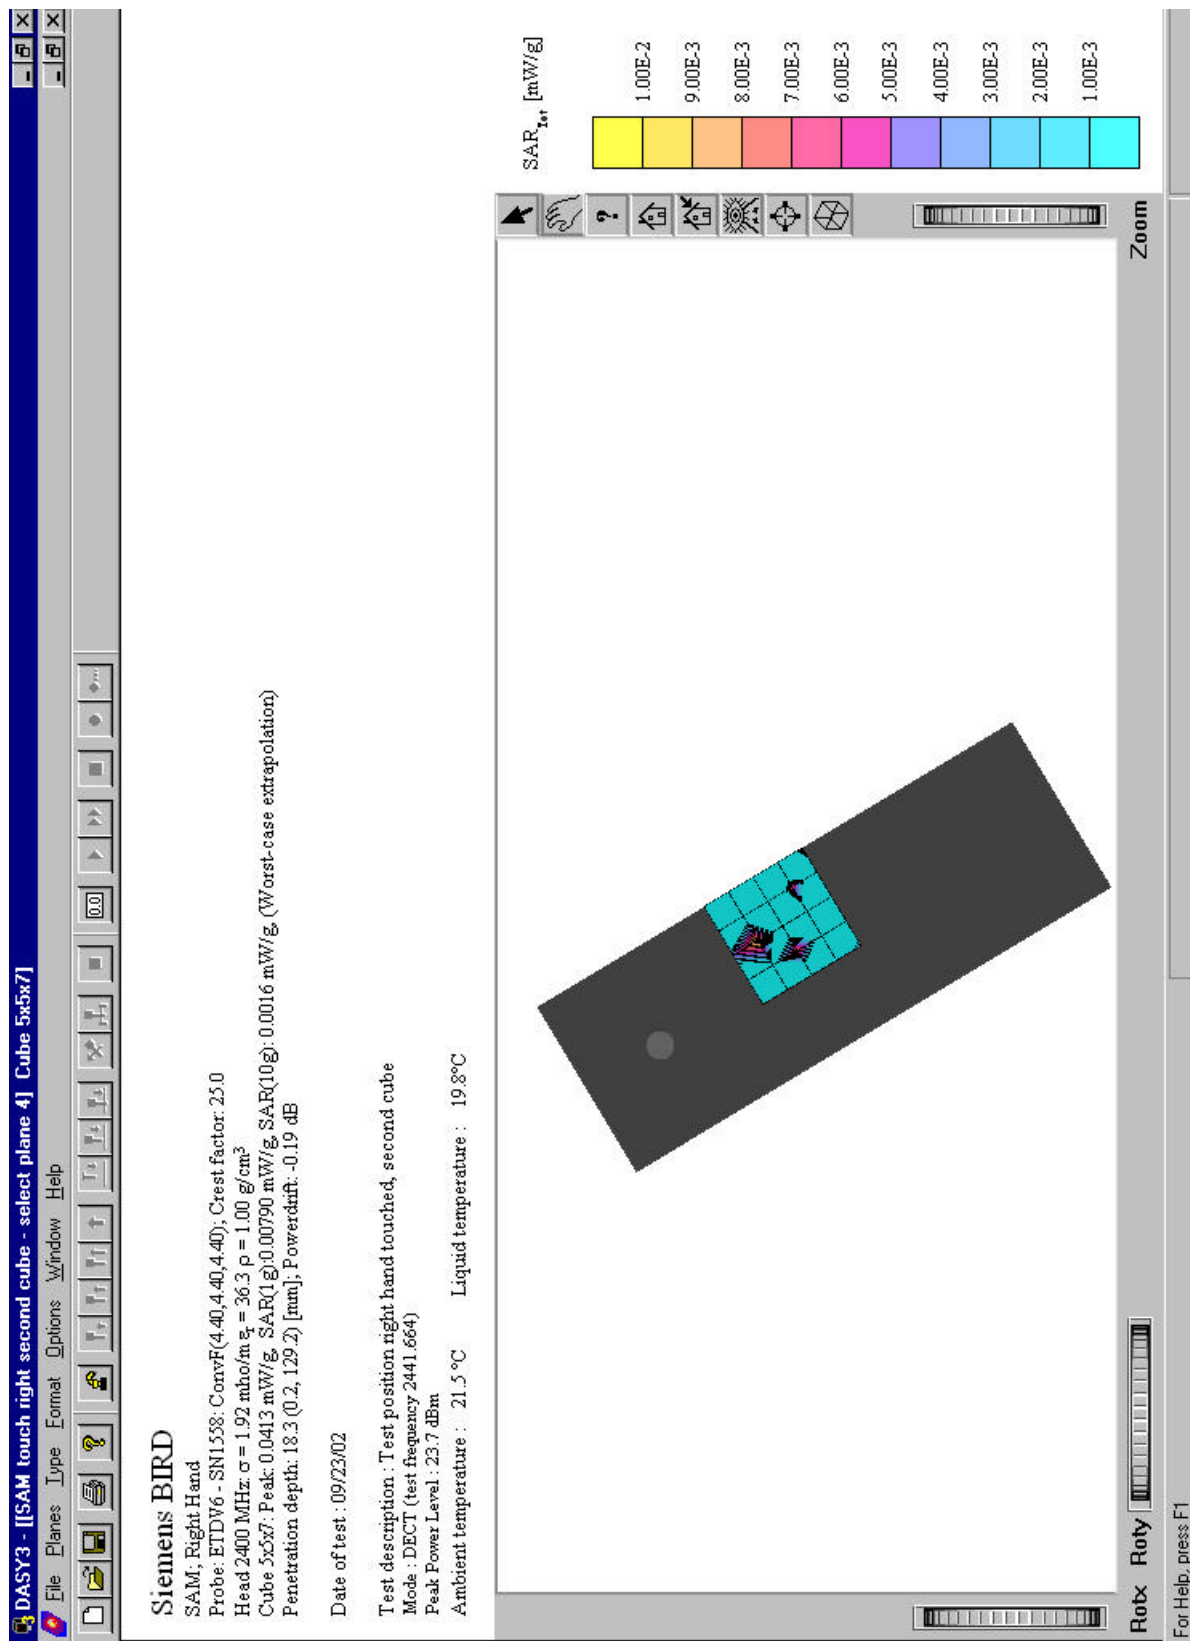

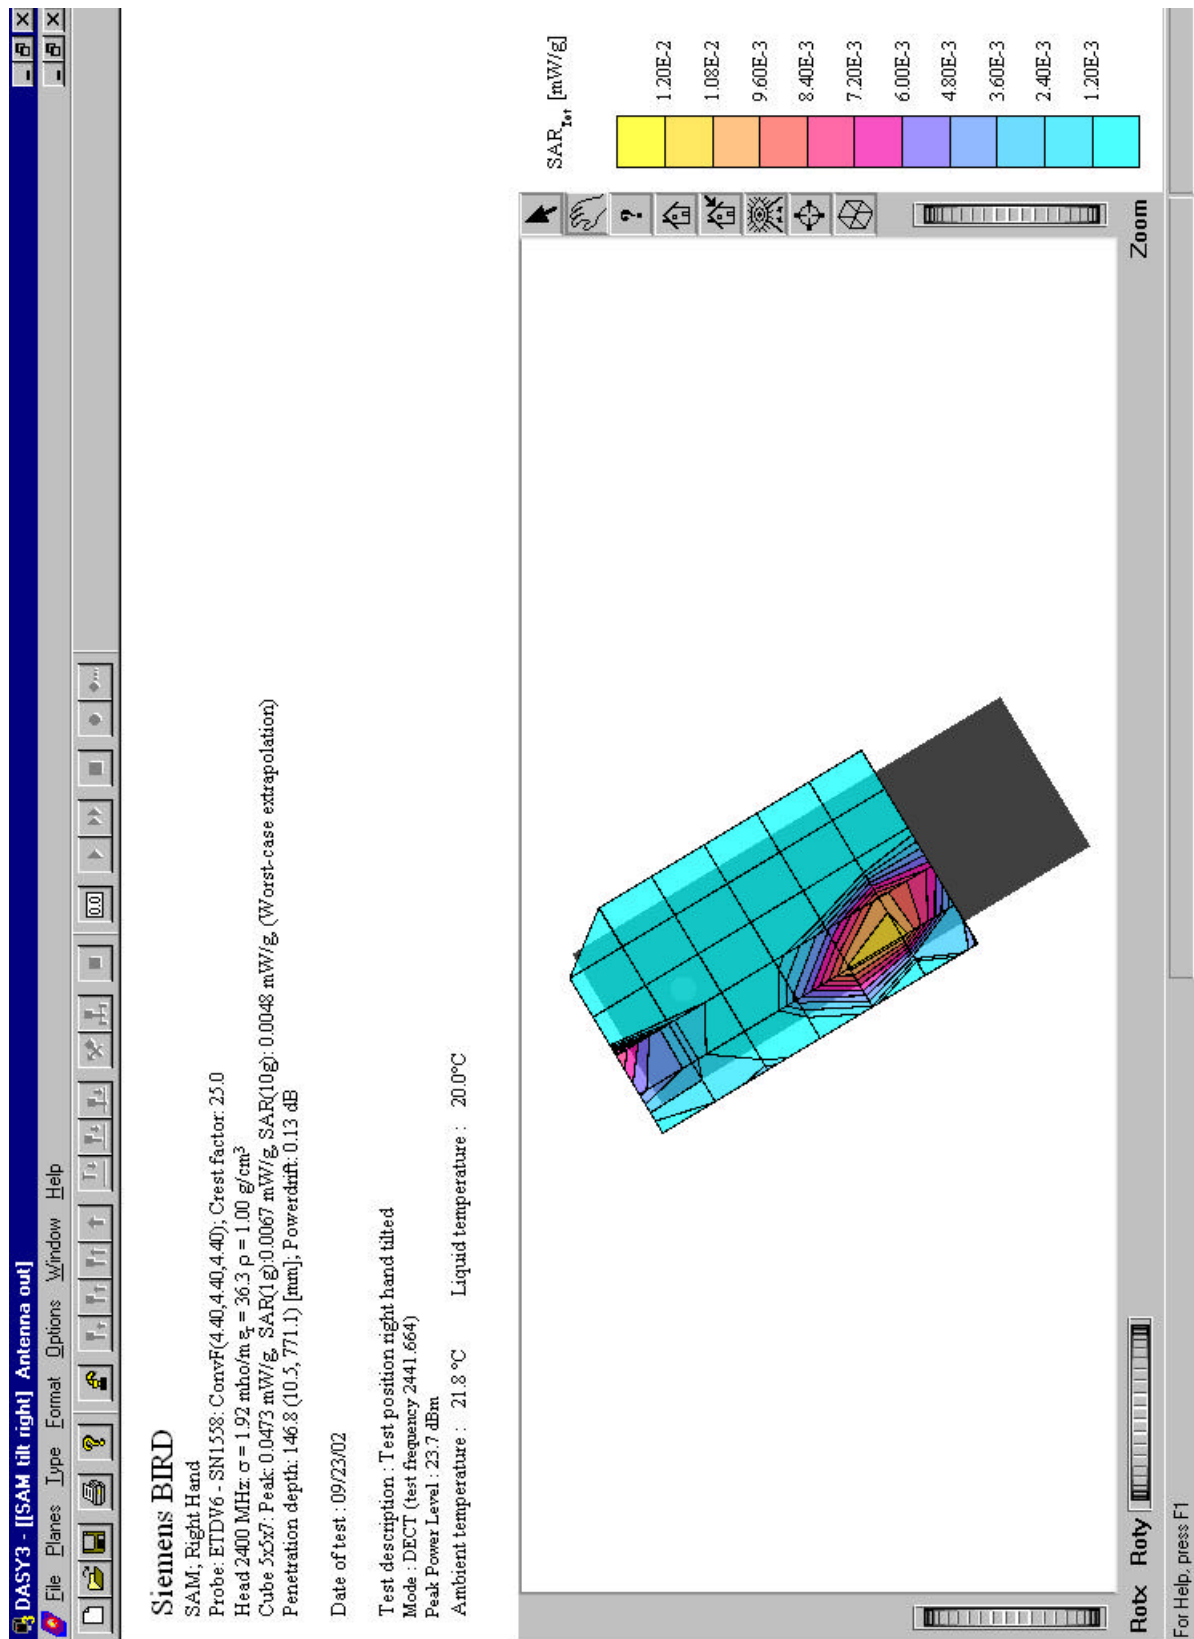

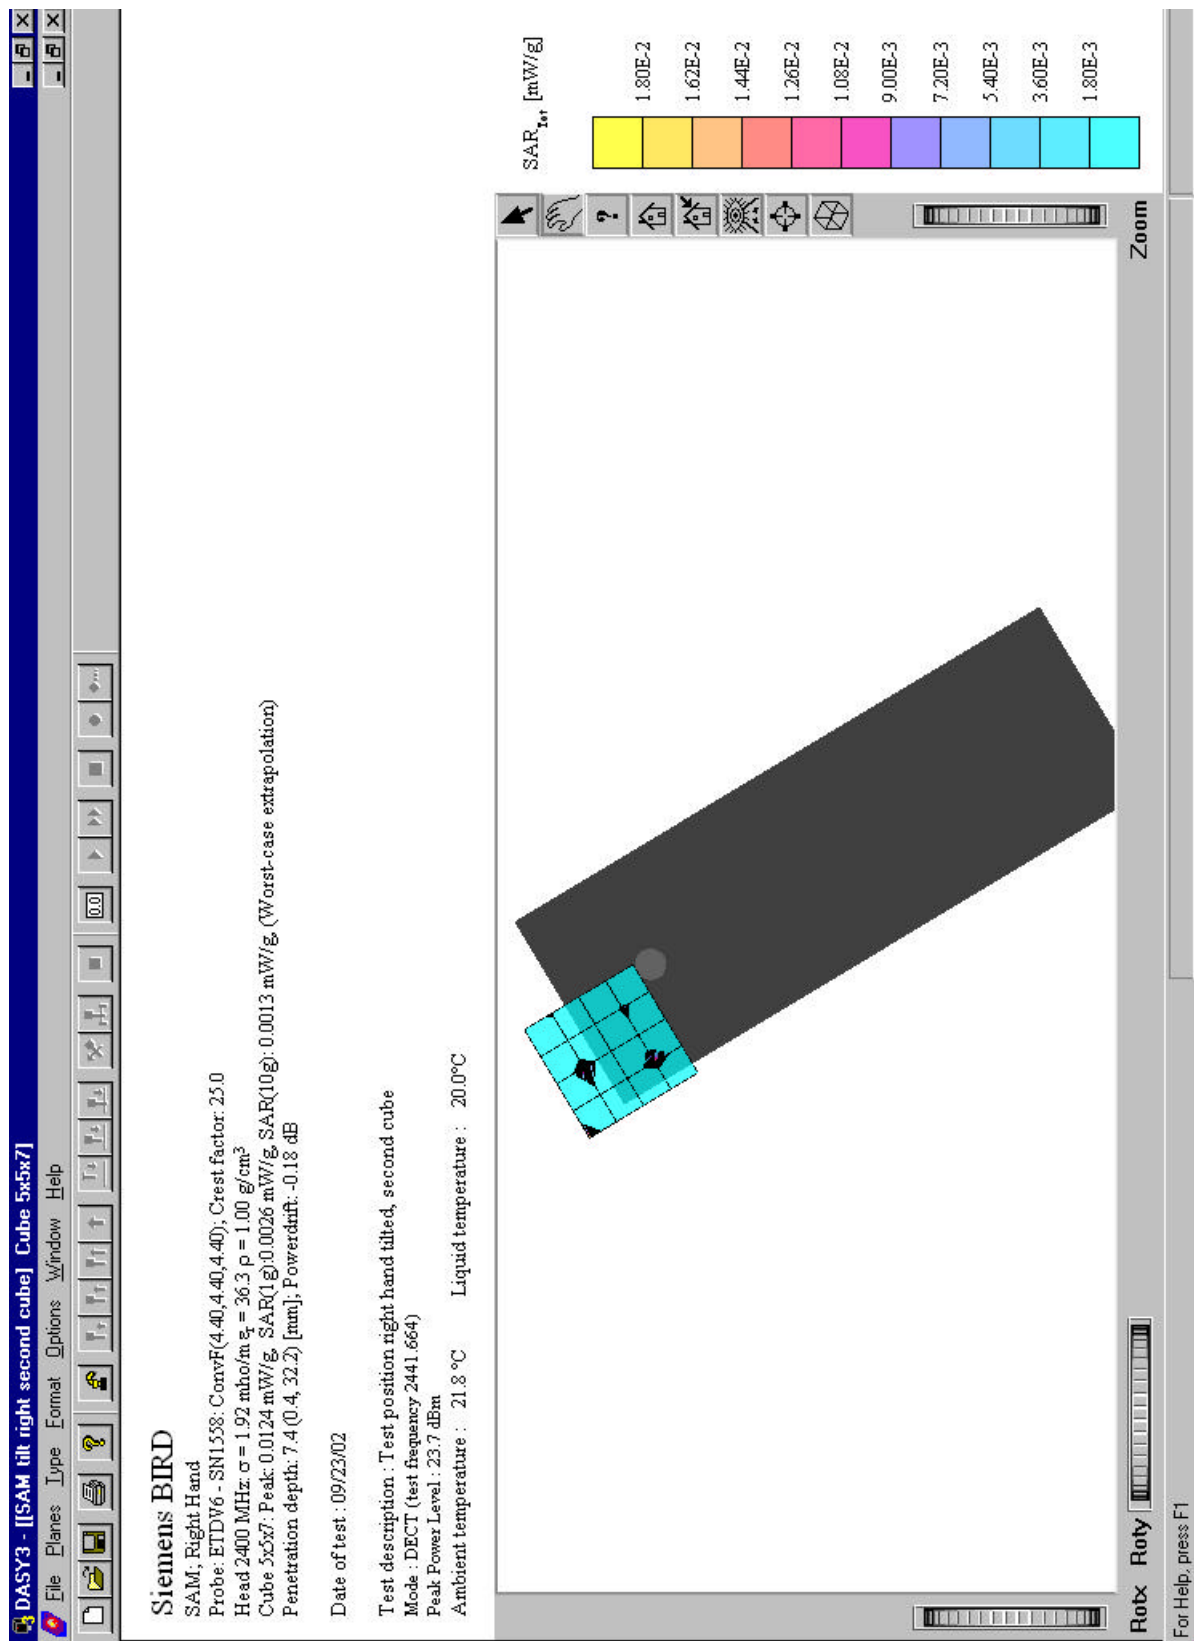

## Annex 3 Photo documentation

### Picture no. 1

Measurement System DASY 3



**Picture no. 2**


Test position touch left side





**Picture no. 3**

Test position touch left side (front view)

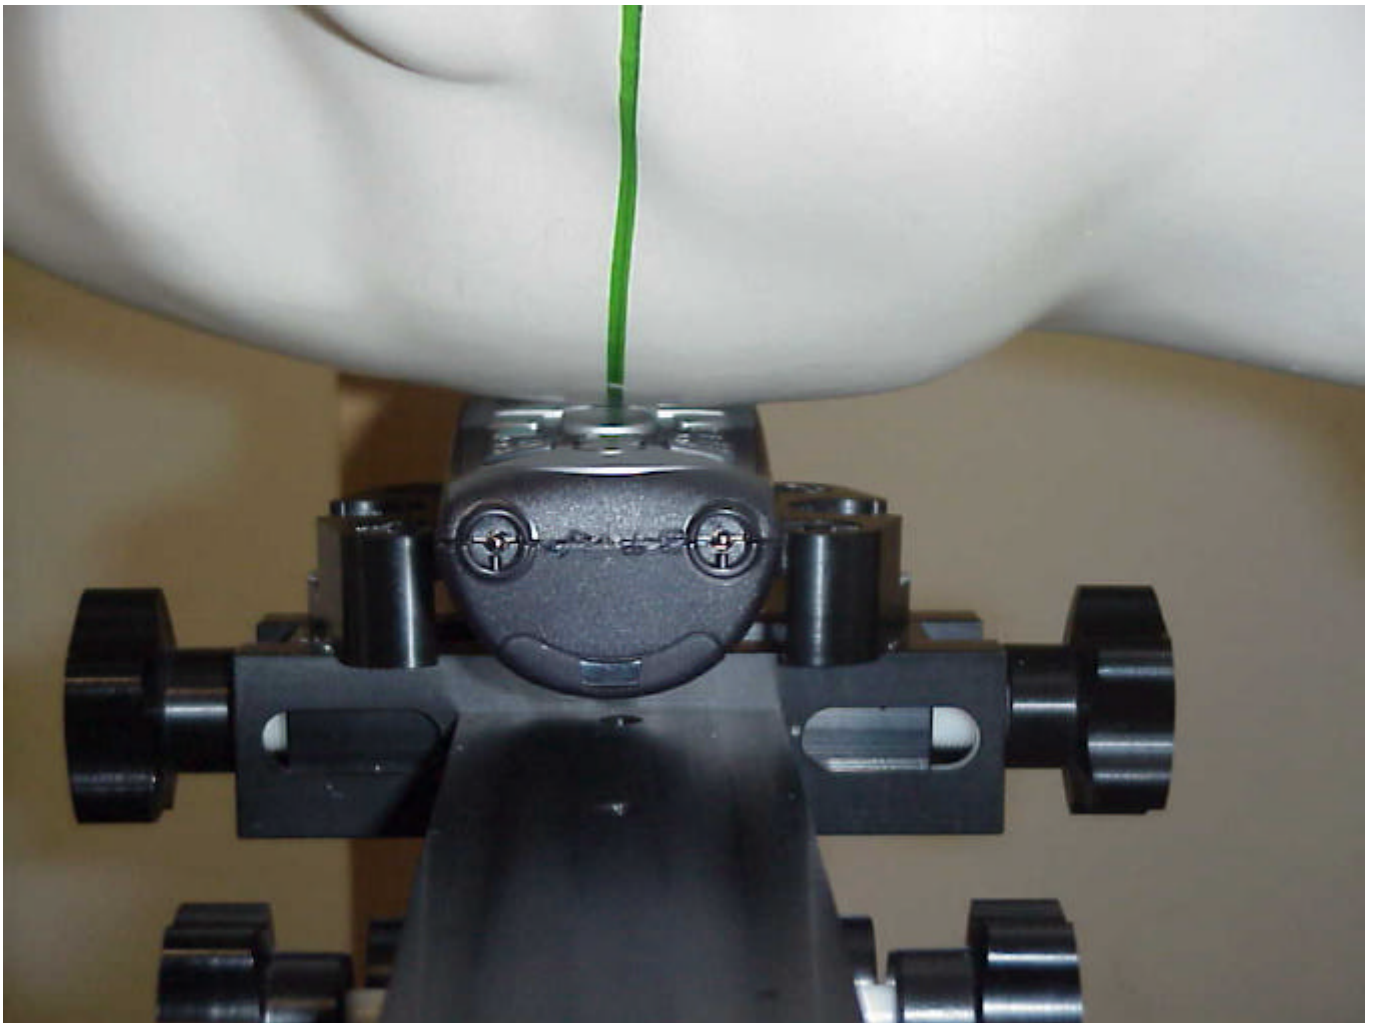

**Picture no. 4**

Test position touch right side



**Picture no. 5**

Test position tilted left side





**Picture no. 6**

Test position tilted left side (front view)



**Picture no. 7**

Test position tilted left side (rear view)



**Picture no. 8**

DUT – front view



**Picture no. 9**

DUT – rear view





**Picture no. 10**

DUT – side view



**Picture no. 11**

DUT – batteries



**Picture no. 12**

Liquid depth





## **Annex 4 Calibration parameters of E-field probe**

**Calibration parameters are described in the additional document**

**‘ Calibration data and Phantom information for test report no. 5-4113/02-1-3’,  
provided together with this document.**