


NORTHWEST EMC

Medtronic Inc.
MyCareLink Monitor, Model 24950B
in Bluetooth Low Energy mode
FCC 15.207:2016
FCC 15.247:2016

Report # MDTR0462.3

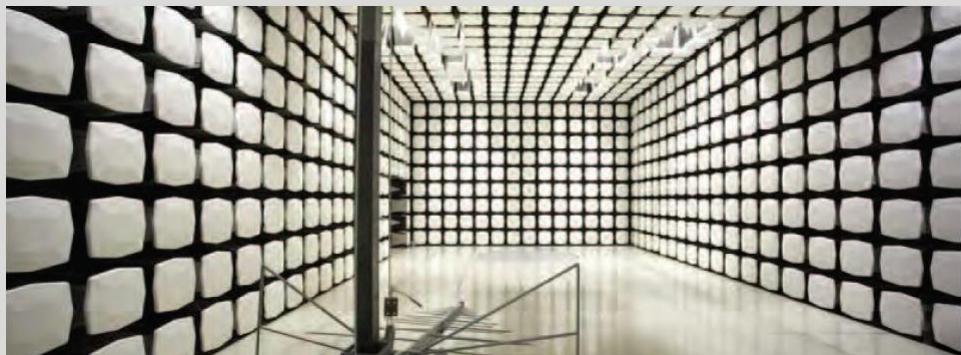

NVLAP Lab Code: 200881-0

This report must not be used to claim product certification, approval, or endorsement by
NVLAP, NIST, or any agency of the federal government of the United States of America.

CERTIFICATE OF TEST

Last Date of Test: May 12, 2016
Medtronic Inc.
Model: MyCareLink Monitor, Model 24950B

Radio Equipment Testing

Standards

Specification	Method
FCC 15.207:2016	ANSI C63.10:2013
FCC 15.247:2016	KDB 558074

Results

Method Clause	Test Description	Applied	Results	Comments
6.2	AC – Powerline Conducted Emissions	Yes	Pass	
6.6, 6.6, 11.12.1, 11.13.2	Spurious Radiated Emissions	Yes	Pass	
11.6	Duty Cycle	Yes	N/A	Characterization of radio
11.8.2	Occupied Bandwidth	Yes	Pass	
11.9.2.2.4	Output Power	Yes	Pass	
11.10.2	Power Spectral Density	Yes	Pass	
11.11	Band Edge Compliance	Yes	Pass	
11.11	Spurious Conducted Emissions	Yes	Pass	

Deviations From Test Standards

None

Approved By:



Tim O'Shea, Operations Manager

Product compliance is the responsibility of the client; therefore, the tests and equipment modes of operation represented in this report were agreed upon by the client, prior to testing. The results of this test pertain only to the sample(s) tested. The specific description is noted in each of the individual sections of the test report supporting this certificate of test. This report reflects only those tests from the referenced standards shown in the certificate of test. It does not include inspection or verification of labels, identification, marking or user information.

REVISION HISTORY

Revision Number	Description	Date	Page Number
00	None		

ACCREDITATIONS AND AUTHORIZATIONS

United States

FCC - Designated by the FCC as a Telecommunications Certification Body (TCB). Certification chambers, Open Area Test Sites, and conducted measurement facilities are listed with the FCC.

A2LA - Accredited by A2LA to ISO / IEC 17065 as a product certifier. This allows Northwest EMC to certify transmitters to FCC and IC specifications.

NVLAP - Each laboratory is accredited by NVLAP to ISO 17025

Canada

IC - Recognized by Industry Canada as a Certification Body (CB). Certification chambers and Open Area Test Sites are filed with IC.

European Union

European Commission – Validated by the European Commission as a Notified Body under the R&TTE Directive.

Australia/New Zealand

ACMA - Recognized by ACMA as a CAB for the acceptance of test data.

Korea

MSIP / RRA - Recognized by KCC's RRA as a CAB for the acceptance of test data.

Japan

VCCI - Associate Member of the VCCI. Conducted and radiated measurement facilities are registered.

Taiwan

BSMI – Recognized by BSMI as a CAB for the acceptance of test data.

NCC - Recognized by NCC as a CAB for the acceptance of test data.

Singapore

IDA – Recognized by IDA as a CAB for the acceptance of test data.

Israel

MOC – Recognized by MOC as a CAB for the acceptance of test data.

Hong Kong

OFCA – Recognized by OFCA as a CAB for the acceptance of test data.

Vietnam

MIC – Recognized by MIC as a CAB for the acceptance of test data.

SCOPE

For details on the Scopes of our Accreditations, please visit:

<http://www.nwemc.com/accreditations/>

<http://gsi.nist.gov/global/docs/cabs/designations.html>

MEASUREMENT UNCERTAINTY

Measurement Uncertainty

When a measurement is made, the result will be different from the true or theoretically correct value. The difference is the result of tolerances in the measurement system that cannot be completely eliminated. To the extent that technology allows us, it has been our aim to minimize this error. Measurement uncertainty is a statistical expression of measurement error qualified by a probability distribution.

A measurement uncertainty estimation has been performed for each test per our internal quality document WP 342. The estimation is used to compare the measured result with its "true" or theoretically correct value. The expanded measurement uncertainty (K=2) for each test is on each data sheet. Our measurement data meets or exceeds the measurement uncertainty requirements of the applicable specification; therefore, the test data can be compared directly to the specification limit to determine compliance. The calculations for estimating measurement uncertainty are based upon ETSI TR 100 028 (or CISPR 16-4-2 as applicable), and are available upon request.


The following table represents the Measurement Uncertainty (MU) budgets for each of the tests that may be contained in this report.

Test	+ MU	- MU
Frequency Accuracy (Hz)	0.0007%	-0.0007%
Amplitude Accuracy (dB)	1.2 dB	-1.2 dB
Conducted Power (dB)	0.3 dB	-0.3 dB
Radiated Power via Substitution (dB)	0.7 dB	-0.7 dB
Temperature (degrees C)	0.7°C	-0.7°C
Humidity (% RH)	2.5% RH	-2.5% RH
Voltage (AC)	1.0%	-1.0%
Voltage (DC)	0.7%	-0.7%
Field Strength (dB)	5.2 dB	-5.2 dB
AC Powerline Conducted Emissions (dB)	2.4 dB	-2.4 dB

FACILITIES



California	Minnesota	New York	Oregon	Texas	Washington
Labs OC01-13 41 Tesla Irvine, CA 92618 (949) 861-8918	Labs MN01-08, MN10 9349 W Broadway Ave. Brooklyn Park, MN 55445 (612)-638-5136	Labs NY01-04 4939 Jordan Rd. Elbridge, NY 13060 (315) 554-8214	Labs EV01-12 22975 NW Evergreen Pkwy Hillsboro, OR 97124 (503) 844-4066	Labs TX01-09 3801 E Plano Pkwy Plano, TX 75074 (469) 304-5255	Labs NC01-05 19201 120 th Ave NE Bothell, WA 98011 (425)984-6600
NVLAP					
NVLAP Lab Code: 200676-0	NVLAP Lab Code: 200881-0	NVLAP Lab Code: 200761-0	NVLAP Lab Code: 200630-0	NVLAP Lab Code: 201049-0	NVLAP Lab Code: 200629-0
Industry Canada					
2834B-1, 2834B-3	2834E-1	N/A	2834D-1, 2834D-2	2834G-1	2834F-1
BSMI					
SL2-IN-E-1154R	SL2-IN-E-1152R	N/A	SL2-IN-E-1017	SL2-IN-E-1158R	SL2-IN-E-1153R
VCCI					
A-0029	A-0109	N/A	A-0108	A-0201	A-0110
Recognized Phase I CAB for ACMA, BSMI, IDA, KCC/RRA, MIC, MOC, NCC, OFCA					
US0158	US0175	N/A	US0017	US0191	US0157

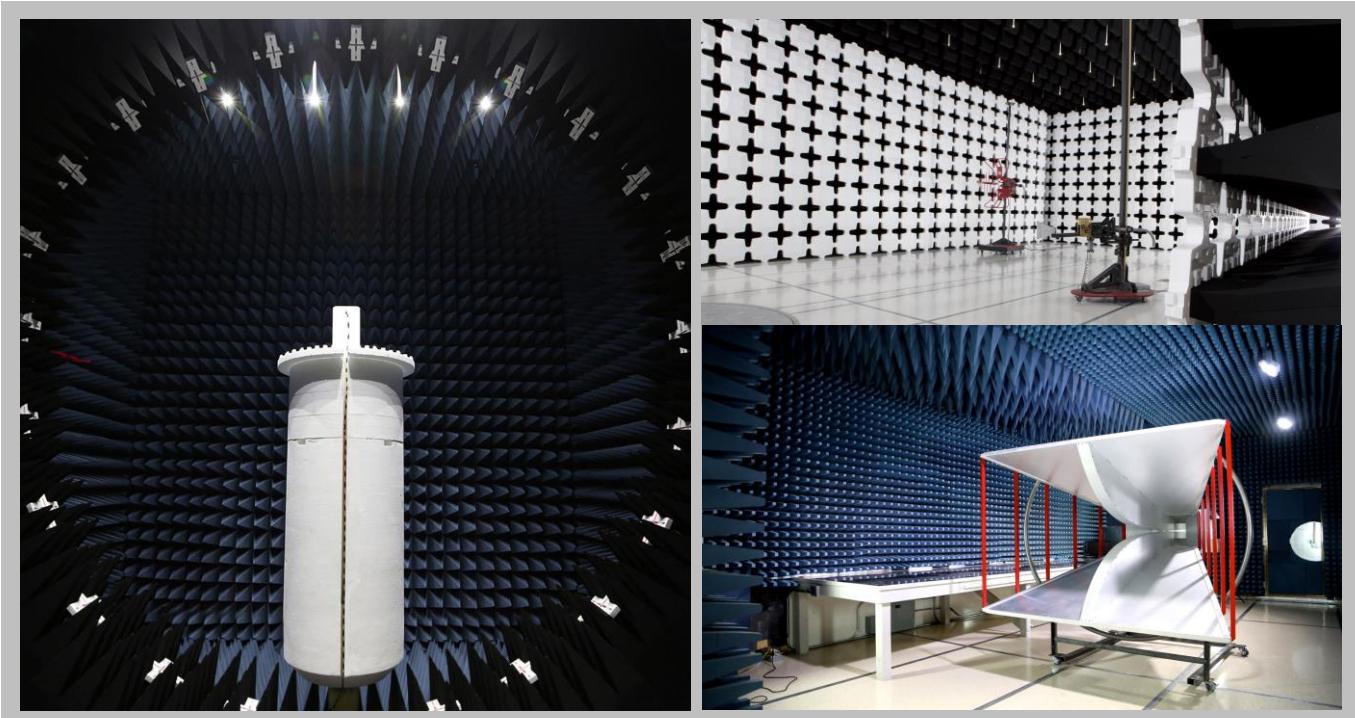

PRODUCT DESCRIPTION

Client and Equipment Under Test (EUT) Information

Company Name:	Medtronic Inc.
Address:	710 Medtronic Parkway
City, State, Zip:	Minneapolis, MN 55432
Test Requested By:	Joel Peltier
Model:	MyCareLink Monitor, Model 24950B
First Date of Test:	April 29, 2016
Last Date of Test:	May 12, 2016
Receipt Date of Samples:	April 29, 2016
Equipment Design Stage:	Production
Equipment Condition:	No Damage

Information Provided by the Party Requesting the Test

Functional Description of the EUT:

The MyCareLink Monitor, Model 24950B, is a Medical instrument designed for remote monitoring of Medtronic implantable medical devices. The MyCareLink Monitor is made up of a base unit and a handset. The MyCareLink Monitor design is being updated to incorporate a Bluetooth (BT) module that will support BT Low Energy (BLE) functionality in the base unit in order to support wireless communication with implanted cardiac devices over a BLE link. Communication between the handset and the base unit is accomplished via BT Classic. The MICS/MEDS radio module design and its associated circuitry as well as the RF Head design remains unchanged.

Testing Objective:

To demonstrate compliance of the Bluetooth Low Energy radio to FCC 15.247 requirements.

CONFIGURATIONS

Configuration MDTR0462- 1

EUT					
Description	Manufacturer	Model/Part Number	Serial Number		
Base Unit	Medtronic	24950	BTL000088A		
Power Supply (5VDC)	BridgePower Corp	M950550A010	1		

Peripherals in test setup boundary					
Description	Manufacturer	Model/Part Number	Serial Number		
POTS Analog Modem	Radicom Research Inc	V95HU-E2-MD	0003691		

Remote Equipment Outside of Test Setup Boundary					
Description	Manufacturer	Model/Part Number	Serial Number		
RF Head 1	Medtronic	24955	RFH549396A		

Cables					
Cable Type	Shield	Length (m)	Ferrite	Connection 1	Connection 2
Power Supply Cable	No	2.0m	Yes	Power Supply	Base Unit
Analog Phone Cable	No	2.1m	No	POTS Analog Modem	Unterminated
USB Cable	Yes	0.15m	No	Base Unit	POTS Analog Modem

Configuration MDTR0462- 3

EUT					
Description	Manufacturer	Model/Part Number	Serial Number		
Base Unit	Medtronic	24950	BTL000088A		
Power Supply (5VDC)	BridgePower Corp	M950550A010	1		

Peripherals in test setup boundary					
Description	Manufacturer	Model/Part Number	Serial Number		
Laptop	Dell	Latitude E6410	7KKGKYN1		
AC Adapter (Laptop)	Dell	LA90PM111	CN-0Y4M8K-72438-38R-C8D9-A01		

Cables					
Cable Type	Shield	Length (m)	Ferrite	Connection 1	Connection 2
Power Supply Cable	No	2.0m	Yes	Power Supply	Base Unit
U.FL to SMA Cable	Yes	0.2m	No	Base Unit	Measurement Equipment (AAX, TIK, MNU, AMI, RFW)
AC Mains Cable (Laptop)	No	0.9m	No	AC Adapter (Laptop)	AC Mains
DC Cable (Laptop)	No	1.8m	No	AC Adapter (Laptop)	Laptop
USB Cable (Laptop)	Yes	3.1m	No	Laptop	Base Unit

MODIFICATIONS

Equipment Modifications

Item	Date	Test	Modification	Note	Disposition of EUT
1	4/29/2016	Spurious Radiated Emissions	Tested as delivered to Test Station.	No EMI suppression devices were added or modified during this test.	EUT remained at Northwest EMC following the test.
2	5/5/2016	Occupied Bandwidth	Tested as delivered to Test Station.	No EMI suppression devices were added or modified during this test.	EUT remained at Northwest EMC following the test.
3	5/9/2016	Output Power	Tested as delivered to Test Station.	No EMI suppression devices were added or modified during this test.	EUT remained at Northwest EMC following the test.
4	5/9/2016	Power Spectral Density	Tested as delivered to Test Station.	No EMI suppression devices were added or modified during this test.	EUT remained at Northwest EMC following the test.
5	5/9/2016	Band Edge Compliance	Tested as delivered to Test Station.	No EMI suppression devices were added or modified during this test.	EUT remained at Northwest EMC following the test.
6	5/9/2016	Spurious Conducted Emissions	Tested as delivered to Test Station.	No EMI suppression devices were added or modified during this test.	EUT remained at Northwest EMC following the test.
7	5/12/2016	AC – Powerline Conducted Emissions	Tested as delivered to Test Station.	No EMI suppression devices were added or modified during this test.	Scheduled testing was completed.

DUTY CYCLE

TEST DESCRIPTION

The Duty Cycle (x) were measured for each of the EUT operating modes. The measurements were made using a zero span on the spectrum analyzer to see the pulses in the time domain. The transmit power was set to its default maximum. A direct connection was made between the RF output of the EUT and a spectrum analyzer. Attenuation and a DC block were used.

The duty cycle was calculated by dividing the transmission pulse duration (T) by the total period of a single on and total off time.

The EUT operates at 100% Duty Cycle.

OCCUPIED BANDWIDTH

Testing was performed using the mode(s) of operation and configuration(s) noted within the report. The individuals and/or the organization requesting the test provided the modes, configurations and settings used to complete the evaluation. The actual test parameters are specified in the test data, this includes items such as investigated frequency range (scanned) and test levels. The testing methods and performance specifications, as well as the test site used for the evaluation are indicated in the test data.

TEST EQUIPMENT

Description	Manufacturer	Model	ID	Last Cal.	Interval (mo)
Attenuator	S.M. Electronics	SA26B-20	RFW	2/26/2016	12
Block - DC	Fairview Microwave	SD3379	AMI	9/18/2015	12
Cable	ESM Cable Corp.	TTBJ141 KMKM-72	MNU	9/18/2015	12
Generator - Signal	Agilent	N5183A	TIK	10/17/2014	36
Analyzer - Spectrum Analyzer	Agilent	E4440A	AAX	3/24/2016	12

TEST DESCRIPTION

The 6dB occupied bandwidth was measured using 100 kHz resolution bandwidth and 300 kHz video bandwidth.

The EUT was set to the channels and modes listed in the datasheet. The measurement was made using a direct connection between the RF output of the EUT and the spectrum analyzer.


OCCUPIED BANDWIDTH

EUT:	MyCareLink Monitor, Model 24950B		Work Order:	MDTR0462	
Serial Number:	BTL.000088A		Date:	05/05/16	
Customer:	Medtronic Inc.		Temperature:	23.2°C	
Attendees:	Nick Blake		Humidity:	25%	
Project:	None		Barometric Pres.:	988.5	
Tested by:	Dustin Sparks, Trevor Buls	Power:	5VDC	Job Site:	MN05
TEST SPECIFICATIONS			Test Method		
FCC 15.247:2016			ANSI C63.10:2013		
COMMENTS					
None					
DEVIATIONS FROM TEST STANDARD					
None					
Configuration #	3	Signature			
			Value	Limit (±)	Result
			688.097 kHz	500 kHz	Pass
			669.564 kHz	500 kHz	Pass
			693.773 kHz	500 kHz	Pass


BLE/GFSK Low Channel, 2402 MHz
BLE/GFSK Mid Channel, 2442 MHz
BLE/GFSK High Channel, 2480 MHz

OCCUPIED BANDWIDTH


BLE/GFSK Low Channel, 2402 MHz			Value	Limit (≥)	Result
			688.097 kHz	500 kHz	Pass

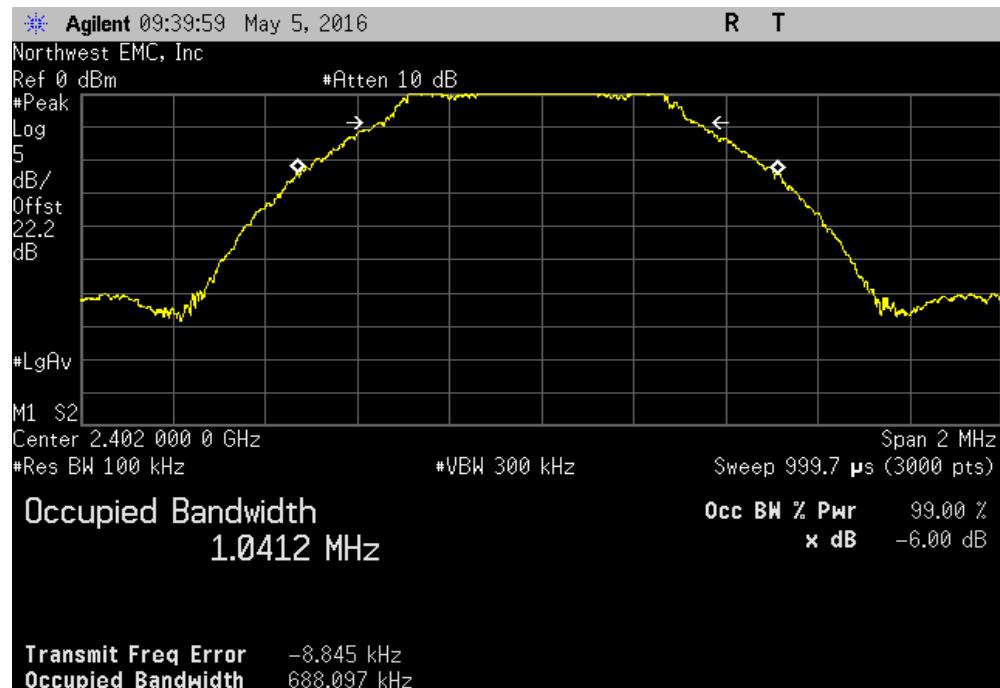

BLE/GFSK Mid Channel, 2442 MHz			Value	Limit (≥)	Result
			669.564 kHz	500 kHz	Pass

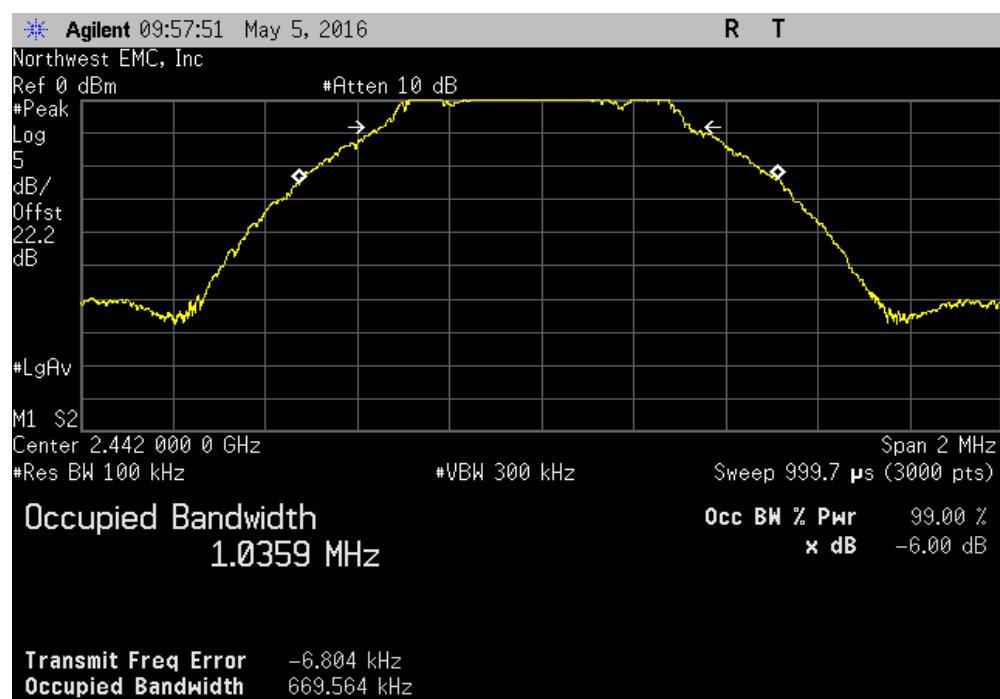

OCCUPIED BANDWIDTH

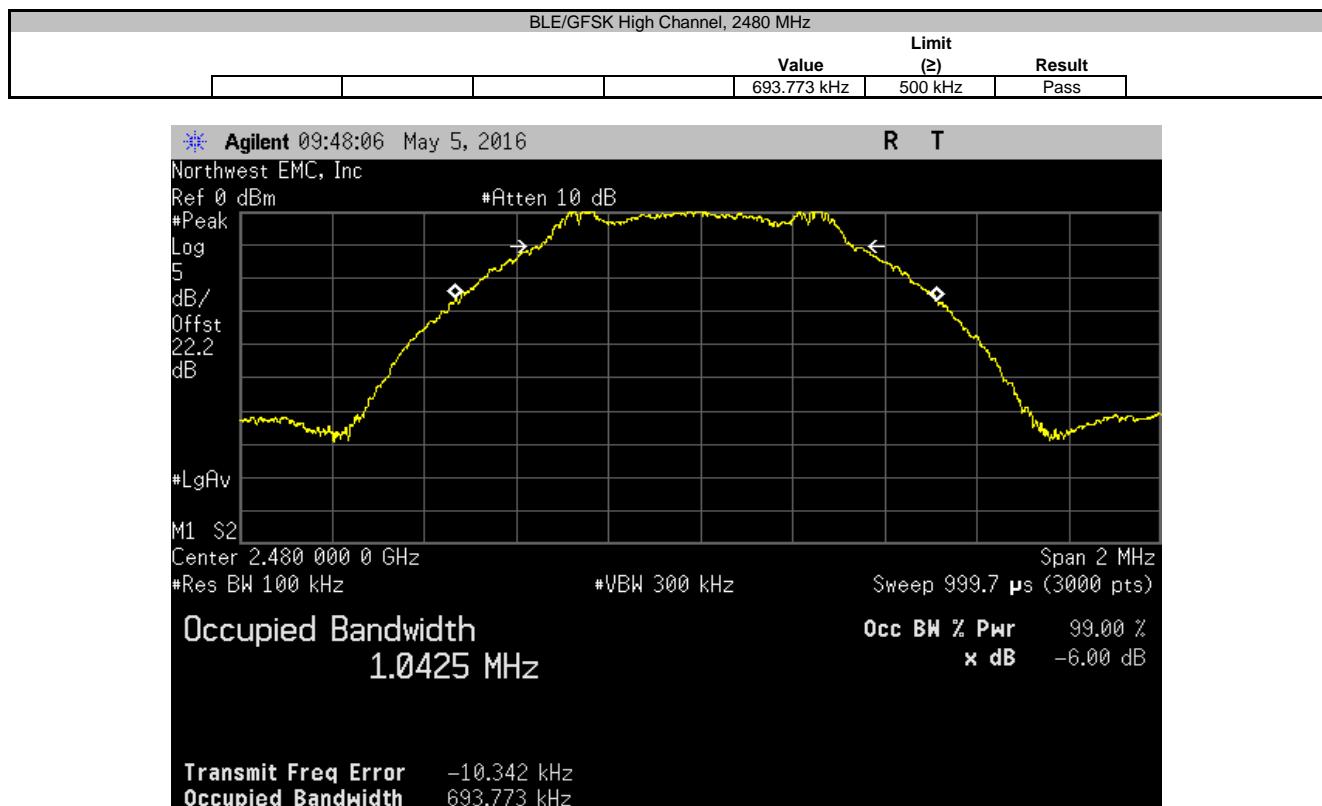

OUTPUT POWER

Testing was performed using the mode(s) of operation and configuration(s) noted within the report. The individuals and/or the organization requesting the test provided the modes, configurations and settings used to complete the evaluation. The actual test parameters are specified in the test data, this includes items such as investigated frequency range (scanned) and test levels. The testing methods and performance specifications, as well as the test site used for the evaluation are indicated in the test data.

TEST EQUIPMENT

Description	Manufacturer	Model	ID	Last Cal.	Interval (mo)
Attenuator	S.M. Electronics	SA26B-20	RFW	2/26/2016	12
Block - DC	Fairview Microwave	SD3379	AMI	9/18/2015	12
Cable	ESM Cable Corp.	TTBJ141 KMKM-72	MNU	9/18/2015	12
Generator - Signal	Agilent	N5183A	TIK	10/17/2014	36
Analyzer - Spectrum Analyzer	Agilent	E4440A	AAX	3/24/2016	12

TEST DESCRIPTION

The transmit frequency was set to the required channels in each band. The transmit power was set to its default maximum. A direct connection was made between the RF output of the EUT and a spectrum analyzer. Attenuation and a DC block were used. The reference level offset on the spectrum analyzer was adjusted to compensate for cable loss and the external attenuation used between the RF output and the spectrum analyzer input.

Prior to measuring peak transmit power the DTS bandwidth (B) and the transmission pulse duration (T) were measured. Both are required to determine the method of measuring Maximum Conducted Output Power. The transmission pulse duration (T) was measured using a zero span on the spectrum analyzer to see the pulses in the time domain.

The method found in ANSI C63.10:2013 Section 11.10.2 was used because the RBW on the analyzer was greater than the DTS Bandwidth of the radio..

De Facto EIRP Limit: Per 47 CFR 15.247 (b)(1-3), the EUT meets the de facto EIRP limit of +36 dBm.


OUTPUT POWER

**NORTHWEST
EMC**


EUT:	MyCareLink Monitor, Model 24950B		Work Order:	MDTR0462
Serial Number:	BTL000088A		Date:	05/09/16
Customer:	Medtronic Inc.		Temperature:	22.5°C
Attendees:	Taylor Dowden		Humidity:	31%
Project:	None		Barometric Pres.:	981.4
Tested by:	Dustin Sparks, Trevor Buls		Job Site:	MN05
TEST SPECIFICATIONS			Test Method	
FCC 15.247:2016			ANSI C63.10:2013	
COMMENTS				
0.885dB cable loss added to reference level offset				
DEVIATIONS FROM TEST STANDARD				
None				
Configuration #	3	Signature	Trevor Buls	
			Value	Limit (<)
BLE/GFSK Low Channel, 2402 MHz			1.972 mW	1 W
BLE/GFSK Mid Channel, 2442 MHz			1.97 mW	1 W
BLE/GFSK High Channel, 2480 MHz			1.589 mW	1 W

OUTPUT POWER

BLE/GFSK Low Channel, 2402 MHz		
Value	Limit (<)	Result
1.972 mW	1 W	Pass

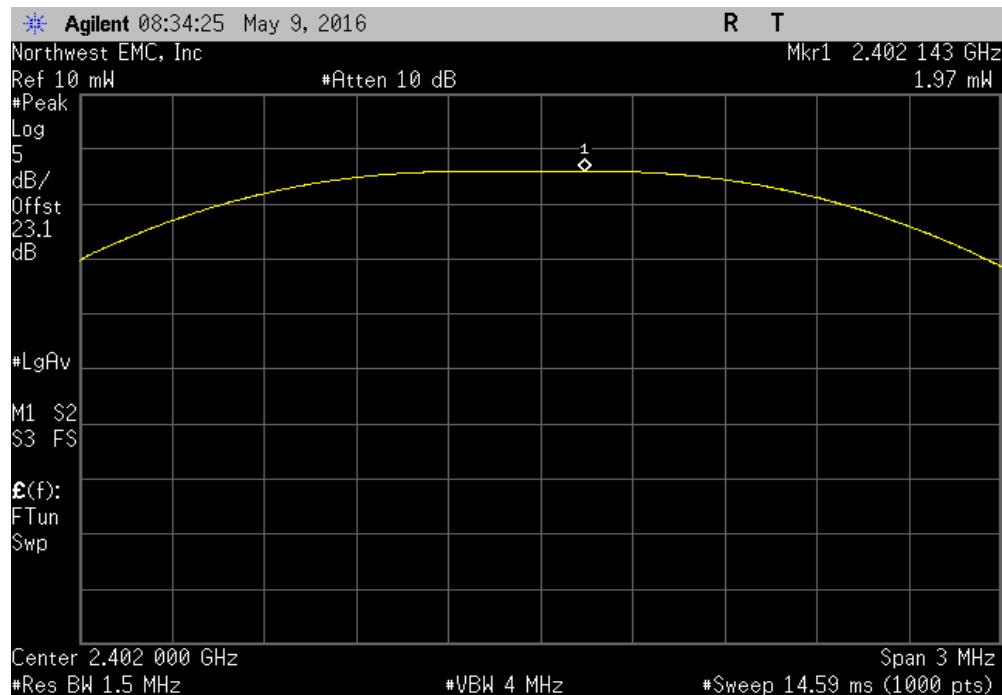


BLE/GFSK Mid Channel, 2442 MHz		
Value	Limit (<)	Result
1.97 mW	1 W	Pass

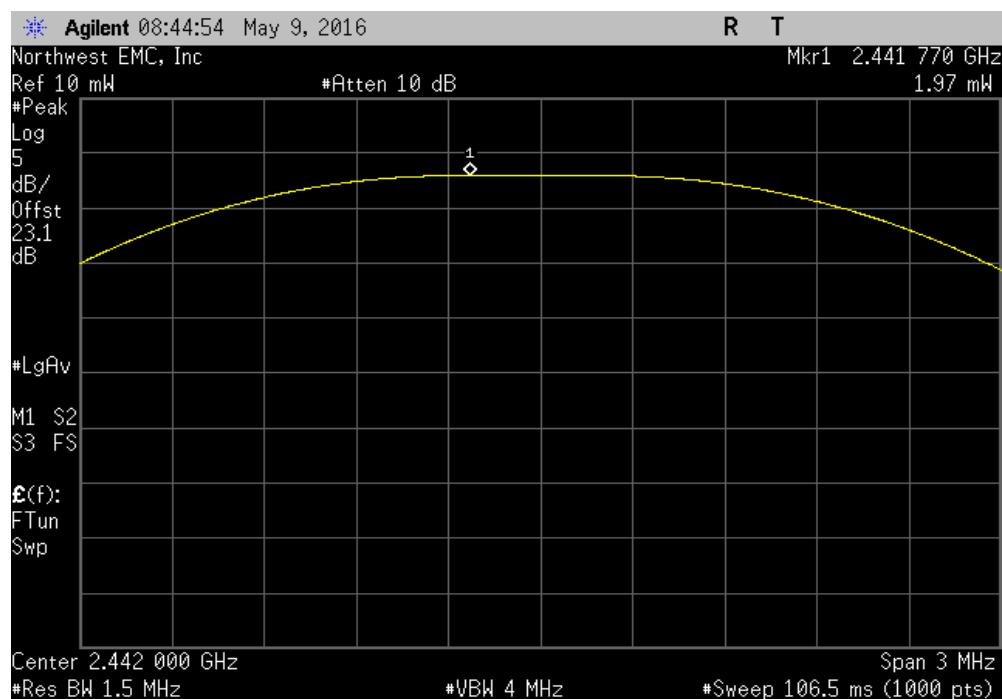

OUTPUT POWER

BLE/GFSK High Channel, 2480 MHz			Value	Limit	Result
			1.589 mW	(<) 1 W	Pass

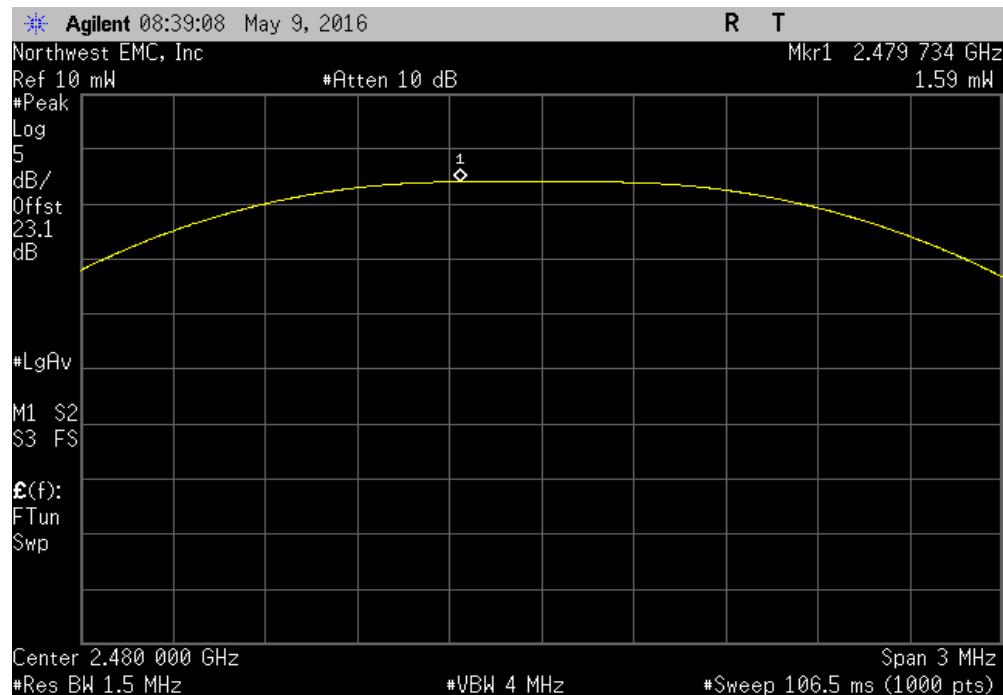

POWER SPECTRAL DENSITY

Testing was performed using the mode(s) of operation and configuration(s) noted within the report. The individuals and/or the organization requesting the test provided the modes, configurations and settings used to complete the evaluation. The actual test parameters are specified in the test data, this includes items such as investigated frequency range (scanned) and test levels. The testing methods and performance specifications, as well as the test site used for the evaluation are indicated in the test data.

TEST EQUIPMENT

Description	Manufacturer	Model	ID	Last Cal.	Interval (mo)
Attenuator	S.M. Electronics	SA26B-20	RFW	2/26/2016	12
Block - DC	Fairview Microwave	SD3379	AMI	9/18/2015	12
Cable	ESM Cable Corp.	TTBJ141 KMKM-72	MNU	9/18/2015	12
Generator - Signal	Agilent	N5183A	TIK	10/17/2014	36
Analyzer - Spectrum Analyzer	Agilent	E4440A	AAX	3/24/2016	12

TEST DESCRIPTION

The maximum power spectral density measurements was measured using the channels and modes as called out on the following data sheets.

A direct connection was made between the RF output of the EUT and a spectrum analyzer. External attenuation and a DC block were used. The reference level offset on the spectrum analyzer was adjusted to compensate for cable loss and the external attenuation used between the RF output and the spectrum analyzer input.

Per the procedure outlined in ANSI C63.10 the peak power spectral density was measured in a 3 kHz RBW.


POWER SPECTRAL DENSITY

**NORTHWEST
EMC**


EUT:	MyCareLink Monitor, Model 24950B		Work Order:	MDTR0462
Serial Number:	BTL000088A		Date:	05/09/16
Customer:	Medtronic Inc.		Temperature:	22.5°C
Attendees:	Taylor Dowden		Humidity:	31%
Project:	None		Barometric Pres.:	981.4
Tested by:	Dustin Sparks, Trevor Buls		Job Site:	MN05
TEST SPECIFICATIONS			Test Method	
FCC 15.247:2016			ANSI C63.10:2013	
COMMENTS				
0.885dB cable loss added to reference level offset				
DEVIATIONS FROM TEST STANDARD				
None				
Configuration #	3	Signature	<i>Trevor Buls</i>	
			Value	Limit
			dBm/3kHz	< dBm/3kHz
			Results	
BLE/GFSK Low Channel, 2402 MHz				
BLE/GFSK Mid Channel, 2442 MHz				
BLE/GFSK High Channel, 2480 MHz				

POWER SPECTRAL DENSITY

BLE/GFSK Low Channel, 2402 MHz				Value	Limit	
				dBm/3kHz	< dBm/3kHz	Results
				-7.519	8	Pass

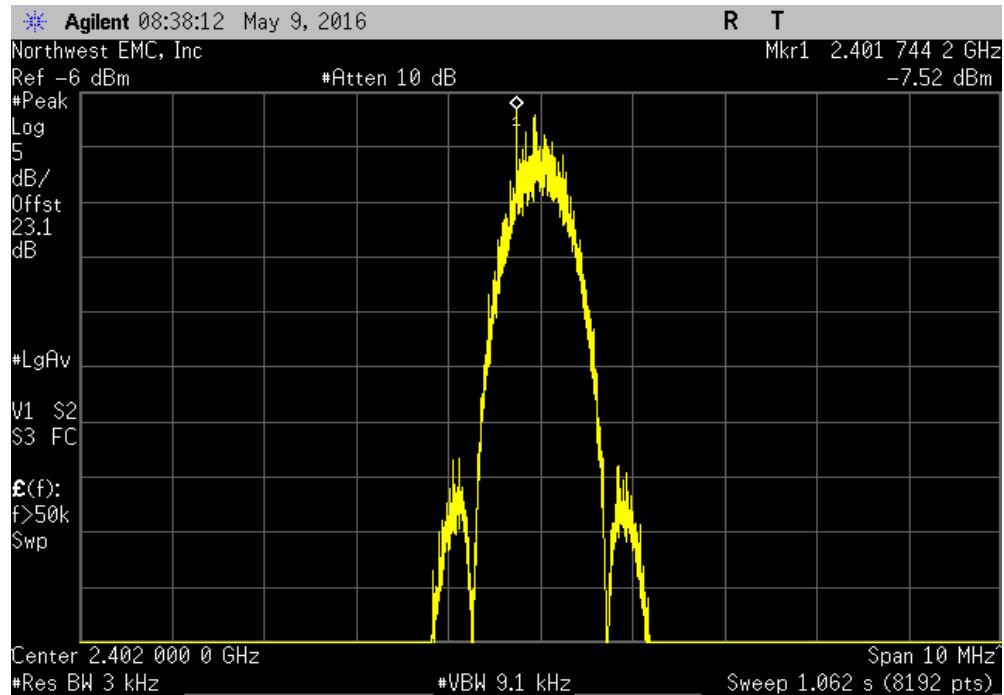


BLE/GFSK Mid Channel, 2442 MHz				Value	Limit	
				dBm/3kHz	< dBm/3kHz	Results
				-8.783	8	Pass

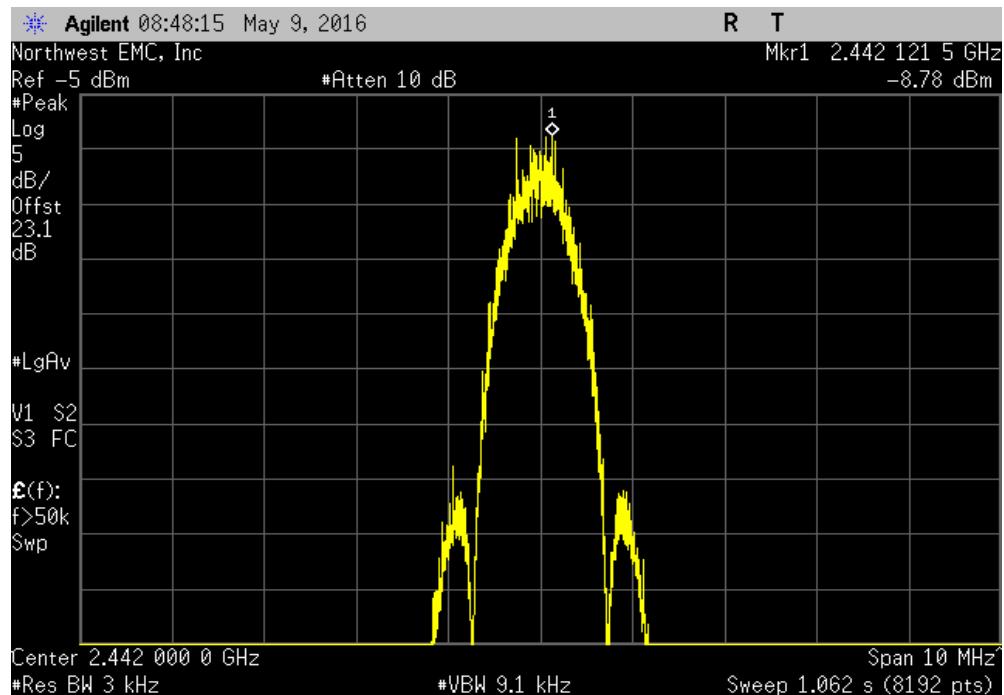

POWER SPECTRAL DENSITY

BLE/GFSK High Channel, 2480 MHz			
Value	Limit	Results	
dBm/3kHz	< dBm/3kHz	Pass	
-10.926	8		

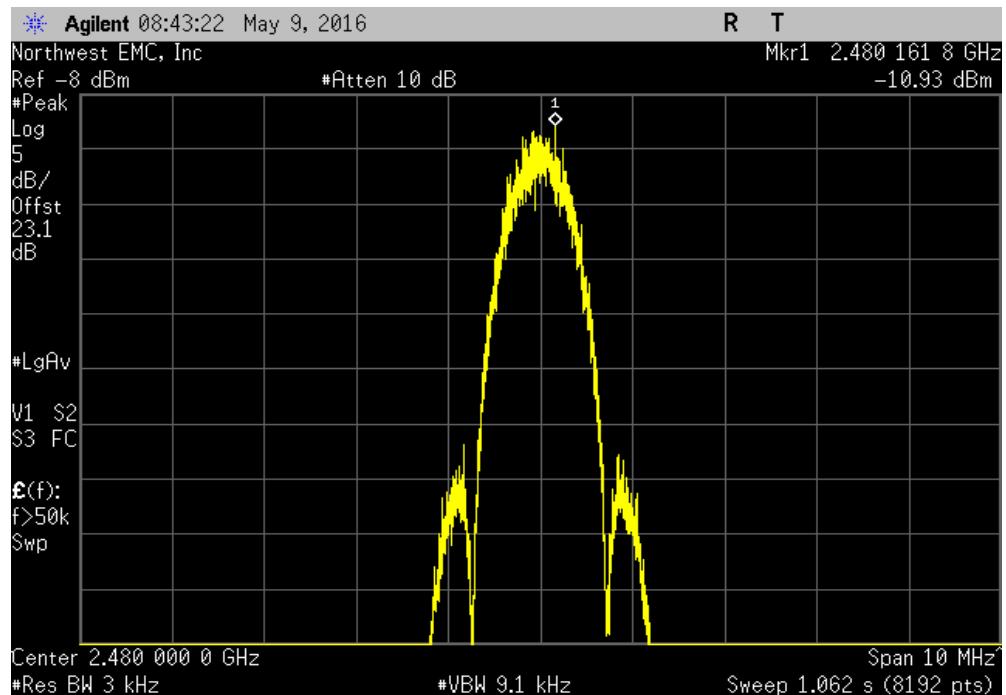

BAND EDGE COMPLIANCE

Testing was performed using the mode(s) of operation and configuration(s) noted within the report. The individuals and/or the organization requesting the test provided the modes, configurations and settings used to complete the evaluation. The actual test parameters are specified in the test data, this includes items such as investigated frequency range (scanned) and test levels. The testing methods and performance specifications, as well as the test site used for the evaluation are indicated in the test data.

TEST EQUIPMENT

Description	Manufacturer	Model	ID	Last Cal.	Interval (mo)
Attenuator	S.M. Electronics	SA26B-20	RFW	2/26/2016	12
Block - DC	Fairview Microwave	SD3379	AMI	9/18/2015	12
Cable	ESM Cable Corp.	TTBJ141 KMKM-72	MNU	9/18/2015	12
Generator - Signal	Agilent	N5183A	TIK	10/17/2014	36
Analyzer - Spectrum Analyzer	Agilent	E4440A	AAX	3/24/2016	12

TEST DESCRIPTION

The spurious RF conducted emissions at the edges of the authorized bands were measured with the EUT set to low and high transmit frequencies in each available band. The channels closest to the band edges were selected. The measurement was made using a direct connection between the RF output of the EUT and the spectrum analyzer. The EUT was transmitting at the data rate(s) listed in the datasheet.


The spectrum was scanned below the lower band edge and above the higher band edge.

BAND EDGE COMPLIANCE


EUT:	MyCareLink Monitor, Model 24950B		Work Order:	MDTR0462	
Serial Number:	BTL.000088A		Date:	05/09/16	
Customer:	Medtronic Inc.		Temperature:	22.5°C	
Attendees:	Taylor Dowden		Humidity:	31%	
Project:	None		Barometric Pres.:	981.4	
Tested by:	Dustin Sparks, Trevor Buls	Power:	5VDC	Job Site:	MN05
TEST SPECIFICATIONS			Test Method		
FCC 15.247:2016			ANSI C63.10:2013		
COMMENTS					
0.885dB cable loss added to reference level offset					
DEVIATIONS FROM TEST STANDARD					
None					
Configuration #	3	Signature	<i>Trevor Buls</i>		
			Value (dBc)	Limit ≤ (dBc)	Result
			-59.1	-20	Pass
			-58.68	-20	Pass
BLE/GFSK Low Channel, 2402 MHz					
BLE/GFSK High Channel, 2480 MHz					

BAND EDGE COMPLIANCE

BLE/GFSK Low Channel, 2402 MHz		
Value (dBc)	Limit ≤ (dBc)	Result
-59.1	-20	Pass

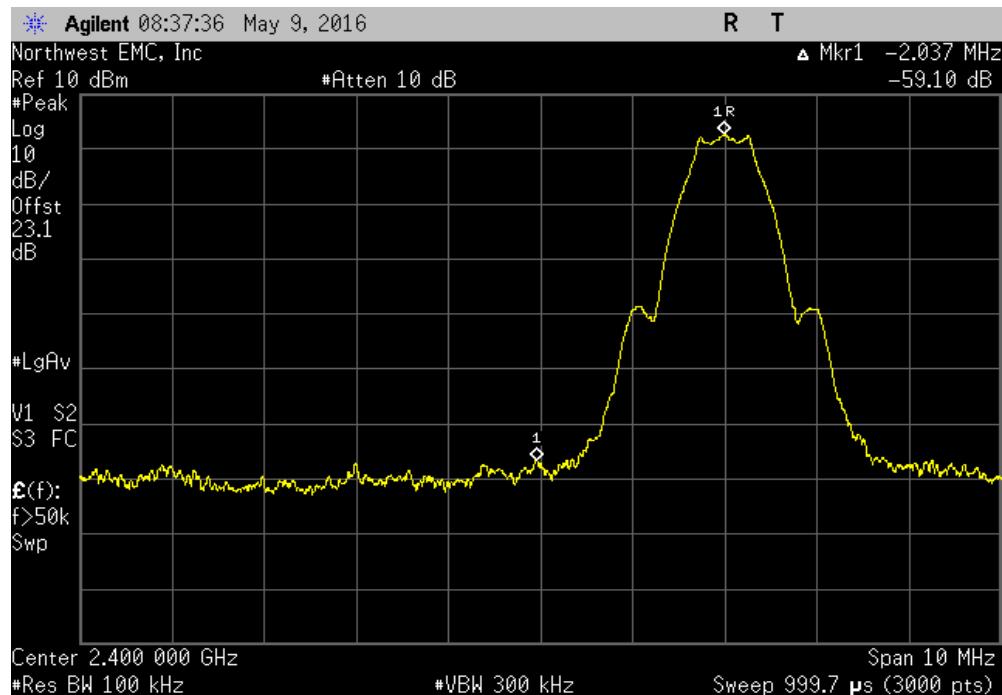

BLE/GFSK High Channel, 2480 MHz		
Value (dBc)	Limit ≤ (dBc)	Result
-58.68	-20	Pass

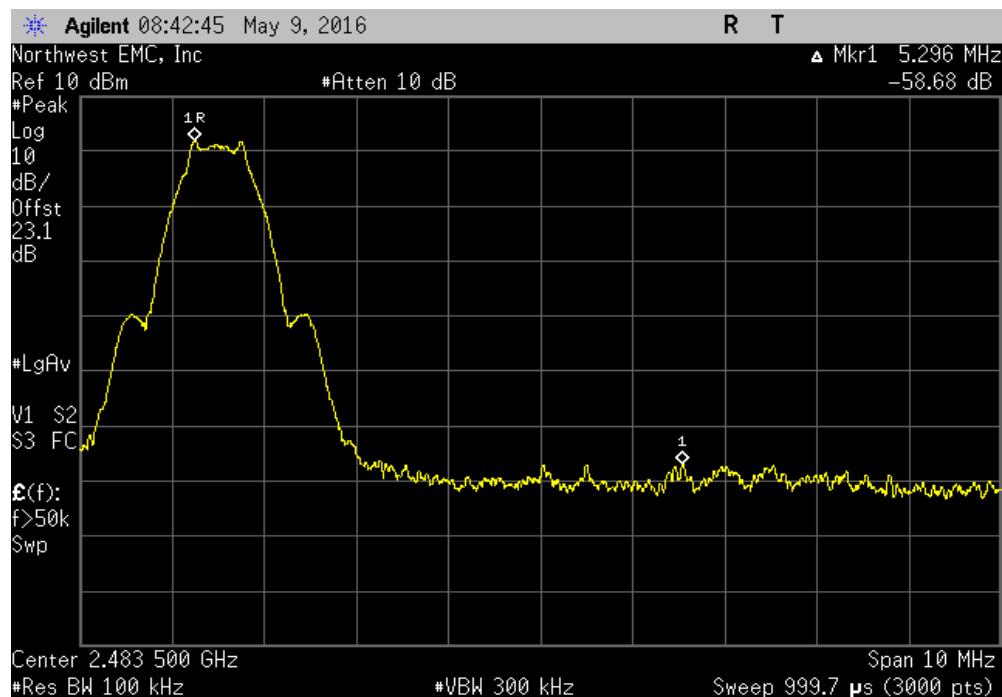

SPURIOUS CONDUCTED EMISSIONS

Testing was performed using the mode(s) of operation and configuration(s) noted within the report. The individuals and/or the organization requesting the test provided the modes, configurations and settings used to complete the evaluation. The actual test parameters are specified in the test data, this includes items such as investigated frequency range (scanned) and test levels. The testing methods and performance specifications, as well as the test site used for the evaluation are indicated in the test data.

TEST EQUIPMENT

Description	Manufacturer	Model	ID	Last Cal.	Interval (mo)
Attenuator	S.M. Electronics	SA26B-20	RFW	2/26/2016	12
Block - DC	Fairview Microwave	SD3379	AMI	9/18/2015	12
Cable	ESM Cable Corp.	TTBJ141 KMKM-72	MNU	9/18/2015	12
Generator - Signal	Agilent	N5183A	TIK	10/17/2014	36
Analyzer - Spectrum Analyzer	Agilent	E4440A	AAX	3/24/2016	12

TEST DESCRIPTION


The spurious RF conducted emissions were measured with the EUT set to low, medium and high transmit frequencies. The measurements were made using a direct connection between the RF output of the EUT and the spectrum analyzer. The EUT was transmitting at the data rate(s) listed in the datasheet. For each transmit frequency, the spectrum was scanned throughout the specified frequency range.

SPURIOUS CONDUCTED EMISSIONS


EUT:	MyCareLink Monitor, Model 24950B		Work Order:	MDTR0462	
Serial Number:	BTL.000088A		Date:	05/09/16	
Customer:	Medtronic Inc.		Temperature:	22.5°C	
Attendees:	Taylor Dowden		Humidity:	31%	
Project:	None		Barometric Pres.:	981.4	
Tested by:	Dustin Sparks, Trevor Buls	Power:	5VDC	Job Site:	MN05
TEST SPECIFICATIONS		Test Method			
FCC 15.247:2016		ANSI C63.10:2013			
COMMENTS					
0.885dB cable loss added to reference level offset					
DEVIATIONS FROM TEST STANDARD					
None					
Configuration #	3	Signature	<i>Trevor Buls</i>		
		Frequency Range	Max Value (dBc)	Limit ≤ (dBc)	Result
BLE/GFSK Low Channel, 2402 MHz		Fundamental	N/A	N/A	N/A
BLE/GFSK Low Channel, 2402 MHz		30 MHz - 12.5 GHz	-46.31	-20	Pass
BLE/GFSK Low Channel, 2402 MHz		12.5 GHz - 25 GHz	-53.7	-20	Pass
BLE/GFSK Mid Channel, 2442 MHz		Fundamental	N/A	N/A	N/A
BLE/GFSK Mid Channel, 2442 MHz		30 MHz - 12.5 GHz	-46.55	-20	Pass
BLE/GFSK Mid Channel, 2442 MHz		12.5 GHz - 25 GHz	-54.4	-20	Pass
BLE/GFSK High Channel, 2480 MHz		Fundamental	N/A	N/A	N/A
BLE/GFSK High Channel, 2480 MHz		30 MHz - 12.5 GHz	-45.88	-20	Pass
BLE/GFSK High Channel, 2480 MHz		12.5 GHz - 25 GHz	-52.82	-20	Pass

SPURIOUS CONDUCTED EMISSIONS

BLE/GFSK Low Channel, 2402 MHz					
Frequency Range	Max Value (dBc)	Limit \leq (dBc)	Result		
Fundamental	N/A	N/A	N/A		

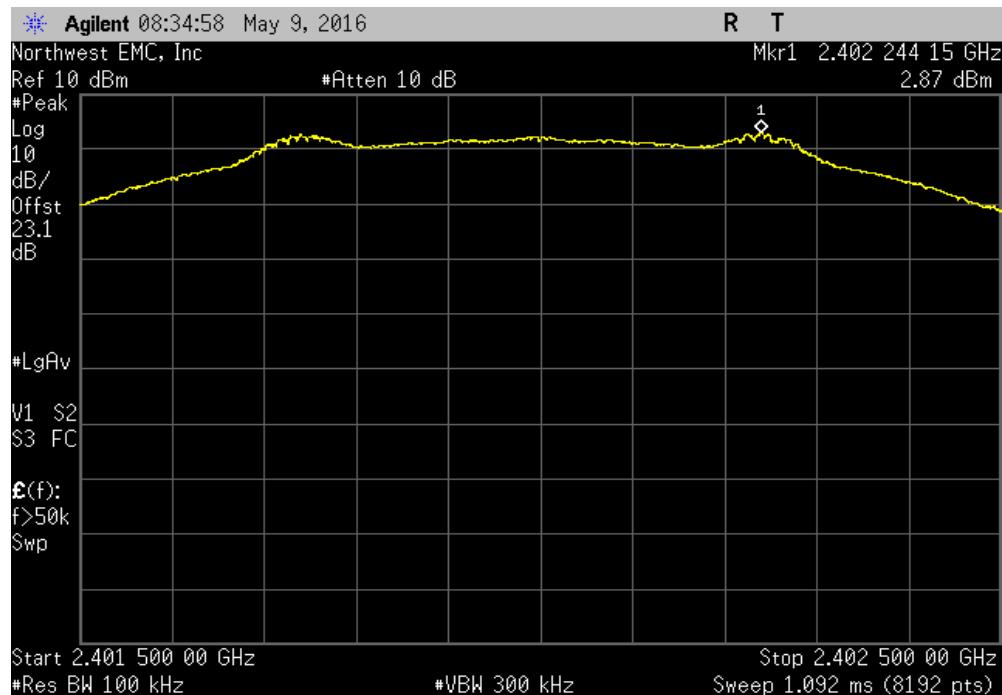


BLE/GFSK Low Channel, 2402 MHz					
Frequency Range	Max Value (dBc)	Limit \leq (dBc)	Result		
30 MHz - 12.5 GHz	-46.31	-20	Pass		

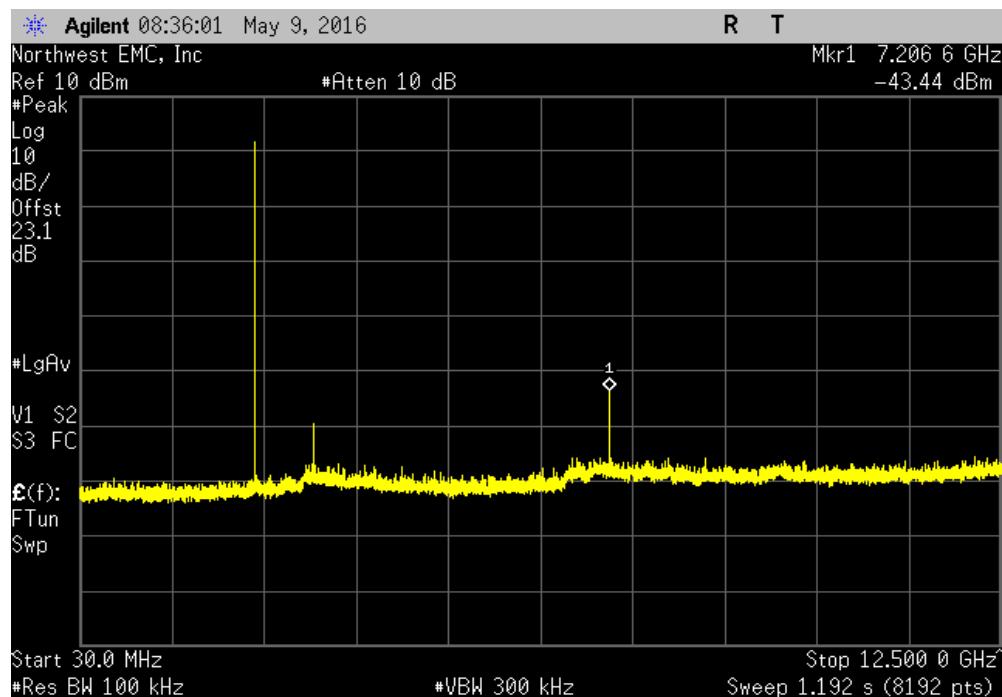


SPURIOUS CONDUCTED EMISSIONS

BLE/GFSK Low Channel, 2402 MHz					
Frequency Range		Max Value (dBc)	Limit \leq (dBc)	Result	
12.5 GHz - 25 GHz		-53.7	-20	Pass	

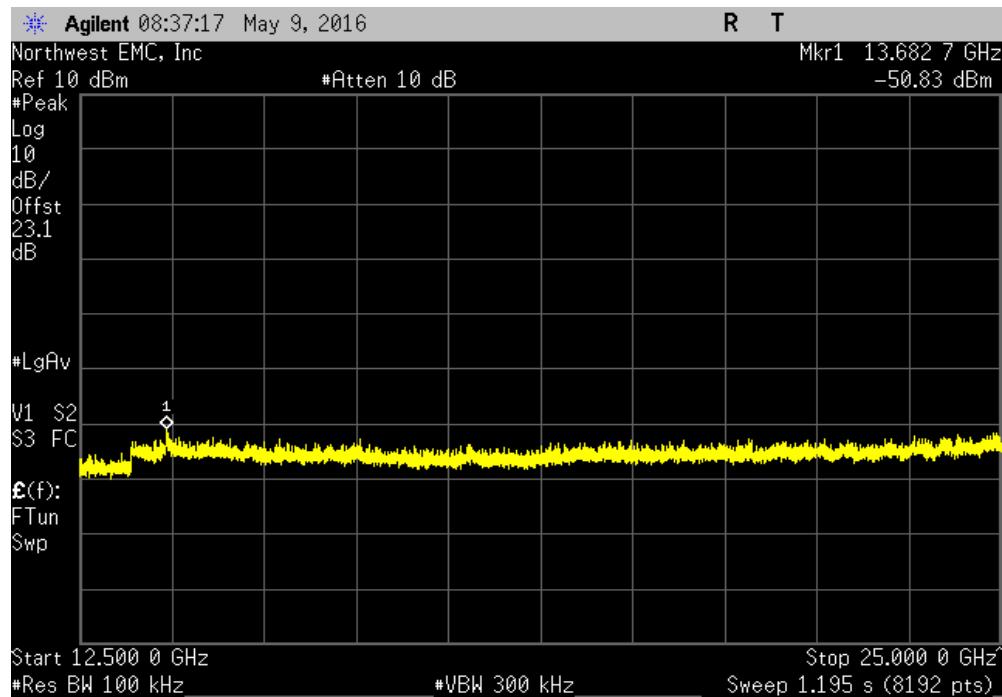


BLE/GFSK Mid Channel, 2442 MHz					
Frequency Range		Max Value (dBc)	Limit \leq (dBc)	Result	
Fundamental		N/A	N/A	N/A	

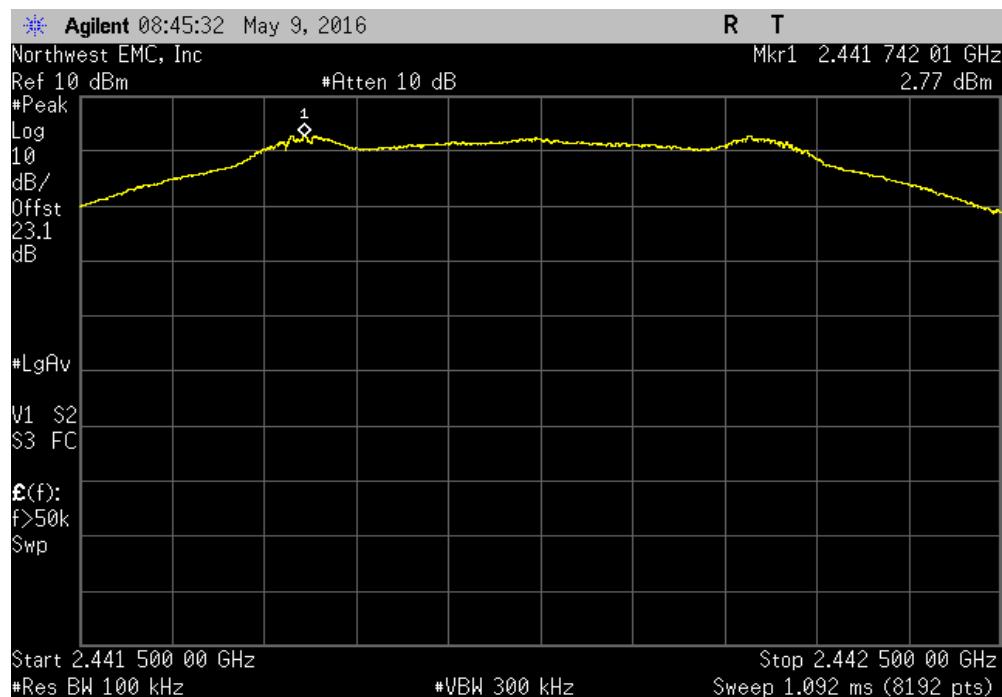


SPURIOUS CONDUCTED EMISSIONS

BLE/GFSK Mid Channel, 2442 MHz				
Frequency Range		Max Value (dBc)	Limit \leq (dBc)	Result
30 MHz - 12.5 GHz		-46.55	-20	Pass

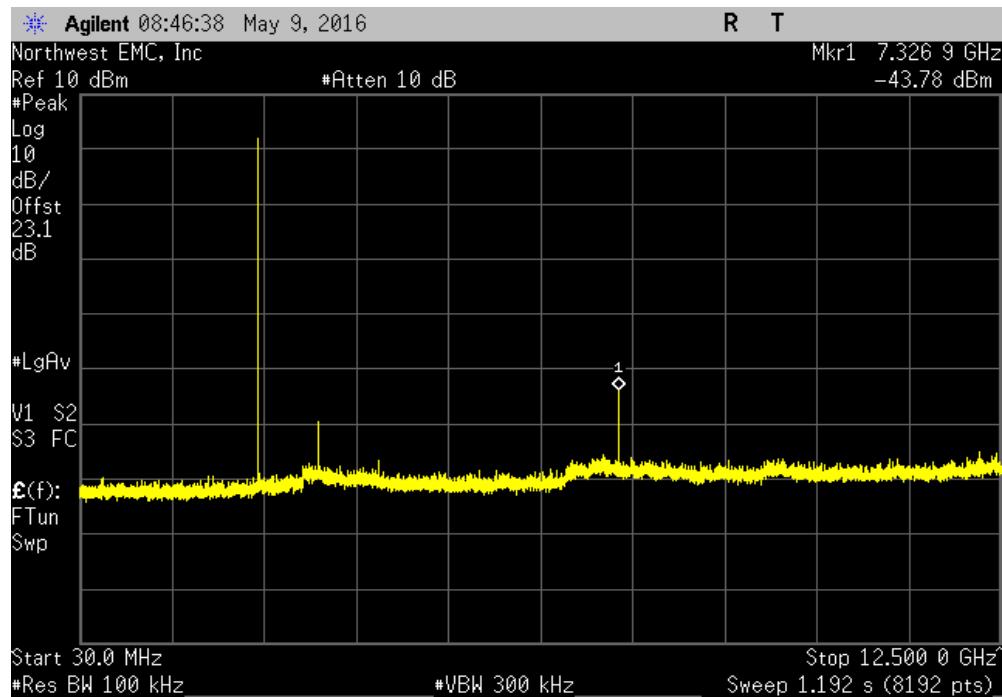


BLE/GFSK Mid Channel, 2442 MHz				
Frequency Range		Max Value (dBc)	Limit \leq (dBc)	Result
12.5 GHz - 25 GHz		-54.4	-20	Pass

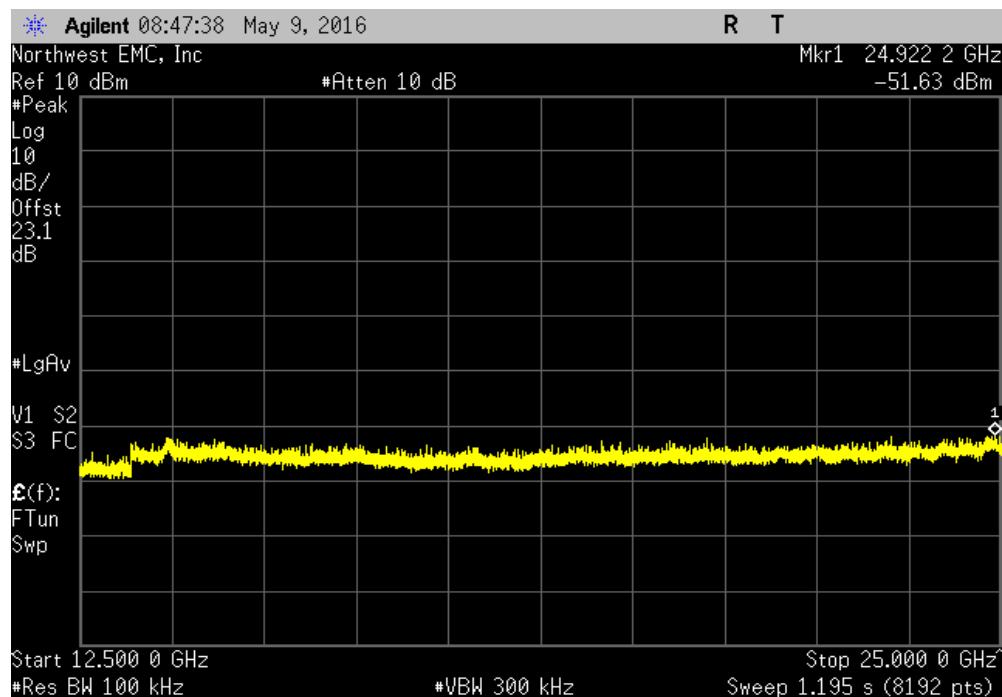


SPURIOUS CONDUCTED EMISSIONS

BLE/GFSK High Channel, 2480 MHz					
Frequency Range	Max Value (dBc)	Limit \leq (dBc)	Result		
Fundamental	N/A	N/A	N/A		

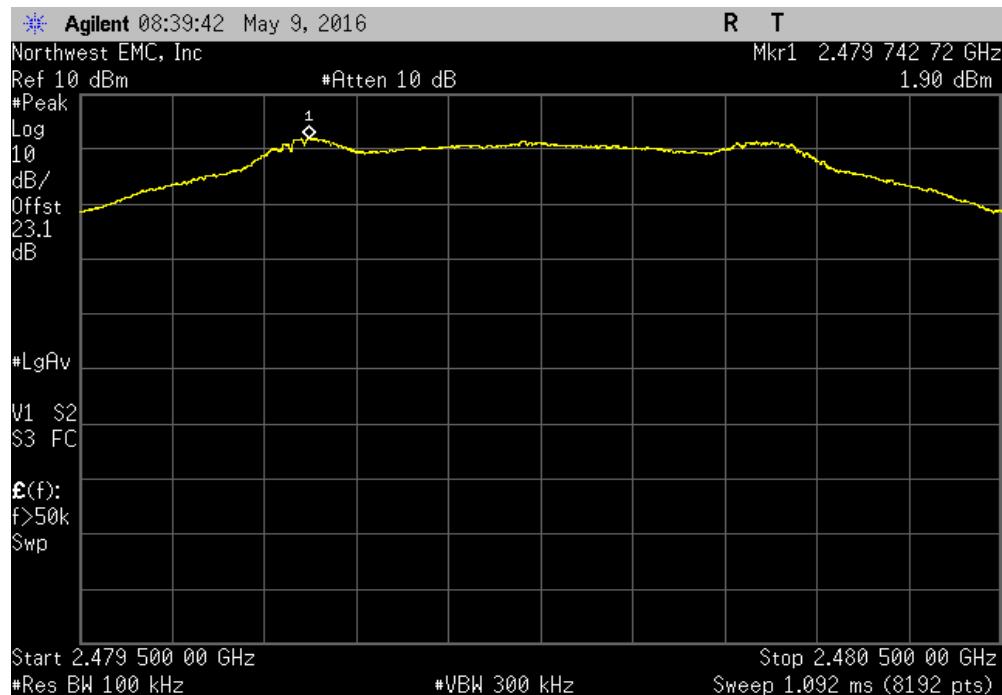


BLE/GFSK High Channel, 2480 MHz					
Frequency Range	Max Value (dBc)	Limit \leq (dBc)	Result		
30 MHz - 12.5 GHz	-45.88	-20	Pass		

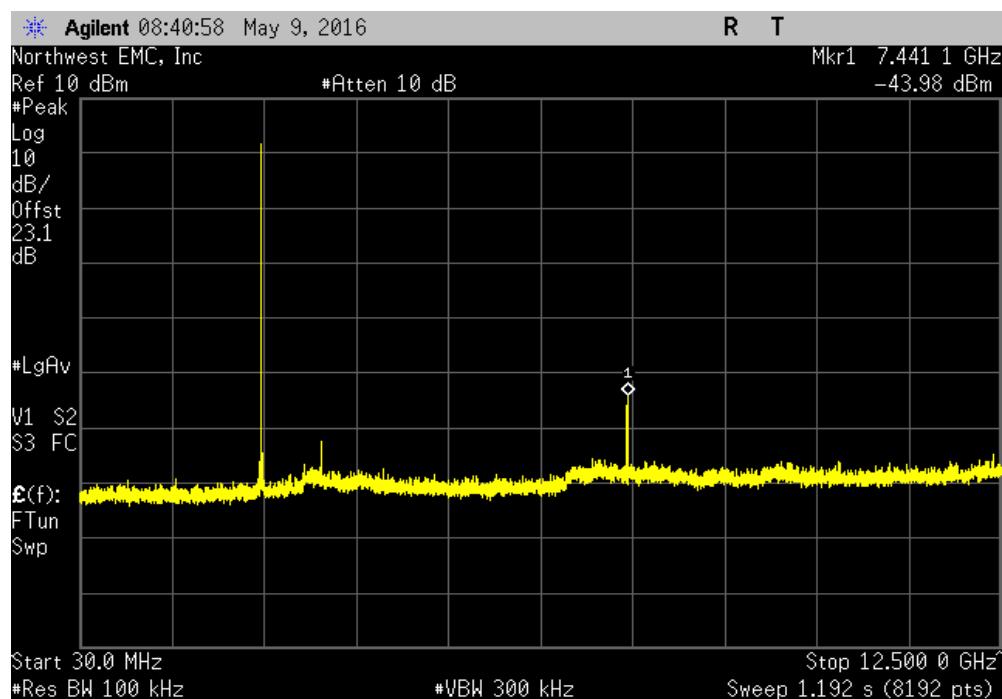

SPURIOUS CONDUCTED EMISSIONS

BLE/GFSK High Channel, 2480 MHz			
Frequency Range	Max Value (dBc)	Limit \leq (dBc)	Result
12.5 GHz - 25 GHz	-52.82	-20	Pass

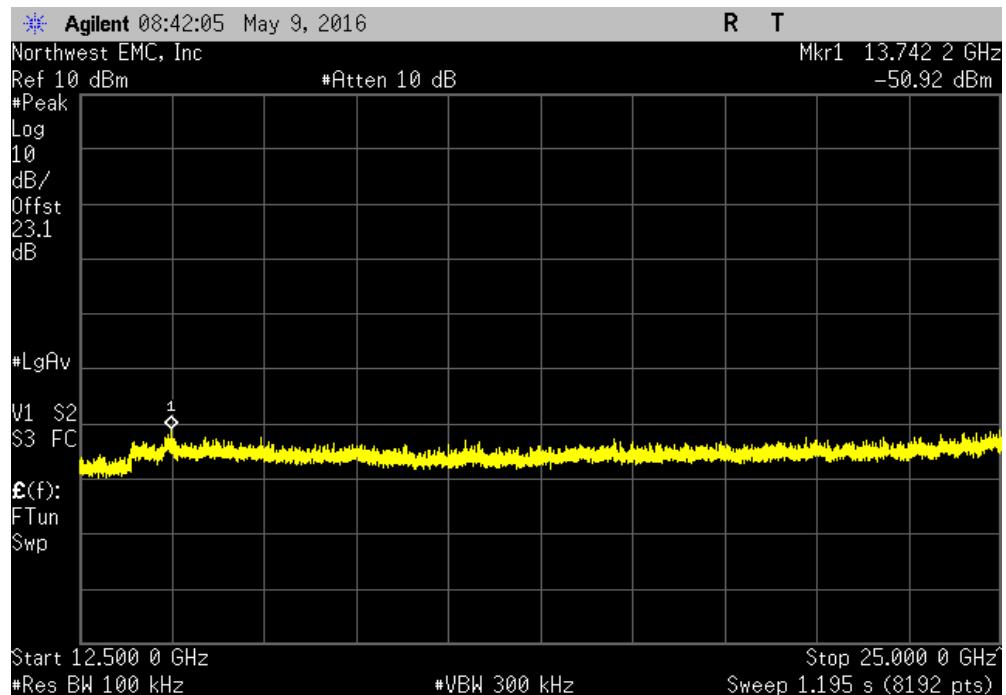

SPURIOUS RADIATED EMISSIONS

Testing was performed using the mode(s) of operation and configuration(s) noted within the report. The individuals and/or the organization requesting the test provided the modes, configurations and settings used to complete the evaluation. The actual test parameters are specified in the test data, this includes items such as investigated frequency range (scanned) and test levels. The testing methods and performance specifications, as well as the test site used for the evaluation are indicated in the test data. The test data represents the configuration / operating mode/ model that produced the highest emission levels as compared to the specification limit.

MODES OF OPERATION

Transmitting BLE - 2402 MHz (low channel), 2442 MHz (mid channel), and 2480 MHz (high channel).

POWER SETTINGS INVESTIGATED

110VAC/60Hz

CONFIGURATIONS INVESTIGATED

MDTR0462 - 1

FREQUENCY RANGE INVESTIGATED

Start Frequency | 30 MHz | Stop Frequency | 26500 MHz

SAMPLE CALCULATIONS

Radiated Emissions: Field Strength = Measured Level + Antenna Factor + Cable Factor - Amplifier Gain + Distance Adjustment Factor + External Attenuation

TEST EQUIPMENT

Description	Manufacturer	Model	ID	Last Cal.	Interval (mo)
Filter - Low Pass	Micro-Tronics	LPM50004	LFK	10/21/2015	12
Filter - High Pass	Micro-Tronics	HPM50111	LFN	10/21/2015	12
Attenuator	Fairview Microwave	SA18E-20	TWZ	10/21/2015	12
Amplifier - Pre-Amplifier	Miteq	JSD4-18002600-26-8P	APU	9/18/2015	12
Cable	Northwest EMC	18-26GHz Standard Gain Horn Cable	MNP	9/18/2015	12
Antenna - Standard Gain	ETS Lindgren	3160-09	AHG	NCR	0
Amplifier - Pre-Amplifier	Miteq	AMF-6F-12001800-30-10P	AVW	3/1/2016	12
Antenna - Standard Gain	ETS Lindgren	3160-08	AIQ	NCR	0
Cable	ESM Cable Corp.	Standard Gain Horn Cables	MNJ	12/7/2015	12
Amplifier - Pre-Amplifier	Miteq	AMF-6F-08001200-30-10P	AVV	3/1/2016	12
Antenna - Standard Gain	ETS Lindgren	3160-07	AXP	NCR	0
Amplifier - Pre-Amplifier	Miteq	AMF-3D-00100800-32-13P	AVT	3/1/2016	12
Cable	ESM Cable Corp.	Double Ridge Guide Horn Cables	MNI	12/7/2015	12
Antenna - Double Ridge	ETS Lindgren	3115	AJA	6/3/2014	24
Amplifier - Pre-Amplifier	Miteq	AM-1616-1000	AVO	12/10/2015	12
Cable	ESM Cable Corp.	Bilog Cables	MNH	12/7/2015	12
Antenna - Biconilog	Teseq	CBL 6141B	AYD	1/6/2016	24
Analyzer - Spectrum Analyzer	Agilent	N9010A	AFI	1/27/2016	12

MEASUREMENT BANDWIDTHS


Frequency Range (MHz)	Peak Data (kHz)	Quasi-Peak Data (kHz)	Average Data (kHz)
0.01 - 0.15	1.0	0.2	0.2
0.15 - 30.0	10.0	9.0	9.0
30.0 - 1000	100.0	120.0	120.0
Above 1000	1000.0	N/A	1000.0

TEST DESCRIPTION

The highest gain of each type of antenna to be used with the EUT was tested. The EUT was configured for low, mid, and high band transmit frequencies. For each configuration, the spectrum was scanned throughout the specified range. In addition, measurements were made in the restricted bands to verify compliance. While scanning, emissions from the EUT were maximized by rotating the EUT on a turntable, adjusting the position of the EUT and the EUT antenna in three orthogonal axis, and adjusting measurement antenna height and polarization. A preamp and high pass filter were used for this test in order to provide sufficient measurement sensitivity.

Work Order:	MDTR0462	Date:	04/29/16	
Project:	None	Temperature:	21.2 °C	
Job Site:	MN05	Humidity:	33.9% RH	
Serial Number:	BTL000088A	Barometric Pres.:	1025 mbar	
EUT:	MyCareLink Monitor, Model 24950B		Tested by:	Dustin Sparks
Configuration:	1			
Customer:	Medtronic Inc.			
Attendees:	Nick Blake			
EUT Power:	110VAC/60Hz			
Operating Mode:	Transmitting BLE - 2402 MHz (low channel), 2442 MHz (mid channel), and 2480 MHz (high channel).			
Deviations:	None			
Comments:	None			

Test Specifications	Test Method
FCC 15.247:2016	ANSI C63.10:2013

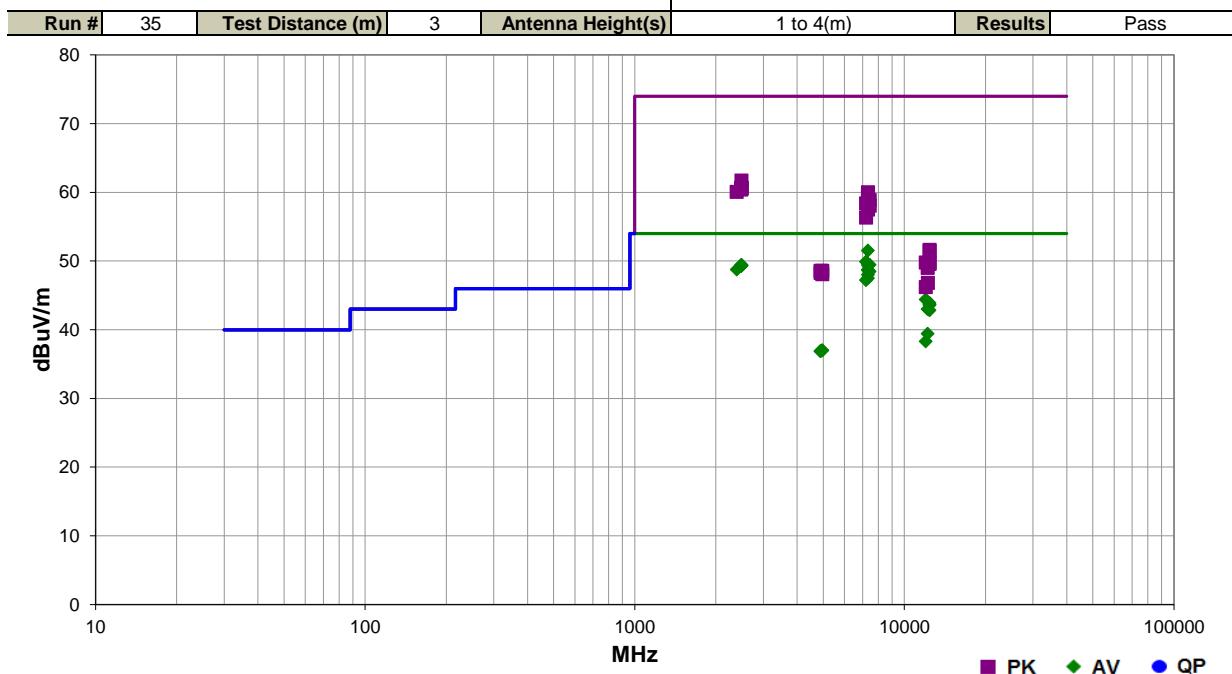

Freq (MHz)	Amplitude (dBuV)	Factor (dB)	Antenna Height (meters)	Azimuth (degrees)	Test Distance (meters)	External Attenuation (dB)	Polarity/Transducer Type	Detector	Distance Adjustment (dB)	Adjusted (dBuV/m)	Spec. Limit (dBuV/m)	Compared to Spec. (dB)	Comments
7325.308	38.2	13.3	1.7	143.0	3.0	0.0	Horz	AV	0.0	51.5	54.0	-2.5	Mid ch, EUT on side
7205.275	37.4	12.5	1.7	243.0	3.0	0.0	Horz	AV	0.0	49.9	54.0	-4.1	Low ch, EUT on side
7439.250	36.0	13.5	1.6	153.0	3.0	0.0	Horz	AV	0.0	49.5	54.0	-4.5	High ch, EUT on side
2486.517	32.8	-3.4	1.0	48.1	3.0	20.0	Vert	AV	0.0	49.4	54.0	-4.6	High ch, EUT on side
2485.267	32.8	-3.4	1.0	63.0	3.0	20.0	Horz	AV	0.0	49.4	54.0	-4.6	High ch, EUT on side
7325.350	36.1	13.3	2.7	133.0	3.0	0.0	Vert	AV	0.0	49.4	54.0	-4.6	Mid ch, EUT horz
2487.983	32.7	-3.4	1.2	93.0	3.0	20.0	Horz	AV	0.0	49.3	54.0	-4.7	High ch, EUT vert
2487.408	32.7	-3.4	3.9	173.1	3.0	20.0	Horz	AV	0.0	49.3	54.0	-4.7	High ch, EUT horz
2487.200	32.7	-3.4	1.0	2.0	3.0	20.0	Vert	AV	0.0	49.3	54.0	-4.7	High ch, EUT horz
2485.733	32.7	-3.4	1.0	336.0	3.0	20.0	Vert	AV	0.0	49.3	54.0	-4.7	High ch, EUT vert
2389.425	32.5	-3.7	1.0	239.9	3.0	20.0	Horz	AV	0.0	48.8	54.0	-5.2	Low ch, EUT horz
7325.267	35.4	13.3	1.0	97.0	3.0	0.0	Horz	AV	0.0	48.7	54.0	-5.3	Mid ch, EUT vert
7325.433	35.4	13.3	1.0	170.1	3.0	0.0	Vert	AV	0.0	48.7	54.0	-5.3	Mid ch, EUT vert
7439.375	35.0	13.5	2.1	35.0	3.0	0.0	Vert	AV	0.0	48.5	54.0	-5.5	High ch, EUT horz
7325.392	34.7	13.3	1.0	318.0	3.0	0.0	Horz	AV	0.0	48.0	54.0	-6.0	Mid ch, EUT horz
7325.492	34.2	13.3	2.4	212.0	3.0	0.0	Vert	AV	0.0	47.5	54.0	-6.5	Mid ch, EUT on side
7205.358	34.7	12.5	1.0	83.1	3.0	0.0	Vert	AV	0.0	47.2	54.0	-6.8	Low ch, EUT horz
12008.770	45.8	-1.4	1.9	34.1	3.0	0.0	Vert	AV	0.0	44.4	54.0	-9.6	Low ch, EUT horz
12398.790	43.9	0.0	1.3	245.0	3.0	0.0	Horz	AV	0.0	43.9	54.0	-10.1	High ch, EUT on side
12401.100	38.1	5.5	2.6	187.0	3.0	0.0	Vert	AV	0.0	43.6	54.0	-10.4	High ch, EUT horz
12398.740	43.6	0.0	2.7	0.0	3.0	0.0	Vert	AV	0.0	43.6	54.0	-10.4	High ch, EUT horz
12208.740	43.7	-0.7	2.0	34.1	3.0	0.0	Vert	AV	0.0	43.0	54.0	-11.0	Mid ch, EUT horz

Freq (MHz)	Amplitude (dBuV)	Factor	Antenna Height (meters)	Azimuth (degrees)	Test Distance (meters)	External Attenuation (dB)	Polarity/ Transducer Type	Detector	Distance Adjustment (dB)	Adjusted (dBuV/m)	Spec. Limit (dBuV/m)	Compared to Spec. (dB)	Comments
												Compared to Spec. (dB)	
12401.060	37.3	5.5	1.0	64.0	3.0	0.0	Horz	AV	0.0	42.8	54.0	-11.2	High ch, EUT on side
2486.808	45.1	-3.4	1.0	2.0	3.0	20.0	Vert	PK	0.0	61.7	74.0	-12.3	High ch, EUT horz
2484.958	44.1	-3.4	1.0	48.1	3.0	20.0	Vert	PK	0.0	60.7	74.0	-13.3	High ch, EUT on side
2487.433	44.0	-3.4	1.2	93.0	3.0	20.0	Horz	PK	0.0	60.6	74.0	-13.4	High ch, EUT vert
2487.175	44.0	-3.4	3.9	173.1	3.0	20.0	Horz	PK	0.0	60.6	74.0	-13.4	High ch, EUT horz
2484.992	43.9	-3.4	1.0	63.0	3.0	20.0	Horz	PK	0.0	60.5	74.0	-13.5	High ch, EUT on side
2484.175	43.8	-3.4	1.0	336.0	3.0	20.0	Vert	PK	0.0	60.4	74.0	-13.6	High ch, EUT vert
2388.433	43.8	-3.7	1.0	239.9	3.0	20.0	Horz	PK	0.0	60.1	74.0	-13.9	Low ch, EUT horz
7326.542	46.7	13.3	1.7	143.0	3.0	0.0	Horz	PK	0.0	60.0	74.0	-14.0	Mid ch, EUT on side
12208.720	40.1	-0.7	1.0	198.0	3.0	0.0	Horz	AV	0.0	39.4	54.0	-14.6	Mid ch, EUT on side
7326.342	46.1	13.3	1.0	170.1	3.0	0.0	Vert	PK	0.0	59.4	74.0	-14.6	Mid ch, EUT vert
7438.883	45.4	13.5	1.6	153.0	3.0	0.0	Horz	PK	0.0	58.9	74.0	-15.1	High ch, EUT on side
7326.542	45.4	13.3	2.7	133.0	3.0	0.0	Vert	PK	0.0	58.7	74.0	-15.3	Mid ch, EUT horz
7325.108	45.2	13.3	1.0	97.0	3.0	0.0	Horz	PK	0.0	58.5	74.0	-15.5	Mid ch, EUT vert
7205.533	45.9	12.5	1.7	243.0	3.0	0.0	Horz	PK	0.0	58.4	74.0	-15.6	Low ch, EUT on side
7326.758	45.1	13.3	1.0	318.0	3.0	0.0	Horz	PK	0.0	58.4	74.0	-15.6	Mid ch, EUT horz
12008.820	39.7	-1.4	1.4	170.1	3.0	0.0	Horz	AV	0.0	38.3	54.0	-15.7	Low ch, EUT on side
7440.958	44.6	13.5	2.1	35.0	3.0	0.0	Vert	PK	0.0	58.1	74.0	-15.9	High ch, EUT horz
7326.442	44.2	13.3	2.4	212.0	3.0	0.0	Vert	PK	0.0	57.5	74.0	-16.5	Mid ch, EUT on side
4962.225	31.4	5.6	1.0	121.0	3.0	0.0	Vert	AV	0.0	37.0	54.0	-17.0	High ch, EUT horz
4962.275	31.4	5.6	1.0	96.0	3.0	0.0	Horz	AV	0.0	37.0	54.0	-17.0	High ch, EUT on side
4885.850	31.5	5.4	2.1	223.0	3.0	0.0	Horz	AV	0.0	36.9	54.0	-17.1	Mid ch, EUT on side
4884.375	31.5	5.4	1.9	229.0	3.0	0.0	Vert	AV	0.0	36.9	54.0	-17.1	Mid ch, EUT horz
7206.458	43.8	12.5	1.0	83.1	3.0	0.0	Vert	PK	0.0	56.3	74.0	-17.7	Low ch, EUT horz
12401.330	46.1	5.5	2.6	187.0	3.0	0.0	Vert	PK	0.0	51.6	74.0	-22.4	High ch, EUT horz
12400.990	45.9	5.5	1.0	64.0	3.0	0.0	Horz	PK	0.0	51.4	74.0	-22.6	High ch, EUT on side
12008.580	51.2	-1.4	1.9	34.1	3.0	0.0	Vert	PK	0.0	49.8	74.0	-24.2	Low ch, EUT horz
12398.670	49.8	0.0	1.3	245.0	3.0	0.0	Horz	PK	0.0	49.8	74.0	-24.2	High ch, EUT on side
12398.690	49.6	0.0	2.7	0.0	3.0	0.0	Vert	PK	0.0	49.6	74.0	-24.4	High ch, EUT horz
12208.580	49.7	-0.7	2.0	34.1	3.0	0.0	Vert	PK	0.0	49.0	74.0	-25.0	Mid ch, EUT horz
4961.075	43.0	5.6	1.0	121.0	3.0	0.0	Vert	PK	0.0	48.6	74.0	-25.4	High ch, EUT horz
4886.142	43.2	5.4	2.1	223.0	3.0	0.0	Horz	PK	0.0	48.6	74.0	-25.4	Mid ch, EUT on side
4886.500	42.9	5.4	1.9	229.0	3.0	0.0	Vert	PK	0.0	48.3	74.0	-25.7	Mid ch, EUT horz
4958.050	42.5	5.6	1.0	96.0	3.0	0.0	Horz	PK	0.0	48.1	74.0	-25.9	High ch, EUT on side
12211.250	47.5	-0.7	1.0	198.0	3.0	0.0	Horz	PK	0.0	46.8	74.0	-27.2	Mid ch, EUT on side
12011.210	47.6	-1.4	1.4	170.1	3.0	0.0	Horz	PK	0.0	46.2	74.0	-27.8	Low ch, EUT on side

AC - POWERLINE CONDUCTED EMISSIONS

TEST DESCRIPTION

Using the mode of operation and configuration noted within this report, conducted emissions tests were performed. The frequency range investigated (scanned), is also noted in this report. Conducted power line measurements are made, unless otherwise specified, over the frequency range from 150 kHz to 30 MHz to determine the line-to-ground radio-noise voltage that is conducted from the EUT power-input terminals that are directly (or indirectly via separate transformer or power supplies) connected to a public power network. Per the standard, an insulating material was also added to ground plane between the EUT's power and remote I/O cables. Equipment is tested with power cords that are normally used or that have electrical or shielding characteristics that are the same as those cords normally used. Typically those measurements are made using a LISN (Line Impedance Stabilization Network), the 50ohm measuring port is terminated by a 50ohm EMI meter or a 50ohm resistive load. All 50ohm measuring ports of the LISN are terminated by 50ohm. The test data represents the configuration / operating mode/ model that produced the highest emission levels as compared to the specification limit.

TEST EQUIPMENT

Description	Manufacturer	Model	ID	Last Cal.	Cal. Due
Cable - Conducted Cable Assembly	Northwest EMC	MNC, HGN, TYK	MNCA	1/29/2016	1/29/2017
Receiver	Rohde & Schwarz	ESR7	ARI	5/21/2015	5/21/2016
LISN	Solar Electronics	9252-50-R-24-BNC	LIY	3/21/2016	3/21/2017

MEASUREMENT UNCERTAINTY

Description		
Expanded k=2	2.4 dB	-2.4 dB

CONFIGURATIONS INVESTIGATED

MDTR0462-1

MODES INVESTIGATED

Transmitting BLE mid channel (2440 MHz)

AC - POWERLINE CONDUCTED EMISSIONS

EUT:	MyCareLink Monitor, Model 24950B	Work Order:	MDTR0462
Serial Number:	BTL000088A	Date:	05/12/2016
Customer:	Medtronic Inc.	Temperature:	22.3°C
Attendees:	Taylor Dowden	Relative Humidity:	43.1%
Customer Project:	None	Bar. Pressure:	1017 mb
Tested By:	Dustin Sparks	Job Site:	MN03
Power:	110VAC/60Hz	Configuration:	MDTR0462-1

TEST SPECIFICATIONS

Specification:	Method:
FCC 15.207:2016	ANSI C63.10:2013

TEST PARAMETERS

Run #:	5	Line:	Neutral	Add. Ext. Attenuation (dB):	0
--------	---	-------	---------	-----------------------------	---

COMMENTS



None

EUT OPERATING MODES

Transmitting BLE mid channel (2442 MHz)

DEVIATIONS FROM TEST STANDARD

None

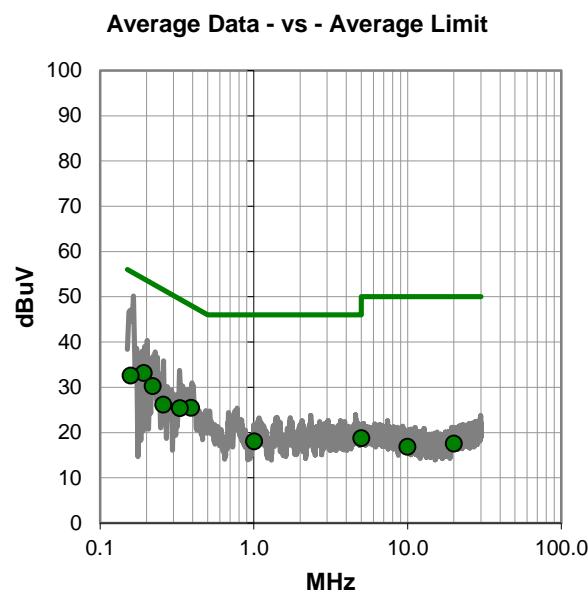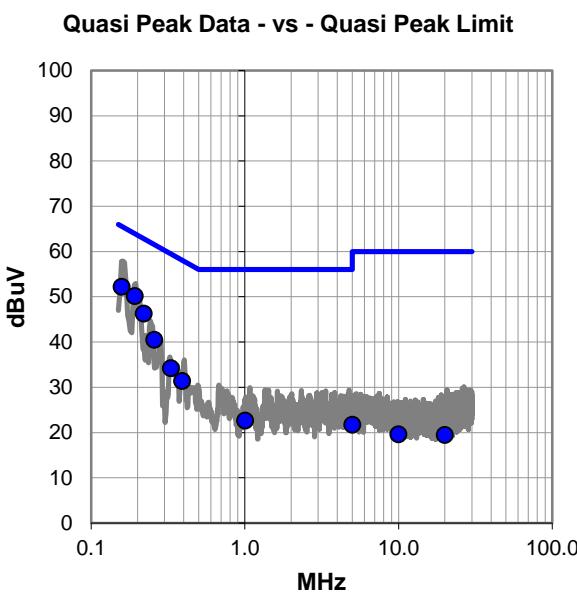

AC - POWERLINE CONDUCTED EMISSIONS

RESULTS - Run #5

Quasi Peak Data - vs - Quasi Peak Limit

Freq (MHz)	Amp. (dBuV)	Factor (dB)	Adjusted (dBuV)	Spec. Limit (dBuV)	Margin (dB)
0.158	31.8	20.4	52.2	65.6	-13.4
0.192	29.8	20.3	50.1	63.9	-13.8
0.220	26.0	20.3	46.3	62.8	-16.6
0.258	20.2	20.2	40.4	61.5	-21.1
0.331	14.0	20.2	34.2	59.4	-25.2
0.391	11.2	20.2	31.4	58.1	-26.7
1.007	2.5	20.1	22.6	56.0	-33.4
5.008	1.3	20.4	21.7	60.0	-38.3
9.993	-1.1	20.7	19.6	60.0	-40.4
19.998	-2.1	21.5	19.4	60.0	-40.6

Average Data - vs - Average Limit

Freq (MHz)	Amp. (dBuV)	Factor (dB)	Adjusted (dBuV)	Spec. Limit (dBuV)	Margin (dB)
0.192	12.8	20.3	33.1	53.9	-20.8
0.220	10.0	20.3	30.3	52.8	-22.6
0.391	5.3	20.2	25.5	48.1	-22.6
0.158	12.2	20.4	32.6	55.6	-23.0
0.331	5.2	20.2	25.4	49.4	-24.0
0.258	5.9	20.2	26.1	51.5	-25.4
1.007	-2.1	20.1	18.0	46.0	-28.0
5.008	-1.7	20.4	18.7	50.0	-31.3
19.998	-4.0	21.5	17.5	50.0	-32.5
9.993	-3.8	20.7	16.9	50.0	-33.1

CONCLUSION

Pass



Tested By

AC - POWERLINE CONDUCTED EMISSIONS

EUT:	MyCareLink Monitor, Model 24950B	Work Order:	MDTR0462
Serial Number:	BTL000088A	Date:	05/12/2016
Customer:	Medtronic Inc.	Temperature:	22.3°C
Attendees:	Taylor Dowden	Relative Humidity:	43.1%
Customer Project:	None	Bar. Pressure:	1017 mb
Tested By:	Dustin Sparks	Job Site:	MN03
Power:	110VAC/60Hz	Configuration:	MDTR0462-1

TEST SPECIFICATIONS

Specification:	Method:
FCC 15.207:2016	ANSI C63.10:2013

TEST PARAMETERS

Run #:	6	Line:	High Line	Add. Ext. Attenuation (dB):	0
--------	---	-------	-----------	-----------------------------	---

COMMENTS



None

EUT OPERATING MODES

Transmitting BLE mid channel (2442 MHz)

DEVIATIONS FROM TEST STANDARD

None

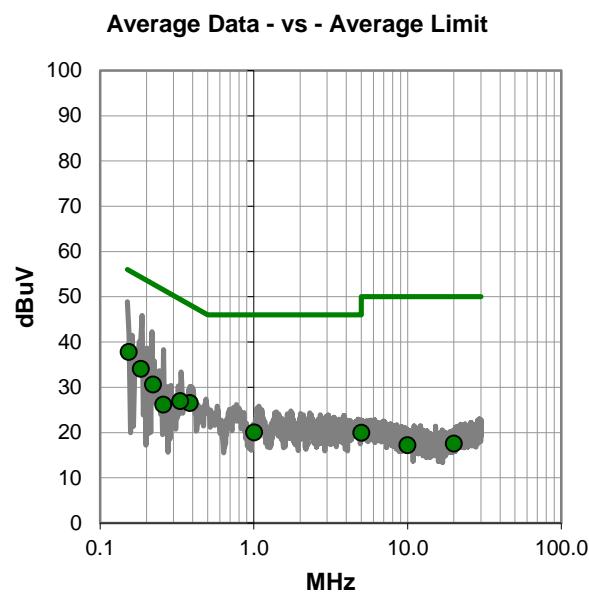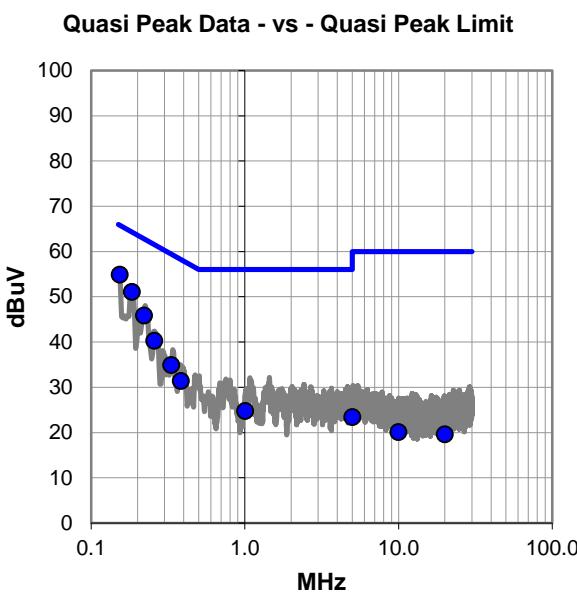

AC - POWERLINE CONDUCTED EMISSIONS

RESULTS - Run #6

Quasi Peak Data - vs - Quasi Peak Limit

Freq (MHz)	Amp. (dBuV)	Factor (dB)	Adjusted (dBuV)	Spec. Limit (dBuV)	Margin (dB)
0.154	34.5	20.4	54.9	65.8	-10.9
0.184	30.7	20.4	51.1	64.3	-13.2
0.221	25.6	20.3	45.9	62.8	-16.9
0.258	20.0	20.2	40.2	61.5	-21.3
0.333	14.7	20.2	34.9	59.4	-24.5
0.383	11.2	20.2	31.4	58.2	-26.8
1.007	4.6	20.1	24.7	56.0	-31.3
5.007	3.0	20.4	23.4	60.0	-36.6
10.009	-0.6	20.7	20.1	60.0	-39.9
20.001	-1.9	21.5	19.6	60.0	-40.4

Average Data - vs - Average Limit

Freq (MHz)	Amp. (dBuV)	Factor (dB)	Adjusted (dBuV)	Spec. Limit (dBuV)	Margin (dB)
0.154	17.4	20.4	37.8	55.8	-18.0
0.184	13.7	20.4	34.1	54.3	-20.2
0.383	6.3	20.2	26.5	48.2	-21.7
0.221	10.3	20.3	30.6	52.8	-22.2
0.333	6.7	20.2	26.9	49.4	-22.5
0.258	5.9	20.2	26.1	51.5	-25.4
1.007	-0.1	20.1	20.0	46.0	-26.0
5.007	-0.5	20.4	19.9	50.0	-30.1
20.001	-4.0	21.5	17.5	50.0	-32.5
10.009	-3.5	20.7	17.2	50.0	-32.8

CONCLUSION

Pass



Tested By