


PCTEST Engineering Laboratory, Inc.

6660-B Dobbin Road · Columbia, MD 21045 · U.S.A.

TEL (410) 290-6652 · FAX (410) 290-6654

<http://www.pctestlab.com>



CERTIFICATE OF COMPLIANCE FCC Part 95 Certification

Medtronic, Inc.
7000 Central Ave.
Minneapolis, MN 55432-3576
Attention: Mr. Len Twetan,
Senior Product Development Manager

Dates of Tests: Aug. 24 - Sept. 7, 2005
Test Report S/N: 0509130630
Test Site: PCTEST Lab, MD U.S.A.

FCC ID

LF5MICSW

APPLICANT

Medtronic, Inc.

Classification:	Licensed Non-Broadcast Transmitter Worn on the Body
FCC Rule Part(s):	§§§ 95
Procedure(s):	EN 301 839-1
EUT Type:	Medtronic Cure Link Monitor
Trade Name(s):	Medtronic
Model(s):	2490C, 2490W
Tx/Rx Frequency Range:	402.15 – 404.85 MHz
Max. RF Output Power:	23.1 µW
Frequency Tolerance:	100ppm
Emission Designator:	135K0F1D
Channel Capacity:	10

This equipment has been shown to be capable of compliance with the applicable technical standards as indicated in the measurement report and was tested in accordance with the measurement procedures specified in §2.947 and RSS-243.

I attest to the accuracy of data. All measurements reported herein were performed by me or were made under my supervision and are correct to the best of my knowledge and belief. I assume full responsibility for the completeness of these measurements and vouch for the qualifications of all persons taking them.


Randy Ortanez
President

*Application has been denied the FCC benefits
Drug Abuse Act of 1988, 21 U.S.C. 862.*





TABLE OF CONTENTS

ATTACHMENT A: COVER LETTER(S)	
ATTACHMENT B: ATTESTATION STATEMENT(S)	
ATTACHMENT C: TEST REPORT	
SCOPE	1
INTRODUCTION	2
INSERTS	3
DESCRIPTION OF TESTS	4-6
RADIATED MEASUREMENTS	7
FREQUENCY STABILITY	8-9
PLOTS OF EMISSIONS	10
LIST OF TEST EQUIPMENT	11
SAMPLE CALCULATIONS	12
CONCLUSION	13
ATTACHMENT D: TEST PLOTS	
ATTACHMENT E: FCC ID LABEL & LOCATION	
ATTACHMENT F: TEST SETUP PHOTOGRAPHS	
ATTACHMENT G: EUT PHOTOGRAPHS	
ATTACHMENT H: BLOCK DIAGRAM(S)	
ATTACHMENT I: SCHEMATIC DIAGRAM(S)	
ATTACHMENT J: USER'S MANUAL	

PCTEST PT. 95 REPORT		FCC Certification		Reviewed By: Quality Manager
Test Report S/N: 0509130630	Test Dates: Aug. 24 - Sept. 7, 2005	EUT Type: Medtronic Cure Link Monitor	FCC ID: LF5MICSW	Page i of i

MEASUREMENT REPORT



1.1 Scope

Measurement and determination of electromagnetic emissions (EME) of radio frequency devices including intentional and/or unintentional radiators for compliance with the technical rules and regulations of the Federal Communications Commission.

General Information

Applicant Name:	Medtronic, Inc.
Address:	7000 Central Ave. Minneapolis, MN 55432-3576
Attention:	Mr. Len Twetan, Senior Product Development Manager

- **FCC ID:** LF5MICSW
- **Model(s):** 2490C, 2490W
- **Quantity:** Quantity production is planned
- **Tx/Rx Freq. Range:** 402.15 – 404.85 MHz
- **Equipment Class:** Licensed Non-Broadcast Transmitter Worn on the Body
- **Equipment Type:** Medtronic Cure Link Monitor
- **Emission Designator:** 46K0F1D
- **Modulation:** FM
- **Frequency Tolerance:** 100 ppm
- **Max. Power:** 21.6 μ W
- **FCC Rule Part(s):** §§§§ 95
- **Dates of Tests:** Aug. 24 - Sept. 7, 2005
- **Place of Tests:** PCTEST Lab, Columbia, MD U.S.A.
- **Test Report S/N:** 0509130630

PCTEST PT. 95 REPORT	 FCC Certification			Reviewed By: Quality Manager
Test Report S/N: 0509130630	Test Dates: Aug. 24 - Sept. 7, 2005	EUT Type: Medtronic Cure Link Monitor	FCC ID: LF5MICSW	Page 1 of 13

2.1 INTRODUCTION

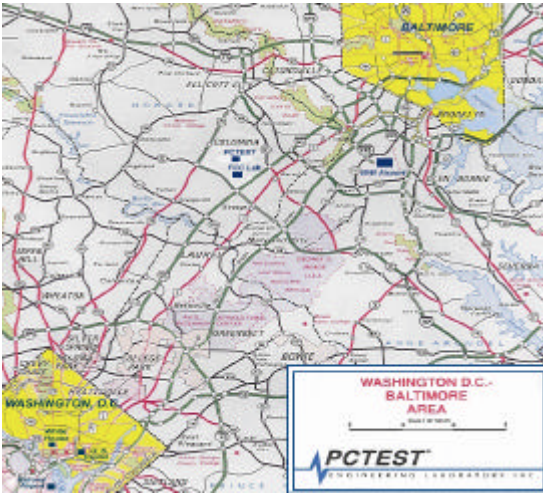


Figure 1. Map of the Greater Baltimore and Metropolitan Washington, D.C. area.

These measurement tests were conducted at **PCTEST Engineering Laboratory, Inc.** facility in New Concept Business Park, Guilford Industrial Park, Columbia, Maryland. The site address is 6660-B Dobbin Road, Columbia, MD 21045. The test site is one of the highest points in the Columbia area with an elevation of 390 feet above mean sea level. The site coordinates are 39° 11'15" N latitude and 76° 49'38" W longitude. The facility is 1.5 miles North of the FCC laboratory, and the ambient signal and ambient signal strength are approximately equal to those of the FCC laboratory. There are no FM or TV transmitters within 15 miles of the site. The detailed description of the measurement facility was found to be in compliance with the requirements of § 2.948 according to ANSI C63.4 on October 19, 1992.

Measurement Procedure

The radiated and spurious measurements were made outdoors at a 3-meter test range (see Figure2). The equipment under testing was placed on a wooden turntable, 3-meters from the receive antenna. The receive antenna height and turntable rotations was adjusted for the highest reading on the receive spectrum analyzer. A half-wave dipole was substituted in place of the EUT. This dipole antenna was driven by a signal generator and the level of the signal generator was adjusted to obtain the same receive spectrum analyzer reading. This level was recorded.

For readings above 1 GHZ, the above procedure would be repeated using horn antennas and the difference between the gain of the horn and an isotropic antenna are taken into consideration.

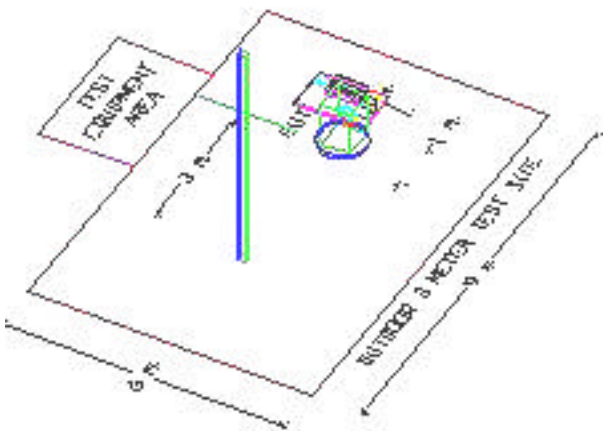


Figure 2. 3-meter outdoor test site

PCTEST® PT. 95 REPORT		FCC Certification		Reviewed By: Quality Manager
Test Report S/N: 0509130630	Test Dates: Aug. 24 - Sept. 7, 2005	EUT Type: Medtronic Cure Link Monitor	FCC ID: LF5MICSW	Page 2 of 13

3.1 INSERTS

Block Diagram(s) & Circuit Diagram(s)

The block diagram is shown in Attachment I, and the circuit diagram is shown in Attachment J.

Operating Instructions

The instruction manual is shown in Attachment K.

PCTEST® PT. 95 REPORT		FCC Certification		Reviewed By: Quality Manager
Test Report S/N: 0509130630	Test Dates: Aug. 24 - Sept. 7, 2005	EUT Type: Medtronic Cure Link Monitor	FCC ID: LF5MICSW	Page 3 of 13

4.1 DESCRIPTION OF TESTS

4.2 Transmitter Audio Frequency Response

N/A

4.3 Modulation Limiting

N/A

PCTEST® PT. 95 REPORT		FCC Certification		Reviewed By: Quality Manager
Test Report S/N: 0509130630	Test Dates: Aug. 24 - Sept. 7, 2005	EUT Type: Medtronic Cure Link Monitor	FCC ID: LF5MICSW	Page 4 of 13

4.1 DESCRIPTION OF TESTS (CONTINUED)

4.4 20dB Bandwidth

The unit was internally modulated and the Spectrum Analyzer was set with a Resolution Bandwidth of 30Hz and a Video Bandwidth of 100Hz. See plots.

4.5 Spurious and Harmonic Emissions at Antenna Terminal

N/A

4.6 Radiation Spurious and Harmonic Emissions

Radiation fundamental emissions were measured on a 3-meter outdoor site. The EUT was placed on the turntable and operated in normal fashion using internal modulation on AC power. A receiving antenna located 3 meters from the turntable receives any signal radiated from the transmitter and its operating accessories. The antenna is varied from 1 to 4 meters and the polarization is varied (horizontal and vertical) to determine the worst-case emission level. To obtain actual radiated signal strength, a signal generator is adjusted in output until a reading identical to that obtained with the actual transmitter is obtained at the receiver. Signal strength is read directly from the generator and recorded on the attached table. Measured levels on a 3 meter outdoor site were used to determine spurious and harmonic emission levels.

PCTEST PT. 95 REPORT		FCC Certification		Reviewed By: Quality Manager
Test Report S/N: 0509130630	Test Dates: Aug. 24 - Sept. 7, 2005	EUT Type: Medtronic Cure Link Monitor	FCC ID: LF5MICSW	Page 5 of 13

4.1 DESCRIPTION OF TESTS (CONTINUED)

4.7 Frequency Stability/Temperature Variation

The frequency stability of the transmitter is measured by:

- a.) **Temperature:** The temperature is varied from 0°C to +55°C using an environmental chamber.
- b.) **Primary Supply Voltage:** The primary supply voltage is varied from 85% to 115% of the voltage normally at the input to the device or at the power supply terminals if cables are not normally supplied.

Specification – The minimum frequency stability shall be +/- 100 ppm at any time during normal operation.

Time Period and Procedure:

1. The carrier frequency of the transmitter and the individual oscillators is measured at room temperature (20°C to provide a reference).
2. The equipment is subjected to an overnight “soak” at 0°C without any power applied.
3. After the overnight “soak” at 0°C (usually 14-16 hours), the equipment is turned on in a “standby” condition for one minute before applying power to the transmitter. Measurement of the carrier frequency of the transmitter and the individual oscillators is made within a three minute interval after applying power to the transmitter.
4. Frequency measurements are made at 10°C interval up to room temperature. At least a period of one and one half-hour is provided to allow stabilization of the equipment at each temperature level.
5. Again the transmitter carrier frequency and the individual oscillators is measured at room temperature to begin measurement of the upper temperature levels.
6. Frequency were made at 10 intervals starting at 0°C up to +55°C allowing at least two hours at each temperature for stabilization. In all measurements the frequency is measured within three minutes after applying power to the transmitter.
7. Any artificial load is mounted external to the temperature chamber.

NOTE: If applicable, the EUT is tested down to the battery endpoint.

PCTEST® PT. 95 REPORT		FCC Certification		Reviewed By: Quality Manager
Test Report S/N: 0509130630	Test Dates: Aug. 24 - Sept. 7, 2005	EUT Type: Medtronic Cure Link Monitor	FCC ID: LF5MICSW	Page 6 of 13

5.1 TEST DATA

5.2 Radiated Measurements

Field Strength of SPURIOUS Radiation –Low

Frequency (MHz)	Level (dBm)	AFCL (dB)	POL (H/V)	F/S (dBμV/m)	F/S (μV/m)	Power (W)	Margin (dB)
402.15	-49.700		H			2.31E-05	N/A
804.30	-97.200	31.45	H	41.25	115.4782	2.44E-09	-4.75
1206.50	-126.000	32.1	H	13.10	4.518559	3.73E-12	-40.9
1608.60	-125.000	34.5	H	16.50	6.683439	8.17E-12	-37.5
2010.80	-135.000	36	H	8.00	2.511886	1.15E-12	-46.0

Field Strength of SPURIOUS Radiation –Medium

Frequency (MHz)	Level (dBm)	AFCL (dB)	POL (H/V)	F/S (dBμV/m)	F/S (μV/m)	Power (W)	Margin (dB)
403.35	-50.000		H			2.18E-05	N/A
806.70	-96.000	31.50	H	42.50	133.3521	3.25E-09	-3.5
1210.10	-124.500	32.20	H	14.70	5.432503	5.4E-12	-39.3
1613.40	-125.100	34.60	H	16.50	6.683439	8.17E-12	-37.5
2016.80	-135.000	36.10	H	8.10	2.540973	1.18E-12	-45.9

Field Strength of SPURIOUS Radiation –High

Frequency (MHz)	Level (dBm)	AFCL (dB)	POL (H/V)	F/S (dBμV/m)	F/S (μV/m)	Power (W)	Margin (dB)
404.85	-49.800		H			2.31E-05	N/A
809.70	-95.600	31.60	H	43.00	141.2538	3.65E-09	-3.0
1214.60	-126.200	32.30	H	13.10	4.518559	3.73E-12	-40.9
1619.40	-126.100	34.70	H	15.60	6.025596	6.64E-12	-38.4
2024.30	-135.000	36.20	H	8.20	2.570396	1.21E-12	-45.8

6.1 Test Data

6.2 FREQUENCY STABILITY

OPERATING FREQUENCY: 403,350,004 Hz

CHANNEL: 5


REFERENCE VOLTAGE: 115.0 VAC

DEVIATION LIMIT: ± 0.01 % or 100 ppm

VOLTAGE (%)	POWER (VAC)	TEMP (°C)	FREQ. (Hz)	Freq. Dev. (Hz)	Deviation (%)
100 %	115.00	+ 20 (Ref)	403,350,004	0.00	0.000000
100 %					
100 %					
100 %					
100 %		0	403,349,988	16.13	0.000004
100 %		+ 10	403,349,605	399.32	0.000099
100 %		+ 20	403,350,004	0.00	0.000000
100 %		+ 25	403,348,665	1,339.12	0.000332
100 %		+ 30	403,349,125	879.30	0.000218
100 %		+ 40	403,347,769	2,234.56	0.000554
100 %		+ 50	403,347,899	2,105.49	0.000522
100 %		+ 55	403,351,359	-1,355.26	-0.000336
85 %	97.75	+ 20	403,350,004	0.00	0.000000
115 %	132.25	+ 20	403,350,004	0.00	0.000000
BATT. ENDPOINT	NA	+ 20	403,350,004	0.00	0.000000

6.1 Test Data (Continued)

6.3 FREQUENCY STABILITY

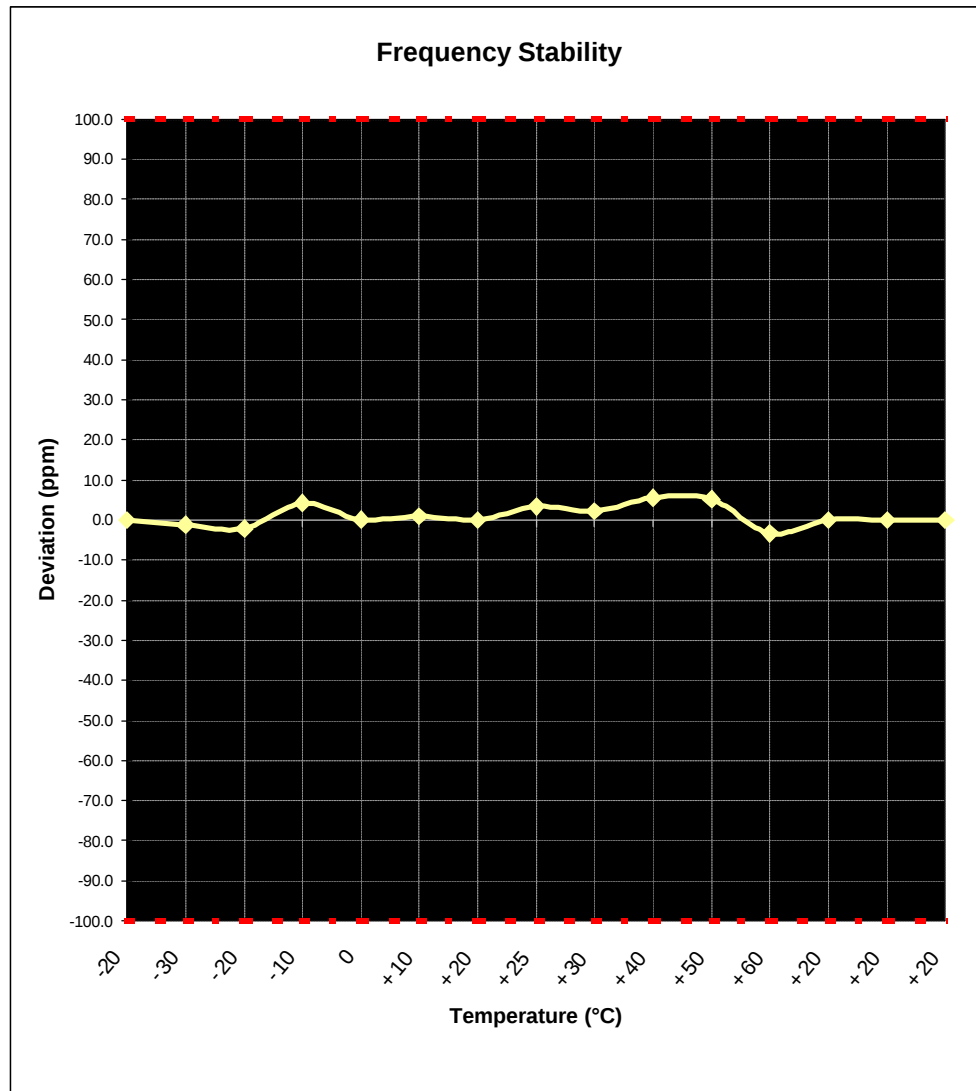

7.1 PLOT(S) OF EMISSIONS

SEE ATTACHMENT D

PCTEST® PT. 95 REPORT		FCC Certification		Reviewed By: Quality Manager
Test Report S/N: 0509130630	Test Dates: Aug. 24 - Sept. 7, 2005	EUT Type: Medtronic Cure Link Monitor	FCC ID: LF5MICSW	Page 10 of 13

8.1 TEST EQUIPMENT

8.2 Type	Model	Cal. Due Date	S/N
Microwave Spectrum Analyzer	HP 8566B (100Hz-22GHz)	08/15/06	3638A08713
Microwave Spectrum Analyzer	HP 8566B (100Hz-22GHz)	04/17/06	2542A11898
Spectrum Analyzer/Tracking Gen.	HP 8591A (100Hz-1.8GHz)	08/10/06	3144A02458
Signal Generator*	HP 8640B (500Hz-1GHz)	06/03/06	2232A19558
Signal Generator*	HP 8640B (500Hz-1GHz)	06/03/06	1851A09816
Signal Generator*	Rohde & Schwarz (0.1-1000MHz)	09/11/06	894215/012
Ailtech/Eaton Receiver	NM 37/57A-SL (30-1000MHz)	04/12/06	0792-03271
Ailtech/Eaton Receiver	NM 37/57A (30-1000MHz)	03/11/06	0805-03334
Ailtech/Eaton Receiver	NM 17/27A (0.1-32MHz)	09/17/06	0608-03241
Quasi-Peak Adapter	HP 85650A	08/15/06	2043A00301
Ailtech/Eaton Adapter	CCA-7 CISPR/ANSI QP Adapter	03/11/06	0194-04082
RG58 Coax Test Cable	No. 167		n/a
Harmonic/Flicker Test System	HP 6841A (IEC 555-2/3)		3531A00115
Broadband Amplifier (2)	HP 8447D		1145A00470, 1937A03348
Broadband Amplifier	HP 8447F		2443A03784
Transient Limiter	HP 11947A (9kHz-200MHz)		2820A00300
Horn Antenna	EMCO Model 3115 (1-18GHz)		9704-5182
Horn Antenna	EMCO Model 3115 (1-18GHz)		9205-3874
Horn Antenna	EMCO Model 3116 (18-40GHz)		9203-2178
Biconical Antenna (4)	Eaton 94455/Eaton 94455-1/Singer 94455-1/Compliance Design		1295, 1332, 0355
Log-Spiral Antenna (3)	Ailtech/Eaton 93490-1		0608, 1103, 1104
Roberts Dipoles	Compliance Design (1 set)		
Ailtech Dipoles	DM-105A (1 set)		33448-111
EMCO LISN	3816/2		1079
EMCO LISN	3816/2		1077
EMCO LISN	3725/2		2009
Microwave Preamplifier 40dB Gain	HP 83017A (0.5-26.5GHz)		3123A00181
Microwave Cables	MicroCoax (1.0-26.5GHz)		
Ailtech/Eaton Receiver	NM37/57A-SL		0792-03271
Spectrum Analyzer	HP 8594A		3051A00187
Spectrum Analyzer (2)	HP 8591A		3034A01395, 3108A02053
Modulation Analyzer	HP 8901A		2432A03467
NTSC Pattern Generator	Leader 408		0377433
Noise Figure Meter	HP 8970B		3106A02189
Noise Figure Meter	Ailtech 7510		TE31700
Noise Generator	Ailtech 7010		1473
Microwave Survey Meter	Holaday Model 1501 (2.450GHz)		80931
Digital Thermometer	Extech Instruments 421305		426966
Attenuator	HP 8495A (0-70dB) DC-4GHz		
Bi-Directional Coax Coupler	Narda 3020A (50-1000MHz)		
Shielded Screen Room	RF Lindgren Model 26-2/2-0		6710 (PCT270)
Shielded Semi-Anechoic Chamber	Ray Proof Model S81		R2437 (PCT278)
Environmental Chamber	Associated Systems Model 1025 (Temperature/Humidity)		PCT285

* Calibration traceable to the National Institute of Standards and Technology (NIST).

PCTEST PT. 95 REPORT		FCC Certification		Reviewed By: Quality Manager
Test Report S/N: 0509130630	Test Dates: Aug. 24 - Sept. 7, 2005	EUT Type: Medtronic Cure Link Monitor	FCC ID: LF5MICSW	Page 11 of 13

9.1 SAMPLE CALCULATIONS

The EIRP for channel 05 (403.35 MHz) was measured at a 3 meter distance on our OATS. The turn table and antenna mast were adjusted to obtain the highest reading on a receiver spectrum analyzer with RBW and VBW set at 3MHz each. A dipole antenna driven by a signal generator was substituted in place of the EUT and adjusted to match the -50.1 dBm receiver spectrum analyzer reading. (The dipole antenna used during the substitution has a gain of 2.14 dBi at 403.35 MHz.) The power at the antenna terminals of the substituted dipole was -18.87 dBm. This value was corrected by adding the 2.14 dBi gain of the substituted dipole to yield -16.73 dBm for EIRP.

PCTEST® PT. 95 REPORT		FCC Certification		Reviewed By: Quality Manager
Test Report S/N: 0509130630	Test Dates: Aug. 24 - Sept. 7, 2005	EUT Type: Medtronic Cure Link Monitor	FCC ID: LF5MICSW	Page 12 of 13

10.1 CONCLUSION

The data collected shows that the **Medtronic Cure Link Monitor FCC ID: LF5MICSW** complies with all the requirements of Parts 2 and 95 of the FCC rules.

PCTEST PT. 95 REPORT		FCC Certification		Reviewed By: Quality Manager
Test Report S/N: 0509130630	Test Dates: Aug. 24 - Sept. 7, 2005	EUT Type: Medtronic Cure Link Monitor	FCC ID: LF5MICSW	Page 13 of 13